

(19)



(11)

EP 2 912 996 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
02.09.2015 Bulletin 2015/36

(51) Int Cl.:
A61B 5/0205 ^(2006.01) **A61B 5/08** ^(2006.01)
A61B 5/021 ^(2006.01) **A61B 5/022** ^(2006.01)
A61B 5/00 ^(2006.01)

(21) Application number: **15155742.8**

(22) Date of filing: **19.02.2015**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(72) Inventors:
• **Kawamoto, Masashi**
Hiroshima (JP)
• **Saeki, Noboru**
Hiroshima (JP)
• **Nakamura, Ryuji**
Hiroshima (JP)
• **Ukawa, Teiji**
Tokyo (JP)
• **Takayanagi, Tsuneo**
Tokyo (JP)
• **Morimoto, Haruka**
Tokyo (JP)

(30) Priority: **28.02.2014 JP 2014038510**

(71) Applicants:
• **Hiroshima University**
Higashi-Hiroshima-shi
Hiroshima (JP)
• **Nihon Kohden Corporation**
Shinjuku-ku
Tokyo (JP)


(74) Representative: **Brevalex**
95, rue d'Amsterdam
75378 Paris Cedex 8 (FR)

(54) **Blood pressure measuring apparatus and blood pressure measuring method**

(57) A blood pressure measuring apparatus (1) includes a pressure control unit (3) that controls an applied pressure applied to a region of a living body in which a vein and artery exist by a cuff (2) mountable to the region, a detection unit (4) that detects pressure waveforms in which pulse wave components from the region overlap with the applied pressure, and an analysis unit (5) that obtains a respiratory variation on the waveform of artery

and a venous pressure based on the pressure waveforms detected by the detection unit (4) through one-time blood pressure measurement. The analysis unit (5) obtains the respiratory variation on the waveform of artery based on data of a first pressure waveform in a first process, and the venous pressure based on data of a second pressure waveform in a second process and the data of the first pressure waveform.

FIG. 1

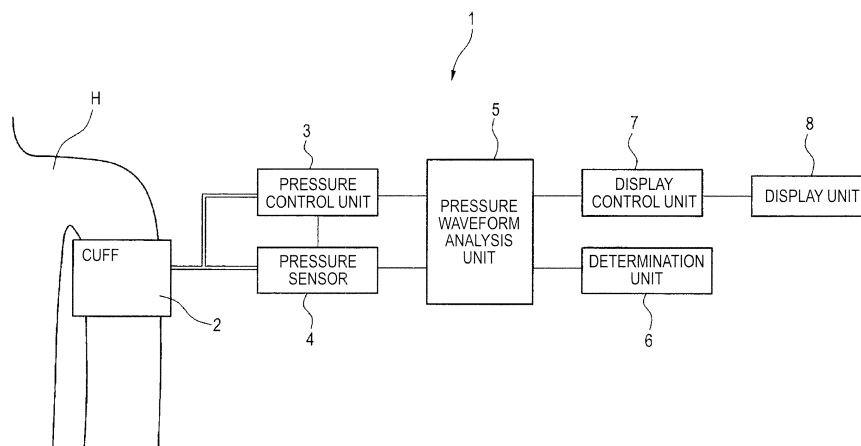

Description

BACKGROUND

[0001] The present invention relates to a blood pressure measuring apparatus and a blood pressure measuring method for measuring a blood pressure by using an oscillometric method.

[0002] When assessing hemodynamics, a respiratory variation on the waveform of artery and a central venous pressure are important indexes. In the related art, in order to obtain the central venous pressure, for example, a catheter is inserted to measure a correct central venous pressure. However, since the measuring method is invasive, an excessive burden may be applied to a subject being tested. Also, a measuring apparatus is enlarged and a measurement time is prolonged. For this reason, a method for measuring the central venous pressure by a non-invasive and simple method has been suggested.

[0003] For example, JP-A-2012-205822 discloses measuring an mean venous pressure by using an oscillometric principle. Also, JP-A-2011-511686 discloses measuring an arterial pressure and a pulse pressure variation (a respiratory variation on the waveform of artery) within a respiratory period by an oscillometric blood pressure measurement.

[0004] However, since the mean venous pressure measured by the method disclosed in JP-A-2012-205822 and the respiratory variation on the waveform of artery measured by the method disclosed in JP-A-2011-511686 are respectively measured by the separate methods, it is thought that a relativity therebetween is not necessarily high. For this reason, it is thought that the hemodynamics assessed based on the measured parameters does not necessarily have the sufficient reliability. Also, since the respective parameters are separately measured, it takes time to measure the parameters and a rapid diagnosis may be disturbed.

[0005] It is therefore an object of the present invention to provide a blood pressure measuring apparatus and a blood pressure measuring method capable of simply and correctly assessing hemodynamics of a living body.

SUMMARY

[0006]

(1) A blood pressure measuring apparatus includes a pressure control unit that controls an applied pressure applied to a region of a living body in which a vein and artery exist by a cuff mountable to the region, a detection unit that detects pressure waveforms in which pulse wave components from the region overlap with the applied pressure, and an analysis unit that obtains a respiratory variation on the waveform of artery and a venous pressure based on the pressure waveforms detected by the detection unit through one-time blood pressure measurement.

The analysis unit obtains the respiratory variation on the waveform of artery based on data of a first pressure waveform of the pressure waveforms in a first process, in which the applied pressure is kept at a constant pressure by the pressure control unit, and the venous pressure based on data of a second pressure waveform of the pressure waveforms in a second process in which the applied pressure is decreased or increased by the pressure control unit, and the data of the first pressure waveform in the first process.

According to the configuration (1), it is possible to obtain the parameters of the respiratory variation on the waveform of artery and the venous pressure at once based on the applied pressure and the pulse wave components overlapping with the applied pressure in one-time blood pressure measurement. For this reason, it is possible to obtain the respective parameters in a non-invasive and simple manner in a series of measuring processes. Also, since the two parameters are obtained based on the applied pressure and the pulse wave components obtained in one-time blood pressure measurement, it is possible to obtain the parameters having higher relativity, as compared to a configuration where the parameters are obtained based on the applied pressure and the pulse wave components obtained by measurement of a separate measuring process or by mounting the cuff to a separate region. Therefore, it is possible to correctly assess the hemodynamics based on the parameters having high relativity. Also, since the respiratory variation on the waveform of artery is obtained during a time period for which the applied pressure is controlled at a constant pressure, it is possible to correctly obtain variation components based on the respiration, which are included in the pressure waveform. Also, since the venous pressure is obtained during a time period for which the applied pressure is decreased or increased, it is possible to gradually change (decrease or increase) the pulse wave components of the arterial pressure included in the pressure waveform, thereby correctly obtaining the venous pressure.

(2) In the blood pressure measuring apparatus of (1), the applied pressure in the first process is equal to or lower than a diastolic blood pressure and within a range which does not include a pulse wave component of the vein in the pulse wave components.

According to the configuration (2), since the applied pressure is kept at a pressure equal to or lower than the diastolic blood pressure and not including the pulse wave components of the vein, it is possible to obtain the respiratory variation on the waveform of artery more correctly.

(3) In the blood pressure measuring apparatus of (1) or (2), the analysis unit is configured to obtain the venous pressure based on the data of the pressure waveform in the second process when correlativity

between the data of the pressure waveform in the second process and the data of the pressure waveform in the first process is low.

According to the configuration (3), since the venous pressure is obtained based on the data of the pressure waveform in the second process having low correlativity with respect to the data of the pressure waveform in the first process, it is possible to suppress an influence of the arterial pressure, thereby obtaining the venous pressure more correctly.

(4) In the blood pressure measuring apparatus of (1) or (2), the analysis unit is configured to obtain an arterial pressure by one-time blood pressure measurement and based on data of a third pressure waveform of the pressure waveforms in a third process, in which the applied pressure is increased or decreased by the pressure control unit.

According to the configuration (4), it is possible to obtain the three parameters of the arterial pressure, the respiratory variation on the waveform of artery and the venous pressure at once in one-time blood pressure measurement. For this reason, it is possible to obtain the respective parameters in a non-invasive and simple manner in a series of measuring processes. Also, when obtaining the arterial pressure during a time period for which the applied pressure is increased, it is possible to complete the measurement of the arterial pressure in a short time. Therefore, since it is possible to secure the longer time necessary for obtaining the respiratory variation on the waveform of artery and the venous pressure in the series of measuring processes, it is possible to obtain the three parameters securely and correctly.

(5) In the blood pressure measuring apparatus of (4), the analysis unit is configured to obtain the venous pressure based on the data of the second pressure waveform in the second process and the data of the third pressure waveform in the third process or the data of the first pressure waveform in the first process.

According to the configuration (5), since the venous pressure is obtained based on any one of the data of the pressure waveform in the first process and the data of the pressure waveform in the third process, a choice of calculation is increased. Thereby, it is possible to sufficiently check the relativity with the pulse wave components of the arterial pressure, thereby obtaining the venous pressure more correctly.

(6) In the blood pressure measuring apparatus of (5), the analysis unit is configured to obtain the venous pressure based on the data of the second pressure waveform in the second process when a correlativity between the data of the second pressure waveform in the second process and the data of the third pressure waveform in the third process or the data of the first pressure waveform in the first process is low.

According to the configuration (6), since the venous pressure is obtained based on the data of the pressure waveform in the second process having low correlativity with respect to one of the data of the waveforms in the first and third processes, it is possible to suppress the influence of the arterial pressure, thereby obtaining the venous pressure more correctly.

(7) In the blood pressure measuring apparatus of any one of (1) to (6), the blood pressure measuring apparatus further includes a display unit, and a display control unit that controls the display unit. The display control unit is configured to display a value of the obtained respiratory variation on the waveform of artery and a value of the obtained venous pressure with a two-dimensional graph on the display unit.

According to the configuration (7), since a relativity between the obtained value of the respiratory variation on the waveform of artery and the obtained value of the venous pressure is displayed as the two-dimensional graph on the display unit, a medical staff who is monitoring the biological information can comprehensively determine the two parameters of the respiratory variation on the waveform of artery and the venous pressure by seeing the display unit, thereby correctly assessing the hemodynamics.

(8) In the blood pressure measuring apparatus of (7), a determination criterion for determining the displayed value of the respiratory variation on the waveform of artery and the displayed value of the venous pressure is displayed on the two-dimensional graph. According to the configuration (8), since it is possible to determine the respiratory variation on the waveform of artery and the venous pressure based on the determination criterion displayed on the two-dimensional graph, the medical staff who is monitoring the biological information can easily assess the hemodynamics.

(9) A blood pressure measuring method for controlling an applied pressure applied to a region of a living body in which a vein and an artery exist by a cuff mountable to the region, detecting pressure waveforms in which pulse wave components are overlapped with the applied pressure, and obtaining a on the waveform of artery of an arterial pressure and a venous pressure based on the detected pressure waveforms, includes obtaining the respiratory variation on the waveform of artery based on data of a first pressure waveform of the pressure waveforms in a first process, in which the applied pressure is kept at a constant pressure, and obtaining the venous pressure based on data of a second pressure waveform of the pressure waveforms in a second process, in which the applied pressure is decreased or increased, and the data of the first pressure waveform. The first process and the second process are performed by one-time blood pressure measurement.

[0007] According to the configuration (9), it is possible to obtain the parameters of the respiratory variation on the waveform of artery and the venous pressure at once based on the applied pressure and the pulse wave components overlapping with the applied pressure in one-time blood pressure measurement. For this reason, it is possible to obtain the respective parameters in a non-invasive and simple manner in a series of measuring processes. Also, since the two parameters are obtained based on the applied pressure and the pulse wave components obtained in one-time blood pressure measurement, it is possible to obtain the parameters having higher relativity, as compared to a configuration where the parameters are obtained based on the applied pressure and the pulse wave components obtained by measurement of a separate measuring process or by mounting the cuff to a separate region. Therefore, it is possible to correctly assess the hemodynamics based on the parameters having high relativity. Also, since the respiratory variation on the waveform of artery is obtained during a time period for which the applied pressure is controlled at a constant pressure, it is possible to correctly obtain variation components based on the respiration, which are included in the pressure waveform. Also, since the venous pressure is obtained during a time period for which the applied pressure is decreased or increased, it is possible to gradually change (decrease or increase) the pulse wave components of the arterial pressure included in the pressure waveform, thereby correctly obtaining the venous pressure.

[0008] According to the blood pressure measuring apparatus of the present invention, it is possible to assess the hemodynamics of the living body simply and correctly.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009]

FIG. 1 is a functional block diagram showing a configuration of a blood pressure measuring apparatus according to an illustrative embodiment of the present invention.

FIG. 2 is a flowchart for illustrating operations of the blood pressure measuring apparatus.

FIG. 3A illustrates a change in a cuff pressure during measurement of the blood measuring apparatus.

FIG. 3B illustrates pulse wave components overlapping with the cuff pressure of FIG. 3A.

FIG. 4 illustrates the overlapping pulse wave components during an arterial pressure measurement time period.

FIG. 5 illustrates the overlapping pulse wave components during a respiratory variation measurement time period.

FIG. 6 illustrates the overlapping pulse wave components during a venous pressure measurement time period.

FIG. 7 is a graph showing a relativity between the respiratory variation and the venous pressure.

DETAILED DESCRIPTION OF EMBODIMENTS

[0010] Hereinafter, an illustrative embodiment of a blood pressure measuring apparatus of the present invention will be described in detail with reference to the drawings.

[0011] FIG. 1 is a functional block diagram showing a configuration of a blood pressure measuring apparatus 1 according to an illustrative embodiment of the present invention.

[0012] As shown in FIG. 1, the blood pressure measuring apparatus 1 has a cuff 2, a pressure control unit 3, a pressure sensor (an example of a detection unit) 4, a pressure waveform analysis unit (an example of an analysis unit) 5, a determination unit 6, a display control unit 7 and a display unit 8.

[0013] The cuff 2 is wound and mounted to a part of a living body at which the vein and artery of a subject being tested (an example of a living body) can be detected, for example, to a brachial region (an example of a region) in the vicinity of an axillary region. The cuff 2 has a pressure pouch (not shown), and a cuff pressure (an example of an applied pressure) is applied from the cuff 2 to the brachial region by an air pressure of the pressure pouch.

[0014] The pressure control unit 3 is configured to control the air pressure of the pressure pouch of the cuff 2. The air pressure of the pressure pouch is controlled by a pressurization pump, an electromagnetic valve, a control circuit and the like included in the pressure control unit 3. All of them are not shown in the drawings.

[0015] The pressure sensor 4 is configured to detect a pressure waveform in which pulse wave components overlap with the cuff pressure. When the cuff pressure is applied to the brachial region, a pulse wave, which is a vibration of a blood vessel wall, overlaps with the cuff pressure in synchronization with the pulse of the subject being tested H. The pressure sensor 4 is configured to detect the pressure waveform in which the pulse wave components from the brachial region overlap, and to transmit the detected pressure waveform to the pressure waveform analysis unit 5.

[0016] The pressure waveform analysis unit 5 is configured to obtain a diastolic blood pressure, an mean blood pressure and a systolic blood pressure (an example of an arterial pressure), a respiratory variation on the waveform of artery, and an mean venous pressure (an example of a venous pressure) measured at the vein of the brachial region in the vicinity of the axillary region, based on the cuff pressures and pulse wave components included in the pressure waveform. The pressure waveform analysis unit 5 is configured to obtain the respiratory variation on the waveform of artery and the mean venous pressure together with the blood pressure in one-time measuring process of measuring the blood pressure. In the meantime, it is said that the mean venous pressure

measured at the vein of the brachial region is substantially equivalent to a central venous pressure measured by an invasive method.

[0017] The determination unit 6 is configured to determine the reliability of the respiratory variation on the waveform of artery and mean venous pressure obtained by the pressure waveform analysis unit 5. The determination unit 6 is configured to determine the reliability by taking correlations between a representative pulse wave and the pulse waves overlapping with the respective cuff pressures during a time period for which the respiratory variation on the waveform of artery is obtained and during a time period for which the mean venous pressure is obtained.

[0018] The display control unit 7 is configured to display on the display unit 8 the information of the diastolic blood pressure, the systolic blood pressure, the mean blood pressure, the respiratory variation on the waveform of artery, the mean venous pressure and the like. The display unit 8 is configured by a touch panel-type liquid crystal screen, for example.

[0019] Subsequently, operations of the blood pressure measuring apparatus 1 are described based on a flow-chart shown in FIG. 2, with reference to FIGS. 3 to 6. In below descriptions, the measurement of the pulse wave component and the determination of the arterial pressure, the respiratory variation on the waveform of artery and the mean venous pressure are made substantially at the same time. However, only the measurement of the cuff pressure and the pulse wave component may be first made and the determination of the arterial pressure, the respiratory variation on the waveform of artery and the mean venous pressure may be separately made using the data of the measured cuff pressure and the like.

[0020] As shown in FIG. 2, when the measurement of the blood pressure measuring apparatus 1 starts, a blood pressure value is first measured (step S101). The blood pressure value is non-invasively measured by the oscillometric method. The cuff pressure of the cuff 2 wound on the brachial region is gradually or stepwise increased by the pressure control unit 3. A pressure waveform in the pressurization process (a third process) is detected by the pressure sensor 4, and the cuff pressures and pulse wave components (an example of data of the pressure waveform) included in the pressure waveform are measured and analyzed by the pressure waveform analysis unit 5. The pressure waveform analysis unit 5 obtains the diastolic blood pressure, the mean blood pressure and the systolic blood pressure based on a change in the pulse wave component.

[0021] Specifically, when the cuff pressure is increased, an amplitude of the pulse wave component overlapping with the cuff pressure is correspondingly increased. When the cuff pressure becomes the same as a blood pressure applied to the blood vessel wall, the amplitude of the pulse wave component becomes largest. When the cuff pressure is further increased, the amplitude of the pulse wave component decreases. The

pressure waveform analysis unit 5 determines, as the mean blood pressure, the cuff pressure at the time that the amplitude of the pulse wave component becomes largest. Also, the pressure waveform analysis unit 5 obtains a pulse wave amplitude at the diastolic blood pressure and a pulse wave amplitude at the systolic blood pressure by a predetermined calculation equation, based on the maximum amplitude of the pulse wave component. At this time, the diastolic blood pressure is a cuff pressure lower than the mean blood pressure and is a cuff pressure at the time that the pulse wave amplitude being measured coincides with the pulse wave amplitude at the diastolic blood pressure obtained by the calculation equation. Also, the systolic blood pressure is a cuff pressure higher than the mean blood pressure and is a cuff pressure at the time that the pulse wave amplitude being measured coincides with the pulse wave amplitude at the systolic blood pressure obtained by the calculation equation. In the meantime, it may be possible to measure the mean blood pressure, the systolic blood pressure and the diastolic blood pressure while the cuff pressure is rapidly increased to a pressure higher than the systolic blood pressure and is then gradually reduced.

[0022] FIG. 3 illustrates a change in the pressure detected during one-time measurement of the blood pressure measuring apparatus 1. FIG. 3A illustrates a change in the pressure waveform (in which the pulse wave components overlap with the cuff pressures) over elapsed measurement time of the blood pressure measuring apparatus 1. Also, FIG. 3B illustrates the pulse wave components in the pressure waveform of FIG. 3A.

[0023] The diastolic blood pressure, the mean blood pressure and the systolic blood pressure are measured during the pressurization process of the cuff pressure, which is a time period A shown in FIG. 3A. The measurement of the above blood pressures is completed at the time that the systolic blood pressure is measured. The blood pressure measurement during the time period A is completed at about 15 seconds after the measurement starts.

[0024] Subsequently, the pressure waveform analysis unit 5 extracts the pulse wave component in the mean blood pressure of the blood pressures obtained in step S101, as a representative pulse wave component (step S102).

[0025] FIG. 4 illustrates the pulse wave components during the time period A in FIG. 3. The pulse wave component having the largest amplitude of the pulse wave components during the time period A is extracted as a representative pulse wave component a1, which is the pulse wave component of the mean blood pressure.

[0026] Subsequently, in order to obtain the respiratory variation on the waveform of artery, the cuff pressure is reduced to a pressure within a range equal to or lower than the diastolic blood pressure and not including the pulse wave component of the vein, for example, 40 to 50 mmHg (step S103). By reducing the cuff pressure to the pressure within the range, when obtaining the respiratory

variation on the waveform of artery, the artery is not excessively occluded and the pulse of the vein does not influence.

[0027] The respiratory variation on the waveform of artery is obtained during a constant pressure (for example, about 50 mmHg) process (a first process) of the cuff pressure, which is a time period B shown in FIG. 3A. During the time period B, the multiple respiratory variations on the waveform of artery are obtained. For this reason, the cuff pressure is kept at a constant pressure equal to or lower than the diastolic blood pressure continuously for a predetermined time period (for example, 60 seconds). In the meantime, the pressure that is kept constant is not limited to the pressure equal to or lower than the diastolic blood pressure inasmuch as an influence of the pulse of the venous pressure does not appear in the pressure. For example, a pressure near the diastolic blood pressure may also be used.

[0028] Subsequently, the determination unit 6 calculates correlation coefficients R1 between the pulse wave components overlapping with the cuff pressure kept at a constant pressure and the representative pulse wave component a1 extracted in step S102 (step S104).

[0029] FIG. 5 illustrates the extracted pulse wave components during the time period B of FIG. 3. During the time period B, individual pulse wave components b1, b2, b3,... are extracted by the pressure waveform analysis unit 5. The correlation coefficients R1 between the extracted individual pulse wave components b1, b2, b3,... and the representative pulse wave component a1 are calculated.

[0030] Subsequently, the determination unit 6 extracts the pulse wave component having low correlativity based on the correlation coefficients R1, and excludes the extracted pulse wave component so that it is not used as a pulse wave component for obtaining the respiratory variation on the waveform of artery (step S105). In order to obtain the respiratory variation on the waveform of artery having the higher reliability, it is preferable that the pulse wave component of the vein does not influence the pulse wave components b1, b2, b3,... during the time period B. The pulse wave components b1, b2, b3,..., which are not influenced by the pulse wave component of the vein, have the high correlativity with the representative pulse wave component a1, which is a typical pulse wave of the artery. For this reason, the pulse wave component having the low correlativity is excluded and the pulse wave component having the high correlativity is used as the pulse wave component for obtaining the respiratory variation on the waveform of artery. Thereby, it is possible to improve the reliability of the obtained respiratory variation on the waveform of artery.

[0031] Subsequently, the pressure waveform analysis unit 5 calculates amplitudes of the extracted pulse wave components b1, b2, b3,..., and calculates a respiratory period of the subject being tested H from a change in the amplitude (step S106). Then, it is determined whether 60 seconds have elapsed after the measurement of the

respiratory variation on the waveform of artery has started (step S107). When 60 seconds have not elapsed, each step from step S104 is repeated. On the other hand, when 60 seconds have elapsed, the pressure waveform analysis unit 5 obtains the respiratory variation on the waveform of artery of the subject being tested H based on the amplitude variation of the pulse wave components during the plurality of calculated respiratory periods (step S108).

[0032] Solid lines p shown in FIG 5 indicate envelope curves connecting peaks of the pulse wave components, and a time period T1 indicates the respiratory period. Also, an amplitude Hmax indicates a maximum amplitude of the pulse wave component, and an amplitude Hmin indicates a minimum amplitude of the pulse wave component. The respiratory variation on the waveform of artery is calculated by an equation of $((H_{\max} - H_{\min}) / ((H_{\max} + H_{\min}) / 2)) * 100[\%]$. By the calculation equation, the respiratory variation on the waveform of artery is calculated during the multiple respiratory periods.

[0033] As shown in FIG. 3A, the measurement of the respiratory variation on the waveform of artery is completed at about 75 seconds after the measurement starts.

[0034] Subsequently, in order to obtain the mean venous pressure, the pressure control unit 3 stepwise (for example, by 5 mmHg) lowers the cuff pressure (step S109).

[0035] The mean venous pressure is obtained in a depressurization process of the cuff pressure (a second process), which is a time period C shown in FIG. 3A. The mean venous pressure is measured continuously to the measurement of the respiratory variation on the waveform of artery, and the cuff pressure is stepwise reduced over time from the constant pressure (for example, about 50 mmHg) at which the respiratory variation on the waveform of artery is measured.

[0036] Subsequently, the pressure waveform analysis unit 5 calculates the amplitudes of the pulse wave components overlapping with the cuff pressure reduced by 5 mmHg (step S110). Then, the determination unit 6 calculates correlation coefficients R2 between the pulse wave components overlapping with the cuff pressure reduced by 5 mmHg and the representative pulse wave component a1 extracted in step S102 (step S111).

[0037] FIG. 6 illustrates the extracted pulse wave components during the time period C of FIG. 3. During the time period C, individual pulse wave components c1, c2, c3,... are extracted and amplitudes thereof are calculated. The correlation coefficients R2 between the extracted individual pulse wave components c1, c2, c3,... and the representative pulse wave component a1 are calculated.

[0038] Subsequently, it is determined whether 6 seconds have elapsed after the cuff pressure is reduced by 5 mmHg (step S112). When 6 seconds have not elapsed, each step from step S110 is repeated. On the other hand, when 6 seconds have elapsed, it is determined whether 140 seconds have elapsed after the measurement of the

blood pressure has started (step S113). When 140 seconds have not elapsed, the processing is returned to step S109, the cuff pressure is further reduced by 5 mmHg and each step from step S110 is then repeated. On the other hand, when 140 seconds have elapsed, the pressure waveform analysis unit 5 obtains the mean venous pressure based on the amplitudes of the pulse wave components calculated in step S110 and the correlation coefficients R2 calculated in step S111 (step S114).

[0039] Specifically, when the cuff pressure is stepwise reduced, the pulse wave components of the artery overlapping with the cuff pressure are correspondingly reduced and the pulse wave components of the vein are gradually increased. For this reason, the correlation coefficient R2 with the representative pulse wave component a1, which is the typical pulse of the artery, is gradually decreased. When the cuff pressure is further reduced, the pulse wave components of the vein are further increased. When the cuff pressure becomes equal to the blood pressure applied to the blood vessel wall, the amplitudes of the pulse wave components of the vein show peaks. Based on this, the mean venous pressure is obtained by the pulse wave components of the second process and the correlativity between the pulse wave components of the second process and the pulse wave components of the first process. In the meantime, since the pulse wave components of the vein are smaller, as compared to the pulse wave components of the artery, even though the cuff pressure is reduced and the pulse wave components of the artery are thus decreased, the pulse wave components of the artery may influence the observation of the pulse wave components of the vein. In this case, it may not possible to clearly detect the peaks of the amplitudes of the pulse wave components of the vein. For this reason, the pressure waveform analysis unit 5 performs the overall analysis on condition that the correlativity is low and the amplitude of the pulse wave component shows a peak, and determines the cuff pressure at that time, as the mean venous pressure. Then, the pressure waveform analysis unit estimates the determined mean venous pressure as a central venous pressure.

[0040] In this way, the measurement of each parameter is completed.

[0041] Subsequently, data that is displayed on the display unit 8 of the blood pressure measuring apparatus 1 is described with reference to FIG. 7.

[0042] As shown in FIG. 7, the values of the respiratory variation on the waveform of artery and the values of the mean venous pressure obtained as described above are displayed as a two-dimensional graph on the display unit 8. Also, a determination criterion for determining the value of the respiratory variation on the waveform of artery and the value of the mean venous pressure is displayed as threshold lines m, n, for example.

[0043] Based on the display of the two-dimensional graph, the hemodynamics of the subject being tested is determined as follows. For example, when the obtained

value of the respiratory variation on the waveform of artery and the obtained value of the mean venous pressure are a point q on the graph, the value of the respiratory variation on the waveform of artery is below the threshold line n and the value of the mean venous pressure is above the threshold line m, it is determined that circulating blood volume is excessive. Also, for example, when the obtained values are a point r, the value of the respiratory variation on the waveform of artery is above the threshold line n and the value of the mean venous pressure is below the threshold line m, it is determined that circulating blood volume is insufficient.

[0044] Also, although not shown in FIG. 7, the values of the diastolic blood pressure, systolic blood pressure and mean blood pressure obtained as described above are also displayed simultaneously with the display of the two-dimensional graph on the display unit 8.

[0045] According to the blood pressure measuring apparatus 1 of the illustrative embodiment, during one-time blood pressure measurement by the oscillometric method, the parameters of the diastolic blood pressure, mean blood pressure, systolic blood pressure, respiratory variation on the waveform of artery and mean venous pressure can be obtained at once based on the cuff pressure applied from the cuff 2 to the brachial region and the pulse wave components overlapping with the cuff pressure. For this reason, it is possible to obtain the respective parameters in a non-invasive and simple manner in a series of measuring processes. Also, since all the parameters are obtained based on the cuff pressure and the pulse wave components overlapping with the cuff pressure obtained in one-time blood pressure measurement, the relativity of the parameters is very high, as compared to a configuration where the parameters are obtained based on the cuff pressure and the pulse wave components overlapping with the cuff pressure obtained by measurement of a separate measuring process or by mounting the cuff 2 to a separate region. That is, while the respiratory variation on the waveform of artery and the mean venous pressure obtained by the method of the related art are the indexes having low reliability, it is possible to correctly assess the hemodynamics of the subject being tested H based on the parameters having high relativity, in accordance with the illustrative embodiment of the present invention.

[0046] Also, since the diastolic blood pressure, mean blood pressure, systolic blood pressure are measured during the pressurization process of the cuff pressure, it is possible to shorten the time necessary to complete the measurement of the above blood pressures, as compared to a configuration where the cuff pressure is increased above the systolic blood pressure and the diastolic blood pressure, mean blood pressure, systolic blood pressure are measured during the depressurization process of the cuff pressure. Thereby, since it is possible to secure the longer time necessary for obtaining the respiratory variation on the waveform of artery and the mean venous pressure in the series of measuring

processes, it is possible to obtain the parameters securely and correctly.

[0047] Also, since the respiratory variation on the waveform of artery is obtained during the time period for which the cuff pressure is kept at a constant pressure, it is possible to clearly plot the envelope curves p connecting the peaks of the pulse wave components, so that it is possible to correctly obtain the variation components based on the respiration of the subject being tested, which are included in the pressure waveform. Also, since about 60 seconds are secured with respect to the time period for which the cuff pressure is kept at a constant pressure, it is possible to calculate the respiratory variation on the waveform of artery during the multiple respiratory periods, so that it is possible to obtain the more correct measurement result. Also, the cuff pressure is kept at the constant pressure within a range close to the diastolic blood pressure and not including the pulse wave components of the vein. Therefore, when obtaining the respiratory variation on the waveform of artery, the pulse of the vein little influences, so that it is possible to correctly extract the respiratory variation on the waveform of artery.

[0048] In the meantime, some subjects being tested may have the low diastolic blood pressure. Therefore, when obtaining the respiratory variation on the waveform of artery, the pulse wave components of the vein may overlap with the pulse wave components of the artery and may influence the same. Regarding this, according to the illustrative embodiment, the correlation coefficients $R1$ between the extracted pulse wave components $b1, b2, b3, \dots$ and the representative pulse wave component $a1$, which is the typical pulse wave of the artery, are calculated and the pulse wave component having low correlativity (a ratio that the pulse wave component of the vein overlaps is high) is excluded to improve the reliability of the respiratory variation on the waveform of artery. In this case, the pulse wave component having low correlativity is excluded based on the correlation coefficients $R1$ between the extracted pulse wave components $b1, b2, b3, \dots$ obtained by one-time blood pressure measurement and the representative pulse wave component $a1$. Therefore, it is possible to obtain the respiratory variation on the waveform of artery by using the pulse wave components having higher relativity, as compared to a configuration where the respective blood pressures and the respiratory variation on the waveform of artery are obtained by measurements of separate measuring processes or by mounting the cuff 2 to separate regions, for example. Thereby, it is possible to obtain the respiratory variation on the waveform of artery having high reliability, so that it is possible to assess the correct hemodynamics.

[0049] Also, since the mean venous pressure is obtained during the depressurization process of the cuff pressure, it is possible to observe the pulse wave components of the vein while gradually decreasing the pulse wave components of the arterial pressure. For this reason, it is possible to easily detect an amplitude variation

in the pulse wave components of the vein, so that it is possible to correctly obtain the mean venous pressure. Also, since the cuff pressure is stepwise decreased, the electromagnetic valve less influences, as compared to a configuration where the cuff pressure is continuously decreased, so that it is possible to more correctly obtain the mean venous pressure.

[0050] In the meantime, for some subjects being tested having the low diastolic blood pressure, even though the cuff pressure is reduced, the pulse wave components of the artery may remain without being all eliminated and thus influence the mean venous pressure. Therefore, according to the illustrative embodiment, the correlation coefficients $R2$ between the extracted pulse wave components $c1, c2, c3, \dots$ and the representative pulse wave component $a1$, which is a typical pulse wave of the artery, are calculated and the pulse wave component having high correlativity (a ratio that the pulse wave component of the artery overlaps is high) is excluded based on the correlation coefficients $R2$. In this case, the pulse wave component having high correlativity is excluded based on the correlation coefficients $R2$ between the pulse wave components $c1, c2, c3, \dots$ obtained by one-time blood pressure measurement and the representative pulse wave component $a1$. Therefore, it is possible to obtain the mean venous pressure by using the pulse wave components having higher relativity, as compared to a configuration where the respective blood pressures and the mean venous pressure are obtained by measurements of separate measuring processes or by mounting the cuff 2 to separate regions and the pulse wave component having high correlativity is excluded based on the correlation coefficients $R2$ of the pulse wave components extracted therefrom, for example. Thereby, it is possible to obtain the mean venous pressure less influenced by the arterial pressure and having high reliability, so that it is possible to assess the correct hemodynamics.

[0051] Also, since the respective parameters can be obtained in the non-invasive manner and the series of measuring processes are completed in a short time such as about 140 seconds, it is possible to considerably reduce the burden of the subject being tested.

[0052] Also, since the relativity between the obtained values of the respiratory variation on the waveform of artery and the obtained values of the venous pressure is displayed as the two-dimensional graph on the display unit 8, a medical staff who is monitoring the biological information can comprehensively determine the two parameters of the respiratory variation on the waveform of artery and the venous pressure by seeing the display unit 8, thereby correctly assessing the hemodynamics of the subject being tested. Furthermore, since the threshold lines m, n , which are the criteria for determining the values of the respiratory variation on the waveform of artery and the values of the mean venous pressure, are displayed on the two-dimensional graph, the medical staff who is monitoring the biological information can easily assess the hemodynamics.

[0053] In the meantime, the present invention is not limited to the above illustrative embodiment and can be appropriately modified and improved. In addition, the materials, shapes, sizes, numerical values, forms, the numbers, arrangement places and the like of the respective constitutional elements in the above illustrative embodiment are arbitrary and are not particularly limited inasmuch as the present invention can be implemented.

[0054] For example, when the pulse wave components of the artery overlap with the pulse wave components of the vein at the time that the value of the diastolic blood pressure is low and the mean venous pressure is obtained, the pulse wave components of the artery detected at the time that the respiratory variation on the waveform of artery is obtained are subtracted from the overlapping pulse wave components. Thereby, it is possible to calculate the correct correlation coefficients R2, thereby improving the reliability of the mean venous pressure. Likewise, when the pulse wave components of the vein overlap with the pulse wave components of the artery at the time that the value of the diastolic blood pressure is low and the respiratory variation on the waveform of artery is obtained, the pulse wave components of the artery detected upon the calculation of the mean venous pressure are subtracted after the calculation of the mean venous pressure is completed. Thereby, it is possible to calculate the correct correlation coefficients R2, thereby improving the reliability of the respiratory variation on the waveform of artery.

[0055] Also, the reduction of the cuff pressure during the time period C for which the mean venous pressure is obtained is not limited to the stepwise reduction and the cuff pressure may be continuously reduced. Further, the cuff pressure may be stepwise or continuously increased to obtain the mean venous pressure during the pressurization process (the second process). Also, when calculating the correlation coefficient R2 of the pulse wave components at the time that the mean venous pressure is obtained, the pulse wave component of the mean blood pressure is used as the representative pulse wave component a1. However, for example, any one of the pulse wave components b1, b2, b3, ... having the highest correlativity with the representative pulse wave component a1 may be used as the representative pulse wave component when measuring the respiratory variation on the waveform of artery. In this case, since the pulse wave components b1, b2, b3 are closer upon the measurement of the mean venous pressure in the elapsed measuring time, it is possible to increase the correctness of the correlation coefficient R2.

[0056] Also, when measuring the mean venous pressure, a representative pulse may be determined from the pulse wave components of the artery during the process of measuring the respiratory variation on the waveform of artery, a correlativity between the representative pulse and a pulse wave component for obtaining the mean venous pressure may be obtained to determine the pulse wave component for obtaining the mean venous pres-

sure. Further, the sequence of measuring the pulse wave components may not be the order of the arterial pressure, the respiratory variation on the waveform of artery and the mean venous pressure. For example, the pulse wave components may be measured in order of the mean venous pressure, the respiratory variation on the waveform of artery and the arterial pressure. Also, only the respiratory variation on the waveform of artery and mean venous pressure may be measured.

Claims

1. A blood pressure measuring apparatus (1) comprising:

a pressure control unit (3) that controls an applied pressure applied to a region of a living body in which a vein and artery exist by a cuff (2) mountable to the region;
a detection unit (4) that detects pressure waveforms in which pulse wave components from the region overlap with the applied pressure; and
an analysis unit (5) that obtains a respiratory variation on the waveform of artery and a venous pressure based on the pressure waveforms detected by the detection unit (4) through one-time blood pressure measurement,
wherein the analysis unit (5) obtains:

the respiratory variation on the waveform of artery based on data of a first pressure waveform of the pressure waveforms in a first process, in which the applied pressure is kept at a constant pressure by the pressure control unit (3); and
the venous pressure based on data of a second pressure waveform of the pressure waveforms in a second process in which the applied pressure is decreased or increased by the pressure control unit (3), and the data of the first pressure waveform in the first process.

2. The blood pressure measuring apparatus (1) according to claim 1, wherein the applied pressure in the first process is equal to or lower than a diastolic blood pressure and within a range which does not include a pulse wave component of the vein in the pulse wave components.
3. The blood pressure measuring apparatus (1) according to claim 1 or 2, wherein the analysis unit (5) is configured to obtain the venous pressure based on the data of the pressure waveform in the second process when a correlativity between the data of the second pressure waveform in the second process and the data of the first pressure waveform in the

first process is low.

4. The blood pressure measuring apparatus (1) according to claim 1 or 2, wherein the analysis unit (5) is configured to obtain an arterial pressure by one-time blood pressure measurement and based on data of a third pressure waveform of the pressure waveforms in a third process, in which the applied pressure is increased or decreased by the pressure control unit (3). 5
10

5. The blood pressure measuring apparatus (1) according to claim 4, wherein the analysis unit (5) is configured to obtain the venous pressure based on the data of the second pressure waveform in the second process and the data of the third pressure waveform in the third process or the data of the first pressure waveform in the first process. 15

6. The blood pressure measuring apparatus (1) according to claim 5, wherein the analysis unit (5) is configured to obtain the venous pressure based on the data of the second pressure waveform in the second process when a correlativity between the data of the second pressure waveform in the second process and the data of the third pressure waveform in the third process or the data of the first pressure waveform in the first process is low. 20
25

7. The blood pressure measuring apparatus (1) according to any one of claims 1 to 6, further comprising: 30
 - a display unit (8); and
 - a display control unit (7) that controls the display unit (8), 35
 - wherein the display control unit (7) is configured to display a value of the obtained respiratory variation on the waveform of artery and a value of the obtained venous pressure with a two-dimensional graph on the display unit (8). 40

8. The blood pressure measuring apparatus (1) according to claim 7, wherein a determination criterion for determining the displayed value of the respiratory variation on the waveform of artery and the displayed value of the venous pressure is displayed on the two-dimensional graph. 45

9. A blood pressure measuring method for controlling an applied pressure applied to a region of a living body in which a vein and an artery exist by a cuff (2) mountable to the region, detecting pressure waveforms in which pulse wave components are overlapped with the applied pressure, and obtaining a on the waveform of artery of an arterial pressure and a venous pressure based on the detected pressure waveforms, the method comprising: 50
55

obtaining the respiratory variation on the waveform of artery based on data of a first pressure waveform of the pressure waveforms in a first process, in which the applied pressure is kept at a constant pressure, and
 obtaining the venous pressure based on data of a second pressure waveform of the pressure waveforms in a second process, in which the applied pressure is decreased or increased, and the data of the first pressure waveform, wherein the first process and the second process are performed by one-time blood pressure measurement.

FIG. 1

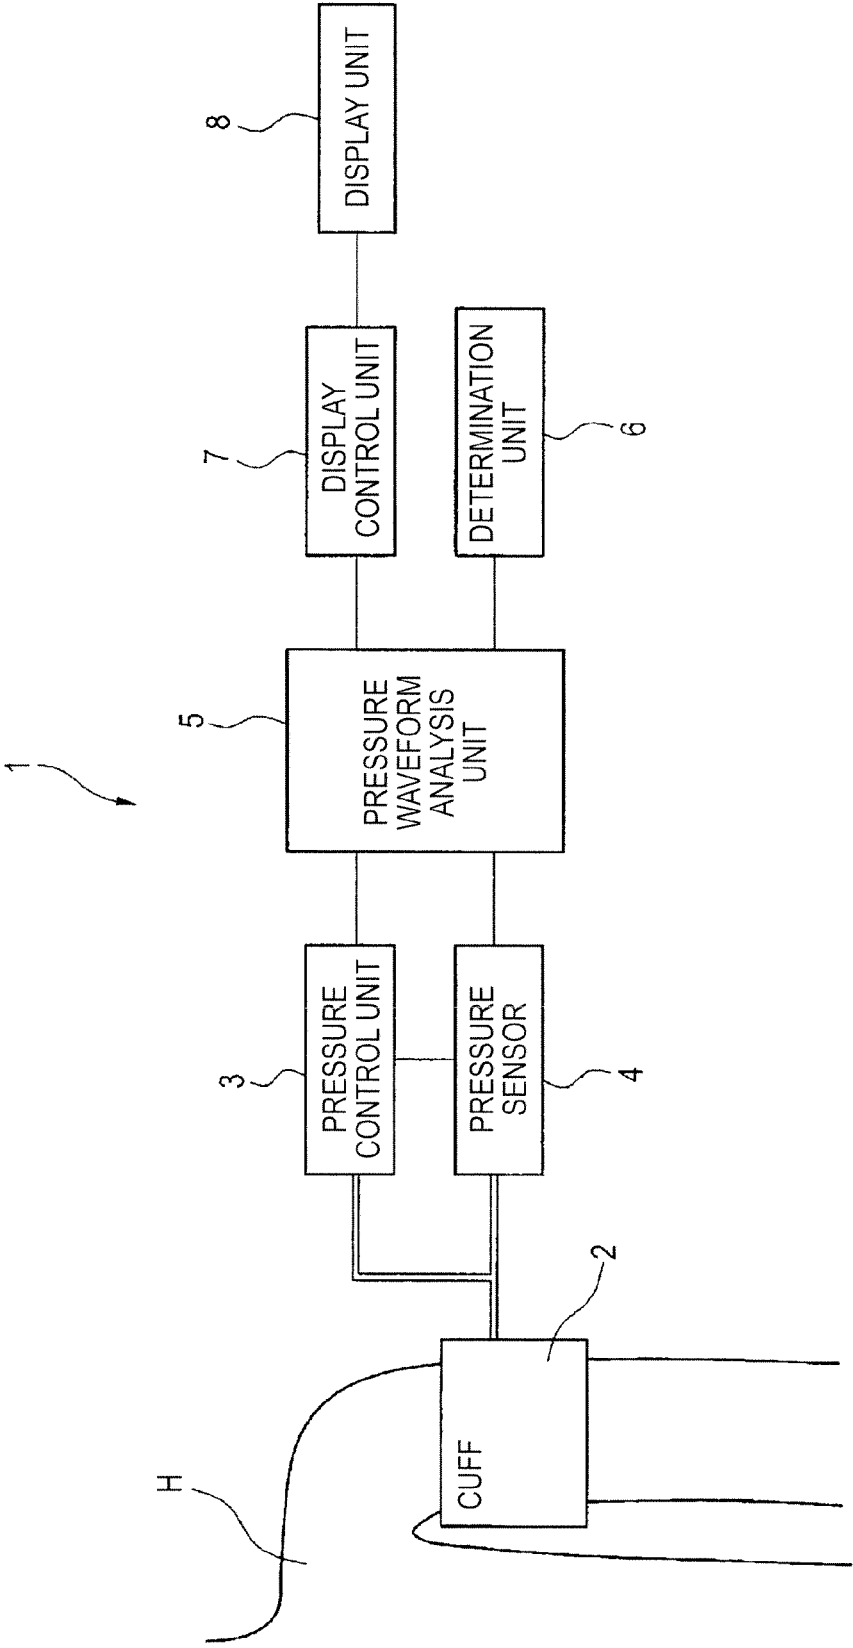
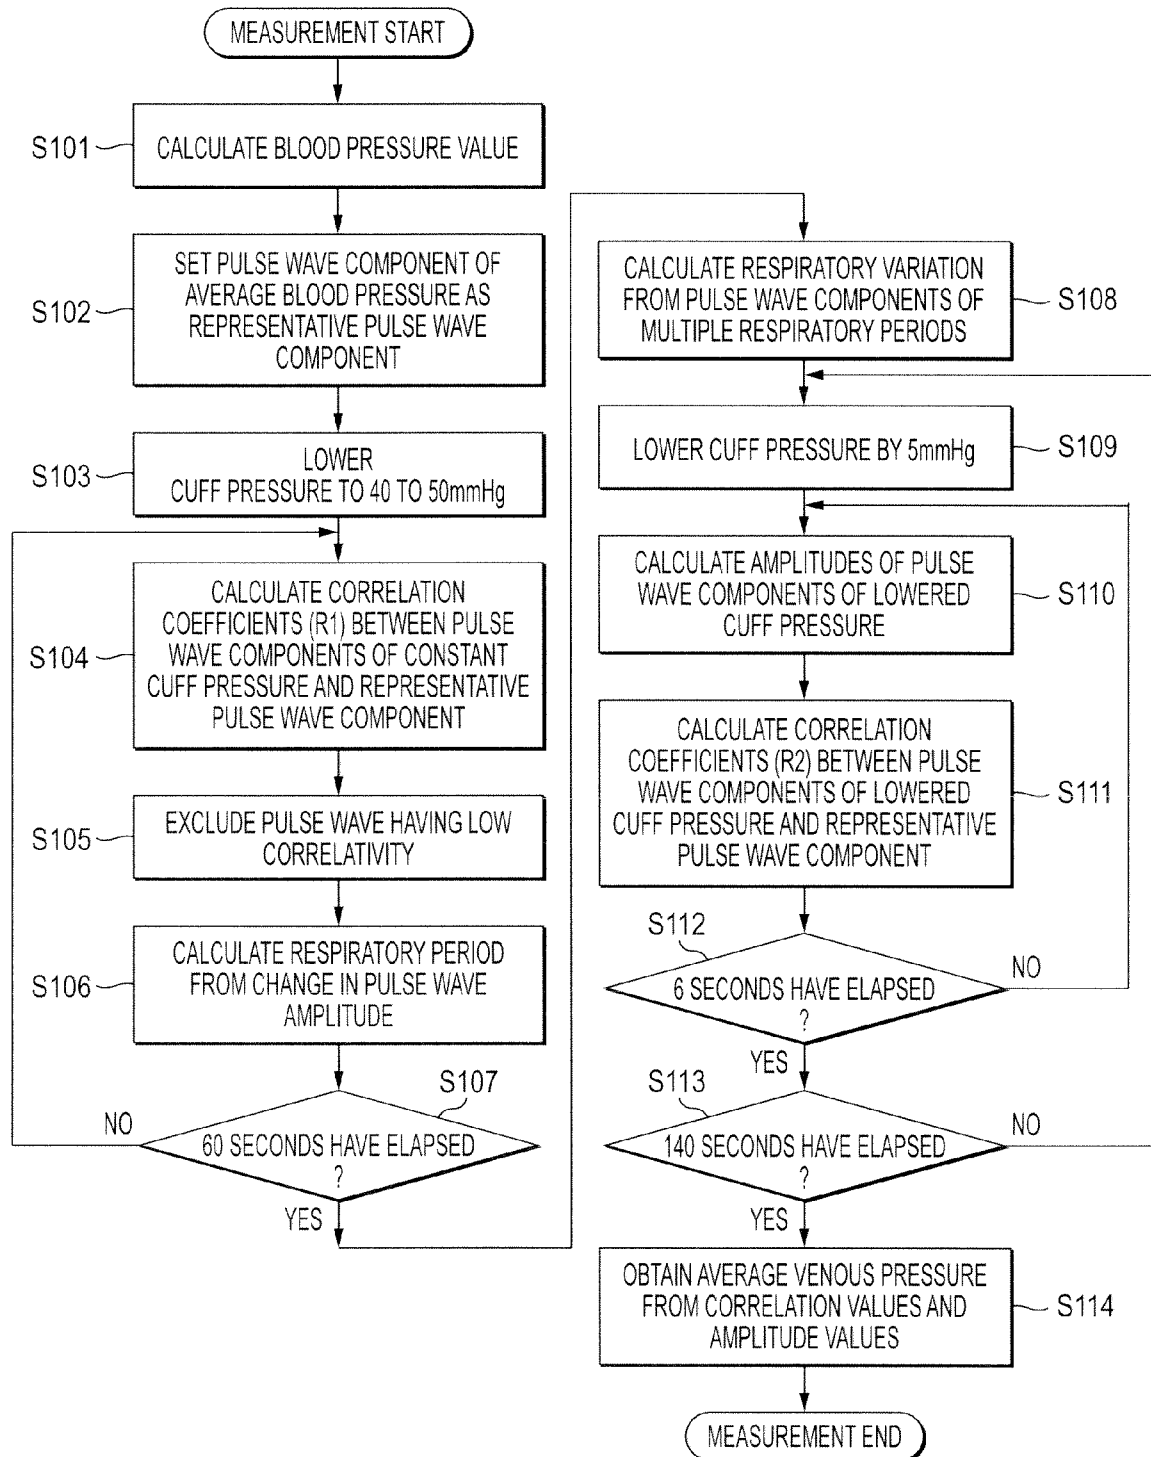


FIG. 2



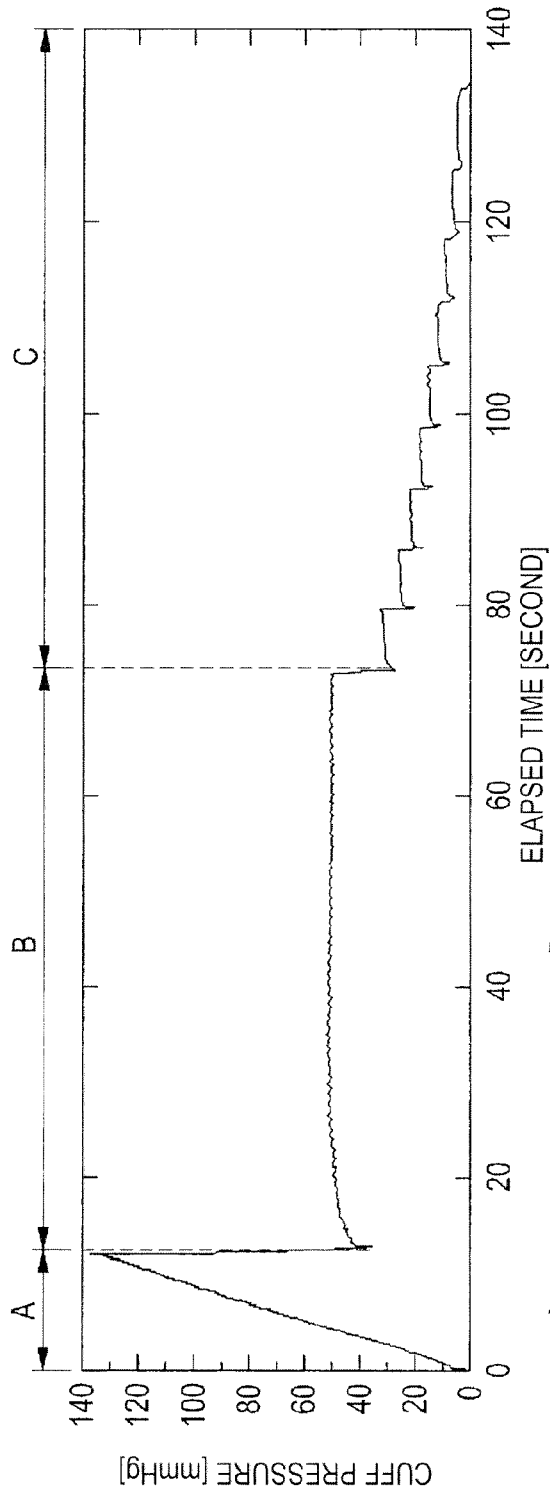


FIG. 3A

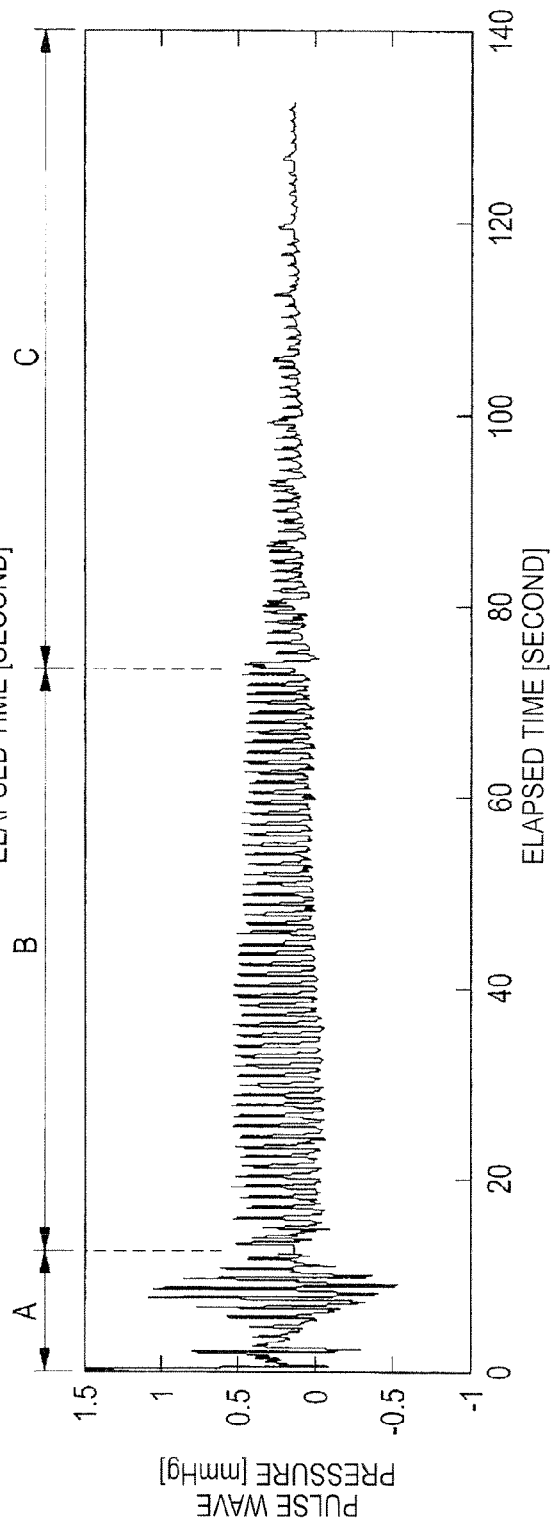
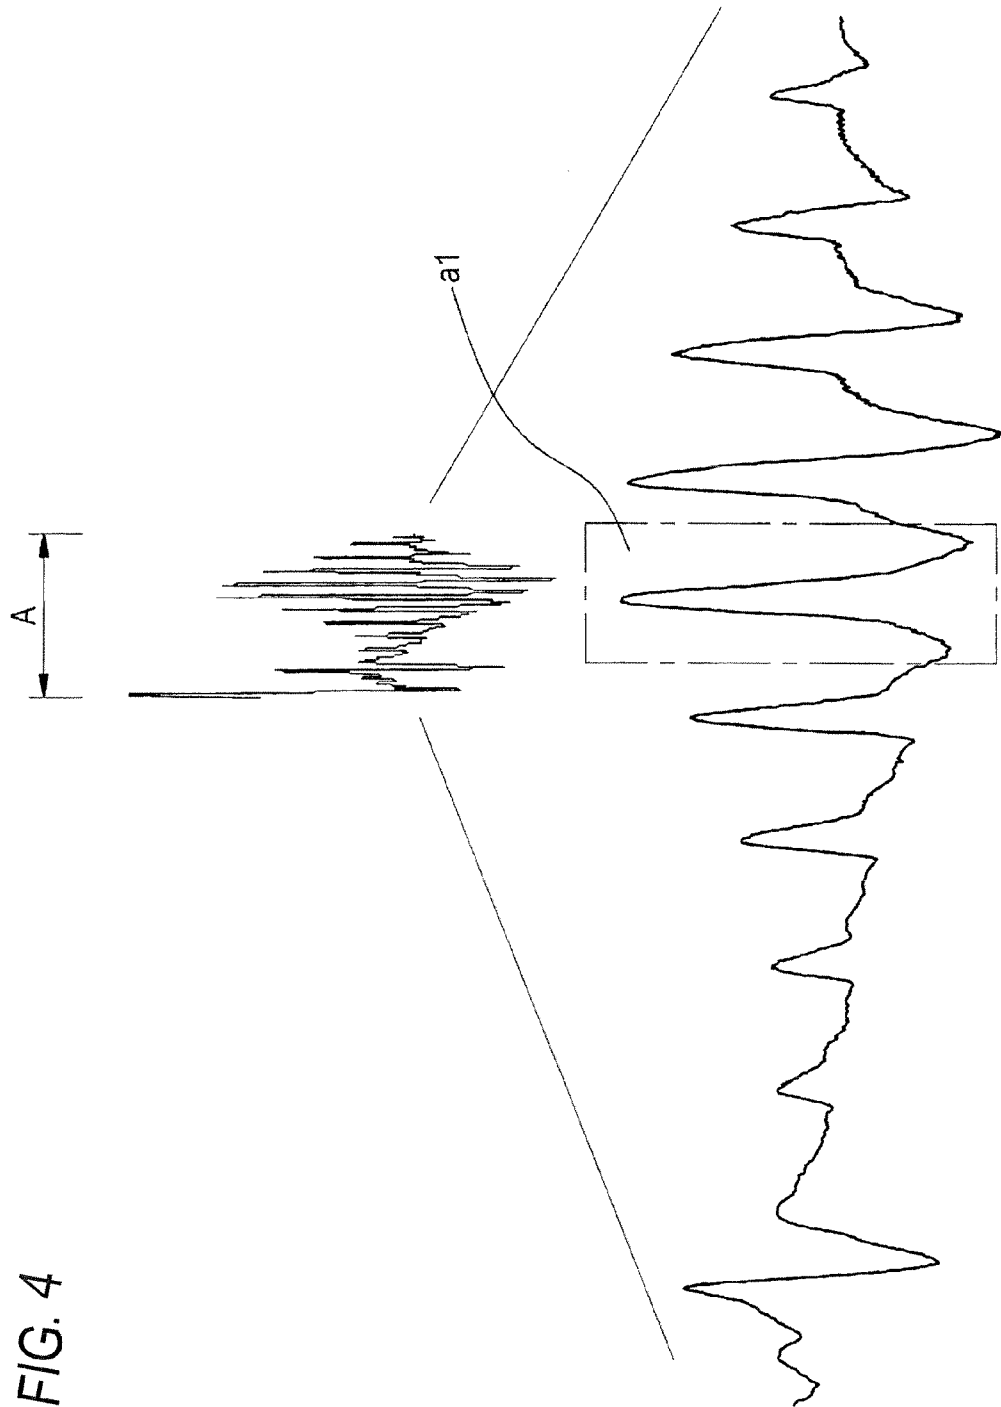


FIG. 3B



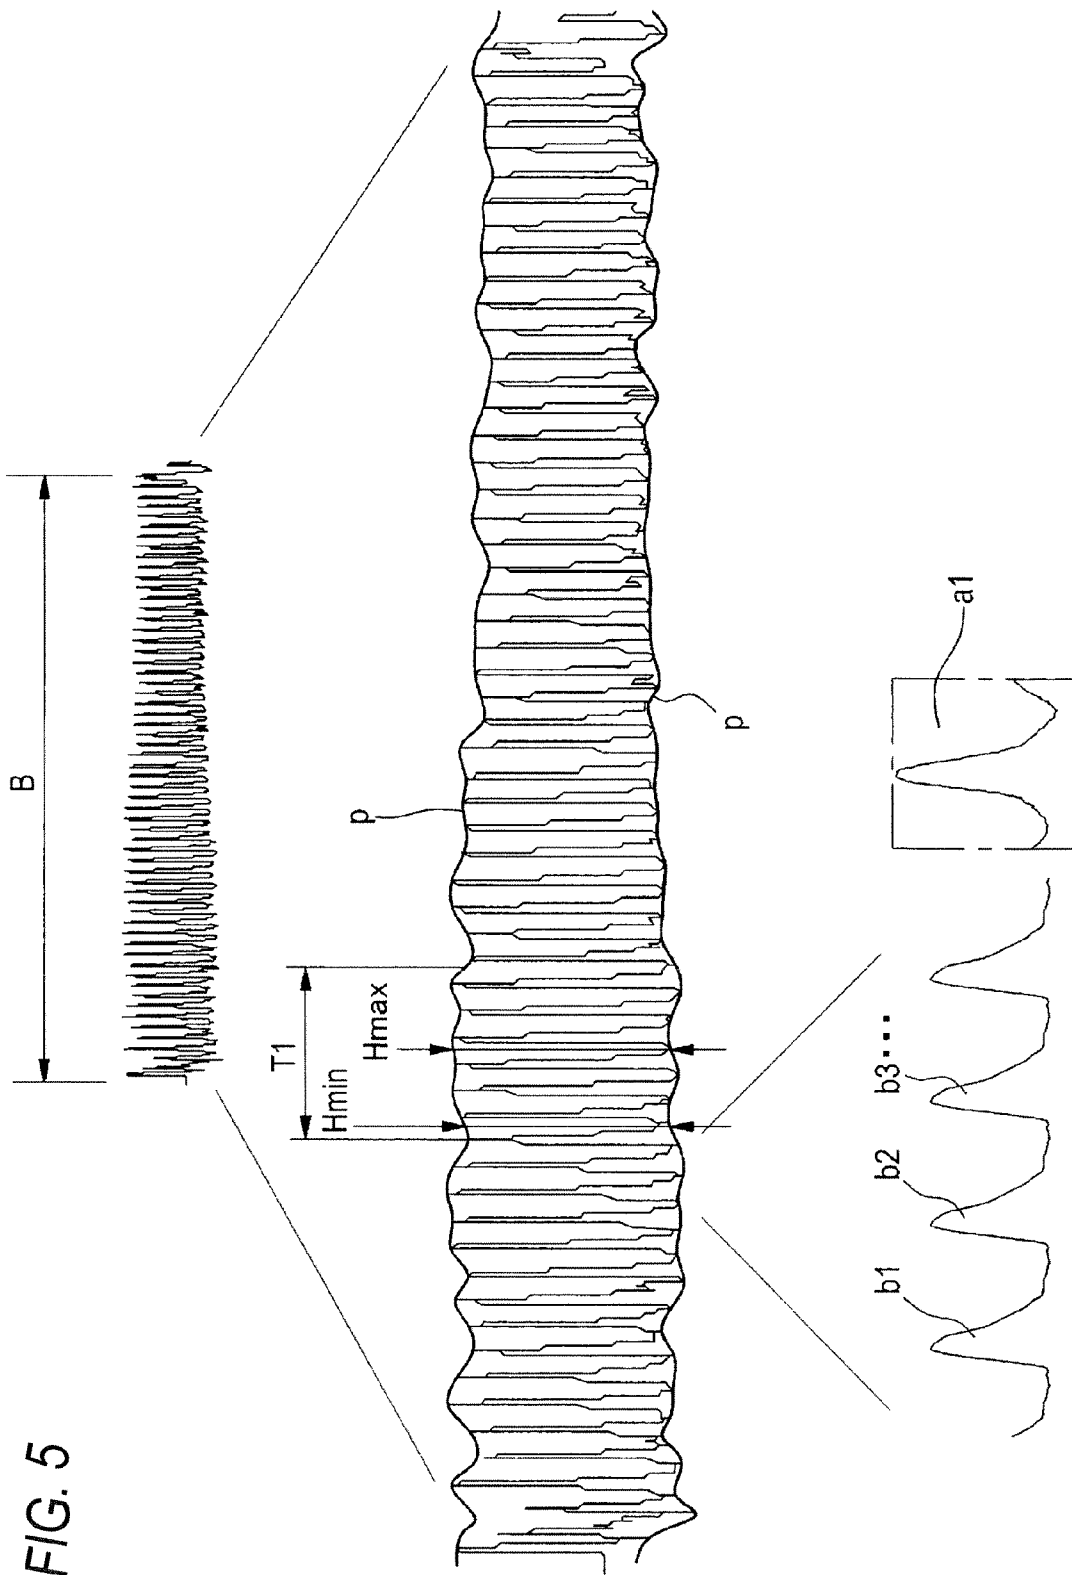


FIG. 6


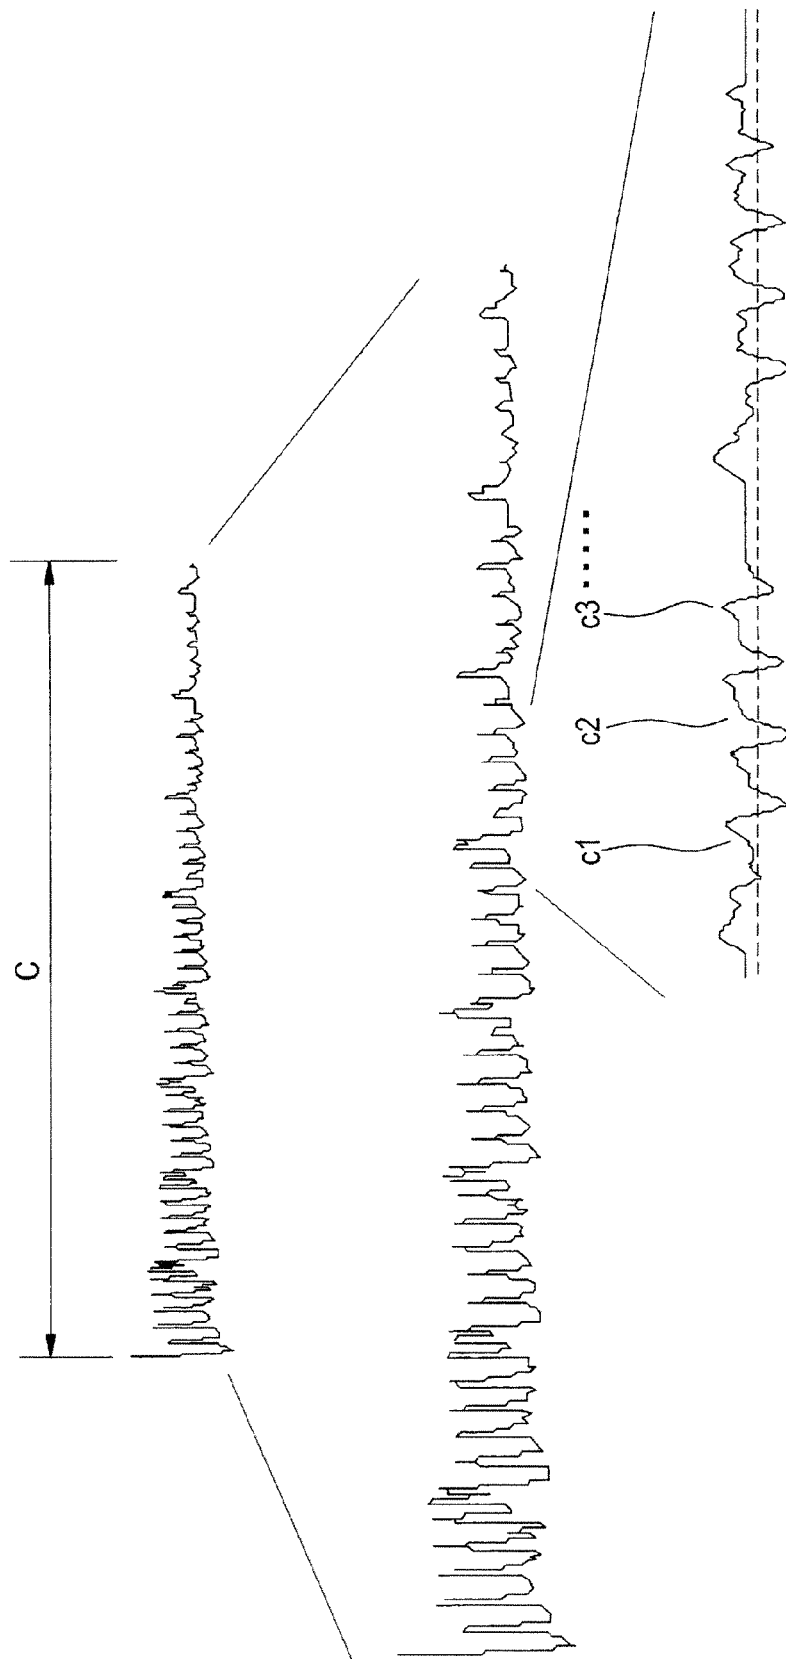


FIG. 7



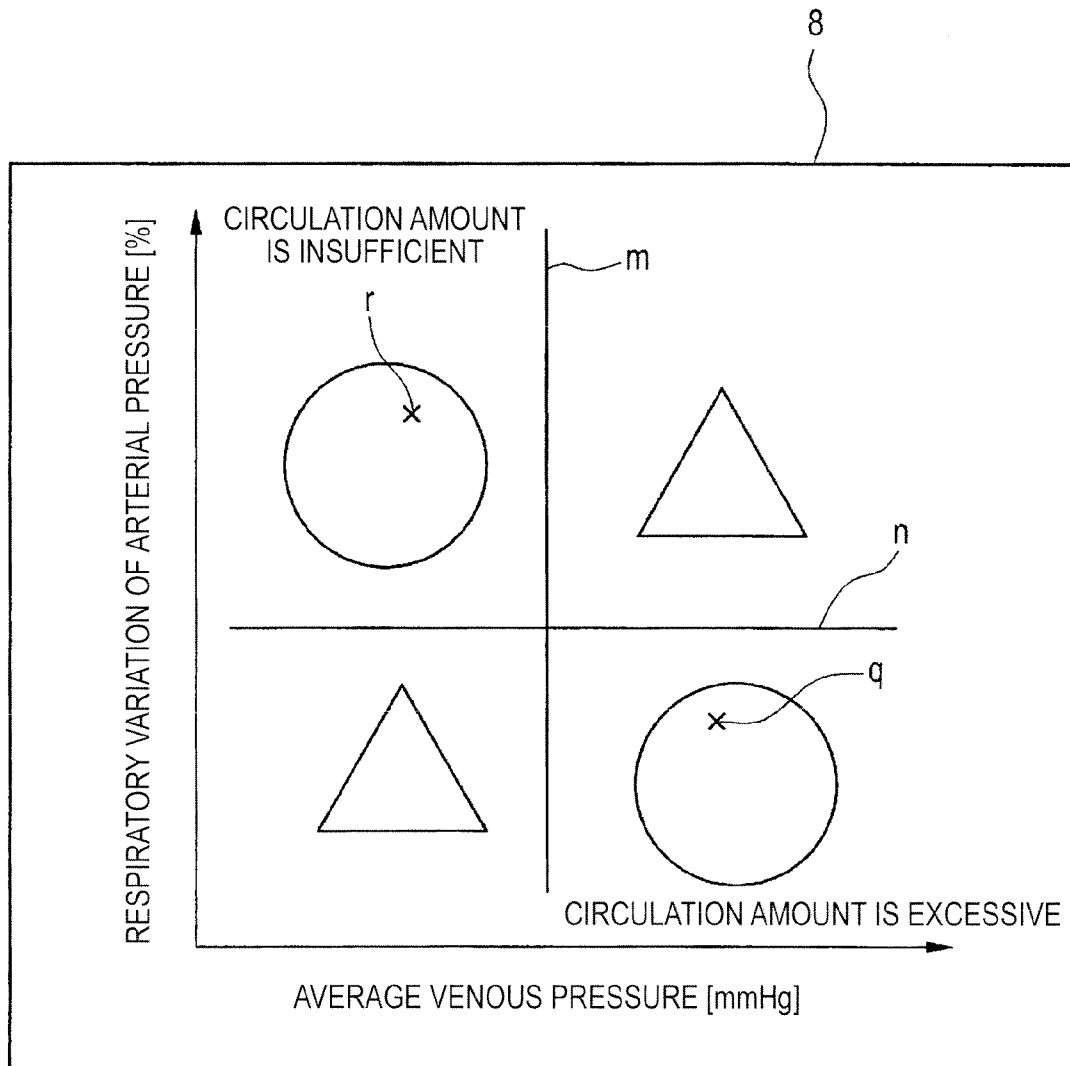

EUROPEAN SEARCH REPORT

Application Number
EP 15 15 5742

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 5 094 244 A (CALLAHAN WAYNE [US] ET AL) 10 March 1992 (1992-03-10)	1,2,4, 7-9	INV. A61B5/0205
Y	* abstract * * column 4, line 35 - column 13 * * column 10, line 31 - line 60 * * claim 12 * * the whole document *	3,5,6	A61B5/08 A61B5/021 A61B5/022 A61B5/00
Y	----- US 2012/253209 A1 (UKAWA TEIJI [JP] ET AL) 4 October 2012 (2012-10-04) * abstract; figures 9-11 * * paragraphs [0005], [0011] * * the whole document *	1-9	
Y,D	& JP 2012 205822 A (NIPPON KODEN KOGYO KK) 25 October 2012 (2012-10-25)	1-9	
Y	----- US 2010/324428 A1 (PFEIFFER ULRICH [DE]) 23 December 2010 (2010-12-23) * abstract * * paragraphs [0007] - [0015] * * the whole document *	1-9	
Y,D	& JP 2011 511686 A 14 April 2011 (2011-04-14)	1-9	TECHNICAL FIELDS SEARCHED (IPC) A61B
Y	----- US 2004/044290 A1 (WARD KEVIN R [US] ET AL) 4 March 2004 (2004-03-04) * abstract * * paragraphs [0020] - [0029] * * the whole document *	1-9	
	----- -/--		
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 23 July 2015	Examiner Furlan, Stéphane
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

1
EPO FORM 1503 03.82 (P04C01)



EUROPEAN SEARCH REPORT

Application Number
EP 15 15 5742

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	WARD K R ET AL: "A new noninvasive method to determine central venous pressure", RESUSCITATION, ELSEVIER, IE, vol. 70, no. 2, 1 August 2006 (2006-08-01), pages 238-246, XP027919915, ISSN: 0300-9572 [retrieved on 2006-08-01] * abstract * * the whole document *	1-9	
A	KEVIN R. WARD ET AL: "A NOVEL NONINVASIVE IMPEDANCE-BASED TECHNIQUE FOR CENTRAL VENOUS PRESSURE MEASUREMENT", SHOCK, vol. 33, no. 3, 1 March 2010 (2010-03-01), pages 269-273, XP055204162, ISSN: 1073-2322, DOI: 10.1097/SHK.0b013e3181ab9b9b * the whole document *	1-9	
			TECHNICAL FIELDS SEARCHED (IPC)
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 23 July 2015	Examiner Furlan, Stéphane
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 15 15 5742

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

23-07-2015

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5094244 A	10-03-1992	NONE	
US 2012253209 A1	04-10-2012	EP 2505133 A1 JP 5694032 B2 JP 2012205822 A US 2012253209 A1	03-10-2012 01-04-2015 25-10-2012 04-10-2012
US 2010324428 A1	23-12-2010	DE 102008008840 A1 EP 2252201 A1 JP 5337821 B2 JP 2011511686 A US 2010324428 A1 WO 2009100927 A1	24-09-2009 24-11-2010 06-11-2013 14-04-2011 23-12-2010 20-08-2009
US 2004044290 A1	04-03-2004	NONE	

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2012205822 A [0003] [0004]
- JP 2011511686 A [0003] [0004]

专利名称(译)	血压测量装置和血压测量方法		
公开(公告)号	EP2912996A1	公开(公告)日	2015-09-02
申请号	EP2015155742	申请日	2015-02-19
[标]申请(专利权)人(译)	日本光电工业株式会社		
申请(专利权)人(译)	广岛大学 日本光电公司		
当前申请(专利权)人(译)	广岛大学 日本光电公司		
[标]发明人	KAWAMOTO MASASHI SAEKI NOBORU NAKAMURA RYUJI UKAWA TEIJI TAKAYANAGI TSUNEO MORIMOTO HARUKA		
发明人	KAWAMOTO, MASASHI SAEKI, NOBORU NAKAMURA, RYUJI UKAWA, TEIJI TAKAYANAGI, TSUNEO MORIMOTO, HARUKA		
IPC分类号	A61B5/0205 A61B5/08 A61B5/021 A61B5/022 A61B5/00		
CPC分类号	A61B5/022 A61B5/0205 A61B5/02108 A61B5/02225 A61B5/0816 A61B5/7203 A61B5/7221 A61B5/7278 A61B5/742		
代理机构(译)	BREVALEX		
审查员(译)	他stÉphane		
优先权	2014038510 2014-02-28 JP		
外部链接	Espacenet		

摘要(译)

血压测量装置 (1) 包括压力控制单元 (3)，该压力控制单元 (3) 通过可安装到该区域的袖带 (2) 控制施加到活体区域的施加压力，其中静脉和动脉存在于该区域中，检测单元 (4) 检测来自该区域的脉搏波分量与施加的压力重叠的压力波形，以及基于由检测到的压力波形获得动脉波形和静脉压的呼吸变化的分析单元 (5)。检测单元 (4) 通过一次性血压测量。分析单元 (5) 基于第一过程中的第一压力波形的数据获得动脉波形的呼吸变化，并且基于第二过程中的第二压力波形的数据和第一过程的数据获得静脉压。压力波形。

FIG. 1

