



(11) **EP 3 456 246 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
**20.03.2019 Bulletin 2019/12**

(51) Int Cl.:  
**A61B 5/00 (2006.01) A61B 5/0452 (2006.01)**  
**A61B 5/0456 (2006.01)**

(21) Application number: **18153347.2**

(22) Date of filing: **25.01.2018**

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**  
Designated Extension States:  
**BA ME**  
Designated Validation States:  
**MA MD TN**

- **Banerjee, Rohan**  
700160 Kolkata, West Bengal (IN)
- **Choudhury, Anirban Dutta**  
700160 Kolkata, West Bengal (IN)
- **Ukil, Arijit**  
700160 Kolkata, West Bengal (IN)
- **Bandyopadhyay, Soma**  
700160 Kolkata, West Bengal (IN)
- **Pal, Arpan**  
700160 Kolkata, West Bengal (IN)
- **Khandelwal, Sundeep**  
201 309 Noida, Uttar Pradesh (IN)
- **Singh, Rituraj**  
700160 Kolkata, West Bengal (IN)

(30) Priority: **19.09.2017 IN 201721033210**

(71) Applicant: **Tata Consultancy Services Limited Maharashtra (IN)**

- (72) Inventors:
- **Datta, Shreyasi**  
700160 Kolkata, West Bengal (IN)
  - **Puri, Chetanya**  
700160 Kolkata, West Bengal (IN)
  - **Mukherjee, Ayan**  
700160 Kolkata, West Bengal (IN)

(74) Representative: **Goddar, Heinz J. Boehmert & Boehmert Anwaltspartnerschaft mbB Pettenkoflerstrasse 22 80336 München (DE)**

(54) **A CASCADED BINARY CLASSIFIER FOR IDENTIFYING RHYTHMS IN A SINGLE-LEAD ELECTROCARDIOGRAM (ECG) SIGNAL**

(57) Current technologies analyze electrocardiogram (ECG) signals for a long duration, which is not always a practical scenario. Moreover the current scenarios perform a binary classification between normal and Atrial Fibrillation (AF) only, whereas there are many abnormal rhythms apart from AF. Conventional systems/methods have their own limitations and may tend to misclassify ECG signals, thereby resulting in an unbalanced multi-label classification problem. Embodiments of the present disclosure provide systems and methods that are robust and more efficient for classifying rhythms for example, normal, AF, other abnormal rhythms and noisy ECG recordings by implementing a spectrogram based noise removal that obtains clean ECG signal from an acquired single-lead ECG signal, an optimum feature selection at each layer of classification that selects optimum features from a pool of extracted features, and a multi-layer cascaded binary classifier that identifies rhythms in the clean ECG signal at each layer of the classifier.

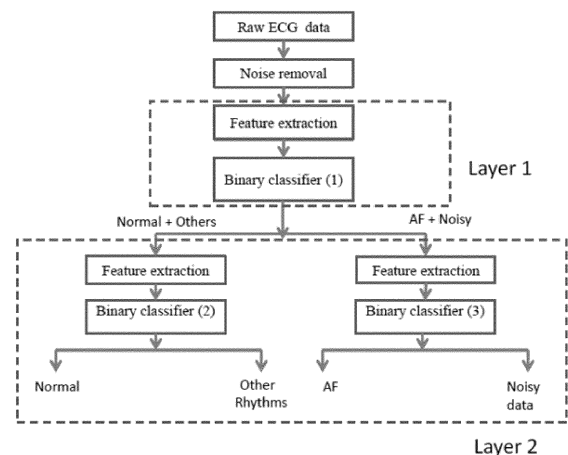


FIG. 3

## Description

### CROSS-REFERENCE TO RELATED APPLICATIONS AND PRIORITY

**[0001]** This patent application claims priority to India Patent Application 201721033210, filed on September 19, 2017.

### TECHNICAL FIELD

**[0002]** The disclosure herein generally relate to electrocardiogram (ECG) signal analysis, and, more particularly, to systems and methods for identifying rhythms in a single-lead electrocardiogram (ECG) signal using a cascaded binary classifier.

### BACKGROUND

**[0003]** Atrial Fibrillation (AF) is a common type of heart disease that leads to stroke, heart failure or other complications. Millions of people get affected by AF every year and the prevalence of the disease is likely to increase. Noninvasive detection of AF is a popular area of research for quite a long time. Irregularities in heart beat is considered to be the most common symptom of AF and can be traced in an ECG. However, being an episodic event an accurate detection of AF is not always trivial. Conventional AF detectors have been mostly of atrial activity analysis based or ventricular response analysis-based methods. The absence of P waves or the presence of f waves in the TQ interval are searched in atrial activity analysis-based AF detectors. On the other hand, time, frequency and morphological features are extracted from RR intervals to identify the heart beat irregularity in ventricular response analysis based methods. However, the traditional methods have certain limitations regarding real time deployments, firstly, most of them are validated on clinically accepted multiples of lead ECG signals, recorded for a relatively longer duration. Secondly, algorithms are mostly applied on carefully selected clean data. However, in practical scenario, ECG signals are often noisy in nature. Thirdly, size of the test dataset may often not be adequate for making a conclusion (or decision) thereby result in misclassification. Lastly, most traditional or conventional methods perform binary classification between AF and normal recordings only. However, there are many non-AF abnormal rhythms (e.g., tachycardia, bradycardia, arrhythmia etc..) which exhibit heart beat pattern similar to AF, however these non-AF abnormal rhythms are not considered for classification. Even if considered them in the dataset makes the classification task more challenging.

### SUMMARY

**[0004]** Embodiments of the present disclosure present technological improvements as solutions to one or more

of the above-mentioned technical problems recognized by the inventors in conventional systems. For example, in one aspect, a processor implemented method for identifying rhythms in a single-lead electrocardiogram (ECG) signal using a cascaded binary classifier is provided. The method comprising: acquiring, via one or more hardware processors, a single-lead electrocardiogram (ECG) signal that is recorded for a predefined time interval; applying in real-time, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal; extracting one or more features from the clean ECG signal; selecting, using an optimum feature selection technique, one or more optimum features from the one or more extracted features, wherein the optimum feature selection technique is at least one of a minimum redundancy maximum relevancy (mRMR) technique and a Maximal Information Coefficient (MIC) technique; and identifying based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms, a first set of abnormal rhythms, and a second set of abnormal rhythms in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal.

**[0005]** In an embodiment, the step of applying in real-time, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal may comprise: dividing in real-time, the acquired single-lead ECG signal into a plurality of windows; computing in real-time, a spectrogram of each of the plurality of windows; performing in real-time, a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold, wherein the dynamically computed threshold is based on a signal to noise ratio (SNR); determining in real-time, noise in at least a subset of the plurality of windows based on the comparison; and extracting the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows.

**[0006]** In an embodiment, the noise is determined in the at least a subset of the plurality of windows when each window from the subset have power that is greater than a threshold power.

**[0007]** In another aspect, a system for identifying rhythms in a single-lead electrocardiogram (ECG) signal using a cascaded binary classifier is provided. The system comprising: a memory storing instructions; one or more communication interfaces; and one or more hardware processors coupled to the memory via the one or more communication interfaces, wherein the one or more hardware processors are configured by the instructions to: acquire a single-lead electrocardiogram (ECG) signal that is recorded for a predefined time interval; apply in real-time, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal; extract one or more features from the clean ECG signal; select, using an optimum feature selection technique, one or more optimum features from

the one or more extracted features, wherein the optimum feature selection technique is at least one of a minimum redundancy maximum relevancy (mRMR) technique and a Maximal Information Coefficient (MIC) technique; and identify based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms, a first set of abnormal rhythms, and a second set of abnormal rhythms in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal.

**[0008]** In an embodiment, the clean ECG signal is extracted by applying in real-time, the spectrogram based noisy data removal technique on the acquired single-lead ECG signal by: dividing in real-time, the acquired single-lead ECG signal into a plurality of windows; computing in real-time, a spectrogram of each of the plurality of windows; performing in real-time, a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold, wherein the dynamically computed threshold is based on a signal to noise ratio (SNR); determining in real-time, noise in at least a subset of the plurality of windows based on the comparison; and extracting in real-time, the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows.

**[0009]** In an embodiment, noise is determined in the at least a subset of the plurality of windows when each window from the subset have power that is greater than a threshold power.

**[0010]** In yet another aspect, one or more non-transitory machine readable information storage mediums comprising one or more instructions is provided. The one or more instructions which when executed by one or more hardware processors causes acquiring, via the one or more hardware processors, a single-lead electrocardiogram (ECG) signal that is recorded for a predefined time interval; applying in real-time, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal; extracting one or more features from the clean ECG signal; selecting, using an optimum feature selection technique, one or more optimum features from the one or more extracted features, wherein the optimum feature selection technique is at least one of a minimum redundancy maximum relevancy (mRMR) technique and a Maximal Information Coefficient (MIC) technique; and identifying based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms, a first set of abnormal rhythms, and a second set of abnormal rhythms in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal.

**[0011]** In an embodiment, the step of applying, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal may comprise: dividing the acquired single-lead ECG signal into a plurality of windows; computing

a spectrogram of each of the plurality of windows; performing a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold, wherein the dynamically computed threshold is based on a signal to noise ratio (SNR); determining noise in at least a subset of the plurality of windows based on the comparison; and extracting the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows.

**[0012]** In an embodiment, the noise is determined in the at least a subset of the plurality of windows when each window from the subset have power that is greater than a threshold power.

**[0013]** It is to be understood that both the foregoing general description and the following detailed description are exemplary and explanatory only and are not restrictive of the invention, as claimed.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0014]** The accompanying drawings, which are incorporated in and constitute a part of this disclosure, illustrate exemplary embodiments and, together with the description, serve to explain the disclosed principles:

FIG. 1 illustrates an exemplary block diagram of a system for identifying rhythms in a single-lead electrocardiogram (ECG) signal using a cascaded binary classifier in accordance with an embodiment of the present disclosure.

FIG. 2 illustrates an exemplary flow diagram of a method for identifying rhythms in the single-lead electrocardiogram (ECG) signal using the cascaded binary classifier executed by the system of FIG. 1 in accordance with an embodiment of the present disclosure.

FIG. 3 illustrates an exemplary architecture of the system of FIG. 1 in accordance with an example embodiment of the present disclosure.

FIG. 4 illustrates a graphical representation of a spectrogram based noise removal in accordance with an example embodiment of the present disclosure.

FIG. 5 illustrates a graphical representation of PQRST detection on the single-lead ECG signal in accordance with an example embodiment of the present disclosure.

#### DETAILED DESCRIPTION OF EMBODIMENTS

**[0015]** Exemplary embodiments are described with reference to the accompanying drawings. In the figures, the left-most digit(s) of a reference number identifies the figure in which the reference number first appears. Wherever convenient, the same reference numbers are used throughout the drawings to refer to the same or like parts. While examples and features of disclosed principles are described herein, modifications, adaptations, and other

implementations are possible without departing from the spirit and scope of the disclosed embodiments. It is intended that the following detailed description be considered as exemplary only, with the true scope and spirit being indicated by the following claims.

**[0016]** As mentioned above (in the background section), traditional (or conventional systems and/or methods) have their own limitations and hence may tend to misclassify ECG signals thereby resulting in an unbalanced multi-label classification problem. Embodiments of the present disclosure provide systems and methods for a robust and more efficient technique for classifying normal, AF, other abnormal rhythms and noisy ECG recordings. More particularly, embodiments of the present disclosure provide systems and methods for identifying rhythms in a single-lead electrocardiogram (ECG) signal using a cascaded binary classifier. Embodiments of the present disclosure provide experiment results of a diverse ECG dataset (provided in Physionet challenge 2017) that was used for internal performance evaluation and creating the training models. Information regarding individual recordings were not available regarding the other rhythms in the dataset as all non AF related abnormal rhythms are clubbed together to form a single class. The embodiments of the present disclosure identify rhythms in a single-lead electrocardiogram (ECG) signal by implementing 1) a multi-layer cascaded binary classifier instead of a single multi-class classifier, 2) front end noise removal and 3) optimum feature selection at each layer of classification from a pool of features.

**[0017]** Referring now to the drawings, and more particularly to FIGS. 1 through 5, where similar reference characters denote corresponding features consistently throughout the figures, there are shown preferred embodiments and these embodiments are described in the context of the following exemplary system and/or method.

**[0018]** FIG. 1 illustrates an exemplary block diagram of a system 100 for identifying rhythms in a single-lead electrocardiogram (ECG) signal using a cascaded binary classifier in accordance with an embodiment of the present disclosure. In an embodiment, the system 100 includes one or more processors 104, communication interface device(s) or input/output (I/O) interface(s) 106, and one or more data storage devices or memory 102 operatively coupled to the one or more processors 104. The one or more processors 104 may be one or more software processing modules and/or hardware processors. In an embodiment, the hardware processors can be implemented as one or more microprocessors, microcomputers, microcontrollers, digital signal processors, central processing units, state machines, logic circuitries, and/or any devices that manipulate signals based on operational instructions. Among other capabilities, the processor(s) is configured to fetch and execute computer-readable instructions stored in the memory. In an embodiment, the device 100 can be implemented in a variety of computing systems, such as laptop computers, note-

books, hand-held devices, workstations, mainframe computers, servers, a network cloud and the like.

**[0019]** The I/O interface device(s) 106 can include a variety of software and hardware interfaces, for example, a web interface, a graphical user interface, and the like and can facilitate multiple communications within a wide variety of networks N/W and protocol types, including wired networks, for example, LAN, cable, etc., and wireless networks, such as WLAN, cellular, or satellite. In an embodiment, the I/O interface device(s) can include one or more ports for connecting a number of devices to one another or to another server.

**[0020]** The memory 102 may include any computer-readable medium known in the art including, for example, volatile memory, such as static random access memory (SRAM) and dynamic random access memory (DRAM), and/or non-volatile memory, such as read only memory (ROM), erasable programmable ROM, flash memories, hard disks, optical disks, and magnetic tapes. In an embodiment a database 108 can be stored in the memory 102, wherein the database 108 may comprise, but are not limited to information pertaining to signal(s) (e.g., raw data and clean signal), extracted features, optimum features, rhythm types (e.g., normal, abnormal, atrial fibrillation (AF), non-AF, training dataset, test dataset, and the like). In an embodiment, the memory 102 may store the classifiers (e.g., cascaded binary classifier(s)), one or more techniques, for example, spectrogram based noisy data removal technique, feature extraction technique, optimum feature selection technique(s) such as minimum redundancy maximum relevancy (mRMR) technique, and/or maximal Information Coefficient (MIC) technique and the like, which are executed by the one or more hardware processors 104 (or by the system 100) to perform the methodology described herein.

**[0021]** FIG. 2, with reference to FIG. 1, illustrates an exemplary flow diagram of a method for identifying rhythms in the single-lead electrocardiogram (ECG) signal using the cascaded binary classifier executed by the system 100 of FIG. 1 in accordance with an embodiment of the present disclosure. In an embodiment, the system(s) 100 comprises one or more data storage devices or the memory 102 operatively coupled to the one or more hardware processors 104 and is configured to store instructions for execution of steps of the method by the one or more processors 104. The system 100 stores values/information (and/or parameters, features, rhythms, and the like) associated with ECG signal(s). The steps of the method of the present disclosure will now be explained with reference to the components of the system 100 as depicted in FIGS. 1 and 3, and the flow diagram of FIG. 2. In an embodiment of the present disclosure, at step 202, the one or more hardware processors 104 acquire a single-lead electrocardiogram (ECG) signal (also referred hereinafter ECG signal or ECG waveform) that is recorded for a predefined time interval (e.g., a short duration - say 30 seconds). In an embodiment, the ECG signal may be recorded by using one or more wear-

able devices (for example, a smart watch, a health band, a fit band, and the like) or any other device that is capable of recording user's health data.

**[0022]** ECG signals, recorded using single-lead, non-medical grade equipment(s) are inherently noisy in nature. Body movement of the user during recording, voltage fluctuation of the sensor device or improper contact between subject body and the sensor electrodes can heavily corrupt the signals. A low frequency component is also present due breathing. Locating and discarding the noisy portions inside a signal is considered a prerequisite before feature extraction and classification. In an embodiment of the present disclosure, at step 204, the one or more hardware processors 104 apply in real-time, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal. In an embodiment of the present disclosure, the clean ECG signal is obtained by dividing the acquired single-lead ECG signal into a plurality of windows, computing a spectrogram of each of the plurality of windows, performing a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold, wherein the threshold is dynamically computed, determining noise in at least a subset of the plurality of windows based on the comparison, and extracting the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows. In an example embodiment, the steps of dividing, computing a spectrogram, performing a comparison, determining the noise are performed in real-time (or near real-time). In an embodiment, the threshold that is dynamically computed (or computed in real-time) is based on a signal to noise ratio (SNR). In an embodiment of the present disclosure, SNR is measured for all the windows in a recording (or an ECG signal). If the difference between maximum and minimum SNR values is 'n' times (e.g., say 3 times) the minimum value, x % of the maximum SNR is measured as threshold (e.g., say 75% of the maximum SNR is measured as threshold - which is also referred as dynamically computed threshold) for discarding the noisy windows. In other words, 75% of the maximum SNR may be referred as dynamically computed threshold. In an embodiment of the present disclosure, noise is determined in the at least a subset of the plurality of windows when each window from the subset have power (e.g., high spectral power) that is greater than a threshold power above 'X' Hertz (e.g., 50 Hz). In other words, each window from the subset comprising portion of the ECG signal (e.g., the acquired single-lead ECG signal) having power that exceeds the threshold power (also referred as threshold ' $P_x$ ') above 50 Hz are considered as noisy windows and thus discarded to obtain the clean ECG signal.

**[0023]** Important cardiac information, are typically stored within 20 Hz in ECG waveform/signal. Thus, following the spectrogram plot across time axis, if regions between successive RR intervals - wherein R is a point corresponding to the peak of the QRS complex (de-

scribed below) of the ECG signal; and RR is the interval between successive R's, having high spectral power above 50 Hz (as shown in graphical representation of FIG. 4) are located, that can be safely marked as noisy and are discarded before further processing. More particularly, FIG. 4, with reference to FIGS. 1 through 3, illustrates a graphical representation of a spectrogram based noise removal in accordance with an example embodiment of the present disclosure. Further, the clean signal is passed through a high pass filter (cut-off frequency 0.5 Hz) to remove the baseline movement of the signal. If more than X% (e.g., say 80%) of a certain waveform (e.g., the single-lead ECG signal) is discarded in this process, it is marked as noisy.

**[0024]** Identifying the differentiating feature set is considered the most important task of any classification problem. An accurate detection P, Q, R, S, T points are the primary requirement for an accurate feature extraction. The system 100 implements one or more techniques (e.g., a modified Pan-Tompkins technique) to identify QRS complex and R peaks. The QRS complex is a name for the combination of three of the graphical deflections seen on a typical electrocardiogram (EKG or ECG). It is usually the central and most visually obvious part of the tracing. It corresponds to the depolarization of the right and left ventricles of the human heart. In the subsequent stage. P, Q, S and T points are located, taking R peaks as reference points (as shown in FIG. 5). More particularly, FIG. 5, with reference to FIGS. 1 through 4, illustrates a graphical representation of PQRST detection on the single-lead ECG signal in accordance with an example embodiment of the present disclosure. In an embodiment of the present disclosure, at step 206, the one or more hardware processors 104 extract one or more features from the clean ECG signal. The one or more features from the clean ECG signal can be broadly classified into one or more categories illustrated by way of example below:

#### 40 **Morphological ECG features:**

**[0025]** The Morphological ECG features are derived from the PQRST points detected in an ECG waveform as depicted in FIG. 5. In an embodiment of the present disclosure, these features may comprise, but are not limited to, median, range and variance of the corrected QT interval (QTc), QR and QRS widths, slopes of QR, RS and ST intervals, depth of the Q and S points with respect to R, amplitude difference of the TR wave; ratio of the number of P waves to the number of R waves and distance of the ST segment crossing from the S point among others. These features are widely used by clinicians for identifying cardiac abnormalities. It is to be noted that some of these features are indicative of AF while others are for detecting the other abnormal rhythms. For example, in AF, P waves are often absent, hence the ratio of number of P waves to the number of R waves detected is supposed to be very small. Hence, this particular fea-

ture was selected by a layer 1 classifier of the cascaded binary classifier and the classifier 3 of layer 2 as depicted in FIG. 3, however, was not selected for the classifier 2 of layer 2. More particularly, FIG. 3, with reference to FIGS. 1-2, illustrates an exemplary architecture of the system 100 of FIG. 1 in accordance with an example embodiment of the present disclosure.

#### AF features:

**[0026]** Several features are used to identify AF events. Irregular RR intervals is a very common symptom present in AF patients. There are several metrics to identify the same. Several measurements have been proposed such as for example, AFEvidence, Original Count, Irregularity Evidence, Pace Count, Density Evidence, Anisotropy Evidence, AFEvidence from Lorentz plot of RR intervals. Certain features are derived from the inter beat intervals using Poincare plots also reported commending accuracy in identifying AF. Other features include approximate and sample entropy based features for AF detection as well as coefficient of variation of RR and delta RR intervals.

#### Heart Rate Variability features:

**[0027]** Several HRV related features are also incorporated in the proposed analysis. Features for example, pNNx (number of NN intervals above x, normalized by duration of recording, where x lies between 20 and 500 ms), SDNN (standard deviation of NN intervals), SDSD (standard deviation of successive differences) and normalized RMSSD (normalized root mean square of successive differences) were used in identifying cardiovascular diseases. Normalized spectral power of the RR interval time series within the frequency region of 0-0.04 Hz, 0.04-0.15 Hz and 0.15-0.5 Hz are also used.

#### Frequency features:

**[0028]** Embodiments of the present disclosure have also explored certain frequency domain features used in biomedical and other applications. Raw time signal is broken into small windows of 'n' seconds duration (e.g., 2 seconds duration) having Y% (e.g., 50%) overlapping using hamming window. Frequency analysis is performed by computing Short Time Fourier Transform (STFT) of each window. Extracted features comprise but are not limited to, mean spectral centroid, spectral roll-off, spectral flux along with normalized spectral power between 0-10 Hz and 10-20 Hz across all windows in a measurement.

#### Statistical features:

**[0029]** Statistical features comprise but are not limited to, mean, median, variance, range, kurtosis and skewness of RR intervals and the probability density estimate

(PDE) of the RR intervals and the delta RR intervals. Additionally, the number of peaks on the PDE of the RR and delta RR intervals along with the variation of energy in between the RR peaks were also used as features. The Shannon, Tsallis and Renyi entropy, Linear Predictive Coefficients (LPC) of the raw time series data were also used as extracted features by the embodiments of the present disclosure for identifying rhythms in the clean ECG signal.

#### Features for other abnormalities:

**[0030]** Embodiments of the present disclosure (or the system 100) attempt to extract some of the major features to detect arrhythmia or other non-AF related abnormalities present in an ECG signal. In an embodiment of the present disclosure, various features used are extracted using sliding window with 'x' peaks per window (e.g., 6 peaks per window) and its average RR interval, maximum of first difference of number of samples in the window with magnitude exceeding 'z' mV (e.g., where  $z = 0.1$  mV), the normalized power spectrum density (nPSD) of the window, etc. The heart rate was estimated using an adaptive frequency tracking algorithm (AMM) to derive the features as mean of RR interval, decrease of HR, max SPI index, average HR, abnormal HR etc.

#### Features for detecting noisy recordings:

**[0031]** There are several works that detect noise/motion artifacts in the different portions of the signals. However, there are times when the complete signal is not of any use (or very little use) for cardiac abnormality derivation. Embodiments of the present disclosure use domain dependent time and frequency features along with certain statistical features that exploit the rise and fall in the morphology of the ECG signal for improved noise detection. These features discriminate well between the regularities of the clean ECG signal versus the randomness in a noisy waveform.

**[0032]** Referring back to FIG. 2, In an embodiment of the present disclosure, at step 208, the one or more hardware processors 104 select, using an optimum feature selection technique, one or more optimum features from the one or more extracted features.

**[0033]** Feature selection often improves classification accuracy by removing the noisy (irrelevant) features and also reduces the computation time by removing redundant features. A separate feature set is used in each of the three classifiers of the proposed methodology, efficiently chosen using one or more statistical feature selection technique(s) (also referred hereinafter optimum feature selection technique(s)), for example, but are not limited to, a Maximal Information Coefficient (MIC) technique and minimum Redundancy Maximum Relevance (mRMR) technique(s) and are finalized during training phase. Features recommended by medical practitioners for a certain level of classification were also incorporated

in the selected feature list.

**[0034]** In an embodiment of the present disclosure, at step 210, the one or more hardware processors 104 identifying based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms (Normal), a first set of abnormal rhythms (others), and a second set of abnormal rhythms (AF and noisy) in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal. In an embodiment of the present disclosure, a first binary classifier of the cascaded binary classifier (as depicted in Layer 1) outputs or identifies 'A' set of rhythms (e.g., Normal and Others), and 'B' set of rhythms (e.g., AF and noisy). In an embodiment of the present disclosure, 'A' set of rhythms may be referred as one or more normal rhythms and other rhythms, and wherein 'B' set of rhythms may be referred as AF rhythms and noisy.

**[0035]** In other words, the system 100 classifies an unknown short single-lead ECG signal into one of the four classes including normal, AF, other noisy rhythms and noisy recordings. The major problem of the task is that there is not a single feature exists that can separate four classes at a single shot (or at a single instance). For example, irregular HRV is a common differentiator between normal and AF. However, other rhythms also have the same properties, which introduces ambiguity in a classifier. Thus the embodiments of the present disclosure and the system 100 comprise a cascaded binary classifier that when executed by the one or more hardware processors 104 identifies 'A' set of rhythms may be referred as one or more normal rhythms and other rhythms, and wherein 'B' set of rhythms may be referred as AF rhythms and noisy in the clean ECG signal.

**[0036]** In an embodiment of the present disclosure, the cascaded binary classifier implemented and executed in the system 100 is a three level classifier, connected in two acceded layer as depicted in FIG. 3. At each layer a binary classification is done. The corresponding discriminative features are selected at each level using one or more statistical feature extraction technique(s) as described above. For example, both AF and noisy rhythms contain high frequency noise components. Whereas normal and AF shows similar frequency feature patterns. Thus features like spectral centroid, spectral roll off spectral flux etc., can very well separate them into two classes "normal + others" and "AF + noisy". Now in the next level the system 100 (or the cascaded binary classifier) performs a more fine classification. For example normal ECG signal has a regular pattern in RR intervals and heart rate value lies within a certain limit. Whereas for other rhythms HRV features are not (or may not be) very stable. These kind of features are selected using the optimum feature selection technique(s) when passed through the three level classifier as depicted in FIG. 3. On the other hand, for AF signals, P wave are often found to be missing, that is not found in noisy recordings, moreover noisy recordings have high frequency spectral components which are not present in AF. These kind of fea-

tures are selected at the third level of classifier (e.g., classifier 3 as depicted in FIG. 3), for classification. In an embodiment of the present disclosure, for each level of classification, Adaptive Boosting (AdaBoost) is used for classification and the details can be found in the draft paper AdaBoost (adaptive boosting) is used in all levels of classification. Adaboost is an ensemble learning approach, where many weak learners are iteratively added in each round of training and a weighting vector is adjusted to reduce the misclassification rate. This technique is less prone to overfitting, more sensitive to noisy data and outliers and can handle the class label imbalance in the training set. For each of the three classifiers, two parameters of the ensemble classifiers, namely, number of learning cycles and learning rate are optimized using Bayesian optimization function.

Experimental Results:

**[0037]** Experiments were performed on the Physionet dataset. This dataset comprised a total of 8528 recordings with mean duration of 32.5 seconds. All of them were single-lead ECG signals, recorded using AliveCor device and sampled at 300 Hz. The distribution of normal, AF, other rhythms and noisy data is largely imbalanced in the dataset. F1-score for normal ( $F_{norm}$ ), AF ( $F_{af}$ ) and other rhythms ( $F_{oth}$ ) were computed for performance analysis and the final accuracy was reported in terms of an illustrative expression as below:

$$F_T = ((F_{norm} + F_{af} + F_{oth})/3)$$

**[0038]** The embodiments of the present disclosure and the proposed methodology of FIG. 2 was initially applied on the entire training dataset using 5-fold cross validation and the performance of the same is shown in Table 1 by way of example below:

Table 1

	$F_{norm}$	$F_{af}$	$F_{oth}$	$F_T$
Average	0.9095	0.7978	0.7719	0.8264
Standard	0.0022	0.0062	0.0040	0.0026

**[0039]** It can be observed from the above Table 1 that the performance of the proposed methodology of FIG. 2 is stable enough across the folds in a 5-fold cross validation, owing to the small standard deviation values across different test scenarios. It can also be observed that the methodology yields a very high F1-score (average value 0.9) in classifying (or identifying) normal recordings, whereas the F1-score of detecting other rhythms is close to 0.77. A detailed inspection reveals that a good amount of other rhythms are wrongly classified as normal. The unavailability of actual disease information corresponding to each recording in this particular

class makes the classification task more challenging to identify the proper features, thus reducing the classification accuracy. A final training model was created on the entire training dataset and evaluated on a subset of the hidden test dataset at a server. Table 2 depicts performance of proposed methodology on a subset of hidden test dataset by way of illustrative example below:

Table 2

Test dataset	$F_{norm}$	$F_{af}$	$F_{oth}$	$F_T$
	0.92	0.86	0.74	0.84

**[0040]** It can be observed from Table 2 that the performance of detecting (or identifying) AF rhythms has significantly improved on the test dataset, compared to internal cross validation on training set. On the other hand, performance of detecting (or identifying) other rhythms has marginally dropped and detection of normal recordings remains almost the same.

**[0041]** Embodiments of the present disclosure and the system 100 identify one or more rhythms in a (short) single-lead ECG recordings, (e.g., say 30 seconds recorded ECG signal) using a series of multi-layer cascaded binary classifiers (also referred as the cascaded binary classifier). The proposed methodology has been successfully validated on Physionet (2017) dataset as mentioned above.

**[0042]** The written description describes the subject matter herein to enable any person skilled in the art to make and use the embodiments. The scope of the subject matter embodiments is defined by the claims and may include other modifications that occur to those skilled in the art. Such other modifications are intended to be within the scope of the claims if they have similar elements that do not differ from the literal language of the claims or if they include equivalent elements with insubstantial differences from the literal language of the claims.

**[0043]** It is to be understood that the scope of the protection is extended to such a program and in addition to a computer-readable means having a message therein; such computer-readable storage means contain program-code means for implementation of one or more steps of the method, when the program runs on a server or mobile device or any suitable programmable device. The hardware device can be any kind of device which can be programmed including e.g. any kind of computer like a server or a personal computer, or the like, or any combination thereof. The device may also include means which could be e.g. hardware means like e.g. an application-specific integrated circuit (ASIC), a field-programmable gate array (FPGA), or a combination of hardware and software means, e.g. an ASIC and an FPGA, or at least one microprocessor and at least one memory with software modules located therein. Thus, the means can include both hardware means and software means. The method embodiments described herein could be imple-

mented in hardware and software. The device may also include software means. Alternatively, the embodiments may be implemented on different hardware devices, e.g. using a plurality of CPUs.

**[0044]** The embodiments herein can comprise hardware and software elements. The embodiments that are implemented in software include but are not limited to, firmware, resident software, microcode, etc. The functions performed by various modules described herein may be implemented in other modules or combinations of other modules. For the purposes of this description, a computer-usable or computer readable medium can be any apparatus that can comprise, store, communicate, propagate, or transport the program for use by or in connection with the instruction execution system, apparatus, or device.

**[0045]** The illustrated steps are set out to explain the exemplary embodiments shown, and it should be anticipated that ongoing technological development will change the manner in which particular functions are performed. These examples are presented herein for purposes of illustration, and not limitation. Further, the boundaries of the functional building blocks have been arbitrarily defined herein for the convenience of the description. Alternative boundaries can be defined so long as the specified functions and relationships thereof are appropriately performed. Alternatives (including equivalents, extensions, variations, deviations, etc., of those described herein) will be apparent to persons skilled in the relevant art(s) based on the teachings contained herein. Such alternatives fall within the scope and spirit of the disclosed embodiments. Also, the words "comprising," "having," "containing," and "including," and other similar forms are intended to be equivalent in meaning and be open ended in that an item or items following any one of these words is not meant to be an exhaustive listing of such item or items, or meant to be limited to only the listed item or items. It must also be noted that as used herein and in the appended claims, the singular forms "a," "an," and "the" include plural references unless the context clearly dictates otherwise.

**[0046]** Furthermore, one or more computer-readable storage media may be utilized in implementing embodiments consistent with the present disclosure. A computer-readable storage medium refers to any type of physical memory on which information or data readable by a processor may be stored. Thus, a computer-readable storage medium may store instructions for execution by one or more processors, including instructions for causing the processor(s) to perform steps or stages consistent with the embodiments described herein. The term "computer-readable medium" should be understood to include tangible items and exclude carrier waves and transient signals, i.e., be non-transitory. Examples include random access memory (RAM), read-only memory (ROM), volatile memory, nonvolatile memory, hard drives, CD ROMs, DVDs, flash drives, disks, and any other known physical storage media.

**[0047]** It is intended that the disclosure and examples be considered as exemplary only, with a true scope and spirit of disclosed embodiments being indicated by the following claims.

### Claims

1. A processor implemented method, comprising:

acquiring, via one or more hardware processors, a single-lead electrocardiogram (ECG) signal that is recorded for a predefined time interval; applying in real-time, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal; extracting one or more features from the clean ECG signal; selecting, using an optimum feature selection technique, one or more optimum features from the one or more extracted features; and identifying based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms, a first set of abnormal rhythms, and a second set of abnormal rhythms in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal.

2. The processor implemented method of claim 1, wherein the step of applying, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal comprises:

dividing the acquired single-lead ECG signal into a plurality of windows; computing a spectrogram of each of the plurality of windows; performing a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold; determining noise in at least a subset of the plurality of windows based on the comparison; and extracting the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows.

3. The processor implemented method of claim 2, wherein noise is determined in the at least a subset of the plurality of windows when each window from the subset has power that is greater than a threshold power.

4. The processor implemented method of claim 1, wherein the optimum feature selection technique is at least one of a minimum redundancy maximum rel-

evancy (mRMR) technique and a Maximal Information Coefficient (MIC) technique.

5. The processor implemented method of claim 2, wherein the dynamically computed threshold is based on a signal to noise ratio (SNR).

6. A system comprising:

a memory storing instructions; one or more communication interfaces; and one or more hardware processors coupled to the memory via the one or more communication interfaces, wherein the one or more hardware processors are configured by the instructions to:

acquire a single-lead electrocardiogram (ECG) signal that is recorded for a predefined time interval; apply in real-time, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal; extract one or more features from the clean ECG signal; select, using an optimum feature selection technique, one or more optimum features from the one or more extracted features; and identify based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms, a first set of abnormal rhythms, and a second set of abnormal rhythms in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal.

7. The system of claim 6, wherein the clean ECG signal is extracted by applying the spectrogram based noisy data removal technique on the acquired single-lead ECG signal by:

dividing the acquired single-lead ECG signal into a plurality of windows; computing a spectrogram of each of the plurality of windows; performing a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold; determining noise in at least a subset of the plurality of windows based on the comparison; and extracting the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows.

8. The system of claim 2, wherein noise is determined in the at least a subset of the plurality of windows

when each window from the subset have power that is greater than a threshold power.

9. The system of claim 6, wherein the optimum feature selection technique is at least one of a minimum redundancy maximum relevancy (mRMR) technique and a Maximal Information Coefficient (MIC) technique. 5
10. The system of claim 7, wherein the dynamically computed threshold is based on a signal to noise ratio (SNR). 10
11. One or more non-transitory machine readable information storage mediums comprising one or more instructions which when executed by one or more hardware processors causes: 15

acquiring, via the one or more hardware processors, a single-lead electrocardiogram (ECG) signal that is recorded for a predefined time interval; 20

applying in real-time, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal to obtain a clean ECG signal; 25

extracting one or more features from the clean ECG signal;

selecting, using an optimum feature selection technique, one or more optimum features from the one or more extracted features; and 30

identifying based on the selected one or more optimum features, using a binary cascade classifier, at least one of one or more normal rhythms, a first set of abnormal rhythms, and a second set of abnormal rhythms in at least one of the single-lead electrocardiogram (ECG) signal, and the clean ECG signal. 35

12. The one or more non-transitory machine readable information storage mediums of claim 11, wherein the step of applying, via the one or more hardware processors, a spectrogram based noisy data removal technique on the acquired single-lead ECG signal comprises: 40

dividing the acquired single-lead ECG signal into a plurality of windows;

computing a spectrogram of each of the plurality of windows; 50

performing a comparison of the computed spectrogram of each of the plurality of windows with a dynamically computed threshold;


determining noise in at least a subset of the plurality of windows based on the comparison; and 55

extracting the clean ECG signal based on the determined noise in the at least a subset of the plurality of windows.

13. The one or more non-transitory machine readable information storage mediums of claim 12, wherein noise is determined in the at least a subset of the plurality of windows when each window from the subset has power that is greater than a threshold power.

14. The one or more non-transitory machine readable information storage mediums of claim 11, wherein the optimum feature selection technique is at least one of a minimum redundancy maximum relevancy (mRMR) technique and a Maximal Information Coefficient (MIC) technique.

15. The one or more non-transitory machine readable information storage mediums of claim 12, wherein the dynamically computed threshold is based on a signal to noise ratio (SNR).

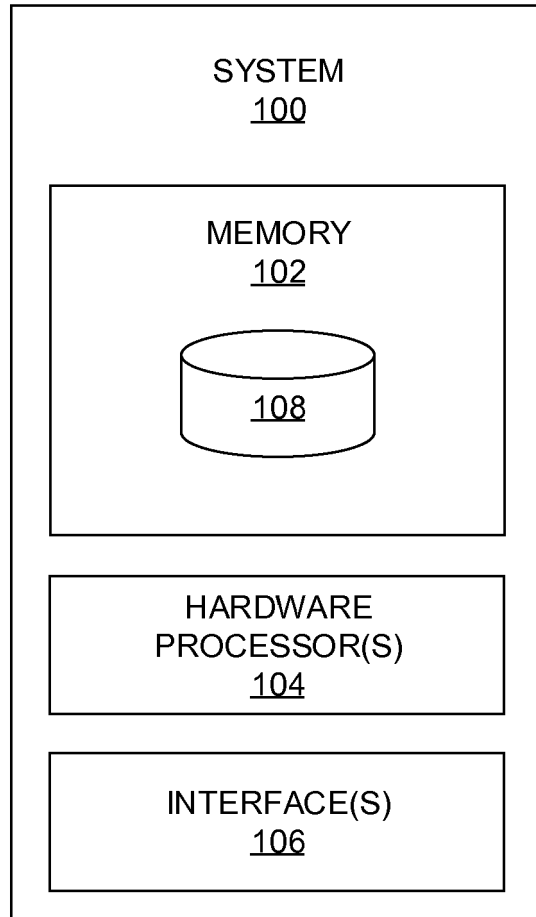

**FIG. 1**

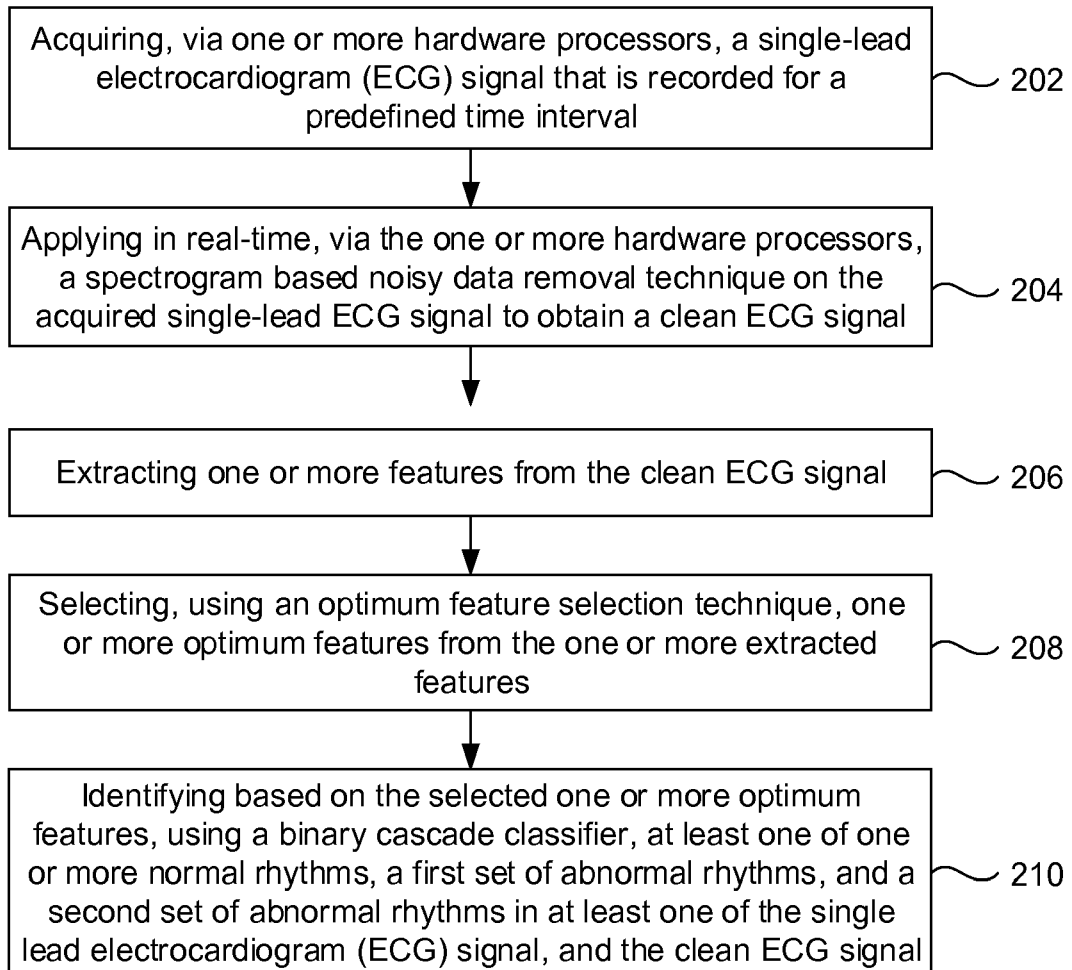


FIG. 2


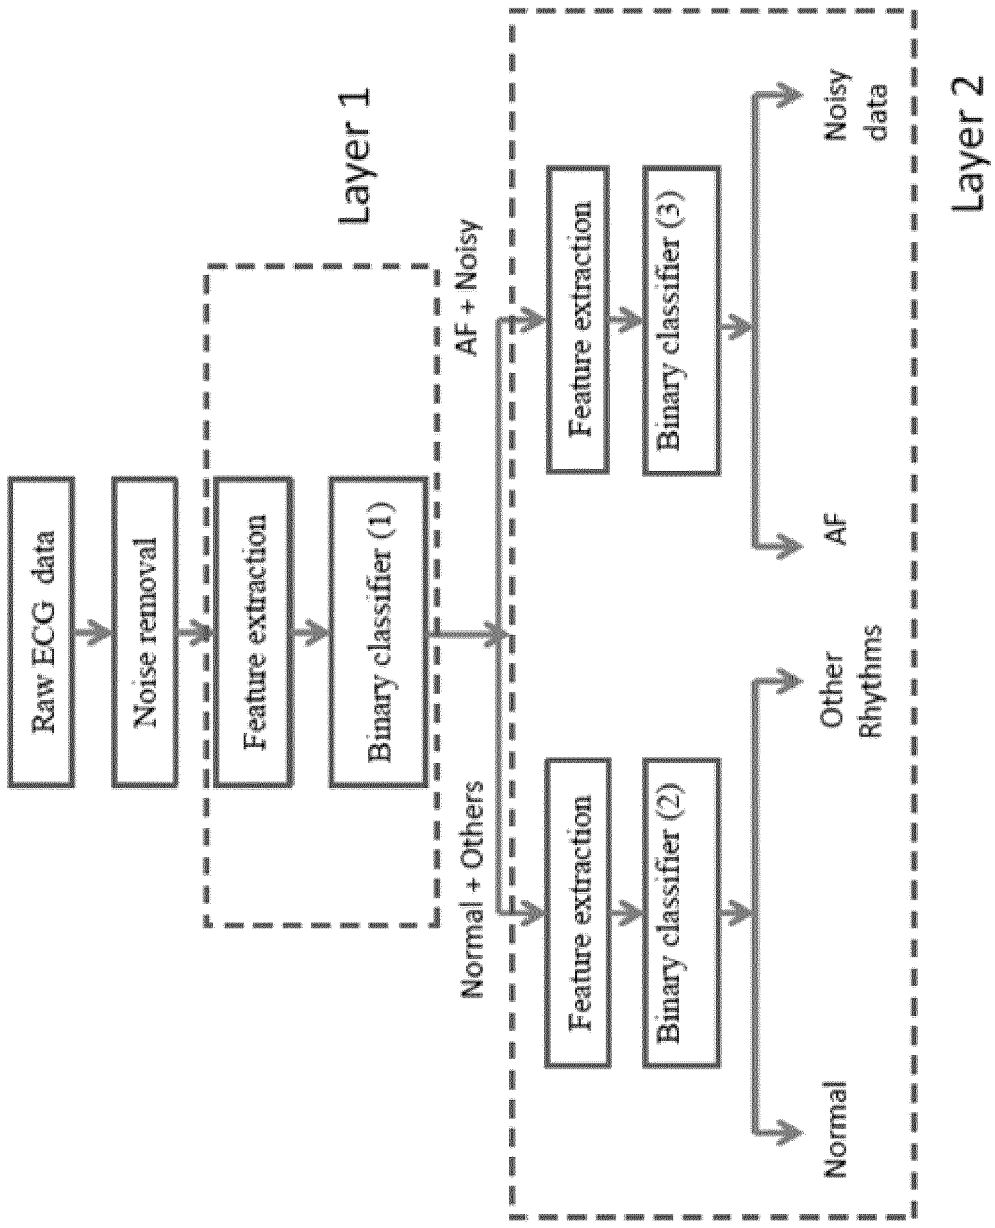


FIG. 3

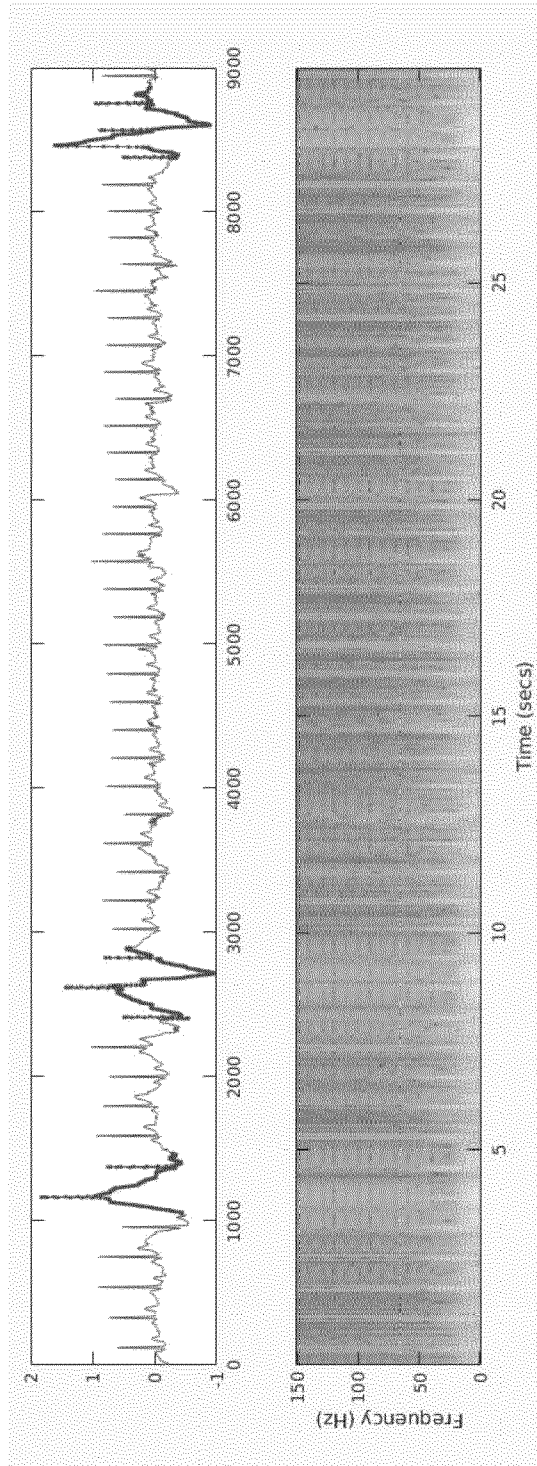

**FIG. 4**

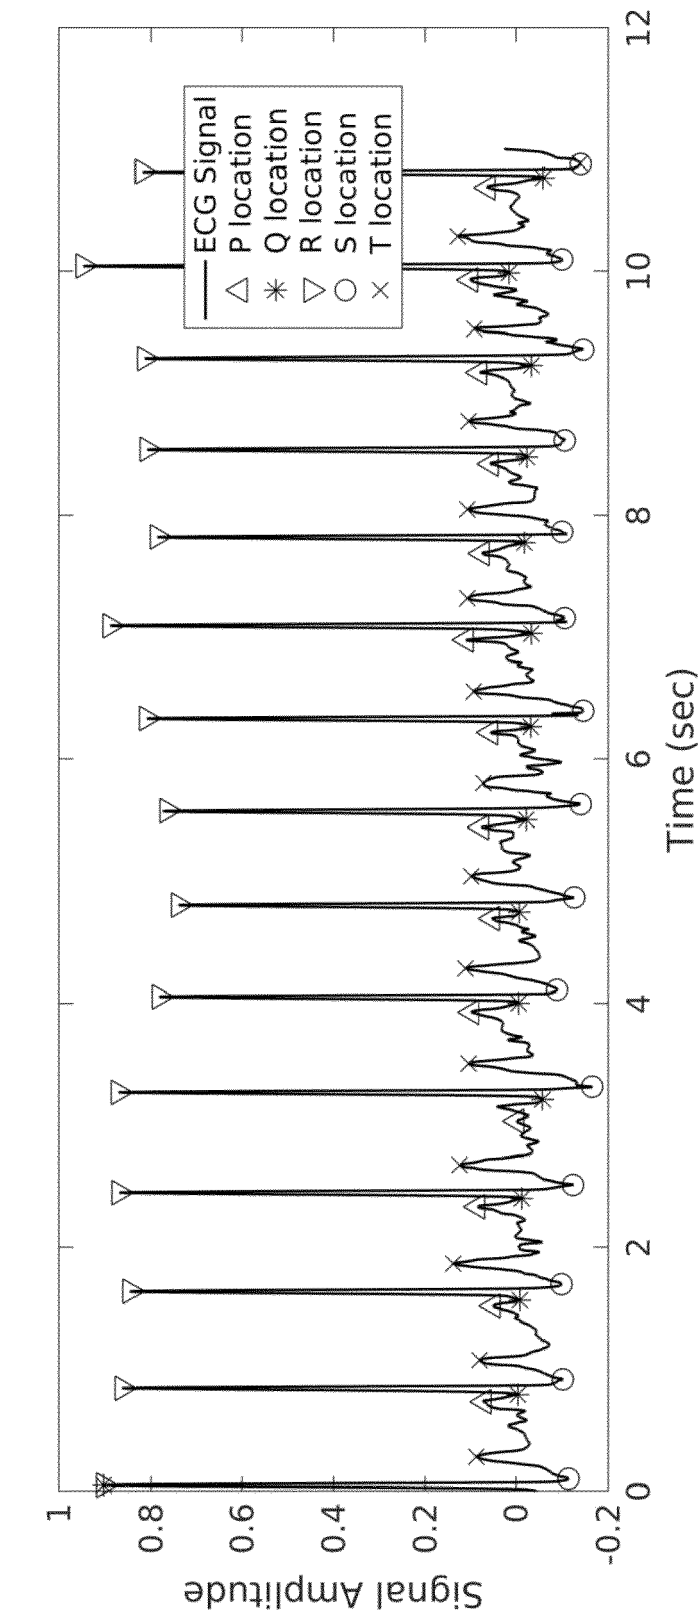


FIG. 5



EUROPEAN SEARCH REPORT

Application Number  
EP 18 15 3347

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	<p>JOACHIM BEHAR ET AL: "ECG Signal Quality During Arrhythmia and Its Application to False Alarm Reduction", IEEE TRANSACTIONS ON BIOMEDICAL ENGINEERING, IEEE SERVICE CENTER, PISCATAWAY, NJ, USA, vol. 60, no. 6, 1 June 2013 (2013-06-01), pages 1660-1666, XP011509829, ISSN: 0018-9294, DOI: 10.1109/TBME.2013.2240452                      * page 1660, column 2, lines 19,29,33; figure 1; tables I, VI-VIII *                      * page 1661, column 2, lines 1,2,7, paragraph 3 *                      * page 1663 *                      * page 1664, column 1, line 9, paragraph 6 *</p>	1-15	<p>INV. A61B5/00 A61B5/0452 A61B5/0456</p>
A	<p>-----                      PATIL D D ET AL: "Intelligent arrhythmia diagnostics system", INTERNATIONAL JOURNAL OF COMPUTER SCIENCE ISSUES, SOFTWAREFIRST, MAHEBOURG                      , vol. 9, no. 6 6-1                      1 January 2012 (2012-01-01), pages 408-413, XP009506671, ISSN: 1694-0784                      Retrieved from the Internet:                      URL:http://www.ijcsi.org/papers/IJCSI-9-6-1-408-413.pdf                      * sections 6, 9;                      figure 2 *</p> <p>-----</p> <p style="text-align: right;">-/--</p>	1,6,11	<p>TECHNICAL FIELDS SEARCHED (IPC) A61B</p>
The present search report has been drawn up for all claims			
Place of search <b>The Hague</b>		Date of completion of the search <b>9 July 2018</b>	Examiner <b>Visser, Robert</b>
<p>CATEGORY OF CITED DOCUMENTS</p> <p>X : particularly relevant if taken alone                      Y : particularly relevant if combined with another document of the same category                      A : technological background                      O : non-written disclosure                      P : intermediate document</p>		<p>T : theory or principle underlying the invention                      E : earlier patent document, but published on, or after the filing date                      D : document cited in the application                      L : document cited for other reasons                      .....                      &amp; : member of the same patent family, corresponding document</p>	

EPO FORM 1503 03.02 (P04C01)



EUROPEAN SEARCH REPORT

Application Number  
EP 18 15 3347

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	<p>LORENZONI GIULIA ET AL: "Cost-effectiveness of early detection of atrial fibrillation via remote control of implanted devices", JOURNAL OF EVALUATION IN CLINICAL PRACTICE (ONLINE), WILEY-BLACKWELL PUBLISHING LTD, UNITED KINGDOM , vol. 20, no. 5 30 September 2014 (2014-09-30), pages 570-577, XP009506675, ISSN: 1365-2753, DOI: 10.1111/JEP.12132 Retrieved from the Internet: URL:https://epo.summon.serialssolutions.com/2.0.0/link/0/eLvHCXMwtV1LS8NAEF6sgngRX-CbRbxIiDSPbZqjlFo9CFJ70FPZbDZQiG6orQd_vbPPREuxHrwsZchuk3wfM70beSB0GYZtRlnIfZankR_TivIps3M5ALsymgeqW8NLLx4NkuFAdmuwfQdr2b8iDTLAWmb0_gFttygI4DdgDiOgDuNKuPfe-8zXURpWkYE_yFUd45zPOLMuItUN0woZ81_qiDjvY0K9KQf06hh2WVLitSolALMsZK * page 571 *</p>	1,6,11	
			TECHNICAL FIELDS SEARCHED (IPC)
A	<p>DALUWATTE C ET AL: "Assessing ECG signal quality indices to discriminate ECGs with artefacts from pathologically different arrhythmic ECGs", PHYSIOLOGICAL MEASUREMENT, INSTITUTE OF PHYSICS PUBLISHING, BRISTOL, GB, vol. 37, no. 8, 25 July 2016 (2016-07-25), pages 1370-1382, XP020307069, ISSN: 0967-3334, DOI: 10.1088/0967-3334/37/8/1370 [retrieved on 2016-07-25] * page 1372; figure 2; table 2 * ----- -/--</p>	1,6,11	
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 9 July 2018	Examiner Visser, Robert
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons ..... & : member of the same patent family, corresponding document	

1  
EPO FORM 1503 03.02 (P04C01)



EUROPEAN SEARCH REPORT

Application Number  
EP 18 15 3347

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	OSTER JULIEN ET AL: "Open source Java-based ECG analysis software and Android app for Atrial Fibrillation screening", COMPUTING IN CARDIOLOGY 2013, N/A, 22 September 2013 (2013-09-22), pages 731-734, XP032550330, ISSN: 2325-8861 ISBN: 978-1-4799-0884-4 [retrieved on 2014-01-15] * pages 731-733; figure 1 *	1,6,11	
A	BEHAR J ET AL: "A single channel ECG quality metric", COMPUTING IN CARDIOLOGY (CINC), 2012, IEEE, 9 September 2012 (2012-09-09), pages 381-384, XP032317135, ISBN: 978-1-4673-2076-4	1,6,11	
A	NAGA PRUDHVI RAJ V ET AL: "ECG signal denoising using Undecimated Wavelet Transform", ELECTRONICS COMPUTER TECHNOLOGY (ICECT), 2011 3RD INTERNATIONAL CONFERENCE ON, IEEE, 8 April 2011 (2011-04-08), pages 94-98, XP031956726, DOI: 10.1109/ICECTECH.2011.5941808 ISBN: 978-1-4244-8678-6 * figures 2,4,6 *	7,10	TECHNICAL FIELDS SEARCHED (IPC)
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 9 July 2018	Examiner Visser, Robert
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03.02 (P04C01)



EUROPEAN SEARCH REPORT

Application Number  
EP 18 15 3347

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	HASSAN GHASEMZADEH ET AL: "Wireless Medical-Embedded Systems: A Review of Signal-Processing Techniques for Classification", IEEE SENSORS JOURNAL, IEEE SERVICE CENTER, NEW YORK, NY, US, vol. 13, no. 2, 1 February 2013 (2013-02-01), pages 423-437, XP011487119, ISSN: 1530-437X, DOI: 10.1109/JSEN.2012.2222572 * page 426; figure 3 *	7,10	
A	KIM YOON JAE ET AL: "Proposition of novel classification approach and features for improved real-time arrhythmia monitoring", COMPUTERS IN BIOLOGY AND MEDICINE, NEW YORK, NY, US, vol. 75, 8 June 2016 (2016-06-08), pages 190-202, XP029629881, ISSN: 0010-4825, DOI: 10.1016/J.COMPBIOMED.2016.06.009 * pages 190,191 *	1,6,11	TECHNICAL FIELDS SEARCHED (IPC)
A	SCOTT DOYLE ET AL: "Cascaded multi-class pairwise classifier (CascaMPa) for normal, cancerous, and cancer confounder classes in prostate histology", 2011 8TH IEEE INTERNATIONAL SYMPOSIUM ON BIOMEDICAL IMAGING: FROM NANO TO MACRO (ISBI 2011), IEEE, UNITED STATES, 30 March 2011 (2011-03-30), pages 715-718, XP031944638, DOI: 10.1109/ISBI.2011.5872506 ISBN: 978-1-4244-4127-3 * figure 1 *	1,6,11	
----- -/--			
The present search report has been drawn up for all claims			
Place of search <b>The Hague</b>		Date of completion of the search <b>9 July 2018</b>	Examiner <b>Visser, Robert</b>
<b>CATEGORY OF CITED DOCUMENTS</b> X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03.02 (P04C01)



EUROPEAN SEARCH REPORT

Application Number  
EP 18 15 3347

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	INDRAJIT MANDAL ET AL: "Accurate Prediction of Coronary Artery Disease Using Reliable Diagnosis System", JOURNAL OF MEDICAL SYSTEMS, KLUWER ACADEMIC PUBLISHERS-PLENUM PUBLISHERS, NE, vol. 36, no. 5, 12 February 2012 (2012-02-12), pages 3353-3373, XP035103422, ISSN: 1573-689X, DOI: 10.1007/S10916-012-9828-0 * page 3358; figure 2 *	1,6,11	
A	ALMARDINI MAMOUN ET AL: "A Supervised Model for Predicting the Risk of Mortality and Hospital Readmissions for Newly Admitted Patients", 14 June 2017 (2017-06-14), MEDICAL IMAGE COMPUTING AND COMPUTER-ASSISTED INTERVENTION - MICCAI 2015 : 18TH INTERNATIONAL CONFERENCE, MUNICH, GERMANY, OCTOBER 5-9, 2015; PROCEEDINGS; [LECTURE NOTES IN COMPUTER SCIENCE; LECT.NOTES COMPUTER], SPRINGER INTERNATIONAL PUBLISHING, CH, XP047417581, ISSN: 0302-9743 ISBN: 978-3-642-38287-1 [retrieved on 2017-06-14] * pages 32,34 *	1,6,11	
The present search report has been drawn up for all claims			TECHNICAL FIELDS SEARCHED (IPC)
Place of search The Hague		Date of completion of the search 9 July 2018	Examiner Visser, Robert
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

1  
EPO FORM 1503 03.82 (P04C01)

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- IN 201721033210 [0001]

专利名称(译)	级联二进制分类器，用于识别单导联心电图 ( ECG ) 信号中的节律		
公开(公告)号	<a href="#">EP3456246A1</a>	公开(公告)日	2019-03-20
申请号	EP2018153347	申请日	2018-01-25
申请(专利权)人(译)	塔塔咨询服务有限公司		
当前申请(专利权)人(译)	塔塔咨询服务有限公司		
[标]发明人	DATTA SHREYASI PURI CHETANYA MUKHERJEE AYAN BANERJEE ROHAN CHOUDHURY ANIRBAN DUTTA UKIL ARIJIT BANDYOPADHYAY SOMA PAL ARPAN KHANDELWAL SUNDEEP SINGH RITURAJ		
发明人	DATTA, SHREYASI PURI, CHETANYA MUKHERJEE, AYAN BANERJEE, ROHAN CHOUDHURY, ANIRBAN DUTTA UKIL, ARIJIT BANDYOPADHYAY, SOMA PAL, ARPAN KHANDELWAL, SUNDEEP SINGH, RITURAJ		
IPC分类号	A61B5/00 A61B5/0452 A61B5/0456		
CPC分类号	G06K9/6257 G06K9/628 A61B5/0452 A61B5/0456 A61B5/7264 G16H50/20 A61B5/04012 A61B5/046 A61B5/0472 A61B5/7203		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

当前技术长时间分析心电图 ( ECG ) 信号，这并不总是实际情况。此外，当前场景仅在正常和心房颤动 ( AF ) 之间执行二元分类，而除了AF之外还存在许多异常节律。传统的系统/方法具有其自身的局限性并且可能倾向于错误分类ECG信号，从而导致不平衡的多标签分类问题。本公开的实施例提供了健壮且更有效的系统和方法，其通过实施基于频谱图的噪声消除来从获取的单引线获得干净的ECG信号，从而对节律（例如，正常，AF，其他异常节律和噪声ECG记录）进行分类。ECG信号，每个分类层的最佳特征选择，从一组提取的特征中选择最佳特征，以及多层级联二元分类器，用于识别分类器每层清洁ECG信号中的节奏。

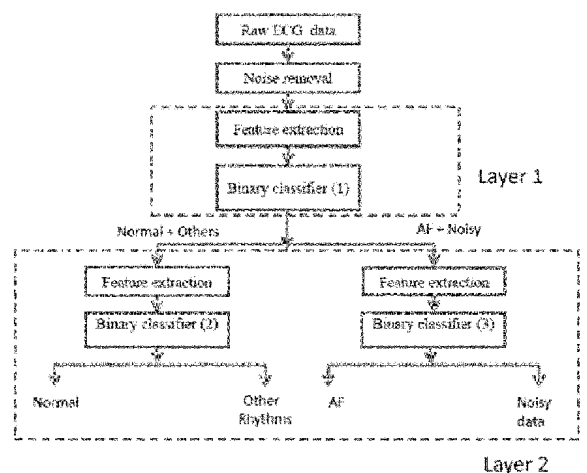


FIG. 3