

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
7 May 2009 (07.05.2009)

PCT

(10) International Publication Number
WO 2009/056859 A1

- (51) International Patent Classification:
A61B 5/00 (2006.01)
- (21) International Application Number:
PCT/GB2008/003708
- (22) International Filing Date:
3 November 2008 (03.11.2008)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
0721575.9 2 November 2007 (02.11.2007) GB
- (71) Applicant (for all designated States except US): **SENSOR TECHNOLOGY & DEVICES LTD** [GB/GB]; 4 Heron Road, Belfast BT3 9LE (GB).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **McLAUGHLIN, James, Andrew** [GB/GB]; 49 North Parade, Belfast, BT7 2GH (GB). **ANDERSON, John, McCune** [GB/GB]; 16 Torrgrange, Hollywood B18 0NG (GB).
- (74) Agent: **MURGITROYD & COMPANY**; 165-169 Scotland Street, Glasgow G5 8PL (GB).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
- with international search report
 - before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

(54) Title: MEASUREMENT OF OXYGEN SATURATION OF BLOOD HAEMOGLOBIN



(57) Abstract: The invention provides a chest-based oximeter (1) for measuring oxygen saturation of haemoglobin in blood of the chest of a subject, comprising at least one radiation source (5,7) adapted to emit radiation onto the chest, at least one radiation detector (9) adapted to detect radiation reflected from the chest, and a pressure device (11) adapted to apply pressure to the oximeter to connect the oximeter to the chest.

WO 2009/056859 A1

Measurement of Oxygen Saturation of Blood Haemoglobin

This invention relates to the measurement of oxygen saturation of blood haemoglobin.

5

The oxygen saturation of haemoglobin in blood is an important indicator of the health of a subject. For example, measurements of oxygen saturation can detect hypoxia before the subject becomes cyanosed. Measurement of oxygen saturation of blood haemoglobin is therefore routinely carried out for subjects receiving medical care in hospitals, and for monitoring the health of subjects in the home.

10

Traditionally, oximeters are used to make measurements of oxygen saturation of blood haemoglobin at peripheral sites of the subject, such as a finger, ear or toe. Thus saturation of peripheral oxygen, commonly referred to as SpO₂, is measured. In use, an oximeter is attached to a peripheral site of the subject, in proximity to an artery, and senses the oxygen saturation of arterial blood. The oximeter comprises two radiation sources and a radiation detector. Commonly, the radiation sources are positioned on a first side of the peripheral site, e.g. on a first side of a finger, and the radiation detector is arranged on a second, opposite, side of the peripheral site. This is referred to as a transmission oximeter. Radiation from the sources is transmitted from the sources into the peripheral site. Some of the radiation is absorbed by the peripheral site, and particularly the blood in the artery of the site, and some of the radiation passes through the peripheral site. At least some of this transmitted radiation is detected by the detector. The radiation sources, usually LEDs, produce radiation at different wavelengths, the first source in the red part of the electromagnetic spectrum, and the second source in the infra red (IR) part of the electromagnetic spectrum. The level of

15

20

25

30

absorption of red and IR radiation in blood, depends on the oxygenation level of haemoglobin in the blood. Further, for blood having a particular haemoglobin oxygenation level, the red and IR radiation will be absorbed by different amounts. By detecting radiation that is transmitted through the arterial blood, it is possible to calculate the absorption of the red and IR radiation and compute the percentage of haemoglobin in the arterial blood which is saturated with oxygen. This is usually expressed as a percentage of total saturation. The blood flow through the artery will be pulsatile in form. The oximeter is designed to detect radiation transmitted through blood in the artery, by being configured to detect pulsatile transmitted radiation. The oximeter is able to distinguish the pulsatile signals from other more static signals, e.g. signals transmitted through tissue or veins. The oximeter is able to measure the heart rate of the subject, and also to produce an indication of the quality of blood flow through the artery.

As measurement of oxygen saturation of haemoglobin in blood finds widespread application, improvements in measurement systems and techniques are constantly being sought.

According to a first aspect of the invention there is provided a chest-based oximeter for measuring oxygen saturation of haemoglobin in blood of the chest of a subject, comprising

at least one radiation source adapted to emit radiation onto the chest, at least one radiation detector adapted to detect radiation reflected from the chest, and

a pressure device adapted to apply pressure to the oximeter to connect the oximeter to the chest.

It has been found that the signals representing radiation reflected from the chest are weaker than signals representing radiation transmitted through

the finger. Nevertheless, the chest signals are measurable, are sufficiently strong to measure accurately oxygen saturation values, oxygen perfusion trends and accurate heart rate values, and are sufficiently repeatability for good quality measurements.

5

The pressure device may be applied to skin of the chest of the subject. The pressure device may comprise a material which has a Young's modulus which is lower than that of the skin of the chest of the subject. The material may comprise a stretchable foam material. The pressure
10 device may stress and apply a pressure on the oximeter towards the skin, to connect the oximeter to the chest. The difference between the Young's modulus of the skin and the Young's modulus of the pressure device material may cause the pressure device to stress and apply a pressure on the oximeter towards the skin. The pressure device may apply pressure
15 on the oximeter which increases with time, for example as the skin absorbs moisture from the material of the pressure device.

The pressure device may be profiled to press onto the chest of the subject to apply pressure to the oximeter towards the chest, to connect the
20 oximeter to the chest. The pressure device may comprise a suction device. The pressure device may comprise a biasing device, for example, a spring. The pressure device may comprise a finger push device. The pressure device may comprise a belt.

25 The pressure device may apply a pressure in the range of approximately 1 Pascal to approximately 100000 Pascal. The pressure device may be provided with a pressure sensitive adhesive.

30 The pressure device may optically couple the radiation from the radiation source to the chest of the subject. The pressure device may optically

couple the radiation reflected from the chest of the subject to the radiation detector.

5 It has been found that the amplitude of detected radiation significantly increases when a pressure is applied to the oximeter. The amplitude of the detected radiation is indicative of the quality of the measure of the oxygen saturation of haemoglobin in blood that is obtained by the oximeter. Accurate measurement of oxygen saturation by oximeters can only be achieved when an adequate pulse is present at the measurement site, i.e. the chest. Applying pressure to the oximeter will increase the strength of the measurement of the pulse and therefore oxygen saturation will be more accurately measured by the oximeter. The pressure to be applied by the pressure device may be determined by applying a range of pressure from zero pressure to heavy pressure to the oximeter, and measuring the radiation reflected from the chest. It has been found that as 10 the pressure is gradually increased, the peak to peak values of measured signals stays approximately constant until a pressure threshold is reached, then the peak to peak values increases as the pressure continues to increase, until a cut-off pressure is reached at which the peak to peak values fall to an unmeasurable size where the quality of the signals has deteriorated significantly. The pressure range between the pressure 20 threshold and the pressure cut-off is the optimum pressure range to use.

The chest-based oximeter may comprise an optical coupling element. 25 This may be positioned in the oximeter to enhance coupling of radiation between the radiation source and the radiation detector and the chest of the subject.

The at least one radiation source and the at least one radiation detector 30 may be mounted in the chest-based oximeter such that they are spaced

apart by a distance in the range of approximately 0.5mm to approximately 2cm. The at least one radiation source and the at least one radiation detector may be mounted in the chest-based oximeter such that, in use, they are positioned in the range of approximately 1cm to approximately 20cm above the chest of the subject.

The at least one radiation source may emit radiation having one or more infra red peak wavelengths. The chest-based oximeter may further comprise a second radiation source which emits radiation having one or more infra red peak wavelengths. The at least one radiation source may emit radiation having at least a first infra red peak wavelength, and the second radiation source may emit radiation having at least a second, different, infra red peak wavelength. The or each infra red peak wavelength is in the range of 600nm to 1500nm, for example 780nm, 810nm, 820nm, 830nm, 840nm, 850nm, 870nm, 880nm, 890nm, 910nm, 940nm, 970nm, 1050nm, 1070nm, 1200nm, 1300nm, 1350nm, 1450nm, 1550nm.

Infra red radiation has a wavelength range which sensitive to the measurement of oxygen saturation in blood. Using one or more radiation sources which emit radiation having infra red wavelengths therefore optimises the detection ability of the oximeter. Effects due to skin, tissue path, etc. can be filtered or monitored and subtracted in order to measure the oxygen saturation and also the heart rate of the subject.

The at least one radiation source may emit radiation having one or more visible peak wavelengths. The chest-based oximeter may further comprise a second radiation source which emits radiation having one or more visible peak wavelengths.

The at least one radiation source may emit radiation having one or more visible peak wavelengths, and the oximeter may further comprise a second radiation source which emits radiation having one or more infra red peak wavelengths.

5

The radiation source or radiation sources may comprise an LED or LEDs. The radiation source or radiation sources may comprise a solid state laser or solid state lasers. When the oximeter comprises two or more radiation sources, the sources may comprise LEDs, or solid state lasers, or a combination of LEDs and solid state lasers.

10

The chest-based oximeter may comprise one or more devices to, for example, process or amplify the radiation detected by the radiation detector. The chest-based oximeter may comprise a processor, which may receive one or more signals representing radiation detected by the radiation detector, and may use the signal or signals to provide a measure of the oxygen saturation of haemoglobin in blood of the chest. The chest-based oximeter may comprise a transmitter. The transmitter may transmit one or more signals representing the measure of the oxygen saturation of haemoglobin in blood of the chest to a remote receiver. The transmitter may relay changes in oxygen saturation in blood of the chest of the subject to, for example, a clinician even when the subject is at home. The chest-based oximeter may comprise a receiver. The receiver may receive instructions which may be used to control the operation of the chest-based oximeter.

15

20

25

Alternatively, the transmitter may transmit signals representing the radiation detected by the detector to a remote receiver, which comprises a processor which uses the signal or signals to provide a measure of the oxygen saturation of haemoglobin in blood of the chest.

30

The transmitter may wirelessly transmit the one or more signals to the remote receiver. This means that the chest-based oximeter does not require leads to connect to the remote receiver, which may otherwise impede movement of the subject.

The chest-based oximeter may comprise a hydrogel interface. The hydrogel interface may, in use, be attached to the chest of the subject. The hydrogel interface may be placed in contact with skin of the chest.

10 The hydrogel interface may comprise adhesive, which is used to attach it to the skin. The adhesive may be a pressure-sensitive adhesive. The hydrogel interface may have substantially similar visco-elastic properties as skin. The hydrogel interface may have a Young's modulus substantially similar to that of skin. The hydrogel interface may be flexible. The

15 hydrogel interface may be flexible to allow it to flex with movement of the subject. The hydrogel interface may be flexible to allow it to flex with movement of the subject, such that it remains attached to the chest. The hydrogel interface may be flexible to allow it to flex with movement of the subject, such that radiation from the radiation source is emitted

20 substantially perpendicular onto the measurement site of the subject. The hydrogel interface may be flexible to allow it to flex with movement of the subject, such that motion-induced artefacts in the reflected radiation detected by the detector are reduced. The hydrogel interface may have substantially similar electrical properties as skin. This will give overall

25 similar ionic content and therefore no potential gradients. The hydrogel interface may act as a second skin for the measurement site.

The hydrogel interface may be situated between the radiation source and radiation detector and the chest of the subject. The hydrogel interface

30 may cover the radiation source. The hydrogel interface may cover the

radiation detector. The radiation source may emit radiation through the hydrogel interface onto the chest. The hydrogel interface may diffuse the radiation emitted from the radiation source. The diffusion of the radiation may average angles of penetration of the radiation into the chest. The diffusion may be, for example, from an approximately 1mm^2 source to an area of approximately 1cm^2 . The hydrogel interface may provide coupling of the radiation from the source to the chest. The radiation detector may detect radiation reflected from the chest which passes through the hydrogel interface. The hydrogel interface may diffuse the radiation reflected from the chest. The diffusion of the radiation may average angles of reflection of the radiation from the chest. The diffusion may be, for example, from an approximately 1mm^2 source to an area of approximately 1cm^2 . The hydrogel interface may provide coupling of the radiation from the chest to the radiation detector. The diffusion allows for improved averaging of the absorption of the radiation, and thus improved accuracy of the oximeter. The coupling improves the detection of the reflected radiation against background noise/artefact. This gives a cleaner and more sensitive analysis leading to higher accuracy. The optical coupling stops stray light from interfering with the detected radiation.

The hydrogel interface may be shaped to fit the chest of the subject. The hydrogel interface may comprise a film. The hydrogel interface may comprise a ball. The hydrogel interface may have a thickness in the range of approximately 0.5mm to approximately 1cm . The hydrogel interface may have an area of approximately 1cm^2 . The hydrogel interface may be up to approximately 85% water based. The hydrogel interface is preferably biocompatible. It will then have a low toxicity and sensitisation effects on the subject.

It has been found that when the chest-based oximeter is provided with a hydrogel interface, the signals produced by the radiation detector have waveforms which can be sharper and more consistent, than those produced when no hydrogel interface is used. When no hydrogel interface is used, the signals produced by the radiation detector are stronger than those produced when a hydrogel interface is used, but the signals may be more prone to influence by slight movements between the oximeter and the skin of the subject and between the skin and underlying bone.

10 The chest-based oximeter may have a low profile. This will make it easier to wear than conventional oximeters used on a finger, ear or toe.

The chest-based oximeter may, in use, be attached to a region of the chest above the notch sternum. Positioning of the chest-based oximeter above the notch region of the chest of the subject will ensure high coupling of the oximeter with the main heart blood paths. Positioning of the chest-based oximeter above the notch region of the chest of the subject avoids hysteresis or time delays in signals detected by the oximeter. Positioning of the chest-based oximeter above the notch region of the chest of the subject also makes the oximeter easy for the subject to wear.

The chest-based oximeter may be used to measure a wide range of oxygen saturation values. This may be tested by the subject carrying out a controlled breathing exercise, which manipulates the subject's blood oxygen saturation values, through a wide range of saturation values. It has been found that decreases in oxygen saturation values were indicated earlier at the chest than at the finger, that measurements of oxygen saturation taken at the chest fell at a faster rate than measurements of oxygen saturation taken at the finger, and that chest oxygen saturation values fell to a lower level than finger oxygen saturation values.

The chest-based oximeter may also measure carbon monoxide saturation in blood of the chest of the subject.

5 The chest-based oximeter may form part of a system which measures one or more vital signs of the subject. The vital signs may comprise any of heart rate, ECG, respiration rate, temperature. The system may comprise the V-patch vital signs measurement system of Sensor Technology & Devices.

10

According to a second aspect of the invention there is provided a method of measuring oxygen saturation of haemoglobin in blood of the chest of a subject, comprising

attaching an oximeter to the chest using a pressure device of the oximeter adapted to apply pressure thereto to connect the oximeter to the chest, operating at least one radiation source of the oximeter to emit radiation onto the chest,

15

operating at least one radiation detector of the oximeter to detect radiation reflected from the chest, and

20

using the radiation detected by the detector to measure the oxygen saturation of haemoglobin in blood of the chest.

Embodiments of the invention will now be described by way of example only, with reference to the accompanying drawings, in which:

25

Figure 1 is a schematic representation of a first embodiment of an chest-based oximeter according to the invention, shown positioned on a subject's chest;

Figure 2 is a schematic representation of the chest-based oximeter of Figure 1, and

5 Figure 3 is a schematic representation of a second embodiment of a chest-based oximeter according to the invention.

Figure 1 shows a first embodiment of a chest-based oximeter 1 according to the invention, placed on a subject's chest. The oximeter 1 is positioned on a region of the chest above the notch sternum, as illustrated, and
10 measures oxygen saturation of haemoglobin in blood of the region of the chest above the notch sternum.

Figure 2 shows the chest-based oximeter 1 in more detail. The oximeter 1 comprises a housing 3, two radiation sources 5, 7, a radiation detector 9
15 and a pressure device 11. The housing comprises a flexible substrate. The radiation sources 5, 7 and the radiation detector 9 are each mounted on a surface of the housing 3, as shown, in a reflectance measurement arrangement. The sources and the detector are spaced apart by a distance in the range of approximately 0.5mm to approximately 2cm. The
20 radiation sources 5, 7 comprise LEDs. The radiation source 5 emits radiation having a visible peak wavelength in the red region of the visible spectrum. The radiation source 7 emits radiation having an infra red peak wavelength of 920nm or 1300nm. The radiation source 7 comprises an IR LED, such as those supplied by Roithner Lasertechnik. The radiation
25 detector 9 comprises a photodiode, such as the TSL220 photodiode supplied by Texas Instruments.

As described, the chest-based oximeter 1 comprises a conventional arrangement of radiation sources in terms of number and wavelength. It
30 will be appreciated that the oximeter 1 could comprise a different number

of radiation sources with different wavelengths, for example a first radiation source which emits radiation having an infra red peak wavelength of 900nm and a second radiation source which emits radiation having an infra red peak wavelength of 1300nm.

5

The pressure device 11 comprises a stretchable foam material, which has a Young's modulus which is lower than that of the skin of the chest of the subject. The pressure device 11 is attached at a first side thereof to the surface of the housing 3 on which the radiation sources and detector are mounted. The pressure device 11 as shown extends along the surface of the housing 3 and around the sides of the housing 3. It will be appreciated that other shapes of pressure device 11 may be used, for example, the pressure device may only extend along part of the surface of the housing 3. In use, the pressure device 11 is applied at a second side thereof to skin of the region of the chest above the notch sternum of the subject. As the Young's modulus of the skin and the Young's modulus of the pressure device material are different, this will cause the pressure device 11 to stress and apply a pressure on the oximeter towards the skin, and connect the oximeter to the chest. The pressure device 11 may apply a pressure in the range of approximately 1 Pascal to approximately 100000 Pascal on the oximeter towards the chest of the subject.

The pressure device 11 is of a thickness to position the radiation sources 5, 7 and the radiation detector 9 between approximately 1cm and approximately 20 cm above the notch region of the chest. The pressure device 11 is shaped to optically couple the radiation from the radiation sources 5, 7 to the notch region of the chest, and to optically couple the radiation reflected from the notch region of the chest to the radiation detector 9.

30

The chest-based oximeter 1 further comprises a power supply, a controller, a processor, a receiver, a transmitter and electronic circuitry, all located within the housing 3. The electronic circuitry connects the radiation sources 5, 7 and the radiation detector 9 to the power supply, for supply of power thereto. It will be appreciated that, alternatively, a power supply could be provided external to the oximeter 1. The electronic circuitry connects the radiation sources 5, 7 to the controller, which acts to control the operation of the sources. The electronic circuitry connects the radiation detector 9 to the processor. The processor receives signals from the radiation detector 9, and uses the signals to provide a measure of the oxygen saturation. The processor may pass measurement of the oxygen saturation to the transmitter, for transmission to a device external to the oximeter. It will be appreciated that the chest-based oximeter 1 may be connected to a processor which is situated external to the oximeter. The oximeter may then transmit signals from the radiation detector 9 to a receiver of the external processor. The controller of the oximeter 1 may receive control signals via the receiver from a source external to the oximeter, to control operation of the oximeter. For example, the control signals may be generated by a physician of the subject. The transmitter and receiver of the oximeter 1 may be connected by wires or, preferably, wirelessly connected to devices external to the oximeter.

The entire chest-based oximeter 1 has a low profile. This will make it easier for the subject to wear than conventional oximeters used on a finger, ear or toe.

In use, the chest-based oximeter 1 is attached to the region of the chest above the notch sternum of the subject using the pressure device 11, and measures oxygen saturation of haemoglobin in blood of the notch region of the chest, as follows. The controller receives a signal via the receiver

causing it to activate the radiation sources 5, 7. These emit red and IR radiation onto the notch region of the chest. The radiation from the sources is transmitted into the notch region, and some of the radiation is absorbed by the notch region of the chest, and particularly haemoglobin in blood in arteries of the chest region. Some of the radiation from the sources is reflected from the notch region of the chest, and particularly haemoglobin in the blood in the arteries. The level of absorption of red and IR radiation in blood, depends on the oxygenation level of haemoglobin in the blood, and, for blood having a particular haemoglobin oxygenation level, the red and IR radiation will be absorbed by different amounts. The detector 9 detects red and IR radiation reflected from the notch region. The detector 9 produces signal representative of the reflected radiation, and passes these signals to the processor. The processor uses the signals in an analysis algorithm and calculates the absorption of the red and IR radiation, and computes a measure of the oxygen saturation of haemoglobin in blood of the arteries of the notch sternum region of the chest. This is usually expressed as a percentage of total saturation. The blood flow through the arteries will be pulsatile in form. The oximeter 1 is designed to detect radiation reflected from blood in the arteries, by being configured to detect pulsatile reflected radiation. The oximeter 1 is able to distinguish the pulsatile signals from other more static signals, e.g. signals transmitted through tissue or veins. The oximeter 1 is also able to measure the heart rate of the subject, and to produce an indication of the quality of blood flow through the arteries.

Positioning of the oximeter 1 above the notch region of the chest of the subject ensures high coupling of the oximeter 1 with the main heart blood arteries. Positioning of the oximeter 1 above the notch region of the chest also avoids hysteresis in signals detected by the oximeter 1, and makes the oximeter easy for the subject to wear.

As stated earlier, it has been found that the signals representing radiation reflected from the chest are weaker than signals representing radiation transmitted through the finger. Nevertheless, the chest signals are measurable, are sufficiently strong to measure accurately oxygen saturation values and accurate heart rate values, and are sufficiently repeatability for good quality measurements.

Figure 3 shows a second embodiment of a chest-based oximeter 21, used to measure oxygen saturation of haemoglobin in blood of a subject. The oximeter 21 comprises a housing 23, two radiation sources 25, 27, a radiation detector 29, a pressure device 30 and a hydrogel interface 31. The housing comprises a flexible substrate. The radiation sources 25, 27 and the radiation detector 29 are each mounted on a surface of the housing 23, as shown, in a reflectance measurement arrangement. The sources and the detector are spaced apart by a distance in the range of approximately 0.5mm to approximately 2cm. The radiation sources 25, 27 comprise LEDs. The radiation source 25 emits radiation having a visible peak wavelength in the red region of the visible spectrum. The radiation source 27 emits radiation having an infra red peak wavelength. As described, the chest-based oximeter 21 again comprises a conventional arrangement of radiation sources in terms of number and wavelength. It will be appreciated that the oximeter 21 could comprise a different number of radiation sources with different wavelengths, for example one or two radiation sources which emit radiation having one or more infra red peak wavelengths.

The pressure device 30 may comprise any of a finger push device, a belt, a biasing device, for example, a spring. The pressure device 30 is attached at a first side thereof to the surface of the housing 23 on which

the radiation sources and detector are not mounted. The pressure device 30 as shown extends along the surface of the housing 23 and around the sides of the housing 23. It will be appreciated that other shapes of pressure device 30 may be used, for example, the pressure device may only extend along part of the surface of the housing. In use, the oximeter 21 is applied to the region of the chest above the notch sternum of the subject. The pressure device 30 is activated and applies a pressure on the oximeter 21 towards the chest, and connects the oximeter 21 to the chest. The pressure device 11 may apply a pressure in the range of approximately 1 Pascal to approximately 100000 Pascal on the oximeter towards the chest of the subject.

The hydrogel interface 31 is shaped to fit the chest of the subject. The hydrogel interface 31 comprises a film, having a thickness in the range of approximately 0.5mm to approximately 1cm. The hydrogel interface 31 is biocompatible, to reduce toxicity and sensitisation effects on the subject.

The hydrogel interface 31 is attached at a first side thereof to the surface of the housing 23 on which the radiation sources and detector are mounted. The hydrogel interface 31 is attached at a second side thereof to the chest of the subject. The hydrogel interface 31 is placed in contact with skin of the measurement site, and comprises adhesive, which is used to attach it to the skin. The adhesive is preferably pressure-sensitive. The hydrogel interface 31 has substantially similar visco-elastic properties as skin, and a Youngs modulus substantially similar to that of skin. The hydrogel interface 31 is flexible, to allow it to flex with movement of the subject, such that it remains attached to the chest and radiation from the radiation sources is emitted substantially perpendicular onto the measurement site. Such flexibility of the hydrogel interface 31 will reduced motion-induced artefacts in the reflected radiation detected by the

detector 29. The hydrogel interface 31 preferably also has substantially similar electrical properties as skin. In effect, the hydrogel interface 31 acts as a second skin for the chest of the subject.

5 The hydrogel interface 31 is situated between the radiation sources 25, 27 and the radiation detector 29, and the chest of the subject, as shown. The hydrogel interface 31 thus covers the radiation sources 25, 27, which emit radiation through the hydrogel interface 31 onto the chest. The hydrogel interface 31 diffuses the radiation emitted from the radiation sources, to
10 average angles of penetration of the radiation into the chest. The hydrogel interface 31 also provides coupling of the radiation from the sources 25, 27 to the chest. The hydrogel interface 31 also covers the radiation detector 29, which detects radiation reflected from the chest which passes through the hydrogel interface 31. The hydrogel interface 31 diffuses the
15 radiation reflected from the chest, to average angles of reflection of the radiation from the chest. The hydrogel interface 31 also provides coupling of the radiation from the chest to the radiation detector 29.

The oximeter 21 further comprises a power supply, a controller, a
20 processor, a receiver, a transmitter and electronic circuitry, all located within the housing 23. The electronic circuitry connects the radiation sources 25, 27 and the radiation detector 29 to the power supply, for supply of power thereto. It will be appreciated that, alternatively, a power supply could be provided external to the oximeter 21. The electronic
25 circuitry connects the radiation sources 25, 27 to the controller, which acts to control the operation of the sources. The electronic circuitry connects the radiation detector 29 to the processor. The processor receives signals from the radiation detector 29, and uses the signals to provide a measure of the oxygen saturation. The processor may pass measurement of the
30 oxygen saturation to the transmitter, for transmission to a device external

to the oximeter. It will be appreciated that the chest-based oximeter may be connected to a processor which is situated external to the oximeter 21. The oximeter may then transmit signals from the radiation detector 29 to a receiver of the external processor. The controller of the oximeter 21 may receive control signals via the receiver from a source external to the oximeter, to control operation of the oximeter. For example, the control signals may be generated by a physician of the subject. The transmitter and receiver of the oximeter 21 may be connected by wires or, preferably, wirelessly connected to devices external to the oximeter.

10

In use, the oximeter 21 is attached to the chest of the subject via the hydrogel interface 31, and the pressure device 30 is activated to apply pressure on the oximeter towards the chest. The region of the chest of the subject may be above the notch sternum of the chest. The controller receives a signal via the receiver causing it to activate the radiation sources 25, 27. These emit red and IR radiation onto the measurement site. The radiation from the sources is transmitted into the chest, and some of the radiation is absorbed by the chest, and particularly haemoglobin in blood in arteries of the chest. Some of the radiation from the sources is reflected from the chest, and particularly haemoglobin in the blood in the arteries. The level of absorption of red and IR radiation in blood, depends on the oxygenation level of haemoglobin in the blood, and, for blood having a particular haemoglobin oxygenation level, the red and IR radiation will be absorbed by different amounts. The detector 29 detects red and IR radiation reflected from the chest. The detector 29 produces a signal representative of the reflected radiation, and passes these signals to the processor. The processor uses the signals in an analysis algorithm and calculates the absorption of the red and IR radiation, and computes a measure of the oxygen saturation of haemoglobin in blood of the arteries of the chest. This is usually expressed as a percentage of

30

total saturation. The blood flow through the arteries will be pulsatile in form. The oximeter 21 is designed to detect radiation reflected from blood in the arteries, by being configured to detect pulsatile reflected radiation. The oximeter 21 is able to distinguish the pulsatile signals from other more static signals, e.g. signals transmitted through tissue or veins. The
5 oximeter 21 is also able to measure the heart rate of the subject, and to produce an indication of the quality of blood flow through the arteries.

It has been found that when the chest-based oximeter 21 is provided with
10 a hydrogel interface 31, the signals produced by the radiation detector 29 have waveforms which are sharper and more consistent, than those produced when no hydrogel interface is used. When no hydrogel interface is used, the signals produced by the radiation detector are stronger than those produced when a hydrogel interface is used, but the signals are
15 more prone to influence by slight movements between the oximeter and the skin of the subject and between the skin and underlying bone.

CLAIMS

1. A chest-based oximeter for measuring oxygen saturation of haemoglobin in blood of the chest of a subject, comprising
5 at least one radiation source adapted to emit radiation onto the chest, at least one radiation detector adapted to detect radiation reflected from the chest, and a pressure device adapted to apply pressure to the oximeter to connect the oximeter to the chest.
10
2. A chest-based oximeter according to claim 1 in which the pressure device is applied to skin of the chest of the subject, and comprises a material which has a Young's modulus which is lower than that of the skin of the chest of the subject.
15
3. A chest-based oximeter according to claim 2 in which the pressure device stresses and applies a pressure on the oximeter towards the skin, to connect the oximeter to the chest.
- 20 4. A chest-based oximeter according to claim 1 in which the pressure device comprises any of a biasing device, a finger push device, a belt.
5. A chest-based oximeter according to any preceding claim in which the pressure device applies a pressure in the range of approximately 1
25 Pascal to approximately 100000 Pascal.
6. A chest-based oximeter according to any preceding claim in which the pressure device optically couples the radiation from the radiation source to the chest of the subject, and optically couples the radiation
30 reflected from the chest of the subject to the radiation detector.

7. A chest-based oximeter according to any preceding claim in which the at least one radiation source and the at least one radiation detector are mounted in the chest-based oximeter such that they are spaced apart by a distance in the range of approximately 0.5mm to approximately 2cm.

5

8. A chest-based oximeter according to any preceding claim in which the at least one radiation source and the at least one radiation detector are mounted in the chest-based oximeter such that, in use, they are positioned in the range of approximately 1cm to approximately 20cm above the chest of the subject.

10

9. A chest-based oximeter according to any preceding claim in which the at least one radiation source emits radiation having one or more infra red peak wavelengths.

15

10. A chest-based oximeter according to claim 9 which further comprises a second radiation source which emits radiation having one or more infra red peak wavelengths.

20

11. A chest-based oximeter according to claim 10 in which the at least one radiation source emits radiation having at least a first infra red peak wavelength, and the second radiation source emits radiation having at least a second, different, infra red peak wavelength.

25

12. A chest-based oximeter according to any of claims 9 to 11 in which the or each infra red peak wavelength is in the range of 600nm to 1500nm, for example 780nm, 810nm, 820nm, 830nm, 840nm, 850nm, 870nm, 880nm, 890nm, 910nm, 940nm, 970nm, 1050nm, 1070nm, 1200nm, 1300nm, 1350nm, 1450nm, 1550nm.

30

13. A chest-based oximeter according to any of claims 1 to 8 in which the at least one radiation source emits radiation having one or more visible peak wavelengths.
- 5 14. A chest-based oximeter according to claim 13 which further comprises a second radiation source which emits radiation having one or more visible peak wavelengths.
- 10 15. A chest-based oximeter according to any of claims 1 to 8 in which the at least one radiation source emits radiation having one or more visible peak wavelengths, and the oximeter further comprises a second radiation source which emits radiation having one or more infra red peak wavelengths.
- 15 16. A chest-based oximeter according to any preceding claim which comprises a hydrogel interface.
17. A chest-based oximeter according to any preceding claim which has a low profile.
- 20 18. A chest-based oximeter according to any preceding claim which also measures carbon monoxide saturation in blood of the chest of the subject.
- 25 19. A chest-based oximeter according to any preceding claim which forms part of a system which measures one or more vital signs of the subject, such as any of heart rate, ECG, respiration rate, temperature.
- 30 20. A method of measuring oxygen saturation of haemoglobin in blood of the chest of a subject, comprising

- attaching an oximeter to the chest using a pressure device of the oximeter adapted to apply pressure thereto to connect the oximeter to the chest, operating at least one radiation source of the oximeter to emit radiation onto the chest,
- 5 operating at least one radiation detector of the oximeter to detect radiation reflected from the chest, and using the radiation detected by the detector to measure the oxygen saturation of haemoglobin in blood of the chest.

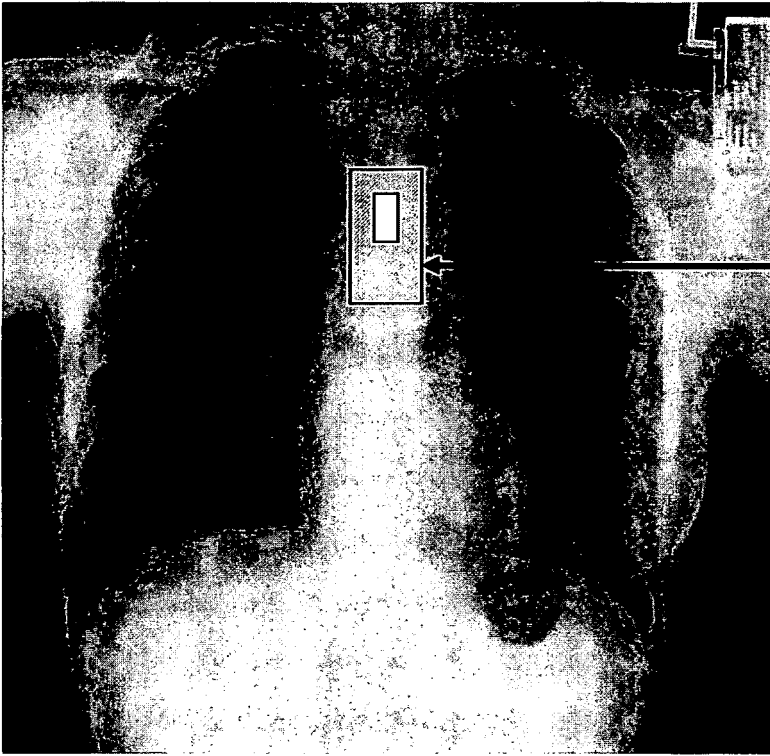


Fig 1

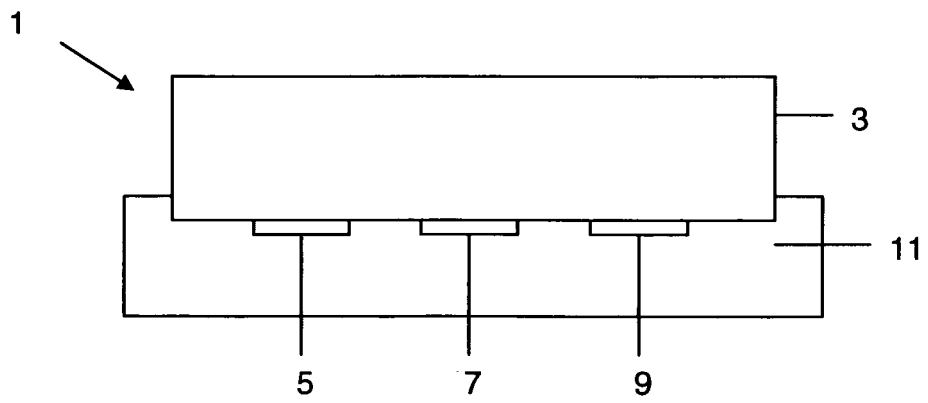


Fig 2

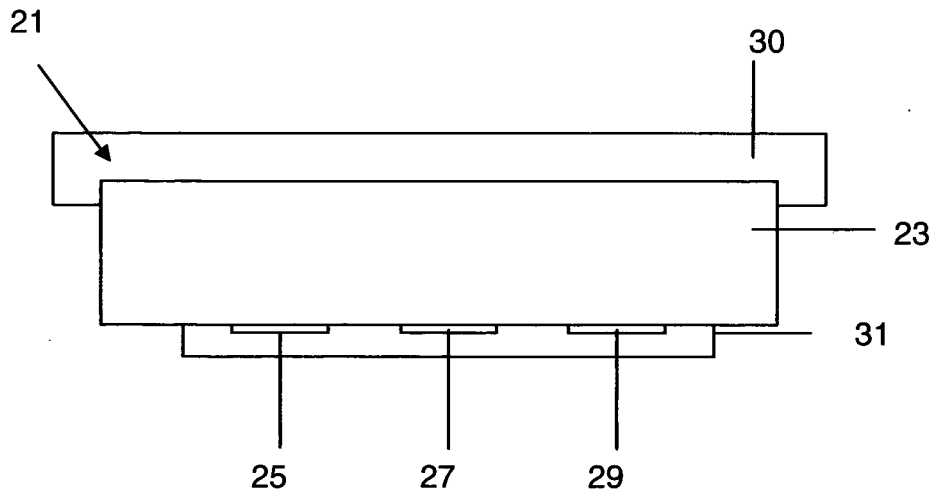


Fig 3

INTERNATIONAL SEARCH REPORT

International application No
PCT/GB2008/003708A. CLASSIFICATION OF SUBJECT MATTER
INV. A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 99/47039 A (AIHONEN JUKKA [FI]; KIRVESKARI JUHA [FI]; PENTTILAE HEIKKI [FI]; SIRKI) 23 September 1999 (1999-09-23) page 7, line 25 - page 11, line 12; figure 5	1, 4, 5, 7, 9-13, 15, 19, 20
X	US 2002/124295 A1 (FENWICK LOEL [US] ET AL) 12 September 2002 (2002-09-12) paragraphs [0070] - [0072]; claims 1-4	1, 4, 5, 8, 9, 12, 13, 15, 17, 19, 20
X	WO 96/16591 A (AIHONEN JUKKA [FI]; PENTTILAE HEIKKI [FI]; SIRKIAE JOUNI [FI]; TUOMINE) 6 June 1996 (1996-06-06) paragraphs [0020] - [0039]; claims ----- -/--	1, 4, 5, 17-20

 Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents :

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

& document member of the same patent family

Date of the actual completion of the international search

17 February 2009

Date of mailing of the international search report

03/03/2009

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Manschot, Jan

INTERNATIONAL SEARCH REPORT

International application No

PCT/GB2008/003708

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	GB 2 425 181 A (PISANI JUSTIN [GB]; HOWARD PETER [GB]; CADE DANIEL [GB]; WARD STEPHEN) 18 October 2006 (2006-10-18) page 5, paragraph 2 -----	1,4,5, 17,19,20
X	US 2007/142715 A1 (BANET MATTHEW J [US] ET AL) 21 June 2007 (2007-06-21) paragraphs [0008], [0009] -----	1,20
P,X	EP 1 946 697 A (SUISSE ELECTRONIQUE MICROTECH [CH]) 23 July 2008 (2008-07-23) the whole document -----	1,4,5, 7-13,15, 17,20

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/GB2008/003708

Patent document cited in search report	Publication date	Publication date	Patent family member(s)	Publication date
WO 9947039	A	23-09-1999	NONE	
US 2002124295	A1	12-09-2002	NONE	
WO 9616591	A	06-06-1996	AU 690764 B2	30-04-1998
			AU 3985095 A	19-06-1996
			EP 0796056 A1	24-09-1997
			FI 945613 A	30-05-1996
			JP 10509083 T	08-09-1998
GB 2425181	A	18-10-2006	NONE	
US 2007142715	A1	21-06-2007	NONE	
EP 1946697	A	23-07-2008	US 2008171926 A1	17-07-2008

专利名称(译)	测量血红蛋白的氧饱和度		
公开(公告)号	EP2214551A1	公开(公告)日	2010-08-11
申请号	EP2008843880	申请日	2008-11-03
[标]申请(专利权)人(译)	INTELESENS		
申请(专利权)人(译)	INTELESENS有限公司		
当前申请(专利权)人(译)	INTELESENS有限公司		
[标]发明人	MCLAUGHLIN JAMES ANDREW ANDERSON JOHN MCCUNE		
发明人	MCLAUGHLIN, JAMES, ANDREW ANDERSON, JOHN, MCCUNE		
IPC分类号	A61B5/00		
CPC分类号	A61B5/6831 A61B5/01 A61B5/024 A61B5/14551		
优先权	2007021575 2007-11-02 GB		
其他公开文献	EP2214551B1		
外部链接	Espacenet		

摘要(译)

本发明提供一种基于胸部的血氧计 (1) , 用于测量受试者胸部血液中血红蛋白的氧饱和度, 包括至少一个适于将辐射发射到胸部的辐射源 (5,7) , 至少一个辐射检测器 (9) 适于检测从胸部反射的辐射, 以及压力装置 (11) , 其适于向血氧计施加压力以将血氧计连接到胸部。