



(51) International Patent Classification:

A61B 5/0476 (2006.01) **A61B 5/16** (2006.01)
A61B 5/00 (2006.01) **G06F 19/00** (2011.01)

(21) International Application Number:

PCT/CA20 13/000769

(22) International Filing Date:

12 September 2013 (12.09.2013)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/700,615 13 September 2012 (13.09.2012) US

(71) Applicant: **YRT LIMITED** [CA/CA]; 1001 Wellington
Crescent, Winnipeg, Manitoba R3M 0A7 (CA).

(72) Inventor: **YOUNES, Magdy**; 1001 Wellington Crescent,
Winnipeg, Manitoba R3M 0A7 (CA).

(74) Agents: **STEWART, Michael, I.** et al; Sim & McBurney,
330 University Avenue 6th Floor, Toronto, Ontario M5G
1R7 (CA).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, ^{EST} IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.


(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: METHOD AND SOFTWARE TO DETERMINE PROBABILITY OF SLEEP/WAKE STATES AND QUALITY OF SLEEP AND WAKEFULNESS FROM AN ELECTROENCEPHALOGRAM

Fig. 1

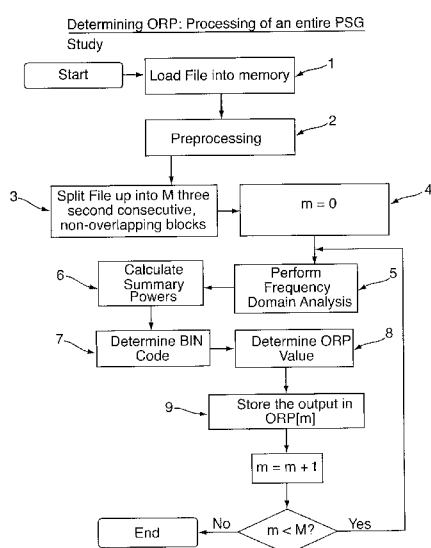

(57) Abstract: Method and software are provided to format a probability index that reflects where an electroencephalogram (EEG) pattern lies within the spectrum of wakefulness to deep sleep, which employs a computer/microprocessor that performs frequency domain analysis of one or more discrete sections (Bins) of the EEG to determine the EEG power at specified frequencies, optionally calculates the total power over specified frequency ranges, assigns a rank to the power at each frequency, or frequency range, assigns a code to the Bin that reflects the ranking of the different frequencies or frequency ranges, and determines an index that reflects where said EEG pattern within said Bin(s) lies within the spectrum of wakefulness to deep sleep by use of a reference source, such as a look-up table or other suitable decoding instrument. The reference source is obtained by calculating the probability of Bins with different codes occurring in epochs scored as awake or asleep in reference files scored by one or more expert technologists or by an automatic scoring software.

TITLE OF INVENTION**METHOD AND SOFTWARE TO DETERMINE PROBABILITY
OF SLEEP/WAKE STATES AND QUALITY OF SLEEP AND
WAKEFULNESS FROM AN ELECTROENCEPHALOGRAM**FIELD OF THE INVENTION

[0001] The invention relates to the determination of the probability of sleep/wake states and quality of sleep and wakefulness from an electroencephalogram.

BACKGROUND TO THE INVENTION

[0002] Determining whether a patient/individual is awake or asleep is an essential first step in the analysis of sleep records obtained during investigation of sleep disorders. In some cases such investigations require only knowledge of whether the patient was awake or asleep. An example would be home monitoring for the diagnosis of sleep apnea. Here, if a patient does not show evidence of sleep apnea (e.g. dips in oxygen saturation, interrupted snoring) a diagnostic dilemma arises in that one does not know whether the negative study was because the patient did not sleep. In other cases, it is necessary to have a more comprehensive description of sleep, such as amount of time spent in each of the different sleep stages, which reflect the type rapid eye movement (REM vs. non-REM) and depth (stages N1, N2, N3) of sleep. This information is needed to evaluate the quality of sleep and is particularly useful in cases of excessive somnolence and insomnia. In the latter cases, distinguishing a sleep state from an awake state is a first step towards determining which stage the patient is in. Typically, once it is clear that the patient is asleep, decisions as to what sleep stage the patient is in is based on the presence of specific features in an electroencephalogram (EEG), Eye movements (EOG), intensity of chin muscle activity (chin EMG), among other findings.

[0003] Apart from analysis of formal sleep records, it is of considerable importance to be able to determine the level of vigilance in situations that require a high level of alertness such as during driving long distances, operating heavy machinery or equipment of critical nature such as air-traffic control. It is well known that decreased alertness, for example, as a result of boredom, alcohol, drugs, or sleep deprivation, are responsible for numerous driving and occupational accidents. There are different levels to what is considered as wakefulness. These range from fully alert to drowsy to having periods (a few seconds) of micro-sleep. Cognitive and motor performance is impaired as level vigilance decreases even if the subject is still technically awake. To my knowledge, there are currently no methods that identify different levels of wakefulness.

[0004] The present invention deals with a method for developing a continuous quantitative scale that describes the level of vigilance/consciousness across the whole spectrum from full alertness to the deepest sleep. When embedded in appropriate equipment this method can be used to a) evaluate the level of vigilance in situations requiring alertness, b) determine whether a subject is awake or asleep, c) determine the quality of sleep in sleep studies and, d) as an initial step in detailed sleep scoring with the subsequent steps relying on identification of the additional features using any of well described approaches in prior art. The current method does not cover steps to classify sleep into its various conventional stages. Rather, the current process generates a value (Probability of being awake (P_w); Odds Ratio Product (ORP)), which reflects the probability of any given section of the EEG record falling in a period that would be staged as awake by experienced scorers or by validated automatic scoring systems. I have established the presence of a clear negative correlation between this value (P_w , ORP) and depth of sleep as measured by conventional visual criteria. As such, P_w / ORP can be used as a continuous scale that describes the quality of wakefulness or sleep in certain sections of the record or as a lumped average for the whole night. Every sleep technologist recognizes that within any given conventional sleep stage there is a continuum of sleep quality. For example, an EEG pattern that is now classified as stage N1 according to conventional criteria could be very close to an awake pattern on one end of the spectrum or very close to the deeper stage 2 on the other end. Likewise, there is a huge range of patterns in what is now classified as an awake state, ranging from full wakefulness to quite wakefulness, to wakefulness interrupted by mini-sleep periods, and so on. The use of this index ($P_w \text{ ORP}$) allows an expression of the quality of sleep on a continuous scale regardless of the conventional classification. It also can be used to reflect the overall quality of sleep in one number. This is much easier to understand and interpret than the conventional histogram of the different stages vs. time (the Hypnogram).

[0005] The current accepted practice for scoring sleep records is manual scoring by expert technologists. This is time consuming, and by extension, quite expensive. Manual scoring is also highly subjective with different experts producing different results. As indicated above, the EEG pattern in many of the epochs (usually 30 seconds in length) are on the border between two stages (e.g. awake vs. N1). Some may score these epochs one way while others may score it another way. Also, there are large differences in how experts interpret the guidelines, which are often vague. Manual scoring is also an extremely tedious task and is often associated with gross errors related to inattention. Automation, accordingly, has many potential advantages, if it can be shown to be accurate.

[0006] Manual scoring of sleep relies primarily on visual appreciation of the different EEG patterns. There have been many attempts at automating EEG scoring but the results have not been up to what is required for acceptance. Virtually all automated methods rely on frequency analysis of the EEG. This analysis produces the power in different frequencies. The relevant frequency content of the EEG is 0.3 to 40Hz. Any EEG pattern can be accurately described by the power spectrum of the EEG, namely the power in each of the relevant frequencies. Many previous approaches have been described that exploit the power spectrum of the EEG to arrive at sleep stages. These approaches typically use various complex signal analysis models. The problem is that there is a huge number of frequency spectra that could be called awake and another huge number of patterns that could fall in what the eye perceives as sleep, and so many patterns that could be called either by eye. A high power in the beta range (>14Hz) may be present in full wakefulness or in the deepest sleep. Likewise, a high alpha power (7 to 14) could be present in wakefulness or in any of the other sleep stages. Thus, the interpretation of power in a given frequency must take into account the power in other relevant frequencies. Yet, as indicated earlier, the various combinations of powers that can be encountered during wakefulness or sleep are enormous and do not lend themselves to a unitary quantitative model. Hence in this invention we use an empiric approach by assigning codes to thousands of EEG frequency patterns and simply determining how often each code is found in epochs that expert scorers score as awake or asleep. Once a reference resource is established (probability of each code to be scored awake or asleep), scoring of un-scored files simply entails determining the spectral code of selected EEG intervals and determining the probability of Sleep/Wake state by use of the reference resource.

SUMMARY OF THE INVENTION

[0007] 1) The present invention takes a radically different approach to scoring the EEG **for** determining the level of vigilance or sleep. It starts by performing frequency analysis of the EEG on discrete time intervals (Bins; e.g. 3 seconds, but clearly other intervals may be used). Also, as done with other methods, the power or amplitude in certain ranges of frequency is combined to reduce the number of variables to a manageable level. For example, the total power in frequencies between 0.3 and 2.5 is added, giving the power in the slowest range of waves (generally called Delta power). The ranges need not conform to any conventional classification (e.g. Delta, Theta, alpha, sigma, betal, beta 2) and may or not be overlapping. Clearly, the more ranges are used, the greater the resolution. But, this greatly affects the number of combinations to be rated and, by extension, processing time and number of files to be expertly scored to produce the reference resource (look-up table, equation... etc). In our preferred embodiment, we have

selected four frequency ranges (0.3 to 2.33Hz (Delta); 2.67 Hz to 6.33 Hz (Theta); 7.33 Hz to 14.00 Hz (Alpha/Sigma); and >14 Hz (Beta)). The frequency range from 6.67 to 7.00 was not included in the Theta power as some alpha waves in clearly awake regions can occasionally be seen in this range in some patients.

[0008] 2) The next step is to assign the power or amplitude in each frequency range in each Bin a rank (expressed as a number, letter or symbol) that reflects its relative magnitude. This is basically a normalization process that takes into account the entire range of powers or amplitudes observed in the relevant frequency range across as many sleep studies as possible. For this step, a number of EEG studies (files) that represent the full spectrum of relevant clinical conditions are scored manually or by a validated automatic system. The power or amplitude in each frequency range (selected in step 1), is then determined in Bins of equal length in these reference files. For example, we used initially 40 files, each about 8 hours long or 9600 3-sec Bins (8*60*20), for a total of approximately 400,000 bins. These values were then sorted in ascending order. The entire range was broken into smaller ranges of equal number. Clearly any number of ranges can be used. In the extreme, the actual power in each Range may be used as the rank. The larger the number of ranges the better the resolution but the more processing power and time are required. We used 10 ranges and each range was assigned a rank (we used numerical rank, 0 to 9). Thus, we divided the entire range of Delta power in the 400,000 samples into 10 equal ranges, the lowest range (Rank 0) includes all values in the lowest 10 percentile and Rank 1 includes all values between the 10th and 20th percentile, and so on until Rank 9 which includes all values above the 90th percentile. The same was done for the other frequency ranges. The result was a table (e.g. Table 1) that can be looked up to determine a Rank to assign to the power in each frequency range in the Bin being examined.

TABLE 1

Rank	Delta	Theta	Alpha/Sigma	Beta
0	5.85	4.55	3.0	0.95
1	9.38	6.97	4.6	1.3
2	13.67	9.63	6.2	1.68
3	19.48	12.9	8.1	2.11
4	28.01	17.15	10.4	2.63
5	41.93	22.98	13.3	3.33
6	66.76	31.37	17.3	4.36
7	117.71	44.64	23.5	6.19
8	258.26	70.84	36.1	10.91
9	258.27+	70.85+	36.08+	10.92+

[0009] This Table is a fixed look-up table in the software. It is based on our results analyzing 40 files obtained from two academic sleep laboratories. Clearly other tables can be used with different frequency groupings, different ranking procedure or different Bin widths. Also, in some laboratories, extrinsic noise or other technical differences can result in somewhat different table values if a large number of files from that laboratory were subjected to the same ranking procedure. An optional feature is therefore to have the ranking table used in a certain laboratory developed specifically from files generated by that laboratory to allow for the technical differences. A variety of Ranking tables can then be available in the library and the appropriate

one is selected when scoring files from laboratories that do not subscribe to recommended guidelines for data acquisition or which have specific noise issues. However, we have found the above table to be satisfactory when used to score files from a variety of laboratories.

[0010] Optionally, a similar table can be developed if other (than spectral power) features of the EEG in the specified frequency ranges are used (e.g. amplitude, Mean Absolute Amplitude (MABs), Total Variation (TV)... etc). In this case, the reference files are processed to generate the feature selected, and the total range of the feature in the reference files is broken into a number of sub-ranges for use in assigning Bin Codes.

[0011] The software determines the power (or amplitude... etc) in each of the selected frequency ranges (4 ranges in the preferred embodiment) in consecutive Bins (3 seconds in the preferred embodiment). Each Bin is then assigned a 4-digit Code based on the value of the feature (power, amplitude... etc) in each frequency range and the corresponding ranks in the look up table. For example, by use of numerical ranks, as in the preferred embodiment, if the powers in the Delta, Theta, Alpha/Sigma and Beta ranges in a given Bin were 52, 10, 17, and 7, the Bin Code would be 6368. This Code then indicates that the power spectrum in this Bin is composed of moderate Delta, relatively low Theta, moderate Alpha/Sigma and High Beta. If letters or symbols are used instead of numbers, the Code is a series of letters and/or symbols that reflect the ranks in the different ranges. From the above description, it is clear that a large number of Bin Codes would result. By using 10 ranks in each of 4 frequency ranges, there results 10,000 different Bin Codes, representing 10,000 different frequency spectra. Clearly this number can be expanded or reduced by different manufacturers of the software. However, we found that this combination provides satisfactory resolution.

[0012] 3) Determining the Awake/Sleep probability for each Bin Code (P_w , ORP): A large number of sleep files, which could be the same files used to develop the ranking tables, are scored manually, or by a validated automatic system, according to conventional criteria (e.g. the

2007 American Academy of Sleep Medicine guidelines). Each file is divided into consecutive bins of the same duration used to develop the ranking table. The Bin Code for each Bin is calculated from the Ranking table. For each Bin Code the fraction of occurrences of this Code in periods scored as awake by the expert technologists, or by the validated automatic system, is determined. For example, if there were 280 instances of Bin Code 1422 in the entire reference dataset and only 20 occurred in epochs staged as awake, the probability of Bins with this Code occurring in awake periods is given a value of 20/280, or 0.07 (or 7%). On the other hand, a Bin number that occurred only in epochs staged as awake by experts would be assigned a probability of 1.0 (or 100%).

[0013] In the preferred embodiment, we obtained conventional manual scoring of 40 files from two academic institutions. The scorer was a very senior certified technologist. She was asked to score each 30-sec epoch as carefully as possible, with no time constraints, using the latest scoring guidelines (AASM 2007 guidelines). The scoring of sleep stages and arousals was reviewed by the inventor and a consensus was reached in epochs where there were differences. The files were broken into 3-sec Bins for an approximate total of 400,000 Bins. Bin Codes were assigned as per step 2. The probability of each of the Bin Codes occurring during epochs scored manually as awake or within scored arousals was determined for each Bin Code. The average number of occurrences of any Bin Code in this data set was 400,000/10,000 or 40. However, as may be expected, there were some Bin Codes that were very frequent (e.g. Bin Codes 0000 and 9999, which occurred several thousand times) and others that were absent or extremely rare. 6200 Bin Codes occurred > 10 times in the dataset and their probability could be determined directly ($\# \text{awake} / \text{total} \#$), while 1000 Bin Codes were completely absent and 2800 Codes occurred only 1-10 times. For these, arbitrary probability values were assigned manually based on their spectral pattern (BIN Code) and the probability of fairly similar Bin Codes that have directly determined probabilities. For example, Bin Codes 1190, 1191, 1192 and 1193 were very poorly represented in the data set (0 to 8 Bins out of 400,000). However, the immediately following bin code (1194) with only slightly higher beta power had good representation (209) and its ORP was 2.5 ($P_w = 100\%$). Furthermore, Bin codes with the same beta rank (0, 1, 2 and 3) but slightly lower alpha rank (namely 1180, 1181, 1182, and 1183) also had a very high ORP values thereby indicating that Bins with very low Delta and Theta powers and high Alpha power occur almost invariably in awake epochs, regardless of Beta rank. Accordingly, the four Bin Codes with little or no representation were assigned a probability of 95%. Clearly with time, the number of files subjected to this process can be increased to obtain a much larger dataset in which fewer Bin Codes are poorly represented. It must be pointed out that because these Bin Codes are quite rare, errors in the assigned arbitrary probabilities would have minimal

consequences. Thus, as an alternative to assuming ORP values in poorly represented bin codes, it may be reasonable to not assign any ORP value to such bin codes or to assign a default value that would indicate that this 3-sec epoch should not be considered in any subsequent analysis.

[0014] From the above steps, a table was generated that contained the probability of being awake for each of the 10,000 Bin Codes. Although the probability values can be used as such (0 to 1.0 or 0 to 100%), we elected to use a different scale where a probability of 40% is assigned a value of 1.0 and other probabilities are assigned a value of (Probability %) / 40. This was because we found that 40% of all 30-second epochs in the reference files were scored awake. So, the odd of being correct if awake is scored at random is 40%. We arbitrarily decided to express all probability values as a ratio (ORP). Thus, a probability of 100% of being awake is given an ORP of 2.5 and a probability of 10% of being awake is given an ORP of 0.25. Clearly which of the 3 scales to use (fraction, percent, or ORP) is optional as they all reflect the same thing.

[0015] A table was developed that contained the ORP value for each of the 10,000 Bin Codes (ORP table; Figure 14). Table 2 below shows the ORP values for the first and last 300 bin codes. Clearly the higher the ORP value the greater the likelihood of the Bin occurring in an epoch that would manually be scored as awake, and vice versa. Further, the ORP (or probability) value should reflect the depth of sleep. For example, an ORP value of 1.25 (probability of falling in an epoch scored awake =50%) means that a Bin with such a spectral pattern occurs equally in epochs scored as awake or asleep. Such Bin Code must, therefore, reflect very light sleep because sleep depth is typically a gradual process. It is true that in some 30-second epochs deep sleep can suddenly change to awake. However, these instances are quite infrequent when viewed within the context of several hundred thousand Bins in representative files. Conversely, an ORP that is close to zero indicates that such a spectral pattern is only seen in sleep and, hence, occurs only in very stable sleep, which is typically deep sleep.

[0016] Once the Bin Codes are assigned as per step 2, the software converts the Codes into probabilities by use of the Probability Look-up table. An example of such conversion for bin code 0126 is shown in Table 2. It is theoretically possible to express the results of Table 2 as a mathematical formula through complex regression analysis. In such case, the formula can be used to convert the Code into probability instead of the look-up table. We have found that such an exercise of attempting to fit the data of Table 2 by a formula is not warranted in view of the ease and speed of utilizing a look-up table. However, use of formulae or other decoding instruments to convert the Codes into probabilities is covered by the present invention.

[0017] The ORP table given here is unique to the reference files we used, the scorers who scored these files, the frequency bands and frequency domain analysis used, bin width (3-seconds), the ranking method used (Table 1), and the output form (ORP). We have obtained excellent results using this combination of techniques and look-up tables (Kuna ST, Benca R, Kushida CA, Walsh J, Younes M, Staley B, Hanlon A, Pack AI, Pien GW, Malhotra A. Agreement in Computer-Assisted Manual Scoring of Polysomnograms Across Sleep Centers. SLEEP 36:583-589, 2013). However, and as mentioned earlier, a software manufacturer may choose to apply the general method described here using other reference files, other scorers, other methods of frequency domain analysis, other frequency bands, another ranking system or output form (e.g. % awake) and generate their own look-up tables. In such cases the Ranking and Probability tables should be constructed from reference files that were analyzed using the same methods (i.e. frequency ranges, bin width, frequency domain analysis... etc). Such different applications of the general method fall within the scope of this invention.

TABLE 2
Representative ORP Values For the First and Last 300 Bin Codes

Bin Code	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19
0000	0.92	1.80	1.88	1.95	2.05	2.13	2.27	2.39	2.50	2.50	1.33	1.72	2.02	2.14	1.97	2.08	2.26	2.42	2.43	2.50
0020	1.81	2.21	2.28	2.24	2.32	2.24	2.30	2.39	2.46	2.50	2.30	2.30	2.31	2.38	2.37	2.39	2.34	2.41	2.45	2.50
0040	1.98	2.38	2.40	2.47	2.44	2.42	2.45	2.41	2.46	2.49	2.50	2.39	2.46	2.46	2.48	2.50	2.49	2.45	2.49	2.50
0060	2.30	2.27	2.50	2.49	2.49	2.47	2.49	2.49	2.48	2.49	2.30	2.37	2.41	2.50	2.50	2.47	2.49	2.48	2.49	2.50
0080	2.30	2.50	2.43	2.44	2.50	2.49	2.49	2.50	2.50	2.50	2.30	2.30	2.30	2.50	2.50	2.50	2.50	2.50	2.50	2.50
0100	0.26	0.52	0.78	0.78	1.03	1.38	1.84	1.93	2.20	2.50	0.48	0.80	0.78	0.95	0.97	1.15	1.63	1.97	2.32	2.50
0120	1.10	1.11	1.34	1.51	1.68	1.52	1.85	2.13	2.32	2.50	1.50	1.60	1.71	1.85	2.06	1.94	2.18	2.21	2.39	2.41
0140	1.60	1.60	1.90	2.24	2.28	2.27	2.25	2.24	2.30	2.47	2.00	2.00	2.16	2.40	2.29	2.48	2.34	2.45	2.42	2.50
0160	2.20	2.20	2.32	2.39	2.42	2.43	2.33	2.44	2.48	2.50	2.30	2.30	2.50	2.47	2.44	2.43	2.45	2.49	2.47	2.49
0180	2.50	2.50	2.50	2.50	2.47	2.50	2.49	2.49	2.48	2.50	2.50	2.50	2.50	2.50	2.50	2.50	2.50	2.48	2.50	2.50
0200	0.19	0.28	0.35	0.66	0.63	0.46	0.80	1.80	2.00	2.20	0.24	0.28	0.37	0.82	0.48	0.58	0.80	1.80	2.35	2.50
0220	0.50	0.56	0.81	1.00	1.15	1.30	1.45	1.60	2.15	2.30	0.80	0.80	0.80	1.04	1.28	1.52	1.76	1.96	2.03	2.50
0240	1.28	1.40	1.52	1.64	2.04	1.97	1.81	2.00	2.31	2.50	1.55	1.65	1.75	1.85	2.19	2.28	2.11	2.21	2.30	2.50
0260	1.82	1.90	1.98	2.08	2.34	2.29	2.23	2.40	2.47	2.47	2.09	2.15	2.21	2.20	2.43	2.39	2.45	2.37	2.48	2.48
0280	2.36	2.40	2.44	2.37	2.44	2.46	2.46	2.44	2.47	2.50	2.50	2.50	2.50	2.50	2.50	2.50	2.50	2.47	2.49	2.50
0300	3.16	3.30	0.15	0.31	0.16	0.80	1.00	1.19	1.38	1.57	0.14	0.25	0.32	0.18	0.24	0.36	1.17	1.35	1.52	1.69

Example: ORP for Bin Code 0126 = 1.85

9700	0.00	0.00	0.00	-0.14	0.02	0.18	0.34	0.51	0.67	0.83	0.00	0.00	0.00	0.00	0.08	0.24	0.41	0.57	0.74	0.91
9720	0.00	0.00	0.00	0.00	0.00	0.30	0.47	0.64	0.81	0.99	0.00	0.00	0.00	0.10	0.00	0.35	0.54	0.71	2.22	2.50
9740	0.00	0.00	0.00	0.00	0.00	0.16	0.28	0.78	2.13	2.50	0.00	0.00	0.00	0.00	0.04	0.05	0.14	0.85	1.04	2.47
9760	0.00	0.00	0.00	0.00	0.12	0.04	0.16	0.50	1.11	2.44	0.00	0.00	0.00	0.10	0.15	0.00	0.17	0.47	1.18	2.40
9780	0.80	0.00	0.00	0.00	0.06	0.04	0.19	0.40	1.19	2.44	0.00	0.00	0.13	0.00	0.53	0.13	0.28	1.13	1.49	2.44
9800	0.00	0.13	0.00	0.00	0.00	0.00	0.11	0.28	0.44	0.60	0.00	0.00	0.00	0.12	0.00	0.00	0.18	0.34	0.51	0.68
9820	0.00	0.00	0.04	0.00	0.00	0.21	0.17	0.41	0.58	0.75	0.00	0.00	0.00	0.02	0.07	0.04	0.05	0.48	0.66	2.35
9840	0.00	0.00	0.00	0.00	0.00	0.21	0.17	0.55	0.73	0.91	0.00	0.00	0.00	0.02	0.07	0.04	0.05	0.62	0.80	2.35
9860	0.00	0.00	0.00	0.00	0.03	0.04	0.10	0.11	0.65	2.35	0.00	0.00	0.00	0.02	0.01	0.08	0.11	0.14	0.58	2.34
9880	0.00	0.00	0.00	0.00	0.05	0.04	0.04	0.10	0.46	2.28	0.00	0.00	0.00	0.00	0.03	0.03	0.09	0.15	0.83	2.38
9900	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.05	0.21	0.37	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.11	0.28	0.45
9920	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.18	0.35	0.52	0.00	0.00	0.00	0.02	0.04	0.00	0.05	0.19	0.43	0.60
9940	0.00	0.00	0.01	0.01	0.03	0.02	0.03	0.26	0.50	0.68	0.00	0.00	0.00	0.00	0.00	0.04	0.06	0.16	0.64	2.26
9960	0.00	0.00	0.00	0.00	0.00	0.02	0.03	0.13	0.50	2.23	0.00	0.00	0.00	0.00	0.01	0.01	0.03	0.07	0.29	1.98
9980	0.00	0.00	0.00	0.01	0.01	0.01	0.03	0.07	0.18	1.94	0.00	0.00	0.00	0.02	0.00	0.03	0.04	0.12	0.17	2.35

[0018] This Patent application is about generating a probability estimate of an electroencephalogram interval (Bin) falling in an epoch that would be scored independently, by expert scorers or systems, as awake. Clearly, rather than estimating the probability of being awake, one may choose to estimate the Probability of the epoch being scored as asleep. (this would simply be (2.5 - ORP), or (100 - Probability%)).

[0019] The probability value generated by the current invention can be used in many different ways:

A) The average Probability Estimate (e.g. ORP) for the entire file can be displayed in the scoring report, and used as a measure of overall sleep quality.

B) The average Probability Estimate for periods scored as specific sleep stages (manually or automatically) can also be displayed in the scoring report. It is generally recognized that a given sleep stage is not homogeneous. Within each sleep stage there is a spectrum of EEG patterns with some being closer to awake patterns while others are closer to deep sleep. Stage N2 in one patient may, for example, have a predominance of deeper sleep Bins or epochs while in another patient lighter sleep epochs predominate. These differences are not currently captured by conventional scoring, which classifies sleep into 4 stages only. By reporting the quality of sleep within each of the four stages, it may be possible to explain why some patients symptoms (fatigue, sleepiness) are not in keeping with the results of conventional scoring. We have found that the P_w in stage N1 sleep ranges from 24% to 72% (ORP 0.6 to 1.8) among different subjects, for N2 the range was 7% to 55% (ORP 0.17 to 1.4), and for N3 it was 2% to 28% (ORP 0.04 to 0.7). It is thus clear that within the same stage defined by visual criteria, there is a wide range of ORP values that reflect different levels of sleep quality.

C) Likewise, within what is conventionally scored as awake time, the average P_w can range from 62% to 96% (ORP 1.55 to 2.40), thereby reflecting different degrees of vigilance during what is conventionally called awake. It can be easily envisioned that a limited EEG monitoring device, attached to the forehead for example, can be equipped with the current software and be used to monitor P_w or ORP in real time in subjects engaged in critical activities. Such a system can also sound an alarm or notify monitoring stations when P_w or ORP falls below a specified level (e.g. 2.2).

D) The probability estimates can be averaged over periods on and off therapy and the averages reported to show the effect of therapy on sleep quality.

E) The probability estimate can be used on its own to score sleep if all that is required is to determine whether the epoch(s) being scored are simply awake or asleep. For example, the average probability estimate for all Bins within a 30-second interval can be calculated. I have found that by using the simple rule of scoring an epoch awake when average ORP is > 1.6 (probability $> 64\%$), and vice versa, the scoring is accurate in 95% of epochs. This is acceptable accuracy for that purpose.

F) Alternatively, the distribution of probability estimates within an epoch (e.g. 30 seconds) can be utilized to improve accuracy, particularly in epochs in which the average ORP is equivocal. For example, a 30-second epoch that contains four 3-second Bins with an ORP < 1.0 and six 3-second Bins with an ORP > 2.0 might have an ambivalent average ORP of 1.4. However, it would be scored as awake since this was clearly an epoch split between a longer period with a dominant awake pattern (ORP > 2.0) and a shorter period with sleep pattern. Several other algorithms that examine the pattern of ORP values within a 30-second epoch can clearly be utilized to improve the accuracy of distinguishing between awake and asleep in an epoch. While we prefer that the software make a decision in every 30-sec epoch, one option is to not score epochs where it is difficult to decide. For example, if all ORP values within an epoch are in the mid-range (1.2 to 1.8) and the average is also equivocal (e.g. 1.2 to 1.6), one may elect to identify the epoch as un-scorable by the current system. This would affect only a small minority of epochs.

G) The current invention can be used as an accessory to the current manual scoring systems. Thus, the file would be run first with the software of the current invention to automatically classify epochs as awake or asleep, to be followed by manual scoring of the different sleep stages.

H) The probability estimate can be incorporated within software that performs comprehensive sleep staging. Here, after the overall status of an epoch (sleep vs. awake), epochs scored as sleep are further identified as one of the standard four stages (Rem, N1, N2, N3) using additional algorithms to detect features used for classifying sleep stages (e.g. eye movements, spindles, K complexes, chin

EMG). Such steps that aim to further identify the different stages of sleep are not part of this invention.

I) The current invention can be incorporated in portable devices that measure the EEG. The results can be displayed or transmitted (wirelessly or through cable) in real time. In this way the results can help evaluate the state of vigilance of the subject being monitored.

[0020] Accordingly, in one aspect of the present invention, there is provided a method for generating a Probability index (Index) that reflects where an electroencephalogram (EEG) pattern lies within the spectrum of wakefulness to deep sleep, which employs a computer/microprocessor that performs frequency domain analysis of one or more discrete sections (Bins) of the EEG to determine the EEG power at specified frequencies, optionally calculates the total power over specified frequency ranges (Ranges), assigns a rank to the power at each frequency, or frequency Range, assigns a code to the Bin that reflects the ranking of the different frequencies or frequency ranges (Bin Code), and determines an index that reflects where said EEG pattern within said Bin(s) lies within the spectrum of wakefulness to deep sleep by use of a Reference Source, such as a look-up table or other suitable decoding instrument, where such Reference Source is obtained by calculating the probability of Bins with different Codes occurring in epochs scored as awake or asleep in reference files scored by one or more expert technologists or by an automatic scoring software.

[0021] In that method, material of calculating power, frequency domain analysis is used to calculate signal amplitude, or other measure of signal strength, in the specified frequency ranges and where the Ranking method and the Reference Source are based on use of the method of calculating signal strength.

[0022] In another aspect of the present invention, there is provided software for estimating the Probability that the electroencephalogram (EEG) pattern reflects a sleeping or awake state, said software executing the following functions performing spectral analysis of one or more discrete sections (Bins) of the EEG to determine the EEG power at different frequencies, optionally calculating the total power over specified frequency ranges (Ranges), assigning a rank to the power at each frequency, or frequency Range, assigning a code to the Bin that reflects the ranking of the different frequencies or frequency ranges (Bin Code), and determining the probability of the EEG pattern within said Bin(s) of reflecting an awake or sleep state by use of a reference source, such as a look-up table or other suitable decoding instrument, where such reference source is obtained by calculating the probability of Bins of different Codes occurring in

epochs scored as awake or asleep in reference files scored by one or more expert technologists or by a properly validated scoring software.

... claim 9.

[0023] In a further aspect of the present invention, there is provided a device for carrying out the method and utilizing the software.

BRIEF DESCRIPTION OF DRAWINGS

[0024] Figure 1 is a block diagram of the major components of software and the data flow in the analysis of processing records to determine ORP;

[0025] Figure 2 is a block diagram showing various pre-processing options;

[0026] Figure 3 is a block diagram of the algorithm for removing the R-wave artifact;

[0027] Figure 4 is a block diagram showing the steps used for Frequency domain analysis;

[0028] Figure 5 is a flow chart of the step of "Calculate Summary Powers";

[0029] Figure 6 is a block diagram showing the assign Bin Code;

[0030] Figure 7 is a flow chart showing the step of assigning the ORP values

[0031] Figure 8 shows the typical results of ORP values over several hours of recording for two patients with the results of conventional sleep scoring into five stages (awake, N1, N2, N3, REM);

[0032] Figure 9 is a flow chart showing the processing of streaming data for ORP determination;

[0033] Figure 10 is a block diagram of the components of a mobile device that implements the present invention;

[0034] Figure 11 shows details of the Front End Analog Circuitry of the instrument of Figure 10;

[0035] Figure 12 shows details of the micro-controller and associated circuitry of the instrument of Figure 10;

[0036] Figure 13 shows details of the power supply and associated circuitry for the instrument of Figure 10; and

[0037] Figure 14 is the ORP Table.

DESCRIPTION OF PREFERRED EMBODIMENTS

[0038] 1) *Analysis of pre-existing records:*

[0039] This form of implementation is particularly suitable when this invention is used on pre-existing files or when the generation of the Probability Value is a preliminary step to be followed by more detailed analysis of the EEG that require examination of large sections of the file (e.g. as an aid to scoring sleep stages). This form of implementation is preferably done on standard computers.

[0040] The software of the preferred embodiment was developed in C# (C sharp) on a standard desktop computer with the following specifications:

- 1) Processor: 3.4GHz
- 2) RAM: 4GB
- 3) Operating System: Windows XP, 32-bit
- 4) Development Environment: Visual Studio 2008
- 5) Hard Drive Size: 1.00 TB

[0041] Figure 1 is a block diagram of the major components of the software and the data flow. The file is loaded in memory (1). The next step involves optional pre-processing (2) (See Figure 2). The file is then split into 3-sec bins (3) with a total number, M, corresponding to 1/3 file length in seconds. Beginning with the first bin (4) frequency domain analysis is performed (5) (see Figure 4) followed by calculation of total power in different frequency ranges (6) (see Figure 5). From this, bin code is assigned (7) by reference to lookup table 1, which is stored in memory. This is followed by determination of ORP for the 3-sec bin (8) (see Figure 7), by reference to the stored ORP lookup table. The ORP value is stored (9). Bin number is increased by one and the process repeats until the end of the file.

[0042] Figure 2 shows the various pre-processing options (2). One or more of these is executed depending on the pre-existing properties of the file. These properties are inputted into the computer along with the file.

[0043] The band-pass filter (0.3-35.0 Hz) option (10) is applied if the file in memory is not pre-filtered. This is to comply with recommended standards for processing of the EEG. The current software operates on the assumption that the sampling frequency in the file is 120 Hz. If the sampling frequency is <120 Hz, the file is rejected. If >120 Hz, the data is re-sampled at 120 Hz (11) using the "Nearest Neighbor Approximation" (the value of the data point nearest the time required for 120Hz is used). This is followed by a 0.05 high-pass filter (12). Finally, if the R wave artifact of the electrocardiogram (EKG) has not been filtered out in the stored file, an R-

wave artifact removal algorithm is applied to the EEG signal (13). This requires the presence of an EKG channel in the file.

[0044] Details of this R-wave artifact removal algorithm are shown in Figure 3. Briefly, the times of R wave peaks (P_i) are located for each cardiac beat in the file (14). Any of a number of standard R wave detection algorithms can be used. For this embodiment, a 5-point derivative of the EKG signal is obtained and then squared. An 11-point integral is performed on the squared derivative (IFRDi). A 10-sec integral of the IFRD is obtained (IFRDi_{0s}) and the difference between IFRDi and IFRDi_{0s} is calculated. Peak R wave is identified as the highest point in a transient in which IFRDi > IFRDi_{0s} for > 100 ms. Subsequent steps are performed on the EEG channel from which the R wave artifact is to be removed. EEG data in the interval $P_i \pm 35$ points (≈ 0.6 sec) of each R wave are stored (15). These stored values are then broken into consecutive blocks, each containing 100 beats (16). The average of the 100 sets of 71 points is then obtained for each block and this 71-point average replaces all 100 sets in the block (17). This process is performed for each block in the file. Finally, the stored averages are subtracted from the original EEG data (18).

[0045] Figure 4 shows the steps used for Frequency domain analysis (5). Our software, which uses a variation of the Fourier transform, calculates the power $X[A]$ at frequency k as:

$$\left[A[k] = \sum_{n=0}^{n-1} x_n \cdot \cos\left(\frac{2\pi}{N}(k+1)(n+1)\right) \right]$$

$$\left[B[k] = \sum_{n=0}^{n-1} x_n \cdot \sin\left(\frac{2\pi}{N}(k+1)(n+1)\right) \right]$$

$$X[k] = ((A[k])^2 + (B[k])^2) / N^2$$

For integer values of k , $k = \left[1, \frac{N}{2}\right]$

$$k = \left[1, \frac{N}{2} - 1\right]$$

Where;

f_s = Sample Rate of the EEG window = 120Hz

N = Length of input EEG window, in samples = $3f_s = 360$

n = Current sample index in EEG window

x_n = Value of the EEG signal for sample n

k = Index of the frequency we are examining. The actual frequency is: $\hat{f}_k = \frac{(k+1)}{3} H_\Sigma$

$$f_k = \frac{(k+1)}{3} Hz$$

$X[k]$ = The power at a frequency index of k

C = Scaling coefficient, equal to $\frac{1}{N} = \frac{1}{360}$

[0046] To save computation time, since the following two terms

$$\cos\left(\frac{2\pi}{N}(k+1)(n+1)\right) \quad \sin\left(\frac{2\pi}{N}(k+1)(n+1)\right)$$

are independent of x_n , and as shown in the top of figure 4 (19), they are calculated ahead of time and stored in memory.

[0047] Figure 5 is a flow chart describing the step "Calculate Summary Powers" (6). In this step the sum of powers in specified frequency ranges is calculate in each 3-sec bin. The frequency ranges used in this embodiment were (6):

- 0.3-2.3 Hz ($k=0-6$): corresponding to conventional delta range (20);
- 2.7-6.3 Hz ($k=7-18$): corresponding to conventional delta range, excluding frequencies 6.7 and 7.0 Hz (21);
- 7.3-12.0 Hz ($k=21-35$): corresponding to conventional alpha range (22),
- 12.3-14.0 Hz ($k=36-41$): corresponding to conventional sigma range (23),
- 14.3-20.0 ($k=42-59$): corresponding to conventional Betal range (24), and
- 20.3-35.0 ($k=60-104$): corresponding to conventional Beta2 range (25).

[0048] For the sake of ORP determination, alpha and sigma powers were combined (alpha/sigma power (26)) and beta 1 and beta 2 powers were also combined (beta power (27)), resulting in 4 frequency ranges.

[0049] Figure 6 shows the approach used to assign Bin Codes (7). The algorithm checks the delta power in the 3-sec bin against the thresholds for the 10 ranks in the delta column of the stored Table 1 and assigns the appropriate rank to the delta power. The same process is repeated for theta, alpha/sigma and beta power, assigning a rank to each. Finally a 4-digit number is

generated having the delta rank, followed by the theta rank, followed by the alpha/sigma rank and finally the beta rank. The process is repeated for each 3-sec bin.

[0050] Figure 7 shows the step of assigning the ORP value (8). This simply consists of checking the ORP code in the ORP table and obtaining the ORP value associated with the code.

[0051] Figure 8 shows results of ORP values (generated according to the preferred embodiment) over several hours of recording in two patients along with the results of conventional sleep scoring into five stages (awake, N1, N2, N3, REM). By conventional criteria, the main difference between the two patients was a somewhat greater awake time in patient 1 (Table 3 below). However, by looking at the ORP values in Figure 8, it is clear that even when patient 1 was technically staged asleep, the ORP was highly unstable, reflecting extensive and frequent intrusion of awake features within the EEG, and that the average ORP (white line within the ORP panel) was substantially higher in patient 1 than in patient 2 for all sleep stages (see also Table 3). Thus, not only was there more awake time in patient 1 but, when he slept, his sleep quality was quite poor. Figure 8 also shows that during awake periods in both patients ORP was not fixed at 2.5 (the highest level) but there were frequent decreases in ORP, reflecting intrusion of sleep features during awake time. Thus, the awake state is not a constant but incorporates different levels of vigilance that can be reflected by the ORP value.

TABLE 3

	Patient 1		Patient 2	
	Time (min)	ORP	Time (min)	ORP
Awake	155	2.28	85	2.28
N1	59	1.84	16	0.86
N2	147	1.39	195	0.42
N3	24	0.72	55	0.18
REM	52	1.59	29	1.00
Total Sleep	282	1.46	294	0.45
Total Recording Time	436	1.75	378	0.86

[0052] 2) Generation of the Probability Index from Streaming Data (i.e. in real time):

[0053] The same procedure, with minor modifications, is used to generate the probability index on a continuous basis by analyzing short segments of recording and outputting the result as the data flows in. It is particularly suited for applications that require rapid feedback about the patient's sleep state or state of vigilance. It can also be utilized as a preliminary step in other software that performs simultaneous scoring of sleep stages concurrently with data

acquisition. This application can be implemented on standard desktop computers, laptops or other mobile computing devices depending on the clinical indication. With all such devices the EEG output of the data acquisition system is channeled to the computer via a USB port or other suitable means. The data is then streamed into memory using existing or custom software.

[0054] Figure 9 is a flow chart showing the processing of streaming data. Here, each specified interval (bin; for example 3 seconds) is treated as a separate file. When data for such interval has been received, the software goes through the same process described in Figures 1 to 7, including preprocessing (2, Figure 2), frequency domain analysis (5, Figure 4), Calculate Summary Powers (6, figure 5), Determine Bin Code (7, Figure 6), and finally Determine ORP value (8, Figure 7). A single ORP value is generated and displayed. The process repeats until the end of the study.

[0055] Figure 10 is a block diagram of the components of a mobile device that implements the present invention. A data acquisition chip (Texas Instruments ADS 1299; 28) is used for collecting up to eight channels, any of which can be an EEG channel. The output is conveyed, via an SPI communication Bus, to a micro-controller (29) that incorporates Atmel ATmega256RFR2 (U1A and U2B) microcontroller (30) and a radio receiver/transmitter (BALUN; 31). The system is powered by a Lithium ion battery (32) with associated battery and power management circuitry (33).

[0056] Figure 11 shows details of the Front End Analog Circuitry (28) associated with Texas Instruments ADS 1299 chip comprising:

- Analog front end for biopotential measurements
- Low noise delta sigma analog to digital converter
- 8 channels, simultaneous sampling
- 24-Bit analog precision
- Sample rates from 250SPS (samples per second) to 16kSPS

[0057] Figure 12 shows details of the micro-controller (29) and associated circuitry comprising:

[0058] Atmel ATmega256RFR2 (U1 A and U2B)(30) with:

- 8-bit Microcontroller at 16MHz
- 256KB Flash Memory
- 32KB Program RAM (random access memory)
- Fully integrated RF Transceiver for the 2.4GHz ISM Band (industrial, scientific and medical)

- RF Data rates from 250 kb/s up to 2 Mb/s
- ZigBee and IEEE 802.15.4 RF compliant

[0059] Würth Electronics - 732-2230-1 -ND (BALUN) (31)

- BALUN - Balanced to unbalanced converter
- blocks common mode waves and allows only differential mode waves to the antenna.

[0060] Microchip - MCP102T (32)

- Micropower voltage supervisor
- Prevents unnecessary microcontroller resets due to brown out conditions

[0061] Figure 13 shows details of the power supply (33) and associated circuitry comprising:

[0062] Lithium ion battery (32)

[0063] Microchip - MCP73831T (34)

- Li-Polymer Charge Management Controller
- Employs battery charging algorithms and measurement logic

[0064] Maxim Integrated - MAX1704 (35)

- Battery fuel gauge and low battery alert
- Provides battery data to the microcontroller
- Alerts the microcontroller in case of low battery percentage

[0065] Texas Instruments - TPS27082L (36)

- PFET Load Switch
- Provides Fast Transient Isolation and Hysteretic control

[0066] Linear - LT3971-3.3 (37)

- 38V, 1.2A, 2MHz - Step Down Regulator
- Switching power supply for the system
- Converts battery power to 3.3V for microcontroller and analog front end power supply

[0067] FTDI - FT230XQ (38)

- USB to UART (serial) converter
- Allows for data transfer between computer and onboard micro-controller.

[0068] SYSTEM OVERVIEW

- Power is applied to system
- Microcontroller enters bootloader which loads the firmware
- Firmware initializes all system settings to allow for operation between the ADS 1299 and itself
- Firmware initializes radio connection between receiver and itself
- START command issued to ADS 1299 to start sampling 2 to 8 channels
- Analog signal is converted to digital via the ADS 1299
- Digital data is sent over a serial protocol interface (SPI) to the microcontroller
- This process repeats until a STOP command is issued
- Appropriate signal conditioning and data analysis: As per steps 2, 5, 6, 7, and 8 (figures 2, 4, 5, 6, and 7)
- Algorithm output is sent over a wireless radio link

SUMMARY OF DISCLOSURE

[0069] In summary of this disclosure, the present invention provides a method of generating a probability index that reflects where an electroencephalogram (EEG) pattern lies within the spectrum of wakefulness to deep sleep, which employs a computer/microprocessor that performs the steps of method. Modifications are possible within the scope of the invention.

CLAIMS

1. A method for generating a Probability index (Index) that reflects where an electroencephalogram (EEG) pattern lies within the spectrum of wakefulness to deep sleep, which employs a computer/microprocessor that:
 - performs frequency domain analysis of one or more discrete sections (Bins) of the EEG to determine the EEG power at specified frequencies,
 - optionally calculates the total power over specified frequency ranges (Ranges),
 - assigns a rank to the power at each frequency, or frequency Range,
 - assigns a code to the Bin that reflects the ranking of the different frequencies or frequency ranges (Bin Code), and
 - determines an index that reflects where said EEG pattern within said Bin(s) lies within the spectrum of wakefulness to deep sleep by use of a Reference Source, such as a look-up table or other suitable decoding instrument, where such Reference Source is obtained by calculating the probability of Bins with different Codes occurring in epochs scored as awake or asleep in reference files scored by one or more expert technologists or by an automatic scoring software.
2. The method of claim 1 wherein, instead of calculating power, frequency domain analysis is used to calculate signal amplitude, or other measure of signal strength, in the specified frequency ranges, and where the Ranking method and the Reference Source are based on use of said method of calculating signal strength.
3. The method of claim 1 wherein Index values of more than one Bin are averaged over specified intervals and the average results are utilized to determine the Sleep/Wake status of said Intervals and/or are reported as such in the scoring Reports.
4. The Method of claim 3 wherein said Intervals are specified time intervals (e.g. 30 seconds, or time on/off therapy), specified sleep stages or the whole file.
5. The methods of any one of claims 1 to 4 when used as a component of other scoring systems that perform other scoring functions, such as staging of sleep, detection of respiratory events, arousals, cardiac arrhythmias, or motor events during sleep.
6. The methods of any one of claims 1 to 5 when incorporated in portable devices that measure EEG activity.
7. The methods of any one of claims 1 to 6 wherein the Index values are outputted after the entire file is analyzed.

8. The methods of any one of claims 1 to 6 wherein the Index values are outputted in real time as streaming data are loaded in computer memory.
9. Software for estimating the Probability that the electroencephalogram (EEG) pattern reflects a sleeping or awake state, said software executing the following functions:
- performing spectral analysis of one or more discrete sections (Bins) of the EEG to determine the EEG power at different frequencies,
 - optionally calculating the total power over specified frequency ranges (Ranges),
 - assigning a rank to the power at each frequency, or frequency Range,
 - assigning a code to the Bin that reflects the ranking of the different frequencies or frequency ranges (Bin Code), and
 - determining the probability of the EEG pattern within said Bin(s) of reflecting an awake or sleep state by use of a reference source, such as a look-up table or other suitable decoding instrument, where such reference source is obtained by calculating the probability of Bins of different Codes occurring in epochs scored as awake or asleep in reference files scored by one or more expert technologists or by a properly validated scoring software.
10. The software of claim 9 wherein said Probability values are averaged over specified intervals and the average results are utilized to determine the Sleep/AVake status of said Intervals and/or are reported as such in the scoring Reports.
11. The software of claim 10 wherein said Intervals are specified time intervals (e.g. 30 seconds, or time on/off therapy), specified sleep stages or the whole file.
12. The software of any one of claims 9 to 11 when used as a component of other scoring systems that perform other scoring functions, such as staging of sleep, detection of respiratory events, arousals, cardiac arrhythmias, or motor events during sleep.

1 / 55

Fig. 1



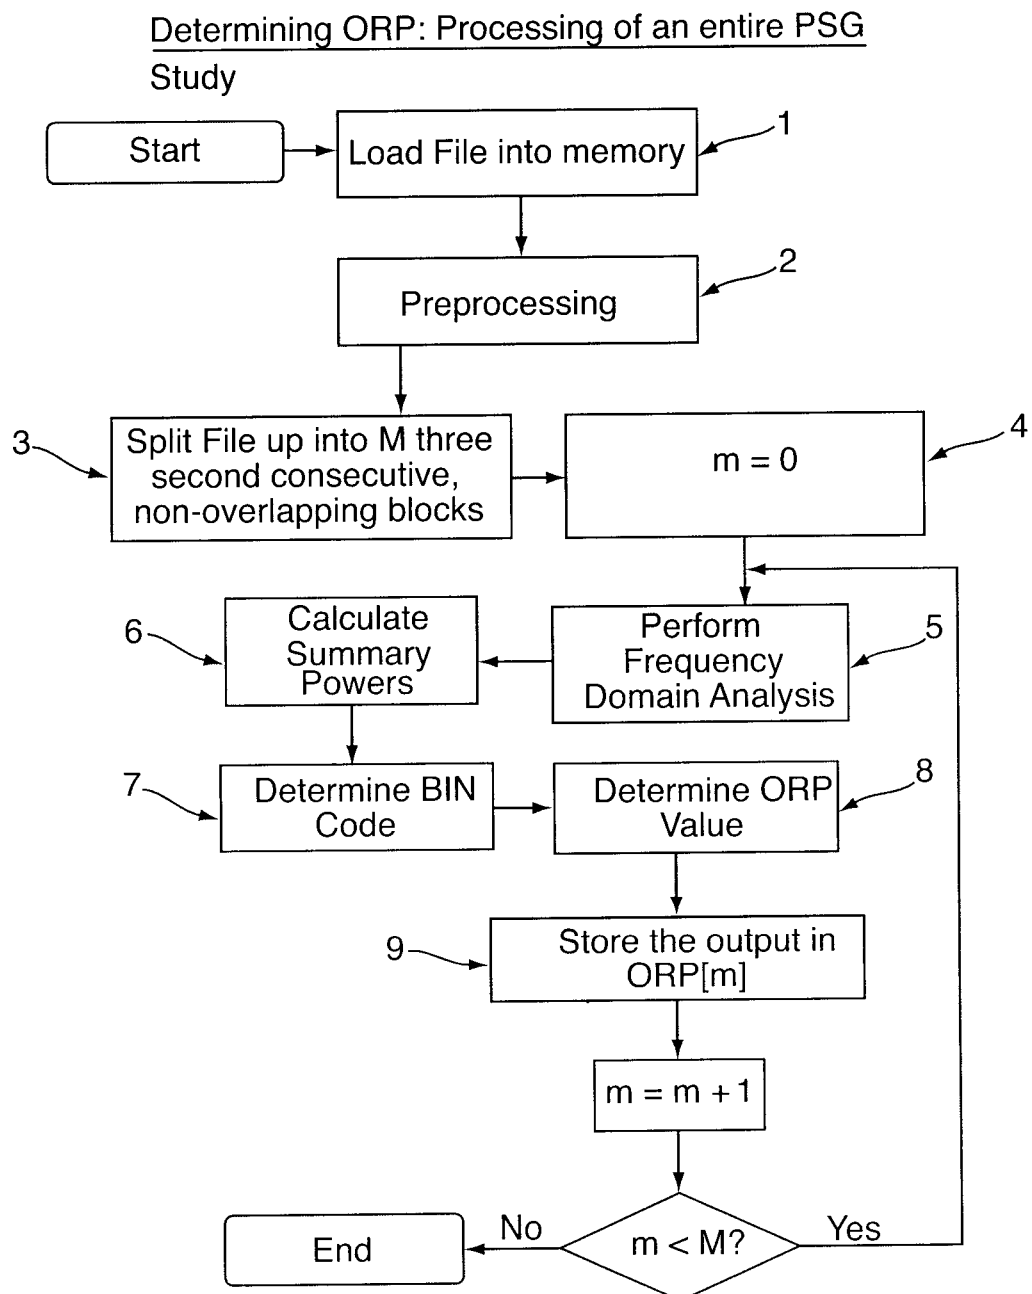


Fig. 2

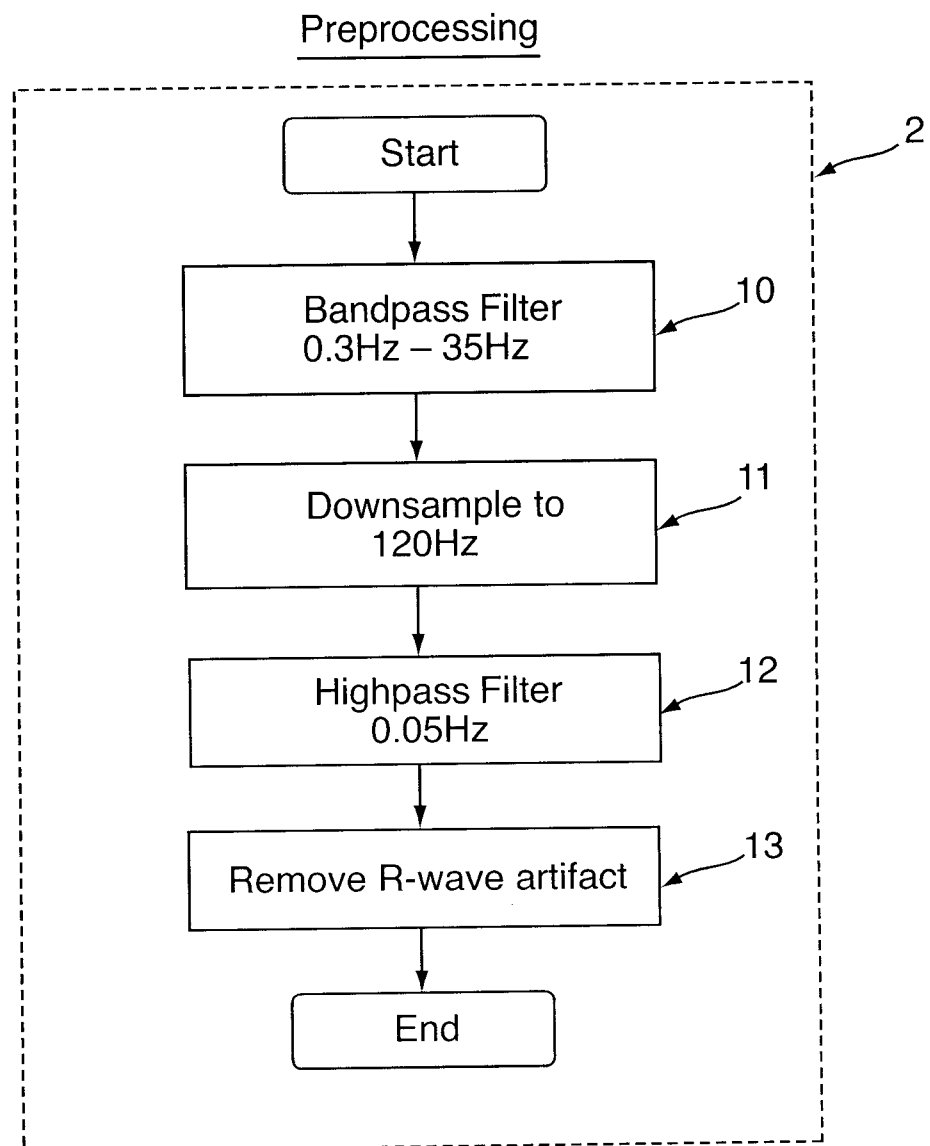


3 / 55

Fig. 3

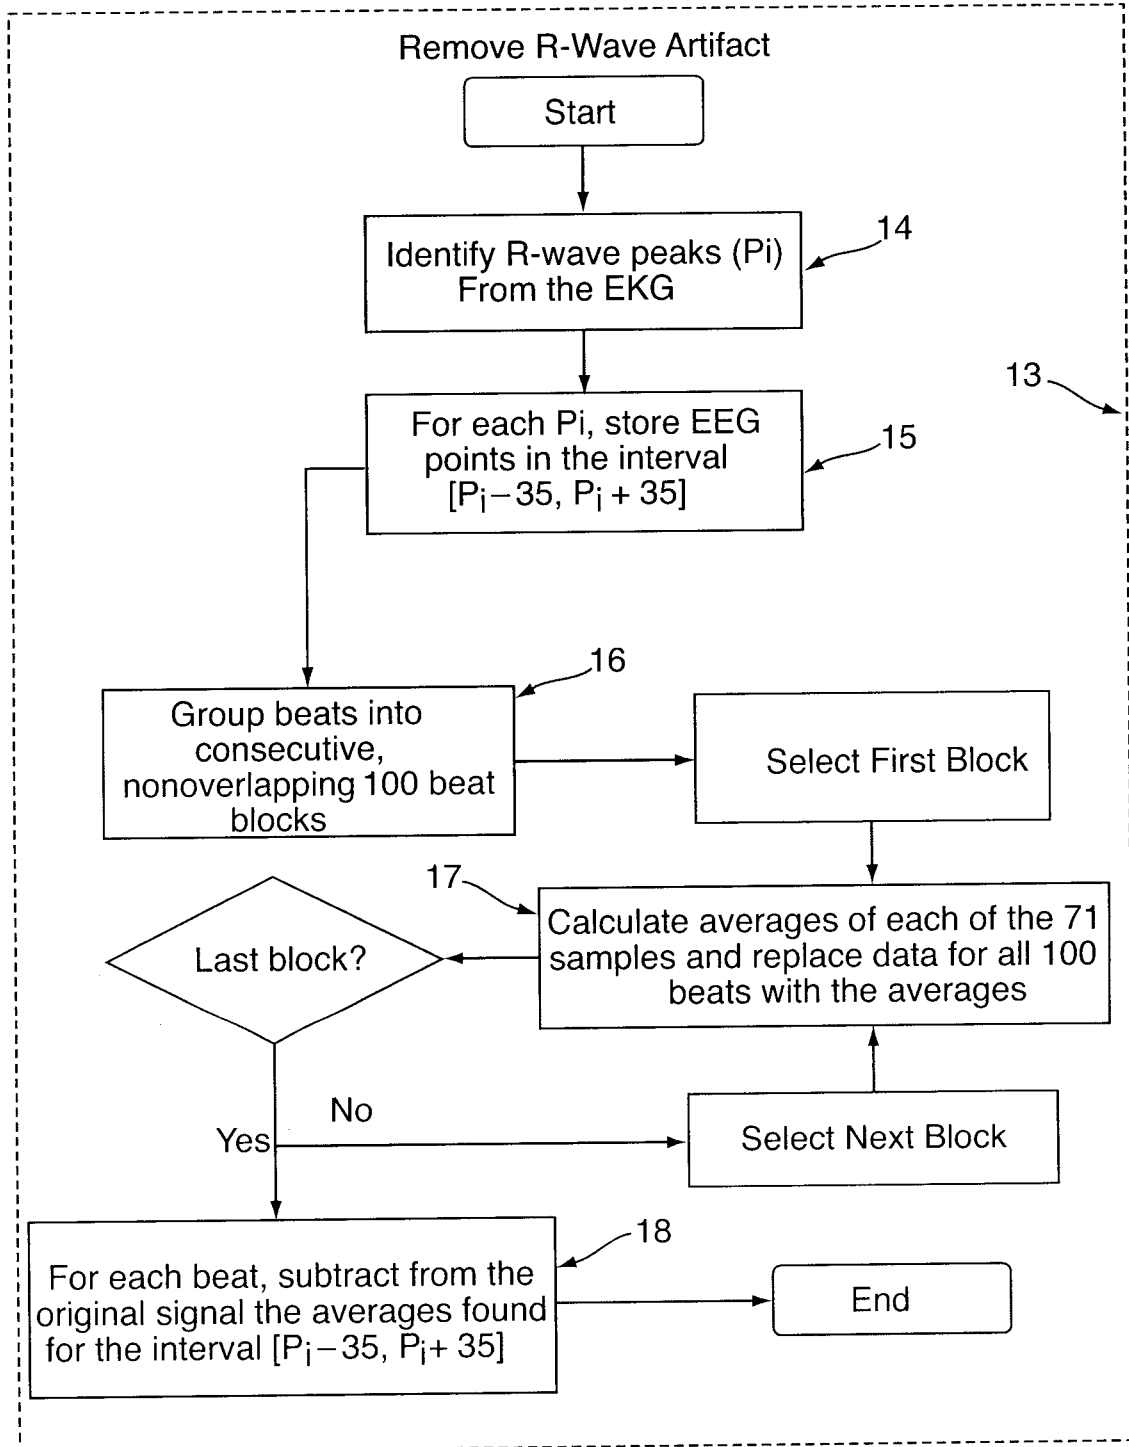


4 / 55

Fig. 4

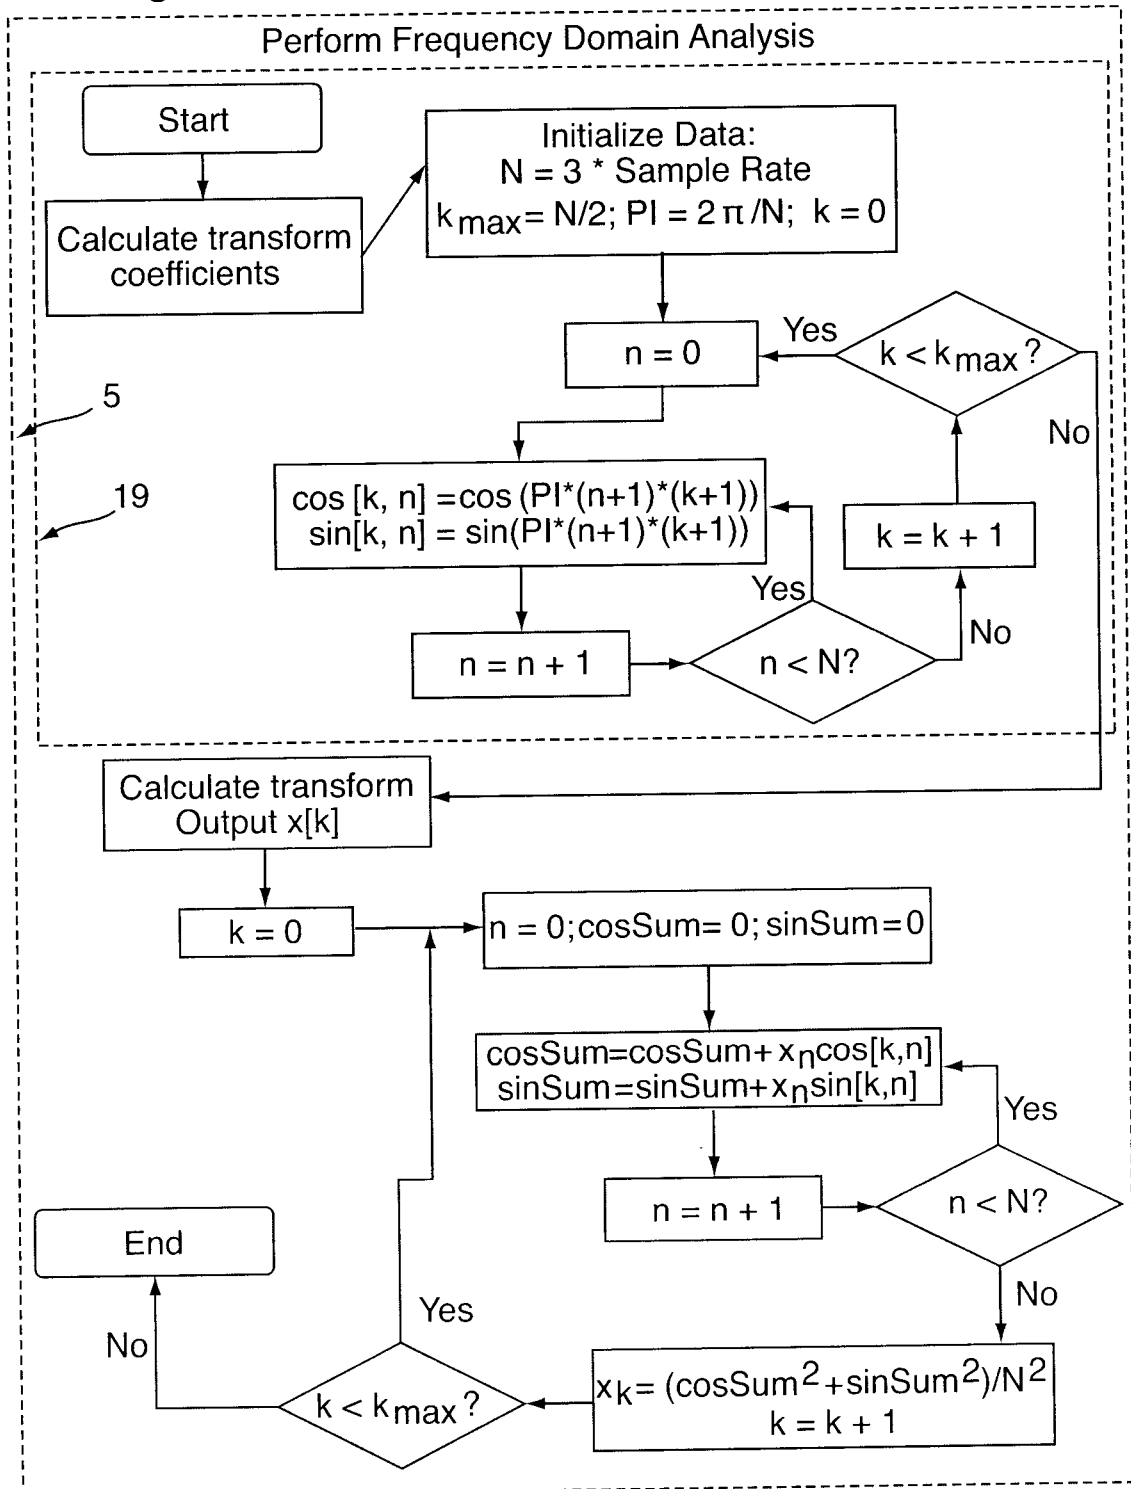


5 / 55

Fig. 5

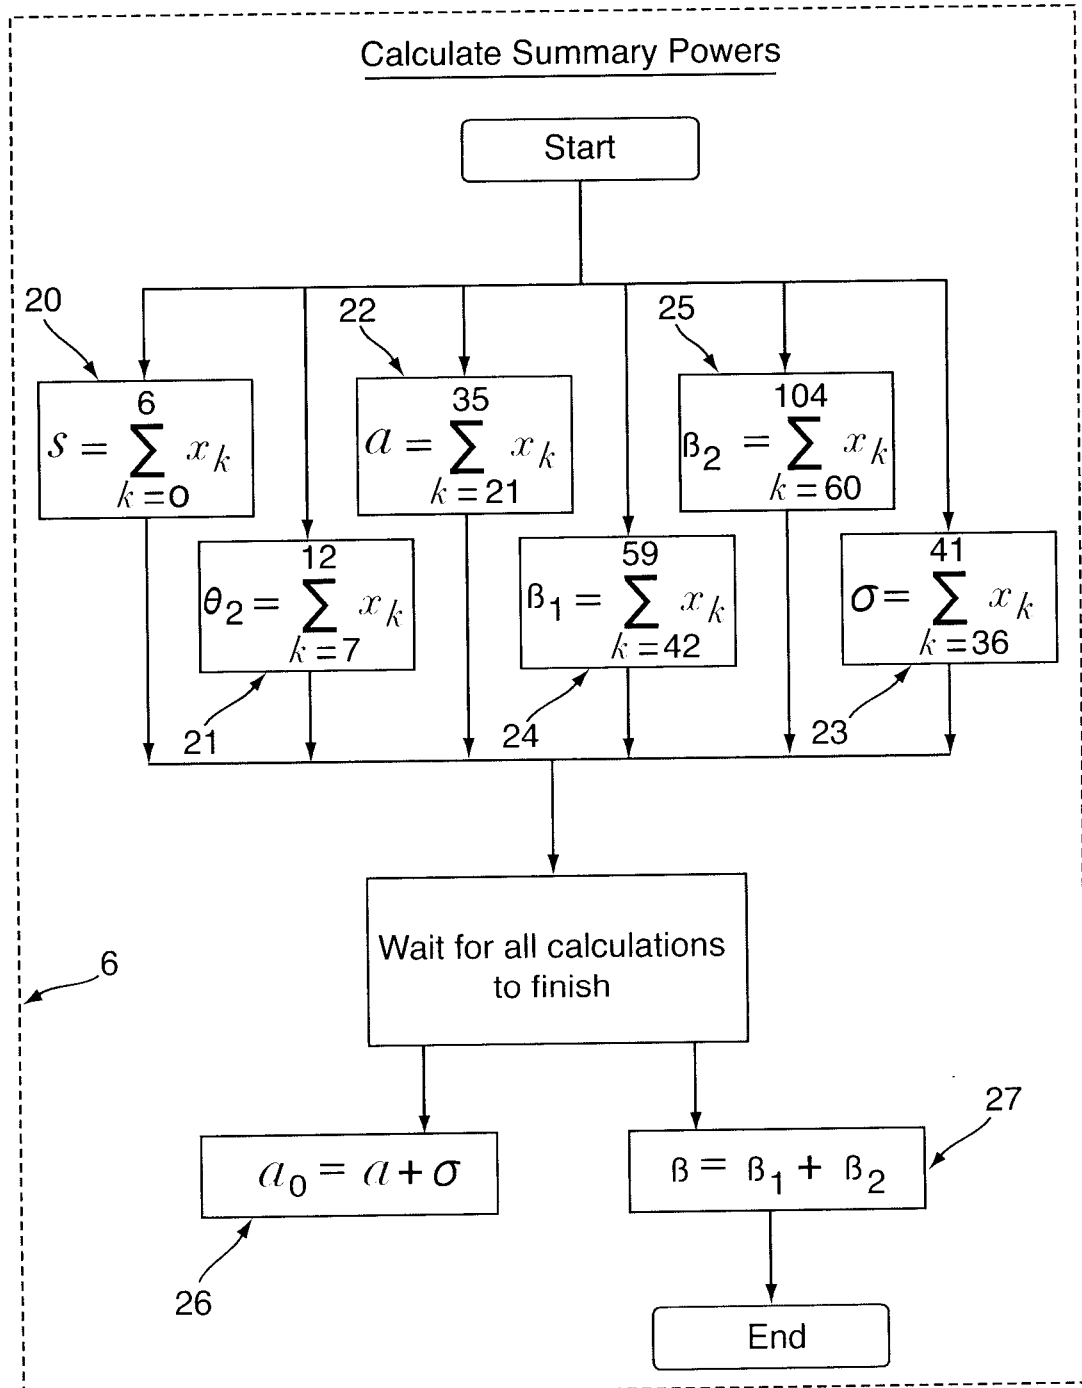

6 / 55

Fig. 6

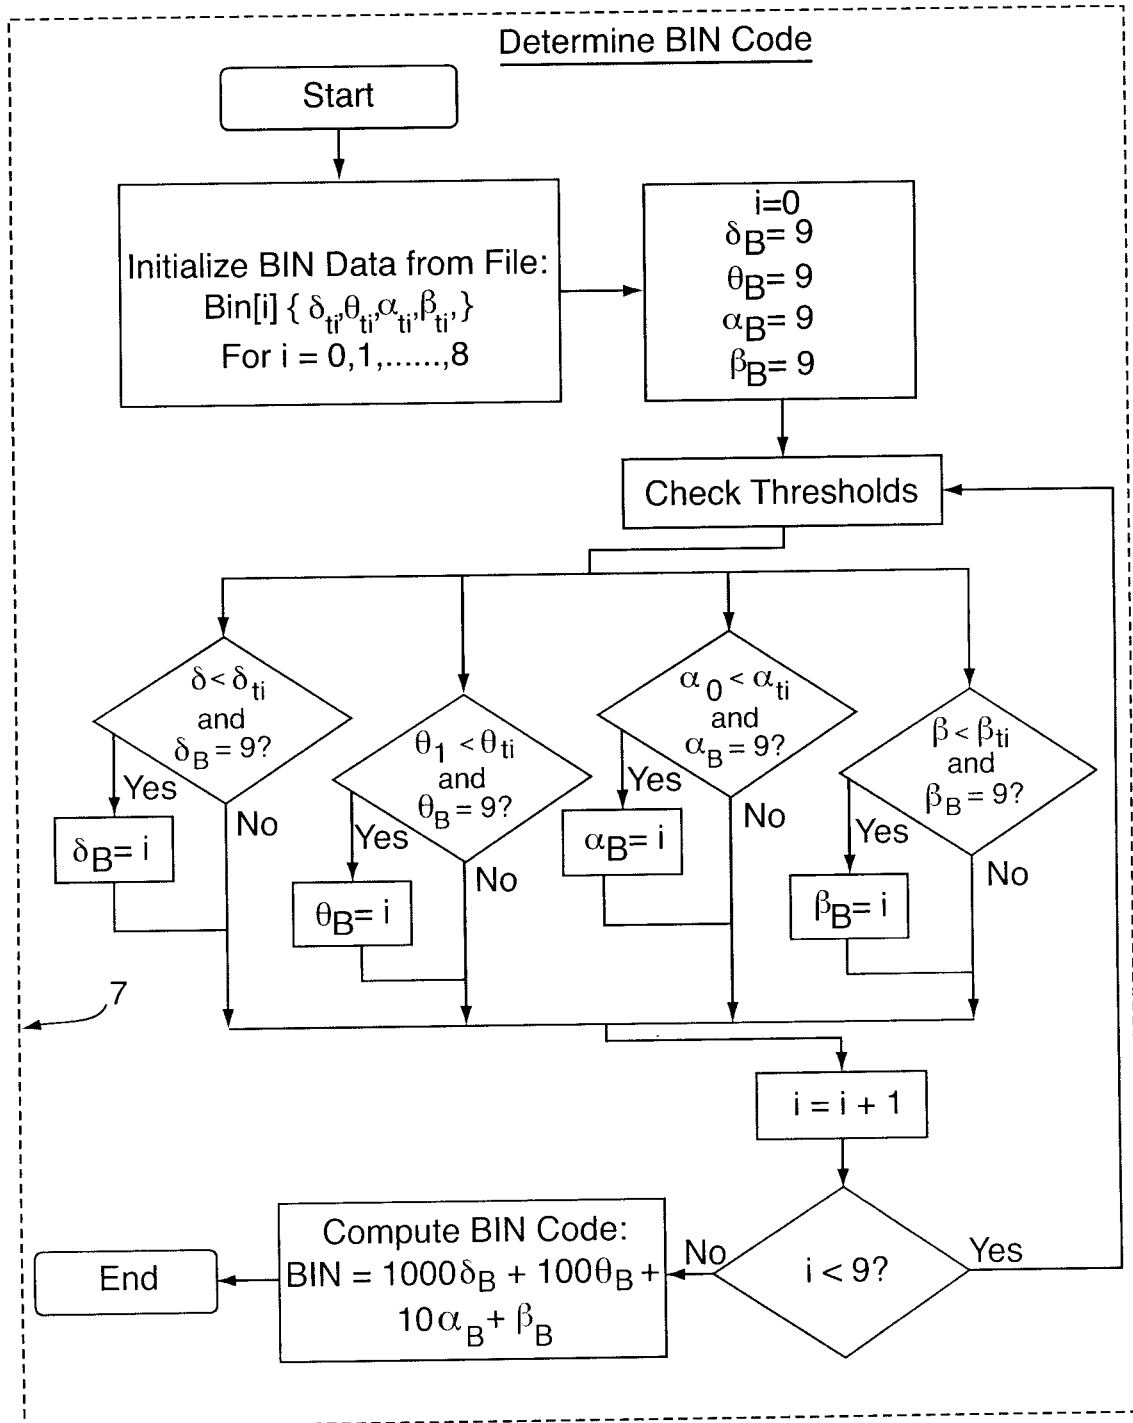

7 / 55

Fig. 7

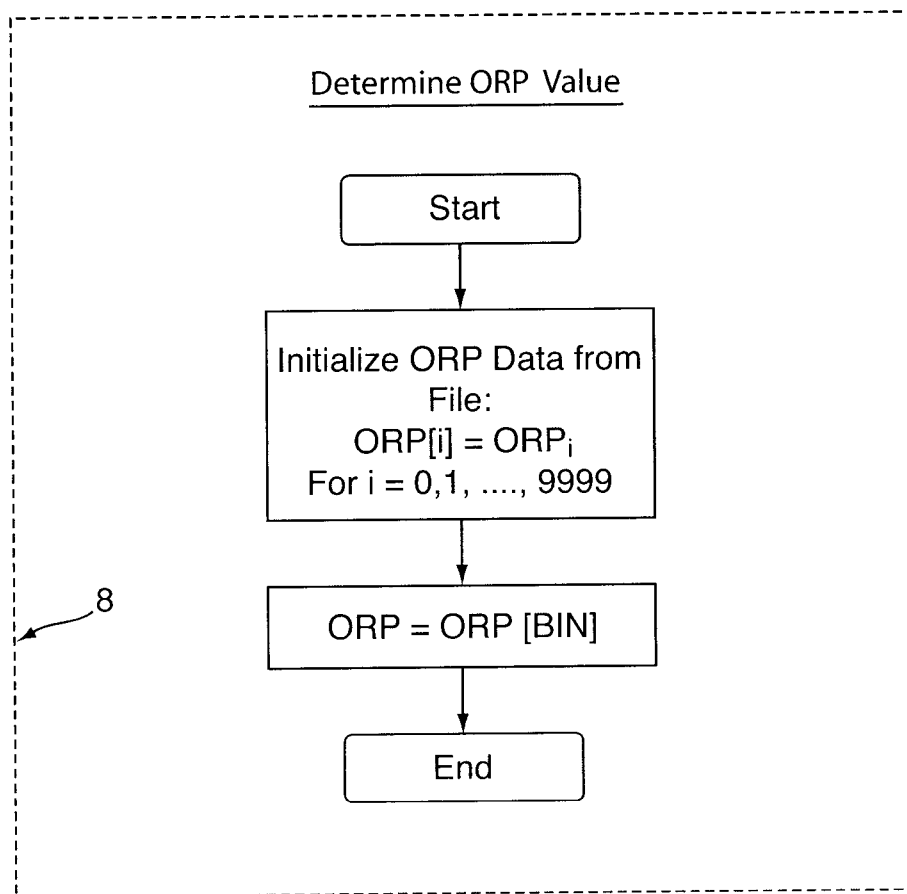


Fig. 8a


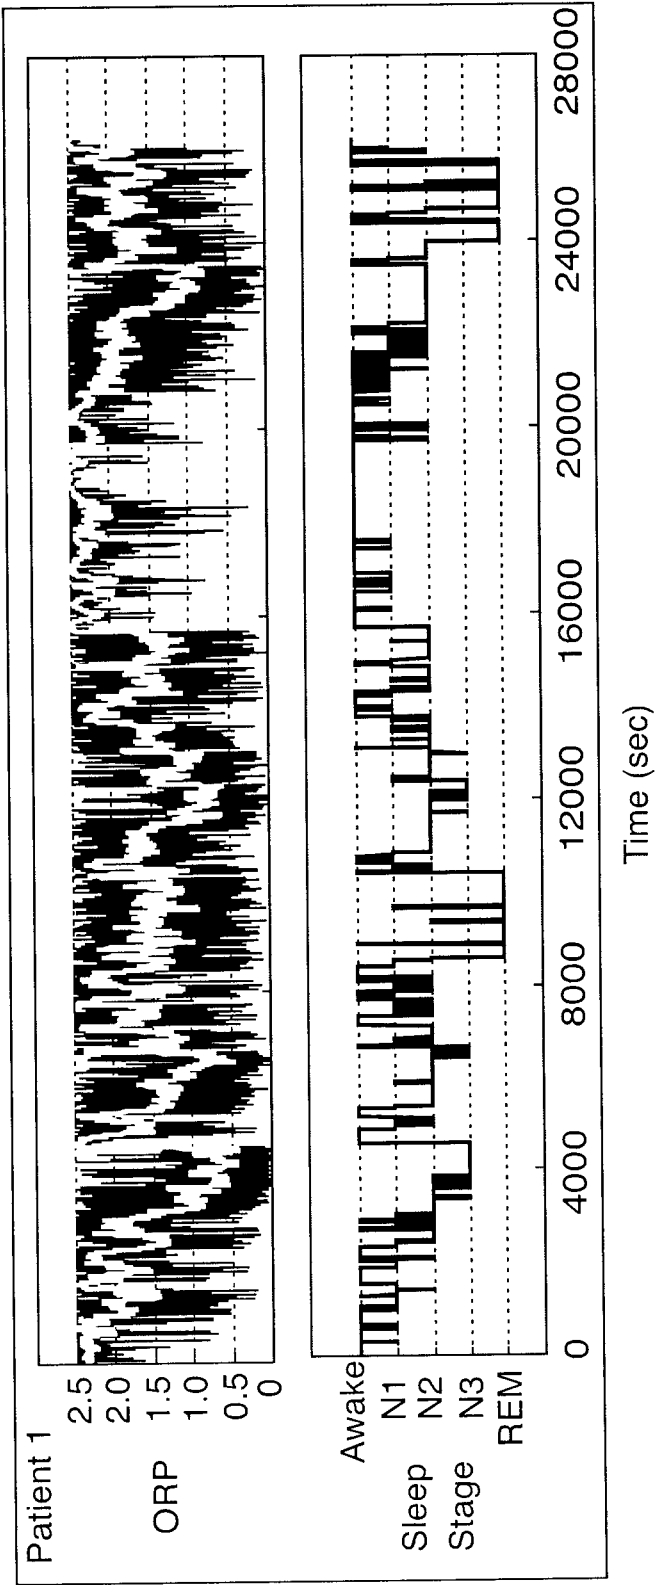


Fig. 8b

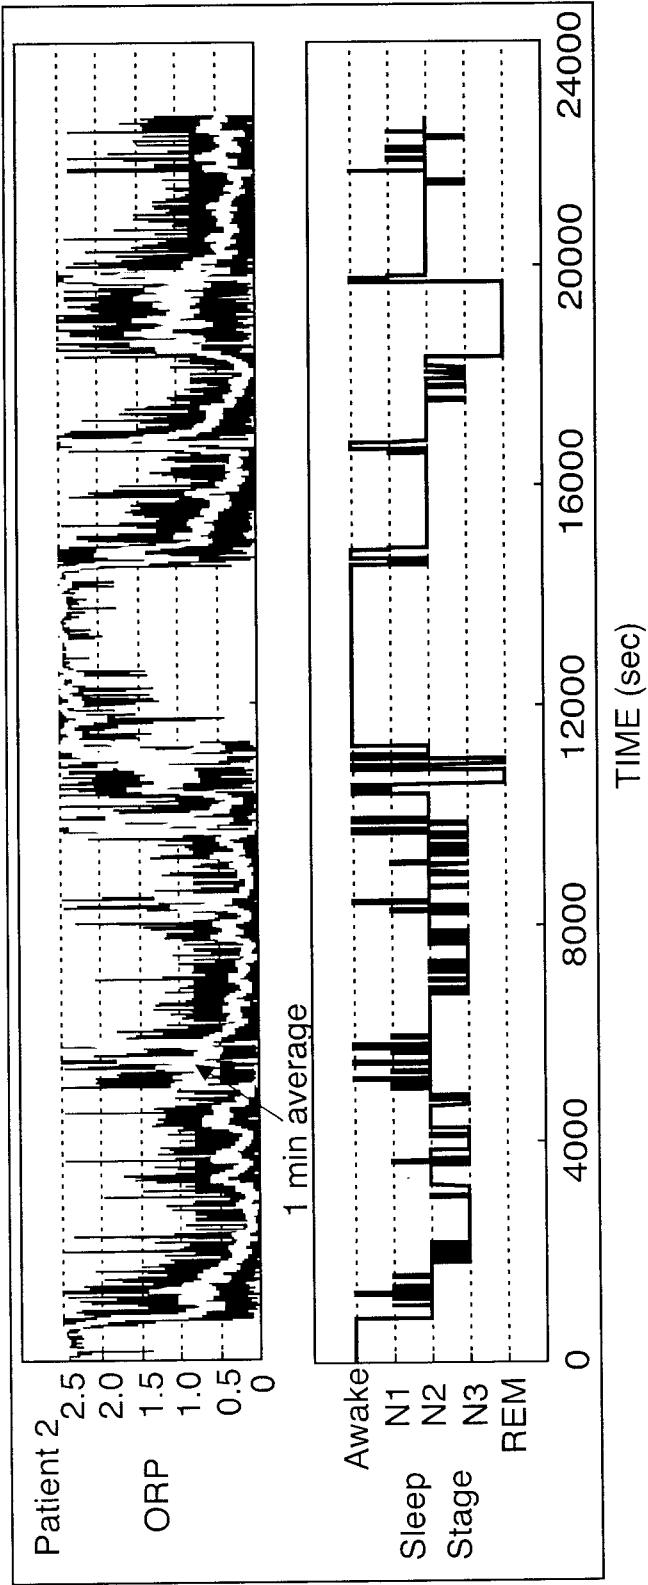

10 / 55

Fig. 9

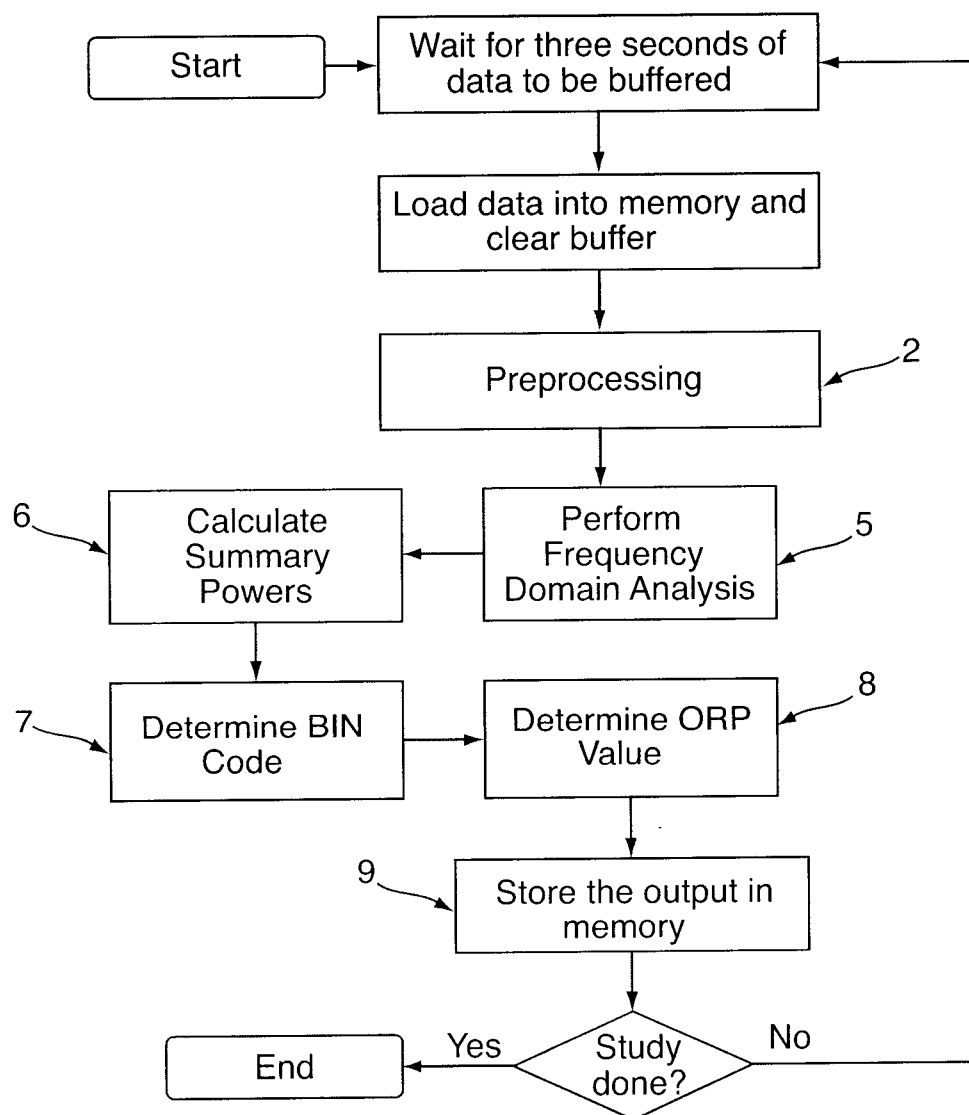
Determining ORP: Processing of streaming PSG data

Fig. 10

YRT - EEG Portable Monitor

Texas Instruments ADS1299

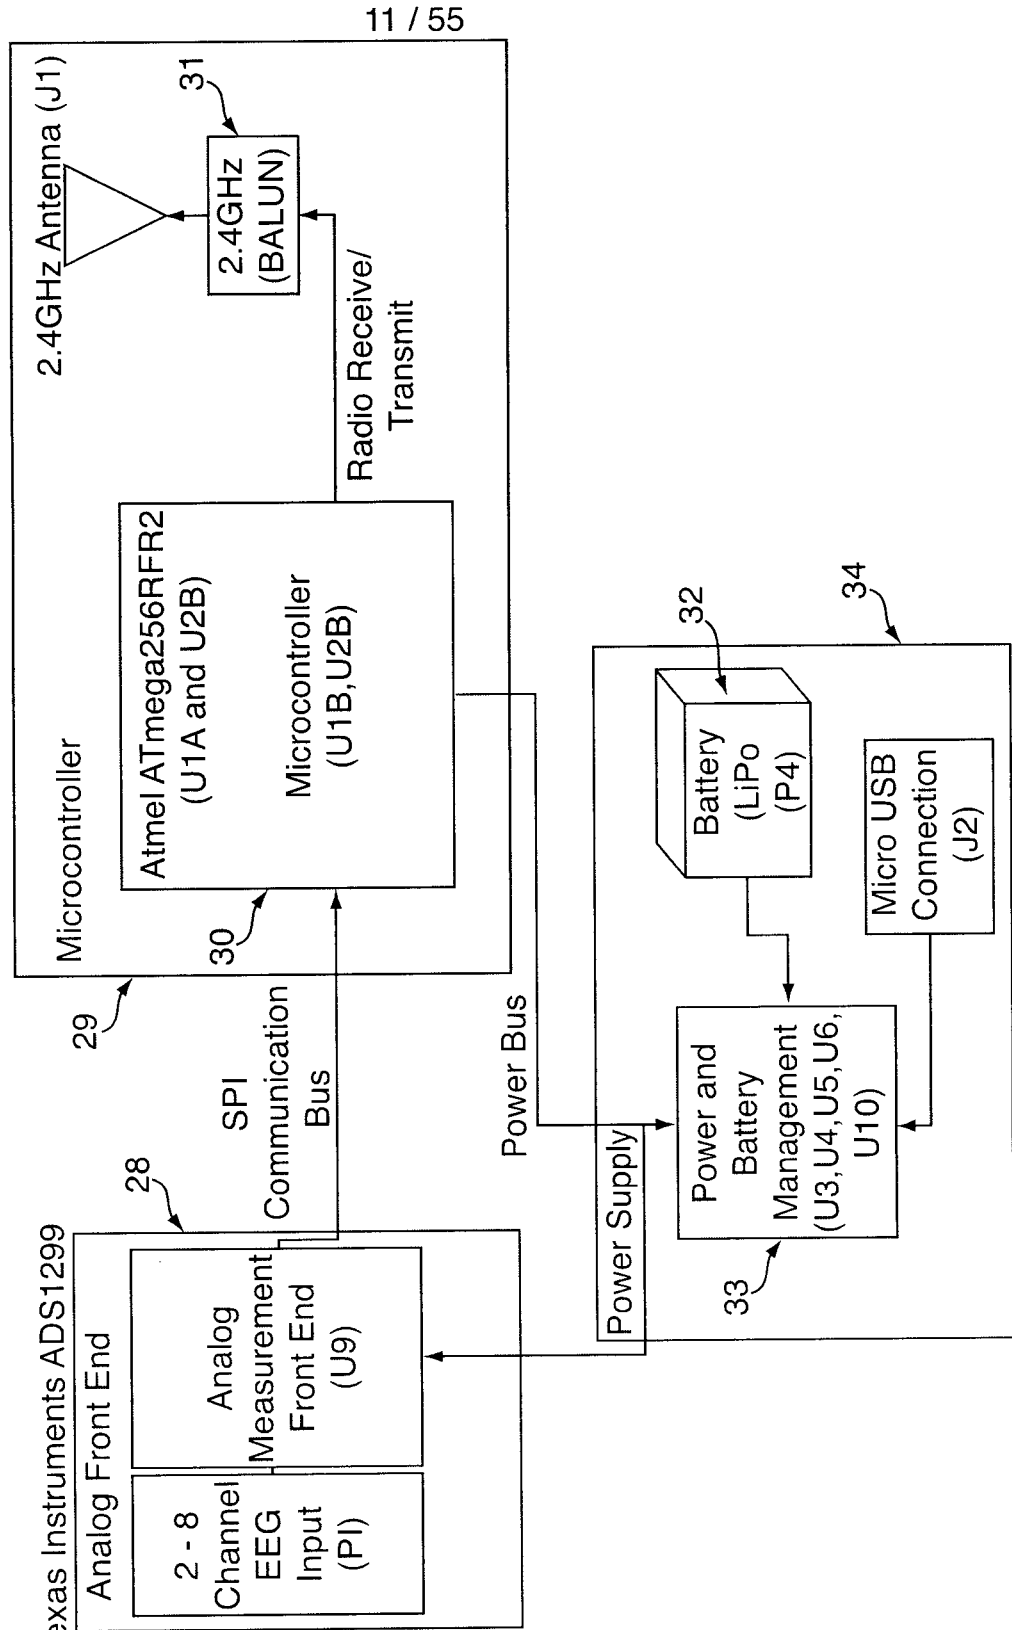


Fig. 11a

Biopotential Measurement Analog Front End

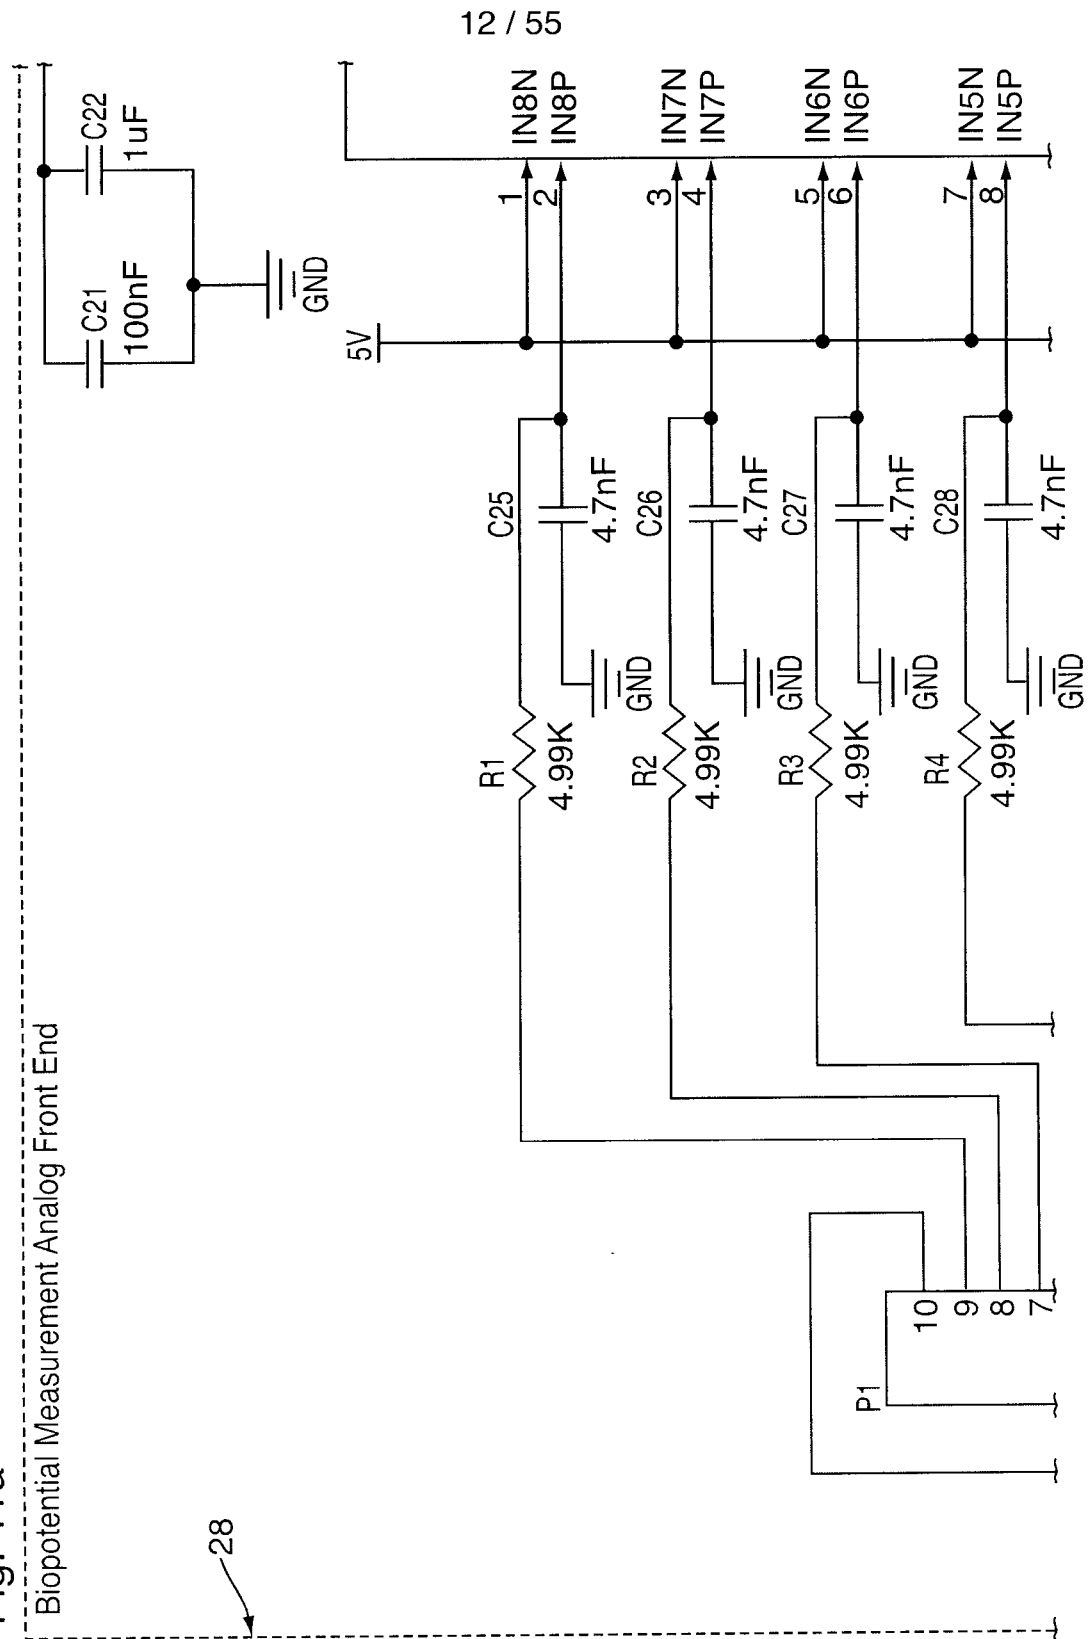
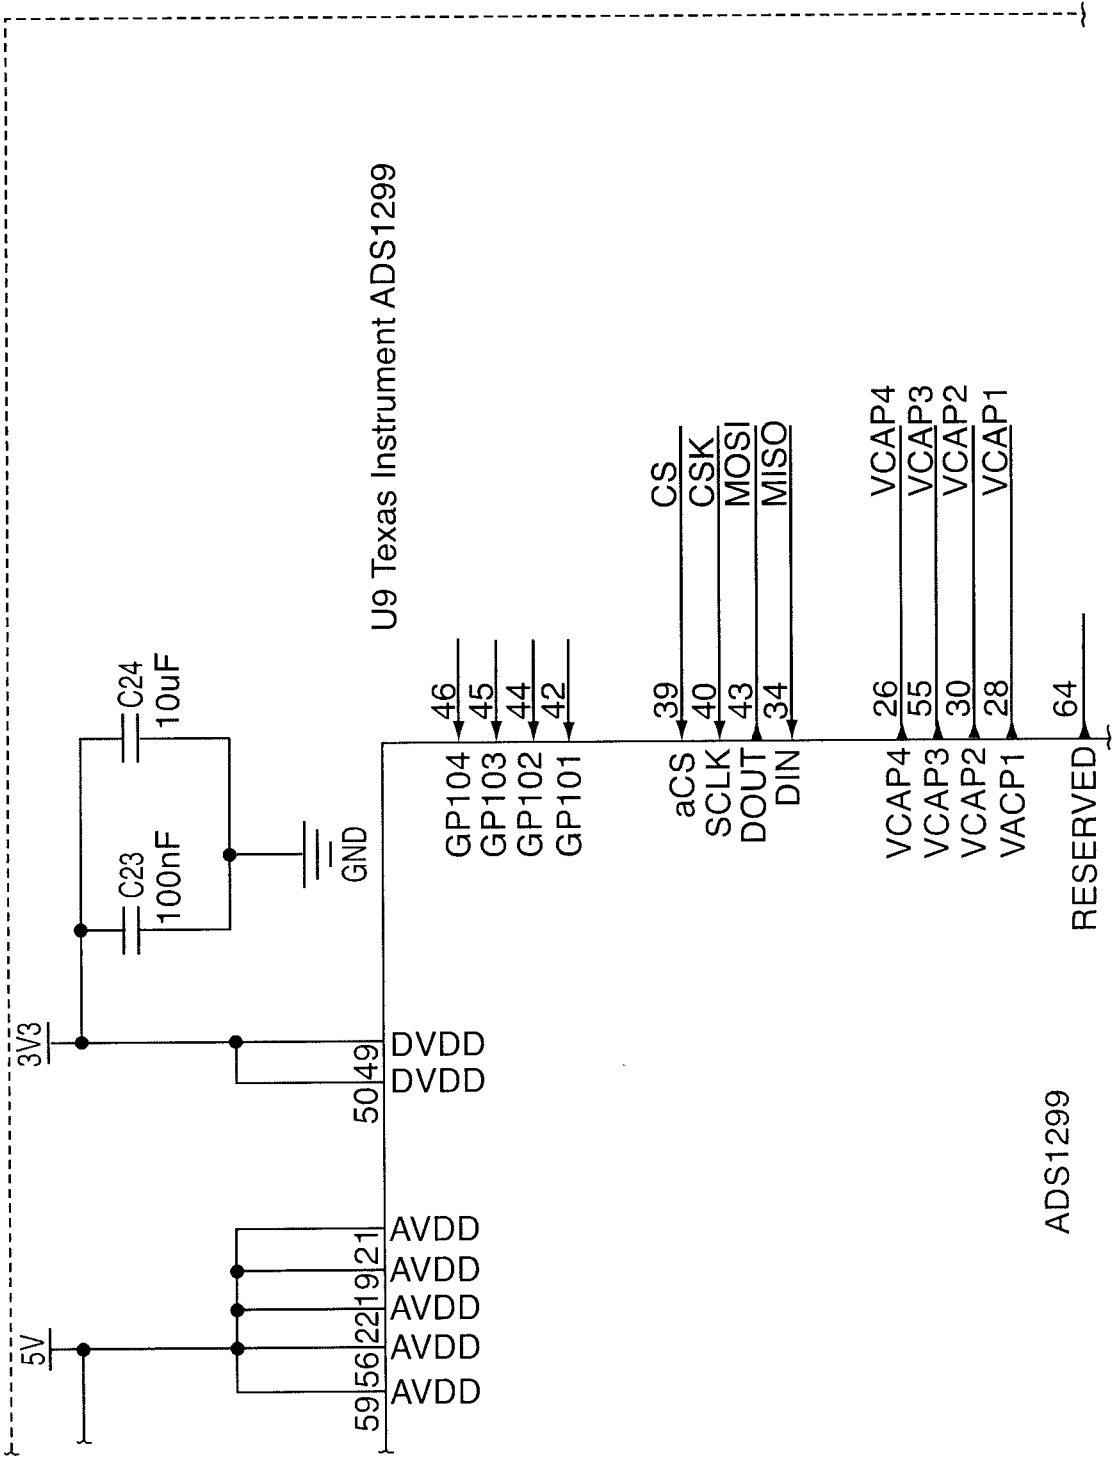


Fig. 11b



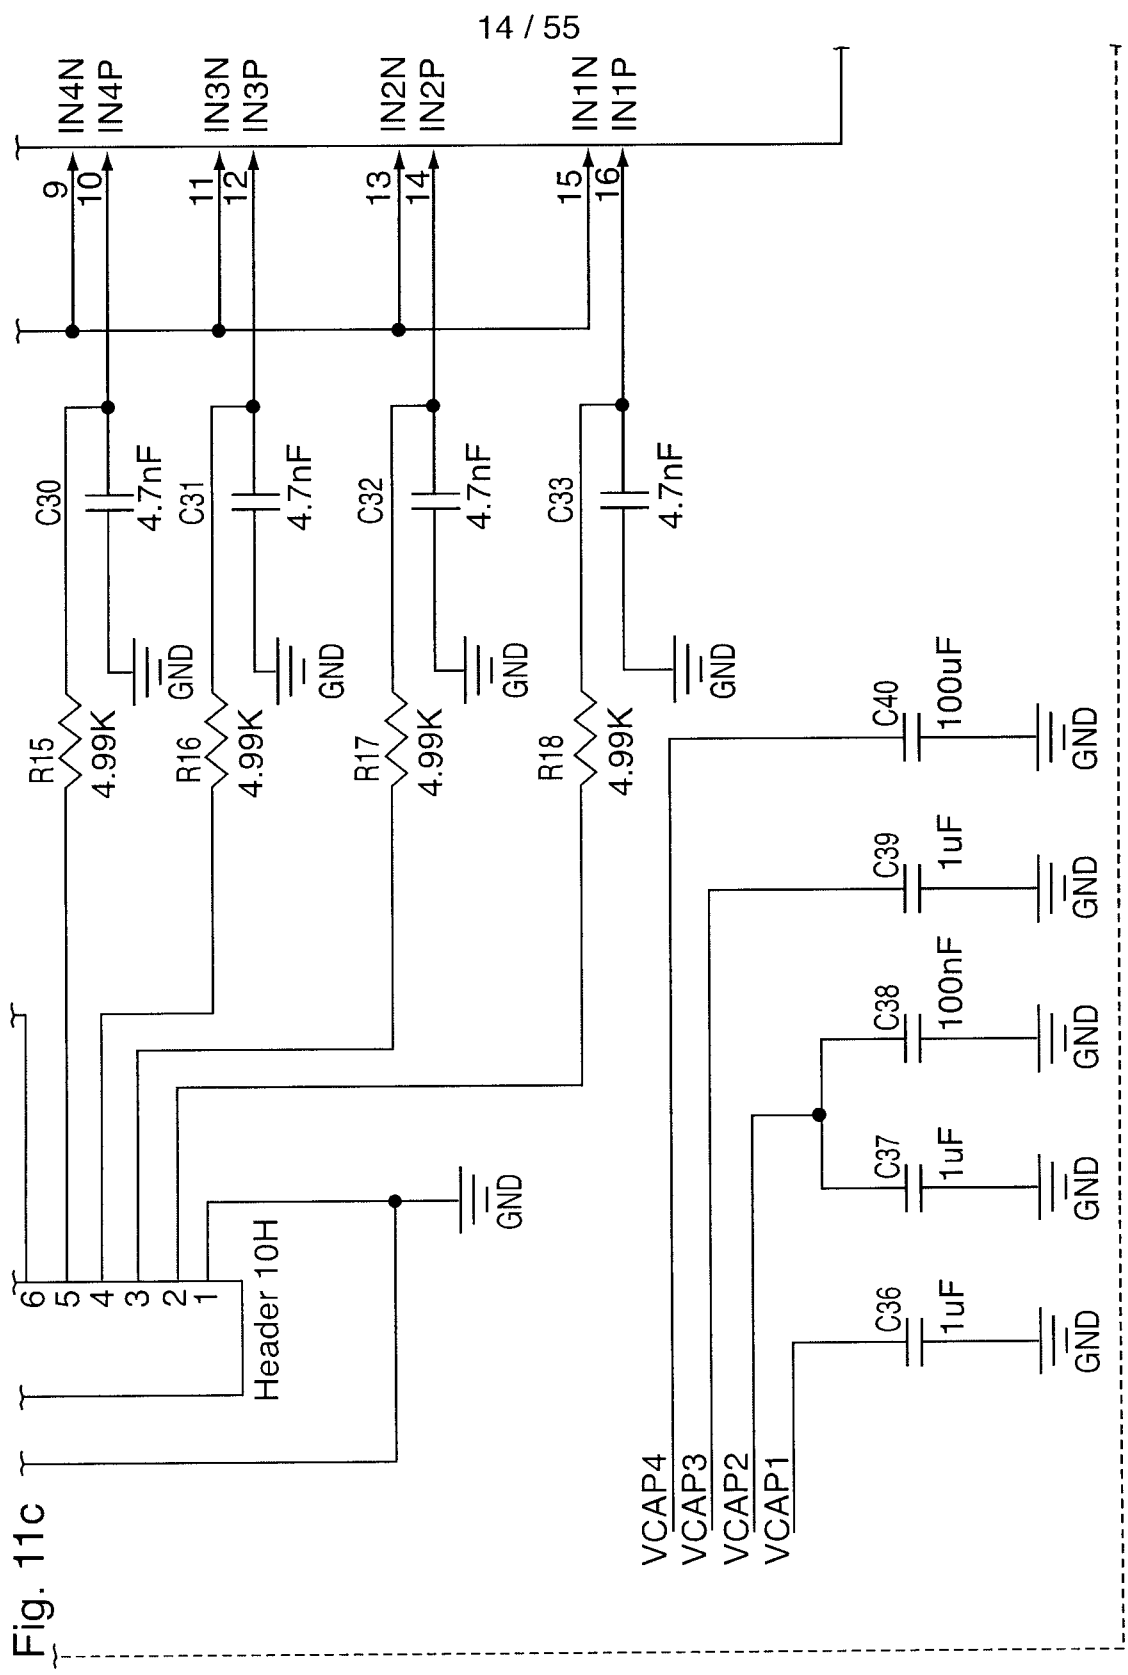


Fig. 11c

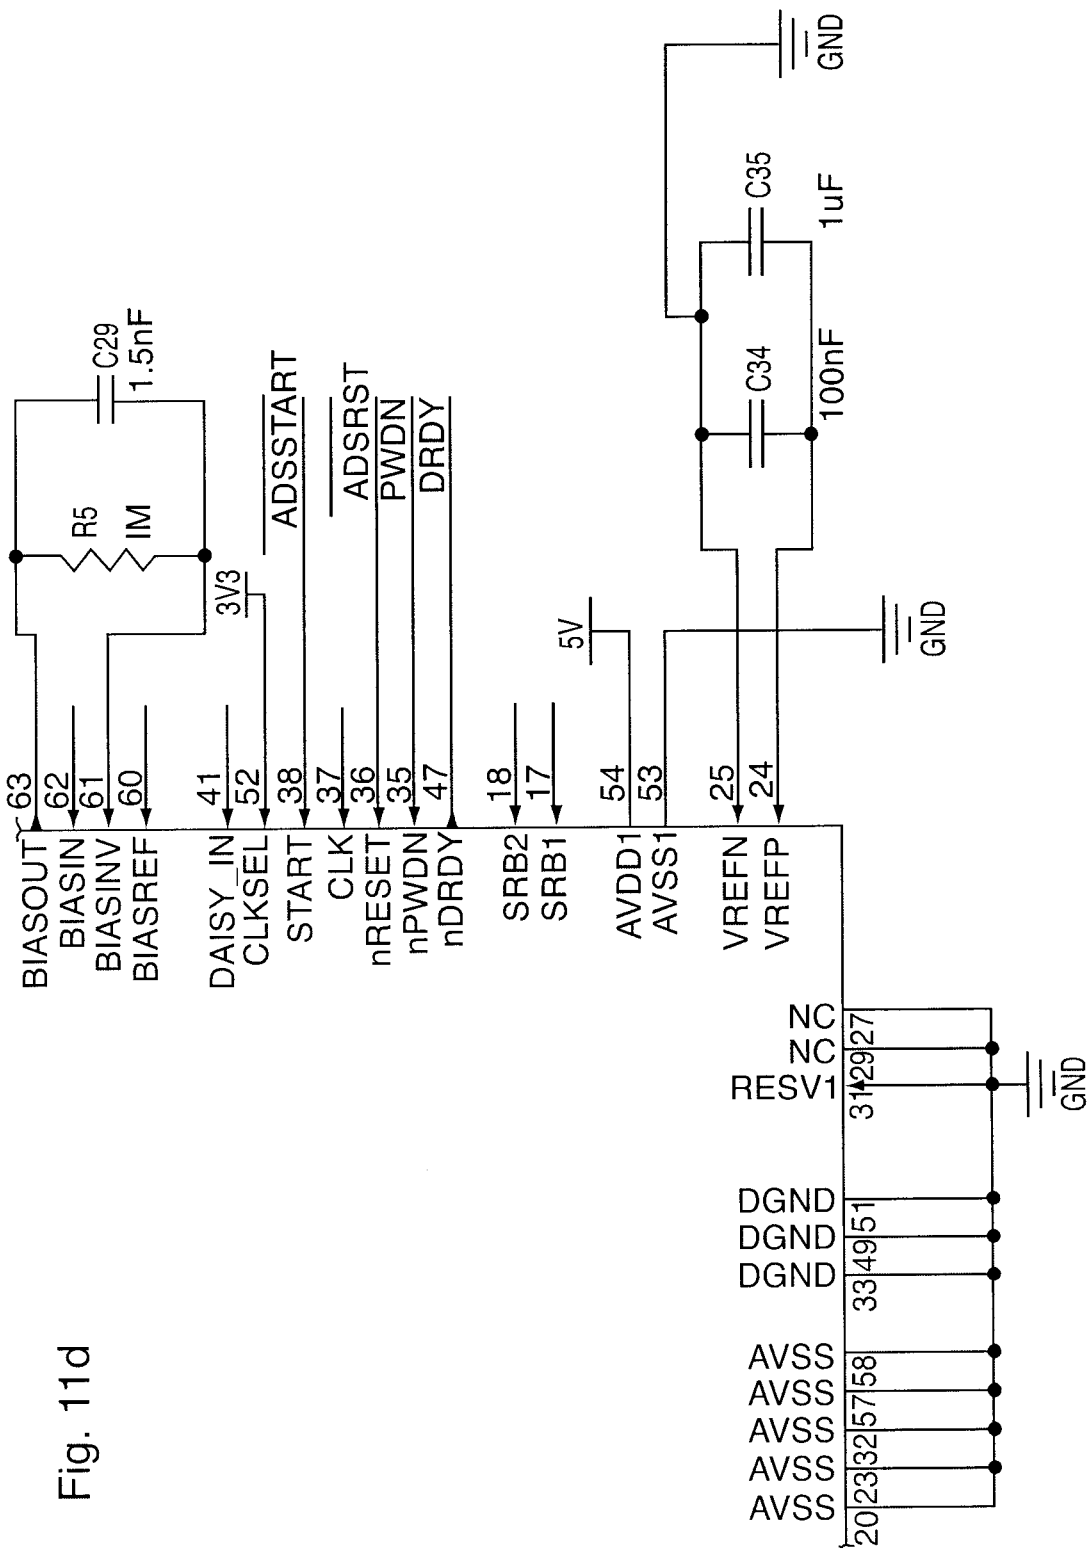


Fig. 11d

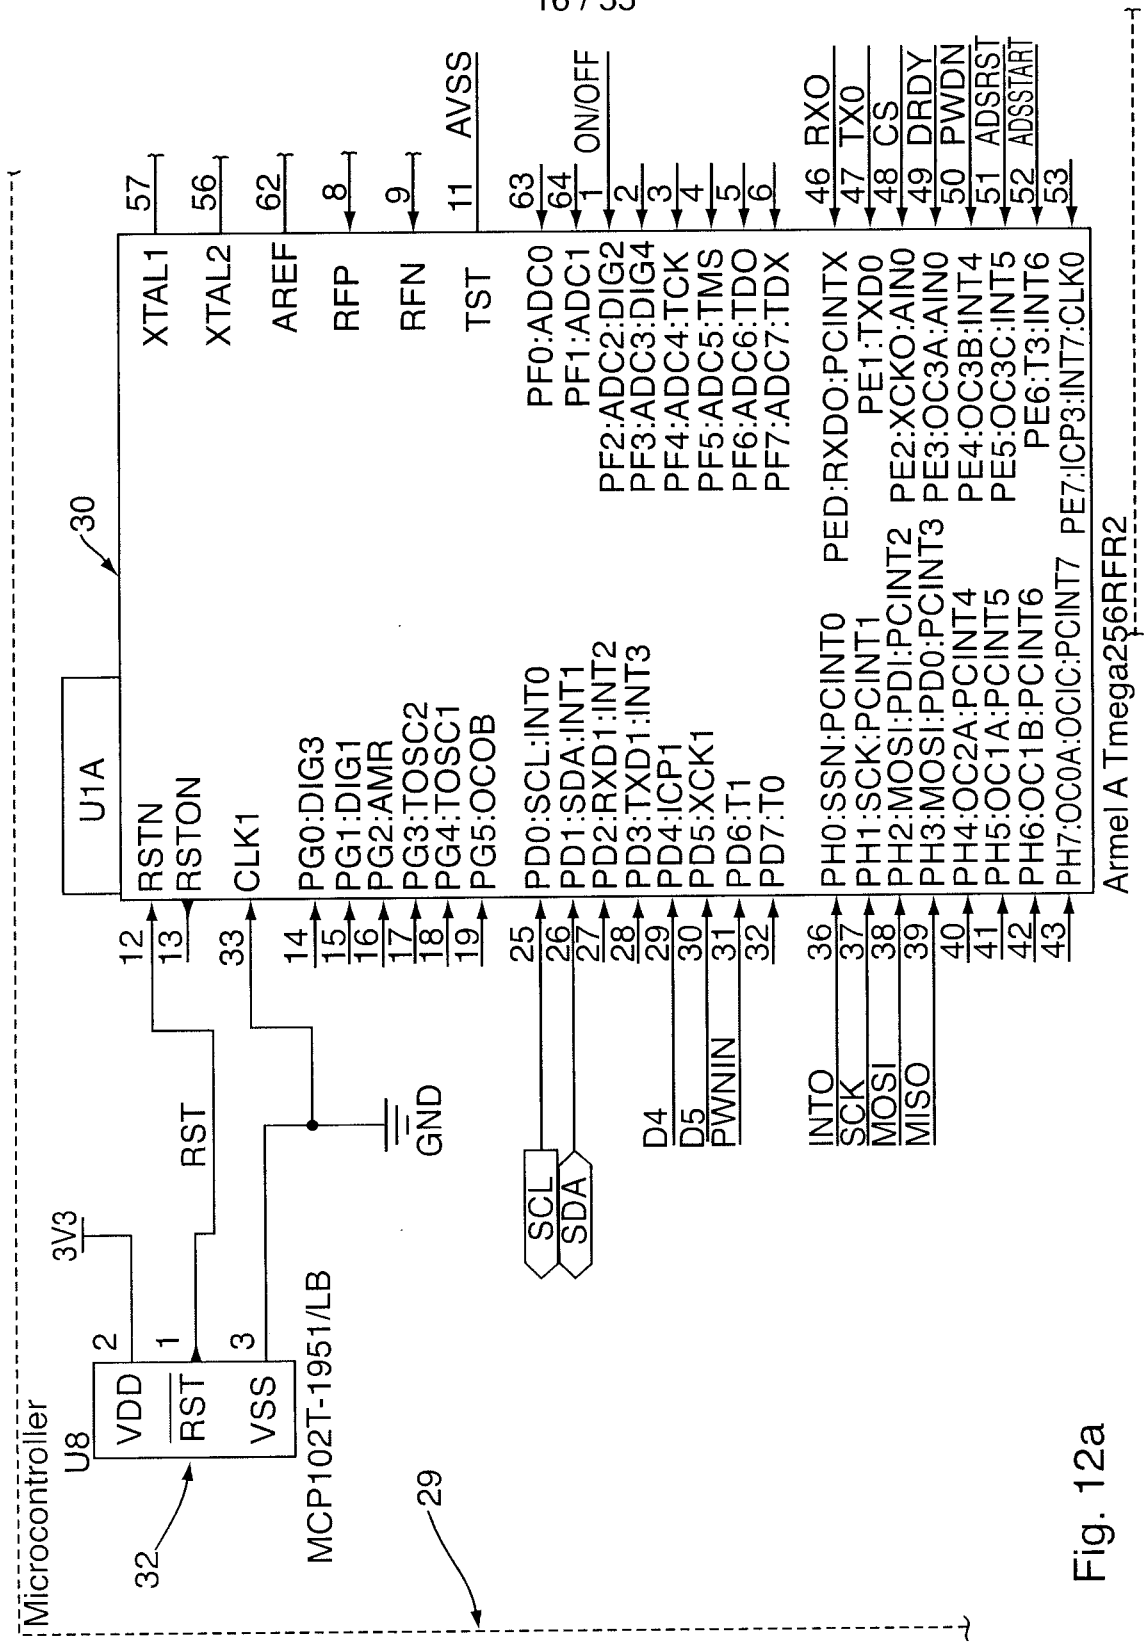


Fig. 12a

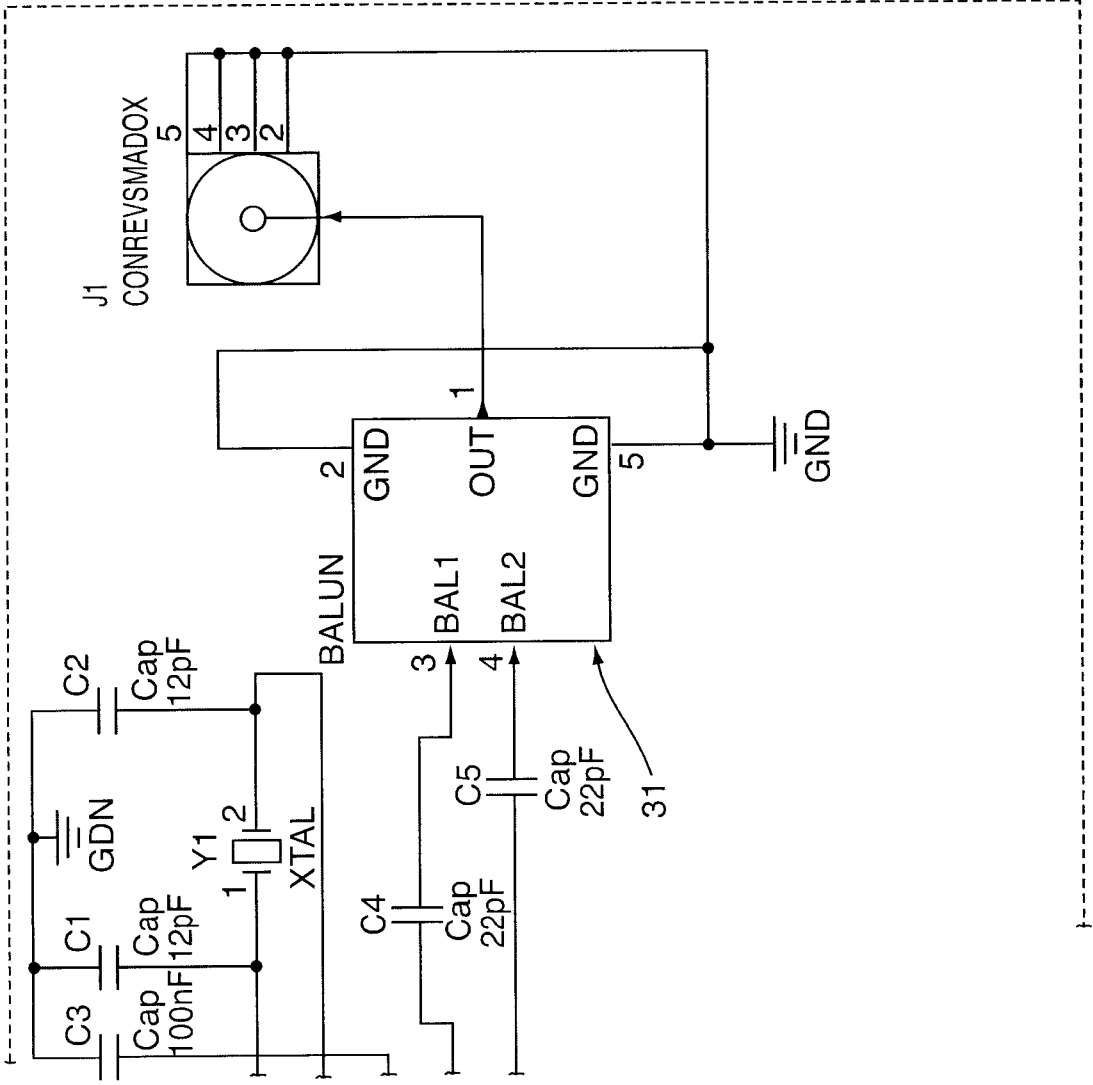


Fig. 12b

Fig. 12c

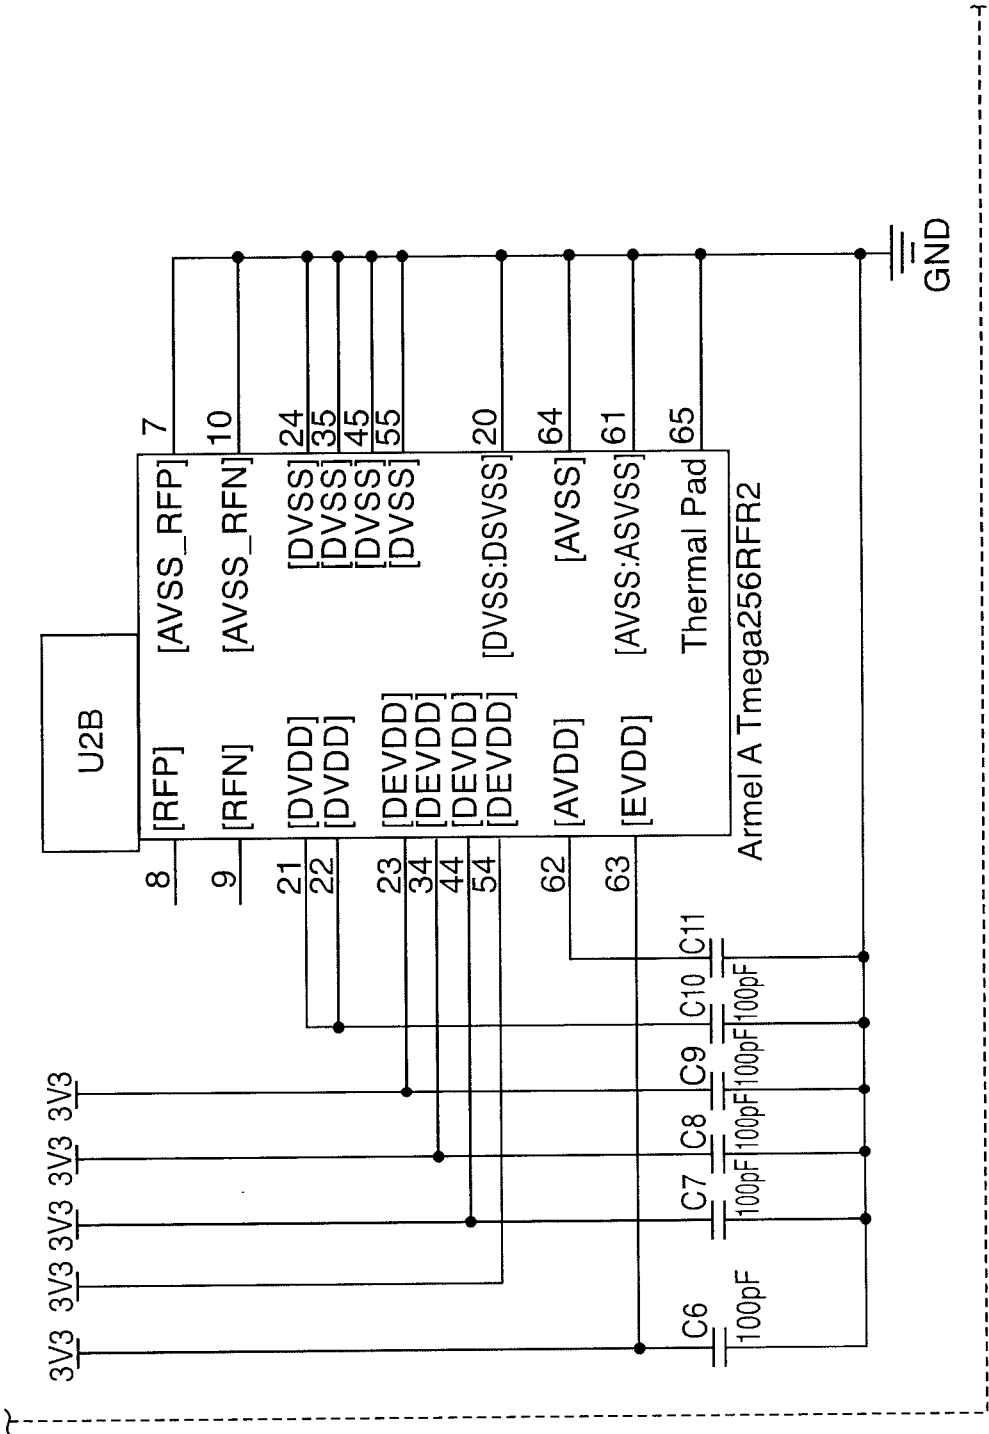
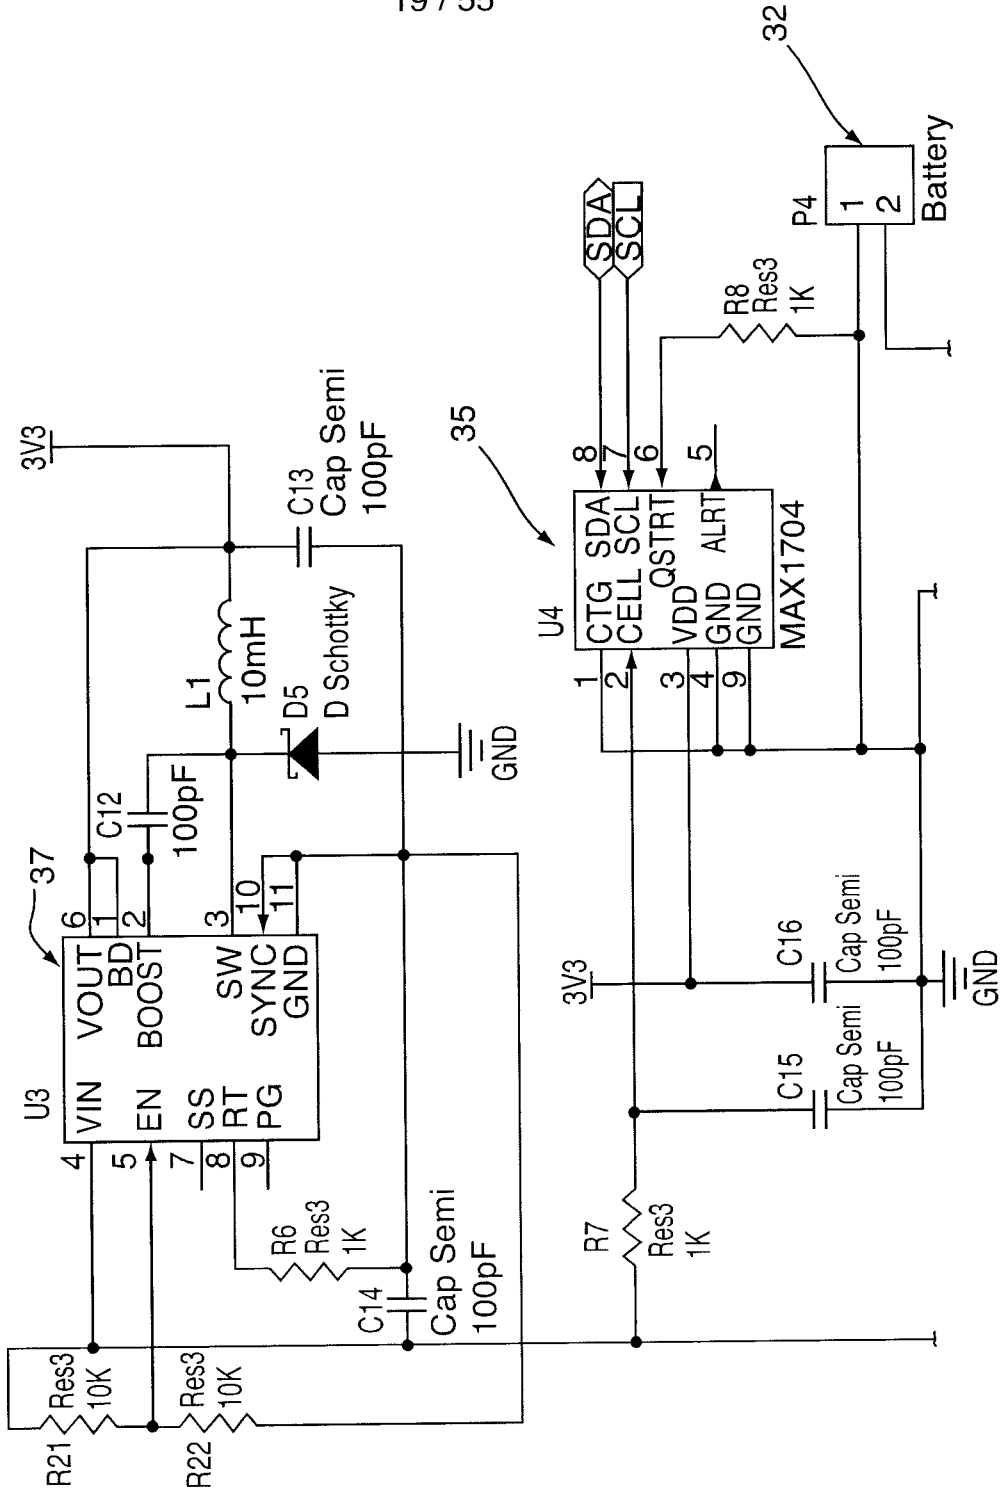


Fig. 13a

Power System-Battery Charge and Measurement



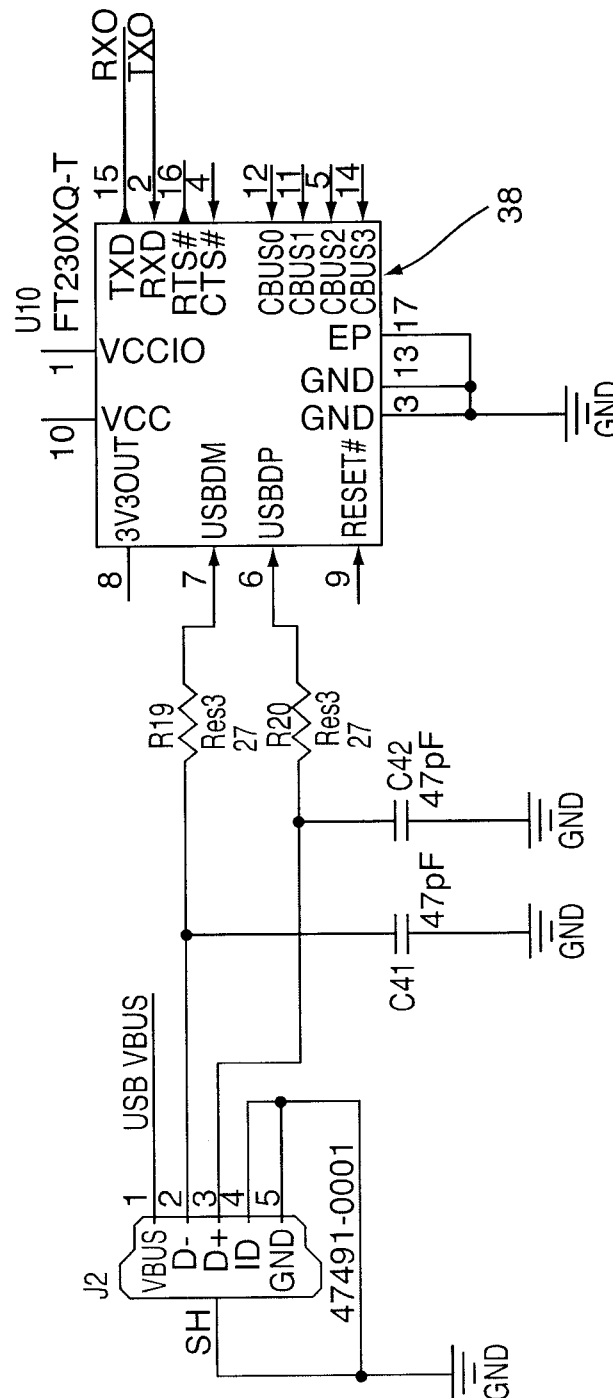


Fig. 13b


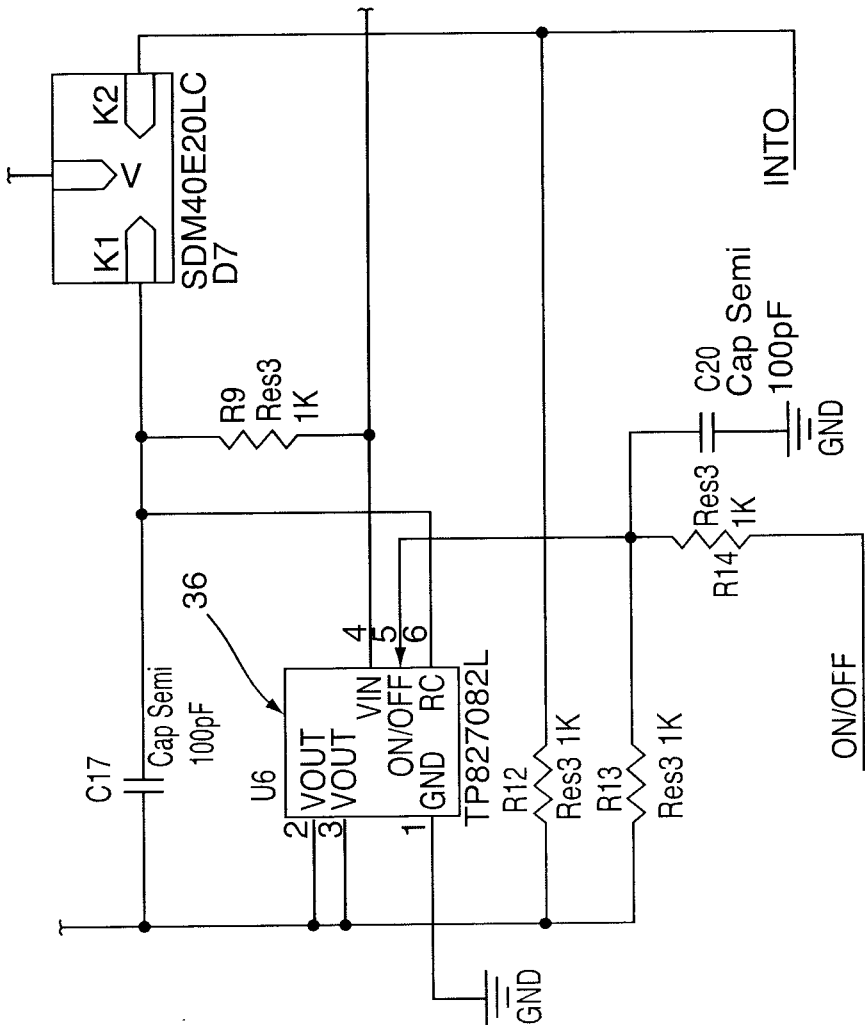


Fig. 13c

Fig. 13d

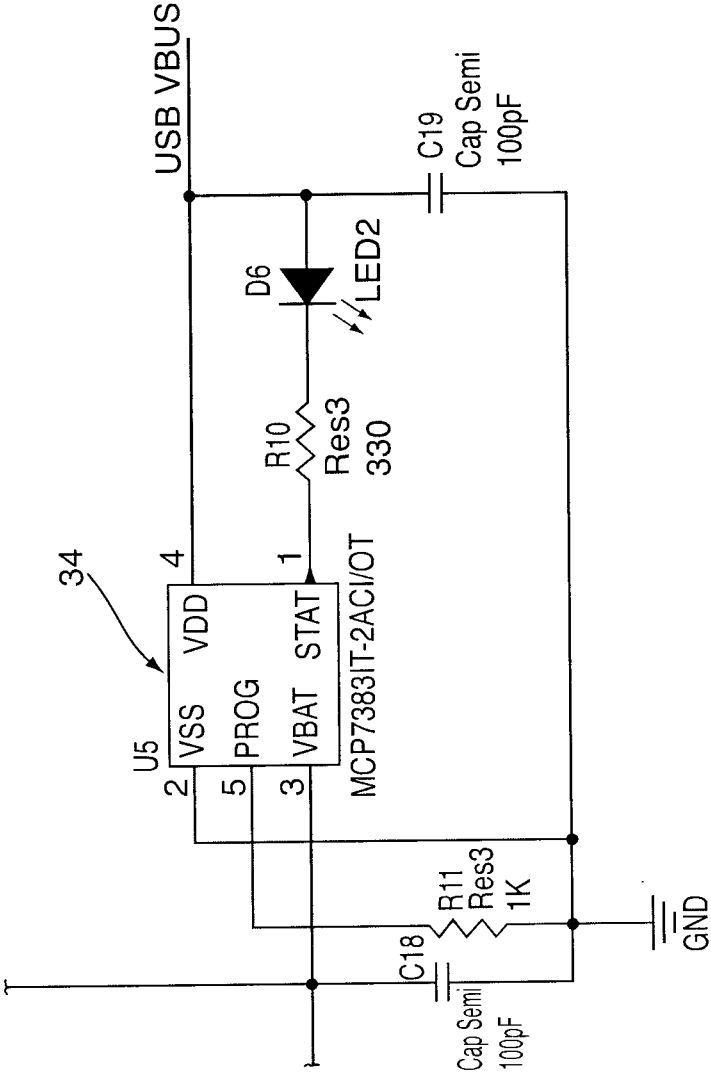

23 / 55

Fig. 14a

	0	1	2	3	4	5	6	7	8	9	10	11	12
0	0.92	1.80	1.88	1.95	2.05	2.13	2.27	2.39	2.50	2.50	1.33	1.72	2.02
20	1.81	2.21	2.28	2.24	2.32	2.24	2.30	2.39	2.46	2.50	2.30	2.30	2.31
40	1.98	2.38	2.40	2.47	2.44	2.42	2.45	2.41	2.46	2.49	2.50	2.39	2.46
60	2.30	2.27	2.50	2.49	2.49	2.47	2.49	2.49	2.48	2.49	2.30	2.37	2.41
80	2.30	2.50	2.43	2.44	2.50	2.49	2.49	2.50	2.50	2.50	2.30	2.30	2.30
100	0.26	0.52	0.78	0.78	1.03	1.38	1.64	1.93	2.20	2.50	0.48	0.80	0.78
120	1.10	1.11	1.34	1.51	1.68	1.52	1.85	2.13	2.32	2.50	1.50	1.60	1.71
140	1.60	1.60	1.90	2.24	2.28	2.27	2.25	2.24	2.30	2.47	2.00	2.00	2.16
160	2.20	2.20	2.32	2.39	2.42	2.43	2.33	2.44	2.48	2.50	2.30	2.30	2.50
180	2.50	2.50	2.50	2.50	2.47	2.50	2.49	2.49	2.48	2.50	2.50	2.50	2.50
200	0.19	0.28	0.35	0.66	0.63	0.46	0.80	1.60	2.00	2.20	0.24	0.28	0.37
220	0.50	0.56	0.81	1.00	1.15	1.30	1.45	1.60	2.15	2.30	0.80	0.80	0.80
240	1.28	1.40	1.52	1.64	2.04	1.97	1.81	2.00	2.31	2.50	1.55	1.65	1.75
260	1.82	1.90	1.98	2.08	2.34	2.29	2.23	2.42	2.47	2.47	2.09	2.15	2.21
280	2.36	2.40	2.44	2.37	2.44	2.46	2.46	2.44	2.47	2.50	2.50	2.50	2.50
300	0.16	0.30	0.15	0.31	0.16	0.80	1.00	1.19	1.38	1.57	0.14	0.25	0.32
320	0.12	0.38	0.40	0.80	0.80	1.00	0.80	1.50	2.34	1.82	0.80	0.80	0.95
340	0.80	0.23	1.19	1.31	1.44	1.56	2.10	1.80	2.18	2.06	1.20	1.31	1.42
360	1.47	1.57	1.66	1.75	2.20	2.34	2.31	2.03	2.28	2.50	1.74	1.82	1.89
380	2.01	2.07	2.13	2.26	2.50	2.50	2.33	2.40	2.47	2.50	2.28	2.32	2.37
400	0.08	0.07	0.10	0.00	0.80	0.80	0.80	0.80	1.03	1.22	0.25	0.00	0.30
420	0.00	0.00	0.18	0.80	0.69	0.85	1.01	1.17	1.33	1.49	0.80	0.00	0.80
440	0.80	0.80	0.80	0.80	1.11	1.24	1.37	1.50	1.63	1.76	0.80	0.80	1.09
460	1.12	1.22	1.33	1.43	1.53	2.50	2.29	2.27	1.93	2.03	1.39	1.48	1.56
480	1.66	1.73	1.80	1.87	1.94	2.41	2.31	2.42	2.50	2.50	1.93	1.98	2.04
500	0.00	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.00	0.80

25 / 55

Fig. 14b

1100	0.23	0.47	0.74	1.05	0.90	1.12	1.69	1.82	2.34	2.22	0.35	0.63	0.81
1120	0.24	0.71	1.20	1.49	1.48	1.85	1.89	2.14	2.37	2.50	1.10	1.25	1.31
1140	1.32	1.46	1.76	1.97	1.91	2.23	2.28	2.25	2.41	2.43	1.55	1.67	2.18
1160	1.78	1.88	1.99	2.22	2.42	2.47	2.38	2.37	2.45	2.50	2.01	2.09	2.18
1180	2.23	2.31	2.50	2.36	2.47	2.50	2.48	2.50	2.47	2.47	2.50	2.50	2.50
1200	0.12	0.24	0.33	0.63	0.64	0.51	1.30	1.50	1.70	1.90	0.17	0.27	0.29
1220	0.26	0.50	0.55	0.87	0.79	1.11	1.31	1.83	2.29	2.50	0.14	0.60	0.73
1240	0.17	0.54	0.84	1.39	1.71	1.77	1.81	2.01	2.16	2.50	0.80	1.37	1.51
1260	1.46	1.59	1.71	2.08	2.20	2.16	2.31	2.36	2.35	2.45	1.69	1.80	2.16
1280	1.92	2.02	2.12	2.33	2.50	2.44	2.41	2.44	2.45	2.47	2.14	2.23	2.32
1300	0.07	0.16	0.22	0.36	0.31	0.80	0.80	1.18	1.38	1.58	0.10	0.20	0.19
1320	0.11	0.22	0.33	0.41	0.64	0.64	1.16	1.48	2.40	2.50	0.17	0.41	0.68
1340	0.00	0.80	1.00	0.82	1.25	1.18	1.40	1.59	1.95	2.50	0.19	0.80	1.00
1360	1.14	0.80	1.41	1.55	1.96	1.90	1.90	2.14	2.26	2.41	1.37	1.50	1.62
1380	1.60	1.71	1.83	1.94	2.41	2.40	2.29	2.32	2.41	2.48	1.83	1.93	2.03
1400	0.09	0.11	0.09	0.19	0.20	0.19	0.80	0.80	1.06	1.26	0.06	0.06	0.12
1420	0.00	0.00	0.18	0.49	0.38	0.39	0.80	1.18	1.36	1.54	0.10	0.29	0.18
1440	0.80	0.26	0.33	0.80	0.80	1.18	0.80	1.50	2.39	1.82	0.80	0.80	0.80
1460	0.80	0.21	0.16	1.25	1.39	1.53	1.67	1.82	1.96	2.50	0.80	1.18	0.80
1480	1.28	1.40	1.52	1.65	1.77	2.36	2.40	2.37	2.29	2.46	1.51	1.62	1.73
1500	0.00	0.00	0.09	0.00	0.00	0.80	0.80	0.80	0.75	0.95	0.00	0.20	0.00
1520	0.06	0.06	0.19	0.17	0.00	0.21	0.80	0.87	1.05	1.24	0.80	0.00	0.00
1540	0.80	0.80	0.13	0.36	0.18	0.87	0.80	1.20	1.36	1.53	0.80	0.80	0.80
1560	0.80	0.80	0.80	0.80	1.09	1.24	1.38	1.53	1.67	2.29	0.80	0.80	1.01
1580	0.96	1.09	1.22	1.35	1.47	1.60	2.16	2.23	2.17	2.11	1.19	1.31	1.43
1600	0.00	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.00	0.00	0.00
1620	0.80	0.00	0.15	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
1640	0.80	0.80	0.00	0.17	0.80	0.80	0.80	0.90	1.06	1.23	0.80	0.80	0.80
1660	0.80	0.80	0.80	0.80	0.80	0.93	1.08	1.23	1.38	1.53	0.80	0.80	0.70
1680	0.80	0.78	0.91	1.04	1.17	1.30	1.43	1.57	1.70	2.27	0.87	1.00	1.12

27 / 55

Fig. 14c

2220	0.18	0.35	0.40	0.72	0.79	1.08	1.49	1.78	2.18	2.50	0.15	0.46	0.79
2240	0.09	0.48	0.59	0.93	1.33	1.51	1.73	1.98	2.10	2.50	0.80	0.80	1.24
2260	0.80	0.80	1.38	1.76	1.84	2.08	2.21	2.18	2.18	2.45	1.19	1.35	1.52
2280	1.33	1.49	1.66	1.82	2.28	2.44	2.36	2.34	2.44	2.48	1.47	1.63	1.80
2300	0.04	0.08	0.14	0.27	0.31	0.58	0.80	1.11	1.29	1.46	0.05	0.05	0.23
2320	0.04	0.14	0.27	0.30	0.63	0.64	0.77	1.13	1.57	1.74	0.12	0.25	0.37
2340	0.20	0.15	0.46	0.48	0.91	1.01	1.41	1.42	1.99	2.31	0.36	0.32	0.65
2360	0.00	0.00	0.80	1.27	1.44	1.67	1.79	1.97	2.04	2.43	0.80	0.80	1.23
2380	0.80	0.80	1.38	1.55	2.08	2.04	2.29	2.38	2.24	2.43	1.17	1.34	1.52
2400	0.06	0.11	0.16	0.27	0.40	0.25	0.64	0.80	0.80	1.16	0.01	0.06	0.07
2420	0.00	0.05	0.09	0.13	0.12	0.42	0.58	1.10	1.28	1.45	0.08	0.18	0.26
2440	0.13	0.18	0.17	0.47	0.32	0.57	1.06	1.22	1.57	1.75	0.00	0.07	0.57
2460	0.80	0.28	0.44	0.80	1.16	1.33	1.54	1.68	1.50	2.50	0.80	0.80	0.80
2480	0.80	0.80	1.09	1.26	1.44	2.06	2.10	2.13	2.40	2.39	0.87	1.05	1.23
2500	0.02	0.03	0.00	0.07	0.15	0.80	0.80	0.80	0.80	0.80	0.02	0.05	0.05
2520	0.00	0.02	0.19	0.11	0.12	0.21	0.44	0.80	0.80	1.16	0.00	0.09	0.34
2540	0.00	0.18	0.40	0.24	0.43	0.80	0.60	0.80	1.29	1.46	0.00	0.09	0.23
2560	0.80	0.00	0.80	0.29	0.87	0.80	1.23	1.41	1.59	2.32	0.80	0.80	0.80
2580	0.80	0.80	0.80	0.80	1.16	1.34	1.52	2.05	2.07	2.26	0.80	0.80	0.80
2600	0.00	0.06	0.23	0.80	0.80	0.80	0.80	0.80	0.80	0.56	0.00	0.00	0.00
2620	0.06	0.14	0.13	0.00	0.10	0.09	0.80	0.80	0.80	0.87	0.00	0.00	0.16
2640	0.80	0.00	0.19	0.29	0.33	0.33	0.31	0.80	0.80	1.18	0.80	0.19	0.00
2660	0.80	0.80	0.21	0.21	0.00	0.80	0.94	0.80	1.30	1.48	0.80	0.80	0.80
2680	0.80	0.80	0.80	0.80	0.80	1.05	1.24	1.42	1.61	1.85	0.80	0.80	0.64
2700	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.19	0.00	0.21
2720	0.00	0.00	0.00	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.00	0.00
2740	0.80	0.00	0.80	0.80	0.80	0.80	0.35	0.80	0.80	0.89	0.80	0.80	0.80
2760	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.83	1.01	1.20	0.80	0.80	0.80

Fig. 14c1

2780	0.80	0.80	0.80	0.80	0.80	0.80	0.76	0.95	1.14	1.32	1.51	0.80	0.80	0.80
2800	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
2820	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.28	0.80	0.80	0.80
2840	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.41	0.59	0.80	0.80	0.80
2860	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.35	0.54	0.72	0.91	0.80	0.80	0.80
2880	0.80	0.80	0.80	0.80	0.80	0.80	0.47	0.66	0.85	1.04	1.22	0.80	0.80	0.80
2900	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
2920	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
2940	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.12	0.30	0.80	0.80	0.80
2960	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.25	0.43	0.62	0.80	0.80	0.80
2980	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.37	0.56	0.75	0.93	0.80	0.80	0.80
3000	0.53	1.25	1.60	2.06	1.92	2.22	2.22	1.89	2.34	2.50	2.13	0.60	1.06	1.74
3020	0.80	1.10	1.26	1.42	2.11	2.33	2.41	2.41	2.38	2.45	2.50	0.80	1.15	1.32
3040	1.03	1.20	1.37	1.54	2.25	2.45	2.30	2.30	2.44	2.50	2.50	1.07	1.25	1.43
3060	1.11	1.30	1.49	1.70	2.50	2.16	2.42	2.42	2.50	2.50	2.50	1.15	1.35	1.54
3080	1.20	1.40	1.60	2.50	2.50	2.50	2.50	2.50	2.50	2.50	2.50	1.24	1.45	1.65
3100	0.16	0.50	0.85	1.00	1.31	1.39	1.96	1.96	1.60	1.74	1.88	0.15	0.31	0.58
3120	0.13	0.33	0.71	1.08	1.55	1.68	1.84	1.84	2.21	2.35	2.50	0.11	0.23	0.80
3140	0.80	0.80	1.14	1.32	1.90	1.68	1.94	1.94	2.21	2.34	2.50	0.80	0.80	1.20
3160	0.80	1.06	1.26	1.46	2.21	2.21	2.23	2.23	2.22	2.34	2.47	0.90	1.11	1.32
3180	0.94	1.16	1.38	2.38	2.39	2.50	2.45	2.45	2.50	2.50	2.47	0.98	1.21	1.44
3200	0.07	0.21	0.38	0.51	0.56	0.77	1.21	1.21	1.35	1.49	1.63	0.04	0.17	0.25
3220	0.06	0.22	0.42	0.47	0.74	0.97	1.36	1.36	1.78	2.28	2.50	0.06	0.29	0.59
3240	0.00	0.44	0.56	0.91	1.14	1.35	1.51	1.51	1.73	2.24	2.35	0.80	0.47	0.80
3260	0.80	0.80	1.02	1.22	1.91	1.74	2.11	2.11	2.01	2.17	2.38	0.80	0.80	1.08
3280	0.80	0.80	1.14	1.36	1.59	2.06	2.33	2.33	2.36	2.36	2.45	0.80	0.80	1.20
3300	0.05	0.13	0.13	0.28	0.30	0.80	0.95	0.95	1.09	1.23	1.37	0.08	0.02	0.21
3320	0.00	0.09	0.18	0.29	0.44	0.38	0.92	0.92	1.29	1.49	1.65	0.05	0.19	0.23

29 / 55

Fig. 14d

3340	0.14	0.15	0.37	0.47	0.57	0.63	1.07	1.35	1.85	2.43	0.20	0.06	0.37
3360	0.21	0.10	0.54	0.80	1.06	1.03	1.59	1.52	1.95	2.41	0.80	0.80	0.80
3380	0.80	0.80	0.80	1.12	1.35	2.07	1.94	2.17	2.22	2.36	0.80	0.80	0.96
3400	0.02	0.05	0.11	0.23	0.28	0.08	0.80	0.80	0.98	1.12	0.03	0.07	0.04
3420	0.01	0.05	0.11	0.13	0.20	0.25	0.34	0.80	1.24	1.40	0.08	0.08	0.16
3440	0.05	0.18	0.18	0.39	0.35	0.44	0.70	1.28	1.50	1.69	0.06	0.11	0.15
3460	0.13	0.10	0.28	0.63	0.61	0.77	1.04	1.33	1.46	2.31	0.00	0.25	0.26
3480	0.80	0.80	0.80	0.87	0.80	1.33	1.56	1.77	2.00	2.41	0.80	0.80	0.80
3500	0.05	0.02	0.18	0.10	0.24	0.14	0.23	0.80	0.80	0.87	0.01	0.01	0.07
3520	0.00	0.00	0.09	0.10	0.13	0.24	0.36	0.52	0.80	1.15	0.00	0.05	0.10
3540	0.00	0.06	0.13	0.14	0.20	0.34	0.44	0.71	1.25	1.44	0.00	0.04	0.06
3560	0.80	0.00	0.15	0.45	0.33	0.80	0.83	1.13	1.51	1.72	0.80	0.00	0.29
3580	0.80	0.80	0.80	0.80	0.85	1.09	1.32	1.55	1.77	2.28	0.80	0.80	0.80
3600	0.00	0.06	0.11	0.00	0.00	0.80	0.80	0.80	0.80	0.80	0.00	0.00	0.00
3620	0.00	0.00	0.09	0.06	0.03	0.11	0.16	0.21	0.80	0.90	0.00	0.03	0.09
3640	0.12	0.00	0.00	0.14	0.19	0.15	0.28	0.43	0.80	1.19	0.00	0.07	0.00
3660	0.00	0.09	0.00	0.29	0.18	0.38	0.58	0.49	1.27	1.48	0.80	0.00	0.13
3680	0.80	0.80	0.00	0.23	0.61	0.80	0.80	1.30	1.53	1.76	0.80	0.80	0.80
3700	0.00	0.80	0.00	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.00	0.14	0.14
3720	0.00	0.12	0.10	0.15	0.00	0.11	0.80	0.80	0.80	0.80	0.80	0.00	0.07
3740	0.00	0.34	0.07	0.00	0.15	0.23	0.14	0.80	0.80	0.94	0.80	0.00	0.00
3760	0.80	0.00	0.00	0.00	0.19	0.16	0.80	0.80	1.02	1.23	0.80	0.80	0.80
3780	0.80	0.80	0.80	0.80	0.16	0.00	0.82	1.05	1.28	1.51	0.80	0.80	0.80
3800	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
3820	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
3840	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.69	0.80	0.80	0.80
3860	0.80	0.80	0.80	0.80	0.80	0.23	0.80	0.80	0.77	0.98	0.80	0.80	0.80
3880	0.80	0.80	0.80	0.80	0.80	0.80	0.57	0.80	1.03	1.27	0.80	0.80	0.80

31 / 55

Fig. 14e

4480	0.80	0.21	0.17	0.34	0.80	0.78	1.64	1.54	1.90	2.13	0.80	0.80	0.80
4500	0.00	0.06	0.13	0.08	0.08	0.00	0.80	0.80	0.84	0.97	0.02	0.01	0.03
4520	0.00	0.03	0.06	0.10	0.17	0.23	0.52	0.64	1.03	1.19	0.00	0.01	0.06
4540	0.03	0.04	0.12	0.08	0.15	0.16	0.40	0.51	1.00	1.41	0.04	0.09	0.11
4560	0.00	0.11	0.03	0.16	0.31	0.30	0.71	0.90	1.01	1.63	0.00	0.00	0.11
4580	0.80	0.00	0.30	0.18	0.46	0.80	0.79	1.19	1.59	2.05	0.80	0.80	0.80
4600	0.02	0.00	0.20	0.17	0.00	0.80	0.80	0.80	0.80	0.74	0.00	0.05	0.04
4620	0.00	0.01	0.04	0.11	0.08	0.04	0.31	0.39	0.17	0.96	0.00	0.00	0.03
4640	0.00	0.00	0.06	0.06	0.15	0.12	0.18	0.19	0.80	1.17	0.07	0.00	0.08
4660	0.00	0.05	0.03	0.18	0.10	0.21	0.37	0.45	0.80	1.39	0.80	0.00	0.06
4680	0.80	0.00	0.00	0.07	0.29	0.48	0.60	0.76	1.18	1.61	0.80	0.80	0.80
4700	0.00	0.00	0.16	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.00	0.09	0.04
4720	0.00	0.00	0.00	0.03	0.00	0.15	0.12	0.80	0.80	0.72	0.00	0.00	0.00
4740	0.00	0.00	0.00	0.00	0.03	0.07	0.15	0.06	0.14	0.94	0.00	0.00	0.09
4760	0.00	0.00	0.00	0.00	0.09	0.23	0.13	0.39	0.37	1.16	0.80	0.00	0.18
4780	0.80	0.80	0.00	0.00	0.06	0.16	0.50	0.63	0.71	1.38	0.80	0.80	0.80
4800	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.17
4820	0.00	0.00	0.11	0.00	0.00	0.15	0.80	0.80	0.80	0.80	0.80	0.00	0.00
4840	0.80	0.00	0.00	0.00	0.09	0.10	0.00	0.00	0.80	0.80	0.80	0.80	0.00
4860	0.80	0.00	0.00	0.00	0.00	0.00	0.34	0.80	0.80	0.80	0.80	0.80	0.80
4880	0.80	0.80	0.80	0.80	0.18	0.10	0.15	0.80	0.80	1.14	0.80	0.80	0.80
4900	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
4920	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
4940	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.47	0.80	0.80	0.80
4960	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.27	0.48	0.69	0.80	0.80	0.80
4980	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.91	0.80	0.80	0.80
5000	0.59	1.02	2.01	2.30	2.35	2.19	2.41	2.50	1.99	2.13	0.80	1.02	1.19
5020	0.80	1.01	1.22	2.50	2.31	2.36	2.50	2.50	2.50	2.36	0.80	1.01	1.22

32 / 55

Fig. 14eI

5040	0.80	1.01	1.29	1.57	2.27	2.14	2.29	2.50	2.50	2.50	2.50	0.80	1.01	1.33
5060	0.80	1.01	1.36	1.71	2.07	2.50	2.50	2.50	2.50	2.50	2.50	0.80	1.01	1.40
5080	0.80	1.00	1.43	1.85	2.28	2.50	2.50	2.50	2.38	2.50	2.50	0.80	1.00	1.46
5100	0.20	0.94	1.19	1.11	1.25	1.39	2.28	1.67	2.50	1.94	2.50	0.08	0.39	0.80
5120	0.18	0.13	0.80	1.16	1.34	2.27	2.05	2.07	2.44	2.50	2.50	0.80	0.80	0.80
5140	0.80	0.80	0.80	1.21	1.43	1.65	1.88	2.33	2.50	2.50	2.50	0.80	0.80	0.99
5160	0.80	0.80	1.00	1.26	1.52	1.79	2.50	2.50	2.50	2.44	2.50	0.80	0.80	1.00
5180	0.80	0.80	1.01	1.31	1.61	1.92	2.32	2.50	2.50	2.50	2.50	0.80	0.80	1.01
5200	0.09	0.23	0.81	0.93	1.07	1.20	1.34	1.48	1.62	1.76	2.50	0.06	0.28	0.38
5220	0.00	0.12	0.31	0.80	1.12	1.29	1.46	1.63	2.43	2.50	2.50	0.08	0.28	0.49
5240	0.00	0.25	0.80	0.80	1.17	1.37	1.57	2.13	2.33	2.50	2.50	0.80	0.80	0.80
5260	0.80	0.80	0.80	0.99	0.80	1.45	1.69	2.13	2.35	2.36	2.50	0.80	0.80	0.75
5280	0.80	0.80	0.80	1.01	1.27	1.53	2.50	2.26	2.45	2.47	2.50	0.80	0.80	0.80
5300	0.06	0.21	0.50	0.80	0.80	1.02	1.16	1.30	1.44	1.58	2.50	0.03	0.21	0.20
5320	0.03	0.04	0.23	0.32	0.59	1.08	1.35	1.41	1.57	2.50	2.50	0.00	0.07	0.35
5340	0.00	0.22	0.32	0.36	0.78	0.72	1.33	1.52	2.22	2.44	2.44	0.00	0.00	0.14
5360	0.80	0.00	0.23	0.18	0.48	1.19	1.41	1.94	2.01	2.40	2.40	0.80	0.80	0.80
5380	0.80	0.80	0.80	0.76	1.01	1.25	1.50	2.10	2.18	2.41	2.41	0.80	0.80	0.80
5400	0.03	0.12	0.57	0.55	0.80	0.84	0.98	1.12	1.25	1.39	1.39	0.01	0.05	0.10
5420	0.00	0.05	0.17	0.17	0.40	0.50	0.73	1.20	1.37	1.53	1.53	0.00	0.00	0.08
5440	0.00	0.00	0.05	0.08	0.38	0.36	0.39	0.77	1.48	2.21	2.21	0.00	0.00	0.03
5460	0.00	0.00	0.11	0.30	0.31	0.37	0.90	1.13	1.73	2.41	2.41	0.80	0.15	0.15
5480	0.80	0.80	0.00	0.00	0.80	0.80	1.24	1.83	1.97	2.30	2.30	0.80	0.80	0.80
5500	0.01	0.02	0.21	0.33	0.80	0.80	0.79	0.93	1.07	1.21	1.21	0.00	0.02	0.07
5520	0.01	0.03	0.04	0.13	0.22	0.37	0.41	0.80	1.17	0.80	0.80	0.00	0.01	0.07
5540	0.03	0.00	0.05	0.12	0.26	0.23	0.31	0.60	1.26	2.26	2.26	0.00	0.03	0.06
5560	0.00	0.03	0.03	0.14	0.24	0.23	0.50	0.66	1.15	1.56	1.56	0.00	0.00	0.05
5580	0.80	0.00	0.00	0.23	0.24	0.54	0.81	1.03	1.53	2.05	2.05	0.80	0.80	0.00
5600	0.04	0.07	0.15	0.18	0.19	0.80	0.80	0.80	0.89	1.03	1.03	0.01	0.03	0.02

33 / 55

Fig. 14f

5620	0.00	0.01	0.07	0.11	0.14	0.13	0.36	0.80	0.97	1.13	0.00	0.01	0.07
5640	0.00	0.03	0.09	0.03	0.12	0.21	0.22	0.43	0.80	1.24	0.00	0.02	0.06
5660	0.00	0.00	0.06	0.07	0.07	0.19	0.24	0.63	0.82	1.34	0.00	0.00	0.00
5680	0.00	0.00	0.16	0.04	0.09	0.23	0.35	0.68	1.19	1.27	0.80	0.00	0.00
5700	0.05	0.16	0.00	0.19	0.23	0.80	0.80	0.80	0.80	0.84	0.00	0.00	0.05
5720	0.02	0.00	0.04	0.05	0.08	0.12	0.00	0.18	0.80	0.94	0.00	0.02	0.02
5740	0.00	0.02	0.02	0.02	0.05	0.13	0.06	0.22	0.80	1.03	0.00	0.06	0.00
5760	0.00	0.00	0.05	0.04	0.04	0.08	0.14	0.28	0.51	1.13	0.00	0.00	0.07
5780	0.00	0.00	0.08	0.09	0.07	0.19	0.19	0.44	0.67	1.22	0.80	0.00	0.00
5800	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.00	0.17	0.00
5820	0.00	0.00	0.04	0.12	0.07	0.28	0.00	0.00	0.80	0.80	0.00	0.00	0.00
5840	0.00	0.00	0.04	0.04	0.04	0.08	0.06	0.00	0.80	0.80	0.00	0.00	0.00
5860	0.00	0.00	0.00	0.12	0.07	0.11	0.10	0.00	0.80	0.92	0.80	0.00	0.00
5880	0.80	0.00	0.00	0.00	0.13	0.05	0.14	0.38	0.55	0.80	0.80	0.80	0.80
5900	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
5920	0.80	0.80	0.80	0.23	0.80	0.00	0.80	0.80	0.80	0.80	0.80	0.00	0.00
5940	0.80	0.80	0.80	0.00	0.00	0.00	0.00	0.80	0.80	0.80	0.80	0.80	0.80
5960	0.80	0.80	0.00	0.00	0.00	0.00	0.00	0.00	0.80	0.80	0.80	0.80	0.80
5980	0.80	0.80	0.80	0.80	0.80	0.18	0.09	0.80	0.80	0.80	0.80	0.80	0.80
6000	0.16	1.04	1.22	2.36	2.27	2.50	1.93	2.11	2.29	2.47	0.80	1.05	1.27
6020	0.80	1.06	1.31	2.27	1.80	2.05	2.50	2.50	2.50	2.50	0.80	1.07	1.36
6040	0.80	1.08	1.40	1.72	2.03	2.35	2.50	2.50	2.50	2.50	0.80	1.09	1.44
6060	0.80	1.10	1.49	1.87	2.26	2.50	2.50	2.50	2.50	2.50	0.80	1.12	1.53
6080	0.80	1.13	1.58	2.03	2.48	2.50	2.50	2.50	2.50	2.50	0.80	1.14	1.62
6100	0.19	0.80	1.04	1.22	2.16	1.58	1.76	2.32	2.50	2.50	0.24	0.80	1.05
6120	0.80	0.80	1.06	1.27	1.48	2.33	2.19	2.50	2.50	2.50	0.80	0.80	1.06
6140	0.80	0.80	1.07	1.31	1.55	1.79	2.03	2.50	2.50	2.50	0.80	0.80	1.08
6160	0.80	0.80	1.09	1.36	1.63	1.90	2.17	2.50	2.50	2.50	0.80	0.80	1.09

34 / 55

Fig. 14f1

6180	0.80	0.80	1.10	1.40	1.71	2.01	2.31	2.33	2.50	2.50	0.80	1.11
6200	0.19	0.55	0.87	1.04	1.22	2.38	2.32	1.76	1.94	2.11	0.80	0.80
6220	0.13	0.00	0.80	1.05	1.25	1.45	1.64	2.24	2.50	2.50	0.80	0.80
6240	0.80	0.80	0.80	1.06	1.28	1.49	1.71	1.92	2.50	2.50	0.80	0.80
6260	0.80	0.80	0.80	1.07	1.30	1.54	1.77	2.39	2.44	2.50	0.80	0.80
6280	0.80	0.80	0.80	1.07	1.33	1.58	2.50	2.09	2.46	2.50	0.80	0.80
6300	0.12	0.37	0.61	0.87	1.05	2.33	1.40	1.58	1.76	1.94	0.15	0.21
6320	0.04	0.04	0.04	0.80	0.80	1.24	1.43	2.29	2.34	2.50	0.00	0.29
6340	0.00	0.10	0.07	0.30	0.80	0.80	1.45	1.66	2.34	2.50	0.00	0.18
6360	0.80	0.00	0.16	0.80	0.80	1.26	1.48	1.69	2.30	2.50	0.80	0.80
6380	0.80	0.80	0.80	0.80	1.05	1.28	1.50	2.05	2.36	2.42	0.80	0.80
6400	0.04	0.47	0.80	0.69	0.87	1.05	1.22	1.40	1.58	1.76	0.01	0.08
6420	0.00	0.04	0.15	0.35	0.74	0.80	1.23	1.41	2.50	2.50	0.03	0.08
6440	0.00	0.04	0.03	0.25	0.38	0.56	0.80	1.43	1.62	2.50	0.00	0.06
6460	0.00	0.00	0.10	0.27	0.47	0.80	0.48	1.44	1.94	2.35	0.00	0.00
6480	0.80	0.80	0.80	0.80	0.81	0.80	1.24	1.45	2.07	2.47	0.80	0.80
6500	0.02	0.35	0.48	0.51	0.69	0.87	1.05	1.22	1.40	1.58	0.00	0.14
6520	0.00	0.02	0.00	0.08	0.17	0.49	0.80	1.22	1.40	2.50	0.00	0.02
6540	0.00	0.04	0.04	0.06	0.21	0.27	0.45	0.80	1.40	1.59	0.00	0.03
6560	0.00	0.00	0.00	0.10	0.28	0.29	0.45	0.73	1.40	2.31	0.00	0.00
6580	0.80	0.00	0.07	0.12	0.31	0.39	0.62	1.22	1.48	2.15	0.00	0.80
6600	0.02	0.05	0.80	0.80	0.51	0.80	0.87	1.05	1.23	1.40	0.00	0.08
6620	0.00	0.00	0.09	0.05	0.11	0.24	0.38	0.80	1.21	1.39	0.00	0.01
6640	0.00	0.00	0.00	0.04	0.05	0.10	0.18	0.56	1.20	1.38	0.00	0.04
6660	0.00	0.00	0.06	0.00	0.04	0.14	0.23	0.51	0.63	1.99	0.00	0.03
6680	0.00	0.00	0.04	0.00	0.10	0.26	0.27	0.58	0.98	1.84	0.80	0.00
6700	0.00	0.11	0.80	0.80	0.80	0.80	0.80	0.80	1.05	1.23	0.00	0.04
6720	0.00	0.03	0.00	0.09	0.02	0.07	0.30	0.80	1.02	1.20	0.00	0.02
6740	0.00	0.00	0.01	0.03	0.07	0.05	0.14	0.11	0.80	1.18	0.00	0.04

35 / 55

Fig. 14g

6760	0.00	0.00	0.02	0.03	0.04	0.09	0.15	0.26	0.64	1.16	0.00	0.00	0.00
6780	0.00	0.00	0.03	0.03	0.02	0.18	0.24	0.31	0.65	1.32	0.00	0.00	0.00
6800	0.00	0.00	0.80	0.80	0.80	0.80	0.80	0.80	0.80	1.05	0.00	0.04	0.05
6820	0.00	0.03	0.00	0.09	0.09	0.14	0.11	0.80	0.80	1.02	0.00	0.00	0.04
6840	0.00	0.00	0.00	0.02	0.02	0.07	0.12	0.11	0.80	0.99	0.00	0.00	0.02
6860	0.00	0.00	0.02	0.04	0.00	0.03	0.10	0.06	0.32	0.80	0.00	0.00	0.00
6880	0.80	0.00	0.00	0.00	0.03	0.14	0.09	0.17	0.21	0.70	0.80	0.80	0.00
6900	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80	0.80
6920	0.80	0.00	0.00	0.00	0.80	0.23	0.80	0.80	0.80	0.80	0.00	0.00	0.00
6940	0.80	0.13	0.00	0.00	0.00	0.00	0.09	0.80	0.80	0.80	0.80	0.00	0.00
6960	0.80	0.00	0.00	0.00	0.00	0.05	0.00	0.00	0.80	0.80	0.80	0.00	0.00
6980	0.80	0.80	0.00	0.00	0.00	0.12	0.06	0.13	0.15	0.72	0.80	0.80	0.80
7000	0.85	1.04	1.24	1.43	1.63	1.82	2.02	2.21	2.41	2.50	0.82	1.05	1.28
7020	0.79	1.06	1.32	1.59	1.86	2.12	2.39	2.50	2.50	2.50	0.76	1.06	1.37
7040	0.80	1.07	1.41	1.75	2.09	2.42	2.50	2.50	2.50	2.50	0.80	1.08	1.45
7060	0.80	1.09	1.50	1.90	2.31	2.50	2.50	2.50	2.50	2.50	0.80	1.09	1.54
7080	0.80	1.10	1.58	2.06	2.50	2.50	2.50	2.50	2.50	2.50	0.80	1.11	1.62
7100	0.33	0.88	1.08	1.27	1.47	2.50	1.86	2.05	2.25	2.44	0.80	0.80	1.08
7120	0.80	0.80	1.08	1.30	1.53	1.76	2.50	2.50	2.50	2.50	0.80	0.80	1.08
7140	0.80	0.80	1.08	1.34	1.59	1.85	2.50	2.50	2.50	2.50	0.80	0.80	1.08
7160	0.80	0.80	1.09	1.37	1.66	1.94	2.23	2.50	2.50	2.50	0.80	0.80	1.09
7180	0.80	0.80	1.09	1.40	1.72	2.04	2.35	2.50	2.50	2.50	0.80	0.80	1.09
7200	0.06	0.80	0.91	1.11	1.30	1.50	1.69	2.27	1.00	1.00	0.00	0.22	0.90
7220	0.80	0.80	0.89	1.10	1.31	2.38	2.27	2.50	2.50	2.50	0.80	0.80	0.80
7240	0.80	0.80	0.80	1.09	1.32	1.55	2.35	2.38	2.50	2.50	0.80	0.80	0.85
7260	0.80	0.80	0.84	1.09	1.33	1.58	1.82	2.06	2.50	2.46	0.80	0.80	0.83
7280	0.80	0.80	0.82	1.08	1.34	1.60	1.86	2.31	2.50	2.50	0.80	0.80	0.80
7300	0.08	0.18	0.75	0.95	1.14	1.34	1.53	1.73	1.92	2.12	0.04	0.16	0.16

36 / 55

Fig. 14g¹

7320	0.08	0.30	0.80	0.92	1.12	1.33	1.53	2.31	2.44	2.50	0.00	0.00	0.31
7340	0.00	0.14	0.80	0.89	1.10	1.32	1.53	2.25	2.18	2.50	0.80	0.80	0.80
7360	0.80	0.80	0.80	0.86	1.09	1.31	1.53	1.76	2.41	2.46	0.80	0.80	0.80
7380	0.80	0.80	0.80	0.83	1.07	1.30	1.53	2.38	2.24	2.48	0.80	0.80	0.80
7400	0.05	0.26	0.59	0.79	0.98	1.18	1.37	1.57	1.76	1.96	0.02	0.16	0.52
7420	0.00	0.04	0.16	0.45	0.80	1.15	1.35	2.30	2.23	2.50	0.00	0.05	0.09
7440	0.00	0.00	0.26	0.33	0.80	0.80	1.32	1.53	2.23	2.44	0.00	0.00	0.00
7460	0.00	0.00	0.00	0.80	0.80	0.80	1.30	1.51	2.27	2.41	0.80	0.80	0.80
7480	0.80	0.80	0.80	0.80	0.80	1.06	1.27	1.49	2.04	2.46	0.80	0.80	0.80
7500	0.06	0.43	0.80	0.80	0.82	1.01	1.21	1.40	1.60	1.79	0.01	0.04	0.10
7520	0.02	0.06	0.07	0.29	0.36	0.97	1.17	1.37	2.21	2.50	0.00	0.00	0.07
7540	0.00	0.06	0.05	0.21	0.19	0.45	0.69	1.33	2.11	2.43	0.00	0.00	0.00
7560	0.00	0.06	0.00	0.06	0.16	0.23	0.48	1.29	1.00	2.47	0.80	0.10	0.00
7580	0.80	0.00	0.00	0.00	0.09	0.80	0.80	1.25	1.70	2.36	0.80	0.80	0.80
7600	0.00	0.22	0.80	1.00	0.80	0.85	1.05	1.24	1.44	1.63	0.00	0.02	0.16
7620	0.00	0.04	0.04	0.22	0.11	0.58	0.54	1.19	2.36	2.50	0.01	0.00	0.03
7640	0.00	0.00	0.00	0.08	0.07	0.16	0.45	0.80	1.33	2.35	0.00	0.00	0.00
7660	0.00	0.00	0.04	0.06	0.05	0.11	0.16	0.48	1.28	2.32	0.00	0.00	0.00
7680	0.00	0.00	0.00	0.04	0.17	0.13	0.33	0.71	1.23	2.24	0.80	0.80	0.00
7700	0.00	0.13	0.00	0.80	0.49	0.69	0.88	1.08	1.27	1.47	0.00	0.00	0.06
7720	0.00	0.01	0.07	0.11	0.13	0.16	0.80	0.80	1.21	1.41	0.00	0.01	0.00
7740	0.00	0.00	0.02	0.00	0.06	0.21	0.37	0.31	0.80	1.34	0.00	0.00	0.01
7760	0.00	0.00	0.01	0.00	0.02	0.10	0.14	0.18	0.63	2.05	0.00	0.00	0.00
7780	0.00	0.00	0.03	0.02	0.02	0.11	0.20	0.31	0.57	1.60	0.80	0.00	0.00
7800	0.09	0.17	0.00	0.14	0.33	0.53	0.72	0.92	1.11	1.31	0.00	0.00	0.00
7820	0.00	0.00	0.00	0.05	0.05	0.14	0.80	0.85	1.04	1.23	0.00	0.01	0.00
7840	0.00	0.00	0.04	0.01	0.06	0.08	0.15	0.30	0.36	1.16	0.00	0.00	0.01
7860	0.00	0.00	0.00	0.01	0.02	0.05	0.10	0.10	0.30	1.09	0.00	0.00	0.00

Fig. 14h

[illegible]

38 / 55

Fig. 14h'

8460	0.80	0.80	0.80	0.80	0.95	1.18	2.29	2.32	2.32	2.50	0.80	0.80	0.80
8480	0.80	0.80	0.80	0.80	0.94	1.19	1.43	1.68	2.50	2.48	0.80	0.80	0.80
8500	0.00	0.09	0.80	0.63	0.82	1.02	1.22	1.42	1.62	1.82	0.00	0.00	0.06
8520	0.00	0.00	0.09	0.28	0.80	1.00	1.21	1.41	1.62	2.50	0.00	0.00	0.28
8540	0.00	0.00	0.10	0.11	0.38	0.19	1.20	1.41	2.31	2.50	0.00	0.00	0.10
8560	0.80	0.00	0.00	0.09	0.00	0.80	1.19	1.40	1.62	2.47	0.80	0.00	0.00
8580	0.80	0.80	0.80	0.80	0.80	0.80	1.17	1.40	1.62	2.42	0.80	0.80	0.80
8600	0.00	0.14	0.34	0.48	0.68	0.88	1.08	1.28	1.48	1.68	0.00	0.00	0.14
8620	0.00	0.02	0.03	0.00	0.16	0.47	1.05	1.25	2.50	2.50	0.02	0.02	0.06
8640	0.00	0.00	0.03	0.03	0.04	0.14	0.80	1.22	2.05	2.50	0.00	0.00	0.03
8660	0.00	0.00	0.00	0.09	0.11	0.18	0.16	0.80	1.40	2.37	0.00	0.00	0.00
8680	0.80	0.00	0.00	0.07	0.07	0.33	0.39	0.80	1.52	2.36	0.80	0.80	0.00
8700	0.00	0.00	0.00	0.80	0.54	0.74	0.94	1.14	1.34	1.53	0.00	0.00	0.06
8720	0.00	0.00	0.00	0.12	0.12	0.80	0.80	1.09	2.35	2.50	0.00	0.00	0.03
8740	0.00	0.00	0.00	0.02	0.02	0.15	0.41	0.65	1.24	2.50	0.00	0.00	0.00
8760	0.00	0.02	0.00	0.07	0.08	0.02	0.32	0.55	0.97	2.29	0.00	0.00	0.00
8780	0.00	0.00	0.03	0.05	0.10	0.08	0.15	0.32	0.75	2.28	0.80	0.00	0.00
8800	0.00	0.00	0.80	0.80	0.80	0.80	0.80	1.00	1.20	1.39	0.00	0.00	0.04
8820	0.00	0.00	0.00	0.03	0.00	0.33	0.80	0.94	1.13	1.33	0.00	0.00	0.00
8840	0.00	0.00	0.05	0.01	0.01	0.08	0.34	0.37	0.80	2.36	0.00	0.00	0.00
8860	0.00	0.00	0.00	0.03	0.03	0.04	0.04	0.14	0.58	2.18	0.00	0.00	0.00
8880	0.00	0.00	0.00	0.01	0.03	0.06	0.08	0.17	0.38	1.91	0.80	0.00	0.00
8900	0.00	0.80	0.80	0.80	0.26	0.46	0.66	0.86	1.05	1.25	0.00	0.00	0.00
8920	0.00	0.00	0.00	0.06	0.07	0.10	0.59	0.78	0.98	1.17	0.00	0.00	0.00
8940	0.00	0.00	0.01	0.00	0.02	0.00	0.06	0.21	0.80	1.09	0.00	0.00	0.00
8960	0.00	0.00	0.00	0.00	0.03	0.03	0.05	0.10	0.17	1.02	0.00	0.00	0.00
8980	0.00	0.00	0.00	0.00	0.01	0.04	0.02	0.04	0.15	1.10	0.80	0.00	0.00
9000	0.98	1.14	1.30	1.47	1.63	1.79	1.95	2.11	2.28	2.44	1.02	1.19	1.36
9020	1.06	1.24	1.41	1.59	1.76	1.94	2.11	2.29	2.46	2.50	1.10	1.28	1.46

39 / 55

Fig. 14i

9040	1.14	1.33	1.52	1.71	1.90	2.08	2.27	2.46	2.50	2.50	1.18	1.38	1.57
9060	1.22	1.42	1.62	1.83	2.03	2.23	2.43	2.50	2.50	2.50	1.26	1.47	1.68
9080	1.30	1.52	1.73	1.95	2.16	2.38	2.50	2.50	2.50	2.50	1.34	1.56	1.78
9100	0.75	0.91	1.07	1.24	1.40	1.56	1.72	1.88	2.05	2.21	0.79	0.96	1.12
9120	0.83	1.00	1.18	1.35	1.52	1.69	1.87	2.04	2.21	2.38	0.87	1.05	1.23
9140	0.91	1.09	1.28	1.46	1.64	1.83	2.01	2.19	2.38	2.50	0.95	1.14	1.33
9160	0.99	1.18	1.38	1.57	1.76	1.96	2.15	2.35	2.50	2.50	1.03	1.23	1.43
9180	1.07	1.27	1.48	1.68	1.89	2.09	2.30	2.50	2.50	2.50	1.11	1.32	1.53
9200	0.52	0.68	0.84	1.01	1.17	1.33	1.49	1.65	1.82	1.98	0.56	0.73	0.89
9220	0.60	0.77	0.94	1.12	1.29	1.46	1.63	1.80	1.97	2.15	0.64	0.82	0.99
9240	0.68	0.86	1.04	1.22	1.41	1.59	1.77	1.95	2.13	2.50	0.72	0.91	1.09
9260	0.76	0.95	1.14	1.33	1.52	1.71	1.91	2.10	2.29	2.50	0.80	1.00	1.19
9280	0.84	1.04	1.24	1.44	1.64	1.84	2.04	2.24	2.44	2.50	0.88	1.09	1.29
9300	0.29	0.45	0.61	0.78	0.94	1.10	1.26	1.42	1.59	1.75	0.33	0.50	0.66
9320	0.37	0.54	0.71	0.88	1.06	1.23	1.40	1.57	2.50	2.50	0.41	0.59	0.76
9340	0.45	0.63	0.81	0.99	1.17	1.35	1.53	1.71	2.33	2.50	0.49	0.68	0.86
9360	0.53	0.72	0.91	1.10	1.29	1.48	1.67	1.86	2.05	2.50	0.57	0.76	0.96
9380	0.61	0.81	1.01	1.21	1.40	1.60	1.80	2.00	2.20	2.50	0.65	0.85	1.06
9400	0.00	0.22	0.39	0.55	0.71	0.87	1.03	1.19	1.36	1.52	0.10	0.27	0.43
9420	0.14	0.31	0.48	0.65	0.82	1.00	1.17	1.34	2.50	2.50	0.18	0.36	0.53
9440	0.22	0.40	0.58	0.76	0.94	1.12	1.30	1.48	2.50	2.50	0.26	0.44	0.63
9460	0.30	0.49	0.68	0.87	1.05	1.24	1.43	1.62	1.81	2.45	0.34	0.53	0.73
9480	0.38	0.58	0.78	0.97	1.17	1.37	1.57	1.76	2.37	2.50	0.42	0.62	0.82
9500	0.00	0.15	0.16	0.32	0.48	0.64	0.80	0.97	1.13	1.29	0.00	0.13	0.20
9520	-0.09	0.08	0.25	0.42	0.59	0.76	0.94	1.11	1.28	1.45	0.00	0.00	0.00
9540	0.00	0.00	0.35	0.53	0.71	0.89	1.07	1.25	2.50	2.42	0.03	0.21	0.40
9560	0.07	0.26	0.45	0.63	0.82	1.01	1.20	1.39	2.32	2.50	0.11	0.30	0.50
9580	0.15	0.35	0.54	0.74	0.94	1.13	1.33	2.29	2.38	2.48	0.19	0.39	0.59
9600	0.00	-0.24	-0.07	0.09	0.25	0.41	0.57	0.74	0.90	1.06	0.00	0.00	0.00

Fig. 14i

9620	0.00	0.00	0.00	0.00	0.00	0.21	0.53	0.70	0.87	2.50	2.50	0.00	0.00	0.07
9640	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.84	1.01	2.13	2.44	0.00	0.00	0.00
9660	0.00	0.00	0.00	0.16	0.17	0.00	0.00	0.97	1.15	1.34	2.50	0.00	0.07	0.26
9680	0.00	0.12	0.31	0.00	0.00	0.00	0.00	1.10	1.29	1.49	2.46	0.00	0.16	0.36
9700	0.00	0.00	0.00	-0.14	0.02	0.18	0.34	0.34	0.51	0.67	0.83	0.00	0.00	0.00
9720	0.00	0.00	0.00	0.00	0.00	0.30	0.47	0.47	0.64	0.81	0.99	0.00	0.00	0.00
9740	0.00	0.00	0.00	0.00	0.00	0.16	0.28	0.28	0.78	2.13	2.50	0.00	0.00	0.00
9760	0.00	0.00	0.00	0.00	0.12	0.04	0.16	0.16	0.50	1.11	2.44	0.00	0.00	0.00
9780	0.80	0.00	0.00	0.00	0.06	0.04	0.19	0.19	0.40	1.19	2.44	0.00	0.00	0.13
9800	0.00	0.13	0.00	0.00	0.00	0.00	0.11	0.11	0.28	0.44	0.60	0.00	0.00	0.00
9820	0.00	0.00	0.04	0.00	0.00	0.21	0.17	0.17	0.41	0.58	0.75	0.00	0.00	0.00
9840	0.00	0.00	0.04	0.00	0.00	0.21	0.17	0.17	0.55	0.73	0.91	0.00	0.00	0.00
9860	0.00	0.00	0.00	0.00	0.03	0.04	0.10	0.10	0.11	0.65	2.35	0.00	0.00	0.00
9880	0.00	0.00	0.00	0.00	0.05	0.04	0.04	0.04	0.10	0.46	2.28	0.00	0.00	0.00
9900	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.05	0.21	0.37	0.00	0.00	0.00
9920	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.01	0.18	0.35	0.52	0.00	0.00	0.00
9940	0.00	0.00	0.01	0.01	0.03	0.02	0.03	0.03	0.26	0.50	0.68	0.00	0.00	0.00
9960	0.00	0.00	0.00	0.00	0.00	0.02	0.03	0.03	0.13	0.50	2.23	0.00	0.00	0.00
9980	0.00	0.00	0.00	0.01	0.01	0.01	0.03	0.03	0.07	0.16	1.94	0.00	0.00	0.00

41 / 55

Fig. 14j

13	14	15	16	17	18	19
2.14	1.97	2.08	2.26	2.42	2.43	2.50
2.39	2.37	2.39	2.34	2.41	2.45	2.50
2.46	2.48	2.50	2.49	2.45	2.49	2.50
2.50	2.50	2.47	2.49	2.48	2.49	2.50
2.50	2.50	2.50	2.50	2.50	2.50	2.50
0.95	0.97	1.15	1.63	1.97	2.32	2.50
1.85	2.06	1.94	2.18	2.21	2.39	2.41
2.40	2.29	2.46	2.34	2.45	2.42	2.50
2.47	2.44	2.43	2.45	2.49	2.47	2.49
2.50	2.50	2.50	2.50	2.48	2.50	2.50
0.62	0.48	0.58	0.80	1.60	2.35	2.50
1.04	1.28	1.52	1.76	1.96	2.03	2.50
1.85	2.19	2.29	2.11	2.21	2.30	2.50
2.20	2.43	2.39	2.45	2.37	2.48	2.48
2.50	2.50	2.50	2.50	2.47	2.49	2.50
0.18	0.24	0.36	1.17	1.35	1.52	1.69
0.80	1.23	1.37	1.52	1.66	1.80	1.94
1.53	1.64	2.02	1.86	2.43	2.33	2.50
1.97	2.50	2.39	2.46	2.39	2.44	2.55
2.41	2.46	2.50	2.50	2.45	2.50	2.50
0.12	0.00	0.80	0.80	1.01	1.18	1.36
0.80	0.80	0.80	1.19	1.33	1.48	1.62
1.20	1.32	1.43	1.55	1.66	1.78	1.89
1.65	2.50	2.41	2.42	2.44	2.26	2.50
2.10	2.15	2.21	2.26	2.50	2.50	2.50
0.80	0.80	0.80	0.80	0.80	0.80	1.01
0.80	0.80	0.80	0.80	1.00	1.15	1.30
0.80	0.80	1.11	1.22	1.34	1.46	1.58
1.32	1.41	2.50	2.29	2.27	1.78	1.87
1.77	1.83	1.90	1.96	2.50	2.40	2.50
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	1.02	1.14	1.26
0.80	1.08	1.17	1.27	1.37	1.46	1.56
1.44	1.51	1.58	1.64	1.71	1.78	1.85
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80

42 / 55

Fig. 14j¹

0.80	0.80	0.80	0.80	1.04	1.14	1.24
1.10	1.17	1.25	1.32	1.39	1.47	1.54
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	1.07	1.14	1.22
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
2.05	2.04	2.17	2.25	2.36	2.41	2.50
2.05	2.31	2.32	2.40	2.45	2.41	2.50
2.38	2.38	2.50	2.50	2.44	2.46	2.48
2.41	2.50	2.46	2.50	2.47	2.49	2.48
2.50	2.50	2.50	2.50	2.50	2.50	2.50
0.85	1.22	1.17	1.64	2.13	2.39	2.30
1.72	1.79	2.10	1.98	2.19	2.37	2.50
2.15	2.17	2.25	2.35	2.43	2.36	2.45
2.39	2.42	2.43	2.45	2.45	2.47	2.49
2.50	2.39	2.43	2.50	2.50	2.50	2.50
0.53	0.56	0.80	1.19	1.37	1.83	2.01
1.11	1.18	1.51	1.51	1.74	2.12	2.50
1.67	1.83	2.15	2.08	2.15	2.21	2.47
2.11	2.28	2.25	2.32	2.36	2.30	2.48
2.41	2.49	2.40	2.50	2.48	2.49	2.49
0.16	0.56	0.63	0.80	1.33	1.52	1.71
0.65	0.67	1.12	1.18	1.83	2.07	2.31
1.00	1.00	1.66	1.74	1.98	2.16	2.50
1.74	1.96	2.13	2.18	2.26	2.31	2.37
2.13	2.50	2.43	2.46	2.48	2.49	2.47
0.26	0.18	0.40	0.80	0.80	1.21	1.40
0.80	0.46	0.80	0.80	1.34	1.51	1.68
0.80	1.20	1.35	1.51	1.66	2.02	2.26
1.45	1.58	1.90	1.91	1.99	2.14	2.50
1.84	1.96	2.26	2.20	2.43	2.50	2.47

43 / 55

Fig. 14k

0.20	0.11	0.00	0.80	0.80	0.90	1.09
0.32	0.80	0.13	0.80	1.04	1.21	1.38
0.19	0.80	1.05	1.21	1.36	1.52	1.67
0.80	1.28	1.42	2.25	2.20	2.20	2.27
1.55	1.66	1.78	1.90	2.50	2.43	2.33
0.00	0.80	0.80	0.80	0.80	0.80	0.80
0.19	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	1.06	1.22	1.38
0.80	0.98	1.12	1.26	1.40	1.54	1.68
1.24	1.36	1.49	1.61	1.73	2.50	2.50
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.60	0.76	0.80	0.80
0.80	0.80	0.81	0.96	1.10	1.24	1.38
0.93	1.06	1.19	1.31	1.44	1.56	1.69
0.80	0.80	0.80	0.80	0.80	0.00	0.15
0.80	0.80	0.80	0.80	0.80	0.28	0.46
0.80	0.80	0.80	0.80	0.45	0.61	0.77
0.80	0.80	0.80	0.80	0.79	0.94	1.08
0.80	0.80	0.88	1.01	1.14	1.27	1.40
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.14	0.30	0.46
0.80	0.05	0.20	0.34	0.49	0.63	0.78
0.31	0.44	0.57	0.70	0.84	0.97	1.10
1.95	1.95	2.01	2.10	2.31	2.41	2.50
2.22	2.23	2.32	2.35	2.41	2.47	2.50
2.33	2.46	2.50	2.50	2.44	2.50	2.50
2.50	2.45	2.46	2.50	2.50	2.47	2.50
2.32	2.50	2.50	2.50	2.45	2.50	2.50
1.00	1.19	1.47	1.51	1.88	2.21	2.50
1.12	1.50	1.92	1.95	2.16	2.42	2.50
2.18	2.26	2.19	2.23	2.40	2.41	2.47
2.38	2.33	2.32	2.40	2.46	2.42	2.48
2.50	2.50	2.43	2.50	2.47	2.48	2.49
0.49	0.74	0.82	1.24	1.63	1.72	2.50
0.90	0.86	1.39	1.53	1.67	2.21	2.50

44 / 55

Fig. 14k^l

1.39	1.65	1.92	2.03	1.99	2.26	2.47
1.68	2.24	2.33	2.33	2.28	2.36	2.42
1.96	2.23	2.44	2.35	2.48	2.47	2.50
0.23	0.36	0.41	1.06	1.25	1.43	1.60
0.39	0.66	0.82	0.90	1.52	1.91	2.50
0.74	1.31	1.50	1.61	1.73	2.12	2.40
1.41	1.58	1.89	2.16	2.07	2.21	2.47
1.69	1.86	2.24	2.42	2.42	2.48	2.50
0.06	0.17	0.26	0.41	0.80	0.80	1.31
0.29	0.36	0.60	0.79	1.02	1.43	1.60
0.63	0.71	1.34	0.99	1.54	1.83	2.30
0.80	1.30	1.48	1.34	2.02	1.85	2.38
1.41	1.59	1.77	2.40	2.36	2.46	2.48
0.06	0.18	0.22	0.17	0.80	0.80	1.00
0.14	0.12	0.33	0.50	0.80	1.14	1.31
0.25	0.80	0.80	0.80	1.26	1.44	1.65
0.80	1.01	1.19	1.37	1.56	1.74	1.92
1.12	1.30	1.49	2.14	2.23	2.35	2.46
0.07	0.00	0.80	0.80	0.80	0.80	0.71
0.09	0.00	0.80	0.80	0.80	0.84	1.02
0.12	0.80	0.13	0.80	0.97	0.80	1.33
0.80	0.80	0.80	0.34	1.27	1.46	1.64
0.80	1.02	1.20	1.39	1.57	2.39	2.21
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.00	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.86	1.04
0.80	0.80	0.80	0.80	0.98	1.17	1.35
0.80	0.80	0.91	1.10	2.27	2.37	2.36
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.26	0.43
0.80	0.80	0.80	0.80	0.39	0.57	0.75
0.80	0.80	0.32	0.51	0.69	0.88	1.07
0.24	0.43	0.62	0.81	1.00	1.19	1.38
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.14
0.80	0.80	0.80	0.80	0.09	0.27	0.46
0.80	0.80	0.80	0.21	0.40	0.59	0.78

45 / 55

Fig. 14l

0.80	0.14	0.33	0.52	0.71	0.90	1.09
1.94	2.19	2.03	2.36	2.31	2.41	2.50
1.48	2.14	2.06	2.34	2.45	2.44	2.50
2.31	2.50	2.41	2.50	2.50	2.50	2.50
1.74	2.50	2.12	2.50	2.44	2.50	2.50
1.86	2.07	2.28	2.50	2.50	2.50	2.50
1.10	1.21	1.58	1.80	2.05	2.37	2.01
1.25	1.33	1.83	2.10	2.01	2.36	2.50
1.39	1.58	2.01	2.02	2.24	2.42	2.44
1.53	2.25	2.37	2.32	2.40	2.40	2.50
1.67	1.90	2.50	2.44	2.43	2.48	2.50
0.50	0.85	0.76	1.31	1.77	2.12	1.76
0.71	0.83	0.98	1.43	1.94	2.19	2.40
0.80	1.34	1.50	1.94	2.14	2.08	2.50
1.29	1.51	2.23	1.96	2.33	2.21	2.48
1.44	1.67	2.50	2.29	2.42	2.45	2.48
0.25	0.30	0.51	0.78	1.21	1.36	1.51
0.33	0.58	0.65	1.27	1.31	1.84	2.50
0.55	1.02	0.95	1.02	1.72	2.06	2.27
1.05	1.26	1.25	1.81	1.96	2.11	2.47
1.19	1.43	2.14	2.33	2.38	2.43	2.45
0.07	0.19	0.30	0.52	0.80	1.11	1.26
0.17	0.37	0.46	0.60	0.92	1.37	1.54
0.51	0.58	0.86	0.96	1.27	1.63	2.35
0.55	0.80	1.00	1.40	1.40	1.69	2.34
0.95	1.19	2.21	2.25	2.31	2.39	2.44
0.14	0.15	0.12	0.23	0.80	0.86	1.01
0.18	0.09	0.34	0.25	0.80	0.80	1.30
0.24	0.15	0.39	0.62	0.87	1.38	2.31
0.18	0.33	0.87	1.21	1.09	1.71	1.86
0.80	0.94	1.18	1.89	2.05	2.28	2.28
0.12	0.15	0.13	0.21	0.80	0.80	0.80
0.00	0.12	0.29	0.07	0.34	0.00	1.05
0.05	0.16	0.52	0.61	0.80	0.80	1.33
0.28	0.80	0.80	0.80	1.18	1.40	1.62
0.80	0.80	0.93	1.18	1.42	2.36	2.34
0.23	0.15	0.00	0.80	0.80	0.80	0.80

46 / 55

Fig. 14l¹

0.00	0.08	0.80	0.10	0.80	0.80	0.81
0.21	0.07	0.26	0.10	0.80	0.89	1.08
0.17	0.13	0.80	0.80	0.80	1.15	1.37
0.80	0.80	0.80	0.93	1.17	2.13	1.66
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.64	0.83
0.80	0.80	0.23	0.80	0.68	0.90	1.12
0.80	0.80	0.80	0.68	0.92	1.17	1.41
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.38	0.58
0.80	0.80	0.80	0.80	0.43	0.65	0.87
0.80	0.80	0.80	0.43	0.67	0.92	1.16
2.35	2.20	2.30	2.50	2.28	2.50	2.25
1.44	1.61	1.79	2.50	2.28	2.50	2.50
1.51	1.71	2.31	2.50	2.32	2.50	2.50
1.58	1.81	2.03	2.26	2.49	2.50	2.50
1.65	1.90	2.16	2.50	2.50	2.40	2.50
0.80	1.50	1.43	1.90	2.17	2.50	2.50
1.20	1.38	1.55	2.03	2.33	2.46	2.50
1.27	1.47	1.67	2.20	2.38	2.41	2.44
1.34	1.56	2.14	2.34	2.50	2.45	2.46
1.41	1.66	2.50	2.50	2.42	2.50	2.50
0.56	0.97	1.30	1.72	1.49	1.63	1.78
0.69	0.90	1.14	1.31	1.88	2.41	2.50
0.80	1.23	1.43	1.63	1.88	2.20	2.46
1.10	1.33	1.55	1.99	2.15	2.43	2.47
1.17	1.42	2.20	2.50	2.47	2.50	2.48
0.26	0.48	0.71	0.80	1.25	2.39	1.55
0.29	0.46	0.59	0.94	1.51	1.79	2.29
0.55	0.57	0.96	1.20	1.51	1.87	2.33
0.37	1.09	1.32	1.87	1.63	1.87	2.30
0.94	1.19	2.12	2.14	2.41	2.48	2.46
0.23	0.28	0.60	0.64	0.80	1.17	0.80
0.24	0.23	0.36	0.72	0.71	1.36	2.31
0.28	0.42	0.49	0.62	1.11	1.45	2.17

47 / 55

Fig. 14m

0.44	0.59	0.88	1.15	1.38	1.46	2.31
0.80	0.95	2.14	1.45	2.26	2.32	2.39
0.05	0.07	0.28	0.29	0.80	0.93	1.08
0.10	0.17	0.27	0.41	0.47	0.80	1.30
0.15	0.21	0.21	0.36	0.75	1.32	1.52
0.21	0.25	0.39	0.47	0.90	1.14	1.83
0.80	0.72	0.96	2.04	1.82	2.26	2.31
0.05	0.00	0.28	0.09	0.80	0.70	0.85
0.09	0.08	0.17	0.25	0.37	0.80	1.06
0.03	0.05	0.21	0.27	0.36	0.51	1.28
0.09	0.27	0.27	0.36	0.70	1.28	1.50
0.00	0.33	0.80	0.98	1.83	2.00	2.13
0.09	0.17	0.25	0.21	0.80	0.80	0.80
0.06	0.03	0.06	0.07	0.29	0.80	0.83
0.04	0.09	0.13	0.15	0.24	0.32	1.05
0.00	0.27	0.19	0.23	0.44	0.37	1.27
0.80	0.18	0.50	0.74	0.99	1.96	2.12
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.20	0.00	0.00	0.19	0.80	0.80	0.80
0.00	0.00	0.80	0.26	0.00	0.23	0.80
0.16	0.00	0.20	0.09	0.80	0.80	0.80
0.80	0.80	0.80	0.51	0.76	1.00	1.25
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.58
0.80	0.80	0.80	0.80	0.80	0.58	0.80
0.80	0.80	0.80	0.80	0.52	0.77	1.02
1.36	2.50	1.71	2.38	2.50	2.50	2.41
1.43	2.50	2.50	2.31	2.29	2.50	2.50
1.64	1.96	2.28	2.60	2.50	2.50	2.50
1.78	2.17	2.50	2.50	2.50	2.50	2.50
1.92	2.38	2.50	2.50	2.50	2.50	2.50
1.14	1.30	2.06	1.61	2.43	2.50	2.09
1.19	1.39	1.59	1.79	2.25	2.50	2.37
1.24	1.48	1.72	1.96	2.33	2.43	2.50
1.28	1.57	1.85	2.34	2.50	2.41	2.50
1.33	1.66	1.99	2.31	2.50	2.50	2.50

48 / 55

Fig. 14m^l

1.04	1.33	1.25	1.40	2.24	2.38	1.86
0.80	1.14	1.33	1.51	2.01	2.19	2.50
0.80	1.19	1.41	1.63	2.08	2.22	2.45
1.00	1.24	1.49	2.06	2.08	2.40	2.50
1.02	1.30	1.58	2.34	2.45	2.50	2.48
0.46	0.82	1.05	1.20	1.35	1.51	1.66
0.50	0.50	0.62	1.05	1.46	2.03	2.40
0.46	0.80	0.80	1.37	1.56	1.94	2.31
0.80	0.80	1.22	1.45	1.96	2.08	2.43
0.76	1.02	2.29	1.54	2.25	2.40	2.50
0.29	0.36	0.49	0.80	1.16	1.31	1.46
0.27	0.23	0.44	0.50	1.25	1.42	2.38
0.36	0.37	0.42	0.58	0.92	1.54	2.27
0.06	0.48	0.60	0.83	1.35	1.52	2.33
0.80	0.78	1.03	2.07	2.26	2.28	2.36
0.15	0.15	0.48	0.80	0.80	1.12	1.27
0.13	0.23	0.13	0.32	0.39	1.00	1.39
0.15	0.15	0.26	0.38	0.56	0.97	2.02
0.12	0.33	0.43	0.63	0.87	1.16	1.93
0.00	0.80	0.80	1.03	1.84	2.17	2.08
0.13	0.06	0.22	0.80	0.78	0.93	1.08
0.04	0.14	0.19	0.27	0.15	0.80	1.18
0.05	0.08	0.16	0.29	0.43	0.67	1.29
0.07	0.08	0.15	0.35	0.58	0.75	1.88
0.10	0.80	0.47	0.81	1.43	1.67	1.98
0.08	0.23	0.22	0.80	0.80	0.80	0.89
0.03	0.09	0.03	0.10	0.16	0.80	0.99
0.00	0.00	0.06	0.14	0.32	0.80	1.08
0.08	0.07	0.08	0.19	0.38	0.35	1.18
0.00	0.21	0.35	0.61	1.29	1.26	1.89
0.00	0.80	0.00	0.80	0.80	0.80	0.80
0.08	0.04	0.00	0.17	0.00	0.80	0.80
0.00	0.08	0.06	0.09	0.00	0.36	0.80
0.04	0.04	0.10	0.04	0.23	0.25	0.15
0.00	0.80	0.20	0.80	0.61	1.47	1.94
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.80	0.80	0.80	0.80	0.80	0.80	0.80

Fig. 14n

0.80	0.15	0.18	0.80	0.00	0.80	0.80
0.80	0.00	0.00	0.00	0.00	0.80	0.80
0.80	0.80	0.80	0.19	0.41	0.80	2.01
1.48	2.50	1.90	2.50	2.50	2.50	2.50
1.64	1.92	2.20	2.48	2.50	2.50	2.50
1.79	2.14	2.49	2.50	2.50	2.50	2.50
1.95	2.37	2.50	2.50	2.50	2.50	2.50
2.11	2.50	2.50	2.50	2.50	2.50	2.50
1.24	1.44	2.50	2.40	2.50	2.50	2.41
1.29	1.51	2.38	1.60	2.36	2.50	2.41
1.33	1.59	2.27	2.10	2.50	2.50	2.50
1.38	1.67	1.95	2.24	2.50	2.50	2.50
1.43	1.74	2.06	2.38	2.50	2.42	2.50
1.05	1.24	2.03	2.16	2.22	2.40	2.17
1.06	1.26	1.47	2.31	2.40	2.50	2.50
1.06	1.29	1.51	1.74	2.31	2.50	2.44
1.07	1.31	1.56	1.80	2.31	2.50	2.50
1.08	1.34	1.60	2.50	2.40	2.46	2.50
0.71	1.05	1.23	1.41	2.21	2.38	1.97
0.80	0.80	1.24	1.44	1.64	2.23	2.50
0.80	0.80	1.26	1.47	1.68	2.18	2.41
0.80	1.05	1.27	1.49	2.33	2.22	2.50
0.80	1.05	1.28	2.50	2.45	2.39	2.50
0.46	0.80	1.04	1.23	1.41	2.50	1.80
0.12	0.63	0.53	0.80	1.42	2.18	2.39
0.24	0.28	0.56	1.23	1.43	1.93	2.42
0.35	0.23	1.03	0.80	1.65	1.86	2.47
0.80	0.80	1.02	1.24	2.37	2.39	2.39
0.25	0.80	0.80	1.04	1.22	1.40	1.58
0.09	0.25	0.53	0.48	0.80	1.40	2.50
0.03	0.14	0.25	0.47	0.58	1.45	2.24
0.06	0.18	0.41	0.56	0.77	1.34	2.23
0.80	0.80	0.80	1.23	2.07	2.08	2.34
0.07	0.13	0.36	0.80	0.80	1.22	1.40
0.06	0.14	0.25	0.28	0.45	1.20	1.39
0.14	0.07	0.15	0.21	0.42	0.93	2.02
0.07	0.07	0.23	0.42	0.39	0.87	1.92

50 / 55

Fig. 14n¹

0.00	0.38	0.29	0.78	1.29	1.43	2.18
0.11	0.13	0.00	0.34	0.80	1.04	1.21
0.00	0.06	0.04	0.29	0.38	1.01	1.19
0.05	0.00	0.17	0.19	0.21	0.39	1.17
0.00	0.05	0.12	0.10	0.32	0.38	1.00
0.00	0.13	0.28	0.54	0.98	1.01	1.82
0.00	0.00	0.00	0.80	0.80	0.80	1.03
0.02	0.05	0.05	0.00	0.80	0.80	1.00
0.03	0.04	0.05	0.02	0.32	0.00	0.80
0.12	0.03	0.03	0.11	0.09	0.20	0.80
0.12	0.17	0.26	0.27	0.59	1.04	1.65
0.80	0.80	0.80	0.80	0.80	0.80	0.80
0.00	0.00	0.00	0.10	0.80	0.80	0.80
0.04	0.00	0.00	0.00	0.00	0.00	0.80
0.00	0.00	0.04	0.00	0.12	0.07	0.73
0.80	0.80	0.00	0.80	0.80	1.25	1.77
1.51	1.74	1.97	2.20	2.44	2.50	2.50
1.67	1.97	2.27	2.50	2.50	2.50	2.50
1.83	2.20	2.50	2.50	2.50	2.50	2.50
1.98	2.43	2.50	2.50	2.50	2.50	2.50
2.14	2.50	2.50	2.50	2.50	2.50	2.50
1.29	1.50	1.71	1.92	2.50	2.50	2.50
1.32	1.56	1.80	2.50	2.50	2.50	2.50
1.35	1.63	1.90	2.50	2.50	2.50	2.50
1.39	1.69	1.99	2.29	2.50	2.50	2.50
1.42	1.75	2.08	2.42	2.50	2.50	2.50
1.11	1.31	1.51	1.72	2.50	2.31	2.50
0.80	1.32	1.54	1.76	2.33	2.50	2.50
1.09	1.33	1.56	1.80	2.04	2.50	2.50
1.08	1.33	1.59	1.84	2.09	2.50	2.50
1.07	1.34	1.61	1.88	2.26	2.50	2.50
0.93	1.13	1.33	1.53	2.50	2.50	2.50
0.80	1.11	1.32	1.53	2.35	2.43	2.50
0.80	0.80	1.31	1.53	2.24	2.50	2.50
0.85	1.08	1.31	1.53	1.76	2.37	2.50
0.82	1.06	1.30	2.27	2.50	2.46	2.48
0.53	0.96	1.16	1.36	2.32	2.50	2.50

51 / 55

Fig. 14o

0.21	0.80	1.13	1.33	1.54	2.39	2.41
0.19	0.29	0.80	1.31	1.52	2.24	2.50
0.80	0.33	1.07	1.29	1.50	2.01	2.44
0.80	0.82	1.04	2.33	2.35	2.32	2.47
0.38	0.80	0.99	1.19	1.38	2.32	2.50
0.07	0.09	0.65	1.15	1.35	2.31	2.50
0.04	0.22	0.23	0.60	1.31	1.51	2.35
0.07	0.35	0.35	0.38	1.27	2.02	2.33
0.80	0.80	1.03	1.23	1.96	2.17	2.44
0.08	0.80	0.82	1.02	1.22	1.41	1.61
0.11	0.25	0.16	0.44	0.80	1.36	1.56
0.05	0.07	0.22	0.24	0.80	1.31	2.15
0.03	0.14	0.07	0.36	0.56	1.05	2.09
0.00	0.09	0.37	0.80	1.01	1.70	2.34
0.12	0.80	0.80	0.85	1.05	1.24	1.44
0.14	0.08	0.08	0.38	0.80	1.18	1.37
0.04	0.08	0.10	0.22	0.28	1.12	2.50
0.01	0.03	0.05	0.21	0.21	0.51	1.88
0.00	0.04	0.19	0.37	0.83	1.12	1.99
0.18	0.80	0.80	0.69	0.88	1.08	1.27
0.04	0.08	0.06	0.05	0.80	0.80	1.20
0.01	0.01	0.02	0.07	0.29	0.42	1.12
0.02	0.01	0.01	0.06	0.16	0.25	1.38
0.00	0.03	0.03	0.18	0.35	0.53	1.86
0.80	0.80	0.80	0.80	0.80	0.91	1.10
0.00	0.05	0.05	0.22	0.80	0.80	1.02
0.05	0.00	0.04	0.11	0.04	0.34	0.94
0.02	0.02	0.05	0.02	0.05	0.09	0.80
0.11	0.00	0.04	0.21	0.21	0.74	1.60
1.50	1.76	2.02	2.28	2.50	2.50	2.50
1.83	2.22	2.50	2.50	2.50	2.50	2.50
2.16	2.68	2.50	2.50	2.50	2.50	2.50
2.50	2.50	2.50	2.50	2.50	2.50	2.50
2.50	2.50	2.50	2.50	2.50	2.50	2.50
1.25	1.47	1.70	1.92	2.15	2.38	2.50
1.36	1.64	1.92	2.20	2.49	2.50	2.50
1.48	1.81	2.15	2.49	2.50	2.50	2.50

52 / 55

Fig. 14o^l

1.59	1.98	2.37	2.50	2.50	2.50	2.38
1.70	2.15	2.50	2.50	2.50	2.50	2.50
1.07	1.28	1.50	2.50	2.50	2.50	2.50
1.11	1.36	1.60	1.85	2.09	2.50	2.50
1.15	1.43	1.70	1.98	2.26	2.40	2.50
1.19	1.50	1.81	2.11	2.42	2.50	2.50
1.24	1.57	1.91	2.25	2.50	2.50	2.50
0.91	1.12	2.29	2.27	2.50	2.50	2.50
0.91	1.14	1.37	1.59	2.31	2.50	2.50
0.80	1.17	1.41	1.66	2.33	2.50	2.50
0.80	1.19	1.45	1.72	2.50	2.38	2.46
0.80	1.21	1.50	1.78	2.06	2.50	2.50
0.80	0.96	1.17	2.36	2.40	2.50	2.50
0.80	0.96	1.17	1.39	2.29	2.43	2.42
0.80	0.80	0.80	2.27	2.40	2.50	2.46
0.80	0.95	1.18	1.42	1.66	2.42	2.50
0.80	0.94	1.19	1.44	2.29	2.44	2.48
0.80	0.81	1.01	1.22	1.42	1.62	1.82
0.80	0.09	1.00	1.20	1.41	2.26	2.50
0.19	0.00	0.80	1.19	1.41	2.43	2.50
0.80	0.23	0.80	0.80	1.40	1.62	2.45
0.80	0.71	0.94	1.17	2.22	2.31	2.43
0.30	0.80	0.86	1.06	1.26	1.46	1.66
0.08	0.11	0.27	0.80	1.23	2.50	2.50
0.04	0.17	0.04	0.29	1.21	1.41	2.43
0.16	0.14	0.28	0.29	0.80	1.39	2.43
0.00	0.00	0.80	0.93	1.15	1.94	2.44
0.29	0.80	0.72	0.92	1.11	1.31	1.51
0.00	0.00	0.15	0.80	0.80	1.27	2.50
0.03	0.09	0.03	0.21	0.44	1.22	2.33
0.02	0.02	0.10	0.29	0.17	0.77	2.29
0.00	0.04	0.12	0.38	0.90	1.17	2.34
0.24	0.10	0.80	0.80	0.97	1.16	1.36
0.00	0.08	0.10	0.36	0.80	1.10	1.30
0.01	0.01	0.09	0.18	0.14	0.80	2.39
0.01	0.05	0.01	0.10	0.18	0.42	2.02
0.00	0.02	0.06	0.24	0.33	0.64	2.04

53 / 55

Fig. 14p

1.59	1.98	2.37	2.50	2.50	2.50	2.38
1.70	2.15	2.50	2.50	2.50	2.50	2.50
1.07	1.28	1.50	2.50	2.50	2.50	2.50
1.11	1.36	1.60	1.85	2.09	2.50	2.50
1.15	1.43	1.70	1.98	2.26	2.40	2.50
1.19	1.50	1.81	2.11	2.42	2.50	2.50
1.24	1.57	1.91	2.25	2.50	2.50	2.50
0.91	1.12	2.29	2.27	2.50	2.50	2.50
0.91	1.14	1.37	1.59	2.31	2.50	2.50
0.80	1.17	1.41	1.66	2.33	2.50	2.50
0.80	1.19	1.45	1.72	2.50	2.38	2.46
0.80	1.21	1.50	1.78	2.06	2.50	2.50
0.80	0.96	1.17	2.36	2.40	2.50	2.50
0.80	0.96	1.17	1.39	2.29	2.43	2.42
0.80	0.80	0.80	2.27	2.40	2.50	2.46
0.80	0.95	1.18	1.42	1.66	2.42	2.50
0.80	0.94	1.19	1.44	2.29	2.44	2.48
0.80	0.81	1.01	1.22	1.42	1.62	1.82
0.80	0.09	1.00	1.20	1.41	2.26	2.50
0.19	0.00	0.80	1.19	1.41	2.43	2.50
0.80	0.23	0.80	0.80	1.40	1.62	2.45
0.80	0.71	0.94	1.17	2.22	2.31	2.43
0.30	0.80	0.86	1.06	1.26	1.46	1.66
0.08	0.11	0.27	0.80	1.23	2.50	2.50
0.04	0.17	0.04	0.29	1.21	1.41	2.43
0.16	0.14	0.28	0.29	0.80	1.39	2.43
0.00	0.00	0.80	0.93	1.15	1.94	2.44
0.29	0.80	0.72	0.92	1.11	1.31	1.51
0.00	0.00	0.15	0.80	0.80	1.27	2.50
0.03	0.09	0.03	0.21	0.44	1.22	2.33
0.02	0.02	0.10	0.29	0.17	0.77	2.29
0.00	0.04	0.12	0.38	0.90	1.17	2.34
0.24	0.10	0.80	0.80	0.97	1.16	1.36
0.00	0.08	0.10	0.36	0.80	1.10	1.30
0.01	0.01	0.09	0.18	0.14	0.80	2.39
0.01	0.05	0.01	0.10	0.18	0.42	2.02
0.00	0.02	0.06	0.24	0.33	0.64	2.04

54 / 55

Fig. 14p¹

0.00	0.80	0.43	0.62	0.82	1.02	1.21
0.03	0.09	0.05	0.00	0.80	0.94	1.13
0.01	0.05	0.02	0.03	0.16	0.40	1.05
0.00	0.02	0.01	0.04	0.08	0.20	1.42
0.00	0.02	0.03	0.08	0.22	0.39	1.61
1.53	1.69	1.86	2.03	2.20	2.37	2.50
1.65	1.83	2.01	2.19	2.37	2.50	2.50
1.77	1.96	2.16	2.35	2.50	2.50	2.50
1.89	2.10	2.30	2.50	2.50	2.50	2.50
2.01	2.23	2.45	2.50	2.50	2.50	2.50
1.29	1.46	1.63	1.79	1.96	2.13	2.30
1.40	1.58	1.76	1.94	2.12	2.29	2.47
1.52	1.70	1.89	2.08	2.27	2.46	2.50
1.63	1.83	2.02	2.22	2.42	2.50	2.50
1.74	1.95	2.16	2.37	2.50	2.50	2.50
1.06	1.23	1.39	1.56	1.73	1.89	2.06
1.17	1.35	1.52	1.70	1.88	2.05	2.23
1.28	1.46	1.65	1.84	2.02	2.21	2.50
1.39	1.58	1.78	1.97	2.17	2.37	2.50
1.50	1.70	1.91	2.11	2.32	2.50	2.50
0.83	1.00	1.16	1.33	1.50	1.66	1.83
0.94	1.11	1.29	1.46	1.64	1.82	1.99
1.05	1.23	1.41	1.60	1.78	2.33	2.40
1.15	1.35	1.54	1.73	1.93	2.50	2.50
1.26	1.46	1.67	1.87	2.07	2.28	2.50
0.60	0.77	0.93	1.10	1.27	1.43	1.60
0.71	0.88	1.06	1.23	1.41	1.58	2.40
0.81	1.00	1.18	1.37	1.55	1.73	2.50
0.92	1.11	1.31	1.50	1.69	2.50	2.50
1.03	1.23	1.43	1.63	2.50	2.29	2.50
0.37	0.54	0.70	0.87	1.04	1.20	1.37
0.48	0.65	0.83	1.00	1.18	2.50	2.39
0.58	0.77	0.95	1.13	1.32	1.50	2.50
0.69	0.88	1.07	1.26	1.46	1.65	2.48
0.79	0.99	1.20	1.40	1.60	2.50	2.49
0.14	0.23	0.80	0.80	0.81	0.97	1.14
0.00	0.14	0.60	0.77	0.94	1.12	2.50

55 / 55

Fig. 14q

0.00	0.12	0.24	0.90	1.08	2.14	2.47
0.46	0.65	0.84	1.03	1.22	1.42	2.46
0.56	0.76	0.96	1.16	1.36	2.17	2.48
0.00	0.08	0.24	0.41	0.57	0.74	0.91
0.10	0.00	0.35	0.54	0.71	2.22	2.50
0.00	0.04	0.05	0.14	0.85	1.04	2.47
0.10	0.15	0.00	0.17	0.47	1.18	2.40
0.00	0.53	0.13	0.28	1.13	1.49	2.44
0.12	0.00	0.00	0.18	0.34	0.51	0.68
0.02	0.07	0.04	0.05	0.48	0.66	2.35
0.02	0.07	0.04	0.05	0.62	0.80	2.35
0.02	0.01	0.08	0.11	0.14	0.58	2.34
0.00	0.03	0.03	0.09	0.15	0.63	2.38
0.00	0.00	0.00	0.00	0.11	0.28	0.45
0.02	0.04	0.00	0.05	0.19	0.43	0.60
0.00	0.00	0.04	0.06	0.16	0.64	2.26
0.00	0.01	0.01	0.03	0.07	0.29	1.98
0.02	0.00	0.03	0.04	0.12	0.17	2.35

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CA20 13/000769

A. CLASSIFICATION OF SUBJECT MATTER

IPC: **A61B 5/0476** (2006.01) , **A61B 5/00** (2006.01) , **A61B 5/16** (2006.01) , **G06F 19/00** (201 1.01)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC: **A61B 5/0476** (2006.01) , **A61B 5/00** (2006.01) , **A61B 5/16** (2006.01) , **G06F 19/00** (201 1.01)

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic database(s) consulted during the international search (name of database(s) and, where practicable, search terms used)

TotalPatents, Canadian Patent Database (Intellect), TEEExplore, Google Patents, World Wide Web. Keywords: sleep, awareness, level, eeg, power, frequency, amplitude, spectral, analysis, probability, index, pattern, database, match/compare, bin, epoch.

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	DRESSLER et al. "Awareness and the EEG power spectrum: analysis of frequencies " (17-09-2004)	1, 3, 4 and 6-11
Y	*See: pg. 807, right-hand-column, L 33 - pg. 808, left-hand-column, l. 12.	2, 5 and 12
Y	EP 1 562 472 (AKSELROD et al.) (17-08-2005) *See: [0006] and [0010].	2, 5 and 12

☐ Further documents are listed in the continuation of Box C.

☒ See patent family annex.

* Special categories of cited documents :	"Y" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance : the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier application or patent but published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

26 November 2013 (26.11.2013)

Date of mailing of the international search report

10 December 2013 (10-12-2013)

Name and mailing address of the ISA/CA
Canadian Intellectual Property Office
Place du Portage I, C114 - 1st Floor, Box PCT
50 Victoria Street
Gatineau, Quebec K1A 0C9
Facsimile No.: 001-819-953-2476

Authorized officer

Bryon Braymore (819) 934-6753

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/CA20 13/000769

Patent Document Cited in Search Report	Publication Date	Patent Family Member(s)	Publication Date
EP1562472B1	17 August 2005 (17-08-2005)	AT496577T AU2003263571A1 CA2499547A1 DE60335899D1 EP1562472B1 EP2286723A1 IL167400A US2006235315A1 US7623912B2 WO2004026133A2	15 February 2011 (15-02-2011) 08 April 2004 (08-04-2004) 01 April 2004 (01-04-2004) 10 March 2011 (10-03-2011) 26 January 2011 (26-01-2011) 23 February 2011 (23-02-2011) 29 December 2011 (29-12-2011) 19 October 2006 (19-10-2006) 24 November 2009 (24-11-2009) 01 April 2004 (01-04-2004)

专利名称(译)	用于从脑电图确定睡眠/觉醒状态的概率以及睡眠和觉醒的质量的方法和软件		
公开(公告)号	EP2895064A1	公开(公告)日	2015-07-22
申请号	EP2013837396	申请日	2013-09-12
[标]申请(专利权)人(译)	YRT有限公司		
申请(专利权)人(译)	YRT有限公司		
当前申请(专利权)人(译)	YRT有限公司		
[标]发明人	YOUNES MAGDY		
发明人	YOUNES, MAGDY		
IPC分类号	A61B5/0476 A61B5/00 A61B5/16 G06F19/00		
CPC分类号	A61B5/0205 A61B5/02405 A61B5/04014 A61B5/0476 A61B5/0826 A61B5/11 A61B5/4809 A61B5/4812 A61B5/4815 A61B5/4818 A61B5/725 A61B5/7264 G16H50/30 G16H10/60		
代理机构(译)	范尼、PETER JOHN		
优先权	61/700615 2012-09-13 US		
其他公开文献	EP2895064A4		
外部链接	Espacenet		

摘要(译)

提供方法和软件以格式化概率指数，该概率指数反映脑电图（ EEG ）模式在深度睡眠的觉醒频谱内的位置，其采用计算机/微处理器执行对一个或多个离散部分（ Bins ）的频域分析。用于确定指定频率的EEG功率的EEG，可选地计算指定频率范围内的总功率，为每个频率或频率范围的功率分配等级，为反映不同频率的等级的Bin分配代码或频率范围，并且通过使用参考源（例如查找表或其他合适的解码仪器）确定反映所述Bin内的所述EEG模式位于深度睡眠的觉醒频谱内的位置的索引。参考源是通过计算在由一个或多个专业技术人员或自动评分软件评分的参考文件中记录为清醒或睡眠的时期中出现的不同代码的区间的概率而获得的。