



(11) **EP 1 467 651 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
29.10.2008 Bulletin 2008/44

(21) Application number: **02794057.6**

(22) Date of filing: **26.11.2002**

(51) Int Cl.:
A61B 5/0245 (2006.01)

(86) International application number:
PCT/US2002/038097

(87) International publication number:
WO 2003/047427 (12.06.2003 Gazette 2003/24)

(54) **WIRELESS ELECTROCARDIOGRAPH SYSTEM**

DRAHTLOSES ELEKTROKARDIOGRAPHISCHES SYSTEM

SYSTEME D'ELECTROCARDIOGRAMME SANS FIL

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
IE IT LI LU MC NL PT SE SK TR**

(30) Priority: **30.11.2001 US 998733**

(43) Date of publication of application:
20.10.2004 Bulletin 2004/43

(73) Proprietor: **LifeSync Corporation
Fort Lauderdale FL 33301 (US)**

(72) Inventors:
• **ISTVAN, Rud
Fort Lauderdale, FL 33301 (US)**
• **GREGORY, Bill
Fort Lauderdale, FL 33316 (US)**
• **SOLOVAY, Kenneth
Weston, FL 33331 (US)**
• **CHASTAIN, David, Paul
Acton, MA 01720 (US)**

- **GUNDLACH, John, David
Acton, MA 01720 (US)**
- **HOPMAN, Nicholas, C.
Lake Zurich, IL 60047 (US)**
- **WILLIAMS, Daniel, L.
Norwell, MA 02061 (US)**
- **LODATO, Franco
Weston, FL 33327 (US)**
- **SALEM, Michael
Ft. Lauderdale, FL 33305 (US)**

(74) Representative: **Jackson, Robert Patrick
Frank B. Dehn & Co.
St Bride's House
10 Salisbury Square
London
EC4Y 8JD (GB)**

(56) References cited:
GB-A- 2 258 587 **US-A- 3 547 104**
US-A- 3 774 594 **US-A- 4 425 921**
US-A- 4 434 801

EP 1 467 651 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] A portion of the disclosure of this patent document contains material that is subject to copyright protection. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the Patent and Trademark Office patent file or records, but otherwise reserves all copyright rights whatsoever.

RELATED APPLICATIONS

[0002] This international application claims priority to U.S. Application Serial No. 09/998,733 for a WIRELESS ECG SYSTEM, filed November 30, 2001, the disclosure and content of which is hereby incorporated by reference in its entirety.

FIELD OF THE INVENTION

[0003] The present invention relates to a cardiac monitoring system and, more particularly, to a wireless electrocardiograph (ECG) system.

BACKGROUND OF THE INVENTION

[0004] An electrocardiograph (ECG) system monitors heart electrical activity in a patient. Conventional ECG systems utilize conductive pads or electrodes placed on a patient in specific locations to detect electrical impulses generated by the heart during each beat. In response to detection of the electrical impulses from the heart, the electrodes produce electrical signals indicative of the heart activity. Typically, these electrical signals are directly transferred from the electrodes to a stationary ECG monitor via multiple cables or wires. The ECG monitor performs various signal processing and computational operations to convert the raw electrical signals into meaningful information that can be displayed on a monitor or printed out for review by a physician.

[0005] Doctors have used ECG systems to monitor a patient's heart activity for decades. Currently, there are several different systems that use ECG signals to monitor a patient's heart activity. These systems, however, are generally stationary and are not developed or suitable for portable use. While portable telemetry systems exist, they are not a direct replacement for stationary ECG monitors. Moreover, because conventional systems use multiple cables or wires, and are cumbersome and uncomfortable for the patient, and require a significant amount of set up time. Thus, a need exists for an ECG system that solves the aforementioned problems.

BRIEF SUMMARY OF THE INVENTION

[0006] The present invention relates to a wireless ECG system that is universally compatible with existing or conventional ECG monitors. The ECG system comprises a

chest assembly, a body electronics unit, and a base station. The chest assembly connects to electrodes specifically located on a patient's body for detecting electrical signals from the patient's heart. The electrical signals are detected by the chest assembly - thus, providing up to a "7 lead" analysis of the heart. Alternatively, the chest assembly can be augmented with a precordial assembly that connects to electrodes specifically located on the patient's body - thus, providing a "12 lead" analysis of the heart.

[0007] Viewed from a first aspect, the present invention provides a chest assembly for detecting electrical signals from a patient's heart comprising:

- an electrode retaining section having a plurality of electrode connectors for releasably connecting to electrodes;
- a chest assembly connector attached to the electrode retaining section; and
- a sensor pin on the chest assembly connector for completing a circuit within a body electronics unit by inserting the chest assembly connector into a chest assembly port of the body electronics unit.

[0008] Viewed from a second aspect, the present invention provides a body electronics unit for use in a system for monitoring cardiac activity in a patient comprising:

- a chest assembly port for removably receiving a chest assembly connector attached to a chest assembly, the chest assembly connector including a sensor pin that completes a circuit within the body electronics unit when the chest assembly connector is inserted into the chest assembly port, wherein electrical signals detected from a patient's heart are transmitted to the body electronics unit via the chest assembly.

[0009] The electrical signals are transmitted through the chest assembly and the precordial assembly to the body electronics unit, which may be removably secured to the patient via an armband. The body electronics unit may transmit the electrical signals to the base station via radio transmission. The base station transmits the electrical signals to a conventional ECG monitor via standard cabling, which, in turn, processes or transforms the electrical signals into meaningful information that can be displayed on the ECG monitor for review by a physician.

[0010] The ECG system eliminates the wires that ordinarily tethers an ECG patient to an ECG monitor by replacing conventional wires with a radio link. The present invention is lightweight and portable - thereby providing increased comfort and mobility to the patient. In addition, the present invention requires decreased set-up times and is more convenient for health practitioners to use than conventional ECG systems.

[0011] These as well as other novel advantages, details, embodiments, features, and objects of the present

invention will be apparent to those skilled in the art from the following detailed description of the invention, the attached claims and accompanying drawings, listed herein below which are useful in explaining the invention.

BRIEF DESCRIPTION OF THE DRAWLING

[0012] The foregoing aspects and many of the advantages of the present invention will become readily appreciated by reference to the following detailed description of the preferred embodiment, when taken in conjunction with the accompanying drawings, wherein: Figure 1 is a perspective view of an exemplary embodiment of the ECG system;

Figure 2 is a cross sectional view of the chest assembly and the precordial assembly;
 Figure 3 is a top view of an exemplary embodiment of the chest assembly;
 Figure 4 is a top view of an exemplary embodiment of the precordial assembly;
 Figure 5 is a perspective view of an exemplary embodiment of the body electronics unit;
 Figure 6 is a top view an exemplary embodiment of the assembly connectors;
 Figure 7 is a front view of an exemplary embodiment of the body electronics unit;
 Figure 7a is an exemplary embodiment of the user interface of the electronics body unit;
 Figure 8 is a block diagram of an exemplary embodiment of the transmitter;
 Figure 9a is a perspective view of an exemplary embodiment of the base station used in conjunction with the token key;
 Figure 9b depicts the body electronics unit used in conjunction with the token key;
 Figure 10 is a perspective view of an exemplary embodiment of the base station;
 Figure 11 is a front view of an exemplary embodiment of the base station;
 Figure 11 a is an exemplary embodiment of the user interface of the base station;
 Figure 12 is a block diagram of an exemplary embodiment of the receiver;
 Figure 13 is a perspective view of an exemplary embodiment of the base station;
 Figure 14 is an exemplary embodiment of the adaptor assembly;
 Figure 15 is another exemplary embodiment of the adaptor assembly;
 Figure 16 is another exemplary embodiment of the adaptor assembly; and
 Figure 17 is a flow chart of an exemplary embodiment for operation of the ECG system.

DESCRIPTION OF THE PREFERRED EMBODIMENT

[0013] For a better understanding of the present inven-

tion, reference may be had to the following detailed description taken in conjunction with the appended claims and accompanying drawings. Briefly, the present invention relates to a wireless, portable ECG system. Referring to Figure 1, the ECG system 10 comprises a chest assembly 12, a body electronics unit 14, and a base station 16.

[0014] The chest assembly 12 is a one-piece flexible circuit that connects a plurality of electrode connectors 18, which are individually labeled 18a, 18b, 18c 18d, and 18e. The electrode connectors 18 have releasable connections that connect to electrodes 20, which are individually labeled 20a, 20b, 20c, 20d, and 20e. Preferably, the electrode connectors 18 have snap terminals that connect to electrodes 20 having snap terminals. Each electrode connector 18 connects to an electrically conductive element or trace for transmitting electrical signals. The electrically conductive elements or traces run along the chest assembly 12 and connect to a chest assembly connector 21.

[0015] Referring to Figure 2, the chest assembly 12 has outer layers 22, 24 that are constructed of a lightweight and reasonably moisture resistant material, such as DuPont Sontara® or other suitable fabric. Adhesive layers 26, 28 secure insulating layers 30, 32 to the outer layers 22, 24 respectively. Insulating layers 30, 32 are constructed of Mylar® (polyester) film or other suitable insulating material. Adhesive layers 34, 36 secure the insulating layers 30, 32 to a base layer 38. The base layer 38 is preferably constructed of Mylar film and has a first side 40 and a second side 42. The electrically conductive elements or traces that connect to the electrode connectors 18 are located on the first side 40 of the base layer 38. One such conductive element or trace is shown at 39. A shielding layer 44 for reducing any external interferences or radio frequency noise with the chest assembly 12 is located on the second side 42 of the base layer 38. The shielding layer 44 may be constructed of single or multiple layers of dielectric, or electrically or magnetically conductive material. The back of the electrode connector 18 may also be covered with Mylar to further insulate the chest assembly 12 and prevent an externally applied electric potential from entering the ECG system. The shielding layer preferably comprises an X-patterned grid.

[0016] Referring back to Figure 1, the chest assembly 12 attaches to five electrodes 20 and provides a means for generally positioning the electrodes on the patient, thereby providing up to a "7 lead" analysis of the electrical activity of the heart. The electrode connectors 18 are preferably labeled and color-coded to ensure that the chest assembly 12 is properly positioned on the patient and connected to the appropriate electrodes 20. For instance, the electrode connectors 18a, 18b, 18c, 18d, 18e are labeled RL, LA, LL, RA, and V, respectively. The chest assembly 12 is constructed such that the RA electrode connector is connected to an electrode positioned on the right side of the patient's chest about level of the first and second intercostal space, the LA electrode con-

nector is connected to an electrode positioned on the left side of the patient's chest about level of the first and second intercostal space, the RL and LL electrode connectors are connected to electrodes positioned on the left side of the patient's torso, and the V electrode connector is connected to an electrode positioned in the middle of the patient's chest about level of the fourth and fifth intercostal space. The chest assembly 12 is designed such that it is centered on the chest below the patient's clavicle.

[0017] Referring to Figure 3, the chest assembly 12 is configured to provide flexible positioning of the chest assembly 12 on the patient. Figure 3 is for illustrative purposes only, and thus, the chest assembly 12, as depicted in Figure 3, is not limited to any particular shape or configuration. The chest assembly 12 has a linear section or tail 46 extending from the chest assembly connector 21. Referring back to Figure 1, the tail 46 has a securing means 46a which allows the tail 46 to extend to either side of the patient. This securing means 46a may be any suitable mechanical device although adhesive or a clip is most preferred. Referring back to Figure 3, the tail 46 flows into an electrode retaining section 47. The electrode retaining section 47 has an arcuate section 48. A first expandable arm 50 attaches to the arcuate section 48. The RA electrode connector attaches to the first expandable arm 50. The arcuate section 48 flows into a transition section 52. The LA electrode connector attaches to the transition section 52. The transition section 52 flows into a linear run 54. The RL electrode connector attaches to the linear run 54. A second expandable arm 56 and an extension arm 58 attach to the linear run 54. The V electrode connector attaches to the second extension arm 58 and the LL electrode connector attaches to the second expandable arm 56.

[0018] The expandable arms 50, 56 are die cut in a serpentine pattern. The expandable arms 50, 56 comprise polypropylene or polyethylene fabric, Kapton, Mylar, or other flexible, memoryless material. The expandable arms 50, 56 expand, if necessary, by elongating the serpentine pattern. When expanded, a portion or all of the expandable arm is extended. Where only a portion of the expandable arm is extended, another portion remains folded. The expandable arms 50, 56 allow for extension as needed to so that the chest assembly 12 can fit patients of various sizes and also allow for patient movement when the patient is wearing the chest assembly 12. The extension arm 58 allows for flexible positioning of the V electrode connector in the middle of the patient's chest such as placement at electrode position V1, V2 or V3. In some instances, the health care practitioner may desire not to utilize the extension arm 58 for taking electrocardiograph measurements. Thus, to keep the extension arm 58 secured to the linear run 58 and to ensure that the extension arm 58 will not interfere with the placement and positioning of the chest assembly 12, the extension arm 58 is die cut with a perforated seam that connects the extension arm 58 and the linear run 54 along the length of the extension arm 58. If the health care

practitioner desires to use the extension arm 58, the perforated seam is unbroken so that the extension arm 58 can be selectively positioned on the patient's chest.

[0019] The chest assembly 12 can be used with a precordial assembly 60 to provide a "12-lead" analysis of the electrical activity of the heart. Similar to the chest assembly 12, the precordial assembly 60 is a one-piece flexible circuit that connects a plurality of electrode connectors 62. The electrode connectors 62 have releasable connections that connect to electrodes 64. Preferably, the electrode connectors 62 have snap terminals that connect to electrodes 64 having snap terminals. Each electrode connector 62 connects to an electrically conductive element or trace for transmitting electrical signals from a patient's heart. The electrically conductive elements or traces run along the precordial assembly 60 and connect to a precordial assembly connector 66. The precordial assembly 60 has the construction as shown in Figure 2.

[0020] As depicted in Figure 1, the precordial assembly 60 attaches to six electrodes 64 that are selectively positioned on the abdomen and middle chest of the patient. The electrode connectors 62 of the precordial assembly 60 are preferably labeled and color-coded so as to prevent a health care provider from applying or positioning the precordial assembly onto the patient improperly. For instance, the electrode connectors 62a, 62b, 62c, 62d, 62e, and 62f are labeled V1, V2, V3, V4, V5, and V6, respectively. When the precordial assembly 60 is used, the V electrode connector on the chest assembly 12 is removed from its electrode and replaced with an electrode connector on the precordial assembly 60.

[0021] As shown in Figure 4, the precordial assembly 60 is configured to provide flexible positioning of the precordial assembly 60 on the patient. Figure 4 is for illustrative purposes only, and thus, the precordial assembly 60, as depicted in Figure 4, is not limited to any particular shape or configuration. The precordial assembly has a linear section or tail 68 extending from the precordial assembly connector 66. The linear section or tail 68 flows into an electrode retaining section 69. The electrode retaining section 69 has a first arcuate section 70 having a first transition section 72. The V2 electrode connector attaches to the first transition section 72. The V1 electrode connector attaches to a first extension arm 74 connected to the first transition section 72. A second arcuate section 76 extends from the first transition section 72. A second transition section 78 abuts the second arcuate section 76 and the V4 electrode connector attaches to the second transition section 76. The V3 electrode connector attaches to a second extension arm 80 connected to the second transition section 78. A third arcuate section 82 flows from the second transition section 78. The third arcuate section 82 abuts a third transition section 84. The V5 electrode connector attaches to the third transition section 84. A fourth arcuate section 86 extends from the third transition section 84. The V6 electrode connector attaches to the fourth arcuate section 86. The configuration of the

precordial assembly 60 allows the health care provider or physician to flexibly position the electrode connectors 62 as needed to properly situate the precordial assembly 60 on the patient and to allow for patient movement when the patient is wearing the precordial assembly 60.

[0022] In operation, the chest assembly 12 and the precordial assembly 60 detect electrical signals generated by the heart during each beat and transfer these signals to the body electronics unit 14. When the system is operating in "7 lead" mode (i.e. when only the chest assembly 12 is being used) the body electronics unit 14 acquires signals from the RL, RA, LL, LA, and V electrodes. The body electronics unit 14 uses the RL electrode as a ground reference. When the system is operating in the "12 lead" mode (i.e. the chest assembly 12 and the precordial assembly 60 are being used) the body electronics unit 14 acquires signals from the RL, RA, LL, and LA electrodes via the chest assembly 12 and acquires signals from the V1, V2, V3, V4, V5, and V6 electrodes via the precordial assembly 60. Alternatively, a various number of electrodes may be monitored by the system. For example, the health care provider or physician may choose to use only two electrodes to monitor the heart, seven electrodes to monitor the heart, or the like. In other words, the present system is not limited to performing a "7 lead" and "12 lead" analysis of the heart. In addition, to detecting electrical signals from the heart, the chest assembly 12 and the precordial assembly 60 may be constructed to detect other vital signs of the patient, for example, pulse, respiration rate, heart rate, temperature EEG signals, and pulse oximeter signals.

[0023] Referring to Figure 5, the chest assembly 12 connects to the body electronics unit 14 via a chest assembly connector 21. Specifically, the chest assembly connector 21 inserts into a chest assembly port 88 located in the body electronics unit 14. Similarly, the precordial assembly 60 connects to the body electronics unit 14 via the precordial assembly connector 66. Specifically, the precordial assembly connector 66 (not shown) inserts into a precordial assembly port 90. Resistors are connected to the chest assembly port 88 and the precordial assembly port 90 to prevent excessive electrical current from entering the body electronics unit 14 - thereby ensuring that the body electronics unit 14 continues to operate properly in the presence a strong electrical current caused by a defibrillator (i.e. a 5 kV defibrillation excitation). The chest assembly connector 21 and the precordial assembly connector 66 are specifically keyed or configured to prevent the assembly connectors 21, 66 from being inserted into the assembly ports 88, 90 backwards, misaligned or otherwise improperly. Moreover, the chest assembly connector 21 is keyed or configured such that it is not compatible with the precordial assembly port 90. Likewise, the precordial assembly connector 66 is keyed or configured such that it is not compatible with the chest assembly port 88. Specifically, as shown in Figure 5A, the chest assembly connector 21 has tongues 21 a specifically configured or arranged to fit into corresponding

grooves 21b of the chest assembly port 88. Accordingly, the chest assembly connector 21 can only be connected to the chest assembly port 88 in one orientation. For example, if the tongues 21a are not aligned with the grooves 21b, the chest assembly connector 21 will not couple to the chest assembly port 88. Likewise, the precordial assembly connector 66 has tongues (not shown) specifically configured or arranged to fit into corresponding grooves (not shown) of the precordial assembly port 90.

[0024] As shown in Figure 6, the chest assembly connector 21 and the precordial assembly connector 66 (not shown) have retaining clips or flanges 92 located on the sides of the connectors 21, 66 for removably securing the connectors 21, 66 into the assembly ports 88, 90. However, other means may be used to removably secure the connectors 21, 66 in the assembly ports 88, 90, such as screws, pins or the like. In addition, the assembly connectors 21, 66 may have spring flanges or clips 94 located at the tip of the connectors 21, 66 for providing a bias or tension against the assembly ports 88, 90. The spring flanges or clips 94 provide the connectors 21, 66 with a secure fit within the assembly ports 88, 90, thereby reducing any play or movement of the connectors 21, 66 within the assembly ports 88, 90. The electrically conductive elements or traces are specifically configured on the connectors 21, 66 so as to ensure that the electrical signals from the heart are properly transmitted to the body electronics unit 14. In other words, the electrically conductive elements or traces must be sufficiently spaced apart or otherwise isolated in some manner to prevent arcing across the electrically conductive elements. In addition, the spacing of the electrically conductive elements or traces permits the chest assembly and the precordial assembly to withstand defibrillation shock. Furthermore, the connectors 21, 66 have ribs 96 for preventing the electrically conductive elements or traces from coming into contact with metal objects or the like when the connectors 21, 66 are not inserted into the assembly ports 88, 90.

[0025] The chest assembly connector 21 has a sensor pin or ground pin 98 that completes a circuit within the body electronics unit 14 when the chest assembly connector 21 is plugged into the chest assembly port 88, thereby activating the power and bringing the body electronic unit 14 out of "sleep mode." The sensor pin has specific tongue that corresponds and fits into a groove located in the chest assembly port 88. The sensor pin 98 serves as a means for the body electronics unit 14 to identify the chest assembly 12 and to prevent the use of other chest assemblies or electrocardiograph wearables that are not designed to be used with the on-body electronic unit 14. In other words, the power of the body electronics unit 14 will not activate unless the body electronics unit 14 identifies or recognizes the sensor pin 98 of the chest assembly 12.

[0026] The outside casing of the body electronics unit 14 is constructed of lightweight, molded plastic, such as acrylonitrile-butadiene-styrene (ABS) or other suitable

material. The shape and configuration of the body electronics 14 unit is not limited to any particular shape or configuration. As shown Figure 1, the body electronic unit 14 removably secures to the patient's arm via an armband 100, thus making the body electronics unit 14 readily accessibly to the patient. The armband 100 wraps around either the patient's right or left arm and attaches via Velcro or other suitable fastening means such as pins, snaps, or the like. The body electronics unit 14 slides under a strap or pocket on the armband 100. Referring to Figure 7, the body electronic unit 14 has a user interface 102 and a battery 104. The user interface 102 provides information to the patient pertaining to the system's operating status or functionality. For example, an exemplary embodiment of the user interface 102 may provide information on whether the body electronics unit 14 is communicating or transmitting normally to the base station 16, whether the battery 104 of the body electronics unit 14 is charging or the battery 104 is low, whether the power of the body electronics unit 12 is activated, or whether the body electronics unit 14 or base station is malfunctioning. In addition the user interface 102 may provide instructions on the correct order or procedure for pairing or coupling the body electronics unit 14 with the base station 16. Such information may be communicated to the patient via the user interface 102 in various ways, for example, LEDs, LCD, text, audible tones, etc. An exemplary embodiment of the user interface is shown in Figure 7a. The user interface 102 is readily accessible to the patient when the body electronics unit 14 is secured to the armband 100.

[0027] The battery 104 is inserted into a battery port 106 located in the bottom of the body electronics unit 14. The battery 104 is retained in the battery port 106 by latches or other suitable fastening means, such as clips, screws or the like. The battery 104 is preferably a 3.6 V Li-ion rechargeable battery. The battery 104 is readily accessible to the patient when the body electronics unit 14 is secured to the armband 100.

[0028] The body electronics unit 14 controls the acquisition of the ECG signals from the chest assembly 12 and the precordial assembly 60. A transmitter 108 within the body electronics unit 14 receives or acquires ECG signals from the chest assembly 12 and the precordial assembly 60 preferably at 3 kbps. When the system is operating in "7 lead" mode (i.e. when only the chest assembly 12 is being used) the body electronics unit 14 acquires signals from the RL, RA, LL, LA, and V electrodes. When the system is operating in the "12 lead mode" (i.e. the chest assembly 12 and the precordial assembly 60 are being used) the body electronics unit 14 acquires signals from the RL, RA, LL, and LA electrodes via the chest assembly 12 and acquires signals from the V1 thru V6 electrodes via the precordial assembly 60. In addition, other vital signs of the patient may be detected by the system and transmitted to the body electronics unit 14, for example pulse, respiration rate, heart rate, temperature, EEG signals and pulse oximeter signals.

[0029] As shown in Figure 8, the transmitter 108 comprises an application specific integrated circuit, a processor or other circuit 110, a plurality of signal channels 112, a multiplexer 114, an analog-to digital converter (ADC) 116, a controller 118, and a radio 120. Additionally, fewer or different components can be used. The body electronics unit 14 has nine signal channels 112 corresponding to the ten electrodes connected to the chest assembly 12 and the precordial assembly 60. The electrode channels 112 each comprise a connector 122, a filter 124, an amplifier 126, a Nyquist filter 128 and a track and hold circuit 130. The connectors 122 of the signal channels 112 connect to either the chest assembly port 88 or the precordial assembly port 90, depending on whether the electrode channel 112 corresponds to an electrode located on the chest assembly 12 or the precordial assembly 60. The filter 124 comprises a low pass filter, such as for removing electromagnetic interference signals. The amplifier 126 amplifies the signals from the electrodes. The Nyquist filter 128 comprises a low pass filter for removing out-of-band high frequency content of the amplified signals to avoid sampling error. The track and hold circuit 130 enables the system to sample all nine electrode channels signals 112 at a same or relative times so that there is not differential error created when these signals are combined later in an ECG monitor.

[0030] The multiplexer 114 sequentially selects signals from the electrode signal channels 112 using time division multiplexing. One of ordinary skill in the art, however, recognizes that other combination functions can be used. The ADC 116 converts the combined analog signals to digital signals for transmission. Preferably the controller 118 comprises a digital signal processor (DSP) that decimates the digitized signals as to lessen the bandwidth required to transmit the signals. The radio 120 modulates the digital signals with a carrier signal for transmission. In an exemplary embodiment, the radio 120 includes a demodulator for receiving information. The controller 118 digitally transmits the ECG data to the base station 16. In addition to transmitting ECG data, the controller 118 may transmit signals pertaining to pacemaker information, battery level information, electrode disconnection information, and other information as required. For example, vital signs such as pulse, respiration rate, heart rate, temperature, EEG signals, and pulse oximeter signals may be transmitted.

[0031] The body electronics unit continuously monitors the integrity of all patient electrode connections. In the event a lead is disconnected, the body electronics unit will send a signal to the base station which in turn causes the base station to trigger the "lead off" alarm on the ECG monitor. Additionally, the body electronics unit has a self-test function which monitors the integrity of the primary functions including the microprocessor, data acquisition, internal voltage references, and radio functionality. In the event a failure is detected, the body electronics unit will capture the fault condition, stop data acquisition and transmission and indicate that fault has occurred through

the lead off alarm.

[0032] The body electronics unit 14 operates to minimize undesired noise or signals. For example, components are matched such that later application to a differential amplifier in a legacy ECG monitor for determining a heart vector is accurate. ECG vectors are not formed by the ECG system 10, but rather by the legacy ECG monitor. Because the ECG system 10 is essentially "in-series" with the legacy ECG monitor, any error may produce undesirable results. One potential source of error is differential error. This differential error can be observed on the legacy ECG monitor when the ECG monitor forms the ECG lead signals by combining the individual electrode signals in the ECG monitor input stage. This input stage comprises a difference, or differential, amplifier to eliminate common mode interference from the signals produced at the electrodes 20.

[0033] An artifact will be present if there is any difference in how each of the electrode signals are processed when the legacy ECG's differential amplifier forms the ECG lead signals or ECG vectors. For example, if there is a difference in the gain of the amplifier, a difference in the phase shift associated with the anti-aliasing (Nyquist) filters, or a difference in how the respective track and hold circuits treat the electrode signals, then this differential error creates an artifact on the legacy ECG monitor. One important technique to minimize this potential source of differential errors is to choose a Nyquist filter cutoff frequency that is very high. This is because each individual filter will have differing group delay performance. To mitigate that difference, the frequency that this group delay will affect is much higher than the frequency of the ECG signals, which are about 0.05 Hz to 150 Hz. By choosing a high cutoff frequency for the Nyquist filters, any mismatch in the Nyquist filter components will not affect accuracy of the individual electrode ECG signals. For example, picking a filter cutoff frequency of 1,200 Hz mitigates this source of error. With this approach, the individual electrode ECG signals are over sampled at about 3,000 Hz in order to not introduce aliasing. Of course higher filter cutoff frequencies and correspondingly higher sampling rates may further reduce error. Lower cutoff frequencies and/or sampling rate may be used.

[0034] Because the electrode signals are now sampled at such a high rate, these signals may be decimated to minimize the required transmission bandwidth. For example the digital samples are decimated by a factor of eight in the controller 118. Greater or lesser rates of decimation can be used, such as decimation as a function of the bandwidth available for transmission, the number of electrode signals to be represented, and the Nyquist sampling rate. Referring back to Figure 1, the base station 16 receives the transmitted signals sent from the body electronics unit 14. The signals are transmitted as radio or other signals modulated with a carrier signal. Various air-interfaces can be used for transmission, such as Bluetooth or IEEE 802.11b. To establish proper com-

munication between the body electronics unit 14 and the base station 16, the base station 16 and body electronics unit 14 need to be paired such that the base station 16 and the body electronics unit 14 only recognize signals from the its pair. This may be accomplished in number of ways including direct connection of the base station 16 and the body electronics unit 14. Preferably, a token key 132 is used to pair or radio frequency link the body electronics unit 14 and the base station 16. Referring to Figure 9a, the token key 132 has memory chip and may optionally have a plurality of tongues or pins 133 that fit within grooves located in a token key port 134 of the base station 16 and within grooves of a token key port 136 of the body electronics unit 14. As shown in Figure 9b, the token key 132 inserts into the token key port 134 of the base station and reads and records an identification number for the base station 16. The token key 132 is then removed from the token key port 134 and inserted into the token key port 136 located in the body electronics unit 14. The electronics unit 14 receives the identification number for the base station 16 from the token key 132. In turn, the token key 132 reads and records the identification number for the body electronics unit 14. The token key 132 is then removed from the body electronics unit 14 and reinserted into the token key port 134 of the base station 16 whereby the base station 16 confirms the presence of its own identification number on the token key 132 and also reads the identification number for the body electronics unit 14 from the token key 132. The body electronics unit 14 and the base station 16 are paired. Alternatively, pairing or coupling can be accomplished by first inserting the token key 132 into the body electronics unit 14, removing the token key 132 and inserting the token key 132 into the base station 16, removing the token key 132 and reinserting the token 132 into the body electronics unit 14. In other words, the order in which the token key 132 is inserted into the body electronics unit 14 and the base station 16 is not critical to the proper operation of the system. Referring back to Figure 7, the user interface 102 may provide the user or health care provider with instructions on the correct order for pairing the body electronics unit 14 with the base station 16. The use of the token key 132 allows the pairing function to occur while the body electronics unit 14 is worn by the patient. This feature eliminates the need to disconnect and reconnect the body electronics unit 14 when a patient needs to be connected to different ECG monitors as a result of being moved around a hospital. The patient's body electronics unit 14 is just repaired with a new base station using the token key 132.

[0035] After the body electronics unit 14 and the base station 16 are paired, the body electronics unit 14 and the base station 16 will remain communicating with each other as long as the token key 132 remains in the token key port 134 of the base station 16 (or the token key port 136 of the body electronics unit 14, depending on the order of the pairing process). In other words, as soon as the token key 132 is removed from the base station 16,

the electronics unit 14 and the base station 16 will discontinue or cease communication. Any specific token key 132 can be used to pair any specific base station 16 with any specific body electronics unit 14.

[0036] The outside casing of the base station 16 is constructed of lightweight, molded plastic, such as acrylonitrile-butadiene-styrene (ABS) or other suitable material. The shape and configuration of the base station 16 is not limited to any particular shape or configuration. The base station 16 is removably secured to an ECG monitor 138 via suitable mounting means, such as Velcro®, dual-lock strips, double-sided foam tape, or the like. Preferably, the base station 16 is removably mounted to a mounting plate secured near the ECG monitor 138 via suitable mounting means. As shown in Figure 10, the base station 16 has a cradle 140 for storing the body electronics unit 14 when the body electronics unit 14 is not in use or otherwise off the patient. In addition, the base station 16 has a battery port 142 in which a base station battery 144 is removably inserted. The base station 16 may be constructed to have a plurality of battery ports that store and charge batteries when the batteries are not being used. When the base station 16 is not plugged into an AC wall power inlet, the base station battery 144 provides power to the base station 16. When the base station 16 is operating on AC wall power, the base station 16 charges the base station battery 144 when the base station battery 144 is in the battery port 142. The base station 16 has a power switch 146 that activates/deactivates the power to the base station 16 and a power cord connection 148 for connecting a power cord to an AC wall power inlet. The base station battery 144 is preferably a 3.6 V Li-ion rechargeable battery. Accordingly, the base station battery 144 and the body electronics unit battery 104 are preferably identical and interchangeable, such that each battery can be used in either the body electronics unit 14 or the base station 16. The system is designed such that a discharged body electronics unit battery 104 is swapped for a charged base station battery 144. In this manner a charged battery is always readily available for the body electronics unit. In addition, the base station 16 has a lead switch 150 that allows the health care provider to instruct the base station 16 to operate in "7 lead" mode or "12 lead" mode.

[0037] As depicted in Figure 11, the base station 16 has a user interface 152 that provides information to the health provider or patient pertaining to the system's operating status or functionality. For example, the user interface 152 may provide information on whether the body electronics unit 14 is communicating or transmitting normally to the base station 16, whether the base station battery 144 is charging or the battery 144 is low, whether the body electronics unit battery 104 is low, or whether the power of the base station 16 is activated, whether the base station 16 is malfunctioning or otherwise requires servicing. In addition the user interface 102 may provide instructions on the correct order or procedure for pairing or coupling the body electronics unit 14 with the

base station 16. Such information may be communicated to the health care provider or patient via the user interface 152 in various ways, for example, LED's, LCD, text, audible tones, etc. An exemplary embodiment of the user interface 102 is shown in Figure 11a.

[0038] Additionally, the base station has a self-test function which monitors the integrity of the primary functions including the microprocessor, data acquisition, internal voltage references, and radio functionality. In the event a failure is detected, the body electronics unit will capture the fault condition, stop data acquisition and transmission and indicate that fault has occurred through the lead off alarm.

[0039] A receiver 154 located within the base station 16 receives signals sent to the base station 16 from the body electronics unit 14. As shown in Figure 12, the receiver 154 includes a radio 156, a controller 158, a digital-to-analog converter (DAC) 160, a de-multiplexer 162, a transceiver 164, and a plurality of electrode signal channels 166. The radio 156 demodulates the received signals for identifying digital data representing the combined electrode signals. In an exemplary embodiment, the radio 156 includes a modulator for transmitting control information. The controller 158 controls operation of the various components and may further process the signals from the radio 156, such as interpolating data, converting the signals to digital information, generating control signals for the transmitter 108 in the electronics unit 14, operating any user output or input devices, and diagnosing operation of the ECG system. Preferably, the controller 118 interpolates the electrode signals to return the effective sample rate to about 3kHz or another frequency. This enables the reconstruction filters to have a cutoff frequency many times the bandwidth of the electrode signals, thus minimizing any differences in group delay at the frequencies of interest, i.e. less than 150 Hz. The DAC 160 converts the digital signals to analog signals. The demultiplexer 162 separates the individual regenerated electrode signals onto the separate electrode signal channels 166. The transceiver 164 operates operable pursuant to the Bluetooth specification for two-way communication with the transmitter 108.

[0040] The receiver 154 has nine electrode signal channels 166 corresponding to the 10 electrodes connected to the chest assembly 12 and the precordial assembly 60. The electrode signal channels 166 each comprise a sample and hold circuit 168, a filter 170, and an attenuator 172. The sample and hold circuit 168 is controlled by the controller 118 so that the converted electrode signals appear simultaneously on each electrode signal channel 166. Other embodiments may include individual DAC's that provide the signal substantially simultaneously. The filter 170 comprises a low pass reconstruction filter for removing high frequency signals associated with the DAC conversion process. The attenuator 172 comprises an amplifier for decreasing the amplitude to a level associated with signals at the electrodes, which were earlier amplified in the amplifiers of the body elec-

tronics unit 14. This results in a unity system gain so as not to introduce error between the electrodes and the conventional ECG monitor.

[0041] The base station 16 transmits the ECG signals to the ECG monitor 138 via pre-existing or conventional monitor cables 174. In turn, the information is displayed on the ECG monitor and reviewed by a physician. As depicted in Figure 13, the monitor cables 174 removably insert onto snap terminals 176 located on the base station 16. Preferably, the base station 16 has ten snap terminals 176 arranged on the left and right side of the base station 16. The snap terminals 176 and the monitor cables 174 are preferably labeled and color-coded so that the monitor cables 174 are properly connected to the base station 16. For instance, the five snap terminals 176 located on the left side of the base station 16 and the monitor cable 174 may be labeled as RL, LA, LL, RA, and V/V1. In addition, the five snap terminals 176 on the right side of the base station 16 and the monitor cable 174 may be labeled V2, V3, V4, V5, and V6. When the ECG system is operating in "7 lead" mode (i.e. only the chest assembly 12 is used) the monitor cable 174 is plugged into the five snap terminals 176 on the left side of the base station 16. When the ECG system is operating in "12 lead" mode (i.e. both the chest assembly 12 and the precordial assembly 60 is used) both the monitor cables 174 are plugged into the snap terminals 176 -- the top four snap terminals 176 on the left side of the base station 16 will be used for chest assembly electrodes and the remaining six snap terminals 176 will be used for precordial assembly electrodes.

[0042] There may be instances where a base station 16 will not be in every ward or hospital room for use with the body electronics unit 14. In such instances, an adaptor assembly 178 may be used to connect the chest assembly 12 or the precordial assembly 60 to the ECG monitor 138. In one exemplary embodiment, the adaptor assembly 178 allows the chest assembly 12 or precordial assembly 60 to be plugged directly into a conventional or existing telemetry transmitter. Figure 14 depicts the adaptor assembly 178 having an assembly receptacle 180 that connects to the chest assembly 12 or the precordial assembly 60 and a telemetry box receptacle 182 that connects to a conventional or existing telemetry transmitter. In another exemplary embodiment, the adaptor assembly 178 allows the chest assembly 12 or precordial assembly 60 to be plugged directly into a conventional or existing ECG monitor trunk cables. Figure 15 depicts the adaptor assembly 178 having an assembly receptacle 184 for connecting to the chest assembly 12 or the precordial assembly 60 and a cable assembly 185 for connecting to a conventional or existing ECG monitor trunk cable. The cable assembly 185 has a cable 186 that connects to a trunk cable adaptor 188 for connecting to an ECG monitor trunk cable. In another exemplary embodiment, the adaptor assembly 178 allows the chest assembly 12 or precordial assembly 60 to be plugged directly into standard lead wires that connect to an ECG

monitor. Figure 16 depicts the adaptor 178 having an assembly receptacle 190 for connecting to the chest assembly 12 or the precordial assembly 60 and a lead wire cable assembly 192 for connecting to a lead wire assembly. The cable assembly 192 has a cable 194 that connects to a lead wire adaptor 196 for connecting to standard lead wires. Various configurations of the adapter 178 are possible depending on the connector configuration of the standard lead wires.

[0043] Figure 17 depicts the method of monitoring the cardiac activity in the patient's heart using the wireless ECG system of the present invention. In step 198, electrodes are placed on the patient's body. In step 200, the chest assembly 12 and/or precordial assembly 60 are positioned on the patient's body by connecting the electrode connectors 21, 62 to the electrodes. In step 202, the chest assembly 12 and/or the precordial assembly 60 are plugged into the body electronics unit 14. In step 204, the electronics unit 14 and the base station 16 are paired or coupled by inserting the token key 132 into the base station 16, removing the token key 132 from the base station 16, inserting the token key 132 into the body electronics unit 14, removing the token key 132 from the electronics unit 14, and reinserting the token key 132 into the base station 16. Alternatively, coupling can be accomplished by inserting the token key 132 into the body electronics unit 14, removing the token key 132 from the body electronics unit, inserting the token key 132 into the base station 16, removing the token key 132 from the base station 16 and reinserting the token key 132 into the body electronics unit 14. In step 206, electrical signals from the patient's heart are detected and transmitted to the body electronics unit 14 via chest assembly 12 and the precordial assembly 60. In step 208, the electrical signals from the heart are transformed by the body electronics unit 14 from analog signals to digital signals. In step 210, the body electronics unit 14 transmits the digital signals to the base station 16 via radio transmission. In step 212, the base station 16 transforms the digital signals into analog signals. In step 214, the base station 16 transmits the analog signals to the ECG monitor 138 via monitor cables 174. In step 216, the ECG monitor 138 processes the analog signals into meaningful information that can be displayed on the monitor 138.

[0044] In the foregoing specification, the present invention has been described with reference to specific exemplary embodiments thereof. It will be apparent to those skilled in the art, that a person understanding this invention may conceive of changes or other embodiments or variations, which utilize the principles of this invention without departing from the broader spirit and scope of the invention. The specification and drawings are, therefore, to be regarded in an illustrative rather than restrictive sense. Accordingly, it is not intended that the invention be limited except as may be necessary in view of the appended claims.

Claims

1. A chest assembly for detecting electrical signals from a patient's heart comprising:
- an electrode retaining section having a plurality of electrode connectors for releasably connecting to electrodes;
- a chest assembly connector attached to the electrode retaining section; and
- a sensor pin on the chest assembly connector for completing a circuit within a body electronics unit, wherein the sensor pin is arranged such that the power of the body electronics unit is activated when the sensor pin completes the circuit within the body electronics unit by inserting the chest assembly connector into a chest assembly port of the body electronics unit.
2. The chest assembly of claim 1 wherein the electrode retaining section includes at least one expandable arm.
3. The chest assembly of claim 2 wherein the electrode retaining section further comprises an arcuate section, a linear run, and an extension arm.
4. The chest assembly of claim 1, 2 or 3 wherein the electrode connectors are arranged so that an electrode can be positioned on the right side of the patient's chest about level of the first and second intercostal space, an electrode can be positioned on the left side of the patient's chest about level of the first and second intercostal space, an electrode can be positioned in the middle of the patient's chest about level of the fourth and fifth intercostal space, and two electrodes can be positioned on the left side of the patient's torso.
5. The chest assembly of claim 3 wherein the electrode retaining section is connected to the chest assembly connector by a linear section.
6. The chest assembly of claim 5 wherein the arcuate section abuts the linear section, a first expandable arm attaches to the arcuate section and an electrode connector attaches to the first expandable arm, a transition section abuts the arcuate section and an electrode connector attached to the transition section, a linear run abuts the transition section and an electrode connector attaches to the linear run, and a second expandable arm and an extension arm attach to the linear run, an electrode connector attaches to the second extension arm and an electrode connector attaches to the second expandable arm.
7. The chest assembly of claim 3 wherein the chest assembly connects to a telemetry transmitter via an adaptor assembly.
8. The chest assembly of claim 3 wherein the chest assembly connects to an electrocardiograph monitor via an adaptor assembly.
9. The chest assembly of claim 3 wherein the chest assembly connector includes a plurality of electrically conductive elements sufficiently spaced to prevent arcing across the electrically conductive elements.
10. The chest assembly of claim 9 wherein the chest assembly connector includes a plurality of ribs to prevent the electrically conductive elements from contacting objects when the chest assembly connector is not secured within the body electronics unit.
11. The chest assembly of claim 9 wherein the electrically conductive elements are spaced to permit the chest assembly to withstand a defibrillation shock.
12. A chest assembly as claimed in claim 1 comprising:
- a base layer having a first side and a second side, the first side attached to a plurality of electrically conductive elements, the second side attached to a shielding layer;
- a first insulating layer positioned above the base layer; and a second insulating layer positioned below the base layer.
13. The chest assembly of claim 12 wherein the electrically conductive elements connect to electrode connectors and a chest assembly connector.
14. The chest assembly of claim 12 or 13 further comprising a shielding layer with an X-pattened grid construction.
15. The chest assembly of claim 12, 13 or 14 wherein the shielding layer comprises a single layer of dielectric material.
16. The chest assembly of claim 12, 13 or 14 wherein the shielding layer comprises multiple layers of dielectric material.
17. A chest assembly as claimed in claim 1, wherein:
- the chest assembly is a precordial assembly, the electrode retaining section is a flexible electrode retaining section connected to the precordial assembly connector by a linear section, the electrode retaining section is removably attached to a plurality of electrode connectors, and the electrode retaining section comprises at least one extension arm, a plurality of arcuate sections, and a plurality of transition segments.

18. The chest assembly of claim 17 wherein a first arcuate section abuts the linear section, a first transition section abuts a first arcuate section and an electrode connector attaches to the first transition segment, the extension arm connects to the first transition section and an electrode connector attaches to the first extension arm, a second arcuate section abuts the first transition section, a second transition section abuts the second arcuate section and an electrode connector attaches to the second transition section, a second extension arm connects to the second transition section and an electrode connector attaches to the second extension arm, a third arcuate section abuts the second transition section, a third transition segment abuts the third arcuate section and an electrode connector attaches to the third transition segment, and a fourth arcuate section abuts the third transition segment and an electrode connector attaches to the fourth arcuate section.
19. The chest assembly of claim 17 or 18 wherein the precordial assembly connects to a telemetry transmitter via an adaptor assembly.
20. The chest assembly of claim 17 or 18 wherein the precordial assembly connects to an electrocardiograph monitor via an adaptor assembly.
21. The chest assembly of any of claims 17 to 20 wherein the precordial assembly connector includes a plurality of electrically conductive elements sufficiently spaced to prevent arcing across the electrically conductive elements.
22. The chest assembly of claim 21 wherein the precordial assembly connector includes a plurality of ribs to prevent the electrically conductive elements from contacting objects when the precordial assembly connector is not secured within the body electronics unit.
23. The chest assembly of claim 21 or 22 wherein the chest assembly connector includes a plurality of spring flanges and at least one tongue corresponding to at least one groove in the chest assembly port.
24. The chest assembly of claim 23 wherein the electrically conductive elements are spaced to permit the precordial assembly to withstand a defibrillation shock.
25. A body electronics unit for use in a system for monitoring cardiac activity in a patient comprising:
- a chest assembly port for removably receiving a chest assembly connector attached to a chest assembly, the chest assembly connector including a sensor pin that completes a circuit within
- the body electronics unit when the chest assembly connector is inserted into the chest assembly port, wherein electrical signals detected from a patient's heart are transmitted to the body electronics unit via the chest assembly, wherein the power of the body electronics unit is activated by when the sensor pin completes the circuit within the body electronics unit.
26. The body electronics unit of claim 25 further comprising a user interface for communicating information to a user.
27. The body electronics unit of claim 26 wherein the information pertains to the system's operating status.
28. The body electronics unit of claim 26 or 27 wherein the information pertains to the order for pairing the body electronics unit to a base station.
29. The body electronics unit of any of claims 25 to 28 wherein the body electronics unit is capable of performing a lead off function for continuously monitoring the integrity of connections between at least one electrode connector attached to the chest assembly and at least one electrode attached to the patient.
30. The body electronics unit of any of claims 25 to 29 wherein the body electronics unit is capable of performing a self test function for monitoring the integrity of the system's functions.
31. The body electronics unit of any of claims 25 to 29 further comprising a resistor connected to the chest assembly port to prevent excessive electrical current from entering the body electronics unit, thereby permitting the body electronics unit to withstand a defibrillation shock.
32. The body electronics unit of any of claims 25 to 31 further comprising at least one battery that is compatible with a battery port in the body electronics unit and a battery port in a base station.
33. The body electronics unit of any of claims 25 to 32 further comprising a port for receiving an apparatus for pairing a base station with the body electronics unit.
34. The body electronics unit of claim 33 wherein the apparatus is a token key.
35. A system for wireless transmission of physiological signals from a patient to a monitor comprising a chest assembly as claimed in any of claims 1 to 24 and a body electronics unit as claimed in any of claims 25 to 34 wherein the chest assembly and body electron-

ics unit are connected by means of the chest assembly connector and the chest assembly port.

Patentansprüche

1. Thoraxanordnung zum Erfassen elektrischer Signale von einem Herz eines Patienten, mit:

einem Elektrodenhalteabschnitt, der eine Mehrzahl von Elektrodenanschlüssen zum lösbaren Verbinden mit Elektroden aufweist, einem Thoraxanordnungsanschluss, der an dem Elektrodenhalteabschnitt angebracht ist, und einem Sensorpin an dem Thoraxanordnungsanschluss zum Schließen eines Schaltkreises innerhalb einer Körperelektronikeinheit, wobei der Sensorpin so angeordnet ist, dass die Energie der Körperelektronikeinheit aktiviert ist, wenn der Sensorpin den Schaltkreis innerhalb der Körperelektronikeinheit schließt, indem der Thoraxanordnungsanschluss in eine Thoraxanordnungsschnittstelle der Körperelektronikeinheit eingefügt ist.

2. Thoraxanordnung nach Anspruch 1, bei der der Elektrodenhalteabschnitt mindestens einen expandierbaren Arm umfasst.

3. Thoraxanordnung nach Anspruch 2, bei der der Elektrodenhalteabschnitt des weiteren einen bogenförmigen Abschnitt, einen linearen Verlaufsabschnitt und einen Auslegerarm umfasst.

4. Thoraxanordnung nach Anspruch 1, 2 oder 3, bei der die Elektrodenanschlüsse so angeordnet sind, dass eine Elektrode auf der rechten Seite des Thorax des Patienten ungefähr auf Höhe des ersten und des zweiten interkostalen Zwischenraums angeordnet sein kann, eine Elektrode auf der linken Seite des Thorax des Patienten ungefähr auf Höhe des ersten und des zweiten interkostalen Zwischenraums angeordnet sein kann, eine Elektrode in der Mitte des Thorax des Patienten ungefähr auf Höhe des vierten und des fünften interkostalen Zwischenraums angeordnet sein kann und zwei Elektroden auf der linken Seite des Torsos des Patienten angeordnet sein können.

5. Thoraxanordnung nach Anspruch 3, bei der der Elektrodenhalteabschnitt mit dem Thoraxanordnungsanschluss mittels eines linearen Abschnitts verbunden ist.

6. Thoraxanordnung nach Anspruch 5, bei der der bogenförmige Abschnitt an dem linearen Abschnitt anliegt, ein erster expandierbarer Arm an dem bogenförmigen Abschnitt angebracht ist und ein Elektro-

denanschluss an dem ersten expandierbaren Arm angebracht ist, ein Übergangsabschnitt an dem bogenförmigen Abschnitt anliegt und ein Elektrodenanschluss an dem Übergangsabschnitt angebracht ist, ein linearer Verlaufsabschnitt an dem Übergangsabschnitt anliegt und ein Elektrodenanschluss an dem linearen Verlaufsabschnitt angebracht ist, und ein zweiter expandierbarer Arm und ein Auslegerarm an dem linearen Verlaufsabschnitt angebracht sind, ein Elektrodenanschluss an dem zweiten Auslegerarm angebracht ist und ein Elektrodenanschluss an dem zweiten expandierbaren Arm angebracht ist.

5

10

15

20

25

30

35

40

45

50

55

7. Thoraxanordnung nach Anspruch 3, bei der die Thoraxanordnung mit einer Telemetrieübertragungsvorrichtung über eine Adapteranordnung verbunden ist.

8. Thoraxanordnung nach Anspruch 3, bei der die Thoraxanordnung mit einem Elektrokardiographiemonitor über eine Adapteranordnung verbunden ist.

9. Thoraxanordnung nach Anspruch 3, bei der der Thoraxanordnungsanschluss eine Mehrzahl von elektrisch leitenden Elementen umfasst, die genügend beabstandet sind, um einen Funkenschlag über die elektrisch leitenden Elemente zu vermeiden.

10. Thoraxanordnung nach Anspruch 9, bei der der Thoraxanordnungsanschluss eine Mehrzahl von Rippen umfasst, um zu vermeiden, dass die elektrisch leitenden Elemente Objekte berühren, wenn der Thoraxanordnungsanschluss nicht innerhalb der Körperelektronikeinheit festgelegt ist.

11. Thoraxanordnung nach Anspruch 9, bei der die elektrisch leitenden Elemente beabstandet sind, um zu ermöglichen, dass die Thoraxanordnung einem Defibrillationsschock widersteht.

12. Thoraxanordnung nach Anspruch 1, mit:

einer Basisschicht, die eine erste Seite und eine zweite Seite aufweist, wobei die erste Seite an einer Mehrzahl von elektrisch leitenden Elementen angebracht ist und die zweite Seite an einer Schutzschicht angebracht ist, einer ersten Isolationsschicht, die über der Basisschicht angeordnet ist und einer zweiten Isolationsschicht, die unter der Basisschicht angeordnet ist.

13. Thoraxanordnung nach Anspruch 12, bei der die elektrisch leitenden Elemente mit Elektrodenanschlüssen und einem Thoraxanordnungsanschluss verbunden sind.

14. Thoraxanordnung nach Anspruch 12 oder 13, die

- des weiteren eine Schutzschicht mit einer X-gemusterten Gitterkonstruktion umfasst.
15. Thoraxanordnung nach Anspruch 12, 13 oder 14, bei der die Schutzschicht eine einzige Schicht eines nichtleitenden Materials umfasst.
16. Thoraxanordnung nach Anspruch 12, 13 oder 14, bei der die Schutzschicht mehrere Schichten eines nichtleitenden Materials umfasst.
17. Thoraxanordnung nach Anspruch 1, bei der:
- die Thoraxanordnung eine Präkordialanordnung ist,
- der Elektrodenhalteabschnitt ein flexibler Elektrodenhalteabschnitt ist, der mit dem Präkordialanordnungsanschluss über einen linearen Abschnitt verbunden ist, der Elektrodenhalteabschnitt lösbar an einer Mehrzahl von Elektrodenanschlüssen angebracht ist, und der Elektrodenhalteabschnitt mindestens einen Auslegerarm, eine Mehrzahl von bogenförmigen Abschnitten und eine Mehrzahl von Übergangsegmenten umfasst.
18. Thoraxanordnung nach Anspruch 17, bei der ein erster bogenförmiger Abschnitt an dem linearen Abschnitt anliegt, ein erster Übergangabschnitt an dem ersten bogenförmigen Abschnitt anliegt und ein Elektrodenanschluss an dem ersten Übergangsegment angebracht ist, der Auslegerarm mit dem ersten Übergangabschnitt verbunden ist und ein Elektrodenanschluss an dem ersten Auslegerarm angebracht ist, ein zweiter bogenförmiger Abschnitt an dem ersten Übergangabschnitt anliegt, ein zweiter Übergangabschnitt an dem zweiten bogenförmigen Abschnitt anliegt und ein Elektrodenanschluss an dem zweiten Übergangabschnitt angebracht ist, ein zweiter Auslegerarm mit dem zweiten Übergangabschnitt verbunden ist und ein Elektrodenanschluss an dem zweiten Auslegerarm angebracht ist, ein dritter bogenförmiger Abschnitt an dem zweiten Übergangabschnitt anliegt, ein drittes Übergangsegment an dem dritten bogenförmigen Abschnitt anliegt und ein Elektrodenanschluss an dem dritten Übergangsegment angebracht ist, und ein vierter bogenförmiger Abschnitt an dem dritten Übergangabschnitt anliegt und ein Elektrodenanschluss an dem vierten bogenförmigen Abschnitt angebracht ist.
19. Thoraxanordnung nach Anspruch 17 oder 18, bei der die Präkordialanordnung mit einer Telemetrieübertragungsvorrichtung über eine Adapteranordnung verbunden ist.
20. Thoraxanordnung nach Anspruch 17 oder 18, bei
- der die Präkordialanordnung mit einem Elektrokardiographiemonitor über eine Adapteranordnung verbunden ist.
21. Thoraxanordnung nach einem der Ansprüche 17 bis 20, bei der der Präkordialanordnungsanschluss eine Mehrzahl von elektrisch leitenden Elementen umfasst, die genügend beabstandet sind, um einen Funkenschlag über die elektrisch leitenden Elemente zu vermeiden.
22. Thoraxanordnung nach Anspruch 21, bei der der Präkordialanordnungsanschluss eine Mehrzahl von Rippen umfasst, um zu vermeiden, dass die elektrisch leitenden Elemente Objekte berühren, wenn der Präkordialanordnungsanschluss nicht innerhalb der Körperelektronikeinheit festgelegt ist.
23. Thoraxanordnung nach Anspruch 21 oder 22, bei der die Thoraxanordnungsanschluss eine Mehrzahl von Federflanschen und mindestens eine Zunge umfasst, die mindestens einer Nut in der Thoraxanordnungsschnittstelle entspricht.
24. Thoraxanordnung nach Anspruch 23, bei der die elektrisch leitenden Elemente beabstandet sind, um der Präkordialanordnung zu ermöglichen, einem Defibrillationsschock zu widerstehen.
25. Körperelektronikeinheit zur Verwendung in einem System zum Überwachen einer Herzaktivität in einem Patienten, mit:
- einer Thoraxanordnungsschnittstelle zum lösbaren Aufnehmen eines Thoraxanordnungsanschlusses, der an einer Thoraxanordnung angebracht ist, wobei der Thoraxanordnungsanschluss einen Sensorpin umfasst, der einen Schaltkreis innerhalb der Körperelektronikeinheit schließt, wenn der Thoraxanordnungsanschluss in die Thoraxanordnungsschnittstelle eingefügt ist, wobei von einem Herz eines Patienten erfasste elektrische Signale über die Thoraxanordnung zu der Körperelektronikeinheit übertragen werden, wobei die Energie der Körperelektronikeinheit aktiviert ist, wenn der Sensorpin den Schaltkreis innerhalb der Körperelektronikeinheit schließt.
26. Körperelektronikeinheit nach Anspruch 25, des weiteren mit einer Benutzerschnittstelle zum Kommunizieren von Information zu einem Benutzer.
27. Körperelektronikeinheit nach Anspruch 26, bei der die Information den Betriebsstatus des Systems betrifft.
28. Körperelektronikeinheit nach Anspruch 26 oder 27,

bei der die Information die Anweisungen zum Zuordnen der Körperelektronikeinheit zu einer Basisstation betrifft.

29. Körperelektronikeinheit nach einem der Ansprüche 25 bis 28, bei der die Körperelektronikeinheit dazu in der Lage ist, eine Ableitungsfunktion zum kontinuierlichen Überwachen der Funktionsfähigkeit von Verbindungen zwischen mindestens einem Elektrodenanschluss, der an der Thoraxanordnung angebracht ist, und mindestens einer Elektrode, die an dem Patienten angebracht ist, zu überwachen. 5
30. Körperelektronikeinheit nach einem der Ansprüche 25 bis 29, bei der die Körperelektronikeinheit dazu in der Lage ist, eine Selbst-Test-Funktion zum Überwachen der Funktionsfähigkeit der Systemfunktionen durchzuführen. 10
31. Körperelektronikeinheit nach einem der Ansprüche 25 bis 29, die des weiteren einen Widerstand umfasst, der mit der Thoraxanordnungsschnittstelle verbunden ist, um zu vermeiden, dass ein zu hoher elektrischer Strom in die Körperelektronikeinheit eintritt, wodurch der Körperelektronikeinheit ermöglicht wird, einem Defibrillationsschock widerstehen. 15
32. Körperelektronikeinheit nach einem der Ansprüche 25 bis 31, die des weiteren mindestens eine Batterie umfasst, die mit einer Batterieschnittstelle in der Körperelektronikeinheit und einer Batterieschnittstelle in einer Basisstation kompatibel ist. 20
33. Körperelektronikeinheit nach einem der Ansprüche 25 bis 32, die des weiteren eine Schnittstelle zum Aufnehmen einer Vorrichtung zum Zuordnen einer Basisstation zu der Körperelektronikeinheit umfasst. 25
34. Körperelektronikeinheit nach Anspruch 33; bei der die Vorrichtung ein Token-Schlüssel ist. 30
35. System zum drahtlosen Übertragen von physiologischen Signalen von einem Patienten zu einer Überwachungs Vorrichtung, die eine Thoraxanordnung nach einem der Ansprüche 1 bis 24 und eine Körperelektronikeinheit nach einem der Ansprüche 25 bis 34 umfasst, bei dem die Thoraxanordnung und die Körperelektronikeinheit mittels des Thoraxanordnungsanschlusses und der Thoraxanordnungsschnittstelle verbunden sind. 35

Revendications

1. Ensemble thoracique pour détecter des signaux électriques provenant du coeur d'un patient, comprenant : 40

une partie de retenue d'électrode ayant une pluralité de connecteurs d'électrode pour connecter des électrodes de manière amovible ; un connecteur d'ensemble thoracique fixé sur la partie de retenue d'électrode ; et une broche de capteur sur le connecteur de l'ensemble thoracique pour compléter un circuit à l'intérieur d'un bloc électronique corporel, dans lequel la broche de capteur est agencée de telle sorte que l'énergie du bloc électronique corporel est activée lorsque la broche de capteur complète le circuit à l'intérieur du bloc électronique corporel en insérant le connecteur d'ensemble thoracique dans un orifice d'ensemble thoracique du bloc électronique corporel.

2. Ensemble thoracique selon la revendication 1, dans lequel la partie de retenue d'électrode inclut au moins un bras extensible. 45
3. Ensemble thoracique selon la revendication 2, dans lequel la partie de retenue d'électrode comprend en outre une partie incurvée, un tronçon linéaire et un bras d'extension. 50
4. Ensemble thoracique selon la revendication 1, 2 ou 3, dans lequel les connecteurs d'électrode sont agencés de telle sorte qu'une électrode peut être positionnée sur le côté droit de la poitrine du patient au-dessus du niveau des premier et deuxième espaces intercostaux, une électrode peut être positionnée sur le côté gauche de la poitrine du patient au-dessus du niveau des premier et deuxième espaces intercostaux, une électrode peut être positionnée au milieu de la poitrine du patient au-dessus du niveau des quatrième et cinquième espaces intercostaux, et deux électrodes peuvent être positionnées sur le côté gauche du torse du patient. 55
5. Ensemble thoracique selon la revendication 3, dans lequel la partie de retenue d'électrode est reliée au connecteur d'ensemble thoracique par une partie linéaire. 60
6. Ensemble thoracique selon la revendication 5, dans lequel la partie incurvée vient en butée contre la partie linéaire, un premier bras extensible est relié à la partie incurvée et un connecteur d'électrode est fixé sur le premier bras extensible, une partie de transition vient en butée contre la partie incurvée et un connecteur d'électrode est fixé sur la partie de transition, un tronçon linéaire vient en butée contre la partie de transition et un connecteur d'électrode est fixé sur le tronçon linéaire, et un second bras extensible et un bras d'extension sont reliés au tronçon linéaire, un connecteur d'électrode est fixé sur le second bras d'extension et un connecteur d'électrode est fixé sur le second bras extensible. 65

7. Ensemble thoracique selon la revendication 3, dans lequel l'ensemble thoracique est relié à un émetteur de télémétrie via un ensemble adaptateur.
8. Ensemble thoracique selon la revendication 3, dans lequel l'ensemble thoracique est relié à un moniteur d'électrocardiogramme via un ensemble adaptateur. 5
9. Ensemble thoracique selon la revendication 3, dans lequel le connecteur d'ensemble thoracique inclut une pluralité d'éléments électriquement conducteurs suffisamment espacés pour empêcher la formation d'arc à travers les éléments électriquement conducteurs. 10
10. Ensemble thoracique selon la revendication 9, dans lequel le connecteur d'ensemble thoracique inclut une pluralité de nervures pour empêcher les éléments électriquement conducteurs d'entrer en contact avec des objets lorsque le connecteur d'ensemble thoracique n'est pas fixé à l'intérieur du bloc électronique corporel. 20
11. Ensemble thoracique selon la revendication 9, dans lequel les éléments électriquement conducteurs sont espacés pour permettre à l'ensemble thoracique de résister à un choc de défibrillation. 25
12. Ensemble thoracique selon la revendication 1, comprenant : 30
- une couche de base ayant une première face et une seconde face, la première face étant reliée à une pluralité d'éléments électriquement conducteurs, la seconde face étant reliée à une couche de blindage ; 35
- une première couche isolante positionnée au-dessus de la couche de base ; et une seconde couche isolante positionnée au-dessous de la couche de base. 40
13. Ensemble thoracique selon la revendication 12, dans lequel les éléments électriquement conducteurs sont reliés aux connecteurs d'électrode et à un connecteur d'ensemble thoracique. 45
14. Ensemble thoracique selon la revendication 12 ou 13, comprenant en outre une couche de blindage ayant une construction de grille à motif en X. 50
15. Ensemble thoracique selon la revendication 12, 13 ou 14, dans lequel la couche de blindage comprend une seule couche de matériau diélectrique. 55
16. Ensemble thoracique selon la revendication 12, 13 ou 14, dans lequel la couche de blindage comprend de multiples couches de matériau diélectrique.
17. Ensemble thoracique selon la revendication 1, dans lequel : 5
- l'ensemble thoracique est un ensemble précordial, 5
- la partie de retenue d'électrode est une partie de retenue d'électrode souple reliée au connecteur d'ensemble précordial par une partie linéaire, la partie de retenue d'électrode est reliée de manière amovible à une pluralité de connecteurs d'électrode, et la partie de retenue d'électrode comprend au moins un bras d'extension, une pluralité de parties incurvées, et une pluralité de segments de transition. 10
18. Ensemble thoracique selon la revendication 17, dans lequel une première partie incurvée vient en butée contre la partie linéaire, une première partie de transition vient en butée contre une première partie incurvée et un connecteur d'électrode est fixé sur le premier segment de transition, le bras d'extension est relié à la première partie de transition et un connecteur d'électrode est fixé au premier bras d'extension, une deuxième partie incurvée vient en butée contre la première partie de transition, une deuxième partie de transition vient en butée contre la deuxième partie incurvée et un connecteur d'électrode est fixé sur la deuxième partie de transition, un second bras d'extension est relié à la deuxième partie de transition et un connecteur d'électrode est fixé sur le second bras d'extension, une troisième partie incurvée vient en butée contre la deuxième partie de transition, un troisième segment de transition vient en butée contre la troisième partie incurvée et un connecteur d'électrode est fixé sur le troisième segment de transition, et une quatrième partie incurvée vient en butée contre le troisième segment de transition et un connecteur d'électrode est fixé sur la quatrième partie incurvée. 20
19. Ensemble thoracique selon la revendication 17 ou 18, dans lequel l'ensemble précordial est relié à un émetteur de télémétrie via un ensemble adaptateur. 25
20. Ensemble thoracique selon la revendication 17 ou 18, dans lequel l'ensemble précordial est relié à un moniteur d'électrocardiogramme via un ensemble adaptateur. 30
21. Ensemble thoracique selon l'une quelconque des revendications 17 à 20, dans lequel le connecteur d'ensemble précordial inclut une pluralité d'éléments électriquement conducteurs suffisamment espacés pour empêcher la formation d'arc à travers les éléments électriquement conducteurs. 35
22. Ensemble thoracique selon la revendication 21, dans lequel le connecteur d'ensemble précordial in-

- clut une pluralité de nervures pour empêcher les éléments électriquement conducteurs d'entrer en contact avec des objets lorsque le connecteur d'ensemble précordial n'est pas fixé à l'intérieur du bloc électronique corporel.
- 23.** Ensemble thoracique selon la revendication 21 ou 22, dans lequel le connecteur d'ensemble thoracique inclut une pluralité de brides à ressort et au moins une languette correspondant à au moins une gorge dans l'orifice d'ensemble thoracique. 10
- 24.** Ensemble thoracique selon la revendication 23, dans lequel les éléments électriquement conducteurs sont espacés pour permettre à l'ensemble précordial de résister à un choc de défibrillation. 15
- 25.** Bloc électronique corporel pour une utilisation dans un système de surveillance de l'activité cardiaque chez un patient, comprenant :
- un orifice d'ensemble thoracique pour recevoir de manière amovible un connecteur d'ensemble thoracique fixé sur un ensemble thoracique, le connecteur d'ensemble thoracique incluant une broche de capteur qui complète un circuit à l'intérieur du bloc électronique corporel lorsque le connecteur d'ensemble thoracique est inséré dans l'orifice d'ensemble thoracique, dans lequel des signaux électriques détectés en provenance du coeur d'un patient sont transmis au bloc électronique corporel via l'ensemble thoracique, dans lequel l'énergie du bloc électronique corporel est activée lorsque la broche de capteur complète le circuit à l'intérieur du bloc électronique corporel. 25
- 26.** Bloc électronique corporel selon la revendication 25, comprenant en outre une interface utilisateur pour communiquer des informations à un utilisateur. 40
- 27.** Bloc électronique corporel selon la revendication 26, dans lequel les informations concernent l'état de fonctionnement du système. 45
- 28.** Bloc électronique corporel selon la revendication 26 ou 27, dans lequel les informations concernent l'ordre d'appariement du bloc électronique corporel à une station de base. 50
- 29.** Bloc électronique corporel selon l'une quelconque des revendications 25 à 28, dans lequel le bloc électronique corporel peut exécuter une fonction sans fil pour surveiller en continu l'intégrité des connexions entre au moins un connecteur d'électrode fixé sur l'ensemble thoracique et au moins une électrode fixée sur le patient. 55
- 30.** Bloc électronique corporel selon l'une quelconque des revendications 25 à 29, dans lequel le bloc électronique corporel peut exécuter une fonction d'auto-test pour surveiller l'intégrité des fonctions du système. 5
- 31.** Bloc électronique corporel selon l'une quelconque des revendications 25 à 29, comprenant en outre une résistance reliée à l'orifice d'ensemble thoracique pour empêcher un courant électrique excessif de pénétrer dans le bloc électronique corporel, en permettant ainsi au bloc électronique corporel de résister à un choc de défibrillation.
- 32.** Bloc électronique corporel selon l'une quelconque des revendications 25 à 31, comprenant également au moins une batterie qui est compatible avec un orifice de batterie dans le bloc électronique corporel et un orifice de batterie dans une station de base.
- 33.** Bloc électronique corporel selon l'une quelconque des revendications 25 à 32, comprenant de plus un orifice destiné à recevoir un appareil pour apparier une station de base avec le bloc électronique corporel.
- 34.** Bloc électronique corporel selon la revendication 33, dans lequel l'appareil est une clef à jeton.
- 35.** Système de transmission sans fil de signaux physiologiques provenant d'un patient à un moniteur comprenant un ensemble thoracique tel que revendiqué dans l'une quelconque des revendications 1 à 24 et un bloc électronique corporel tel que revendiqué dans l'une quelconque des revendications 25 à 34, dans lequel l'ensemble thoracique et le bloc électronique corporel sont reliés au moyen du connecteur d'ensemble thoracique et de l'orifice d'ensemble thoracique.

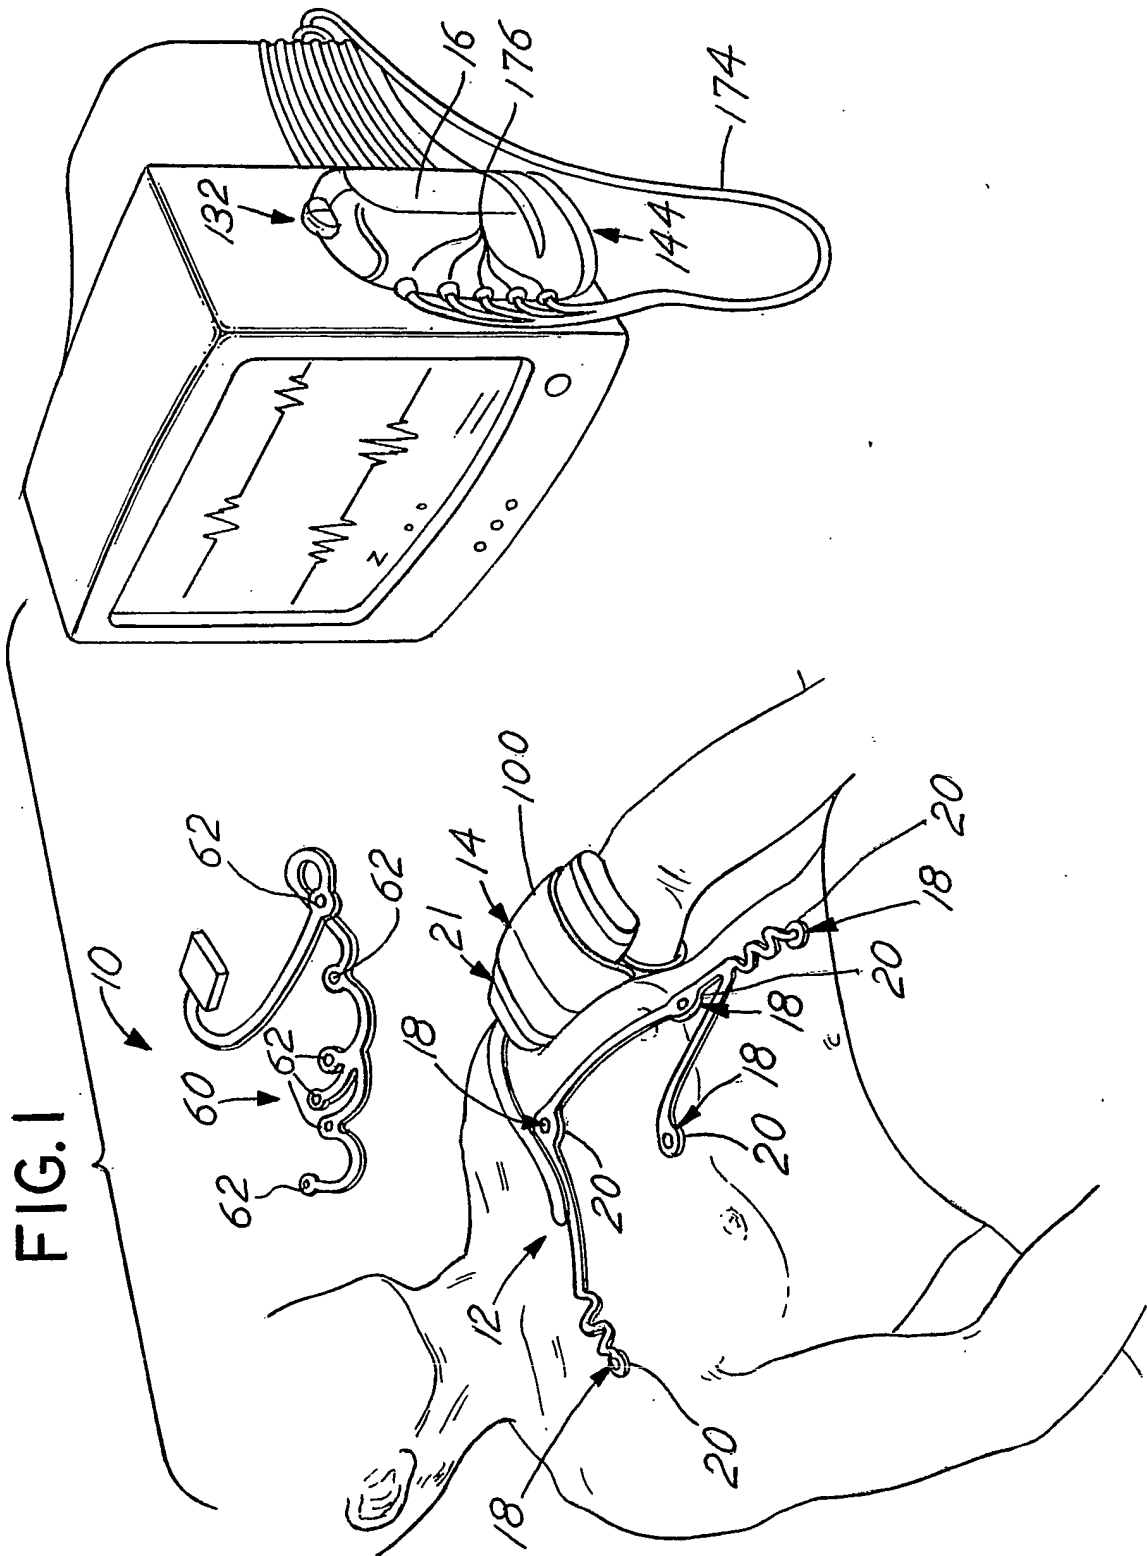


FIG.2

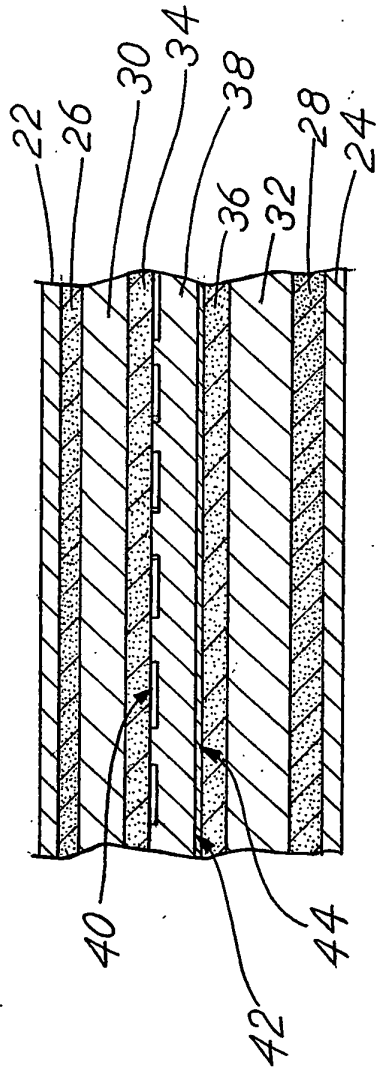


FIG.3

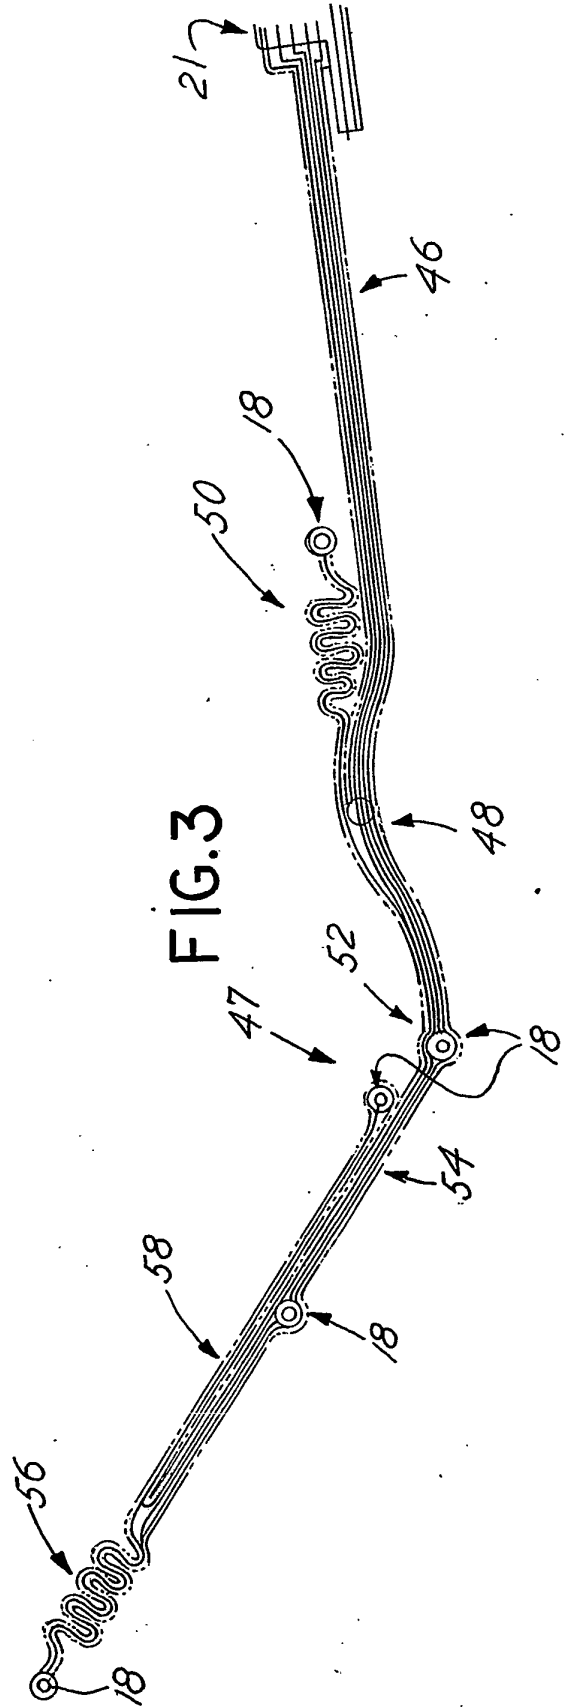


FIG. 4 60

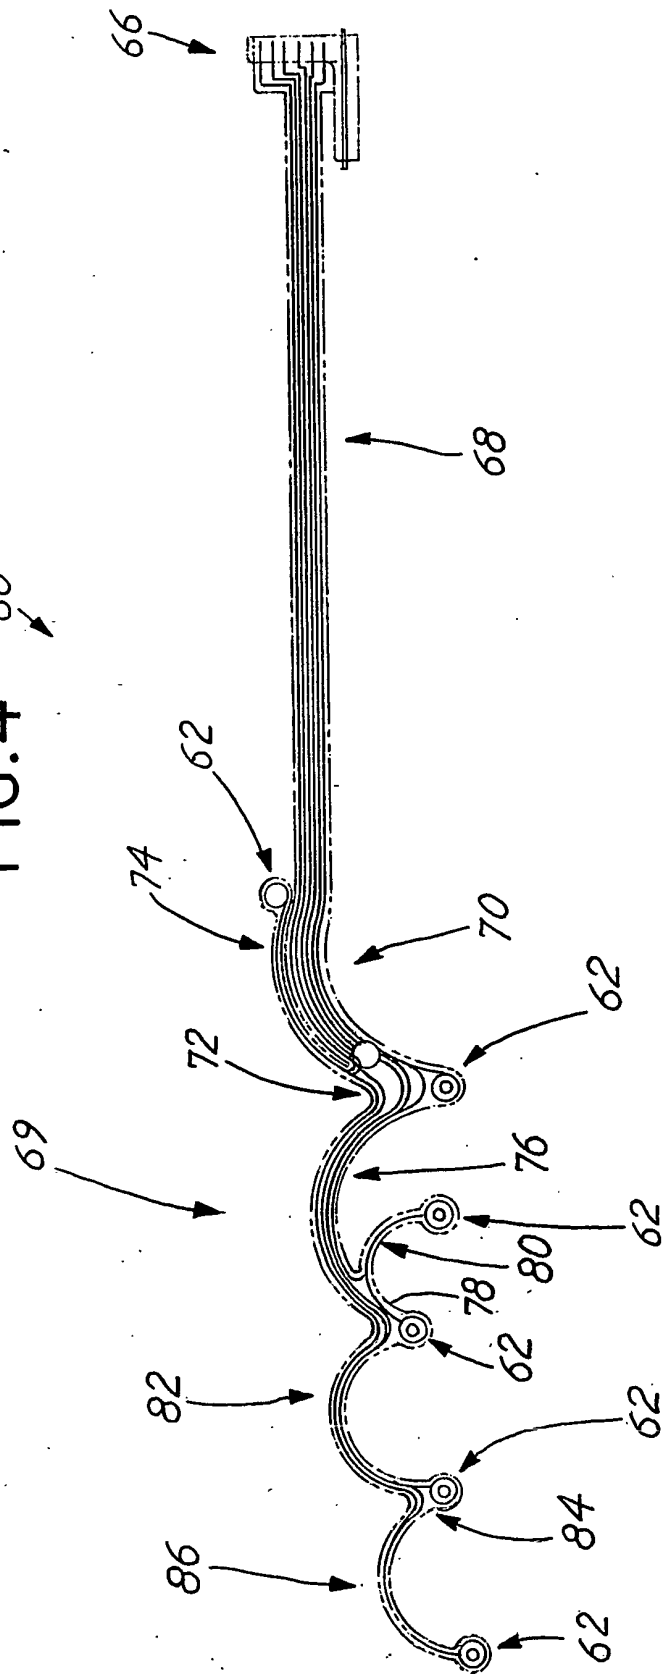


FIG.5

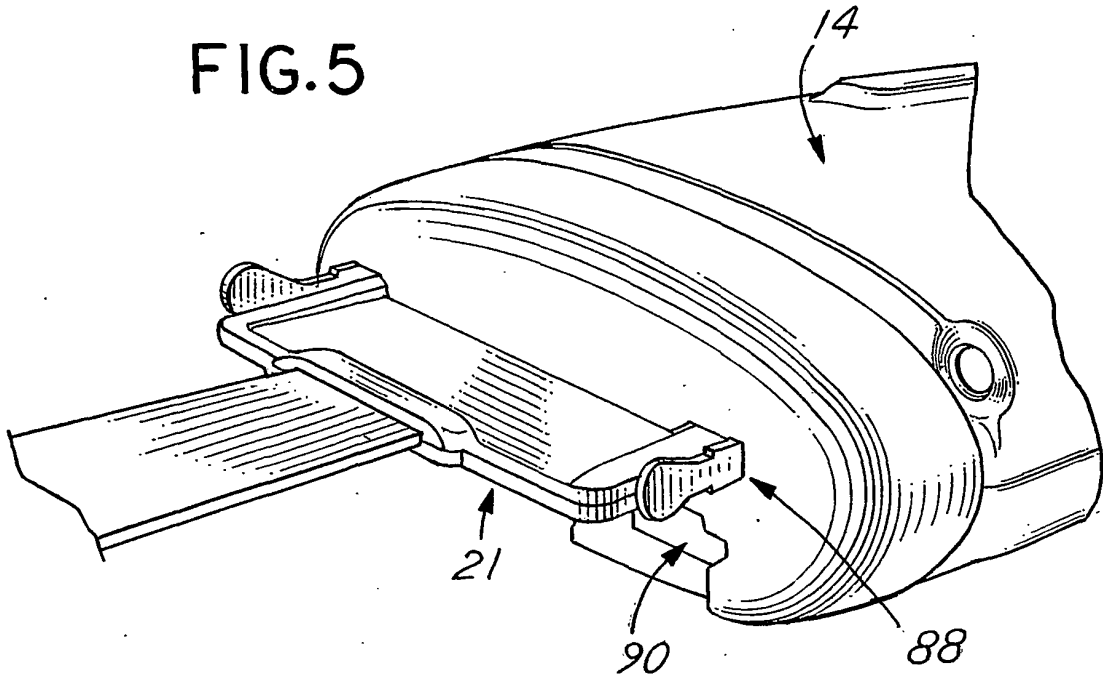


FIG.6

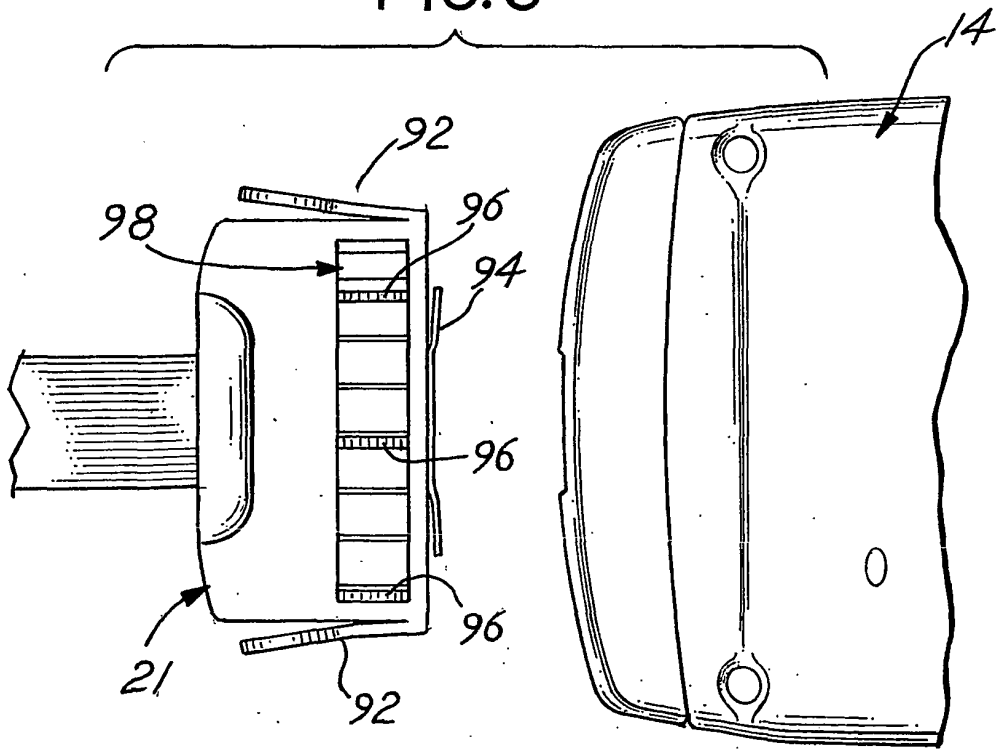


FIG.7

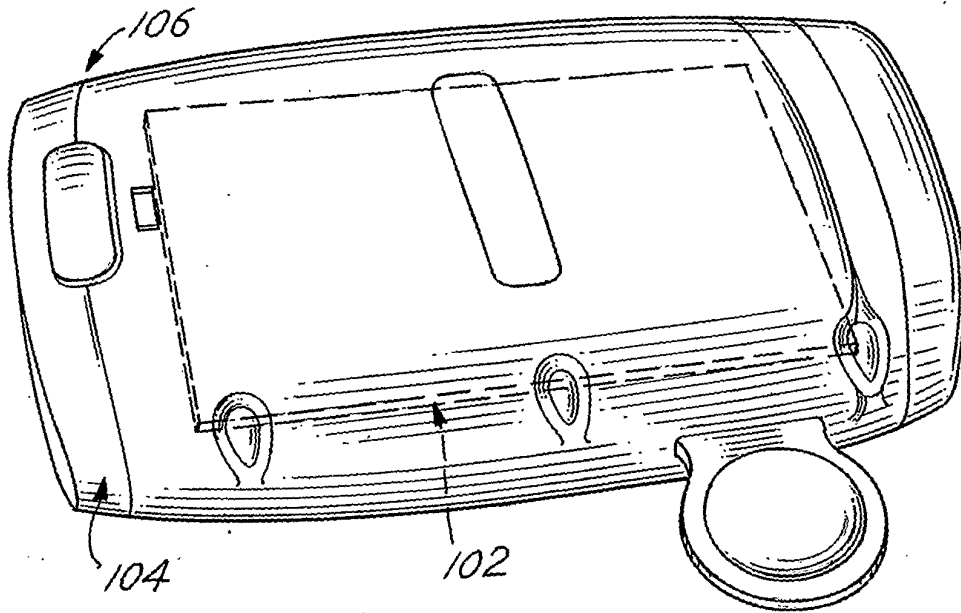


FIG.7A

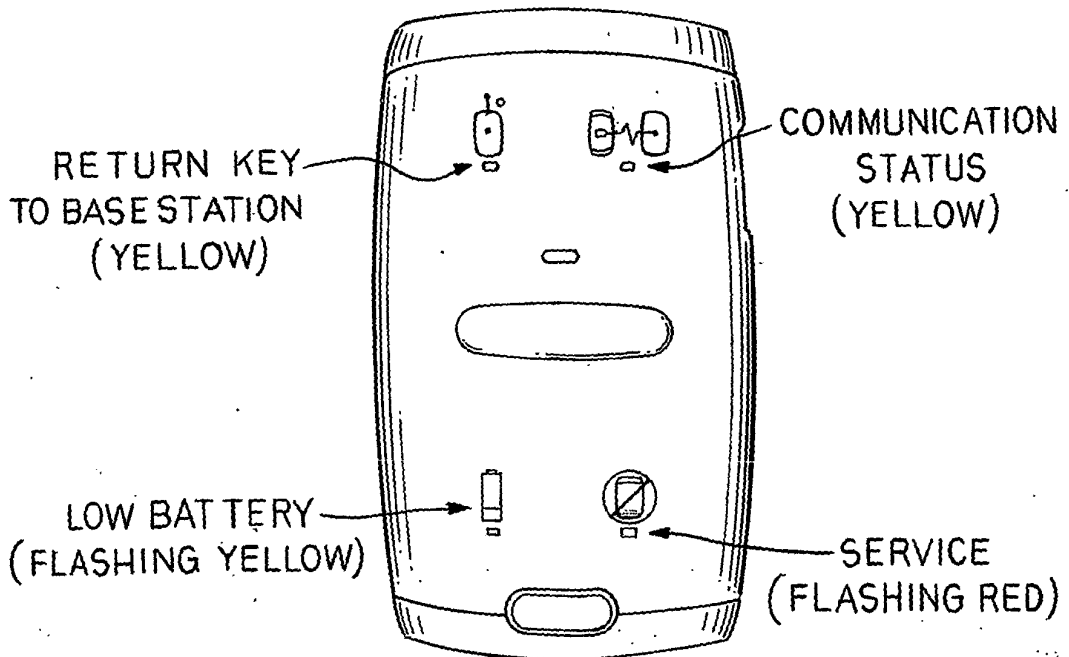
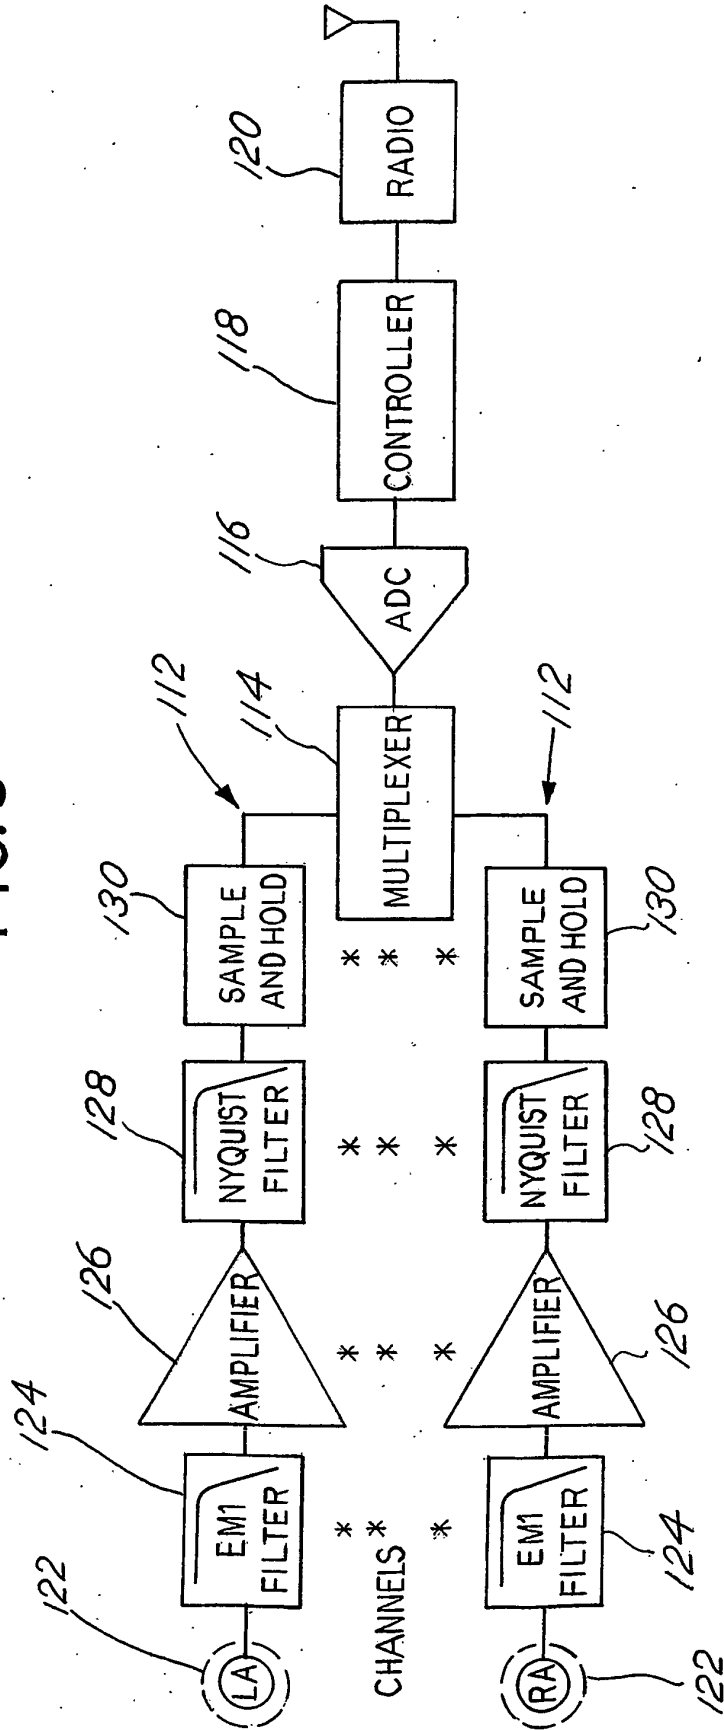


FIG. 8



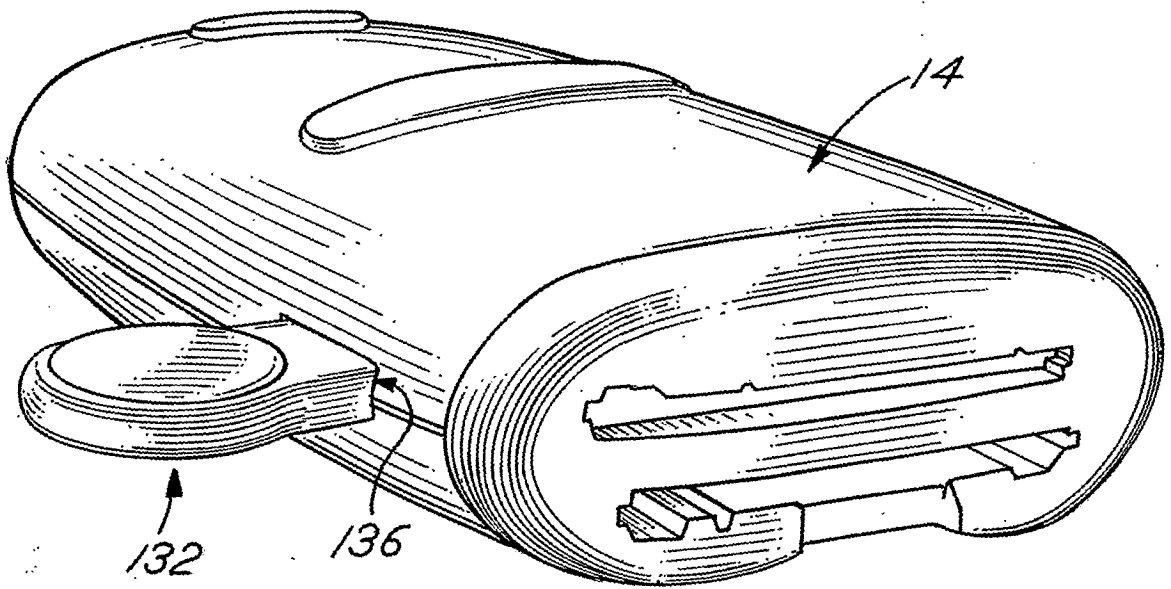
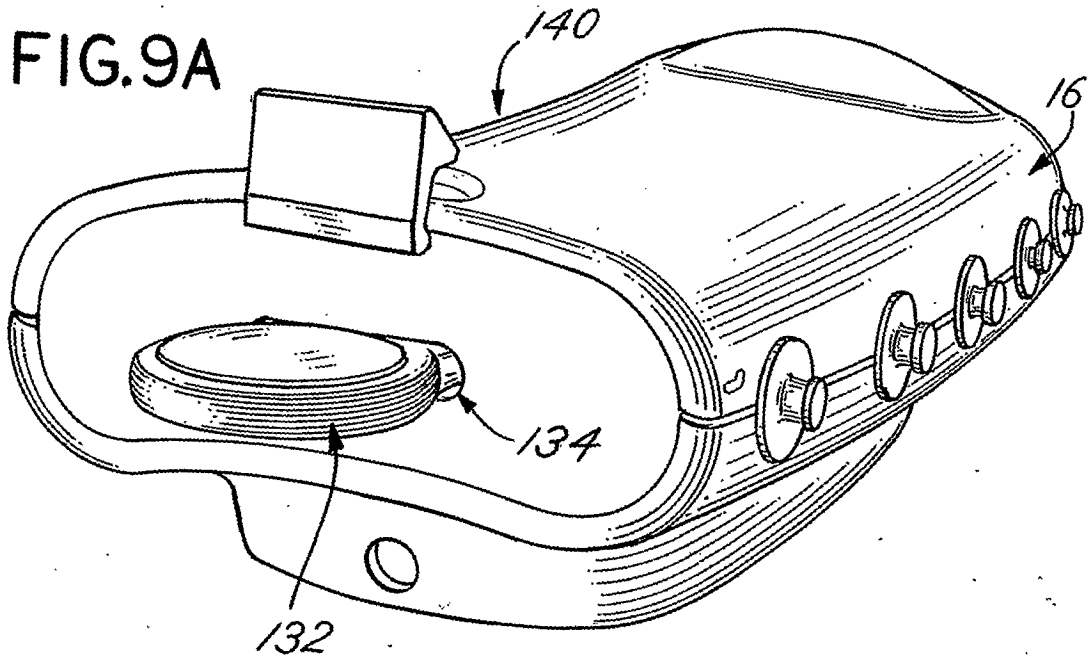


FIG.9B

FIG.10

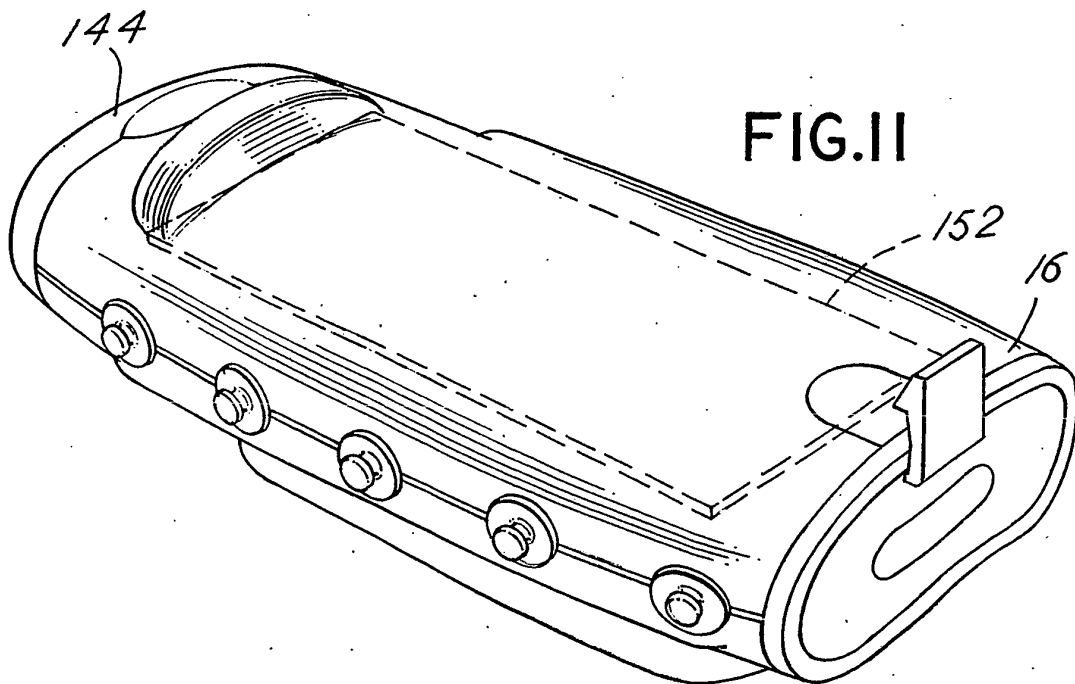
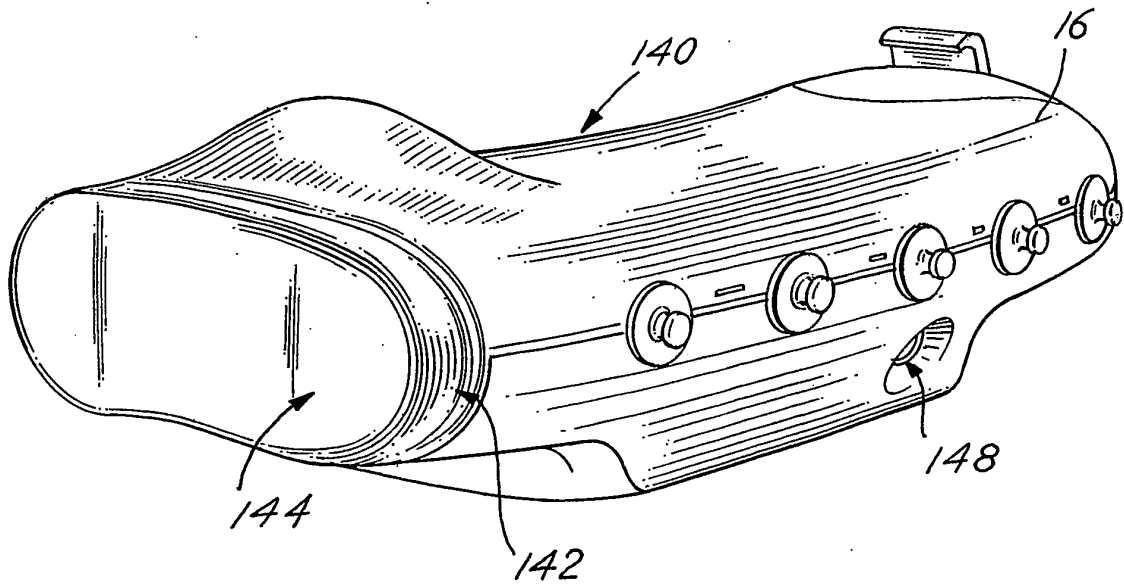


FIG. IIA

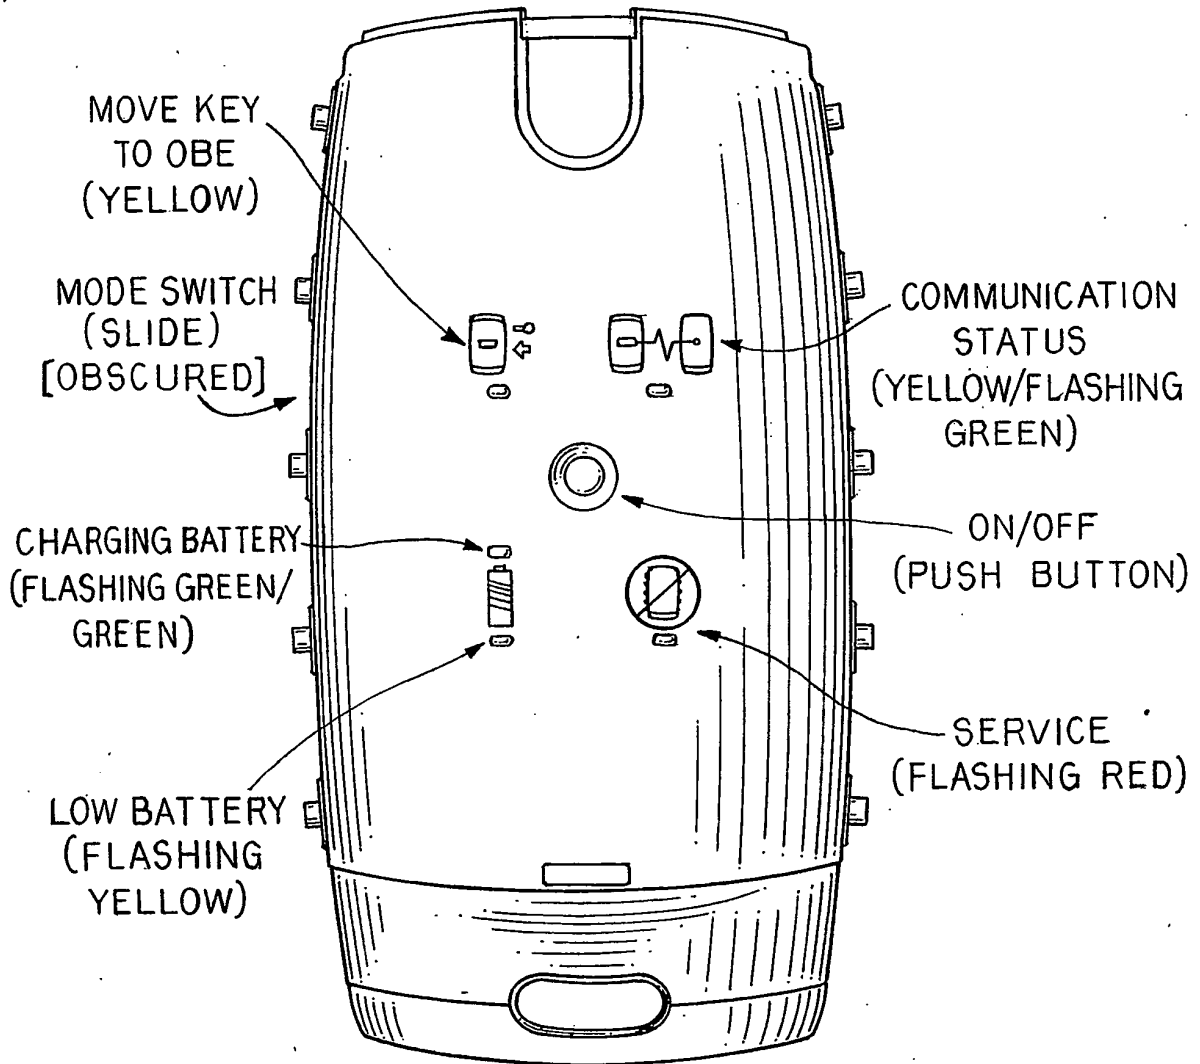


FIG.12

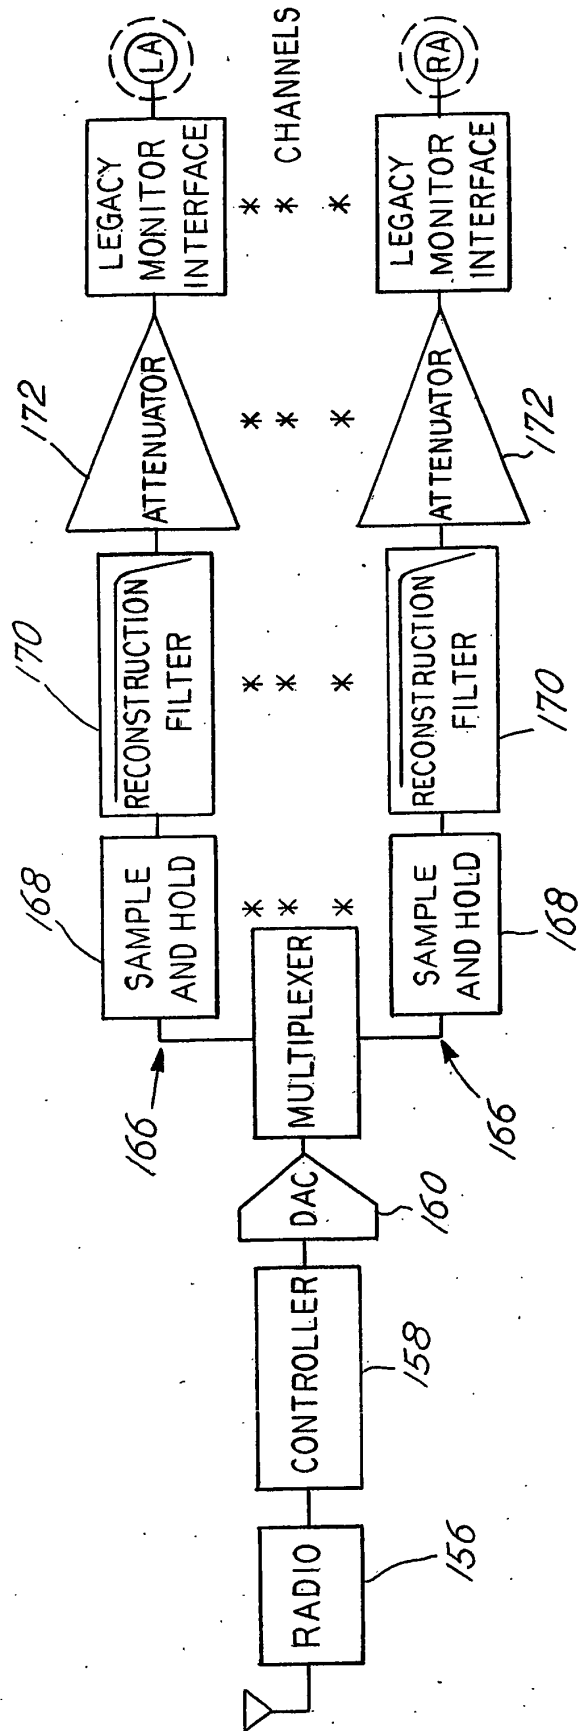
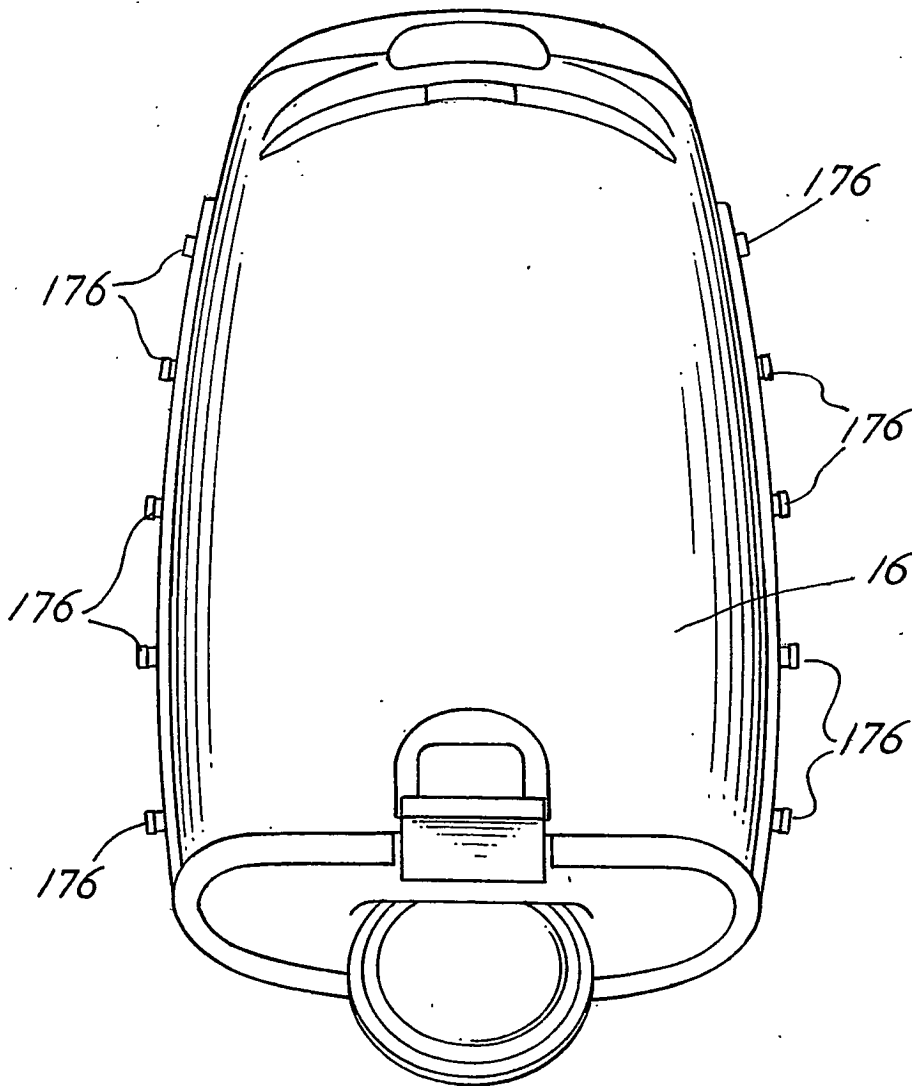


FIG. 13



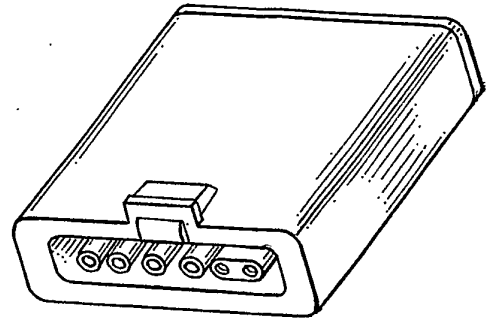
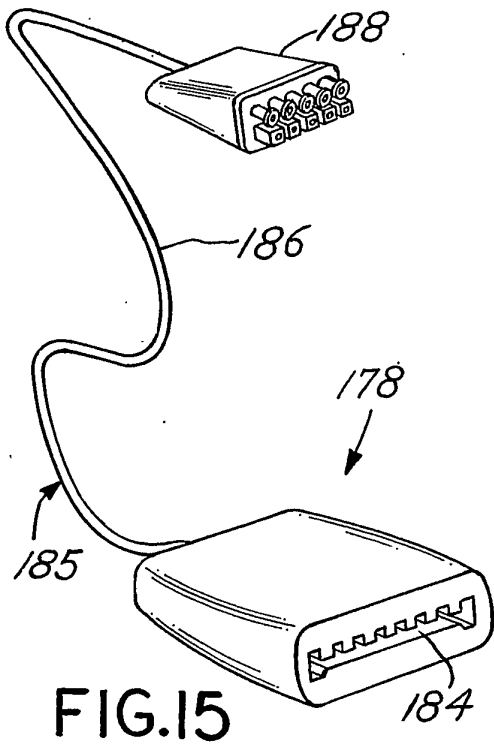


FIG. 14

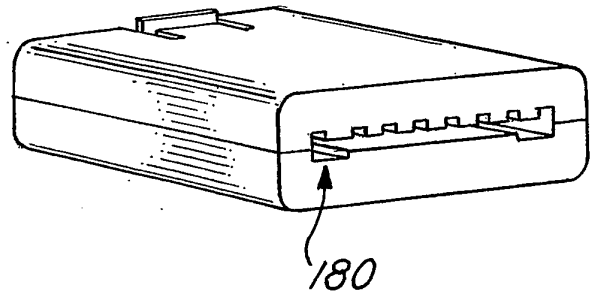


FIG. 16


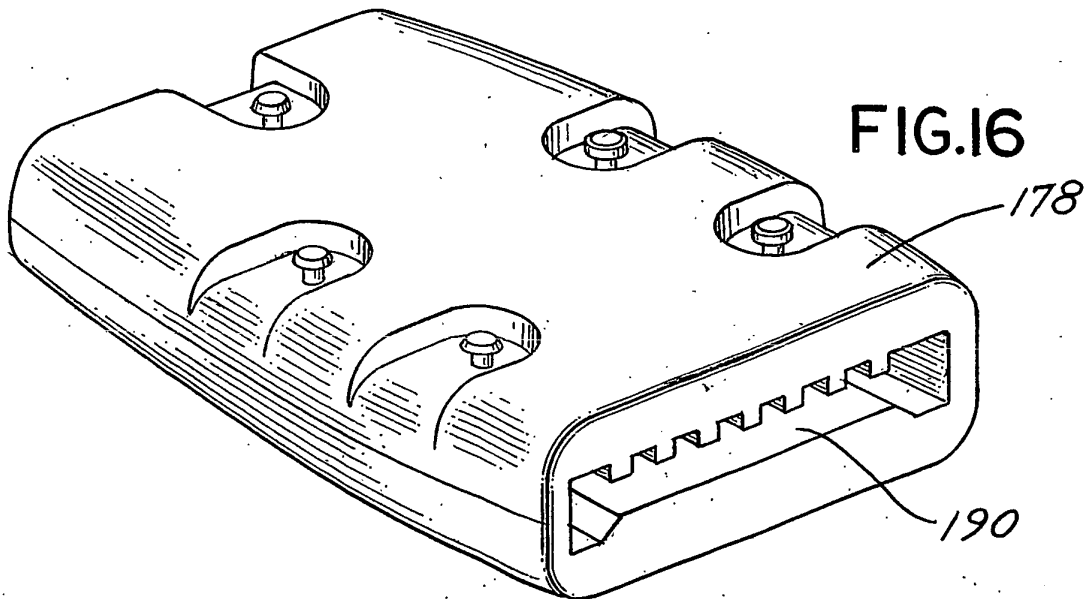


FIG.17

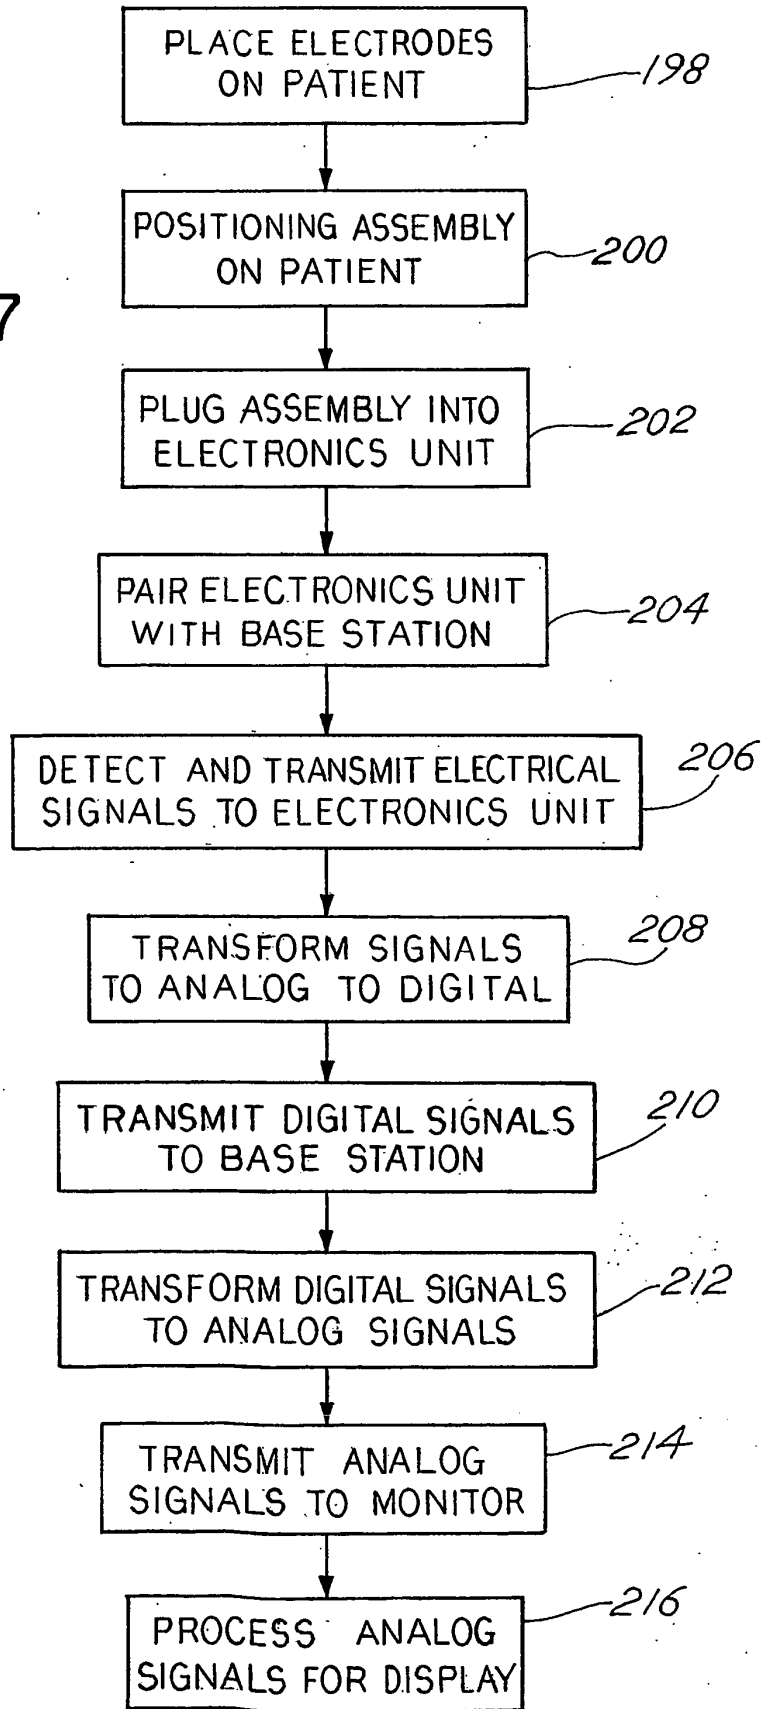

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 99873301 A [0002]

专利名称(译)	无线心电图系统		
公开(公告)号	EP1467651B1	公开(公告)日	2008-10-29
申请号	EP2002794057	申请日	2002-11-26
[标]申请(专利权)人(译)	GMP WIRELESS医药		
申请(专利权)人(译)	GMP WIRELESS医药, INC.		
当前申请(专利权)人(译)	LIFESYNC CORPORATION		
[标]发明人	ISTVAN RUD GREGORY BILL SOLOVAY KENNETH CHASTAIN DAVID PAUL GUNDLACH JOHN DAVID HOPMAN NICHOLAS C WILLIAMS DANIEL L LODATO FRANCO SALEM MICHAEL		
发明人	ISTVAN, RUD GREGORY, BILL SOLOVAY, KENNETH CHASTAIN, DAVID, PAUL GUNDLACH, JOHN, DAVID HOPMAN, NICHOLAS, C. WILLIAMS, DANIEL, L. LODATO, FRANCO SALEM, MICHAEL		
IPC分类号	A61B5/0245 A61B5/00 A61B5/0408		
CPC分类号	A61B5/0006 A61B5/04085		
代理机构(译)	杰克逊, 罗伯特·帕特里克		
优先权	10/998733 2001-11-30 US		
其他公开文献	EP1467651A2		
外部链接	Espacenet		

摘要(译)

心脏监测系统, 更具体地, 无线心电图 (ECG) 系统。本发明检测来自患者心脏的电信号, 并通过遥测技术将信号数字地发送到远程基站。基站将数字信号转换回可由ECG监视器读取的模拟电信号。

