



(11) **EP 1 757 224 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
05.01.2011 Bulletin 2011/01

(51) Int Cl.:
A61B 5/00 (2006.01)

(21) Application number: **06017637.7**

(22) Date of filing: **24.08.2006**

(54) **Apparatus and method for measuring oxygen saturation in blood**

Vorrichtung und Methode zur Bestimmung der Sauerstoffsättigung von Blut

Dispositif et procédé de mesure de la saturation en oxygene du sang

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI SK TR

(30) Priority: **24.08.2005 JP 2005242574**
28.07.2006 JP 2006205453

(43) Date of publication of application:
28.02.2007 Bulletin 2007/09

(73) Proprietor: **Nihon Kohden Corporation**
Shinjuku-ku
Tokyo (JP)

(72) Inventors:
• **Kobayashi, Naoki**
Shinjuku-ku
Tokyo (JP)

- **Miyata, Kenji**
Shinjuku-ku
Tokyo (JP)
- **Yarita, Masaru**
Shinjuku-ku
Tokyo (JP)
- **Ito, Kazumasa**
Shinjuku-ku
Tokyo (JP)

(74) Representative: **Grünecker, Kinkeldey, Stockmair & Schwanhäusser**
Anwaltssozietät
Leopoldstrasse 4
80802 München (DE)

(56) References cited:
US-A- 4 934 372 **US-A1- 2004 059 209**
US-A1- 2004 267 140 **US-A1- 2005 033 129**

EP 1 757 224 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionBACKGROUND OF THE INVENTION

5 **[0001]** The present invention relates to signal processing in a pulse oximeter used in a patient monitoring or for diagnosing a respiratory system or a circulatory system.

[0002] Various methods have been proposed to separate a signal component and a noise component from two signals substantially simultaneously extracted from a single medium. The methods are usually conducted by performing processing in a frequency region and a time region.

10 **[0003]** In medical fields, it is known a pulse photometer including: an apparatus called a photoplethysmograph for measuring a pulse waveform and a pulse rate; and an apparatus for measuring the concentration of a light absorbing material in blood such as an apparatus for measuring an oxygen saturation in blood (SpO₂), an apparatus for measuring the concentration of abnormal hemoglobins such as carboxyhemoglobin and methemoglobin, and an apparatus for measuring the concentration of an injected dye. Particularly, the apparatus for measuring the SpO₂ is called a pulse
15 oximeter.

[0004] The principle of the pulse photometer is to determine the concentration of an object material from a pulse wave signal obtained by causing a living tissue to transmit or reflect light beams, which have a plurality of wavelengths respectively correspond to different absorbances of the object material, and by continuously measuring an intensity of transmitted or reflected light. In a case where noise are superimposed on pulse wave data, calculation of a correct
20 concentration or pulse rate cannot be achieved. Consequently, there is an anxious that an erroneous treatment may be performed.

[0005] There is proposed a method performed in the pulse photometer, in which pulse wave signals are divided into a plurality of frequency bands and a correlation between the signals is examined in each of the divided frequency bands to reduce noises. However, this method has a problem in that analysis is time-consuming.

25 **[0006]** Japanese Patent No. 3270917 discloses a method comprising: irradiating light beams respectively having different wavelengths onto a living tissue; drawing a graph in which the longitudinal axis and the transverse axis thereof respectively represent the magnitudes of two signals obtained from transmitted light; and obtaining a regression line to thereby obtain an oxygen saturation or the concentration of a light absorbing material in arterial blood according to the gradient of the regression line.

30 **[0007]** However, a large amount of calculation is needed to obtain a regression line and the gradient thereof by using a great amount of sampling-data on each of the pulse wave signals.

[0008] Japanese Patent Publication No. 2003-135434A discloses a method of using frequency analysis, in which the fundamental frequency of a pulse wave signal is obtained instead of conventional extraction of the pulse wave signal itself, and the pulse wave signal is filtered by using a filter employing a higher harmonic wave frequency to enhance
35 accuracy. Japanese Patent Publication Nos. 2005-95581A and 2005-245574A disclose a method for separating noise from a pulse wave signal.

[0009] However, in a case where noise due to a body movement of a patient, whose amplitude is about ten times that of the pulse wave, is superimposed on a pulse wave signal, it is difficult according to any of these methods to compute a pulse rate and an oxygen saturation in arterial blood. Thus, a further improvement in signal processing is desired.

40 **[0010]** US 4,934,372 A discloses a method and apparatus for detecting optical pulses, whereby the collected optical signals are converted into the frequency domain, and the spectral components of the frequency spectrum are analyzed, thereby determining the red and infrared relative maximum intensity at the fundamental frequency, and relative minima at the background intensity zero frequency. These are used as maxima and minima in the percentage modulation ratio for calculating oxygen saturation. In the analyzing process, the oxygen saturation is calculated from red and infrared
45 relative maximum intensity at the fundamental frequency and relative minima at the background intensity zero frequency.

SUMMARY OF THE INVENTION

50 **[0011]** It is therefore an object of the invention to provide a signal processing method enabled to alleviate load calculation for extracting a common signal component by processing two signals of a same kind, which are substantially simultaneously extracted from a same medium.

[0012] It is also an object of the invention to measure the oxygen saturation of an object material with high accuracy by applying the signal processing method even when noise due to the body movement of the medium is superimposed on a pulse wave signal, thereby obtaining a pulse rate with high precision.

55 **[0013]** In order to achieve the above objects, according to the invention, there is provided an apparatus for measuring an oxygen saturation in blood, comprising:

a plurality of light emitters, adapted to irradiate a living tissue with a plurality of light beams having different wave-

lengths;

a light receiver, adapted to receive the light beams reflected from or transmitted through the living tissue to generate pulse wave signals in accordance with pulsations of the blood in the living tissue;

a separator, operable to separate each of the pulse wave signals into a plurality of amplitude signals each of which is associated with one frequency, thereby generating pairs of amplitude signals each of which is associated with one of a plurality of frequencies;

a first processor, operable to calculate a ratio between the amplitude signals in each of the pairs of the amplitude signals;

a selector, operable to select one of the pairs of the amplitude signals; and

a second processor, operable to calculate the oxygen saturation based on the ratio of the selected one of the pairs of the amplitude signals.

[0014] The separator may comprise either an FFT processor or a digital filter.

[0015] The selector may be operable to select such a pair of the amplitude signals that have maximum amplitude values.

[0016] The selector may be operable to select such a pair of the amplitude signals that the ratio takes a minimum value.

[0017] The first processor may comprise: a first calculator, operable to define a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals, and operable to calculate an average value of the amplitude signals in each of the frequency bands, thereby generating pairs of average values each of which is associated with one of the frequency bands; and a second calculator, operable to calculate an average ratio between the average values in each of the pairs of the average values. The selector may be operable to select such a frequency band that the average ratio takes a minimum value.

[0018] The apparatus first processor may comprise: a first calculator, operable to: define a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals; judge whether there is a maximal point of the amplitude signals in each of the frequency bands; and calculate an average value of the amplitude signals in at least one of the frequency bands which is judged as one including the maximal point, thereby at least one pair of average values each of which is associated with one of the frequency bands; and a second calculator, operable to calculate an average ratio between the average values in each of the at least one pair of the average values. The selector may be operable to select such a frequency band that the average ratio takes a minimum value.

[0019] The first processor may comprise: a first calculator, operable to calculate ratios each of which is a ratio between each of the pairs of the amplitude signals; and a second calculator, operable to define a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals, and operable to calculate an average value of the ratios in each of the frequency bands, thereby generating a plurality of average values. The selector may be operable to select such a frequency band that the average value takes a minimum value.

[0020] A part of one of the frequency bands may be overlapped with a part of another one of the frequency bands.

[0021] The selector may be operable to select either such a pair of the amplitude signals that have maximum amplitude values or such a pair of the amplitude signals that the ratio takes a minimum value in accordance with a prescribed condition.

[0022] The prescribed condition may include a waveform of the amplitude signals.

[0023] The light beams may include a red light beam and an infrared light beam.

[0024] According to the invention, there is also provided a method for measuring an oxygen saturation in blood, comprising:

irradiating a living tissue with a plurality of light beams having different wavelengths;

receiving the light beams reflected from or transmitted through the living tissue to generate pulse wave signals in accordance with pulsations of the blood in the living tissue;

separating each of the pulse wave signals into a plurality of amplitude signals each of which is associated with one frequency, thereby generating pairs of amplitude signals each of which is associated with one of a plurality of frequencies;

calculating a ratio between the amplitude signals in each of the pairs of the amplitude signals;

selecting one of the pairs of the amplitude signals; and

calculating the oxygen saturation based on the ratio of the selected one of the pairs of the amplitude signals.

[0025] The separating may be performed with either an FFT processing or a digital filtering.

[0026] Such a pair of the amplitude signals that have maximum amplitude values may be selected as the one of the pairs of the amplitude signals.

[0027] Such a pair of the amplitude signals that the ratio takes a minimum value may be selected as the one of the pairs of the amplitude signals.

[0028] The method may further comprise:

defining a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals;
 calculating an average value of the amplitude signals in each of the frequency bands, thereby generating pairs of average values each of which is associated with one of the frequency bands;
 5 calculating an average ratio between the average values in each of the pairs of the average values; and
 selecting such a frequency band that the average ratio takes a minimum value.

[0029] The method may further comprise:

10 defining a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals;
 judging whether there is a maximal point of the amplitude signals in each of the frequency bands;
 calculating an average value of the amplitude signals in at least one of the frequency bands which is judged as one including the maximal point, thereby at least one pair of average values each of which is associated with one of the
 15 frequency bands;
 calculating an average ratio between the average values in each of the at least one pair of the average values; and
 selecting such a frequency band that the average ratio takes a minimum value.

[0030] The method may further comprise:

20 calculating ratios each of which is a ratio between each of the pairs of the amplitude signals;
 defining a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals;
 calculating an average value of the ratios in each of the frequency bands, thereby generating a plurality of average
 25 values; and
 selecting such a frequency band that the average value takes a minimum value.

[0031] A part of one of the frequency bands may be overlapped with a part of another one of the frequency bands.

[0032] Either such a pair of the amplitude signals that have maximum amplitude values or such a pair of the amplitude signals that the ratio takes a minimum value may be selected as the one of the pairs of the amplitude signals in accordance with a prescribed condition.

[0033] The prescribed condition may include a waveform of the amplitude signals.

BRIEF DESCRIPTION OF THE DRAWINGS

[0034] The above objects and advantages of the present invention will become more apparent by describing in detail preferred exemplary embodiments thereof with reference to the accompanying drawings, wherein:

Fig. 1 is a block diagram schematically showing a pulse oximeter;
 40 Fig. 2A is a graph showing attenuation change signals obtained from pulse wave signals measured by the pulse oximeter, in a case where no noise is superimposed;
 Fig. 2B is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 2A;
 Fig. 2C is a graph showing a ratio between amplitudes of the spectra shown in Fig. 2B;
 45 Fig. 3A is a graph showing attenuation change signals obtained from pulse wave signals pulse wave signals measured by the pulse oximeter, in a case where noise is superimposed thereon;
 Fig. 3B is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 3A;
 Fig. 3C is a graph showing a ratio between amplitudes of the spectra shown in Fig. 3B, for explaining a signal
 50 processing according to a first embodiment of the invention;
 Fig. 3D is a graph showing the ratio between amplitudes of the spectra shown in Fig. 3B, for explaining a signal processing according to a second embodiment of the invention;
 Fig. 4A is a graph showing attenuation change signals obtained from pulse wave signals measured by the pulse
 55 oximeter, in a case where large noise is superimposed;
 Fig. 4B is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 4A;
 Fig. 4C is a graph showing attenuation change signals obtained from pulse wave signals measured by the pulse oximeter, in a case where a signal separation method is applied;

Fig. 4D is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 4C;

Fig. 4E is a graph showing a ratio between amplitudes of the spectra shown in Fig. 4D;

Fig. 5A is a graph showing attenuation change signals obtained from pulse wave signals measured by the pulse oximeter, in a case where extreme large noise is superimposed;

Fig. 5B is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 5A;

Fig. 5C is a graph showing attenuation change signals obtained from pulse wave signals measured by the pulse oximeter, in a case where a signal separation method is applied;

Fig. 5D is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 5C;

Fig. 5E is a graph showing a ratio between amplitudes of the spectra shown in Fig. 5D;

Fig. 6 is a graph showing an actual measurement example;

Fig. 7A is a diagram showing a blood pulsation model in a case where no body movement is present;

Fig. 7B is a diagram showing the blood pulsation model in a case where a body movement is present;

Fig. 8 is a diagram showing a vector representation of attenuation ratios derived from the model shown in Fig. 7B;

Fig. 9 is a diagram showing a correlation between the attenuation ratio and an oxygen saturation in blood;

Fig. 10A is a graph showing attenuation change signals obtained from pulse wave signals pulse wave signals measured by the pulse oximeter, in a case where noise is superimposed thereon;

Fig. 10B is a graph showing amplitude spectra obtained by applying a FFT processing with respect to the pulse wave signals shown in Fig. 10A, for explaining a third embodiment of the invention;

Fig. 10C is a graph showing values each of which is an average value of amplitudes in each of divided frequency bands shown in Fig. 10B; and

Fig. 10D is a graph showing values each of which is a ratio between the average values shown in Fig. 10C in each of the divided frequency bands.

DETAILED DESCRIPTION OF THE EMBODIMENTS

[0035] Embodiments of the invention will be described below in detail with reference to the accompanying drawings.

[0036] As shown in Fig. 1, in a pulse oximeter of the invention, light emitters 1 a (LED R) and 1b (LED IR) are driven by a first LED driver 2a, a second LED driver 2b and an LED selector 3 to alternately emit light.

[0037] Preferably, light emitted from the light emitter 1 a is red light (for example, the wavelength is 660nm), which is highly sensitive to change in the oxygen saturation in arterial blood, and light emitted from the light emitter 1 b is infrared light (for example, the wavelength is 940nm), which is less sensitive to the change in the oxygen saturation in arterial blood.

[0038] Light beams coming from these light emitters 1 a and 1b are transmitted (or reflected) by a living tissue 12 and are subsequently received by a photodiode 8 that converts the received light to photoelectric current. Then, a current-voltage converter 9 converts the photoelectric current to a voltage signal that is outputted to an A/D converter 11 through a pulse wave demodulator 10.

[0039] An LED selection signal is applied from the LED selector 3 to the pulse wave demodulator 10 as a timing signal. Thus, the red light and the infrared light received by the single photodiode 8 are extracted as separate pulse wave signals.

[0040] Pulse wave signals digitalized by the A/D converter 11 are processed by a CPU (adapted to perform computing, processing, and control). The digital pulse wave signals are displayed on a display 5 and are recorded in a recorder 6.

[0041] A control panel 7 is operative to perform the setting for performing processing in the CPU.

[0042] Each of pulse waves respectively corresponding to red light R and infrared light IR is separated into an AC component and a DC component by filtering. In addition, the ratio AC/DC of the magnitude of the AC component to that of the DC component is calculated corresponding to each of the pulse waves R and IR to thereby calculate signals representing attenuation changes ΔA .

[0043] The magnitude of the AC component in the pulse wave for the red light R is denoted as $R_AC(t)$. The magnitude of the DC component in the pulse wave for the red light R is denoted as $R_DC(t)$. The magnitude of the AC component in the pulse wave for the infrared light IR is denoted as $IR_AC(t)$. The magnitude of the DC component in the pulse wave for the infrared light IR is denoted as $IR_DC(t)$.

[0044] Thus, the attenuation change signal for the red light R is expressed by $\Delta Ar(t) = R_AC(t) / R_DC(t)$, and the attenuation change signal for the infrared light IR is expressed by $\Delta Air(t) = IR_AC(t) / IR_DC(t)$. Fig. 2A shows these attenuation change signals.

[0045] Fig. 2B shows amplitude spectra obtained after FFT processing is performed on the pulse waves shown in Fig. 2A. The amplitude spectrum corresponding to $\Delta Ar(t)$ is denoted as $R_F, FT(f)$ and the amplitude spectrum corresponding to $\Delta Air(t)$ is denoted as $IR_FFT(f)$. Because no noise are superimposed on the pulse waves, each of the amplitude spectra shows a maximum value at a frequency of the pulse wave.

[0046] Fig. 2C shows a ratio between the amplitudes of the spectra shown in Fig. 2B ($R_FFT(f) / IR_FFT(f)$). This ratio represents an attenuation ratio Φ at each frequency of the spectra. Thus, the attenuation ratio Φ can be expressed by $\Phi(f) = R_FFT(f) / IR_FFT(f)$.

[0047] When the frequency resolution of FFT is 0.1 Hz, $\Phi(f)$ is computed by separating the pulse wave into frequencies at intervals of 0.1 Hz.

[0048] Figs. 2A to 2C illustrate a case where no noise are superimposed on the pulse wave. However, in the case of actually measured pulse wave, the attenuation ratio Φ includes Φ_s which corresponds to the attenuation changes in arterial blood, and Φ_n which corresponds to the attenuation changes of noise.

[0049] In a first embodiment of the invention, the attenuation ratios Φ are calculated for a plurality of frequencies, and the attenuation ratio Φ at a frequency f_{max} , at which the amplitude of each of the spectra becomes maximum, is set to be the attenuation ratio Φ_s of arterial blood.

[0050] Figs. 3A to 3C respectively correspond to Figs. 2A to 2C and are showing a case where noise is superimposed on the pulse wave signals.

[0051] In comparison with the waveforms shown in Fig. 2B, it is apparent that, in Fig. 3B, peaks due to the noise appear at frequencies other than the frequency of the pulse wave.

[0052] In a case where the amplitude due to the noise is relatively smaller than the amplitude of the pulse wave signal (e.g., in a case where the ratio of the amplitude due to the noise to the amplitude of the pulse wave signal is no greater than 0.7, preferably, no greater than 0.5), the attenuation ratio Φ at the frequency, at which each of the amplitude spectra shows a maximum value, is read and is determined to be the attenuation ratio Φ_s of arterial blood as shown in Fig. 3C. Thus, the attenuation ratio Φ_s of arterial blood can easily be obtained.

[0053] In a second embodiment of the invention, the attenuation ratios Φ are calculated for a plurality of frequencies, and a minimum value of the attenuation ratios Φ is set to be the attenuation ratio Φ_s of arterial blood.

[0054] Generally, the attenuation ratio Φ_n in the frequency, at which the amplitude due to noise appears, tends to be higher than the attenuation ratio Φ_s in the frequency at which the amplitude due to the pulse wave appears.

[0055] This is because of the fact that the change in the attenuation ratio, which is caused by the noise, results mainly from change in the thickness of venous blood. Because the oxygen saturation in venous blood is lower than that of arterial blood, the attenuation ratio Φ_n due to the change in thickness of venous blood is lower than the attenuation ratio Φ_s . Therefore, the minimum value of the attenuation ratios Φ can be read as the attenuation ratio Φ_s of arterial blood. Fig. 3D shows this processing.

[0056] It is apparent that the ratio Φ_s obtained by this processing is almost the same as that obtained by the processing illustrated in Fig. 3C. Here, the ratio Φ_s obtained by this processing may be taken into account of the judgment performed in the first embodiment.

[0057] In a case where the frequency, at which the amplitude peak due to the noise appears, overlaps with the frequency, at which the amplitude peak due to the pulse wave appears, the attenuation ratio Φ obtained at such a frequency becomes lower than the actual attenuation ratio Φ_s of arterial blood. Thus, the SpO_2 cannot correctly be measured when the attenuation ratio Φ obtained at the above frequency is employed. In such a case, a second-minimum attenuation ratio Φ obtained at a frequency other than the above frequency may be regarded as that Φ_s of arterial blood.

[0058] Next, grounds for the above determination will be described below by using a model in which arterial blood pulsates and increases in thickness when no body movement is present with reference to Fig. 7A, and in which the thickness of arterial blood and that of venous blood simultaneously change when a body movement is present with reference to Fig. 7B.

[0059] In the case illustrated in Fig. 7A, the attenuation change ΔA is measured according to Lambert-Beer's law as follows.

$$\Delta A = \Delta A_a = E_a \cdot H_b \cdot \Delta D_a$$

where A_a designates an attenuation change caused by change in the thickness of arterial blood; E_a designates an absorption coefficient of arterial blood (dL/g/cm); H_b denotes a hemoglobin concentration (g/dL); and ΔD_a designates change in the thickness of arterial blood (cm). The attenuation ratio Φ to be measured is given by the following equation.

$$\Phi = \Delta A_1 / \Delta A_2 = (E_{a1} \cdot H_b \cdot \Delta D_a) / (E_{a2} \cdot H_b \cdot \Delta D_a) = E_{a1} / E_{a2}$$

where the suffixes designate wavelength numbers, and the suffix 1 corresponds to a wavelength of 660nm, and the

suffix 2 corresponds to a wavelength of 940nm.

[0060] The attenuation ratio Φ_m to be measured in the case, in which no body movement is present, is given by the following equation.

5

$$\Phi_m = \Delta A_1 / \Delta A_2 = \Delta A_{a1} / \Delta A_{a2}$$

10 Thus, the measured Φ_m is the attenuation ratio Φ_a of arterial blood, that is, $\Phi_a = \Delta A_{a1} / \Delta A_{a2}$.

[0061] On the other hand, in the case where a body movement is present, not only the thickness of arterial blood but the thickness of venous blood changes, as shown in Fig. 7B. The attenuation change ΔA caused in this case is a sum of the attenuation change ΔA_a , which is caused by change in the thickness of arterial blood, and the attenuation change ΔA_v , which is caused by change in the thickness of venous blood (i.e., $\Delta A = \Delta A_a + \Delta A_v$). The attenuation ratio Φ_m to be measured in this case is given by the following equation.

15

$$\Phi_m = \Delta A_1 / \Delta A_2 = (\Delta A_{a1} + \Delta A_{v1}) / (\Delta A_{a2} + \Delta A_{v2})$$

20

[0062] The attenuation changes are given in the following equations expressed in vector notation below.

25

$$A_a = (\Delta A_{a2}, \Delta A_{a1})$$

$$A_v = (\Delta A_{v2}, \Delta A_{v1})$$

30

$$A_m = (\Delta A_{a2} + \Delta A_{v2}, \Delta A_{a1} + \Delta A_{v1})$$

35

The attenuation ratios Φ corresponding to the above attenuation changes are represented by the respective gradients of the vectors shown in Fig. 8.

[0063] Incidentally, oxygen contained in arterial blood is taken into the tissue. Thus, the oxygen saturation S_v in venous blood is lower than that S_a in arterial blood ($S_a > S_v$). However, because of the correlation between the attenuation ratio Φ and the oxygen saturation S of blood as shown in Fig. 9, the inequality $\Phi_a < \Phi_v$ holds.

40

[0064] Therefore, as shown in Fig. 8, the measured attenuation ratio vector A_m appears between the vector A_a , whose gradient is small, and the vector A_v whose gradient is large. The gradient Φ_m of the measured signal A_m is determined by the ratio in length between the vectors A_a and A_v on condition that the values of the ratios Φ_a and Φ_v are constant.

45

[0065] In a case where a body movement is small and where the length of the vector A_v is nearly equal to 0 ($|A_v| \approx 0$), $\Phi_m \approx \Phi_a$. In a case where a body movement is large and where the length of the vector A_v is much larger than that of the vector A_a ($|A_v| \gg |A_a|$), $\Phi_m \approx \Phi_v$.

[0066] In a case where the attenuation change ratio Φ_m is observed by separating the pulse wave into a plurality of frequencies, the ratio Φ obtained at the frequency, at which the value of the ratio Φ_m is minimum, has a value closest to the attenuation ratio Φ_a of arterial blood.

50

[0067] The condition for minimizing the ratio Φ_m is that the ratio ($|A_a| / |A_v|$) is maximum. However, the length $|A_a|$ is maximum at the fundamental frequency of the pulse wave, among the plurality of frequencies. Thus, assuming that the noise is random like white noise, the ratio ($|A_a| / |A_v|$) is maximum at the fundamental frequency of the pulse wave.

[0068] Consequently, on condition that the noise is random, the fundamental frequency of the pulse wave can be determined by searching for a frequency at which the ratio Φ_m is minimum.

55

[0069] Next, a third embodiment of the invention will be described. Figs. 10A and 10B respectively correspond to Figs. 3A and 3B. In this embodiment, an effective frequency band (e.g., from 0.5Hz to 5.0Hz) of each of the amplitude spectra is divided into a plurality of frequency bands (e.g., eight bands) each of which has a plurality of measurement points

(e.g., four points) denoted by dashed lines in Fig. 10B.

[0070] In this embodiment, the divided frequency bands arranged such that parts of adjacent divided frequency bands are overlapped to each other. However, the adjacent divided frequency bands may not be overlapped to each other.

[0071] Next, as shown in Fig. 10C, an average value of the amplitudes at the plural measurement points is calculated for each of the divided frequency bands. The average value calculated for the spectrum corresponding to the red light R is denoted as R_FFT_ave . The average value calculated for the spectrum corresponding to the infrared light IR is denoted as IR_FFT_ave .

[0072] Further, as shown in Fig. 10D, a ratio between the thus calculated average values (R_FFT_ave / IR_FFT_ave) is calculated for each of the divided frequency bands.

[0073] Finally, the minimum value R_{min} of the thus calculated ratios is regarded as an attenuation ratio in arterial blood, and the frequency associated with the minimum value is regarded as a fundamental frequency f_p of the pulse wave.

[0074] In this embodiment, the average value of the amplitudes at the plural measurement points is first calculated for each of the divided frequency bands, and the ratio between the average values is then calculated as the attenuation ratio. However, a ratio between the amplitudes for each of the measurement points may be first calculated as an attenuation ratio, and an average value of the thus calculated ratios may be then calculated for each of the divided frequency bands.

[0075] In addition, the following processing may be adopted. It is determined whether a maximal point of the amplitude spectrum is included for each of the divided frequency shown in Fig. 10B. A divided frequency band which is judged as one including the maximal point becomes a candidate for a frequency band including an attenuation ratio in arterial blood. Among such candidates, one including the minimum value of the ratio between the average values (R_FFT_ave / IR_FFT_ave) is determined as the frequency band including an attenuation ratio in arterial blood.

[0076] The above judgment may be performed at least one of the amplitude spectrum corresponding to the red light R (R_FFT) and the amplitude spectrum corresponding to the infrared light IR (IR_FFT).

[0077] A divided frequency band which is judged as one not including the maximal point will not become the candidate even if the ratio of the average values (R_FFT_ave / IR_FFT_ave) of the divided frequency band has a relatively small value.

[0078] Specifically, in order to judge whether one divided frequency band has a maximal point of the amplitude spectrum, it is judged an n -th measurement point in the divided frequency band denoted as $FFT(n)$ is the maximal point when the $FFT(n)$ satisfies both of the following inequalities: $FFT(n-1) < FFT(n)$ and $FFT(n) > FFT(n+1)$.

[0079] However, if the n -th measurement point judged as the maximal point is located at one of both ends of one of the divided frequency bands (2) through (7) shown in Fig. 10B, the frequency band including such an n -th measurement point will not be regarded as one including the maximal point. This is because both ends of one of these divided frequency bands is contained in an adjacent one of the divided frequency bands. In other words, since the measurement points corresponding to the minimum frequency in the divided frequency band (1) and the maximum frequency in the divided frequency band (8) are not contained in another divided frequency band, if these measurement points are judged as the maximal point, the judgment is made valid.

[0080] The above judgment in connection with the maximal point may be executed after the execution of the processings shown in Figs. 10A to 10D in order to enhance the accuracy of the determination of the attenuation ratio in arterial blood based on the minimum value R_{min} .

[0081] In a case where the amplitude of the noise is relatively smaller than the amplitude of the pulse wave, the attenuation ratio Φ at the frequency, at which the amplitude spectrum shows a maximum value, can be read and is determined to be the attenuation ratio Φ_s of arterial blood. However, in a case where the amplitude of the noise is somewhat large, it is difficult to find out a peak corresponding to the pulse wave from the amplitude spectrum obtained by the FFT or the like.

[0082] Figs. 4A and 4B respectively correspond to Figs. 2A and 2B and are showing a case where large noise is superimposed on the pulse wave signals. The amplitude of the noise is almost the same as the amplitude of the pulse wave signal. Although the pulse wave can be still recognized in Fig. 4A, and the peak corresponding to the pulse wave can be recognized in Fig. 4B, in a case where a plurality of peaks having similar amplitudes, it is difficult to identify the peak corresponding to the pulse wave.

[0083] In such a case, a well-known signal separation method may be applied before the FFT processing is performed. As shown in Fig. 4C, the pulse wave signal and the noise can clearly be separated from each other. After the FFT processing is performed with respect to the thus separated signals, the frequency of the pulse wave can clearly be determined in the spectra as shown in Fig. 4D.

[0084] The attenuation ratio Φ of the arterial blood can be determined as well as the first or second embodiment as shown in Fig. 4E.

[0085] Figs. 5A to 5E respectively correspond to Figs. 4A to 4E and are showing a case where extreme large noise is superimposed on the pulse wave signals. The amplitude of the noise is about ten times the amplitude of the pulse wave signal. As shown in Figs. 5A and 5B, it is impossible to recognize pulse wave components from the measured

waveforms and the amplitude spectra. During such a vigorous body movement, arterial blood is often moved due to the body movement. Thus, even if the signal separation method is applied, the obtained waveform of the signal shown in Fig. 5C entirely differs from the pulse wave.

[0086] Therefore, even when the movement of an arterial blood component corresponding to the signal can be separated from the movement of a venous blood component corresponding to the noise, the frequency of each of the pulse waves cannot be identified according to the waveforms shown in Fig. 5C and the those obtained after the FFT processing, which are shown in Fig. 5D.

[0087] In a case where the amplitude corresponding to the noise is larger than the amplitude of the pulse wave signal, it is difficult to calculate a pulse rate and an oxygen saturation by employing a frequency, at which the amplitude of the spectrum is maximum, as the fundamental frequency of the pulse wave. However, according to the method as explained in the second and third embodiments, the frequency of a pulse wave can be determined by searching a frequency, at which the attenuation ratio is minimum, as shown in Fig. 5E. The attenuation ratio at the determined frequency can be obtained as the oxygen saturation in arterial blood.

[0088] In a case where no noise is superimposed on the pulse wave, a maximum amplitude appears at the fundamental frequency of the pulse wave, and higher harmonic waves appear at frequencies which are twice and three times the fundamental frequency as shown in Fig. 2B. In a case where a large noise is superimposed on the pulse wave, frequencies, at each of which a peak amplitude is present, is not distributed in a narrow band, but is distributed in a wide band as shown in Fig. 5B. In a case where the amplitudes corresponding to noise are distributed in a narrow band, as shown in Fig. 3B, a peak appears at a frequency that differs from the fundamental frequency and from the frequencies of the higher harmonic waves.

[0089] In view of the above, the pulse oximeter may comprise a selector operable to select a frequency, at which the attenuation ratio is minimum, as a frequency representing an oxygen saturation in arterial blood, in a case where the frequency corresponding to the second-highest peak obtained by FFT is not twice the fundamental frequency that is the highest peak, or where the half-value width of the first peak obtained by FFT is neither equal to nor less than a prescribed value.

[0090] Fig. 6 shows an example in which a pulse wave, the SpO₂ of which cannot be calculated by the conventional method because of the large noise, is divided into 8 frequency bands such that each of the bands has a band width of 1 Hz and center frequencies are ranged from 1.0Hz to 4.5Hz at a fixed interval of 0.5Hz, and SpO₂ is calculated for each of the divided bands. It is apparent that different values of SpO₂ corresponding to different attenuation ratios are obtained by the above measurement. Since arterial blood exhibits a higher oxygen saturation than venous blood, the SpO₂ of the band, which exhibits a highest value of the oxygen saturation, can be regarded as the oxygen saturation of arterial blood. Further, a representative frequency (e.g., a center frequency) of the frequency band including the highest value in the oxygen saturation can be regarded as the frequency of the pulse wave.

[0091] In the conventional method, the pulse wave signal and the noise are separated on the basis of the attenuation ratio. That is, in order to separate a pulse wave signal and noise at an analysis section of interest, it is necessary to input an attenuation ratio which is obtained in a previous section (i.e., data in the past is necessary). On the other hand, according to the method of the invention, since it is not necessary to refer data in the past, processing speed can be enhanced.

[0092] Although the present invention has been shown and described with reference to specific embodiments, various changes and modifications will be apparent to those skilled in the art from the teachings herein. Such changes and modifications as are obvious are deemed to come within the spirit, scope and contemplation of the invention as defined in the appended claims.

[0093] For example, in the above embodiments, the pulse wave is separated into a plurality of frequencies by the FFT. However, a plurality of bandpass filters, whose central frequencies differ from one another, may be used for separating the pulse wave into a plurality of frequencies.

[0094] The oxygen saturation measuring apparatus and method of the invention described in the appended claims 1 to 12 can realize a signal processing method enabled to alleviate a burden of calculation for extracting a common signal component by processing two signals of the same kind, which are substantially simultaneously extracted from a same medium. Also, the concentration of an object material can be measured with good accuracy by applying the signal processing method even when a noise due to the body movement of the medium is generated in a pulse wave signal. Also, even when a noise due to the body movement is generated in a pulse wave data signal, a pulse rate can be obtained with good precision by removing a noise from a pulse wave signal.

Claims

1. An apparatus for measuring an oxygen saturation in blood, comprising:

a plurality of light emitters (1a,1b), adapted to irradiate a living tissue (12) with a plurality of light beams having different wavelengths;

a light receiver (8), adapted to receive the light beams reflected from or transmitted through the living tissue to generate pulse wave signals in accordance with pulsations of the blood in the living tissue; and

a separator (4), configured to separate each of the pulse wave signals into a plurality of amplitude signals each of which is associated with one frequency (f), thereby generating pairs of amplitude signals (R_FFT(f), IR_FFT(f)) each of which is associated with one of a plurality of frequencies,

characterized in that

the apparatus further comprises:

a first processor (4), configured to calculate a ratio ($\Phi(f)$) between the amplitude signals in each of the pairs of the amplitude signals (R_FFT(f), IR_FFT(f));

a selector (4), configured to select one of the pairs of the amplitude signals (R_FFT(f), IR_FFT(f)); and

a second processor (4), configured to calculate the oxygen saturation based on the ratio ($\Phi(f)$) of the selected one of the pairs of the amplitude signals (R_FFT(f), IR_FFT(f)).

2. The apparatus as set forth in claim 1, wherein:

the separator comprises either an FFT processor or a digital filter.

3. The apparatus as set forth in claim 1, wherein:

the selector is configured to select such a pair of the amplitude signals that have maximum amplitude values.

4. The apparatus as set forth in claim 1, wherein:

the selector is configured to select such a pair of the amplitude signals that the ratio takes a minimum value.

5. The apparatus as set forth in claim 4, wherein:

the first processor comprises:

a first calculator, configured to define a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals, and configured to calculate an average value of the amplitude signals in each of the frequency bands, thereby generating pairs of average values each of which is associated with one of the frequency bands; and

a second calculator, configured to calculate an average ratio between the average values in each of the pairs of the average values; and

the selector is configured to select such a frequency band that the average ratio takes a minimum value.

6. The apparatus as set forth in claim 4, wherein:

the first processor comprises:

a first calculator, configured to:

define a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals;

judge whether there is a maximal point of the amplitude signals in each of the frequency bands; and

calculate an average value of the amplitude signals in at least one of the frequency bands which is judged as one including the maximal point, thereby at least one pair of average values each of which is associated with one of the frequency bands; and

a second calculator, configured to calculate an average ratio between the average values in each of the at least one pair of the average values; and

the selector is configured to select such a frequency band that the average ratio takes a minimum value.

7. The apparatus as set forth in claim 4, wherein:

the first processor comprises:

a first calculator, configured to calculate ratios each of which is a ratio between each of the pairs of the amplitude signals; and

a second calculator, configured to define a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from each of the pulse wave signals, and configured to calculate an average value of the ratios in each of the frequency bands, thereby generating a plurality of average values; and the selector is configured to select such a frequency band that the average value takes a minimum value.

8. The apparatus as set forth in any of claims 5 to 7, wherein:

a part of one of the frequency bands is overlapped with a part of another one of the frequency bands.

9. The apparatus as set forth in claim 1, wherein:

the selector is configured to select either such a pair of the amplitude signals that have maximum amplitude values or such a pair of the amplitude signals that the ratio takes a minimum value in accordance with a prescribed condition.

10. The apparatus as set forth in claim 9, wherein:

the prescribed condition includes a waveform of the amplitude signals.

11. The apparatus as set forth in claim 1, wherein

the light beams include a red light beam and an infrared light beam.

12. A method for measuring an oxygen saturation in blood, comprising:

irradiating a living tissue with a plurality of light beams having different wavelengths;
receiving the light beams reflected from or transmitted through the living tissue to generate pulse wave signals in accordance with pulsations of the blood in the living tissue; and
separating each of the pulse wave signals into a plurality of amplitude signals each of which is associated with one frequency, thereby generating pairs of amplitude signals each of which is associated with one of a plurality of frequencies,

characterized in that

the method further comprises:

calculating a ratio between the amplitude signals in each of the pairs of the amplitude signals;

selecting one of the pairs of the amplitude signals; and

calculating the oxygen saturation based on the ratio of the selected one of the pairs of the amplitude signals.

13. The method as set forth in claim 12, wherein:

the separating is performed with either an FFT processing or a digital filtering.

14. The method as set forth in claim 12, wherein:

such a pair of the amplitude signals that have maximum amplitude values is selected as the one of the pairs of the amplitude signals.

15. The method as set forth in claim 12, wherein:

such a pair of the amplitude signals that the ratio takes a minimum value is selected as the one of the pairs of the amplitude signals.

16. The method as set forth in claim 15, further comprising:

defining a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from

each of the pulse wave signals;
calculating an average value of the amplitude signals in each of the frequency bands, thereby generating pairs
of average values each of which is associated with one of the frequency bands;
calculating an average ratio between the average values in each of the pairs of the average values; and
5 selecting such a frequency band that the average ratio takes a minimum value.

17. The method as set forth in claim 15, further comprising:

10 defining a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from
each of the pulse wave signals;
judging whether there is a maximal point of the amplitude signals in each of the frequency bands;
calculating an average value of the amplitude signals in at least one of the frequency bands which is judged as
one including the maximal point, thereby at least one pair of average values each of which is associated with
15 one of the frequency bands;
calculating an average ratio between the average values in each of the at least one pair of the average values; and
selecting such a frequency band that the average ratio takes a minimum value.

18. The method as set forth in claim 15, further comprising:

20 calculating ratios each of which is a ratio between each of the pairs of the amplitude signals;
defining a plurality of frequency bands each of which includes a plurality of amplitude signals obtained from
each of the pulse wave signals;
calculating an average value of the ratios in each of the frequency bands, thereby generating a plurality of
average values; and
25 selecting such a frequency band that the average value takes a minimum value.

19. The method as set forth in any of claims 16 to 18, wherein:

30 a part of one of the frequency bands is overlapped with a part of another one of the frequency bands.

20. The method as set forth in claim 12, wherein:

35 either such a pair of the amplitude signals that have maximum amplitude values or such a pair of the amplitude
signals that the ratio takes a minimum value is selected as the one of the pairs of the amplitude signals in
accordance with a prescribed condition.

21. The method as set forth in claim 20, wherein:

40 the prescribed condition includes a waveform of the amplitude signals.

Patentansprüche

45 1. Vorrichtung zum Messen einer Sauerstoffsättigung in Blut, die umfasst:

eine Vielzahl von Lichtemissionseinrichtungen (1a, 1b), die so eingerichtet sind, dass sie ein lebendes Gewebe
(12) mit einer Vielzahl von Lichtstrahlen bestrahlen, die unterschiedliche Wellenlängen haben;
eine Lichtempfangseinrichtung (8), die so eingerichtet ist, dass sie die Lichtstrahlen empfängt, die von dem
lebenden Gewebe reflektiert oder durchgelassen werden, um Impulswellensignale entsprechend Pulsationen
50 des Blutes in dem lebenden Gewebe zu erzeugen; und
ein Trennelement (4), das so konfiguriert ist, dass es jedes der Impulswellensignale in eine Vielzahl von Am-
plitudensignalen trennt, von denen jedes mit einer Frequenz (f) zusammenhängt, um so Paare von Amplitu-
densignalen (R_FFT(f), IR_FFT(f)) zu erzeugen, von denen jedes mit einer einer Vielzahl von Frequenzen
zusammenhängt,

55 **dadurch gekennzeichnet, dass**
die Vorrichtung des Weiteren umfasst:

einen ersten Prozessor (4), der so konfiguriert ist, dass er ein Verhältnis ($\Phi(f)$) zwischen den Amplituden-

EP 1 757 224 B1

signalen in jedem der Paare der Amplitudensignale ($R_{\text{FFT}}(f)$, $IR_{\text{FFT}}(f)$) berechnet;
eine Auswähleinrichtung (4), die so konfiguriert ist, dass sie eines der Paare der Amplitudensignale ($R_{\text{FFT}}(f)$) auswählt; und
eine zweite Verarbeitungseinrichtung (4), die so konfiguriert ist, dass sie die Sauerstoffsättigung auf Basis des Verhältnisses ($\Phi(f)$) des ausgewählten einen der Paare der Amplitudensignale ($R_{\text{FFT}}(f)$, $IR_{\text{FFT}}(f)$) berechnet.

2. Vorrichtung nach Anspruch 1, wobei die Trenneinrichtung entweder eine FFT-Verarbeitungseinrichtung oder ein digitales Filter umfasst.

3. Vorrichtung nach Anspruch 1, wobei:

die Auswähleinrichtung so konfiguriert ist, dass sie ein Paar der Amplitudensignale auswählt, die maximale Amplitudenwerte aufweisen.

4. Vorrichtung nach Anspruch 1, wobei:

die Auswähleinrichtung so konfiguriert ist, dass sie ein Paar der Amplitudensignale auswählt, bei dem das Verhältnis einen Minimalwert annimmt.

5. Vorrichtung nach Anspruch 4, wobei:

die erste Verarbeitungseinrichtung umfasst:

eine erste Recheneinrichtung, die so konfiguriert ist, dass sie eine Vielzahl von Frequenzbändern definiert, von denen jedes eine Vielzahl von Amplitudensignalen enthält, die aus jedem der Impulswellensignale gewonnen werden, und so konfiguriert ist, dass sie einen Durchschnittswert der Amplitudensignale in jedem der Frequenzbänder berechnet, um so Paare von Durchschnittswerten zu erzeugen, von denen jedes mit einem der Frequenzbänder zusammenhängt; und
eine zweite Recheneinrichtung, die so konfiguriert ist, dass sie ein Durchschnittsverhältnis zwischen den Durchschnittswerten in jedem der Paare der Durchschnittswerte berechnet; und
die Auswähleinrichtung so konfiguriert ist, dass sie ein Frequenzband auswählt, bei dem das Durchschnittsverhältnis einen Minimalwert annimmt.

6. Vorrichtung nach Anspruch 4, wobei:

die erste Verarbeitungseinrichtung umfasst:

eine erste Recheneinrichtung, die so konfiguriert ist, dass sie:

eine Vielzahl von Frequenzbändern definiert, von denen jedes eine Vielzahl von Amplitudensignalen enthält, die aus jedem der Impulswellensignale gewonnen werden;
feststellt, ob ein Maximalpunkt der Amplitudensignale in jedem der Frequenzbänder vorhanden ist; und
einen Durchschnittswert der Amplitudensignale in wenigstens einem der Frequenzbänder berechnet, für das festgestellt wird, dass es den Maximalpunkt enthält, um so wenigstens ein Paar von Durchschnittswerten zu erzeugen, von denen jedes mit einem der Frequenzbänder zusammenhängt; und
eine zweite Recheneinrichtung, die so konfiguriert ist, dass sie ein Durchschnittsverhältnis zwischen den Durchschnittswerten in jedem von dem wenigstens einen Paar der Durchschnittswerte berechnet; und
die Auswähleinrichtung so konfiguriert ist, dass sie ein Frequenzband auswählt, bei dem das Durchschnittsverhältnis einen Minimalwert annimmt.

7. Vorrichtung nach Anspruch 4, wobei:

die erste Verarbeitungseinrichtung umfasst:

eine erste Recheneinrichtung, die so konfiguriert ist, dass sie Verhältnisse berechnet, von denen jedes ein

EP 1 757 224 B1

Verhältnis zwischen jedem der Paare der Amplitudensignale ist; und eine zweite Recheneinrichtung, die so konfiguriert ist, dass sie eine Vielzahl von Frequenzbändern definiert, von denen jedes eine Vielzahl von Amplitudensignalen enthält, die aus jedem der Impulswellensignale gewonnen werden, und so konfiguriert ist, dass sie einen Durchschnittswert der Verhältnisse in jedem der Frequenzbänder berechnet, um so eine Vielzahl von Durchschnittswerten zu erzeugen; und die Auswähleinrichtung so konfiguriert ist, dass sie ein Frequenzband auswählt, bei dem der Durchschnittswert einen Minimalwert annimmt.

8. Vorrichtung nach einem der Ansprüche 5 bis 7, wobei:

ein Teil eines der Frequenzbänder einen Teil eines anderen der Frequenzbänder überlappt.

9. Vorrichtung nach Anspruch 1, wobei:

die Auswähleinrichtung so konfiguriert ist, dass sie gemäß einer vorgeschriebenen Bedingung entweder ein Paar der Amplitudensignale auswählt, die maximale Amplitudenwerte haben, oder ein Paar der Amplitudensignale, bei dem das Verhältnis einen Minimalwert annimmt.

10. Vorrichtung nach Anspruch 9, wobei:

die vorgeschriebene Bedingung eine Wellenform der Amplitudensignale einschließt.

11. Vorrichtung nach Anspruch 1, wobei:

die Lichtstrahlen einen roten Lichtstrahl und einen Infrarot-Lichtstrahl einschließen.

12. Verfahren zum Messen einer Sauerstoffsättigung in Blut, das umfasst:

Bestrahlen eines lebenden Gewebes mit einer Vielzahl von Lichtstrahlen, die unterschiedliche Wellenlängen haben;

Empfangen der von dem lebenden Gewebe reflektierten oder durchgelassenen Lichtstrahlen, um Impulswellensignale entsprechend Pulsationen des Blutes in dem lebenden Gewebe zu erzeugen; und

Trennen jedes der Impulswellensignale in eine Vielzahl von Amplitudensignalen, von denen jedes mit einer Frequenz zusammenhängt, um so Paare von Amplitudensignalen zu erzeugen, von denen jedes mit einer der Vielzahl von Frequenzen zusammenhängt,

dadurch gekennzeichnet, dass
das Verfahren des Weiteren umfasst:

Berechnen eines Verhältnisses zwischen den Amplitudensignalen in jedem der Paare der Amplitudensignale;

Auswählen eines der Paare der Amplitudensignale; und

Berechnen der Sauerstoffsättigung auf Basis des Verhältnisses des ausgewählten einen der Paare der Amplitudensignale.

13. Verfahren nach Anspruch 12, wobei:

das Trennen entweder mit einer FFT-Verarbeitung oder einem digitalen Filtern durchgeführt wird.

14. Verfahren nach Anspruch 12, wobei:

ein Paar der Amplitudensignale, die maximale Amplitudenwerte haben, als das eine der Paare der Amplitudensignale ausgewählt wird.

15. Verfahren nach Anspruch 12, wobei:

ein Paar der Amplitudensignale, bei denen das Verhältnis einen Minimalwert hat, als das eine der Paare der Amplitudensignale ausgewählt wird.

16. Verfahren nach Anspruch 15, das des Weiteren umfasst:

5 Definieren eine Vielzahl von Frequenzbändern, von denen jedes eine Vielzahl von Amplitudensignalen enthält, die aus jedem der Impulswellensignale gewonnen werden;
Berechnen eines Durchschnittswertes der Amplitudensignale in jedem der Frequenzbänder, um so Paare von Durchschnittswerten zu erzeugen, von denen jedes mit einem der Frequenzbänder zusammenhängt;
Berechnen eines Durchschnittsverhältnisses zwischen den Durchschnittswerten in jedem der Paare der Durchschnittswerte; und
10 Auswählen eines Frequenzbandes, bei dem das Durchschnittsverhältnis einen Minimalwert annimmt.

17. Verfahren nach Anspruch 15, das des Weiteren umfasst:

15 Definieren einer Vielzahl von Frequenzbändern, von denen jedes eine Vielzahl von Amplitudensignalen enthält, die aus jedem der Impulswellensignale gewonnen werden;
Feststellen, ob ein Maximalpunkt der Amplitudensignale in jedem der Frequenzbänder vorhanden ist;
Berechnen eines Durchschnittswertes der Amplitudensignale in wenigstens einem der Frequenzbänder, für das festgestellt wird, dass es den Maximalpunkt enthält, um so wenigstens ein Paar von Durchschnittswerten zu erzeugen, von denen jedes mit einem der Frequenzbänder zusammenhängt;
Berechnen eines Durchschnittsverhältnisses zwischen den Durchschnittswerten in jedem von dem wenigstens einen Paar der Durchschnittswerte; und
20 Auswählen eines Frequenzbandes, bei dem das Durchschnittsverhältnis einen Minimalwert annimmt.

18. Verfahren nach Anspruch 15, das des Weiteren umfasst:

25 Berechnen von Verhältnissen, von denen jedes ein Verhältnis zwischen jedem der Paare der Amplitudensignale ist;
Definieren einer Vielzahl von Frequenzbändern, von denen jedes eine Vielzahl von Amplitudensignalen enthält, die aus jedem der Impulswellensignale gewonnen werden;
Berechnen eines Durchschnittswertes der Verhältnisse in jedem der Frequenzbänder, um so eine Vielzahl von Durchschnittswerten zu erzeugen; und
30 Auswählen eines Frequenzbandes, bei dem der Durchschnittswert einen Minimalwert annimmt.

19. Verfahren nach einem der Ansprüche 16 bis 18, wobei:

35 ein Teil eines der Frequenzbänder einen Teil eines anderen der Frequenzbänder überlappt.

20. Verfahren nach Anspruch 12, wobei:

40 gemäß einer vorgeschriebenen Bedingung entweder ein Paar der Amplitudensignale, die maximale Amplitudenwerte haben, oder ein Paar der Amplitudensignale, bei dem das Verhältnis einen Minimalwert annimmt, als das eine der Paare der Amplitudensignale ausgewählt wird.

21. Verfahren nach Anspruch 20, wobei:

45 die vorgeschriebene Bedingung eine Wellenform der Amplitudensignale einschließt.

Revendications

50 1. Appareil pour mesurer une saturation d'oxygène dans le sang, comportant :

une pluralité d'émetteurs lumineux (1a, 1b), adaptés pour irradier un tissu vivant (12) grâce à une pluralité de faisceaux lumineux possédant différentes longueurs d'onde ;
un récepteur de lumière (8), adapté pour recevoir les faisceaux lumineux réfléchis de ou transmis à travers le tissu vivant pour générer des signaux d'ondes d'impulsion conformément aux pulsations du sang dans le tissu vivant ;
55 et
un séparateur (4), configuré pour séparer chacun des signaux d'ondes d'impulsion en une pluralité de signaux

EP 1 757 224 B1

d'amplitude, dont chacun est associé à une fréquence (f), générant ainsi des paires de signaux d'amplitude (R_FFT(f), IR_FFT(f)) dont chacun est associé à l'une d'une pluralité de fréquences,

caractérisé en ce que

l'appareil comporte en outre :

- 5
- un premier processeur (4), configuré pour calculer un rapport ($\Phi(f)$) entre les signaux d'amplitude dans chacune des paires de signaux d'amplitude (R_FFT(f), IR_FFT(f)) ;
 - un sélecteur (4), configuré pour sélectionner l'une des paires de signaux d'amplitude (R_FFT(f), IR_FFT(f)) ; et
 - 10 un second processeur (4), configuré pour calculer la saturation en oxygène en fonction du rapport ($\Phi(f)$) de l'une sélectionnée des paires de signaux d'amplitude (R_FFT(f), IR_FFT(f)).

2. Appareil selon la revendication 1, dans lequel :

15 le séparateur comporte soit un processeur FFT soit un filtre numérique.

3. Appareil selon la revendication 1, dans lequel :

20 le sélecteur est configuré pour sélectionner une paire de signaux d'amplitude de sorte qu'ils ont des valeurs d'amplitude maximum.

4. Appareil selon la revendication 1, dans lequel :

25 le sélecteur est configuré pour sélectionner une paire de signaux d'amplitude de sorte que le rapport prend une valeur minimum.

5. Appareil selon la revendication 4, dans lequel :

30 le premier processeur comporte :

- un premier calculateur, configuré pour définir une pluralité de bandes de fréquence dont chacune comprend une pluralité de signaux d'amplitude obtenus à partir de chacun des signaux d'ondes d'impulsion, et configuré pour calculer une valeur moyenne des signaux d'amplitude dans chacune des bandes de fréquence, générant ainsi des paires de valeurs moyennes dont chacune est associée à l'une des bandes de fréquence ;
- 35 et
- un second calculateur, configuré pour calculer un rapport moyen entre les valeurs moyennes dans chacune des paires de valeurs moyennes ; et
- le sélecteur est configuré pour sélectionner une bande de fréquence de sorte que le rapport moyen prend une valeur minimum.

40 6. Appareil selon la revendication 4, dans lequel :

le premier processeur comporte :

45 un premier calculateur, configuré pour :

- définir une pluralité de bandes de fréquence dont chacune comprend une pluralité de signaux d'amplitude obtenus à partir de chacun des signaux d'onde d'impulsion ;
- estimer s'il existe un point maximum des signaux d'amplitude dans chacune des bandes de fréquence ;
- 50 et
- calculer une valeur moyenne des signaux d'amplitude dans au moins l'une des bandes de fréquence qui est estimée comme étant celle comprenant le point maximum, ainsi au moins une paire des valeurs moyennes dont chacune est associée à l'une des bandes de fréquence ; et un second calculateur, configuré pour calculer un rapport moyen entre les valeurs moyennes dans chacune de la au moins
- 55 une paire de valeurs moyennes ; et
- le sélecteur est configuré pour sélectionner une bande de fréquence telle que le rapport moyen prend une valeur minimum.

EP 1 757 224 B1

7. Appareil dans la revendication 4, dans lequel :

le premier processeur comporte :

5 un premier calculateur, configuré pour calculer des rapports dont chacun est un rapport entre chacune des paires de signaux d'amplitude ; et
un second calculateur, configuré pour définir une pluralité de bandes de fréquence dont chacune comprend une pluralité de signaux d'amplitude obtenus à partir de chacun des signaux d'ondes d'impulsion, et configuré pour calculer une valeur moyenne des rapports dans chacune des bandes de fréquence, générant
10 ainsi une pluralité de valeurs moyenne; et
le sélecteur est configuré pour sélectionner une bande de fréquence telle que la valeur moyenne prend une valeur minimum.

8. Appareil selon l'une quelconque des revendications 5 à 7, dans lequel :

15 une partie de l'une des bandes de fréquence est chevauchée par une partie d'une autre des bandes de fréquence.

9. Appareil selon la revendication 1, dans lequel :

20 le sélecteur est configuré pour sélectionner soit une paire de signaux d'amplitude de sorte qu'ils ont des valeurs d'amplitude maximum soit une paire de signaux d'amplitude de sorte que le rapport prend une valeur minimum conformément à une condition prescrite.

10. Appareil selon la revendication 9, dans lequel :

25 la condition prescrite comprend une forme d'onde des signaux d'amplitude.

11. Appareil selon la revendication 1, dans lequel les faisceaux lumineux comprennent un faisceau de lumière rouge et un faisceau de lumière infrarouge.

30 12. Procédé pour mesurer la saturation en oxygène dans le sang, comportant :

l'irradiation d'un tissu vivant par une pluralité de faisceaux lumineux possédant différentes longueurs d'onde; la réception des faisceaux lumineux réfléchis de ou transmis à travers le tissu vivant pour générer des signaux d'onde d'impulsion conformément aux pulsations du sang dans le tissu vivant ; et
35 la séparation de chacun des signaux d'onde d'impulsion en une pluralité de signaux d'amplitude dont chacun est associé à une fréquence, générant ainsi des paires de signaux d'amplitude dont chacun est associé à l'une d'une pluralité de fréquences,

caractérisé en ce que

40 le procédé comporte en outre :

le calcul d'un rapport entre les signaux d'amplitude dans chacune de la paire de signaux d'amplitude; la sélection d'une des paires des signaux d'amplitude ; et
45 le calcul de la saturation d'oxygène en fonction du rapport de l'une sélectionnée des paires de signaux d'amplitude.

13. Procédé selon la revendication 12, dans lequel :

50 la séparation est effectuée par soit un traitement FFT soit un filtrage numérique.

14. Procédé selon la revendication 12, dans lequel :

55 une paire de signaux d'amplitude tels qu'ils ont des valeurs d'amplitude maximum est sélectionné en tant que l'une des paires de signaux d'amplitude.

15. Procédé selon la revendication 12, dans lequel :

une paire de signaux d'amplitude de sorte que le rapport prend une valeur minimum est sélectionnée en tant

EP 1 757 224 B1

que l'une des paires de signaux d'amplitude.

16. Procédé selon la revendication 15, comportant en outre :

5 la définition d'une pluralité de bandes de fréquence dont chacune comporte une pluralité de signaux d'amplitude obtenus à partir de chacun des signaux d'onde d'impulsion ;
le calcul d'une valeur moyenne des signaux d'amplitude dans chacune des bandes de fréquence, générant ainsi des paires de valeurs moyennes dont chacune est associée avec l'une des bandes de fréquence ;
10 le calcul d'un rapport moyen entre les valeurs moyennes dans chacune des paires de valeurs moyennes ; et
la sélection d'une bande de fréquence de sorte que le rapport moyen prend une valeur minimum.

17. Procédé selon la revendication 15, comportant en outre :

15 la définition d'une pluralité de bandes de fréquence dont chacune comprend une pluralité de signaux d'amplitude obtenus à partir de chacun des signaux d'ondes d'impulsion ;
l'estimation s'il existe un point maximum des signaux d'amplitude dans chacune des bandes de fréquence ;
le calcul d'une valeur moyenne des signaux d'amplitude dans au moins l'une des bandes de fréquence qui est estimé comme étant celle comprenant le point maximum, ainsi au moins une paire de valeurs moyennes dont
20 chacune est associée à l'une des bandes de fréquence ;
le calcul d'un rapport moyen entre les valeurs moyennes dans chacune de la au moins une paire de valeurs moyennes ; et
la sélection d'une bande de fréquence de sorte que le rapport moyen prend une valeur minimum.

18. Procédé selon la revendication 15, comportant en outre :

25 le calcul de rapports dont chacun est un rapport entre chacune des paires de signaux d'amplitude ;
la définition d'une pluralité de bandes de fréquence dont chacune comprend une pluralité de signaux d'amplitude obtenus à partir de chacun des signaux d'ondes d'impulsion ;
le calcul d'une valeur moyenne des rapports dans chacune des bandes de fréquence, générant ainsi une
30 pluralité de valeurs moyennes ; et
la sélection d'une bande de fréquence de sorte que la valeur moyenne prend une valeur minimum.

19. Procédé selon l'une quelconque des revendications 16 à 18, dans lequel :

35 une partie de l'une des bandes de fréquence est chevauchée par une partie d'une autre des bandes de fréquence.

20. Procédé selon la revendication 12, dans lequel :

40 soit une paire des signaux d'amplitude de sorte qu'ils ont des valeurs d'amplitude maximum soit une paire de signaux d'amplitude de sorte que le rapport prend une valeur minimum est sélectionnée en tant que l'une des paires de signaux d'amplitude conformément à une condition prescrite.

21. Procédé selon la revendication 20, dans lequel :

45 la condition prescrite comprend une forme d'onde des signaux d'amplitude.

50

55

FIG. 1

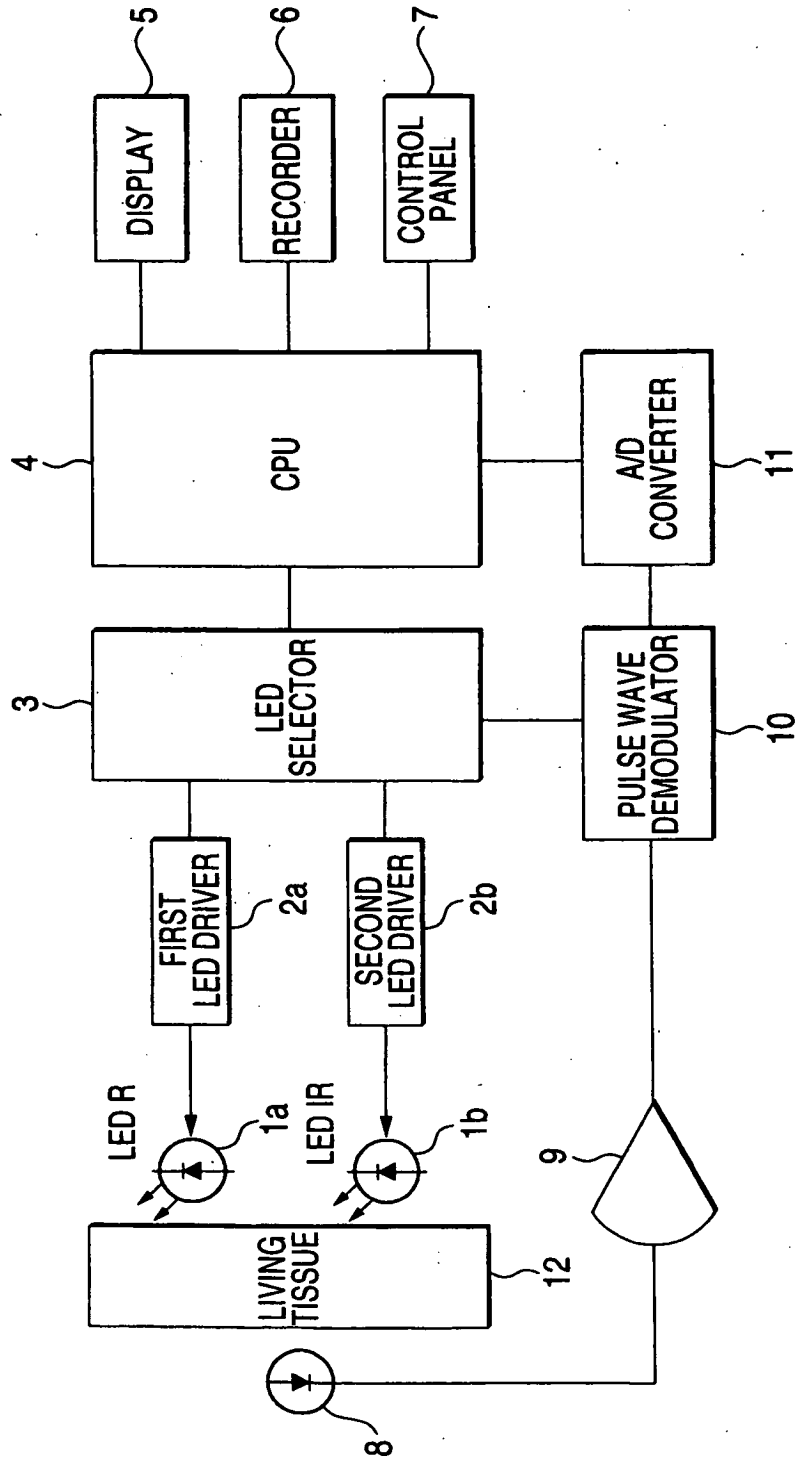


FIG. 2A

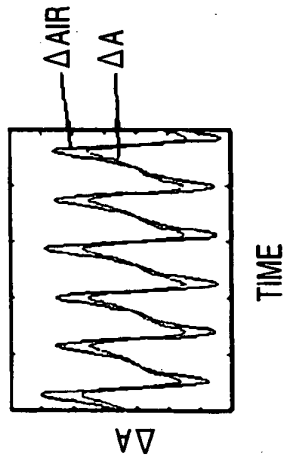


FIG. 2B

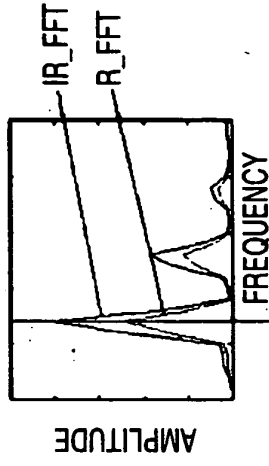


FIG. 2C



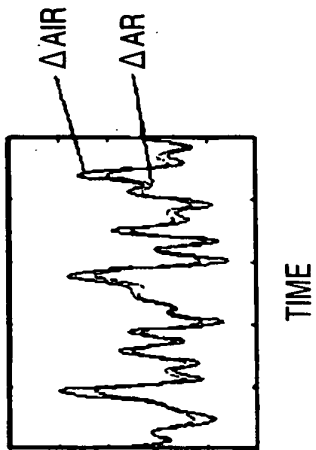


FIG. 3A

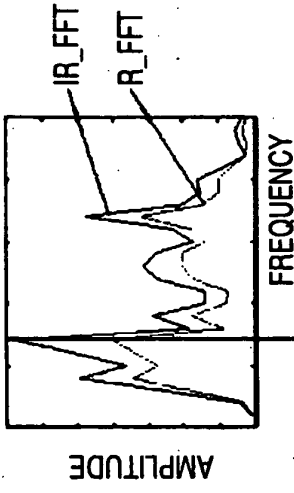


FIG. 3B

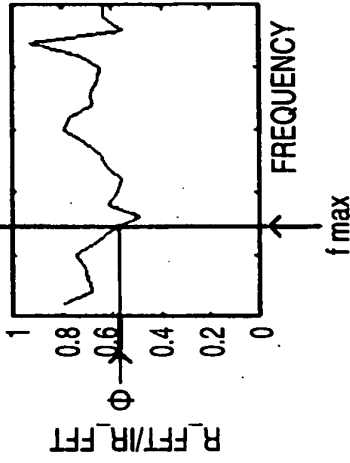


FIG. 3C

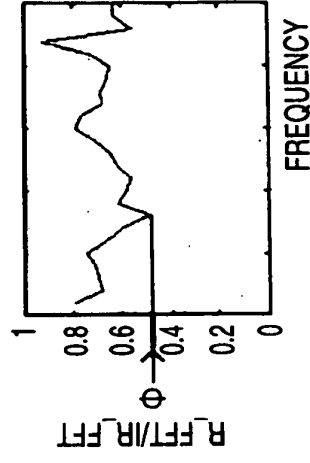


FIG. 3D

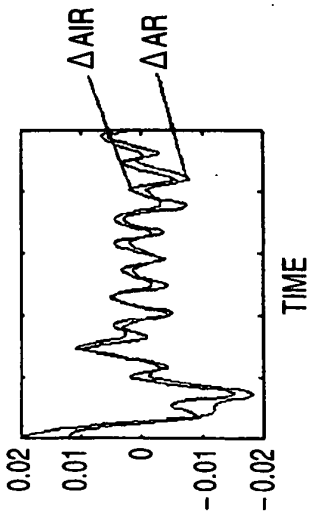


FIG. 4A

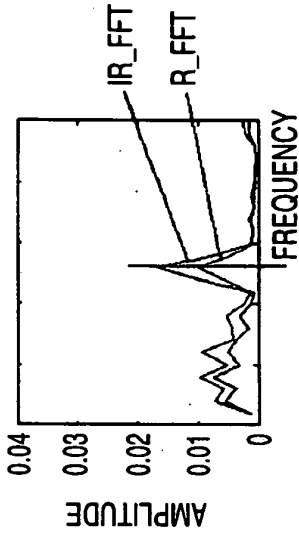


FIG. 4B

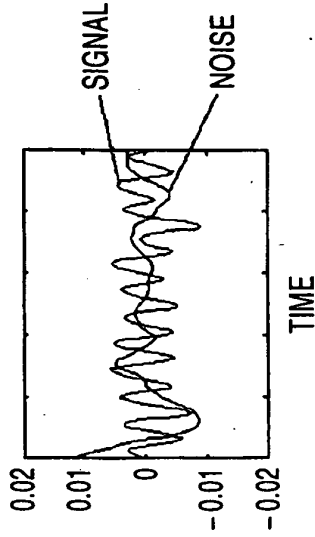


FIG. 4C

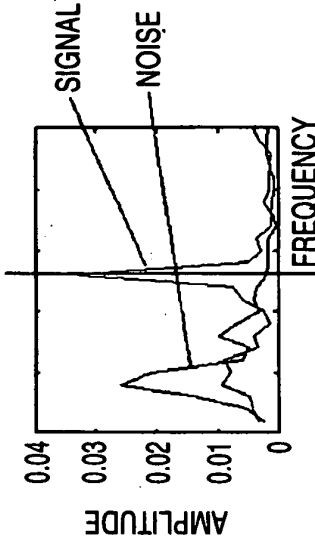


FIG. 4D

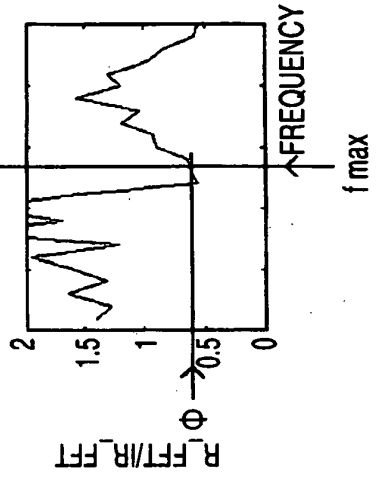


FIG. 4E

FIG. 5A

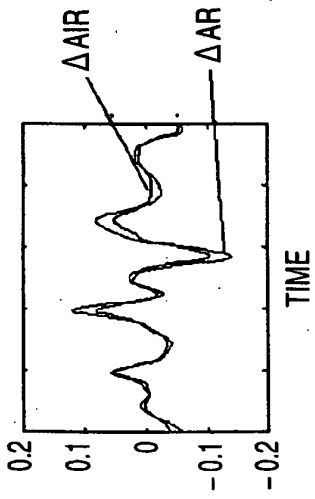


FIG. 5B

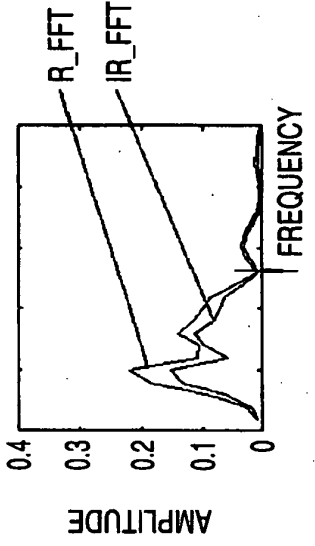


FIG. 5C

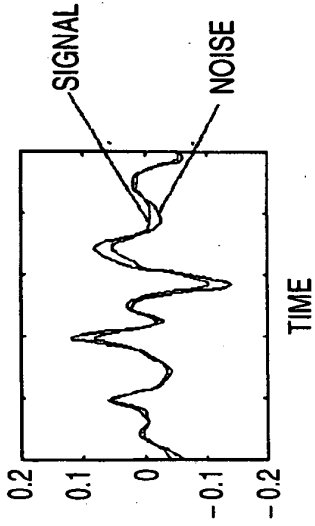


FIG. 5D

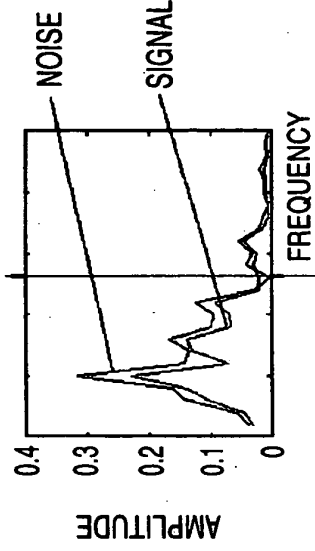


FIG. 5E

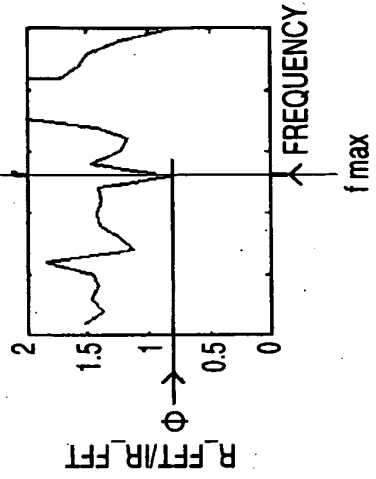


FIG. 6

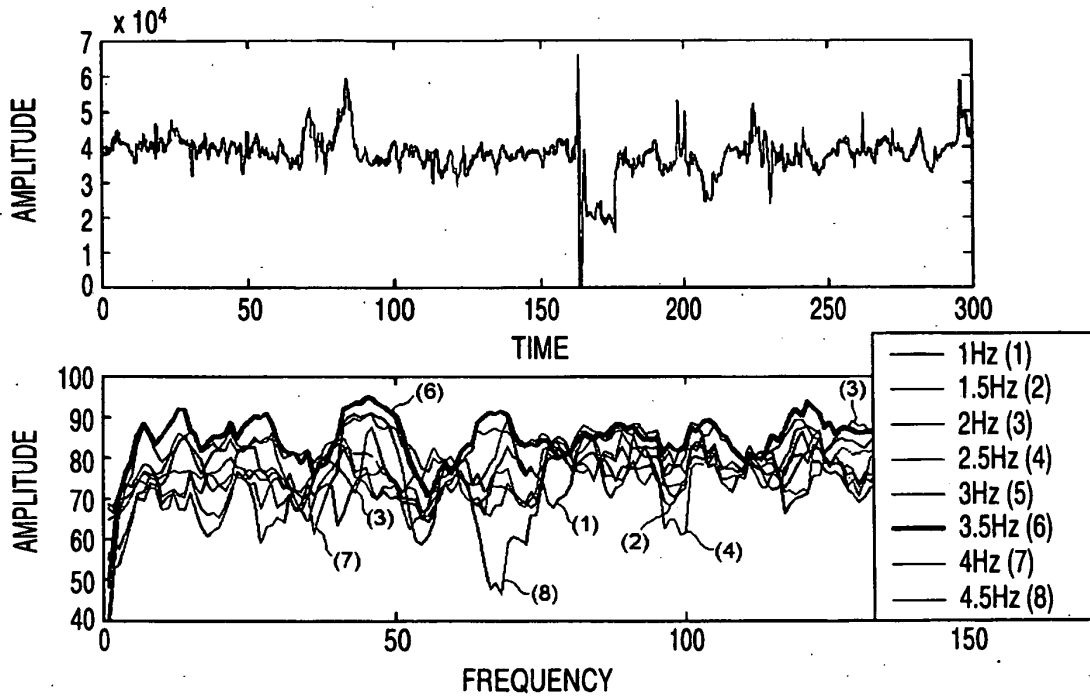


FIG. 7A

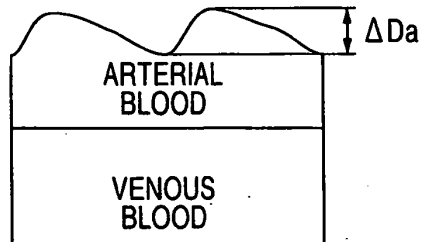


FIG. 7B

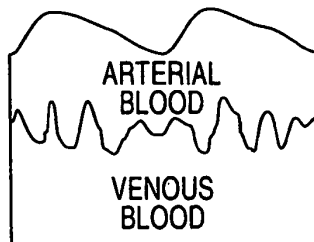


FIG. 8

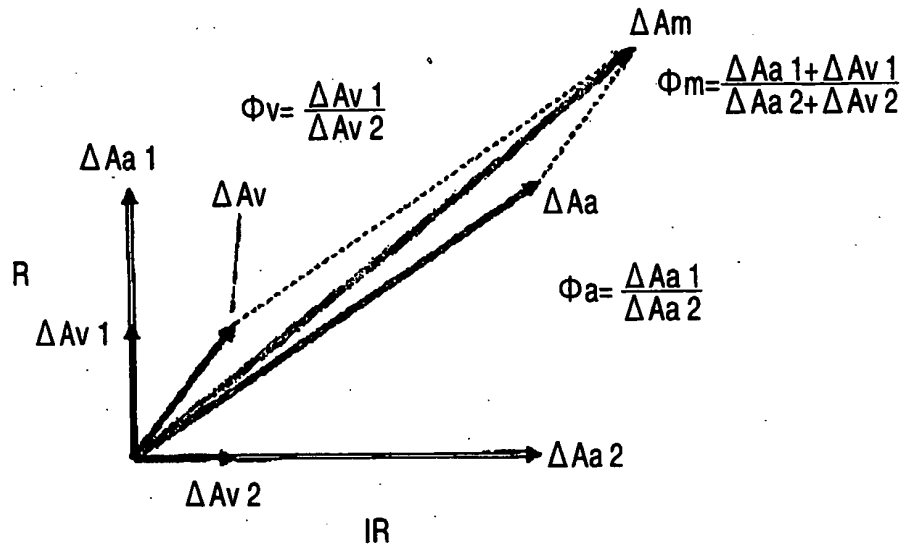


FIG. 9

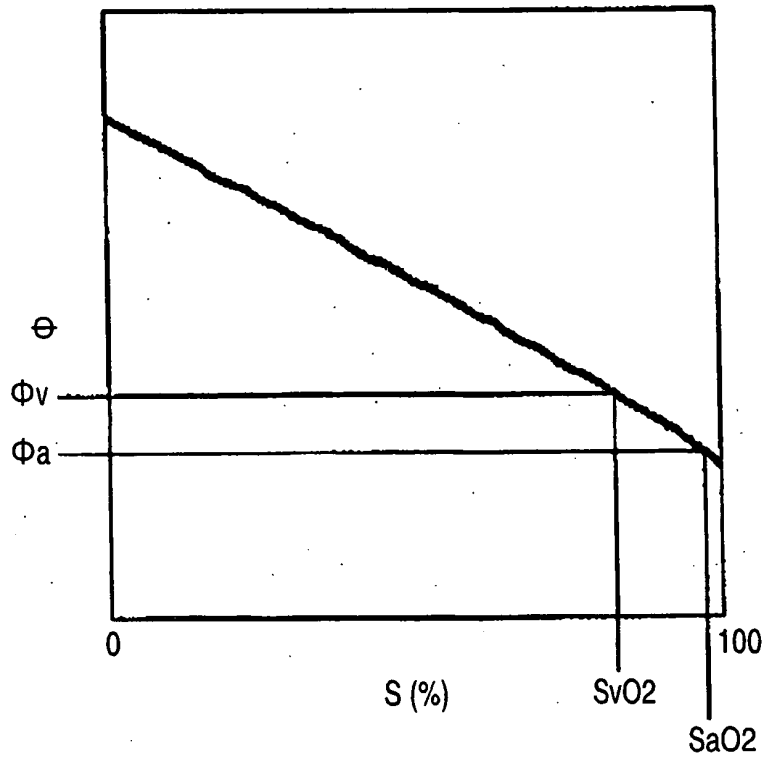


FIG. 10B

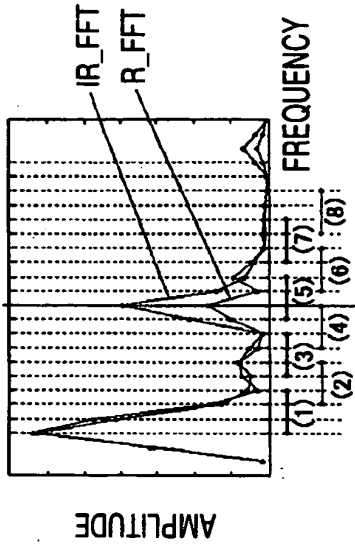


FIG. 10C

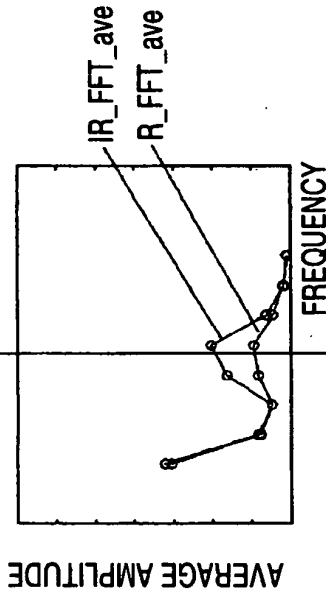


FIG. 10D


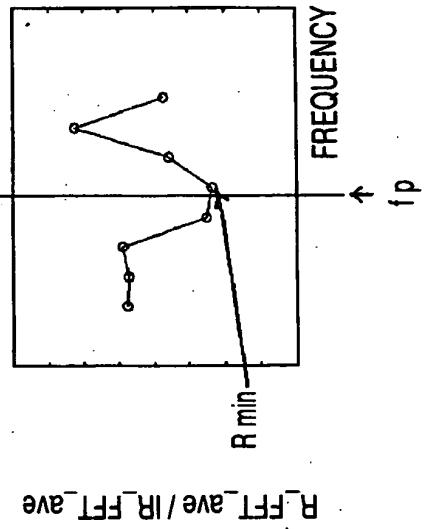


FIG. 10A

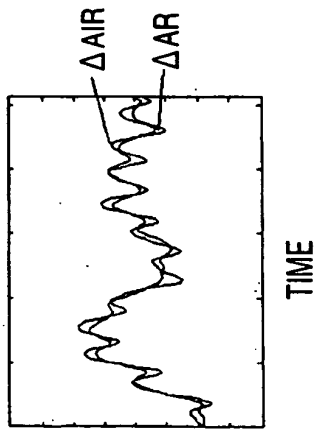

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 3270917 B [0006]
- JP 2003135434 A [0008]
- JP 2005095581 A [0008]
- JP 2005245574 A [0008]
- US 4934372 A [0010]

| | | | |
|----------------|--|---------|------------|
| 专利名称(译) | 用于测量血液中氧饱和度的装置和方法 | | |
| 公开(公告)号 | EP1757224B1 | 公开(公告)日 | 2011-01-05 |
| 申请号 | EP2006017637 | 申请日 | 2006-08-24 |
| [标]申请(专利权)人(译) | 日本光电工业株式会社 | | |
| 申请(专利权)人(译) | 日本光电公司 | | |
| 当前申请(专利权)人(译) | 日本光电公司 | | |
| [标]发明人 | KOBAYASHI NAOKI MIYATA KENJI YARITA MASARU ITO KAZUMASA | | |
| 发明人 | KOBAYASHI, NAOKI MIYATA, KENJI YARITA, MASARU ITO, KAZUMASA | | |
| IPC分类号 | A61B5/00 | | |
| CPC分类号 | A61B5/14551 A61B5/7257 | | |
| 优先权 | 2006205453 2006-07-28 JP 2005242574 2005-08-24 JP | | |
| 其他公开文献 | EP1757224A2 EP1757224A3 | | |
| 外部链接 | Espacenet | | |

摘要(译)

在用于测量血液中的氧饱和度的装置中，多个光发射器适于用具有不同波长的多个光束照射活组织。光接收器适于接收从活组织反射或透过活组织的光束，以根据活组织中血液的脉动产生脉冲波信号。分离器可操作以将每个脉冲波信号分离成多个幅度信号，每个幅度信号与一个频率相关联，从而产生幅度信号对，每个幅度信号与多个频率之一相关联。第一处理器可操作用于计算每对振幅信号中的振幅信号之间的比率。选择器可操作以选择幅度信号对中的一对。第二处理器可操作以基于所选择的一对振幅信号的比率来计算氧饱和度。

$$\Delta A = \Delta A_a = E_a \cdot H_b \cdot \Delta D_a$$