



(11) **EP 3 669 775 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
24.06.2020 Bulletin 2020/26

(51) Int Cl.:
A61B 5/053 ^(2006.01) **A61B 5/0402** ^(2006.01)
A61B 5/00 ^(2006.01) **A61B 5/0404** ^(2006.01)

(21) Application number: **19217937.2**

(22) Date of filing: **19.12.2019**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
KH MA MD TN

(72) Inventors:
• **GOVARI, Assaf**
2066717 Yokneam (IL)
• **EPHRATH, Yaron**
370969 Karkar (IL)

(74) Representative: **Small, Gary James**
Carpmaels & Ransford LLP
One Southampton Row
London WC1B 5HA (GB)

(30) Priority: **21.12.2018 US 201816230654**

(71) Applicant: **Biosense Webster (Israel) Ltd.**
Yokneam, 2066717 (IL)

(54) **IMPEDANCE MEASUREMENTS TO PREVENT NOISE ON ECG**

(57) A system and method for measuring the impedance of one or more of a plurality of leads in an electrocardiogram (ECG) are disclosed. These may include applying a plurality of leads to a patient's body, applying a plurality impedance pads to the patient's body, providing a burst pulse from the catheter electrode of the ECG, measuring impedance signals across ones of the plurality of impedance pads and the plurality of leads, and determining the impedance for one or more leads from the measure impedance signals. The plurality of impedance pads may define a first axis from the ride side of the patient's chest to the left side of the patient's chest, a second axis from the upper chest area of the patient to the lower abdomen area of the patient, and a third axis from the center of the patient's back to the center of the patient's chest. It is further described a method for measuring impedance in a bipolar configuration comprising applying a plurality of ECG leads to a patient's body and measuring impedance signals across paired ones of the plurality of leads during periods between ECG measurements.

400

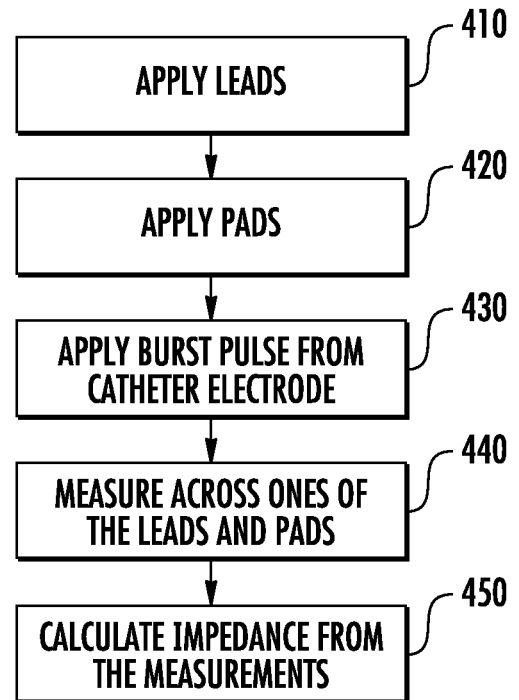


FIG. 4

EP 3 669 775 A1

Description

FIELD OF INVENTION

[0001] The present invention is related to electrocardiography, referred to herein as ECG, and may also be referred to as EKG. More particularly, the present invention is related to impedance measurements using burst pulses to prevent noise on ECG.

BACKGROUND

[0002] Currently, electrocardiography, referred to herein as ECG, and may also be referred to as EKG, is effected by the impedance of the patient's body, of the contact to connect the probes to the patient's body, and from the connections themselves. In order to understand and read the ECG, this impedance needs to be accounted for. When physicians use an ECG to study heart activity, an accounting for the impedance needs to occur in order to effectively isolate the electrical signals from the heart. Previous attempts to determine the impedance have been made using frequency multiplexing. In these frequency multiplexing attempts, other frequencies are used to measure the impedance. These other frequencies are generally high frequency and do not interfere with the measurements of the electrical signals from the heart. However, the significantly different frequencies used effects the accuracy of the measurements of the impedance. That is, the response may vary based on the frequency of the signal, and because of the difference in frequency, frequency multiplexing, tends to affect the accuracy. Therefore, a need exists to provide improved methods of measuring the impedance so that the effects of such impedance may be removed from the ECG study thereby allowing the electrical signals of the heart to be discerned more clearly.

BRIEF DESCRIPTION OF THE DRAWINGS

[0003] A more detailed understanding may be had from the following description, given by way of example in conjunction with the accompanying drawings wherein:

Figure 1 illustrates a block diagram of an ECG device for performing impedance measurements using burst pulses to prevent noise;

Figure 2 illustrates a depiction of the impedance configuration using impedance pads for measuring the impedance in conjunction with the device of Figure 1;

Figure 3 illustrates a depiction of the lead configuration in conjunction with the device of Figure 1;

Figure 4 illustrates a method of the present invention for measuring impedance using burst pulses in a unipolar configuration; and

Figure 5 illustrates a method of the present invention for measuring impedance in a bipolar configuration.

DETAILED DESCRIPTION

[0004] Electrocardiography, referred to herein as ECG, and may also be referred to as EKG, is the process of recording the electrical activity of the heart over a period of time using electrodes placed on the skin, or inside the heart using a specialized catheter (i.e. intracardiac ECG). These electrodes detect the small electrical changes that arise from the heart muscle's electro-physiologic pattern of depolarizing during each heartbeat. ECGs are commonly or routinely performed cardiology tests.

[0005] An intracardiac electrogram (ICEG) is an ECG with some added intracardiac leads (that is, inside the heart). Such an electrogram may be utilized in combination with, or in the alternative to, a conventional 12-lead ECG. In a conventional 12-lead ECG, 10 electrodes are placed on the patient's limbs and on the surface of the chest. The overall magnitude of the heart's electrical potential is then measured from 12 different angles ("leads") and is recorded over a period of time. The procedure duration may vary from tens of minutes to several hours. During each procedure usually there are several dozens of ablation sessions, each of which last several seconds up to approximately 1 minute, for example. By way of example, a conventional 12-lead ECG may be performed over a period of time, such as 10 seconds, for example. In this way, the overall magnitude and direction of the heart's electrical depolarization is captured at each moment throughout the cardiac cycle. A graph of voltage versus time produced by this medical procedure is referred to as an electrocardiogram.

[0006] During each heartbeat, a healthy heart has an orderly progression of depolarization. This orderly pattern of depolarization gives rise to the characteristic ECG tracing. To the trained clinician, an ECG conveys a large amount of information about the structure of the heart and the function of its electrical conduction system. Among other things, an ECG can be used to measure the rate and rhythm of heartbeats, the size and position of the heart chambers, the presence of any damage to the heart's muscle cells or conduction system, the effects of cardiac drugs, and the function of implanted pacemakers. Interpretation of the ECG is fundamentally about understanding the electrical conduction system of the heart. Normal conduction starts and propagates in a predictable pattern, and deviation from this pattern can be a normal variation or be pathological.

[0007] However, in order to ascertain the signals from the electrical conduction system of the heart, the measured signals need to be filtered to remove any unwanted and spurious signals or noise.

[0008] A system and method for measuring the impedance of one or more of a plurality of leads in an electrocardiogram (ECG) are disclosed. The system and method may include applying a plurality of leads to a patient's body, applying a plurality impedance pads to the patient's body, providing a burst pulse from the catheter electrode

of the ECG, measuring impedance signals across ones of the plurality of impedance pads and the plurality of leads, and determining the impedance for one or more leads from the measured impedance signals. The plurality of impedance pads defines a first axis from the right side of the patient's chest to the left side of the patient's chest. The plurality of impedance pads defines a second axis from the upper chest area of the patient to the lower abdomen area of the patient. The plurality of impedance pads defines a third axis from the center of the patient's back to the center of the patient's chest. The plurality of leads includes a standard 12-lead ECG including three limb leads, three augmented limb leads arranged in a spoke fashion in the coronal plane, and six precordial leads configured on the perpendicular traverse plane.

[0009] The system and method may alternatively include applying a plurality of leads to a patient's body and measuring impedance signals across paired ones of the plurality of the plurality of leads during periods between ECG measurements. The plurality of leads includes a standard 12-lead ECG including three limb leads, three augmented limb leads arranged in a spoke fashion in the coronal plane, and six precordial leads configured on the perpendicular traverse plane. The plurality of leads is each paired to an adjacent one of the plurality of leads.

[0010] The system for performing an ECG and measuring impedance includes a plurality of leads for attaching to a subject in order to capture electric signals, a signal processor to process the captured electrical signals, and an output device to output the process captured electrical signals, wherein the impedance of the measurements is monitored and the signal processor removes the impedance from the process captured electrical signals. The system may include a plurality of impedance pads configured to provide impedance information for the measurements. A catheter electrode may provide a burst pulse to enable the measurement of the impedance information. The system may alternatively measure the impedance information across pairs of the plurality of electrodes.

[0011] Figure 1 illustrates a block diagram of a device 100 in which the impedance measurements using burst pulses may be utilized. Device 100 may take the form of an ECG machine. Device 100 includes a series of leads 110 that taper into a single multiplexed input 115. The series of leads 110 may be placed on a human test subject 105. Additional leads 107, which may be included with series of leads 110, or separate therefrom (as shown) may be intracardiac leads 107.

[0012] Intracardiac leads 107 may be used for diagnostic or therapeutic treatment, such as for mapping electrical potentials in a heart 126 of a patient 105. Alternatively, intracardiac leads 107 may be used, *mutatis mutandis*, for other therapeutic and/or diagnostic purposes in the heart or in other body organs.

[0013] Intracardiac leads 107 may be inserted in the vascular system of the patient 105 so that a distal end 132 of the leads 107 enters a chamber of the patient's

heart 126. Although Figure 1 shows a single lead 107 with a single location sensor, embodiments of the present invention may utilize probes with more than one location sensor.

[0014] The signals on the series of leads 110 are input into an analog front-end 125 via an input multiplexor 120. The analog front-end 125 provides to, and is controlled by, a processor 130. Processor 130 may include, as shown, a video controller 135, digital signal processor 140, a microprocessor 145, and a micro controller 150. Processor 130 is coupled to a data storage 155. Data ports and printers 160 may be coupled to processor 130. Other input/output devices 165 may be coupled to processor 130. A display 170 may be used to provide output of the signals of the ECG. A power/battery management system 175 may be included to provide power for device 100 to operate.

[0015] Series of leads 110 includes both the generally used forms of electrodes and may also include leads used for ECG procedures. Each of the series of leads 110 may include a conductive pad in contact with the body 105 that makes an electrical circuit with the electrocardiograph. On a standard 12-lead ECG there are only 10 leads 110. Series of leads 110 may be grouped into three sets: limb, augmented limb, and precordial. Generally, the 12-lead ECG has a total of three limb leads and three augmented limb leads arranged like spokes of a wheel in the coronal plane (vertical) and six precordial leads that lie on the perpendicular transverse plane (horizontal).

[0016] Analog front-end 125 receives the signals from the series of leads 110 and performs analog processing, such as filtering, of the signals.

[0017] Data storage 155 is any device that records information. Data storage may provide a storage medium for the signals includes within device 100 and a place for calculations of processor 130 to be stored.

[0018] Microprocessor 145 may be a computer processor which incorporates the functions of a computer's central processing unit (CPU) on a single integrated circuit (IC), or a few integrated circuits. Microprocessor 145 may be a multipurpose, clock driven, register based, programmable electronic device which accepts digital or binary data as input, processes it according to instructions stored in its memory or data storage 155, and provides results as output. Microprocessor 145 contains both combinational logic and sequential digital logic.

[0019] Micro controller 150 may be one or more small computers on a single integrated circuit. Micro controller 150 may contain one or more CPUs along with memory and programmable input/output peripherals. Program memory in the form of Ferroelectric RAM, NOR flash or OTP ROM is also often included on chip, as well as a small amount of RAM. Microcontrollers are designed for embedded applications, in contrast to the microprocessors used in personal computers or other general purpose applications consisting of various discrete chips.

[0020] Digital signal processor 140 may perform digital

signal processing to perform a wide variety of signal processing operations. The signals processed in this manner are a sequence of numbers that represent samples of a continuous variable in a domain such as time, space, or frequency. Digital signal processing can involve linear or nonlinear operations. Nonlinear signal processing is closely related to nonlinear system identification and can be implemented in the time, frequency, and spatio-temporal domains. The application of digital computation to signal processing allows for many advantages over analog processing in many applications, such as error detection and correction in transmission as well as data compression. DSP is applicable to both streaming data and static (stored) data.

[0021] Figure 2 illustrates a depiction of the impedance configuration 200 using impedance pads for measuring the impedance in conjunction with the device of Figure 1. Configuration 200 includes a series of impedance pads configured to measure impedance in each of three axes with respect to a patient 250. A first axis first impedance pad 205 may be placed on the right side of a patient's 250 chest. Pad 205 may form an axis (first axis) (shown horizontal in Figure 2) with a first axis second impedance pad 210 located on the left side of the patient's 250 chest.

[0022] A second impedance axis (second axis) (shown vertical in Figure 2) may be defined by a second axis first impedance pad 215 and a second axis second impedance pad 220. Second axis first impedance pad 215 may be placed on the upper chest or throat of the patient 250. Second axis second impedance pad 220 may be located on the patient's 250 abdomen.

[0023] A third impedance axis (third axis) (shown coming in and out of page of Figure 2) may be defined by a third axis first impedance pad 225 and a third axis second impedance pad 230. Third axis first impedance pad 225 may be placed in the center of the patient's 250 back. Third axis second impedance pad 230 may be placed in the center of a patient's 250 chest.

[0024] The present system for coordinating impedance measurements with ECG studies utilizes electrical signals transmitted from a catheter electrode (not shown in Figure 2) to six pads 205, 210, 215, 220, 225, 230 on the patient 250 to measure the impedance. As would be understood to those familiar with an ECG procedure, the catheter electrode may be located directly in the patient's heart. For example, the catheter may be inserted internally into the patient's heart. The catheter electrode may be contained at the tip of the shaft of the catheter, for example. The catheter electrode emits burst pulses of low-frequency electrical signals, from less than 1 millampere to 100 microamperes, which are absorbed by the six pads 205, 210, 215, 220, 225, 230 on the patient's 250 body. Generally, the use of pads 205, 210, 215, 220, 225, 230 and the catheter electrode is a unipolar measurement. The burst pulses may be of the same, or approximately the same, frequency as the signals that are measured during the ECG in order to remove any frequency error in the measurement and removal of the im-

pedance.

[0025] By way of example only, each channel in an ECG test may be sampled 20,000 times per second with a measurement time of 1/640 seconds. This allows for approximately slightly less than 1/20000 of a second in between measurements during which time, the time multiplexing may be employed to measure the impedance. More specifically, in this example, the time between measurements may be 1/19200 seconds.

[0026] The burst pulses from the catheter may be provided when the ECG is not sampling the electrical signals from the heart. This time multiplexing avoids interference with the ECG readings. Because the system uses time multiplexing (and not frequency multiplexing), any frequency may be used for the burst pulse. This allows signals at the same or approximately the same frequency to be used to measure the impedance. The electrical signals from the heart are not sampled continuously, only sampled in multiplex. Thus, the catheter electrode may be used when the electrical signals from the heart are not being sampled. Typical values are approximately 100-200 ohms.

[0027] Figure 3 illustrates a depiction of the lead configuration 300 in conjunction with the device of Figure 1. Lead configuration 300 includes a series of leads configured to measure electrical signals with respect to a patient 350. Generally, there are ten leads that are connected to specific parts of the body. The leads are of two groups: six chest leads 325 and four peripheral leads 335.

[0028] Six chest leads 325 are generally positioned with respect to the rib cage of the patient 350. The first of the chest leads 325₁ is located near the center of the patient's 350 chest. Side lead 325₆ is located on the side of the patient's 350 body. The other chest leads 325₂, 325₃, 325₄, 325₅ are located in between first chest lead 325₁ side chest lead 325₆. By way of information, chest lead 325₂ is located at the intersection of the 4th intercostal space and the sternum of the patient 350. Chest lead 325₄ is located in the 5th intercostal space, in line with the middle of the clavicle. Chest lead 325₃ may be positioned midway between chest lead 325₂ and chest lead 325₄. Chest lead 325₅ may be located in the 5th intercostal space in the under-arm area.

[0029] The four peripheral leads 335 may be located to capture signals at the left and right wrists and left and right legs. While referencing the signal from the arms and legs, these leads may be located on the shoulders and abdomen (as shown) or on the limbs directly. For example, lead 335_{RA} may be located on the right shoulder of the patient 350, lead 335_{LA} may be located on the left shoulder of the patient 350, lead 335_{RL} may be located on the lower right abdomen of the patient 350, and 335_{RL} may be located on the lower left abdomen of the patient 350. Individually, the leads may be utilized as described in a unipolar configuration where each leads operates alone. Such leads may be brought together and tied to a ground or the pads, for example.

[0030] Alternatively, the leads may be used in a bipolar

configuration. That is, the leads may be used in a pair with the signal gathered between the leads. For example, the leads across the imaginary Einthoven triangle may be used.

[0031] Impedance may be measured by transmitting from one lead to another. Such impedance measurements may utilize the leads 325 already included on the patient's 350 body, and therefore may not require the pads shown and described with respect to Figure 2. The measuring of impedance between two leads is referred to as a bipolar measurement of impedance.

[0032] The use of the leads in a bipolar measurement may provide the additional benefit that the leads furthest from the most recent measurement may be used to measure impedance. For example, if the electrical signals of the heart are being measured on leads 1 and 2, then the impedance may be measured on leads 16 and 17. A lead may be defined as the link between two electrodes. For example, lead 1 may be defined as being the link between leads 335_{LA} and 335_{RA}, for example. Lead 2 may include the link between leads 335_{RA} and 335_{LL}. Lead 3 may include the link between leads 335_{LA} and 335_{LL}. One pattern that may be used is by connecting an electrode to the adjacent electrode to form the pair, for example. Other leads formed from the combinations of electrodes may also be used as would be evident to those possessing an ordinary skill in the pertinent art based on the disclosure contained herein.

[0033] During bipolar operation, the window of opportunity for making a bipolar impedance measurement at a minimum of 20 kHz sampling provides a 50 μ s per electrode. In order to achieve the measurement, a multiplexer may provide a connection over which to measure the impedance between two electrodes for 3 μ s. Sampling up to 200 kHz may be utilized. During a given window of opportunity only a single lead is connected while N-1 leads are not connected.

[0034] Figure 4 illustrates a method 400 that may be performed in a unipolar configuration. Method 400 includes applying a plurality of leads at step 410. At step 420, method 400 includes applying a plurality impedance pads. At step 430, a unipolar impedance measurement may be performed by applying a burst pulse from the catheter electrode. A plurality of measurements may be taken across ones of the plurality of impedance pads and the plurality of leads at step 440. At step 450, the impedance for one or more leads may be determined from the plurality of measurements.

[0035] Figure 5 illustrates a method 500 that may be performed in a bipolar configuration. Method 500 includes applying a plurality of leads at step 510. At step 520, a bipolar impedance measurement may be performed across ones of the pairs of leads between ECG measurements.

[0036] The methods provided can be implemented in a general purpose computer, a processor, or a processor core. Suitable processors include, by way of example, a general purpose processor, a special purpose processor,

a conventional processor, a digital signal processor (DSP), a plurality of microprocessors, one or more microprocessors in association with a DSP core, a controller, a microcontroller, Application Specific Integrated Circuits (ASICs), Field Programmable Gate Arrays (FPGAs) circuits, any other type of integrated circuit (IC), and/or a state machine. Such processors can be manufactured by configuring a manufacturing process using the results of processed hardware description language (HDL) instructions and other intermediary data including netlists (such instructions capable of being stored on a computer readable media). The results of such processing can be maskworks that are then used in a semiconductor manufacturing process to manufacture a processor which implements features of the disclosure.

[0037] The methods or flow charts provided herein can be implemented in a computer program, software, or firmware incorporated in a non-transitory computer-readable storage medium for execution by a general purpose computer or a processor. Examples of non-transitory computer-readable storage mediums include a read only memory (ROM), a random access memory (RAM), a register, cache memory, semiconductor memory devices, magnetic media such as internal hard disks and removable disks, magneto-optical media, and optical media such as CD-ROM disks, and digital versatile disks (DVDs).

30 Claims

1. A method for measuring the impedance of one or more of a plurality of leads in an electrocardiogram (ECG), the method comprising:
 - applying a plurality of leads to a patient's body;
 - applying a plurality impedance pads to the patient's body;
 - providing a burst pulse from the catheter electrode of the ECG;
 - measuring impedance signals across ones of the plurality of impedance pads and the plurality of leads; and
 - determining the impedance for one or more leads from the measure impedance signals.
2. The method of claim 1 wherein the plurality of impedance pads defines (i) a first axis from the right side of the patient's chest to the left side of the patient's chest, (ii) a second axis from the upper chest area of the patient to the lower abdomen area of the patient, and/or (iii) a third axis from the center of the patient's back to the center of the patient's chest.
3. A method for measuring the impedance of one or more of a plurality of leads in an electrocardiogram (ECG), the method comprising:

- applying a plurality of leads to a patient's body;
and
measuring impedance signals across paired
ones of the plurality of the plurality of leads dur-
ing periods between ECG measurements. 5
4. The method of claim 1 or claim 3 wherein the plurality
of leads includes a standard 12-lead ECG.
5. The method of claim 1 or claim 3 wherein the plurality 10
of leads includes three limb leads.
6. The method of claim 1 or claim 3 wherein the plurality
of leads includes three augmented limb leads ar-
ranged in a spoke fashion in the coronal plane. 15
7. The method of claim 1 or claim 3 wherein the plurality
of leads includes six precordial leads configured on
the perpendicular traverse plane. 20
8. The method of claim 3 wherein ones of the plurality
of leads are each paired to an adjacent one of the
plurality of leads.
9. The method of claim 8 wherein the pairing provides 25
two impedance measurements for each of the ones
of the plurality of leads.
10. The method of claim 9 wherein the two impedance
measurements are averaged to provide the imped-
ance of the lead. 30
11. A system for performing an electrocardiograph
(ECG) and measuring impedance, the system com-
prising: 35
- a plurality of leads for attaching to a subject in
order to capture electric signals;
a signal processor to process the captured elec-
trical signals; and 40
- an output device to output the process captured
electrical signals,
wherein the impedance of the measurements is
monitored and the signal processor removes the
impedance from the process captured electrical 45
signals.
12. The system of claim 11 further comprising a plurality
of impedance pads configured to provide impedance
information for the measurements. 50
13. The system of claim 12 wherein a catheter electrode
provides a burst pulse to enable the measurement
of the impedance information. 55
14. The system of claim 11 wherein the impedance in-
formation for the measurements is measured across
pairs of the plurality of electrodes.

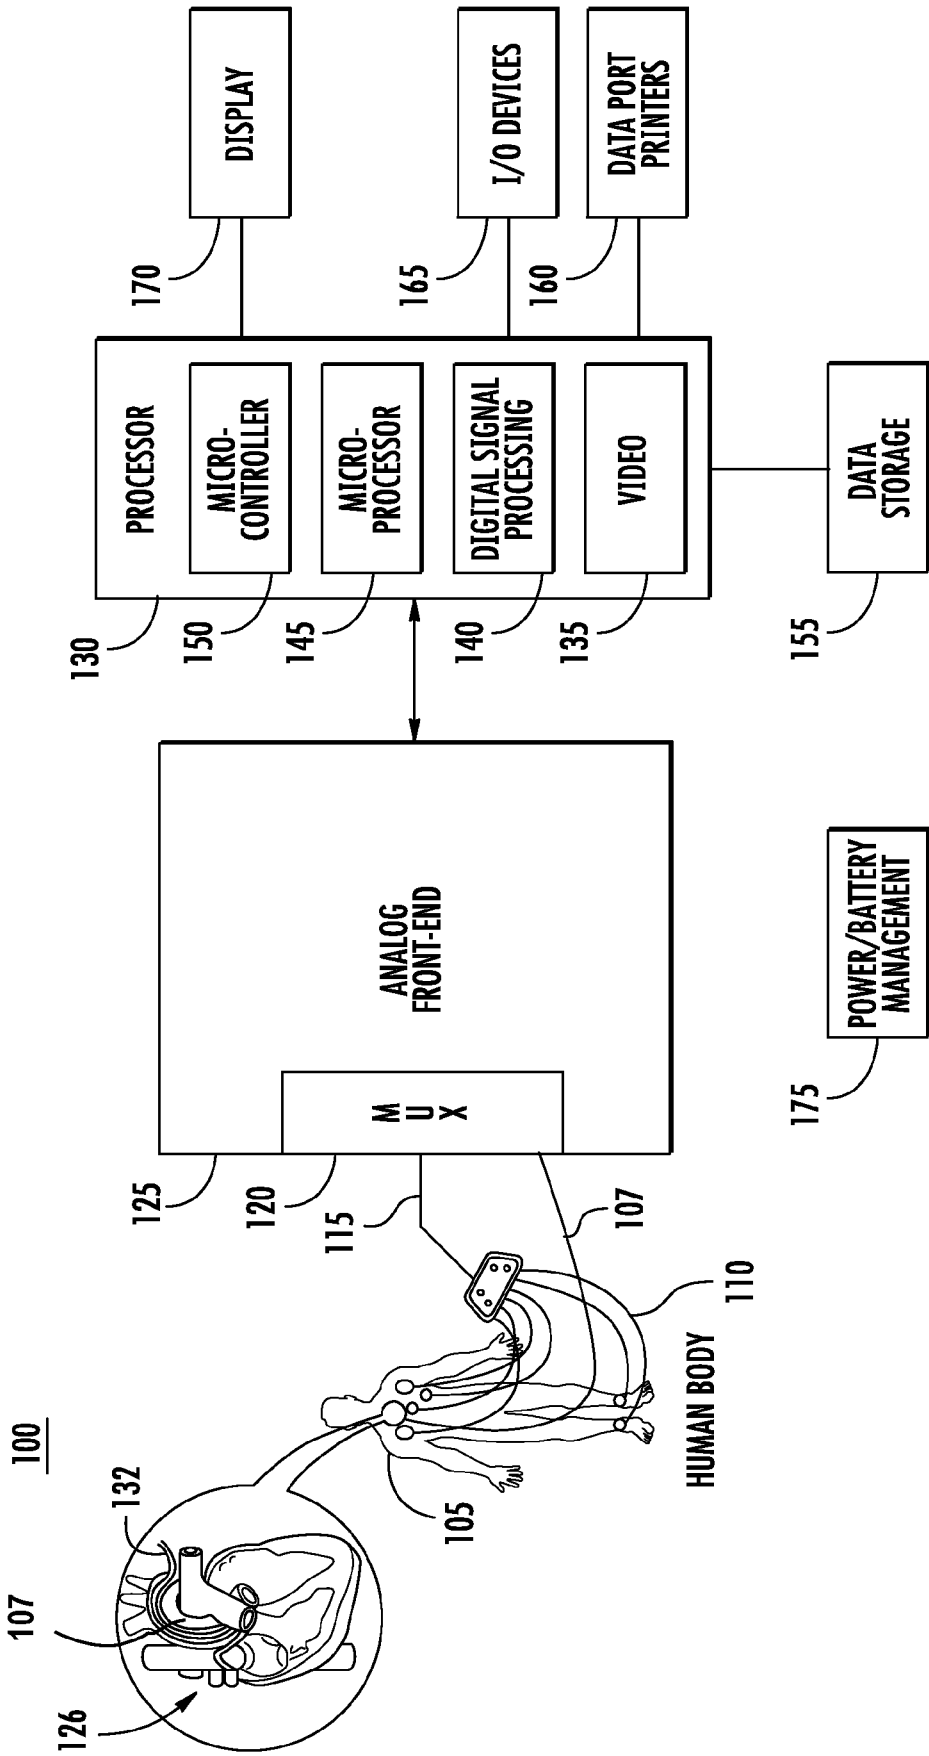


FIG. 1

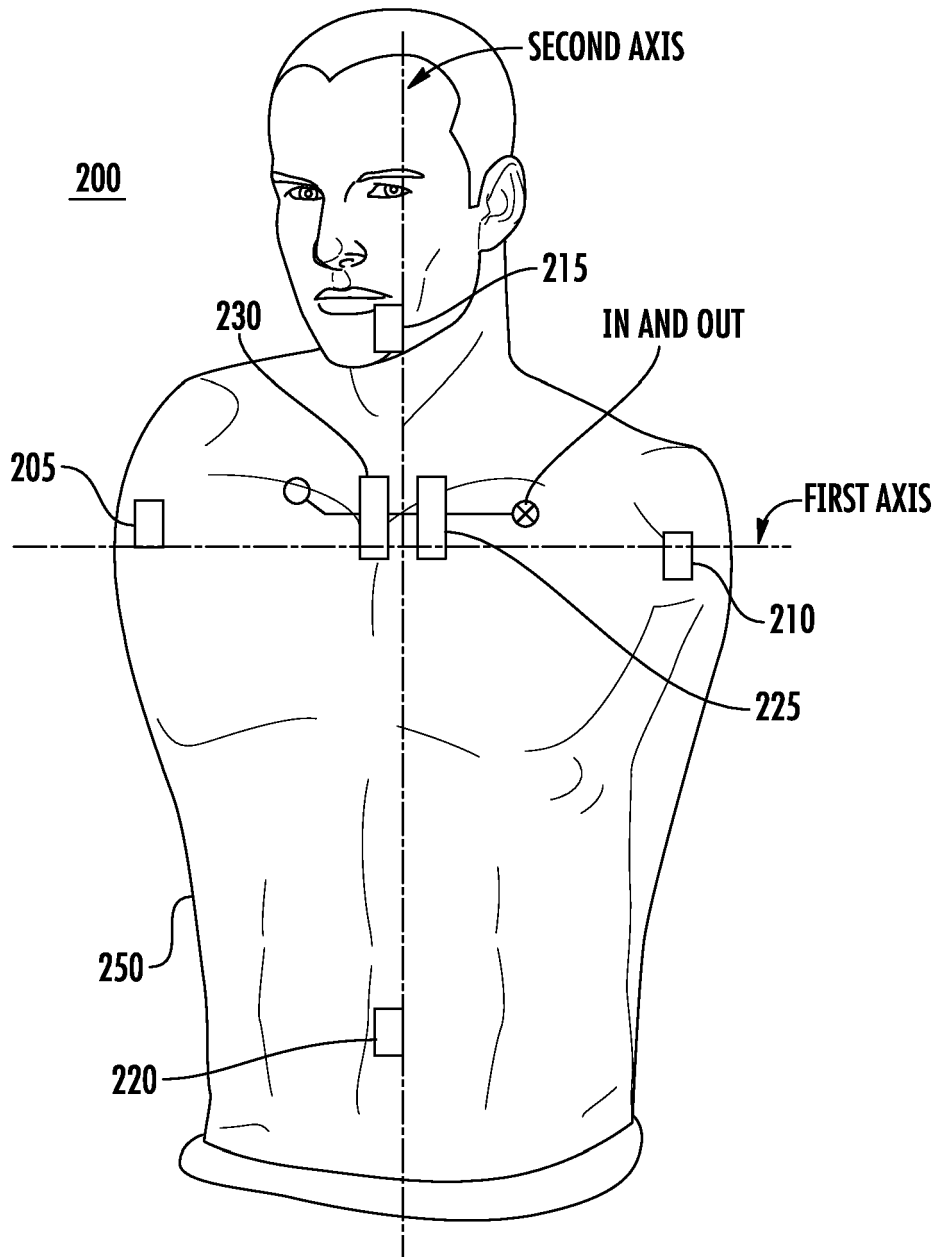


FIG. 2

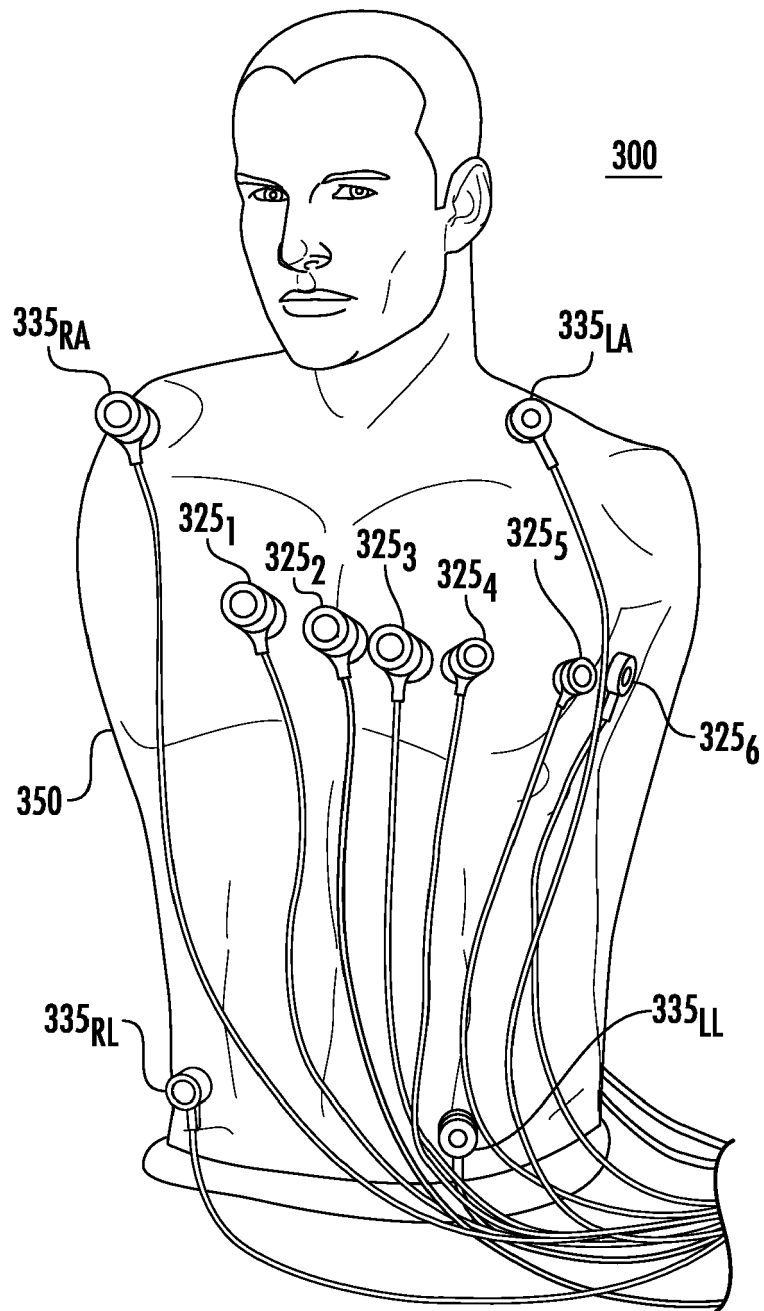


FIG. 3

400

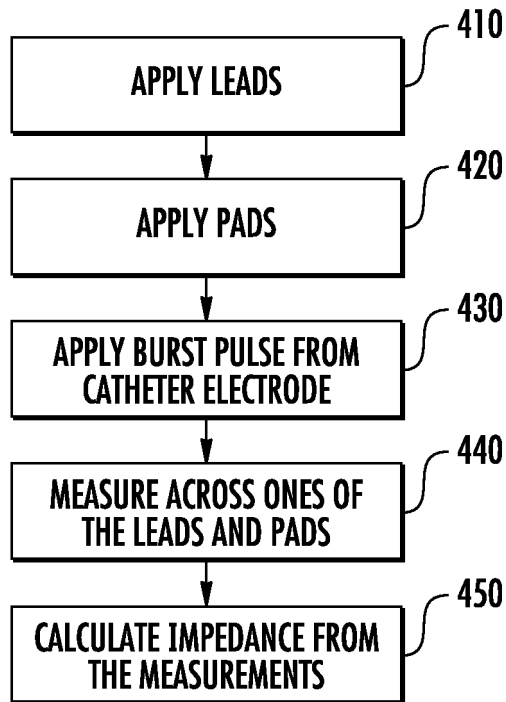


FIG. 4

500

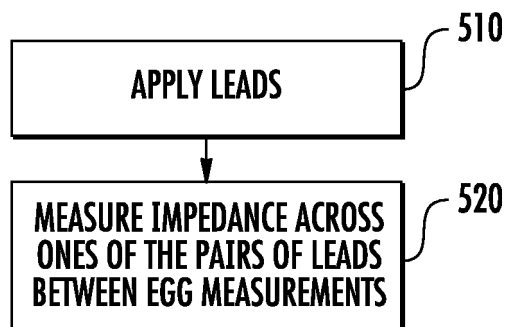


FIG. 5



EUROPEAN SEARCH REPORT

Application Number
EP 19 21 7937

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	WO 2014/051590 A1 (DRAEGER MEDICAL SYSTEMS INC [US]) 3 April 2014 (2014-04-03) * the whole document * -----	3-14	INV. A61B5/053 A61B5/0402 A61B5/00
X	US 2016/203608 A1 (IZMIRLI ALON [IL] ET AL) 14 July 2016 (2016-07-14) * paragraphs [0055] - [0056] * -----	3-10	ADD. A61B5/0404
X	WO 2009/036313 A1 (CORVENTIS INC [US]; MANICKA YATHEENDHAR D [US] ET AL.) 19 March 2009 (2009-03-19) * paragraphs [0195], [0200] - [0203]; figures 3,4 * -----	3-10	
A	US 5 704 365 A (ALBRECHT PAUL [US] ET AL) 6 January 1998 (1998-01-06) * the whole document * -----	1-14	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61B
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 12 May 2020	Examiner Dhervé, Gwenaëlle
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

1
EPO FORM 1503 03/02 (P04C01)

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 19 21 7937

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

12-05-2020

10

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2014051590 A1	03-04-2014	NONE	
US 2016203608 A1	14-07-2016	NONE	
WO 2009036313 A1	19-03-2009	EP 2194847 A1 US RE46926 E US 2009076345 A1 US 2009076363 A1 US 2012108920 A1 US 2013085347 A1 US 2013253285 A1 US 2014330136 A1 US 2015005589 A1 WO 2009036313 A1	16-06-2010 03-07-2018 19-03-2009 19-03-2009 03-05-2012 04-04-2013 26-09-2013 06-11-2014 01-01-2015 19-03-2009
US 5704365 A	06-01-1998	EP 0957760 A1 US 5704365 A US 5713367 A WO 9614796 A1	24-11-1999 06-01-1998 03-02-1998 23-05-1996

15

20

25

30

35

40

45

50

55

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

专利名称(译)	使用突发脉冲来预防ECG上的噪声的阻抗测量		
公开(公告)号	EP3669775A1	公开(公告)日	2020-06-24
申请号	EP2019217937	申请日	2019-12-19
[标]申请(专利权)人(译)	韦伯斯特生物官能(以色列)有限公司		
申请(专利权)人(译)	生物传感韦伯斯特(以色列)LTD.		
当前申请(专利权)人(译)	生物传感韦伯斯特(以色列)LTD.		
[标]发明人	GOVARI ASSAF EPHRATH YARON		
发明人	GOVARI, ASSAF EPHRATH, YARON		
IPC分类号	A61B5/053 A61B5/0402 A61B5/00 A61B5/0404		
CPC分类号	A61B5/04011 A61B5/0402 A61B5/0404 A61B5/053 A61B5/7203 A61B5/0006 A61B5/04017 A61B5/0408 A61B5/6823		
优先权	16/230654 2018-12-21 US		
外部链接	Espacenet		

摘要(译)

公开了一种用于测量心电图 (ECG) 中的多个引线中的一个或多个的阻抗的系统和方法。 这些可包括：将多个引线施加到患者的身体；将多个阻抗垫施加到患者的身体；提供来自ECG的导管电极的突发脉冲；测量跨多个阻抗垫和多个阻抗垫中的一个的阻抗信号。 导线，并根据测量阻抗信号确定一根或多根导线的阻抗。 多个阻抗垫可以限定从患者的胸部的乘坐侧到患者的胸部的左侧的第一轴线，从患者的上胸部区域到患者的下腹部区域的第二轴线以及第三轴线。 从患者背部中心到患者胸部中心的轴线。 还描述了一种用于在双极配置中测量阻抗的方法，该方法包括将多个ECG引线施加到患者的身体，并在ECG测量之间的时间间隔内跨多个引线中的成对引线测量阻抗信号。

400

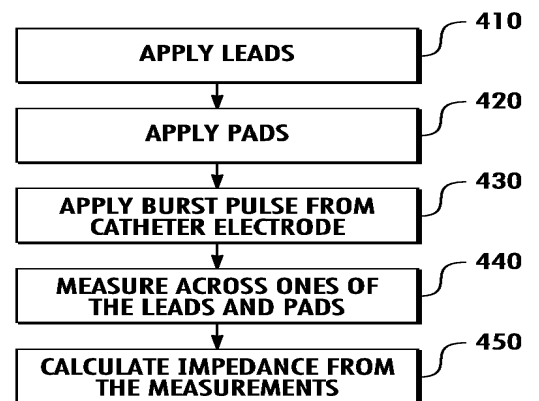


FIG. 4