

(19) World Intellectual Property
Organization
International Bureau




(43) International Publication Date
29 April 2004 (29.04.2004)

PCT

(10) International Publication Number
WO 2004/034896 A1

- (51) International Patent Classification⁷: **A61B 5/00**
- (21) International Application Number: PCT/GB2003/004487
- (22) International Filing Date: 16 October 2003 (16.10.2003)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
0224299.8 18 October 2002 (18.10.2002) GB
- (71) Applicant (for all designated States except US):
CAMBRIDGE NEUROTECHNOLOGY LIMITED [GB/GB]; Upper Pendrill Court, Ermine Street North, Papworth Everard, Cambridgeshire CB3 8UY (GB).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **UNGLESS, Gary, Steven** [GB/GB]; c/o Cambridge Neurotechnology Limited, Upper Pendrill Court, Ermine Street North, Papworth Everard, Cambridgeshire CB3 8UY (GB). **OAKELY, Nigel, Robert** [GB/GB]; c/o Cambridge Neurotechnology Limited, Upper Pendrill Court, Ermine Street North, Papworth Everard, Cambridgeshire CB3 8UY (GB).
- (74) Agent: **GOODMAN, Simon, John, Nye**; Reddie & Grose, 16 Theobalds Road, London WC1X 8PL (GB).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
- with international search report
 - before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: CARDIAC MONITORING APPARATUS AND METHOD

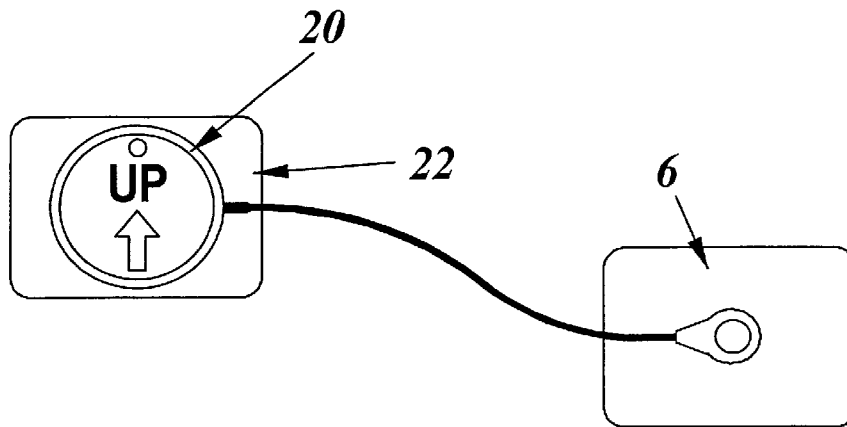

(57) Abstract: A monitor includes a cardiac sensor (36) responsive to a user's heart beat. The monitor includes a processor coupled to the sensor for generating heart-rate or other cardiac data. These data can be stored in a memory. The monitor is physically supported by and receives electrical signals from a single ECG electrode, and is coupled by an electrical lead to a second ECG electrode.

WO 2004/034896 A1

Cardiac Monitoring Apparatus and Method

This invention relates to a cardiac monitoring apparatus and method for monitoring a user's heart rate, or other parameters derived from heart-beat sensing.

5 Heart rate is a physiological parameter that is measured in a wide variety of situations, for example to determine the health status and fitness of a person or animal. It can be used, for example, to give a measure of energy expenditure of an individual and a number of devices exist
10 for doing this by converting heart rate to calories used. Many conventional systems comprise a belt worn around a user's chest and carrying a heart-beat sensor and a radio transmitter for transmitting measured data to a wrist-worn display unit.

15 Such conventional systems are generally uncomfortable or impractical to wear for extended periods and also suffer a significant problem in that correlating heart rate with calories used may only be effective for exercise rates achieving significant heart rate increases. Smaller
20 increases in heart rate can be due to, for example, stress rather than physical exertion and may therefore be misinterpreted by conventional heart-rate monitoring systems.

The invention provides an apparatus and a method for
25 monitoring a user's heart as defined in the appended independent claims. Preferred or advantageous features of the invention are set out in dependent subclaims.

- 2 -

The invention may thus advantageously provide a monitor for monitoring a user's heart, comprising a cardiac sensor and a support means for mounting the monitor only on a single adhesive pad, which is preferably an
5 electrocardiogram (ECG) electrode. The monitor is then advantageously both physically supported by the single electrode and electrically connected to it for receiving signals for monitoring the user's heart. A lead extends from the monitor to receive signals from a second ECG
10 electrode, spaced from the first, to enable cardiac monitoring. Further leads coupling the monitor to further ECG electrodes may advantageously allow monitoring of more than one ECG channel. The leads may either extend from a monitor housing or plug into sockets in the monitor
15 housing.

The monitor may comprise a memory for recording data from the cardiac sensor over a period of time, which may then be downloaded for analysis. If more than one ECG channel is to be monitored, it preferably contains sufficient
20 memory to store data from multiple channels for an extended period, such as 24 hours or more. Since the monitor is advantageously of light weight and small size, its housing preferably being of smaller lateral dimension than an ECG pad, it may advantageously be comfortable to
25 wear continuously for periods of as long as days or more.

In a preferred embodiment, the apparatus of the invention consists of a small, lightweight monitor that may measure not only heart rate but also inter-beat interval and/or other cardiac parameters.

30 The following description of the invention refers mainly to a preferred embodiment in which the monitor further comprises an accelerometer for actigraph measurement. It

- 3 -

should be noted, however, that the skilled person will be readily able to identify and assess those features and advantages of this embodiment which similarly apply to the cardiac monitor mounted on a single ECG pad described
5 above.

In the preferred embodiment, the invention may advantageously provide a monitor comprising a heart-beat sensor and an accelerometer which can be secured in position on a single adhesive pad for sensing a user's
10 heart-beat and movement, or activity. The monitor further comprises a processor for receiving signals from the heart-beat sensor and the accelerometer and for generating heart-rate or other cardiac data, and movement or activity data. The monitor preferably comprises a memory in which
15 the data can be stored.

The monitoring of both a user's heart rate and movement addresses the problem outlined above, that heart rate increases are not necessarily correlated to physical exertion. Thus, a record of the user's movement can be
20 correlated with heart rate measurements to improve evaluation of the user's energy expenditure. The range of uses for such an apparatus or method in the medical field is widespread. For instance, it can be used in cardiology, sleep medicine, diabetes, obesity, eating
25 disorders, psychiatric disorders etc. It can also be used in monitoring the fitness levels of individuals and as a means for assessing their energy expenditure. This may be done for a variety of reasons, such as weight loss, rehabilitation, encouragement to exercise etc.

30 The monitor is preferably couplable to a conventional adhesive electrocardiogram (ECG) electrode or pad attachable to the user's chest. Two such ECG electrodes

- 4 -

are preferably used, as in conventional ECG measurement. The monitor may then clip directly to one of the ECG electrodes, achieving both electrical connection and mechanical support. An electrical lead may then couple
5 the monitor to the other ECG electrode.

Many different types of ECG electrode pads are available for many different applications, for example to cater for different patient skin types, shapes, and sensitivity, or for long term or short term applications. Thus, some
10 types of electrode have adhesive allowing for easy removal after short term use and others have stronger adhesive allowing for long term skin adhesion. As illustrated in Figure 11 some electrode types comprise an electrode gel
15 82 beneath a central portion of the pad 84 to improve electrical connection to the skin, surrounded by an adhesive portion 86 of the pad which secures the pad to the skin and retains the gel in position. ECG pads are typically fitted with a standard 4mm stud 74, couplable to an ECG lead. A monitor that mounts directly on to an ECG
20 electrode should preferably be compatible with all these types of pads.

Preferably, a zero insertion force clip is used to connect the monitor embodying the invention to a conventional ECG electrode. If an ECG electrode comprises an electrode gel
25 as described above, and a large force is applied to connect the monitor to such a pad, then this gel may be forced out past the adhesive surrounding it.

Advantageously, a zero insertion force clip, for example a slider clip, may prevent the gel being forced out. A high
30 application force for attaching a monitor to a clip may also cause the ECG electrode to deform thereby making attachment of the monitor difficult or even damaging to the electrode. This problem may be exacerbated if the

- 5 -

user, or patient, has normal or large amounts of body fat. A zero insertion force clip may, advantageously, make the monitor easier to mount and prevent distortion of the ECG electrode during mounting of the monitor.

5 Preferably, the unit is securely fixed to the ECG electrode pad so that it will not rotate on the pad during normal use. Any rotation of the monitor on the pad may cause a loss of resolution of the movement (preferably vertical movement) detected by the accelerometer.

10 Advantageously, a clip with a high clamping force may reduce rotation on the pad during normal use. A high clamping force may also, advantageously, reduce contact resistance problems. These factors may favour a high clamping force and so may further exacerbate the problems

15 arising if a zero-insertion-force clip is not used, because otherwise a high clamping force typically requires a high insertion force. In a preferred embodiment, therefore, the monitor is attached to the electrode pad by means of a zero insertion force slider clip, clamping

20 force being provided by a spring contact and the spring being manually retracted as the monitor is attached.

Being small and of light weight, the monitor is advantageously unobtrusive and can be worn for long periods by people of all ages and health or fitness

25 status.

Data from the heart-beat sensor and the accelerometer are advantageously stored in a memory within the monitor, which negates the need for radio or other transmission of data from the monitor. Data may then be downloaded from

30 the monitor by interfacing it to, for example, a computer such as a PC. In a preferred embodiment, the monitor interfaces to the PC through the same contacts as used for

- 6 -

coupling to the ECG electrodes. Particularly advantageously, the same contacts may also be used for charging a battery within the monitor.

By analysing data downloaded to a PC, it may
5 advantageously be possible to establish whether small but significant changes in heart rate (usually increases in heart rate) are due to physical exertion or not, and therefore whether heart rate increases may be due to, for example, stress. This may improve estimation of energy
10 expenditure derived from physical activity and its consequences in terms of heart rate and performance.

Alternatively, by identifying changes in heart rate which are not associated with physical activity, conditions such as stress may be identified and/or monitored.

15 In another embodiment, the monitor may interface with an external device such as a wrist-worn actigraphy device, by means of radio transmission. In this embodiment, the ECG input lead may be used as an antenna for RF output. Heart rate and activity data may then be transmitted to a wrist-
20 worn actigraphy device. Advantageously, for example this wrist-worn actigraphy device may sense reduced upper-body activity whilst the user is seated and engaged in activities such as typing or knitting, which might otherwise cause a wrist-worn actigraph, on detecting
25 significant movement, to estimate an inaccurately high level of energy expenditure. The device may then combine all the data to further enhance the measurement of physical activity and stress. More accurate measurements may be made using both chest-worn and wrist-worn
30 actigraphs in this way, but in alternative embodiments other systems may be implemented. For example a chest-worn monitor for cardiac and activity data may transmit

- 7 -

data by radio transmission to a fixed receiver, for example next to an exercise machine for monitoring the user's heart rate and activity while exercising. Alternatively a chest-worn cardiac monitor (not
5 incorporating an actigraph) could transmit cardiac data to a wrist-worn actigraph or to a fixed receiver.

Normal commercial electrode pad adhesives are designed to retain normal ECG leads and clips. In many monitoring applications, longer lead wires are required, and are
10 separately supported to prevent pulling on the electrode pad. Preferably, the monitor embodying the invention is of similar weight to a single short ECG lead wire and clip. This means that the weight of the monitor does not pull on a normal electrode pad beyond the pad's design
15 load. By being light weight, the monitor places a low load on the adhesive pad. Advantageously, this means that the monitor does not require the separate safety straps or wires that are deemed necessary for other, heavier, units mounted on multiple pads.

20 Preferably, the weight of the monitor is less than 50g, or particularly preferably less than 25g or 15g. In a preferred embodiment the monitor weighs about 10g or less.

Devices that mount on to multiple adhesive pads, or any device mounted on a single adhesive pad larger than a
25 conventional ECG electrode pad, will disadvantageously require complicated mechanical arrangements, for example articulation or a flexible housing, to allow for the free movement of the body and resulting skin expansion and contraction. Advantageously, mounting at a single point,
30 particularly on a standard ECG electrode pad, reduces the problems associated with free body movement and skin expansion and contraction. It is notable that this

- 8 -

problem is taken into account in designing conventional ECG electrodes; these are of limited size in order to avoid problems arising from skin stretching and contraction.

5 These features of preferred embodiments of the invention may solve a number of problems in prior art heart-rate monitors. In prior art systems, for example, the transmission of data from a chest band using a radio link is subject to a wide range of interference, such as from
10 electric motors, televisions, telephones etc., which typically leads to a large number of data points being lost and classed as "dropouts". Typically 10-20% of data points are lost in this way per day of monitoring. On-board storage of data within the apparatus embodying the
15 invention solves this problem, as well as advantageously eliminating any electromagnetic transmissions from the apparatus which may interfere with other apparatus, such as medical apparatus.

In prior art systems, there is a lack of data storage
20 facilities to allow for long-term accumulation of data, for example over periods of more than 24 hours. The memory in the monitor embodying the invention solves this problem.

The use of a chest-worn band for supporting a heart-rate
25 monitor is not suitable for various categories of people, such as the very young, the very old and the obese, and is not comfortable for long-term use. The use of ECG electrodes to support and connect the monitor of the embodiment solves this problem and makes the monitor more
30 comfortable to use.

- 9 -

Prior art heart-beat sensors are typically only used to measure heart-rate itself and not other important cardiac parameters such as inter-beat interval. The on-board processor of the embodiment can be programmed to measure any such parameters, particularly when combined with the use of ECG electrodes as these provide a very clear heart-beat signal.

In a preferred embodiment, when the monitor is supported on a user's chest or torso, the accelerometer should be oriented to detect vertical movements of the user's chest or torso. The inventors have found that this provides the most effective sensing of user movement, or activity.

The inventors have also found that the processing of the heart-beat sensor output to extract heart-rate and other cardiac information may advantageously be modified in response to the output from the accelerometer. Thus, for example, the gain and thresholds for ECG measurement are preferably adjusted based on the current user activity level measured by the accelerometer. During periods of activity, noise artefacts tend to be induced in the ECG signal by variations in skin potentials and using the activity data to improve the signal-to-noise ratio of the ECG signal helps to ensure a clean and uninterrupted data stream.

Although reference has been made to storing movement and heart-rate measurements in a memory housed within the apparatus of a preferred embodiment, other possibilities are envisaged within the scope of the invention. Thus, heart-beat or heart-rate data and movement data may be downloaded or transmitted to a remote display unit or data storage unit during use so that these signals may be monitored by a user, for example during exercise. If a

- 10 -

user is engaged in a repetitive physical exercise such as, for example, running, output from the movement sensor may not only be valuable in combination with heart-rate measurement as described above but may also be used to
5 determine the user's stride rate or the number of strides performed, for example.

An apparatus or method embodying the invention may be used for monitoring human or animal users.

Specific Embodiments and Best Mode of the Invention

10 Specific embodiments of the invention will now be described by way of example, with reference to the accompanying drawings, in which:

Figure 1 shows front, side and rear views of a first embodiment of the invention;

15 Figure 2 is a schematic diagram of the embodiment of Figure 1 coupled to two ECG electrodes for use;

Figure 3 is a schematic diagram of the embodiment of Figure 1 coupled to two rectangular ECG electrodes for use;

20 Figure 4 illustrates an embodiment of the invention comprising a monitor and a lead, in which the lead functions as an RF aerial;

Figure 5 is a block diagram of the circuitry of a monitor embodying the invention;

25 Figure 6 is a more detailed circuit diagram of the circuitry of Figure 5;

- 11 -

Figure 7 is a block diagram of an interface for coupling the monitor of Figure 5 to a PC;

Figure 8 is a flow diagram illustrating the operation of the monitor of Figure 5;

5 Figure 9 is a state diagram providing an overview of the operation of the monitor of Figure 5;

Figure 10 is a flow diagram illustrating the functionality of the monitor of Figure 5.

10 Figure 11 is a transverse section of an ECG electrode incorporating an electrode gel;

Figure 12 illustrates a zero-insertion-force mounting for a monitor embodying the invention; and

Figure 13 is a side view of a monitor embodying the invention mounted on an ECG pad.

15 Figure 1 shows the external appearance of a housing of a monitor 2 according to a first embodiment of the invention, viewed from the front, side and rear. The monitor is substantially disc shaped, having a diameter of about 31 mm and a thickness of about 5.5 mm. The rear of
20 the monitor comprises a recessed clip 4 which is removably attachable to an electrical contact of a conventional ECG electrode.

Figure 2 illustrates the monitor of Figure 1 in use. Two
25 conventional ECG electrodes 6, 8 each comprise a circular adhesive pad which can be stuck to a user's chest. Each also comprises an electrical contact positioned near a lower edge of the pad and extending forwards from the pad.

- 12 -

The clip 4 of the monitor 2 mounts on the electrical contact of one electrode 6. The monitor comprises an electrical lead 10 for coupling to the other ECG electrode 8. The lead carries at one end a plug 12 which is
5 removably insertable into a socket in one side of the monitor housing, and at the other end a clip 14 which is removably connectable to the ECG electrode contact.

For user comfort, the lead 10 should be longer than the distance between the ECG electrodes, to accommodate user
10 movement.

The monitor comprises an accelerometer, as described below, which is primarily sensitive to movement in a particular direction. In the embodiment the accelerometer is mounted within the monitor so as to detect vertical
15 motion of the user's chest, which requires that the monitor is mounted and retained in the correct orientation on the ECG pad. The correct orientation for mounting the monitor is indicated to the user by a marking on the monitor casing. Once fitted to the ECG electrode, the
20 clip 4 holds the monitor in position. The lead connecting the monitor to the second ECG pad also helps to orient the monitor correctly.

Figure 3 illustrates a similar monitor 20 mounted on conventional ECG electrodes 22, 24 of a different type,
25 which are of generally rectangular shape.

Figure 4 illustrates a further embodiment in which the lead 10 coupling the monitor to a second ECG electrode acts as an RF (radio frequency) aerial, allowing the monitor to transmit such data to an RF receiver. In this
30 embodiment the lead terminates at a 1mH inductor 26 to enhance its functionality as a aerial.

- 13 -

Figure 12 illustrates the clip 4, for securing the monitor of Figure 1 to an ECG electrode, in more detail. Similar clips may be used in the embodiments of Figures 2 to 4. This zero-insertion-force clip comprises a slider 70 in which an opening 71 is formed, the opening having an enlarged portion 72 at one end through which a conventional 4mm stud 74 of an ECG electrode may be received. An anvil 76 extends into the opening and must be manually withdrawn from the opening (or the slider moved relative to the anvil) against a spring force to allow the stud to enter the opening. From the enlarged portion 72 the opening tapers inwardly between two straight sides 78 at an acute angle to each other. After entry of the stud into the opening, the anvil (or the slider) is released and the anvil abuts the stud so that the spring force urges the stud between the tapering sides 78 of the opening. The spring force is designed to be high enough and the angle between the tapering sides small enough to provide a firm grip between the clip and the stud, to produce good electrical contact and to resist rotation of the monitor relative to the ECG electrode.

As shown in Figure 12 the slider is a plate approximately 1mm thick. This allows it to grip a lower neck portion 80 of the conventional ECG electrode stud (see Figure 11) and hold the base of the monitor flush with or close to the upper surface of the ECG electrode. This clip may advantageously allow zero insertion force and a much more secure mounting than the spring clips conventionally used to secure leads to ECG electrodes.

The monitors illustrated in Figures 1, 2, 3 and 4 are of diameter 31mm and thickness 5.5mm. However, a monitor embodying the invention should advantageously be less than

- 14 -

70mm, and particularly preferably less than 50mm in lateral dimension.

Preferably, the monitor is less than 35 mm in diameter (or lateral or vertical dimension). The preferred position
5 for both actigraphy measurement and ECG electrode pad positioning is on or near the sternum. In order to fit comfortably between female breasts, the size of the monitor housing should be similar to or smaller than that of many normal ECG electrodes. Advantageously, a diameter
10 of about 30mm, or a lateral dimension of about 30mm, is of this order.

In addition, the monitor should advantageously be less than 15mm in thickness and particularly preferably less than 10mm or less than 6mm in thickness. These dimensions
15 aim to ensure user comfort.

Advantageously, these thickness dimensions mean that the monitor housing is of low profile. A low profile may, advantageously, render the monitor almost invisible when worn under clothing. The low profile may also reduce
20 interactions between the monitor and clothing which would otherwise cause movement or tipping of the monitor, or even rip the monitor from its mounting. Interaction with clothing may cause undesirable movement of a monitor of larger diameter or a monitor having a greater thickness.
25 Devices that hang from an ECG electrode by a wire may also suffer from the same excessive movement problem.

When the monitor is clipped to an electrode pad, there may be a gap between the monitor and the pad. Preferably, this gap is narrow. A large gap may allow the monitor to tip or
30 allow clothing to rip the monitor from the pad. Tipping of the monitor is also undesirable as it may generate

- 15 -

spurious movement data or affect the ability of the accelerometer to detect vertical movement. A narrow gap, or no gap, between monitor and pad may, advantageously, lessen these undesirable effects.

5 Figure 13 is a side view of a monitor 20 mounted on an ECG pad 22 as in Figure 3. The monitor is about 5mm thick and the support, or clip, fastening the monitor to the pad is positioned within the monitor housing so that the base of the monitor housing is flush with, or spaced by less than
10 1mm or 2mm from, the upper surface of the ECG electrode to minimise tipping of the monitor relative to the electrode. The outer rim 26 of the monitor housing is bevelled to reduce further the risk of the monitor catching on clothing.

15 Movements of the monitor, such as twisting or tipping, on the electrode pad may cause ECG noise artifacts. A small size and low profile may help to reduce excessive noise artifacts caused by movement of the monitor. The monitor may then, advantageously, be used during vigorous exercise
20 without generating excessive noise artefacts.

Figure 5 is a block diagram of a monitor circuit embodying the invention. Figure 6 is a more detailed circuit diagram corresponding to the block diagram of Figure 5.

The circuit comprises a microcontroller 30 which receives
25 inputs from a clock (crystal oscillator) 32, an accelerometer 34, two ECG electrodes 6, 8 and a communications and power management module 38. The microcontroller 30 is also coupled to a memory 40 and a battery (re-chargeable coin cell) 42. All of these
30 components are mounted on a printed circuit board (PCB)

- 16 -

which is housed within a monitor casing or housing such as illustrated in Figures 1 to 4.

The accelerometer is a piezoelectric accelerometer, which is mounted on the PCB in a predetermined orientation such that it is most sensitive to motion in a predetermined direction when the PCB is housed in the monitor casing and the monitor is in use. For example, in the chest-mounted embodiments of figures 1 to 4, the accelerometer is oriented to be most sensitive to movement in the vertical plane (i.e. sensitive to physical movement in the up/down direction), during use when the user is upright. In this way, a good approximation of the physical activity of the user may be deduced. In other applications for sensing other movements of a human or animal body it may be desirable to mount the accelerometer in different predetermined orientations within the monitor casing.

The signal from the accelerometer is amplified by an amplifier 44 and filtered by a filter 46 before being input to an analog input of the microcontroller.

The ECG electrodes are usually attached to the mid-left region of the user's chest and the monitor is coupled between them. The monitor may comprise a small light emitting diode (LED) which flashes for several beats to indicate when an ECG signal is initially detected. It may additionally flash whenever a heartbeat is detected, allowing the user to confirm that the monitor is picking up an ECG signal.

Preferably, the LED flash is modulated at high frequency so that a light receiver can easily detect its light. Advantageously, this enables remote electrically-isolated

- 17 -

short-range readout of the heart rate in fitness tests such as treadmill tests.

The signals from the ECG electrodes pass through two monitor contacts 48 and are amplified in two stages by two
5 amplifiers 50, 52 and filtered by a filter 54 before being input to an analog input of the microcontroller.

The ECG signal is processed within the microcontroller to remove noise artefacts. As the monitor is totally self-contained, there are no problems with interference from
10 radio frequency devices or other sources of electromagnetic interference.

The microcontroller uses a 4.0 MHz internal clock for instruction timing but uses an external 32.768 kHz oscillator, shown in Figure 5 as the clock 32, for real-
15 time clock functions.

The communications and power management block 38 is coupled to the monitor contacts 48 and comprises discrete circuitry which allows various signal levels and frequencies at the contacts to be discriminated by the
20 microcontroller. This allows the monitor contacts to be used as monitor inputs or outputs for multiple functions depending on the device to which the contacts are coupled. Thus, if the contacts are coupled to ECG electrodes, ECG signals can be identified and received by the
25 microcontroller. If the contacts are coupled to an interface unit or reader as described below, the same contacts can be used by the microcontroller to download data, re-charge the battery, or other applications as described below.

- 18 -

The battery 42 is a surface-mounted manganese lithium secondary (re-chargeable) coin cell that provides up to 22 days of continuous operation from a full charge. During operation, the monitor may continuously record heart rate and physical activity at one minute intervals. All of the other components are also surface-mounted on the PCB to provide compact size, simplified production and increased reliability.

The circuit is provided with protection from reverse polarity connection, over-voltage and ESD (electro-static discharge). The ultra-low power and integrated nature of the monitor ensures no EMI (electro-magnetic) emissions.

The device is waterproof and can hence be worn continually to provide an uninterrupted data stream.

15 Firmware

In the monitor, certain firmware (embedded software) is programmed into an internal ROM (read only memory) area of the microcontroller 30 and controls many of the monitor's functions. In particular, the firmware enables the sampling of signals from the accelerometer and the ECG electrodes under timed interrupts, with movement being sampled at 16 Hz and ECG at 128 Hz or 256 Hz. These signals are sampled at different rates to reflect the different rates at which the signals typically vary. The movement data are integrated over one minute epochs and stored into non-volatile memory 40. The heart rate data are stored as beats per minute in the non-volatile memory.

The microcontroller performs several signal processing functions and executes internal algorithms on the ECG data. The key processing functions are as follows.

- 19 -

Dynamic threshold: the threshold for detection of the ECG R-wave pulse is dynamically adjusted within a window period to aid discrimination of true pulse signals during periods of high noise.

5 Variable gain: the gain and dV/dt (rate of change of voltage) thresholds for ECG measurement are adjusted based on the current user movement level detected by the accelerometer. During periods of movement, noise artefacts are induced by variations in the user's skin
10 potentials. Using the movement data to improve the signal-to-noise ratio of the ECG signal helps to ensure a clean and uninterrupted data stream.

The monitor uses a digitally computed reference level to determine whether the dV/dt (rate of change of voltage) of
15 the input signal meets the requirements of an ECG R-wave. This threshold varies with time and has an absolute minimum level to prevent spurious noise being seen as an R-wave. During periods of high activity the minimum threshold level is raised, as described above, to prevent
20 spurious triggering on movement noise artifacts.

IBI Tracking: the inter-beat interval (IBI) is computed and used to update an internally stored histogram. The histogram contains discrete time windows and an IBI value falling within a histogram window causes the histogram to
25 be incremented. An indication of variation of the inter-beat interval is very useful in determining certain medical conditions.

IBI variability logging: normal regular heart-rate data are stored as beats per minute. If serious variability is
30 detected, the heart rate is automatically stored at a higher resolution to allow a more detailed analysis.

- 20 -

Figure 9 provides an overview of the firmware operation.

Reader

Figure 7 is a block diagram of a reader, or interface, for coupling the monitor to a PC. The reader comprises
5 terminals 60 connectable to the ECG electrode contacts 48
of the monitor. Within the reader, these are connected to
a bi-directional communications module 62 and a
charge/monitor/re-set module 64. Each of these modules is
connected by an RS232 connector 66, or other connector
10 suitable for interfacing to a PC, such as a USB connector.

The reader is thus a small module that contains the electronics necessary for level shifting to and from RS232 (or USB) in addition to providing control signals for power management of the monitor. Once the monitor is
15 connected to the reader via the ECG leads, after simply unclipping the monitor from the ECG electrodes and connecting the same contacts to the reader, bi-directional communications may take place between the monitor and the serial port of the PC. As well as allowing data to be
20 downloaded from the monitor to the PC, the reader can also charge the monitor battery, drawing power from the PC serial port or optionally from a plug-in mains adaptor.

Software

This software runs on a PC having a serial port to which
25 the monitor may be coupled via the reader described above. The software is a 32-bit Windows application written in Visual Basic with an underlying database used for data management. The software has the following broad functions.

- 21 -

Store details of users and test data in structured and manageable database tables.

Write user and test parameters to the monitor.

Read logged data from the monitor.

5 Present reports in a user-friendly and flexible manner.

Provide portable data storage. This means that data can be exported to other software packages for additional analysis.

Figure 8 shows a block diagram of the software structure.

10 A core database 100, which is Access compatible, contains tables for user information such as name, date of birth, height etc. The database also has tables to contain downloaded heart rate, or other cardiac data, and movement, or activity, data. The tables have relational
15 interlinking and the software generates queries to present users seamlessly with the correct downloaded data.

When a new user is added 102, their personal details are stored into the database. A set of test-specific parameters (i.e. user weight, test start date and time
20 etc.) are also set and stored 106. Alternatively, existing users may be located 108 from the database using search facilities and the test parameters then set or selected. Set-up information is then transferred to the monitor by means of a communications module 104 and a
25 serial link (coupled through the reader to the monitor).

The communications module 104 also controls monitor status management 116, including monitoring the level of charge

- 22 -

in the monitor battery and re-setting the monitor microcontroller where required.

In addition, data may be downloaded through the serial link under the control of the communications module from
5 the monitor to the database 100 and viewed using a graphical reports module 110. Graphical reports may be printed 112 or data may be exported 114 directly from the database or via the clipboard from the graphical reports module.

10 Functionality of the Monitor Contacts

As described above, the monitor comprises two electrical contacts, which can be coupled either to ECG electrodes for heart-beat sensing or to an external device such as the reader for various other purposes.

15 Figure 10 illustrates the various functions of the monitor contacts.

In total, the two contacts for the ECG electrodes are also used for five other functions: reading data, writing data, charging battery, power management and re-setting the CPU
20 of the microcontroller. This shared functionality of connections allows greatly reduced size and complexity of the electronics of the monitor and provides a simplified user interface.

As shown in Figure 10, when the monitor contacts are
25 coupled to ECG electrodes (200), the ECG signals are taken directly from those electrodes. In a preferred embodiment, the monitor mounts directly onto one electrode and connects via a cable to the other.

- 23 -

When the monitor contacts are coupled to a PC via a serial interface (202), data can be written by the PC to the monitor. This allows set-up data to be written to the monitor, including user identification and any other
5 desired test parameters.

Similarly, when the monitor contacts are coupled to the serial interface (204), data can be read from the monitor by the PC. This allows stored movement (activity) and cardiac data to be downloaded.

10 When the monitor contacts are coupled either to a suitable serial interface or to a battery charger (206), the same connections allow the internal re-chargeable battery to be charged.

When the monitor contacts are coupled to a suitable
15 interface, such as the reader described above, battery status can be monitored and managed (208).

Finally, when the monitor contacts are coupled to a suitable interface such as the reader described above, the micro-controller can be re-set (210) following a total
20 discharge or re-charge of the battery.

Claims

1. A monitor for monitoring a user's heart, comprising;

a support means for securing the monitor in position
for sensing the user's heart beat, the support means
5 being for attachment to a single adhesive ECG
electrode both to support the monitor and for
receiving electrical signals from the ECG electrode;

a means for electrically coupling the monitor to a
second ECG electrode for receiving signals therefrom;

10 a cardiac sensor for receiving signals from the ECG
electrodes, and

a processor coupled to the cardiac sensor for
generating cardiac data.
- 15 2. A monitor according to claim 1, in which the coupling
means comprises an electrical lead extending from a
housing of the monitor or a socket in the housing of
the monitor for receiving an electrical lead.
- 20 3. A monitor according to claim 1 or 2, in which the
single adhesive ECG electrode is a standard ECG
electrode.
4. A monitor according to any preceding claim, in which
the maximum lateral dimension of the ECG electrode is
55mm or less.

- 25 -

5. A monitor according to any preceding claim, in which the maximum lateral dimension of the monitor is 35mm or less.
- 5 6. A monitor according to any preceding claim, in which the maximum lateral dimension of the monitor is less than or equal to the maximum lateral dimension of the ECG electrode.
- 10 7. A monitor according to any preceding claim, in which the monitor, in use, does not extend beyond an outer edge of the ECG electrode.
8. A monitor according to any preceding claim, in which the weight of the monitor is less than 50 grams.
- 15 9. A monitor according to any preceding claim, comprising a memory coupled to an output of the processor for storing the cardiac data.
10. A monitor according to any preceding claim, in which the processor generates inter-beat interval data from signals it receives from the cardiac sensor.
- 20 11. A monitor according to any preceding claim, further comprising an accelerometer coupled to the processor, so that the processor can generate movement data.
- 25 12. A monitor according to claim 11, in which the processor processes signals it receives from the cardiac sensor according to a predetermined parameter in order to generate the cardiac data and modifies that parameter in response to signals it receives from the accelerometer.

- 26 -

- 5 13. A monitor according to claim 11 or 12, in which a parameter, such as a gain parameter or a threshold voltage, used in deriving the cardiac data from an output of the cardiac sensor is variable in response to an output from the accelerometer or a movement or activity parameter derived therefrom.
- 10 14. A monitor according to any preceding claim, comprising contacts for making electrical contact with two ECG electrodes, in which the same contacts are couplable to an interface for transferring data from and/or to the monitor, and/or for resetting or reprogramming the monitor, and/or for recharging a battery for powering the monitor.
- 15 15. A monitor according to any of claims 11 to 13, in which the monitor in use is secured to the chest or torso of the user so that the accelerometer is oriented to sense vertical movements of the user's chest or torso.
- 20 16. A monitor according to any preceding claim, which is of small size and weight so as to be comfortable for a user to wear for extended data sampling periods.
- 25 17. A method for monitoring a user's heart, comprising the steps of;
- sensing the user's heart beat by using a cardiac sensor secured to the user's body by means of a single ECG electrode;
- processing cardiac signals to generate cardiac data;
- and

- 27 -

storing or displaying the data.

18. A method according to claim 12, comprising the step
of sensing movement of the cardiac sensor and
processing movement signals to generate movement
5 data.
19. A monitor for monitoring a user's heart beat
substantially as described herein with reference to
the drawings.
20. A monitor for monitoring a user's heart beat and
10 movement substantially as described herein with
reference to the drawings.
21. A method for monitoring a user's heart beat
substantially as described herein with reference to
the drawings.
- 15 22. A method for monitoring a user's heart beat and
movement substantially as described herein with
reference to the drawings.

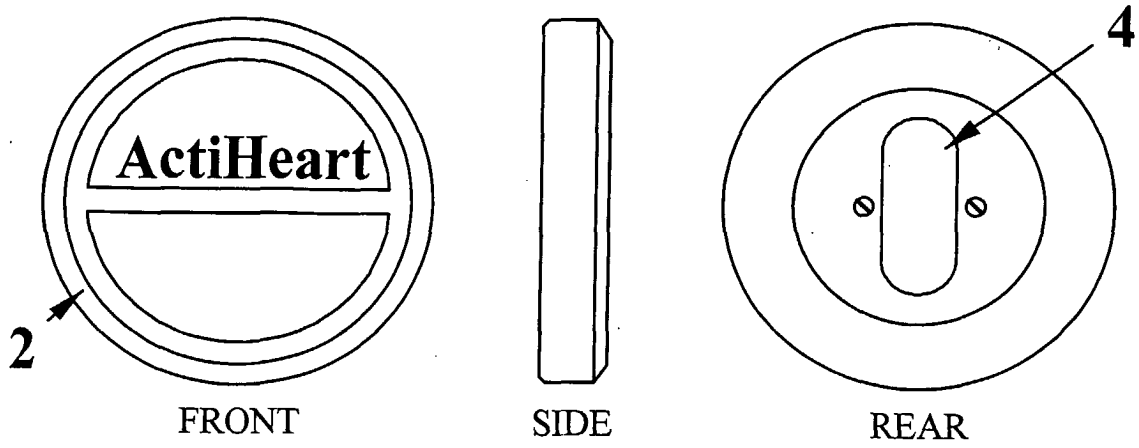


FIGURE 1

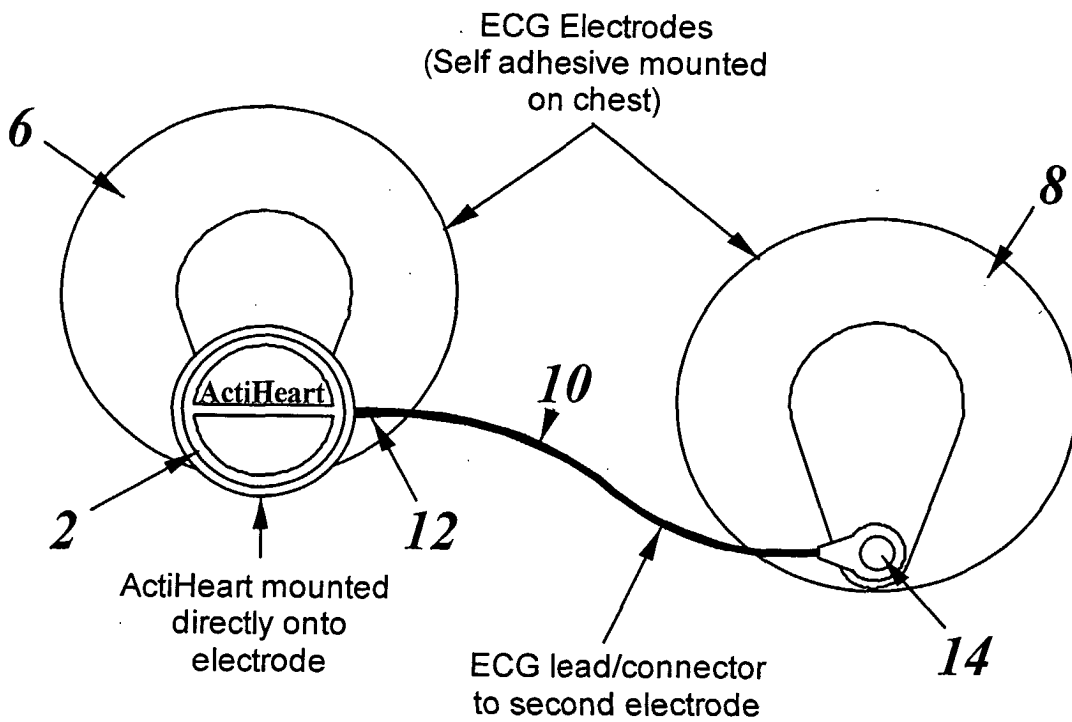


FIGURE 2

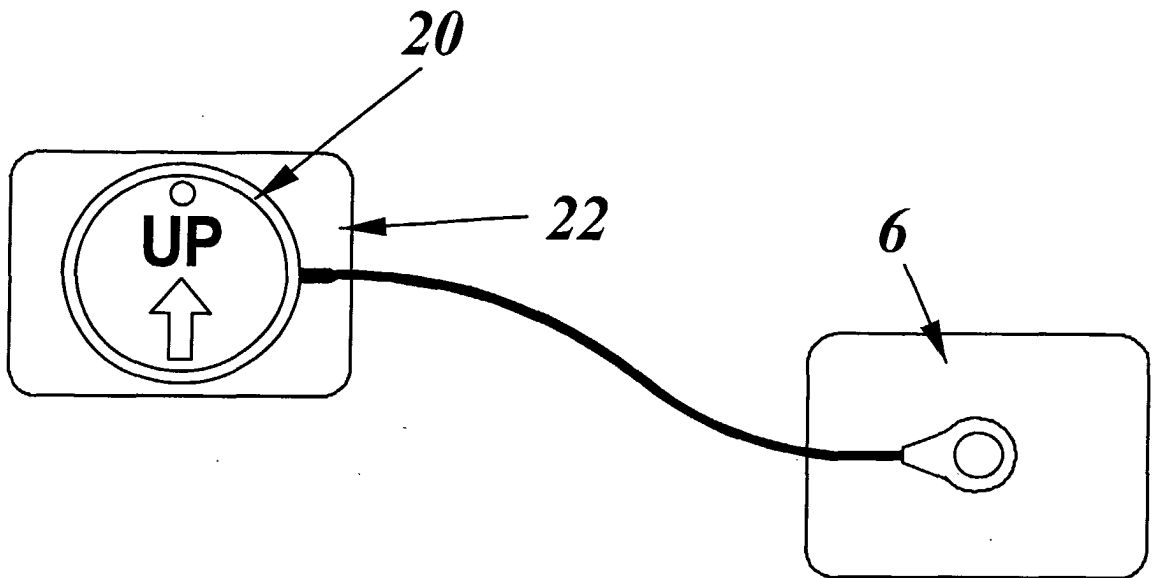


FIGURE 3

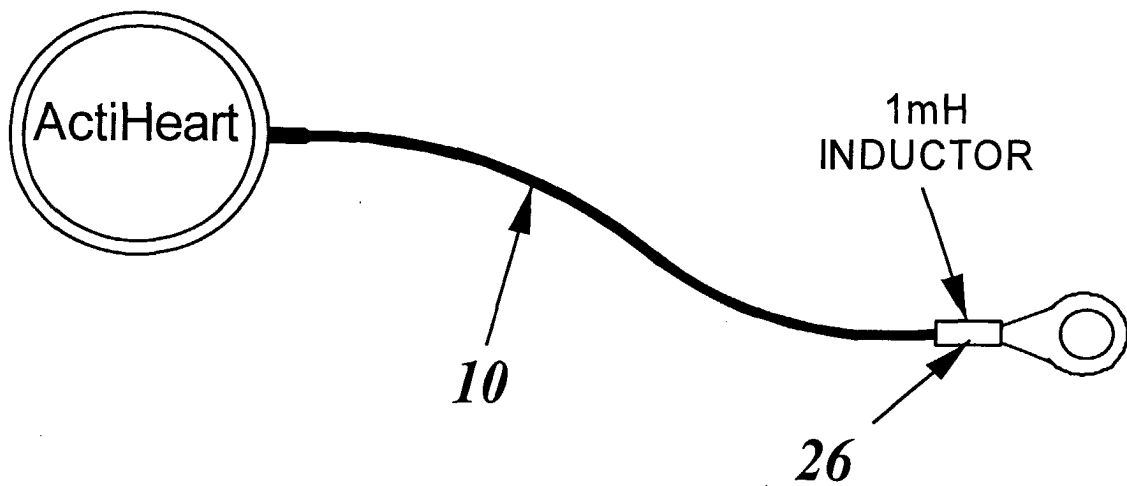


FIGURE 4

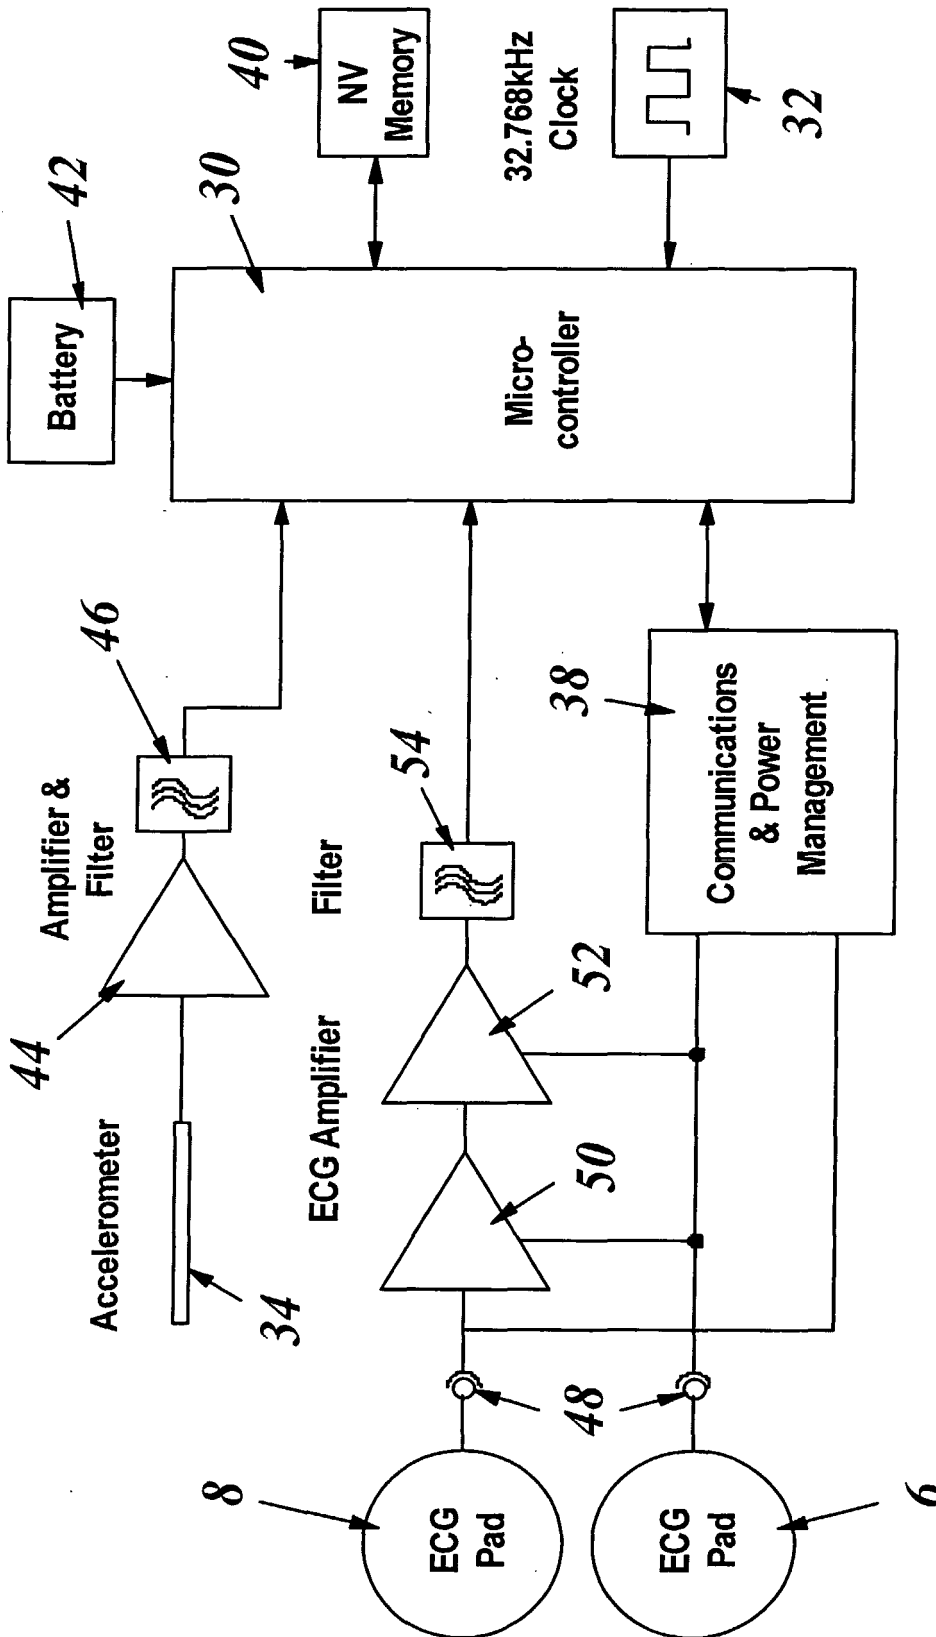


FIGURE 5

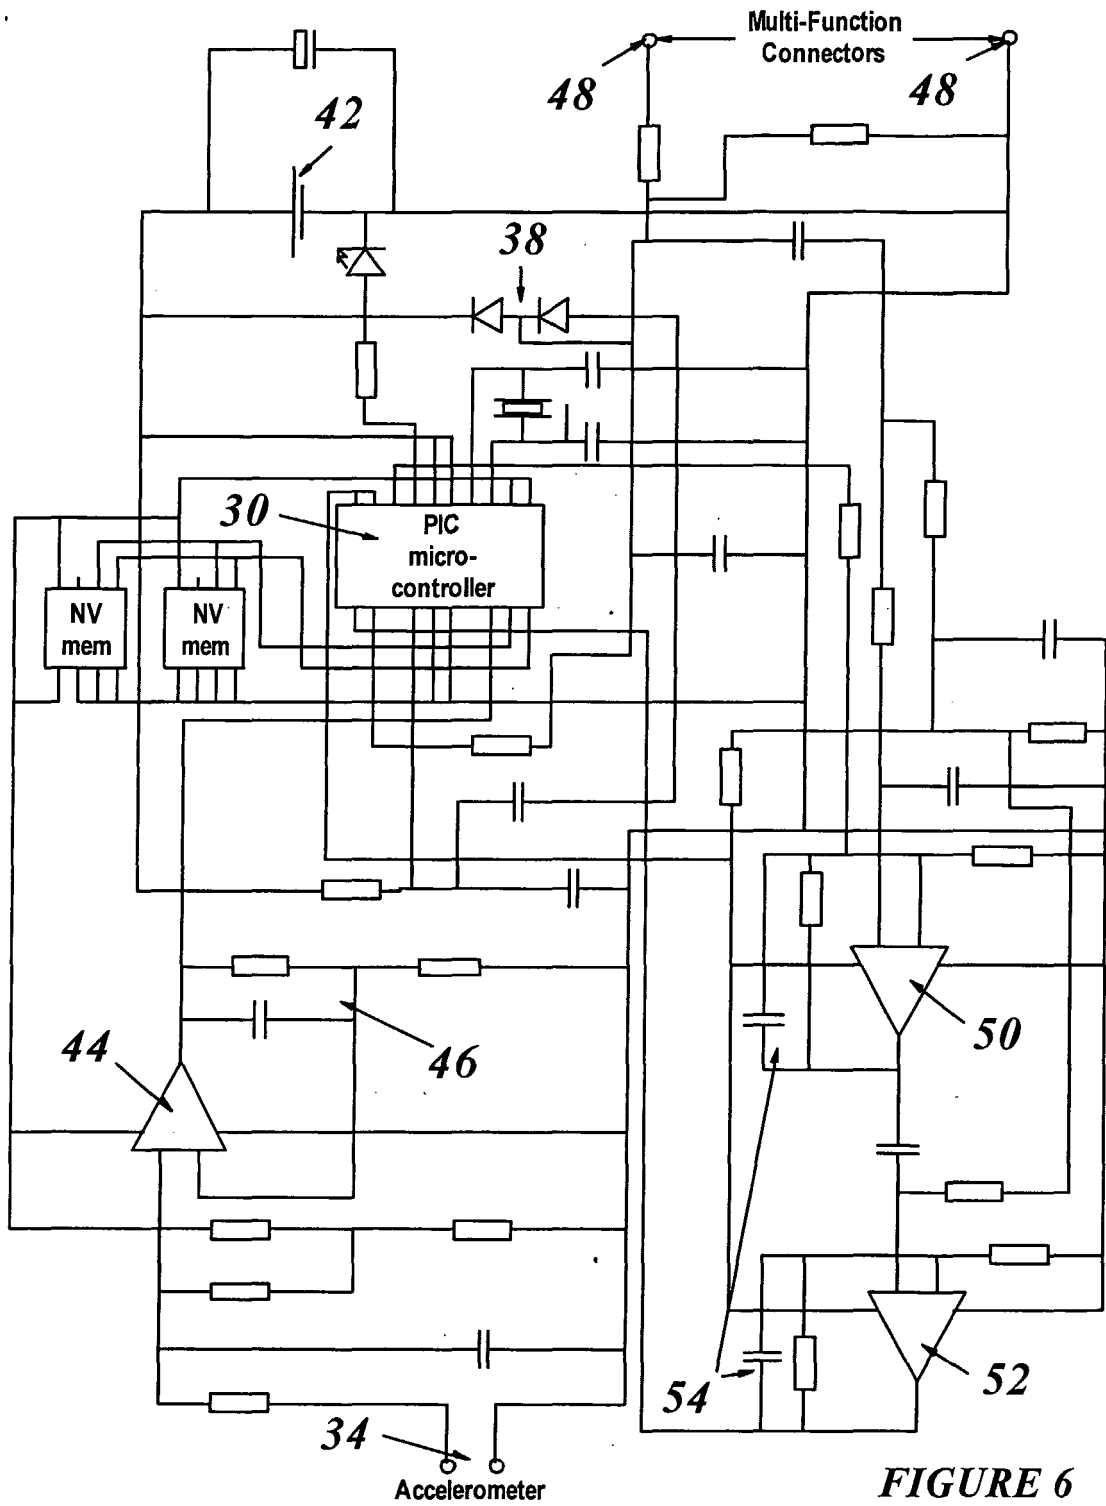


FIGURE 6

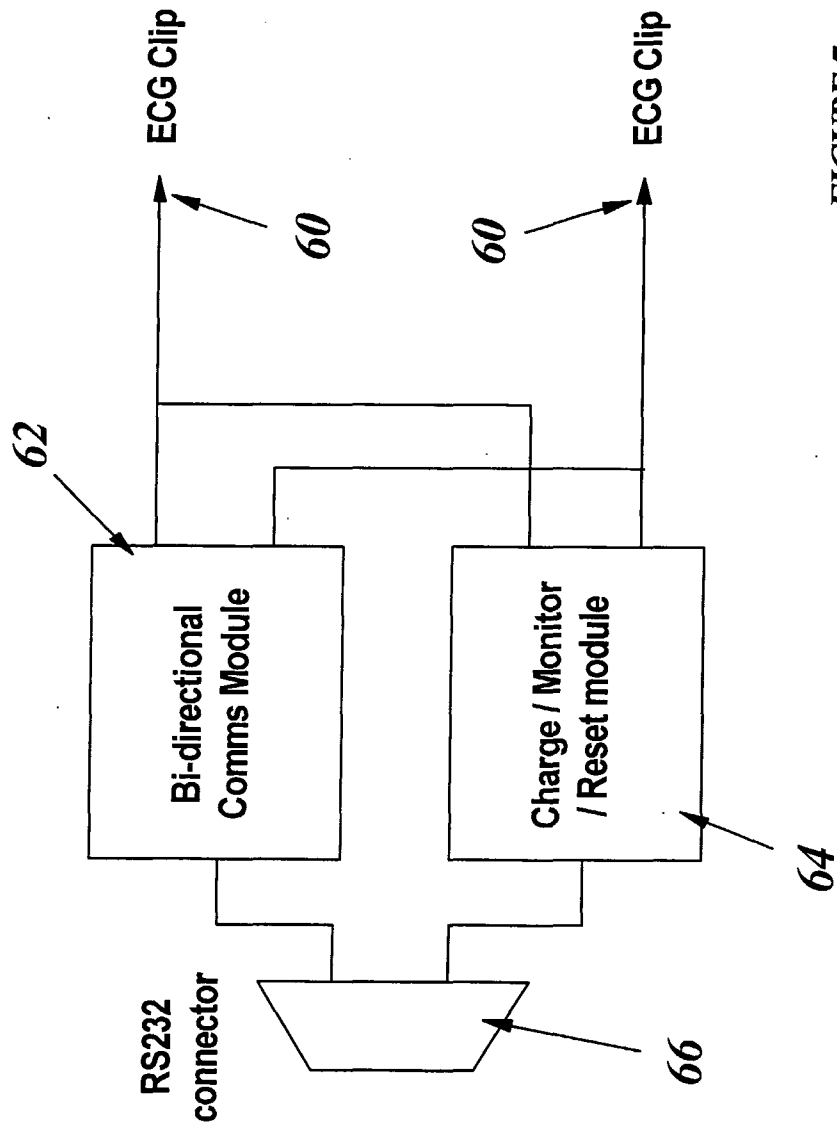


FIGURE 7

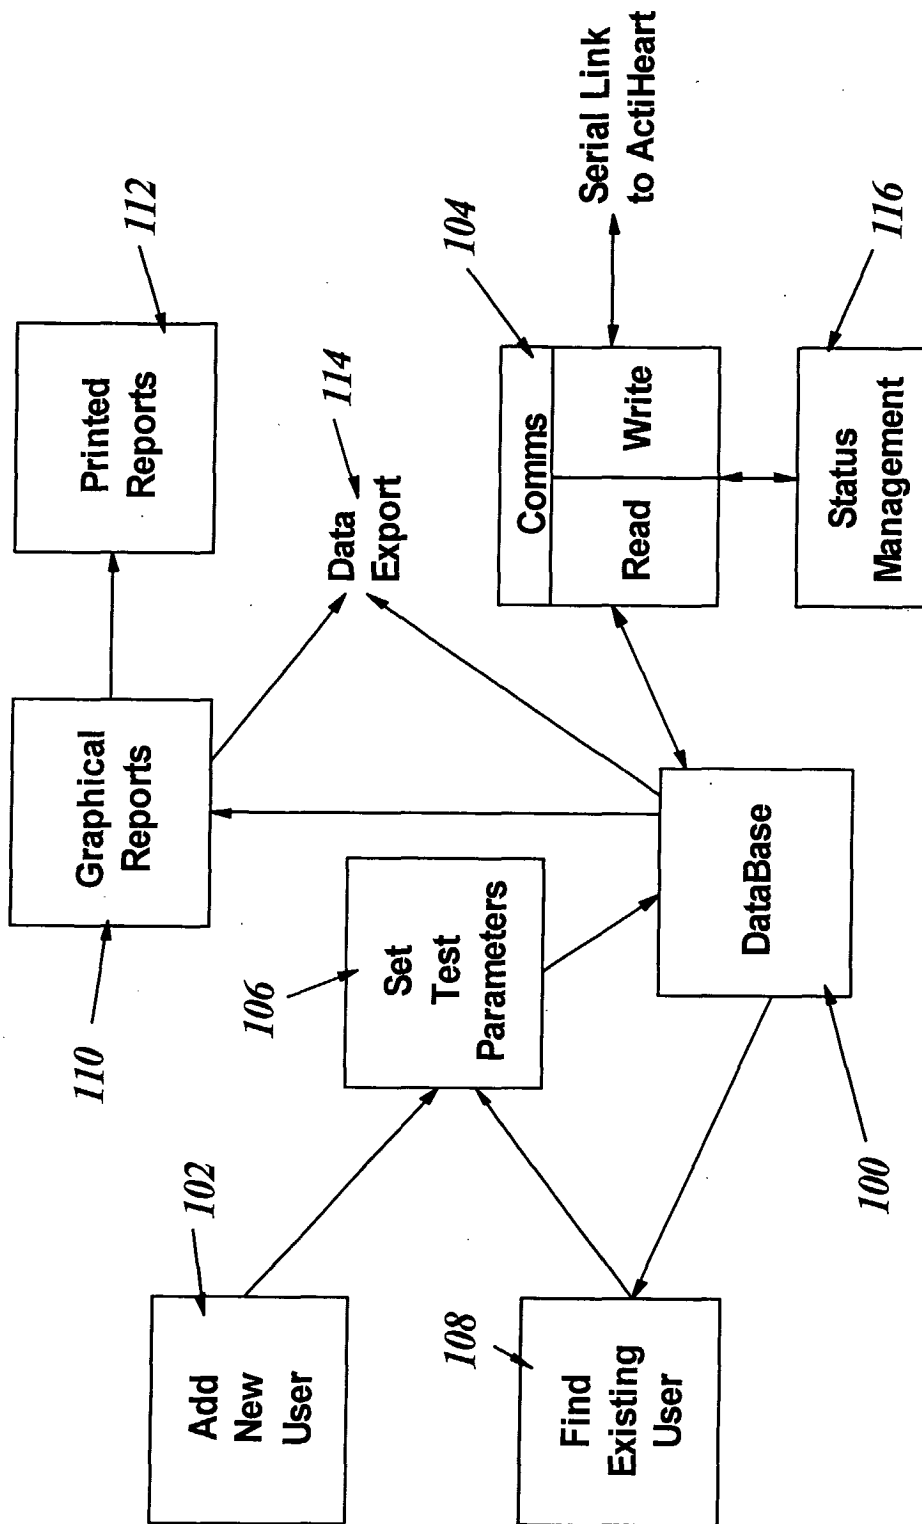


FIGURE 8

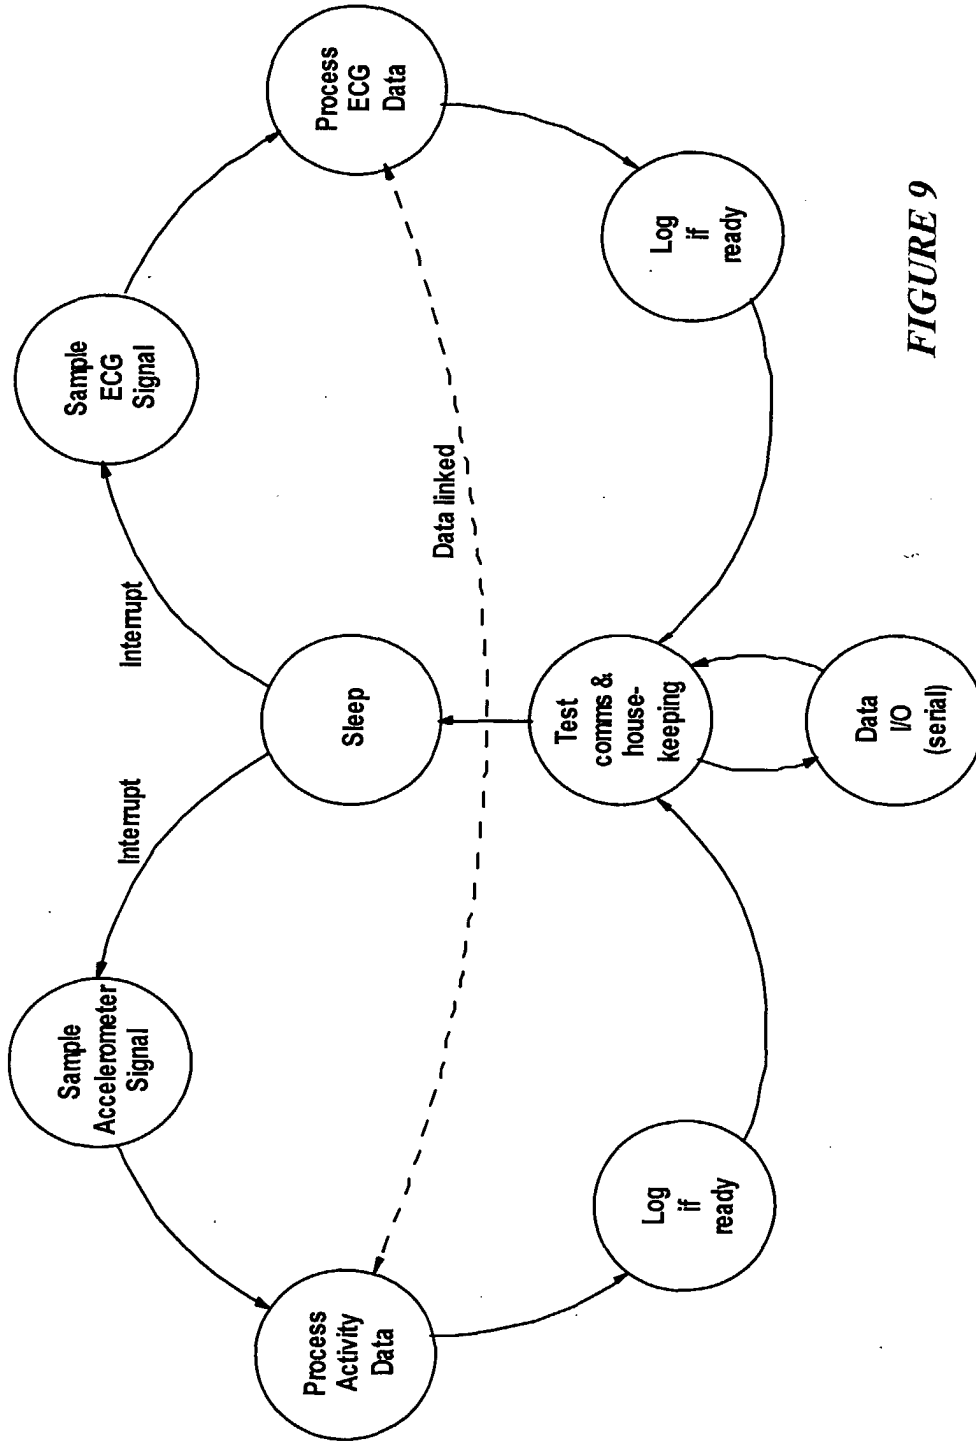


FIGURE 9

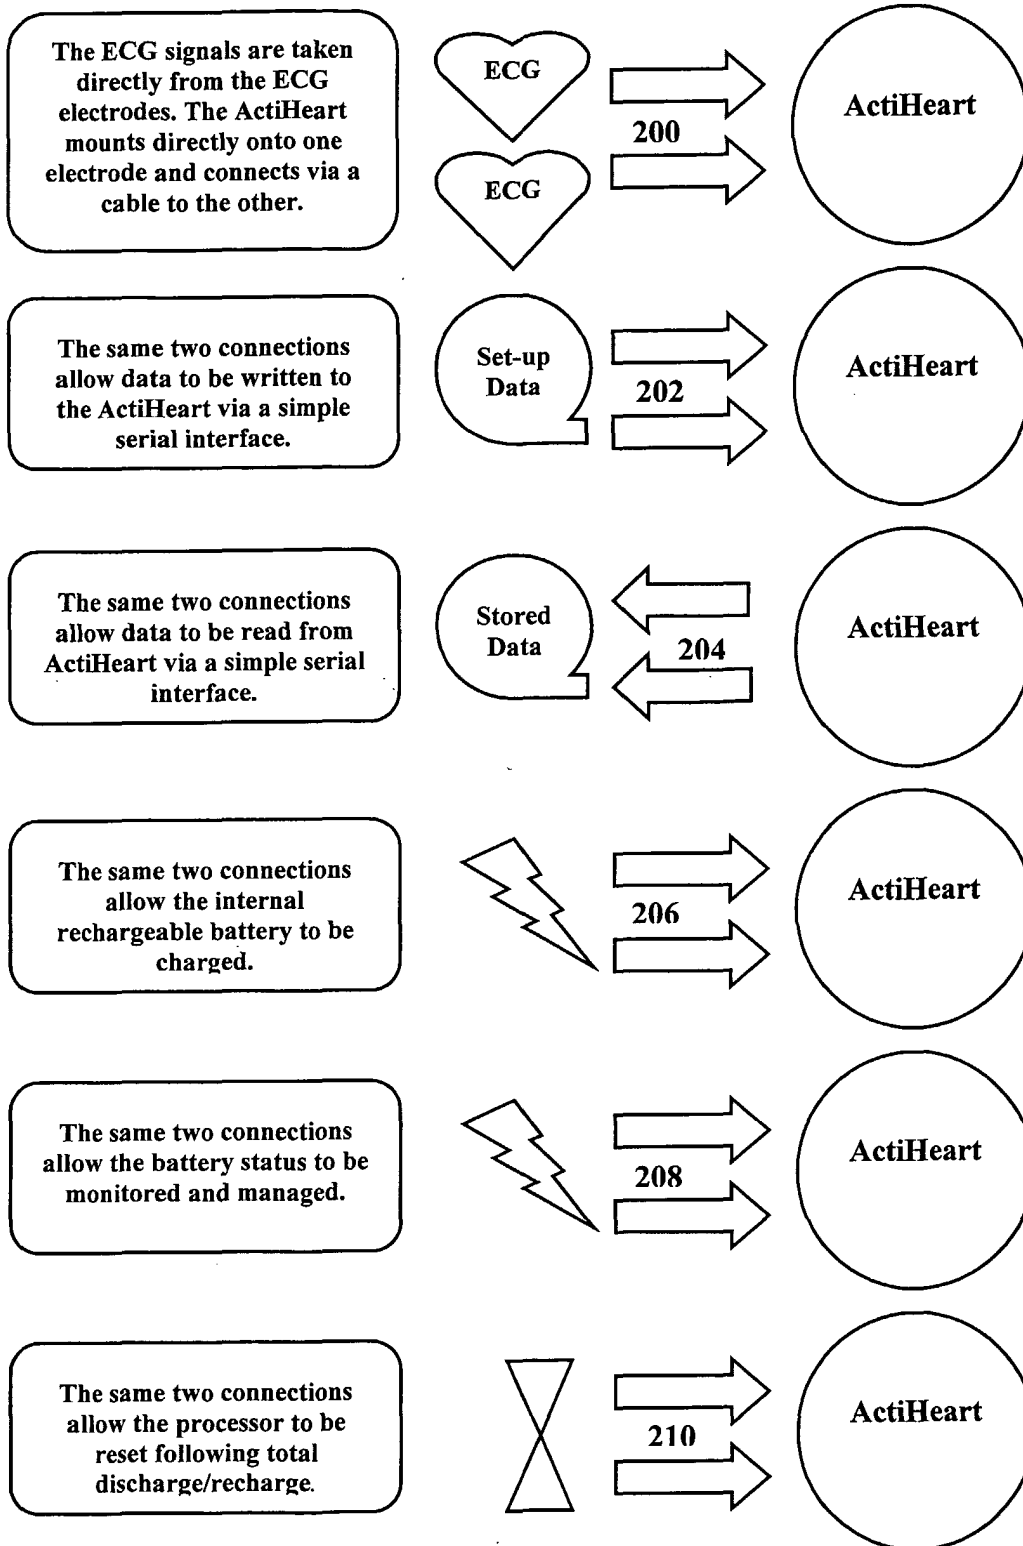


FIGURE 10

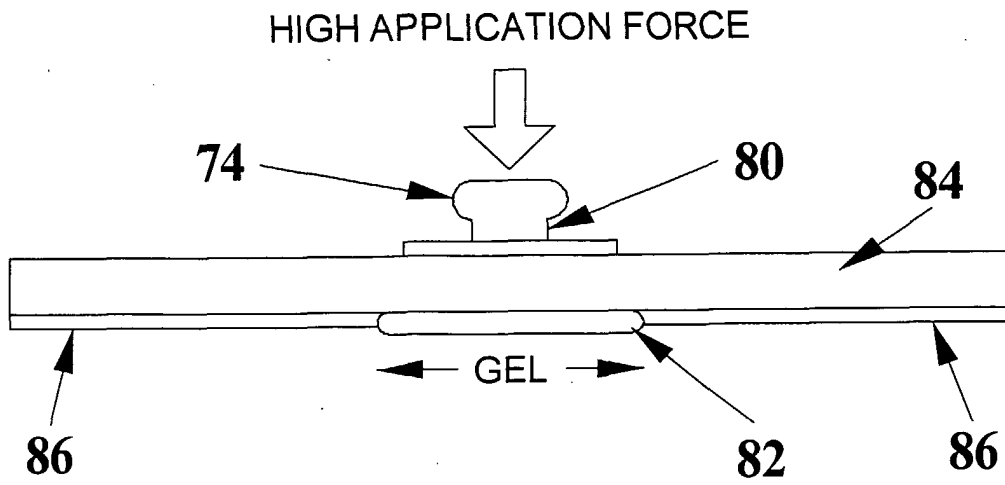


FIGURE 11

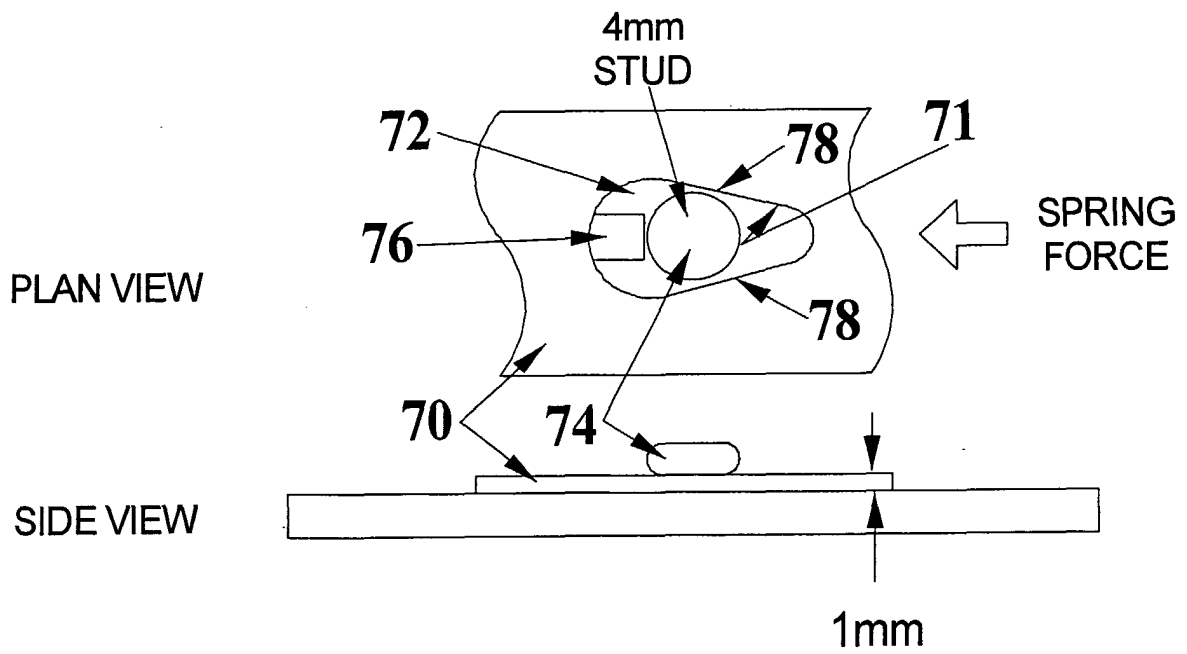


FIGURE 12

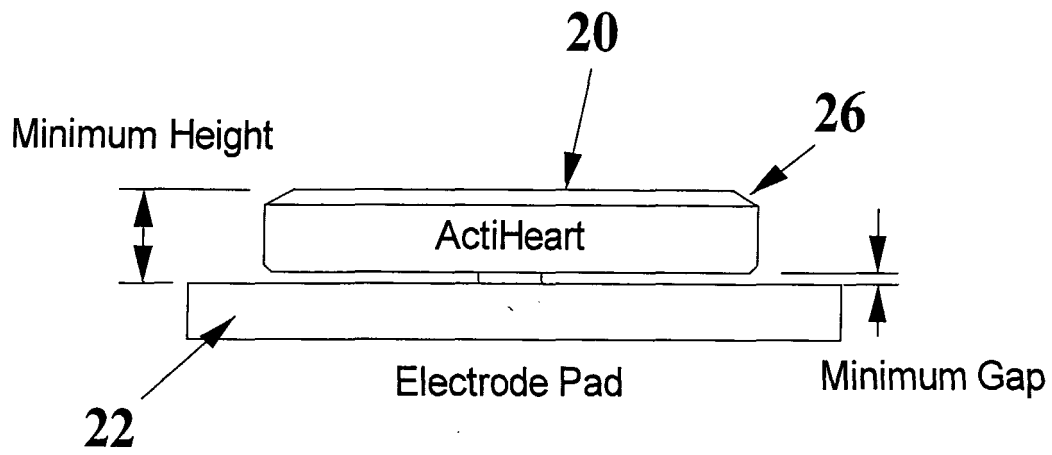


FIGURE 13

INTERNATIONAL SEARCH REPORT

Inter al Application No
PCT/GB 03/04487

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)
EPO-Internal, PAJ, INSPEC

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	GB 2 207 579 A (BACH TOM;COLEMAN PAUL) 1 February 1989 (1989-02-01) page 3, line 1 -page 3, line 12; figures 1-3 ---	1-8, 16
X A	EP 0 925 756 A (NIHON KOHDEN CORP) 30 June 1999 (1999-06-30) paragraph '0025! - paragraph '0034! figure 4 ---	1, 2, 16
X	PATENT ABSTRACTS OF JAPAN vol. 2000, no. 24, 11 May 2001 (2001-05-11) & JP 2001 198096 A (TERUMO CORP), 24 July 2001 (2001-07-24) abstract ---	1-7, 9, 16, 17
Y	-/--	10-15, 18

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *g* document member of the same patent family

Date of the actual completion of the international search

Date of mailing of the international search report

16 February 2004

26/02/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Lommel, A

INTERNATIONAL SEARCH REPORT

 Inte: 1st Application No
 PCT/GB 03/04487

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 6 117 077 A (BACHMAN JOHN A ET AL) 12 September 2000 (2000-09-12) column 6, line 10 -column 9, line 7; figures 5-8 ---	1-4,9-16
X	US 6 441 747 B1 (GHAEM SANJAR ET AL) 27 August 2002 (2002-08-27) column 6, line 6 -column 6, line 12 column 6, line 63 -column 7, line 67 figures 1-3,10 ---	17
Y	EP 0 513 548 A (MATSUSHITA ELECTRIC IND CO LTD) 19 November 1992 (1992-11-19) figure 1 ---	1-4,9-17
Y	EP 0 513 548 A (MATSUSHITA ELECTRIC IND CO LTD) 19 November 1992 (1992-11-19) figure 1 ---	1-3,9-16
A	MAKIKAWA M; IMAI K; SHINDOI T; TANOOKA K; IIZUMI H; MITANI H: "Microprocessor-based memory device for ambulatory heart rate and physical activity recording" METHODS OF INFORMATION IN MEDICINE, ISSN 0026-1270, vol. 33, no. 1, March 1994 (1994-03), pages 94-96, XP008027621 German * whole article * ---	1-18
Y	TONG, DAVID A: "Investigation into Electrocardiogram Motion Artifact Reduction, 10-9191" , 'Online! 1 April 2000 (2000-04-01), XP002270312 IR&D Southwest Research Institute, San Antonio, TX, USA Retrieved from the Internet: <URL:http://www.swri.edu/3pubs/IRD2001/10- 9191.htm> 'retrieved on 2004-02-12! * whole article * ---	1,11-13, 17,18
L	RAYA M A D ; SISON L G : " Adaptive noise cancelling of motion artifact in stress ECG signals using accelerometer " CONFERENCE PROCEEDINGS. 24TH ANNUAL INTERNATIONAL CONFERENCE OF THE ENGINEERING IN MEDICINE AND BIOLOGY SOCIETY. ANNUAL FALL MEETING OF THE BIOMEDICAL ENGINEERING SOCIETY, HOUSTON, TX, USA, 23-26 OCT. 2002, ISBN 0-7803-7612-9, vol. 2, 2002, pages 1756-1757, XP002270313 Piscataway, NJ, USA, IEEE, USA ---	
X	JP 62 202804 U (MATSUSHITA ELECTRIC WORKS LTD) 1987 * whole document * -----	1,2,7,16

INTERNATIONAL SEARCH REPORT

International application No.
PCT/GB 03/04487

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.: 19-22
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
see FURTHER INFORMATION sheet PCT/ISA/210

3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.

2. As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.

3. As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest.
- No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

Continuation of Box I.2

Claims Nos.: 19-22

The subject-matter of claims 19-22 is defined by reference to the description and drawings which is not allowed by the PCT (Rule 6.2 PCT). The claims do not define any clear structural features or limitations. Consequently, the scope of the claim is not clear (see Article 6 PCT) and a meaningful search is not possible (Article 17 PCT).

The applicant's attention is drawn to the fact that claims, or parts of claims, relating to inventions in respect of which no international search report has been established need not be the subject of an international preliminary examination (Rule 66.1(e) PCT). The applicant is advised that the EPO policy when acting as an International Preliminary Examining Authority is normally not to carry out a preliminary examination on matter which has not been searched. This is the case irrespective of whether or not the claims are amended following receipt of the search report or during any Chapter II procedure.

INTERNATIONAL SEARCH REPORT

 International Application No
 PCT/GB 03/04487

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
GB 2207579	A	01-02-1989	NONE	
EP 0925756	A	30-06-1999	EP 0925756 A2	30-06-1999
			JP 11262476 A	28-09-1999
			US 2002103441 A1	01-08-2002
			US 2002107453 A1	08-08-2002
			US 6161036 A	12-12-2000
			US 6389309 B1	14-05-2002
JP 2001198096	A	24-07-2001	NONE	
US 6117077	A	12-09-2000	WO 0042904 A1	27-07-2000
US 6441747	B1	27-08-2002	AU 5708301 A	30-10-2001
			CA 2405861 A1	25-10-2001
			EP 1290658 A2	12-03-2003
			WO 0178831 A2	25-10-2001
			US 2002109621 A1	15-08-2002
EP 0513548	A	19-11-1992	JP 4318352 A	09-11-1992
			JP 2701576 B2	21-01-1998
			JP 4318364 A	09-11-1992
			JP 2778280 B2	23-07-1998
			JP 4318355 A	09-11-1992
			JP 4318353 A	09-11-1992
			JP 4316725 A	09-11-1992
			DE 69227145 D1	05-11-1998
			DE 69227145 T2	18-03-1999
			DE 69231231 D1	10-08-2000
			DE 69231231 T2	22-02-2001
			EP 0513548 A2	19-11-1992
			EP 0859360 A1	19-08-1998
			US 5490019 A	06-02-1996
			US 5636080 A	03-06-1997
JP 62202804	U		NONE	

专利名称(译)	心脏监测设备和方法		
公开(公告)号	EP1553869A1	公开(公告)日	2005-07-20
申请号	EP2003753807	申请日	2003-10-16
[标]申请(专利权)人(译)	CAMBRIDGE NEUROTECH		
申请(专利权)人(译)	剑桥神网科技有限公司		
当前申请(专利权)人(译)	CAMNTECH有限公司		
[标]发明人	UNGLESS GARY STEVEN OAKLEY NIGEL ROBERT		
发明人	UNGLESS, GARY STEVEN OAKLEY, NIGEL, ROBERT		
IPC分类号	A61B5/11 A61B5/00 A61B5/0432		
CPC分类号	A61B5/0006 A61B5/04325 A61B5/11 A61B5/1118 A61B5/6823 A61B5/721 A61B2560/0412 A61B2562/0219		
优先权	2002024299 2002-10-18 GB		
其他公开文献	EP1553869B1		
外部链接	Espacenet		

摘要(译)

监视器包括响应于用户心跳的心脏传感器 (36)。监视器包括耦合到传感器的处理器，用于产生心率或其他心脏数据。这些数据可以存储在存储器中。监视器由单个ECG电极物理支持并接收来自单个ECG电极的信号，并且通过电引线耦合到第二ECG电极。