



(11) **EP 1 631 350 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
08.08.2012 Bulletin 2012/32

(21) Application number: **04753836.8**

(22) Date of filing: **02.06.2004**

(51) Int Cl.:
A61N 1/365 (2006.01)

(86) International application number:
PCT/US2004/017094

(87) International publication number:
WO 2004/108212 (16.12.2004 Gazette 2004/51)

(54) **DEVICE FOR PERFORMING CARDIAC WAVEFORM APPRAISAL**

VORRICHTUNG ZUR KARDIALEN WELLENFORMBEWERTUNG

DISPOSITIF D'EVALUATION DE FORMES D'ONDES CARDIAQUES

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR

(30) Priority: **02.06.2003 US 475279 P**
01.06.2004 US 858598

(43) Date of publication of application:
08.03.2006 Bulletin 2006/10

(73) Proprietor: **Cameron Health, Inc.**
San Clemente, CA 92673 (US)

(72) Inventors:
• **PALREDDY, Surekha**
Mission Viejo, CA 92692 (US)

• **WARREN, Jay, A.**
San Juan Capistrano, CA 92675 (US)
• **PHILLIPS, James, William**
Fountain Valley, CA 92708 (US)

(74) Representative: **Vossius & Partner**
Siebertstrasse 4
81675 München (DE)

(56) References cited:
WO-A-91/19452 GB-A- 2 034 046
US-A- 4 979 110 US-B1- 6 192 273
US-B1- 6 240 313 US-B1- 6 532 389

EP 1 631 350 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionField

5 [0001] The present invention is related to the field of implantable cardiac treatment devices.

Background

10 [0002] Implantable cardiac rhythm management devices are an effective treatment in managing irregular cardiac rhythms in particular patients. Implantable cardiac rhythm management devices are capable of recognizing and treating arrhythmias with a variety of therapies. These therapies range from providing anti-bradycardia pacing for treating bradycardia, anti-tachycardia pacing or cardioversion energy for treating ventricular tachycardia, to high energy shock for treating ventricular fibrillation. Frequently, the cardiac rhythm management device delivers these therapies for the treatment of tachyarrhythmias in sequence; starting with anti-tachycardia pacing and then proceeding to low energy shocks, and then, finally, to high energy shocks. Sometimes, however, only one of these therapies is selected depending upon the tachyarrhythmia detected.

15 [0003] To effectively deliver these treatments, cardiac rhythm management devices must first accurately detect and classify an episode. Through accurate determination and quantification of sensed cardiac events, these cardiac rhythm management devices are able to classify the type of arrhythmia that is occurring and assess the appropriate therapy to provide to the heart, if any. A problem arises, however, when the cardiac rhythm management device senses noise, and mistakenly declares an episode. As a result, in particular instances, the cardiac rhythm management device may inappropriately deliver therapy.

20 [0004] Extra-cardiac noise may cause a cardiac rhythm management device to misclassify noise events as a tachyarrhythmia. In illustration, by incorporating skeletal muscle noise artifact, or other noise, into a cardiac rate calculation, the cardiac rhythm management device might inaccurately calculate the ventricular rate as one that is elevated. If the ventricular rate is mistakenly calculated to be elevated over a threshold rate boundary, a frequent determiner of tachyarrhythmias, the cardiac rhythm management device may inappropriately deliver therapy to a patient.

25 [0005] Additionally, problems arise when the cardiac therapy device withholds therapy after mischaracterizing a sensed event. For example, anti-bradycardia devices deliver a pacing pulse based on whether a cardiac event is sensed within a particular time frame. If the sensing architecture fails to sense a cardiac event within a preset time period, the cardiac rhythm management device will deliver a pacing pulse to the heart. This pacing pulse is timed in a preset sequence to induce the patient's heart to contract in a proper rhythm. This therapy, however, may be compromised by having the cardiac rhythm management device sense and characterize an extraneous event as a "true" cardiac event. If the sensing architecture erroneously classifies noise (such as skeletal muscle artifact or other noise) as a "true" cardiac event, then a pacing pulse may be incorrectly withheld. This is particularly problematic when a pacing pulse is required to maintain a physiologically necessary rate of the patient's heart.

30 [0006] Besides being noticeable and sometimes physically painful to the patient, when a cardiac rhythm management device delivers inappropriate treatment, it can be extremely disconcerting to the patient. Moreover, delivery of an inappropriate therapy can intensify the malignancy of the cardiac arrhythmia. Therefore, the accuracy of a sensing architecture is an important factor in ensuring that appropriate therapy is delivered to a patient.

35 [0007] Current implantable cardiac rhythm management devices incorporate a sensing architecture that detects likely cardiac events and renders a decision regardless of the accuracy of those originally detected events. As such, current implantable cardiac rhythm management devices must include painstakingly designed sensing architectures to try and avoid erroneous detections. Prior art devices have been developed with rudimentary systems and methods in an attempt to determine whether noise is present on a sampled cardiac signal. If noise is detected in these devices, the manner in which the cardiac signal is acquired, or the manner in which the device operates in response to the acquired signal, is altered. This reduces the impact of erroneously detecting noise and, therefore, inappropriately triggering or withholding therapy. This methodology, however, leaves the cardiac rhythm management device open to significant sensing drawbacks, one of which is that it continually perturbs the sensing architecture.

40 [0008] Certain prior art implantable cardiac rhythm management devices continuously adjust parameters such as amplifier gain in response to extra-cardiac noise, which allows for the possibility that the sensing architecture may miss cardiac events. When adjusting the gain control to lessen sensitivity by raising the sensing floor to avoid noise, it is possible to miss actual cardiac events especially during polymorphic rhythms including ventricular fibrillation. In particular, the sensing architecture may miss discrete cardiac beats, or otherwise stated, miss true positives. By missing a cardiac event, rhythm and beat sensitivity is diminished.

45 [0009] Other implantable cardiac rhythm management devices in the prior art repeatedly extend a noise window during continuous noise. When these window extensions either reach a specific number, or more commonly reach the end of a predetermined interval, the device reverts to a non-sensing or asynchronous behavior for a limited period of time. This

type of reversion behavior can miss a cardiac event, therefore reducing rhythm and beat sensitivity. Additionally, these reversion approaches to noise are generally only useful for continuous noise. Noise is most frequently burst in nature, for which most reversion schemes are not effective. This often results in overdetection and a potential for inappropriate therapy. Prior art cardiac rhythm management devices frequently utilize these methodologies contiguously.

5 **[0010]** GB 2034046 discloses a wearable cardiac arrhythmia detector which uses the duration between zero crossings of the first derivative of the cardiac signal as a measurement of the width of the QRS complex. EP 0554208A2 discloses implantable cardiac systems which can monitor for noise in the cardiac signal by identifying zero crossings in captured data during the ST segment.

10 Summary

[0011] The present invention, in an illustrative embodiment, is directed toward a sensing architecture for use in cardiac rhythm management devices. The sensing architecture of the present invention provides a method and means for certifying detected events by the cardiac rhythm management device. Moreover, by exploiting the enhanced capability for accurately identifying and using information from only those sensed events that are certified, the sensing architecture of the present invention can better discriminate between rhythms appropriate for device therapy and those that are not.

15 **[0012]** In an illustrative method embodiment which is not part of the invention, the present invention includes a method of signal detection enhancement for a cardiac rhythm device comprising receiving a signal from electrodes implanted for cardiac observation, observing characteristic features of the signal, counting the characteristic features, and comparing the number of characteristic features to a threshold either to certify the signal for use in characterizing a cardiac complex, or to determine the signal is unsuitable for use in characterizing a cardiac complex. In some embodiments, the characteristic features may include a number of significant maximum slope points in the sensed signal. In some embodiments, the characteristic features may include a number of monotonic segments in the sensed signal, or may include a number of sample groups within the sensed signal that are monotonic.

25 Brief Description

[0013]

30 Figures 1A-1B illustrate, respectively, representative subcutaneous and intravenous ICD systems;
 Figure 2 illustrates a block diagram of a sensing architecture in accordance with an illustrative embodiment of the present invention;
 Figure 3 shows an electrocardiogram having a plurality of certified cardiac complexes used in classification and a plurality of cardiac complexes being marked suspect by the sensing architecture and not used in classification;
 35 Figure 4 shows an electrocardiogram sample having no waveform appraisal phase implemented by the sensing architecture;
 Figure 5 shows the same electrocardiogram sample as that depicted in Figure 3, but with the waveform appraisal phase implemented;
 Figure 6 shows a block diagram illustrating the steps employed in some embodiments of the present invention for waveform appraisal;
 40 Figure 7 shows a block diagram illustrating the steps employed in another embodiment of the present invention for waveform appraisal;
 Figure 8 shows a block diagram illustrating the steps employed in another embodiment of the present invention for waveform appraisal;
 45 Figures 9A-9B illustrate, graphically, operation of the waveform appraisal methods of Figures 7 and 8 on a clean QRS signal;
 Figures 10A-10B illustrate, graphically, operation of the waveform appraisal methods of Figures 7 and 8 on a noisy signal that is not suitable for beat classification;
 Figure 11 illustrates, graphically, operation of another waveform appraisal method further illustrated in Figure 12; and
 50 Figure 12 shows a block diagram illustrating the steps employed in a maximum slope point method of waveform appraisal.

Detailed Description

55 **[0014]** The invention is as described in the appended set of claims.

[0015] The following detailed description should be read with reference to the drawings, in which like elements in different drawings are numbered identically. The drawings, which are not necessarily to scale, depict selected embodiments and are not intended to limit the scope of the invention. Those skilled in the art will recognize that many of the

examples provided have suitable alternatives that may be utilized.

5 [0016] The present invention is generally related to cardiac rhythm management devices (e.g., an Implantable Cardioverter/Defibrillator (ICD) system) that provide therapy for patients experiencing particular arrhythmias. The present invention is directed toward sensing architectures for use in cardiac rhythm management devices. In particular, the present invention is suited for ICD systems capable of detecting and defibrillating harmful arrhythmias. Although the sensing architecture is intended primarily for use in an implantable medical device that provides defibrillation therapy, the invention is also applicable to cardiac rhythm management devices directed toward anti-tachyarrhythmia pacing (ATP) therapy, pacing, and other cardiac rhythm devices capable of performing a combination of therapies to treat rhythm disorders, including external devices.

10 [0017] To date, ICD systems have been epicardial systems or transvenous systems implanted generally as shown in Figure 1B, however, as further explained herein, the present invention is also adapted to function with a subcutaneous ICD system as shown in Figure 1A.

15 [0018] Figure 1A illustrates a subcutaneously placed ICD system. In this illustrative embodiment, the heart 1 is monitored using a canister 2 coupled to a lead system 3. The canister 2 may include an electrode 4 thereon, while the lead system 3 connects to sensing electrodes 5, 6, and a coil electrode 7 that may serve as a shock or stimulus delivery electrode as well as a sensing electrode. The various electrodes define a number of sensing vectors V1, V2, V3, V4. It can be seen that each vector provides a different vector "view" of the heart's electrical activity. The system may be implanted subcutaneously as illustrated, for example, in U.S. Patent Nos. 6,647,292 and 6,721,597. By subcutaneous placement, it is meant that electrode placement does not require insertion of an electrode into a heart chamber, the heart muscle, or the patient's vasculature.

20 [0019] Figure 1B illustrates a transvenous ICD system. The heart 10 is monitored and treated by a system including a canister 11 coupled to a lead system 12 including atrial electrodes 13 and ventricular electrodes 14. A number of configurations for the electrodes may be used, including placement within the heart, adherence to the heart, or disposition within the patient's vasculature. For example, Olson et al., in U.S. Patent No. 6,731,978, illustrate electrodes disposed in each chamber of the heart for sensing, as well as shocking electrodes in addition to the sensing electrodes.

25 [0020] The present invention, in some embodiments, is also embodied by operational circuitry including select electrical components provided within the canister 2 (Figure 1A) or canister 11 (Figure 1B). In such embodiments, the operational circuitry may be configured to enable the methods to be performed. In some similar embodiments, the present invention may be embodied in readable instruction sets such as a program encoded in machine or controller readable media, wherein the readable instruction sets are provided to enable the operational circuitry to perform the analysis discussed in the above embodiments. Further embodiments may include a controller or microcontroller adapted to read and execute the above methods.

30 [0021] Figure 2 illustrates a sensing architecture embodiment 20 of the present invention. The sensing architecture 20 is separated into three distinct and autonomous phases. The three phases are (1) the detection phase 21, (2) the waveform appraisal phase 22 and (3) the classification phase 23. Decisions are made in each of the three phases. Moreover, decisions made in each phase may affect the decision-making process in subsequent phases. However, it is not necessarily the case that decisions made in an individual phase will affect the decision-making process in preceding phases. In illustration, a decision made in the waveform appraisal phase 22 may affect the decision-making process in the classification phase 23, but it may have no effect on the detection phase 21, or in any future decisions made in the detection phase 21.

35 [0022] The first phase of the sensing architecture 20 is the detection phase 21. Within the detection phase 21 of the sensing architecture 20, data is collected by a cardiac rhythm management device. The manner in which the data is collected and the type of data collected is dependent on the cardiac rhythm management device being used. Moreover, the cardiac rhythm management device can be programmed to, or may automatically adapt to, optimally detect a particular form of data which is sought by the cardiac rhythm management device. In a subcutaneous ICD system, subcutaneous electrodes are used to detect cardiac signals emitted from the patient's heart.

40 [0023] Once the raw detected signal data is received by the cardiac rhythm management device, the detected data is then preprocessed, if required or desired. Preprocessing steps may include smoothing of the detected data, differentiation, filtering and other preprocessing methodologies known in the art. Finally, the detected data, whether preprocessed or raw, is initially classified as being either an event or not an event - indicated in the block diagram at 24. More specifically, a determination is made that an event was detected by the sensing architecture 20. An illustrative determination that an event was detected may include, for example, a determination that a signal has been received having at least a certain amplitude likely indicating an R-wave from a cardiac complex or noise. The result is that the detection phase 21 provides a sensed event to the waveform appraisal phase 22.

45 [0024] Following the detection phase 21 of the sensing architecture 20, sensed events are appraised in the second phase, the waveform appraisal phase 22. In the illustrative embodiment, the waveform appraisal phase 22 is a separate and independent phase in the sensing architecture 20. It is within the waveform appraisal phase 22 where an analysis is performed on the sensed event 24 recognized in the detection phase 21 of the sensing architecture 20. In the waveform

appraisal phase 22, an operation is performed on the sensed event. More specifically, the appraisal operator 25 evaluates and certifies that what is sensed during the detection phase 21 is a high quality sensed event. A high quality sensed event is a sensed event that can be used in classifying a cardiac rhythm, such as a sensed event that closely represents a cardiac "beat" without excessive noise. In contrast, a low quality event may be a noise signal that does not represent the desired cardiac signal, or may represent a sensed cardiac beat but the beat is superimposed with a noise artifact sufficient to render the sensed event unsuitable for classification.

[0025] In particular embodiments of the present invention, the sensed event being certified in the waveform appraisal phase 22 is the detection of a cardiac ventricular depolarization. In the art, a cardiac ventricular depolarization is often referred to as a QRS complex or R-wave. In this embodiment, the waveform appraisal phase 22 evaluates and certifies that the sensed event is a high quality R-wave that can be used for further decision making. In alternative embodiments of the present invention, the events being certified may be the detection of a P-wave (cardiac atrial depolarization), T-wave (cardiac ventricular repolarization), a pacing artifact, or any other sensed signal that may be utilized within a rhythm classification architecture. The present invention may also evaluate whether the sensed event was not an R-wave, P-wave, T-wave, pacing artifact, or any other sensed signal that could be misidentified as the sensed event of particular interest.

[0026] In particularly noisy conditions, certain noise may appear as a cardiac event, and thus be mistakenly sensed as such. Examples of noise that may create a low quality electrocardiogram signal include extra-cardiac (skeletal) muscle artifact, 50/60 Hertz interference, electromagnetic interference, electrocautery, or any other passing or intermittent electrical occurrence.

[0027] Assuming that the detection phase 21 does sense noise as an event, this sensed event is then processed through the waveform appraisal phase 22 so that the sensed event may be certified. For the illustrative embodiment, at least some, but preferably all sensed events are processed through the waveform appraisal phase 22. In the waveform appraisal phase 22, the appraisal operator 25 examines the sensed event through various methods and procedures (described below). In this example, noise may diminish the quality of the sensed event. Thus, the sensed event would be determined by the appraisal operator 25 to be something other than a certifiable event. A non-certifiable event is one that is "suspect". Once the appraisal operator 25 has determined that the sensed event cannot be a certifiable event, the appraisal operator 25 further makes the determination to refrain from presenting the suspect event to the third phase of the sensing architecture 20, the classification phase 23. Specifically, the appraisal operator 25 prevents information from suspect event 26 from proceeding any further in the decision making process of the sensing architecture 20. As such, the waveform appraisal phase 25 greatly reduces the likelihood that suspect events will inappropriately direct treatment.

[0028] In further illustration, the appraisal operator 25 also confirms accurately sensed events. When an accurately sensed event is presented to the appraisal operator 25 of the sensing architecture 20, it will be certified. After the appraisal operator 25 has confirmed that the sensed event is certifiable, the appraisal operator 25 then presents the sensed event to the classification phase 23 for its consideration. Thus, again, only sensed events that have been processed through the waveform appraisal phase 22 will be presented to the classification phase 23 of the sensing architecture 20. All suspect events are prevented 26 by the appraisal operator 25 from being available to the classification phase 23.

[0029] The third and final phase of the sensing architecture 20 is the classification phase 23. The classification phase 23 receives data corresponding to events certified by the appraisal operator 25 and performs certain mathematical operations to this certified data. Through these mathematical operations, the classification phase 23 examines attributes such as rate, template comparisons and morphological characteristics, among others. Some illustrative classification phase 23 operations are further discussed in U.S. Patent 7,330,757. Any other suitable classification or analytical methods may also be used, as desired. These analyses aid the sensing architecture 20 in determining whether the certified events are associated with a particular class of rhythms. The classification phase 23 preferably accumulates a sufficient amount of data to render a determination which directs the cardiac rhythm management device to either withhold or deliver therapy to a patient.

[0030] The incorporation of a waveform appraisal phase 22 into a sensing architecture 20 enables the present invention to possess enhanced positive predictivity values. The mathematical formula for positive predictivity is as follows:

$$\text{Positive Predictivity} = (\text{True Positives}) / (\text{True Positives} + \text{False Positives})$$

In several illustrative embodiments, only certified events, and therefore only the highest quality, accurate and representative data, are designed to be sent to the classification phase 23 for evaluation. As such, even legitimate cardiac signals possessing poor quality may not be sent to the classification phase 23 for evaluation. The waveform appraisal phase 22, therefore, is designed to eliminate the preponderance of false positives from consideration by the classification phase. By reducing the number of false positives observed in a classification scheme, the positive predictivity increases

and the system benefits from the reduction in inappropriate therapies delivered to a patient.

5 [0031] This heightened positive predictivity is directly observable in counting schemes used within the classification phase 23 employed by cardiac rhythm management devices. For example, the sensing architecture 20 of an embodiment of the present invention may utilize an X out of Y parameter requiring the classification of eighteen malignant cardiac events out of twenty-four total detected and certified events to declare an episode. The present invention can utilize this classic X out of Y filter; however, the Y input in the present invention will only comprise those events that have been certified. Suspect events, which will include the preponderance of false positives, will have been rejected by the appraisal operator 25 and would not be included in the Y input. Similarly, the X input comprises only those events that are appraised as being certified events through the waveform appraisal phase 22 and classified as dysrhythmic events through the classification phase 23. Thus, a preponderance of false positives are removed by the present invention, dramatically improving the system's positive predictivity.

10 [0032] In contrast, the inclusion of false positive events in the X out of Y filter will result in the reduction of positive predictivity. Therefore, in systems without a waveform appraisal phase 22, the positive predictivity of the counting scheme may be compromised during low quality electrocardiograms. If the positive predictivity is compromised, this may decrease the system's ability to accurately and reliably direct therapy to a patient.

15 [0033] Figure 3 shows an approximately nine second segment of a patient's electrocardiogram 30 that is of low quality. Referring both to Figures 2 and 3, the electrocardiogram in Figure 3 was processed through the sensing architecture 20; including the waveform appraisal phase 22 of the illustrative embodiment. The electrocardiogram 30 shows seven certified events (depicted by the symbol of an inverted triangle) and ten suspect events that were attributed as possessing low quality (depicted by the symbol of a dotted upright triangle). In this particular example, the low quality of the electrocardiogram is attributable to muscle artifact noise.

20 [0034] The first five sensed events 32 in the electrocardiogram were sensed by the detection phase 21, certified through the waveform appraisal phase 22, and presented to the classification phase 23 of the sensing architecture 20 as true cardiac complexes. In contrast, the ten subsequently following sensed events 34 in time were sensed by the detection phase 21, and evaluated and rejected through the waveform appraisal phase 22 as being suspect. Thus, these ten suspect events were not presented to the classification phase 23 - as noted illustratively by the placement of a solid dot in an upright triangle. The last two sensed events 36 in time in the electrocardiogram, however, are depicted as being sensed and certified, and were presented to the classification phase 23.

25 [0035] If the overall system makes use of a counter or register to determine when to provide therapy to a patient, the occurrence of suspect events 34-34 need not necessarily reset or undermine the counting scheme to any great extent. In the illustrative example, counting during a low-quality signal is suspended during the occurrence of one, or a series of suspect events - such as those sensed events 34 graphically illustrated in Figure 3. Embodiments of the classification phase 23 of the present invention could suspend the count through the low quality signal detection, and again continue the count where it left off following the passage of the low quality signal detection. Thus, in the above described example, the classification phase 23 of the present invention would detect the non-continuity of the stream of sensed data, but could still attribute the first certified event following the interruption, the count of eleven and not one. This feature permits the sensing architecture 20 of the present embodiment to greatly reduce any delay in detection. More specifically, the counting requirement could be fulfilled more quickly by the present invention's ability to hold a count as non-certifiable (suspect) events are rejected by the waveform appraisal phase 22, and therefore, would be quicker to declare an episode than a prior art device that must restart the count following the detection of noise. Thus, the present invention is capable of swift and accurate episode detection, which significantly increases the success of therapy delivered to a patient.

30 [0036] Certain embodiments of the present invention and counting operations may also limit the ability to suspend a count. For example, it would be less desirable to have a counting operation, requiring a preset number of events before declaring an episode, be one event shy of the required number, experience a considerable low-quality signal detection period, and then declare an episode on the first certified event following the low-quality signal detection. In this last example, the present invention may hold the count out longer to assure that the most recently sensed events are part of the trend observed prior to the low-quality signal detection. Similarly, if a lengthy low-quality signal is observed by the present invention (one that far outnumbers the previously certified events) or the continuity of the sensed signal is extremely poor, the present invention could also restart a count to assure that the declaration is accurate.

35 [0037] Figures 4 and 5 show how the application of an illustrative embodiment can enhance ICD operation in directing therapy to a patient. The rate threshold for arrhythmia declaration in both Figures 4 and 5 is approximately 180 BPM, and is depicted as a solid line 48. The running average cardiac rate is depicted generally as line 47.

40 [0038] The electrocardiogram in Figure 4 illustrates a scenario where the calculated rate is the only determinative factor in deciding whether to apply or withhold therapy. Therefore, the analytical method applied to the electrocardiogram in Figure 4 does not include a waveform appraisal phase. In the electrocardiogram of Figure 4, a normal sinus rhythm interspersed with low quality cardiac events is depicted as segment 40, and a high quality segment of normal sinus rhythm is shown as segment 42.

45 [0039] The upward excursions of the running cardiac rate 47 during segment 40 are caused by the inappropriate

counting of low-quality events. As a result of this inappropriate rate counting, the patient would have been delivered at least one inappropriate shock, because the only determinative factor for therapy is rate. The points in the electrocardiogram where an event is declared using a prior art algorithm is shown as lines 44 and 46.

5 [0040] The electrocardiogram in Figure 5 illustrates a scenario where a sensing architecture such as sensing architecture 20 in Figure 2 is used, including a waveform appraisal phase 22, as discussed above with reference to Figure 2. The inclusion of the waveform appraisal phase 22 greatly reduces the instances of inappropriate rate counting, and, therefore, inappropriate shocks, such as the ones declared in Figure 4. When the illustrative sensing architecture 20 evaluates the same electrocardiogram signal as Figure 4, it rejects the non-certifiable events as suspect. After the appraisal operator phase 22 rejects the suspect events, it is observed that the illustrative embodiment does not include those suspect events in calculating the running average cardiac rate, and therefore does not deliver therapy. Specifically, 10 when the appraisal operator 20 is presented with the low-quality segment 40, the waveform appraisal phase 14 evaluates the low-quality segment 40, and finds it to be of insufficient quality to use for declaring an event. Thus, in striking comparison to an industry standard sensing architecture as used for the evaluation shown in Figure 4, the illustrative embodiment does not deliver therapy based on the low-quality signals observed in segment 40.

15 [0041] In preferred embodiments of the present invention, whether a cardiac event is accurately detected by the detection phase 21 of the sensing architecture 20, the detection phase 21 is not adjusted by the waveform appraisal phase's determinations. The detection phase 21 continues to operate independently of the remaining portions of the sensing architecture 20. Thus, although the waveform appraisal phase 22 may be evaluating detected events as suspect beats, the detection phase 21 of the sensing architecture 20 continues to sense such events in its customary manner. 20 In alternative embodiments of the present invention, the detection phase 21 may adjust its sensing parameters to compensate for the frequency and number of mischaracterized, and therefore, suspect events.

[0042] Although the present invention has been described with relation to an ICD, a pacing device such as a pacemaker may utilize the present invention when in an ATP state. Thus, when a pacemaker is pacing a heart out of a tachyarrhythmia, the pacemaker may utilize the multi-phase sensing architecture of the present invention to certify whether sensed events 25 have high quality or whether they are of low quality such that they may cause a mischaracterized detection. Additionally, there are other cardiac rhythm management devices that may have applicable states where the sensing architecture of the present invention is particularly suited and beneficial.

[0043] Referring again to Figure 2, the sensing architecture 20 of the illustrative embodiment is capable of implementing several appraisal operators 25, and mechanisms necessary for the performance of the waveform appraisal phase 22. 30 As described above, the events sensed are highly dependent on the type of cardiac rhythm management device used. Likewise, the appraisal operator 25, and the mechanics behinds its operation, is highly dependent on both the cardiac rhythm management device used and the type of events sensed and requiring certification. The present invention, therefore, is not limited in terms of the particular mechanics used during the waveform appraisal phase of the sensing architecture 20. The following descriptions are to illustrate an exemplary mode or configuration chosen from numerous 35 plausible examples.

[0044] Figure 6 shows a block diagram illustrating the steps employed in some embodiments of the present invention for waveform appraisal. From a start block 50, the waveform appraisal is triggered when an event is sensed, as noted at 52. Next, characteristic features of the sensed event are observed, as shown at 54. As noted, the "characteristic features" may take many forms. In illustrative embodiments, the characteristic features concern the shape of the sensed 40 event. Some characteristic features that relate to the event's shape include the inclusion of monotonic segments, monotonic sample groups, or significant maximum slope points (example methods incorporating each are shown, respectively, in Figures 7, 8, and 12). Those skilled in the art will recognize that many of the characteristic features provided have suitable alternatives that may be utilized.

[0045] The waveform appraisal method in Figure 6 continues with the step of counting the characteristic features, as shown at 56. The number of characteristic features is then compared to a threshold, as noted at 58. If the threshold is met, the event is certified as shown at 60, and the waveform appraisal is complete 62. The system then submits the certified event to the classification phase for further analysis. If the threshold is not met, the event is found to be a suspect event that is unsuitable for further analysis, as shown at 64. Then, the system is directed to return to the event sensing module or step until a next event is sensed, as shown at 66.

50 [0046] Figure 7 shows a block diagram illustrating the steps employed in another embodiment of the present invention for waveform appraisal. From a start block 70, the system senses an event 72. Once the event is sensed 72, the system then implements the waveform appraisal phase, including at least some of steps 74-86. First, a collection of Z samples is taken from the sensed event, as shown at 74. This collection of Z samples is analyzed to count the monotonic groups therein, as noted at 76.

55 [0047] The step of counting monotonic groups 76 may be performed, for example, by comparing each successive sample to its predecessor. First a value for a group counter (typically stored in a counter, register or other memory location) is set to zero. Starting with a first sample, the next sample is compared. If the second sample has a value that is greater than the first sample, a direction register can be set to indicate that the samples are increasing in amplitude

with time; alternatively, if the second sample has a value that is less than the first sample, the direction register may be set to indicate that the samples are decreasing. If the second sample has the same amplitude as the first sample, then the direction register may be left at its previous value (which is irrelevant until set). If desired, there may be a minimum change in amplitude required to cause a change in the direction register. Each successive sample is then compared in turn. Whenever the direction register is set to a new value, indicating a change in direction of sensed amplitude change over time, the group counter is incremented to indicate that a new monotonic segment has started.

[0048] After the step of counting monotonic groups shown at 76, the number of monotonic groups is compared to a threshold Y, as noted at 78. If there are less than Y monotonic groups in the Z samples, this indicates a high quality sensed event. A YES result 80 calls for certifying the event, and the system goes to an end 82 that directs the certified event to the classification phase. If a NO result 84 occurs, the system rejects the set of Z samples as a suspect event, discarding the samples from memory, and returns to the sensing step as shown at 86.

[0049] Figure 8 is a block diagram of another illustrative embodiment of an appraisal system 80 including a waveform appraisal phase. The system begins at start block 90 by the system detecting an event. This illustrative embodiment is adapted to work with a sensing architecture that operates in terms of blocks of samples that are received and then sent forward in the analysis structure. As shown at step 92, a set of Z samples are received by the system. The Z samples are then divided into groups of n samples as shown at 94. Each group of samples is evaluated to determine whether it is monotonic or not, and these groups are counted as shown at 96. The system next checks whether at least a threshold value, Y, of the groups are monotonic, as shown at 98. For example, given thirty-two samples, the system may divide the set into eight groups of four samples and determine how many of the groups are monotonic. For such an example, a value of Y=5 could be used, such that five or more of the groups of samples would have to be monotonic to indicate a certified event.

[0050] If there are at least Y monotonic groups, the event is certified as a high-quality sensed event, as shown at 100. The waveform appraisal phase then ends and the system directs the certified event to the classification phase, as shown at 102. Otherwise, if there are less than Y monotonic groups in the set of Z samples, the method rejects the set of samples as a suspect event, as shown at 104, and returns to the sensing block as shown at 106.

[0051] Figures 9A-9B show operation of an illustrative waveform appraisal system on a sensed event. The sensed event 110, as shown in its continuous time analog representation in Figure 9A, is rather idealized and includes only that portion of the cardiac signal including the QRS complex. The T wave, in particular, has been excluded by keeping the time window of sensing narrow. For example, the time window of sensing may be less than one second, less than six-hundred milliseconds, or in the range of about fifty to two-hundred-fifty milliseconds. Figure 9B illustrates a sampled, discrete time representation of the sensed event 110, with the signal including thirty-two samples. The representation of Figure 9B, as can be appreciated by looking at Figure 9A, is a temporally ordered set of samples. The numbers illustrate the number of monotonic segments and when they start by a method similar to the method of Figure 7. The brackets with Y and N letters placed above illustrate whether grouped samples are monotonic by the method of Figure 8, with the thirty-two samples placed in groups of four.

[0052] As can be seen, the event in Figure 9B includes six monotonic segments as counted in the manner illustrated in Figure 7. If a further refinement is included where a segment illustrating no change is not considered a separate monotonic segment, segments 1-2 and 5-6 would each count as a single monotonic segment such that the beat would have only four monotonic segments. If a maximum number of segments is set at six, then the sensed event 110 of Figures 9A-9B would be certified.

[0053] For the method of Figure 8, the results of the group checks yields six monotonic groups and two groups that are not monotonic. If a threshold of 5/8 groups being monotonic is used, then the sensed event 110 of Figures 9A-9B would be certified.

[0054] Figures 10A-10B show operation of an illustrative appraisal operation on a sensed event 120, however, in this example, the sensed event 120 is a low quality event that does not resemble a typical cardiac event. Again, Figure 10A illustrates the sensed event 120 in continuous, analog form. Figure 10B is a sampled (and, if desired, digitized), temporally ordered form of the event, and again indicates analytical results with numbers, brackets, and letters. Using the method of Figure 7, the sensed event 120 includes sixteen monotonic segments. Again using the threshold of six, this sensed event 120 fails to meet the threshold and would be considered suspect. As a result, the method of Figure 7 would not certify the sensed event 120.

[0055] Applying the method of Figure 8, the sensed event 120 has four groups that are monotonic segments. Again, using a threshold of five monotonic segments to be certifiable, the sensed event 120 would be found suspect. Application of the method of Figure 7 would, again, not certify the sensed event 120.

[0056] In another illustrative embodiment, the present invention includes a method of waveform appraisal that includes counting certain maximum slope points in a cardiac signal. The purpose of the maximum slope counter is to capture slope variation in the signal during the generated set of data. Low quality signals tend to have much more first derivative variation than a clean high quality cardiac signal. To capture the variation of the first derivative, the second derivative of the generated set is computed and checked for zero crossings. For an illustrative embodiment, a zero crossing of the

second derivative is defined as one where the second derivative crosses from a non-zero negative to a non-zero positive value and vice versa. Preferably, simply reaching zero is not considered a zero crossing point. Zero crossings of the second derivative of a single generally correspond to the points of local maximum slope (either positive or negative) of the original signal.

[0057] For the illustrative embodiment, the first second derivative zero crossing is accepted as a significant maximum slope point. After that, as each maximum slope point is encountered, it is checked to see if it is significant by applying two rules based on path length. The path length is defined as an accumulation of the magnitude of amplitude changes in the original signal. The rules for the illustrative embodiment are as follows:

1. The path length of the signal between the last significant maximum slope point and the current maximum slope point must be greater than the amplitude difference between the two points.
2. The path length of the signal between the last significant maximum slope point and the current maximum slope point must be greater than a programmed threshold value, derived as a percentage (50%) of the average peak amplitudes of the beats recorded prior to the current detection. If desired, a maximum or minimum for the threshold value may be set. In an illustrative example, using an 8 bit ADC, if the derived threshold value is less than 7 ADC units, the threshold is set at 7 ADC units. If the derived threshold value is greater than 20 ADC units, the threshold is set at 20 ADC units.

[0058] Figure 11 illustrates a method of signal analysis for counting significant maximum slope points. In the illustrative example, a number of signal sample points are shown along with a corresponding analog signal 130. The method includes determining where the second derivative of the sampled signal crosses zero, indicating a maximum magnitude for the slope of the signal at each point. Points A, B, C, D, E and F indicate these points.

[0059] Next, the method includes the step of determining which of points A-F are significant for the purpose of appraising the signal. The magnitude of amplitude change from point to point is determined, including the magnitude of such changes for the intermediate points between points A-F. These amplitude changes are indicated as segments Δ_0 - Δ_7 in Figure 11. A path length value is then determined. The path length value, as noted above, is the accumulation of the magnitude of amplitude changes in the sampled signal occurring between two points. Thus, the sum of the magnitudes of segments Δ_0 to Δ_2 is the path length from C to D, the sum of the magnitudes of segments Δ_0 to Δ_7 is the path length from C to E, and the sum of the magnitudes of segments Δ_3 to Δ_7 is the path length from D to E.

[0060] Next, the actual change in signal amplitude between the points is measured. With these values, the two rules noted above are applied to determine which maximum slope points are significant for appraising the signal. For illustrative purposes, point C is assumed to be certified (C would in fact be certified in the Figure). Using point C as a reference point, from point C to point D, the path length is the same as the amplitude change, therefore, point D is not a significant maximum slope point under Rule 1. Therefore, point D is rejected.

[0061] The next step is to go to the next identified maximum slope point, point E, to determine if it is significant for the appraisal method. In this case, the path length from point C to point E exceeds the amplitude change between these two points. Rule 2 is passed because the path length exceeds the illustrated threshold path length minimum. Because the requirements of both rules are met, point E is a significant maximum slope point for the appraisal method.

[0062] In further illustration, it can be seen that point B is not a significant maximum slope point because the path length from point A to point B does not exceed the threshold path length minimum. This fails Rule 1, above, and point B would be rejected.

[0063] The above analysis yields three significant maximum slope points in the signal shown in Figure 11. If, for example, the threshold maximum number of significant maximum slope points is set at six, then the illustrated signal is considered a certified signal.

[0064] Figure 12 shows in block form steps of an illustrative maximum slope point counting method for appraising a received signal. The method begins by receiving a signal, as shown at 140. Next, the maximum slope points are identified, as noted at 142. The first maximum slope point is identified as a significant maximum slope point, as noted at 144. As illustrated in block 146, the rest of the significant maximum slope points are identified by taking a next maximum slope point as shown at 148, and applying the first rule as shown at 150 and the second rule as shown at 152. After the significant maximum slope points are identified in block 148, the number of significant maximum slope points is compared to a threshold, as shown at 154. If the threshold is not exceeded, the signal is certified, as noted at 156. If the threshold is exceeded, then the signal is marked as suspect, as noted at 158. In some embodiments, after the signal is marked as suspect, it may be subjected to further analysis, for example, to determine if changes in the event detection architecture are needed. In other embodiments, suspect signals are discarded.

[0065] The following illustrative embodiments are explained in terms of operational circuitry. The operational circuitry may be configured to include such controllers, microcontrollers, logic devices, memory, and the like, as selected, needed, or desired, for performing the steps for which each is configured.

[0066] An illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode as-

sembly including a number of electrodes, and a canister housing operational circuitry. For the illustrative embodiment, the lead electrode assembly is coupled to the canister; and the operational circuitry is configured to receive a cardiac signal from implanted electrodes, observe characteristic features of the shape of the signal, count the characteristic features, and compare the number of characteristic features to a threshold. With the comparison to the threshold, the operational circuitry is further configured to certify the signal for use in characterizing a cardiac complex, or determine the signal is unsuitable for use in characterizing a cardiac complex. In another embodiment, the operational circuitry is configured such that the step of receiving a signal includes sensing electrical activity and using an event detector to determine the parameters of the signal. In yet a further embodiment, the operational circuitry is configured such that the step of observing characteristic features includes identifying a number of points in the signal where the signal slope reaches a local maximum magnitude.

[0067] For a related illustrative embodiment, the implantable cardioverter/defibrillator includes operational circuitry configured such that the step of identifying a number of points in the signal includes identifying zero crossings of the second derivative of the signal. In another embodiment, the operational circuitry is configured such that the step of observing characteristic features includes selecting a first zero crossing as a significant maximum slope point, and characterizing subsequent zero crossings as either significant maximum slope points or not significant maximum slope points, wherein the significant maximum slope points are observed to be the characteristic features. In a related embodiment, the operational circuitry is configured such that the step of characterizing subsequent zero crossings includes application of a rule related to a threshold for consideration of separate points in the signal. In yet another embodiment, the operational circuitry is configured such that the rule calls for determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds a path length threshold. A further related embodiment includes operational circuitry configured such that the path length threshold is related to a selected percentage of the maximum signal amplitude for a chosen cardiac complex.

[0068] In another embodiment, the operational circuitry is configured such that the step of characterizing subsequent zero crossings includes application of a rule related to the signal shape between two points in the signal. In a further, related embodiment, the operational circuitry is configured such that the rule calls for determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds the magnitude of the difference in amplitude between the signal at the time of the most recent significant maximum slope point, and the signal at the time of the zero crossing under consideration.

[0069] In another embodiment, the operational circuitry is configured such that a step of characterizing subsequent zero crossings includes analysis using a first rule and a second rule, the first rule being related to a threshold for consideration of separate points in the signal, the second rule being related to the signal shape between two points in the signal. In a further embodiment, the operational circuitry is configured such that the first rule calls for determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds a path length threshold, and the second rule calls for determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds the magnitude of the difference in amplitude between, the signal at the time of the most recent significant maximum slope point, and the signal at the time of the zero crossing under consideration. In another related embodiment, the operational circuitry is configured such that the step of observing characteristic features of the signal includes assessment of the degree of monotonicity of the signal.

[0070] In another embodiment, the operational circuitry is configured such that the step of observing characteristic features of the signal includes counting a number of monotonic segments of the signal. Yet another embodiment includes operational circuitry configured such that the signal has a duration of less than one second. In several embodiments, the implantable cardioverter/defibrillator includes operational circuitry comprising a controller and a controller readable memory.

[0071] An illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to: sample a signal from an implanted electrode; identify maximum slope points in the sample signal corresponding to local signal slope maximums; analyze the sample signal to determine which of the maximum slope points are significant; and compare the number of significant maximum slope points to a threshold.

[0072] Another illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to: receive a signal from a pair of implanted electrodes; sense whether a likely cardiac event has occurred; observe the monotonic characteristics of the signal during a time period corresponding to the likely cardiac event; and determine whether the signal during the time period is sufficiently monotonic to indicate the cardiac signal can be certified for classifying a cardiac rhythm. In a further embodiment, the operational circuitry is configured such that the step of observing the monotonic characteristics includes grouping together samples of the cardiac signal from the time period into sample groups, and observing whether each

sample group is monotonic. In yet another embodiment, the operational circuitry is configured such that the step of observing the monotonic characteristics includes counting the number of times that an ordered set of samples of the cardiac signal corresponding to the time period changes its direction of amplitude change. Another illustrative embodiment includes operational circuitry is configured such that the step of observing the monotonic characteristics includes counting a number of monotonic segments found in a sampling of the cardiac signal corresponding to the time period. An illustrative embodiment further includes operational circuitry configured to classify the event to determine whether the event indicates treatment. In another embodiment, the operational circuitry is further configured to determine whether a cardiac signal appears to indicate a patient's heart is beating at a rate above a rate threshold before performing the receive, sense, observe, and determine steps. In yet another embodiment, the operational circuitry comprises a controller and a controller readable memory.

[0073] An illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to: sample a cardiac signal from a pair of implanted electrodes; define a number of groups of samples from a portion of the signal; determine how many of the groups of samples are monotonic; and, if the number of monotonic groups does not exceed a threshold, discard the portion of the signal.

[0074] Another illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to determine whether a heart is pumping at a rate exceeding a threshold, and, if so, perform the following steps: sample a cardiac signal from a pair of implanted electrodes; define a number of groups of samples from a portion of the signal; determine how many of the groups of samples are monotonic; and if the number of monotonic groups does not exceed a threshold, discard the portion of the signal. In another embodiment, the operational circuitry is further configured to classify the signal by analyzing non-discarded portions of the signal, wherein the step of classifying the signal includes classifying portions of the signal as either indicating treatment or not indicating treatment. In yet another illustrative embodiment, the operational circuitry is further configured such that the step of classifying the signal includes keeping a count of classified portions until a threshold number of portions are classified; wherein, when the threshold number of portions are classified, the method further includes determining whether to provide treatment based upon whether a predetermined number of classified portions indicate treatment.

[0075] Another illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to: sample a signal from first and second implanted electrodes; set a threshold for the monotonicity of a sensed signal; determine whether the sampled signal meets the threshold; and if the sampled signal does not meet the threshold, discard the signal.

[0076] Yet another illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to: receive a signal from first and second implanted electrodes; observe a point in the signal; observe a number of samples of the signal following the point; group the samples into a number of groups; observe which of the groups are monotonic; count the monotonic groups; determine whether the number of monotonic groups exceeds a threshold; and, if the number of monotonic groups does not exceed the threshold, discard the portion of the signal from which the number of signals following the point were taken.

[0077] An illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to: receive a signal from first and second implanted electrodes; observe a monotonic segment of the signal; measure the length of the monotonic segment; compare the length to a threshold; and, if the length is less than the threshold, determine that the monotonic segment does not correspond to a certifiable cardiac event. In a related embodiment, the operational circuitry is further configured to observe a portion of the signal around the monotonic segment, determine whether the monotonic segment ends in a highest signal strength for the portion, and, if the monotonic segment does not end in a highest signal strength for the portion, determining that the monotonic segment does not correspond to a certifiable cardiac event. In another embodiment, the operational circuitry is further configured such that the portion corresponds to time window around the monotonic segment, at least a portion of the time window occurring before the monotonic segment begins, and at least a portion of the time window occurring after the monotonic segment ends, the window having a duration in the range of 50-250 milliseconds.

[0078] Another embodiment includes an implantable cardiac treatment system comprising first and second electrodes, and circuitry contained in a housing, the circuitry electrically coupled to the first and second electrodes, wherein the circuitry is adapted to perform the following steps: sampling a signal from first and second implanted electrodes; setting a threshold for the monotonicity of a sensed signal; determining whether the sampled signal meets the threshold; and,

if the sampled signal does not meet the threshold, discarding the signal. In a further embodiment, the circuitry includes a controller and a controller readable medium, the controller readable medium containing instructions thereon for performing the steps of sampling, setting, determining and discarding.

5 [0079] Yet another embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to monitor a signal produced between implanted electrodes to observe an event, observe an event and gathering a signal corresponding to the event, observe characteristic features of the shape of the signal, count the characteristic features, and compare the number of characteristic features to a threshold to certify the signal for use in characterizing a cardiac complex, or determine the signal is unsuitable for use in characterizing a cardiac complex. In the illustrative embodiment, if the signal is certified, the operational circuitry is also configured to use the signal to determine whether a malignant cardiac rhythm is likely occurring.

10 [0080] An illustrative embodiment includes an implantable cardioverter/defibrillator comprising a lead electrode assembly including a number of electrodes, and a canister housing operational circuitry, wherein the lead electrode assembly is coupled to the canister, and the operational circuitry is configured to capture a signal using implanted electrodes placed for observing electrical cardiac activity, analyze the signal to determine whether the signal is suitable for characterizing a cardiac rhythm, and, if the signal is suitable, use the signal to determine whether a malignant cardiac rhythm is likely occurring, or, if the signal is not suitable, reject the signal.

15 [0081] Numerous characteristics and advantages of the invention covered by this document have been set forth in the foregoing description. It will be understood, however, that this disclosure is, in many aspects, only illustrative. Changes may be made in details, particularly in matters of shape, size and arrangement of parts without exceeding the scope of the invention. The invention's scope is defined, of course, in the language in which the claims are expressed.

25 Claims

1. An implantable cardioverter/defibrillator comprising:

30 a lead electrode assembly (3,12) including a number of electrodes (5,6,7,13,14), and a canister (2,11) housing operational circuitry; wherein the lead electrode assembly (3,12) is coupled to the canister (2,11), **characterized in that** the operational circuitry is configured to:

35 receive a cardiac signal from implanted electrodes (5,6,7,13,14);
observe characteristic features of the shape of the signal;
count the characteristic features to determine the quantity of said characteristic features; and
compare the quantity of said characteristic features to a threshold to:

40 certify the signal for use in characterizing a cardiac complex; or
determine the signal is unsuitable for use in characterizing a cardiac complex;

wherein the operational circuitry is further configured such that the step of observing characteristic features includes:

45 identifying a number of points in the signal where the signal slope reaches a local maximum magnitude by identifying zero crossings of the second derivative of the signal;
selecting a first zero crossing as a significant maximum slope point; and
characterizing subsequent zero crossings as either significant maximum slope points or not significant maximum slope points;

50 wherein the significant maximum slope points are observed to be the characteristic features.

2. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry is configured such that the step of receiving a signal includes sensing electrical activity and using an event detector to determine the parameters of the signal.

3. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry is configured such that the step of characterizing subsequent zero crossings includes determining whether the path length from a most recent

significant maximum slope point to the zero crossing under consideration exceeds a path length threshold.

4. The implantable cardioverter/defibrillator of claim 3, wherein the operational circuitry is configured such that the path length threshold is related to a selected percentage of the maximum signal amplitude for a chosen cardiac complex.

5. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry is configured such that the step of characterizing subsequent zero crossings includes determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds the magnitude of the difference in amplitude between:

the signal at the time of the most recent significant maximum slope point; and
the signal at the time of the zero crossing under consideration.

6. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry is configured such that the step of characterizing subsequent zero crossings includes analysis using a first rule and a second rule; wherein the first rule calls for determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds a path length threshold; and the second rule calls for determining whether the path length from a most recent significant maximum slope point to the zero crossing under consideration exceeds the magnitude of the difference in amplitude between:

the signal at the time of the most recent significant maximum slope point; and
the signal at the time of the zero crossing under consideration.

7. The implantable cardioverter/defibrillator of claim 6, wherein the operational circuitry is configured such that the step of observing characteristic features of the signal includes assessment of the degree of monotonicity of the signal.

8. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry is configured such that the step of observing characteristic features of the signal includes counting a number of monotonic segments of the signal.

9. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry is configured such that the signal has a duration of less than one second.

10. The implantable cardioverter/defibrillator of claim 1, wherein the operational circuitry comprises a controller and a controller readable memory.

Patentansprüche

1. Implantierbarer Cardioverter/Defibrillator mit:

einer Leitungselektrodenanordnung (3, 12) mit mehreren Elektroden (5,6,7,13,14); und einem Behälter (2, 11), in dem eine Betriebsschaltung untergebracht ist; wobei die Leitungselektrodenanordnung (3, 12) mit dem Behälter (2,11) verbunden ist; **dadurch gekennzeichnet, dass** die Betriebsschaltung konfiguriert ist:

ein kardiales Signal von den implantierten Elektroden (5,6,7,13,14) zu empfangen;
charakteristische Merkmale der Signalf orm zu beobachten;
die charakteristischen Merkmale zu zählen, um die Quantität der charakteristischen Merkmale zu bestimmen; und

die Quantität der charakteristischen Merkmale mit einem Schwellenwert zu vergleichen, um das Signal für eine Verwendung bei einer Charakterisierung eines kardialen Komplexes zu zertifizieren; oder um zu bestimmen, dass das Signal für eine Verwendung bei einer Charakterisierung eines kardialen Komplexes ungeeignet ist;

wobei die Betriebsschaltung außerdem derart konfiguriert ist, dass der Schritt zur Beobachtung charakteristischer Merkmale aufweist:

Identifizieren von mehreren Punkten in dem Signal, an welchen die Steigung des Signals ein lokales Maximum erreicht, durch Identifizieren von Nulldurchgängen der zweiten Ableitung des Signals;

EP 1 631 350 B1

Wählen eines ersten Nulldurchgangs als signifikanten Punkt maximaler Steigung; und
Charakterisieren nachfolgender Nulldurchgänge entweder als signifikante Punkte maximaler Steigung
oder als nicht-signifikante Punkte maximaler Steigung;
wobei die signifikanten Punkte maximaler Steigung als die charakteristischen Merkmale beobachtet
werden.

- 5
2. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schritt des Empfangens eines Signals das Messen einer elektrischen Aktivität und Verwenden eines Ereignisdetektors, um die Parameter des Signals zu bestimmen, aufweist.
- 10
3. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schritt zur Charakterisierung nachfolgender Nulldurchgänge aufweist: Bestimmen, ob die Pfadlänge zwischen einem unmittelbar vorausgehenden signifikanten Punkt maximaler Steigung und dem betrachteten Nulldurchgang größer ist als ein Schwellenwert für die Pfadlänge.
- 15
4. Implantierbarer Cardioverter/Defibrillator nach Anspruch 3, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schwellenwert für die Pfadlänge verknüpft ist mit einem gewählten Prozentsatz der maximalen Signalamplitude für einen gewählten kardialen Komplex.
- 20
5. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schritt zur Charakterisierung nachfolgender Nulldurchgänge aufweist: Bestimmen, ob die Pfadlänge zwischen einem unmittelbar vorausgehenden signifikanten Punkt maximaler Steigung und dem betrachteten Nulldurchgang größer ist als der Betrag der Differenz zwischen der Signalamplitude zum Zeitpunkt des unmittelbar vorausgehenden signifikanten Punkts maximaler Steigung und der Signalamplitude zum Zeitpunkt des betrachteten Nulldurchgangs.
- 25
6. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schritt zur Charakterisierung nachfolgender Nulldurchgänge aufweist: Analysieren unter Verwendung einer ersten Regel und einer zweiten Regel; wobei die erste Regel eine Ermittlung verlangt, ob die Pfadlänge zwischen einem unmittelbar vorausgehenden signifikanten Punkt maximaler Steigung und dem betrachteten Nulldurchgang größer ist als ein Schwellenwert für die Pfadlänge; und die zweite Regel eine Ermittlung verlangt, ob die Pfadlänge zwischen einem unmittelbar vorausgehenden signifikanten Punkt maximaler Steigung und dem betrachteten Nulldurchgang größer ist als der Betrag der Differenz zwischen der Signalamplitude zum Zeitpunkt des unmittelbar vorausgehenden signifikanten Punkts maximaler Steigung und der Signalamplitude zum Zeitpunkt des betrachteten Nulldurchgangs.
- 30
7. Implantierbarer Cardioverter/Defibrillator nach Anspruch 6, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schritt zur Beobachtung charakteristischer Merkmale des Signals eine Abschätzung des Monotonizitätsgrads des Signals aufweist.
- 35
8. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung derart konfiguriert ist, dass der Schritt zur Beobachtung charakteristischer Merkmale des Signals ein Zählen der Anzahl der monotonen Segmente des Signals aufweist.
- 40
9. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung derart konfiguriert ist, dass das Signal eine Dauer von weniger als eine Sekunde hat.
- 45
10. Implantierbarer Cardioverter/Defibrillator nach Anspruch 1, wobei die Betriebsschaltung einen Controller und ein controllerlesbarer Speicher aufweist.

50

Revendications

1. Défibrillateur cardiovertteur implantable comprenant :

55 un assemblage d'électrodes de dérivation (3,12) englobant plusieurs électrodes (5,6,7,13,14), et un boîtier (2,11) dans lequel vient se loger un ensemble de circuits d'exploitation, l'assemblage d'électrodes de dérivation(3,12) étant couplé au boîtier(2,11), **caractérisé en ce que:**

EP 1 631 350 B1

l'ensemble de circuits d'exploitation est configuré pour recevoir un signal cardiaque émis par des électrodes implantées (5,6,7,13,14); observer les caractéristiques techniques de la configuration du signal ; compter les caractéristiques techniques pour déterminer la quantité desdites caractéristiques techniques ; et comparer la quantité desdites caractéristiques techniques à une valeur seuil pour :

certifier le signal pour son utilisation dans la caractérisation d'un complexe cardiaque ; ou déterminer le fait que le signal est inapproprié pour être utilisé dans la caractérisation d'un complexe cardiaque ;

dans lequel l'ensemble de circuits d'exploitation est en outre configuré de telle sorte que l'étape d'observation des caractéristiques techniques englobe le fait de :

identifier un certain nombre de points dans le signal auquel la pente du signal atteint une valeur maximale locale par identification des passages par la valeur zéro de la dérivée seconde du signal ; sélectionner un premier passage par la valeur zéro comme étant un point de la pente correspondant à une valeur maximale significative ; et caractériser les passages ultérieurs par la valeur zéro comme étant soit des points de la pente correspondant à des valeurs maximales significatives, soit des points de la pente correspondant à des valeurs maximales non significatives ;

les points de la pente correspondant à des valeurs maximales significatives étant considérés comme étant les caractéristiques techniques.

2. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que l'étape de réception d'un signal englobe la détection d'une activité électrique et l'utilisation d'un détecteur d'événement pour déterminer les paramètres du signal.

3. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que l'étape de caractérisation des passages ultérieurs par la valeur zéro englobe la détermination du fait de savoir si la longueur de parcours depuis le point le plus récent de la pente représentant une valeur maximale significative jusqu'au passage par zéro pris en considération dépasse un seuil de longueur de parcours.

4. Défibrillateur cardiovertteur implantable selon la revendication 3, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que le seuil de longueur de parcours est lié à un pourcentage sélectionné de l'amplitude maximale du signal pour un complexe cardiaque sélectionné.

5. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que l'étape de caractérisation des passages ultérieurs par la valeur zéro englobe la détermination du fait de savoir si la longueur de parcours depuis le point le plus récent de la pente représentant une valeur maximale significative jusqu'au passage par zéro pris en considération dépasse la valeur de la différence d'amplitude entre :

le signal en vigueur au moment du point le plus récent de la pente correspondant à la valeur maximale significative ; et

le signal en vigueur au moment du passage par la valeur zéro, pris en considération.

6. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que l'étape de caractérisation des passages ultérieurs par la valeur zéro englobe une analyse en utilisant une première règle et une deuxième règle, la première règle servant à déterminer le fait de savoir si la longueur de parcours depuis le point le plus récent de la pente représentant une valeur maximale significative jusqu'au passage par zéro pris en considération dépasse un seuil de longueur de parcours et la deuxième règle servant à déterminer le fait de savoir si la longueur de parcours depuis le point le plus récent de la pente représentant une valeur maximale significative jusqu'au passage par zéro pris en considération dépasse la valeur de la différence d'amplitude entre :



le signal en vigueur au moment du point le plus récent de la pente correspondant à la valeur maximale

EP 1 631 350 B1

significative ; et

le signal en vigueur au moment du passage par la valeur zéro, pris en considération.

- 5
7. Défibrillateur cardiovertteur implantable selon la revendication 6, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que l'étape d'observation des caractéristiques techniques du signal englobe l'évaluation du degré de monotonie du signal.
- 10
8. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que l'étape d'observation des caractéristiques techniques du signal englobe le comptage du nombre de segments monotones du signal.
- 15
9. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation est configuré de telle sorte que le signal possède une durée inférieure à une seconde.
- 20
- 25
- 30
- 35
- 40
- 45
- 50
- 55
10. Défibrillateur cardiovertteur implantable selon la revendication 1, dans lequel l'ensemble de circuits d'exploitation comprend un contrôleur et une mémoire lisible par le contrôleur.

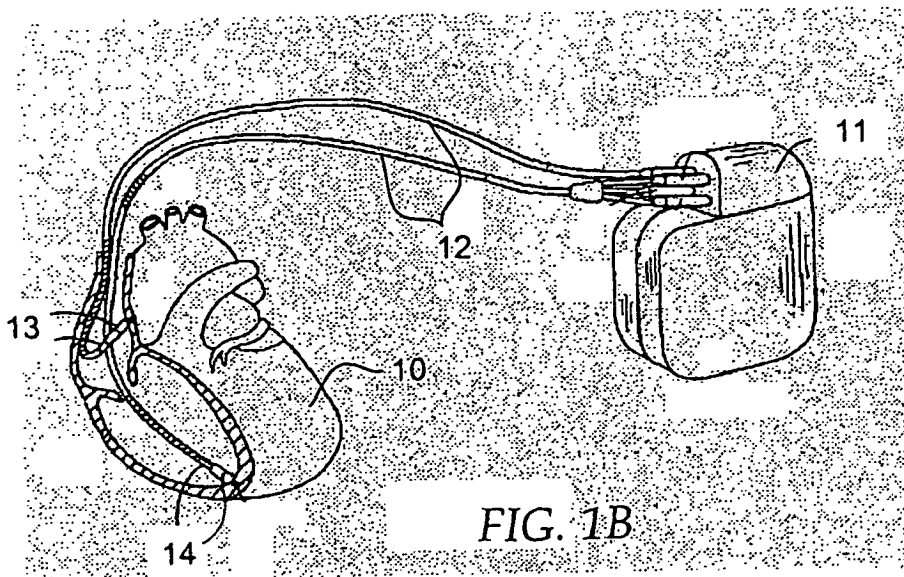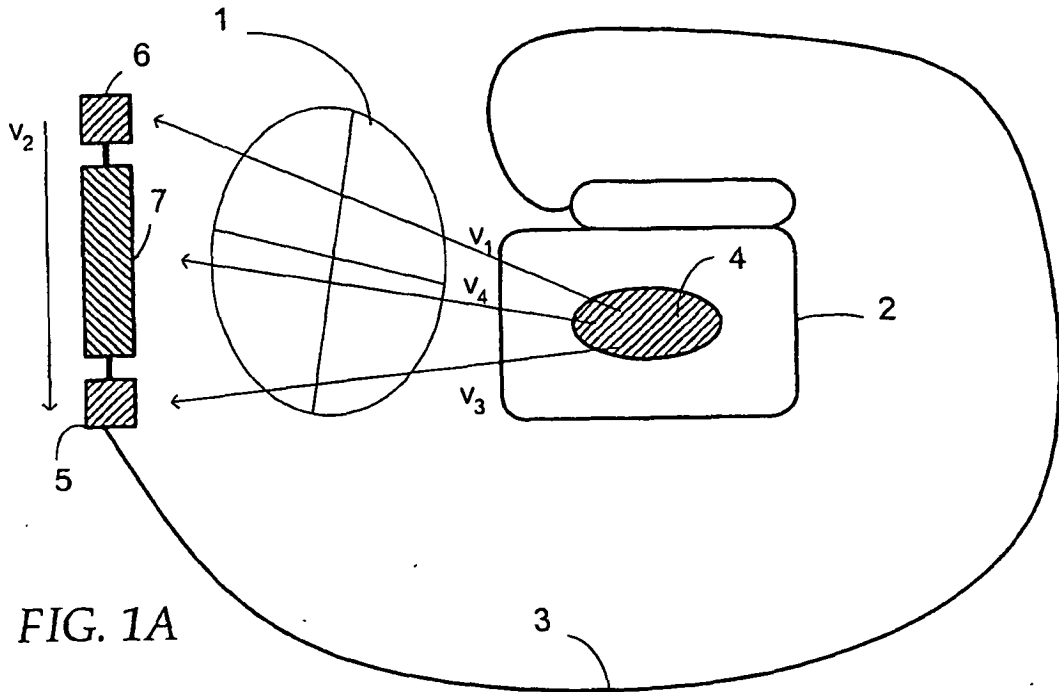

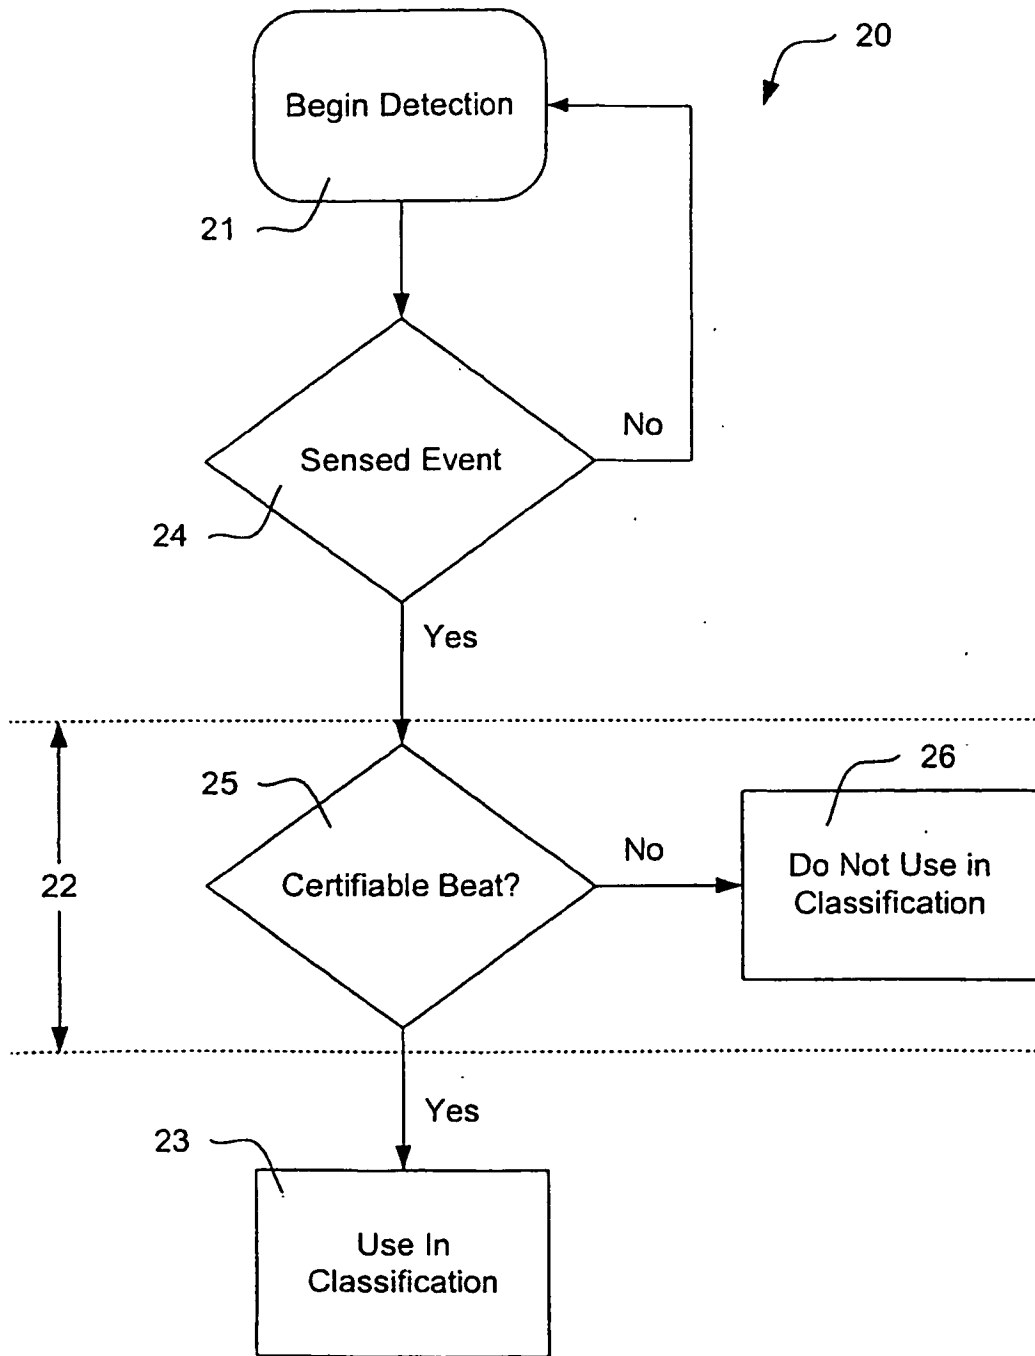


FIG. 2

FIG. 3

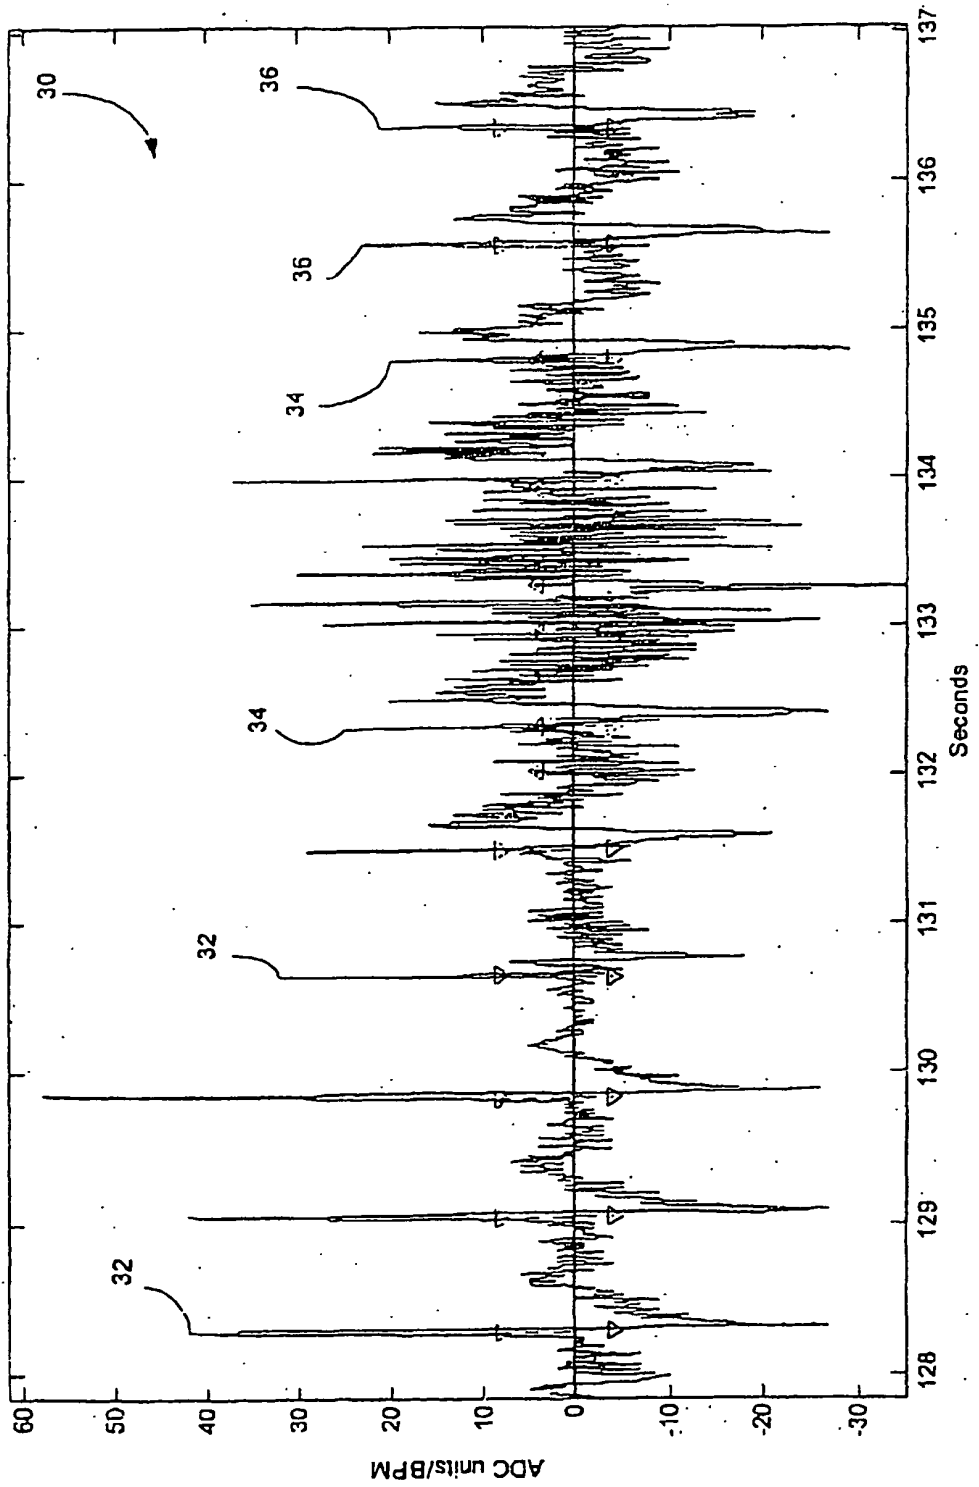


FIG. 4

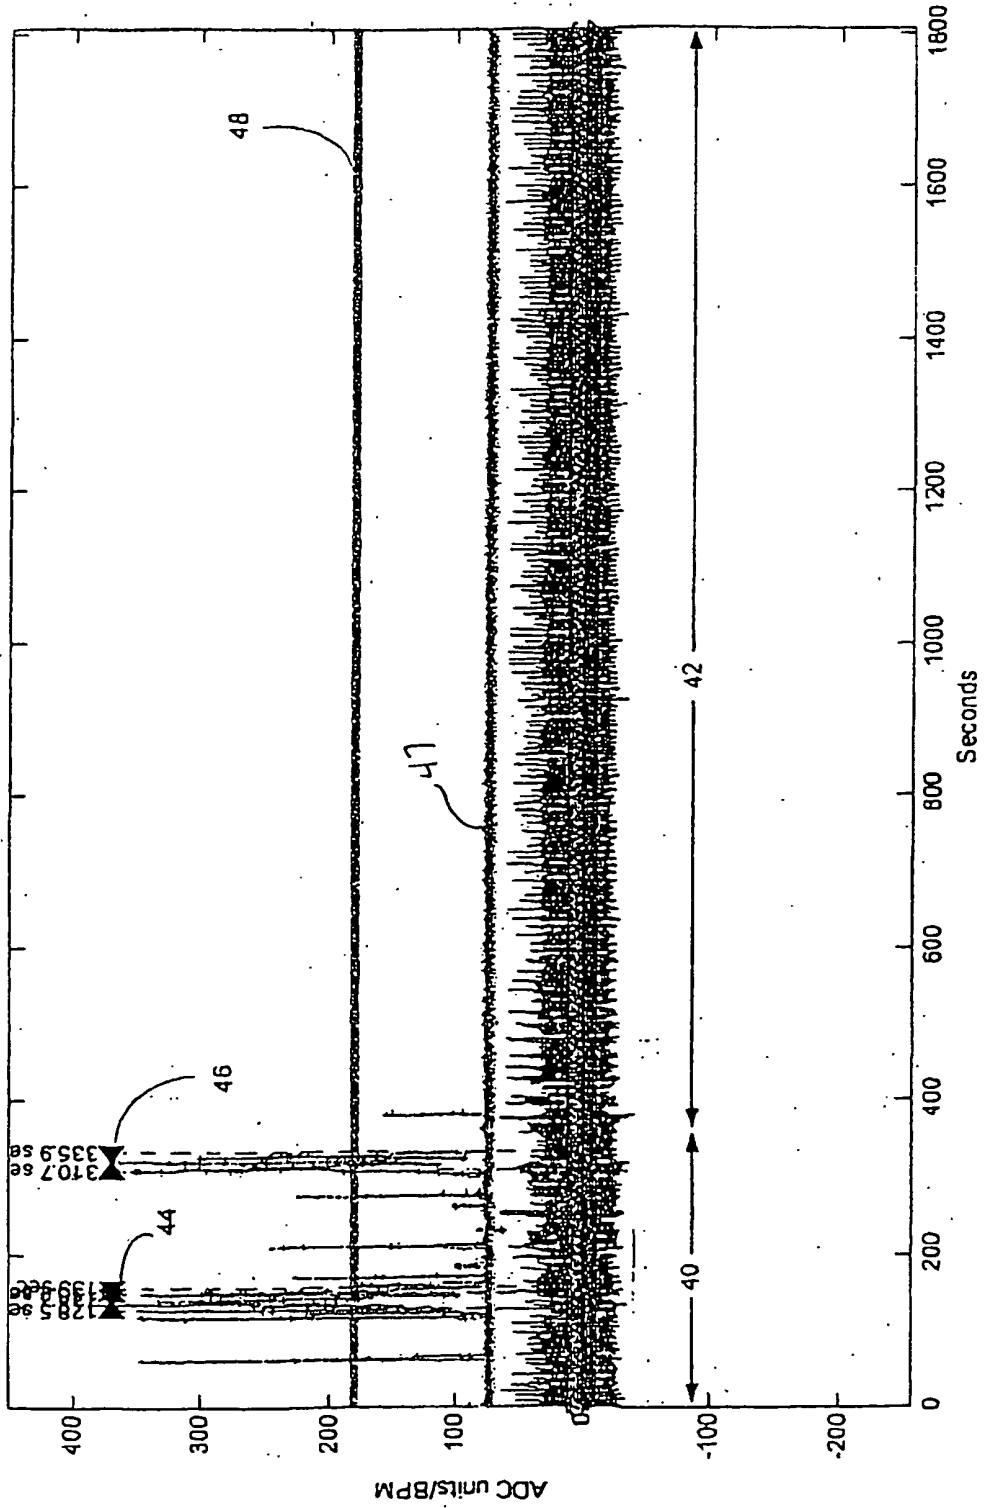
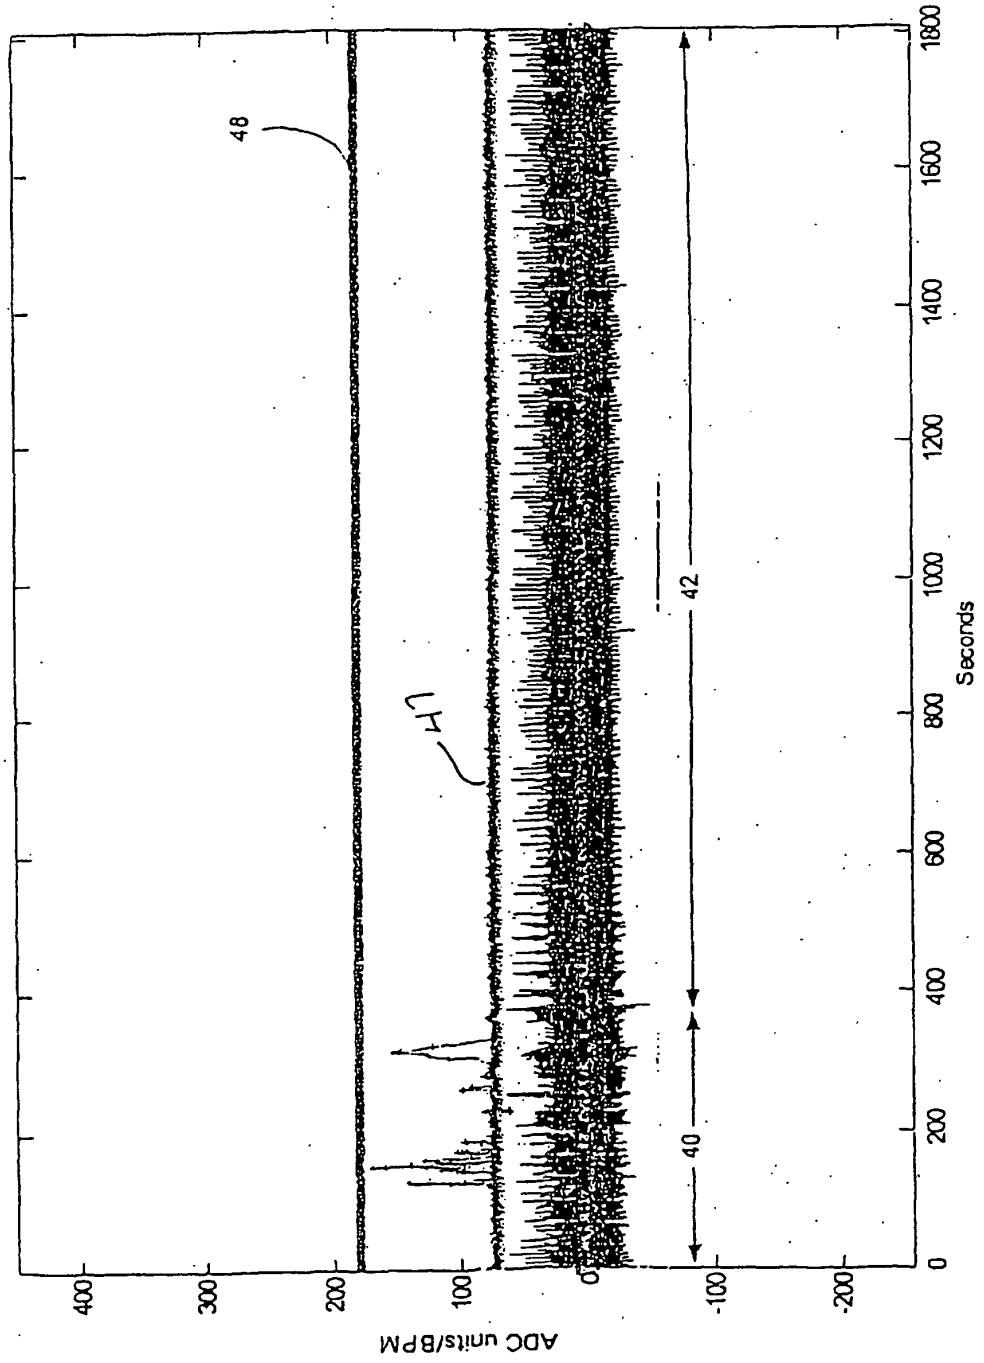


FIG. 5



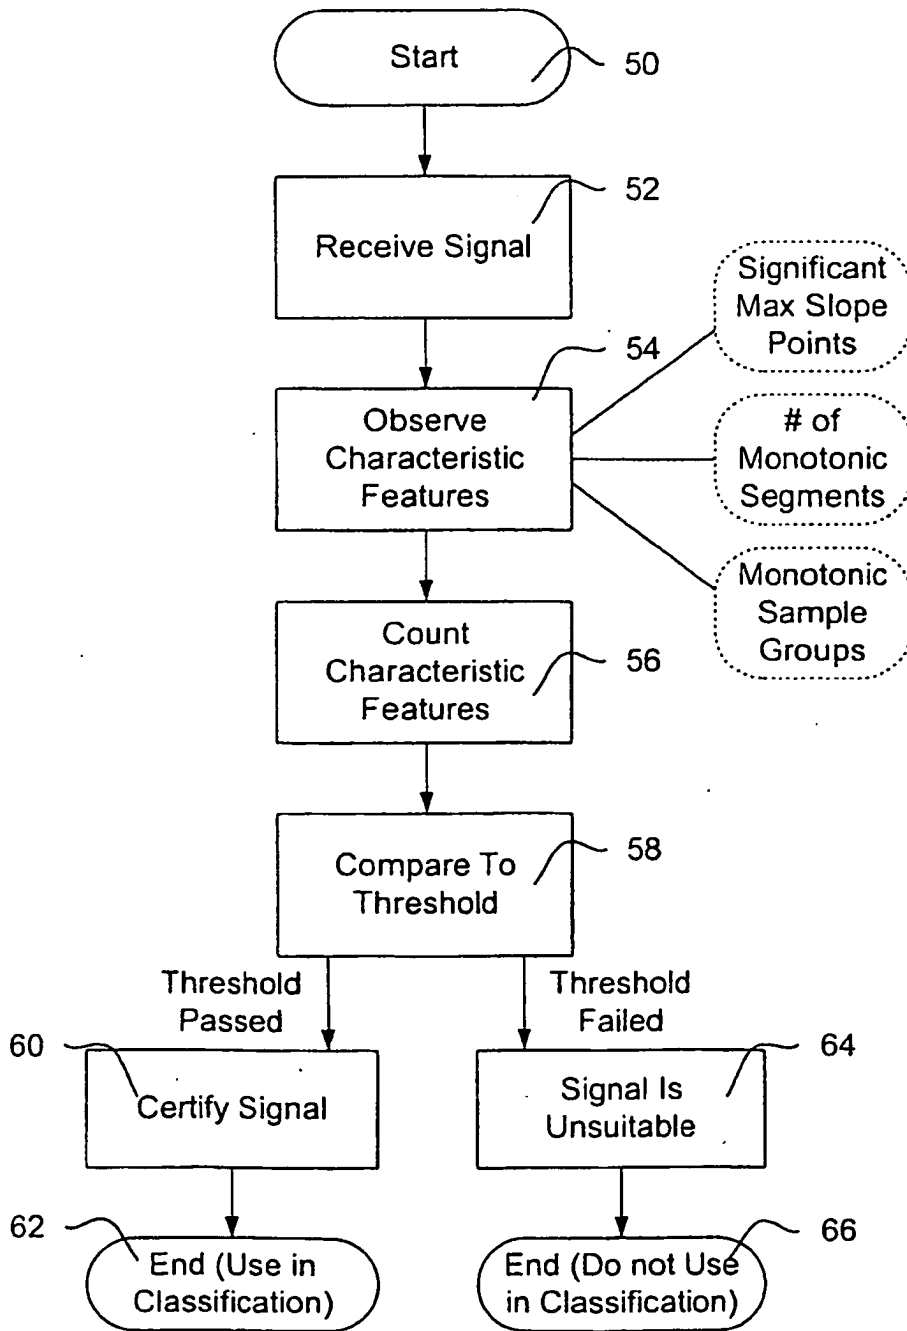


FIG. 6

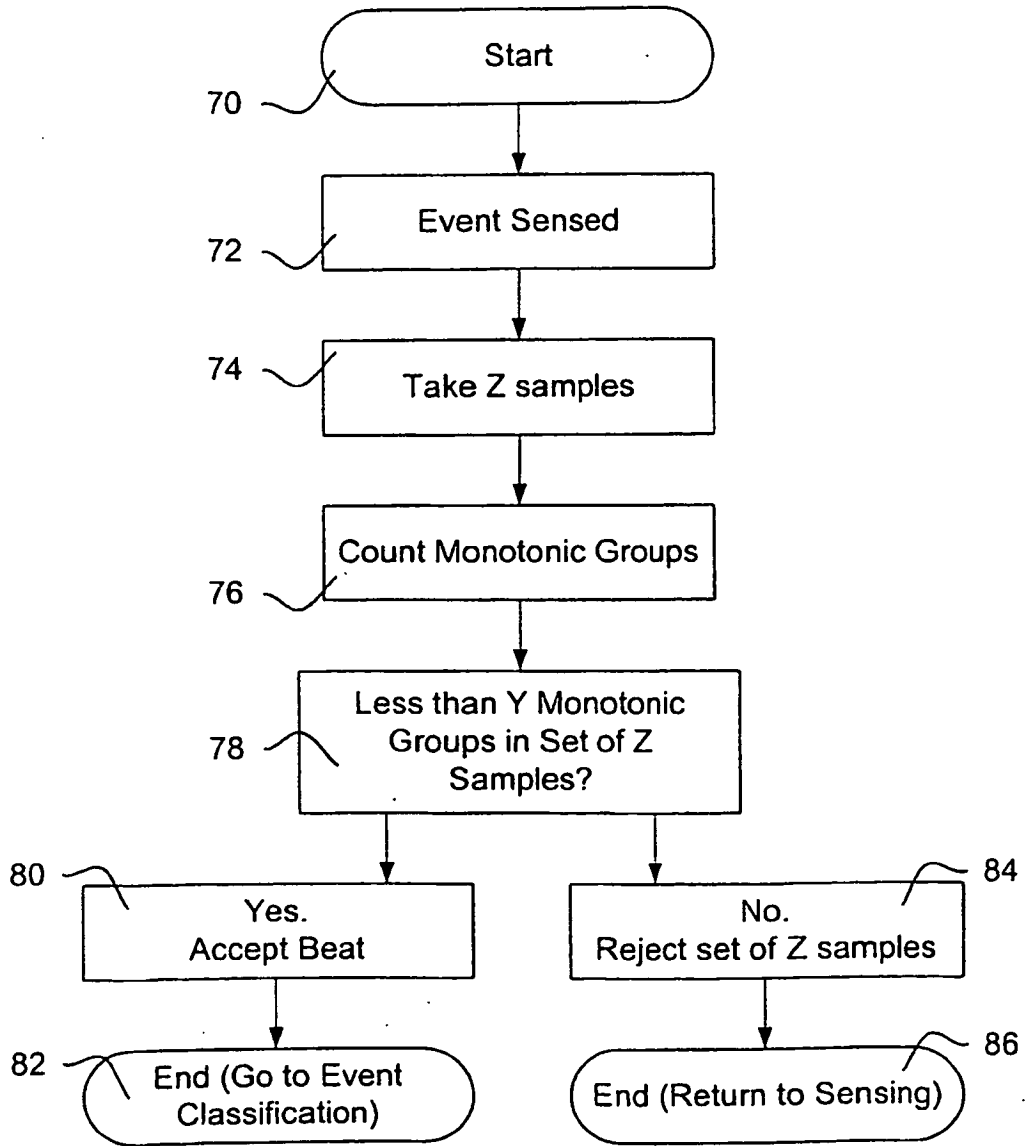


FIG. 7

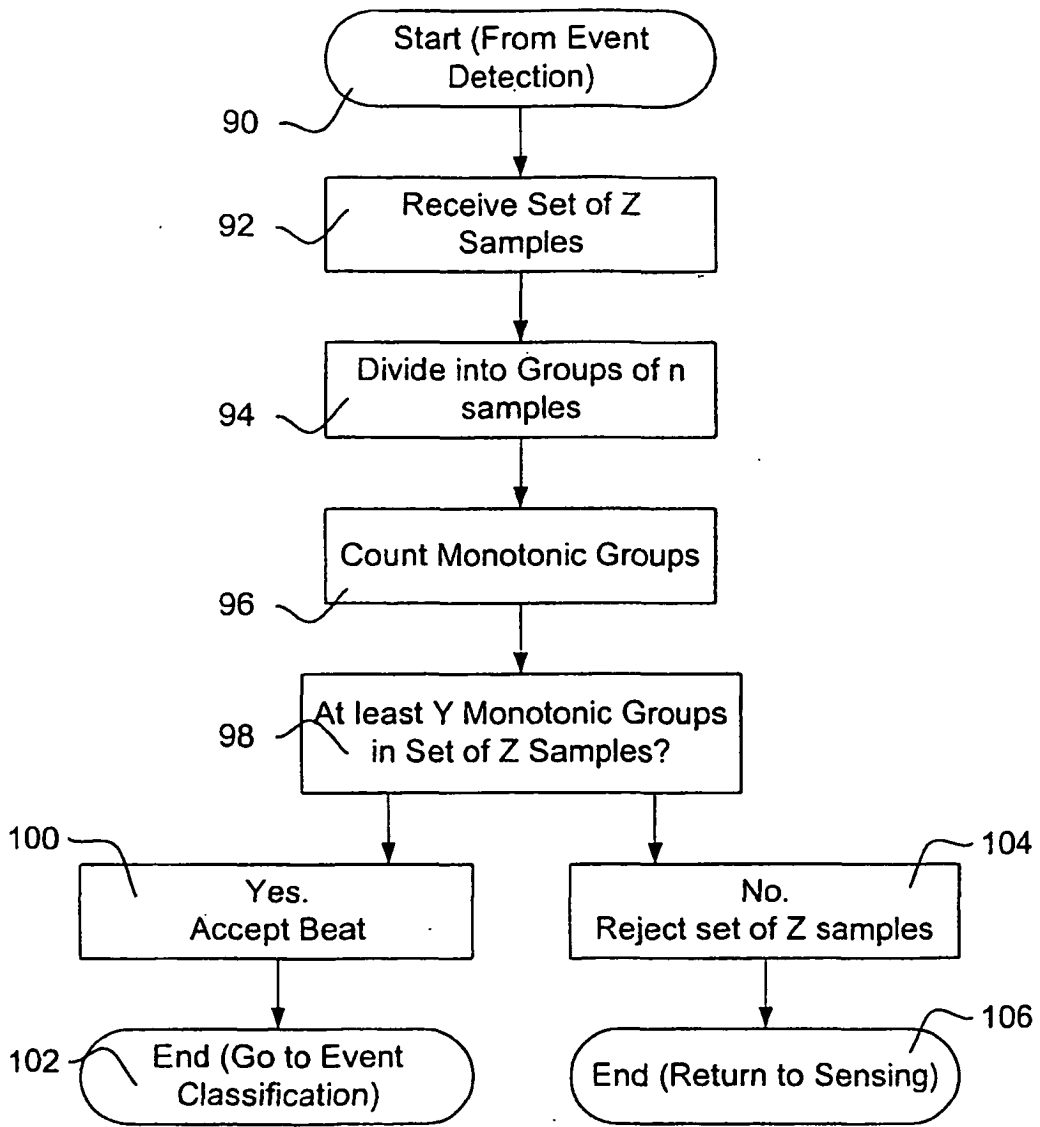


FIG. 8

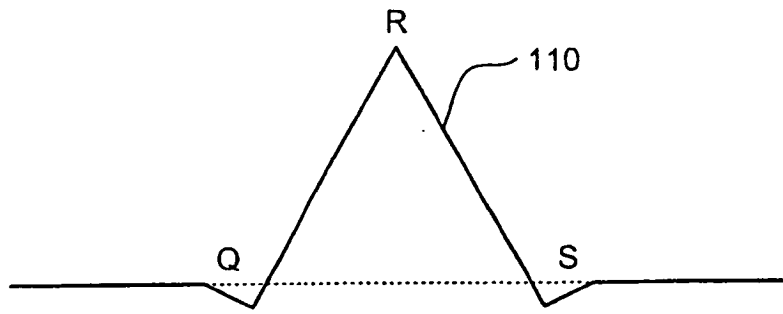


FIG. 9A

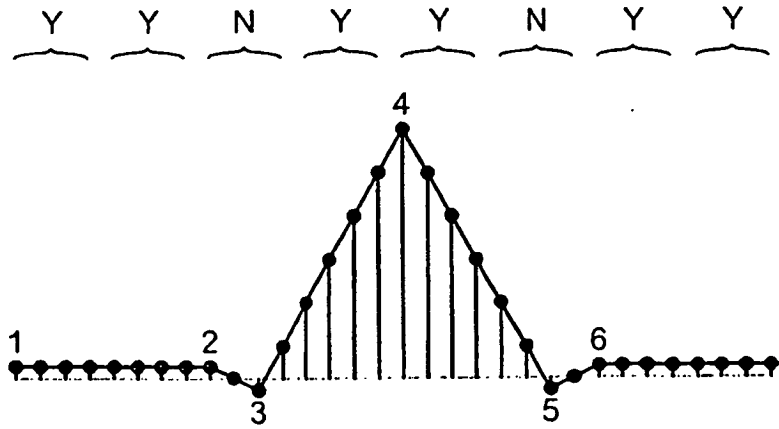


FIG. 9B

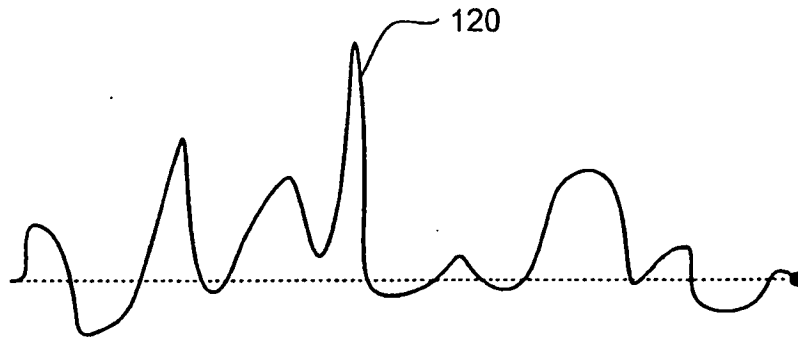


FIG. 10A

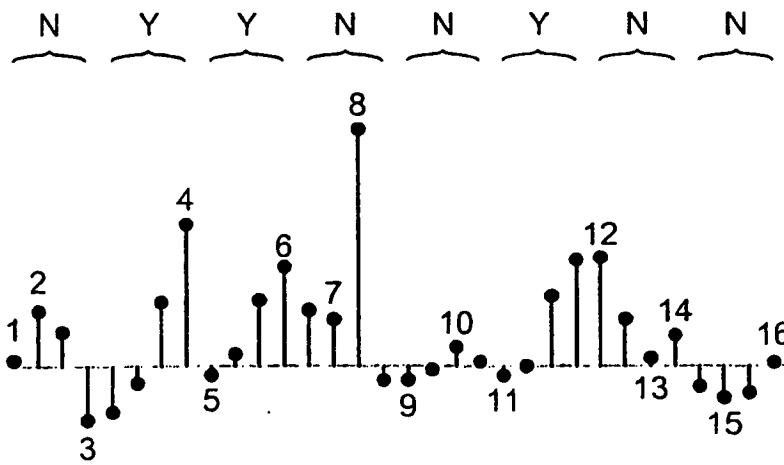


FIG. 10B

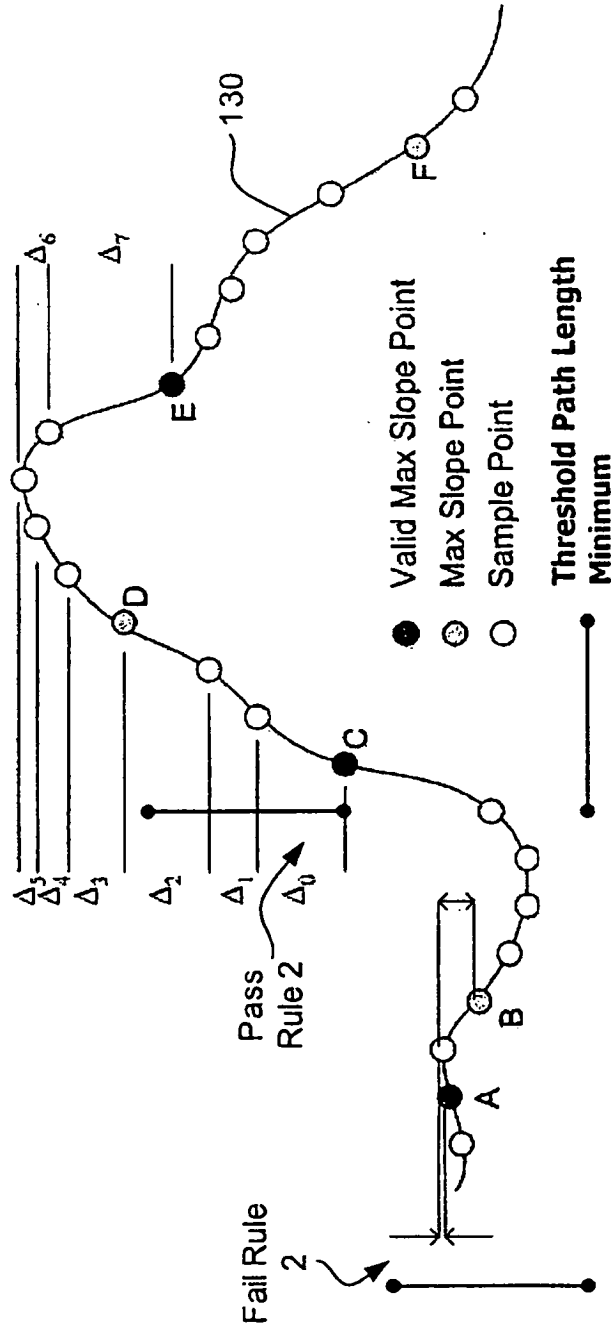


FIG. 11

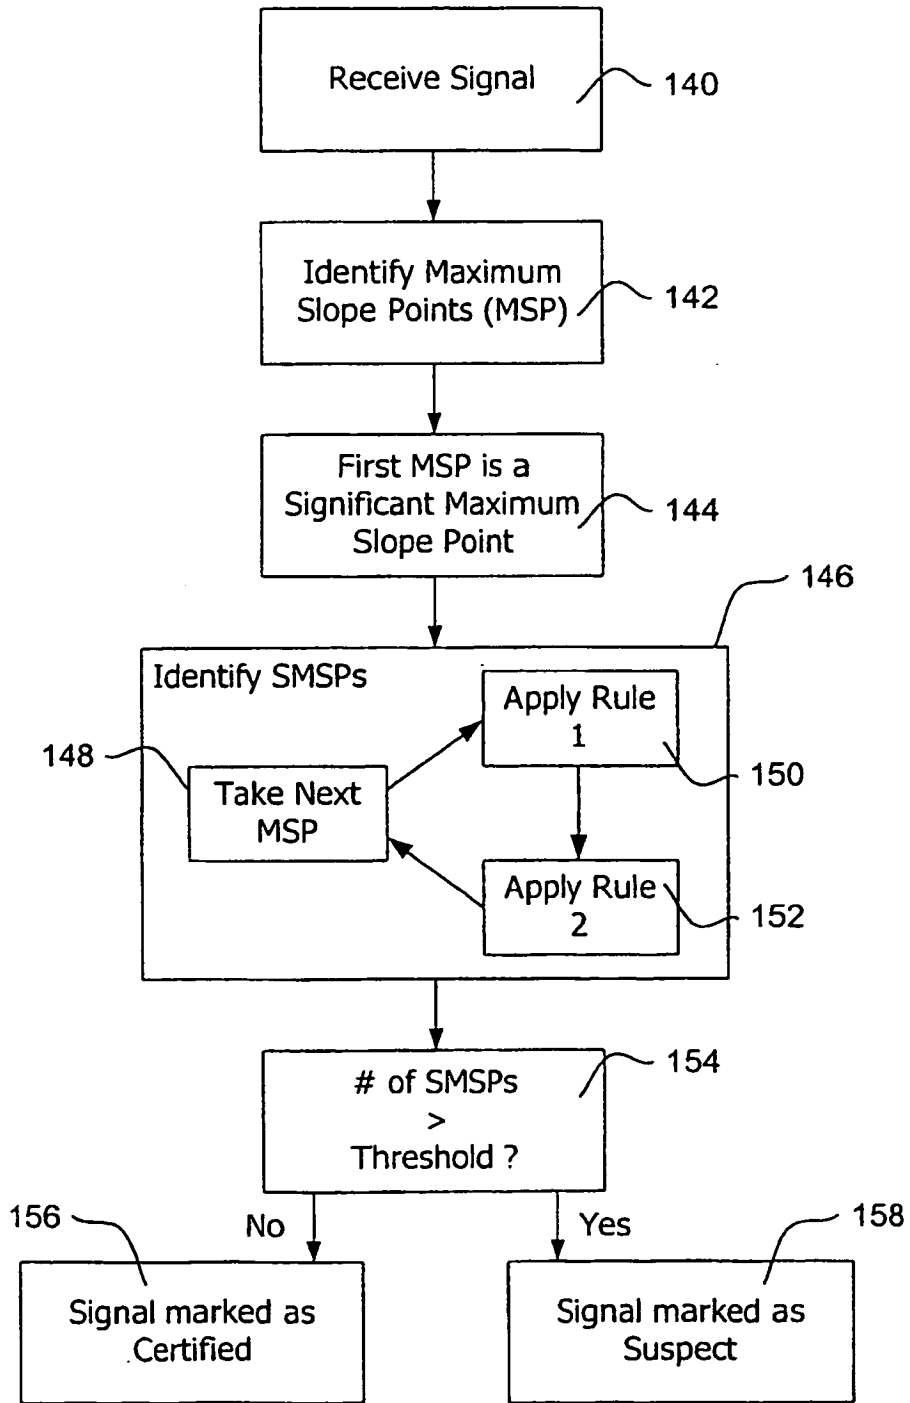


FIG. 12

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- GB 2034046 A [0010]
- EP 0554208 A2 [0010]
- US 6647292 B [0018]
- US 6721597 B [0018]
- US 6731978 B, Olson [0019]
- US 7330757 B [0029]

专利名称(译)	用于执行心脏波形评估的装置		
公开(公告)号	EP1631350B1	公开(公告)日	2012-08-08
申请号	EP2004753836	申请日	2004-06-02
[标]申请(专利权)人(译)	卡梅伦保健公司		
申请(专利权)人(译)	CAMERON HEALTH , INC.		
当前申请(专利权)人(译)	CAMERON HEALTH , INC.		
[标]发明人	PALREDDY SUREKHA WARREN JAY A PHILLIPS JAMES WILLIAM		
发明人	PALREDDY, SUREKHA WARREN, JAY, A. PHILLIPS, JAMES, WILLIAM		
IPC分类号	A61N1/365 A61B5/00 A61B5/042 A61B5/0452 A61N1/362 A61N1/368		
CPC分类号	A61N1/365 A61B5/0031 A61B5/0422 A61B5/04525 A61B5/7207 A61B5/7239 A61N1/3622 A61N1/368		
代理机构(译)	法思博事务所		
优先权	60/475279 2003-06-02 US 10/858598 2004-06-01 US		
其他公开文献	EP1631350A2		
外部链接	Espacenet		

摘要(译)

本发明涉及一种用于心律管理装置的传感结构。本发明的感测架构提供了用于通过心律管理设备认证检测到的事件的方法和装置。此外，通过利用增强的能力来仅精确地识别所需的那些感测事件，并防止使用标记为可疑的事件，本发明的感测架构可以更好地区分适合于设备治疗的节奏和不适合于设备治疗的节奏。

