



(11) **EP 2 040 608 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
25.03.2015 Bulletin 2015/13

(51) Int Cl.:
A61B 5/0476 ^(2006.01) **A61B 5/145** ^(2006.01)
A61B 5/00 ^(2006.01)

(21) Application number: **07729990.7**

(86) International application number:
PCT/EP2007/055628

(22) Date of filing: **07.06.2007**

(87) International publication number:
WO 2007/144307 (21.12.2007 Gazette 2007/51)

(54) **ANALYSIS OF EEG SIGNALS TO DETECT HYPOGLYCAEMIA**

ANALYSE VON EEG-SIGNALLEN ZUM NACHWEIS VON HYPOGLYKÄMIE

ANALYSE DE SIGNAUX EEG POUR DETECTER L'HYPOGLYCEMIE

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR

(56) References cited:
WO-A-02/069798 **WO-A-2005/037092**
US-A- 3 195 533 **US-A- 4 608 635**
US-A- 5 311 876 **US-A1- 2003 195 429**
US-A1- 2004 267 152 **US-B1- 6 572 542**

(30) Priority: **15.06.2006 GB 0611872**

(43) Date of publication of application:
01.04.2009 Bulletin 2009/14

(73) Proprietor: **Hypo-safe A/s**
5800 Nyborg (DK)

(72) Inventors:
• **BECK-NIELSEN, Henning**
DK-5800 Nyborg (DK)
• **MADSEN, Rasmus Elsborg**
DK-2920 Charlottenlund (DK)

(74) Representative: **Beck Greener**
Fulwood House
12 Fulwood Place
London WC1V 6HR (GB)

- **BJORGASS, M; ET AL.:** "Quantitative EEG during Controlled Hypoglycaemia in Diabetic and Non-diabetic Children" **DIABETIC MEDICINE**, vol. 15, no. 1, 1998, pages 30-37, XP002444890
- **JASPER, H. H.:** "Report of the Committee on methods of clinical examination in electroencephalography" **ELECTROENCEPHALOGRAPHY AND CLINICAL NEUROPHYSIOLOGY**, vol. 10, no. 2, 1958, pages 370-375, XP002445056
- **TUPOLA, S.; ET AL.:** "Abnormal electroencephalogram at diagnosis of insulin-dependent diabetes mellitus may predict severe symptoms of hypoglycemia in children" **JOURNAL OF PEDIATRICS**, vol. 133, no. 6, December 1998 (1998-12), pages 792-794, XP002444889

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 040 608 B1

Description

[0001] The invention relates to a method of predicting and warning of hypoglycaemic attacks for people such as but not limited to diabetics. Moreover the invention relates a device for prediction and warning of hypoglycaemic attacks for people such as but not limited to diabetics.

[0002] Hypoglycaemic attacks occur as a result of a too low blood sugar concentration, which is mostly a problem for diabetics, who are treated with insulin or other blood sugar regulating medical drugs. Others at risk include those having a genetic predisposition to having a low blood sugar. The attacks can be highly severe and often entail unconsciousness. The risk of an attack therefore often limits the possible activities of the people concerned, which furthermore decreases their quality of life. Attacks can be prevented in a simple way, e.g. by consuming appropriate food when glucose values become critical. The problem is however that many in the risk group cannot by themselves sense when their blood sugar concentration reaches a critically low level with risk of an attack. The number of people in the risk group is approximately 10 million.

[0003] There are known methods and devices for prediction of hypoglycaemic attacks.

[0004] In US patent No. 6,572,542 a method and a device are described, which among others have the purpose of warning of hypoglycaemic attacks. This uses a combination of EEG measurements to indicate an individual's blood glucose level and the individual's ECG (electrocardiographic) signals to indicate the rate of change of blood sugar concentration as inputs to an artificial neural network learning processor, from which is obtained a signal that is used for alerting the user or to control administration of a therapeutic material.

[0005] However, no specific method of obtaining or analysing EEG signals is described and nor are any results of practising the described methods given.

[0006] Gade J., Rosenfalck A. and Bendtson I., Meth Inform Med 1994; 33: 153-6 investigates the possibility of providing a patient hypoglycaemia alarm and describes the detection of EEG patterns related to nocturnal hypoglycaemia. EEG signals from bipolar EEG surface electrodes C4-A1 and C3-A2 are digitised offline and are divided into 2 second time segments. Amplitude and spectral content from these is fed to a Bayes probabilistic classifier of undisclosed type which is trained according to an unsupervised learning process. The rate of occurrence of events classified as indicative of hypoglycaemia is observed. It is concluded that inter-patient variability does not allow for the construction of a common learning set for all patients and that construction of a personal learning set will be required for all patients.

[0007] We have now found that in order to obtain sufficient specificity and sensitivity of detection of EEG changes indicative of the onset of hypoglycaemia, it is not sufficient to consider only the occurrence of such changes nor the rate at which they occur. Otherwise, sporadic EEG events consistent with hypoglycaemia or temporary bursts of such events can lead to a false alarm being triggered.

[0008] Accordingly, the present invention now provides a method for the analysis of EEG signals to detect features therein which are indicative of hypoglycaemia comprising:

- dividing EEG signals into a sequence of time segments,
- for each time segment determining whether a pattern of EEG signals is present which is indicative of hypoglycaemia and, where a pattern of EEG signals indicative of hypoglycaemia is determined to be present in a time segment, recording this as an event,
- integrating the number of events recorded during a selected number of preceding time segments which together constitute a selected time period, and
- determining that the EEG signals are indicative that hypoglycaemia is present based on said integration, for instance, when the said integrated number of events exceeds a preset threshold number and/or when there exists a threshold level of matching between a curve of said integration over time and a previously established ideal model of said curve indicative of hypoglycaemia.

Basing the determination on the integration avoids false positive results due to sporadic time segments containing events or sporadic clusters of such time segments. The determination is therefore made when a characteristic rising incidence of such events occurs.

[0009] Preferably, said integration is performed as a weighted integration in which events detected in time segments further back in time are given a lesser weighting than events detected in more recent time segments. Such a weighted integration may be performed using a linear weighting function or a sine-curve weighting function or other weighting functions.

[0010] Preferably, determination of whether a pattern of EEG signals is present in a time segment which is indicative of hypoglycaemia is performed by applying to said signals a previously trained Bayes classifier, a support vector machine (SVM), a relevance vector machine (RVM), a Gaussian process classifier, a classifier based on Fisher's discriminant, a boosted classifier, a naive Bayes classifier, a K-nearest neighbour classifier, a Binary Decision Tree, a Parzen Window classifier, or a neural network. A suitable Bayes classifier may be a Bayes Gaussian classifier.

[0011] Optionally, during a period of monitoring EEG signals there is carried out a re-estimation of the mean and covariance parameters of the Gaussian model over time. This may be used to compensate for drift in these parameters.

[0012] Preferably, said classifier is a quadratic Bayes Gaussian classifier.

[0013] The previously trained classifier applied to said signals is preferably a classifier trained by supervised learning, however an unsupervised learning trained classifier may be employed. A supervised Bayes classifier may use a Gaussian PDF (probability density function) as a model or a mixture of Gaussian PDF's as a model.

[0014] The raw EEG signals are preferably subjected to spectrum analysis to extract therefrom power averages in at least four frequency bands upon which is based the said determination of whether a pattern of EEG signals is present which is indicative of hypoglycaemia in a time segment of said signals. The at least five frequency bands preferably cover frequencies from 2Hz to 32Hz and suitable values for the bands include bands of approximately (2Hz-5Hz), (5Hz-8Hz), (8Hz-11Hz), (11Hz-14Hz) and (14Hz-32Hz), wherein all of the boundaries of said frequency bands are variable by up to 20%. The ideal number of bands and their respective coverage may vary from person to person and may be optimised for an individual.

[0015] Prior to said spectrum analysis, artefact or noise elements in said EEG signals are preferably identified and eliminated.

[0016] The EEG signals may be obtained from electrodes applied to the surface of the scalp, but in order to reduce noise and to obtain a more consistent output, the use of subcutaneously implanted electrodes is preferred. Electrodes may additionally or alternatively be inserted into the brain itself. The position of these will affect the content of the signals that is modulated by glycaemic status and also the amount of noise due to non-relevant signal generators such as motor activity.

[0017] Preferably, said EEG signals are obtained from one or more electrodes positioned within the area bounded by the FC3-FC1-C1-CP1-P1-PO3-P5-CP5-C5 standard EEG electrode positions and/or in an equivalent area around C4. Reference may be made to Figure 2 for an illustration of these positions.

[0018] More preferably, the electrodes are positioned within the area bounded by the FC3-FC1-C1-CP1-CP3-C5 positions and/or in the equivalent area around C4 and still more preferably within the area bounded by the FC3-C1-CP3-C5 positions and/or in the equivalent area around C4.

[0019] Thus, most preferably said EEG signals have been obtained from one or more electrodes positioned in at least approximately the C3 and/or C4, but electrodes at the P3 and/or P4 standard EEG electrode positions would be acceptable.

[0020] Preferably, said signals are measured with reference to signals obtained from a reference electrode positioned approximately on the frontal-occipital mid-line, e.g. in approximately the Cz or Pz standard EEG electrode position.

[0021] Optionally, one derives signals from a number of electrodes (suitably up to five) along the "line" T3,C5,C3,C1,Cz,C2,C4,C6,T4 or the line TP7,CP5,CP3,CP1,CPz,CP2,CP4,CP6,TP8 or the line T5,P5,P3,P1,Pz,P2,P4,P6,T6. Using more than two differential electrodes allows to use techniques such as Independent Component Analysis (ICA) to find artefact noise, and remove this noise from the EEG signals as discussed further below. The use of multiple electrode positions spaced along a straight or curved line facilitates the use of implanted electrodes as the conductors connecting thereto can all be led out in the same direction along a common path.

[0022] Preferably, the time period is adjusted to optimise the sensitivity and specificity of the determination that the obtained signals are indicative of hypoglycaemia for an individual from whom the signals originate. A similar individual optimisation may be carried out by adjustment also of the duration of the time segment or of the overlap of one time segment with the next, which may for instance be within the range of 0 to 50%. Time segments may also be spaced from each other with signals in between time segments being ignored.

[0023] EEG signals are optionally determined to be indicative of hypoglycaemia by establishing that a threshold level of matching between the curve of said integration over time and a previously established ideal model of said curve indicative of hypoglycaemia exists, wherein said matching is carried out by a mathematical convolution of the measured and ideal curves. Alternative pattern matching techniques are discussed below. The ideal curve used as the basis for the comparison may be a generic one applied to all users or may be individually determined based on observation of the shape of curve characteristic of a hypoglycaemic attack in that particular user.

[0024] In the methods exemplified below, each time segment is considered to contain an event characteristic of hypoglycaemia on the basis of features constituted by the power averages of each of the (typically five) frequency bands in that time segment for each electrode. These are the features operated on by the classifiers discussed. Whilst this has been found to be adequate, alternative methods may prove more robust to noise in the system. These may include splitting the signal into frequency bands by the use of filters matched to the characteristic form of the EEG signals in a hypoglycaemia event. Alternatively, one may use features found by mathematically convolving the actual EEG signal during the time period with an ideal form for the EEG signal in a hypoglycaemic episode. Alternatively, use can be made of features found from wavelet transformation of the measured curve or from singular value decomposition, or of features found by Independent Component Analysis or from a non-zero matrix factorisation (NMF) or other matrix factorisation or decomposition technique.

[0025] The method preferably includes activating an alarm upon determination that the EEG signals are indicative of hypoglycaemia. The alarm may take any form suitable to alert the user or a carer. In particular, it may be audible, visible, a mild electric shock, and/or a vibration alarm.

[0026] The invention includes apparatus for use in a method as described and comprising pre-programmed computation means comprising inputs for receiving EEG signals from EEG electrodes, and means for

- dividing said EEG signals into a sequence of time segments,
- for each time segment determining whether a pattern of EEG signals is present which is indicative of hypoglycaemia and, where a pattern of EEG signals indicative of hypoglycaemia is determined to be present in a time segment, recording this as an event,
- integrating the number of events recorded during a selected number of preceding time segments which together constitute a selected time period,
- determining that the EEG signals are indicative that hypoglycaemia is present based upon said integration, and
- providing an output indicating that said threshold number has been exceeded.

[0027] Said output preferably takes the form of an alarm as described above.

[0028] The apparatus may comprise one or more electrodes for positioning on a user, or actually in position on a user, from which to obtain such EEG signals.

[0029] The conditions for triggering the giving of an alarm may be differently set according to whether the user is going to be awake or asleep during the period of monitoring. EEG signals from an awake user on the one hand and EEG signals from a sleeping user on the other each present different complicating factors in distinguishing the EEG changes associated with hypoglycaemia from other features of the EEG. Thus, EEG signals from an awake user are likely to be contaminated with a higher level of artefact signals relating to motor functions. On the other hand, when the user is asleep, changes in the EEG caused by sleep will to some degree mimic the changes which would be due to hypoglycaemia, making the task of distinguishing the EEG changes due to hypoglycaemia more difficult. Thus, the awake/asleep status of the user may be used as an input to the computation in the device so as to have an effect on the threshold levels of the integration or the degree of matching of the integration curve to an ideal curve (or the shape of the ideal curve).

[0030] Other factors may also be included in determining the threshold levels of the integration or the degree of matching of the integration curve to an ideal curve (or the shape of the ideal curve). These may include, the time of day, the heart rate, the temperature as measured at the skin surface and other relevant inputs. However, it is preferred that ECG signals are not used as inputs to the apparatus or in the method of the invention. The determination of a hypoglycaemic condition will ordinarily be based exclusively on the EEG signals.

[0031] As a further aid to determining when hypoglycaemia is beginning, the integration threshold method describe above may be supplemented by matching the measured shape of the integration curve to a previously established characteristic ideal shape for the curve, which is indicative of hypoglycaemia. Such matching to the ideal curve may be carried out as a mathematical convolution of the measured curve with the ideal curve, or by template matching, or cross-correlation. Thus, for hypoglycaemia to be determined to be present and for an alarm signal to be triggered it may be required that the integration threshold should be reached or that a sufficient degree of match should exist between the integration curve and an ideal curve, or both. The invention includes a method of monitoring the glycaemic status of a user comprising, attaching or implanting electrodes to gather EEG signals containing information relating to glycaemic status, acquiring said EEG signals, and subjecting said signals to a method of analysis as described above.

[0032] The invention will be further illustrated and explained by the following description of preferred embodiments with reference to the accompanying drawings, in which:

Figure 1 shows schematically a person equipped with an example of apparatus according to the invention for detecting the onset of hypoglycaemia;

Figure 2 shows the electrode array of the apparatus of Figure 1 seen from above superimposed on a standard map of EEG electrode positions;

Figure 3 shows signals from 16 EEG channels marked with artefacts (lowest trace) identified by calculation of signal variance;

Figure 4 shows the same signals after removal of the major artefacts;

Figure 5 shows the result of Independent Component Analysis (ICA) performed on 16 channels of EEG signals following major artefact removal;

Figure 6 shows EEG signals further cleaned of artefacts identified by ICA;

Figure 7 shows results of the analysis of EEG signals from six individual volunteers in which events relevant to the occurrence of hypoglycaemia have been identified and integrated over a selected time period;

Figure 8 shows ROC curves for each volunteer based on the signal analysis for which results are shown in Figure 7; and

Figure 9 shows the effect of varying the selected time period on the integration results for one volunteer.

[0033] As shown in Figure 1, apparatus according to the invention may comprise an array of subcutaneous EEG electrodes 20, 22 (Fig 2) and 24, connected by implanted electrical connection wires 10 to an implanted signal processing/transmitting unit 14 positioned adjacent an externally worn signal processing/alarm unit 16.

[0034] Power may be provided from unit 16 to unit 14, for instance by magnetic induction, and unit 16 itself may be powered by conventional rechargeable batteries.

[0035] The array of electrodes 10 may comprise any desired number of electrodes. Also, although the illustrated apparatus uses implanted subcutaneous electrodes, skin surface electrodes may alternatively be used, or a combination of external and subcutaneously or intracranially implanted electrodes may be used. For convenience, it is desirable to reduce the number of electrodes to the minimum consistent with producing reliable results. Preferably therefore, as illustrated, the array consists of three electrodes arranged along a path defined by a set of electrical conductors which run parallel and closely adjacent to one another as seen in Figure 2. Here, two signal electrodes 20 and 22 are positioned in approximately the C3 and C4 positions respectively and a reference electrode 24 is positioned in the Cz position, referring here to the standard International 10-20 position mapping for EEG electrodes as described for instance in 'Primer of EEG with a Mini-Atlas', Rowan and Tolunsky (Butterworth Heinemann) Chapter 1, Figures 1-1 to 1-6, or the extended 10-20 system as described in 'Current Practice of Clinical Electroencephalography' third edition, Ebersole and Pedley Ed, Lippincott, Williams & Wilkiks pub, Chapter 4, pages 72- 74.

[0036] Whilst these positions are favoured, they are not critical and may be varied. For instance, any position within the area bounded by the FC3-FC1-C1-CP1-P1-PO3-P5-CP5-C5 positions (and similarly around C4), e.g. within the area bounded by FC3-FC1-C1-CP1-CP3-C5 positions (and similarly around C4) would be acceptable with in the preferred practice of the invention, especially in the area bounded by FC3-C1-CP3-C5 (and similarly around C4). Suitably alternative specific electrode positions would be P3 and P4. For the reference electrode, any position between Fz and POz would be preferred, especially between FCz and Pz.

[0037] As described in detail below, considerable amplification and computer processing of the raw EEG signals derived from the electrodes is necessary in the methods and apparatus of the invention. This may be conducted either in the implanted unit 14 or in the externally worn unit 16 or may be split between the units in any desired manner.

[0038] Amplification of the EEG electrode signals may be performed in a standard manner, e.g. by op-amp instrumentation amplifiers. The signals may be converted from analogue to digital in a known manner for further processing and analysis. The digitised signals may be segmented into time segments or epochs, suitably of from 0.5 to 2 seconds, one second being preferred. As explained above, the time segments may overlap so that data from the end of one time period is re-used in the next, or may be spaced leaving some data out. In the preferred apparatus, the 1 second time segments are sub-sampled to a frequency of 64Hz. Each segment consists of data from two differentially recorded channels (C4-Cz) and (C3-Cz), giving 128 bits of data in each segment.

[0039] The apparatus contains, either in the unit 14, or in the unit 16, or split between them, computation means for carrying out the following operations.

Artefact removal

[0040] The raw EEG signals contain signal elements deriving from brain activity modulated by glycaemic status but also noise or artefact signal elements relating to irrelevant matters, especially body movements, including eye movements. In one approach, time segments containing excessive noise/artefact signals are rejected prior to further signal analysis. In another approach, the data within time segments is corrected to exclude the artefact signals without losing the relevant signals. One may include either or both of these approaches in the handling of the signals.

[0041] Various methods may be employed for artefact removal. In one preferred method, the variance or sample variance of the signal (maximum value of the mean power for each EEG channel) in each time segment is evaluated. Time segments with a variance above a threshold level are rejected. The threshold may be set such that about 10% or 20% of the data is rejected.

[0042] A more subtle alternative which may be employed additionally to or instead of the above approach is to apply an algorithm to the EEG signals to identify artefact signal patterns and to remove them more specifically. An example

of such an algorithm follows that operates unsupervised and bases its whole analysis on the EEG signal itself. This kind of algorithm is mostly referred to as blind-source-separation (BSS) and independent-component-analysis (ICA). These algorithms have previously been used when analyzing EEG signals, to find EEG sources in the brain, but are not known to have been used previously for cleaning signals relating to hypoglycemia. ICA works well when there are many input dimensions (here EEG electrode signals), but not as well when using fewer electrodes. Accordingly, this approach will be favoured when more than just the C3 and C4 electrodes referred to above are employed. For instance, more electrodes may be provided on or close to the line from C3 to C4. An alternative approach where the number of electrodes is low (e.g. just C4, Cz, and C3) would be to use "sparse regression", a technique that assumes that there exists an underlying subspace of signal components that are used sparsely. Sparse regression is also sometimes referred to as: basis pursuit, atomic decomposition, and Sparse Component Analysis.

[0043] One option is to provide further electrodes for signal gathering, to employ ICA to identify and remove artefacts and then to base the detection of hypoglycaemia on the cleaned signals from a more limited set of the electrodes such as just C3, C4 and Cz. An example of this will be illustrated. Figure 3 shows EEG signals from 16 channels over 3000 seconds subjected to variance analysis to identify periods containing artefacts, mainly associated with eye movement. The bottom signal (Artefact) shows the time segments where artefacts are detected due to the high EEG signal variance. These parts of the EEG signal, constituting in this instance 20%, are removed. These large artefacts may be associated with major motor activity such as jaw movements. The 20% of the EEG signals that have been removed are determined by analysis of the EEG signal power histogram using a reject fraction of 0.2.

[0044] The remaining signals after removal of the artefacts identified in Figure 3 are shown in Figure 4. However, the signals are still contaminated to a degree with artefacts mainly related to more minor motor activity such as eye movements and these are further reduced by the use of ICA.

[0045] The artefact parts originating from subject eye movement are determined in this case by the use of a maximum likelihood independent component analysis (ICA) algorithm. The ICA algorithm finds 16 independent signal components from the 16 EEG signals. Three of these independent signal components are directly related to eye movement. The three components are removed by subtracting them from the original EEG signal, whereby none of the remaining EEG time slices are removed. Figure 5 shows the 16 independent components found in the EEG signals. The first three independent components are here directly related to eye movement. Components related to eye movement can be identified by consideration of the extent to which they appear in signals from frontal electrodes or by comparing signals obtained when the subject is asked to make a lot of eye movements or to blink frequently. After removing the three most active eye movement components, the EEG signals are sufficiently cleaned from artefacts, for the machine learning algorithms to be applied as described in the next section. Figure 6 shows the cleaned EEG signals. Traces from eye movement artefacts can still be spotted, but the signal is sufficiently clean for the machine learning algorithms to be applied.

Feature extraction

[0046] Following artefact removal, it is desirable to extract the information that is contained in separate frequency bands within the overall signals. We have found that it is preferable to use as many as five bands, each of 3Hz in width, as follows: 2-5Hz, 5-8Hz, 8-11Hz, 11-14Hz and 14Hz-32Hz.

[0047] Many other patterns of band division can be used of course. The general pattern observed in an EEG upon the onset of hypoglycaemia is an increase in the power present in the delta band (1-4Hz) but more especially in the theta band (4-8Hz) and a lowering of the frequency of the component in the alpha band (8-12Hz) at which most power is present. These effects are particularly noticeable in EEG signals from the C3 and C4 regions.

[0048] Previous work has often concentrated exclusively on the information in the theta and alpha wave bands, but we have found it much better to sub-divide the frequencies in a finer manner. Also, better results are obtained by leaving out frequencies below 2Hz. However, an alternative division of the frequencies with which we have produced good results is 0.8Hz-1.3Hz, 1.3Hz-2.2Hz, 2.2Hz-3.6Hz, 3.6-5.9Hz, 5.9Hz-9.5Hz, 9.5Hz-15.6Hz, 15.6Hz-25.6Hz and 25.6Hz-32Hz. Good results can also be achieved at least in some cases by using fewer bands, e.g. 3.6-5.9Hz and 5.9-9.8Hz. The limits of each band indicated above are only exemplary and can freely be changed, e.g. by $\pm 10\%$ to 20% .

[0049] The above described division of the signals into from 5 to 8 frequency bins in each of the two channels C3-Cz and C4-Cz enhances the classification results obtained in the next stage when compared to the traditional division of frequencies into alpha, beta, theta and delta bands. However, using only two bands can result in a model that is so general that it can be used as an inter-subject model, rather than requiring the training of a model for each individual. One can use fewer bands and a more generally applicable model for more 'typical' individuals and use more bands and an individually trained model for users who do not suit the general model.

[0050] One can also include in the data the value of the frequency in the range 2-12Hz at which maximal power is contained, as this we have found to decrease during hypoglycaemia.

Event detection

[0051] We shall describe the extraction from the frequency filtered signals of events signalling hypoglycaemia using in one case a quadratic Bayes Gaussian Classifier (QBGC) and in the other case a neural network. It will be appreciated that one may classify the information in the time sliced, frequency divided signals using many other classifiers of known types as described above.

Software for carrying out classification to identify relevant events may be obtained from a number of sources, for instance <http://www.ll.mit.edu/IST/lnknet/>.

[0052] In our QBGC, The classification of the EEG signals is partly based on the quadratic measure shown in Equation 1, which defines the Bayesian normal distributed classifier, with a diagonal covariance matrix, a simplification of the full quadratic classifier. It should be noted that all the parameters in the equation are vectors.

$$\text{Quadratic Measure} = \frac{(x - \mu_{pos})^2}{\sigma_{pos}^2} - \frac{(x - \mu_{neu})^2}{\sigma_{neu}^2}$$

[0053] This Quadratic Measure is used for simple discrimination between hypoglycaemic and neutral events. Each 1 second of data (or other selected length of time segment or epoch) is classified in a binary manner as either hypoglycaemic or neutral. The neutral events are when the signals indicative of an hypoglycaemic event are not present. The variables (x , μ , and σ) all are vectors of dimension (channels \times features per channel). The 'features' here are the total or average power within each band in each time segment for each channel.

[0054] In the quadratic measure, all the features in the channels are all contributing equally to the measure. The good and bad (relevant and irrelevant) features are therefore represented equally when using the quadratic measure for classification. To get a better weighting of the features, we can instead use a neural network based measure, where the features are weighted according to their ability to discriminate between the hypoglycaemic and neutral events.

[0055] A neural network classifier finds the best combination of the inputs, where the quadratic classifier used an averaged combination of the inputs.

[0056] An example of a suitable artificial neural network is one that is a regularized two layer feed-forward neural network with a hyperbolic tangent function for the hidden layer and a logistic sigmoid function for the output layer. The weights may be optimized using the cross-entropy error function augmented with a Gaussian prior over the weights. Suitably this may be a 7-10 hidden units network. More hidden units can result in overtraining and less units may give to little flexibility. The optimal number of hidden units is dependent on the amount of training data, meaning that using slightly more units might give better results if more training examples are available.

[0057] The Bayes classifier or the neural network is trained using supervised learning. Events indicative of hypoglycaemia are manually marked in signals obtained from an individual. The markings are done by experts in the use of EEG who visually detect what they consider to be relevant EEG signal patterns. Some hundreds of time segments of data are used for training and within these there must be at least one representing a hypoglycaemic event.

[0058] The trained classifier is then used in real time to classify the digitised, cleaned and feature extracted signals from the EEG electrodes.

Determination of the onset of hypoglycaemia

[0059] At intervals, events will occur that are classified as hypoglycaemic amongst a stream of events classified as neutral. In order to form a sound basis for judging that a real hypoglycaemic condition is developing however, with adequate specificity and sensitivity, it is not sufficient to rely on the occurrence of one such classified event nor even to determine when the rate at which such events occur exceeds some threshold level. Such events may be detected sporadically and may come in clusters at a high rate for a period, even when no actual hypoglycaemic condition exists.

[0060] Accordingly, according to the invention, the apparatus integrates the detected events over a selected time period. Events cease to be counted in the integration when a sufficient time has passed since they occurred. According to a preferred practice of the invention, as events recede in time, they are given a decreasing weighting in the integration. Suitably the weighting may be according to a sine function, e.g. according to the equation:

$$\text{Weight} = \sin\left(\frac{\pi \times T_d}{600}\right)$$

where T_d is the time in seconds since the classified hypoglycaemic event happened, where only events within the last

300 seconds are considered. More generally, '600' is replaced by $2xT_p$ where T_p is the selected time period.

[0061] Alternatively, a linear weighting reducing from one to zero over T_p may be employed.

[0062] These schemes treat events classified as hypoglycaemic as being of more predictive value if they are recent than if they happened some time ago.

[0063] A more complex weighting scheme may be employed in which the weighting given to events further in the past is decreased if the rate of events occurring at that time is higher. For instance, an event that occurred three minutes ago could be given a weighting of 1.0 if up to that time the integrated number of events is only 1, but a decreased weighting on a continuous sliding scale if the integrated number of events up to then is higher, for instance a weighting of 0.66 if the integrated number of events up to then is 2 and 0.5 if the integrated number of events up to then is 3. This will lead to a penalisation of the integration function when events do not follow the pattern that genuinely signals hypoglycaemia, where the rate of occurrence of events characteristically increases in a roughly exponential manner.

[0064] Examples of the effect of the use of the QBGC and the integration of events are seen in Figures 7 and 8. Figure 7 shows results obtained for six individuals identified by anonymised initials AP, AS, BL, EK, GL and HY. Data was gathered for each volunteer over a period during which the blood glucose level was caused to fall. Blood glucose measurements are plotted in the upper panel of each volunteer's results. Here, in a simulation of the operation of the invention, the classifier for each individual has been trained on one half of the available data divided into nonoverlapping 1 second time segments for four 3Hz wide bands from 2Hz upwards plus a 14Hz-32Hz band and has then been used to classify the remaining half of the data offline. Integration curves are plotted of events within a 600 second time period using the sine weighting described above. The effect of setting a 5 event threshold is indicated. Due to the weighting process, the threshold could of course be set to a non-integral value. The solid curves show the output of the classifier and the dotted integration curves show results based on manual marking.

[0065] In Figure 8 are shown ROC curves for each volunteer. A high figure (close to 1.0) for the area under the curve indicates a better result, 0.5 being effectively the worst possible outcome.

[0066] It can be seen that for each volunteer the general shape of the integration curve is similar. Hypoglycaemia is indicated by a rising frequency of the occurrence of events giving rise to integration curves that rise in a roughly exponential manner. The threshold value of 5 events is crossed in time for an alarm given at that point to allow a user sufficient time to take action to raise the blood sugar before hypoglycaemia renders them not competent to do so.

[0067] It may be observed however that the integration curve for user HY shows a comparatively gradual rise. The effect on this of adjusting the selected time period for the integration is shown in Figure 9. Here, the following integration lengths (selected time periods) have been used: 300, 600, and 900 seconds. When comparing the 300 seconds integration (upper left) with the 600 seconds integration (upper right) and the 900 seconds integration (lower left), we see that the longer integration period has produced a curve that looks more similar to the curves for the other 5 subjects as seen in Figure 7.

[0068] Many variations of the apparatus as specifically described may be made within the scope of the invention. For instance, the computation means need not be worn by the user. Especially for use by the bed bound or at night, the computation means may be contained in a separate (e.g. bedside) unit receiving the EEG signals in an unprocessed or partially processed form.

[0069] The signal processing and alarm functions can all be accommodated within the implanted unit 14, and that battery power for that may be either rechargeable from an external source of may be of the non-rechargeable type. The alarm signals may be progressively increased as long as an alarm condition is continuously detected. Should the apparatus enter into a state in which it is unable to provide accurate monitoring of the user's glycaemic status, it may provide a second form of alarm to notify the user of this.

[0070] Rather than, or in addition to, an alarm, the apparatus described above for determining the onset of hypoglycaemia may be interlinked with apparatus for administering a blood sugar control substance. For instance, it may be interlinked with an insulin pump to prevent action of the insulin pump when hypoglycaemia is detected, should the insulin pump and its own blood sugar measuring device be malfunctioning.

[0071] In this specification, unless expressly otherwise indicated, the word 'or' is used in the sense of an operator that returns a true value when either or both of the stated conditions is met, as opposed to the operator 'exclusive or' which requires that only one of the conditions is met. The word 'comprising' is used in the sense of 'including' rather than in to mean 'consisting of'.

Claims

1. A method for the analysis of EEG signals to detect features therein which are indicative of hypoglycaemia comprising:
 - dividing EEG signals into a sequence of time segments,
 - for each time segment determining whether a pattern of EEG signals is present which is indicative of hypogly-

caemia and, where a pattern of EEG signals indicative of hypoglycaemia is determined to be present in a time segment, recording this as an event,

- integrating the number of events recorded during a selected number of preceding time segments which together constitute a selected time period, and

- determining that the EEG signals are indicative that hypoglycaemia is present based on said integration.

2. A method as claimed in claim 1, wherein it is determined that the EEG signals are indicative that hypoglycaemia is present when the said integrated number of events exceeds a preset threshold number and/or when there exists a threshold level of matching between a curve of said integration over time and a previously established ideal model of said curve indicative of hypoglycaemia.

3. A method as claimed in claim 1, wherein said integration is performed as a weighted integration in which events detected in time segments further back in time are given a lesser weighting than events detected in more recent time segments.

4. A method as claimed in any preceding claim, wherein determination of whether a pattern of EEG signals is present in a time segment which is indicative of hypoglycaemia is performed by applying to said signals a previously trained Bayes classifier, a support vector machine (SVM), a relevance vector machine (RVM), a Gaussian process classifier, a classifier based on Fisher's discriminant, a boosted classifier, a naive Bayes classifier, a K-nearest neighbour classifier, a Binary Decision Tree, a Parzen Window classifier, or a neural network.

5. A method as claimed in claim 4, wherein during a period of monitoring EEG signals there is carried out a re-estimation of the mean and covariance parameters of the Gaussian model over time.

6. A method as claimed in any preceding claim, wherein raw EEG signals are subjected to spectrum analysis to extract therefrom power averages in at least four frequency bands upon which is based the said determination of whether a pattern of EEG signals is present which is indicative of hypoglycaemia in a time segment of said signals.

7. A method as claimed in claim 6, wherein said at least four frequency bands cover frequencies from 2Hz to and 32Hz said frequency bands include bands of approximately (2Hz-5Hz), (5Hz-8Hz), (8Hz-11Hz), (11Hz-14Hz), and (14Hz-32Hz), wherein all of the boundaries of said frequency bands are variable by up to 20%.

8. A method as claimed in any preceding claim, wherein said EEG signals have been obtained from one or more electrodes positioned within the area bounded the FC3-C1-CP3-C5 positions and/or in the equivalent area around C4.

9. A method as claimed in claim 8, wherein said EEG signals have been obtained from one or more electrodes positioned in at least approximately the C3 and/or C4 or P3 and/or P4 standard EEG electrode positions.

10. A method as claimed in claim 8 or claim 9, wherein said EEG signals are measured with respect to signals obtained from a reference electrode in approximately the Cz or Pz standard EEG electrode position.

11. A method as claimed in any preceding claim, wherein EEG signals are determined to be indicative of hypoglycaemia by establishing that a threshold level of matching between the curve of said integration over time and a previously established ideal model of said curve indicative of hypoglycaemia exists, wherein said matching is carried out by a mathematical convolution of the measured and ideal curves.

12. A method as claimed in any preceding claim, further comprising activating an alarm upon determination that the EEG signals are indicative of hypoglycaemia.

13. Apparatus for use in a method as claimed in any preceding claim and comprising pre-programmed computation means comprising inputs for receiving EEG signals from EEG electrodes, and means for

- dividing said EEG signals into a sequence of time segments,

- for each time segment determining whether a pattern of EEG signals is present which is indicative of hypoglycaemia and, where a pattern of EEG signals indicative of hypoglycaemia is determined to be present in a time segment, recording this as an event,

- integrating the number of events recorded during a selected number of preceding time segments which together constitute a selected time period,

- determining that the EEG signals are indicative that hypoglycaemia is present when the said integrated number of events exceeds a preset threshold number, and
- providing an output indicating that said threshold number has been exceeded.

- 5 **14.** Apparatus as claimed in claim 13, wherein said output takes the form of an alarm.
- 15.** Apparatus as claimed in claim 13 or claim 14, further comprising one or more electrodes for positioning on a user to receive EEG signals.

10

Patentansprüche

- 15 **1.** Verfahren zur Analyse von EEG-Signalen zur Erkennung von darin enthaltenen Merkmalen, die auf Hypoglykämie hinweisen, Folgendes umfassend:

15

- Einteilung der EEG-Signale in eine Reihe von Zeitsegmenten,
- Feststellung für jedes Zeitsegment, ob ein Muster an EEG-Signalen vorhanden ist, das auf Hypoglykämie hinweist, und, wenn in einem Zeitsegment das Vorhandensein eines Musters an EEG-Signalen, das auf Hypoglykämie hinweist, festgestellt wird, die Aufzeichnung dieser Feststellung als Ereignis,
- 20 - Integration der während einer ausgewählten Anzahl an vorhergehenden Zeitsegmenten, die zusammen einen ausgewählten Zeitraum ergeben, aufgezeichneten Anzahl an Ereignissen, und
- Feststellung, dass die EEG-Signale basierend auf der besagten Integration auf eine vorhandene Hypoglykämie hinweisen.

25

- 2.** Verfahren nach Anspruch 1, wobei festgestellt wird, dass die EEG-Signale auf das Vorhandensein von Hypoglykämie hinweisen, wenn die besagte integrierte Anzahl an Ereignissen einen vorher festgelegten Schwellenwert übersteigt und / oder wenn ein Schwellenwert an Übereinstimmung zwischen einer Kurve der besagten Integration im Laufe der Zeit und einem zuvor festgelegten Idealmodell der besagten Kurve, die auf Hypoglykämie hinweist, vorhanden ist.

30

- 3.** Verfahren nach Anspruch 1, wobei die besagte Integration als gewichtete Integration durchgeführt wird, bei der Ereignisse, die in Zeitsegmenten festgestellt wurden, die zeitlich weiter zurückliegen, weniger schwer gewichtet werden als Ereignisse, die in jüngeren Zeitsegmenten festgestellt wurden.

35

- 4.** Verfahren nach allen vorhergehenden Ansprüchen, wobei die Feststellung, ob ein Muster an EEG-Signalen in einem Zeitsegment vorhanden ist, das auf Hypoglykämie hinweist, dadurch erfolgt, dass für die besagten Signale ein zuvor trainierter Bayes-Klassifikator, eine Support-Vektor-Maschine (SVM), eine Relevanz-Vektor-Maschine (RVM), ein Gauß-Prozess-Klassifikator, ein Klassifikator basierend auf der Fisher-Diskriminante, ein verstärkter Klassifikator, ein naiver Bayes-Klassifikator, ein K-Nächster-Nachbar-Klassifikator, ein binärer Entscheidungsbaum, ein Parzen-Fenster-Klassifikator oder ein neuronales Netz angewandt wird.

40

- 5.** Verfahren nach Anspruch 4, wobei während eines Zeitraums der Beobachtung der EEG-Signale eine Neueinschätzung der Mittelwertparameter und der Kovarianzparameter des Gauß-Modells im Laufe der Zeit erfolgt.

45

- 6.** Verfahren nach allen vorhergehenden Ansprüchen, wobei EEG-Rohsignale einer Spektralanalyse unterzogen werden, um davon Leistungsmittelwerte in mindestens vier Frequenzbändern zu extrahieren, worauf die besagte Feststellung basiert, ob ein Muster an EEG-Signalen vorhanden ist, das auf Hypoglykämie in einem Zeitsegment der besagten Signale hinweist.

50

- 7.** Verfahren nach Anspruch 6, wobei die besagten mindestens vier Frequenzbänder Frequenzen von 2 Hz bis 32 Hz abdecken und die besagten Frequenzbänder Bänder mit ca. (2 Hz - 5 Hz), (5 Hz - 8 Hz), (8 Hz - 11 Hz), (11 Hz - 14 Hz) und (14 Hz - 32 Hz) umfassen, wobei alle Grenzen der besagten Frequenzbänder bis zu 20 % variabel sind.

55

- 8.** Verfahren nach allen vorhergehenden Ansprüchen, wobei die besagten EEG-Signale von einer Elektrode oder mehreren Elektroden erhalten wurden, die innerhalb des durch die Positionen FC3-C1-CP3-C5 abgegrenzten Bereichs und / oder im äquivalenten Bereich um C4 positioniert wurden.

- 9.** Verfahren nach Anspruch 8, wobei die besagten EEG-Signale von einer Elektrode oder mehreren Elektroden erhalten wurden, die mindestens ungefähr in den standardmäßigen EEG-Elektrodenpositionen C3 und / oder C4 oder P3

und / oder P4 positioniert wurden.

10. Verfahren nach Anspruch 8 oder 9, wobei die besagten EEG-Signale in Bezug auf von einer Referenzelektrode in ungefähr der standardmäßigen EEG-Elektrodenposition Cz oder Pz erhaltene Signale gemessen werden.

11. Verfahren nach allen vorhergehenden Ansprüchen, wobei EEG-Signale auf Hypoglykämie hinweisen, indem festgelegt wird, dass ein Schwellenwert an Übereinstimmung zwischen der Kurve der besagten Integration im Laufe der Zeit und einem zuvor festgelegten Idealmodell der besagten Kurve, die auf Hypoglykämie hinweist, vorhanden ist, wobei die besagte Übereinstimmung von einer mathematischen Faltung der gemessenen Kurven und der Idealkurven durchgeführt wird.

12. Verfahren nach allen vorhergehenden Ansprüchen, weiter umfassend die Aktivierung eines Alarms bei Feststellung, dass die EEG-Signale auf Hypoglykämie hinweisen.

13. Gerät zur Nutzung für ein Verfahren nach allen vorhergehenden Ansprüchen und Folgendes umfassend: vorprogrammierte Berechnungseinrichtungen, umfassend Eingaben zum Empfang von EEG-Signalen von EEG-Elektroden und Einrichtungen für Folgendes:

- die Einteilung der besagten EEG-Signale in eine Reihe von Zeitsegmenten,
- für jedes Zeitsegment die Feststellung, ob ein Muster an EEG-Signalen vorhanden ist, das auf Hypoglykämie hinweist, und, wenn in einem Zeitsegment ein Muster an EEG-Signalen, das auf Hypoglykämie hinweist, vorhanden ist, dessen Aufzeichnung als Ereignis,
- die Integration der Anzahl an während einer festgelegten Anzahl an vorhergehenden Zeitsegmenten, die zusammen einen ausgewählten Zeitraum ergeben, aufgezeichneten Ereignissen,
- die Feststellung, dass die EEG-Signale auf Hypoglykämie hinweisen, wenn die besagte integrierte Anzahl an Ereignissen einen vorher festgelegten Schwellenwert übersteigt, und eine Ausgabe, die anzeigt, dass der besagte Schwellenwert überschritten wurde.

14. Gerät nach Anspruch 13, wobei die besagte Ausgabe in Form eines Alarms erfolgt.

15. Gerät nach Anspruch 13 oder Anspruch 14, weiter umfassend eine Elektrode oder mehrere Elektroden zur Positionierung an einem Nutzer zum Empfang von EEG-Signalen.

Revendications

1. Procédé d'analyse des signaux EEG pour y détecter les caractéristiques indicatifs d'une hypoglycémie comprenant les phases suivantes:

- division des signaux EEG en une séquence de segments temporels,
- détermination pour chaque segment temporel de la présence ou non d'un schéma de signaux EEG indiquant une hypoglycémie et, si l'on détermine la présence d'un schéma de signaux EEG indicatif d'hypoglycémie dans un segment temporel, enregistrement de celui-ci comme événement,
- intégration du nombre d'événement enregistrés pendant un nombre sélectionné de segments temporels précédents qui constituent ensemble une période de temps sélectionnée, et
- détermination que les signaux EEG indiquent la présence d'une hypoglycémie sur la base de ladite intégration.

2. Procédé selon la revendication 1, où l'on détermine que les signaux EEG indiquent la présence d'une hypoglycémie lorsque ledit nombre intégré d'événements dépasse un nombre seuil prédéfini et/ou s'il existe un niveau seuil d'appariement entre une courbe de ladite intégration dans le temps et un modèle idéal établi au préalable de ladite courbe indicative d'hypoglycémie.

3. Procédé selon la revendication 1, où ladite intégration prend la forme d'une d'intégration pondérée dans laquelle les événements détectés dans des segments temporels plus éloignés dans le temps se voient affecter une pondération moindre que les événements détectés dans des segments temporels plus récents.

4. Procédé selon l'une quelconque des revendications précédentes, où la détermination de présence d'un schéma de signaux EEG dans un segment temporel indiquant une hypoglycémie, est réalisée en appliquant auxdits signaux

EP 2 040 608 B1

un classificateur Bayes préalablement confirmé, une machine à vecteurs de support (acronyme anglais SVM) une machine à vecteurs de pertinence (acronyme anglais RVM), un classificateur de processus gaussien, un classificateur fondé sur le discriminant de Fisher, un classificateur renforcé, un classificateur Bayes naïf, un classificateur des K plus proches voisins, un arbre de décision binaire, un classificateur de Parzen Window ou un réseau neural.

5

5. Procédé selon la revendication 4, où l'on réalise une nouvelle estimation des paramètres de moyenne et de covariance du modèle gaussien dans le temps, et ce pendant une période de surveillance des signaux EEG.

10

6. Procédé selon l'une quelconque des revendications précédentes, où l'on soumet les signaux EEG bruts à une analyse spectrale pour en extraire des moyennes de puissance sur au moins quatre bandes de fréquence, analyse sur laquelle se fonde la détermination de la présence d'un schéma de signaux EEG indiquant une hypoglycémie dans un segment temporel desdits signaux.

15

7. Procédé selon la revendication 6, où lesdites au moins quatre bandes de fréquence recouvrent des fréquences allant de 2 Hz à 32 Hz, lesdites bandes de fréquence comprenant des bandes d'environ (2Hz-5Hz), (5Hz-8Hz), (8Hz-11Hz), (11Hz-14Hz) et (14Hz-32Hz), où toutes les limites desdites bandes de fréquence sont variables dans une proportion maximale de 20%.

20

8. Procédé selon l'une quelconque des revendications précédentes, où lesdits signaux EEG sont obtenus grâce à une ou plusieurs électrodes positionnées dans la zone reliée aux positions FC3-C1-CP3-C5 et/ou dans la zone équivalente entourant C4.

25

9. Procédé selon la revendication 8, où lesdits signaux EEG sont obtenus grâce à une ou plusieurs électrodes positionnées au moins aux positions d'électrodes EEG standards C3 et/C4 ou P3 et/ou P4 environ.

30

10. Procédé selon la revendication 8 ou la revendication 9, où l'on mesure les signaux EEG par rapport aux signaux obtenus à partir d'une électrode de référence en gros dans la position d'électrode EEG standard Cz ou Pz.

35

11. Procédé selon l'une quelconque des revendications précédentes, où les signaux EEG sont déterminés comme indicatifs de l'hypoglycémie en établissant qu'il existe un niveau seuil d'appariement entre la courbe de ladite intégration dans le temps et un modèle idéal établi au préalable de ladite courbe indicative d'hypoglycémie, où ledit appariement est réalisé par une convolution mathématique de la courbe mesurée et de la courbe idéale.

40

12. Procédé selon l'une quelconque des revendications précédentes, consistant en outre à déclencher une alarme lorsque l'on détermine que les signaux EEG sont indicatifs de l'hypoglycémie.

45

13. Appareil pour utilisation dans un procédé selon l'une quelconque des revendications précédentes et comprenant des moyens informatiques préprogrammés intégrant des entrées permettant de recevoir des signaux EEG à partir d'électrodes EEG, et des moyens

50

- de division des signaux EEG en une séquence de segments temporels,
- de détermination pour chaque segment temporel de la présence ou non d'un schéma de signaux EEG indiquant une hypoglycémie et, si l'on détermine la présence d'un schéma de signaux EEG indicatif d'hypoglycémie dans un segment temporel, enregistrement de celui-ci comme événement,
- d'intégration du nombre d'événement enregistrés pendant un nombre sélectionné de segments temporels précédents qui constituent ensemble une période de temps sélectionnée,
- de détermination que les signaux EEG indiquent la présence d'une hypoglycémie lorsque ledit nombre intégré d'événements dépasse un nombre seuil prédéfini, et
- de fourniture d'une sortie indiquant un dépassement dudit nombre seuil.

55

14. Appareil selon la revendication 13, où ladite sortie prend la forme d'une alarme.

15. Appareil selon la revendication 13 ou la revendication 14, comprenant en outre une ou plusieurs électrodes disposées sur un utilisateur recevant les signaux EEG.

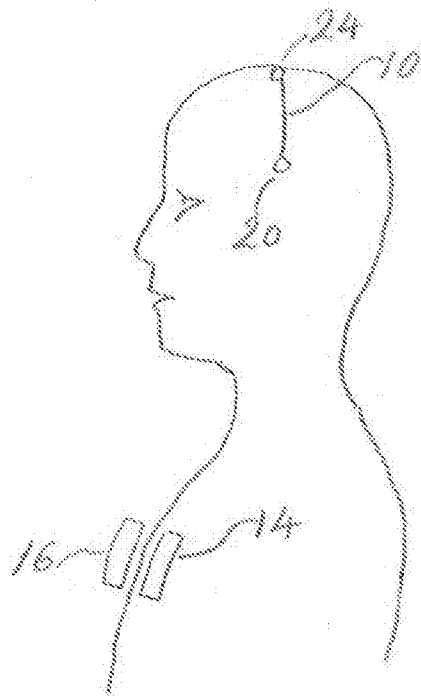


Figure 1

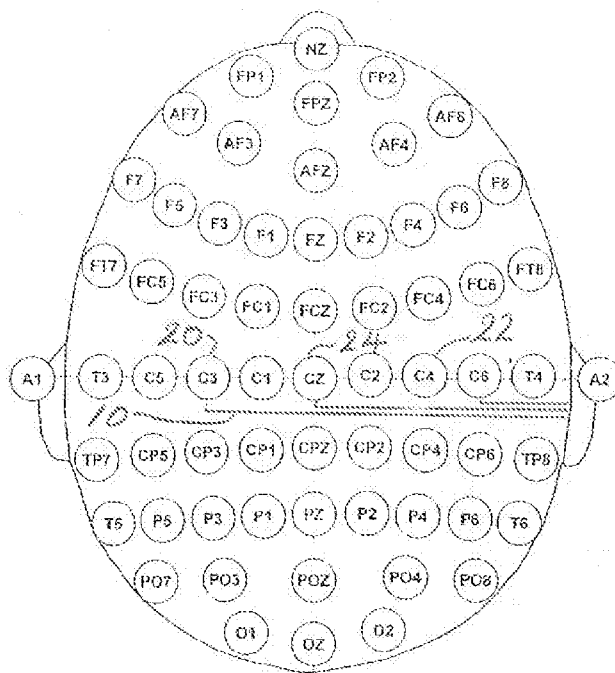


Figure 2

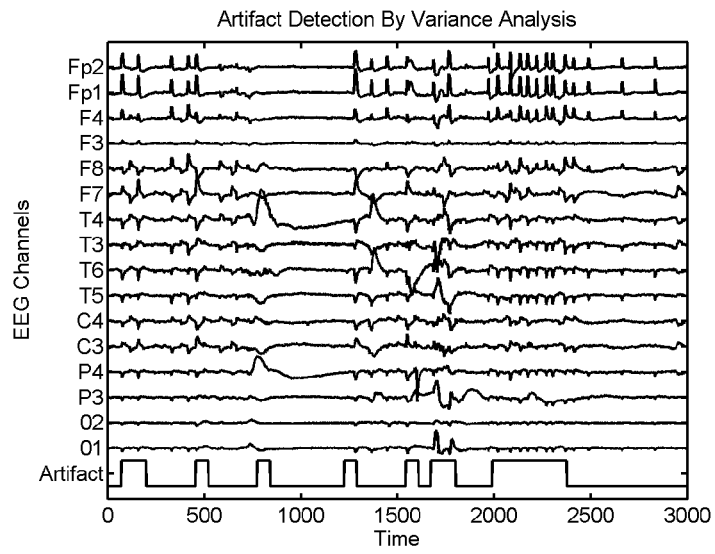


Figure 3

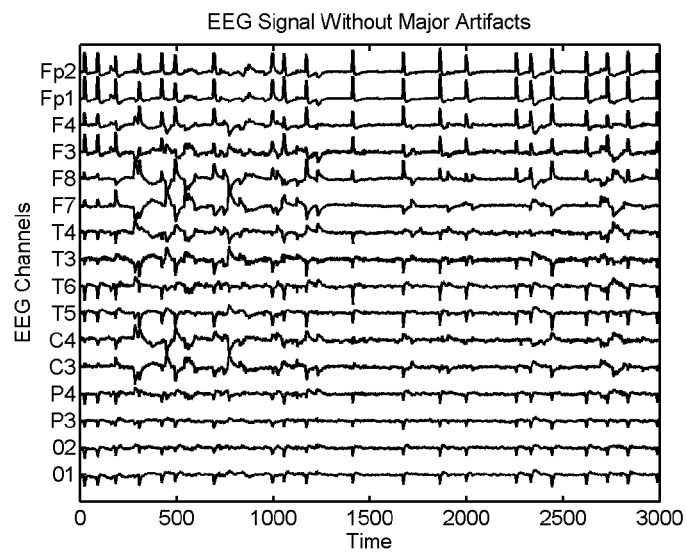


Figure 4

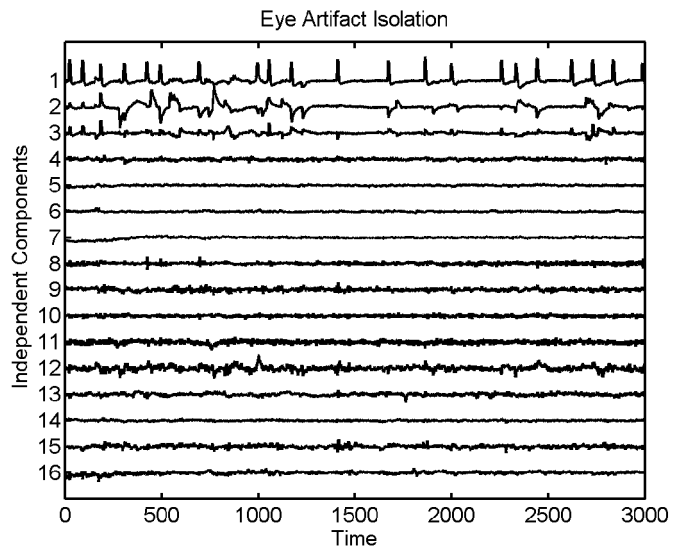


Figure 5

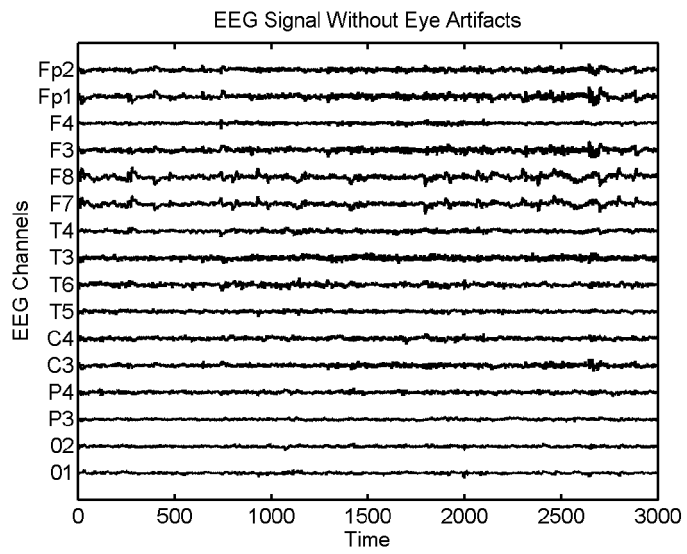


Figure 6

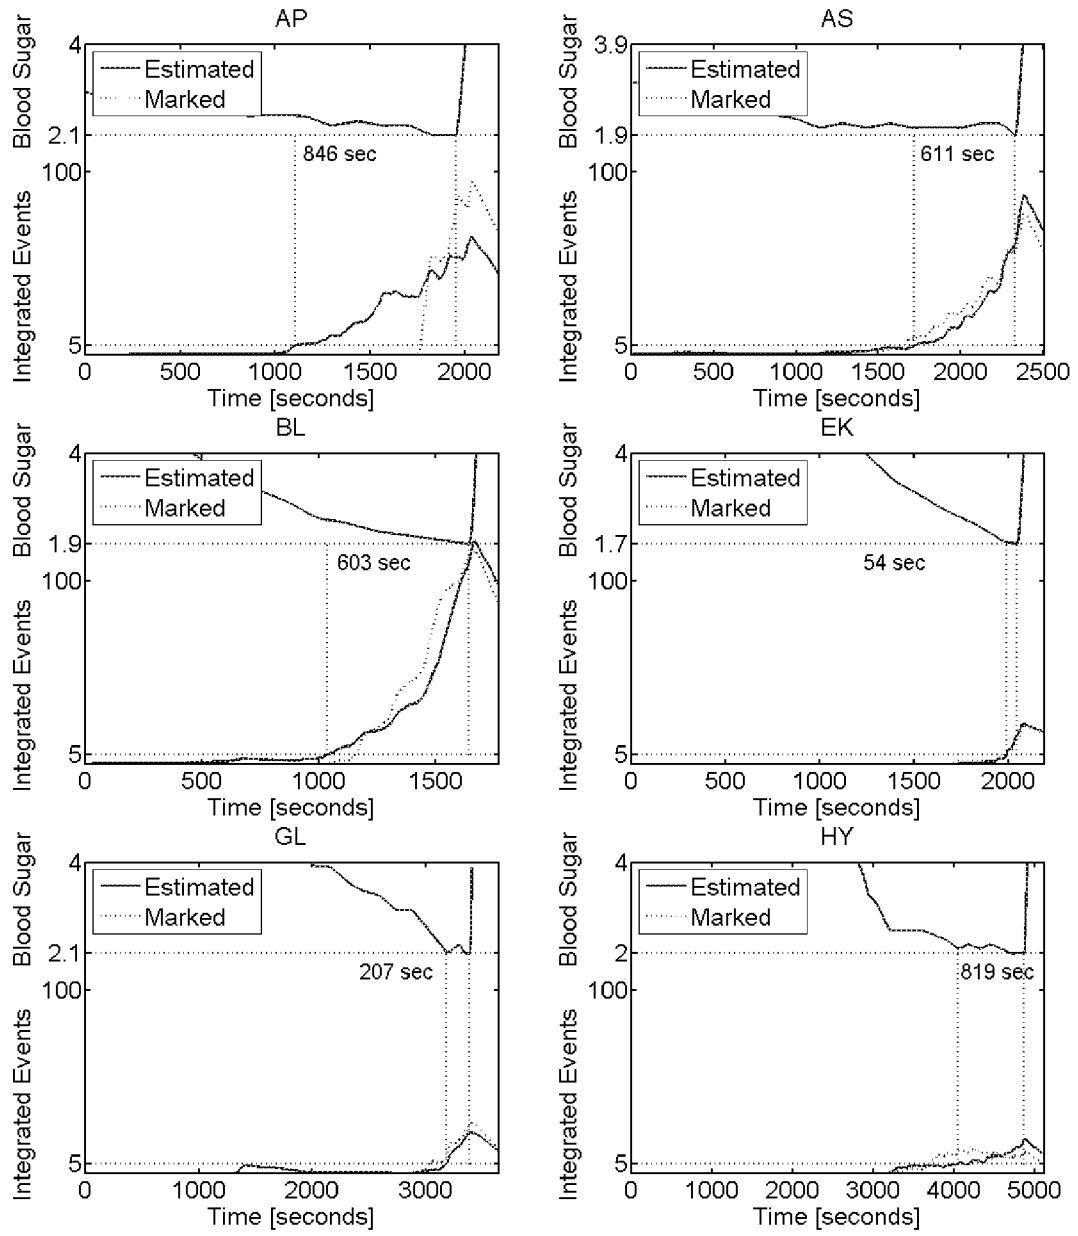


Figure 7

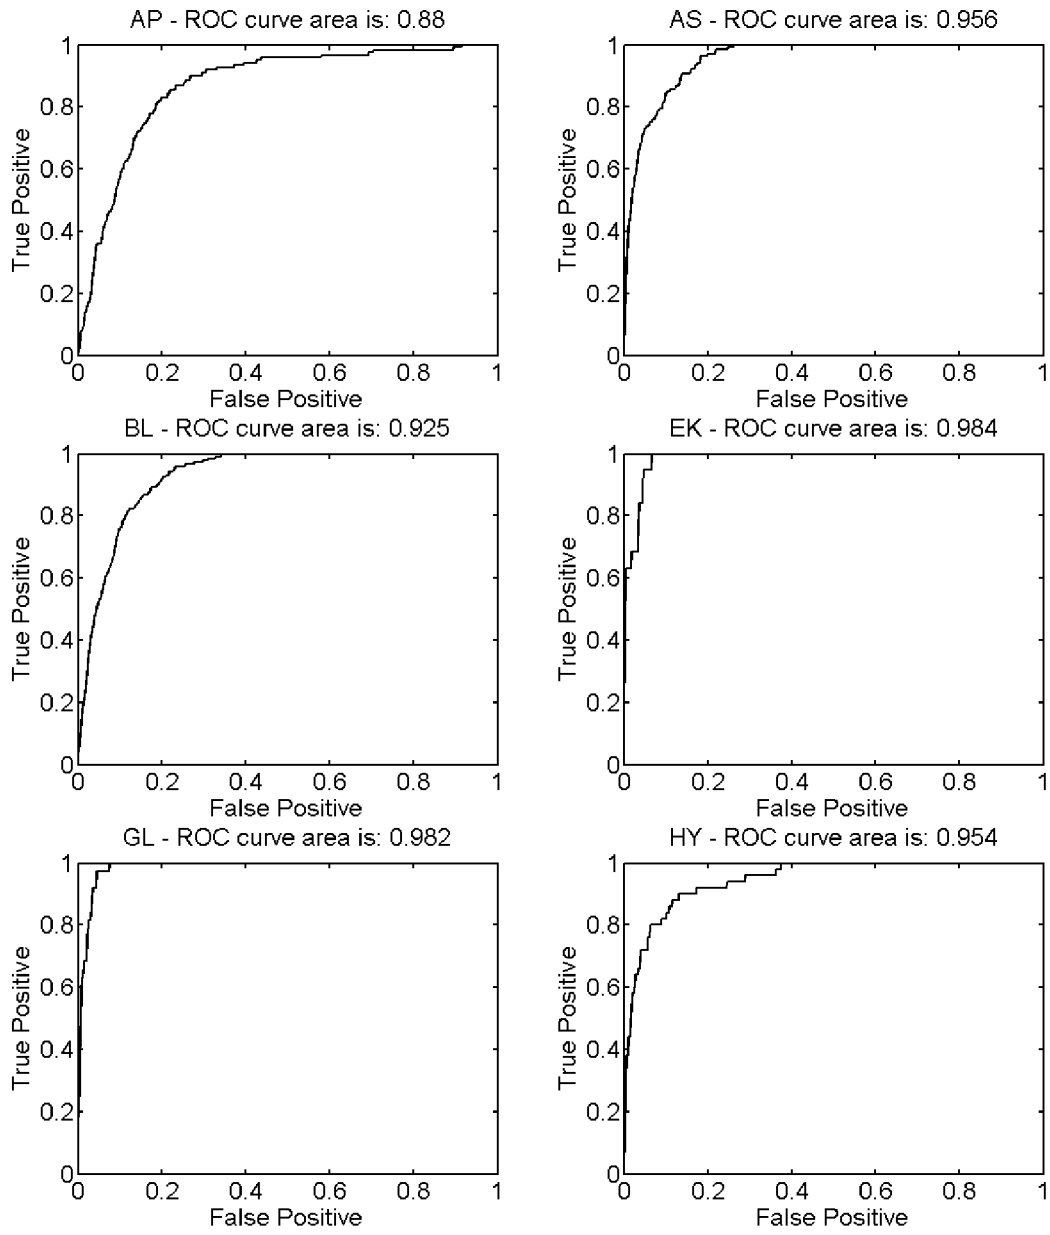


Figure 8

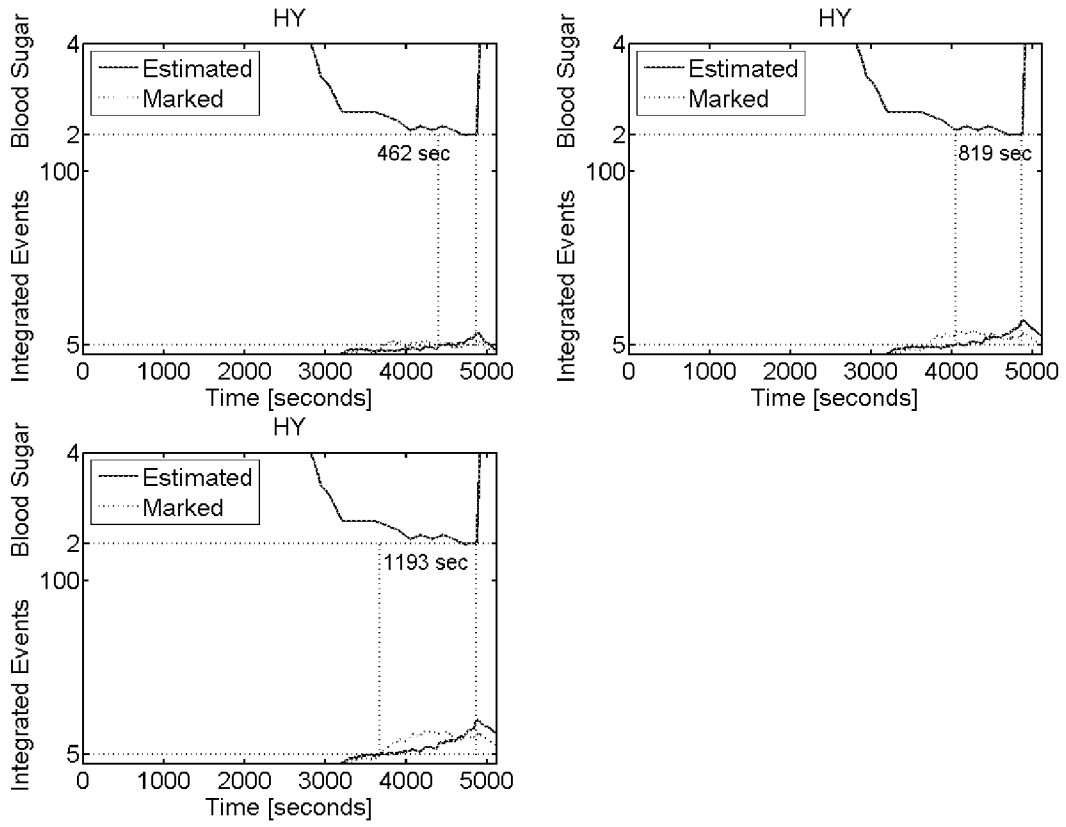


Figure 9

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6572542 A [0004]

Non-patent literature cited in the description

- **GADE J. ; ROSENFALCK A. ; BENDTSON I.** *Meth Inform Med*, 1994, vol. 33, 153-6 [0006]
- *Current Practice of Clinical Electroencephalography.* Lippincott, Williams & Wilkiks pub, 72-74 [0035]

专利名称(译)	分析脑电信号以检测低血糖		
公开(公告)号	EP2040608B1	公开(公告)日	2015-03-25
申请号	EP2007729990	申请日	2007-06-07
[标]申请(专利权)人(译)	HYPO SAFE		
申请(专利权)人(译)	HYPO-SAFE A / S		
当前申请(专利权)人(译)	HYPO-SAFE A / S		
[标]发明人	BECK NIELSEN HENNING MADSEN RASMUS ELSBORG		
发明人	BECK-NIELSEN, HENNING MADSEN, RASMUS ELSBORG		
IPC分类号	A61B5/0476 A61B5/145 A61B5/00		
CPC分类号	A61B5/14532 A61B5/0476 A61B5/726 A61B5/7267		
优先权	2006011872 2006-06-15 GB		
其他公开文献	EP2040608A2		
外部链接	Espacenet		

摘要(译)

通过以下方式检测指示EEG信号中的低血糖的特征： - 将EEG信号分成一系列时间段， - 对于每个时间段确定是否存在指示低血糖的EEG信号模式，并且其中EEG信号的模式指示确定低血糖症存在于时间段中，将其记录为事件， - 将在选定数量的先前时间段期间记录的事件的数量进行积分，这些时间段一起构成选定的时间段，可选地以时间加权的方式，并且 - 当所述积分事件数超过预设阈值数时和/或当所述积分随时间的曲线与先前建立的曲线之间存在匹配阈值水平时，确定EEG信号指示基于所述积分存在低血糖。所述曲线的理想模型指示低血糖。

$$\text{Quadratic Measure} = \frac{(x - \mu_{pos})^2}{\sigma_{pos}^2} - \frac{(x - \mu_{neu})^2}{\sigma_{neu}^2}$$