



(11) **EP 2 723 229 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
26.09.2018 Bulletin 2018/39

(51) Int Cl.:
A61B 5/00 (2006.01) G06F 19/00 (2018.01)

(21) Application number: **12802310.8**

(86) International application number:
PCT/US2012/043910

(22) Date of filing: **23.06.2012**

(87) International publication number:
WO 2012/178134 (27.12.2012 Gazette 2012/52)

(54) **UNIFIED PLATFORM FOR MONITORING AND CONTROL OF BLOOD GLUCOSE LEVELS IN DIABETIC PATIENTS**

VEREINHEITLICHTE PLATTFORM ZUR ÜBERWACHUNG UND STEUERUNG DES BLUTZUCKERSPIEGELS BEI DIABETESPATIENTEN

PLATEFORME UNIFIÉE POUR LA SURVEILLANCE ET LA RÉGULATION DES NIVEAUX DE GLUCOSE DANS LE SANG CHEZ DES PATIENTS DIABÉTIQUES

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **KEITH-HYNES, Patrick, T.**
Charlottesville, VA 22901 (US)
- **BRETON, Marc, D.**
Charlottesville, VA 22901 (US)
- **PATEK, Stephen, D.**
Charlottesville, VA 22901 (US)

(30) Priority: **23.06.2011 US 201161500545 P**

(43) Date of publication of application:
30.04.2014 Bulletin 2014/18

(74) Representative: **Slingsby Partners LLP**
1 Kingsway
London WC2B 6AN (GB)

(73) Proprietor: **University of Virginia Patent Foundation**
Charlottesville, VA 22902 (US)

(56) References cited:
WO-A1-2010/062898 WO-A1-2010/138848
WO-A1-2011/050337 US-A1- 2003 212 317
US-A1- 2008 172 205 US-A1- 2009 006 129
US-A1- 2010 185 175 US-A1- 2011 028 817

(72) Inventors:
• **KOVATCHEV, Boris, P.**
Charlottesville, VA 22901 (US)

EP 2 723 229 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

[0001] Diabetes mellitus (DM), often simply referred to as diabetes, is a group of metabolic diseases characterized by high glucose levels in the blood (i.e. hyperglycemia), either because the body does not produce enough insulin (Type 1 DM or T1DM), or because cells do not respond to the insulin that is produced (Type 2 DM or T2DM). Intensive treatment with insulin and with oral medications to maintain nearly normal levels of glycemia (i.e. euglycemia) markedly reduces chronic complications in both T1DM and T2DM [1,2,3], but may risk symptomatic hypoglycemia and potentially life-threatening severe hypoglycemia. Therefore, hypoglycemia has been identified as the primary barrier to optimal diabetes management [4,5]. People with T1DM and T2DM face a life-long optimization problem: to maintain strict glycemic control without increasing their risk for hypoglycemia. However, the struggle for close glycemic control could result in large blood glucose (BG) fluctuations over time. This process is influenced by many external factors, including the timing and amount of insulin injected, food eaten, physical activity, etc. In other words, BG fluctuations in diabetes are the measurable result of the interactions of a complex and dynamic biological system, influenced by many internal and external factors.

[0002] The optimization of this system depends largely on self-treatment behavior, which has to be informed by glucose monitoring and has to utilize data and technology available in the field. The currently accessible data sources include self-monitoring of blood glucose (SMBG), continuous glucose monitoring (CGM), as well as assessment of symptoms and self-treatment practices. The available treatments include medication (exclusively for T2DM), multiple daily insulin injections (MDI), and insulin pumps (CSII - continuous subcutaneous insulin injection). Currently, these treatments are at various stages of development and clinical acceptance, with SMBG now a routine practice, CGM rapidly developing, and emerging integrated systems that combine CGM with CSII and pave the way for the artificial pancreas of the near future.

Self-Monitoring of Blood Glucose

[0003] Contemporary home BG meters offer convenient means for frequent and accurate BG determinations through SMBG [6,7]. Most meters are capable of storing BG readings (typically over 150 readings) and have interfaces to download these readings into a computing device such as a PC. The meters are usually accompanied by software that has capabilities for basic data analysis (e.g. calculation of mean BG, estimates of the average BG over the previous two weeks, percentages in target, hypoglycemic and hyperglycemic zones, etc.), logging of the data, and graphical representations of the BG data (e.g. histograms, pie charts, etc.). In a series of studies

we have shown that specific risk analysis of SMBG data could also capture long-term trends towards increased risk for hypoglycemia [8, 9,10], and could identify 24-hour periods of increased risk for hypoglycemia [11,12]. The basics of the risk analysis are presented below. The methods outlined here have been applied to both SMBG and CGM data.

[0004] Evaluating Risk for Hypoglycemia and Hyperglycemia: These methods are based on the concept of Risk Analysis of BG data [13], and on the recognition of a specific asymmetry of the BG measurement scale that can be corrected by a mathematical data transformation [14]. The risk analysis steps are as follows:

1. Symmetrization of the BG scale: A nonlinear transformation is applied to the BG measurements scale to map the entire BG range (20 to 600 mg/dl, or 1.1 to 33.3 mmol/l) to a symmetric interval. The BG value of 112.5 mg/dl (6.25 mmol/l) is mapped to zero, corresponding to zero risk for hypo- or hyperglycemia. The analytical form of this transformation is $f(BG, \alpha, \beta) = [(\ln(BG))^{\alpha-\beta}]$, $\alpha, \beta > 0$, where the parameters are estimated as $\alpha=1.084$, $\beta=5.381$, $\gamma=1.509$, if BG is measured in mg/dl and $\alpha=1.026$, $\beta=1.861$, $\gamma=1.794$ if BG is measured in mmol/l [14].

2. Assignment of a risk value to each SMBG reading: We define the quadratic risk function $r(BG)=10f(BG)^2$. The function $r(BG)$ ranges from 0 to 100. Its minimum value is achieved at $BG=112.5$ mg/dl (a safe euglycemic BG reading), while its maximum is reached at the extreme ends of the BG scale. Thus, $r(BG)$ can be interpreted as a measure of the risk associated with a certain BG level. The left branch of this parabola identifies the risk of hypoglycemia, while the right branch identifies the risk of hyperglycemia.

3. Computing measures of risk for hypoglycemia and glucose variability: Let x_1, x_2, \dots, x_n be a series of n BG readings, and let $rl(BG)=r(BG)$ if $f(BG)<0$ and 0 otherwise; $rh(BG)=r(BG)$ if $f(BG)>0$ and 0 otherwise. Then the Low Blood Glucose Index (LBGI) is computed as:

$$LBGI = \frac{1}{n} \sum_{i=1}^n rl(x_i)$$

[0005] In other words, the LBGI is a non-negative quantity that increases when the number and/or extent of low BG readings increases. In studies, the LBGI typically accounted for 40-55% of the variance of future significant hypoglycemia in the subsequent 3-6 months [8,9,10], which made it a potent predictor of hypoglycemia based on SMBG. Similarly, we compute the High Blood Glucose Index (HBGI) as follows:

$$HBGI = \frac{1}{n} \sum_{i=1}^n rh(x_i)$$

[0006] The HBGI is a non-negative quantity that increases when the number and/or extent of high BG readings increases.

Continuous Glucose Monitoring

[0007] Since the advent of continuous glucose monitoring technology 10 years ago [15,16,17], which initially had limited performance particularly in the hypoglycemic range [18,19], significant progress has been made towards versatile and reliable CGM devices that not only monitor the entire course of BG day and night, but also provide feedback to the patient, such as alarms when BG reaches preset low or high levels. A number of studies have documented the benefits of continuous glucose monitoring [20,21,22,23] and charted guidelines for clinical use and its future as a precursor to closed-loop control [24,25,26,27]. However, while CGM has the potential to revolutionize the control of diabetes, it also generates data streams that are both voluminous and complex. The utilization of such data requires an understanding of the physical, biochemical, and mathematical principles and properties involved in this new technology. It is important to know that CGM devices measure glucose concentration in a different compartment - the interstitium. Interstitial glucose (IG) fluctuations are related to BG presumably via the diffusion process [28,29,30]. To account for the gradient between BG and IG, CGM devices are calibrated with capillary glucose, which brings the typically lower IG concentration to corresponding BG levels. Successful calibration would adjust the amplitude of IG fluctuations with respect to BG, but would not eliminate the possible time lag due to BG-to-IG glucose transport and the sensor processing time (instrument delay). Because such a time lag could greatly influence the accuracy of CGM, a number of studies were dedicated to its investigation, yielding various results [31,32,33,34]. For example, it was hypothesized that if glucose fall is due to peripheral glucose consumption the physiologic time lag would be negative, i.e. fall in IG would precede fall in BG [28,35]. In most studies IG lagged behind BG (most of the time) by 4-10 minutes, regardless of the direction of BG change [30,31]. The formulation of the push-pull phenomenon offered reconciliation of these results and provided arguments for a more complex BG-IG relationship than a simple constant or directional time lag [34,36]. In addition, errors from calibration, loss of sensitivity, and random noise confound CGM data [37]. Nevertheless, the accuracy of CGM is increasing and may be reaching a physiological limit for subcutaneous glucose monitoring [38,39,40].

The Artificial Pancreas

[0008] The next step in the progression of diabetes management is automated glucose control, or the artificial pancreas, which links a continuous glucose monitor with an insulin pump. A key element of this combination is a closed-loop control algorithm or method, which monitors blood glucose fluctuations and the actions of the insulin pump, and recommends insulin delivery at appropriate times.

[0009] The artificial pancreas idea can be traced back to developments that took place over thirty years ago when the possibility for external BG regulation in people with diabetes had been established by studies using intravenous (i.v.) glucose measurement and i.v. infusion of glucose and insulin. Systems such as the Biostator™ have been introduced and used in hospital settings to maintain normoglycemia (or euglycemia) by exerting both positive (via glucose or glucagon) and negative (via insulin) control [51,52,53,54,55]. Detailed descriptions of the major early designs can be found in [56,57,58,59,60,61]. More work followed, spanning a broader range of BG control techniques, powered by physiologic mathematical modeling and computer simulation control [62,63,64,65]. A review of methods for i.v. glucose control can be found in [66]. However, i.v. closed-loop control remains cumbersome and unsuited for outpatient use. An alternative to extracorporeal i.v. control has been presented by implantable intra-peritoneal (i.p.) systems employing intravenous BG sampling and i.p. insulin delivery [67,68]. The implementation of these systems, however, requires considerable surgery. Thus, with the advent of minimally-invasive subcutaneous (s.c.) CGM, increasing academic and industrial effort has been focused on the development of s.c.-s.c. systems, using CGM coupled with an insulin infusion pump and a control algorithm or method [69,70,71,72]. In September 2006, the Juvenile Diabetes Research Foundation (JDRF) initiated the Artificial Pancreas Project and funded a consortium of centers to carry closed-loop control research [73]. So far, encouraging pilot results have been reported by several centers [74,75,76,77,78].

[0010] Thus, in the past 30 years the monitoring and control of BG levels in diabetes has progressed from assessment of average glycemia once in several months, through daily SMBG, to minutely CGM. The increasing temporal resolution of the monitoring technology has enabled increasingly intensive diabetes treatment, from daily insulin injections or oral medication, through insulin pump therapy, to the artificial pancreas of the near future.

[0011] US 2009/006129 describes a diagnosis, therapy and prognosis system (DTPS) to help a healthcare provider or patient in diagnosing, treating and interpreting data. The apparatus provides data collection based on protocols, and a mechanism for testing data integrity and accuracy. The data is then analysed to characterise the patient's metabolic state to provide a diagnosis.

[0012] US 2010/185175 describes a system for at least partial closed-loop control of a medical condition. The system comprises a medical fluid pump and a continuous analyte monitor and controller. The controller includes a processor that controls delivery of the medical fluid based on data received from the continuous analyte monitor.

BRIEF SUMMARY OF THE INVENTION

[0013] As evident from the discussion above, a multitude of methods exist for BG monitoring and control in diabetes, ranging from traditional SMBG, medication, and MDI treatment, to CGM and artificial pancreas. These methods are currently dissimilar and there is no system that can handle more than one monitoring or control method at a time. An aspect of an embodiment of the present invention introduces the first flexible system capable of utilizing data from different monitoring techniques and capable of providing assistance to patients with diabetes at several scalable levels, ranging from advice about long-term trends and prognosis to real-time automated closed-loop control (artificial pancreas). These scalable monitoring and treatment strategies are delivered by a unified system - named by the present inventors as the Diabetes Assistant (**DiAs**) platform - that provides a foundation for implementation of various monitoring, advisory, and automated diabetes treatment algorithms or methods. The DiAs recommendations are tailored to the specifics of an individual patient, and to the patient risk assessment at any given moment. Some nonlimiting and exemplary unique characteristics of DiAs are:

- Informed by a Body Sensor Network;
- Modular - layered architecture distributes data processing tasks across various application modules; individual modules are easily replaceable;
- Scalable - naturally support new and expanded functionality, multiple data sources, and multiple data utilization strategies;
- Portable - DiAs can run easily on portable computing devices, such as a cell phone, tablet computer, portal digital assistant (PDA), etc; thus it is deployable on a wide variety of rugged, inexpensive, and readily available devices;
- Local and Global modes of operation - certain processes and patient interactions are available through the portable device; other services and remote monitoring of subject and system states are available via wireless communications (e.g. 3G, WiFi, etc.).

[0014] According to the invention there are provided an apparatus and a method according to claims 1 and 10. Preferable features of the invention are defined in the dependent claims.

BRIEF SUMMARY OF THE DRAWINGS

[0015]

5 **Figure 1** is a schematic illustration of the DiAs platform inputs and outputs according to an aspect of the invention;

Figure 2 is a schematic illustration of DiAs processes and services according to an aspect of the invention;

10 **Figure 3** is a block diagram of the DiAs system including applications and communication functions according to an embodiment of the invention;

Figure 4 shows an example implementation of the DiAs system on a cell phone platform according to an embodiment of the invention;

15 **Figure 5** is a schematic illustration of an implementation of the DiAs system as a hub for a body sensor network; and

20 **Figure 6** is a schematic block diagram of an example data processing system for implementation of the present invention in whole or in part.

DETAILED DESCRIPTION OF THE INVENTION

25 Overview

[0016] As shown in Fig. 5, a principal application of the DiAs system is the dynamic aggregation of body sensor network (BSN) data toward the goal of supporting long-term and efficient treatment of diabetes. DiAs is based on a wearable or handheld Diabetes Assistant platform that collects and pre-processes data from each individual's BSN, and uploads summary statistics to a remote location. The interface/algorithmic/methodology framework of DiAs: (i) ensures plug and play functionality with different metabolic sensors, (ii) allows for a general framework for prioritization of sensor data, making it clear how scarce computational, memory, and communication resources will be allocated to various sensing modalities, (iii) manages access to multiple uplink channels of varying reliability to a remote site, and (iv) resolves tradeoffs relating to where heavy computations should be performed (e.g., locally within the DiAs platform or remotely).

45 DiAs Inputs and Outputs

[0017] Fig. 1 presents the data sources available to the DiAs platform and the output services that DiAs provides. The data sources include SMBG, CGM, insulin delivery data (MDI and CSII), and other BSN data inputs such as heart rate, body accelerometer data, blood pressure, respiration, EKG data, etc. Depending on data availability (intermittent or continuous, blood glucose alone, or a multivariate data stream), DiAs provides different types of services that can be generally classified as:

- Local Services: Applications that run on a portable

device (e.g. a cell phone or tablet computer) communicating with an array of self-SMBG monitoring and CGM devices, an array of insulin delivery devices, and with other sensors in a BSN. The local service of DiAs is equipped with intelligent processing to provide an array of patient services, including safety supervision, local alerts, patient advisory functions, and closed-loop control (described further below);

- **Global Services:** A centralized server communicating with multiple local services to provide different levels of data processing, advice, and training to patients; enable remote monitoring of glucose control profiles (e.g. parents monitoring remotely their children with diabetes); enable global alerts (e.g. a 911 call with GPS service to pinpoint a patient in need of emergency assistance), and to provide a physician-oriented information service presenting key data for multiple patients at a glance.

DiAs Processes

[0018] The general flow of DiAs processes is presented in Fig. 2 and includes the following steps:

1. Incoming data are directed to a Data Availability Classifier (DAC), which assesses the frequency, dimensionality, and quality of the incoming data. Based on the assessment, the DAC recommends different classes of data processing algorithms for the incoming data. Many of these algorithms already exist and are generally known, and can be classified as follows:

- **SMBG:** This is currently the most established algorithmic class, including methods for the retrieval of SMBG data, evaluation of glycemic control, estimation of the risk for hypoglycemia, and information displays. SMBG acquisition and processing methods are described in several U.S. patents and published patent applications (see references [79-85]). A 5-year clinical trial testing a SMBG-based system in 120 people with T1DM was recently completed, resulting in improved glycemic control, reduction of the risk for severe hypoglycemia, and high patient approval rating (results published in [86]);
- **CGM:** Key elements applicable to these methods have been defined (references [87-92]). These methods are currently under development and testing in a large NIH-funded research project (Grant RO1 DK 085623, Principal Investigator Dr. Boris Kovatchev);
- **CGM + insulin pump:** Most of the methods applicable to CGM alone have extensions capable of dealing with input/output to/from an insulin pump. We have recently completed an extensive series of clinical trials of closed-loop control to date.

◦ **Other:** Heart rate changes can be used to indicate periods of physical activity, and more specifically periods of increased insulin sensitivity associated with exercise. These data inform diabetes control at several levels, including risk assessment for hypoglycemia and closed-loop control [93,94].

2. The first step of data processing is Patient State Estimation, given available data and using one of the methods described above. The state estimation results in assessment of the patient's risk status, which can be based on the risk analysis metrics presented in the background discussion above, and on biosystem observers or sensors, which process physiologic (and possibly behavioral) data to produce quantitative biosystem state estimators. These algorithms or methods are based on underlying mathematical models of the human metabolism and a Kalman filter, which produces system state estimation. Each system state estimator is a physiological or behavioral parameter of importance to the functioning of a person. The ensemble (vector) of biosystem estimators for a particular person represents the status of this person in terms of the blood glucose trend, availability of insulin, and risk for hypoglycemia. In essence, biosystem observers personalize the metabolic observation to a specific subject and extract composite information from the vast array of raw data that allows the precise evaluation of the subject's condition. It is anticipated that the biosystem observers will reside within a wearable DiAs system, while their summarized output will be sent to both the local predictive and control algorithms or methods and to remote observers as follows:

◦ The primary output from the Patient State Estimation will be assessment of the patient's risk status for hypo- or hyperglycemia, based on the risk analysis and the LBG1/HBGI presented above. If the data quality and density is adequate for the risk status of the patient (e.g. the patient is in a steady state performing regular SMBG resulting in LBG1 and HBGI lower than certain preset thresholds), then DiAs refers the data to algorithms that maintain the current patient status or fine-tune the patient's glycemic control. These algorithms can work in either an advisory or automated (closed-loop control) mode as follows:

◦ In advisory mode, DiAs activates the following services modules:

- Advisory Module 1: Prediction of elevated risk for hypoglycemia (24 hours ahead);

- Advisory Module 2: Bolus calculator suggesting pre-meal insulin doses;
- Advisory Module 3: Suggestion of basal rate profiles for the next 24 hours.

◦ In closed-loop control mode, DiAs activates the following service modules:

- Control Module 1: Real-time detection and prevention of hypoglycemia;
- Control Module 2: Stochastic control of pre-meal insulin boluses, and
- Control Module 3: Deterministic control of basal rate and overnight steady state.

◦ If the data quality and density is inadequate for the risk status of the patient (e.g. the patient is at high risk for hypoglycemia, hyperglycemia, or both as indicated by the LBG1 and HBG1 exceeding certain preset thresholds), then:

- In advisory mode, DiAs recommends enhanced monitoring (e.g. more frequent SMBG or switching to CGM for a certain period of time);
- In automated control mode, DiAs switches the monitoring device to higher frequency SMBG measurement or to CGM mode (Note: such flexible monitoring devices are not currently manufactured, but are anticipated to be available in the future).

[0019] Fig. 3 presents a detailed schematic of the DiAs architecture:

- Central to this architecture is the Biometric State Estimator, which is the hub for exchange of data between the DiAs monitoring devices and algorithmic services or related methods. The Biometric State Estimator may also exchange data with remote physicians and/or patient care centers over the Internet through a network interface;
- The inputs used for state estimation are provided by various peripheral devices that monitor blood glucose fluctuations (SMBG Service, CGM Service), execute insulin delivery (Pump Service), or monitor other physiological parameters (Heart Rate Service, Esc. Service) as shown in Fig. 3;
- In turn, the Biometric State Estimator provides feedback to these devices as determined by a Safety Service, which assesses the integrity of the received data and judges whether the peripheral input/output devices are functioning properly. Methods employed by the Safety Service include previously introduced detection of CGM sensor errors [91] or judging the safety of insulin delivery [92];
- DiAs Applications may include various advisory

and/or control algorithms, system and patient state alarms and indicators. These applications may be external to the DiAs system, and may be developed by third parties. Such applications may use DiAs services provided that they comply with the data exchange standards of the system. For example, a Hyperglycemia Mitigation Service (HMS) is a closed-loop control algorithm or method included in one of the embodiments of DiAs;

[0020] The user interface with the DiAs system can be custom designed to meet the needs of specific DiAs implementations. One such implementation of a user interface is shown in Fig. 4:

- Two "traffic lights" signify the patient's present risk status for hypoglycemia and hyperglycemia, respectively, indicating low risk (green light), moderate risk/system action to mitigate the risk (yellow light) and high risk/necessity for immediate human intervention (red light);
- Several system/patient status inquiry icons open additional interfaces allowing the patient to access graphical and numerical representation of his/her glucose control, or inform the system of events (such as carbohydrate intake or exercise), which are treated as additional inputs by the DiAs analytical system;
- Network service (described in the next section) ensures remote monitoring and transmission of alerts and critical information in high-risk states.

Implementation of DiAs

[0021] Fig. 5 shows two major components of a DiAs implementation as a Body Sensor Network:

◦ Local Services (within the wearable/portable DiAs device) use predictive and control algorithms or methods based on simplified models of the human metabolic system that are trackable in real time. These are simple, typically linearized macro-level models that focus only on the principal system components. One example of such a model is the classic Minimal Model of Glucose Kinetics developed 30 years ago [95]. Available algorithms or methods include assessment, prediction, and control of glucose fluctuations in diabetes:

- Risk analysis of metabolic state with respect to normative limits;
- Detection of abrupt system changes, i.e. transitions of the system (person) from a stable to a critical state;
- Prediction of trends and gradual system changes, and outcome evaluation;
- Estimation of the probability for abrupt critical transitions;
- Warnings, alarms, and advisory messages

when critical thresholds are approached;

- Automated intervention to prevent critical events;
- Communication to remote location and global algorithms or methods.

As shown in Fig. 5, a portable DiAs device (such as shown in Fig. 4) is communicatively connected (e.g. wirelessly through a wireless communication protocol such as Bluetooth, IEEE 802.11, etc.) to a plurality of BSN sensors, such as an ICP sensor, ECG sensor, blood pressure sensor, pulse oximetry sensor, inertial sensor, EMG sensor, artificial pancreas sensor, etc. Additionally, the DiAs device may have an interface to accept SMBG data.

◦ Global services rely on predictive and control algorithms or methods deployed at a central location and receiving information from an array of individual system observers. These algorithms or methods will be based on large-scale probability models, risk analysis, clustering, and discriminant algorithms or methods. The output of these algorithms or methods will allow:

- The monitoring of vital signs and metabolic processes by health care providers;
- The detection of critical cases that require immediate intervention;
- Collection of population-level anonymous public health statistics of interest to health care organizations.

◦ Software/Hardware Implementation: Central to DiAs is a scalable software stack with a modular design that can be efficiently adapted to a variety of hardware platforms. The software architecture, the availability of suitable hardware platforms and opportunities to transfer software modules to commercial partners will factor into the choice of DiAs operating systems. For clinical trials and ambulatory implementation, hardware is needed that is portable, rugged, reliable, inexpensive and easily available. In this regard, a cell phone or a tablet computer could be selected. Consequently, the DiAs system may run within a customized version of the Android operating system. Android has a robust development environment, is available with source code, is backed by Google and runs on an ever-increasing array of cell phones and tablets from a variety of manufacturers. Android is being adopted by many commercial developers for new embedded software projects. Although many current products with embedded control software either have no operating system at all or use a simple control loop the trend is towards basing new embedded software projects on Android and embedded Linux. Since Android is built on top of Linux, an Android-based operating system for DiAs

would allow transfer of software code to industry partners for commercial use. Android also provides a rich software development kit that supports multi-touch graphical user interface design, data communications, geo-location and telephony. Specifically:

At the highest level the AAPP Software Stack is composed of three major functional blocks: Device I/O Services, Core Services, and Control. As described above, Fig. 3 presents a diagram of the software stack depicting these blocks.

Device I/O Services handles all communication with sensors, pumps and other devices and provides a data interface to other elements of the system. The Device I/O modules store SMBG, CGM, and delivered insulin data and provide it to other components upon request.

Device I/O modules also implement a sensor and pump command service that validates and delivers commands received from the Safety Service.

Core Services is responsible for providing a runtime environment for applications such as the Closed-Loop Control App or the User Advice App and for supervising their operation. It generates state estimates based upon available data and provides this data to applications upon request.

Safety Service screens insulin bolus commands for safety before delivering them to the pump module and monitors the functioning of I/O devices detecting errors and potentially unsafe deviations.

[0022] While a preferred operating system has been discussed above, it will be recognized by those skilled in the art that the DiAs system may be implemented using any operating system that has features necessary to implement the DiAs system as contemplated above.

[0023] Turning now to Fig. 6, a functional block diagram is shown for a computer system 600 for exemplary implementation of an embodiment or portion of an embodiment of the present invention. For example, a method or system of an embodiment of the present invention may be implemented using hardware, software or a combination thereof and may be implemented in one or more computer systems or other processing systems, such as personal digit assistants (PDAs) equipped with adequate memory and processing capabilities. In an example embodiment, the invention was implemented in software running on a general purpose computer 600 as illustrated in Figure 6. The computer system 600 may include one or more processors, such as processor 604. The Processor 604 is connected to a communication infrastructure 606 (e.g., a communications bus, cross-over bar, or network). The computer system 600 may include a display interface 602 that forwards graphics, text, and/or other

data from the communication infrastructure **606** (or from a frame buffer not shown) for display on the display unit **630**. Display unit **630** may be digital and/or analog.

[0024] The computer system **600** may also include a main memory **608**, preferably random access memory (RAM), and may also include a secondary memory **610**. The secondary memory **610** may include, for example, a hard disk drive **612** and/or a removable storage drive **614**, representing a floppy disk drive, a magnetic tape drive, an optical disk drive, a flash memory, etc. The removable storage drive **614** reads from and/or writes to a removable storage unit **618** in a well known manner. Removable storage unit **618**, represents a floppy disk, magnetic tape, optical disk, etc. which is read by and written to by removable storage drive **614**. As will be appreciated, the removable storage unit **618** includes a computer usable storage medium having stored therein computer software and/or data.

[0025] In alternative embodiments, secondary memory **610** may include other means for allowing computer programs or other instructions to be loaded into computer system **600**. Such means may include, for example, a removable storage unit **622** and an interface **620**. Examples of such removable storage units/interfaces include a program cartridge and cartridge interface (such as that found in video game devices), a removable memory chip (such as a ROM, PROM, EPROM or EEPROM) and associated socket, and other removable storage units **622** and interfaces **620** which allow software and data to be transferred from the removable storage unit **622** to computer system **600**.

[0026] The computer system **600** may also include a communications interface **624**. Communications interface **624** allows software and data to be transferred between computer system **600** and external devices. Examples of communications interface **624** may include a modem, a network interface (such as an Ethernet card), a communications port (e.g., serial or parallel, etc.), a PCMCIA slot and card, a modem, etc. Software and data transferred via communications interface **624** are in the form of signals **628** which may be electronic, electromagnetic, optical or other signals capable of being received by communications interface **624**. Signals **628** are provided to communications interface **624** via a communications path (i.e., channel) **626**. Channel **626** (or any other communication means or channel disclosed herein) carries signals **628** and may be implemented using wire or cable, fiber optics, blue tooth, a phone line, a cellular phone link, an RF link, an infrared link, wireless link or connection and other communications channels.

[0027] In this document, the terms "computer program medium" and "computer usable medium" are used to generally refer to media or medium such as various software, firmware, disks, drives, removable storage drive **614**, a hard disk installed in hard disk drive **612**, and signals **628**. These computer program products ("computer program medium" and "computer usable medium") are means for providing software to computer system

600. The computer program product may comprise a computer useable medium having computer program logic thereon. The invention includes such computer program products. The "computer program product" and "computer useable medium" may be any computer readable medium having computer logic thereon.

[0028] Computer programs (also called computer control logic or computer program logic) are may be stored in main memory **608** and/or secondary memory **610**. Computer programs may also be received via communications interface **624**. Such computer programs, when executed, enable computer system **600** to perform the features of the present invention as discussed herein. In particular, the computer programs, when executed, enable processor **604** to perform the functions of the present invention. Accordingly, such computer programs represent controllers of computer system **600**.

[0029] In an embodiment where the invention is implemented using software, the software may be stored in a computer program product and loaded into computer system **600** using removable storage drive **614**, hard drive **612** or communications interface **624**. The control logic (software or computer program logic), when executed by the processor **604**, causes the processor **604** to perform the functions of the invention as described herein.

[0030] In another embodiment, the invention is implemented primarily in hardware using, for example, hardware components such as application specific integrated circuits (ASICs). Implementation of the hardware state machine to perform the functions described herein will be apparent to persons skilled in the relevant art(s).

[0031] In yet another embodiment, the invention is implemented using a combination of both hardware and software.

[0032] In an example software embodiment of the invention, the methods described above may be implemented in SPSS control language or C++ programming language, but could be implemented in other various programs, computer simulation and computer-aided design, computer simulation environment, MATLAB, or any other software platform or program, windows interface or operating system (or other operating system) or other programs known or available to those skilled in the art.

REFERENCES

[0033]

1. Reichard P, Phil M. Mortality and treatment side effects during long-term intensified conventional insulin treatment in the Stockholm Diabetes Intervention study. *Diabetes* 43: 313-317, 1994
2. The Diabetes Control and Complications Trial Research Group. The effect of intensive treatment of diabetes on the development and progression of long-term complications of insulin-dependent diabetes mellitus. *N Engl J Med* 329: 978-986, 1993

3. UK Prospective Diabetes Study Group (UKPDS). Intensive blood-glucose control with sulphonylureas or insulin compared with conventional treatment and risk of complications in patients with type 2 diabetes. *Lancet* 352: 837-853, 1998
4. Cryer PE. Hypoglycaemia: The limiting factor in the glycaemic management of type I and type II diabetes. *Diabetologia* 45: 937-948, 2002
5. Cryer PE: Hypoglycemia: The Limiting factor in the management of IDDM. *Diabetes* 43: 1378-1389, 1994
6. Clarke WL, Cox D, Gonder-Frederick LA, Carter W, Pohl SL. Evaluating the clinical accuracy of self-blood glucose monitoring systems. *Diabetes Care*, 10: 622-628, 1987.
7. The diabetes research in children network (DirecNet) study group. A multicenter study of the accuracy of the One Touch® Ultra® home glucose meter in children with Type 1 diabetes. *Diabetes Technol Ther*, 5: 933-942, 2003
8. Kovatchev BP, Cox DJ, Gonder-Frederick LA Young-Hyman D, Schlundt D, Clarke WL. Assessment of risk for severe hypoglycemia among adults with IDDM: Validation of the Low Blood Glucose Index. *Diabetes Care* 21: 1870-1875, 1998.
9. Cox DJ, Kovatchev B, Julian D, Gonder-Frederick LA, Polonsky WH, Schlundt DG, Clarke WL. Frequency of severe hypoglycemia in IDDM can be predicted from self-monitoring blood glucose data. *J Clin Endocrinol Metab* 79: 1659-1662, 1994.
10. Kovatchev BP, Cox DJ, Kumar A, Gonder-Frederick LA and WL Clarke. Algorithmic Evaluation of Metabolic Control and Risk of Severe Hypoglycemia in Type 1 and Type 2 Diabetes Using Self-Monitoring Blood Glucose (SMBG) Data. *Diabetes Technol Ther*, 5 (5): 817-828, 2003.
11. Cox DJ, Gonder-Frederick LA, Ritterband L, Clarke WL, and Kovatchev BP. Prediction of Severe Hypoglycemia. *Diabetes Care*, 30: 1370-1373, 2007.
12. Kovatchev BP, Cox DJ, Farhy LS, Straume M, Gonder-Frederick LA, Clarke, WL. Episodes of Severe Hypoglycemia in Type 1 Diabetes are Preceded, and Followed, within 48 Hours by Measurable Disturbances in Blood Glucose. *J Clin Endocrinol Metab*, 85: 4287-4292, 2000.
13. Kovatchev BP, Straume M, Cox DJ, Farhy LS. Risk analysis of blood glucose data: A quantitative approach to optimizing the control of insulin dependent diabetes. *J of Theoretical Medicine*, 3:1-10, 2001.
14. Kovatchev BP, Cox DJ, Gonder-Frederick LA and WL Clarke. Symmetrization of the blood glucose measurement scale and its applications. *Diabetes Care*, 20: 1655-1658, 1997.
15. Mastrototaro J.J. The MiniMed Continuous Glucose Monitoring System. *Diabetes Technol Ther*, 2: Supplement 1: S-13 - S-18, 2000.
16. Bode B.W. Clinical Utility of the Continuous Glucose Monitoring System. *Diabetes Technol Ther*, 2: Supplement 1: S-35 - S-42, 2000.
17. Feldman B, Brazg R, Schwartz S, Weinstein R. A continuous glucose sensor based on wired enzyme technology - results from a 3-day trial in patients with Type 1 diabetes. *Diabetes Technol Ther*, 5: 769-778, 2003.
18. The diabetes research in children network (DirecNet) study group. The accuracy of the CGMS™ in children with Type 1 diabetes: Results of the diabetes research in children network (DirecNet) accuracy study. *Diabetes Technol Ther*, 5: 781-790, 2003.
19. Kovatchev BP, Anderson SM, Heinemann L, Clarke WL. Comparison of the numerical and clinical accuracy of four continuous glucose monitors. *Diabetes Care*, 31: 1160-1164, 2008.
20. Deiss, D, Bolinder, J, Riveline, J, Battelino, T, Bosi, E, Tubiana-Rufi, N, Kerr, D, Phillip, M: Improved glycemic control in poorly controlled patients with type 1 diabetes using real-time continuous glucose monitoring. *Diabetes Care* 29: 2730-2732, 2006.
21. Garg, K, Zisser, H, Schwartz, S, Bailey, T, Kaplan, R, Ellis, S, Jovanovic, L: Improvement in Glycemic Excursions With a Transcutaneous, Real-time Continuous Glucose Sensor. *Diabetes Care* 29:44-50, 2006.
22. Kovatchev BP, Clarke WL. Continuous glucose monitoring reduces risks for hypo- and hyperglycemia and glucose variability in diabetes. *Diabetes*, 56, Supplement 1: 0086OR, 2007.
23. The Juvenile Diabetes Research Foundation Continuous Glucose Monitoring Study Group: Continuous glucose monitoring and intensive treatment of type 1 diabetes. *N Engl J Med*, 359:1464-76, 2008.
24. Klonoff DC: Continuous glucose monitoring: roadmap for 21st century diabetes therapy. *Diabetes Care* 28:1231-1239, 2005.
25. Hovorka R: Continuous glucose monitoring and closed-loop systems. *Diabet Med* 23:1-12, 2006.
26. Klonoff DC: The Artificial Pancreas: How Sweet Engineering Will Solve Bitter Problems. *J Diabetes Sci Technol*, 1: 72-81, 2007.
27. Hirsch IB, Armstrong D, Bergenstal RM, Buckingham B, Childs BP, Clarke WL, Peters A, Wolpert H. Clinical Application of Emerging Sensor Technologies in Diabetes Management: Consensus Guidelines for Continuous Glucose Monitoring. *Diabetes Tech Ther*, 10: 232-246, 2008.
28. Rebrin K, Steil GM, van Antwerp WP, and Mastrototaro JJ: Subcutaneous glucose predicts plasma glucose independent of insulin: implications for continuous monitoring. *Am J Physiol Endocrinol Metab*, 277:E561-E571, 1999.
29. Rebrin K and Steil GM: Can interstitial glucose assessment replace blood glucose measurements?

Diabetes Technol Ther, 2:461-472, 2000.

30. Steil GM, Rebrin K, Hariri F, Jinagonda S, Tadros S, Darwin C, Saad MF: Interstitial fluid glucose dynamics during insulin-induced hypoglycaemia. *Diabetologia*, 48:1833-40, 2005.

31. Boyne M, Silver D, Kaplan J, and Saudek C: Timing of Changes in Interstitial and Venous Blood Glucose Measured With a Continuous Subcutaneous Glucose Sensor. *Diabetes*, 52:2790-2794, 2003.

32. Kulcu E, Tamada JA, Reach G, Potts RO, Lesho MJ: Physiological differences between interstitial glucose and blood glucose measured in human subjects. *Diabetes Care*, 26:2405-2409, 2003.

33. Stout PJ, Racchini JR, Hilgers ME: A Novel Approach to Mitigating the Physiological Lag between Blood and Interstitial Fluid Glucose Measurements. *Diabetes Technol Ther*, 6:635-644, 2004.

34. Wentholt IME, Hart AAM, Hoekstra JBL, DeVries JH. Relationship Between Interstitial and Blood Glucose in Type 1 Diabetes Patients: Delay and the Push-Pull Phenomenon Revisited. *Diabetes Technol Ther*, 9:169-175, 2004.

35. Wientjes KJ, Schoonen AJ: Determination of time delay between blood and interstitial adipose tissue glucose concentration change by microdialysis in healthy volunteers. *Int J Artif Organs*, 24:884-889, 2001.

36. Aussedat B, Dupire-Angel M, Gifford R, Klein JC, Wilson GS, Reach G: Interstitial glucose concentration and glycemia: implications for continuous subcutaneous glucose monitoring. *Am J Physiol Endocrinol Metab*, 278:E716-E728, 2000.

37. Kovatchev BP and Clarke WL. Peculiarities of the Continuous Glucose Monitoring Data Stream and Their Impact on Developing Closed-Loop Control Technology. *J Diabetes Sci Technol*, 2:158-163, 2008.

38. Clarke WL, Kovatchev BP: Continuous glucose sensors - continuing questions about clinical accuracy. *J Diabetes Sci Technol* 1:164-170, 2007.

39. The Diabetes Research in Children Network (DirecNet) Study Group. The Accuracy of the Guardian® RT Continuous Glucose Monitor in Children with Type 1 Diabetes. *Diabetes Tech Ther*, 10: 266-272, 2008.

40. Garg SK, Smith J, Beatson C, Lopez-Baca B, Voelmler M, Gottlieb PA. Comparison of Accuracy and Safety of the SEVEN and the Navigator Continuous Glucose Monitoring Systems. *Diabetes Tech Ther*, 11: 65-72, 2009.

41. T. Heise, T. Koschinsky, L. Heinemann, and V. Lodwig, "Glucose Monitoring Study Group. Hypoglycemia warning signal and glucose sensors: requirements and concepts," *Diabetes Technol Ther*, 5: 563-571, 2003.

42. B. Bode, K. Gross, N. Rikalo, S. Schwartz, T. Wahl, C. Page, T. Gross, and J. Mastrototaro. Alarms based on real-time sensor glucose values

alert patients to hypo- and hyperglycemia: the guardian continuous monitoring system. *Diabetes Technol Ther*, 6: 105-113, 2004.

43. G. McGarraugh and R. Bergenstal, "Detection of hypoglycemia with continuous interstitial and traditional blood glucose monitoring using the FreeStyle Navigator Continuous Glucose Monitoring System," *Diabetes Technol Ther*, 11: 145-150, 2009.

44. S.E. Noujaim, D. Horwitz, M. Sharma, J. Marhoul, "Accuracy requirements for a hypoglycemia detector: an analytical model to evaluate the effects of bias, precision, and rate of glucose change," *J Diabetes Sci Technol*, 1: 653-668, 2007.

45. W.K. Ward, "The role of new technology in the early detection of hypoglycemia," *Diabetes Technol Ther*, 6: 115-117, 2004.

46. B. Buckingham, E. Cobry, P. Clinton, V. Gage, K. Caswell, E. Kunselman, F. Cameron, and H.P. Chase. Preventing hypoglycemia using predictive alarm algorithms and insulin pump suspension. *Diabetes Technol Ther*, 11: 93-97, 2009.

47. Miller M, Strange P: Use of Fourier Models for Analysis and Interpretation of Continuous Glucose Monitoring Glucose Profiles. *J Diabetes Sci Technol*, 1: 630-638, 2007.

48. Kovatchev BP, Gonder-Frederick LA, Cox DJ, Clarke WL: Evaluating the accuracy of continuous glucose-monitoring sensors: continuous glucose-error grid analysis illustrated by TheraSense Freestyle Navigator data. *Diabetes Care*, 27:1922-28, 2004.

49. McDonnell CM, Donath SM, Vidmar SI, Werther GA, Cameron FJ: A Novel Approach to Continuous Glucose Analysis Utilizing Glycemic Variation. *Diabetes Technol Ther*, 7: 253-263, 2005.

50. Clarke WL & Kovatchev BP. Statistical Tools to Analyze CGM Data. *Diabetes Technol Ther*, 11: S45-S54, 2009.

51. Albisser AM, Leibel BS, Ewart TG, Davidovac Z, Botz CK, Zinggg W. An artificial endocrine pancreas. *Diabetes*, 23:389-396, 1974.

52. Clemens AH, Chang PH, Myers RW. The development of Biostator, a glucose-controlled insulin infusion system. *Horm Metab Res Supplement*, 7: 23-33, 1977.

53. Marliss EB, Murray FT, Stokes EF, Zinman B, Nakhoda AF, Denoga A, Leibel BS, and Albisser AM: Normalization of glycemia in diabetics during meals with insulin and glucagon delivery by the artificial pancreas. *Diabetes* 26: 663-672, 1977.

54. Pfeiffer EF, Thum Ch, and Clemens AH: The artificial beta cell - A continuous control of blood sugar by external regulation of insulin infusion (glucose controlled insulin infusion system). *Horm Metab Res* 487: 339-342, 1974.

55. Santiago JV, Clemens AH, Clarke WL, Kipnis DM. Closed-loop and open-loop devices for blood glucose control in normal and diabetic subjects. *Diabetes*, 28: 71-84, 1979.

56. Broekhuysen HM, Nelson JD, Zinman B, and Al-bisser AM: Comparison of algorithms for the closed-loop control of blood glucose using the artificial beta cell. *IEEE Trans Biomed Eng* 28: 678-687, 1981.
57. Clemens AH: Feedback control dynamics for glucose controlled insulin infusion system. *MedProg Technol* 6: 91-98, 1979.
58. Cobelli C, Ruggeri A: Evaluation of portal/peripheral route and of algorithms for insulin delivery in the closed-loop control of glucose in diabetes. A modeling study. *IEEE Trans Biomed Eng* 30: 93-103, 1983.
59. EW, Campbell LV, Chia YO, Meler H, and Lazarus L: Control of blood glucose in diabetics using an artificial pancreas. *Aust N Z J Med* 7: 280-286, 1977.
60. Fischer U, Jutzi E, Freyse E-J, and Salzsieder E: Derivation and experimental proof of a new algorithm for the artificial beta-cell based on the individual analysis of the physiological insulin- glucose relationship. *Endokrinologie* 71:65-75, 1978.
61. Salzsieder E, Albrecht G, Fischer U, and Freyse E-J: Kinetic modeling of the gluco-regulatory system to improve insulin therapy. *IEEE Trans Biomed Eng* 32: 846-855, 1985.
62. Brunetti P., Cobelli C., Cruciani P., Fabietti P.G., Filippucci F., Santeusano F.: A simulation study on a self-tuning portable controller of blood glucose. *Int J Artificial Organs* 16: 51-57, 1993.
63. Fischer U, Schenk W, Salzsieder E, Albrecht G, Abel P, and Freyse E-J: Does physiological blood glucose control require an adaptive strategy? *IEEE Trans Biomed Eng* 34:575-582, 1987.
64. Sorensen JT: A Physiologic Model of Glucose Metabolism in Man and its Use to Design and Assess Improved Insulin Therapies for Diabetes, Ph.D. dissertation, Dept Chemical Engineering, MIT, 1985.
65. Parker RS, Doyle FJ 3rd, Peppas NA. A model-based algorithm for blood glucose control in Type I diabetic patients. *IEEE Trans Biomed Eng*, 48:148-157, 1999.
66. Parker RS, Doyle FJ 3rd, Peppas NA. The intravenous route to blood glucose control. *IEEE Eng Med Biol*, 20:65-73, 2001.
67. Leblanc H, Chauvet D, Lombrail P, Robert JJ : Glycemic control with closed-loop intraperitoneal insulin in type I diabetes. *Diabetes Care*, 9: 124- 128, 1986.
68. Renard E: Implantable closed-loop glucose-sensing and insulin delivery: the future for insulin pump therapy, *Current Opinion in Pharmacology*, 2: 708-716, 2002.
69. Bellazzi R, Nucci G, Cobelli C: The subcutaneous route to insulin-dependent diabetes therapy: closed-loop and partially closed-loop control strategies for insulin delivery and measuring glucose concentration. *IEEE Eng Med Biol*, 20: 54-64, 2001.
70. Hovorka R, Chassin LJ, Wilinska ME, et al. Closing the loop: the ADICOL experience. *Diabetes Technol Ther.* 6: 307-318, 2004.
71. Steil GM, Rebrin K, Darwin C, Hariri F, Saad MF. Feasibility of automating insulin delivery for the treatment of type 1 diabetes. *Diabetes*, 55: 3344-3350, 2006.
72. Clarke WL and Kovatchev BP. The Artificial Pancreas: How Close We Are to Closing the Loop? *Ped Endocrinol Rev*, 4: 314-316, 2007.
73. The JDRF e-Newsletter: Emerging Technologies in Diabetes Research, September, 2006.
74. Weinzimer SA, Steil GM, Swan KL, Dziura J, Kurtz N, Tamborlane WV: Fully automated closed-loop insulin delivery versus semi-automated hybrid control in pediatric patients with type 1 diabetes using an artificial pancreas. *Diabetes Care*, 31:934-939, 2008.
75. Clarke WL, Anderson SM, Breton MD, Patek SD, Kashmer L, and Kovatchev BP. Closed-Loop Artificial Pancreas Using Subcutaneous Glucose Sensing and Insulin Delivery and a Model Predictive Control Algorithm: The Virginia Experience. *J Diabetes Sci Technol*, 3: 1031-1038, 2009.
76. Bruttomesso D, Farret A, Costa S, Marescotti MC, Vettore M, Avogaro A, Tiengo A, C. et al: Closed-Loop Artificial Pancreas Using Subcutaneous Glucose Sensing & Insulin Delivery, and a Model Predictive Control Algorithm: Preliminary Studies in Padova and Montpellier. *J Diabetes Sci Technol*, 3: 1014-1021, 2009.
77. Hovorka R, Allen JM, Elleri D, et al., Manual closed-loop insulin delivery in children and adolescents with type 1 diabetes: a phase 2 randomised crossover trial. *The Lancet*, 375: 743-751, 2010.
78. El-Khatib FH, Russell SJ, Nathan DM, Sutherland RG, Damiano ER. A Bihormonal Closed-Loop Artificial Pancreas for Type 1 Diabetes. *Science Transl Med*, 2: 27ra27, 2010.
79. Kovatchev BP & Cox DJ. Method, system, and computer program product for the evaluation of glycemic control in diabetes from self-monitoring data; U.S. Patent # 7,025,425 issued on April 11, 2006.
80. Kovatchev BP & Cox DJ. Method, system, and computer program product for the evaluation of glycemic control in diabetes from self-monitoring data; U.S. Patent # 7,874,985 B2 issued on January 25, 2011.
81. Kovatchev BP. Method, system, and computer program product for evaluation of blood glucose variability in diabetes from self-monitoring data; PCT/US2007/000370; 2007.
82. Kovatchev BP. Systems, methods and computer program codes for recognition of patterns of hyperglycemia and hypoglycemia, increased glucose variability, and ineffective self-monitoring in diabetes. PCT/US2008/0154513 A1, 2008.
83. Kovatchev BP and Breton MD. Method, System, and Computer Program Product for Visual and Quantitative Tracking of Blood Glucose Variability in

Diabetes from Self-Monitoring Data. U.S. Provisional PCT/US2009/065725, 2009.

84. International Patent Application Serial No. PCT/US2010/047711, Kovatchev, et al., "Tracking the Probability for Imminent Hypoglycemia in Diabetes from Self-Monitoring Blood Glucose (SMBG) Data", filed September 2, 2010.

85. Kovatchev BP and Breton MD. Method, system and computer program product for evaluation of insulin sensitivity, insulin/carbohydrate ratio, and insulin correction factors in diabetes from self-monitoring data; PCT/US2008/069416 and U.S. Publication Application US2010/0198520.

86. Kovatchev BP, Mendosa P, Anderson SM, Hawley JS, Ritterband LM, & Gonder-Frederick L. Effect of automated bio-behavioral feedback on the control of type 1 diabetes. *Diabetes Care*, 34:302-307, 2011

87. Kovatchev BP, Gonder-Frederick LA, Cox DJ, Clarke WL. Method, system and computer program for evaluating the accuracy of blood glucose monitoring sensors/devices, U.S. Patent # 7,815,569 issued on October 19, 2010.

88. Breton MD and Kovatchev BP. Method, system and computer program product for real-time detection of sensitivity decline in analyte sensors; PCT/US2007/082744, 2007.

89. Patek SD and Breton MD. LQG Artificial Pancreas Control System And Related Method. International Application Serial No. PCT/US2008/067723.

90. Kovatchev BP, Breton MD, and Patek SD. Method, System and Computer Program Product for CGM-Based Prevention of Hypoglycemia Risk Assessment and Smooth Reduction of Insulin. International Application Serial No. PCT/US2010/025405.

91. A. International Patent Application Serial No. PCT/US2011/029793, Kovatchev et al., entitled "Method, System, and Computer Program Product for Improving the Accuracy of Glucose Sensors Using Insulin Delivery Observation in Diabetes," filed March 24, 2011.

92. PCT/US2011/028163, Breton, et al., entitled "Method and System for the Safety, Analysis and Supervision of Insulin Pump Action and Other Modes of Insulin Delivery in Diabetes", filed March 11, 2011.

93. Kovatchev BP and Breton MD. Method, system, and computer program product for the detection of physical activity by changes in heart rate, assessment of fast changing metabolic states, and applications to closed and open control loop in diabetes. PCT/US2007/085588; 2007.

94. Kovatchev BP, Patek SD, Breton MD, and. System Coordinator and Modular Architecture for Open-Loop and Closed-Loop Control for Diabetes. PCT/US2010/036629, filed May 28, 2010.

95. Bergman RN, Ider YZ, Bowden CR, Cobelli C. Quantitative estimation of insulin sensitivity. *Am J Physiol.* 236:E667-E677, 1979.

[0034] The devices, systems, computer program products, and methods of various embodiments of the invention disclosed herein may utilize aspects disclosed in the following references, applications, publications and patents:

A. International Patent Application Serial No. PCT/US2011/029793, Kovatchev et al., entitled "Method, System, and Computer Program Product for Improving the Accuracy of Glucose Sensors Using Insulin Delivery Observation in Diabetes," filed March 24, 2011

B. PCT/US2011/028163, Breton, et al., entitled "Method and System for the Safety, Analysis and Supervision of Insulin Pump Action and Other Modes of Insulin Delivery in Diabetes", filed March 11, 2011.

C. International Patent Application Serial No. PCT/US2010/047711, Kovatchev, et al., "Tracking the Probability for Imminent Hypoglycemia in Diabetes from Self-Monitoring Blood Glucose (SMBG) Data", filed September 2, 2010.

D. International Patent Application Serial No. PCT/US2010/047386, Kovatchev, et al., "System, Method and Computer Program Product for Adjustment of Insulin Delivery (AID) in Diabetes Using Nominal Open-Loop Profiles", filed August 31, 2010.

E. International Patent Application Serial No. PCT/US2010/040097, Kovatchev, et al., "System, Method, and Computer Simulation Environment for In Silico Trials in Prediabetes and Type 2 Diabetes", filed June 25, 2010.

F. International Patent Application Serial No. PCT/US2010/036629, Kovatchev, et al., "System Coordinator and Modular Architecture for Open-Loop and Closed-Loop Control of Diabetes", filed May 28, 2010 (Publication No. WO 2010/138848, December 2, 2010).

G. International Patent Application Serial No. PCT/US2010/025405, Kovatchev, et al., entitled "Method, System and Computer Program Product for CGM-Based Prevention of Hypoglycemia via Hypoglycemia Risk Assessment and Smooth Reduction Insulin Delivery," filed February 25, 2010.

H. International Patent Application Serial No. PCT/US2009/065725, Kovatchev, et al., filed November 24, 2009, entitled "Method, System, and Computer Program Product for Tracking of Blood Glucose Variability in Diabetes from Data."

I. International Patent Application Serial No. PCT/US2008/082063, Magni, et al., entitled "Model Predictive Control Based Method for Closed-Loop Control of Insulin Delivery in Diabetes Using Continuous Glucose Sensing", filed October 31, 2008; U.S. Patent Application Serial No. 12/740,275, Magni, et al., entitled "Predictive Control Based System and Method for Control of Insulin Delivery in Diabetes Using Glucose Sensing", filed April 28, 2010.

J. International Patent Application Serial No.

PCT/US2008/069416, Breton, et al., entitled "Method, System and Computer Program Product for Evaluation of Insulin Sensitivity, Insulin/Carbohydrate Ratio, and Insulin Correction Factors in Diabetes from Self-Monitoring Data", filed July 8, 2008, (Publication No. WO 2009/009528, January 15, 2009); U.S. Patent Application Serial No. 12/665,149, Breton, et al., "Method, System and Computer Program Product for Evaluation of Insulin Sensitivity, Insulin/Carbohydrate Ratio, and Insulin Correction Factors in Diabetes from Self-Monitoring Data", filed December 17, 2009.

K. International Patent Application Serial No. PCT/US2008/067725, Kovatchev, et al., entitled "Method, System and Computer Simulation Environment for Testing of Monitoring and Control Strategies in Diabetes," filed June 20, 2008, (Publication No. WO 2008/157781, December 24, 2008); U.S. Patent Application Publication Serial No. 12/664,444, Kovatchev, et al., filed December 14, 2009, entitled "Method, System and Computer Simulation Environment for Testing of Monitoring and Control Strategies in Diabetes", (Publication No. 2010/0-179768, July 15, 2010).

L. International Patent Application Serial No. PCT/US2008/067723, Patek, et al., entitled "LQG Artificial Pancreas Control System and Related Method", filed on 6/20/2008.

M. U.S. Patent Application Serial No. 12/516,044, Kovatchev, et al., filed May 22, 2009, entitled "Method, System, and Computer Program Product for the Detection of Physical Activity by Changes in Heart Rate, Assessment of Fast Changing Metabolic States, and Applications of Closed and Open Control Loop in Diabetes".

N. International Patent Application Serial No. PCT/US2007/085588, Kovatchev, et al., filed November 27, 2007, entitled "Method, System, and Computer Program Product for the Detection of Physical Activity by Changes in Heart Rate, Assessment of Fast Changing Metabolic States, and Applications of Closed and Open Control Loop in Diabetes", (Publication No. WO2008/067284, June 5, 2008)

O. U.S. Patent Application Serial No. 11/943,226, Kovatchev, et al., filed November 20, 2007, entitled "Systems, Methods and Computer Program Codes for Recognition of Patterns of Hyperglycemia and Hypoglycemia, Increased Glucose Variability, and Ineffective Self-Monitoring in Diabetes".

P. U.S. Patent Application Serial No. 11/578,831, Kovatchev, et al., filed October 18, 2006 entitled "Method, System and Computer Program Product for Evaluating the Accuracy of Blood Glucose Monitoring Sensors/Devices", (Publication No. US2007/0232878, October 4, 2007), U.S. Patent No. 7,815,569, Kovatchev, et al., issued October 29, 2010

Q. International Application Serial No. PCT/US2005/013792, Kovatchev, et al., filed April 21, 2005, entitled "Method, System, and Computer Program Product for Evaluation of the Accuracy of Blood Glucose Monitoring Sensors/Devices", (Publication No. WO 05106017, November 10, 2005

R. International Patent Application Serial No. PCT/US01/09884, Kovatchev, et al., filed March 29 2001, entitled "Method, System, and Computer Program Product for Evaluation of Glycemic Control in Diabetes Self-Monitoring Data", (Publication No. WO 01/72208, October 4, 2001).

S. U.S. Patent Application Serial No. 10/240,228, Kovatchev, et al., filed September 26, 2002, (Publication No. 0212317, November 13, 2003), U.S. Patent No. 7,025,425 B2, Kovatchev, et al., issued April 11, 2006, entitled "Method, System, and Computer Program Product for the Evaluation of Glycemic Control in Diabetes from Self-Monitoring Data".

T. U.S. Patent Application Serial No. 11/305,946, Kovatchev, et al., filed December 19, 2005 entitled "Method, System, and Computer Program Product for the Evaluation of Glycemic Control in Diabetes from Self-Monitoring Data" (Publication No. 2006/0094947, May 4, 2006), U.S. Patent No. 7,874,985, Kovatchev, et al., issued January 25, 2011.

U. U.S. Patent Application Serial No. 12/975,580, Kovatchev, et al., "Method, System, and Computer Program Product for the Evaluation of Glycemic Control in Diabetes from Self-Monitoring Data", filed December 22, 2010.

V. International Patent Application Serial No. PCT/US2003/025053, Kovatchev, et al., filed August 8, 2003, entitled "Method, System, and Computer Program Product for the Processing of Self-Monitoring Blood Glucose (SMBG) Data to Enhance Diabetic Self-Management", (Publication No. WO 2004/015539, February 19, 2004).

W. U.S. Patent Application Serial No. 10/524,094, Kovatchev, et al., filed February 9, 2005 entitled "Managing and Processing Self-Monitoring Blood Glucose" (Publication No. 2005/214892, September 29, 2005).

X. U.S. Patent Application Serial No. 12/065,257, Kovatchev, et al., filed August 29, 2008, entitled "Accuracy of Continuous Glucose Sensors", (Publication No. 2008/0314395, December 25, 2008).

Y. International Patent Application Serial No. PCT/US2006/033724, Kovatchev, et al., filed August 29, 2006, entitled "Method for Improving Accuracy of Continuous Glucose Sensors and a Continuous Glucose Sensor Using the Same", (Publication No. WO 07027691, March 8, 2007).

Z. U.S. Patent Application Serial No. 12/159,891, Kovatchev, B., filed July 2, 2008, entitled "Method, System and Computer Program Product for Evaluation of Blood Glucose Variability in Diabetes from Self-

Monitoring Data", (Publication No. 2009/0171589, July 2, 2009).

AA. International Application No. PCT/US2007/000370, Kovatchev, B., filed January 5, 2007, entitled "Method, System and Computer Program Product for Evaluation of Blood Glucose Variability in Diabetes from Self-Monitoring Data", (Publication No. WO 07081853, July 19, 2007).

BB. U.S. Patent Application Serial No. 11/925,689 and PCT International Patent Application No. PCT/US2007/082744, Breton, et al., both filed October 26, 2007, entitled "For Method, System and Computer Program Product for Real-Time Detection of Sensitivity Decline in Analyte Sensors", (Publication Nos. 2008/0172205, July 17, 2008 and WO 2008/052199, May 2, 2008).

CC. U.S. Patent Application Serial No. 10/069,674, Kovatchev, et al., filed February 22, 2002, entitled "Method and Apparatus for Predicting the Risk of Hypoglycemia".

DD. International Application No. PCT/US00/22886, Kovatchev, et al., filed August 21, 2000, entitled "Method and Apparatus for Predicting the Risk of Hypoglycemia", (Publication No. WO 01/13786, March 1, 2001).

EE. U.S. Patent Application Serial No. 6,923,763 B1, Kovatchev, et al., issued August 2, 2005, entitled "Method and Apparatus for Predicting the Risk of Hypoglycemia".

FF. U.S. Patent Application Publication No. US 2004/0254434 A1, "Glucose Measuring Module and "Insulin Pump Combination", published December 16, 2004., Goodnow, et al. Serial No. 10/458,914, filed June 10, 2003.

GG. U.S. Patent Application Publication No. US 2009/00697456 A1, Estes, et al., "Operating an Infusion Pump System", published March 12, 2009. Serial No. 11/851,194, September 6, 2007.

HH. Fernandez-Luque, et al., eDiab: A System for Monitoring, Assisting and Educating People with Diabetes", ICCHP 2006, LNCS 4061, pp. 1342-1349, 2006.

II. U.S. Patent No. 6,602,191 B2, Quy, R., Method and Apparatus for Health and Disease Management Combining Patient Data Monitoring with Wireless Internet Connectivity, August 5, 2003.

JJ. International Patent Application Publication No. WO 2008/064053 A2, Patel, et al., Systems and Methods for Diabetes Management Using Consumer Electronic Devices, May 29, 2008; International Patent Application Serial No. PCT/US2007/084769, filed November 15, 2007.

KK. International Patent Application Publication No. WO 2010/138817 A1, Ow-Wing, K., Glucose Monitoring System with Wireless Communications, December 2, 2010; International Patent Application Serial No. WO 2010/138817 A1, filed May 28, 2010.

LL. International Patent Application Publication No.

WO 2004/052204 A1, Kim, Kwan-Ho, Blood Glucose Monitoring System, June 24, 2004; International Patent Application Serial No. PCT/KR2003/000398, filed February 28, 2003.

Claims

1. A system for managing glycemic control of a patient, comprising:

an input module configured to accept input data from one or more of a plurality of diverse blood glucose measurement devices and one or more of a plurality of diverse insulin delivery devices; a data classifier module configured to assess the frequency, dimensionality and quality of data accepted by said input module to classify said input data and to determine appropriate processing of said input data according to its classification;

a patient state estimation module configured to process input data in accordance with at least one data processing algorithm corresponding to the classification of the input data as determined by the data classifier module;

a patient risk status module configured to determine a level of risk of said patient with respect to abnormal glycemic states using processed data from said patient state estimation module; and

an output module configured to output advisory messages, patient alerts, and control signals for said blood glucose measurement devices and said insulin delivery devices based on the level of risk determined by said patient risk status module.

2. A system as set forth in claim 1, wherein said input data is classified as one of SMBG data, SMBG plus insulin pump data, CGM data, or CGM plus insulin pump data.

3. A system as set forth in claim 1, wherein said input module is further configured to receive data from at least one of a heart rate sensor, a blood pressure sensor, an accelerometer sensor, and a ECG/EKG sensor.

4. A system as set forth in claim 1, wherein said input module is further configured to receive data from a plurality of different physiological sensors for said patient, said plurality of sensors forming a body sensor network.

5. A system as set forth in claim 1, further comprising a telecommunications module configured to communicate patient status data to at least one of a remote

health care provider, an emergency responder, and a public health care organization.

6. A system as set forth in claim 1 wherein said diverse insulin delivery devices comprise a multiple daily insulin injection pump and a continuous subcutaneous insulin injection pump, the system further comprising a safety service module configured to analyze data from at least one of said insulin injection pumps and to determine an operational state of said pump from said data analysis.
7. A system as set forth in claim 6, wherein said safety service module is further configured to screen insulin bolus commands for safety prior to said commands being delivered to an insulin injection pump.
8. A system as set forth in claim 1, wherein said control signals are configured to cause monitoring of said patient to be modified from a current level of monitoring to a higher level of monitoring in dependence on a determined risk status of said patient and a determination of data quality and/or density.
9. A system as set forth in claim 1, wherein said control signals are configured to carry out closed-loop control of insulin delivery to said patient in dependence on a determined risk status of said patient.
10. A method for managing glycemic control of a patient, comprising:
- accepting at an input module input data from one or more of a plurality of diverse blood glucose measurement devices and one or more of a plurality of diverse insulin delivery devices; assessing the frequency, dimensionality and quality of data accepted by said input module to classify said input data and to determine appropriate processing of said input data according to its classification; processing input data in accordance with at least one data processing algorithm corresponding to the classification of the input data as determined by the data classifier module; determining a level of risk of said patient with respect to abnormal glycemic states using processed data from said patient state estimation module; and outputting from an output module advisory messages and patient alerts based on the level of risk determined by said patient risk status module.
11. A method as set forth in claim 10, further comprising receiving data from at least one of a heart rate sensor, a blood pressure sensor, an accelerometer sensor, and an ECG/EKG sensor.

12. A method as set forth in claim 10, further comprising receiving data from a plurality of different physiological sensors for said patient, said plurality of sensors forming a body sensor network.
13. A method as set forth in claim 10, further comprising communicating patient status data to at least one of a remote health care provider, an emergency responder, and a public health care organization over a telecommunications network.
14. A method as set forth in claim 10 wherein said diverse insulin delivery devices comprise a multiple daily insulin injection pump and a continuous subcutaneous insulin injection pump, further comprising analyzing data from at least one of said insulin injection pumps and determining an operational state of said pump from said data analysis.
15. A method as set forth in claim 10, wherein the method further comprises outputting control signals causing monitoring of said patient to be modified from a current level of monitoring to a higher level of monitoring in dependence on a determined risk status of said patient and a determination of data quality and/or density.

Patentansprüche

1. System zur Steuerung der Blutzuckerkontrolle eines Patienten, umfassend:
- Eingabemodul, das konfiguriert ist, Eingabedaten von einer oder mehreren einer Vielzahl von verschiedenen Blutzuckermessvorrichtungen und einer oder mehreren einer Vielzahl von verschiedenen Insulinabgabevorrichtungen zu akzeptieren;
- Datenklassifizieremodul, das konfiguriert ist, die Häufigkeit, Dimensionalität und Qualität von Daten zu bewerten, die von dem Eingabemodul akzeptiert werden, um die Eingabedaten zu klassifizieren und um eine geeignete Verarbeitung der Eingabedaten gemäß ihrer Klassifizierung zu bestimmen;
- Patientenzustandsschätzmodul, das konfiguriert ist, Eingabedaten in Übereinstimmung mit mindestens einem Datenverarbeitungsalgorithmus entsprechend der Klassifizierung der Eingabedaten, wie durch das Datenklassifizieremodul bestimmt, zu verarbeiten;
- Patientenrisikozustandsmodul, das zum Bestimmen eines Risikozustands des Patienten in Bezug auf anormale Blutzuckerzustände unter Verwendung verarbeiteter Daten von dem Patientenzustandsschätzmodul konfiguriert ist; und

- Ausgabemodul, das konfiguriert ist, ratschlaggebende Mitteilungen, Patientenalarne und Steuersignale für die Blutzuckermessvorrichtungen und die Insulinzuführungsvorrichtungen basierend auf dem Risikoniveau, das von dem Patientenrisikozustandsmodul bestimmt wird, auszugeben.
2. System nach Anspruch 1, wobei die Eingabedaten von einem von SMBG-Daten, SMBG plus-Insulinpumpendaten, CGM-Daten oder CGM plus-Insulinpumpendaten klassifiziert werden.
 3. System nach Anspruch 1, wobei das Eingabemodul ferner konfiguriert ist, Daten von mindestens einem von einem Herzfrequenzsensor, einem Blutdrucksensor, einem Beschleunigungsmess-Sensor und einem ECG/EKG-Sensor zu empfangen.
 4. System nach Anspruch 1, wobei das Eingabemodul ferner konfiguriert ist, Daten von einer Vielzahl von verschiedenen physiologischen Sensoren des Patienten zu empfangen, wobei die Vielzahl von Sensoren ein Körpersensornetzwerk bildet.
 5. System nach Anspruch 1, ferner umfassend ein Telekommunikationsmodul, das konfiguriert ist, Patientenzustandsdaten an mindestens einen von einem entfernten Gesundheitsdienstleister, einem Notfallhelfer und einer öffentlichen Gesundheitsdienstleistungsorganisation zu übermitteln.
 6. System nach Anspruch 1, wobei die verschiedenen Insulinabgabevorrichtungen eine Insulineinspritzpumpe für mehrfache tägliche Abgaben und eine subkutane Insulineinspritzpumpe für kontinuierliche Abgaben umfassen, wobei das System ferner ein Sicherheitsservicemodul umfasst, das zum Analysieren von Daten von mindestens einer der Insulineinspritzpumpen konfiguriert ist und um aus der Datenanalyse einen Betriebszustand der Pumpe zu bestimmen.
 7. System nach Anspruch 6, wobei das Sicherheitsservicemodul ferner konfiguriert ist, Insulinbolusbefehle aus Sicherheitsgründen zu überprüfen, bevor die Befehle an eine Insulineinspritzpumpe abgegeben werden.
 8. System nach Anspruch 1, wobei die Steuersignale konfiguriert sind, zu bewirken, dass die Überwachung des Patienten von einem aktuellen Überwachungsniveau auf ein höheres Überwachungsniveau, in Abhängigkeit von einem bestimmten Risikozustand des Patienten und einer Bestimmung der Datenqualität und/oder Dichte, geändert wird.
 9. System nach Anspruch 1, wobei die Steuersignale
- konfiguriert sind, eine Regelung der Insulinabgabe an den Patienten mit Rückkopplung, in Abhängigkeit von einem bestimmten Risikozustand des Patienten, durchzuführen.
10. Verfahren zur Steuerung der Blutzuckerkontrolle eines Patienten, umfassend:
 - Akzeptieren von Eingabedaten von einer oder mehreren einer Vielzahl von verschiedenen Blutzuckermessvorrichtungen und einer oder mehreren einer Vielzahl von verschiedenen Insulinabgabevorrichtungen an einem Eingabemodul;
 - Bewerten der Häufigkeit, Dimensionalität und Qualität von Daten, die von dem Eingabemodul akzeptiert werden, um die Eingabedaten zu klassifizieren und um eine geeignete Verarbeitung der Eingabedaten entsprechend ihrer Klassifizierung zu bestimmen;
 - Verarbeiten von Eingabedaten in Übereinstimmung mit mindestens einem Datenverarbeitungsalgorithmus entsprechend der Klassifizierung der Eingabedaten, wie diese durch das Datenklassifizieremodul bestimmt werden;
 - Bestimmen eines Risikoniveaus des Patienten in Bezug auf anomale Blutzuckerzustände unter Verwendung verarbeiteter Daten von dem Patientenzustandsschätzungsmodul; und
 - Ausgeben von ratschlaggebenden Mitteilungen und Patientenalarmen von einem Ausgabemodul basierend auf dem Risikoniveau, das durch das Patientenrisikozustandsmodul bestimmt wird.
 11. Verfahren nach Anspruch 10, ferner umfassend das Empfangen von Daten von mindestens einem von einem Herzfrequenzsensor, einem Blutdrucksensor, einem Beschleunigungsmess-Sensor und einem ECG/EKG-Sensor.
 12. Verfahren nach Anspruch 10, ferner umfassend das Empfangen von Daten von einer Vielzahl von verschiedenen physiologischen Sensoren für Patienten, wobei die Vielzahl von Sensoren ein Körpersensornetzwerk bildet.
 13. Verfahren nach Anspruch 10, ferner umfassend das Übermitteln von Patientenzustandsdaten an mindestens einen von einem entfernten Gesundheitsdienstleister, einem Notfallhelfer und einer öffentlichen Gesundheitsdienstleistungsorganisation über ein Telekommunikationsnetzwerk.
 14. Verfahren nach Anspruch 10, wobei die verschiedenen Insulinabgabevorrichtungen eine Insulineinspritzpumpe für mehrfache tägliche Abgaben und eine subkutane Insulineinspritzpumpe für kontinuier-

liche Abgaben umfassen, ferner umfassend das Analysieren von Daten von mindestens einer der Insulineinspritzpumpen und das Bestimmen eines Betriebszustands der Pumpe aus besagter Datenanalyse.

15. Verfahren nach Anspruch 10, wobei das Verfahren ferner das Ausgeben von Kontrollsignalen zum Veranlassen der Änderung der Überwachung des Patienten von einem aktuellen Überwachungsniveau auf ein höheres Überwachungsniveau, in Abhängigkeit von einem bestimmten Risikozustand des Patienten und einer Bestimmung der Datenqualität und/oder Dichte, umfasst.

Revendications

1. Système pour la gestion du contrôle glycémique d'un patient, comprenant :

un module d'entrée configuré pour accepter des données d'entrée depuis un ou plusieurs parmi une pluralité de différents dispositifs pour la mesure de glycémie et un ou plusieurs parmi une pluralité de différents dispositifs d'administration d'insuline ;

un module classificateur de données configuré pour l'évaluation de la fréquence, de la dimensionnalité et de la qualité de données acceptées par ledit module d'entrée pour classifier lesdites données d'entrée et pour déterminer un traitement adéquat desdites données d'entrée selon leur classification ;

un module d'estimation d'état du patient configuré pour traiter des données d'entrée selon au moins un algorithme de traitement de données correspondant à la classification des données d'entrée telle que déterminée par le module classificateur de données ;

un module du statut de risque pour le patient configuré pour déterminer un niveau de risque dudit patient par rapport aux états anormaux de glycémie à l'aide de données traitées dudit module d'estimation d'état du patient ; et

un module de sortie configuré pour émettre des messages consultatifs, des alertes pour les patients et des signaux de commande pour lesdits dispositifs de mesure de glycémie et pour lesdits dispositifs d'administration d'insuline sur base du niveau de risque déterminé par ledit module du statut de risque pour le patient.

2. Système selon la revendication 1, dans lequel lesdites données d'entrée sont classifiées selon un groupe de données parmi les données SMBG, les données SMBG et de la pompe à insuline, les données de CGM, ou les données de CGM et de la pom-

pe à insuline.

3. Système selon la revendication 1, dans lequel ledit module d'entrée est en outre configuré pour recevoir des données d'au moins un parmi un capteur du rythme cardiaque, un capteur de pression sanguine, un capteur accélérométrique et un capteur ECG/EKG.

4. Système selon la revendication 1, dans lequel ledit module d'entrée est en outre configuré pour recevoir des données depuis une pluralité de différents capteurs physiologiques pour ledit patient, ladite pluralité de capteurs formant un réseau de capteurs corporels.

5. Système selon la revendication 1, comprenant en outre un module de télécommunications configuré pour communiquer les données d'état du patient à au moins un parmi un fournisseur à distance de soins de santé, un répondeur d'urgence et une organisation publique de soins de santé.

6. Système selon la revendication 1, dans lequel lesdits différents dispositifs d'administration d'insuline comprennent une pompe à injection d'insuline multiple quotidienne et une pompe à injection d'insuline sous-cutanée continue, le système comprenant en outre un module de service de sécurité configuré pour analyser des données d'au moins un parmi lesdites pompes à injection d'insuline et pour déterminer un état fonctionnel de ladite pompe à partir de ladite analyse de données.

7. Système selon la revendication 6, dans lequel ledit module de service de sécurité est en outre configuré pour contrôler des commandes du bolus d'insuline pour des raisons de sécurité avant que lesdites commandes soient transmises à une pompe à injection d'insuline.

8. Système selon la revendication 1, dans lequel lesdits signaux de commande sont configurés pour provoquer la modification de la surveillance dudit patient d'un niveau actuel de surveillance à un niveau supérieur de surveillance en fonction d'un état déterminé de risque dudit patient et une détermination des densité et/ou qualité des données.

9. Système selon la revendication 1, dans lequel lesdits signaux de commande sont configurés pour exécuter une commande en circuit fermé d'administration d'insuline audit patient en fonction d'un état déterminé de risque dudit patient.

10. Procédé pour la gestion du contrôle glycémique d'un patient, comprenant :

l'acceptation au niveau d'un module d'entrée,

- de données d'entrée depuis un ou plusieurs parmi une pluralité de différents dispositifs pour la mesure de glycémie et un ou plusieurs d'une pluralité de différents dispositifs d'administration d'insuline ; 5
- l'évaluation de la fréquence, de la dimensionnalité et de la qualité de données acceptées par ledit module d'entrée pour classifier lesdites données d'entrée et pour déterminer le traitement adéquat desdites données d'entrée selon leur classification ; 10
- le traitement de données d'entrée selon au moins un algorithme de traitement de données correspondant à la classification des données d'entrée telle que déterminée par le module classificateur de données ; 15
- la détermination d'un niveau de risque dudit patient par rapport aux états anormaux de glycémie à l'aide de données traitées dudit module d'estimation d'état du patient ; et 20
- l'émission à partir de messages consultatifs du module de sortie et d'alertes pour les patients sur base du niveau de risque déterminé par ledit module du statut de risque pour le patient. 25
- 11.** Procédé selon la revendication 10, comprenant en outre la réception de données d'au moins un parmi un capteur du rythme cardiaque, un capteur de pression sanguine, un capteur accélérométrique et un capteur ECG/EKG. 30
- 12.** Procédé selon la revendication 10, comprenant en outre la réception de données depuis une pluralité de différents capteurs physiologiques pour ledit patient, ladite pluralité de capteurs formant un réseau de capteurs corporels. 35
- 13.** Procédé selon la revendication 10, comprenant en outre la communication de données d'état du patient à au moins un parmi un fournisseur à distance de soins de santé, un répondeur d'urgence et une organisation publique de soins de santé sur un réseau de télécommunications. 40
- 14.** Procédé selon la revendication 10, dans lequel lesdits différents dispositifs d'administration d'insuline comprennent une pompe à injection d'insuline multiple quotidienne et une pompe à injection d'insuline sous-cutanée continue, comprenant en outre l'analyse de données d'au moins un parmi lesdites pompes à injection d'insuline et la détermination d'un état fonctionnel de ladite pompe à partir de ladite analyse de données. 45 50
- 15.** Procédé selon la revendication 10, dans lequel le procédé comprend en outre l'émission de signaux de commande provoquant la modification de la surveillance dudit patient d'un niveau actuel de sur- 55
- veillance à un niveau supérieur de surveillance en fonction d'un état déterminé de risque dudit patient et une détermination des densité et/ou qualité des données.

Figure 1: DiAs Inputs and Outputs

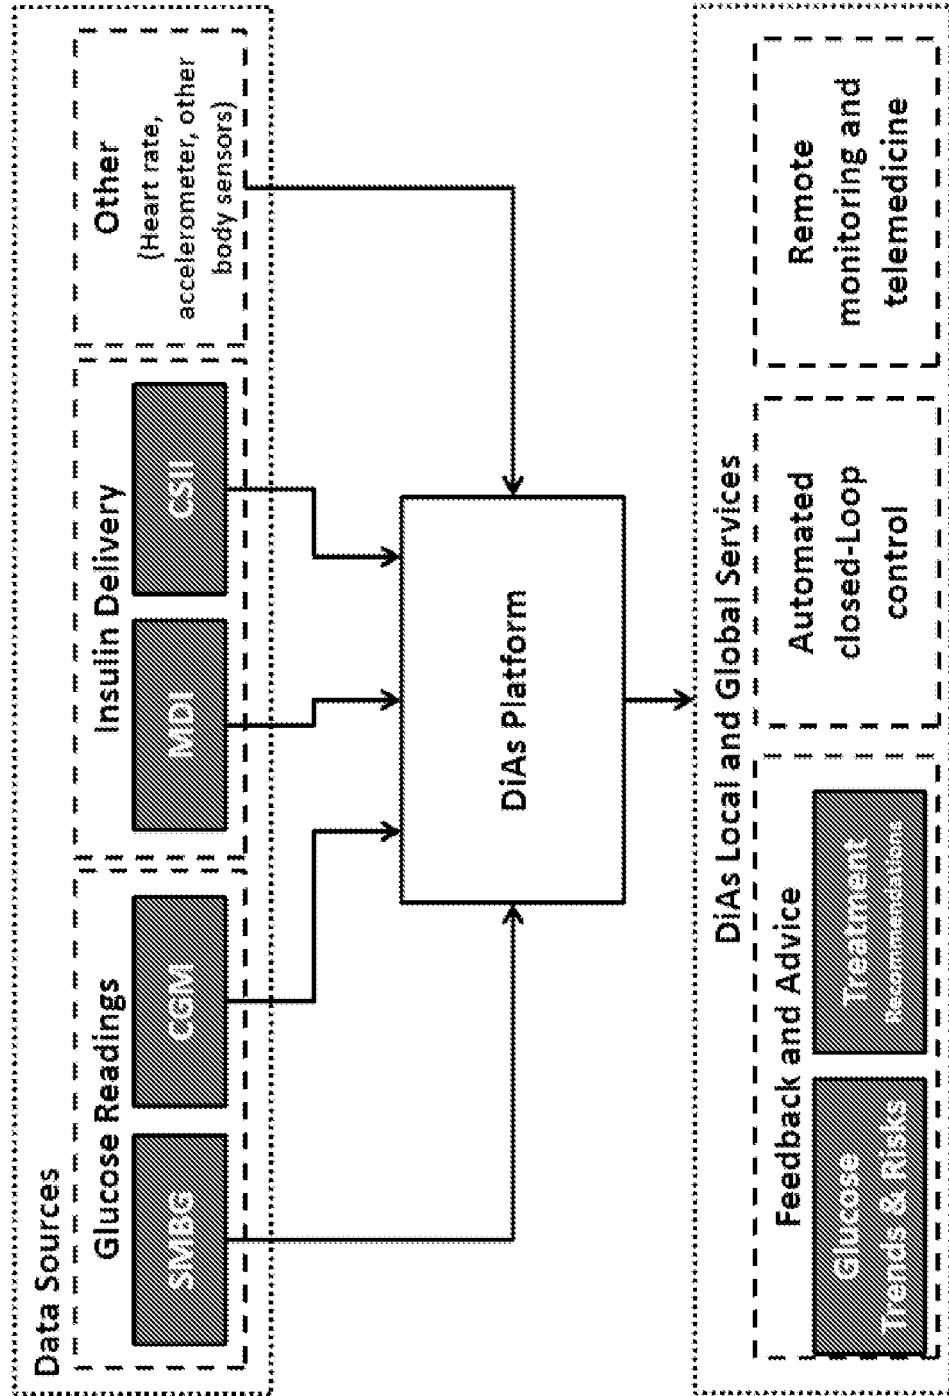


Figure 2: DiAs Processes and Services

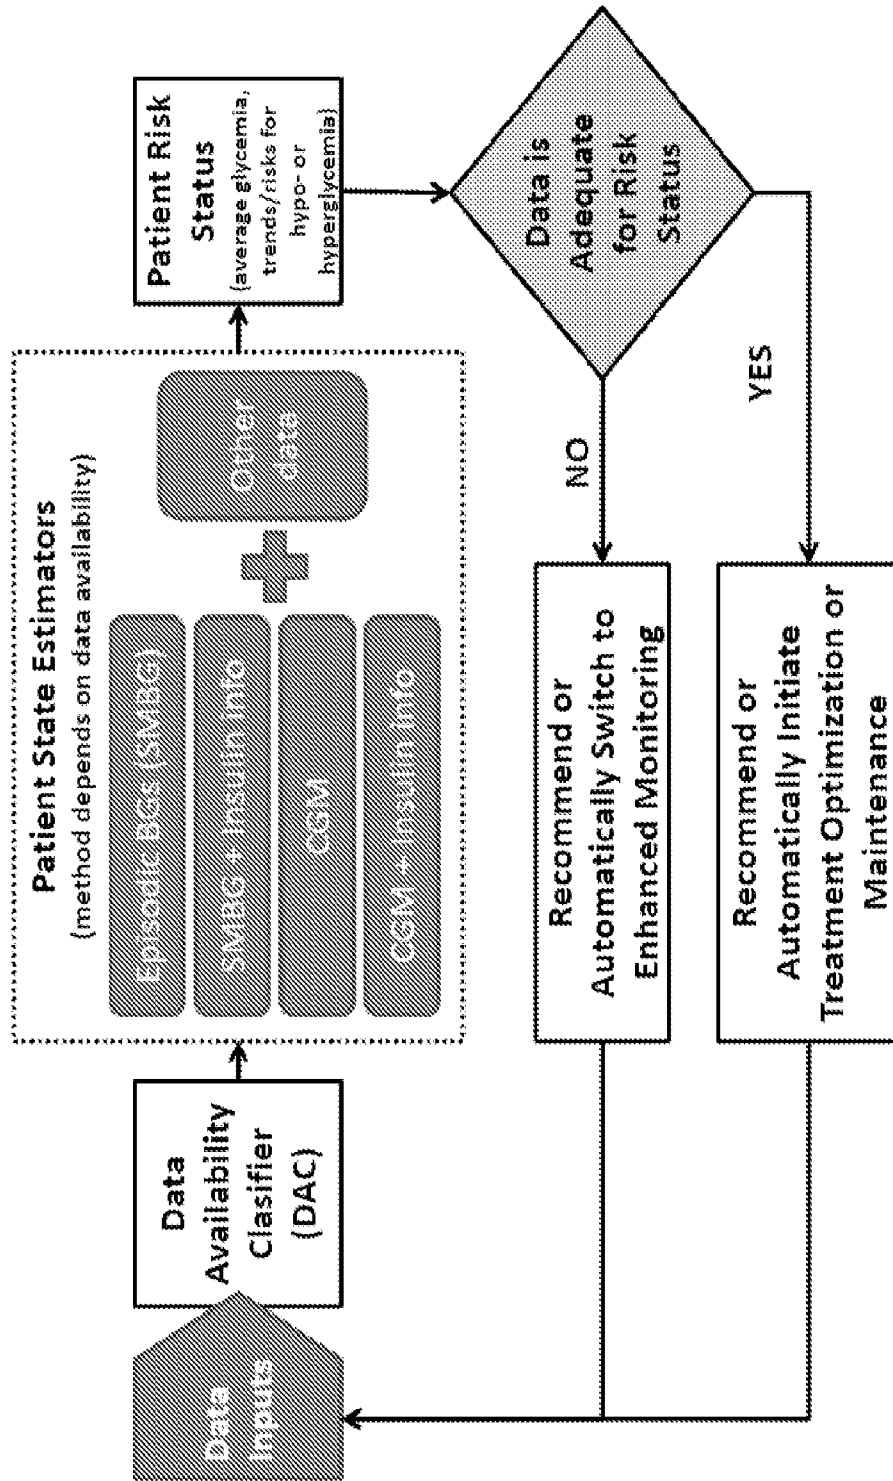


Figure 4: Implementation of DiAs on a Cell Phone Platform

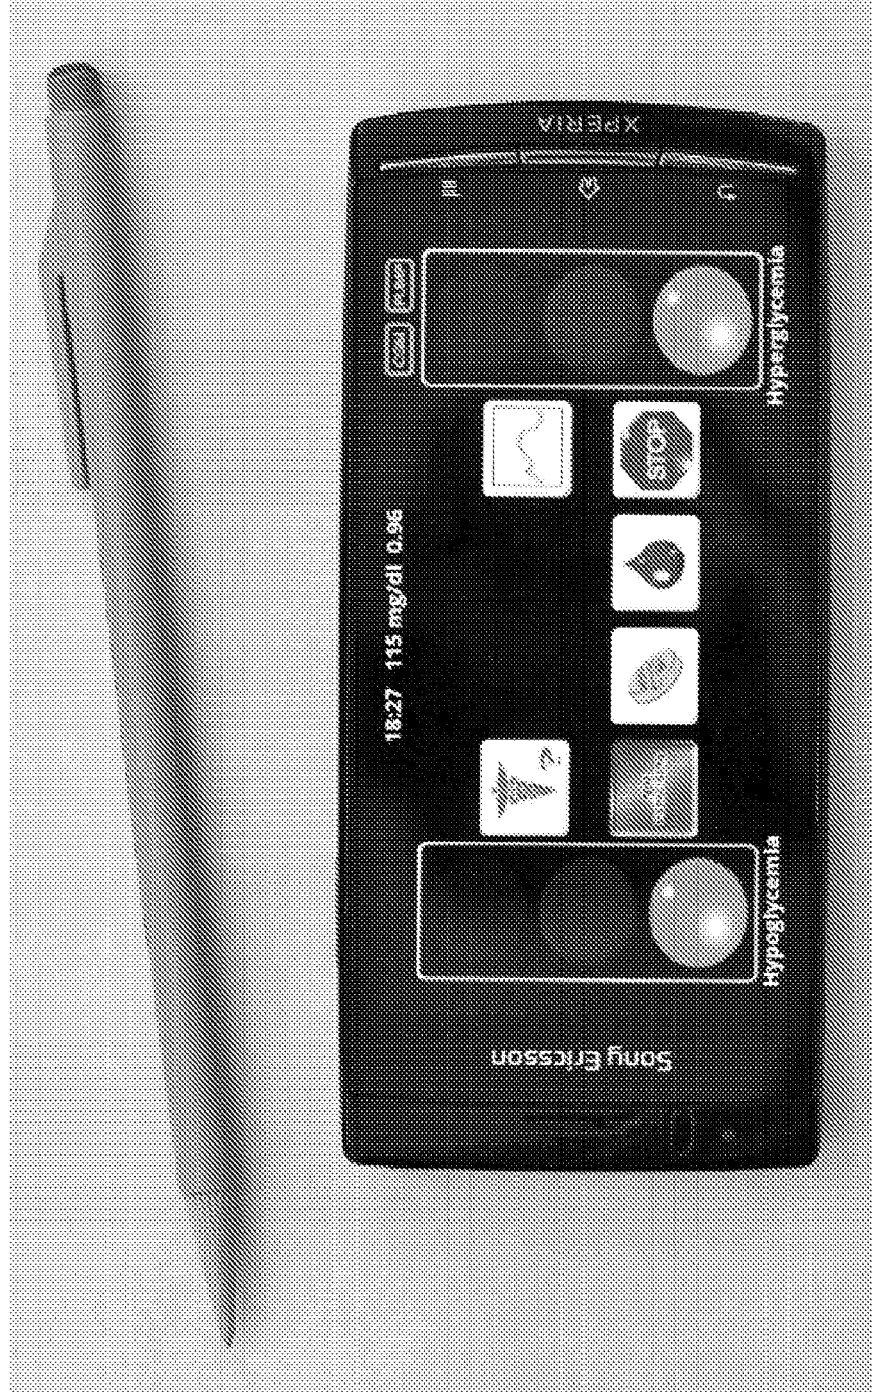
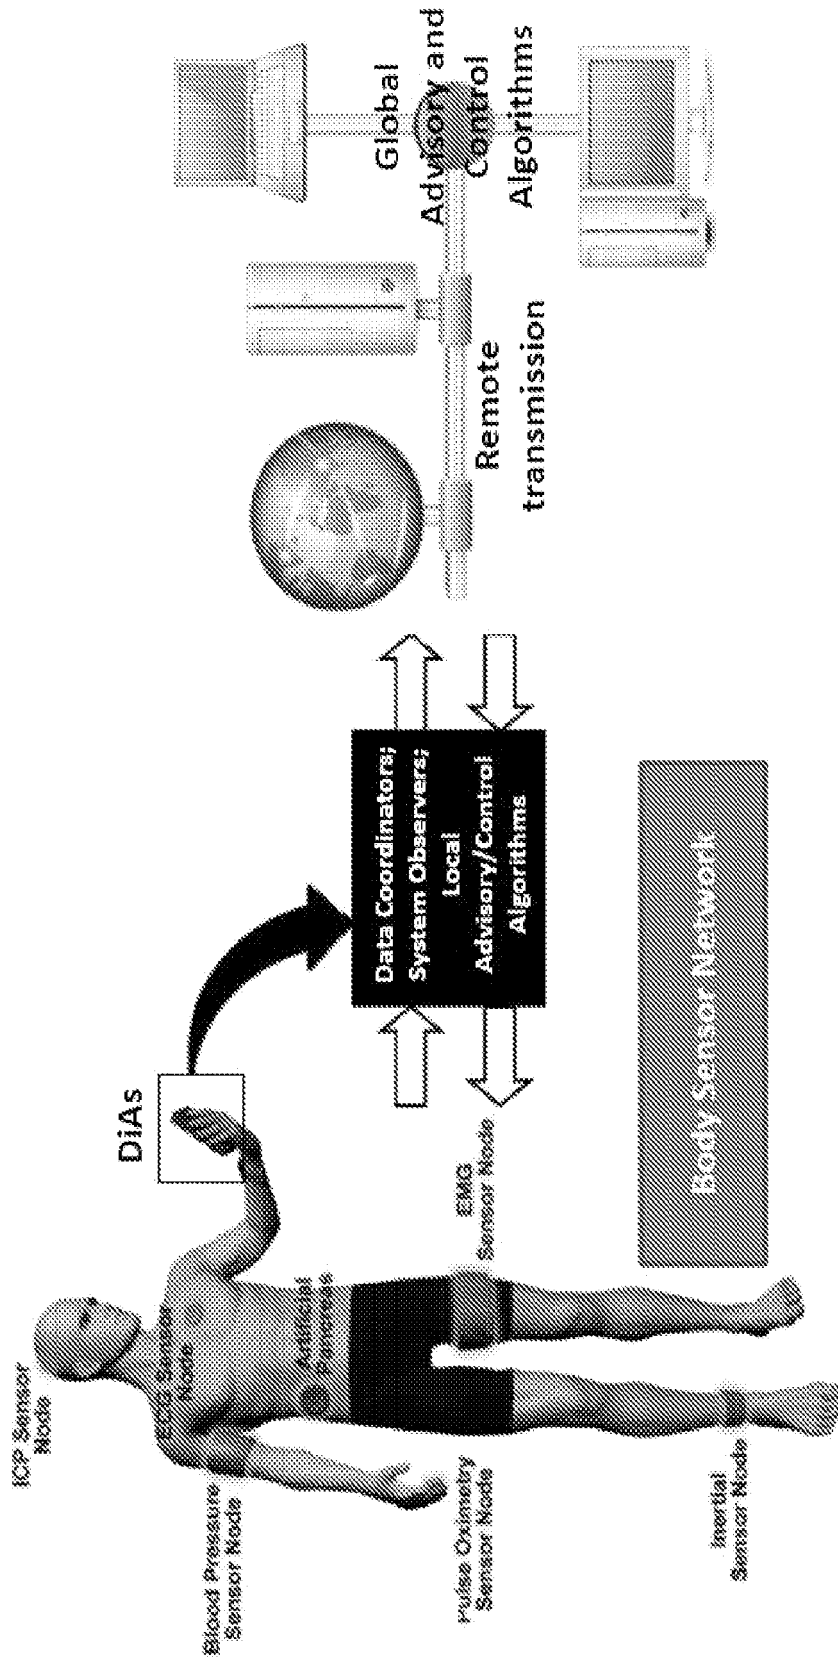


Figure 5: Implementation of DiAs - Hub for Body Sensor Network



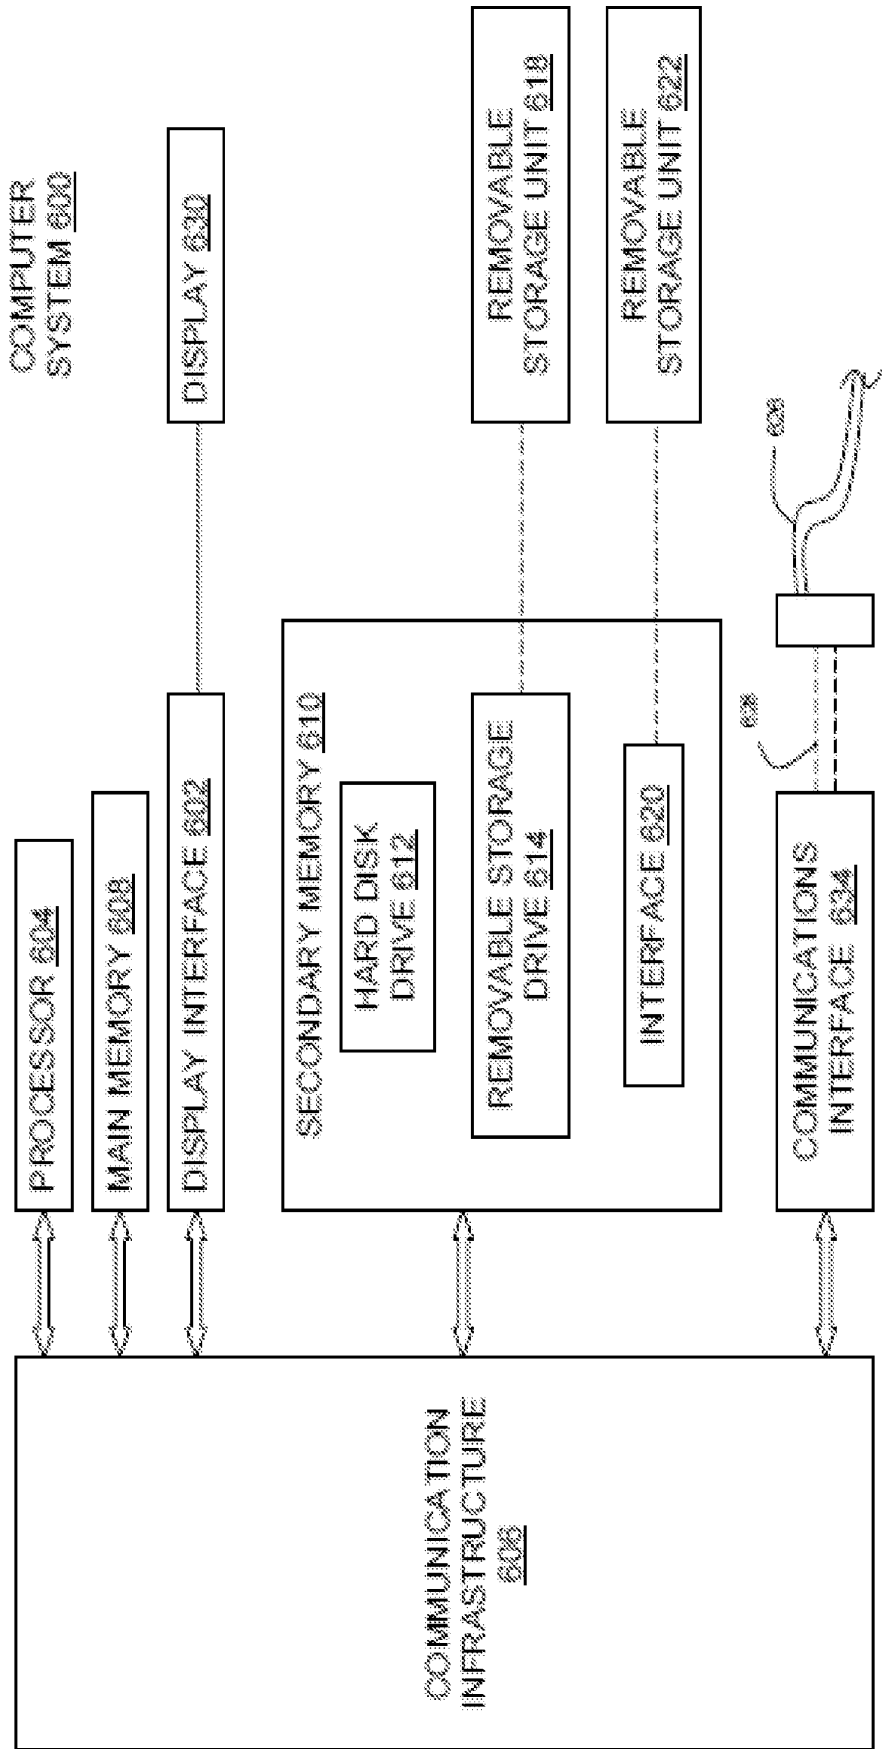


FIG. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2009006129 A [0011]
- US 2010185175 A [0012]
- US 7025425 B [0033]
- US 7874985 B2 [0033]
- US 2007000370 W [0033] [0034]
- US 20080154513A1 W [0033]
- US 2009065725 W [0033] [0034]
- US 2010047711 W, Kovatchev [0033] [0034]
- US 2008069416 W [0033] [0034]
- US 20100198520 A [0033]
- US 7815569 B [0033] [0034]
- US 2007082744 W [0033] [0034]
- US 2008067723 W [0033] [0034]
- US 2010025405 W [0033] [0034]
- US 2011029793 W, Kovatchev [0033] [0034]
- US 2011028163 W, Breton [0033] [0034]
- US 2007085588 W [0033] [0034]
- US 2010036629 W [0033] [0034]
- US 2010047386 W, Kovatchev [0034]
- US 2010040097 W, Kovatchev [0034]
- WO 2010138848 A [0034]
- US 2008082063 W, Magni [0034]
- US 74027510 A, Magni [0034]
- WO 2009009528 A [0034]
- US 66514909 A, Breton [0034]
- US 2008067725 W, Kovatchev [0034]
- WO 2008157781 A [0034]
- US 66444409 A, Kovatchev [0034]
- US 20100179768 A [0034]
- US 51604409 A, Kovatchev [0034]
- WO 2008067284 A [0034]
- US 94322607 A, Kovatchev [0034]
- US 57883106 A, Kovatchev [0034]
- US 20070232878 A [0034]
- US 2005013792 W, Kovatchev [0034]
- WO 05106017 A [0034]
- US 0109884 W, Kovatchev [0034]
- WO 0172208 A [0034]
- US 24022802 A, Kovatchev [0034]
- US 0212317 A [0034]
- US 7025425 B2, Kovatchev [0034]
- US 30594605 A, Kovatchev [0034]
- US 20060094947 A [0034]
- US 7874985 B, Kovatchev [0034]
- US 97558010 A, Kovatchev [0034]
- US 2003025053 W, Kovatchev [0034]
- WO 2004015539 A [0034]
- US 52409405 A, Kovatchev [0034]
- US 2005214892 A [0034]
- US 06525708 A, Kovatchev [0034]
- US 20080314395 A [0034]
- US 2006033724 W, Kovatchev [0034]
- WO 07027691 A [0034]
- US 15989108 A, Kovatchev, B. [0034]
- US 20090171589 A [0034]
- WO 07081853 A [0034]
- US 925689 A [0034]
- US 20080172205 A [0034]
- WO 2008052199 A [0034]
- US 06967402 A, Kovatchev [0034]
- US 0022886 W, Kovatchev [0034]
- WO 0113786 A [0034]
- US 6923763 B1, Kovatchev [0034]
- US 20040254434 A1 [0034]
- US 10458914 B [0034]
- US 200900697456 A1, Estes [0034]
- US 11851194 B [0034]
- US 6602191 B2, Quy, R. [0034]
- WO 2008064053 A2, Patel [0034]
- US 2007084769 W [0034]
- WO 2010138817 A1, Ow-Wing, K. [0034]
- WO 2004052204 A1, Kim, Kwan-Ho [0034]
- KR 2003000398 W [0034]

Non-patent literature cited in the description

- **REICHARD P ; PHIL M.** Mortality and treatment side effects during long-term intensified conventional insulin treatment in the Stockholm Diabetes Intervention study. *Diabetes*, 1994, vol. 43, 313-317 [0033]
- The Diabetes Control and Complications Trial Research Group. The effect of intensive treatment of diabetes on the development and progression of long-term complications of insulin-dependent diabetes mellitus. *N Engl J Med*, 1993, vol. 329, 978-986 [0033]

- UK Prospective Diabetes Study Group (UKPDS). Intensive blood-glucose control with sulphonylureas or insulin compared with conventional treatment and risk of complications in patients with type 2 diabetes. *Lancet*, 1998, vol. 352, 837-853 [0033]
- **CRYER PE.** Hypoglycaemia: The limiting factor in the glycaemic management of type I and type II diabetes. *Diabetologia*, 2002, vol. 45, 937-948 [0033]
- **CRYER PE.** Hypoglycemia: The Limiting factor in the management of IDDM. *Diabetes*, 1994, vol. 43, 1378-1389 [0033]
- **CLARKE WL ; COX D ; GONDER-FREDERICK LA ; CARTER W ; POHL SL.** Evaluating the clinical accuracy of self-blood glucose monitoring systems. *Diabetes Care*, 1987, vol. 10, 622-628 [0033]
- The diabetes research in children network (DirecNet) study group. A multicenter study of the accuracy of the One Touch® Ultra® home glucose meter in children with Type 1 diabetes. *Diabetes Technol Ther*, 2003, vol. 5, 933-942 [0033]
- **KOVATCHEV BP ; COX DJ ; GONDER-FREDERICK LA YOUNG-HYMAN D ; SCHLUNDT D ; CLARKE WL.** Assessment of risk for severe hypoglycemia among adults with IDDM: Validation of the Low Blood Glucose Index. *Diabetes Care*, 1998, vol. 21, 1870-1875 [0033]
- **COX DJ ; KOVATCHEV B ; JULIAN D ; GONDER-FREDERICK LA ; POLONSKY WH ; SCHLUNDT DG ; CLARKE WL.** Frequency of severe hypoglycemia in IDDM can be predicted from self-monitoring blood glucose data. *J Clin Endocrinol Metab*, 1994, vol. 79, 1659-1662 [0033]
- **KOVATCHEV BP ; COX DJ ; KUMAR A ; GONDER-FREDERICK LA AND WL CLARKE.** Algorithmic Evaluation of Metabolic Control and Risk of Severe Hypoglycemia in Type 1 and Type 2 Diabetes Using Self-Monitoring Blood Glucose (SMBG) Data. *Diabetes Technol Ther*, 2003, vol. 5 (5), 817-828 [0033]
- **COX DJ ; GONDER-FREDERICK LA ; RITTER-BAND L ; CLARKE WL ; KOVATCHEV BP.** Prediction of Severe Hypoglycemia. *Diabetes Care*, 2007, vol. 30, 1370-1373 [0033]
- **KOVATCHEV BP ; COX DJ ; FARHY LS ; STRAUME M ; GONDER-FREDERICK LA ; CLARKE, WL.** Episodes of Severe Hypoglycemia in Type 1 Diabetes are Preceded, and Followed, within 48 Hours by Measurable Disturbances in Blood Glucose. *J Clin Endocrinol Metab*, 2000, vol. 85, 4287-4292 [0033]
- **KOVATCHEV BP ; STRAUME M ; COX DJ ; FARHY LS.** Risk analysis of blood glucose data: A quantitative approach to optimizing the control of insulin dependent diabetes. *J of Theoretical Medicine*, 2001, vol. 3, 1-10 [0033]
- **KOVATCHEV BP ; COX DJ ; GONDER-FREDERICK LA ; WL CLARKE.** Symmetrization of the blood glucose measurement scale and its applications. *Diabetes Care*, 1997, vol. 20, 1655-1658 [0033]
- **MASTROTOTARO J.J.** The MiniMed Continuous Glucose Monitoring System. *Diabetes Technol Ther*, 2000, vol. 2 (1), S-13-S-18 [0033]
- **BODE B.W.** Clinical Utility of the Continuous Glucose Monitoring System. *Diabetes Technol Ther*, 2000, vol. 2 (1), S-35-S-42 [0033]
- **FELDMAN B ; BRAZG R ; SCHWARTZ S ; WEINSTEIN R.** A continuous glucose sensor based on wired enzyme technology - results from a 3-day trial in patients with Type 1 diabetes. *Diabetes Technol Ther*, 2003, vol. 5, 769-778 [0033]
- The diabetes research in children network (DirecNet) study group. The accuracy of the CGMS™ in children with Type 1 diabetes: Results of the diabetes research in children network (DirecNet) accuracy study. *Diabetes Technol Ther*, 2003, vol. 5, 781-790 [0033]
- **KOVATCHEV BP ; ANDERSON SM ; HEINEMANN L ; CLARKE WL.** Comparison of the numerical and clinical accuracy of four continuous glucose monitors. *Diabetes Care*, 2008, vol. 31, 1160-1164 [0033]
- **DEISS, D ; BOLINDER, J ; RIVELINE, J ; BATTELINO, T ; BOSI, E ; TUBIANA-RUFI, N ; KERR, D ; PHILLIP, M.** Improved glycemic control in poorly controlled patients with type 1 diabetes using real-time continuous glucose monitoring. *Diabetes Care*, 2006, vol. 29, 2730-2732 [0033]
- **GARG, K ; ZISSER, H ; SCHWARTZ, S ; BAILEY, T ; KAPLAN, R ; ELLIS, S ; JOVANOVIC, L.** Improvement in Glycemic Excursions With a Transcutaneous, Real-time Continuous Glucose Sensor. *Diabetes Care*, 2006, vol. 29, 44-50 [0033]
- **KOVATCHEV BP ; CLARKE WL.** Continuous glucose monitoring reduces risks for hypo- and hyperglycemia and glucose variability in diabetes. *Diabetes*, 2007, vol. 56 (1), 0086OR [0033]
- The Juvenile Diabetes Research Foundation Continuous Glucose Monitoring Study Group: Continuous glucose monitoring and intensive treatment of type 1 diabetes. *N Engl J Med*, 2008, vol. 359, 1464-76 [0033]
- **KLONOFF DC.** Continuous glucose monitoring: roadmap for 21st century diabetes therapy. *Diabetes Care*, 2005, vol. 28, 1231-1239 [0033]
- **HOVORKA R.** Continuous glucose monitoring and closed-loop systems. *Diabet Med*, 2006, vol. 23, 1-12 [0033]
- **KLONOFF DC.** The Artificial Pancreas: How Sweet Engineering Will Solve Bitter Problems. *J Diabetes Sci Technol*, 2007, vol. 1, 72-81 [0033]

- **HIRSCH IB ; ARMSTRONG D ; BERGENSTAL RM ; BUCKINGHAM B ; CHILDS BP ; CLARKE WL ; PETERS A ; WOLPERT H.** Clinical Application of Emerging Sensor Technologies in Diabetes Management: Consensus Guidelines for Continuous Glucose Monitoring. *Diabetes Tech Ther*, 2008, vol. 10, 232-246 [0033]
- **REBRIN K ; STEIL GM ; VAN ANTWERP WP ; MASTROTOTARO JJ.** Subcutaneous glucose predicts plasma glucose independent of insulin: implications for continuous monitoring. *Am J Physiol Endocrinol Metab*, 1999, vol. 277, E561-E571 [0033]
- **REBRIN K ; STEIL GM.** Can interstitial glucose assessment replace blood glucose measurements?. *Diabetes Technol Ther*, 2000, vol. 2, 461-472 [0033]
- **STEIL GM ; REBRIN K ; HARIRI F ; JINAGONDA S ; TADROS S ; DARWIN C ; SAAD MF.** Interstitial fluid glucose dynamics during insulin-induced hypoglycaemia. *Diabetologia*, 2005, vol. 48, 1833-40 [0033]
- **BOYNE M ; SILVER D ; KAPLAN J ; SAUDEK C.** Timing of Changes in Interstitial and Venous Blood Glucose Measured With a Continuous Subcutaneous Glucose Sensor. *Diabetes*, 2003, vol. 52, 2790-2794 [0033]
- **KULCU E ; TAMADA JA ; REACH G ; POTTS RO ; LESHOM MJ.** Physiological differences between interstitial glucose and blood glucose measured in human subjects. *Diabetes Care*, 2003, vol. 26, 2405-2409 [0033]
- **STOUT PJ ; RACCHINI JR ; HILGERS ME.** A Novel Approach to Mitigating the Physiological Lag between Blood and Interstitial Fluid Glucose Measurements. *Diabetes Technol Ther*, 2004, vol. 6, 635-644 [0033]
- **WENTHOLT IME ; HART AAM ; HOEKSTRA JBL ; DEVRIES JH.** Relationship Between Interstitial and Blood Glucose in Type 1 Diabetes Patients: Delay and the Push-Pull Phenomenon Revisited. *Diabetes Technol Ther*, 2004, vol. 9, 169-175 [0033]
- **WIENTJES KJ ; SCHOONEN AJ.** Determination of time delay between blood and interstitial adipose tissue glucose concentration change by microdialysis in healthy volunteers. *Int J Artif Organs*, 2001, vol. 24, 884-889 [0033]
- **AUSSEDAT B ; DUPIRE-ANGEL M ; GIFFORD R ; KLEIN JC ; WILSON GS ; REACH G.** Interstitial glucose concentration and glycemia: implications for continuous subcutaneous glucose monitoring. *Am J Physiol Endocrinol Metab*, 2000, vol. 278, E716-E728 [0033]
- **KOVATCHEV BP ; CLARKE WL.** Peculiarities of the Continuous Glucose Monitoring Data Stream and Their Impact on Developing Closed-Loop Control Technology. *J Diabetes Sci Technol*, 2008, vol. 2, 158-163 [0033]
- **CLARKE WL ; KOVATCHEV BP.** Continuous glucose sensors - continuing questions about clinical accuracy. *J Diabetes Sci Technol*, 2007, vol. 1, 164-170 [0033]
- The Diabetes Research in Children Network (DirecNet) Study Group. The Accuracy of the Guardian® RT Continuous Glucose Monitor in Children with Type 1 Diabetes. *Diabetes Tech Ther*, 2008, vol. 10, 266-272 [0033]
- **GARG SK ; SMITH J ; BEATSON C ; LOPEZ-BACAB ; VOELMLE M ; GOTTLIEB PA.** Comparison of Accuracy and Safety of the SEVEN and the Navigator Continuous Glucose Monitoring Systems. *Diabetes Technol Ther*, 2009, vol. 11, 65-72 [0033]
- **T. HEISE ; T. KOSCHINSKY ; L. HEINEMANN ; V. LODWIG.** Glucose Monitoring Study Group. Hypoglycemia warning signal and glucose sensors: requirements and concepts. *Diabetes Technol Ther*, 2003, vol. 5, 563-571 [0033]
- **B. BODE ; K. GROSS ; N. RIKALO ; S. SCHWARTZ ; T. WAHL ; C. PAGE ; T. GROSS ; J. MASTROTOTARO.** Alarms based on real-time sensor glucose values alert patients to hypo- and hyperglycemia: the guardian continuous monitoring system. *Diabetes Technol Ther*, 2004, vol. 6, 105-113 [0033]
- **G. MCGARRAUGH ; R. BERGENSTAL.** Detection of hypoglycemia with continuous interstitial and traditional blood glucose monitoring using the FreeStyle Navigator Continuous Glucose Monitoring System. *Diabetes Technol Ther*, 2009, vol. 11, 145-150 [0033]
- **S.E. NOUJAIM ; D. HORWITZ ; M. SHARMA ; J. MARHOUL.** Accuracy requirements for a hypoglycemia detector: an analytical model to evaluate the effects of bias, precision, and rate of glucose change. *J Diabetes Sci Technol*, 2007, vol. 1, 653-668 [0033]
- **W.K. WARD.** The role of new technology in the early detection of hypoglycemia. *Diabetes Technol Ther*, 2004, vol. 6, 115-117 [0033]
- **B. BUCKINGHAM ; E. COBRY ; P. CLINTON ; V. GAGE ; K. CASWELL ; E. KUNSELMAN ; F. CAMERON ; H.P. CHASE.** Preventing hypoglycemia using predictive alarm algorithms and insulin pump suspension. *Diabetes Technol Ther*, 2009, vol. 11, 93-97 [0033]
- **MILLER M ; STRANGE P.** Use of Fourier Models for Analysis and Interpretation of Continuous Glucose Monitoring Glucose Profiles. *J Diabetes Sci Technol*, 2007, vol. 1, 630-638 [0033]
- **KOVATCHEV BP ; GONDER-FREDERICK LA ; COX DJ ; CLARKE WL.** Evaluating the accuracy of continuous glucose-monitoring sensors: continuous glucose-error grid analysis illustrated by TheraSense Freestyle Navigator data. *Diabetes Care*, 2004, vol. 27, 1922-28 [0033]

- **MCDONNELL CM ; DONATH SM ; VIDMAR SI ; WERTHER GA ; CAMERON FJ.** A Novel Approach to Continuous Glucose Analysis Utilizing Glycemic Variation. *Diabetes Technol Ther*, 2005, vol. 7, 253-263 [0033]
- **CLARKE WL ; KOVATCHEV BP.** Statistical Tools to Analyze CGM Data. *Diabetes Technol Ther*, 2009, vol. 11, S45-S54 [0033]
- **ALBISSER AM ; LEIBEL BS ; EWART TG ; DAVIDOVAC Z ; BOTZ CK ; ZINGGG W.** An artificial endocrine pancreas. *Diabetes*, 1974, vol. 23, 389-396 [0033]
- **CLEMENS AH ; CHANG PH ; MYERS RW.** The development of Biostator, a glucose-controlled insulin infusion system. *Horm Metab Res Supplement*, 1977, vol. 7, 23-33 [0033]
- **MARLISS EB ; MURRAY FT ; STOKES EF ; ZINMAN B ; NAKHOODA AF ; DENOGA A ; LEIBEL BS ; ALBISSER AM.** Normalization of glycemia in diabetics during meals with insulin and glucagon delivery by the artificial pancreas. *Diabetes*, 1977, vol. 26, 663-672 [0033]
- **PFEIFFER EF ; THUM CH ; CLEMENS AH.** The artificial beta cell - A continuous control of blood sugar by external regulation of insulin infusion (glucose controlled insulin infusion system). *Horm Metab Res*, 1974, vol. 487, 339-342 [0033]
- **SANTIAGO JV ; CLEMENS AH ; CLARKE WL ; KIPNIS DM.** Closed-loop and open-loop devices for blood glucose control in normal and diabetic subjects. *Diabetes*, 1979, vol. 28, 71-84 [0033]
- **BROEKHUYSE HM ; NELSON JD ; ZINMAN B ; ALBISSER AM.** Comparison of algorithms for the closed-loop control of blood glucose using the artificial beta cell. *IEEE Trans Biomed Eng*, 1981, vol. 28, 678-687 [0033]
- **CLEMENS AH.** Feedback control dynamics for glucose controlled insulin infusion system. *MedProg Technol*, 1979, vol. 6, 91-98 [0033]
- **COBELLI C ; RUGGERI A.** Evaluation of portal/peripheral route and of algorithms for insulin delivery in the closed-loop control of glucose in diabetes. A modeling study. *IEEE Trans Biomed Eng*, 1983, vol. 30, 93-103 [0033]
- **EW, CAMPBELL LV ; CHIA YO ; MELER H ; LAZARUS L.** Control of blood glucose in diabetics using an artificial pancreas. *Aust N Z J Med*, 1977, vol. 7, 280-286 [0033]
- **FISCHER U ; JUTZI E ; FREYSE E-J ; SALZSIEDER E.** Derivation and experimental proof of a new algorithm for the artificial beta-cell based on the individual analysis of the physiological insulin- glucose relationship. *Endokrinologie*, 1978, vol. 71, 65-75 [0033]
- **SALZSIEDER E ; ALBRECHT G ; FISCHER U ; FREYSE E-J.** Kinetic modeling of the gluco-regulatory system to improve insulin therapy. *IEEE Trans Biomed Eng*, 1985, vol. 32, 846-855 [0033]
- **BRUNETTI P. ; COBELLI C. ; CRUCIANI P. ; FABIETTI P.G. ; FILIPPUCCI F. ; SANTEUSANIO F.** A simulation study on a self-tuning portable controller of blood glucose. *Int J Artificial Organs*, 1993, vol. 16, 51-57 [0033]
- **FISCHER U ; SCHENK W ; SALZSIEDER E ; ALBRECHT G ; ABEL P ; FREYSE E-J.** Does physiological blood glucose control require an adaptive strategy?. *IEEE Trans Biomed Eng*, 1987, vol. 34, 575-582 [0033]
- A Physiologic Model of Glucose Metabolism in Man and its Use to Design and Assess Improved Insulin Therapies for Diabetes. **SORENSEN JT.** Ph.D. dissertation, Dept Chemical Engineering. MIT, 1985 [0033]
- **PARKER RS ; DOYLE FJ 3RD ; PEPPAS NA.** A model-based algorithm for blood glucose control in Type I diabetic patients. *IEEE Trans Biomed Eng*, 1999, vol. 48, 148-157 [0033]
- **PARKER RS ; DOYLE FJ 3RD ; PEPPAS NA.** The intravenous route to blood glucose control. *IEEE Eng Med Biol*, 2001, vol. 20, 65-73 [0033]
- **LEBLANC H ; CHAUVET D ; LOMBRIL P ; ROBERT JJ.** Glycemic control with closed-loop intraperitoneal insulin in type I diabetes. *Diabetes Care*, 1986, vol. 9, 124-128 [0033]
- **RENARD E.** Implantable closed-loop glucose-sensing and insulin delivery: the future for insulin pump therapy. *Current Opinion in Pharmacology*, 2002, vol. 2, 708-716 [0033]
- **BELLAZZI R ; NUCCI G ; COBELLI C.** The subcutaneous route to insulin-dependent diabetes therapy: closed-loop and partially closed-loop control strategies for insulin delivery and measuring glucose concentration. *IEEE Eng Med Biol*, 2001, vol. 20, 54-64 [0033]
- **HOVORKA R ; CHASSIN LJ ; WILINSKA ME et al.** Closing the loop: the ADICOL experience. *Diabetes Technol Ther.*, 2004, vol. 6, 307-318 [0033]
- **STEIL GM ; REBRIN K ; DARWIN C ; HARIRI F ; SAAD MF.** Feasibility of automating insulin delivery for the treatment of type 1 diabetes. *Diabetes*, 2006, vol. 55, 3344-3350 [0033]
- **CLARKE WL ; KOVATCHEV BP.** The Artificial Pancreas: How Close We Are to Closing the Loop?. *Ped Endocrinol Rev*, 2007, vol. 4, 314-316 [0033]
- *The JDRF e-Newsletter: Emerging Technologies in Diabetes Research*, September 2006 [0033]
- **WEINZIMER SA ; STEIL GM ; SWAN KL ; DZIURA J ; KURTZN ; TAMBORLANE WV.** Fully automated closed-loop insulin delivery versus semi-automated hybrid control in pediatric patients with type 1 diabetes using an artificial pancreas. *Diabetes Care*, 2008, vol. 31, 934-939 [0033]

- **CLARKE WL ; ANDERSON SM ; BRETON MD ; PATEK SD ; KASHMER L ; KOVATCHEV BP.** Closed-Loop Artificial Pancreas Using Subcutaneous Glucose Sensing and Insulin Delivery and a Model Predictive Control Algorithm: The Virginia Experience. *J Diabetes Sci Technol*, 2009, vol. 3, 1031-1038 [0033]
- **BRUTTOMESSO D ; FARRET A ; COSTA S ; MARESCOTTI MC ; VETTORE M ; AVOGARO A ; TIENGO A, C. et al.** Closed-Loop Artificial Pancreas Using Subcutaneous Glucose Sensing & Insulin Delivery, and a Model Predictive Control Algorithm: Preliminary Studies in Padova and Montpellier. *J Diabetes Sci Technol*, 2009, vol. 3, 1014-1021 [0033]
- **HOVORKA R ; ALLEN JM ; ELLERI D et al.** Manual closed-loop insulin delivery in children and adolescents with type 1 diabetes: a phase 2 randomised crossover trial. *The Lancet*, 2010, vol. 375, 743-751 [0033]
- **EL-KHATIB FH ; RUSSELL SJ ; NATHAN DM ; SUTHERLIN RG ; DAMIANO ER.** A Bihormonal Closed-Loop Artificial Pancreas for Type 1 Diabetes. *Science Transl Med*, 2010, vol. 2, 27ra27 [0033]
- **KOVATCHEV BP ; MENDOSA P ; ANDERSON SM ; HAWLEY JS ; RITTERBAND LM ; GONDER-FREDERICK L.** Effect of automated bio-behavioral feedback on the control of type 1 diabetes. *Diabetes Care*, 2011, vol. 34, 302-307 [0033]
- **BERGMAN RN ; IDERYZ ; BOWDEN CR ; COBEL-LI C.** Quantitative estimation of insulin sensitivity. *Am J Physiol.*, 1979, vol. 236, E667-E677 [0033]
- **FERNANDEZ-LUQUE et al.** eDiab: A System for Monitoring, Assisting and Educating People with Diabetes. *ICCHP 2006, LNCS*, 2006, vol. 4061, 1342-1349 [0034]

专利名称(译)	监测和控制糖尿病患者血糖水平的统一平台		
公开(公告)号	EP2723229B1	公开(公告)日	2018-09-26
申请号	EP2012802310	申请日	2012-06-23
[标]申请(专利权)人(译)	弗吉尼亚大学专利基金会		
申请(专利权)人(译)	VIRGINIA专利大学基金会		
当前申请(专利权)人(译)	VIRGINIA专利大学基金会		
[标]发明人	KOVATCHEV BORIS P KEITH HYNES PATRICK T BRETON MARC D PATEK STEPHEN D		
发明人	KOVATCHEV, BORIS, P. KEITH-HYNES, PATRICK, T. BRETON, MARC, D. PATEK, STEPHEN, D.		
IPC分类号	A61B5/00 G06F19/00		
CPC分类号	A61B5/0022 A61B5/14532 A61B5/4839 A61B5/7275 A61K38/28 G06F19/00 G06F19/3418 G06F19/3456 G16H20/17 G16H40/63 G16H40/67 G16H50/20 G16H50/30 A61B5/0024 A61B5/0205 A61B5/021 A61B5/024 A61B5/0402 A61B5/11 A61B5/486 A61B5/7264 A61B5/742 A61B5/746 A61B5/747 A61M5/16831 A61M5/1723 G16H20/10		
优先权	61/500545 2011-06-23 US		
其他公开文献	EP2723229A2 EP2723229A4		
外部链接	Espacenet		

摘要(译)

灵活的系统，能够利用来自不同监测技术的数据，并能够在几个可扩展的水平上为糖尿病患者提供帮助，从长期趋势和预后的建议到实时自动闭环控制（人工胰腺）。这些可扩展的监测和治疗策略由称为糖尿病助理（DiAs）平台的统一系统提供。该系统为实施各种监测，咨询和自动化糖尿病治疗算法或方法提供了基础。DiAs建议针对个体患者的具体情况以及任何给定时刻的患者风险评估而定制。

$$LBGI = \frac{1}{n} \sum_{i=1}^n rl(x_i)$$