



(11) **EP 2 939 592 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**19.06.2019 Bulletin 2019/25**

(51) Int Cl.:  
**A61B 5/02 (2006.01) A61B 5/021 (2006.01)**  
**A61B 5/024 (2006.01) A61B 5/00 (2006.01)**

(21) Application number: **15168200.2**

(22) Date of filing: **11.02.2010**

(54) **DETECTION OF PARAMETERS IN CARDIAC OUTPUT RELATED WAVEFORMS**

NACHWEIS VON PARAMETERN IN HERZLEISTUNGSBEZOGENEN WELLENFORMEN

DÉTECTION DE PARAMÈTRES DANS DES FORMES D'ONDES LIÉES AU DÉBIT CARDIAQUE

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO SE SI SK SM TR**

(30) Priority: **11.02.2009 US 151670 P**  
**03.02.2010 US 699540**

(43) Date of publication of application:  
**04.11.2015 Bulletin 2015/45**

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:  
**10741699.2 / 2 395 908**

(73) Proprietor: **Edwards Lifesciences Corporation**  
**Irvine, CA 92614 (US)**

(72) Inventors:  
• **Hatib, Feras**  
**Irvine, CA 92614 (US)**  
• **Roteliuk, Luchy D.**  
**Irvine, CA 92614 (US)**

(74) Representative: **Eisenführ Speiser**  
**Patentanwälte Rechtsanwälte PartGmbB**  
**Postfach 31 02 60**  
**80102 München (DE)**

(56) References cited:  
**US-A- 5 265 011 US-A1- 2004 147 850**  
**US-A1- 2005 283 086 US-A1- 2006 264 766**

**EP 2 939 592 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### BACKGROUND

**[0001]** Many of the parameters that can be determined from cardiac output related waveforms, e.g., peripheral pressure waveforms, are important not only for diagnosis of disease, but also for "real-time," i.e., continual, monitoring of clinically significant changes in a subject. Various methods exist to identify and/or calculate these parameters based on analysis of various features in cardiac output related waveforms. Few hospitals are without equipment that employ these methods to monitor one or more cardiac output related parameters in an effort to provide a warning that a subject's condition is changing.

**[0002]** Document US 2004/0147850 A1 discloses determination of the dirotic notch as the second maximum in the second derivative of a cardiac output related waveform (fig. 8) following the starting time point of the heart beat cycle.

### SUMMARY

**[0003]** The present invention is defined by the appended claims.

**[0004]** Methods for detecting parameters in cardiac output related waveforms are described. The methods include methods for detecting individual heart beat cycles in a cardiac output related waveform, methods for detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related waveform, methods for detecting a dichrotic notch for an individual heart beat cycle in a cardiac output related waveform, and methods for detecting an error in an assigned dichrotic notch for an individual heart beat cycle in a cardiac output related waveform.

**[0005]** The methods for detecting individual heart beat cycles in a cardiac output related waveform include providing cardiac output related waveform data and calculating a first derivative function for the waveform data. The order of the data for the first derivative function is then reversed in time. Next the amplitude of the first derivative function is compared to a threshold value, with the threshold value being a percentage of the maximum amplitude in the first derivative function. The start of a heart beat cycle is then determined by identifying the first time the first derivative function equals zero immediately after the point (i.e., prior in time) at which the amplitude of the first derivative function is greater than the threshold value in the reversed time order data. The first time the first derivative function equals zero indicates the beginning of a heart beat cycle.

**[0006]** The methods for detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related waveform include providing cardiac output related waveform data for an individual heart beat cycle, the individual heart beat cycle having a predetermined starting point, and determining a maximum

value of the cardiac output related waveform data. Next a first point in the cardiac output related waveform is determined, the first point being the first point on the cardiac output related waveform prior to the maximum value that has a value equal to one-half the maximum value. The portion of the heart beat cycle between the starting point and the first point is then searched for a local maximum. If a local maximum is found, the portion of the heart beat cycle between the first point and the local maximum is searched for a local minimum point, and the starting point for the individual heart beat is reassigned to the local minimum point.

**[0007]** The methods for detecting a dichrotic notch for an individual heart beat cycle in a cardiac output related waveform include providing cardiac output related waveform data for an individual heart beat cycle, the individual heart beat cycle having a previously determined starting time point, and calculating a first derivative function for the waveform data. Next a first time point and a second time point are determined from the first derivative function, the first time point being the first zero crossing after the starting time point for the first derivative function and the second time point being the second zero crossing after the starting time point for the first derivative function.

A second derivative function is also calculated for the waveform data and a third time point and a fourth time point are determined from the second derivative function, the third time point being the first zero crossing after the second time point for the second derivative function and the fourth time point being the second zero crossing after the second time point for the second derivative function. Then the portion of the second derivative function between the third time point and the fourth time point is searched for a local maximum, the local maximum occurring at a fifth time point. The fifth time point corresponds to the time point at which the dichrotic notch is located in the cardiac output related waveform data for the individual heart beat cycle.

**[0008]** The methods for detecting an error in an assigned dichrotic notch for an individual heart beat cycle in a cardiac output related waveform include providing cardiac output related waveform data for an individual heart beat cycle, the individual heart beat cycle having a previously determined dichrotic notch time point, a previously determined starting time point, a previously determined cardiac output maximum point, and a previously determined ending time point, and calculating a first derivative function for the waveform data. Then all the local maximums between the cardiac output maximum point and a search time point in the first derivative function are determined, the search time point being starting time point plus two-thirds the time between the starting time point and the ending time point. If more than one local maximum is found, the dichrotic notch is assigned to the time point at the second local maximum.

## DESCRIPTION OF DRAWINGS

### [0009]

Fig. 1 shows a flow chart illustrating an example of logic for detecting individual heart beat cycles in cardiac output related waveforms.

Fig. 2A shows an arterial pressure waveform taken over several heart beat cycles.

Fig. 2B shows the first derivative function of the arterial pressure waveform shown in Fig. 2A.

Fig. 3 shows a flow chart illustrating an example of logic for verifying the number of individual heart beat cycles in cardiac output related waveforms.

Figs. 4A-D show examples of cardiac output waveforms in which arrhythmia is occurring.

Fig. 5 shows a flow chart illustrating an example of logic for detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related waveform.

Fig. 6A shows an arterial pressure waveform taken over several heart beat cycles in which the initiation of heart beat cycles have been incorrectly identified.

Fig. 6B shows the relevant points of a heart beat cycle for the application of methods for detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related waveform.

Fig. 7 shows a flow chart illustrating an example of logic for detecting a dichrotic notch for an individual heart beat cycle in a cardiac output related waveform.

Fig. 8A shows an arterial pressure waveform taken over several heart beat cycles.

Fig. 8B shows the first derivative function of the waveform from Fig. 8A.

Fig. 8C shows the second derivative function of the waveform from Fig. 8A.

Fig. 9 shows a flow chart illustrating an example of logic for detecting an error in an assigned dichrotic notch for an individual heart beat cycle in a cardiac output related waveform.

Fig. 10A shows an arterial pressure waveform taken over several heart beat cycles.

Fig. 10B shows the first derivative function of the waveform from Fig. 10A.

Fig. 11 is a block diagram showing the main components of a system to implement the methods described herein.

## DETAILED DESCRIPTION

[0010] Methods for detecting parameters in cardiac output related waveforms are described. Specifically, the methods described herein include detecting individual heart beat cycles in a cardiac output related waveform, detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related

waveform, detecting a dichrotic notch for an individual heart beat cycle in a cardiac output related waveform, and detecting an error in an assigned dichrotic notch for an individual heart beat cycle in a cardiac output related waveform. The individual heart beat cycles and the dichrotic notch in a cardiac output related waveform, in addition to themselves being important parameters for a clinician, form the basis for the calculation of many other cardiac output related parameters, thus, the initial accurate identification of heart beat cycles and dichrotic notch forms the basis for a clinician to appropriately provide treatment to a subject.

[0011] As used herein, the phrase cardiac output related waveform is used to indicate a signal related to, e.g., proportional to, derived from, or a function of, cardiac output. Examples of such signals include, but are not limited to, peripheral arterial and central aortic pressure and/or flow, pulse oxymetry waveforms, impedance plethysmography waveforms, and Doppler waveforms. The term peripheral arterial pressure is intended to mean pressure measured at any point in the arterial tree, e.g., radial, femoral, or brachial, either invasively or non-invasively. If invasive instruments are used, in particular, catheter-mounted pressure transducers, then any artery is a possible measurement point. Placement of non-invasive transducers will typically be dictated by the instruments themselves, e.g., finger cuffs, upper arm pressure cuffs, and earlobe clamps. Peripheral arterial pressure increases the further away from the heart the measurement is taken. Regardless of the specific instrument or measurement used, the data obtained will ultimately yield an electric signal corresponding (for example, proportional) to cardiac output.

[0012] The method for detecting individual heart beat cycles in cardiac output related waveforms as disclosed herein is shown as a flow chart in Fig. 1 and involves providing cardiac output related waveform data (10), and calculating a first derivative function for the waveform data and reversing the time order of the data (20). The amplitude of the first derivative function is compared to a threshold value (30), i.e., a percentage of the maximum amplitude in the first derivative function. The start of a heart beat cycle is determined by identifying the first time the first derivative function equals zero immediately after the point at which the amplitude of the first derivative function is greater than the threshold value in the reversed time order data (40), i.e., the first time the first derivative function equals zero indicates the beginning of a heart beat cycle (50).

[0013] Fig. 2A is an example of an arterial pressure waveform taken over several heart beat cycles. The individual heart beat cycles are indicated by dots near the waveform minimum values. Applying the method for detecting individual heart beat cycles just described involves calculating the first derivative function, which for the waveform shown in Fig. 2A is shown in Fig. 2B (note the first derivative function is not shown in Fig. 2B as reversed in time order). Next the first derivative function

is compared to a threshold value, which is shown in Fig. 2B for the purpose of this example as a thick line. Next, the first zero crossing immediately after (shown as prior in time to) the point at which the amplitude of the first derivative function is greater than the threshold value is located. The first zero crossing for the portion of the first derivative function indicated by a dashed line is noted in Fig. 2B. For a derivative function as shown in Fig. 2B, the choice of a threshold crossing on the rising or descending portion of the first derivative function peak does not impact the identification of the first zero crossing prior to the peak. The identified zero crossing time is the time at which the individual heart beat cycle began (see dashed arrow pointing from Fig. 2B to Fig. 2A). To calculate the next heart beat cycle, the first derivative function is searched for the next point at which the amplitude of the first derivative function is greater than the threshold value and the process is repeated. The method can be repeated until the end of the provided waveform is reached (or indefinitely if data is continuously provided, e.g., in real-time monitoring).

**[0014]** The waveform data can be filtered to remove high and low frequency noise prior to taking the calculating the first derivative waveform. A high-pass filter, for example, can be used to suppress baseline drift and to eliminate the effect of respiration in the subject. A high-pass filter useful with the methods described herein could achieve zero-phase distortion by using forward and reverse digital filtering techniques to retain the same phase as the input signal. Another parameter for a high-pass filter useful with the methods described herein includes a low frequency (e.g., 0.25 Hz) cut-off frequency to remove baseline drift and respiration. For further example, a low-pass filter can be used to smooth the waveform signal prior to calculating the first derivative. A low-pass filter can reduce the effect of any rapid time-domain transitions and/or variations in the arterial pulse pressure signal. A finite impulse response filter can be used to limit time delay in the low-pass filtering operation. The use of low- and high-pass filters to aid in the processability of data is well known to those of skill in the art.

**[0015]** A common problem in detecting the cardiac beat cycles in cardiac output-related waveforms is heart rate irregularities. Examples of such heart rate irregularities include, but are not limited to, the occurrence of premature atrial or ventricular contractions, arrhythmia, and atrial fibrillation. Heart rate irregularities typically include premature beats, which could occur at any time. These premature beats typically generate less volume and lower pressure than the main beats. The lower volume and pressure of these beats causes the appearance of small beats in the signal of all cardiac output related waveforms. The small beats generated by the premature cardiac contractions have very similar amplitude and frequency characteristics as the pressure reflections that could occur during the diastolic phase or during the late systolic phase of the cardiac output related waveform making these beats hard to differentiate from pressure

reflections. For example, if lower thresholds are used to detect the small beats generated by premature cardiac contractions, large pressure reflections could be erroneously counted as cardiac cycles.

**[0016]** To overcome the potential for counting pressure reflections as cardiac cycles, the method for detecting individual heart beat cycles in cardiac output related waveforms as described above can be repeated at different threshold levels to verify the number of heart beat cycles detected. To verify the number of heart beat cycles (as shown in Fig. 3), the method is performed as described above using a first threshold (10), then performed a second time using a second (lower) threshold value (20). Next, the number of heart beats detected using the different threshold values is compared (30). If the ratio of the number of heart beat cycles using the first threshold value to the number of heart beat cycles using the second threshold value is less than 65%, but the number of beats per minute above 150 is not greater than 35% of the beats per minute detected then using the heart beat cycles determined using the second threshold value as the actual number of heart beat cycles (40). If the ratio of the number of heart beat cycles using the threshold value to the number of heart beat cycles using the second threshold value is less than 65% and the number of beats per minute above 150 is greater than 35% of the beats per minute detected then using the heart beat cycles determined using the first threshold value as the actual number of heart beat cycles (50). If the ratio of the number of heart beat cycles using the first threshold value to the number of heart beat cycles using the second threshold value is not less than 65%, then using the heart beat cycles determined using the second threshold value as the actual number of heart beat cycles (60). The method can be repeated using additional pairs of first threshold and second (lower) threshold values.

**[0017]** The choice of a threshold value for use in the method to detect individual heart beat cycles depends upon a variety of factors. Examples of threshold values useful with the methods described herein include 0.8, 0.75, 0.7, 0.65, 0.6, 0.55, 0.5, 0.45, 0.4, 0.35 and 0.3. Examples of pairs of threshold and lower threshold values useful with these methods include various combinations of these threshold values, such as, 0.75 and 0.6 or 0.6 and 0.3. Other threshold values and pairs of threshold values can be useful depending on the circumstances. Figs. 4A-4D show examples of cardiac output waveforms in which arrhythmia is occurring. Each of these waveforms represent very challenging situations of beat detection from cardiac output related waveforms. The present method was used to successfully detect the beats shown with the dots. Figs. 4A-4D demonstrate the excellent performance of this method in very challenging conditions.

**[0018]** Also described herein (and shown as flow chart in Fig. 5) is a method for detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related waveform. Examples of situations in which

an assigned starting point may be incorrectly assigned include arrhythmia conditions or tachycardia conditions, in which large pressure reflections occur during the diastolic phase of the waveform and the next cardiac cycle starts before the end of the reflection of the diastolic phase of the previous cardiac cycle. In these cases the beginning of a heart beat cycle contains a small peak like that shown in Figs. 6A and 6B. In these types of situations, standard beat detection methods can erroneously detect the beginning of the beat before the small peak at the minimum point of the diastolic phase of the previous cycle rather than after the peak, where the true start of the beat is located. Such an incorrect detection of the beginning of a beat could cause significant errors in the determination of other cardiac parameters based on the waveform being analyzed. The method for detecting an error in an assigned starting point for an individual heart beat cycle (as shown in Fig. 5) includes providing cardiac output related waveform data for an individual heart beat cycle with a predetermined starting point (10). Next a maximum value of the cardiac output related waveform data is determined (20) and a first point is found (30). The first point being the first point on the cardiac output related waveform prior to the maximum value that has a value equal to one-half the maximum value. Then the portion of the heart beat cycle between the starting point and the first point is searched for a local maximum (40). If a local maximum is found between the starting point and the first point, the portion of the heart beat cycle between the first point and the local maximum is searched for a local minimum point (50), and the starting point for the individual heart beat is reassigned as the local minimum point (60). If a local maximum is not found between the starting point and the first point, the current starting point for the beat is retained (70). The method may further include finding the starting point of the next individual heart beat, which will also be the ending point for the current individual heart beat cycle.

**[0019]** To further illustrate this method, Fig. 6A shows a waveform in which the beginning of each heart beat cycle has been incorrectly detected (see the dots at the local minimums). Fig. 6B shows the relevant points of a heart beat cycle for the application of this method, i.e.,  $k$  is the predetermined starting point for the heart beat cycle ( $k+1$  is the beginning of the next heart beat cycle),  $s$  is the maximum value of the cardiac output related waveform data,  $h$  is the first point on the cardiac output related waveform prior to the maximum value that has a value equal to one-half the maximum value,  $1$  is the local maximum between the starting point and the first point, and  $d$  is the correct start of the heart beat cycle as calculated using the method.

**[0020]** Further described herein (and shown in a flow chart in Fig. 7) is a method for detecting a dichrotic notch for an individual heart beat cycle in a cardiac output related waveform. This method includes providing cardiac output related waveform data for an individual heart beat cycle with a previously determined starting point (10) and

calculating a first derivative function for the waveform data (20). Next a first time point (the first zero crossing after the starting time point for the first derivative function) and a second time point (the second zero crossing after the starting time point for the first derivative function) are determined from the first derivative function (30). A second derivative function is also calculated for the waveform data (40). Then a third time point (the first zero crossing after the second time point for the second derivative function) and a fourth time point (the second zero crossing after the second time point for the second derivative function) are determined from the second derivative function (50). Next the portion of the second derivative function between the third time point and the fourth time point is searched for a local maximum, the local maximum occurring at a fifth time point (60). Finally, the fifth time point is assigned to be the dichrotic notch. The functions used in this method can be filtered as described above.

**[0021]** To further illustrate this method, Fig. 8 shows cardiac output data analyzed using this method. Specifically, Fig. 8A shows a waveform with three indicated heart beat cycles (dots at local minima), Fig. 8B shows the first derivative function of the waveform shown in Fig. 8A, and Fig. 8C shows the second derivative function of the waveform shown in Fig. 8A. Point 1 of Fig. 8A is the start of the heart beat cycle being analyzed and dashed line 2 between Figs. 8A and 8B shows the starting time point for the heart beat cycle in the first derivative function and also occurs just prior to the first time point (i.e., the first zero crossing after the starting point) in the first derivative function. Point 3 in Fig. 8B shows the second time point in the first derivative function (i.e., the second zero crossing after the starting time point). Dashed line 4 shows where the second time point is transferred to the second derivative function shown in Fig. 8C to start the search for the third time point (i.e., the first zero crossing after the second time point in the second derivative function) and point 5 in Fig. 8C is the third time point. Point 6 in Fig. 8C is the fourth time point (i.e., the second zero crossing after the second time point in the second derivative function). Point 7 in Fig. 8C (i.e., the fifth time point) is the local maximum between the third time point and the second time point. The time of the fifth point is shown to be transferred back to the waveform of Fig. 8A where the time point indicates the position of the dichrotic notch (shown at point 9).

**[0022]** Additionally described herein (and shown in a flow chart in Fig. 9) is a method for detecting an error in an assigned dichrotic notch for an individual heart beat cycle in a cardiac output related waveform. These types of errors commonly occur in dichrotic notch detection when large reflected waves are present in the signal around the dichrotic notch location. This method includes providing cardiac output related waveform data for an individual heart beat cycle with a previously determined dichrotic notch time point, a previously determined starting time point, a previously determined cardiac output maximum, and a previously determined end time point

(10), and calculating a first derivative function for the waveform data (20). Next, all the local maximums between the cardiac output maximum point and a search time point in the first derivative function are determined (30). The search time point is determined by adding the starting time point and two-thirds of the time interval between the starting time point and the ending time point. If more than one local maximum is found, the dichrotic notch is reassigned to the time point at the second local maximum (40). If only one local maximum is found, the dichrotic notch remains the previously determined dichrotic notch (50).

**[0023]** To further illustrate this method, Fig. 10 shows cardiac output data analyzed using this method. Specifically, Fig. 10A shows a waveform with about three heart beat cycles (and two local minima that could be the dichrotic notch) and Fig. 10B shows the first derivative function of the waveform shown in Fig. 10A. Point 10 of Fig. 10A is the start of the heart beat cycle being analyzed and dashed line 20 between Figs. 10A and 10B shows the starting time point for the analysis of the first derivative function. Dashed line 30 indicates the search time point which is two-thirds the time interval between the starting point and the ending point 40, thus the period between dashed line 20 and dashed line 50 indicates the search window for finding local maximums in the first derivative function. Two local minimums  $M_1$  and  $M_2$  are found in the search window. Because more than one local maximum was found, the dichrotic notch is assigned to the second local minimum  $M_2$ , which corresponds to point 60 in Fig. 10A.

**[0024]** Fig. 11 shows the main components of a system that can be used to implement the methods described herein for detecting individual heart beat cycles in a cardiac output related waveform, detecting an error in an assigned starting point for an individual heart beat cycle in a cardiac output related waveform, detecting a dichrotic notch for an individual heart beat cycle in a cardiac output related waveform, and detecting an error in an assigned dichrotic notch for an individual heart beat cycle in a cardiac output related waveform. The methods may be implemented within an existing patient-monitoring device, or it may be implemented as a dedicated monitor. As is mentioned above, a cardiac output related waveform, or some other input signal proportional to, derived from, or a function of cardiac output, may be sensed in either or, indeed, both, of two ways: invasively and non-invasively. For convenience, the system is described as measuring arterial blood.

**[0025]** Fig. 11 shows both types of pressure sensing for the sake of completeness. In most practical applications of the methods described herein, either one or several variations will typically be implemented. In invasive applications of the methods described herein, a conventional pressure sensor 100 is mounted on a catheter 110, which is inserted in an artery 120 of a portion 130 of the body of a human or animal patient. The artery 120 is any artery in the arterial system, such as, for example, the

femoral, radial or brachial artery. In the non-invasive applications of the methods described herein, a conventional pressure sensor 200, such as a photo-plethysmographic blood pressure probe, is mounted externally in any conventional manner, for example using a cuff around a finger 230 or a transducer mounted on the wrist of the patient. Fig. 11 schematically shows both types.

**[0026]** The signals from the sensors 100, 200 are passed via any known connectors as inputs to a processing system 300, which includes one or more processors and other supporting hardware and system software (not shown) usually included to process signals and execute code. The methods described herein may be implemented using a modified, standard, personal computer, or may be incorporated into a larger, specialized monitoring system. For use with the methods described herein, the processing system 300 also may include, or is connected to, conditioning circuitry 302 which performs normal signal processing tasks such as amplification, filtering, or ranging, as needed. The conditioned, sensed input pressure signal  $P(t)$  is then converted to digital form by a conventional analog-to-digital converter ADC 304, which has or takes its time reference from a clock circuit 305. As is well understood, the sampling frequency of the ADC 304 should be chosen with regard to the Nyquist criterion so as to avoid aliasing of the pressure signal (this procedure is very well known in the art of digital signal processing). The output from the ADC 304 will be the discrete pressure signal  $P(k)$ , whose values may be stored in conventional memory circuitry (not shown).

**[0027]** The values  $P(k)$  are passed to or accessed from memory by a software module 310 comprising computer-executable code for implementing one or more aspects of the methods as described herein. The design of such a software module 310 will be straight forward to one of skill in the art of computer programming. Additional comparisons and/or processing as used by a method can be performed in additional modules such as 320 and 330.

**[0028]** If used, signal-specific data such as a previously determined dichrotic notch time point, a previously determined starting time point, and a previously determined end time point can be stored in a memory region 315, which may also store other predetermined parameters as needed. These values may be entered using any known input device 400 in the conventional manner.

**[0029]** As illustrated by Fig. 11, the results may be ultimately displayed on a conventional display or recording device 500 for presentation to and interpretation by a user. As with the input device 400, the display 500 will typically be the same as is used by the processing system for other purposes.

**[0030]** Exemplary embodiments of the present invention have been described above with reference to block diagrams and flowchart illustrations of methods, apparatuses, and computer program products. One of skill will understand that each block of the block diagrams and flowchart illustrations, and combinations of blocks in the block diagrams and flowchart illustrations, respectively,

can be implemented by various means including computer program instructions. These computer program instructions may be loaded onto a general purpose computer, special purpose computer, or other programmable data processing apparatus to produce a machine, such that the instructions which execute on the computer or other programmable data processing apparatus create a means for implementing the functions specified in the flowchart block or blocks.

**[0031]** The methods described herein further relate to computer program instructions that may be stored in a computer-readable memory that can direct a computer or other programmable data processing apparatus, such as in a processor or processing system (shown as 300 in Fig. 11), to function in a particular manner, such that the instructions stored in the computer-readable memory produce an article of manufacture including computer-readable instructions for implementing the function specified in the blocks illustrated in Fig. 11. The computer program instructions may also be loaded onto a computer, the processing system 300, or other programmable data processing apparatus to cause a series of operational steps to be performed on the computer, the processing system 300, or other programmable apparatus to produce a computer-implemented process such that the instructions that execute on the computer or other programmable apparatus provide steps for implementing the functions specified in the blocks. Moreover, various software modules 310, 320, and 330 can be used to perform the various calculations and perform related method steps described herein also can be stored as computer-executable instructions on a computer-readable medium in order to allow the methods to be loaded into and executed by different processing systems.

**[0032]** Accordingly, blocks of the block diagrams and flowchart illustrations support combinations of means for performing the specified functions, combinations of steps for performing the specified functions, and program instruction means for performing the specified functions. One of skill will understand that each block of the block diagrams and flowchart illustrations, and combinations of blocks in the block diagrams and flowchart illustrations, can be implemented by special purpose hardware-based computer systems that perform the specified functions or steps, or combinations of special purpose hardware and computer instructions.

**[0033]** The present invention is not limited in scope by the embodiments disclosed herein which are intended as illustrations of a few aspects of the invention. The term "comprising" and variations thereof as used herein is used synonymously with the term "including" and variations thereof and are open, non-limiting terms.

## Claims

1. A processor-implemented method for detecting an error in an assigned dicrotic notch for an individual

heart beat cycle in a cardiac output related waveform comprising:

providing (10) cardiac output related waveform data for an individual heart beat cycle, the individual heart beat cycle having a previously determined dicrotic notch time point, a previously determined starting time point identified as the first time the first derivative function of the waveform data equals zero immediately after, in the reversed time order of the waveform data, the point at which the amplitude of the first derivative function is greater than a threshold value (30), a previously determined cardiac output maximum point representing the time point of maximum of the waveform data for the individual heart beat cycle, and a previously determined ending time point;  
calculating (20) a second derivative function for the waveform data;  
determining (30) all the local maxima between the cardiac output maximum point and a search time point in the second derivative function, the search time point being starting time point plus two-thirds the time between the starting time point and the ending time point, wherein if more than one local maximum is found, the dicrotic notch is reassigned (40) to the time point at the second local maximum.

2. A system for detecting an error in an assigned dicrotic notch for an individual heart beat cycle in a cardiac output related waveform, comprising

a pressure sensor (100, 200);  
a processing system (300) configured to receive signals from the pressure sensor (100, 200) as input;  
wherein the processing system is configured to perform the method of claim 1.

3. The system of claim 2, wherein the system comprises a catheter (110) and the pressure sensor is mounted on the catheter (110).

4. The system of claim 2, wherein the pressure sensor is a photo-plethysmographic blood pressure probe (200) configured to be mounted externally or a transducer configured to be mounted on the wrist of a patient.

5. The system of one of the claims 2 to 4, further comprising a conditioning circuitry (302) configured to perform normal signal processing tasks such as amplification, filtering, or ranging.

6. The system of one of the claims 2 to 5, further comprising a display or recording device (500) for pres-

entation to and interpretation by a user.

7. A computer-readable medium comprising computer-executable instructions which, when executed by a processor, cause the processor to perform the method according to claim 1.

### Patentansprüche

1. Prozessorimplementiertes Verfahren zum Erkennen eines Fehlers in einer zugeordneten dikrotischen Kerbe eines individuellen Herzschlagzyklus in einer herzleistungsbezogenen Wellenform, umfassend:

Bereitstellen (10) von Daten von herzleistungsbezogenen Wellenformen für einen individuellen Herzschlagzyklus, wobei der individuelle Herzschlagzyklus einen zuvor bestimmten Zeitpunkt der dikrotischen Kerbe, einen zuvor bestimmten Startzeitpunkt, der als die erste Zeit, bei der die erste Ableitungsfunktion der Wellenformdaten Null ergibt, in umgekehrter zeitlicher Reihenfolge der Wellenformdaten unmittelbar nach dem Punkt identifiziert wird, an dem die Amplitude der ersten Ableitungsfunktion größer als ein Schwellenwert (30) ist, einen zuvor bestimmten Maximalpunkt der Herzleistung, der den Zeitpunkt des Maximums der Wellenformdaten für den individuellen Herzschlagzyklus wiedergibt, und einen zuvor bestimmten Endzeitpunkt aufweist;

Berechnen (20) einer zweiten Ableitungsfunktion für die Wellenformdaten;

Bestimmen (30) aller lokalen Maxima zwischen dem Maximalpunkt der Herzleistung und einem Suchzeitpunkt in der zweiten Ableitungsfunktion, wobei der Suchzeitpunkt der Startzeitpunkt plus zwei Drittel der Zeit zwischen dem Startzeitpunkt und dem Endzeitpunkt ist,

wobei, falls mehr als ein lokales Maximum gefunden wird, die dikrotische Kerbe dem Zeitpunkt an dem zweiten lokalen Maximum neu zugewiesen (40) wird.

2. System zum Erkennen eines Fehlers in einer zugeordneten dikrotischen Kerbe eines individuellen Herzschlagzyklus in einer herzleistungsbezogenen Wellenform, umfassend:

einen Drucksensor (100, 200);  
ein Verarbeitungssystem (300), das konfiguriert ist, um Signale von dem Drucksensor (100, 200) als Eingabe zu empfangen;  
wobei das Verarbeitungssystem konfiguriert ist, um das Verfahren gemäß Anspruch 1 durchzuführen.

3. System nach Anspruch 2, wobei das System einen Katheter (110) umfasst und der Drucksensor auf dem Katheter (110) angebracht ist.

4. System nach Anspruch 2, wobei der Drucksensor eine Blutdrucksonde (200) für Photoplethysmographie, die konfiguriert ist, um extern angebracht zu werden, oder ein Messwertwandler ist, der konfiguriert ist, um am Handgelenk eines Patienten angebracht zu werden.

5. System nach einem der Ansprüche 2 bis 4, ferner umfassend eine Konditionierungsschaltung (302), die konfiguriert ist, um normale Signalverarbeitungsaufgaben zu übernehmen, wie Verstärkung, Filterung oder Bereichsabgrenzung.

6. System nach einem der Ansprüche 2 bis 5, ferner umfassend eine Anzeige- oder Aufzeichnungsvorrichtung (500) zur Präsentation an einen Anwender und zur Interpretation durch diesen.

7. Computerlesbares Medium, welches computerausführbare Anweisungen umfasst, die bei Ausführung durch einen Prozessor bewirken, dass der Prozessor das Verfahren gemäß Anspruch 1 durchführt.

### Revendications

1. Procédé mis en oeuvre par un processeur pour détecter une erreur dans une incisure dicrote attribuée pour un cycle de battement cardiaque individuel dans une forme d'onde associée au débit cardiaque comprenant:

la mise à disposition (10) de données de forme d'onde associée au débit cardiaque pour un cycle de battement cardiaque individuel, le cycle de battement cardiaque individuel ayant un point temporel d'incisure dicrote préalablement déterminé, un point temporel de départ préalablement déterminé identifié comme la première fois où la première fonction dérivée des données de forme d'onde est égale à zéro immédiatement après, dans l'ordre chronologique inversé des données de forme d'onde, le point où l'amplitude de la première fonction dérivée est supérieure à une valeur seuil (30), un point maximum de débit cardiaque préalablement déterminé représentant le point temporel de maximum des données de forme d'onde pour le cycle de battement cardiaque individuel et un point temporel de fin préalablement déterminé;  
le calcul (20) d'une deuxième fonction dérivée pour les données de forme d'onde;  
la détermination (30) de tous les maxima locaux entre le point maximal de débit cardiaque et un

- point temporel de recherche dans la deuxième fonction dérivée, le point temporel de recherche étant le point temporel de départ plus deux tiers du temps entre le point temporel de départ et le point temporel de fin, 5  
l'incisure dicrote étant réattribuée (40) au point temporel au niveau du deuxième maximum local si plus d'un maximum local est trouvé.
2. Système de détection d'une erreur dans une incisure dicrote attribuée pour un cycle de battement cardiaque individuel dans une forme d'onde associée à un débit cardiaque, comprenant 10  
un capteur de pression (100, 200);  
un système de traitement (300) configuré pour recevoir des signaux provenant du capteur de pression (100, 200) en tant qu'entrée; 15  
le système de traitement étant configuré pour effectuer le procédé de la revendication 1. 20
3. Système selon la revendication 2, le système comprenant un cathéter (110) et le capteur de pression étant monté sur le cathéter (110).
4. Système selon la revendication 2, le capteur de pression étant une sonde de pression artérielle photopléthysmographique (200) conçue pour être montée de manière externe ou un transducteur conçu pour être monté sur le poignet d'un patient. 25  
30
5. Système selon l'une quelconque des revendications 2 à 4, comprenant en outre un circuit de conditionnement (302) conçu pour effectuer des tâches normales de traitement de signal, telles que l'amplification, le filtrage ou la télémétrie. 35
6. Système selon l'une quelconque des revendications 2 à 5, comprenant en outre un dispositif d'affichage ou d'enregistrement (500) pour la présentation à un utilisateur et l'interprétation par celui-ci. 40
7. Support lisible par ordinateur comprenant des instructions exécutables par ordinateur qui, lorsqu'elles sont exécutées par un processeur, amènent le processeur à effectuer le procédé selon la revendication 1. 45

50

55

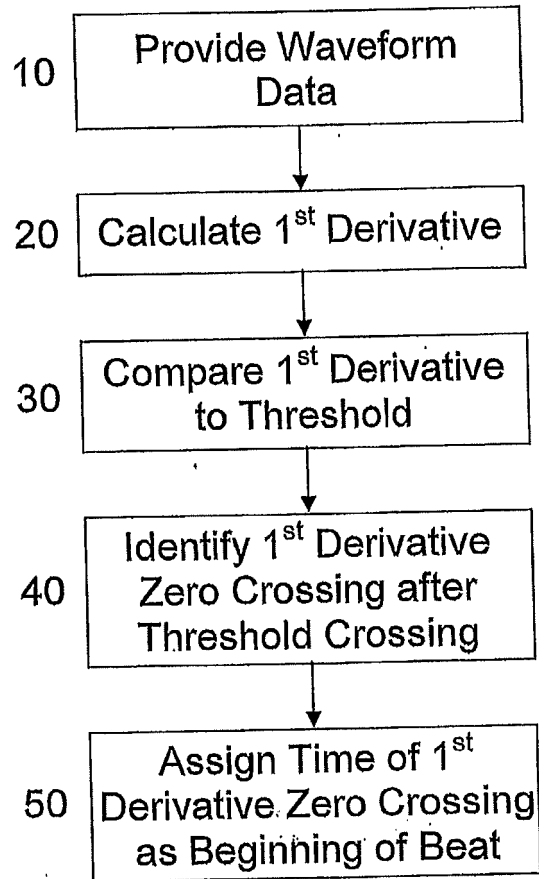


Fig. 1

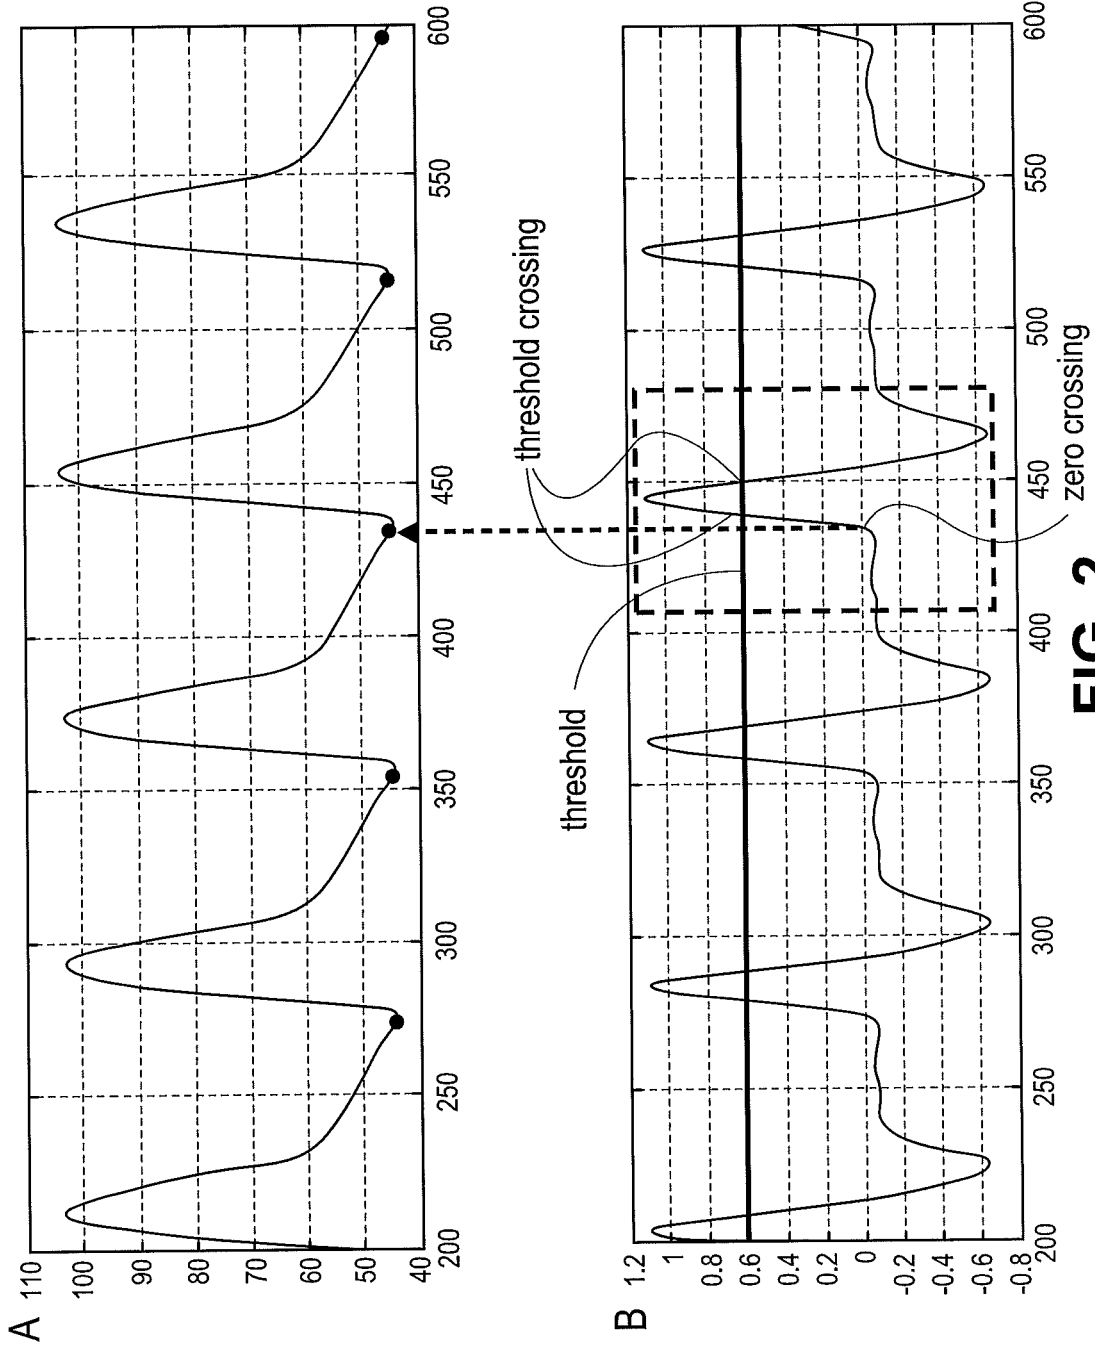


FIG. 2

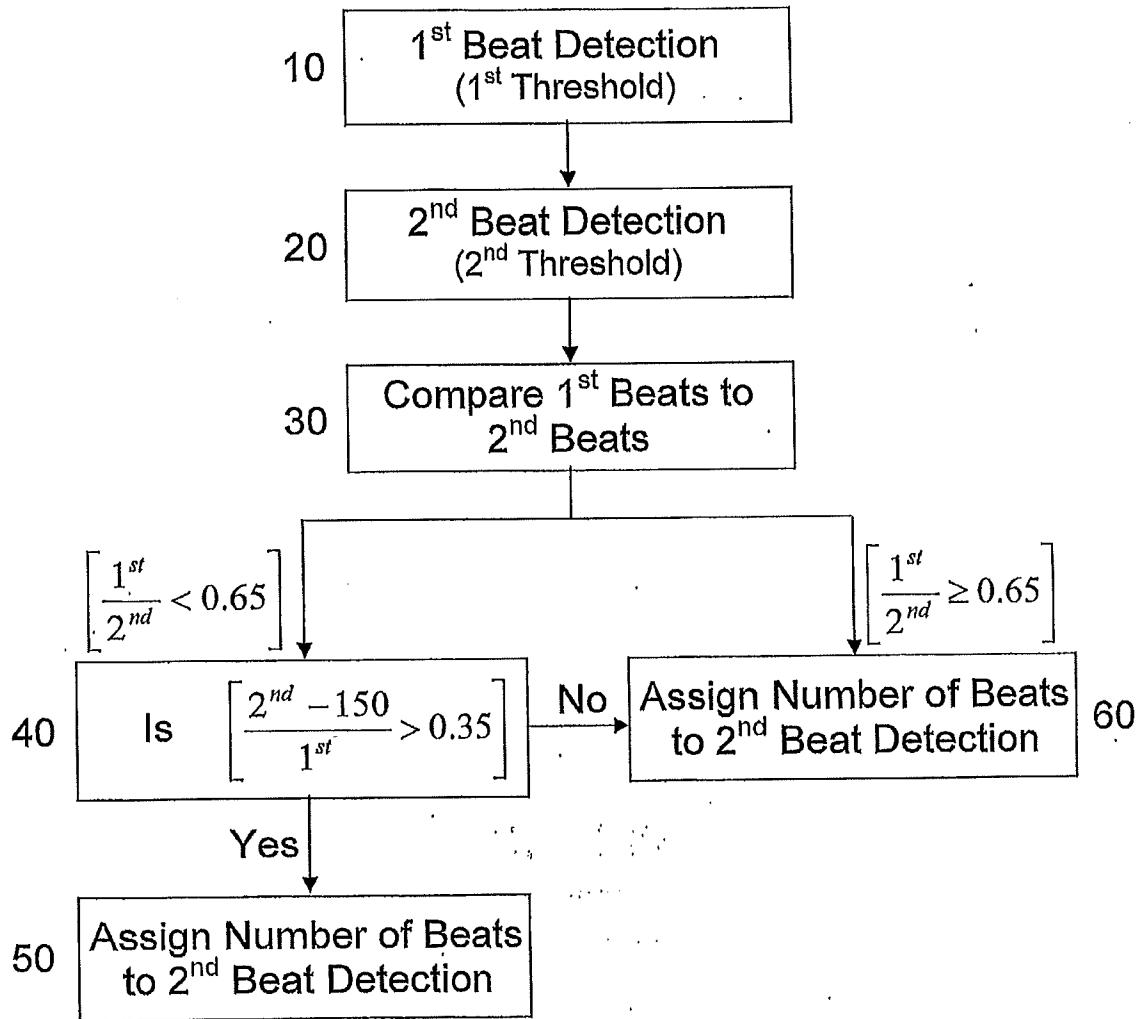
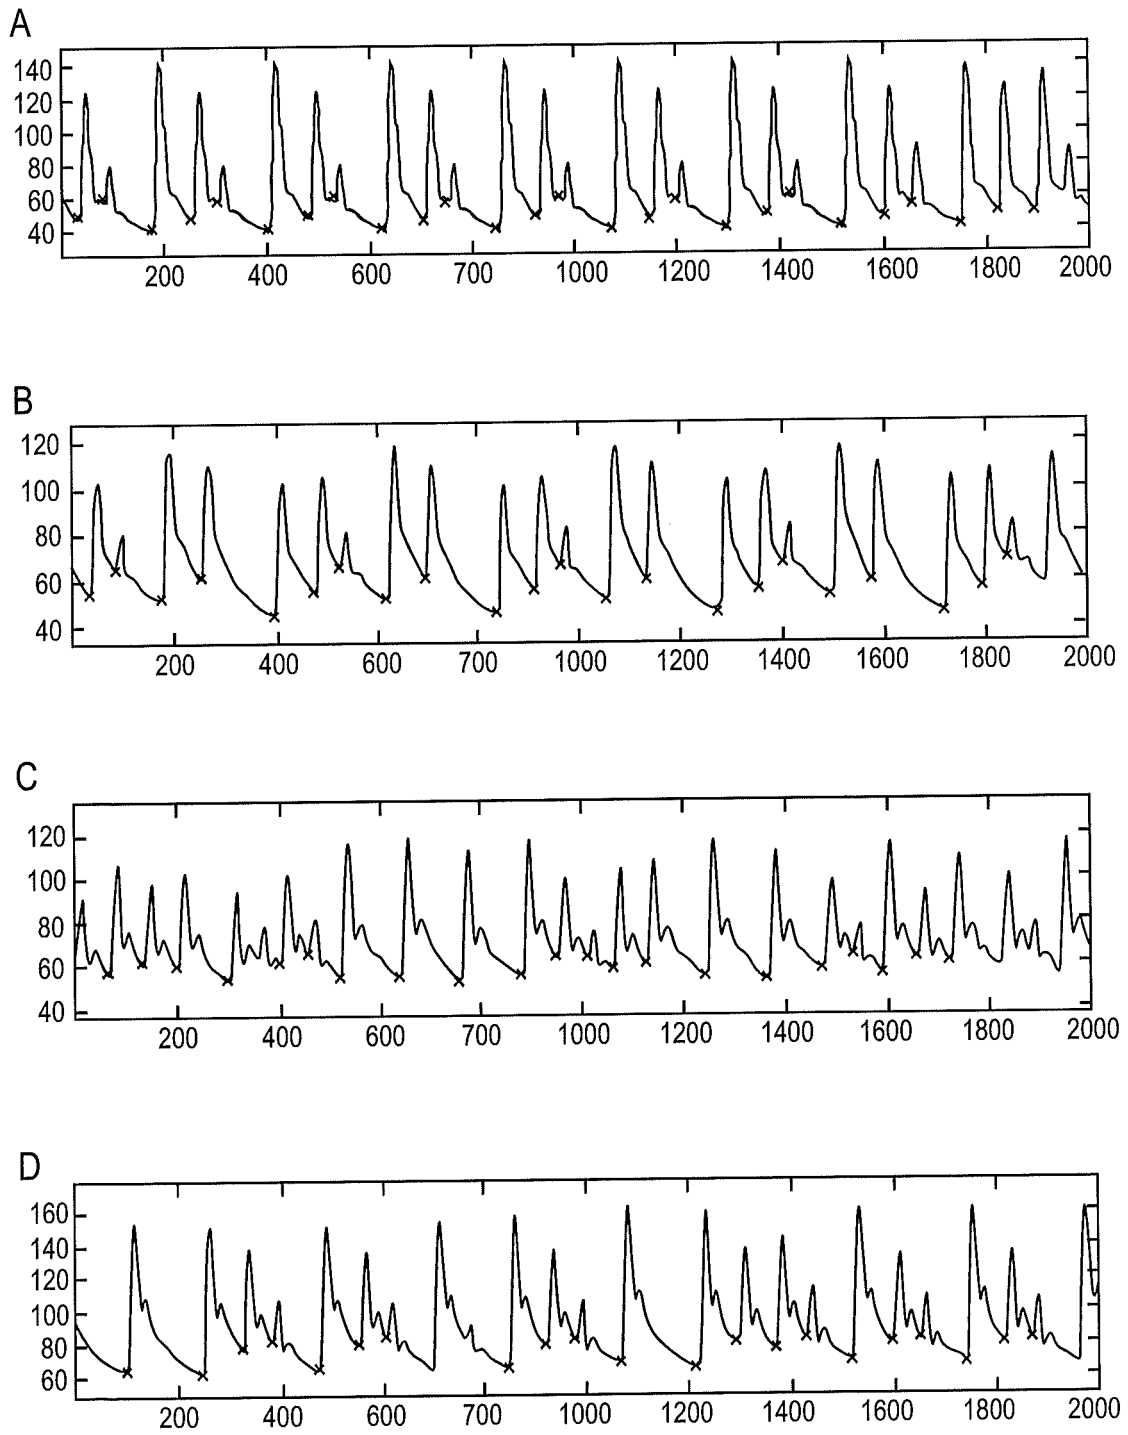


Fig. 3



**FIG. 4**

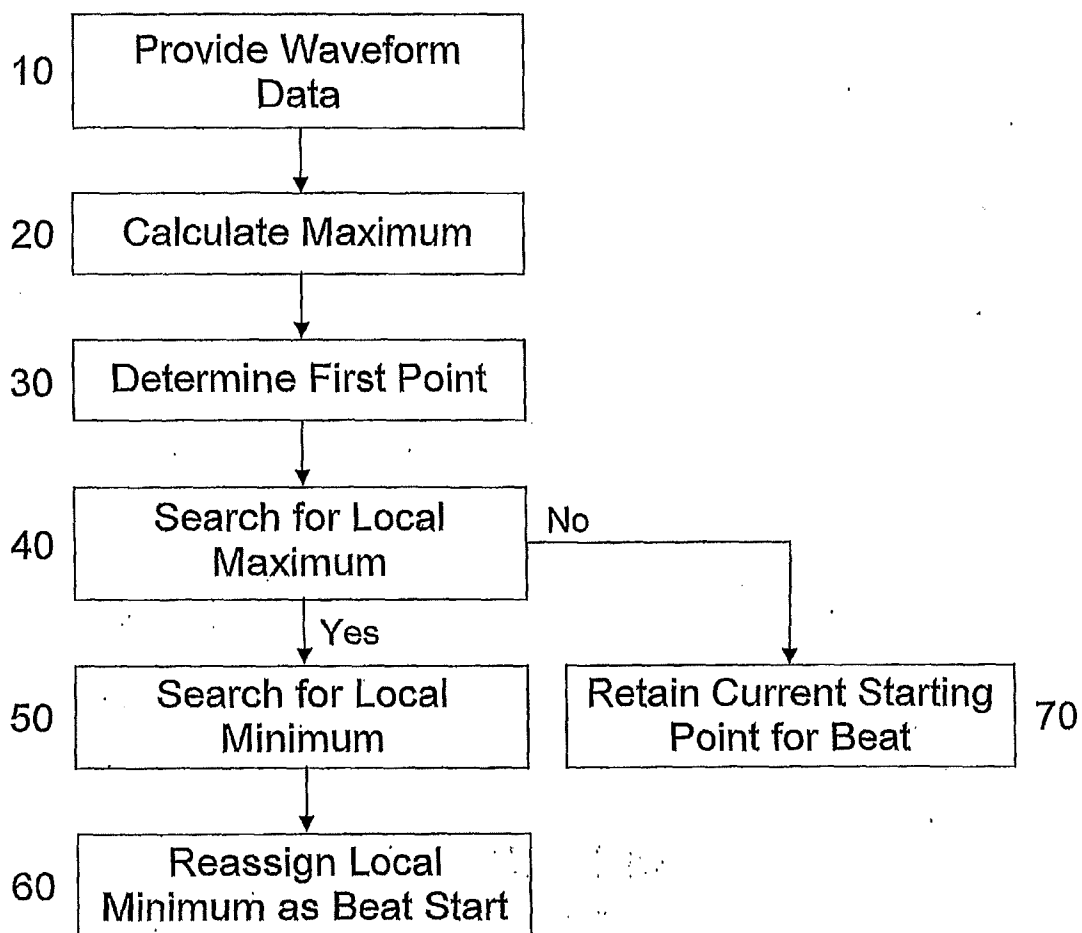


Fig. 5

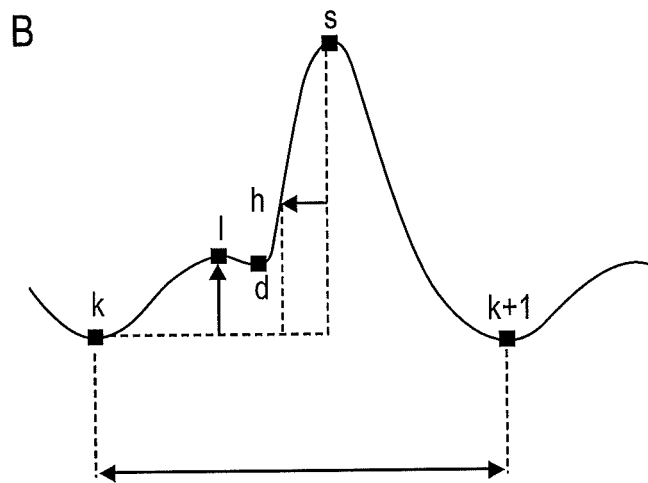
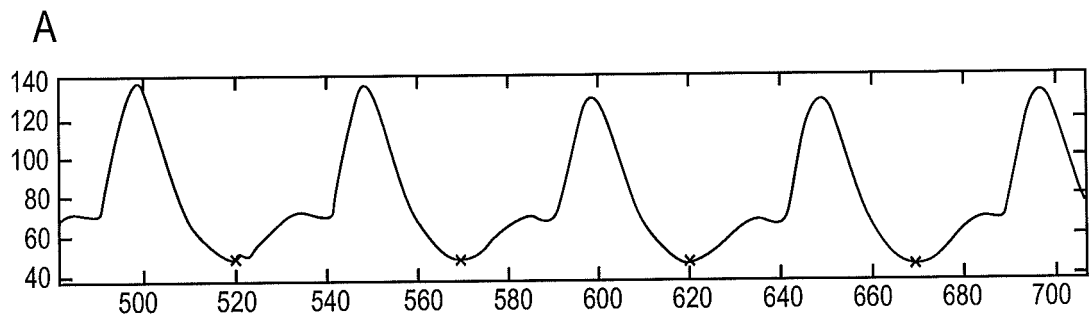


FIG. 6

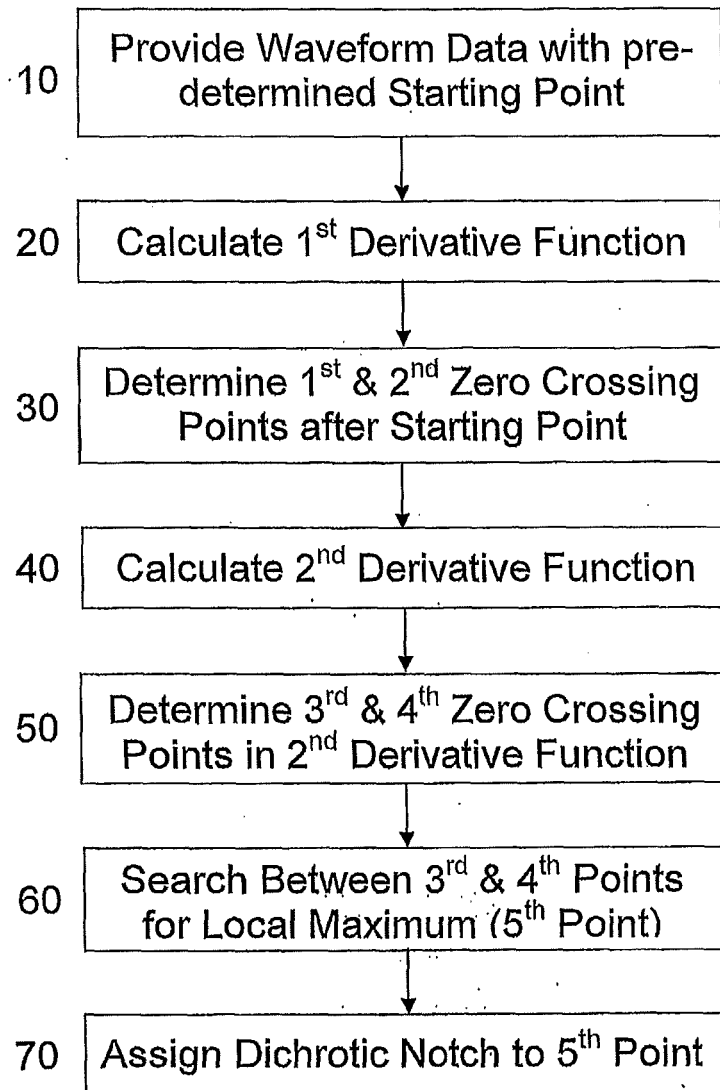
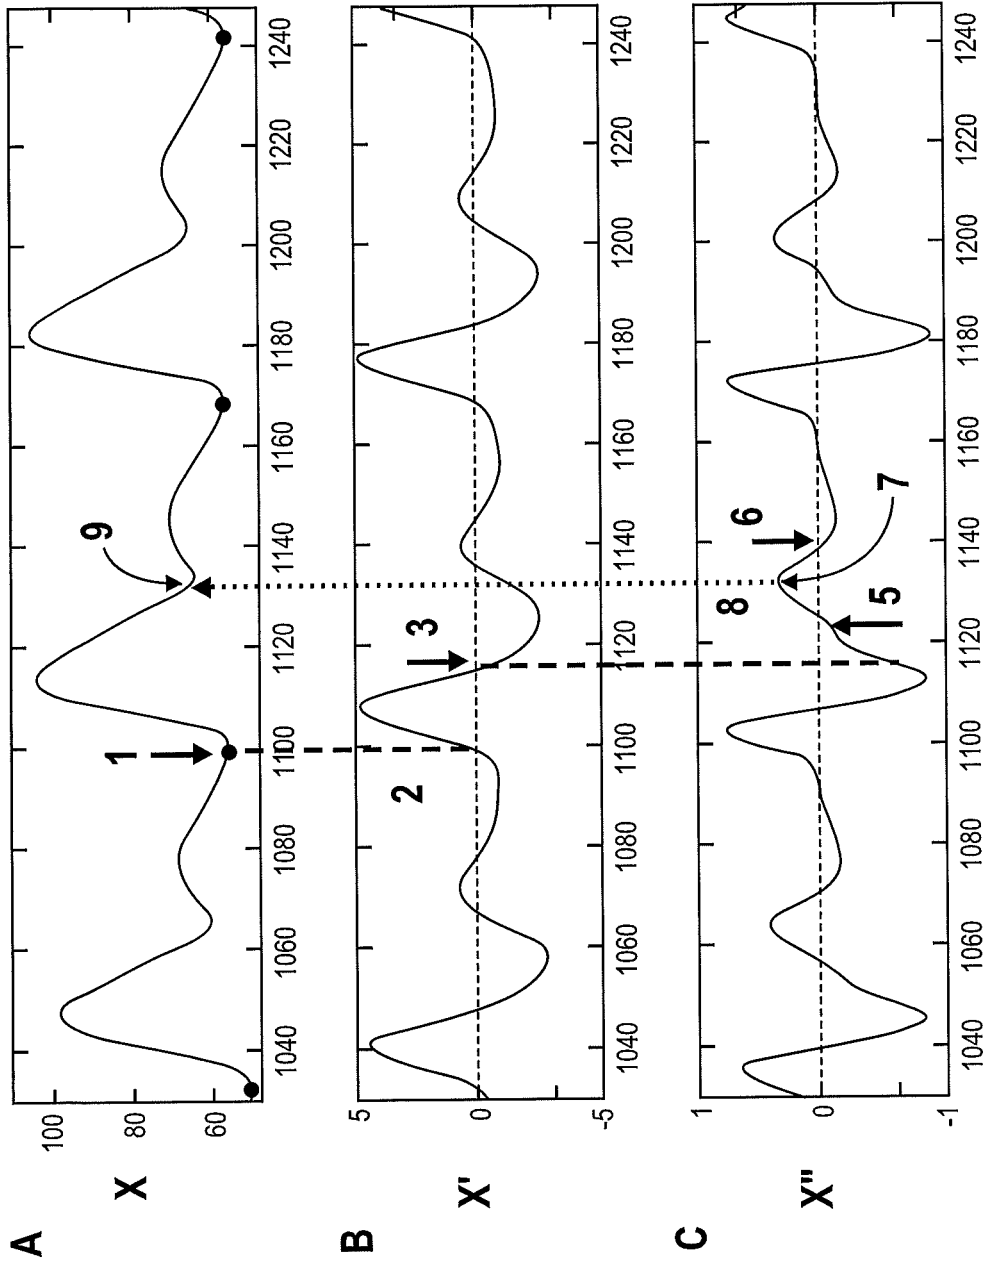


Fig. 7



**FIG. 8**



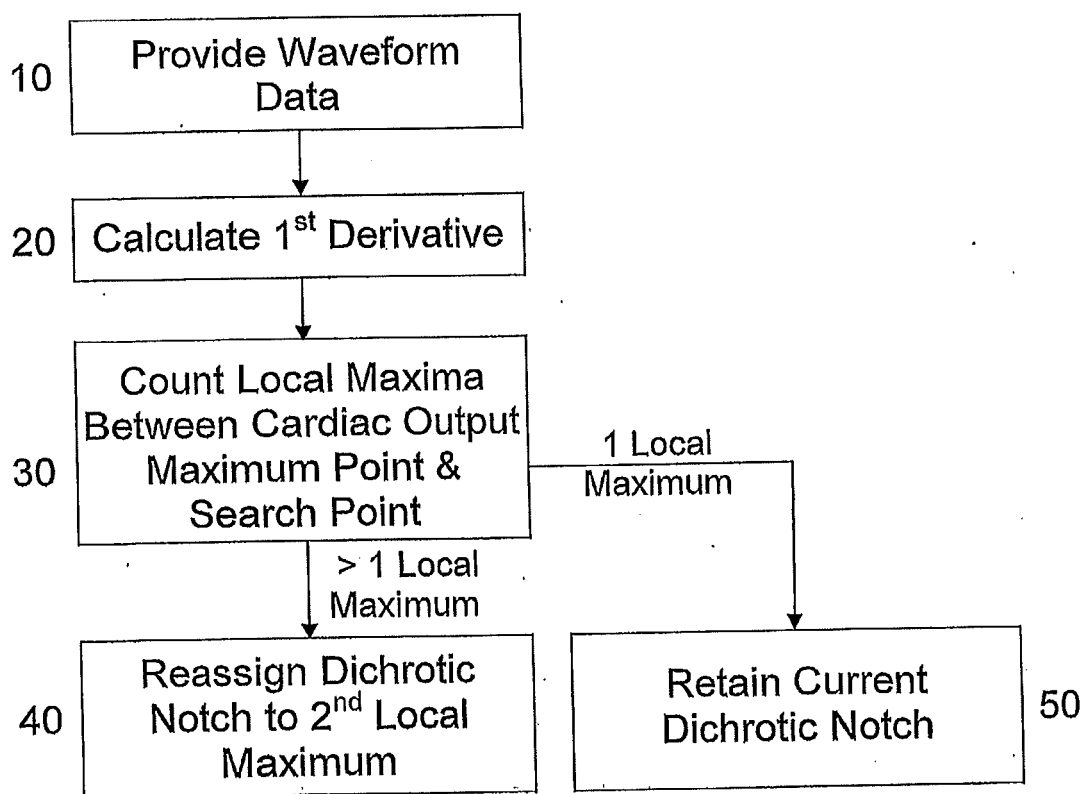


Fig. 9

**A**

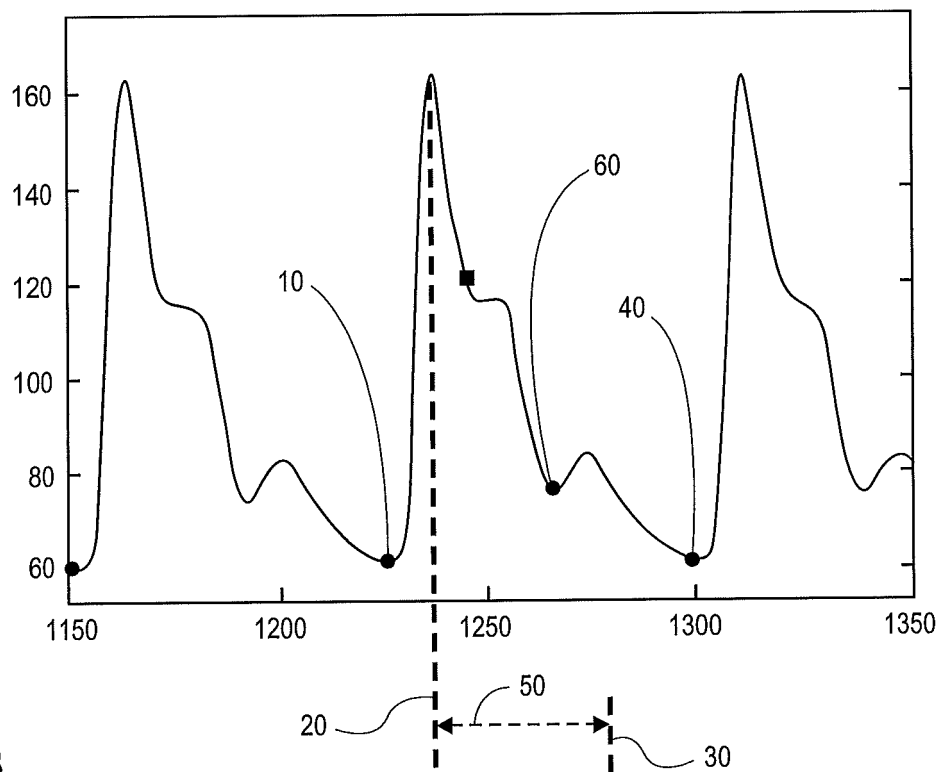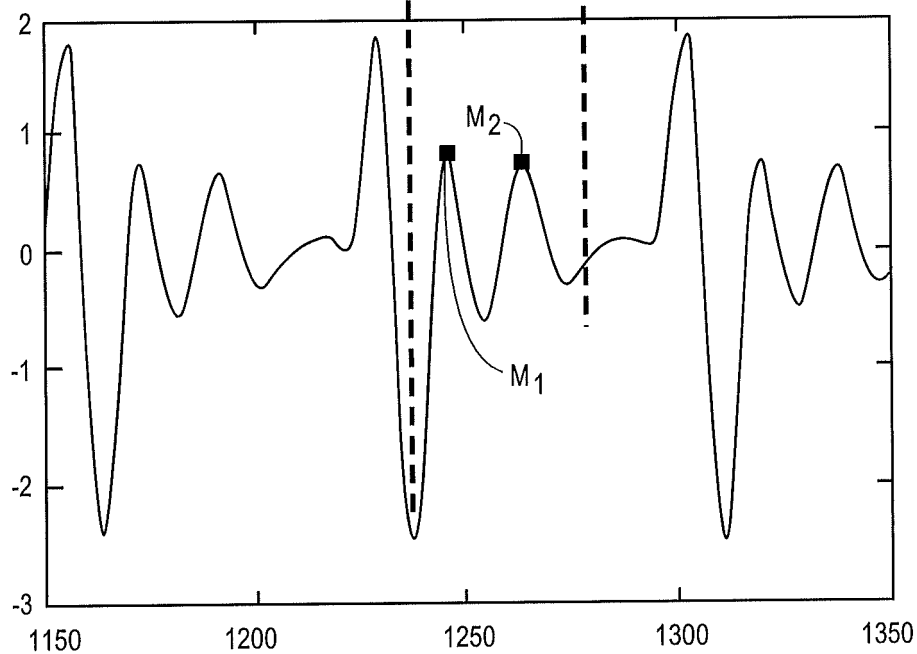

**B**



**FIG. 10**

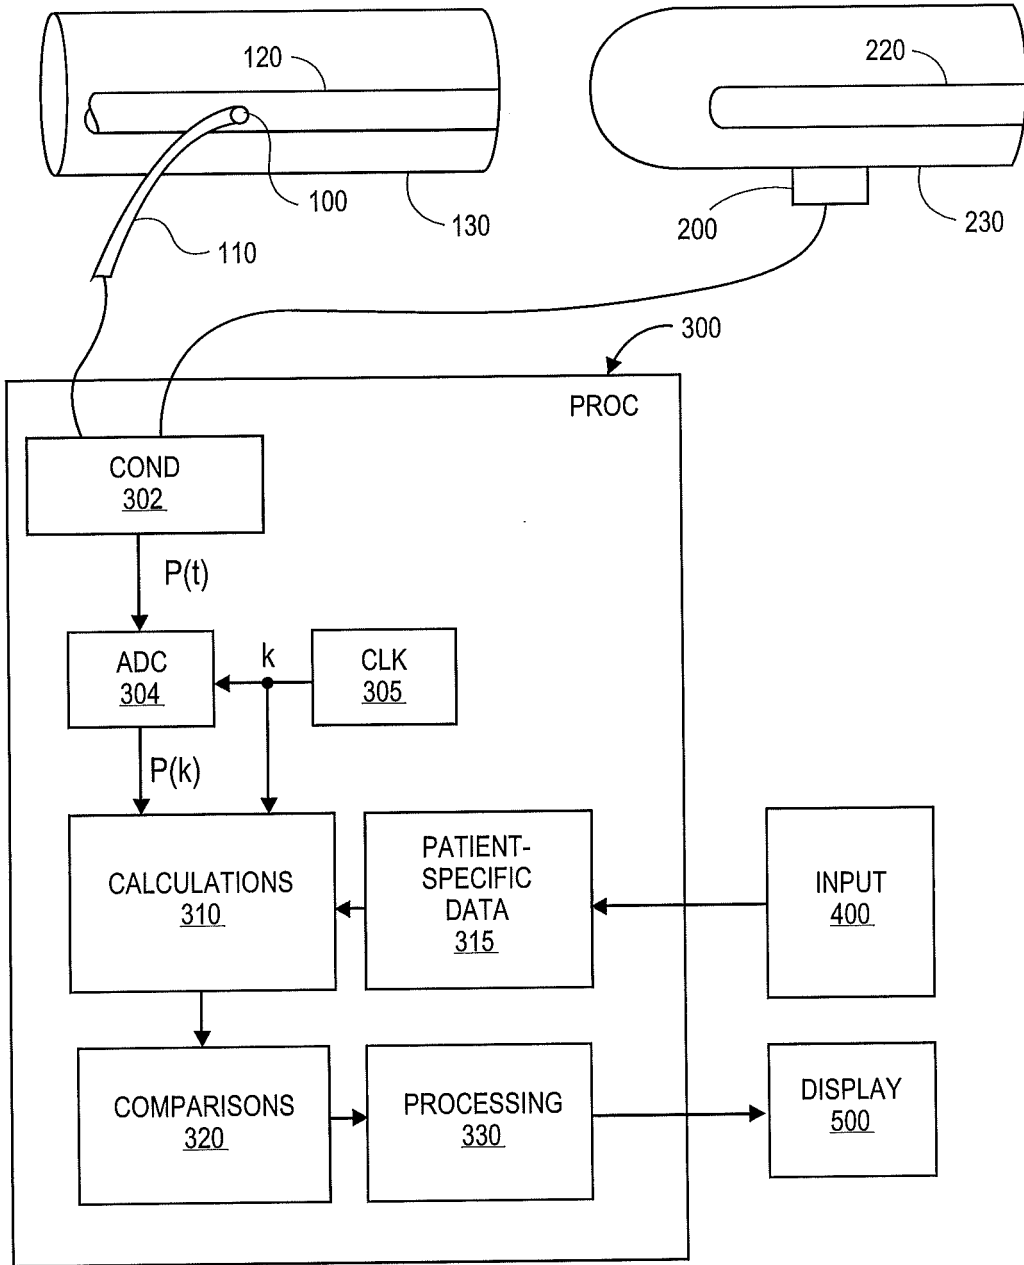


FIG. 11

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 20040147850 A1 [0002]

专利名称(译)	检测心输出量相关波形中的参数		
公开(公告)号	<a href="#">EP2939592B1</a>	公开(公告)日	2019-06-19
申请号	EP2015168200	申请日	2010-02-11
[标]申请(专利权)人(译)	爱德华兹生命科学公司		
申请(专利权)人(译)	爱德华兹生命科学公司		
当前申请(专利权)人(译)	爱德华兹生命科学公司		
[标]发明人	HATIB FERAS ROTELIUK LUCHY D		
发明人	HATIB, FERAS ROTELIUK, LUCHY D.		
IPC分类号	A61B5/02 A61B5/021 A61B5/024 A61B5/00		
CPC分类号	A61B5/02028 A61B5/021 A61B5/024 A61B5/7239 A61B5/029 A61B5/725		
优先权	61/151670 2009-02-11 US 12/699540 2010-02-03 US PCT/US2010/023841 2010-02-11 WO		
其他公开文献	EP2939592A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

描述了用于检测心输出相关波形中的参数的方法。该方法包括用于检测心输出相关波形中的各个心跳周期的方法，用于检测心输出相关波形中的个体心跳周期的指定起始点中的误差的方法，用于检测个体心脏的二色性切口的方法心输出相关波形中的拍频周期，以及用于检测心输出相关波形中的单个心跳周期的指定双重凹口中的误差的方法。这些参数的识别对于临床医生是重要的，因为这些参数形成了计算许多其他心输出量相关参数的基础。

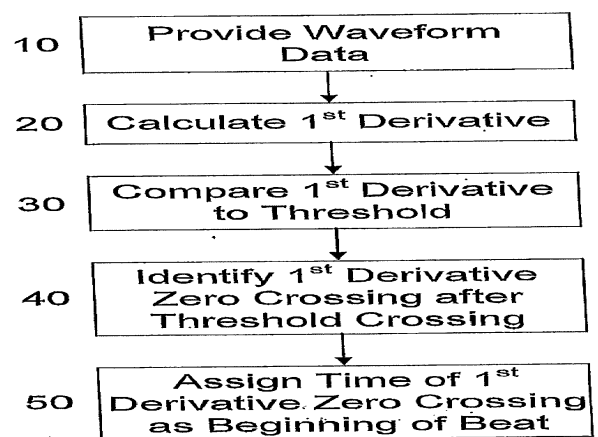


Fig. 1