



- (51) International Patent Classification:
A61B 5/022 (2006.01) *A61B 5/00* (2006.01)
- (21) International Application Number:
PCT/US2018/034078
- (22) International Filing Date:
23 May 2018 (23.05.2018)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
62/509,877 23 May 2017 (23.05.2017) US
15/984,634 21 May 2018 (21.05.2018) US
- (71) Applicant: EDWARDS LIFESCIENCES CORPORATION [US/US]; One Edwards Way, Irvine, CA 92614 (US).
- (72) Inventor: SETTELS, Jacobus Jozef, Gerardus Maria; Edwards Lifesciences, One Edwards Way, Legal Department, Irvine, CA 92614 (US).
- (74) Agent: CRAPENHOFT, Michael et al.; Edwards Lifesciences, One Edwards Way, Irvine, CA 92614 (US).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(54) Title: METHOD FOR CORRECTING CUFF PRESSURE IN A NON-INVASIVE BLOOD PRESSURE MEASUREMENT

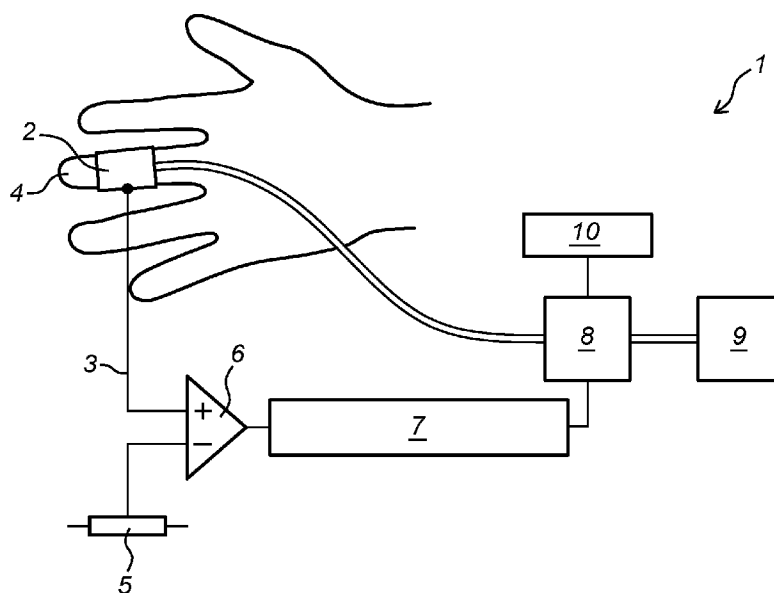


Fig. 1

(57) Abstract: A method for correcting cuff pressure in a non-invasive continuous blood pressure measurement with a plethysmograph comprising the steps of: determining a value of the plethysmograph signal corresponding to a predetermined arterial volume, and setting the determined value as set point; comparing measured plethysmograph signals with the set point; monitoring the adjustments of the cuff pressure for a certain amount of heartbeats; storing the pressure adjustments of the cuff during at least one first heartbeat; applying a varying cuff pressure to the pressure cuff during at least one second heartbeat and measuring the corresponding signals of the plethysmograph; using the stored pressure adjustments of the first heartbeat, the cuff pressure and plethysmograph signal of the second heartbeat, to determine a pressure-volume relation; and determining a value of the plethysmograph signal corresponding to predetermined arterial volume, based on the determined relation; and setting the determined value as new set point.



(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

Method for correcting cuff pressure in a non-invasive blood pressure measurement

The present invention relates to a method for correcting cuff pressure in a non-
5 invasive continuous pressure blood pressure measurement, as well as to a device
for carrying out said method.

It has been known for several years to measure blood pressures wherein a
pressure cuff is placed around a body extremity, such as a finger. EP 0 048 060 for
10 instance describes that the pressure of a fluid inside the pressure cuff is controlled
on the basis on a signal of an optical plethysmograph by a pressure valve, in turn
controlled by a control loop.

The signal of the optical plethysmograph is representing the volume of blood inside
15 the blood vessels of the finger. The more blood inside the vessels, the more light
from a light source of the plethysmograph is absorbed, which results in a lower
signal of the detector side of the plethysmograph (and vice versa). During every
heartbeat, blood is forced through the blood vessels in the finger, causing the
vessels to expand and allow more blood to flow through the vessels. This also
20 causes a volume increase of the vessels, and thus a signal decrease of the
plethysmograph.

In the known method, the cuff pressure of the pressure cuff is controlled such that
the signal of the plethysmograph, and thus the volume of blood inside the blood
25 vessels, is kept constant. The pressure exerted on the internal blood vessel walls
is continuously counteracted by a pressure exerted by the pressure cuff on the
external blood vessel walls, which results in a constant diameter of the blood
vessels and an unloading of the vessels. The counter pressure exerted by the
pressure cuff is a measure for the actual blood pressure inside the blood vessel,
30 and allows for a continuous non-invasive blood pressure measurement.

This control is arranged such that at any moment the difference between a servo
reference level or set point value for the diameter of the blood vessels and the
actual plethysmograph signal or real value is minimized, ideally to zero. The servo-

reference level in the known method is initially determined automatically and the servo feedback control is operated in a way such that the cuff pressure continuously corresponds substantially with the momentary arterial pressure under the cuff both for pulsations and for absolute pressure level.

5

The known method requires correction of the reference or set point value over time. This correction is required mainly due to changes in the physiological status of the measured body part. US 4,510,940 for instance describes a method and a device for correcting the cuff pressure in the indirect, non-invasive and continuous measurement of the blood pressure in a part of the body by using a plethysmograph in a fluid-filled pressure cuff, an electronic control circuit, and an electric pressure valve. The cuff pressure is controlled by the plethysmograph signal in closed-loop operation with the aid of a servo-reference level obtained via a memory circuit. The servo-reference level, in operation of the device, is adjusted by opening the closed loop of the control circuit for a short interval, after which, in open-loop operation the cuff pressure is adjusted at an intermediate pressure derived from the pressure last measured and the servo-reference level is adjusted via the memory circuit.

10

15

Although these methods work, the servo-reference level is adjusted or corrected based only on volume measurements of the plethysmograph as a function of time, over only a part of the heart beat duration, and with only constant cuff pressures. These reference computations make assumptions on the blood pressure levels inside the vessels over the time of the correction computation and are sensitive to external influences. Also, these methods are relatively slow. For adjustment determination of the reference level, often several heartbeats are required to determine the response in volume to many different pressures in the pressure cuff, during which heartbeats a measurement of the blood pressure cannot be performed.

25

30

It is therefore an objective of the present invention to provide an improved method for correcting cuff pressure in a non-invasive continuous blood pressure measurement.

The invention thereto provides a method for correcting cuff pressure in a non-invasive blood pressure measurement with a plethysmograph in a fluid filled pressure cuff wrapped around a body part, such as a finger, comprising the steps of: varying pressures inside the pressure cuff and measuring the corresponding signals of the plethysmograph; determining a value of the plethysmograph signal corresponding to a predetermined arterial volume, in particular the un-stretched or unloaded arterial volume; and setting the determined value as set point; comparing measured plethysmograph signals with the set point for a servo system; adjusting cuff pressure in the pressure cuff to minimise the difference between the measured signals and the set point; monitoring the cuff pressure for a certain amount of heartbeats; storing the pressure adjustments of the cuff during at least one first heartbeat; applying a varying cuff pressure to the pressure cuff during at least one second heartbeat and measuring the corresponding signals of the plethysmograph; using the stored pressure adjustments of the at least one first heartbeat, and the cuff pressure and plethysmograph signal of the at least one second heartbeat, to determine a pressure-volume relation of the blood vessel under the cuff; and determining a value of the plethysmograph signal corresponding to predetermined arterial volume, preferably an un-stretched arterial volume, based on the determined relation; and setting the determined value as new set point. A fluid according to the invention may for instance be a liquid such as water, or a gas like air.

In the method according to the invention, the blood pressure inside the blood vessel is followed for a certain period of time, to monitor the blood pressure. To do so, a first set point is determined, which approximately corresponds to an unloaded volume of the blood vessel. The pressure in the cuff is adjusted to keep the volume constant, and this pressure is thus a measure for the internal blood pressure (or intra-arterial pressure). Due to multiple factors, this set points typically drifts with time such that calibration, or setting a new set point, is required after a certain period of time.

The set point, or unloaded volume of the blood vessel, can be determined based on a pressure-volume relation between the transmural pressure, which is the internal blood pressure (or intra-arterial pressure) minus the cuff pressure, and the

volume of blood inside the blood vessel. The volume is determined by the plethysmograph signal. In the determination of the transmural pressure, the cuff pressure is available and adjustable, but the present (or actual) internal blood pressure is an unknown.

5

However, changes between blood pressure waveforms generally occur gradually, and if they differ from one heartbeat to the next, the changes are mostly in pulse pressure, which changes can be predicted based on changes of the duration of the heart beat and compensated for. In the determination of the pressure-volume
10 relation according to the invention, the second set of blood pressure waveform for the second heart beat is assumed to be identical to the first set of blood pressure waveform or assumed to be correctly adapted from the first based on heart beat interval. Instead of the present blood pressure in the blood vessel, the blood pressure of the first, preceding set is used. The pressure of the cuff can now be
15 chosen dynamically to cover a range of pressures suitable for the determination of the pressure-volume relation.

The advantage of such method is that a large dynamic range of transmural pressures may be used to compute an actual pressure-volume relation of the
20 blood vessel on which the set point is based, whereas in the prior art the set point is based only a determination on volume information over time.

Another advantage of such method is that it is relatively fast. Because the internal blood pressure, or intra-arterial pressure, is assumed to be known, only one or two
25 heartbeats are required which can be used to dynamically cover a large range of transmural pressures, as the cuff pressure may be varied based on the information from the assumed intra-arterial pressure.

Another advantage of such method is that it allows the analysis of visco-elastic
30 properties of the arterial wall of the blood vessel by determining the phase relationship, compliance and hysteresis characteristics between the transmural pressure dynamics and the resulting volume dynamics.

The beat duration of the second heart beat can be determined from the first heartbeat, and the pulse pressure of the second heart beat can be adapted when the beat duration differs from the first heartbeat.

- 5 The at least one first heartbeat and the at least one second heartbeat may comprise the same number of heartbeats, for instance one or two heartbeats.

The method according to the invention may repeat the monitoring of blood pressure and correcting the set point after a number of heartbeats. Because the
10 correction of the set point only takes one or a few heartbeats to perform, and the blood pressures during these heartbeat(s) are available as predicted by simulation, only a little bit of actual blood pressure measurement is lost. This allows for as many corrections over time as needed, which improves the quality of the blood pressure determination.

15

The varying cuff pressure applied during the at least one second heartbeat may comprise a pressure below venous pressure in the body part under the cuff and distal to it. In the finger, the use of a pressure cuff to determine arterial blood pressure in the described way typically blocks or impedes to a major extent the
20 venous return of blood, since the cuff pressure, equalling the arterial pressure, exceeds the venous pressures. The venous blood vessels under the cuff are thus typically collapsed during blood pressure measurements with pressure cuffs. Same is true for the capillary bed under the cuff. This will, after a period of time, result in venous congestion in the body part distal to the cuff, increased venous and
25 capillary pressure and potentially reduced oxygenation in the extremity of the body part, such as the fingertip. When the varying cuff pressure applied during the at least one second heartbeat comprises a pressure below the venous pressure in the fingertip, it allows venous return from the distal part of the extremity to the collecting veins, and avoids to abovementioned congestion problems. In order to
30 achieve this, the cuff pressure below fingertip venous pressure may lie between 0 and diastolic arterial pressure, preferably between 0 and 50 mmHg, in particular around 30 mmHg.

The varying cuff pressure applied during the at least one second heartbeat may be a dynamic pressure waveform, such as a sinusoidal waveform. Because the arterial pressure is assumed to be known during the second heartbeat, the pressure-volume relation may be determined with any cuff pressure. The pressure-volume relation relies on the transmural pressure over the arterial wall and the corresponding volume information based on the plethysmograph signal. The transmural pressure is the difference between the cuff pressure and the arterial pressure. As the blood pressure has a somewhat sinusoidal progression itself also, a sinusoidal cuff pressure waveform in counter phase with the blood pressure waveform would allow to generate transmural pressures over a relative large range along with its volume information from the plethysmograph, both positive and negative transmural pressures.

The varying cuff pressure applied during the at least one second heartbeat may also be a ramp waveform, wherein preferably the lowest pressure below diastolic pressure in the body part allows venous return in the body part, and/or the highest pressure is above systolic pressure in the body part. The ramp pressure can be in phase or in counter phase with the blood pressure dynamics, or any phase relationship in between. A ramp in pressure is relatively easy to apply. The ramp waveform may comprise multiple ramps, such that the waveform is more like a saw tooth waveform.

The varying cuff pressure applied during the at least one second heartbeat may be chosen such that the transmural pressure between the blood vessel of the body part and the cuff pressure is set over a predetermined range. The transmural pressure depends on the arterial pressure and the cuff pressure, of which the arterial pressure is known, and the cuff pressure can be set. In order to determine the transmural pressure over a predetermined range, the cuff pressure can be varied based on the arterial pressure. The varying pressure profile may thus be determined based on the stored blood pressure of the at least one first heartbeat.

The method may further comprise the step of determining the central blood pressure based on the measured blood pressure inside the body part, preferably the finger. When the blood pressure inside the body part is transformed in the

central blood pressure, measurements of different body parts may be compared, as all can be related to central blood pressure. Central blood pressure is for instance the aortic blood pressure or the brachial blood pressure.

5 The step of using the stored pressure adjustments of the at least one first heartbeat, and the cuff pressure and plethysmograph signal of the at least one second heartbeat, to determine a pressure-volume relation for instance involves plotting the transmural pressure against the volume signal of the plethysmograph. In each heartbeat, this pressure/volume relation substantially forms a loop, with an
10 upswing and a downswing distinguished from each other because of the hysteresis of the arterial wall. The gradient, or angle/steepness of these swings is a measure for the compliance of the blood vessel being measured. In order to better study this gradient or steepness, instead of the volume one could take the first derivative of the volume signal, and plot this derivative over the transmural pressure. The
15 location where this first derivative is maximal (or where a second derivative would be zero) represents the transmural pressure with maximal compliance. This transmural pressure could be used in the pressure-volume relation to determine the volume where compliance is maximal, and it is this volume which could serve as new set point according to the invention.

20

The invention further relates to a device for correcting cuff pressure in a non-invasive blood pressure measurement with a plethysmograph in a fluid filled pressure cuff wrapped around a body part, such as a finger, comprising a pressure cuff, provided with: a bladder, for wrapping around the body part and applying
25 counter pressure; a light source, for sending light through the body part, and a light detector, for detecting the light passed through the body part and for providing a signal in dependence of the amount of detected light; a pressure generator, for supplying pressurized fluid to the bladder; a controller, for adjusting the pressure of the fluid supplied to the bladder based on the signal, and for determining the blood
30 pressure inside the body part; a memory, for storing the determined blood pressure of at least one first heartbeat; wherein the controller is arranged to apply a varying dynamic cuff pressure during at least one second heartbeat, and to receive the signal during the at least one second heartbeat, and wherein the controller is arranged to determine a pressure volume relation based on the stored

blood pressure of the at least one first heartbeat, the signal of the at least one second heartbeat and the varying cuff pressure applied during the at least one second heartbeat.

- 5 The device may further comprise a pressure sensor arranged to determine the pressure inside the bladder. The pressure inside the bladder is an indication of the blood pressure inside the body part when the pressure is adjusted to maintain a constant plethysmograph signal.
- 10 The invention will be explained by means of the non-limiting working examples depicted in the following figures. Specifically:
- figure 1 schematically shows a device for non-invasive blood pressure measurements according to the present invention;
 - figure 2 schematically shows a first approximate determination of the set point according to the present invention;
 - 15 - figure 3 schematically shows the monitoring of blood pressure after the first setting of the set point according to the present invention;
 - figures 4A-4E schematically shows the determination of a new, changed, set point according to the present invention; and
 - 20 - figure 5A-5E shows the actual determination of a new, changed, set point according to the present invention using a ramp as the varying cuff pressure and
 - figure 6A-6E shows the actual determination of a new, changed, set point according to the present invention using a sinusoidal waveform as the
 - 25 varying cuff pressure.

Figure 1 schematically shows a device (1) for non-invasive blood pressure measurements, comprising a pressure cuff (2), which generates a signal (3) based on the detected light. This signal (3), representative for the volume of blood in the finger arteries (4) is compared to a set-point (5) by a comparator (6), which comparison is then communicated to a controller (7). Based on the information, the controller (7) in turn controls a control valve (8). The valve (8) regulates the pressure supplied to the pressure cuff (2) by a pump (9). The pressure supplied to the pressure cuff (2) is measured by a transducer (10).

Figure 2 schematically shows a first determination of the first set point (SET). In the upper graph, the pressures (P_{cuff}) inside the pressure cuff are plotted over time (t). The pressures are varied in this example by applying them in a step pattern with increasing cuff pressures. Such pattern can however be selected from a number of patterns, also for instance including a ramp pattern.

In the bottom graph, the corresponding plethysmograph signal is shown. At low cuff pressures (on the left of the graph), the arteries of the finger are open and a large amount of blood is present in the arteries. The plethysmograph signal (PLET), corresponding to the amount of blood in the measured arteries, is thus relatively high. At high cuff pressures (on the middle/right of the graph), the cuff exerts a large pressure on the finger and the arteries, causing them to collapse at least partially during the diastolic phase of the heartbeat. This collapse of the arteries reduces the blood volume, and thus results in a decreased plethysmograph signal.

The blood pressure in the arteries also pulsates with every heartbeat. Every heartbeat blood is expelled from the heart into the aorta during systole, which is followed by the filling of the heart during diastole. The pressure in the arteries follows the same pattern, and increases due to the expulsion of blood, and decreases during filling of the heart. This pulsation causes an expansion of the arteries in the finger, and thus in a varying volume of blood in the arteries. This varying volume also results in a varying plethysmograph signal.

The variations in the plethysmograph signal are small when the cuff pressure is high (for instance above systolic pressure), as the arteries are subjected to high external pressures, working against the internal pressure variations. The variations in the plethysmograph signal are also small when the cuff pressure is low (for instance below diastolic pressure), as then arteries are loaded by the blood pressure from within.

When the external pressure of the pressure cuff and the internal blood pressure of the arteries are close or equal, they balance each other out. This is also referred to

as the unloaded state of the arteries, wherein the pressure difference over the arterial walls (also referred to as transmural pressure) is zero. In this state, the varying blood pressure causes, relatively unobstructed and directly, the expansion of the arteries. It is in this state that the variations in the plethysmograph signal are largest. The initial set point, is for instance chosen as the middle between the top and bottom of the plethysmograph signal where the variations are largest. This procedure does not provide a very accurate volume set point, but it suffices to start a measurement with the new set point adjustments as described, which quickly converges to a stable and more accurate volume set point value.

10

Figure 3 schematically shows the monitoring of blood pressure after the setting of the initial set point. The pressure in the cuff (P_{cuff}) is varied such that the plethysmograph signal (PLET) is kept constant, at the set point value. The pressure in the cuff is now representing the blood pressure inside the arteries.

15

The set point, representing the predetermined or unloaded volume of the arteries, changes over time. Performing the same step pattern in cuff pressures to determine the changed set point takes a relative long time to do, and is not very accurate and the blood pressure measurement is then temporarily not available.

20

Figure 4 schematically shows the determination of the information leading to a new, changed, set point. Figure 4A shows a changing pressure in the cuff, P_{cuff} , and figure 4B shows the changing plethysmograph signal over that time, PLET. In figure 4A, the blood pressure is monitored for a number, for example four, heartbeats before determination of the new set points. During this monitoring the plethysmograph signal (PLET) in figure 4B is kept constant at or around the previously determined set point, and the pressure in the cuff is adjusted accordingly.

25

The cuff pressures, representing blood pressures, of the last two heartbeats (11) are stored. In figure 4 two heartbeats are stored, but the same can hold for one or more heartbeats. For the next two heartbeats (12), the blood pressures are assumed to be identical to the stored heartbeats (11), as indicated with the dotted line (13) in the upper graph of figure 3. During these two heartbeats (12), a varying

30

cuff pressure pattern (P_{cuff}) is applied to the pressure cuff, as indicated by e.g. the ramp (14). The plethysmograph signal (PLET) is measured over this range of cuff pressures.

- 5 The blood pressures during the two heartbeats are known, as they are assumed to be the same as the previous two heartbeats. In addition, they can be slightly modified based on the variation in heart beat interval. The cuff pressures (P_{cuff}) during the two heartbeats are the pressures according to the ramp (14), and the blood volume in the arteries is provided by the plethysmograph signal (PLET). The
10 pressure over the arterial walls, or transmural pressure, is the difference between the cuff pressure and the arterial blood pressure, and can thus be determined. The volume can subsequently be plotted as a function of transmural pressure.

Figure 4C schematically shows a pressure volume relation according to the
15 invention, which can be obtained using the steps described with regard to figures 4A and 4B. For sake of simplicity, the relation is shown for a single heartbeat. On the horizontal axis, the transmural pressure (P_{tr}) is shown, which pressure is the internal blood pressure, or arterial pressure, minus the cuff pressure. On the vertical axis, a volume (in internal units) is shown, which is provided by the signal
20 received by the plethysmograph. In the shown relation, two curves (A, B) can be identified, curve A being related to the inflow and curve B being related to the outflow of blood. The gradient, or steepness, of each of the curves is a measure for the compliance of the blood vessel, and is the derivative of these curves.

- 25 Figure 4D schematically shows the (first) derivative of these curves (A, B) schematically. For each of these curves (A, B) a maximum can be determined, which corresponds to a certain transmural pressure (P_{tr}), one for curve A (C), and one for curve B (D). Figure 4E schematically shows how these transmural pressures where compliance is maximal can be used to determine a new set point.
30 The new (volume) set point is the volume (15) in the pressure-volume relation as for instance shown in figure 4C which corresponds to the transmural pressures where compliance is maximal. This volume (15), will be the new (volume) set point (V_{set}) of the plethysmograph. It should be noted that the actual transmural pressure is used in this method (just) for referencing, and its precise value is of minor

relevance. When the two curves (A, B) would have volumes (15) which are not coinciding, but would be different, the new set point could for instance be the average volume of the two volumes (15).

- 5 Figures 5A-5E show the determination of a new, changed, set point according to figure 4 in an actual measurement, using a ramp as the varying cuff pressure. The steps of the determination are according to the ones of figure 4.

- 10 Figures 6A-6E show the determination of a new, changed, set point in an actual measurement, using a sinusoidal waveform as the varying cuff pressure. The steps of the determination are according to the ones of figure 4 and 5.

By including cuff pressure profiles that contain both transitions from low pressure, e.g. below diastolic to high pressure, e.g. above systolic and transitions from high
15 to low pressure, the phase relationship between pressure and volume will show in the pressure-volume diagram as hysteresis if that is present, and provide information on the arteries. The hysteresis will provide at least two different values for the unloaded volume at zero transmural pressure. These values can be used to compute a more accurate determination of the set point at the unloaded volume,
20 by computing an average of the two or more values, where the average can be a weighted average.

Because of its visco-elastic properties, the arterial wall of the body part under the cuffs has low pass filtering characteristics which can be determined by applying a
25 step function in transmural pressure up and down around a predetermined cuff pressure level; this level is preferably at mean arterial pressure or at mid pressure, half way in between systolic and diastolic pressure. The varying cuff pressure in this case has the profile of a step up or down, followed by cuff pressure tracking the pressure inside the finger artery over a certain period, thus keeping the
30 transmural pressure constant over a certain period which preferably is in the order of several 100 milliseconds. The resulting volume transient will have a characteristic which can be approximated by a first order time constant and estimated by the controller. This time constant will vary from person to person, and will vary over time within a person. For better robustness, the average value of the

time constant up and the time constant down can be determined. The resulting time constant value can be used to individualize an important compensation component in the servo feedback loop that maintains the volume to the set point value; to individualize to each patient, and to adapt to changes over time. As a
5 result, the servo will have improved bandwidth which will result in higher quality waveform details. The time constant can also be determined using a step in cuff pressure up or down, followed by a constant cuff pressure over a certain period. In this case, however, the transmural pressure will not be kept constant and the resulting time constant estimate will have a bias depending on the individual
10 pressure shape in the finger artery.

It will be apparent that the invention is not limited to the exemplary embodiments shown and described here, but that within the scope of the appended claims numerous variants are possible which will be self-evident to the skilled person in
15 this field.

Claims

1. A method for correcting cuff pressure in a non-invasive continuous blood pressure measurement with a plethysmograph in a fluid filled pressure cuff wrapped around a body part, the method comprising the steps of:
- a) varying pressures inside the pressure cuff and measuring the corresponding signals of the plethysmograph;
 - b) determining a value of the plethysmograph signal corresponding to an unloaded arterial volume; and setting the determined value as an initial set point;
 - c) comparing measured plethysmograph signals with the set point;
 - d) adjusting cuff pressure in the pressure cuff to minimise the difference between the measured signals and the set point;
 - e) monitoring the cuff pressure for a number of heartbeats;
 - f) storing the pressure adjustments of the cuff during at least one first heartbeat;
 - g) applying a varying cuff pressure to the pressure cuff during at least one second heartbeat and measuring the corresponding signals of the plethysmograph
 - h) using the stored pressure adjustments of the at least one first heartbeat, and the cuff pressure and plethysmograph signal of the at least one second heartbeat, to determine a pressure-volume relation
 - i) determining a value of the plethysmograph signal corresponding to an unstretched arterial volume, based on the determined relation; and setting the determined value as a new set point.
2. A method according to claim 1, comprising step j) of repeating steps c)-i).
3. A method according to claim 1, wherein the varying cuff pressure applied in step g) comprises a pressure below venous pressure in the body part distal to the cuff.

4. A method according to claim 3, wherein the pressure below venous pressure in the body part distal to the cuff reaches values below diastolic blood pressure, preferably between 0 and 50 mmHg, in particular around 30 mmHg.
- 5 5. A method according to claim 1, wherein the varying cuff pressure applied in step g) is a dynamic pressure waveform, in which the lowest pressure is below diastolic pressure in the body part, which allows venous return in the body part, and the highest pressure is above systolic pressure in the body part.
- 10 6. A method according to claim 1, wherein the varying cuff pressure applied in step g) is a ramp waveform in which the lowest pressure is below diastolic pressure in the body part, which allows venous return in the body part, and the highest pressure is above systolic pressure in the body part.
- 15 7. A method according to claim 1, wherein the varying cuff pressure applied in step g) comprises a transition from a low pressure below diastolic pressure to a high pressure above systolic pressure, and thereafter multiple transitions between said low and high pressures.
- 20 8. A method according to claim 1, and further comprising a step of applying a cuff pressure having a step function around a predetermined cuff pressure level, which level is one of (i) mean arterial pressure and (ii) a pressure halfway between systolic and diastolic pressure.
- 25 9. A method according to claim 1, wherein the pressure-volume relation is determined by the signal of the plethysmograph and the transmural pressure between the blood vessel of the body part and the cuff pressure.
- 30 10. Method according to any of the preceding claims, wherein the varying cuff pressure applied during step g) is chosen such that the transmural pressure between the blood vessel of the body part and the cuff pressure is set over a predetermined range.

11. Method according to any of the preceding claims, wherein the varying cuff pressure applied during step g) is determined based on stored blood pressure of the at least one first heartbeat.

5 12. Method according to any of the preceding claims, wherein in step b), the set point value is the volume wherein the amplitude of the plethysmograph signal is maximal.

13 Method according to any of the preceding claims, comprising the step of
10 determining the central blood pressure based on the measured blood pressure inside the body part, preferably the finger.

14. Method according to any of the preceding claims, wherein in step i), the
new set point is determined in relation to the volume where a compliance of the
15 measured body part, such as the finger artery, is maximal.

15. Device for correcting cuff pressure in a non-invasive blood pressure measurement with a plethysmograph in a fluid filled pressure cuff wrapped around a body part, such as a finger, comprising:

- 20 a) a pressure cuff, provided with:
- a. a bladder, for wrapping around the body part and for applying a counter pressure;
 - b. a light source, for sending light through the body part, and
 - c. a light detector, for detecting the light passed through the body part
25 and for providing a signal in dependence of the amount of detected light;
- b) a pressure generator, for supplying pressurized fluid to the bladder;
- c) a controller, for adjusting the pressure of the fluid supplied to the bladder based on the signal, and for determining the blood pressure inside the body
30 part;
- d) a memory, for storing the determined blood pressure of at least one first heartbeat;

e) wherein the controller is arranged to apply a varying cuff pressure during at least one second heartbeat, and to receive the signal during the at least one second heartbeat, and

5 f) wherein the controller is arranged to determine a pressure volume relation based on the stored blood pressure of the at least one first heartbeat, the signal of the at least one second heartbeat and the varying cuff pressure applied during the at least one second heartbeat.

10 16. Device according to claim 15, specifically arranged to perform the method according to any of the claims 1-14.

17. Device according to claim 15 or 16, comprising a pressure sensor arranged to determine the pressure inside the bladder.

15

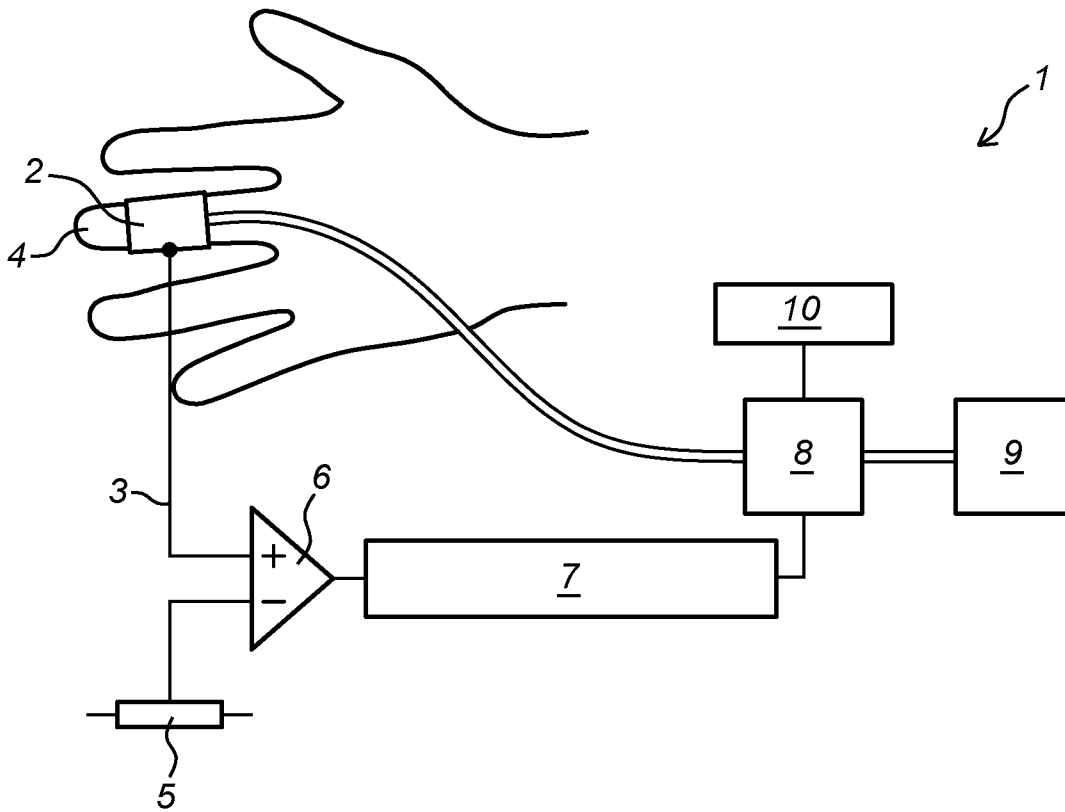


Fig. 1

2/12

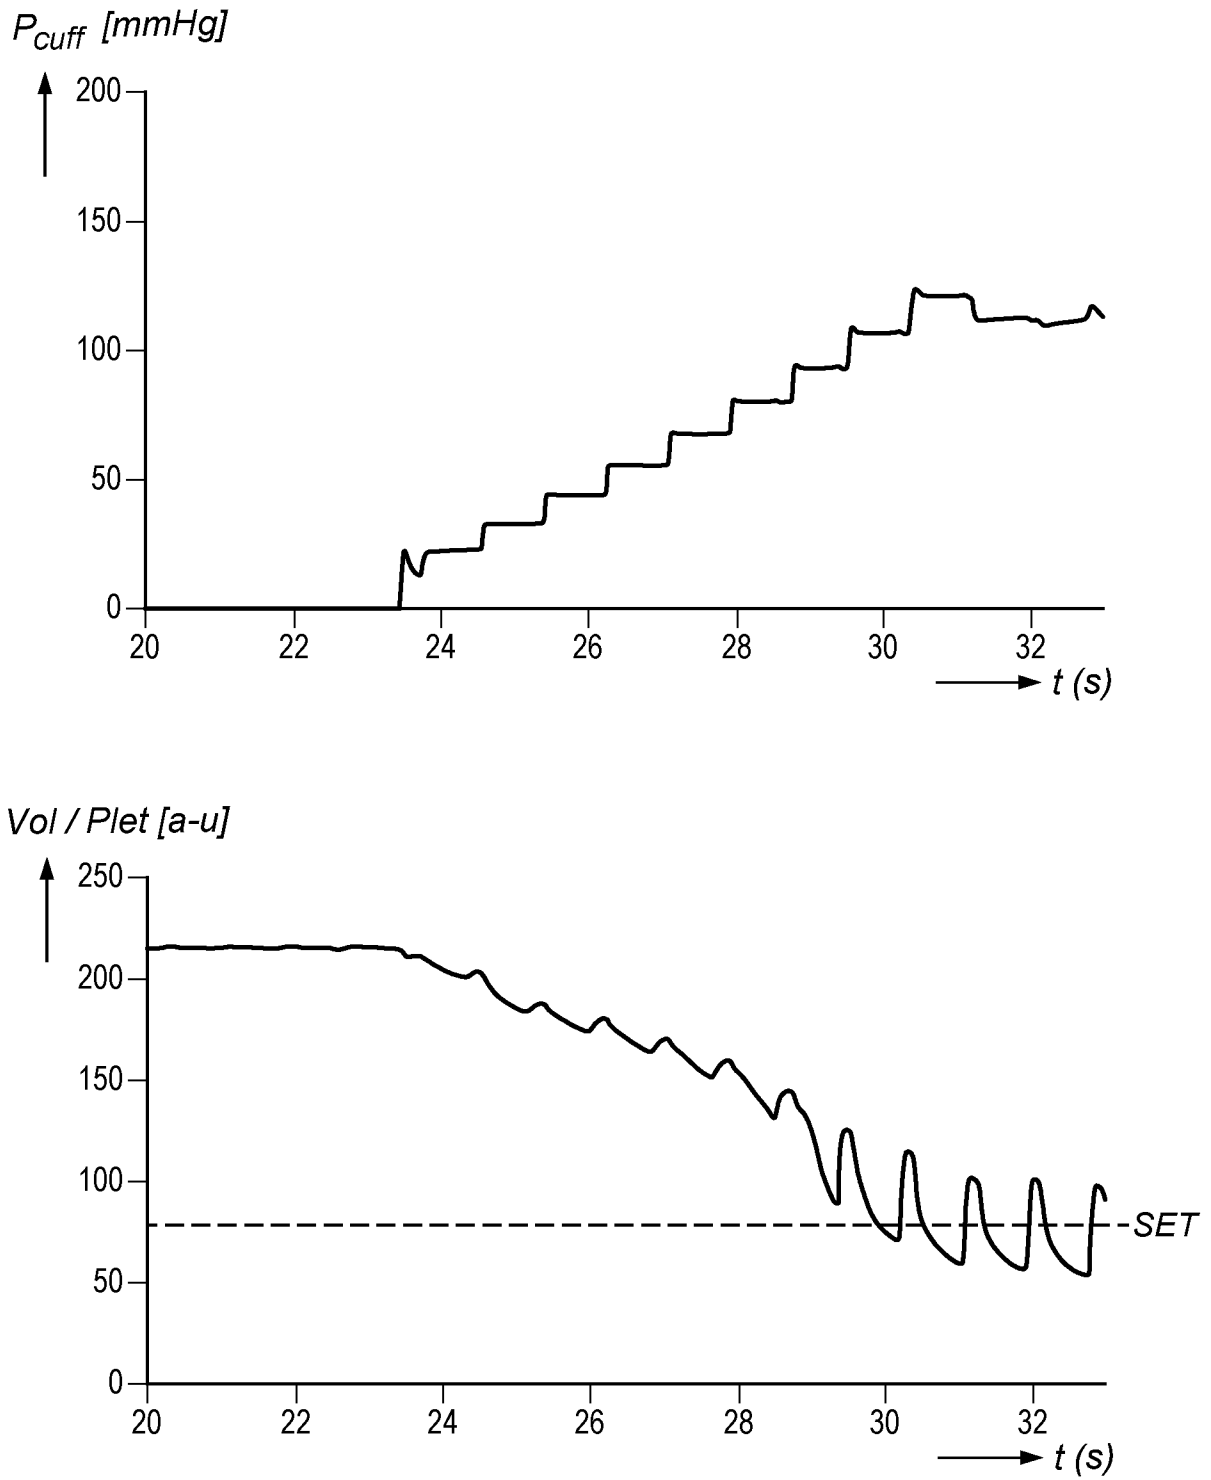


Fig. 2

3/12

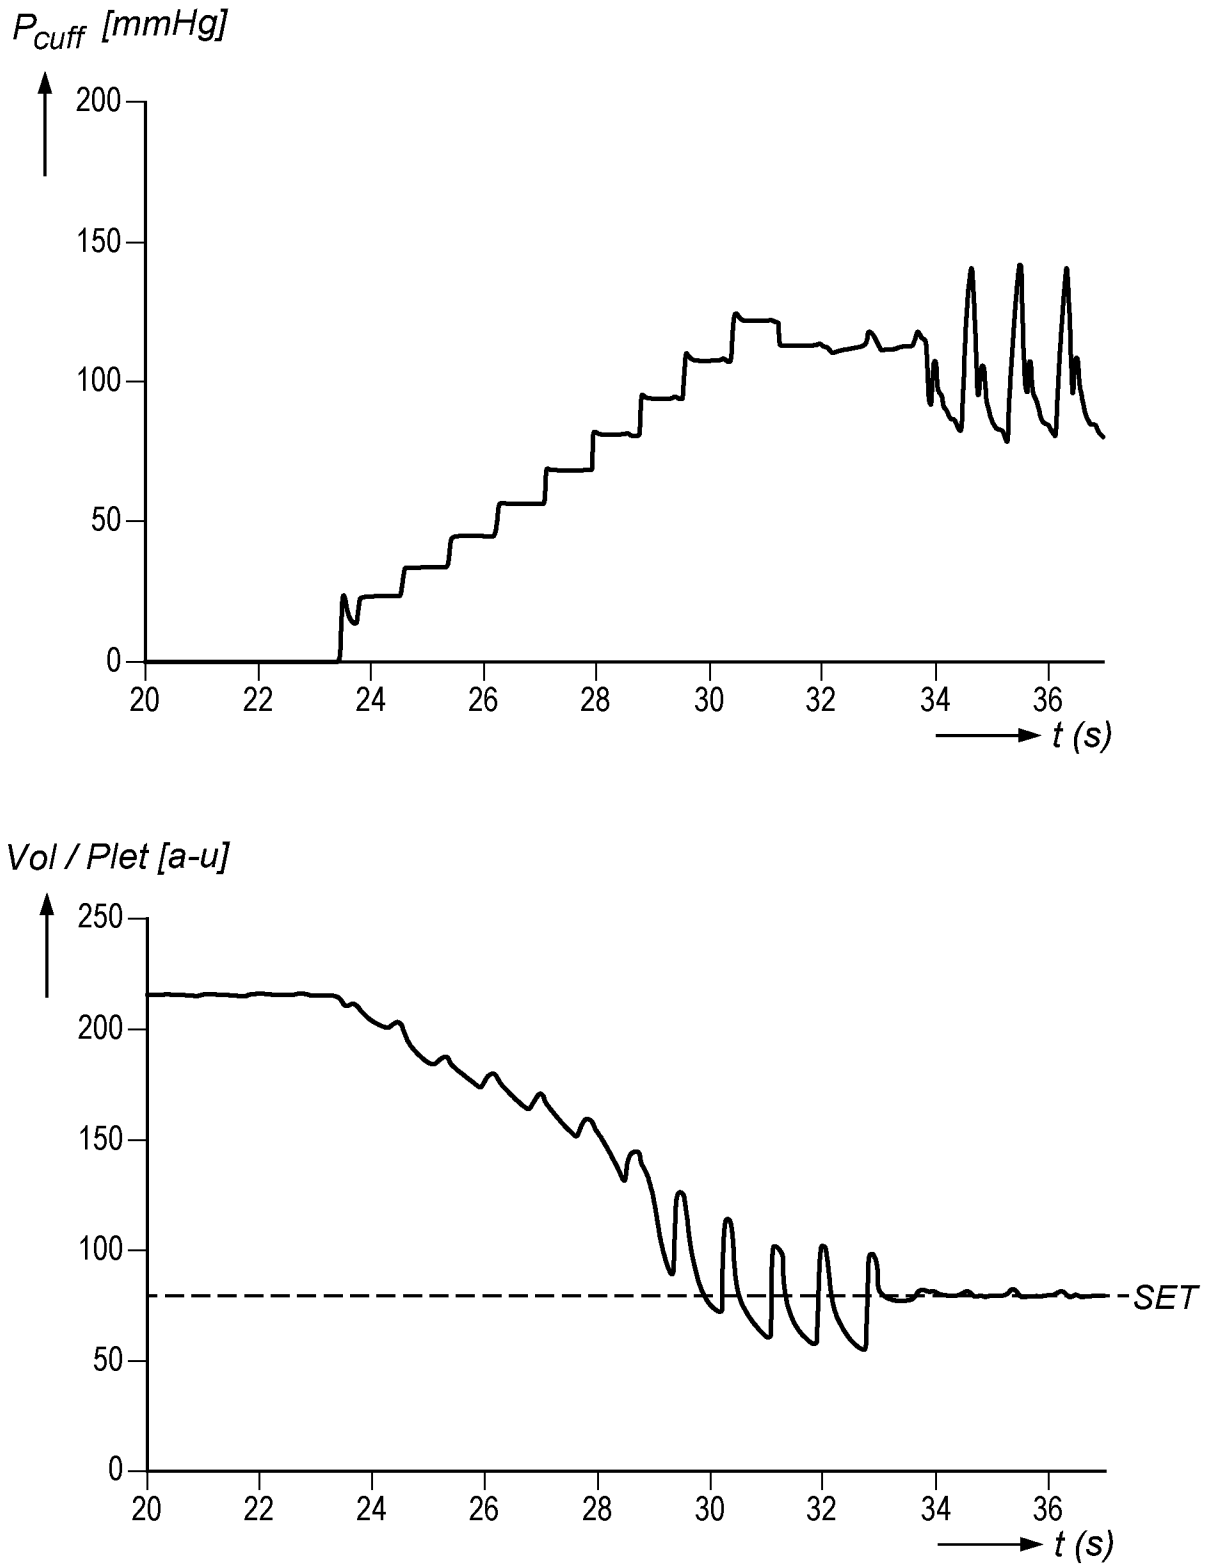


Fig. 3

4/12

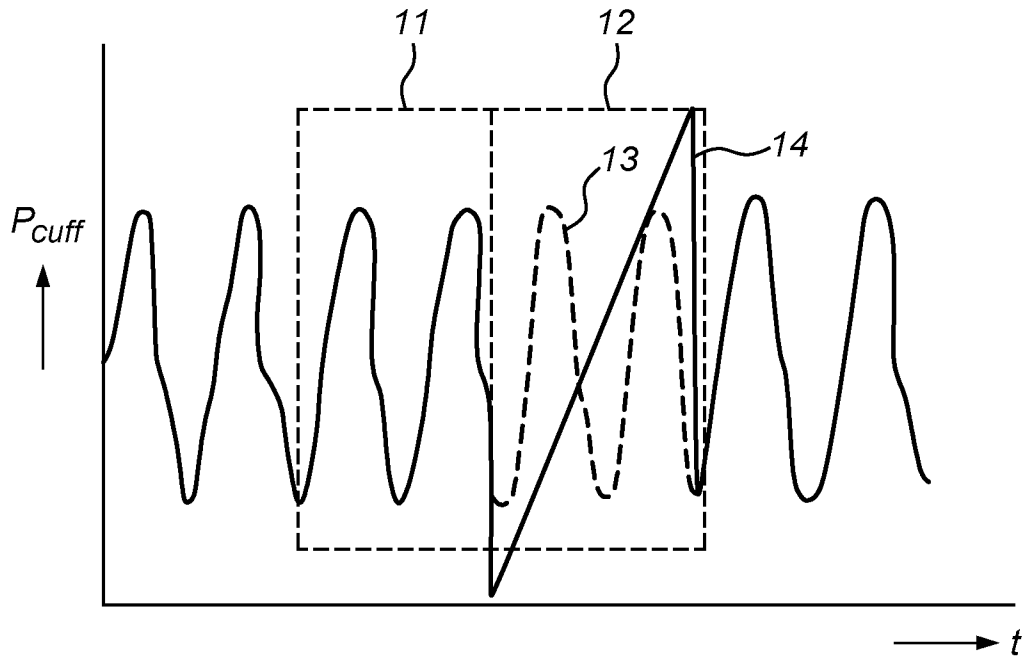


Fig. 4A

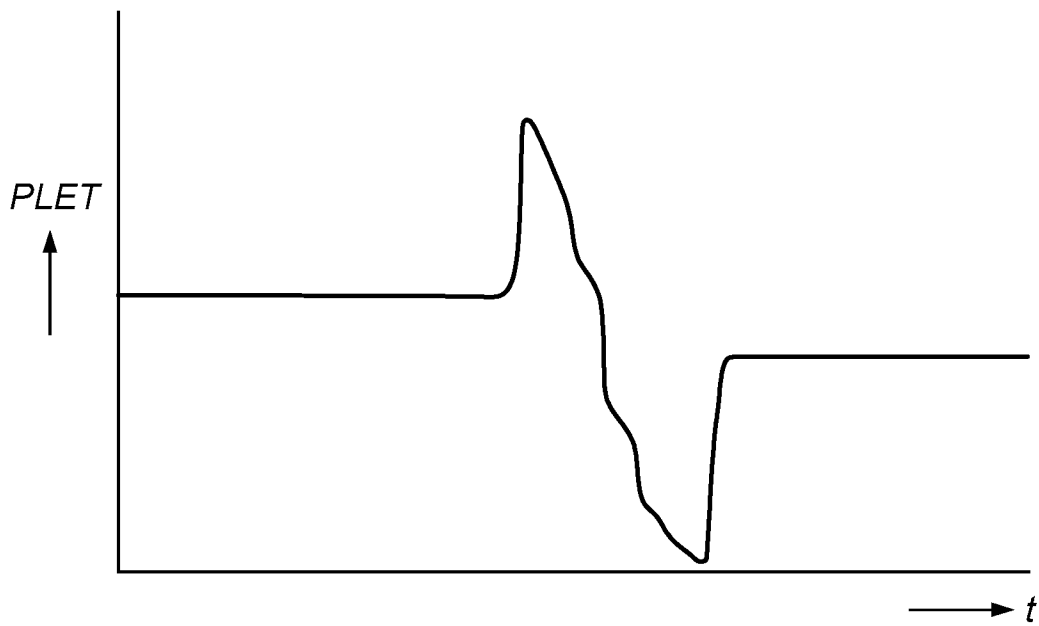


Fig. 4B

5/12

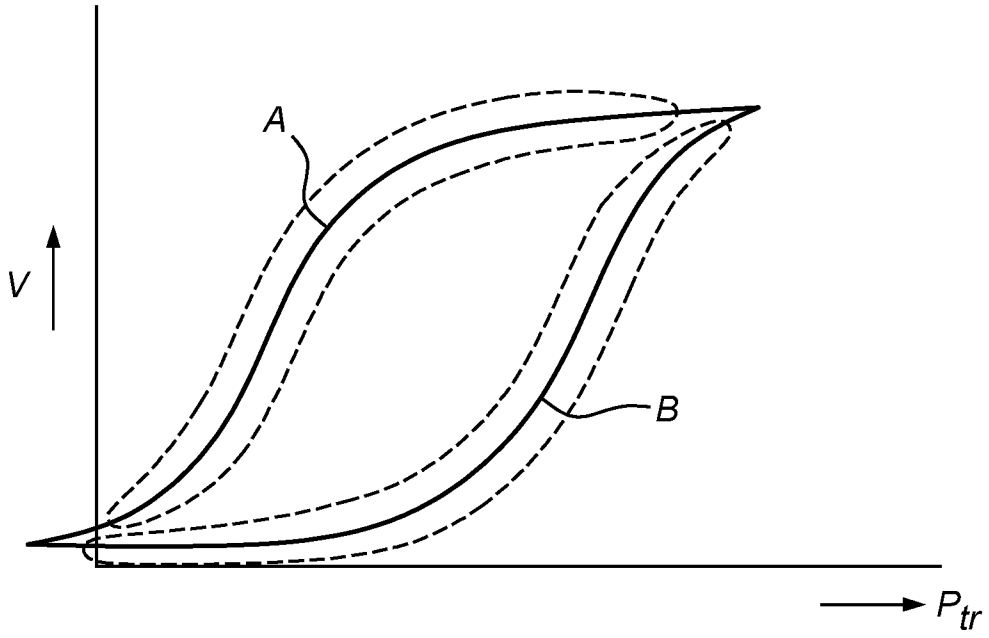


Fig. 4C

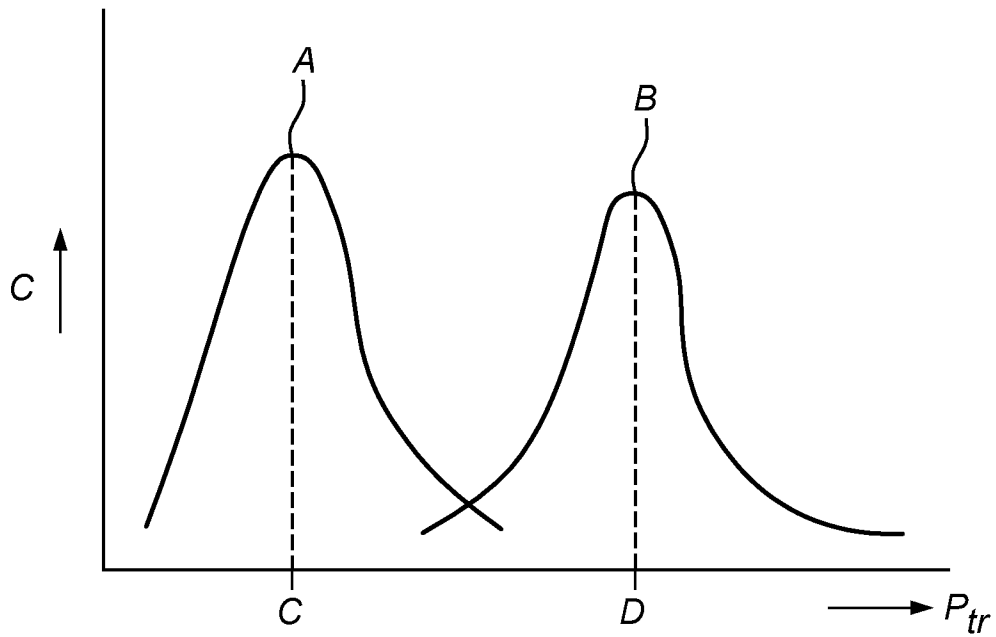


Fig. 4D

6/12

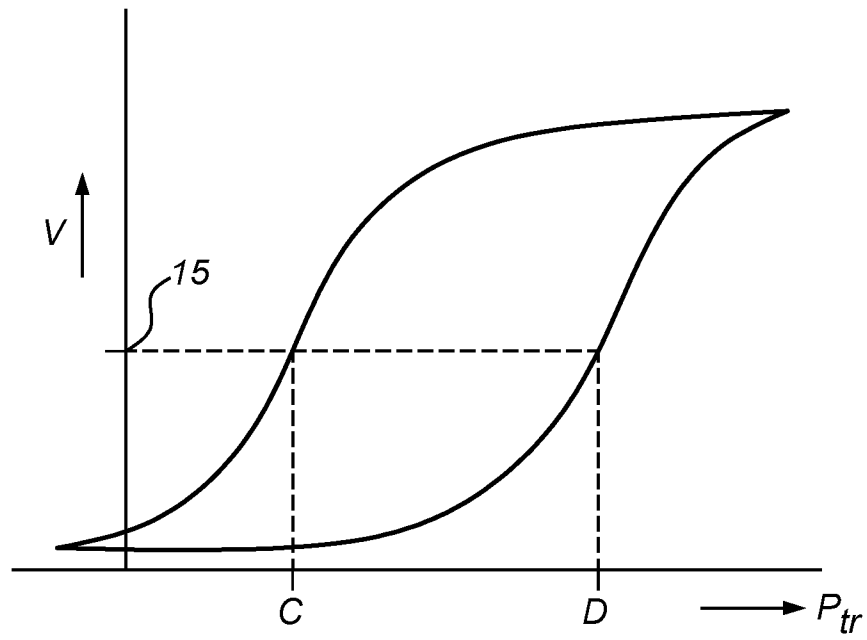


Fig. 4E

7/12

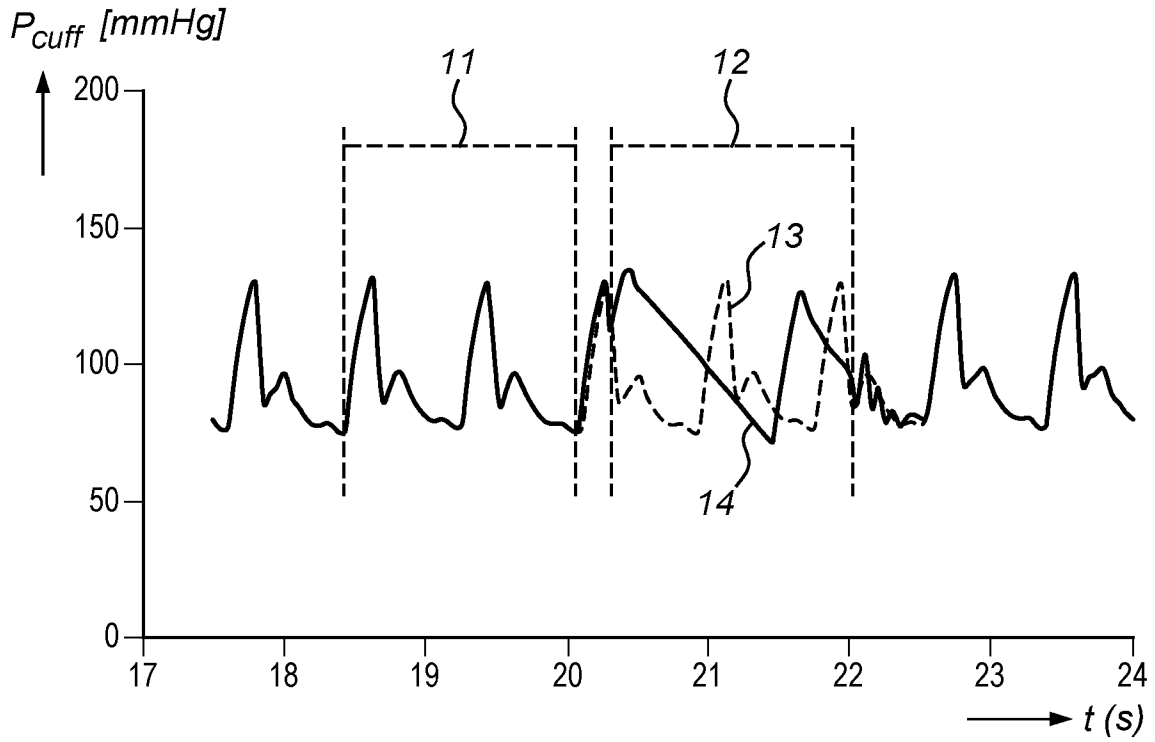


Fig. 5A

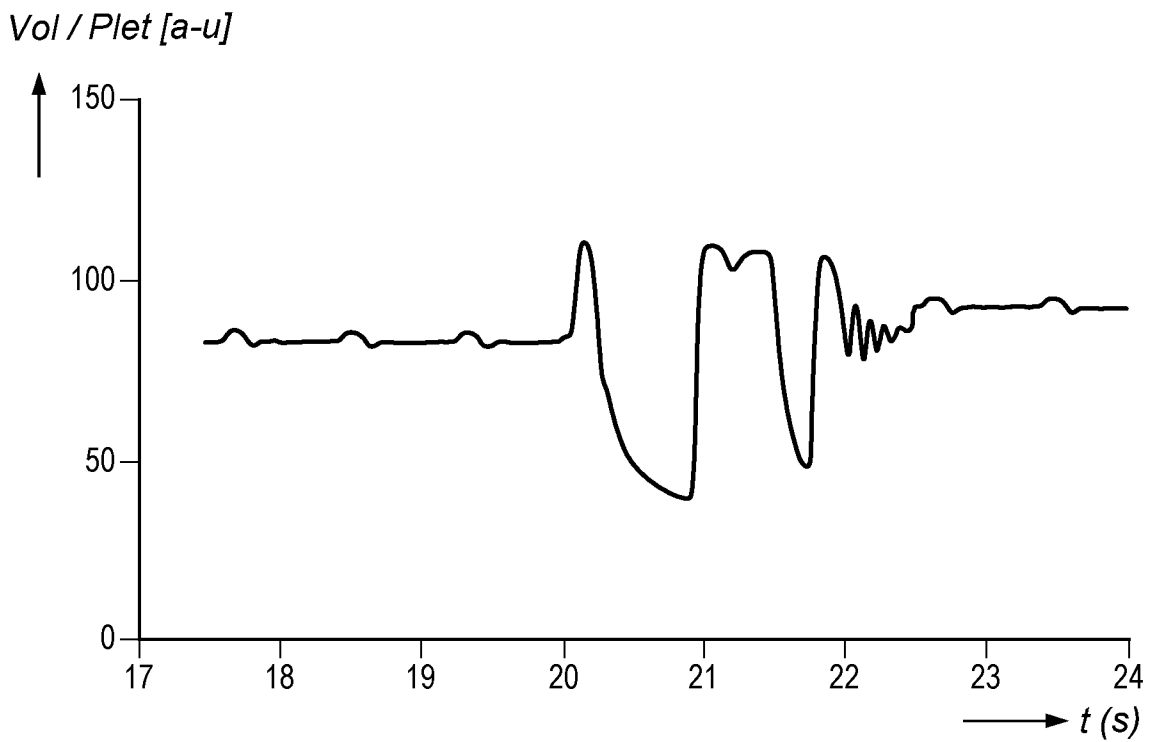


Fig. 5B

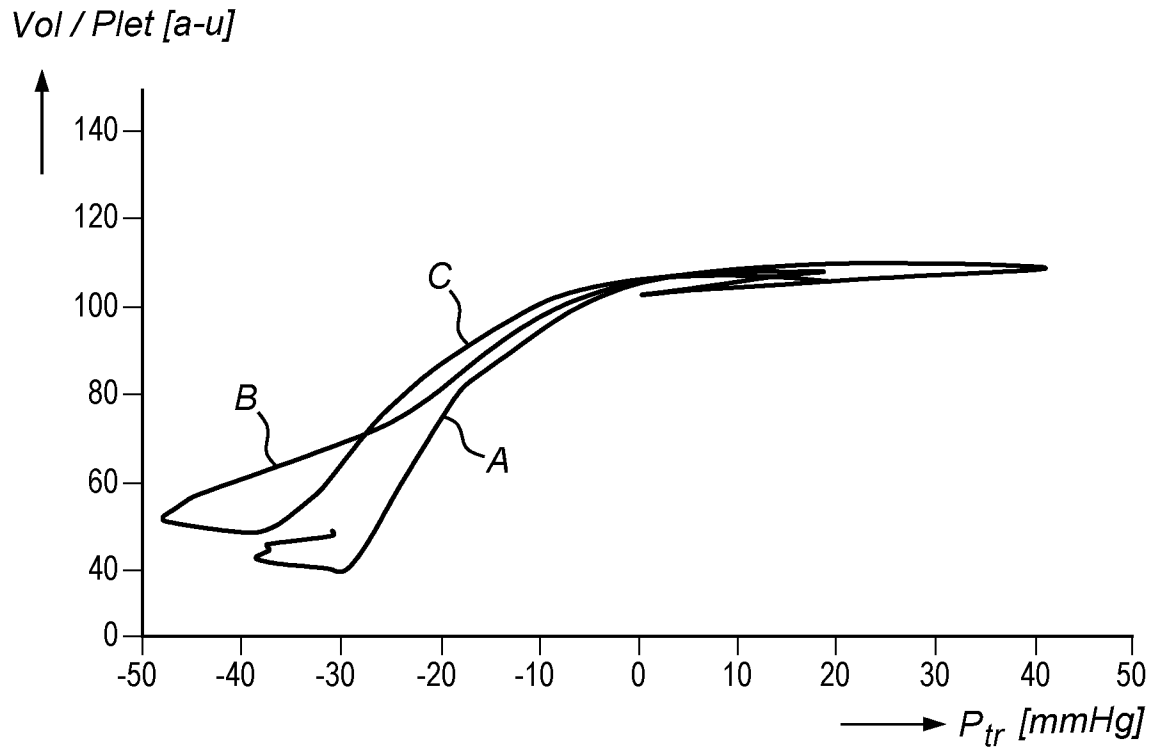


Fig. 5C

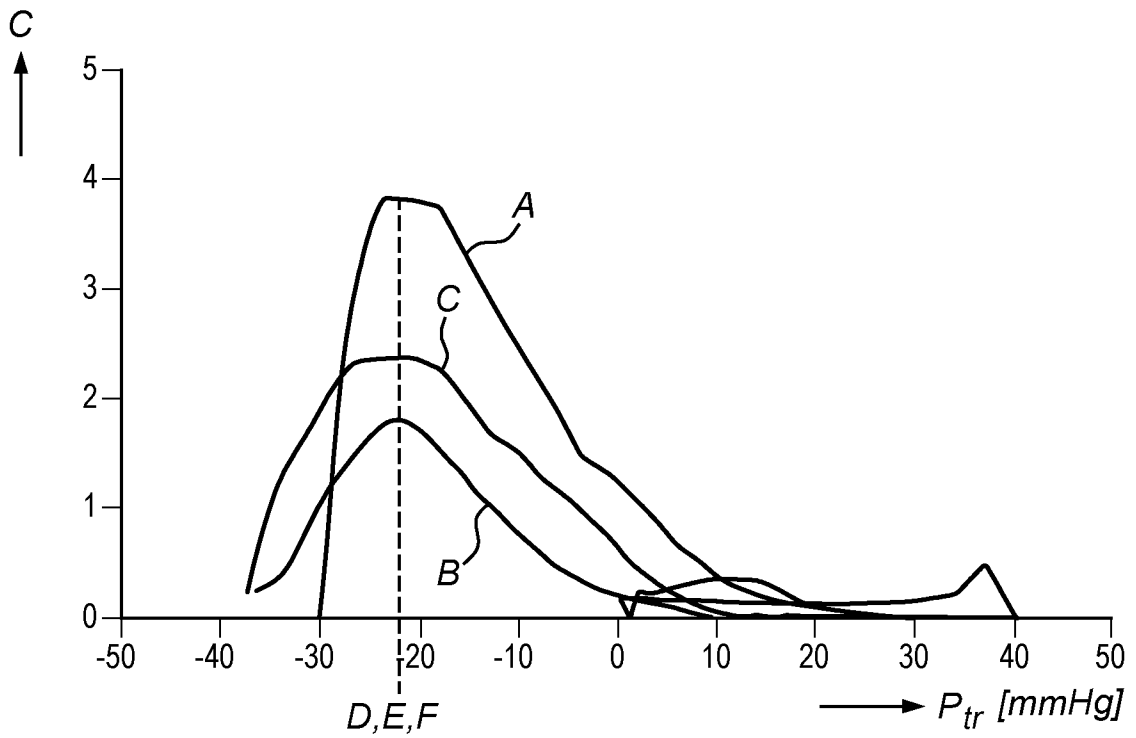


Fig. 5D

9/12

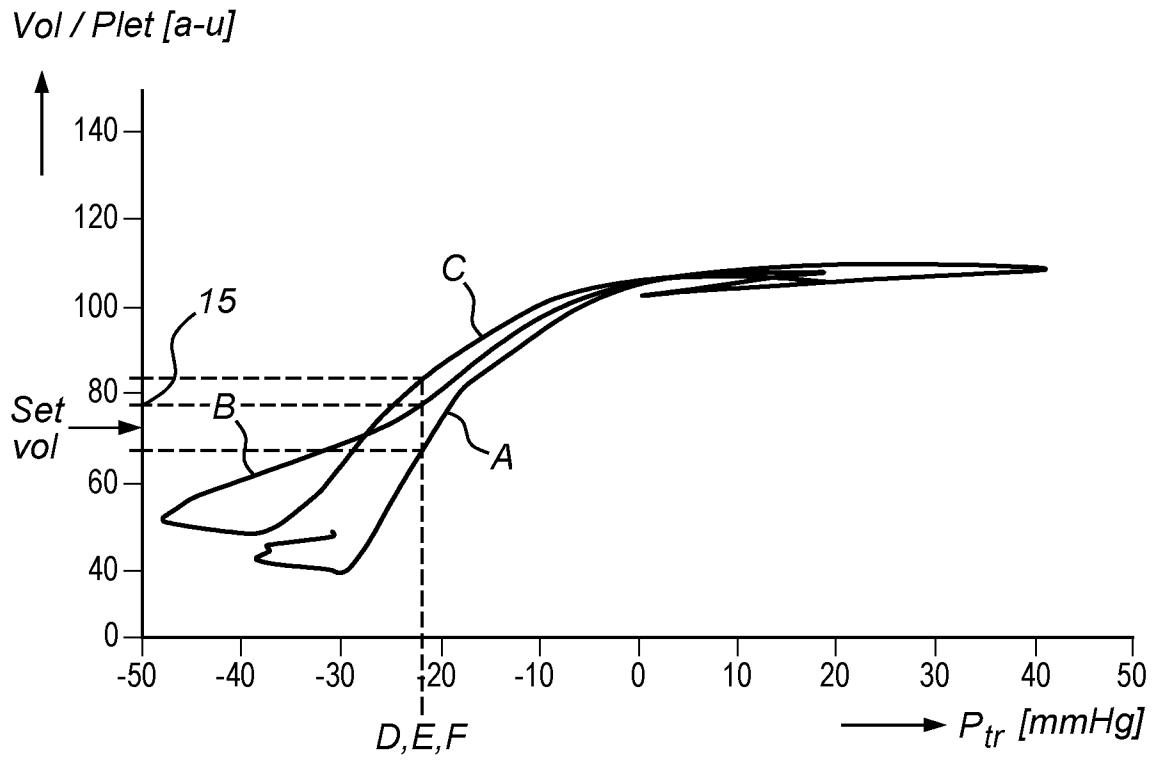


Fig. 5E

10/12

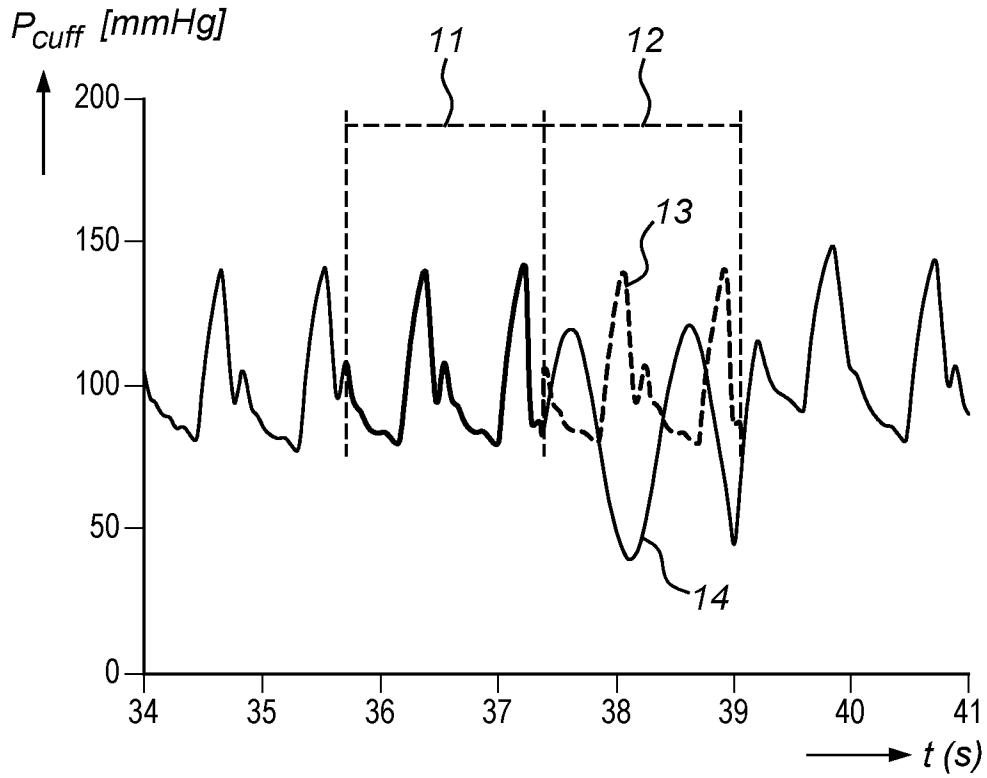


Fig. 6A

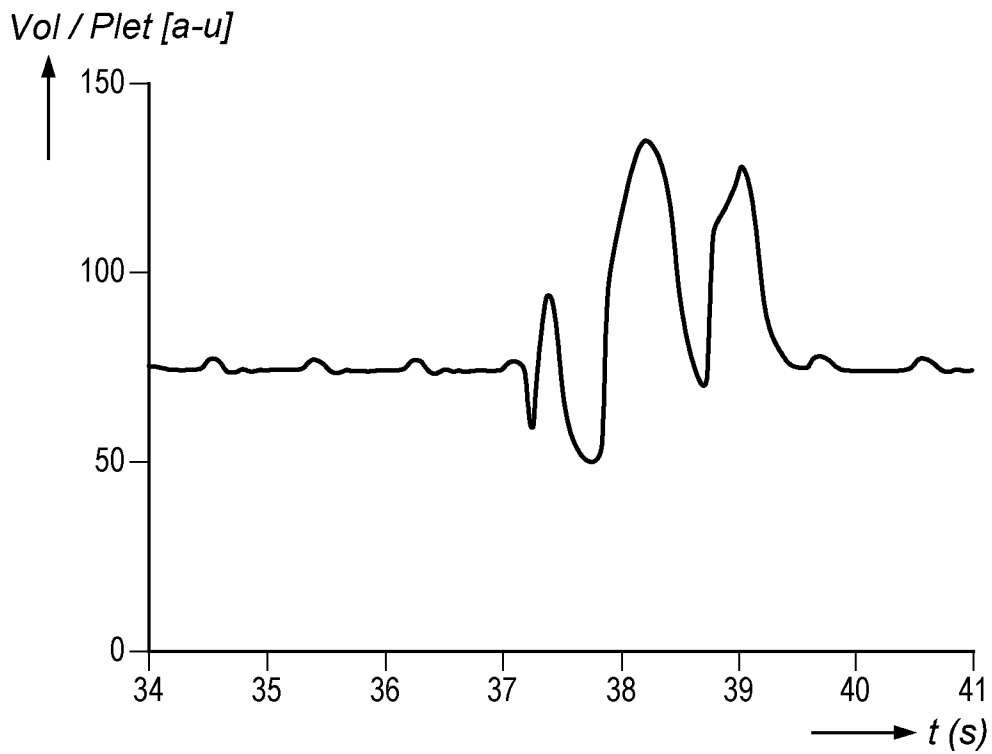


Fig. 6B

11/12

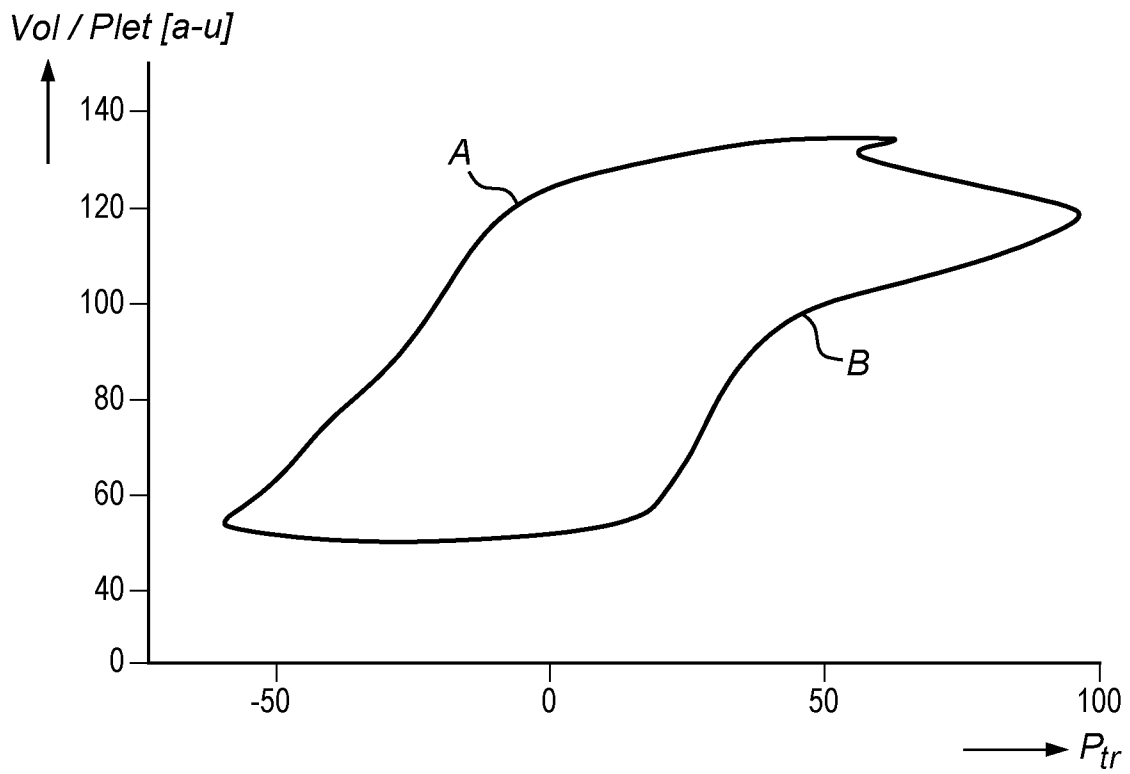


Fig. 6C

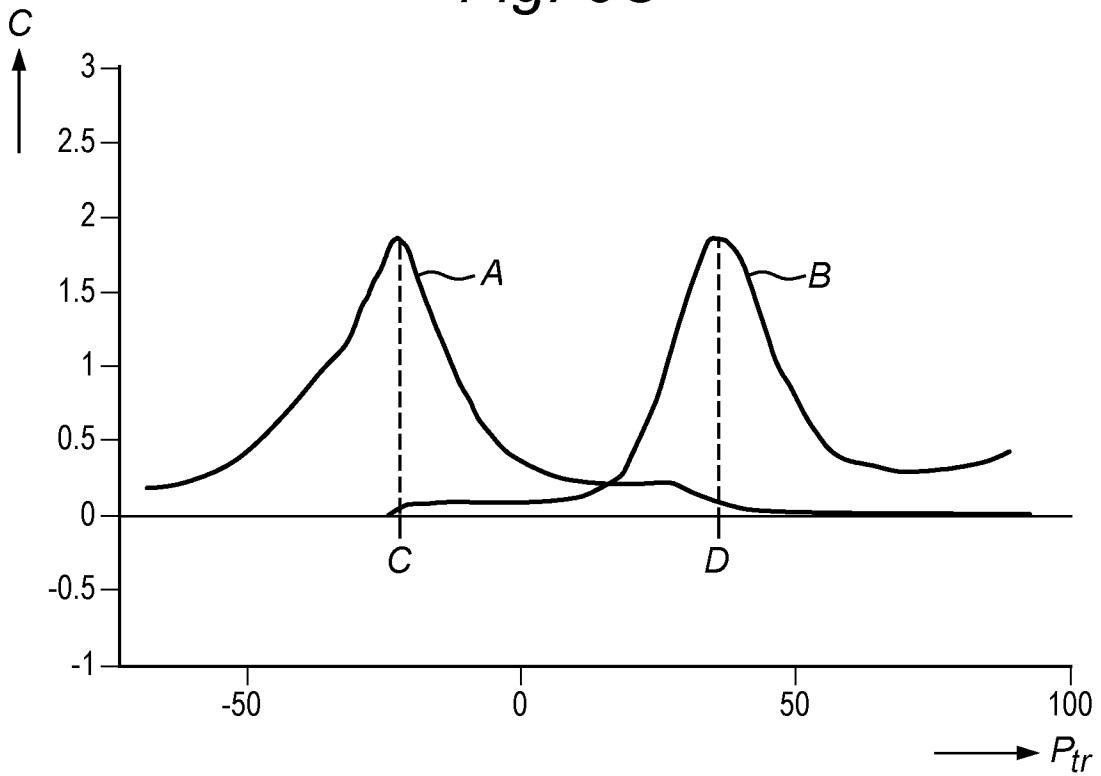


Fig. 6D

12/12

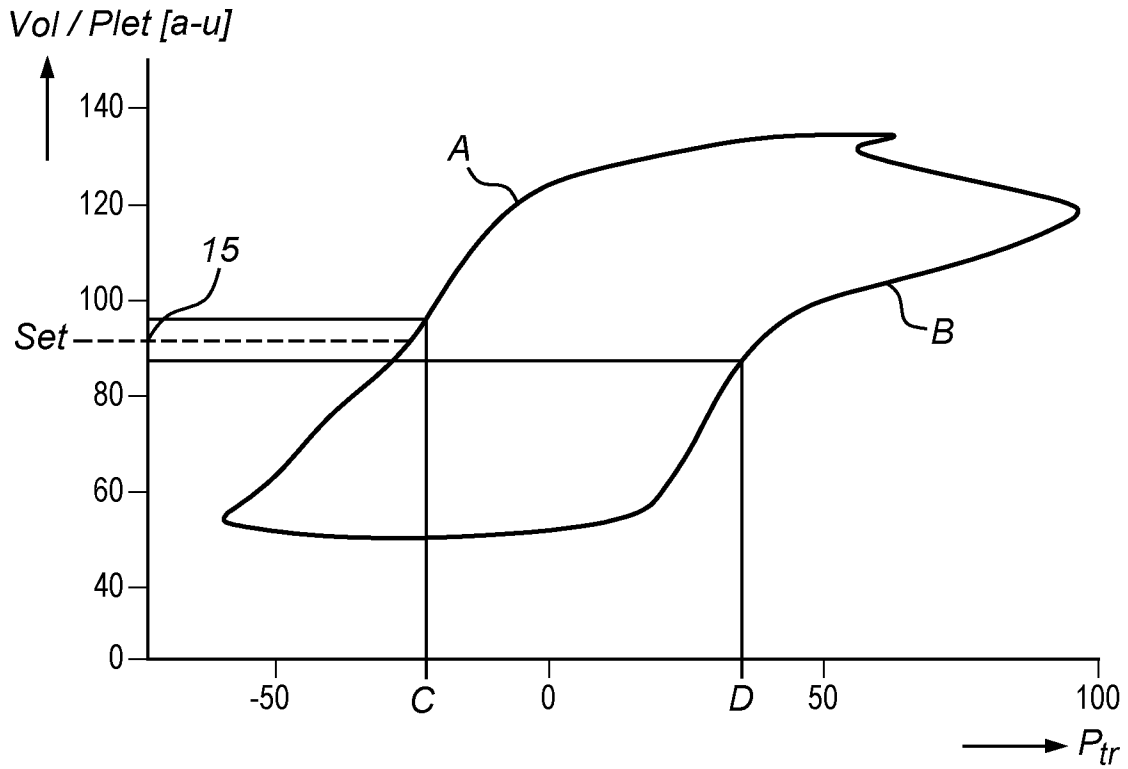


Fig. 6E

A. CLASSIFICATION OF SUBJECT MATTER**A61B 5/022(2006.01)i, A61B 5/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHEDMinimum documentation searched (classification system followed by classification symbols)
A61B 5/022; A61B 5/02; A61B 5/025; A61B 5/0225; A61B 5/00Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
Korean utility models and applications for utility models
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)
eKOMPASS(KIPO internal) & Keywords: cuff, pressure, correct, plethysmograph, heartbeat**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2013-0023777 A1 (OMRON HEALTHCARE CO., LTD.) 24 January 2013 See paragraphs [48]-[91], claims 1,2,7 and figures 2,8.	1-10,15
Y	US 2016-0100805 A1 (KONINKLIJKE PHILIPS N.V.) 14 April 2016 See paragraph [115], claim 1 and figures 2-9.	1-10,15
A	US 2011-0105918 A1 (FORTIN et al.) 05 May 2011 See the whole document.	1-10,15
A	WO 96-003914 A1 (VASOCOR, INC.) 15 February 1996 See the whole document.	1-10,15
A	US 2002-0099298 A1 (YOKOZEKI) 25 July 2002 See the whole document.	1-10,15

 Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

05 September 2018 (05.09.2018)

Date of mailing of the international search report

05 September 2018 (05.09.2018)

Name and mailing address of the ISA/KR


International Application Division
Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea

Facsimile No. +82-42-481-8578

Authorized officer

Kim, Yeonkyung

Telephone No. +82-42-481-3325



Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. Claims Nos.: 11-14,16,17
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3. As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2018/034078

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2013-0023777 A1	24/01/2013	CN 102811660 A	05/12/2012
		CN 102811660 B	03/12/2014
		DE 112011101044 T5	17/01/2013
		JP 2011-200405 A	13/10/2011
		JP 5418352 B2	19/02/2014
		US 9332912 B2	10/05/2016
		WO 2011-118269 A1	29/09/2011
		US 2016-0100805 A1	14/04/2016
EP 3203899 A1	16/08/2017		
JP 2017-529948 A	12/10/2017		
MX 2017004413 A	26/06/2017		
US 2017-0303795 A1	26/10/2017		
WO 2016-055356 A1	14/04/2016		
US 2011-0105918 A1	05/05/2011		
		CN 102647940 B	04/02/2015
		CN 102791192 A	21/11/2012
		CN 102791192 B	25/02/2015
		EP 2493370 A1	05/09/2012
		EP 2493370 B1	16/03/2016
		EP 2493373 A1	05/09/2012
		EP 2493373 B1	16/03/2016
		JP 2013-509225 A	14/03/2013
		JP 2013-509226 A	14/03/2013
		JP 2016-025935 A	12/02/2016
		JP 6058397 B2	11/01/2017
		US 2011-0105917 A1	05/05/2011
		US 8343062 B2	01/01/2013
		US 8814800 B2	26/08/2014
		WO 2011-051819 A1	05/05/2011
WO 2011-051822 A1	05/05/2011		
WO 96-003914 A1	15/02/1996	AU 3208295 A	04/03/1996
		AU 3236195 A	04/03/1996
		US 5566677 A	22/10/1996
		US 5630424 A	20/05/1997
		US 5715828 A	10/02/1998
		US 5718232 A	17/02/1998
		WO 96-003915 A1	15/02/1996
		US 2002-0099298 A1	25/07/2002
EP 1224906 A3	26/02/2003		
JP 2002-209859 A	30/07/2002		
JP 3618297 B2	09/02/2005		
US 6582374 B2	24/06/2003		

专利名称(译)	在无创血液压力测量中校正小杯压力的程序		
公开(公告)号	EP3629909A1	公开(公告)日	2020-04-08
申请号	EP2018805101	申请日	2018-05-23
[标]申请(专利权)人(译)	爱德华兹生命科学公司		
申请(专利权)人(译)	爱德华生命科学公司		
当前申请(专利权)人(译)	爱德华生命科学公司		
[标]发明人	SETTELS JACOBUS JOZEF GERARDUS MARIA		
发明人	SETTELS, JACOBUS JOZEF, GERARDUS MARIA		
IPC分类号	A61B5/022 A61B5/00		
CPC分类号	A61B5/02241 A61B5/02255 A61B5/6826		
优先权	62/509877 2017-05-23 US 15/984634 2018-05-21 US		
其他公开文献	EP3629909A4		
外部链接	Espacenet		

摘要(译)

一种用体积描记器校正无创连续血压测量中的袖带压的方法，包括以下步骤：确定与预定动脉容积相对应的体积描记器信号的值，并将所确定的值设置为设定点；比较体积描记器测得的信号和设定点；监测一定程度的心跳时袖带压力的调节；在至少一个第一心跳期间存储袖带的压力调节；在至少一秒钟的心跳期间向压力袖带施加变化的袖带压力，并测量体积描记器的相应信号；使用存储的第一心跳的压力调整，第二心跳的袖带压力和体积描记器信号，确定压力-体积关系；基于所确定的关系，确定与预定动脉容积相对应的体积描记器信号的值；并将确定的值设置为新的设定点。