



(11) **EP 1 350 466 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
14.09.2011 Bulletin 2011/37

(51) Int Cl.:
A61B 5/11 (2006.01) A61B 5/08 (2006.01)
A61B 5/00 (2006.01)

(21) Application number: **01999317.9**

(86) International application number:
PCT/JP2001/010685

(22) Date of filing: **06.12.2001**

(87) International publication number:
WO 2002/045585 (13.06.2002 Gazette 2002/24)

(54) **MONITOR**

MONITOR

MONITEUR

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR**

(30) Priority: **07.12.2000 JP 2000372820**

(43) Date of publication of application:
08.10.2003 Bulletin 2003/41

(73) Proprietors:
• **Keio University**
Tokyo 108-8345 (JP)
• **SUMITOMO OSAKA CEMENT CO., LTD.**
Tokyo 102-8465 (JP)

(72) Inventors:
• **AOKI, Hirooki**
KEIO UNI.Faculty of Sc. andTech.
Yokohama-shi, Kanagawa 223-0061 (JP)
• **NAKAJIMA, Masato**
KEIO UNI.Fac. of Sc.and Tech.
Yokohama-shi, Kanagawa 223-0061 (JP)

• **TAKEMURA, Yasuhiro**
SUMITOMO OSAKA CEMENT CO., LTD.
Chiyoda-ku, Tokyo 102-8465 (JP)
• **MIMURA, Kazuhiro**
SUMITOMO OSAKA CEMENT CO., LTD.
Chiyoda-ku, Tokyo 102-8465 (JP)

(74) Representative: **Appelt, Christian W.**
Forrester & Boehmert
Pettenkofersstrasse 20-22
80336 München (DE)

(56) References cited:
WO-A-01/82785 WO-A-90/09560
WO-A-97/26824 DE-A1- 3 109 026
FR-A- 1 570 640 JP-A- 3 258 246
JP-A- 11 086 002 JP-A- 11 099 140
JP-A- 11 225 997 JP-A- 11 276 443
JP-A- 2000 189 389 JP-A- 2001 037 739
US-A- 3 796 208 US-A- 5 107 845
US-A- 6 062 216

EP 1 350 466 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Technical Field

5 **[0001]** The invention of this application relates to a monitor. More particularly, the present invention relates to a monitor capable of monitoring the body movement etc., of a sleeping person in a noncontact manner with image measurement.

Background Art

10 **[0002]** With the advent of an aging welfare society, the importance of home health monitoring for disease prevention and self care is expected to continue to grow, and various bioinstrumentation methods have been proposed. An aged but healthy normal person who can live an ordinary life can be mentioned as an example of a person to be the subject of such home health monitoring. However, under the present circumstances, such a person lacks the motivation to exercise health control and perform a troublesome device operation, because he/she does not need imminent health care. Therefore, a proposal has been made of various bioinstrumentation devices capable of measuring biomedical information under an unconscious condition without any device operation. As measurement methods employed in such bioinstrumentation devices, there are known a method of arranging temperature sensors in a bed or a bottom mattress and, from a temperature distribution, recording body movements at the time of getting into bed, at the time of rising from bed, and during sleep in bed, a method of deriving an electrocardiogram from an electrically conductive sheet and a pillow cover, and a method of measuring respiration and heart beat during sleep by use of a load sensor such as a highly accurate strain gauge or a load cell.

15 **[0003]** Recently, a proposal has been made to use such bioinstrumentation technology as a security device applied in the safety confirmation of an aged person besides the usage of health monitoring. For example, a leaving-bed sensor has been generally sold for detecting the leaving or falling out of bed of a person during sleep by measuring an electrostatic capacity etc. Additionally, an apnea detector is well known in which an apnea state, caused by an apnea syndrome by which breathing ceases during sleep, is detected by measuring respiration with a pressure-sensitive sensor, and a third party can be informed of the state (e.g., Japanese publication of unexamined patent application No. (hereinafter referred to as JP-A-) 2000-107154).

20 **[0004]** As a matter of course, respiration provides a very useful clue for immediately knowing the health condition of a person. Respiration measurement performed during sleep is expected to be useful not only in detecting an apnea syndrome but also in discovering a spasmodic incident caused by a sudden attack during sleep. As mentioned above, a typical respiration detecting method during sleep is a method of detecting respiration based on time base measured values of a load sensor or a pressure-sensitive sensor. Additionally, a method of using a vibration sensor, a radio-wave sensor, or air-pressure detection is publicly known (e.g., JP-A-H7-327939, JP-A-H11-28195, and JP-A-2000-83927). In these methods, since a measured signal is weak, a high-performance signal amplifier or some kind of signal processing is required to acquire and detect a stable signal, and, as a system, it becomes expensive and large in scale.

25 **[0005]** On the other hand, some proposals have been also made of a method of acquiring an image of a sleeping person by use of an image pickup device and detecting respiration based on the acquired image. With recent developments in electronic equipment, a high-performance image pickup device has appeared on the market at an extremely low price, and, since the device has noncontact properties, the method of detecting respiration based on an image has been brought to public attention as a technique having high practical usefulness.

30 **[0006]** For example, in "Image-processing device and patient-observing device" of JP-A-H11-86002 and "Region-of-interest setting device of respiration monitoring and respiration-monitoring system" of JP-A-H11-225997, the basic features of those inventions is to monitor respiration by examining a difference between images acquired in different time by the image pickup device.

35 **[0007]** The "image-processing device and patient-observing device" of JP-A-H11-86002 is composed of a TV camera, a respiration monitoring device, and a local-region automatic setting processing device. The local-region automatic setting processing device is composed of an edge detecting section that detects an edge included in a local region image set on an image for which a patient who requires care is photographed by the TV camera, a brightness distribution measuring section that measures the brightness distribution of each local partial region image divided by the edge in the local region image, and a determining section that sets a local region image to extract movement information by analyzing information about a detected edge and information about a measured brightness distribution. The local region image is divided into a plurality of local partial regions that are identical in brightness, and a time differentiation process is applied to each pixel included in each local partial region, and the total amount of the time differentiation is calculated. A time base change of this amount is analyzed, and a periodic appearance is detected as respiration, whereas irregularities in the period and amplitude are detected as great body movements, such as a body twist.

40 **[0008]** In the "Region-of-interest setting device of respiration monitoring and respiration-monitoring system" of JP-A-H11-225997, a calculation is first performed of the absolute value of a difference between every one frame of a plurality

of frame images picked up by a CCD camera over 1/2 periods of respiration. Thereafter, the difference images are integrated and stored, the positions and sizes of variation regions are then calculated from variation information that has been integrated and stored, and they are set as temporary regions in order from the largest to the smallest region in the variation ones. Thereafter, a judgment is made of whether a concentration-value histogram, that shows the distribution of the number of pixels of each concentration value, exhibits a two-peak characteristic having a height greater than a predetermined value in the temporary regions and whether the area value of the variation regions is greater than a given value. If this condition is satisfied, the temporary region is set as a region of interest (abbreviated as ROI). Further, a time differentiation process is performed in the set ROI, the absolute value of the difference between each pixel is then obtained, and a surface integral is applied. The surface integral is performed in a time series manner, and, like the invention of JP-A-H11-86002 a time base change in this surface integral is analyzed, and a periodic appearance is detected as respiration, whereas irregularities in the period and amplitude are detected as great body movements, such as a body twist.

[0009] Further, a method of detecting respiration by an optical flow of movement of a sleeping person is known as an image-using technique other than the aforementioned methods. The optical flow is characterized by detecting the movement of a sleeping person as a velocity vector, and a respiration waveform having a periodic rhythm and a body-movement waveform having a high peak can be obtained from a vector field by employing the fact that most upward vectors are detected in inspiration whereas most downward vectors are detected in expiration.

[0010] The respective methods described above are to observe the movement of shadows on a quilt by use of illumination light, and there remains the fundamental problem of being sometimes incapable of detecting the movement of shadows depending on lighting conditions, the posture of a sleeping person, or the design of the quilt. Additionally, since an image pickup device must be set close to the sleeping person in order to photograph the shadow on the quilt, the respiration monitoring according to the aforementioned methods is considered to entail a psychologically overpowered feeling when the person to be monitored goes to bed.

[0011] Additionally, it is said that the method based on a time differentiation can evaluate a frequency of the movement of a targeted person, but cannot make a quantitative evaluation of the movement thereof. In contrast, in the optical-flow method, the optical flow enables a quantitative evaluation of the movement of a sleeping person, but, in practice, much computation time is needed to calculate the optical flow, and there remains the problem of requiring expensive processing equipment.

[0012] US Patent 6,062,216 discloses an apnea monitor that projects a single lighting spot or speckle pattern at a sleep surface of a sleeping patient to detect a signal that varies with external motion of the patient's upper body.

[0013] In the international patent application WO 90/09560, an optical distance measuring gauge is described in which a first beam is shone through a first pair of rectangles, and a second beam is shone through a second pair of rectangles to form a pattern of two corresponding pairs of rectangles on the surface of the target. The distance between the gauge and the target is then calculated from the relative motion of the two pairs of rectangles on the surface of the target.

Disclosure of Invention

[0014] Therefore, the invention of this application has been made in consideration of the foregoing circumstances, and it is an object of the invention to provide a monitor capable of detecting respiration of a sleeping person without being affected by the posture of the sleeping person or the indoor illumination light and capable of easily evaluating detected respiration quantitatively through image measurement.

[0015] The invention is defined in claim 1. The monitor of the present invention comprises lighting pattern projecting means for projecting a specified lighting pattern, image pickup means for picking up light of projected wavelength continuously, moving amount calculating means for calculating an inter-frame moving amount of the lighting pattern from two frames of images acquired by the image pickup means at different times, moving amount waveform generating means for generating moving amount waveform data comprising inter-frame moving amounts arranged in time series, and waveform detecting means for detecting a movement of an object to be picked up from the moving amount waveform data.

[0016] The waveform detecting means is to detect the body movement and respiration of a sleeping person, and the monitor further comprises safety deciding means for deciding the safety of the sleeping person from the body movement and respiration of the sleeping person and signal outputting means for, when the safety deciding means decides that the sleeping person is in a dangerous state, outputting a signal indicating it.

[0017] The moving amount calculating means can easily calculate the moving amount of the lighting pattern by calculating the inter-frame moving amount of the lighting pattern in an axial direction connecting the lighting pattern projecting means and the image pickup means.

[0018] The waveform detecting means can detect a respiratory pattern and a body movement pattern by detecting a periodic pattern as the respiratory pattern and by detecting a variation having a high peak as the body movement pattern from moving-amount waveform data.

[0019] The safety deciding means can decide a dangerous state of a sleeping person by deciding that the sleeping person is in a dangerous state when a period of the respiratory pattern falls into disarray in a short time, when the period of the respiratory pattern suddenly changes, when the respiratory pattern continuously disappears, or when the body movement pattern frequently appears in a short time.

[0020] The moving amount calculating means can easily and reliably detect the movement of an object to be photographed by calculating an inter-frame moving amount of the lighting pattern in an axial direction connecting the lighting pattern projecting means and the image pickup means while providing a positive or negative sign in accordance with a moving direction.

[0021] The waveform detecting means can reliably detect a respiratory pattern by, from among respiratory patterns, detecting a value having a positive or negative sign corresponding to a movement in a direction from the lighting pattern projecting means to the image pickup means on an image and a value having a positive or negative sign corresponding to a movement in a direction from the image pickup means to the lighting pattern projecting means on the image as an expiratory pattern and as an inspiratory pattern, respectively, or vice versa.

[0022] The waveform detecting means can well adapt to processing in a computer by counting zero crosses where signs are reversed between an expiratory pattern and an inspiratory pattern to count respirations.

[0023] The waveform detecting means can further exactly calculate a respiration number per unit time or a respiration period by calculating the respiration number per unit time or the respiration period from the counted respirations.

[0024] The waveform detecting means can further easily and exactly calculate a respiration number per unit time or a respiration period by conducting a frequency analysis of moving-amount waveform data or sampling data obtained by sampling respiratory patterns, by calculating the most prominent frequency from a resulting frequency spectrum, and by calculating the respiration number per unit time or the respiration period from this frequency.

[0025] The waveform detecting means can further calculate the respiration number per unit time or the respiration period through digital signal processing by conducting a frequency analysis with discrete Fourier transform or discrete wavelet transform.

[0026] The safety deciding means can reliably decide that a sleeping person is in a dangerous state by deciding whether respiration belongs to normal respiration, Cheyne-Stokes respiration, central hyperventilation, ataxic respiration, or Kussmaul respiration from expiratory patterns and inspiratory patterns and by deciding that the sleeping person is in a dangerous state when the respiration belongs to any one of Cheyne-Stokes respiration, central hyperventilation, ataxic respiration, and Kussmaul respiration.

[0027] The moving amount calculating means calculates an inter-frame moving amount in a partial region of the lighting pattern in an axial direction connecting the lighting pattern projecting means and the image pickup means, and determines a region in an image where an inter-frame moving amount in the partial region appears much greater than a predetermined amount or where an inter-frame movement in the partial region appears frequently beyond a predetermined amount as a region where the sleeping person exists, and the safety deciding means can safely and reliably decide that the sleeping person is in a dangerous state by deciding that the sleeping person is in a dangerous state when the region where the sleeping person exists moves in a shorter time than a predetermined time and moves frequently beyond a predetermined amount.

[0028] The moving amount calculating means calculates an inter-frame moving amount in a partial region of the lighting pattern in an axial direction connecting the lighting pattern projecting means and the image pickup means, and determines a region in an image where an inter-frame moving amount in the partial region appears much greater than a predetermined amount or where an inter-frame movement in the partial region appears more frequently than a predetermined frequency as a region where the sleeping person exists, and the safety deciding means can reliably decide that the sleeping person is in a state of imminently falling from a bed by deciding that the sleeping person is in a dangerous state when the region where the sleeping person exists is brought closer to one end of the bed than a predetermined distance.

[0029] Additionally, it is possible to know that the sleeping person is in a dangerous state at a location remote therefrom by providing informing means for, based on a signal output from signal outputting means, informing a third party that the sleeping person is in a dangerous state.

[0030] The informing means can urge a third party to swiftly deal with the situation by informing the third party that the sleeping person is in a dangerous state by voice, characters, symbols, intensity of light including interior illumination light, or vibrations through a telecommunication line.

[0031] The lighting pattern projecting means projects a lighting pattern that has a plurality of lighting spots, and the moving amount calculating means calculates an inter-frame moving amount of each lighting spot in an axial direction connecting the lighting pattern projecting means and the image pickup means while providing a positive or negative sign in accordance with a moving direction, and calculates an inter-frame moving amount of the lighting pattern by use of a moving amount of one or more of the lighting spots, whereby the moving amount of the lighting pattern can be easily calculated.

[0032] The lighting pattern projecting means projects a lighting pattern that has a plurality of lighting spots, and the moving amount calculating means calculates an inter-frame moving amount of each lighting spot in an axial direction

connecting the lighting pattern projecting means and the image pickup means while providing a positive or negative sign in accordance with a moving direction, and calculates the total moving amount of each lighting spot as an inter-frame moving amount of the lighting pattern, whereby a statistical noise influence can be reduced.

5 [0033] The lighting pattern projecting means projects a lighting pattern that has a single slit ray or a plurality of slit rays, and the moving amount calculating means calculates an inter-frame moving amount of each lighting spot in an axial direction connecting the lighting pattern projecting means and the image pickup means while providing a positive or negative sign in accordance with a moving direction, and calculates an inter-frame moving amount of the lighting pattern by use of a moving amount of a pixel corresponding to the single or plural slit rays, whereby the moving amount of the lighting pattern can be easily calculated.

10 [0034] The lighting pattern projecting means projects a lighting pattern that has a single slit ray or a plurality of slit rays, and the moving amount calculating means calculates an inter-frame moving amount of each pixel corresponding to a slit ray in an axial direction connecting the lighting pattern projecting means and the image pickup means while providing a positive or negative sign in accordance with a moving direction, and calculates the total moving amount of each pixel corresponding to the slit ray as an inter-frame moving amount of the lighting pattern, whereby the number of measurement points can be increased, and a statistical noise influence can be reduced.

15 [0035] The lighting pattern projecting means is disposed directly above a part close to one end of an edge of bedding facing a head of or a foot of a person sleeping on the bedding, and the image pickup means is disposed directly above a part close to an opposite end thereof, whereby monitoring can be performed without allowing the sleeping person to have an intense consciousness of being monitored.

20 [0036] The provision of presence-in-bed detecting means for detecting the presence/absence of a sleeping person makes it possible to swiftly and accurately judge whether the sleeping person is absent or the sleeping person has stopped his/her breathing.

25 [0037] The provision of a pressure sensitive switch that can be placed under the sleeping person and can be used to detect the presence/absence of the sleeping person makes it possible to swiftly and accurately judge whether the sleeping person is absent or the sleeping person has stopped his/her breathing.

Brief Description of the Drawings

[0038]

30 Fig. 1 is a schematic diagram showing the structure of a monitor according to the invention of this application;
 Fig. 2 is a schematic diagram explaining the calculation of an inter-frame moving amount of a lighting pattern on an image in a moving amount calculating means;
 Fig. 3 is a schematic diagram showing the principle of the monitor according to the invention of this application;
 35 Fig. 4 shows an example of a waveform pattern of moving-amount waveform data;
 Fig. 5 is a schematic diagram showing the principle of the respiration detection of the monitor according to the invention of this application;
 Fig. 6(a), Fig. 6(b), Fig. 6(c), and Fig. 6(d) show examples of normal and abnormal respiratory patterns;
 Fig. 7 is a schematic diagram showing a lighting pattern projected by a lighting pattern projecting means;
 40 Fig. 8 is a schematic diagram showing a lighting pattern projected by the lighting pattern projecting means;
 Fig. 9 is a schematic diagram showing an arrangement of the lighting pattern projecting means and an image pickup means;
 Fig. 10 is a schematic diagram showing an arrangement of the lighting pattern projecting means and the image pickup means;
 45 Fig. 11 is a schematic diagram showing an arrangement of the lighting pattern projecting means and the image pickup means;
 Fig. 12 is a schematic diagram showing the structure of an indoor safety monitor that is the invention of this application;
 and
 Fig. 13 is a schematic diagram showing the structure of an indoor safety monitor that is the invention of this application.

Best Mode for Carrying Out the Invention

[0039] The invention of this application has the aforementioned features, and embodiments thereof will hereinafter be described.

55 [0040] Fig. 1 is a schematic diagram showing the structure of a monitor according to the invention of this application. The monitor 6 is composed of a lighting pattern projecting means 1, an image pickup means 5, a moving amount calculating means 7, a moving amount waveform generating means 8, a waveform detecting means 9, a safety deciding means 10, a signal outputting means 11, and an informing means 12. A lighting pattern 4 is first projected from the

lighting pattern projecting means 1 onto a body 2 of a sleeping person or onto bedding 3. It is preferable to set the wavelength of projected light to be infrared rays, so as to project without allowing the sleeping person to have consciousness of being monitored. The lighting pattern 4 projected to the body 2 or the bedding 3 is continuously picked up as an image by the image pickup means 5. The image pickup means 5 can pick up, for example, an infrared ray that is a wavelength of the projected light. In response to a movement in an optical axial direction of the image pickup means resulting from a movement of the body 2 or resulting from a movement of the bedding 3 responding to the movement of the body 2, a movement of a lighting pattern, whose optical axis is different from that of the image pickup means, in an pickup image plane occurs, and an inter-frame moving amount of this lighting pattern is calculated by the moving amount calculating means 7 from two frames of images different in time that have been acquired by the image pickup means 5.

[0041] Thereafter, in the moving amount waveform generating means 8, moving amount waveform data is generated by arranging the inter-frame moving amounts calculated by the moving amount calculating means 7 in time series. Further, in the waveform detecting means 9, the body movement and respiration of the sleeping person are detected from the moving amount waveform data. Even 2 or 3 frames/second of images to be acquired are enough to generate the waveform of respiration. Preferably, the images are acquired at regular intervals in order to generate the moving amount waveform data.

[0042] The monitor 6 of the invention of this application may be provided with the safety deciding means 10 by which the safety of a sleeping person is decided from the body movement and respiration of the sleeping person detected by the waveform detecting means 9. When it is decided that the sleeping person is in a dangerous state in the safety deciding means 10, the signal outputting means 11 outputs a signal indicating it. As a result, the dangerous state can be recorded, for example, together with its time. Further, based on the signal output by the signal outputting means 11, the informing means 12 automatically informs a third party the sleeping person is in a dangerous state.

[0043] Fig. 2 is a schematic diagram explaining the calculation of an inter-frame moving amount of a lighting pattern on an image in the moving amount calculating means. In the moving amount calculating means 7, an inter-frame moving amount of the lighting pattern in an axial direction connecting the lighting pattern projecting means 1 and the image pickup means 5 is calculated from two frames different in time among images acquired by the image pickup means 5.

[0044] Fig. 3 is a schematic diagram showing the principle of the monitor according to the invention of this application. In an optical arrangement shown in Fig. 3, the following equation is established.

$$\delta = dlz / \{ h (h - z) \}$$

where δ : inter-frame moving amount of a lighting pattern,

h: installation heights of the lighting pattern projecting means and the image pickup means,

d: distance between the lighting pattern projecting means and the image pickup means,

l: focal length of the image pickup means, and

Z: displacement amount in the height direction.

That is, the inter-frame moving amount δ of the lighting pattern corresponds to a displacement amount Z in the height direction resulting from a movement of the body 2 of a sleeping person or resulting from a movement of bedding 3 in response to the movement of the body 2. Therefore, in the waveform detecting means 9, a waveform showing a periodic pattern can be detected as a respiratory pattern, and a waveform showing a variation having a high peak can be detected as a body movement pattern (i.e., pattern in which the waveform is varied by a body movement, such as turning over in bed) separately from each other in the moving amount waveform data generated by the moving amount waveform generating means 8. In the respiratory pattern, a respiration number per unit time can be known from its periodicity. Further, the time transition of the periodicity shows the stability of the respiration of the sleeping person. Further, since the inter-frame moving amount of the lighting pattern corresponds to a displacement amount in the height direction as mentioned above, it serves also as a means for knowing the depth of the respiration.

[0045] A predominant frequency component can be calculated by conducting a frequency analysis of moving amount waveform data or respiratory pattern with discrete Fourier transform or discrete wavelet transform, and a respiration number per unit time can also be calculated from the value of this frequency. Fast Fourier transform can be mentioned as a typical example of discrete Fourier transform. For example, on the assumption that the most prominent sample in a result obtained by applying fast Fourier transform to the respiratory pattern is the M-th sample in sampling data in which N samples of respiratory patterns have been sampled at sampling intervals of Δt second, the most prominent frequency f can be obtained by $M/(\Delta t \times N)$, and a respiration number per minute can be obtained by $60xf$. A respiration period can be obtained by $1 \div f$. As a matter of course, various frequency analysis techniques other than fast Fourier transform can be applied in the invention of this application.

[0046] In the safety deciding means 10, for example,

- (i) when the period of a respiratory pattern falls into disarray in a short time,
- (ii) when the period of a respiratory pattern suddenly changes,
- (iii) when a respiratory pattern continuously disappears, and
- (iv) when a body movement pattern frequently appears in a short time,

5 it is decided that a sleeping person is in a dangerous state. The condition of (i) or (ii) is considered to be caused by an infirmity of the lungs, such as spontaneous pneumothorax or bronchial asthma, a cardiopathy, such as congestive heart failure, or a cerebrovascular disease, such as cerebral hemorrhage. The condition of (iii) appears when respiration stops. A possible condition of (iv) is the fact that the sleeping person suffers from some reason and is in distress.

10 **[0047]** In the moving amount calculating means 7, preferably, an inter-frame moving amount of a lighting pattern in an axial direction connecting the lighting pattern projecting means 1 and the image pickup means 5 is calculated from two frames of images different in time while applying a positive or negative sign in accordance with a moving direction. Hereby, concerning the respiration, an expiratory pattern and an inspiratory pattern shown in Fig. 4 are always obtained, and the respiration can be counted by measuring the number of "zero crosses" (intersections where the sign is reversed) appearing from the expiratory pattern to the inspiratory pattern or from the inspiratory pattern to the expiratory pattern. This is advantageous when processing is performed by a computer.

15 **[0048]** Fig. 4 shows an example of a waveform pattern of moving-amount waveform data. The moving amount waveform data generated by the moving amount waveform generating means 8 shows a waveform pattern, for example, shown in Fig. 4.

20 **[0049]** Fig. 5 is a schematic diagram showing the principle of the respiration detection of the monitor according to the invention of this application. In an optical arrangement shown in Fig. 5, when the height changes upward "A," a lighting pattern on an image moves in a direction "A" from the image pickup means to the lighting pattern projecting means. In contrast, when the height changes downward "B," the lighting pattern on the image moves in a direction "B" from the lighting pattern projecting means to the image pickup means on the image.

25 **[0050]** Therefore, concerning the inter-frame moving amount of the lighting pattern, if movingamountwaveformdata is generated from the inter-frame moving amount calculated while having a positive or negative sign in accordance with the moving direction, and if a waveform showing a periodic pattern among the moving amount waveform data is detected as a respiratory pattern, a part 41 having a sign corresponding to a movement in the direction "A" can be detected as an expiratory pattern, whereas a part 42 having a sign corresponding to a movement in the direction "B" can be detected as an inspiratory pattern among the detected respiratory patterns.

30 **[0051]** Since the moving direction of a lighting pattern follows a horizontal or vertical direction in the picked-up image by setting the horizontal or vertical direction of a picked-up image to coincide with the axial direction connecting the lighting pattern projecting means and the image pickup means, the moving amount of the lighting pattern can be easily calculated.

35 **[0052]** Further, a respiration number per unit time (or respiration period) can be known by a time point where the part 41 having a sign corresponding to a movement in the direction "A" and the part 42 having a sign corresponding to a movement in the direction "B" each appear once as a single breath.

40 **[0053]** In the safety deciding means, a decision may be made as to whether the respiration of a sleeping person is a normal respiration by pre-storing each respiratory pattern concerning normal and abnormal respirations and comparing these with a respiratory pattern of the sleeping person.

45 **[0054]** Fig. 6(a), Fig. 6(b), Fig. 6(c), and Fig. 6(d) show examples of normal and abnormal respiratory patterns. A normal respiratory pattern to be registered is a periodic pattern shown in Fig. 6(a). On the other hand, a respiratory pattern, such as Cheyne-Stokes respiration, central hyperventilation, ataxic respiration, or Kussmaul respiration, that is considered to occur when a physiologically disorder arises in the body, is registered as an abnormal respiratory pattern. As an example, a respiratory pattern of Cheyne-Stokes respiration is shown in Fig. 6(b), a respiratory pattern of central hyperventilation is shown in Fig. 6(c), and a respiratory pattern of ataxic respiration is shown in Fig. 6(d). These respiratory patterns are obviously different in the waveform from the normal respiratory pattern, and a decision is made as to a respiratory pattern to which that of a sleeping person belongs on the basis of the fact that they are different in the frequency of respiration, the occurrence count thereof, and the depth thereof.

50 **[0055]** When it is decided that the respiration of the sleeping person belongs to a respiratory pattern that is considered to occur when physiologically disorders arise in the body, the safety deciding means decides that the sleeping person is carrying out abnormal respiration and is in a dangerous state. When the sleeping person displays abnormal respiration, the informing means may inform a third party about the name of the respiratory pattern of the sleeping person, the name of a disease considered to cause the respiration, the disease organ, the disease part, etc. Table 1 shows the disease name or disease part when the abnormal respiratory pattern occurs.

Table 1

Cheyne-Stokes respiration	Disorder under both-sides cerebral cortex and of diencephalon
Central hyperventilation	Disorder from lower midbrain to upper pons
Ataxic respiration	Disorder from lower pons to upper medulla oblongata
Kussmaul respiration	Diabetic coma or uremia

[0056] Fig. 7 and Fig. 8 are each a schematic diagram showing a lighting pattern projected by the lighting pattern projecting means. Preferably, a lighting pattern projected by the lighting pattern projecting means has a spatially discrete distribution. For example, a plurality of lighting spots 71 shown in Fig. 7, a single slit ray 81 shown in Fig. 8, or a plurality of slit rays 82 are selected and used.

[0057] In a lighting pattern having a plurality of lighting spots, an inter-frame moving amount of each lighting spot is calculated while adding a positive or negative sign in accordance with a moving direction, and the total moving amount of each lighting spot is calculated as an inter-frame moving amount of the lighting pattern. Likewise, in a lighting pattern having a single or a plurality of slit rays, an inter-frame moving amount of each pixel corresponding to the slit ray is calculated while adding a positive or negative sign in accordance with a moving direction, and the total moving amount of each pixel corresponding to the slit ray is calculated as an inter-frame moving amount of the lighting pattern. A statistical noise influence can be reduced by calculating the total inter-frame moving amount when spatially discrete lighting patterns are used.

[0058] In the moving amount calculating means, a region in an image where the inter-frame moving amount of a lighting pattern appears greatly or where an inter-frame movement of the lighting pattern appears frequently is determined as a region where the sleeping person exists. When this region frequently moves in a short time, the safety deciding means may decide that the sleeping person is in a dangerous state. This can be regarded as a condition where the sleeping person suffers from some reason and is in distress.

[0059] The safety deciding means may decide that the sleeping person is in a dangerous state when the region where the sleeping person exists is brought extremely close to one of the sides of a bed and when the sleeping person on the bed is being monitored. This can be regarded as a situation where the sleeping person is in a dangerous position as if to fall from the bed.

[0060] In the monitor of the invention of this application, preferably, a range where the lighting pattern is projected is set within a range covering positions that can be occupied by the belly, chest, back, and shoulders of the sleeping person. Likewise, preferably, a range of a region photographed by an image pickup device is set within a range covering positions that can be occupied by the belly, chest, back, and shoulders of the sleeping person.

[0061] Fig. 9 and Fig. 10 are each a schematic diagram showing an arrangement of the lighting pattern projecting means and the image pickup means. For example, as shown in Fig. 9, the lighting pattern projecting means 91 is disposed directly above a part close to the head 92 or the foot 93 of the sleeping person, and the image pickup means 94 is disposed directly above a part around the belly 95 of the sleeping person. At an edge 104 of bedding 101 placed under the sleeping person facing the head 92 or the foot 93 of the sleeping person as shown in Fig. 10, the lighting pattern projecting means 106 may be disposed directly above a part close to one end 105 of the edge 104, and the image pickup means 108 may be disposed directly above a part close to an opposite end 107 of the edge 104. The arrangement shown in Fig. 9 can capture the respiration of the sleeping person extremely sensitively, and has the advantage of being able to detect a detailed respiratory pattern. However, since the image pickup device comes into view of the sleeping person, there can be a case in which the arrangement is accompanied by a psychologically oppressive feeling. In contrast, an arrangement shown in Fig. 10 cannot specifically catch the respiration unlike the arrangement shown in Fig. 9, but this arrangement is considered to have a weaker psychologically oppressive feeling. Of course, the arrangement shown in Fig. 9 can be formed to sacrifice slightly the sensitivity of respiration as in Fig. 11, and an oppressive feeling may be reduced by disposing the lighting pattern projecting means 111 and the image pickup means 112 at one side end 113 of the bedding. These arrangements are to be appropriately selected depending on the situation.

[0062] Any type of lighting pattern projecting means can be used if the lighting pattern projecting means can project light spatially discretely. Use can be made of, for example, a fiber grating, a diffraction grating, a lens array, a formed image of a light source array or an aperture array, a device that collimates an outgoing beam of the light source array or the aperture array, etc.

[0063] In the monitor of the invention of this application, as an auxiliary means for accurately detecting whether a sleeping person is present or absent, a pressure sensitive switch may be disposed in the bedding placed under the sleeping person. The presence/absence of the sleeping person is determined by ON/OFF of this switch.

[0064] Further, in the monitor of the invention of this application, the informing means has a voice outputting function and informs a third party by voice that the sleeping person is in a dangerous state. It may inform the third party by

characters, symbols, intensity of light including interior illumination light, or vibrations. Further, the informing means may have a function to connect to a telecommunications line, such as a general telephone line, ISDN line, PHS line, or cellular telephone line, and may inform the third party by voices, characters, or symbols that the sleeping person is in a dangerous state.

5 [0065] Fig. 12 is a schematic diagram showing an arrangement of the lighting pattern projecting means and the image pickup means. The principle of the invention of this application is not applied limitedly to a monitor for a sleeping person, of course. For example, as a matter of course, the principle can be applied also to an indoor safety monitor that monitors the safety of a person in a room. The indoor safety monitor has the same structure as the monitor of the invention of this application, and is shown, for example, in Fig. 12.

10 [0066] First, a lighting pattern 123 is projected from a lighting pattern projecting means 121 to a body 122 of a person to be monitored. The lighting pattern 123 projected to the body 122 is continuously picked up as an image by an image pickup means 124, and, from two frames of images different in time acquired by the image pickup means 124, an inter-frame moving amount of the lighting pattern 123 resulting from a movement of the body 122 is calculated by the moving amount calculating means.

15 [0067] Thereafter, in the moving amount waveform generating means, moving amount waveform data is generated by arranging the inter-frame moving amounts calculated by the moving amount calculating means in time series. Further, in the waveform detecting means, a body movement and respiration of the person to be monitored are detected from the moving amount waveform data.

20 [0068] The indoor safety monitor is provided with a safety deciding means. From the body movement and respiration of the person detected by the waveform detecting means, the safety deciding means decides whether the person to be monitored is safe or not. When the safety deciding means decides that the person is in a dangerous state, the informing means automatically informs a third party the person to be monitored is in a dangerous state.

25 [0069] In the moving amount calculating means, an inter-frame moving amount of a lighting pattern on an image in an axial direction connecting the lighting pattern projecting means 121 and the image pickup means 124 is calculated from two frames different in time among images acquired by the image pickup means 124.

[0070] In the waveform detecting means, a waveform indicating a periodic pattern is detected as a respiratory pattern, whereas a waveform indicating a variation having a high peak is detected as a body movement pattern among the moving amount waveform data generated by the moving amount waveform generating means.

30 [0071] The safety deciding means decides that a time zone where a body-movement pattern of the person to be monitored disappears indicates a state where the person stops moving, and, in this time zone, the safety deciding means decides that the person is in a dangerous state when the period of the respiratory pattern falls into disarray in a short time, when the period of the respiratory pattern suddenly changes, or when the respiratory pattern continuously disappears.

35 [0072] The indoor safety monitor mentioned above works effectively especially when a monitoring region is limited. For example, this is extremely adaptable for monitoring a person having a bath as shown in Fig. 13. Likewise, this works effectively to monitor the safety of a person in a bathroom.

[0073] The present invention is not limited to the aforementioned embodiments.

40 [0074] It is permissible to project light that has been subjected to amplitude modulation and extract a modulating signal from a picked-up signal. Thereby, it is possible to reduce an influence by which general light, such as indoor illumination light, is changed into a noise.

[0075] If precision is sacrificed to some degree, the frame may be a field. Therefore, the frame set forth in the appended claims has a broad concept including a field.

Industrial Applicability

45 [0076] As described in detail in the foregoing description, according to the invention of this application, it is possible to provide a monitor by image measurement capable of reliably detecting the respiration of a sleeping person and easily making a quantitative evaluation of the detected respiration without being influenced by the posture of the sleeping person, illumination light, and design of a quilt.

50 [0077] The invention of this application is strongly expected to be put into practical use as a technique that can support the achievement of swift emergency treatment when a senior citizen or sick person falls into a crisis condition.

Claims

- 55 1. A monitor comprising:
 lighting pattern projecting means (1; 91; 106; 111; 121; 131) adapted to project a specified lighting pattern (4;

123; 133);

image pickup means (5; 94; 108; 112; 124; 134) adapted to pick up the projected lighting pattern(4; 123; 133) continuously as an image and to acquire the images as frames of images;

moving amount calculating means (7) for calculating an inter-frame moving amount of the lighting pattern (4; 123; 133) from two frames of images acquired by the image pickup means (5; 94; 108; 112; 124; 134) at different times;

moving amount waveform generating means (8) adapted to generate moving amount waveform data comprising inter-frame moving amounts arranged in time series, and

waveform detecting means (9) adapted to detect a movement of an object to be picked up from the moving amount waveform data;

characterized in that

the optical axis of the image pickup means (5; 94; 108; 112; 124; 134) differs from the optical axis of the lighting pattern projecting means (1; 91; 106; 111; 121; 131);

the lighting pattern (4; 123; 133) has a plurality of lighting spots (71) or slit rays (81; 82); and

the moving amount calculating means (7) are configured to calculate an inter-frame moving amount of each lighting spot (71) or an inter-frame moving amount of each pixel corresponding to a slit ray (81; 82), respectively, in an axial direction connecting the lighting pattern projecting means (1; 91; 106; 111; 121; 131) and the image pickup means (5; 94; 108; 112; 124; 134) while providing a positive or negative sign in accordance with a moving direction, and are further configured to calculate a total moving amount of each lighting spot (71) or a total moving amount of each pixel corresponding to the slit ray (81; 82), respectively, as an inter-frame moving amount of the lighting pattern (4; 123; 133).

2. The monitor as set forth in Claim 1, wherein the waveform detecting means (9) is adapted to detect a body movement and respiration of a sleeping person, the monitor further comprising:

safety deciding means (10) adapted to decide the safety of the sleeping person from the body movement and respiration of the sleeping person; and

signal outputting means (11) adapted to, when the safety deciding means (10) decides that the sleeping person is in a dangerous state, output a signal indicating it.

3. The monitor as set forth in Claim 2, wherein the waveform detecting means (9) is adapted to detect a periodic pattern as a respiratory pattern, and to detect a variation having a high peak as a body movement pattern from the moving amount waveform data.

4. The monitor as set forth in Claim 3, wherein the safety deciding means (10) is adapted to decide that the sleeping person is in a dangerous state when a period of the respiratory pattern falls into disarray in a short time, when the period of the respiratory pattern suddenly changes, when the respiratory pattern continuously disappears, or when the body movement pattern frequently appears in a short time.

5. The monitor as set forth in Claim 3 or 4, wherein from among respiratory patterns, the waveform detecting means (9) is adapted to detect a value having a positive or negative sign corresponding to a movement in a direction from the lighting pattern projecting means (1; 91; 106; 111; 121; 131) to the image pickup means (5; 94; 108; 112; 124; 134) on an image and a value having a positive or negative sign corresponding to a movement in a direction from the image pickup means (5; 94; 108; 112; 124; 134) to the lighting pattern projecting means (1; 91; 106; 111; 121; 131) on the image as an expiratory pattern and as an inspiratory pattern, respectively, or vice versa.

6. The monitor as set forth in Claim 5, wherein the waveform detecting means (9) is adapted to count zero crosses where signs are reversed between an expiratory pattern and an inspiratory pattern to count respirations.

7. The monitor as set forth in Claim 6, wherein the waveform detecting means (9) is adapted to calculate a respiration number per unit time or a respiration period from the counted respirations.

8. The monitor as set forth in Claims 1 or 5, wherein the waveform detecting means (9) is adapted to calculate a respiration number per unit time or a respiration period by conducting a frequency analysis of the moving-amount waveform data set forth in Claim 1 or the sampling data obtained by sampling respiratory patterns set forth in Claim 5, by calculating the most prominent frequency from a resulting frequency spectrum, and by calculating the respiration number per unit time or the respiration period from this frequency.

9. The monitor as set forth in Claim 8, wherein the waveform detecting means (9) is adapted to conduct a frequency analysis with discrete Fourier transform or discrete wavelet transform.
- 5 10. The monitor as set forth in any one of Claims 5 through 7, wherein the safety deciding means (10) is adapted to decide whether respiration belongs to normal respiration, Cheyne-Stokes respiration, central hyperventilation, ataxic respiration, or Kussmaul respiration from expiratory patterns and inspiratory patterns and to decide that the sleeping person is in a dangerous state when the respiration belongs to any one of Cheyne-Stokes respiration, central hyperventilation, ataxic respiration, and Kussmaul respiration.
- 10 11. The monitor as set forth in Claim 2, wherein the moving amount calculating means (7) is adapted to calculate an inter-frame moving amount in a partial region of the lighting pattern (4; 123; 133) in an axial direction connecting the lighting pattern projecting means (1; 91; 106; 111; 121; 131) and the image pickup means (5; 94; 108; 112; 124; 134), and to determine a region in an image where an inter-frame moving amount in the partial region appears much greater than a predetermined amount or where an inter-frame movement in the partial region appears frequently beyond a predetermined amount as a region where the sleeping person exists, and the safety deciding means (10) is adapted to decide that the sleeping person is in a dangerous state when the region where the sleeping person exists moves in a shorter time than a predetermined time and moves frequently beyond a predetermined amount.
- 15 12. The monitor as set forth in Claim 2, wherein the moving amount calculating means (7) is adapted to calculate an inter-frame moving amount in a partial region of the lighting pattern (4; 123; 133) in an axial direction connecting the lighting pattern projecting means (1; 91; 106; 111; 121; 131) and the image pickup means (5; 94; 108; 112; 124; 134), and determine a region in an image where an inter-frame moving amount in the partial region appears much greater than a predetermined amount or where an inter-frame movement in the partial region appears more frequently than a predetermined frequency as a region where the sleeping person exists, and the safety deciding means (10) is adapted to decide that the sleeping person is in a dangerous state when the region where the sleeping person exists is brought closer to one end of the bed than a predetermined distance.
- 20 25 13. The monitor as set forth in any one of Claims 2 through 12, comprising informing means (12) adapted to, based on a signal output from signal outputting means (11), inform a third party that the sleeping person is in a dangerous state.
- 30 14. The monitor as set forth in Claim 13, wherein the informing means (12) is adapted to inform the third party that the sleeping person is in a dangerous state by voices, characters, symbols, intensity of light including interior illumination light, or vibrations through a telecommunications line.
- 35 15. The monitor as set forth in any one of Claims 1 through 14, comprising presence-in-bed detecting means adapted to detect the presence/absence of a sleeping person.
- 40 16. The monitor as set forth in any one of Claims 1 through 15, comprising a pressure sensitive switch placeable under the sleeping person to detect the presence/absence of the sleeping person.

Patentansprüche

- 45 1. Monitor mit:
- Beleuchtungsmusterprojizierungsmitteln (1; 91; 106; 111; 121; 131), welche zum Projizieren eines vorbestimmten Beleuchtungsmusters (4; 123; 133) eingerichtet sind;
- 50 Bilderfassungsmitteln (5; 94; 108; 112; 124; 134), welche zum kontinuierlichen Erfassen des Beleuchtungsmusters (4; 123; 133) als ein Bild und zum Erfassen der Bilder als Einzelbilder eingerichtet sind;
- Bewegungsbetragberechnungsmitteln (7) zum Errechnen eines Bild-zu-Bild-Bewegungsbetrags des Beleuchtungsmusters (4; 123; 133) aus zwei mittels der Bilderfassungsmittel (5; 94; 108; 112; 124; 134) zu unterschiedlichen Zeitpunkten erfassten Einzelbildern;
- 55 Bewegungsbetragwellenformerzeugungsmitteln (8), welche zum Erzeugen von Bewegungsbetragwellenformdaten eingerichtet sind, welche in einer Zeitreihe angeordnete Bild-zu-Bild-Bewegungsbeträge umfassen; und Wellenformerfassungsmitteln (9), welche zum Erfassen einer Bewegung eines zu erfassenden Objektes aus den Bewegungsbetragwellenformdaten eingerichtet sind;
- dadurch gekennzeichnet, dass**

EP 1 350 466 B1

die optische Achse der Bilderfassungsmittel (5; 94; 108; 112; 124; 134) von der optischen Achse der Beleuchtungsmusterprojizierungsmittel (1; 91; 106; 111; 121; 131) verschieden ist; das Lichtmuster (4; 123; 133) mehrere Leuchtflecken (71) oder Schlitzstrahlen (81; 82) aufweist; und die Bewegungsbetragberechnungsmittel (7) dazu eingerichtet sind, einen Bild-zu-Bild-Bewegungsbetrag jedes Leuchtflecks (71) bzw. einen Bild-zu-Bild-Bewegungsbetrag jedes einem Schlitzstrahl (81; 82) entsprechenden Pixels in einer die Beleuchtungsmusterprojizierungsmittel (1; 91; 106; 111; 121; 131) und die Bilderfassungsmittel (5; 94; 108; 112; 124; 134) verbindenden Axialrichtung zu berechnen, während sie gemäß einer Bewegungsrichtung ein positives oder negatives Vorzeichen zuweisen, und ferner dazu eingerichtet sind, einen Gesamtbewegungsbetrag jedes Leuchtflecks (71) bzw. einen Gesamtbewegungsbetrag jedes dem Schlitzstrahl (81; 82) entsprechenden Pixels als einen Bild-zu-Bild-Bewegungsbetrag des Beleuchtungsmusters (4; 123; 133) zu berechnen.

2. Monitor nach Anspruch 1, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, eine Körperbewegung und Atmung einer schlafenden Person zu erfassen, wobei der Monitor ferner umfasst:

Sicherheitsbeurteilungsmittel (10), welche dazu eingerichtet sind, die Sicherheit der schlafenden Person aus der Körperbewegung und der Atmung der schlafenden Person zu beurteilen; und Signalausgabemittel (11), welche dazu eingerichtet sind, wenn die Sicherheitsbeurteilungsmittel (11) entscheiden, dass sich die schlafende Person in einem gefährlichen Zustand befindet, ein Signal auszugeben, welches dies anzeigt.

3. Monitor nach Anspruch 2, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, ein periodisches Muster als ein Atmungsmuster zu umfassen und eine Variation, welche einen hohen Scheitelpunkt aufweist, als ein Körperbewegungsmuster aus den Bewegungsbetragswellenformdaten zu erfassen.

4. Monitor nach Anspruch 3, bei welchem die Sicherheitsbeurteilungsmittel (10) dazu eingerichtet sind, zu entscheiden, dass sich die schlafende Person in einem gefährlichen Zustand befindet, wenn eine Periode des Atmungsmusters innerhalb einer kurzen Zeit in einen ungeordneten Zustand übergeht, wenn sich die Periode des Atmungsmusters plötzlich ändert, wenn das Atmungsmuster dauerhaft verschwindet oder wenn das Körperbewegungsmuster innerhalb einer kurzen Zeitspanne oft erscheint.

5. Monitor nach Anspruch 3 oder 4, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, unter den Atmungsmustern einen Wert zu erfassen, welcher entsprechend einer Bewegung in einer Richtung von den Beleuchtungsmusterprojizierungsmitteln (1; 91; 106; 111; 121; 131) zu den Bilderfassungsmitteln (5; 94; 108; 112; 124; 134) auf einem Bild ein positives oder negatives Vorzeichen aufweist sowie einen Wert zu erfassen, welcher entsprechend einer Bewegung in einer Richtung von den Bilderfassungsmitteln (5; 94; 108; 112; 124; 134) zu den Beleuchtungsmusterprojizierungsmitteln (1; 91; 106; 111; 121; 131) auf dem Bild ein positives oder negatives Vorzeichen aufweist, als ein Ausatmungsmuster bzw. als ein Einatmungsmuster, oder umgekehrt.

6. Monitor nach Anspruch 5, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, Nulldurchgänge zu zählen, bei welchen sich die Vorzeichen zwischen einem Ausatmungsmuster und einem Einatmungsmuster umkehren, um Atmungen zu zählen.

7. Monitor nach Anspruch 6, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, aus den gezählten Atmungen eine Atmungszahl pro Zeiteinheit oder eine Atmungsperiode zu errechnen.

8. Monitor nach Anspruch 1 oder 5, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, eine Atmungszahl pro Zeiteinheit oder eine Atmungsperiode zu berechnen, indem sie eine Frequenzanalyse der Bewegungsbetragswellenformdaten nach Anspruch 1 oder der durch Abtasten der Atmungsmuster nach Anspruch 5 gewonnenen Abtastdaten durchführen, aus dem sich ergebenden Frequenzspektrum die hervorstechendste Frequenz errechnen und aus dieser Frequenz die Atmungszahl pro Zeiteinheit oder die Atmungsperiode errechnen.

9. Monitor nach Anspruch 8, bei welchem die Wellenformerfassungsmittel (9) dazu eingerichtet sind, eine Frequenzanalyse mittels einer diskreten Fourier-Transformation oder einer diskreten Wavelet-Transformation auszuführen.

10. Monitor nach einem der Ansprüche 5 bis 7, bei welchem die Sicherheitsbeurteilungsmittel (10) dazu eingerichtet sind, aus den Ausatmungsmustern und Einatmungsmustern zu entscheiden, ob die Atmung eine normale Atmung, eine Cheyne-Stokes-Atmung, eine zentrale Hyperventilation, eine ataktische Atmung oder eine Kussmaul-Atmung

ist, und zu entscheiden, dass sich die schlafende Person in einem gefährlichen Zustand befindet, wenn die Atmung eine Cheyne-Stokes-Atmung, eine zentrale Hyperventilation, eine ataktische Atmung oder eine Kussmaul-Atmung ist.

- 5 11. Monitor nach Anspruch 2, bei welchem die Bewegungsbetragsberechnungsmittel (7) dazu eingerichtet sind, einen Bild-zu-Bild-Bewegungsbetrag in einem Teilbereich des Beleuchtungsmusters (4; 123; 133) in einer Axialrichtung, welche die Beleuchtungsmusterprojizierungsmittel (1; 91; 106; 111; 121; 131) und die Bilderfassungsmittel (5; 94; 108; 112; 124; 134) verbindet, zu berechnen und einen Bereich in einem Bild, in welchem ein Bild-zu-Bild-Bewegungsbetrag in dem Teilbereich viel größer erscheint als ein vorbestimmter Betrag oder in welchem eine Bild-zu-Bild-Bewegung in dem Teilbereich einen vorbestimmten Betrag oft überschreitet, als einen Bereich zu bestimmen, in welchem sich die schlafende Person aufhält, und bei welchem die Sicherheitsbeurteilungsmittel (10) dazu eingerichtet sind, zu entscheiden, dass sich die schlafende Person in einem gefährlichen Zustand befindet, wenn sich der Bereich, in welchem sich die schlafende Person aufhält, in kürzerer Zeit bewegt als eine vorbestimmte Zeit und sich häufig über einen vorbestimmten Betrag hinausbewegt.
- 15 12. Monitor nach Anspruch 2, bei welchem die Bewegungsbetragsberechnungsmittel (7) dazu eingerichtet sind, einen Bild-zu-Bild-Bewegungsbetrag in einem Teilbereich des Beleuchtungsmusters (4; 123; 133) in einer Axialrichtung, welche die Beleuchtungsmusterprojizierungsmittel (1; 91; 106; 111; 121; 131) und die Bilderfassungsmittel (5; 94; 108; 112; 124; 134) verbindet, zu berechnen und einen Bereich in einem Bild, in welchem ein Bild-zu-Bild-Bewegungsbetrag in dem Teilbereich viel größer erscheint als ein vorbestimmter Betrag oder in welchem eine Bild-zu-Bild-Bewegung in dem Teilbereich öfter erscheint als eine vorbestimmte Häufigkeit, als einen Bereich zu bestimmen, in welchem sich die schlafende Person aufhält, und bei welchem die Sicherheitsbeurteilungsmittel (10) dazu eingerichtet sind, zu entscheiden, dass sich die schlafende Person in einem gefährlichen Zustand befindet, wenn sich der Bereich, in welchem sich die schlafende Person befindet, näher als ein vorbestimmter Abstand einem Ende des Bettes nähert.
- 20 13. Monitor nach einem der Ansprüche 2 bis 12 mit Informierungsmitteln (12), welche dazu eingerichtet sind, auf der Grundlage eines Signalausgangs von den Signalausgabemitteln (11) eine dritte Partei zu informieren, dass sich die schlafende Person in einem gefährlichen Zustand befindet.
- 25 30 14. Monitor nach Anspruch 13, bei welchem die Informierungsmittel (12), dazu eingerichtet sind, die dritte Partei mittels Stimmen, Zeichen, Symbolen, Lichtintensität, einschließlich innerer Umgebungsbeleuchtung, oder Vibrationen über eine Telekommunikationsleitung zu informieren, dass sich die schlafende Person in einem gefährlichen Zustand befindet.
- 35 15. Monitor nach einem der Ansprüche 1 bis 14 mit Bettpräsenzerfassungsmitteln, welche dazu eingerichtet sind, die Anwesenheit/Abwesenheit einer schlafenden Person zu erfassen.
- 40 16. Monitor nach einem der Ansprüche 1 bis 15 mit einem druckempfindlichen Schalter, welcher unter der schlafenden Person platzierbar ist, um die Anwesenheit/Abwesenheit der schlafenden Person zu erfassen.

Revendications

- 45 1. Moniteur comprenant :
- des moyens de projection de motif d'éclairage (1 ; 91 ; 106 ; 111 ; 121 ; 131) conçus pour projeter un motif d'éclairage (4 ; 123 ; 133) spécifié ;
- des moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134) conçus pour prendre un motif d'éclairage projeté
- 50 continûment en tant qu'image et pour acquérir les images en tant que trames d'images ;
- des moyens de calcul de quantité de mouvement (7) pour calculer une quantité de mouvement inter-trames du motif d'éclairage (4 ; 123 ; 133) à partir de deux trames d'images acquises par les moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134) à différents instants ;
- des moyens de génération de forme d'onde de quantité de mouvement (8) conçus pour générer des données
- 55 de forme d'onde de quantité de mouvement comprenant des quantités de mouvement inter-trames agencées en une série temporelle ; et
- des moyens de détection de forme d'onde (9) conçus pour détecter un mouvement d'un objet dont une image doit être prise dans les données de forme d'onde de quantité de mouvement ;

caractérisé en ce que

l'axe optique des moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134) diffère de l'axe optique des moyens de projection de motif d'éclairage (1 ; 91 ; 106;111;121;131);

le motif d'éclairage (4 ; 123 ; 133) comporte une pluralité de points d'éclairage (71) ou de rayons de fente (81 ; 82) ; et

les moyens de calcul de quantité de mouvement (7) sont configurés pour calculer une quantité de mouvement inter-trames de chaque point d'éclairage (71) ou une quantité de mouvement inter-trames de chaque pixel correspondant à un rayon de fente (81 ; 82), respectivement, dans une direction axiale reliant les moyens de projection de motif d'éclairage (1 ; 91 ; 106 ; 111 ; 121 ; 131) et les moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134) tout en fournissant un signe positif ou négatif en fonction d'une direction de mouvement, et sont en outre configurés pour calculer une quantité de mouvement totale de chaque point d'éclairage (71) ou une quantité de mouvement totale de chaque pixel correspondant au rayon de fente (81 ; 82), respectivement, en tant que quantité de mouvement inter-trames du motif d'éclairage (4 ; 123 ; 133).

2. Moniteur selon la revendication 1, dans lequel les moyens de détection de forme d'onde (9) sont conçus pour détecter un mouvement corporel et une respiration d'une personne endormie, le moniteur comprenant en outre : des moyens de décision de sécurité (10) conçus pour décider de la sécurité de la personne endormie à partir du mouvement corporel et de la respiration de la personne endormie ; et des moyens de sortie de signal (11) conçus pour, lorsque les moyens de décision de sécurité (10) décident que la personne endormie est dans un état dangereux, délivrer un signal indiquant cela.

3. Moniteur selon la revendication 2, dans lequel les moyens de détection de forme d'onde (9) sont conçus pour détecter un motif périodique en tant que motif respiratoire, et pour détecter une variation ayant un pic élevé en tant que motif de mouvement corporel à partir des données de forme d'onde de quantité de mouvement.

4. Moniteur selon la revendication 3, dans lequel les moyens de décision de sécurité (10) sont conçus pour décider que la personne endormie est dans un état dangereux lorsqu'une période du motif respiratoire devient chaotique dans une courte période de temps, lorsque la période du motif respiratoire change brusquement, lorsque le motif respiratoire disparaît continûment, ou lorsque le motif de mouvement corporel apparaît fréquemment dans une courte période de temps.

5. Moniteur selon la revendication 3 ou 4, dans lequel, parmi des motifs respiratoires, les moyens de détection de forme d'onde (9) sont conçus pour détecter une valeur ayant un signe positif ou négatif correspondant à un mouvement dans une direction des moyens de projection de motif d'éclairage (1 ; 91 ; 106 ; 111 ; 121 ; 131) vers les moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134) sur une image et une valeur ayant un signe positif ou négatif correspondant à un mouvement dans une direction des moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134) vers les moyens de projection de motif d'éclairage (1 ; 91 ; 106 ; 111 ; 121 ; 131) sur l'image en tant que motif expiratoire et en tant que motif inspiratoire, respectivement, ou vice versa.

6. Moniteur selon la revendication 5, dans lequel les moyens de détection de forme d'onde (9) sont conçus pour compter les passages par zéro où les signes sont inversés entre un motif expiratoire et un motif inspiratoire pour compter les respirations.

7. Moniteur selon la revendication 6, dans lequel les moyens de détection de forme d'onde (9) sont conçus pour calculer un nombre de respirations par temps unitaire ou une période de respirations à partir des respirations comptées.

8. Moniteur selon la revendication 1 ou 5, dans lequel les moyens de détection de forme d'onde (9) sont conçus pour calculer un nombre de respirations par temps unitaire ou une période de respirations en effectuant une analyse fréquentielle des données de forme d'onde de quantité de mouvement exposées dans la revendication 1 ou des données d'échantillonnage obtenues en échantillonnant les motifs respiratoires exposés dans la revendication 5, en calculant la fréquence la plus importante à partir d'un spectre fréquentiel résultant, et en calculant le nombre de respirations par temps unitaire ou la période de respirations à partir de cette fréquence.

9. Moniteur selon la revendication 8, dans lequel les moyens de détection de forme d'onde (9) sont conçus pour effectuer une analyse fréquentielle avec une transformée de Fourier discrète ou une transformée en ondelettes discrète.

EP 1 350 466 B1

- 5
10
15
20
25
30
35
40
45
50
55
10. Moniteur selon l'une quelconque des revendications 5 à 7, dans lequel les moyens de décision de sécurité (10) sont conçus pour décider si la respiration est une respiration normale, une respiration de Cheyne-Stokes, une hyperventilation centrale, une respiration ataxique, ou une respiration de Kussmaul à partir de motifs expiratoires et de motifs inspiratoires et pour décider que la personne endormie est dans un état dangereux lorsque la respiration est l'une quelconque d'une respiration de Cheyne-Stokes, d'une hyperventilation centrale, d'une respiration ataxique et d'une respiration de Kussmaul.
 11. Moniteur selon la revendication 2, dans lequel les moyens de calcul de quantité de mouvement (7) sont conçus pour calculer une quantité de mouvement inter-trames dans une région partielle du motif d'éclairage (4 ; 123 ; 133) dans une direction axiale reliant les moyens de projection de motif d'éclairage (1 ; 91 ; 106 ; 111 ; 121 ; 131) et les moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134), et pour déterminer une région dans une image où une quantité de mouvement inter-trames dans la région partielle est plus grande qu'une quantité prédéterminée ou où un mouvement inter-trames dans la région partielle est fréquemment au-delà d'une quantité prédéterminée en tant que région où la personne endormie existe, et les moyens de décision de sécurité (10) sont conçus pour décider que la personne endormie est dans un état dangereux lorsque la région où la personne endormie existe se déplace dans un temps plus court qu'un temps prédéterminé et se déplace fréquemment au-delà d'une quantité prédéterminée.
 12. Moniteur selon la revendication 2, dans lequel les moyens de calcul de quantité de mouvement (7) sont conçus pour calculer une quantité de mouvement inter-trames dans une région partielle du motif d'éclairage (4 ; 123 ; 133) dans une direction axiale reliant les moyens de projection de motif d'éclairage (1 ; 91 ; 106 ; 111 ; 121 ; 131) et les moyens de prise d'image (5 ; 94 ; 108 ; 112 ; 124 ; 134), et pour déterminer une région dans une image où une quantité de mouvement inter-trames dans la région partielle est beaucoup plus grande qu'une quantité prédéterminée ou où un mouvement inter-trames dans la région partielle apparaît à une fréquence supérieure à une fréquence prédéterminée en tant que région où la personne endormie existe, et les moyens de décision de sécurité (10) sont conçus pour décider que la personne endormie est dans un état dangereux lorsque la région où la personne endormie existe est à une distance d'une extrémité du lit inférieure à une distance prédéterminée.
 13. Moniteur selon l'une quelconque des revendications 2 à 12, comprenant des moyens d'information (12) conçus pour, sur la base d'un signal délivré par des moyens de sortie de signal (11), informer un tiers du fait que la personne endormie est dans un état dangereux.
 14. Moniteur selon la revendication 13, dans lequel les moyens d'information (12) sont conçus pour informer le tiers du fait que la personne endormie est dans un état dangereux par des voix, des caractères, des symboles, une intensité de lumière comprenant une lumière d'éclairage intérieur, ou des vibrations par l'intermédiaire d'une ligne de télécommunication.
 15. Moniteur selon l'une quelconque des revendications 1 à 14, comprenant des moyens de détection de présence dans le lit conçus pour détecter la présence/l'absence d'une personne endormie.
 16. Moniteur selon l'une quelconque des revendications 1 à 15, comprenant un commutateur sensible à la pression qui peut être placé sous la personne endormie pour détecter la présence/l'absence de la personne endormie.

FIG.1

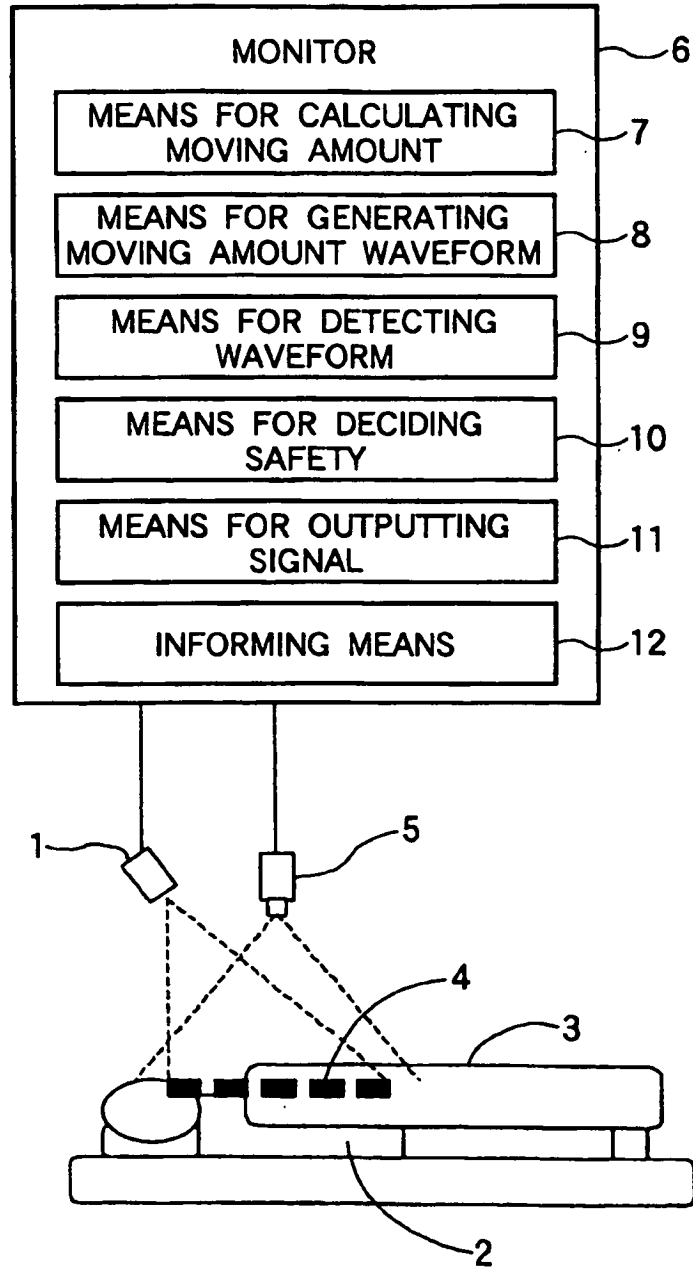


FIG.2

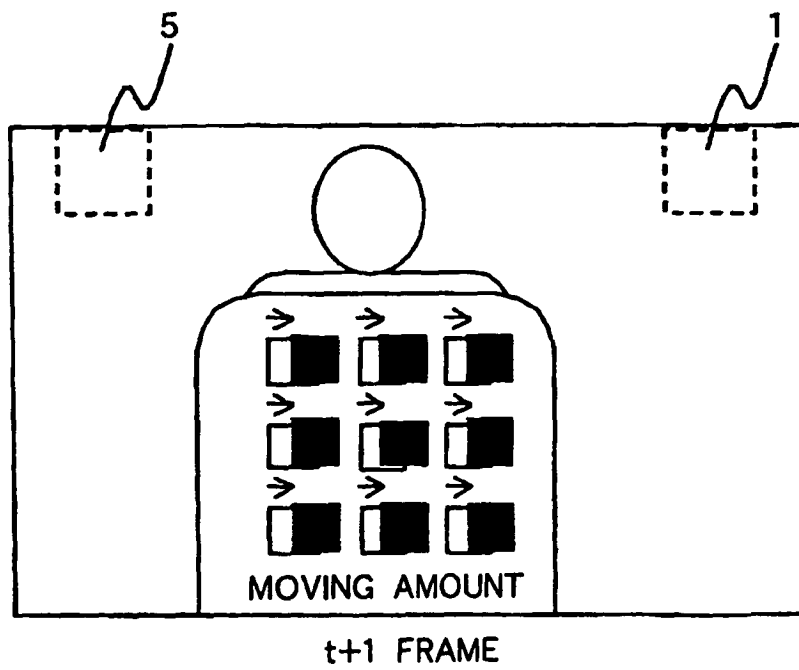
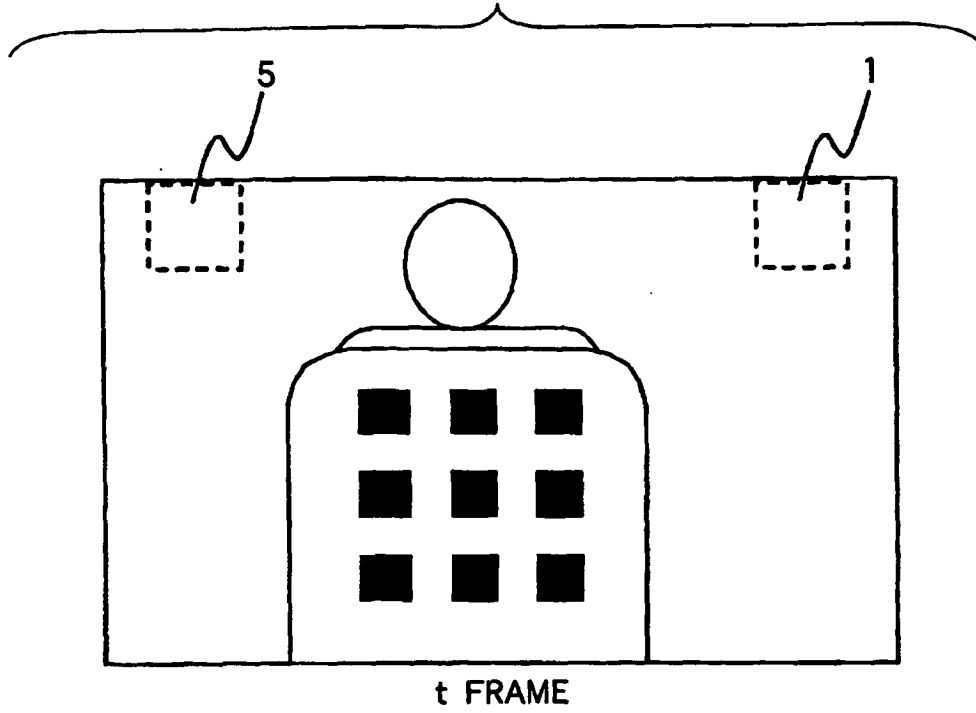


FIG.3

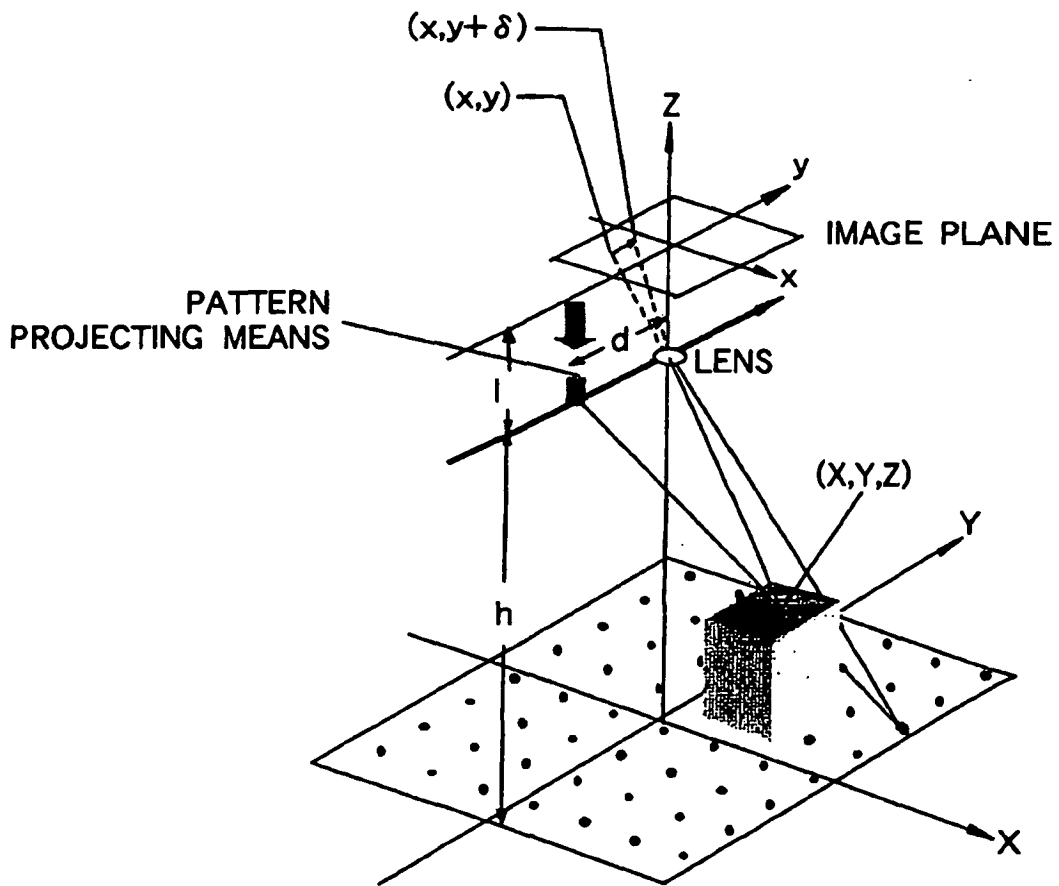


FIG.4

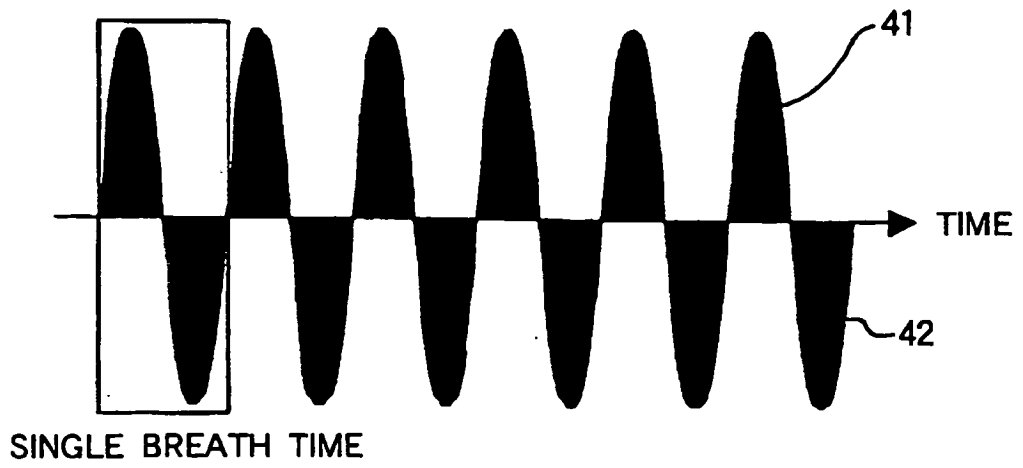
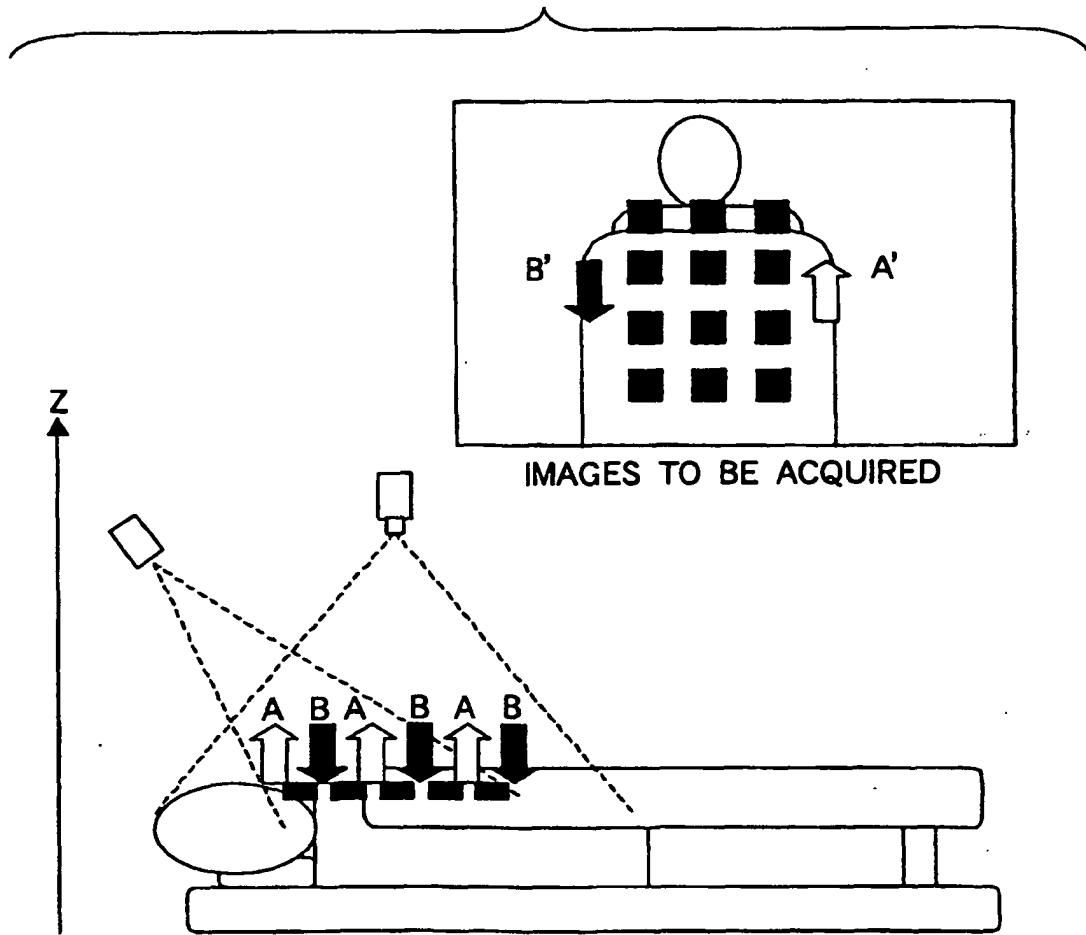


FIG.5



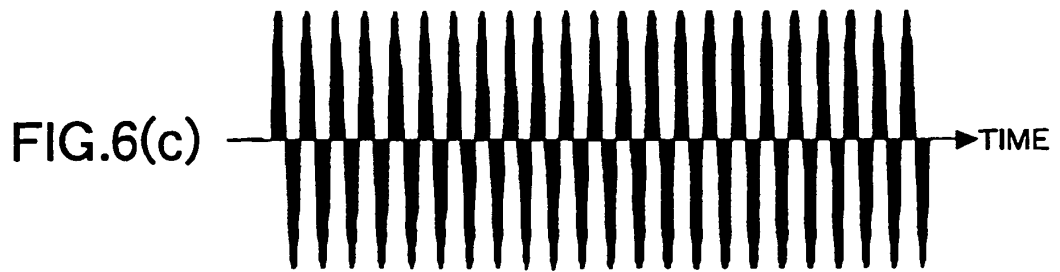
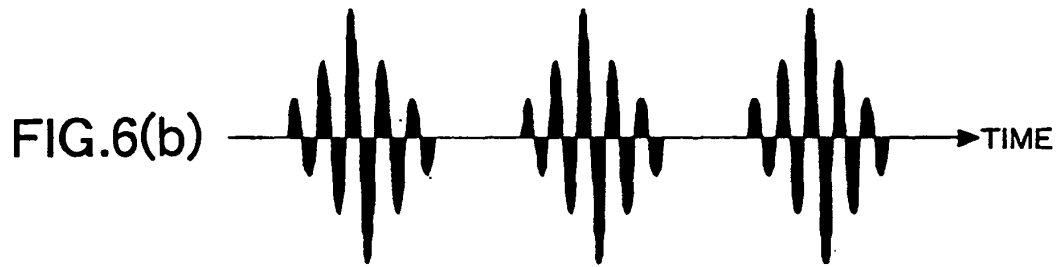
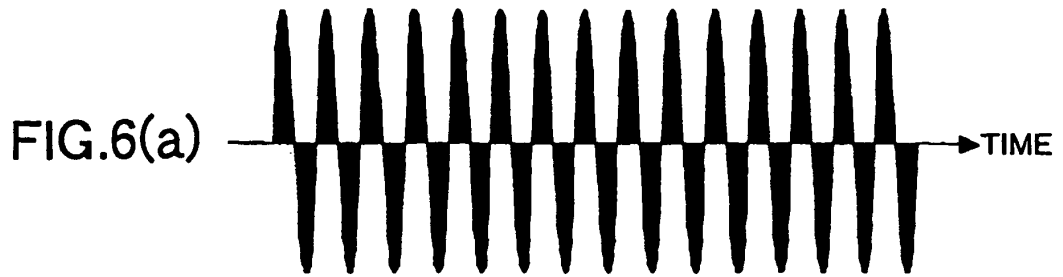


FIG.7

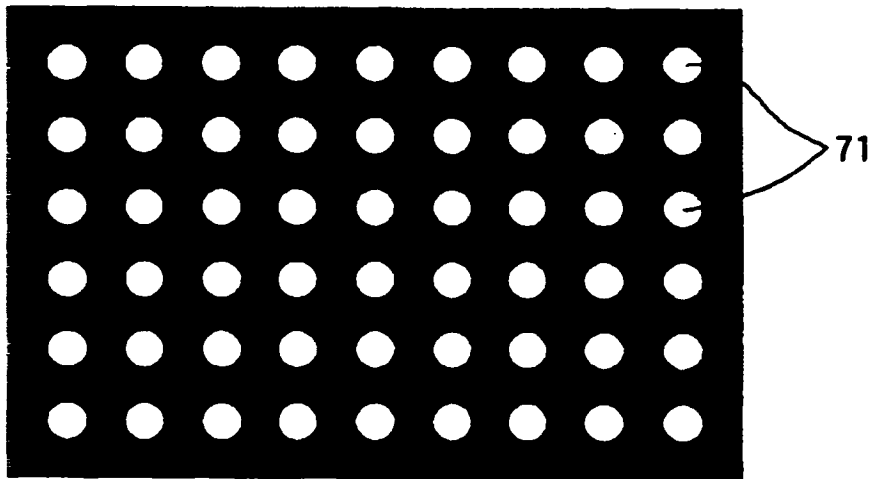


FIG.8

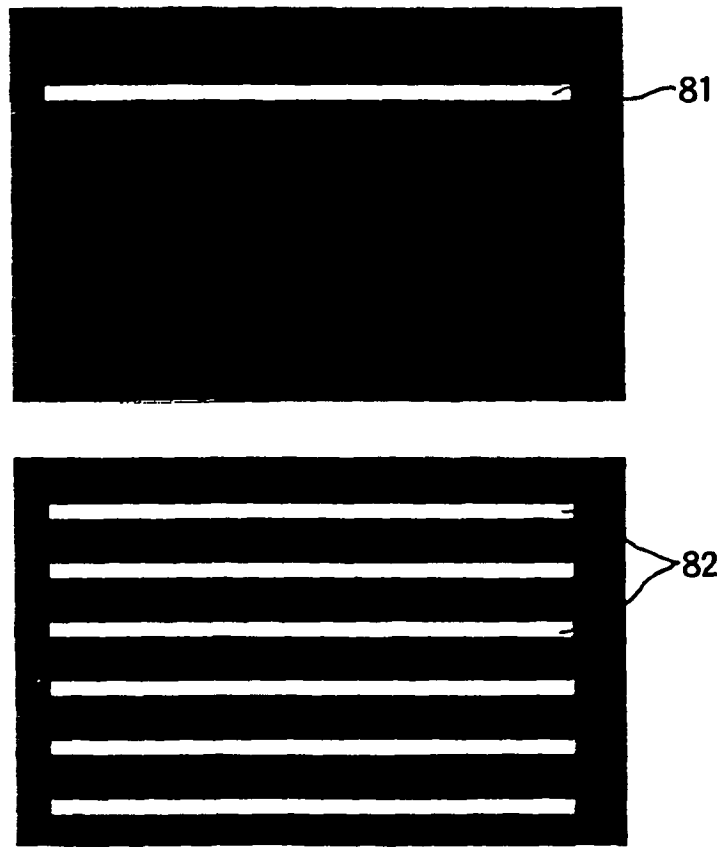


FIG.9

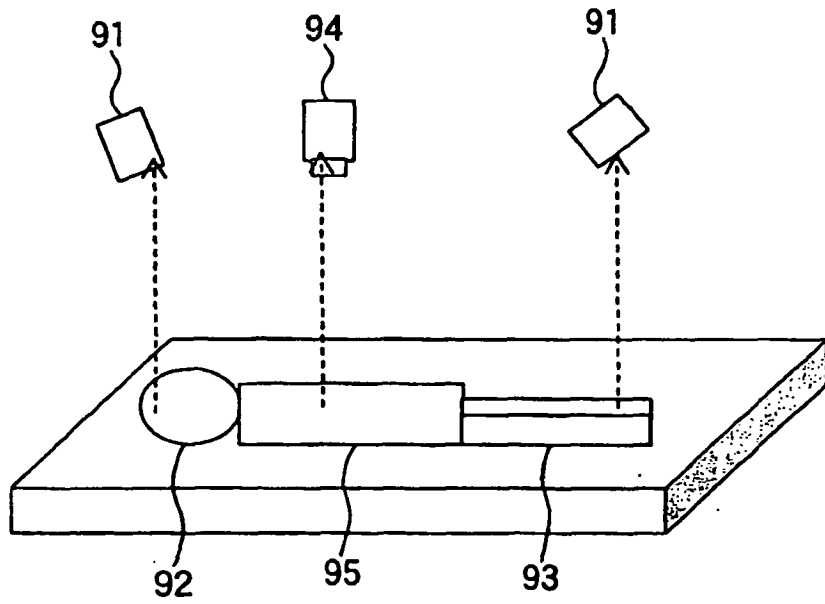


FIG.10

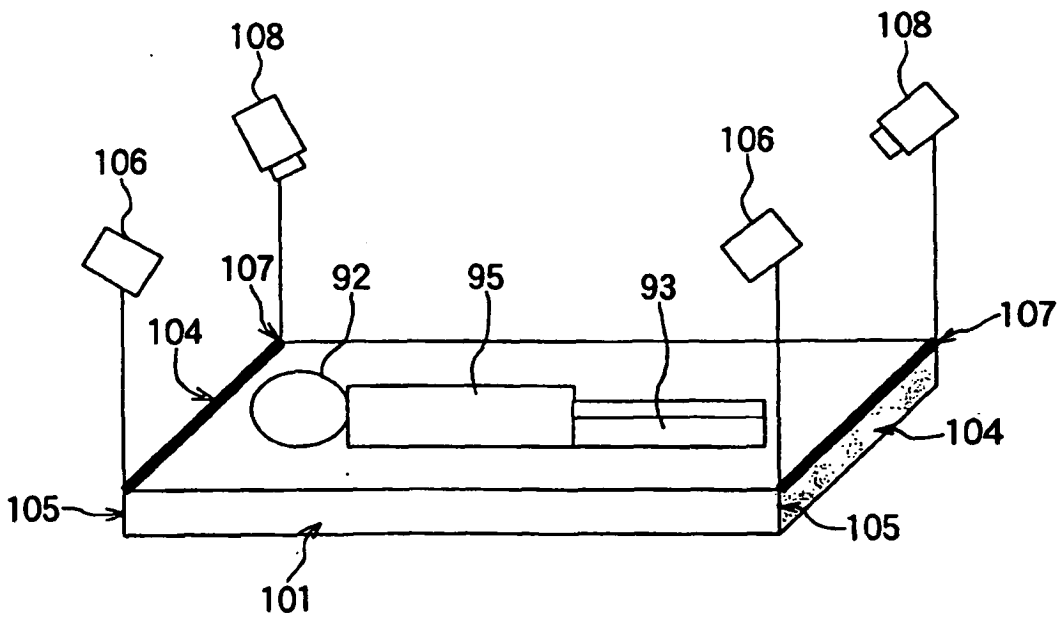


FIG.11

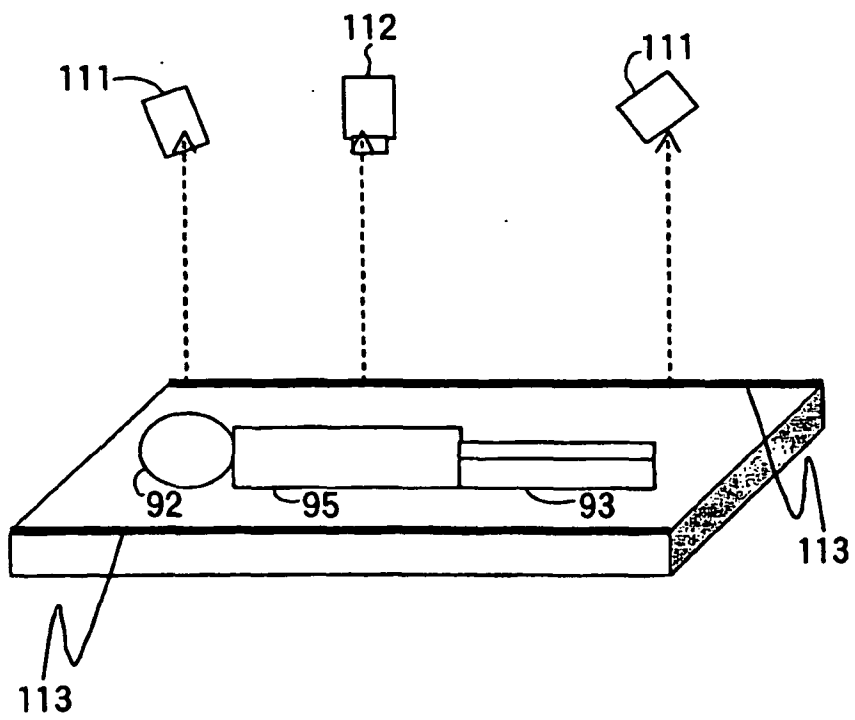


FIG.12


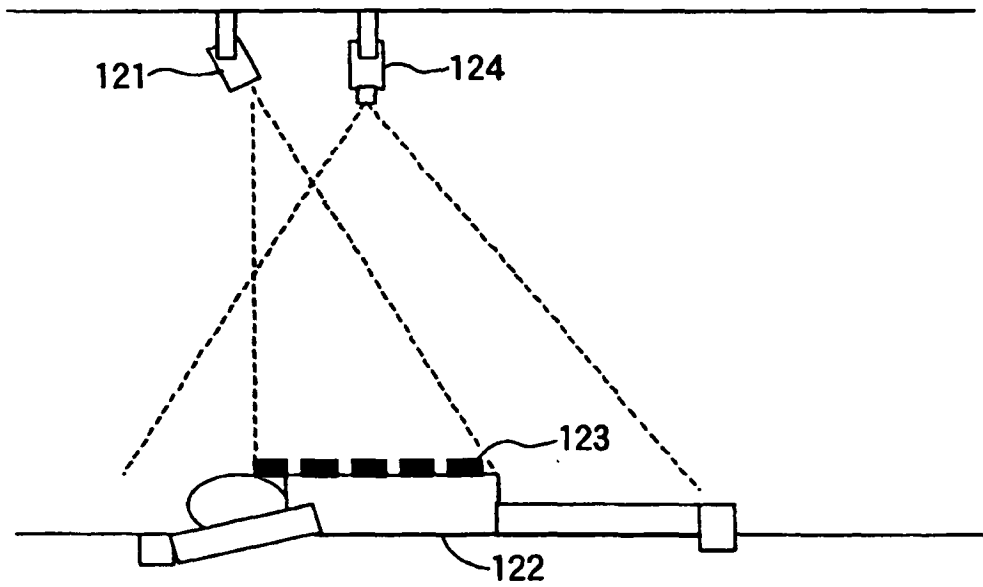


FIG.13

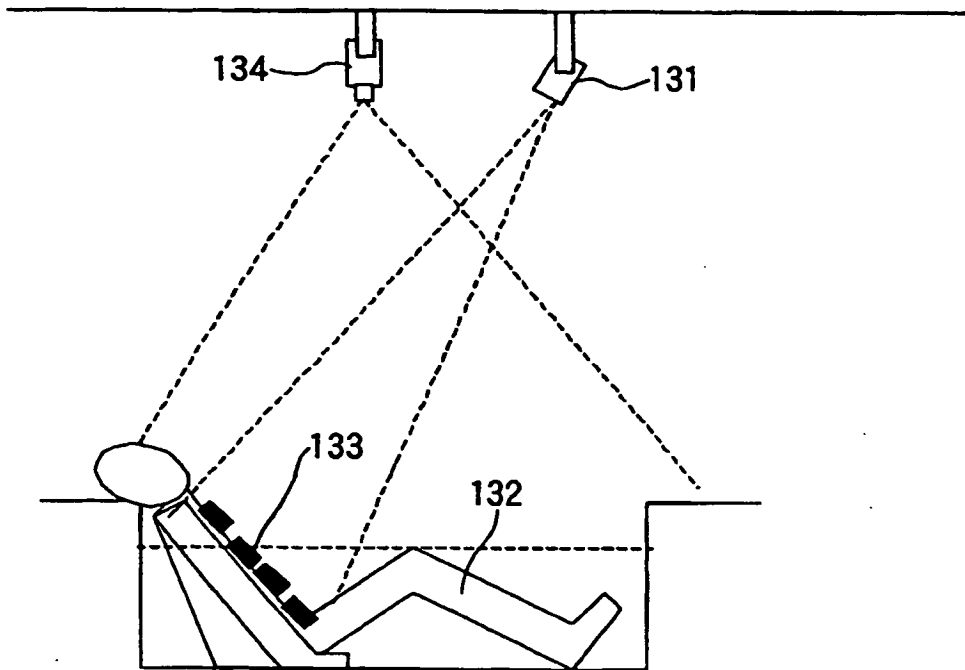

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2000107154 A [0003]
- JP H7327939 A [0004]
- JP H1128195 A [0004]
- JP 2000083927 A [0004]
- JP H1186002 A [0006] [0007] [0008]
- JP H11225997 A [0006] [0008]
- US 6062216 A [0012]
- WO 9009560 A [0013]

专利名称(译)	监控		
公开(公告)号	EP1350466B1	公开(公告)日	2011-09-14
申请号	EP2001999317	申请日	2001-12-06
[标]申请(专利权)人(译)	学校法人庆应义塾 住友大阪水泥股份有限公司		
申请(专利权)人(译)	庆应大学 住友大阪水泥有限公司.		
当前申请(专利权)人(译)	庆应大学 住友大阪水泥有限公司.		
[标]发明人	AOKI HIROOKI KEIO UNI FACULTY OF SC ANDTECH NAKAJIMA MASATO KEIO UNI FAC OF SC AND TECH TAKEMURA YASUHIRO SUMITOMO OSAKA CEMENT CO LTD MIMURA KAZUHIRO SUMITOMO OSAKA CEMENT CO LTD		
发明人	AOKI, HIROOKI KEIO UNI.FACULTY OF SC. ANDTECH. NAKAJIMA, MASATO KEIO UNI.FAC. OF SC.AND TECH. TAKEMURA, YASUHIRO SUMITOMO OSAKA CEMENT CO., LTD. MIMURA, KAZUHIRO SUMITOMO OSAKA CEMENT CO., LTD.		
IPC分类号	A61B5/11 A61B5/08 A61B5/00 A61B5/113 G06Q50/22 G08B21/02 G08B25/04		
CPC分类号	A61B5/4818 A61B5/1135 A61B5/726		
优先权	2000372820 2000-12-07 JP		
其他公开文献	EP1350466A1 EP1350466A4		
外部链接	Espacenet		

摘要(译)

一种监视器，其能够在不受睡眠者或室内照明光的姿势影响的情况下检测睡眠者的呼吸，并且可以通过图像测量容易地定量地评估检测到的呼吸。监视器包括用于投射指定照明图案的装置（1），用于连续拍摄投射光图像的装置（5），用于从所获取的两帧图像计算照明图案的帧间移动量的装置（7）通过图像拾取装置在不同时间，用于产生包括按时间序列排列的帧间移动量的移动量波形数据的装置（8），以及用于从移动量波形数据中检测物体移动的装置（9）。

$$\delta = d1z / \{h(h-z)\}$$