

(19)



(11)

EP 1 662 985 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
22.05.2013 Bulletin 2013/21

(51) Int Cl.:
A61B 5/00 (2006.01) A61B 5/024 (2006.01)

(21) Application number: **04788709.6**

(86) International application number:
PCT/US2004/029791

(22) Date of filing: **10.09.2004**

(87) International publication number:
WO 2005/025414 (24.03.2005 Gazette 2005/12)

(54) BLOOD PRESSURE MONITORING SYSTEM AND METHOD

BLUTDRUCKÜBERWACHUNGSSYSTEM UND VERFAHREN

SYSTEME ET PROCÉDE DE SURVEILLANCE DE LA PRESSION SANGUINE

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR

(72) Inventors:
• **COULSTON, George, W.**
Pittsburgh, PA 15238 (US)
• **MICKA, Thomas, A.**
West Grove, PA 19390-0068 (US)

(30) Priority: **11.09.2003 US 502760 P**
11.09.2003 US 502751 P
11.09.2003 US 502750 P
02.12.2003 US 526187 P
02.12.2003 US 526429 P
02.12.2003 US 526188 P

(74) Representative: **Wegner, Hans et al**
Bardehle Pagenberg Partnerschaft
Patentanwälte, Rechtsanwälte
Postfach 86 06 20
81633 München (DE)

(43) Date of publication of application:
07.06.2006 Bulletin 2006/23

(56) References cited:
EP-A- 0 724 860 EP-A- 0 847 724
US-A- 3 517 999 US-A- 5 222 020
US-B1- 6 511 435

(73) Proprietor: **Textronics, Inc.**
Wilmington, DE 19808 (US)

EP 1 662 985 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

Field of the Invention

[0001] This invention relates to a system and a method for monitoring blood pressure using a fabric having predetermined optical properties that respond to the motion(s) generated by geometric changes in a body due to the conduction of blood through an artery located beneath the fabric.

Description of the Prior Art

[0002] The "pulse" of the heart is associated with pressure pulses known to exist in the arteries carrying blood throughout the body. The periodic pumping of the heart produces these pressure pulses, which in turn flex the artery walls in rhythm with the pumping of the heart. The maximum, or peak, pressure exerted against the arterial wall occurs during the systole phase of the beat and is termed "systolic pressure". The lowest, or baseline, pressure (known as the "diastolic pressure") occurs during the diastole phase of the beat.

[0003] As the heart beats the pressure in the arteries fluctuates (higher during the systole phase and lower during the diastole phase of each beat), and is best described by the values for the systolic and diastolic pressures. Typical practice is to express blood pressure as a ratio of the maximum and minimum values.

[0004] The generally known method to determine these two blood pressure extremes is the auscultatory method. In this method a pressure cuff is applied to a person's upper arm. This cuff includes a bladder capable of holding air at a predetermined known pressure. The cuff bladder is inflated to a pressure above the highest expected pressure to be measured, i.e., above the systolic pressure. When inflated at this highest pressure, the cuff prevents the flow of blood in the brachial artery of the arm underlying the pressure cuff. The bladder is equipped with a valve, which allows the pressure to be reduced in a controlled way.

[0005] As air is released from the bladder, blood flow in the brachial artery is re-established. The inflow of blood through the artery is accompanied by pulsing sounds known as the Korotkoff sounds. These sounds are detected using a stethoscope at a point on the brachial artery just below the pressure cuff. The falling pressure in the cuff bladder is observed while air is released.

[0006] The Korotkoff sounds are divided in five phases based on loudness and certain qualitative features. The five phases of the Korotkoff sounds are also identified with certain pressure regimes, as normal arterial blood flow is being re-established. The first phase of the Korotkoff sounds (Phase 1) is heard at about 120 millimeters of mercury (mm Hg) characterized by a sharp "thud"; this is the systolic (maximum) blood pressure. Phase 2 is

identified with a pressure of about 110 mm Hg and is heard as a swishing or blowing sound. Phase 3 is identified with a pressure of about 100 mm Hg and is described as a thud that is softer than that of Phase 1. At a pressure of about 90 mm Hg the first diastolic pressure is detected, called the Phase 4 Korotkoff sound, and heard as a softer blowing sound which disappears. Phase 5 is identified with about 80 mm Hg, and is called the second diastolic pressure. This last phase is silent, meaning that a laminar blood flow has been again established. Phase 5 may be absent in some human subjects. For this reason, the first diastolic pressure of Phase 4 is recorded as the lowest pressure in the artery.

[0007] An automated auscultatory apparatus relies on detecting sound levels and complex processing of these sounds into electronic signals, which are correlated with the phases of the Korotkoff sounds. Representative of an automated arrangement that uses an auscultatory method is the measurement system disclosed in U.S. Patent 6,511,435 (Bluth et al.)

[0008] The re-establishment of blood flow in an occluded artery is also accompanied by a relatively significant flexure of the arterial wall. The flexure diminishes as the artery widens with the decrease in cuff pressure. In an alternative form of blood pressure measuring apparatus, known as an oscillatory measurement system, the mechanical vibrations accompanying arterial wall flexure are transformed into sound as they enter the inflated bladder of the cuff. This sound is detectable using a microphone located in the bladder. U.S. Patent 6,458,085 (VVu et al.) discloses an oscillatory blood pressure measurement arrangement. An oscillatory blood pressure measurement arrangement is also disclosed in the above-mentioned U.S. Patent 6,511,435 (Bluth et al.).

[0009] One drawback of oscillatory measuring apparatus is the reliance upon a cuff bladder modified to contain a microphone and associated connections to an external signal processor. Using a microphone to detect changes in sound pressure level and recognizing a pattern from the waveform so generated is difficult.

[0010] Document EP o 847 724 A1 describes a sphygmomanometer capable of highly accurately judging the maximum blood pressure and minimum blood pressure, which has a cuff 10 which is attached to an appointed portion of a patient and presses the artery by supplying air therein; an optical range sensor 12 which is located opposite said cuff 10 and is able to detect the pulsation displacement of said artery; a digital processing section 14 which is able to judge the maximum and minimum blood pressure of said patient on the basis of photoelectric volumetric pulse wave signals sent out by said optical range sensor 12; and a display section 38 which is able to display the maximum and minimum blood pressure values judged by said digital data processing section 14

[0011] Further, document US 3,517,999 relates to an optical strain gauge comprising a flexible body which is deformable according to the sense of an external force. A source of light and a photo cell in spaced relationship

in the source of light are embedded in the body. The photo cell is responsive to light transmission through the material of the body and produces a signal according to the deformation produced in the body by the external force.

[0012] Further, document US 2003/095263 discloses a fiber optic interferometric vital sign monitor for use in magnetic resonance imaging, confined care facilities and in-hospital. A fiber optic monitor that utilizes optical phase interferometry to monitor a patient's vital signs such as respiration, cardiac activity or blood pressure comprises an optical fiber proximately situated to the patient so that time varying acousto-mechanical signal from the patient are coupled into the optical fiber.

SUMMARY OF THE INVENTION

[0013] The invention is defined in independent claims 1 and 7. The present Invention is directed to a system and method for monitoring blood pressure by detecting motion due to geometric changes in the wearer's body.

[0014] The present invention is usable with an inflatable arm cuff that is selectably inflatable to differing air pressures and incorporates a fabric which has both a light transmission property and a light reflection property when the fabric is illuminated with light having wavelength(s) in the range of from about 400 nanometers to about 2200 nanometers, and particularly in the ranges from about 400 to about 800 nanometers and from about 700 to about 2200 nanometers. The amount of light transmitted through the fabric relative to the amount of light reflected by the fabric is able to change when the fabric stretches in response to motion in the wearer's body due to changes in the flow of blood through an artery disposed beneath the fabric.

[0015] A radiation source that emits radiation with wavelength(s) in the range from about 400 nanometers to about 2200 nanometers, and particularly in the ranges from about 400 to about 800 nanometers and from about 700 to about 2200 nanometers, and a radiation detector are attached to the fabric in relative positions such that the reception of incident radiation by the detector is directly affected by a change in the amount of light transmitted through the fabric relative to the amount of light reflected by the fabric as the fabric stretches in response to motion in the body of a wearer due to changes in the flow of blood through an artery disposed beneath the patch occurring in consonance with variations in the air pressure within the inflatable cuff. A pressure recorder responsive to the signal output from the detector records the pressure of the cuff when the output of the detector is at a minimum value and the pressure in the cuff following the minimum when the signal from the detector again lies within a predetermined range of a baseline signal value. In one embodiment, the fabric forms a patch that is disposed on or over the inflatable arm cuff.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] The invention will be more fully understood from the following detailed description, taken in connection with the accompanying drawings, which form a part of this application, and in which:

Figure 1 is a schematic diagram of a system useful for the monitoring blood pressure of a subject by sensing geometric changes in the body of the subject due to the motion of blood passing through blood vessels underlying a patch of monitoring fabric; Figures 2A and 2B are diagrammatic views illustrating possible light transmission and reflection response of the fabric used in the monitoring system of the present invention during normal systole and diastole phases of heart action;

Figures 2C and 2D are respective diagrammatic views illustrating possible light transmission and reflection response of the fabric when a blood vessel underlying a patch formed of such fabric is totally occluded and when blood flow is re-established;

Figure 2E is a graphical representation of the change in the amount of light transmitted through the fabric relative to the amount of light reflected by the fabric as the fabric stretches and recovers during normal systole and diastole phases of heart action (Figures 2A and 2B), and when a blood vessel underlying the fabric is totally occluded and when blood flow is thereafter re-established (Figures 2C and 2D);

Figure 2F is a graphical representation of a signal, periodic in time, representing the changes in the amount of light transmitted through the monitoring fabric relative to the amount of light reflected by the monitoring fabric as represented in Figure 2E; and Figure 3 is a diagram illustrating the temporal relationship between pressure measured in an inflatable cuff disposed over an artery of a wearer and the voltage appearing of the detector when the method and system of the present invention is used to monitor blood pressure of the wearer.

DETAILED DESCRIPTION OF THE INVENTION

[0017] Throughout the following detailed description similar reference characters refer to similar elements in all figures of the drawings.

[0018] Figure 1 is a stylized pictorial representation of a system **10** useful with the method of the present invention for directly monitoring blood pressure of a subject by sensing motion due to geometric changes in the body of the subject associated with the flexing of arterial walls produced by blood pressure pulses.

[0019] As seen in Figure 1, the system **10** includes a sleeve **12** having any convenient fabric construction (e.g., knitting, weaving) and made from any suitable textile filament apparel denier yarn. The sleeve **12** includes at least a portion, or patch, **14** formed from a monitoring

fabric **16**. The monitoring fabric **16** has an inner surface **16I** and exterior or outer surface **16E**. Although the patch **14** is represented as rectangular in shape in Figure 1, it should be understood that the patch **14** may take any convenient or desired shape. If desired, a portion or even the entirety of the sleeve **12** may be made from the monitoring fabric **16**.

[0020] The monitoring fabric **16** in accordance with the present invention exhibits both a light transmission property and a light reflection property when the fabric is illuminated with light having a wavelength in the extended range from about 400 to about 2200 nanometers. This range is extended in the sense that it encompasses both near infrared light and visible broad spectrum white light.

[0021] As used herein the term "broad spectrum white light" means light having a wavelength in the range from about four hundred (400) nanometers to about eight hundred (800) nanometers.

[0022] As used herein the term "near infrared light" means light having a wavelength in the range from about seven hundred (700) nanometers to about twenty two hundred (2200) nanometers. The wavelength of 805 nanometers or the wavelength of 880 nanometers may be used in systems operating in the near infrared spectrum. The wavelength of 805 nanometers is preferred.

[0023] In accordance with the present invention, the amount of light transmitted through the fabric **16** relative to the amount of light reflected by the fabric **16** is able to change as the fabric stretches. The fabric stretches in response to geometric changes of the body of the subject due to the flexing of the arteries in response to blood pressure pulses. The term "light balance" may be used herein to refer to the amount of light transmitted through the fabric **16** relative to the amount of light reflected by the fabric **16**.

[0024] Light reflected by the fabric toward an aperture of acceptance defined with respect to an axis extending from the surface of the fabric is useful in producing a signal output from a detector located in the aperture. Alternatively, light transmitted through the fabric is "lost" to a detector placed at the aperture of acceptance.

[0025] The monitoring fabric **16** used in the patch **14** can be made from a reflective yarns, stretchable yarns any combination of reflective and stretchable yarn or any like material. In one exemplary construction a first plurality of reflective yarns is combined with a second plurality of stretchable yarns. The yarns can be combined in any conventional manner including woven or non-woven construction.

[0026] For woven constructions, yarns can be combined in plain weave, satin weave, twill weave or any other well known constructions. Woven fabrics may also include weft elastic, warp elastic or bielastic woven fabrics for varying fabric elasticity.

[0027] For non-woven constructions such as knit constructions, yarns can be combined by circular knit, warp knit or any other suitable knit construction. In circular knits, typical constructions are single jersey (i.e. different

structure in front and back, e.g. 1x1 knit) and double jersey (i.e. same structure in front and back, e.g. 2x1 knit). The stitch size and distance determine the openness of the knit fabric. Warp knits may include tricot and raschel constructions where the tightness is determined by the number of needles/inch or the stitch size.

[0028] Any suitable apparel denier and any suitable needle combination or warp/weft intensity may be used in making the monitoring fabric. Each reflective yarn may comprise a coating of a specularly reflective material thereon. The coating may also be electrically conductive. Furthermore, the reflective yarn may be elastic. Each stretchable yarn is formed as a combination of an elastic yarn component and a hard yarn component.

[0029] In the preferred instance, the reflective yarn is that yarn sold by Laird Sauquoit Technologies, Inc. (300 Palm Street, Scranton, Pennsylvania, 18505) under the trademark X-static® yarn. X-static® yarn is based upon a 70 denier (77 dtex), 34 filament textured nylon available from INVISTA North America S. à r.l., Wilmington, Delaware 19805, as product ID 70-XS-34X2 TEX 5Z electroplated with electrically conductive silver.

[0030] Alternatively, another method of forming the monitoring fabric **16** is to screen-print a pattern using an electrically conductive ink after constructing the yarns in any conventional woven or non-woven manner. Suitable electrically conductive inks include, but are not limited to, those sold by DuPont Microcircuit Materials, Research Triangle Park, NC 27709, as silver ink 5021 or silver ink 5096, and the like.

[0031] A screen-printed pattern of conductive inks must also allow the fabric to move. Preferably, the conductive ink does not affect the ability of the fabric to stretch and recover. One way to prevent affecting the stretch and recovery properties of fabric is to screen-print a pattern of conductive ink(s) in the form of a matrix of dots. Such a dot matrix pattern provides full freedom of movement for the yarns in the fabric, while still exhibiting desired light reflection and transmission properties.

[0032] The patch **14** of monitoring fabric **16** can alternatively be formed from elastic and electrically conductive composite yarn comprising a core yarn made of, for instance, LYCRA® spandex yarn wrapped with insulated silver-copper metal wire obtained from ELEKTRO-FEINDRAHT AG, Escholzmatt, Switzerland, using a standard spandex covering process. The core yarn may further be covered with any nylon hard yarn or polyester hard yarn.

[0033] Stretchable yarn can be formed in any conventional manner. For example, the stretchable yarn can be formed as a combination of a covered elastic yarn and a hard yarn.

[0034] In one preferred embodiment, the covered elastic yarn can be comprised of a twenty (20) denier (22 dtex) LYCRA® spandex yarn single-covered with a ten (10) denier (11 dtex) seven filament nylon yarn. LYCRA® spandex yarn is available from INVISTA North America S. à r.l., Wilmington, Delaware 19805. Alternatively, the elastic yarn component of the present invention may

comprise elastane yarn or polyester bicomponent yarns, such as those known as ELASTERELL-P™ from INVISTA North America S.à r.l., Wilmington, Delaware 19805. The terms spandex and elastane are used interchangeably in the art. An example of a branded spandex yarn suitable for use with the present invention is LYCRA®.

[0035] Synthetic bicomponent multifilament textile yarns may also be used to form the elastic yarn component. One preferred synthetic bicomponent filament component polymer can be thermoplastic. The synthetic bicomponent filaments can be melt spun or formed in any other manner common in the art of filament formation. In the most preferred embodiment, the component polymers can be polyamides or polyesters.

[0036] A preferred class of polyamide bicomponent multifilament textile yarns comprises those nylon bicomponent yarns which are self-crimping, also called "self-texturing". These bicomponent yarns comprise a component of nylon 66 polymer or copolyamide having a first relative viscosity and a component of nylon 66 polymer or copolyamide having a second relative viscosity, wherein both components of polymer or copolyamide are in side-by-side relationship as viewed in the cross section of the individual filament. Self-crimping nylon yarn such as that yarn sold by INVISTA North America S.à r.l., Wilmington, Delaware 19805 under the trademark TACTEL® T-800™ is an especially useful bicomponent elastic yarn.

[0037] Some examples of polyester component polymers include polyethylene terephthalate (PET), polytrimethylene terephthalate (PTT) and polytetraethylene terephthalate. In one preferred embodiment, polyester bicomponent filaments comprise a component of PET polymer and a component of PTT polymer in a side-by-side relationship as viewed in the cross section of the individual filament. One exemplary yarn having this structure is sold by INVISTA North America S.à r.l., Wilmington, Delaware 19805 under the trademark T-400™ *Next Generation Fiber*.

[0038] The hard component could be made from any inelastic synthetic polymer fiber(s) or from natural textile fibers, such as wool, cotton, ramie, linen, rayon, silk, and the like. The synthetic polymer fibers may be continuous filament or staple yarns selected from the multifilament flat yarns, partially oriented yarns, textured yarns, bicomponent yarns selected from nylon, polyester or filament yarn blends. The hard component is preferably 260 denier (286 dtex) 68 filament nylon yarn.

[0039] Nylon yarns may comprise synthetic polyamide component polymers, such as nylon 6, nylon 66, nylon 46, nylon 7, nylon 9, nylon 10, nylon 11, nylon 610, nylon 612, nylon 12 and mixtures and copolyamides thereof. In the case of copolyamides, especially preferred are those including nylon 66 with up to 40 mole percent of a polyadipamide wherein the aliphatic diamine component is selected from the group of diamines available from E.I. Du Pont de Nemours and Company of Wilmington, Delaware under the respective trademarks DYTEK A® and DYTEK EP®.

[0040] Further in accordance with the present invention, the hard yarn portion may comprise polyesters such as, for example, polyethylene terephthalate (PET), polytrimethylene terephthalate (PTT), polybutylene terephthalate and copolyesters thereof.

[0041] The monitoring fabric **16** may also be formed from composite yarns in which the reflective and stretchable components are combined in the same yarn. Such a composite yarn would include a covering yarn having a spectrally reflective outer surface that is wrapped about an elastic yarn component in one or more layers.

[0042] The remainder of the structure of the sleeve **12**, if not also formed of the monitoring fabric, may exhibit any convenient textile construction (e.g. knitting or weaving as described above), and may be made from any suitable textile filament apparel denier yarn.

[0043] In one embodiment, the monitoring fabric **16** used in the patch **14** is attached to the sleeve **12**. The patch **14** could be sewn, glued, taped, buttoned, interwoven or attached to the sleeve by any conventional means. In another embodiment, the sleeve **12** is completely constructed of the monitoring fabric **16**.

[0044] The present invention is directed to monitoring the light balance of a monitoring fabric **16** as it stretches and recovers. For this purpose, the system **10** includes a suitable source **18** of radiation operable in the wavelength range from about 400 nanometers to about 2200 nanometers, and particularly in the ranges from about 400 to about 800 nanometers and from about 700 to about 2200 nanometers. An associated detector **22** is responsive to incident radiation in the given wavelength range and subranges for producing signals in response thereto.

[0045] In the case of operation with near infrared light, the radiation source **18** can be a compound semiconductor-based (e.g., gallium arsenide or gallium aluminum arsenide) photo-emitting diode operating in the infrared range (at a wavelength of, for example, 805 nanometers or 880 nanometers). The detector **22** can be any device that can detect radiation, for instance, a photodiode coupled to appropriately configured output amplification stages. Any well known semiconductors can be used for forming the photodiode including silicon or germanium. A commercially available radiation source and detector package suitable for use in the system of the present invention is that available from Fourier Systems Ltd. (9635 Huntcliff Trace, Atlanta, Georgia, 30350) as model DT155 (0-5 volt output).

[0046] For broad spectrum white light (400 to 800 nanometers) operation, the source **18** can be a compound semiconductor-based "white LED" (e.g., a light emitting diode employing an indium gallium nitride based device with suitable phosphors to provide broad spectrum white light emission). An LED source of broad spectrum white light is available from Lumitex® Inc., 8443 Dow Circle, Strongsville, Ohio 44136, USA; Part No. 003387. Such an LED provides radiation in the wavelength range of 430 to 700 nanometers. The detector **22** is a preferably

a silicon phototransistor coupled to appropriately configured output amplification stages.

[0047] The radiation source **18** and the detector **22** are attached to monitoring fabric **16** in predetermined relative positions. The positions were determined such that the reception of incident radiation by the detector **22** is directly affected by a change in the amount of light transmitted through the monitoring fabric **16** relative to the amount of light reflected by the monitoring fabric **16** when the fabric stretches and recovers. In the preferred case, the radiation source **18** and detector **22** are embedded, or fixed firmly, into the textile structure of the monitoring fabric **16**. The radiation source **18** and detector **22** can be fixed using any well known attachment method, including, but not limited to, clamping, gluing, sewing, taping, or hook and loop fasteners (Velcro). Optionally, it may be desirable in some operational configurations of the invention to dispose both the source and the detector remotely from and not in direct contact with the fabric **16**. In such a remote arrangement, the radiation source **18** and detector **22** could be located in any arrangement that permits the detector **22** to detect changes in the transmission and reflection of radiation during stretching and recovery.

[0048] The source **18** may be arranged in such a way as to maintain its relative position to the detector **22**. For instance, the source **18** and the detector **22** may be rigidly connected together on one side of the fabric **16** to maintain a spatial relationship. Alternatively, the position of the source **18** relative to the detector **22** can be maintained on opposite sides of the monitoring fabric **16** for monitoring light transmission. In such an embodiment, the radiation source is connected to the radiation detector using a "clothes-pin" or alligator style clamp. Other well known means of maintaining spatial relationship between the source and the detector are contemplated.

[0049] The apparatus **10** represented in Figure 1 further includes an inflatable cuff **28** substantially similar to a standard cuff known in the blood pressure measurement art. The cuff **28** is typically a woven nylon sleeve with a seamless inner bladder **30** of latex rubber. The inner bladder **30** communicates with an external air pump **32**, valve **34** and a pressure measurement device **36** for measuring the internal pressure of the bladder **30**. The pressure measurement device **36** communicates electrically with the processor **26** over an electrical connection **38**. The valve **34** may be configured for automatic operation by the signal processor **26** over a control line **40**.

[0050] The pump **32** may take the form of any conventional pump including a manually operated device, an automated piston or diaphragm air pump. The pressure measurement device **36** may be implemented using a manometer of known design. Such a manometer is constructed using known barometric measurement techniques that include a column of mercury, a Bourdon gauge movement, and a measurement device having a high reproducibility of measurement in the expected range of operation, for example, from about ten (10) mil-

limeters of mercury to about five hundred (500) millimeters of mercury (mm Hg). A suitable pressure measurement device **36** could be a direct capacitance measurement device provided with a fully electronic output suitable for use with traditional digital signal processors. A pressure transducer operable to measure the pressure within the cuff at predetermined sampling time intervals is also suitable for use as the pressure measurement device. The miniature silicon pressure sensor package available from Advanced Custom Sensors, Inc. Irvine, California, 92618 as Model 7277 (zero to five volt output; zero to seven pounds per square inch gage rating) is such a device, though any similar means for measuring pressure is contemplated.

[0051] The principles of operation by which the motion of a subject's body due to geometric changes generated by blood pressure pulses may be monitored in accordance with the system of the present invention may be more clearly understood with reference to Figures 2A through 2F. In the discussion that follows both the source **18** and the detector **22** are mounted adjacent to the same surface **16E** of the monitoring fabric **16** so as to operate in a "reflection mode". Alternatively, it is contemplated within the scope of the invention to operate in a "transmission mode". In the alternative transmission mode of operation, the source **18** and the detector **22** are mounted to opposite sides of the monitoring fabric **16**.

[0052] The reaction of the fabric **16** during normal diastole and systole phases of heart action are depicted in Figures 2A and 2B.

[0053] As represented in Figure 2A in a normal diastole phase the yarns **16Y** forming the monitoring fabric **16** lie within a relatively close distance of each other to define a pattern of relatively narrow gaps **16G**. A generally circular spot indicated by the reference character **17** represents the area of the monitoring fabric **16** illuminated by the source **18**. Of the photons emitted from the radiation source **18** toward the surface **16E** of the fabric **16** some photons are absorbed (*e.g.*, represented by a ray **18C**) by the yarns **16Y** of the fabric while other photons (*e.g.*, the rays **18A** and **18B**) pass through gaps **16G** therein. These photons are lost to the detector **22**. The major portion of the light (*e.g.*, represented by the rays **18D** through **18G**) is reflected from the surface **16E** of the monitoring fabric **16** toward the detector **22**. This major portion of the light is detected by detector **22**, which in turn produces a corresponding output signal.

[0054] During a normal systole phase of a heart beat, the size of the gaps **16G** formed in the monitoring fabric **16** increases in response to motion induced by the flexure of the underlying blood vessels. This increase in size of the gaps **16G** (Figure 2B) increases the likelihood that a photon will pass through the fabric **16**, and decreases the likelihood that a photon will reflect toward the detector **22**. The total number of photons lost to the detector **22** by transmission through or absorption by the fabric (*e.g.*, represented by the rays **18A**, **18B** and **18C**) increases. The signal output from the detector **22** concomitantly de-

creases. Although the number of photons lost to the detector **22** by absorption (e.g., represented by the ray **18C**) does not necessarily change, the likelihood that a photon will strike a yarn **16F** and be reflected or absorbed decreases since the spot size **17** remains constant in the area while the gap **16G** size increases.

[0055] As the systolic phase of the pulse beat gives way to the diastolic phase, the fabric **16** undergoes the elastic recovery. The gaps **16G** return to their original size (Figure 2A). The major portion of the light is again reflected toward the detector **22**, increasing the output signal therefrom.

[0056] The left hand portion of Figure 2E illustrates the waveform of the signal generated at the detector **22** as the fabric undergoes its stretch cycle from the initial diastolic phase (represented by the reference character "I") through a systolic phase (represented by the reference character "II") and back to the diastolic phase ("I"). This portion of Figure 2E graphically illustrates that during the course of a stretch cycle the light balance (reference character "LB" in Figure 2E) of the fabric changes.

[0057] As shown in Figure 2E, at diastolic phase ("I") of Figure 2A, the reflected light represented by the bottom portion below the "LB" is greater than the transmitted light represented by the upper portion above the "LB". In contrast, Figure 2E shows that at systolic phase ("II") of Figure 2B, the reflected light represented by the bottom portion below the "LB" is less than the transmitted light represented by the upper portion above the "LB".

[0058] Comparison between the diastolic and systolic phases indicates that the amount of light transmitted through the monitoring fabric **16** relative to the amount of light reflected by the monitoring fabric **16** changes in a periodic fashion over time as the fabric stretches. Light lost to the detector **22** by absorption may be considered as contributing to the "transmitted light" section of the graph of Figure 2E. This periodic variation in light balance is represented in the left-hand portion of Figure 2F as a time-varying signal synchronized with the elongation and recovery stages of fabric stretch (e.g., diastolic phase represented by character "I" and systolic phase represented by character "II").

[0059] The situation that arises when a cuff is fully pressurized is depicted in Figure 2C. In this case the flow of blood is completely interrupted and no flexure of the underlying artery occurs. The fabric **16** reverts to a fully unstretched condition with the gap spacing **16G** between yarns **16Y** being at its minimum. Substantially all of the photons falling on the illuminated spot **17** are reflected toward the detector **22** resulting in the light balance depicted at reference character "III" in the right hand portion of Figure 2E. At reference "III", the reflected light represented by the bottom portion below the "LB" is significantly greater than the transmitted light represented by the upper portion above the "LB".

[0060] Figure 2D depicts the situation when blood flow through the previously occluded artery is re-established. The sudden rush of blood through the artery elongates

the fabric **16** and extends the gaps **16G** to a wider extent than in the systolic phase (shown in Figure 2B). The amount of light transmitted through the fabric **16** increases commensurately while the amount of light reflected significantly decreases. This result is illustrated in the change in light balance depicted at reference character "IV" in the right hand portion of Figure 2E. In Figure 2E, at reference character "IV", the reflected light represented by the bottom portion below the "LB" is less than the transmitted light represented by the upper portion above the "LB". The right hand portion of Figure 2F illustrates the rapid decrease in signal output from the detector **22** caused by the sudden rush of blood through the previously occluded artery (e.g., the change in detector output voltage from phase "III" to phase "IV" shown in Figure 2F)

[0061] As the rush of blood diminishes the light balance and the signal output from the detector **22** would revert toward the ranges exhibited during normal diastolic and systolic operation.

OPERATION

[0062] In an exemplary mode of operation the apparatus of the present invention would be applied to the arm of a person generally in the position indicated by the dotted outline in Figure 1, with the fabric patch **14** of sleeve **12** over the brachial artery. The inflatable cuff **28** is applied over the sleeve **12**.

[0063] Figure 3 illustrates the temporal relationship between pressure measured in the cuff **28** and a voltage resulting from the radiation detected by the detector **22** in reflection mode. In a reflection mode of operation, the source **18** and the detector **22** are arranged adjacent to side **16E** of the fabric **16**. As discussed in connection with Figures 2A through 2F, any fabric **16** elongation is accompanied by a decreasing signal (voltage) from the detector **22**, corresponding to increased light transmission through the fabric **16**.

[0064] Considering again Figure 3, the pressure in the cuff **28** is at atmospheric pressure P_0 during the time interval between t_0 and t_1 . Also, during this same time interval the signal at detector **22** is a mean value V_N varying between the limits of $(V_N + \Delta)$ and $(V_N - \Delta)$

[0065] This mean voltage V_N results from the subtle flexing of the arterial walls and subsequent subtle movement of tissue underlying the fabric **16**. This subtle movement is due to the arterial pressure fluctuations from the systolic to the diastolic pressure extremes. Because blood flow is laminar and silent during this interval, the net average force on the arterial walls is constant. During the arbitrary time interval t_0 to t_1 , the voltage reading from detector **22** is sampled; and a voltage $V_N (+/-\Delta)$ is stored in memory of the processor **26**.

[0066] Next, at time t_1 , under control of the processor **26**, the valve **34** is closed and the pump **32** activated. Accordingly, during the time interval from t_1 to t_2 , the pressure in the cuff **28** rises to a pressure P_H , a pressure

value chosen to be above the highest expected systolic pressure (e.g. 300 to 330 mm Hg). This pressure value is also stored in memory of the processor 26. During this time interval, the brachial arterial blood flow becomes totally interrupted. Effectively, there is no arterial wall flexing or underlying body tissue movement because blood flow is occluded. As explained in connection with Figure 2C, the voltage output from the detector 22 rises to V_H .

[0067] During the time interval from t_1 to t_2 , the cuff pressure and detector voltage are sampled and stored at a fixed sampling frequency (chosen in a frequency range from ten (10) Hertz to ten thousand (10,000) Hertz). The voltage reading from detector 22 when the pressure in cuff 28 reaches its maximum value P_H (at time t_2 in Figure 3) is stored in processor 26.

[0068] At t_2 the pressure in the cuff 28 is released by opening valve 34 under control of the processor 26. During the time interval t_2 to t_3 the voltage output from detector 22 and the pressure in the cuff 28 are sampled and stored at the sampling frequency. During the interval t_2 to t_3 the rate of pressure change within the cuff 28 is about two (2) mm Hg to about six (6) mm Hg per second.

[0069] As the cuff pressure is reduced, at some time within the interval t_2 to t_3 , the pressure in the cuff 28 is equal to the systolic (highest) arterial blood pressure and the artery snaps open with a sudden flow of blood. In turn, as explained in connection with Figure 2D, the voltage at the detector 22 experiences a maximum in rate of change and falls to a maximum deviation from V_N to a voltage value V_L . As shown in Figure 3, this voltage V_L , detected at t_3 , corresponds to the sudden rush of arterial blood filling the formerly occluded artery with a sharp flexing of the artery walls. This sharp flexing of the walls in turn stimulates movement of the tissue overlying the artery and underlying the fabric 16. This movement corresponds to a maximum amplitude for the motion of the tissue underlying the fabric 16. At t_3 , corresponding to voltage V_L , this maximum amplitude in tissue movement forces maximum fabric 16 flexing, sudden elongation, signaling that a peak or systolic pressure P_s is present in the brachial artery.

[0070] During the interval of time t_3 to t_4 the pressure in the cuff 28 is further decreasing. The voltage and pressure values are sampled at the predetermined frequency. The voltage output at the detector 22 continues to rise during this time interval t_3 to t_4 .

[0071] Following the occurrence of the minimum voltage V_L , the output voltage of the detector again returns to within the predetermined range about the baseline value (within the limits $(V_N + \Delta)$ and $(V_N - \Delta)$) and the pressure in the cuff 20 passes through a point of equivalence with the diastolic (lowest) pressure in the brachial artery, uniquely defining t_4 . Any further drop in pressure in the cuff 28, to atmospheric pressure, produces no further rise in voltage at detector 22 during the time interval t_4 to t_1 .

[0072] The system and method of the present invention may alternatively be operated in a transmission mode

where the source 18 is disposed on side 16E of the fabric 16 while the detector 22 is disposed on the opposite side 16I. The dot-dashed outline of detector 22, shown in Figures 2A through 2D represents the location of detector 22 in transmission mode. The light balance between reflection and transmission will be the same as the situation discussed in connection with the reflection mode. However, the detector output voltage shown in Figure 2F is reversed since more fabric stretch results in higher light transmission providing a commensurately higher detector voltage. The detector voltage waveform shown in Figure 3 is therefore reversed or inverted as well. In contrast to the reflection mode shown in Figure 3, the transmission mode measures a decrease in voltage between the interval of time t_1 to t_2 and an increase between the interval of time t_2 to t_3 . Finally, in contrast to Figure 3 the detector voltage decreases between t_3 and t_4 to return to voltage V_N .

[0073] The measurement of pressures P_s and P_D is, in principle, determined by means of signal processing techniques known in the art. For example, one commercially available pressure transducer 36, Model 7277 from Advanced Custom Sensors, Inc. Irvine, California, 92618, is a miniature silicon pressure sensor package, with 0 to 5 volt output, and 0 to 0,048 MPa (0 to 7 pound per square inch) gage rating. This pressure transducer 36 will communicate directly with signal processor 26 such as a Z8[®] microcontroller, Model Z86C08 from ZILOG, Inc., Campbell, California, 95008-6600 with electronically programmable memory and associated circuitry.

[0074] Those skilled in the art, having the benefit of the teachings of the present invention as hereinabove set forth, may effect modifications thereto. Such modifications are to be construed as lying within the scope of the present invention, as defined by the appended claims.

Claims

1. A system (10) for monitoring blood pressure, comprising:

an inflatable arm cuff (28) that is selectably inflatable to differing air pressures;
 a patch (14) disposed in or on the arm cuff (28) comprising textile fabric (16) that has both a light transmission property and a light reflection property that change when the fabric (16) stretches;
 a radiation source (18) which directs radiation onto the textile fabric (16); and
 a radiation detector (22), wherein the reception of incident radiation by the detector (22) is directly affected by a change in the amount of light transmitted through the textile fabric (16) relative to the amount of light reflected by the textile fabric (16) as the textile fabric (16) stretches in

- response to motion in the wearer's body;
 wherein the textile fabric (16) has a first side and a second side and wherein the radiation source (18) and the radiation detector (22) are mounted on the same side or on opposite sides of the fabric (16).
2. The system of claim 1, wherein the radiation source (18) emits radiation with a wavelength in the range of from about 400 to about 2200 nanometers; and the detector (22) responds to incident radiation with a wavelength in the range of from about 400 to about 2200 nanometers.
 3. The system of claim 1, wherein the fabric (16) is attached to a surface of the cuff (28).
 4. The system of claim 1, wherein the fabric (16) is integral with the cuff (28).
 5. The system of claim 1, wherein the fabric (16) comprises reflective yarns and stretchable yarns.
 6. The system (10) of any of the claims 1 to 5 wherein the inflatable arm cuff (28) is sized for receipt over a portion of a wearer's body and wherein the cuff (28) is selectively inflatable to differing air pressures to modify the flow of blood through an artery located in the portion of the wearer's body over which the cuff (28) is disposed, wherein the amount of light transmitted through the textile fabric (16) relative to the amount of light reflected by the textile fabric (16) changes when the textile fabric (16) stretches in response to changes in blood flow through an artery disposed beneath the patch (14); wherein the source (18) and the detector (22) are attached to the fabric (16) in relative positions such that the reception of incident radiation by the detector (22) is directly affected by a change in the amount of light transmitted through the textile fabric (16) relative to the amount of light reflected by the textile fabric (16) as the textile fabric (16) stretches in response to motion in the wearer's body due to changes in the flow of blood through an artery disposed beneath the textile fabric (16) occurring in consonance with variations in the air pressure within the inflatable cuff (28); and a pressure recorder responsive to the signal output from the detector (22) for recording the pressure of the cuff (28) when the output of the detector (22) is at a minimum value, and for recording the pressure in the cuff (28) following the minimum value when the signal from the detector again lies within a predetermined range of a baseline signal value.
 7. A method for monitoring blood pressure, comprising the steps of:
 - inflating an inflatable cuff (28) disposed over a portion of a wearer's body over which the cuff (28) is disposed;
 - disposing within or over the inflatable cuff a textile fabric (16) which has both a light transmission property and a light reflection property and in which the amount of light transmitted through the textile fabric (16) relative to the light reflected by the fabric (16) changes when the textile fabric (16) stretches;
 - using a radiation source (18), illuminating the fabric (16) with radiation having wavelength (s) in the range of from about 400 to about 2200 nanometers;
 - detecting the amount of light reflected or transmitted by the textile fabric (16) with a radiation detector (22) responsive to incident radiation having wavelength (s) in the range of from about 400 to about 2200 nanometers, wherein the amount of light detected by the detector (22) is directly affected by a change in the amount of light transmitted through the textile fabric (16) relative to the amount of light reflected by the textile fabric (16) as the textile fabric (16) stretches in response to motion in the wearer's body; and
 - recording the pressure in the cuff (28) in response to the signal output from the detector (22).
 8. The method of claim 7, wherein recording the pressure comprises measuring the pressure in the cuff (28) when the output of the detector (22) is at a minimum value, and measuring the pressure in the cuff (28) when the signal from the detector (22) lies within a predetermined range of a baseline signal value.
 9. The method of claim 7, wherein the source (18) and the detector (22) are attached to the textile fabric (16) in relative positions such that the reception of incident radiation by the detector (22) is directly affected by a change in the amount of light transmitted through the textile fabric (16) relative to the amount of light reflected by the textile fabric (16) as the textile fabric (16) stretches in response to motion in the wearer's body due to changes in the flow of blood through an artery disposed beneath the fabric (16) occurring in consonance with variations in the air pressure within the inflatable cuff (28).
 10. The method of any of the claims 7 to 9, wherein inflating an inflatable cuff (28) comprises inflating to differing air pressures thereby to modify the flow of blood through an artery located in the portion of the wearer's body over which the cuff (28) is disposed; and further comprising the step of:
 - recording the pressure in the cuff (28) in response to the signal output from the detector

(22) when the output of the detector (22) is at a minimum value and recording the pressure in the cuff (28) following the minimum when the signal from the detector (22) again lies within a predetermined range of a baseline signal value.

Patentansprüche

1. System (10) zur Blutdrucküberwachung, aufweisend:

eine aufblasbare Armmanschette (28), welche wählbar auf verschiedene Luftdrücke aufblasbar ist;

eine in oder auf der Armmanschette (28) angebrachte Patte (14), welche textilen Stoff (16) aufweist, welcher sowohl eine Lichttransmissionseigenschaft, als auch eine Lichtreflexionseigenschaft aufweist, welche sich verändern, wenn der Stoff (16) gedehnt wird;

eine Strahlungsquelle (18), welche Strahlung auf den textilen Stoff (16) lenkt; und

einen Strahlungsdetektor (22), wobei der Empfang von eintreffender Strahlung durch den Detektor (22) direkt beeinflusst wird durch eine Veränderung der Lichtmenge, welche durch den textilen Stoff (16) transmittiert wird, relativ zur Lichtmenge, welche durch den textilen Stoff (16) reflektiert wird, während sich der textile Stoff (16) verursacht durch Bewegung des Körpers des Trägers dehnt;

wobei der textile Stoff (16) eine erste Seite und eine zweite Seite aufweist und wobei die Strahlungsquelle (18) und der Strahlungsdetektor (22) auf derselben Seite oder auf entgegengesetzten Seiten des Stoffes (16) angebracht sind.

2. System nach Anspruch 1, wobei die Strahlungsquelle (18) Strahlung mit einer Wellenlänge im Bereich von ungefähr 400 bis ungefähr 2200 Nanometer emittiert; und wobei der Detektor (22) für eintreffende Strahlung mit einer Wellenlänge im Bereich von ungefähr 400 bis ungefähr 2200 Nanometer empfindlich ist.

3. System nach Anspruch 1, wobei der Stoff (16) an einer Oberfläche der Manschette (28) angebracht ist.

4. System nach Anspruch 1, wobei der Stoff (16) und die Manschette (28) einstückig sind.

5. System nach Anspruch 1, wobei der Stoff (16) reflektierende und dehnbare Garne aufweist.

6. System (10) nach einem der Ansprüche 1 bis 5, wobei die aufblasbare Armmanschette (28) eine derar-

tige Größe aufweist, dass sie über einen Teil des Körpers eines Trägers gezogen werden kann und wobei die Manschette (28) wählbar auf verschiedene Luftdrücke aufgeblasen werden kann, um den Blutfluss durch eine Arterie zu verändern, welche sich in dem Bereich des Körpers des Trägers befindet, über welchem die Manschette (28) angebracht ist, wobei die Lichtmenge, welche durch den textilen Stoff (16) transmittiert wird, relativ zur Lichtmenge, welche von dem textilen Stoff (16) reflektiert wird, sich verändert, wenn sich der textile Stoff (16) dehnt verursacht durch Veränderungen des Blutflusses durch eine Arterie, welche unter der Patte (14) verläuft; wobei die Quelle (18) und der Detektor (22) an dem Stoff (16) so relativ zueinander angeordnet sind, dass der Empfang von eintreffender Strahlung durch den Detektor (22) direkt durch eine Veränderung der Lichtmenge beeinflusst wird, welche durch den textilen Stoff (16) transmittiert wird, relativ zur Lichtmenge, welche durch den textilen Stoff (16) reflektiert wird, wenn sich der textile Stoff (16) dehnt verursacht durch Bewegung des Körpers des Trägers durch Veränderungen im Blutfluss durch eine Arterie, welche unter dem textilen Stoff (16) verläuft, welche zusammen mit Variationen des Luftdrucks in der aufblasbaren Armmanschette auftreten; und einen Druckrekorder, welcher auf das durch den Detektor (22) ausgegebene Signal reagiert, zum Aufnehmen des Drucks der Manschette (28), wenn die Ausgabe des Detektors (22) einen minimalen Wert annimmt, und zum Aufnehmen des Drucks in der Manschette (28), welcher dem minimalen Wert folgt, wenn das Signal des Detektors wieder innerhalb eines vorbestimmten Bereichs eines Grundliniensignalwertes liegt.

7. Verfahren zur Blutdrucküberwachung, aufweisend die Schritte:

Aufblasen einer aufblasbaren Manschette (28), welche über einem Teil eines Körpers eines Trägers angeordnet ist, über welchem die Manschette (28) angeordnet ist;

Anordnen in oder über der aufblasbaren Manschette einen textilen Stoff (16), welcher sowohl eine Lichttransmissionseigenschaft, als auch eine Lichtreflexionseigenschaft aufweist, wobei die Lichtmenge, welche durch den textilen Stoff (16) transmittiert wird, relativ zum Licht, welches durch den textilen Stoff (16) reflektiert wird, sich verändert, wenn sich der Stoff (16) dehnt;

Verwenden einer Strahlungsquelle (18), Beleuchten des Stoffes (16) mit einer Strahlung, welche (eine) Wellenlänge(n) im Bereich von ungefähr 400 bis ungefähr 2200 Nanometer aufweist; Detektieren der Lichtmenge, welche durch den textilen Stoff (16) reflektiert oder transmittiert wird, mit einem Strahlungsdetektor (22), wel-

cher für eintreffende Strahlung mit (einer) Wellenlänge(n) im Bereich von ungefähr 400 bis ungefähr 2200 Nanometer empfindlich ist, wobei die Lichtmenge, welche durch den Detektor (22) detektiert wird, direkt beeinflusst wird durch eine Veränderung der Lichtmenge, welche durch den textilen Stoff (16) transmittiert wird, relativ zur Lichtmenge, welche durch den textilen Stoff (16) reflektiert wird, während sich der textile Stoff (16) verursacht durch Bewegung des Körpers des Trägers dehnt; und
Aufnehmen des Drucks in der Manschette (28) als Antwort auf das durch den Detektor (22) ausgegebene Signal.

8. Verfahren nach Anspruch 7, wobei das Aufnehmen des Drucks das Messen des Drucks in der Manschette (28) aufweist, wenn die Ausgabe des Detektors (22) bei einem minimalen Wert liegt, und Messen des Drucks in der Manschette (28), wenn das Signal des Detektors (22) innerhalb einer vorbestimmten Spanne eines Grundliniensignalwertes liegt.
9. Verfahren nach Anspruch 7, wobei die Quelle (18) und der Detektor (22) an dem textilen Stoff (16) relativ zueinander so angebracht sind, dass der Empfang von auftreffender Strahlung durch den Detektor (22) direkt beeinflusst wird durch eine Veränderung in der Lichtmenge, welche durch den textilen Stoff (16) transmittiert wird, relativ zur Lichtmenge, welche durch den textilen Stoff (16) reflektiert wird, wenn sich der textile Stoff (16) dehnt als Antwort auf Bewegung des Körpers des Trägers durch Veränderungen im Blutfluss durch eine Arterie, welche unter dem Stoff (16) verläuft, wobei die Veränderungen zusammen mit Variationen des Luftdrucks in der aufblasbaren Manschette (28) auftreten.
10. Verfahren nach einem der Ansprüche 7 bis 9, wobei das Aufblasen einer aufblasbaren Manschette (28) das Aufblasen auf verschiedene Luftdrücke aufweist, wodurch der Blutfluss durch eine Arterie in dem Abschnitt des Körpers des Trägers über welchem die Manschette (28) angeordnet ist, verändert wird; und weiter aufweisend den Schritt:

Aufnehmen des Drucks in der Manschette (28) als Antwort auf das Signal, welches von dem Detektor (22) ausgegeben wird, wenn die Ausgabe des Detektors (22) bei einem minimalen Wert ist und Aufnehmen des Drucks in der Manschette (28), welcher auf das Minimum folgt, wenn das Signal von dem Detektor (22) wieder in einem vorbestimmten Bereich eines Grundliniensignalwertes liegt.

Revendications

1. Un système (10) de surveillance de la pression sanguine, comprenant :
 - un manchon brassard gonflable (28) qui est gonflable sélectivement à différentes pressions d'air ;
 - une pièce (14) disposée à l'intérieur ou sur le manchon brassard (28) comprenant un textile tissé (16) qui présente à la fois une propriété de transmission de la lumière et une propriété de réflexion de la lumière qui varient lorsque le tissu (16) est étiré ;
 - une source de rayonnement (18) qui dirige du rayonnement sur le textile tissé (16) ; et
 - un détecteur de rayonnement (22), la réception de rayonnement incident par le détecteur (22) étant directement affectée par une modification de la quantité de lumière transmise au travers dudit textile tissé (16) par rapport à la quantité de lumière réfléchie par le textile tissé (16) lorsque le textile tissé (16) est étiré en réponse à un mouvement du corps du porteur ;
 - le textile tissé (16) présentant une première face et une seconde face et la source de rayonnement (18) et le détecteur de rayonnement (22) étant montés sur la même face ou sur des faces opposées du tissu (16).
2. Le système de la revendication 1, dans lequel la source de rayonnement (18) émet du rayonnement avec une longueur d'onde comprise dans la plage allant d'environ 400 à environ 2200 nanomètres ; et le détecteur (22) répond au rayonnement incident de longueur d'onde comprise dans la plage allant d'environ 400 à environ 2200 nanomètres.
3. Le système de la revendication 1, dans lequel ledit tissu (16) est solidarisé à une surface du manchon (28).
4. Le système de la revendication 1, dans lequel le tissu (16) fait partie intégrante du manchon (28).
5. Le système de la revendication 1, dans lequel le tissu comprend des fils réfléchissants et des fils étirables.
6. Le système (10) de l'une des revendications 1 à 5, dans lequel le manchon brassard gonflable (28) est dimensionné pour pouvoir être placé au-dessus d'une partie du corps d'un porteur et dans lequel le manchon (28) est sélectivement gonflable à des pressions d'air différentes pour modifier le flux sanguin dans une artère située dans la partie du corps du porteur au-dessus de laquelle est disposé le manchon (28), la quantité de lumière transmise au travers du textile tissé (16) par rapport à la quantité de

lumière réfléchi par le textile tissé (16) se modifiant lorsque le textile tissé (16) est étiré en réponse à des modifications du flux sanguin au travers d'une artère disposée au-dessous de la pièce (14) ; dans lequel la source (18) et le détecteur (22) sont solidarisés au tissu (16) dans des positions relatives telles que la réception de rayonnement incident par le détecteur (22) soit directement affectée par une modification de la quantité de lumière transmise au travers du textile tissé (16) par rapport à la quantité de lumière réfléchi par le textile tissé (16) lorsque le textile tissé (16) s'étire en réponse au déplacement du corps du porteur dû à des modifications du flux sanguin dans une artère située au-dessous du textile tissé (16) qui survient concomitamment avec des variations de la pression d'air à l'intérieur du manchon gonflable (28) ; et un enregistreur de pression sensible au signal délivré en sortie de détecteur (22) pour enregistrer la pression du manchon (28) lorsque la sortie du détecteur (22) est à une valeur minimale, et pour enregistrer la pression dans le manchon (28) qui suit la valeur minimale lorsque le signal provenant du détecteur se situe à nouveau à l'intérieur d'une plage prédéterminée d'une valeur de signal de ligne de base.

7. Un procédé de surveillance de la pression sanguine, comprenant les étapes suivantes :

le gonflage d'un manchon gonflable (18) disposé au-dessus d'une partie du corps d'un porteur au-dessus de laquelle est disposé le manchon (28) ;

la disposition à l'intérieur ou au-dessus du manchon gonflable d'un textile tissé (16) qui présente à la fois une propriété de transmission de la lumière et une propriété de réflexion de la lumière et dans lequel la quantité de lumière transmise au travers du textile tissé (16) par rapport à la lumière réfléchi par le tissu (16) change lorsque le textile tissé (16) s'étire ;

l'utilisation d'une source de rayonnement (18), illuminant le tissu (16) par un rayonnement présentant une ou des longueurs d'onde dans la plage allant d'environ 400 à environ 2200 nanomètres ;

la détection de la quantité de lumière réfléchi ou transmise par le textile tissé (16) par un détecteur de rayonnement (22) en réponse à un rayonnement incident présentant une ou des longueurs d'onde dans la plage allant d'environ 400 à environ 2200 nanomètres, la quantité de lumière détectée par le détecteur (22) étant directement affectée par une modification de la quantité de lumière transmise au travers du textile tissé (16) par rapport à la quantité de lumière réfléchi par le textile tissé (16) lorsque le textile

tissé (16) s'étire en réponse à un déplacement du corps du porteur ; et l'enregistrement de la pression dans le manchon (28) en réponse au signal délivré en sortie par le détecteur (22).

8. Le procédé de la revendication 7, dans lequel l'enregistrement de la pression comprend la mesure de la pression dans le manchon (28) lorsque la sortie du détecteur (22) est à une valeur minimale, et la mesure de la pression dans le manchon (28) lorsque le signal en provenance du détecteur (22) se situe à l'intérieur d'une plage prédéterminée d'une valeur de signal de ligne de base.

9. Le procédé de la revendication 7, dans lequel la source (18) et le détecteur (22) sont solidarisés au textile tissé (16) en des positions relatives telles que la réception de rayonnement incident par le détecteur (22) soit directement affectée par une modification de la quantité de lumière transmise au travers du textile tissé (16) par rapport à la quantité de lumière réfléchi par le textile tissé (16) lorsque le textile tissé (16) s'étire en réponse à un déplacement du corps du porteur dû à des modifications du débit sanguin dans une artère située au-dessous du tissu (16) survenant concomitamment avec des variations de la pression d'air à l'intérieur du manchon gonflable (28).

10. Le procédé de l'une des revendications 7 à 9, dans lequel le gonflage d'un manchon gonflable (28) comprend le gonflage à différentes pressions d'air afin de modifier ainsi le débit sanguin dans une artère située dans la partie du corps du porteur au-dessus de laquelle est disposé le manchon (28) ; et comprenant en outre l'étape suivante :

l'enregistrement de la pression dans le manchon (28) en réponse au signal délivré en sortie par le détecteur (22) lorsque la sortie du détecteur (22) est à une valeur minimale et l'enregistrement de la pression dans le manchon (28) après le minimum lorsque le signal en provenance du détecteur (22) se situe à nouveau à l'intérieur d'une plage prédéterminée d'une valeur de signal de ligne de base.

Figure 1.

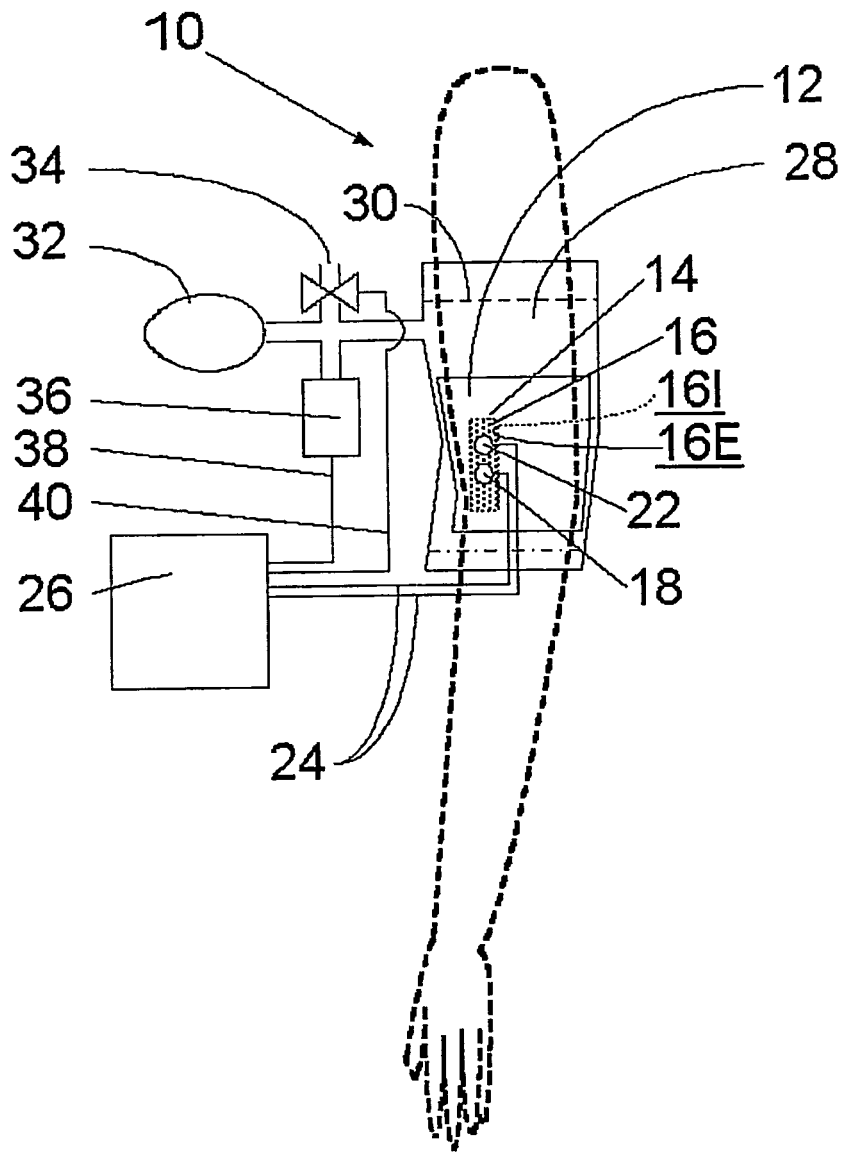


Figure 2A

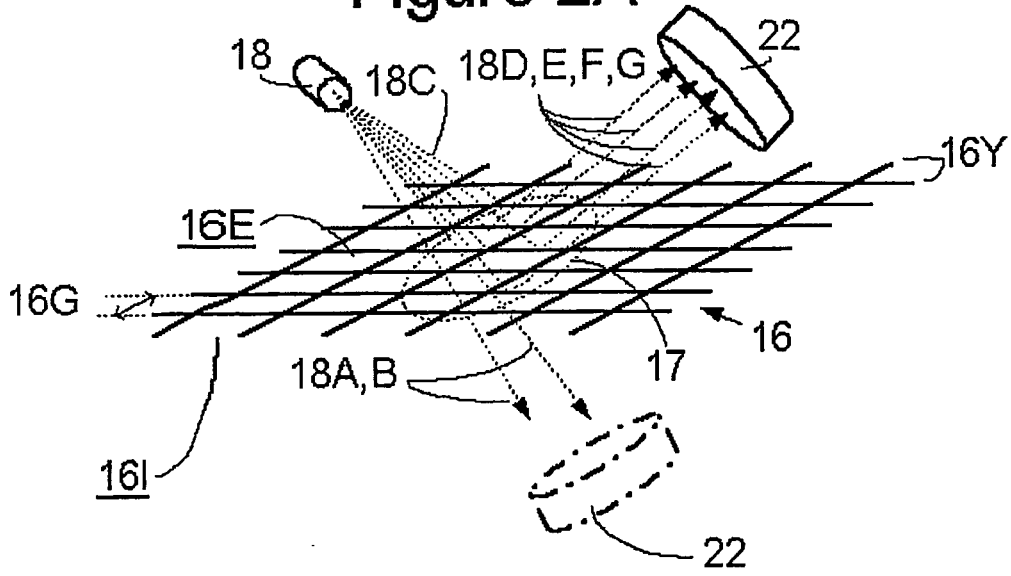


Figure 2B

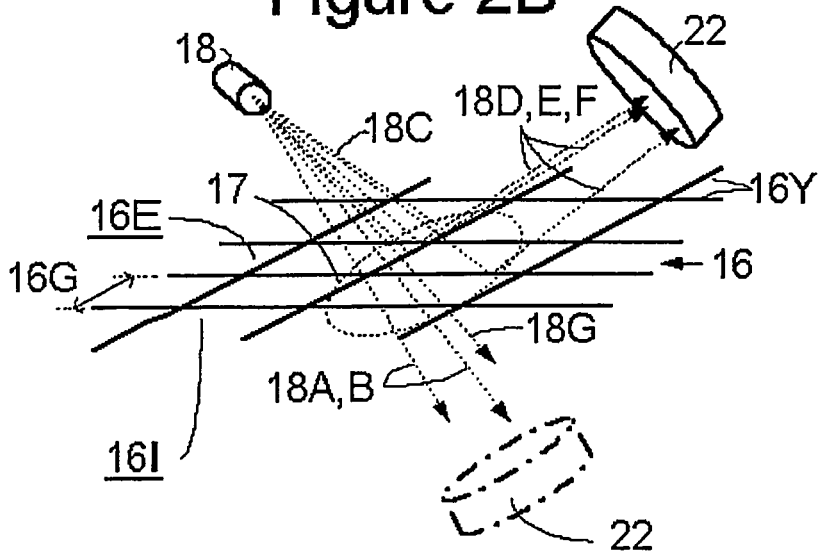


Figure 2C

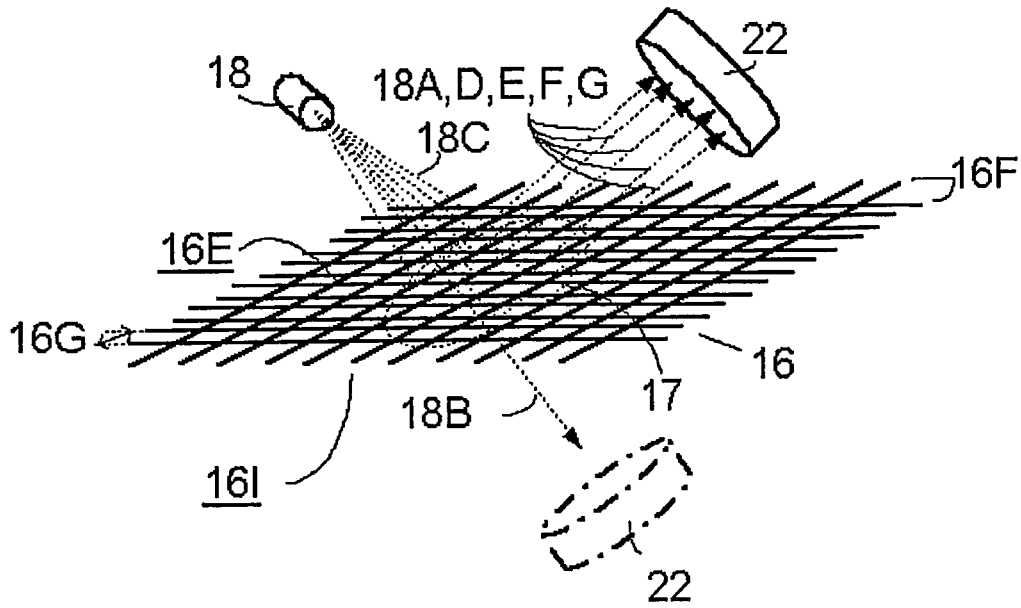


Figure 2D

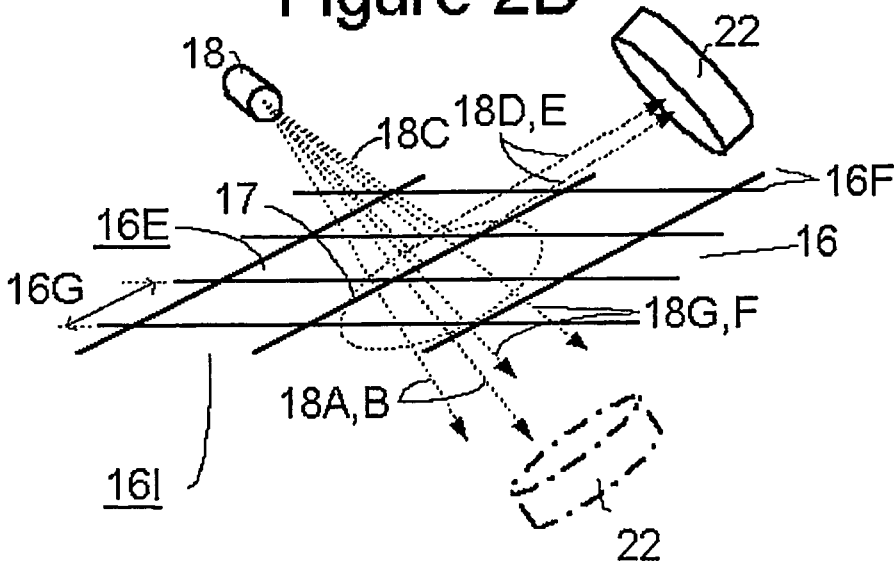


Figure 2E.

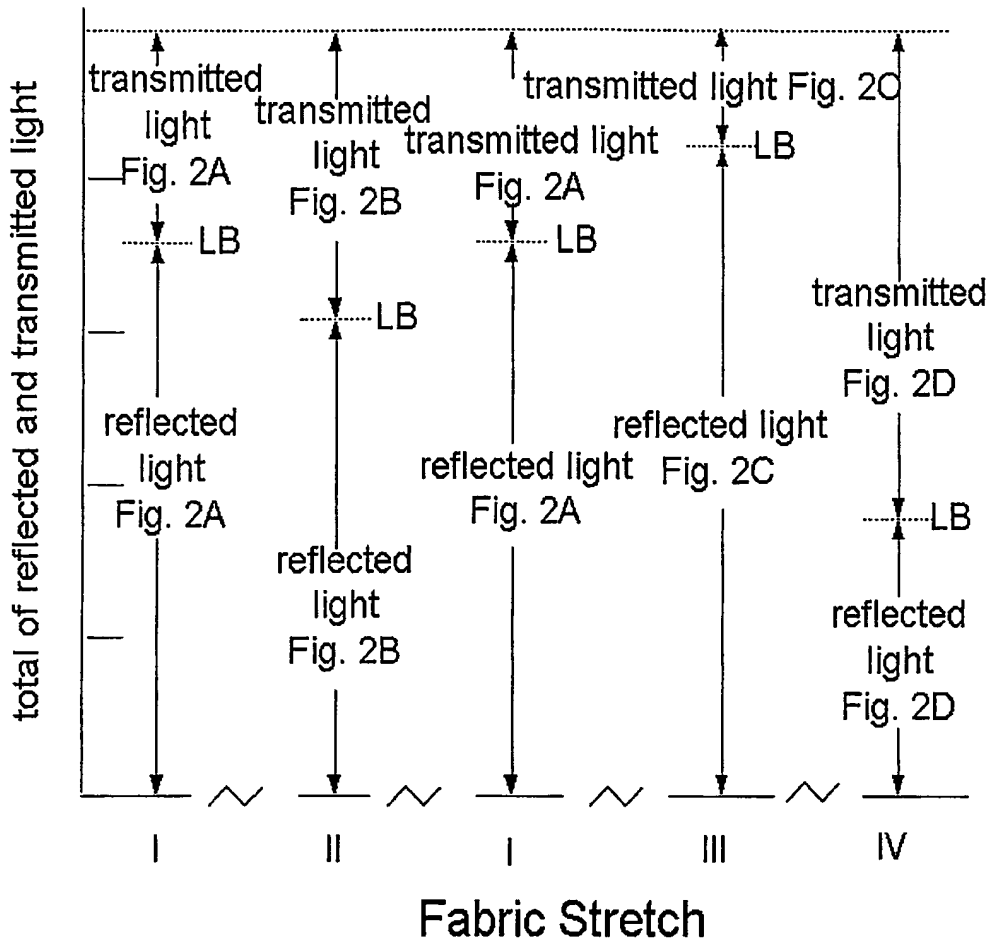


Figure 2F


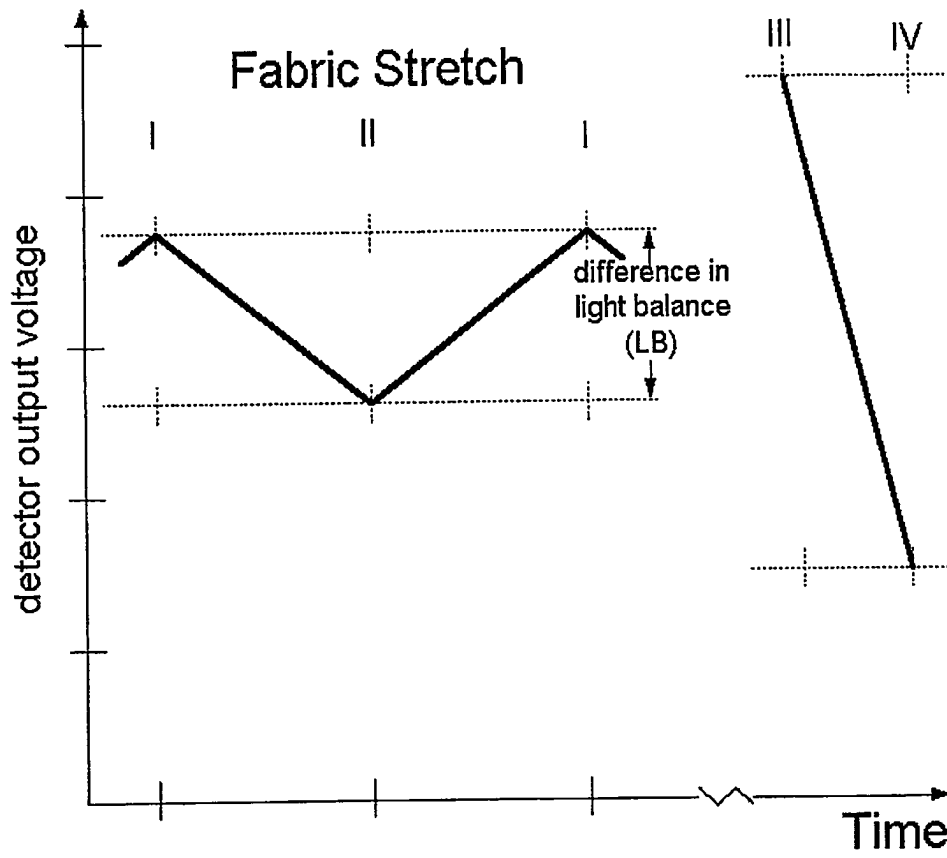


Figure 3.

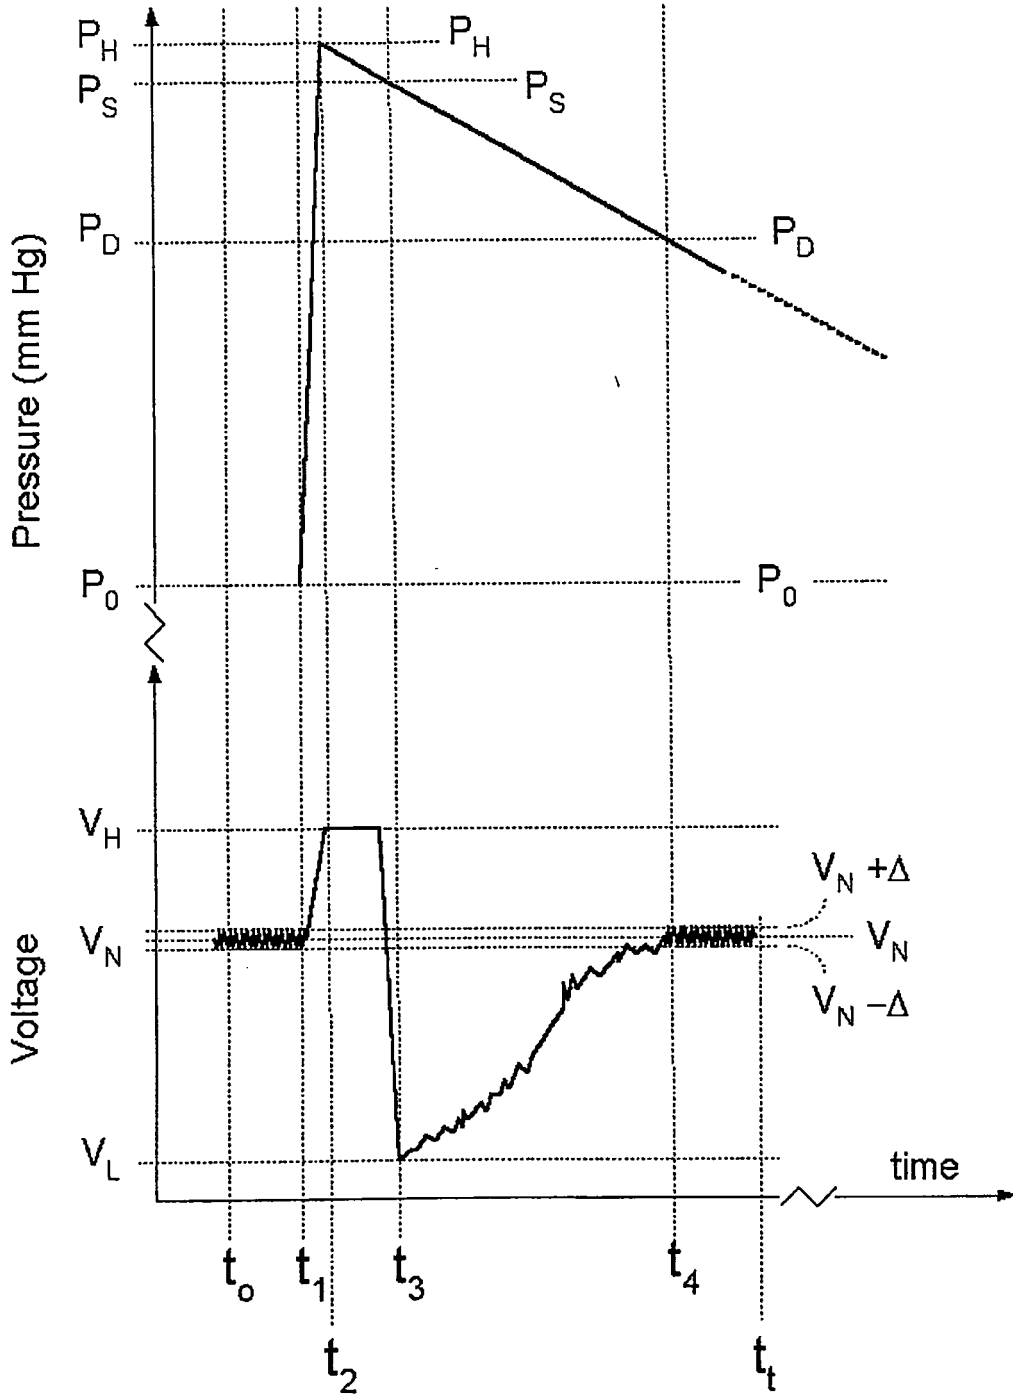

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6511435 B, Bluth [0007] [0008]
- US 6458085 B, VVu [0008]
- EP 0847724 A1 [0010]
- US 3517999 A [0011]
- US 2003095263 A [0012]

专利名称(译)	血压监测系统和方法		
公开(公告)号	EP1662985B1	公开(公告)日	2013-05-22
申请号	EP2004788709	申请日	2004-09-10
[标]申请(专利权)人(译)	因温斯特技术公司		
申请(专利权)人(译)	英威达科技S.A.R.L.		
当前申请(专利权)人(译)	TEXTRONICS INC.		
[标]发明人	COULSTON GEORGE W MICKA THOMAS A		
发明人	COULSTON, GEORGE, W. MICKA, THOMAS, A.		
IPC分类号	A61B5/00 A61B5/024 A41D13/12 A61B5/02 A61B5/022 A61B5/11 A61B5/113 D04B1/14 G01L1/24		
CPC分类号	A41D13/1281 A61B5/022 A61B5/02233 A61B5/02416 A61B5/02438 A61B5/02444 A61B5/1126 A61B5/1128 A61B5/1135 A61B5/6804 A61B5/6805 D04B1/14 D10B2403/02431 Y10T442/30 Y10T442/3008 Y10T442/3024 Y10T442/3382 Y10T442/3976 Y10T442/40 Y10T442/413		
优先权	60/526188 2003-12-02 US 60/526187 2003-12-02 US 60/526429 2003-12-02 US 60/502751 2003-09-12 US 60/502750 2003-09-12 US 60/502760 2003-09-12 US		
其他公开文献	EP1662985A1		
外部链接	Espacenet		

摘要(译)

一种用于监测穿着者的血压的系统和方法具有可充气的袖带，该袖带可选择地对不同的气压进行充气，当使用具有波长的光照射织物时，所述气囊包括具有透光性和光反射性的织物。) 在约400至约2200纳米的范围内。辐射源和检测器在相对位置附着到织物上，使得检测器对入射辐射的接收直接受到透过织物的光量相对于织物反射的光量的变化的影响。由于血液流过布置在织物下方的动脉的变化，织物随着可充气袖带内的气压变化而发生，以响应穿着者身体的运动而伸展。

