

(19)



(11)

EP 2 275 021 A2

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
19.01.2011 Bulletin 2011/03

(51) Int Cl.:
A61B 5/00 (2006.01)

(21) Application number: **10010975.0**

(22) Date of filing: **24.06.2004**

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR

• **Mannheimer, Paul, D.**
Danville, CA 94506 (US)

(30) Priority: **25.06.2003 US 606668**

(74) Representative: **Kinsler, Maureen Catherine et al**
Marks & Clerk LLP
Aurora
120 Bothwell Street
Glasgow
G2 7JS (GB)

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
04756238.4 / 1 635 701

(71) Applicant: **Nellcor Puritan Bennett LLC**
North Haven, CT 06473 (US)

Remarks:

This application was filed on 28-09-2010 as a divisional application to the application mentioned under INID code 62.

(72) Inventors:
• **Hannula, Dan**
San Luis Obispo, CA 93401 (US)

(54) **A pulse oximetry sensor adapted for use on a patient's forehead**

(57) A pulse oximetry sensor adapted for use on a patient's forehead comprising:

a resilient substrate conformable to a patient's forehead; an emitter disposed on the substrate; and a detector disposed on the substrate.

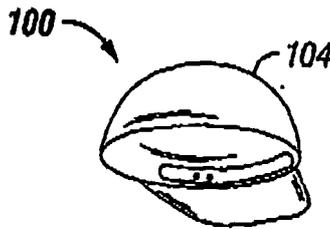


FIG. 1A

EP 2 275 021 A2

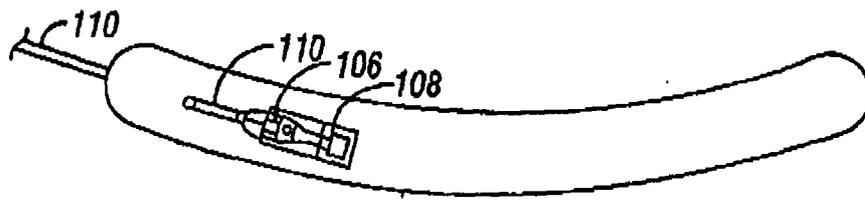


FIG. 1B

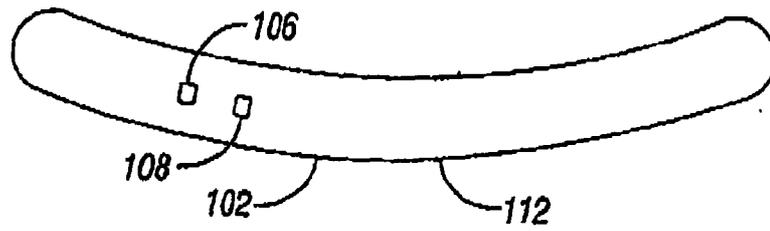


FIG. 1C

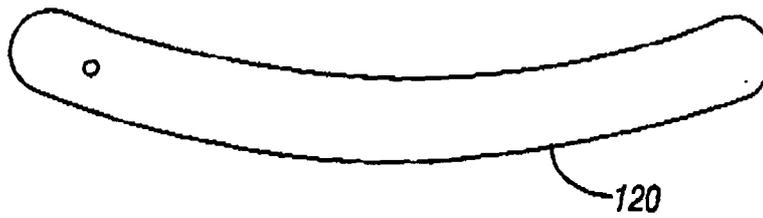


FIG. 1D

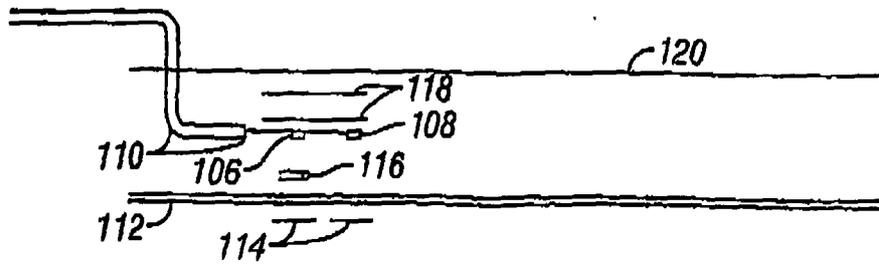


FIG. 1E

Description

[0001] The present invention relates to optical oximeter sensors, and in particular to hat-based pulse oximeter sensors.

[0002] Many types of optical sensors are used to measure physiological characteristics of a patient. Typically, an optical sensor provides emitted light which is then scattered through a portion of a patient's tissue and detected. Various characteristics of a patient can be determined from analyzing such light, such as oxygen saturation, pulse rate, tissue bilirubin, etc.

[0003] Pulse oximetry is typically used to measure various blood flow characteristics including, but not limited to, the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and the rate of blood pulsations corresponding to each heartbeat of a patient. Measurement of these characteristics has been accomplished by use of a non-invasive sensor which scatters light through a portion of the patient's tissue where blood perfuses the tissue, and photoelectrically senses the absorption of light in such tissue. The amount of light absorbed is then used to calculate the amount of blood constituent being measured.

[0004] The light scattered through the tissue is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of transmitted light scattered through the tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption. For measuring blood oxygen level, such sensors have typically been provided with a light source that is adapted to generate light of at least two different wavelengths, and with photodetectors sensitive to both of those wavelengths, in accordance with known techniques for measuring blood oxygen saturation.

[0005] Known non-invasive sensors include devices that are secured to a portion of the body, such as a finger, an ear or the scalp. In animals and humans, the tissue of these body portions is perfused with blood and the tissue surface is readily accessible to the sensor.

[0006] Certain types of oximeter sensors are applied to a patient's forehead. To aid in the sensor's proper placement and the proper application of pressure by the sensor to the forehead site, some forehead sensors are maintained at the forehead site by either the assistance of an adhesive layer and/or a headband. While these approaches are helpful, there is still a need for an improved and easy way of placing, retaining, and locating the sensor on the forehead of its user.

BRIEF SUMMARY OF THE INVENTION

[0007] The present invention provides an oximeter sensor which will attach to a patient's forehead in an improved manner. In certain embodiments, the securing of

the sensor to the forehead of the patient is achieved by attaching the sensor to the inside of hat which is worn by the patient when the sensor is in use.

[0008] In one embodiment, the present invention is an oximeter sensor, having: a substrate having a shape similar to a shape of at least a portion of a patient's forehead and including a section adapted to substantially fit over a portion of a forehead of a patient; an emitter disposed on the substrate at a position located on the section; and a detector disposed on the substrate at a distance from the emitter.

[0009] In one embodiment, the substrate is resilient and has a shape conformable to the forehead of a patient.

[0010] In one embodiment, the substrate includes an adhesive layer for adhering to the forehead of a patient.

[0011] In one embodiment, a hat is used for holding the sensor against the patient's forehead.

[0012] In one embodiment, the substrate is adhered to the inside of said hat.

[0013] In one embodiment, the substrate is adhesively attached to the inside of the hat. Alternately, the substrate is sewn into the hat.

[0014] In another embodiment, the present invention provides a method for determination of a blood characteristic, including: applying an emitter and a detector to spaced-apart positions on a forehead of a patient in the lower forehead region, above the eyebrow, with both the detector and the emitter placed above and predominantly lateral of the iris; securing the emitter and detector to the patient; emitting electromagnetic radiation with the emitter; detecting electromagnetic radiation scattered by the tissues of the forehead by the detector and producing a detector signal; and determining a blood characteristic in the patient from the detector signal.

[0015] In one embodiment, the securing of the emitter and the detector to the patient's forehead is achieved by attaching the emitter and the detector to an inside of a hat, and placing the hat on the head of the patient.

[0016] For a further understanding of the nature and advantages of the present invention, reference should be made to the following description in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] Fig. 1 is an assembly drawing of an embodiment of the sensor in accordance with the present invention that can be placed within a hat or cap.

[0018] Fig. 2 is a drawing of a stocking hat, with an embodiment of the sensor in accordance with the present invention shown mounted in the hat.

[0019] Fig. 3 is an assembly drawing of an embodiment of the sensor of Figs. 1 or 2.

DETAILED DESCRIPTION OF THE INVENTION

[0020] The embodiments of the present invention are directed towards configuring a reflectance-type oximeter

sensor for placement in a hat in order to provide a relatively easy means of placing, retaining, and locating the sensor on the forehead of the user. With regard to the location of the sensor on the patient's forehead, it is preferred to have the sensor be located on the lower forehead region, above the eyebrow, with the sensor optics (emitter and detector) located above and predominantly lateral to or centered over the iris. The oximeter sensor can be attached to the inside band of a hat. The precise location of the reflectance sensor in the hat allows appropriate placement of the sensor in the optimal forehead location by a user not skilled in sensor placement. It has been found that the placement of a reflectance forehead sensor is a factor in the accurate determination of a blood flow characteristic, due to the vasculature of the forehead. In addition, it has been shown that having a certain amount of pressure on the forehead sensor can reduce the incidence of venous pulsations effects on the oximeter reading. The placement of the sensor in the band of the hat would minimize these issues, as the placement of a hat is fairly repeatable and predictable. A hat-based oximeter sensor as embodied by the present invention can be used on patients in clinical settings, or by athletes, soldiers, firemen, or in any environment where information related to a physiological parameter, such as heart rate or oxygen saturation information is desired.

[0021] Fig. 1 is an assembly drawing of an embodiment of the sensor in accordance with the present invention that can be placed within a hat or cap. This figure shows an oximeter sensor placed on a substrate 102 that can be placed or adhered to the inside of a hat 104. In the hat-based embodiment, the sensor uses an emitter 106 containing two discrete wavelengths and a detector 108 placed more than 2 mm away, and ideally 10mm - 15mm from the emitter. The surface 102 can be black in order to minimize any shunting of light between sensor and patient skin. The sensor in a hat could be used in conjunction with a small, portable oximeter to allow mobility of the user during activities. Similarly, the sensor could be incorporated into a headband. Alternately, it may be desirable to provide a sensor with adhesive backing that would allow the user to place the sensor in a hat of their choice. Also shown in Fig. 1 is a cable 110 for providing drive current to the LED and for providing the detector signal to the oximeter. The cable provides the electrical connection to the monitor; it also provides power for the emitter, signal carrying conductors from the detector, and shielding to protect the small signals from the detector against external electrical interference.

[0022] The sensor is shown in a multi-layer structure having a face portion 112. The face 112 is the surface that is placed against the patient's skin. The face material may have an adhesive layer such as an acrylic or synthetic rubber adhesive, or it may be without adhesive, and typically made from a foam PVC or foam polyurethane material. The face 112 component is preferably black so as to minimize the incidence of reflected light that does not go through the tissue. Below the face layer

112 are two windows 114. The windows 114 are generally a clear component, such as for example, a thin film or a clear molded plastic component that makes contact with the skin. The thin film window may be a polyurethane or an acrylic adhesive on a polyester film. The intent of the window 114 is to provide an efficient optical coupling mechanism between the optical components (emitter and detector) and the skin. Located above the face 114, is a Faraday shield 116. The Faraday shield 116 is a conductive material, for example, a copper film or copper mesh, that is electrically connected to the monitor ground to help shield the detector from extraneous electrical interference while passing light to the detector. Next located are the LED 106 and the detector 108. Above the LED and the detector is a mask layer, which may include more than one mask layer. The mask layer 118 is generally a thin film that is intended to block light from entering the back side of the sensor, or from traveling directly from emitter to detector (shunt light). The purpose of the mask 118 is to ensure that all of the light reaching the detector is light from the emitter that has traveled through the capillary bed. Above the mask layer 118 is the back layer 120. The back or the top layer is the non-tissue contacting surface of the sensor. This layer may include a cosmetic finish for the sensor, which can be white with some printed artwork identifying the sensor. Typical materials may be Velcro loop, or soft PVC foam. In a case where the sensor is mounted inside a hat or cap, the top layer is sometimes referred to as the back layer. In this case, the back layer may include a double stick adhesive so that it can be mounted inside the hat.

[0023] Fig. 2 shows a stocking hat, with an embodiment of the sensor in accordance with the present invention shown mounted in the hat. This alternate embodiment of the present invention, is directed towards the placement of a small reflectance sensor 202 in a stocking cap or beanie 204. Fig. 2 shows the sensor carrier layer 202 holding an LED 206 and a detector 208 and a cable 210, similar to the ones described above in conjunction with Fig. 1. This embodiment may be used for neonates. This embodiment would allow easy placement of a sensor on the forehead of a patient while applying a predictable pressure on the sensor. The sensor in a hat also resolves a concern about the cosmetic appearance of having a sensor on the forehead of the patient. A sensor in a stocking cap is much more acceptable to a parent than having a sensor located on the forehead. Depending on the tension of the stocking cap, provided by its own stretchiness or by an adjustable integral headband strap, the sensor may have a light tack adhesive, or no adhesive at all. The lack of an adhesive layer is a desirable feature, especially on neonates as adhesives may sometimes leave visible damage to the fragile skin of a neonate.

[0024] Fig. 3 is an assembly drawing for an embodiment of the sensor of Figs. 1 or 2. Fig. 3 shows that the sensor portion generally includes a face layer 302, a top layer 304 and a flex circuit 306 that is placed between the face and top layers. Also shown in Fig. 3 is a multi-

layer unassembled view showing the relative positions of the face 302, flex circuit 306, a cable 308 and the top layer 304. The flex circuit layer 306 holds the emitter (LED) 310 and the detector 312 as well as the mask layer 314 and Faraday shield as described above. The flex circuit 306 also has several holes 316 to allow for electrical connections between the leads in the cable and the LED and the detector.

[0025] As will be understood by those skilled in the art, the present invention may be embodied in other specific forms without departing from the essential characteristics thereof. For example, the sensor may include adhesive layers for adhering to the inside of a hat or the user's skin, or that that the sensor may be sewn into the hat. These other embodiments are intended to be included within the scope of the present invention, which is set forth in the following claims.

[0026] The following clauses are included and form part of this description:

Clause 1. An oximeter sensor, comprising:

a substrate having a shape similar to a shape of at least a portion of a patient's forehead and including a section adapted to substantially fit over a portion of a forehead of a patient;
an emitter disposed on said substrate at a position located on said section; and a detector disposed on said substrate at a distance from said emitter.

Clause 2. The sensor of clause 1 wherein said substrate is resilient and has a shape conformable to the forehead of a patient.

Clause 3. The sensor of clause 1 wherein said substrate comprises an adhesive layer for adhering to the forehead of a patient.

Clause 4. The sensor of clause 1 wherein said substrate comprises a darkened layer so as to minimize the incidence of reflected light that does not go through the tissue of a patient onto said detector.

Clause 5. The sensor of clause 1 further comprising leads connected to said emitter and said detector, said leads extending along said substrate away from one of the top or a side of a patient's forehead.

Clause 6. The sensor of clause 1 further comprising a hat for holding said substrate against the patient's forehead.

Clause 7. The sensor of clause 6 wherein said substrate is adhered to the inside of said hat.

Clause 8. The sensor of clause 7 wherein said substrate is adhesively adhered to the inside of said hat.

Clause 9. The sensor of clause 1 wherein said substrate comprises a plurality of laminated layers.

Clause 10. An oximeter sensor, comprising:

a substrate having a shape similar to a shape of at least a portion of a patient's forehead and including a section adapted to substantially fit over a portion of a forehead of a patient;

an emitter disposed on said substrate at a position located on said section;
a detector disposed on said substrate at a distance from said emitter; and a hat for holding said substrate against the patient's forehead.

Clause 11. A method for determination of a blood characteristic, comprising: applying an emitter and a detector to spaced-apart positions on a forehead of a patient in the lower forehead region, above the eyebrow, with both the detector and the emitter placed lateral of the iris;
securing said emitter and detector to said patient;
emitting electromagnetic radiation with said emitter;
detecting electromagnetic radiation scattered by the forehead by said detector and producing a detector signal; and
determining a blood characteristic in the patient from said detector signal.

Clause 12. The method of clause 11 wherein said blood characteristic is oxygen saturation.

Clause 13. The method of clause 11 wherein said securing comprises placing a hat over said emitter and said detector.

Clause 14. The method of clause 11 wherein said securing comprises securing said emitter and said detector to the patient by attaching said emitter and said detector to an inside of a hat, and placing said hat on the head of the patient.

Clause 15. The method of clause 11 comprising detecting light reflected from the forehead of the patient with said detector.

Clause 16. A method for determination of a blood characteristic, comprising: applying an emitter and a detector to spaced-apart positions on a forehead of a patient in the lower forehead region, above the eyebrow, with both the detector and the emitter placed lateral of the iris;
securing said emitter and detector to said patient, by attaching said emitter and said detector to an inside of a hat, and placing said hat on the head of the patient; emitting electromagnetic radiation with said

emitter;
 detecting electromagnetic radiation scattered by the forehead by said detector and producing a detector signal; and
 determining a blood characteristic in the patient from said detector signal.

Clause 17. The method of clause 16 wherein said blood characteristic is oxygen saturation.

Claims

1. A pulse oximetry sensor adapted for use on a patient's forehead comprising:

a resilient substrate conformable to a patient's forehead, wherein the substrate is arcuate; an emitter disposed on the substrate; and a detector disposed on the substrate.

2. The sensor of claim 1 wherein the detector is placed more than 2 mm from the emitter, preferably 10mm-15mm.

3. The sensor of any of the preceding claims wherein the resilient substrate is black.

4. The sensor of any of the preceding claims comprising a cable on the resilient substrate.

5. The sensor of any of the preceding claims comprising a face portion that is placed against the patient's skin, optionally wherein the face portion comprises an adhesive layer adapted to contact the patient's forehead and/or wherein the face portion is black.

6. The sensor of any of the preceding claims comprising a Faraday shield electrically connected to ground.

7. The sensor of any of the preceding claims comprising a mask layer for blocking light from entering a back side of the sensor to ensure that all light reaching the detector is light from the emitter that has travelled through the patient.

8. The sensor of claim 9 comprising a back non-tissue contacting surface adjacent the mask layer, optionally wherein the non-tissue contacting surface of the sensor has a double stick adhesive so that it can be mounted inside a hat.

9. A hat that includes a sensor according to any of the preceding claims.

10. A hat as claimed in claim 9 wherein the sensor is positioned on the hat, preferably on an inside band

of the hat, so that when the hat is worn, the sensor is positioned on the patient's forehead and pressure is applied to the sensor to reduce the incidence of venous pulsations effects on the oximeter reading.

11. A hat as claimed in claim 9 or claim 10, wherein the sensor is positioned on the hat so that when the hat is worn the sensor is positioned on the lower forehead region, above the eyebrow, with the emitter and detector located above and lateral to or centered over the iris

12. A method of manufacturing a pulse oximetry sensor comprising:

providing a resilient substrate conformable to a patient's forehead, wherein the substrate is arcuate; providing an emitter disposed on a substrate; and
 providing a detector disposed on the substrate.

13. The method of claim 12 comprising providing the substrate having an adhesive layer adapted to contact the patient's forehead.

14. The method of claim 12, comprising providing a cable disposed on the substrate.

15. The system or hat or method of any of the preceding claims, wherein the emitter comprises at least one light emitting diode and/or the detector comprises at least one photodetector.

16. A method for determination of a blood characteristic, including: applying an emitter and a detector to spaced-apart positions on a forehead of a patient in the lower forehead region, above the eyebrow, with both the detector and the emitter placed above and predominantly lateral of the iris; securing the emitter and detector to the patient; emitting electromagnetic radiation with the emitter; detecting electromagnetic radiation scattered by the tissues of the forehead by the detector and producing a detector signal; and determining a blood characteristic in the patient from the detector signal.

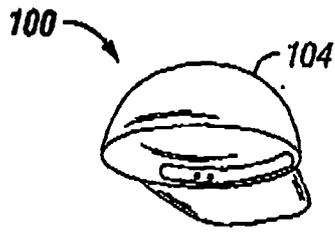


FIG. 1A

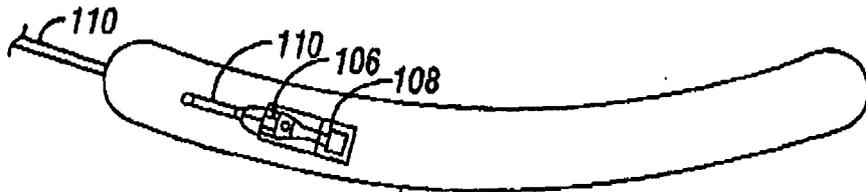


FIG. 1B

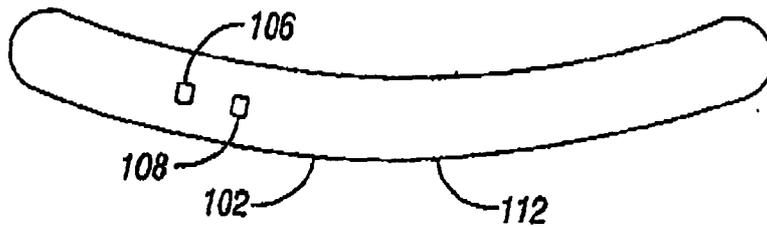


FIG. 1C

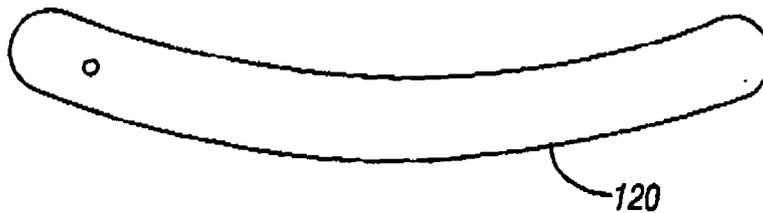


FIG. 1D

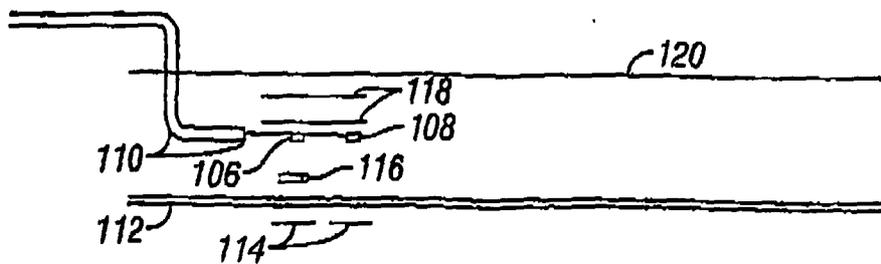


FIG. 1E

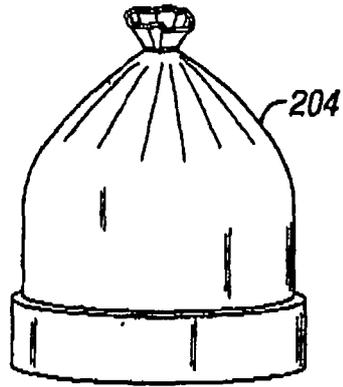


FIG. 2A




FIG. 2B

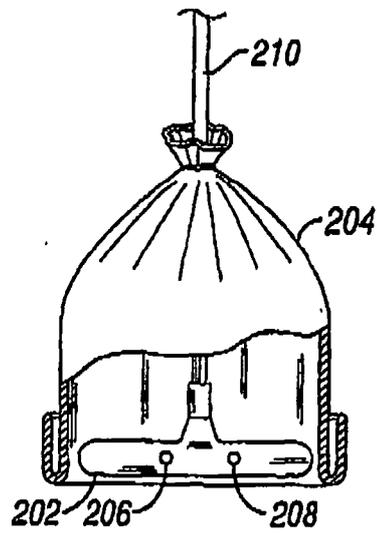


FIG. 2C

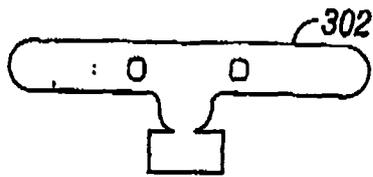


FIG. 3A

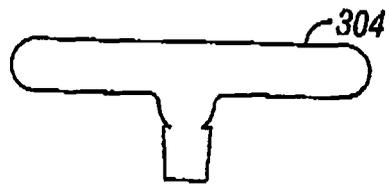


FIG. 3B

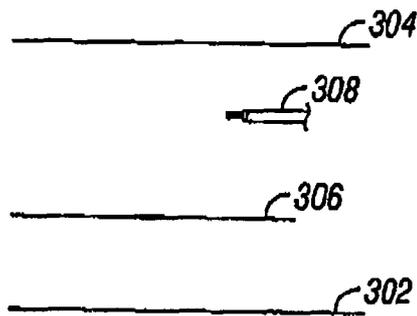


FIG. 3C



FIG. 3D

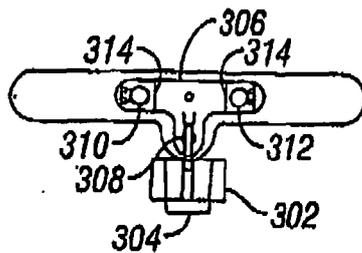


FIG. 3E




FIG. 3F

专利名称(译)	脉搏血氧饱和度传感器，适用于患者的前额		
公开(公告)号	EP2275021A2	公开(公告)日	2011-01-19
申请号	EP2010010975	申请日	2004-06-24
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
当前申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
[标]发明人	HANNULA DAN MANNHEIMER PAUL D		
发明人	HANNULA, DAN MANNHEIMER, PAUL, D.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/6833 A61B5/14552 A61B5/14553 A61B5/6804 A61B5/6814 A61B2503/06		
优先权	10/606668 2003-06-25 US		
其他公开文献	EP2275021A3		
外部链接	Espacenet		

摘要(译)

一种适用于患者前额的脉搏血氧饱和度传感器，包括：适合患者前额的弹性基底；发射极设置在基板上；和设置在基板上的检测器。

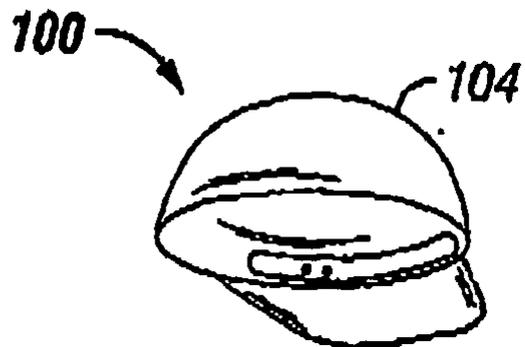


FIG. 1A