



(11) **EP 2 903 509 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**04.09.2019 Bulletin 2019/36**

(21) Application number: **13843561.5**

(22) Date of filing: **07.10.2013**

(51) Int Cl.:  
**A61B 5/0402** <sup>(2006.01)</sup> **A61B 5/00** <sup>(2006.01)</sup>  
**A61B 5/0205** <sup>(2006.01)</sup> **A61B 5/0408** <sup>(2006.01)</sup>  
**A61B 5/0432** <sup>(2006.01)</sup> **A61B 5/1455** <sup>(2006.01)</sup>  
**A61B 5/024** <sup>(2006.01)</sup> **A61B 5/11** <sup>(2006.01)</sup>  
**A61B 5/0456** <sup>(2006.01)</sup>

(86) International application number:  
**PCT/US2013/063748**

(87) International publication number:  
**WO 2014/055994 (10.04.2014 Gazette 2014/15)**

(54) **WEARABLE CARDIAC MONITOR**

TRAGBARER HERZMONITOR

MONITEUR CARDIAQUE INTÉGRÉ DANS UN VÊTEMENT

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

(30) Priority: **07.10.2012 US 201261710768 P**  
**15.03.2013 US 201313837748**

(43) Date of publication of application:  
**12.08.2015 Bulletin 2015/33**

(73) Proprietor: **Rhythm Diagnostic Systems Inc.**  
**San Francisco, California 94118 (US)**

(72) Inventors:  
• **GOLDA, George Stefan**  
**El Granada, California 94018 (US)**  
• **MOYER, Daniel Van Zandt**  
**Menlo Park, California 94025 (US)**

- **MARRIOTT, Mark P.**  
**Palo Alto, California 94301 (US)**
- **ELETR, Sam**  
**Kensington, California 94707 (US)**
- **O'NEIL, Bruce**  
**San Francisco, California 94115 (US)**

(74) Representative: **ZBM Patents - Zea, Barlocchi & Markvardsen**  
**Plaza Catalunya, 1**  
**08002 Barcelona (ES)**

(56) References cited:  
**EP-A2- 2 438 851** **CN-U- 202 288 274**  
**US-A- 5 184 620** **US-A1- 2006 224 072**  
**US-A1- 2006 224 072** **US-A1- 2007 191 728**  
**US-A1- 2008 139 953** **US-A1- 2012 232 369**  
**US-B1- 6 453 186**

**EP 2 903 509 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description****BACKGROUND**

5 **[0001]** Advances in electronics, sensor technology and materials science have revolutionized patient monitoring technologies. In particular, many light and wearable devices are becoming available for a variety of cardiac monitoring applications. However, improvements may yet be desired for robust wearable devices that provide effective data collection, in some cases also with increased patient convenience and comfort. Other alternatives may include developments in one or more of device attachment, size, flexibility, data transfer, among others.

10 **[0002]** Further alternatives for cardiac patients and their physicians may then include robust and convenient personal cardiac monitors that in some instances may collect and transfer long-term data as well as monitor events in real-time. Document US2008139953 discloses a body worn patient monitoring device that includes at least one module including a plurality of electrical connections to the body.

15 Document US2006224072 describes a disposable sensor patch for non-invasive monitoring and recording of infrequent cardiac events.

Document CN202288274 discloses a physiological signal monitoring system that comprises at least one physiological signal monitoring device, at least one mobile communication device and at least one background processing center server.

**SUMMARY**

20 **[0003]** Described herein are several medical monitoring devices and systems, in some instances for long-term sensing and/or recording of cardiac and/or respiratory data of an individual, such as a neonate, athlete, or cardiac patient. A number of alternative implementations and applications are summarized and/or exemplified herein below and throughout this specification.

25 **[0004]** In one aspect, the developments hereof include a wearable device for monitoring a plurality of physiological parameters of an individual from time-concordant measurements collected by a plurality of sensor, including but not limited to, electrodes for measuring ionic potential changes for electrocardiograms (ECGs), light source and photodetectors, such as LED-photodiode pairs, for optically based oxygen saturation measurements, xyz accelerometer for movement and exertion measurements, and the like. In some embodiments, methods and devices of the developments hereof include a circuit that mimics a driven right-leg circuit (sometimes referred to herein as "a proxy driven right-leg circuit") that permits reduction in common mode noise in a small-footprint device conveniently adhered or having the capacity to be adhered to an individual.

30 **[0005]** In another aspect, the developments hereof include methods and/or devices for measuring oxygen saturation parameters from time concordant pulse oximetry signals and ECG signals. In one embodiment, ECG signals may be used to define intervals, or "frames" of pulse oximetry data that are collected and averaged for determining the constant and main periodic components (i.e. DC and AC components) of the pulse oximetry signals from which, in turn, values for oxygen saturation may be determined. Patient-wearable devices of such embodiments with pulse oximetry and ECG sensors may be particularly useful when placed on a patient's chest for such signal acquisition.

35 **[0006]** These as well as other aspects are exemplified in a number of illustrated alternative implementations and applications, some of which are shown in the figures and characterized in the claims section that follows. The invention is defined by the appended claims 1-12.

**BRIEF DESCRIPTION OF THE DRAWINGS**

45 **[0007]** The drawings include:

Fig. 1, which includes sub-part Figs. 1A-1H, illustrates several alternatives of the present developments, including various of isometric, top and bottom plan and elevational views of devices and alternative conductive adhesive structures.

50 Fig. 2, which includes sub-part Figs. 2A-2C, provides circuit diagrams of alternatives to a driven right leg circuit.

Fig. 3 is a flow chart including alternative methods of use.

Fig. 4 illustrates an exemplary computer system or computing resources with which implementations hereof may be utilized.

55 Fig. 5, which includes sub-part Figs. 5A-5D, provides alternative screenshots of alternative software implementations according hereto.

Figs. 6A-6B illustrate features of one embodiment for measuring oxygen saturation using pulse oximetry signals and electrocardiogram signals.

Fig. 6C is a flow chart showing steps of one embodiment for determining oxygen saturation values.

Figs. 6D-6E illustrate an embodiment for determining depth of respiration values.

#### DETAILED DESCRIPTION

5 **[0008]** In one aspect, a system hereof may include a device for monitoring physiological parameters such as one or more or all of electrocardiogram (aka ECG or EKG), photoplethysmogram (aka PPG), pulse oximetry and/or patient acceleration or movement signals. Systems hereof may be established to measure and process such signals of a patient using or including one or more of the following elements: (a) a circuit, sometimes flexible as in or on or forming a flexible or flex circuit board, embedded in a flat elastic substrate or board having a top surface and a bottom surface, the circuit having (i) at least one sensor mounted in or adjacent the bottom surface of the flat elastic substrate, the at least one sensor being capable of electrical or optical communication with the patient, (ii) at least one signal processing module for receiving and/or accepting signals from the at least one sensor in some implementations also providing for transforming such signals for storage as patient data; (iii) at least one memory module for receiving and/or accepting and storing patient data, (iv) at least one data communication module for transferring stored patient data to an external device, and (v) a control module for controlling the timing and operation of the at least one sensor, one or more of the at least one signal processing module, the at least one memory module, the at least one data communication module, and/or the control module capable of receiving commands to implement transfer of patient data by the at least one data communication module and to erase and/or wipe patient data from the at least one memory module; and (b) a conductive adhesive removably attached to the bottom surface of the flat elastic substrate, the conductive adhesive capable of adhering to skin of the patient and of conducting an electrical signal substantially only in a direction perpendicular to the bottom surface of the flat elastic substrate, and/or in some implementations including a conductive portion adjacent the sensor or sensors and a non-conductive portion. In some implementations, the conductive adhesive is an anisotropically conductive adhesive in that it comprises regions of material that conducts current substantially only in a direction perpendicular to the skin (i.e. "z-axis" conduction).

25 **[0009]** In some examples, devices hereof will be for comprehensive long-term cardiac monitoring. Features of such may include one or more of a Lead 1 ECG, PPG, pulse oximeter, accelerometer, and a button or other indicator for manual patient event marking. Such a device may be adapted to store up to, for example, about two weeks of continuous data (though more will also be feasible in alternative implementations), which may in some examples be downloaded to a clinic or other computer in a short time period, as for one example, in only about 90 seconds (though less time will be viable in alternative implementations) via computer connection, whether wireless or wired as in one example by USB or other acceptable data connection. A companion software data analysis package may be adapted to provide automated event capture and/or allow immediate, local data interpretation.

35 **[0010]** Intermittent cardiac anomalies are often difficult for physicians to detect and/or diagnose, as they would typically have to occur during a physical examination of the patient. A device hereof may address this problem with what in some examples may be a continuous or substantially continuous monitoring of a number of vital signs.

40 **[0011]** Some alternative features may include (i) a driven "Right Leg" circuit with electrodes located only on the chest, (ii) a "z-Axis" or anisotropic conductive adhesive electrode interface that may permit electrical communication only between an electrode and a patient's skin immediately beneath the electrode, (iii) data transmission to and interpretation by a local computer accessible to CCU/ICU personnel, (iv) a unique combination of hardware allows correlation of multiple data sources in time concordance to aid in diagnosis.

45 **[0012]** In some alternative examples, devices and systems hereof may provide 1) reusability (in some cases near or greater than about 1000 patients) allows recouping cost of the device in just about 10-15 patient tests, 2) one or more of ecg waveform data, inertial exertion sensing, manual event marking, and/or pulse oximeter, any or all of which in time concordance to better detect and analyze arrhythmic events. 3) efficient watertightness or waterproofing (the patient can even swim while wearing the device), and 4) a comprehensive analysis package for immediate, local data interpretation. An alternative device may be adapted to take advantage of flex-circuit technology, to provide a device that is light-weight, thin, durable, and flexible to conform to the patient's skin.

**[0013]** Figs. 1 and 2 illustrate examples of alternative examples of devices that may be so adapted.

50 **[0014]** Fig. 1 shows a device 100 that has a component side or top side 101, patient side or circuit side 102, and one or more inner electrical layer(s), generally identified by the reference 103 and an elongated strip layer 105. The strip layer 105 may have electronics thereon and/or therewithin. FIG. 1A shows isometrically these together with some other elements that may be used herewith. FIG. 1B is more specifically directed to a top side 101 plan view and FIG. 1C to an underside, patient side 102 plan view and FIG. 1D a first elevational, side view.

55 **[0015]** Many of the electronics hereof may be disposed in the electronics layer or layers 103, and as generally indicated here, the electronics may be encapsulated in a material 104 (see FIGs. 1A, 1B and 1D for some examples), plastic or the like, or potting material, to fix them in operative position on or in or otherwise functionally disposed relative to the elongated strip layer 105. The potting or other material may in many implementations also or alternatively provide a waterproof or watertight or water resistant coverage of the electronics to keep them operative even in water or sweat

usage environments. One or more access points, junctions or other functional units 106 may be provided on and/or through any side of the encapsulation material 104 for exterior access and/or communication with the electronics disposed therewithin, or thereunder. FIGs. 1A, 1B and 1D show four such accesses 106 on the top side. These may include high Z data communication ports and/or charging contacts, inter alia. This upper or component side 101 of device 100 may be coated in a silicone compound for protection and/or waterproofing, with only, in some examples, a HS USB connector exposed via one or more ports 106, e.g., for data communication or transfer and/or for charging.

**[0016]** The elongated strip layer 105 may be or may include a circuit or circuit portions such as electrical leads or other inner layer conductors, e.g., leads 107 shown in FIG. 1D, for communication between the electronics 103 and the electrically conductive pads or contacts 108, 109 and 110 described further below (108 and 109 being in some examples, high impedance/high Z silver or copper/silver electrodes for electrocardiograph, ECG, and 110 at times being a reference electrode). In many implementations, the strip layer 105 may be or may include flex circuitry understood to provide acceptable deformation, twisting, bending and the like, and yet retain robust electrical circuitry connections therewithin. Note, though the electronics 103 and electrodes 108, 109, 110 are shown attached to layer 105; on top for electronics 103, and to the bottom or patient side for electrodes 108, 109, 110; it may be that such elements may be formed in or otherwise disposed within the layer 105, or at least be relatively indistinguishably disposed in relative operational positions in one or more layers with or adjacent layer 105 in practice. Similarly, the leads or traces 107 are shown embedded (by dashed line representation in FIG. 1D); however, these may be on the top or bottom side, though more likely top side to insulate from other skin side electrical communications. If initially top side (or bottom), the traces may be subsequently covered with an insulative encapsulant or like protective cover (not separately shown), in many implementations, a flexible material to maintain a flexible alternative for the entire, or majority of layer 105.

**[0017]** On the patient side 102, the ECG electrodes 108, 109 and 110 may be left exposed for substantially direct patient skin contact (though likely with at least a conductive gel applied therebetween); and/or, in many implementations, the patient side electrodes 108, 109 and/or 110 may be covered by a conductive adhesive material as will be described below. The electrodes may be or may be may be plated with a robust high conductive material, as for example, silver/silver chloride for biocompatibility and high signal quality, and in some implementations may be highly robust and, for one non-limiting example, be adapted to withstand over about 1000 alcohol cleaning cycles between patients. Windows or other communication channels or openings 111, 112 may be provided for a pulse oximeter, for example, for LEDs and a sensor. Such openings 111, 112 would typically be disposed for optimum light communication to and from the patient skin. An alternative disposition of one or more light conduits 111a/112a is shown in a non-limiting example in FIG. 1D more nearly disposed and/or connected to the electronics 103. A variety of alternative placements may be usable herein/herewith.

**[0018]** In some examples, sampling of the ambient light (with the LEDs off) may be provided, and then subtracting this from each of the pulse-ox signals in order to cancel out the noise caused by sunlight or other ambient light sources.

**[0019]** The LEDs and photodiode sensor may also and/or alternatively be covered with a layer of silicone to remove any air gap between the sensor/LEDs and the patient skin. An example of such is set forth in FIG. 1H; where a silicone layer 121 is shown covering/surrounding the sensors/LEDs 111a/111b/112a. LED 111a might be a Red LED, LED 111b might be an IR (infrared) LED and the device 112a might be a sensor. This may reduce the light lost to reflection off the skin, and thereby greatly increase the signal and reduce the noise caused by motion of the skin relative to the sensor. In some examples this silicone might be referred to as a light pipe and in some situations may be clear, colorless, and/or medical grade silicone.

**[0020]** FIG. 1D provides a first example of an adhesive 113 that may be used herewith. The adhesive layer 113 is here a double-sided adhesive for application to the bottom side 102 of the device 100, and a second side, perhaps with a different type of adhesive for adhering to the skin of the human patient (not shown). Different types of materials for adhesion might be used in that the material of choice to which the adhesive layer is to be attached are different; typically, circuit or circuit board material for connection to the device 100, and patient skin (not separately shown) on the patient side.. A protective backing 114 may be employed on the patient side until application to the patient is desired. Note, in many applications, the adhesive 113 is anisotropic in that it may preferably be only conductive in a single or substantially a single direction, e.g., the axis perpendicular to the surface of adhesive contact. Thus, good electrically conductive contact for signal communication can be had through such adhesive to/through the adhesive to the electrical contacts or electrodes, 108, 109 and 110. Note, a corresponding one or more light apertures 111b/112b are shown in the adhesive of 113 of the example of FIG. 1D to communicate light therethrough in cooperation with the light conduit(s) 111a/112a in/through layer 105 for communication of light data typically involved in pulse oximetry.

**[0021]** The adhesive may thus be placed or disposed on the device 100, in some implementations substantially permanently, or with some replaceability. In some examples, the device as shown in FIGs. 1A-1D and/or 1G without (or with in some implementations) the adhesive may be reusable. In many such cases, the adhesive layer 113 may be removed and replaced before each subsequent use, though subsequent re-use of and with a layer 113 is not foreclosed. In a first or subsequent use with a replaceable adhesive layer 113, it may be that the user applying the device to the patient, e.g., the physician or technician or even the patient, him/herself, applies the conductive transfer adhesive 113

to the patient side 102 of the device 100. The protective backing 114 may then be removed, and the device adhered to the patient and activated. Activation may occur in a number of ways; in some, it may be pre-set that an affirmative activation interaction may not be necessary from the doctor or patient or like due to either an inertial and/or a pulse oximeter activation which may be substantially automatically activating, e.g., upon receiving sufficient minimum input (movement in case of inertial system or light reflection of blood flow for pulse oximetry); however, a button may be provided at access 106 or in some other location adjacent the electronics to allow the patient to start or stop the device or otherwise mark an event if desired. In one exemplar implementation the device may be worn for a period such as two weeks for collection of data substantially continuously, or at intervals as may be preferred and established in or by the systems hereof.

**[0022]** After a monitoring period is over a physician, technician, patient or other person may then remove the device from the patient body, remove the adhesive, in some instances with alcohol, and may establish a data communication connection for data transfer, e.g., by wireless communication or by insertion/connection of a USB or like data connector to download the data. The data may then be processed and/or interpreted and in many instances, interpreted immediately if desired. A power source on board may include a battery and this can then also be re-charged between uses, in some implementations, fully recharged quickly as within about 24 hours, after which the device could then be considered ready for the next patient.

**[0023]** Some alternative conductive adhesives may be used herewith. FIGs. 1E, 1F and 1G show one such alternative conductive adhesive 113a; a bottom plan view in FIG 1E and elevational side views thereof in FIGs. 1F and 1G (as being connected to a device 100 in FIG. 1G). In some implementations, the conductivity may be anisotropic as introduced above; in some conductive primarily if not entirely in the direction of the Z-Axis; perpendicular to the page (into and/or out of the page) in FIG. 1E, and/or vertically or transversally relative to the long horizontal shown axis of device 100 in the implementation view of FIG. 1F.

**[0024]** This particular example includes a composite adhesive 113a which itself may include some non-conductive portion(s) 113b and some one or more conductive portions 113c. The adhesive composite 113a may, as described for adhesive 113 above be double sided such that one side adheres to the patient while the other side would adhere to the underside 102 of the device 100 (see FIG. 1G) so that one or more conductive portions 113c may be disposed or placed in electrically communicative and/or conductive contact with the integrated electrodes on the electronic monitoring device 100. Since the electrodes would operate better where they may be electrically isolated or insulated from each other, yet each making electrical contact or communication with the patient's skin, the adhesive may further be more specifically disposed in some implementations as follows.

**[0025]** As shown in FIGs. 1E and 1F, three isolated conductive portions 113c may be disposed separated from each other by a body portion 113b which may be non-conductive. These could then correspond to the electrodes 108, 109, 110 from the above-described examples, and as more particularly shown schematically in FIG. 1G (note the scale is exaggerated for the adhesive 113a and thus, exact matching to the electrodes of device 100 is not necessarily shown). In some examples, the electrode areas 113c may be a conductive hydrogel that may or may not be adhesive, and in some examples, may be made of a conductive adhesive conductive material such as 3M Corporation 9880 Hydrogel adhesive (3M Company, St. Paul, Minnesota). These areas 113c may then be isolated from each other by a non-conductive material 113b such as 3M Corporation 9836 tape or 3M double-sided Transfer Adhesive 9917 (3M, St. Paul, MN) or equivalent. The additional layer 113d, if used, might be a 3M 9917 adhesive together with the 113b of a 9836 material. These constructs may provide the effect of creating a low electrical impedance path in the Z-axis direction (perpendicular to page for FIG. 1E and vertically/transversally for FIGs. 1F and 1G) for the electrode areas 113c, and high electrical impedance path between the electrodes in the X/Y directions. (See FIGs. 1E, 1F and 1G; coplanar with the page in FIG. 1E and horizontal and perpendicular to the page in FIGs. 1F and 1G). Thus, a composite adhesive strip can ensure not only device adhering to the patient, but also that the electrodes whether two or as shown three electrodes are conductively connected by conductive portions of the adhesive strip, where the combination of conductive and non-conductive portions can then reduce signal noise and/or enhance noise free characteristics. Electrodes that move relative to skin can introduce noise; that is, electrodes electrically communicative/connected to the skin via a gel may move relative to the skin and thus introduce noise. However, with one or more conductive adhesive portions in a composite adhesive connected to respective electrodes and then substantially securely connected to the skin will keep the respective electrodes substantially fixed relative to the skin and thereby reduce or even eliminate electrode movement relative to the skin. Removal of such movement would then remove noise which would thereby provide a clean signal that can allow for monitoring cardiac P waves which enhances the possibility to detect arrhythmias that couldn't otherwise be detected. Further description is set forth below.

**[0026]** In some examples, a further optional connective and/or insulative structure 113d may be implemented as shown in FIG. 113d to provide further structural and insulative separation between electrodes with connected to a device 100 on the underside 102 thereof (see FIG. 1G). Though shown separate in FIGs. 1F and 1G, it may be contiguous with the insulative adhesive 113b of these views.

**[0027]** Some alternative examples hereof may include a driven right leg ECG circuit with one or more chest only

electrodes ("Driven Chest Electrode"). In addition to the electrodes used to measure a single or multiple lead electrocardiogram signal, a device 100 may use an additional electrode, as for example the reference electrode 110 (see FIGs. 1A, 1C, 1D and 1G, e.g.) to reduce common mode noise. Such an electrode may function in a manner similar to the commonly-used driven right leg electrode, but may here be located on the patient's chest rather than on the patient's right leg but nevertheless this third/reference electrode may play the role of the leg electrode. This chest electrode may thus mimic a right leg electrode and/or be considered a proxy driven right leg electrode. A circuit, or portion of an overall circuit, adapted to operate in this fashion may include a number of amplifier stages to provide gain, as well as filtering to ensure circuit stability and to shape the overall frequency response. Such a circuit may be biased to control the common mode bias of the electrocardiogram signal. This driven chest electrode implementation may be used in conjunction with a differential or instrumentation amplifier to reduce common mode noise. In this case, the sense electrode may be used as one of the electrocardiogram electrodes. Alternatively, a single-ended electrocardiogram amplifier may be used where the differential electrocardiogram signal is referenced to ground or to some other known voltage.

**[0028]** A circuit or sub-circuit 200 using a transistor 201 as shown in Fig. 2 may be such a circuit (aka module) and may thus include as further shown in FIG. 2A, a sense electrode 202, a drive electrode 203, and an amplifier 204. Both the sense and drive electrodes 202, 203 are placed on the patient's chest such that they provide an electrical connection to the patient. The amplifier 204 may include gain and filtering. The amplifier output is connected to the drive electrode, the inverting input to the sense electrode, and the non-inverting input to a bias voltage 205. The amplifier maintains the voltage of the sense electrode at a level close to the bias voltage. An electrocardiogram signal may then be measured using additional electrodes. Indeed, as was the case for the improved conductivity through use of anisotropic adhesive portions above, here also or alternatively, the use of this third electrode as a proxy for a right leg electrode (i.e., proxy driven right leg electrode) can provide signal reception otherwise unavailable. Clean signals may thus allow for receiving cardiac P waves which enhances the possibility to detect arrhythmias that couldn't otherwise be detected.

**[0029]** Further alternative descriptions of circuitry include that which is shown in FIGs. 2B and 2C; in which are shown non-limiting alternatives in which three adjacent electrodes E1, E2, and E3 may be used to pick up the ECG signal, one of which electrodes playing the role of the distant limb electrode of traditional ECG monitors. Because the electrode-patient interface has an associated impedance ( $Re_1$  and  $Re_2$ ), current flowing through this interface will cause a difference in voltage between the patient and the electrode. The circuit may use a sense electrode (E1) to detect the patient voltage. Because this exemplar circuit node has a high impedance to circuit ground (GND), very little current flows through the electrode interface, so that the voltage drop between the patient and this node is minimized. The first of these alternative, non-limiting circuits (FIG. 2B) also contains an amplifier (U1) whose low-impedance output is connected to a separate drive electrode (E2). The amplifier uses negative feedback to control the drive electrode such that the patient voltage (as measured by the sense electrode E1) is equal to the bias voltage (V1). This may effectively maintain the patient voltage equal to the bias voltage despite any voltage difference between the driven electrode (E2) and the patient. This can include voltage differences caused by power line-induced current flowing between the drive electrode and the patient (through  $Re_2$ ). This arrangement differs from a traditional 'driven-right-leg' circuit in at least two ways: the driven electrode is placed on the patient's chest (rather than the right leg), and the ECG signal is a single-ended (not differential) measurement taken from a third electrode (E3). Because all electrodes are located on the patient's chest, a small device placed there may contain all the necessary electrodes for ECG measurement. One possible benefit of the single-ended measurement is that gain and filtering circuitry (U2 and associated components (Fig. 2C)) necessary to condition the ECG signal prior to recording (ECG Output) requires fewer components and may be less sensitive to component tolerance matching. The examples of FIGs. 2A, 2B and 2C are non-limiting examples and not intended to limit the scope of the claims hereto as other circuits with other circuit elements can be formed by skilled artisans in view hereof and yet remain within the spirit and scope of claims hereof.

**[0030]** In many examples, a system hereof may include other circuitry operative together with the ECG electrodes, which may thus be accompanied by other sensors to provide time concordant traces of: i) ECG p-, qrs-, and t- waves; ii) O<sub>2</sub> Saturation, as measured by Pulse Oxymetry; and/or iii) xyz acceleration, to provide an index of physical activity. Such circuitry may be implemented to one or more of the following electrical specifications. The overall system might in some implementations include as much as two weeks (or more) of continuous run time; gathering data during such time. Some implementations may be adapted to provide as many or even greater than 1000 uses. Alternatives may include operability even after or during exposure to fluids or wetness; in some such examples being water resistant, or waterproof, or watertight, in some cases continuing to be fully operable when fully submerged (in low saline water). Other implementations may include fast data transfer, as for an example where using an HS USB for full data transfer in less than about 90 seconds. A rechargeable battery may typically be used.

**[0031]** A further alternative example may include an electronic "ground": In a device hereof, mounted entirely on a flexible circuit board, the ground plane function may be provided by coaxial ground leads adjacent to the signal leads. The main contribution of this type of grounding system may be that it may allow the device the flexibility required to conform and adhere to the skin.

**[0032]** For electrocardiograph; EKG or ECG, some examples may include greater than about 10 Meg Ohms input

impedance; some implementations may operate with a 0.1 - 48 Hz bandwidth; and some with an approximate 256 Hz Sampling Rate; and may be implementing 12 Bit Resolution. For PPG and Pulse Oximeter, operation may be with 660 and 940 nm Wavelength; about 80 - 100 SpO<sub>2</sub> Range; a 0.05 - 4.8 Hz Bandwidth; a 16 Hz Sampling Rate; and 12 bit resolution. For an accelerometer: a 3-Axis Measurement may be employed, and in some implementations using a  $\pm 2$  G Range; with a 16 Hz Sampling Rate; and a 12 Bit Resolution.

**[0033]** Some summary methodologies may now be understood with relation to FIG. 3, though others may be understood through and as parts of the remainder of the disclosure hereof. A flow chart 300 as in Fig. 3 may demonstrate some of the alternatives; where an initial maneuver 301 might be the application of the device 100 to the patient. Indeed, this might include some one or more of the alternatives for adhesive application as described here above, whether by/through use of an adhesive such as that 113 of Fig. 1D, or that of FIGs. 1E, 1F and/or 1G. Then, as shown, in moving by flow line 311, a data collection operation 302 may be implemented. Note, this might include a continuous or substantially continuous collection or an interval or periodic collection or perhaps even a one time event collection. This may depend upon the type of data to be collected and/or be dependent upon other features or alternatives, as for example whether a long term quantity of data is desired, for ECG for example, or whether for example a relative single data point might be useful, as in some cases of pulse oximetry (sometimes a single saturation point might be of interest, as for example, if clearly too low, though comparison data showing trending over time, may indeed be more typical).

**[0034]** Several alternatives then present in FIG. 3, flow chart 300; a first such might be the following of flowline 312 to the transmission of data operation 303, which could then involve either wireless (e.g., USB or other) data communication from the device 100 to data analysis and/or storage devices and/or systems (not separately shown in FIG. 3; could include computing devices, see e.g., FIG. 4 described below, or the like). Options from this point also appear; however, a first such might include following flow line 313 to the data analysis operation 304 for analyzing the data for determination of the relative health and/or for condition diagnosis of a patient. Computing systems, e.g., a computer (could be of many types, whether hand-held, personal or mainframe or other; see FIG. 4 and description below) could be used for this analysis; however, it could be that sufficient intelligence might be incorporated within the electronics 103 of device 100 such that some analysis might be operable on or within device 100 itself. A non-limiting example, might be a threshold comparison, as for example relative to pulse oximetry where when a low (or in some examples, perhaps a high) threshold level is reached an indicator or alarm might be activated all on/by the electronics 103 of the device 100.

**[0035]** A similar such example, might be considered by the optional alternative flow path 312a which itself branches into parts 312b and 312c. Following flow path 312 a, and then, in a first example path 312b, a skip of the transmit data operation 303 can be understood whereby analysis 304 might be achieved without substantial data transfer. This could explain on board analysis, whether as for example according to the threshold example above, or might in some instances include more detailed analysis depending upon how much intelligence is incorporated on/in the electronics 103. Another view, is relative to how much transmission may be involved even if the transmission operation 303 is used; inasmuch as this could include at one level the transmission of data from the patient skin through the conductors 108, 109 and/or 110 through the traces 107 to the electronics 103 for analysis there. In other examples, of course, the transmission may include off-board downloading to other computing resources (e.g., FIG. 4). In some cases, such off-loading of the data may allow or provide for more sophisticated analysis using higher computing power resources.

**[0036]** Further alternatives primarily may involve data storage, both when and where, if used. As with intelligence, it may be that either some or no storage or memory may be made available in/by the electronics 103 on-board device 100. If some storage, whether a little or a lot, is made available on device 100, then, flow path 312a to and through path 312c may be used to achieve some storing of data 305. This may in many cases then, though not necessarily be before transmission or analysis (note, for some types of data multiple paths may be taken simultaneously, in parallel though perhaps not at the same time or serially (eg., paths 312b and 312c need not be taken totally to the exclusion of the other), so that storage and transmission or storage and analysis may occur without necessarily requiring a completion of any particular operation before beginning or otherwise implementing another). Thus, after (or during) storage 305, flow path 315a may be followed for stored data which may then be transmitted, by path 315b to operation 303, and/or analyzed, by path 315c to operation 304. In such a storage example, which in many cases may also be an on-board storage example, data can be collected then stored in local memory and later off-loaded/transmitted to one or more robust computing resources (e.g., FIG. 4) for analysis. Frequently, this can include long term data collection, e.g., in the manner of days or weeks or even longer, and may thus include remote collection when a patient is away from a doctor's office or other medical facilities. Thus, data can be collected from the patient in the patient's real world circumstances. Then, after collection, the data can be transmitted from its storage on device 100 back to the desired computing resource (FIG. 4, e.g.), and such transmission might be wireless or wired or come combination of both, as for example a blue tooth or WiFi connection to a personal computer (FIG. 4 for one example) which might then communicate the data over the internet to the designated computer for final analysis. Another example might include a USB connection to a computer, either to a PC or a mainframe (FIG. 4), and may be to the patient computer or to the doctor computer for analysis.

**[0037]** If little or no storage or memory is resident on device 100 (or in some examples even where there may be a

large amount of resident memory available), then, relatively soon after collection, the data would need to or otherwise might desirably either or both be transmitted and then stored, see path 313a after operation 303, and/or transmitted and analyzed, paths 312 and 313. If path 313a is used, then, more typically, the data storage may be in/on computing resources (not shown in FIG. 3, but see FIG. 4 described below) off-board (though on-board memory could be used as well), and then, any of paths 315a, 315b and 315c may be used.

**[0038]** A feature hereof may include an overall system including one or more devices 100 and computing resources (see Fig. 4, for example) whether on-board device(s) 100, or separate, as for example in personal or mobile or hand-held computing devices (generally by FIG. 4), the overall system then providing the ability for the physician or doctor to have immediate, in-office analysis and presentation of collected test data. This would in some implementations allow for on-site data analysis from the device without utilization of a third party for data extraction and analysis.

**[0039]** Alternative examples hereof may thus include one or more hardware and software combinations for multiple alternative data source interpretations. As noted above, a device 100 hereof includes hardware that monitors one or more of various physiologic parameters, then generates and stores the associated data representative of the monitored parameters. Then, a system which includes hardware such as device 100 and/or the parts thereof, *and* software and computing resources (FIG. 4, generally) for the processing thereof. The system then includes not only the collection of data but also interpretation and correlation of the data.

**[0040]** For example, an electrocardiogram trace that reveals a ventricular arrhythmia during intense exercise may be interpreted differently than the same arrhythmia during a period of rest. Blood oxygen saturation levels that vary greatly with movement can indicate conditions that may be more serious than when at rest, *inter alia*. Many more combinations of the four physiologic parameters are possible, and the ability of software hereof to display and highlight possible problems will greatly aid the physician in diagnosis. Thus, a system as described hereof can provide beneficial data interpretation.

**[0041]** Some of the features which can assist toward this end may be subsumed within one or more of operations 303 and 304 of FIG. 3, wherein data collected on a device 100 can rather simply be communicated/transmitted to computing resources (again, whether on-board device 100 or discrete therefrom as e.g., FIG. 4). For an example, when a patient having had a device applied (operation 301) may return to a physician's office after a test period wherein data was collected (operation 302) the device is connected via one or more data transmission alternatives, as for example, USB to a computer (Windows or Mac) (generally with reference to FIG. 4 and description thereof) in the office, allowing immediate analysis by the physician while the patient waits (note, the device 100 may first have been removed from the patient or might remain thereon pending transmission and analysis for determination of whether more data may be desired). In some implementations, data analysis time may be relatively quick, at approximately 15 minutes in some implementations, and might be achieved with a user-friendly GUI (Graphic User Interface) to guide the physician through the analysis software.

**[0042]** The analysis/software package may be disposed to present the physician with results in a variety of formats. In some implementations, an overview of the test results may be presented, either together with or in lieu of more detailed results. In either case, a summary of detected anomalies and/or patient-triggered events may be provided, either as part of an overview and/or as part of the more detailed presentation. Selecting individual anomalies or patient-triggered events may provide desirable flexibility to allow a physician to view additional detail, including raw data from the ECG and/or from other sensors. The package may also allow data to be printed and saved with annotations in industry-standard EHR formats.

**[0043]** In one example, patient data may be analyzed with software having the one or more of the following specifications. Some alternative capabilities may include: 1. Data Acquisition; i.e., loading of data files from device; 2. Data Formatting; i.e., formatting raw data to industry standard file formats (whether, e.g., aECG (xml); DICOM; or SCP-ECG) (note, such data formatting may be a part of Acquisition, Storage or Analysis, or may have translation from one to another (e.g., data might be better stored in a compact format that may need translation or other un-packing to analyze)); 3. Data Storage (whether local, at a clinic/medical facility level or e.g., in the Cloud (optional and allows offline portable browser based presentation/analysis)); 4. Analysis which *inter alia*, may include, e.g., noise filtering (High pass/Low pass digital filtering); and/or QRS (Beat) detection (in some cases, may include Continuous Wave Transform (CWT) for speed and accuracy); and/or 5. Data/Results Presentation, whether including one or more graphical user interface(s) (GUIs) perhaps more particularly with an overall Summary and/or General Statistics and/or Anomaly Summary of Patient triggered event(s); presentation of additional levels of detail whether of Strip view(s) of anomaly data by incident (previous, next) Blood Oxygen saturation, stress correlation or the like; and/or allowing care provider bookmarking/annotations/notes by incident and/or Print capability.

**[0044]** Further, on alternative combinations of hardware with proprietary software packages: I) One on-device software package may be adapted to store the measurements from the data signals acquired from one or more of EKG/ECG (whether right leg and/or p-, qrs- and/or t-waves), or O2 saturation, or xyz acceleration, in a time concordant manner, so that a physician may access a temporal history of the measurements (say, in some examples, over a 1-2 week interval), which would provide useful information on what the patient's activity level was prior to, during, and after the

## EP 2 903 509 B1

occurrence of a cardiac event. ii) an alternative to alternately manage the real-time transmission of the real-time measured parameters to a nearby station or relay. And/or; iii) an off-device ECG analysis software aimed at recognizing arrhythmias.

**[0045]** The software mentioned above may be industry understood software provided by a 3rd party, or specially adapted for the data developed and transmitted by and /or received from a wearable device 100 hereof. Thorough testing using standard (MIT-BIH/AHA/NST) arrhythmia databases, FDA 510(k) approvals preferred. Such software may be adapted to allow one or more of automated ECG analysis and interpretation by providing callable functions for ECG signal processing, QRS detection and measurement, QRS feature extraction, classification of normal and ventricular ectopic beats, heart rate measurement, measurement of PR and QT intervals, and rhythm interpretation.

**[0046]** In many examples, the software may be adapted to provide and/or may be made capable of supplying one or more of the following measurements:

Table 1:

1. Heart Rate Min, Max and Average
2. QRS duration average
3. PR interval average
4. QT interval average
5. ST deviation average

and, may be adapted to recognize a broad range of arrhythmias such as those set forth here:

Table 2A:

1. SINUS RHYTHM
2. SINUS RHYTHM + IVCD
3. SINUS BRADYCARDIA
4. SINUS BRADYCARDIA + IVCD
5. SINUS TACHYCARDIA
6. PAUSE
7. UNCLASSIFIED RHYTHM
8. ARTIFACT

**[0047]** This first group of 8 given above are arrhythmia types that may be recognizable even if there is no discernible P wave. They are the ones typically recognized by existing products in the outpatient monitoring market that we propose to address.

**[0048]** A second set or group of arrhythmias; below, may require a discernible and measurable P wave. Some implementations hereof may be adapted to be able to detect and recognize them, as device 100 may be able as described above to detect P waves, depending of course, and for example, on whether the strength of the P wave is affected by device 100 placement or patient physiology.

Table 2B:

9. ATRIAL FIBRILLATION/FLUTTER SVR (slow)
10. ATRIAL FIBRILLATION/FLUTTER CVR (normal rate)
11. ATRIAL FIBRILLATION/FLUTTER RVR (rapid)
12. FIRST DEGREE AV BLOCK + SINUS RHYTHM
13. FIRST DEGREE AV BLOCK + SINUS TACHYCARDIA
14. FIRST DEGREE AV BLOCK + SINUS BRADYCARDIA
15. SECOND DEGREE AV BLOCK
16. THIRD DEGREE AV BLOCK
17. PREMATURE ATRIAL CONTRACTION
18. SUPRAVENTRICULAR TACHYCARDIA
19. PREMATURE VENTRICULAR CONTRACTION
20. VENTRICULAR COUPLET
21. VENTRICULAR BIGEMINY
22. VENTRICULAR TRIGEMINY
23. IDIOVENTRICULAR RHYTHM

(continued)

## 24. VENTRICULAR TACHYCARDIA

## 25. SLOW VENTRICULAR TACHYCARDIA

5

**[0049]** Further in alternative software examples some sample screenshots are shown in FIG. 5. A first such alternative is shown in FIG. 5A, which is an example screenshot showing ECG and Oxygen Saturation data taken by using a patch device such as a device 100 hereof. An extremely clean signal is shown (no filtering or smoothing has been done on this data). Distinct p-waves are also shown (3 of which are shown as an example with arrows). P wave detection can be extremely important for ECG anomaly detection. Oxygen Saturation, as measured by Pulse Oxymetry, is shown on the bottom plot. This is data taken by the a device on the chest, and is taken in time concordance with the ECG data.

10

**[0050]** Another alternative is shown in Fig. 5B, which is an example screenshot of Analysis Software. This is a sample of ECG data taken from the MIT-BIH Arrhythmia Database, Record 205. As analyzed by the Analysis system hereof, we see in the Event Occurrences Summary list (top, left) five (5) anomaly types (plus normal sinus rhythm). This list also shows the number of occurrences of each anomaly, total duration of the anomaly in the complete ECG, and the percent time this anomaly occurs in the complete ECG. To view specific instances of each anomaly, the user double clicks the specific row in the Event Occurrences Summary list, as shown in Figure 5C.

15

**[0051]** As introduced, Fig. 5C is an example screenshot showing specific instance of Ventricular Tachycardia. The ECG plot automatically navigates to the specific time in the ECG waveform, and marks the beginning and end of the event. More detailed data about this specific event is now shown in the Occurrence Details: HR Average, HR Max, etc. for the duration of this event. To show the instances of another anomaly in this ECT, the user can click on the Premature Ventricular Contraction (PVC) row of the Event Occurrences Summary, as shown Figure 5D.

20

**[0052]** As introduced, Fig. 5D is an example screenshot showing specific instance of Premature Ventricular Contraction. This shows occurrences of the PVC. The Start Times list (middle top) shows all instances of PVC occurrences in this ECG, and lists the start time for each occurrence. In this case, the user can click on the PVC that starts at 00:15:27 (the 11<sup>th</sup> occurrence). The ECG plot is automatically taken to this point in time to show and indicate the PVC instances in the waveform. Since there are 3 instances of a PVC in this timeslot, all 3 occurrences are marked.

25

**[0053]** As mentioned above, in one aspect of the developments hereof, ECG signals collected in time concordance with pulse oximetry signals may be used to reduce the noise in the pulse oximetry signals and to permit the calculation of values for oxygen saturation, particularly in circumstances where sensors pulse oximetry data are placed on noise-prone locations of a patient, such as the chest. In some embodiments, this aspect may be implemented by the following steps: (a) measuring an electrocardiogram signal over multiple heart beats; (b) measuring one or more pulse oximetry signals over multiple heart beats such that the electrocardiogram signal and the one or more pulse oximetry signals are in time concordance over one or more heart beats; (c) comparing a portion of the electrocardiogram signal and the one or more pulse oximetry signals in time concordance over one or more heart beats to determine a constant component and a primary periodic component of each of the one or more pulse oximetry signals; and (d) determining oxygen saturation from the constant components and primary periodic components of the one or more pulse oximetry signals. Measurement of the ECG signals and pulse oximetry signals may be implemented by embodiments of devices hereof. In particular, pulse oximetry signals may be a reflective infrared signal and a reflective red light signal collected by a photodetector in a device hereof. Intervals of pulse oximetry signals corresponding to heart beats may be determined by comparing such signals to the time concordant ECG signals. For example (not intended to be limiting), successive R-wave peaks of a time concordant ECG signal may be used to identify such intervals, although other features of the ECG signal may be used as well. Once such intervals are identified, values at corresponding times within the intervals may be averaged to reduce signal noise and to obtain more reliable values for the constant components (sometimes referred to as the "DC components") and the main periodic components (sometimes referred to as the "AC components") of the pulse oximetry signals, e.g. Warner et al, Anesthesiology, 108: 950-958 (2008). The number of signal values recorded in an interval depends on the signal sampling rate of the detectors and processing electronics employed. Also, as the intervals may vary in duration, the averaging may be applied to a subset of values in the intervals. As described below, oxygen saturation values may be computed from such DC and AC components using conventional algorithms. The number of heart beats or intervals over which such averages may be computed may vary widely, as noted below. In some embodiments, signals from one or more heart beats or intervals may be analyzed; in other embodiments, signals from a plurality of heart beats or intervals may be analyzed; and in some embodiments, such plurality may be in the range of from 2 to 25, or in the range of from 5 to 20, or in the range of from 10 to 20.

30

35

40

45

50

**[0054]** As mentioned above, patient wearable devices hereof for implementing the above aspect may be particularly useful for monitoring oxygen saturation in noisy regions for such measurements, for example, where there is significant local skin movement, such as the chest location.

55

**[0055]** One example of the above aspect hereof is illustrated in Figs. 6A-6C. In Fig. 6A, curve A (600) illustrates time varying output of the photodiode of a device hereof for infrared (IR) reflection and curve B (602) illustrates time varying

output of the photodiode of the device for red light reflection. In some embodiments, the skin is alternatively illuminated by the red and IR LEDs to generate the signals collected by the same photodiode. In Fig. 6B, time synchronized (i.e. time concordant) ECG data, illustrated by curve C (604), is added to the plot of Fig. 6A. Peak values in the ECG data (e.g. peaks 606 and 608) may be used to define frames or intervals of pulse oximetry data. Additional consecutive frames or intervals are indicated by 612 and 614, and further frames may be similarly determined. In accordance with this aspect, pulse oximetry data from a plurality of frames is collected. The magnitude of the plurality may vary widely depending on particular applications. In some embodiments, the plurality of frames collected is from 5 to 25; in one embodiment, a plurality is between 8 and 10 frames. Typically, frames or intervals of pulse oximetry data contain different numbers of signal samples. That is, output from the sensors may be sampled at a predetermined rate, such as a 32 samples per second. If the time between ECG peaks varies, then the number of samples per frame will vary. In one embodiment, features in the ECG data serving as the starting points of a frame are selected so that an associated peak in the pulse oximetry data is approximately in the mid-point, or center, of the frame, after which a predetermined number of signal samples are recorded for each frame. Preferably in this embodiment, the predetermined number is selected to be large enough to ensure that the pulse oximetry signal peak is roughly mid-frame. Sample values corresponding to time points above the predetermined value are not used. After a plurality of frames of data is collected, averages of the values at corresponding time points of the frames are computed. The values from such averages AC and DC components of the pulse oximetry data are determined and are then used to compute relative oxygen saturation by conventional methods, such as the ratio-of-ratios algorithm, e.g Cypress Semiconductor document No. 001-26779 Rev A (January 18, 2010). This basic procedure is summarized in the flow chart of Fig. 6C. Frame size (in terms of number of samples) is determined (620). Values of samples at corresponding time points within each frame are summed (622), after which average values for each time point are computed which, in turn, give the AC and DC components of IR and red light reflection with reduced noise. In some embodiments, values for these components can be used to compute oxygen saturation using conventional algorithms (626). Relative values for oxygen saturation may be converted into absolute values by calibrating the measurements for particular embodiments. Calibration may be carried out in controlled environments where individuals are exposed to varying atmospheric concentrations of oxygen and measured oxygen saturation values are related to corresponding oxygen levels.

**[0056]** In addition to the above example for comparing ECG signals with pulse oximetry signals, a range of other alternatives for such comparing is within the comprehension of those of ordinary skill in the art. For example, in order to find peaks of the AC component of pulse oximetry signals in the presence of noise, features of the time concordant ECG signal that are located at characteristic times preceding and succeeding the pulse oximetry maximum and/or minimum values may be used to reliably determine the pulse oximetry peak and minimum values when averaged over a plurality of heart beats (without the need to average all values of the pulse oximetry signal over the heart beats). For example, if, within an interval, the R wave peak of an ECG signal characteristically preceded a pulse oximetry signal maximum by x milliseconds and trailed a pulse oximetry signal minimum by y milliseconds, then the essential information about the AC component of the pulse oximetry signal may be obtained by repeated measurements of just two values of pulse oximetry signals.

**[0057]** In some examples, values for IR or red reflection measured by the photodiode may be used to estimate depth of respiration. In Fig. 6D, a curve (630) of Red or IR values over time is illustrated. In Fig. 6E, maximum values and minimum values of curve (630) are shown by dashed curves (632) and (634), respectively. The difference between the maximum and minimum values at a time point is monotonically related to the depth of breath in an individual being monitored. Thus, as illustrated, breaths at time (636) are shallower than those at time (638). In some examples, depth of breath versus time may be computed and monitored in an individual.

**[0058]** Some further alternatives may include data transmission and/or interpretation by local medical facilities, whether physician or doctor offices or e.g., ICU/CCU (Intensive Care/Coronary Care Units). Accordingly, a device 100 hereof that will measure one or more of a variety of physiologic signals, possibly including electrocardiogram, photoplethysmogram, pulse oximetry and/or patient acceleration signals will be placed on the patient's chest and held with an adhesive as described herein. The device transmits the physiologic signals wirelessly or by wire (e.g., USB) to a nearby base station for interpretation and further transmission, if desired. The wireless transmission may use Bluetooth, WiFi, Infrared, RFID (Radio Frequency Identification) or another wireless protocol. The device may be powered by wireless induction, battery, or a combination of the two. The device 100 monitors physiological signals and/or collects data representative thereof. The collected data may then be transmitted wirelessly or by wire connection, in real time, to the nearby base station. The device may be wirelessly powered by the base station or by battery, removing the need for wires between the patient and the station.

**[0059]** Thus, some of the alternative combinations hereof may include one or more of: 1) medical grade adhesives (from many possible sources) selected for their ability to maintain in intimate contact with the skin without damaging it, for several days (up to, say 10 days or two weeks in some examples), as well as operability with different types of sensors; 2) conductive electrodes or photo-sensitive detectors able to supply electrical signals from the skin or from the photo-response of cutaneous or subcutaneous tissues to photo-excitation; 3) amplifiers, microprocessors and memories,

capable of treating these signals and storing them; 4) power supply for the electronics hereof with stored or with wirelessly accessible re-chargeability; 5) flex circuits capable of tying the above elements together within a flexible strip capable of conforming to a cutaneous region of interest.

**[0060]** Examples of physiological parameters that may be subject to monitoring, recordation/collection and/or analyzing may include one or more of: electrocardiograms, photo responses of photo-excited tissues for e.g., oxygen saturation of blood; pulse rates and associated fluctuations; indications of physical activity/acceleration. One or more of these may be used in monitoring ambulatory cardiac outpatients over several days and nights, which could thereby provide for recording, for post-test analysis, several days' worth of continuous ECG signals together with simultaneous recording of O<sub>2</sub> saturation and an index of physical exertion. Similarly, one or more of these may be used in monitoring ambulatory pulmonary outpatients over several days and nights for recording, for post-test analysis, O<sub>2</sub> saturation together with simultaneous recording of an index of physical activity. Alternatively and/or additionally, one or more of these could be used for monitoring in-patients or other patients of interest, as for example neonates, wirelessly (or in some cases wired), whether in clinics, emergency rooms, or ICUs, in some instances detecting the parameters of EKG, O<sub>2</sub> and/or physical exertion, but instead of storing them would transmit them wirelessly to either a bedside monitor or a central station monitor, thus freeing the patient from attachment to physical wires. In particular, devices hereof may be adhered to the forehead of a neonate for monitoring respiration and oxygen saturation. In further alternatives, devices hereof may be used to monitor respiration and ECG of patients suffering from sleep apnea.

**[0061]** An exemplary computer system or computing resources which may be used herewith will now be described, though it should be noted that many alternatives in computing systems and resources may be available and operable within the reasonably foreseeable scope hereof so that the following is intended in no way to be limiting of the myriad possible computational alternatives properly intended within both the spirit and scope hereof.

**[0062]** Some of the examples of the present developments include various steps. A variety of these steps may be performed by hardware components or may be embodied in machine-executable instructions, which may be used to cause a general-purpose or special-purpose processor programmed with the instructions to perform the steps. Alternatively, the steps may be performed by a combination of hardware, software, and/or firmware. As such, FIG. 4 is an example of computing resources or a computer system 400 with which implementations hereof may be utilized. According to the present example, a sample such computer system 400 may include a bus 401, at least one processor 402, at least one communication port 403, a main memory 404, a removable storage media 405, a read only memory 406, and a mass storage 407. More or fewer of these elements may be used in a particular examples hereof.

**[0063]** Processor(s) 402 can be any known processor, such as, but not limited to, an Intel® Itanium® or Itanium 2® processor(s), or AMD® Opteron® or Athlon MP® processor(s), or Motorola® lines of processors. Communication port(s) 403 can be any of an RS-232 port for use with a modem based dialup connection, a 10/100 Ethernet port, a Universal Serial Bus (USB) port, or a Gigabit port using copper or fiber. Communication port(s) 403 may be chosen depending on a network such a Local Area Network (LAN), Wide Area Network (WAN), or any network to which the computer system 400 connects or may be adapted to connect.

**[0064]** Main memory 404 can be Random Access Memory (RAM), or any other dynamic storage device(s) commonly known in the art. Read only memory 406 can be any static storage device(s) such as Programmable Read Only Memory (PROM) chips for storing static information such as instructions for processor 402.

**[0065]** Mass storage 407 can be used to store information and instructions. For example, hard disks such as the Adaptec® family of SCSI drives, an optical disc, an array of disks such as RAID, such as the Adaptec family of RAID drives, or any other mass storage devices may be used.

**[0066]** Bus 401 communicatively couples processor(s) 402 with the other memory, storage and communication blocks. Bus 401 can be a PCI/PCI-X or SCSI based system bus depending on the storage devices used.

**[0067]** Removable storage media 405 can be any kind of external hard-drives, floppy drives, IOMEGA® Zip Drives, Compact Disc--Read Only Memory (CD-ROM), Compact Disc--ReWritable (CD-RW), Digital Video Dis--Read Only Memory (DVD-ROM).

**[0068]** The components described above are meant to exemplify some types of possibilities. In no way should the aforementioned examples limit the scope of the invention, as they are only exemplary embodiments.

**[0069]** The invention is defined by the appended claims 1-12.

## Claims

1. A device (100) for monitoring physiological parameters of a patient comprising:

a circuit (200) for mimicking a driven right leg electrode using a chest reference electrode as proxy therefor; the circuit comprising:

a connection (202) to a first electrocardiogram electrode (108, 109);  
 a connection (203) to a second electrocardiogram electrode (108, 109);  
 a connection to a reference electrocardiogram electrode (110); and,  
 an amplifier (204);

the electrode connections (202, 204) all connected to the amplifier (204); the amplifier (204) maintaining the voltage of the first and second electrodes (108, 109) level, the proxy driven right leg signal being measurable using the reference electrode (110),

wherein the circuit is a flexible circuit (107) embedded in a flat elastic substrate (105) having a top surface (101) and a bottom surface (102), the flexible circuit (107) having

(i) the electrodes (108, 109, 110) mounted in and communicative through the bottom surface (102) of the flat elastic substrate (105), the electrodes (108, 109, 110) being capable of electrical communication with the patient, and the circuit (200) further having

(ii) at least one signal processing module for accepting signals from the electrodes and transforming such signals for storage as patient data;

(iii) at least one memory module for accepting and storing patient data,

(iv) at least one data communication module for transferring stored patient data to an external device, and

(v) a control module for controlling the timing and operation of the electrodes, the at least one signal processing module, the at least one memory module, and the at least one data communication module, the control module capable of receiving commands to implement transfer of patient data by the at least one data communication module and to erase and/or wipe patient data from the at least one memory module;

**characterized by**

an anisotropically conductive adhesive (113; 113a) removably attached to the bottom surface (102) of the flat elastic substrate (105), the anisotropically conductive adhesive (113; 113a) capable of adhering to skin of the patient and of conducting an electrical signal substantially only in a direction perpendicular to the skin, the anisotropically conductive adhesive (113a) including non-conductive portions (113b) and conductive portions (113c), the conductive portions (113c) being disposed in conductive contact with the electrodes (108, 109, 110).

2. The device of claim 1, further comprising an optical blood sensor and the electrodes include an electrode for measuring electrical signals from said patient's heart.

3. The device of claim 1 or 2, wherein said at least one data communication module is capable of transmitting said patient data by wireless signals to an external device.

4. The device of claim 3, wherein said external device receiving said patient data is a signal relay device.

5. The device of claim 1 or 2, wherein said flexible circuit is capable of being powered wirelessly.

6. The device of claim 1 or 2, wherein said at least one signal processing module receives a signal from at least one electrode from measuring electrical signals from said patient's heart and a signal from a driven right leg circuit for reducing common mode noise from said patient data.

7. A system for monitoring physiological parameters of a patient comprising the device of claim 1; and a computer for accepting patient data from said data communication module and for displaying the patient data and/or for generating an alert if values of patient data exceed predetermined limits.

8. A method for reducing noise in cardiac monitoring using a wearable monitoring device according to claim 1; the method comprising:

applying the wearable monitoring device to a subject; including:

using the anisotropically conductive adhesive (113a) having at least one conductive portion (113c); and

using circuitry adaptations for the at least one electrode (108, 109, 110) to act as a proxy driven- right-leg electrode;

collecting data representative of physiological signals; and

analyzing the data.

9. The method of claim 8, further comprising:  
transmitting the data from the wearable device.

10. The method of claim 8 further comprising;  
transmitting the data from the wearable device; and,  
storing the data prior to one or both of transmitting or analyzing the data.

11. The method of any of claims 8 - 10, wherein circuitry adaptations comprise:

a first electrode;  
a second electrode; and  
a third electrode being a proxy driven-right-leg electrode configured to mimic a right leg electrode; the third electrode being affixed on the subject on the chest of the subject;  
a voltage or current driver operatively connected to the third electrode and the first and second electrodes to drive one or both a voltage or current to the third electrode;  
one or more of a bias or reference voltage or ground voltage configured to be operatively associated with the third electrode and the first and second electrodes; and the method further comprises driving by application of a voltage or current, to the third electrode, maintaining one or both of: the voltage of the first electrode and second electrode at a relationship to the bias voltage; or the voltage of the first electrode and second electrode at a relationship, other than the common mode voltage of one or a multiple additional electrodes, to the voltage of at least one additional electrode; and generating an output representative of a physiological signal.

12. The device of claim 1, further comprising an insulative structure (113d) provided on a bottom surface (102), between the electrodes (108, 109, 110).

## Patentansprüche

1. Ein Gerät (100) zur Überwachung von physiologischen Parametern eines Patienten umfassend:

eine Schaltung (200) zur Nachahmung von einer DRL (*Driven-Right-Leg*)-Elektrode unter Verwendung von einer stellvertretenden Brustreferenzelektrode; wobei die Schaltung folgendes umfasst:

einen Anschluss (202) an eine erste EKG-Elektrode (108, 109);  
einen Anschluss (203) an eine zweite EKG-Elektrode (108, 109);  
einen Anschluss an eine Referenz-EKG-Elektrode (110); und  
einen Verstärker (204);  
wobei die Elektrodenanschlüsse (202, 204) alle mit dem Verstärker (204) verbunden sind; wobei der Verstärker (204) die Spannung der ersten und der zweiten Elektroden (108, 109) bei einem Wert hält, wobei das stellvertretende DRL-Signal mittels der Referenzelektrode (110) gemessen werden kann,

wobei die Schaltung eine flexible Schaltung (107) ist, die in einem flachen elastischen Substrat (105) eingebettet ist, das eine obere Fläche (101) und eine untere Fläche (102) hat, wobei die flexible Schaltung (107) folgendes hat

(i) die Elektroden (108, 109, 110), die auf der unteren (102) Fläche des flachen elastischen Substrats (105) montiert und durch diese verbunden sind, wobei die Elektroden (108, 109, 110) mit dem Patienten elektrisch verbunden werden können, und wobei die Schaltung (200) weiterhin folgendes hat  
(ii) mindestens ein Signalverarbeitungsmodul zur Annahme von aus den Elektroden empfangenen Signalen und zur Umwandlung der Signale zur Speicherung als Patientendaten;  
(iii) mindestens ein Speichermodul zur Annahme und zur Speicherung von Patientendaten,  
(iv) mindestens ein Datenverbindungsmodul zur Übertragung von gespeicherten Patientendaten an eine externe Vorrichtung, und  
(v) ein Steuermodul zur Steuerung der Zeitabstimmung und des Betriebs der Elektroden, des mindestens einen Signalverarbeitungsmoduls, des mindestens einen Speichermoduls, und des mindestens einen Datenverbindungsmoduls, wobei das Steuermodul Befehle empfangen kann, um die Übertragung von Patientendaten durch das mindestens eine Datenverbindungsmodul durchzuführen und Patientendaten aus dem mindestens einen Speichermodul zu löschen und/oder zu entfernen; **gekennzeichnet durch**

einen anisotropisch leitenden Klebstoff (113; 113a), der an der unteren Fläche (102) des flachen elastischen Substrats (105) entfernter befestigt ist, wobei der anisotropisch leitende Klebstoff (113; 113a) an die Haut des Patienten haften kann und ein elektrisches Signal im Wesentlichen nur in einer zur Haut senkrechten Richtung leiten kann, wobei der anisotropisch leitende Klebstoff (113a) nicht leitende Teile (113b) und leitende Teile (113c) umfasst, wobei die leitenden Teile (113c) im leitenden Kontakt mit den Elektroden (108, 109, 110) angeordnet sind.

2. Das Gerät des Anspruchs 1, weiterhin umfassend einen optischen Blutsensor und wobei die Elektroden eine Elektrode zur Messung von elektrischen Signalen aus dem Herzen des Patienten umfassen.

3. Das Gerät des Anspruchs 1 oder 2, wobei das mindestens eine Datenverbindungsmodul die Patientendaten an eine externe Vorrichtung durch drahtlose Signale übertragen kann.

4. Das Gerät des Anspruchs 3, wobei die externe Vorrichtung, welche die Patientendaten empfängt, ein Signalrelais ist.

5. Das Gerät des Anspruchs 1 oder 2, wobei die flexible Schaltung drahtlos angetrieben werden kann.

6. Das Gerät des Anspruchs 1 oder 2, wobei das mindestens eine Signalverarbeitungsmodul ein Signal aus mindestens einer Elektrode zur Messung von elektrischen Signalen aus dem Herzen des Patienten und ein Signal aus einer DRL-Schaltung zur Reduktion von Gleichtaktrausch aus den Patientendaten empfängt.

7. Ein System zur Überwachung von physiologischen Parametern von einem Patienten umfassend das Gerät des Anspruchs 1; und einen Computer zur Annahme von Patientendaten aus dem Datenverbindungsmodul und zur Anzeige der Patientendaten und/oder zur Erzeugung von einer Warnmeldung, wenn Werte der Patientendaten vorherbestimmte Schwellenwerte überschreiten.

8. Ein Verfahren zur Rauschreduktion bei einer Herzüberwachung unter Verwendung von einem tragbaren Überwachungsgerät nach Anspruch 1; wobei das Verfahren folgendes umfasst:

das Anwenden des tragbaren Überwachungsgeräts auf einen Patienten; umfassend:  
das Verwenden des anisotropisch leitenden Klebstoffs (113a), der mindestens einen leitenden Teil (113c) hat; und  
das Verwenden von Schaltungsanpassungen, damit die mindestens eine Elektrode (108, 109, 110) als stellvertretende DRL-Elektrode dient;  
das Sammeln von Daten, die für physiologische Signale repräsentativ sind; und  
das Analysieren der Daten.

9. Das Verfahren des Anspruchs 8, weiterhin umfassend:  
das Übertragen der Daten aus dem tragbaren Gerät.

10. Das Verfahren des Anspruchs 8 weiterhin umfassend;  
das Übertragen der Daten aus dem tragbaren Gerät; und,  
das Speichern der Daten vor der Übertragung oder vor der Analyse der Daten, oder vor den beiden.

11. Das Verfahren von einem der Ansprüche 8 - 10, wobei die Schaltungsanpassungen folgendes umfassen:

eine erste Elektrode;  
eine zweite Elektrode; und  
eine dritte Elektrode, die eine stellvertretende DRL-Elektrode ist, die konfiguriert ist, um eine Right-Leg-Elektrode nachzuahmen; wobei die dritte Elektrode an dem Patienten an der Brust des Patienten befestigt wird;  
einen Spannungs- oder Stromtreiber, der mit der dritten Elektrode und mit der ersten und der zweiten Elektroden betriebsfähig verbunden ist, um eine Spannung oder einen Strom, oder beide, an die dritte Elektrode zu treiben;  
eine oder mehrere aus einer Vorspannung oder Bezugsspannung oder Erdspannung, die konfiguriert ist bzw. sind, um betriebsfähig mit der dritten Elektrode und mit der ersten und der zweiten Elektroden verknüpft zu werden; und das Verfahren weiterhin folgendes umfasst:  
das Antreiben durch die Anwendung von einer Spannung oder eines Stroms auf die dritte Elektrode,  
das Halten von einer oder beiden von: der Spannung der ersten Elektrode und der zweiten Elektrode bei einem

Verhältnis zu der Vorspannung; oder der Spannung der ersten Elektrode und der zweiten Elektrode bei einem Verhältnis, das verschieden von der Gleichtaktspannung von einer oder von mehreren zusätzlichen Elektroden ist, zu der Spannung von mindestens einer zusätzlichen Elektrode; und das Erzeugen von einem Ausgang, der für ein physiologisches Signal repräsentativ ist.

5

12. Das Gerät des Anspruchs 1, weiterhin umfassend eine auf einer unteren Fläche (102), zwischen den Elektroden (108, 109, 110), bereitgestellte isolierende Struktur (113d).

10 **Revendications**

1. Un dispositif (100) pour surveiller des paramètres physiologiques d'un patient comprenant:

15

un circuit (200) pour reproduire une électrode DRL (*driven right leg*, « pilotée » par la jambe droite) en utilisant une électrode de référence de poitrine comme une électrode proxy de celle-là ; le circuit comprenant :

20

une connexion (202) à une première électrode d'électrocardiogramme (108, 109) ;  
 une connexion (203) à une deuxième électrode d'électrocardiogramme (108, 109) ;  
 une connexion à une électrode d'électrocardiogramme de référence (110) ; et  
 un amplificateur (204) ;  
 les connexions d'électrode (202, 204) étant toutes connectées à l'amplificateur (204) ; l'amplificateur (204) maintenant la tension des électrodes première et deuxième (108, 109) à un niveau donné, le signal DRL proxy étant mesurable moyennant l'électrode de référence (110),

25

dans lequel le circuit est un circuit flexible (107) intégré dans un substrat élastique plat (105) ayant une surface supérieure (101) et une surface inférieure (102), le circuit flexible (107) ayant

30

(i) les électrodes (108, 109, 110) montées dans et en communication à travers la surface inférieure (102) du substrat élastique plat (105), les électrodes (108, 109, 110) étant capables d'être en communication électrique avec le patient, et le circuit (200) ayant en outre

35

(ii) au moins un module de traitement de signaux pour accepter des signaux des électrodes et transformer lesdits signaux pour le stockage comme des données du patient ;  
 (iii) au moins un module de mémoire pour accepter et stocker des données du patient,  
 (iv) au moins un module de communication de données pour transférer des données du patient stockées à un dispositif extérieur, et

40

(v) un module de contrôle pour contrôler le timing et le fonctionnement des électrodes, l'au moins un module de traitement de signaux, l'au moins un module de mémoire, et l'au moins un module de communication de données, le module de contrôle étant capable de recevoir des commandes pour implémenter le transfert de données du patient par l'au moins un module de communication de données et pour effacer et/ou éliminer des données du patient de l'au moins un module de mémoire ; **caractérisé par** un adhésif à conduction anisotropique (113 ; 113a) attaché de façon amovible à la surface inférieure (102) du substrat élastique plat (105), l'adhésif à conduction anisotropique (113 ; 113a) étant capable de s'adhérer à la peau du patient et de conduire un signal électrique essentiellement seulement dans une direction perpendiculaire à la peau, l'adhésif à conduction anisotropique (113a) incluant des parties non conductrices (113b) et des parties conductrices (113c), les parties conductrices (113c) étant disposées en contact de conduction avec les électrodes (108, 109, 110).

45

2. Le dispositif de la revendication 1, comprenant en outre un détecteur de sang optique et les électrodes incluant une électrode pour mesurer des signaux électriques du coeur dudit patient.

50

3. Le dispositif de la revendication 1 ou 2, dans lequel ledit au moins un module de communication de données est capable de transmettre lesdites données du patient moyennant de signaux sans fil à un dispositif extérieur.

55

4. Le dispositif de la revendication 3, dans lequel ledit dispositif extérieur recevant lesdites données du patient est un relais de signalisation.

5. Le dispositif de la revendication 1 ou 2, dans lequel ledit circuit flexible est capable d'être alimenté sans fil.

## EP 2 903 509 B1

6. Le dispositif de la revendication 1 ou 2, dans lequel ledit au moins un module de traitement de signaux reçoit un signal d'au moins une électrode pour mesurer des signaux électriques du coeur dudit patient et un signal d'un circuit DRL pour réduire le bruit de mode commun des données dudit patient.
- 5 7. Un système pour surveiller des paramètres physiologiques d'un patient comprenant le dispositif de la revendication 1 ; et  
un ordinateur pour accepter des données du patient dudit module de communication de données et pour afficher les données du patient et/ou pour générer un avertissement si des valeurs de données du patient dépassent des valeurs de seuil prédéterminées.
- 10 8. Un procédé pour réduire le bruit dans la surveillance cardiaque en utilisant un dispositif de surveillance portable selon la revendication 1 ; le procédé comprenant :  
appliquer le dispositif de surveillance portable à un patient ; incluant :
- 15 utiliser l'adhésif à conduction anisotropique (113a) ayant au moins une partie conductrice (113c) ; et  
utiliser des adaptations de circuit de manière à ce que l'au moins une électrode (108, 109, 110) agisse comme une électrode DRL proxy ;  
recueillir des données représentatives de signaux physiologiques ; et  
analyser les données.
- 20 9. Le procédé de la revendication 8 comprenant en outre :  
transmettre les données du dispositif portable.
- 25 10. Le procédé de la revendication 8 comprenant en outre ;  
transmettre les données du dispositif portable ; et,  
stocker les données avant de transmettre ou d'analyser les données, ou avant de tous deux.
- 30 11. Le procédé de l'une quelconque des revendications 8 - 10, dans lequel les adaptations de circuit comprennent :  
une première électrode ;  
une deuxième électrode ; et  
une troisième électrode étant une électrode DRL proxy configurée pour reproduire une électrode de la jambe droite ; la troisième électrode étant fixée sur l'individu sur la poitrine de l'individu ;  
35 un circuit d'attaque de tension ou de courant connecté de manière opérationnelle à la troisième électrode et aux électrodes première et deuxième pour faire une attaque en tension ou en courant, ou toutes deux, à la troisième électrode ;  
une ou plusieurs d'une tension de polarisation ou de référence ou d'une tension de terre configurée pour être liée de manière opérationnelle à la troisième électrode et aux électrodes première et deuxième ;  
40 et le procédé comprenant en outre  
attaquer moyennant l'application d'une tension ou d'un courant, à la troisième électrode,  
maintenir une ou toutes deux de : la tension de la première électrode et la deuxième électrode à un rapport à la tension de polarisation ; ou la tension de la première électrode et la deuxième électrode à un rapport, différente de la tension de mode commun d'une ou de plusieurs électrodes additionnelles, à la tension d'au moins une  
45 électrode additionnelle ; et  
générer une sortie représentative d'un signal physiologique.
- 50 12. Le dispositif de la revendication 1, comprenant en outre une structure isolante (113d) fournie sur une surface inférieure (102), entre les électrodes (108, 109, 110).
- 55

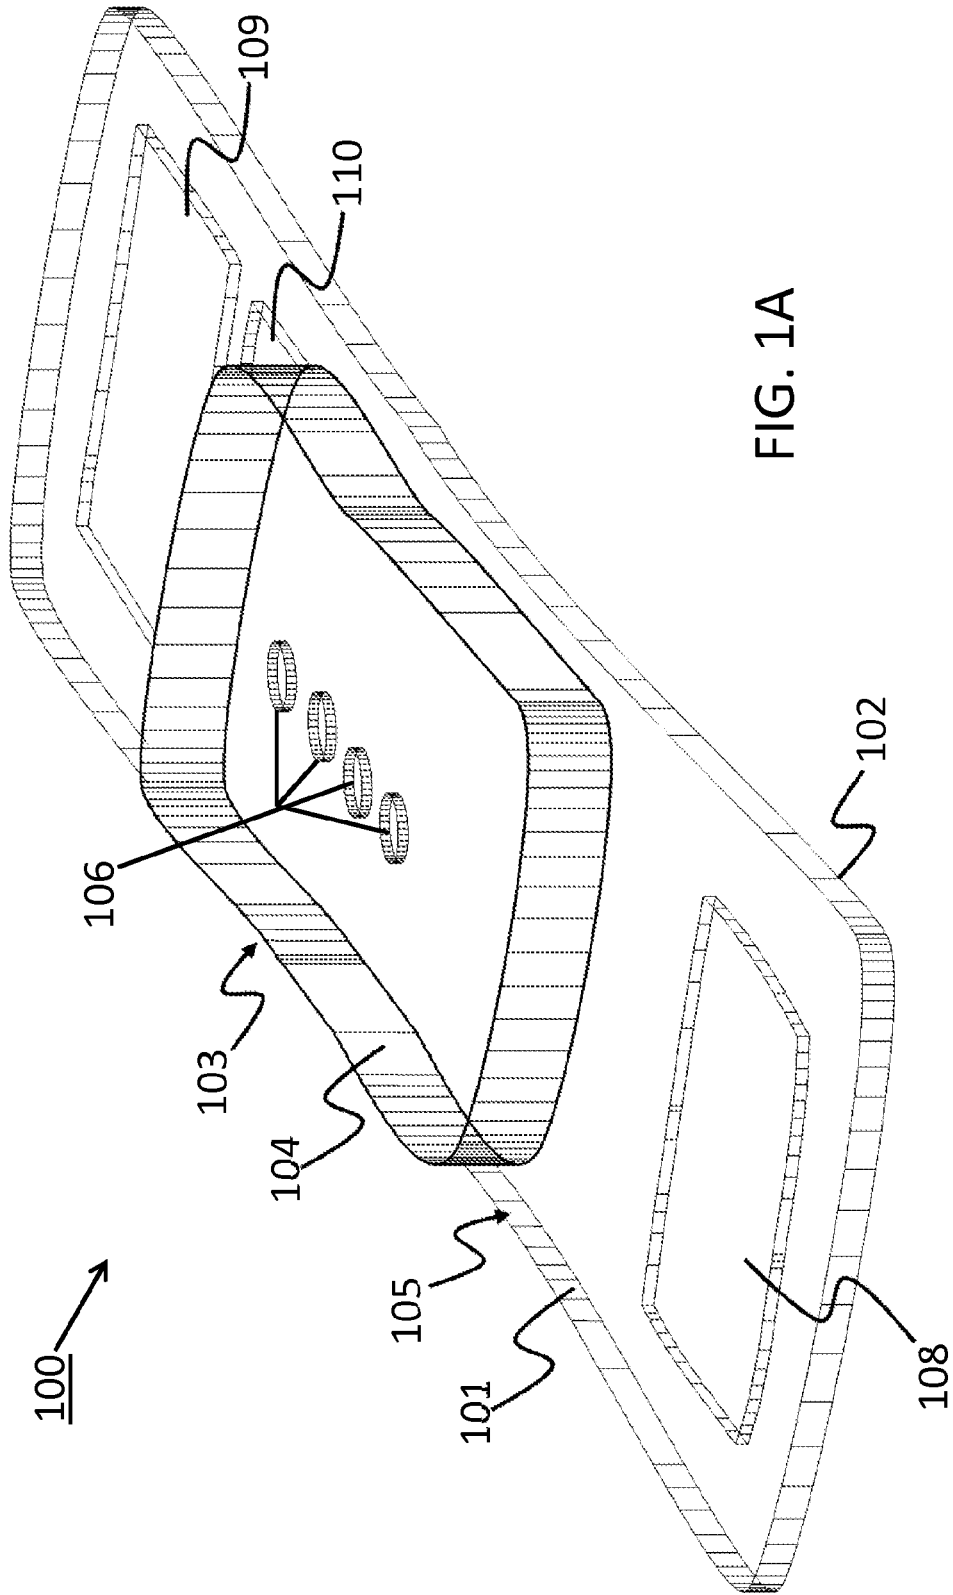


FIG. 1A

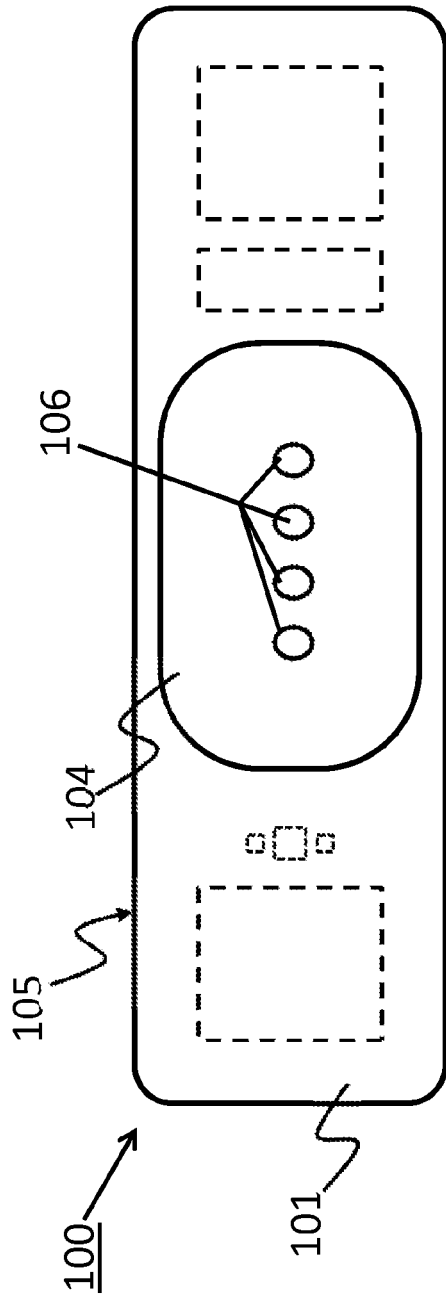


FIG. 1B

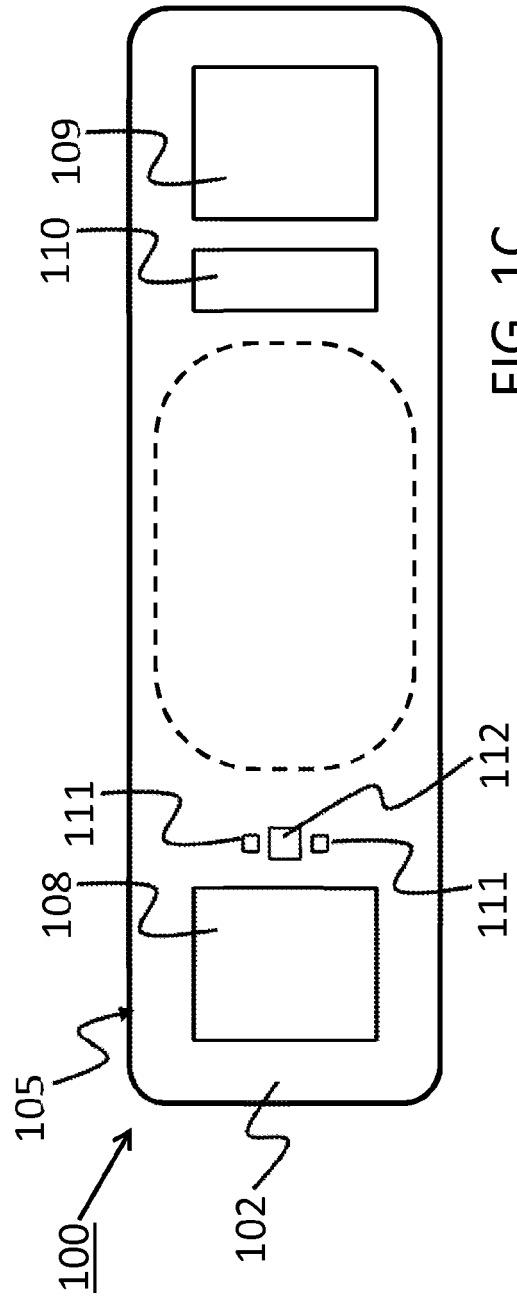


FIG. 1C

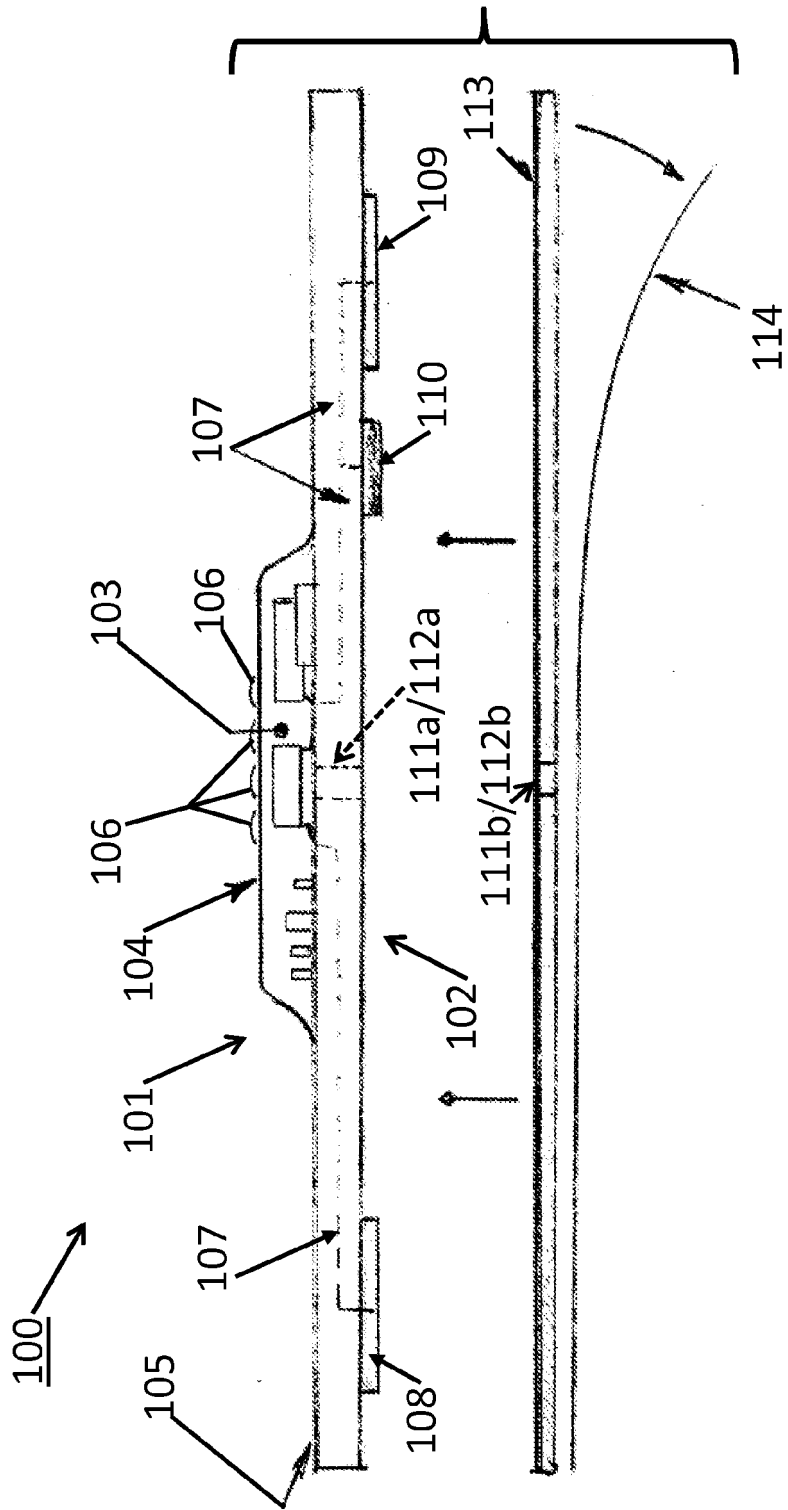


FIG. 1D

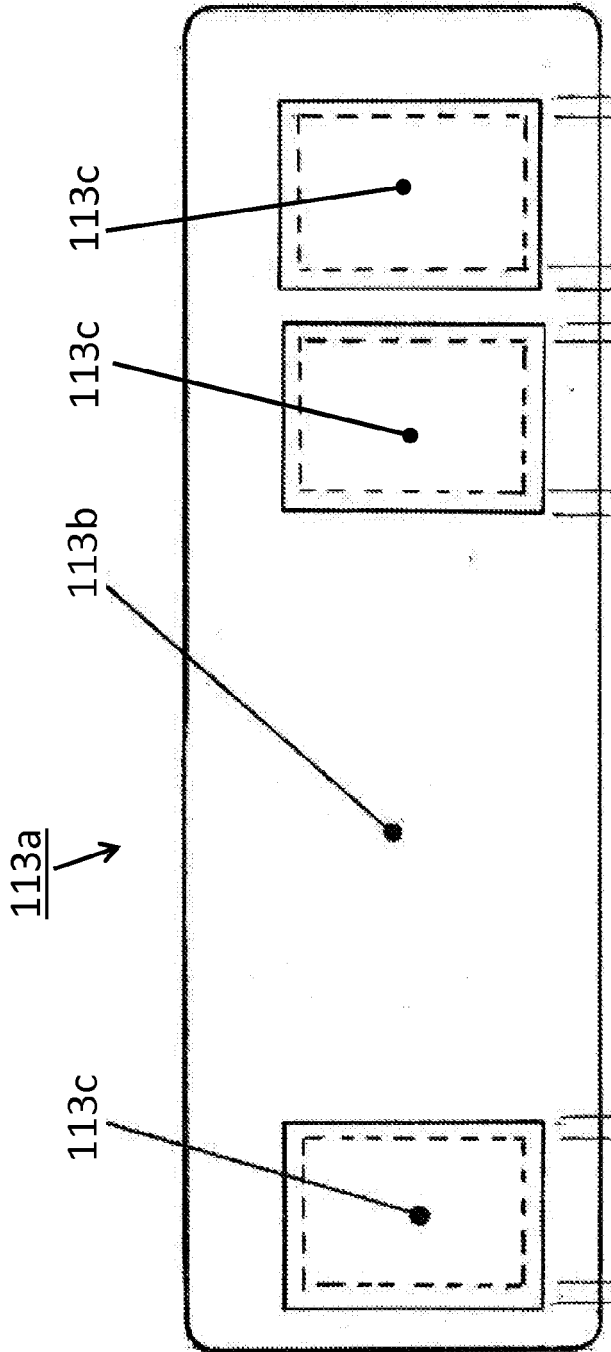


FIG. 1E

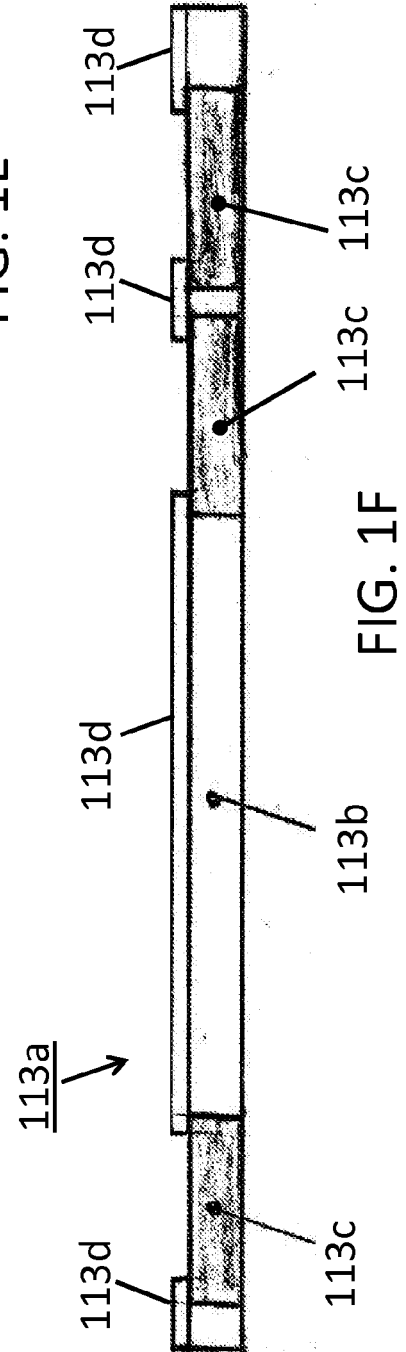


FIG. 1F

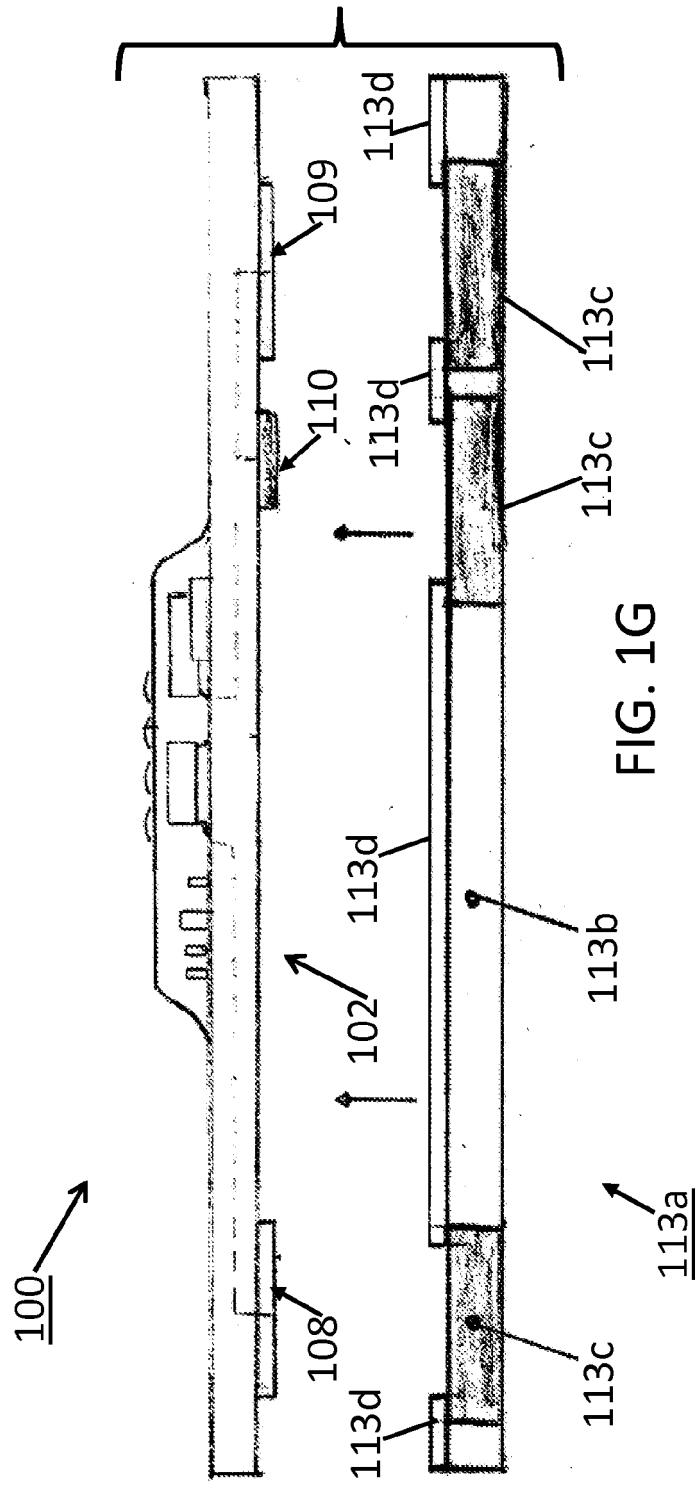


FIG. 1G

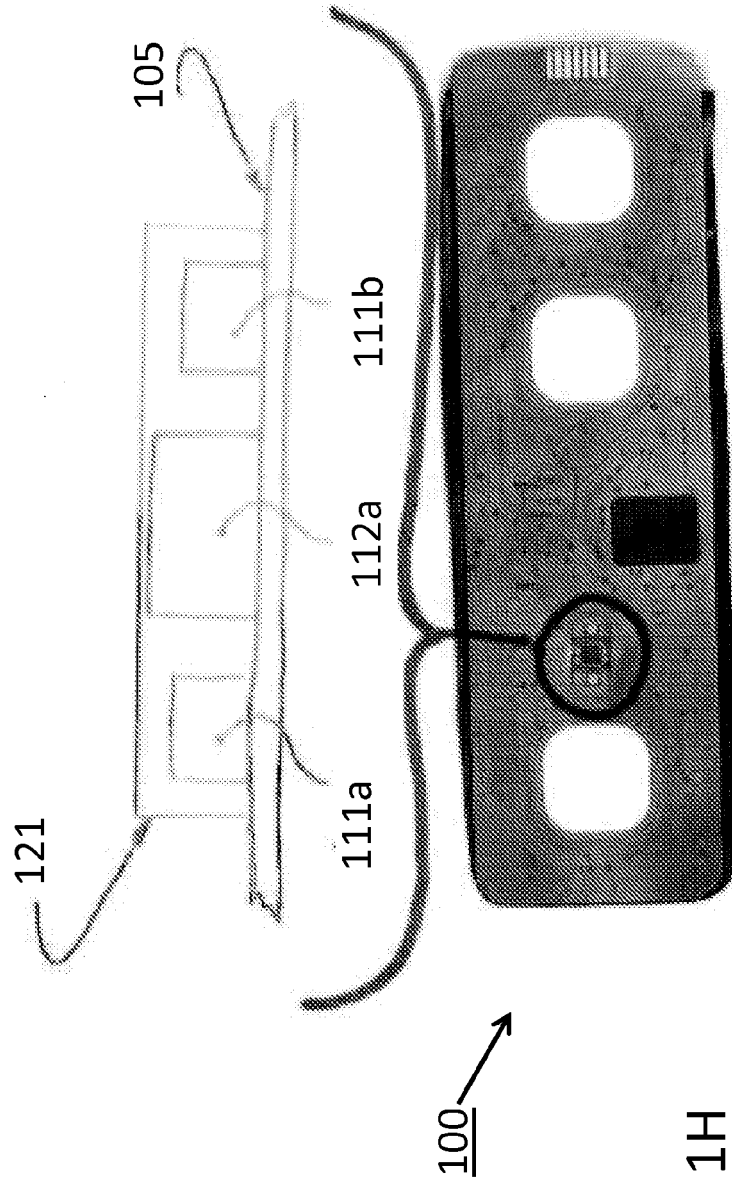


FIG. 1H

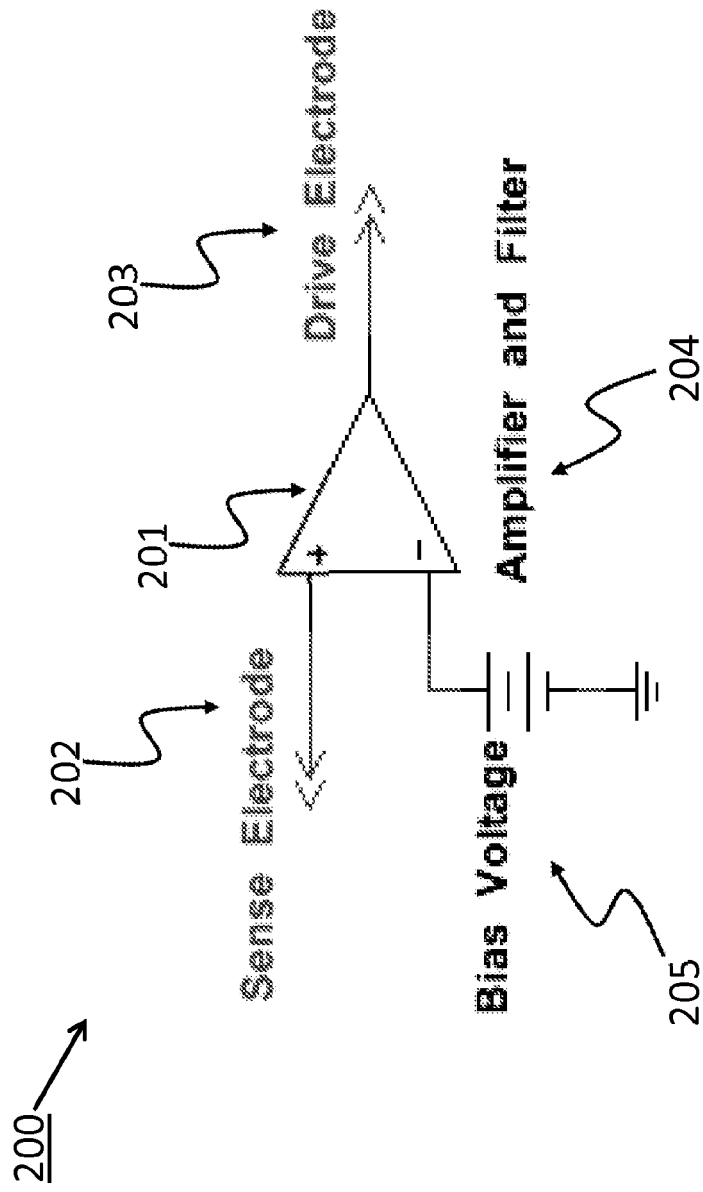


FIG. 2A

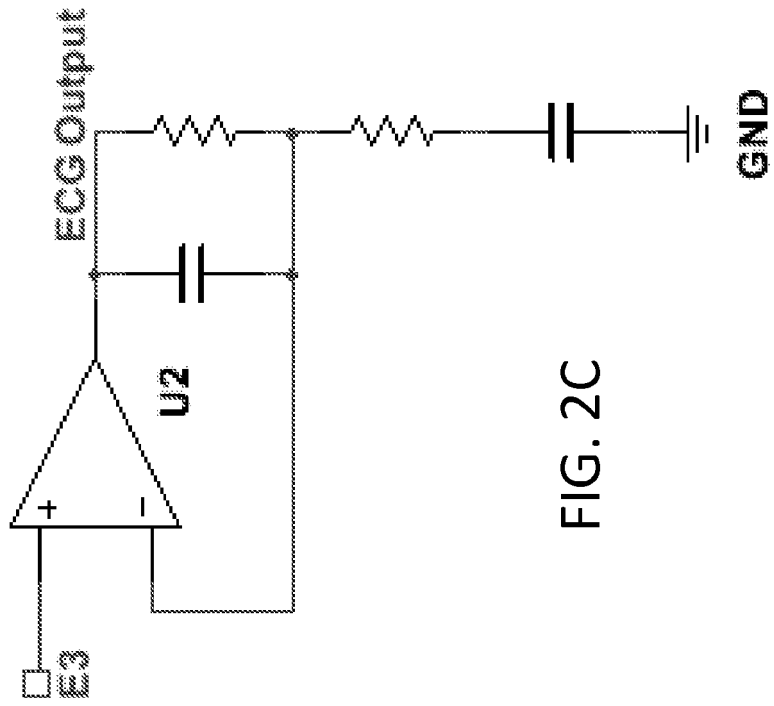


FIG. 2C

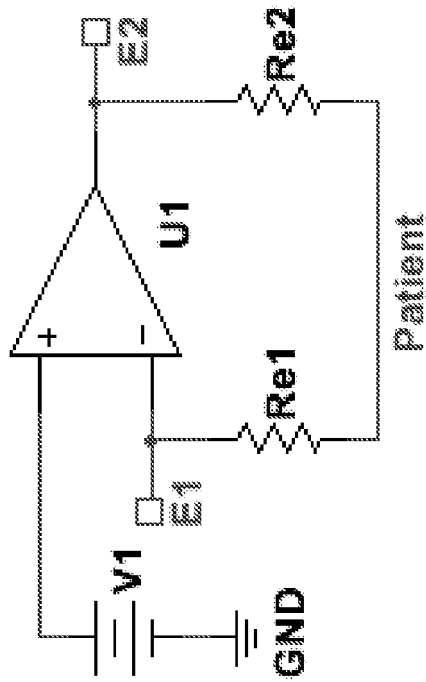


FIG. 2B

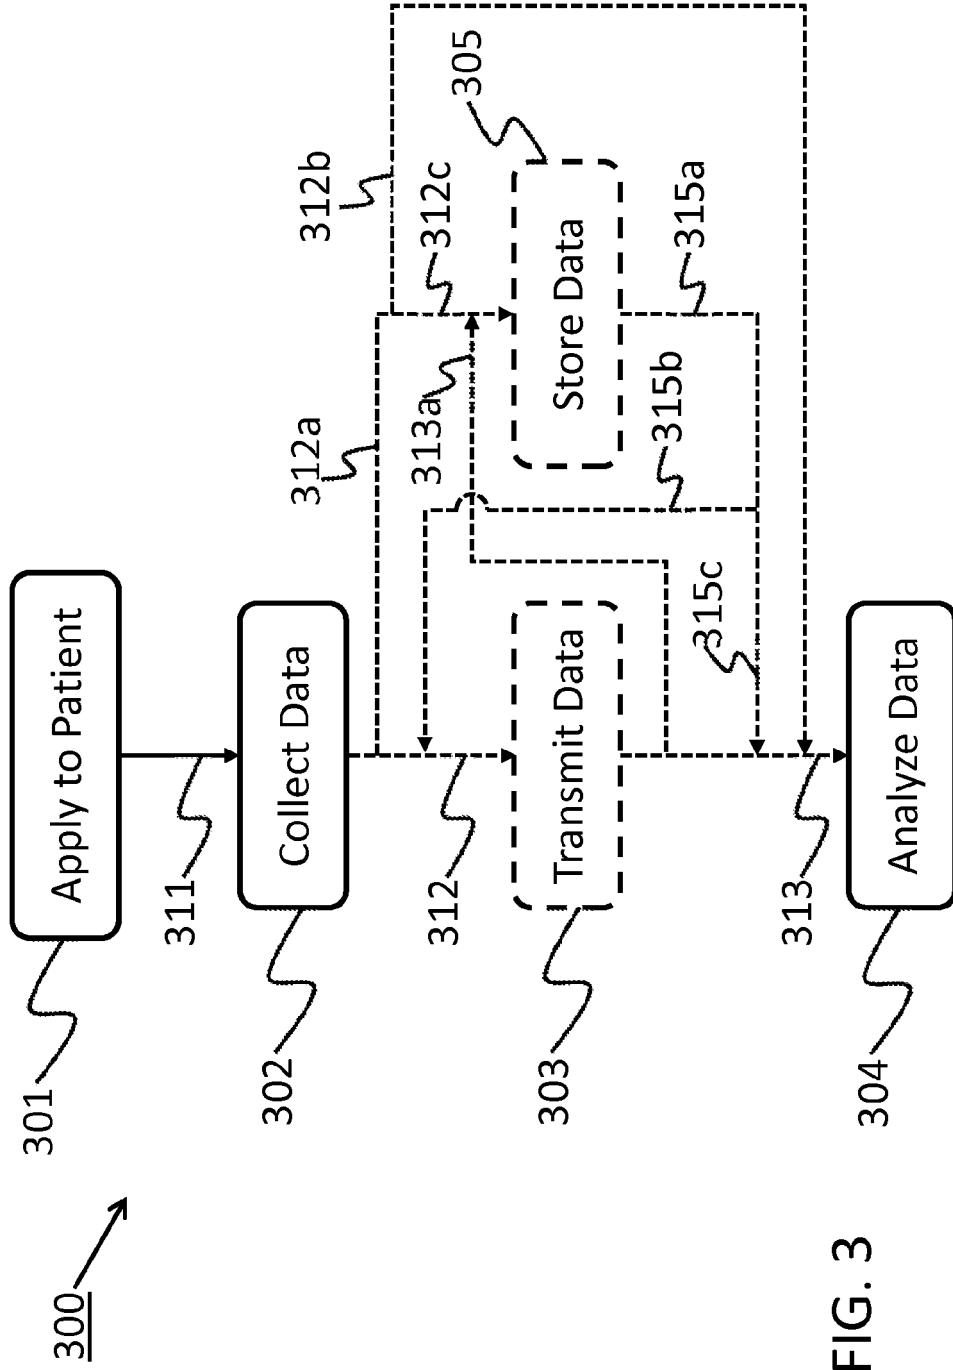


FIG. 3

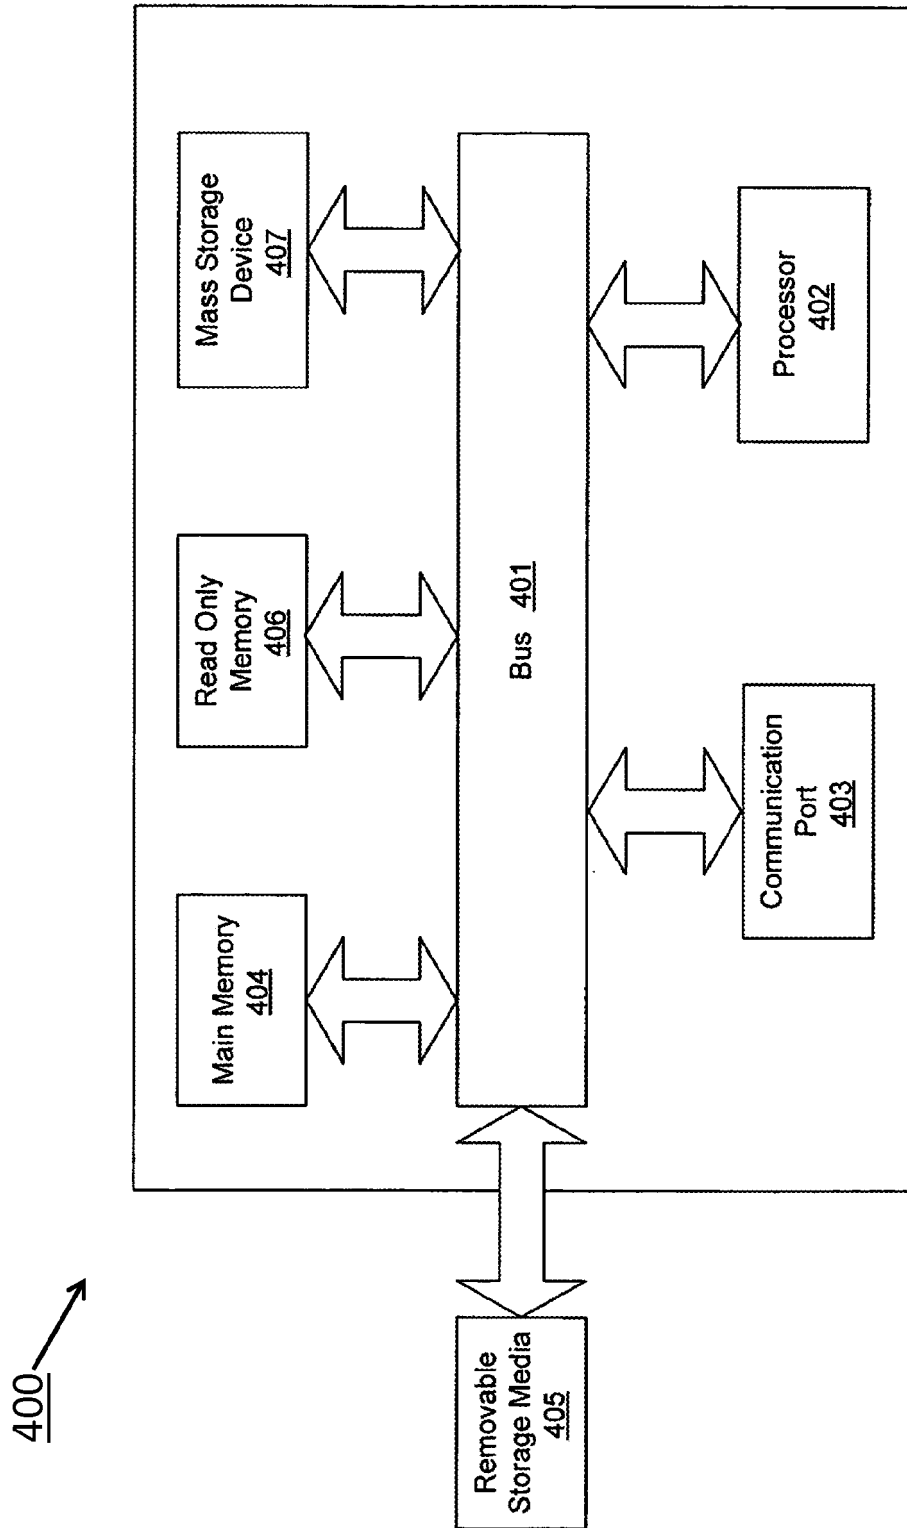


FIG. 4

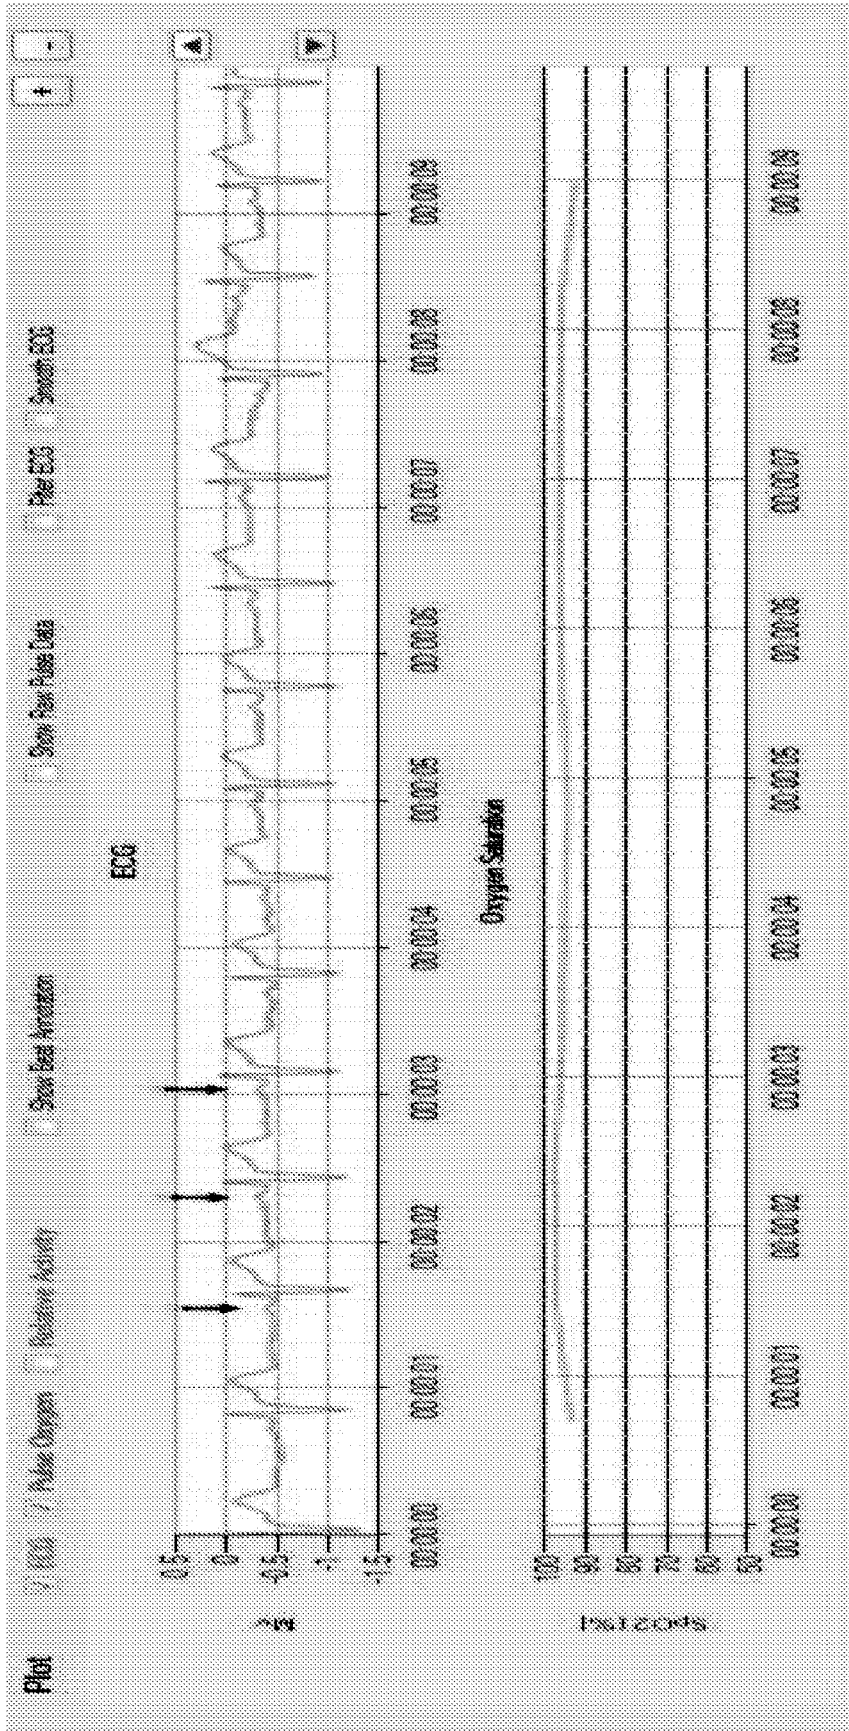


FIG. 5A

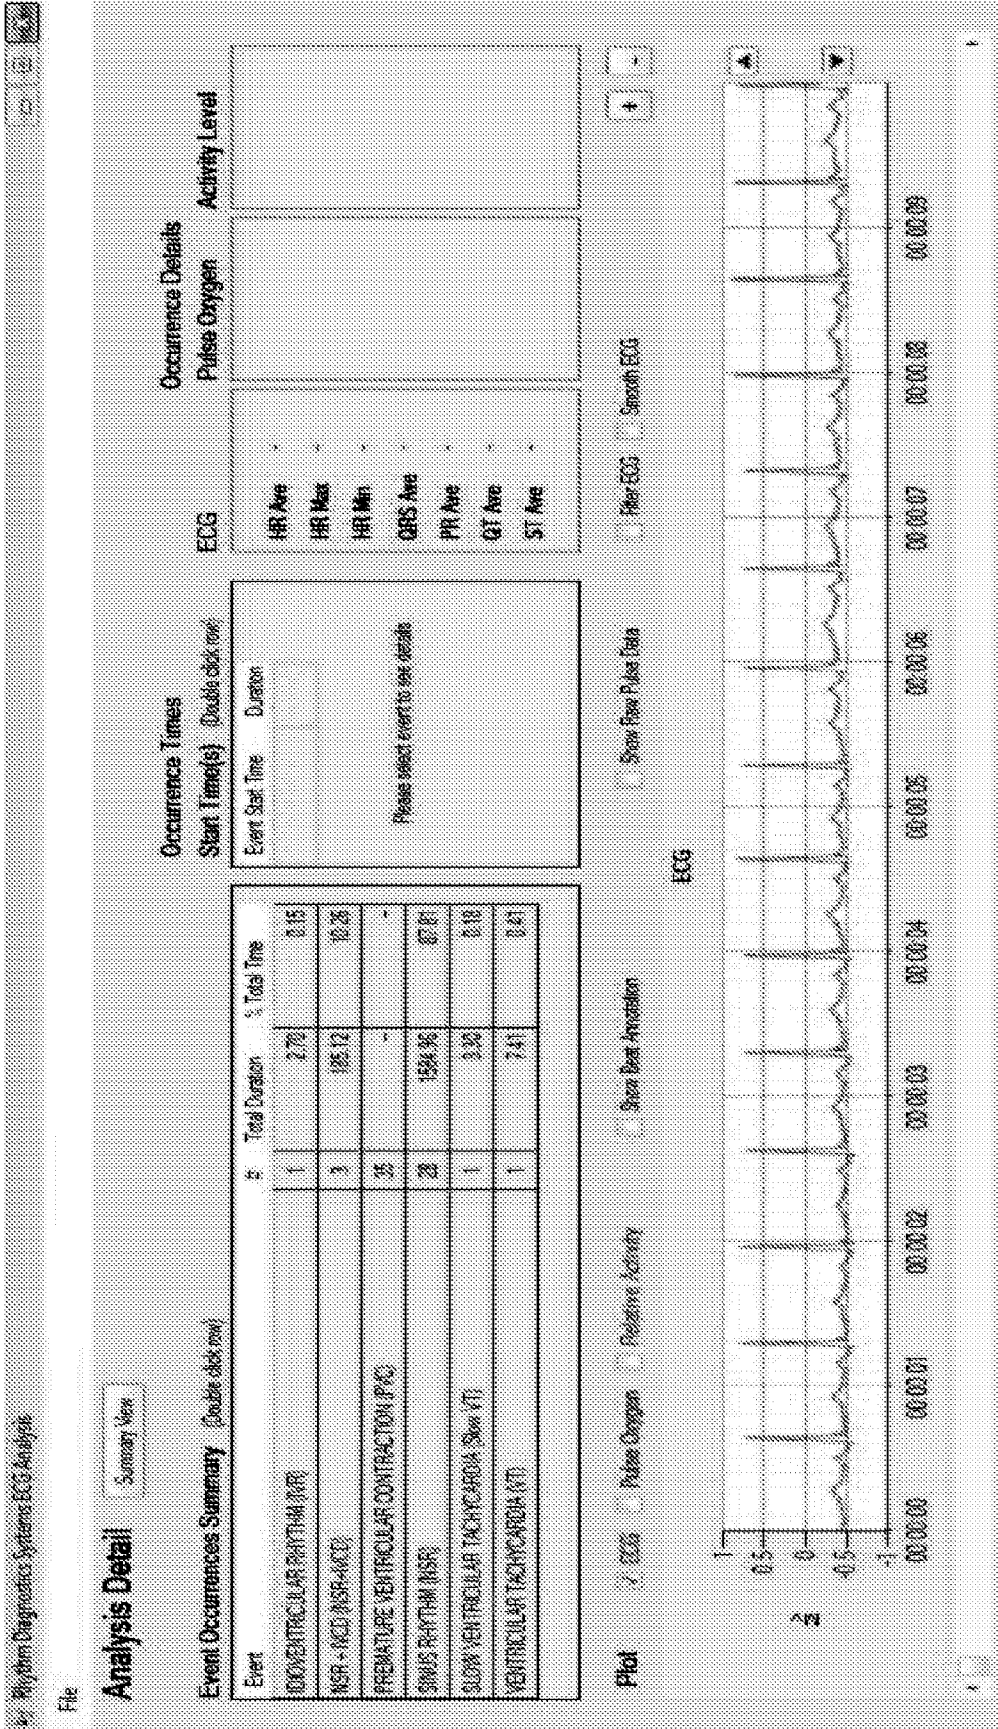


FIG. 5B

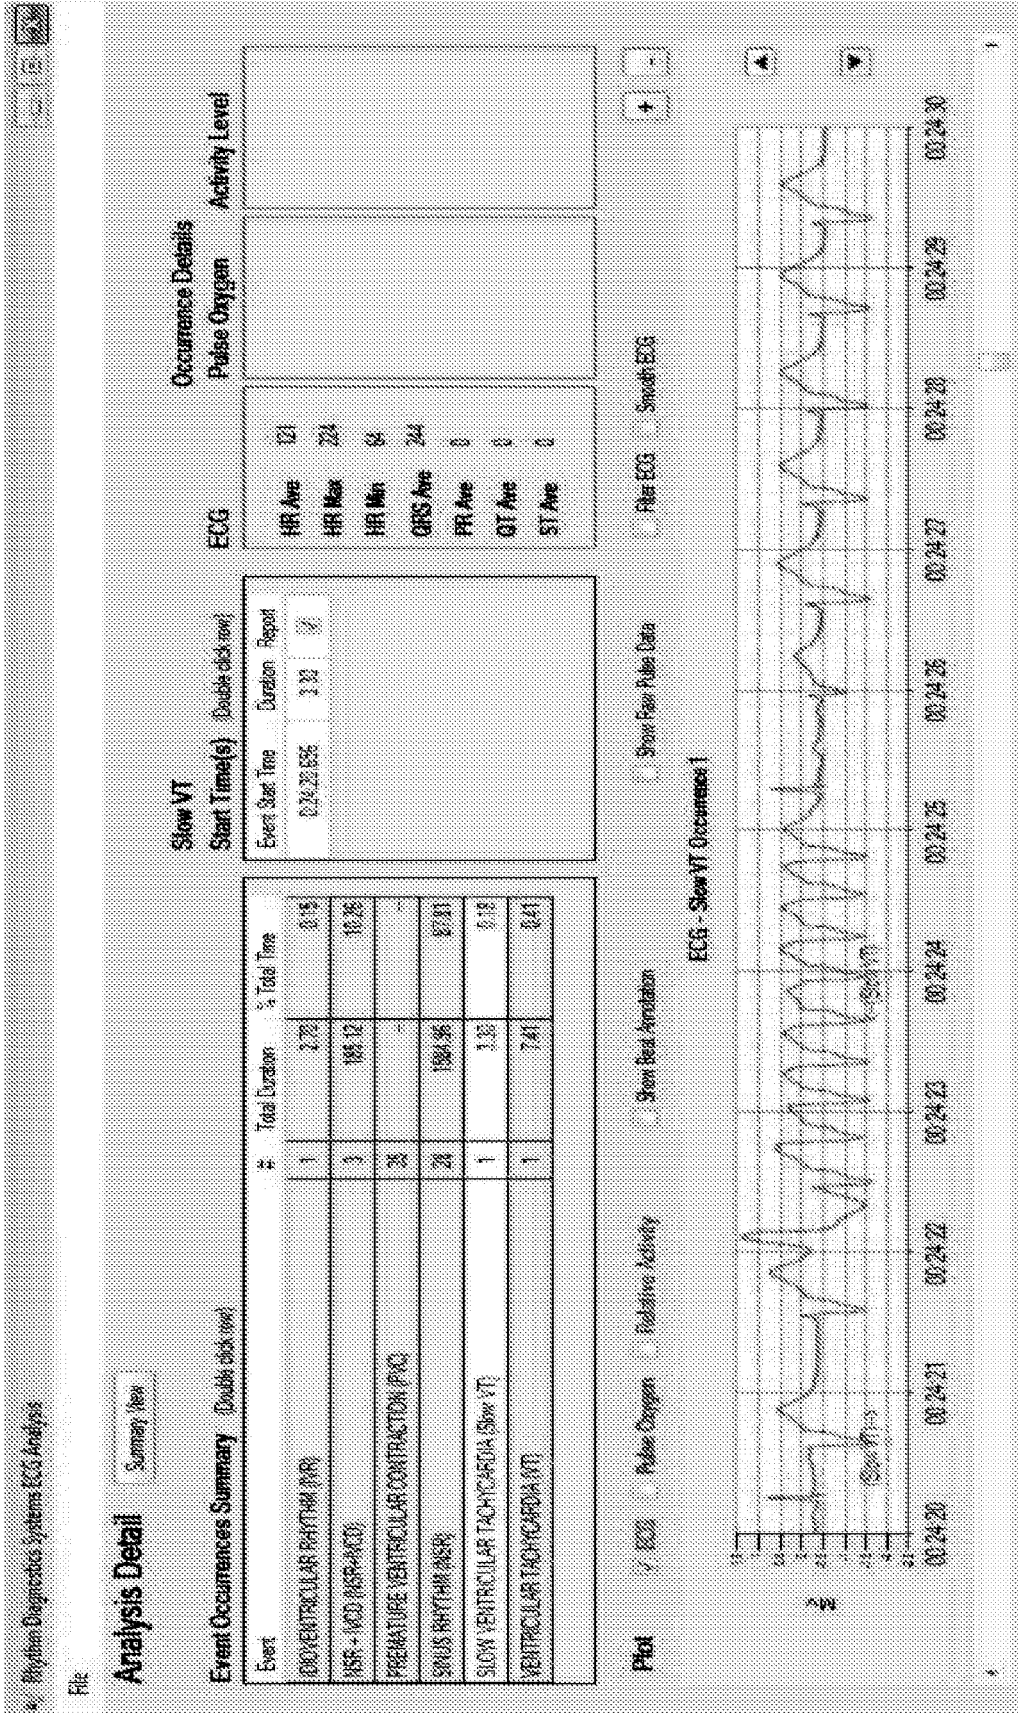


FIG. 5C

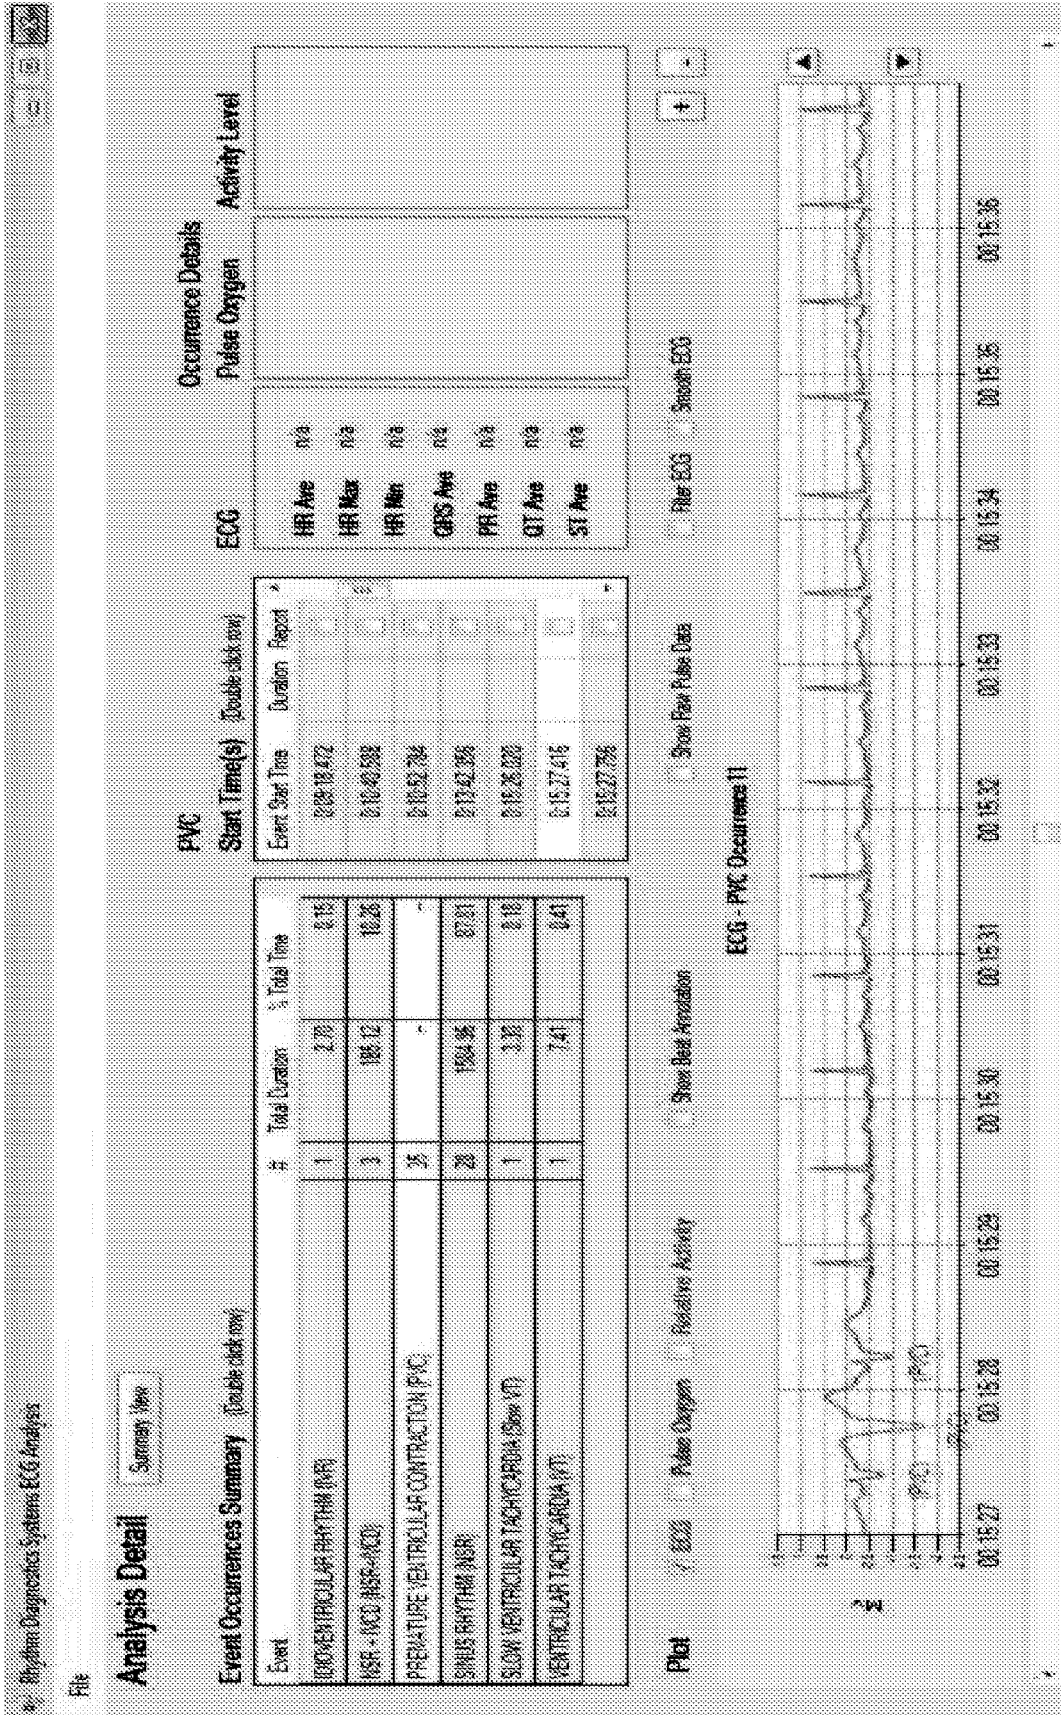


FIG. 5D

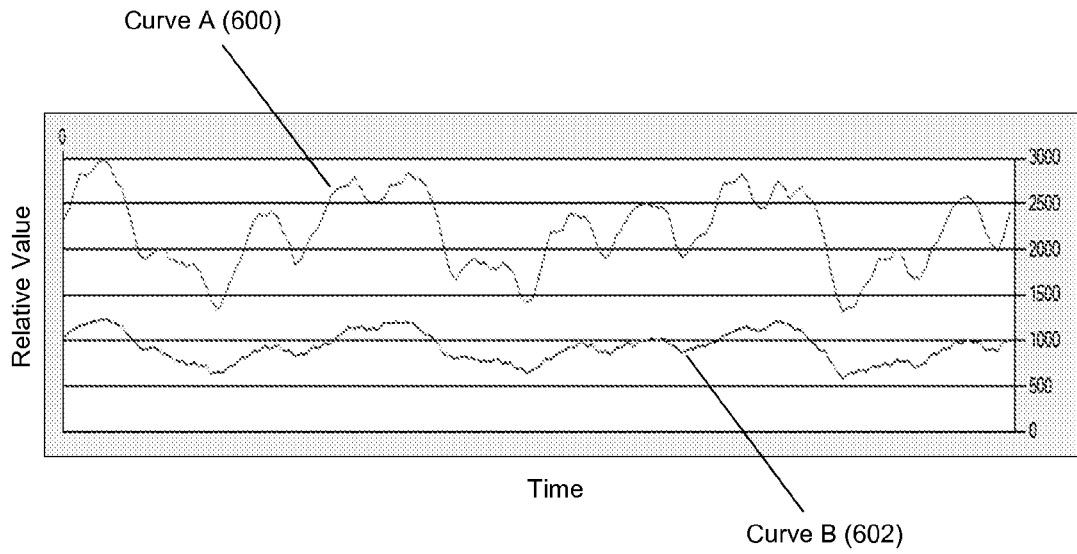


FIG. 6A

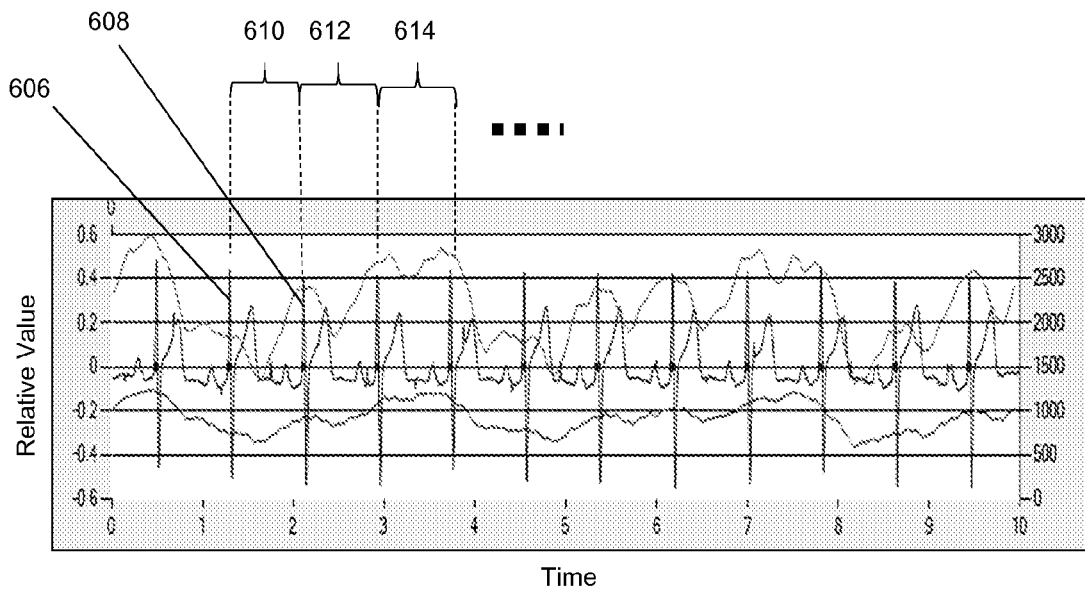


FIG. 6B

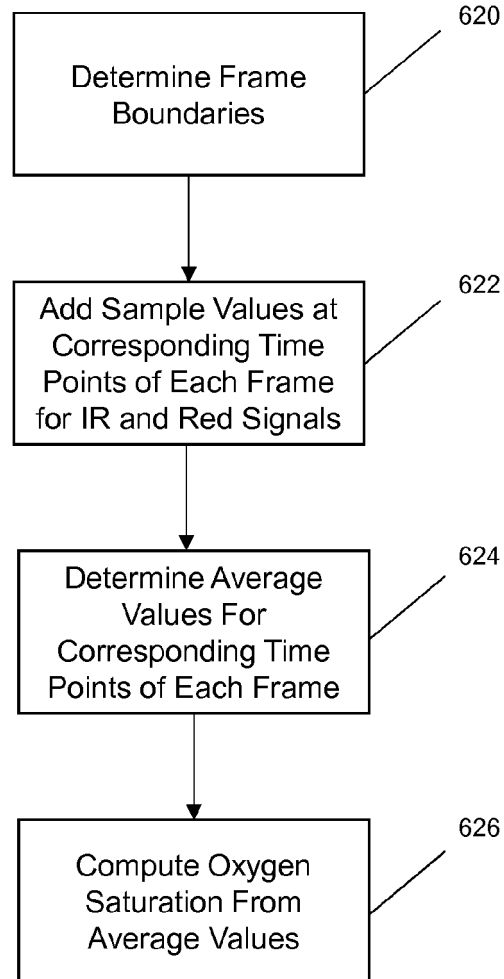


FIG. 6C

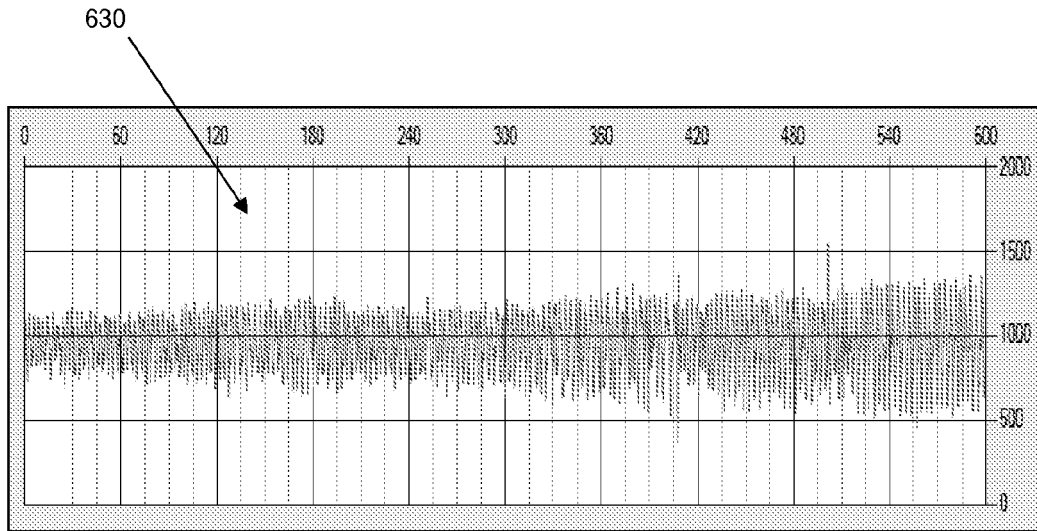


FIG. 6D

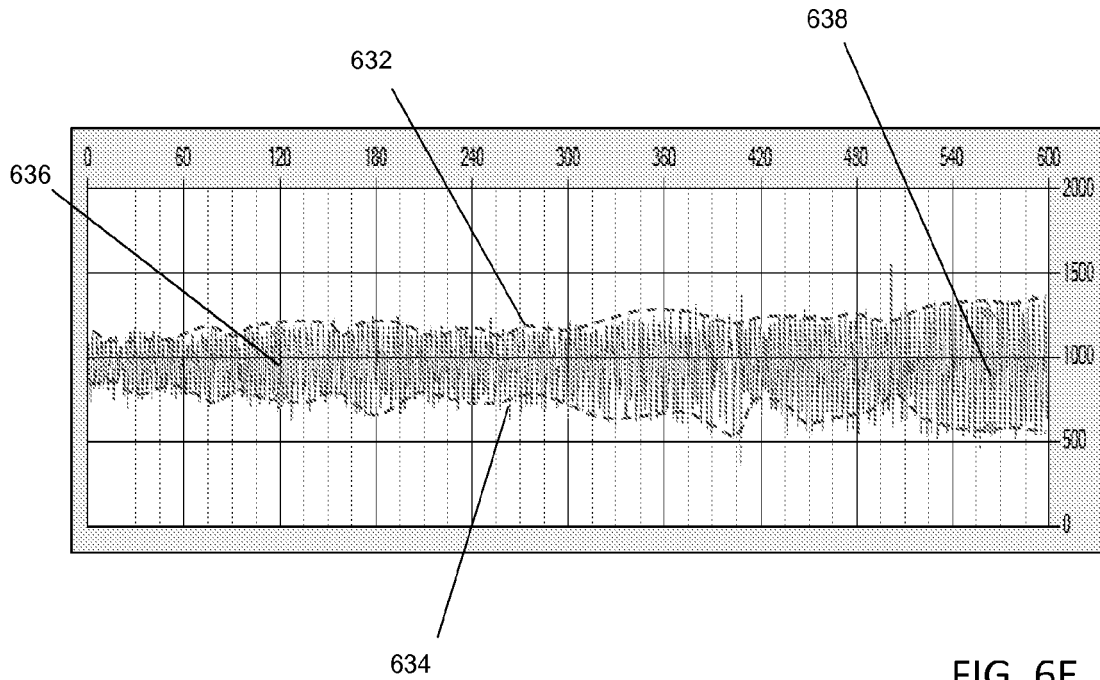


FIG. 6E

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 2008139953 A [0002]
- US 2006224072 A [0002]
- CN 202288274 [0002]
- WO 00126779 A [0055]

**Non-patent literature cited in the description**

- **WARNER et al.** *Anesthesiology*, 2008, vol. 108, 950-958 [0053]

专利名称(译)	可穿戴式心脏监护仪		
公开(公告)号	<a href="#">EP2903509A1</a>	公开(公告)日	2015-08-12
申请号	EP2013843561	申请日	2013-10-07
[标]申请(专利权)人(译)	RHYTHM诊断SYST		
申请(专利权)人(译)	RHYTHM诊断系统INC.		
当前申请(专利权)人(译)	RHYTHM诊断系统INC.		
[标]发明人	GOLDA GEORGE STEFAN MOYER DANIEL VAN ZANDT MARRIOTT MARK P ELETR SAM ONEIL BRUCE		
发明人	GOLDA, GEORGE STEFAN MOYER, DANIEL VAN ZANDT MARRIOTT, MARK P. ELETR, SAM O'NEIL, BRUCE		
IPC分类号	A61B5/0402 A61B5/00 A61B5/0205 A61B5/024 A61B5/0408 A61B5/0432 A61B5/0456 A61B5/11 A61B5/1455		
CPC分类号	A61B5/0002 A61B5/0006 A61B5/0059 A61B5/0205 A61B5/02125 A61B5/02141 A61B5/02438 A61B5/ /0261 A61B5/0295 A61B5/0402 A61B5/04085 A61B5/04087 A61B5/04325 A61B5/0456 A61B5/08 A61B5/11 A61B5/1118 A61B5/14551 A61B5/14552 A61B5/6828 A61B5/72 A61B5/7207 A61B5/721 A61B5/7214 A61B5/7275 A61B2560/0295 A61B2560/0412 A61B5/6833		
优先权	61/710768 2012-10-07 US 13/837748 2013-03-15 US		
其他公开文献	EP2903509A4 EP2903509B1		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

用于降低心脏监测中的噪声的系统，方法和设备，包括具有至少一个用于心脏监测的电极的可穿戴监测设备；在一些实施方式中，可穿戴设备使用复合粘合剂，该复合粘合剂具有邻近电极施加的至少一个导电部分；并且，在一些实施方案中，包括用于所述至少一个电极的电路适应性以充当代理驱动的右腿电极。