



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
25.01.2017 Bulletin 2017/04

(51) Int Cl.:
A61B 5/00 (2006.01) **A61B 5/0456** (2006.01)
A61B 5/042 (2006.01) **A61B 5/0408** (2006.01)
A61B 5/0428 (2006.01) **A61B 5/0432** (2006.01)
G06F 19/00 (2011.01)

(21) Application number: **16178933.4**

(22) Date of filing: **12.07.2016**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
MA MD

• **Nihon Kohden Corporation**
Shinjuku-ku
Tokyo (JP)

(72) Inventors:
• **Nogami, Akihiko**
Tsukuba-shi, Ibaraki 305-8577 (JP)
• **Takizawa, Koji**
Shinjuku-ku, Tokyo (JP)

(30) Priority: **14.07.2015 JP 2015140573**

(71) Applicants:
• **University of Tsukuba**
Tsukuba-shi, Ibaraki 305-8577 (JP)


(74) Representative: **Grünecker Patent- und Rechtsanwälte**
PartG mbB
Leopoldstraße 4
80802 München (DE)

(54) **ELECTROCARDIOGRAM ANALYZER**

(57) An electrocardiogram analyzer includes a first acquiring section that acquires a body surface electrocardiogram of a subject, a second acquiring section that acquires an intracardiac electrocardiogram of a ventricle of a heart of the subject, and an analyzing section that performs a frequency analysis on the intracardiac electrocardiogram and includes a range setting section that sets an analysis time range of the frequency analysis in

the intracardiac electrocardiogram based on a unit waveform of the body surface electrocardiogram, and a calculating section that, in the analysis time range, performs the frequency analysis on the intracardiac electrocardiogram, and that calculates an index value indicating a ratio of local abnormal ventricular activities in the intracardiac electrocardiogram.

FIG. 1

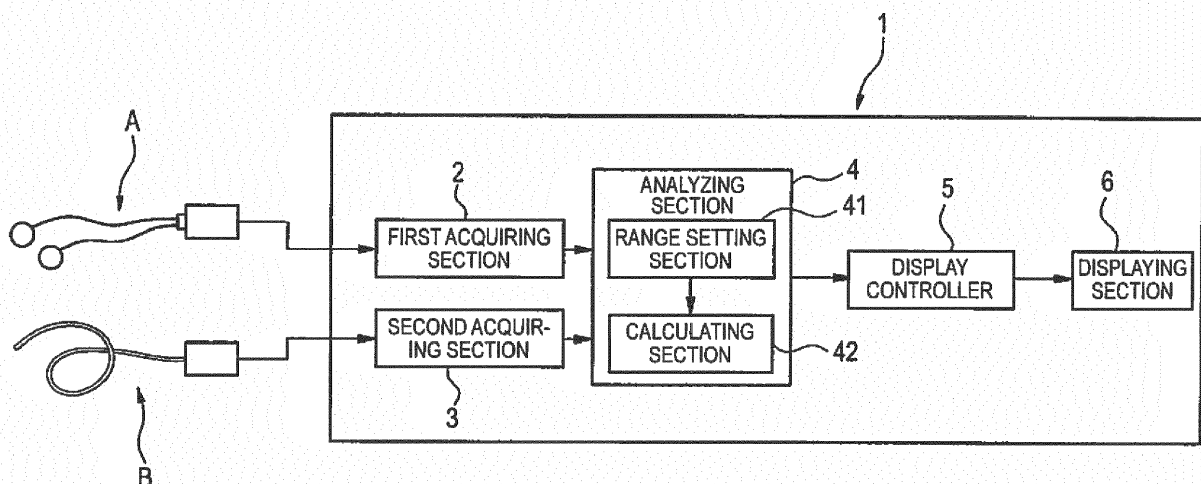

Description**BACKGROUND**

5 **[0001]** The present invention relates to an apparatus for analyzing an electrocardiogram acquired from a subject.

[0002] Usually, ventricular tachycardia means a condition where the heartbeat is different from the normal rhythm of the heart, and premature ventricular contraction occurs frequently in the ventricle. Ventricular tachycardia may cause worsening of heart failure, and sudden death, and therefore requires attention.

10 **[0003]** Conventionally, therefore, it is known that ventricular tachycardia is treated by selectively performing ablation on the abnormal site which causes ventricular tachycardia, by using a cardiac catheter. In order to perform the treatment, it is important to correctly identify the position where ablation is to be performed.

[0004] With respect to identification of the position of an abnormal site in the ventricle, it has been reported that, in a myocardium portion of the ventricle in which a substrate for ventricular tachycardia exists, high-frequency LAVA (Local Abnormal Ventricular Activities) are observed in addition to a sinus rhythm ventricular wave (V-wave). There is a non-patent Literature 1, Bieito Campos et al., "Use of Novel Fragmentation Map to Identify the Substrate for Ventricular Tachycardia in Post Infarction Cardiomyopathy," Heart Rhythm, 2014 October. The non-patent Literature 1 proposes an analysis technique in which a frequency analysis is performed on an intracardiac electrocardiogram of the ventricle, thereby quantitatively analyzing a ratio of LAVA contained in a sinus rhythm ventricular wave.

15 **[0005]** In an intracardiac electrocardiogram of the ventricle, however, LAVA sometimes appear after a sinus rhythm ventricular wave, and in other cases appears overlappingly with a ventricular wave. Moreover, an intracardiac electrocardiogram may contain noises due to the contact state of an electrode of a catheter, those caused by influences of myocardial sites which are remote from the measurement site (an atrial wave and a far-field potential), etc. In the case where a frequency analysis is to be performed on an intracardiac electrocardiogram of the ventricle as disclosed in Non-patent Literature 1, therefore, a medical person must adequately adjust and set an analysis time range of the frequency analysis while the shape of each unit waveform contained in the intracardiac electrocardiogram, and waveforms before and after the unit waveform are checked so that LAVA do not leak from the analysis time range. In the technique, in the case where points (mapping points) from which an electrocardiogram is to be acquired are as many as several hundreds, a process of setting the analysis time range takes a long time. Therefore, it is difficult to, during catheter treatment, identify the position of the abnormal site by a frequency analysis.

20 **[0006]** Therefore, it is an object of the invention to provide an electrocardiogram analyzer in which a frequency analysis can be performed on an intracardiac electrocardiogram of a ventricle in a manner easier than the conventional technique.

SUMMARY

35 **[0007]** According to an aspect of the invention, the electrocardiogram analyzer of the invention includes, a first acquiring section which acquires a body surface electrocardiogram of a subject, a second acquiring section which acquires an intracardiac electrocardiogram of a ventricle of a heart of the subject, and an analyzing section which performs a frequency analysis on the intracardiac electrocardiogram, and the analyzing section has a range setting section which sets an analysis time range of the frequency analysis in the intracardiac electrocardiogram based on a unit waveform of the body surface electrocardiogram, and a calculating section which, in the analysis time range, performs the frequency analysis on the intracardiac electrocardiogram, and which calculates an index value indicating a ratio of local abnormal ventricular activities (LAVA) in the intracardiac electrocardiogram.

40 **[0008]** A body surface electrocardiogram is less affected by noises than an intracardiac electrocardiogram, and in linkage with the sinus rhythm in an intracardiac electrocardiogram. According to the configuration, based on a unit waveform of a body surface electrocardiogram, therefore, the analysis time range in the intracardiac electrocardiogram of the ventricle can be set accurately and automatically so as to contain the potential variation of the measurement place in the ventricle and LAVA accompanying thereto. Then, also the index value indicating the ratio of LAVA with respect to the intracardiac electrocardiogram within the analysis time range is automatically calculated. Even during the process of measuring the intracardiac electrocardiogram of the ventricle through, for example, an electrode disposed in a catheter, therefore, the index value indicating the ratio of LAVA in the intracardiac electrocardiogram within the analysis time range is automatically calculated, and the position of the abnormal site in the ventricle can be identified. According to the configuration, a medical person can omit the work of setting the analysis time range of the frequency analysis, which is manually performed in the prior art, and perform the frequency analysis in a manner easier than the conventional technique.

55 **[0009]** According to the electrocardiogram analyzer of the invention, a frequency analysis can be performed on an intracardiac electrocardiogram of the ventricle in a manner easier than the conventional technique.

BRIEF DESCRIPTION OF DRAWINGS

[0010]

Fig. 1 is a diagram illustrating an electrocardiogram analyzer of an embodiment of the invention.
 Figs. 2A and 2B illustrates the operation principle of the analyzer.
 Figs. 3A and 3B illustrates the operation principle of the analyzer.
 Fig. 4 illustrates a display example of a displaying section disposed in the analyzer.
 Fig. 5 illustrates another display example displayed on the displaying section.
 Fig. 6 illustrates a further display example displayed on the displaying section.
 Fig. 7 illustrates an example a frequency range which is used in calculation of an index value by the analyzer.
 Fig. 8 illustrates an example of the configuration of the analyzer.
 Fig. 9 illustrates a visualized result of an analysis performed by the analyzer.

[0011] DETAILED DESCRIPTION OF EMBODIMENTS

Hereinafter, an embodiment of the invention will be described in detail with reference to the drawings. Fig. 1 is a functional block diagram showing an electrocardiogram analyzer 1. The electrocardiogram analyzer 1 is an apparatus in which an abnormal site in the ventricle can be identified by performing a frequency analysis on an intracardiac electrocardiogram acquired from the ventricle of the heart of the subject. As illustrated in Fig. 1, the electrocardiogram analyzer 1 may include a first acquiring section 2, a second acquiring section 3, an analyzing section 4, a display controller 5, and a displaying section 6.

[0012] The first acquiring section 2 acquires a body surface electrocardiogram of the subject which is recorded by a recording unit A. The recording unit A is configured by, for example, electrodes for recording a standard 12-lead electrocardiogram, and the like.

[0013] The second acquiring section 3 acquires an intracardiac electrocardiogram of the subject which is recorded by a recording unit B. The recording unit B is configured by, for example, a cardiac catheter which is inserted into the heart through the vein to record an intracardiac electrocardiogram, and the like. As an intracardiac electrocardiogram, an intracardiac electrocardiogram in which a ventricular wave (V-wave) is recorded is used. An intracardiac electrocardiogram of the subject is recorded at a plurality of mapping points while moving the position of the electrode of the cardiac catheter.

[0014] Preferably, the first acquiring section 2 and the second acquiring section 3 are configured so that the timing when the first acquiring section 2 acquires a body surface electrocardiogram is synchronized with that when the second acquiring section 3 acquires an intracardiac electrocardiogram.

[0015] An analyzing section 4 performs a frequency analysis (for example, a fast Fourier transform) on the electrocardiogram by using the body surface electrocardiogram acquired by the first acquiring section 2, and the intracardiac electrocardiogram acquired by the second acquiring section 3. The analyzing section 4 may include a range setting section 41 and a calculating section 42.

[0016] The range setting section 41 sets an analysis time range where the frequency analysis is to be performed on the intracardiac electrocardiogram, based on each beat (hereinafter, referred to as a unit waveform) appearing in the body surface electrocardiogram. The analysis time range of the intracardiac electrocardiogram is set by means a pre-determined period of time before and after, for example, the QRS waveform in each unit waveform of the body surface electrocardiogram. The QRS waveform means a waveform which is produced during ventricular activation.

[0017] The calculating section 42 performs the frequency analysis on the intracardiac electrocardiogram, in the analysis time range which is set by the range setting section 41. Moreover, the calculating section 42 calculates an index value for identifying an abnormal site in the ventricle, based on a result of the frequency analysis on the intracardiac electrocardiogram. The index value indicates the ratio of the LAVA (Local Abnormal Ventricular Activities) in the intracardiac electrocardiogram. The LAVA means a local abnormal potential which, in a sinus rhythm intracardiac electrocardiogram recorded in the ventricle, is fused (overlaps) with a potential variation of the ventricular wave or occurs separately from the potential variation of the ventricular wave.

[0018] The display controller 5 controls the contents to be displayed on the displaying section 6. Under control of the display controller 5, the displaying section 6 displays analysis information of the electrocardiogram which is supplied from the analyzing section 4. The displaying section 6 is configured by, for example, a touch panel liquid crystal display.

[0019] The operation principle of the electrocardiogram analyzer 1 will be described with reference to Figs. 2A and 3B.

[0020] As a preparation step, the electrodes of the recording unit A are attached to the body surface (the four limbs, the chest, and the like) of the subject. The cardiac catheter of the recording unit B is inserted into the ventricle of the subject, and the electrode is indwelled at a mapping point. Each time when the electrocardiogram analysis at each mapping point has been ended, the position of the mapping point where the electrode of the cardiac catheter is to be

indwelled is moved to the next mapping point.

[0021] When the operation of analyzing the electrocardiogram is started, as illustrated in the upper portions of Figs. 2A and 3A, the body surface electrocardiogram 21 or the subject is recorded by the recording unit A. In synchronization with the timing of recording the body surface electrocardiogram 21, as illustrated in the lower portions of Figs. 2A and 3A, intracardiac electrocardiograms 31 A, 31 B of the subject are recorded by the recording unit B. The intracardiac electrocardiograms 31A, 31B are intracardiac electrocardiograms which are recorded in different mapping points.

[0022] The intracardiac electrocardiogram 31A illustrated in Fig. 2A indicates an intracardiac electrocardiogram which is recorded while an abnormal site in the ventricle is set as the mapping point. By contrast, the intracardiac electrocardiogram 31B illustrated in Fig. 3A indicates an intracardiac electrocardiogram which is recorded while a normal myocardium site in the ventricle is set as the mapping point. In a myocardium site (abnormal site) in which a substrate for ventricular tachycardia exists, LAVA may sometimes occur in an intracardiac electrocardiogram during a sinus rhythm. The intracardiac electrocardiogram 31A indicates an intracardiac electrocardiogram which occurs as a result of fusion of LAVA 33 with a potential variation of a ventricular wave 32. By contrast, the intracardiac electrocardiogram 31B indicates an intracardiac electrocardiogram in which LAVA do not occur and only a potential variation of a ventricular wave 34 is recorded.

[0023] LAVA sometimes occur after a position where a potential variation of the ventricular wave occurs, while separating from the ventricular wave, or in other cases, as indicated in the intracardiac electrocardiogram 31A, occur while fusing with a potential variation of the ventricular wave. Surrounding noises are easily superimposed on an intracardiac electrocardiogram. In the case where LAVA occur while fusing with a potential variation of the ventricular wave, therefore, it is difficult to visually check LAVA, and hence an occurrence of LAVA is often overlooked.

[0024] Therefore, the inventors have focused attention on the phenomenon in which the frequency components of LAVA contain a larger amount of high-frequency components than those of a potential variation of the ventricular wave, and studied a method in which a frequency analysis is performed on an intracardiac electrocardiogram to detect an occurrence of LAVA.

[0025] In this case, it is important to set an analysis time range where the frequency analysis is to be performed, so as to contain at least LAVA. In the embodiment, when the analysis time range is to be set, an R wave peak in the body surface electrocardiogram is used as a reference point.

[0026] In Fig. 2A, an area designating line 11 which surrounds an area in a rectangular shape indicates the analysis time range. The analysis time range 11 is configured by a front period 12 which is in front of the peak 23 of the R-wave in the body surface electrocardiogram 21, and a rear period 13 which is in rear of the peak. The front period 12 is set so as to contain the Q-wave which indicates the starting timing of ventricular contraction. The rear period 13 is set to a period which can include LAVA that occurs after the ventricular wave while separating from the ventricular wave. Specifically, the rear period is set to a period which is in front of the P-wave that indicates the timing when the atrium starts the next operation. The periods are previously set by the operator through an input operating section. The range setting section 41 detects the peak 23 of the R-wave in a unit waveform 22 of the body surface electrocardiogram 21, and sets the front period 12 and rear period 13 with respect to the detected peak 23, as the analysis time range 11 of the intracardiac electrocardiogram 31A.

[0027] Also in Fig. 3A, the analysis time range 11 is set in a same or similar manner. The range setting section 41 detects the peak 25 of the R-wave in a unit waveform 24 of the body surface electrocardiogram 21, and sets the front period 12 and rear period 13 with respect to the detected peak 25, as the analysis time range 11 of the intracardiac electrocardiogram 31B.

[0028] The calculating section 42 performs the frequency analysis on the intracardiac electrocardiograms 31A, 31B in the preset analysis time range 11.

[0029] Fig. 2B illustrates the frequency distribution in the analysis time range 11 of the intracardiac electrocardiogram 31A (see Fig. 2A), and Fig. 3B illustrates the frequency distribution in the analysis time range 11 of the intracardiac electrocardiogram 31B (see Fig. 3A). When comparing the two frequency distributions with each other, it is seen that the frequency distribution (Fig. 2B) of the intracardiac electrocardiogram 31A in which LAVA 33 are fused with the potential variation of the ventricular wave 32 contains a larger amount of high-frequency components than the frequency distribution (Fig. 3B) of the intracardiac electrocardiogram 31B in which only the potential variation of the ventricular wave 34 exists (LAVA do not occur).

[0030] The calculating section 42 calculates the ratio of predetermined frequency components (in the example, 40 to 100 Hz) contained in a certain range (in the example, 1 to 100 Hz) of the frequency distribution, as an AR (Area Ratio). For example, the area ratio AR can be indicated by following Exp. 1 :

$$AR = \text{Area [40 to 100 Hz]} / \text{Area [1 to 100 Hz]} \dots\dots\dots (\text{Exp. 1}).$$

[0031] Exp. 1 shows the ratio of the frequency distribution amount of 40 to 100 Hz with respect to that of 1 to 100 Hz. In Figs. 2B and 3B, this indicates the area ratio of the hatched area 52 with respect to the hatched area (51, 52). The AR value is defined as a ratio of LAVA contained in the analysis time range of the intracardiac electrocardiogram, and used as an index value for identifying an abnormal site in the ventricle.

[0032] As illustrated in Fig. 4, electrocardiogram analysis information 60 which is analyzed in the electrocardiogram analyzer 1 is displayed on the displaying section 6. The electrocardiogram analysis information 60 includes, for example, the body surface electrocardiogram 21, the intracardiac electrocardiogram 31, the frequency distribution 50, the AR value (index value) 53, and the like. The body surface electrocardiogram 21 and the intracardiac electrocardiogram 31 which is recorded in synchronization with the body surface electrocardiogram 21 are displayed, for example, in a vertically juxtaposed manner. The body surface electrocardiogram 21 and the intracardiac electrocardiogram 31 are sequentially displayed in each unit waveform. The displaying section is configured so that the timing of switching the display of each unit waveform can be arbitrarily set. For example, the switching may be performed at each time when a peak of the R wave is detected, in order to display all unit waveforms, or every several seconds. The analysis time range 11 indicating the ranges where the frequency analysis is to be performed is displayed on the body surface electrocardiogram 21 and the intracardiac electrocardiogram 31. On the left side of the body surface electrocardiogram 21 and the intracardiac electrocardiogram 31, for example, the frequency distribution 50 and AR value 53 which are obtained by performing frequency analysis on the analysis time range 11 of the intracardiac electrocardiogram 31 are juxtaposedly displayed. The frequency distribution 50 and the AR value 53 are set so that they are acquired at each time when the unit waveform is detected, and their display is switched in synchronization with the display switching timing of the unit waveform.

[0033] According to the configuration, the QRS waveform of the body surface electrocardiogram is used for setting the analysis time range of the frequency analysis in the intracardiac electrocardiogram. A body surface electrocardiogram is less affected by noises than an intracardiac electrocardiogram, and in linkage with the sinus rhythm in an intracardiac electrocardiogram. Based on the unit waveform 22 of the body surface electrocardiogram, therefore, the analysis time range in the intracardiac electrocardiograms 31 A, 31B of the ventricle can be set accurately and automatically so as to contain the potential variations of the ventricular waves 32, 34 at mapping points of the ventricle, and LAVA which occur (accompany thereto) while fusing with or separating from them. Moreover, a frequency analysis is performed on the intracardiac electrocardiograms 31A, 31B in the thus set analysis time range 11, whereby also the AR value (index value) indicating the ratio of the LAVA 33 to the intracardiac electrocardiograms 31 A, 31B can be automatically calculated. Even during the process of recording the intracardiac electrocardiograms 31 A, 31B of the ventricle through the electrode of the cardiac catheter, therefore, the AR value indicating the ratio of the LAVA 33 in the intracardiac electrocardiograms 31 A, 31B within the analysis time range 11 can be automatically calculated, and the position of the abnormal site in the ventricle can be identified in a short time. A medical person can omit the work of setting the analysis time range of the frequency analysis, which is manually performed in prior art, and perform the frequency analysis on an intracardiac electrocardiogram of the ventricle in a manner easier than the conventional technique.

[0034] Moreover, the body surface electrocardiogram 21 and intracardiac electrocardiograms 31A, 31B which are recorded from the subject are acquired in synchronization with each other by the electrocardiogram analyzer 1. Therefore, the analysis time range 11 in which the linkage between the electrocardiograms is considered can be easily set, and the analysis time range 11 can be set further accurately.

[0035] As indicated by the broken lines 12 in Fig. 4, the analysis time range 11 in which the frequency analysis is to be performed in the intracardiac electrocardiogram 31 can be configured so as to be adjusted based on an operation by the operator. The analysis time range 11 can be adjusted by, for example, touch-operating operation buttons (not shown) displayed on the displaying section 6. In this case, the frequency distribution 50 and the AR value 53 are again analyzed and calculated in accordance with the adjustment of the analysis time range 11, and then updated.

[0036] According to the configuration, the analysis time range 11 can be adequately adjusted in accordance with the features of the acquired electrocardiogram waveforms. Therefore, the frequency analysis can be performed more accurately, and the position of an abnormal site in the ventricle can be accurately identified.

[0037] As illustrated in Fig. 5, the plural (in the example, two) sets of electrocardiogram analysis information 61, 62 which are analyzed by the electrocardiogram analyzer 1 may be simultaneously displayed on the displaying section 6. In the case where the analysis time range where the frequency analysis is to be performed in the intracardiac electrocardiogram 31 is adjusted by an operation by the operator, for example, the sets of electrocardiogram analysis information 61, 62 in analysis time ranges 11A, 11B before and after the adjustment can be simultaneously displayed in a juxtaposed manner on the displaying section 6. The switching to this screen can be performed by, for example, touch-operating operation buttons (not shown) displayed on the displaying section 6.

[0038] According to the configuration, AR values 53A, 53B before and after the adjustment of the analysis time range are simultaneously displayed. Therefore, an adequate analysis time range can be selected while comparing results (AR values) of a plurality of adjustments with one another, and the frequency analysis can be performed more accurately.

[0039] As illustrated in Fig. 6, AR values 53C, 53D, 53E which are calculated with respect to a plurality (in the example, three) of successive unit waveforms, respectively may be simultaneously displayed on the displaying section 6. Among

the three frequency distributions and AR values which are juxtaposedly displayed on the displaying section 6, the frequency distribution 50C and the AR value 53C indicate electrocardiogram analysis information which is obtained with respect to unit waveforms of the body surface electrocardiogram 21 and intracardiac electrocardiogram 31 that are currently displayed. The frequency distribution 50D and the AR value 53D indicate electrocardiogram analysis information which is obtained with respect to unit waveforms of one beat earlier, and the frequency distribution 50E and the AR value 53E indicate electrocardiogram analysis information which is obtained with respect to unit waveforms of two beats earlier. The average AR value 53F indicate electrocardiogram analysis information which is obtained by averaging the AR values 53C, 53D, 53E. The switching to this screen can be performed by touch-operating operation buttons in a similar manner as described above.

[0040] According to the configuration, since the AR values which are successively calculated are compared with each other, it is possible to confirm whether an intracardiac electrocardiogram of the subject is acquired in a stabilized state or not.

[0041] As illustrated in Fig. 7, the frequency range of the predetermined area which is used for calculating the AR value can be arbitrarily set. In the above-described calculation of (Exp. 1), for example, the frequency ranges indicated by S1 and S2 of a setting example 73 in Fig. 7 are used. In (Exp. 1) above, namely, the frequency range of the numerator is set to 40 to 100 Hz, and that of the denominator is set to 1 to 100 Hz. These frequency ranges can be changed by operating setting buttons 75 to arbitrary frequency ranges such as setting examples 71, 72, 74. The preset plural frequency ranges (setting examples 71 to 74) can be simultaneously displayed together with the calculated AR values on the displaying section 6. The operator can select the frequency range to be used, from the displayed setting examples 71 to 74. The switching to this screen can be performed by touch-operating operation buttons in a similar manner as described above.

[0042] According to the configuration, even in the case where frequency components of LAVA are dispersed, when the frequency range is changed to an adequate range, it is possible to calculate an appropriate AR value. Therefore, the position of an abnormal site in the ventricle can be identified more accurately. Moreover, AR values in a plurality of frequency ranges which are arbitrarily set can be simultaneously displayed on the displaying section 6. Therefore, an adequate frequency range can be selected while comparing the values with one another, and the position of an abnormal site can be identified more accurately.

[0043] As illustrated in Fig. 8, an electrocardiogram analyzer 1A may include a producing section 43. The producing section 43 is disposed in, for example, the analyzing section 4, and, based on the AR value calculated by the calculating section 42, determines whether the mapping point (measurement site) of the ventricle is an abnormal site or not. The AR value indicates the contained ratio of LAVA in the analysis time range of the intracardiac electrocardiogram. Therefore, in the case where the AR value exceeds a preset threshold, for example, it is determined that the mapping point is an abnormal site. Based on the position data of the mapping point and the result of the determination of the AR value, the producing section 43 produces visualization data for visually discriminating normal and abnormal sites in the ventricle from each other. The visualization data are configured by color data for displaying normal and abnormal sites in different display modes (for example, different colors or patterns). Based on the visualization data, the display controller 5 may cause a 3D map 81 such as illustrated in Fig. 9 to be displayed on the displaying section 6. In the example, in the 3D map 81, a site indicated by the cross-hatching lines 82 is illustrated as an abnormal site.

[0044] As illustrated in Fig. 8, the electrocardiogram analyzer 1A may include a transmitter 7. The transmitter 7 transmits the visualization data produced by the producing section 43, to an external 3D mapping apparatus. In this case, the transmitter 7 is configured so as to transmit the visualization data each time when the mapping point is moved in the ventricle and the AR value for the mapping point is calculated. Based on the transmitted visualization data, the 3D mapping apparatus may display the 3D map 81 such as illustrated in Fig. 9.

[0045] According to the configuration, a medical person or the like can visually check the position of an abnormal site, and perform, for example, ablation by using the catheter. During treatment, the AR value can be quickly reflected in the 3D mapping apparatus, and a substrate for tachycardia can be identified from the whole map. This can be useful to ablation treatment.

[0046] The above-described embodiment is a mere example for facilitating understanding of the invention, and does not limit the invention. It is obvious that the embodiment may be adequately changed or improved without departing the spirit of the invention, and equivalents are included within the scope of the invention.

Claims

1. An electrocardiogram analyzer comprising:

- a first acquiring section that acquires a body surface electrocardiogram of a subject;
- a second acquiring section that acquires an intracardiac electrocardiogram of a ventricle of a heart of the subject;

and

an analyzing section that performs a frequency analysis on the intracardiac electrocardiogram and includes:

a range setting section that sets an analysis time range of the frequency analysis in the intracardiac electrocardiogram based on a unit waveform of the body surface electrocardiogram; and
a calculating section that, in the analysis time range, performs the frequency analysis on the intracardiac electrocardiogram, and that calculates an index value indicating a ratio of local abnormal ventricular activities in the intracardiac electrocardiogram.

2. The electrocardiogram analyzer according to claim 1, wherein the analysis time range which is set by the range setting section is adjustable based on an operation by an operator.

3. The electrocardiogram analyzer according to claim 2 further comprising:

a displaying section; and
a display controller that controls display contents of the displaying section, wherein the display controller causes a plurality of index values which are based on the analysis time range that has been adjusted by the operator, to be simultaneously displayed on the displaying section.

4. The electrocardiogram analyzer according to claim 1 further comprising:

a displaying section; and
a display controller that controls display contents of the displaying section, wherein the display controller causes a plurality of index values which are successively calculated, to be simultaneously displayed on the displaying section.

5. The electrocardiogram analyzer according to any one of claims 1 to 4, further comprising:

a producing section that determines whether a measurement site of a ventricle is an abnormal site or not, based on the index value, and which produces visualization data for displaying the abnormal site in a display mode that is different from a display mode of a normal site.

6. The electrocardiogram analyzer according to any one of claims 1 to 5, wherein a timing when the first acquiring section acquires the body surface electrocardiogram is synchronized with a timing when the second acquiring section acquires the intracardiac electrocardiogram.

FIG. 1

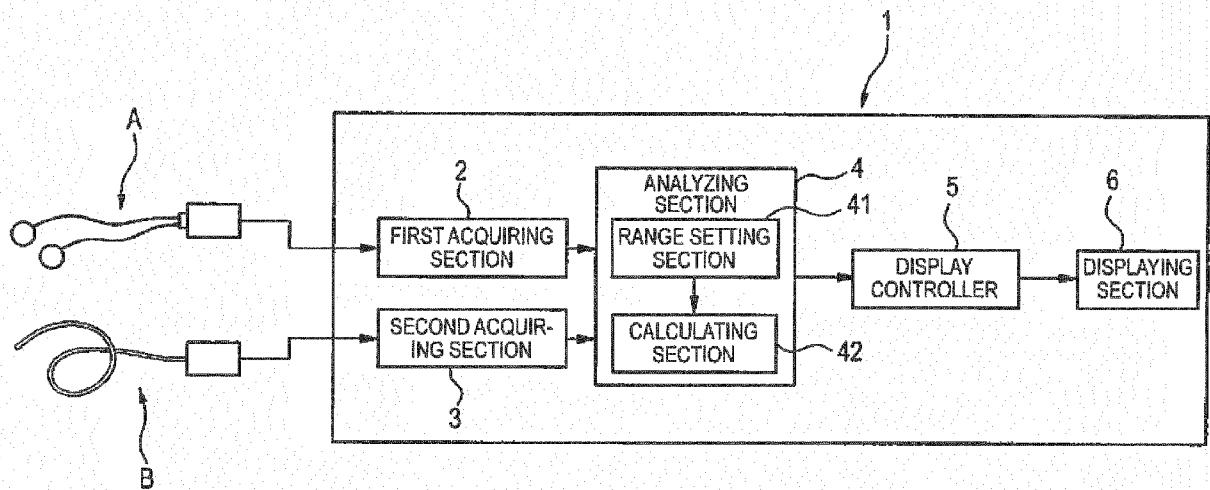


FIG. 2A

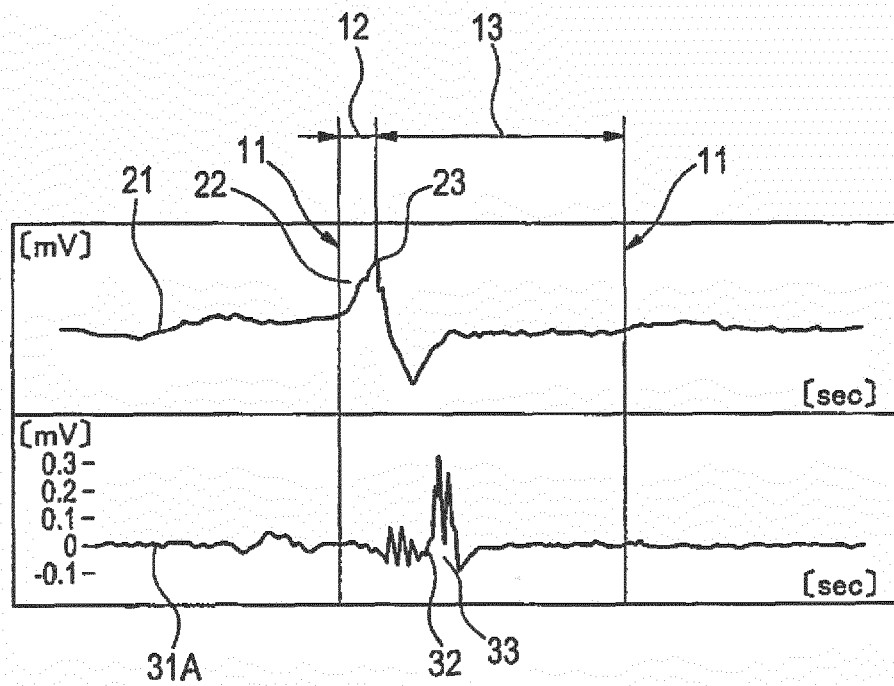


FIG. 2B

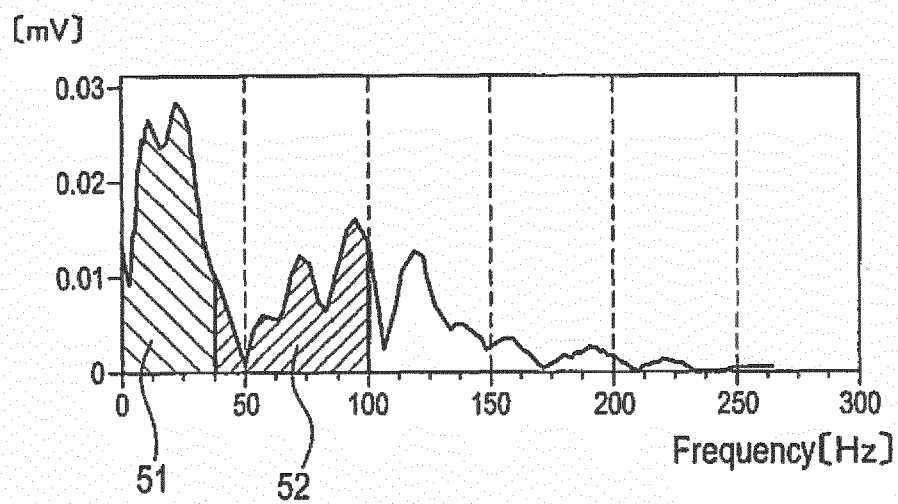


FIG. 3A

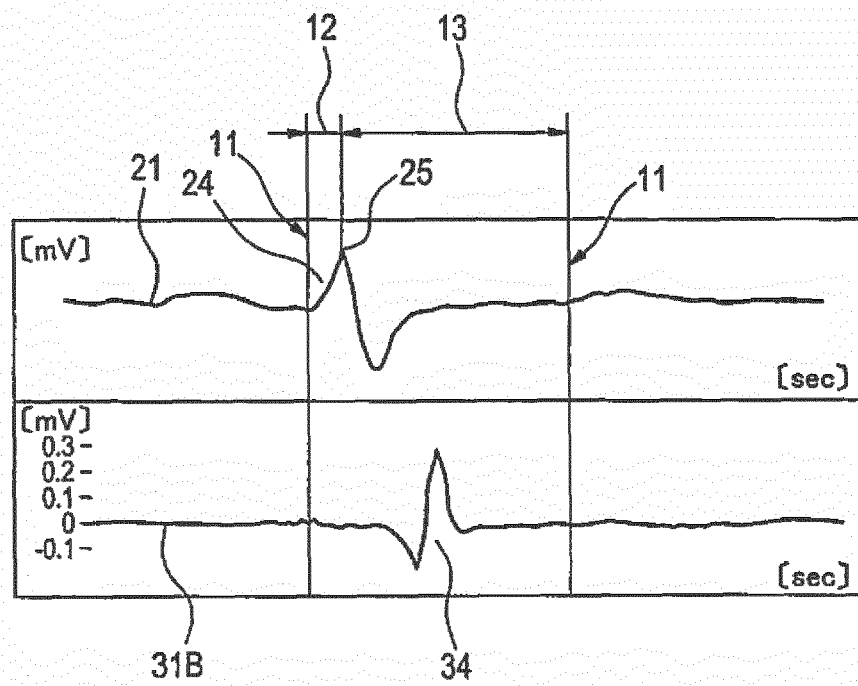


FIG. 3B

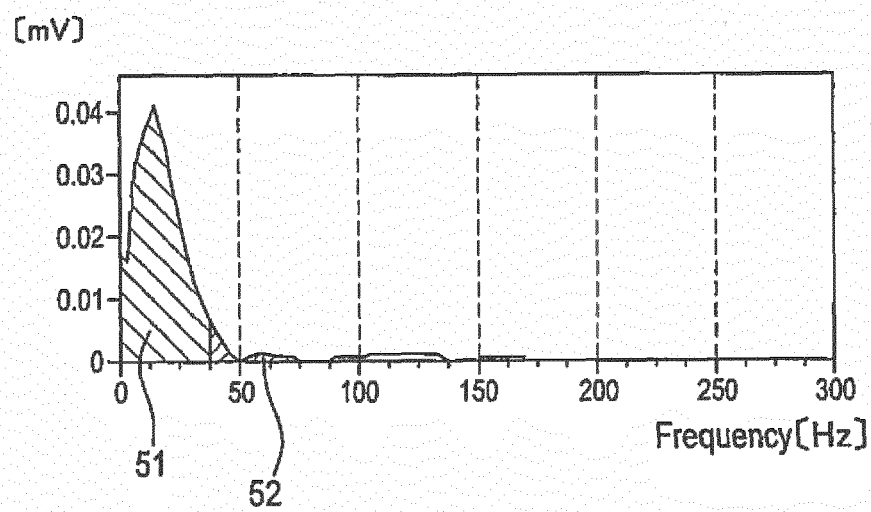


FIG. 4

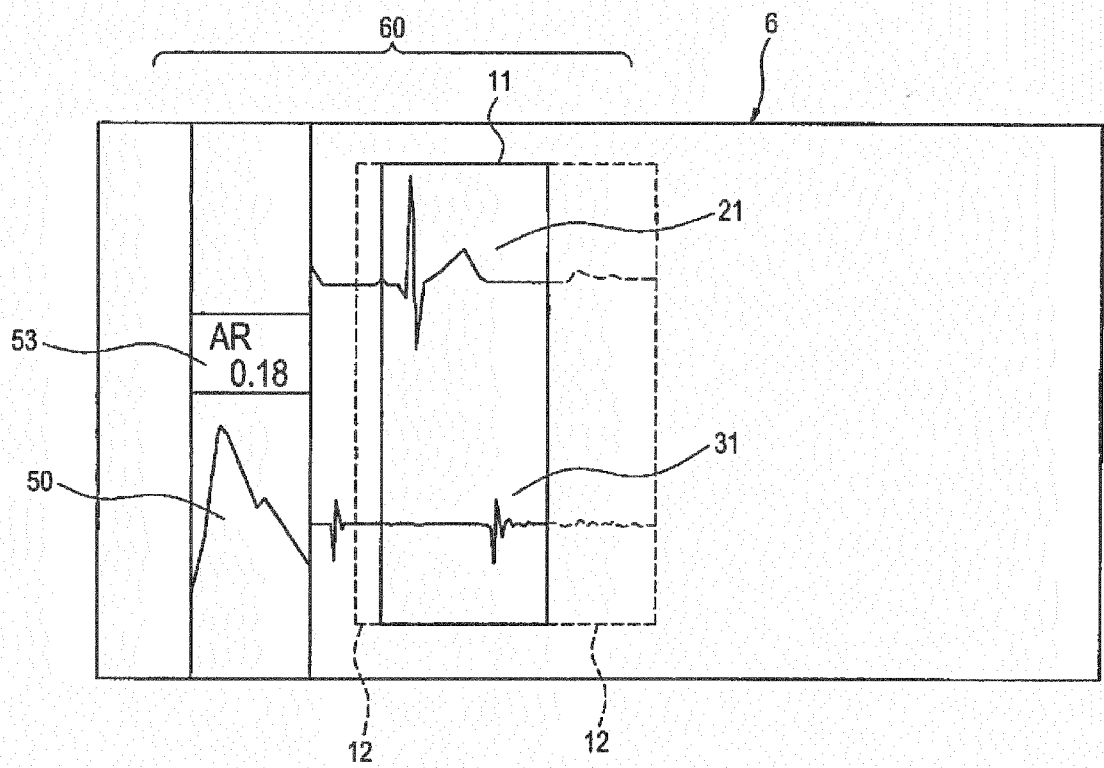


FIG. 5

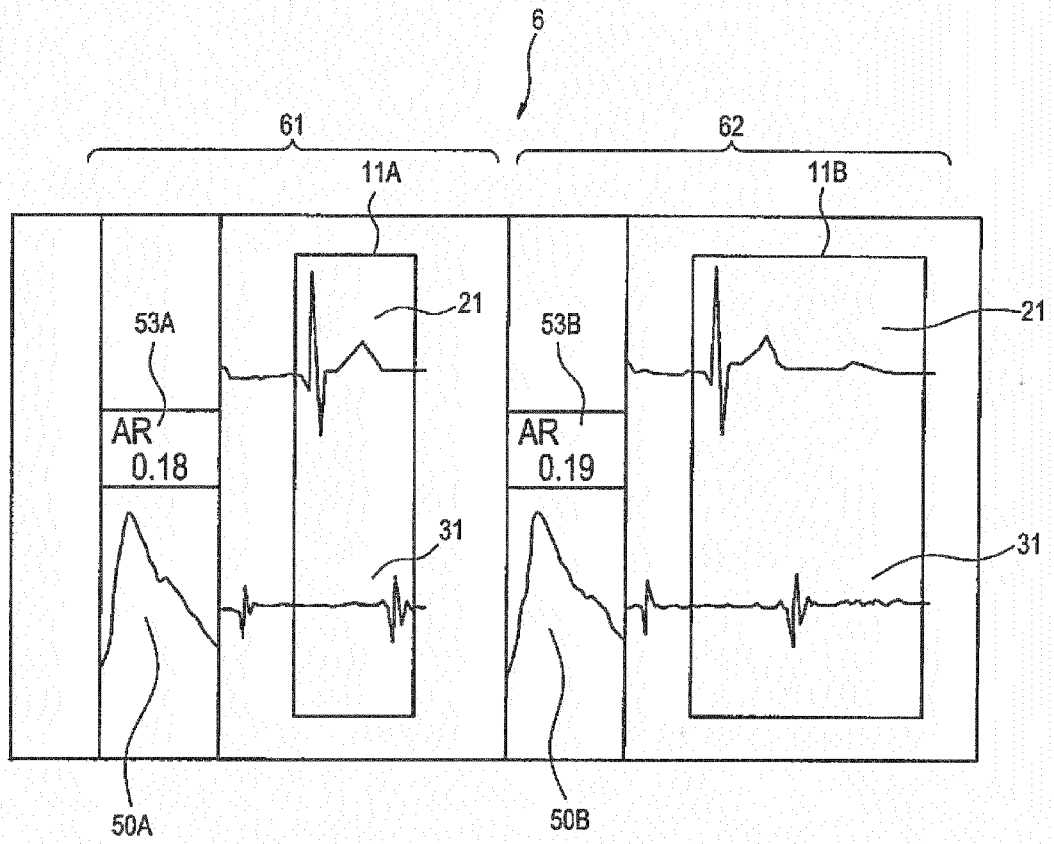


FIG. 6

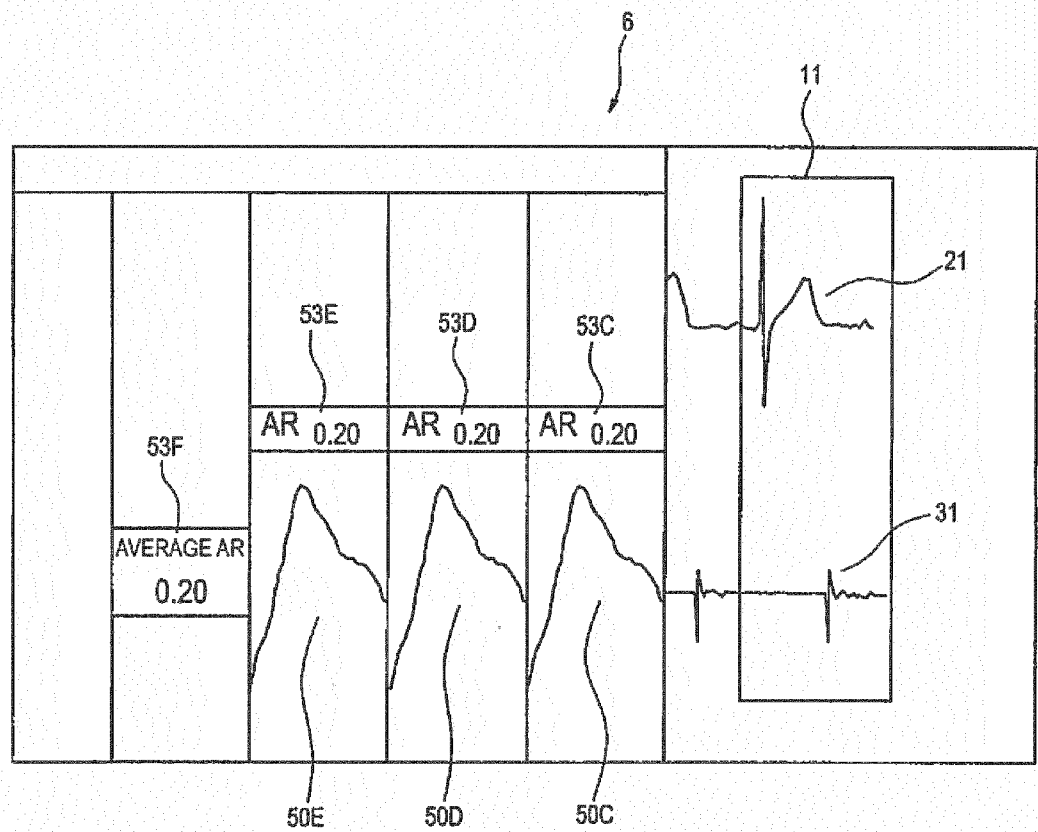


FIG. 7

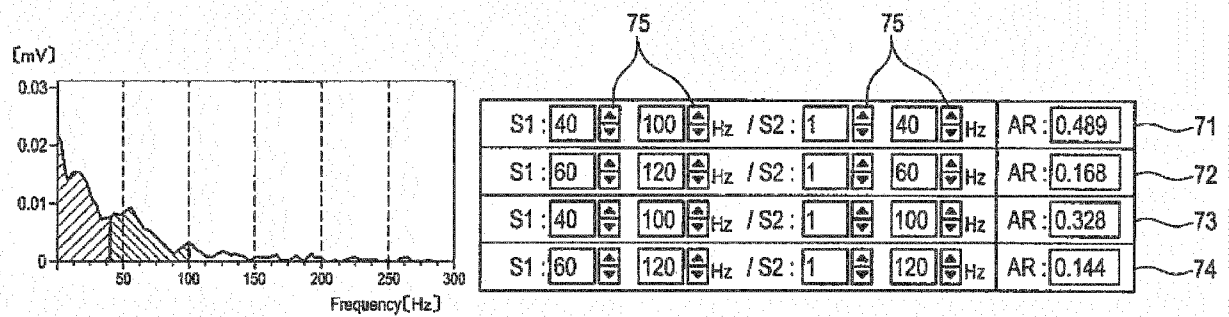


FIG. 8


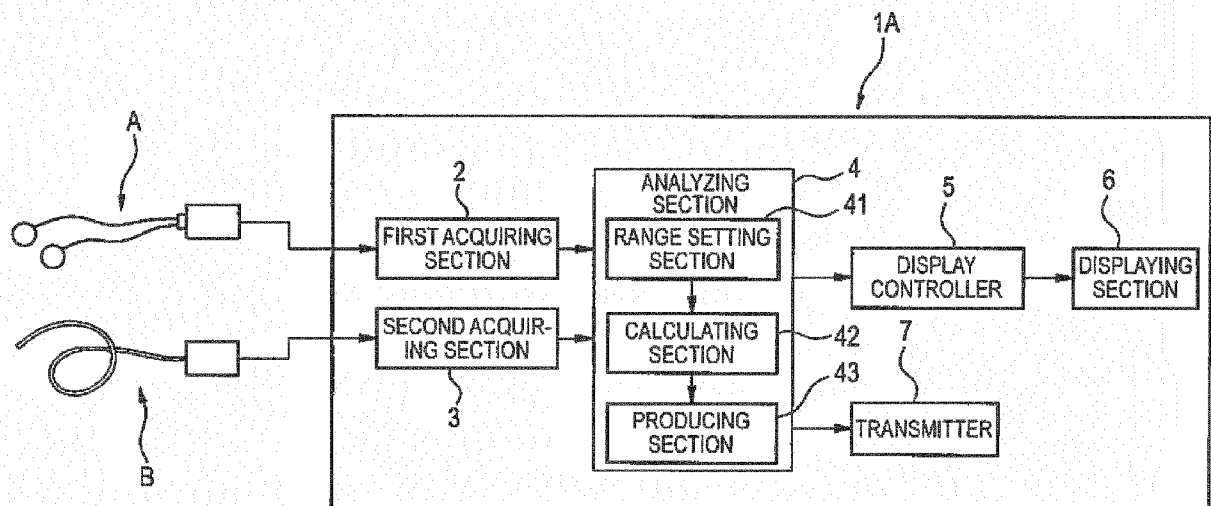


FIG. 9



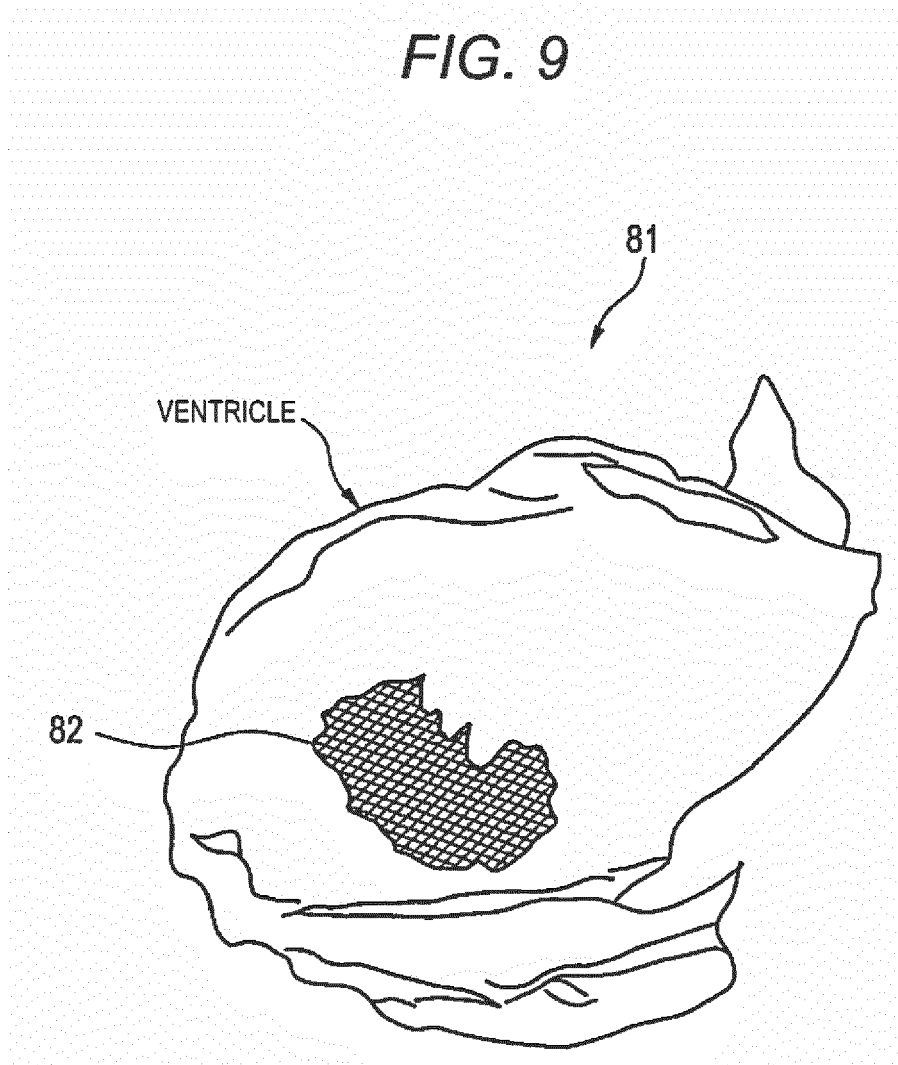

EUROPEAN SEARCH REPORT

Application Number
EP 16 17 8933

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2013/274623 A1 (ZHANG HONGXUAN [US]) 17 October 2013 (2013-10-17) * paragraphs [0015], [0018], [0022], [0030] - [0032], [0040] * * figure 1 *	1-5	INV. A61B5/00 A61B5/0456 A61B5/042 A61B5/0408
X	WO 95/02995 A1 (BIOSENSE INC [US]) 2 February 1995 (1995-02-02) * page 10, lines 22-33 * * page 11, line 4 * * page 13, lines 13-27 * * page 17, line 33 * * figures 5, 6, 9, 10 *	1-6	ADD. A61B5/0428 A61B5/0432 G06F19/00
X	US 2009/281441 A1 (ZHANG HONGXUAN [US] ET AL) 12 November 2009 (2009-11-12) * paragraphs [0021], [0025], [0028], [0029], [0031], [0032], [0035], [0036] * * figures 1, 6 *	1-5	
A	US 2010/268059 A1 (RYU KYUNGMOO [US] ET AL) 21 October 2010 (2010-10-21) * the whole document *	1-6	TECHNICAL FIELDS SEARCHED (IPC) A61B
A	WO 95/10225 A1 (EP TECHNOLOGIES [US]) 20 April 1995 (1995-04-20) * the whole document *	1-6	
A	WO 96/05768 A1 (BIOSENSE INC [US]; BEN HAIM SHLOMO [IL]; OSADCHY DANIEL [IL]; PELESS U) 29 February 1996 (1996-02-29) * the whole document *	1-6	
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 14 December 2016	Examiner Meyer, Wolfgang
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 16 17 8933

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

14-12-2016

10

15

20

25

30

35

40

45

50

55

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2013274623 A1	17-10-2013	NONE	
WO 9502995 A1	02-02-1995	AT 290818 T AU 692789 B2 AU 7372394 A CA 2144946 A1 DE 69434296 D1 DE 69434296 T2 DK 0679068 T3 EP 0679068 A1 ES 2240964 T3 JP 4040672 B2 JP H08504653 A PT 679068 E US 5391199 A US 5443489 A US 5480422 A US 5546951 A US 5568809 A US 5694945 A US 5713946 A US 5840025 A WO 9502995 A1	15-04-2005 18-06-1998 20-02-1995 02-02-1995 21-04-2005 08-06-2006 11-07-2005 02-11-1995 16-10-2005 30-01-2008 21-05-1996 29-07-2005 21-02-1995 22-08-1995 02-01-1996 20-08-1996 29-10-1996 09-12-1997 03-02-1998 24-11-1998 02-02-1995
US 2009281441 A1	12-11-2009	NONE	
US 2010268059 A1	21-10-2010	US 2010268059 A1 US 2011092809 A1	21-10-2010 21-04-2011
WO 9510225 A1	20-04-1995	US 5637090 A WO 9510225 A1	10-06-1997 20-04-1995
WO 9605768 A1	29-02-1996	AT 188108 T AT 253864 T AU 1693095 A CA 2197986 A1 CA 2607769 A1 CN 1168625 A DE 69514238 D1 DE 69514238 T2 DE 69532139 D1 DE 69532139 T2 EP 0776176 A1 EP 0894473 A2 ES 2144123 T3 ES 2210662 T3	15-01-2000 15-11-2003 14-03-1996 29-02-1996 29-02-1996 24-12-1997 03-02-2000 11-05-2000 18-12-2003 26-08-2004 04-06-1997 03-02-1999 01-06-2000 01-07-2004

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 16 17 8933

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

14-12-2016

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		HK 1007059 A1	04-08-2006
		JP 3708121 B2	19-10-2005
		JP 4025309 B2	19-12-2007
		JP 4394733 B2	06-01-2010
		JP 4448194 B2	07-04-2010
		JP H10507104 A	14-07-1998
		JP 2004275776 A	07-10-2004
		JP 2004283601 A	14-10-2004
		JP 2009066429 A	02-04-2009
		JP 2009207926 A	17-09-2009
		WO 9605768 A1	29-02-1996

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

专利名称(译)	心电图分析仪		
公开(公告)号	EP3120753A1	公开(公告)日	2017-01-25
申请号	EP2016178933	申请日	2016-07-12
[标]申请(专利权)人(译)	国立大学法人筑波 日本光电工业株式会社		
申请(专利权)人(译)	筑波大学 日本光电公司		
当前申请(专利权)人(译)	筑波大学 日本光电公司		
[标]发明人	NOGAMI AKIHIKO TAKIZAWA KOJI		
发明人	NOGAMI, AKIHIKO TAKIZAWA, KOJI		
IPC分类号	A61B5/00 A61B5/0456 A61B5/042 A61B5/0408 A61B5/0428 A61B5/0432 G06F19/00		
CPC分类号	A61B5/04085 A61B5/0422 A61B5/0428 A61B5/0432 A61B5/0456 A61B5/6852 A61B5/7203 A61B5/7221 A61B5/7253 A61B5/7275 A61B2505/05 G16H50/20 G16H50/30 A61B5/04012 A61B5/042 A61B5/044		
审查员(译)	MEYER , WOLFGANG		
优先权	2015140573 2015-07-14 JP		
外部链接	Espacenet		

摘要(译)

心电图分析仪包括：第一获取部分，其获取对象的体表心电图；第二获取部分，其获取所述对象的心脏的心室的心内心电图；以及分析部分，其对所述心内心电图执行频率分析。并且包括：范围设定部分，其基于体表心电图的单位波形设定心内心电图中的频率分析的分析时间范围；以及计算部分，其在分析时间范围内，对心内进行频率分析。心电图，并计算指示心内心电图中局部异常心室活动的比率的指标值。

