

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
23 April 2009 (23.04.2009)

PCT

(10) International Publication Number
WO 2009/051963 A1

- (51) International Patent Classification:
A61B 5/00 (2006.01)
 - (21) International Application Number:
PCT/US2008/078433
 - (22) International Filing Date: 1 October 2008 (01.10.2008)
 - (25) Filing Language: English
 - (26) Publication Language: English
 - (30) Priority Data:
11/873,842 17 October 2007 (17.10.2007) US
 - (71) Applicant (for all designated States except US): **INTELECT MEDICAL, INC.** [US/US]; 1300 East 9th Street, Cleveland, OH 44114 (US).
 - (72) Inventors; and
 - (75) Inventors/Applicants (for US only): **KOKONES, Scott** [US/US]; 8414 Chester Parkway, Cleveland, OH 44106 (US). **CARLTON, Keith** [US/US]; 8418 Chester Parkway, Cleveland, OH 44106 (US).
 - (74) Agents: **BIRDE, Patrick, J.** et al.; KENYON & KENYON LLP, One Broadway, New York, NY 10004 (US).
 - (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
 - (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
— with international search report

(54) Title: PATIENT PROGRAMMER WITH INPUT AND SENSING CAPABILITIES

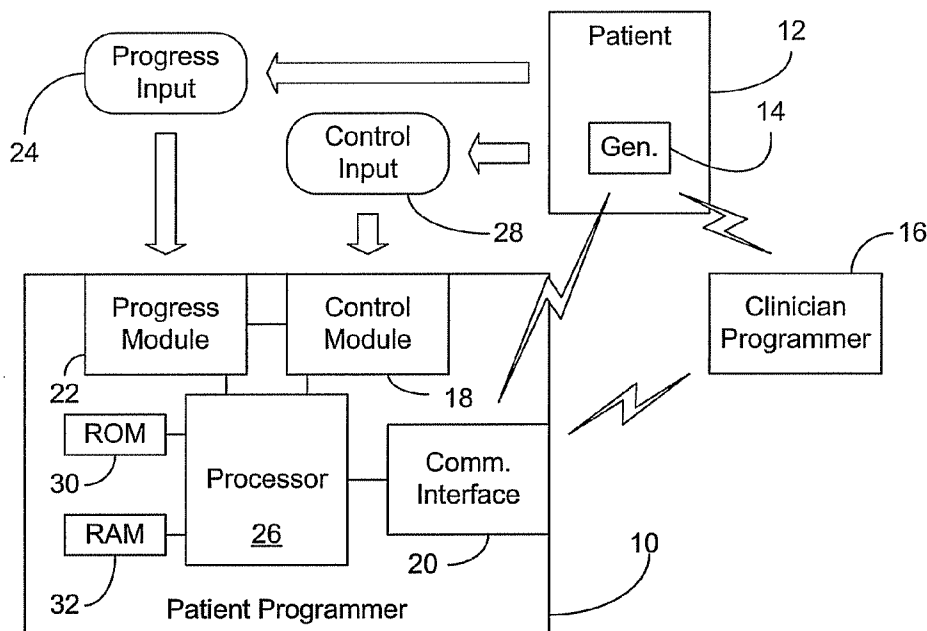


FIG. 1

(57) Abstract: A patient programmer can have a progress module, wherein the progress module may obtain progress input from a patient in which the generator is implanted. The progress module may include sensors that are able to obtain progress input based on patient interactions with sensors coupled to the patient programmer. The progress module may also include an interface that poses progress-related questions to the patient and obtains responses to the questions from the patient. The patient programmer is also able to store the progress input for reporting purposes.

WO 2009/051963 A1

PATIENT PROGRAMMER WITH INPUT AND SENSING CAPABILITIES

BACKGROUND

Technical Field

[0001] This disclosure generally relates to the treatment and rehabilitation of patients having implanted medical devices. More particularly, the disclosure relates to patient programmers used with implantable neuro-stimulators.

Discussion

[0002] Implantable neuro-stimulators have begun to demonstrate clinical usefulness for a wide variety of conditions such as spinal cord injury, traumatic brain injury (TBI), stroke, Parkinson's disease and Parkinson's tremor. For example, deep brain stimulation (DBS) systems have been used to successfully improve motor control in Parkinson's patients by delivering electrical pulses to selected areas of the brain. While certain developments in neuro-stimulators have advanced rehabilitation and treatment in a number of areas, certain challenges remain.

[0003] For example, when a patient having an implanted device is discharged from a medical facility, the patient is often provided with a patient programmer, which gives the patient limited control over the implanted device. Indeed, early patient programmers often only provided the patient with the ability to turn the implanted device on and off. While more recent patient programmers have given patients slightly more control over the functionality of the implanted device, there still remains considerable room for improvement.

BRIEF DESCRIPTION OF THE DRAWINGS

[0004] The various advantages of the embodiments of the present invention will become apparent to one skilled in the art by reading the following specification and appended claims, and by referencing the following drawings, in which:

[0005] FIG. 1 is a block diagram of an example of a patient programmer according to an embodiment of the invention;

[0006] FIG. 2 is a block diagram of an example of a progress module according to an embodiment of the invention;

[0007] FIG. 3A is a front view of an example of a patient programmer having a pressure bar according to an embodiment of the invention;

[0008] FIG. 3B is a front view of an example of a patient programmer having a plurality of pressure sensors according to an embodiment of the invention;

[0009] FIG. 4 is a flowchart of an example of a method of operating a patient programmer according to an embodiment of the invention;

[0010] FIG. 5A is a flowchart of an example of a process of obtaining progress input from a sensor according to an embodiment of the invention; and

[0011] FIG. 5B is a flowchart of an example of a process of obtaining answers that define progress input according to an embodiment of the invention.

DETAILED DESCRIPTION

[0012] Embodiments of the present invention provide for a patient programmer having a control module, a communication interface, and a progress module. The control module may generate a control signal and the communication interface can transmit the control signal to a generator of a stimulation signal. The progress module can obtain progress input from a patient in which the generator is implanted.

[0013] In another embodiment of the invention, a deep brain stimulation (DBS) patient programmer includes a control module that generates a switching signal, wherein the switching signal instructs a generator of a brain stimulation signal to transition between an on-state and an off-state. A short range wireless interface may transmit the switching signal to the generator. The patient programmer may also include a progress module having a sensor mounted to the patient programmer to obtain a first set of progress inputs from a patient in which the generator is implanted. The progress module can also include a display or other output device that presents a plurality of questions to the patient, and an input device to receive answers to the plurality of questions from the patient. The answers can therefore define a second set of progress inputs. The progress module may further include a memory location to store the first and second sets of progress inputs, wherein the patient programmer can include a wired or wireless interface to transmit report data representing the first and second sets of progress inputs to a clinician programmer.

[0014] In yet another embodiment of the invention, a method of operating a patient programmer can provide for generating a switching signal and transmitting the switching signal from the patient programmer to a generator of a brain stimulation signal. The switching signal can instruct the generator to transition between an on-state and an off-state. The method may also provide for using a progress module of

the patient programmer to obtain progress input from a patient in which the generator is implanted.

[0015] FIG. 1 shows a patient programmer 10 that can generally be used to enhance the treatment and rehabilitation of a patient 12 having an implanted medical device such as a neuro-stimulation generator 14. The generator 14 may be used to deliver electrical pulses to areas of the patient's body such as, for example, the brain, spinal cord, or other parts of the nervous system, via one or more suitable electrical leads (not shown), which may also be implanted in the patient 12. For example, the generator 14 may be implanted by placing the generator 14 in a sub-cutaneous pocket created by making a blunt dissection in the subclavicular region, wherein the generator 14 can include one or more suture holes for securing the generator 14 to the muscle fascia. In addition, the corresponding electrical leads may be tunneled to the distal end of an extension (not shown), and the extension may be tunneled to the generator 14 using well-known implantation procedures.

[0016] In this regard, the generator 14 may have a wide range of non-invasively programmable parameters and stimulation modes, and can exchange parameter information, via telemetry, with a clinician programmer 16 and the patient programmer 10. Communication with the illustrated patient programmer 10 is implemented through a communication interface 20 of the patient programmer 10. The stimulation pulses delivered to each lead can be determined by a parameter called a program, wherein a program can be a specific combination of amplitude, rate and pulse width parameters acting on a specific lead electrode set. For the stimulation signals, example amplitudes might range from 0.0-20.0 mA, example pulse widths may range from 10-1000 μ sec per phase, example frequencies may range from 1-1200 Hz, and the waveform shape might be square, sine, or triangle wave. Other parameter ranges and characteristics may also be used.

[0017] In one embodiment, the clinician programmer 16, which typically runs as an application on a laptop- or PC-based platform, can be used to determine which programs are to be run on the generator 14 and may display instruction prompts for the clinician and show parameter data. The clinician programmer 16 can also be used to provide stimulation parameters and patient programmer adjustment limits for multiple programs, collect measurements and diagnostic data from the generator 14 and may be used to switch the generator 14 on and off, and obtain the battery status

of the generator 14, which may be powered by a hermetically sealed silver vanadium oxide cell, a lithium ion cell, or other state of the art battery chemistries. In particular, upon interrogation by the clinician programmer 16, the generator 14 might transmit via an RF link to the clinician programmer 16 for display or printing: patient progress reports received from the patient programmer 10, model and serial number identification, programmed parameters and values, generator battery status, number of patient activations (since last reset), total stimulation time (since last reset), elapsed time (since last reset) and verification of program changes. After a program entry, the clinician programmer 16 can compare stimulation signal parameters, via telemetry, with the entries made during programming.

[0018] The illustrated patient programmer 10, which may be a relatively small handheld device, has a control module 18 that generates a control signal such as a switching signal to instruct the generator 14 to transition between the on and off state based on control input 28 from the patient 12. Thus, the patient 12 can use the patient programmer 10 to power the generator 14 on and off. Other control input 28 such as selection of program parameters and stimulation modes may also be obtained from the patient 12, although it may be desirable to limit such control by the patient 12 for safety concerns. Likewise, other control signals, such as program parameter and stimulation mode selection signals, may also be generated based on the control input 28 and transmitted to the generator 14. Such control input 28 may be obtained from the patient 12 via an appropriate user interface such as a touch screen display, keypad and/or button. A processor 26 may use the communication interface 20 to transmit the switching signal to the generator 14 wirelessly, using a short range wireless interface such as a WPAN (Wireless Personal Area Network; e.g., IEEE 802.15.4) module, a Bluetooth (e.g., IEEE 802.15.1) module, a WiFi (Wireless Fidelity; e.g., IEEE 802.11) module, or an RF (Radio Frequency) module using the MICS (Medical Implant Communication Service; e.g., 47 CFR 95.601-95.673 Subpart E), for example.

[0019] The patient programmer 10 may also include a progress module 22 that can obtain progress input 24 from the patient 12. Enabling the patient to provide progress input 24 through the patient programmer 10 represents a substantial improvement over conventional approaches. For example, the patient programmer 10 is typically much more accessible to the patient 12 than other devices such as the clinician programmer 16, and the patient programmer 10 tends to be much more

“personal” to the patient. Accordingly, the illustrated patient programmer 10 can collect progress input 24 more frequently (e.g., daily) and is more likely to obtain accurate results and/or truthful responses from the patient 12. In addition, while the patient programmer 10 may have substantially more functionality than traditional patient programmers, the programmer 10 can maintain a desired level of safety by limiting control input 28 to only certain features such as on/off control and predefined parameter set selection. Meanwhile, the illustrated patient programmer 10 is able to provide robust progress input 24 collection and reporting functionality that may significantly enhance patient recovery.

[0020] The progress input 24 may also be used in a closed-loop fashion by the patient programmer 10 to select and/or modify program parameters and/or stimulation modes in real-time, wherein the patient programmer 10 can generate the appropriate control signals and transmit them to the generator 14. In such a case, certain precautions such as patient authentication features can be implemented in order to better ensure patient safety. Examples of such precautions are described in greater detail below.

[0021] The progress input 24 can include measurements taken from sensors mounted on or otherwise coupled to the patient programmer 10, answers to rehabilitation related questions, and so on. The processor 26 can store the progress input 24 to a memory location in read only memory (ROM) 30, random access memory (RAM) 32, or any other suitable memory structure. The progress input 24 can also be transmitted, via the communication interface 20, to the generator 14 as report data, wherein the clinician programmer 16 may obtain the report data from the generator 14 over a long range wireless interface such as an RF telemetry module or a WiMAX (Worldwide Interoperability for Microwave Access; e.g., IEEE 802.16) module, or a short range wireless interface. The clinician programmer 16 may also obtain the report data directly from the patient programmer 10 via a short range wireless interface, wired interface such as a USB (Universal Serial Bus) connection or an Ethernet (e.g., IEEE 802.3) connection, or long range wireless interface, depending upon the circumstances. The short and long range wireless interfaces would be suited for communications that take place during office visits, whereas the long range wireless interface could permit more frequent transmissions of data between the generator 14, patient programmer 10 and the clinician programmer 16.

In addition, the report data may be transmitted to a home monitor and/or Internet connection.

[0022] Turning now to FIG. 2, one example of progress input 24 being obtained from the patient's interaction with a plurality of sensors 34 (34a-34e) is shown. The illustrated sensors 34 may be mounted on the patient programmer, wired to the patient programmer or linked to the patient programmer through a wireless connection, and may be used to assess the progress of the patient. In particular, the patient could perform a task with the patient programmer, wherein the sensors 34 may take measurements associated with the task. For example, the patient could be instructed to manipulate one or more pressure sensors 34a so that the amount of pressure exerted by the patient could be measured and tracked over time to show improvement. In another task, the patient could be asked to pull on a strain gauge (not shown) in order to measure the strength of the patient. A temperature sensor 34b may be used to measure body and/or ambient temperature associated with particular tasks and a motion sensor 34c could be used for a motor skills task such as lifting the patient programmer off of a table and raising it above one's head. The motion sensor 34c may therefore track the speed and duration of the task and output this information for storage on the patient programmer and reporting purposes.

[0023] The illustrated progress module 22 also interacts with sensors external to the patient programmer to give a more complete view of the patient recovery. For example, the motion sensor 34c could interact with a sensor held by the patient during rehabilitation tasks. This interaction could indicate the distance traveled by the patient's extremity during the course of a specific rehabilitation task. Another example is that the motion sensor 34c could interact with a sensor implanted in the patient as part of the implantable therapeutic system. One possibility is that the interaction of these sensors could indicate overall movement of the patient in both body and head movement, which could be informative as to the overall rehabilitation status of the patient. Another possibility is that each of the sensors could generate independent readings, wherein the patient programmer conducts an analysis of the readings to obtain information regarding the patient's progress. The illustrated progress module 22 also includes a heart rate sensor link 34d and an EEG sensor link 34e, which can receive measurement signals from heart rate and EEG sensors coupled to the patient, respectively. Based on the progress input from the EEG sensors, for example (which could detect brain activity, sleep cycles, etc.), the

patient programmer can instruct the patient to perform different tasks. Other sensors, such as chemical pH sensors, may also be used.

[0024] FIG. 3A shows an external view of an example of a patient programmer 36. In particular, the patient programmer 36 may be able to obtain progress input from a patient having an implanted medical device such as a DBS neuro-stimulation generator, store the progress input, and report the progress input to another device such as the generator or a clinician programmer. In the illustrated example, the patient programmer 36 has a display 38, an input device including a plurality of buttons 40 (40a, 40b), and a pressure bar 42. The patient programmer 36 can use the display 38 and/or other output device such as a speaker to provide instructions and information to the patient. The instructions could be output periodically, such as daily, and/or in a closed-loop fashion in response to progress input already obtained from the patient. For example, the patient programmer 36 may use the display 38 to instruct the patient to press on the pressure bar for a certain amount of time, wherein the pressure bar 42 measures the amount of pressure applied by the patient. This progress input may be registered and time stamped by a processor 26 and/or progress module 22 (FIG. 1), and stored to a memory location within the patient programmer 36. Tracking such progress input over time and reporting the information back to the clinician programmer enables the medical professional to more readily ascertain the progress of the patient and the effectiveness of the underlying medical treatment. The progress input from the pressure bar 42 may also be used to select subsequent instructions to be presented to the patient. Examples of instructions include, but are not limited to, instructions to squeeze sensors on the patient programmer 36, press down on sensors on the patient programmer 36, perform range of motion exercises with the patient programmer 36 in hand, pick up and put down the patient programmer 36, and manipulate a button on the patient programmer 36 when an object on the display 38 disappears/appears as part of a reaction time test.

[0025] The display 38 may also be used to present questions to the patient that are tailored to the patient's progress, wherein the patient can provide answers to the questions via the illustrated buttons 40. Thus, the progress input may be obtained from the patient through the illustrated buttons 40 as well as the illustrated pressure bar 42. The questions could be related to the patient's perception of improvement, the patient's psychological state, objective yes/no issues, or anything else related to

the patient’s well-being or state of recovery. In general, questions may be related to quality of life (e.g., physical, emotional, task oriented), object recognition (e.g., display and apple, plane, basketball, etc., and have the patient choose from a multiple choice list what the object is), diary input (e.g., time/date stamp for eating, bathing, voiding), and cognitive state (e.g., IQ).

[0026] For example, Table 1 shows a plurality of Barthel Index questions, which may be presented to the patient on display 38 of the patient programmer 36.

Barthel Index Activity	Score
FEEDING 0 = unable 5 = needs help cutting, spreading butter, etc., or requires modified diet 10 = independent	
BATHING 0 = dependent 5 = independent (or in shower)	
GROOMING 0 = needs to help with personal care 5 = independent face/hair/teeth/shaving (implements provided)	
DRESSING 0 = dependent 5 = needs help but can do about half unaided 10 = independent (including buttons, zips, laces, etc.)	
BOWELS 0 = incontinent (or needs to be given enemas) 5 = occasional accident 10 = continent	
BLADDER 0 = incontinent, or catheterized and unable to manage alone 5 = occasional accident 10 = continent	
TOILET USE 0 = dependent 5 = needs some help, but can do something alone 10 = independent (on and off, dressing, wiping)	
TRANSFERS (BED TO CHAIR AND BACK) 0 = unable, no sitting balance 5 = major help (one or two people, physical), can sit 10 = minor help (verbal or physical) 15 = independent	
MOBILITY (ON LEVEL SURFACES) 0 = immobile or < 50 yards 5 = wheelchair independent, including corners, > 50 yards 10 = walks with help of one person (verbal or physical) > 50 yards 15 = independent (but may use any aid; for example, stick) > 50 yards	
STAIRS 0 = unable 5 = needs help (verbal, physical, carrying aid) 10 = independent	

Table 1

[0027] Table 2 shows a plurality of Short Form 36 (SF-36) Health Survey questions, which may be presented to the patient on display 38 of the patient programmer 36.

SF-36 Health Survey Question	
1. In general, would you say your health is:	<input type="checkbox"/> Excellent <input type="checkbox"/> Very Good <input type="checkbox"/> Good <input type="checkbox"/> Fair <input type="checkbox"/> Poor
2. Compared to one year ago, how would you rate your health in general now?	<input type="checkbox"/> Much better now than a year ago <input type="checkbox"/> Somewhat better now than a year ago <input type="checkbox"/> About the same as one year ago <input type="checkbox"/> Somewhat worse now than one year ago <input type="checkbox"/> Much worse now than one year ago
• • •	
11. How TRUE or FALSE is each of the following statements for you?	a. I seem to get sick a little easier than other people <input type="checkbox"/> Definitely true <input type="checkbox"/> Mostly true <input type="checkbox"/> Don't know <input type="checkbox"/> Mostly false <input type="checkbox"/> Definitely false b. I am as healthy as anybody I know <input type="checkbox"/> Definitely true <input type="checkbox"/> Mostly true <input type="checkbox"/> Don't know <input type="checkbox"/> Mostly false <input type="checkbox"/> Definitely false c. I expect my health to get worse <input type="checkbox"/> Definitely true <input type="checkbox"/> Mostly true <input type="checkbox"/> Don't know <input type="checkbox"/> Mostly false <input type="checkbox"/> Definitely false d. My health is excellent <input type="checkbox"/> Definitely true <input type="checkbox"/> Mostly True <input type="checkbox"/> Don't know <input type="checkbox"/> Mostly false <input type="checkbox"/> Definitely false

Table 2

[0028] Table 3 shows a plurality of Stroke Specific Quality of Life Scale (SS-QOL) questions, which may be presented to the patient on the display 38 of the patient programmer 36.

SS-QOL Item	Score
Energy 1. I felt tired most of the time. 2. I had to stop and rest during the day.	

SS-QOL Item	Score
3. I was too tired to do what I wanted to do.	
Family Roles 1. I didn't join in activities just for fun with my family. 2. I felt I was a burden to my family. 3. My physical condition interfered with my personal life.	
Language 1. Did you have trouble speaking? For example, get stuck, stutter, stammer, or slur your words? 2. Did you have trouble speaking clearly enough to use the telephone? 3. Did other people have trouble in understanding what you said? 4. Did you have trouble finding the word you wanted to say? 5. Did you have to repeat yourself so others could understand you?	
• • •	
Work Productivity 1. Did you have trouble doing daily work around the house? 2. Did you have trouble finishing jobs that you started? 3. Did you have trouble doing the work you used to do?	

Table 3
Copyright © 1997-2007 – Internet Stroke Center

[0029] The patient programmer 36 may also provide instructions for tasks to be performed with other objects, wherein the patient and/or rehab technician may enter performance scores into to the patient programmer. Table 4 shows a plurality of Action Research Arm Test instructions/questions, which may be presented to the patient on the display 38 of the patient programmer 36.

Action Research Arm Test Activity	Score
Grasp 1. Block, wood, 10 cm cube (If score = 3, total = 18 and go to Grip) Pick up a 10 cm block 2. Block, wood, 2.5 cm cube (If score = 0, total = 0 and go to Grip) Pick up 2.5 cm block 3. Block, wood, 5 cm cube 4. Block, wood, 7.5 cm cube 5. Ball (Cricket), 7.5 cm diameter 6. Stone 10 x 2.5 x 1 cm Coefficient of reproducibility = 0.98 Coefficient of scalability = 0.94	
Grip 1. Pour water from glass to glass (If score = 3, total = 12, and go to Pinch) 2. Tube 2.25 cm (If score = 0, total = 0 and go to Pinch) 3. Tube 1 x 16 cm 4. Washer (3.5 cm diameter) over bolt Coefficient of reproducibility = 0.99 Coefficient of scalability = 0.98	
Pinch	

Action Research Arm Test Activity	Score
1. Ball bearing, 6 mm, 3 rd finger and thumb (If score = 3, total = 18 and go to Grossmt) 2. Marble, 1.5 cm, index finger and thumb (If score = 0, total = 0 and go to Grossmt) 3. Ball bearing 2 nd finger and thumb 4. Ball bearing 1 st finger and thumb 5. Marble 3 rd finger and thumb 6. Marble 2 nd finger and thumb Coefficient of reproducibility = 0.99 Coefficient of scalability = 0.98	
Grossmt (Gross Movement) 1. Place hand behind head (If score = 3, total = 9 and finish) 2. (If score = 0, total = 0 and finish) 3. Place hand on top of head 4. Hand to mouth Coefficient of reproducibility = 0.98 Coefficient of scalability = 0.97	

Table 4

[0030] The Action Research Arm Test is ordered so that if the patient passes the first task in a subtest, no more tasks need to be administered and the patient scores top marks for that subtest. If the patient fails the first task and fails the second task, the patient scores zero, and again no more tests need to be performed in that subtest. Otherwise, the patient is instructed to complete all tasks within the subtest.

[0031] The illustrated patient programmer 36 also includes a patient authentication interface such as a fingerprint identification pad 43 to verify that the individual performing tasks, answering questions, and/or otherwise using the patient programmer 36 is in fact the patient. Such a solution is particularly advantageous in closed loop situations wherein real-time modification of simulation signal parameters may be possible. Other biometric authentication solutions such as retinal scans and hair follicle analysis may also be used. To further address safety concerns, the patient programmer 36 may require the patient programmer 36 and the pulse generator to be maintained in proximity to one another, as well as the maintenance of constant communication between the patient programmer 36 and the pulse generator while patient progress input is being obtained.

[0032] FIG. 3B shows an alternative design of a patient programmer 44. In the illustrated example, the patient programmer 44 has a display 38, a plurality of buttons 40 and a plurality of force transducers/pressure sensors 46 (46a, 46b), which may be squeezed by the patient to determine, for example, the patient's hand strength before, during, and/or after delivery of stimulation pulses to a desired treatment site within the patient's body. Thus, the patient programmer 44 may use

the display 38 to instruct the patient to squeeze the pressure sensors 46 for a certain amount of time, wherein the pressure sensors 46 measure the amount of pressure applied by the patient. This progress input may be registered and time stamped by a processor 26 and/or progress module 22 (FIG. 1), and stored to a memory location within the patient programmer 44.

[0033] Turning now to FIG. 4, a method 50 of operating a patient programmer is shown. The method 50 may be implemented in a patient programmer as a set of processor-executable instructions stored in ROM, RAM, electrically erasable programmable ROM (EEPROM), flash memory, etc., as fixed functionality hardware such as an embedded microcontroller, application specific integrated circuit (ASIC), etc. using complementary metal oxide semiconductor (CMOS) technology or transistor-transistor-logic (TTL), or any combination thereof. In the illustrated processing block 52, a switching signal is generated and transmitted to a generator of a stimulation signal, wherein the switching signal instructs the generator to transition between an on state and an off state. Thus, in the illustrated example, the patient programmer is able to power the generator on and off. Block 54 provides for receiving progress input from the patient and block 56 provides for storing the progress input to a memory location on the patient programmer.

[0034] If a link, such as a short range wireless link, to the generator is detected at block 58, report data representing the progress input is transmitted to the generator at block 60. Block 62 provides for determining whether a link to a clinician programmer exists and, if so, report data representing the progress input is transmitted to the clinician programmer at block 64. Once the report data is uploaded to the clinician programmer, the data may be analyzed and displayed graphically, and sorted by specific task and/or date. Graphical display of the data could be used to show trends in improvement levels and gauge the amount of patient recovery, and may lead the medical professional to a change in the stimulation parameters.

[0035] FIG. 5A shows one approach to receiving progress input from the patient at block 66, in which the progress input is obtained from a sensor of the patient programmer. As already discussed, the sensor may be a wide variety of sensors such as pressure sensors, temperature sensors, motion/acceleration sensors, heart rate sensors EEG sensors, strain gauges, and so on.

[0036] FIG. 5B shows an approach to receiving progress input from the patient, wherein a question is displayed to the patient at block 68. As already discussed, the question could be related to the patient's perception of improvement, the patient's psychological state, objective yes/no issues, or anything else regarding the patient's well-being or state of recovery. Block 70 provides for receiving an answer to the displayed question and block 72 provides for determining whether there are any remaining questions. If so, the illustrated process steps through the questions until the last question is completed.

[0037] The present invention also provides methods of monitoring the progress of a patient who has been treated with neuromodulation using a patient programmer as described herein. Such a patient programmer can be used to monitor the progress of various different types of patients including those receiving neuromodulation for treatment of stroke, traumatic brain injury, or other conditions.

[0038] The terms "connected", "coupled" and "attached" are used herein to refer to any type of relationship, direct or indirect, between the components in question, and may apply to electrical, mechanical, RF, optical or other couplings, unless otherwise indicated. In addition, the term "first", "second", and so on are used herein only to facilitate discussion, and do not necessarily infer any type of temporal or chronological relationship.

[0039] Those skilled in the art will appreciate from the foregoing description that the broad techniques of the embodiments of the present invention can be implemented in a variety of forms. Therefore, while the embodiments of this invention have been described in connection with particular examples thereof, the true scope of the embodiments of the invention should not be so limited since other modifications will become apparent to the skilled practitioner upon a study of the drawings, specifications, and following claims.

CLAIMS

What is claimed is:

1. A deep brain stimulation patient programmer comprising:
 - a control module to generate a switching signal, the switching signal to instruct a generator of a brain stimulation signal to transition between an on state and an off state;
 - an authentication interface to verify that an individual using the patient programmer is a patient in which the generator is implanted;
 - a short range wireless interface to transmit the switching signal to the generator;
 - a wireless interface; and
 - a progress module having a sensor mounted to the patient programmer to obtain a first set of progress inputs from the patient, a display to present a plurality of questions to the patient, an input device to receive answers to the plurality of questions from the patient, the answers to define a second set of progress inputs, the progress module further including a memory location to store the first and second sets of progress inputs, the wired interface to transmit report data representing the first and second sets of progress inputs to a clinician programmer.
2. The patient programmer of claim 1, wherein the sensor is at least one of a pressure sensor, a temperature sensor, a motion sensor, a heart rate sensor, a chemical sensor and an electroencephalogram (EEG) sensor.
3. The patient programmer of claim 1, wherein the input device includes at least one of a touch-screen component of the display and a plurality of buttons.
4. The patient programmer of claim 1, wherein the plurality questions include at least one of quality of life questions, object recognition questions, diary questions and cognitive questions.
5. The patient programmer of claim 1, wherein the short range wireless interface includes at least one of a Wireless Personal Area Network (WPAN), a

Bluetooth module, a Wireless Fidelity (WiFi) module and a radio frequency (RF) module.

6. A patient programmer comprising:
a control module to generate a control signal;
a communication interface to transmit the control signal to a generator of a stimulation signal; and
a progress module to obtain progress input from a patient in which the generator is implanted.

7. The patient programmer of claim 6, wherein the progress module includes a sensor.

8. The patient programmer of claim 7, wherein the sensor is at least one of a pressure sensor, a temperature sensor, a motion sensor, a heart rate sensor and an electroencephalogram (EEG) sensor.

9. The patient programmer of claim 6, wherein the progress module includes:
a display to present a plurality of questions to the patient; and
an input device to receive answers to the plurality of questions.

10. The patient programmer of claim 9, wherein the input device includes at least one of a touch-screen component of the display and a plurality of buttons.

11. The patient programmer of claim 9, wherein the plurality questions include questions from at least one of a Barthel Index, a Short Form 36 (SF-36) Health Survey, an Action Research Arm Test and a Stroke Specific Quality of Life Scale (SS-QOL).

12. The patient programmer of claim 6, further including a memory location to store the progress input.

13. The patient programmer of claim 12, wherein the communication interface includes a short range wireless interface, the communication interface to transmit report data representing the progress input to the generator.

14. The patient programmer of claim 12, wherein the communication interface includes at least one of a short range wireless interface, a long range wireless interface and a wired interface, the communication interface to transmit report data representing the progress input to a clinician programmer.

15. The patient programmer of claim 6, further including an authentication interface to verify that an individual using the patient programmer is the patient.

16. A method of operating a patient programmer comprising:
generating a switching signal;
transmitting the switching signal from the patient programmer to a generator of a stimulation signal, the switching signal to instruct the generator to transition between an on state and an off state; and
using a progress module of the patient programmer to obtain progress input from a patient in which the generator is implanted.

17. The method of claim 16, wherein the progress input is obtained from a sensor of the patient programmer.

18. The method of claim 16, wherein the progress input is obtained by displaying a plurality of questions to the patient and receiving answers to the plurality of questions.

19. The method of claim 16, further including storing the progress input to a memory location on the patient programmer.

20. The method of claim 16, further including transmitting report data representing the progress input to the generator.

21. The method of claim 16, further including transmitting report data representing the progress input to a clinician programmer.

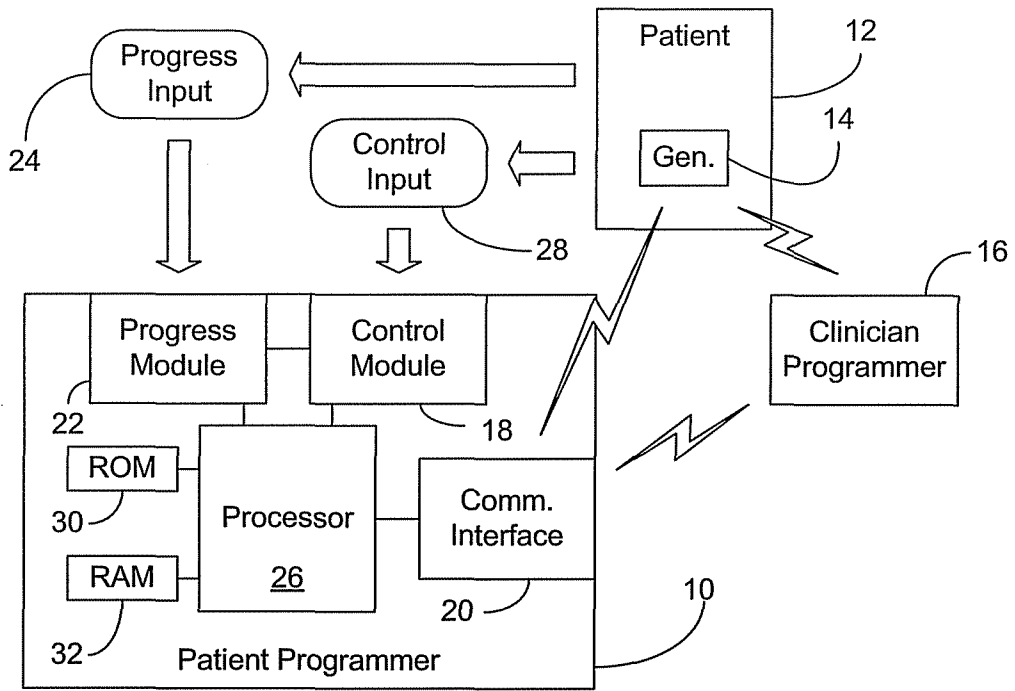


FIG. 1

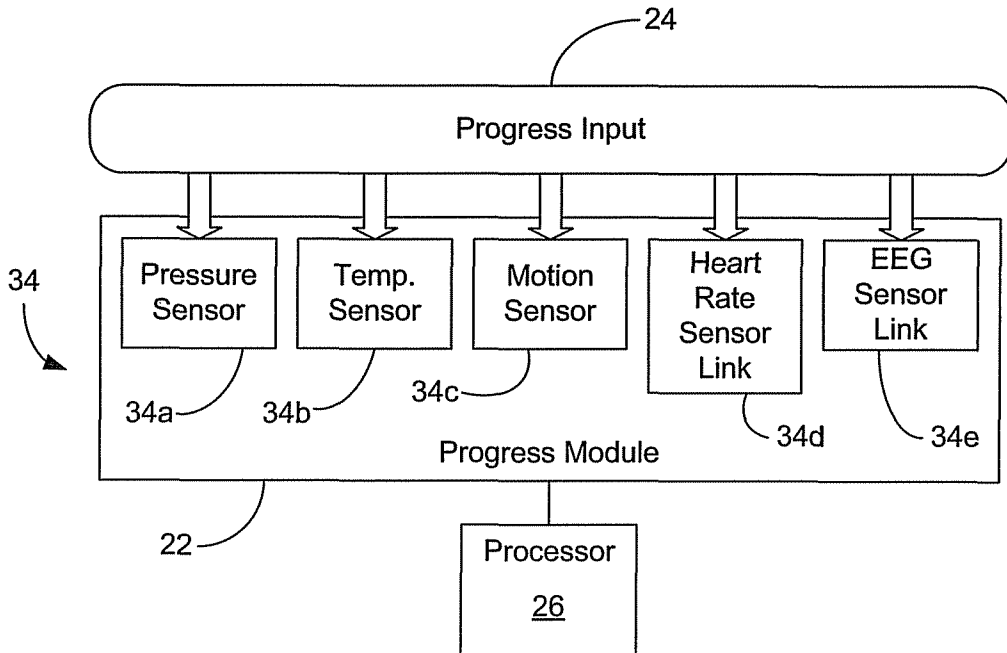


FIG. 2

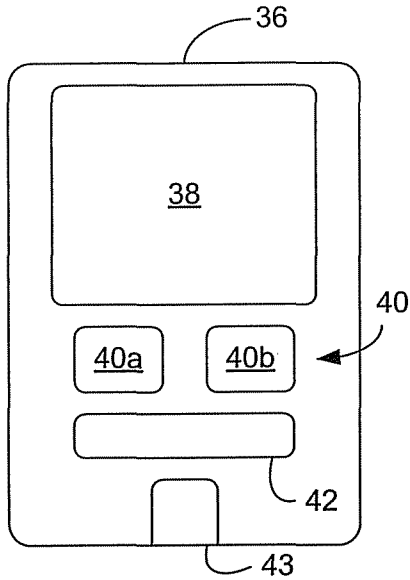


FIG. 3A

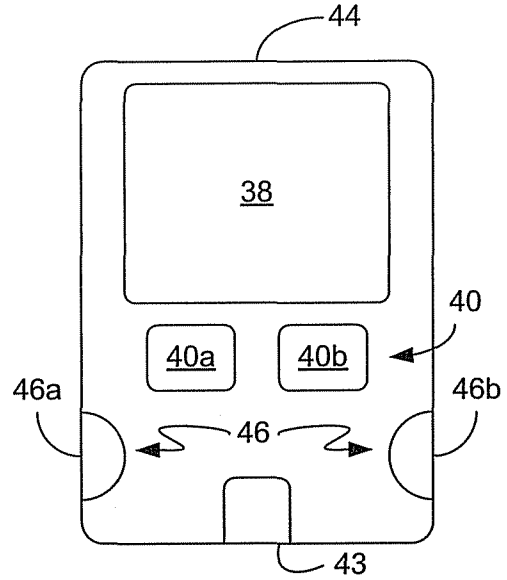


FIG. 3B

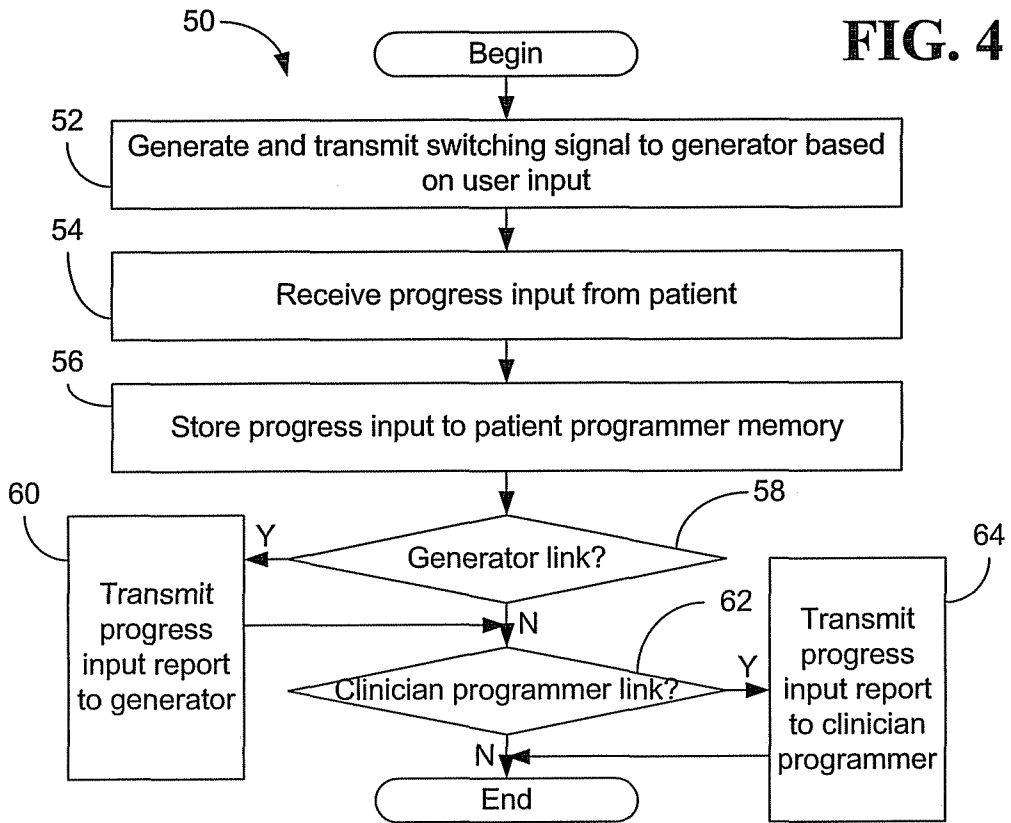


FIG. 4

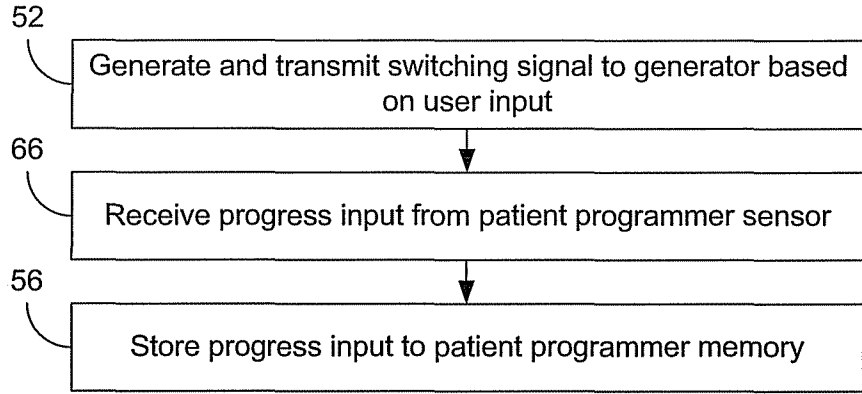


FIG. 5A

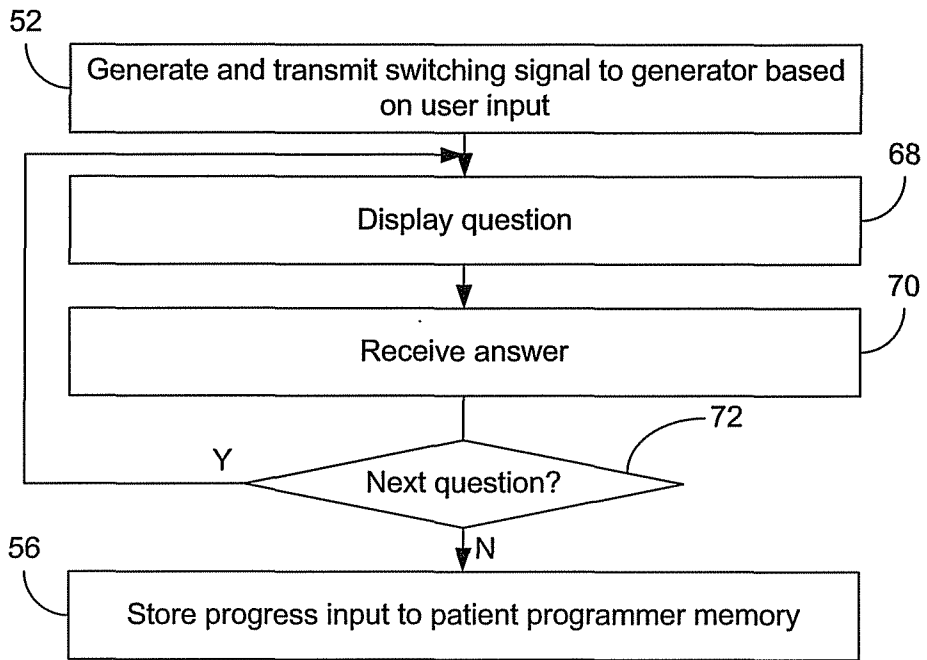


FIG. 5B

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 08/78433

A. CLASSIFICATION OF SUBJECT MATTER IPC(8) - A61B 5/00 (2008.04) USPC - 600/300 According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) USPC 600/300 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched All USPC; USPC 600/300, 600/301; IPC A61B 5/00 (text search) Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) PubWEST(USPT,PGPB,EPAB,JPAB); Google; deep brain stim\$; control; module; switch; signal; generator; on; off; state; authenti\$; short range wireless; sensor; display; input; answer; memory; pressure; temperature; motion sensor; heart rate; chemical; electroencephalogram; EEG; touch screen; button; etc.		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2004/0054297 A1 (Wingeier, et. al.) 18 March 2004 (18.03.2004); para [0107], [0121]-[0122], [0125]-[0126], [0129]-[0136]	1-21
Y	US 2006/0218007 A1 (Bjorner, et. al.) 28 September 2006 (28.09.2006); Abstract; para [0014], [0021], [0046], [0054], [0056], [0103], [0125]	1-21
Y	US 2004/0152957 A1 (Stivoric, et. al.) 05 August 2004 (05.08.2004); Abstract; para [0065], [0083]	1-5, 15
<input type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/>		
* Special categories of cited documents: "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family	
Date of the actual completion of the international search 11 November 2008 (11.11.2008)	Date of mailing of the international search report 05 DEC 2008	
Name and mailing address of the ISA/US Mail Stop PCT, Attn: ISA/US, Commissioner for Patents P.O. Box 1450, Alexandria, Virginia 22313-1450 Facsimile No. 571-273-3201	Authorized officer: Lee W. Young PCT Helpdesk: 571-272-4300 PCT OSP: 571-272-7774	

专利名称(译)	具有输入和传感功能的患者编程器		
公开(公告)号	EP2211691A4	公开(公告)日	2010-12-08
申请号	EP2008838653	申请日	2008-10-01
[标]申请(专利权)人(译)	INTELECT 医疗		
申请(专利权)人(译)	INTELECT MEDICAL INC.		
当前申请(专利权)人(译)	INTELECT MEDICAL INC.		
[标]发明人	KOKONES SCOTT CARLTON KEITH		
发明人	KOKONES, SCOTT CARLTON, KEITH		
IPC分类号	A61B5/00 A61N1/08 A61N1/36 A61N1/372		
CPC分类号	A61N1/37235 A61N1/36082 A61N1/37247		
优先权	11/873842 2007-10-17 US		
其他公开文献	EP2211691A1		
外部链接	Espacenet		

摘要(译)

患者程序员可以具有进展模块，其中进展模块可以从植入发生器的患者获得进展输入。进展模块可以包括能够基于患者与耦合到患者程序员的传感器的交互来获得进展输入的传感器。进度模块还可以包括向患者提出与进展相关的问题并获得对来自患者的问题的响应的界面。患者程序员还能够存储进度输入以用于报告目的。