

(19)



(11)

**EP 1 222 894 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention  
of the grant of the patent:  
**26.01.2011 Bulletin 2011/04**

(51) Int Cl.:  
**A61B 5/00** (2006.01) **A61B 5/055** (2006.01)

(21) Application number: **01310925.1**

(22) Date of filing: **28.12.2001**

**(54) Reusable pulse oximeter probe and disposable bandage**

Wiederverwendbare Pulsoximetersonde mit wegwerfbarer Bandage

Sonde oxymètre réutilisable avec un bandage jetable

(84) Designated Contracting States:  
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU  
MC NL PT SE TR**

(30) Priority: **11.01.2001 US 758038**

(43) Date of publication of application:  
**17.07.2002 Bulletin 2002/29**

(73) Proprietor: **Masimo Corporation**  
**Irvine, CA 92618 (US)**

(72) Inventor: **Parker, Brent**  
**Murietta,**  
**CA 92563 (US)**

(74) Representative: **Vossius & Partner**  
**Siebertstrasse 4**  
**81675 München (DE)**

(56) References cited:  
**WO-A-00/21433 WO-A-00/42911**  
**WO-A-92/21281 US-A- 5 273 041**  
**US-A- 5 279 295 US-A- 5 387 122**  
**US-A- 5 437 275 US-A- 5 664 270**  
**US-A- 5 786 592 US-A- 5 910 108**  
**US-A- 5 991 648 US-A- 6 014 576**

**EP 1 222 894 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

**[0001]** Heretofore the use of pulse oximeter probes has been limited to the use of a costly reusable probe, which is contaminated by use on a patient, or cheaper, single-use probes, which, in the aggregate, amount to a considerable expenditure for a health care institution. The present invention relates to a method of making and affixing a reusable probe to a patient by means of disposable bandage apparatus so that there is no contact between the costly, reusable portion of the probe and the patient. The contaminated bandage apparatus, which is relatively inexpensive, can then be discarded after single patient use and the probe can be reused with a new bandage apparatus.

**[0002]** Others have attempted to convert single-use probes into multi-use probes through a lamination process. In that process, the original adhesive material is removed from the original manufacturer's sensor. The sensor is then laminated in a plastic sheath and the entire sheath is then inserted into a transparent, adhesive-backed sleeve, which is then adhered to a patient. After use, the probe can then be extracted from the sleeve and inserted into a new sleeve for use on another patient.

**[0003]** There are certain disadvantages to this method. Firstly, it is difficult to insert the flexible laminated sensor into a long sleeve. Secondly, the thickness of a laminated sensor inside of a sleeve makes it difficult to bend around, and to stick properly to, a human appendage. Thirdly, transmission and reception of infrared light can be affected by extraneous light entering from the sides of the sleeve. And, Fourthly, there is some dispute as to the affect on infrared light transmission when passing through the sleeve and the adhesive material coupled thereto.

**[0004]** One of the problems with pulse oximetry, and the continuity of monitoring a patient, is the vast array of different monitors used in different hospital departments. Many times a patient will start out in the emergency room (ER) where the hospital utilizes one particular brand of monitor. If a disposable probe is affixed to the patient, and the patient is then admitted to intensive care, the disposable probe that was affixed in the ER will only work if the pulse oximeter used in intensive care is of the same make as the one in the ER. If that same patient is once again taken to radiology, or to have an MRI done, once again these different departments may have different pulse oximeter monitors. What happens many times is that the disposable probes affixed in one department are thrown away and new ones are affixed in other departments. Obviously, this creates additional expense in providing pulse oximetry monitoring.

**[0005]** A device according to the preamble of claim 1 is known from document WO-A-00/21344.

**[0006]** The present invention is a device as defined in claim 1. It solves the problems outlined above and offers an alternative that is cheap to manufacture and easy to use. The present invention relates also to the use of a

device according to claim 1 as defined in claim 2.

**[0007]** The device of the present invention facilitates the intra-departmental or inter-institutional transport of a patient or patients requiring the pulse oximeter monitoring, and wherein said pulse oximeters used for monitoring said patient may be of different manufacturers. The device allows to affix to said patient a bandage apparatus having receptacles incorporated thereon, providing each said different manufacturers' pulse oximeter probe with modular housings adapted to matedly engage and/or disengage with receptacles of the disposable bandage apparatus, thus enabling said patient to be monitored by pulse oximeters of different manufacturers without changing the affixed bandage apparatus.

**[0008]** With the present invention, intra-departmental or inter-institutional transport is greatly facilitated by having a bandage device which will accept probes of various manufacturers, as long as those probes contain housings that will matedly engage the receptacles of the disposable bandage apparatus.

**[0009]** A disposable bandage apparatus which is a bandage strip having adhesive on at least a portion of at least one face thereof and at least two plastic receptacles mounted thereon, each receptacle having at least one aperture or radiation transparent window located therein. The probe housings matedly engage the bandage receptacles and transmit and receive light through the apertures or radiation transparent windows of the mated housings and receptacles, and through the appendage of a patient. The apertures of the receptacles are large enough to accept the tubular protrusions of the housings for the purpose of concentric location and alignment of the housings to the receptacles and the proper transmission and reception of light therethrough. Sandwiched between the adhesive strip and the receptacles attached thereto, are translucent silicone windows or windows of another radiation transparent material for isolation of the reusable probe assembly from the patient. The bandage apparatus may be discarded after single patient use and the reusable probe may be used again on another patient in conjunction with another bandage apparatus. Additionally, the receptacles of the bandage apparatus may have a concave surface on one side thereof in order to seat conformably on a human digit, or they have a flat surface on at least one side thereof in order to attach conformably to a human foot, nose, or ear. The housings and receptacles also contain "mushroom hook" type hook and loop material for the purpose of adhering and detaching the housings to and from the receptacles. Additionally, the housings and receptacles have recessed areas for adhesion of the "mushroom hook" hook and loop material.

**[0010]** The above and other advantages of the invention will become more clear when considered with the following specification and accompanying drawings wherein:

Figure 1 is an exploded view of a reusable pulse oximeter probe and disposable bandage apparatus;

Figure 2 is a view of the reusable pulse oximeter probe and disposable bandage apparatus shown individually as components;

Figure 3 illustrates the probe in use on a human finger or digit;

Figure 4 illustrates an exploded view of another reusable pulse oximeter probe in which the "mushroom hook" material itself is used as the receptacle of the disposable bandage apparatus;

Figure 5 illustrates an assembled view of the reusable pulse oximeter sensor in which the light-emitting diode and photocell detector of the reusable probe are mounted in modular housings with locking levers;

Figure 6 illustrates an exploded view of the reusable pulse oximeter sensor;

Figure 7 illustrates an exploded view of the bandage apparatus in which the receptacle tops incorporate a slot for engaging the locking levers of the modular probe housings, and wherein the radiation transparent windows are mounted on the opposite side of the bandage strip thus sandwiching and securing the bandage in between the two receptacle halves by means of locking levers;

Figure 8 illustrates the reusable pulse oximeter probe as it would appear ready for use on a human digit;

Figure 9 is a patient flow diagram showing the intra-departmental or inter-institutional transport of a patient, and

Figure 10 is a schematic illustration of how the probe housings utilizes a fiberoptic cable connecting the light emitter and detector to the disposable bandage according to the invention.

[0011] Figs. 1-8 do not fall under the wording of the claims.

### Description of the Reusable Pulse Oximeter Sensor

[0012] The reusable pulse oximeter sensor constitutes a "Y" style pulse oximeter probe shown in Figure 1, Item F. The probe incorporates two plastic housings shown as Figure 1, Items G. The housings contain apertures or radiation transparent windows L therein. One housing contains the light-emitting diode of the probe, Figure 1, Item H, and other contains the photocell detector, Figure 1, Item I. The emitter and detectors are aligned with the apertures or windows L of the housings in order to transmit and receive light through a human appendage.

[0013] Seated within a recessed area of each housing, and attached permanently thereto, is a "mushroom hook" adhesive-backed pad, Figure 1, Item K. The purpose of these pads is to selectively engage the "mushroom hook" pads, Figure 1, Items J, attached permanently to the plastic discs, Figure 1, Items D, and to attach the reusable probe assembly to the Disposable Bandage Apparatus. The reusable pulse oximeter sensor is shown assembled as Figure 2, Item A.

[0014] In the preferred embodiment of the reusable pulse oximeter sensor, the light-emitting diode (Figure 5, Item A) and photocell detector (Figure 5, Item B) of the probe assembly are housed in modular receptacles (Figure 5, Items C) having locking levers (Figure 5, Items D) for engaging the receptacles of the disposable bandage apparatus, and locking them into place. In this embodiment, the light-emitting diode (Figure 6, Item A) and the photocell detector (Figure 6, Item B) are sandwiched between interlocking receptacle halves, the bottom halves of which (Figure 6, Items C) are made of a radiation transparent material. According to the present invention, intra-departmental or inter-institutional transport is greatly facilitated by having a bandage device which will accept probes of various manufacturers, as long as those probes contain housings that will matedly engage the receptacles of the disposable bandage apparatus.

### Description of the Disposable Bandage Apparatus

[0015] The components of the apparatus include an adhesive-backed strip, shown as Figure 1, Item A, the strip A incorporating two oval protrusions B centered thereon and shown as Figure 1. The strip also incorporates two apertures, centrally located within the oval protrusions, each aperture C having a diameter sufficient in size to accommodate the transmission and reception of light from a light-emitting diode and photocell detector of a pulse oximeter probe.

[0016] On top of the apertures C are seated two plastic discs, Figure 1, Item D, each having a concave base designed to conform to the radius of a human digit, and an aperture of slightly larger diameter than the apertures in the adhesive backed planar strip. The plastic discs are affixed to the adhesive planar strip by means of a permanent adhesive.

[0017] Seated in a recessed area on top of each plastic disc is a "mushroom hook", adhesive backed pad shown as Figure 1, Item J. The purpose of the "mushroom hook" pads is to selectively engage the "mushroom hook" pads attached to the probe, Figure 1, Items K, and to attach the probe to the disposable bandage apparatus. Sandwiched between the two plastic discs and the planar adhesive strip are two translucent silicone windows, Figure 1, Item E. The windows are designed to permit the passage of infrared light and yet prevent contact between probe and patient, and consequently, contamination of the reusable probe itself.

[0018] The above items constitute the disposable bandage apparatus of the invention, the apparatus being shown assembled as Figure 2, Item B.

[0019] In another embodiment of the invention, the disposable bandage apparatus may be configured as in Figure 4 of the drawings. Figure 4 is an exploded view of the apparatus in which the "mushroom hook" pads of the bandage apparatus, Figure 4, Items J, are bonded directly to the adhesive planar strip, Figure 4, Item A, for the selective engagement of the "mushroom hook" pads

of the probe, Figure 4, Items K, the pads being attached permanently to the housings of the probe, Figure 4, Items G.

[0020] In the preferred embodiment of the disposable bandage apparatus, the bandage strip (Figure 7, Item A) is sandwiched between interlocking receptacle halves. The top halves of the receptacles (Figure 7, Items B) contain locking levers (Figure 7, Items C) that are pushed through slots cut in the bandage strip (Figure 7, Items D) and lockingly engage indentations (Figure 7, Items E) in the bottom halves of the receptacles (Figure 7, Items F), thus sandwiching and locking the bandage in between. The bandage strip contains two apertures (Figure 7, Items G) for the transmission and reception of light from the light-emitting diode and photocell detector of the pulse oximeter sensor which are encased in modular housings having locking levers (Figure 5, Items D) where-in the levers engage slots in the receptacles (Figure 7, Items H) thereby locking the housings into place within the receptacles. In addition, the bottom halves of the receptacles (Figure 7, Items F) are of a radiation transparent material, thus allowing the light-emitting diode and photocell detector contained in the probe housings, when engaged in the bandage receptacles, to transmit and receive light through the apertures of the bandage strip and through the radiation transparent material of the bottom halves of the receptacles, and through the appendage of a patient. The complete reusable pulse oximeter probe and bandage assembly is shown assembled and ready for use on a human digit in Figure 8.

#### Other Fastening Means

[0021] As can be appreciated, there are many ways of fabricating the above components of the invention. The above description describes attachment of the reusable pulse oximeter sensor to the disposable bandage apparatus by way of a "mushroom hook" type hook and loop material and by the use of telephone type modular connectors and receptacles. In addition to this means, a number of other methods may be used including standard hook and loop material, "ring and groove" type snap-on connectors, "push and twist" type Luerlock connectors, and threaded flange type connectors.

#### Method of Use

[0022] For use on each individual patient, the probe is affixed in the following manner:

Firstly, the backing is removed from the adhesive strip of the disposable bandage apparatus. One of the apertures of the apparatus is visually positioned on the center of the nail bed of the patient's appendage and one side of the adhesive strip and the oval protrusions are adhered to the patient's digit. The rest of the strip is then looped over the end of the patient's appendage, and the plastic disc is aligned

so as to exactly oppose the plastic disc already attached to the other side of the digit. Once the disposable bandage apparatus has been properly adhered to the patient, the plastic housings of the probe assembly can be easily snapped into place on opposing sides of the digit. The entire assembled probe is shown as it would appear in use on a patient in Figure 3.

[0023] For use with each patient, the modular probe and bandage assembly, which is the preferred embodiment of the invention, would be attached as follows:

Firstly, the backing is removed from the adhesive strip. The strip is then folded where indicated on the bandage and the strip is then adhered to opposing sides of the human digit. Once the bandage apparatus is in place, the housings of the probe are pushed into the receptacles and locked in place by means of the locking levers. When the patient is moved between different service areas of a hospital, the probes can be removed and the patient transported to a new service area where that area's oximeter probes are pushed into the receptacles for further oximeter readings.

[0024] As shown in Figure 9, the invention is easily adaptable to different manufacturers' oximeters being used in different departments or institutions when the patient is to be transported between the departments or institutions. As shown in Figure 9, at the admissions area AD, when the patient is admitted to the hospital or facility, an oximeter bandage is initially applied. Then the patient may go through another testing area or department D1 where various serological, pathological tests may be run. Then the patient is shown as being transported to a radiology area such as where X-ray and magnetic resonance images (MRI) scans are made. Other departments may have the patient transported thereto such as a surgery department DS and a recovery room RR and the patient's room PR where, in each instance, a different manufacturer or different oximeter probes may be attached where, according to the invention, the receptacles on the bandages are able to receive and retain housings on the emitter and detector elements of the probe.

[0025] An example of the flexibility of the system of this invention is illustrated in Figure 10. In this pictorial embodiment, a magnetic resonance image system or an MRI machine is shown as being positioned in one room with the patient and having applicant's disposable bandage apparatus attached to the finger of a patient. In this case, the patient is in the MRI facility where the patient is just having MRI work done. The probe housings are shown attached at the ends of fiberoptic cable connected to a connector which has the light-emitting diode and the light detector incorporated therein with a connector or plug for plugging into a pulse oximeter PO. The light-emitting and light-receiving ends of the fiberoptic cable

are directed or oriented in the modular housings to emit IR light into the finger and receive IR light transmitted through the finger. It will be noted that since in the MRI application no ferrous materials are allowed, the LED's are placed in a room many feet away (up to fifty or more feet away) and the oximeter device is in optimal communication with the applicant's bandage apparatus. Thus, since non-ferrous materials are required, the probe has non-ferrous housings and materials designed to matedly engage with the receptacles of applicant's disposable bandage apparatus. The housings of the probe are in fiberoptic communication with the LED's which are at the other end of the probe near the pulse oximeter.

**[0026]** As shown above, in case of magnetic resonance imaging (MRI) situations where the presence of any metal in the environment can effect the MRI readings, the probe and emitter elements are situated remotely from the MRI machine and fiberoptic cable conveys light to and from the patient's finger. The oximeter probe housings are the termination ends of the fiberoptic cable and the modular housings are therefore able to be inserted into the bandage receptacles and the oximeter readings taken in this fashion from a remote area.

**[0027]** In all embodiments of the invention, when the probe is no longer required on the patient, the housings of the reusable probe are simply unsnapped from the disposable bandage apparatus, the bandage apparatus is thrown away, and the probe can then be reused on a new patient in conjunction with a new bandage apparatus.

#### ADVANTAGES OF THE PRESENT INVENTION

**[0028]** Intra-departmental or inter-institutional transport is greatly facilitated by having a bandage device which will accept probes of various manufacturers, as long as those probes contain housings that will matedly engage the receptacles of the disposable bandage apparatus.

- Current reusable pulse oximeter probes are either "clam shell" type clamping devices which can restrict circuit or "Y" type probes which are taped directly to the patient. Both types also come in direct contact with the patient's skin and bodily fluids and need sterilization after use. Because of the fact that these devices incorporate many surfaces and at times, porous materials, proper sterilization is very difficult. With the present invention there is no contact between the reusable probe and the skin or bodily fluids of the patient.
- Disposable probes are very costly because of the fact that the cable, connectors and photodiodes are all disposed of after use. the present invention accomplishes the same goals as a disposable probe from a cleanliness standpoint, but since only the attachment apparatus is discarded after use, the cost is much less to a healthcare institution.

- With the concave shape of the plastic discs of the bandage apparatus, when backed by the adhesive strip, the device is extremely effective in preventing the entrance of extraneous light from the sides of the patient's digit.

**[0029]** Current probes on the market, whether disposable or reusable, because of the nature of their shape and affixation means, have problems in dealing with extraneous light reception.

- The present invention is facilitated by easy snap-on, snap-off, or modular connector attachment means for attaching the probe to the disposable bandage apparatus. Probe-shield type devices available in the past not only required the modification of the original manufacturer's probe, but required the difficult procedure of inserting a flexible laminated probe into a sheath for each patient.
- Probe-shield devices, because of the lamination process involved, raised some concern over the transmission and reception of infrared light through the laminating material. The present invention uses a silicone window for the isolation of the probe from the patient. Infrared light transmission and reception is not affected by passage through translucent silicone.
- In these days of environmental consciousness, the annual waste generated from tens of millions of disposable probes is enormous. The present invention, if used in considerable numbers, would greatly reduce the amount of environmental waste generated by disposable pulse oximeter probes.

**[0030]** While the invention has been described in relation to preferred embodiments of the invention, it will be appreciated that other embodiments, adaptations and modifications of the invention will be apparent to those skilled in the art.

#### Claims

1. A device for use with a pulse oximeter; the device comprising:

a reusable pulse oximeter probe comprising a cable having a first end and a second end, the first end of the cable comprising a connector having a plug for plugging into a pulse oximeter, the second end of the cable comprising a pair of modular housings, the modular housings being adapted to, respectively, emit and receive light, and

a disposable bandage comprising receptacles positionable on each side of a digit of a patient; wherein the modular housings of the reusable probe are insertable into the receptacles of the

disposable bandage, and wherein the modular housings are capable of being unsnapped from the recaptacles; **characterized in that** the cable is a fiberoptic cable, the connector has a light-emitting diode and a light detector incorporated therein, and the modular housings are non-ferrous modular housings.

2. Use of the device of claim 1 in combination with an MRI machine and a pulse oximeter located at a remote location from the MRI machine, wherein the reusable probe connects the pulse oximeter to the disposable bandage fitted on the patient.

## Patentansprüche

1. Vorrichtung zur Verwendung mit einem Pulsoximeter, wobei die Vorrichtung aufweist:

eine wiederverwendbare Pulsoximetersonde mit einem Kabel, das ein erstes Ende und ein zweites Ende hat, wobei das erste Ende des Kabels einen Verbinder mit einem Stecker zum Einstecken in ein Pulsoximeter aufweist, das zweite Ende des Kabels ein Paar Modulgehäuse aufweist und die Modulgehäuse geeignet sind, jeweils Licht abzustrahlen und zu empfangen, und

eine Wegwerfbandage mit Aufnahmen, die auf jeder Seite eines Digitus eines Patienten positionierbar sind;

wobei die Modulgehäuse der wiederverwendbaren Sonde in die Aufnahmen der Wegwerfbandage einsetzbar sind und wobei die Modulgehäuse aus den Aufnahmen ausgerastet werden können;

**dadurch gekennzeichnet, daß** das Kabel ein faseroptisches Kabel ist, der Verbinder eine Leuchtdiode und einen Lichtdetektor hat, die darin eingebaut sind, und die Modulgehäuse nichteisenhaltige Modulgehäuse sind.

2. Verwendung der Vorrichtung nach Anspruch 1 in Kombination mit einer MRI-Maschine und einem Pulsoximeter, das an einer entfernten Stelle von der MRI-Maschine angeordnet ist, wobei die wiederverwendbare Sonde das Pulsoximeter mit der am Patienten angebrachten Wegwerfbandage verbindet.

## Revendications

1. Dispositif à utiliser avec un sphygmo-oxymètre, le dispositif comprenant : une sonde réutilisable de sphygmo-oxymètre comprenant un câble possédant une première extrémité et une deuxième extrémité,

la première extrémité du câble comprenant un raccord possédant une fiche à des fins d'enfichage dans un sphygmo-oxymètre, la deuxième extrémité du câble comprenant une paire de boîtiers modulaires, les boîtiers modulaires étant conçus pour respectivement émettre et recevoir de la lumière, et un bandage à jeter comprenant des logements qui peuvent venir se placer sur chaque côté d'un doigt d'un patient, dans lequel les boîtiers modulaires de la sonde réutilisable peuvent venir s'insérer dans les logements du bandage à jeter et dans lequel les boîtiers modulaires peuvent être détachés rapidement des logements, **caractérisé en ce que** le câble est un câble de fibre optique, le raccord possède une diode électroluminescente et un détecteur de lumière qui y sont incorporés, et les boîtiers modulaires sont des boîtiers modulaires non ferreux.

2. Utilisation du dispositif selon la revendication 1, en combinaison avec un appareil d'imagerie par résonance magnétique et un sphygmo-oxymètre disposé à distance de l'appareil d'imagerie par résonance magnétique, la sonde réutilisable reliant le sphygmo-oxymètre au bandage à jeter disposé sur le patient.

FIGURE 1

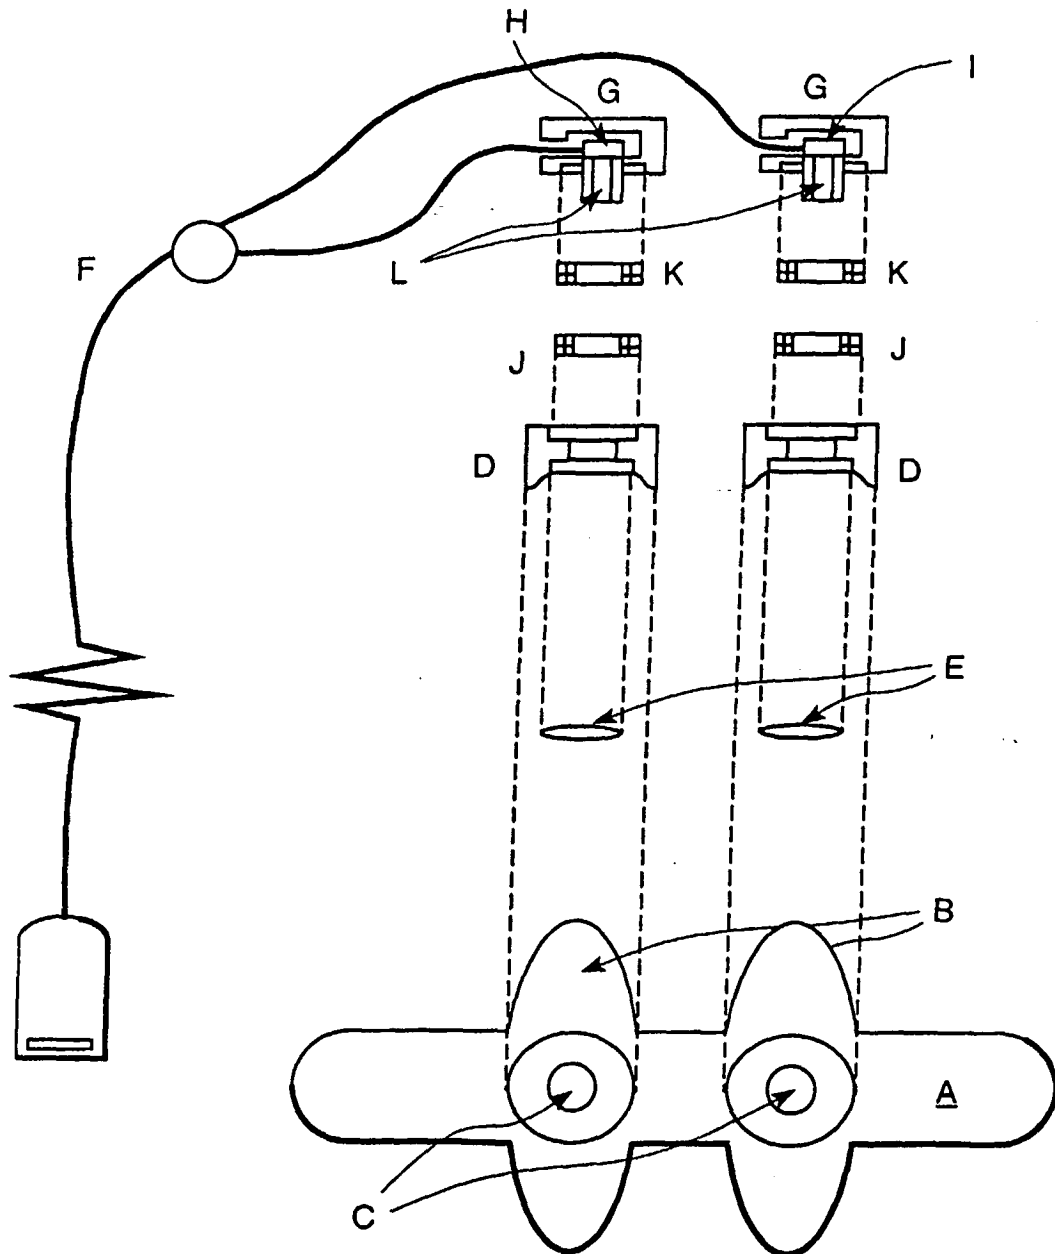


FIGURE 2

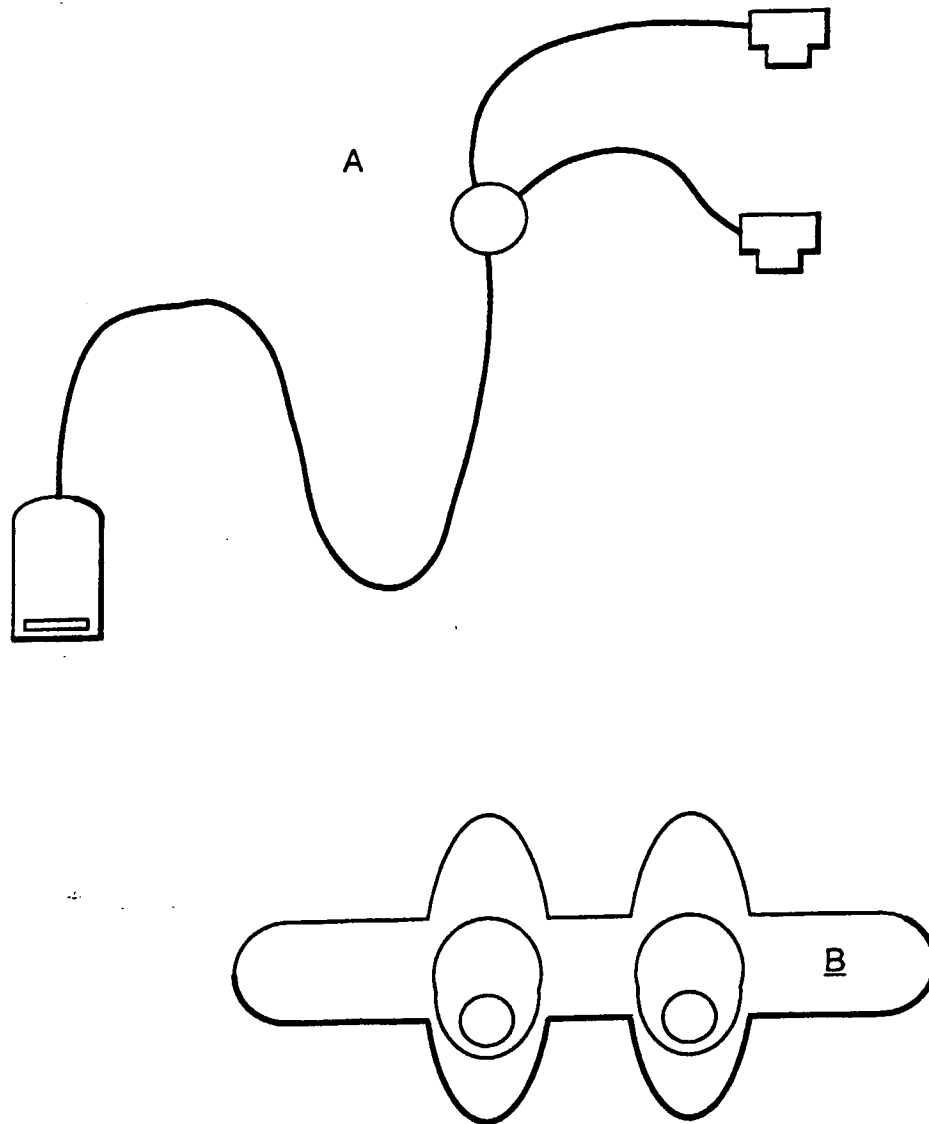




FIGURE 3

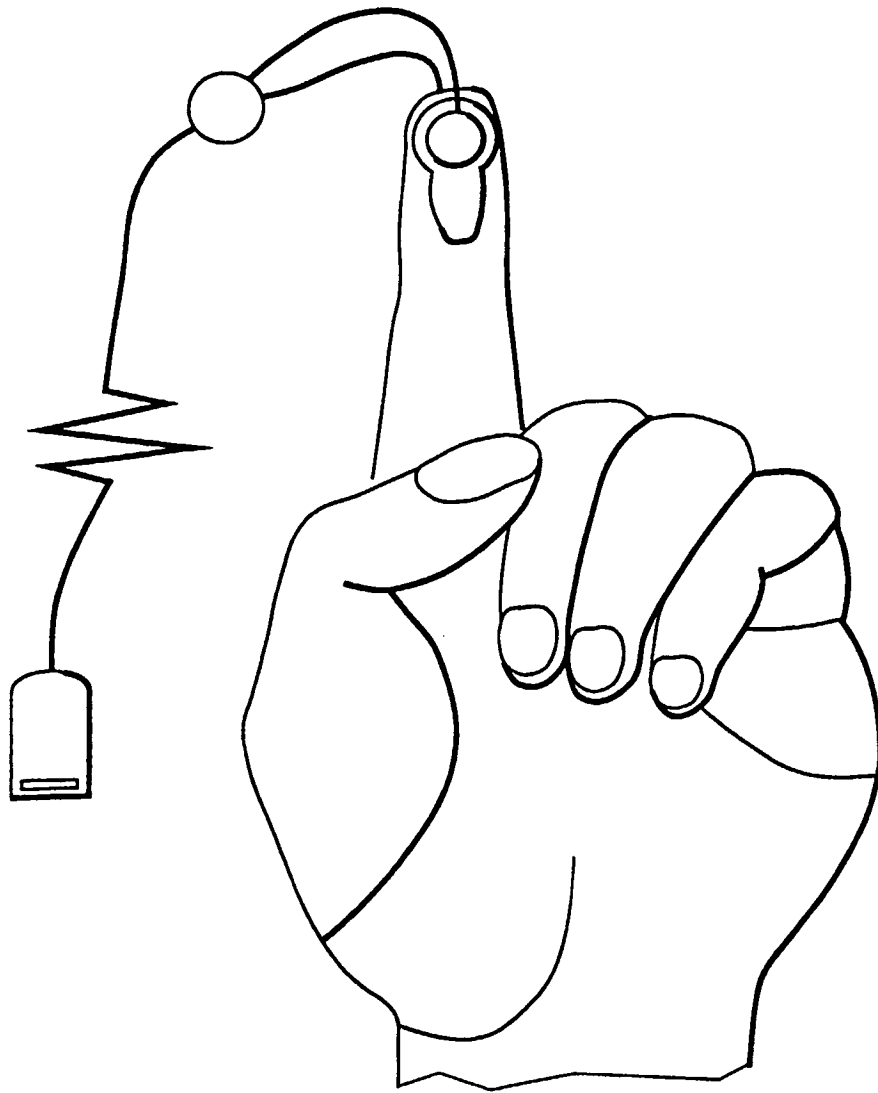


FIGURE 4

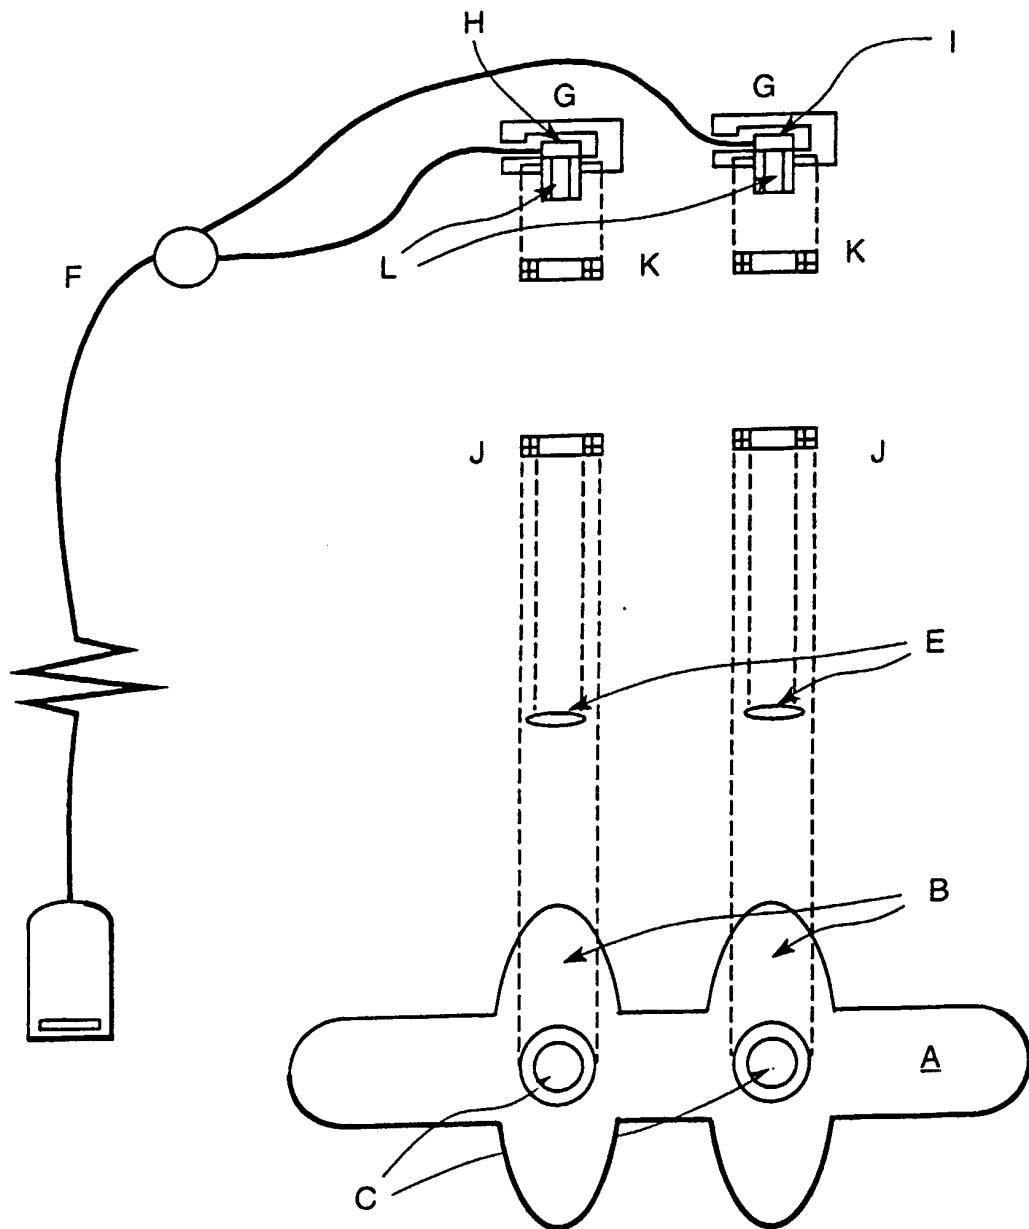


FIGURE 5

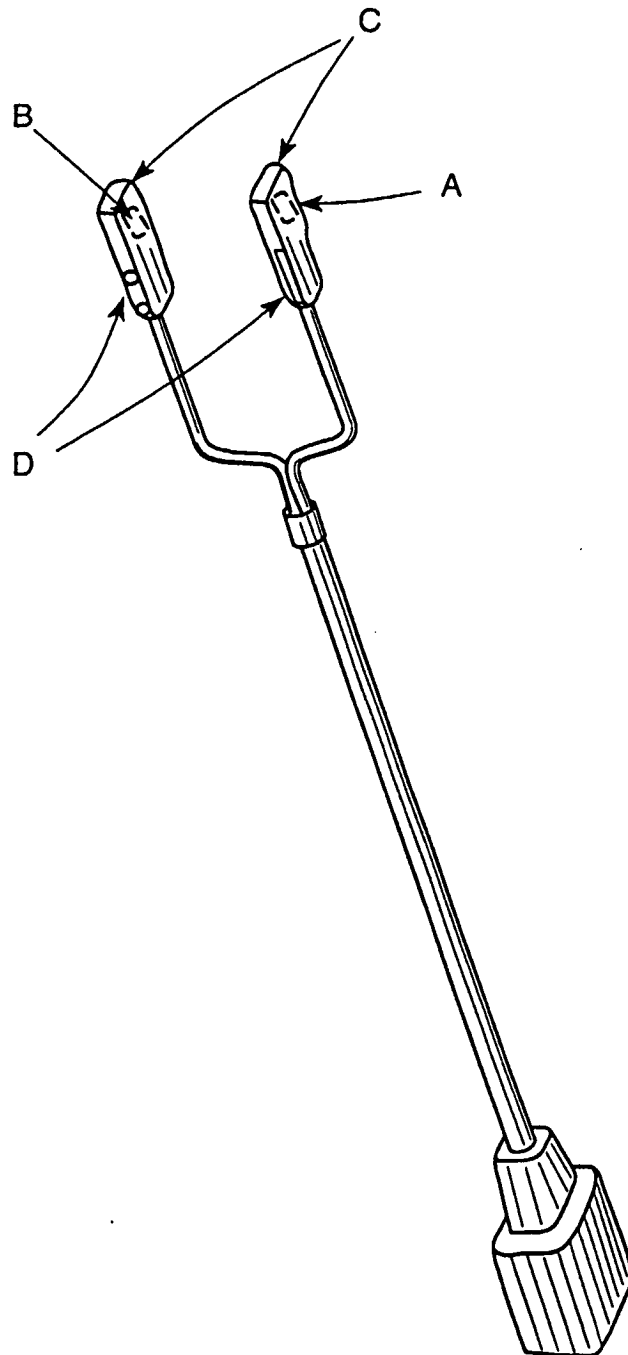


FIGURE 6

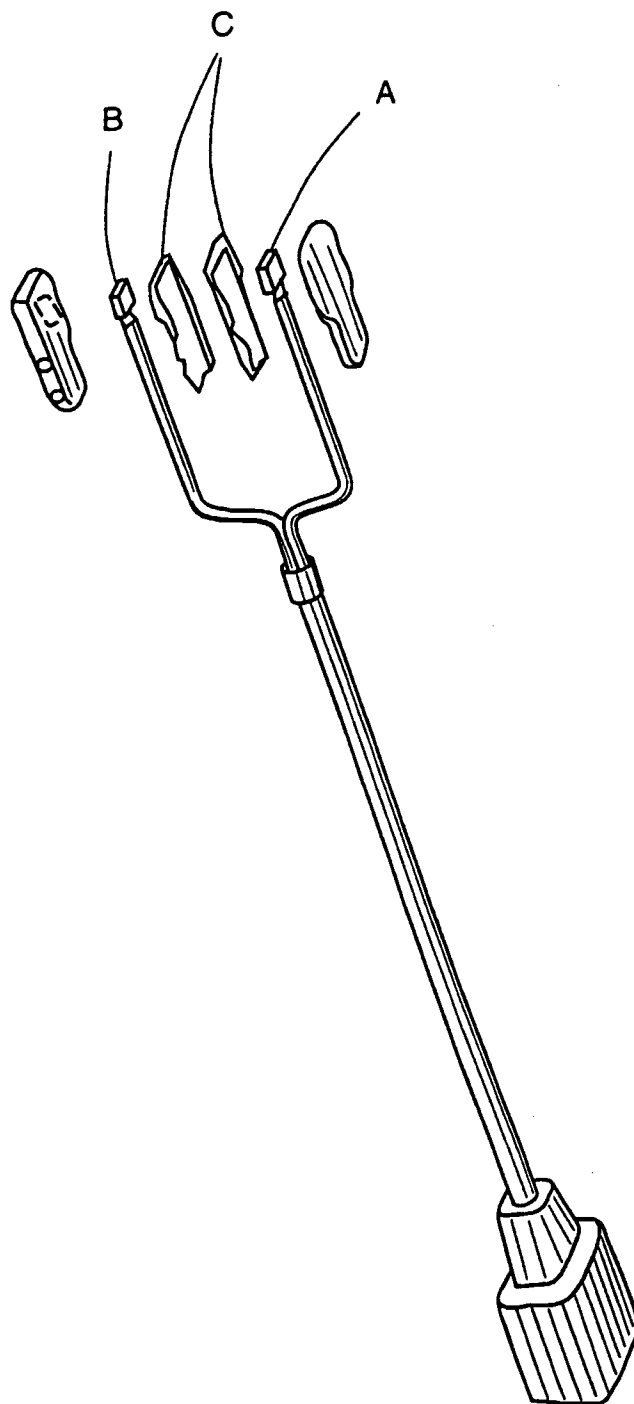


FIGURE 7




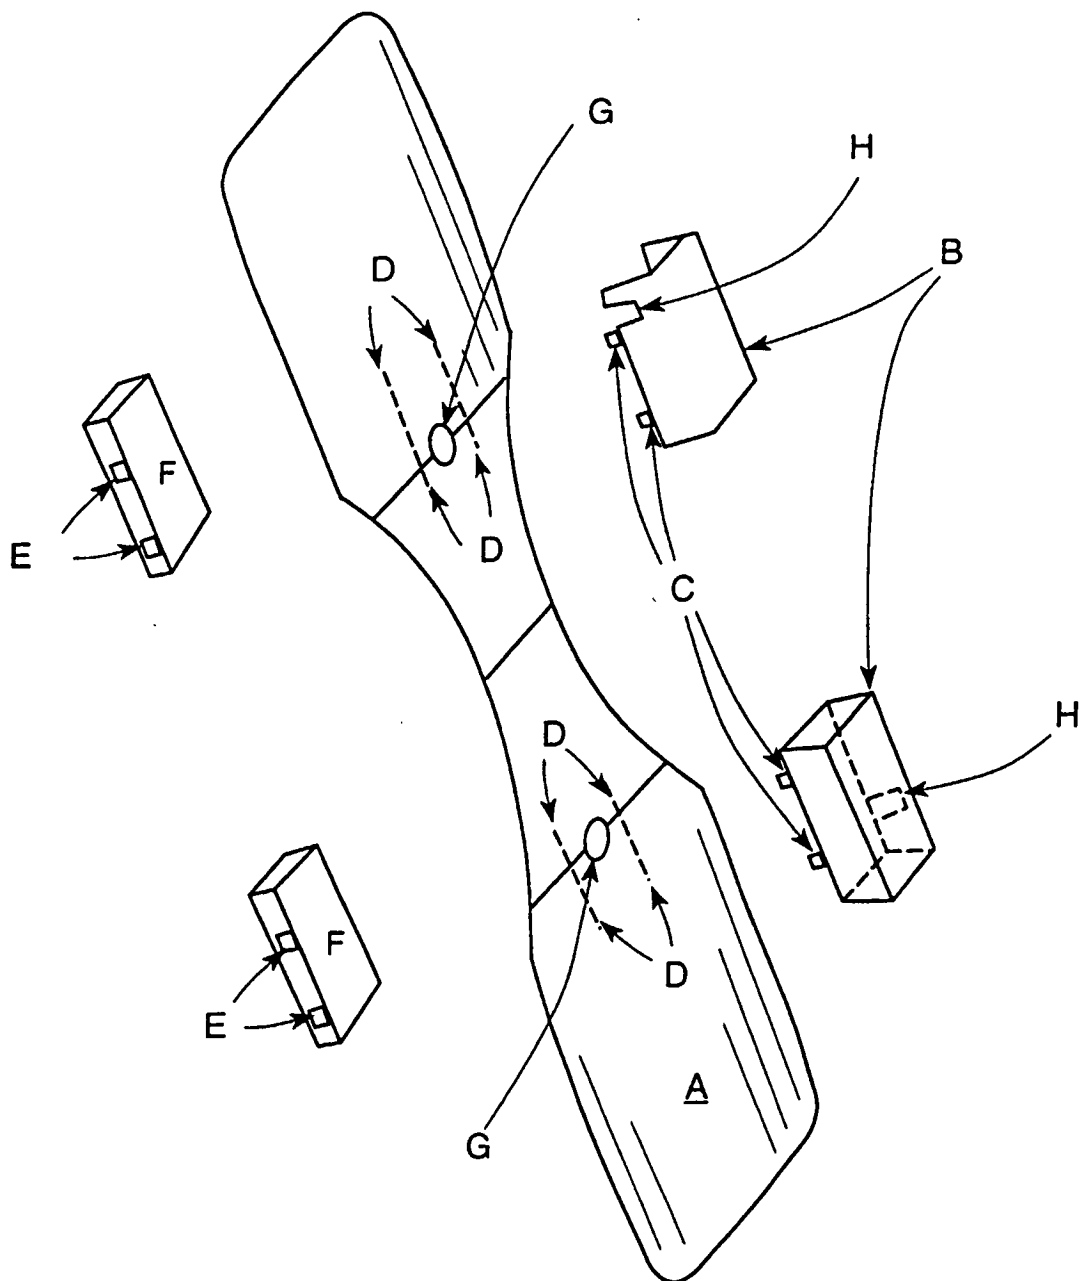


FIGURE 8

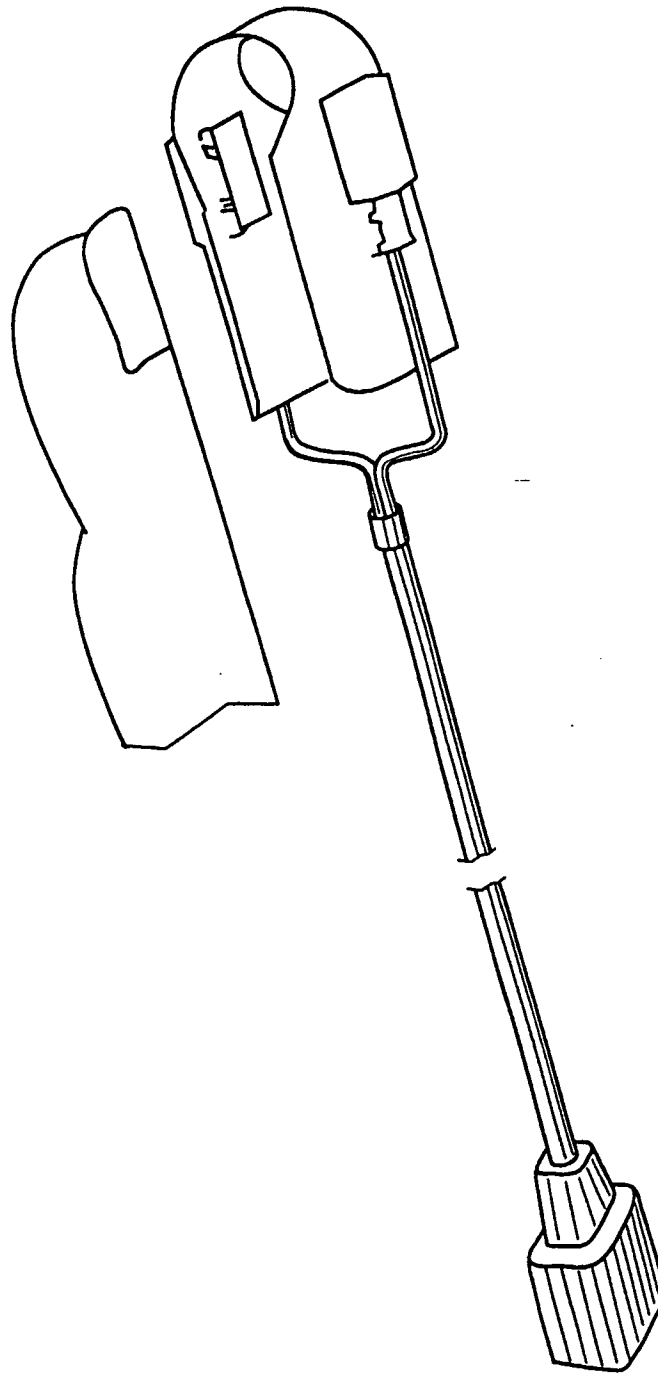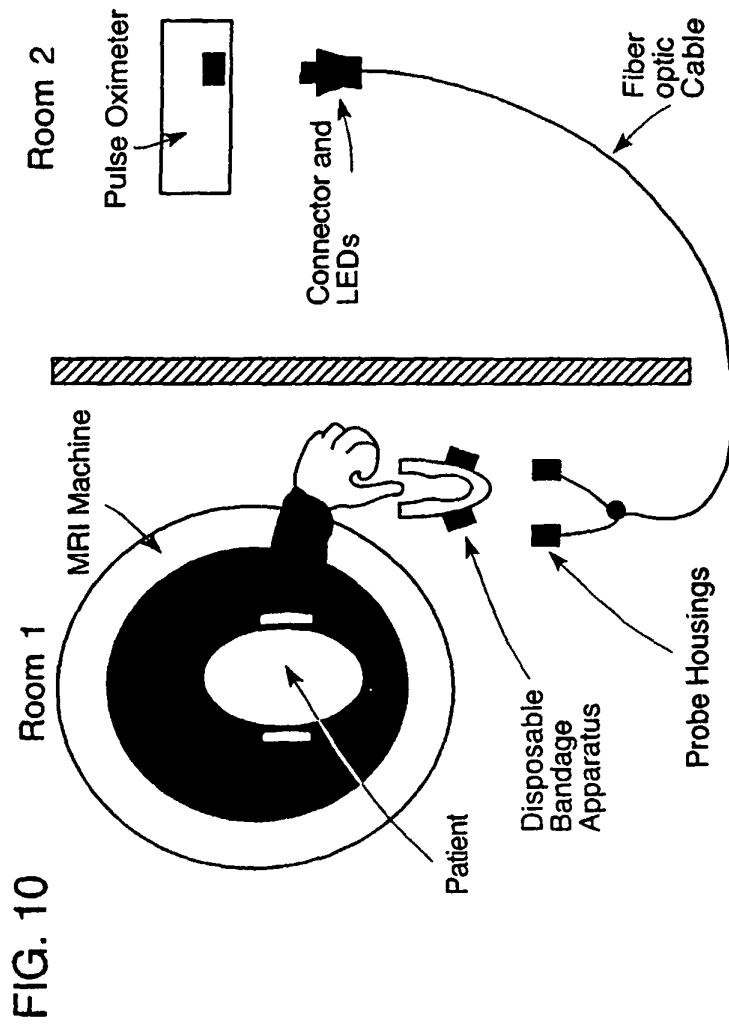

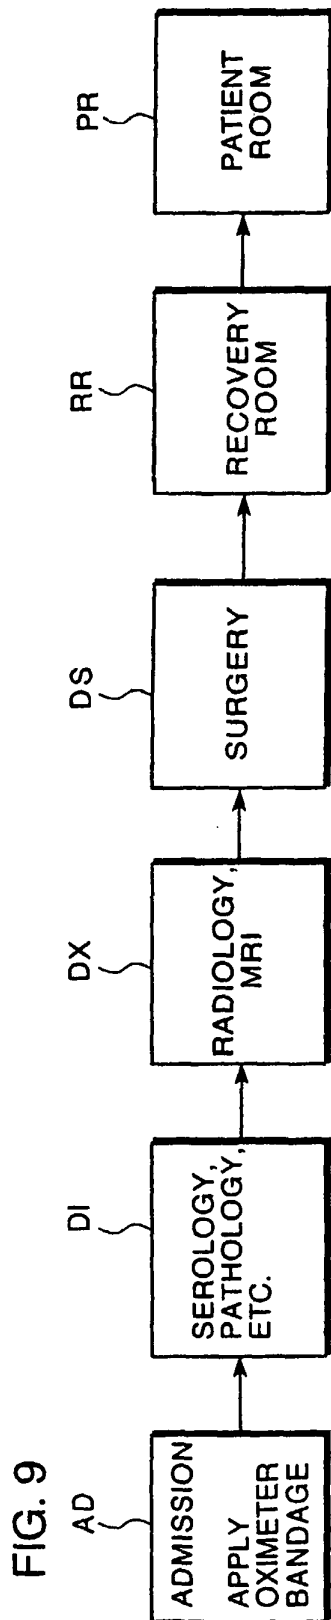

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- WO 0021344 A [0005]



专利名称(译)	可重复使用的脉搏血氧仪探头和一次性绷带		
公开(公告)号	<a href="#">EP1222894B1</a>	公开(公告)日	2011-01-26
申请号	EP2001310925	申请日	2001-12-28
[标]申请(专利权)人(译)	SENSIDYNE		
申请(专利权)人(译)	SENSIDYNE INC.		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	PARKER BRENT		
发明人	PARKER, BRENT		
IPC分类号	A61B5/00 A61B5/055 A61B5/145 A61B5/1455		
CPC分类号	A61B5/6826 A61B5/14552 A61B5/6838		
代理机构(译)	法思博事务所		
优先权	09/758038 2001-01-11 US		
其他公开文献	EP1222894A3 EP1222894A2		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

一种促进需要脉搏血氧计监测的患者或患者的部门内或机构间运输的方法，并且其中用于监测患者的脉搏血氧计可以是不同的制造商，包括将具有绷带的绷带装置固定到患者身上。模块化发射器和检测器插座结合在其上。每个不同制造商的脉搏血氧计探针设置有模块化外壳，其适于配合地接合和/或脱离一次性绷带装置的容器，从而使得患者能够由不同制造商的脉搏血氧计监测而无需改变绷带装置。

