

(19)



(11)

EP 2 750 604 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
04.10.2017 Bulletin 2017/40

(51) Int Cl.:
A61B 5/145^(2006.01) A61B 5/00^(2006.01)

(21) Application number: **12827666.4**

(86) International application number:
PCT/IB2012/054349

(22) Date of filing: **26.08.2012**

(87) International publication number:
WO 2013/030744 (07.03.2013 Gazette 2013/10)

(54) WEARABLE PULSE OXIMETRY DEVICE

TRAGBARE PULSOXIMETRIEVORRICHTUNG

DISPOSITIF D'OXYMÉTRIE PULSÉE PORTABLE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(74) Representative: **Crump, Julian Richard John et al Beresford Crump LLP**
16 High Holborn London WC1V 6BX (GB)

(30) Priority: **30.08.2011 US 201161528851 P**
30.08.2011 GB 201114881

(56) References cited:
EP-A2- 2 178 438 WO-A1-2006/089763
WO-A1-2011/013132 WO-A1-2011/028913
JP-A- 2009 254 523 US-A1- 2006 129 040
US-A1- 2007 142 717 US-A1- 2009 054 751
US-A1- 2009 209 834 US-A1- 2009 306 487

(43) Date of publication of application:
09.07.2014 Bulletin 2014/28

(73) Proprietor: **Oxitone Medical Ltd.**
78172 Ashkelon (IL)

• **AMIR KUGELMAN ET AL: "Reflectance Pulse Oximetry from Core Body in Neonates and Infants: Comparison to Arterial Blood Oxygen Saturation and to Transmission Pulse Oximetry", JOURNAL OF PERINATOLOGY, vol. 24, no. 6, 1 June 2004 (2004-06-01), pages 366-371, XP055174783, ISSN: 0743-8346, DOI: 10.1038/sj.jp.7211102**

(72) Inventors:
• **EISEN, Leon**
77452 Ashdod (IL)
• **FINE, Ilya**
76302 Rechovot (IL)
• **GOLDINOV, Leonid**
76343 Rechovot (IL)

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 750 604 B1

Description

BACKGROUND

1. TECHNICAL FIELD

[0001] The present invention relates to systems and methods for pulse oximetry measurements at the wrist, particularly, the present invention relates to a pulse oximetry device that can be worn on a wrist.

DISCUSSION OF THE RELATED ART

[0002] This section is intended to introduce the reader to various aspects of art that may be related to various aspects of the present invention, which are described and/or claimed below. This discussion is believed to be helpful in providing the reader with background information to facilitate a better understanding of the various aspects of the present invention. Accordingly, it should be understood that these statements are to be read in this light, and not as admissions of prior art.

[0003] In the field of medicine, doctors often desire to monitor certain physiological characteristics of their patients. Accordingly, a wide variety of devices have been developed for monitoring physiological characteristics of a patient. Such devices provide patients, doctors, and other healthcare personnel with the information they need to secure the best possible healthcare for their patients. As a result, such monitoring devices have become an indispensable part of modern medicine.

[0004] One technique for monitoring certain physiological characteristics of a patient is commonly referred to as pulse oximetry, and the devices built based upon pulse oximetry techniques are commonly referred to as pulse oximeters. Pulse oximetry may be used to measure various blood characteristics, such as the arterial blood oxygen saturation of hemoglobin (SPO₂), and/or the rate of blood pulsations corresponding to each heartbeat of a patient. In fact, the "pulse" in pulse oximetry refers to the time varying amount of arterial blood at the measurement site during each cardiac cycle. Those skilled in the art will appreciate the pulse oximetry techniques used for obtaining the above physiological parameters which may also be termed photoplethysmography or, in short, PPG.

[0005] Pulse oximeters typically utilize a non-invasive optical sensor that detects the light response from within a patient's tissue indicative of the amount of light absorbed within the tissue at the illuminated site. One or more of the above physiological characteristics may then be calculated based upon the amount of the absorbed light. More specifically, the light passed through the tissue is typically selected to be of one or more light wavelengths that may be absorbed by the blood in an amount correlative to the amount of the hemoglobin constituent present in the blood. The amount of light absorbed at different light wavelengths may then be used to estimate

the arterial blood hemoglobin related parameters using various algorithms. Pulsatile changes in the volume of the arterial blood at the illuminated site during blood pressure wave propagation alter the intensity of the light response detected by the sensor's photodetector.

[0006] The quality of the pulse oximetry measurement depends in part on the blood perfusion characteristics of the tissue illuminated by the light and in part on the magnitude of the pulsatile changes in the blood volume within the illuminated tissue. Pulse oximetry techniques typically utilize a tissue site that is well perfused with blood, such as a patient's finger, toe, or earlobe, on which to place the sensor.

[0007] For example, **Figure 1** illustrates a sensor **10** adapted to be placed on a finger **12** of a user, such as a patient, according to the prior art. The sensor **10** includes a clip formed of two portions **14** and **16** adapted to clip and constrain the sensor **10** to finger **12** while pulse oximetry measurements are taken. Sensors of a type similar to the sensor **10** are typically coupled to cables **18** that couple the sensor **10** to monitoring systems adapted to receive and process the signals from the sensor **10**. Accordingly, such sensor using in continuous monitoring mode typically requires the patient (or user) to be confined to a certain area, in close vicinity of the monitoring system, thereby limiting patient mobility. In addition, pinch pressure applied by clip portions **14** and **16** on the finger **12** of the patient may overtime feel uncomfortable or become overbearing to the patient to the extent the patient may want to remove the sensor **10** and cease otherwise required monitoring. As a result, such sensors are not suitable for the prolonged and continuous pulse oximetry measurements.

[0008] Further, as may occur with any physiological signals measuring device, appearance of artifacts and other anomalies in the measured data can alter and/or degrade the quality of collected data to the extent that data may not be useful for providing reliable indication of occurring physiological processes. In that regard, pulse oximetry devices are no exception, as such devices may generally be prone to artifacts arising, for example, from patient motion, which may be random, voluntary or involuntary. Consequently, artifacts arising out of such circumstances can distort and skew obtained data, ultimately adversely affecting the quality of the pulse oximetry measurements. Although the accuracy and reliability of the physiological signals measurements is in large affected by the amount of blood perfusion, as well as by the distribution of the nonpulsatile blood within a tissue site, an increased or excessive amount of motion artifact can become a significant contributing factor to the overall pulse oximetry measurement. Due to aforementioned facts, reflection geometry of the pulse oximetry measurements may not be applicable to various portions of user's body, such as those characterized as having weak blood perfusion, as well being prone to strong motion artifacts. In addition, such body portions may not be suitable for accommodating pulse oximetry devices employ-

ing forward transmission geometry in which light emitters and detector are disposed at opposite sides. In such a configuration, portions of the body from pulse oximetry measurements are desired may have tissue layers that are too thick for the light penetrate, thereby impeding the pulse oximetry measurements.

[0009] U.S. published patent applications 2010/056934, 2009/247885, 2010/331709, 2002/188210 and U.S. patent no. 6210340 illustrate prior art pulse and/or oximetry devices that are worn on the wrist. Japanese patent documents nos. 2009160274, 20052705443, 2009254522, 2010220939 and 2005040261, WO. 2010/111127, Korean patent document no. 20110006990 and British patent document no. 2341233 describe devices in which either reflection (at 0°) or transmission (at 180°) modes of light detection are used. WO 2011/013132 teaches a system and method for measuring one or more light-absorption related blood analyte concentration parameters, using a photoplethysmography (PPG) device configured to effect a PPG measurement by illuminating the patient with at least two distinct wavelengths of light and determining relative absorbance at each of the wavelengths to assess value(s) of one or more light-absorption related blood analyte concentration parameter(s). WO 2006-089763-A refers to a pulse oximetry device in which emitters and a sensor are positioned on opposite sides of a patient's forearm to allow light to pass from the emitters to the sensor through the free space between the radius and ulna bones.

BRIEF SUMMARY

[0010] The present invention provides a pulse oximetry device as defined in claim 1. A second aspect of the invention provides a method as defined in claim 10 of measuring and oxygen level using the device.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] For a better understanding of embodiments of the invention and to show how the same may be carried into effect, reference will now be made, purely by way of example, to the accompanying drawings in which like numerals designate corresponding elements or sections throughout.

[0012] In the accompanying drawings:

Figure 1 is an illustration of a pulse oximeter,

Figure 2 is a perspective view of a general wrist-type pulse oximeter, in accordance with exemplary embodiment of the present technique,

Figure 3 is a general view of a pulse oximeter worn on a user, in accordance with an exemplary embodiment of the present technique,

Figure 4 is a side view of a pulse oximeter, in ac-

cordance with an exemplary embodiment of the present technique,

Figure 5 is a perspective view of a pulse oximeter, in accordance with the present technique,

Figure 6 is a side view of a structure used with a pulse oximeter, in accordance with an exemplary embodiment of the present technique,

Figures 7A and 7B are side views of other pulse oximeters, in accordance with an exemplary embodiment of the present technique,

Figure 8 illustrates a set of graphs depicting pulse oximetry data,

Figure 9 illustrates a set of graphs depicting pulse oximetry data, in accordance with an embodiment of the present technique,

Figure 10 is a flow chart illustrating a process of acquiring pulse oximetry data, in accordance with an embodiment of the present technique,

Figure 11 is a graph depicting pulse oximetry data, in accordance with an embodiment of the present technique,

Figure 12 is a correlation chart, in accordance with an embodiment of the present technique,

Figure 13 is a histogram, in accordance with an embodiment of the present technique,

Figure 14 is another histogram, in accordance with an embodiment of the present technique,

Figures 15A-C schematically illustrate the difference between prior art reflection (Figure 15A) and transmission (Figure 15B) modes and the present invention's trans-illumination (Figure 15C) mode of measurement, according to some embodiments of the invention,

Figures 16A-E schematically illustrate measurement configurations of the pulse oximetry device, according to some embodiments of the invention,

Figures 17A and 17B schematically illustrate a perspective view of the wrist worn pulse oximetry device in an unworn position, according to some embodiments of the invention, and

Figure 18 is a schematic flowchart illustrating a method of oximetry measurement, according to some embodiments of the invention.

DETAILED DESCRIPTION

[0013] With specific reference now to the drawings in detail, it is stressed that the particulars shown are by way of example and for purposes of illustrative discussion of the preferred embodiments of the present invention only, and are presented in the cause of providing what is believed to be the most useful and readily understood description of the principles and conceptual aspects of the invention. In this regard, no attempt is made to show structural details of the invention in more detail than is necessary for a fundamental understanding of the invention, the description taken with the drawings making apparent to those skilled in the art how the several forms of the invention may be embodied in practice.

[0014] Before explaining at least one embodiment of the invention in detail, it is to be understood that the invention is not limited in its application to the details of construction and the arrangement of the components set forth in the following description or illustrated in the drawings. The invention is applicable to other embodiments or of being practiced or carried out in various ways. Also, it is to be understood that the phraseology and terminology employed herein is for the purpose of description and should not be regarded as limiting.

[0015] The term "trans-illumination" as used herein in this application, is defined as a mode of optical measurement, in which the measured light is reflected off a surface at an angle larger than 0° (which correspond to simple reflection) and smaller than 180° (which correspond to simple transmission). Commonly, but not exclusively, the reflection angles in trans-illumination mode are between approximately 20° and approximately 160° . In trans-illumination mode, the measured light is emitted from the light source, hits the reflective surface, which may be curved, at an angle, and is reflected at an angle to the detector. In practice, trans-illumination includes light going over various light paths, having in common an origin in the light source and a measurement in the detector.

[0016] Embodiments of the invention include a pulse oximetry device that is mounted on a wrist strap and fixates an area above a distal end of the ulna with a dome shaped structure. This area is used as measuring area. The measurement is carried out by a detector positioned above the fixated area, that detects light emitted by light sources having different wave lengths that are located at a periphery of the fixated area. Hence, the reflections are measured at neither a reflection mode nor a transmission mode, but are at an angle between 20° and 160° from the emitted light. This mode, termed trans-illumination, allows achieving an excellent signal to noise ratio that for the first time enables continuous and reliable measurement of oximetry data on the wrist.

[0017] In embodiments, the present invention comprises a pulse oximetry device comprising (i) a dome shaped structure arranged to fixate an area above a distal end of the ulna to remove venous blood from the fixated area,

and (ii) at least two light sources having different wave lengths and at least one detector responsive to the different wave lengths, wherein the at least one detector is arranged to measure light emitted by the at least two light sources that is trans-illuminated from the distal end of the ulna and through the fixated area.

[0018] The present invention is a substantial advance in respect to the prior art listed above due to the following features. In respect to WIPO patent document no. 2011/013132 by the present inventor, at least the following features are novel and non-obvious: Photoplethysmography (PPG) measurement using the distal end of the ulna bone as a convex reflector to measure at a trans-illumination mode (with an angle between 20° and 160° between the detected and the emitted light), use of the area above the distal end of the ulna bone as the measurement area, fixating the device on the distal end of the ulna bone by a dome like structure. In respect to the other listed prior art, additional advances are the integration of pulse and oximetry measuring devices and the integration of their features.

[0019] Turning now to the figures, **Figure 2** is a perspective view of a general wrist-type pulse oximeter **30**, in accordance with exemplary embodiment of the present technique. Accordingly, the oximeter **30** is a wrist-type oximeter device adapted to be worn on a wrist **31** of a user, as further shown by **Figure 3**. The oximeter **30** is adapted to obtain pulse oximetry data including pulse data, as well as, oxygen saturation (SPO2) data from a user while the user wears the oximeter **30** on the wrist **31**. Hence, a user can wear the oximeter **30** in manner similar to that of wearing a watch, a wrist band or any article of clothing, ornament, or garment adapted to be worn on the wrist **31** of the user. In this manner, a user can wear the oximeter **30** while performing any routine and ordinary operation the user would otherwise perform in everyday life, such as walking, running, cycling and so forth. In accordance with embodiments of the present technique, the oximeter **30** can be conveniently worn at any time or place by those users required or wishing to obtain pulse oximetry and pulse rate data without being attached to elaborate monitoring device or being confined to certain monitoring areas. Thus, the pulse oximeter **30** is a self contained, self powered device adapted to obtain, analyze and process various light electromagnetic signals from which pulse oximetry data is ultimately obtained. The oximeter **30** may further include wired or wireless interfaces whereby the oximeter **30** can communicate and/or relay data signals to external and/or remote devices. Hence, the oximeter **30** can collect and provide the oximetry data to any remote users, institutions, i.e. hospitals or clinics, or anyone who requires or has interest in such pulse oximetry data of the user.

[0020] As further illustrated by **Figures 2** and **3**, oximeter **30** is made up of a wrist band **32**, coupled to casing **34**. The wrist band **32** may be made up of any flexible and/or stretchable material, such as rubber, silicon, soft plastic, cloth or polished metal or any combination thereof

for providing the user a comfortable fit and feeling while wearing the oximeter **30**. The casing **34** may be made up of any strong and durable material, i.e. metal, hard plastic, adapted for housing and protecting all functioning components of the oximeter **30** from external elements and forces. Although not shown, components housed by the casing **34** may include various electrical, mechanical, optical and other devices, such as batteries, processors, integrated circuit boards, light emitting diodes, shunts, and/or other devices contributing to the overall functionality and integrity of the oximeter **30**.

[0021] As further illustrated, on top of casing **34** there is disposed a display **36** adapted to provide the user a visual indication of pulse oximetry and other data. Those skilled in the art will appreciate that the display **36** may be made of any general display, such as a liquid display (LCD) or similar types of display devices. Adjacent to the display **36** there are further disposed buttons/knobs **37** providing a user with additional functionalities and features through which the user can access, set and/or view parameters provided by the oximeter **30**. In an exemplary embodiment, the buttons **37** may form numerical button or alphanumeric buttons where by the user can enter any combination of numbers and/or letters as desired or needed while the oximeter is in use. In some embodiments, buttons **37** could, alternatively be placed at any side of casing **34**, or any other area along the casing easily accessible to the user.

[0022] **Figure 4** is a cross section view of a pulse oximeter, in accordance with an exemplary embodiment of the present technique. The illustrated pulse oximeter is similar to the oximeter **30**, generally incorporating the above discussed features. Accordingly, **Figure 5** is a perspective view of the pulse oximeter **30**, in accordance with the present technique. Both of the **Figures 4** and **5** provide general views of the systems and structures making up the oximeter **30**, as will be discussed further below.

[0023] More specifically, the illustrated oximeter **30**, as shown in **Figure 4**, is disposed around the wrist **31** of the user. Accordingly, in a preferred embodiment, the oximeter **30** includes a structure **40** disposed on an inner side of the oximeter **30**, whereby the structure **40** is adapted to fit on top of an ulna bone **38** of the wrist **31**. In so doing, the structure **40** includes a dome-like structure adapted to comfortably snug on top of and/or against the ulna bone **38** so that the oximeter **30** is securely fixed around the wrist **31**. As further shown in **Figure 5**, the structure **40** includes an interior portion/surface **42** adapted to receive the bone **38** when the user wears the oximeter **30** around wrist **31**. Hence, the shape of structure **40** conforms to the general shape of the ulna bone **38** so that the oximeter **30** straps onto wrist **31** in a complementary fashion for achieving a good contact between the oximeter **30** and the wrist **31**. Apart from being comfortable, such good contact between the wrist of the user and the oximeter promotes a better interface between functional probing elements of the oximeter **30** and user skin tissue, thereby achieving an appropriate data col-

lection interface between the user and the oximeter **30**. In certain embodiments of the present technique sensor components may be embedded within padding or other protective material, such as rubber, for protecting the sensor components from any outside vibrations, shocks and/or other forces that the user can experience while wearing the sensor. Such material could dampen any outside forces, further facilitating better data collection while reduce motion artifacts that could appear within pulse oximetry measurements.

[0024] Those skilled in the art will appreciate that the dome-like structure **40** can be made up of flexible materials, such as silicon and/or other types of combinations of plastics, or soft metals, enabling the structure **40** to easily deform and conform to the shape of the bone, i.e. ulna bone **38**, to which the oximeter **30** couples. Accordingly, the present technique contemplates a structure, such as the structure **40** that is adjustable and conformable for fitting users having ulna bones of various sizes and shapes. As discussed further below, apart from providing an accommodating structure for the bone **38** while the oximeter **30** is worn over the wrist **31**, the structure **40** also serves as an intermediary structure disposed between the user and various electro-optical elements, also part of oximeter **30**, adapted for emitting and detecting electro-magnetic waves used for obtaining pulse oximetry measurements. Another function of the structure **40** is to shield detector from ambient light incidence.

[0025] Accordingly, the pulse oximeter **30** further includes an optical device, including multiple light emitting diodes (LEDs) **50** disposed in proximity of structure **40**, light detector **52** disposed at a portion of the structure **40**. As illustrated in **Figure 5**, the inner portion/surface **42** includes opening **44** from which light emitted by the LEDs **50** can be emitted to propagate within the wrist **31**. Similarly, portion **42** also includes opening/aperture **46**, through which light can be received at detectors **52**.

[0026] As illustrated in the embodiment shown in **Figure 4**, the LEDs **50** and the detectors **52** are disposed relative to one another such that light provided by the LEDs **50** is transmitted through the wrist tissue and collected by the light detectors **52**. Accordingly, the ulna bone **38** of wrist **31** is disposed in between the LEDs **50** and the detector **52**, whereby the LEDs **50** is disposed such that the light emitted therefrom scatters off the ulna bone **38** before reaching the detector **52**. While the illustrated embodiment may generally depict a certain emitter/detector configuration disposed around wrist **31**, particularly, around the bone **38**, those skilled in the art will appreciate that such a configuration is exemplary and that the present technique contemplates other configurations and placements of the LEDs **50** and the detectors **52** around and/or in vicinity of bone **38** for achieving good and reliable pulse oximetry data. In such a trans-illumination sensor configuration only diffused multiple scattering component of the light transmitted to the detector is measured while specular component and transmitted forward component of the light is not detected.

[0027] Further, in a preferred embodiment, the LEDs **50** may be made up of an LEDs adapted to emit light in the visible red spectrum having a wavelength, for example, of 660 nanometers (nm) but not limited to, and another LED adapted to emit light in the infrared spectrum, having, a wavelength, for example, of 940 nm, but not limited to, where the light emitted by both LEDs are detectable by the photodetector **52**. Light diffused through the tissues to the photo detector **52** is absorbed by blood and soft tissues, depending on the concentration of hemoglobin in blood. Hence, the amount of light absorption at each light wavelength depends upon the degree of oxygenation of hemoglobin within the blood. As further described herein light emitted by the LEDs **50** scatters at multiple sites of the bone **38**, for ultimately reaching the detector **52**. Advantageously, the scattering of the light by the ulna bone **38** increases absorption of light by blood present in tissue and other structures carrying blood throughout various anatomical regions through which the light may propagate. An increased optical path length, as provided by the configuration of the oximeter **30**, brings about an increase of interaction between the propagating light and surrounding tissue for ultimately providing a robust signal from which pulse oximetry data can be obtained.

[0028] More specifically, the present technique, as implemented by the oximeter **30**, for detection of oxygen saturation of hemoglobin by spectrophotometry is based on Beer-Lambert law, which relates the concentration of a solute to the intensity of light transmitted through a solution. Combined with the pulsatile blood measurement technique such techniques may also be termed photoplethysmography (PPG). In order to estimate the concentration of a light absorbing substance in a clear solution from the intensity of light transmitted through the solution, it is required to know the intensity and wavelength of incident light, the transmission path length, and absorbance of the substance at a specific wavelength, i.e. the extinction coefficient of the medium through the which the light propagates.

[0029] Generally pulsatile expansion of a vascular bed produces an increase in propagation light path length thereby increasing light absorbance. Hence, a detected light response is typically made up of a time dependent AC signal, and a nonpulsatile background DC signal. Accordingly, specific signal processing algorithms can be used to first determine the AC component of absorbance at each wavelength and divide such component by a corresponding DC component at each wavelength. By using two different, Red and IR wavelengths of light, as would be produced by two different LEDs **50**, proportions of light absorbed by each component at the two frequencies can be used to provide a ratio (R) of a "pulse-added" absorbance, often referred to as γ (gamma) parameter in the literature, mathematically defined as:

$$R = \frac{AC_{660}/DC_{660}}{AC_{940}/DC_{940}} \quad (\text{Equation 1})$$

[0030] The pulse oximetry measurements obtained where difference in measured light absorption is accruing at different point in time corresponding to different vascular blood volume are said to be 'volumetric measurements,' indicative of the differential volumes of blood present at a measurement sites within the patient's vascular bed at different times.

[0031] In accordance with further embodiments of the present technique, the above described data collection, data analysis, and data processing is performed locally, that is, by processing components disposed within the oximeter **30**. Thus, **Figure 4** further illustrates inner components **56** disposed within casing **34** of oximeter **30**. The components **56** may include various electronic components adapted to electrically support the various operations performed by the oximeter **30**. Such components may include microprocessors, batteries, integrated circuits, memory devices, wireline and/or wireless communication devices and so forth. The components **56** may further operate according and/or execute and/or store various software platforms and algorithms adapted to support various signal processing activities implemented by the oximeter **30**. For example, such signal processing may include utilizing Fast Fourier Transforms (FFTs) algorithms, as well as various pattern recognition routines for analyzing collected physiological data. The components **56** may further be coupled to input/output (I/O) devices adapted to couple the oximeter **30** to external devices, enabling the device **30** to download or upload various data, such user data, physiological parameters and other data that could be useful to the user or any healthcare professional monitoring, for example, physiological or other parameters of the patient.

[0032] Turning now to **Figure 6**, there is further shown structure **40** adapted to receive the ulna bone **38** of wrist **31**. As illustrated, the structure **40** may generally have a dome-like shape, or a cone-like shape, adapted to be placed over and receive the ulna bone **38**. Accordingly, the structure **40** is made up of an inner surface (e.g., portion **42** of **Figure 5**) whose geometrical dimensions and attributes conform to an exterior surface of the ulna bone **38** and its surrounding tissue disposed on wrist **31** of the user. In this manner, the structure **40** is adapted to receive the ulna bone **38** and surrounding tissue so that the bone and tissue complement the portion **42**. In the illustrated embodiment, the structure **40** is generally shaped to be circular such that it receives the bone **38** in a manner similar to that of a cap placed over a rounded structure, i.e. bone **38**, having a somewhat corresponding circular outer surface.

[0033] **Figure 7A** is a side view of another pulse oximeter **70**, in accordance with an exemplary embodiment of the present technique. Accordingly, the pulse oximeter **70** is a wearable pulse oximeter similar to the wearable

oximeter **30** described above with reference to **Figures 1-6**. As illustrated, the oximeter **70** includes components similar to those included within the oximeter **30**, whereby the oximeter **70** is also adapted to perform pulse oximetry operations similar to those performed by the oximeter **30**. **[0034]** Further, in the illustrated embodiment of **Figure 7A**, the oximeter **70** includes a coherent light scattering (CLS) apparatus **72** adapted to detect pulse rate that could supplement and/or otherwise enhance the overall pulse oximetry measurements obtained by the oximeter **70**. Accordingly, the CLS device **70** may be particularly adapted to detect artifacts within the pulse oximetry data, such as those arising from user motion and the like. Hence, the CLS device **70** may include a coherent light source, such as a diode laser, adapted for emitting coherent light, as well as at least one photodetector devices adapted to detect the coherent light scattering response. Thus, the device **70** is adapted to continuously measure coherent light scattering responses from within tissue of hand wrist **31** for generating data indicative Doppler signals and/or dynamic speckle signals. Accordingly, methods for detecting and obtaining pulse oximetry measurements in a presence of motion artifact using dynamic light scattering (DLS) methods are described in U.S. Publication Number 2011/0082355, teaching a photoplethysmography device and method.

[0035] **Figure 7B** is a schematic illustration of an embodiment in which CLS apparatus **72** is located near light sources **50** and is arranged to measure the pulse in that area. In embodiments, some of the light scattered from CLS apparatus **72** may be used as one of light sources **50** to measure oximetry data. Although the coherency of the light from CLS apparatus **72** is lost in the scattered light, coherency is important only for pulse measurements and not for oximetry measurements. Hence, the scattered light may be used for oximetry measurements if the light source is selected to the appropriate frequencies.

[0036] As part of the aforementioned disclosure covering the theory of DLS as it pertains to physiological settings discussed herein, it has been further observed that under good blood perfusion conditions in which motion artifacts are not significant, then there appears to be a general correlation between DLS signal taken over time and the time derivative of corresponding plethysmography (PPG) signals.

[0037] **Figure 8** illustrates a set of graphs **100** depicting pulse oximetry data, in accordance with an exemplary embodiment of the present technique. The set of plots **100** are indicative of PPG and CLS measurements taken in the presence of motion artifacts. Accordingly, the depicted set of graphs includes a graph **102**, graph **104** and graph **106**. The graphs **102-106** are all plotted on similar axes where a vertical axis **108** indicates signal amplitude and a horizontal axis **110** indicates time. The plot **102** is a PPG measurement obtained using a red LED (e.g., LEDs **50**), for example, that emitting light of wavelength 660 nm, while the plot **104** is indicative of PPG measure-

ments obtained by the IR LED, i.e. one emitting 940 nm. The plot **106** are those pulse rate and pulse waveform measurements obtained using the CLS sensor **72**, more particularly, using coherent light scattering (CLS) techniques. As illustrated, in the presence of motion artifacts each of the plots **102-106** includes a transition point in time where the obtained pulse is distorted by the occurrence and initiation of motion artifacts. For example, in plot **102** such an occurrence of motion artifacts is indicated by point **112**, where in plot **104**, the occurrence is give by point **114**. By further example, occurrence of motion artifacts is indicated by point **116**, again, indicating the on set of motion artifacts. It should be borne in mind that such motion artifacts may be a result of motion imparted by the user wearing the oximeter **30/70**, such as when the user may voluntarily or involuntarily move the wrist **31** to which the oximeter is coupled.

[0038] **Figure 9** illustrates a set of graphs **150** depicting pulse oximetry data, in accordance with an embodiment of the present technique. The set of graphs **150** includes plots of PPG and CLS data similar to that shown in the previously discussed **Figure 8**, however, the plots **150** are indicative of PPG and CLS measurements taken in the absence of motion artifacts. Accordingly, plots **150** include a plot **152** in which PPG measurements are taken with the 660 nm wavelength LED. The plots **150** further includes plot **154** indicative of PPG measurements taken with the 940 nm wavelength LED, and plot **156** indicative of pulse rate and pulse waveform data taken with a CLS sensor, as described above.

[0039] As illustrated by the plots **150**, in the absence of motion artifacts, PPG signals appear to be different in character and form those appearing in plots **100**. Indeed, in the absence of motion artifacts, pulse oximetry measurements appear to be more ascertainable and determinative than when such motion artifacts exist. Those skilled in the art will appreciate that CLS devices and techniques used along with standard PPG methods can yield filtered pulse oximetry data. Hence, to the extent such filtration is used, the above disclosed wearable pulse oximeter **70** can be adapted to provide a user with reliable pulse oximetry data, providing heart beat pulse, as well as, oxygen saturation (SPO2) measurements.

[0040] **Figure 10** is a flow chart **200** illustrating a process of acquiring pulse oximetry data, in accordance with an embodiment of the present technique. The flow chart **200** describes a process whereby a pulse oximeter, such as the pulse oximeter **30** and/or **70**, obtains pulse oximetry data, using PPG and CLS correlation methods, in the presence of motion artifacts. Further, the process **200** is adapted to correlate the obtained CLS and PPG data so as to minimize or otherwise reject data indicative of the motion artifacts, thereby producing reliable pulse oximetry measurements, indicative of the SPO2 levels of the user.

[0041] Accordingly the process flow **200** begins at step **202**, whereby DLS/CLS devices and methods thereof are used along with PPG and spectrophotometry techniques

for obtaining pulse oximetry data taken from a wrist of a user wearing the wearable pulse oximetry **70** described hereinabove. The collection of the PPG data is obtained using the LEDs **50** and detectors **52**, particularly, PPG data is obtained via the use and detection of two distinct electromagnetic signals emanating from two LEDs adapted to produce signals at two wavelengths, i.e. 660 nm and 940 nm. The aforementioned two measurements are further used with a third light measurement, as used with the above-mentioned DLS/CLS devices **72** disposed within the oximeter **70**. Further, at step **204** the three light measurements including the obtained CLS and PPG data are further processed. Particularly, in box **204**, the process flow **200** utilizes various algorithms and routines for performing, for example, Fast Fourier Transform (FFT) on the CLS time dependent waveform data, thereby obtaining a frequency power spectrum. In addition, at step **204**, the process flow **200** utilizes the CLS and/or PPG data for extracting pulse waveforms from which a pulse rate of the user can be identified. Such processing of the initially obtained data is implemented, for example, using processing components **56** of the oximeter **70**.

[0042] The processed CLS and PPG data in the form of waveforms distorted by the occurrence the motion artifacts are presented in a **Figure 11** within the time frame 10 sec which can be also 4, 6, 8, 12 seconds, etc. Time derivative of the PPG IR data is plotted on one side of vertical axis **300**, and CLS data is plotted on other side of vertical axis **302**. Both CLS and PPG waveforms are plotted versus time axis **304**.

[0043] At decision junction **206** the process flow **200** determines a correlation existing between modified PPG waveform and the obtained CLS waveform over certain moving time frame through which data is continuously collected using the oximeter **70**. The correlation provided by the step **206** enables to set specified criteria for ascertaining the extent of motion artifacts present in the pulse oximetry data.

[0044] Indeed, a correlation of step **206** is found to be below a specified threshold or criteria (for example <0.8), the process flow moves from decision junction **206** to step **208**, where a moving regression algorithm is implemented by the oximeter **70** for rejecting those data signals indicative of artifacts arising out of user motion. The manner by which is such rejection is performed can be illustrated by **Figure 12**, in which resulting PPG-CLS correlation is plotted on vertical axis **350** versus data points collected within corresponding moving time frame. The correlations displayed by **Figure 12** are those correlations found for each moving time frame with the step **20** data points which can be 1, 2, 3, 4, 5 etc. points, from which an optimal magnitude range of correlations (e.g., 03-06) is chosen using adaptive algorithm for quantifying the amount of motion artifacts and for using such quantification to filter or otherwise reject such motion artifacts that screens the correct pulse oximetry data. Hence, this reduces or otherwise eliminates certain motion related characteristics that may cause erroneous SPO2. Hence,

at step **210** such data is provided for further processing, particularly, the filtered data is used to calculate actual SPO2 levels using a moving histogram method.

[0045] In so doing, **Figures 13** and **14** provide graphs of measured pulse oximetry measurements, particularly measurements of γ , without and with filtered data of motion artifacts. Accordingly, as plotted on a vertical axes **400** of **Figure 13**, there is displayed a number of counts, plotted versus γ on a horizontal axis. **Figure 13** can be compared with **Figure 14** plotting parameters similar to those shown in **Figure 13**. More specifically, **Figure 14** illustrates filtered gamma measurements obtained by using the above described CLS-PPG correlations for rejecting those signals arising out of motion artifacts. As further seen by **Figure 14**, a first peak **404**, indicative of a true gamma, is clearly discernible when compared with motion artifact-riddled data of **Figure 13**.

[0046] Returning once more to process flow **200**, if at decision junction **206** the correlation between modified PPG and CLS data is greater than the specified threshold or criteria, the process flow proceeds to step **210** where SPO2 is calculated using a conventional methods.

[0047] It should be borne in mind that the above steps of process flow **200** may be implemented and executed using various schemes including software and algorithm storable and executable by the pulse oximeters described above.

[0048] Exemplary embodiments of the present technique disclose a pulse oximeter in the form of a wrist band, watch, or strap adapted to be worn on a wrist of a user. The disclosed pulse oximeter includes at least two light emitters and at least one light detector disposed on the strap-type oximeter, whereby the emitters and detectors are part of a structure adapted to receive an ulna bone located on the wrist of the user. In one embodiment, the emitters and detectors are disposed relative to one another in such a configuration, where wrist ulna bone become disposed in between the light emitters and the light detectors when the strap-type oximeter is worn on the wrist of the user. In this manner, the emitted light propagates through the tissue in transmission mode, and repeatedly scatters off the bone until the light reaches the detector where the light is detected for providing pulse oximetry measurements. Hence, having desired light absorption and reflection characteristics, the wrist ulna bone provides a suitable medium for diffusing, reflecting and directing the light from the emitter to the detector inasmuch as the size and shape of the ulna bone provides a prolonged optical path length between the light emitters and detectors. In this sense, the bone disposed between the emitter and detector serves as a specific diffuser and reflector, whereby the structural, chemical and physical makeup of the bone and its surrounding tissue increases light scattering within the tissue and bone thereby, consequently, providing increased probability of light absorption. Due to the fact that such a configuration facilitates light transmission through the wrist tissue between light emitters and detector trans-illumination light signal

measurement geometry is achieved. Under this geometry, specular component of the light is not detected and it is only the diffused multiple scattering transmission component of the light signal that gets measured. Advantageously, the present technique provides a device in which optical path length, as existing between the emitter and detector, is increased. Consequently, this increases the amount of scattering experienced by the light, which further facilitates a robust detected light signal from which reliable pulse oximetry data can be obtained.

[0049] In other embodiments of the present technique, the wrist-band type oximeter utilizes a system for detecting and/or mitigating signal artifacts arising out user motion, for example, hand motion, thereby achieving a reliable pulse oximetry measurement. Specifically, the disclosed wrist band oximeter includes a coherent light scattering (CLS) sensor for the pulse rate measurements. Generally, CLS includes any scattering of light caused induced, or otherwise generated by coherent light. This could involve dynamic light scattering, caused by a multiple scattering by multitude of moving objects, resulting in dynamic speckle, or Doppler scattering. CLS could also involve elastic or inelastic scattering, such as Raman scattering. It should be borne in mind that while the term CLS defined herein includes the aforementioned light scattering phenomena, the present technique may utilize any form of dynamic light scattering (DLS), or any other scattering processes for achieving pulse rate measurements. In certain embodiments of the present technique utilizes a CLS device including a sensor having a coherent light source, such as a vertical-cavity surface-emitting laser (VCSEL), or other diode lasers used for illuminating those regions of tissue and bone in close proximity from the pulse oximetry measurement site. The device also has a detector used for coherent light scattering response measurements. The light response to multiple scattering of the coherent light at the flowing and pulsatile blood generates an instantaneous light intensity pattern at the surface of detector which, being processed, allows pulse rate calculation. Such information may be combined with the pulse oximetry data for identification, removal and filtration of artifacts that may arise out of user motion, thereby producing true and reliable pulse and SPO2 data of the user.

[0050] Other aspects of the invention may include a system arranged to execute the aforementioned method. These, additional, and/or other aspects and/or advantages of the embodiments of the present invention are set forth in the detailed description which follows; possibly inferable from the detailed description; and/or learnable by practice of the embodiments of the present invention.

[0051] **Figures 15A-C** schematically illustrate the difference between prior art reflection (**Figure 15A**) and transmission (**Figure 15B**) modes and the present invention's trans-illumination (**Figure 15C**) mode of measurement, according to some embodiments of the invention. In contrast to prior art measurement, done in either re-

flexion mode (approximately $\alpha=0^\circ$ between light emitted from source **50** and light detected by detector **52**, i.e. detector **52** is adjacent to source **50**) or transmission mode (approximately $\alpha=180^\circ$ between light emitted from source **50** and light detected by detector **52**, i.e. detector **52** faces source **50**), the present invention teaches measurement in trans-illumination mode that incorporates various and multiple light paths between source **50** and detector **52**, most of which include reflections at angles different than back-reflection such as $20^\circ < \alpha < 160^\circ$, e.g. from the convex surface of the distal end of the ulna bone in case of a wrist oximeter. An additional advantage of the distal end of the ulna bone is the ease to find it by different users, with different wrist characteristics. For example, parts of the distal end of the radius bone could have also been used from an optical point of view, but they would be more difficult to detect and correctly place device **30** on by the user.

[0052] The exact angle α changes from user to user and may even change from use to use, depending on the wrist anatomy and the way device **30** is worn on the wrist. The use of trans-illumination over the head of the ulna bone overcomes handles this variance by allowing for a wide range of tolerance regarding the exact angle α . Device **30** determines the position of detector **52** on dome **40** which is fixated on the head of the ulna bone and a distance d (**Figures 16A** and **17A**, and see below) determines the spacing of source **50** and dome **40** with detector **52**, with a variance resulting from possible elasticity of strap **32**. The distance d determines thus the range of possible angles α for different users, all of which allow measurement using the trans-illumination principle. Distance d may be between 0.5 cm and 3 cm or between 1 cm and 2.5 cm, depending on the specific design, efficiency of optical measurements and intended users.

[0053] **Figures 16A-E** schematically illustrate measurement configurations of pulse oximetry device **30**, according to some embodiments of the invention. **Figure 16A** illustrates a schematic cross section of the wrist, showing the distal end of the ulna bone and the radius bone. CLS apparatus **72** with a laser light source **71** and detector **73** may be positioned remotely from dome **40**. Light source **71** emits a coherent light **74A** which is reflected and measured as reflection **74B** by CLS detector **73**. PPG is measured at an area **41** above a distal end of the ulna that is fixated by dome shaped structure **40**. At least one detector **52** is positioned above fixated area **41**, while at least two light sources **50A**, **50B** having different wave lengths are located at a periphery of fixated area **41**. Detector **52** is arranged to measure reflections **51B** by the distal end of the ulna of light **51A** emitted from at least two light sources **50A**, **50B**. Reflections **51B** are at an angle between 20° and 160° from emitted light **51A**. In embodiments, detector **52** and two light sources **50A**, **50B** may be positioned to detect reflections **51B** at an angle between 70° and 110° from emitted light **50A**. **Figures 16A-B** illustrate two embodiments in which the CLS apparatus **72** is located near PPG light sources **50A**, **50B**.

In **Figure 16B**, laser light source **71** of CLS apparatus **72** is used for two purposes - the first as a coherent light source for CLS apparatus **72** - emitting light **74A** for detector **73** to measure reflection **74B** and CLS apparatus **72** to calculate the pulse therefrom, and the second as a source of non-coherent light (coherency lost due to movement through the tissue and combination of different optical paths) functioning as one of the two PPG light sources (in **Figure 16B** replacing light source **50B**). **Figure 16C** illustrates an embodiment in which CLS apparatus **72** is located near PPG light sources **50A**, **50B**, but is not used as one of the light sources, e.g. due to frequency limitations. In another embodiment, both light sources **50A** and **50B** may be laser diodes and detector **52** is arranged to detect light emitted thereof to determine PPG data. Using the trans-illumination mode of measurement, the light loses its coherence by going through the tissue and reflecting from the head of the ulna bone, and is used only in respect to the dependency of intensity on wavelength, which indicates oxygen saturation of the blood. In embodiments, light sources **50A** and **50B** may be further used in reflection mode to measure pulse by utilizing their coherency, i.e. light source **50B** may function as laser light source **71** of CLS apparatus **72** (**Figure 16B**). In embodiments, at least two light sources **50** may comprise any of the following options: two LEDs having different wavelength ranges, two laser diodes with different wavelengths, or one LED and one laser diode outside a wavelength range of the LEDs. **Figure 16D** illustrates a configuration in which light sources **50** are within dome **40**, for example, a LED **50A** and another LED **50B** or a coherent light source **71** with its detector **73** which transmit light that is reflected by the ulna to detector **52**. Another possibility is that one light source **50A** is within dome **40** and another light source **50B** (and/or coherent light source **71** with its detector **73**) is outside dome **40**. **Figure 16E** illustrates a configuration in which light sources **50** (**50A** and **50B** or coherent light source **71**) are within dome **40**, while detector **52** is outside dome **40**. Any combination of positions of light source **50** and detector **52** which yields measurement by trans-illumination over the distal end of the ulna may be realized in pulse oximetry device **30**.

[0054] **Figures 17A** and **17B** schematically illustrate a perspective view of the wrist worn pulse oximetry device **30** in an unworn position, according to some embodiments of the invention. Dome **40** with detector **52**, CLS apparatus **72** and at least two light source **50** may be mounted on strap **32** at functional positions, with dome **40** fitting the distal end of the ulna bone as reference point. Dome **40** may be padded internally by a soft material to establish good contact and good fitting to the bone, and improving the signal to noise ratio by pressing gently on the area above it to remove venous blood from the area. **Figure 17A** illustrates a configuration with detector **52** within dome **40** and light sources **50** and coherent light source **71** outside dome **40** (light sources **50** at distance d from dome **40**). Coherent light source **71**

may replace light source(s) **50** by configuring detector **52** to measure light emitted from coherent light source **71** and reflected by ulna (thereby losing its coherence). **Figure 17A** further illustrates an alternative configuration with one or more of light sources **50** within dome **40**, a configuration similar to the one illustrated in **Figure 16D**. **Figure 17B** illustrates a configuration with detector **52** outside dome **40** and light sources **50** outside dome **40**, a configuration similar to the one illustrated in **Figure 16E**.

[0055] **Figure 18** is a schematic flowchart illustrating a method **500** of oximetry measurement, according to some embodiments of the invention.

[0056] Method **500** comprises: fixating an area above a distal end of the ulna (stage **510**), carried out e.g. by a dome shaped structure configured to fit over the distal end of the ulna, positioning a detector above the fixated area (stage **520**), locating at least two light sources having different wave lengths at a periphery of the fixated area (stage **525**), emitting light into the wrist by the located light sources (stage **540**), and detecting reflections by the distal end of the ulna of the at least two light sources (stage **550**). The angle between the emitted light and the detected reflections is between 20° and 160° . Method **500** may further comprise locating the light sources in the dome and positioning the detector inside or outside the dome (stage **530**) as alternatives to stages **520** and **525**.

[0057] Method **500** may further comprise measuring a pulse by reflecting a coherent light source off a bone (stage **560**), comprising emitting coherent light by at least one coherent light source coupled to a strap holding the detector and the at least two light sources, detecting by at least one light detector light resulting from the emitted coherent light, obtaining coherent light scattering (CLS) data based on the detected light resulting from the emitted coherent light, and obtaining pulse rate and pulse waveform usable for SPO2 calculation based on CLS data, wherein the at least one coherent light source and the at least one light detector are coupled to the strap.

[0058] Method **500** may further comprise using the coherent light source as one of the at least two light sources (stage **535**).

[0059] In the above description, an embodiment is an example or implementation of the invention. The various appearances of "one embodiment", "an embodiment" or "some embodiments" do not necessarily all refer to the same embodiments.

[0060] Although various features of the invention may be described in the context of a single embodiment, the features may also be provided separately or in any suitable combination. Conversely, although the invention may be described herein in the context of separate embodiments for clarity, the invention may also be implemented in a single embodiment.

[0061] Embodiments of the invention may include features from different embodiments disclosed above, and embodiments may incorporate elements from other em-

bodiments disclosed above. The disclosure of elements of the invention in the context of a specific embodiment is not to be taken as limiting their use in the specific embodiment alone.

[0062] Furthermore, it is to be understood that the invention can be carried out or practiced in various ways and that the invention can be implemented in embodiments other than the ones outlined in the description above.

[0063] The invention is not limited to those diagrams or to the corresponding descriptions. For example, flow need not move through each illustrated box or state, or in exactly the same order as illustrated and described.

[0064] Meanings of technical and scientific terms used herein are to be commonly understood as by one of ordinary skill in the art to which the invention belongs, unless otherwise defined.

[0065] While the invention has been described with respect to a limited number of embodiments, these should not be construed as limitations on the scope of the invention, but rather as exemplifications of some of the preferred embodiments.

Claims

1. A pulse oximetry device comprising at least two light sources (50A, 50B) having different wavelengths and at least one detector (52) responsive to said different wavelengths, **characterised in that** said device further comprises:

a dome-shaped or cone-shaped structure (40) adapted to be placed over and receive the distal end of the ulna bone (38) and to fixate the device at a fixated area (41) above the distal end of the ulna; wherein said at least two light sources (50A, 50B) and/or said at least one detector (52) is positioned within said structure (40); and wherein said at least one detector is adapted to detect light for providing pulse oximetry measurements, said detected light being trans-illumination light originating from said at least two light sources and reflecting off a surface of the distal end of the ulna at an angle larger than 0° and smaller than 180° and passing through the fixated area.

2. The device of claim 1, wherein said at least one detector is adapted to measure said trans-illumination at an angle between about 20° and 160° relative to an incident path of the emitted light.
3. The device of claim 1, wherein said at least one detector is adapted to measure said trans-illumination at an angle between about 70° and 110° relative to an incident path of the emitted light.

4. The device of claim 1, wherein said at least two light sources are components selected from the group consisting of: LEDs having different wavelength ranges, laser diodes having different wavelengths, and a combination of LEDs and laser diodes having wavelengths outside the wavelength range of the LEDs.

5. The device of claim 1, the device further comprising a processor (56) configured to calculate oximetry data from said trans-illumination.

6. The device of claim 5, wherein said processor is further configured to obtain pulse rates and pulse waveforms usable for SpO₂ calculations.

7. The device of claim 1, the device further comprising a casing (34) for housing said structure (40), said at least two light sources (50A, 50B), and said at least one detector (52).

8. The device of claim 1, wherein said at least one detector (52) is positioned within said structure (40) and said at least two light sources (50A, 50B) are positioned adjacent to said structure (40).

9. The device of claim 1, wherein said at least two light sources (50A, 50B) are positioned within said structure (40) and said at least one detector (52) is positioned adjacent to said structure (40).

10. A method of measuring an oxygen level in the blood, the method comprising the steps of measuring the oxygen level using a device according to any of claims 1 to 9, **characterised by:**

fixating the device at the fixated area (41) by receiving the distal end of the ulna in the dome-shaped or cone-shaped structure (40), wherein at least one of said at least two light sources (50A, 50B) and said at least one detector (52) is positioned within said structure and measuring, by said at least one detector, trans-illumination via the distal end of the ulna through said fixated area, wherein said trans-illumination originates from emitted light from said at least two light sources and is reflected off the surface of the distal end of the ulna at an angle larger than 0° and smaller than 180°.

11. The method of claim 10, wherein said at least one detector measures said trans-illumination at an angle between about 20° and 160° relative to an incident path of said emitted light.

12. The method of claim 10, wherein said at least one detector measures said trans-illumination at an angle between about 70° and 110° relative to an inci-

dent path of said emitted light.

13. The method of claim 10, the method further comprising the step of calculating oximetry data from said trans-illumination.
14. The method of claim 13, wherein the step of calculating includes obtaining pulse rates and pulse waveforms usable for SpO₂ calculations.

Patentansprüche

1. Pulsoximetrievorrichtung mit mindestens zwei Lichtquellen (50A, 50B) mit unterschiedlichen Wellenlängen und mindestens einem Detektor (42), der auf die unterschiedlichen Wellenlängen empfindlich reagiert, **dadurch gekennzeichnet, dass** die Vorrichtung ferner aufweist:

eine Dom-förmige oder Konus-förmige Struktur (40), die dazu angepasst ist, über dem distalen Ende des Ellen-Knochens (38) platziert zu werden, dieses aufzunehmen und die Vorrichtung bei einem fixierten Gebiet (41) über dem distalen Ende der Elle zu fixieren;

wobei die mindestens zwei Lichtquellen (50A, 50B) und/oder der mindestens eine Detektor (52) in der Struktur (40) positioniert ist; und wobei der mindestens einen Detektor dazu angepasst ist, Licht zum Bereitstellen von Pulsoximetriemessungen zu detektieren, wobei das detektierte Licht Durchleuchtungslicht ist, welches von den mindestens zwei Lichtquellen stammt und von einer Oberfläche des distalen Endes der Elle unter einem Winkel größer als 0° und kleiner als 180° reflektiert wird und durch das fixierte Gebiet tritt.

2. Vorrichtung nach Anspruch 1, wobei der mindestens eine Detektor dazu angepasst ist, das Durchleuchtungslicht unter einem Winkel zwischen ungefähr 20° und 160° relativ zu einem Einfallsweg des emittierten Lichts zu messen.
3. Vorrichtung nach Anspruch 1, wobei der mindestens eine Detektor dazu angepasst ist, dass Durchleuchtungslicht unter einem Winkel zwischen ungefähr 70° und 110° relativ zu einem Einfallsweg des emittierten Lichts zu messen.
4. Vorrichtung nach Anspruch 1, wobei die mindestens zwei Lichtquellen Bauteile sind, die aus der folgenden Gruppe gewählt wurden: LEDs mit unterschiedlichen Wellenlängenbereichen, Laserdioden mit unterschiedlichen Wellenlängen und einer Kombination von LEDs und Laserdioden mit Wellenlängen außerhalb des Wellenlängenbereichs der LEDs.

5. Vorrichtung nach Anspruch 1, ferner mit einem Prozessor (56), der dazu ausgebildet ist, Oximetriedaten von dem Durchleuchtungslicht zu berechnen.

6. Vorrichtung nach Anspruch 5, wobei der Prozessor ferner dazu ausgebildet ist, Pulsraten und Pulswellenformen, die für SpO₂-Berechnungen verwendbar sind, zu erhalten.

7. Vorrichtung nach Anspruch 1, ferner mit einem Gehäuse (34) zum Aufnehmen der Struktur (40), der mindestens zwei Lichtquellen (50A, 50B) und dem mindestens einen Detektor (52).

8. Vorrichtung nach Anspruch 1, wobei der mindestens eine Detektor (52) innerhalb der Struktur (40) positioniert ist und die mindestens zwei Lichtquellen (50A, 50B) neben der Struktur (40) positioniert sind.

9. Vorrichtung nach Anspruch 1, wobei die mindestens zwei Lichtquellen (50A, 50B) innerhalb der Struktur (40) positioniert sind und der mindestens eine Detektor (52) neben der Struktur (40) positioniert ist.

10. Verfahren zum Messen eines Sauerstoffgehalts in dem Blut, wobei das Verfahren die Schritte zum Messen des Sauerstoffgehalts unter Verwendung einer Vorrichtung nach einem der Ansprüche 1 bis 9 aufweist, **gekennzeichnet durch:**

Fixieren der Vorrichtung in dem fixierten Gebiet (41) durch Aufnehmen des distalen Endes der Elle in der Dom-förmigen oder Konus-förmigen Struktur (40), wobei die mindestens zwei Lichtquellen (50A, 50B) und/oder der mindestens einen Detektor (52) in der Struktur positioniert ist und

Messen, mit dem mindestens einen Detektor, eine Durchleuchtung durch das distale Ende der Elle durch das fixierte Gebiet, wobei die Durchleuchtung vom emittierten Licht der mindestens zwei Lichtquellen stammt und von der Oberfläche des distalen Endes der Elle unter einem Winkel größer als 0° und kleiner als 180° reflektiert wird.

11. Verfahren nach Anspruch 10, wobei der mindestens eine Detektor die Durchleuchtung bei einem Winkel zwischen ungefähr 20° und 160° relativ zu einem Einfallsweg des emittierten Lichts misst.

12. Verfahren nach Anspruch 10, wobei der mindestens eine Detektor die Durchleuchtung bei einem Winkel zwischen ungefähr 70° und 110° relativ zu einem Einfallsweg des emittierten Lichts misst.

13. Verfahren nach Anspruch 10, wobei das Verfahren ferner den Schritt des Berechnens von Oximetrieda-

ten von der Durchleuchtung umfasst.

14. Verfahren nach Anspruch 13, wobei der Schritt des Berechnens ein Erhalten von Pulsraten und Pulswellenformen, die für SpO₂-Berechnungen verwendbar sind, aufweist.

Revendications

1. Dispositif d'oxymétrie pulsée, comprenant au moins deux sources de lumière (50A, 50B) ayant différentes longueurs d'ondes et au moins un détecteur (52) répondant auxdites longueurs d'ondes différentes, **caractérisé en ce que** ledit dispositif comprend en outre :

une structure en forme de dôme ou en forme de cône (40) adaptée pour être placée sur l'extrémité distale de l'os ulna (38) et recevoir celle-ci et pour fixer le dispositif sur une surface fixée (41) au-dessus de l'extrémité distale de l'ulna ; dans lequel lesdites au moins deux sources de lumière (50A, 50B) et/ou ledit au moins un détecteur (52) sont positionnés à l'intérieur de ladite structure (40) ; et

dans lequel ledit au moins un détecteur est adapté pour détecter une lumière pour fournir des mesures d'oxymétrie pulsée, ladite lumière détectée étant une lumière trans-éclairage provenant desdites au moins deux sources de lumière et réfléchissant une surface de l'extrémité distale de l'ulna sur un angle supérieur à 0° et inférieur à 180° et passant au travers de la surface fixée.

2. Dispositif selon la revendication 1, dans lequel ledit au moins un détecteur est adapté pour mesurer ledit trans-éclairage à un angle entre environ 20° et 160° par rapport à une voie incidente de la lumière émise.
3. Dispositif selon la revendication 1, dans lequel ledit au moins un détecteur est adapté pour mesurer ledit trans-éclairage à un angle entre environ 70° et 110° par rapport à une voie incidente de la lumière émise.
4. Dispositif selon la revendication 1, dans lequel lesdites au moins deux sources de lumière sont des composants choisis dans le groupe consistant en LED ayant différentes plages de longueurs d'ondes, des diodes lasers ayant différentes longueurs d'ondes, et une combinaison de LED et de diodes laser ayant des longueurs d'ondes hors de la plage de longueurs d'ondes des LED.
5. Dispositif selon la revendication 1, dans lequel le dispositif comprend en outre un processeur (56) configuré pour calculer des données d'oxymétrie dudit

trans-éclairage.

6. Dispositif selon la revendication 5, dans lequel ledit processeur est en outre configuré pour obtenir des taux d'impulsion et des formes d'ondes d'impulsion utilisables pour des calculs de SpO₂.
7. Dispositif selon la revendication 1, le dispositif comprenant en outre un boîtier (34) pour loger ladite structure (40), lesdites au moins deux sources de lumière (50A, 50B) et ledit au moins un détecteur (52).
8. Dispositif selon la revendication 1, dans lequel ledit au moins un détecteur (52) est positionné à l'intérieur de ladite structure (40) et lesdites au moins deux sources de lumière (50A, 50B), sont positionnées de manière adjacente à ladite structure (40).
9. Dispositif selon la revendication 1, dans lequel lesdites au moins deux sources de lumière (50A, 50B) sont positionnées à l'intérieure de ladite structure (40) et ledit au moins un détecteur (52) est positionné de manière adjacente auxdites structures (40).
10. Procédé de mesure d'un niveau d'oxygène dans le sang, le procédé comprenant les étapes de mesure du niveau d'oxygène en utilisant un dispositif selon l'une quelconque des revendications 1 à 9, **caractérisé par** :
- la fixation du dispositif sur la surface fixée (41) en recevant l'extrémité distale de l'ulna dans la structure en forme de dôme ou en forme de cône (40), dans lequel au moins l'une desdites au moins deux sources de lumière (50A, 50B) et ledit au moins un détecteur (52) est positionné à l'intérieur de ladite structure, la mesure, par ledit au moins un détecteur, du trans-éclairage via l'extrémité distale de l'ulna dans ladite zone fixée, dans lequel ledit trans-éclairage provient d'une lumière émise desdites au moins deux sources de lumière et est réfléchi de la surface de l'extrémité distale de l'ulna à un angle supérieur à 0° et inférieur à 180°.
11. Procédé selon la revendication 10, dans lequel ledit au moins un détecteur mesure ledit trans-éclairage à un angle entre environ 20° et 160° par rapport à une voie incidente de ladite lumière émise.
12. Procédé selon la revendication 10, dans lequel ledit au moins un détecteur mesure ledit trans-éclairage à un angle entre environ 70° et 110° par rapport à une voie incidente de ladite lumière émise.
13. Procédé selon la revendication 10, le procédé comprenant en outre l'étape de calcul de données d'oxy-

métrie à partir dudit trans-éclairage.

14. Procédé selon la revendication 13, dans lequel l'étape de calcul comporte l'obtention de taux pulsés et les formes d'ondes d'impulsion utilisables pour des calculs de SpO₂.

5

10

15

20

25

30

35

40

45

50

55

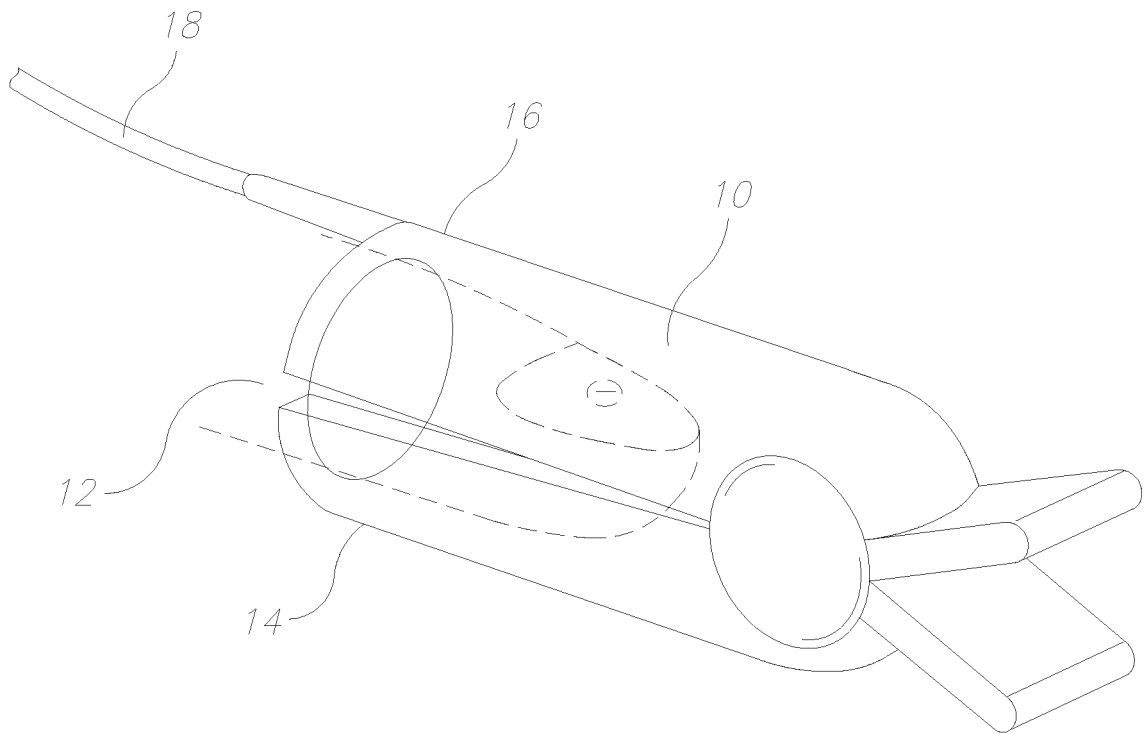


Figure 1
PRIOR ART

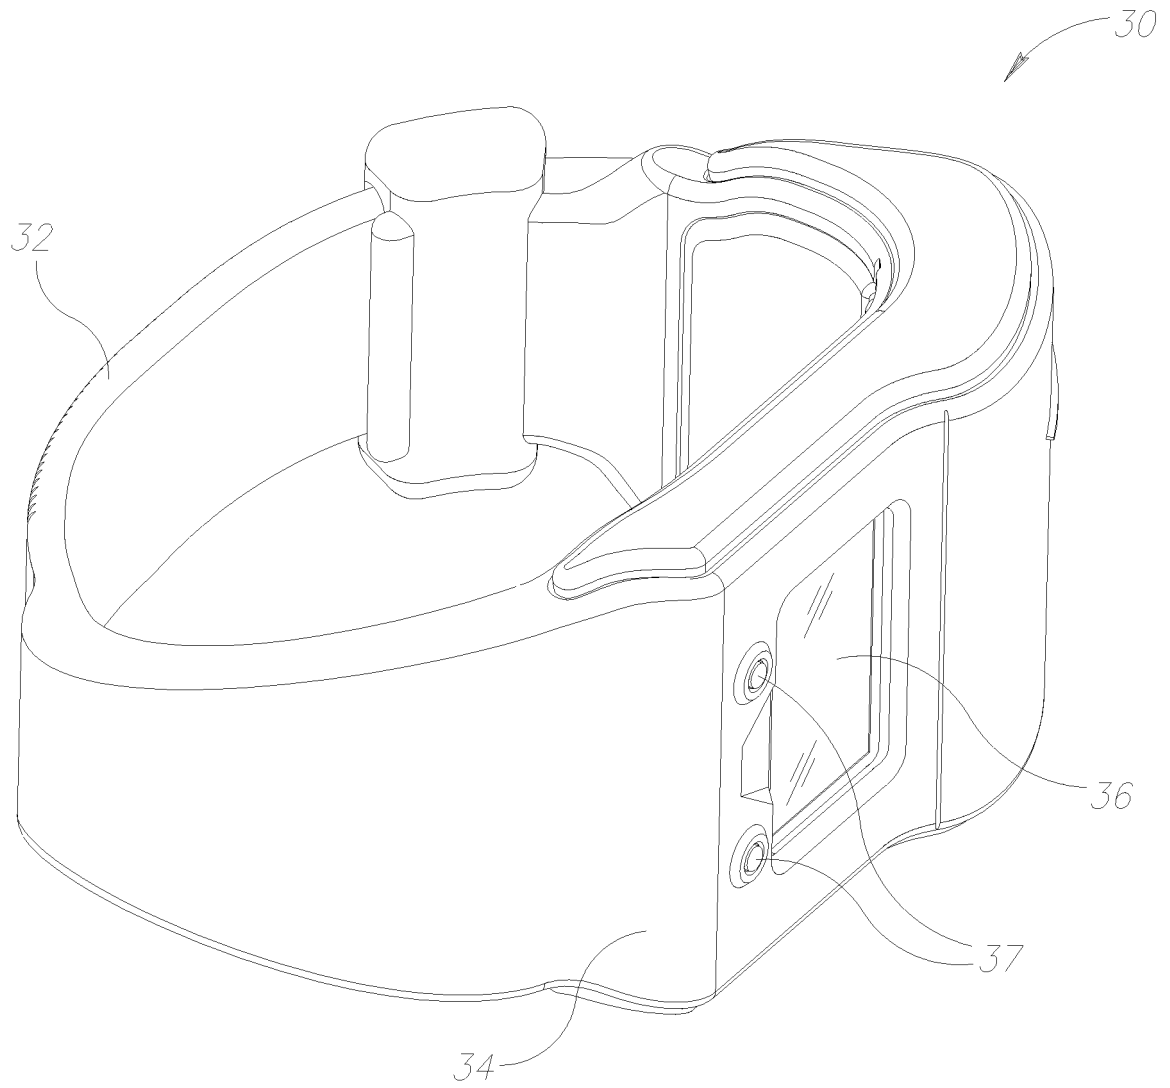


Figure 2

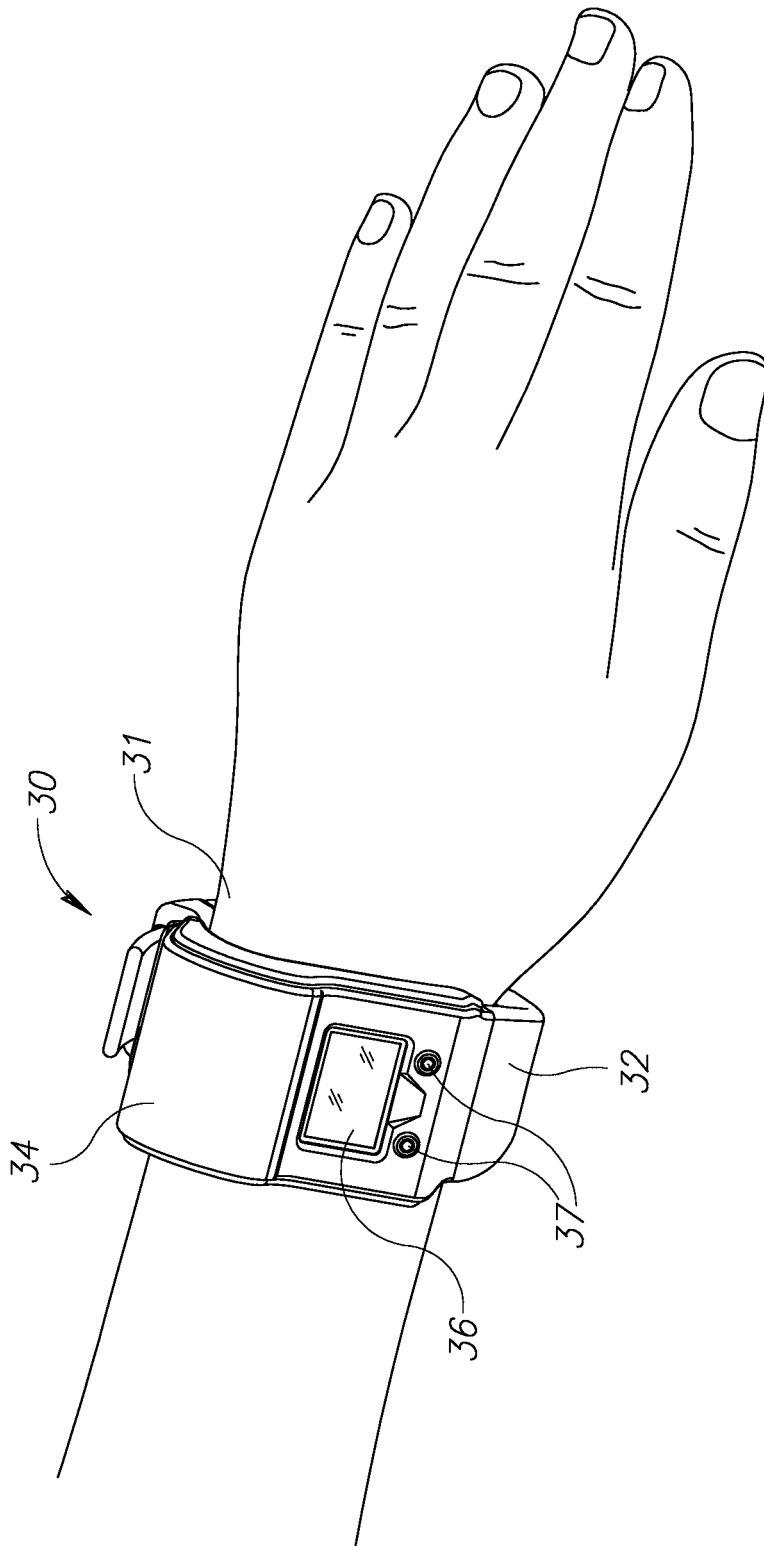


Figure 3

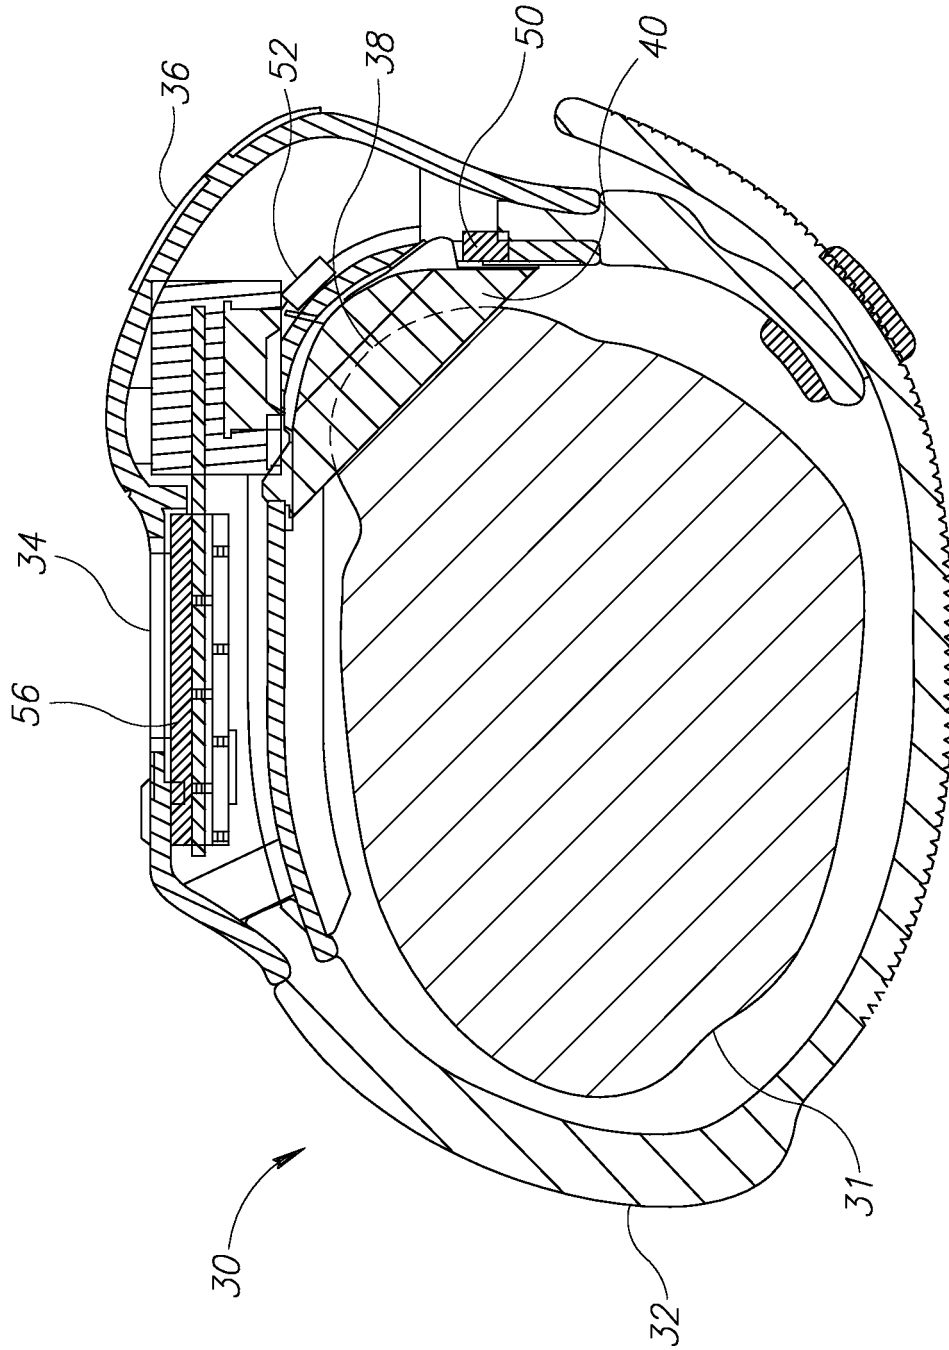


Figure 4

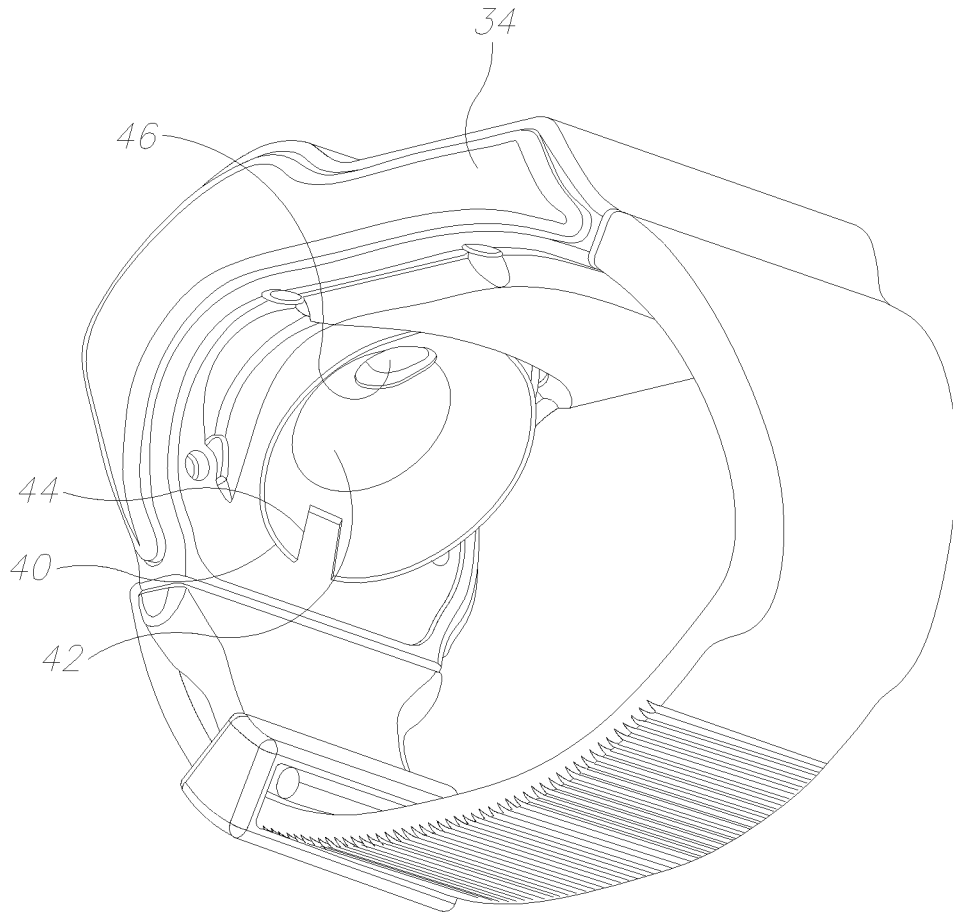


Figure 5

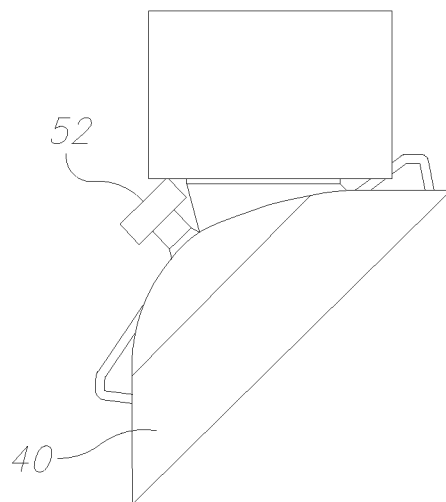


Figure 6

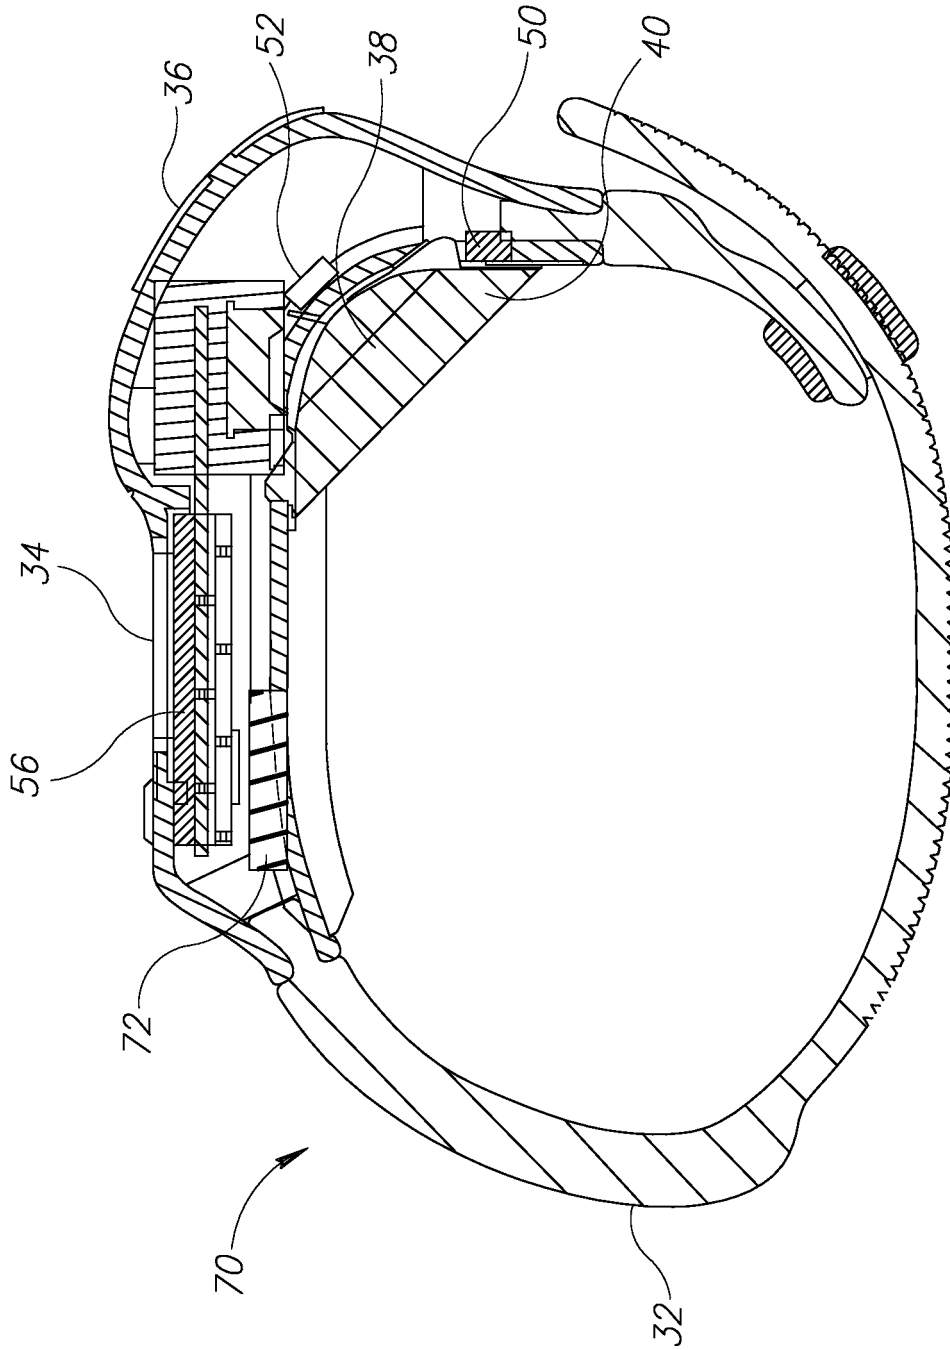


Figure 7A

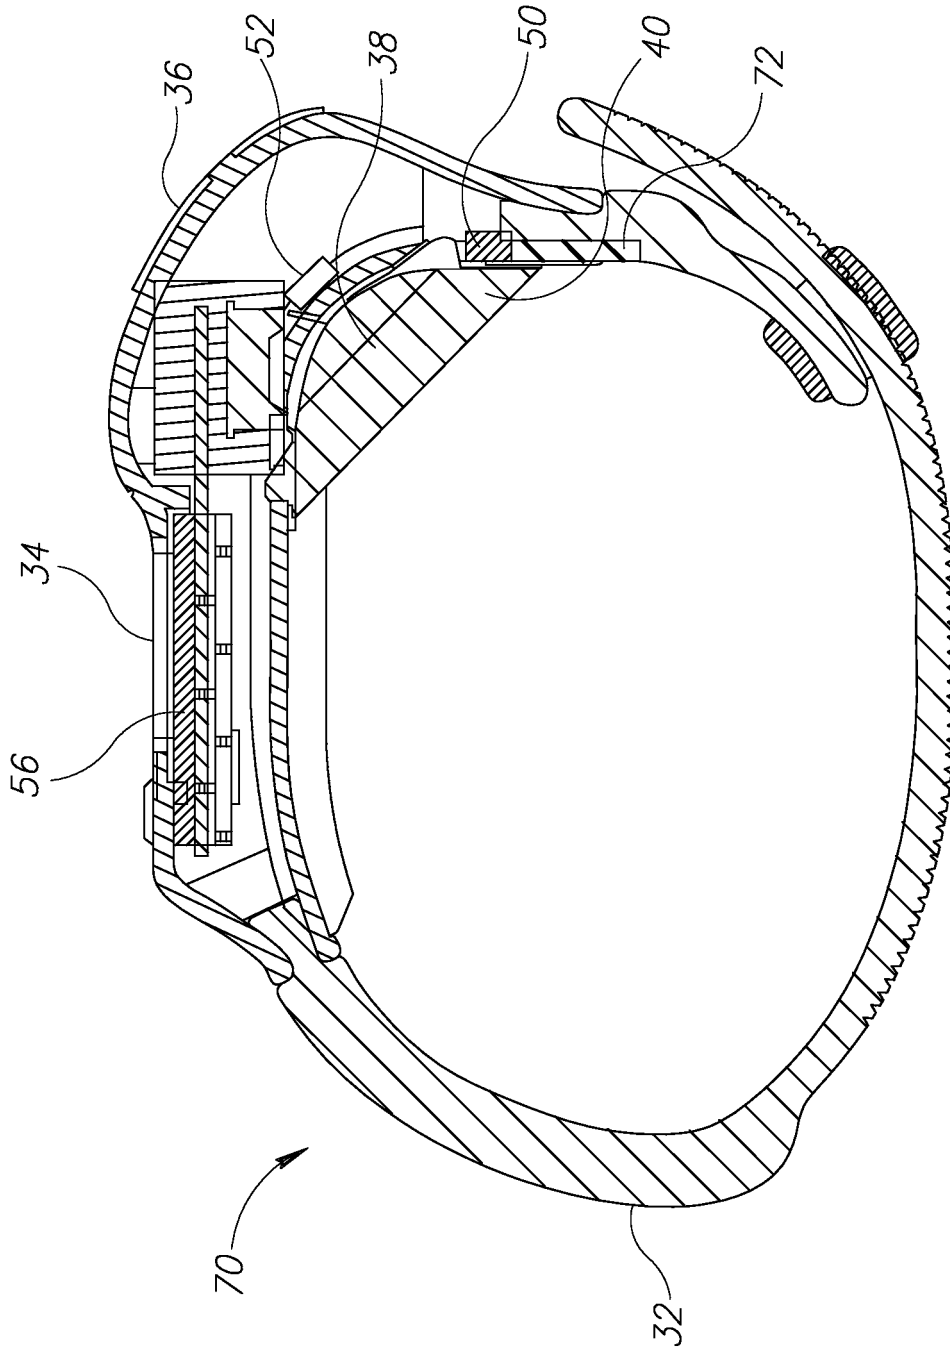


Figure 7B

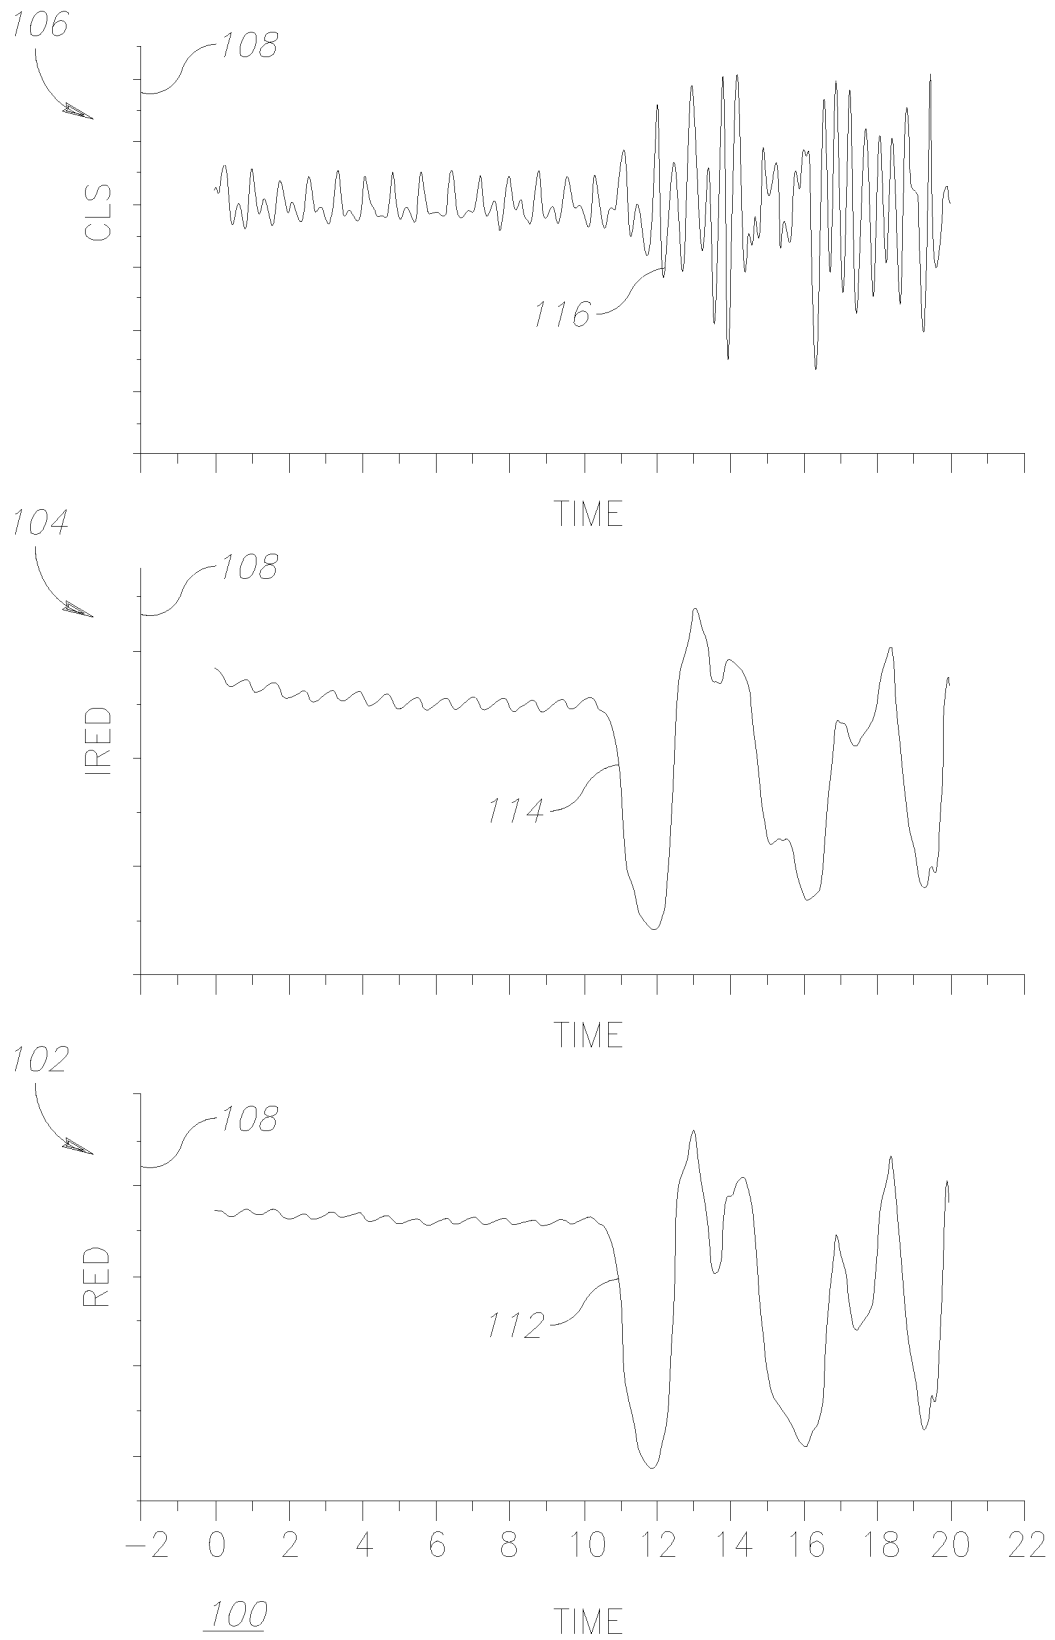


Figure 8

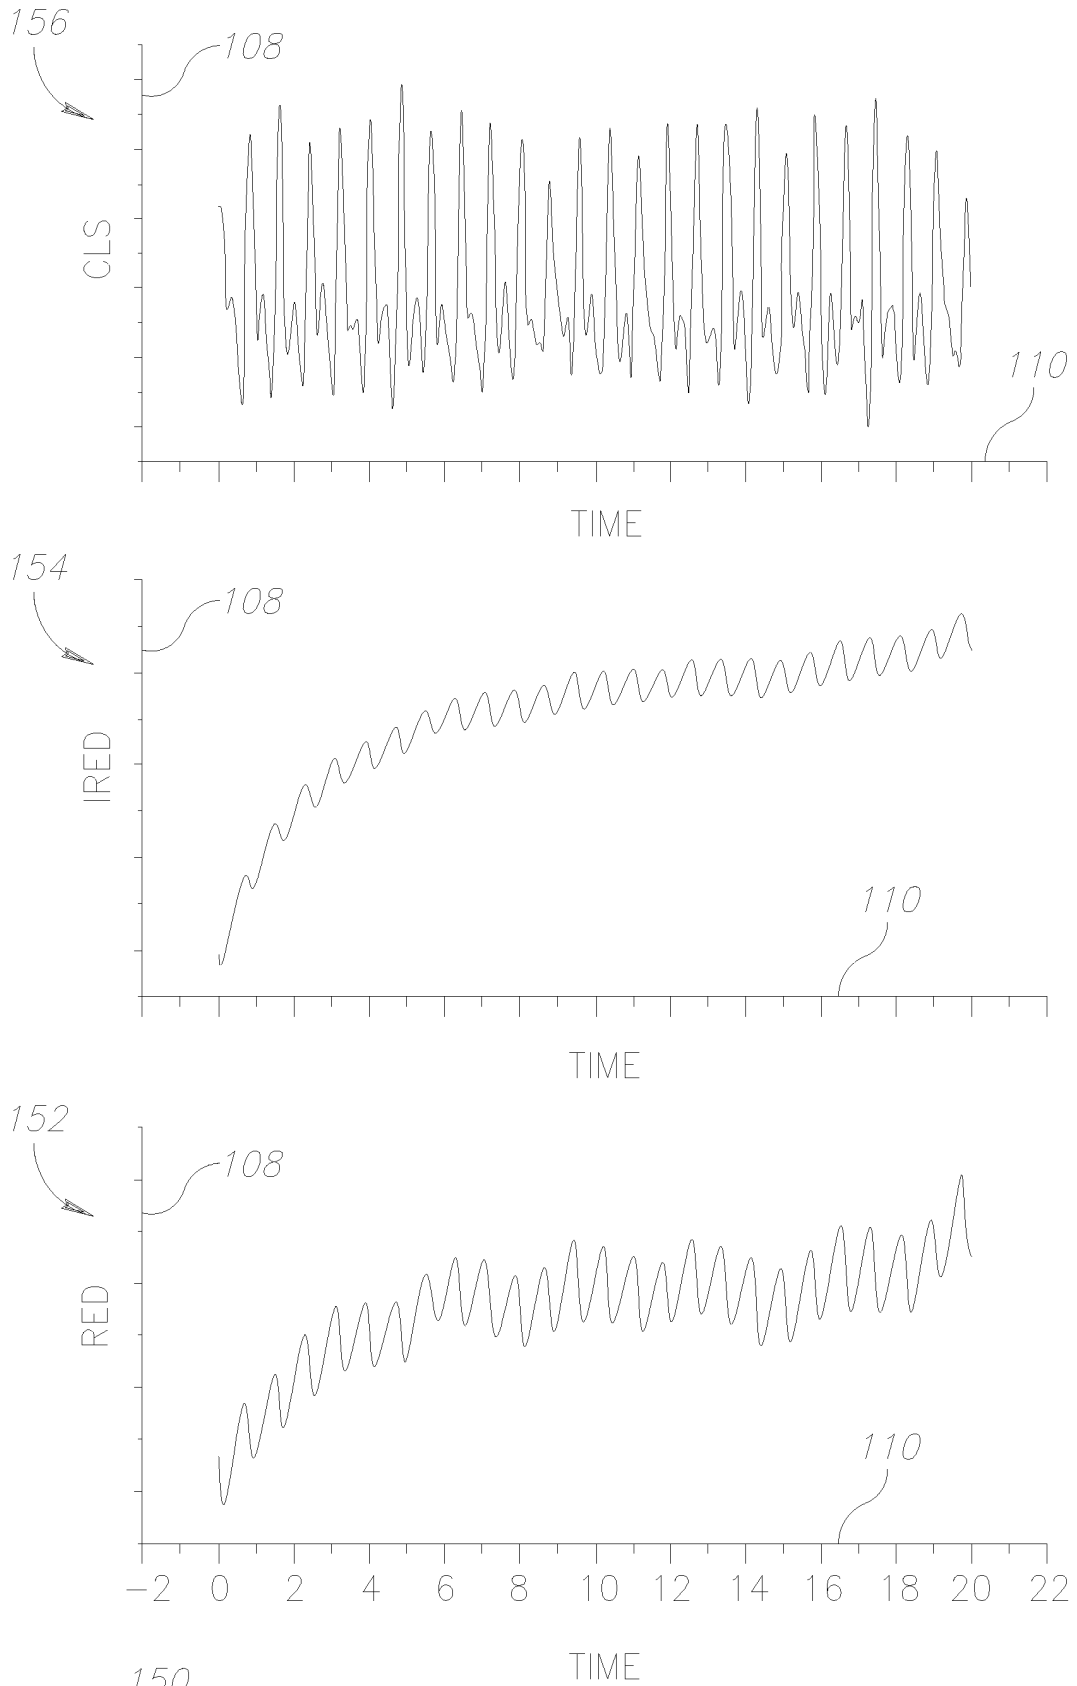


Figure 9

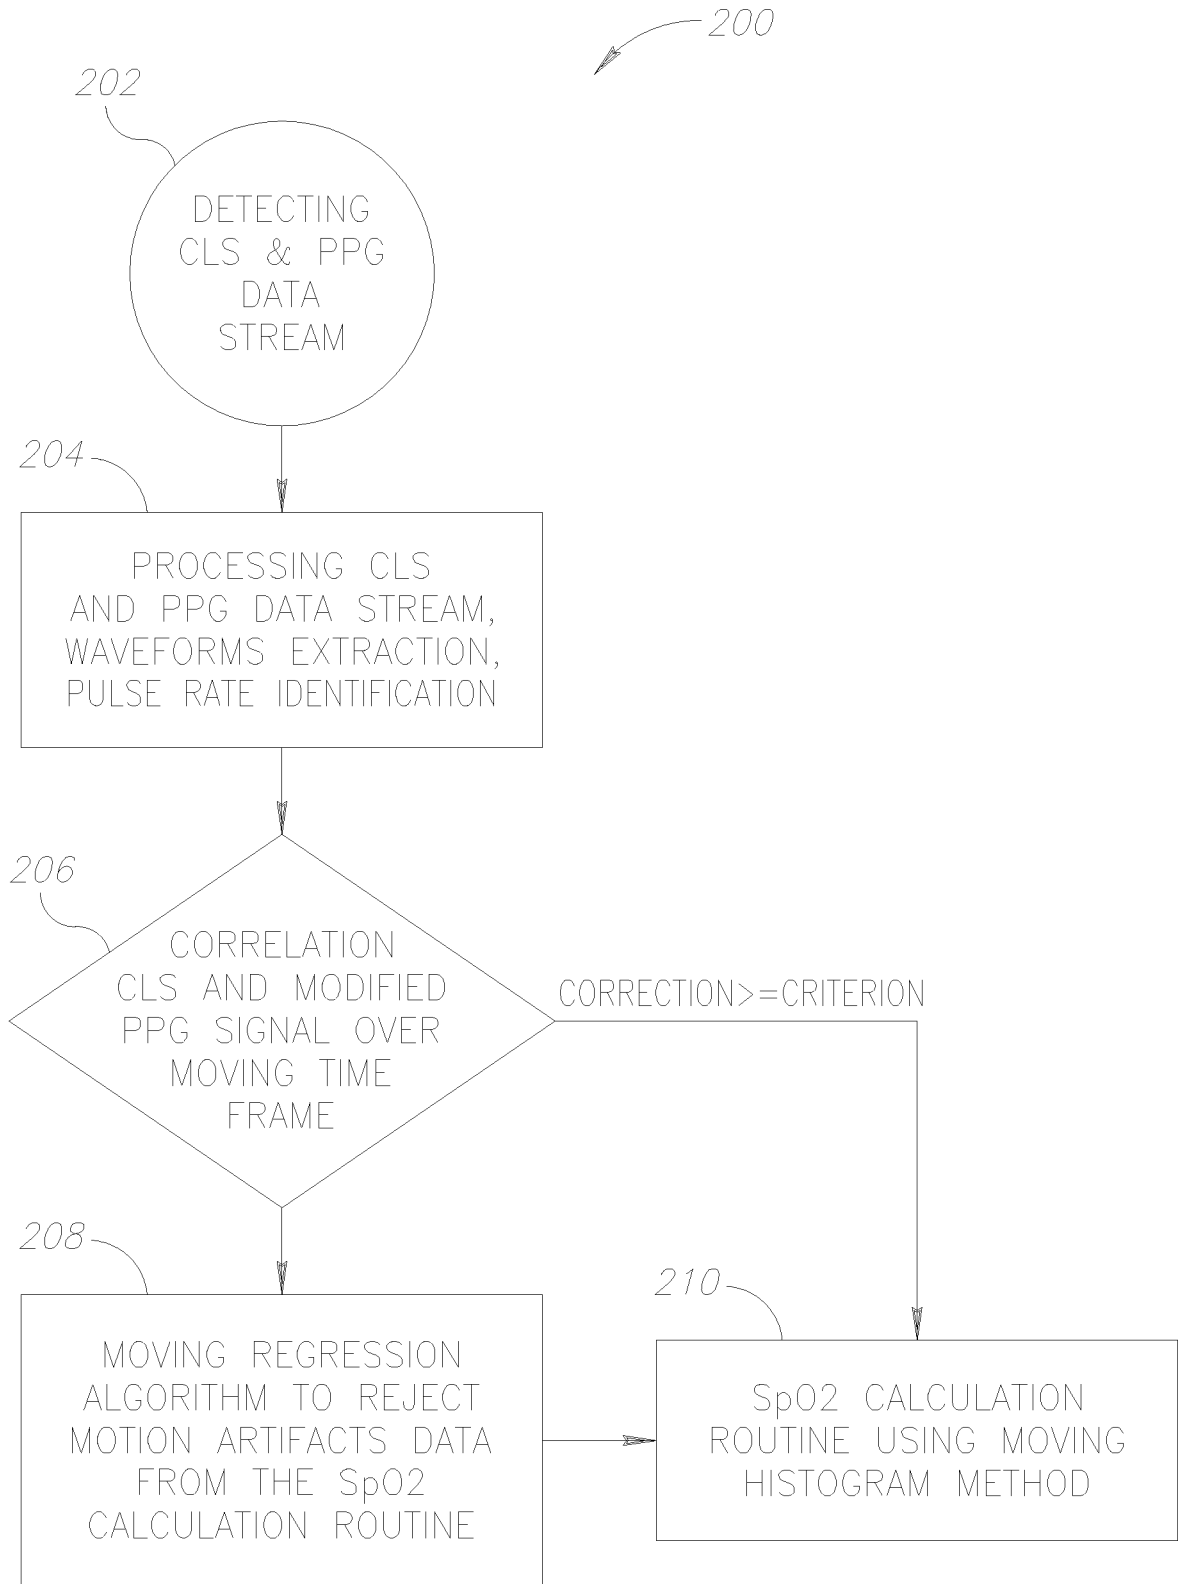


Figure 10

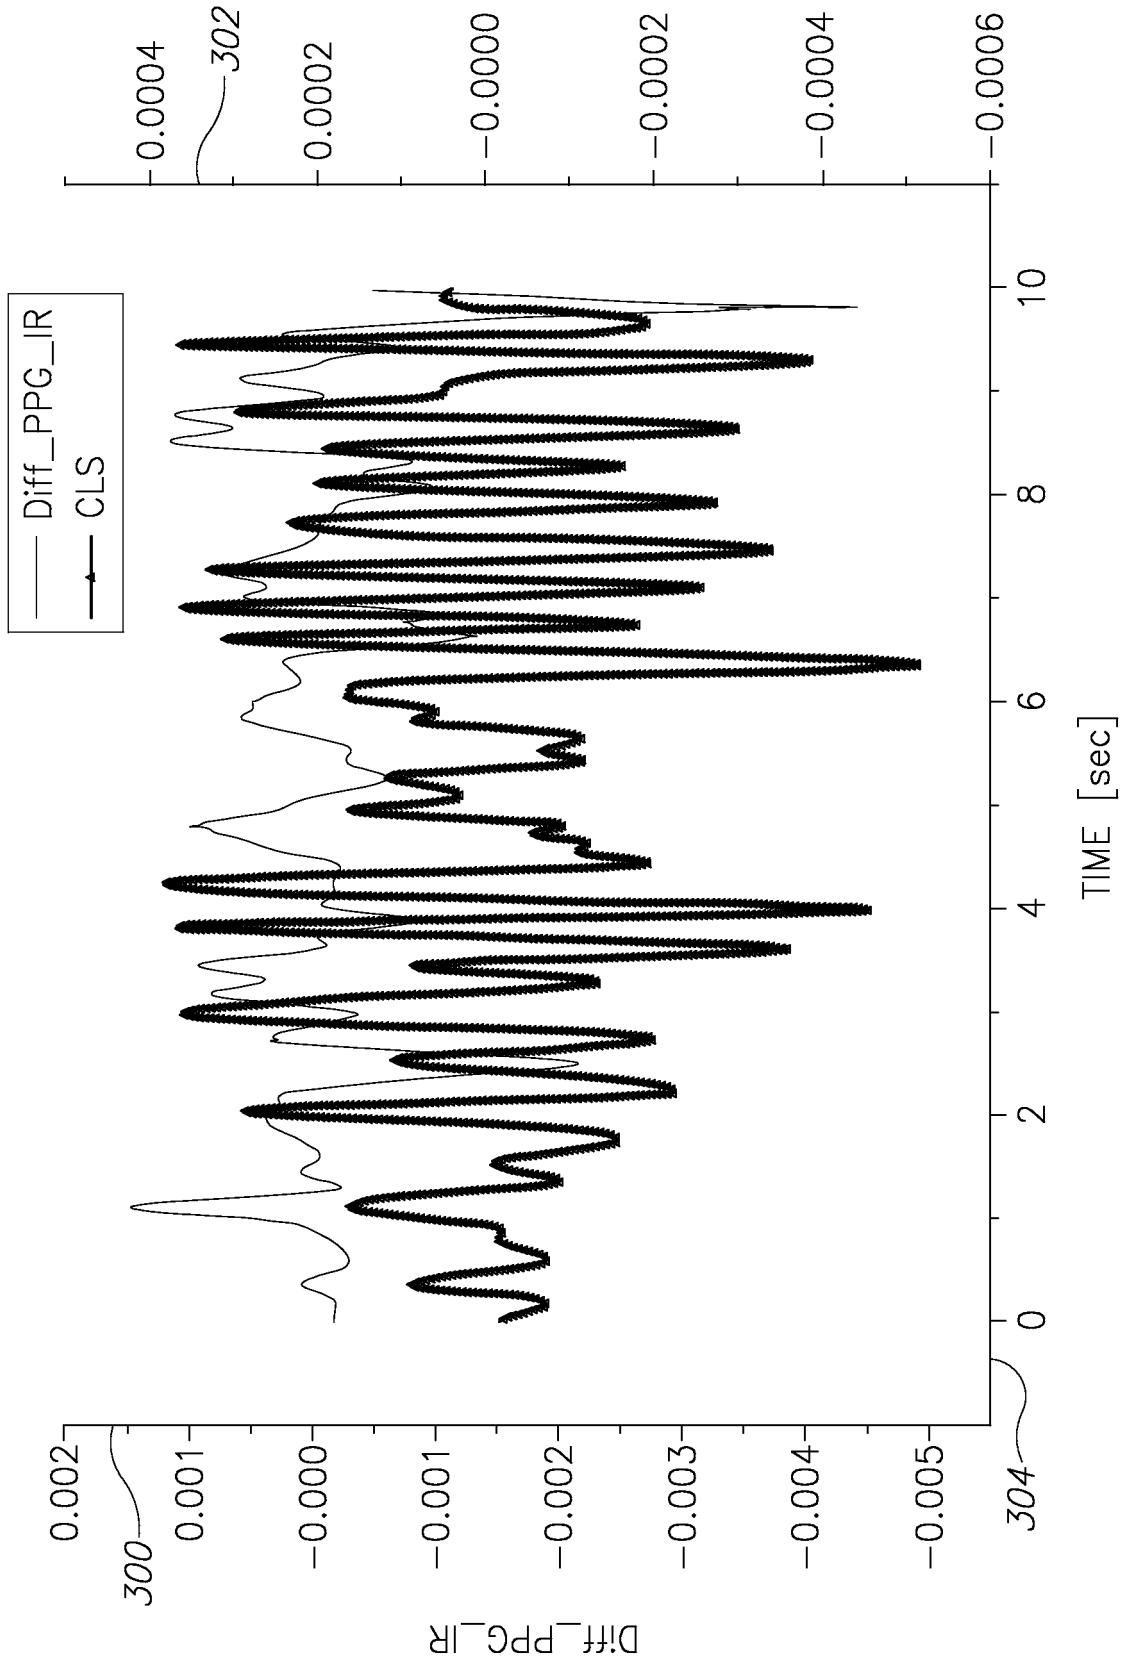


Figure 11

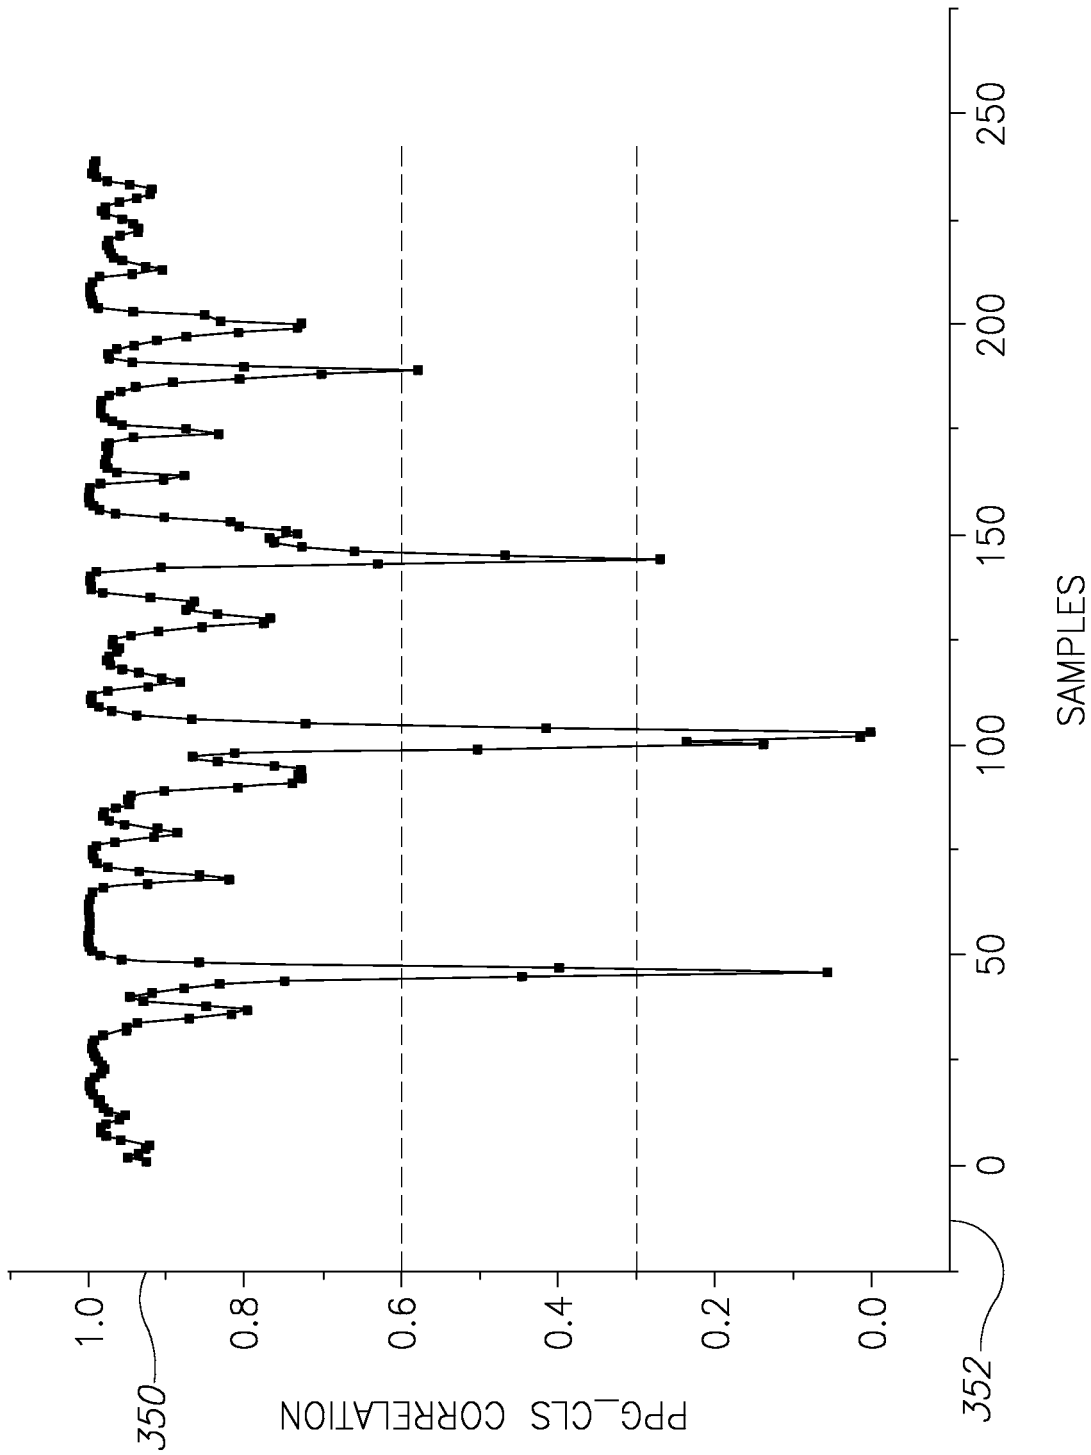


Figure 12

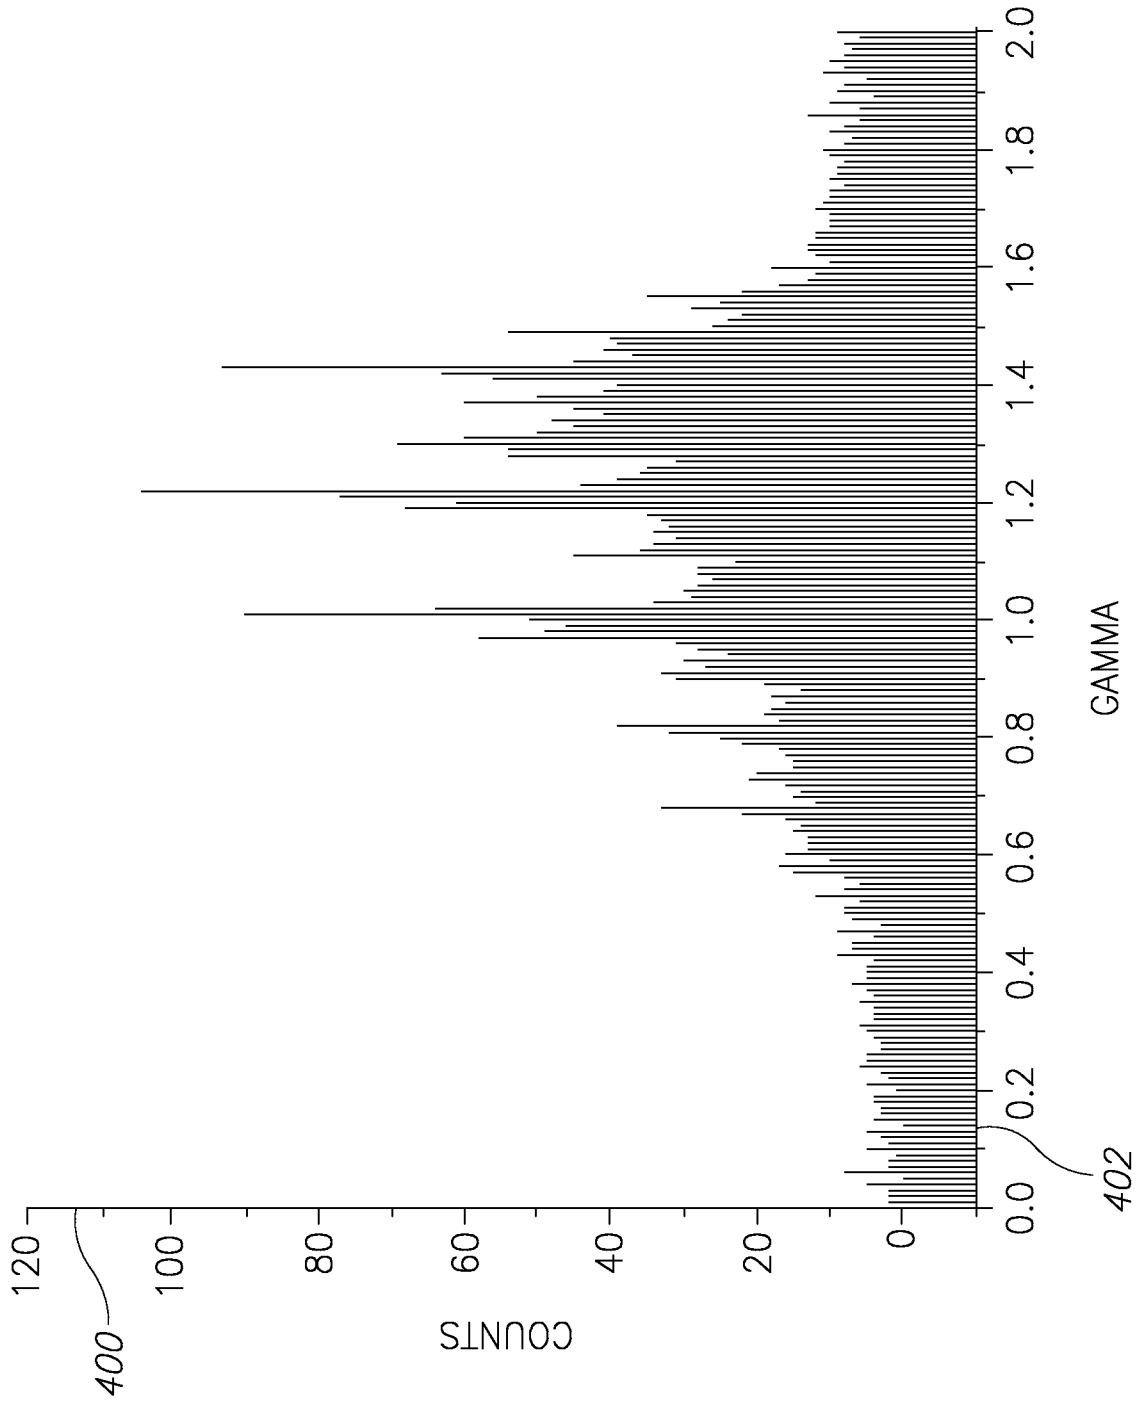


Figure 13

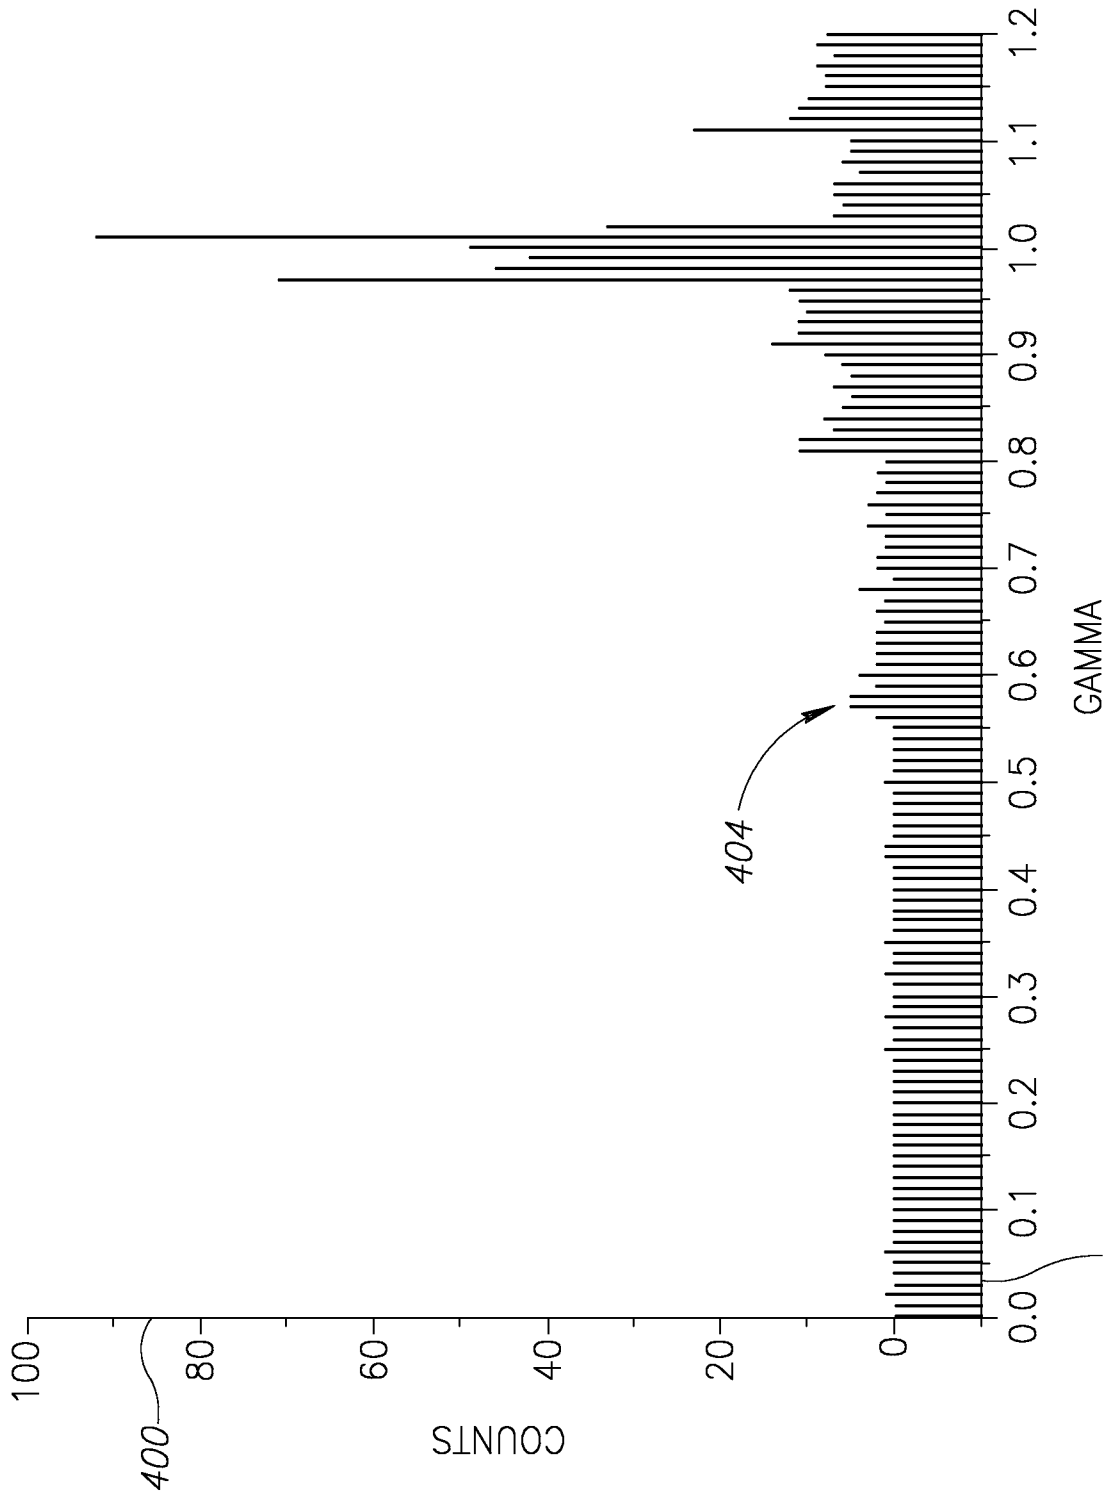


Figure 14

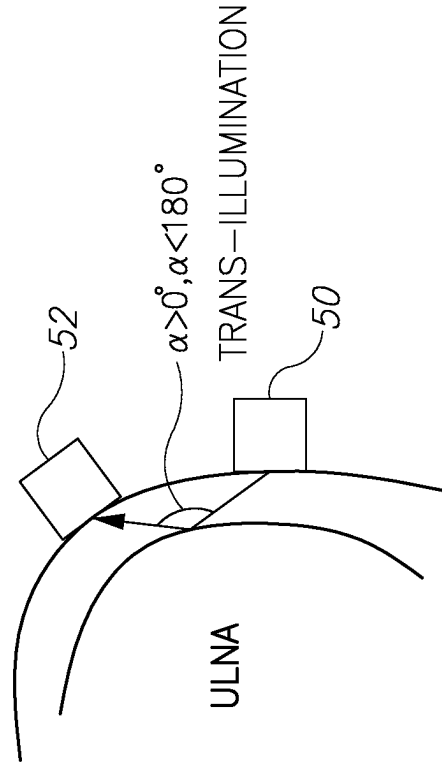
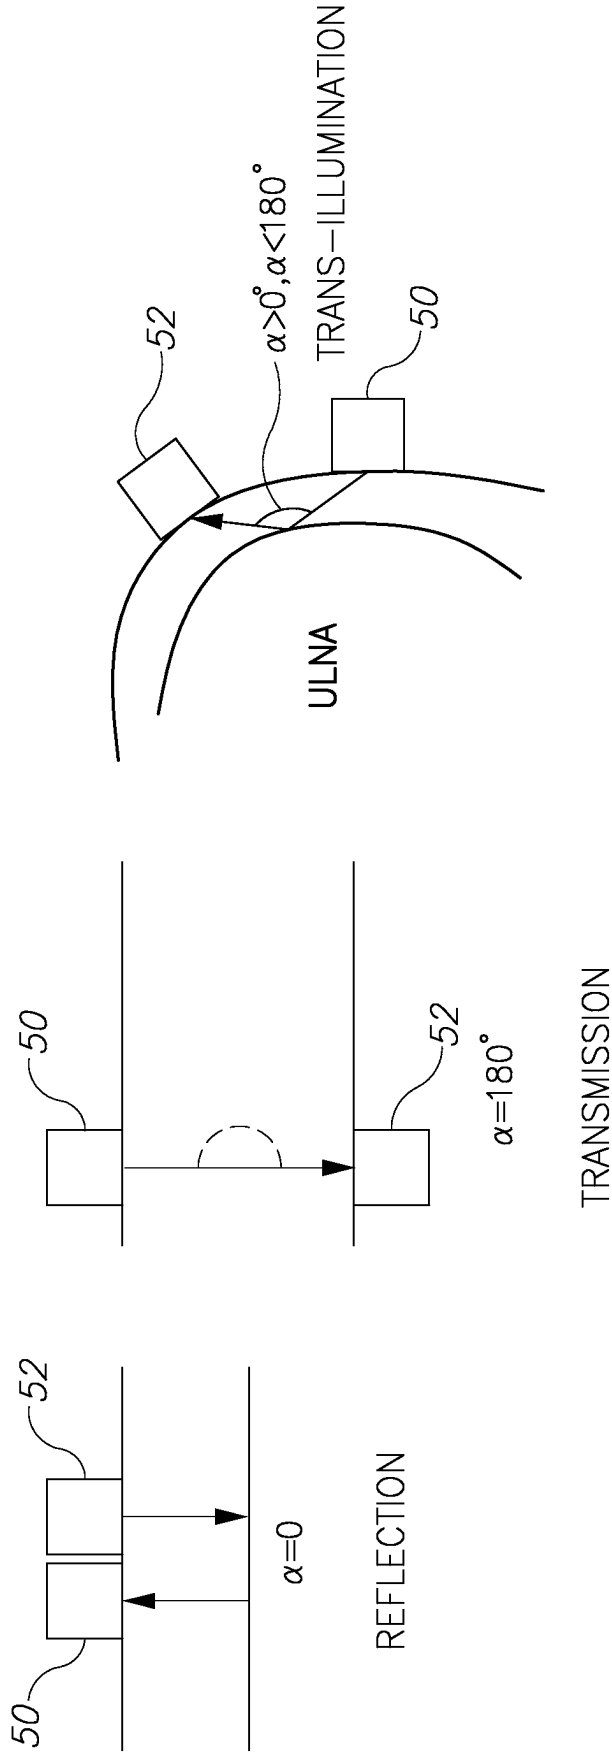


Figure 15A
PRIOR ART

Figure 15B

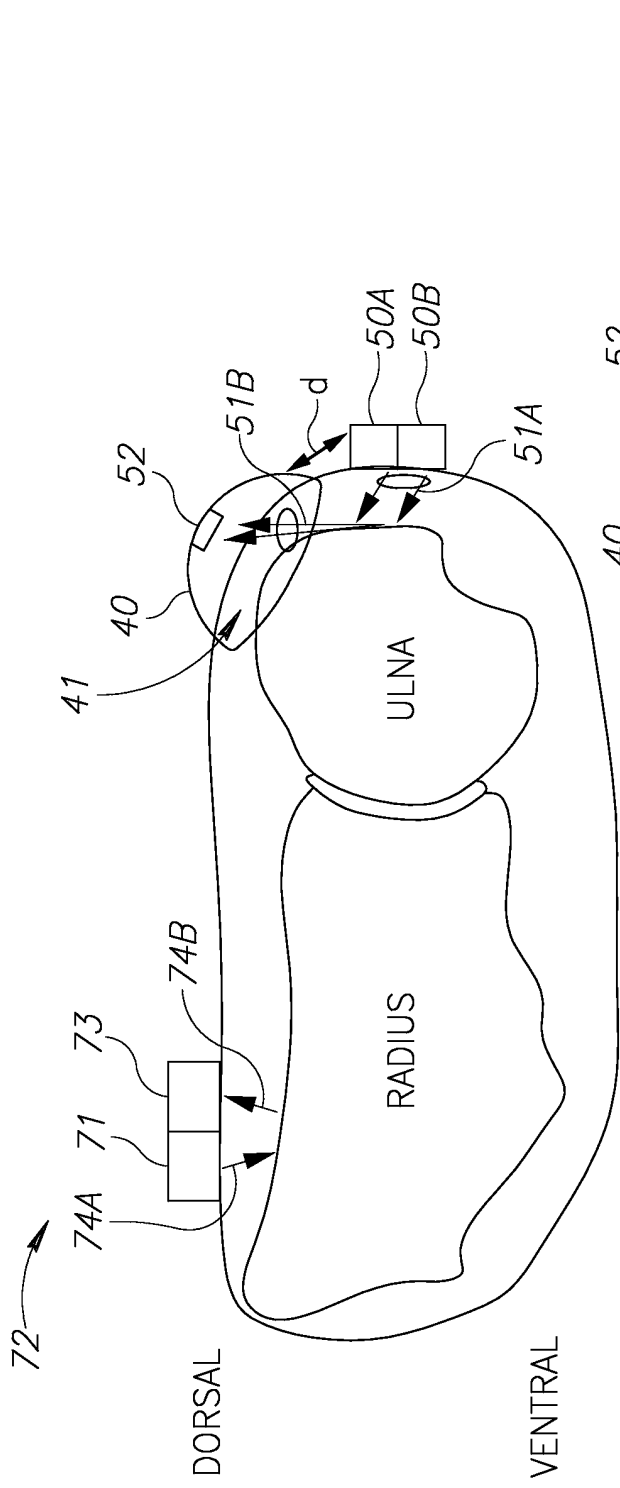


Figure 16A

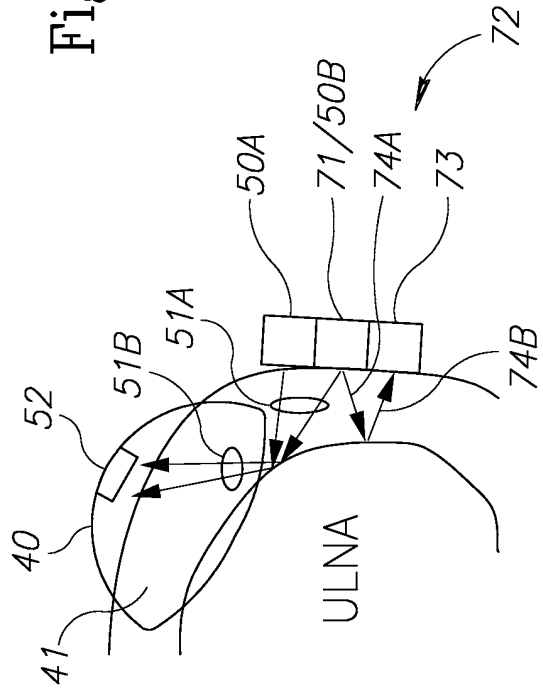


Figure 16B

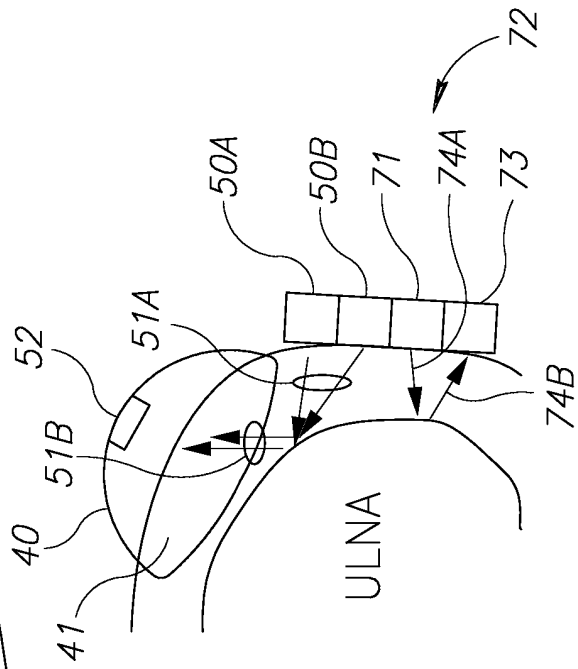


Figure 16C

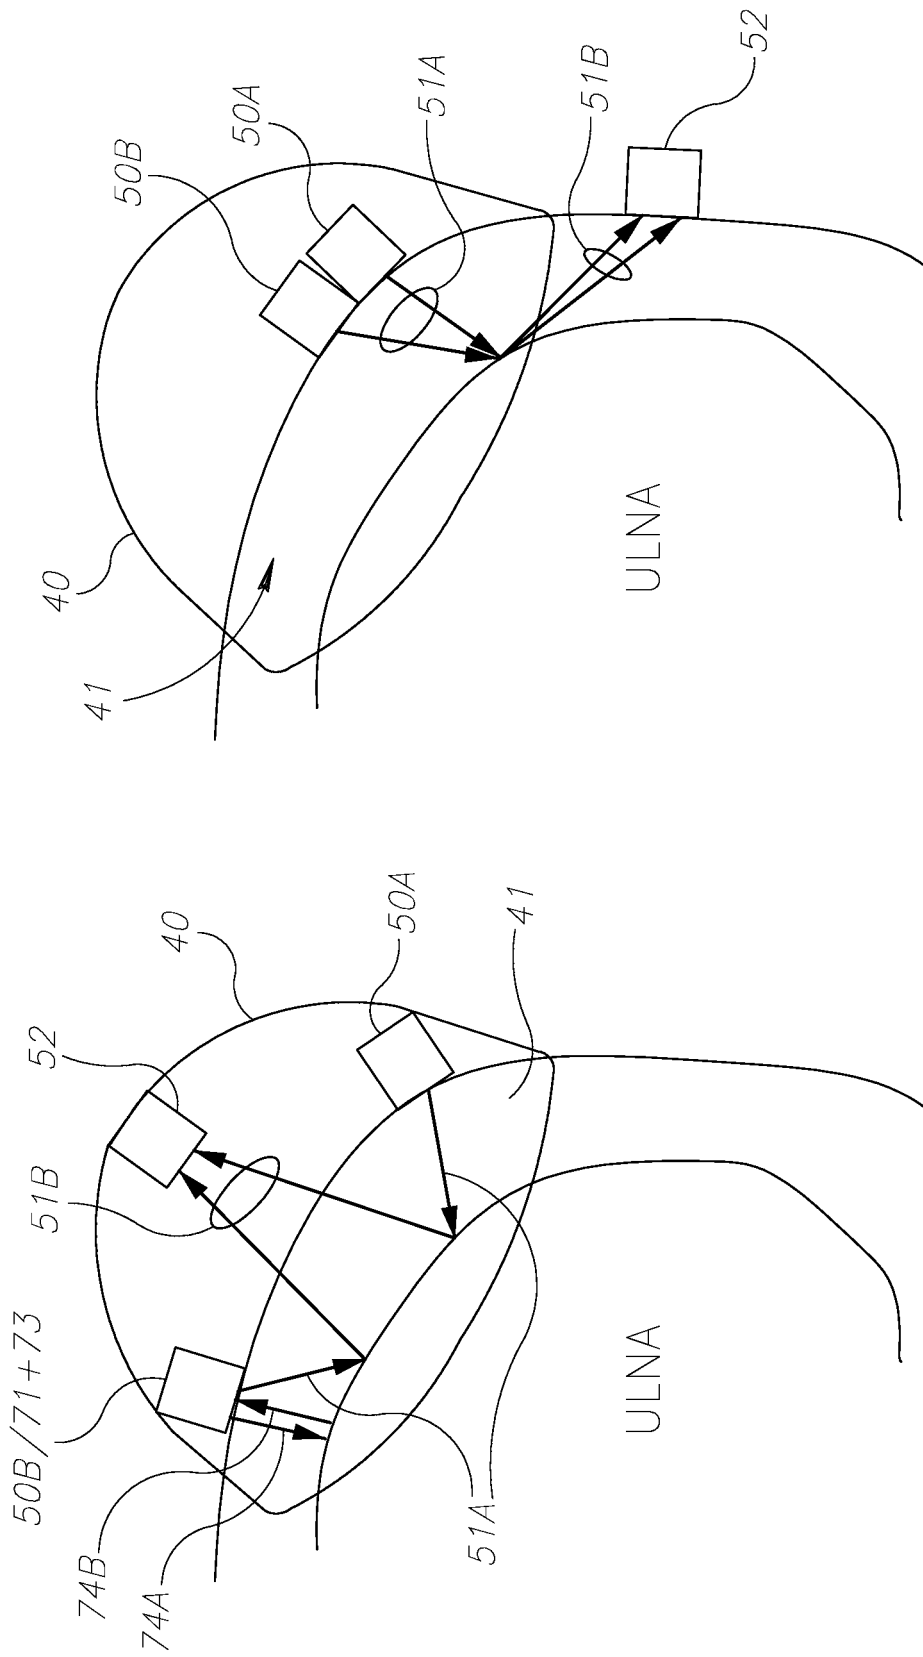


Figure 16E

Figure 16D

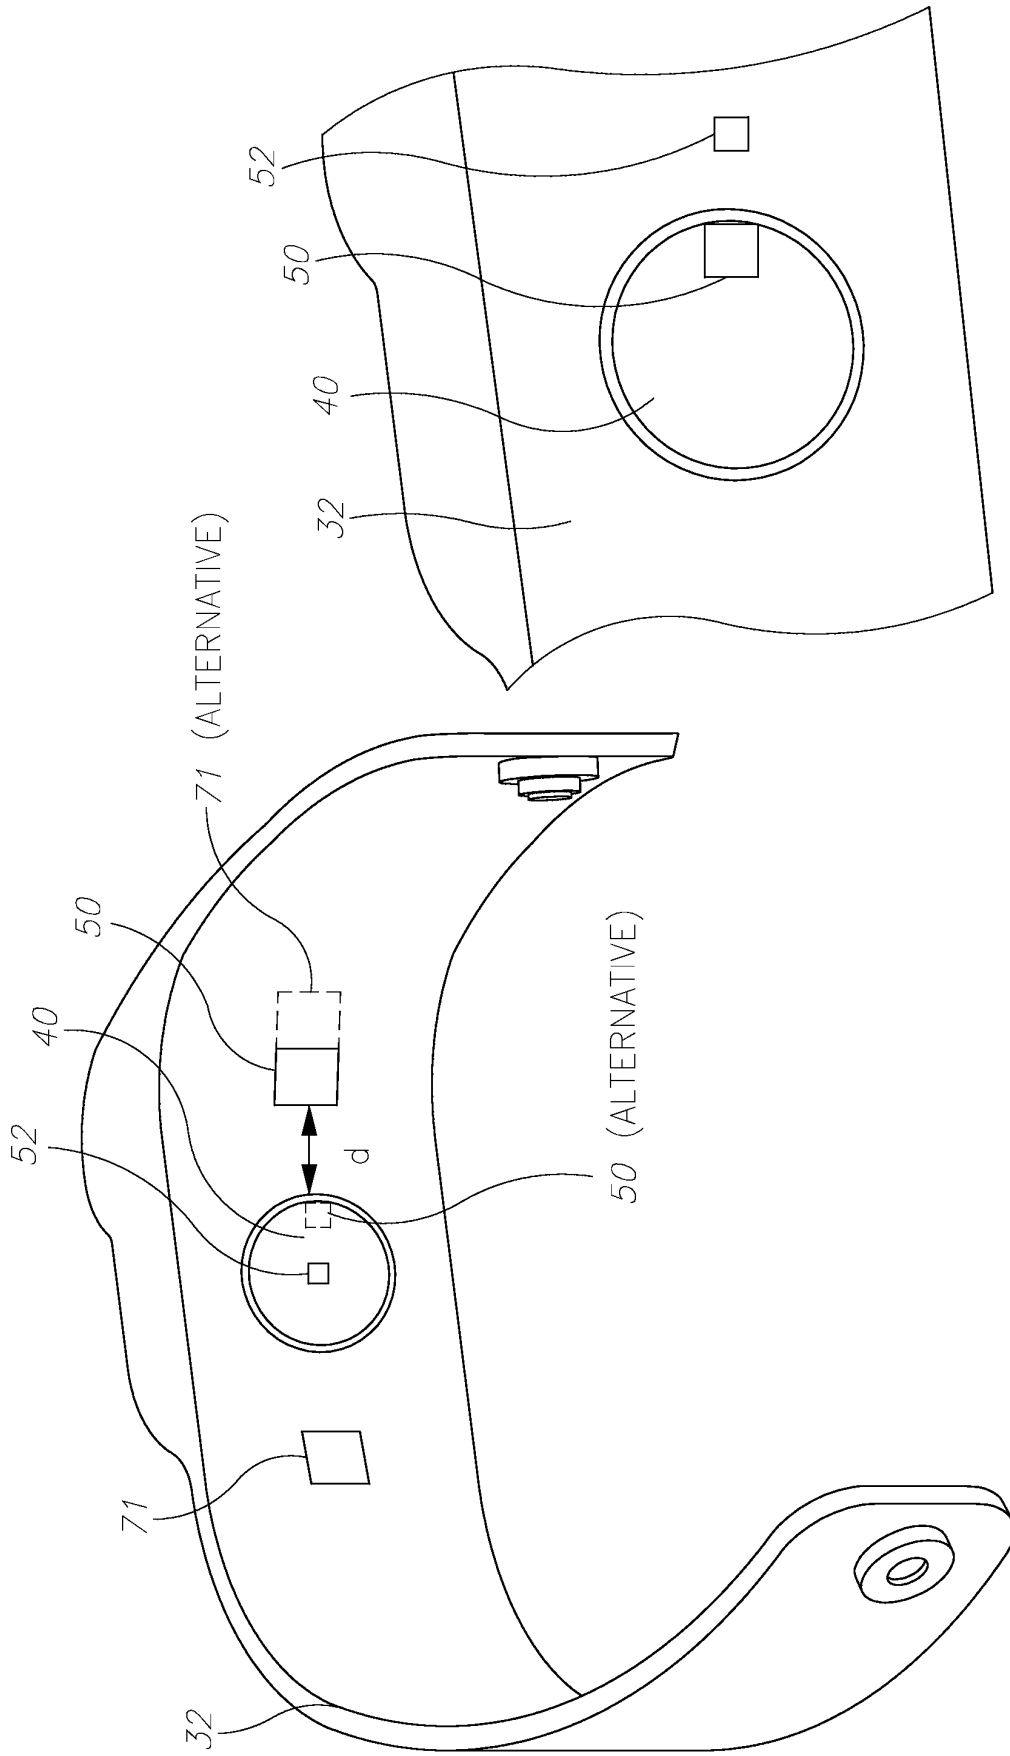


Figure 17A

Figure 17B

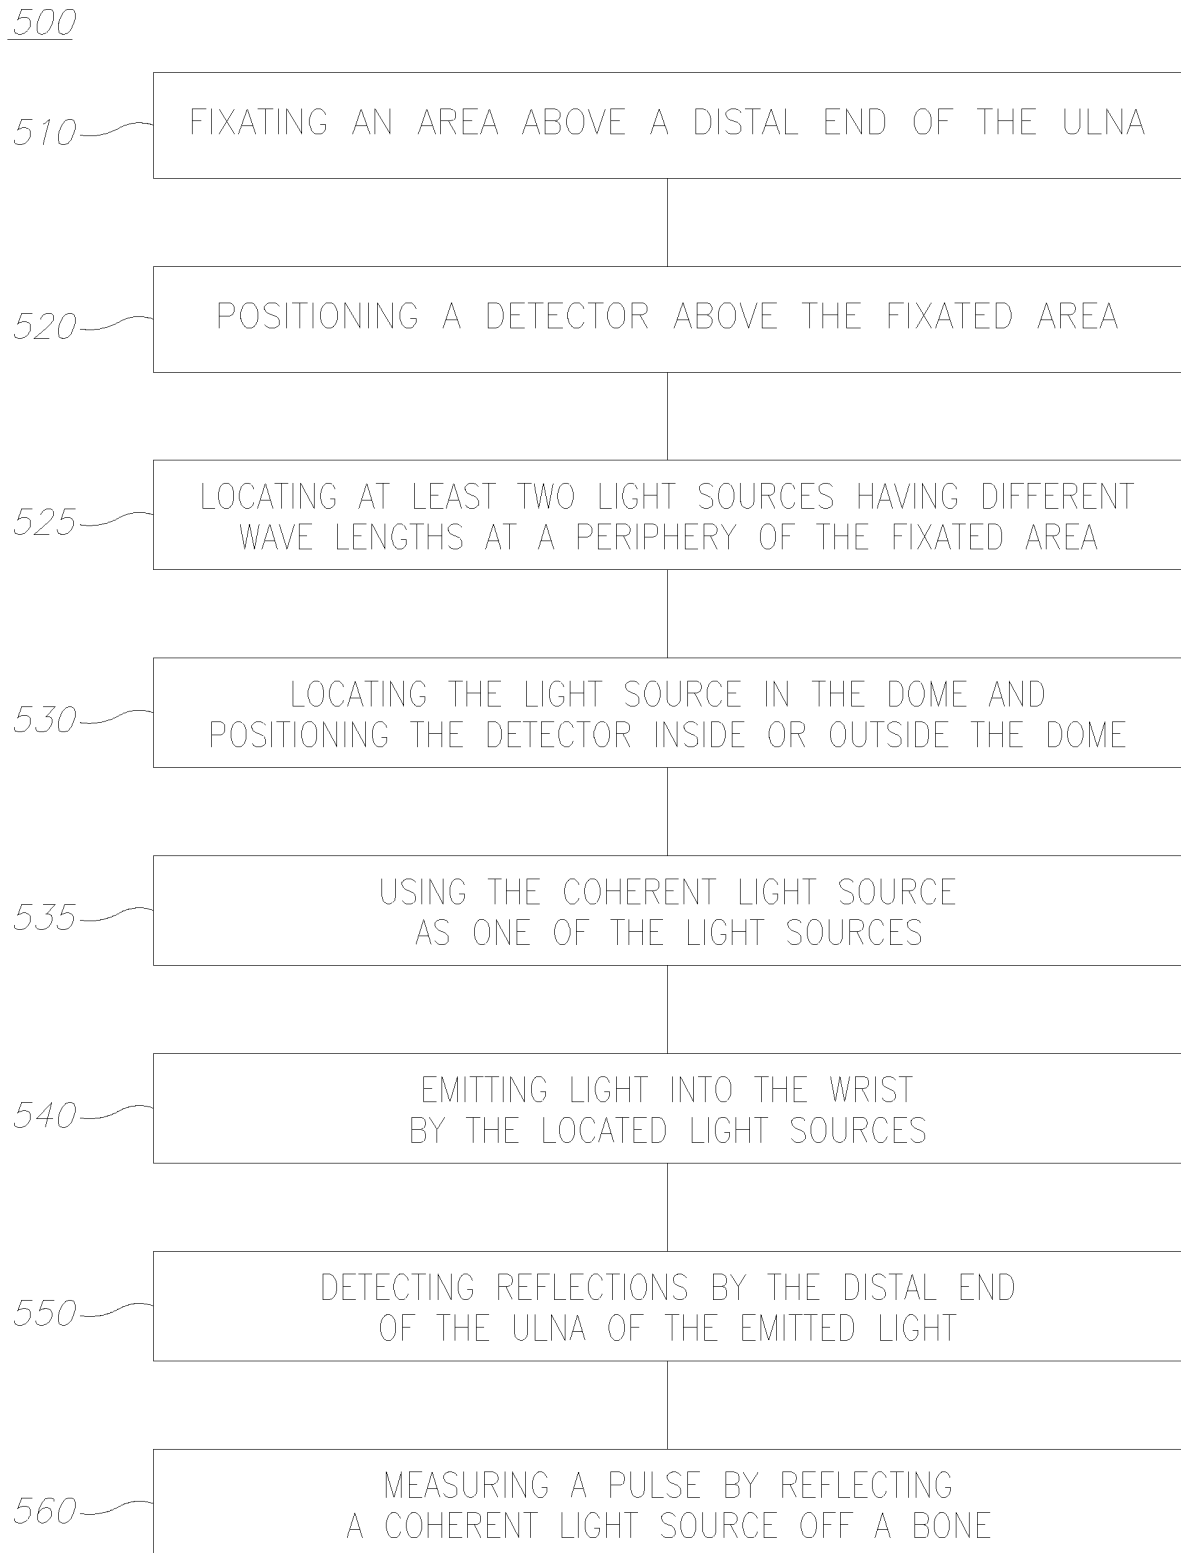


Figure 18

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2010056934 A [0009]
- US 2009247885 A [0009]
- US 2010331709 A [0009]
- US 2002188210 A [0009]
- US 6210340 B [0009]
- JP 2009160274 B [0009]
- JP 20052705443 B [0009]
- JP 2009254522 B [0009]
- JP 2010220939 B [0009]
- WO 2005040261 A [0009]
- WO 2010111127 A [0009]
- KR 20110006990 [0009]
- GB 2341233 A [0009]
- WO 2011013132 A [0009] [0018]
- WO 2006089763 A [0009]
- US 20110082355 A [0034]

专利名称(译)	可穿戴式脉搏血氧仪		
公开(公告)号	EP2750604A4	公开(公告)日	2015-04-22
申请号	EP2012827666	申请日	2012-08-26
[标]申请(专利权)人(译)	奥希顿医疗有限公司		
申请(专利权)人(译)	OXITONE MEDICAL LTD.		
当前申请(专利权)人(译)	OXITONE MEDICAL LTD.		
[标]发明人	EISEN LEON FINE ILYA GOLDINOV LEONID		
发明人	EISEN, LEON FINE, ILYA GOLDINOV, LEONID		
IPC分类号	A61B5/145 A61B5/00		
CPC分类号	A61B5/14552 A61B5/02416 A61B5/02438 A61B5/14551 A61B5/681 A61B5/6824 A61B5/7278 A61B5/742		
优先权	61/528851 2011-08-30 US 2011014881 2011-08-30 GB		
其他公开文献	EP2750604B1 EP2750604A1		
外部链接	Espacenet		

摘要(译)

一种脉搏血氧测量装置，安装在腕带上并用圆顶形结构固定尺骨远端上方的区域。该区域用作测量区域。通过位于固定区域上方的检测器执行测量，该检测器检测由具有不同波长的光源发射的光，所述光源位于固定区域的周边。因此，反射既不在反射模式也不在透射模式下测量，而是与发射光成20°和160°之间的角度。这种称为透射照明的模式可以实现出色的信噪比，这是第一次能够连续可靠地测量手腕上的血氧测量数据。