

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
9 September 2005 (09.09.2005)

PCT

(10) International Publication Number
WO 2005/082455 A1

- (51) International Patent Classification⁷: A61N 5/00, H05B 33/08
- (21) International Application Number: PCT/US2005/006205
- (22) International Filing Date: 25 February 2005 (25.02.2005)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data: 10/788,243 25 February 2004 (25.02.2004) US
- (71) Applicant (for all designated States except US): **NELCOR PURITAN BENNETT INCORPORATED** [US/US]; 4280 Hacienda Drive, Pleasanton, California 94588 (US).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **CHEW, Bradford, B.** [US/US]; 805 Springbrook Drive, San Ramon, California 94583 (US). **PETERSEN, Ethan** [US/US]; 18968 Thornbury Avenue, Castro Valley, California 94546 (US). **SHEA, William** [US/US]; 4049 Findlay Way, Livermore, California 94550 (US).
- (74) Agents: **SLAYDEN, Bruce, W., II** et al.; Baker Botts L.L.P., 1500 San Jacinto Center, 98 San Jacinto Blvd., Austin, Texas 78701-4039 (US).


- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declaration under Rule 4.17:

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii)) for the following designations AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY,

[Continued on next page]

(54) Title: LED FORWARD VOLTAGE ESTIMATION IN PULSE OXIMETER

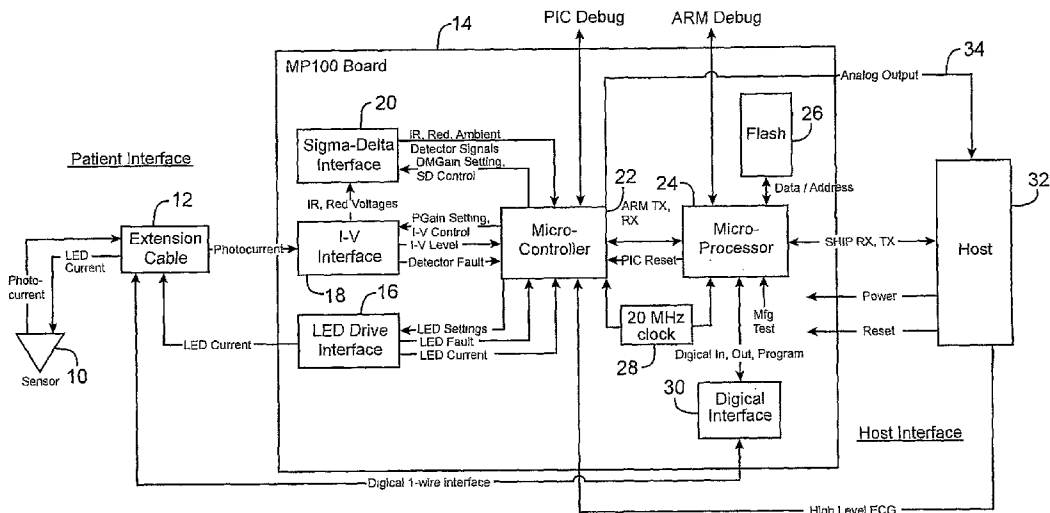

(57) Abstract: An apparatus and method for determining if a forward voltage of an LED in a pulse oximeter is within a predetermined range. This is accomplished by measuring the current through the LED, and also by knowing the duty cycle of the pulse width modulator (PWM) drive signal to the LED.

WO 2005/082455 A1



TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW, ARIPO patent (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG)

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— *with international search report*

LED FORWARD VOLTAGE ESTIMATION IN PULSE OXIMETER

BACKGROUND OF THE INVENTION

[0001] The present invention relates to oximeters, and in particular to controlling the LED voltage.

[0002] Pulse oximetry is typically used to measure various blood chemistry characteristics including, but not limited to, the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and the rate of blood pulsations corresponding to each heartbeat of a patient. Measurement of these characteristics has been accomplished by use of a non-invasive sensor which scatters light through a portion of the patient's tissue where blood perfuses the tissue, and photoelectrically senses the absorption of light in such tissue. The amount of light absorbed is then used to calculate the amount of blood constituent being measured.

[0003] The light scattered through the tissue is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of transmitted light scattered through the tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption. For measuring blood oxygen level, such sensors have typically been provided with a light source that is adapted to generate light of at least two different wavelengths, and with photodetectors sensitive to both of those wavelengths, in accordance with known techniques for measuring blood oxygen saturation.

[0004] Known non-invasive sensors include devices that are secured to a portion of the body, such as a finger, an ear or the scalp. In animals and humans, the tissue of these body portions is perfused with blood and the tissue surface is readily accessible to the sensor.

[0005] The light sources, typically light emitting diodes (LEDs), need to be driven with current to activate them. In order to determine sensor failure, such as an open or shorted LED, the current through the LED can be measured. Typically, this is done with a feedback resistor across which the voltage is measured to determine if any current is flowing. If no current is flowing, there is assumed to be an open connection.

BRIEF SUMMARY OF THE INVENTION

[0006] The present invention provides an apparatus and method for determining if a forward voltage of an LED in a pulse oximeter is within a predetermined range. This is accomplished by measuring the current through the LED, and also by knowing the duty cycle of the pulse width modulator (PWM) drive signal to the LED.

[0007] In one embodiment, the determination of the forward voltage being within a predetermined range is done within a processor, which provides an error signal if the forward voltage is outside the range. The error signal could indicate, for example, a short or open connection in the LED sensor.

[0008] In one embodiment, the processor includes a proportional integral (PI) loop which generates the PWM signal from an error signal corresponding to the difference between the actual current and desired current delivered to the LED.

[0009] For a further understanding of the nature and advantages of the present invention, reference should be made to the following description taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] Fig. 1 is a block diagram of an oximeter incorporating the present invention.

[0011] Fig. 2 is a circuit diagram of a LED drive circuit according to an embodiment of the present invention.

[0012] Figs. 3 and 4 are graphs illustrating the forward voltage versus current and PWM duty cycle versus power, respectively, for an LED in an embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

Oximeter Front-End

[0013] Fig. 1 illustrates an embodiment of an oximetry system incorporating the present invention. A sensor 10 includes red and infrared LEDs and a photodetector. These are connected by a cable 12 to a board 14. LED drive current is provided by an LED drive interface 16. The received photocurrent from the sensor is provided to an I-V interface 18. The IR and red voltages are then provided to a sigma-delta interface 20 incorporating the present invention. The output of sigma-delta interface 20 is provided to a microcontroller 22

which includes a 10-bit A/D converter. Microcontroller 22 includes flash memory for a program, and SRAM memory for data. The oximeter also includes a microprocessor 24 connected to a flash memory 26. Finally, a clock 28 is used and an interface 30 to a digital calibration in the sensor 10 is provided. A separate host 32 receives the processed information, as well as receiving an analog signal on a line 34 for providing an analog display.

LED Drive Circuit

[0014] Fig. 2 is a circuit diagram of the LED drive circuit according to an embodiment of the invention, which forms a portion of LED drive interface 16 of Fig. 1. A voltage regulator 36 provides a voltage separate from the voltage supply for the overall oximeter circuitry. The output is provided as a 4.5 volt signal on line 38, with the level being set by the feedback resistor divider of resistors R89 and R90. The voltage on line 38 is provided to a FET transistor Q11 to an inductor L6. The current through inductor L6 is provided by a switch 40 to one of capacitors C65 and C66, which store charge for the red and IR LEDs, respectively. A red/IR control signal on line 42 selects the switch position under control of the oximeter processor. A control signal LED PWM gate on line 44 controls the switching of transistor switch Q11.

[0015] Once the capacitors are charged up, the control signal on line 44 turns off switch Q11 and current is provided from either capacitor C65 or C66, through switch 40 and inductor L6 to either the red anode line 46 or the IR anode line 48 by way of transistors Q5 and Q6, respectively. A signal "red gate" turns on transistor Q5, while its inverse, "/red gate" turns off transistor Q7. This provides current through the red anode line 46 to the back LEDs 50, with the current returning through the IR anode to transistor Q8 and through resistor R10 to ground. Transistor Q8 is turned on by the signal "/IR gate" while the inverse of this signal, "IR gate" turns off transistor Q6. The signals are reversed when the IR anode is to be driven, with the "IR gate" and "red gate" signals, and their inverses, changing state, so that current is provided through transistor Q6 to IR anode 48 and returns through red anode 46 and through transistor Q7 to resistor R10 and ground. The "LED current sense" signal is read for calibration purposes not relevant to the present invention.

[0016] When the current from the capacitor C65 or C66 is provided through inductor L6 to the LEDs, and that current is switched off at the desired time, transistor Q11 is turned on so that the remaining current during the transition can be dumped into capacitor C64. This

addresses the fact that the FET transistor switching is not instantaneous. Subsequently, C64 will dump its current through Q11 and inductor L6 into the capacitors when they are recharged.

[0017] Resistor R38 and capacitor C67 are connected in parallel to inductor L6 to protect against signal spikes, and provide a smooth transition. Connected to inductor L6 is a sampling circuit with a switch 52 controlled by an LED sample hold signal on line 54 to sample the signals and provide them through an amplifier 56 to a "LED current" signal on line 58 which is read by the processor. An integrating capacitor C68 provides feedback for amplifier 56. A switch 60 responds to a "clear LED sample" signal to operate the switch to short out the capacitor between samples.

[0018] Operational amplifier 56 operates between 4.5 volts and ground. Thus, a voltage reference slightly above ground, of 0.2 volts, is provided as a voltage reference on pin 3.

[0019] The sample and hold circuit measures the voltage at node T18, between capacitor C69 and inductor L6, to determine the current. Capacitor C69 is 1/1000 of the value of capacitors C65 and C66. Thus, a proportional current is provided through C69, which is injected through switch 52 to integrating capacitor C68 to provide a voltage which can be measured at the output of amplifier 56 on line 58. The voltage measured by the processor on line 58 is used as a feedback, with the processor varying the width of the pulse delivered to transistor Q11 to selectively vary the amount of energy that's delivered to the capacitors 65 and 66, and then is eventually discharged to the LEDs 50. A PI (Proportional Integral) loop inside the processor then controls the PWM signal that controls Q11. This allows precise control of the LED intensity, allowing it to be maximized, if desired, without exceeding the desired limits.

[0020] The lower left of the diagram shows a "4.5 v LED disable" signal which is used by the microprocessor to turn off the voltage regulator 36 in certain instances. For example, diagnostics looking for shorts in a new sensor plugged in may turn off the voltage regulator if there is a problem with the LED line.

LED Voltage Determination

[0021] Figs. 3 and 4 illustrate the properties discovered by the present inventors which allowed development of the present invention. Fig. 3 is a graph of LED forward voltage versus LED current. The three different graphs produce three different lines with three

different slopes for different types of loads: an IR LED, a red LED and a functional tester (SRC) which has a diode and a resistor in series. As can be seen, measuring the current alone does not indicate what the LED forward voltage is unless one also knows the type of load, and has stored a curve such as that shown in Fig. 3.

[0022] Fig. 4 illustrates a plot of LED PWM duty cycle, which is the pulse width modulated drive signal for driving the LED. This is plotted on the vertical axis versus the power on a horizontal axis (LED voltage times LED current). As can be seen, for four different types of LED or SRC devices plotted, the plots are nearly identical with nearly identical slopes. From this recognition, the inventors determined that the voltage could be determined if one knows the PWM duty cycle and the current. The current is available from line 58 in Fig. 2, the LED current signal provided to the processor. The processor itself produces the PWM signal, and thus the processor has the two pieces of information needed to calculate the LED voltage for a particular LED, without knowing the type of LED. By using the information in Fig. 4, showing that the duty cycle is proportional by a constant to the power dissipated in the LED, a forward voltage can be derived.

[0023] In one embodiment, the PWM signal is generated using a PI (proportional integral) loop. This loop takes the formal equation set forth below:

$$y = Ae(t) + B \int e(t)dt$$

where:

A and B are constants

e = error signal, difference between desired and actual current

y = PWM signal

[0024] In one embodiment, a PWM duty cycle generated by the processor is provided to a lookup table which stores the data in the graph of Fig. 4. The lookup table will produce the power dissipated as an output. This value can then be divided by the LED current as provided on line 58. The result of the division will be the forward voltage of the LED.

[0025] Alternately, in another embodiment, a lookup table can be eliminated and a comparison can be done of the duty cycle and the current. Since the duty cycle is equal to the current times the voltage times a constant, upper and lower ranges for the ratio of duty cycle/LED current can be established to indicate conditions such as a short circuit or open connection in the LED. Alternately, a series of ranges could be used, with an outer range

indicating the short or open condition, and an inner range, in one example, indicating the desired operating range for the LED. For example, the oximeter may need to drive the LED harder, near its maximum current, for certain patients with weak pulse signals.

[0026] As will be understood by those with skill in the art, the present invention may be embodied in other specific forms without departing from the essential characteristics thereof. For example, the determination of forward voltage could be done entirely in hardware, rather than in software in a processor. Accordingly, the foregoing description is intended to be illustrative, but not limiting, of the scope of the invention which is set forth in the following claims.

WHAT IS CLAIMED IS:

1. A pulse oximeter comprising:
at least one light emitting diode (LED) drive circuit;
a current measuring circuit for measuring a current through said LED;
a controller for generating a pulse width modulator (PWM) drive signal to said LED; and
a processor, coupled to said controller and to said current measuring circuit, configured to determine if a forward voltage of said LED is within a predetermined range using a measurement of said current and said PWM signal.
2. The pulse oximeter of claim 1 wherein said processor is configured to provide an error signal if said forward voltage is outside said range.
3. The pulse oximeter of claim 1 wherein said processor is configured to compare said PWM drive signal to said measurement of said current to determine if the ratio is within an acceptable voltage range.
4. The pulse oximeter of claim 1 wherein said processor includes a proportional integral (PI) loop which generates said PWM signal from a current error signal reflecting a difference between said measurement of said current and a desired current.
5. A pulse oximeter comprising:
at least one light emitting diode (LED) drive circuit;
a current measuring circuit for measuring a current through said LED;
a controller for generating a pulse width modulator (PWM) drive signal to said LED;
a processor, coupled to said controller and to said current measuring circuit, configured to determine if a forward voltage of said LED is within a predetermined voltage range using a measurement of said current and said PWM signal, by comparing said PWM drive signal to said measurement of said current to determine if the ratio is within an acceptable voltage range;
wherein said processor is configured to provide an error signal if said forward voltage is outside said voltage range; and

wherein said processor includes a proportional integral (PI) loop which generates said PWM signal from a current error signal reflecting a difference between said measurement of said current and a desired current.

6. A method for operating a pulse oximeter comprising:
providing a current using at least one light emitting diode (LED) drive circuit;
measuring a current through said LED;
generating a pulse width modulator (PWM) drive signal to said LED; and
determining if a forward voltage of said LED is within a predetermined range using a measurement of said current and said PWM signal.

7. The method of claim 6 further comprising providing an error signal if said forward voltage is outside said range.

8. The method of claim 6 further comprising comparing said PWM drive signal to said measurement of said current to determine if the ratio is within an acceptable voltage range.

9. The method of claim 6 further comprising using a proportional integral (PI) loop to generate said PWM signal from a current error signal reflecting a difference between said measurement of said current and a desired current.

10. A method for operating a pulse oximeter comprising:
providing a current using at least one light emitting diode (LED) drive circuit;
measuring a current through said LED;
generating a pulse width modulator (PWM) drive signal to said LED;
determining if a forward voltage of said LED is within a predetermined voltage range using a measurement of said current and said PWM signal, by comparing said PWM drive signal to said measurement of said current to determine if the ratio is within an acceptable voltage range;

providing an error signal if said forward voltage is outside said voltage range;
and

using a proportional integral (PI) loop to generate said PWM signal from a current error signal reflecting a difference between said measurement of said current and a desired current.

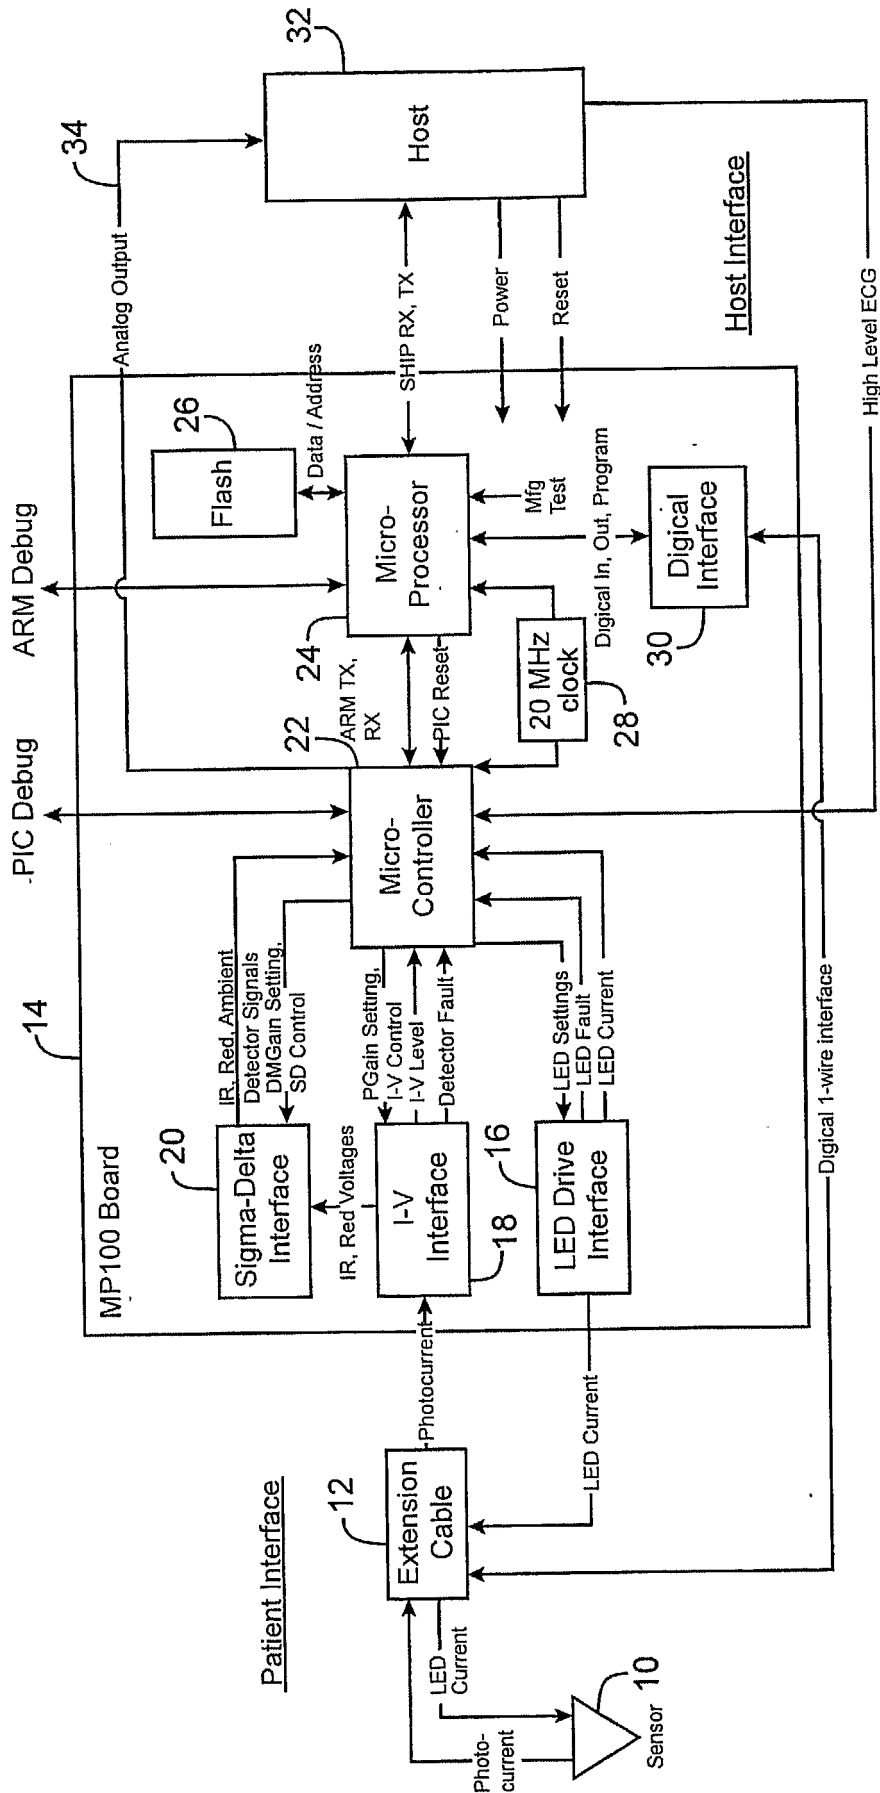


FIG. 1

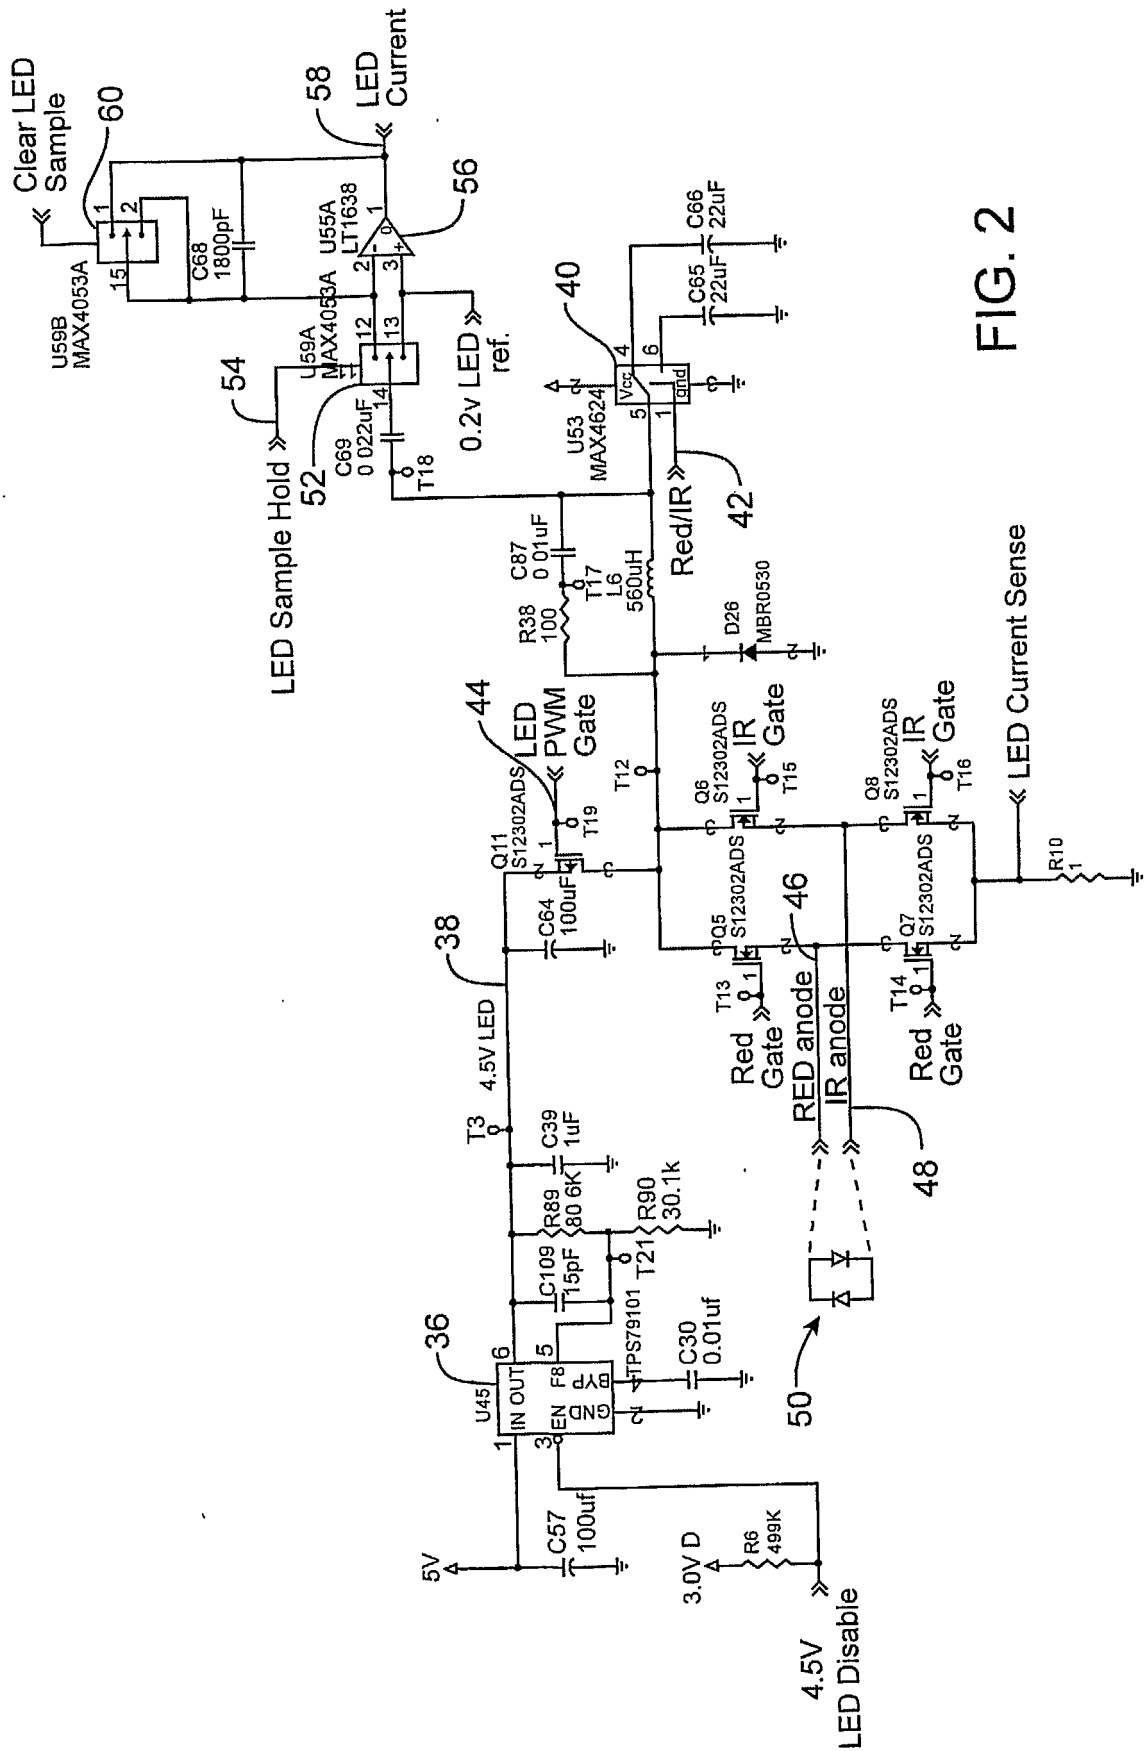


FIG. 2

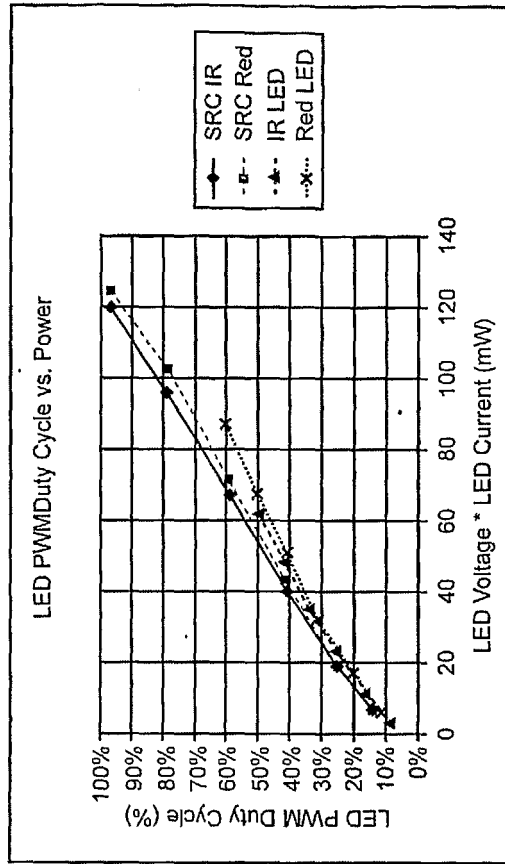


FIG. 4

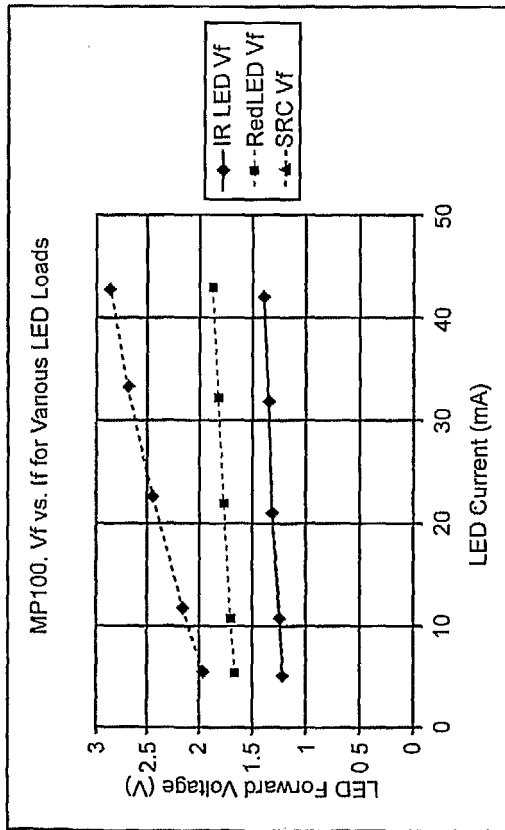


FIG. 3

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US2005/006205

A. CLASSIFICATION OF SUBJECT MATTER IPC 7 A61N5/00 H05B33/08				
According to International Patent Classification (IPC) or to both national classification and IPC				
B. FIELDS SEARCHED				
Minimum documentation searched (classification system followed by classification symbols) IPC 7 A61B H05B				
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched				
Electronic data base consulted during the international search (name of data base and, where practical, search terms used) EPO-Internal, WPI Data, PAJ				
C. DOCUMENTS CONSIDERED TO BE RELEVANT				
Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.		
X	EP 0 477 417 A (HEWLETT-PACKARD GMBH) 1 April 1992 (1992-04-01) page 3, line 3 - line 34; figures 1,2 page 4, line 2 - line 55 page 5, line 44 - line 7, paragraph 47 -----	1-10		
X	WO 03/068060 A (DATEX-OHMEDA, INC; HUIKU, MATTI) 21 August 2003 (2003-08-21) page 1, line 15 - page 2, line 7; figures 1,2,12 page 8, line 1 - page 9, line 8 page 14, line 26 - page 15, line 25 page 19, line 1 - line 29 page 21, line 1 - page 22, line 26 page 31, line 16 - line 17 ----- -/--	1-10		
<table style="width: 100%; border: none;"> <tr> <td style="width: 50%; border: none;"> <input checked="" type="checkbox"/> Further documents are listed in the continuation of box C. </td> <td style="width: 50%; border: none;"> <input checked="" type="checkbox"/> Patent family members are listed in annex. </td> </tr> </table>			<input checked="" type="checkbox"/> Further documents are listed in the continuation of box C.	<input checked="" type="checkbox"/> Patent family members are listed in annex.
<input checked="" type="checkbox"/> Further documents are listed in the continuation of box C.	<input checked="" type="checkbox"/> Patent family members are listed in annex.			
° Special categories of cited documents :				
A document defining the general state of the art which is not considered to be of particular relevance *E* earlier document but published on or after the international filing date *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) *O* document referring to an oral disclosure, use, exhibition or other means *P* document published prior to the international filing date but later than the priority date claimed	*T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art. *&* document member of the same patent family			
Date of the actual completion of the international search - 3 June 2005	Date of mailing of the international search report 10/06/2005			
Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Authorized officer Neef, T			

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US2005/006205

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61N5/00 H05B33/08

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61B H05B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 0 477 417 A (HEWLETT-PACKARD GMBH) 1 April 1992 (1992-04-01) page 3, line 3 - line 34; figures 1,2 page 4, line 2 - line 55 page 5, line 44 - line 7, paragraph 47	1-10
X	WO 03/068060 A (DATEX-OHMEDA, INC; HUIKU, MATTI) 21 August 2003 (2003-08-21) page 1, line 15 - page 2, line 7; figures 1,2,12 page 8, line 1 - page 9, line 8 page 14, line 26 - page 15, line 25 page 19, line 1 - line 29 page 21, line 1 - page 22, line 26 page 31, line 16 - line 17 ----- -/--	1-10

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *&* document member of the same patent family

Date of the actual completion of the international search

Date of mailing of the international search report

- 3 June 2005

10/06/2005

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Neef, T

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US2005/006205

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6 560 470 B1 (POLOGE JONAS A) 6 May 2003 (2003-05-06) column 1, line 50 - column 3, line 8; figures 1,2 column 3, line 25 - line 65 column 5, line 66 - column 6, line 25 -----	1-10
A	US 5 859 658 A (HAMMOND ET AL) 12 January 1999 (1999-01-12) column 2, line 21 - line 67 column 5, line 7 - column 7, line 47 -----	1,5,6,10
A	US 6 356 774 B1 (BERNSTEIN MICHAEL J ET AL) 12 March 2002 (2002-03-12) column 1, line 16 - line 60; figures 3,8-12 column 2, line 59 - column 3, line 45 column 4, line 48 - column 5, line 44 column 11, line 10 - column 13, line 41 column 17, line 27 - line 45 -----	1-10

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US2005/006205

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 0477417	A	01-04-1992	EP 0477417 A1	01-04-1992
			JP 4256733 A	11-09-1992
			US 5522389 A	04-06-1996

WO 03068060	A	21-08-2003	US 2003176776 A1	18-09-2003
			AU 2003202603 A1	04-09-2003
			EP 1474036 A1	10-11-2004
			WO 03068060 A1	21-08-2003

US 6560470	B1	06-05-2003	WO 02051299 A2	04-07-2002

US 5859658	A	12-01-1999	JP 9123518 A	13-05-1997

US 6356774	B1	12-03-2002	AU 758458 B2	20-03-2003
			AU 6271799 A	17-04-2000
			CA 2345731 A1	06-04-2000
			EP 1117326 A1	25-07-2001
			JP 2002525151 T	13-08-2002
			WO 0018290 A1	06-04-2000

专利名称(译)	脉冲血氧仪中的LED正向电压估计		
公开(公告)号	EP1722854A1	公开(公告)日	2006-11-22
申请号	EP2005723884	申请日	2005-02-25
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT INCORPORATED		
当前申请(专利权)人(译)	NELLCOR PURITAN BENNETT INCORPORATED		
[标]发明人	CHEW BRADFORD B PETERSEN ETHAN SHEA WILLIAM		
发明人	CHEW, BRADFORD, B. PETERSEN, ETHAN SHEA, WILLIAM		
IPC分类号	A61N5/00 H05B33/08 A61B5/00 A61B5/024		
CPC分类号	A61B5/14546 A61B5/02427 A61B5/14552 A61B5/1495		
代理机构(译)	GRUBERT , ANDREAS		
优先权	10/788243 2004-02-25 US		
外部链接	Espacenet		

摘要(译)

一种用于确定脉冲血氧计中的LED的正向电压是否在预定范围内的装置和方法。这是通过测量通过LED的电流，以及通过知道脉冲宽度调制器（PWM）驱动信号到LED的占空比来实现的。