

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
29 September 2005 (29.09.2005)

PCT

(10) International Publication Number
WO 2005/089648 A1

(51) International Patent Classification⁷: **A61B 5/11**,
A61N 1/365

(US). MIESEL, Keith, A. [US/US]; 896 Ashland Avenue,
St. Paul, MN 55104 (US).

(21) International Application Number:
PCT/US2005/008800

(74) Agents: CAMPBELL, Keith, M. et al.; MS LC340, 710
Medtronic Parkway, Minneapolis, MN 55432 (US).

(22) International Filing Date: 16 March 2005 (16.03.2005)

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD,
MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG,
PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA,
ZM, ZW.

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/553,778 16 March 2004 (16.03.2004) US
10/825,965 15 April 2004 (15.04.2004) US

(71) Applicant (for all designated States except US):
MEDTRONIC, INC. [US/US]; MS LC340, 710
Medtronic Parkway, Minneapolis, MN 55432 (US).


(72) Inventors; and

(75) Inventors/Applicants (for US only): HERUTH, Ken-
neth, T. [US/US]; 4904 Bruce Avenue, Edina, MN 55424

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),

[Continued on next page]

(54) Title: COLLECTING ACTIVITY INFORMATION TO EVALUATE THERAPY

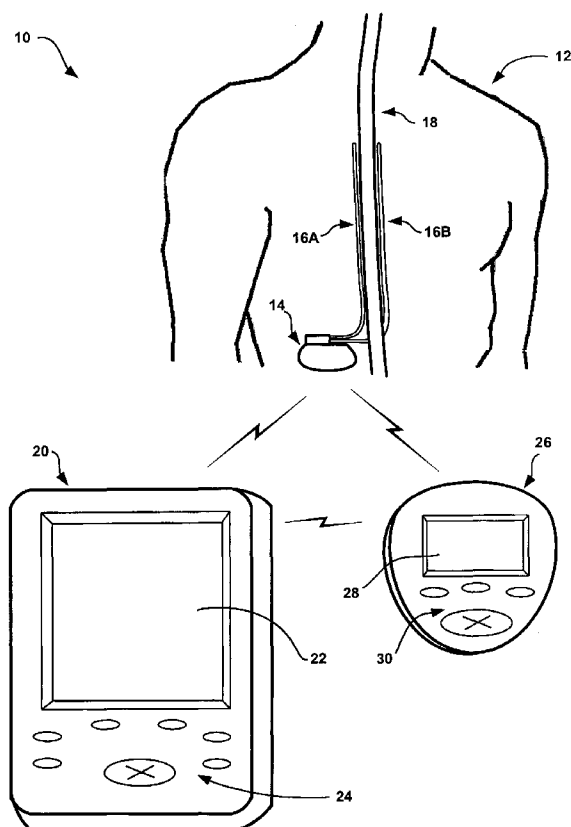

(57) Abstract: A medical device delivers a therapy to a patient. The medical device or another device may periodically determine an activity level of the patient, and associate each determined activity level with a current therapy parameter set. A value of at least one activity metric is determined for each of a plurality of therapy parameter sets based on the activity levels associated with that therapy parameter set. A list of the therapy parameter sets is presented to a user, such as a clinician, for evaluation of the relative efficacy of the therapy parameter sets. The list may be ordered according to the one or more activity metric values to aid in evaluation of the therapy parameter sets. Where values are determined for a plurality of activity metrics, the list may be ordered according to the one of the activity metrics selected by the user.

WO 2005/089648 A1



European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii)) for the following designations AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW, ARIPO patent (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT,

BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG)

- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii)) for all designations
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii)) for all designations

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

COLLECTING ACTIVITY INFORMATION TO EVALUATE THERAPY

TECHNICAL FIELD

The invention relates to medical devices and, more particularly, to medical devices that deliver therapy.

BACKGROUND

In some cases, an ailment may affect a patient's activity level or range of activities by preventing the patient from being active. For example, chronic pain may cause a patient to avoid particular physical activities, or physical activity in general, where such activities increase the pain experienced by the patient. Other ailments that may affect patient activity include movement disorders and congestive heart failure.

In some cases, these ailments are treated via a medical device, such as an implantable medical device (IMD). For example, patients may receive an implantable neurostimulator or drug delivery device to treat chronic pain or a movement disorder. Congestive heart failure may be treated by, for example, a cardiac pacemaker.

SUMMARY

In general, the invention is directed to techniques for evaluating a therapy delivered to a patient by a medical device based on patient activity. At any given time, the medical device delivers the therapy according to a current set of therapy parameters. The therapy parameters may change over time such that the therapy is delivered according to a plurality of different therapy parameter sets. The medical device, or another device, periodically determines an activity level of the patient, and associates each determined activity level with the current therapy parameter set. A value of at least one activity metric is determined for each of the therapy parameter sets based on the activity levels associated with that parameter set. A list of the therapy parameter sets and associated activity metrics is presented to a user, such as a clinician, for evaluation of the relative efficacy of the therapy parameter sets. The list may be ordered according to the activity metric values to

aid in evaluation of the therapy parameter sets. In this manner, the user may readily identify the therapy parameter sets that support the highest activity levels for the patient, and evaluate the relative efficacy of the parameter sets.

The therapy delivering medical device or another device may monitor at least one signal that is generated by a sensor and varies as a function of patient activity. For example, the device may monitor a signal generated by an accelerometer, a bonded piezoelectric crystal, a mercury switch, or a gyro. In some embodiments, the device may monitor a signal that indicates a physiological parameter of the patient, which in turn varies as a function of patient activity. For example, the device may monitor a signal that indicates the heart rate, electrocardiogram (ECG) morphology, respiration rate, respiratory volume, core temperature, subcutaneous temperature, or muscular activity of the patient.

The therapy delivering medical device or another device may periodically determine an activity level of the patient based on the one or more signals. In some embodiments, the device periodically determines a number of activity counts based on the signals, and the number of activity counts is stored as the activity level. The number of activity counts may be a number of threshold crossings by a signal generated by a sensor such as an accelerometer or piezoelectric crystal during a sample period, or a number of switch contacts indicated by the signal generated by a sensor such as mercury switch during a sample period.

In some embodiments, the device may periodically determine a heart rate, measured value of one or more ECG morphological features, respiration rate, respiratory volume, core temperature, subcutaneous temperature, and/or muscular activity level of the patient based on one or more signals. The determined values of these parameters may be mean or median values. The device may compare a determined value of such a physiological parameter to one or more thresholds to determine a number of activity counts, which may be stored as a determined activity level. In other embodiments, the device may store the determined physiological parameter value as a determined activity level.

The use of activity counts, however, may allow the device to determine an activity level based on a plurality of signals. For example, the device may determine a first number of activity counts based on an accelerometer signal and a second number of

activity counts based on a heart rate determined at the time the accelerometer signal was sampled. The device may determine an activity level by calculating the sum or average, which may be a weighted sum or average, of first and second activity counts.

As mentioned above, the device may associate each determined activity level with a current set of therapy parameters and, for each of a plurality of therapy parameter sets used by the medical device over time, a value of one or more activity metrics is determined. An activity metric value may be, for example, a mean or median activity level, such as an average number of activity counts per unit time. In other embodiments, an activity metric value may be chosen from a predetermined scale of activity metric values based on comparison of a mean or median activity level to one or more threshold values. The scale may be numeric, such as activity metric values from 1-10, or qualitative, such as low, medium or high activity.

In some embodiments, each activity level associated with a therapy parameter set is compared with the one or more thresholds, and percentages of time above and/or below the thresholds are determined as one or more activity metric values for that therapy parameter set. In other embodiments, each activity level associated with a therapy parameter set is compared with a threshold, and an average length of time that consecutively determined activity levels remain above the threshold is determined as an activity metric value for that therapy parameter set. One or both of the medical device or another device, such as a programming device or other computing device, may determine the activity metric values as described herein.

The computing device or, in some external medical device embodiments, the medical device, presents a list of the plurality of parameter sets and associated activity metric values via a display. The computing device may order the list according to the activity metric values. Where values are determined for a plurality of activity metrics for each of the therapy parameter sets, the computing device may order the list according to the values of a user selected one of the activity metrics. The computing device may also present other activity information to a user, such as a trend diagram of activity over time, or a histogram or pie chart illustrating percentages of time that activity levels were within certain ranges. The computing device may generate such charts or diagrams using activity

levels associated with a particular one of the therapy parameter sets, or all of the determined activity levels.

In one embodiment, the invention is directed to a method in which a signal that varies as a function of patient activity is monitored, and an activity level of the patient is periodically determined based on the signal. Each of the determined activity levels is associated with a therapy parameter set currently used by a medical device to deliver therapy to the patient when the activity level is determined, and a value of an activity metric is determined for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets.

In another embodiment, the invention is directed to a medical system comprising a medical device that delivers a therapy to a patient and a processor. The processor monitors a signal that varies as a function of patient activity, periodically determines an activity level of the patient based on the signal, associates each of the determined activity levels with a therapy parameter set currently used by the medical device to deliver the therapy to the patient when the activity level is determined, and determines a value of an activity metric for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets.

In another embodiment, the invention is directed to a medical system comprising means for monitoring a signal that varies as a function of patient activity via a medical device that delivers a therapy to a patient, means for periodically determining an activity level of the patient based on the signal, means for associating each of the determined activity levels with a current therapy parameter set, means for determining a value of an activity metric for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets, and means for presenting a list of the plurality of therapy parameter sets and activity metric values associated with the therapy parameter sets.

In another embodiment, the invention is directed to a medical system comprising an implantable medical device and an external programming device including a display. The implantable medical device delivers a therapy to a patient, monitors a signal that varies as a function of patient activity, periodically determines an activity level of the patient based on the signal, and associates each of the determined activity levels with a

current therapy parameter set. The external programming device receives information identifying a plurality of therapy parameter sets and associated activity levels from the implantable medical device via telemetry, determines a value of an activity metric for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets, and presents a list of the plurality of therapy parameter sets and activity metric values associated with the therapy parameter sets via the display.

In another embodiment the invention is directed to a programming device comprising a telemetry circuit, a user interface including a display, and a processor. The processor receives information identifying a plurality of therapy parameter sets and associated activity levels from an implantable medical device via the telemetry circuit, determines a value of an activity metric for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets, and presents a list of the plurality of therapy parameter sets and activity metric values associated with the therapy parameter sets via the display.

In another embodiment, the invention is directed to a computer-readable medium comprising program instructions. The program instructions cause a programmable processor to receive information identifying a plurality of therapy parameter sets and associated activity levels from an implantable medical device, determine a value of an activity metric for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets, and present a list of the plurality of therapy parameter sets and activity metric values associated with the therapy parameter sets.

The invention is capable of providing one or more advantages. For example, a medical system according to the invention may provide a clinician with an objective indication of the efficacy different sets of therapy parameters. Further, by displaying therapy parameter sets and associated activity metric values in an ordered and, in some cases, sortable list, the medical system may allow the clinician to more easily compare the relative efficacies of a plurality of therapy parameter sets. The medical system may be particularly useful in the context of trial neurostimulation for treatment of chronic pain, where the patient is encouraged to try a plurality of therapy parameter sets to allow the patient and clinician to identify efficacious therapy parameter sets.

The details of one or more embodiments of the invention are set forth in the accompanying drawings and the description below. Other features, objects, and advantages of the invention will be apparent from the description and drawings, and from the claims.

BRIEF DESCRIPTION OF DRAWINGS

FIG. 1 is a conceptual diagram illustrating an example system that includes an implantable medical device that collects activity information according to the invention.

FIG. 2 is a block diagram further illustrating the example system and implantable medical device of FIG. 1.

FIG. 3 is a block diagram illustrating an example memory of the implantable medical device of FIG. 1.

FIG. 4 is a flow diagram illustrating an example method for collecting activity information that may be employed by an implantable medical device.

FIG. 5 is a block diagram illustrating an example clinician programmer.

FIG. 6 illustrates an example list of therapy parameter sets and associated activity metric values that may be presented by a clinician programmer.

FIG. 7 is a flow diagram illustrating an example method for displaying a list of therapy parameter sets and associated activity metric values that may be employed by a clinician programmer.

FIG. 8 is a conceptual diagram illustrating a monitor that monitors values of one or more physiological parameters of the patient.

DETAILED DESCRIPTION

FIG. 1 is a conceptual diagram illustrating an example system 10 that includes an implantable medical device (IMD) 14 that collects information relating to the activity of a patient 12. In the illustrated example system 10, IMD 14 takes the form of an implantable neurostimulator that delivers neurostimulation therapy in the form of electrical pulses to patient 12. However, the invention is not limited to implementation via an implantable neurostimulator. For example, in some embodiments of the invention, IMD 14 may take the form of an implantable pump or implantable cardiac rhythm management device, such

as a pacemaker, that collects activity information. Further, the invention is not limited to implementation via an IMD. In other words, any implantable or external device may collect activity information according to the invention.

In the illustrated example, IMD 14 delivers neurostimulation therapy to patient 12 via leads 16A and 16B (collectively "leads 16"). Leads 16 may, as shown in FIG. 1, be implanted proximate to the spinal cord 18 of patient 12, and IMD 14 may deliver spinal cord stimulation (SCS) therapy to patient 12 in order to, for example, reduce pain experienced by patient 12. However, the invention is not limited to the configuration of leads 16 shown in FIG. 1 or the delivery of SCS therapy. For example, one or more leads 16 may extend from IMD 14 to the brain (not shown) of patient 12, and IMD 14 may deliver deep brain stimulation (DBS) therapy to patient 12 to, for example, treat tremor or epilepsy. As further examples, one or more leads 16 may be implanted proximate to the pelvic nerves (not shown) or stomach (not shown), and IMD 14 may deliver neurostimulation therapy to treat incontinence, sexual dysfunction, or gastroparesis. IMD 14 delivers therapy according to a set of therapy parameters, i.e., a set of values for a number of parameters that define the therapy delivered according to that therapy parameter set. In embodiments where IMD 14 delivers neurostimulation therapy in the form of electrical pulses, the parameters for each therapy parameter set may include voltage or current pulse amplitudes, pulse widths, pulse rates, duration, duty cycle and the like. Further, each of leads 16 includes electrodes (not shown in FIG. 1), and a therapy parameter set may include information identifying which electrodes have been selected for delivery of pulses, and the polarities of the selected electrodes. Therapy parameter sets used by IMD 14 may include a number of parameter sets programmed by a clinician (not shown), and parameter sets representing adjustments made by patient 12 to these preprogrammed sets.

System 10 also includes a clinician programmer 20. The clinician may use clinician programmer 20 to program therapy for patient 12, e.g., specify a number of therapy parameter sets and provide the parameter sets to IMD 14. The clinician may also use clinician programmer 20 to retrieve information collected by IMD 14. The clinician may use clinician programmer 20 to communicate with IMD 14 both during initial

programming of IMD 14, and for collection of information and further programming during follow-up visits.

Clinician programmer 20 may, as shown in FIG. 1, be a handheld computing device. Clinician programmer 20 includes a display 22, such as a LCD or LED display, to display information to a user. Clinician programmer 20 may also include a keypad 24, which may be used by a user to interact with clinician programmer 20. In some embodiments, display 22 may be a touch screen display, and a user may interact with clinician programmer 20 via display 22. A user may also interact with clinician programmer 20 using peripheral pointing devices, such as a stylus or mouse. Keypad 24 may take the form of an alphanumeric keypad or a reduced set of keys associated with particular functions.

System 10 also includes a patient programmer 26, which also may, as shown in FIG. 1, be a handheld computing device. Patient 12 may use patient programmer 26 to control the delivery of therapy by IMD 14. For example, using patient programmer 26, patient 12 may select a current therapy parameter set from among the therapy parameter sets preprogrammed by the clinician, or may adjust one or more parameters of a preprogrammed therapy parameter set to arrive at the current therapy parameter set. Patient programmer 26 may include a display 28 and a keypad 30, to allow patient 12 to interact with patient programmer 26. In some embodiments, display 28 may be a touch screen display, and patient 12 may interact with patient programmer 26 via display 28. Patient 12 may also interact with patient programmer 26 using peripheral pointing devices, such as a stylus, mouse, or the like.

Clinician and patient programmers 20, 26 are not limited to the hand-held computer embodiments illustrated in FIG. 1. Programmers 20, 26 according to the invention may be any sort of computing device. For example, a programmer 20, 26 according to the invention may be a tablet-based computing device, a desktop computing device, or a workstation.

IMD 14, clinician programmer 20 and patient programmer 26 may, as shown in FIG. 1, communicate via wireless communication. Clinician programmer 20 and patient programmer 26 may, for example, communicate via wireless communication with IMD 14 using radio frequency (RF) or infrared telemetry techniques known in the art. Clinician

programmer 20 and patient programmer 26 may communicate with each other using any of a variety of local wireless communication techniques, such as RF communication according to the 802.11 or Bluetooth specification sets, infrared communication according to the IRDA specification set, or other standard or proprietary telemetry protocols.

Clinician programmer 20 and patient programmer 26 need not communicate wirelessly, however. For example, programmers 20 and 26 may communicate via a wired connection, such as via a serial communication cable, or via exchange of removable media, such as magnetic or optical disks, or memory cards or sticks. Further, clinician programmer 20 may communicate with one or both of IMD 14 and patient programmer 26 via remote telemetry techniques known in the art, communicating via a local area network (LAN), wide area network (WAN), public switched telephone network (PSTN), or cellular telephone network, for example.

As mentioned above, IMD 14 collects patient activity information. Specifically, as will be described in greater detail below, IMD 14 may periodically determine an activity level of patient 12 based on a signal that varies as a function of patient activity. IMD 14 may associate each determined activity level with the therapy parameter set that is currently active when the activity level is determined. An activity level may comprise, for example, a number of activity counts, or a value for a physiological parameter that reflects patient activity.

Over time, IMD 14 uses a plurality of therapy parameter sets to deliver the therapy to patient 12. A processor within IMD 14 or another device, such as one of programmers 20,26 or another computing device, determines a value of one or more activity metrics for each of the plurality of therapy parameter sets based on the activity levels associated with the therapy parameter sets. An activity metric value may be, for example, a mean or median activity level, such as an average number of activity counts per unit time. In other embodiments, an activity metric value may be chosen from a predetermined scale of activity metric values based on a comparison of a mean or median activity level to one or more threshold values. The scale may be numeric, such as activity metric values from 1-10, or qualitative, such as low, medium or high activity.

In some embodiments, each activity level associated with a therapy parameter set is compared with the one or more thresholds, and percentages of time above and/or below

the thresholds are determined as one or more activity metric values for that therapy parameter set. In other embodiments, each activity level associated with a therapy parameter set is compared with a threshold, and an average length of time that consecutively determined activity levels remain above the threshold is determined as an activity metric value for that therapy parameter set.

In some embodiments, a plurality of activity metric values are determined for each of the plurality of therapy parameter sets. In such embodiments, an overall activity metric value may be determined. For example, the plurality of individual activity metric values may be used as indices to identify an overall activity metric value from a look-up table. The overall activity metric may be selected from a predetermined scale of activity metric values, which may be numeric, such as activity metric values from 1-10, or qualitative, such as low, medium or high activity.

One or more of IMD 14, programmers 20, 26, or another computing device may determine the activity metric values as described herein. In some embodiments, IMD 14 determines and stores activity metric values for each of a plurality of therapy parameter sets, and provides information identifying the therapy parameter sets and the associated activity metric values to clinician programmer 20. In other embodiments, IMD 14 provides information identifying the therapy parameter sets and associated activity levels to clinician programmer 20, and clinician programmer 20 determines the activity metric values for each of the therapy parameter sets.

In either of these embodiments, clinician programmer 20 presents a list of the plurality of parameter sets and associated activity metric values to the clinician via display 22. Programmer 20 may order the list according to the activity metric values. Where values are determined for a plurality of activity metrics for each of the therapy parameter sets, programmer 20 may order the list according to the values of one of the activity metrics that is selected by the clinician. Programmer 20 may also present other activity information to the clinician, such as a trend diagram of activity over time, or a histogram or pie chart illustrating percentages of time that activity levels were within certain ranges. Programmer 20 may generate such charts or diagrams using activity levels associated with a particular one of the therapy parameter sets, or all of the activity levels determined by IMD 14.

However, the invention is not limited to embodiments that include programmer 20, or embodiments in which programmer 20 presents activity information to the clinician. For example, in some embodiments, programmer 26 presents activity information as described herein to one or both of the clinician and patient 12. Further, in some embodiments, an external medical device comprises a display. In such embodiments, the external medical device may both determine activity metric values for the plurality of therapy parameter sets, and present the list of therapy parameter sets and activity metric values. Additionally, in some embodiments, any type of computing device, e.g., personal computer, workstation, or server, may identify activity levels, determine activity metric values, and/or present a list to a patient or clinician.

Further, the invention is not limited to embodiments in which a medical device determines activity levels. For example, in some embodiments, IMD 14 may instead periodically record samples of one or more signals that vary as a function of patient activity, and associated the samples with a current therapy parameter set. In such embodiments, programmer 20 or 26, or another computing device, may receive information identifying a plurality of therapy parameter sets and the samples associated with the parameter sets, may determine activity levels based on the samples, and may determine one or more activity metric values for each of the therapy parameter sets based on the determined activity levels.

FIG. 2 is a block diagram further illustrating system 10. In particular, FIG. 2 illustrates an example configuration of IMD 14 and leads 16A and 16B. FIG. 2 also illustrates sensors 40A and 40B (collectively “sensors 40”) that generate signals that vary as a function of patient activity. As will be described in greater detail below, IMD 14 monitors the signals, and may periodically determine an activity level based on the signals.

IMD 14 may deliver neurostimulation therapy via electrodes 42A-D of lead 16A and electrodes 42E-H of lead 16B (collectively “electrodes 42”). Electrodes 42 may be ring electrodes. The configuration, type and number of electrodes 42 illustrated in FIG. 2 are merely exemplary. For example, leads 16A and 16B may each include eight electrodes 42, and the electrodes 42 need not be arranged linearly on each of leads 16A and 16B. Electrodes 42 are electrically coupled to a therapy delivery module 44 via leads 16A and 16B. Therapy delivery module 44 may, for example, include an output pulse generator

coupled to a power source such as a battery. Therapy delivery module 44 may deliver electrical pulses to patient 12 via at least some of electrodes 42 under the control of a processor 46, which controls therapy delivery module 44 to deliver neurostimulation therapy according to a current therapy parameter set. However, the invention is not limited to implantable neurostimulator embodiments or even to IMDs that deliver electrical stimulation. For example, in some embodiments a therapy delivery module 44 of an IMD may include a pump, circuitry to control the pump, and a reservoir to store a therapeutic agent for delivery via the pump.

Processor 46 may include a microprocessor, a controller, a digital signal processor (DSP), an application specific integrated circuit (ASIC), a field-programmable gate array (FPGA), discrete logic circuitry, or the like. Memory 48 may include any volatile, non-volatile, magnetic, optical, or electrical media, such as a random access memory (RAM), read-only memory (ROM), non-volatile RAM (NVRAM), electrically-erasable programmable ROM (EEPROM), flash memory, and the like. In some embodiments, memory 48 stores program instructions that, when executed by processor 46, cause IMD 14 and processor 46 to perform the functions attributed to them herein.

Each of sensors 40 generates a signal that varies as a function of patient activity. IMD 14 may include circuitry (not shown) that conditions the signals generated by sensors 40 such that they may be analyzed by processor 46. For example, IMD 14 may include one or more analog to digital converters to convert analog signals generated by sensors 40 into digital signals usable by processor 46, as well as suitable filter and amplifier circuitry. Although shown as including two sensors 40, system 10 may include any number of sensors.

Further, as illustrated in FIG. 2, sensors 40 may be included as part of IMD 14, or coupled to IMD 14 via leads 16. Sensors 40 may be coupled to IMD 14 via therapy leads 16A and 16B, or via other leads 16, such as lead 16C depicted in FIG. 2. In some embodiments, a sensor 40 located outside of IMD 14 may be in wireless communication with processor 46. Wireless communication between sensors 40 and IMD 14 may, as examples, include RF communication or communication via electrical signals conducted through the tissue and/or fluid of patient 12.

A sensor 40 may be, for example, an accelerometer, a bonded piezoelectric crystal, a mercury switch, or a gyro that generates a signal as a function of patient activity, e.g., body motion, footfalls or other impact events, and the like. Processor 46 may determine an activity level based on a signal generated by one of these types of sensors 40 by sampling the signal and determining a number of activity counts during the sample period. Processor 46 may then store the determined number of activity counts in memory 48 as an activity level.

For example, processor 46 may compare the sample of a signal generated by an accelerometer or piezoelectric crystal to one or more amplitude thresholds stored within memory 48. Processor 46 may identify each threshold crossing as an activity count. Where processor 46 compares the sample to multiple thresholds with varying amplitudes, processor 46 may identify crossing of higher amplitude thresholds as multiple activity counts. Using multiple thresholds to identify activity counts, processor 46 may be able to more accurately determine the extent of patient activity for both high impact, low frequency and low impact, high frequency activities. In embodiments in which a sensor 40 takes the form of a mercury switch, processor 46 may identify the number of switch contacts indicated during the sample period as the number of activity counts. In embodiments in which a sensor 40 comprises an accelerometer or piezoelectric crystal, IMD 14 may include a filter (not shown), or processor 46 may apply a digital filter, that passes a band from approximately 0.1 Hz to 10 Hz. The filter may reduce noise in the signal, and pass the portion of the signal that reflects patient activity.

In some embodiments, processor 46 may monitor a signal that indicates a physiological parameter of patient 12, which in turn varies as a function of patient activity. For example, processor 46 may monitor a signal that indicates the heart rate, ECG morphology, respiration rate, respiratory volume, core temperature, subcutaneous temperature, or muscular activity of the patient. In such embodiments, processor 46 may periodically determine the heart rate, measured value of one or more ECG morphological features, respiration rate, respiratory volume, core temperature, subcutaneous temperature, or muscular activity level of patient 12 based on the signal. The determined values of these parameters may be mean or median values.

Sensors 40 may include electrodes located on leads 16 or integrated as part of the housing of IMD 14 that generates an electrogram signal as a function of electrical activity of the heart of patient 12, and processor 46 may periodically determine the heart rate of patient 12 based on the electrogram signal. In other embodiments, a sensor 40 may include an acoustic sensor within IMD 14, a pressure sensor within the bloodstream or cerebrospinal fluid of patient 12, or a temperature sensor located within the bloodstream of patient 12. The signals generated by such sensors 40 may vary as a function of contraction of the heart of patient 12, and can be used by processor 46 to periodically determine the heart rate of patient 12.

In some embodiments, processor 46 may detect, and measure values for one or more ECG morphological features within an electrogram generated by electrodes as described above. ECG morphological features may vary in a manner that indicates the activity level of patient. For example, the amplitude of the ST segment of the ECG may increase with increased patient activity. Further, the amplitude of QRS complex or T-wave may increase, and the widths of the QRS complex and T-wave may decrease with increased patient activity. The QT interval and the latency of an evoked response may decrease with increased patient activity, and the amplitude of the evoked response may increase with increased patient activity.

In some embodiments, sensors 40 may include an electrode pair, including one electrode integrated with the housing of IMD 14 and one of electrodes 42, that generates a signal as a function of the thoracic impedance of patient 12, which varies as a function of respiration by patient 12. The electrodes of the pair may be located on opposite sides of the patient's thorax. For example, the electrode pair may include one of electrodes 42 located proximate to the spine of a patient for delivery of SCS therapy, and IMD 14 with an electrode integrated in its housing may be implanted in the abdomen of patient 12.

In other embodiments, sensors 40 may include a strain gauge, bonded piezoelectric element, or pressure sensor within the blood or cerebrospinal fluid that generates a signal that varies based on patient respiration. Processor 46 may monitor the signals generated by such sensors 40 to periodically determine a respiration rate and/or respiratory volume of patient 12. An electrogram generated by electrodes as discussed above may also be

modulated by patient respiration, and processor 46 may use the electrogram as an indirect representation of respiration rate.

In some embodiments, sensors 40 may include one or more electrodes that generate an electromyogram (EMG) signal as a function of muscle electrical activity. The amplitude and/or frequency of an EMG signal may vary based on the activity level of a patient. The electrodes may be, for example, located in the legs, abdomen, chest, back or buttocks of patient 12 to detect muscle activity associated with walking, running, or the like. The electrodes may be coupled to IMD 14 wirelessly or by leads 16 or, if IMD 14 is implanted in these locations, integrated with a housing of IMD 14.

However, bonded piezoelectric crystals located in these areas generate signals as a function of muscle contraction in addition to body motion, footfalls or other impact events. Consequently, use of bonded piezoelectric crystals to detect activity of patient 12 may be preferred in some embodiments in which it is desired to detect muscle activity in addition to body motion, footfalls, or other impact events. Bonded piezoelectric crystals may be coupled to IMD 14 wirelessly or via leads 16, or piezoelectric crystals may be bonded to the can of IMD 14 when the IMD is implanted in these areas, e.g., in the back, chest buttocks or abdomen of patient 12.

Further, sensors 40 may include any of a variety of known temperature sensors to generate a signal as a function of a core or subcutaneous temperature of patient 12. Core or subcutaneous temperature may vary as a function of the activity level of patient 12. Such temperature sensors may be incorporated within the housing of IMD 14, or coupled to IMD 14 wirelessly or via leads.

In some embodiments, processor 46 compares a determined value of such a physiological parameter to one or more thresholds or a look-up table stored in memory to determine a number of activity counts, and stores the determined number of activity counts in memory 48 as a determined activity level. In other embodiments, processor 46 may store the determined physiological parameter value as a determined activity level. The use of activity counts, however, may allow processor 46 to determine an activity level based on a plurality of signals generated by a plurality of sensors 40. For example, processor 46 may determine a first number of activity counts based on a sample of an accelerometer signal and a second number of activity counts based on a heart rate

determined from an electrogram signal at the time the accelerometer signal was sampled. Processor 46 may determine an activity level by calculating the sum or average, which may be a weighted sum or average, of first and second activity counts.

Processor 46 may record activity levels continuously or periodically, e.g., one sample every minute or continuously for ten minutes each hour. In some embodiments, processor 46 limits recording of activity levels to relevant time periods, i.e., when patient 12 is awake or likely to be awake, and therefore likely to be active. For example, patient may indicate via patient programmer 26 when patient is going to sleep or awake. Processor 46 may receive these indications via a telemetry circuit 50 of IMD 14, and may suspend or resume recording of activity levels based on the indications. In other embodiments, processor 46 may maintain a real-time clock, and may record activity levels based on the time of day indicated by the clock, e.g., processor 46 may limit activity level recording to daytime hours.

In some embodiments, processor 46 may monitor one or more physiological parameters of patient 12 via signals generated by sensors 40, and may determine when patient 12 is attempting to sleep or asleep based on the physiological parameters. For example, processor 46 may determine when patient 12 is attempting to sleep by receiving an indication from patient programmer 26, or by monitoring the posture of patient 12 to determine when patient 12 is recumbent. Sensors 40 may include a plurality of orthogonally arranged accelerometers, and processor 46 may monitor the DC components of the signals generated by the accelerometers to determine when patient is recumbent.

In other embodiments, processor 46 determines when patient 12 is attempting to fall asleep based on the level of melatonin in a bodily fluid. In such embodiments, a sensor 40 may take the form of a chemical sensor that is sensitive to the level of melatonin or a metabolite of melatonin in the bodily fluid, and estimate the time that patient 12 will attempt to fall asleep based on the detection. For example, processor 46 may compare the melatonin level or rate of change in the melatonin level to a threshold level stored in memory 48, and identify the time that threshold value is exceeded. Processor 46 may identify the time that patient 12 is attempting to fall asleep as the time that the threshold is exceeded, or some amount of time after the threshold is exceeded. Any of a variety of combinations or variations of the above-described techniques may be used to determine

when patient 12 is attempting to fall asleep, and a specific one or more techniques may be selected based on the sleeping and activity habits of a particular patient.

In order to determine whether patient 12 is asleep, processor 46 may monitor any one or more physiological parameters that discernibly change when patient 12 falls asleep, such as activity level, posture, heart rate, ECG morphology, respiration rate, respiratory volume, blood pressure, blood oxygen saturation, partial pressure of oxygen within blood, partial pressure of oxygen within cerebrospinal fluid, muscular activity and tone, core temperature, subcutaneous temperature, arterial blood flow, brain electrical activity, eye motion, and galvanic skin response. Processor 46 may additionally or alternatively monitor the variability of one or more of these physiological parameters, such as heart rate and respiration rate, which may discernible change when patient 12 is asleep. Further details regarding monitoring physiological parameters to identify when a patient is attempting to sleep and when the patient is asleep may be found in a commonly-assigned and co-pending U.S. Patent Application Serial No. 60/553,771 by Kenneth Heruth and Keith Miesel, entitled "DETECTING SLEEP," which was assigned Attorney Docket No. 1023-360US02 and filed 16 March 2004, and is incorporated herein by reference in its entirety.

In other embodiments, processor 46 may record activity levels in response to receiving an indication from patient 12 via patient programmer 26. For example, processor 46 may record activity levels during times when patient 12 believes the therapy delivered by IMD 14 is ineffective and/or the symptoms experienced by patient 12 have worsened. In this manner, processor 46 may limit data collection to periods in which more probative data is likely to be collected, and thereby conserve a battery and/or storage space within memory 48.

Further, as described above, the invention is not limited to embodiments in which IMD 14 determines activity levels. In some embodiments, processor 46 may periodically store samples of the signals generated by sensors 40 in memory 48, rather than activity levels, and may associate those samples with the current therapy parameter set.

FIG. 3 illustrates memory 48 of IMD 14 in greater detail. As shown in FIG. 3, memory 48 stores information describing a plurality of therapy parameter sets 60. Therapy parameter sets 60 may include parameter sets specified by a clinician using

clinician programmer 20. Therapy parameter sets 60 may also include parameter sets that are the result of patient 12 changing one or more parameters of one of the preprogrammed therapy parameter sets. For example, patient 12 may change parameters such as pulse amplitude, frequency or pulse width via patient programmer 26.

Memory 48 also stores the activity levels 62 determined by processor 46. When processor 46 determines an activity level as discussed above, processor 46 associates the determined activity level with the current one of therapy parameter sets 60, e.g., the one of therapy parameter sets 60 that processor 46 is currently using to control delivery of therapy by therapy module 44 to patient 12. For example, processor 46 may store determined activity levels 62 within memory 48 with an indication of the parameter sets 60 with which they are associated. In other embodiments, processor 46 stores samples (not shown) of signals generated by sensors 40 within memory 48 with an indication of the parameter sets 60 with which they are associated.

In some embodiments, processor 46 determines a value of one or more activity metrics for each of therapy parameter sets 60 based on the activity levels 62 associated with the parameter sets 60. Processor 46 may store the determined activity metric values 66 within memory 48 with an indication as to which of therapy parameter sets 60 the determined values are associated with. For example, processor 46 may determine a mean or median of activity levels associated with a therapy parameter set, and store the mean or median activity level as an activity metric value 66 for the therapy parameter set.

In embodiments in which activity levels 62 comprise activity counts, processor 46 may store, for example, an average number of activity counts per unit time as an activity metric value. An average number of activity counts over a some period substantially between ten and sixty minutes, for example, may provide a more accurate indication of activity than an average over shorter periods by ameliorating the effect of transient activities on an activity signal or physiological parameters. For example, rolling over in bed may briefly increase the amplitude of an activity signal and a heart rate, thereby confounding the activity analysis.

In other embodiments, processor 46 may compare a mean or median activity level to one or more threshold values 64, and may select an activity metric value from a predetermined scale of activity metric values based on the comparison. The scale may be

numeric, such as activity metric values from 1-10, or qualitative, such as low, medium or high activity. The scale of activity metric values may be, for example, stored as a look-up table within memory 48. Processor 46 stores the activity metric value 66 selected from the scale within memory 48.

In some embodiments, processor 46 compares each activity level 62 associated with a therapy parameter set 60 to one or more threshold values 64. Based on the comparison, processor 46 may determine percentages of time above and/or below the thresholds, or within threshold ranges. Processor 46 may store the one or more determined percentages within memory 48 as one or more activity metric values 66 for that therapy parameter set. In other embodiments, processor 46 compares each activity level 62 associated with a therapy parameter set 66 to a threshold values 64, and determines an average length of time that consecutively recorded activity levels 62 remained above the threshold as an activity metric value 66 for that therapy parameter set.

In some embodiments, processor 46 determines a plurality of activity metric values for each of the plurality of therapy parameter sets, and determines an overall activity metric value for a parameter set based on the values of the individual activity metrics for that parameter set. For example, processor 46 may use the plurality of individual activity metric values as indices to identify an overall activity metric value from a look-up table stored in memory 48. Processor 46 may select the overall metric value from a predetermined scale of activity metric values, which may be numeric, such as activity metric values from 1-10, or qualitative, such as low, medium or high activity.

As shown in FIG. 2, IMD 14 includes a telemetry circuit 50, and processor 46 communicates with programmers 20, 26 via telemetry circuit 50. In some embodiments, processor 46 provides information identifying therapy parameter sets 60 and activity metric values 66 associated with the parameter sets to programmer 20, and programmer 20 displays a list of therapy parameter sets 60 and associated activity metric values 66. In other embodiments, as will be described in greater detail below, processor 46 does not determine activity metric values 66. Instead, processor 46 provides activity levels 62 to programmer 20 via telemetry circuit 50, and programmer 20 determines activity metric values 66 for display to the clinician. Further, in other embodiments, processor 46 provides samples of signals generated by sensors 40 to programmer 20 via telemetry

circuit 50, and programmer 20 may both determine activity levels 62 and activity metric values 66 based on the samples. Some external medical device embodiments of the invention include a display, and a processor of such an external medical device may both determine activity metric values 66 and display a list of therapy parameter sets 60 and associated activity metric values 66 to a clinician.

FIG. 4 is a flow diagram illustrating an example method for collecting activity information that may be employed by IMD 14. IMD 14 monitors one or more activity signals (70). For example, IMD 14 may monitor a signal generated by an accelerometer or piezoelectric crystal, and/or a signal that indicates a physiological parameter that varies as a function of patient activity, such heart rate, ECG morphology, respiration rate, respiratory volume, core temperature, subcutaneous temperature, or muscle activity.

IMD 14 determines an activity level 62 (72). For example, IMD 14 may determine a number of activity counts based on the one or more signals, as described above. IMD 14 identifies the current therapy parameter set 60, and associates the determined activity level 62 with the current therapy parameter set 60 (74). For example, IMD 14 may store the determined activity level 62 in memory 48 with an indication of the current therapy parameter set 60. IMD 14 may then update one or more activity metric values 66 associated with the current therapy parameter set 60, as described above (76).

IMD 14 may periodically perform the example method illustrated in FIG. 4, e.g., may periodically monitor the activity signal (70), determine activity levels 62 (72), and associate the determined activity levels 62 with a current therapy parameter set 60 (74). As described above, IMD 14 may only perform the example method during daytime hours, or when patient is awake and not attempting to sleep, and/or only in response to an indication received from patient 12 via patient programmer 20. IMD 14 need not update activity metric values 66 each time an activity level 62 is determined. In some embodiments, for example, IMD 14 may store activity levels 62 within memory, and may determine the activity metric values 66 upon receiving a request for the values from clinician programmer 20.

Further, in some embodiments, as will be described in greater detail below, IMD 14 does not determine the activity metric values 66, but instead provides activity levels 62 to a computing device, such as clinician programmer 20 or patient programmer 26. In

such embodiments, the computing device determines the activity metric values 66 associated with each of the therapy parameter sets 60. Additionally, as described above, IMD 14 need not determine activity levels 62, but may instead store samples of the signals generated by sensors 40. In such embodiments, the computing device may determine both activity levels 62 and activity metric values 66 based on the samples.

FIG. 5 is a block diagram illustrating clinician programmer 20. A clinician may interact with a processor 80 via a user interface 82 in order to program therapy for patient 12, e.g., specify therapy parameter sets. Processor 80 may provide the specified therapy parameter sets to IMD 14 via telemetry circuit 84.

At another time, e.g., during a follow up visit, processor 80 may receive information identifying a plurality of therapy parameter sets 60 from IMD 14 via telemetry circuit 84, which may be stored in a memory 86. The therapy parameter sets 60 may include the originally specified parameter sets, and parameter sets resulting from manipulation of one or more therapy parameters by patient 12 using patient programmer 26. In some embodiments, processor 80 also receives activity metric values 66 associated with the therapy parameter sets 60, and stores the activity metric values in memory 86.

In other embodiments, processor 80 receives activity levels 62 associated with the therapy parameter sets 60, and determines values 66 of one or more activity metrics for each of the plurality of therapy parameter sets 60 using any of the techniques described above with reference to IMD 14 and FIGS. 2 and 3. Processor 80 may, for example, use threshold values 64 stored in memory 86 to determine activity metric values 66, as described above. In still other embodiments, processor 80 receives samples of activity signals from IMD 14, and determines activity levels 62 and activity metric values 66 based on signals using any of the techniques described above with reference to IMD 14 and FIGS. 2 and 3.

Upon receiving or determining activity metric values 66, processor 80 generates a list of the therapy parameter sets 60 and associated activity metric values 66, and presents the list to the clinician. User interface 82 may include display 22, and processor 80 may display the list via display 22. The list of therapy parameter sets 60 may be ordered according to the associated activity metric values 66. Where a plurality of activity metric values are associated with each of the parameter sets, the list may be ordered according to

the values of the activity metric selected by the clinician. Processor 80 may also present other activity information to a user, such as a trend diagram of activity over time, or a histogram, pie chart, or other illustration of percentages of time that activity levels 62 were within certain ranges. Processor 80 may generate such charts or diagrams using activity levels 62 associated with a particular one of the therapy parameter sets 66, or all of the activity levels 62 recorded by IMD 14.

User interface 82 may include display 22 and keypad 24, and may also include a touch screen or peripheral pointing devices as described above. Processor 80 may include a microprocessor, a controller, a DSP, an ASIC, an FPGA, discrete logic circuitry, or the like. Memory 86 may include program instructions that, when executed by processor 80, cause clinician programmer 20 to perform the functions ascribed to clinician programmer 20 herein. Memory 86 may include any volatile, non-volatile, fixed, removable, magnetic, optical, or electrical media, such as a RAM, ROM, CD-ROM, hard disk, removable magnetic disk, memory cards or sticks, NVRAM, EEPROM, flash memory, and the like.

FIG. 6 illustrates an example list 90 of therapy parameter sets and associated activity metric values 66 that may be presented by clinician programmer 20. Each row of example list 90 includes an identification of one of therapy parameter sets 60, the parameters of the therapy parameter set, and values 66 associated with the therapy parameter set for each of two illustrated activity metrics. Programmer 20 may order list 90 according to a user-selected one of the activity metrics.

The activity metrics illustrated in FIG. 6 are a percentage of time active, and an average number of activity counts per hour. IMD 14 or programmer 20 may determine the average number of activity counts per hour for one of the illustrated therapy parameter sets by identifying the total number of activity counts associated with the parameter set and the total amount of time that IMD 14 was using the parameter set. IMD 14 or programmer 20 may determine the percentage of time active for one of parameter sets 60 by comparing each activity level 62 associated with the parameter set to an “active” threshold, and determining the percentage of activity levels 62 above the threshold. As illustrated in FIG. 9, IMD 14 or programmer 20 may also compare each activity level for the therapy parameter set to an additional, “high activity” threshold, and determine a percentage of activity levels 62 above that threshold.

FIG. 7 is a flow diagram illustrating an example method for displaying a list of therapy parameter sets 60 and associated activity metric values 66 that may be employed by a clinician programmer 20. Programmer 20 receives information identifying therapy parameter sets 60 and associated activity levels 62 from IMD 14 (100). Programmer 20 then determines one or more activity metric values 66 for each of the therapy parameter sets based on the activity levels 62 associated with the therapy parameter sets (102). In other embodiments, IMD 14 determines the activity metric values 66, and provides them to programmer 20, or provides samples of activity signals associated with therapy parameter sets to programmer 20 for determination of activity metric values, as described above. After receiving or determining activity metric values 66, programmer 20 presents a list 90 of therapy parameter sets 60 and associated activity metric values 66 to the clinician, e.g., via display 22 (104). Programmer 20 may order list 90 of therapy parameter sets 60 according to the associated activity metric values 66, and the clinician may select which of a plurality of activity metrics list 90 is ordered according to via a user interface 82 (106).

Various embodiments of the invention have been described. However, one skilled in the art will recognize that various modifications may be made to the described embodiments without departing from the scope of the invention. For example, although described herein primarily in the context of treatment of pain with an implantable neurostimulator, the invention is not so limited. The invention may be embodied in any implantable medical device that delivers a therapy, such as a cardiac pacemaker or an implantable pump. Further, the invention may be implemented via an external, e.g., non-implantable, medical device.

Additionally, the invention is not limited to embodiments in which a programming device receives information from the medical device, or presents information to a user. Other computing devices, such as handheld computers, desktop computers, workstations, or servers may receive information from the medical device and present information to a user as described herein with reference to programmers 20, 26. A computing device, such as a server, may receive information from the medical device and present information to a user via a network, such as a local area network (LAN), wide area network (WAN), or the Internet. Further, in some embodiments, the medical device is an external medical device,

and may itself include user interface and display to present activity information to a user, such as a clinician or patient, for evaluation of therapy parameter sets.

As another example, the invention may be embodied in a trial neurostimulator, which is coupled to percutaneous leads implanted within the patient to determine whether the patient is a candidate for neurostimulation, and to evaluate prospective neurostimulation therapy parameter sets. Similarly, the invention may be embodied in a trial drug pump, which is coupled to a percutaneous catheter implanted within the patient to determine whether the patient is a candidate for an implantable pump, and to evaluate prospective therapeutic agent delivery parameter sets. Activity metric values collected during use of the trial neurostimulator or pump may be used by a clinician to evaluate the prospective therapy parameter sets, and select parameter sets for use by the later implanted non-trial neurostimulator or pump. For example, a trial neurostimulator or pump may determine values of one or more activity metrics for each of a plurality of prospective therapy parameter sets, and a clinician programmer may present a list of prospective parameter sets and associated activity metric values to a clinician. The clinician may use the list to identify potentially efficacious parameter sets, and may program a permanent implantable neurostimulator or pump for the patient with the identified parameter sets.

Additionally, the invention is not limited to embodiments in which the therapy delivering medical device monitors the physiological parameters of the patient described herein. In some embodiments, a separate monitoring device monitors values of one or more physiological parameters of the patient instead of, or in addition to, a therapy delivering medical device. The monitor may include a processor 46 and memory 48, and may be coupled to or include sensors 40, as illustrated above with reference to IMD 14 and FIGS. 2 and 3. The monitor may identify activity levels and activity metric values based on the values of the monitored physiological parameter values, or may transmit activity levels or the physiological parameter values to a computing device for determination of the activity metric values.

In embodiments in which the medical device determines activity levels or activity metric values, the medical device may identify the current therapy parameter set when a value of one or more sleep quality metrics is collected, and may associate that value with the therapy parameter set. In embodiments in which a programming device or other

computing device determines activity levels or activity metric values, the medical device may associate recorded physiological parameter values or activity levels with the current therapy parameter set in the memory. Further, in embodiments in which a separate monitoring device records physiological parameter values or determines activity levels or activity metric values, the monitoring device may mark recorded physiological parameter values, activity levels, or activity metric values with a current time in a memory, and the medical device may store an indication of a current therapy parameter set and time in a memory. A programming device or other computing device may receive indications of the physiological parameter values, activity levels, or activity metric values and associated times from the monitoring device, and indications of the therapy parameter sets and associated times from the medical device, and may associate the physiological parameter values, activity levels, or activity metric values with the therapy parameter set that was delivered by the medical device when the values or levels were recorded.

FIG. 8 is a conceptual diagram illustrating a monitor 110 that monitors values of one or more physiological parameters of the patient instead of, or in addition to, a therapy delivering medical device. In the illustrated example, monitor 110 is configured to be attached to or otherwise carried by a belt 112, and may thereby be worn by patient 12. FIG. 8 also illustrates various sensors 40 that may be coupled to monitor 110 by leads, wires, cables, or wireless connections, such as EEG electrodes 114A-C placed on the scalp of patient 12, a plurality of EOG electrodes 116A and 116B placed proximate to the eyes of patient 12, and one or more EMG electrodes 118 placed on the chin or jaw the patient. The number and positions of electrodes 114, 116 and 118 illustrated in FIG. 12 are merely exemplary. For example, although only three EEG electrodes 174 are illustrated in FIG. 1, an array of between 16 and 25 EEG electrodes 114 may be placed on the scalp of patient 12, as is known in the art. EEG electrodes 114 may be individually placed on patient 12, or integrated within a cap or hair net worn by the patient.

In the illustrated example, patient 12 wears an ECG belt 120. ECG belt 120 incorporates a plurality of electrodes for sensing the electrical activity of the heart of patient 12. The heart rate and, in some embodiments, ECG morphology of patient 12 may be monitored by monitor 110 based on the signal provided by ECG belt 120. Examples of suitable belts 120 for sensing the heart rate of patient 12 are the "M" and "F" heart rate

monitor models commercially available from Polar Electro. In some embodiments, instead of belt 120, patient 12 may wear of plurality of ECG electrodes attached, e.g., via adhesive patches, at various locations on the chest of the patient, as is known in the art. An ECG signal derived from the signals sensed by such an array of electrodes may enable both heart rate and ECG morphology monitoring, as is known in the art.

As shown in FIG. 8, patient 12 may also wear a respiration belt 122 that outputs a signal that varies as a function of respiration of the patient. Respiration belt 122 may be a plethysmography belt, and the signal output by respiration belt 122 may vary as a function of the changes in the thoracic or abdominal circumference of patient 12 that accompany breathing by the patient. An example of a suitable belt 122 is the TSD201 Respiratory Effort Transducer commercially available from Biopac Systems, Inc. Alternatively, respiration belt 122 may incorporate or be replaced by a plurality of electrodes that direct an electrical signal through the thorax of the patient, and circuitry to sense the impedance of the thorax, which varies as a function of respiration of the patient, based on the signal. In some embodiments, ECG and respiration belts 120 and 122 may be a common belt worn by patient 12, and the relative locations of belts 120 and 122 depicted in FIG. 8 are merely exemplary.

In the example illustrated by FIG. 8, patient 12 also wears a transducer 124 that outputs a signal as a function of the oxygen saturation of the blood of patient 12. Transducer 124 may be an infrared transducer. Transducer 124 may be located on one of the fingers or earlobes of patient 12. Sensors 40 coupled to monitor 110 may additionally or alternatively include or be coupled to any of the variety of sensors 40 described above with reference to FIG. 2 that output signals that vary as a function of patient activity, such as EMG electrodes, accelerometers, piezoelectric crystals, or pressure sensors.

Further, the invention may be embodied as a computer-readable medium that includes instructions to cause a processor to perform any of the methods described herein. These and other embodiments are within the scope of the following claims.

CLAIMS:

1. A medical system comprising:
 - means for monitoring a signal that varies as a function of activity of a patient;
 - means for periodically determining an activity level of the patient based on the signal;
 - means for associating each of the determined activity levels with a therapy parameter set currently used by a medical device to deliver a therapy to the patient when the activity level is determined; and
 - means for determining a value of an activity metric for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets.
2. The system of claim 1, wherein the signal comprises a signal generated by an accelerometer, the method further comprising filtering the signal to pass a band from approximately 0.1 Hz to approximately 10 Hz.
3. The system of claims 1 or 2, wherein the means for periodically determining an activity level comprises:
 - a means for determining when the patient is awake; and
 - a means for periodically determining an activity level while the patient is awake.
4. The system of any of claims 1 to 3, wherein the means for determining a value of an activity metric comprises a means for determining at least one of a mean and a median of activity levels associated with the therapy parameter set.
5. The system of any of claims 1 to 3, wherein the means for determining a value of an activity metric comprises:
 - a means for comparing the at least one of the mean and the median activity level to at least one threshold; and
 - a means for selecting the activity metric value from a plurality of predetermined possible activity metric values based on the comparison.

6. The system of any of claims 1 to 3, wherein the means for determining a value of an activity metric for a therapy parameter set comprises:
 - means for comparing each of the activity levels associated with the therapy parameter set to a threshold value; and
 - means for determining at least one of a percentage of time above the threshold and a percentage of time below the threshold.
7. The system of any of claims 1 to 3, wherein the means for determining a value of an activity metric for a therapy parameter set comprises:
 - means for comparing each of the activity levels associated with the therapy parameter set to a threshold value; and
 - means for determining an average length of time that consecutively determined activity levels associated with the therapy parameter set were above the threshold.
8. The system of any of claims 1 to 7, wherein the means for periodically determining an activity level comprises a means for periodically determining a number of activity counts.
9. The system of claim 8, wherein the means for determining an activity metric value for each of a plurality of therapy parameter sets comprises a means for determining an average number of activity counts per a unit of time for each of the plurality of therapy parameter sets based on the numbers of activity counts associated with the therapy parameter sets.
10. The system of claim 9, wherein the means for determining an average number of activity counts per a unit of time comprises a means for determining an average number of activity counts over a period of time substantially within a range from 10 to 60 minutes.

11. The system of any of claims 1 to 7, wherein the means for periodically determining an activity level comprises a means for periodically determining a value of at least one physiological parameter of the patient.
12. The system of claim 11, wherein the means for periodically determining a value of a physiological parameter comprises a means for periodically determining at least one of a heart rate, a value of an ECG morphological feature, a respiration rate, respiratory volume, a core temperature, subcutaneous temperature, and a muscular activity level.
13. The system of any of claims 1 to 12, further comprising a means for presenting a list of the plurality of therapy parameter sets and activity metric values associated with the therapy parameter sets.
14. The system of claim 13, further comprising a means for ordering the list of therapy parameter sets according to the associated activity metric values.
15. The system of claim 14, wherein determining the means for a value of an activity metric comprises a means for determining a value of each of a plurality of activity metrics for each of a plurality of therapy parameter sets based on activity levels associated with the therapy parameter sets, and a means for ordering the list comprises ordering the list according to a user selected one of the activity metrics.
16. The system of any of claims 1 to 15, wherein the means for determining a value of an activity metric comprises:
 - a means for determining a value of each of a plurality of activity metrics; and
 - a means for determining a value of an overall activity metric based on the plurality of activity metric values.
17. The system of any of claims 1 to 16, further comprising a means for presenting a graphical representation of the determined activity levels.

18. The system of claim 17, wherein the means for presenting a graphical representation comprises presenting at least one of a trend diagram, a histogram and a pie chart based on the determined activity levels.

19. The system of any of claims 1 to 18, wherein the medical device comprises an implantable medical device.

20. The system of claim 19, wherein the implantable medical device comprises at least one of an implantable neurostimulator and an implantable drug pump.

The system of any of claims 1 to 18, wherein the medical device comprises a trial neurostimulator.

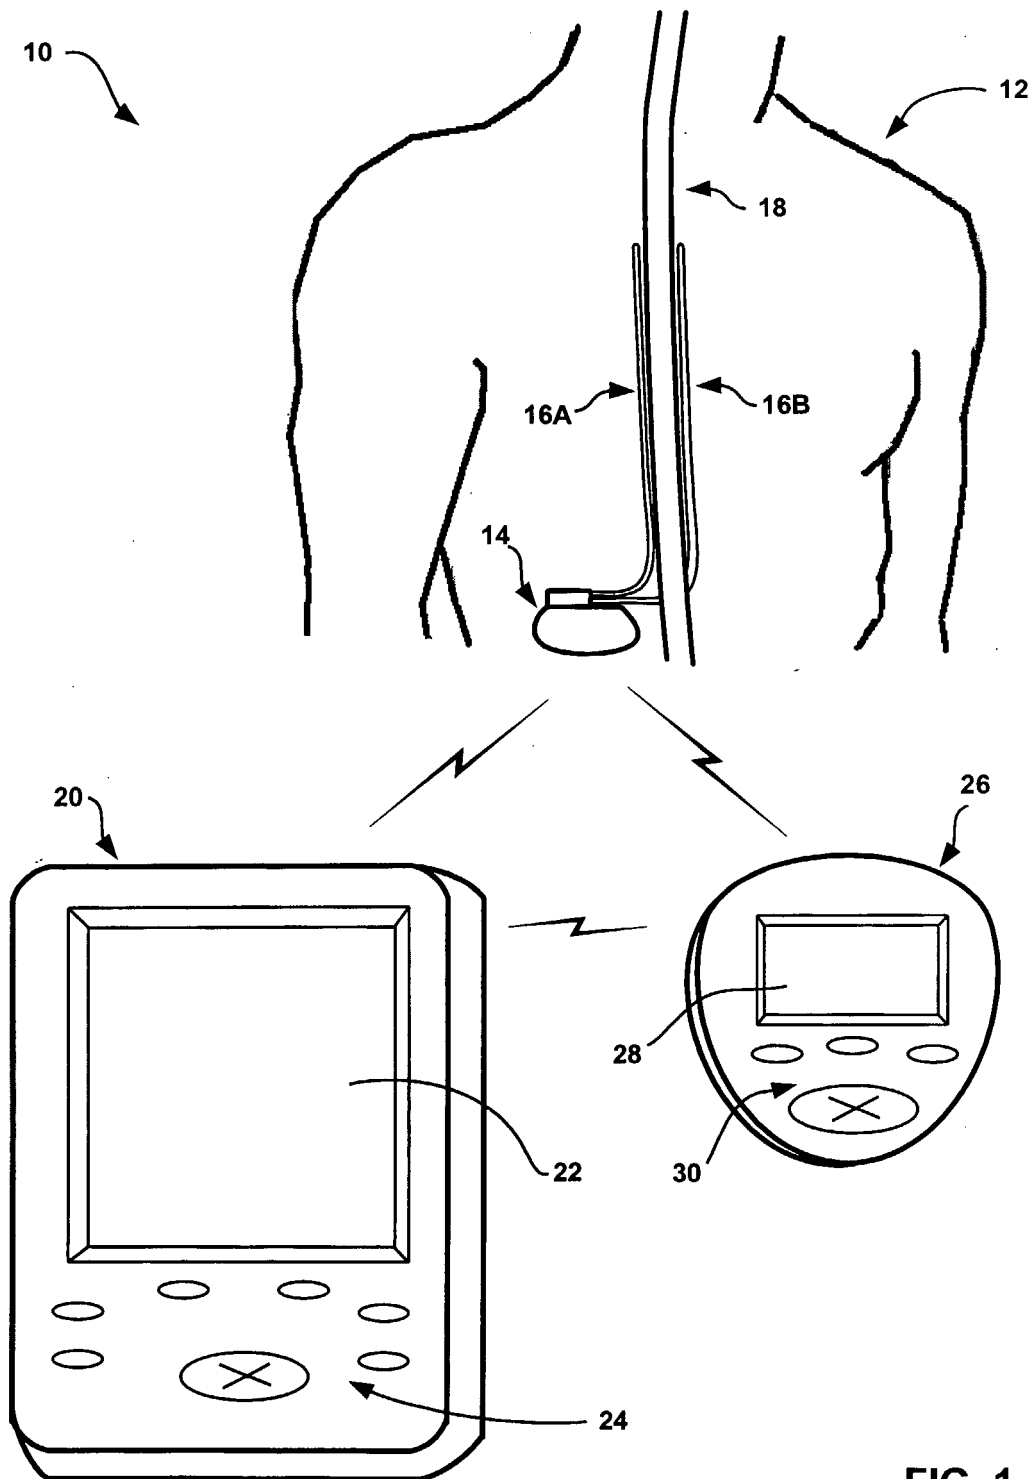


FIG. 1

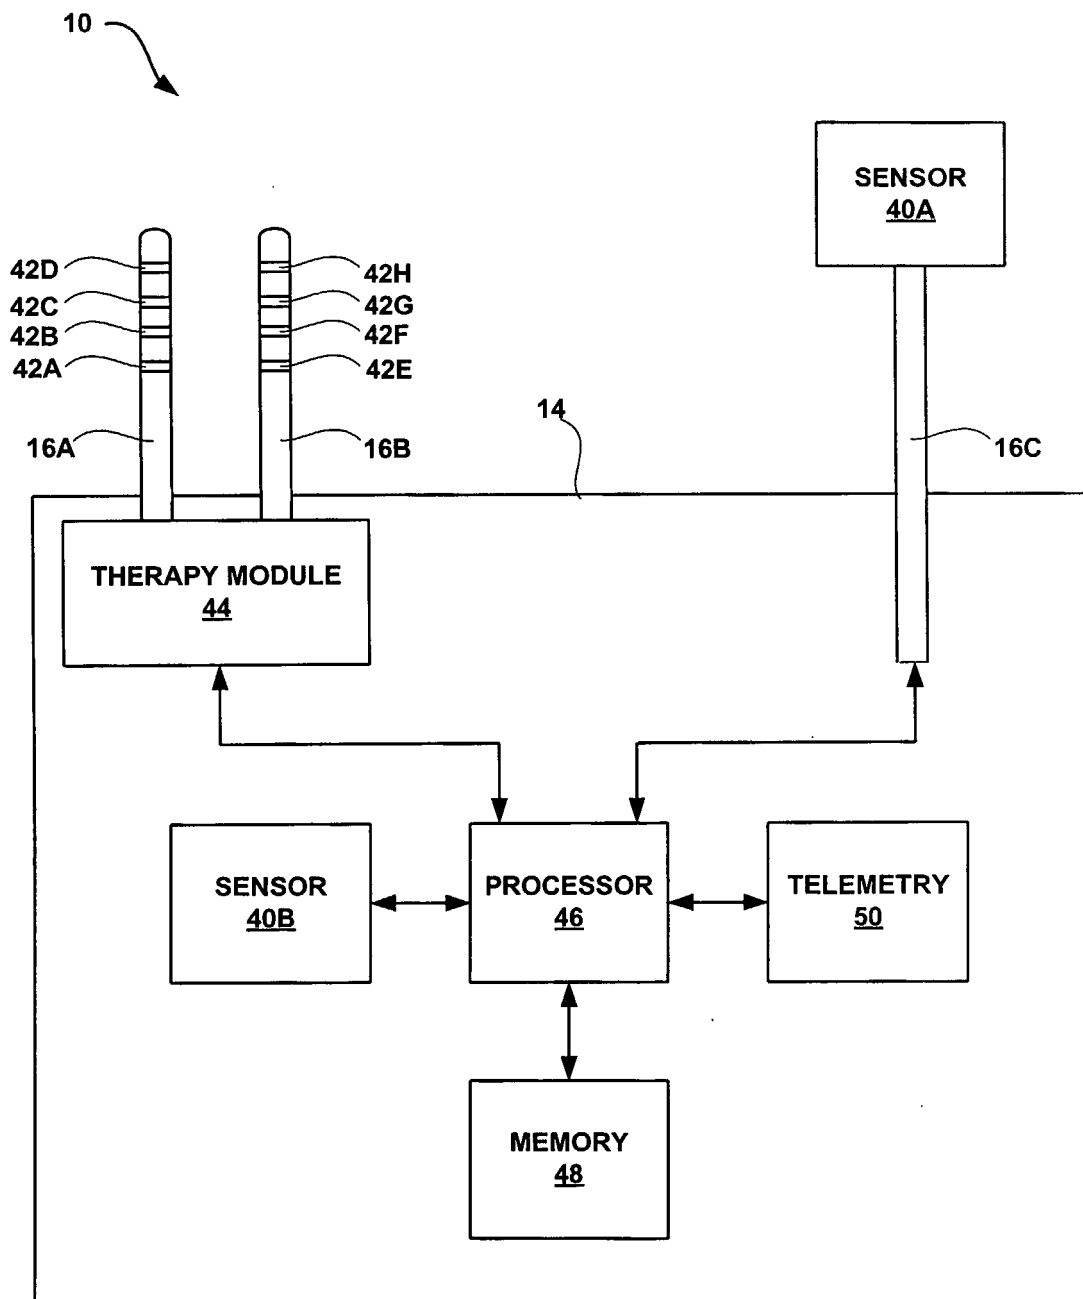


FIG. 2

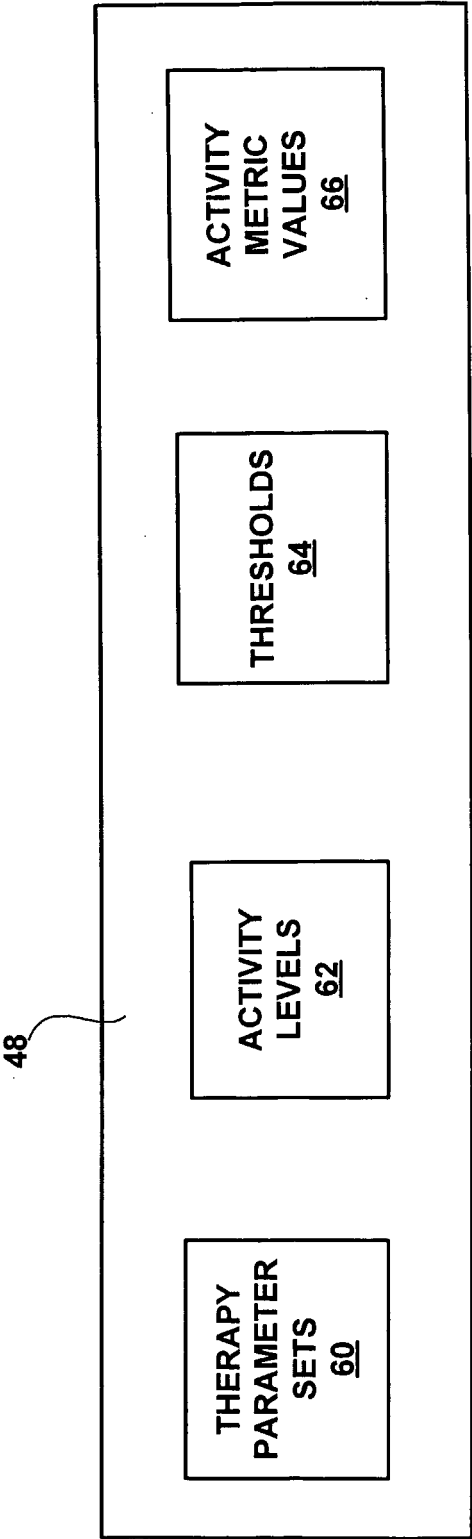


FIG. 3

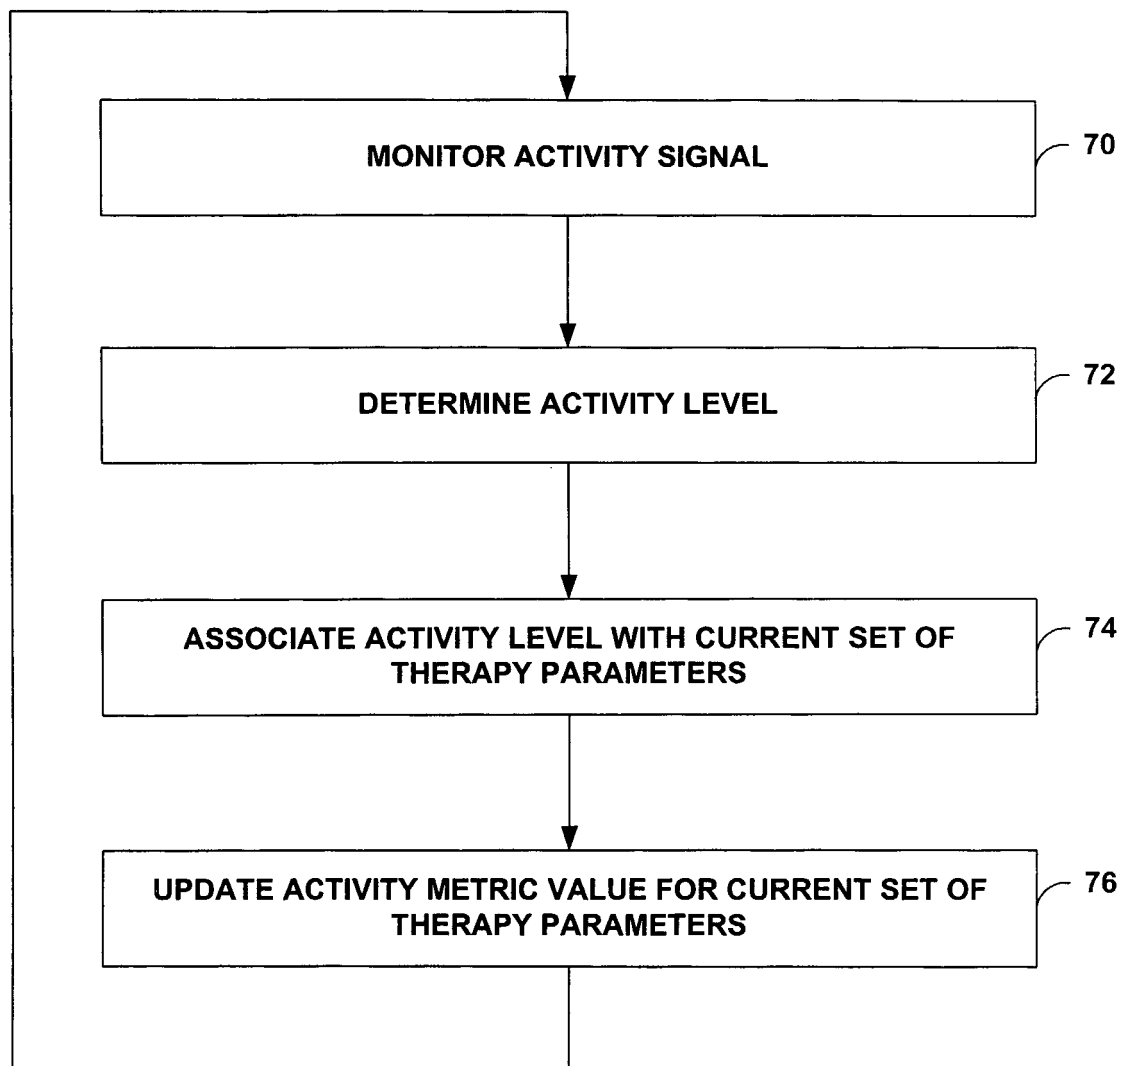


FIG. 4

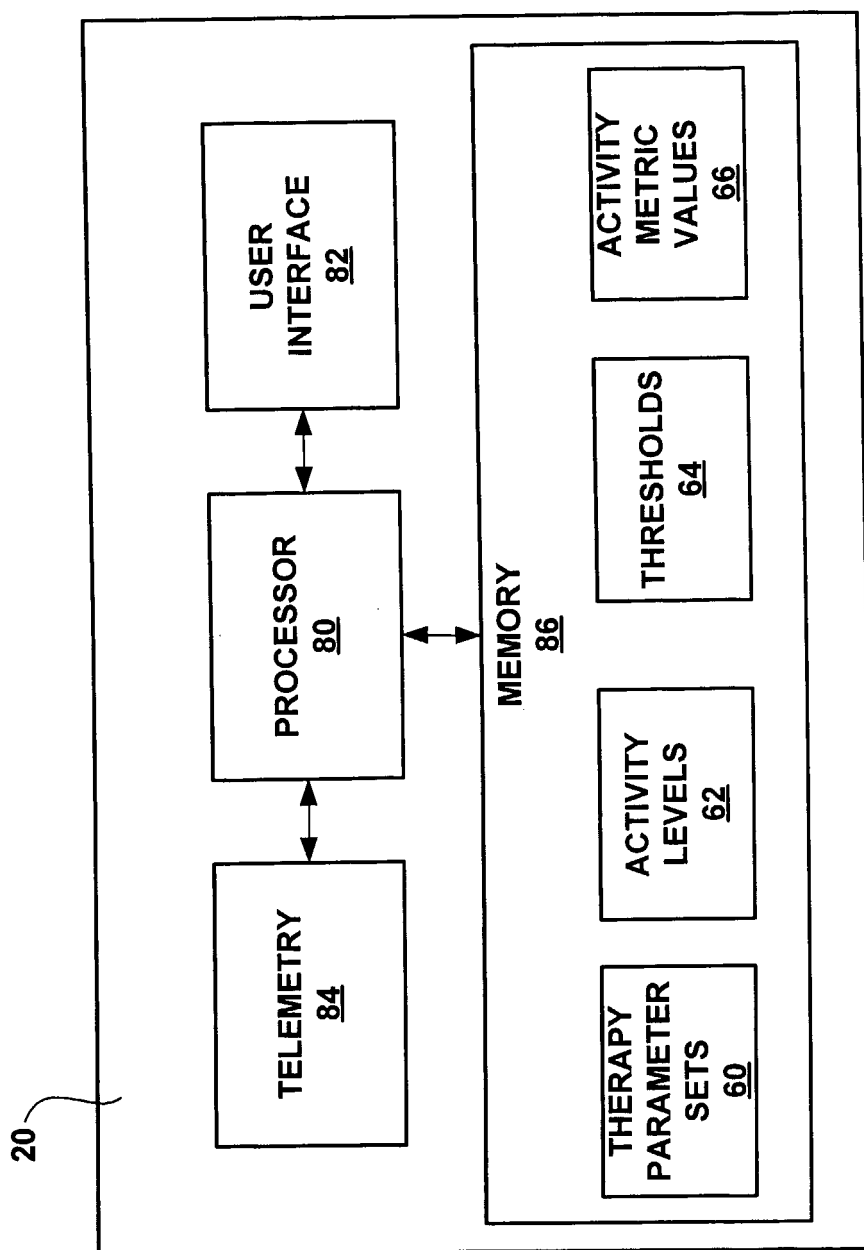



FIG. 5

90



<u>PARAMETER SET</u>	<u>PARAMETERS</u>	<u>% OF TIME ACTIVE</u>	<u>COUNTS/HOUR</u>
1	PA = 5.5V PW = 210ms PR = 90Hz	75% (15% HIGH)	100
2	PA = 5V PW = 190ms PR = 95Hz	60% (5% HIGH)	67
• • •			
N	PA = 4.6V PW = 215ms PR = 80Hz	55% (8% HIGH)	72

FIG. 6

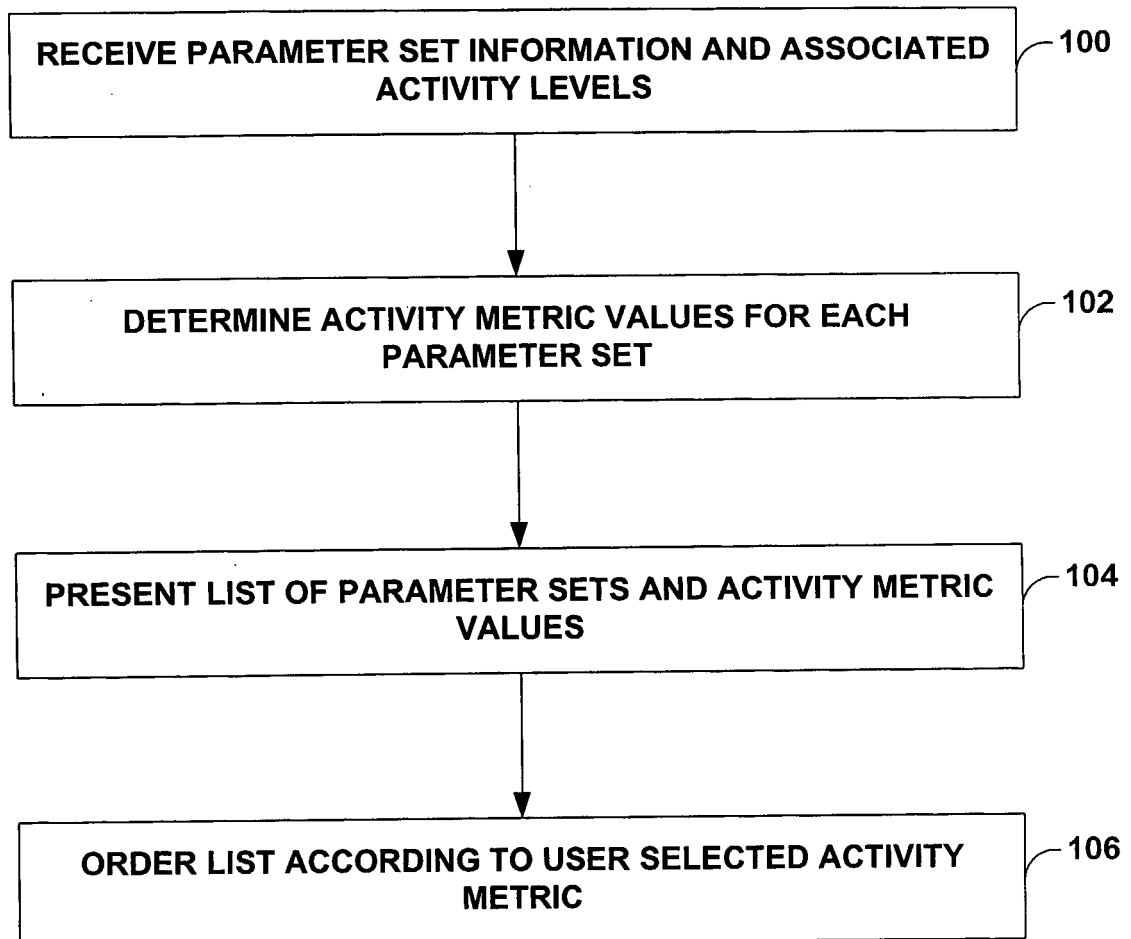**FIG. 7**

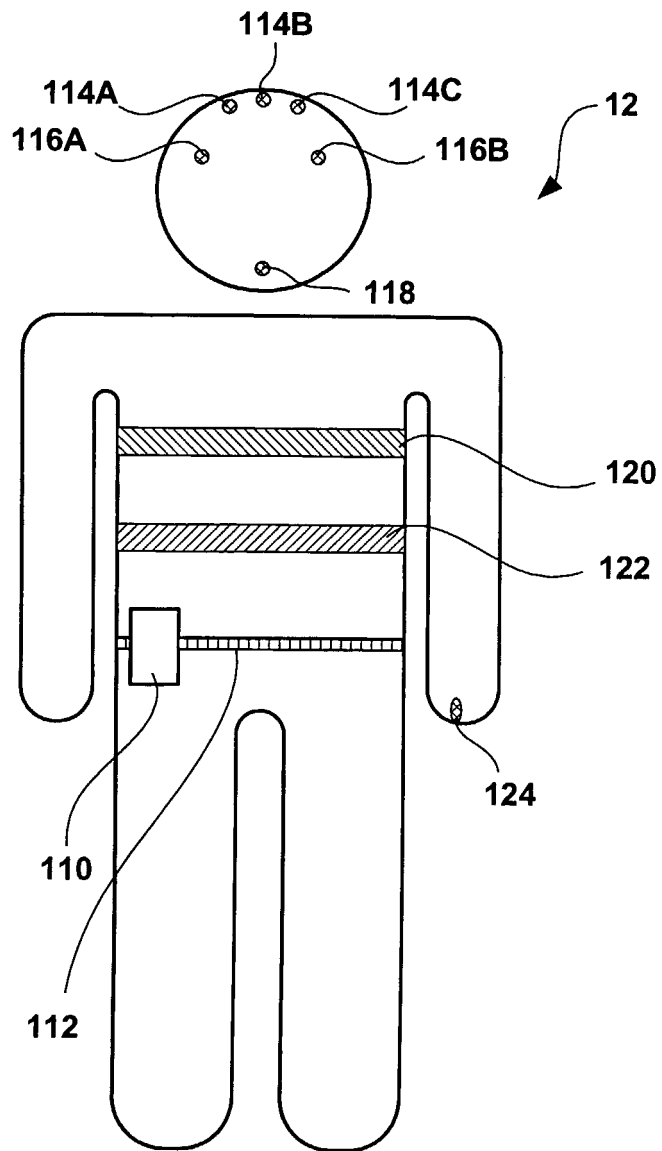


FIG. 8

INTERNATIONAL SEARCH REPORT

Int

pplication No

PCT/US2005/008800

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B5/11 A61N1/365

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 6 659 968 B1 (MCCLURE KELLY H) 9 December 2003 (2003-12-09)	1,11,12, 19,20
Y	column 5, line 52 - column 6, line 11; figures 1-3,6 column 6, lines 12-22 column 6, lines 31-54	2,3,8-10
Y	WO 01/37930 A (INTERMEDICS, INC) 31 May 2001 (2001-05-31) abstract page 6, line 13 - page 7, line 4; claims 2,3; figure 1 page 9, line 16 - page 13, line 2 page 15, line 11 - page 18, line 21 ----- -/--	2

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

* Special categories of cited documents:

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *G* document member of the same patent family

Date of the actual completion of the international search

16 August 2005

Date of mailing of the international search report

30. 08. 2005

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Kronberger, R

INTERNATIONAL SEARCH REPORT

Inter

al Application No .

PCT/US2005/008800

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 6 045 513 A (STONE ET AL) 4 April 2000 (2000-04-04) column 6, line 58 - column 7, line 28 column 7, lines 50-63 column 9, line 1 - column 10, line 13 column 13, line 55 - column 14, line 18 -----	8-10
X	US 6 120 467 A (SCHALLHORN ET AL) 19 September 2000 (2000-09-19) column 5, lines 35-65; figures 3a,3b column 3, lines 31-38 -----	1,4-6, 11,12,20
X	US 6 539 249 B1 (KADHIRESAN VEERICHETTY A ET AL) 25 March 2003 (2003-03-25) column 2, lines 32-61 column 3, line 45 - column 4, line 33 column 5, lines 1-19 column 5, lines 20-39 -----	1,4-6,8, 9,11,12, 16
E	WO 2005/035050 A (MEDTRONIC, INC) 21 April 2005 (2005-04-21) paragraphs '0041!', '0049!; claims 1-3,9; figures 1,2,6 -----	1
X	US 6 459 934 B1 (KADHIRESAN VEERICHETTY) 1 October 2002 (2002-10-01) column 3, lines 11-29; figures 1,9,10 column 6, lines 42-64 -----	1,13,14, 17,18
X	US 2002/161412 A1 (SUN WEIMIN ET AL) 31 October 2002 (2002-10-31) paragraphs '0011!', '0023! - '0030!, '0035! - '0037!; figures 4-6 -----	1,17,18
X	US 2002/077562 A1 (KALGREN JAMES ET AL) 20 June 2002 (2002-06-20) paragraphs '0010!', '0011!', '0046! - '0048!', '0053!', '0054!; figures 7,8 -----	1,17,18
Y	US 2003/212445 A1 (WEINBERG LISA P) 13 November 2003 (2003-11-13) paragraphs '0006!', '0036!', '0037!; figures 1,3 -----	3
A	US 2003/153953 A1 (PARK EULJOON ET AL) 14 August 2003 (2003-08-14) paragraphs '0045!', '0054!', '0055!, '0090! -----	3

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2005/008800

Box II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☒ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☒ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1, 2, 4-7, 8-10, 11-12, 16, 19-20

A medical system for associating a determined activity metric with a therapy parameter set.

1.1. claim: 2

A medical system for associating a determined activity metric with a therapy parameter set whereby an accelerometer signal is filtered by a passband filter with cutoff frequencies at 0.1Hz and 10Hz.

1.2. claims: 4-7, 8-10, 16

A medical system for associating a determined activity metric with a therapy parameter set having special means for the determination of the activity levels and of the activity metric from the activity levels.

2. claim: 3

A medical system for associating a determined activity metric with a therapy parameter set having means for determining when the patient is awake and for determining activity while the patient is awake.

3. claims: 13-15, 17-18

A medical system for associating a determined activity metric with a therapy parameter set having means for presenting a representation of the parameter sets, activity metric and activity levels.

INTERNATIONAL SEARCH REPORT

Int al Application No
PCT/US2005/008800

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 6659968	B1	09-12-2003	NONE
WO 0137930	A	31-05-2001	US 6249700 B1 19-06-2001 AU 1659401 A 04-06-2001 CA 2392354 A1 31-05-2001 EP 1233813 A1 28-08-2002 JP 2003514637 T 22-04-2003 WO 0137930 A1 31-05-2001
US 6045513	A	04-04-2000	CA 2331500 A1 18-11-1999 EP 1079733 A1 07-03-2001 JP 2002514454 T 21-05-2002 WO 9958056 A1 18-11-1999 US 6280409 B1 28-08-2001 US 6102874 A 15-08-2000
US 6120467	A	19-09-2000	EP 1075305 A1 14-02-2001 WO 9956820 A1 11-11-1999 US 6440090 B1 27-08-2002
US 6539249	B1	25-03-2003	US 6021351 A 01-02-2000 US 6135970 A 24-10-2000
WO 2005035050	A	21-04-2005	US 2005060001 A1 17-03-2005 WO 2005035050 A1 21-04-2005
US 6459934	B1	01-10-2002	AU 7335801 A 05-02-2002 EP 1301240 A1 16-04-2003 WO 0207814 A1 31-01-2002
US 2002161412	A1	31-10-2002	NONE
US 2002077562	A1	20-06-2002	US 2004082976 A1 29-04-2004
US 2003212445	A1	13-11-2003	NONE
US 2003153953	A1	14-08-2003	US 2003153956 A1 14-08-2003

专利名称(译)	收集活动信息以评估治疗		
公开(公告)号	EP1737343A1	公开(公告)日	2007-01-03
申请号	EP2005727233	申请日	2005-03-16
[标]申请(专利权)人(译)	美敦力公司		
申请(专利权)人(译)	美敦力公司，INC.		
当前申请(专利权)人(译)	美敦力公司，INC.		
[标]发明人	HERUTH KENNETH T MIESEL KEITH A		
发明人	HERUTH, KENNETH, T. MIESEL, KEITH, A.		
IPC分类号	A61B5/11 A61N1/365 A61B5/00 A61B5/0205 A61B5/0476 A61B5/0488 A61M5/142 A61M5/172 A61N1/05 A61N1/34 A61N1/36 A61N1/372		
CPC分类号	A61M5/1723 A61B5/0031 A61B5/02055 A61B5/0476 A61B5/0488 A61B5/1118 A61B5/1455 A61B5/6814 A61B5/6826 A61B5/6831 A61B5/6838 A61B2562/0219 A61M5/14276 A61N1/36071 A61N1/365 A61N1/36521 A61N1/36542 A61N1/36557		
优先权	60/553778 2004-03-16 US 10/825965 2004-04-15 US		
其他公开文献	EP1737343B1		
外部链接	Espacenet		

摘要(译)

医疗设备向患者提供治疗。医疗设备或另一设备可周期性地确定患者的活动水平，并将每个确定的活动水平与当前治疗参数组相关联。基于与该治疗参数集相关联的活动水平，为多个治疗参数集中的每一个确定至少一个活动度量的值。将治疗参数集的列表呈现给用户，例如临床医生，用于评估治疗参数集的相对功效。可以根据一个或多个活动度量值对列表进行排序，以帮助评估治疗参数集。在针对多个活动度量确定值的情况下，可以根据用户选择的活动度量之一来对列表进行排序。