



Europäisches
Patentamt
European
Patent Office
Office européen
des brevets



(11)

EP 1 424 934 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
06.08.2008 Bulletin 2008/32

(21) Application number: **01981641.2**

(22) Date of filing: **15.10.2001**

(51) Int Cl.:
A61B 5/00 (2006.01) **G06F 17/00 (2006.01)**

(86) International application number:
PCT/US2001/032282

(87) International publication number:
WO 2003/022141 (20.03.2003 Gazette 2003/12)

(54) A SIGNAL PROCESSING METHOD AND DEVICE FOR SIGNAL-TO-NOISE IMPROVEMENT

SIGNALVERARBEITUNGSVERFAHREN UND GERÄT ZUR VERBESSERUNG DES SIGNAL
RAUSCH VERHÄLTNISSES

PROCEDE ET DISPOSITIF DE TRAITEMENT DE SIGNAL PERMETTANT D'AMELIORER LE
RAPPORT SIGNAL SUR BRUIT

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR**

(30) Priority: **13.09.2001 IL 14544501**

(43) Date of publication of application:
09.06.2004 Bulletin 2004/24

(73) Proprietor: **ConMed Corporation
Utica NY 13502 (US)**

(72) Inventor: **WASSERMAN, Yoram
Haifa 34995 (IL)**

(74) Representative: **Becker Kurig Straus
Patentanwälte
Bavariastrasse 7
80336 München (DE)**

(56) References cited:
WO-A-00/13172 **US-A- 5 825 672**
US-A- 5 924 980 **US-A- 5 995 859**
US-A- 6 083 172

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionField of the Invention

[0001] This invention is generally in the field of signal-to-noise improvement techniques, and relates to a method and device for processing a periodic signal. The present invention is particularly useful in pulse oximeters or other non-invasive measurement devices for determining oxygen saturation and/or cardiac output.

Background of the Invention

[0002] Signal processing is an intrinsic procedure of any measurement technique, and always requires sufficient signal-to-noise ratio to enable extraction of a signal component indicative of a desired parameter from a noise component contained in the measured signal. For example, measurement techniques aimed at determining physiological parameters consist of detecting and analyzing a signal response, e.g., light response, of a sample to the application of an external field, e.g., electromagnetic radiation, and typically require suitable signal processing to extract the signal component in the detected response.

[0003] Various techniques for non-invasive measurements of blood parameters have been developed. One of such techniques is the so-called "bio-impedance technique" consisting of the following. A current source produces an alternating current, which is applied to the body through electrodes, and voltage induced by this current passage through the body is measured at additional electrodes. Other techniques utilize spectrophotometry consisting of illumination of a body part by incident light of various wavelengths and measurement of an absorption spectrum.

[0004] The most popular spectrophotometric techniques are oximetry and pulse oximetry. Oximetry is based on the strong dependence of the optical property of blood in the visible (between 500 and 700nm) and near-infrared (between 700 and 1000nm) spectra on the amount of oxygen in blood. Pulse oximetry, which utilizes transmission and reflection modes, relies on the detection of a photoplethysmographic signal caused by variations in the quantity of arterial blood associated with periodic contraction and relaxation of a patient's heart. The magnitude of this signal depends on the amount of blood ejected from the heart into the peripheral vascular bed with each systolic cycle, the optical absorption of the blood, absorption by skin and tissue components, and the specific wavelengths that are used to illuminate the tissue. Oxyhemoglobin saturation (SaO_2) is determined by computing the relative magnitudes of red (R) and infrared (IR) photoplethysmograms.

[0005] Electronic circuits, or suitable software (algorithm) inside the pulse oximeter, separate the R and IR photoplethysmograms into their respective pulsatile (AC) and non-pulsatile (DC) signal components. An algorithm

inside the pulse oximeter performs a mathematical normalization by which the time-varying AC signal at each wavelength is divided by the corresponding time-invariant DC component which results mainly from the light absorbed and scattered by the bloodless tissue, residual arterial blood when the heart is in diastole, venous blood and skin pigmentation. Since it is assumed that the AC portion results only from the arterial blood component, this scaling process provides a normalized R/IR ratio,

5 i.e., the ratio of AC/DC values corresponding to Rand IR-spectrum wavelengths, respectively, which is highly dependent on SaO_2 , but is largely independent of the volume of arterial blood entering the tissue during systole, skin pigmentation, skin thickness and vascular structure.

[0006] Pulse oximetry operating in reflection mode, while being based on similar spectrophotometric principles as that of transmission mode, is more challenging to perform and has unique problems that cannot always be solved by solutions suitable for solving the problems

20 associated with transmission-mode pulse oximetry. Generally, when comparing transmission and reflection pulse oximetry, the problems associated with reflection pulse oximetry consist of the following. In reflection pulse oximetry, the pulsatile AC signals are generally very small

25 and, depending on sensor configuration and placement, have larger DC components as compared to those of transmission pulse oximetry. In addition to optical absorption and reflection due to blood, the DC signal of the R and IR photoplethysmograms in reflection pulse oximetry can be adversely affected by strong reflections from a bone. This problem becomes more apparent when applying measurements at such body locations as the forehead and the scalp, or when the sensor is mounted on the chest over the ribcage. Similarly, variations in contact pressure between the sensor and the skin can cause larger errors in reflection pulse oximetry (as compared to transmission pulse oximetry) since some of the blood near the superficial layers of the skin may be normally displaced away from the sensor housing towards deeper

30 subcutaneous structures. Consequently, the highly reflective bloodless tissue compartment near the surface of the skin can cause significant errors even at body locations where the bone is located too far away to influence the incident light generated by the sensor.

35 **[0007]** Another problem with reflectance sensors currently available is the potential for specular reflection caused by the superficial layers of the skin, when an air gap exists between the sensor and the skin, or by the direct shunting of light between the LEDs and the photodetector through a thin layer of fluid (which may be due to excessive sweating or from amniotic fluid present during delivery).

[0008] It is important to keep in mind the two fundamental assumptions underlying conventional dual-wavelength pulse oximetry: The path of light rays with different illuminating wavelengths in tissue are substantially equal, and therefore, cancel each other. Each light source illuminates the same pulsatile change in arterial

blood volume. Furthermore, the correlation between optical measurements and tissue absorption in pulse oximetry are based on the fundamental assumption that light propagation is determined primarily by absorbance due to Lambert-Beer's law neglecting multiple scattering effects in biological tissues. In practice, however, the optical paths of different wavelengths in biological tissues are known to vary more in reflectance oximetry compared to transmission oximetry, since they strongly depend on the light scattering properties of the illuminated tissue and sensor mounting.

[0009] The relevant in vivo studies are disclosed, for example, in the following publications:

[0010] Dassel, et al., "Effect of location of the sensor on reflectance pulse oximetry", British Journal of Obstetrics and Gynecology, vol. 104, pp. 910-916, (1997);

[0011] Dassel, et al., "Reflectance pulse oximetry at the forehead of newborns: The influence of varying pressure on the probe", Journal of Clinical Monitoring, vol. 12, pp. 421-428, (1996).

[0012] It should be understood that the signal-to-noise ratio improvement is also needed in tissue simulated model measurements (*in vitro*). The problems arising with *in vitro* measurements are disclosed, for example in the following publication: Edrich et al., "Fetal pulse oximetry: influence of tissue blood content and hemoglobin concentration in a new *in-vitro* model", European Journal of Obstetrics and Gynecology and Reproductive Biology, vol. 72, suppl. 1, pp. S29-S34, (1997).

Document US-A-5 825 672 discloses a method according to the preamble of claim 1.

[0013] Improved sensors for application in dual-wavelength reflectance pulse oximetry have been developed, and are disclosed, for example, in the following publication: Mendelson, et al., "Noninvasive pulse oximetry utilizing skin reflectance photoplethysmography", IEEE Transactions on Biomedical Engineering, vol. 35, no. 10, pp. 798-805 (1988). According to this technique, the total amount of backscattered light that can be detected by a reflectance sensor is directly proportional to the number of photodetectors placed around the LEDs. Additional improvements in signal-to-noise ratio were achieved by increasing the active area of the photodetector and optimizing the separation distance between the light sources and photodetectors.

[0014] A different approach, based on the use of a sensor having six photodiodes arranged symmetrically around the LEDs, is disclosed in the following publications:

[0015] - Mendelson, et al., "Design and evaluation of a new reflectance pulse oximeter sensor", Medical Instrumentation, vol. 22, no. 4, pp. 167-173 (1988); and

[0016] - Mendelson, et al., "Skin reflectance pulse oximetry: *in vivo* measurements from the forearm and calf", Journal of Clinical Monitoring, vol. 7, pp. 7-12, (1991).

[0017] According to this approach, in order to maximize the fraction of backscattered light collected by the sensor, the currents from all six photodiodes are summed

electronically by internal circuitry in the pulse oximeter. This configuration essentially creates a large area photodetector made of six discrete photodiodes connected in parallel to produce a single current that is proportional to the amount of light backscattered from the skin.

[0018] A reflectance sensor based on the use of eight dual-wavelength LEDs and a single photodiode is disclosed in the following publication: Takatani et al., "Experimental and clinical evaluation of a noninvasive reflectance pulse oximeter sensor", Journal of Clinical Monitoring, vol. 8, pp. 257-266 (1992). Here, four R and four IR LEDs are spaced at 90-degree intervals around the substrate and at an equal radial distance from the photodiode. A similar sensor configuration based on six photodetectors mounted in the center of the sensor around the LEDs is disclosed in the following publication: Konig, et al., "Reflectance pulse oximetry - principles and obstetric application in the Zurich system", Journal of Clinical Monitoring, vol. 14, pp. 403-412 (1998).

[0019] Pulse oximeter probes of the type comprising three or more LEDs for filtering noise and monitoring other functions, such as carboxyhemoglobin or various indicator dyes injected into the blood stream, have been developed and are disclosed, for example, in WO 00/32099 and US 5,842,981. The techniques disclosed in these publications are aimed at providing an improved method for direct digital signal formation from input signals produced by the sensor and for filtering noise.

[0020] As indicated above, in pulse oximetry, SpO_2 and the heart rate are calculated from the detected signal, which is relatively small with a reflection-mode pulse oximeter. Methods for processing the signals detected by a pulse oximeter are described in the following U.S. Patents: 5,482,036; 5,490,505; 5,685,299; 5,632,272; 5,769,785; 6,036,642; 6,081,735; 6,067,462; and 6,083,172. These methods, however, utilize a specific model based on certain assumptions of noise reference.

SUMMARY

[0021] There is a need in the art to improve the signal-to-noise ratio (SNR) in measured data by providing a novel method for processing a measured signal, which has certain known characteristics.

[0022] The present invention is associated with the fact that the characteristics of most physiological signals are known, being for example periodic with certain well-defined peak-to-peak intensity value (such as a pulsatile blood-related signal), or periodic with a specific asymmetric shape (such as blood pressure pulse or ECG). On the contrary, a noise component in the measured signal is typically associated with artifacts of various kinds, and therefore has no specific characteristics.

[0023] The main idea of the present invention is as follows. The time variation of a response (measured signal or measured data) of a sample to the application of an external field is detected by any suitable means and a measured signal representative of the response is gen-

erated. If a signal component in the measured signal is a periodic signal with a certain well-defined peak-to-peak intensity value, upper and lower envelopes of the measured signal are determined and analyzed to extract said signal component of the measured signal. This signal component can further be used to calculate a desired parameter of the sample. The DC component of the signal is determined as the median value of the upper envelope, and the AC component is determined as the median value of the difference between the upper and lower envelopes. If a signal component of the measured signal is a periodic signal characterized by a specific asymmetric shape, a specific adaptive filtering is applied to the measured signal, resulting in the enhancement of the signal component relative to a noise component. This adaptive filtering is based on a derivative of the Gaussian Kernel having specific parameters matching the characteristics of the signal component.

[0024] The term "measured signal" used herein signifies a signal obtained by any measurement device and including a signal component, which is to be extracted and further used for determining a desired parameter, and a noise component caused by various noise and artifact conditions. The term "measured data" used herein refers to data indicative of two measured signals of different kinds. One kind of a measured signal suitable to be processed by the technique of the present invention is such containing a signal component in the form of a periodic signal with well-defined peak-to-peak value, e.g., sinusoidal-like signal. The other kind of a measured signal suitable to be processed by the technique of the present invention is one containing a signal component in the form of a periodic signal characterized by a specific asymmetric shape. Such a periodic asymmetrically shaped signal is characterized by the following: each cycle (period) of the signal contains a region including frequencies higher than those of the other regions. The present invention consists of a signal processing technique that can be carried out by a corresponding data processing and analyzing utility incorporated in a control unit of the measurement device, or in a separate unit connectable to the measurement device to receive and process the output thereof.

[0025] There is thus provided, according to one broad aspect of the present invention, a method as defined in claim 1, an apparatus as defined in claim 22, and a computer program storage device as defined in claim 28. Preferred embodiments of the invention are defined in the dependent claims.

[0026] More specifically, the present invention is used in non-invasive measurements of blood parameters and is therefore described below with respect to this application. It should, however, be understood that the present invention presents a method and utility for signal processing suitable for use in various applications (e.g., *in vivo* or *in vitro* measurements in a biological sample), provided that the signal component to be extracted from the measured signal for further analysis is either a substan-

tially periodic signal with a well-defined peak-to-peak value, or a substantially periodic signal characterized by a specific asymmetric shape as defined above.

5 BRIEF DESCRIPTION OF THE DRAWINGS

[0027] Other advantages of the present invention will be readily appreciated as the same becomes better understood by reference to the following detailed description when considered in connection with the accompanying drawings wherein:

[0028] In order to understand the invention and to see how it may be carried out in practice, a preferred embodiment will now be described, by way of non-limiting example only, with reference to the accompanying drawings, in which:

[0029] Figs. 1A and 1B illustrate a block diagram and a flow chart of main operation steps, respectively, of a control unit according to the invention;

[0030] Figs. 1C and 1D illustrate block diagrams of pulse oximetry and bio-impedance based systems, respectively, utilizing the present invention;

[0031] Figs. 1E and 1F illustrate the main operational steps of a method according to the invention carried out by the systems of Figs. 1C and 1D, respectively;

[0032] Figs. 2A and 2B illustrate experimental results of the method according to the invention used with the pulse oximetry, wherein Fig. 2A shows the envelope detection technique, and Fig. 2B shows how this technique can be used to extract the pulse amplitude (AC) from the detected signal;

[0033] Figs. 3A-3B and 4A-4B illustrate, respectively, two more examples showing experimental results of the method according to the invention used with the pulse oximetry;

[0034] Figs. 5A and 5B illustrate experimental results of the method according to the invention used with the bio-impedance technique, wherein Fig. 5A shows the envelope detection technique, and Fig. 5B shows how this technique can be used to extract the pulse amplitude (AC) from the detected signal;

[0035] Figs. 6A-6B, 7A-7B, 8A-8B and 9A-9B illustrate, respectively, four more examples showing experimental results of the method according to the invention used with the bio-impedance technique;

[0036] Fig. 10 illustrates the determination of a DC component of the pulsatile signal according to the invented method, as compared to that of the conventional technique;

[0037] Fig. 11 illustrates the typical shape and timing of a blood pressure pulse in an artery;

[0038] Fig. 12 illustrates the kernel function to be used in a method according to the invention;

[0039] Figs. 13A and 13B illustrate the experimental results of applying a reflectance pulse oximeter to the patient's chest, presenting a measured signal, respectively, prior to and after the filtering with the kernel function parameters;

[0040] Figs. 14A and 14B illustrate the spectra of a measured signal, respectively, prior to and after the filtering with DG Kernel parameters; and

[0041] Figs. 15A and 15B illustrate how the technique of the present invention can be used for enhancement of QRS segment in the ECG signal.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0042] With reference to the Figs. 1A and 1B, and in operation, the present invention provides a method and device for processing a measured signal. More specifically, the present invention extracts a signal component from the noise component and suppresses a noise component.

[0043] A control unit, generally designated 1, constructed and operated according to the invention for processing an input signal IS coming from a measurement device comprises a data processing and analyzing utility 2 having two software modules (components) C₁ and C₂ operating together to extract or enhance a signal component and suppress a noise component contained in the input signal. The software component C₁ processes the input signal, and the software component C₂ analyzes the processed data to either extract or enhance the signal component.

[0044] As shown in Fig. 1B, when a signal component S₁ in the form of a periodic signal with well-defined peak-to-peak value, e.g., sinusoidal-like signal, is to be extracted from the input measured signal IS, the processing of the measured signal includes determination of upper and lower envelopes E_{up} and E_{low} thereof (step 4), which are then analyzed to extract this signal component S₁ from a noise component (step 6).

[0045] If a signal component to be enhanced relative to a noise component is a periodic signal characterized by a specific asymmetric shape (i.e., each cycle (period) of the signal component contains a region including frequencies higher than those of the other regions), the data processing and analyzing utility 2 operates to define a specific kernel function (a derivative of a Gaussian with parameters matching the characteristics of the asymmetrically shaped signal component), and apply filtering to the measured signal with these kernel function parameters, thereby enhancing the signal component relative to the noise component in the filtered measured signal.

[0046] Referring to Fig. 1C, the present invention will now be described in the context of a measurement system 10 for non-invasive measurement of physiological parameters. It should be understood that the application of the present invention to such a measurement system 10 is for discussion purposes only and the present invention is not limited to such applications. The present invention has equal application to other uses where signal component of the kind specified is to be extracted from a measured containing a noise component.

[0047] In the present example, the system 10 is a re-

flectance pulse oximeter applied to a measurement location (not shown) on the patient's body and operable to detect a light response (reflection) of the measurement location and determine oxyhemoglobin saturation in the patient's blood and the heart rate. The system 10 comprises such main constructional parts as a measurement device 12 (probe) and a control unit 13.

[0048] The measurement device 12 comprises an illuminator and a detector unit. In the present example, the illuminator is composed of three light emitting elements (e.g., LEDs) 14A, 14B and 14C operated by three drivers D1-D3, respectively. LEDs 14A-14C illuminate the measurement location with three different wavelengths: one wavelength $\lambda 1$ lying in the red spectrum and the two other wavelengths $\lambda 2$ and $\lambda 3$ lying in a spectrum range including near infrared and infrared spectrum of radiation. Wavelengths $\lambda 2$ and $\lambda 3$ are selected to coincide with a spectral region of the optical absorption curve, where oxyhemoglobin (HbO₂) absorbs slightly more light than deoxyhemoglobin (Hb), and where the extinction coefficients of Hb and HbO₂ are nearly equal and remain relatively constant as a function of wavelength. The detector unit comprises two photodetectors PD₁ and PD₂, which receive light components reflected from the measurement location and generate measured data (current) indicative thereof.

[0049] It should be noted, although not specifically shown, that the photodetectors 14A, 14B, 14C are preferably designed and arranged so as to provide collection of light reflected from the measurement location at different detection points arranged along closed paths around the light emitting elements. For example, the photodetectors are two concentric rings (the so-called "near" and "far" rings), and the light emitting elements are located at the center of the rings. This arrangement enables optimal positioning of the detectors for high quality measurements, and enables distinguishing between photodetectors receiving "good" information (i.e., AC and DC values which would result in accurate calculations of SpO₂) and "bad" information (i.e., AC and DC values which would result in inaccurate calculations of SpO₂).

[0050] The operation of the measurement device and calculation of a blood parameter (e.g., oxyhemoglobin saturation) do not form part of the present invention, and therefore need not be specifically described, except to note the following. In this specific example of three wavelengths of incident radiation and a plurality of detection points, data indicative of AC/DC ratio in the light detected at each of the detection points for the three wavelengths is calculated, and analyzed to determine accepted detection points and select corresponding AC/DC ratios for each of three wavelengths. These selected ratios are then utilized to calculate the blood parameter. The analysis consists of the following: Values of the ratio W₂/W₃ (W₂=I₂(AC)/I₂(DC) and W₃=I₃(AC)/I₃(DC), I being the intensity) for the accepted detection points in at least one closed path are calculated. Each of these values is analyzed to determine whether it satisfies a certain prede-

terminated condition (e.g., the calculated value W_2/W_3 is inside a predetermined range defined by a threshold value), and generate a signal indicative of whether the position of the probe (sensor) is to be adjusted or not. If the condition is satisfied, the quality of a photoplethysmogram is analyzed to determine whether it is acceptable or not. If the quality is acceptable, the selected ratios are analyzed to calculate ratios W_1/W_2 and W_1/W_3 (wherein $W_1=I_1(\text{AC})/I_1(\text{DC})$) from the data detected in at least one closed path, and calculate the differences $\text{ABS}(W_1/W_2 - W_1/W_3)$. The calculated differences are analyzed to determine whether each of the differences satisfies a certain predetermined condition (e.g., the calculated difference $\text{ABS}(W_1/W_2 - W_1/W_3)$ is less than a certain threshold value for determining the blood parameter if the condition is satisfied.

[0051] As further shown in Fig. 1C, outputs of the photodetectors PD_1 and PD_2 are connected to analog-to-digital converters ADC_1 and ADC_2 , respectively, which are connected to a micro-controller 16 to thereby enable simultaneous signal conversion by sampling the signal and band pass filtering. By this, noise having spectral components other than that of the signal component is suppressed. The control unit further comprises a processor 17 (composed of data processing and analyzing utilities U_1 and U_2) preprogrammed to carry out a signal processing according to the invention, and a display 18. The provision of two utilities U_1 and U_2 is aimed at determining both the SpO_2 and the heart rate, wherein SpO_2 is derived from a measured signal of the kind having a signal component S_1 in the form of a periodic signal with well-defined peak-to-peak value, and the heart rate is derived from a measured signal of the kind having a signal component characterized by a specific asymmetric shape.

[0052] It should be understood that for the purpose of the present invention, the light source (with respective drivers), detector, analog-to-digital converters and micro-controller constitute together a measurement device for generating data indicative of a measured signal, which includes a signal component and a noise component (noise and artifacts). Such a measurement device may be of any kind. Actually, the processor, having either one of the utilities U_1 and U_2 or both of them, may be incorporated in a separate unit connectable to the measurement device to receive and process the measured signal to thereby enable the determination of a desired parameter. For the purposes of the present invention, the signal component in the measured signal is a periodic signal with a well-defined peak-to-peak value (e.g., a pulse related signal of blood), or a signal with a specific asymmetric shape (e.g., a heart pulse signal). By using the reflectance pulse oximeter 10 applied to a location on the patient's body, the measured data contains both the signal component S_1 representative of the pulse related signal of the patient's blood (a substantially periodic signal with substantially well-defined peak-to-peak intensity value) and the signal component S_2 representative of the

pulse related signal of the heart (a periodic signal characterized by a specific asymmetric shape).

[0053] Fig. 1D illustrates a block diagram of a measurement system 100 for bio-impedance measurements. To facilitate understanding, the same reference numbers are used to identify those components that are common in the examples of Figs. 1C and 1D. Thus, the measurement system 100 is composed of a measurement device 12 and a control unit 13, which comprises a processor 17 (composed of data processing and analyzing utilities U_1 and U_2) preprogrammed for carrying out the method according to the invention. In the present example of Fig. 1D, the measurement device 12 comprises an alternating current source 114 operated by the micro-controller 16 to inject an electric current to the patient's body by stimulating body electrodes 115; electrodes 116 sensitive to voltage induced by the injected alternating current; and electronic components 117 (demodulators and amplifiers) for detecting and amplifying the amplitude of the alternating voltage received from the sensing electrodes 116. In the measurement device of this kind, different electrodes' arrangements are typically used for producing the bio-impedance and ECG measured signals MS_1 and MS_2 .

[0054] Reference is made to Figs. 1E and 1F, illustrating the principles of the method according to the invention in the pulse oximeter and bio-impedance applications, respectively. To facilitate understanding, the same reference numbers are used to identify steps that are common in the examples of Figs. 1E and 1F.

[0055] As shown, measured data MD received from a measurement device first undergoes sampling and frequency filtering. In the example of Fig. 1E (pulse oximetry), the measured data MD, indicative of a pulsatile blood-related signal including both the periodic signal component with well-defined peak-to-peak intensity value and the periodic signal component characterized by a specific asymmetric shape, is supplied from the measurement device of a pulse oximeter, sampled (step 20), and then undergoes frequency filtering (step 22). The measured data MD is then split so as to undergo two concurrent processes carried out by respective data processing and analyzing utilities: a processing to determine the upper and lower envelopes of the measured data MD (step 26), and filtering of the measured data MD with a specific DG Kernel, as will be described more specifically further below.

[0056] In the example of Fig. 1F, measured signals MS_1 and MS_2 (indicative of, respectively, a bio-impedance and an ECG) are supplied from different electrode arrangements of the measurement device. Consequently, the measured signals are sampled by separate sampling utilities (steps 20A and 20B). Data indicative of the sampled measured signal MS_1 undergoes frequency filtering (step 22), and data indicative of the sampled measured signal MS_2 undergoes DG kernel filtering (step 24). The frequency-filtered measured signals MS_1 is processed to calculate upper and lower envelopes thereof

(step 26).

[0057] The upper and lower envelopes are used to determine AC and DC components of a pulsatile blood-related signal component of the measured signal (steps 28 and 30). The so-determined AC and DC components are used to calculate oxyhemoglobin saturation SpO_2 (step 32 in Fig. 1E), or the normalized impedance $Z=\text{AC}/\text{DC}$ (step 33 in Fig. 1F), and the calculation results are then displayed (step 34). The DG Kernel filtered data is processed to calculate the spectrum (step 36), which is analyzed to determine the biggest peak which is the heart rate (step 38). The calculation results are presented on the display (step 40).

[0058] Reference is made to Figs. 2A-2B, 3A-3B and 4A-4B illustrating three examples, respectively, of processing a measured signal obtained with a pulse oximeter. Figs. 2A, 3A and 4A illustrate the sampled and frequency filtered measured signals $MS^{(1)}_1$, $MS^{(2)}_1$ and $MS^{(3)}_1$ (each having a signal component representative of a pulsatile blood-related signal distorted by motion and respiration artifacts (noise component)), and upper and lower envelopes $E^{(1)}_{\text{up}}$ and $E^{(1)}_{\text{low}}$, $E^{(2)}_{\text{up}}$ and $E^{(2)}_{\text{low}}$ and $E^{(3)}_{\text{up}}$ and $E^{(3)}_{\text{low}}$ of the measured signals $MS^{(1)}_1$, $MS^{(2)}_1$ and $MS^{(3)}_1$, respectively. As shown in the example of Fig. 2A, the amplitude of the artifacts is about 6 times larger than the pulse amplitude (AC).

[0059] In order to calculate the upper and lower envelopes of a signal, the location of the local maximum and minimum values of the periodic signal are first calculated. Then, the values between the local minimum points are estimated producing a continuous line that defines the lower envelope, and the values between the local maximum points are estimated producing a continuous line that defines the upper envelope. The line estimation between extreme points can for example utilize linear interpolation or cubic spline interpolation methods.

[0060] Figs. 2B, 3B and 4B illustrate (in the enlarged scale) a signal resulting from the subtraction of the upper envelope from the respective measured signal (determination of the difference between the intensity values of the measured signal and the upper envelope for each point in time). As seen, distortions are now smaller than the signal amplitude, and hence, the signal-to-noise ratio is improved (by a factor of 10 in the example of Figs. 2A-2B).

[0061] In order to calculate the amplitude of the blood pulsation (AC component of the pulsatile blood-related signal), the lower envelope value is subtracted from the upper envelope value ($E_{\text{up}} - E_{\text{low}}$) for each time moment, thereby obtaining a vector of the same length as the vector representing the measured signal. Then, the vector values are sorted, and the median is calculated. Thus, according to the present invention, the alternating value (AC component) of a periodic signal with well-defined peak-to-peak intensity value is calculated as:

[0062]

$$\text{AC} = \text{MEDIAN}(E_{\text{up}} - E_{\text{low}})$$

5

[0063] It should be noted that, according to conventional techniques, extreme points are used to calculate the pulse amplitude. Hence, for a frame of 256 points (about 3sec), 3 heartbeats are observed (assuming a heart rate of 60 beats per minute), namely, only 3 maximal and 3 minimal values (one for each pulse). The calculation of the amplitudes of 3 pulses in the 3sec frame enables to obtain only 3 numbers, and the mean amplitude in the frame is calculated from these 3 pulse amplitudes. If the detected signal includes data representative of an additional pulse that does not really exist, this will affect the data analysis results (one wrong amplitude number from three values: two correct values and one false).

[0064] On the contrary, the present invention utilizes the statistical analysis of 256 values obtained after the subtraction of the two envelopes to estimate the most likely to appear amplitude in the frame. In order to reduce the influence of artifacts and to find the median of the signal (i.e., amplitude value that is most likely to appear) resulted from the subtraction ($E_{\text{up}} - E_{\text{low}}$), the values are sorted, 10% of the extreme values (the smallest and the largest ones) are excluded, and the median is taken from the remaining values.

[0065] Figs. 5A-5B, 6A-6B, 7A-7B, 8A-8B and 9A-9B illustrate five different examples, respectively, of processing a measured signal obtained with bio-impedance measurements of heart activity in a cardiac output measurement device. Here, Figs. 5A, 6A, 7A, 8A and 9A show the sampled and frequency filtered measured signals (each having a signal component representative of a pulsatile blood-related signal distorted by motion and respiration artifacts), and upper and lower envelopes of the measured signals. Figs. 5B, 6B, 7B, 8B and 9B signals with the improved signal-to-noise ratio obtained by subtracting the upper envelopes from the respective measured signals.

[0066] Calculation of the DC component of a blood-related signal contained in the measured signal MS_1 will now be described with reference to Fig. 10. When illuminating the measurement location during the pulse (when blood fills a blood vessel), more of the incident light is absorbed. Therefore, the detected signal reflected from the skin is decreased accordingly (proportional to the light absorption).

[0067] According to the conventional approach, the constant value of the reflected light intensity (i.e., the DC component of the photoplethysmogram) is calculated as the average value of a signal S_1 measured in the middle of the measured signal MS_1 . This approach is based on the fact that the average value contains the constant level of reflected light (between arterial pulses) and the pulsation value (AC component). This averaging value is a

result of the base line, the amplitude of the pulse, and the shape of the pulse.

[0068] According to the technique of the present invention, the real constant absorption component defined by the upper envelope E_{up} of the measured signal MS_1 , is used to calculate the DC component value, which gives better accuracy, as compared to the conventional approach. Thus, according to the invention, the upper envelope values are sorted, and the median is taken as the DC component, i.e., $DC = MEDIAN(E_{up})$. Alternatively, the DC component of such a periodic signal with well-defined peak-to-peak value may be calculated as the median of the half of the sum of the upper and lower envelope values, i.e., $DC = MEDIAN((E_{up} + E_{low})/2)$.

[0069] The signal processing according to the invention suitable to be used for the calculation of the heart rate will now be described. This technique is based on the knowledge about the physiological properties of the biophysical signals related to the heart cycle, and consists of a spectral filtering kernel preprocessing in order to enhance the pulse signal from the additive noise and disturbances, thus improving the signal-to-noise ratio. This makes further processing techniques, such as Fast Fourier Transform and auto correlation, more efficient when processing the signal to calculate the heart rate.

[0070] Fig. 11 illustrates a graph G of the typical shape and timing of the blood pressure pulse in an artery which represents a biophysical signal related to the change in the blood pressure, induced by the heart cycle, and presents a signal component in the measured signal MS_2 . This signal component has the active phase (systolic phase) P_{act} and the passive phase (diastolic phase) P_{pas} of the pulse. The duration of the active phase P_{act} is defined by the heart's contraction phase and ranges between 80 and 140ms, and the duration of the passive phase P_{pas} is the remaining time, i.e., the difference between the heart rate duration and the active phase duration. The typical human heart rate ranges between 40bpm and 280bpm, and is equivalent to the frequency range of 0.67-4.7Hz. In order to filter out noise and artifacts, the pulse oximeter, as well as any other suitable measurement device, typically utilizes filters with the band pass of 0.5-10HZ. Examining the frequency content of the systolic phase P_{act} in the heart pulse, it is evident that it contains frequencies above 10Hz. For example, in a 80ms rising phase, the frequency content of 12.5Hz is included (i.e., $1/0.08=12.5$).

[0071] In order to enhance the heart pulse signal, the present invention utilizes the specific asymmetric shape of the blood pressure pulse by adapting the filtering to the fast rising phase of the signal, and thereby distinguishing the pulse signal component from the noise component in the measured signal MS_2 . In order to prevent disruption of the fast rising phase, the pass band of such an adaptive filter has to include frequencies above 12.5Hz. As for the lower bound, 0.5Hz is a proper cut-off frequency, since the heart rate goes down to the frequency of 0.67Hz, and below this value just a slow artifact

takes place, being caused by respiration or motion.

[0072] To this end, a special DG Kernel is used based on an analytic function in the form of the Derivative of a Gaussian (DG). The DG Kernel (DGK) analytic equation is:

[0073]

$$10 \quad DGK(t) = \frac{-t}{\sigma\sqrt{2\pi\sigma^2}} \exp\left[-\frac{1}{2\sigma^2}t^2\right]$$

[0074] wherein t and σ are the time and Gaussian width parameters. These parameters of the DG Kernel function should be matched to the pulse characteristics in order to have the best SNR.

[0075] Fig. 12 illustrates the function $DGK(t)$. This kind of kernel can advantageously function as a low pass filter to thereby filter high frequency noise. Additionally, this kernel can enhance the signal component in the measured signal when the signal component includes fast slopes at a specific range. This is due to the fact that the derivative operation of the filter is limited to its pass band region. One pass operation of filtering and heart pulse enhancement allow for real time fast determination of the heart rate.

[0076] The parameters of this kernel can be adjusted to enhance the systolic phase of the heart pulse signal or even of the QRS segment in an ECG signal, since the frequency content of the QRS segment includes frequencies higher than the frequencies in other segments of the ECG signal. Irrespective of that the shape of the ECG signal is different from the shape of the heart pulse, the DGK can be adapted to enhance the QRS segment relative to other segments in the ECG and to noise and artifacts contained in the ECG measured signal. This technique assists in the detection of the QRS segment, as will be described more specifically further below. Due to the fact that the signal processing according to the invention utilizes the asymmetric property of the pulse signal distinguishing it from other components (noise and artifacts) in the measured signal, the improved signal-to-noise ratio can be obtained, even when the noise and artifact frequency content overlaps with the heart rate frequency.

[0077] Thus, the present invention utilizes the Gaussian analytic equation, calculation of the analytic derivative, digitization at the relevant signal sampling frequency, optimization of the length t of the Kernel and the Gaussian width σ for the best performance, and then utilizes the result parameters as a general Finite Impulse Response (FIR) filter parameter. After filtering the measured signal MS_2 with the DG Kernel parameters, the energy in the measured signal related to the pulse is enhanced in relation to other artifacts and noise. The general Fast Fourier Transform can then be used to extract the heart rate.

[0078] Figs. 13A and 13B illustrate the experimental results of applying a reflectance pulse oximeter to the patient's chest. Fig. 13A shows a graph H_1 presenting the measured signal MS_2 . Here, respiration and other motion disturbances are presented as relatively slow changes in the signal base line. Heart signals are relatively fast and characterized by periodic small changes in the signal amplitude. It is evident that artifacts are dominant over the heart pulses, as they are about three to four times larger. Fig. 13B illustrates a graph H_2 presenting the result of the filtering of the measured signal of Fig. 13A with the DG Kernel parameters. Here, the heart pulses are dominant. Although the pulse amplitudes are modulated by the artifacts' trend, signal-to-noise ratio is significantly improved. As shown, small pulses that were distorted in the signal of Fig. 13A by the artifacts, have proper amplitudes in the signal of Fig. 13B.

[0079] Figs. 14A and 14B illustrate the spectra S_1 and S_2 of the measured signal containing an asymmetrically shaped signal component, respectively, prior to and after the filtering with DG Kernel parameters. Comparing these spectra to each other, it is clear that the peak representing the heart rate at 2.2Hz in much larger than the artifact peaks after the DG Kernel filtering. In other words, the DG Kernel filtering results in the enhancement of the heart rate peak at about 2.2Hz relative to other double peaks.

[0080] Many medical procedures require detection of the QRS segment of the ECG signal. The use of DG Kernel parameters for filtering enables enhancement of the QRS segment relative to other segments in the ECG signal. Figs. 15A and 15B illustrate respectively, the typical ECG signal with QRS segment, respectively prior to and after the filtering with the DG Kernel method, showing that the QRS segments are enhanced in the filtered signal.

[0081] Turning back to Figs. 1E and 1F, the DG Kernel method is applied to the measured signal after being frequency-filtered to suppress noise having a frequency other than that of the heart pulse signal. In other words, DG Kernel filtering is applied to the signal in which the noise and artifacts frequency spectra overlap the heart rate frequency spectrum. By this, pulse related information is enhanced, and then a general spectrum method can be applied to obtain the heart rate. The SpO_2 level is calculated using the envelope technique: The median of the difference ($E_{up} - E_{low}$) between the upper and lower envelope values is used for the pulse amplitude calculation (AC component of the pulsatile blood-related signal). The median of the upper envelope E_{up} is used for the calculation of the constant detected light (DC component of the pulsatile blood-related signal). The so-obtained AC and DC components are utilized to extract SpO_2 according to any suitable conventional technique.

[0082] Those skilled in the art will readily appreciate that various modifications and changes can be applied to the embodiments of the invention as hereinbefore exemplified without departing from its scope as defined in

and by the appended claims.

Claims

- 5 1. A method for processing a first measured signal to extract a first signal component and suppress a noise component of the first measured signal, wherein the first signal component is a substantially periodic signal **characterized by** a substantially well-defined peak-to-peak intensity value, the method comprising the steps of:
 - 15 a) determining upper and lower envelopes of the first measured signal; and
 - b) analyzing the upper and lower envelope values to extract the first signal component from the first measured signal,

characterized in that the step of analyzing the upper and lower envelope values includes the step of determining a median of the difference between the upper and lower envelope values.
- 20 2. The method of claim 1, wherein the median is determined as an alternating value in the first signal component.
- 30 3. The method of claim 1, wherein the median is determined as a constant value in the first signal component.
- 35 4. The method as set forth in claim 1 or 2, wherein the step of analyzing the upper and lower envelope values includes the step of determining a median of the upper envelope values, as a constant value in the first signal component.
- 40 5. The method as set forth in claim 1 or 2, wherein the step of analyzing the upper and lower envelope values includes the step of determining a median of the half of the sum of the upper and lower envelope values, as a constant value in the first signal component.
- 45 6. The method as set forth in any previous claim, wherein the first measured signal is a physiological signal.
- 50 7. The method as set forth in claim 6, wherein the first signal component is a pulsatile blood-related signal.
8. The method as set forth in claim 7, wherein the pulsatile blood-related signal is indicative of oxyhemoglobin saturation level.
- 55 9. The method as set forth in any previous claim, wherein the measured signal is a response of a sample to the application of an external field.

10. The method as set forth in claim 9, wherein the measured signal is a light response of the sample to incident light.
11. The method as set forth in claim 9 or 10, wherein the sample is biological. 5
12. The method as set forth in any previous claim, for use with a measurement device for non-invasive measurements of patient's blood and heart conditions, the first signal component being a pulsatile blood-related signal and containing a second signal component **characterized by** a specific asymmetric shape, the method further comprising the steps of: 10
- defining a kernel function being a derivative of a Gaussian with parameters matching the characteristics of the second signal component with the asymmetric shape; and
 - applying spectral filtering to the measured signal with the kernel function, thereby enhancing the second signal component **characterized by** the specific asymmetric shape relative to a noise component in the filtered signal, to thereby enable further processing of the enhanced pulse signal to determine the heart rate.
13. The method as set forth in any previous claim, further comprising the step of: 25
- providing said measured signal representative of a response of the sample to an external field, the measured signal comprising a signal component indicative of a desired parameter, and a noise component, the signal component being a substantially periodic signal **characterized by** a substantially well-defined peak-to-peak intensity value.
14. The method as set forth in claim 13, wherein the step of providing the measured signal includes the step of sampling and frequency filtering of the response. 30
15. The method of any previous claim, wherein said measured signal further includes a second signal component **characterized by** a specific asymmetric shape, the method further comprising the step of: 45
- defining a kernel function being a derivative of a Gaussian with parameters matching the characteristics of the second signal component, and processing the measured signal by filtering it with the kernel function parameters, thereby enhancing the second signal component relative to the noise component in the filtered measured signal. 50
16. The method of any of claims 1 to 14, further comprising the processing of a second measured signal including a second signal component **characterized by** a specific asymmetric shape, the method further comprising the step of: 55
- defining a kernel function being a derivative of a Gaussian with parameters matching characteristics of the second signal component, and processing the second measured signal by filtering it with the kernel function parameters, thereby enhancing the second signal component relative to the noise component in the filtered second measured signal.
- 15 17. The method as set forth in claim 16, wherein said second measured signal is ECG, the second signal component being representative of a QRS segment in the ECG signal.
- 20 18. The method as set forth in any previous claim, further comprising determining a parameter of the signal as a function of the extracted signal component.
19. The method as set forth in any previous claim, where- 25 in the step of analyzing the upper and lower envelopes includes the step of suppressing noise.
20. The method as set forth in any previous claim, in- 30 cluding the steps of applying an external field to a sample and sensing the signal, wherein the signal is a response of the sample to the external field.
21. The method as set forth in any previous claim, in- 35 cluding the steps of applying incident radiation to a sample and sensing the signal, where the signal is a response of the sample to the incident radiation.
22. An apparatus comprising:
- (a) a measurement device operable to illuminate a measurement location with incident light of predetermined frequencies, detect a light response of the measurement location to said incident light, and generate a measured signal indicative thereof including a signal component; and
 - (b) a control unit connectable to the measurement device for receiving and processing the measured signal, the control unit comprising a data processing and analyzing utility preprogrammed to determine upper and lower envelopes of the measured signal, and analyze the upper and lower envelope values to extract said signal component from a noise component in the measured signal, wherein said analyzing comprises determining a median of the difference between said upper and lower envelopes of said measured signal as an AC component

- of the signal.
23. The apparatus as set forth in claim 22, wherein said control unit is further preprogrammed to determine a median of the upper envelope values as a DC component of the signal.
24. The apparatus as set forth in claim 22 or 23, wherein said control unit is further preprogrammed to determine a median of a half of the sum of the upper and lower envelope values as a DC component of the signal component.
25. The apparatus as set forth in any of claims 22 to 24, the measured signal comprising a signal component **characterized by** a specific asymmetric shape, the control unit being preprogrammed to process the measured signal by filtering it with a predefined kernel function being a derivative of a Gaussian with parameters matching the characteristics of said signal component, thereby enhancing said signal component **characterized by** the specific asymmetric shape relative to a noise component in the filtered measured signal.
26. The apparatus as set forth in any of claims 22 to 25, wherein said measured signal is a pulsatile blood-related signal.
27. The apparatus as set forth in any of claims 22 to 26, wherein said apparatus is a pulse oximeter.
28. A computer program storage device readable by a machine, comprising a program of instructions executable by a machine to perform method steps of any of claims 1 to 21.
- werte den Schritt des Bestimmens eines Medians der Differenz zwischen den oberen und unteren Einhüllendenwerten einschließt.
- 5 2. Verfahren nach Anspruch, wobei der Median als ein alternierender Wert in der ersten Signalkomponente bestimmt wird.
- 10 3. Verfahren nach Anspruch 1, wobei der Median als ein konstanter Wert in der ersten Signalkomponente bestimmt wird.
- 15 4. Verfahren nach Anspruch 1 oder 2, wobei der Schritt des Analysierens der oberen und unteren Einhüllendenwerte den Schritt des Bestimmens eines Medians der oberen Einhüllendenwerte als einen konstanten Wert in der ersten Signalkomponente einschließt.
- 20 5. Verfahren nach Anspruch 1 oder 2, wobei der Schritt des Analysierens der oberen und unteren Einhüllendenwerte den Schritt des Bestimmens eines Medians der Hälfte der Summe des oberen und unteren Einhüllendenwerts als einen konstanten Wert in der ersten Signalkomponente einschließt.
- 25 6. Verfahren nach einem der vorhergehenden Ansprüche, wobei das erste gemessene Signal ein physiologisches Signal ist.
- 30 7. Verfahren nach Anspruch 6, wobei die erste Signalkomponente ein pulsierendes, blutbezogenes Signal ist.
- 35 8. Verfahren nach Anspruch 7, wobei das pulsierende, blutbezogene Signal einen Oxyhämoglobin-Sättigungspegel anzeigt.
- 40 9. Verfahren nach einem der vorhergehenden Ansprüche, wobei das gemessene Signal eine Reaktion einer Probe auf die Anwendung eines äußeren Feldes ist.
- 45 10. Verfahren nach Anspruch 9, wobei das gemessene Signal eine Lichtreaktion der Probe auf einfallendes Licht ist.
- 50 11. Verfahren nach Anspruch 9 oder 10, wobei die Probe biologisch ist.
- 55 12. Verfahren nach einem der vorhergehenden Ansprüche zur Verwendung mit einer Messvorrichtung für nicht-invasive Messungen von Blut- und Herzbedingungen eines Patienten, wobei die erste Signalkomponente ein pulsierendes, blutbezogenes Signal ist und eine zweite Signalkomponente einschließt, welche durch eine spezifische asymmetrische Form **gekennzeichnet** ist, wobei das Verfahren weiter die

Patentansprüche

1. Verfahren zur Verarbeitung eines ersten gemessenen Signals, um eine erste Signalkomponente zu extrahieren und eine Rauschkomponente des ersten gemessenen Signals zu unterdrücken, wobei die erste Signalkomponente ein im Wesentlichen periodisches Signal ist, **gekennzeichnet durch** einen im Wesentlichen wohldefinierten Spitze-Spitze-Intensitätswert, wobei das Verfahren die Schritte umfasst:
- a. Bestimmen der oberen und unteren Einhüllenden des ersten gemessenen Signals; und
b. Analysieren der oberen und unteren Einhüllendenwerte, um die erste Signalkomponente aus dem ersten gemessenen Signal zu extrahieren,
- dadurch gekennzeichnet, dass** der Schritt des Analysierens der oberen und unteren Einhüllenden-

Schritte umfasst:

- Definieren einer Kernfunktion, welche eine Ableitung einer Gaußverteilung mit Parametern darstellt, die mit den Merkmalen der zweiten Signalkomponente mit der asymmetrischen Form übereinstimmen; und 5
- Anwenden von Spektralfilterung auf das gemessene Signal mit der Kernfunktion, wobei **dadurch** die zweite Signalkomponente, welche durch die spezifische, asymmetrische Form **gekennzeichnet** ist, relativ zu einer Rauschkomponente in dem gefilterten Signal verstärkt wird, um **dadurch** eine weitere Verarbeitung des verstärkten Pulssignals zu ermöglichen, um die Herzrate zu bestimmen. 10
- 13.** Verfahren nach einem der vorhergehenden Ansprüche, weiter umfassend den Schritt: 15
- Bereitstellen des gemessenen Signals, welches eine Reaktion der Probe auf ein äußeres Feld wiedergibt, wobei das gemessene Signal eine Signalkomponente, welche auf einen erwünschten Parameter angibt und eine Rauschkomponente umfasst, wobei die Signalkomponente ein im Wesentlichen periodisches Signal ist, welches durch einen im Wesentlichen wohldefinierten Spitze-Spitze-Intensitätswert **gekennzeichnet** ist. 20
- 14.** Verfahren nach Anspruch 13, wobei der Schritt des Bereitstellens des gemessenen Signals den Schritt des Abtastens und Frequenzfilters der Reaktion einschließt. 25
- 15.** Verfahren nach einem der vorhergehenden Ansprüche, wobei das gemessene Signal weiter eine zweite Signalkomponente einschließt, welche durch eine spezifische, asymmetrische Form **gekennzeichnet** ist, wobei das Verfahren weiter den Schritt umfasst: 30
- Definieren einer Kernfunktion, welche eine Ableitung einer Gaußverteilung mit Parametern darstellt, die mit den Merkmalen der zweiten Signalkomponente übereinstimmen, und Verarbeiten des gemessenen Signals durch dessen Filtern mit den Kernfunktions-Parametern, wobei **dadurch** die zweite Signalkomponente relativ zu der Rauschkomponente in dem gefilterten gemessenen Signal verstärkt wird. 35
- 16.** Verfahren nach einem der Ansprüche 1 bis 14, weiter umfassend das Verarbeiten eines zweiten gemessenen Signals, welches eine zweite Signalkomponente einschließt, welche durch eine spezifische asymmetrische Form **gekennzeichnet** ist, wobei das Verfahren weiter den Schritt umfasst: 40
- Definieren einer Kernfunktion, welche eine Ableitung einer Gaußverteilung mit Parametern darstellt, die mit den Merkmalen der zweiten Signalkomponente übereinstimmen, und Verarbeiten des zweiten gemessenen Signals durch dessen Filtern mit den Kernfunktions-Parametern, wobei **dadurch** die zweite Signalkomponente relativ zu der Rauschkomponente in dem gefilterten zweiten gemessenen Signal verstärkt wird. 45
- 17.** Verfahren nach Anspruch 16, wobei das zweite gemessene Signal ein EKG ist, wobei die zweite Signalkomponente ein QRS-Segment in dem EKG-Signal darstellt. 50
- 18.** Verfahren nach einem der vorhergehenden Ansprüche, weiter umfassend Bestimmen eines Parameters des Signals als eine Funktion der extrahierten Signalkomponente. 55
- 19.** Verfahren nach einem der vorhergehenden Ansprüche, wobei der Schritt des Analysierens der oberen und unteren Einhüllenden den Schritt eines Unterdrückens von Rauschen einschließt. 60
- 20.** Verfahren nach einem der vorhergehenden Ansprüche, einschließlich den Schritt des Anlegens einer äußeren Feldes an die Probe und Erfassen des Signals, wobei das Signal eine Reaktion der Probe auf das äußere Feld darstellt. 65
- 21.** Verfahren nach einem der vorhergehenden Ansprüche, einschließlich den Schritt des Anlegens von einfallender Strahlung auf die Probe und Erfassen des Signals, wobei das Signal eine Reaktion der Probe auf die einfallende Strahlung darstellt. 70
- 22.** Vorrichtung, umfassend: 75
- a. eine Messvorrichtung, welche betriebsfähig ist, einen Messort mit einfallender Strahlung vorbestimmter Frequenzen zu beleuchten, eine Lichtreaktion des Messorts auf das einfallende Licht zu erfassen und ein entsprechendes gemessenes Signal zu erzeugen, welches eine Signalkomponente einschließt; und 80
- b. eine Steuereinheit, welche mit der Messvorrichtung verbindbar ist, um das gemessene Signal zu empfangen und zu verarbeiten, wobei die Steuereinheit eine Datenverarbeitungs- und Analysierungs-Dienstprogramm umfasst, welches vorprogrammiert ist, um die obere und untere Einhüllende des gemessenen Signals zu bestimmen und die oberen und unteren Einhüllendenwerte zu analysieren, um die Signalkomponente von einer Rauschkomponente in dem gemessenen Signal zu extrahieren, wobei das 85

- | | | |
|-----|--|-----|
| | Analysieren ein Bestimmen eines Medians der Differenz zwischen der oberen und unteren Einhüllenden des gemessenen Signals als eine AC-Komponente des Signals umfasst. | |
| 23. | Vorrichtung nach Anspruch 22, wobei die Steuereinheit weiter vorprogrammiert ist, einen Median der oberen Einhüllendenwerte als eine DC-Komponente des Signals zu bestimmen. | 5 |
| 24. | Vorrichtung nach Anspruch 22 oder 23, wobei die Steuereinheit weiter vorprogrammiert ist, einen Median von der Hälfte der Summe der oberen und unteren Einhüllendenwerte als eine DC-Komponente der Signalkomponente zu bestimmen. | 10 |
| 25. | Vorrichtung nach einem der Ansprüche 22 bis 24, wobei das gemessene Signal eine Signalkomponente einschließt, welche durch eine spezifische, asymmetrische Form gekennzeichnet ist, wobei die Steuereinheit vorprogrammiert ist, das gemessene Signal durch dessen Filtern mit einer vorbestimmten Kernfunktion zu verarbeiten, welche eine Ableitung einer Gaußverteilung mit Parametern darstellt, die mit den Merkmalen der Signalkomponente übereinstimmen, wobei dadurch die Signalkomponente, welche durch die spezifische, asymmetrische Form gekennzeichnet ist, relativ zu einer Rauschkomponente in dem gefilterten gemessenen Signal verstärkt wird. | 15 |
| 26. | Vorrichtung nach einem der Ansprüche 22 bis 25, wobei das gemessene Signal ein pulsierendes, blutbezogenes Signal ist. | 20 |
| 27. | Vorrichtung nach einem der Ansprüche 22 bis 26, wobei die Vorrichtung ein Puls-Oximeter ist. | 25 |
| 28. | Computerprogramm-Speicher-Vorrichtung, welche von einer Maschine lesbar ist, umfassend ein Programm von Anweisungen, welche von einer Maschine ausführbar sind, um Verfahrensschritte aus einem der Ansprüche 1 bis 21 auszuführen. | 30 |
| | Revendications | |
| 1. | Procédé de traitement d'un premier signal mesuré afin d'extraire une première composante de signal et de supprimer une composante de bruit du premier signal mesuré, dans lequel la première composante de signal est un signal sensiblement périodique caractérisé par une valeur d'intensité de crête à crête sensiblement bien définie, le procédé comprenant les étapes consistant à : | 35 |
| | a) déterminer des enveloppes supérieure et inférieure du premier signal mesuré ; et | 40 |
| | b) analyser les valeurs d'enveloppes supérieure et inférieure afin d'extraire la première composante de signal du premier signal mesuré, | 45 |
| | caractérisé en ce que l'étape d'analyse des valeurs d'enveloppes supérieure et inférieure comprend l'étape de détermination d'une médiane de la différence entre les valeurs d'enveloppes supérieure et inférieure. | 50 |
| | 2. Procédé selon la revendication 1, dans lequel la médiane est déterminée comme une valeur alternative dans la première composante de signal. | 55 |
| | 3. Procédé selon la revendication 1, dans lequel la médiane est déterminée comme une valeur constante dans la première composante de signal. | 60 |
| | 4. Procédé selon la revendication 1 ou 2, dans lequel l'étape d'analyse des valeurs d'enveloppes supérieure et inférieure comprend l'étape de détermination d'une médiane des valeurs d'enveloppe supérieure, comme une valeur constante dans la première composante de signal. | 65 |
| | 5. Procédé selon la revendication 1 ou 2, dans lequel l'étape d'analyse des valeurs d'enveloppes supérieure et inférieure comprend l'étape de détermination d'une médiane de la moitié de la somme des valeurs d'enveloppes supérieure et inférieure, comme une valeur constante dans la première composante de signal. | 70 |
| | 6. Procédé selon l'une quelconque des revendications précédentes, dans lequel le premier signal mesuré est un signal physiologique. | 75 |
| | 7. Procédé selon la revendication 6, dans lequel la première composante de signal est un signal lié à une impulsion sanguine. | 80 |
| | 8. Procédé selon la revendication 7, dans lequel le signal lié à une impulsion sanguine indique un niveau de saturation en oxyhémoglobine. | 85 |
| | 9. Procédé selon l'une quelconque des revendications précédentes, dans lequel le signal mesuré est une réponse d'un échantillon à l'application d'un champ externe. | 90 |
| | 10. Procédé selon la revendication 9, dans lequel le signal mesuré est une réponse lumineuse de l'échantillon à la lumière incidente. | 95 |
| | 11. Procédé selon la revendication 9 ou 10, dans lequel l'échantillon est biologique. | 100 |
| | 12. Procédé selon l'une quelconque des revendications | 105 |

Revendications

précédentes, destiné à être utilisé avec un dispositif de mesure en vue de mesures non-invasives des conditions sanguine et cardiaque d'un patient, la première composante de signal étant un signal lié à une impulsion sanguine et contenant une seconde composante de signal **caractérisée par** une forme asymétrique spécifique, le procédé comprenant en outre les étapes consistant à :

- définir une fonction de noyau qui est une dérivée d'une fonction gaussienne avec des paramètres correspondant aux caractéristiques de la seconde composante de signal ayant la forme asymétrique ; et

- appliquer un filtrage spectral au signal mesuré avec la fonction de noyau, améliorant ainsi la seconde composante de signal **caractérisée par** la forme asymétrique spécifique par rapport à une composante de bruit dans le signal filtré, de façon à permettre un autre traitement du signal d'impulsion amélioré afin de déterminer le rythme cardiaque.

13. Procédé selon l'une quelconque des revendications précédentes, comprenant en outre l'étape consistant à :

- fournir ledit signal mesuré représentant une réponse de l'échantillon à un champ externe, le signal mesuré comprenant une composante de signal indiquant un paramètre souhaité, et une composante de bruit, la composante de signal étant un signal sensiblement périodique **caractérisé par** une valeur d'intensité de crête à crête sensiblement bien définie.

14. Procédé selon la revendication 13, dans lequel l'étape consistant à fournir le signal mesuré comprend l'étape d'échantillonnage et de filtrage de fréquence de la réponse.

15. Procédé selon l'une quelconque des revendications précédentes, dans lequel ledit signal mesuré comprend en outre une seconde composante de signal **caractérisée par** une forme asymétrique spécifique, le procédé comprenant en outre l'étape consistant à :

- définir une fonction de noyau qui est une dérivée d'une fonction gaussienne avec des paramètres correspondant aux caractéristiques de la seconde composante de signal, et traiter le signal mesuré en le filtrant avec les paramètres de la fonction de noyau, améliorant ainsi la seconde composante de signal par rapport à la composante de bruit dans le signal mesuré filtré.

16. Procédé selon l'une quelconque des revendications

5

1 à 14, comprenant en outre le traitement d'un second signal mesuré comprenant une seconde composante de signal **caractérisée par** une forme asymétrique spécifique, le procédé comprenant en outre l'étape consistant à :

- définir une fonction de noyau qui est une dérivée d'une fonction gaussienne avec des paramètres correspondant aux caractéristiques de la seconde composante de signal, et traiter le second signal mesuré en le filtrant avec les paramètres de la fonction de noyau, améliorant ainsi la seconde composante de signal par rapport à la composante de bruit dans le second signal mesuré filtré.

15

20

25

30

35

40

45

50

55

17. Procédé selon la revendication 16, dans lequel ledit second signal mesuré est un électrocardiogramme, la seconde composante de signal étant représentative d'un segment QRS dans le signal d'électrocardiogramme.

18. Procédé selon l'une quelconque des revendications précédentes, comprenant en outre la détermination d'un paramètre du signal en fonction de la composante de signal extraite.

19. Procédé selon l'une quelconque des revendications précédentes, dans lequel l'étape d'analyse des enveloppes supérieure et inférieure comprend l'étape de suppression du bruit.

20. Procédé selon l'une quelconque des revendications précédentes, comprenant les étapes d'application d'un champ externe à un échantillon et de détection du signal, dans lequel le signal est une réponse de l'échantillon au champ externe.

21. Procédé selon l'une quelconque des revendications précédentes, comprenant les étapes d'application d'un rayonnement incident à un échantillon et de détection du signal, dans lequel le signal est une réponse de l'échantillon au rayonnement incident.

22. Appareil comprenant :

(a) un dispositif de mesure capable d'éclairer un emplacement de mesure avec une lumière incidente ayant des fréquences prédéterminées, de détecter une réponse lumineuse de l'emplacement de mesure à ladite lumière incidente, et de générer un signal mesuré indiquant celui-ci comprenant une composante de signal ; et
 (b) une unité de commande pouvant être reliée au dispositif de mesure afin de recevoir et de traiter le signal mesuré, l'unité de commande comprenant un module de traitement et d'analyse de données préprogrammé afin de déter-

miner les enveloppes supérieure et inférieure du signal mesuré, et d'analyser les valeurs d'enveloppes supérieure et inférieure afin d'extraire ladite composante de signal d'une composante de bruit dans le signal mesuré, dans lequel ladite analyse comprend la détermination d'une médiane de la différence entre lesdites enveloppes supérieure et inférieure dudit signal mesuré comme une composante CA du signal.

5

10

23. Appareil selon la revendication 22, dans lequel ladite unité de commande est en outre préprogrammée afin de déterminer une médiane des valeurs d'enveloppe supérieure comme une composante CC du signal.

15

24. Appareil selon la revendication 22 ou 23, dans lequel ladite unité de commande est en outre préprogrammée afin de déterminer une médiane d'une moitié de la somme des valeurs d'enveloppes supérieure et inférieure comme une composante CC de la composante de signal.

20

25. Appareil selon l'une quelconque des revendications 22 à 24, le signal mesuré comprenant une composante de signal **caractérisée par** une forme asymétrique spécifique, l'unité de commande étant préprogrammée afin de traiter le signal mesuré en le filtrant avec une fonction de noyau prédéfinie qui est une dérivée d'une fonction gaussienne avec des paramètres correspondant aux caractéristiques de ladite composante de signal, améliorant ainsi ladite composante de signal **caractérisée par** la forme asymétrique spécifique par rapport à une composante de bruit dans le signal mesuré filtré.

25

30

35

26. Appareil selon l'une quelconque des revendications 22 à 25, dans lequel ledit signal mesuré est un signal lié à une impulsion sanguine.

40

27. Appareil selon l'une quelconque des revendications 22 à 26, dans lequel ledit appareil est un sphygmo-oxymètre.

28. Dispositif de stockage de programme informatique lisible par une machine, comprenant un programme d'instructions exécutables par une machine afin d'effectuer les étapes selon l'une quelconque des revendications 1 à 21.

45

50

55

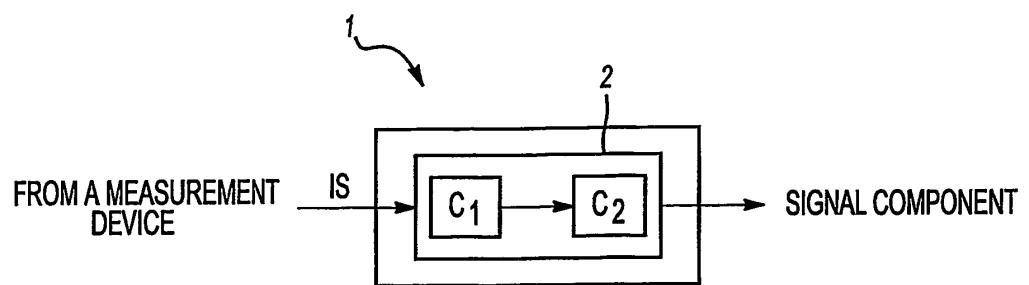


Fig-1A

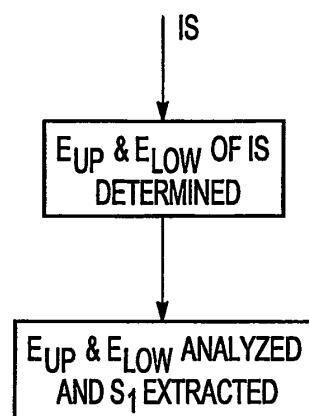
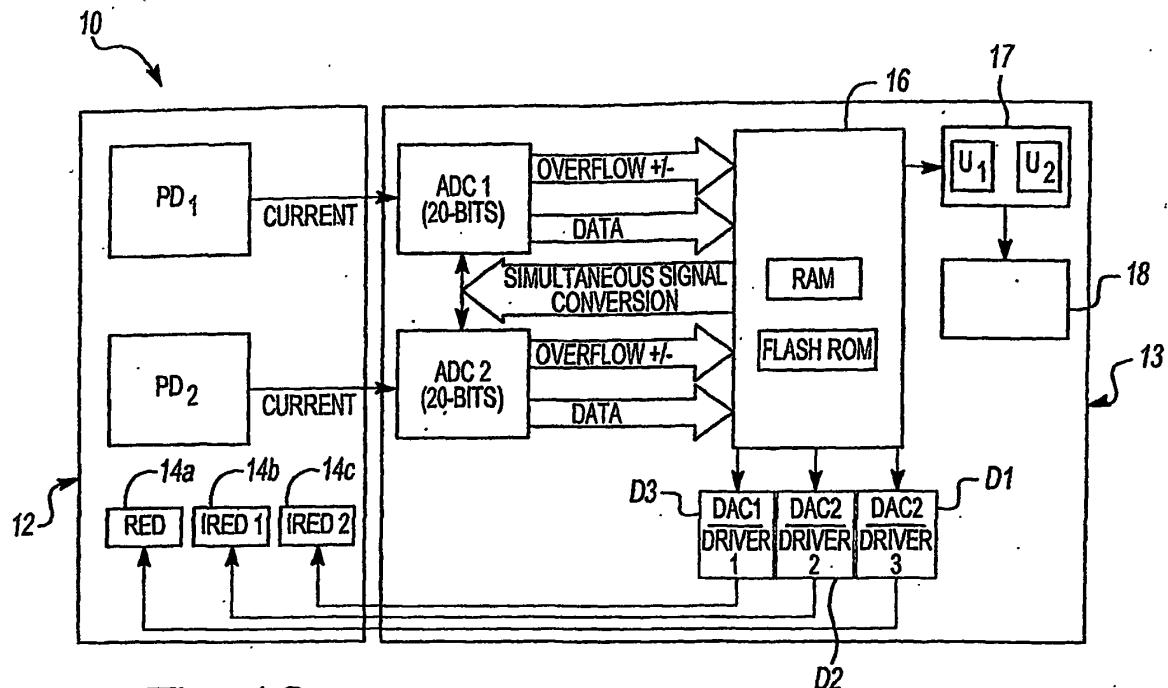
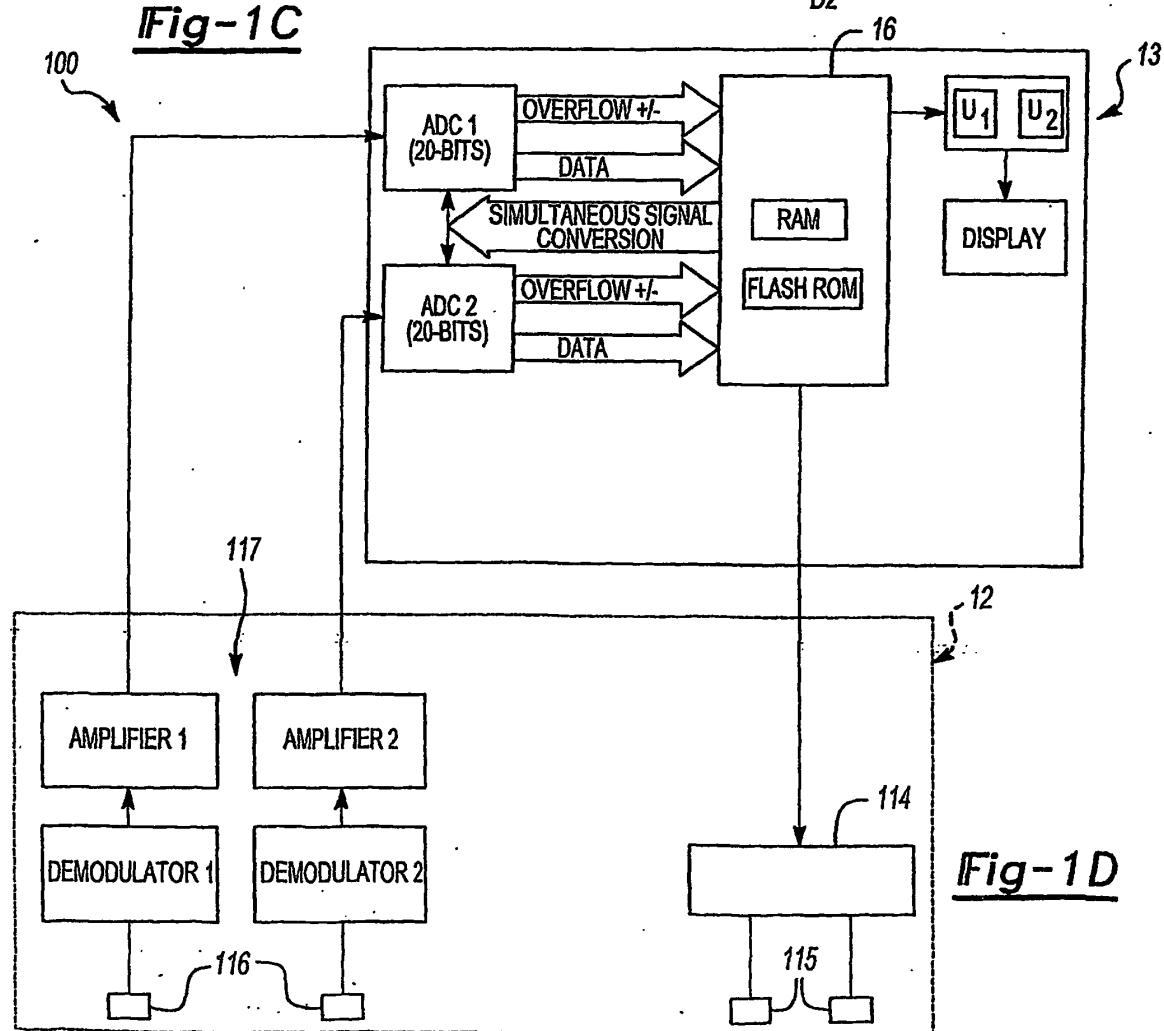
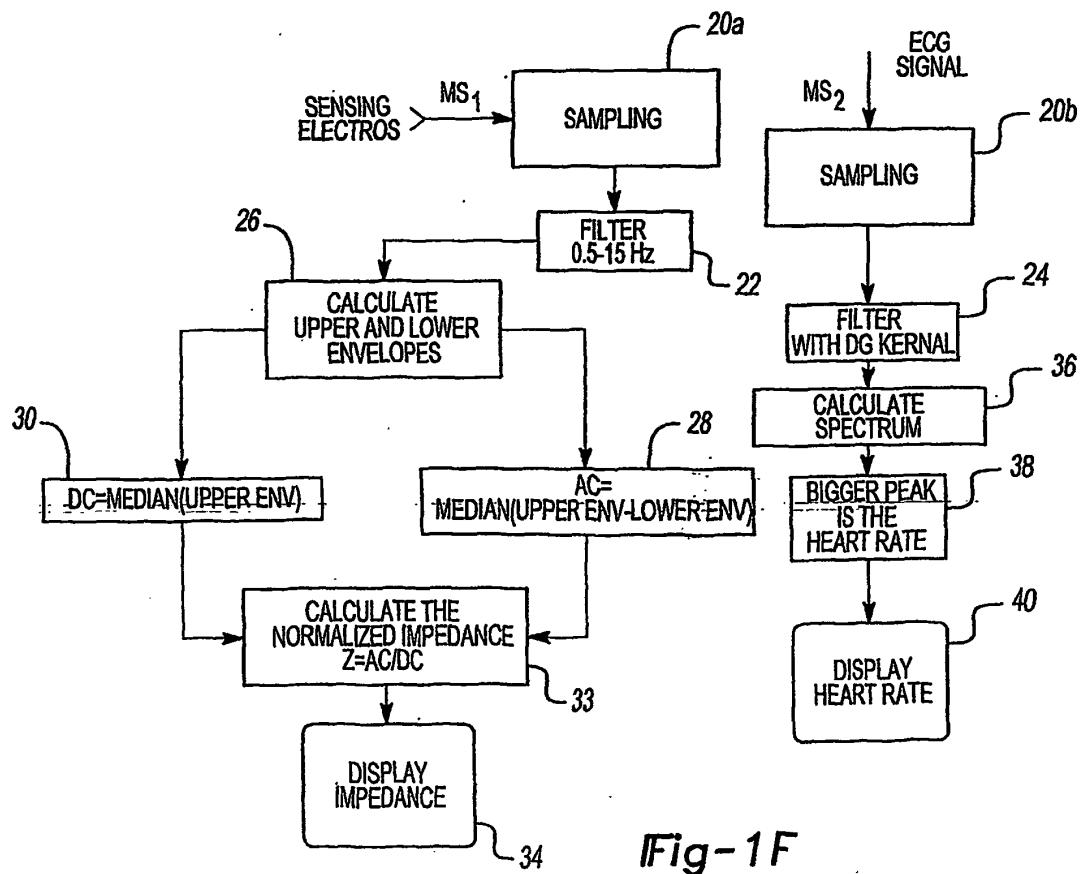
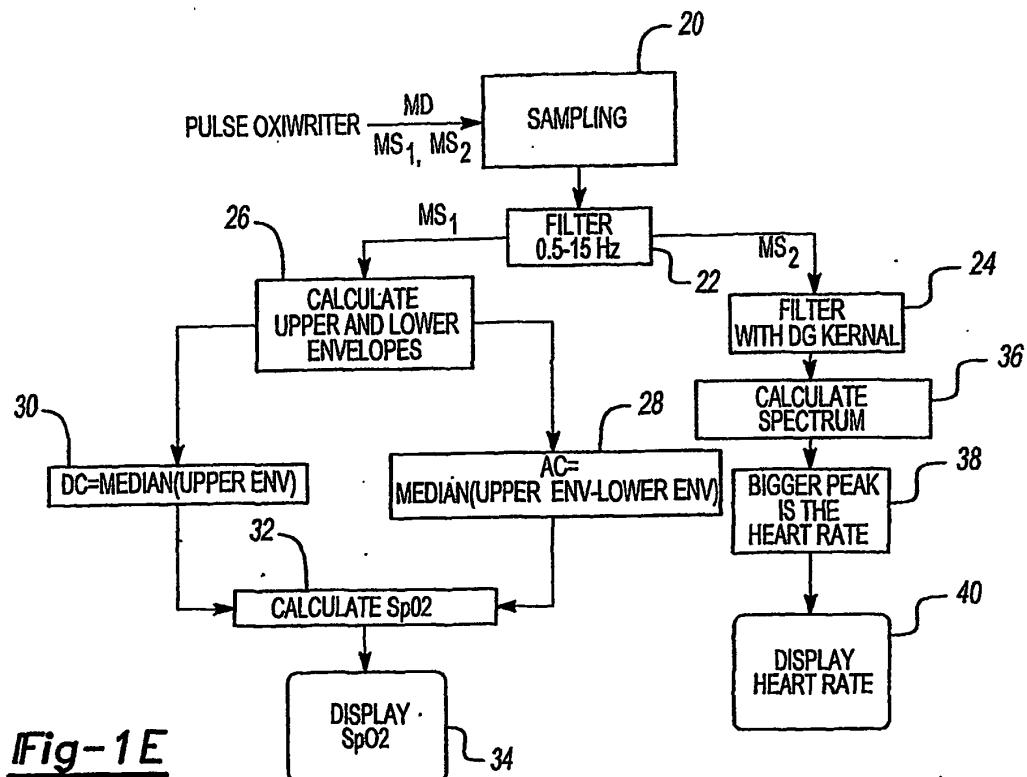
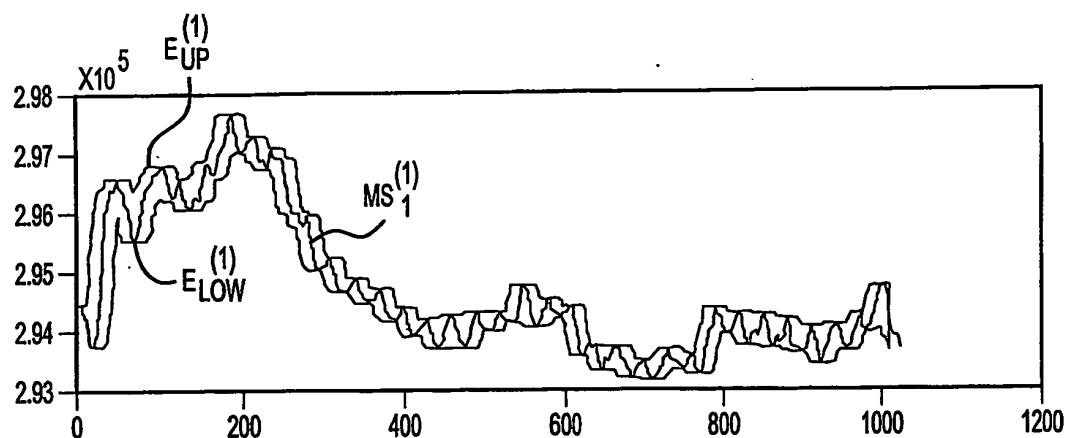
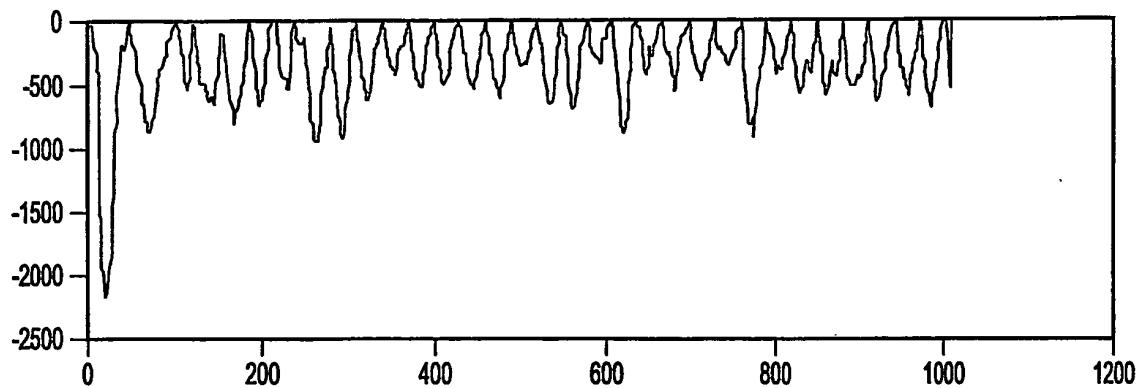
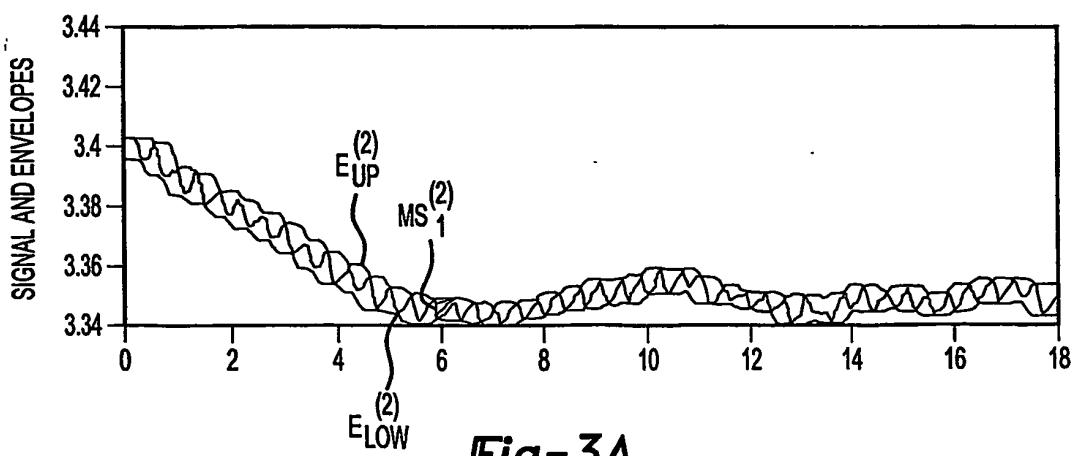
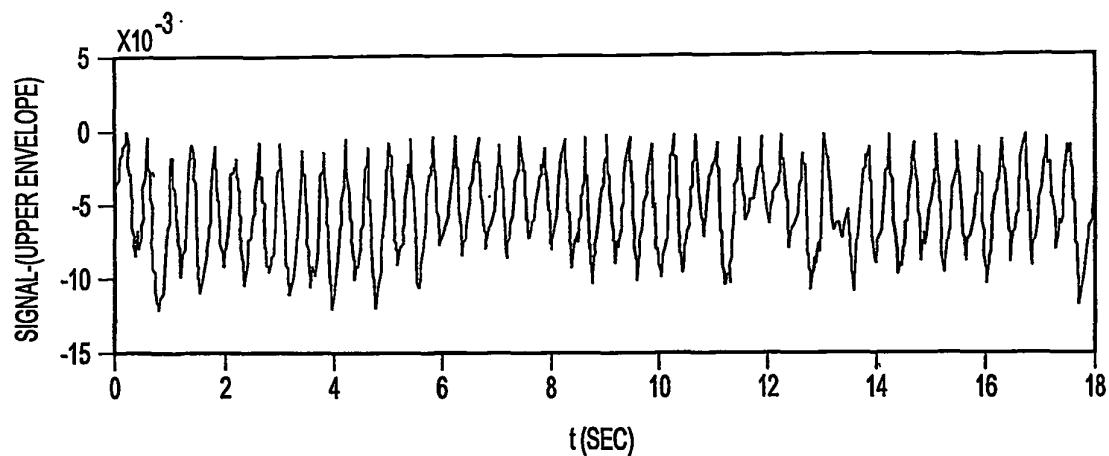
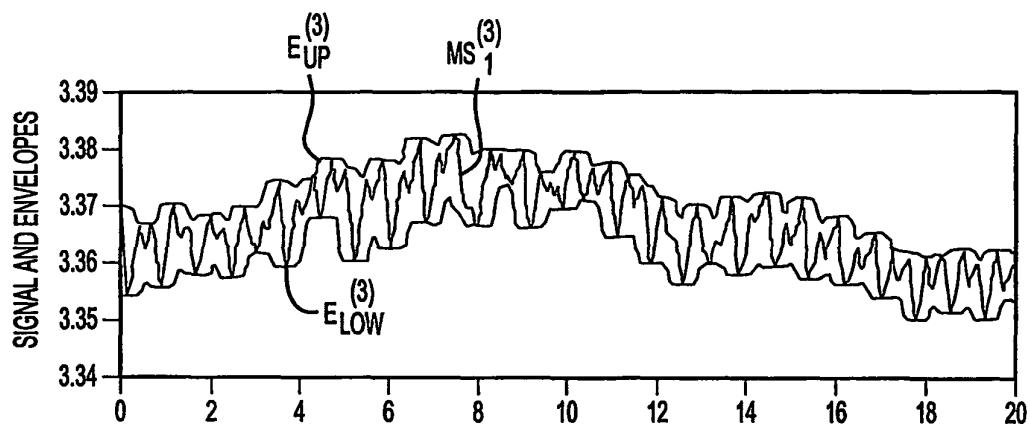
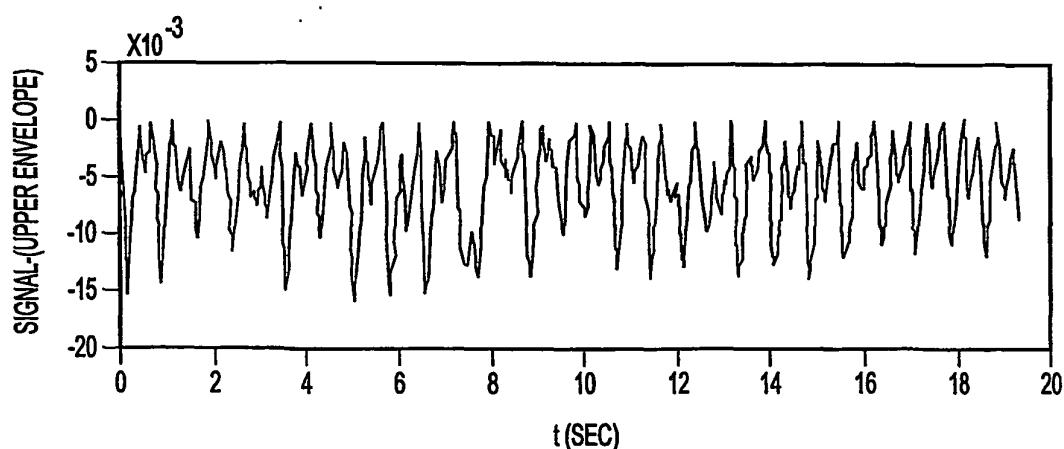


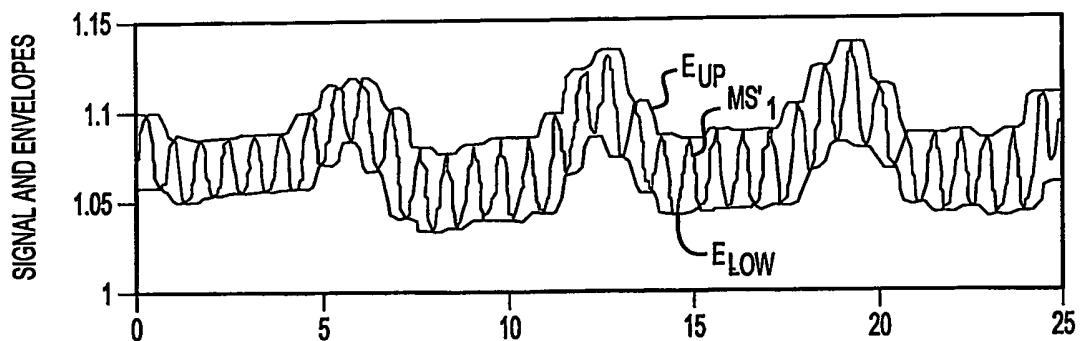
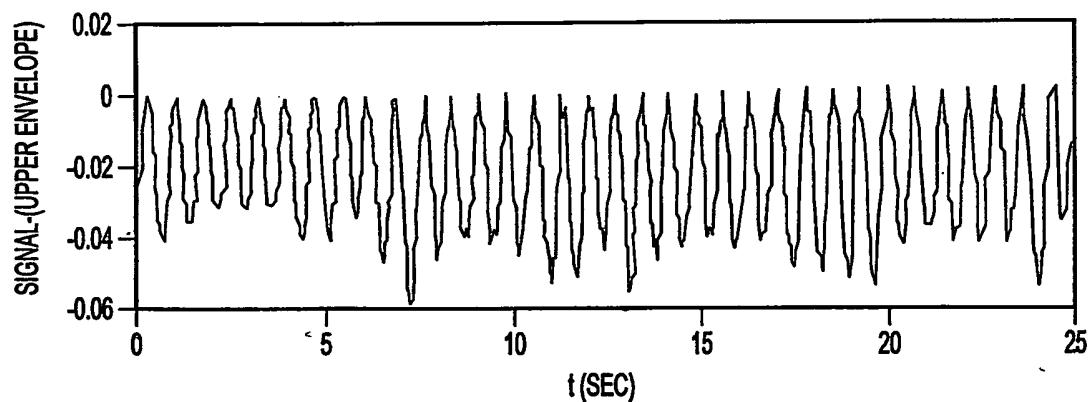
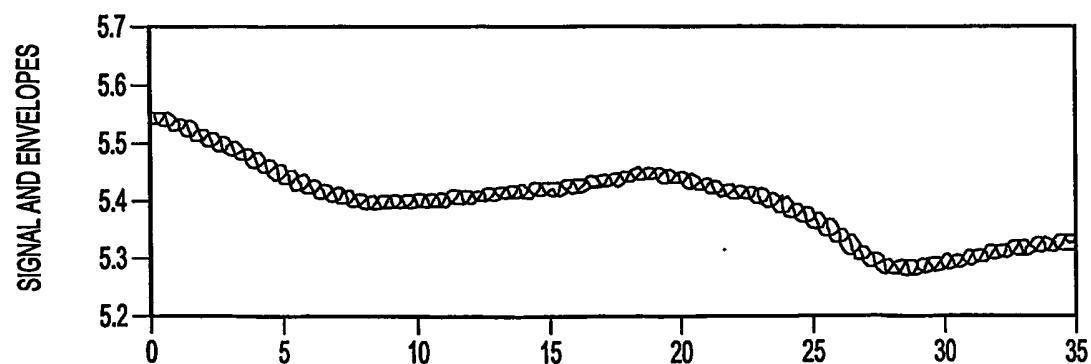
Fig-1B

Fig-1CFig-1D



Fig-2AFig-2BFig-3A

Fig-3BFig-4AFig-4B

Fig-5AFig-5BFig-6A

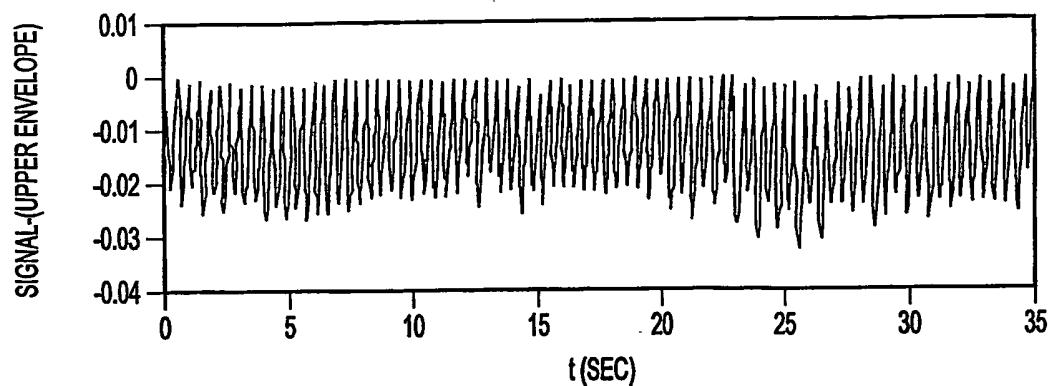


Fig-6B

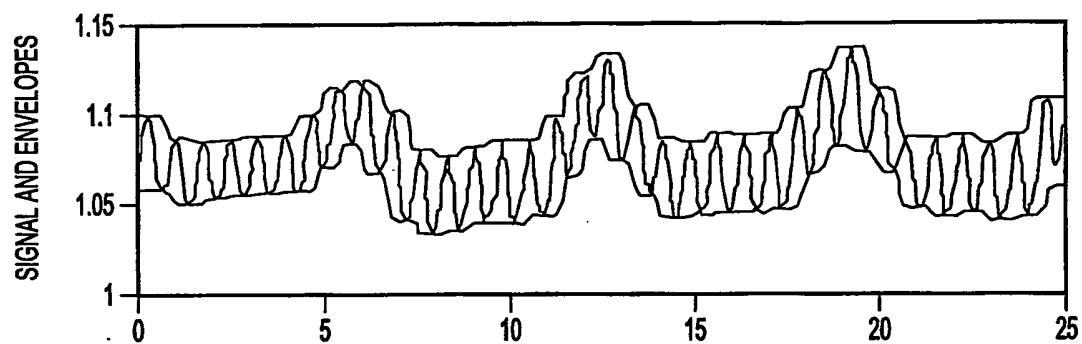


Fig-7A

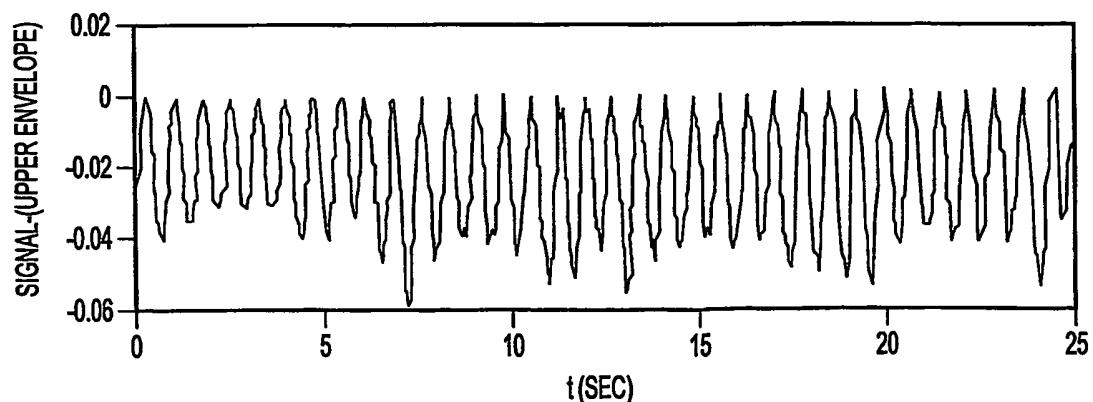


Fig-7B

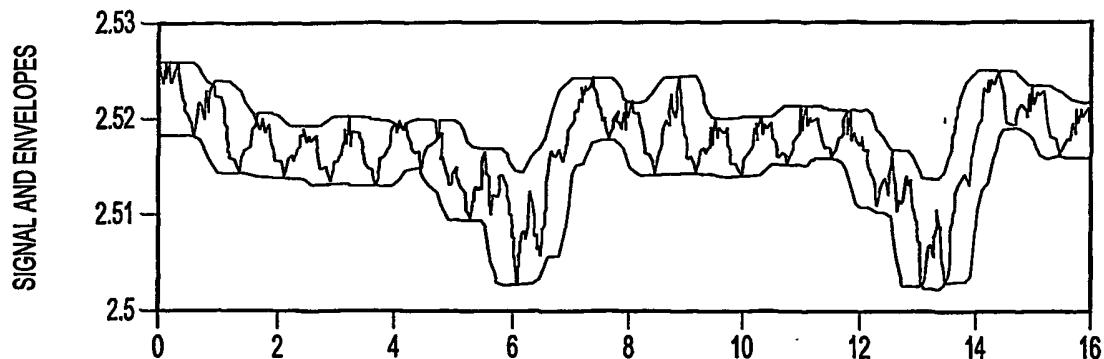


Fig-8A

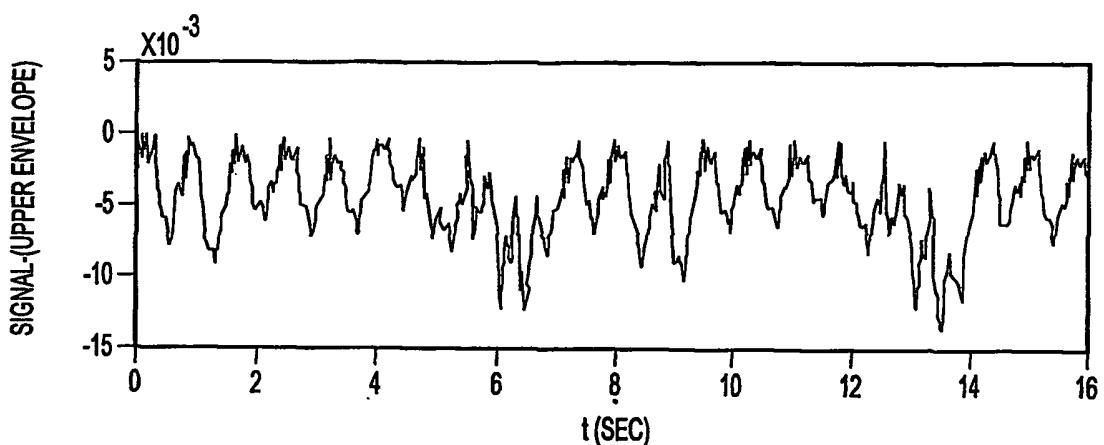


Fig-8B

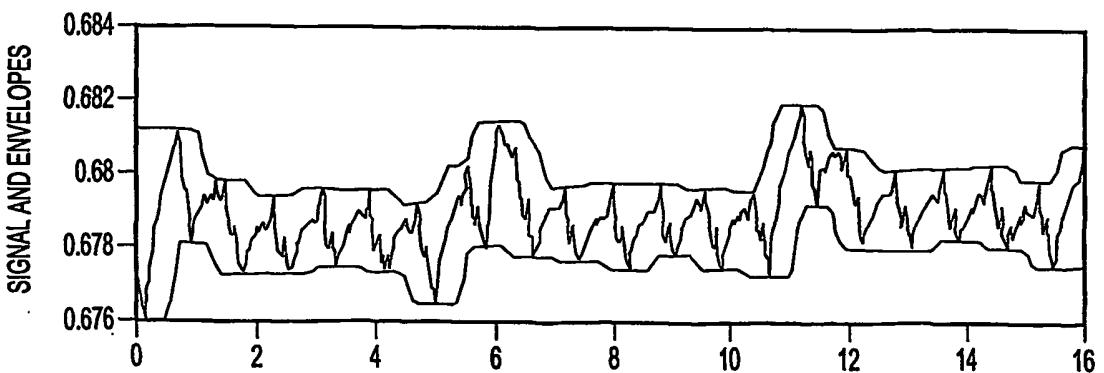
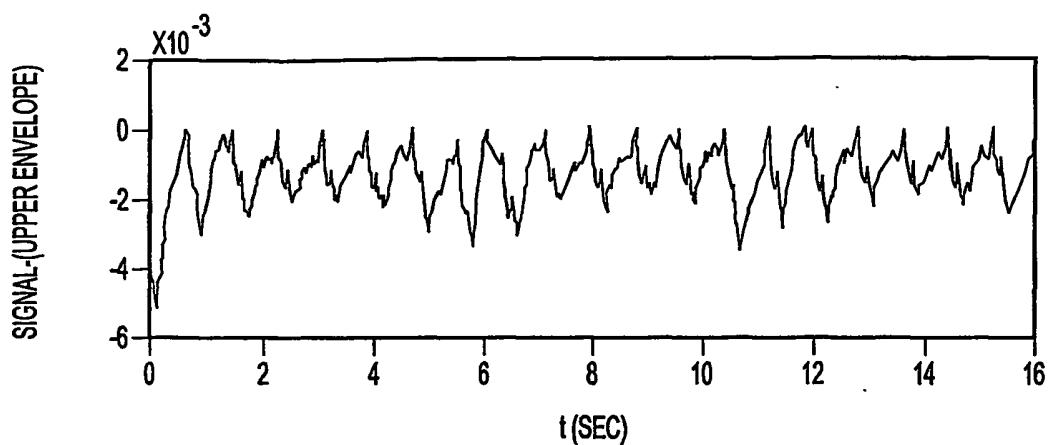
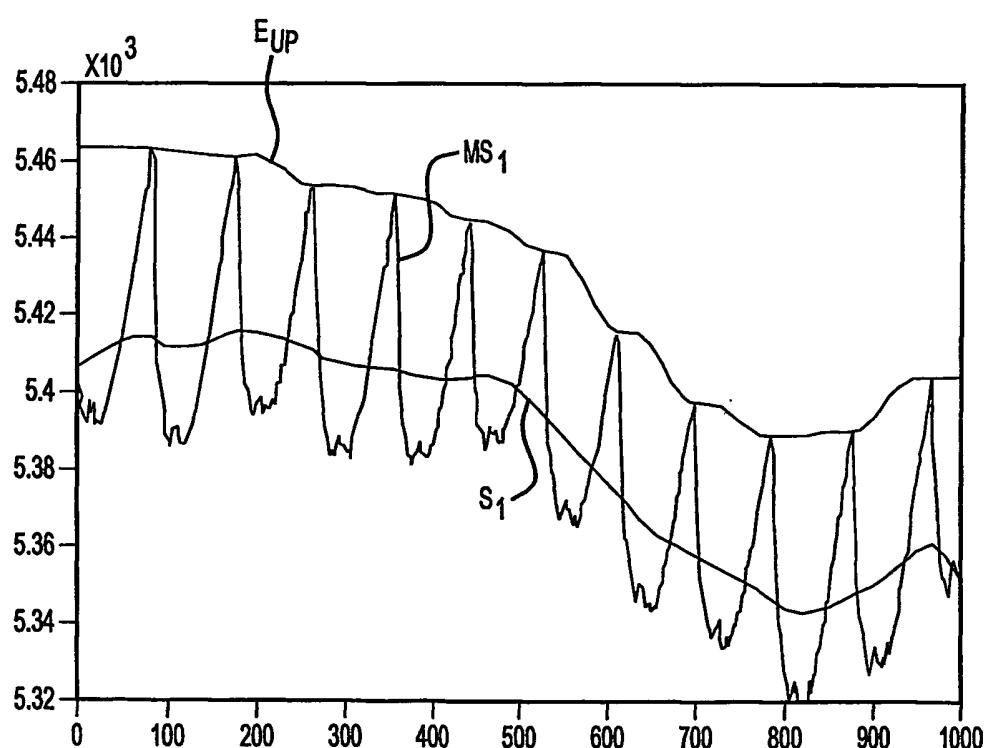


Fig-9A

*Fig-9B**Fig-10*

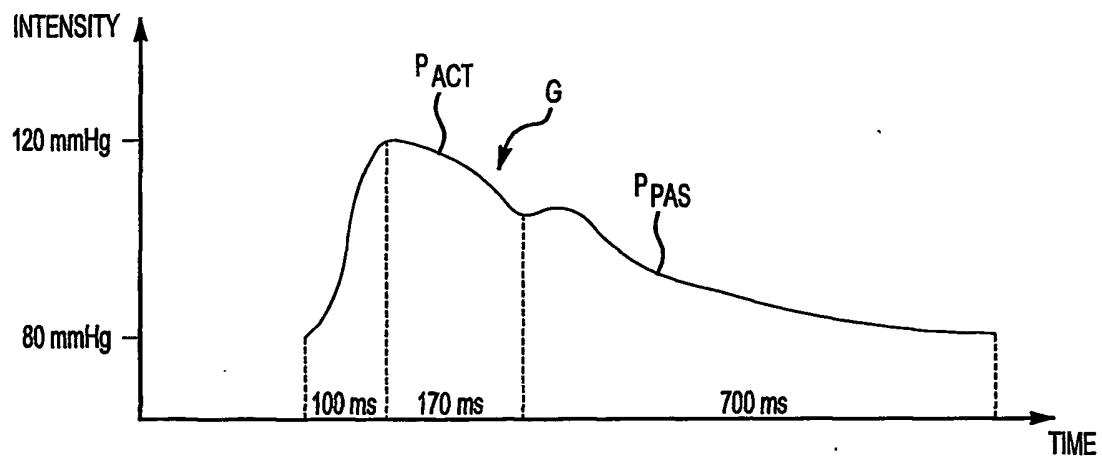


Fig-11

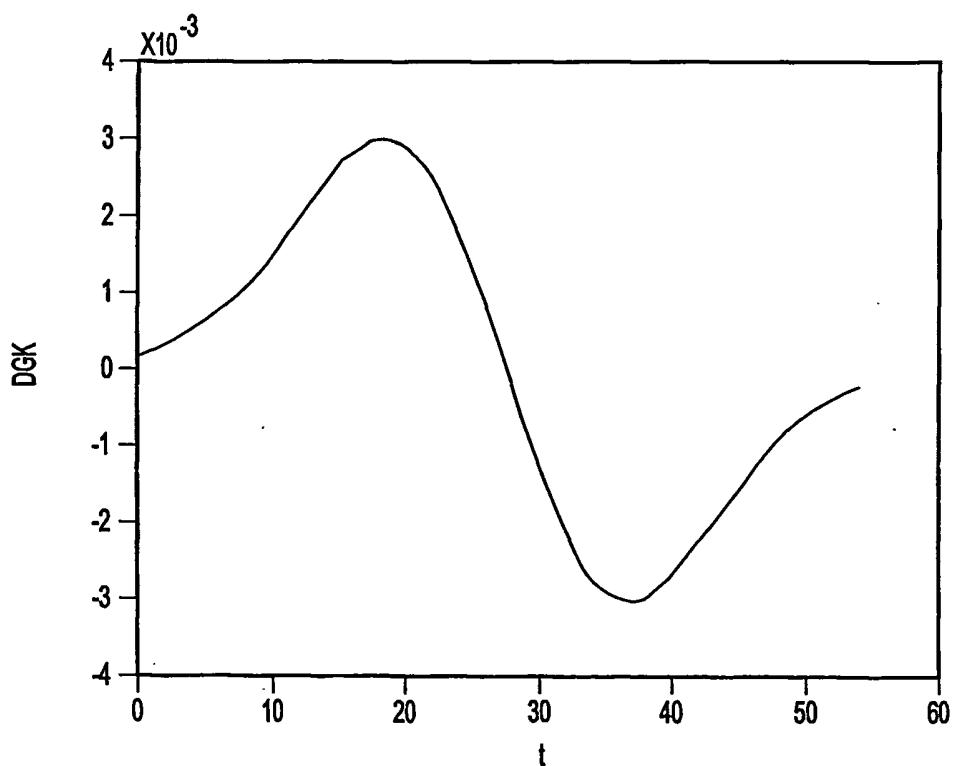


Fig-12

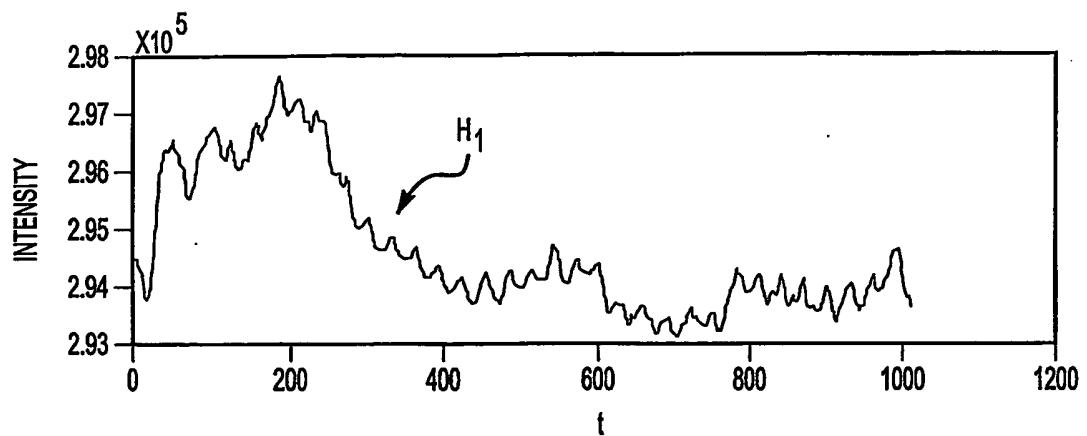


Fig-13A

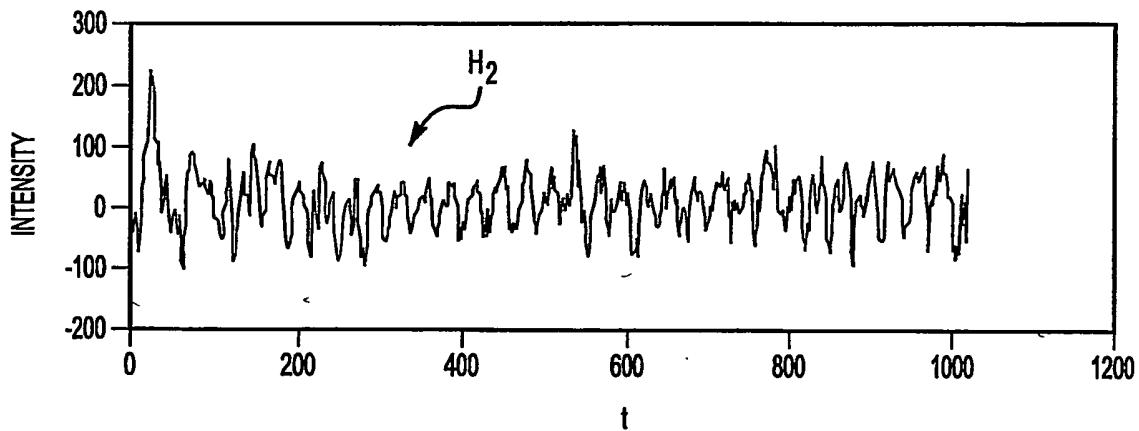


Fig-13B

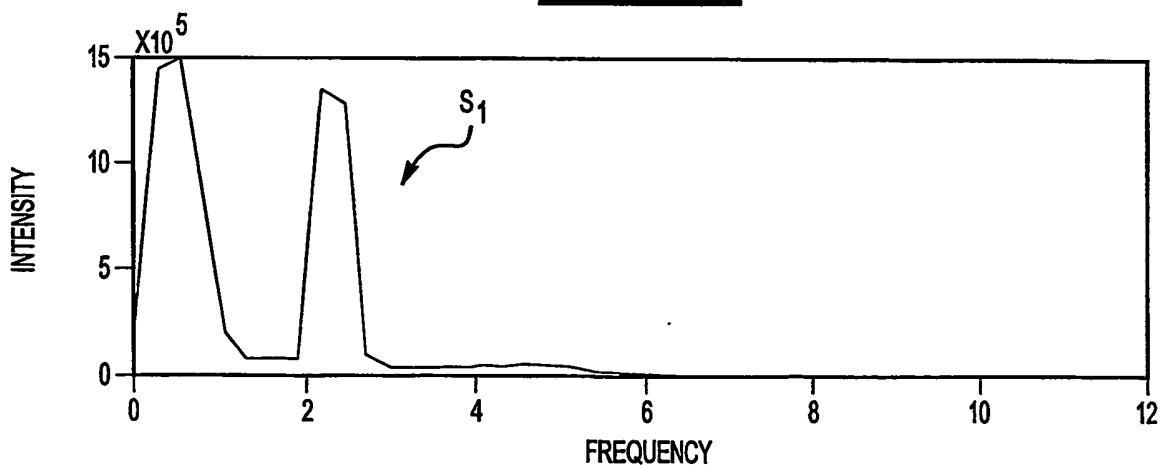


Fig-14A

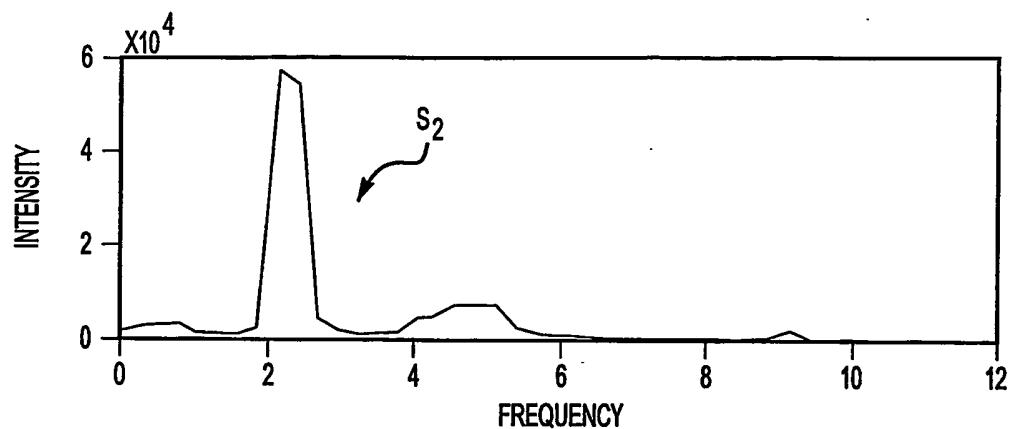


Fig-14B

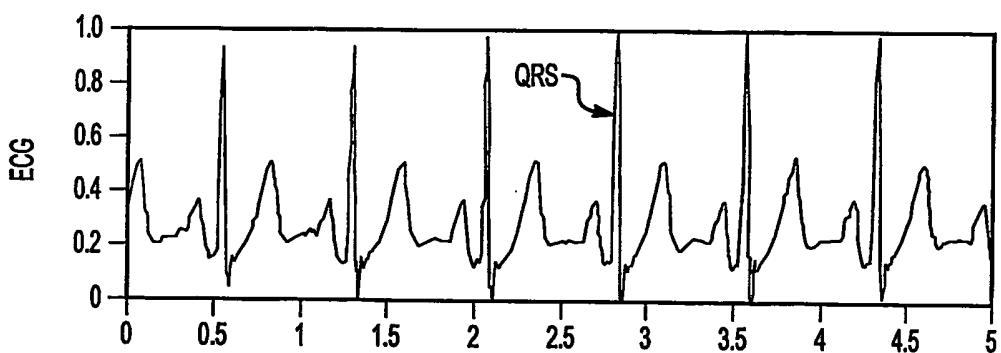


Fig-15A

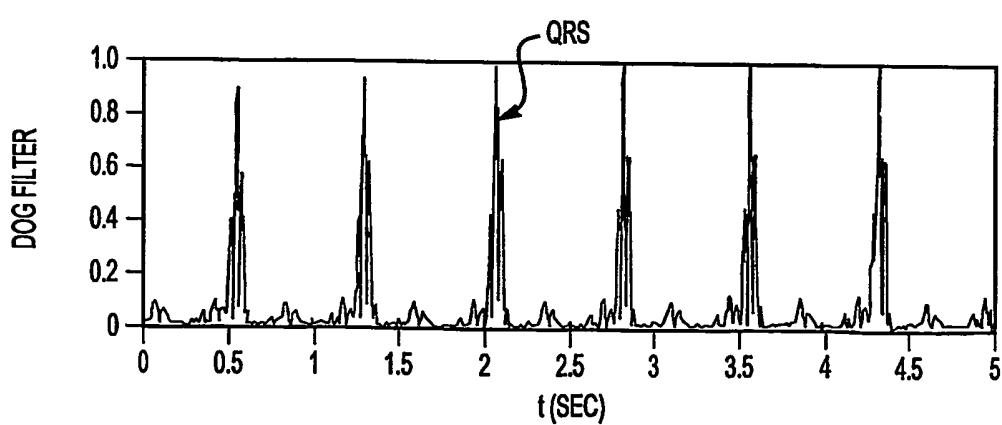


Fig-15B

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5825672 A [0012]
- WO 0032099 A [0019]
- US 5842981 A [0019]
- US 5482036 A [0020]
- US 5490505 A [0020]
- US 5685299 A [0020]
- US 5632272 A [0020]
- US 5769785 A [0020]
- US 6036642 A [0020]
- US 6081735 A [0020]
- US 6067462 A [0020]
- US 6083172 A [0020]

Non-patent literature cited in the description

- **DASSEL et al.** Effect of location of the sensor on reflectance pulse oximetry. *British Journal of Obstetrics and Gynecology*, 1997, vol. 104, 910-916 [0010]
- **DASSEL et al.** Reflectance pulse oximetry at the forehead of newborns: The influence of varying pressure on the probe. *Journal of Clinical Monitoring*, 1996, vol. 12, 421-428 [0011]
- **EDRICH et al.** Fetal pulse oximetry: influence of tissue blood content and hemoglobin concentration in a new in-vitro model. *European Journal of Obstetrics and Gynecology and Reproductive Biology*, 1997, vol. 72 (1), S29-S34 [0012]
- **MENDELSON et al.** Noninvasive pulse oximetry utilizing skin reflectance photoplethysmography. *IEEE Transactions on Biomedical Engineering*, 1988, vol. 35 (10), 798-805 [0013]
- **MENDELSON et al.** Design and evaluation of a new reflectance pulse oximeter sensor. *Medical Instrumentation*, 1988, vol. 22 (4), 167-173 [0015]
- **MENDELSON et al.** Skin reflectance pulse oximetry: in vivo measurements from the forearm and calf. *Journal of Clinical Monitoring*, 1991, vol. 7, 7-12 [0016]
- **TAKATANI et al.** Experimental and clinical evaluation of a noninvasive reflectance pulse oximeter sensor. *Journal of Clinical Monitoring*, 1992, vol. 8, 257-266 [0018]
- **KONIG et al.** Reflectance pulse oximetry - principles and obstetric application in the Zurich system. *Journal of Clinical Monitoring*, 1998, vol. 14, 403-412 [0018]

专利名称(译)	一种用于信噪比改善的信号处理方法和装置		
公开(公告)号	EP1424934B1	公开(公告)日	2008-08-06
申请号	EP2001981641	申请日	2001-10-15
[标]申请(专利权)人(译)	IMAGYN医疗TECH		
申请(专利权)人(译)	IMAGYN MEDICAL TECHNOLOGIES , INC.		
当前申请(专利权)人(译)	CONMED CORPORATION		
[标]发明人	WASSERMAN YORAM		
发明人	WASSERMAN, YORAM		
IPC分类号	A61B5/00 G06F17/00 A61B5/145 A61B5/04 A61B5/053 A61B5/1455		
CPC分类号	A61B5/04017 A61B5/0535 A61B5/1455 A61B5/7239		
优先权	145445 2001-09-13 IL		
其他公开文献	EP1424934A1		
外部链接	Espacenet		

摘要(译)

方法和设备提取是使用两种方法之一的测量信号的信号分量。如果测量信号中的信号分量是具有某个明确定义的峰 - 峰强度值的周期信号，则测量信号的上包络线和下包络线。该信号分量还可用于计算样品的所需参数。信号的DC分量被确定为上包络的中值，并且AC分量被确定为上包络和下包络之间的差的中值。如果测量信号的信号分量是由特定不对称形状表征的周期信号，则对测量信号应用特定自适应滤波，导致信号分量相对于噪声分量的增强。该自适应滤波基于高斯核的导数，其具有与信号分量的特征匹配的特定参数。

$$AC = \text{MEDIAN}(E_{\text{up}} - E_{\text{low}})$$