

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
27 January 2005 (27.01.2005)

PCT

(10) International Publication Number
WO 2005/006956 A2

- (51) International Patent Classification⁷: **A61B**
- (21) International Application Number:
PCT/US2004/022210
- (22) International Filing Date: 9 July 2004 (09.07.2004)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
60/485,979 9 July 2003 (09.07.2003) US
- (71) Applicant (for all designated States except US): **MEDICAL TECHNOLOGIES UNLIMITED, INC.** [US/US]; 9495 Sunset Drive, Suite B 282, Miami, FL 33173 (US).

- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii)) for all designations
- of inventorship (Rule 4.17(iv)) for US only

Published:

- without international search report and to be republished upon receipt of that report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **VITIELLO, Marco, N.** [US/US]; 5825 SW 131 Terrace, Miami, FL 33156 (US). **CYPHERY, Dean** [US/US]; 7504 Rancho Verde-Court NW, Albuquerque, NM 87120 (US). **BUTLER, Lance, H.** [US/US]; 29B North View Trail, Edgewood, NM 87015 (US).
- (74) Agents: **LIPTON, Robert, S.** et al.; Lipton, Weinberger & Husick, 201 North Jackson Street, P.O. Box 934, Media, PA 19063-0934 (US).

(54) Title: COMPREHENSIVE NEUROMUSCULAR PROFILER

(57) Abstract: A Comprehensive Neuromuscular Profiler (CNMP) allows the observation of human and equine muscle functionality and characteristics. The CNMP consists of an integrated system which combines EMG technology, electromagnetic range-of-motion (ROM) technology, and functional capacity sensors. Output signals from the devices are digitized and stored in computer memory. The data may be transmitted to a server computer for further analysis. The server computer examines the data to determine patterns and consults an expert database to determine a diagnosis based on the patterns and combinations of patterns detected.



WO 2005/006956 A2

COMPREHENSIVE NEUROMUSCULAR PROFILER

CROSS-REFERENCE TO RELATED APPLICATIONS

5 This application claims the benefit of U.S. Provisional Patent Application No. 60/485,979 filed on July 9, 2003 entitled Comprehensive Neuromuscular Profiler.

Field of the Invention

10 The Invention relates to the collection of data for an expert diagnostic system, and more specifically, to the collection of data for a comprehensive neuromuscular profiler for monitoring general muscular status and assessing muscle and soft tissue injuries. The Invention is an integrated biomechanical information gathering and expert analysis system for evaluating health and functioning of
15 human muscles and the joints operated by the muscles.

Description of the Related Art

 The range and dynamics of motion of a patient, the strength of the patient's muscles and the electrical characteristics of the muscles provide information useful to a clinician making treatment
20 decisions for a patient. The same information also may be useful to determine the existence, severity or cause of an injury and whether an injury is acute or chronic for purposes of determining questions of insurance or other liability.

 Soft tissue injuries and pathology may occur in any area of the
25 body and may include repetitive stress injuries, injuries to muscles, myofascial injuries, damage to vertebral disks, radiculopathy, and others. These injuries may be difficult to diagnose and hence may be difficult to treat properly.

 Electromyography ("EMG") has proved to be useful in
30 diagnosing some injuries, especially those that are related to repetitive motion. More generally, EMG is useful in diagnosing injuries which can be identified from the examination of static muscle activity. However, EMG cannot provide a comprehensive examination of muscular compensation patterns. These patterns are
35 a key aspect of identifying and properly diagnosing myofascial injuries.

Range-of-motion ("ROM") testing has also been used to identify injury by examining the characteristics of dynamic muscle activity. However, like EMG testing, ROM testing has limitations in providing a full examination of compensation patterns, and is not
5 adequately effective as a stand-alone method for injury diagnosis.

There have been attempts to integrate EMG and ROM technology to provide a more comprehensive diagnosis process.

Summary of the Invention

The Invention integrates several muscle and joint monitoring
10 measurements into a single apparatus so that an expert diagnosis may be provided based on the data collected by the apparatus. The apparatus gathers four types of information, which may be collected simultaneously or serially: motion, video, muscle capacity and electromyography ("EMG").

15 Motion information is collected by remote sensing technology. A suitable technology is pulsed DC magnetic field sensing, although other sensing technologies such as optical sensing or AC magnetic field sensing may be used. In pulsed DC magnetic field sensing, an electromagnetic transmitter generates a pulsed electromagnetic field.
20 One or more ROM sensors, each comprising three axis ring-core flux-gate magnetometer, are attached to the patient. Changes in the electromagnetic field are detected by the ROM sensors. The detected changes in the electromagnetic field are measured and analyzed by a ROM signal processor, which translates the ROM
25 signal from the ROM sensors into information defining the position and motion of the ROM sensors and hence of the patient. The motions measured include the range of motion ("ROM") and also may include the dynamic motion of the patient within the ROM.

Muscle strength measurements are collected by having the
30 patient exert force using the muscle in question against a fixed object and measuring the force exerted by the muscle. Grip strength, finger pinch strength and isometric functional test measurements are made by having the patient grip, pinch or otherwise exert force on the appropriate sensors. EMG
35 measurements are collected by attaching electrodes (referred to in this application as "EMG sensors") to the patient and recording electrical activity of the muscles in question.

The signals collected from the various sensors are digitized and recorded in the memory of a client computer. The client computer may communicate the data to a server computer over a computer network. Software resident in the server computer
5 includes an expert system that evaluates the data for patterns and for combinations of patterns among the types of data collected. The server computer is programmed to compare the patterns, or lack of patterns, detected in the data to predetermined patterns associated with injuries, pathologies, and lack of injuries and pathologies. The
10 expert system may diagnose, for example, sprains, strains, vertebral disk injury and radiculopathies. The expert system also may determine whether the injury is of recent origin, thereby distinguishing acute from chronic injury. The expert system may look for changes in other muscles or behaviors compensating for
15 pain or loss of use as the result of pathology or injury. An issue with the interpretation of EMG results historically has been the variability in interpretation among different healthcare professionals. The expert system serves to resolve that variability and to achieve consistency of interpretation. The server computer assigns a patient
20 profile to the patient based on the diagnosis made by the server computer. The server computer may communicate the patient profile to the client computer for display to the user. Alternatively, the patient profile may be communicated to any other authorized person. The functions of the client and server computers may be
25 integrated into a single stand-alone computer.

The client computer is programmed to administer any of several "protocols" to the patient and to record the resulting data. A "protocol" is a sequence of tasks, or tests, that the patient performs while the appropriate sensors collect data concerning the portion of
30 the patient's body in question. Each protocol specifies the identity, number and location of the sensors to be used. The client computer is programmed to provide step-by-step instructions to the patient and to the technician, or user, administering the protocol to the patient. The client computer is programmed to collect and record
35 the appropriate sensor data for each protocol. For purposes of this application, the specific data specified to be collected for a particular protocol is referred to as "protocol data."

As used in this application, the term "client computer" means any computer or system of computers capable of communicating with another computer over a computer network. The term "server computer" means any computer or system of computers that is
5 capable of receiving a communication over a computer network from a client computer and performing an evaluation based on the received communication.

The apparatus may be equipped with automated, interactive instructions to an operator who has no or little knowledge of
10 anatomy. The apparatus therefore may be operated at a relatively modest cost. The apparatus may be equipped with a video camera or other remote imaging technology to allow a physician or other medical personnel to remotely monitor the procedure and to create a visual record of the tests performed and the patient's response to
15 the tests. The apparatus may be equipped with the capacity to automatically generate billing forms or electronic files, such as the HCFA form or file.

The server computer may be programmed to generate appropriate billing files or forms and to transmit those billing files or
20 forms to a payor. The server computer also may be programmed to compare the patient profile assigned to a patient to predetermined criteria for disability ratings.

Brief Description of the Drawings

The accompanying drawings, which are incorporated in and
25 form a part of the specification, illustrate the embodiments of the present invention and, together with the description, serve to explain the principles of the invention.

Fig. 1 is block diagram of the Invention and the information collected by the Invention.

30 Fig. 2 is a schematic diagram of the connection of the client computer to the server computer.

Fig. 3 is a schematic diagram of the collection of EMG data.

Fig. 4 is a schematic diagram of the collection of ROM data.

35 Fig. 5 is a schematic diagram of the collection of isometric function data.

Fig. 6 is a schematic diagram of the collection of grip data.

Fig. 7 is a schematic diagram of the collection of pinch data.

Fig. 8 is a block diagram of signal flow through the CNMP housing.

Fig. 9 is a block diagram of the signal conditioning and conversion circuit

5 board.

Fig. 10 is a block diagram of information flow through the client computer and server computer.

Fig. 11 is a flowchart of the select patient function of the client computer software.

10 Fig. 12 is a flowchart of the new patient function of the client computer software.

Fig. 13 is a flowchart of the zoom patient protocol function of the client computer software.

15 Fig. 14 is a flowchart of the run test function of the client computer software.

Fig. 15 is a flowchart of the upload data function of the client computer software.

Fig. 16 is a flowchart of the download data function of the client computer software.

20 Fig. 17 is a flowchart of the 'about' function of the client computer software.

Fig. 18 is a flowchart of the 'quit' function of the client computer software.

Fig. 19 is a flowchart of the server computer analysis.

Description of the Preferred Embodiment

As shown by Fig. 1, the 'Comprehensive Neuromuscular Profiler' ("CNMP") 2 of the present invention is an integrated data acquisition device for detecting, recording and analyzing information relating to a patient. The CNMP 2 comprises surface electromyography ("EMG") sensors 4, range of motion ("ROM") sensor 6, grip strength sensor 8, finger pinch strength sensor 10, isometric function capacity sensor 12, and a video camera 14, all connected to the client computer 34. The sensors respectively generate EMG signals 16, ROM signal 18, grip signal 20, pinch signal 22, isometric function signal 24 and video information 26. Signals generated by the sensors are conveyed to a CNMP housing 28. In the CNMP housing 28, the EMG signals 16, isometric function signal 24, grip signal 20 and pinch signal 22 are processed and digitized to become EMG data, isometric function data, grip data and pinch data, referred to collectively in this application as "CNMP data" 30. The ROM signal 18 also is processed in the CNMP housing 28 to become ROM data 32. The video information 26 from the video camera 14 is passed directly to a first client computer 34, which may be a personal computer. CNMP data 30 and ROM data 32 are transmitted from the CNMP housing 28 to the first client computer 34. The CNMP data 30, ROM data 32 and video information 26 may be transmitted to a server computer 36 over a network 38.

As illustrated by Fig. 2, the server computer 36 evaluates the CNMP data 30 and ROM data 32. The server computer 36 assigns a patient profile 40 to the patient based on the evaluation and transmits the patient profile 40 to a second client computer 35 for display 42 to an authorized user such as an insurer or employer. Alternatively, some or all of the data analysis may be performed by the first client computer 34 and some or all of the generation of patient profile 40 may occur within the first client computer 34.

Generation of EMG signal 16 by the EMG sensors 4 is illustrated by Fig. 3. As shown by Fig. 3, a grounding sensor and one or more differential pairs of EMG sensors 4 are attached to predetermined locations 44, as specified in Table 1 below, on patient 46. A total of thirty-six EMG sensors 4 (18 signal pairs) may be

attached to the patient **46** using techniques well known in the art. An EMG sensor **4** is connected by EMG cable assembly **48** to CNMP housing **28**. Two EMG cable assemblies **48** are provided. Each EMG cable assembly **48** is conventional and comprises nineteen
5 individual coaxial sensor cables (9 pairs of differential leads) plus a single ground sensor. Each EMG cable assembly **48** is able to accommodate nine EMG signal pairs and the ground sensor **4** and is capable of conveying these nine separate EMG signal pairs **16**. Each coaxial cable is shielded to help eliminate any cross channel noise.
10 The CNMP housing **28** is capable of processing each of the eighteen channels of EMG signals **16** generated by the EMG sensors **4** and samples the EMG signals **6** at a rate of 15 KHz. The Invention is not limited to thirty-six EMG sensors **4** (18 pairs), and any number of EMG sensors **4** may be utilized.

15 The appropriate number of EMG sensors **4** is specified for each test to be performed on patient **46**. The EMG sensors **4** are conventional silver chloride electrodes. Pairs of EMG sensors **4** are selected for each predetermined location **44** on the patient **46**. The predetermined locations **44** on the patient **46** are selected to provide
20 EMG signals **4** relating to the muscles in question and relating to muscles that may be compensating for the muscles in question.

Fig. 4 illustrates generation of a range-of-motion ("ROM") signal **18**. A ROM transmitter **50** creates an electromagnetic field **52** in the vicinity of patient **46**. A ROM sensor **6** is attached to the
25 body of patient **46** at a ROM sensor predetermined location **56**, as specified in Table 2, below. The ROM sensor **6** generates a ROM signal **18** in response to a position of the ROM sensor **6** within the electromagnetic field **52**. The ROM sensor **6** is connected by a ROM sensor cable **58** to the CNMP housing **28**. A ROM signal processor
30 **60**, as shown by Fig. 8, processes the ROM signal **18** into ROM data **32**.

The electromagnetic field **52** generated by the ROM transmitter **50** is a DC-based pulsed electromagnetic field. A single ROM sensor **6** is adequate for purposes of the Invention, although
35 any number of ROM sensors **6** may be used. The ROM sensor **6** attached to the patient **46** contains circuitry that relays the position of the ROM sensor **6**, and hence the position of the patient's **46**

body to which the ROM sensor **6** is attached, in the electromagnetic field **52**. The position of the ROM sensor **6** and of the patient **46** are represented through position and angular movements in six degrees of freedom: x, y, z, pitch, roll, and yaw. The ROM sensor **6**
5 operates at a frequency of 100 Hz or more, although any suitable frequency may be used.

A suitable ROM transmitter **50**, ROM sensor **6** and ROM signal processing unit **60** is the Nest of Birds™ pulsed DC electromagnetic sensing product available from Ascension Technology Corporation,
10 P.O. Box 527, Burlington, Vermont 05402. The Internet address of Ascension Technologies is www.ascension-tech.com.

Other ROM sensing technologies may be suitable, such as AC electromagnetic sensing or optical sensing. Pulsed DC electromagnetic sensing offers advantages over these technologies.
15 Optical sensing requires that a clear line of sight be maintained, which is not required in magnetic sensing. AC electromagnetic sensing involves a rapidly-fluctuating magnetic field, which induces eddy currents in conductive materials in the electromagnetic field. The eddy currents introduce interference and noise into the data and
20 environment, greatly increasing electromagnetic interference issues with other equipment in the general vicinity of the CNMP. Pulsed DC electromagnetic sensing reduces the problem of eddy currents, although stray magnetic fields and nearby metallic objects can reduce the performance of the pulsed DC system.

25 As used in this application the term "remote sensing technology" means any technology involving the location of a detector with respect to a source of energy or in an energy field. The term "remote sensing technology" includes pulsed DC electromagnetic sensing, as described above, AC electromagnetic
30 sensing, optical sensing, and any other position sensing technology that involves location of a detector with respect to an energy source or an energy field.

Fig. 5 illustrates the generation of an isometric function signal **24** from a isometric function sensor **12**. The isometric function
35 sensor **12** comprises a footplate **62** and a strain gauge **64** mounted on the footplate **62**. A cord **66** is attached to strain gauge **64** and a handle **68** is attached to cord **66**. The patient **46** stands on the

footplate **62** and pulls upward on the handle **68**, exerting a force on cord **66** and hence on strain gauge **64**. Strain gauge **64** generates an isometric function signal **24** in response to force exerted by patient **46**.

5 A suitable strain gauge **64** is an S-beam load cell, model L2350, from Futek Advanced Sensor Technology ("Futek"), **10** Thomas, Irvine, CA 92618. The strain gauge **64** has a rated capacity of 300 pounds of force and can detect increments of .3 pounds of force. The isometric function signal **24** varies between
10 -2.5 and +2.5 volts, depending on the force exerted on the strain gauge **64**.

 Isometric function signal **24** is conveyed by isometric function cable **70** to CNMP housing **28**. The isometric function signal **24** is processed to isometric function data within the CNMP housing by a
15 single channel, which operates at 100 Hz or more, but which may be operated at any suitable frequency.

 Fig. 6 illustrates generation of the grip strength signal **20** by the grip strength sensor **8**. The patient **46** grips the grip strength
20 sensor **8** in his or her hand and exerts as much gripping force as possible. A pressure transducer within the grip strength sensor **8** generates the grip strength signal **20**, which may vary between -2.5 and +2.5 volts, depending on the gripping force exerted by patient **46**. The grip strength signal **20** is transmitted through grip
25 sensor cable **74** to the CNMP housing **28**. The grip strength signal **20** is converted to grip data within the CNMP housing **28** by a single channel that operates at a frequency of 100 Hz or more, but which may operate at any suitable frequency. A suitable grip strength sensor **8** is the Jamar Grip Strength Gage model 5030PT
30 manufactured by Sammons Preston, Inc. The internet address for Sammons Preston is www.sammonspreston.com.

 Fig. 7 illustrates generation of the pinch strength signal **22** by the pinch strength sensor **10**. The patient **46** pinches the pinch strength sensor **10** between a thumb and a finger. The pinch
35 strength sensor **10** generates a pinch strength signal **22** in response to the force applied by the patient **46** to the pinch strength sensor **10**. A suitable pinch sensor **10** is model L1020-Q10510 from Futek.

The pinch strength signal **22** varies between -2.5 to $+2.5$ volts, depending on the force exerted on the pinch strength sensor **10** by the patient **46**. The pinch strength signal **22** is transmitted through the pinch strength sensor cable **72** to the CNMP housing **28**. The
5 pinch strength signal **22** is processed within the CNMP housing **28** by a single channel that operates at a frequency of 100 Hz or more, but which may operate at any suitable frequency.

As shown by Figs. 3 through 7, video camera **14** records video images of the patient **46** while any or all of EMG sensors **4**,
10 ROM sensor **6**, grip strength sensor **8**, pinch strength sensor **10** or isometric function sensor **12** are in use. The video camera **14** generates video information **26** that is transmitted through video cable **76** to the first client computer **34**. The video information **26** is passed into a PCMCIA card acting as a USB hub and is stored for
15 future reference. The video information **26** may be monitored by a healthcare provider during the tests and may be stored as a visual record of the tests.

Fig. 8 illustrates the operations occurring in the CNMP housing **28**. ROM signal **18** enters CNMP housing **28** by way of a suitable
20 input jack and is conveyed to ROM signal processing device **60**. ROM signal processing device **60** converts ROM signal **18** to ROM data **32**, ready for further processing by first client computer **34**. As indicated above, a suitable ROM signal processing device **60** is the Nest of Birds™ product by Ascension Technologies Corporation.
25 ROM data **32** is conveyed to a suitable output jack.

Isometric function signal **24**, grip signal **20** and pinch signal **22**, each appearing as a single channel, enter the CNMP housing **28** through suitable input jacks and are processed by signal conditioning and conversion board **78**. Two EMG cable assemblies **48** are
30 connected to the CNMP housing **28** by suitable jack connections, each of the EMG cable assemblies **48** is able to convey nine channels of EMG signal **16** from eighteen separate EMG sensors **4**. Each channel of EMG signal **16** is processed by the signal conditioning and conversion board **78**. The output of the signal
35 conditioning and conversion board **78** is CNMP data **30** comprising EMG data **82**, isometric function data **84**, grip data **86** and pinch

data **88**, all ready for further processing by client computer **34**.
CNMP data **30** is output at a suitable output jack.

Fig. 9 illustrates operation of the signal conditioning and conversion board **78**. The signal conditioning and conversion board
5 **78** conditions EMG signal **16**, isometric function signal **24**, pinch signal **22**, and grip signal **20** and converts those signals **16**, **24**, **22**, **20** to digital form to be used by the client computer **34** for further processing and analysis.

A shown by Fig. 9, The EMG section of the signal conditioning and conversion board **78** begins with the EMG cable assemblies **48**
10 being fed into an input protection device **90** in order to isolate any high voltage that is potentially dangerous. The resulting signals are sent through an amplification and filtering module **92**. The EMG signals **16** are converting to a corresponding voltage, based on the resistance between the EMG sensor **4** pairs. The filtering module **92**
15 provides 60Hz filtering, with a common mode rejection ratio of 90dB at a range of 0-100Hz. The resulting signals are fed through analog multiplexers **94**, in order to account for the numerous channels of the surface EMG signal **16**. The multiplexers **94** are controlled by a
20 master timing and control mechanism **96**, which allows a consistent pass-through of signals through the multiplexer **94** array.

Once the processed EMG signals **16** are passed through the multiplexers **94**, the signals **16** are sent through an analog-to-digital converter circuit **98**, which changes the EMG signals **16** signals to a
25 digital EMG data **82** in order to prepare the EMG signals **16** for further processing in client computer **34**.

The grip, pinch, and functional capacity section of the signal conditioning and conversion board **60** begins with the grip strength sensor cable **74**, pinch strength sensor cable **72** and isometric
30 function sensor cable **70** feeding the grip signal **20**, pinch signal **22** or isometric function signal **24** into an amplification and bridge gain circuit **100**. The differential grip signal **20**, pinch signal **22** or isometric function signal **24** is converted into a corresponding voltage. The bridge gain circuit **100** also provides a DC amplification
35 voltage along with an isolated ground component to provide sensor bridge amplification. The resulting processed grip signal **20**, pinch signal **22** or isometric function signal **24** is fed through analog

multiplexers **102, 94**, in order to account for the numerous channels of EMG signal **16**. The multiplexers **102, 94** are controlled by a master timing and control mechanism **96**, which allows a consistent pass-through of signals through the multiplexer **102, 94** array.

5 Once the processed grip signal **20**, pinch signal **22** or isometric function signal **24** is passed through the multiplexer array **102, 94**, the signal is sent through an analog-to-digital converter circuit **98**, which changes the grip signal **20**, pinch signal **22** or isometric function signal **24** to a digital grip data **86**, pinch data **88**
10 or isometric function data **84** in order to prepare the grip signal **20**, pinch signal **22** or isometric function signal **24** for further processing by first client computer **34**.

 The system voltages component **104** of the signal conditioning and conversion board **60** is a stand-alone power supply.
15 The system voltages component **104** operates at a constant voltage of 5 volts at a current of 2 amps. The system voltages component **104** also contains a differential voltage of -1.2 to $+12$ volts at an approximate current of 0.4 amps. The resulting signals from the power supply are fed into a multiplexer **106** for distribution in the
20 circuit.

 All of the resulting digital EMG data **82**, grip data **86**, pinch data **88** and isometric function data **84** from the analog-to-digital converters **98** are passed on to a parallel-to-serial converter **108**, which prepares the output of the converters **108** to be sent over a
25 standard USB interface to the first client computer **34**. The resulting EMG data **82**, grip data **86**, pinch data **88** and isometric function data **84** are subject to a digital isolation circuit **110**, in order to isolate the patient **46** and other participants from the signal conditioning and conversion board **78**. The EMG data **82**, grip data
30 **86**, pinch data **88** and isometric function data **84** are sent from the signal conditioning and conversion board **78** over a USB interface into a USB port on the first client computer **34**.

 Fig. 10 illustrates the flow of information from the CNMP housing **28**. From the CNMP housing **28**, ROM data **32** and CNMP
35 data **30** are fed to first client computer **34**. CNMP data **30** comprises EMG data **82**, grip data **86**, pinch data **88** and isometric function data **84**. Video information **26** also is fed to the first client

computer **34**. First client computer **34** memory **112** contains first client computer software **114** that controls operation of first client computer microprocessor **116**. In response to appropriate commands from a user, first client computer microprocessor **116**
5 directs storage of ROM data **32**, video information **26** and CNMP data **30** in first client computer memory **112**. Instructions and other information are displayed to user by display **42**.

On instruction from user, first client computer microprocessor **116** may connect to computer network **38** and negotiate a network
10 connection with server computer **36**. First client computer microprocessor **116** may direct that ROM data **32**, video information **26** and CNMP data **30** be sent to server computer **36** over computer network **38** in an encrypted format to protect patient information.

Server computer **36** includes server computer microprocessor
15 **118** and server computer memory **120**. Server computer memory **120** contains an expert database **122**. Server computer microprocessor **118** is programmed to analyze ROM data **32** and CNMP data **30** and to extract patterns from these data. Server computer microprocessor **118** compares the patterns detected to
20 expert database **122** and associates a patient profile **40** with the detected patterns. Server computer **36** may transmit the patient profile **40** to the first client computer **34** over network **38** for display **42** to user. Alternatively, server computer **36** may transmit patient profile **40** over computer network **38** to the second client computer
25 **35** for display to any authorized person, such as an insurer or employer.

Figs. 11-17 describe the operation of first client computer software **114**. The software **114** is resident in the first client computer memory **112** and operates the comprehensive
30 neuromuscular profiler system. In overview, the first client computer software **114** allows a user to select or to enter information about a patient **46** into the first client computer memory **112**. The first client computer software **114** allows the user to select among several different protocols for tests to be administered to a patient
35 **46**. Each protocol is designed to collect information about the functioning of a particular portion of the patient's **46** body. The first client computer software **114** allows first client computer **34** to

display to the user or to the patient **46** information about a selected protocol, including which of the EMG sensors **4**, ROM sensor **6**, isometric function sensor **12**, grip strength sensor **8** or pinch strength sensor **10** should be used during each portion of the
5 protocol. The first client computer software **114** may instruct the user as to the correct location and placement of the EMG sensors **4** and ROM sensor **6**. The first client computer software **114** may instruct the patient as to the correct performance of each task in the selected protocol.

10 The first client computer software **114** oversees collection of the appropriate EMG data **82**, ROM data **32**, grip data **86**, pinch data **88** and isometric function data **84** and also oversees recording of video information **26**. The first client computer software **114** allows first client computer **34** to transmit CNMP data **30**, ROM data **32**
15 and video information **30** to a server computer **36** over computer network **38**. The first client computer software may allow first client computer to receive the patient profile **40** from the server computer **36** after completion of the analysis by the server computer **36**.

20 Each of the above steps relating to the first client computer software **114** is described in more detail in the following paragraphs.

A first client computer **34** running the client computer software **114** displays a 'main' screen **124** to a user. The user is a technician who administers the test protocols to the patient **46**. The
25 user is presented with several options on the Main screen **124**, and the user may select any of the options using any of the techniques that are well known in the art.

As shown by Fig. 11, from the Main screen **124** the user may select the "open patient" option **126**. The user is presented with a
30 select patient screen **128** that allows the user to select the identity of the patient **46** (either by name or by some other unique identifier) from a list of patient **46** identities. Patient **46** information includes identifying information for the patient **46** and such other information as is deemed necessary, which may include insurance information,
35 diagnosis information, prior test results, and any other information that may be desirable. Patient **46** information is stored in encrypted form on the first client computer memory **112**. The user selects **130**

one of the unique patient identifiers and the patient **46** information for that patient **46** is decrypted and displayed **132** to the user in one or more screens. The user then may edit or add to the patient information **134**, including performing additional protocols as
5 described below. After the entry of new patient information is completed, the user may elect to save **136** the new patient information, in which case the patient information is encrypted and saved **138** to the hard disk. Alternately, the user may elect to cancel **140** the entry of patient information at any time and return to
10 the Main menu. The user also may clear patient information **142** entered without returning to the main menu. The user may elect to cancel opening of a patient file **144**, in which case existing patient files are not amended.

As shown by Fig. 12, the user may enter information
15 concerning a new patient for whom no file is saved within the computer system. From the Main menu **124**, the user selects "new patient" **144**. The user is presented with patient information screens with the fields blank **146**. The user then enters information into the blank fields, as appropriate **148**. The information entered may
20 include new protocol data derived from the administration of a protocol to the patient, as discussed below. Once the entry of the new patient information **148** is complete, the user may elect to save the information **150**. The information is then encrypted and saved to the hard disk drive **152** of the first client computer **34**. The user
25 also may elect to clear the new patient information **154** or to cancel the operation **156** and return to the main screen.

Fig. 13 shows the "Zoom patient protocol" option presented to the user by the Main menu **124**. As used in this application, the term "zoom" means to selectably enlarge an image on the display
30 screen. For the "zoom patient protocol," the user is presented with an image of a region on the human body. The user selects **158** the region of the human body corresponding to the protocol to be administered to the patient. The image of the body region selected "zooms" **160**; that is, enlarges, on the display monitor **42**. The
35 proper location of the EMG sensor **4** locations for the selected patient protocol are illustrated on the enlarged image of the body and a list of the muscles to be monitored is displayed to the user.

Eight different protocols are available to the user, and hence eight different locations may be "zoomed" 160. Those protocols are as follows: Cervical, Thoracic, Lumbosacral, Carpal Tunnel, Shoulder, Lower Extremities, Custom Ankle, and Hip & Groin. Each of the protocols provide EMG sensor 4 locations for the left and the right sides of the patient's 46 body, resulting in a total of sixteen different sets of EMG sensor locations 44. The appropriate EMG sensor locations 44 for the eight protocols are contained in Table 1.

TABLE 1

10

ELECTRODE PLACEMENTS

CERVICAL PROTOCOL

RIGHT

CH1:	Right Sternocleidomastoid
CH2:	Right Scalene
CH3:	Right Paracervical
CH4:	Right Upper Trapezius

LEFT

CH10:	Left Sternocleidomastoid
CH11:	Left Scalene
CH12:	Left Paracervical
CH13:	Left Upper Trapezius

**THORACIC
PROTOCOL**

RIGHT

CH1:	Right Middle Trapezius
CH2:	Right Lower Trapezius
CH3:	Right Paraspinal T5-T8
CH4:	Right Paraspinal T8-T12
CH5:	Right Latissimus Dorsi
CH6:	Right Serratus Posterior Inferior

LEFT

CH10:	Left Middle Trapezius
CH11:	Left Lower Trapezius
CH12:	Left Paraspinal T5- T8
CH13:	Left Paraspinal T8- T12
CH14:	Left Latissimus Dorsi
CH15:	Left Serratus Posterior Inferior

**LUMBOSACRA
L PROTOCOL**

RIGHT

CH1:	Right Paraspinal L1-L3
CH2:	Right Paraspinal L5-S1
CH3:	Right Quadratus Lumborum
CH4:	Right Gluteus Maximus
CH5:	Right Rectus Abdominis
CH6:	Right Abdominal Oblique
CH7:	Right Hamstring

LEFT

CH10:	Left Paraspinal L1-L3
CH11:	Left Paraspinal L5-S1
CH12:	Left Quadratus Lumborum
CH13:	Left Gluteus Maximus
CH14:	Left Rectus Abdominis
CH15:	Left Abdominal Oblique
CH16:	Left Hamstring

**CARPAL
TUNNEL
PROTOCOL**
RIGHT

CH1:	Right Sternocleidomast oid
CH2:	Right Scalene
CH3:	Right Paracervical
CH4:	Right Upper Trapezius
CH5:	Right Deltoid
CH6:	Right Biceps
CH7:	Right Triceps
CH8:	Right Wrist Flexor/Extensor
CH9:	Right Thenar/Palmer

LEFT

CH10:	Left Sternocleidomastoid
CH11:	Left Scalene
CH12:	Left Paracervical
CH13:	Left Upper Trapezius
CH14:	Left Deltoid
CH15:	Left Biceps
CH16:	Left Triceps
CH17:	Left Wrist Flexor/Extensor
CH18:	Left Thenar/Palmer

**SHOULDER
PROTOCOL**
RIGHT

CH1:	Right Scalene
CH2:	Right Paracervical
CH3:	Right Upper Trapezius
CH4:	Right Pectoralis Major
CH5:	Right Supraspinatus
CH6:	Right Teres

LEFT

CH10:	Left Scalene
CH11:	Left Paracervical
CH12:	Left Upper Trapezius
CH13:	Left Pectoralis Major
CH14:	Left Supraspinatus
CH15:	Left Teres Major

	Major
CH7:	Right Latissimus Dorsi
CH8:	Right Deltoid
CH9:	Right Biceps

CH16:	Left Latissimus Dorsi
CH17:	Left Deltoid
CH18:	Left Biceps

**LOWER
EXTREMITIES
PROTOCOL**

RIGHT

CH1:	Right Quadriceps
CH2:	Right Hamstring
CH3:	Right Tibialis Anterior
CH4:	Right Gastrocnemius

LEFT

CH10:	Left Quadriceps
CH11:	Left Hamstring
CH12:	Left Tibialis Anterior
CH13:	Left Gastrocnemius

**CUSTOM
ANKLE
PROTOCOL**

RIGHT

CH1:	Right Tibialis Anterior
CH2:	Right Gastrocnemius
CH3:	Right Lateral Ankle
CH4:	Right Medial Ankle

LEFT

CH10:	Left Tibialis Anterior
CH11:	Left Gastrocnemius
CH12:	Left Lateral Ankle
CH13:	Left Medial Ankle

HIP & GROIN PROTOCOL			
RIGHT		LEFT	
CH1:	Right Paraspinal L5-S1	CH10:	Left Paraspinal L5-S1
CH2:	Right Gluteus Maximus	CH11:	Left Gluteus Maximus
CH3:	Right Iliopsoas	CH12:	Left Iliopsoas
CH4:	Right Rectus Abdominus	CH13:	Left Rectus Abdominus
CH5:	Right Abdominal Oblique	CH14:	Left Abdominal Oblique
CH6:	Right Gracilis	CH15:	Left Gracilis
CH7:	Right Hamstrings	CH16:	Left Hamstrings

The EMG sensors 4 are attached to the patient in a conventional manner for use of EMG technology. Conventional connection requires that a patient 46 ground be established with one EMG sensor 4 as a reference and that two EMG sensors 4 be attached to each muscle to be evaluated. The data collected by the two EMG sensors 4 represents a difference in electrical potential between the two EMG sensors 4 connected to each muscle.

Each protocol also involves the use of a remote tracking device (ROM sensor 6). The ROM sensor 6 is attached to the body of the patient 46 at the location specified by Table 2. The ROM sensor 6 is attached by an elastic bandage, by a strap, by incorporating the ROM sensor 6 into an article of clothing, by an adhesive or by any other suitable means.

TABLE 2

Protocol	Motion detector location
Cervical Protocol	Back of the head
Thoracic Protocol	Vicinity of T4-T5 vertebrae
Lumbosacral Protocol	Top of the Head
Carpal Tunnel Protocol	Hand or Wrist
Shoulder Protocol	Back of the head
Lower Extremities Protocol	Knee Cap
Custom Ankle Protocol	Ankle or Foot
Hip & Groin Protocol	Top of the Quadriceps Femoris

5

The "zoom patient protocol" screens of Fig. 13 are useful for user training and as a check to the user concerning EMG sensor 4 placement. It is anticipated that as a user becomes facile with the operation of the apparatus that the user will not require instruction by the "zoom patient protocol" 158, 160.

10

Fig. 14 illustrates the use of the first client computer software 114 to perform a protocol and record the results of the protocol. From the Main menu 124, the user elects to run a protocol 162 and selects the protocol that will be run. The cervical protocol is the default if no other protocol is selected. The user is unable to select the "run test" 162 command unless a new or existing patient file 136, 150 has been loaded. The user may elect to "zoom patient protocol" 164, as described above, to see an illustration of proper EMG sensor 4 placement and a list of muscles to be monitored.

15

20

The user will then administer the protocol 166 to the patient. Each protocol comprises several steps. Each protocol includes tests requiring that the patient 46 be connected to a plurality of EMG sensors 4 and to an ROM sensor 6 that are in turn connected to the

CNMP housing 28 through EMG sensor cables 48 and a ROM sensor cable 58. Some of the protocols also involve the patient 46 exerting force against an isometric function sensor 12, a grip strength sensor 8, or a finger pinch sensor 10, each of which is connected to the
5 CNMP housing 28. The patient 46 follows instructions by the user or as instructed by the software as the patient 46 performs several tasks. The instructions are displayed to the user and the user verbally instructs the patient 46 to perform the task. Alternatively, the instructions may be displayed to the user on, for example, a
10 computer monitor 42. The tasks are designed to challenge specific muscles to allow measurement of the electrical characteristics of the muscles as they are challenged. Each of the tasks are timed and the patient 46 is allowed fifteen seconds to complete each task.

The first client computer 34 records data as the tests are
15 administered 168. EMG data 82 of the monitored muscles is recorded continuously. The ROM data 32 is collected during the time that the patient 46 is performing a task relating to motion of a body part of the patient 46. The patient 46 is recorded by video camera 14 to create a video record of patient 46 compliance and to
20 allow monitoring by a health care professional. The user also monitors patient 46 compliance and proper performance of the test by the patient 46.

The sequential instructions and challenges to the patient 46 for each step of each protocol is provided below. The protocol
25 instructions below also include instructions to the user to connect or disconnect the isometric function sensor 12 (also referred to as the 'IFT'), the grip sensor 8 and the finger pinch sensor 10, as appropriate for the particular protocol being administered. The ROM sensor 6 is referred to as the "motion tracking device" in the
30 descriptions below. The patient 46 is provided a rest period of fifteen seconds between each of the protocol steps listed below.

Cervical Protocol

a. (flexion/extension) "Slowly bend your head at a constant speed in an arc such that you bend forward to look at the floor and
35 then sweep it backwards such that you are looking at the ceiling. Repeat three times, pausing for two seconds between each repetition."

b. (rotation) "Slowly turn your head at a constant speed to the right, back to center and then to the left. Repeat three times, pausing for two seconds between each repetition."

5 c. (lateral bending) "Slowly and at a constant speed with your gaze fixed on the wall straight ahead at eye level, try to bring your right ear to your right shoulder, then sweep back through the center to try to bring your left ear to your left shoulder without moving anything but your head. Repeat three times, pausing for two seconds between each repetition."

10 **Thoracic Protocol**

a. (Flexion/extension) "Slowly bend forward at the waist at a constant speed while keeping your legs straight, then return to center and then bend backwards and return to center. Repeat three times, pausing for two seconds between each repetition. "

15 b. (Rotation) "Bend over at the waist such that your upper body and lower body are at a 90 degree angle and cross your arms over your chest. Slowly and at a constant speed, twist your upper body to the right, return to center, then twist to the left and return to center. Repeat three times, pausing for two seconds between
20 each repetition"

c. (Lateral Bending) "Stand upright at rest with your gaze fixed on the wall straight ahead at eye level with your arms hanging straight down at your sides. Slowly and at a constant speed, lean to your right and slide your right hand down your right leg, return to
25 rest and then lean to your left and slide your left hand down your left leg and return to rest. Repeat three times, pausing for two seconds between each repetition."

d. (Rowing) "Stand upright with your arms straight out from your body at shoulder level while looking straight forward with your
30 gaze fixed on a spot on the wall at eye level. Slowly and at a constant speed, pull each hand to its respected shoulder by bending your elbows, then return to full extension. Repeat three times, pausing for two seconds between each repetition."

e. (Abduction/Adduction) "Stand upright with your arms
35 relaxed at your sides while looking straight forward with your gaze fixed on a spot on the wall at eye level. Slowly and at a constant speed while keeping your elbows locked, lift your arms sideways

from your body over your head and then bring them down again to your sides. Repeat three times pausing, for two seconds between each repetition."

- 5 f. (Upright Rowing) "Stand upright with your arms relaxed at your sides while looking straight forward with your gaze fixed on a spot on the wall at eye level. Slowly and at a constant speed, simulate pulling a bar up with both hands to your chin by bending your elbows. Repeat three times, pausing for two seconds between each repetition."

10 **Lumbosacral Protocol**

- a. (Flexion/Extension) "Slowly bend forward at the waist at a constant speed while keeping your legs straight, then return to center and then bend backwards and return to center. Repeat three times, pausing for two seconds between each repetition."
- 15 b. (Rotation) "Stand upright with your arms relaxed at your sides while looking straight forward with your gaze fixed on a spot on the wall at eye level. Slowly and at a constant speed, twist your upper body to the right, back to center, to the left and return to center. Repeat three times, pausing for two seconds between each
- 20 repetition."
- c. (Lateral Bending) "Stand upright at rest with your gaze fixed on the wall straight ahead at eye level with your arms hanging straight down at your sides. Slowly and at a constant speed, lean to your right and slide your right hand down your right leg, return to
- 25 rest and then lean to your left and slide your left hand down your left leg and return to rest. Repeat three times, pausing for two seconds between each repetition."
- d. (IFT Underhand Lifting) "Place your feet on either side of the [IFT] bar at shoulder width while gripping the handle UNDERHANDED
- 30 with the handle held a few inches above your knees. While keeping your arms straight and knees bent, straighten your legs to lift up on the bar as hard as you can and then return to rest. Repeat three times, pausing for two seconds between each repetition."
- e. (IFT Overhand Lifting) "Place your feet on either side of the
- 35 bar at shoulder width while gripping the handle OVERHANDED with the handle held a few inches above your knees. While keeping your arms straight and knees bent, straighten your legs to lift up on the

bar as hard as you can and then return to rest. Repeat three times, pausing for two seconds between each repetition."

Carpal Tunnel Protocol

- 5 a. (Flexion/Extension) "Slowly bend your head at a constant speed in an arc such that you bend forward to look at the floor and then sweep it backwards such that you are looking at the ceiling. Repeat three times."
- 10 b. (Rotation) "Slowly turn your head at a constant speed to the right, back to center and then to the left. Repeat three times, pausing for two seconds between each repetition."
- 15 c. (Lateral Bending) "Slowly and at a constant speed with your gaze fixed on the wall straight ahead at eye level, try to bring your right ear to your right shoulder, then sweep back through the center to try to bring your left ear to your left shoulder without moving anything but your head. Repeat three times, pausing for two seconds between each repetition."
- Rest Standing "Stand upright with your arms relaxed at your sides while looking straight forward with your gaze fixed on a spot on the wall at eye level."
- 20 d. (System Check) "Ensure the Motion Tracking Device is installed on the back of the patient's RIGHT hand."
- e. (Wrist Extension RIGHT) "Bring your RIGHT arm straight out in front of your body at shoulder level and slowly and at a constant speed bend the wrist up and then return it to rest. Repeat three times, pausing for two seconds between each repetition."
- 25 f. (Wrist Flexion/Finger Grasp RIGHT) "Bring your RIGHT arm straight out in front of your body at shoulder level with your fingers spread and bend your wrist down and then close your fingers and make a fist, then relax your fingers and return your wrist to rest. Repeat three times, pausing for two seconds between each repetition."
- 30 g. (System check) "Ensure the Motion Tracking Device is installed on the back of the patient's LEFT hand."
- 35 h. (Wrist Extension LEFT) "Bring your LEFT arm straight out in front of your body at shoulder level and slowly and at a constant speed bend the wrist up and then return it to rest. Repeat three times, pausing for two seconds between each repetition."

- i. (Wrist Flexion/Finger Grasp LEFT) "Bring your LEFT arm straight out in front of your body at shoulder level with your fingers spread and bend your wrist down and then close your fingers and make a fist, then relax your fingers and return your wrist to rest.
5 Repeat three times, pausing for two seconds between each repetition."
- j. (IFT Installation) "Place the IFT plate on the floor and adjust the strap length as dictated by the protocol."
- k. (IFT Underhand Lifting) "Place your feet on either side of
10 the bar at shoulder width while gripping the handle UNDERHANDED with the handle held a few inches above your knees. While keeping your arms straight and knees bent, straighten your legs to lift up on the bar as hard as you can and then return to rest. Repeat three times, pausing for two seconds between each repetition."
- l. (IFT Overhand Lifting) "Place your feet on either side of
15 the bar at shoulder width while gripping the handle OVERHANDED with the handle held a few inches above your knees. While keeping your arms straight and knees bent, straighten your legs to lift up on the bar as hard as you can and then return to rest. Repeat three
20 times, pausing for two seconds between each repetition."
- m. (Jamar grip installation) "Give the patient the Jamar Grip Device to hold in their right hand."
- n. (Grip RIGHT) "Hold the Jamar Grip Device in your RIGHT hand
25 with your arm at your side and lift it with a slightly bent elbow to waist level with your wrist held straight and grip/squeeze the Jamar as hard as you can, then release and return your arm to your side. Repeat three times, pausing for two seconds between each repetition."
- o. (Grip LEFT) "Hold the Jamar Grip Device in your LEFT hand
30 with your arm at your side and lift it with a slightly bent elbow to waist level with your wrist held straight and grip/squeeze the Jamar as hard as you can, then release and return your arm to your side. Repeat three times, pausing for two seconds between each repetition."
- 35 p. (Pinch Device Installation) "Take the Jamar Grip Device from the patient and give them the Pinch Sensor Device to hold in their right hand."

q. (Pinch RIGHT) "Hold the pinch sensor in your RIGHT hand between your thumb and index finger with your arm at your side and squeeze the sensor as hard as you can. Repeat three times, pausing for two seconds between each repetition."

- 5 r. (Pinch LEFT) "Hold the pinch sensor in your LEFT hand between your thumb and index finger with your arm at your side and squeeze the sensor as hard as you can. Repeat three times, pausing for two seconds between each repetition."

Shoulder

- 10 a. (Flexion/Extension) "Slowly bend your head at a constant speed in an arc such that you bend forward to look at the floor and then sweep it backwards such that you are looking at the ceiling. Repeat three times, pausing for two seconds between each repetition."

- 15 b. (Rotation) "Slowly turn your head at a constant speed to the right, back to center and then to the left. Repeat three times, pausing for two seconds between each repetition."

- c. (Lateral Bending) "Slowly and at a constant speed with your gaze fixed on the wall straight ahead at eye level, try to bring your
20 right ear to your right shoulder, then sweep back through the center to try to bring your left ear to your left shoulder without moving anything but your head. Repeat three times, pausing for two seconds between each repetition."

- d. (Shoulder Shrug) "Standing in an upright position with your
25 arms at your sides, elevate your shoulders towards your ears and hold for approximately two seconds and then return to rest. Repeat three times."

- e. (Abduction/Adduction) "Stand upright with your arms relaxed at your sides while looking straight forward with your gaze
30 fixed on a spot on the wall at eye level. Slowly and at a constant speed while keeping your elbows locked, lift your arms sideways from your body over your head and then bring them down again to your sides. Repeat three times pausing, for two seconds between each repetition."

- 35 f. (Interior/Exterior Rotation) "While standing upright with your arms at your side with the elbows locked at 90 degrees; slowly and at a constant speed bring your hands up towards and past your ears

and then bring them back down and to the back as far as possible then return to rest. Repeat three times, pausing for two seconds between each repetition."

- 5 g. (IFT Installation) "Place the IFT plate on the floor and adjust the strap length as dictated by the protocol."
- 10 h. (IFT Underhand Lifting) "Place your feet on either side of the bar at shoulder width while gripping the handle UNDERHANDED with the handle held a few inches above your knees. While keeping your arms straight and knees bent, straighten your legs to lift up on the bar as hard as you can and then return to rest. Repeat three times, pausing for two seconds between each repetition."
- 15 i. (IFT Overhand Lifting) "Place your feet on either side of the bar at shoulder width while gripping the handle OVERHANDED with the handle held a few inches above your knees. While keeping your arms straight and knees bent, straighten your legs to lift up on the bar as hard as you can and then return to rest. Repeat three times, pausing for two seconds between each repetition."

Lower Extremities Protocol

- 20 a. (Walking) "Take 3 steps forward and then 3 steps backwards to return to the original position. Repeat three times, pausing for two seconds between each repetition."
- b. (Walking) "Take 3 steps forward and then 3 steps backwards to return to the original position. Repeat three times, pausing for two seconds between each repetition."
- 25 c. (Knee Flexion/Extension RIGHT) "While supporting yourself on a stationary object, raise your RIGHT leg straight forward in front of your body and then bend the knee, straighten your leg again and then return to a standing position. Repeat three times, pausing for two seconds between each repetition."
- 30 d. (Knee Flexion/Extension LEFT) "While supporting yourself on a stationary object, raise your LEFT leg straight forward in front of your body and then bend the knee, straighten your leg again and then return to a standing position. Repeat three times, pausing for two seconds between each repetition."
- 35 e. (Deep Knee Bends) "While supporting yourself on a stationary object, perform a deep knee bend while ensuring that your legs never

exceed a maximum angle of 90 degrees to one another. Repeat three times, pausing for two seconds between each repetition."

Custom Ankle Protocol

- 5 a. (Walking) "Take 3 steps forward and then 3 steps backwards to return to the original position. Repeat three times, pausing for two seconds between each repetition."
- b. (Walking) "Take 3 steps forward and then 3 steps backwards to return to the original position. Repeat three times, pausing for two seconds between each repetition."
- 10 c. (Ankle Flexion/Extension RIGHT) "While supporting yourself on a stationary object while keeping your LEFT leg straight, lift your RIGHT leg by bending at the knee and bend your ankle slowly and at a constant speed such that your toes point down, center and then up and back to center. Repeat three times, pausing
15 for two seconds between each repetition."
- d. (Ankle Rotation RIGHT) "While supporting yourself on a stationary object while keeping your LEFT leg straight, lift your RIGHT leg by bending at the knee and rotate your ankle slowly and at a constant speed to the right, back to center, back to left and
20 finally returning to center. Repeat three times, pausing for two seconds between each repetition."
- e. (Ankle Flexion/Extension LEFT) "While supporting yourself on a stationary object while keeping your RIGHT leg straight, lift your LEFT leg by bending at the knee and bend your ankle slowly and at a
25 constant speed such that your toes point down, center and then up and back to center. Repeat three times, pausing for two seconds between each repetition."
- f. (Ankle Rotation LEFT) "While supporting yourself on a stationary object while keeping your RIGHT leg straight, lift your
30 LEFT leg by bending at the knee and rotate your ankle slowly and at a constant speed to the right, back to center, back to left and finally returning to center. Repeat three times, pausing for two seconds between each repetition."

Hip & Groin protocol

- 35 a. (Flexion/Extension RIGHT) "While supporting yourself on a stationary object while keeping your RIGHT leg straight with the toes pointed upwards, slowly and at a constant speed raise your leg

forward as high as possible, back to rest and then backwards as high as possible and then return to rest. Repeat three times, pausing for two seconds between each repetition."

5 b. (Abduction/Adduction RIGHT) "While supporting yourself on a stationary object and keeping your RIGHT leg straight with the toes pointed upwards swing your leg inwards to the left as far as possible, back to center and then as far right as possible and return to rest. Repeat three times, pausing for two seconds between each repetition."

10 c. (Flexion/Extension LEFT) "While supporting yourself on a stationary object while keeping your LEFT leg straight with the toes pointed upwards, slowly and at a constant speed raise your leg forward as high as possible, back to rest and then backwards as high as possible and then return to rest. Repeat three times, pausing
15 for two seconds between each repetition."

d. (Abduction/Adduction LEFT) "While supporting yourself on a stationary object and keeping your LEFT leg straight with the toes pointed upwards swing your leg inwards to the right as far as possible, back to center and then as far left as possible and return to
20 rest. Repeat three times, pausing for two seconds between each repetition."

e. (Deep Knee Bends) "While supporting yourself on a stationary object, perform a deep knee bend while ensuring that your legs never exceed a maximum angle of 90 degrees to one another. Repeat
25 three times, pausing for two seconds between each repetition."

Upon completion of each step of the selected protocol, the user may review graphs of the data collected to determine that the CNMP apparatus 2 and the patient performed the step properly and that the data was properly recorded. In the 'review step data,'
30 screen 170, the user is presented with small images of data graphs for the ROM data 32 and the EMG data 82 collected. The user may "zoom" (enlarge) 172, 174 the data graphs to verify the proper conduct of the step. On the 'review step data' screen 170, the user also is presented with a small image of the collected video
35 information 26, which can also be zoomed for closer examination. If the user is satisfied that the data was properly collected and the test properly run, the user may accept and save the data 176. If the

user detects an error in the data, for example a failure of an EMG sensor 4 or failure of the patient 46 to comply fully with the instructions, the user may reject 178 the data and request that the patient 46 repeat the step. The user may 'zoom' a demonstration
5 video file 180 for display to the patient 46 to show the patient 46 the actions that the patient 46 will perform in the step.

The user may abort the protocol 182, deleting all collected data. The user also may save the protocol 184, which 'zips' (compresses) the CNMP data 30 and ROM data 32 to create a
10 smaller data file for transmission over a network 38 to a server computer 36.

Fig. 15 illustrates the upload process for transferring the CNMP data 30, ROM data 30 and video information 26 to a server computer 36 for analysis. From the 'Main' screen 124, patient data
15 is uploaded 186. The user logs onto the network 188, assuring the server computer 36 that user is authorized to access server computer 36. The user instructs the client computer 34 to upload the data to the server computer 36 and the data is transferred 190. The user may instruct the client computer 34 to abort 192 the
20 upload process and is provided an opportunity to ok 196 or cancel 194 the abort command. If the upload is aborted 196, the user is returned to the main screen 124.

Fig. 16. illustrates the download by the first client computer 34 of the results of the data analysis by the server computer 36.
25 The results of the data analysis also may be downloaded by an authorized person using a second client computer 35. An authorized person, such as a healthcare provider or insurance company, selects 'download reports' 198 from the 'main' menu 124. The user logs onto the network 200, assuring the server computer 36 that the
30 person is authorized to receive the requested report. The person instructs the server computer 36 as to the patient information that the person desires to receive. The server computer 36 then transmits the requested information to the first or second client computer 34/35, over the network 38 for display to the authorized
35 person. The first or second client computer 34/35, follows the progress of the download 202. The download may be aborted 204 and the abort may be cancelled 206.

From Figs. 17 and 18, the 'main' menu **124** also allows the user to access an 'about' screen **208** providing information about the software. The main menu also allows the user to 'quit' **210** the program.

5 The first client computer software **114** provides methods for failure detection and override. If any sensor **4, 6, 8, 10, 12** or cable **48, 58, 70, 72, 74, 76** is detected to be faulty, the first client computer software **114** alerts the user, and allows the user to override the detection, or halt the test to allow for fault correction.

10 The first client computer software **114** also employs data encryption, to ensure the integrity of the CNMP data **30** or ROM data **32**.

Fig. 19 illustrates the operation of the server computer **36** evaluating the CNMP data **30** and ROM data **32**. In step **212** of Fig. 18, server computer **36** receives ROM data **32**. The ROM data **32** comprises information relating to range of motion of a body part of the patient **46** and the dynamic motion of the patient **46** within that range. The server computer also receives CNMP data **30** comprising pinch data **88**, grip data **86**, isometric function data **84** and EMG data **82**. The server computer microprocessor **118** is programmed to perform pre-determined data evaluation on the data received. As indicated on step **214** of Fig. 19, the data evaluation comprises pattern recognition evaluation using techniques as known in the art, either alone or in combination. The evaluation of the data may reveal patterns in the CNMP data **30** and ROM data **32**. As indicated on step **216** of Fig. 18, the server microprocessor **118** consults an expert database **122** of patterns and combinations of patterns resident in server computer memory **120**. The expert database **122** associates one or more diagnoses, or patient profiles **40**, with each of the patterns or combinations of patterns. From step **218**, the expert database **122** informs the server microprocessor **118** of the patient profile **40** identified by the patterns and combination of patterns. From step **220**, the server microprocessor **118** supplies a report of the patient profile **40** to the user or other authorized person over the computer network **38**.

35 Evaluation and analysis of the data collected by the first client computer **34** may be performed in whole or in part by a human

expert. During collection of data for creation of the expert database, an expert physician will review all results of the analysis and the expert database will be amended to incorporate the results of the physician's review. Once the system has a large track record, only
5 abnormal patterns detected during the analysis will be referred for expert physician review.

The Invention is designed to provide medical professionals and other interested parties with an accurate method of simultaneously observing muscular functionality and additional muscular and
10 nervous system characteristics. This will provide the users a pinpoint procedure to identify and properly diagnose myofascial and other injuries. The Invention achieves its goals through combining surface EMG and pulsed DC electromagnetic range-of-motion technology, along with isometric functional capacity and grip/pinch
15 strength sensors, to obtain a comprehensive set of necessary functional output signals. The Invention uses a custom signal conditioning and conversion circuit board **78** to condition and digitize the signals, which are then fed to a first client computer **34**.

The Invention is non-invasive, non-loading and portable. The
20 Invention uses a combination of surface EMG sensors **4**, a ROM sensor **6**, an isometric function sensor **12**, a grip sensor **8** and a pinch sensor **10** in order to determine the functional capability and characteristics of muscle group and surrounding tissues. The EMG sensors **4** obtain readings related to the pathophysiological processes
25 within a muscle, pressure exerted by blood vessels on the muscle and surrounding tissue, as well as observing muscle characteristics such as muscle tone and presence of spasms. The isometric function sensor **12**, along with pinch **10** and grip **8** strength sensors allow a higher level of accuracy in identifying certain types of
30 injuries. The isometric function sensor allows the Invention to monitor the patients' potential lifting force. This is a major factor in identifying lower back injuries and in monitoring compliance by the patient **46** with the performance of the test. A person who is feigning injury may be detected through the isometric function data
35 **84** alone or in combination with EMG data **82**. The pinch and grip strength sensors **10**, **8** accomplish the same task as the isometric function sensor **12**, except that the pinch and grip sensors **10**, **8**

observe the functional characteristics of those body parts which typically correspond to carpal tunnel syndrome and other related injuries. As used in this application, the term "functional capacity data" means data relating to the ability of the patient to exert force using the muscles of the patient and includes isometric function data **84**, pinch data **88** and grip data **86**.

The Invention uses the combination of different technologies in order to simultaneously monitor muscle groups in order to thoroughly obtain information about muscle functionality, rate of fatigue, muscle response, and other associated muscular characteristics. The simultaneous use of complementary technologies allows the user to accurately monitor the muscular compensation patterns typically seen in injured muscle groups and their surrounding areas. These compensation patterns are usually a key element in identifying the age and type of injury present.

The accuracy of the Invention allows medical professionals to have a much higher degree of certainty when diagnosing injuries. This allows the patient **46** and medical professional to prescribe a more detailed course of action for treatment and rehabilitation, saving time and money. It also allows a higher level of objectivity when diagnosing work-related injuries, saving businesses time and money that would be lost through workers' compensation and ADA-related lawsuits.

The Invention allows for a high level of portability and patient **46** comfort. The pulsed DC electromagnetic ROM sensor **6**, transmitter **50** and ROM device signal processing unit **60** provide a more accurate method of obtaining range-of-motion data than previously available, while providing a very compact device which increases the ease of transportation. The use of the electromagnetic device also does not require the use of harnesses or belts to attach the device to the patient. Instead, the device is attached by a single small sensor, in a manner similar to the EMG sensors **4** used by the surface EMG component. This provides the patient **46** with a much more comfortable testing experience, and makes the entire system less cumbersome to use than prior art testing systems.

Use of the Invention is not limited to human injuries and may accurately monitor muscle groups for injury diagnosis in animals, primarily horses.

5 The Invention may be used to measure actual muscular potential independent of patient effort. The ROM data **32** and surface EMG data **82** in combination allows the Invention to objectively measure the actual range-of-motion or lifting potential of the patient **46**, reducing the likelihood of false discrimination cases and workers' compensation claims.

10 The Invention also may differentiate between related injuries. This includes related injuries such as paraspinal and herniated discs, vasoconstriction, and carpal tunnel syndrome and cubital tunnel syndrome. The use of simultaneous monitoring allows for the observation of compensation patterns and additional inter-muscle
15 relations, which assists in the differentiation process. The Invention may assist in pre-employment screening, in order to provide pre and post-injury comparison. The apparatus also may monitor injury healing during the rehabilitation process. The apparatus may be used in the athletic community, allowing the monitoring of rate of
20 muscle fatigue, and allowing a diagnosis of muscle relationships and the subsequent strengths and weaknesses in an athletes' makeup.

The server computer may be equipped and programmed to create a permanent record of the protocol data collected concerning
25 a patient, such as by creating CDs or DVDs or by utilizing other storage means known in the art.

The invention may be adapted to collect and to analyze electrocardiogram ("EKG") information.

30 A copy of the source code for the first client computer software **114**, written in the LabVIEW language and recorded on a CD ROM, is attached hereto and incorporated by reference herein.

35 Although this invention has been described and illustrated by reference to specific embodiments, it will be apparent to those skilled in the art that various changes and modifications may be made which clearly fall within the scope of this invention. The present invention is intended to be protected broadly within the spirit and scope of the appended claims.

1 I Claim:

- 1 1. An apparatus for generating neuromuscular profile data for a patient, the
2 apparatus comprising:
3 a. means for generating EMG data for a patient;
4 b. means for generating ROM data for a patient, said means for
5 generating ROM data utilizing a remote sensing technology;
6 c. a computer having a computer memory, said computer being
7 operatively connected to said means for generating said EMG data and said ROM
8 data, said computer being adapted to receive said EMG data and said ROM data
9 and to store said EMG data and said ROM data in said computer memory.
- 1 2. The apparatus of Claim 1 wherein said remote sensing technology comprises
2 pulsed DC electromagnetic field technology, AC electromagnetic field technology or
3 optical technology.
- 1 3. The apparatus of Claim 2 wherein said remote sensing technology comprises
2 a pulsed DC electromagnetic field technology.
- 1 4. The apparatus of Claim 3 wherein said pulsed DC electromagnetic field
2 technology comprises a ROM transmitter and a ROM sensor, said ROM transmitter
3 adapted to be placed in a predetermined relationship with a body of the patient and
4 further adapted to generate an electromagnetic field, said ROM sensor adapted to
5 be attached to said body of the patient, said ROM sensor being adapted to
6 generate a ROM signal in response to a location of said ROM sensor within said
7 electromagnetic field.
- 1 5. The apparatus of Claim 4, further comprising: means for generating isometric
2 function data for the patient, said computer being operatively connected to said
3 means for generating said isometric function data, said computer being adapted to
4 receive said isometric function data and to store said isometric function data in said
5 computer memory.
- 1 6. The apparatus of Claim 5, further comprising: means for generating grip
2 strength data for the patient, said computer being operatively connected to said
3 means for generating grip data, said computer being adapted to receive said grip
4 data and to store said grip data in said computer memory;
- 1 7. The apparatus of Claim 6, further comprising: means for generating finger
2 pinch data for the patient, said computer being operatively connected to said
3 means for generating said finger pinch data, said computer being adapted to

4 receive said finger pinch data and to store said finger pinch data in said computer
5 memory.

1 8. The apparatus of Claim 7, further comprising: means for generating video
2 information, said computer being operatively connected to said means for
3 generating said video information, said computer being adapted to receive said
4 video information and to store said video information in said computer memory.

1 9. The apparatus of Claim 8, further comprising: a protocol, said computer
2 having a memory, said protocol being resident in said memory of said computer;
3 said protocol comprising an instruction for a task to be performed by the patient,
4 said protocol further comprising a specification for protocol data to be collected
5 during performance of said task by the patient, said computer being adapted to
6 collect and to record said protocol data to said computer memory.

1 10. The apparatus of Claim 9 wherein said protocol data comprises one or more
2 of said EMG data, said ROM data, said isometric function data, said grip data, said
3 pinch data or said video information.

1 11. The apparatus of Claim 10 wherein said computer is adapted to provide to a
2 user said instruction for said task to be performed by the patient.

1 12. The apparatus of Claim 11, further comprising:

2 a. a server computer;

3 b. a computer network, said computer being a first client computer, said
4 server computer and said first client computer being adapted to communicate one
5 with the other over said computer network, said first client computer being adapted
6 to transmit said protocol data to said server computer over said computer network.

1 13. An apparatus for generating neuromuscular profile data for a patient, the
2 apparatus comprising:

3 a. a signal conditioning and conversion circuit board;

4 b. an EMG sensor adapted to be attached to the patient at a
5 predetermined EMG sensor location, said EMG sensor being adapted to generate an
6 EMG signal; said EMG sensor being electrically connected to said signal
7 conditioning and conversion circuit board, said signal conditioning and conversion
8 circuit board being adapted to receive said EMG signal and to convert said EMG
9 signal into EMG data;

10 c. a ROM transmitter adapted to be placed in a predetermined transmitter
11 location with respect to the patient and to generate an electromagnetic field;

12 d. a ROM sensor adapted to be attached to a body of the patient at a
13 predetermined ROM sensor location and to interact with said electromagnetic field
14 to generate a ROM signal;

15 e. a ROM signal processor electrically connected to said ROM sensor,
16 said ROM signal processor being adapted to receive said ROM signal and to convert
17 said ROM signal to ROM data;

18 f. a computer having a computer memory, said computer being
19 electrically connected to said signal conditioning and conversion circuit board and
20 to said ROM signal processor, said computer being adapted to receive said EMG
21 data and said ROM data and to store said EMG data and said ROM data in said
22 computer memory.

1 14. The apparatus of Claim 13, further comprising said computer being a first
2 client computer, said first client computer being adapted to transmit said EMG data
3 and said ROM data to a server computer over a computer network.

1 15. The apparatus of Claim 13, further comprising: an isometric function sensor
2 adapted to generate an isometric function signal in response to a force applied by
3 the patient; said isometric function sensor being electrically connected to said
4 signal conditioning and conversion circuit board, said signal conditioning and
5 conversion circuit board being adapted to convert said isometric function signal into
6 isometric function data, said computer being adapted to receive said isometric
7 function data and to store said isometric function data in said computer memory.

1 16. The apparatus of Claim 15, further comprising: a grip strength sensor
2 adapted to generate a grip signal in response to a grip of the patient; said grip
3 strength sensor being electrically connected to said signal conditioning and
4 conversion circuit board, said signal conditioning and conversion circuit board being
5 adapted to convert said grip strength signal into grip data, said computer being
6 adapted to receive said grip data and to store said grip data in said computer
7 memory.

1 17. The apparatus of Claim 16, further comprising: a finger pinch strength
2 sensor, said finger pinch strength sensor generating a pinch strength signal in
3 response to a finger pinch of the patient; said pinch strength sensor being
4 electrically connected to said signal conditioning and conversion circuit board, said
5 circuit board converting said finger pinch strength signal into pinch data, said
6 computer being adapted to receive said pinch data and to store said pinch data in
7 said computer memory.

- 1 18. The apparatus of Claim 17, further comprising: a video camera adapted to
2 generate video information of the patient, said video camera being electrically
3 connected to said computer, said computer being adapted to receive said video
4 information from said signal conditioning and conversion circuit board and to store
5 said video information in said computer memory.
- 1 19. The apparatus of Claim 13, further comprising: a protocol, said protocol
2 being resident in said computer memory of said computer; said protocol comprising
3 an instruction for a task to be performed by the patient, said protocol further
4 comprising a specification for protocol data to be collected during performance of
5 said task by the patient, said computer being adapted to administer said protocol
6 and to collect said protocol data.
- 1 20. The apparatus of Claim 19 wherein said protocol data comprises one or more
2 of said EMG data, said ROM data, an isometric function data, a grip data, a pinch
3 data or a video information.
- 1 21. The apparatus of Claim 20 wherein said computer is adapted to provide to a
2 user said instruction for said task to be performed by the patient.
- 1 22. The apparatus of Claim 21 wherein said computer is a first client computer,
2 said first client computer is adapted to transmit said protocol data to a server
3 computer over a computer network.
- 1 23. A method for collecting neuromuscular data for a patient, the method
2 comprising the steps of:
3 a. generating EMG data for the patient;
4 b. generating ROM data for the patient, said ROM data being generated
5 using a remote sensing technology;
6 c. storing said EMG data and said ROM data in a computer memory.
- 1 24. The method of Claim 23, further comprising:
2 a. comparing said EMG data and said ROM data in combination to an
3 expert database, said expert database associating a profile with said combination of
4 said EMG data and said ROM data;
5 b. assigning to the patient said profile;
6 c. communicating to a user said assigned profile.
- 1 25. The method of Claim 23 wherein said remote sensing technology is selected
2 from the group consisting of pulsed DC electromagnetic field technology, AC
3 electromagnetic field technology and optical technology

- 1 26. The method of Claim 25 wherein said remote sensing technology comprises
2 pulsed DC electromagnetic field technology.
- 1 27. The method of Claim 26, further comprising the steps of:
2 a. generating functional capacity data for the patient;
3 b. recording said functional capacity data in said computer memory.
- 1 28. The method of Claim 27 wherein said functional capacity data comprises
2 pinch data, grip data and isometric function data.

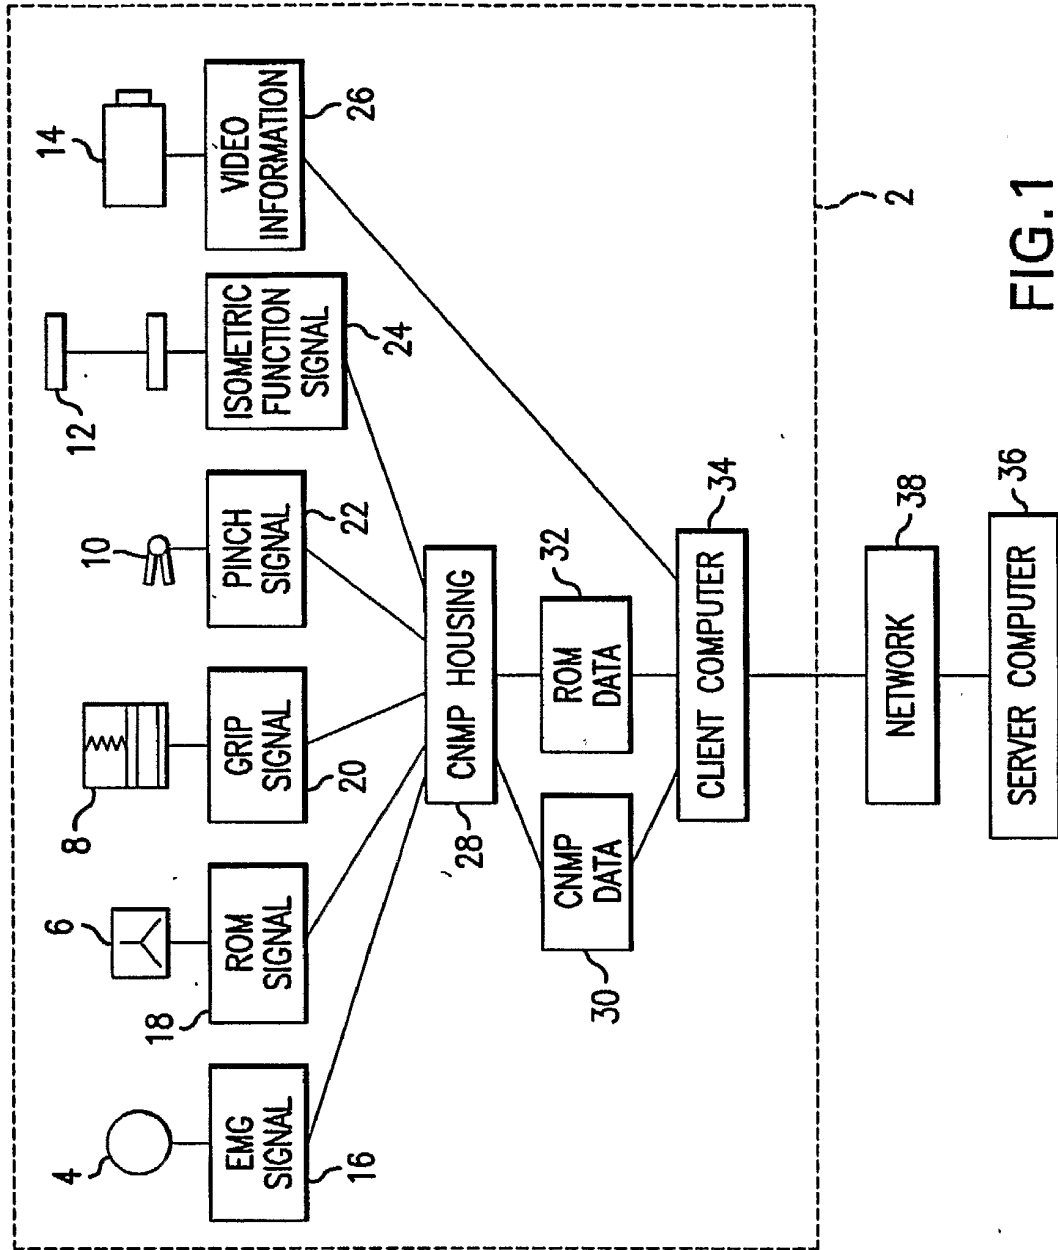


FIG. 1

2/20

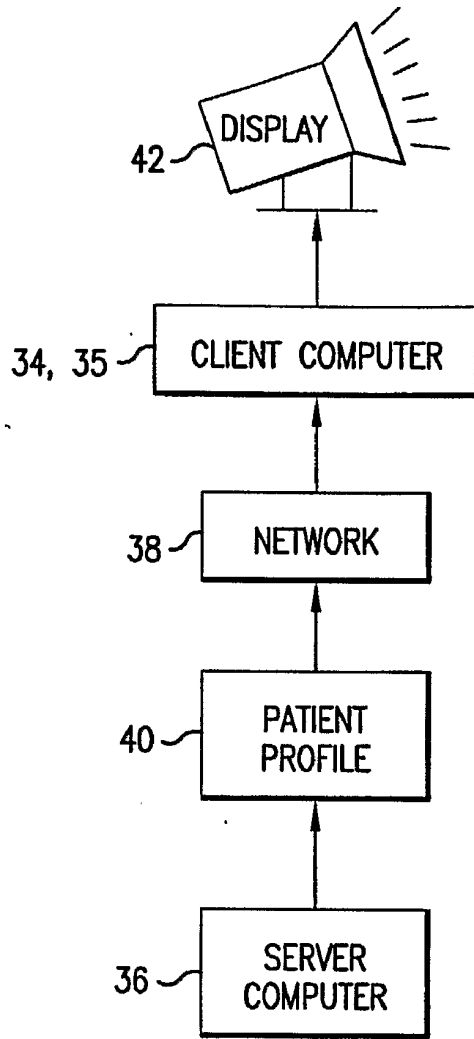


FIG.2

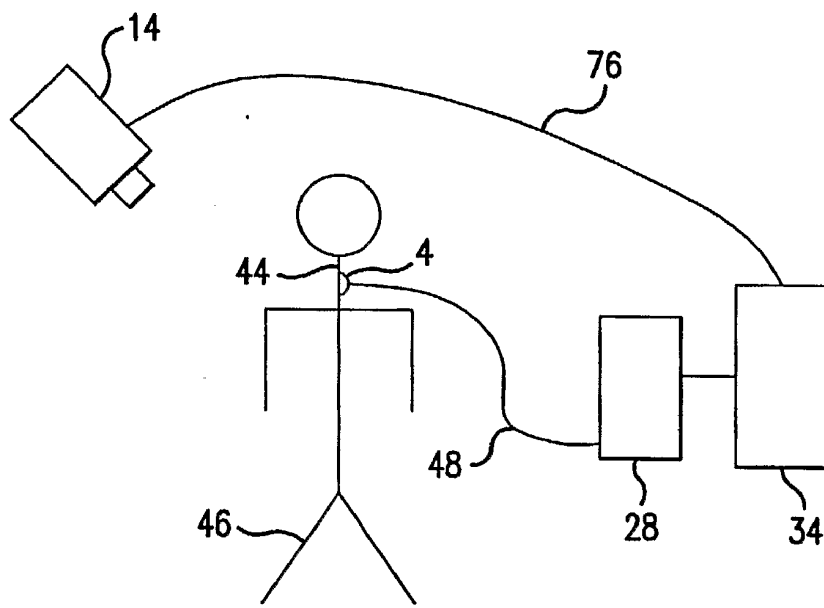


FIG.3

4/20

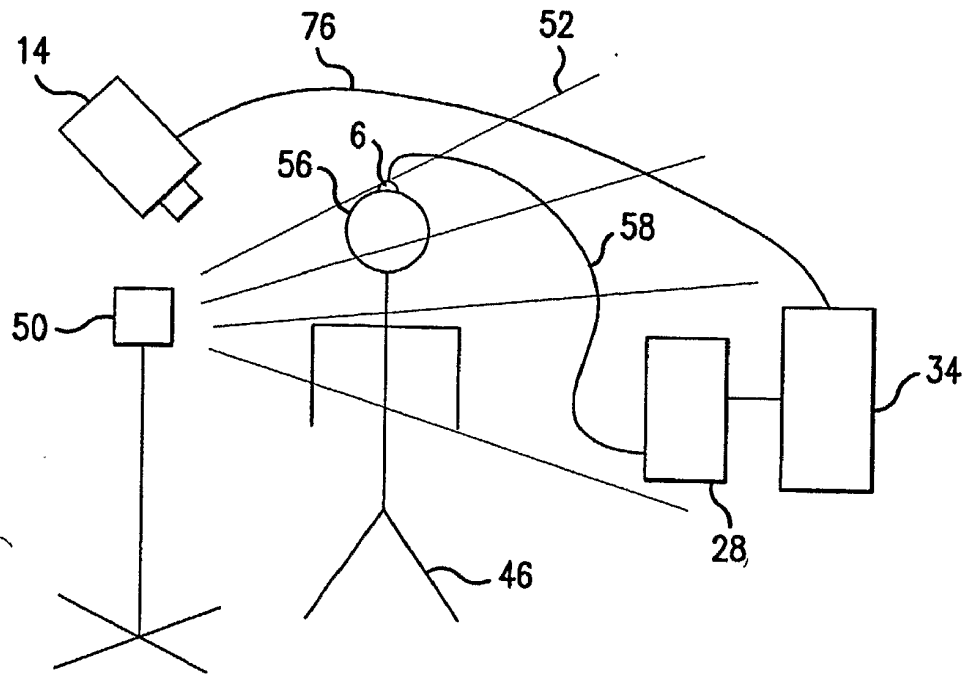


FIG. 4

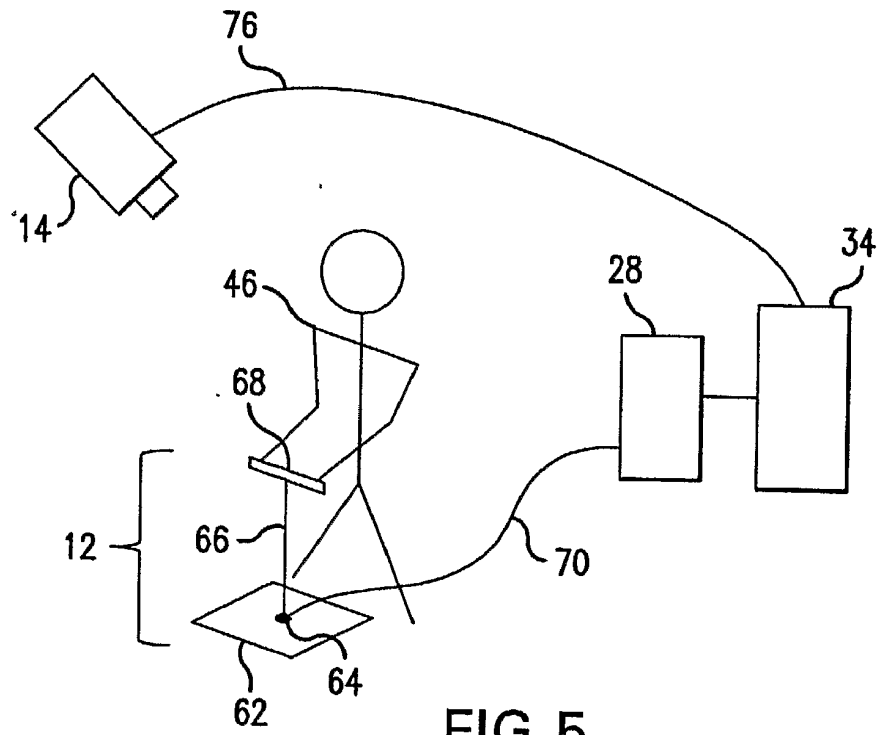


FIG. 5

5/20

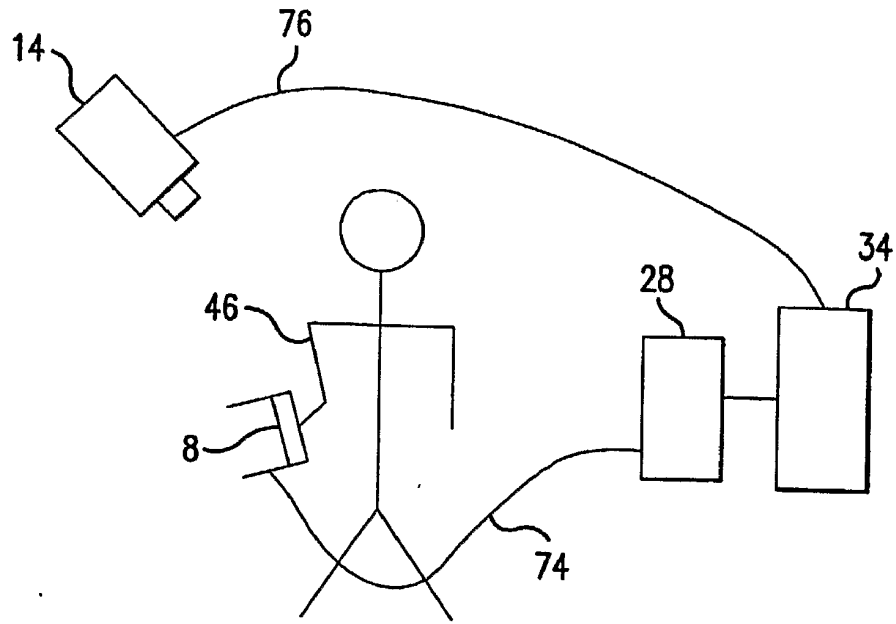


FIG. 6

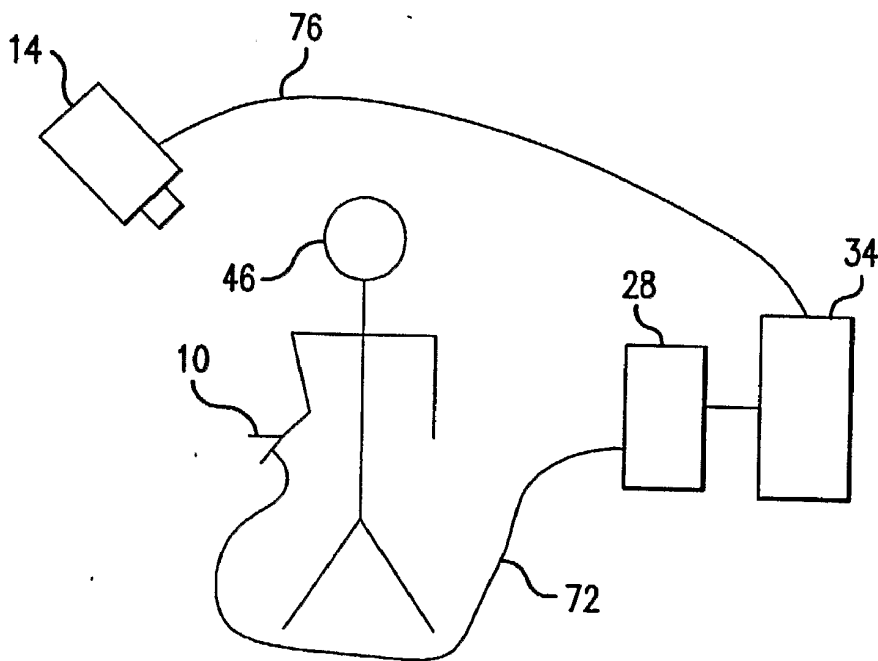


FIG. 7

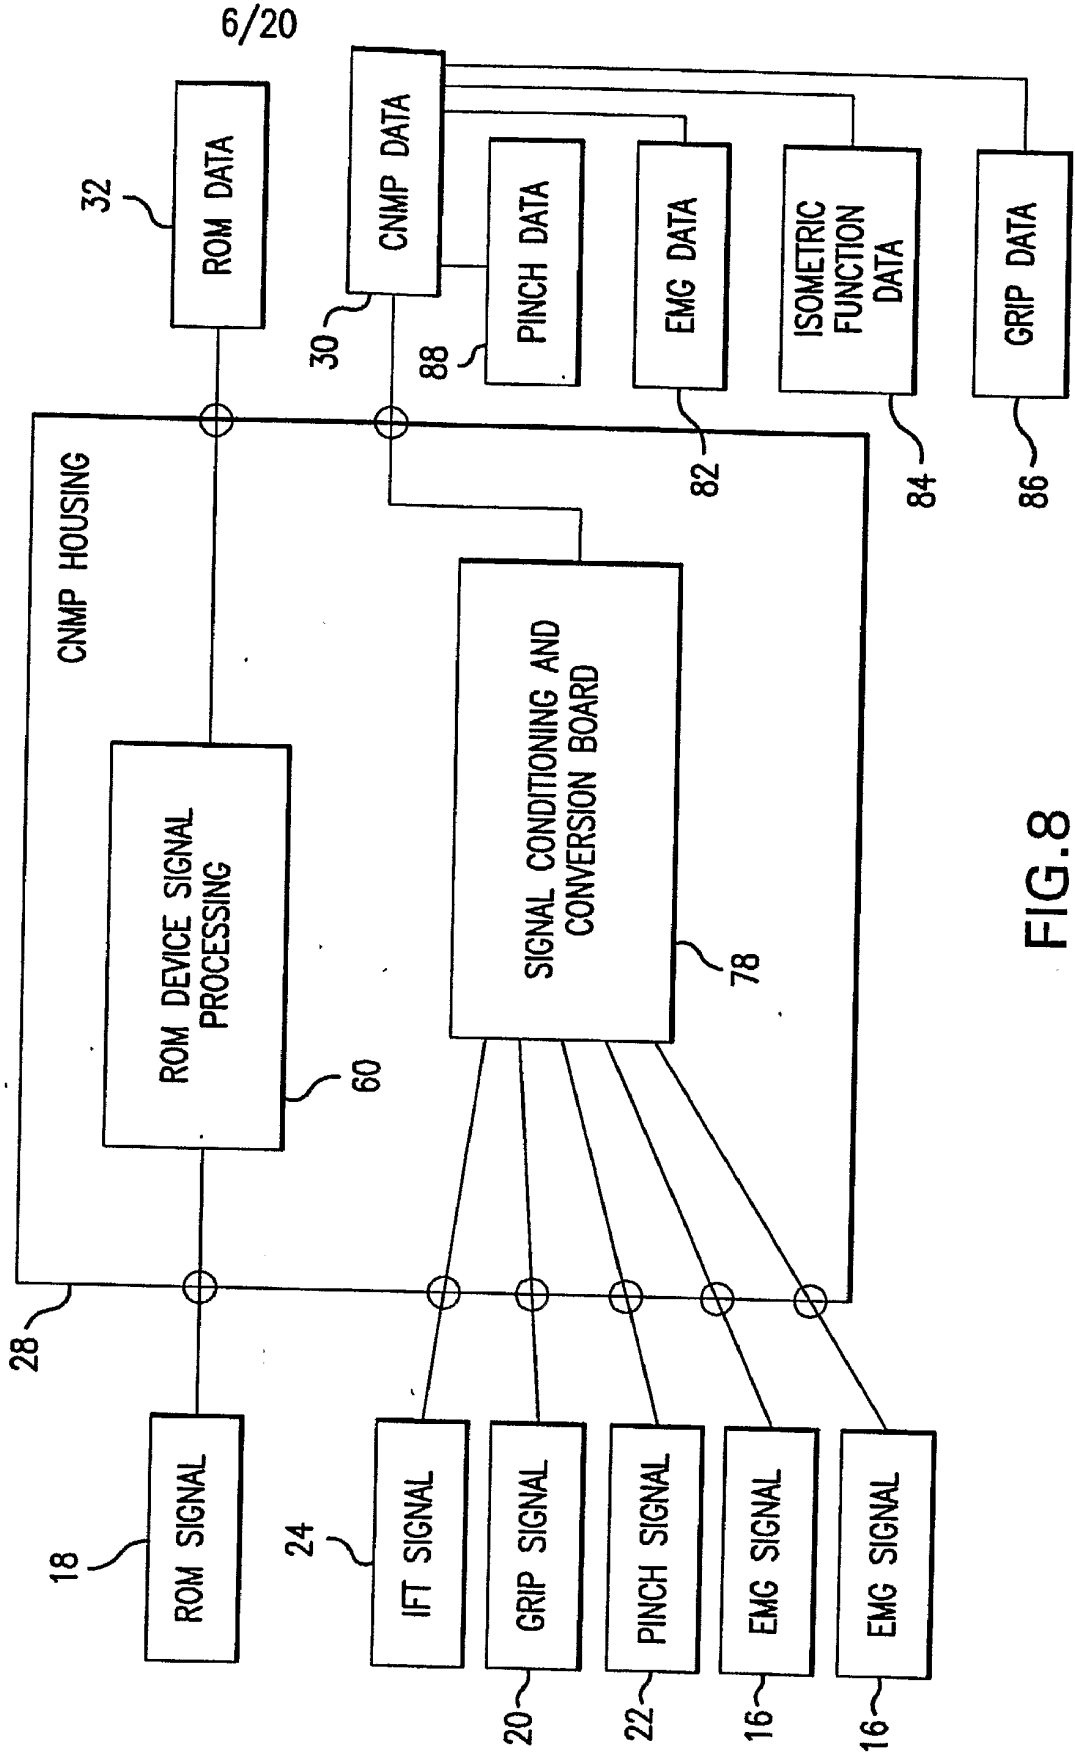


FIG.8

7/20

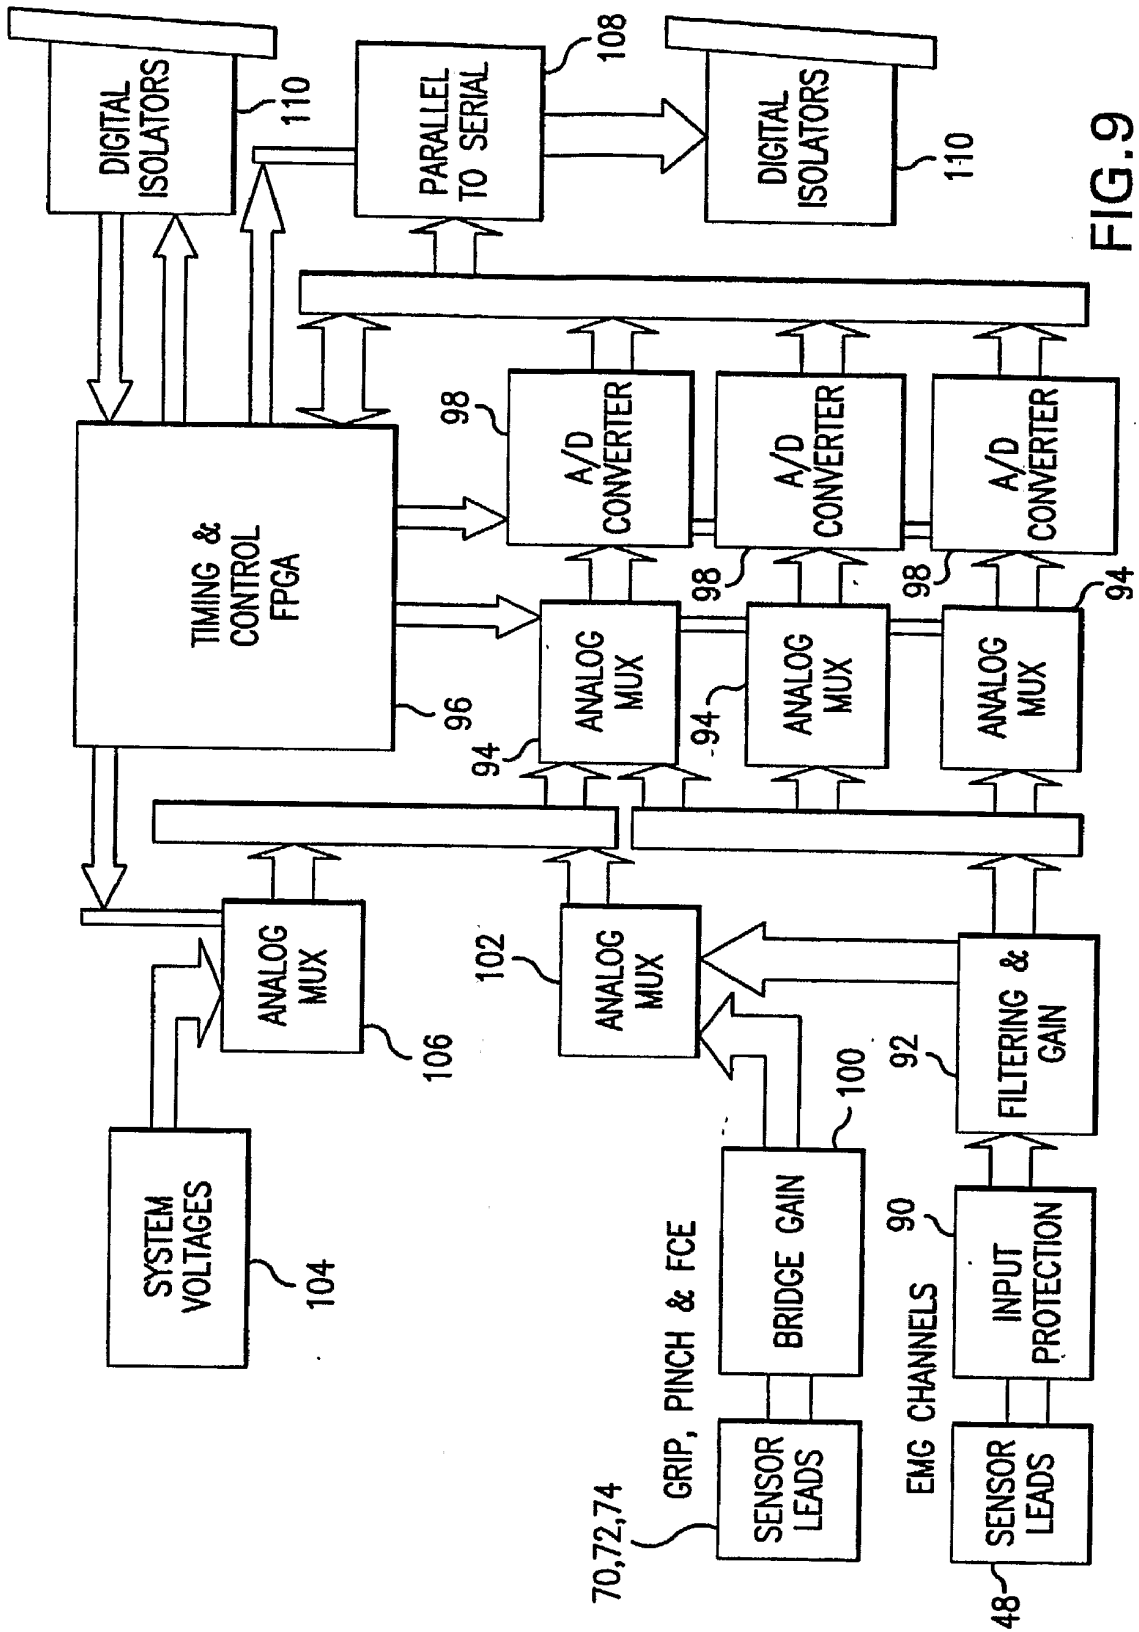


FIG. 9

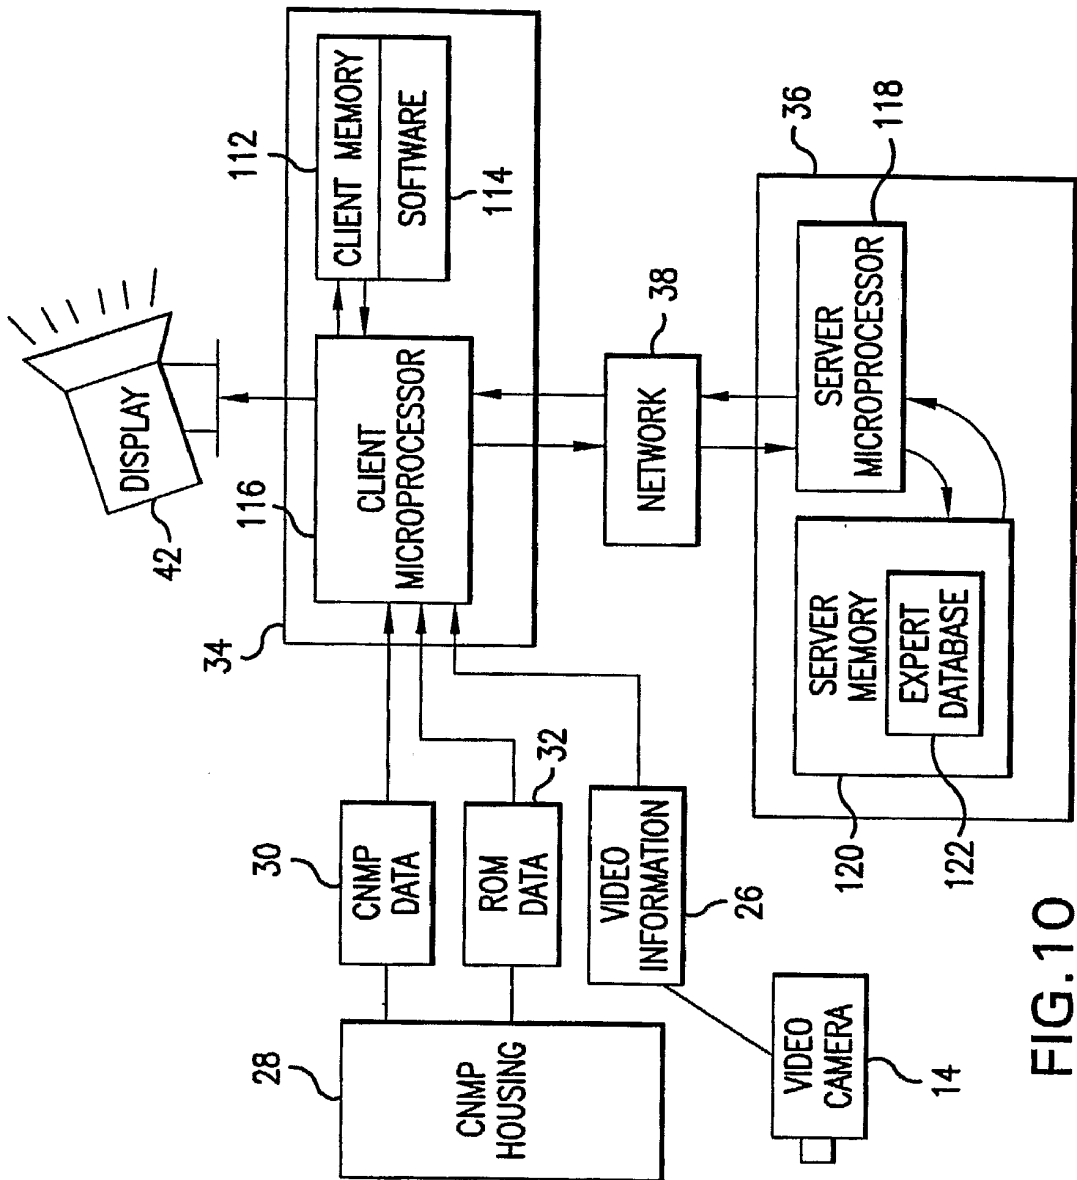


FIG. 10

9/20

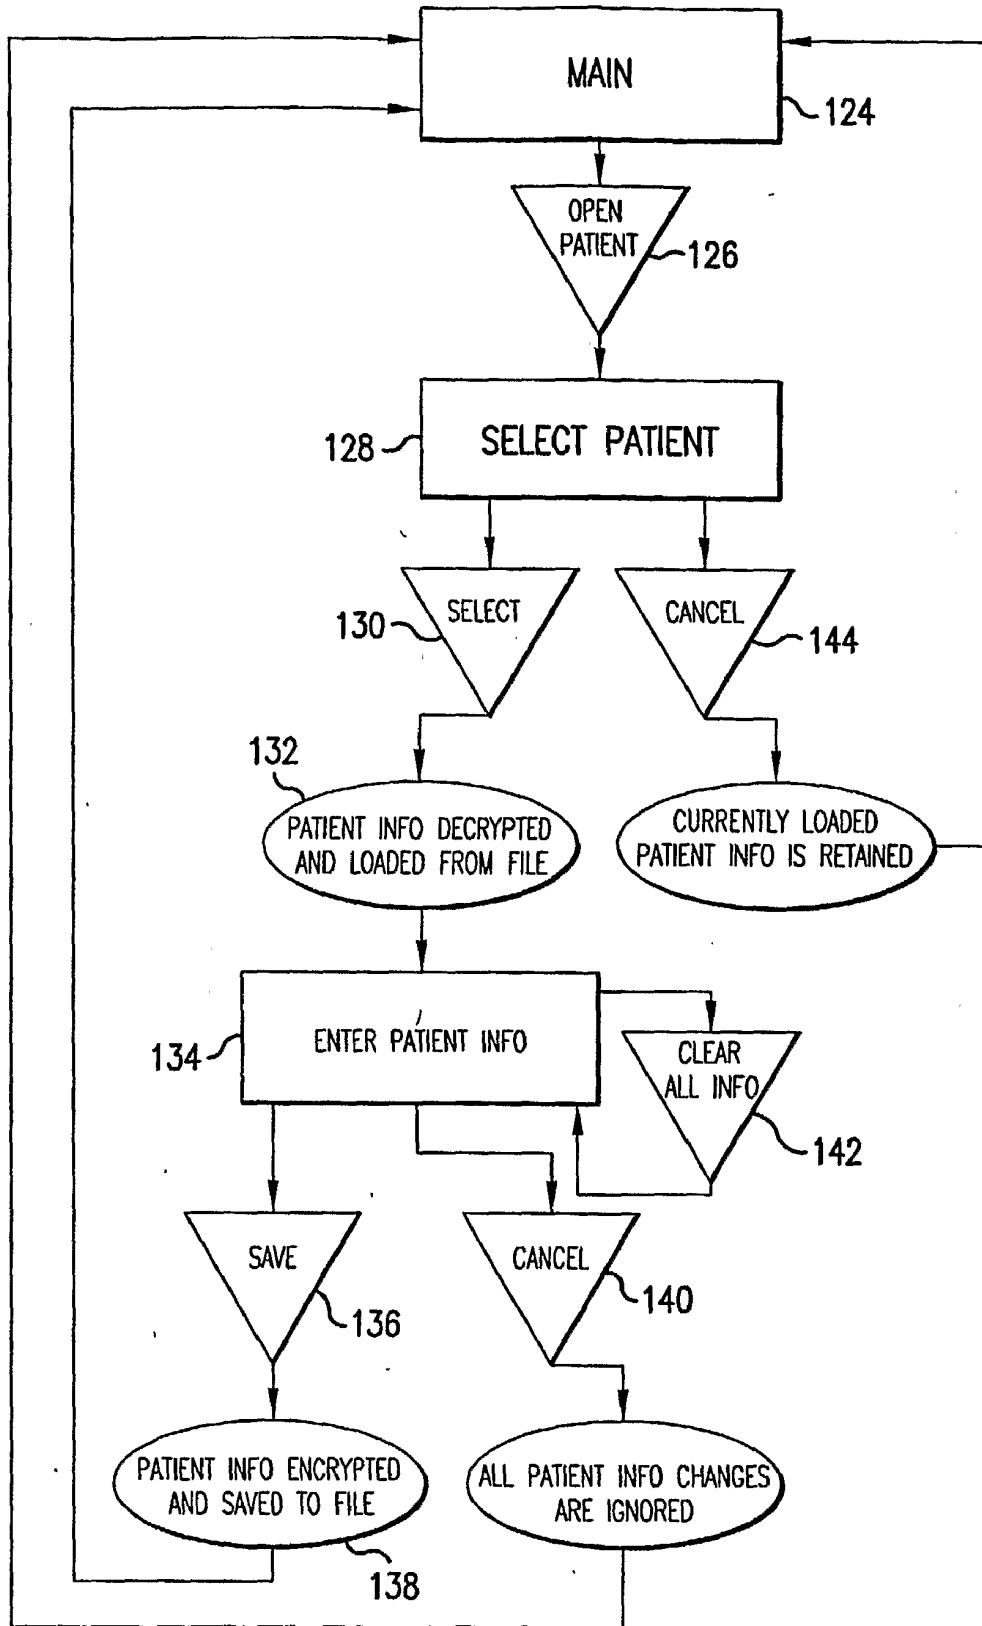


FIG.11

10/20

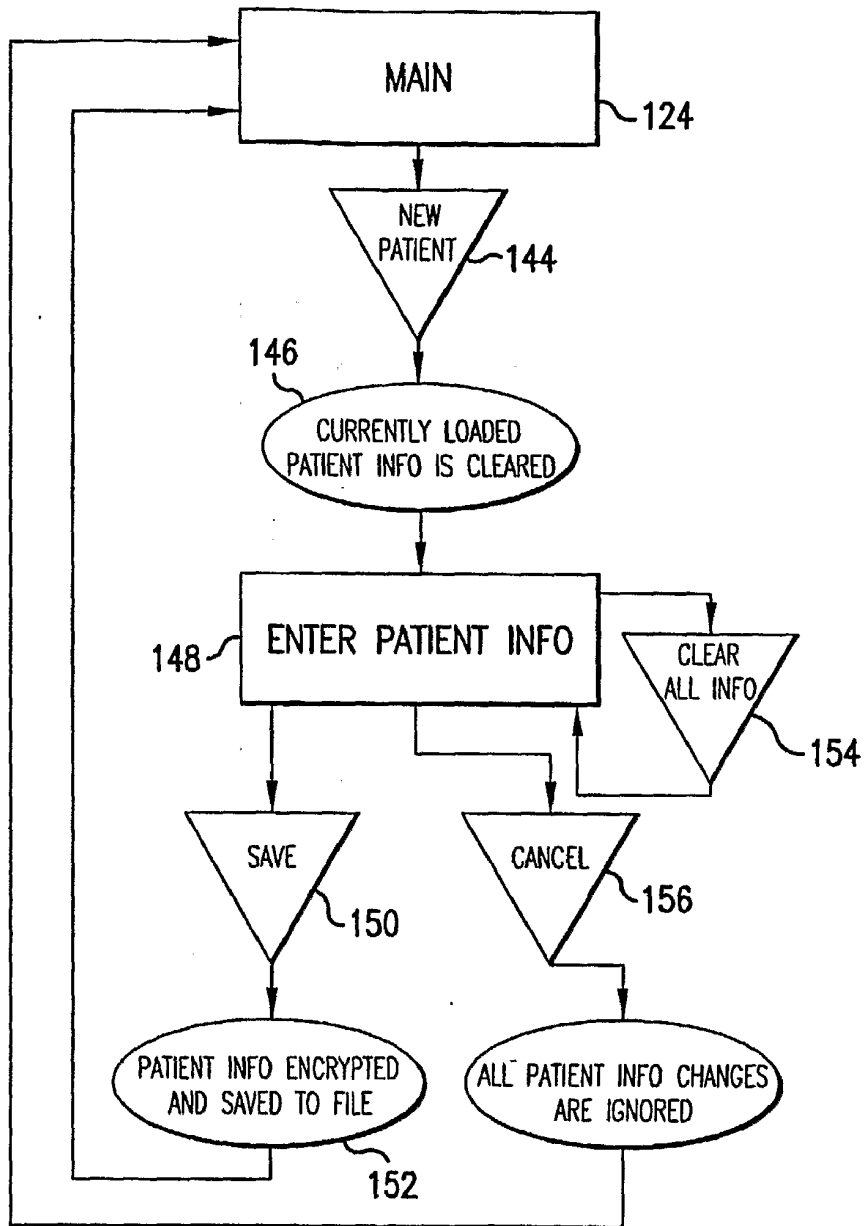


FIG.12

11/20

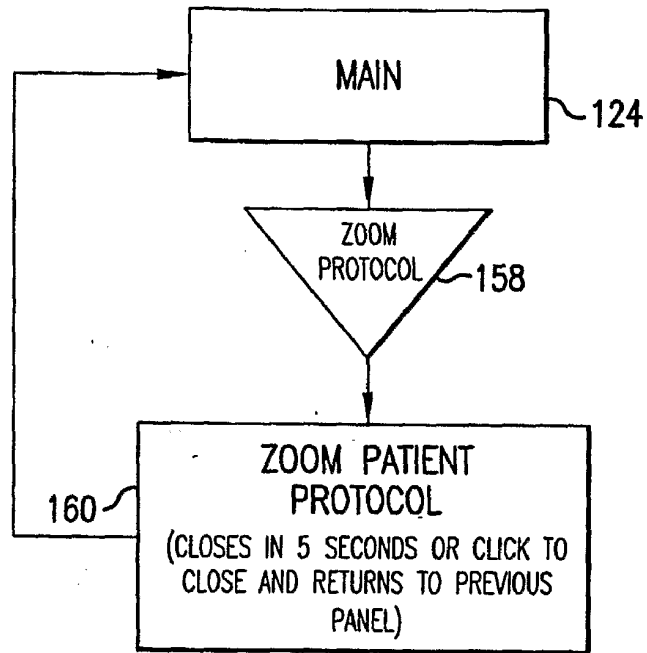


FIG.13

12/20

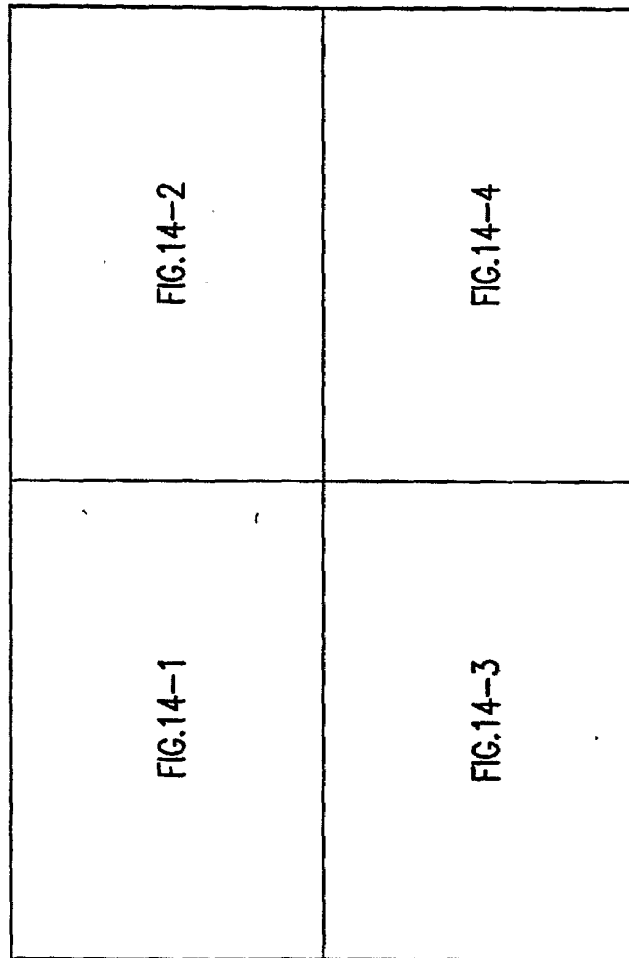


FIG.14

13/20

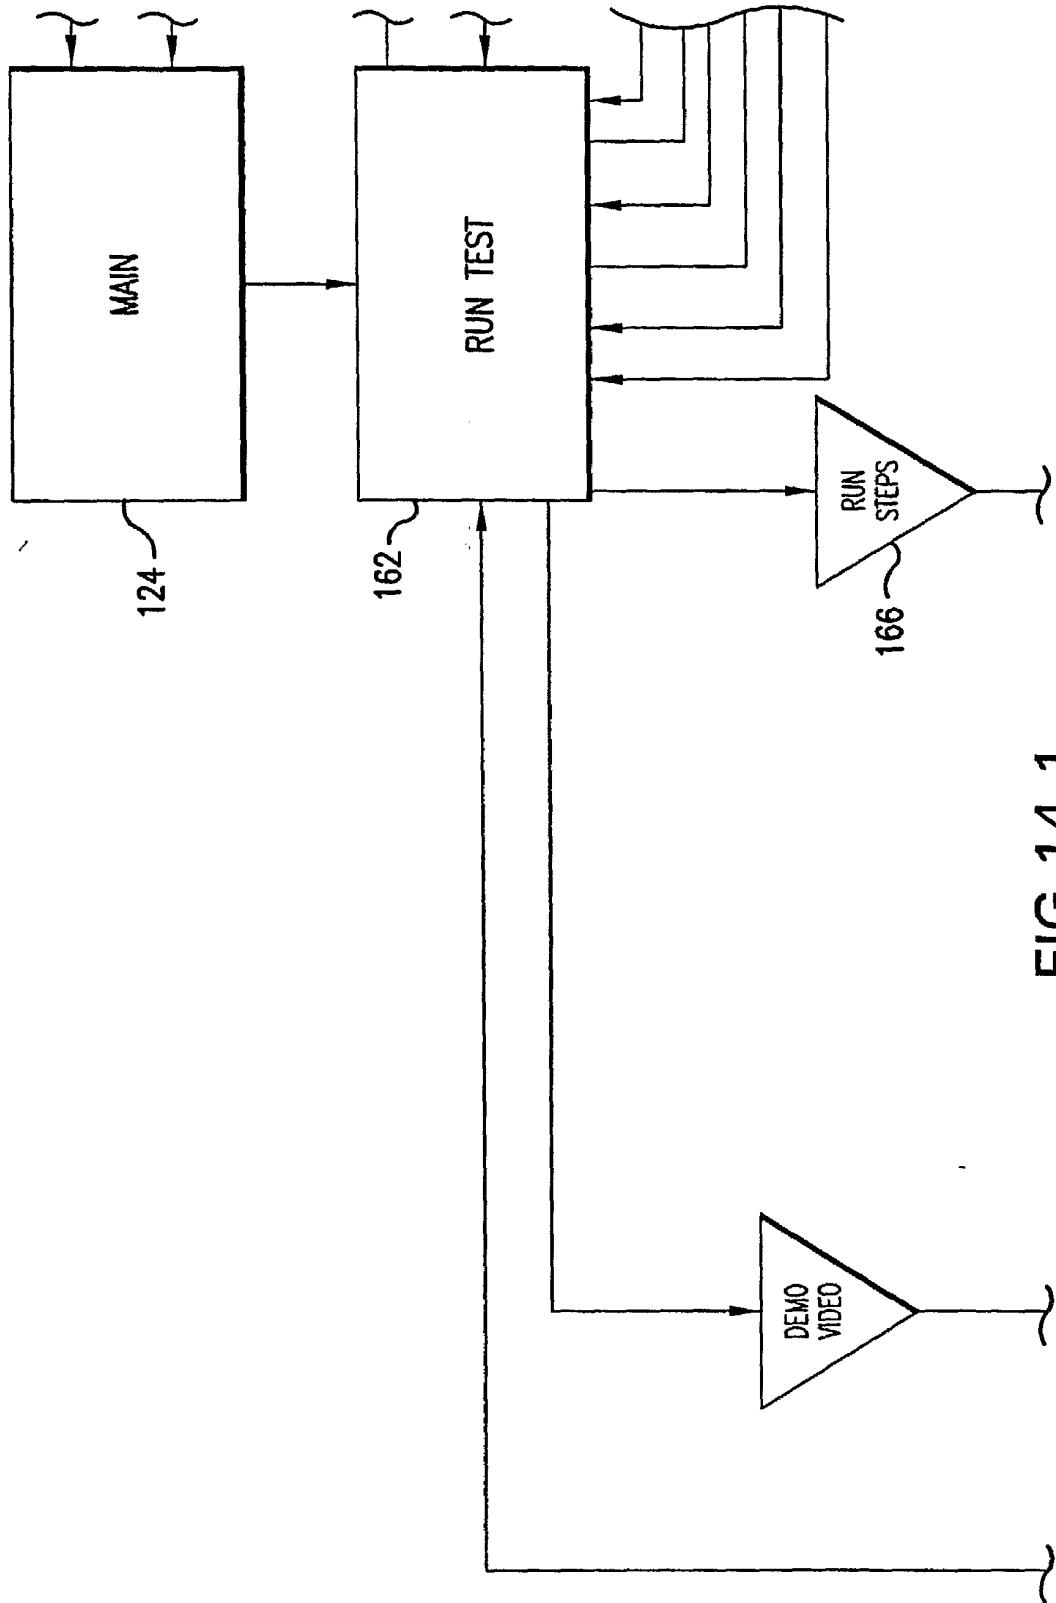


FIG.14-1

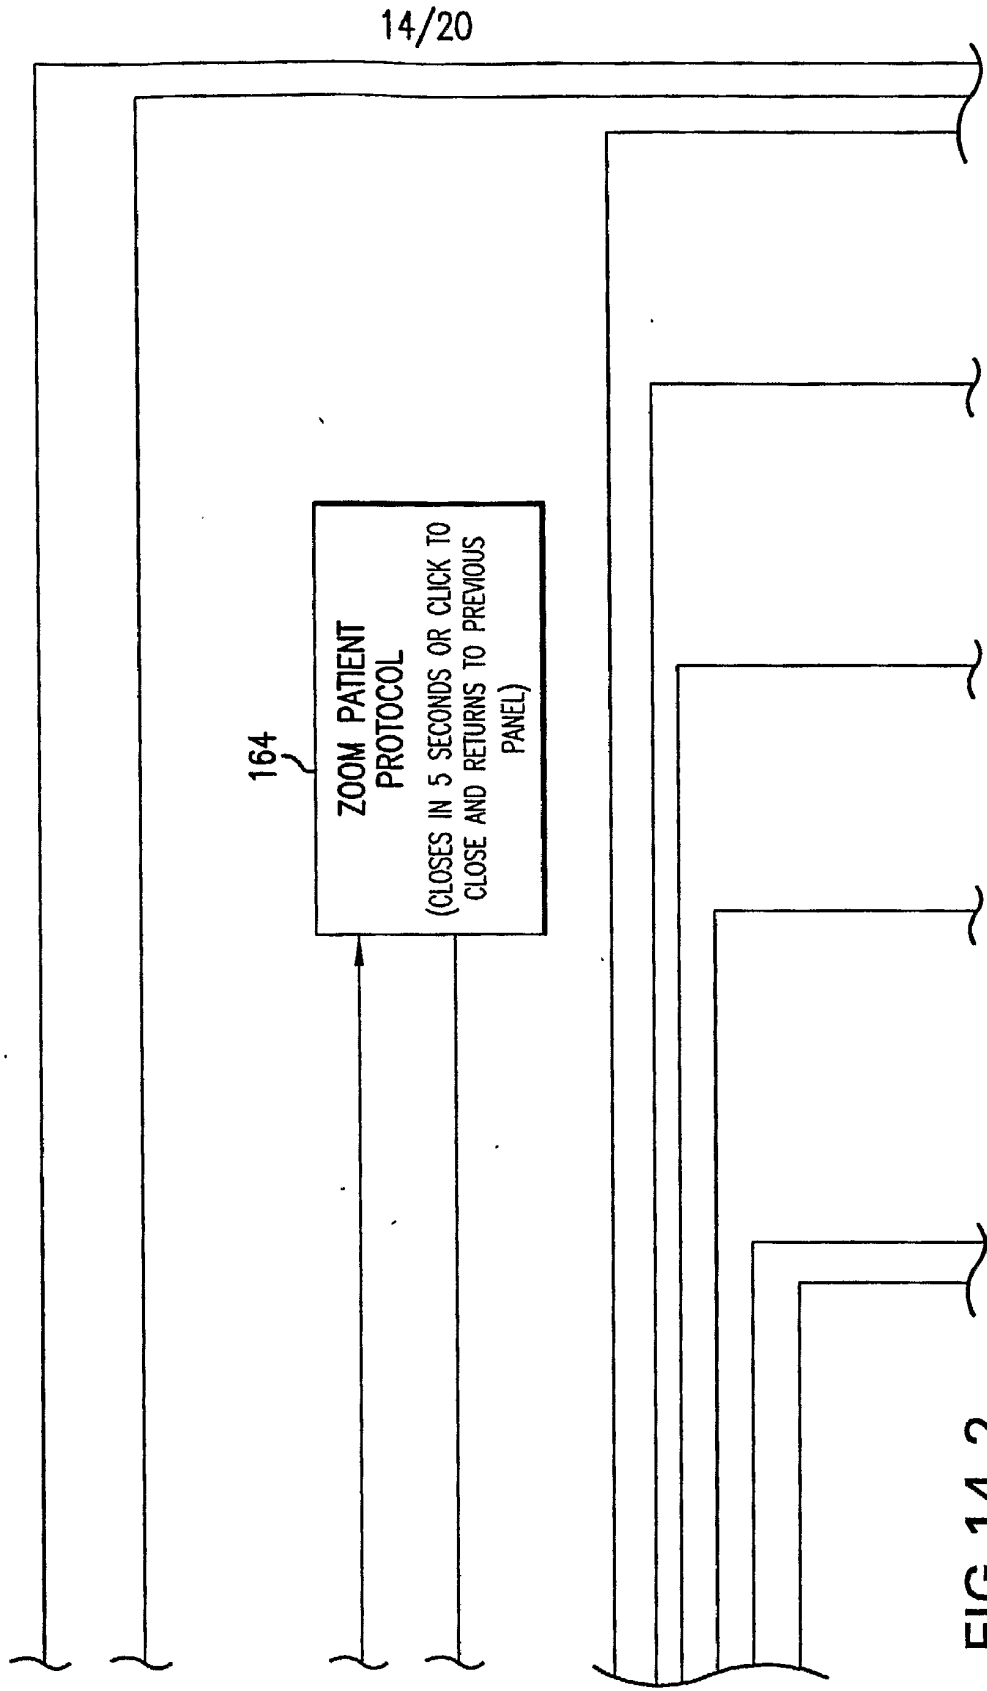


FIG. 14-2

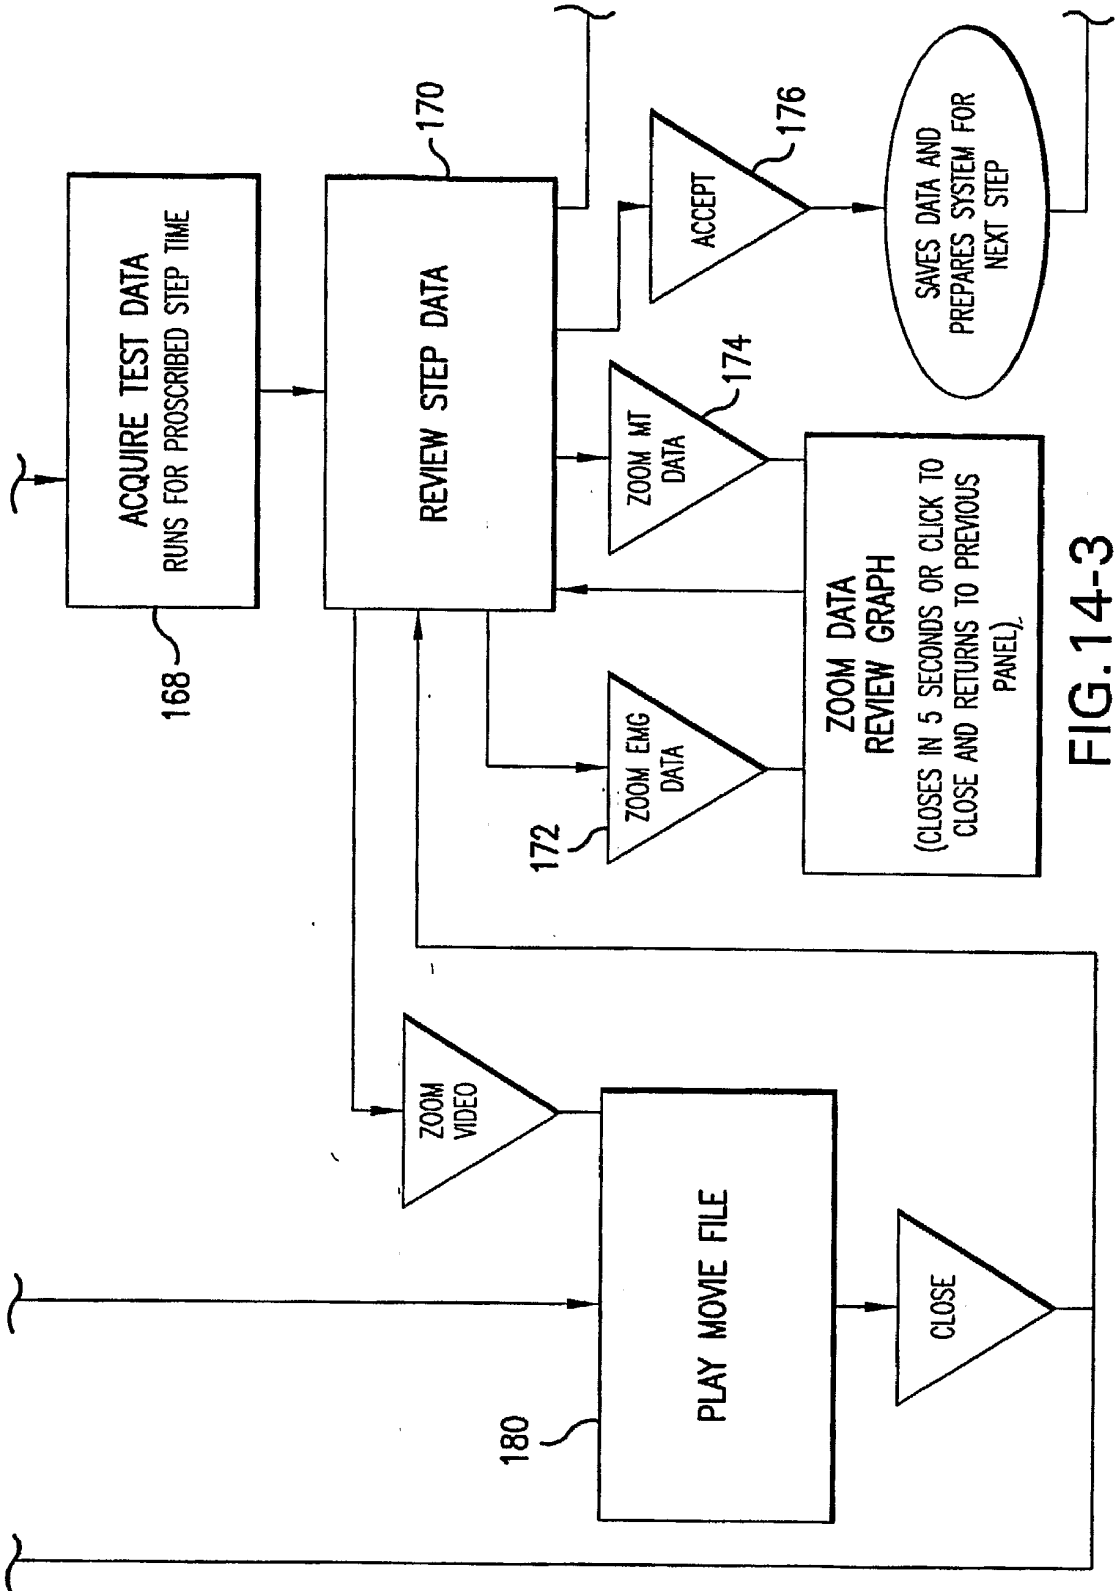


FIG. 14-3

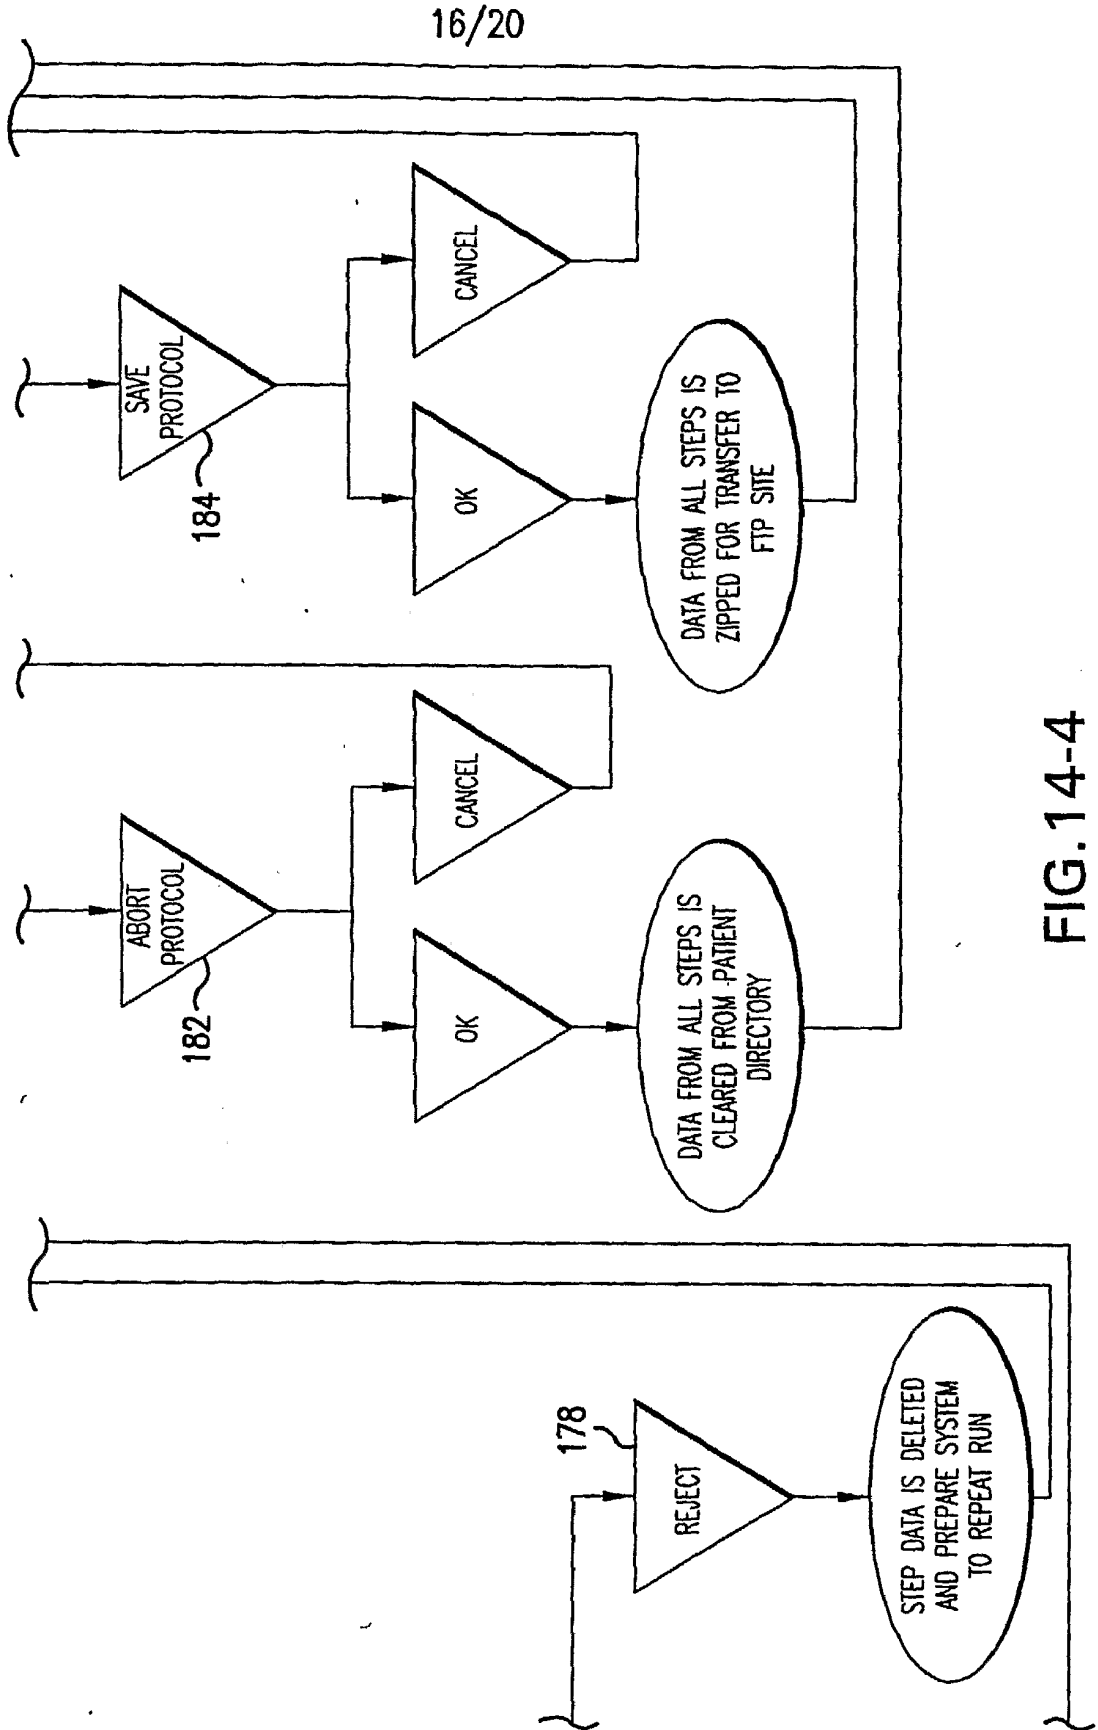


FIG. 14-4

17/20

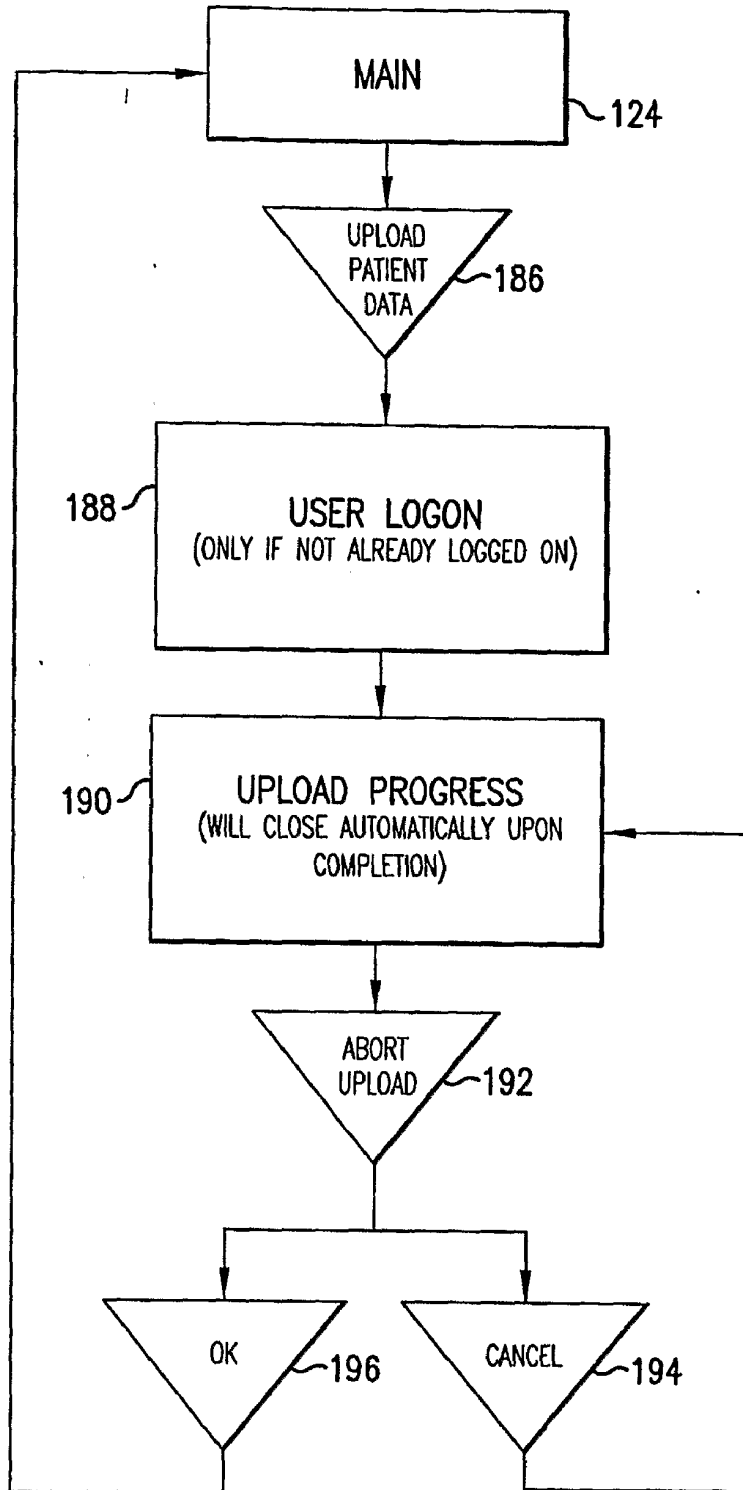


FIG. 15

18/20

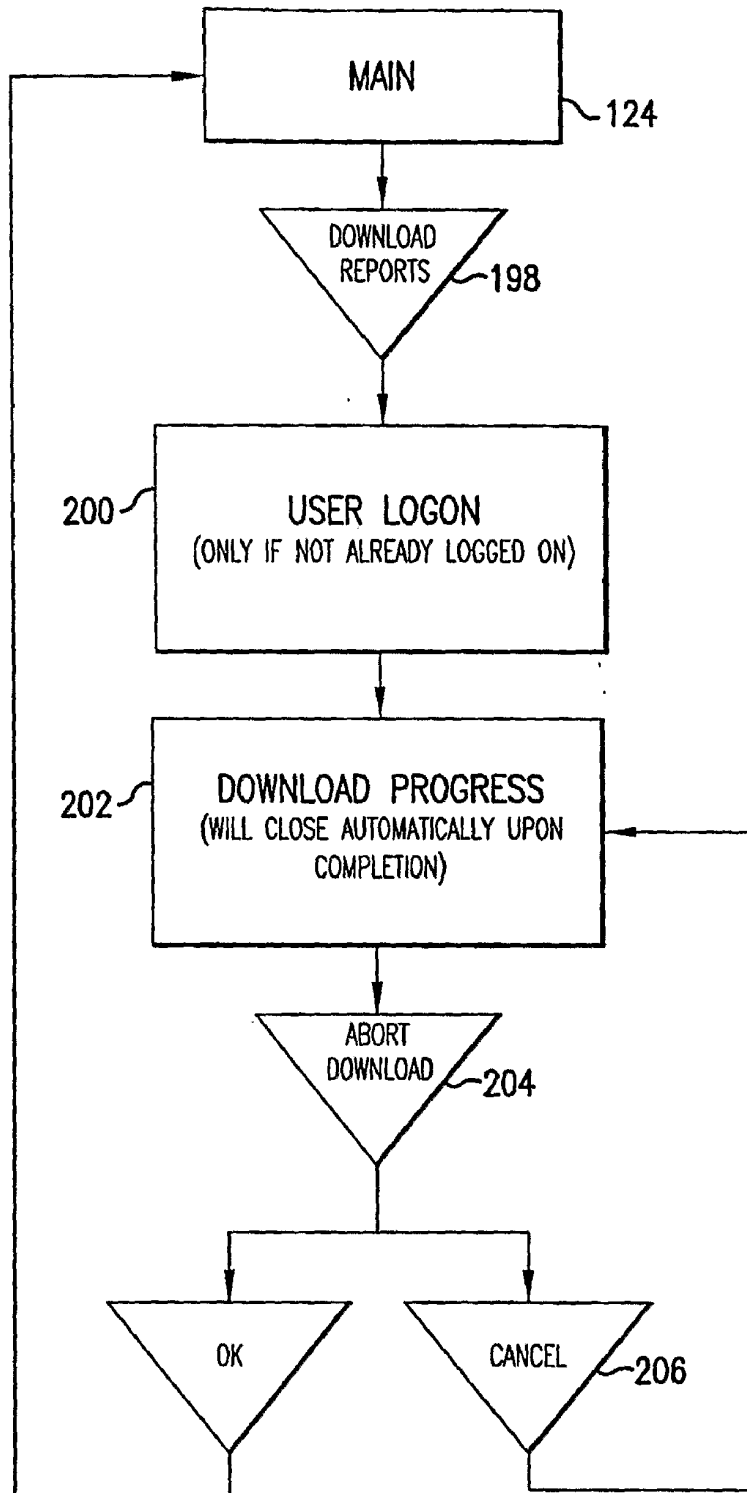


FIG. 16

19/20

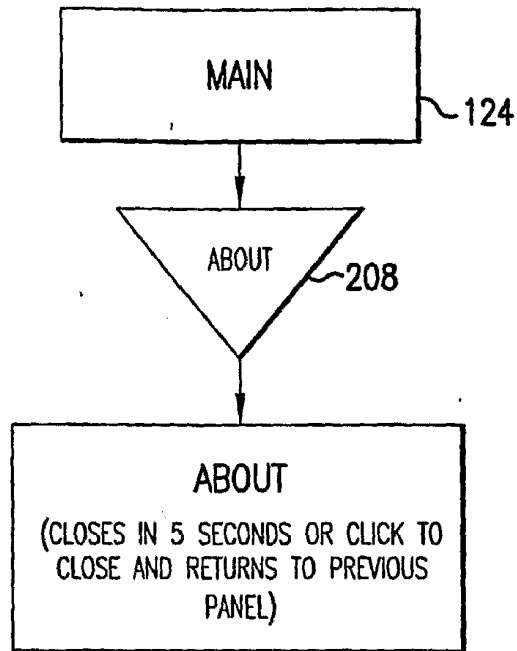


FIG. 17

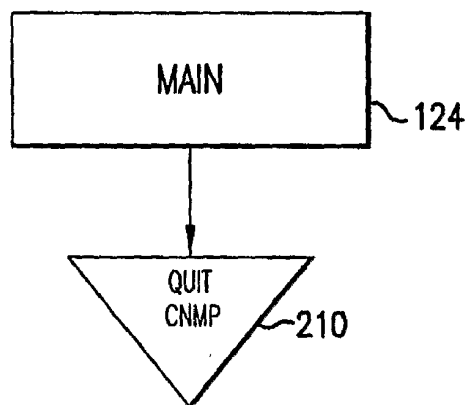


FIG. 18

20/20

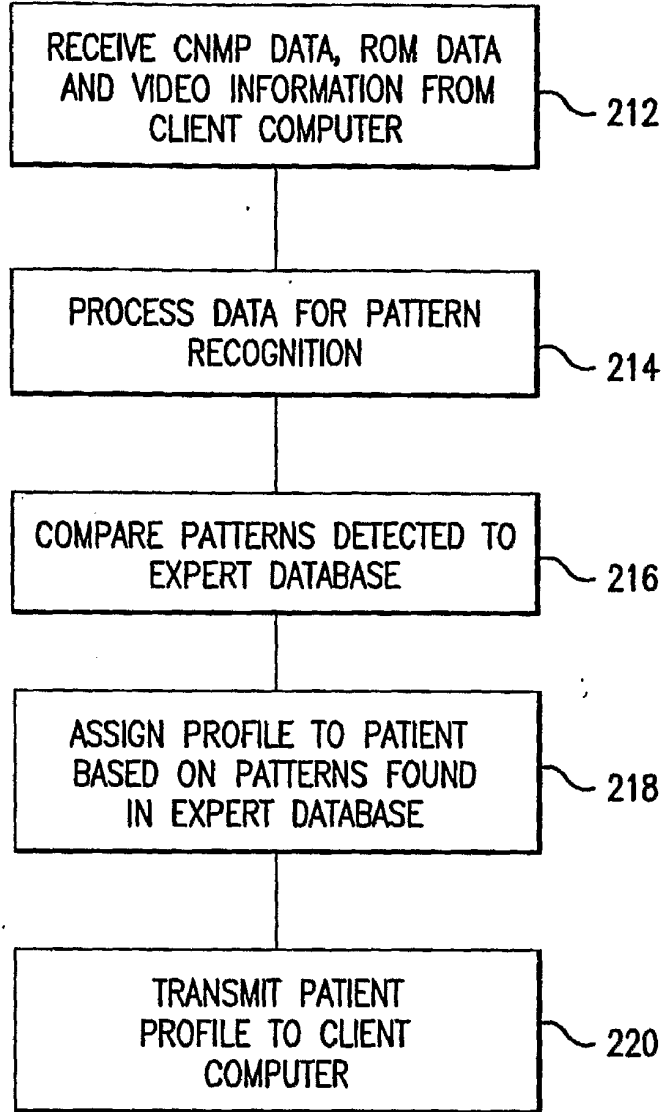


FIG. 19

专利名称(译)	综合神经肌肉探查器		
公开(公告)号	EP1651106A4	公开(公告)日	2009-05-27
申请号	EP2004777963	申请日	2004-07-09
[标]申请(专利权)人(译)	医疗科技UNLTD		
申请(专利权)人(译)	医疗技术UNLIMITED INC.		
当前申请(专利权)人(译)	医疗技术UNLIMITED INC.		
[标]发明人	VITIELLO MARCO N CYPHERY DEAN BUTLER LANCE H		
发明人	VITIELLO, MARCO, N. CYPHERY, DEAN BUTLER, LANCE, H.		
IPC分类号	A61B5/04 A61B A61B5/00 A61B5/0488 A61B5/11 A61B5/22		
CPC分类号	A61B5/1123 A61B5/0002 A61B5/0488 A61B5/1127 A61B5/224 A61B5/225 A61B5/4519 A61B5/4528 A61B2503/40		
代理机构(译)	GILL , DAVID ALAN		
优先权	60/485979 2003-07-09 US		
其他公开文献	EP1651106A2		
外部链接	Espacenet		

摘要(译)

全面的神经肌肉轮廓仪 (CNMP) 可以观察人体和马肌的功能和特征。CNMP由一个集成EMG技术，电磁运动范围 (ROM) 技术和功能容量传感器的集成系统组成。来自设备的输出信号被数字化并存储在计算机存储器中。可以将数据发送到服务器计算机以进行进一步分析。服务器计算机检查数据以确定模式并咨询专家数据库以基于检测到的模式和模式组合确定诊断。