



EUROPEAN PATENT APPLICATION

(43) Date of publication:

23.10.2013 Bulletin 2013/43

(51) Int Cl.:

A61B 5/00 (2006.01)

G06F 19/00 (2011.01)

A61B 5/1495 (2006.01)

A61B 10/00 (2006.01)

(21) Application number: **13163712.6**

(22) Date of filing: **15.04.2013**

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

Designated Extension States:

BA ME

(72) Inventors:

- **Hosaka, Shoichi**
Tokyo (JP)
- **Aoki, Toshiki**
Tokyo (JP)
- **Maeda, Shogo**
Tokyo (JP)
- **Uchida, Osamu**
Osaka (JP)

(30) Priority: **16.04.2012 JP 2012092790**

(71) Applicant: **Nihon Kohden Corporation**
Shinjuku-ku
Tokyo (JP)


(74) Representative: **Ilgart, Jean-Christophe et al**
BREVALEX
95 rue d'Amsterdam
75378 Paris Cedex 8 (FR)

(54) **Biological information monitoring apparatus**

(57) A biological information monitoring apparatus includes: a measurer which is configured to measure biological information of a subject; a display on which a measurement value of the biological information measured by the measurer is displayed; a calibration controller which, when a predetermined condition is satisfied, is

configured to perform a calibration process on the measurer; a time measurer which is configured to acquire a remaining time before the calibration process is ended; and a display controller which is configured to cause an index indicating the remaining time to be displayed on the display.

FIG. 1

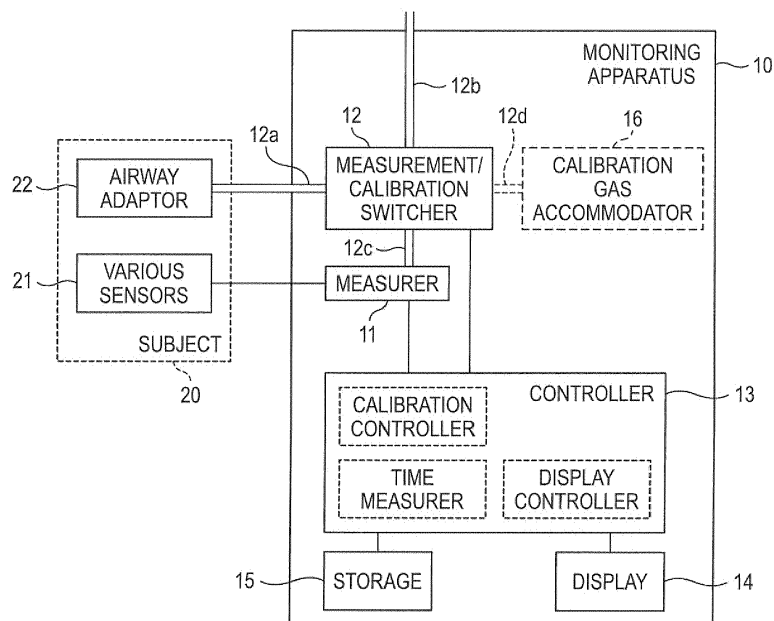

Description

CROSS-REFERENCE TO RELATED APPLICATION(S)

[0001] This application is based upon and claims the benefit of priority from prior Japanese patent application No. 2012-092790, filed on April 16, 2012, the entire contents of which are incorporated herein by reference.

BACKGROUND

[0002] The presently disclosed subject matter relates to a biological information monitoring apparatus which measures biological information of the subject, and which includes a display that displays the measurement value of the biological information.

[0003] As an apparatus of this kind, there is an apparatus in which the concentration of a predetermined gas (carbon dioxide, oxygen, a volatile anesthetic agent, or the like) contained in the expired gas of the subject is measured as biological information by a sensor, and the measurement value is displayed on a display (for example, see JP- T- 2010- 508523 and JP- A- 2000- 245711) .

[0004] In a sensor, the measurement accuracy may be sometimes lowered over time by various causes, and therefore calibration must be performed at an adequate timing. In an apparatus of this kind, when a given requirement is satisfied (for example, in activation of the apparatus, or elapse of a prescribed time period from a previous calibration process), the operation mode is automatically shifted to a mode in which a calibration process is performed. During a period when a calibration process is performed, biological information cannot be measured, and therefore the portion in which the biological information is to be displayed is set to a state where a measurement value is not displayed (for example, "---" is displayed) (hereinafter, the state is referred to as the measurement value non-displayed state).

[0005] From the standpoint of the observer monitoring biological information, it is often that the shifting to the calibration mode cannot be expected. Furthermore, the time period required for calibration is different in each case. Therefore, waiting for the end of the calibration process in which the end of the process is not known, and which is performed in the state measurement value non-displayed state causes the observer to have serious stress. In the case where such a monitoring apparatus is used for monitoring the condition of the patient under surgery, moreover, waiting for the end of the calibration process causes the working efficiency of the surgery personnel to be lowered.

SUMMARY

[0006] The presently disclosed subject matter may provide a biological information monitoring apparatus which can relieve the stress that, during shifting to the calibration mode, is applied to the observer monitoring

biological information, and avoid lowering of the working efficiency.

[0007] The biological information monitoring apparatus may comprise: a measurer which is configured to measure biological information of a subject; a display on which a measurement value of the biological information measured by the measurer is displayed; a calibration controller which, when a predetermined condition is satisfied, is configured to perform a calibration process on the measurer; a time measurer which is configured to acquire a remaining time before the calibration process is ended; and a display controller which is configured to cause an index indicating the remaining time to be displayed on the display.

[0008] The index may be at least one of a numeral and a progress bar.

[0009] Based on the predetermined condition, the time measurer may select one of a plurality of predetermined values which indicate times required for the calibration process, respectively, and, based on the selected one of the plurality of predetermined values, acquire the remaining time.

[0010] Based on information indicating a relationship between the predetermined condition and a time required for the calibration process, the time measurer may calculate or acquire the remaining time.

[0011] The biological information may include at least one of a concentration of a predetermined gas contained in an expired gas of the subject, a concentration of an anesthetic agent contained in an expired gas of the subject, a respiratory volume, and an airway pressure.

[0012] The biological information may include at least two or more of an electrocardiogram, a pulse wave, and a blood pressure, and the measurer may include a calculator which is configured to calculate a cardiac output of the subject, based on the at least two or more biological information.

[0013] The predetermined condition may relate to at least one of an elapsed time from a previous calibration process, an elapsed time from activation of the biological information monitoring apparatus, a current time, a temperature in the biological information monitoring apparatus, an atmospheric pressure, an input of an instruction by an operator, and stabilization of a signal relating to the biological information.

BRIEF DESCRIPTION OF THE DRAWINGS

[0014]

Fig. 1 is a functional block diagram showing the configuration of a monitoring apparatus of a first embodiment of the presently disclosed subject matter.

Fig. 2 is a view showing an example of a screen displayed on a display of the monitoring apparatus of Fig. 1.

Fig. 3 is a view showing another example of the screen displayed on the display of the monitoring

apparatus of Fig. 1.

Fig. 4 is a functional block diagram showing the configuration of a monitoring apparatus of a second embodiment of the presently disclosed subject matter.

Fig. 5 is a view showing a further example of the screen displayed on the display of the monitoring apparatus of Fig. 1.

Fig. 6 is a view showing a still further example of the screen displayed on the display of the monitoring apparatus of Fig. 1.

DETAILED DESCRIPTION OF EXEMPLARY EMBODIMENTS

[0015] Hereinafter, embodiments of the presently disclosed subject matter will be described in detail with reference to the accompanying drawings.

[0016] Fig. 1 is a functional block diagram showing the configuration of a biological information monitoring apparatus 10 (hereinafter, referred to simply as the monitoring apparatus) of a first embodiment of the presently disclosed subject matter. The monitoring apparatus 10 includes a measurer 11, a measurement/calibration switcher 12, a controller 13, a display 14, and a storage 15.

[0017] A plurality of kinds of signals relating to biological information which is acquired through various sensors 21 (including electrodes, a cuff, and the like) attached to the subject 20 are supplied to the measurer 11 directly or through a network. Examples of biological information of the subject are the pulse rate, an electrocardiogram, the blood pressure, the oxygen saturation, etc. The measurer 11 obtains measurement values of various kinds of biological information based on the supplied signals.

[0018] The measurement/calibration switcher 12 includes a related-art valve device (not shown) which selectively causes one of a respiratory gas introducing passage 12a and an atmosphere opening passage 12b to communicate with a measurement gas passage 12c. The respiratory gas introducing passage 12a is connected an airway adaptor 22 which is attached to the mouth or nose of the subject 20. One end of the atmosphere opening passage 12b is opened in the atmosphere.

[0019] The valve device of the measurement/calibration switcher 12 normally causes the respiratory gas introducing passage 12a to communicate with the measurement gas passage 12c. The respiratory gas of the subject 20 is introduced into the measurer 11 through the respiratory gas introducing passage 12a and the measurement gas passage 12c.

[0020] The measurer 11 includes various related-art gas sensors (not shown), and is configured so as to measure the concentrations of specific gasses contained in the respiratory gas of the subject. In the embodiment, the measurer 11 acquires measurement values of the concentrations of specific gasses, i.e., carbon dioxide (CO₂), oxygen (O₂), laughing gas (N₂O), and isoflurane

(ISO) which is a volatile anesthetic agent.

[0021] The controller 13 is communicably connected to the measurer 11, and receives measurement values which are acquired by the measurer 11 based on the inputs from the various sensors 21, and measurement values of the concentrations of the various gasses which are acquired from the respiratory gas of the subject.

[0022] The display 14 is a displaying device which is disposed in the front surface of the apparatus, and communicably connected to the controller 13. The controller 13 causes the various measurement values which are received through the measurer 11, to be displayed in real time on the display 14.

[0023] Fig. 2 is a view showing an example of a screen displayed on the display 14. Based on the measurement values which are supplied from the measurer 11 to the controller 13, the various kinds of biological information are displayed in the form of a waveform or numerals. In the lower left portion of the screen, an area for displaying the measurement values of the concentrations of carbon dioxide, oxygen, laughing gas, and isoflurane which are contained in the expired gas of the subject 20 is disposed. Specifically, the measurement value of the concentration of carbon dioxide is displayed in a first concentration display region 14a, that of oxygen is displayed in a second concentration display region 14b, and the measurement values of the concentrations of laughing gas and isoflurane are displayed in a third concentration display region 14c.

[0024] The accuracies of the gas sensors provided in the measurer 11 are varied over time or depending on the surrounding environment. In order to supply correct measurement values to the controller 13, it is necessary to calibrate the gas sensors at an adequate timing. The controller 13 functions as the calibration controller in the presently disclosed subject matter, and is configured so that, when predetermined conditions are satisfied, it is automatically shifted to a calibration mode, and performs a calibration process on the gas sensors.

[0025] Specifically, the calibration process for the gas sensors is performed immediately after activation of the monitoring apparatus 10, and at a timing when the elapsed time from the previous calibration process exceeds a predetermined value. In this case, the controller 13 functions as a time measurer to perform time measurement, and it is determined that the elapsed time from the previous calibration reaches the predetermined value.

[0026] As shown in Fig. 1, the controller 13 is communicably connected to the measurement/calibration switcher 12. When the predetermined conditions are satisfied, the controller 13 controls the valve device of the measurement/calibration switcher 12 so as to cause the atmosphere opening passage 12b to communicate with the measurement gas passage 12c. As a result, the atmosphere is introduced into the measurer 11 through the atmosphere opening passage 12b and the measurement gas passage 12c, and the gas sensors are calibrated

based on the composition of the atmosphere. The calibration process is well known, and therefore its detailed description is omitted.

[0027] During execution of the calibration process, the respiratory gas of the subject 20 is not introduced into the measurer 11 through the respiratory gas introducing passage 12a. Therefore, the measurer 11 cannot acquire measurement values of the concentrations of the specific gasses contained in the expired gas of the subject 20. In this case, as shown in Fig. 3, the second concentration display region 14b and the third concentration display region 14c are set to the measurement value non-displayed state where "---" is displayed.

[0028] By contrast, the controller 13 which functions as the time measurer acquires the remaining time before the calibration process for the gas sensors is ended. In the case where the calibration process which is to be performed after activation of the apparatus requires 60 seconds, and those which are to be periodically executed after each elapse of a predetermined time (for example, each elapse of 1 hour after activation) require 20 second, for example, two predetermined values which indicate the required times for the calibration process, respectively, i.e., 60 seconds and 20 seconds are stored in the storage 15. In accordance with the conditions which are satisfied at the timing when the calibration process is to be performed, the controller 13 selects one of the predetermined values, and reads out it.

[0029] The controller 13 which functions as the time measurer starts the time measuring process for the predetermined value that is read out from the storage 15. In the calibration process which is performed immediately after activation of the apparatus, for example, the process of measuring the time or 60 seconds which is the predetermined value read out from the storage 15 is started. The remaining time before the calibration process is ended is acquired by direct subtraction of the read out predetermined value, or by subtracting the measured time from the read out predetermined value.

[0030] The controller 13 also functions as the display controller in the presently disclosed subject matter, and causes an index indicating the acquired remaining time to be displayed on the display 14. In the first concentration display region 14a, as shown in Fig. 3, a message which is an index, and which indicates the remaining time is displayed in place of the display of "---" showing the state where the measurement of the concentration of carbon dioxide is disabled. The example of Fig. 3 shows a state where 30 seconds have elapsed after starting of the calibration process which is performed after activation of the monitoring apparatus 10, and a message 30 of "30 seconds remain" is displayed in the first concentration display region 14a.

[0031] According to the configuration of the embodiment, the observer monitoring the biological information can view the remaining time before the calibration process is ended. Even when the shifting to the calibration mode is unexpected to the observer monitoring the bio-

logical information, therefore, the operator can know the remaining time, and hence stress during the waiting state can be largely relieved. When the remaining time which is known by the observer is allocated for another work, or like, the working efficiency of nursing care or surgery can be improved.

[0032] Based on predetermined conditions, the controller 13 functioning as the time measurer selects one of a plurality of predetermined values which indicate required times for the calibration process, respectively, from the storage 15, and, based on the selected predetermined value, acquires the remaining time. Therefore, it is possible to provide a display mode in which stress can be relieved while suppressing the calculation load of the controller 13.

[0033] The controller 13 is an arithmetic processing circuit which is configured by including an arithmetic device such as a CPU. The functions as the above-described calibration controller, time measurer, and display controller can be realized by the operation of hardware such as circuit devices, that of software such as programs stored in the arithmetic device, or a combination of these operations.

[0034] Next, a monitoring apparatus 10A of a second embodiment of the presently disclosed subject matter will be described with reference to Fig. 4. Components which are identical with or equivalent to those of the monitoring apparatus 10 of the first embodiment are denoted by the same reference numerals, and duplicated description is omitted.

[0035] The monitoring apparatus 10A of the embodiment includes a measurer 11A. The measurer 11A calculates the cardiac output based on an electrocardiogram (ECG) and pulse wave which are biological information measured from the subject 20.

[0036] Signals which relate to the electrocardiogram and the pulse wave, respectively, and which are acquired through an ECG sensor 21a and pulse wave sensor 21b that are attached to the subject 20 are supplied to an ECG measurer 11a and pulse wave measurer 11b in the measurer 11A. The measurer 11A further includes a calculator 11c. The calculator 11c obtains by calculation the cardiac output of the subject 20 by, for example, the technique disclosed in Japanese Patent No. 4,742,644. It is assumed that "measurement value" in the presently disclosed subject matter includes a value which is obtained by calculation based on biological information in this way.

[0037] In order to obtain the cardiac output, the calculator 11c requires information (for details, see JP-A-2010-246801) of the subject, and an ECG signal and pulse wave signal which are stably obtained for several minutes. Therefore, the calculation result (measurement value) of the cardiac output cannot be immediately sent to the controller 13, and hence a calibration process for several minutes is necessary for obtaining the average value of the cardiac output. When the controller 13 functions as the calibration controller, the calibration process

is performed.

[0038] The calibration time depends also on the measurement environment, and therefore is hardly identified in an unambiguous manner. This causes the observer to have serious stress. In the embodiment, therefore, a measurement/calibration switcher 12A transmits either one of a calculation result (measurement value) of the cardiac output which is obtained as a result of calculation, and a signal indicating that the measurer 11A is performing a calculation process, to the controller 13 in accordance with the operation status of the calculator 11c.

[0039] Upon receiving the signal indicating that the measurer 11A is performing a calculation process, the controller 13 which functions as the time measurer in the presently disclosed subject matter acquires the remaining time before the calibration process performed by the measurer 11A is ended (i.e., the time elapsing before the state where the calculation result can display is attained) in a similar manner as the first embodiment. The controller 13 which functions as the display controller in the presently disclosed subject matter causes the index indicating the acquired remaining time to be displayed on the display 14 in a similar manner as the first embodiment.

[0040] The embodiments have been described in order to facilitate understanding of the presently disclosed subject matter, and are not intended to limit the presently disclosed subject matter. It is a matter of course that the presently disclosed subject matter may be changed or improved without departing the spirit thereof, and includes equivalents thereof.

[0041] The index which is displayed on the display 14 by the controller 13 functioning as the display controller, and which indicates the remaining time before the calibration process is ended is not limited to the above-described one, and may be displayed by using adequate characters, symbol, graph, chart, or the like from which the remaining time can be known.

[0042] As shown in Fig. 5, for example, a progress bar 40 which visualizes the progress of the process may be used as the index. The controller 13 functioning as the time measurer obtains the rate of the elapsed time from the calibration process with respect to the predetermined value which is read out from the storage 15, and which indicates the required time for the calibration process, and the controller 13 functioning as the display controller changes the length of the progress bar 40 in accordance with the obtained rate. According to the configuration, the observer monitoring a biological signal can know the progress situation (the amount of the remaining time) of the calibration process by means of viewing, and stress during the waiting state can be relieved.

[0043] As shown in Fig. 6, both the message 30 including numerals and the progress bar 40 may be used as the index. In this example, a dedicated display region 14d for displaying the index indicating the remaining time before the calibration process is ended is displayed in place of the first to third concentration display regions 14a to 14c where the measurement non-displayed state

is set. In the figure, the state where 2 seconds have elapsed after the measurement of 20 seconds read out as the predetermined value from the storage 15 is started as a result that the elapsed time from the previous calibration reaches the predetermined value is exemplarily shown.

[0044] In place of or in addition to the configuration where the predetermined value indicating the required calibration time is previously stored in the storage 15, a configuration may be employed where the storage 15 stores information indicating relationships between the predetermined conditions and the required calibration time in the form of a table or a function, and the controller 13 functioning as the time measurer calculates or acquires the remaining time before the calibration process is ended, based on the information.

[0045] In place of or in addition to the conditions where the monitoring apparatus 10 has been activated, and where the elapsed time from the previous calibration process reaches the predetermined value, conditions such as the elapsed time from activation of the monitoring apparatus 10, the current time, the temperature in the apparatus, the atmospheric pressure, an input of an instruction for executing the calibration process by the operator, and stabilization of a signal relating to the biological information may set as the predetermined conditions. According to the configuration, even in a situation where the required time is different depending on the predetermined conditions, the remaining time can be correctly acquired.

[0046] With respect to the elapsed time and the current time, the time measurer provided in the controller 13, an internal timer (not shown), or the like is used, and, with respect to the temperature in the apparatus and the atmospheric pressure, sensors which can measure these parameters are disposed, whereby it is enabled to determine whether the predetermined conditions are satisfied or not.

[0047] The biological information which relates to the respiration of the subject 20, and which is measured by the measurer 11 of the monitoring apparatus 10 of the first embodiment is not limited to the above-described concentrations of carbon dioxide, oxygen, laughing gas, and isoflurane. Another example of the volatile anesthetic agent which is to be measured is at least one of enflurane, sevoflurane, halothane, and desfluran. Alternatively, a configuration where the respiratory volume and the airway pressure are measured as biological information may be employed.

[0048] A configuration where, as indicated by the broken line in Fig. 1, a calibration gas passage 12d connected to a calibration gas accommodator 16 is disposed in place of or in addition to the atmosphere opening passage 12b may be employed. An adequate gas which is necessary for the calibration process is filled in the calibration gas accommodator 16. When the predetermined conditions are satisfied, the controller 13 functioning as the calibration controller controls the valve device of the

measurement/calibration switcher 12 so as to cause the calibration gas passage 12d to communicate with the measurement gas passage 12c. The calibration gas filled in the calibration gas accommodator 16 is introduced into the measurer 11 through the calibration gas passage 12d and the measurement gas passage 12c, and the gas sensors are calibrated based on the composition of the calibration gas.

[0049] Alternatively, a configuration where a cylinder in which a calibration gas of known concentration is filled is connected to the atmosphere opening passage 12b may be employed. In this case, the controller 13 functioning as the calibration controller controls the valve device so as to cause the atmosphere opening passage 12b to communicate with the measurement gas passage 12c. The calibration gas filled in the cylinder is introduced into the measurer 11 through the atmosphere opening passage 12b and the measurement gas passage 12c.

[0050] The biological information of the subject 20 which is to be measured by the measurer 11A of the monitoring apparatus 10A of the second embodiment is not limited to an ECG and the pulse wave. As required, the biological information may include information relating to the blood pressure, such as the pulse pressure, or a configuration where the cardiac output is obtained by using at least two of the kinds of information may be employed.

[0051] In the monitoring apparatus 10A of the second embodiment, a configuration may be employed where the function as the time measurer is realized by at least one of the calculator 11c and the measurement/calibration switcher 12A in place of or in addition to the controller 13.

[0052] The display 14 is not always necessary to be disposed as a part of the monitoring apparatus 10. A configuration where a displaying device which is disposed outside the monitoring apparatus 10, and which is communicably connected to the controller 13 functions as the display 14 may be employed.

[0053] The storage 15 is not always necessary to be disposed separately from the controller 13, and may be configured as a part of a memory of the processing circuit constituting the controller 13.

Claims

1. A biological information monitoring apparatus comprising:

a measurer which is configured to measure biological information of a subject;
 a display on which a measurement value of the biological information measured by the measurer is displayed;
 a calibration controller which, when a predetermined condition is satisfied, is configured to perform a calibration process on the measurer;

a time measurer which is configured to acquire a remaining time before the calibration process is ended; and
 a display controller which is configured to cause an index indicating the remaining time to be displayed on the display.

2. The biological information monitoring apparatus according to claim 1, wherein the index is at least one of a numeral and a progress bar.
3. The biological information monitoring apparatus according to claim 1, wherein, based on the predetermined condition, the time measurer selects one of a plurality of predetermined values which indicate times required for the calibration process, respectively, and, based on the selected one of the plurality of predetermined values, acquires the remaining time.
4. The biological information monitoring apparatus according to claim 1, wherein, based on information indicating a relationship between the predetermined condition and a time required for the calibration process, the time measurer calculates or acquires the remaining time.
5. The biological information monitoring apparatus according to claim 1, wherein the biological information includes at least one of a concentration of a predetermined gas contained in an expired gas of the subject, a concentration of an anesthetic agent contained in an expired gas of the subject, a respiratory volume, and an airway pressure.
6. The biological information monitoring apparatus according to claim 1, wherein the biological information includes at least two or more of an electrocardiogram, a pulse wave, and a blood pressure, and the measurer includes a calculator which is configured to calculate a cardiac output of the subject, based on the at least two or more biological information.
7. The biological information monitoring apparatus according to claim 1, wherein the predetermined condition relates to at least one of an elapsed time from a previous calibration process, an elapsed time from activation of the biological information monitoring apparatus, a current time, a temperature in the biological information monitoring apparatus, an atmospheric pressure, an input of an instruction by an operator, and stabilization of a signal relating to the biological information.

FIG. 1

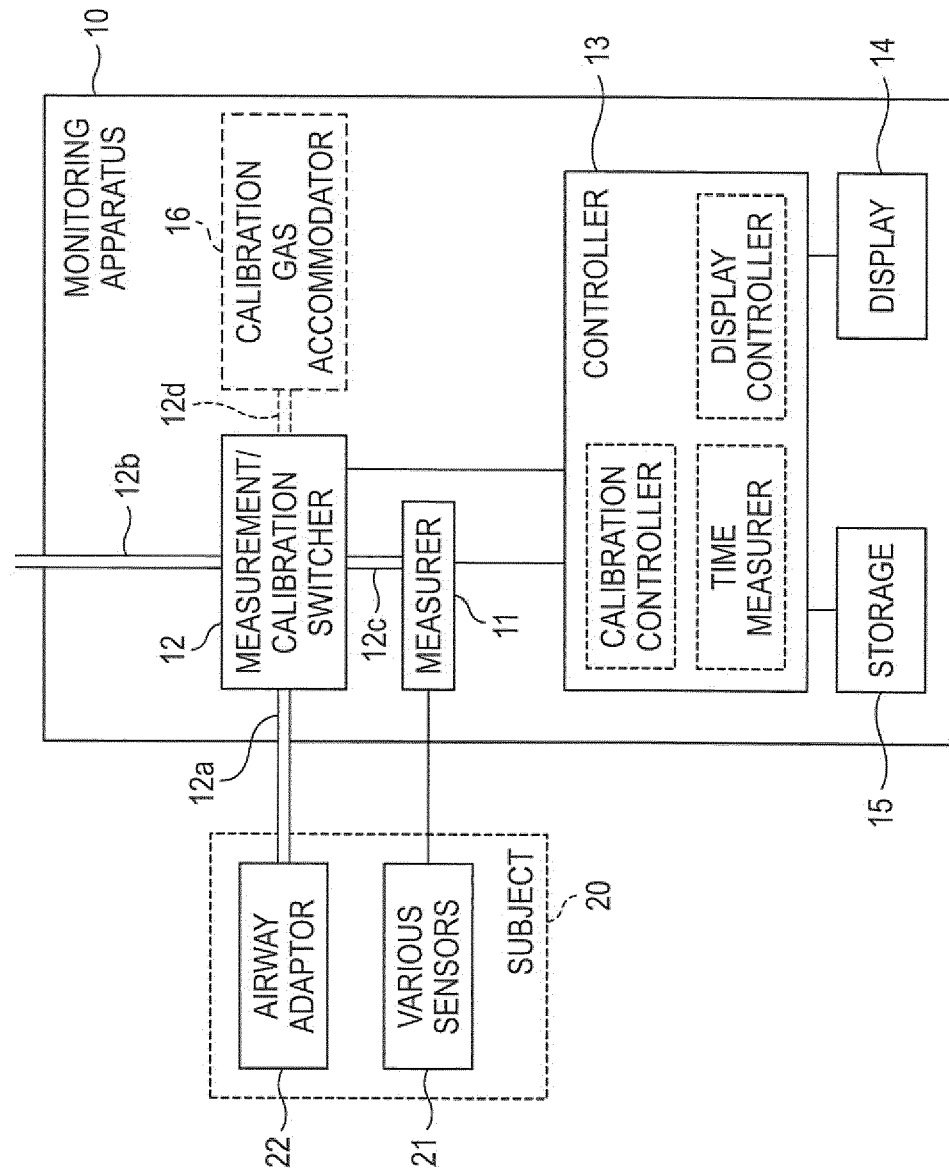


FIG. 2

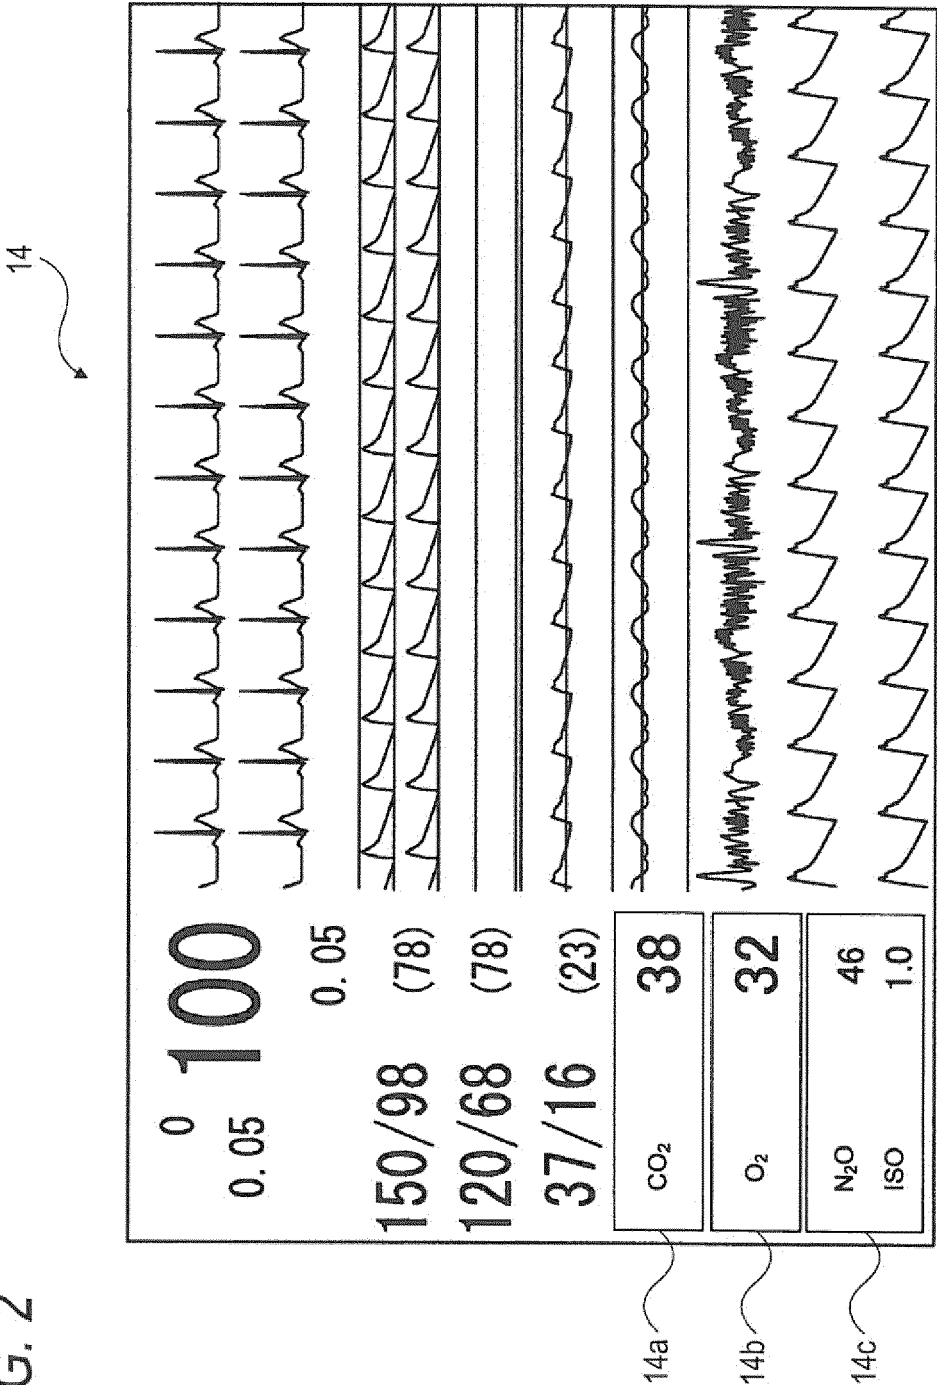


FIG. 3

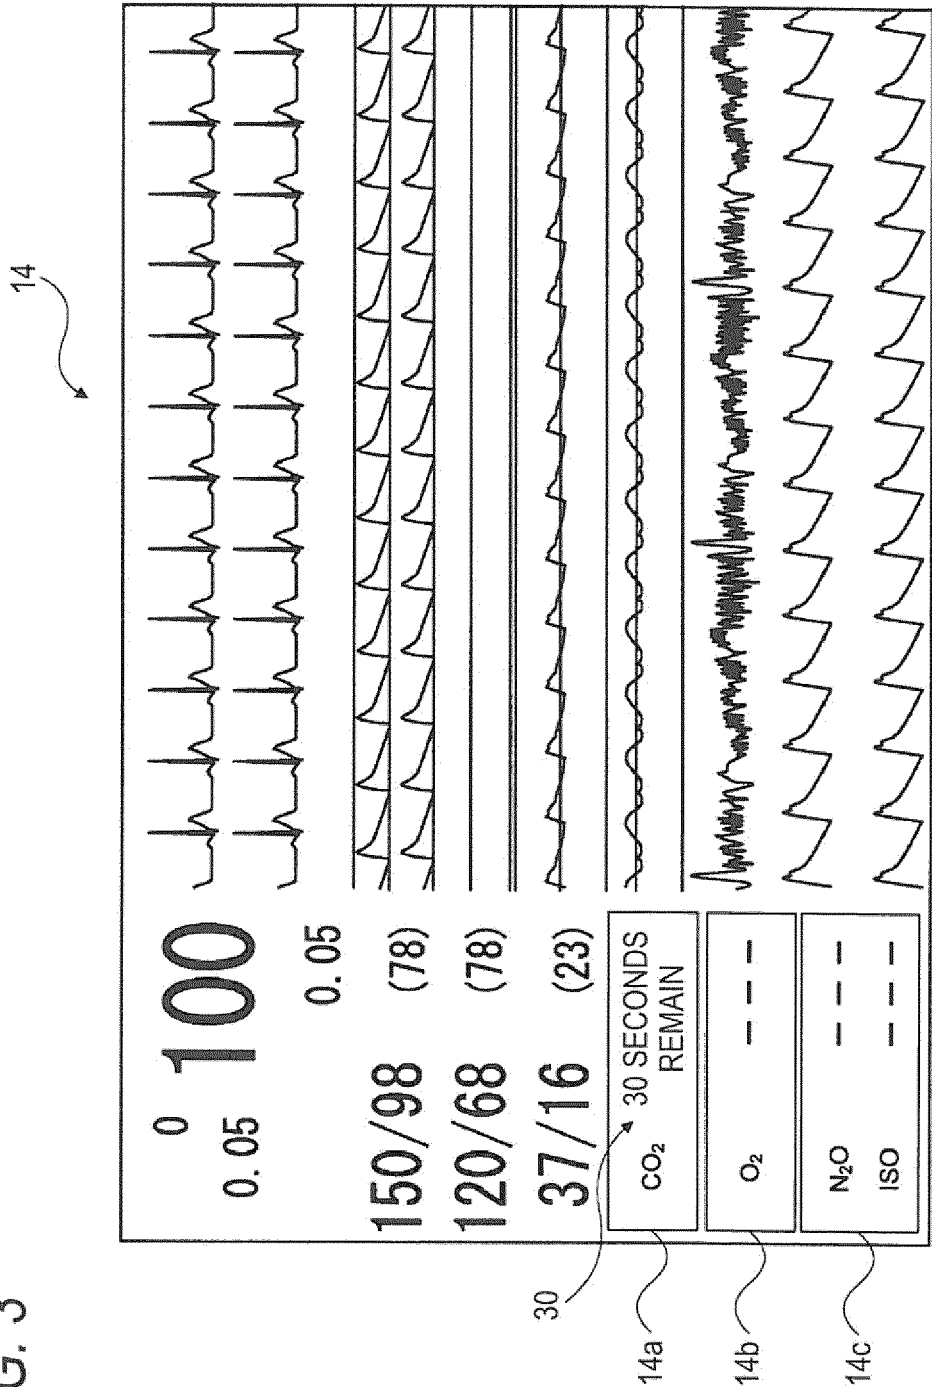


FIG. 4

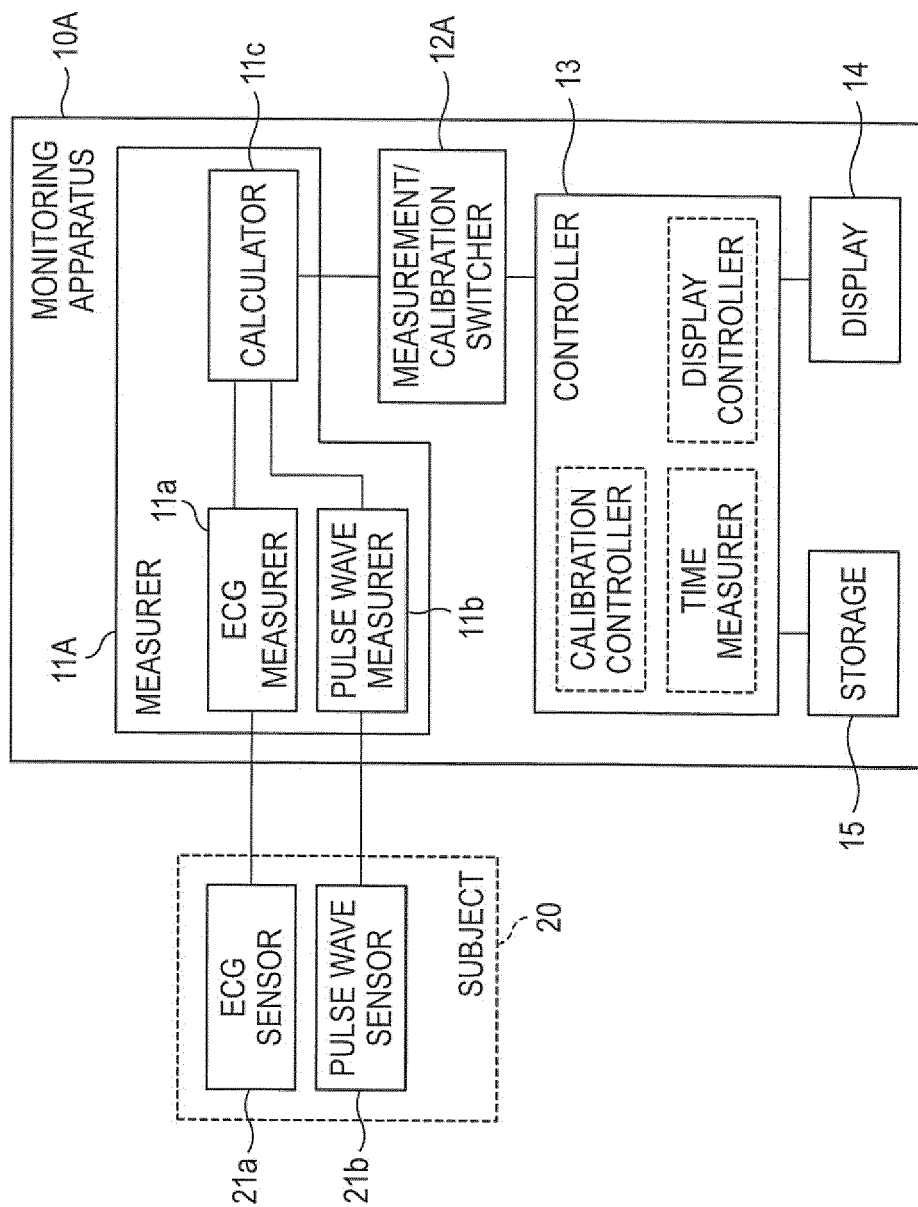


FIG. 5


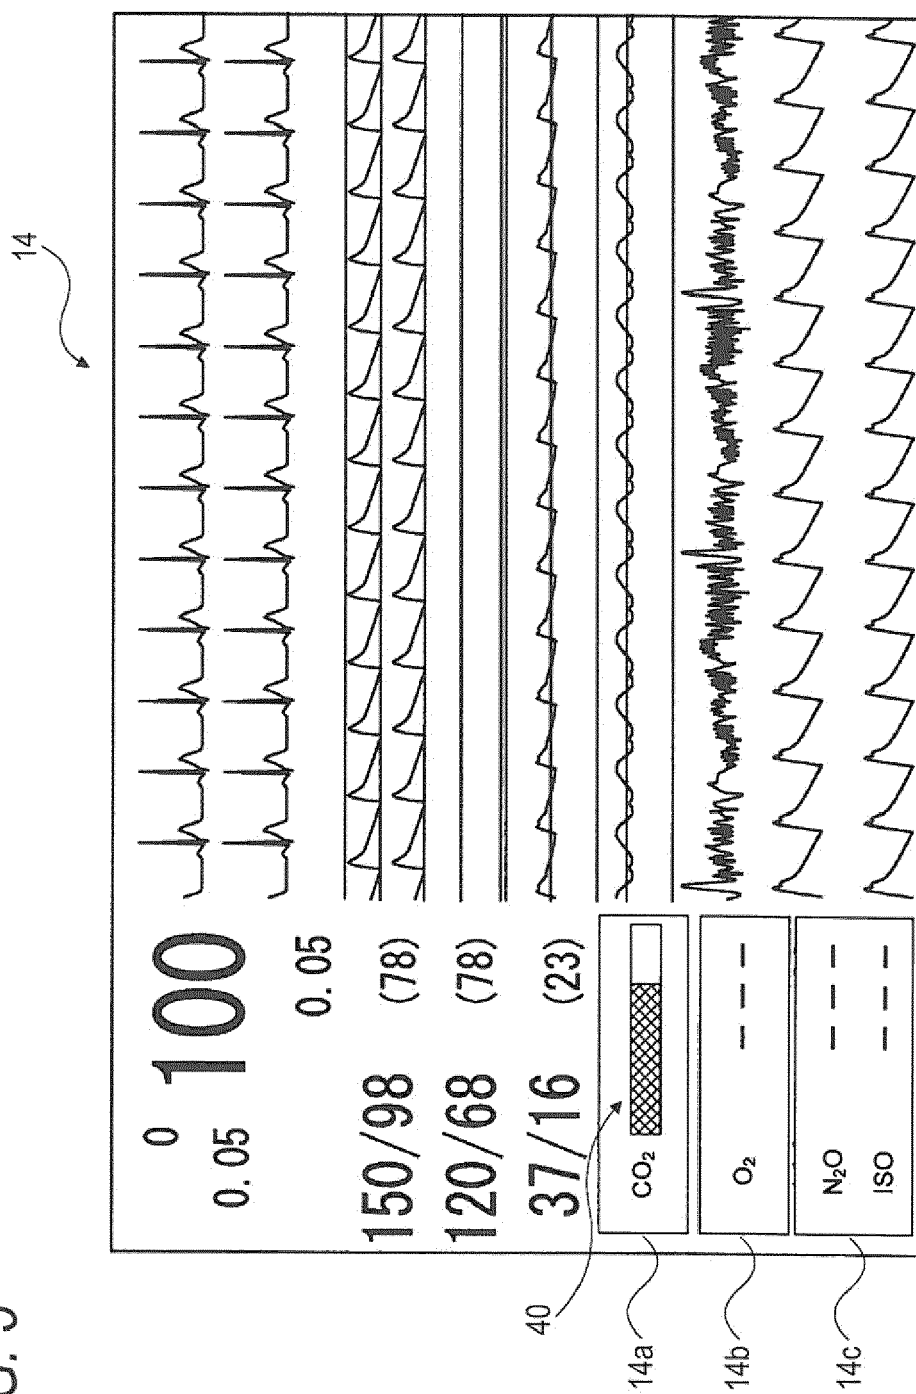


FIG. 6



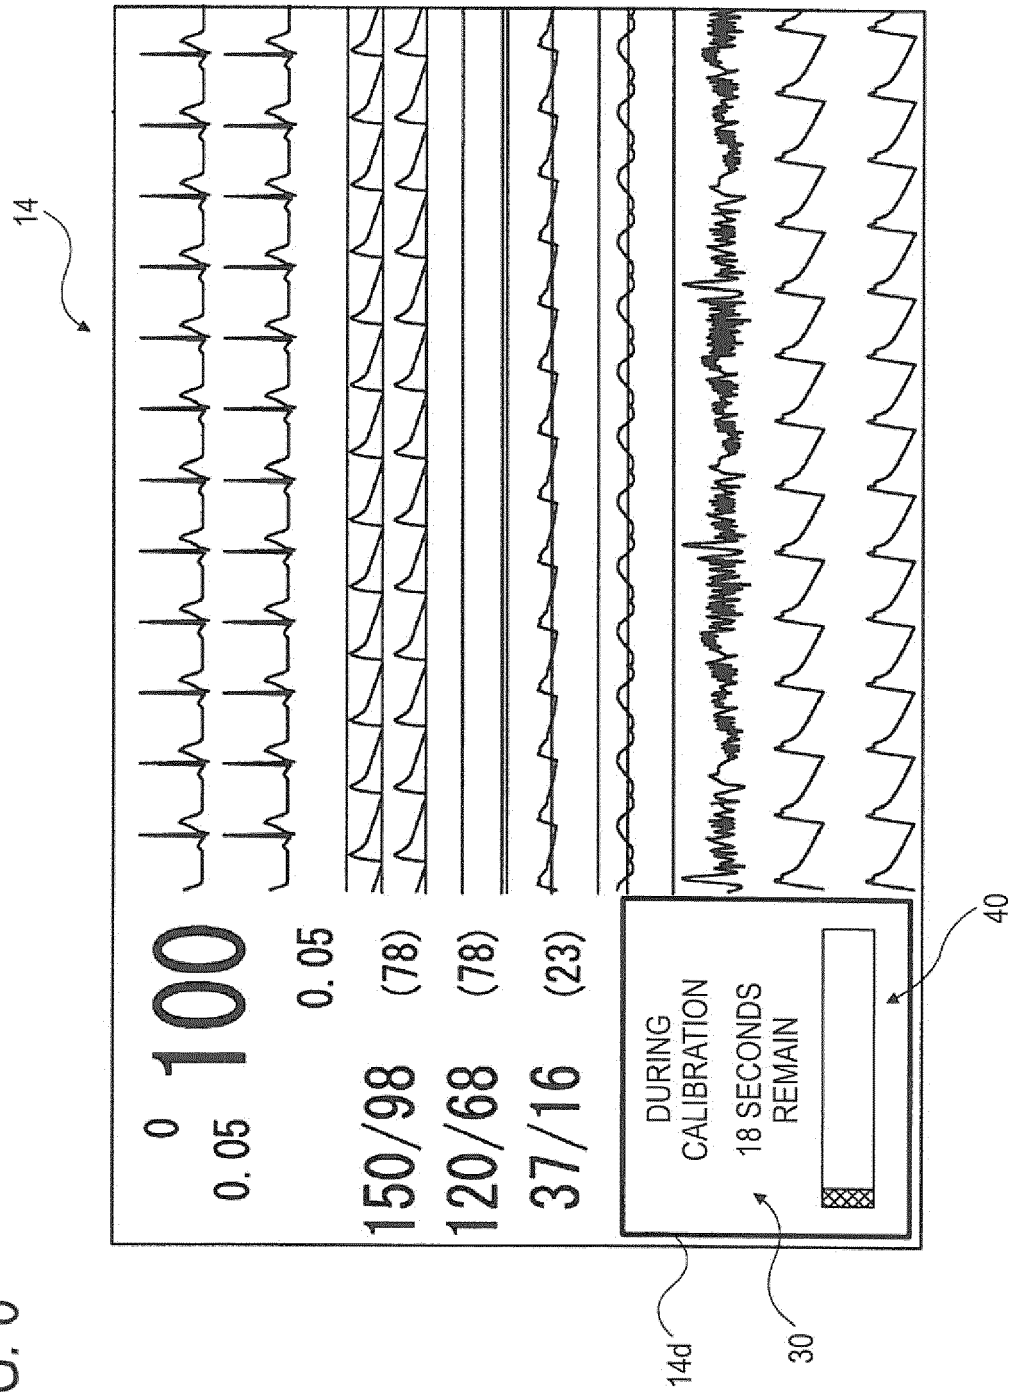

EUROPEAN SEARCH REPORT

Application Number
EP 13 16 3712

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2009/326335 A1 (BAKER CLARK R [US] ET AL) 31 December 2009 (2009-12-31)	1-4,7	INV. A61B5/00 G06F19/00 A61B5/1495 ADD. A61B10/00
Y	* paragraphs [0014], [0015], [0018], [0019] * * paragraph [0022] - paragraph [0024] * * figures 1-3 *	5,6	
Y	US 2007/034792 A1 (ZHANG WEI [CN] ET AL) 15 February 2007 (2007-02-15) * paragraph [0028] *	5	
Y	CN 101 176 663 B (UNIV SHANDONG [CN] UNIV SHANDONG) 27 October 2010 (2010-10-27) * paragraphs [0006], [0010] *	6	
A	US 5 899 855 A (BROWN STEPHEN JAMES [US]) 4 May 1999 (1999-05-04) * the whole document *	1-7	
A	WO 2011/026053 A1 (ABBOTT DIABETES CARE INC [US]; HARPER WESLEY SCOTT [US]; TAN ANNIE C []) 3 March 2011 (2011-03-03) * the whole document *	1-7	
The present search report has been drawn up for all claims			TECHNICAL FIELDS SEARCHED (IPC)
			A61B G06F G01N G01D
2	Place of search The Hague	Date of completion of the search 19 July 2013	Examiner Meyer, Wolfgang
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 13 16 3712

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

19-07-2013

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2009326335 A1	31-12-2009	NONE	
US 2007034792 A1	15-02-2007	CN 1912585 A	14-02-2007
		US 2007034792 A1	15-02-2007
CN 101176663 B	27-10-2010	NONE	
US 5899855 A	04-05-1999	NONE	
WO 2011026053 A1	03-03-2011	EP 2473422 A1	11-07-2012
		US 2011193704 A1	11-08-2011
		WO 2011026053 A1	03-03-2011

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2010508523 T [0003]
- JP 2000245711 A [0003]
- JP 4742644 B [0036]
- JP 2010246801 A [0037]

专利名称(译)	生物信息监测装置		
公开(公告)号	EP2653097A1	公开(公告)日	2013-10-23
申请号	EP2013163712	申请日	2013-04-15
[标]申请(专利权)人(译)	日本光电工业株式会社		
申请(专利权)人(译)	日本光电公司		
当前申请(专利权)人(译)	日本光电公司		
[标]发明人	HOSAKA SHOICHI AOKI TOSHIKI MAEDA SHOGO UCHIDA OSAMU		
发明人	HOSAKA, SHOICHI AOKI, TOSHIKI MAEDA, SHOGO UCHIDA, OSAMU		
IPC分类号	A61B5/00 G06F19/00 A61B5/1495 A61B10/00		
CPC分类号	A61B5/72 A61B5/082 A61B5/091 A61B5/1495 A61B5/742 A61B2010/0087 A61B2505/05 G01N33/48 G16H40/40		
审查员(译)	MEYER , WOLFGANG		
优先权	2012092790 2012-04-16 JP		
外部链接	Espacenet		

摘要(译)

一种生物信息监测装置，包括：测量器，被配置为测量对象的生物信息；显示由测量者测量的生物信息的测量值的显示器；校准控制器，当满足预定条件时，被配置为对测量器执行校准处理；时间测量器，用于获取校准过程结束前的剩余时间；显示控制器，用于使指示剩余时间的索引显示在显示器上。

FIG. 1

