



(11) **EP 3 071 303 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:

**01.08.2018 Bulletin 2018/31**

(21) Application number: **14864289.5**

(22) Date of filing: **28.10.2014**

(51) Int Cl.:

**A63B 23/04** <sup>(2006.01)</sup> **A63B 22/04** <sup>(2006.01)</sup>  
**A61B 5/11** <sup>(2006.01)</sup> **A61B 5/00** <sup>(2006.01)</sup>  
**A63B 69/00** <sup>(2006.01)</sup> **A63B 21/068** <sup>(2006.01)</sup>  
**A63B 24/00** <sup>(2006.01)</sup> **A63B 71/06** <sup>(2006.01)</sup>  
**A63B 21/00** <sup>(2006.01)</sup>

(86) International application number:  
**PCT/IB2014/065659**

(87) International publication number:  
**WO 2015/075583 (28.05.2015 Gazette 2015/21)**

(54) **COMPUTER-AIDED PHYSIOTHERAPEUTIC STAIR AND GAIT SYSTEM**

COMPUTERGESTÜTZTE PHYSIOTHERAPEUTISCHE TREPPE UND GANGSYSTEM

SYSTÈME D'ESCALIER ET DE DÉMARCHE PHYSIOTHÉRAPEUTIQUE ASSISTÉ PAR ORDINATEUR

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

(30) Priority: **20.11.2013 US 201314084639**

(43) Date of publication of application:  
**28.09.2016 Bulletin 2016/39**

(73) Proprietor: **DPE Medical Ltd.**  
**9085500 Shoeva (IL)**

(72) Inventor: **ORGAL, Daniel**  
**9085500 Shoeva (IL)**

(74) Representative: **Kancelaria Eupatent.pl Sp. z.o.o**  
**Ul. Kilinskiego 185**  
**90-348 Lodz (PL)**

(56) References cited:  
**WO-A1-2012/057595 JP-A- H11 181 983**  
**US-A- 5 769 759 US-A- 5 901 813**  
**US-A1- 2010 099 541 US-A1- 2010 099 541**  
**US-A1- 2012 238 409 US-A1- 2012 264 572**

**EP 3 071 303 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description**FIELD AND BACKGROUND OF THE INVENTION

**[0001]** The present invention relates to physiotherapy devices and, in particular, it concerns a physiotherapeutic stair system in which treatment is enhanced and/or documented by use of a computer system associated with an integrated sensor set.

**[0002]** Many patients require physiological rehabilitation for various reasons. These include, for example, victims of traffic accidents, patients who have suffered from a cardiac episode or underwent a cardiac medical procedure, as well as individuals that have had a cerebral episode, invasive medical procedures, or sustained injuries of violence and the like. These patients need to receive physiotherapeutic treatment in rehabilitation wards of various institutions or by professional physiotherapists, for the purpose of a gradual return to regular life.

**[0003]** The practicing of walking, ascending and descending stairs is a central part of the rehabilitation process. The ability to ascend and descend stairs is a vital component in the assessment process performed by the medical staff when deciding whether a patient can be discharged from the rehabilitative institution to his or her home.

**[0004]** One example of a suitable device for practicing ascending and descending of stairs is described in US patent number 5,901,813, and is commercially available from DPE Medical Ltd. (Israel) under the name Dynamic Stair Trainer (DST). The device consists of number of stairs whose height can be altered simultaneously according to the need and ability of the current patients.

**[0005]** Other step trainer examples with adjustable rise height are disclosed in documents US 5 769 759, WO 2012/057595 and US 2010/099541. Stair trainers used in physiotherapy for ascending and descending stairs are preferably static during use with a uniform pitch, simulating the look and feel of conventional stairs. It is also preferable that adjustment of the height occurs through a purely vertical motion without changing the depth of the tread surface of each step, and that the steps have closed riser surfaces without overlap between steps to minimize risk of tripping.

**[0006]** Existing step trainers of this type do not provide integrated tools to facilitate analysis and assessment of progress in stair-mobility treatment.

**[0007]** There is therefore a need for a physiotherapeutic stair system in which treatment would be enhanced and/or documented by use of a computer system associated with an integrated sensor set.

SUMMARY OF THE INVENTION

**[0008]** The present invention is a physiotherapeutic stair system in which treatment is enhanced and/or documented by use of a computer system associated with

an integrated sensor set.

**[0009]** According to the teachings of an embodiment of the present invention there is provided, a system comprising: (a) a set of at least three horizontal tread surfaces; (b) a drive system mechanically linked to the set of tread surfaces and configured to displace at least two of the tread surfaces vertically so as to adjust a rise height between adjacent of the tread surfaces in such a manner as to form a set of stairs with uniform pitch for a range of different rise heights; (c) a sensor set comprising at least one sensor deployed for measuring a parameter related to physiotherapy performed using the set of stairs; and (d) a computer system comprising at least one processor and a non-volatile data storage medium, the computer system being associated with the sensor set so as to receive the at least one parameter, wherein the at least one sensor comprises a sensor deployed to measure a parameter indicative of a current rise height between adjacent of the tread surfaces, characterized in that each of the displaceable tread surfaces has an adjacent riser surface so as to form a closed set of stairs at any position within the range of different rise heights, and wherein said at least one sensor comprises a plurality of load cells deployed to measure a load applied to said tread surfaces, and wherein said computer system is configured to process signals from said load cells to determine a time period taken by a patient to move from one of said tread surfaces to another of said tread surfaces. According to a further feature of an embodiment of the present invention, the computer system comprises a user interface configured to receive an input indicative of the identity of a patient undergoing treatment, and wherein the computer system stores records of a plurality of treatment sessions for each patient, the records including the current rise height.

**[0010]** According to a further feature of an embodiment of the present invention, the computer system is configured to generate a stair-capability measure for the patient, the stair-capability measure being indicative of a current ability of the patient to climb stairs and a rate of improvement of the current ability.

**[0011]** According to a further feature of an embodiment of the present invention, the at least one sensor comprises at least one heart rate sensor deployed to measure a parameter indicative of a heart rate of a patient on the set of stairs.

**[0012]** According to a further feature of an embodiment of the present invention, the system further comprises a handrail extending along at least one side of the set of stairs, and wherein the at least one heart rate sensor is integrated into the handrail.

**[0013]** According to a further feature of an embodiment of the present invention, the system further comprises a handrail extending along at least one side of the set of stairs, and wherein the at least one sensor comprises at least one contact sensor deployed to generate an output indicative of a location at which a patient using the set of stairs is holding the handrail.

**[0014]** According to a further feature of an embodiment of the present invention, the computer system is configured to: (a) monitor a sum of the loads measured by said plurality of load cells; (b) determine a current weight of a patient on said set of stairs; (c) subtract a current sum of said loads from said current weight to determine a current patient load on said handrail; and (d) generate a warning signal if said current patient load on the handrail exceeds a predefined percentage of said current weight of the patient. According to a further feature of an embodiment of the present invention, the computer system is configured to process signals from the load cells to determine at least one measure of gross motor skill control during stair usage.

**[0015]** According to a further feature of an embodiment of the present invention, the plurality of load cells is implemented as at least two load cells per tread surface being deployed so as to generate signals allowing determination of a loading position relative to a length of each of the tread surfaces.

**[0016]** According to a further feature of an embodiment of the present invention, the computer system is configured to determine, for each stair transition by a patient, whether the patient has lead with a right leg or a left leg, and to generate an indication of bilateral or unilateral usage.

**[0017]** According to a further feature of an embodiment of the present invention, the at least one load cell is implemented as a set of load cells deployed so as to generate signals allowing determination of a loading position in two dimensions for each of the tread surfaces.

**[0018]** According to a further feature of an embodiment of the present invention, the computer system is configured to generate a warning signal when loading of a tread surface satisfies conditions identifying excess front-edge loading of the tread surface.

**[0019]** According to a further feature of an embodiment of the present invention, the computer system is functionally interconnected with the drive system, the computer system being configured to retrieve from the data storage medium or from remote data storage data relating to at least one past treatment session for a given patient, the computer system being configured to actuate the drive system to bring the set of stairs to an initial rise height for a next treatment session, the initial rise height being derived at least in part from the data.

**[0020]** According to an example, the drive system is configured to displace the tread surfaces so as to form the set of stairs with a plurality of rise heights substantially spanning a majority of a range from 0 cm to 18 cm.

**[0021]** According to a further example, the drive system is further configured to displace the tread surfaces so that all of the plurality of tread surfaces are juxtaposed as a continuous flat surface.

**[0022]** According to a further example, the drive system is configured to displace the tread surfaces in a purely vertical motion, and wherein a plurality of the tread surfaces each has an associated vertical riser surface.

**[0023]** According to a further example, the computer system further comprises communication components for connection to a wired or wireless network, and wherein the computer system is configured to transfer via the network a report containing data relating to treatment sessions of a patient.

**[0024]** The invention being entirely defined by the appended claims 1-13.

## 10 BRIEF DESCRIPTION OF THE DRAWINGS

**[0025]** The invention is herein described, by way of example only, with reference to the accompanying drawings, wherein:

FIG. 1 is an isometric view of a physiotherapeutic stair system, constructed and operative according to an embodiment of the present invention, showing the system deployed to an intermediate rise height; FIG. 2 is a block diagram of the physiotherapeutic stair system of FIG. 1;

FIGS. 3A and 3B are isometric views of the physiotherapeutic stair system of FIG. 1 showing the system deployed, respectively, to a maximum rise height and a zero rise height, useful for ambulatory therapy between parallel bars;

FIG. 4 is a rear isometric view of the physiotherapeutic stair system of FIG. 1 deployed to the maximum height, with rear covers removed to reveal components of a drive system;

FIG. 5 is an enlarged isometric view of a step unit from the physiotherapeutic stair system of FIG. 1;

FIG. 6 is a schematic isometric view of a section of a handrail from the physiotherapeutic stair system of FIG. 1, illustrating a preferred deployment of sensing elements;

FIGS. 7A and 7B are schematic graphs illustrating variation of a total load on the physiotherapeutic stair system of FIG. 1 with time under normal usage and in a case of excessive load applied to a handrail, respectively;

FIG. 8 is a schematic graph illustrating variation of a load on each successive tread surface during use of the physiotherapeutic stair system of FIG. 1;

FIGS. 9A and 9B are enlarged views of a region of the graph of FIG. 8 for cases of patients with normal stability and poor stability, respectively;

FIGS. 10A and 10B are schematic graphs similar to FIG. 8 but resolved into load applied to the left side and the right side of each tread surface, respectively, for a case of a patient leading repeatedly with the right foot;

FIGS. 11A and 11B are schematic graphs similar to FIGS. 10A and 10B, respectively, for a patient leading bilaterally; and

FIGS. 12A and 12B are schematic graphs illustrating a front-back loading balance for a given tread surface under conditions of normal usage and dangerous

foot positioning on the edge of a step, respectively.

#### DESCRIPTION OF THE PREFERRED EMBODIMENTS

**[0026]** The present invention is a physiotherapeutic stair system in which treatment is enhanced and/or documented by use of a computer system associated with an integrated sensor set, and corresponding methods for managing and/or assessing treatment using such a device.

**[0027]** The principles and operation of stair systems according to the present invention may be better understood with reference to the drawings and the accompanying description.

**[0028]** Referring now to the drawings, Figures 1-6 show various full or partial views of a physiotherapeutic stair training system, generally designated **10**, constructed and operative according to a particularly preferred embodiment of the present invention.

#### Mechanical Structure

**[0029]** The structural basis of system **10** according to this particularly preferred example closely parallels the implementation of the aforementioned Dynamic Stair Trainer (DST) commercially available from DPE Medical Ltd. (Israel). The device has a set **12** of at least three, and in the case shown here four, horizontal tread surfaces, individually referred to as **TR0**, **TR1**, **TR2** and **TR3**. A drive system **14** is mechanically linked to the set **12** of tread surfaces and configured to displace at least two of the tread surfaces **TR1-TR3** vertically so as to adjust a rise height between adjacent of the tread surfaces in such a manner as to form a set of stairs **12** with uniform pitch for a range of different rise heights.

**[0030]** A preferred but non-limiting implementation of drive system **14** is best seen in FIG. 4. Under each tread surface is a scissors mechanism **16**, preferably doubled so as to support each side of the tread surface, which allows vertical movement of the tread surface while ensuring that it remains parallel to the floor. A linear drive, shown here in the form of a screw actuator **18**, is deployed in a column **20** at the back of the top tread surface **TR3** and deployed to move tread surface **TR3** vertically. Other types of actuators, such as hydraulic or pneumatic actuators, may also be used. Two side rails **22** are pivotally linked to top tread surface **TR3** so as to be lifted at one end as the top tread surface rises. Each of the other tread surfaces has lateral projections **24** (see FIG. 5) which engage rails **22** as a track, thereby lifting each tread surface in proportion to the elevation of the top surface and maintaining a set of stairs **12** of uniform pitch.

**[0031]** Parenthetically, it will be noted that the drawings show the system of the present invention with various covers and a protective skirt removed to reveal various components of the mechanism.

**[0032]** It is important for stair therapy treatment that the steps are closed steps, i.e., with closed riser surfaces,

so that the toes of a patient do not get caught beneath the step. To this end, each tread surface (other than **TR0**) is generally integrally formed with a riser surface **26** to form a step structure. Drive system **14** is preferably configured to displace the tread surfaces in a purely vertical motion, such as through the aforementioned scissors mechanisms **16**.

**[0033]** In the particularly preferred case illustrated in FIG. 5, each step also includes a telescopic extension portion **28** which provides an extension to riser surface **26** in the higher raised positions of the system, such as is seen in FIG. 3A. The use of a telescopic extension portion allows the system to assume a fully lowered state (FIG. 3B) in which a spacing from the floor is less than the maximum rise height of the set of stairs **12** in the fully raised state.

**[0034]** The system preferably also includes at least one handrail extending alongside the set of stairs **12**. In the implementation illustrated here, an adjustable-height handrail **30** is provided on each side of the set of stairs **12**, and is complemented by a handrail portion **32** extending around the top tread surface, which is here extended to form an upper platform to facilitate turning around between the ascent and descent. The handrail may additionally or alternatively be adjustable in horizontal position, to allow adjustment of the spacing between the right and left rails.

**[0035]** Drive system **14** is preferably configured to displace the tread surfaces so as to form the set of stairs **12** with a plurality of rise heights substantially spanning a majority of a range from 0 cm to 18 cm. "Substantially spanning" in this context refers to adjustability which provides either continuous adjustment or a plurality of discrete positions which are spaced apart by no more than 2 cm, and more typically in steps of 1 cm or less. In a particularly preferred implementation, the system provides adjustment to substantially span the entirety of a range of at least 0-18 cm, thereby facilitating practice of all common step sizes.

**[0036]** The system preferably assumes a fully flattened (zero step) state, as illustrated in FIG. 3B. In this stage, the plurality of tread surfaces are juxtaposed as a continuous flat surface, which is useful for ambulatory parallel bars therapy.

**[0037]** In addition to the aforementioned components, the present invention features a computer system **34** comprising at least one processor **36** and a non-volatile data storage medium **38**, typically together with networking components **40** for connection to a wired or wireless network. Computer system **34** may be any type of suitable computer, including but not limited to, a general purpose computer running suitable software under a suitable operating system, and a dedicated computer system configured by suitable hardware, software and/or firmware to perform the various functions required. In some implementations, computer system **34** may be implemented using a mobile electronics device such as a smartphone operating suitable software and in wireless communica-

tion with the various other components of the system.

[0038] Computer system **34** is preferably associated with, and possibly integrated with, one or more user input device **42** and a display **44**. In one preferred case, the entire computer system **34** is integrated in a "tablet" configuration with a touch-screen which serves as both the input device and the display, as illustrated schematically in FIG. 1.

[0039] Control of the up/down motion of drive system **14** may be achieved by pressing directly on up/down buttons on a controller **46** associated with drive system **14**. Additionally, or alternatively, control of drive system **14** may be achieved via the user interface of computer system **34**.

[0040] Computer system **34** is associated with a sensor set **48** including at least one sensor deployed for measuring a parameter related to physiotherapy performed using the set of stairs **12**. Preferred examples of the sensors, and corresponding modes of operation of the system, are described below.

#### Sensor Set

[0041] Sensor set **48** may include a wide range of sensors for sensing a variety of parameters related to physiotherapy performed using the set of stairs **12**. These parameters may relate to the current state of the set of stairs themselves or to the manner in which a patient is using the set of stairs. Each of the sensors described below is of utility when used alone. Certain particularly preferred implementations include multiple types of sensor, and may combine the data from the various sensors to derive additional information. The particular sensors described herein are exemplary, and are not an exhaustive list.

[0042] In certain embodiments, the present invention provides a sensor **50** deployed to measure a parameter indicative of a current rise height between adjacent of the tread surfaces. Sensor **50** may take various forms, including but not limited to: a laser or other rangefinder deployed to measure a distance between the top platform **TR3** and the base of the system; an optical or magnetic encoder associated with the screw drive mechanism to count revolutions of the drive; and an angle encoder associated with a mechanical component of one of the scissors mechanisms. This output, after correction of any offset and dividing by the number of steps, provides a direct indication of the current pitch of the set of stairs **12**.

[0043] In certain embodiments, the present invention provides at least one heart rate sensor **52** deployed to measure a parameter indicative of a heart rate of a patient on the set of stairs **12**, before, during and/or after ascending or descending the stairs. According to one preferred implementation, the heart rate sensing is performed via electrodes located on handrails **30** and/or **32** using technology commonly available and implemented in hand grips of many treadmills and other aerobic exercise devices. This technology is well known, and will not be de-

scribed here in detail. In certain cases, electrodes for heart rate monitoring may be provided only at the positions corresponding to a bottom step grip and a top step grip, for detecting the heart rate prior to and after ascending or descending.

[0044] According to a further feature of certain preferred embodiments of the present invention, at least one contact sensor **54** is deployed to generate an output indicative of a location at which a patient using the set of stairs **12** is holding the handrail. The handrail grip position sensors are typically implemented as a series of capacitive or conductive sensors spaced along the handrail, allowing the supporting circuitry to determine where along the handrail the user is currently gripping, as illustrated schematically in FIG. 6. Particularly in the case of conductive sensors, the grip position sensors may advantageously be integrated with heart rate sensing via the same conductive electrodes.

[0045] According to a further feature of certain preferred embodiments of the present invention, at least one load cell **56** is deployed to measure a load applied to each of the tread surfaces. In the particularly preferred example of FIG. 5, the upper plate of each tread surface is supported by four load cells, one in each corner, which provides stability and allows detailed analysis of real-time weight distribution over the surface of the tread surface. Similar structures are known in the field of children's games, and are described in the literature such as, for example, in US Patent No. 8100770 to Yamazaki et al.

#### Operation

[0046] The various sensors of sensor set **48** in conjunction with computer system **34** provide a range of functionality for recording treatment sessions, enhancing and/or rendering safer the treatment itself, and analyzing patient progress, which were not heretofore available in the context of physiotherapeutic stair training or rehabilitation.

[0047] For example, the computer system preferably keeps track of patient treatment sessions, either in local data storage or via network access to a remote database, storing records of at least the patient identity as entered or selected via user input **42**, the dates of previous treatment sessions, and the maximum rise height achieved in each session. The rise height is preferably derived directly by the system from rise height sensor **50**, optionally additionally with input from the load cells **56** to verify that the patient successfully negotiated the stairs at that height. This data allows accurate evaluation of the patient's ability and rate of progress in managing stairs.

[0048] This data is preferably used as a basis for computer system **34** to generate a stair-capability measure for the patient, also referred to as a "Stair Factor of Progress" or SFP. The stair-capability measure is indicative of a current ability of the patient to climb stairs and a rate of improvement of the current ability. This may, for example, consist of a number corresponding to the high-

est rise height in centimeters which the patient is currently able to negotiate plus a letter indicating the rate of progress (corresponding to a range of gradients of a rise-height vs. date graph), such that for example "a" indicates rapid progress or full capability with the range of rise heights considered, "b" indicates a moderate rate of progress, and "c" indicates slow or negligible progress. Thus, for example, a SFP of (4-a) would indicate a current limitation to 4 cm steps, but a rapid rate of improvement whereas (8-c) would indicate a capability of managing 8 cm steps but with expectations that progress beyond that point is currently slow. This SFP will be a standardized parameter which is preferably generated automatically by system 10, and will greatly facilitate communication between medical staff regarding patient capabilities and progress. This stair-capability measure and/or other data relating to an individual therapy session or an entire sequence of treatment sessions can be forwarded to a medical professional or other authorized recipient by computer system 34 via a network.

[0049] An additional preferred feature of system 10 is the automatic adjustment of the set of stairs to the correct initial rise height for the beginning of a physiotherapy session. Specifically, computer system 34 is preferably configured to retrieve from data storage medium 38 or from remote data storage, data relating to at least one past treatment session for a given patient, the computer system being configured to actuate drive system 14 to bring the set of stairs 12 to an initial rise height for a next treatment session, the initial rise height being derived at least in part from the data relating to the past treatment. For example, therapy sessions may begin with steps of 5 cm smaller than the maximum rise height reached in the previous session, and will therefore automatically bring the steps to the appropriate height once a new therapy session for that user is selected.

[0050] Turning now to FIGS. 7A-12B, there are shown a range of applications which employ outputs from load cells 56. Although described primarily in the context of stair training, it will be appreciated that most of the functions described below are also applicable to gait therapy implemented when the system is at zero rise height, functioning as an ambulatory parallel-bars system.

[0051] Referring first to FIGS. 7A and 7B, it will be appreciated that by summing the loads applied to the tread surfaces at a given instant, it is possible to generate a measure of the total load applied to the set of stairs, and thus to determine a current weight of a patient on the set of stairs. FIGS. 7A and 7B illustrate variations of this total load with time during use of the system. It will be noted that the weight is not constant since it undergoes perturbations (due to slight vertical accelerations) as the patient's feet are moved from step to step and the body ascends or descends, as well as through weight transferred to the handrail. However, the variation of total load with time typically exhibits a clear modal value (i.e., the most frequently occurring value) which defines a baseline about which the perturbations occur. The modal value is

illustrated in FIG. 7A by a dashed line 60. This value can readily be picked out by computer system 34 via simple processing techniques, and is preferably then used to provide additional functionality.

5 [0052] By way of example, once the current weight of the patient has been determined, computer system 34 is preferably configured to subtract a current sum of the loads from this current weight to determine a current patient load on the handrail. Optionally, a safety limit can be set, for example at a predefined percentage (e.g., 15%) of the current weight, and computer system 34 may be configured to generate a warning signal, for example to an audible buzzer, if the current patient load on the handrail exceeds that predefined percentage of the current weight of the patient. In FIG. 7B, the warning level is represented by dashed line 62 and point 64 represents an incident in which the weight on the handrail has exceeded the allowed limit (shown here as a corresponding decrease in the total measured load), resulting in generation of an alarm.

20 [0053] Turning now to FIGS. 8, 9A and 9B, these illustrate separately the load measured on each tread surface, each curve being labeled with the corresponding tread surface label: TR0, TR1, TR2 and TR3. Analysis of these curves and the timing of transferring load between the tread surfaces provides significant information about the ability of the patient to negotiate stairs.

25 [0054] For example, referring to FIG. 8, computer system 34 is preferably configured to process signals from load cells 56 to determine a time period taken by a patient to climb the set of stairs, optionally calculated as a time-per-step or steps-per-minute rate. The time for negotiating each step transfer can be variously defined. In the illustration shown here, the foot-lift from the previous step is taken as the standard reference point from which step transfer duration is measured.

30 [0055] In addition to speed, the form of the load cell signal output can also be used to provide valuable information about the strength and stability of the patient's motion, indicative of their gross motor skill control during stair usage. Thus, in the enlarged views of FIGS. 9A and 9B, the smooth signals of FIG. 9A is indicative of well controlled continuous movements, whereas the unsteady signals of FIG. 9B are indicative of lack of muscle control and/or problems of instability during motion. Computer system 34 is preferably configured to process signals from load cells 56 to determine at least one measure of gross motor skill control during stair usage. In a simple implementation, this may be a measure of the "smoothness" of the signals, determined by the relative weights of low- and high-frequency components in a Fourier transform of the signal. Other forms of processing, such as identifying reversal of the direction of weight transfer between steps, may also provide valuable additional or alternative information.

35 [0056] The data represented by plots such as FIG. 8 may also be used to advantage with output of grip position sensors 54, identifying whether the grip position is within

a normal range of positions relative to the current center of gravity of the patient's weight on the tread surfaces. This allows the system to identify whether the patient is reaching ahead to drag himself or herself up to the next step, in contrast to a normal usage of the handrail just for stabilization.

**[0057]** It will be noted that the various functions described thus far can be implemented using a single load cell deployed to support each step. Particularly preferred implementations in which two, or more preferably four, load cells support each step allow for additional functionality, as will now be discussed.

**[0058]** FIGS. 10A-11B illustrate additional functionality which is available when the deployment of load cells allows determination of a loading position relative to a length of each of the tread surfaces, i.e., whether the load is central, to the right or to the left of the step. This can be achieved either by use of two load cells, one supporting each end of the step, or by use of four load cells, by summing the outputs of the right-hand and left-hand sides of each step.

**[0059]** FIGS. 10A and 10B illustrate plots of load on successive steps against time, similar to that of FIG. 8, but where the load on each step is resolved into separate measures of the load on the left side of the step (FIG. 10A) and the load on the right side of the step (FIG. 10B). The dashed line **60'** here corresponds to 50% of the current patient weight, which is the load that would be expected if the patient were to be standing on a single step with his or her weight evenly distributed along the length of the step between right and left.

**[0060]** Using this data, computer system **34** is preferably configured to determine, for each stair transition by a patient, whether the patient has lead with a right leg or a left leg, and to generate an indication of bilateral or unilateral usage. Thus, in the example of FIGS. 10A and 10B, the plot for load variation against time for each step shows an initial bias towards the right side, and a final bias prior to lifting of the foot towards the left side. This is indicative (during ascent) of the patient repeatedly leading with the right foot. During descent, when the patient is facing in the opposite direction, the polarity is reversed.

**[0061]** FIGS. 11A and 11B are a further example of a similar pair of plots, this time indicating initial and final bias on tread surface TR1 to the right side, and initial and final bias on tread surface TR2 to the left side. This is indicative of leading with alternate feet.

**[0062]** It will be noted that the average of right-left loading is not necessarily in the middle of the step, and that the modal value of loading for the plots of FIGS. 10A-11B will not necessarily lie on line **60'**. An offset from right-left balance is indicative of the patient holding his or her body closer to one handrail than the other. This information is also useful to record. The foot with which the user is leading can still readily be determined by the relative shifts of loading to the right and left, even where there is a consistent trend to one side.

**[0063]** Turning finally to FIGS. 12A and 12B, in the case of an arrangement of three or more non-colinear load cells supporting each tread surface, the set of load cells for each tread surface preferably generate signals allowing determination of a loading position in two dimensions for each of the tread surfaces. This allows assessment of the foot position relative to the front and back edges of the step, and particularly, allows identification of potentially dangerous scenarios in which a patient is transferring their load to a foot which is overlapping the front edge of a step. For this purpose, computer system **34** is preferably configured to generate a warning signal when loading of a tread surface satisfies conditions identifying excess front-edge loading of the tread surface. FIGS. 12A and 12B illustrate a position of the center of loading for a given step along the front-back direction as a function of time. FIG. 12A shows a normal variation. The weight may initially be biased momentarily towards the front of the step, for example as the patient's heel is planted on the step, and may move heavily to the rear of the step as the toe pushes off last. A transient frontal bias on the step is thus not considered problematic.

**[0064]** FIG. 12B illustrates a case in which the frontal bias of the weight remains above a threshold value for an extended period, indicative of a dangerously positioned foot. In this case, the system would preferably generate a warning, typically by sounding a buzzer or other audible alert. The invention is entirely defined by appended claims 1-13.

## Claims

1. A system (10) comprising:

- (a) a set (12) of at least three horizontal tread surfaces (TRO, TR1, TR2, TR3);
- (b) a drive system (14) mechanically linked to said set of tread surfaces and configured to displace at least two of said tread surfaces (TR1, TR2, TR3) vertically so as to adjust a rise height between adjacent of said tread surfaces in such a manner as to form a set of stairs with uniform pitch for a range of different rise heights;
- (c) a sensor set (48) comprising at least one sensor deployed for measuring a parameter related to physiotherapy performed using said set of stairs; and
- (d) a computer system (34) comprising at least one processor (36) and a non-volatile data storage medium (38), said computer system being in communication with said sensor set so as to receive said at least one parameter,

wherein said at least one sensor comprises a sensor (50) deployed to measure a parameter indicative of a current rise height between adjacent of said tread surfaces,

- characterized in that** each of the displaceable tread surfaces has an adjacent riser surface (26) so as to form a closed set of stairs at any position within the range of different rise heights,  
and wherein said at least one sensor comprises a plurality of load cells (56) deployed to measure a load applied to said tread surfaces, and wherein said computer system (34) is configured to process signals from said load cells (56) to determine a time period taken by a patient to move from one of said tread surfaces to another of said tread surfaces.
2. The system (10) of claim 1, wherein said computer system (34) comprises a user interface configured to receive an input indicative of the identity of a patient undergoing treatment, and wherein said computer system (34) stores records of a plurality of treatment sessions for each patient, said records including said current rise height.
  3. The system (10) of claim 2, wherein said computer system (34) is configured to generate a stair-capability measure for the patient, the stair-capability measure being indicative of a current ability of the patient to climb stairs and a rate of improvement of the current ability.
  4. The system (10) of claim 1, wherein said at least one sensor comprises at least one heart rate sensor (52) deployed to measure a parameter indicative of a heart rate of a patient on said set of stairs.
  5. The system (10) of claim 4, wherein the system further comprises a handrail extending along at least one side of said set of stairs, and wherein said at least one heart rate sensor (52) is integrated into said handrail (30).
  6. The system (10) of claim 1, wherein the system further comprises a handrail (30) extending along at least one side of said set of stairs, and wherein said at least one sensor comprises at least one contact sensor (54) deployed to generate an output indicative of a location at which a patient using said set of stairs is holding said handrail (30).
  7. The system (10) of claim 1, further comprising a handrail (30) extending along at least one side of said set of stairs, and wherein said computer system (34) is configured to:
    - (a) monitor a sum of the loads measured by said plurality of load cells (56);
    - (b) determine a current weight of a patient on said set of stairs (12);
    - (c) subtract a current sum of said loads from said current weight to determine a current patient load on said handrail; and
    - (d) generate a warning signal if said current patient load on said handrail exceeds a predefined percentage of said current weight of the patient.
8. The system (10) of claim 1, wherein said computer system (34) is configured to process signals from said load cells (56) to determine at least one measure of gross motor skill control during stair usage.
  9. The system (10) of claim 1, wherein said plurality of load cells (56) is implemented as at least two load cells per tread surface, said at least two load cells being deployed so as to generate signals allowing determination of a loading position relative to a length of each of said tread surfaces.
  10. The system (10) of claim 9, wherein said computer system (34) is configured to determine, for each stair transition by a patient, whether the patient has lead with a right leg or a left leg, and to generate an indication of bilateral or unilateral usage.
  11. The system (10) of claim 1, wherein said plurality of load cells (56) is implemented as a set of load cells deployed so as to generate signals allowing determination of a loading position in two dimensions for each of said tread surfaces.
  12. The system (10) of claim 11, wherein said computer system (34) is configured to generate a warning signal when loading of a tread surface satisfies conditions identifying excess front-edge loading of said tread surface.
  13. The system (10) of claim 1, wherein said computer system (34) is functionally interconnected with said drive system (14), said computer system being configured to retrieve from said data storage medium or from remote data storage data relating to at least one past treatment session for a given patient, said computer system (34) being configured to actuate said drive system to bring said set of stairs to an initial rise height for a next treatment session, said initial rise height being derived at least in part from said data.

#### Patentansprüche

1. System (10), umfassend:
  - (a) einen Satz (12) aus mindestens drei horizontalen Trittplächen (TRO, TR1, TR2, TR3);
  - (b) ein Antriebssystem (14), das mechanisch mit dem Satz Trittplächen verbunden und dazu ausgelegt ist, mindestens zwei der Trittplächen (TR1, TR2, TR3) vertikal zu verlagern, um eine Stufenhöhe zwischen benachbarten Trittplä-

chen derart einzustellen, dass ein Satz Treppenstufen mit einheitlicher Steigung für einen Bereich von unterschiedlichen Stufenhöhen gebildet wird;

(c) einen Sensorsatz (48), der mindestens einen Sensor umfasst, der zum Messen eines Parameters bezogen auf mithilfe des Satzes Treppenstufen durchgeführte Physiotherapie genutzt wird,

(d) ein Computersystem (34), das mindestens einen Prozessor (36) und ein nichtflüchtiges Datenspeichermedium (38) umfasst, wobei das Computersystem in Kommunikation mit dem Sensorsatz steht, um den mindestens einen Parameter zu empfangen,

wobei der mindestens eine Sensor einen Sensor (50) umfasst, der genutzt wird, um einen Parameter zu messen, der eine aktuelle Stufenhöhe zwischen benachbarten Trittplächen anzeigt,

**dadurch gekennzeichnet, dass** jede der verlagerbaren Trittplächen eine benachbarte Steigungsfläche (26) aufweist, um einen geschlossenen Satz Treppenstufen in einer beliebigen Position innerhalb des Bereichs von unterschiedlichen Stufenhöhen zu bilden,

und wobei der mindestens eine Sensor eine Mehrzahl von Kraftaufnehmern (56) umfasst, die genutzt werden, um eine Kraft zu messen, die auf die Trittplächen aufgebracht wird, und wobei das Computersystem (34) dazu ausgelegt ist, Signale von den Kraftaufnehmern (56) zu verarbeiten, um einen Zeitraum zu bestimmen, der von einem Patienten benötigt wird, um sich von einer der Trittplächen auf eine andere der Trittplächen zu bewegen.

2. System (10) nach Anspruch 1, wobei das Computersystem (34) eine Benutzerschnittstelle umfasst, die dazu ausgelegt ist, eine Eingabe zu empfangen, die die Identität eines Patienten anzeigt, der sich einer Behandlung unterzieht, und wobei das Computersystem (34) Berichte einer Mehrzahl von Behandlungssitzungen für jeden Patienten speichert, wobei die Berichte die aktuelle Stufenhöhe umfassen.
3. System (10) nach Anspruch 2, wobei das Computersystem (34) dazu ausgelegt ist, eine Treppensteigfähigkeitsmessung für den Patienten zu erzeugen, wobei die Treppensteigfähigkeit eine aktuelle Fähigkeit des Patienten, Treppen zu steigen, und eine Verbesserungsrate der aktuellen Fähigkeit anzeigt.
4. System (10) nach Anspruch 2, wobei der mindestens eine Sensor mindestens einen Herzfrequenzsensor (52) umfasst, der genutzt wird, um einen Parameter zu messen, der eine Herzfrequenz eines Patienten auf dem Satz Treppenstufen anzeigt.

5. System (10) nach Anspruch 4, wobei das System ferner einen Handlauf umfasst, der sich entlang mindestens einer Seite des Satzes Treppenstufen erstreckt, und wobei der mindestens eine Herzfrequenzsensor (52) in den Handlauf (30) integriert ist.
6. System (10) nach Anspruch 1, wobei das System ferner einen Handlauf (30) umfasst, der sich entlang mindestens einer Seite des Satzes Treppenstufen erstreckt, und wobei der mindestens eine Sensor mindestens einen Kontaktsensor (54) umfasst, der genutzt wird, um eine Ausgabe zu erzeugen, die eine Position anzeigt, in der ein Patient, der den Satz Treppenstufen nutzt, den Handlauf (30) hält.
7. System (10) nach Anspruch 1, wobei das System ferner einen Handlauf (30) umfasst, der sich entlang mindestens einer Seite des Satzes Treppenstufen erstreckt, und wobei das Computersystem (34) dazu ausgelegt ist:
  - (a) eine Summe der von der Mehrzahl Kraftaufnehmer (56) gemessenen Kräfte zu überwachen;
  - (b) ein aktuelles Gewicht eines Patienten auf dem Satz Treppenstufen (12) zu bestimmen;
  - (c) eine aktuelle Summe der Kräfte von dem aktuellen Gewicht zu subtrahieren, um eine aktuelle Patientenkraft auf dem Handlauf zu bestimmen; und
  - (d) ein Warnsignal zu erzeugen, wenn die aktuelle Patientenkraft auf dem Handlauf einen vordefinierten Prozentsatz des aktuellen Gewichts des Patienten übersteigt.
8. System (10) nach Anspruch 1, wobei das Computersystem (34) dazu ausgelegt ist, Signale von den Kraftaufnehmern (56) zu verarbeiten, um mindestens eine Messung der Grobmotorikkontrolle während der Treppenstufennutzung zu bestimmen.
9. System (10) nach Anspruch 1, wobei die Mehrzahl Kraftaufnehmer (56) als mindestens zwei Kraftaufnehmer pro Trittpläche implementiert ist, wobei die mindestens zwei Kraftaufnehmer genutzt werden, um Signale zu erzeugen, die die Bestimmung einer Belastungsposition bezogen auf eine Länge einer jeden der Trittplächen ermöglicht.
10. System (10) nach Anspruch 9, wobei das Computersystem (34) dazu ausgelegt ist, für jeden Stufenübergang durch einen Patienten zu bestimmen, ob der Patient mit dem rechten Bein oder dem linken Bein geführt hat, und einen Hinweis auf beidseitige oder einseitige Nutzung zu erzeugen.
11. System (10) nach Anspruch 1, wobei die Mehrzahl der Kraftaufnehmer (56) als ein Satz Kraftaufnehmer

implementiert ist, die genutzt werden, um Signale zu erzeugen, die eine Bestimmung einer Belastungsposition in zwei Dimensionen für jede der Trittflächen ermöglichen.

12. System (10) nach Anspruch 11, wobei das Computersystem (34) dazu ausgelegt ist, ein Warnsignal zu erzeugen, wenn das Belasten einer Trittfläche die Bedingungen erfüllt, die eine übermäßige Vorderkantenbelastung der Trittfläche identifizieren.
13. System (10) nach Anspruch 1, wobei das Computersystem (34) funktional mit dem Antriebssystem (14) zusammengeschaltet ist, wobei das Computersystem dazu ausgelegt ist, aus dem Datenspeichermedium oder aus einem entfernten Datenspeicher Daten bezogen auf mindestens eine frühere Behandlungssitzung für einen gegebenen Patienten abzufragen, wobei das Computersystem (34) dazu ausgelegt ist, das Antriebssystem zu betätigen, um den Satz Treppenstufen auf eine Anfangsstufenhöhe für eine nächste Behandlungssitzung zu bringen, wobei die Anfangsstufenhöhe zumindest teilweise aus den Daten abgeleitet wird.

#### Revendications

1. Système (10) comprenant :

(a) un ensemble (12) d'au moins trois surfaces de marche horizontales (TRO, TR1, TR2, TR3) ;  
 (b) un système d'entraînement (14) relié mécaniquement audit ensemble de surfaces de marche et configuré pour déplacer au moins deux desdites surfaces de marche (TR1, TR2, TR3) verticalement de façon à ajuster une hauteur d'élévation entre des surfaces adjacentes parmi lesdites surfaces de marche de manière à former un ensemble escalier ayant une pente uniforme pour une plage de hauteurs d'élévation différentes ;  
 (c) un ensemble (48) de capteurs, comprenant au moins un capteur déployé pour mesurer un paramètre associé à une physiothérapie réalisée à l'aide dudit ensemble escalier ; et  
 (d) un système informatique (34) comprenant au moins un processeur (36) et un support de stockage de données non volatil (38), ledit système informatique étant en communication avec ledit ensemble de capteurs de façon à recevoir ledit au moins un paramètre,

ledit au moins un capteur comprenant un capteur (50) déployé pour mesurer un paramètre indicateur d'une hauteur d'élévation courante entre des surfaces adjacentes parmi lesdites surfaces de marche, **caractérisé par le fait que** chacune des surfaces

de marche mobiles a une surface de contremarche adjacente (26) de façon à former un ensemble escalier fermé dans n'importe quelle position dans la plage de hauteurs d'élévation différentes, et ledit au moins un capteur comprenant une pluralité de cellules de mesure (56) déployées pour mesurer une charge appliquée auxdites surfaces de marche, et ledit système informatique (34) étant configuré pour traiter des signaux provenant desdites cellules de mesure (56) pour déterminer une durée prise par un patient pour se déplacer de l'une desdites surfaces de marche à une autre desdites surfaces de marche.

2. Système (10) selon la revendication 1, dans lequel ledit système informatique (34) comprend une interface utilisateur configurée pour recevoir une entrée indicatrice de l'identité d'un patient soumis au traitement, et ledit système informatique (34) stockant des enregistrements d'une pluralité de séances de traitement pour chaque patient, lesdits enregistrements comprenant ladite hauteur d'élévation courante.
3. Système (10) selon la revendication 2, dans lequel ledit système informatique (34) est configuré pour générer une mesure de capacité d'escalier pour le patient, la mesure de capacité d'escalier étant indicatrice d'une capacité courante du patient à monter un escalier et un taux d'amélioration de la capacité courante.
4. Système (10) selon la revendication 1, dans lequel ledit au moins un capteur comprend au moins un capteur de fréquence cardiaque (52) déployé pour mesurer un paramètre indicateur d'une fréquence cardiaque d'un patient sur ledit ensemble escalier.
5. Système (10) selon la revendication 4, dans lequel le système comprend en outre une rampe s'étendant le long d'au moins un côté dudit ensemble escalier, et ledit au moins un capteur de fréquence cardiaque (52) étant intégré dans ladite rampe (30).
6. Système (10) selon la revendication 1, dans lequel le système comprend en outre une rampe (30) s'étendant le long d'au moins un côté dudit ensemble d'escalier, et ledit au moins un capteur comprend au moins un capteur de contact (54) déployé pour générer une sortie indicatrice d'un emplacement au niveau duquel un patient utilisant ledit ensemble escalier tient ladite rampe (30).
7. Système (10) selon la revendication 1, comprenant en outre une rampe (30) s'étendant le long d'au moins un côté dudit ensemble escalier, et ledit système informatique (34) étant configuré pour :

(a) surveiller une somme des charges mesurées

- par ladite pluralité de cellules de mesure (56) ;  
 (b) déterminer un poids courant d'un patient sur ledit ensemble escalier (12) ;  
 (c) soustraire une somme courante desdites charges audit poids courant pour déterminer une charge de patient courante sur ladite rampe ; et  
 (d) générer un signal d'avertissement si ladite charge de patient courante sur ladite rampe dépasse un pourcentage prédéfini dudit poids courant du patient.
- 5  
10
8. Système (10) selon la revendication 1, dans lequel ledit système informatique (34) est configuré pour traiter des signaux provenant desdites cellules de mesure (56) pour déterminer au moins une mesure du contrôle de facultés motrices approximatif pendant l'utilisation de l'escalier.
- 15
9. Système (10) selon la revendication 1, dans lequel ladite pluralité de cellules de mesure (56) est mise en oeuvre de façon à avoir au moins deux cellules de mesure par surface de marche, lesdites au moins deux cellules de mesure étant déployées de façon à générer des signaux permettant la détermination d'une position de chargement par rapport à une longueur de chacune desdites surfaces de marche.
- 20  
25
10. Système (10) selon la revendication 9, dans lequel ledit système informatique (34) est configuré pour déterminer, pour chaque transition de marche par un patient, si le patient a avancé avec une jambe droite ou une jambe gauche, et générer une indication d'utilisation bilatérale ou unilatérale.
- 30  
35
11. Système (10) selon la revendication 1, dans lequel ladite pluralité de cellules de mesure (56) est mise en oeuvre sous la forme d'un ensemble de cellules de mesure déployées de façon à générer des signaux permettant la détermination d'une position de chargement en deux dimensions pour chacune desdites surfaces de marche.
- 40
12. Système (10) selon la revendication 11, dans lequel ledit système informatique (34) est configuré pour générer un signal d'avertissement lorsque le chargement d'une surface de marche satisfait à des conditions identifiant un chargement de bord avant excessif de ladite surface de marche.
- 45  
50
13. Système (10) selon la revendication 1, dans lequel ledit système informatique (34) est connecté de manière fonctionnelle audit système d'entraînement (14), ledit système informatique étant configuré pour récupérer, à partir dudit support de stockage de données ou d'une mémoire de données à distance, des données associées à au moins une séance de traitement passée pour un patient donné, ledit système
- 55
- informatique (34) étant configuré pour actionner ledit système d'entraînement pour amener ledit ensemble escalier à une hauteur d'élévation initiale pour une séance de traitement suivante, ladite hauteur d'élévation initiale étant déduite au moins en partie desdites données.

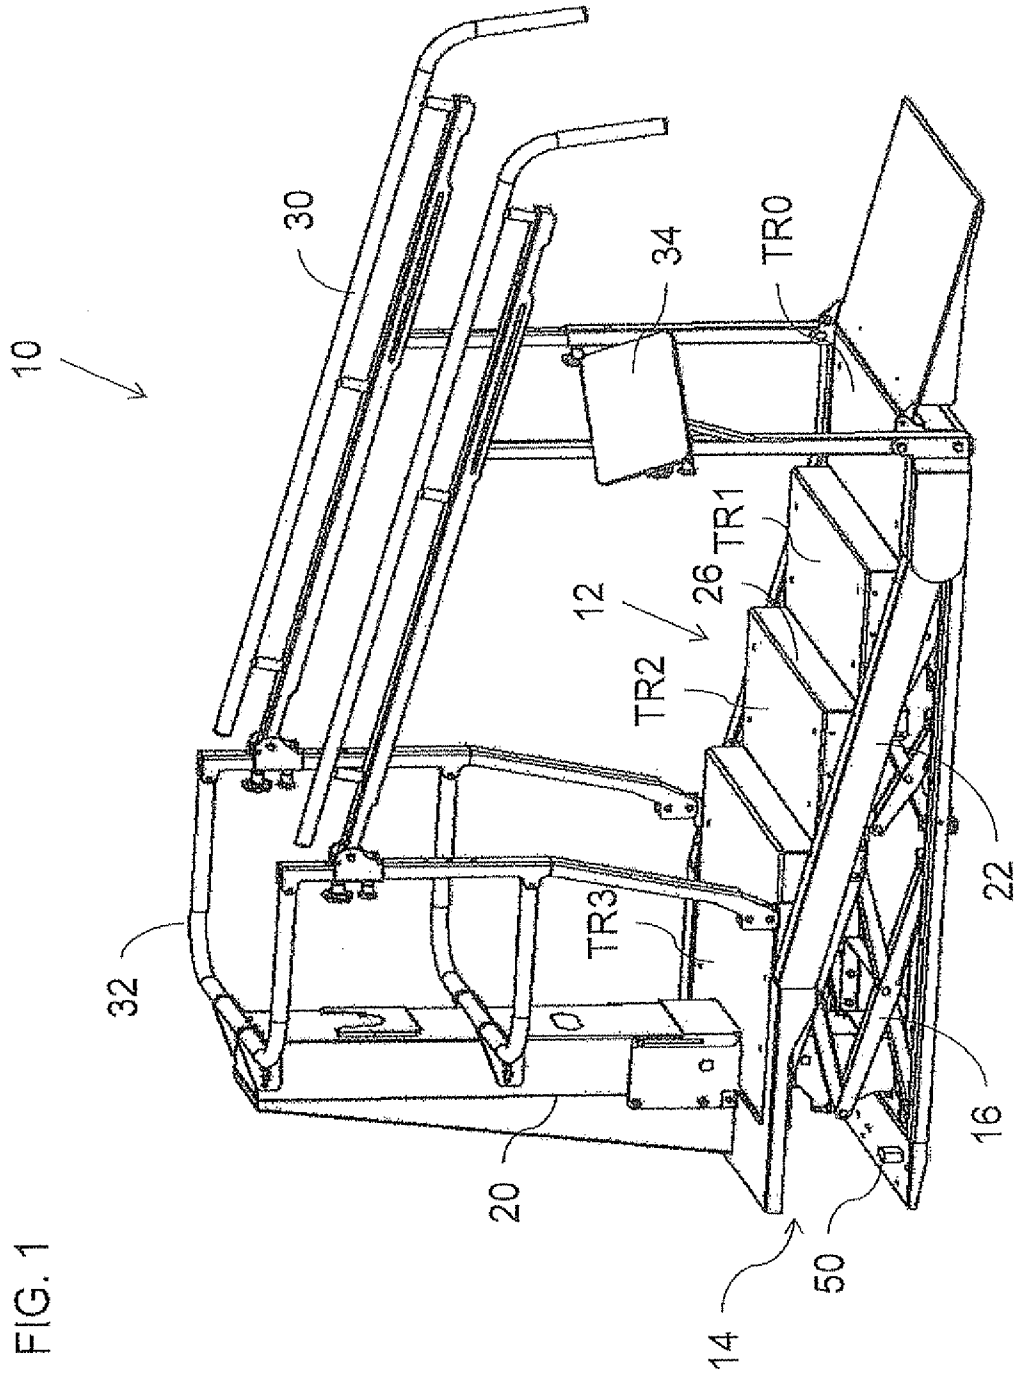
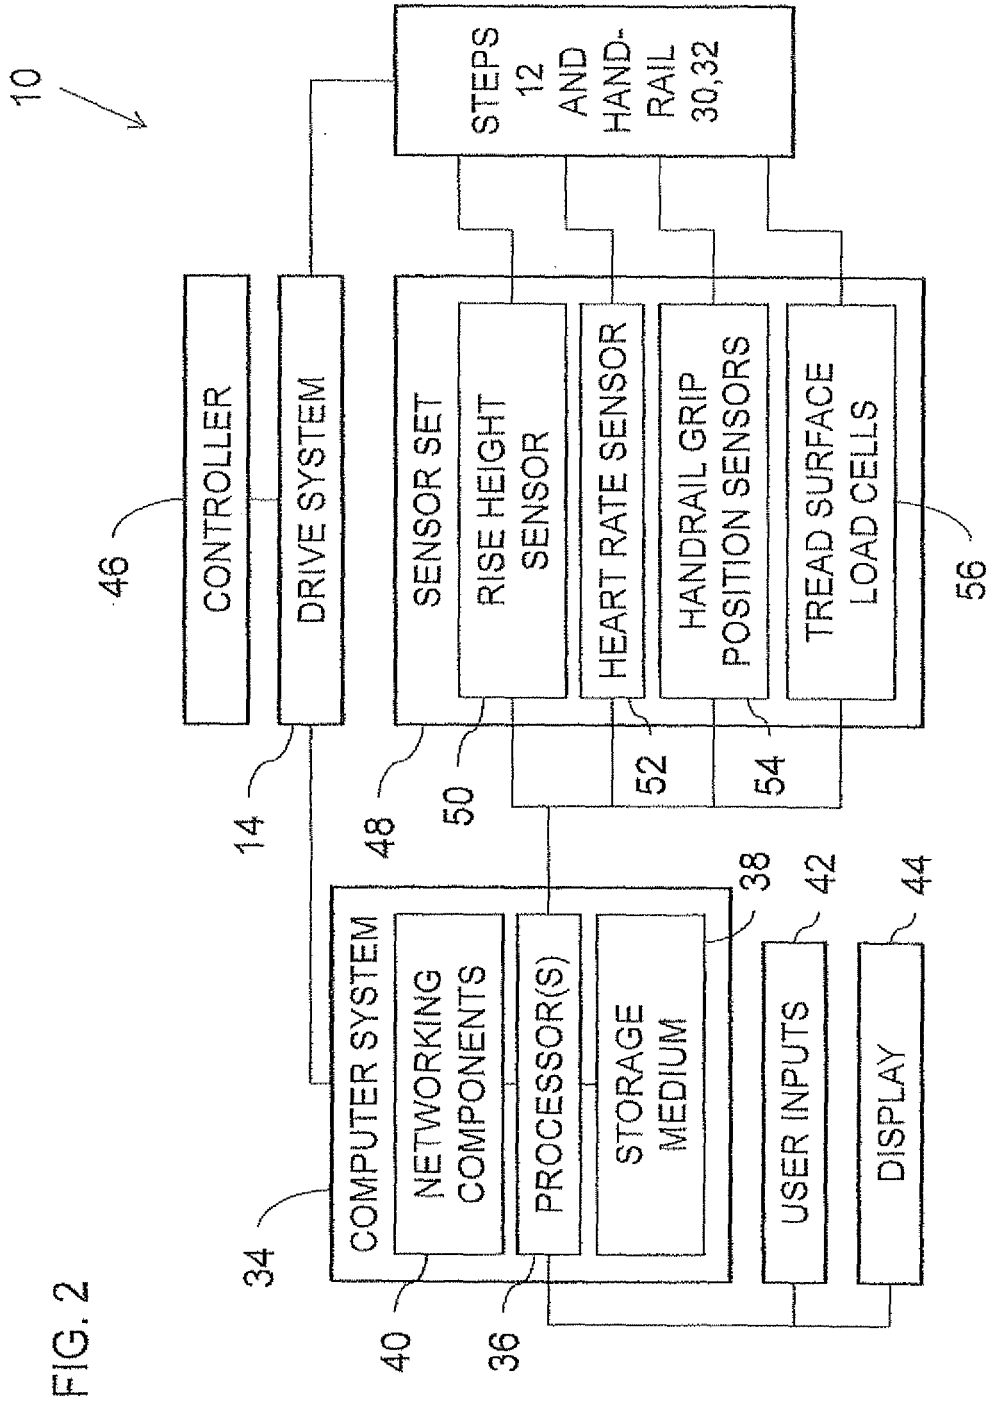
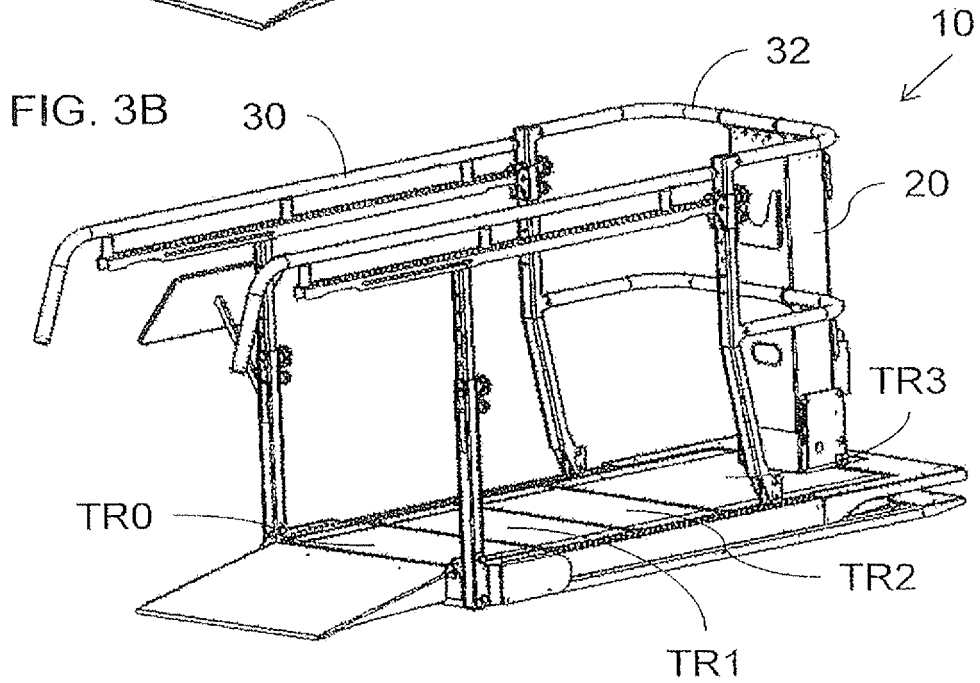
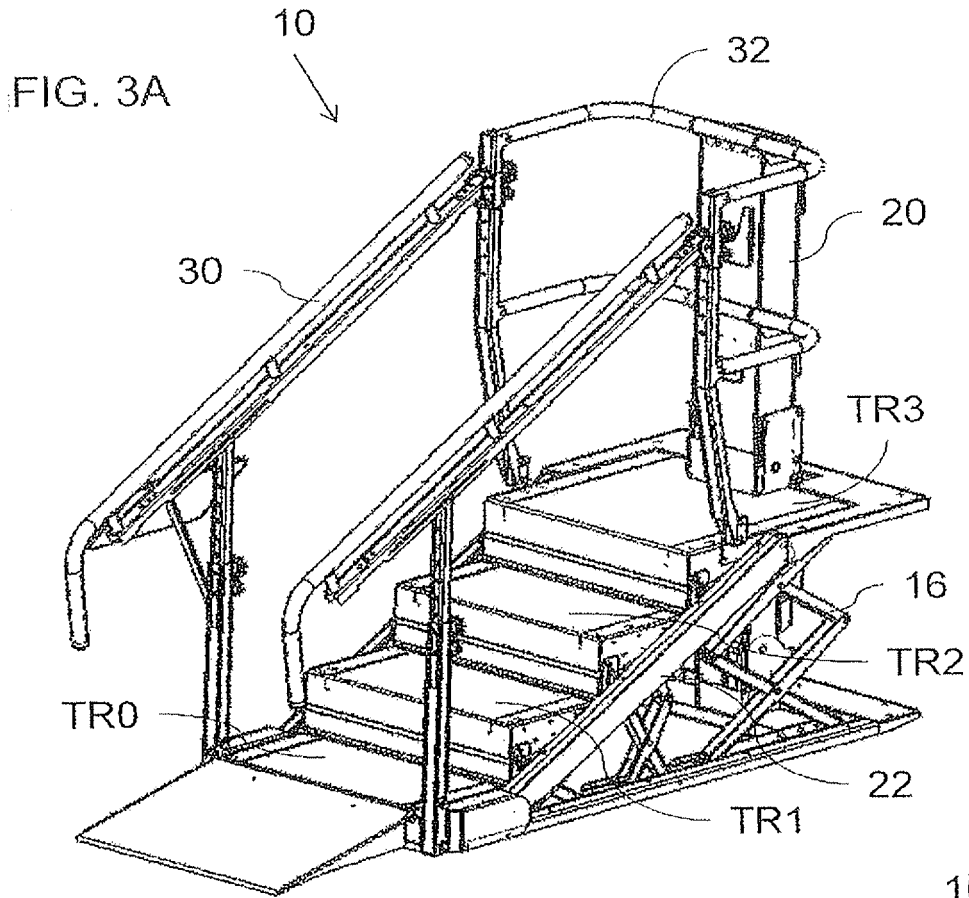


FIG. 1





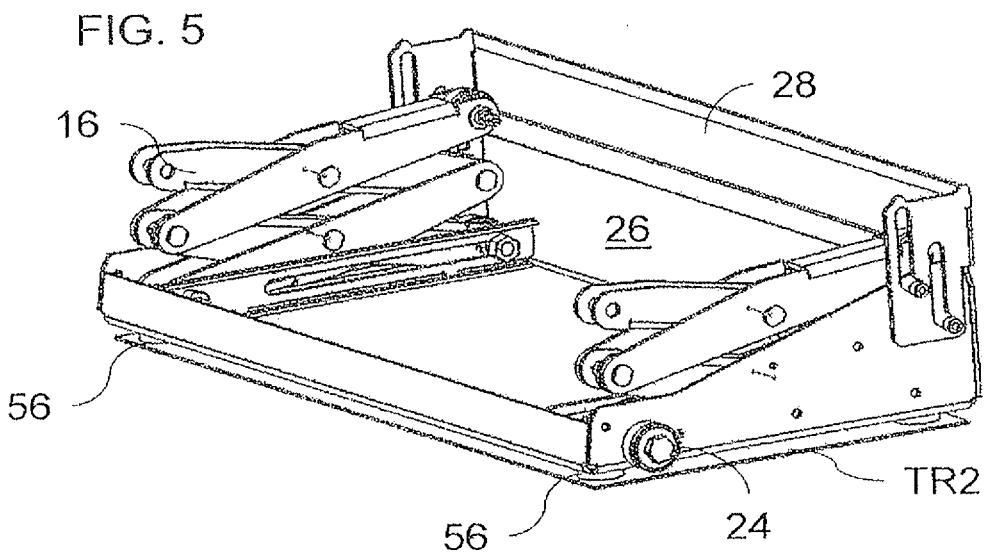
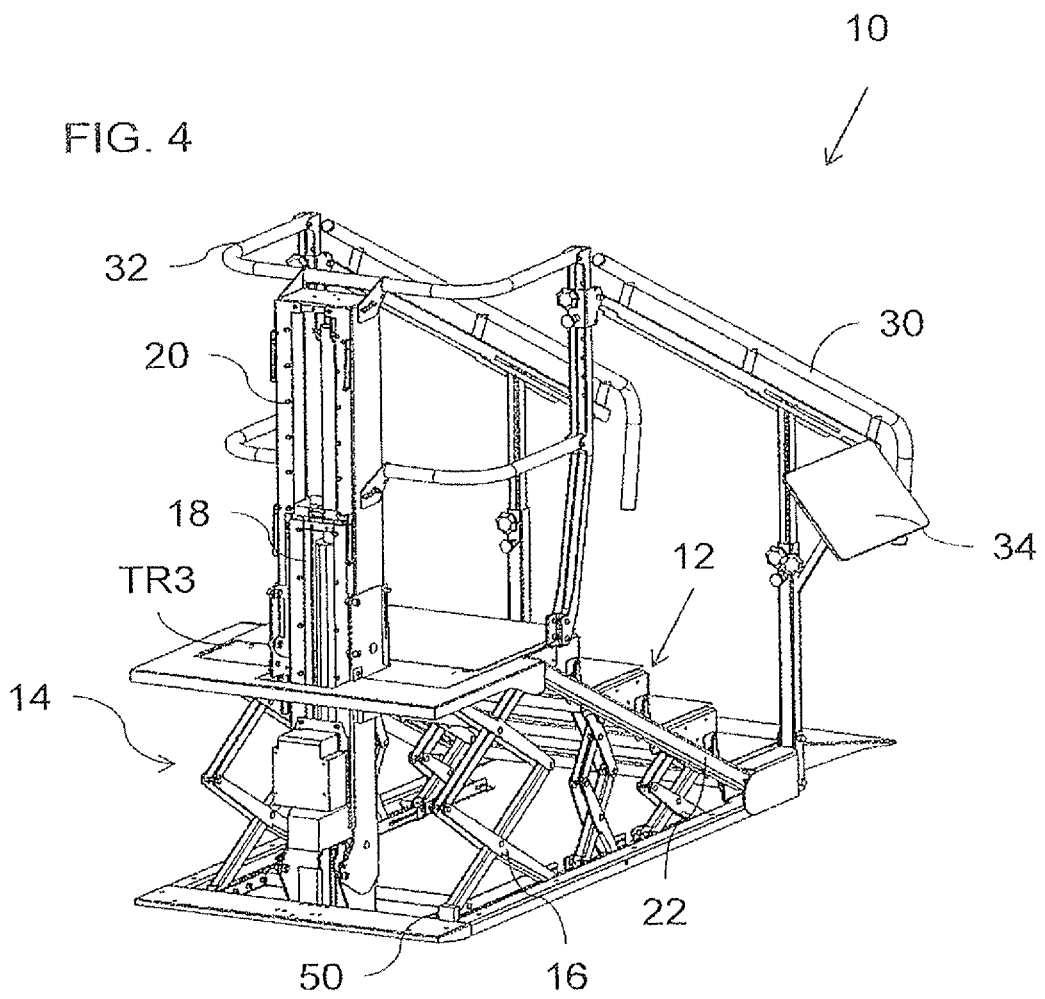


FIG. 6

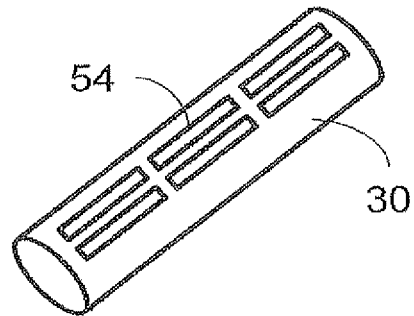


FIG. 7A

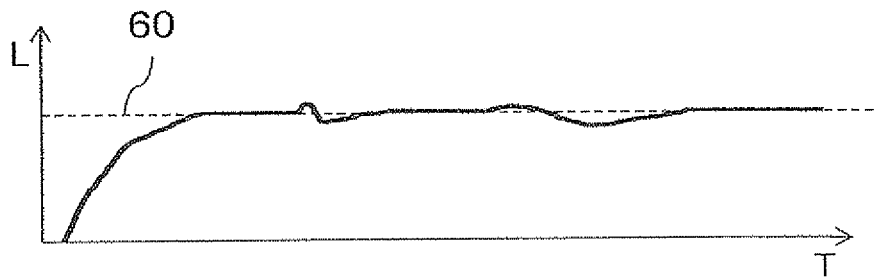


FIG. 7B

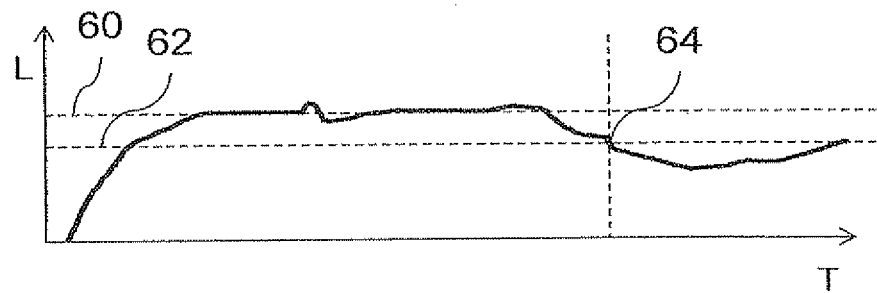


FIG. 8

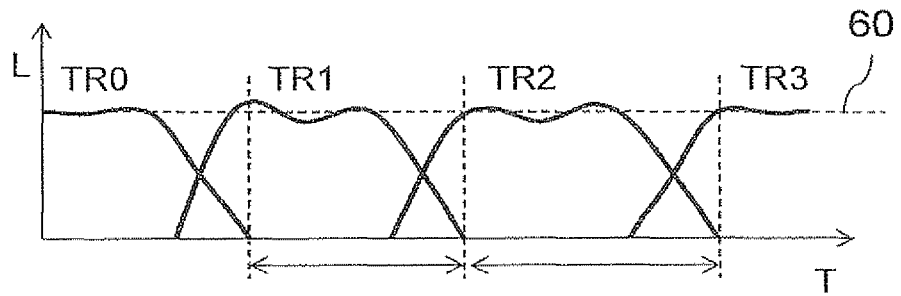


FIG. 9A

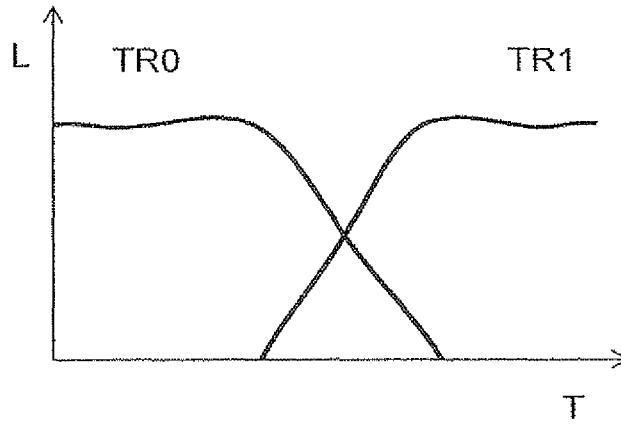


FIG. 9B

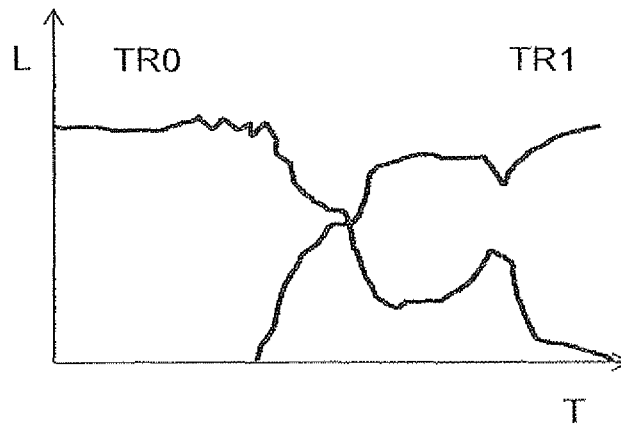


FIG. 10A

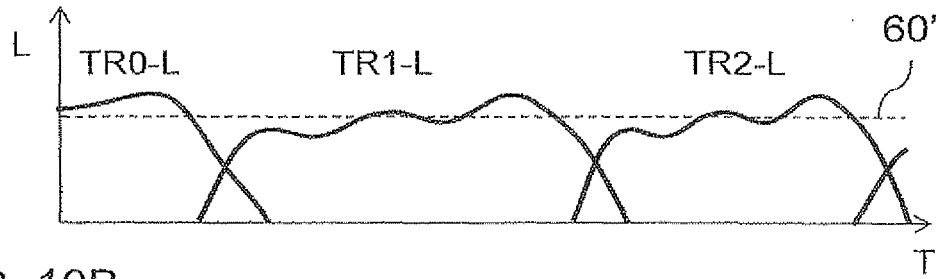


FIG. 10B

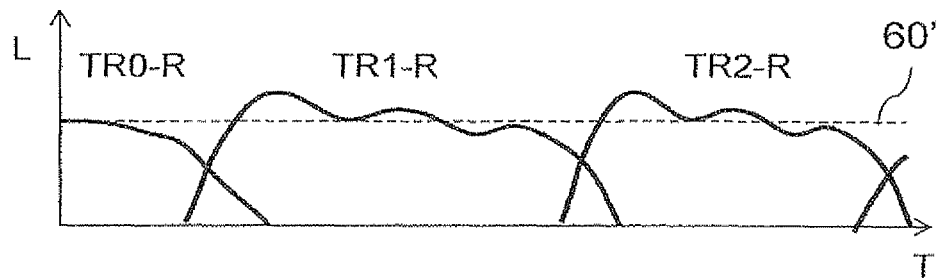


FIG. 11A

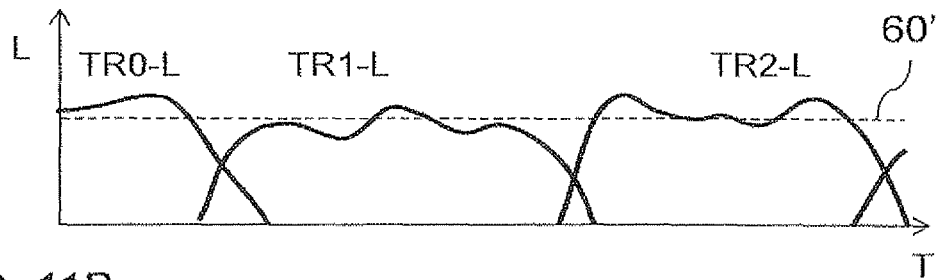


FIG. 11B

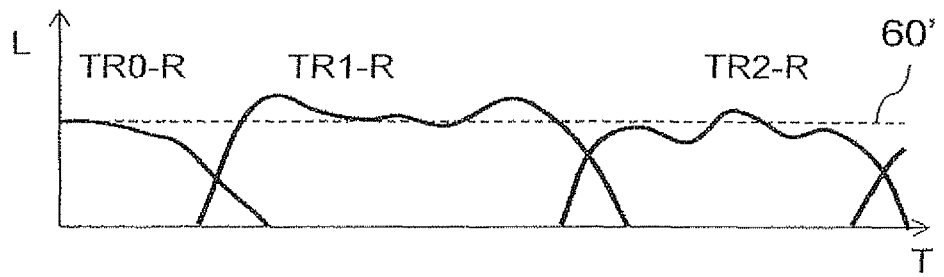


FIG. 12A


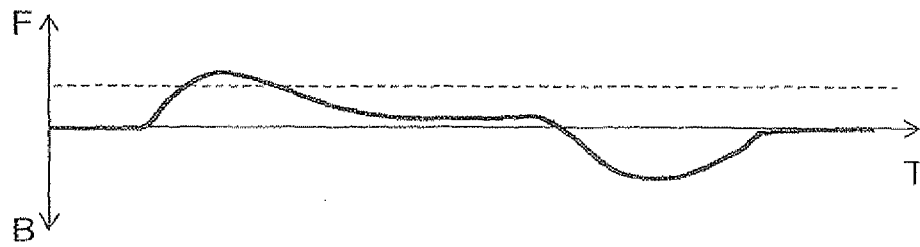


FIG. 12B

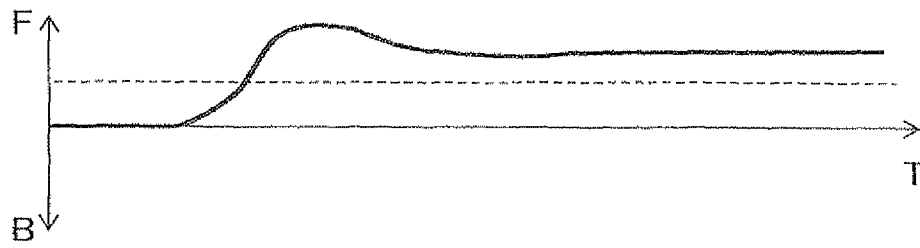

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 5901813 A [0004]
- US 5769759 A [0005]
- WO 2012057595 A [0005]
- US 2010099541 A [0005]
- US 8100770 B, Yamazaki [0045]

专利名称(译)	计算机辅助理疗楼梯和步态系统		
公开(公告)号	<a href="#">EP3071303A4</a>	公开(公告)日	2016-11-16
申请号	EP2014864289	申请日	2014-10-28
[标]申请(专利权)人(译)	DPE医疗		
申请(专利权)人(译)	DPE MEDICAL LTD.		
当前申请(专利权)人(译)	DPE MEDICAL LTD.		
[标]发明人	ORGAL DANIEL		
发明人	ORGAL, DANIEL		
IPC分类号	A63B23/04 A63B22/04 A61B5/00 A61B5/11 A63B21/00 A63B21/068 A63B24/00 A63B69/00 A63B71/06		
CPC分类号	A63B23/0405 A61B5/1114 A61B5/112 A61B5/1124 A61B5/6895 A61B2505/09 A61B2562/0252 A63B21/00181 A63B21/068 A63B22/04 A63B23/0458 A63B23/0464 A63B24/0087 A63B69/0057 A63B2024/0093 A63B2071/0627 A63B2071/0652 A63B2220/52 A63B2225/093 A63B2225/096 A63B2225/20 A63B2225/50 A63B2230/015 A63B2230/062		
优先权	14/084639 2013-11-20 US		
其他公开文献	EP3071303B1 EP3071303A1		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

计算机辅助的物理治疗台阶和步态系统具有一组至少三个水平胎面表面和相关联的驱动系统，用于调节相邻胎面表面之间的上升高度，以形成具有均匀节距的一组楼梯，用于不同上升的范围高度。传感器组测量与使用该组楼梯执行的物理治疗有关的参数，并向计算机系统提供输出。传感器包括以下中的一个或多个：用于感测楼梯的俯仰的上升高度传感器，心率传感器，扶手夹持位置传感器以及用于分析在系统使用期间患者的体重分布的测力传感器。