



(11)

EP 3 324 839 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

22.05.2019 Bulletin 2019/21

(51) Int Cl.:

A61B 5/026 ^(2006.01) **A61N 1/39** ^(2006.01)
A61B 5/00 ^(2006.01) **A61B 5/024** ^(2006.01)
A61B 5/1455 ^(2006.01)

(21) Application number: **16745513.8**

(86) International application number:

PCT/JP2016/003318

(22) Date of filing: **13.07.2016**

(87) International publication number:

WO 2017/013856 (26.01.2017 Gazette 2017/04)

(54) **LIFESAVING ASSISTING APPARATUS**

LEBENSRETTENDE HILFSVORRICHTUNG

APPAREIL D'AIDE AU SAUVETAGE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **17.07.2015 JP 2015143008**

12.05.2016 JP 2016096356

(43) Date of publication of application:

30.05.2018 Bulletin 2018/22

(73) Proprietors:

- **Nihon Kohden Corporation**
Tokyo 161-8560 (JP)
- **Kyoto University**
Kyoto-shi, Kyoto 606-8501 (JP)

(72) Inventors:

- **NATSUI, Tomoyoshi**
Tokyo 161-8560 (JP)
- **HAYASHI, Satoshi**
Tokyo 161-8560 (JP)

• **WAKABAYASHI, Tsutomu**

Tokyo 161-8560 (JP)

• **IWAMI, Taku**

Kyoto-shi

Kyoto 606-8501 (JP)

• **HATAKEYAMA, Toshihiro**

Kyoto-shi

Kyoto 606-8501 (JP)

• **NISHIMURA, Tetsuro**

Osaka-shi

Osaka 540-0006 (JP)

• **OTANI, Takayuki**

Suita-shi

Osaka 565-0862 (JP)

(74) Representative: **Hoffmann Eitle**

Patent- und Rechtsanwälte PartmbB

Arabellastraße 30

81925 München (DE)

(56) References cited:

US-A1- 2001 047 140 US-A1- 2004 116 969
US-A1- 2013 324 855 US-A1- 2014 247 274

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

2012-061361A

[PTL 2] US 2014/247274 A1

[PTL 3] US 2004/116969 A1

Technical Field

[0001] The present disclosure relates to a lifesaving assisting apparatus for determining whether to perform an act of lifesaving.

[0002] Use of an AED (Automatic External Defibrillator) can be exemplified as an act of lifesaving. The AED is an apparatus which delivers an electric shock to a patient in which fatal arrhythmia such as ventricular fibrillation or pulseless ventricular tachycardia has been detected, in order to revive the patient. Specifically, when the patient has no consciousness and respiration, electrode pads of the AED are pasted on the naked chest of the patient. The AED analyzes an electrocardiogram acquired through the electrode pads to detect the fatal arrhythmia (for example, see Patent Literature 1).

[0003] Patent Literature 2 relates to a display apparatus which can prevent erroneous recognition of a result of measurement of biological information from occurring and assist prompt determination. The display apparatus includes an instruction receiving section for receiving instructions from a user, a signal receiving section, a controlling section, and a displaying section. A probe is connected to the display apparatus and includes a light emitting section which emits a first light beam with a first wavelength and a second light beam with a second wavelength and a light receiving section which receives the first and second light beams passed through for example the finger of a patient and outputs a first and second signal. The signal receiving section supplies the first and second signal to the controlling section which performs measurements based on the received signals and acquires the light attenuation of the first light beam based on the first signal and the light attenuation of the second light beam based on the second signal. The display section displays a graph showing the temporal change of a blood-derived light attenuation as a blood refill curve such that the medical person is enabled to accurately recognize the blood refill time and the blood refill curve.

[0004] Patent Literature 3 relates to the detection of a cardiac pulse and the use of pulse detection in delivering therapy, wherein physiological signals in a patient are evaluated. A medical device evaluates optical characteristics of light transmitted into a patient to ascertain physiological signals such as pulsating changes in general blood volume proximate a light detector module. Using these features, the medical device determines whether a cardiac pulse is present in the patient.

Citation List**Patent Literature****[0005]**

[PTL 1] Japanese Patent Publication No.

5 Summary of Invention**Technical Problem**

[0006] In a case where a general citizen who is not a health care provider encounters a patient falling down in front of the citizen, even if the citizen can bring the AED to the patient, the citizen tends to hesitate about using the AED. Particularly, a patient who is in an agonal stage has unique respiration called gasping respiration though the patient is in a cardiopulmonary arrest state. Therefore, it is difficult for the citizen to accurately judge an unconscious and breathless state. As a result, the citizen may delay applying an electric shock to the patient. This contributes to the lowering of a lifesaving rate.

[0007] In addition, unconscious patients include patients caused by encephalopathy, low blood sugar, hemorrhagic shock, drowning, carbon monoxide poisoning, etc. Although it is unnecessary to use the AED on such a patient, it is difficult for a general citizen to make an accurate judgment on this. Accordingly, in some cases, privacy of the patient may be unable to be sufficiently protected because the chest of the patient is made naked unnecessarily in front of the general public. In addition, the necessity of a measure to make the chest naked also contributes to the hesitation of a lifesaver in using the AED.

[0008] Accordingly, there is an object to provide a lifesaver with proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking privacy of a patient into consideration.

Solution to Problem

[0009] The object of the invention is achieved by the subject-matter of the independent claims. Advantageous embodiments are defined in the dependent claims. Further examples are provided for facilitating the understanding of the invention. For example, there is provided a lifesaving assisting apparatus comprising:

a light-emitting section configured to emit light to be irradiated on a body of a patient;

a light-receiving section configured to output a signal corresponding to an intensity of light which has been transmitted through or reflected from the body of the patient; a pulse-amplitude Index acquiring section configured to analyze amplitude of the signal to acquire a pulse-amplitude Index of the patient; a pulse determining section configured to determine presence or absence of a pulse of the patient in accordance with the pulse-amplitude Index; and a notifying section configured to notify a result of determination made by the pulse determining section.

[0010] It is difficult even for an expert to judge presence or absence of the pulse accurately and rapidly. Particularly, a patient who is in an agonal stage has unique respiration called gasping respiration though the patient is in a cardiopulmonary arrest state. Therefore, there may be a case where presence of the pulse may be judged based on the fact of breathing. According to the above configuration, an objective parameter which is the pulse-amplitude Index of the patient is used. Accordingly, presence or absence of the pulse of the patient can be determined accurately no matter who handles the lifesaving assisting apparatus. In addition, presence or absence of the pulse can be determined by the pulse determining section as long as a pulse wave signal corresponding to several cycles to about ten cycles can be acquired. Accordingly, presence or absence of the pulse of the patient can be determined rapidly no matter who handles the lifesaving assisting apparatus.

[0011] A lifesaver can be notified of an accurate determination result about presence or absence of the pulse of the patient. Accordingly, for example, the lifesaver can avoid unnecessarily undressing the patient when it is not necessary to use the AED. In this manner, it is possible to protect privacy of the patient. Thus, it is possible to provide the lifesaver with proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration. The invention is defined in claim 1. Preferred embodiments are defined in the dependent claims.

Brief Description of Drawings

[0012]

Fig. 1 is a diagram showing the functional configuration of a lifesaving assisting apparatus according to one embodiment.

Fig. 2A is a diagram for explaining a definition of a pulse rate.

Fig. 2B is a diagram for explaining a definition of an inflection point number.

Fig. 2C is a diagram for explaining the definition of the inflection point number.

Fig. 2D is a diagram for explaining the definition of the inflection point number.

Fig. 3A is a flowchart showing process performed by the lifesaving assisting apparatus of Fig. 1.

Fig. 3B is a diagram showing a typical normalized pulse wave determined as presence of the pulse.

Fig. 3C is a diagram showing a typical normalized pulse wave determined as absence of the pulse.

Fig. 4A is a flowchart showing process performed by the lifesaving assisting apparatus of Fig. 1.

Fig. 4B is a flowchart showing process performed by the lifesaving assisting apparatus of Fig. 1.

Fig. 5 is a diagram showing one example of how to use the lifesaving assisting apparatus of Fig. 1.

Description of Embodiment

[0013] Exemplary embodiments will be described below in detail with reference to the accompanying drawings. The respective drawings which will be used in the following description are changed in scale suitably to make the sizes of respective members recognizable.

[0014] Fig. 1 shows the functional configuration of a lifesaving assisting apparatus 1 according to one embodiment. The lifesaving assisting apparatus 1 is an apparatus which detects presence or absence of a pulse of a patient 100 to thereby determine whether to perform an act of lifesaving.

[0015] The lifesaving assisting apparatus 1 is provided with a light-emitting section 21. The light-emitting section 21 is configured to emit light to be irradiated on the body of the patient 100. The body of the patient 100 means tissues where a blood flow exists. For example, a semiconductor light-emitting element which can emit light having a predetermined wavelength may be used as the light-emitting section 21. Examples of the semiconductor light-emitting element include a light-emitting diode (LED), a laser diode, an organic EL element, etc. Infrared light IR and red light R may be used as examples of the light having the predetermined wavelength.

[0016] The lifesaving assisting apparatus 1 is provided with a light emission controlling section 31. The light emission controlling section 31 is configured to control switching on/off of a light source in the light-emitting section 21.

[0017] The lifesaving assisting apparatus 1 is provided with a light-receiving section 22. The light-receiving section 22 is configured to output a signal corresponding to intensity of the light transmitted through or reflected from the body of the patient 100. For example, an optical sensor having sensitivity to the wavelength of the light emitted from the light-emitting section 21 may be used as the light-receiving section 22. Examples of the optical sensor include a photodiode, a phototransistor and a photoreistor.

[0018] The lifesaving assisting apparatus 1 is provided with a pulse-amplitude Index acquiring section 32. The pulse-amplitude Index acquiring section 32 is configured to analyze amplitude of a signal outputted from the light-receiving section 22 to acquire a pulse-amplitude Index of the patient 100. The pulse-amplitude Index will be described with reference to Fig. 2A.

[0019] When the patient 100 has a pulse, a blood amount in the tissues on which the light is irradiated by the light-emitting section 21 changes. Accordingly, the intensity of the light detected by the light-receiving section 22 changes, and the amplitude of the signal outputted from the light-receiving section 22 changes. That is, the signal outputted from the light-receiving section 22 is a pulse wave.

[0020] The pulse-amplitude Index acquiring section 32 is provided with a filter which extracts a DC component from the pulse wave. That is, the pulse-amplitude Index

acquiring section 32 is configured to obtain a pulsating component and a non-pulsating component from the pulse wave signal outputted from the light-receiving section 22. When the light emitted from the light-emitting section 21 is infrared light IR or red light R, the pulsating component during the change of the intensity of the light detected by the light-receiving section 22 is mainly an amount of contribution from arterial blood, and the non-pulsating component is mainly an amount of contribution from the tissues or venous blood. The pulse-amplitude Index acquiring section 32 is configured to acquire a normalized pulse wave PW in order to eliminate a component depending on the patient 100 personally. The normalized pulse wave PW is obtained by dividing the pulsating component by the non-pulsating component.

[0021] Amplitude of the normalized pulse wave PW is defined as pulse-amplitude Index X. There is however a case where the amplitude may change between a maximum value P1 and a next maximum value P2 which exist before and behind a minimum value B of a certain specific wave because the normalized pulse wave PW drifts. On this occasion, the amplitude in the minimum value B takes a value between (P1-B) and (P2-B). Accordingly, the pulse-amplitude Index X can be expressed by the following expression by way of example.

$$X = (A1+A2)/2$$

[0022] Here, A1 designates a difference in amplitude (absolute value) between the maximum value P1 at a time point at which the amplitude of the normalized pulse wave PW takes the maximum value P1 and the minimum value B. A2 designates a difference in amplitude (absolute value) between the maximum value P2 at a time point at which the amplitude of the normalized pulse wave PW takes the maximum value P2 and the minimum value B. That is, the pulse-amplitude Index X in the example is given as an average value of A1 and A2. However, the pulse-amplitude Index X may be set at any value between A1 and A2.

[0023] Similarly, the pulse-amplitude Index acquiring section 32 acquires a pulse-amplitude Index X as to a next signal cycle defined by the maximum value P2 and a maximum value P3. The pulse-amplitude Index acquiring section 32 is configured to acquire a representative pulse-amplitude Index based on a plurality of pulse-amplitude Indices X acquired thus within a predetermined period. The representative pulse-amplitude Index is defined as an average value of the plurality of pulse-amplitude Indices X.

[0024] Incidentally, in order to acquire the representative pulse-amplitude Index, it is preferable that samples accounting for a predetermined percentage are removed from the plurality of pulse-amplitude Indices X acquired within the predetermined period and an average value of the remaining samples is obtained. For example, top

25% may be used as the predetermined percentage. For example, in a case where eight samples have been acquired, two samples are removed in descending order in the value of the pulse-amplitude Index X from the eight samples and a representative pulse-amplitude Index is obtained as an average value of the remaining six samples.

[0025] The lifesaving assisting apparatus 1 is provided with a pulse determining section 33. The pulse determining section 33 is configured to determine presence or absence of the pulse of the patient 100 based on the pulse-amplitude Indices X acquired by the pulse-amplitude Index acquiring section 32. Specifically, the pulse determining section 33 is configured to determine presence or absence of the pulse of the patient 100 based on whether the representative pulse-amplitude Index acquired by the pulse-amplitude Index acquiring section 32 is lower than a predetermined threshold. For example, 1% may be used as the threshold. The pulse determining section 33 is configured as follows. That is, in a case where the representative pulse-amplitude Index is lower than the threshold, the pulse determining section 33 determines that the patient 100 has no pulse. When the representative pulse-amplitude Index is no lower than the threshold, the pulse determining section 33 determines that the patient 100 has a pulse.

[0026] The lifesaving assisting apparatus 1 is provided with a notifying section 34. The notifying section 34 is configured to notify a result of the determination made by the pulse determining section 33. The notification is performed by at least one of optical notification (light emission of an LED, display of a message on a display device, etc.), acoustic notification (a guidance message, a melody, a beep, etc.), and vibratory notification.

[0027] As described above, there are various reasons causing the patient's syncope. In some cases, it is not necessary to use the AED to deliver an electric shock. Cardiogenic syncope belongs to a case in which an electric shock does not have to be delivered. The cardiogenic syncope can be judged based on the fact that there is no pulse. Syncope caused by encephalopathy, massive bleeding, low blood sugar, anemia, hypocapnia, etc. belongs to a case in which an electric shock does not have to (or must not) be delivered. Such cardiogenic syncope can be judged based on the fact that there is a pulse.

[0028] However, it is difficult even for an expert to judge presence or absence of the pulse accurately and rapidly. Particularly, a patient who is in an agonal stage has unique respiration called gasping respiration though the patient is in a cardiopulmonary arrest state. Therefore, there may be a case where presence of the pulse may be judged based on the fact of breathing. According to the configuration of the lifesaving assisting apparatus 1 according to the embodiment, an objective parameter which is the pulse-amplitude Index X of the patient 100 is used. Accordingly, presence or absence of the pulse of the patient 100 can be determined accurately no matter who handles the lifesaving assisting apparatus 1. In ad-

dition, presence or absence of the pulse can be determined by the pulse determining section 33 as long as a pulse wave signal corresponding to several cycles to about ten cycles can be acquired. Accordingly, presence or absence of the pulse of the patient 100 can be determined rapidly no matter who handles the lifesaving assisting apparatus 1.

[0029] The lifesaver can be notified of an accurate determination result about presence or absence of the pulse of the patient 100. Accordingly, for example, the lifesaver can avoid unnecessarily undressing the patient 100 when it is not necessary to use the AED. In this manner, it is possible to protect privacy of the patient 100. Thus, it is possible to provide the lifesaver with proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration.

[0030] The pulse-amplitude Index acquiring section 32 is configured to acquire the pulse-amplitude Index X based on the infrared light IR emitted from the light-emitting section 21.

[0031] According to such a configuration, a light source used in a probe of a pulse oximeter generally used in critical care can be used. It is unnecessary to prepare a separate light source. Therefore, it is possible to suppress the total cost for providing the lifesaving assisting apparatus 1. In addition, the infrared light is hardly affected by the color of skin when it is transmitted through or reflected from the body of the patient 100. In this manner, accuracy of the acquired pulse-amplitude Index X is improved, and accuracy of determination of presence or absence of the pulse made by the pulse determining section 33 in the subsequent stage is also improved. Accordingly, it is possible to provide the lifesaver with more proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration.

[0032] The pulse determining section 33 may be configured to determine presence or absence of the pulse of the patient 100 based on not only the aforementioned pulse-amplitude Index X but also an inflection point number N within a predetermined time duration in the signal outputted from the light-receiving section 22. For example, one second may be used as the predetermined time duration.

[0033] As shown in Figs. 2B, 2C and 2D, the "inflection point number" herein is defined as the number of times in which a differential value of a normalized pulse wave PW alternates between positive and negative. In the example shown in Fig. 2B, the differential value of the normalized pulse wave PW changes from positive to negative and changes to positive again. Accordingly, the inflection point number N is 2. On the other hand, in the examples shown in Figs. 2C and 2D, the differential value of the normalized pulse wave PW reaches zero in the middle but does not alternate between positive and negative before and behind the zero. Accordingly, the inflection point number N is 0.

[0034] Fig. 3A is a flowchart showing a determination process performed by the pulse determining section 33 in this embodiment. First, the pulse determining section 33 determines whether the pulse-amplitude Index X (representative pulse-amplitude Index) of the patient 100 acquired by the pulse-amplitude Index acquiring section 32 is lower than a predetermined threshold (step S11).

[0035] When it is determined that the pulse-amplitude Index X is lower than the predetermined threshold (Y in the step S11), the pulse determining section 33 counts the inflection point number N of the normalized pulse wave PW in a predetermined period, and determines whether the inflection point number N is lower than a first threshold (step S12). For example, 10 may be used as the first threshold.

[0036] When it is determined that the inflection point number N is lower than the first threshold (Y in the step S12), the pulse determining section 33 determines that the patient 100 has a pulse (step S13). This situation means that the result determined as absence of the pulse based on the pulse-amplitude Index X is reversed by the determination based on the inflection point number N.

[0037] When it is determined that the inflection point number N is no lower than the first threshold (N in the step S12), the pulse determining section 33 determines that the patient 100 has no pulse (step S14). This situation means that the result determined as absence of the pulse based on the pulse-amplitude Index X is confirmed by the determination based on the inflection point number N.

[0038] When it is determined that the pulse-amplitude Index X is no lower than the predetermined threshold (N in the step S11), the pulse determining section 33 counts the inflection point number N of the normalized pulse wave PW within the predetermined period and determines whether the inflection point number N is lower than a second threshold (step S15). For example, 15 may be used as the second threshold.

[0039] When it is determined that the inflection point number N is lower than the second threshold (Y in the step S15), the pulse determining section 33 determines that the patient 100 has a pulse (step S16). This situation means that the result determined as presence of the pulse based on the pulse-amplitude Index X is confirmed by the determination based on the inflection point number N.

[0040] When it is determined that the inflection point number N is no lower than the second threshold (N in the step S15), the pulse determining section 33 determines that the patient 100 has no pulse (step S17). This situation means that the result determined as presence of the pulse based on the pulse-amplitude Index X is reversed by the determination based on the inflection point number N.

[0041] Fig. 3B shows a typical normalized pulse wave PW determined as presence of the pulse. The inflection point number N in an illustrated period is lower than 10. Fig. 3C shows a typical normalized pulse wave PW de-

terminated as absence of the pulse. The inflection point number N in the illustrated period is higher than 100.

[0042] As shown in the situation of the step S13 or S17, the inflection point number N is added to determination criteria. In this manner, accuracy of determination of presence or absence of the pulse is improved. Accordingly, it is possible to provide the lifesaver with more proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration.

[0043] The pulse determining section 33 is configured to acquire the inflection point number N based on the infrared light IR emitted from the light-emitting section 21.

[0044] According to such a configuration, it is possible to use a light source used in a probe of a pulse oximeter generally used in critical care. It is therefore unnecessary to prepare a separate light source. Accordingly, it is possible to suppress the total cost for providing the lifesaving assisting apparatus 1. In addition, the infrared light is hardly affected by the color of skin when it is transmitted through or reflected from the body of the patient 100. In this manner, accuracy of the acquired inflection point number N is improved, and accuracy of determination of presence or absence of the pulse made by the pulse determining section 33 in the subsequent stage is also improved. Accordingly, it is possible to provide the lifesaver with more proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration.

[0045] As shown in Fig. 1, the lifesaving assisting apparatus 1 may be provided with a pulse re-determining section 35. In this case, the light-emitting section 21 is configured to emit infrared light IR and red light R. In addition, the light-receiving section 22 is configured to output signals respectively corresponding to intensities of the infrared light IR and the red light R transmitted through or reflected from the body of the patient 100. The pulse re-determining section 35 is configured as follows. That is, in a case where it is determined by the pulse determining section 33 that the patient 100 has a pulse, the pulse re-determining section 35 acquires arterial oxygen saturation (SpO₂) and a heart rate of the patient 100 based on the signals outputted from the light-receiving section 22 and re-determines presence or absence of the pulse of the patient 100 based on these biological parameters.

[0046] A process for acquiring the arterial oxygen saturation and the heart rate from the intensities of the infrared light and the red light transmitted through or reflected from biological tissues is based on the principles of the pulse oximeter. Since the process per se is widely known, detailed description thereof will be omitted.

[0047] Fig. 4A is a flowchart illustrating operation of the pulse re-determining section 35 in the example. As described previously, a determination process is performed by the pulse determining section 33 (step S1). When the determination process results in a conclusion that the patient 100 has a pulse, a re-determination process

is executed by the pulse re-determining section 35 (step S2).

[0048] Fig. 4B is a flowchart showing a specific flow of the re-determination process. First, the pulse re-determining section 35 determines whether the acquired arterial oxygen saturation of the patient 100 is lower than a predetermined threshold (step S21). For example, 85% may be used as the threshold.

[0049] When it is determined that the arterial oxygen saturation of the patient 100 is no lower than the threshold (N in the step S21), the pulse re-determining section 35 determines whether the acquired heart rate of the patient 100 is lower than a predetermined threshold (step S22). For example, 40 times per minute may be used as the threshold.

[0050] When it is determined that the heart rate of the patient 100 is no lower than the threshold (N in the step S22), the pulse re-determining section 35 determines that the patient 100 has a pulse (step S23). This situation means that the result determined as presence of the pulse by the pulse determining section 33 is confirmed by the re-determination made by the pulse re-determining section 35.

[0051] When it is determined that the arterial oxygen saturation of the patient 100 is lower than the predetermined threshold (Y in the step S21) or in a case where it is determined that the heart rate of the patient 100 is lower than the predetermined value (Y in the step S22), the pulse re-determining section 35 determines that the patient 100 has no pulse (step S24). This situation means that the result determined as presence of the pulse by the pulse determining section 33 is reversed by the re-determination made by the pulse re-determining section 35.

[0052] That is, the pulse re-determining section 35 provides a fail-safe function in the lifesaving assisting apparatus 1. In this manner, even when the patient 100 who should be essentially determined as having no pulse has been determined as having a pulse by the pulse determining section 33 for some reason, the patient 100 can be determined as having no pulse by the pulse re-determining section 35. Accordingly, it is possible to provide the lifesaver with more proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration.

[0053] In the re-determination process shown in Fig. 4B, the sequence of the determination about the arterial oxygen saturation (step S21) and the determination about the heart rate (step S22) may be reverse to each other. In addition, configuration may be made so that only one of the determination about the arterial oxygen saturation (step S21) and the determination about the heart rate (step S22) is performed.

[0054] Fig. 5 schematically shows one example of how to use the lifesaving assisting apparatus 1. The lifesaving assisting apparatus 1 is provided with a probe 2 and a casing 3. The probe 2 includes the light-emitting section

21 and the light-receiving section 22. The light emission controlling section 31, the pulse-amplitude Index acquiring section 32, the pulse determining section 33, the notifying section 34 and the pulse re-determining section 35 are received in the casing 3.

[0055] The probe 2 including the light-emitting section 21 and the light-receiving section 22 is configured to be able to be mounted on a forehead 101 of the patient 100.

[0056] According to such a configuration, it is not necessary to undress the patient 100 when it is first determined whether the patient 100 has a pulse. In addition, the forehead 101 is a region which is hardly affected by body motion. It is therefore possible to improve accuracy of determination of presence or absence of the pulse. Accordingly, it is possible to provide the lifesaver with more proper information about whether to perform an act of lifesaving in order to assist the lifesaver while taking the privacy of the patient into consideration.

[0057] When the light-emitting section 21 is configured to emit infrared light or red light, a probe of a pulse oximeter can be used. Since a separate probe does not have to be prepared, it is possible to suppress the total cost for providing the lifesaving assisting apparatus 1.

[0058] As shown in Fig. 4A, the lifesaving assisting apparatus 1 executes a notification process (step S3) when the determination process (step S1) results in a conclusion that the patient 100 has no pulse or when the re-determination process (step S2) results in a conclusion that the patient 100 has no pulse. Specifically, the notifying section 34 provides information for promoting the lifesaver to use the AED. For example, voice guidance "No pulse can be detected. Please use AED." can be outputted. As shown in Fig. 5, the lifesaver mounts electrodes 201 of an AED 200 on a chest 102 of the patient 100 and executes a lifesaving measure in accordance with the voice guidance of the AED 200.

[0059] According to such a configuration, it is possible to expect an effect to strongly promote the hesitating lifesaver to use the AED 200. In addition, for example, the lifesaver may be replaced by another lifesaver who can use the AED 200. Thus, certainty of leading to use of the AED 200 can be improved.

[0060] In addition to or in place of this, the notifying section 34 provides information for promoting the lifesaver to perform sternum compressions. For example, voice guidance "No pulse can be detected. Please perform sternum compressions." can be outputted. The lifesaver performs sternum compressions on the chest 102 of the patient 100.

[0061] According to such a configuration, it is possible to expect an effect to strongly promote the hesitating lifesaver to perform a specific action. In addition, for example, the lifesaver may be replaced by another lifesaver who can perform a measure. Thus, certainty of leading to lifesaving can be improved.

[0062] Even after determining that the patient 100 has no pulse, the pulse determining section 33 can continuously perform the determination process for determining

presence or absence of the pulse. In this case, the notifying section 34 may be configured to provide information for promoting the lifesaver to suspend performance of sternum compressions in a case where it is determined that the patient 100 has a pulse although it has been once determined as having no pulse. For example, voice guidance "Pulse has been restarted. Please do not perform sternum compressions." can be outputted.

[0063] According to such a configuration, it is possible to properly deal with the case where the condition of the patient 100 determined once as having no pulse has been improved. That is, it is possible to avoid performing unnecessary chest compressions on the patient 100 whose heart has restarted beating. Accordingly, it is possible to prevent an unnecessary load from being imposed on the sternum of the patient 100.

[0064] When the re-determination process (step S2) made by the pulse re-determining section 35 results in a conclusion that the patient 100 has a pulse as designated by a dashed line in Fig. 4A, the lifesaving assisting apparatus 1 may perform the notification process (step S3) for sending notification of the fact that the patient 100 has a pulse. Then, the lifesaving assisting apparatus 1 re-execute the determination process (step S1) with the pulse determining section 33. In other words, the pulse determining section 33 continuously performs the determination process for determining presence or absence of the pulse even after determining that the patient 100 has a pulse.

[0065] According to such a configuration, it is possible to properly deal with the case where the condition of the patient 100 who was determined once as having a pulse has changed suddenly. That is, the aforementioned notification process is performed in a case where the determination process performed continuously results in a conclusion that the patient 100 has fallen into a no-pulse condition.

[0066] In the embodiment, the functions of the light emission controlling section 31, the pulse-amplitude Index acquiring section 32, the pulse determining section 33, the notifying section 34 and the pulse re-determining section 35 are at least partially achieved by software executed by the cooperation of a processor and a memory which are connected to each other communicably. A CPU or an MPU may be used as the processor by way of example. An RAM or an ROM may be used as the memory by way of example. However, the functions of the light emission controlling section 31, the pulse-amplitude Index acquiring section 32, the pulse determining section 33, the notifying section 34 and the pulse re-determining section 35 may be at least partially achieved by hardware such as an ASIC and an FPGA, or by a combination of hardware and software.

[0067] The aforementioned embodiment is merely exemplified in order to make the disclosed concept easy to understand. The configuration according to the aforementioned embodiment can be changed or modified suitably without departing from the disclosed concept. In ad-

dition, it is obvious that equivalents are contained in the claimed scope.

[0068] Only the infrared light IR is used for acquiring the pulse-amplitude Index X and the inflection point number N in the aforementioned embodiment. However, both the infrared light IR and the red light R may be used for acquiring the pulse-amplitude Index X and the inflection point number N, or only the red light R may be used for acquiring the pulse-amplitude Index X and the inflection point number N. Switching on/off of light sources for emitting the respective lights may be controlled suitably by the light emission controlling section 31.

[0069] The region where the probe 2 is mounted does not have to be always the forehead 101 of the patient 100. A transmissive type pulse oximeter may be configured to be mounted on the tip of a finger, the tip of a toe, an ear, etc. Also in the case, it is possible to determine presence or absence of the pulse without undressing the patient 100.

[0070] The probe 2 does not have to be always a probe of a pulse oximeter. As long as information about the blood flow can be acquired, the probe 2 may be configured as at least a part of an instrument (an ultrasonic blood flowmeter, an electromagnetic blood flowmeter, a laser blood flowmeter, a Doppler blood flowmeter, etc.) using any of an ultrasonic wave, an electromagnetic wave and laser light. In this case, the probe 2 may be mounted on a neck portion, an arm portion or a leg portion of the patient 100. In any case, it is possible to determine presence or absence of the pulse while suppressing exposure of the skin of the patient 100 to the minimum.

[0071] The example in which the lifesaver is promoted to use the AED 200 by the notifying section 34 has been described in the aforementioned embodiment. The notifying section 34 may be configured to promote the lifesaver to use not just the AED 200 but any general defibrillator.

[0072] The present application is based on Japanese Patent Application No. 2015-143008 filed on July 17, 2015 and Japanese Patent Application No. 2016-096356 filed on May 12, 2016, the contents of which are hereby incorporated by reference.

Claims

1. A lifesaving assisting apparatus (1) comprising:

a light-emitting section (21) configured to emit light to be irradiated on a body of a patient (100);
a light-receiving section (22) configured to output a signal corresponding to an intensity of light which has been transmitted through or reflected from the body of the patient (100);
a pulse-amplitude Index acquiring section (32) configured to analyse amplitude of the signal to acquire a pulse-amplitude Index of the patient (100) wherein the pulse-amplitude Index acquiring

section (32) is further configured to acquire a representative pulse-amplitude Index based on a plurality of pulse-amplitude Indices acquired within a predetermined period and wherein the representative pulse-amplitude Index is defined as an average value of the plurality of pulse-amplitude Indices;
a pulse determining section (33) configured to determine presence or absence of a pulse of the patient (100) in accordance with the representative pulse-amplitude Index; and
a notifying section (34) configured to notify a result of determination made by the pulse determining section (33).

2. The lifesaving assisting apparatus according to Claim 1,
wherein the pulse determining section is configured to determine the presence or absence of the pulse in accordance with an inflection point number of the signal within a predetermined time duration, in addition to the representative pulse-amplitude Index.
3. The lifesaving assisting apparatus (1) according to Claim 1 or 2,
wherein the light-emitting section (21) is configured to emit infrared light as the light; and
wherein the pulse-amplitude Index acquiring section (32) is configured to acquire the pulse-amplitude Index in accordance with the infrared light.
4. The lifesaving assisting apparatus (1) according to Claim 2 or 3,
wherein the light-emitting section (21) is configured to emit infrared light as the light; and
wherein the pulse-amplitude Index acquiring section (32) is configured to acquire the inflection point number in accordance with the infrared light.
5. The lifesaving assisting apparatus (1) according to any one of Claims 1 to 4,
wherein the light-emitting section (21) is configured to emit infrared light and red light as the light; and
wherein the lifesaving assisting apparatus (1) comprises a pulse re-determining section (35) configured to redetermine the presence or absence of the pulse of the patient (100) in accordance with at least one of arterial oxygen saturation and a heart rate obtained from the signal, in a case where the pulse determining section (33) has determined the presence of the pulse.
6. The lifesaving assisting apparatus (1) according to any one of Claims 1 to 5,
wherein the light-emitting section (21) and the light-receiving section (22) are configured to be attached on a forehead of the patient (100).

7. The lifesaving assisting apparatus (1) according to any one of Claims 1 to 6,
wherein the notifying section (34) is configured to provide information promoting usage of a defibrillator, in a case where the pulse determining section (33) has determined the absence of the pulse. 5
8. The lifesaving assisting apparatus (1) according to any one of Claims 1 to 7,
wherein the notifying section (34) is configured to provide information promoting to perform sternum compressions, in a case where the pulse determining section (33) has determined the absence of the pulse. 10
9. The lifesaving assisting apparatus (1) according to any one of Claims 1 to 8,
wherein the pulse determining section (33) is configured to continue determining the presence or absence of the pulse even after the presence of the pulse has once been determined. 15 20
10. The lifesaving assisting apparatus (1) according to any one of Claims 7 to 9,
wherein the notifying section (34) is configured to notify a result of determination as to the presence or absence of the pulse made by the pulse determining section (33) after the presence of the pulse has once been determined. 25
11. The lifesaving assisting apparatus (1) according to any one of Claims 1 to 10,
wherein the pulse determining section (33) is configured to continue determining the presence or absence of the pulse even after the presence of the pulse has once determined; and
wherein the notifying section (34) is configured to provide information promoting to suspend performance of sternum compressions, in a case where the pulse determining section (33) determines the presence of the pulse after the absence of the pulse has once been determined. 30 35 40

Patentansprüche

1. Lebensrettende Hilfseinrichtung (1), umfassend:

einen lichtemittierenden Abschnitt (21), der konfiguriert ist, um Licht zu emittieren, das auf einen Körper eines Patienten (100) zu strahlen ist;
einen lichtempfangenden Abschnitt (22), der konfiguriert ist, um ein Signal auszugeben, das einer Intensität eines Lichts entspricht, das durch den Körper des Patienten (100) geleitet oder von diesem zurückgeworfen wurde;
einen Abschnitt zum Erfassen eines Pulsamplitudenindexes (32), der konfiguriert ist, um eine 50 55

Amplitude des Signals zu analysieren, um einen Pulsamplitudenindex des Patienten (100) zu erfassen, wobei der Abschnitt zum Erfassen eines Pulsamplitudenindexes (32) weiter konfiguriert ist, um basierend auf einer Vielzahl von Pulsamplitudenindizes, die innerhalb einer vorbestimmten Periode erfasst werden, einen repräsentativen Pulsamplitudenindex zu erfassen, und wobei der repräsentative Pulsamplitudenindex als ein Durchschnittswert der Vielzahl von Pulsamplitudenindizes definiert ist;
einen Pulsbestimmungsabschnitt (33), der konfiguriert ist, um in Übereinstimmung mit dem repräsentativen Pulsamplitudenindex eine Anwesenheit oder Abwesenheit eines Pulses des Patienten (100) zu bestimmen; und
einen Anzeigeabschnitt (34), der konfiguriert ist, um ein Ergebnis einer Bestimmung, die durch den Pulsbestimmungsabschnitt (33) gemacht wird, anzuzeigen.

2. Lebensrettende Hilfseinrichtung nach Anspruch 1, wobei der Pulsbestimmungsabschnitt konfiguriert ist, um die Anwesenheit oder Abwesenheit des Pulses in Übereinstimmung mit einer Wendepunkanzahl des Signals innerhalb einer vorbestimmten Zeitdauer, zusätzlich zum repräsentativen Pulsamplitudenindex, zu bestimmen.

3. Lebensrettende Hilfseinrichtung (1) nach Anspruch 1 oder 2, wobei der lichtemittierende Abschnitt (21) konfiguriert ist, um Infrarotlicht als das Licht zu emittieren; und
wobei der Abschnitt zum Erfassen eines Pulsamplitudenindexes (32) konfiguriert ist, um den Pulsamplitudenindex in Übereinstimmung mit dem Infrarotlicht zu erfassen. 30 35

4. Lebensrettende Hilfseinrichtung (1) nach Anspruch 2 oder 3, wobei der lichtemittierende Abschnitt (21) konfiguriert ist, um Infrarotlicht als das Licht zu emittieren; und
wobei der Abschnitt zum Erfassen eines Pulsamplitudenindexes (32) konfiguriert ist, um die Wendepunkanzahl in Übereinstimmung mit dem Infrarotlicht zu erfassen. 40 45

5. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 1 bis 4, wobei der lichtemittierende Abschnitt (21) konfiguriert ist, um Infrarotlicht und Rotlicht als das Licht zu emittieren; und
wobei die lebensrettende Hilfseinrichtung (1) einen Pulswiederbestimmungsabschnitt (35) umfasst, der konfiguriert ist, um in einem Fall, in dem der Pulsbestimmungsabschnitt (33) die Anwesenheit des Pul- 50 55

ses bestimmt hat, die Anwesenheit oder Abwesenheit des Pulses des Patienten (100) in Übereinstimmung mit mindestens einem von arterieller Sauerstoffsättigung und einer vom Signal erhaltenen Herzfrequenz wiederzubestimmen.

6. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 1 bis 5,
wobei der lichtemittierende Abschnitt (21) und der lichtempfangende Abschnitt (22) konfiguriert sind, um an eine Stirn des Patienten (100) befestigt zu werden. 10
7. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 1 bis 6,
wobei der Anzeigeabschnitt (34) konfiguriert ist, um in einem Fall, in dem der Pulsbestimmungsabschnitt (33) die Abwesenheit des Pulses bestimmt hat, Informationen bereitzustellen, die den Gebrauch eines Defibrillators fördern. 15 20
8. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 1 bis 7,
wobei der Anzeigeabschnitt (34) konfiguriert ist, um in einem Fall, in dem der Pulsbestimmungsabschnitt (33) die Abwesenheit des Pulses bestimmt hat, Informationen bereitzustellen, die ein Durchführen von Sternumkompressionen fördern. 25
9. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 1 bis 8,
wobei der Pulsbestimmungsabschnitt (33) konfiguriert ist, um weiterhin die Anwesenheit oder Abwesenheit des Pulses zu bestimmen, sogar nachdem die Anwesenheit des Pulses einmal bestimmt wurde. 30 35
10. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 7 bis 9,
wobei der Anzeigeabschnitt (34) konfiguriert ist, um ein Ergebnis einer Bestimmung hinsichtlich der Anwesenheit oder der Abwesenheit des Pulses, die vom Pulsbestimmungsabschnitt (33) gemacht wird, anzuzeigen, nachdem die Anwesenheit des Pulses einmal bestimmt wurde. 40
11. Lebensrettende Hilfseinrichtung (1) nach einem der Ansprüche 1 bis 10,
wobei der Pulsbestimmungsabschnitt (33) konfiguriert ist, um weiterhin die Anwesenheit oder Abwesenheit des Pulses zu bestimmen, sogar nachdem die Anwesenheit des Pulses einmal bestimmt wurde; und
wobei der Anzeigeabschnitt (34) konfiguriert ist, um in einem Fall, in dem der Pulsbestimmungsabschnitt (33) die Anwesenheit des Pulses bestimmt, nachdem die Abwesenheit des Pulses einmal bestimmt wurde, Informationen bereitzustellen, die ein Aussetzen einer Durchführung von Sternumkompressionen fördern. 45 50 55

onen fördern.

Revendications

1. Appareil d'aide au sauvetage (1) comprenant :

une section d'émission de lumière (21) configurée pour émettre une lumière à irradier sur un corps d'un patient (100) ;
une section de réception de lumière (22) configurée pour produire un signal correspondant à une intensité de lumière qui a été transmise à travers ou réfléchi par le corps du patient (100) ;
une section d'acquisition d'indice d'amplitude de pouls (32) configurée pour analyser l'amplitude du signal pour acquérir un indice d'amplitude de pouls du patient (100) dans lequel la section d'acquisition de l'indice d'amplitude de pouls (32) est en outre configurée pour acquérir un indice d'amplitude de pouls représentatif basé sur une pluralité d'indices d'amplitude de pouls acquis durant une période prédéterminée et dans lequel l'indice d'amplitude de pouls représentatif est défini comme une valeur moyenne de la pluralité d'indices d'amplitude de pouls ;
une section de détermination de pouls (33) configurée pour déterminer la présence ou l'absence d'un pouls du patient (100) selon l'indice d'amplitude de pouls représentatif ; et
une section de notification (34) configurée pour notifier un résultat de détermination établi par la section de détermination de pouls (33).

2. Appareil d'aide au sauvetage selon la revendication 1, dans lequel la section de détermination de pouls est configurée pour déterminer la présence ou l'absence du pouls selon un nombre de points d'inflexion du signal pendant une durée prédéterminée, outre l'indice d'amplitude de pouls représentatif.


3. Appareil d'aide au sauvetage (1) selon la revendication 1 ou 2, dans lequel la section d'émission de lumière (21) est configurée pour émettre une lumière infrarouge en tant que lumière ; et dans lequel la section d'acquisition d'indice d'amplitude de pouls (32) est configurée pour acquérir l'indice d'amplitude de pouls selon la lumière infrarouge.

4. Appareil d'aide au sauvetage (1) selon la revendication 2 ou 3, dans lequel la section d'émission de lumière (21) est configurée pour émettre une lumière infrarouge en tant que lumière ; et


- dans lequel la section d'acquisition d'indice d'amplitude de pouls (32) est configurée pour acquérir le nombre de points d'inflexion selon la lumière infrarouge.
- 5
5. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 1 à 4,
dans lequel la section d'émission de lumière (21) est configurée pour émettre une lumière infrarouge et une lumière rouge en tant que lumière ; et
dans lequel l'appareil d'aide au sauvetage (1) comprend une section de re-détermination de pouls (35) configurée pour redéterminer la présence ou l'absence du pouls du patient (100) selon au moins une saturation en oxygène artériel et une fréquence cardiaque obtenues du signal, dans un cas où la section de détermination de pouls (33) a déterminé la présence du pouls.
- 10
- 15
6. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 1 à 5,
dans lequel la section d'émission de lumière (21) et la section de réception de lumière (22) sont configurées pour être fixées sur un front du patient (100).
- 20
- 25
7. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 1 à 6,
dans lequel la section de notification (34) est configurée pour fournir des informations favorisant l'utilisation d'un défibrillateur, dans un cas où la section de détermination de pouls (33) a déterminé l'absence du pouls.
- 30
8. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 1 à 7,
dans lequel la section de notification (34) est configurée pour fournir des informations favorisant la réalisation de compressions thoraciques, dans un cas où la section de détermination d'impulsions (33) a déterminé l'absence du pouls.
- 35
- 40
9. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 1 à 8,
dans lequel la section de détermination de pouls (33) est configurée pour continuer de déterminer la présence ou l'absence du pouls même après que la présence du pouls a été déterminée une fois.
- 45
10. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 7 à 9,
dans lequel la section de notification (34) est configurée pour notifier un résultat de détermination relativement à la présence ou l'absence du pouls établi par la section de détermination de pouls (33) après que la présence du pouls a été déterminée une fois.
- 50
- 55
11. Appareil d'aide au sauvetage (1) selon l'une quelconque des revendications 1 à 10,

dans lequel la section de détermination de pouls (33) est configurée pour continuer de déterminer la présence ou l'absence du pouls même après que la présence du pouls a été déterminée une fois ; et dans lequel la section de notification (34) est configurée pour fournir des informations favorisant la suspension de la réalisation de compressions thoraciques, dans un cas où la section de détermination de pouls (33) détermine la présence du pouls après que l'absence du pouls a été déterminée une fois.

[Fig. 1]

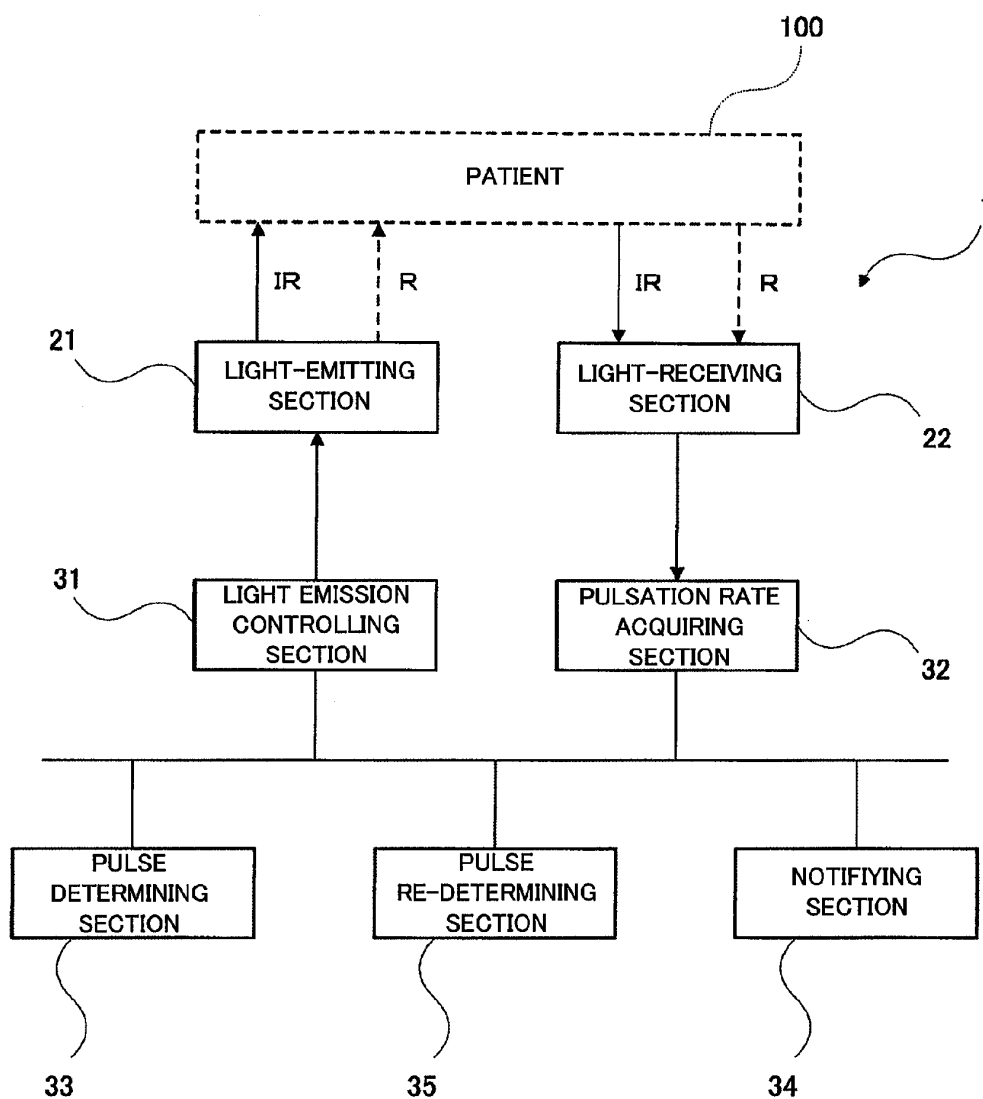
FIG. 1

[Fig. 2A]

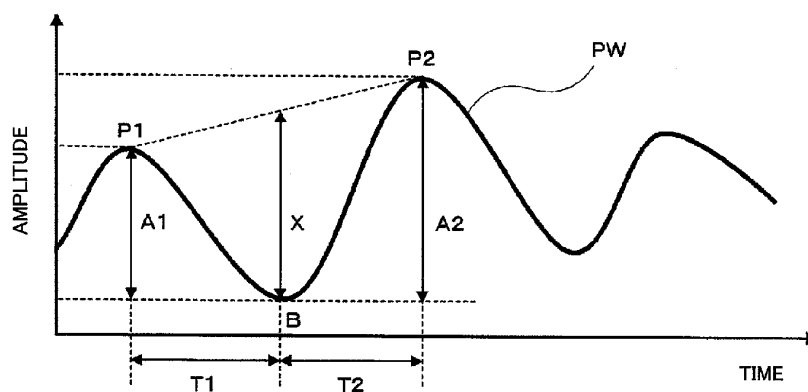FIG. 2A

[Fig. 2B]


FIG. 2B

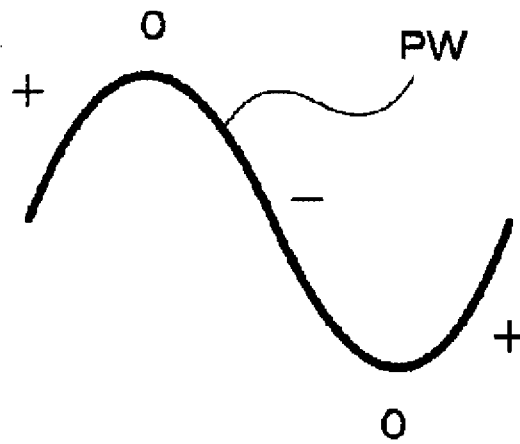

$N=2$

[Fig. 2C]


FIG. 2C

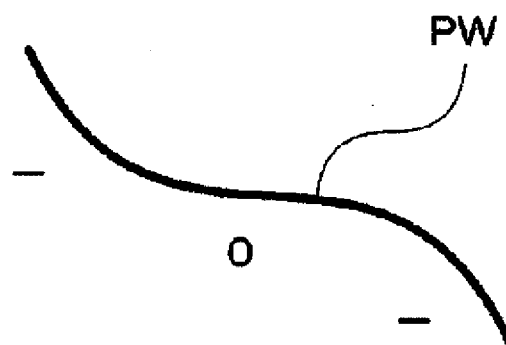

$N=0$

[Fig. 2D]


FIG. 2D

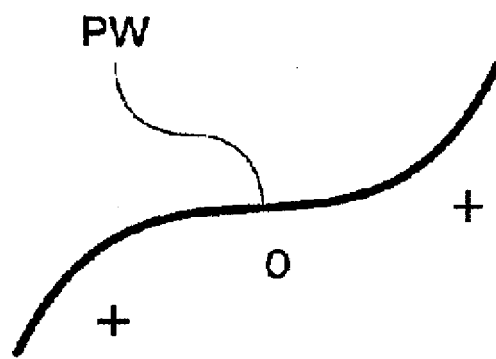

$N=0$


[Fig. 3A]

FIG. 3A

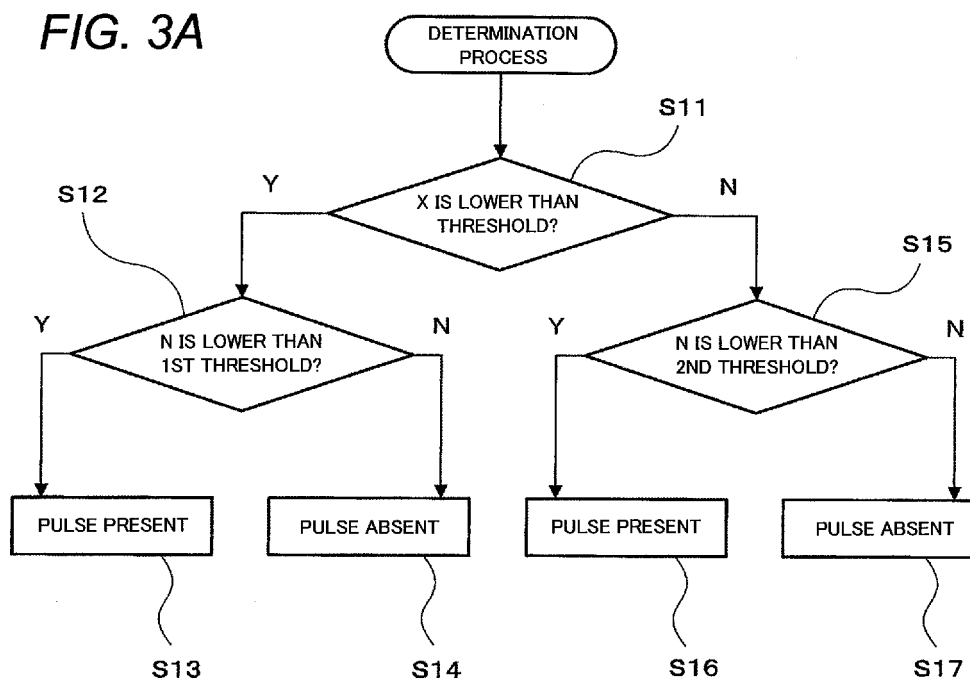


[Fig. 3B]

FIG. 3B

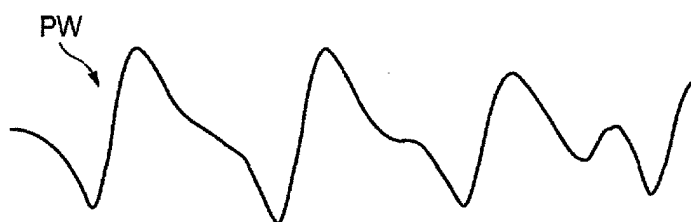


[Fig. 3C]

FIG. 3C

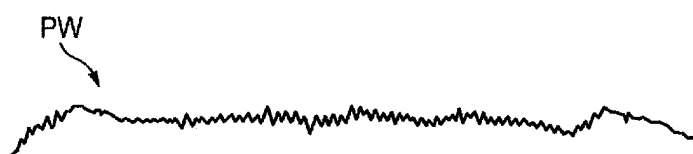


[Fig. 4A]

FIG. 4A

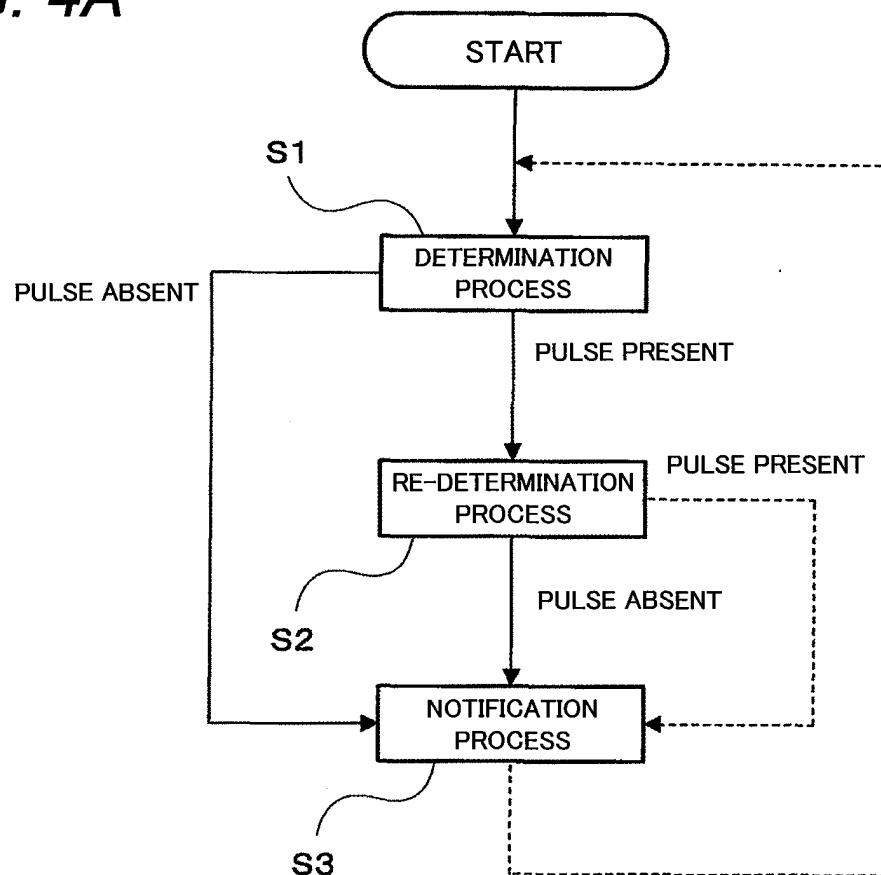

[Fig. 4B]

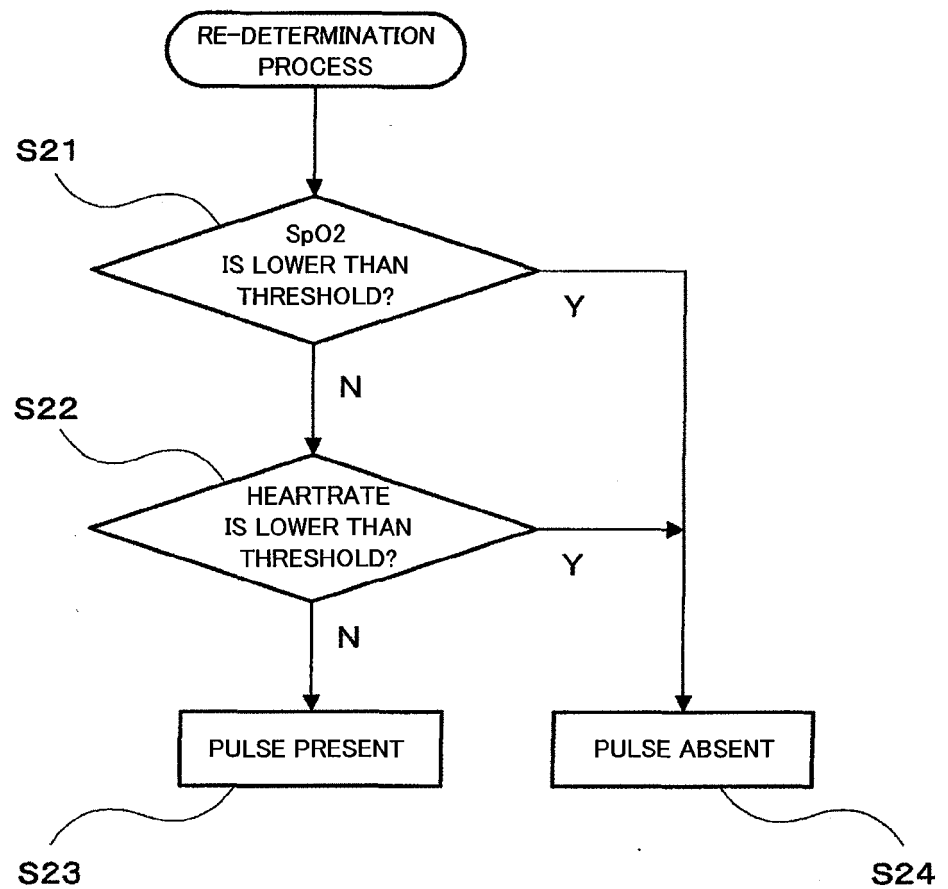FIG. 4B

[Fig. 5]

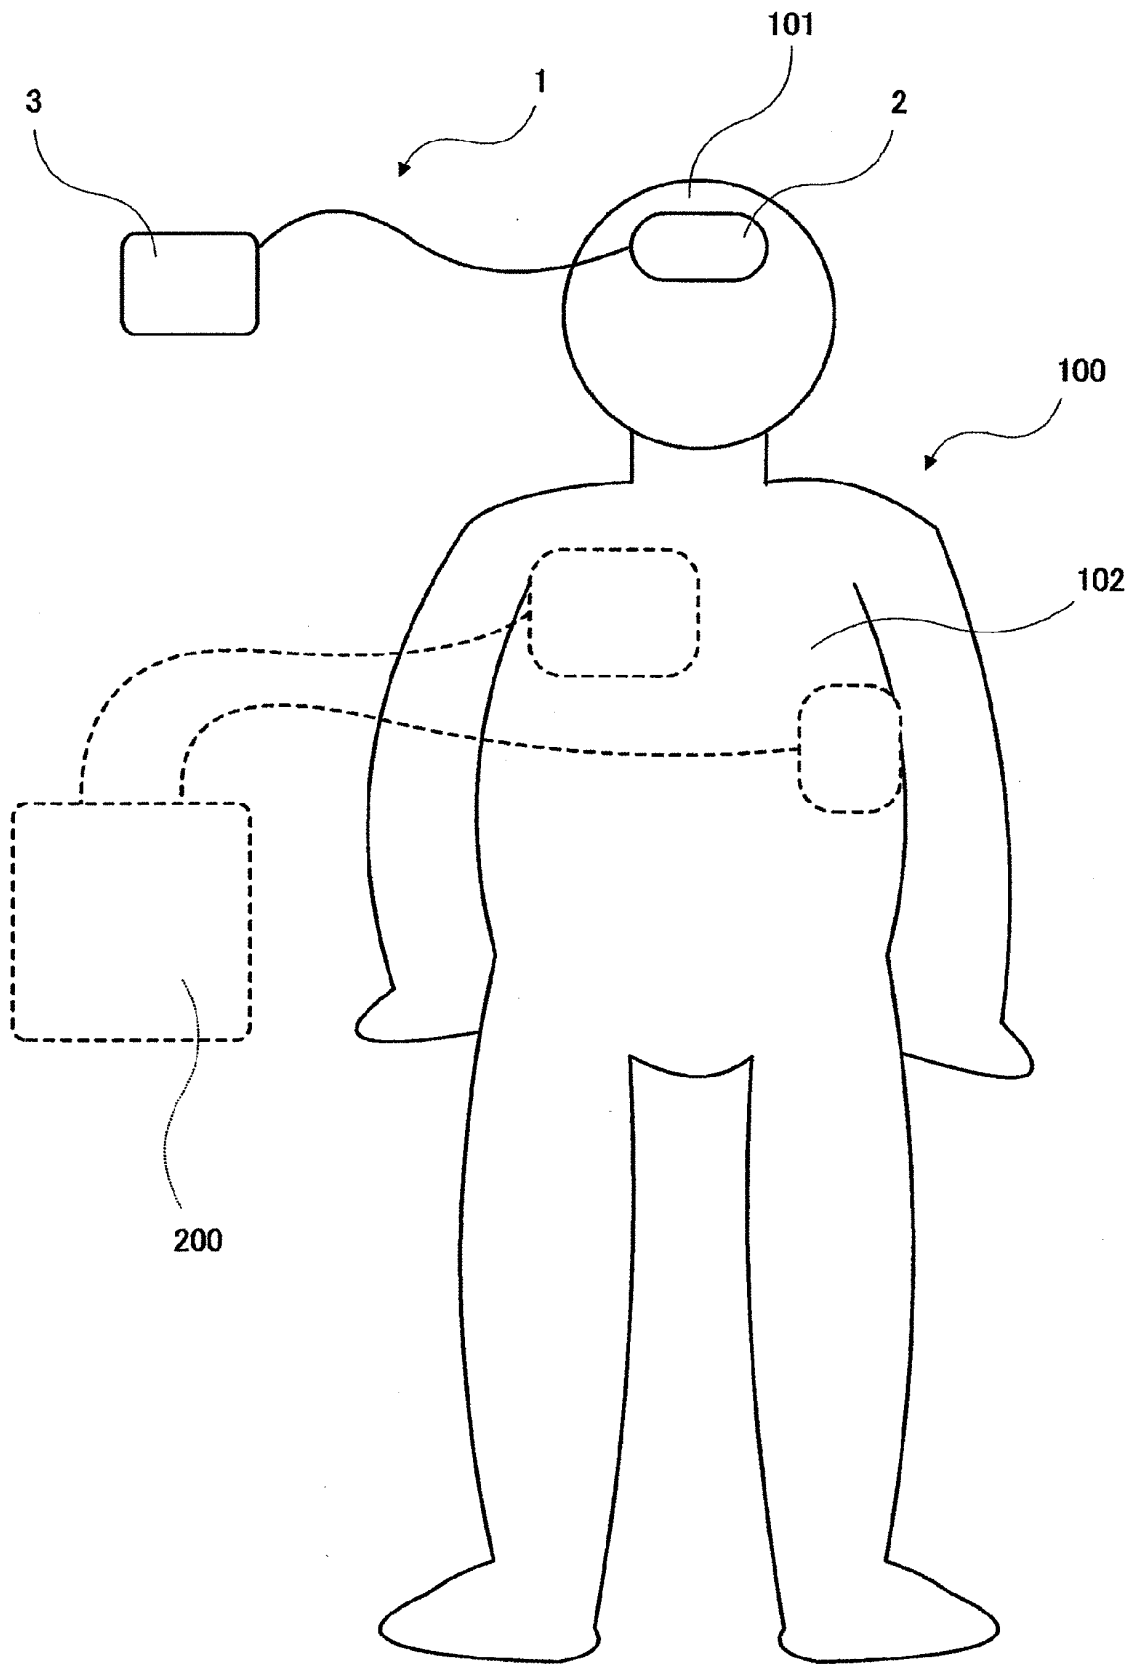


FIG. 5

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2012061361 A [0005]
- US 2014247274 A1 [0005]
- US 2004116969 A1 [0005]
- JP 2015143008 A [0072]
- JP 2016096356 A [0072]

专利名称(译)	救生辅助器具		
公开(公告)号	EP3324839B1	公开(公告)日	2019-05-22
申请号	EP2016745513	申请日	2016-07-13
[标]申请(专利权)人(译)	日本光电工业株式会社 国立大学法人京都大学		
申请(专利权)人(译)	日本光电公司 京都大学		
当前申请(专利权)人(译)	日本光电公司 京都大学		
[标]发明人	NATSUI TOMOYOSHI HAYASHI SATOSHI WAKABAYASHI TSUTOMU IWAMI TAKU HATAKEYAMA TOSHIHIRO NISHIMURA TETSURO OTANI TAKAYUKI		
发明人	NATSUI, TOMOYOSHI HAYASHI, SATOSHI WAKABAYASHI, TSUTOMU IWAMI, TAKU HATAKEYAMA, TOSHIHIRO NISHIMURA, TETSURO OTANI, TAKAYUKI		
IPC分类号	A61B5/026 A61N1/39 A61B5/00 A61B5/024 A61B5/1455		
CPC分类号	A61B5/02433 A61B5/026 A61B5/14552 A61B5/7405 A61N1/39		
优先权	2016096356 2016-05-12 JP 2015143008 2015-07-17 JP		
其他公开文献	EP3324839A1		
外部链接	Espacenet		

摘要(译)

发光部分 (21) 发射光以照射在患者 (100) 的身体上。光接收部分 (22) 输出对应于已经透过患者体 (100) 或从患者体内反射的光强度的信号。脉冲幅度指数获取部分 (32) 分析信号的幅度以获取患者 (100) 的脉冲幅度指数。脉冲确定部分 (33) 根据脉冲幅度指数确定患者 (100) 的脉搏的存在或不存在。通知部分 (34) 通知由脉冲确定部分 (33) 作出的确定结果。

$$X = \frac{(A1 + A2)}{2}$$