

(19)



(11)

EP 3 130 285 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
15.02.2017 Bulletin 2017/07

(51) Int Cl.:
A61B 5/0452 ^(2006.01) **A61B 5/0464** ^(2006.01)
A61B 5/042 ^(2006.01) **A61B 5/046** ^(2006.01)
A61B 5/00 ^(2006.01)

(21) Application number: **16183500.4**

(22) Date of filing: **10.08.2016**

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**
Designated Extension States:
BA ME
Designated Validation States:
MA MD

(71) Applicant: **Biosense Webster (Israel) Ltd.**
2066717 Yokneam (IL)

(72) Inventors:
• **Rubinstein, Vladimir**
2066717 Yokneam (IL)
• **Bar-Tal, Meir**
2066717 Yokneam (IL)

(30) Priority: **11.08.2015 US 201562203422 P**
11.07.2016 US 201615206418

(74) Representative: **Carpmaels & Ransford LLP**
One Southampton Row
London WC1B 5HA (GB)

(54) **MATCHING AND TRACKING TIME SEQUENCES OF HEART ACTIVATION**

(57) A method, including, receiving a first group of electrocardiograph (ECG) signals derived from a single heartbeat and generated at a respective plurality of electrodes on a catheter in a heart of a subject, formulating a template relating times of annotations of the first group of the ECG signals, and assigning the template an index. The method further includes receiving a second group of ECG signals derived from a subsequent single heartbeat and generated at the electrodes, calculating times

of annotations of the second group, formulating a comparison between the template and the times of annotations of the second group, and, when the comparison indicates that the times of annotations of the second group correspond to the template, assigning the index to the second group of ECG signals, and presenting graphically on a display an occurrence of the template relative to a timeline representing heartbeats from the heart.

EP 3 130 285 A1

Description**CROSS-REFERENCE TO RELATED APPLICATION**

- 5 **[0001]** This application claims the benefit of U.S. Provisional Patent Application 62/203,422, filed August 11, 2015, which is incorporated herein by reference.

FIELD OF THE INVENTION

- 10 **[0002]** This invention relates generally to analysis of electrocardiograph (ECG) signals, and specifically to analysis of groups of such signals.

BACKGROUND OF THE INVENTION

- 15 **[0003]** An article titled "Pattern and Timing of the Coronary Sinus Activation to Guide Rapid Diagnosis of Atrial Tachycardia After Atrial Fibrillation Ablation" by Pascale et al, published in Circ Arrhythm Electrophysiol. 2013, is incorporated herein by reference. In the article, the authors state that atrial tachycardias (AT) during or after ablation of atrial fibrillation frequently pose a diagnostic challenge. The authors hypothesize that both the patterns and the timing of coronary sinus (CS) activation could facilitate AT mapping.
- 20 **[0004]** U.S. Patent Application 2015/0208938, to Houben et al., whose disclosure is incorporated herein by reference, describes detection of an activation wavefront generated in the heart, using bipolar and unipolar electrograms.
- [0005]** The description above is presented as a general overview of related art in this field and should not be construed as an admission that any of the information it contains constitutes prior art against the present patent application.
- 25 **[0006]** Documents incorporated by reference in the present patent application are to be considered an integral part of the application except that, to the extent that any terms are defined in these incorporated documents in a manner that conflicts with definitions made explicitly or implicitly in the present specification, only the definitions in the present specification should be considered.

SUMMARY OF THE INVENTION

- 30 **[0007]** An embodiment of the present invention provides a method, including:
- receiving a first group of electrocardiograph (ECG) signals derived from a single heartbeat and generated at a respective plurality of electrodes on a catheter in a heart of a subject;
- 35 formulating a template relating times of annotations of the first group of the ECG signals, and assigning the template an index;
- receiving a second group of ECG signals derived from a subsequent single heartbeat and generated at the plurality of electrodes;
- calculating times of annotations of the second group of ECG signals;
- 40 formulating a comparison between the template and the times of annotations of the second group; and
- when the comparison indicates that the times of annotations of the second group correspond to the template, assigning the index to the second group of ECG signals, and presenting graphically on a display an occurrence of the template relative to a timeline representing heartbeats from the heart.
- 45 **[0008]** A disclosed embodiment includes using the first group and the second group to formulate a common map of the heart.
- [0009]** A further disclosed embodiment includes, when the comparison indicates that the times of annotations of the second group do not correspond to the template, formulating a further template relating the times of annotations of the second group of the ECG signals, and assigning the further template a further index, and presenting graphically on the
- 50 display a further occurrence of the further template relative to the timeline. Typically, the method includes using the first group to formulate a first map of the heart, and the second group to formulate a second map, different from the first map of the heart.
- [0010]** A yet further disclosed embodiment includes receiving a stream of channel annotations, slicing the stream into segments corresponding to respective heartbeats, estimating a reference annotation as one of an average, a weighted average, or a median, of the channel annotations of the segments in the stream, and applying the reference annotation in formulating the template. Typically, the template includes differences between the times of annotations of the first group with the reference annotation.
- 55 **[0011]** In an alternative embodiment the catheter is located in a coronary sinus of the heart.

[0012] In a further alternative embodiment the plurality of electrodes are evenly spaced along the catheter.

[0013] In a yet further alternative embodiment the catheter is linear.

[0014] In some embodiments the template is assigned to a first type of arrhythmia, and the method further includes receiving a subsequent group of ECG signals, and monitoring if the times of annotations of the subsequent group do not correspond to the template, thus indicating that the subsequent group of ECG signals corresponds to a second type of arrhythmia, different from the first type.

[0015] There is further provided, according to an embodiment of the present invention, apparatus, including:

a catheter, located in a heart of a subject and configured to:

receive a first group of electrocardiograph (ECG) signals derived from a single heartbeat and generated at a respective plurality of electrodes on the catheter, and
receive a second group of ECG signals derived from a subsequent single heartbeat and generated at the plurality of electrodes;

a processor configured to:

formulate a template relating times of annotations of the first group of the ECG signals, and assign the template an index,
calculate times of annotations of the second group of ECG signals,
formulate a comparison between the template and the times of annotations of the second group, and
when the comparison indicates that the times of annotations of the second group correspond to the template, assign the index to the second group of ECG signals; and

a display configured to present graphically an occurrence of the template relative to a timeline representing heartbeats from the heart.

[0016] The present disclosure will be more fully understood from the following detailed description of the embodiments thereof, taken together with the drawings, in which:

Brief description of the drawings

[0017]

Fig. 1 is a schematic block diagram illustrating operation of a signal analyzing algorithm, according to an embodiment of the present invention;

Fig. 2 is an example of unipolar ECG signals with their annotations and their weighted average, according to an embodiment of the present invention;

Fig. 3 is a graphical presentation of the time pattern of the signals of Fig. 2, according to an embodiment of the present invention;

Fig. 4 is a flowchart illustrating steps of a template tracking mode of an algorithm, according to an embodiment of the present invention;

Fig. 5 is a flowchart illustrating steps of a template matching mode of the algorithm, according to an embodiment of the present invention;

Fig. 6 is a schematic graph of a template number as a function of beat, or group of annotations, number, that is presented on a display, according to an embodiment of the present invention;

Fig. 7 illustrates a correlation between a template and a group of annotations, according to an embodiment of the present invention; and

Fig. 8 illustrates an anti-correlation between a template and a group of annotations, according to an embodiment of the present invention.

DETAILED DESCRIPTION OF EMBODIMENTS

OVERVIEW

[0018] The time patterns of the coronary sinus (CS) activations can be helpful in atrial tachycardia (AT) mapping. The analysis of time patterns of CS activation provides a rapid stratification, or ordering, of most likely macro-reentrant ATs, and the analysis also points toward the likely origin of focal ATs.

[0019] The inventors have developed a method that analyzes multi-channel unipolar ECG signals so as to match and track time patterns of the signals. In one embodiment, the method finds, and keeps track of, certain "time configuration of activities" specific to different types of cardiac behavior. A "time configuration of activities," also referred to herein as a "time pattern," corresponds to specific time interrelations between unipolar annotations of the ECG signals. The annotations correspond to a local activation time (LAT) of the signal.

[0020] LAT maps, derived from the ECG signals, may be used in analyzing functioning of the heart, and such maps are constructed by the CARTO® system, produced by Biosense-Webster of Diamond Bar CA. The maps typically illustrate the results produced by several mechanisms of electrical wave generation in the heart under arrhythmias. Embodiments of the present invention may automatically separate and track these different mechanisms so as to build LAT maps that may contain only a single type of the heart activation. Embodiments of the present invention enable faster and more accurate production of LAT maps.

DETAILED DESCRIPTION

1. Introduction

[0021] Fig. 1 is a schematic block diagram illustrating operation of a signal analyzing algorithm, according to an embodiment of the present invention. The algorithm is operated by a processor 10 which receives multiple electrocardiograph (ECG) signals from a reference catheter distal end 14 that is located in the coronary sinus (CS), and results of the operation of the algorithm may be presented by the processor on a display 18 of the system. Results of the operation may be incorporated into a map 21 of the heart, and/or in the form of a graph 24, and both types of results are described below. In one embodiment catheter distal end 14 is approximately linear and has ten (10) electrodes evenly spaced along the distal end. In some embodiments the electrodes are arranged in pairs.

[0022] As is described in more detail below, the algorithm analyzes incoming ECG signals of the reference catheter, and from the analysis identifies different types of uniform heart activations. The heart activations are supplied to an LAT mapping procedure, and the algorithm may also be used as a filter that indicates when to acquire a new point in the mapping procedure. Elements used to implement the algorithm, i.e., the processor, the catheter, and the display, may be present in the CARTO® system referenced above. The algorithm may be used in real-time analysis of ECG signals, and/or for analysis of recorded signals.

[0023] The processor uses a time pattern tracker block 22, to determine and keep track of "time configuration of activities" or "time patterns" that describe specific time interrelations between annotations, or LATs, of ECG signals. As is illustrated in Fig. 1, the processor sets a time interval, a window of interest, $\{\text{ref_Anno}(t_i) - \tau_1 \text{WOI}, \text{ref_Anno}(t_i) + \tau_2 \text{WOI}\}$ when the tracker is to operate. (t_i is an identifying time of the time interval, $\tau_1 \text{WOI}$ is an initial time of the interval, and $\tau_2 \text{WOI}$ is a final time of the interval.) During this interval the tracker receives results of Wave Front annotation calculations performed by the processor on the ECG signals. The calculations are performed in a wave front annotation block 26, wherein the processor operates a wavefront algorithm to calculate the annotation time for each ECG signal. A suitable algorithm is described in U.S. Patent Application 2015/0208938, referenced above.

[0024] The tracker estimates a similarity of the current activation to a pre-set template (Template(n), where n, a positive integer, is a template index. A template is a descriptor of a time pattern of annotations.

[0025] As described below, the algorithm run by processor 10 and tracker block 22 may operate in two modes, a template tracking (TT) mode wherein the time pattern is calculated from incoming ECG signals and is compared with an existing (pre-set) template, and a template matching (TM) mode wherein new templates may be generated from the signals.

2. Calculation of a time pattern

[0026] To calculate the time pattern of a plurality of the CS reference channels the processor annotates each channel of a given heartbeat (in a given time interval comprising the heartbeat) - $\text{annUniChn}(k, t_i)$, where k is an index of the channels, forming a group of annotations. The processor then calculates a weighted average $w\text{Average}(t_i)$ of the group of annotations according to equation (1):

$$w\text{Average}(t_i) = \sum_k^K \left| \frac{d\text{Uni}(k, t_i)}{dt} \right| * \text{annUniChn}(k, t_i) / \sum_k^K \left| \frac{d\text{Uni}(k, t_i)}{dt} \right| \quad (1)$$

where $\text{Uni}(k, t_i)$ is the k^{th} ECG signal in the time interval $\{\text{ref_Anno}(t_i) - \tau_1 \text{WOI}, \text{ref_Anno}(t_i) + \tau_2 \text{WOI}\}$, $\text{annUniChn}(k, t_i)$ is the annotation of the k^{th} ECG signal,

$\frac{dUni(k,t_i)}{dt}$ is a derivative of the k^{th} ECG signal in a neighborhood of the annotation $annUniChn(k, ti)$,
 and

k is the total number of channels, i.e., the total number of electrodes on the CS catheter distal end.

[0027] An example of unipolar ECG signals with their annotations (solid circles) and their weighted average (black vertical line) is presented in Fig. 2. The processor then calculates the difference between each annotation in the group and the weighted average ($dT(k,ti)$). The k -dimensional vector of the differences we call the "time pattern" of this group. A graphical presentation of the time pattern is shown in Fig. 3.

3. Algorithm Description

[0028] Processor 10 uses tracker block 22 (Fig. 1) to operate an algorithm working in one of two modes: the Template Tracking (TT) mode and the Template Matching (TM) mode referred to above. The TT mode is typically implemented initially.

[0029] Fig. 4 is a flowchart illustrating steps of the TT mode, according to an embodiment of the present invention. In an initial step 30, the processor initially provides block 22 with a reference annotation ($ref_Anno(ti)$), a window of interest ($\{\tau1WOI, \tau2WOI\}$) and a template of the time pattern ($Template(n)$). Template(n) is produced in the TM mode, described below, and may be selected by a user of the algorithm. Alternatively, Template(n) may be generated by the user choosing a group of ECG signals from a selected single heartbeat, and using the TM mode to generate the time pattern which then becomes Template(n).

[0030] In some embodiments the value of $ref_Anno(t_i)$ provided by the processor is derived from an external input provided from a user of the algorithm. In alternative embodiments, the processor estimates the value of $ref_Anno(t_i)$ automatically. The automatic estimation is typically by the processor receiving a stream of channel annotations from wave front annotation block 26, slicing the stream into groups, each group corresponding to a heartbeat, and estimating $ref_Anno(t_i)$ as one of an average, a weighted average, or a median, of the channel annotations of the groups in the stream.

[0031] In the initial step the processor also provides block 22 with values of CS unipolar annotations. The annotations are continually calculated using the wave front algorithm of block 26, and from the stream of the annotations the processor selects a group for a single heartbeat according to the time interval ($\{ref_Anno(ti)-\tau1WOI, ref_Anno(ti)+\tau2WOI\}$).

[0032] In a similarity step 34 the processor calculates the time pattern for the current group, as described above in section 2. The calculation gives a k -dimensional vector for the time pattern. The processor then estimates a similarity of the current group to the pre-set template ($Template(n)$) received in step 30. The similarity is determined by the following formula:

$$s_n(t_i) = \frac{1}{M} \left(\sum_m^M [dT(m, t_i) - dT(m, n)]^2 \right)^{0.5} \quad (2)$$

where $s_n(t_i)$ is a value of the similarity between the calculated time pattern $\{dT(k,ti)\}$ and the vector corresponding to Template(n) $\{dT(k,n)\}$, and

M is the number of channels in the group of annotations received in step 30. In some embodiments not all channels provide annotations, so that $M \leq K$.

[0033] In a decision step 38 the processor checks if $s_n(t_i)$ is less than a pre-set threshold, typically in a range of approximately 0.5 - approximately 1.2, although it may be larger or smaller than this range. In this case the decision returns true and the processor recognizes that this group belongs to Template(n), and proceeds to a buffer storage step 42. As is described below with reference to Fig. 6, the processor then presents the result of the identified template on display 18. The flowchart then returns to step 30 to receive a group of annotations for a subsequent heartbeat.

[0034] If decision step 38 returns false the flowchart returns to step 30 and the processor processes a new group of values of CS unipolar annotations.

[0035] Fig. 5 is a flowchart illustrating steps of the TM mode, according to an embodiment of the present invention. Unlike the template tracking mode, the template matching mode doesn't get a template as an input parameter. As shown in Fig. 5, in the TM mode the processor repeats steps 30 and 34 of the TT mode, as described above. In a decision step

68 the TM mode seeks matching between a current time pattern and all templates that have been found before. If step 68 returns false, i.e., if the processor cannot match a template to the current pattern, then in a new template step 76 it opens a new template using the current time pattern, and the new template may be presented on display 18 (described below with reference to Fig. 6).

[0036] If the matching is recognized, i.e., if the processor is able to match a template to the current pattern, then in a recalculation step 72 the selected template may be re-calculated to reflect a new member of a cluster of time patterns used to generate the template. The recalculation typically comprises incorporating the values found in step 72 into the calculation of the time pattern by averaging values of $dT(k,n)$ for a number of the groups in the cluster. In some embodiments the recalculation is only performed for the first q members in the cluster, where q may be approximately 10.

[0037] Fig. 6 is a schematic graph presented on display 18, according to an embodiment of the present invention. As explained above with reference to step 42, identified templates may be presented on display 18 as a graph 24 (Fig. 1). Graph 24 plots template number vs. group of annotations number, and the group of annotations number corresponds to a timeline of the heartbeats received. As shown in the graph approximately 430 groups have been analyzed, corresponding to the same number of heartbeats. As is also illustrated in the graph, most heartbeats of the timeline are classified as Template 2, but some heartbeats are classified as Template 1 and some are classified as Template 3.

[0038] Fig. 7 illustrates a correlation between a template and a group of annotations, according to an embodiment of the present invention. The figure is a graph of channel number vs. dT for a template based on heartbeat 412, the solid line, and for a group of annotations from heartbeat 463, the broken line, and illustrates the close similarity between the template and the group of annotations being analyzed.

[0039] Pairs of graphs such as those illustrated in Fig. 7 typically depict a situation where two heartbeats originate from the same region in the heart.

[0040] Fig. 8 illustrates an anti-correlation between a template and a group of annotations, according to an embodiment of the present invention. The figure illustrates how a group of annotations from heartbeat 123, the broken line, does not correlate with the template based on heartbeat 412, the solid line. Rather, since the slopes of the two graphs have opposite signs, there is an anti-correlation between the template and the group of annotations being analyzed.

[0041] Pairs of graphs such as those illustrated in Fig. 8 typically occur where two heartbeats originate from two regions in the heart that are separated from each other. For example, such a situation may occur when one region is in the right atrium, and the other region is in the left atrium.

[0042] A cardiac electrophysiological map, such as a map of LAT in the heart chambers, is typically produced by acquiring sets of ECG signals, and incorporating results of the signals, i.e., measured LATs, into the map. However, the sets of ECG signals typically include signals having more than one template, and this leads to inaccuracies in the produced map.

[0043] Embodiments of the present invention enable the different sets of signals to be separated into subsets, each subset corresponding to a different template. Each subset may be used to construct a respective LAT map of the heart. Thus, returning to Fig. 6, for the three different templates shown in the graph, the acquired signals may be separated into three different subsets, and a map produced for each subset. Typically the different subsets, each for a different template, correspond to different types of arrhythmia.

[0044] It will also be appreciated that by analyzing sets of ECG signals as templates, as has been described above, embodiments of the present invention may be used to monitor for a change in arrhythmia, since an arrhythmia change corresponds to a change in template.

[0045] It will be appreciated that the embodiments described above are cited by way of example, and that the present invention is not limited to what has been particularly shown and described hereinabove. Rather, the scope of the present invention includes both combinations and subcombinations of the various features described hereinabove, as well as variations and modifications thereof which would occur to persons skilled in the art upon reading the foregoing description and which are not disclosed in the prior art.

[0046] Aspects of the invention:

1. A method, comprising:

receiving a first group of electrocardiograph (ECG) signals derived from a single heartbeat and generated at a respective plurality of electrodes on a catheter in a heart of a subject;
 formulating a template relating times of annotations of the first group of the ECG signals, and assigning the template an index;
 receiving a second group of ECG signals derived from a subsequent single heartbeat and generated at the plurality of electrodes;
 calculating times of annotations of the second group of ECG signals;
 formulating a comparison between the template and the times of annotations of the second group; and
 when the comparison indicates that the times of annotations of the second group correspond to the template,

assigning the index to the second group of ECG signals, and presenting graphically on a display an occurrence of the template relative to a timeline representing heartbeats from the heart.

2. The method according to aspect 1, and comprising using the first group and the second group to formulate a common map of the heart.

3. The method according to aspect 1, and further comprising, when the comparison indicates that the times of annotations of the second group do not correspond to the template, formulating a further template relating the times of annotations of the second group of the ECG signals, and assigning the further template a further index, and presenting graphically on the display a further occurrence of the further template relative to the timeline.

4. The method according to aspect 3, and comprising using the first group to formulate a first map of the heart, and the second group to formulate a second map, different from the first map of the heart.

5. The method according to aspect 1, and comprising receiving a stream of channel annotations, slicing the stream into segments corresponding to respective heartbeats, estimating a reference annotation as one of an average, a weighted average, or a median, of the channel annotations of the segments in the stream, and applying the reference annotation in formulating the template.

6. The method according to aspect 5, wherein the template comprises differences between the times of annotations of the first group with the reference annotation.

7. The method according to aspect 1, wherein the catheter is located in a coronary sinus of the heart.

8. The method according to aspect 1, wherein the plurality of electrodes are evenly spaced along the catheter.

9. The method according to aspect 1, wherein the catheter is linear.

10. The method according to aspect 1, wherein the template is assigned to a first type of arrhythmia, the method further comprising receiving a subsequent group of ECG signals, and monitoring if the times of annotations of the subsequent group do not correspond to the template, thus indicating that the subsequent group of ECG signals corresponds to a second type of arrhythmia, different from the first type.

Claims

1. Apparatus, comprising:

a catheter, located in a heart of a subject and configured to:

receive a first group of electrocardiograph (ECG) signals derived from a single heartbeat and generated at a respective plurality of electrodes on the catheter, and
receive a second group of ECG signals derived from a subsequent single heartbeat and generated at the plurality of electrodes;

a processor configured to:

formulate a template relating times of annotations of the first group of the ECG signals, and assign the template an index,
calculate times of annotations of the second group of ECG signals,
formulate a comparison between the template and the times of annotations of the second group, and
when the comparison indicates that the times of annotations of the second group correspond to the template, assign the index to the second group of ECG signals; and

a display configured to present graphically an occurrence of the template relative to a timeline representing heartbeats from the heart.

2. The apparatus according to claim 1, wherein the processor is configured to use the first group and the second group

to formulate a common map of the heart.

- 5 **3.** The apparatus according to claim 1, and further comprising, when the comparison indicates that the times of annotations of the second group do not correspond to the template, the processor being configured to formulate a further template relating the times of annotations of the second group of the ECG signals, and to assign the further template a further index, and to present graphically on the display a further occurrence of the further template relative to the timeline.
- 10 **4.** The apparatus according to claim 3, and comprising using the first group to formulate a first map of the heart, and the second group to formulate a second map, different from the first map of the heart.
- 15 **5.** The apparatus according to claim 1, and comprising configuring the processor to receive a stream of channel annotations, slice the stream into segments corresponding to respective heartbeats, estimate a reference annotation as one of an average, a weighted average, or a median, of the channel annotations of the segments in the stream, and apply the reference annotation in formulating the template.
- 20 **6.** The apparatus according to claim 5, wherein the template comprises differences between the times of annotations of the first group with the reference annotation.
- 7.** The apparatus according to claim 1, wherein the catheter is located in a coronary sinus of the heart.
- 8.** The apparatus according to claim 1, wherein the plurality of electrodes are evenly spaced along the catheter.
- 25 **9.** The apparatus according to claim 1, wherein the catheter is linear.
- 10.** The apparatus according to claim 1, wherein the template is assigned to a first type of arrhythmia, and wherein the processor is configured to receive a subsequent group of ECG signals, and monitor if the times of annotations of the subsequent group do not correspond to the template, thus indicating that the subsequent group of ECG signals corresponds to a second type of arrhythmia, different from the first type.

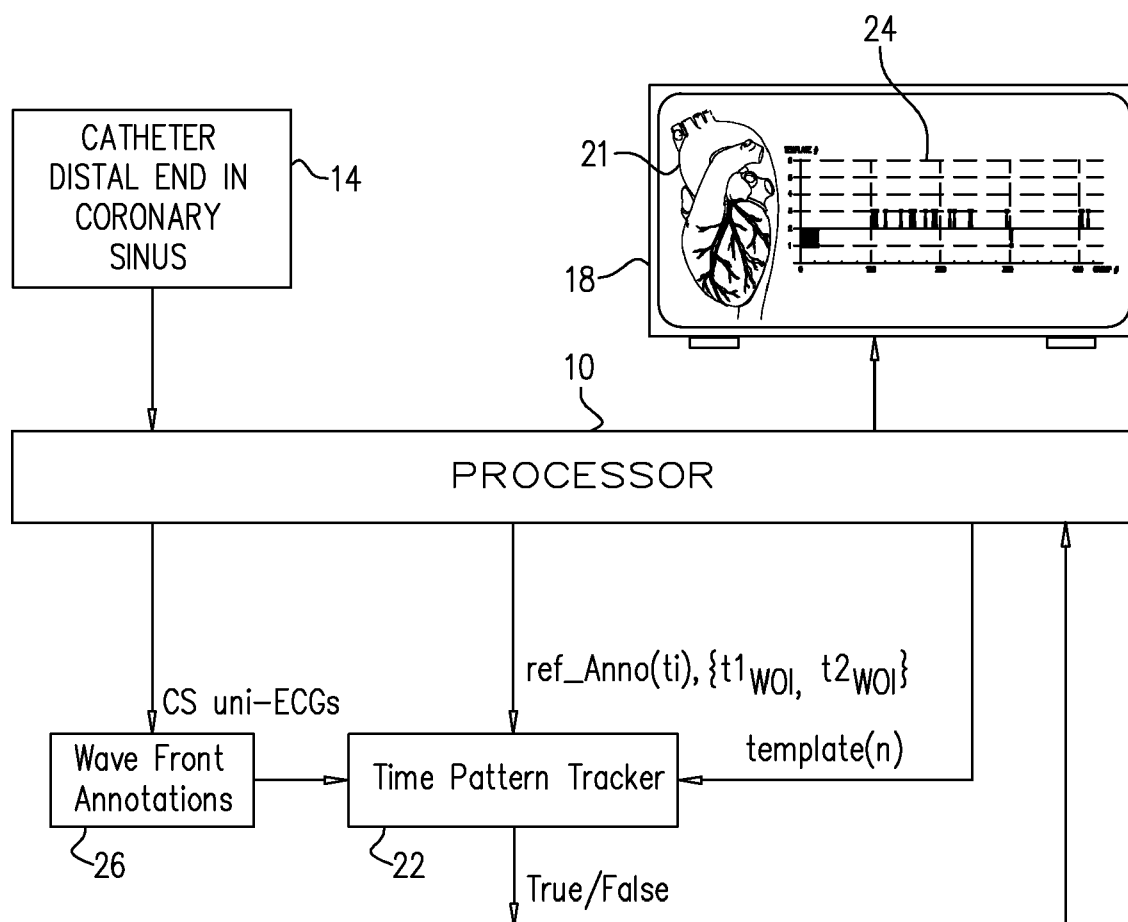


FIG. 1

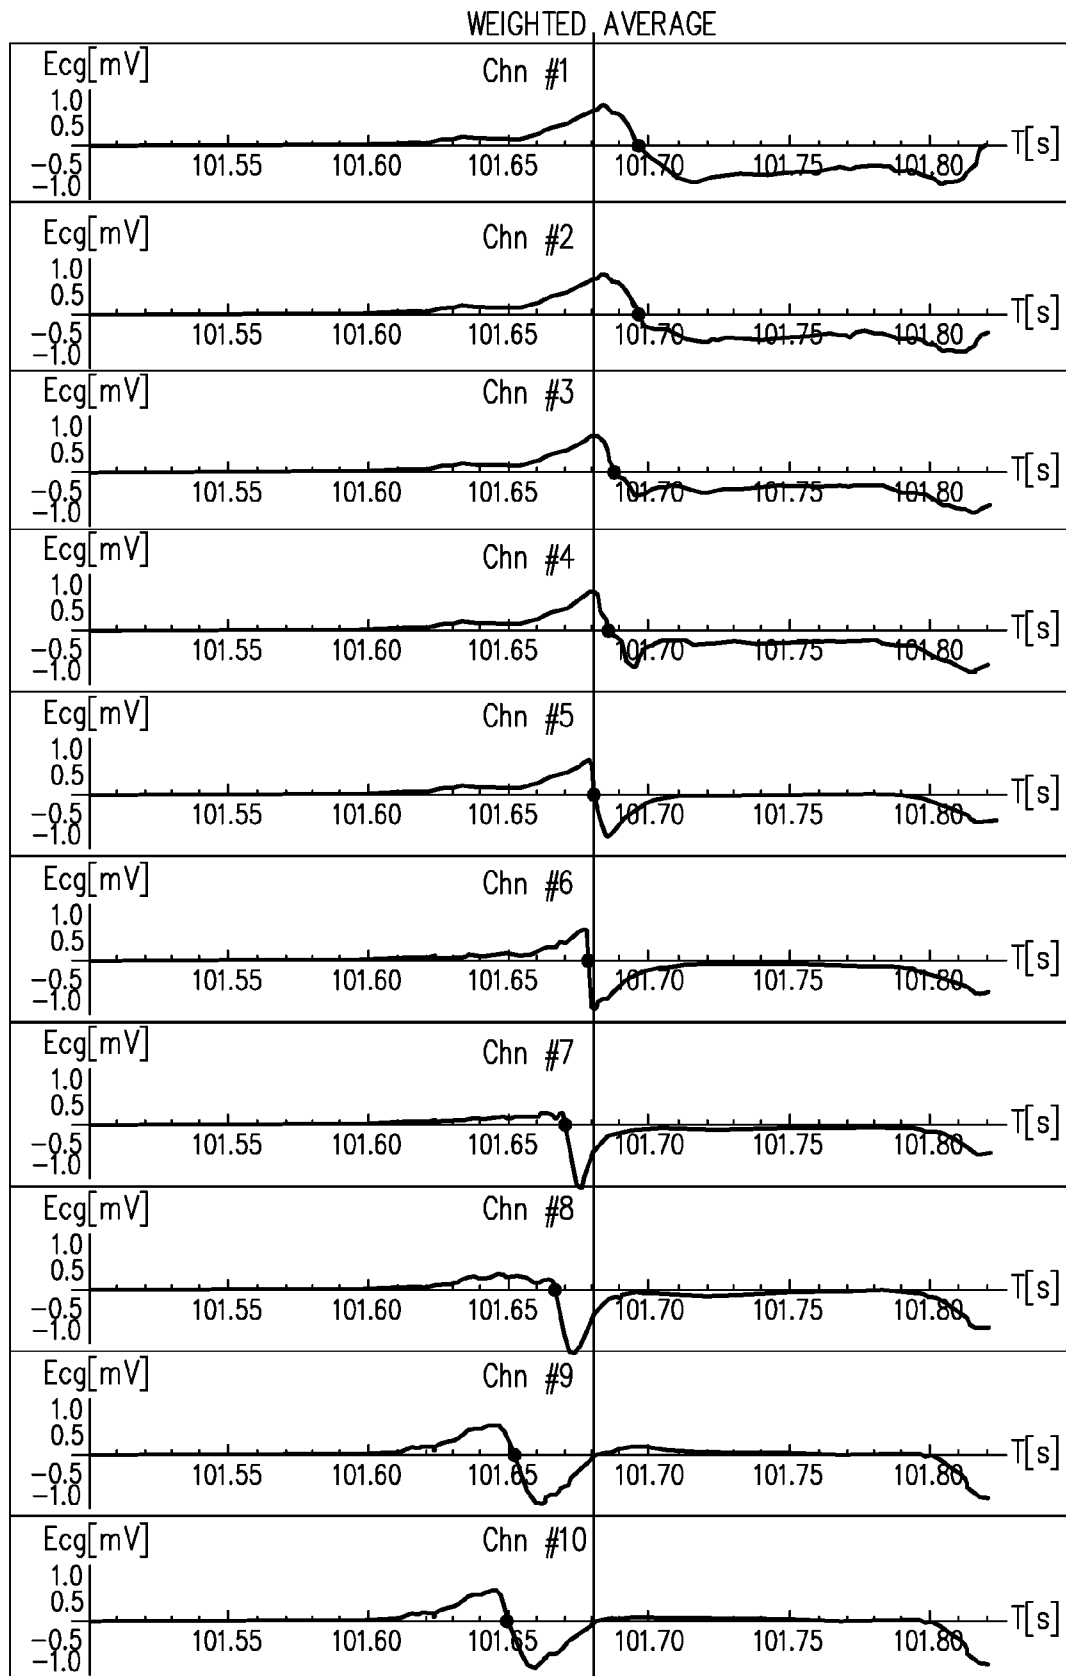


FIG. 2

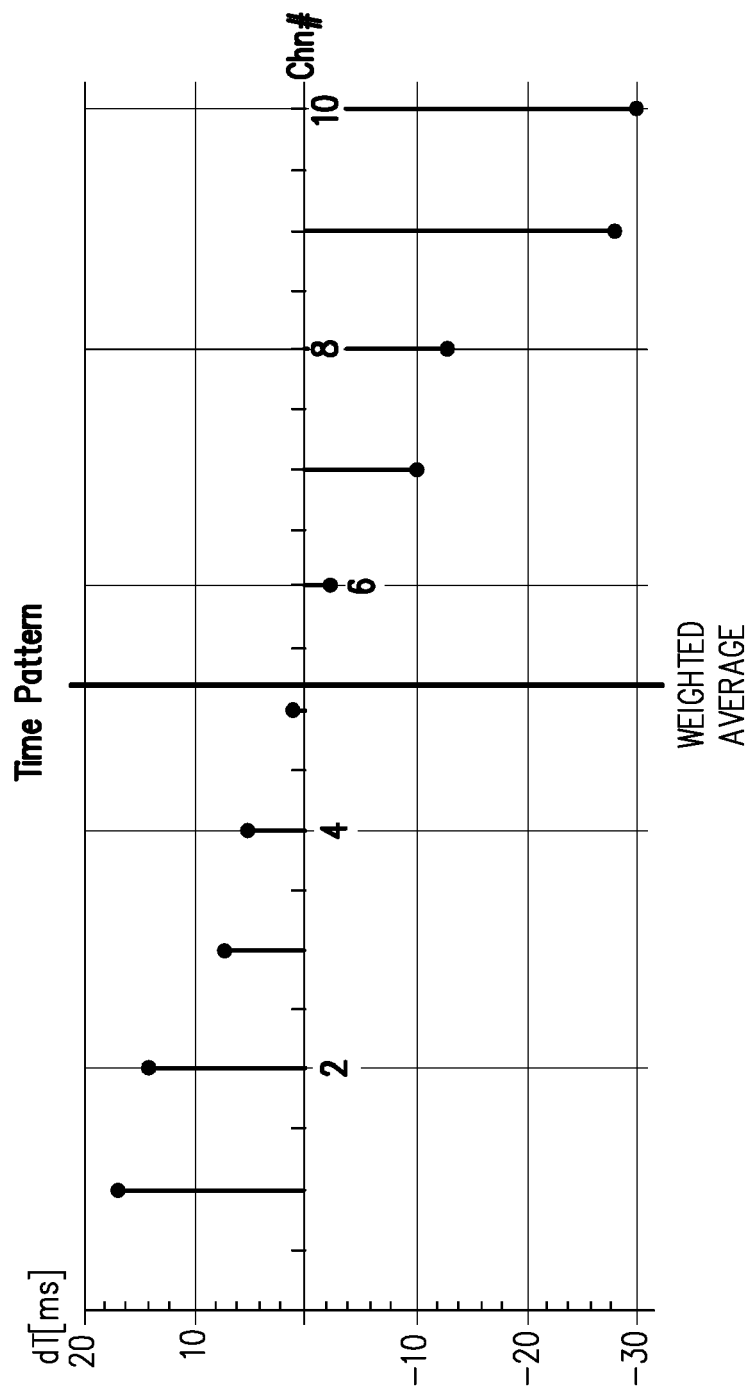


FIG. 3

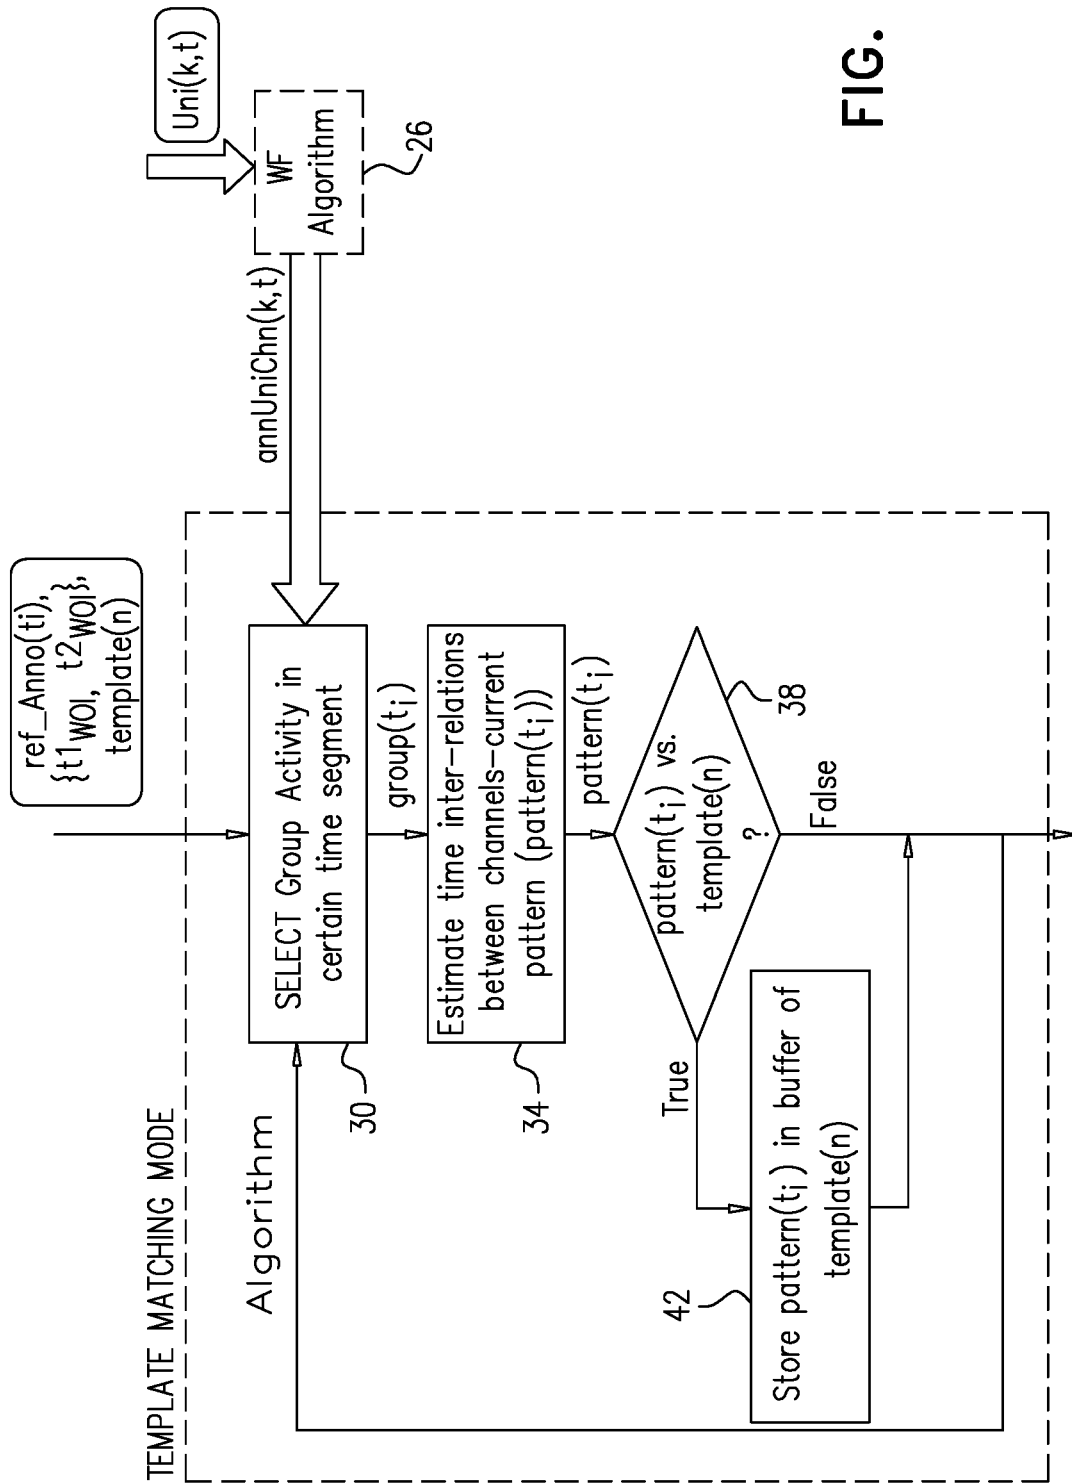


FIG. 4

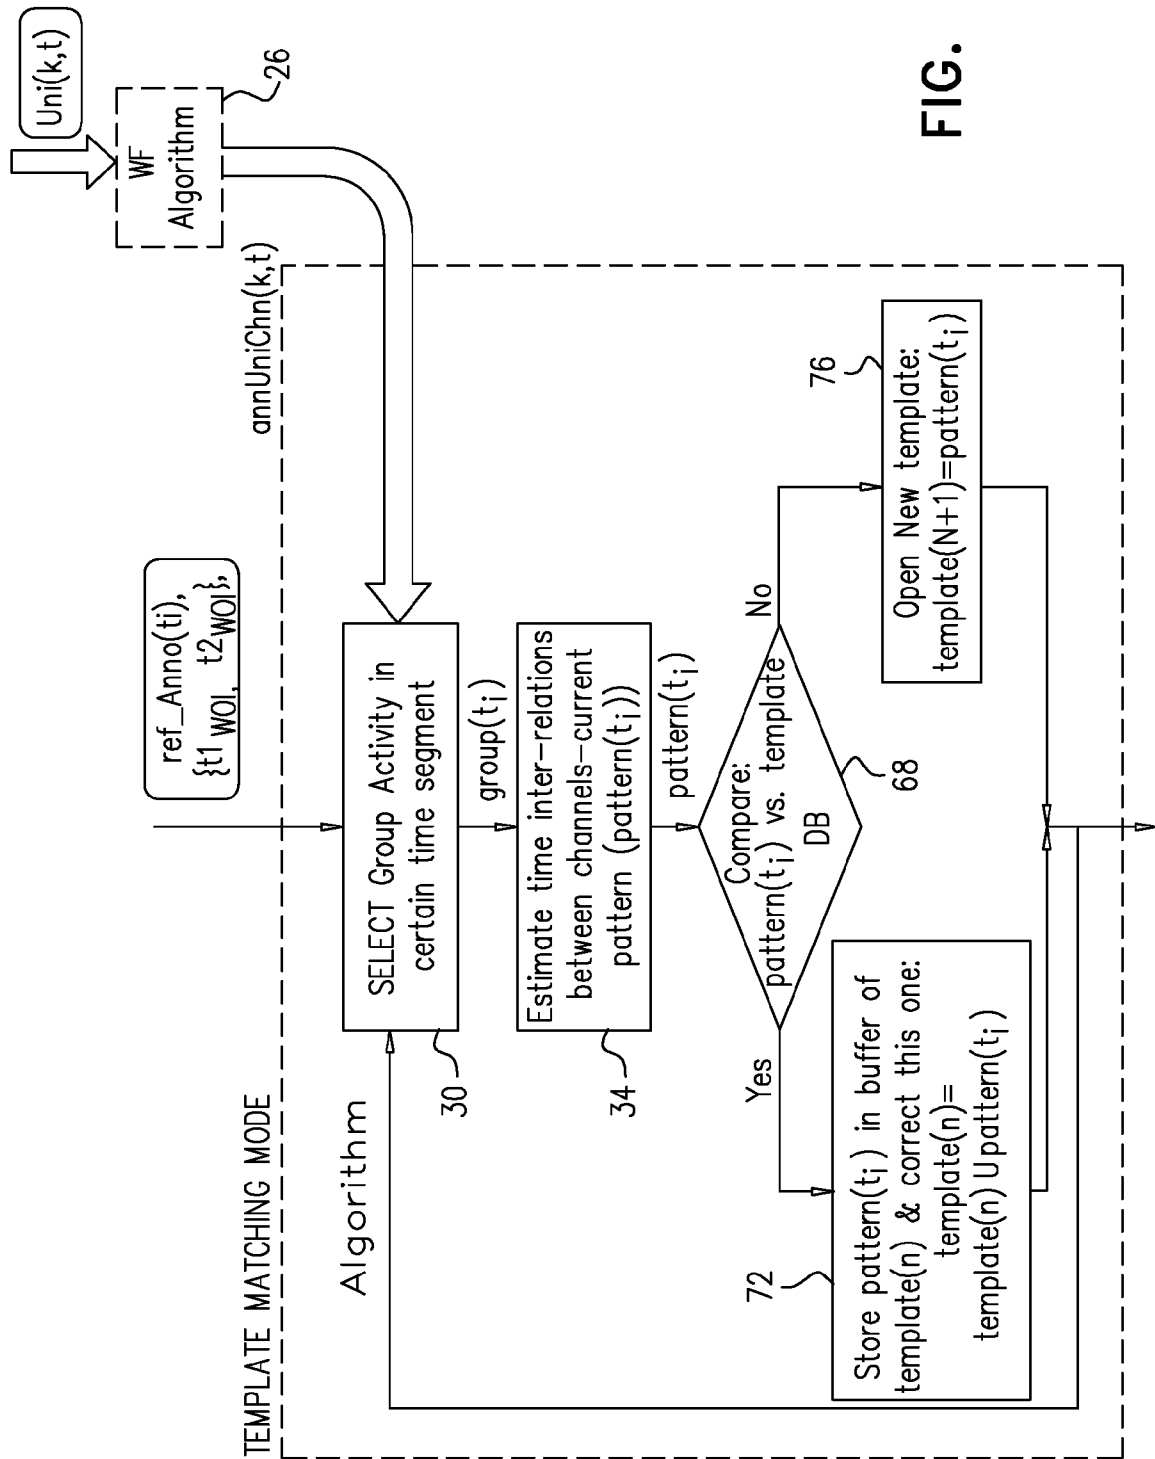


FIG. 5

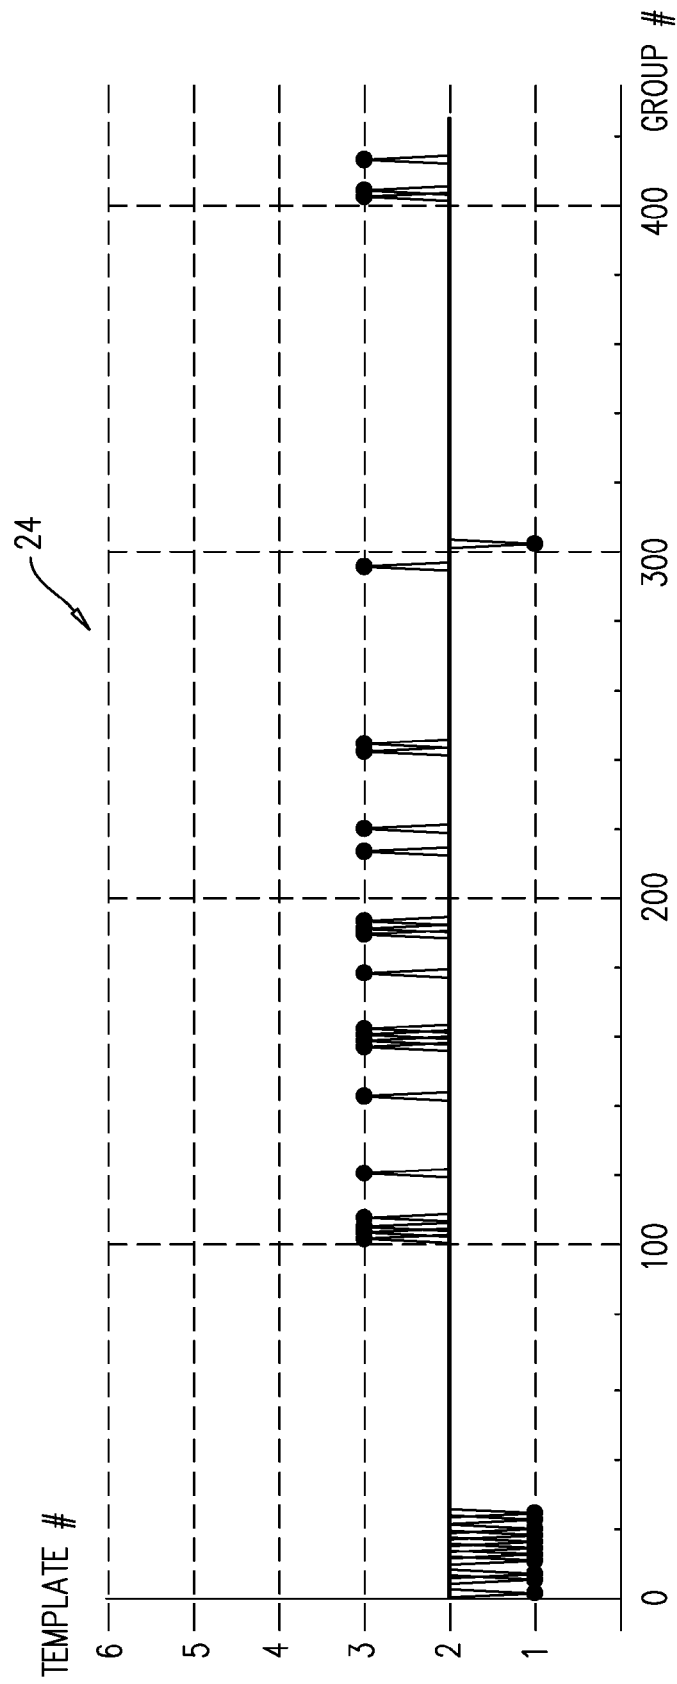


FIG. 6

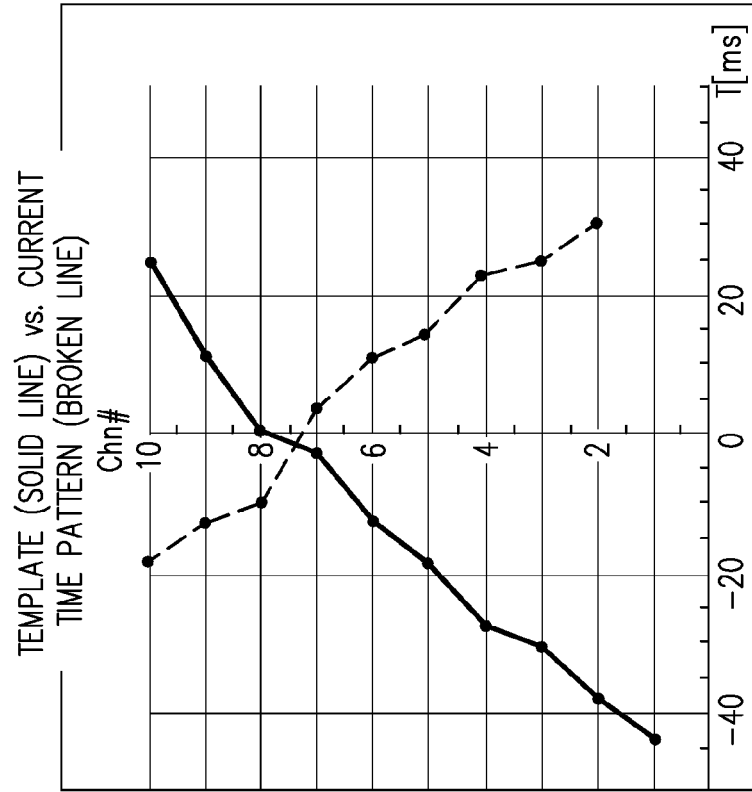


FIG. 7

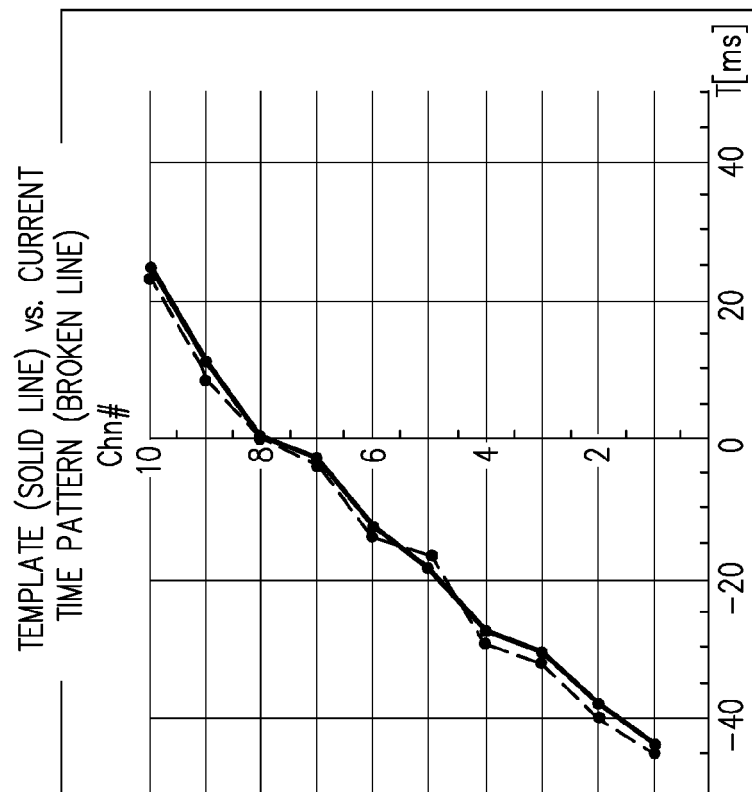


FIG. 8



EUROPEAN SEARCH REPORT

Application Number
EP 16 18 3500

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2005/137485 A1 (CAO JIAN [US] ET AL) 23 June 2005 (2005-06-23) * paragraphs [0005], [0017] - [0021], [0025], [0026], [0044], [0047], [0054], [0082] * * figures 1, 5-7 *	1-10	INV. A61B5/0452 A61B5/0464 A61B5/042
A	WO 2014/174274 A1 (IMP INNOVATIONS LTD [GB]) 30 October 2014 (2014-10-30) * figures 1-3 *	2,4	ADD. A61B5/046 A61B5/00
A	US 5 545 186 A (OLSON WALTER H [US] ET AL) 13 August 1996 (1996-08-13) * column 16, line 47 - line 62 * * figures 1, 2, 11 *	2,4	
A	WO 01/03578 A2 (CARDIAC PACEMAKERS INC [US]) 18 January 2001 (2001-01-18) * abstract * * page 12, line 15 - line 20 *	6	
A	US 2004/019366 A1 (ROTTENBERG WILLIAM B [US] ET AL) 29 January 2004 (2004-01-29) * figure 2 *	8,9	TECHNICAL FIELDS SEARCHED (IPC) A61B
A	US 2006/161069 A1 (LI DAN [US]) 20 July 2006 (2006-07-20) * the whole document *	1-10	
A	US 2014/343388 A1 (THAKUR PRAMODSINGH H [US] ET AL) 20 November 2014 (2014-11-20) * the whole document *	1-10	
A	US 2009/112106 A1 (ZHANG HONGXUAN [US]) 30 April 2009 (2009-04-30) * the whole document *	1-10	
		-/--	
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 4 January 2017	Examiner Meyer, Wolfgang
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03/02 (P04C01)



EUROPEAN SEARCH REPORT

Application Number
EP 16 18 3500

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	US 2014/180051 A1 (THAKUR PRAMODSINGH H [US] ET AL) 26 June 2014 (2014-06-26) * the whole document *	1-10	
A	US 6 477 406 B1 (TURCOTT ROBERT [US]) 5 November 2002 (2002-11-05) * the whole document *	1-10	
			TECHNICAL FIELDS SEARCHED (IPC)
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 4 January 2017	Examiner Meyer, Wolfgang
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03/02 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 16 18 3500

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

04-01-2017

10

15

20

25

30

35

40

45

50

55

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2005137485 A1	23-06-2005	US 2005137485 A1	23-06-2005
		US 2007276276 A1	29-11-2007
WO 2014174274 A1	30-10-2014	EP 2988664 A1	02-03-2016
		US 2016073913 A1	17-03-2016
		WO 2014174274 A1	30-10-2014
US 5545186 A	13-08-1996	AU 695634 B2	20-08-1998
		AU 5429996 A	16-10-1996
		CA 2215899 A1	03-10-1996
		DE 69626227 D1	20-03-2003
		DE 69626227 T2	13-11-2003
		DE 69632601 D1	01-07-2004
		DE 69632601 T2	23-06-2005
		EP 0939660 A1	08-09-1999
		EP 1179355 A1	13-02-2002
		JP 3768535 B2	19-04-2006
		JP H11503038 A	23-03-1999
		JP 2006068549 A	16-03-2006
		US 5545186 A	13-08-1996
		US 5855593 A	05-01-1999
		US 5991656 A	23-11-1999
		US 6141581 A	31-10-2000
		US 6259947 B1	10-07-2001
		US 2001034538 A1	25-10-2001
		US 2003125772 A1	03-07-2003
		WO 9630081 A1	03-10-1996
WO 0103578 A2	18-01-2001	AT 282986 T	15-12-2004
		AU 6348800 A	30-01-2001
		DE 60016276 D1	30-12-2004
		DE 60016276 T2	02-03-2006
		EP 1241977 A2	25-09-2002
		US 6449503 B1	10-09-2002
		US 2003060849 A1	27-03-2003
		US 2005159781 A1	21-07-2005
		US 2009312811 A1	17-12-2009
		US 2012046566 A1	23-02-2012
		WO 0103578 A2	18-01-2001
US 2004019366 A1	29-01-2004	NONE	
US 2006161069 A1	20-07-2006	US 2006161069 A1	20-07-2006
		US 2009005826 A1	01-01-2009
		US 2012310102 A1	06-12-2012

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 16 18 3500

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

04-01-2017

10

15

20

25

30

35

40

45

50

55

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2014343388 A1	20-11-2014	CN 105228510 A	06-01-2016
		EP 2996550 A1	23-03-2016
		JP 2016518217 A	23-06-2016
		US 2014343388 A1	20-11-2014
		WO 2014185977 A1	20-11-2014

US 2009112106 A1	30-04-2009	NONE	

US 2014180051 A1	26-06-2014	CN 104883969 A	02-09-2015
		EP 2934312 A1	28-10-2015
		JP 2016501640 A	21-01-2016
		US 2014180051 A1	26-06-2014
		WO 2014100464 A1	26-06-2014

US 6477406 B1	05-11-2002	NONE	

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 62203422 A [0001]
- US 20150208938 A, Houben [0004] [0023]

专利名称(译)	匹配和跟踪心脏激活的时间序列		
公开(公告)号	EP3130285A1	公开(公告)日	2017-02-15
申请号	EP2016183500	申请日	2016-08-10
[标]申请(专利权)人(译)	韦伯斯特生物官能(以色列)有限公司		
申请(专利权)人(译)	生物传感韦伯斯特 (以色列) LTD.		
当前申请(专利权)人(译)	生物传感韦伯斯特 (以色列) LTD.		
[标]发明人	RUBINSTEIN VLADIMIR BAR TAL MEIR		
发明人	RUBINSTEIN, VLADIMIR BAR-TAL, MEIR		
IPC分类号	A61B5/0452 A61B5/0464 A61B5/042 A61B5/046 A61B5/00		
CPC分类号	A61B5/04012 A61B5/0402 A61B5/0422 A61B5/04525 A61B5/0464 A61B5/6852 A61B5/6869 A61B5/72 A61B5/046 A61B5/7246 A61B2505/05 A61B5/044		
审查员(译)	MEYER , WOLFGANG		
优先权	62/203422 2015-08-11 US 15/206418 2016-07-11 US		
外部链接	Espacenet		

摘要(译)

一种方法，包括：接收从单个心跳导出的并且在对象的心脏中的导管上的相应多个电极处生成的第一组心电图（ECG）信号，公式化与所述第一组的注释的时间相关的模板所述ECG信号，以及向所述模板分配索引。该方法还包括接收从随后的单个心跳导出的并且在电极处生成的第二组ECG信号，计算第二组的注释的时间，形成模板与第二组的注释的时间之间的比较，当所述比较指示所述第二组的注释的时间对应于所述模板时，将所述索引分配给所述第二组ECG信号，以及在显示器上图形地呈现所述模板相对于表示来自所述心脏的心跳的时间线的发生。



(11)
EP 3 130 285 A1

(12)
EUROPEAN PATENT APPLICATION

(43)
Date of publication:
15.02.2017 Bulletin **2017/07**
(21) Application number: **16183500.4**
(22) Date of filing: **10.08.2016**
(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IT LI LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
DA ME
Designated Validation States:
MA MD
(30) Priority: **11.08.2015 US 20150220322 P**
11.07.2016 US 201615206418
(54)
MATCHING AND TRACKING TIME SEQUENCES OF HEART ACTIVATION
(57) A method, including: receiving a first group of electrocardiograph (ECG) signals derived from a single heartbeat and generated at a respective plurality of electrodes on a catheter in a heart of a subject; formulating a template relating times of annotations of the first group of the ECG signals; and assigning the template an index. The method further includes receiving a second group of ECG signals derived from a subsequent single heartbeat and generated at the electrodes; calculating times of annotations of the second group; formulating a comparison between the template and the times of annotations of the second group; and, when the comparison indicates that the times of annotations of the second group correspond to the template, assigning the index to the second group of ECG signals; and presenting graphically on a display an occurrence of the template relative to a timeline representing heartbeats from the heart.

(51) Int. Cl.
A61B 5/0452 (2006.01)
A61B 5/0464 (2006.01)
A61B 5/046 (2006.01)
A61B 5/048 (2006.01)
(71) Applicant: **Biosense Webster (Israel) Ltd.**
2056717 Yokneam (IL)
(72) Inventors:
• **Rubinstein, Vladimir**
2056717 Yokneam (IL)
• **Bar-Tal, Meir**
2056717 Yokneam (IL)
(74) Representative: **Cartmada & Ranaford LLP**
One Southampton Row
London WC1B 5HA (GB)

EP 3 130 285 A1

Published by: Janssen, 75001 PARIS (FR)