



(12) **EUROPEAN PATENT APPLICATION**  
 published in accordance with Art. 153(4) EPC

(43) Date of publication:  
**23.01.2019 Bulletin 2019/04**

(51) Int Cl.:  
**A61B 5/0484** <sup>(2006.01)</sup> **A61B 5/00** <sup>(2006.01)</sup>  
**A61B 5/16** <sup>(2006.01)</sup> **G06F 19/00** <sup>(2019.01)</sup>  
**A61B 5/05** <sup>(2006.01)</sup>

(21) Application number: **17765600.6**

(22) Date of filing: **17.03.2017**

(86) International application number:  
**PCT/BR2017/050062**

(87) International publication number:  
**WO 2017/156613 (21.09.2017 Gazette 2017/38)**

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**  
 Designated Extension States:  
**BA ME**  
 Designated Validation States:  
**MA MD**

(72) Inventors:  
 • **ABRAMOV, Dimitri, Marques**  
**20261-120 Rio de Janeiro - RJ (BR)**  
 • **GALHANONE, Paulo, Ricardo**  
**21930-290 Rio de Janeiro - RJ (BR)**  
 • **LIMA, Marcos, Antonio, Dias**  
**23050-070 Rio de Janeiro - RJ (BR)**  
 • **MARTINS, Carlos, Henrique, Quintanilha**  
**20521-050 Rio de Janeiro - RJ (BR)**

(30) Priority: **18.03.2016 BR 102016060109**


(74) Representative: **Lavoix**  
**Bayerstrasse 83**  
**80335 München (DE)**

(71) Applicant: **Fundação Oswaldo Cruz**  
**21045-900 Rio de Janeiro, RJ (BR)**

(54) **MODULAR APPARATUS AND METHOD FOR THE ANALOGOUS SYNCHRONISATION OF ELECTROENCEPHALOGRAMS WITH LUMINOUS EVENTS, OSCILLATORY EVENTS OF ELECTRICAL NATURE, AND MOTOR BEHAVIOUR EVENTS**

(57) This invention relates to a device that is intended to synchronize electroencephalograms (EEGs), recorded by any digital equipment, to physical events (sensorial, visual or auditory stimuli) and behavioral events (motor response, vocal response), in order to allow EEG signal mediation for the purpose of visualizing Evoked Potentials or Event-Related Potentials, which are important research subjects in the neurosciences and clinical investigations into neurological and psychiatric pathologies. This invention allows any digital EEG device to be transformed into equipment that can record Evoked Potentials. This invention also provides a method for analog synchronization of EEGs with oscillating electric light-related events and motor behaviors.

FIGURE 6

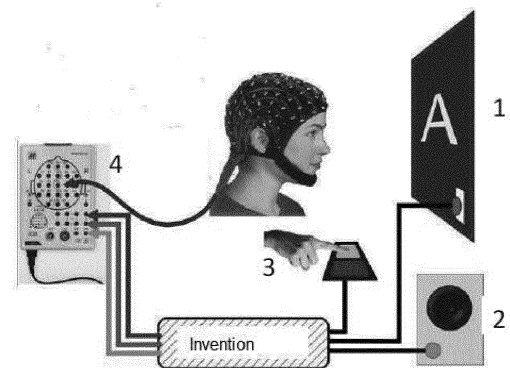

**Description**FIELD OF THE INVENTION

5 **[0001]** The device constituting this invention is intended to synchronize electroencephalograms (EEGs), recorded by any digital equipment, with physical events (sensorial, visual or auditory stimuli) and behavioral events (motor response, vocal response), thus allowing EEG signal mediation for the purpose of visualizing Evoked Potentials or Event-Related Potentials, which are important research subjects in the neurosciences and clinical investigations into neurological and psychiatric pathologies. This invention allows any digital EEG device to be transformed into equipment that can record  
10 Evoked Potentials. The invention also provides a method for the analog synchronization of EEGs with oscillating electric light-related events and motor behaviors.

BACKGROUND OF THE INVENTION

15 **[0002]** Evoked Potentials (PE) are electrophysiological responses evoked from the nervous system by a variety of events, such as endogenous cognitive processes or sensorial stimuli synchronized with a behavioral response. There are currently two alternative methodologies for materializing Evoked Potentials:

- 20 - using dedicated equipment for materializing Evoked Potentials (such as that made by the Nicolet®, Nihon Kohden® and Neurotec® manufacturers, for example). Despite the high quality of the tests that they produce, they are systems designed to provide medical care and with few stimulation protocols, hampering the customization of tests. Consequently, such equipment is of little use for research purposes. These items of equipment are extremely expensive (they are more costly than the electroencephalogram equipment made by the same manufacturers) and have few channels (average of four). Equipment prices rise steeply for more channels.
- 25 - Methodologies using digital electroencephalography equipment linked to computer systems, such as the following, for example:
  - 30 - Pscychotoolbox-MatLab®, CORTEX® and Presentation®. These computer systems produce stimulation protocols for obtaining Evoked Potentials, in parallel to a programmable trigger, synchronized with the events in these protocols, which is sent to the EEG equipment through an outlet port on the computer. These systems are feasible only for scientific research, for the following reasons: high complexity of these systems (for their installation, maintenance, operation and programming) which normally require a technician with professional qualifications, found only in laboratories with ample expertise; possibility of synchronization errors resulting from programming mistakes or even computer problems intrinsic to extremely complex operating systems (such as Windows®) that might adversely affect the accurate timing of software-hardware-EEG interactions. All these variables undermine the feasibility of  
35 using this methodology for medical care.

40 **[0003]** There is a need at the state of the art for the development of a definitive and innovative conceptual technology that can handle the materialization of Neurophysiology Event Protocols (Evoked Potentials) and ensuring: accurate synchronization of events and signals; procedures that are easy to perform; low costs; and universal access to Evoked Potential tests by countless electroencephalography units already in place or to be implemented

BACKGROUND OF THE INVENTION

45 **[0004]** This purpose of this invention is to provide accurate marking of stimuli presentation instants and responses to these stimuli in Neuroscience and Evoked Potentials research protocols for clinical neurophysiology, with no need for computer systems equipped with stimulation management applications.

**[0005]** This invention proposes a method and a method and a device that allows synchronization between sensorial stimuli and an electroencephalogram (EEG) in order to obtain Evoked Potentials.

50 **[0006]** The device resulting from this invention allows Event-Related Potentials (Evoked Potentials) to be obtained through using ordinary EEG equipment, through the transduction of the events submitted to the subject (or behavioral events) in an analog signal that synchronizes these events with the encephalographic recording, generating trustworthy latencies in the evoked potential wave.

55 **[0007]** The device resulting from this invention allows **synchronization of the electroencephalogram (EEG)** recorded by any digital equipment or through analog-digital conversion with **events**: (1) **light**, emitted by any source, such as the sun, liquid-crystal display (LCD), cathode-ray tube (CRT), cinematographic projections, all types of lamps and all types of light-emitting diodes (LEDs), in any color (wavelength) within the visible spectrum and at any intensity; (2) **electrical oscillations** at any frequency, voltage and current, deriving from (2.a) from the outlet of an analog or digital electronic sound source (electric signal outlet to loudspeakers, earphones or amplifiers, either monophonic or stereophonic); (2.b)

from a transduction device for another physical event into an electrical event (transducer of voltage, vibration, sound, pressure, temperature, humidity, flow or any biological events); (2.c.) From an electric signal conditioning device (amplifiers or transformers), (2.d) from a skin impedance measurement device, with or without reproduction of the respective electric signal to a parallel outlet; and (3) **behavioral motor responses** produced actively in all four limbs, either individually or in pairs, through activating switch devices; producing square electrical envelopment waves (i.e., triggers) whose lengths vary in order to demarcate the event in time, transmitting these triggers to the EEG equipment through its DC channels (at voltages between -5V and +5V) or AC (for example, -50mV a +50 mV), that are recorded on the electroencephalogram concomitantly with the biological signal.

**[0008]** Through the device constituting this invention, it is possible to produce EEG signal mediation for the purpose of visualizing Evoked Potentials or Event-Related Potentials, after the recording thereof, as a subject for neuroscience research and clinical investigations of neurological and psychiatric pathologies. This invention allows any digital EEG device to be transformed into equipment that can record Evoked Potentials.

**[0009]** Among the advantages of this invention, we may mention:

- with markings taken directly from the presented stimuli and the responses generated by patients, delays are fixed and known, defined only by the electronic signal spread times, which can thus be easily offset through software during the post-analysis stage;
- with the analog generation circuit of the trigger, the signal is already defined by being introduced directly into the DC or even AC channels;
- any digital EEG equipment may be used as off-line Evoked Potentials (ERP) equipment, which could make the use of medium and long latency Evoked Potentials more popular in neurological clinical practice, disseminating a low-cost safety technology for functional research into the nervous system (useful for monitoring patients with demyelinating diseases and diagnoses of visual tract lesions, for example); and,
- stimuli management applications are not required. Any software or even a sequence of stimuli recorded in a media file may be used for stimulation

**[0010]** This invention proposes a novel functional concept that lies in the analog synchronization of EEG signals with physical and behavioral events in order to obtain Evoked Potentials through a device linked to the EEG and external to this unit.

**[0011]** The device presented here exemplifies the implementation of the invention in question, as it allows Event-Related Potentials (Evoked Potentials) to be obtained through using ordinary digital EEG equipment by electronic manipulation of the events submitted to the subject (light stimuli transduced by photocell, or electrical oscillations deriving from sound equipment outlets, the transduction of other physical events, conditioning, biological signals or skin impedance measurements related to such events or behavioral events (motor responses of the upper and / or lower limbs) in an analog signal that synchronizes these events with the encephalographic recording, for easier examination of the exact evoked potential wave latencies, as the trigger markings are directly derived from analog processing of the presented stimuli and the responses generated by the patients. The delays inherent to analog processing time are set and known, defined only by the electronic signals spread time, which can thus be easily offset through software in the post-analysis stage. With the analog generation circuit of the trigger, the signal is already defined by being introduced directly into the DC or even AC channels. This means that any digital EEG equipment may be used for off-line processing of evoked potentials. As digital EEG equipment has a relatively low analog-digital conversion time (1000 points per second or less), only medium and long latency evoked potentials (greater than 50 ms) can be analyzed safely with this conventional equipment. We note that this methodology will be appropriate for detecting visual, medium-latency auditory and cognitive evoked potentials (endogenous, related to the motor responses), thus disseminating a safe and low-cost functional technology for examining the central nervous system during research activities as well as medical care (where it is very useful for monitoring patients with demyelinating diseases, visual system alterations evaluations and studies of the progression of cognitive diseases, for example); there is no need for very expensive dedicated equipment and computer systems with stimuli management applications. Any software may be used for stimulation or even a sequence of stimuli recorded in a media file.

#### BRIEF DESCRIPTION OF THE FIGURES

**[0012]**

**Figures 1A and 1B** offer a general schematic overview of the device constituting the invention in a preferred embodiment.

**Figures 2.1, 2.2 and 2.3** offer a schematic view of the necessary elements in the top and back panels of the standard device addressed by the invention, schematized with dashed lines showing the functional

- divisions of the system into modules.
- Figure 3** shows the button unit for the device addressed by the invention.
- Figure 4** conceptually demonstrates the function of the invention.
- Figure 5** shows the scheme in concept blocks for the functioning of the invention, which can be generalized or any circuit playing this role.
- Figure 6** is a representation of the modular device addressed by the invention.

#### DETAILED DESCRIPTION OF THE INVENTION

**[0013]** The basic elements of the device addressed by the invention are presented below.

**[0014]** The device constituting the invention is a **modular item of equipment**, with three types of function modules: a motor response processing module (A, as shown in **Figure 2.1**); electrical oscillation processing module (B, as shown in **Figure 2.1**); and the light processing module (C, as shown in **Figure 2.1**). Module D is the power feed and control module, containing the power switches, the power input and the voltage safety control (fuse), that distributes electricity to all three (or more) function modules.

**[0015]** A unit of the device constituting the invention may contain as many function modules as wished, in a customized manner. For example, two modules B, one module A and two modules C. As modules A and B have two input channels each, generating trigger waves at the outlet in a single channel, with different amplitude levels, which can indicate whether there was a response or the presence of a stimulus in one, the other or both module input channels.

**[0016]** In order to demonstrate the operations of this invention, a unit was set up for the device (described here) with three function modules (with 5 input channels and three output channels that together produce five individual response patterns), in the belief that much of the demand will be met with this configuration. Nevertheless, other configurations may be set up through arraying the function modules side-by-side on a single level (keeping the thickness of the device), with a single circuit board. Further explanations are presented in greater detail in the references for the **Figures**.

**[0017]** The numerical references in **Figure 1** represent a unit of the device constituting the invention with three modules, one of each type: A, B and C. Representing a preferred mode of the invention, **Figure 1** presents the following structural elements:

**(1) Housing Lid:** sheet made from metal or plastic material forming the top and sides of the outer housing of the device, with top openings for the 4a-c switches.

**(2) Housing Body:** composed of the outer front, back and lower parts of the housing with all the plugs and outlets of the device, and holding its circuit board. There are screws on the side of the body to hold the housing lid in place. There is a crossbar on the housing body along the length of the device, fixed to its sides, where the 4a-c selection switches are attached.

**(3) Button Unit:** composed of two buttons for entering motor responses.

**(4) a-c switches** that select voltage levels at the outlets for each outlook function module (a - motor response module; b - electrical oscillations module; and c - light detection module). If DC is selected, the output voltage varies between -5V and +5V (for entering the DC channels of the EEG equipment). If AC is selected, the output voltage varies between -50 and +50mV (for the AC channels of the EEG equipment, or for entering the EEG channel).

**(5) Power Source:** the device uses a regular power source with a switch, with an inflow of alternating current at 100-240V, 50-60Hz, and an outflow of continuous current at no more than 12V and 1000mA.

**(6) Threaded fuse port**

**(7) Power switch.**

**(8) Screws a-d: for attaching** the lid of the device to its body

**(9) Photocell input cable**

**(10) Suction cup:** the photocell is attached to a smooth surface (an LCD or CRT screen, for example) by a suction cup. When necessary, this allows the photocell to be attached to any other type of surface by any other means whatsoever, such as adhesive tape.

**(11) Photocell:** on the device, we use a broad-spectrum visible light energy uptake current-breaking photocell.

**(12) Function module trigger output tables:** these are the cables connecting to the DC and AC channels on the EEG equipment. The standard outlets on the embodied device are PI mono type. Many types of equipment use different connectors (such as RCA); in this case, adapters (*rabichos*) that are found easily on the market would be needed to use the device constituting the invention.

**(13) Electrical oscillations input table:** set up with a stereo P2 connector, in order to link directly into an audio outlet (speaker out) on many different types of equipment, ranging from computers to television sets, mp3 and DVD players, as the use of this module to synchronize sound stimuli will be the rule. In order to connect other devices, adapters may be needed or even signal adjusters (for electrical oscillations coming from sensors or other measurement devices/biological examinations).

[0018] **Figure 2.1** shows a schematic view of the top panel of the device addressed by the invention. The dashed lines represent imaginary divisions of the four modules constituting the preferred configuration, with three function modules (A: motor response module, B: electrical oscillations module, C: light detection module), and the power feed module (D), which constitutes the entire front part of the device, as shown in **Figure 1**. It is noted that the switches (corresponding to Switches 4a-c in **Figure 01**) of the respective modules define the output voltage range for each module: in the AC position, the voltage range is compatible with the standards for digital EEG devices (no more than 50mV to +50mV), and for the DC position, the voltage range is -5 a +5V. The arrows represent the number of inlets and outlets for each function module.

[0019] **Figure 2.2** shows a rear view of the device in a preferred embodiment (see **Figure 2.1**), containing the device signal inlets and outlets. All outlets are square waves with durations identical to the input signal, with ranges depending on whether they are intended for a DC or AC channel (defined by the position of Selector Switches 4a to c). Specifically, the elements in the **Figure** are:

(1) **Behavioral response inlet:** two single-reference channels that are connected to the button unit (see **Figure 3**) by a stereo connector (2 phases, 1 neutral).

(2) **Electrical oscillations inlet:** two single-reference input channels with a stereo connector (2 phases, 1 neutral), that detects oscillations at less than 100 Hz as individual events, and oscillations at more than 100Hz at a frequency compatible with most soundwaves, as a single event.

(3) **Photocell inlet**

(4) **Motor response module trigger outlet:** Pressing Button 1 (channel 1) produces a positive wave of +3V (+30mV if the AC option is selected on corresponding Switch 4 - see **Figure 1**); pressing Button 2 (channel 2) produces a positive wave of +2V (+20mV if the AC option is selected); while pressing both buttons simultaneously produces a positive wave of +5V(+50mV if the AC option is selected)

(5) **Electrical oscillation module trigger outlet:** detecting electrical oscillations events produces 2, 3 or 5V waves (20, 30 or 50mV for the respective AC options), for either the right, the left or both input channels during the event, which has a set response latency (measured between the peak of the first oscillation and maximum trigger voltage) of 4 mseg (four oscillations lasting 10 mseg or more), or 3 mseg (four oscillations lasting less than 10 mseg).

(6) **Electrical oscillation outlet:** a female stereo connector that reproduces the respective input signal from both channels. This is useful for signal sharing with another device or to activate a speaker (loudspeakers, earphones, etc).

(7) **Light module trigger outlet:** the light module produces a 5V trigger wave (50mV for the AC option), with latency set for a maximum voltage of 2mseg. On the threshold of inactivity, the maximum detection frequency for light pulses is 30Hz or more. For the xenon lamp flashes (color 6500 K, 30 cd/m<sup>2</sup>/W, pulse duration: 20 ps), the maximum detection frequency is 60Hz or more. For an LCD or CRT display operating at 60Hz (our standard), the maximum stimulation frequency is 30 Hz (one light cycle, one dark cycle). See **Figure 8**.

[0020] **Figure 2.3** provides a front view of the back of the device in a preferred embodiment, which has the controls and the module D input. Specifically, the elements in this **Figure** are:

(1) Threaded fuse port.

(2) Power switch.

(3) Power cable input: from the power source. (see **Figure 1**)

[0021] **Figure 3** shows a preferred button unit fitted to the device addressed by the invention. Each button is a channel (channel 1, left button; channel 2, right button). Note the output cable with a two-channel connector (stereo). The preferred button unit is lightweight (under 0.5 kg), with large buttons that are well adapted to use by the hands and big toes. A broader variation of this button unit may be implemented for behavioral responses with the feet.

[0022] **Figure 4** presents an illustration of the functional paradigms of the device addressed by this invention, for a general understanding of the functioning of the device. Using any application (software) or even a media file played on a media player (such as audio files or video files in formats such as \*.avi or \*.mp4, as shown in this **Figure**), the stimulation pattern is presented to the subject whose evoked potentials are being evaluated. With the stimulation pattern, a small area along the edges alternate between white and black (presence and absence of light, indicated by the straight arrow) depending on light reversals in the target pattern fields, synchronizing the alternation of these patterns through the light detection module. On the electroencephalogram, the device constituting this invention "marks" the moment of each reversal (see the curved arrows), in order to allow studies of the evoked potentials in terms of the visual stimulation provided by this reversed pattern. The dotted line with the square waves represents the figure signal, sent from the device through the DC channel (through which the trigger signal from the light detection model enters the EEG equipment), overlaid on the electroencephalogram. The unbroken line is the EEG readings.

[0023] **Figure 5:** presents the function block diagram of the invention:

Figure 5.A: describes the functioning of the motor response processing module. Pressing the right and/or left buttons on the button unit triggers the V1 and/or V2 voltage signal generator that, depending on the selector switch position, transmits in the form of square waves (with the same duration as the button is pressed) at voltages compatible with the DC or AC channels ( $\div 100$ ).

**[0024]** Figure 5-B: describes the functioning of the electrical oscillation processing module. The electrical signals that enter through channel 1 and / or channel 2 runs through enveloping detector that generates a V1 and / or V2 voltage signal that, depending on the selector switch position, transmits in the form of square waves (with the same duration as the electrical oscillations in the input channels) at voltages compatible with the DC or AC channels ( $\div 100$ ). In parallel, there is a repeat system sending signals in channel 1 and 2 to an electrical oscillation output.

**[0025]** Figure 5-C: describes the functioning of the light processing module. The electrical signal from the photocell runs through the threshold detector that generates a V1 voltage signal that, depending on the selector switch position, transmits in the form of square waves (with the same duration as the light signal activating the photocell) at voltages compatible with the DC or AC channels ( $\div 100$ ).

**[0026]** Figure 6 shows a representation with three modules of the modular device constituting the invention, in a preferred presentation, with one motor response processing module (3), one electrical oscillation processing module (2), and one light processing module (1). In the context of this Figure, we present a schematic diagram of the application of the device constituting the invention during the examination of a subject completing a test in which pictures are displayed (synchronized with the EEG [4] through the light processing module) and sounds (synchronized with the EEG through the electrical oscillation processing module), with the motor responses collected (and synchronized with the EEG) through the motor response processing module.

**[0027]** Consequently, so the device described here, it is possible to define and record markings taken directly from the presented stimuli and the responses generated by patients through only the electronic signal spread time.

**[0028]** Although the invention is described in details and refers to specific examples thereof, it will be clear to any specialist in this field that many changes and modifications may be made without moving away from its spirit and scope.

## Claims

1. MODULAR DEVICE FOR ANALOG ELECTROENCEPHALOGRAPHY SYNCHRONIZATION WITH OSCILLATING ELECTRICAL LIGHT-RELATED EVENTS, AND MOTOR BEHAVIORS **characterized in that** it comprises function modules of the following types:

motor response processing module; electrical oscillation processing module; and light processing module, whereby the device also contains a power feed and control module in which the power switches are located, as well as, the power input and voltage safety control (fuse), that distributes electricity to the above-mentioned function modules.

2. DEVICE according to Claim 1 **characterized in that** it contains as many function modules as desired.

3. DEVICE according to Claim 1 **characterized in that** motor response processing module has a device switch inlet with two mixed subchannels that respond with square waves when the switches are off.

4. DEVICE according to Claim 1 **characterized in that** the electrical oscillation processing module has an electrical oscillation inlet that is compatible with signals from standard audio channel outputs, which responds with square waves lasting as long as the oscillation.

5. DEVICE according to Claim 4 **characterized in that** the electrical oscillation processing module input makes provision for connecting specific transducers for physical events, such as temperatures, pressures or magnetic fields, and also for physiological events such as muscle activity, strength, skin conductance or ECG.

6. DEVICE according to Claim 1 **characterized in that** the light processing module has a photocell inlet photocell that detects light energy and responds with square waves corresponding to the duration of the light event.

7. METHOD FOR ANALOG SYNCHRONIZATION OF ELECTROENCEPHALOGRAPHY WITH OSCILLATING ELECTRICAL LIGHT-RELATED EVENTS, AND MOTOR BEHAVIORS, **characterized in that** it comprises the following stages:

uptake of physical light-type events, electrical oscillations and similar and/or behavioral type motor responses

**EP 3 430 997 A1**

from a subject; generation square wave trigger signal with the same duration as the recorded events; and, transmission of the trigger signal to the digital electroencephalogram through AC or DC channels.

5

10

15

20

25

30

35

40

45

50

55

FIGURE 1A

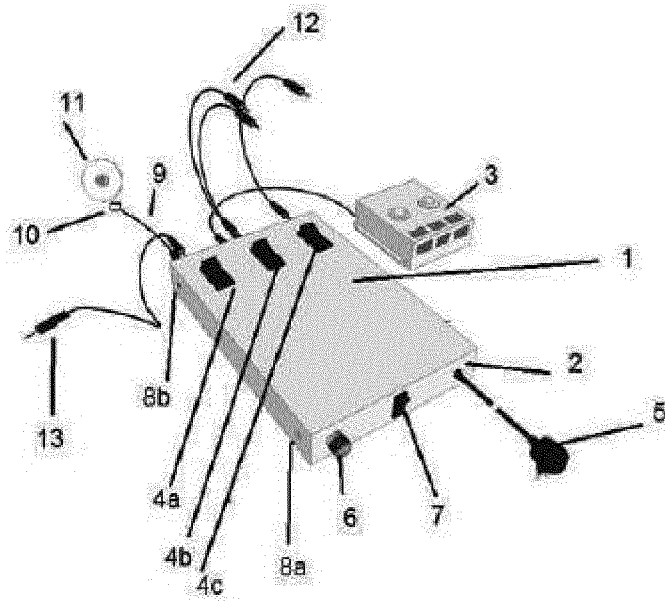


FIGURE 1B

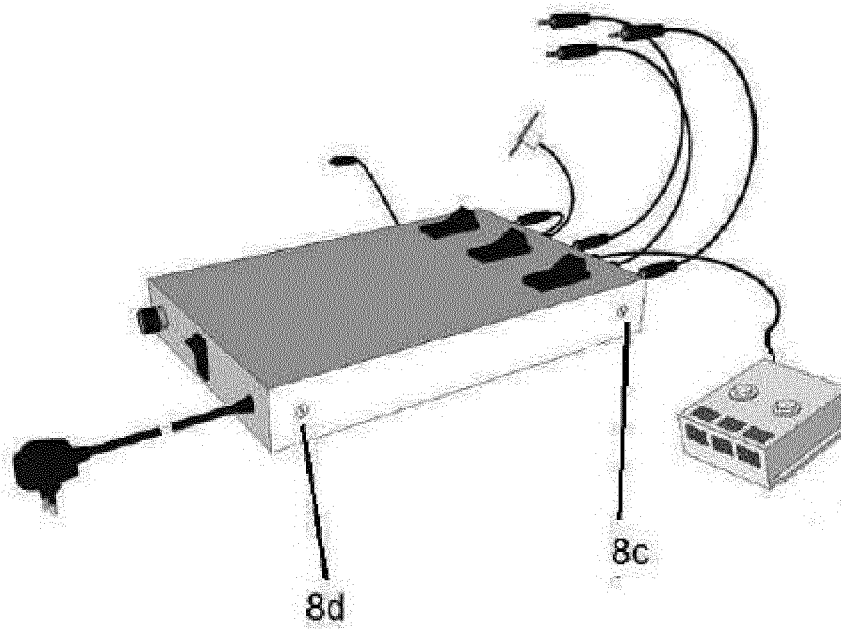


FIGURE 2.1

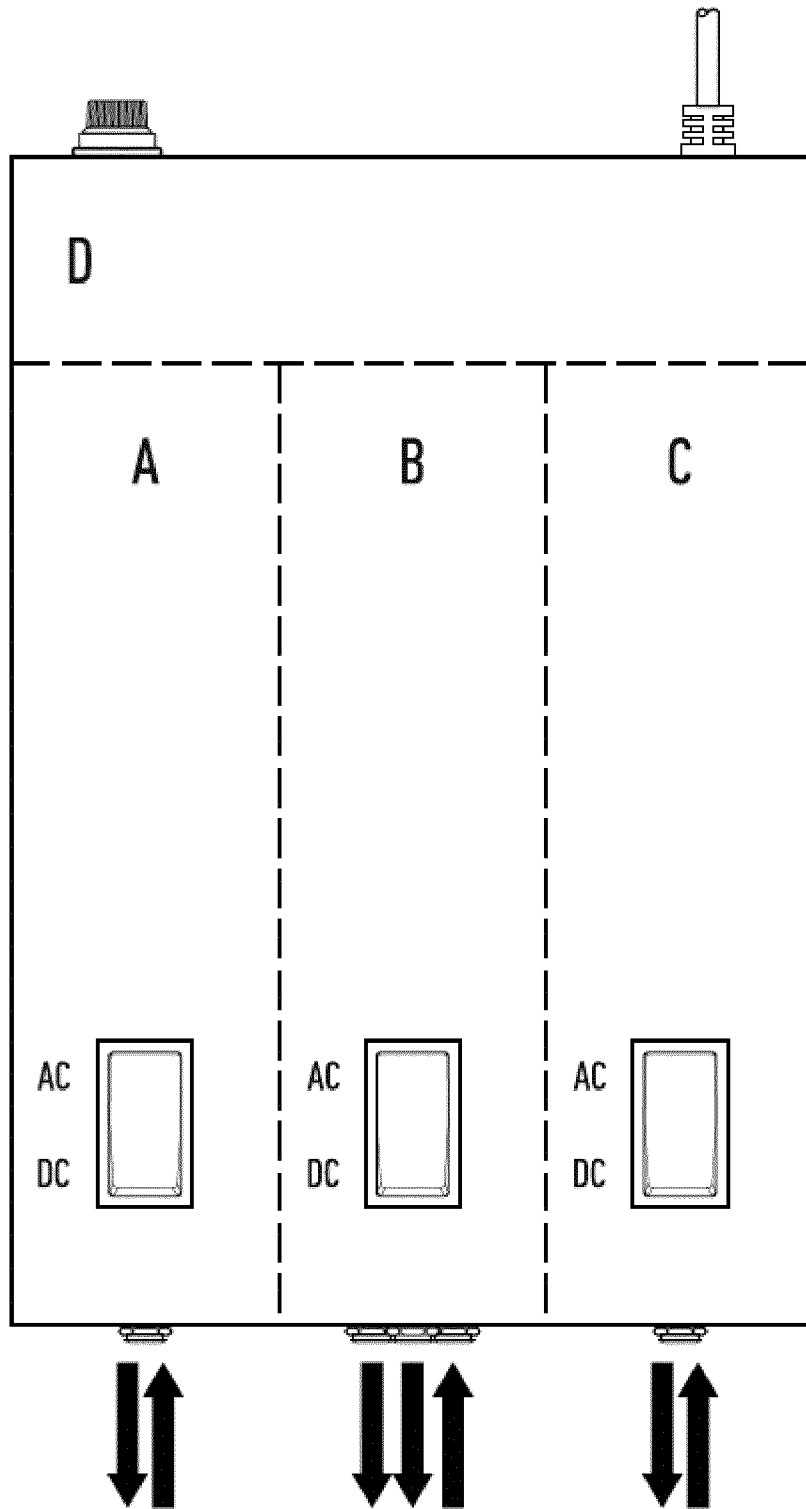


FIGURE 2.2

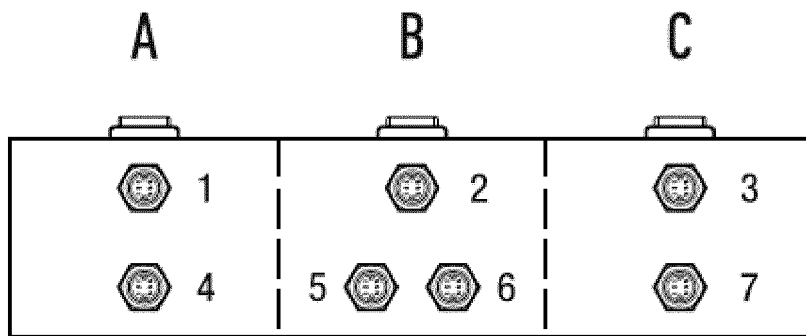


FIGURE 2.3

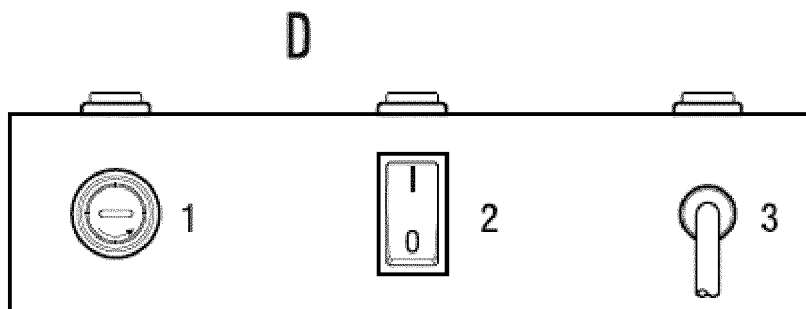


FIGURE 3

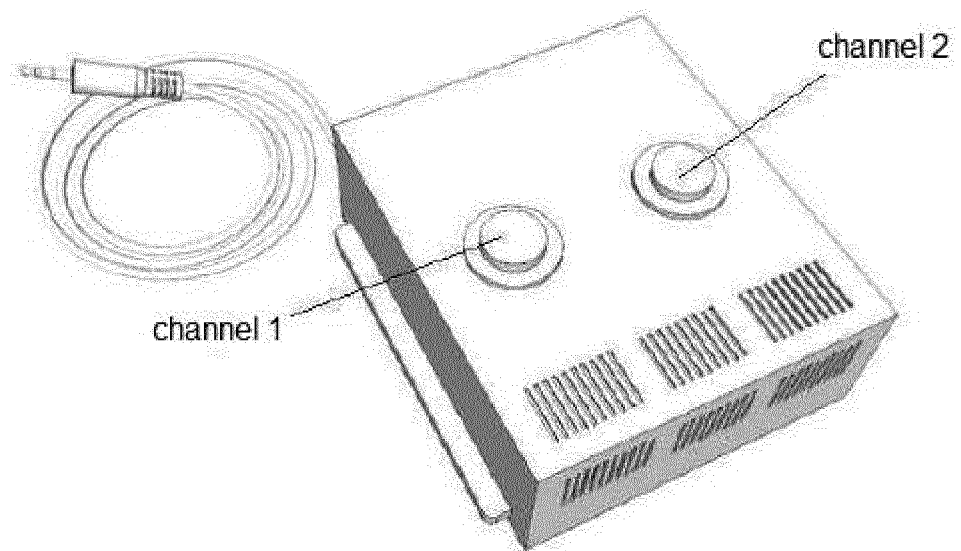


FIGURE 4

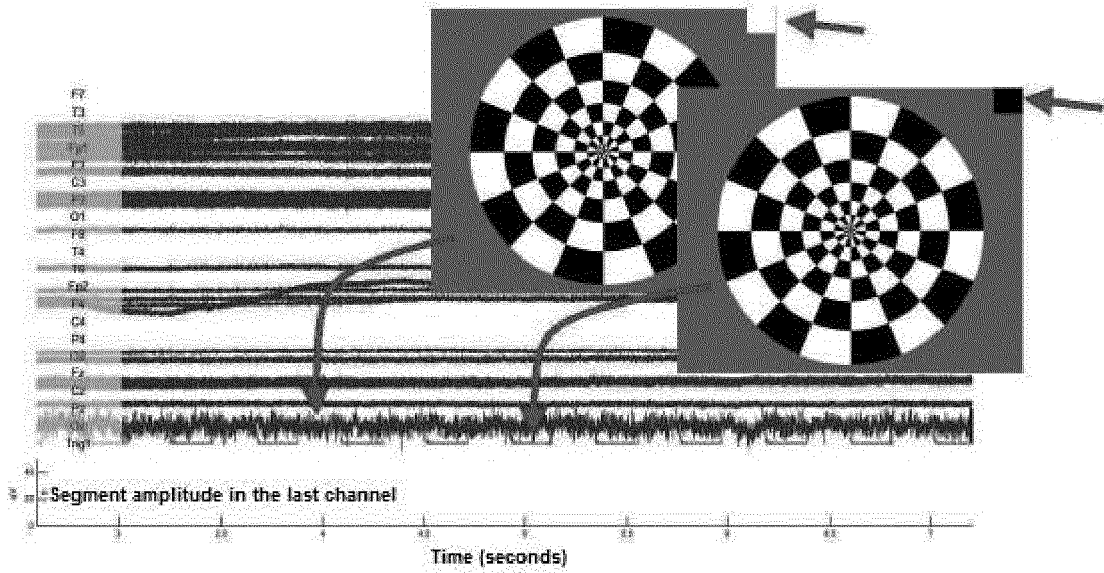


FIGURE 5A

**Module A**

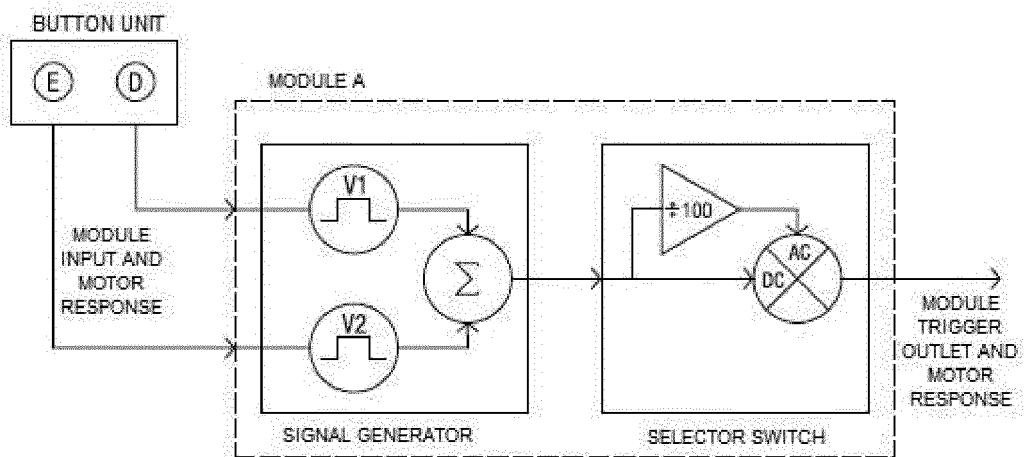


FIGURE 5B

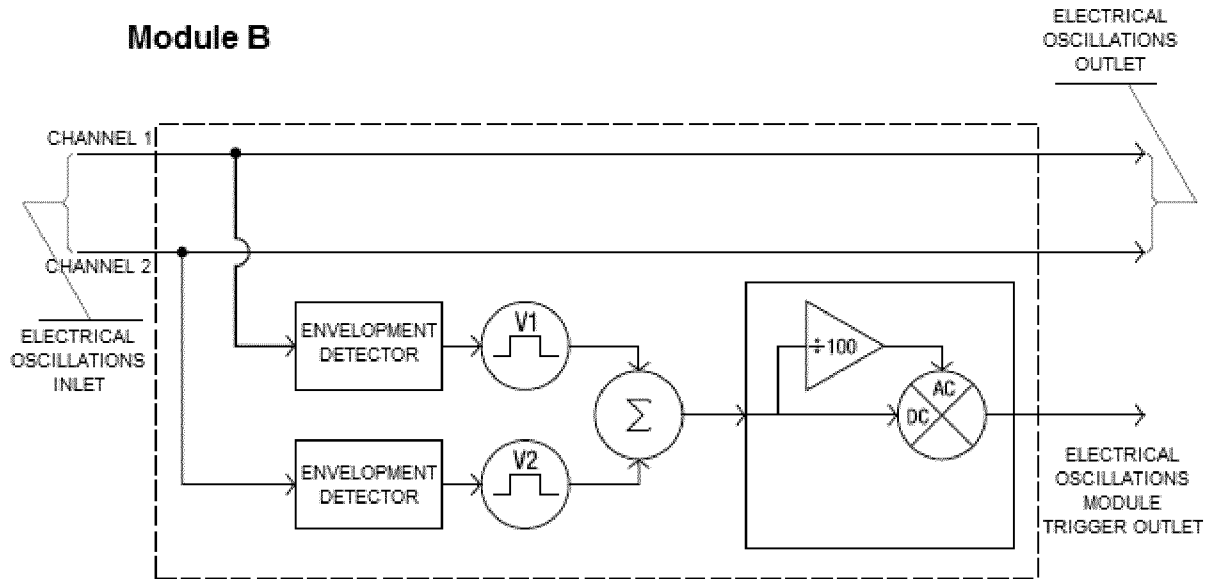


FIGURE 5C


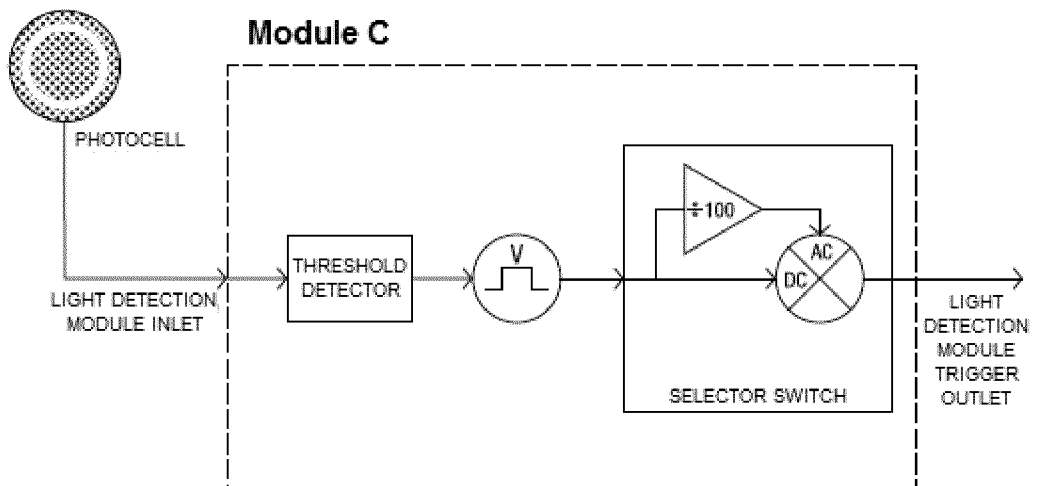


FIGURE 6

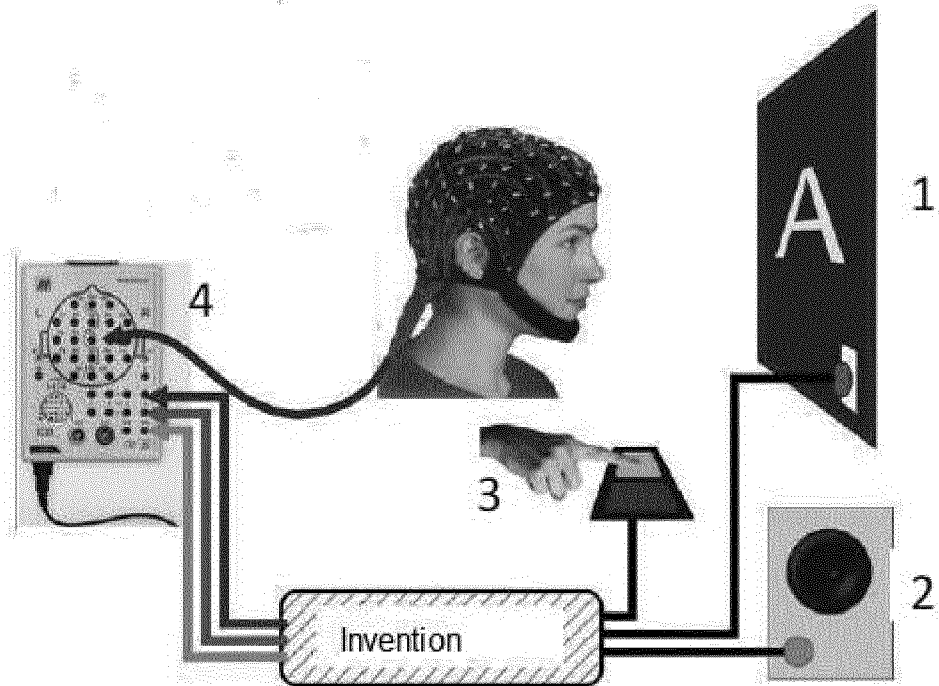

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/BR2017/050062

## A. CLASSIFICATION OF SUBJECT MATTER

IPC: **A61B5/0484 (2006.01), A61B5/00 (2006.01), A61B5/16 (2006.01), G06F19/00 (2011.01), A61B5/05 (2006.01)**  
 CPC: **A61B5/4064, A61H2230/10, G06F19/345, A61H2201/165, A61H2205/021**

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

**A61B, G06F19/00**

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

**GOOGLE PATENTS**

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

**EPODOC**

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2005177065 A1 ( Jamshid Ghajar [US] ) 11 August 2005 (2005-08-11) (see abstract; claims 2,7, 9 and 24; paragraphs 17, 029; figs. 1,3,4and 6)	1-7
A	US 4913160 A ( UNIV NEW YORK [US] ) 03 April 1990 (1990-04-03) (see abstract; claims 2 and 3; fig. 1)	1-7
A	US 20150126802 A1 (Regents University Of Minnesota [US] ) 07 May 2015 (2015-05-07) (see abstract; paragraphs 65-89 and 93)	1-7
A	US 8938289 B2 ( MOTORIKA LTD [BM] ) 20 January 2015 (2015-01-20) (see abstract; figs 6A, 7 and 11)	1-7

 Further documents are listed in the continuation of Box C. See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

**08/06/2017**

Date of mailing of the international search report

28/06/2017

Name and mailing address of the ISA/  
 INSTITUTO NACIONAL DA  
 PROPRIEDADE INDUSTRIAL  
 Rua Sao Bento nº 1, 17º andar  
 cep: 20090-010, Centro - Rio de Janeiro/RJ  
 Facsimile No. +55 21 3037-3663

Authorized officer

**Rony Leite Giffoni**

Telephone No.

**+55 21 3037-3493/3742**

INTERNATIONAL SEARCH REPORT

International application No.  
**PCT/BR2017/050062**

5  
 10  
 15  
 20  
 25  
 30  
 35  
 40  
 45  
 50  
 55

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2010145215 A1 (NEUROFOCUS INC [US]) 10 June 2010 (2010-06-10) (see abstract; paragraphs 22 and 39; claim 5; figures 1, 2, 4 and 7) -----	1-7

Form PCT/ISA/210 (continuation of second sheet) (January 2015)

EP 3 430 997 A1

INTERNATIONAL SEARCH REPORT  
Information on patent family members

International application No.

PCT/BR2017/050062

5  
10  
15  
20  
25  
30  
35  
40  
45  
50  
55

US 2005177065 A1	2005-08-11	US 7384399 B2	2008-06-10
		EP 1942803 A1	2008-07-16
		US 2008206727 A1	2008-08-28
		US 7708700 B2	2010-05-04
		US 2006270945 A1	2006-11-30
		US 7819818 B2	2010-10-26
		US 2010167246 A1	2010-07-01
		US 8048002 B2	2011-11-01
		WO 2007040857 A1	2007-04-12
-----	-----	-----	-----
US 4913160 A	1990-04-03	EP 0437012 A1	1991-07-17
-----	-----	-----	-----
US 20150126802 A1	2015-05-07	None	
-----	-----	-----	-----
US 8938289 B2	2015-01-20	None	
-----	-----	-----	-----
US 2010145215 A1	2010-06-10	EP 2377084 A1	2011-10-19
		IL 213459 D0	2011-07-31
		JP 2012511397 A	2012-05-24
		KR 20110100271 A	2011-09-09
		WO 2010068392 A1	2010-06-17
-----	-----	-----	-----

专利名称(译)	具有光事件，电自然振荡事件和电机行为事件的电子照相的模拟同步的模块化装置和方法		
公开(公告)号	<a href="#">EP3430997A4</a>	公开(公告)日	2019-11-13
申请号	EP2017765600	申请日	2017-03-17
[标]申请(专利权)人(译)	FUNDACAO OSWALDO CRUZ		
申请(专利权)人(译)	FUNDAÇÃO OSWALDO CRUZ		
当前申请(专利权)人(译)	奥斯瓦尔多·克鲁斯基金会		
[标]发明人	ABRAMOV DIMITRI MARQUES GALHANONE PAULO RICARDO LIMA MARCOS ANTONIO DIAS MARTINS CARLOS HENRIQUE QUINTANILHA		
发明人	ABRAMOV, DIMITRI, MARQUES GALHANONE, PAULO, RICARDO LIMA, MARCOS, ANTONIO, DIAS MARTINS, CARLOS, HENRIQUE, QUINTANILHA		
IPC分类号	A61B5/0484 A61B5/00 A61B5/16 G06F19/00 A61B5/05		
CPC分类号	A61B5/04842 A61B5/04845 A61B5/1104 A61B5/162 A61B5/7285		
代理机构(译)	LAVOIX		
优先权	102016060109 2016-03-18 BR		
其他公开文献	EP3430997A1		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

本发明涉及一种旨在使任何数字设备记录的脑电图 ( EEG ) 与物理事件 ( 感觉, 视觉或听觉刺激 ) 和行为事件 ( 运动反应, 声音反应 ) 同步的设备, 以允许 EEG 信号为了可视化诱发电位或与事件相关的电位, 这些介导是神经科学和神经病学和精神病学病理学临床研究中的重要研究主题。本发明允许将任何数字 EEG 设备转换成可以记录诱发电位的设备。本发明还提供一种用于使 EEG 与振荡的电光相关事件和电动机行为进行模拟同步的方法。