


(43) International Publication Date
19 March 2009 (19.03.2009)

(10) International Publication Number
WO 2009/036306 A1

- (51) **International Patent Classification:**
A61B 5/04 (2006.01)
- (21) **International Application Number:**
PCT/US2008/076217
- (22) **International Filing Date:**
12 September 2008 (12.09.2008)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
60/972,537 14 September 2007 (14.09.2007) US
61/055,662 23 May 2008 (23.05.2008) US
61/055,666 23 May 2008 (23.05.2008) US
- (71) **Applicant (for all designated States except US):** COR-
VENTIS, INC. [US/US]; 2226 North First Street, San
Jose, CA 95131 (US).
- (72) **Inventors; and**
- (75) **Inventors/Applicants (for US only):** LIBBUS, Imad
[US/US]; 1726 Stanford Avenue, Saint Paul, MN 55105
(US). MANICKA, Yatheendhar, D. [US/US]; 10544
Hawthorn Trail, Woodbury, MN 55129 (US). FOGOROS,
Rich [US/US]; 929 Old Hickory Road, Pittsburgh, PA
15243 (US).
- (74) **Agents:** SHIMMICK, John, K. et al.; Townsend And
Townsend And Crew LLP, Two Embarcadero Center, 8th
Floor, San Francisco, CA 94111-3834 (US).
- (81) **Designated States (unless otherwise indicated, for every
kind of national protection available):** AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA,
CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE,
EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID,
IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK,
LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW,
MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT,
RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.
- (84) **Designated States (unless otherwise indicated, for every
kind of regional protection available):** ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL,
NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG,
CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Declaration under Rule 4.17:**
— as to applicant's entitlement to apply for and be granted a
patent (Rule 4.17(ii))
- Published:**
— with international search report

(54) Title: ADHERENT CARDIAC MONITOR WITH ADVANCED SENSING CAPABILITIES

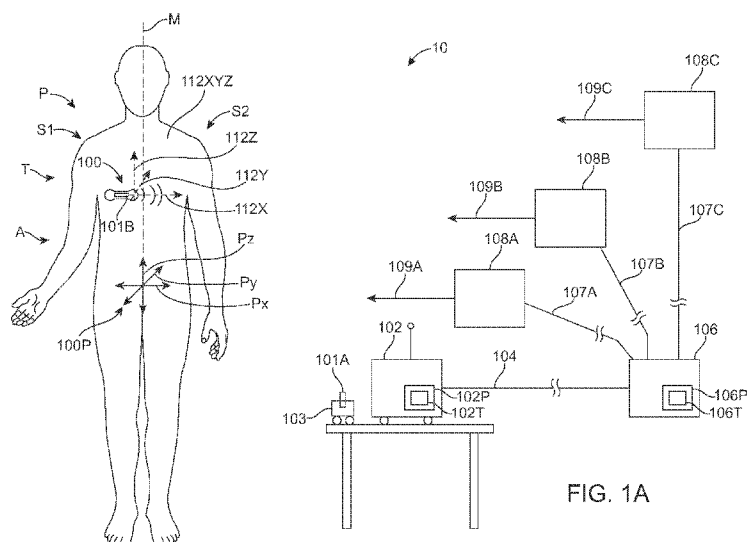

(S7) Abstract: An adherent device comprises an adhesive patch with at least two electrodes and an accelerometer. The accelerometer can be used to determine an orientation of the at least two measurement electrodes on a patient. By determining the orientation of the electrodes of the patch on the patient, physiologic measurements with the at least two electrodes can be adjusted and/or corrected in response to the orientation of the patch on the patient. The adherent patch and/or electrodes can be replaced with a second adherent patch and/or electrodes, and the orientation of the second adherent patch and/or electrodes can be determined with the accelerometer or a second accelerometer. The determined orientation of the second patch and/or electrodes on the patient can be used to correct measurements made with the second adherent patch and/or electrodes.

ADHERENT CARDIAC MONITOR WITH ADVANCED SENSING CAPABILITIES

CROSS-REFERENCES TO RELATED APPLICATIONS

- 5 [0001] The present application claims the benefit under 35 USC 119(e) of US Provisional Application Nos. 60/972,537 filed September 14, 2007, 61/055,666 and 61/055,662 both of which were filed May 23, 2008; the full disclosures of which are incorporated herein by reference in their entirety.

BACKGROUND OF THE INVENTION

- 10 [0002] 1. Field of the Invention. The present invention relates to patient monitoring. Although embodiments make specific reference to monitoring impedance and electrocardiogram signals with an adherent patch, the system methods and device described herein may be applicable to many applications in which physiological monitoring is used, for example wireless physiological monitoring for extended periods.

- 15 [0003] Patients are often treated for diseases and/or conditions associated with a compromised status of the patient, for example a compromised physiologic status. In some instances, a patient may report symptoms that require diagnosis to determine the underlying cause. For example, a patient may report fainting or dizziness that requires diagnosis, in which long term monitoring of the patient can provide useful information as to the physiologic status of the patient. In some
20 instances a patient may have suffered a heart attack and require care and/or monitoring after release from the hospital. One example of a device to provide long term monitoring of a patient is the Holter monitor, or ambulatory electrocardiography device.

- [0004] In addition to measuring heart signals with electrocardiograms, known physiologic measurements include impedance measurements. For example, transthoracic impedance
25 measurements can be used to measure hydration and respiration.

- [0005] Work in relation to embodiments of the present invention suggests that known methods and apparatus for long term monitoring of patients may be less than ideal. Although transthoracic measurements can be useful, such measurements may use electrodes that may be somewhat uncomfortable and/or cumbersome for the patient to wear. Also, it would be helpful
30 to detect subtle changes in patient physiology, for example based on subtle changes in

electrocardiogram signals and/or patient hydration signals. In at least some instances, electrodes that are held against the skin of the patient can become detached and/or dehydrated, such that the electrodes must be replaced. Replacement of electrodes can result in a change in the orientation of the electrodes that may affect the measured signal in at least some instances. Examples of physiological measurements that may be affected by electrode placement include electrocardiogram signals and tissue impedance signals to measure hydration and/or respiration of a patient. Therefore, a need exists to improve the quality of long term patient measurements with external devices, for example those worn by the patient.

[0006] Although implantable devices may be used in some instances, many of these devices can be invasive and/or costly, and may suffer at least some of the shortcomings of known wearable devices.

[0007] Therefore, a need exists for improved patient monitoring. Ideally, such improved patient monitoring would avoid at least some of the short-comings of the present methods and devices.

[0008] 2. Description of the Background Art. The following US Patents and Publications may describe relevant background art: 4,121,573; 4,478,223; 4,850,370; 4,955,381; 4,981,139; 5,080,099; 5,125,412; 5,331,966; 5,353,793; 5,511,553; 5,544,661; 5,558,638; 5,724,025; 5,772,586; 5,862,802; 5,970,986; 5,987,352; 6,047,203; 6,052,615; 6,117,077; 6,129,744; 6,225,901; 6,385,473; 6,416,471; 6,454,707; 6,480,733; 6,496,715; 6,527,711; 6,527,729; 6,551,252; 6,595,927; 6,595,929; 6,605,038; 6,611,705; 6,645,153; 6,699,200; 6,821,249; 6,912,414; 6,881,191; 6,980,851; 7,020,508; 7,054,679; 7,153,262; 7,206,630; 2002/0045836; 2003/0092975; 2003/0149349; 2005/0065445; 2005/0113703; 2005/0131288; 2005/0267381; 2006/0010090; 2006/0031102; 2006/0089679; 2006/0116592; 2006/0122474; 2006/0155183; 2006/0253044; 2006/0224051; 2006/0264730; 2007/0016089; 2007/0021678; 2007/0038038; 2007/0073132; 2007/0142715; 2007/0167849; 2007/0167850; and 2007/0208233.

BRIEF SUMMARY OF THE INVENTION

[0009] The present invention relates to patient monitoring. Although embodiments make specific reference to monitoring impedance and electrocardiogram signals with an adherent patch, the system methods and device described herein may be applicable to any application in which physiological monitoring is used, for example wireless physiological monitoring for extended periods.

[0010] In many embodiments, an adherent device comprises an adhesive patch with at least two electrodes and an accelerometer. The accelerometer can be used to determine an orientation of the at least two measurement electrodes on a patient, for example a measurement axis defined by the at least two electrodes. This use of the accelerometer and the at least two measurement electrodes can be particularly advantageous with patient monitoring for an extended period, for example when it is desirable to detect subtle changes in patient physiology and the adherent patch with electrodes is replaced. By determining the orientation of the electrodes of the patch on the patient, physiologic measurements with the at least two electrodes can be adjusted and/or corrected in response to the orientation of the patch on the patient. In many embodiments, the accelerometer may be oriented with respect to an electrode measurement axis in a predetermined configuration, which can facilitate determination of the electrode measurement axis in response to the accelerometer signal. In many embodiments, the adherent patch and/or electrodes are replaced with a second adherent patch and/or electrodes, and the orientation of the second adherent patch and/or electrodes determined with the accelerometer or a second accelerometer. The determined orientation of the second patch and/or electrodes on the patient can be used to correct measurements made with the second adherent patch and/or electrodes, such that errors associated with the alignment of the first and second patch on the patient can be minimized, even inhibited.

[0011] In a first aspect, embodiments of the present invention provide a method of monitoring a patient. An adherent device is adhered to a skin of the patient. The adherent device comprises an accelerometer and at least two measurement electrodes. The at least two measurement electrodes can be separated by a distance to define an electrode measurement axis. An accelerometer signal is measured when the device is adhered to the patient. An orientation of the electrode measurement axis on the patient is determined in response to the accelerometer signal.

[0012] In many embodiments, the accelerometer comprises at least one measurement axis sensitive to gravity aligned with the electrode measurement axis. The at least one accelerometer measurement axis can be configured to extend substantially horizontally on the patient when the device is adhered to the patient. The accelerometer signal may correspond to at least one accelerometer measurement vector in a direction along the at least one accelerometer measurement axis.

[0013] In many embodiments, the accelerometer comprises at least one accelerometer measurement axis sensitive to gravity, and the at least one accelerometer measurement axis is oriented with respect to the electrode measurement axis in a predetermined configuration.

[0014] The at least two electrodes may comprise a positive electrode and a negative electrode that define an orientation of an electrode measurement vector along the electrode measurement axis. The accelerometer signal may correspond to at least one accelerometer measurement vector that extends away from the electrode measurement axis. The at least one accelerometer measurement vector can be sensitive to gravity such that the accelerometer signal indicates when the patch adhered to the patient is upside down.

[0015] In many embodiments, the adherent device comprises an adherent surface to adhere to a skin of the patient, and electrode measurement axis extends along the adherent surface. The accelerometer may comprise three axes, and a first axis and a second axis of the three axes may extend along the measurement surface. A third axis of the three axes may extend away from the measurement surface.

[0016] In a specific embodiment, the accelerometer measurement signal may correspond to three orthogonal measurement vectors and each of the three orthogonal measurement vectors can extend along one of the accelerometer measurement axes.

[0017] In many embodiments, an electrocardiogram signal is measured with the at least two measurement electrodes, and the electrocardiogram signal is modified in response to the accelerometer signal. For example, the electrocardiogram vector can be rotated in response to the accelerometer signal to obtain a standard electrocardiogram vector. As a result of the rotation, the amplitude and direction of electrocardiogram features can be modified so as to approximate those of a standard electrocardiogram vector.

[0018] In another aspect, embodiments of the present invention provide a method of monitoring a patient. A first adherent patch is adhered to a skin of the patient, and the first patch comprises an adhesive and electrodes. A first accelerometer signal is measured when the first adherent patch is adhered to the patient. A second adherent patch is adhered to the skin of the patient, and the second patch comprises an adhesive and electrodes. A second accelerometer signal is measured when the second adherent patch is adhered to the patient. An orientation on the patient of at least one of the first patch or the second patch is determined in response to at least one of the first accelerometer signal or the second accelerometer signal.

[0019] In many embodiments, a first electrocardiogram signal is measured when the first adherent patch is adhered to the patient. A second electrocardiogram signal is measured when the second adherent patch is adhered to the patient. At least one of the first electrocardiogram

signal or the second electrocardiogram signal is adjusted in response to at least one of the first accelerometer signal or the second accelerometer signal.

[0020] In another aspect, embodiments of the present invention provide a method of monitoring a patient. A first adherent measurement device is adhered to a skin of the patient.

5 The first adherent measurement device comprises a first accelerometer and a first at least two measurement electrodes. A second adherent measurement device is adhered to a skin of the patient. The second adherent measurement device comprises a second accelerometer and a second at least two measurement electrodes. A first accelerometer signal is measured and a first electrocardiogram signal is measured with the first at least two measurement electrodes. The
10 first accelerometer signal and the first electrocardiogram signal are measured when the first adherent measurement device is adhered to the skin of the patient. A second accelerometer signal is measured and a second electrocardiogram signal is measured with the second at least two measurement electrodes. The second accelerometer signal and the second electrocardiogram signal are measured when the second adherent measurement device is adhered to the skin of the
15 patient. The first electrocardiogram signal is combined with the second electrocardiogram signal in response to the first accelerometer signal and the second accelerometer signal. The electrocardiogram signals can be combined by summing a scaled version of each signal.

[0021] In many embodiments, the first accelerometer comprises a first accelerometer measurement axis and the first at least two electrodes are separated by a first distance to define a
20 first electrode measurement axis. The first accelerometer measurement axis can be aligned with the first electrode measurement axis. The second accelerometer may comprise a second accelerometer measurement axis and the second at least two electrodes can be separated by a second distance to define a second electrode measurement axis. The second accelerometer measurement axis may be aligned with the second electrode measurement axis.

25 [0022] In many embodiments, an orientation of the first electrode measurement axis is determined in response to the first accelerometer signal. An orientation of the second electrode measurement axis is determined in response to the to the accelerometer signal.

[0023] In many embodiments, the first electrocardiogram signal is combined with the second electrocardiogram signal when the second adherent measurement device is adhered to the skin of
30 the patient.

[0024] In another aspect, embodiments of the present invention provide a device for monitoring a patient. The device comprises a support with an adhesive to adhere to a skin of the

patient, and an accelerometer to generate an accelerometer signal with the accelerometer supported with the support. At least two measurement electrodes are supported with the support, and the at least two measurement electrodes are separated by a distance to define an electrode measurement axis. The device comprises circuitry to measure the accelerometer signal when the device is adhered to the patient. A processor comprises a tangible medium configured to determine an orientation of the electrode measurement axis on the patient in response to the accelerometer signal.

[0025] In many embodiments, the support comprises an adhesive patch with an adhesive to adhere the support to the patient. The adhesive patch may comprise a breathable tape with adhesive to adhere the support to the patient.

[0026] In many embodiments, the accelerometer comprises at least one measurement axis sensitive to gravity aligned with the electrode measurement axis. The accelerometer may comprise at least one accelerometer measurement axis sensitive to gravity, and the accelerometer may be positioned and supported with the support such that the measurement axis extends substantially horizontally on the patient when the support is adhered to the patient.

[0027] In many embodiments, the accelerometer signal corresponds to at least one accelerometer measurement vector along the at least one accelerometer measurement axis.

[0028] In many embodiments, the accelerometer comprises at least one accelerometer measurement axis sensitive to gravity, and the at least one accelerometer measurement axis is oriented with respect to the electrode measurement axis in a predetermined configuration. The at least two electrodes may comprise a positive electrode and a negative electrode that define an orientation of an electrode measurement vector along the electrode measurement axis.

[0029] In many embodiments, the accelerometer signal corresponds to at least one measurement vector that extends away from the electrode measurement axis such that the accelerometer signal indicates when the patch adhered to the patient is upside down.

[0030] In many embodiments, the adherent device comprises an adherent surface to adhere to a skin of the patient, and the electrode measurement axis extends along the adherent surface. The accelerometer may comprise three axes, and a first axis and a second axis of the three axes can extend along the adherent surface. A third axis of the three axes can extend away from the adherent surface.

[0031] In many embodiments, the accelerometer signal corresponds to three orthogonal measurement vectors, and each of the three orthogonal measurement vectors extends along one of the accelerometer measurement axes.

[0032] In many embodiments, measurement circuitry is coupled to the at least two measurement electrode to measure an electrocardiogram signal. A processor is coupled to the measurement circuitry and comprises a tangible medium configured to modify the electrocardiogram signal in response to the accelerometer signal.

[0033] In another aspect, embodiments of the present invention provide a system for monitoring a patient. The system comprises a first support with a first adhesive to adhere to a skin of the patient. First electrodes are supported with the support to couple to the skin of the patient. The system comprises a second support with a second adhesive to adhere to the skin of the patient. Second electrodes are supported with the second support to couple to the skin of the patient. At least one accelerometer is coupled to at least one of the first support or the second support to determine an orientation of at least one of the first electrodes or the second electrodes when the at least one of the first electrodes or the second electrodes are coupled to the patient.

[0034] In many embodiments, the at least one accelerometer comprises a first accelerometer removably coupled to the first support in a first predetermined orientation and a second accelerometer removably coupled to the second support in a second predetermined orientation.

[0035] In many embodiments, the at least one accelerometer comprises an accelerometer removably coupled to the first support in a first predetermined orientation and wherein the accelerometer is removably coupled to the second support in a second predetermined orientation such that the accelerometer can be reused.

[0036] In many embodiments, the first support with the first adhesive comprises a first breathable tape and the second support with the second adhesive comprises a second breathable tape.

[0037] In another aspect, embodiments of the present invention provide a system for monitoring a patient. The system comprises a first adherent measurement device comprising a first support with a first adhesive to adhere the first support to a skin of the patient. The first adherent measurement device comprises a first accelerometer and a first at least two measurement electrodes. The first adherent device comprises first measurement circuitry to measure a first accelerometer signal with the accelerometer and a first electrocardiogram signal with the first at least two measurement electrodes. A second adherent measurement device

comprises a second support with a second adhesive to adhere the second support to a skin of the patient. The second adherent measurement device comprises a second accelerometer and a second at least two measurement electrodes. The second accelerometer comprises second circuitry to measure a second accelerometer signal with the second accelerometer and a second electrocardiogram signal with the second at least two measurement electrodes. A processor system comprises a tangible medium configured to combine the first electrocardiogram signal with the second electrocardiogram signal in response to the first accelerometer signal and the second accelerometer signal.

[0038] In many embodiments, the first accelerometer comprises a first accelerometer measurement axis and the first at least two electrodes are separated by a first distance to define a first electrode measurement axis. The first accelerometer measurement axis is aligned with the first electrode measurement axis. The second accelerometer comprises a second accelerometer measurement axis and the second at least two electrodes are separated by a second distance to define a second electrode measurement axis. The second accelerometer measurement axis may be aligned with the second electrode measurement axis. The processor system can be configured to determine an orientation of the first electrode measurement axis in response to the first accelerometer signal and determine an orientation of the second electrode measurement axis in response to the to the accelerometer signal.

[0039] The processor system may comprise at least one processor supported with at least one of the first support or the second support, and the at least one processor can be configured to combine the first electrocardiogram signal with the second electrocardiogram signal in response to the first accelerometer signal and the second accelerometer signal. Combining may include scaling each signal and summing the signals together.

BRIEF DESCRIPTION OF THE DRAWINGS

[0040] Figure 1A shows a patient and a monitoring system comprising an adherent device, according to embodiments of the present invention;

[0041] Figure 1B shows a bottom view of the adherent device as in Figure 1A comprising an adherent patch;

[0042] Figure 1C shows a top view of the adherent patch, as in Figure 1B;

[0043] Figure 1D shows a printed circuit boards and electronic components over the adherent patch, as in Figure 1C;

[0044] Figure 1D1 shows an equivalent circuit that can be used to determine optimal frequencies for determining patient hydration, according to embodiments of the present invention;

5 [0045] Figure 1D2 shows an adherent devices as in Figs. 1A-1D positioned on a patient to determine orientation of the adherent patch on the patient, according to embodiments of the present invention;

[0046] Figure 1D3 shows vectors from a 3D accelerometer to determine orientation of the measurement axis of the patch adhered on the patient, according to embodiments of the present invention;

10 [0047] Figure 1E shows batteries positioned over the printed circuit board and electronic components as in Figure 1D;

[0048] Figure 1F shows a top view of an electronics housing and a breathable cover over the batteries, electronic components and printed circuit board as in Figure 1E;

[0049] Figure 1G shows a side view of the adherent device as in Figures 1A to 1F;

15 [0050] Figure 1H shown a bottom isometric view of the adherent device as in Figures 1A to 1G;

[0051] Figures 1I and 1J show a side cross-sectional view and an exploded view, respectively, of the adherent device as in Figures 1A to 1H;

20 [0052] Figure 1K shows at least one electrode configured to electrically couple to a skin of the patient through a breathable tape, according to embodiments of the present invention;

[0053] Figures 2A to 2C show a system to monitor a patient for an extended period comprising a reusable electronic component and a plurality of disposable patch components, according to embodiments of the present invention;

[0054] Figure 2D shows a method of using the system as in Figures 2A to 2C;

25 [0055] Figures 3A to 3D show a method of monitoring a patient for an extended period with an adherent patch with adherent patches alternatively adhered to the right side or the left side of the patient; and

[0056] Figure 4A shows a method of monitoring a patient, according to embodiments of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0057] Embodiments of the present invention relate to patient monitoring. Although embodiments make specific reference to monitoring impedance and electrocardiogram signals with an adherent patch, the system methods and device described herein may be applicable to any application in which physiological monitoring is used, for example wireless physiological monitoring for extended periods.

[0058] In many embodiments, an adherent device comprises an adhesive patch with at least two electrodes and an accelerometer. The accelerometer can be used to determine an orientation of the at least two measurement electrodes on a patient, for example a measurement axis defined by the at least two electrodes. This use of the accelerometer and the at least two measurement electrodes can be particularly advantageous with patient monitoring for an extended period, for example when it is desirable to detect subtle changes in patient physiology and the adherent patch with electrodes is replaced. By determining the orientation of the electrodes of the patch on the patient, physiologic measurements with the at least two electrodes can be adjusted and/or corrected in response to the orientation of the patch on the patient. In many embodiments, the accelerometer may be oriented with respect to an electrode measurement axis in a predetermined configuration, which can facilitate determination of the electrode measurement axis in response to the accelerometer signal. In many embodiments, the adherent patch and/or electrodes are replaced with a second adherent patch and/or electrodes, and the orientation of the second adherent patch and/or electrodes determined with the accelerometer or a second accelerometer. The determined orientation of the second patch and/or electrodes on the patient can be used to correct measurements made with the second adherent patch and/or electrodes, such that errors associated with the alignment of the first and second patch on the patient can be minimized, even inhibited.

[0059] As used herein, an adhesive patch encompasses a piece of soft material with an adhesive that can cover a part of the body.

[0060] In many embodiments, the adherent devices described herein may be used for 90 day monitoring, or more, and may comprise completely disposable components and/or reusable components, and can provide reliable data acquisition and transfer. In many embodiments, the patch is configured for patient comfort, such that the patch can be worn and/or tolerated by the patient for extended periods, for example 90 days or more. In many embodiments, the adherent patch comprises a tape, which comprises a material, preferably breathable, with an adhesive, such that trauma to the patient skin can be minimized while the patch is worn for the extended

period. In many embodiments, the printed circuit board comprises a flex printed circuit board that can flex with the patient to provide improved patient comfort.

[0061] Figure 1A shows a patient P and a monitoring system 10. Patient P comprises a midline M, a first side S1, for example a right side, and a second side S2, for example a left side. Monitoring system 10 comprises an adherent device 100. Adherent device 100 can be adhered to a patient P at many locations, for example thorax T of patient P. In many embodiments, the adherent device may adhere to one side of the patient, from which side data can be collected. Work in relation with embodiments of the present invention suggests that location on a side of the patient can provide comfort for the patient while the device is adhered to the patient.

[0062] Adherent device 100 can be aligned and/or oriented with respect to axes of patient P. Orientation of adherent device 100 can comprise orientation of device 100 with a patient coordinate system 100P aligned with axes of the patient. Patient P comprises a horizontal axis Px that extends laterally from one side of the patient to the other, for example from side S1 to side S1 across midline M. Patient P comprises an anterior posterior axis Py that extends from the front, or anterior, of the patient to the back, or posterior of the patient. Patient P comprises a vertical axis Pz that extends vertically along the patient, for example vertically along the midline of the patient from the feet of the patient toward the head of the patient. In many embodiments, horizontal axis Px, anterior posterior axis Py and vertical axis Pz may comprise a right handed triple of orthogonal coordinate references.

[0063] Adherent device 100 may comprise a 3D coordinate reference system 112XYZ. Device 100 may comprise an X-axis 112X for alignment with horizontal axis Px of the patient, a Y-axis for alignment with anterior posterior axis Py of the patient and a Z axis for alignment with vertical axis Pz of the patient. Coordinate reference system 112XYZ may comprise X-axis 112X, Y-axis 112Y and Z-axis 112Z. Coordinate reference system 112XYZ may comprise a right handed triple, although other non-orthogonal and orthogonal reference systems may be used.

[0064] Adherent device 100 may comprise indicia for alignment with an axis of the patient. The indicia can be used to align at least one axis of device 100 with at least one axis of the patient. The indicia can be positioned on at least one of the adherent patch, a cover, or an electronics module. The indicia can be visible to the patient and/or a care provider to adhere device 100 to the patient in alignment with at least one axis of the patient. A vertical line along Z-axis 112Z can indicate vertical axis 112Z to the patient and/or care provider, and a horizontal

line along X-axis 112X can indicate horizontal X-axis 112X to the patient and/or care provider. A name, logo and/or trademark can be visible the outside of device 100 to indicate that device 100 correctly oriented, and arrows can also be used, for example a vertical arrow pointing up and a horizontal arrow pointing to the right.

- 5 [0065] Monitoring system 10 includes components to transmit data to a remote center 106. Remote center 106 can be located in a different building from the patient, for example in the same town as the patient, and can be located as far from the patient as a separate continent from the patient, for example the patient located on a first continent and the remote center located on a second continent. Adherent device 100 can communicate wirelessly to an intermediate device
- 10 102, for example with a single wireless hop from the adherent device on the patient to the intermediate device. Intermediate device 102 can communicate with remote center 106 in many ways, for example with an internet connection and/or with a cellular connection. In many embodiments, monitoring system 10 comprises a distributed processing system with at least one processor comprising a tangible medium of device 100, at least one processor 102P of
- 15 intermediate device 102, and at least one processor 106P at remote center 106, each of which processors can be in electronic communication with the other processors. At least one processor 102P comprises a tangible medium 102T, and at least one processor 106P comprises a tangible medium 106T. Remote processor 106P may comprise a backend server located at the remote center. Remote center 106 can be in communication with a health care provider 108A with a
- 20 communication system 107A, such as the Internet, an intranet, phone lines, wireless and/or satellite phone. Health care provider 108A, for example a family member, can be in communication with patient P with a communication, for example with a two way communication system, as indicated by arrow 109A, for example by cell phone, email, landline. Remote center 106 can be in communication with a health care professional, for example a
- 25 physician 108B, with a communication system 107B, such as the Internet, an intranet, phone lines, wireless and/or satellite phone. Physician 108B can be in communication with patient P with a communication, for example with a two way communication system, as indicated by arrow 109B, for example by cell phone, email, landline. Remote center 106 can be in communication with an emergency responder 108C, for example a 911 operator and/or
- 30 paramedic, with a communication system 107C, such as the Internet, an intranet, phone lines, wireless and/or satellite phone. Emergency responder 108C can travel to the patient as indicated by arrow 109C. Thus, in many embodiments, monitoring system 10 comprises a closed loop system in which patient care can be monitored and implemented from the remote center in response to signals from the adherent device.

[0066] In many embodiments, the adherent device may continuously monitor physiological parameters, communicate wirelessly with a remote center, and provide alerts when necessary. The system may comprise an adherent patch, which attaches to the patient's thorax and contains sensing electrodes, battery, memory, logic, and wireless communication capabilities. In some
5 embodiments, the patch can communicate with the remote center, via the intermediate device in the patient's home. In some embodiments, remote center 106 receives the patient data and applies a patient evaluation algorithm, for example an algorithm to calculate the apnea hypopnea index. When a flag is raised, the center may communicate with the patient, hospital, nurse, and/or physician to allow for therapeutic intervention.

10 [0067] The adherent device may be affixed and/or adhered to the body in many ways. For example, with at least one of the following: an adhesive tape, a constant-force spring, suspenders around shoulders, a screw-in microneedle electrode, a pre-shaped electronics module to shape fabric to a thorax, a pinch onto roll of skin, or transcutaneous anchoring. Patch and/or device
15 replacement may occur with a keyed patch (e.g. two-part patch), an outline or anatomical mark, a low-adhesive guide (place guide | remove old patch | place new patch | remove guide), or a keyed attachment for chatter reduction. The patch and/or device may comprise an adhesiveless embodiment (e.g. chest strap), and/or a low-irritation adhesive for sensitive skin. The adherent patch and/or device can comprise many shapes, for example at least one of a dogbone, an hourglass, an oblong, a circular or an oval shape.

20 [0068] In many embodiments, the adherent device may comprise a reusable electronics module with replaceable patches, and each of the replaceable patches may include a battery. The module may collect cumulative data for approximately 90 days and/or the entire adherent component (electronics + patch) may be disposable. In a completely disposable embodiment, a "baton" mechanism may be used for data transfer and retention, for example baton transfer may include
25 baseline information. In some embodiments, the device may have a rechargeable module, and may use dual battery and/or electronics modules, wherein one module 101A can be recharged using a charging station 103 while the other module 101B is placed on the adherent patch with connectors. In some embodiments, the intermediate device 102 may comprise the charging module, data transfer, storage and/or transmission, such that one of the electronics modules can
30 be placed in the intermediate device for charging and/or data transfer while the other electronics module is worn by the patient.

[0069] System 10 can perform the following functions: initiation, programming, measuring, storing, analyzing, communicating, predicting, and displaying. The adherent device may contain

a subset of the following physiological sensors: bioimpedance, respiration, respiration rate variability, heart rate (ave, min, max), heart rhythm, heart rate variability (HRV), heart rate turbulence (HRT), heart sounds (e.g. S3), respiratory sounds, blood pressure, activity, posture, wake/sleep, orthopnea, temperature/heat flux, and weight. The activity sensor may comprise one or more of the following: ball switch, accelerometer, minute ventilation, HR, bioimpedance noise, skin temperature/heat flux, BP, muscle noise, posture.

[0070] The adherent device can wirelessly communicate with remote center 106. The communication may occur directly (via a cellular or Wi-Fi network), or indirectly through intermediate device 102. Intermediate device 102 may consist of multiple devices, which can communicate wired or wirelessly to relay data to remote center 106.

[0071] In many embodiments, instructions are transmitted from remote site 106 to a processor supported with the adherent patch on the patient, and the processor supported with the patient can receive updated instructions for the patient treatment and/or monitoring, for example while worn by the patient.

[0072] Figure 1B shows a bottom view of adherent device 100 as in Figure 1A comprising an adherent patch 110. Adherent patch 110 comprises a first side, or a lower side 110A, that is oriented toward the skin of the patient when placed on the patient. In many embodiments, adherent patch 110 comprises a tape 110T which is a material, preferably breathable, with an adhesive 116A. Patient side 110A comprises adhesive 116A to adhere the patch 110 and adherent device 100 to patient P. Electrodes 112A, 112B, 112C and 112D are affixed to adherent patch 110. In many embodiments, at least four electrodes are attached to the patch, for example six electrodes. In some embodiments the patch comprises two electrodes, for example two electrodes to measure the electrocardiogram (ECG) of the patient. Gel 114A, gel 114B, gel 114C and gel 114D can each be positioned over electrodes 112A, 112B, 112C and 112D, respectively, to provide electrical conductivity between the electrodes and the skin of the patient. In many embodiments, the electrodes can be affixed to the patch 110, for example with known methods and structures such as rivets, adhesive, stitches, etc. In many embodiments, patch 110 comprises a breathable material to permit air and/or vapor to flow to and from the surface of the skin.

[0073] Electrodes 112A, 112B, 112C and 112D extend substantially along a horizontal measurement axis that corresponds to X axis-112X of the measurement device. Electrodes 112, 112B, 112C and 112D can be affixed to adherent patch 110A, such that the positions of

electrodes 112A, 112B, 112C and 112D comprise predetermined positions on adherent patch 110A. Z-axis 112Z can extend perpendicular to the electrode measurement axis, for example vertically and perpendicular to X-axis 112 when adhered on the patient. X-axis 112X and Z-axis 112Z can extend along an adhesive surface of adherent patch 110A, and a Y-axis 112Y can
5 extend away from the adhesive surface of adherent device 110A.

[0074] Figure 1C shows a top view of the adherent patch 100, as in Figure 1B. Adherent patch 100 comprises a second side, or upper side 110B. In many embodiments, electrodes 112A, 112B, 112C and 112D extend from lower side 110A through adherent patch 110 to upper side 110B. An adhesive 116B can be applied to upper side 110B to adhere structures, for example a
10 breathable cover, to the patch such that the patch can support the electronics and other structures when the patch is adhered to the patient. The PCB may comprise completely flex PCB, rigid PCB, rigid PCB combined flex PCB and/or rigid PCB boards connected by cable.

[0075] Figure 1D shows a printed circuit boards and electronic components over adherent patch 110, as in Figure 1A to 1C. In some embodiments, a printed circuit board (PCB), for
15 example flex printed circuit board 120, may be connected to electrodes 112A, 112B, 112C and 112D with connectors 122A, 122B, 122C and 122D. Flex printed circuit board 120 can include traces 123A, 123B, 123C and 123D that extend to connectors 122A, 122B, 122C and 122D, respectively, on the flex PCB. Connectors 122A, 122B, 122C and 122D can be positioned on flex printed circuit board 120 in alignment with electrodes 112A, 112B, 112C and 112D so as to
20 electrically couple the flex PCB with the electrodes. For example, connectors 122A and 122D may comprise a flexible polyester film coated with conductive silver ink. In some embodiments, connectors 122A, 122B, 122C and 122D may comprise insulated wires and/or a film with conductive ink that provide strain relief between the PCB and the electrodes. In some embodiments, additional PCB's, for example rigid PCB's 120A, 120B, 120C and 120D, can be
25 connected to flex printed circuit board 120. Electronic components 130 can be connected to flex printed circuit board 120 and/or mounted thereon. In some embodiments, electronic components 130 can be mounted on the additional PCB's.

[0076] Electronic components 130 comprise components to take physiologic measurements, transmit data to remote center 106 and receive commands from remote center 106. In many
30 embodiments, electronics components 130 may comprise known low power circuitry, for example complementary metal oxide semiconductor (CMOS) circuitry components. Electronics components 130 comprise an activity sensor and activity circuitry 134, impedance circuitry 136 and electrocardiogram circuitry, for example ECG circuitry 136. In some embodiments,

electronics circuitry 130 may comprise a microphone and microphone circuitry 142 to detect an audio signal from within the patient, and the audio signal may comprise a heart sound and/or a respiratory sound, for example an S3 heart sound and a respiratory sound with rales and/or crackles.

5 **[0077]** Electronics circuitry 130 may comprise a temperature sensor, for example a thermistor in contact with the skin of the patient, and temperature sensor circuitry 144 to measure a temperature of the patient, for example a temperature of the skin of the patient. A temperature sensor may be used to determine the sleep and wake state of the patient. The temperature of the patient can decrease as the patient goes to sleep and increase when the patient wakes up.

10 **[0078]** Work in relation to embodiments of the present invention suggests that skin temperature may effect impedance and/or hydration measurements, and that skin temperature measurements may be used to correct impedance and/or hydration measurements. In some embodiments, increase in skin temperature or heat flux can be associated with increased vaso-dilation near the skin surface, such that measured impedance measurement decreased, even
15 through the hydration of the patient in deeper tissues under the skin remains substantially unchanged. Thus, use of the temperature sensor can allow for correction of the hydration signals to more accurately assess the hydration, for example extra cellular hydration, of deeper tissues of the patient, for example deeper tissues in the thorax.

[0079] Electronics circuitry 130 may comprise a processor 146. Processor 146 comprises a
20 tangible medium, for example read only memory (ROM), electrically erasable programmable read only memory (EEPROM) and/or random access memory (RAM). Processor 146 may comprise many known processors with real time clock and frequency generator circuitry, for example the PIC series of processors available from Microchip, of Chandler AZ.. In some embodiments, processor 136 may comprise the frequency generator and real time clock. The
25 processor can be configured to control a collection and transmission of data from the impedance circuitry electrocardiogram circuitry and the accelerometer. In many embodiments, device 100 comprise a distributed processor system, for example with multiple processors on device 100.

[0080] In many embodiments, electronics components 130 comprise wireless communications circuitry 132 to communicate with remote center 106. The wireless communication circuitry can
30 be coupled to the impedance circuitry, the electrocardiogram circuitry and the accelerometer to transmit to a remote center with a communication protocol at least one of the hydration signal, the electrocardiogram signal or the inclination signal. In specific embodiments, wireless

communication circuitry is configured to transmit the hydration signal, the electrocardiogram signal and the inclination signal to the remote center with a single wireless hop, for example from wireless communication circuitry 132 to intermediate device 102. The communication protocol comprises at least one of Bluetooth, Zigbee, WiFi, WiMax, IR, amplitude modulation or frequency modulation. In many embodiments, the communications protocol comprises a two way protocol such that the remote center is capable of issuing commands to control data collection.

[0081] Intermediate device 102 may comprise a data collection system to collect and store data from the wireless transmitter. The data collection system can be configured to communicate periodically with the remote center. The data collection system can transmit data in response to commands from remote center 106 and/or in response to commands from the adherent device.

[0082] Activity sensor and activity circuitry 134 can comprise many known activity sensors and circuitry. In many embodiments, the accelerometer comprises at least one of a piezoelectric accelerometer, capacitive accelerometer or electromechanical accelerometer. The accelerometer may comprise a 3-axis accelerometer to measure at least one of an inclination, a position, an orientation or acceleration of the patient in three dimensions. Work in relation to embodiments of the present invention suggests that three dimensional orientation of the patient and associated positions, for example sitting, standing, lying down, can be very useful when combined with data from other sensors, for example ECG data and/or bioimpedance data, for example a respiration rate of the patient.

[0083] Activity sensor 134 may comprise an accelerometer with at least one measurement axis, for example two or more measurement axes. In some embodiments, activity sensor 134 comprises three axis accelerometer 134A. Three axis accelerometer 134A may comprise an X-axis 134X, a Y-axis 134Y and a Z-axis 134Z with each axis sensitive to gravity such that the orientation of the accelerometer can be determined in relation to gravity. Three axis accelerometer 134A can be aligned with electrodes of adherent patch 110A. X-axis 134X can be aligned with X-axis 112X of adherent patch 110. Y-axis 134Y can be aligned with Y-axis 112Y of adherent patch 110. Z-axis 134Z can be aligned with Z-axis 112Z of adherent patch 110. Axes of accelerometer 134A can be aligned with axes of patch 110A, for example with connectors 122A, 122B, 122C and 122D, such that the axes of the accelerometer are aligned with adherent patch and/or the electrodes in a predetermined configuration. Although the axes of the patch and accelerometer are shown substantially parallel, the axes of the patch can be aligned with the axes of the accelerometer in a non-parallel configuration, for example an oblique

configuration with oblique angles between axes of the accelerometer and axes of the adherent patch and/or electrodes.

[0084] Impedance circuitry 136 can generate both hydration data and respiration data. In many embodiments, impedance circuitry 136 is electrically connected to electrodes 112A, 112B, 112C and 112D in a four pole configuration, such that electrodes 112A and 112D comprise outer electrodes that are driven with a current and comprise force electrodes that force the current through the tissue. The current delivered between electrodes 112A and 112D generates a measurable voltage between electrodes 112B and 112C, such that electrodes 112B and 112C comprise inner, sense, electrodes that sense and/or measure the voltage in response to the current from the force electrodes. In some embodiments, electrodes 112B and 112C may comprise force electrodes and electrodes 112A and 112D may comprise sense electrodes. The voltage measured by the sense electrodes can be used to measure the impedance of the patient and determine the respiration rate and/or hydration of the patient.

[0085] Figure 1D1 shows an equivalent circuit 152 that can be used to determine optimal frequencies for measuring patient hydration. Work in relation to embodiments of the present invention indicates that the frequency of the current and/or voltage at the force electrodes can be selected so as to provide impedance signals related to the extracellular and/or intracellular hydration of the patient tissue. Equivalent circuit 152 comprises an intracellular resistance 156, or R_{ICW} in series with a capacitor 154, and an extracellular resistance 158, or R_{ECW} . Extracellular resistance 158 is in parallel with intracellular resistance 156 and capacitor 154 related to capacitance of cell membranes. In many embodiments, impedances can be measured and provide useful information over a wide range of frequencies, for example from about 0.5 kHz to about 200 KHz. Work in relation to embodiments of the present invention suggests that extracellular resistance 158 can be significantly related extracellular fluid and to cardiac decompensation, and that extracellular resistance 158 and extracellular fluid can be effectively measured with frequencies in a range from about 0.5 kHz to about 20 kHz, for example from about 1 kHz to about 10 kHz. In some embodiments, a single frequency can be used to determine the extracellular resistance and/or fluid. As sample frequencies increase from about 10 kHz to about 20 kHz, capacitance related to cell membranes decrease the impedance, such that the intracellular fluid contributes to the impedance and/or hydration measurements. Thus, many embodiments of the present invention measure hydration with frequencies from about 0.5 kHz to about 20 kHz to determine patient hydration.

[0086] In many embodiments, impedance circuitry 136 can be configured to determine respiration of the patient. In specific embodiments, the impedance circuitry can measure the hydration at 25 Hz intervals, for example at 25 Hz intervals using impedance measurements with a frequency from about 0.5 kHz to about 20 kHz.

5 **[0087]** ECG circuitry 138 can generate electrocardiogram signals and data from two or more of electrodes 112A, 112B, 112C and 112D in many ways. In some embodiments, ECG circuitry 138 is connected to inner electrodes 112B and 112C, which may comprise sense electrodes of the impedance circuitry as described above. In some embodiments, ECG circuitry 138 can be connected to electrodes 112A and 112D so as to increase spacing of the electrodes. The inner
10 electrodes may be positioned near the outer electrodes to increase the voltage of the ECG signal measured by ECG circuitry 138. In many embodiments, the ECG circuitry may measure the ECG signal from electrodes 112A and 112D when current is not passed through electrodes 112A and 112D.

[0088] ECG circuitry 138 can be coupled to the electrodes in many ways to define an
15 electrocardiogram vector. For example electrode 112A can be coupled to a positive amplifier terminal of ECG circuitry 138 and electrode 112D can be coupled to a negative amplifier terminal of ECG circuitry 138 to define an orientation of an electrocardiogram vector along the electrode measurement axis. To define an electrocardiogram vector with an opposite orientation electrode 112D can be couple to the positive amplifier terminal of ECG circuitry 138 and
20 electrode 112A can be coupled to the negative amplifier terminal of ECG circuitry 138. The ECG circuitry may be coupled to the inner electrodes so as to define an ECG vector along a measurement axis of the inner electrodes.

[0089] Figure 1D2 shows adherent device 100 positioned on patient P to determine orientation of the adherent patch. X-axis 112X of device 100 is inclined at an angle α to horizontal axis Px
25 of patient P. Z-axis 112Z of device 100 is inclined at angle α to vertical axis Pz of patient P. Y-axis 112Y may be inclined at a second angle, for example β , to anterior posterior axis Py and vertical axis Pz. As the accelerometer of adherent device 100 can be sensitive to gravity, inclination of the patch relative to axis of the patient can be measured, for example when the patient stands.

30 **[0090]** Figure 1D3 shows vectors from a 3D accelerometer to determine orientation of the measurement axis of the patch adhered on the patient. A Z-axis vector 112ZV can be measured along vertical axis 112Z with an accelerometer signal from axis 134Z of accelerometer 134A.

An X-axis vector 112XV can be measured along horizontal axis 112X with an accelerometer signal from axis 134X of accelerometer 134A. Inclination angle α can be determined in response to X-axis vector 112XV and Z-axis vector 112ZV, for example with vector addition of X-axis vector 112XV and Z-axis vector 112ZV. An inclination angle β for the patch along the Y and Z axes can be similarly obtained an accelerometer signal from axis 134Y of accelerometer 134A and vector 112ZV.

[0091] Figure 1E shows batteries 150 positioned over the flex printed circuit board and electronic components as in Figure 1D. Batteries 150 may comprise rechargeable batteries that can be removed and/or recharged. In some embodiments, batteries 150 can be removed from the adherent patch and recharged and/or replaced.

[0092] Figure 1F shows a top view of a cover 162 over the batteries, electronic components and flex printed circuit board as in Figures 1A to 1E. In many embodiments, an electronics housing 160 may be disposed under cover 162 to protect the electronic components, and in some embodiments electronics housing 160 may comprise an encapsulant over the electronic components and PCB. In some embodiments, cover 162 can be adhered to adherent patch 110 with an adhesive 164 on an underside of cover 162. In many embodiments, electronics housing 160 may comprise a water proof material, for example a sealant adhesive such as epoxy or silicone coated over the electronics components and/or PCB. In some embodiments, electronics housing 160 may comprise metal and/or plastic. Metal or plastic may be potted with a material such as epoxy or silicone.

[0093] Cover 162 may comprise many known biocompatible cover, casing and/or housing materials, such as elastomers, for example silicone. The elastomer may be fenestrated to improve breathability. In some embodiments, cover 162 may comprise many known breathable materials, for example polyester, polyamide, and/or elastane (Spandex). The breathable fabric may be coated to make it water resistant, waterproof, and/or to aid in wicking moisture away from the patch.

[0094] Figure 1G shows a side view of adherent device 100 as in Figures 1A to 1F. Adherent device 100 comprises a maximum dimension, for example a length 170 from about 2 to 10 inches (from about 50 mm to about 250 mm), for example from about 4 to 6 inches (from about 100 mm to about 150 mm). In some embodiments, length 170 may be no more than about 6 inches (no more than about 150 mm). Adherent device 100 comprises a thickness 172. Thickness 172 may comprise a maximum thickness along a profile of the device. Thickness 172

can be from about 0.1 inches to about 0.4 inches (from about 5 mm to about 10 mm), for example about 0.3 inches (about 7.5 mm) .

[0095] Figure 1H shown a bottom isometric view of adherent device 100 as in Figures 1A to 1G. Adherent device 100 comprises a width 174, for example a maximum width along a width profile of adherent device 100. Width 174 can be from about 1 to about 4 inches (from about 25 mm to 100 mm), for example about 2 inches (about 50 mm).

[0096] Figures 1I and 1J show a side cross-sectional view and an exploded view, respectively, of adherent device 100 as in Figures 1A to 1H. Device 100 comprises several layers. Gel 114A, or gel layer, is positioned on electrode 112A to provide electrical conductivity between the electrode and the skin. Electrode 112A may comprise an electrode layer. Adhesive patch 110 may comprise a layer of breathable tape 110T, for example a known breathable tape, such as tricot-knit polyester fabric. An adhesive 116A, for example a layer of acrylate pressure sensitive adhesive, can be disposed on underside 110A of adherent patch 110. A gel cover 180, or gel cover layer, for example a polyurethane non-woven tape, can be positioned over patch 110 comprising the breathable tape. A PCB layer, for example flex printed circuit board 120, or flex PCB layer, can be positioned over gel cover 180 with electronic components 130 connected and/or mounted to flex printed circuit board 120, for example mounted on flex PCB so as to comprise an electronics layer disposed on the flex PCB layer. In many embodiments, the adherent device may comprise a segmented inner component, for example the PCB may be segmented to provide at least some flexibility. In many embodiments, the electronics layer may be encapsulated in electronics housing 160 which may comprise a waterproof material, for example silicone or epoxy. In many embodiments, the electrodes are connected to the PCB with a flex connection, for example trace 123A of flex printed circuit board 120, so as to provide strain relive between the electrodes 112A, 112B, 112C and 112D and the PCB. Gel cover 180 can inhibit flow of gel 114A and liquid. In many embodiments, gel cover 180 can inhibit gel 114A from seeping through breathable tape 110T to maintain gel integrity over time. Gel cover 180 can also keep external moisture, for example liquid water, from penetrating though the gel cover into gel 114A while allowing moisture vapor from the gel, for example moisture vapor from the skin, to transmit through the gel cover. In many embodiments, cover 162 can encase the flex PCB and/or electronics and can be adhered to at least one of the electronics, the flex PCB or adherent patch 110, so as to protect at least the electronics components and the PCB. Cover 162 can attach to adhesive patch 110 with adhesive 116B. Cover 162 can comprise many known biocompatible cover materials, for example silicone. Cover 162 can comprise an outer

polymer cover to provide smooth contour without limiting flexibility. In many embodiments, cover 162 may comprise a breathable fabric. Cover 162 may comprise many known breathable fabrics, for example breathable fabrics as described above. In some embodiments, the breathable cover may comprise a breathable water resistant cover. In some embodiments, the breathable
5 fabric may comprise polyester, nylon, polyamide, and/or elastane (Spandex) to allow the breathable fabric to stretch with body movement. In some embodiments, the breathable tape may contain and elute a pharmaceutical agent, such as an antibiotic, anti-inflammatory or antifungal agent, when the adherent device is placed on the patient.

[0097] The breathable cover 162 and adherent patch 110 comprises breathable tape can be
10 configured to couple continuously for at least one week the at least one electrode to the skin so as to measure breathing of the patient. The breathable tape may comprise the stretchable breathable material with the adhesive and the breathable cover may comprises a stretchable water resistant material connected to the breathable tape, as described above, such that both the adherent patch and cover can stretch with the skin of the patient. Arrows 182 show stretching of adherent patch
15 110, and the stretching of adherent patch can be at least two dimensional along the surface of the skin of the patient. As noted above, connectors 122A, 122B, 122C and 122D between PCB 130 and electrodes 112A, 112B, 112C and 112D may comprise insulated wires that provide strain relief between the PCB and the electrodes, such that the electrodes can move with the adherent patch as the adherent patch comprising breathable tape stretches. Arrows 184 show stretching of
20 cover 162, and the stretching of the cover can be at least two dimensional along the surface of the skin of the patient. Cover 162 can be attached to adherent patch 110 with adhesive 116B such that cover 162 stretches and/or retracts when adherent patch 110 stretches and/or retracts with the skin of the patient. For example, cover 162 and adhesive patch 110 can stretch in two dimensions along length 170 and width 174 with the skin of the patient, and stretching along
25 length 170 can increase spacing between electrodes. Stretching of the cover and adhesive patch 110, for example in two dimensions, can extend the time the patch is adhered to the skin as the patch can move with the skin such that the patch remains adhered to the skin. Cover 162 can be attached to adherent patch 110 with adhesive 116B such that cover 162 stretches and/or retracts when adherent patch 110 stretches and/or retracts with the skin of the patient, for example along
30 two dimensions comprising length 170 and width 174. Electronics housing 160 can be smooth and allow breathable cover 162 to slide over electronics housing 160, such that motion and/or stretching of cover 162 is slidably coupled with housing 160. The printed circuit board can be slidably coupled with adherent patch 110 that comprises breathable tape 110T, such that the breathable tape can stretch with the skin of the patient when the breathable tape is adhered to the

skin of the patient. Electronics components 130 can be affixed to printed circuit board 120, for example with solder, and the electronics housing can be affixed over the PCB and electronics components, for example with dip coating, such that electronics components 130, printed circuit board 120 and electronics housing 160 are coupled together. Electronics components 130, printed circuit board 120, and electronics housing 160 are disposed between the stretchable breathable material of adherent patch 110 and the stretchable water resistant material of cover 160 so as to allow the adherent patch 110 and cover 160 to stretch together while electronics components 130, printed circuit board 120, and electronics housing 160 do not stretch substantially, if at all. This decoupling of electronics housing 160, printed circuit board 120 and electronic components 130 can allow the adherent patch 110 comprising breathable tape to move with the skin of the patient, such that the adherent patch can remain adhered to the skin for an extended time of at least one week, for example two or more weeks.

[0098] An air gap 169 may extend from adherent patch 110 to the electronics module and/or PCB, so as to provide patient comfort. Air gap 169 allows adherent patch 110 and breathable tape 110T to remain supple and move, for example bend, with the skin of the patient with minimal flexing and/or bending of printed circuit board 120 and electronic components 130, as indicated by arrows 186. Printed circuit board 120 and electronics components 130 that are separated from the breathable tape 110T with air gap 169 can allow the skin to release moisture as water vapor through the breathable tape, gel cover, and breathable cover. This release of moisture from the skin through the air gap can minimize, and even avoid, excess moisture, for example when the patient sweats and/or showers.

[0099] The breathable tape of adhesive patch 110 may comprise a first mesh with a first porosity and gel cover 180 may comprise a breathable tape with a second porosity, in which the second porosity is less than the first porosity to minimize, and even inhibit, flow of the gel through the breathable tape. The gel cover may comprise a polyurethane film with the second porosity.

[0100] In many embodiments, the adherent device comprises a patch component and at least one electronics module. The patch component may comprise adhesive patch 110 comprising the breathable tape with adhesive coating 116A, at least one electrode, for example electrode 114A and gel 114. The at least one electronics module can be separable from the patch component. In many embodiments, the at least one electronics module comprises the flex printed circuit board 120, electronic components 130, electronics housing 160 and cover 162, such that the flex printed circuit board, electronic components, electronics housing and cover are reusable and/or

removable for recharging and data transfer, for example as described above. In many
embodiments, adhesive 116B is coated on upper side 110A of adhesive patch 110B, such that the
electronics module can be adhered to and/or separated from the adhesive component. In specific
embodiments, the electronic module can be adhered to the patch component with a releasable
5 connection, for example with Velcro™, a known hook and loop connection, and/or snap directly
to the electrodes. Two electronics modules can be provided, such that one electronics module
can be worn by the patient while the other is charged, as described above. Monitoring with
multiple adherent patches for an extended period is described in U.S. Pat. App. No. 60/972,537,
the full disclosure of which is incorporated herein by reference and may be suitable for
10 combination with some embodiments of the present invention. Many patch components can be
provided for monitoring over the extended period. For example, about 12 patches can be used to
monitor the patient for at least 90 days with at least one electronics module, for example with
two reusable electronics modules.

[0101] At least one electrode 112A can extend through at least one aperture 180A in the
15 breathable tape 110 and gel cover 180.

[0102] In some embodiments, the adhesive patch may comprise a medicated patch that releases
a medicament, such as antibiotic, beta-blocker, ACE inhibitor, diuretic, or steroid to reduce skin
irritation. The adhesive patch may comprise a thin, flexible, breathable patch with a polymer
grid for stiffening. This grid may be anisotropic, may use electronic components to act as a
20 stiffener, may use electronics-enhanced adhesive elution, and may use an alternating elution of
adhesive and steroid.

[0103] Figure 1K shows at least one electrode 190 configured to electrically couple to a skin of
the patient through a breathable tape 192. In many embodiments, at least one electrode 190 and
breathable tape 192 comprise electrodes and materials similar to those described above.

25 Electrode 190 and breathable tape 192 can be incorporated into adherent devices as described
above, so as to provide electrical coupling between the skin and electrode through the breathable
tape, for example with the gel.

[0104] Figures 2A to 2C show a schematic illustration of a system 200 to monitor a patient for
an extended period.

30 [0105] Figure 2A shows a schematic illustration of system 200 comprising a reusable
electronics module 210 and a plurality of disposable patch components. Figure 2B shows a
schematic illustration of a side cross-sectional view of reusable electronics module 210. System

200 may comprise a first disposable patch component 220A, a second disposable patch component 220B, a third disposable patch component 220C and a fourth disposable patch component 220D. Although four patch components are shown the plurality may comprise as few as two patch component and as many as three or more patch components, for example 25 patch components.

[0106] Reusable electronics module 210 may comprise a connector 219 adapted to connect to each of the disposable patch components, sequentially, for example one disposable patch component at a time. Connector 219 can be formed in many ways, and may comprise known connectors as described above, for example a snap. In some embodiments, the connectors on the electronics module and adhesive component can be disposed at several locations on the reusable electronics module and disposable patch component, for example near each electrode, such that each electrode can couple directly to a corresponding location on the flex PCB of the reusable electronics component.

[0107] Reusable electronics module 210 may comprise additional reusable electronics modules, for example two or more rechargeable electronics modules each with a 3D accelerometer, such that the first module comprising a first 3D accelerometer can be recharged while the second module comprising a second 3D accelerometer is worn by the patient. The second module can be recharged and connected to a third adhesive patch when the first adhesive patch is removed from the patient. The second module comprising the second accelerometer can be removably coupled to the adhesive patch such that the second accelerometer can be recharged and connected to a fourth adhesive patch when the second adhesive patch is removed from the patient.

[0108] Reusable electronics module 210 may comprise many of the structures described above that may comprise the electronics module. In many embodiments, reusable electronics module 210 comprises a PCB, for example a flex PCB 212, electronics components 214, batteries 216, and a cover 217, for example as described above. In some embodiments, reusable electronics module 210 may comprise an electronics housing over the electronics components and/or PCB as described above. The electronics components may comprise circuitry and/or sensors for measuring ECG signals, hydration impedance signals, respiration impedance signals and accelerometer signals, for example as described above.

[0109] Electronics components 214 may comprise an accelerometer 214A. Accelerometer 214A may comprise a three axis accelerometer, for example as described above. Accelerometer

214A may comprise an X-axis 234X, a Y-axis 234Y and a Z-axis 234Z with each axis sensitive to gravity such that the orientation of the accelerometer, for example 3D orientation, can be determined in relation to gravity, as described above. Alignment of the accelerometer, for example the axes of the accelerometer 214A, can be aligned with the axes of the adherent patches using the connectors. For example connector 219 can connect with at least one of connector 229A, connector 229B, connector 229C and connector 229D to align the respective patch with accelerometer 214A.

[0110] First disposable patch component 220A comprises a connector 229A to mate with connector 219 on reusable electronics module 210 such that the first disposable patch component 220A is aligned with the reusable electronics module with a predetermined orientation. First disposable patch component 220A comprises a first axis 220AX substantially aligned with electrodes 222A. A second axis 220AZ corresponds to vertical on the patient when first disposable patch component 220A is adhered to the patient. Connector 229A is configured to mate with connector 219 such that axis 234X is aligned with first axis 220AX and axis 234Z is aligned with axis 220AZ.

[0111] Second disposable patch component 220B comprises a connector 229B to mate with connector 219 on reusable electronics module 210 such that the second disposable patch component 220B is aligned with the reusable electronics module with the predetermined orientation similar to first disposable patch component 220A. Second disposable patch component 220B comprises a first axis 220BX substantially aligned with electrodes 222B. A second axis 220BZ corresponds to vertical on the patient when second disposable patch component 220B is adhered to the patient. Connector 229B is configured to mate with connector 219 such that axis 234X is aligned with first axis 220BX and axis 234Z is aligned with axis 220BZ.

[0112] Third disposable patch component 220C comprises a connector 229C to mate with connector 219 on reusable electronics module 210 such that the third disposable patch component 220C is aligned with the reusable electronics module with the predetermined orientation similar to second disposable patch component 220B. Third disposable patch component 220C comprises a first axis 220CX substantially aligned with electrodes 222C. A second axis 220CZ corresponds to vertical on the patient when second disposable patch component 220C is adhered to the patient. Connector 229C is configured to mate with connector 219 such that axis 234X is aligned with first axis 220CX and axis 234Z is aligned with axis 220CZ.

[0113] Fourth disposable patch component 220D comprises a connector 229D to mate with connector 219 on reusable electronics module 210 such that the fourth disposable patch component 220D is aligned with the reusable electronics module with the predetermined orientation similar to third disposable patch component 220C. Fourth disposable patch component 220D comprises a first axis 220DX substantially aligned with electrodes 222D. A second axis 220DZ corresponds to vertical on the patient when second disposable patch component 220D is adhered to the patient. Connector 229D is configured to mate with connector 219 such that axis 234X is aligned with first axis 220DX and axis 234Z is aligned with axis 220DZ.

[0114] Figure 2C shows a schematic illustration first disposable patch component 220A of the plurality of disposable patch components that is similar to the other disposable patch components, for example second disposable patch component 220B, third disposable patch component 220C and fourth disposable patch component 220C. The disposable patch component comprises a breathable tape 227A, an adhesive 226A on an underside of breathable tape 227A to adhere to the skin of the patient, and at least four electrodes 222A. The at least four electrodes 224A are configured to couple to the skin of a patient, for example with a gel 226A, in some embodiments the electrodes may extend through the breathable tape to couple directly to the skin of the patient with aid form the gel. In some embodiments, the at least four electrodes may be indirectly coupled to the skin through a gel and/or the breathable tape, for example as described above. A connector 229A on the upper side of the disposable adhesive component can be configured for attachment to connector 219 on reusable electronics module 210 so as to electrically couple the electrodes with the electronics module. The upper side of the disposable patch component may comprise an adhesive 224A to adhere the disposable patch component to the reusable electronics module. The reusable electronics module can be adhered to the patch component with many additional known ways to adhere components, for example with Velcro™ comprising hooks and loops, snaps, a snap fit, a lock and key mechanisms, magnets, detents and the like.

[0115] Figure 2D shows a method 250 of using system 200, as in Figures 2A to 2C. A step 252 adheres electronics module 210 to first disposable adherent patch component 220A of the plurality of adherent patch components and adheres the first disposable patch component to the skin of the patient, for example with the first adherent patch component adhered to the reusable electronics module. The orientation on the patient of first disposable patch component 220A is determined with the accelerometer, for example as described above, when the first disposable

patch component is adhered to the patient. Patient measurements can be taken with the electronics module and/or adjusted in response to the orientation of the first patch on the patient. A step 254 removes the first disposable adherent patch from the patient and separates first disposable adherent patch component 220A from reusable electronics module 210.

- 5 **[0116]** A step 256 adheres electronics module 210 to second disposable adherent patch component 220B and adheres the second disposable patch component to the skin of the patient, for example with the second adherent patch component adhered to the reusable electronics module. The orientation on the patient of second disposable patch component 220B is determined with the accelerometer, for example as described above, when the second disposable
- 10 patch component is adhered to the patient. Patient measurements can be taken with the electronics module and/or adjusted in response to the orientation of the second patch on the patient. A step 258 removes the second disposable adherent patch from the patient and separates second disposable adherent patch component 220B from reusable electronics module 210.

- [0117]** A step 260 adheres electronics module 210 to third disposable adherent patch
- 15 component 220C and adheres the third disposable patch component to the skin of the patient, for example with the third adherent patch component adhered to the reusable electronics module. The orientation on the patient of third disposable patch component 220C is determined with the accelerometer, for example as described above, when the third disposable patch component is adhered to the patient. Patient measurements can be taken with the electronics module and/or
- 20 adjusted in response to the orientation of the third patch on the patient. A step 262 removes the third disposable adherent patch from the patient and separates third disposable adherent patch component 220C from reusable electronics module 210.

- [0118]** A step 264 adheres electronics module 210 to fourth disposable adherent patch component 220D and adheres the fourth disposable patch component to the skin of the patient,
- 25 for example with the third adherent patch component adhered to the reusable electronics module. The orientation on the patient of fourth disposable patch component 220D is determined with the accelerometer, for example as described above, when the fourth disposable patch component is adhered to the patient. Patient measurements can be taken with the electronics module and/or
- 30 adjusted in response to the orientation of the fourth patch on the patient. A step 268 removes the fourth disposable adherent patch from the patient and separates fourth disposable adherent patch component 220D from reusable electronics module 210.

[0119] In many embodiments, physiologic signals, for example ECG, hydration impedance, respiration impedance and accelerometer impedance are measured when the adherent patch component is adhered to the patient, for example when any of the first, second, third or fourth disposable adherent patches is adhered to the patient.

5 [0120] Figures 3A to 3D show a method 300 of monitoring a patient for an extended period with adherent patches alternatively adhered to a right side 302 and a left side 304 of the patient. Work in relation to embodiments of the present invention suggests that repeated positioning of a patch at the same location can irritate the skin and may cause patient discomfort. This can be minimized, even avoided, by alternating the patch placement between left and right sides of the
10 patient, often a front left and a front right side of the patient where the patient can reach easily to replace the patch. In some embodiments, the patch location can be alternated on the same side of the patient, for example higher and/or lower on the same side of the patient without substantial overlap to allow the skin to recover and/or heal. In many embodiments, the patch can be
15 symmetrically positioned on an opposite side such that signals may be similar to a previous position of the patch symmetrically disposed on an opposite side of the patient. In many embodiments, the duration between removal of one patch and placement of the other patch can be short, such that any differences between the signals may be assumed to be related to placement of the patch, and these differences can be removed with signal processing.

[0121] In many embodiments each patch comprises at least four electrodes configured to
20 measure an ECG signal and impedance, for example hydration and/or respiration impedance. In many embodiments, the patient comprises a midline 306, with first side, for example right side 302, and second side, for example left side 304, symmetrically disposed about the midline. A step 310 adheres a first adherent patch 312 to at a first location 314 on a first side 302 of the patient for a first period of time, for example about 1 week. When the adherent patch 312 is
25 position at first location 314 on the first side of the patient, the accelerometer signals are measured to determine the orientation of the patch and the electrodes of the patch are coupled to the skin of the patient to measure the ECG signal and impedance signals.

[0122] A step 320 removes patch 312 and adheres a second adherent patch 322 at a second
location 324 on a second side 206 of the patient for a second period of time, for example about 1
30 week. In many embodiments, second location 324 can be symmetrically disposed opposite first location 314 across midline 304, for example so as to minimize changes in the sequential impedance signals measured from the second side and first side. When adherent patch 322 is position at second location 324 on the second side of the patient, the orientation of the patch can

be measured with the accelerometer and the electrodes of the patch are coupled to the skin of the patient to measure the ECG signal and impedance signals. In many embodiments, while adherent patch 322 is positioned at second location 324, skin at first location 314 can heal and recover from adherent coverage of the first patch. In many embodiments, second location 324 is
5 symmetrically disposed opposite first location 314 across midline 304, for example so as to minimize changes in the impedance signals measured between the first side and second side. In many embodiments, the duration between removal of one patch and placement of the other patch can be short, such that any differences between the signals may be determined to be related to orientation of the patch, and these differences can be corrected in response to the measured
10 orientation of the patch on the patient.

[0123] A step 330 removes second patch 322 and adheres a third adherent patch 332 at a third location 334 on the first side, for example right side 302, of the patient for a third period of time, for example about 1 week. In many embodiments, third location 334 can be symmetrically
15 disposed opposite second location 324 across midline 304, for example so as to minimize changes in the sequential impedance signals measured from the third side and second side. In many embodiments, third location 334 substantially overlaps with first location 314, so as to minimize differences in measurements between the first adherent patch and third adherent patch that may be due to patch location. When adherent patch 332 is positioned at third location 334
20 on the first side of the patient, the orientation of the patch is measured with the accelerometer and the electrodes of the patch are coupled to the skin of the patient to measure the ECG signal and impedance signals. In many embodiments, while adherent patch 332 is positioned at third location 334, skin at second location 324 can heal and recover from adherent coverage of the second patch. In many embodiments, the duration between removal of one patch and placement of the other patch can be short, such that differences between the signals may be determined to
25 be related to orientation of the patch, and these differences can be corrected in response to the measured orientation of the patch on the patient.

[0124] A step 340 removes third patch 332 and adheres a fourth adherent patch 342 at a fourth location 344 on the second side, for example left side 306, of the patient for a fourth period of time, for example about 1 week. In many embodiments, fourth location 344 can be
30 symmetrically disposed opposite third location 334 across midline 304, for example so as to minimize changes in the sequential impedance signal measured from the fourth side and third side. In many embodiments, fourth location 344 substantially overlaps with second location 324, so as to minimize differences in measurements between the second adherent patch and fourth

adherent patch that may be due to patch location. When adherent patch 342 is positioned at fourth location 344 on the second side of the patient, the orientation of patch is measured with the accelerometer and the electrodes of the patch are coupled to the skin of the patient to measure the ECG signal and impedance signals. In many embodiments, while adherent patch 342 is positioned at fourth location 324, skin at third location 334 can heal and recover from adherent coverage of the third patch. In many embodiments, the duration between removal of one patch and placement of the other patch can be short, such that differences between the signals may be determined to be related to orientation of the patch, and these differences can be corrected in response to the measured orientation of the patch on the patient.

[0125] The accelerometer signal measured to determine the orientation on the patient for each of adherent patch 312, adherent patch 322, adherent patch 332 or adherent patch 342 can be measured with a reusable accelerometer of a reusable electronics module, for example as described above, or measured with a disposable accelerometer affixed to each patch and disposed of with the patch after the patch is removed from the patient.

[0126] It should be appreciated that the specific steps illustrated in Figures 3A to 3D provide a particular method of monitoring a patient for an extended period, according to an embodiment of the present invention. Other sequences of steps may also be performed according to alternative embodiments. For example, alternative embodiments of the present invention may perform the steps outlined above in a different order. Moreover, the individual steps illustrated in Figures 3A to 3D may include multiple sub-steps that may be performed in various sequences as appropriate to the individual step. Furthermore, additional steps may be added or removed depending on the particular applications. One of ordinary skill in the art would recognize many variations, modifications, and alternatives.

[0127] Figure 4A shows a method 400 of monitoring a patient. A step 405 adheres a first adherent patch to the patient, for example an adherent patch as described above. The first adherent patch may comprise a first patch that is separable from an electronics module, as described above. The first adherent patch may comprise a first patch of a first device with the electronics module fixed to the adherent patch, for example disposable electronics with a disposable patch.

[0128] A step 410A measures a first accelerometer signal along a first axis, for example an X-axis of a 3D accelerometer responsive to gravity as described above. A step 410B measures a first accelerometer signal along a second axis, for example a y-axis of a 3D accelerometer as

described above. A step 410C measures a first accelerometer signal along a third axis, for example a Z-axis of a 3D accelerometer as described above. Measurement of the accelerometer signal with step 410A, step 410B and step 41C, which may comprise sub-steps, can be performed with the patient in a known and/or determined position. The patient may be asked to stand and/or sit upright in a chair and the first signal measured. In some embodiments, the 3D accelerometer signal can be analyzed to determine that the patient is standing, walking and the first signal determined from a plurality of measurements to indicate that the patient is upright for the measurement of the first signal.

[0129] A step 415 determines an orientation of the first patch on the patient. The accelerometer can be coupled to the patch with a pre-determined orientation, for example with connectors as described above, such that the orientation of the patch can be determined from the accelerometer signal and the orientation of the 3D accelerometer on the adherent patch and the orientation of the patient.

[0130] A step 420 measures a first ECG signal. The first ECG signal can be measured with the electrodes attached to the patient when the patch comprises the first orientation. The ECG signal can be measured with electronics components and electrodes, as described above.

[0131] A step 425 determines a first orientation of an electrode measurement axis on the patient. The electrode measurement axis may correspond to one of the measurement axes of the 3D accelerometer, for example an X-axis of the accelerometer as described above. However, the orientation of the electrode measurement axis can be aligned in relation to the axes of the accelerometer in many ways, for example at oblique angles, such that the alignment of the accelerometer with the electrode measurement axis is known and the signal from the accelerometer can be used to determine the alignment of the electrode measurement axis.

[0132] A step 430 determines a first orientation of the ECG vector. The orientation of the ECG vector can be determined in response to the polarity of the measurement electrodes and orientation of the electrode measurement axis, as described above.

[0133] A step 435 rotates a first ECG vector. The first ECG vector orientation of the ECG vector can be used to rotate the ECG vector onto a desired axis, for example an X-axis of the patient in response to the first orientation of the ECG vector and the accelerometer signal. For example, if the first measurement axis of the first ECG vector is rotated five degrees based on the accelerometer signal, the first ECG vector can be rotated by five degrees so as to align the first ECG vector with the patient axis.

[0134] A step 440 measures a first patient temperature. The first temperature of the patient can be measured with electronics of the adherent device, as described above.

[0135] A step 445 measures a first patient impedance. The first patient impedance may comprise a four pole impedance measurement, as described above. The first patient impedance
5 can be used to determine respiration of the patient and/or hydration of the patient.

[0136] A step 450 adheres a second patch to the patient. The second patch may comprise a second patch connected to a reusable electronics module, for example a reusable electronics module connected to the first patch for the first patient measurements above. The second patch may comprise a second patch of a second adherent device comprising a second electronics
10 module in which the second patch and second electronics module comprise a disposable second adherent device and the first adherent patch and first electronics module comprise a first disposable adherent device.

[0137] A step 455A measures a second accelerometer signal along a first axis, for example an x-axis of the accelerometer as described above. The first axis may comprise the first axis of the
15 first accelerometer as described above, for example the X-axis of the accelerometer used to measure the X-axis signal with the first measurement. In some embodiments, the second accelerometer signal along the first axis may comprise an X-axis of a second accelerometer, for example a second disposable electronics module, aligned with an electrode measurement axis as described above.

[0138] A step 455B measures a second accelerometer signal along a second axis. The second axis may comprise the second axis of the first accelerometer as described above, for example the Y-axis of the accelerometer used to measure the Y-axis signal with the first measurement. In
20 some embodiments, the second accelerometer signal along the second axis may comprise a Y-axis of a second accelerometer, for example a second disposable electronics module, aligned
25 with an electrode measurement axis as described above.

[0139] A step 455C measures a second accelerometer signal along a third axis. The third axis may comprise the third axis of the first accelerometer as described above, for example the Z-axis of the accelerometer used to measure the Z-axis signal with the first measurement. In some
30 embodiments, the second accelerometer signal along the third axis may comprise a Z-axis of a second accelerometer, for example a second disposable electronics module, aligned with an electrode measurement axis as described above.

[0140] A step 460 determines an orientation of the second patch on the patient. The accelerometer can be coupled to the second patch with a pre-determined orientation, for example with connectors as described above, such that the orientation of the second patch can be determined from the second accelerometer signal and the orientation of the 3D accelerometer on the adherent patch and the orientation of the patient.

[0141] A step 465 measures a second ECG signal. The second ECG signal can be measured with the electrodes attached to the patient when the second patch comprises the second orientation, for example after the first patch has been removed and the second patch has been positioned on the patient as described above. The ECG signal can be measured with electronics components and electrodes, as described above.

[0142] A step 470 determines a second orientation of the electrode measurement axis on the patient. The second orientation of the electrode measurement axis may comprise orientation of an axis of a second set of electrodes, for example a second set of electrodes disposed along an axis of the second patch. The second orientation of the electrode measurement axis may correspond to one of the measurement axes of the 3D accelerometer, for example an X-axis of the accelerometer as described above. However, the second orientation of the electrode measurement axis can be aligned in relation to the axes of the accelerometer in many ways, for example at oblique angles, such that the alignment of the accelerometer with the second electrode measurement axis is known and the signal from the accelerometer can be used to determine the alignment of the electrode measurement axis.

[0143] A step 475 determines a second orientation of the ECG vector. The second orientation of the ECG vector can be determined in response to the polarity of the second measurement electrodes and second orientation of the electrode measurement axis, for example second measurement electrodes on the second adherent patch that extend along the electrode measurement axis of the second adherent patch.

[0144] A step 480 rotates a second ECG vector. The second ECG vector orientation of the second ECG vector can be used to rotate the second ECG vector onto the desired axis, for example the X-axis of the patient in response to the first orientation of the ECG vector and the accelerometer signal. For example, if the first measurement axis of the first ECG vector is rotated five degrees from the X-axis based on the accelerometer signal, the first ECG vector can be rotated by five degrees so as to align the first ECG vector with the X-axis of the patient, for example the horizontal axis of the patient.

[0145] A step 485 measures a second patient temperature. The second temperature of the patient can be measured with electronics of the adherent device, as described above.

[0146] A step 490 measures a second patient impedance. The second patient impedance may comprise a four pole impedance measurement, as described above. The second patient
5 impedance can be used to determine respiration of the patient and/or hydration of the patient.

[0147] A step 495 repeats the above steps. The above steps can be repeated to provide longitudinal monitoring of the patient with differential measurement of patient status. The monitoring of the patient may comprise a comparison of baseline patient data with subsequent patient date.

10 [0148] Many of the steps of method 400 can be performed with the processor system, as described above.

[0149] It should be appreciated that the specific steps illustrated in Figure 4A provides a particular method of monitoring a patient, according to an embodiment of the present invention. Other sequences of steps may also be performed according to alternative embodiments. For
15 example, alternative embodiments of the present invention may perform the steps outlined above in a different order. Moreover, the individual steps illustrated in Figure 4A may include multiple sub-steps that may be performed in various sequences as appropriate to the individual step. Furthermore, additional steps may be added or removed depending on the particular applications. One of ordinary skill in the art would recognize many variations, modifications, and alternatives.

20 [0150] While the exemplary embodiments have been described in some detail, by way of example and for clarity of understanding, those of skill in the art will recognize that a variety of modifications, adaptations, and changes may be employed. Hence, the scope of the present invention should be limited solely by the appended claims.

WHAT IS CLAIMED IS:

1 1. A method of monitoring a patient, the method comprising:
2 adhering an adherent device to a skin of the patient, the adherent device
3 comprising an accelerometer and at least two measurement electrodes, the at least two
4 measurement electrodes separated by a distance to define an electrode measurement axis;
5 measuring an accelerometer signal when the device is adhered to the patient;
6 and
7 determining an orientation of the electrode measurement axis on the patient in
8 response to the accelerometer signal.

1 2. The method of claim 1 wherein the accelerometer comprises at least
2 one measurement axis sensitive to gravity aligned with the electrode measurement axis.

1 3. The method of claim 1 wherein the accelerometer comprises at least
2 one accelerometer measurement axis sensitive to gravity, the at least one accelerometer
3 measurement axis configured to extend substantially horizontally on the patient when the
4 device is adhered to the patient.

1 4. The method of claim 1 wherein the accelerometer signal correspond to
2 at least one accelerometer measurement vector in a direction along the at least one
3 accelerometer measurement axis.

1 5. The method of claim 1 wherein the accelerometer comprises at least
2 one accelerometer measurement axis sensitive to gravity and wherein the at least one
3 accelerometer measurement axis is oriented with respect to the electrode measurement axis in
4 a predetermined configuration.

1 6. The method of claim 1 wherein the at least two electrodes comprise a
2 positive electrode and a negative electrode that define an orientation of an electrode
3 measurement vector along the electrode measurement axis.

1 7. The method of claim 6 wherein the accelerometer signal corresponds
2 to at least one accelerometer measurement vector that extends away from the electrode
3 measurement axis and wherein the at least one accelerometer measurement vector is sensitive

4 to gravity such that the accelerometer signal indicates when the patch adhered to the patient is
5 upside down.

1 8. The method of claim 1 wherein the adherent device comprises an
2 adherent surface to adhere to a skin of the patient and wherein the electrode measurement
3 axis extends along the adherent surface.

1 9. The method of claim 1 wherein the accelerometer comprises three axes
2 and wherein a first axis and a second axis of the three axes extend along the measurement
3 surface and wherein a third axis of the three axes extends away from the measurement
4 surface.

1 10. The method of claim 9 wherein the accelerometer measurement signal
2 corresponds to three orthogonal measurement vectors and wherein each of the three
3 orthogonal measurement vectors extends along one of the accelerometer measurement axes.

1 11. The method of claim 1 further comprising measuring an
2 electrocardiogram signal with the at least two measurement electrodes and modifying the
3 electrocardiogram signal in response to the accelerometer signal.

1 12. The method of claim 11 wherein modifying comprises rotating the
2 electrocardiogram vector in response to the accelerometer signal to obtain a standard
3 electrocardiogram vector.

1 13. The method of claim 12 wherein an amplitude and a direction of
2 features of the electrocardiogram signal are modified to approximate a standard
3 electrocardiogram vector.

1 14. A method of monitoring a patient, the method comprising:
2 adhering a first adherent patch to a skin of the patient, the first patch
3 comprising an adhesive and electrodes;
4 measuring a first accelerometer signal when the first adherent patch is adhered
5 to the patient;
6 adhering a second adherent patch to the skin of the patient, the second patch
7 comprising an adhesive and electrodes;

8 measuring a second accelerometer signal when the second adherent patch is
9 adhered to the patient; and
10 determining an orientation on the patient of at least one of the first patch or the
11 second patch in response to at least one of the first accelerometer signal or the second
12 accelerometer signal.

1 15. The method of claim 14 further comprising:
2 measuring a first electrocardiogram signal when the first adherent patch is
3 adhered to the patient;
4 measuring a second electrocardiogram signal when the second adherent patch
5 is adhered to the patient; and
6 adjusting at least one of the first electrocardiogram signal or the second
7 electrocardiogram signal in response to at least one of the first accelerometer signal or the
8 second accelerometer signal.

1 16. A method of monitoring a patient, the method comprising:
2 adhering a first adherent measurement device to a skin of the patient, the first
3 adherent measurement device comprising a first accelerometer and a first at least two
4 measurement electrodes;
5 adhering a second adherent measurement device to a skin of the patient, the
6 second adherent measurement device comprising a second accelerometer and a second at
7 least two measurement electrodes;
8 measuring a first accelerometer signal and a first electrocardiogram signal
9 with the first at least two measurement electrodes when the first adherent measurement
10 device is adhered to the skin of the patient;
11 measuring a second accelerometer signal and a second electrocardiogram
12 signal with the second at least two measurement electrodes when the second adherent
13 measurement device is adhered to the skin of the patient; and
14 combining the first electrocardiogram signal with the second
15 electrocardiogram signal in response to the first accelerometer signal and the second
16 accelerometer signal.

1 17. The method of claim 16 wherein the processor is configured to scale
2 each of the first electrocardiogram signal and the second electrocardiogram signal to a scaled

3 version of each signal and combine the scaled version of each signal to form a combined
4 signal.

1 18. The method of claim 16 wherein the first accelerometer comprises a
2 first accelerometer measurement axis and the first at least two electrodes are separated by a
3 first distance to define a first electrode measurement axis, the first accelerometer
4 measurement axis aligned with the first electrode measurement axis, and wherein the second
5 accelerometer comprises a second accelerometer measurement axis and the second at least
6 two electrodes are separated by a second distance to define a second electrode measurement
7 axis, the second accelerometer measurement axis aligned with the second electrode
8 measurement axis.

1 19. The method of claim 16 further comprising:
2 determining an orientation of the first electrode measurement axis in response
3 to the first accelerometer signal; and
4 determining an orientation of the second electrode measurement axis in
5 response to the to the accelerometer signal.

1 20. The method of claim 16 wherein the first electrocardiogram signal is
2 combined with the second electrocardiogram signal when the second adherent measurement
3 device is adhered to the skin of the patient.

1 21. A device for monitoring a patient, the device comprising:
2 a support with an adhesive to adhere to a skin of the patient;
3 an accelerometer to generate an accelerometer signal supported with the
4 support;
5 at least two measurement electrodes supported with the support, the at least
6 two measurement electrodes separated by a distance to define an electrode measurement axis;
7 circuitry to measure the accelerometer signal when the device is adhered to the
8 patient; and
9 a processor comprising a tangible medium configured to determine an
10 orientation of the electrode measurement axis on the patient in response to the accelerometer
11 signal.

1 22. The device of claim 21 wherein the support comprises an adhesive
2 patch with an adhesive to adhere the support to the patient.

1 23. The device of claim 22 wherein the adhesive patch comprises a
2 breathable tape with adhesive to adhere the support to the patient.

1 24. The device of claim 21 wherein the accelerometer comprises at least
2 one measurement axis sensitive to gravity aligned with the electrode measurement axis.

1 25. The device of claim 21 wherein the accelerometer comprises at least
2 one accelerometer measurement axis sensitive to gravity and wherein the accelerometer is
3 positioned and supported with the support such that the measurement axis extends
4 substantially horizontally on the patient when the support is adhered to the patient.

1 26. The device of claim 21 wherein the accelerometer signal corresponds
2 to at least one accelerometer measurement vector along the at least one accelerometer
3 measurement axis.

1 27. The device of claim 21 wherein the accelerometer comprises at least
2 one accelerometer measurement axis sensitive to gravity and wherein the at least one
3 accelerometer measurement axis is oriented with respect to the electrode measurement axis in
4 a predetermined configuration.

1 28. The device of claim 21 wherein the at least two electrodes comprise a
2 positive electrode and a negative electrode that define an orientation of an electrode
3 measurement vector along the electrode measurement axis.

1 29. The device of claim 28 wherein the accelerometer signal corresponds
2 to at least one measurement vector that extends away from the electrode measurement axis
3 such that the accelerometer signal indicates when the patch adhered to the patient is upside
4 down.

1 30. The device of claim 21 wherein the adherent device comprises an
2 adherent surface to adhere to a skin of the patient and wherein the electrode measurement
3 axis extends along the adherent surface.

1 31. The device of claim 21 wherein the accelerometer comprises three axes
2 and wherein a first axis and a second axis of the three axes extend along the adherent surface
3 and wherein a third axis of the three axes extends away from the adherent surface.

1 32. The device of claim 21 wherein the accelerometer signal corresponds
2 to three orthogonal measurement vectors and wherein each of the three orthogonal
3 measurement vectors extends along one of the accelerometer measurement axes.

1 33. The device of claim 21 further comprising:
2 measurement circuitry coupled to the at least two measurement electrode to
3 measure an electrocardiogram signal;
4 a processor coupled to the measurement circuitry and comprising a tangible
5 medium configured to modify the electrocardiogram signal in response to the accelerometer
6 signal.

1 34. A system for monitoring a patient, the system comprising:
2 a first support with a first adhesive to adhere the first support to a skin of the
3 patient,
4 first electrodes supported with the first support to couple to the skin of the
5 patient;
6 a second support with a second adhesive to adhere the second support to the
7 skin of the patient,
8 second electrodes supported with the second support to couple to the skin of
9 the patient;
10 at least one accelerometer coupled to at least one of the first support or the
11 second support to determine an orientation of at least one of the first electrodes or the second
12 electrodes when the at least one of the first electrodes or the second electrodes are coupled to
13 the patient.

1 35. The system of claim 34 wherein the at least one accelerometer
2 comprises a first accelerometer removably coupled to the first support in a first
3 predetermined orientation and a second accelerometer removably coupled to the second
4 support in a second predetermined orientation.

1 36. The system of claim 34 wherein the at least one accelerometer
2 comprises an accelerometer removably coupled to the first support in a first predetermined
3 orientation and wherein the accelerometer is removably coupled to the second support in a
4 second predetermined orientation such that the accelerometer can be reused.

1 37. The system of claim 37 wherein the first predetermined orientation is
2 substantially similar to the second predetermined orientation.

1 38. The system of claim 34 wherein the at least one accelerometer
2 comprises a first accelerometer connected to the first support in a first predetermined
3 orientation and a second accelerometer connected to the second support in a second
4 predetermined configuration.

1 39. The system of claim 38 wherein first accelerometer is removably
2 connected to the first support such the first accelerometer can be recharged and connected to
3 a third support when first support is removed from the patient and wherein the second
4 accelerometer is removably coupled to the second support such that the second accelerometer
5 can be recharged and connected to a fourth support when the second support is removed from
6 the patient.

1 40. The system of claim 38 wherein first accelerometer is affixed to the
2 first support such the first accelerometer is disposable with first support when first support is
3 removed from the patient and wherein the second accelerometer is affixed to the second
4 support such that the second accelerometer is disposable with the second support when the
5 second support is removed from the patient.

1 41. The system of claim 34 wherein the first support with the first adhesive
2 comprises a first breathable tape and the second support with the second adhesive comprises
3 a second breathable tape.

1 42. A system monitoring a patient, the system comprising:
2 a first adherent measurement device comprising a first support with a first
3 adhesive to adhere the first support to a skin of the patient, the first adherent measurement
4 device comprising a first accelerometer and a first at least two measurement electrodes, the
5 first adherent device comprising first measurement circuitry to measure a first accelerometer
6 signal with the accelerometer and a first electrocardiogram signal with the first at least two
7 measurement electrodes;

8 a second adherent measurement device comprising a second support with a
9 second adhesive to adhere the second support to a skin of the patient, the second adherent
10 measurement device comprising a second accelerometer and a second at least two

11 measurement electrodes, the second accelerometer comprising second circuitry to measure a
12 second accelerometer signal with the second accelerometer and a second electrocardiogram
13 signal with the second at least two measurement electrodes; and
14 a processor system comprising a tangible medium configured to combine the
15 first electrocardiogram signal with the second electrocardiogram signal in response to the first
16 accelerometer signal and the second accelerometer signal.


1 43. The system of claim 42 wherein the first accelerometer comprises a
2 first accelerometer measurement axis and the first at least two electrodes are separated by a
3 first distance to define a first electrode measurement axis, the first accelerometer
4 measurement axis aligned with the first electrode measurement axis, and wherein the second
5 accelerometer comprises a second accelerometer measurement axis and the second at least
6 two electrodes are separated by a second distance to define a second electrode measurement
7 axis, the second accelerometer measurement axis aligned with the second electrode
8 measurement axis.

1 44. The system of claim 42 wherein the processor system is configured to
2 determine an orientation of the first electrode measurement axis in response to the first
3 accelerometer signal and determine an orientation of the second electrode measurement axis
4 in response to the to the accelerometer signal.

1 45. The system of claim 42 wherein the processor system comprises at
2 least one processor supported with at least one of the first support or the second support, the
3 at least one processor configured to combine the first electrocardiogram signal and the second
4 electrocardiogram signal in response to the first accelerometer signal and the second
5 accelerometer signal.

1 46. The system of claim 42 wherein the processor is configured to scale
2 each signal and sum the scaled signals together to combine the signals.

1 / 14

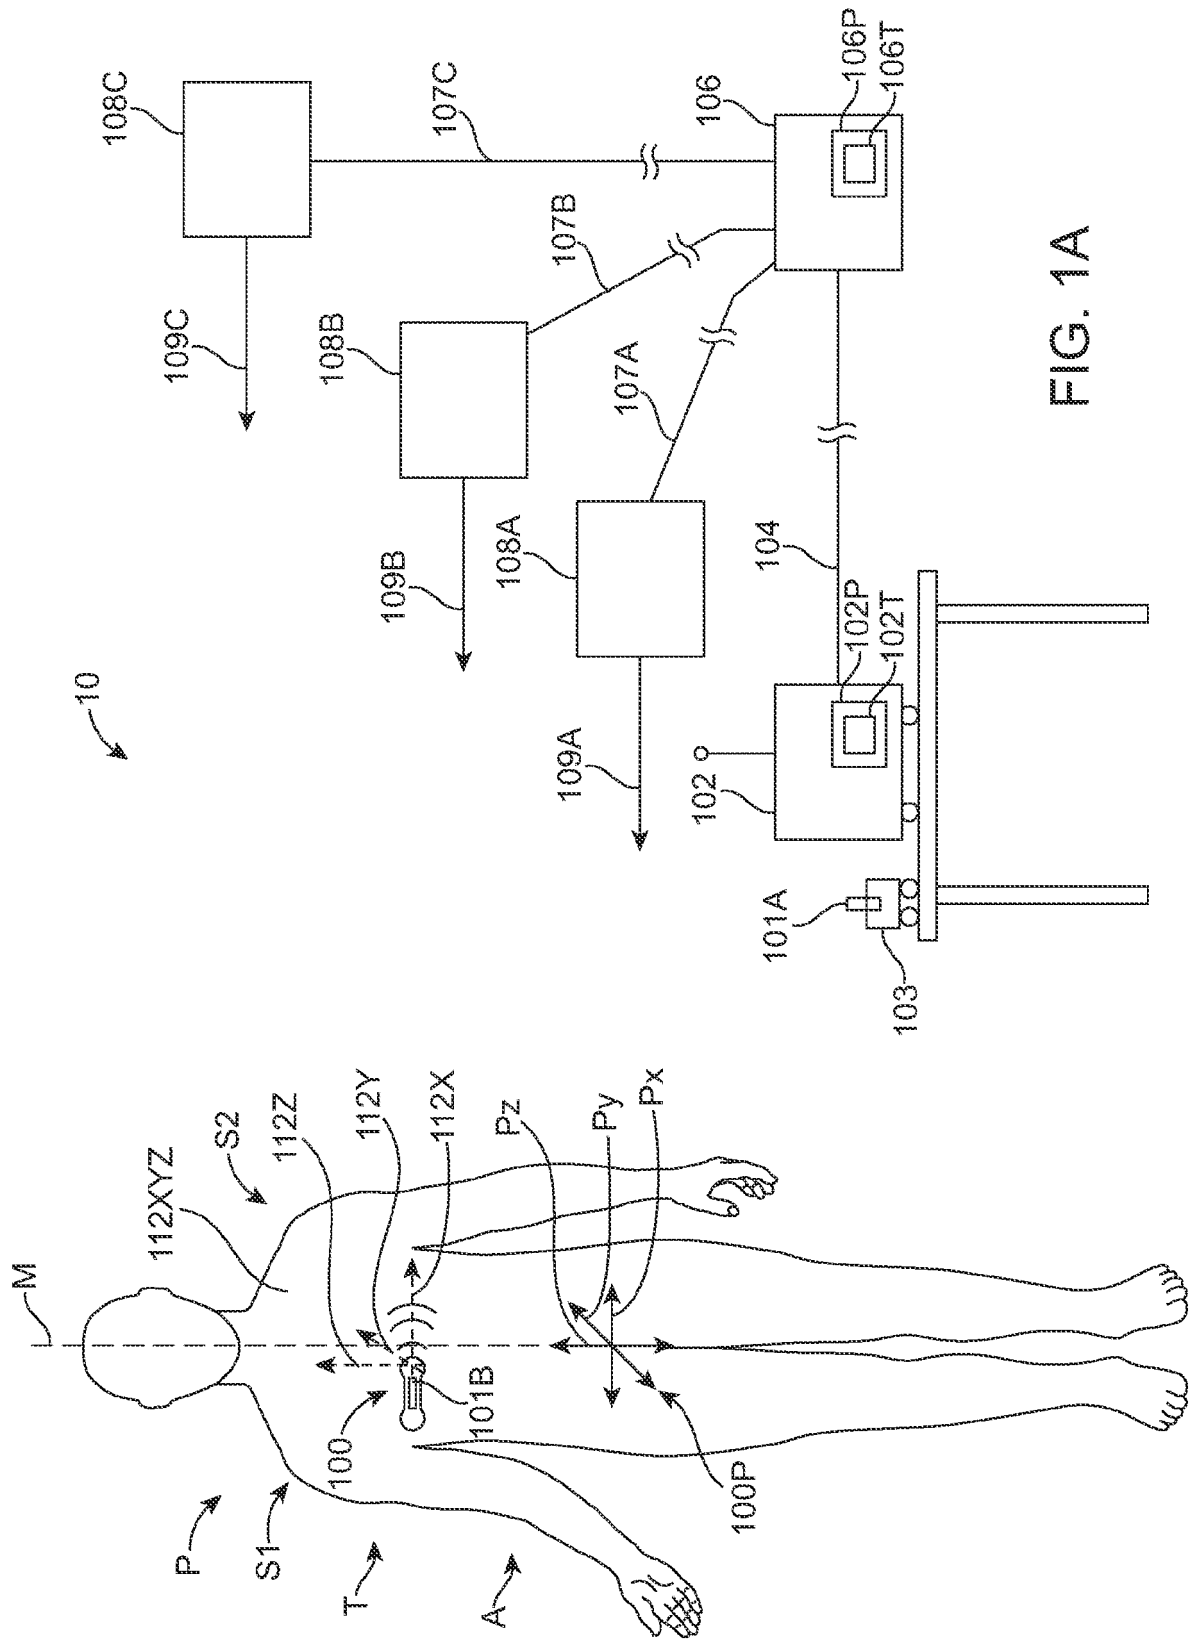

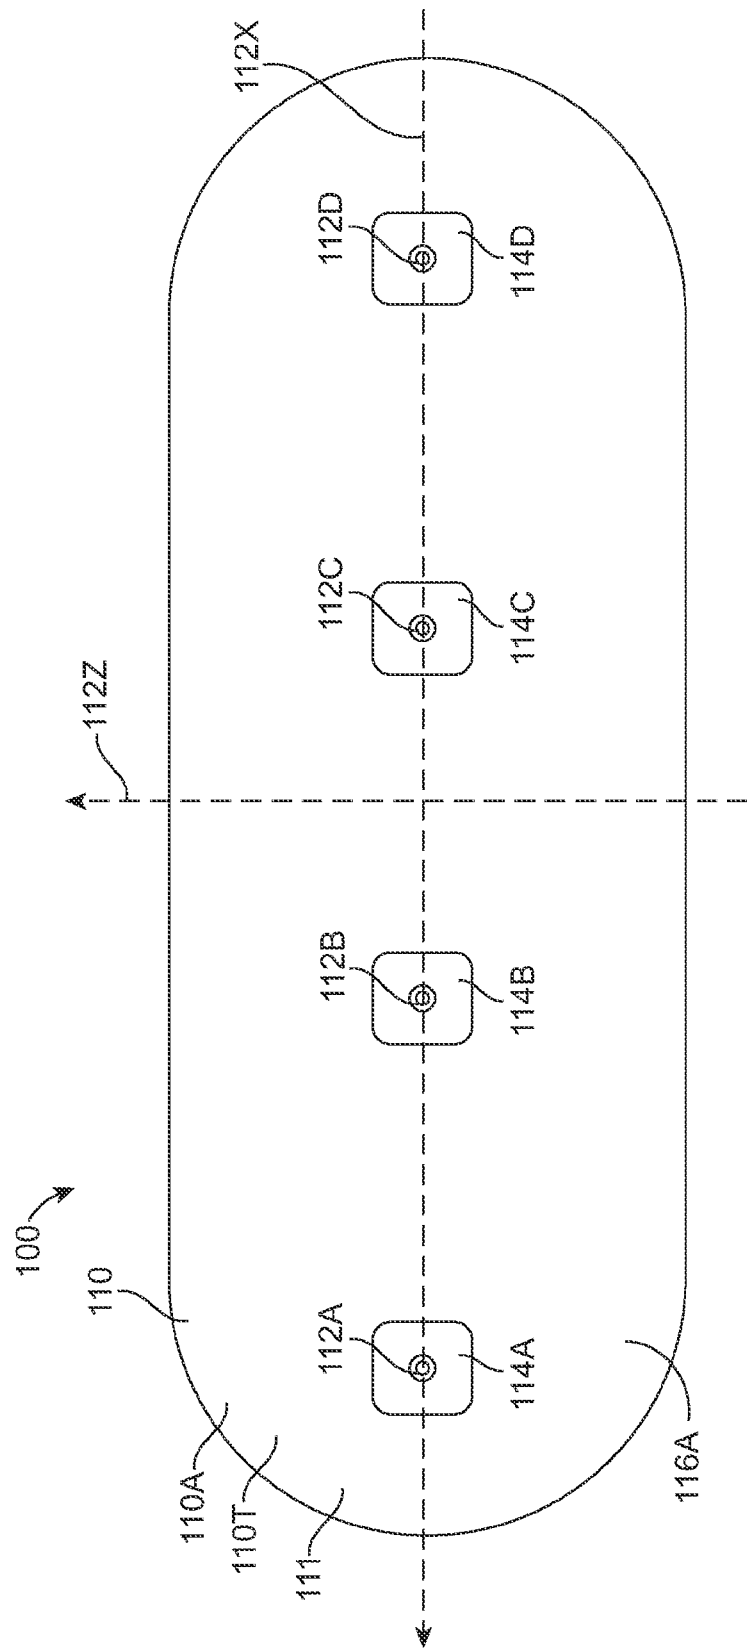


FIG. 1B



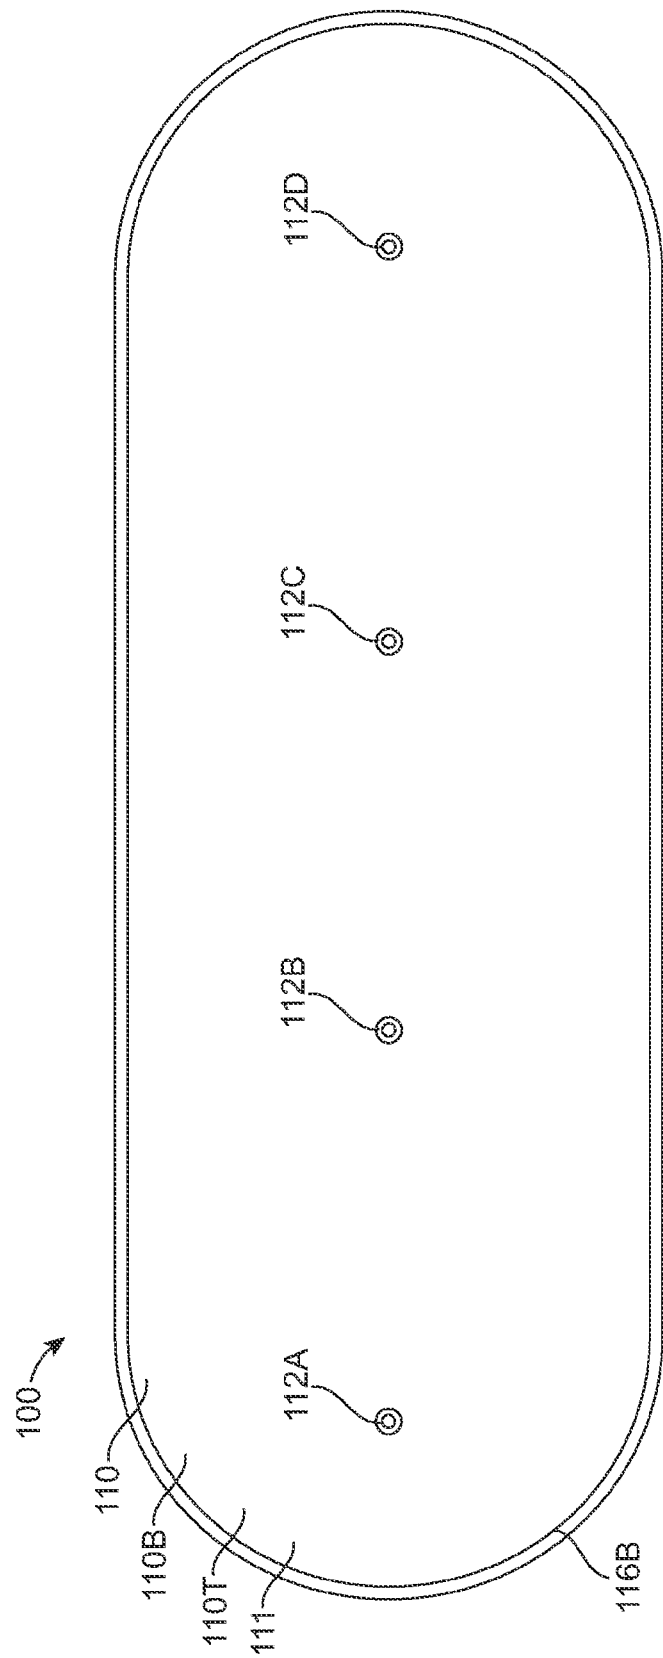


FIG. 1C

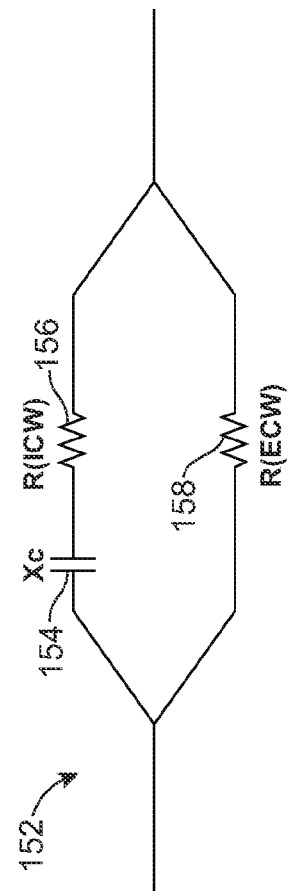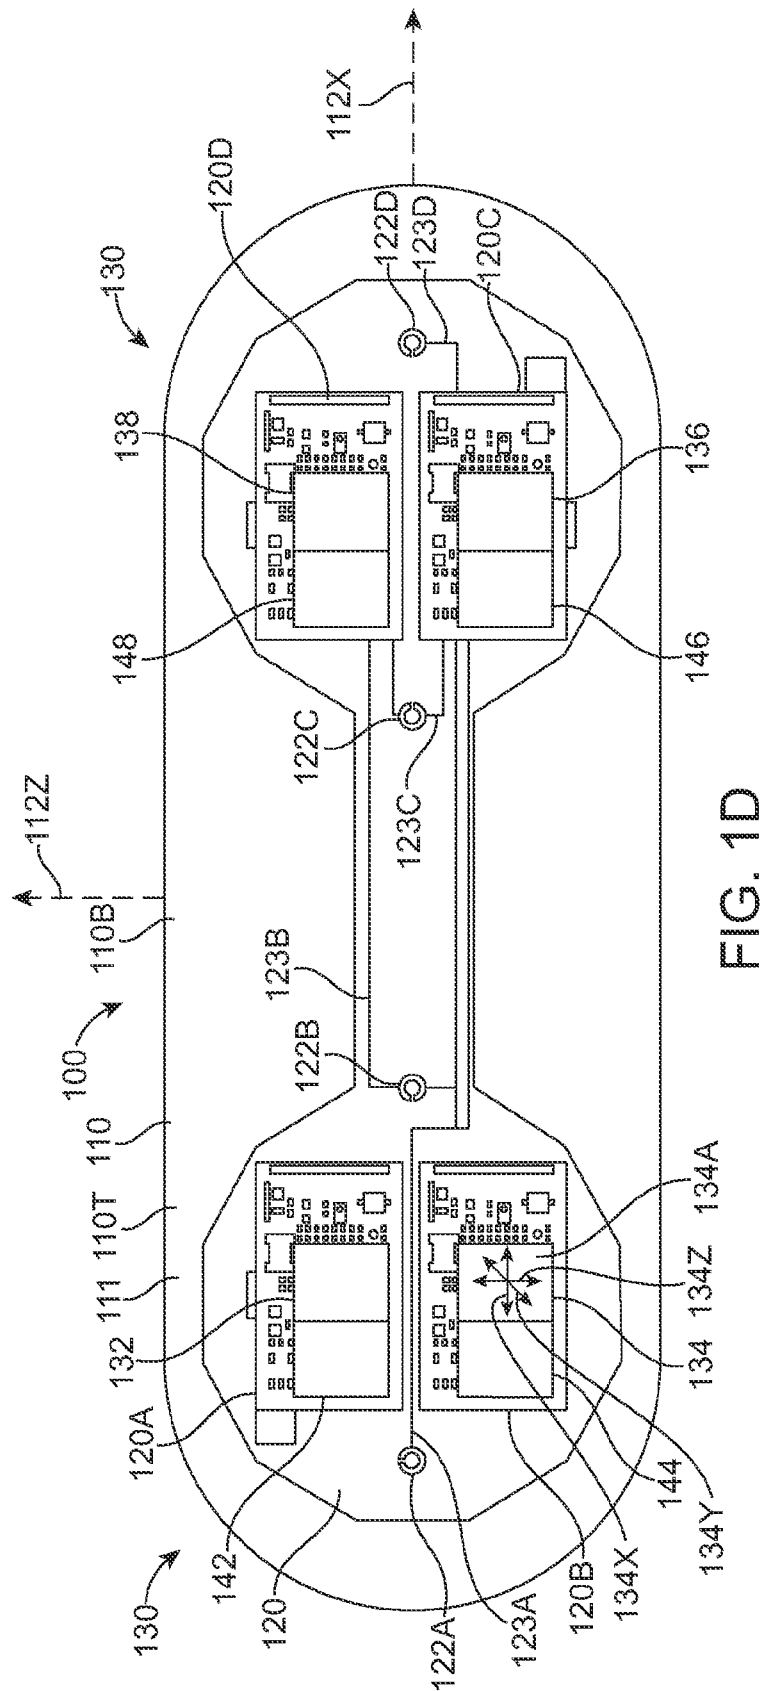

5 / 14

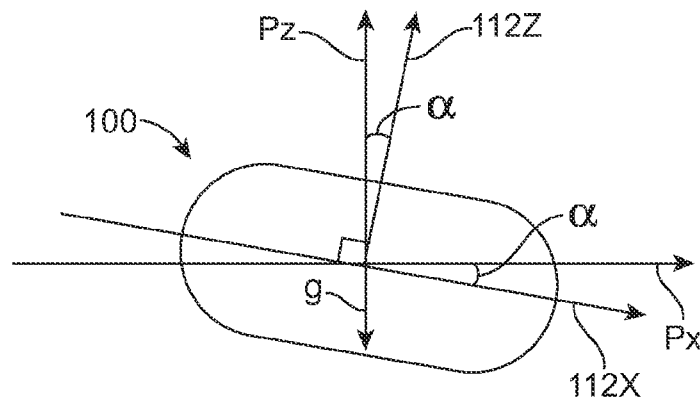


FIG. 1D2

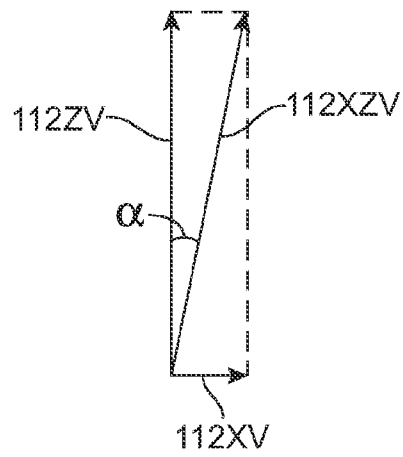


FIG. 1D3

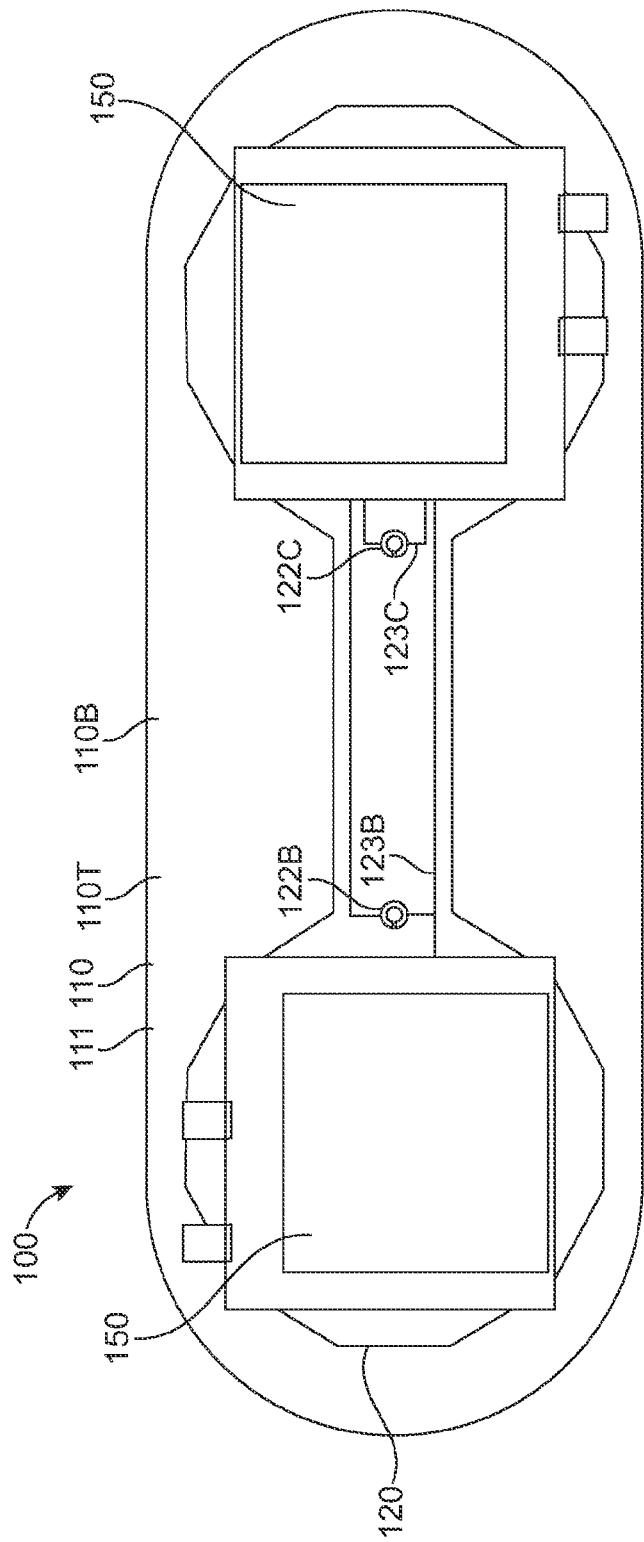


FIG. 1E

7 / 14

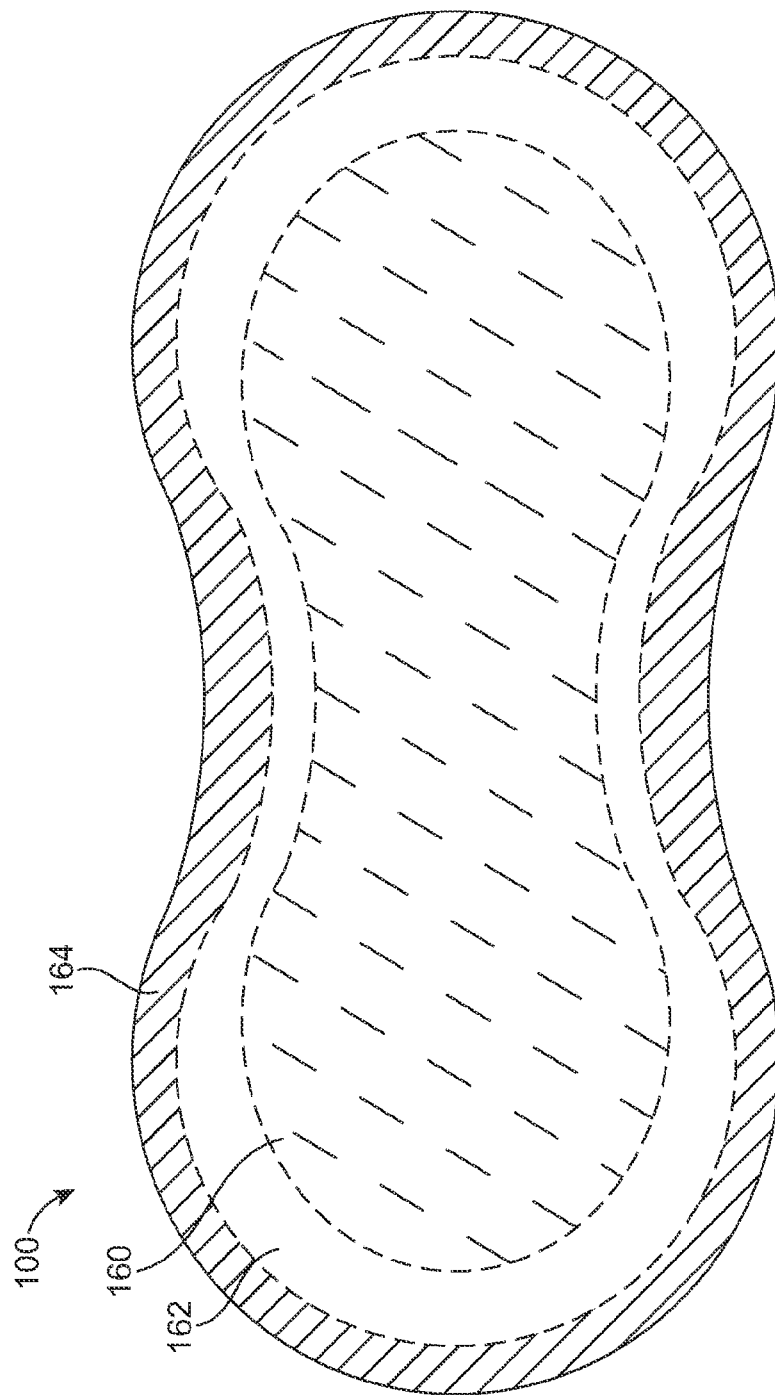


FIG. 1F

8 / 14

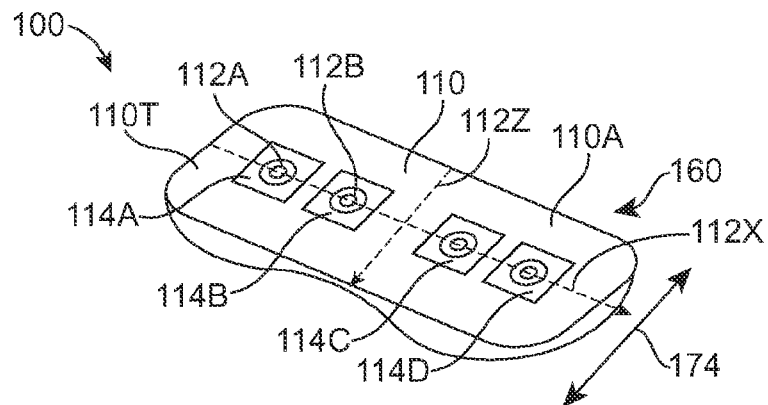


FIG. 1H

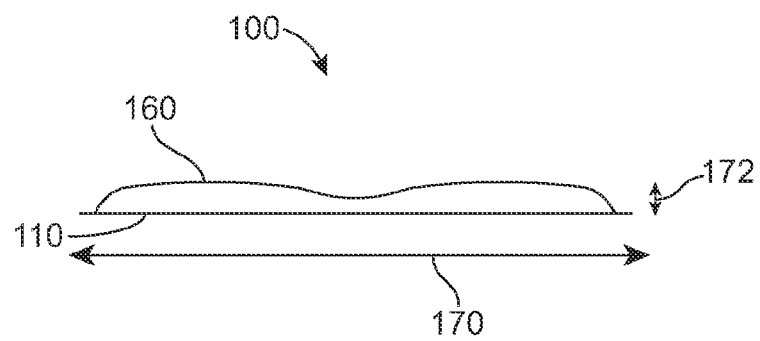


FIG. 1G

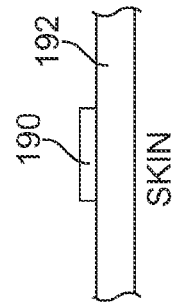


FIG. 1K

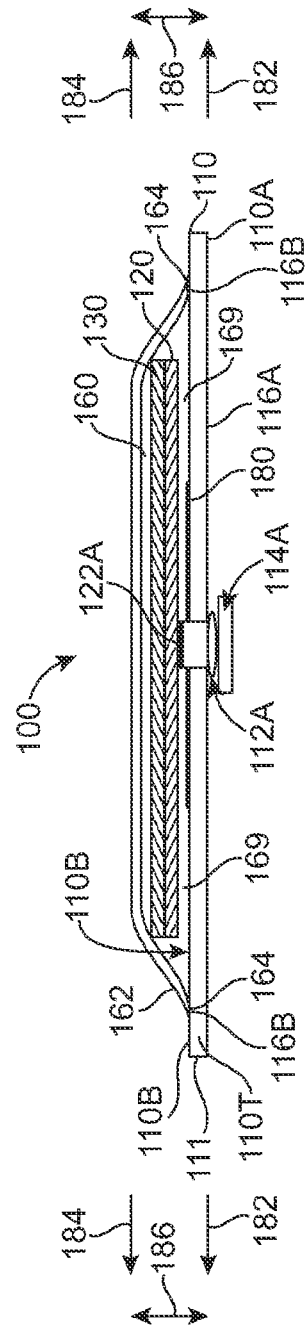
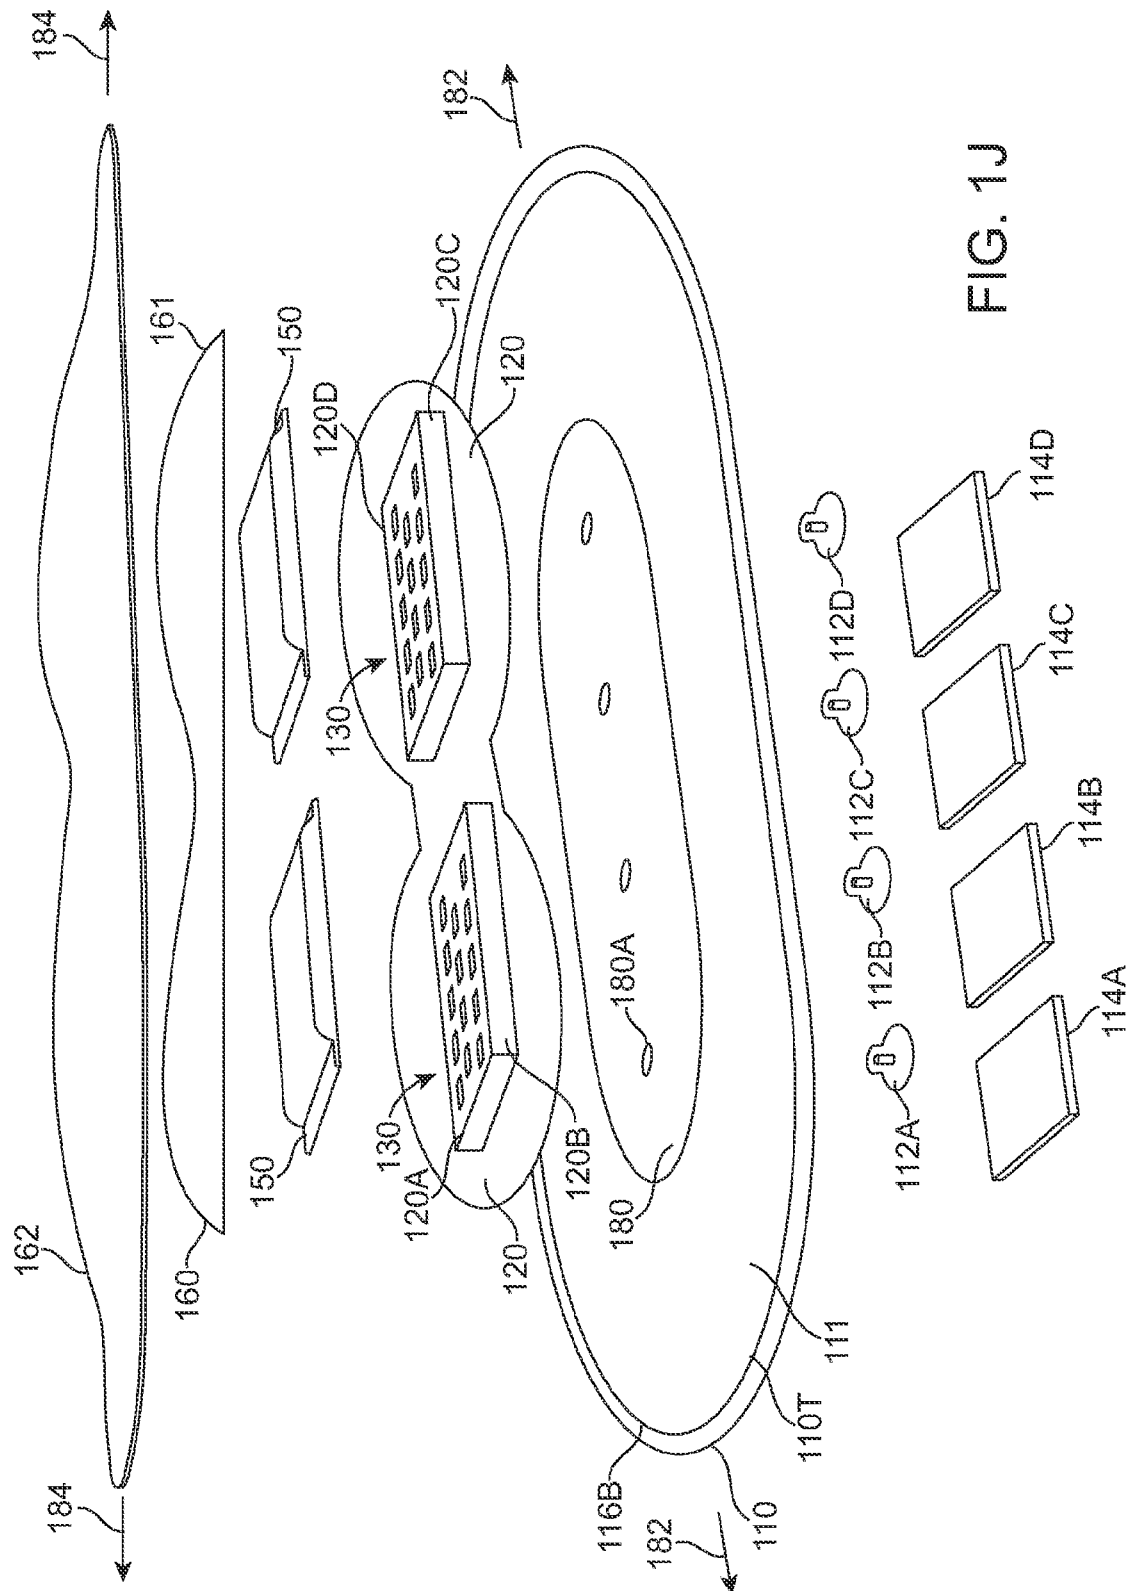


FIG. 1I

10 / 14



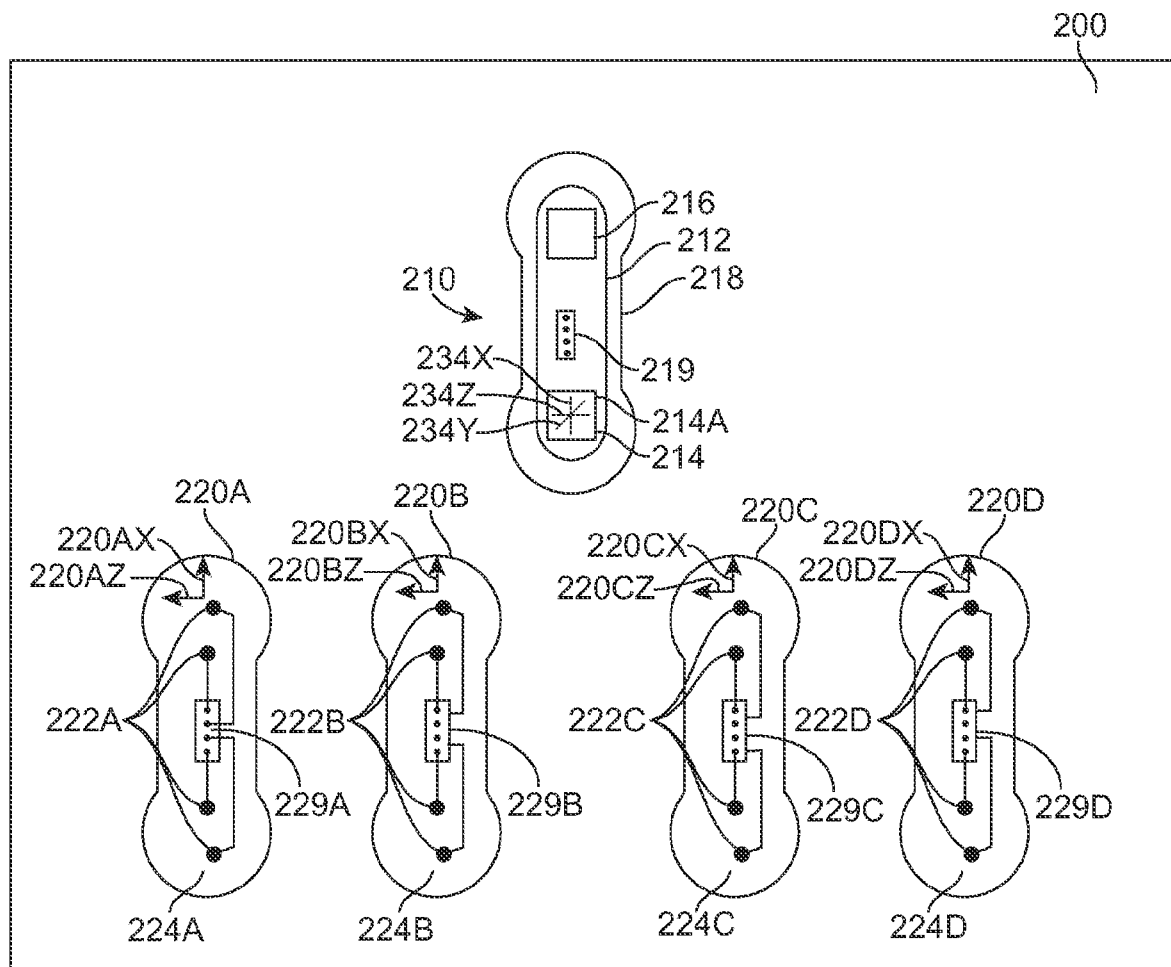


FIG. 2A

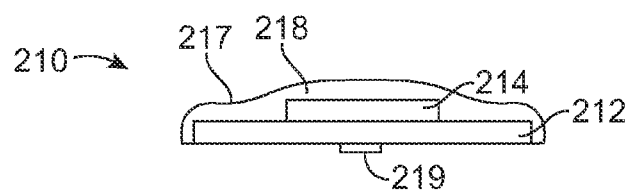


FIG. 2B

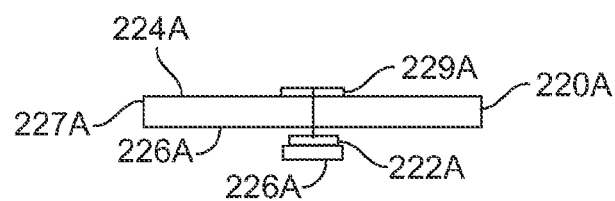


FIG. 2C

12 / 14

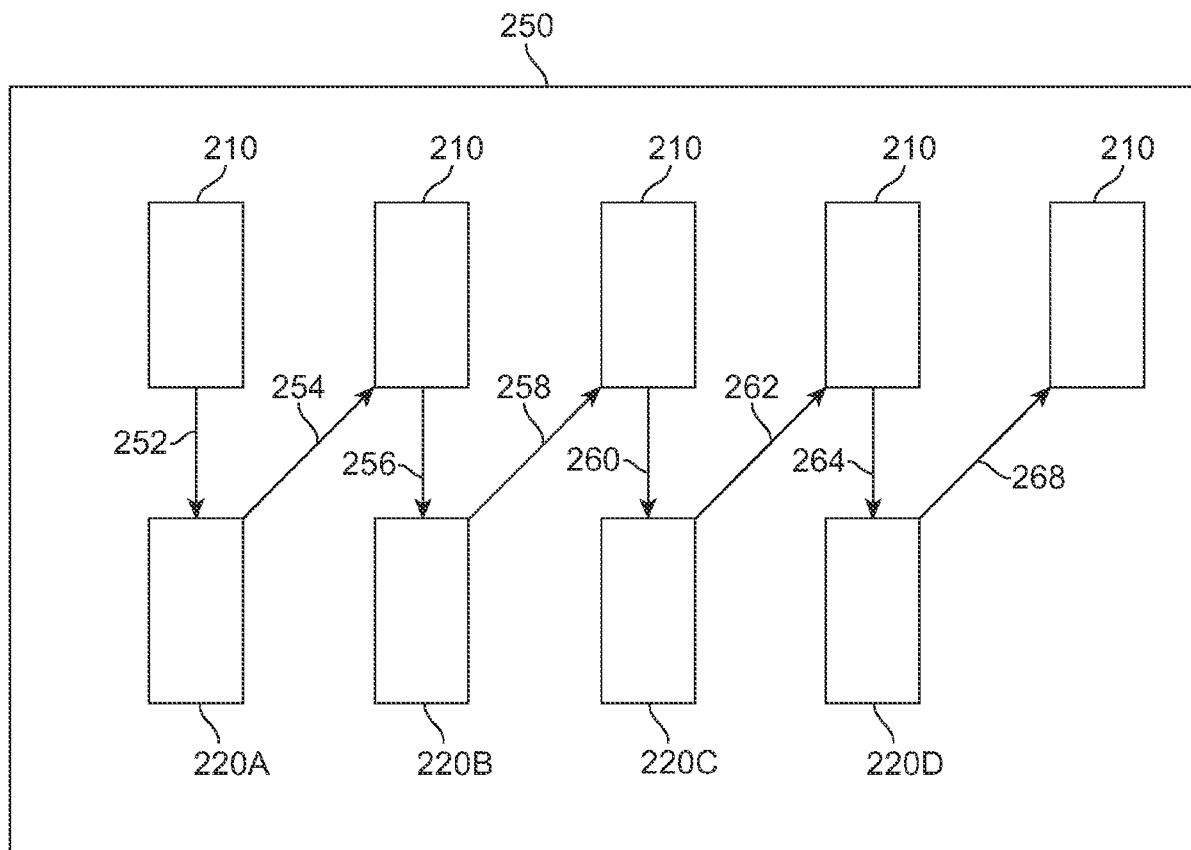


FIG. 2D

13 / 14

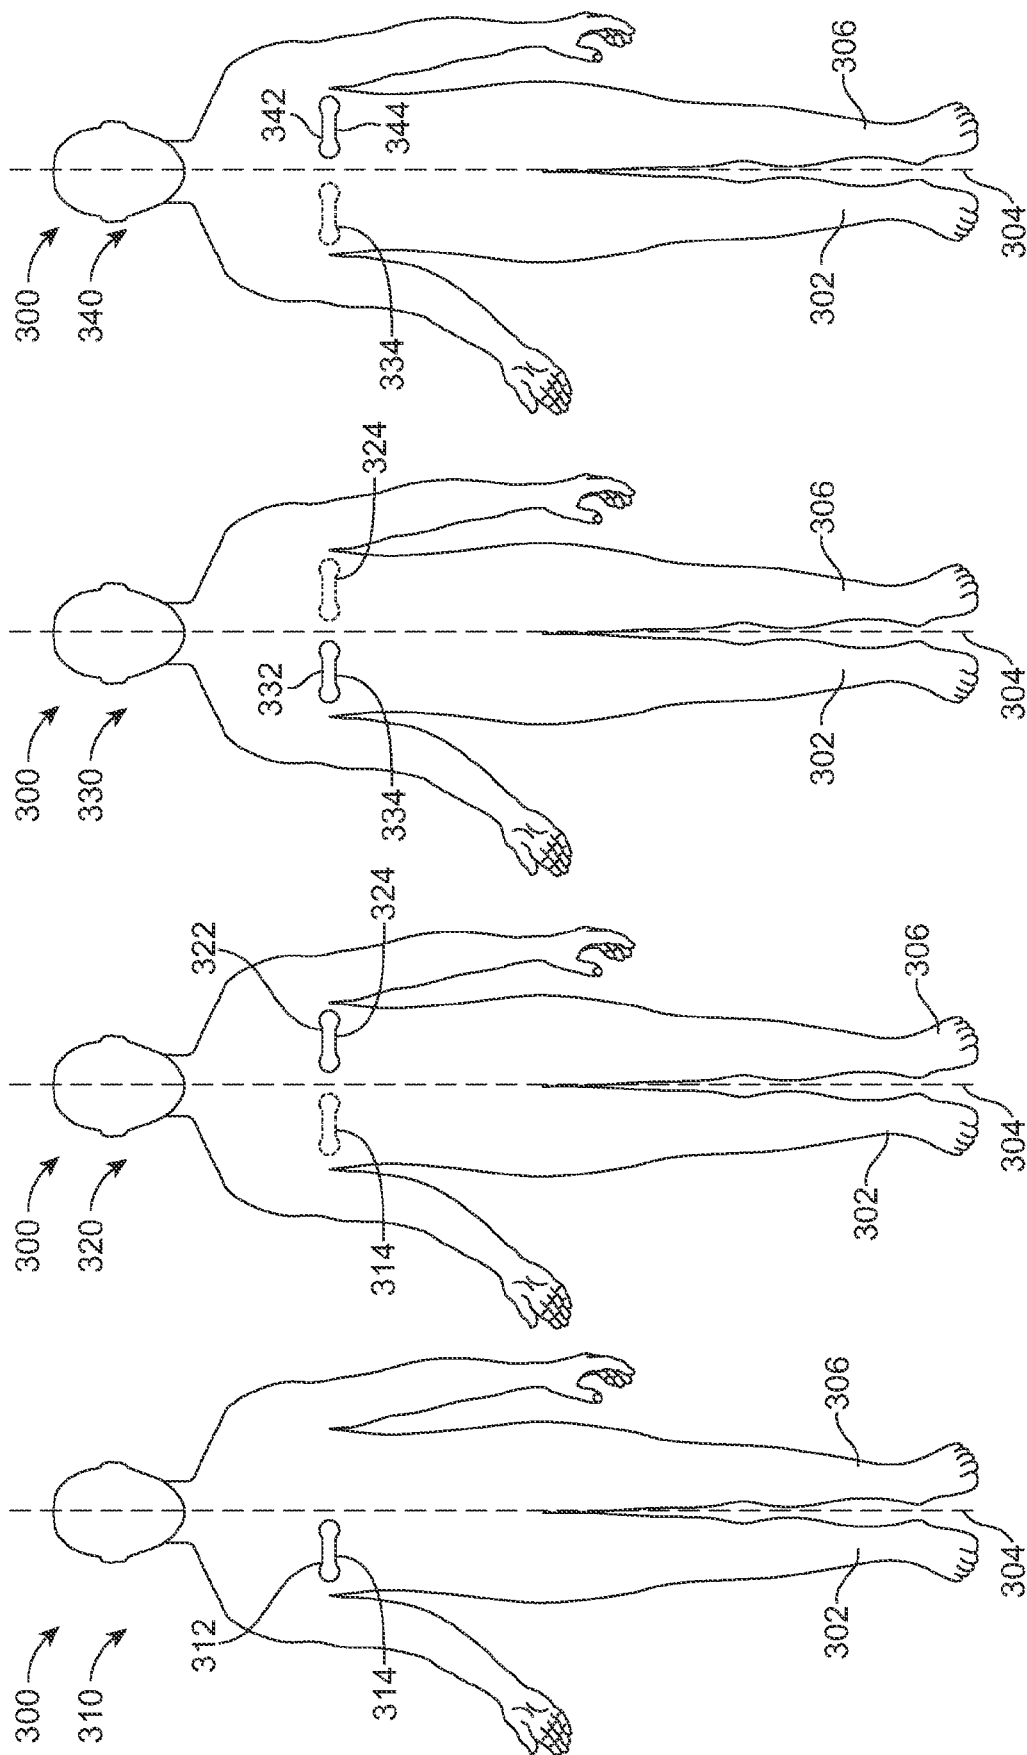


FIG. 3D

FIG. 3C

FIG. 3B

FIG. 3A

14 / 14

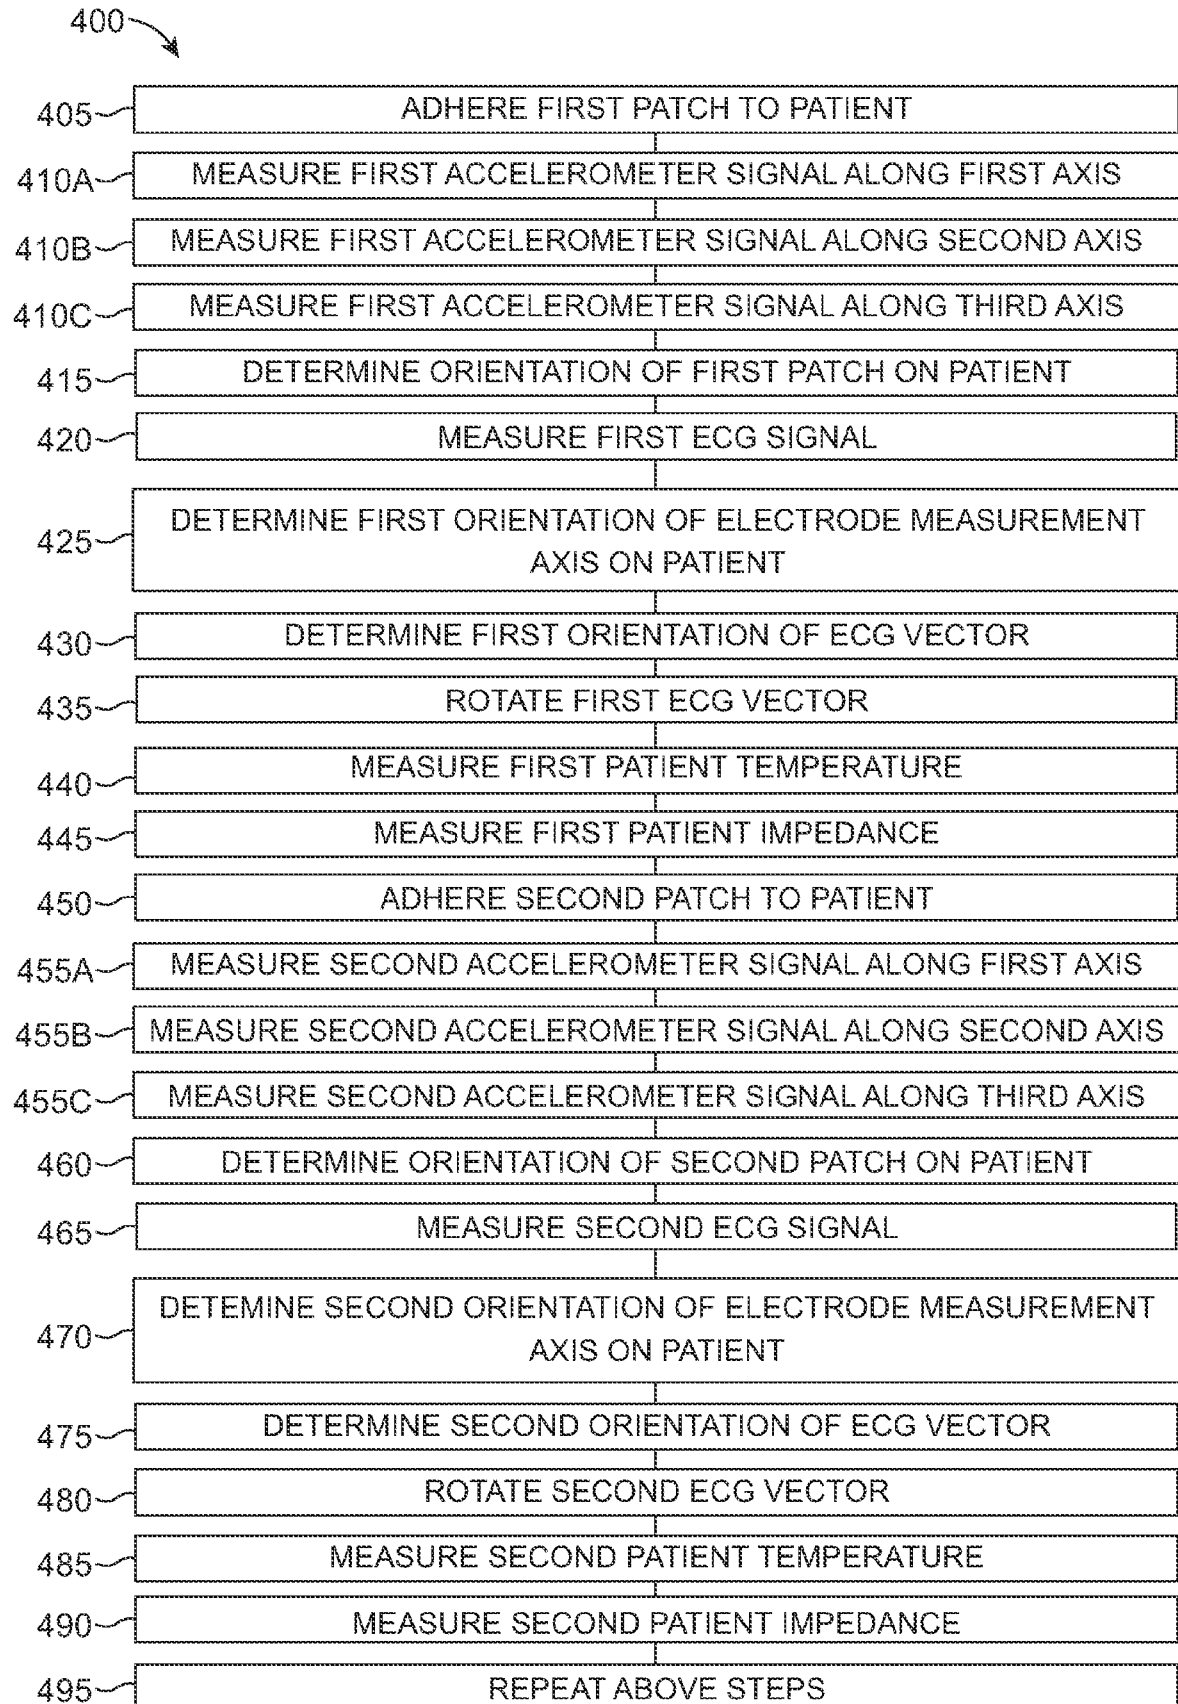


FIG. 4A

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 08/76217

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 5/04

USPC - 600/509

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
600/300,301,508

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
Google Scholar

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
accelerometer; ECG; EKG; electrocardiogram; three-dimensional; correction factor; transformation; ambulatory; electrodes; vector; adhering; adhesive

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2007/0208262 A1 (Kovacs) 6 September 2007 (06.09.2007) paras. [0024], [0026], [0031], [0033], [0035], [0038]-[0040]; Fig. 1A	1-46
Y	US 6049730 A (Kristbjarnarson) 11 April 2000 (11.04.2000) col. 1, Ins. 21-25, col. 2, Ins. 33-46, col. 2, 66-67, col. 3, Ins. 1-13, col. 3, 19-35, col. 3, 50-67, col. 4, Ins. 1-14, col. 4, 19-29, col. 4, 38-53, col. 5, Ins. 18-24, col. 7, Ins. 7-24, col. 8, Ins. 1-55, col. 9, 31-36	1-46
Y	US 6473640 B1 (Erlebach) 29 October 2002 (29.10.2002) col. 9, Ins. 46-53, 57-67	7, 29
Y	US 2007/0167850 A1 (Russel et al.) 19 July 2007 (19.07.2007) paras. [0027]-[0028]	8, 30
Y	US 2005/0158539 A1 (Murphy et al.) 21 July 2005 (21.07.2005) para. [0023]	23, 41
Y	US 2007/0173705 A1 (Teller et al.) 26 July 2007 (26.07.2007) para. [0104], Fig. 19	39
A	US 2007/0129622 A1 (Bourget et al.) 07 June 2007 (07.06.2007)	1-46
A	US 2007/0106167 A1 (Kinast) 10 May 2007 (10.05.2007)	1-46
A	US 2006/0235316 A1 (Ungless et al.) 19 October 2006 (19.10.2006)	1-46
A	US 2006/0064030 A1 (Cosentino et al.) 23 March 2006 (23.03.2006)	1-46
A	US 2005/0113703 A1 (Farrington et al.) 26 May 2005 (26.05.2005)	1-46

☐ Further documents are listed in the continuation of Box C. ☐

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

04 November 2008 (04.11.2008)

Date of mailing of the international search report

10 NOV 2008

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450
Facsimile No. 571-273-3201

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774

专利名称(译)	具有先进传感功能的贴壁心脏监护仪		
公开(公告)号	EP2194856A1	公开(公告)日	2010-06-16
申请号	EP2008830769	申请日	2008-09-12
[标]申请(专利权)人(译)	科文迪斯有限公司		
申请(专利权)人(译)	CORVENTIS INC.		
当前申请(专利权)人(译)	CORVENTIS INC.		
[标]发明人	LIBBUS IMAD MANICKA YATHEENDHAR D FOGOROS RICH		
发明人	LIBBUS, IMAD MANICKA, YATHEENDHAR, D. FOGOROS, RICH		
IPC分类号	A61B5/04 A61B5/00 A61B5/0402 A61B5/0404 A61B5/0408 A61B5/053 A61B5/06 A61B5/11 G01C9/06		
CPC分类号	A61B5/0006 A61B5/04028 A61B5/0404 A61B5/04085 A61B5/0537 A61B5/061 A61B5/11 A61B5/4869 A61B5/6823 A61B5/6833 A61B5/684 A61B5/721 A61B2560/0412 A61B2562/0219 G01C9/06		
优先权	60/972537 2007-09-14 US 61/055662 2008-05-23 US 61/055666 2008-05-23 US		
其他公开文献	EP2194856A4		
外部链接	Espacenet		

摘要(译)

粘附装置包括具有至少两个电极和加速度计的粘性贴片。加速度计可用于确定患者上的至少两个测量电极的取向。通过确定患者上的贴片的电极的取向，可以响应于患者上的贴片的取向来调整和/或校正具有至少两个电极的生理测量。粘附贴片和/或电极可以用第二粘附贴片和/或电极代替，并且第二粘附贴片和/或电极的取向可以用加速计或第二加速计确定。所确定的患者上的第二贴片和/或电极的取向可用于校正用第二贴附贴片和/或电极进行的测量。