



(11) **EP 1 965 703 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**07.06.2017 Bulletin 2017/23**

(51) Int Cl.:  
**A61B 6/03** (2006.01) **A61B 6/00** (2006.01)  
**G06T 11/00** (2006.01) **A61B 5/00** (2006.01)

(21) Application number: **06832175.1**

(86) International application number:  
**PCT/IB2006/054702**

(22) Date of filing: **08.12.2006**

(87) International publication number:  
**WO 2007/072281 (28.06.2007 Gazette 2007/26)**

(54) **RECONSTRUCTION UNIT FOR RECONSTRUCTING A FINE REPRODUCTION OF AT LEAST A PART OF AN OBJECT**

REKONSTRUKTIONSEINHEIT ZUR REKONSTRUKTION EINER FEINEN WIEDERGABE  
MINDESTENS EINES TEILS EINES OBJEKTS

UNITE DE RECONSTRUCTION SERVANT A LA REPRODUCTION FINE D'AU MOINS UNE PARTIE  
D'UN OBJET

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI SK TR**

(30) Priority: **20.12.2005 EP 05112496**

(43) Date of publication of application:  
**10.09.2008 Bulletin 2008/37**

(73) Proprietors:  
• **Philips Intellectual Property & Standards GmbH**  
**20099 Hamburg (DE)**  
Designated Contracting States:  
**DE**  
• **Koninklijke Philips N.V.**  
**5656 AE Eindhoven (NL)**  
Designated Contracting States:  
**AT BE BG CH CY CZ DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI SK TR**

(72) Inventors:  
• **GRAß, Michael**  
**NL-5656 AA Eindhoven (NL)**  
• **VON BERG, Jens**  
**NL-5656 AA Eindhoven (NL)**  
• **LORENZ, Cristian**  
**NL-5656 AA Eindhoven (NL)**

(74) Representative: **de Haan, Poul Erik et al**  
**Philips International B.V.**  
**Philips Intellectual Property & Standards**  
**High Tech Campus 5**  
**5656 AE Eindhoven (NL)**

(56) References cited:  
**WO-A-2004/057539 WO-A-2004/111936**  
**WO-A-2005/008597 WO-A-2005/048193**  
**WO-A2-02/103639 US-A1- 2003 016 851**  
**US-B1- 6 526 117**

- **N. P. SMITH ET AL: "Generation of an Anatomically Based Geometric Coronary Model", ANNALS OF BIOMEDICAL ENGINEERING, vol. 28, no. 1, 1 January 2000 (2000-01-01), pages 14-25, XP055156881, ISSN: 0090-6964, DOI: 10.1114/1.250**
- **Johan Montagnat ET AL: "Spatial and temporal shape constrained deformable surfaces for 3D and 4D medical image segmentation" In: "Spatial and temporal shape constrained deformable surfaces for 3D and 4D medical image segmentation", 1 November 2000 (2000-11-01), INRIA, Sophia Antipolis, XP055056767, pages 1-70,**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**EP 1 965 703 B1**

- MONTAGNAT J ET AL: "4D deformable models with temporal constraints: application to 4D cardiac image segmentation", MEDICAL IMAGE ANALYSIS, OXFORD UNIVERSITY PRESS, OXFORD, GB, vol. 9, no. 1, 1 February 2005 (2005-02-01), pages 87-100, XP027847007, ISSN: 1361-8415 [retrieved on 2005-02-01]
- MONTAGNAT J ET AL: "Space and time shape constrained deformable surfaces for 4D medical image segmentation", LECTURE NOTES IN COMPUTER SCIENCE/COMPUTATIONAL SCIENCE, SPRINGER, DE, vol. 1935, 1 January 2000 (2000-01-01), pages 196-205, XP002329562, ISBN: 978-3-540-24128-7
- JOHAN MONTAGNAT ET AL: "Space and Time Shape Constrained Deformable Surfaces for 4D Medical Image Segmentation", 11 February 2004 (2004-02-11), MEDICAL IMAGE COMPUTING AND COMPUTER-ASSISTED INTERVENTION. MICCAI. INTERNATIONAL CONFERENCE. PROCEEDINGS,, PAGE(S) 196 - 205, XP019001259, ISBN: 978-3-540-41189-5

## Description

**[0001]** The invention relates to a reconstruction unit for reconstructing a fine reproduction of at least a part of an object, a corresponding method, a computer-readable medium and a program element. In particular, the invention relates to a reconstruction unit for reconstructing a fine reproduction of at least a part of an object, wherein the reproduction is executed on data detected by a tomography device.

**[0002]** Deploying computer tomography (CT) for object reconstruction aims to scan an object and to reconstruct a reproduction of the object, which object is enclosed by a body. The non-invasive method of scanning the object is a common procedure to obtain information about the object for diagnostic purposes.

**[0003]** Usually an image of the object is generated. The image can be analysed and an abnormality of an inner structure of the object may be detected. CT scanning is quite often deployed to obtain information of a heart in the body of a human being e.g. calcification in the coronary arteries can be detected.

**[0004]** Since the heart is always in motion the reconstructed pictures may be blurry depending on the phase point of the cardiac cycle when the scan was performed or the projection data were selected and the image of the heart was reconstructed. The phase point determines the centre of the interval of the cardiac cycle, or also named RR-interval, were the projection data have been selected or measured.

**[0005]** The automatic determination of an applicable phase point for retrospectively gated cardiac reconstruction remains as one of the key problems for CT based non-invasive coronary angiography. The determination of an applicable phase point can improve the quality of a reconstructed image of an object. For finding an applicable phase point as a first step, model based approaches have been used, followed by image processing based methods.

**[0006]** An image based approach is known from R. Manzke, et al.: Automatic phase determination for retrospectively gated cardiac CT, Medical Physics, Vol 31, No. 12, December 2004.

**[0007]** A model based approach is known from Vembar, et al.: A dynamic approach to identifying desired physiological phases for cardiac imaging using multislice spiral CT, Medical Physics, Vol. 30, No. 7, July 2003.

**[0008]** Further information can be found in US 6,628,743 B1.

**[0009]** WO 2005/008597 A discloses a motion compensation for CT imaging of the heart or the coronary vessel tree in which a motion of the object is estimated, time points where these areas have minimal motion are determined based thereon. Then, an image is reconstructed using these respective time points.

**[0010]** WO 02/103639 A2 discloses a motion compensation algorithm comprising reconstructing low-resolution images from 3D image data of a 3D image data set

which has been acquired during different phases of motion of the periodic motion. Motion information is determined from the low-resolution images and used to reconstruct high resolution images.

5 **[0011]** It may be desirable to provide efficient object reconstruction.

**[0012]** According to the present invention a reconstruction unit for reconstructing a fine reproduction of at least a part of an object is provided, as defined in claim 1. Further, according to the present invention, a method for reconstructing a fine reproduction of at least a part of an object is provided as defined in claim 8. According to a further exemplary embodiment an examination apparatus for reconstructing a fine reproduction of at least a part of an object is provided, the examination apparatus comprising the reconstruction unit as described above. The examination apparatus further comprises a detector unit and a time scheduling unit, wherein the detector unit is connected to the reconstruction unit. Furthermore, the time scheduling unit is connected to the reconstruction unit and the detector unit is adapted for providing the data set containing structural information about the object. The time scheduling unit is adapted for providing the scheduling information related to the data set. Further according to the present invention, a computer-readable medium is provided, as defined in claim claim 13.

20 **[0013]** Further according to the present invention, a program element for reconstructing a fine reproduction of at least a part of the object is provided, as defined in claim 14.

30 **[0014]** In this context retrospective gating is used to express the process of scanning an object preferred and afterwards analysing of the gathered information. While the scanning of the object is performed a sequence of data sets is generated. These data sets may represent a digitized information of a projection of the object. Structural information of the object, in particular structural information of an interior area of the object may be contained in the projection preferred set. After having collected the plurality of data sets, particular data sets can be selected to reconstruct a reproduction of the object.

35 **[0015]** In the following a basic idea of the invention is described in greater detail.

**[0016]** The reconstruction unit may be adapted for receiving a sequence of data sets, wherein the data sets represent structural information of the object. Further the reconstruction unit may receive scheduling information related to the data sets of the sequence of data sets. The scheduling information may be gathered in parallel to the process of gathering the data sets. Each data set may have a corresponding scheduling information and thus, an order of the data sets belonging to the sequence of data sets is provided. The scheduling information may be seen as a time scale to relate the data sets to the scheduling information. Thus, each data set may have a timing information or a time point information to determine the point in time when the data set was recorded.

40 **[0017]** By using the sequence of data sets and the

scheduling information it may be possible to reconstruct a sequence of coarse reconstructions of the object. preferred combination may allow to reconstruct a movement or motion of the scanned object. Information about the motion may be available by comparing subsequent coarse reconstructions of the model. Using a coarse reconstruction may quickly provide results of calculations and automated operations like mathematical comparisons of the models and in particular of specific elements of the models may be possible.

**[0018]** A coarse reconstruction or a coarse reproduction may use less information than a fine reconstruction or a fine reproduction. Thus, a fine reproduction may show a more detailed information of the object.

**[0019]** It may also be possible to use all available information of the data sets and thus, instead of reconstructing a coarse reconstruction to reconstruct a fine reconstruction, already in this phase of the process. Thereby the performance of the process may be reduced, however smaller landmarks, i.e. portions, may be observed or detected and the phase of minimum motion of the small portions may be detected. The fine reproduction, which may be used instead of the coarse reproduction, may be an image of high resolution.

**[0020]** An example of a coarse reconstruction may be a two dimensional sectional view with a low resolution or a three dimensional picture with a low resolution. In a two dimensional view or picture pixels may be used to mark different sub-structures of the object. Therefore pixels may provide grey scale values or colour values to mark different sub-structures. Accordingly a three dimensional picture may use voxels to distinguish between different substructures. A low resolution of a three dimensional picture may have a spatial resolution of e.g.  $64^3$  (=64<sup>3</sup>) voxels or  $128^3$  (=128<sup>3</sup>) voxels.

**[0021]** These pictures may be recorded at different points in time. Thus, the time resolution may be 20 to 50 three dimensional pictures in a defined time period wherein the time period may be substantially 1 second. The time period may also be expressed by a sampling rate, which is the inverse value of the duration of a period.

**[0022]** Since the coarse reconstructions may be computer generated pictures, it may be possible to detect different sub-structures in the coarse reconstructions by methods of automatic image processing. Therefore processing of the coarse reconstructions with the reconstruction unit may be possible. The reconstruction unit may deploy e.g. filter operations to select the borders of different structures.

**[0023]** Thus, it may also be possible that the reconstruction unit is able to automatically distinguish and recognize different sub-structures in the coarse reconstruction of the object. In other words, parts of a representation of a real physical object, in particular interior structures of the physical object, may be converted into a machine-readable format.

**[0024]** Having a machine-readable format of the structural information of coarse reconstructions, the recon-

struction unit may be able to automatically generate a sequence of adapted models of the object by adapting a respective basic model to each of the coarse reconstructions. In particular the reconstruction unit may be able to adapt the basic model to the detected sub-structures of the coarse reconstructions.

**[0025]** A model may be a mesh model. A mesh model may comprise a plurality of lines and edges to rebuild a structure of an object. For rebuilding the structure of the object of interest, the mesh model may use an a priori knowledge about the structure of the object of interest. In other words the basic structure of the object or the inner structure of the object may be known in advance and a basic mesh model using this knowledge may be provided. Then, for reconstructing the individual form of the object of interest, the basic model may have to be adapted to the recognised structures of the coarse reconstructions, which may be an image of the object of interest.

**[0026]** The edges and lines of the model may make such a model virtually deformable. The higher the number of edges the higher the granularity or resolution of the model. Since the mesh model may be deformable the model may be adapted to the detected structures or sub-structures of the coarse reconstructions of the physical object. For this adaptation landmarks are deployed, which may be specific points for finding related points of the coarse reconstructions. Such landmarks may be a known artery or a known ventricle in case of a heart.

**[0027]** After having adapted a single model to a sequence of coarse reconstructions or after having generated a sequence of adapted models a motion of a portion of the mesh model may be determined. The motion may be determined by tracking the position of a known specific point of the model in the sequence of adapted models. An example for a specific point may be an edge of the mesh model.

**[0028]** A motion vector field of the portion of interest may be generated in order to determine the strength of the motion of that portion. A motion vector field is a plurality of motion vectors. Each motion vector may correspond to the relevant portion of the object and may indicate the strength of the motion of the relevant portion.

**[0029]** The portion may be selected in advance since the portion of the model may correspond to a relevant portion or area in the physical object.

**[0030]** Using the determined information about the motion may allow selecting a specific data set of the sequence of data sets, wherein the specific data set may correspond to the adapted model with the minimum motion of the predetermined portion. The relevant data set may be determined by backward tracking from the adapted model to the relevant data set. The backward tracking may be possible, since the sequence of data sets is linked to the scheduling information.

**[0031]** When the relevant data set of minimum motion may be found it may be possible to reconstruct a fine reconstruction of at least the part of the object using the

relevant data set. There may be additional information available in the data set for reconstructing a fine reproduction, since not all the information available in the data set may be used for the coarse reconstruction. Using the additional information from the relevant data set may achieve a high granularity of the reproduction, i.e. with this additional information it may be possible to reconstruct a picture with a high resolution.

**[0032]** In other words, using the method of retrospectively gated object reconstruction may produce a plurality of projections or scanner data sets. Scanning an oscillating object may produce artefacts or un-sharp reconstructed structures. If the object may oscillate irregularly the plurality of data sets may contain data sets corresponding to phases or phase points or points in time of high motion activity and data sets corresponding to phases or phase points or points in time of minimum motion activity.

**[0033]** Finding the data sets corresponding to phase points of minimum activity of a part of interest of the object may allow a sharp reproduction of the part of interest of the object. The sharpness may be increased by using data sets corresponding to phase points of minimum or nearly no motion of the part of interest of the object. The sharpness in addition may be increased by using all information available in a data set for reconstructing the object. This may lead to a sharp image of high resolution or a fine reproduction of high resolution.

**[0034]** Providing a high resolution may mean that an area is represented by a higher number of voxel or pixel. Thus, more details of the part of interest of the object may be visualized. Therefore structures, which usually cannot be seen in un-sharp pictures may now be visible. Thus, fine structures of the object may also be seen. The fine structures may be seen even if the models have been adapted to other coarse shapes, which may be located nearby or underneath the fine structures.

**[0035]** In the following, further exemplary embodiments of the reconstruction unit will be described. These embodiments apply also for the method for reconstructing a fine reproduction of at least a part of an object, for the examination apparatus, for the computer-readable medium, and for the program element.

**[0036]** According to a further preferred embodiment of the present invention, the reconstruction unit is adapted for reconstructing a cardiac structure.

**[0037]** A reconstruction unit, which is adapted for reconstructing a cardiac structure may allow to reconstruct a fine reproduction of the heart or parts of the heart. Since such a reproduction is not limited to the selected portion it may be possible that other structures are reconstructed. Therefore small coronaries may be visible on such reproductions.

**[0038]** The models of a heart may be permanently stored in a reconstruction unit, which is adapted for reconstructing a cardiac structure since the reconstruction unit may only be used for analyses concerning the heart and the reconstructing unit may be optimised for recon-

structing cardiac structures.

**[0039]** According to another preferred embodiment of the present invention, the respective model is at least one selected from the group consisting of a mesh and a cardiac model.

**[0040]** Using a specific mesh or cardiac model may allow recognition of the different sub structures or different compartments of the cardiac anatomy. Therefore the detection and reconstruction process may be accelerated.

**[0041]** According to a further preferred embodiment of the present invention the above-mentioned respective model comprises adaptable shapes.

**[0042]** The more shapes are provided by the relevant model the better reconstruction may be performed. Using as much information of the model as possible may result in a better and sharper fine reproduction of the cardiac anatomy.

**[0043]** According to a further preferred embodiment of the present invention the fine reproduction is at least one selected from the group of a fine mesh, fine sub mesh, a high resolution computer picture, a vector graphic, a high resolution 2D picture, a high resolution 3D picture, a coronal sectional view, and a sagittal sectional view of the part of the object.

**[0044]** The different reproductions may provide exemplary reproductions, which may be used in a computer system for representing a physical object. The different reproductions may be different representations of the same set of data. The different representations may be selectively switched on to provide different views of the part of interest of the object or cardiac structure to an user.

**[0045]** According to a further exemplary embodiment of the present invention, the reconstruction unit is adapted to process scheduling information, which is a sequence of points in time.

**[0046]** The points in time may correspond to specific events. The sequence of points in time may be an ordered list, listing sampling points. Having an ordered list of points in time, which may correspond to a relevant data set recorded in that special point in time may allow to relate a specific data set to a point in time, the data set corresponds to. This information of the relationship of the data set and the relevant point in time may be used when backtracking for finding the relevant data set for the fine reproduction.

**[0047]** According to a further preferred embodiment of the present invention, the reconstruction unit is adapted to process scheduling information, which is a sequence of phase points.

**[0048]** A phase may be a regularly repeating interval, which is a part of the cardiac cycle. The cardiac cycle is a sequence of phase points and a sequence of phases. The phase points may allow to relate a data set to a defined point in time of the cardiac phase.

**[0049]** According to a further preferred embodiment of the present invention, the phase points are phase points of a cardiac phase.

**[0050]** According to the present invention, the reconstruction unit is adapted to receive scheduling information from an ECG (electro cardiogram) recording. An ECG recording is a plot which represents the activity of an heart over the time. High activity may be represented by a high amplitude. Low activity may be represented by a low amplitude in the plot. Therefore defined phases of the cardiac cycle may be seen on the plot.

**[0051]** The ECG may be recorded in parallel to the sampling of the data sets. Since the time is recorded when the relevant data set is sampled, the data set can be related to a phase of the cardiac cycle. The link may be made by a common point in time of the sequence of data sets and the scheduling information.

**[0052]** According to a further exemplary embodiment the reconstruction unit is adapted to process a sequence of data, which is a sequence of CT projection data sets. Computer tomography (CT) is a process of using digital processing to generate a three-dimensional image of the internal structure of an object under investigation (object of interest) from a series of two-dimensional X-ray images taken around a single axis of rotation. The reconstruction of CT images can be done by applying appropriate algorithms.

**[0053]** For each point in time, when a X-ray image is recorded, a set of data is generated. The generated set of data may include information about a direction or angle in relation to the object and the corresponding attenuation of a X-ray through the body or object.

**[0054]** According to another exemplary embodiment the reconstruction unit is adapted for selecting the specific data set by generating a set of motion vectors belonging to the predetermined portion of the model, wherein the set of motion vectors is generated at each position of the adapted models. Once a set of motion vectors is generated the absolute length of the set of motion vectors of the predetermined portion of the adapted models is determined.

**[0055]** It may be possible to select from the sequence of adapted models at least one adapted model, which offers the minimum motion of the portion of interest. Since the adapted model is adapted to a coarse reconstruction of a data set, the relevant data set can be determined. This determination may be possible since the coarse reproduction may be related to a phase point of a cardiac cycle, and thus the relevant phase point of the cardiac cycle may be determined. This phase point may be, in retrospectively gated cardiac reconstruction to achieve a good diagnostic image quality.

**[0056]** In the following, a further exemplary Preferred of the method will be described. This embodiment applies also for the reconstruction unit for reconstructing a fine reproduction of at least a part of an object, for the examination apparatus, for the computer-readable medium, and for the program element.

**[0057]** According to another preferred embodiment of the present invention, the method comprises selecting the part of the object as a structure nearby a coronary.

**[0058]** A coronary may be not directly detectable and visual in a coarse reproduction of the part of the object. The coronary therefore may also be no part of the model.

**[0059]** However, for visualizing the coronary or a plurality of coronaries or another fine structure, a part of the object that is known to be in the neighbourhood or lying underneath the coronary or the fine structure may be selected to be sharply reproduced. Indirectly and automatically the coronary may be visible on the sharp reproduction of the object.

**[0060]** In the following, further exemplary embodiments of the examination apparatus will be described. These embodiments apply also for the reconstruction unit for reconstructing a fine reproduction of at least a part of an object, for the method, for the computer-readable medium, and for the program element.

**[0061]** Furthermore, according to another preferred embodiment of the present invention, the examination apparatus may comprise a memory unit wherein the memory unit is adapted for storing the sequence of data sets and the scheduling information.

**[0062]** Storing the information may allow to collect the information about the object and to analyze the information after collecting the information. Thus, backtracking may be possible.

**[0063]** According to another preferred embodiment of the present invention the examination apparatus comprises a graphical user-interface.

**[0064]** The graphical user-interface may be adapted to display information calculated by the examination apparatus. The fine reproduction may be a graphical representation of a list of graphical information. The graphical user interface may convert this graphical information into an image, viewable by an user. The graphical user interface may also provide the option to select between different views of the fine reproduction of the object.

**[0065]** The graphical user interface may also provide the possibility to send commands to the examination apparatus, in particular to control the reconstruction unit. The whole process of reconstructing a fine reproduction may be controllable through the graphical user interface.

**[0066]** According to another exemplary embodiment, the examination apparatus is at least one selected of the group consisting of a material testing apparatus, a baggage inspection apparatus, a medical application apparatus, a computer tomography apparatus, a coherent scatter computed tomography apparatus, a positron emission computed tomography apparatus, a single photon emission computed tomography apparatus, ultra sound apparatus, electron beam tomography apparatus, magnetic resonance apparatus, and an interventional 3D rotational X-ray device.

**[0067]** By use of such an examination apparatus information may be provided about an inner structure of an object.

**[0068]** It may be seen as the gist of an exemplary embodiment of the present invention that automatically a phase point is determined, which phase point allows to

reconstruct a high resolution reproduction to achieve a good diagnostic image quality. For achieving this high resolution reproduction, a model is adapted to coarse reconstructions so that a series of adapted models can be reconstructed. From this consecutive adapted models areas of minimum motion can be determined. To improve the quality of the high resolution reproduction preferably just a portion of the model is selected, leading to better results then just using global information of motion of the whole object.

**[0069]** Also if the reconstruction process uses a structure different from the structure of interest, the knowledge about the position of the structure of interest can be used to focus on a structure nearby the structure of interest. Since these different structures may have similar motion properties a point in time, which is good for reconstructing the nearby structure may also be good for reconstructing the structure of interest.

**[0070]** Thus, the structure of interest may be visible, even if this structure may not be part of a model used for reconstruction.

**[0071]** These and other aspects of the present invention will become apparent from and elucidated with reference to the embodiments described hereinafter.

**[0072]** Exemplary embodiments of the present invention will be described in the following, with reference to the following drawings.

Fig. 1 shows a simplified schematic representation of an examination apparatus according to an exemplary embodiment of the present invention.

Fig. 2 shows a 3D model representation after adaptation to a low resolution 4D data set in an end systolic phase point.

Fig. 3 shows a 3D model representation after adaptation to a low resolution 4D data set in an end diastolic phase point.

Fig. 4 shows an exemplary embodiment of an image processing device according to the present invention, for executing an exemplary embodiment of a method in accordance with the present invention.

Fig. 5 shows a 3D mesh model with coronaries.

Fig. 6 shows a flow-chart of an exemplary method according to the present invention.

**[0073]** The illustration in the drawings is schematically. In different drawings, similar or identical elements are provided with the same reference numerals.

**[0074]** Fig. 1 shows an exemplary embodiment of a computed tomography scanner system according to the present invention.

**[0075]** The computer tomography apparatus 100 depicted in Fig. 1 is a cone-beam CT scanner. However, the invention may also be carried out with a fan-beam geometry. The CT scanner depicted in Fig. 1 comprises a gantry 101, which is rotatable around a rotational axis 102. The gantry 101 is driven by means of a motor 103. Reference numeral 104 designates a source of radiation

such as an X-ray source, which, according to an aspect of the present invention, emits polychromatic or monochromatic radiation.

**[0076]** Reference numeral 105 designates an aperture system which forms the radiation beam emitted from the radiation source to a cone-shaped radiation beam 106. The cone-beam 106 is directed such that it penetrates an object of interest 107 arranged in the center of the gantry 101, i.e. in an examination region of the CT scanner, and impinges onto the detector 108. As may be taken from Fig. 1, the detector 108 is arranged on the gantry 101 opposite to the source of radiation 104, such that the surface of the detector 108 is covered by the cone beam 106. The detector 108 depicted in Fig. 1 comprises a plurality of detector elements 123 each capable of detecting X-rays which have been scattered by or passed through the object of interest 107.

**[0077]** The detector 108 may be a multi slice detector to increase the resolution in the z axis.

**[0078]** During scanning the object of interest 107, the source of radiation 104, the aperture system 105 and the detector 108 are rotated along the gantry 101 in the direction indicated by an arrow 116. For rotation of the gantry 101 with the source of radiation 104, the aperture system 105 and the detector 108, the motor 103 is connected to a motor control unit 117, which is connected to a control unit 118 (which might also be denoted as a calculation, determination unit or reconstruction unit).

**[0079]** In Fig. 1, the object of interest 107 is a human being which is disposed on an operation table 119. During the scan of a heart 130 of the human being 107, while the gantry 101 rotates around the human being 107, the operation table 119 displaces the human being 107 along a direction parallel to the rotational axis 102 of the gantry 101. By this, the heart 130 is scanned along a helical scan path. The operation table 119 may also be stopped during the scans to thereby measure signal slices. It should be noted that in all of the described cases it is also possible to perform a circular scan, where there is no displacement in a direction parallel to the rotational axis 102, but only the rotation of the gantry 101 around the rotational axis 102.

**[0080]** Moreover, an electrocardiogram (ECG) device 135 is provided which measures an electrocardiogram of the heart 130 of the human being 107 while X-rays attenuated by passing the heart 130 are detected by detector 108. The data sets detected by detector 108 are transmitted to the control unit 118 via interface or input terminal 142. The data related to the measured electrocardiogram are transmitted to the control unit 118 via interface or input terminal 140.

**[0081]** Further, it shall be emphasized that, as an alternative to the cone-beam configuration shown in Fig. 1, the invention can be realized by a fan-beam configuration. In order to generate a primary fan-beam, the aperture system 105 can be configured as a slit collimator.

**[0082]** The detector 108 is connected to the control unit 118. The control unit 118 receives the detection result

in the form of a sequence of data sets, i.e. the read-outs from the detector elements 123 of the detector 108 and determines a scanning result on the basis of these read-outs. Furthermore, the control unit 118 communicates with the motor control unit 117 in order to coordinate the movement of the gantry 101 with motors 103 and 120 with the operation table 11.

**[0083]** The control unit 118 may be adapted for reconstructing an image from read-outs or data sets of the detector 108. A reconstructed image or fine reproduction generated by the control unit 118 may be output to a display or graphical user-interface 121.

**[0084]** The graphical user-interface 121 is connected to the interface or output terminal 144. The output 144 provides a bidirectional communication with the reconstruction unit 118. Therefore information can be displayed and control signals can be sent to the reconstruction unit.

**[0085]** Instead or in addition to the graphical user-interface 121 the reconstructed image, which may also be a digital image, is provided to a storage device (not shown in Fig. 1) or a data communication network. The data communication network may be an ATM (asynchronous transfer mode) or Ethernet based network and providing telemedicine applications.

**[0086]** The control unit 118 may be realized by a data processor to process read-outs from the detector elements 123 of the detector 108.

**[0087]** The computer tomography apparatus shown in Fig. 1 captures multi-cycle cardiac computer tomography data of the heart 130. In other words, when the gantry 101 rotates and when the operation table 119 is shifted linearly, then a helical scan is performed by the X-ray source 104 and the detector 108 with respect to the heart 130. During this helical scan, the heart 130 may beat a plurality of times. During these beats, a plurality of cardiac computer tomography data are acquired. Simultaneously, an electrocardiogram is measured by the electrocardiogram unit 135. After having acquired these data, the data are transferred to the control unit 118, and the measured data may be analyzed retrospectively.

**[0088]** The measured data, namely the cardiac computer tomography data and the electrocardiogram data are processed by the reconstruction unit 118 which may be further controlled via a graphical user-interface (GUI) 121. This retrospective analysis is based on a helical cardiac cone beam reconstruction scheme using retrospectively gating. It should be noted, however, that the present invention is not limited to this specific data acquisition and reconstruction.

**[0089]** The reconstruction unit 118 is adapted to analyze the multi-cycle cardiac computer tomography data detected by attenuating X-rays passing the heart 130 in the following manner, to automatically calculate phase points for spatially different cardiac structures using a model. A sequence of data sets is received from detector 108. The data sets represent structural information of the heart 130. In parallel scheduling information related to

the data sets of the sequence of data sets is received by the reconstruction unit 118 from ECG 135. Then a sequence of coarse reconstructions of the heart 130 is reconstructed by using the sequence of data sets and the scheduling information.

**[0090]** A sequence of adapted models of the heart 130 is generated by adapting a respective model to each of the coarse reconstructions. Then a motion of a predetermined portion of each of the adapted models is determined and a specific data set of the sequence of data sets is selected. This specific data set corresponds to the adapted model with the minimum motion of the predetermined portion. Then a fine reproduction of at least the part of the object is reconstructed using the specific data set and the fine reproduction is displayed on the graphical user-interface 121 or sent to a remote graphical user-interface via a network.

**[0091]** In other words this means, that an automatic method is described to determine patient and anatomy selective optimal phase points in a fully automatic manner.

**[0092]** After the acquisition of the cardiac CT projection data set with parallel ECG 135 recording, a straightforward 4D reconstruction of the complete cardiac volume at low spatial resolution is performed. This data set may consist e.g. of  $64^3$  or  $128^3$  voxels and 20 to 50 different phases within the cardiac cycle. A 4D reconstruction is a reconstruction that combines a 3D image with the scheduling information as a fourth dimension.

**[0093]** Subsequently, a cardiac model consisting of adaptive shapes of the main compartments of the heart is fitted into one of the phases and propagated through the complete 4D data set. For all different phases the shape is adapted to the low resolution image data. Since the points used for the description of the model are assigned to the different compartments of the cardiac anatomy, their position can be tracked through the complete 4D data set.

**[0094]** As a measurement for the optimal phase point for the reconstruction of a certain cardiac structure, the absolute length of all motion vectors of all points belonging to this part of the model may be suitable. The minimum of this function then delivers the optimal phase point. Other measures are imaginable.

**[0095]** After having calculated the phase point for the cardiac structure of interest, this phase point is used in a high resolution reconstruction to achieve high diagnostic image quality.

**[0096]** The phase point may be good for structures like the coronaries, which may not directly be part of the model, to be determined by the phase point of their underlying structure or a structure nearby the coronaries.

**[0097]** Thus, phase points for different cardiac compartments for cardiac CT reconstruction can be determined. The detection can be performed for patient selective phase point for different coronary artery segments. Thus, patient individual characteristics of the cardiac phase can be regarded and a phase point can be

derived in an anatomy selective manner. It is known from the statistical analysis of a large amount of cardiac image data sets that e.g. the right and the left coronary artery have their resting phase at different positions within the RR interval. The RR interval is the duration from the appearance of a R impulse in an ECG recording to the next R impulse. The R impulse shows in an ECG plot the start of a cardiac cycle. Usually 10 - 20 % of the cardiac cycle after the appearance of the R impulse, the maximum motion of the heart may be expected, i.e. the phase of the compression of the left ventricle. In the close neighbourhood of the R impulse less motion may be expected since the contraction of the atrium is finished.

**[0098]** Fig. 2 shows a 3D model representation after adaptation to a low resolution 4D data set in an end systolic phase point. In Fig. 2 different compartments 201', 202, 203 and 204 are shown in an end systolic phase point. The mesh model 206 comprises a plurality of edges 207 and lines 208 building triangular structures. The triangular structures represent the structure of the relevant compartment taken from a coarse reconstruction.

**[0099]** E.g. compartment 201' represents the left ventricle at the end systolic phase point.

**[0100]** A reference point 205' is shown in Fig. 2. Tracking the motion of the reference point 205' allows to determine the motion of a portion of the mesh model 206 the reference point 205' is belonging to.

**[0101]** Fig. 3 shows a 3D model representation after adaptation to a low resolution 4D data set in an end diastolic phase point. In comparison with Fig. 2 it can be seen that the left ventricle 205" has a larger volume than the left ventricle 205' of Fig. 2. It can also be seen from Fig. 3 that reference point 205" has moved. Thus, by tracking the trajectory of reference point 205' and 205" and the calculation of the motion vectors in the relevant phases would indicate area of high motion. Therefore end systolic or end diastolic phase points may not be applicable for a fine reproduction for the portion of the object 130 the reference point 205' is part of.

**[0102]** Fig. 4 depicts an exemplary embodiment of a data processing device 118 or reconstruction unit according to the present invention for executing an exemplary embodiment of a method in accordance with the present invention. The data processing device 118 depicted in Fig. 4 comprises a central processing unit (CPU) or image processor 401 connected to a memory 402 for storing an image depicting an object of interest, such as a patient or an item of baggage. The data processor 401 may be connected to a plurality of input/output networks or diagnosis devices, such as a CT device. The data processor 401 may furthermore be connected to a display device 403, for example, a computer monitor or a graphical user interface, for displaying information or an image computed or adapted in the data processor 401. An operator or user may interact with the data processor 401 via a keyboard 404 and/or other output devices, which are not depicted in Fig. 4.

**[0103]** Furthermore, via the bus system 405, it may

also be possible to connect the image processing and control processor 401 to, for example, an ECG 135 and detector 108.

**[0104]** Fig. 5 shows a 3D mesh model with coronaries. The mesh model 503 is a model of the object of interest 130, e.g. the heart of a patient 107. The model of Fig. 5 is a basic model that is not adapted to patient individual anatomy.

**[0105]** The mesh model 503 has edges 207 and lines 208. By providing edges 207 and lines 208 the model has a computer readable and computer processable format, which may allow to adapt the model to an image of the heart by means of the computer. The compartments 201, 202, 203 and 204 are modelled and can be adapted to the relevant structures on a corresponding image. Additional coronaries 501 and 502 are shown which lay in the neighbourhood of the compartments 201 and 202. The left ventricle 201 is the underlying structure of coronary 501 which provides a plurality of branches. The compartment 202 is the underlying structure of coronary 502. The left ventricle 201 in Fig. 2 and Fig. 3 is labelled with 201' and 201" to show the different phases in which the left ventricle is depicted and to show the different sizes of the left ventricle in the different phases of the cardiac cycle.

**[0106]** The coronaries 501 and 502 may be not visible on a coarse reproduction. But determining a fine reproduction of the relevant compartments 201 and 202 can make the coronaries 501, 502 visible on the fine reproduction.

**[0107]** Fig. 6 shows a flow-chart of an exemplary method according to the present invention. The method starts with recording of a sequence of data sets in step S1 and with parallel recording of scheduling information in the form of ECG recording S2.

**[0108]** Then in step S3 a 4D coarse reconstructions of a sequence of cardiac volume is performed at low spatial resolution. For the reconstruction the data sets and the scheduling information of the ECG is combined.

**[0109]** After the reconstruction of the sequence of coarse reconstructions in step S4 a model is adapted to the coarse reconstructions and a sequence of adapted models is determined. Using these models allows to determine motion vectors.

**[0110]** In step S5 the minimum length of all motion vectors belonging to a part of the model is determined. With this information about the minimum motion an adequate phase point can be determined.

**[0111]** The phase point calculated in step S5 can be used in step S6 to find out the relevant data set belonging to the phase point. This data set is used to reconstruct a fine reconstruction. Preferred embodiments of the invention may be distributed as a software option to CT scanner console, imaging workstations or PACS workstations.

**[0112]** It should be noted that the term "comprising" does not exclude other elements or steps and the "a" or "an" does not exclude a plurality. Also elements de-

scribed in association with different embodiments may be combined.

**[0113]** It should also be noted that reference signs in the claims shall not be construed as limiting the scope of the claims.

### Claims

1. An image reconstruction unit for reconstructing a fine reproduction of at least a part (501,502) of an object (130), wherein the reconstruction unit (118) is adapted for:

receiving a sequence of measured data sets measured by an examination apparatus, the data sets representing structural information of the object (130);

receiving scheduling information from a time scheduling unit (135), said scheduling information related to a sequencing of the sequence of data sets;

reconstructing a sequence of coarse reconstructions of the object (130) by using the sequence of data sets and the scheduling information;

detecting sub-structures in the sequence of coarse reconstructions by processing the sequence of coarse reconstructions;

generating a sequence of adapted shape models (206) of the object (130) by adapting a deformable shape model (503) to the detected sub-structures of each of the coarse reconstructions; determining a motion of a predetermined portion (205'), which is neighbored to a part (501,502) of the object to be reconstructed, of each of the adapted shape models (206);

selecting a specific data set of the sequence of data sets, wherein the specific data set corresponds to the adapted shape model (206) with the minimum motion of the predetermined portion; and

reconstructing the fine reproduction of at least the part (501,502) of the object (130) using the specific data set, and

wherein the part of the object is a coronary of a heart and wherein the predetermined portion corresponds to the left or right ventricle of the human heart and wherein the time scheduling unit (135) is an ECG device.

2. The reconstruction unit of claim 1, wherein the reconstruction unit is adapted to process scheduling information which is a sequence of points in time.
3. The reconstruction unit of claim 2, wherein the reconstruction unit is adapted to process scheduling information which is a sequence of phase points.

4. The reconstruction unit of claim 3, wherein the phase points are phase points of a cardiac phase.

5. The reconstruction unit of one of the claims 1 to 4, wherein the time scheduling unit (135) is an ECG device, wherein the reconstruction unit is adapted for receiving scheduling information from an ECG recording.

6. The reconstruction unit of one of the claims 1 to 5, wherein the reconstruction unit is adapted to process a sequence of data sets, which is a sequence of CT projection data sets.

7. The reconstruction unit of one of the claims 1 to 6, wherein the reconstruction unit is adapted for selecting the specific data set of the predetermined portion with minimum motion by:

generating a set of motion vectors belonging to the predetermined portion of the shape model, wherein the set of motion vectors is generated at each of the adapted models (206);

determining the minimum of the absolute length of the set of motion vectors of the predetermined portion of the adapted models (206).

8. A computer-implemented method for image reconstructing a fine reproduction of at least a part (501,502) of an object (130), the method comprising:

receiving a sequence of measured data sets measured by an examination apparatus, the data sets representing structural information of the object (130);

receiving scheduling information from a time scheduling unit (135), said scheduling information related to a sequencing of the sequence of data sets;

reconstructing a sequence of coarse reconstructions of the object (130) by using the sequence of data sets and the scheduling information;

detecting sub-structures in the sequence of coarse reconstructions by processing the sequence of coarse reconstructions;

generating a sequence of adapted shape models (206) of the object (130) by adapting a deformable shape model (503) to the detected sub-structures of each of the coarse reconstructions;

determining a motion of a predetermined portion (205'), which is neighbored to a part (501,502) of the object to be reconstructed, of each of the adapted shape models (206);

selecting a specific data set of the sequence of data sets, wherein the specific data set corresponds to the shape adapted model (206) with

- the minimum motion of the predetermined portion; and  
reconstructing the fine reproduction of at least the part (501,502) of the object (130) using the specific data set, and  
wherein the part of the object is a coronary of a heart and wherein the predetermined portion corresponds to the left or right ventricle of the human heart and wherein the time scheduling unit (135) is an ECG device.
- 5
9. An examination apparatus for reconstructing a fine reproduction of at least a part (501,502) of an object, the examination apparatus comprising:
- 10
- a reconstruction unit (118) of one of the claims 1 to 7;  
a detector unit (108);  
the time scheduling unit (135);
- 15
- wherein the detector unit (108) is connected to the reconstruction unit (118);
- 20
- wherein the time scheduling unit 108 is connected to the reconstruction unit (118);
- 25
- wherein the detector unit (108) is adapted for providing the data set containing structural information about the object (130);  
wherein the time scheduling unit (135) is adapted for providing the scheduling information related to the data set.
- 30
10. The examination apparatus of claim 9, further comprising:
- 35
- a memory unit (402);
- wherein the memory unit (402) is adapted for storing the sequence of data sets and the scheduling information.
- 40
11. The examination apparatus of claim 9 or 10, further comprising:
- 45
- a graphical user-interface (121);
- wherein the graphical user interface (121) is adapted for controlling the examination apparatus.
- 50
12. The examination apparatus of one of the claims 9 to 11, wherein the examination apparatus is at least one selected of the group consisting of a material testing apparatus, a baggage inspection apparatus, a medical application apparatus, a computer tomography apparatus, a coherent scatter computed tomography apparatus, a positron emission computed tomography apparatus, a single photon emission
- 55
- computed tomography apparatus, ultra sound apparatus, electron beam tomography apparatus, magnetic resonance apparatus, and an interventional 3D rotational X-ray device.
13. A computer-readable medium, in which a computer program for image reconstructing a fine reproduction of at least a part (501,502) of an object is stored, which, when being executed by a processor, is adapted to carry out:
- receiving a sequence of measured data sets measured by an examination apparatus, the data sets representing structural information of the object (130);  
receiving scheduling information from a time scheduling unit (135), said scheduling information related to a sequencing of the sequence of data sets;  
reconstructing a sequence of coarse reconstructions of the object (130) by using the sequence of data sets and the scheduling information;  
detecting sub-structures in the sequence of coarse reconstructions by processing the sequence of coarse reconstructions;  
generating a sequence of adapted shape models (206) of the object (130) by adapting a deformable shape model (503) to the detected sub-structures of each of the coarse reconstructions;  
determining a motion of a predetermined portion (205'), which is neighbored to a part (501,502) of the object to be reconstructed, of each of the adapted shape models (206);  
selecting a specific data set of the sequence of data sets, wherein the specific data set corresponds to the adapted shape model (206) with the minimum motion of the predetermined portion; and  
reconstructing the fine reproduction of at least the part (501,502) of the object (130) using the specific data set, and  
wherein the part of the object is a coronary of a heart and wherein the predetermined portion corresponds to the left or right ventricle of the human heart and wherein the time scheduling unit (135) is an ECG device.
14. A program element for image reconstructing a fine reproduction of at least a part (501,502) of the object, which, when being executed by a processor, is adapted to carry out:
- receiving a sequence of measured data sets measured by an examination apparatus, the data sets representing structural information of the object (130);  
receiving scheduling information from a time

scheduling unit (135), said scheduling information related to a sequencing of the sequence of data sets;

reconstructing a sequence of coarse reconstructions of the object (130) by using the sequence of data sets and the scheduling information;

detecting sub-structures in the sequence of coarse reconstructions by processing the sequence of coarse reconstructions;

generating a sequence of adapted shape models (206) of the object (130) by adapting a deformable shape model (503) to the detected sub-structures of each of the coarse reconstructions;

determining a motion of a predetermined portion (205'), which is neighbored to a part (501,502) of the object to be reconstructed, of each of the adapted shape models (206);

selecting a specific data set of the sequence of data sets, wherein the specific data set corresponds to the adapted shape model (206) with the minimum motion of the predetermined portion; and

reconstructing the fine reproduction of at least the part (501,502) of the object (130) using the specific data set, and wherein the part of the object is a coronary of a heart and wherein the predetermined portion corresponds to the left or right ventricle of the human heart and wherein the time scheduling unit (135) is an ECG device.

## Patentansprüche

1. Bildrekonstruktionseinheit zur Rekonstruktion einer Feinreproduktion von zumindest einem Teil (501,502) eines Objekts (130), wobei die Rekonstruktionseinheit (118) so eingerichtet ist, dass sie:

eine Sequenz von, von einer Untersuchungsvorrichtung gemessenen Messdatensätzen empfängt, wobei die Datensätze strukturelle Informationen des Objekts (130) darstellen;

Planungsinformationen von einer Zeitplanungseinheit (135) empfängt, wobei die Planungsinformationen auf eine Sequenzierung der Sequenz von Datensätzen bezogen sind;

eine Sequenz von groben Rekonstruktionen des Objekts (130) unter Verwendung der Sequenz von Datensätzen und der Planungsinformationen rekonstruiert;

Substrukturen in der Sequenz von groben Rekonstruktionen durch Verarbeiten der Sequenz von groben Rekonstruktionen detektiert;

eine Sequenz von adaptierten Formmodellen (206) des Objekts (130) durch Adaptieren eines deformierbaren Formmodells (503) an die de-

tektierten Substrukturen von jeder der groben Rekonstruktionen erzeugt;

eine Bewegung eines vorher festgelegten Abschnitts (205'), der an einen zu rekonstruierenden Teil (501,502) des Objekts angrenzt, von jedem der adaptierten Formmodelle (206) ermittelt;

einen spezifischen Datensatz der Sequenz von Datensätzen auswählt, wobei der spezifische Datensatz dem adaptierten Formmodell (206) mit der minimalen Bewegung des vorher festgelegten Abschnitts entspricht; und

die Feinreproduktion von zumindest dem Teil (501,502) des Objekts (130) unter Verwendung des spezifischen Datensatzes rekonstruiert, und

wobei es sich bei dem Teil des Objekts um einen koronaren Teil eines Herzens handelt, und wobei der vorher festgelegte Abschnitt der linken oder rechten Herzkammer des menschlichen Herzens entspricht, und wobei die Zeitplanungseinheit (135) ein EKG-Gerät ist.

2. Rekonstruktionseinheit nach Anspruch 1, wobei die Rekonstruktionseinheit so eingerichtet ist, dass sie Planungsinformationen, die eine Sequenz von Zeitpunkten darstellen, verarbeitet.

3. Rekonstruktionseinheit nach Anspruch 2, wobei die Rekonstruktionseinheit so eingerichtet ist, dass sie Planungsinformationen, die eine Sequenz von Phasenpunkten darstellen, verarbeitet.

4. Rekonstruktionseinheit nach Anspruch 3, wobei es sich bei den Phasenpunkten um Phasenpunkte einer kardialen Phase handelt.

5. Rekonstruktionseinheit nach einem der Ansprüche 1 bis 4, wobei die Zeitplanungseinheit (135) ein EKG-Gerät ist, wobei die Rekonstruktionseinheit so eingerichtet ist, dass sie Planungsinformationen aus einer EKG-Aufzeichnung empfängt.

6. Rekonstruktionseinheit nach einem der Ansprüche 1 bis 5, wobei die Rekonstruktionseinheit so eingerichtet ist, dass sie eine Sequenz von Datensätzen verarbeitet, bei der es sich um eine Sequenz von CT-Projektionsdatensätzen handelt.

7. Rekonstruktionseinheit nach einem der Ansprüche 1 bis 6, wobei die Rekonstruktionseinheit so eingerichtet ist, dass sie den spezifischen Datensatz des vorher festgelegten Abschnitts mit minimaler Bewegung auswählt durch:

Erzeugen eines Satzes von Bewegungsvektoren, die zu dem vorher festgelegten Abschnitt des Formmodells gehören, wobei der Satz von

- Bewegungsvektoren bei jedem der adaptierten Modelle (206) erzeugt wird;  
Ermitteln des Minimums der absoluten Länge des Satzes von Bewegungsvektoren des vorher festgelegten Abschnitts der adaptierten Modelle (206). 5
- 8.** Computerimplementiertes Verfahren zur Bildrekonstruktion einer Feinreproduktion von zumindest einem Teil (501,502) eines Objekts (130), wobei das Verfahren die folgenden Schritte umfasst, wonach: 10
- eine Sequenz von, von einer Untersuchungsvorrichtung gemessenen Messdatensätzen empfangen wird, wobei die Datensätze Strukturinformationen des Objekts (130) darstellen; 15
- Planungsinformationen von einer Zeitplanungseinheit (135) empfangen werden, wobei die Planungsinformationen auf eine Sequenzierung der Sequenz von Datensätzen bezogen sind; 20
- eine Sequenz von groben Rekonstruktionen des Objekts (130) unter Verwendung der Sequenz von Datensätzen und der Planungsinformationen rekonstruiert wird; 25
- Substrukturen in der Sequenz von groben Rekonstruktionen durch Verarbeiten der Sequenz von groben Rekonstruktionen detektiert werden; 30
- eine Sequenz von adaptierten Formmodellen (206) des Objekts (130) durch Adaptieren eines deformierbaren Formmodells (503) an die detektierten Substrukturen von jeder der groben Rekonstruktionen erzeugt wird; 35
- eine Bewegung eines vorher festgelegten Abschnitts (205'), der an einen zu rekonstruierenden Teil (501,502) des Objekts angrenzt, von jedem der adaptierten Formmodelle (206) ermittelt wird; 40
- ein spezifischer Datensatz der Sequenz von Datensätzen ausgewählt wird, wobei der spezifische Datensatz dem formadaptierten Modell (206) mit der minimalen Bewegung des vorher festgelegten Abschnitts entspricht; und 45
- die Feinreproduktion von zumindest dem Teil (501,502) des Objekts (130) unter Verwendung des spezifischen Datensatzes rekonstruiert wird, und 50
- wobei es sich bei dem Teil des Objekts um einen koronaren Teil eines Herzens handelt, und wobei der vorher festgelegte Abschnitt der linken oder rechten Herzkammer des menschlichen Herzens entspricht, und wobei die Zeitplanungseinheit (135) ein EKG-Gerät ist. 55
- 9.** Untersuchungsvorrichtung zur Rekonstruktion einer Feinreproduktion von zumindest einem Teil (501,502) eines Objekts, wobei die Untersuchungsvorrichtung umfasst:
- eine Rekonstruktionseinheit (118) nach einem der Ansprüche 1 bis 7;  
eine Detektoreinheit (108);  
eine Zeitplanungseinheit (135);  
wobei die Detektoreinheit (108) mit der Rekonstruktionseinheit (118) verbunden ist;  
wobei die Zeitplanungseinheit (135) mit der Rekonstruktionseinheit (118) verbunden ist;  
wobei die Detektoreinheit (108) so eingerichtet ist, dass sie den, strukturelle Informationen über das Objekt (130) enthaltenden Datensatz bereitstellt;  
wobei die Zeitplanungseinheit (135) so eingerichtet ist, dass sie die auf den Datensatz bezogenen Planungsinformationen bereitstellt.
- 10.** Untersuchungsvorrichtung nach Anspruch 9, weiterhin umfassend:
- eine Speichereinheit (402);  
wobei die Speichereinheit (402) so eingerichtet ist, dass sie die Sequenz von Datensätzen sowie die Planungsinformationen speichert.
- 11.** Untersuchungsvorrichtung nach Anspruch 9 oder 10, weiterhin umfassend:
- eine grafische Benutzeroberfläche (121);  
wobei die grafische Benutzeroberfläche (121) so eingerichtet ist, dass sie die Untersuchungsvorrichtung steuert.
- 12.** Untersuchungsvorrichtung nach einem der Ansprüche 9 bis 11, wobei die Untersuchungsvorrichtung mindestens eine solche ist, die aus der Gruppe, bestehend aus einer Materialprüfungsvorrichtung, einer Gepäckkontrollvorrichtung, einer Vorrichtung für medizinische Anwendungen, einer Computertomographievorrichtung, einer Computertomographievorrichtung mit kohärenter Streustrahlung, einer Positronen-Emissions-Computertomographievorrichtung, einer Einzelphotonen-Emissions-Computertomographievorrichtung, einer Ultraschallvorrichtung, einer Elektronenstrahltomographievorrichtung, einer Magnetresonanzvorrichtung sowie einer interventionellen 3D-Rotationsröntgenvorrichtung, ausgewählt wird.
- 13.** Computerlesbares Medium, in dem ein Computerprogramm zur Bildrekonstruktion einer Feinreproduktion von zumindest einem Teil (501,502) eines Objekts gespeichert wird, das bei Ausführung durch einen Prozessor so eingerichtet ist, dass es;  
eine Sequenz von, von einer Untersuchungsvorrichtung gemessenen Messdatensätzen empfängt, wobei die Datensätze strukturelle Informationen des Objekts (130) darstellen;

Planungsinformationen von einer Zeitplanungseinheit (135) empfängt, wobei die Planungsinformationen auf eine Sequenzierung der Sequenz von Datensätzen bezogen sind;

eine Sequenz von groben Rekonstruktionen des Objekts (130) unter Verwendung der Sequenz von Datensätzen und der Planungsinformationen rekonstruiert;

Substrukturen in der Sequenz von groben Rekonstruktionen durch Verarbeiten der Sequenz von groben Rekonstruktionen detektiert;

eine Sequenz von adaptierten Formmodellen (206) des Objekts (130) durch Adaptieren eines deformierbaren Formmodells (503) an die detektierten Substrukturen von jeder der groben Rekonstruktionen erzeugt;

eine Bewegung eines vorher festgelegten Abschnitts (205'), der an einen zu rekonstruierenden Teil (501,502) des Objekts angrenzt, von jedem der adaptierten Formmodelle (206) ermittelt;

einen spezifischen Datensatz der Sequenz von Datensätzen auswählt, wobei der spezifische Datensatz dem adaptierten Formmodell (206) mit der minimalen Bewegung des vorher festgelegten Abschnitts entspricht; und

die Feinreproduktion von zumindest dem Teil (501,502) des Objekts (130) unter Verwendung des spezifischen Datensatzes rekonstruiert, und wobei es sich bei dem Teil des Objekts um einen koronaren Teil eines Herzens handelt, und wobei der vorher festgelegte Abschnitt der linken oder rechten Herzkammer des menschlichen Herzens entspricht, und wobei die Zeitplanungseinheit (135) ein EKG-Gerät ist.

14. Programmelement zur Bildrekonstruktion einer Feinreproduktion von zumindest einem Teil (501,502) des Objekts, das bei Ausführung durch einen Prozessor so eingerichtet ist, dass es die folgenden Schritte ausführt, wonach es:

eine Sequenz von, von einer Untersuchungsvorrichtung gemessenen Messdatensätzen empfängt, wobei die Datensätze strukturelle Informationen des Objekts (130) darstellen;

Planungsinformationen von einer Zeitplanungseinheit (135) empfängt, wobei die Planungsinformationen auf eine Sequenzierung der Sequenz von Datensätzen bezogen sind;

eine Sequenz von groben Rekonstruktionen des Objekts (130) unter Verwendung der Sequenz von Datensätzen und der Planungsinformationen rekonstruiert;

Substrukturen in der Sequenz von groben Rekonstruktionen durch Verarbeiten der Sequenz von groben Rekonstruktionen detektiert;

eine Sequenz von adaptierten Formmodellen (206) des Objekts (130) durch Adaptieren eines

deformierbaren Formmodells (503) an die detektierten Substrukturen von jeder der groben Rekonstruktionen erzeugt;

eine Bewegung eines vorher festgelegten Abschnitts (205'), der an einen zu rekonstruierenden Teil (501,502) des Objekts angrenzt, von jedem der adaptierten Formmodelle (206) ermittelt;

einen spezifischen Datensatz der Sequenz von Datensätzen auswählt, wobei der spezifische Datensatz dem adaptierten Formmodell (206) mit der minimalen Bewegung des vorher festgelegten Abschnitts entspricht; und

die Feinreproduktion von zumindest dem Teil (501,502) des Objekts (130) unter Verwendung des spezifischen Datensatzes rekonstruiert, und

wobei es sich bei dem Teil des Objekts um einen koronaren Teil eines Herzens handelt, und wobei der vorher festgelegte Abschnitt der linken oder rechten Herzkammer des menschlichen Herzens entspricht, und wobei die Zeitplanungseinheit (135) ein EKG-Gerät ist.

#### Revendications

1. Unité de reconstruction d'image pour reconstruire une reproduction fine d'au moins une partie (501, 502) d'un objet (130), dans laquelle l'unité de reconstruction (118) est adaptée pour :

recevoir une séquence d'ensembles de données mesurées mesurés par un appareil d'examen, les ensembles de données représentant des informations structurales de l'objet (130) ; recevoir des informations d'ordonnement en provenance d'une unité d'ordonnement temporel (135), lesdites informations d'ordonnement se rapportant à un séquençage de la séquence d'ensembles de données ;

reconstruire une séquence de reconstructions grossières de l'objet (130) en utilisant la séquence d'ensembles de données et les informations d'ordonnement ;

détecter des sous-structures dans la séquence de reconstructions grossières en traitant la séquence de reconstructions grossières ;

générer une séquence de modèles de forme adaptés (206) de l'objet (130) en adaptant un modèle de forme déformable (503) aux sous-structures détectées de chacune des reconstructions grossières ;

déterminer un mouvement d'une portion prédéterminée (205'), qui est voisine d'une partie (501, 502) de l'objet à reconstruire, de chacun des modèles de forme adaptés (206) ;

sélectionner un ensemble de données spécifi-

- ques de la séquence d'ensembles de données, dans laquelle l'ensemble de données spécifique correspond au modèle de forme adapté (206) avec le mouvement minimum de la portion prédéterminée ; et
- reconstruire la reproduction fine d'au moins la partie (501, 502) de l'objet (130) à l'aide de l'ensemble de données spécifique, et
- dans laquelle la partie de l'objet est un coronaire d'un coeur et dans laquelle la portion prédéterminée correspond au ventricule gauche ou droit du coeur humain et dans laquelle l'unité d'ordonnement temporel (135) est un dispositif d'ECG.
2. Unité de reconstruction selon la revendication 1, dans laquelle l'unité de reconstruction est adaptée pour traiter des informations d'ordonnement qui sont une séquence de points dans le temps.
  3. Unité de reconstruction selon la revendication 2, dans laquelle l'unité de reconstruction est adaptée pour traiter des informations d'ordonnement qui sont une séquence de points de phase.
  4. Unité de reconstruction selon la revendication 3, dans laquelle les points de phase sont des points de phase d'une phase cardiaque.
  5. Unité de reconstruction selon l'une des revendications 1 à 4, dans laquelle l'unité d'ordonnement temporel (135) est un dispositif d'ECG, dans laquelle l'unité de reconstruction est adaptée pour recevoir des informations d'ordonnement en provenance d'un enregistrement d'ECG.
  6. Unité de reconstruction selon l'une des revendications 1 à 5, dans laquelle l'unité de reconstruction est adaptée pour traiter une séquence d'ensembles de données, qui est une séquence d'ensembles de données de projection CT.
  7. Unité de reconstruction selon l'une des revendications 1 à 6, dans laquelle l'unité de reconstruction est adaptée pour sélectionner l'ensemble de données spécifique de la portion prédéterminée avec un mouvement minimum en :

général un ensemble de vecteurs de mouvement appartenant à la portion prédéterminée du modèle de forme, dans laquelle l'ensemble de vecteurs de mouvement est généré au niveau de chacun des modèles adaptés (206) ; déterminant le minimum de la longueur absolue de l'ensemble de vecteurs de mouvement de la portion prédéterminée des modèles adaptés (206).

8. Procédé mis en oeuvre par ordinateur pour la reconstruction en image d'une reproduction fine d'au moins une partie (501, 502) d'un objet (130), le procédé comprenant :
  - la réception d'une séquence d'ensembles de données mesurées mesurés par un appareil d'examen, les ensembles de données représentant des informations structurales de l'objet (130) ;
  - la réception d'informations d'ordonnement en provenance d'une unité d'ordonnement temporel (135), lesdites informations d'ordonnement se rapportant à un séquençage de la séquence d'ensembles de données ;
  - la reconstruction d'une séquence de reconstructions grossières de l'objet (130) en utilisant la séquence d'ensembles de données et les informations d'ordonnement ;
  - la détection de sous-structures dans la séquence de reconstructions grossières en traitant la séquence de reconstructions grossières ;
  - la génération d'une séquence de modèles de forme adaptés (206) de l'objet (130) en adaptant un modèle de forme déformable (503) aux sous-structures détectées de chacune des reconstructions grossières ;
  - la détermination d'un mouvement d'une portion prédéterminée (205'), qui est voisine d'une partie (501, 502) de l'objet à reconstruire, de chacun des modèles de forme adaptés (206) ;
  - la sélection d'un ensemble de données spécifiques de la séquence d'ensembles de données, dans laquelle l'ensemble de données spécifique correspond au modèle de forme adapté (206) avec le mouvement minimum de la portion prédéterminée ; et
  - la reconstruction de la reproduction fine d'au moins la partie (501, 502) de l'objet (130) à l'aide de l'ensemble de données spécifique, et dans lequel la partie de l'objet est un coronaire d'un coeur et dans lequel la portion prédéterminée correspond au ventricule gauche ou droit du coeur humain et dans lequel l'unité d'ordonnement temporel (135) est un dispositif d'ECG.

9. Appareil d'examen pour reconstruire une reproduction fine d'au moins une partie (501, 502) d'un objet, l'appareil d'examen comprenant :
  - une unité de reconstruction (118) selon l'une des revendications 1 à 7 ;
  - une unité de détection (108) ;
  - l'unité d'ordonnement temporel (135) ;
  - dans lequel l'unité de détection (108) est connectée à l'unité de reconstruction (118) ;
  - dans lequel l'unité d'ordonnement temporel

- (135) est connectée à l'unité de reconstruction (118) ;  
dans lequel l'unité de détection (108) est adaptée pour fournir l'ensemble de données contenant des informations structurelles concernant l'objet (130) ;  
dans lequel l'unité d'ordonnement temporel (135) est adaptée pour fournir les informations d'ordonnement liées à l'ensemble de données.
- 5
- 10
10. Appareil d'examen selon la revendication 9, comprenant en outre :
- une unité de mémoire (402) ;  
dans lequel l'unité de mémoire (402) est adaptée pour stocker la séquence d'ensembles de données et les informations d'ordonnement.
- 15
11. Appareil d'examen selon la revendication 9 ou 10, comprenant en outre :
- une interface utilisateur graphique (121) ;  
dans lequel l'interface utilisateur graphique (121) est adaptée pour commander l'appareil d'examen.
- 20
- 25
12. Appareil d'examen selon l'une des revendications 9 à 11, dans lequel l'appareil d'examen est au moins l'un sélectionné dans le groupe constitué d'un appareil de test de matériel, d'un appareil d'inspection de bagages, d'un appareil d'application médicale, d'un appareil de tomographie à diffusion cohérente, d'un appareil de tomographie à émission de positrons, d'un appareil de tomographie à émission de photon unique, d'un appareil à ultrasons, d'un appareil de tomographie à faisceau d'électrons, d'un appareil à résonance magnétique, et d'un dispositif à rayons X rotatif en 3D d'intervention.
- 30
- 35
- 40
13. Support lisible par ordinateur, dans lequel un programme informatique pour la reconstruction en image d'une reproduction fine d'au moins une partie (501, 502) d'un objet est stocké, qui, lorsqu'il est exécuté par un processeur, est adapté pour réaliser :
- 45
- la réception d'une séquence d'ensembles de données mesurées mesurés par un appareil d'examen, les ensembles de données représentant des informations structurelles de l'objet (130) ;  
la réception d'informations d'ordonnement en provenance d'une unité d'ordonnement temporel (135), lesdites informations d'ordonnement se rapportant à un séquençage de la séquence d'ensembles de données ;  
la reconstruction d'une séquence de reconstructions grossières de l'objet (130) en utilisant la séquence d'ensembles de données et les informations d'ordonnement ;  
la détection de sous-structures dans la séquence de reconstructions grossières en traitant la séquence de reconstructions grossières ;  
la génération d'une séquence de modèles de forme adaptés (206) de l'objet (130) en adaptant un modèle de forme déformable (503) aux sous-structures détectées de chacune des reconstructions grossières ;
- 50
- 55
- tions grossières de l'objet (130) en utilisant la séquence d'ensembles de données et les informations d'ordonnement ;  
la détection de sous-structures dans la séquence de reconstructions grossières en traitant la séquence de reconstructions grossières ;  
la génération d'une séquence de modèles de forme adaptés (206) de l'objet (130) en adaptant un modèle de forme déformable (503) aux sous-structures détectées de chacune des reconstructions grossières ;  
la détermination d'un mouvement d'une portion prédéterminée (205'), qui est voisine d'une partie (501, 502) de l'objet à reconstruire, de chacun des modèles de forme adaptés (206) ;  
la sélection d'un ensemble de données spécifiques de la séquence d'ensembles de données, dans laquelle l'ensemble de données spécifique correspond au modèle de forme adapté (206) avec le mouvement minimum de la portion prédéterminée ; et  
la reconstruction de la reproduction fine d'au moins la partie (501, 502) de l'objet (130) à l'aide de l'ensemble de données spécifique, et dans lequel la partie de l'objet est un coronaire d'un coeur et dans lequel la portion prédéterminée correspond au ventricule gauche ou droit du coeur humain et dans lequel l'unité d'ordonnement temporel (135) est un dispositif d'ECG.
14. Élément de programme pour la reconstruction en image d'une reproduction fine d'au moins une partie (501, 502) de l'objet, qui, lorsqu'il est exécuté par un processeur, est adapté pour réaliser :
- la réception d'une séquence d'ensembles de données mesurées mesurés par un appareil d'examen, les ensembles de données représentant des informations structurelles de l'objet (130) ;  
la réception d'informations d'ordonnement en provenance d'une unité d'ordonnement temporel (135), lesdites informations d'ordonnement se rapportant à un séquençage de la séquence d'ensembles de données ;  
la reconstruction d'une séquence de reconstructions grossières de l'objet (130) en utilisant la séquence d'ensembles de données et les informations d'ordonnement ;  
la détection de sous-structures dans la séquence de reconstructions grossières en traitant la séquence de reconstructions grossières ;  
la génération d'une séquence de modèles de forme adaptés (206) de l'objet (130) en adaptant un modèle de forme déformable (503) aux sous-structures détectées de chacune des reconstructions grossières ;

la détermination d'un mouvement d'une portion prédéterminée (205'), qui est voisine d'une partie (501, 502) de l'objet à reconstruire, de chacun des modèles de forme adaptés (206) ;  
la sélection d'un ensemble de données spécifiques de la séquence d'ensembles de données, dans laquelle l'ensemble de données spécifique correspond au modèle de forme adapté (206) avec le mouvement minimum de la portion prédéterminée ; et  
la reconstruction de la reproduction fine d'au moins la partie (501, 502) de l'objet (130) à l'aide de l'ensemble de données spécifique, et dans lequel la partie de l'objet est un coronaire d'un coeur et dans lequel la portion prédéterminée correspond au ventricule gauche ou droit du coeur humain et dans lequel l'unité d'ordonnement temporel (135) est un dispositif d'ECG.

5

10

15

20

25

30

35

40

45

50

55



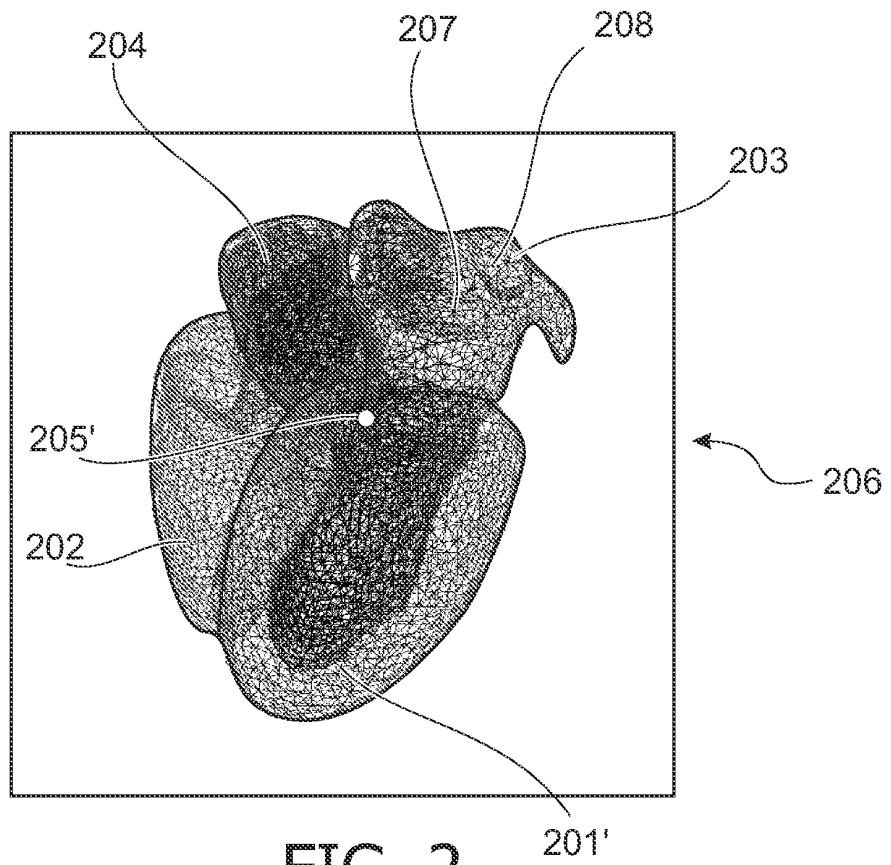


FIG. 2

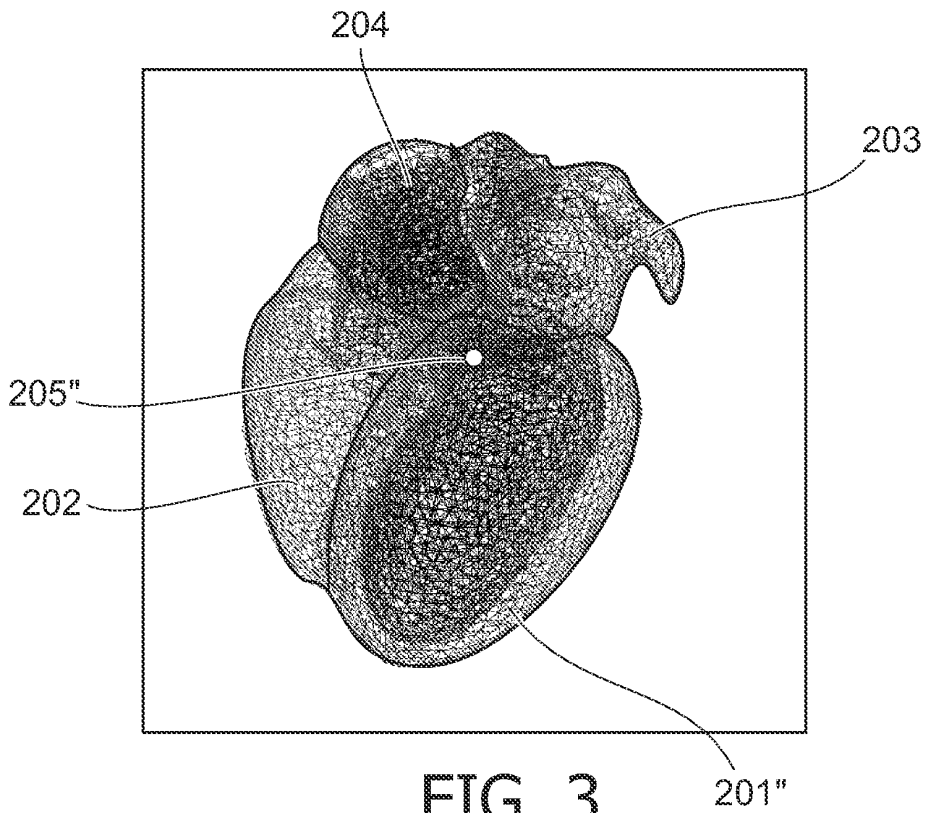


FIG. 3

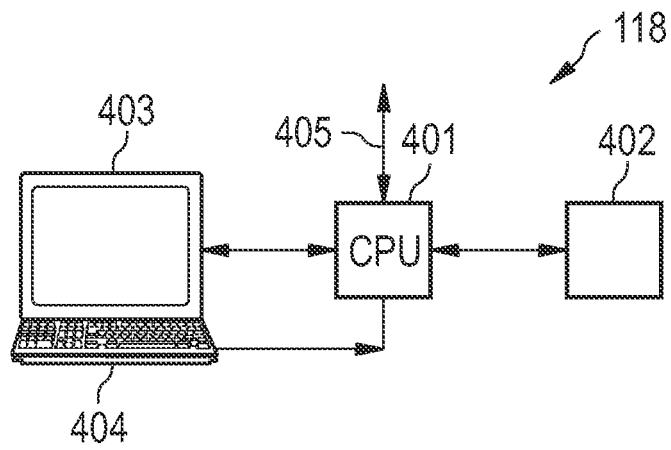


FIG. 4

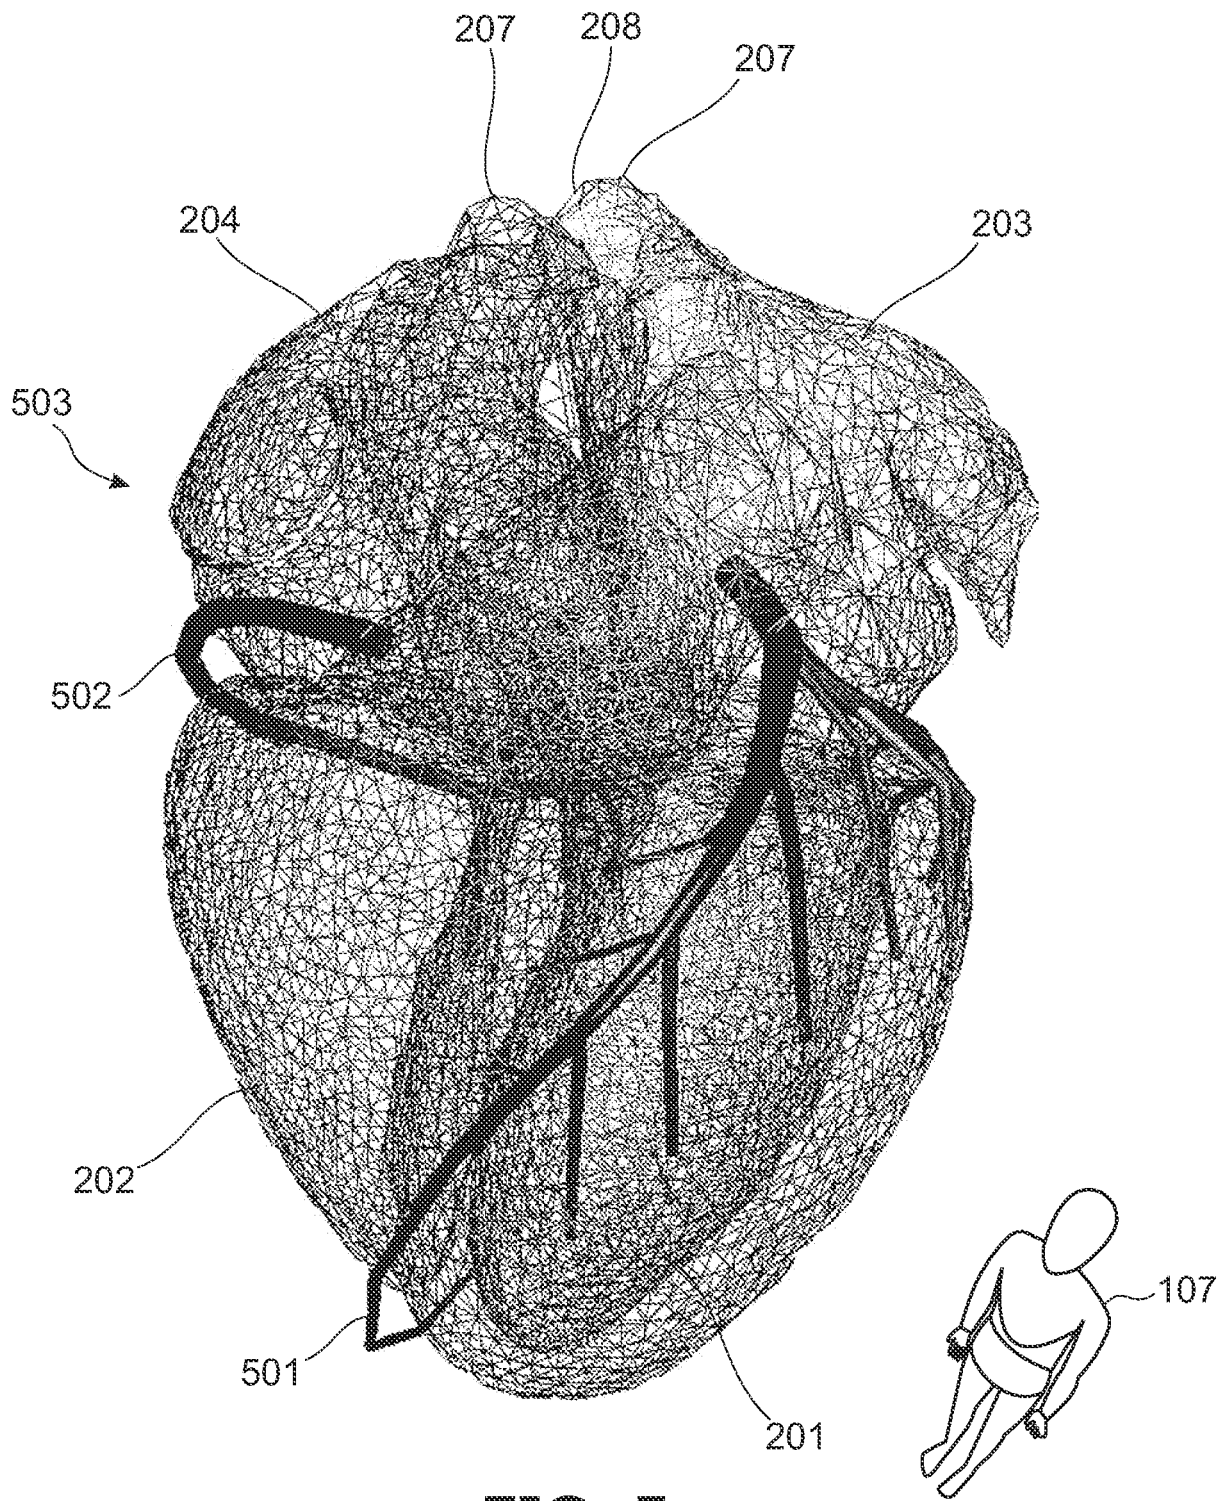


FIG. 5

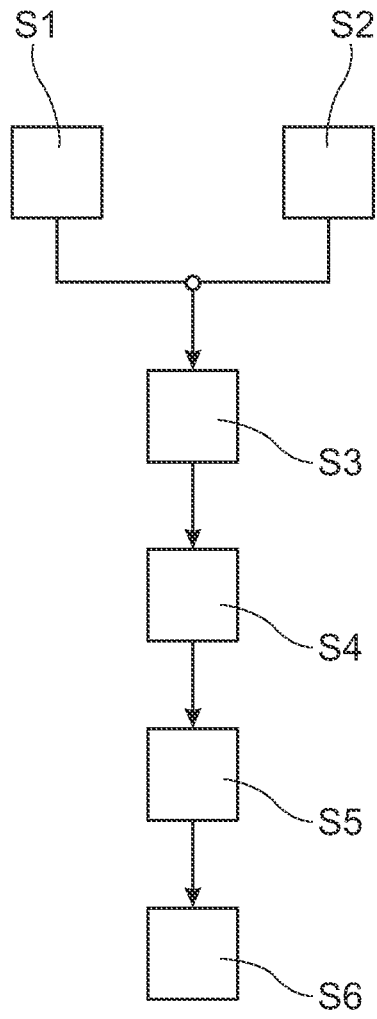


FIG. 6

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 6628743 B1 [0008]
- WO 2005008597 A [0009]
- WO 02103639 A2 [0010]

**Non-patent literature cited in the description**

- **R. MANZKE et al.** Automatic phase determination for retrospectively gated cardiac CT. *Medical Physics*, December 2004, vol. 31 (12 [0006])
- **VEMBAR et al.** A dynamic approach to identifying desired physiological phases for cardiac imaging using multislice spiral CT. *Medical Physics*, July 2003, vol. 30 (7 [0007])

专利名称(译)	重建单元，用于重建对象的至少一部分的精细再现		
公开(公告)号	<a href="#">EP1965703B1</a>	公开(公告)日	2017-06-07
申请号	EP2006832175	申请日	2006-12-08
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	飞利浦知识产权及标准部GMBH 皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	飞利浦知识产权及标准部GMBH 皇家飞利浦N.V.		
[标]发明人	GRASS MICHAEL VON BERG JENS LORENZ CRISTIAN		
发明人	GRASS, MICHAEL VON BERG, JENS LORENZ, CRISTIAN		
IPC分类号	A61B6/03 A61B6/00 G06T11/00 A61B5/00		
CPC分类号	A61B5/7289 A61B6/032 A61B6/4085 A61B6/503 G06T11/005 G06T2211/412		
代理机构(译)	德哈恩波尔ERIK		
优先权	2005112496 2005-12-20 EP		
其他公开文献	EP1965703A2		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

提供重建单元用于接收数据集序列，该数据集表示对象的结构信息。重建单元执行接收与数据集序列的数据集有关的调度信息。然后，通过使用数据集序列和调度信息重建对象的粗略重建序列。然后，通过使相应的模型适应每个粗略重建来生成对象的一系列适应模型。然后，确定每个适应模型的预定部分的运动，并选择数据序列序列的特定数据集，其中特定数据集对应于具有预定部分的最小运动的适应模型。最后，重建单元使用特定数据集执行至少部分对象的精细重建。

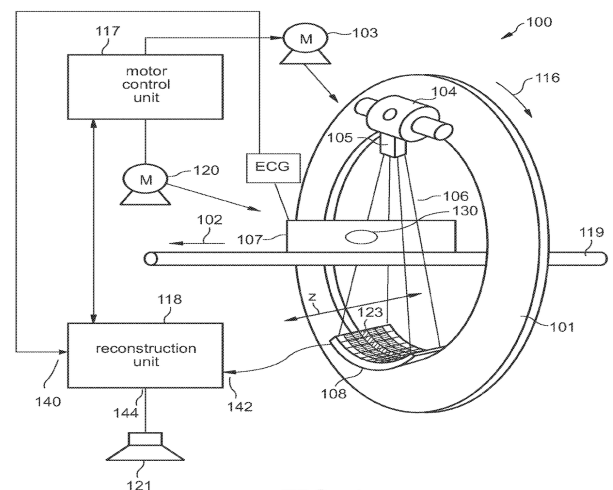


FIG. 1