

(19)



(11)

**EP 2 765 907 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:

**18.05.2016 Bulletin 2016/20**

(51) Int Cl.:

**A61B 5/053** <sup>(2006.01)</sup>      **A61B 5/107** <sup>(2006.01)</sup>  
**A61B 5/02** <sup>(2006.01)</sup>      **A61B 5/00** <sup>(2006.01)</sup>  
**A61B 5/0215** <sup>(2006.01)</sup>

(21) Application number: **12787943.5**

(86) International application number:

**PCT/US2012/059718**

(22) Date of filing: **11.10.2012**

(87) International publication number:

**WO 2013/055896 (18.04.2013 Gazette 2013/16)**

**(54) DEVICE FOR MEASURING AN ANATOMICAL STRUCTURE**

VORRICHTUNG ZUR MESSUNG EINER ANATOMISCHEN STRUKTUR

DISPOSITIF DE MESURE D'UNE STRUCTURE ANATOMIQUE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB  
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO  
PL PT RO RS SE SI SK SM TR**

(73) Proprietor: **Acist Medical Systems, Inc.**

**Eden Prairie, MN 55344 (US)**

(30) Priority: **14.10.2011 US 201161547306 P**

(72) Inventor: **HILTNER, Jason, Fredrick**

**Minnetonka, MN 55343 (US)**

(43) Date of publication of application:

**20.08.2014 Bulletin 2014/34**

(74) Representative: **Belloni, Giancarlo et al**

**Dragotti & Associati Srl**

**Via Nino Bixio, 7**

**20129 Milano (IT)**

(60) Divisional application:

**16163119.7**

(56) References cited:

**WO-A1-98/35611 WO-A2-2008/005388**

**EP 2 765 907 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### FIELD

**[0001]** This application relates generally to the field of medical device technology and, more particularly, to devices and methods for positioning and utilizing physiological sensors in anatomical structures of patients, such as in blood vessels or across heart valves. This application also relates generally to methods for calculating cross-sectional areas of anatomical structures.

### BACKGROUND

**[0002]** Patients sometimes experience stenosis in an anatomical structure. Stenosis occurs when an abnormal narrowing or stenotic lesion appears in the anatomical structure. Physicians generally evaluate the stenotic lesion before selecting a therapy to treat it. For example, in the case of blood vessels, if the stenotic lesion obstructs blood flow through the vessel to a large degree, physicians often elect to place a stent within the lesion site. On the other hand, if the stenotic lesion only minimally obstructs blood flow, physicians sometimes elect not to use a stent.

**[0003]** One technique for evaluating the degree to which a stenotic lesion obstructs flow through a blood vessel is called the Fractional Flow Reserve measurement (FFR). To calculate the FFR for a given stenotic lesion, two blood pressure readings are taken. One pressure reading is taken on the distal side of the lesion (e.g., downstream from the lesion) and the other pressure reading is taken on the proximal side of the lesion (e.g., upstream from the lesion, towards the aorta). The FFR is defined as the ratio of maximal blood flow in a stenotic lesion, taken distal to the lesion, to normal maximal flow, and is typically calculated based on a measured pressure gradient of the distal pressure to the proximal pressure. The FFR is therefore a unitless ratio of the distal and proximal pressures. The pressure gradient, or pressure drop, across a stenotic lesion is an indicator of the severity of the stenosis, and the FFR is a useful tool in assessing the pressure drop. The more restrictive the stenosis is, the greater the pressure drop, and the lower the resulting FFR.

**[0004]** The FFR measurement is considered a useful diagnostic tool. For example, clinical studies have shown that an FFR of less than about 0.8 or about 0.75 can be a useful criterion on which to base certain therapy decisions. A physician might decide, for example, to perform an interventional procedure (e.g., angioplasty or stent placement) when the FFR for a given stenotic lesion is below 0.8 or 0.75, and may decide to forego such treatment for lesions where the FFR is above 0.8 or 0.75. Thus, the FFR measurement provides a decision point for guiding treatment decisions.

**[0005]** Certain drawbacks are sometimes seen with the FFR method. First, the FFR method is designed

merely to determine whether an interventional procedure such as a stent is needed or not needed. It does not provide any tools for enabling a physician to select a stent size that is ideal for the specific stenotic lesion at issue.

5 Stents come in a variety of sizes, and physicians generally need to select an appropriate size and shape depending on the lesion characteristics. Physicians often need to use a separate procedure to determine what stent size to use. Commonly, physicians use an intravascular  
10 ultrasound method to determine a diameter of the vessel having the stenotic lesion. This method involves the advancement of a separate ultrasound catheter and the use of a separate ultrasound machine. This adds significant cost and time and more risk to the patient. Thus, it would  
15 also be desirable to provide a more simple system capable of both obtaining FFR measurements and selecting an appropriate stent size.

**[0006]** Another drawback seen with the FFR method is that the presence of a measuring device itself in the  
20 anatomical structure can affect the accuracy of the measurement. For example, as the measuring device crosses the stenotic lesion, the device itself introduces flow obstruction, in addition to that caused by the lesion itself. The measured distal pressure is sometimes lower than  
25 it would be without the additional flow obstruction, which may exaggerate the measured pressure gradient across the lesion. Thus, it would also be desirable to provide an improved system for obtaining more accurate FFR measurements.

30 **[0007]** Document WO 2008/005388 discloses the preamble of claim 1.

### BRIEF DESCRIPTION OF THE DRAWINGS

35 **[0008]** The following drawings are illustrative of particular embodiments of the invention and therefore do not limit the scope of the invention. The drawings are not to scale (unless so stated) and are intended for use in conjunction with the explanations in the following detailed  
40 description. Embodiments of the invention will hereinafter be described in conjunction with the appended drawings, wherein like numerals denote like elements.

45 Figure 1 is a perspective view of a sensor delivery device according to an embodiment of the invention;

Figure 2 is a perspective view of a sensor delivery device according to another embodiment of the invention;

50 Figure 3 is a perspective view of a sensor delivery device according to yet another embodiment of the invention;

55 Figure 4 is a perspective view of a sensor delivery device having a furncation tube according to an embodiment of the invention;

Figure 5 is a flow diagram of a method of using the sensor delivery device to measure a cross-sectional area of an anatomical structure;

Figure 6 is a flow diagram of a method of using the sensor delivery device to measure and adjust a FFR value of an anatomical structure;

Figure 7 is a flow diagram of a method of using the sensor delivery device to measure blood conductivity and fluid conductivity to calculate a cross-sectional area of an anatomical structure;

Figure 8 is a flow diagram of a method of using the sensor delivery device to measure conductivity of a first fluid and a second fluid to calculate a cross-sectional area of an anatomical structure;

Figure 9 is a flow diagram of a method of using the sensor delivery device to measure blood conductivity and fluid conductivity to calculate a cross-sectional area of an anatomical structure; and

Figure 10 is a flow diagram of a method of using the sensor delivery device to measure conductivity of a first fluid and a second fluid to calculate a cross-sectional area of an anatomical structure.

## SUMMARY

**[0009]** The invention is defined by claim 1.

**[0010]** Certain embodiments provide an intravascular sensor delivery device. The device can include a distal sleeve having a guidewire lumen for slidably receiving a medical guidewire, a first sensor coupled to the distal sleeve, wherein the first sensor is adapted to measure blood pressure and generate a signal representative of the blood pressure, a second sensor coupled to the distal sleeve, wherein the second sensor is adapted to measure cross-sectional area of a surrounding anatomical structure and generate a signal representative of the cross-sectional area, a proximal portion coupled to the distal sleeve, the proximal portion comprising a communication channel, wherein the communication channel communicates the signal from the first sensor and the signal from the second sensor to a location outside of the patient.

**[0011]** The second sensor of the intravascular sensor delivery device is an electrode arrangement, for example an electrode arrangement that includes source electrodes and sense electrodes, wherein the source electrodes generate a current and the sense electrodes measure voltage resulting from the current. The signal representative of the cross-sectional area can be voltage measured by the sense electrodes. The source electrodes and the sense electrodes can also be ring-shaped

electrodes that surround a periphery of the distal sleeve. The device can also include a movable sheath that is adapted to cover and uncover the electrode arrangement. The second sensor can be attached to an outer surface of the distal sleeve, perhaps at a location that is distal or proximal to the first sensor. In certain cases, the second sensor is coupled to both the distal sleeve and the proximal portion at a location that is proximal to the first sensor.

**[0012]** The intravascular sensor delivery device can also include third sensor. In such cases, the third sensor can be adapted to measure temperature and generate a signal representative of the temperature and wherein the communication channel communicates the signal from the first sensor, the signal from the second sensor, and the signal from the third sensor to a location outside of the patient. The first sensor and the third sensor can also be a single sensor, wherein the single sensor is adapted to both measure blood pressure and measure temperature.

**[0013]** Other embodiments not forming part of the invention provide an intravascular measuring system. The system can include a guidewire, an intravascular sensor delivery device, an injection device that is adapted to inject a fluid with a known conductivity to the anatomical structure, and a processor that is adapted to receive the first signal from the first sensor and the second signal from the second sensor. The injection device can be adapted to inject a first fluid (e.g., a NaCl solution having a first concentration, such as a 9% concentration) and a second fluid (e.g., a NaCl solution having a first concentration, such as a 4.5% concentration) into to the anatomical structure, wherein the first fluid has a first known conductivity and the second fluid has a second known conductivity, wherein the known conductivity of the first fluid is different than the known conductivity of the second fluid.

**[0014]** Further embodiments not forming part of the invention provide a method of determining cross-sectional area in an anatomical structure of a patient that includes steps of providing a sensor delivery device, wherein the sensor delivery device includes a distal sleeve having a guidewire lumen for slidably receiving a medical guidewire and a sensor coupled to the distal sleeve, wherein the sensor is adapted to measure fluid conductivity of a surrounding anatomical structure, (b) positioning the sensor delivery device within the anatomical structure, (c) administering a first fluid with a known conductivity to the anatomical structure (e.g., a NaCl solution having a first concentration, such as a 9% concentration), (d) using the sensor to measure a first conductivity for the first fluid, (e) administering a second fluid with a known conductivity to the anatomical structure (e.g., a NaCl solution having a first concentration, such as a 4.5% concentration), wherein the known conductivity of the first fluid is different than the known conductivity of the second fluid, (f) using the sensor to measure a second conductivity for the second fluid, and (g) using the first conduc-

tivity and the second conductivity to calculate a cross-sectional area of the anatomical structure.

**[0015]** Yet other embodiments not forming part of the invention provide a method of treating an anatomical structure in patient that includes steps of (a) providing a sensor delivery device, (b) positioning the sensor delivery device within the anatomical structure; (c) using the first sensor to obtain blood pressure measurements; (d) using the blood pressure measurements to calculate an FFR value; (e) electing to use a stent when the FFR value is lower than a threshold value, e.g., about 0.8, (f) using the second sensor to obtain one or more fluid conductivity measurements; (g) using the fluid conductivity measurements to calculate a cross-sectional area of the anatomical structure; and (h) using the cross-sectional area to select a stent size.

**[0016]** The step of using the cross-sectional area measurements to select a stent size can be a step of correlating a specific cross-sectional area measurement to a specific stent size. Also, the second sensor can be an electrode arrangement adapted to measure conductivity of fluid in the anatomical structure and the step of using the second sensor to obtain one or more cross-sectional area measurements can include steps of obtaining fluid conductivity measurements and calculating cross-sectional area measurements using the fluid conductivity measurements. The step of using the second sensor to obtain one or more cross-sectional area measurements can also include steps of (a) administering a first fluid (e.g., a NaCl solution having a first concentration, such as a 9% concentration)) with a known conductivity to the anatomical structure, (b) using the second sensor to measure a first conductivity for the first fluid, (c) administering a second fluid (e.g., a NaCl solution having a first concentration, such as a 4.5% concentration) with a known conductivity to the anatomical structure, wherein the conductivity of the first fluid is different than the conductivity of the second fluid, (d) using the second sensor to measure a second conductivity for the second fluid, and (e) using the first conductivity and the second conductivity to calculate a cross-sectional area of the anatomical structure.

**[0017]** The method can further include providing the sensor delivery device with a third sensor adapted to measure temperature of fluid in the anatomical structure, wherein the method includes steps of using the third sensor to measure fluid temperature and using the second sensor to obtain one or more cross-sectional area measurements after the fluid temperature reaches a desired temperature value.

**[0018]** Further embodiments not forming part of the invention provide a method of determining cross-sectional area in an anatomical structure of a patient that can include steps of (a) providing a sensor delivery device, wherein the sensor delivery device includes a distal sleeve having a guidewire lumen for slidably receiving a medical guidewire and a sensor coupled to the distal sleeve, wherein the sensor is adapted to measure fluid

conductivity, (b) positioning the sensor delivery device within the anatomical structure, (c) using the sensor to measure a conductivity for the patient's blood, (d) administering fluid with a known conductivity to the anatomical structure, (e) using the sensor to measure a conductivity for the fluid, and (f) using the measured blood conductivity and the measured fluid conductivity to calculate a cross-sectional area of the anatomical structure.

## 10 DETAILED DESCRIPTION

**[0019]** For the purpose of promoting an understanding of the principles of the invention, reference will now be made to the embodiments illustrated in the drawing and specific language will be used to describe the same. It will, nevertheless, be understood that no limitation of the scope of the invention is thereby intended; any alterations and further modifications of the described or illustrated embodiments, and any further applications of the principles of the invention as illustrated therein, are contemplated as would normally occur to one skilled in the art to which the invention relates.

**[0020]** In the foregoing detailed description, the invention has been described with reference to specific embodiments. However, it can be appreciated that various modifications and changes can be made without departing from the scope of the invention.

**[0021]** Figures 1-3 show a sensor delivery device 210 being deployed in an anatomical structure. Here, the anatomical structure is a blood vessel of a patient (e.g., coronary artery 234) across a stenotic lesion 236. As used herein, the term "anatomical structure" refers to any body structure having a cross-sectional area or a hollow, tubular or luminal structure.

**[0022]** The sensor delivery device 210 includes a distal sleeve 220 having a guidewire lumen 222 for slidably receiving a medical guidewire 230. A first sensor 240 and a second sensor 270 are each coupled to the distal sleeve 220. The first sensor 240 is capable of measuring blood pressure in the anatomical structure and generating a signal representative of the blood pressure. The second sensor 270 is capable of measuring cross-sectional area of the anatomical structure and generating a signal representative of the cross-sectional area. In some cases, the delivery device also includes a third sensor that is adapted to measure temperature of fluid in the anatomical structure and generate a signal representative of the temperature. In some cases, the first sensor and third sensor are combined into a single sensor that measures both blood pressure and temperature.

**[0023]** While the terms "first sensor," "second sensor," and "third sensor" are used herein, each of these terms are not limited to single or separate sensors. Skilled artisans would understand that any number of sensors can be used for each the "first sensor," "second sensor," and/or the "third sensor." Likewise, the "first sensor," "second sensor," and/or the "third sensor" can be combined into a single sensor. Moreover, any of the sensors

described herein can be provided on any of the embodiments described in U.S. Patent Publication No. 2010/0234698 (Application No. 12/557,685).

**[0024]** The first sensor 240 is adapted to measure blood pressure and generate a signal representative of the blood pressure. In certain embodiments, the first sensor 240 is a fiber optic pressure sensor adapted to measure blood pressure. An example of a fiber optic pressure sensor is a Fabry-Perot fiber optic pressure sensor, which is a commercially available sensor. Examples of Fabry-Perot fiber optic sensors are the "OPP-M" MEMS-based fiber optic pressure sensor (400 micron size) manufactured by Opsens (Quebec, Canada), and the "FOP-MIV" sensor (515 micron size) manufactured by Fiso Technologies, Inc. (Quebec, Canada). In other embodiments, first sensor 240 can be a piezo-resistive pressure sensor (e.g., a MEMS piezo-resistive pressure sensor). In yet other embodiments, first sensor 240 can be a capacitive pressure sensor (e.g., a MEMS capacitive pressure sensor). A pressure sensing range from about -50 mm Hg to about +300 mm Hg (relative to atmospheric pressure) is desired for making most physiological measurements with the first sensor 240, for example.

**[0025]** The second sensor 270 can include any sensor type that is capable of measuring a cross-sectional area of a surrounding anatomical structure. In some cases, the sensor 270 measure conductivity of fluid in an anatomical structure. The fluid conductivity measurements can then be used to calculate a cross-sectional area measurement. In Figures 1-3, the second sensor 270 is an electrode arrangement that includes source electrodes 272, 274 and sense electrodes 276, 278. The source electrodes 272, 274 deliver a current and the sense electrodes 276, 278 measure voltage resulting from the current. The voltage measurement from the sense electrodes 276, 278 can be used to calculate the fluid conductivity and thus the cross-sectional area of the surrounding anatomical structure. Examples of suitable algorithms and methods for calculating a cross-sectional area measurement using voltage and/or fluid conductivity measurements can be found in U.S. Patent No. 7,454,244 (Application No. 10/782,149).

**[0026]** The sensor delivery device 10 also includes a proximal portion 250, which is coupled to the distal sleeve 220. The proximal portion 250 includes a communication channel 260 and the sensors are communicably connected to the communication channel 260. The communication channel communicates signals from the sensors to a location outside of the patient (e.g., to a processor, display, computer, monitor, or to another medical device). The communication channel 260 can be any suitable channel that transmits signals generated by the sensors to a location outside of the patient. Exemplary communication channels include fiber optic, electrically conductive, wireless, infrared, acoustic, and/or ultrasound mediums. The communication channel 260 can be disposed along an outer surface of proximal portion 250, or can be formed within the proximal portion 250, as shown

in Figures 1-3. For example, the communication channel 260 can be a communication lumen that extends longitudinally through proximal portion 250 in some embodiments.

**[0027]** The first sensor 240, the second sensor 270 and the third sensor are each coupled to a distal sleeve 220. The sensors can be provided at any suitable location along the distal sleeve 220. In some cases, the sensors can be provided on an outer surface of the distal sleeve 220.

**[0028]** Figures 1-3 each show an electrode arrangement 270 that is coupled to the distal sleeve 220 at different locations. In Figure 1, each of the electrodes 272, 274, 276, 278 are coupled to the distal sleeve 220 at a position that is proximal to the first sensor 240. In Figure 2, the source electrodes 272, 274 are coupled to both the distal sleeve 220 and the proximal portion 250 whereas the sense electrodes 276, 278 coupled only to the distal sleeve. Specifically, the sense electrodes are coupled to the distal sleeve 220 at a position that is distal to the proximal portion 250 and proximal to the first sensor 240. In Figure 3, each of the electrodes 272, 274, 276, 278 are coupled to the distal sleeve 220 at a position that is distal to the first sensor 240.

**[0029]** In Figures 1-3, the electrodes 272, 274, 276, 278 each have a ring shape so that they surround a circumference or periphery of the distal sleeve (and proximal portion in some embodiments). Of course, the electrodes 272, 274, 276, 278 can instead be point electrodes or have other suitable configurations. The electrodes 272, 274, 276, 278 can also be made of any suitable conductive material such as platinum iridium or a carbon-coated surface. Additionally, the electrodes 272, 274, 276, 278 can be provided in communication with the communication channel 260 using any desired method. For example, in FIG. 1, one or more wires 275 connect the electrodes 272, 274, 276, 278 to the communication channel 60.

**[0030]** The sensor delivery device further includes a movable sheath, wherein the movable sheath is adapted to cover and uncover the sensor 270 or the electrode arrangement 270. Such a movable sheath is valuable in cases where it is desired to trap the patient's blood between the sheath and the electrodes, as will be further discussed below.

**[0031]** The proximal portion 250 is also adapted to assist an operator in positioning the distal sleeve 220 and the sensors within the anatomical structure of the patient. This is typically accomplished by an operator first inserting a "standard" medical guidewire 230 into a patient's vasculature and advancing it to an anatomical structure of interest. The sensor delivery device 210 is then deployed by "threading" the distal sleeve 220 onto the guidewire 230 such that the lumen 222 slides over the guidewire 230, and advancing the distal sleeve 220 (and the associated sensors) by moving (e.g., pushing and/or pulling) the proximal portion 250 until sensors are in the desired location. Thus, the distal sleeve 220, and hence,

the sensors, can be positioned within an anatomical structure of a patient by causing the distal sleeve 220 to slide over the medical guidewire 230 to the desired position.

**[0032]** The proximal portion 250 can also be formed of a material of sufficient stiffness in order to assist an operator in positioning the distal sleeve 220 and the sensors within an anatomical structure of the patient. Suitable materials for the proximal portion 250 can be materials such as stainless steel, nitinol, nylon, and plastic, for example, or composites of multiple materials. Depending on the application, the proximal portion 250 can be made stiffer and more rigid than the distal sleeve 220 in order to provide a reasonable amount of control to push, pull and otherwise maneuver the device to the location of interest within the patient.

**[0033]** The device 210 and the guidewire 230 are typically manipulated inside a guiding catheter (not shown), which has been placed in the anatomical structure of interest. In certain embodiments of the invention, the guidewire lumen 222 may be sized to slide over "standard" sized medical guidewires. For example, a number of manufacturers make medical guidewires that range in size from less than about 0.014 inches outer diameter to more than about 0.038 inches outer diameter, typically having a finite number of common sizes within this range. "Standard" size medical guidewires might, for example, have outer diameters of 0.0254, 0.03556, 0.04572, 0.05334, 0.0635, 0.07112, 0.08128, 0.0889, and 0.09652 cm (0.10, 0.014, 0.018, 0.021, 0.025, 0.028, 0.032, 0.035, and 0.038 inches). Thus, in certain preferred embodiments of the invention, the guidewire lumen 222 may be sized appropriately to slide over a particular standard size medical guidewire. A device according to preferred embodiments of the invention may therefore be made available in a range of sizes corresponding to standard medical guidewire sizes.

**[0034]** In certain embodiments of the invention, the distal sleeve 220 of the device can be substantially concentric with the guidewire 230. The coupling of the proximal portion 250 to the distal sleeve 220 allows the guidewire 320 to separate from the rest of device 210 (e.g., in what is sometimes referred to as a "monorail" catheter configuration); this would typically occur inside a guiding catheter. The guidewire 230 and device 210 would both exit the patient at the proximal end of a guiding catheter as separate devices. Having the device 210 and guidewire 230 separate allows the physician to independently control device 210 and guidewire 230, as necessary. It may also allow a physician to use a shorter guidewire for catheter exchange. For example, a monorail-type configuration may allow for the use of a guidewire that is approximately 170 to 200 cm long, whereas an "over-the-wire" configuration might require the use of a much longer (e.g., up to 300 cm or more) guidewire. Having the device 210 and guidewire 230 separate (except at the distal sleeve 220) may also result in less friction than if the device 210 and guidewire 230 had to be moved together as a unit.

In some embodiments, a hydrophilic coating may be applied to various portions of the device to further reduce the amount of friction encountered, for example, when advancing or retracting device 210.

**[0035]** The distal sleeve 220 can be substantially tubular, as shown, or can have any shape that allows distal sleeve 220 to slide over a medical guidewire 230 in an anatomical structure of interest. The distal sleeve 220 can be formed of a flexible material in some embodiments to facilitate positioning and placement of the distal sleeve 220 (and sensors) over a guidewire 230 through narrow vascular structures such as coronary arteries. In certain embodiments, the distal sleeve 220 comprises a flexible polyimide tube or flexible microcoil tube sized for placement in vascular structures, such as in coronary arteries or peripheral arteries. In some embodiments, flexibility may be achieved and/or enhanced by applying a series of cuts along the surface of the distal sleeve 220. The length of distal sleeve 220 can also vary. In embodiments to be used deep within coronary arteries, for example, distal sleeve 220 can be up to about 15 inches long. The distal sleeve 220 can also include a thin covering to provide additional structural support and/or improve handling characteristics of the device. Such a covering can comprise, for example, polyester (PET) shrink tubing that substantially covers the distal sleeve.

**[0036]** One advantage of the sensor delivery device 210 is that it does not require repositioning of the guidewire in order to make multiple sensor readings. Once the guidewire has been positioned across a stenotic lesion, for example, the sensor delivery device 210 can be positioned (e.g., advanced and/or retracted) over the guidewire and the sensors can therefore be advanced and retracted across lesions to make pressure, temperature and cross-sectional area readings, for example, without moving the guidewire. A physician may also save time by not having to reposition the guidewire across the lesion or lesions to make such measurements.

**[0037]** The sensor delivery device 210 can also interact with other devices and/or display equipment. In some embodiments, as shown in FIG. 4, the sensor delivery device 210 interacts with a processor 296. The sensor delivery device 210 and processor 296 can interact using any known connection mechanism in the art. In certain cases, a furcation tube 290 and a connector 294 can be used to send signals from the sensors 240, 270 to the processor 296. The processor 296 can be, for example, a standalone display monitor to show signal waveforms and/or numerical values of the signals from sensors 240, 270. The processor 296 could include data recording capabilities in some embodiments.

**[0038]** The processor 296 is adapted to receive signals from each of the sensors and to use those signals to make calculations. Typically, the processor 296 uses one or more algorithms to make calculations. For example, in cases where the sensor 270 is an electrode arrangement, the electrode arrangement obtains a voltage measurement representative of the conductivity of the sur-

rounding fluid and then sends that measurement to the processor 296. The processor 296 then uses the measured voltage to calculate fluid conductivity and thus cross-sectional area of the anatomical structure.

**[0039]** In other embodiments, the sensor delivery device 210 also interacts with a medical fluid injection device, such as a powered fluid injector used to inject contrast media and/or saline during certain medical procedures (e.g., angiography, computed tomography, MRI, ultrasound, etc.). Exemplary powered injection systems that can be used with the sensor delivery device 210 are described in U.S. Patent Publication No. 2010/0234698 (Application No. 12/557,685). In some embodiments, the injection device is adapted to inject a first fluid and a second fluid into the anatomical structure. Typically, the first fluid has a first known conductivity and the second fluid has a second known conductivity, wherein the known conductivity of the first fluid is different than the known conductivity of the second fluid. In certain embodiments, the first fluid can be a NaCl solution having a first concentration and the second fluid can be a NaCl solution having a second concentration, wherein the first concentration is higher than the second concentration. As an example, the first fluid can be a NaCl solution having a 9% concentration and the second fluid can be a NaCl solution having a 4.5% concentration.

**[0040]** Figures 5-10 are flow diagrams that illustrate certain methods of using the sensor delivery device. Each of these methods do not form part of the invention and will now be described. Figure 5 is a flow diagram that illustrates a method 300 of using the sensor delivery device to measure a cross-sectional area of an anatomical structure. Step 305 comprises a guidewire into the patient and into an anatomical structure of interest. Step 310 comprises deploying a sensor delivery device 210 including one or more sensors over the guidewire and positions the device (and thus the sensors) in the anatomical structure. Step 315 comprises using one of the sensors to measure and calculate cross-sectional area of the anatomical structure. Finally, step 320 comprises using the cross-sectional area calculation to select a stent size for the anatomical structure. In certain cases, the stent size is selected by correlating a specific cross-sectional area measurement to a specific stent size.

**[0041]** Figure 6 is a flow diagram of a method 400 of using the sensor delivery device to measure and adjust a FFR value of an anatomical structure. Step 405 comprises placing a guidewire into the patient and into an anatomical structure of interest. Step 410 comprises deploying a sensor delivery device 210 including one or more sensors over the guidewire and positions the device (and thus the sensors) in the anatomical structure. Step 415 comprises using one of the sensors to measure and calculate an initial FFR value. Exemplary methods and algorithms for calculating an FFR value are described in U.S. Patent Publication No. 2010/0234698 (Application No. 12/557,685). Step 410 comprises using one of the sensors to measure and calculate cross-sectional area.

Step 425 comprises using the initial FFR value and cross-sectional area to calculate a corrected FFR value.

**[0042]** Figure 7 is a flow diagram of a method 500 of using the sensor delivery device to measure blood conductivity and fluid conductivity to calculate a cross-sectional area of an anatomical structure. Step 505 comprises placing a guidewire into the patient and into an anatomical structure of interest. Step 510 comprises deploying a sensor delivery device 210 including one or more sensors over the guidewire and positions the device (and thus the sensors) in the anatomical structure. Step 515 comprises using one of the sensors to measure a conductivity of the patient's blood. Step 520 comprises administering a fluid with a known conductivity to the anatomical structure. Step 525 comprises using one of the sensors to measure a conductivity of the fluid. Finally, step 530 comprises using the measured blood conductivity and fluid conductivity to calculate a cross-sectional area of the anatomical structure. Exemplary methods of using measured conductivities to calculate a cross-sectional area of an anatomical structure can be found in U.S. Patent No. 7,454,244 (Application No. 10/782,149).

**[0043]** Figure 8 is a flow diagram of a method 600 of using the sensor delivery device to measure conductivity of a first fluid and a second fluid to calculate a cross-sectional area of an anatomical structure. Step 605 comprises placing a guidewire into the patient and into an anatomical structure of interest. Step 610 comprises deploying a sensor delivery device 210 including one or more sensors over the guidewire and positioning the device (and thus the sensors) in the anatomical structure. Step 615 comprises administering a first fluid with a known conductivity to the anatomical structure. Step 620 comprises using one of the sensors to measure a first conductivity for the first fluid. Step 625 comprises administering a second fluid with a known conductivity to the anatomical structure. Step 630 comprises using the sensor to measure a second conductivity for the second fluid. Finally, step 635 comprises using the measured first conductivity and second conductivity to calculate cross-sectional area of the anatomical structure.

**[0044]** Figure 9 is a flow diagram of a method 700 of using the sensor delivery device to measure blood conductivity and fluid conductivity to calculate a cross-sectional area of an anatomical structure. Step 705 comprises placing a guidewire into the patient and into an anatomical structure of interest. Step 710 comprises deploying a sensor delivery device 210 including one or more sensors over the guidewire and positioning the device (and thus the sensors) in the anatomical structure. Step 715 comprises using one of the sensors to measure conductivity for a patient's blood. Step 720 comprises using a temperature sensor to measure fluid temperature in the anatomical structure. Step 725 comprises administering a fluid with a known conductivity to the anatomical structure. Step 730 comprises using one of the sensors to measure conductivity of the fluid when the fluid temperature reaches a desired temperature value. Step 735

comprises using the measured blood conductivity and fluid conductivity to calculate cross-sectional area of the anatomical structure.

**[0045]** Figure 10 is a flow diagram of a method 800 of using the sensor delivery device to measure conductivity of a first fluid and a second fluid to calculate a cross-sectional area of an anatomical structure. Step 805 comprises placing a guidewire into the patient and into an anatomical structure of interest. Step 810 comprises deploying a sensor delivery device 210 including one or more sensors over the guidewire and positioning the device (and thus the sensors) in the anatomical structure. Step 815 comprises using a temperature sensor to measure fluid temperature in the anatomical structure. Step 820 comprises administering a first fluid with a known conductivity to the anatomical structure. Step 825 comprises using one of the sensors to measure a first conductivity for the first fluid when the fluid temperature reaches a desired temperature value. Step 830 comprises administering a second fluid with a known conductivity to the anatomical structure. Step 835 comprises using one of the sensors to measure a second conductivity for the second fluid when the fluid temperature reaches a desired temperature value. Finally, step 840 comprises using the measured first conductivity and second conductivity to calculate cross-sectional area of the anatomical structure.

**[0046]** Certain specific embodiments of the methods illustrated in Figures 5-10 will now be described. In certain embodiments, a method is provided that enables a physician to first determine an FFR value of an anatomical structure and then to calculate cross-sectional area of the anatomical structure in order to select an appropriate stent size. Such a method includes providing a sensor delivery device, wherein the sensor delivery device includes a first sensor that is adapted to measure blood pressure and a second sensor that is adapted to measure cross-sectional area of the anatomical structure, positioning the sensor delivery device within the anatomical structure, using the first sensor to obtain one or more blood pressure measurements, using the blood pressure measurements to calculate an FFR value, electing to use a stent when the FFR value is lower than a threshold value, using the second sensor to obtain one or more cross-sectional area measurements, and using the cross-sectional area measurements to select a stent size. The FFR threshold value can be about 0.8, for example. In many cases, the step of using the cross-sectional area measurements to select a stent size comprises correlating a specific cross-sectional area measurement to a specific stent size.

**[0047]** In other embodiments, a method is provided that includes enables a physician to obtain an initial FFR value of an anatomical structure and then to calculate fluid conductivity measurements of fluid of the anatomical structure in order to correct or adjust the initial FFR value. Such a method includes providing a sensor delivery device, wherein the sensor delivery device includes a first

sensor is adapted to measure blood pressure and a second sensor adapted to measure conductivity of fluid in the anatomical structure, positioning the sensor delivery device within the anatomical structure, using the first sensor to obtain one or more blood pressure measurements, using the blood pressure measurements to calculate an initial FFR value, using the second sensor to obtain one or more cross-sectional area measurements, using the cross-sectional area measurements to calculate a corrected FFR value. The corrected FFR value closer to what the FFR value would have been if the sensor delivery device was not present (or if just a guidewire was present) in the anatomical structure. In certain cases, the corrected FFR value is calculated using an algorithm that combines the initial FFR value with the cross-sectional area measurements. The algorithm could also account for cross-sectional area measurements taken proximal and/or distal to the stenotic lesion and the volumetric flow rate or blood velocity. The method can further include electing to use a stent when the corrected FFR value is beneath a threshold value, for example a value of about 0.8. In this case, the method can even further include using the cross-sectional area to select a stent size.

**[0048]** In certain embodiments, the second sensor is used to measure fluid conductivity, which can then be used to calculate a cross-sectional area of the anatomical structure. Typically, the second sensor measures fluid conductivities for two different fluids and uses those conductivity measurements to calculate cross-sectional area. In some cases, two fluids other than the patient's blood are used. In such cases, the method includes administering a first fluid with a known conductivity to the anatomical structure, using the second sensor to measure a first conductivity for the first fluid, administering a second fluid with a known conductivity to the anatomical structure, wherein the conductivity of the first fluid is different than the conductivity of the second fluid, using the second sensor to measure a second conductivity for the second fluid, and using the first conductivity and the second conductivity to calculate a cross-sectional area of the anatomical structure. In certain embodiments, the first fluid is a NaCl solution having a first concentration, for example a 9% concentration, and the second solution is a NaCl solution having a second concentration, for example a 4.5% concentration, wherein the first concentration is higher than the second concentration.

**[0049]** In other cases, the patient's blood is used as one of the fluids if its conductivity is known. In such cases, the method includes using the second sensor to measure conductivity for the patient's blood, administering fluid with a known conductivity to the anatomical structure, using the second sensor to measure conductivity for the fluid, and using the measured blood conductivity and the measured fluid conductivity to calculate a cross-sectional area of the anatomical structure. Using the patient's blood as one of the fluids is advantageous because it eliminates having to perform two fluid administrations, which provides time savings and convenience. In certain

cases, the sensor delivery device can include a movable sheath that is movable by a user to cover and uncover the second sensor. For example, when the second sensor is an electrode arrangement, the sheath covers and uncovers the electrodes. When moved to cover the electrodes, the sheath traps a small amount of the patient's blood between the electrodes and the conductivity of the blood can be directly measured. This allows for the amount of current used by the electrodes for such a blood conductivity measurement to be less than the amount of current needed to measure a fluid in the surrounding anatomical structure.

**[0050]** In each of these methods, the second sensor can be an electrode arrangement that is adapted to measure fluid conductivity. In such cases, the method includes using the electrodes to obtain fluid conductivity measurements and calculating cross-sectional area measurements using the fluid conductivity measurements. In certain preferred cases, the electrode arrangement includes source electrodes and sense electrodes, wherein the source electrodes generate a current, for example a constant current, and the sense electrodes measure voltage resulting from the current. As such, in some cases, the method comprises obtaining voltage measurements and calculating fluid conductivity (and thus calculating cross-sectional area measurements) using the voltage measurements.

**[0051]** In embodiments where the second sensor is an electrode arrangement, the electrodes can also measure blood flow velocity. For example, the electrode arrangement can be configured to measure resistance between the source electrodes (for example between a first and a second source electrode) and the resistance between sense electrodes (for example between a first and a second sense electrode). When a fluid having conductivity different than the patient's blood travels past the electrodes, the time difference in when the measured change in resistance occurs on each set of electrodes can be used to measure the blood flow velocity at the anatomical structure. In other words, the blood flow velocity can be calculated by dividing the time difference by the distance between these sets of electrodes. The blood flow velocity measurement and the cross-sectional area measurement can also both be used to calculate a volumetric blood flow.

**[0052]** In certain cases, the above methods can also include providing a third sensor, wherein the third sensor is a temperature sensor that measures temperature of fluid in the anatomical structure. The third sensor and the first sensor can be a single sensor in some embodiments, wherein the single sensor is adapted to measure both blood pressure and fluid temperature. Such a temperature sensor is useful because it provides the ability to create a timing signal that the physician and/or processor could use to determine when the fluid (which has a lower temperature than blood) is present in the anatomical structure. For example, in cases where the second sensor measures conductivity of patient's blood and an out-

side fluid, the method comprises using the second sensor to measure a conductivity for the patient's blood, administering fluid with a known conductivity to the anatomical structure, using the third sensor to measure fluid temperature, using the second sensor to measure a conductivity for the fluid after the fluid temperature reaches a desired temperature value, and using the measured blood conductivity and the measured fluid conductivity to calculate a cross-sectional area of the anatomical structure.

**[0053]** Likewise, in cases where the second sensor measures conductivities of two fluids other than a patient's blood, the method comprises administering a first fluid with a known conductivity to the anatomical structure, using the third sensor to measure fluid temperature, using the second sensor to measure a conductivity for the first fluid after the fluid temperature reaches a desired temperature value, administering a second fluid with a known conductivity to the anatomical structure, wherein the conductivity of the first fluid is different than the conductivity of the second fluid, using the second sensor to measure a conductivity for the second fluid after the fluid temperature reaches a desired temperature value, and using the first conductivity and the second conductivity to calculate a cross-sectional area of the anatomical structure.

**[0054]** Further, in cases where a third sensor or temperature sensor is used, both the fluid conductivities and the temperature can be measured and recorded in real time. Such a real time or continuous recording arrangement provides several advantages. First, when a fluid is injected, a user and/or processor can select a fluid conductivity measurement that corresponds to the lowest temperature measurement (or select the lowest fluid conductivity measurement obtained). This ensures that the measurement selected is actually the measurement of the injected fluid. Also, a real time measuring system allows for a user to continuously monitor the fluid conductivity while the sensor delivery device is moved through the body. Once the sensor delivery device is placed near or within the anatomical structure of interest, the user can manipulate the device until the lowest fluid conductivity measurement is located. At this point, the user then fixes the device at that location in order to perform the above-described methods. This allows for a user to fix the device at a location that likely has a minimum lumen diameter and is thus a location that is most affected by the stenosis.

#### Example

**[0055]** The following steps illustrate one exemplary method.

- 1) A clinician identifies a stenotic lesion via angiogram.
- 2) The clinician determines that the lesion is "intermediate," that is, it is not clear whether or not intervention (e.g., stenting) would be beneficial or harmful

to the patient.

3) The clinician inserts the sensor delivery device including sensors into place and equalizes to aortic pressure.

4) The clinician administers adenosine.

5) The clinician calculates a FFR value using a sensor on the sensor delivery device.

6) If the FFR value is below a certain threshold value, the clinician decides to insert a stent.

7) With the sensory delivery device still in place, the clinician measures cross-sectional area (CSA) as follows:

a. A first conductance value (C1) is measured (with blood in lumen).

b. 0.9% saline is administered (injected) while measuring and/or monitoring conductance. The minimum reading is recorded as C2.

c. 0.45% saline is administered (injected) while measuring and/or monitoring conductance. The minimum reading is recorded as C3.

d. C3 and C2 are utilized along with known fluid conductivities to calculate CSA.

e. Alternatively, C1 is used along with a separate measurement of blood conductivity (e.g., C2), to calculate CSA, and the C3 measurement could be dropped.

8) The clinician uses the CSA measurement to select a stent size.

9) The clinician inserts the appropriately sized stent into the stenotic lesion.

10) The sensor delivery device can also include a special marker band with a pattern recognizable to a computer algorithm. Based on locating the marker band, a computer could automatically place visual information (such as the FFR reading and/or the vessel sizing information) on the angiogram itself.

## Claims

1. An intravascular sensor delivery device (210) comprising:

a distal sleeve (220) having a guidewire lumen (222) for slidably receiving a medical guidewire (230),

a first sensor (240) coupled to the distal sleeve (220), wherein the first sensor (240) is adapted to measure blood pressure and generate a signal representative of the blood pressure;

a second sensor (270) coupled to the distal sleeve (220), wherein the second sensor (270) is adapted to measure cross-sectional area of a surrounding anatomical structure and generate signal representative of the cross-sectional area, wherein the second sensor (270) comprises

an electrode arrangement (270),

a proximal portion (250) coupled to the distal sleeve (220), the proximal portions (250) comprising a communication channel (260), wherein the communication channel (260) is adapted to communicate the signal from the first sensor (240) and the signal from the second sensor (270) to a location outside of a patient; **characterised in** a movable sheath, wherein the movable sheath is adapted to cover and uncover the electrode arrangement (270).

2. The device of claim 1 wherein the electrode arrangement includes source electrodes (272,274) and sense electrodes (276,278) wherein the source electrodes (272,274) are adapted to generate a current and the sense electrodes (276,278) are adapted to measure voltage resulting from the current.

3. The device of claim 2 wherein the signal representative of the cross-sectional area is the voltage measured by the sense electrodes (272,274).

4. The device of claim 2 wherein the electrode arrangement includes two source electrodes (272,274) and two sense electrodes (276,278).

5. The device of claim 2 wherein the source electrodes (272,274) and the sense electrodes (276,278) are ring-shaped electrodes that surround a periphery of the distal sleeve (220).

6. The device of claim 1 wherein the second sensor (270) is attached to an outer surface of the distal sleeve (220).

7. The device of claim 1 wherein the second sensor (270) is coupled to the distal sleeve (220) at a location that is distal to the first sensor (240).

8. The device of claim 1 wherein the second sensor (270) is coupled to the distal sleeve (220) at a location that is proximal to the first sensor (240).

9. The device of claim 1 wherein the second sensor (270) is coupled to both the distal sleeve (220) and the proximal portion (250) at a location that is proximal to the first sensor (240).

10. The device of claim 1 further comprising a third sensor, wherein the third sensor is adapted to measure temperature and generate a signal representative of the temperature and wherein the communication channel (260) is adapted to communicate the signal from the first sensor, the signal from the second sensor, and the signal from the third sensor to a location outside of the patient.

11. The device of claim 10 wherein the first sensor (240) and the third sensor are a single sensor, wherein the single sensor is adapted to both measure blood pressure and measure temperature.
12. The device of claim 1 wherein the signal representative of the cross-sectional area is a signal that can be used to calculate the cross-sectional area using one or more algorithms.

### Patentansprüche

1. Intravaskuläre Sensorliefer-Einrichtung (210), welche umfasst:

eine distale Buchse (220) mit einem Lumen (222) für einen Führungsdraht, um einen medizinischen Führungsdraht (230) gleitend aufzunehmen,

einen ersten Sensor (240), der mit der distalen Buchse (220) gekoppelt ist, worin der erste Sensor (240) angepasst ist, Blutdruck zu messen und ein Signal zu erzeugen, das den Blutdruck anzeigt;

einen zweiten Sensor (270), die mit der distalen Buchse (220) gekoppelt ist, worin der zweite Sensor (270) angepasst ist, einen Querschnittsbereich der umgebenden anatomischen Struktur zu erfassen und ein Signal zu erzeugen, das den Querschnittsbereich anzeigt, worin der zweite Sensor (270) einen Elektroden-Aufbau (270) umfasst,

einen proximalen Bereich (250), der mit der distalen Buchse (220) gekoppelt ist, worin der proximale Bereich (250) einen Verbindungskanal (260) umfasst, worin der Verbindungskanal (260) angepasst ist, das Signal von dem ersten Sensor (240) zu einer Position außerhalb eines Patienten zu übermitteln,

**gekennzeichnet durch** eine bewegbare Lage, worin die bewegbare Lage angepasst ist, die Elektrodenanordnung (270) zu bedecken und freizulegen.

2. Einrichtung nach Anspruch 1, worin die Elektrodenanordnung Quellenelektroden (272, 274) und Erfassungselektroden (276, 278) umfasst, worin die Quellenelektroden (272, 274) einen Strom erzeugen und die Erfassungselektroden (276, 278) angepasst sind, eine von dem Stromfluss herrührende Spannung zu erfassen.
3. Einrichtung nach Anspruch 2, worin das für den Querschnittsbereich repräsentative Signal die durch die Erfassungselektroden (276, 278) gemessene Spannung ist.

4. Einrichtung nach Anspruch 2, worin die Elektrodenanordnung zwei Quellenelektroden (272, 274) und zwei Erfassungselektroden (276, 278) umfasst.

5. Einrichtung nach Anspruch 2, worin die Quellenelektroden (272, 274) und die Erfassungselektroden (276, 278) ringförmige Elektroden sind, die einen Umfang der distalen Buchse (220) umgeben.

6. Einrichtung nach Anspruch 1, worin der zweite Sensor (270) an eine äußere Oberfläche der distalen Buchse (220) gekoppelt ist.

7. Einrichtung nach Anspruch 1, worin der zweite Sensor (270) mit der distalen Buchse (220) an einer Stelle gekoppelt ist, die distal zum ersten Sensor (240) liegt.

8. Einrichtung nach Anspruch 1, worin der zweite Sensor (270) mit der distalen Buchse (220) an einer Stelle gekoppelt ist, die proximal zum ersten Sensor (240) liegt.

9. Einrichtung nach Anspruch 1, worin der zweite Sensor (270) mit der distalen Buchse (220) und dem proximalen Bereich (250) an einer Stelle gekoppelt ist, die proximal zum ersten Sensor (240) liegt.

10. Einrichtung nach Anspruch 1, welche weiter einen dritten Sensor umfasst, worin der dritte Sensor angepasst ist, Temperatur zu erfassen und ein Signal zu erzeugen, das die Temperatur anzeigt, und worin der Verbindungskanal (260) angepasst ist, das Signal von dem ersten Sensor, das Signal von dem zweiten Sensor und das Signal von dem dritten Sensor zu einer Stelle außerhalb des Patienten zu leiten.

11. Einrichtung nach Anspruch 1, worin der erste Sensor (240) und der dritte Sensor ein einzelner Sensor sind, worin der einzelne Sensor angepasst ist, den Blutdruck und die Temperatur zu messen.

12. Einrichtung nach Anspruch 1, worin das Signal, das den Querschnittsbereich anzeigt, ein Signal ist, das dazu verwendet werden kann, den Querschnittsbereich unter Verwendung ein oder mehrerer Algorithmen zu berechnen.

### Revendications

1. Dispositif de délivrance d'un capteur intravasculaire (210) qui comprend :

un manchon distal (220) qui possède une lumière de fil de guidage (222) destinée à recevoir de manière coulissante un fil de guidage médical (230) ;

- un premier capteur (240) relié au manchon distal (220), le premier capteur (240) étant adapté pour mesurer la pression sanguine et générer un signal représentatif de la pression sanguine ; un second capteur (270) relié au manchon distal (220), le second capteur (270) étant adapté pour mesurer la surface transversale d'une structure anatomique située autour et générer un signal représentatif de la surface transversale, le second capteur (270) comprenant un ensemble d'électrodes (270) ; une partie proximale (250) reliée au manchon distal (220), la partie proximale (250) comprenant un canal de communication (260), le canal de communication (260) étant adapté pour communiquer le signal qui provient du premier capteur (240) et le signal qui provient du second capteur (270) à un emplacement qui se trouve à l'extérieur d'un patient ; **caractérisé en ce que** qu'il comprend une gaine mobile, la gaine mobile étant adaptée pour recouvrir et découvrir l'ensemble d'électrodes (270).
2. Dispositif selon la revendication 1, dans lequel l'ensemble d'électrodes comprend des électrodes source (272, 274) et des électrodes de détection (276, 278), dans lequel les électrodes source (272, 274) sont adaptées pour générer un courant et les électrodes de détection (276, 278) sont adaptées pour mesurer la tension qui résulte du courant. 25
  3. Dispositif selon la revendication 2, dans lequel le signal représentatif de la surface transversale est la tension mesurée par les électrodes de détection (272, 274). 35
  4. Dispositif selon la revendication 2, dans lequel l'ensemble d'électrodes comprend deux électrodes source (272, 274) et deux électrodes de détection (276, 278). 40
  5. Dispositif selon la revendication 2, dans lequel les électrodes source (272, 274) et les électrodes de détection (276, 278) sont des électrodes en forme d'anneau qui entourent une périphérie du manchon distal (220). 45
  6. Dispositif selon la revendication 1, dans lequel le second capteur (270) est relié à une surface extérieure du manchon distal (220). 50
  7. Dispositif selon la revendication 1, dans lequel le second capteur (270) est relié au manchon distal (220) à un emplacement distal par rapport au premier capteur (240). 55
  8. Dispositif selon la revendication 1, dans lequel le se-
9. Dispositif selon la revendication 1, dans lequel le second capteur (270) est relié au manchon distal (220) à un emplacement proximal par rapport au premier capteur (240).
  10. Dispositif selon la revendication 1, qui comprend en outre un troisième capteur, dans lequel le troisième capteur est adapté pour mesurer la température et générer un signal représentatif de la température, et dans lequel le canal de communication (260) est adapté pour communiquer le signal qui provient du premier capteur, le signal qui provient du second capteur, et le signal qui provient du troisième capteur à un emplacement qui se trouve à l'extérieur du patient. 20
  11. Dispositif selon la revendication 10, dans lequel le premier capteur (240) et le troisième capteur sont un seul capteur, qui est adapté pour mesurer la pression sanguine et la température. 25
  12. Dispositif selon la revendication 1, dans lequel le signal représentatif de la surface transversale est un signal qui peut être utilisé pour calculer la surface transversale à l'aide d'un ou plusieurs algorithme(s).

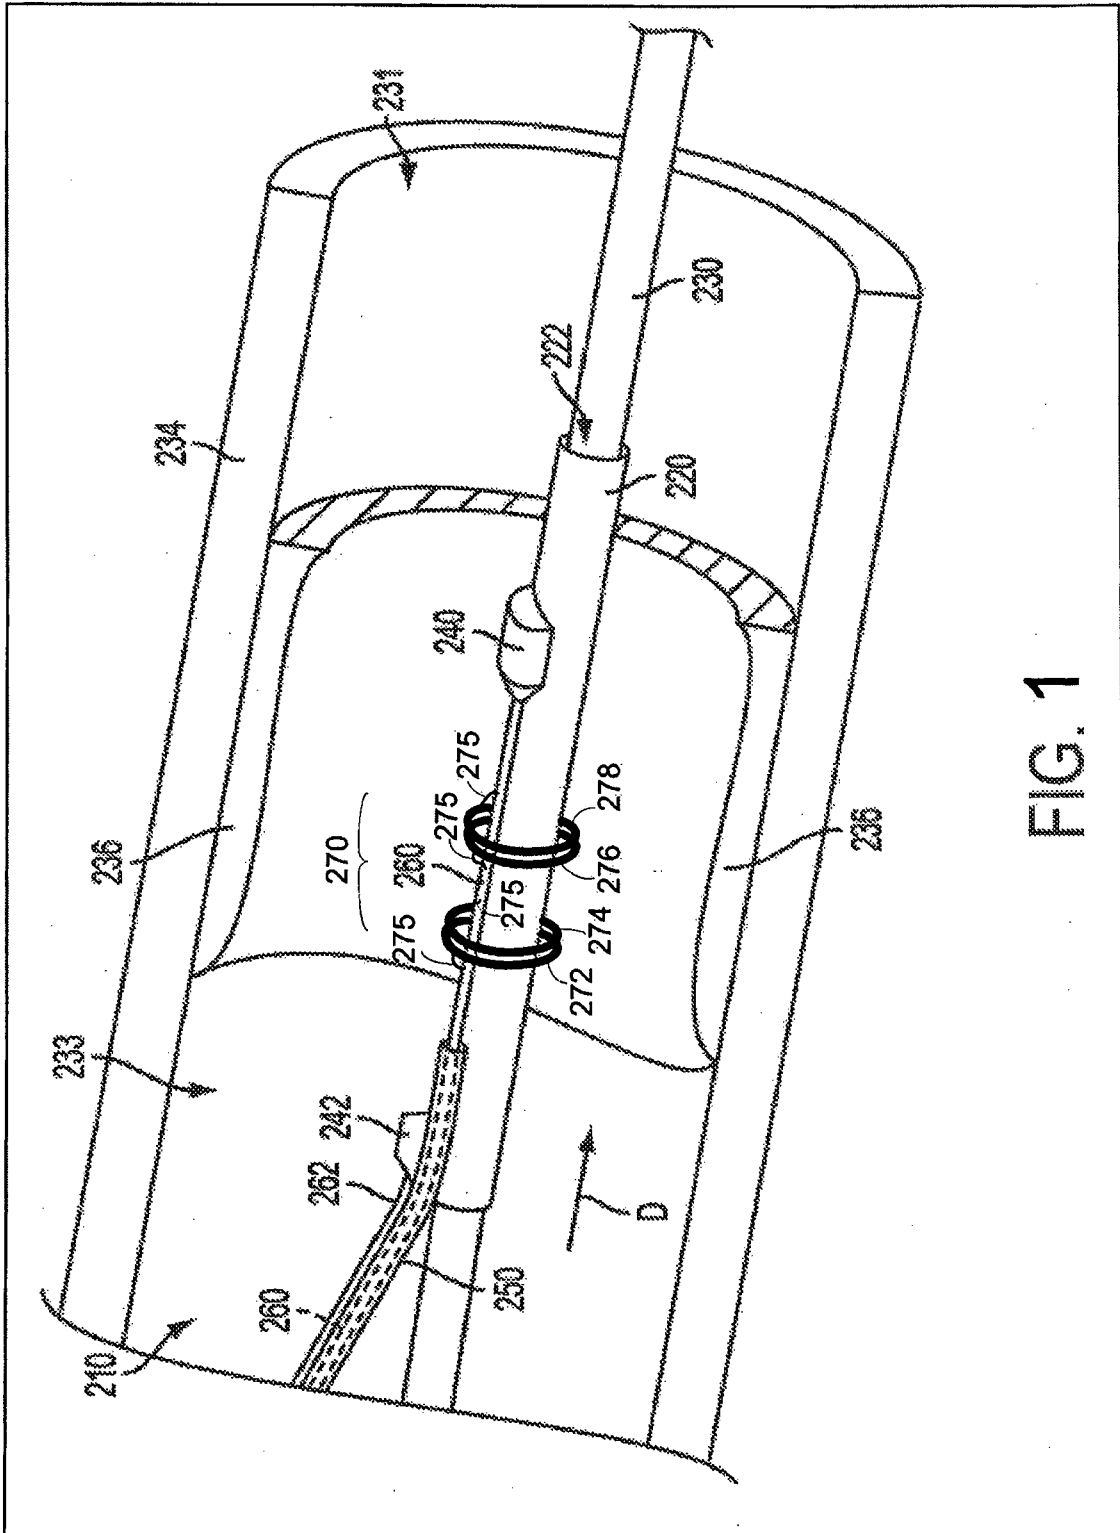


FIG. 1

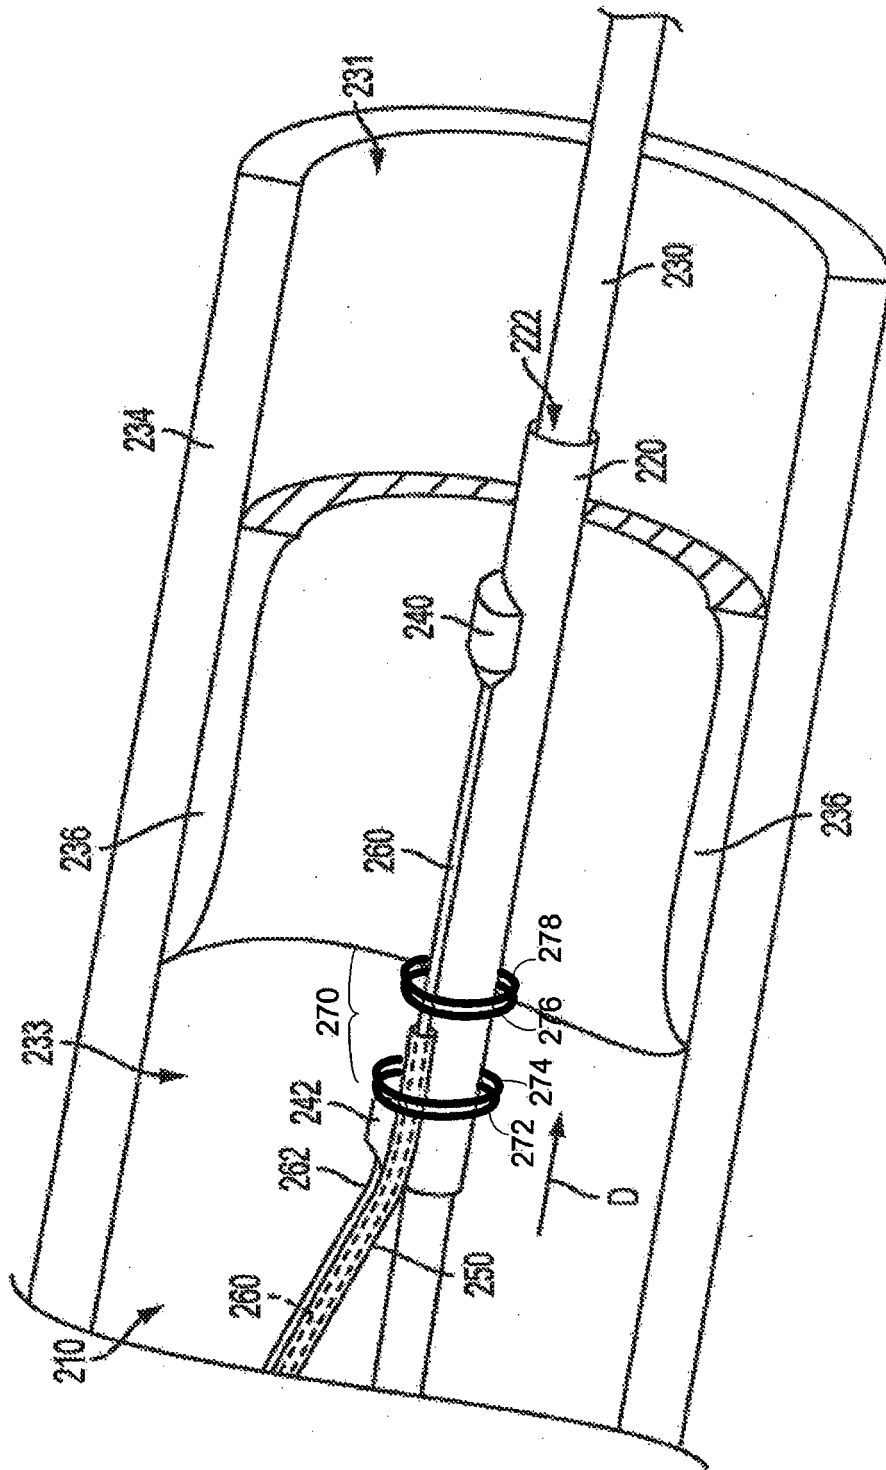


FIG. 2

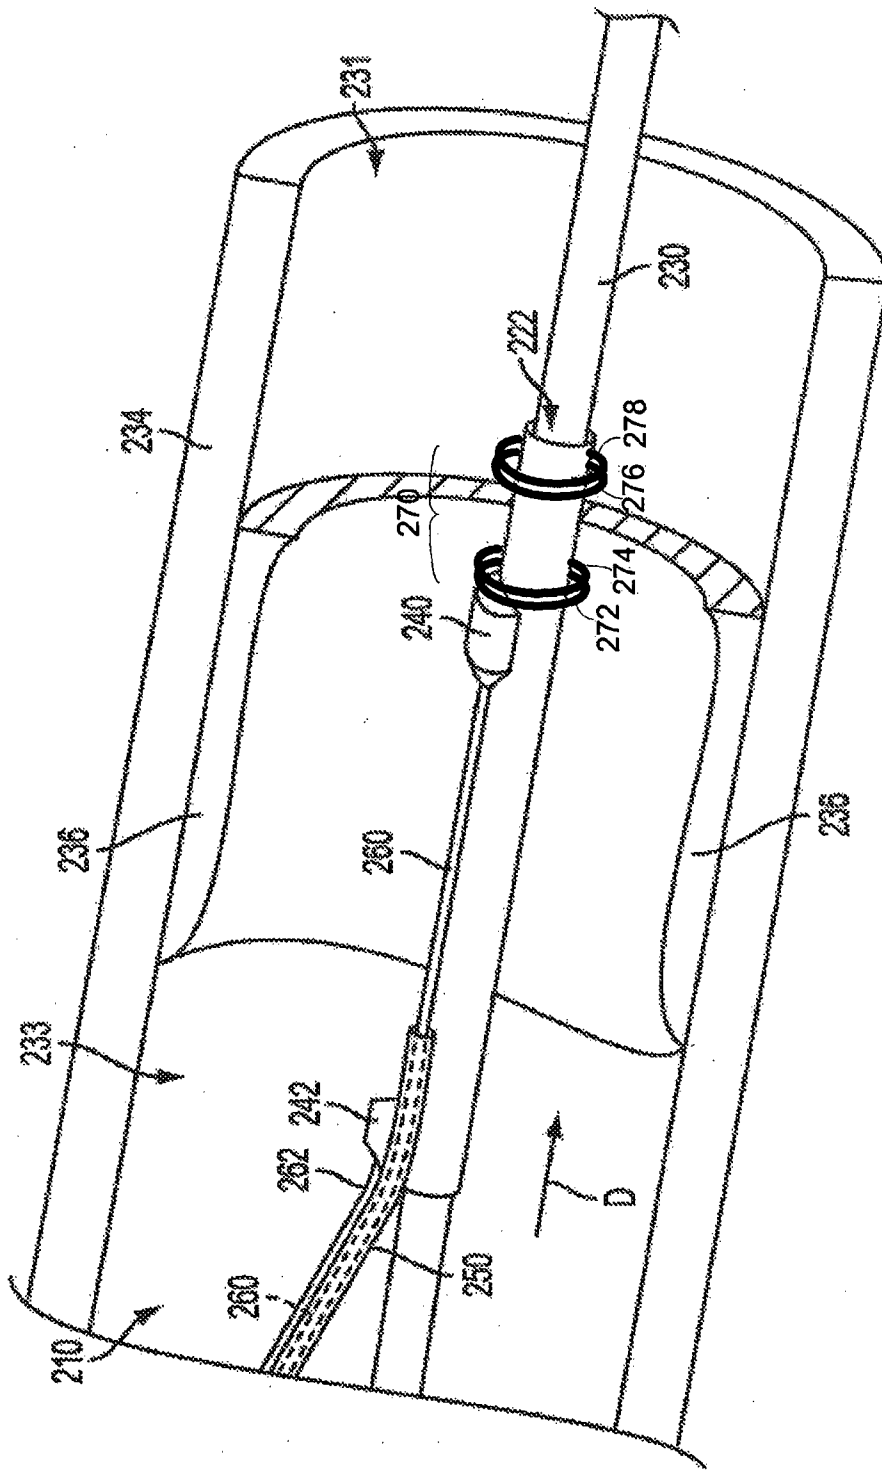


FIG. 3

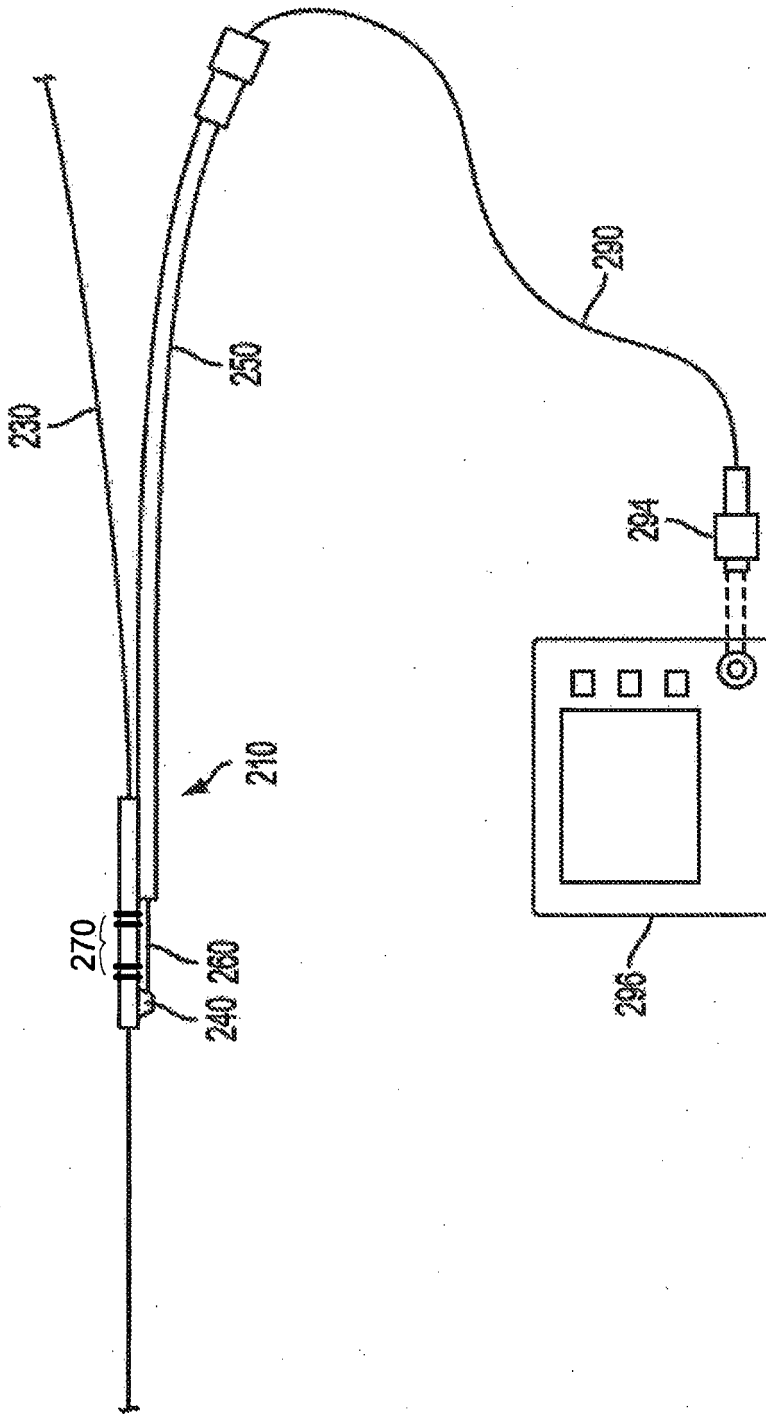


FIG. 4

FIG. 5

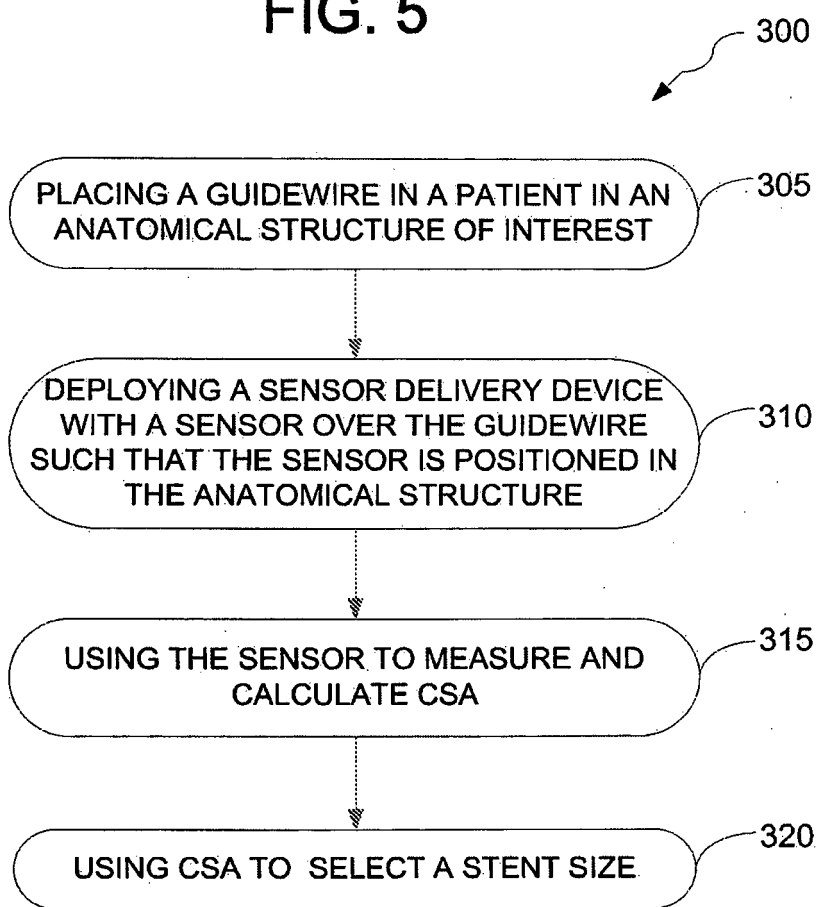


FIG. 6

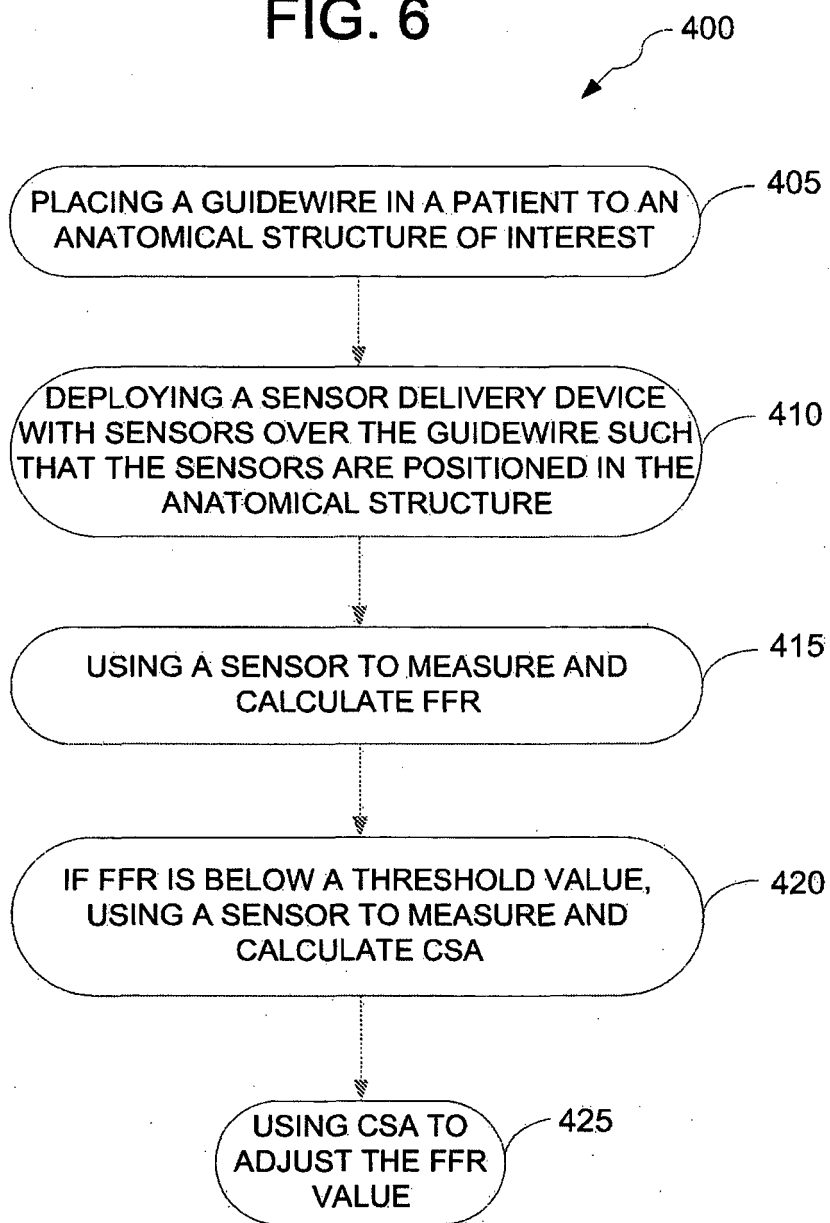


FIG. 7

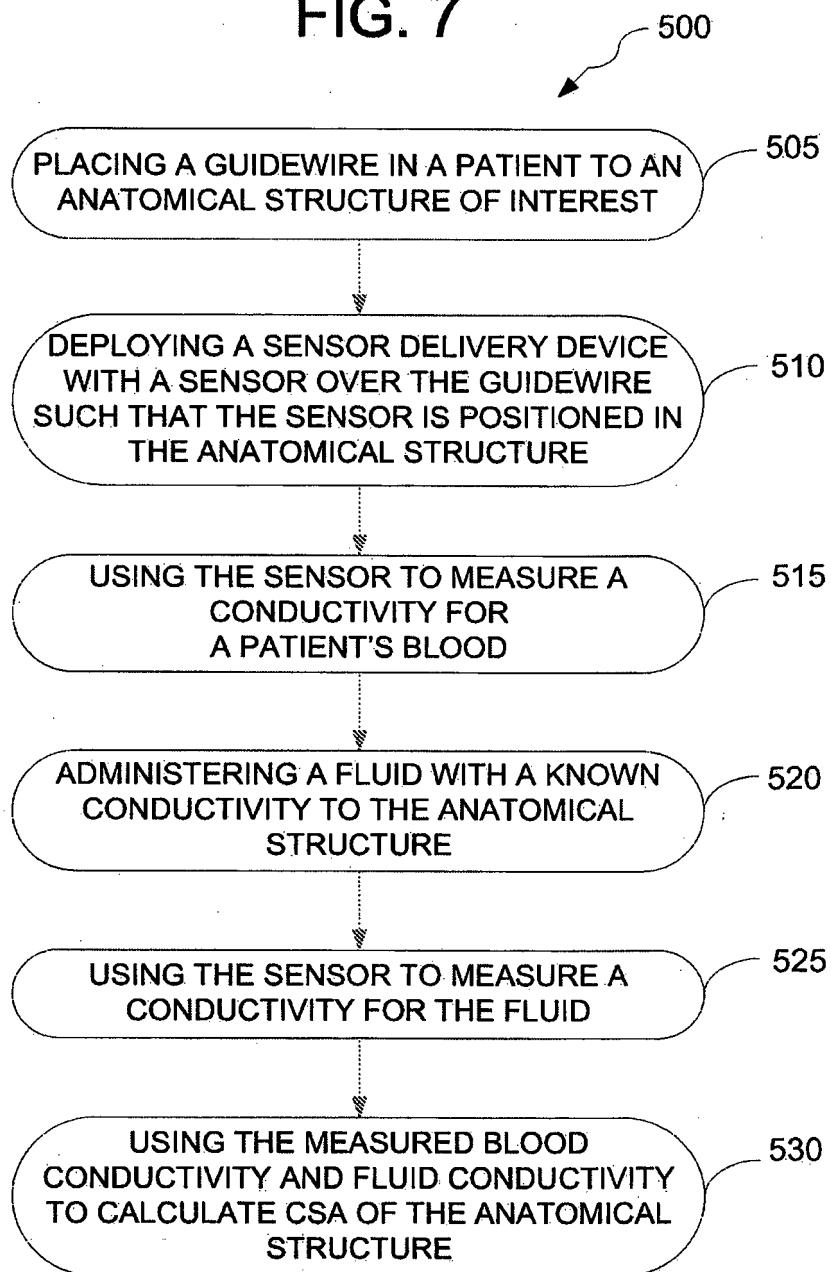


FIG. 8

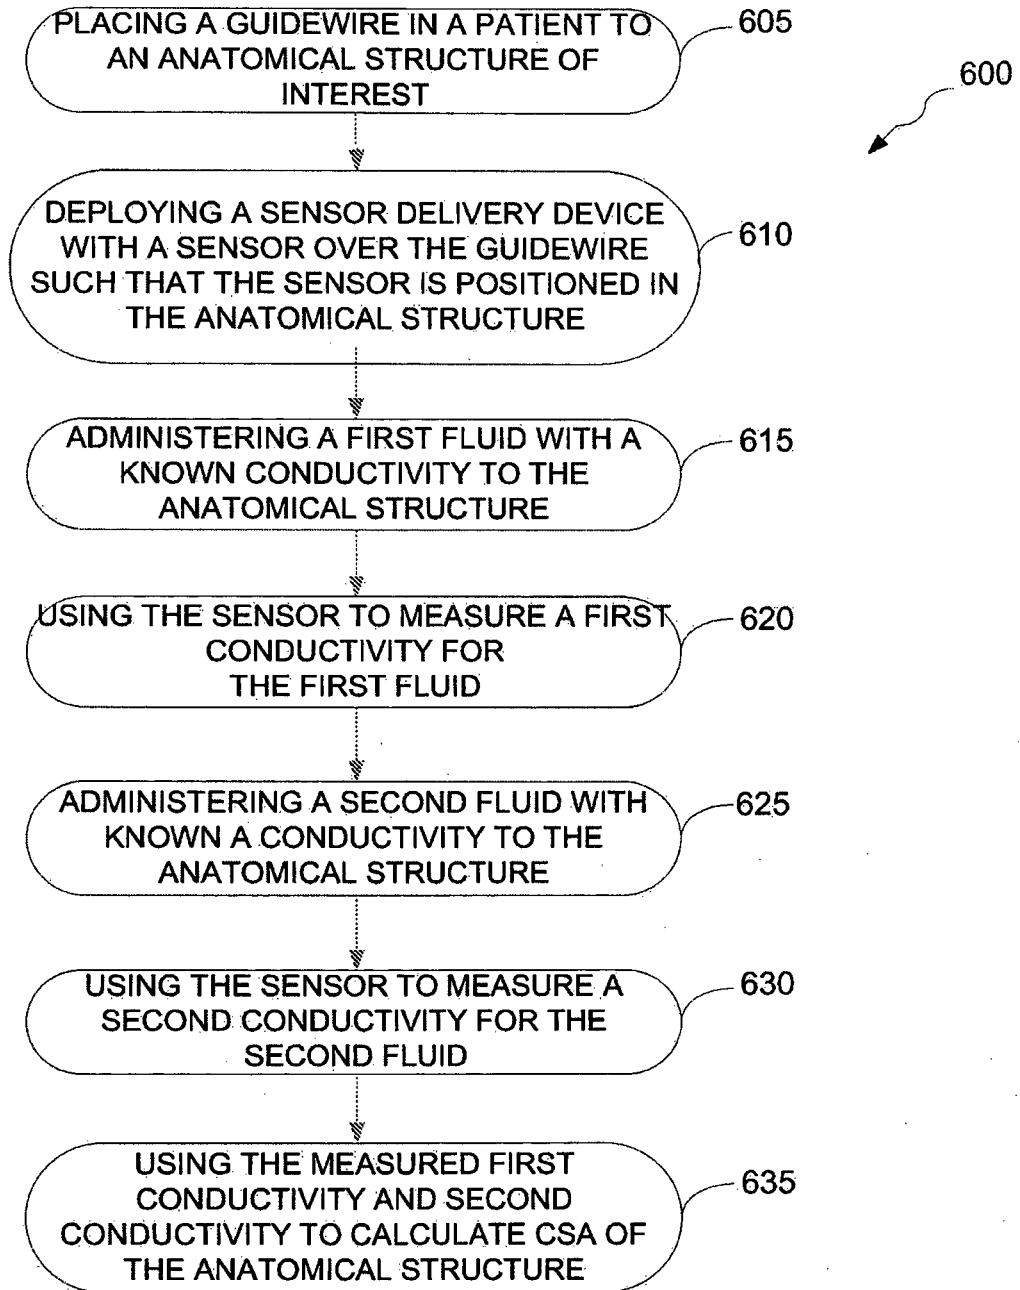


FIG. 9


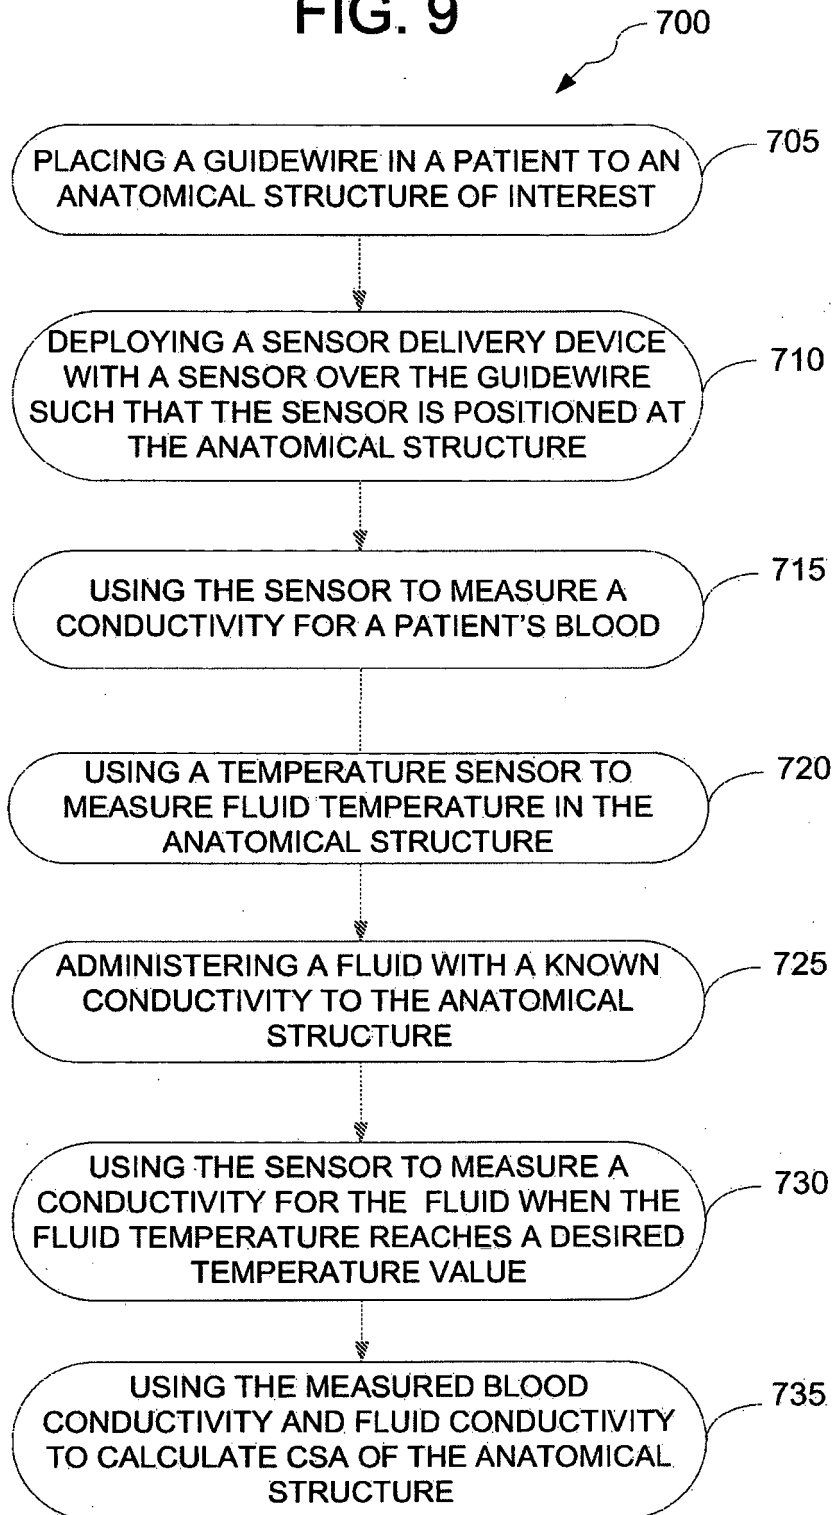


FIG. 10

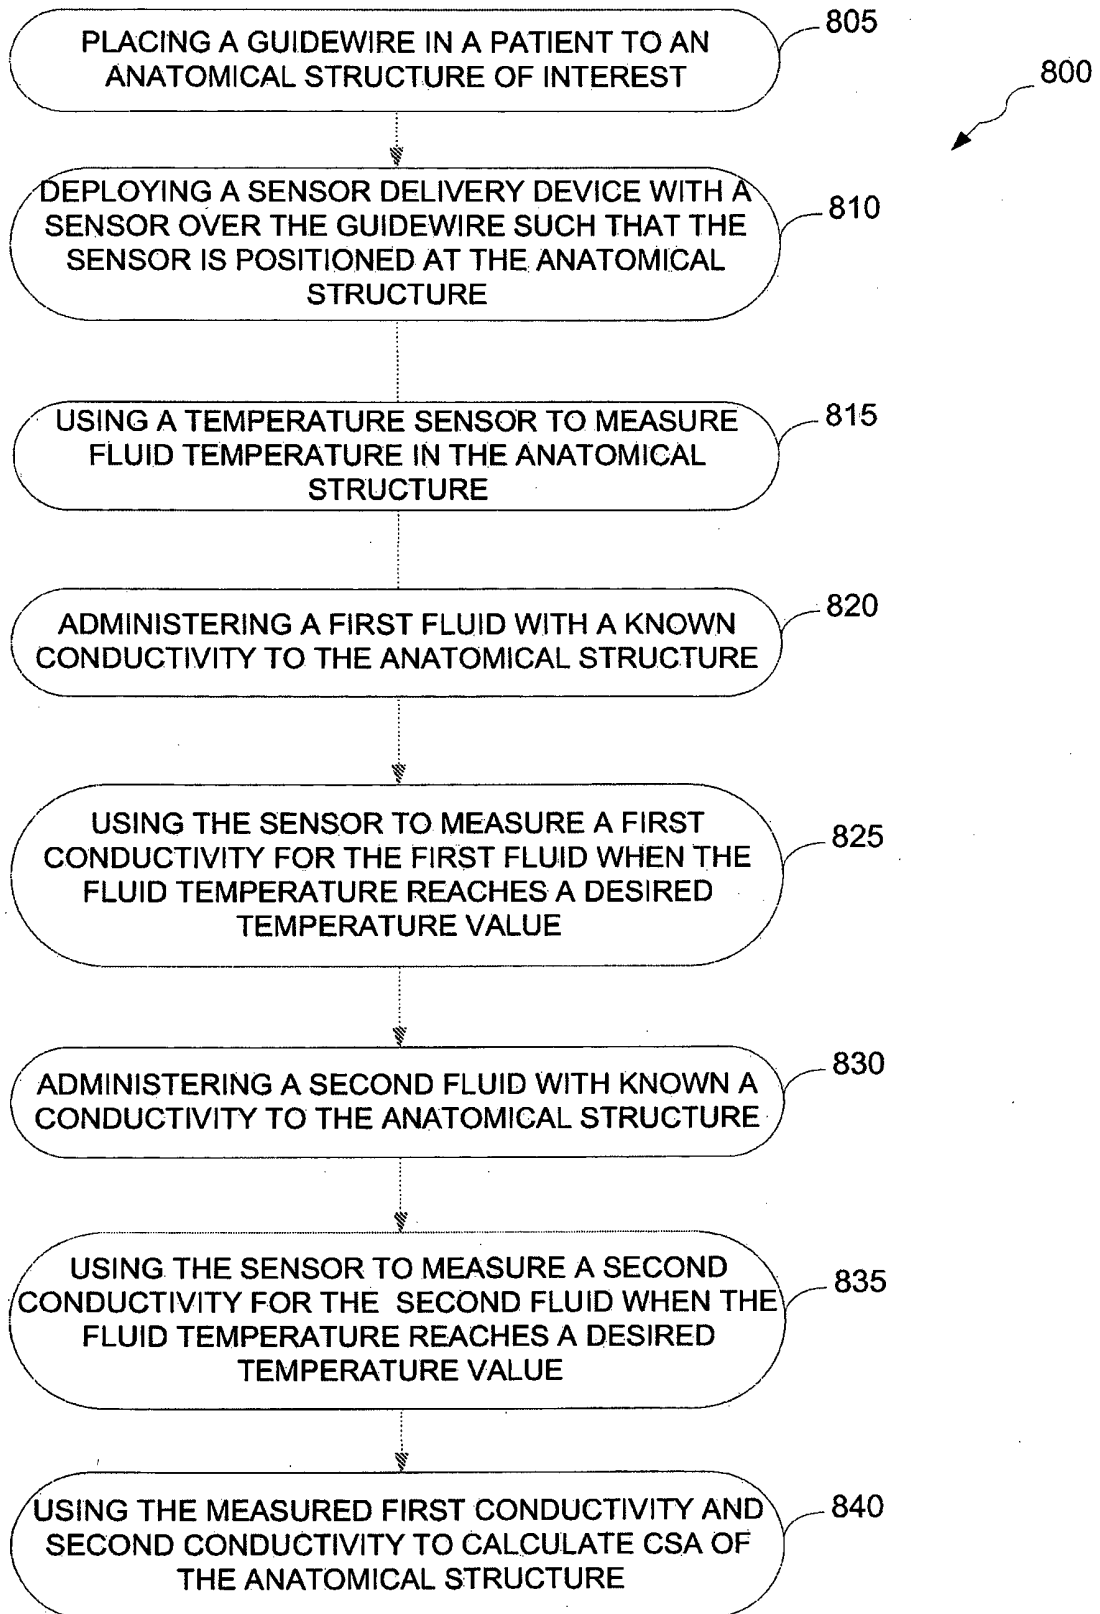

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- WO 2008005388 A [0007]
- US 20100234698 A [0023] [0039] [0041]
- US 12557685 B [0023] [0039] [0041]
- US 7454244 B [0025] [0042]
- US 10782149 B [0025] [0042]

专利名称(译)	用于测量解剖结构的装置		
公开(公告)号	<a href="#">EP2765907B1</a>	公开(公告)日	2016-05-18
申请号	EP2012787943	申请日	2012-10-11
申请(专利权)人(译)	ACIST医疗系统, INC.		
当前申请(专利权)人(译)	ACIST医疗系统, INC.		
[标]发明人	HILTNER JASON FREDRICK		
发明人	HILTNER, JASON, FREDRICK		
IPC分类号	A61B5/053 A61B5/107 A61B5/02 A61B5/00 A61B5/0215		
CPC分类号	A61B5/02007 A61B5/02055 A61B5/02154 A61B5/0535 A61B5/0538 A61B5/1076 A61B5/6851 A61B5/01 A61B5/0205 A61F2/82		
代理机构(译)	BELLONI, GIANCARLO		
优先权	61/547306 2011-10-14 US		
其他公开文献	EP2765907A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

提供了一种传感器输送装置和使用该装置的方法，其中传感器输送装置包括传感器，该传感器适于获得可用于计算周围解剖结构的横截面积的测量值。在某些情况下，传感器是电极布置，其中电极布置产生电流并测量由电流产生的电压。然后使用电压测量来计算周围解剖结构中的流体的导电率，从而计算横截面积。

