

(19)



(11)

EP 1 304 955 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
17.12.2008 Bulletin 2008/51

(51) Int Cl.:
A61B 5/00 (2006.01) A61B 6/00 (2006.01)

(21) Application number: **01951068.4**

(86) International application number:
PCT/US2001/022187

(22) Date of filing: **13.07.2001**

(87) International publication number:
WO 2002/007585 (31.01.2002 Gazette 2002/05)

(54) **USE OF ULTRAVIOLET, NEAR-ULTRAVIOLET AND NEAR INFRARED RESONANCE RAMAN SPECTROSCOPY AND FLUORESCENCE SPECTROSCOPY FOR TISSUE INTERROGATION OF SHOCK STATES, CRITICAL ILLNESSES, AND OTHER DISEASE STATES**

VERWENDUNG VON ULTRAVIOLETT, NAHULTRAVIOLETT UND NAHINFRAROT-RESONANZRAMANSPEKTROSKOPIE UND FLUORESENZSPEKTOSKOPIE ZUR GEWEBEUNTERSUCHUNG AUF SCHOCKZUSTAND, KRITISCHE KRANKHEITEN ODER ANDERE KRANKHEITZUSTÄNDE

UTILISATION DE LA SPECTROSCOPIE RAMAN DE RESONANCE DANS L'ULTRAVIOLET, LE PROCHE ULTRAVIOLET ET LE PROCHE INFRAROUGE ET DE LA SPECTROSCOPIE DE FLUORESCENCE POUR LA DETERMINATION DANS DES TISSUS D'ETATS DE CHOC, DE MALADIES CRITIQUES, ET D'AUTRES TROUBLES

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE TR
 Designated Extension States:
AL LT LV MK RO SI

- **BARBEE, R., Wayne**
 Richmond, VA 23233 (US)
- **TERNER, James**
 Richmond, VA 23229 (US)
- **IVATURY, Rao, R.**
 Richmond, VA 23236 (US)
- **HAWKRIDGE, Fred**
 Glen Allen, VA 23060 (US)

(30) Priority: **13.07.2000 US 218055 P**

(43) Date of publication of application:
02.05.2003 Bulletin 2003/18

(74) Representative: **Lins, Edgar et al**
GRAMM, LINS & PARTNER
Theodor-Heuss-Strasse 1
38122 Braunschweig (DE)

(73) Proprietor: **VIRGINIA COMMONWEALTH UNIVERSITY**
Richmond, VA 23298 (US)

(72) Inventors:
 • **WARD, Kevin, R.**
Glenn Allen, VA 23259 (US)

(56) References cited:
WO-A-00/37917 US-A- 4 832 483
US-A- 5 261 410 US-A- 5 582 168
US-A- 5 769 081 US-A- 5 919 140
US-A- 5 991 653 US-A- 6 069 689

EP 1 304 955 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Field of the Invention

[0001] The invention generally relates to emergency medicine, and especially relates to shock states and critical illnesses and disease states.

BACKGROUND OF THE INVENTION

[0002] Shock is a complex entity, which traditionally has been defined as a state in which the metabolic demands of tissues are not matched by sufficient delivery of metabolic substrates, with the major substrate being oxygen. This mismatch commonly results from altered states of organ perfusion such as hemorrhage. Shock additionally involves complex inflammatory and immune mediated events which result from, and may further exacerbate, this initial metabolic mismatch. Many of these events play an important role in the development of subsequent multiorgan dysfunction, failure and death, with this latter mode responsible for over 60% of trauma deaths. Haljamae, H., "Cellular metabolic consequences of altered perfusion," in Gutierrez, G., Vincent, J., eds., "Update in Intensive Care and Emergency Medicine: Tissue oxygen utilization (Springer Verlag, 1991), pp. 71-86. Despite the complexities of the inflammatory and immune components of trauma and hemorrhage, there is little debate on linking the severity of these events to the severity of initial perfusion deficits and tissue hypoxia. It is therefore essential to recognize and correct perfusion deficits at their earliest possible time. Although this seems intuitive, up to 80% of trauma patients on close monitoring continue to demonstrate evidence of tissue hypoxia secondary to perfusion deficits after what was considered to be complete resuscitation. Abou-Khalil, B., Scalea, T.M., Trooskin, S.Z., Henry, S.M., Hitchcock, R., "Hemodynamic responses to shock in young trauma patients; need for invasive monitoring," Crit. Care Med., 22:633-639 (1994).

[0003] Traditional clinical signs of tissue perfusion such as capillary refill, mental status, heart rate, pulse pressure and systemic blood pressure are very gross indicators of tissue perfusion and can only be considered to be of historic interest except at extreme values. Porter, J., Ivatury, R., "In search of optimal end points of resuscitation in trauma patients," J. Trauma, 44:908-914 (1998). Current markers of tissue perfusion include systemic lactate and base deficit measurements; transcutaneous and subcutaneous gas measurements, gastric and sublingual tonometry and spectroscopic techniques such as NIR absorption spectroscopy, fluorescence quenching, and orthogonal polarization spectral imaging. While these techniques have respective advantages, each is plagued by the relative singularity of its measure, lack of tissue specificity, inability to quantitate, or inability to easily apply or adapt for field use. Identification of any other useful markers is an important objective, and the

search continues for further markers of shock states and the like. Effectively measuring and working with both known markers as well as markers being discovered would be highly beneficial to emergency medicine but is not provided in conventional technology. Information about biochemistry in shock states and disease states has not yet fully found its way and been used in practical applications. Rather, currently emergency medicine is left to rely on physical examination not much advanced by conventional, relatively limited spectroscopic measurement technology.

[0004] That is, much still turns on observation of simple vital signs. Yet, the diagnosis of shock and its severity can be difficult, and cannot be accomplished with certainty, from simple vital signs. A physical exam, including vital signs, is inadequate in detecting states of uncompensated shock. Ward, K.R., Ivatury, R.R., Barbee, R.W., "Endpoints of resuscitation for the victim of trauma," J. Intensive Care Med., 16:55-75 (2001). Dysoxia can be present despite normal vital signs. Ward et al., id.; Abou-Khalil, B., Scalea, T.M., Trooskin, S.Z., Henry, S.M., Hitchcock, R., "Hemodynamic response to shock in young trauma patients: need for invasive monitoring," Crit Care Med. 22(4):633-9 (1994); Scalea, T.M., Maltz, S., Yelon, J., Trooskin, S.Z., Duncan, A.O., Scalafani, S.J., "Resuscitation of multiple trauma and head injury: role of crystalloid fluids and inotropes," Crit Care Med. 22(10):1610-5 (1994); Ivatury, R.R., Simon, R.J., Havriliak, D., Garcia, C., Greebarg, J., Stahl, W.M., "Gastric mucosal pH and oxygen delivery and oxygen consumption indices in the assessment of adequacy of resuscitation after trauma: a prospective, randomized study," J. Trauma, 39 (1):128-34; discussion 34-6 (1995).

[0005] In addition, resuscitation of victims of uncompensated shock back to "normal" vital signs is inadequate as a resuscitation endpoint. Unrecognized continued accumulation of additional oxygen debt is still possible and may contribute to later development of multisystem organ failure and death. Shoemaker, W.C., Appel, P.L., Kram, H.B., "Tissue oxygen debt as a determinant of lethal and nonlethal postoperative organ failure," Crit. Care Med., 16(11):1117-20 (1988).

[0006] Adding, to a physical exam, global measures of oxygen transport still does not ensure detection of early shock states or provide adequate information to act as sole end-points of resuscitation once shock is recognized and therapy instituted. For an outline of all of the current major technologies that have been used to detect the presence of shock and to guide its treatment, see Ward, Ivatury et al., supra. For various reasons, all have been problematic.

[0007] To better understand the difficulties in detecting shock states it is helpful to examine the biphasic relationship between oxygen delivery (DO_2) and consumption (VO_2) to understand the potential inadequacies of currently available monitoring systems. Figure 1 demonstrates that VO_2 can remain constant over a wide range of DO_2 . This is possible because cells have the ability to

increase their extraction of oxygen (OER) in the face of decreased delivery. This is generally reflected by lower hemoglobin oxygen saturations in blood leaving the organ system (SvO₂), which may change before it is apparent in the physical exam. Scalea, T.M., Hartnett, R.W., Duncan, A.O., Atrweh, N.A., Phillips, T.F., Sclafani, S.J., et al., "Central venous oxygen saturation: a useful clinical tool in trauma patients," *J. Trauma*, 30(12):1539-43 (1990); McKinley, B.A., Marvin R.G., Cocanour, C.S., Moore, F.A., "Tissue hemoglobin O₂ saturation during resuscitation of traumatic shock monitored using near infrared spectrometry," *J. Trauma*, 48(4):637-42 (2000). However, there is a point at which OER cannot keep pace with reductions in delivery. At this point VO₂ of the cell or organ falls (critical oxygen delivery: DO₂crit and cells become dysoxic. This results in an increase in the oxidation-reduction (redox) value of the cell, effectively blocking the flow of electrons through the NADH-cytochrome a, a₃ cascade in the mitochondria which prevents the formation of ATP. Cytochrome a, a₃ (cytochrome oxidase) is the terminal electron acceptor in the mitochondrial electron transport chain. Dysoxia can be recognized by the accumulation of a number of metabolic products such as lactate and intracellular reduced nicotinamide adenine dinucleotide (NADH). NADH offers one of the main sources of energy transfer from the TCA cycle to the respiratory chain in the mitochondria. NADH is situated on the high-energy site of the respiratory chain and during tissue dysoxia it accumulates because less NADH is oxidized to NAD⁺. The redox state of the mitochondria (NADH/NAD⁺) therefore reflects the mitochondrial energy state, which in turn is determined by the balance of oxygen availability in the cell and the metabolic rate of the cell. Siegemund, M., van Bommel, J., Ince, C., "Assessment of regional tissue oxygenation," *Intensive Care Med.*, 25(10):1044-60 (1999). Conventional monitoring and measuring used in emergency medicine do not adequately take into account such biochemistry of shock states and the like. Knowing the biochemistry of shock states and the like but not being able to measure and monitor pertinent information thereto has been a frustrating, unresolved problem in emergency medicine. **[0008]** Conventionally, a primary means of assessing tissue perfusion is through infrared (IR) or near-infrared (NIR) spectroscopy. Human skin and tissue are semi-transparent to wavelengths in this range. However, problems with IR technology arise because water strongly absorbs IR radiation. While NIR absorption spectroscopy does not suffer from water absorption as does classical IR, and NIR absorption spectroscopy is useful for the relative quantification of several specific chromophores such as hemoglobin, myoglobin, and cytochrome oxidase. Nakamoto, K., Czernuszewicz, W.S., "Infrared Spectroscopy," in: *Methods in Enzymology*, 226:259-289 (1993); Piantadis, C., Parsons, W., Griebel, "Application of NIR Spectroscopy to problems of tissue oxygenation," in Gutierrez, G., Vincent, J., eds., *Update in Intensive Care and Emergency Medicine: Tissue oxygen utilisation*

(Springer Verlag, 1991) pp. 41-44. Other recent work reports the ability of using NIR absorption shift of hemoglobin to measure pH. However, disadvantageously, NIR signals are so broad as to not be well-suited to quantification of overlapping species. Examples of NIR absorption spectroscopy signals being too broad to lend themselves to quantification of overlapping species include the spectra for oxy and deoxy hemoglobin and cytochrome oxidase (see Figure 2). Owen-Reece, H., Smith, M., Elwell, C.E., Goldstone, J.C., "Near infrared spectroscopy," *Br J Anaesth*, 82(3): 418-26 (1999). Figure 2 is a graph of typical broad signals of oxy and deoxy hemoglobin and cytochrome oxidase obtained by NIR absorption spectroscopy. (In Figure 2, the HbO₂ and Hb signals also would include those from myoglobin.)

[0009] Conventional NADH-fluorescence techniques are more specific and quantitative than classical NIR absorption spectra but can only measure a single marker. The technique has relied on use of excitation wavelengths in the carcinogenic UV region and has not been reduced to clinical practice. Conventional noninvasive or minimally invasive measures of tissue perfusion include transcutaneous and tonometric (gastric or sublingual) monitoring of various gases such as oxygen and carbon dioxide. The major limitations of these devices are that they are limited to monitoring those specific gases and cannot provide additional information that, if provided, could be useful in diagnosis and stratification of patients. Methods such as tonometry can be cumbersome due to its invasive nature. These methods are also prone to deviations through changes either in minute ventilation or inspired oxygen concentration. Transcutaneous gas monitoring, gastric tonometry, and even sublingual tonometry are one-dimensional and are prone to non-flow related changes caused by hypo or hyper ventilation. Also, with the exception of sublingual tonometry, application of these methods in the field is problematic. Weil, M., Nakagawa, Y., Tang, W., et al., "Sublingual capnometry: A new noninvasive measurement for diagnosis and quantification of severity of circulatory shock," *Crit. Care Med.*, 27:1225-1229 (1999).

[0010] Another concern associated with measurement of shock states, and balanced with other factors relating to measurement, is invasiveness. NIR absorption spectroscopy is being aggressively studied to use signals from these chromophores to noninvasively monitor oxygen transport at the tissue level. McKinley et al., supra. Perhaps the best-known use of this technology is in the monitoring of cerebral hemodynamics. The basis for this is that the majority of blood volume in an organ is venous and thus the tissue hemoglobin saturation should reflect the state of oxygen consumption of the tissue. Again, broad overlap of signals in addition to needing to know the pathlength of light presents challenges in quantification and differentiation of signals. For example it is difficult to distinguish hemoglobin and myoglobin making NIR use in hemorrhage problematic since myoglobin has a p50 of only 5 mmHg. Gayeski, T.E., Honig, C.R., "Direct

measurement of intracellular O₂ gradients; role of convection and myoglobin," *Adv Exp Med Biol*, 159:613-21 (1983). Because soft tissue and bone are translucent to NIR light, NIR can penetrate to significant depths, a feature with both advantages and disadvantages. Monitoring the redox state of cytochrome oxidase is also difficult unless baseline absorptions are known. There is also significant overlap between the cytochrome oxidase and hemoglobin signals. Despite this, NIR measurements of tissue saturation (StO₂) are being marketed.

[0011] Although some manufacturers of NIR absorption spectroscopy equipment claim to differentiate between the two species of oxygen hemoglobin and myoglobin, no work to this effect exists in the medical literature. In fact, evidence exists that a major portion of the NIR absorption spectroscopy signal reported from hemoglobin actually originates from myoglobin.

[0012] Another problem for NIR is that in terms of use on hollow organ systems such as the stomach, data from NIR absorption spectroscopy would likely include signals from non-stomach organs and thus not reflect data from the mucosal surface of the stomach.

[0013] Surface NADH fluorescence has been used to detect cellular dysoxia in a number of organ systems. Siegemund et al., *supra*. The traditional technique uses unique excitation light sources and detection filters to take advantage of the fact that NADH will fluoresce (emit light at 460 nm) when excited at a wavelength of 360 nm (near-UV). This technique has been used in video microscopy/fluorometry experiments. Van der Laan, L., Coremans, A., Ince, C., Bruining, H.A., "NADH videofluorimetry to monitor the energy state of skeletal muscle in vivo," *J. Surg. Res.*, 74(2):155-60 (1998). However, such conventional methods do not necessarily provide optimum resolution.

[0014] Adverse effects of certain compounds (such as vasopressin and norepinephrine) on oxygen transport and the immune/inflammatory response are now beginning to be appreciated with manipulation of their actions being studied as therapeutic strategies. Kincaid, E.H., Miller, P.R., Meredith, J.W., Chang, M.C., "Enalaprilat improves gut perfusion in critically injured patients," *Shock*, 9(2):79-83 (1998); Catania, R.A., Chaudry, I.H., "Immunological consequences of trauma and shock," *Ann. Acad. Med. Singapore*, 28(1):120-32 (1999). However, satisfactory measurement of such compounds in vivo without invasive probing has not yet been provided.

[0015] Thus, current technology includes pulmonary artery catheters, repetitive measures of lactate and base deficit, splanchnic tonometry, sublingual tonometry, NIR absorption spectroscopy, transcutaneous gas monitoring, phosphorescence quenching and fluorescence technology (indwelling blood gas/pH catheters). No such technology is without a substantial disadvantage. Civilian prehospital emergency medical services systems, emergency physicians, trauma surgeons, intensive care physicians, cardiologists, anesthesiologists, and military medical personnel continue to be plagued by the insensitivity

of the physical exam, lack of readily available physiologic and metabolic markers to judge the presence and severity of shock states, and lack of real-time relevant measurement approaches. In addition, it has been difficult to use singular measures to guide treatment or predict outcome. These problems are greatly magnified as the scale of the wounded population increases (such as on the battlefield and the various pre-definitive echelons of care provided to wounded soldiers or in a natural disaster). To the inventors' knowledge, currently no conventional techniques are available for real-time monitoring of a broad range of potentially valuable emergency medicine markers of shock, tissue ischemia, tissue injury, tissue inflammation, or tissue immune dysfunction.

SUMMARY OF THE INVENTION

[0016] The invention realizes methods, profiles, medical measurement devices, and other products for accurate measurement of change or lack thereof from non-shock, non-ischemic, non-inflammation, non-tissue injury, non-immune dysfunction conditions which are referred to herein as "baseline conditions". In attention to advantageous accuracy in such measurement, the invention provides practical, real-time approaches for accurately characterizing a patient's condition with respect to baseline conditions. With Raman and/or fluorescence spectroscopy according to the invention, change from baseline conditions is measured, characterized, monitored, identified and/or followed with a high degree of accuracy with measurement times on the order of seconds. Such high-accuracy measurement is achieved with Raman spectroscopy (such as resonance Raman spectroscopy) interrogation of tissue, optionally with simultaneous interrogation by fluorescence spectroscopy of compounds such as NADH. The tissue interrogation advantageously may be non-invasive to minimally invasive to totally invasive. With methods and products according to the present invention, advantageously preclinical (ultra-early) states of shock, tissue ischemia, tissue injury, and tissue inflammation can be detected, severity can be determined, and the effectiveness of various treatments aimed at resolving the shock state can be determined, and other beneficial effects for patient care can be achieved. The invention is as defined in the appended set of claims.

[0017] In order to accomplish these and other objects of the invention, the present invention in a preferred embodiment provides a tissue analysis method, comprising interrogating a biological material (such as a biological tissue or a bodily fluid) with Raman spectroscopy and fluorescence spectroscopy to obtain spectroscopy results.

[0018] In another preferred embodiment, the invention provides a method of diagnosing shock, tissue ischemia, tissue inflammation, or tissue immune dysfunction, comprising: (A) for a target molecule population, taking a sample Raman spectroscopy, and/or fluorescence spectroscopy

copy, profile for a patient; (B) comparing the sample spectroscopy profile with a pre-established Raman spectroscopy and/or fluorescence spectroscopy profile for the target molecule population under baseline conditions.

[0019] A further preferred embodiment provides a spectroscopy comparative profile, comprising: a pre-established Raman spectroscopy and fluorescence spectroscopy profile for a target molecule population under baseline conditions; and a sample Raman spectroscopy and fluorescence spectroscopy profile for the target molecule population.

[0020] The invention also provides for a preferred embodiment which is a method of diagnosing abnormalities in vivo and in situ, comprising: (A) for a target molecule population, taking a sample Raman spectroscopy and/or fluorescence spectroscopy profile for a patient; (B) comparing the sample Raman spectroscopy or fluorescence spectroscopy profile with a pre-established Raman spectroscopy or fluorescence spectroscopy profile for the target molecule population under baseline conditions; and (C) using differences identified in said comparing step to identify an abnormality.

[0021] In a particularly preferred embodiment of the inventive methods, simultaneous fluorescence spectroscopy probing of NADH and resonance Raman spectroscopy are performed.

[0022] Another preferred embodiment of the invention provides a medical measurement device comprising: a spectrometer with multiple wavelength settings for resonance Raman spectroscopy; and a biological probe electrically connected to the spectrometer.

[0023] Additionally, the invention in another preferred embodiment provides a spectroscopy comparative profile, comprising: a pair of Raman spectroscopy or fluorescence spectroscopy profiles for a target molecule population, wherein one profile was taken from a patient after a medical event concerning the patient.

[0024] A further preferred embodiment of the invention provides a computer system comprising: a database of stored baseline Raman spectroscopy and/or fluorescence spectroscopy profiles and a means to store patient Raman spectroscopy and/or fluorescence spectroscopy profiles.

BRIEF DESCRIPTION OF THE DRAWINGS

[0025] The foregoing and other objects, aspects and advantages will be better understood from the following detailed description of the preferred embodiments of the invention with reference to the drawings, in which:

Figure 1 is a traditional biphasic oxygen delivery and consumption curve.

Figure 2 is a graph of oxy and deoxy hemoglobin and cytochrome oxidase obtained by NIR absorption spectroscopy, with Δ optical density plotted versus wavelength (nm).

Figure 3 shows near-UV resonance Raman spec-

troscopy according to the invention for human blood at various oxygen saturation levels.

Figure 4 shows resonance Raman spectroscopy according to the invention of both oxygen hemoglobin and myoglobin.

Figure 5 shows near-UV resonance Raman spectra of isolated ischemic rat skeletal muscle over time.

Figure 6 is a baseline Resonance Raman spectrum for rat muscle, with the signal obtained in one second.

Figures 7, 8, 9 and 10 each is a Resonance Raman spectrum for the same muscle as Figure 6, with respective bleeding of 1 ml, 2 ml, 5 ml and 7.5 ml.

Figure 11 is an overlay of the Raman spectra of Figures 6, 7, 8,9 and 10.

Figure 12 are resonance Raman spectra of a rat tongue.

Figure 13 are near UV resonance Raman spectra of hemoglobin.

Figure 14 is a spectra of baseline NADH fluorescence of the same quadricep muscle from the same animal in which NADH fluoresces after being excited with light at 406.5 nm which is the same wavelength used to produce the previous resonance Raman spectroscopy of Figures 5-10. Figures 15, 16, 17 and 18 each is a spectra of NADH fluorescence for the same muscle as Figure 14, with respective bleeding of 5 ml, 7.5 mls, 9 mls and 12 mls.

Figure 19 is an overlay of NADH fluorescence spectra (Figures 14-18) from the quadriceps muscle.

Figure 20 is an overlay of NADH fluorescence spectra of a rat tongue, for baseline and after 2 cc hemorrhage for 50 minutes.

Figure 21 is an overlay of NADH fluorescence spectra of a rat liver during graded hemorrhage over time (baseline, 40 min, 90 min and 120 min).

Figure 22(a) are preliminary Raman spectra of β -nicotinamide adenine dinucleotide in the oxidized (NAD) and reduced (NADH or NADH) forms. Fig. 22 (b) are preliminary Raman spectra of the high energy phosphates ATP and ADP. Fig. 22(c) are preliminary Raman spectra of the glycolytic end-products pyruvate and lactate, along with the excitatory amino acid and neurotoxin glutamate. Fig. 22(d) are preliminary Raman spectra of the oxygen transporters hemoglobin (Hb) and myoglobin (Mb), from an equine. Figure 22(e) includes preliminary Raman scans of uncooked beef, with the top scan taken in a darker area, and the bottom scan taken in a lighter area with more saturated myoglobin.

Figure 23 is a near-UV resonance Raman spectrum of myeloperoxidase.

Figure 24 is a UV resonance Raman spectrum of vasopressin.

Figure 25 is a UV resonance Raman spectrum of norepinephrine.

Figures 26(a), 26(b), 26(c) and 26(d) are schematic views of devices according to the invention. Figure

26(e) is a top view of a fiber optic bundle shown schematically in Figures 26(b), 26(c) and 26(d).

Figure 27 depicts resonant Raman spectra for horse Hb dilutions.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS OF THE INVENTION

[0026] The present invention provides methods and products in which resonance Raman spectroscopy interrogates biological material (such as tissue or a bodily fluid) at near-UV excitation. The Raman spectroscopy may proceed with or without simultaneous fluorescence spectroscopy (such as NADH fluorescence spectroscopy). The interrogation advantageously may be in a non-invasive to minimally-invasive manner, but is not required to be so and if desired may be invasive. Data from interrogating tissue according to the invention may be used to detect preclinical (ultra-early) states of shock and other tissue injury and disease states, determine severity, and determine the effectiveness of various treatments aimed at resolving the shock or tissue disease/injury state of a patient.

[0027] In a preferred embodiment of the invention, a tissue analysis method comprises interrogating a biological tissue with Raman spectroscopy and fluorescence spectroscopy to obtain spectroscopy results. The Raman spectroscopy used in the present invention is that based on the Raman effect, which has been known for over 70 years and is caused by absorption of light leading to the transition of a molecule from the ground state to an excited state, followed by the emission of light with a different wavelength. Raman, C.V., Krishnan, K.S., "The colour of the sea," *Nature (London)*, 121:619 (1928). The Raman effect has only recently, through the advancements and miniaturization of fiber optic, laser, and detector technology, become a practical technique for clinical use. Because each molecular species has its own characteristic molecular vibrations, a Raman spectrum provides a unique "fingerprint" useful for sample or marker identification. Hanlon, E.B., Manoharan, R., Koo, T.W., Shafer, K.E., Motz, J.T., Fitzmaurice, M., et al., "Prospects for in vivo Raman spectroscopy," *Phys Med Biol*, 45(2):R1-59 (2000); Diem, M., "Introduction to modern vibrational spectroscopy," New York: Wiley (1993). While any wavelength of light theoretically can be used as an excitation source to provide a Raman spectrum, visible excitation can produce strong broadband fluorescence, which undesirably can overwhelm Raman signals. Nevertheless, wavelengths can be chosen that produce resonance due to matching of the excitation wavelength and the electronic energy state of the scattering molecule. While Raman scattering is a rather low energy phenomenon requiring sensitive detectors, the signal is greatly enhanced when the molecule of interest is resonant (absorption maximum near the laser wavelength). This signal enhancement at a resonant frequency may be referred to as "resonance Raman spectroscopy" and allows

for the selective detection of individual species of very low concentration within a complex mixture. Hanlon et al., *supra*.

[0028] If the excitation wavelength does not induce fluorescence within the wavelength region of interest, then remarkably high resolution Raman spectra can be obtained. If fluorescence does occur, this can be reduced or even eliminated in many instances by tuning of the excitation wavelength. Thus, while interfering fluorescence may occur with a particular excitation wavelength, it may not occur within the UV or NIR range where one could detect signals either above or below the fluorescing region, as the case may be. Hanlon, E.B., Manoharan, R., Koo, T.W., Shafer, K.E., Motz, J.T., Fitzmaurice, M., Kramer, J.R, Itzkan, I, Dasari, R.R, and Feld, M.S., "Prospects for in vivo Raman spectroscopy," *Phys. Med. Biol.*; 45: R1-R59 (2000).

[0029] In the invention, the wavelengths for the Raman spectroscopy and/or fluorescence spectroscopy are wavelengths for which such spectroscopy equipment may be set, suitably for interrogating biological tissue in a living patient. Preferably resonance Raman spectroscopy according to the invention is performed at a deep ultraviolet wavelength, i.e., at 390 to 420 nm. Modifications of Raman spectroscopy that can be applied include Fourier Transform Raman Spectroscopy, Nonlinear Raman Spectroscopy, Raman difference spectroscopy, and Raman Optical Activity.

[0030] Examples of Raman spectra are Figures 3, 4, 5, 6, 7, 8, 9, 10, 11, 12, 13, 22(a)-(e), 23, 24, 25. Examples of NADH fluorescence spectra are Figures 14, 15, 16, 17, 18, 19, 20, 21.

[0031] The inventive methods, products and profiles may include signal enhancement at a resonant frequency for a target molecule of the target molecule population. The inventive methods may include operating an electromagnetic radiation generator at a range of selectable wavelengths from about 270 nm to about 20,000 nm. Spectroscopy may be performed for multiple wavelengths. Preferably the Raman spectroscopy is resonance Raman spectroscopy at 390 to 420 nm wavelength. Because basic Raman scattering is a rather low intensity phenomenon requiring sensitive detectors, preferably Resonance Raman Spectroscopy (RRS) techniques are used, to enhance the signal when the molecule of interest is resonant (absorption maximum near the laser wavelength). The signal strength of Raman can be boosted by several orders of magnitude by providing areas of resonance. Also, use of resonant wavelengths will allow limiting laser power density to a minimum (well below the skin damage threshold of 4 watts/cm²). Fluorescence can be avoided by choosing wavelengths not prone to this phenomenon, and through fluorescence quenching. Conversely, fluorescence may be advantageously used for quantification if a particular target is found to have identifiable Raman spectra in one light range such as the NIR but fluoresces at another light range such as the UV. Use of near UV wavelengths (vi-

olet, ~ 406 nm) will avoid the mutagenic potential of UV radiation, while insuring a strong Raman signal.

[0032] The use of Raman spectroscopy in the near-UV range within the clinical settings according to the invention has several advantages with respect to other optical techniques such as IR and NIR absorption spectroscopy. Use of resonance Raman spectroscopy in the near-UV range (406.7 nm) may overcome many problems associated with NIR absorbance spectroscopy and other markers of tissue perfusion. Raman spectroscopy in the NIR takes advantage of the remark transparency of tissue at these wavelengths, while at the same time providing high-resolution vibrational signals. Spiro, T.G., "Resonance Raman spectroscopy: A new structure probe for biological chromophores," *Accts. Chem. Res.*, 7:339-344 (1974); Turner, J., El-Sayeh, M.A., "Time-resolved resonance Raman spectroscopy of photobiological and photochemical systems," *Accts. Chem. Res.*, 18: 331-338 (1985). Hemoglobin has strong absorption and resonance properties in the near-UV range. Figure 3 depicts data from human blood samples in the laboratory demonstrating the sharp peaks of oxy and deoxy human hemoglobin samples. (The area under the curve (AUC) in Figure 3 of the Raman spectra produce oxygen saturations comparable to that from a multiwavelength coximeter.) Comparison of area under the curves of the oxy-peak and blood gas saturations yielded a correlation coefficient of 0.997. These sharp peaks should be compared to the broad overlapping peaks of oxy and deoxy hemoglobin obtained by NIR absorption spectroscopy in Figure 2. Furthermore, the resonance Raman effect for hemoglobin is so specific that it can be differentiated from the resonance Raman effect of myoglobin (see Figure 4). Figure 4 shows resonance Raman spectroscopy of both oxygen hemoglobin and myoglobin, demonstrating an ability to distinguish between the two.

[0033] Analyzing the spectroscopy data by computing the AUC has been mentioned. Alternately to computing area, peak height analysis may be performed. For example, tissue hemoglobin oxygen saturation (StO₂) may be determined by either comparing area under the curve of the spectra for both oxyhemoglobin and deoxyhemoglobin and/or comparison of the peak heights between the two species. Each computation provides a percentage. The latter technique is likely to be preferable.

[0034] A characteristic of near-UV light is that it can only penetrate tissue to a depth of 1-2 mm and is non-carcinogenic. Although at first thought, depth of penetration might seem to be a disadvantage, actually there is not such a disadvantage. Pathlength becomes less important in this case in terms of quantification issue. Probe contact may be unnecessary, and fiber optics may be simplified. In terms of shock states, blood flow to the surface of any organ is compromised first. In terms of use on hollow organ systems such as the stomach, signals from near-UV resonance Raman spectroscopy would be only from the mucosal surface (an advantage over data from NIR absorption spectroscopy which would likely in-

clude signals from non-stomach organs and thus not reflect data from the mucosal surface of the stomach.)

[0035] While taking the Raman spectroscopy profile and the fluorescence spectroscopy measurement on the patient at the same time is a preferred embodiment, it will be appreciated that in other embodiments the invention does not require using both Raman and fluorescence spectroscopy.

[0036] The fluorescence spectroscopy (such as broadband fluorescence spectroscopy) of the present invention, is performed at between 390 and 800 nm. A most preferred example of fluorescence spectroscopy according to the invention is NADH surface-subsurface fluorescence spectroscopy.

[0037] As examples of the biological tissue according to the invention may be the brain, heart, lung, liver, blood, tongue or other oral mucosa, eye (such as the cornea or retina), the esophagus and stomach, peripheral skeletal muscle, skin, intestines, pancreas, kidney, bladder, urethra, skin, nailbed, cervix, uterus, oropharynx, nasopharynx, esophagus, blood etc. Probing on the tongue/oral mucosal, skin, or cornea/retina optionally may be totally noninvasive, without the requirement for probe contact with tissue. For probing the esophagus or stomach, simple fiber optics are constructed into a nasogastric tube for measurements at the level of the esophageal or stomach mucosa. Fiber optics also can be used in urinary catheters for monitoring of substances in the urine or for interrogation of the bladder mucosa. Skeletal muscle or dermis can be assessed with fiber optics of a size insertible through small needles, inserted into a muscle belly such as the deltoid or quadriceps.

[0038] The inventive methods may include monitoring a specific tissue bed (brain, heart, lung, liver, eye, blood, etc.) in the patient; placing a probe on or near any mucosal or epithelial covered surface of a body or an organ; detecting exhaled markers or mediators of organ injury (such as by placing a detector at the airway of the patient). Examples of exhaled markers or mediators are isoprostanes and/or myeloperoxidase.

[0039] Markers also may be present in a biological material according to the present wherein the markers are contained in urine, saliva, wound exudates, vitreous humor, aqueous humor, tissue exudate, gastric contents, fecal matter, or other biological materials.

[0040] The interrogating of biological material such as tissue according to the invention may be, but is not required to be, noninvasive. To maximize the number of markers and mediators that can be measured, a minimally invasive approach is preferred. Interrogating may be intermittently or continuously. A preferred example of minimally invasive probing is by minimally invasively probing the patient by a fiber optic probe or probe array inserted into a tissue bed. The tissue may be in vivo and in situ, but is not required to be. Alternately, the tissue may be removed from a patient before the tissue interrogation. As examples of interrogating tissue are mentioned inserting a probe or probe array into a muscle.

Preferably interrogation is by a minimally invasive probe approach, with muscle and interstitium being interrogated directly. Such a minimally invasive approach is preferred for several reasons. UV light does not significantly penetrate epidermis. NIR light can penetrate several centimeters of tissue and can thus probe epidermis, dermis, and muscle. The inability to know the path length of light and to separate the signal of myoglobin from hemoglobin make interpretation of data for the noninvasive use of NIR absorption spectroscopy at any site other than the brain to be conventionally difficult, and a drawback to be avoided. The large number of valuable markers, which can be detected in the UV and NIR range by Raman spectroscopy, more than outweigh any drawback to placing a small probe intramuscularly. Bench experiments have allowed measures to be made of such substances as hemoglobin within cells in the UV range. (See J. Turner, T.G. Spiro, M. Nagumo, M.F. Nicol, and M.A. El-Sayed, "Resonance Raman spectroscopy in the picosecond timescale: the CO hemoglobin photo-intermediate," J. Amer. Chem. Soc., 102: 3238-3239 (1980); J. Turner, J.D. Stong, T.G. Spiro, M. Nagumo, M.F. Nicol, and M.A. El-Sayed (1980), "Picosecond resonance Raman spectroscopic evidence for excited state spin conversion in carbonmonoxy-hemoglobin photolysis," Proc. Natl. Acad. Sci. USA, 78: 1313-1317; J. Turner, T.G. Spiro, D.F. Voss, C. Paddock and R.B. Miles, "Picosecond resonance Raman spectroscopy of oxyhemoglobin photolysis," J. Phys. Chem., 86: 859-861 (1982)). Such results indicate that cell penetration of the near-UV wavelength in the interstitium will not pose a major problem.

[0041] In the inventive methods and products, the obtained spectroscopy results preferably may be for at least one mediator or marker associated with a shock state and/or tissue injury; tissue ischemia, tissue inflammation and/or tissue immune dysfunction; for presence and/or proportions for the at least one shock state and/or tissue injury mediator or marker; for at least one mediator associated with a shock state and/or tissue injury or tissue ischemia, inflammation or immune dysfunction and/or for at least one marker of tissue perfusion or injury.

[0042] A marker and/or mediator according to the present invention may be within intracellular, interstitial or intravascular space or within exhaled air from a patient. The marker and/or mediator may be selected from the group consisting of lactate, pyruvate, ATP, PCr, AMP, ADP, Pi, NAD, NADH, albumin, endotoxin, exotoxin, microbes, cytokines-chemokines, procalcitonin, hormones, myeloperoxidase, elastase, xanthine oxidase, xanthine dehydrogenase, fatty acid binding proteins, catecholamines and vasoactive peptides. The marker or mediator may be a metabolic or pro or anti-inflammatory marker or mediator. Cardiac biomarkers, GI markers, cerebral markers, skin markers, lung markers, blood markers, and/or eye markers, etc. are mentioned as examples.

[0043] Examples of spectroscopy results according to the invention may be, e.g., data relating to diagnosing and/or following progression or resolution of shock states

and/or tissue injury (such as inflammatory or immune dysfunction), and/or tissue ischemia; determining whether the tissue has insufficient oxygen delivery to meet metabolic demands of the tissue while simultaneously determining whether mitochondrial dysfunction or injury exists; monitoring for appearance of one or more tissue markers specific for a specific disease state; determining tissue viability; diagnosing tissue injury, tissue inflammation or tissue immune dysfunction; and/or continuously interrogating the patient for appearance of abnormal tissue markers specific for a suspected disease state. A preferred example of spectroscopy results are results relating to diagnosing shock.

[0044] As examples of spectroscopy results according to the present invention may be given data for tissue hemoglobin oxygen saturation including amount of oxyhemoglobin and deoxyhemoglobin by Raman spectroscopy; data for NADH presence and/or accumulation by fluorescence spectroscopy; data for oxygenated hemoglobin, deoxygenated hemoglobin and/or NADH; data for myoglobin oxygenation saturation; data for cytochrome oxidase redox status; data for pH of the tissue. A most preferred example of spectroscopy results is data for tissue hemoglobin oxygen saturation by Raman spectroscopy combined with data for NADH presence and/or accumulation by fluorescence spectroscopy.

[0045] The spectroscopy results according to the invention may be for absolute concentration (such as absolute concentration of hemoglobin in the tissue) or for relative concentration. Examples of relative concentrations are NAD/NADH; lactate/pyruvate; Pcr-ATP; ATP-ADP; Pcr-Pi; oxidized cytochrome oxidase to reduced cytochrome oxidase, and/or oxyhemoglobin with deoxyhemoglobin.

[0046] The spectroscopy results according to the invention advantageously are available on the order of seconds. Signal processing and computer algorithms may be used to process the spectroscopy data.

[0047] Another preferred embodiment of the invention provides a medical measurement device comprising: a spectrometer with multiple wavelength settings for resonance Raman spectroscopy; and a biological probe electrically connected to the spectrometer. Inventive medical measurement devices optionally may include a fluorescence spectrometer electrically connected to the biological probe; a laser source (such as a laser tunable to multiple wavelengths) and a charge coupled device. By using a laser tunable to multiple wavelengths, multiple target molecules may be detected. Such multiple target molecules may have useful detectable absorption, resonance Raman and fluorescence spectra at differing wavelengths. Exemplary devices according to the invention may be seen with regard to Figure 26(a)-(e).

[0048] With reference to Figure 26(a), a fixed frequency laser (preferably such as a laser **LS** including, but not limited to, wavelengths of approximately 290 to 420 nm) is piped **1** through one leg of a fiber ' optic bundle. An example of fiber optic bundle **100** is seen in further detail

in Figure 26(e), shown in a configuration of one emitting fiber optic **101** (in the center) surrounded by eight collecting bundles **102**. A fiber optic bundle **100** is only one example, and the fiber optic bundle may be otherwise configured, such as containing one emitter and one or several sensor fibers, in a ratio of one emitter to one sensor up to one emitter to twelve sensors. The number of emitters could be increased and the spaces between emitters and detectors changed. The emitters and detectors might also be placed along the length of the probe as opposed to its end. The fiber optic bundle **100** may be positioned on or within a tissue sample. Re-emission from the tissue sample is collected in back-scattering configuration by the same fiber optic bundle. The end of the fiber optic bundle preferably is placeable directly onto the surface of a tissue such as the oral mucosal or heart. Alternatively, the fiber optic bundle is placeable directly into a tissue such as the brain or liver. The fiber optic arrangement does not require contact with the tissue especially when extraneous light (ambient light) is prevented from entering the fiber optic sensor.

[0049] A preferred example of an invasive fiber optic probe is one that is less than 0.2 mm, and which can be rapidly placed singularly or in an array in a muscle bed through a small gauge hypodermic needle. When such a needle is used to place a probe, after insertion the needle may then be removed and the probe secured in place such as by medical tape.

[0050] Again referring to Fig. 26(a), the light collected by the fiber optic is notch filtered by a laser notch filter system **200** (comprising at least one and preferably two laser notch filters) and then distributed to a spectrograph system **300** (preferably such as a spectrograph system comprising a Raman spectrograph system and a fluorescence spectrograph system). The spectrograph system **300** has a respective CCD detector system **400** associated with it. The CCD detector system preferably comprises a CCD detector for each spectrograph system, i.e., when using a Raman spectrograph system with a fluorescence system, the Raman spectrograph system has an associated CCD detector and the fluorescence system has an associated CCD detector. The CCD detector system **400** provides signals to a signal analyzer **500** (such as a PC type computer). It will be appreciated that respective systems **200**, **300** and **400** each respectively may include one, two, three or more components, with some examples of such systems being given in Figures 26(b), 26(c) and 26(d). Preferably, laser notch filter system **200** comprises at least one laser notch filter, spectrograph **300** comprises at least one spectrometer and CCD detector system **400** comprises at least one CCD detector.

[0051] In a particularly preferred embodiment of the invention, an exemplary device is provided incorporating both Raman spectroscopy and fluorescence spectroscopy. The exemplary device according to Figure 26(b) is an example of such an inventive device combining Raman and fluorescence spectroscopy. With reference to

Figure 26(b), the light collected by the fiber optic is notch filtered **2**, **2'b** and distributed to spectrometers such a spectrograph system set for Raman **3** and a spectrograph set for broadband fluorescence **30**. An example of the Raman spectroscopy system **3** may include two spectrometers containing high groove density gratings, one set to collect Raman scattering between 300 and 3700 cm^{-1} from the laser line (collecting the Raman signal of water to use as an intensity standard) and one set to collect Raman scattering between 1200 and 1700 cm^{-1} (heme vibrations). An example of the fluorescence spectroscopy system **30** contains a low groove density grating and is set to collect broadband fluorescence emission within the region 200 to 800 nm. The Raman spectrograph system **3** has a respective CCD detector system **4** associated with it, and the fluorescence spectroscopy system **30** has a respective CCD detector system **40** associated with it. The CCD detector systems **4**, **40** provide signals to an analysis system, such as a PC type computer **5**.

[0052] With an equipment set-up according to Figure 26(b), levels of oxyhemoglobin, deoxyhemoglobin (and thus tissue hemoglobin saturation), and NADH accumulation, may be determined. Information necessary to determine blood pH within the tissue as well as the absolute concentration of hemoglobin within the tissue may be obtained. As for computing concentration, an example may be appreciated with reference to Figure 27, demonstrating that the resonant Raman spectroscopy technique can detect differences in the amount of hemoglobin present. Hemoglobin levels (in absolute terms) may be determined in tissue, by examining the intensity of the signals (y-axis in Figure 27). The more hemoglobin present in the tissue, the higher the resulting signal intensity. These intensities may be compared to known standards for the determination of hemoglobin amount.

[0053] Another example of an exemplary inventive device is one comprising an electromagnetic radiation generator (such as a laser) with a wide range of selectable wavelengths (such as deep ultraviolet, less than 270 nm to shortwave infrared all the way to 20,000 nm), filters, lenses, fiber optics, a charge coupled device (CCD), a spectrograph, and the software necessary to interpret the Raman shifts. The device can obtain resonance Raman spectra at a variety of wavelengths corresponding to the "fingerprint" or "signature" of molecules associated with tissue oxygen metabolism (such as hemoglobin (Hb), myoglobin (Mb), cytochrome oxidase (cyt a, a3), dissolved or free gases (i.e., O_2 , CO_2 , CO, NO, etc. in tissues, exhaled respiratory gas or intraluminal gastrointestinal gas), glucose, lactate, pyruvate, and bicarbonate. Various mediators associated with shock such as tumor necrosis factor (TNF) and other pro and anti-inflammatory cytokines, catecholamines (epinephrine, norepinephrine and dopamine), general and destructive proteins such as albumin and myeloperoxidase respectively, high energy phosphates (ATP, PCr, ADP, Pi), metabolic energy intermediates (NAD, NADH), excitatory

amino acids (glutamate, aspartate), and vasocative peptides (vasopressin, angiotensin II, natriuretic peptides, etc) can also be measured with such a technique.

[0054] Devices according to the invention may be used in a multiparametric system for non-invasive or minimally invasive monitoring of tissue perfusion and metabolism in critically ill or injured patients. Because the technique permits identification of an almost unlimited number of target compounds, ultra-early detection may be provided, as well as complete characterization and differentiation of various pathologic states. The invention provides also for determining when treatment is complete. The inventive methods and devices may be applied with regard to various shock states, and ischemia of various organ or organ systems such as the heart, brain, and gastrointestinal tract. Probes for the device may be placed within any tissue bed to monitor the state of a specific tissue. The probes and techniques also may be used to reflect the state of the organism as a whole. Probes may be constructed for intravascular placement as well as placement into other devices such as urinary catheters, gastrointestinal tubes and endoscopes, heart catheterization equipment, brain and other tissue monitoring devices.

[0055] Devices may be used in the operating room to examine target molecules and the status of various organs such as the liver, GI tract, brain or heart or other tissues of interest. Implantable probes may be placed in transplanted tissues to allow for their interrogation at subsequent time points to monitor for rejection.

[0056] In another preferred embodiment, the invention provides a method of diagnosing shock, tissue ischemia, tissue inflammation, or tissue immune dysfunction, comprising: (A) for a target molecule population, taking a sample Raman spectroscopy, and/or fluorescence spectroscopy, profile for a patient; (B) comparing the sample spectroscopy profile with a pre-established Raman spectroscopy and/or fluorescence spectroscopy profile for the target molecule population under baseline conditions. A further preferred embodiment provides a spectroscopy comparative profile, comprising: a pre-established Raman spectroscopy and fluorescence spectroscopy profile for a target molecule population under baseline conditions; and a sample Raman spectroscopy and fluorescence spectroscopy profile for the target molecule population.

[0057] The profiles according to the invention may be of relative amounts, or of absolute amounts. The sample profile may be taken from a tissue or a space in a body, or taken from a tissue or a space out of the body. The respective profiles are not required to be from the same species. The comparative profiles in a preferred example include a pre-established fluorescence spectroscopy profile for NADH under baseline conditions and a sample fluorescence profile for NADH. In another preferred example, a spectroscopy comparative profile includes a pair of Raman spectroscopy profiles and a pair of fluorescence spectroscopy profiles (such as one Raman

spectroscopy profile and one fluorescence spectroscopy profile taken from a patient after a medical event concerning the patient).

[0058] Preferred examples of target molecule populations are NAD/NADH; lactate/pyruvate; PCr-ATP; ATP-ADP; PCr-Pi; oxidized cytochrome oxidase to reduced cytochrome oxidase, and/or oxyhemoglobin with deoxyhemoglobin. However, it will be appreciated that further potential target molecule populations may be screened and selected as target molecule populations according to the invention.

[0059] Desired features of a marker(s) of tissue perfusion are its early change after injury; and, that its normalization would indicate that resuscitation is complete. This would help to ensure that shock is detected at its earliest possible time point and that resuscitation would not be prematurely stopped. In addition, the marker(s) would not be subject to misinterpretation from factors such as changes in minute ventilation, pain, etc.

Experimentation: Markers

[0060] Using lab bench versions with diode array detection, Raman spectroscopy was used in the UV and NIR in both reflectance and transmission mode to identify several compounds having utility as markers of hemorrhage severity and its sequelae. The first group are oxygen sensitive markers of ischemia and include hemoglobin (Hb), myoglobin (Mb) and cytochrome oxidase (Cyt aa₃). The second group is of exquisitely sensitive oxygen-related metabolic markers of shock including lactate, pyruvate, nicotinamide adenine dinucleotide phosphate (NAD) and NAD reduced form (NADH). A third group includes the high-energy phosphates phosphocreatine (PCr), adenosine-5'-triphosphate (ATP) and adenosine-5'-diphosphate (ADP). The fourth group includes the vasoactive chemicals epinephrine and norepinephrine.

[0061] Raman spectra were obtained of post-hemorrhage markers in inflammation such as lipopolysaccharide (LPS) and cytokines such as tumor necrosis factor- α (TNF- α). Sample spectra of lactate, pyruvate, NADH, NAD, PCr, and ATP are shown in Figures 27(a), 27(b) and 27(c). Lactate and pyruvate can be easily discriminated by comparing the intensities measured at 1625 cm⁻¹. NAD/NADH can be discriminated by examining the peak around 1690 1625 cm⁻¹. PCr can be separated from other high-energy phosphates with the intensity at 1475 cm⁻¹, while ATP and ADP can be separated with the peaks at 1100 and 1400 cm⁻¹.

[0062] Of particular interest in detecting the presence and severity of hemorrhagic shock are lactate/pyruvate, NADH/NAD, PCr/ATP ratios and the redox status of cytochrome oxidase in skeletal muscle. In addition, hemoglobin concentration, oxygen saturation, and potentially myoglobin oxygen saturation may be obtained. The lactate/pyruvate ratio provides information on the coupling of glycolysis to oxidative phosphorylation, the

NADH/NAD ratio provides information concerning the mitochondrial energy state, and the PCr/ATP ratio provides information concerning utilization of high-energy phosphate stores. Haljamae, H., "Cellular metabolic consequences of altered perfusion," in Gutierrez, G., Vincent, J., eds., "Update in Intensive Care and Emergency Medicine: Tissue oxygen utilization (Springer Verlag, 1991), pp. 71-86. These indices are considered significantly more sensitive than the redox status of cytochrome oxidase or the local level of hemoglobin concentration, oxygen saturation or pH. Even so, monitoring of current NIR absorption spectroscopy derived parameters such as the redox status of cytochrome oxidase and hemoglobin concentration and saturation may be obtained with Raman spectroscopy and can be performed with greater confidence for potential quantification. One of the major advantages of the use of Raman spectroscopy over NIR absorption spectroscopy is its potential to differentiate the signal of hemoglobin from myoglobin.

[0063] Measuring lactate alone is known to be problematic because of the contribution of increased aerobic glycolysis on lactate production secondary to elevations in systemic catecholamine levels. This may occur in the absence of continuing tissue hypoxia. Luchette, F., Roboinson, B., Friend, L., McCarter, F., Frame, S.B., James, J.H., "Adrenergic antagonist reduce lactic acidosis in response to hemorrhagic shock," J. Trauma, 46: 873-880 (1999). However, knowing the lactate/pyruvate ratio along with NADH/NAD and PCr/ATP ratios will provide the operator clear insight into whether true tissue hypoxia is occurring and its severity. In addition, because there is a definite lag in metabolism of lactate, restoration of adequate perfusion will likely result in return of the above ratios before normalization of lactate, thus informing the operator that instituted therapies are working or failing. Additional sensitivity could be added by external stimulation of a few muscle fibers to examine the rate of degradation and restoration of the above metabolic intermediates. Failure to normalize these values in a timely manner indicates a state of intractable shock.

[0064] The use of Raman in the near-UV and NIR has additional advantages of allowing caretakers to detect the progression of hemorrhagic shock to more complex forms of shock such as sepsis. Spectra have been obtained for inflammatory markers such as myeloperoxidase and cytokines such as TNF- α . In addition, spectra have been obtained on lipopolysaccharide, and d-lactate, which are markers indicative of intestinal barrier breakdown. Spectra on the catecholamines epinephrine and norepinephrine have been obtained. These vasoactive substances are now being recognized as sensitive markers of the level of hypoperfusion and stress caused in various shock states. These observations may be extended to vasoactive peptides such as vasopressin and angiotensin, which have been measured in rat pheochromocytoma cells by Schulze et al. Schulze, H.G., Greek, L.S., Barbosa, C.J., Blades, M.W., Gorzalka, B.B., Turner, R.F.B., "Measurement of some small-mol-

ecule and peptide neurotransmitters in-vitro using a fiberoptic probe with pulsed ultraviolet resonance ultraviolet resonance Raman spectroscopy," J. Neurosci. Meth., 92: 15-24 (1999).

[0065] Thus, markers mentioned herein have remarkable utility when examined in a manner of ratios. Also, absolute quantification can be obtained using embedded standards in probes placed in parallel with other emitting and sensing probes, from which can be determined an exact path length of light. The markers mentioned in this experiment were found to be detected by UV and NIR Raman spectroscopy in both the reflectance and transmission mode gives flexibility of design of methods and products according to the invention.

In Vivo Spectroscopic Experimentation

[0066] Techniques according to the invention have been successfully applied to several tissue sites in animals, demonstrating feasibility. Techniques according to the invention require no probe contact (although probe contact with tissue can take place if desired) with tissue and acquisition times are on the order of seconds.

[0067] Figure 5 represents near UV resonance Raman signals taken from skeletal muscle subjected to isolated tourniquet ischemia. Signals were obtained in one minute (i.e., scans were acquired in one minute segments). The oxyhemoglobin signal (1375) decreases simultaneous to the increase in the deoxy hemoglobin signal (1357).

[0068] Figures 6-11 represent near UV-resonance Raman spectroscopy data of oxy and deoxy hemoglobin (with only gross signal processing) from the exposed quadriceps muscle from a rat during hemorrhage. Using area under the curve and peak height comparison analysis, tissue saturations are demonstrated to decrease during hemorrhage. Of importance is that significant tissue desaturation occurs despite the maintenance of normal vital signs. These values for oxyhemoglobin are very similar to those reported with NIR absorption spectroscopy.

[0069] Figure 7 is for 1 ml bleeding of the same muscle as Figure 6, which is the baseline spectrum. At 1 ml bleeding, no change in the oxy or deoxy peak was observed, and there was no change in vital signs. Figure 8 is for 2 ml bleeding of the same muscle as Figures 6 and 7. At 2 ml bleeding, an evolving deoxy peak is to be noted, while the animal maintained normal vital signs. At 5 ml bleeding (Figure 9) for the same muscle as Figures 6-8, a progressively greater deoxy signal is observed, and, although vital signs (MAP decreasing) are still within the normal range. Where 7.5 ml of bleeding (Figure 10) has occurred for the same muscle as Figures 6-9, the animal demonstrated physical evidence of decompensate shock; however, Raman spectroscopy indicates greater severity than the vital signs might predict. Results from Figures 6-10 are summarized in Table 1 below.

Table 1

	OxyHb	DeoxyHb
Baseline (Fig. 6).	69%	31%
1 ml bleed (Fig. 7)	68%	32%
2 ml bleed (Fig. 8)	53%	47%
5 ml bleed (Fig. 9)	30%	70%
7.5 ml bleed (Fig. 10)	14%	86%

[0070] A similar experiment to that of Figures 6-11 was performed using the tongue as the target organ, as seen with reference to Figure 12, which shows resonance Raman spectra demonstrating saturation changes during 3 cc hemorrhage. The signal was obtained in 5 seconds. Again, changes in tissue saturation occurred prior to changes in vital signs, demonstrating that the use of Raman spectroscopy according to the invention can be totally noninvasive.

[0071] Figure 13 demonstrates that near-UV resonance Raman spectroscopy of hemoglobin may be used to monitor tissue pH in a manner similar to that of NIRS. The spectra of Figure 13 are from pure oxyhemoglobin samples at different pH levels. Subtraction of the two scans provides clear evidence for a difference indicating that pH alone was responsible for the effect. Figure 13 is for Horse Hb. Near UV resonance Raman spectra of hemoglobin are shown at pH of 8 (scan 1) and 6 (scan 2) with a subsequent subtraction scan (scan 3) demonstrating the likelihood of pH sensitive changes in the spectra.

[0072] Another important finding according to the present invention is that at this same near-UV wavelength, NADH demonstrates significant fluorescence. The present inventors have observed significant fluorescence from tissue excited in the near-UV range (406.7 nm) using a portable spectrometer. Exciting tissue in the near-UV range (406.7 nm) according to the invention provides better resolution than traditional filtering in which unique excitation light sources and detection filters are used for the conventional set-up relying on NADH fluorescing (emitting light at 460 nm) when excited at a wavelength of 360 nm (near-UV).

[0073] Based on the importance of NADH in cellular oxygen utilization (as set forth above), from this aspect of the invention may be determined the point of tissue dysoxia or critical DO_2 (ischemia) prior to being able to note increases in systemic lactate. Although NADH also exists in the cytoplasm, it does so in insignificant amounts compared to those produced within the mitochondria during states of dysoxia. In conjunction with the tissue saturation experiments above, NADH fluorescence from quadriceps (Figures 14-19), tongue (Figure 20) and additionally liver (Figure 21) was obtained during graded hemorrhage.

[0074] Figure 14 is a baseline, and Figure 15 reports spectra after 5 mls bleeding for the same quadriceps

muscle. Significant NADH fluorescence is observed after 5 ml hemorrhage. Although the animal has relatively normal vital signs, fluorescence indicated that critical dysoxia has occurred. (Figure 15.) At 7.5 mls of bleeding (Figure 16) for the same muscle, increasing fluorescence indicates additional ischemia. At 9 mls of bleeding (Figure 17), even more fluorescence is observed, indicating the ability to grade severity in real time. At 12 mls of bleeding (Figure 18), the animal is almost terminal.

[0075] In the experiment in which blood pressure was monitored, significant fluorescence occurred prior to and after changes in vital signs. With equipment according to the present invention, tissue oxygen saturation and NADH fluorescence may be simultaneously obtained. Again, the depth of tissue interrogated is the same as that for tissue oxygen saturation. Thus may be determined the point at which critical oxygen delivery (dysoxia) occurs. Significant warning prior to this time will occur as reflected in reductions in tissue oxygen saturation.

[0076] Continued NADH fluorescence after restoration of oxygen delivery indicates ongoing dysoxia despite the potential for normalization of tissue oxygen saturation. The normal heart shows little or no NADH surface fluorescence. The beginning of ischemia and maximum ischemia may be observed. Continued patch fluorescence may be observed after reperfusion. Thus, NADH fluorescence data has value in monitoring tissue even after perfusion has been restored.

[0077] Because of the kinetics of lactate production and transport, it is very likely dysoxia detected by NADH accumulation and fluorescence will occur significantly earlier than with detection of regional or systemic lactate or even CO_2 . In short, the combined use of near-UV resonance Raman spectroscopy and near-UV NADH, fluorescence serve as an exquisitely sensitive early warning system for pending defects in tissue perfusion and in ensuring the completeness of resuscitation.

[0078] Other heme proteins, which have importance in ischemia-reperfusion diseases can be detected using resonance Raman spectroscopy at the same near-UV wavelength (406.7 nm). These include myeloperoxidase, which is an injurious enzyme produced and released by neutrophils, and xanthine oxidase, which is converted from xanthine dehydrogenase after reperfusion of ischemia and is responsible for the production of free radicals. Hayward, R., Lefer, A.M., "Time course of endothelial-neutrophil interaction in splanchnic artery ischemia-reperfusion," *Am J Physiol* 275 (6 Pt 2): H2080-6 (1998); Tan, S., Yokoyama, Y., Dickens, E., Cash, T.G., Freeman, B.A., Parks, D.A., "Xanthine oxidase activity in the circulation of rats following hemorrhagic shock," *Free Radic Biol Med*, 15(4):407-14 (1993).

[0079] A resonance Raman spectroscopy spectrum taken for a human is shown for myeloperoxidase (Figure 23). The ability to detect myeloperoxidase would be helpful in evaluation of wounds and systemic reperfusion injury and sepsis.

[0080] Another group of potentially useful markers of

preclinical shock secondary to hypovolemia are endogenously produced catecholamines such as epinephrine and norepinephrine and the vasoactive peptides such as angiotensin, vasopressin, endothelin, and adrenomedullin, all of which are known to be significantly elevated in the setting of hypovolemia and other shock states. Jak-schik, B.A., Marshall, G.R., Kourik, J.L. Needleman, P., "profile of circulating vasoactive substances in hemorrhagic shock and their pharmacologic manipulation," *J Clin Invest*, 54(4):842-52 (1974); Lanza, V., Palazzadriano, M., Scardulla, C., Mercadante, S., Valdes, L., Bellanca, G., "Hemodynamics, prolactin and catecholamine levels during hemorrhagic shock in dogs pretreated with ap prolactin inhibitor, (bromocriptine)," *Pharmacol Res Commun.*, 19(4):307-18 (1987); Yilmazlar, A., Yilmazlar, T., Ozcan, B., Kutlay, O., "Vasopressin, renin, and adrenocorticotrophic hormone levels during the resuscitation of hemorrhagic shock in dogs," *J Emerg Med*, 18(4):405-8 (2000); Kitajima, T., Tani, K., Yamaguchi, T., Kubota, Y., Okuhira, M., Mizuno, T., et al., "Role of endogenous endothelin in gastric mucosal injury induced by hemorrhagic shock in rats," *Digestion*, 56(2):111-6 (1995); Fujioka, S., Ono, Y., Kangawa, K., Okada, K., "Plasma concentration of adrenomedullin is increased in hemorrhagic shock in dogs," *Anesth Analg*, 88(2):326-8 (1999); Lindner, K.H., Strohmenger, H.U., Ensinger, H., Hetzel, W.D., Ahnefeld, F.W., Georgieff, M., "Stress hormone response during and after cardiopulmonary resuscitation," *Anesthesiology*, 77(4):662-8 (1992); Lindner, K.H., Haak, T., Keller, A., Bothner, U., Lurie, K.G., "Release of endogenous vasopressors during and after cardiopulmonary resuscitation," *Heart*, 75(2):145-50 (1996).

[0081] Raman spectra of vasopressin in the UV spectrum at 350 nm is shown at Figure 24, and for norepinephrine in the same UV spectrum at Figure 25. Ability to detect, quantitate, and trend these markers can be used with regard to evaluating and treating numerous disease states such as shock, congestive heart failure, pain states, burns, etc. These and other similar mediators can be detected and quantitated using resonance Raman spectroscopy. Schulze, H.G., Greek, L.S., Barbosa, C.J., Blades, M.W., Gorzalka, B.B., Turner, R.F., "Measurement of some small-molecule and peptide neurotransmitters in-vitro using a fiber-optic probe with pulsed ultraviolet resonance Raman spectroscopy," *J. Neurosci Methods*, 92(1-2):15-24 (1999).

[0082] The ability to detect dysoxia and ensure its resolution at the earliest possible time has great value for the triage of ill or injured patients. Therapy and resources can be better allocated and victim's progress better monitored, reducing the incidence of under-resuscitation as well as provision of needless resuscitation. Based on the biphasic relationship of oxygen delivery and consumption of a tissue, the present invention measures hemoglobin saturation in conjunction with NADH as a reflection of the oxygen dependent bioenergetic state of the cell.

[0083] Based on experimental results herein, it is seen that near UV excitation can be exploited to simultane-

ously perform Raman resonance spectroscopy of oxy and deoxyhemoglobin, and surface-subsurface fluorescence of NADH. Also, UV and NIR RRS have been obtained from a number of compounds (including high-energy phosphates PCr, ATP and ADP, NAD, NADH, the glycolytic metabolites pyruvate and lactate, and the excitatory amino acid glutamate) in solid and aqueous states.

[0084] From the experimental data set forth above, it may be seen that with the use of combined UV, near UV and NIR Raman spectroscopy, identification and monitoring of a large number of useful target compounds may be accomplished, for detecting and monitoring the presence and severity of hemorrhagic shock and development or resolution of its sequelae such as sepsis. The present inventors have successfully shown that the various compounds discussed above are amenable to detection by UV, near UV and NIR Raman.

[0085] It has recently been demonstrated that NIR absorption spectroscopy can be used to determine tissue pH by examining shifts in the broad bands of hemoglobin. This is based on the known fact that histidine residues of hemoglobin are pH sensitive. NIR absorption spectroscopy is being examined to determine hematocrit in a similar manner. Because pH sensitive shift is observed in all of the oxy and deoxy bands of the resonance Raman spectra and hemoglobin concentration differences in the heights of the bands, it may be concluded (by such techniques as partial least squares) that tissue pH and hematocrit/hemoglobin levels may be determined using resonance Raman spectroscopy.

[0086] Of recent importance has been the development of the concept of cytopathic hypoxia as an explanation for the oxygen transport abnormalities, which exist during sepsis. This theory suggests that such inflammatory compounds as tumor necrosis factor and endotoxin damage mitochondria. This damage prevents the mitochondria from utilizing oxygen. Data for studies using NIR absorption spectroscopy appear to support this theory. The combination of near-UV resonance Raman spectroscopy of hemoglobin tissue saturation and NADH fluorescence would help detect this if it existed. In such a setting, tissue saturation would be normal or elevated but NADH fluorescence would be significant. This entity of cytopathic hypoxia may be one factor which confounds the use of other monitoring modalities such as splanchnic tonometry and monitoring of mixed venous oxygen saturation.

[0087] Methods and devices according to the invention may be used in various manners, such as to exploit shifts in the spectra of molecules such as hemoglobin and myoglobin to calculate blood and tissue pH as well as detect and determine the actual hemoglobin and myoglobin oxygen saturation. Spectroscopy equipment may be coupled with probe(s) and sensor(s) to construct a device to interrogate the perfusion and metabolic status of individual tissues as well as the organism as a whole, advantageously in a noninvasive or minimally invasive manner.

For instance, the invention provides a minimally invasive fiber optic probe or arrays of probes (each probe less than 0.2 mm) which are insertible into a muscle or other tissue bed with a small gauge needle. Resonance Raman spectroscopy in the deep ultraviolet wavelength (less than 270 nm) is used for interstitial fluid analysis (micron level penetration), while longer UV or near UV wavelengths are used for cellular analysis, due to slightly longer wavelengths that could penetrate to levels near 1 mm. Both the deep and near UV wavelengths also may be used with a probe placed on the oral cheek mucosal epithelium. NIR Raman spectroscopy may be used with non-invasive optical fibers placed on the skin or within tissue beds. Surface Raman spectroscopy is used to interrogate standards of detected substances for quantification.

[0088] When spectroscopy according to the present invention operates at multiple wavelengths, additional valuable metabolic and humoral targets may be selected for identification and tracking. The one-dimensionality problem of conventional emergency medical measurement technology is avoided. As has been mentioned above, for conventional IR or NIR technology, problems arise because water strongly absorbs IR radiation, and thus presents strong interference to the use of IR absorption spectroscopy in the clinical setting. The present invention is not burdened with such problems because water is a rather weak Raman scatterer. Raman spectroscopy can be used to provide the same vibrational information as the more common NIR absorption spectroscopy with no significant interference from water. In addition, the use of Raman allows one to take advantage of the resonance Raman enhancement effect, plus polarization effects, neither of which have parallels in IR absorption spectroscopy. Thus, a principal advantage of the invention is that Raman spectroscopy does not suffer the same problems with water as normal IR spectroscopy, and, additionally, Raman spectroscopy is not limited to a single wavelength but can use a variety of wavelengths to interrogate molecules of interest at different tissue depths (skin, muscle, etc). Normal and transmission spectroscopy may be used to complement Raman spectroscopy for calibration, determination of tissue depth, and other enhancement of obtained information. Issues such as weakness of signal, potential tissue damage, and interference from fluorescence can be managed.

[0089] The ability to target multiple compounds in real-time provided by the present invention is a substantial advantage for detection and treatment of certain disease states and shock states. For example, the ability to monitor levels of catecholamines and vasoactive peptides may prove to be more sensitive of early shock states or states of intractable shock. Elevations of these compounds may indicate the severity of such states as acute sickle cell pain crises. Thus, resuscitation and treatment of such states using markers such as catecholamines or vasoactive peptides as endpoints may provide a relative-

ly objective means to determine treatment efficacy.

[0090] Another example of methods according to the invention are uses in conjunction with maneuvers such as simple muscle contraction or use of a tourniquet. Monitoring rates of high-energy phosphoate degradation and regeneration or intermediary compound ratios such as lactate-pyruvate or NAD-NADH in disease states may provide relatively sensitive information concerning the state of the microvasculature.

[0091] Outpatient applications also are provided. Depending on the sensitivity of the device, the technology of the invention may be used in the outpatient setting for determination of various target compounds such as hemoglobin. The device may be used to diagnose certain precancerous or cancerous lesions (such as skin melanoma, etc.) in vivo. Point of care or continuous real-time tissue monitoring is provided with the inventive method and its components.

[0092] Because probes may be relatively small, patients may be continuously interrogated for the appearance of abnormal tissue markers specific for a suspected disease state. Examples of such markers are cardiac biomarkers such as troponin or myocardial fatty acid binding protein, GI markers of ischemia such as D-lactate and intestinal fatty acid-binding protein, and cerebral markers such as neuronal enolase.

[0093] Combining resonance Raman spectroscopy of tissue hemoglobin saturation and NADH fluorescence of the same region provides for detecting ultra-early perfusion deficits and determining adequacy of resuscitation. The present invention provides at least the following advantages: 1) little or no tissue contact (point and click technology); 2) rapid acquisition (such as acquisition times on the order of 1 second); 3) data (tissue saturation and point of critical oxygen delivery) that is not confounded by hypo or hypercarbia; 4) differentiation of sepsis (cytopathic hypoxia) from flow dependent dysoxia; 5) true data from mucosa (oral or other points in the GI or GU tract); 6) pH and hemoglobin (on a par with NIR absorption technology); and 7) other important markers of tissue injury such as myeloperoxidase, xanthine oxidase, vasoactive substances, etc.

[0094] The present invention may be applied to known markers and also to markers as newly reported, because of the nature of resonance Raman spectroscopy. As a new marker (such as procalcitonin, etc.) is reported, the present invention provides for its study by resonance Raman spectroscopy.

[0095] The inventive methods and devices may be used for evaluation of any general shock state (trauma, cardiogenic, septic). Applications include hypoxic-hypoxia, hemorrhagic shock, cardiogenic shock, septic shock, and isolated organ ischemia (including wounds).

[0096] The inventive methods and devices may be used to evaluate the oxygen status of any organ during surgery (e.g., the heart during cardiopulmonary bypass surgery, the brain during neurosurgery, and various organs during transplant); to evaluate donor organs prior

to transplant; to include in devices such as pacemakers to interrogate areas of myocardium at risk of injury; to evaluate a patient with congestive heart failure (such as at the hospital, office, home, etc.) to determine symptom etiology (such as fluid overload versus deterioration in heart function); to determine if a patient requires blood transfusion; to care for wounds.

[0097] The invention fills the current void of no universally accepted way of determining when a patient requires blood transfusion. Because each patient may have a different requirement based on past medical history and the current event, the invention is highly advantageous in allowing repetitive noninvasive measures of a sensitive tissue.

[0098] The invention benefits wound care (chronic and acute), by providing information about the oxygenation status of wounds. Care of chronic wounds is improved by the present invention providing the ability to determine oxygenation status of wounds. The use of near-UV resonance Raman spectroscopy determines tissue oxygen saturation at multiple points within the wound (within seconds) with tissue contact being unnecessary. In conjunction with the Raman spectroscopy, NADH fluorescence may be used to determine if the wound is becoming necrotic. The wound may be sampled for injurious substances interfering with wound-healing, such as myeloperoxidase.

[0099] The methods and products of the present invention have civilian and military uses. Using UV, near UV or NIR Raman spectroscopy according to the present invention provides for real-time monitoring of a broad range of valuable markers. An operator (such as a combat medic) may use a portable probe according to the invention, with the probe being pluggable into a hand held UV-NIR Raman spectrometer (such as a device the size of a hand held palm PC device). The Raman spectrometer before use on a patient may be programmed to perform UV, near UV and NIR Raman spectroscopy for the markers of interest and to report them in a manner readily interpretable to indicate the presence and degree of shock. In the case of a combat medic using such a portable probe that plugs into a Raman spectrometer, the medic may then institute or order appropriate therapy while instrumenting and interrogating the next soldier using the same hand held spectrometer. In this manner, the medic can move back and forth between patients to determine the effect of the instituted therapy and to make triage decisions. When a marker or a combination of markers indicates intractable shock, an appropriate triage decision may be more readily reached than without the measurement information according to the present invention, and thus other more salvageable patients may be more likely to have access to resources and have increased chances of survival.

[0100] Data collected according to the present invention may be stored and/or transmitted. For example, data collected by a hand held device (such as a combat medic device) may be transmitted to a remote data bank. As

the patient is transported, medics and physicians taking over care may use their own devices (which may be hand held devices) to hook into the previously implanted fiber optic probe. Data measured during a new hook-up may be compared to data previously collected on the patient (such as data transmitted earlier from the field). New or additional probes optionally may be placed during surgery. The same devices, once placed, may be maintained in place and used to continuously interrogate tissue to monitor the efficacy of ongoing resuscitative efforts and to detect the development of post-hemorrhagic shock and surgical sequelae such as early sepsis. Multiple tissues beds may be interrogated, especially by using small, disposable probes.

[0101] While an operator has been referred to hereinabove, it will be appreciated that the inventive methods do not necessarily require a human operator, and that the invention may include partly and entirely automatic, such as computer-assisted, methods and devices. Such automatic and semi-automatic methods and devices may include those in which, upon measurement of ratios or amounts in a certain predetermined adverse range, preformulated reactive therapies are applied. The invention provides for an optional computer system, such as a computer system comprising a database of stored baseline Raman spectroscopy and/or fluorescence spectroscopy profiles and a means to store patient Raman spectroscopy and/or fluorescence spectroscopy profiles. Such a computer system preferably includes a computing system for comparing patient profiles to baseline profiles.

[0102] While the invention has been described in terms of its preferred embodiments, those skilled in the art will recognize that the invention can be practiced with modification within the scope of the appended claims.

Claims

1. A biological material analysis method, comprising:
 - interrogating a biological material selected from the group consisting of tissue or bodily fluid, including urine, saliva, wound exudates, vitreous humor, aqueous humor, tissue exudates, gastric contents, and fecal matter with Raman spectroscopy and fluorescence spectroscopy to obtain spectroscopy results, and analyzing the obtained spectroscopy results for at least one mediator or marker associated with a shock state.
2. The method of claim 1 including determining the presence and/or proportions and preferably the relative or absolute concentration of at least one mediator or marker.
3. The method of claim 1, including intermittently or continuously interrogating the tissue of a patient.

4. The method of claim 3, including monitoring for appearance of one or more tissue markers specific for a specific disease state.
5. The method of claim 1, including determining tissue viability.
6. The method of claim 1, whereby the marker is associated with the progression or resolution of shock states or abnormalities associated with a shock state.
7. The method of claim 1, whereby the marker is associated with the progression or resolution of tissue ischemia, tissue injury, tissue inflammation or tissue immune dysfunction.
8. The method of claim 1, wherein the tissue interrogating is non-invasive.
9. The method of claim 1, wherein the tissue is in vivo and in situ.
10. The method of claim 1, wherein the tissue has been removed from a patient before the tissue interrogation.
11. The method of claim 1, including measuring tissue hemoglobin oxygen saturation including amount of oxyhemoglobin and deoxyhemoglobin by Raman spectroscopy.
12. The method of claim 1, including measuring NADH presence and/or accumulation by fluorescence spectroscopy.
13. The method of claim 1, including determining whether the tissue has insufficient oxygen delivery to meet metabolic demands of the tissue while simultaneously determining whether mitochondrial dysfunction or injury exists.
14. The method of claim 1, including measuring myoglobin oxygenation saturation.
15. The method of claim 1, including determining cytochrome oxidase redox status.
16. The method of claim 1 or 11, including determining absolute concentration of hemoglobin in the tissue.
17. The method of claim 1 or 11, including determining pH of the tissue.
18. The method of claim 1, wherein the obtained spectroscopy results are for at least one mediator associated with a shock state selected from the group consisting of tissue injury or tissue ischemia, inflammation or immune dysfunction, and at least one marker of tissue perfusion or injury.
19. The method of claim 18, wherein the marker may be within intracellular, interstitial or intravascular space or within exhaled air from a patient.
20. The method of claim 18, wherein the marker is selected from the group consisting of lactate, pyruvate, ATP, Pcr, AMP, ADP, Pi, NAD, NADH, albumin, endotoxin, exotoxin, microbes, cytokines-chemokines, procalcitonin, hormones, myeloperoxidase, elastase, xanthine oxidase, xanthine dehydrogenase, fatty acid binding proteins, catecholamines and vasoactive peptides.
21. The method of claim 18, wherein the marker or mediator is a metabolic or pro or anti-inflammatory marker or mediator.
22. The method of claim 6 or 7, comprising:
- (A) for a target molecule population, taking a sample Raman spectroscopy, and/or fluorescence spectroscopy, profile for a patient;
- (B) comparing the sample spectroscopy profile with a pre-established Raman spectroscopy and/or fluorescence spectroscopy profile for the target molecule population under baseline conditions.
23. The method of claim 22, wherein the target molecule population comprises oxygenated haemoglobin, deoxygenated haemoglobin and/or NADH.
24. The method of claim 22, wherein the profiles are of relative amounts of NAD/NADH; lactate/pyruvate; Pcr-ATP; ATP-ADP; Pcr-Pi; oxidized cytochrome oxidase to reduced cytochrome oxidase, and/or oxyhemoglobin with deoxyhemoglobin.
25. The method of claim 22, including taking the profiles by Raman spectroscopy with signal enhancement at a resonant frequency for a target molecule of the target molecule population.
26. The method of claim 22, including operating an electromagnetic radiation generator at a range of selectable wavelengths from about 270 nm to about 20,000 nm.
27. The method of claim 22, including monitoring a specific tissue bed in the patient, preferably a brain, heart, lung, liver, eye, intestine, stomach, pancreas, kidney, bladder, urethra, nailbed, cervix, uterus, oropharynx, nasopharynx, esophagus or blood.
28. The method of claim 27, including detecting exhaled

- markers or mediators of organ injury, preferably a lung injury.
29. The method of claim 28, wherein a detector is placed at the airway of the patient. 5
30. The method of claim 28, wherein the exhaled markers or mediators are isoprostanes and/or myeloperoxidase. 10
31. The method of claim 22, including calculating pH of blood and/or tissue. 15
32. The method of claim 22, including analysis of interstitial fluid. 20
33. The method of claim 1, including resonance Raman spectroscopy at 390 to 420 nm wavelength. 25
34. The method of claim 33, wherein the sample profile is taken from a tissue or a space out of the body. 30
35. The method of claim 22, including cellular analysis. 35
36. The method of claim 22, including simultaneously performing fluorescence spectroscopy probing of NADH while performing Raman spectroscopy. 40
37. The method of claim 22, wherein spectroscopy is performed for multiple wavelengths. 45
38. The method of claim 22, including continuously interrogating the patient for appearance of abnormal tissue markers specific for a suspected disease state. 50
39. The method of claim 22, wherein the markers are cardiac biomarkers, GI markers, cerebral markers, skin markers, lung markers, blood markers, and/or eye markers. 55
40. A spectroscopy comparative profile obtained by a method according to one of claims 22 to 37 and comprising:
 a pre-established Raman spectroscopy and fluorescence spectroscopy profile for a target molecule population under baseline conditions, and a sample Raman spectroscopy and fluorescence spectroscopy profile for the target molecule population.
41. The comparative profile of claim 40, including a pre-established fluorescence spectroscopy profile for NADH under baseline conditions and a sample fluorescence profile for NADH.
42. A computer system comprising:
 a database of stored baseline Raman spectroscopy and a database of stored fluorescence spectroscopy profiles and
 a means to store patient Raman spectroscopy and fluorescence spectroscopy profiles including a computing system for comparing patient profiles to baseline profiles with regard to a shock state.
43. A medical measurement device for performing the method according to one of claims 1 to 41, comprising:
 a computer system of claim 42 and Raman spectrometer and a fluorescence spectrometer electrically connectable with a probe of a biological material, preferably a tissue or a bodily fluid.

Patentansprüche

1. Verfahren zur Analyse von biologischem Material umfassend:

Untersuchen eines biologischen Materials ausgewählt aus der Gruppe bestehend aus Gewebe oder Körperflüssigkeit, einschließlich Harn, Speichel, Wundexudate, Glaskörperflüssigkeit, Kammerwasser, Gewebeexudate, Mageninhalt, Fäkalmaterialien mit Raman-Spektroskopie und Fluoreszenzspektroskopie, um Spektroskopieergebnisse zu erhalten, und Analysieren der erhaltenen Spektroskopieergebnisse auf mindestens einen Mediator oder Marker, der mit einem Schockzustand assoziiert ist.

2. Verfahren nach Anspruch 1, einschließlich die Bestimmung des Vorhandenseins und/oder der Anteile und, bevorzugt, der relativen oder absoluten Konzentration von mindestens einem Mediator oder Marker.

3. Verfahren nach Anspruch 1, einschließlich periodische oder kontinuierliche Untersuchungen des Gewebes eines Patienten.

4. Verfahren nach Anspruch 3, einschließlich das Überwachen des Auftretens von einem oder mehreren Gewebemarkern spezifisch für ein spezifisches Erkrankungsstadium.

5. Verfahren nach Anspruch 1, einschließlich die Bestimmung der Gewebeviabilität.

6. Verfahren nach Anspruch 1, wobei der Marker mit dem Fortschreiten oder dem Auflösen der Schockzustände oder der Abnormalitäten mit einem Schockzustand assoziiert ist.

7. Verfahren nach Anspruch 1, wobei der Marker assoziiert ist mit dem Fortschreiten oder dem Auflösen von Gewebeischämie, Gewebeverletzung, Gewebeentzündung oder einer Immunfehlfunktion im Gewebe. 5
8. Verfahren nach Anspruch 1, wobei die Gewebeuntersuchung nicht invasiv ist.
9. Verfahren nach Anspruch 1, wobei das Gewebe in vivo oder in-situ ist. 10
10. Verfahren nach Anspruch 1, wobei das Gewebe dem Patienten vor der Untersuchung des Gewebes entnommen wurde. 15
11. Verfahren nach Anspruch 1, einschließend das Messen der Hämoglobinsauerstoffsättigung im Gewebe einschließlich der Menge an Oxyhämoglobin und Deoxyhämoglobin durch Raman-Spektroskopie. 20
12. Verfahren nach Anspruch 1, einschließend das Messen des Vorhandenseins von NADH und/oder der Anreicherung hiervon durch Fluoreszenzspektroskopie. 25
13. Verfahren nach Anspruch 1, einschließend die Bestimmung, ob das Gewebe eine unzureichende Sauerstoffzufuhr aufweist, um die Anforderungen des Stoffwechsel im Gewebe zu erfüllen, während simultan bestimmt wird, ob eine mitochondriale Disfunktion oder Verletzung vorliegt. 30
14. Verfahren nach Anspruch 1, einschließend das Messen der Myoglobinsauerstoffsättigung. 35
15. Verfahren nach Anspruch 1, einschließend das Bestimmen des Cytochromoxidase-Redoxstatus.
16. Verfahren nach Anspruch 1 oder 11, einschließend das Bestimmen der absoluten Konzentration von Hämoglobin im Gewebe. 40
17. Verfahren nach Anspruch 1 oder 11, einschließend die Bestimmung des pH-Wertes des Gewebes. 45
18. Verfahren nach Anspruch 1, wobei Spektroskopieergebnisse für mindestens einen Mediator assoziiert mit einem Schockzustand ausgewählt aus der Gruppe bestehend aus Gewebeverletzung oder Gewebeischämie, Entzündung und Immundisfunktion und mindestens einem Marker für eine Gewebepfusion oder Verletzung erhalten werden. 50
19. Verfahren nach Anspruch 18, wobei der Marker sich im intrazellulären, interstitialen oder intravaskulären Bereich oder in der ausgeatmeten Luft eines Patienten befinden kann. 55
20. Verfahren nach Anspruch 18, wobei der Marker ausgewählt ist aus der Gruppe bestehend aus Lactat, Pyruvat, ATP, Pcr, AMP, ADP, Pi, NAD, NADH, Albumin, Endotoxin, Exotoxin, Mikroben, Zytokine-Chemokine, Procalcitonin, Hormone, Myeloperoxidase, Elastase, Xanthinoxidase, Xanthindehydrogenase, fettsäurebindende Proteine, Catecholamine und vasoaktive Peptide ist.
21. Verfahren nach Anspruch 18, wobei der Marker oder Mediator ein Stoffwechsel- oder pro- oder anti-Inflammatorischer Marker oder Mediator ist.
22. Verfahren nach Anspruch 6 oder 7, umfassend: 15
 (A) für eine Population an Zielmolekülen, Aufnahme eines Probenprofils mittels Raman-Spektroskopie und/oder Fluoreszenzspektroskopie für einen Patienten;
 (B) Vergleich des Spektroskopieprofils der Probe mit einem voretablierten Raman-Spektroskopie- und/oder Fluoreszenzspektroskopieprofil für die Population an Zielmolekülen unter Basisbedingungen.
23. Verfahren nach Anspruch 22, wobei die Population an Zielmolekülen, oxygeniertes Hämoglobin, deoxygeniertes Hämoglobin und/oder NADH umfasst.
24. Verfahren nach Anspruch 22, wobei die Profile relative Mengen an NAD/NADH; Lactat/Pyruvat; Pcr-ATP; ATP-ADP; Pcr-Pi; oxidierte Zytochromoxidase zu reduzierte Zytochromoxidase und/oder Oxyhämoglobin mit Deoxyhämoglobin sind. 30
25. Verfahren nach Anspruch 22, einschließend die Aufnahme eines Raman-Spektroskopieprofils mit Signalverstärkung bei einer Resonanzfrequenz für ein Zielmolekül der Population an Zielmolekülen. 35
26. Verfahren nach Anspruch 22, einschließend die Anwendung eines elektromagnetischen Strahlungsgenerators mit einem Bereich an auswählbaren Wellenlängen von ca. 270 nm bis ca. 20000 nm. 40
27. Verfahren nach Anspruch 22, einschließend das Überwachen eines spezifischen Gewebebetts in dem Patienten bevorzugt Hirn, Herz, Lunge, Leber, Auge, Darm, Magen, Pankreas, Niere, Blase, Harnleiter, Nagelbett, Cervix, Uterus, Oropharynx, Nasopharynx, Esopharynx oder Blut. 45
28. Verfahren nach Anspruch 27, einschließend das Bestimmen von ausgeatmeten Markern oder Mediatoren einer Organverletzung, bevorzugt einer Lungenverletzung. 50
29. Verfahren nach Anspruch 28, wobei der Detektor in 55

- den Luftweg des Patienten platziert wird.
30. Verfahren nach Anspruch 28, wobei die ausgeatmeten Marker oder Mediatoren Isoprostan und/oder Myeloperoxidase sind. 5
31. Verfahren nach Anspruch 22, einschließlich des Berechnen des pH-Wertes von Blut und/oder Gewebe.
32. Verfahren nach Anspruch 22, einschließlich die Analyse der interstitiellen Flüssigkeit. 10
33. Verfahren nach Anspruch 1, einschließlich die Resonanz-Raman-Spektroskopie bei 390 bis 420 nm Wellenlänge. 15
34. Verfahren nach Anspruch 33, wobei das Probenprofil von einem Gewebe oder einem Bereich außerhalb des Körpers genommen wird. 20
35. Verfahren nach Anspruch 22, einschließlich die zelluläre Analyse.
36. Verfahren nach Anspruch 22, einschließlich die gleichzeitige Durchführung einer Fluoreszenzspektroskopie für NADH während des Durchführens der Raman-Spektroskopie. 25
37. Verfahren nach Anspruch 22, wobei die Spektroskopie für eine Vielzahl von Wellenlängen durchgeführt wird. 30
38. Verfahren nach Anspruch 22, einschließlich die kontinuierlichen Untersuchung des Patienten auf das Vorhandensein von abnormalen Gewebemarkern spezifisch für einen vermuteten Gesundheitszustand. 35
39. Verfahren nach Anspruch 22, wobei die Marker Herzbiomarker, GI-Marker, cerebrale Marker, Hautmarker, Lungenmarker, Blutmarker und/oder Augenmarker sind. 40
40. Vergleich des Spektroskopieprofils erhalten nach einem Verfahren gemäß einem der Ansprüche 22 bis 37 und umfassend: 45
- ein voretabliertes Profil 1 einer Raman-Spektroskopie und einer Fluoreszenzspektroskopie für eine Population an Zielmolekülen unter Grundbedingungen und eines Profils einer Raman-Spektroskopie und Fluoreszenzspektroskopie einer Probe für die Population an Zielmolekülen. 50
41. Vergleich des Profils nach Anspruch 40, einschließlich ein voretabliertes Profil der Fluoreszenzspektroskopie für NADH unter Grundbedingungen und eines Fluoreszenzprobenprofils für NADH. 55

42. Computersystem umfassend:

eine Datenbank mit gespeicherten Grundprofilen von Raman-Spektroskopien und einer Datenbank von gespeicherten Fluoreszenzspektroskopieprofilen und ein Mittel zum Speichern von Raman-Spektroskopie- und Fluoreszenzspektroskopieprofilen von Patienten einschließlich einem Computersystem zum Vergleich von Patientenprofilen mit Grundprofilen in Bezug auf einen Schockzustand.

43. Eine medizinische Messvorrichtung zur Durchführung des Verfahrens gemäß einem der Ansprüche 1 bis 41 umfassend:

ein Computersystem nach Anspruch 42 und ein Raman-Spektrometer und ein Fluoreszenzspektrometer, elektrisch verbindbar mit einer Probe eines biologischen Materials, bevorzugt eines Gewebes oder einer Körperflüssigkeit.

Revendications

1. Procédé d'analyse de matière biologique, comprenant les étapes suivantes :
- interrogation d'une matière biologique choisie parmi le groupe constitué de tissu ou fluide corporel, incluant l'urine, la salive, des exsudations de plaie, humeur vitreuse, humeur aqueuse, exsudations de tissu, contenus gastriques, et matière fécale par une spectroscopie Raman et spectroscopie de fluorescence pour obtenir des résultats de spectroscopie ; et analyse des résultats de spectroscopie obtenus pour au moins un médiateur ou marqueur associé à un état de choc.
2. Procédé selon la revendication 1, comprenant une détermination de la présence et/ou des proportions et de préférence de la concentration relative ou absolue d'au moins un médiateur ou marqueur.
3. Procédé selon la revendication 1, comprenant une interrogation de façon continue ou intermittente du tissu d'un patient.
4. Procédé selon la revendication 3, comprenant une surveillance de l'apparition d'un ou plusieurs marqueurs de tissu spécifiques à un état pathologique spécifique.
5. Procédé selon la revendication 1, comprenant une détermination de viabilité de tissu.
6. Procédé selon la revendication 1, dans lequel le mar-

- queur est associé à la progression ou la résolution d'états de choc ou des irrégularités associées à un état de choc.
7. Procédé selon la revendication 1, dans lequel le marqueur est associé à la progression ou la résolution d'ischémie tissulaire, lésion tissulaire, inflammation tissulaire ou dysfonctionnement immunitaire de tissu. 5
8. Procédé selon la revendication 1, dans lequel l'interrogation de tissu est non invasive. 10
9. Procédé selon la revendication 1, dans lequel le tissu est *in vivo* et *in situ*. 15
10. Procédé selon la revendication 1, dans lequel le tissu est prélevé à un patient avant l'interrogation du tissu. 20
11. Procédé selon la revendication 1, comprenant une mesure de saturation en oxygène de l'hémoglobine tissulaire comprenant une quantité d'oxyhémoglobine et de désoxyhémoglobine par spectroscopie Raman. 25
12. Procédé selon la revendication 1, comprenant une mesure de la présence et/ou l'accumulation de NADH par spectroscopie de fluorescence. 30
13. Procédé selon la revendication 1, comprenant une étape pour déterminer si le tissu a une alimentation insuffisante en oxygène pour satisfaire la demande métabolique du tissu, et une étape pour déterminer de façon simultanée si un dysfonctionnement mitochondrial ou une lésion existe. 35
14. Procédé selon la revendication 1, comprenant une mesure de la saturation en oxygène de la myoglobine. 40
15. Procédé selon la revendication 1, comprenant une détermination d'un état d'oxydoréduction de cytochrome oxydase. 45
16. Procédé selon la revendication 1 ou 11, comprenant une détermination de la concentration absolue de l'hémoglobine dans les tissus. 50
17. Procédé selon la revendication 1 ou 11, comprenant une détermination du pH du tissu. 55
18. Procédé selon la revendication 1, dans lequel des résultats de spectroscopie obtenus sont pour au moins un médiateur associé à un état de choc choisis dans le groupe constitué de lésion tissulaire ou ischémie tissulaire, dysfonctionnement immunitaire ou inflammatoire, et au moins un marqueur de lésion ou perfusion tissulaire.
19. Procédé selon la revendication 18, dans lequel le marqueur peut être dans un espace intracellulaire, interstitiel ou intravasculaire ou dans l'air expiré d'un patient.
20. Procédé selon la revendication 18, dans lequel le marqueur est choisi dans le groupe composé de lactate, pyruvate, ATP, Pcr, AMP, ADP, Pi, NAD, NADH, albumine, endotoxine, exotoxine, microbes, cytokines-chémokines, procalcitonine, hormones, myéloperoxidase, élastase, xanthine oxydase, la xanthine déshydrogénase, protéines de fixation à l'acide gras, catécholamines et peptides vasoactifs.
21. Procédé selon la revendication 18, dans lequel le marqueur ou médiateur est un marqueur ou un médiateur métabolique ou pro ou anti-inflammatoire.
22. Procédé selon la revendication 6 ou 7, comprenant:
- (A) pour une population de molécule cible, le prélèvement du profil d'un échantillon d'un patient par spectroscopie Raman et/ou spectroscopie de fluorescence,
- (B), comparaison du profil spectroscopique de l'échantillon avec un profil préétabli par spectroscopie Raman et/ou spectroscopie de fluorescence pour la population de molécule cible sous des conditions de la ligne base.
23. Procédé selon la revendication 22, dans lequel la population de molécule cible comprend l'hémoglobine oxygénée, l'hémoglobine désoxygénée et/ou le NADH.
24. Procédé selon la revendication 22, dans lequel les profils sont pour des quantités relatives de NAD / NADH; lactate / pyruvate; Pcr-ATP; ATP-ADP; Pcr-Pi; de la cytochrome oxydase oxydée à la cytochrome oxydase réduite, et/ou de l'oxyhémoglobine avec de la désoxyhémoglobine.
25. Procédé selon la revendication 22, comprenant un prélèvement des profils par spectroscopie Raman avec une mise en valeur de signal à une fréquence de résonance pour une molécule cible de la population de molécule cible.
26. Procédé selon la revendication 22, comprenant la mise en oeuvre d'un générateur de rayonnement électromagnétique à une gamme de longueurs d'ondes au choix d'environ 270 nm à environ 20000nm.
27. Procédé selon la revendication 22, comprenant la surveillance d'un tissu spécifique présent chez le patient, de préférence, un cerveau, coeur, poumon, foie, oeil, intestin, estomac, pancréas, rein, vessie, urètre, lit d'ongle, col de l'utérus, utérus, oropharynx,

- nasopharynx, oesophage ou sang.
28. Procédé selon la revendication 27, comprenant la détection de marqueurs ou médiateurs expirés de lésion d'organe, de préférence une lésion pulmonaire.
29. Procédé selon la revendication 28, dans lequel un détecteur est placé dans les bronches du patient.
30. Procédé selon la revendication 28, dans lequel les marqueurs ou médiateurs expirés sont des isoprostanes et/ou de la myéloperoxidase.
31. Procédé selon la revendication 22, comprenant le calcul du pH de sang et/ou de tissu.
32. Procédé selon la revendication 22, comprenant une analyse du fluide interstitiel.
33. Procédé selon la revendication 1, comprenant une spectroscopie Raman de résonance de 390 à 420 nm de longueur d'onde.
34. Procédé selon la revendication 33, dans lequel le profil d'un échantillon est prélevé à partir d'un tissu ou un espace à l'extérieur du corps.
35. Procédé selon la revendication 22, comprenant une analyse cellulaire.
36. Procédé selon la revendication 22, comprenant une réalisation simultanée d'un sondage de NADH par spectroscopie de fluorescence lors de la réalisation d'une spectroscopie Raman.
37. Procédé selon la revendication 22, dans lequel la spectroscopie est réalisée pour des longueurs d'onde multiples.
38. Procédé selon la revendication 22, comprenant une interrogation de façon continue du patient pour l'apparition de marqueurs de tissu anormaux spécifiques à un état pathologique suspecté.
39. Procédé selon la revendication 22, dans lequel les marqueurs sont des biomarqueurs, des marqueurs GI, des marqueurs cérébraux, des marqueurs de la peau, des marqueurs du poumon, des marqueurs du sang, et/ou des marqueurs de l'oeil.
40. Profil comparatif de spectroscopie obtenu par une méthode selon l'une des revendications 22 à 37 et comprenant :
- un profil pour une population de molécule cible préétabli par spectroscopie Raman et spectroscopie de fluorescence sous des conditions de

la ligne base, et un profil pour une population de molécule cible d'un échantillon par spectroscopie Raman et spectroscopie de fluorescence.

- 5 41. Profil comparatif selon la revendication 40, comprenant un profil par spectroscopie de fluorescence pour NADH sous des conditions de la ligne base et un profil de fluorescence d'un échantillon pour NADH.
- 10 42. Système de traitement comprenant :
- une base de données pour stocker une spectroscopie Raman de la ligne base et une base de données pour stocker des profils de spectroscopie de fluorescence et des moyens pour stocker une spectroscopie du patient et des profils de spectroscopie de fluorescence comprenant un système de traitement pour comparer des profils du patient à des profils de la ligne de base par rapport à un état de choc.
- 15 43. Dispositif de mesure médical pour la mise en oeuvre du procédé selon l'une des revendications 1 à 41, comprenant :
- 20 un système de traitement selon la revendication 42 ; et un spectromètre Raman et un spectromètre de fluorescence électriquement connectable à une sonde d'une matière biologique, de préférence un tissu ou un fluide corporel.
- 25
- 30
- 35
- 40
- 45
- 50
- 55

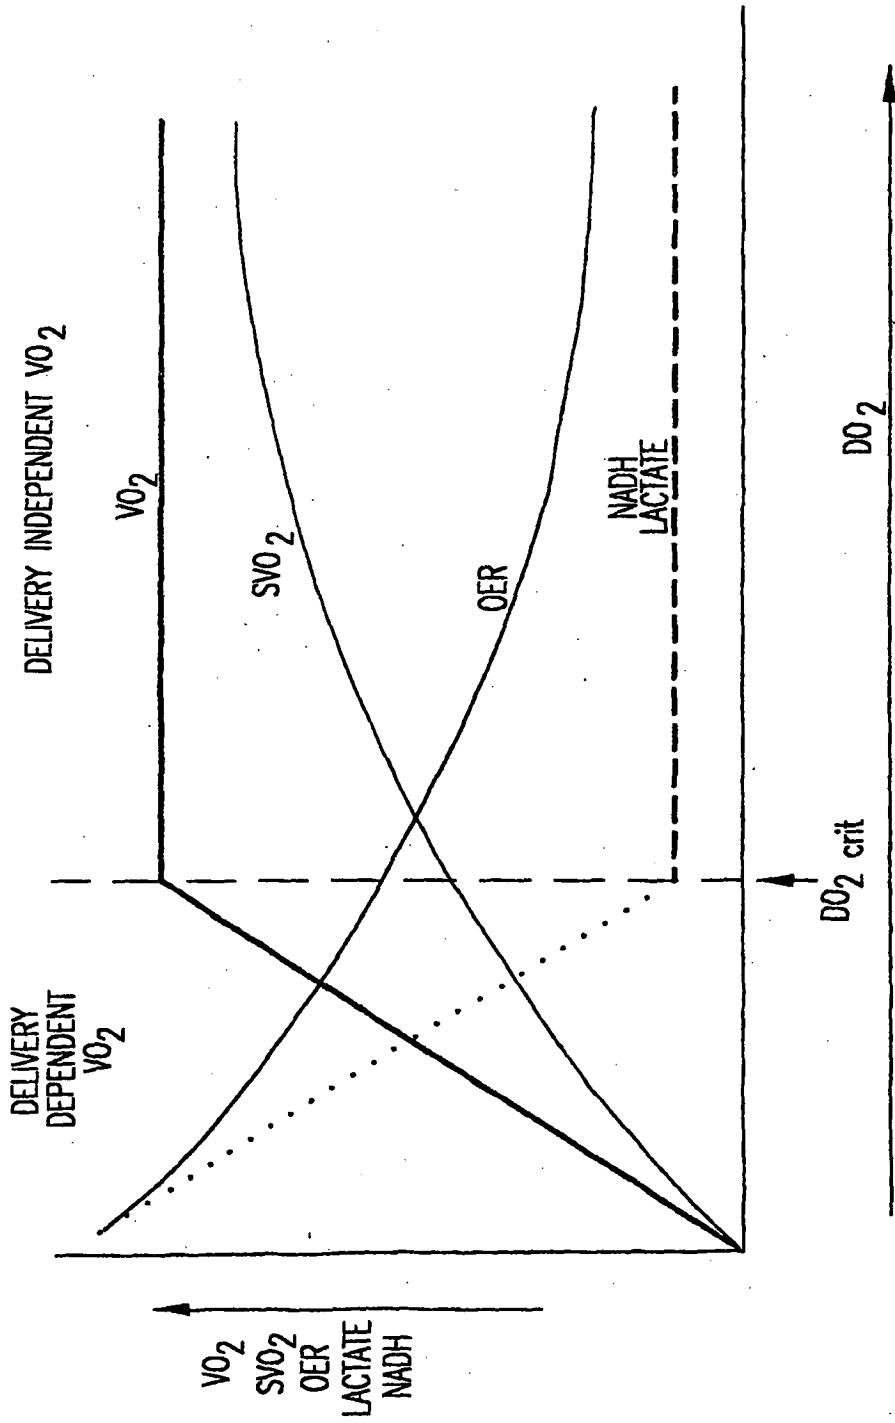


FIG.1

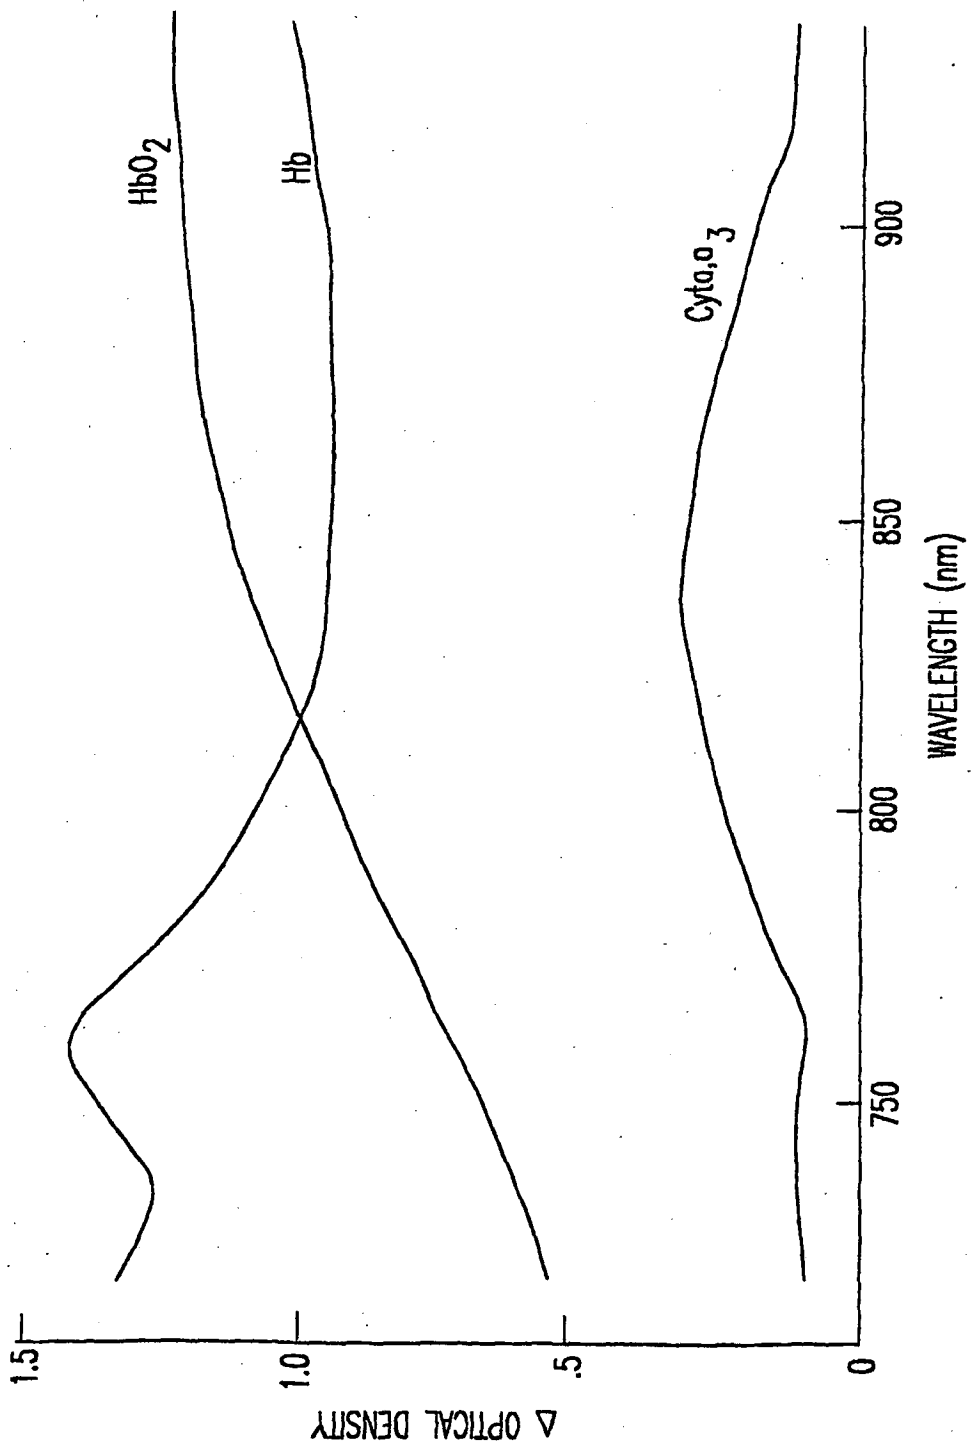


FIG.2

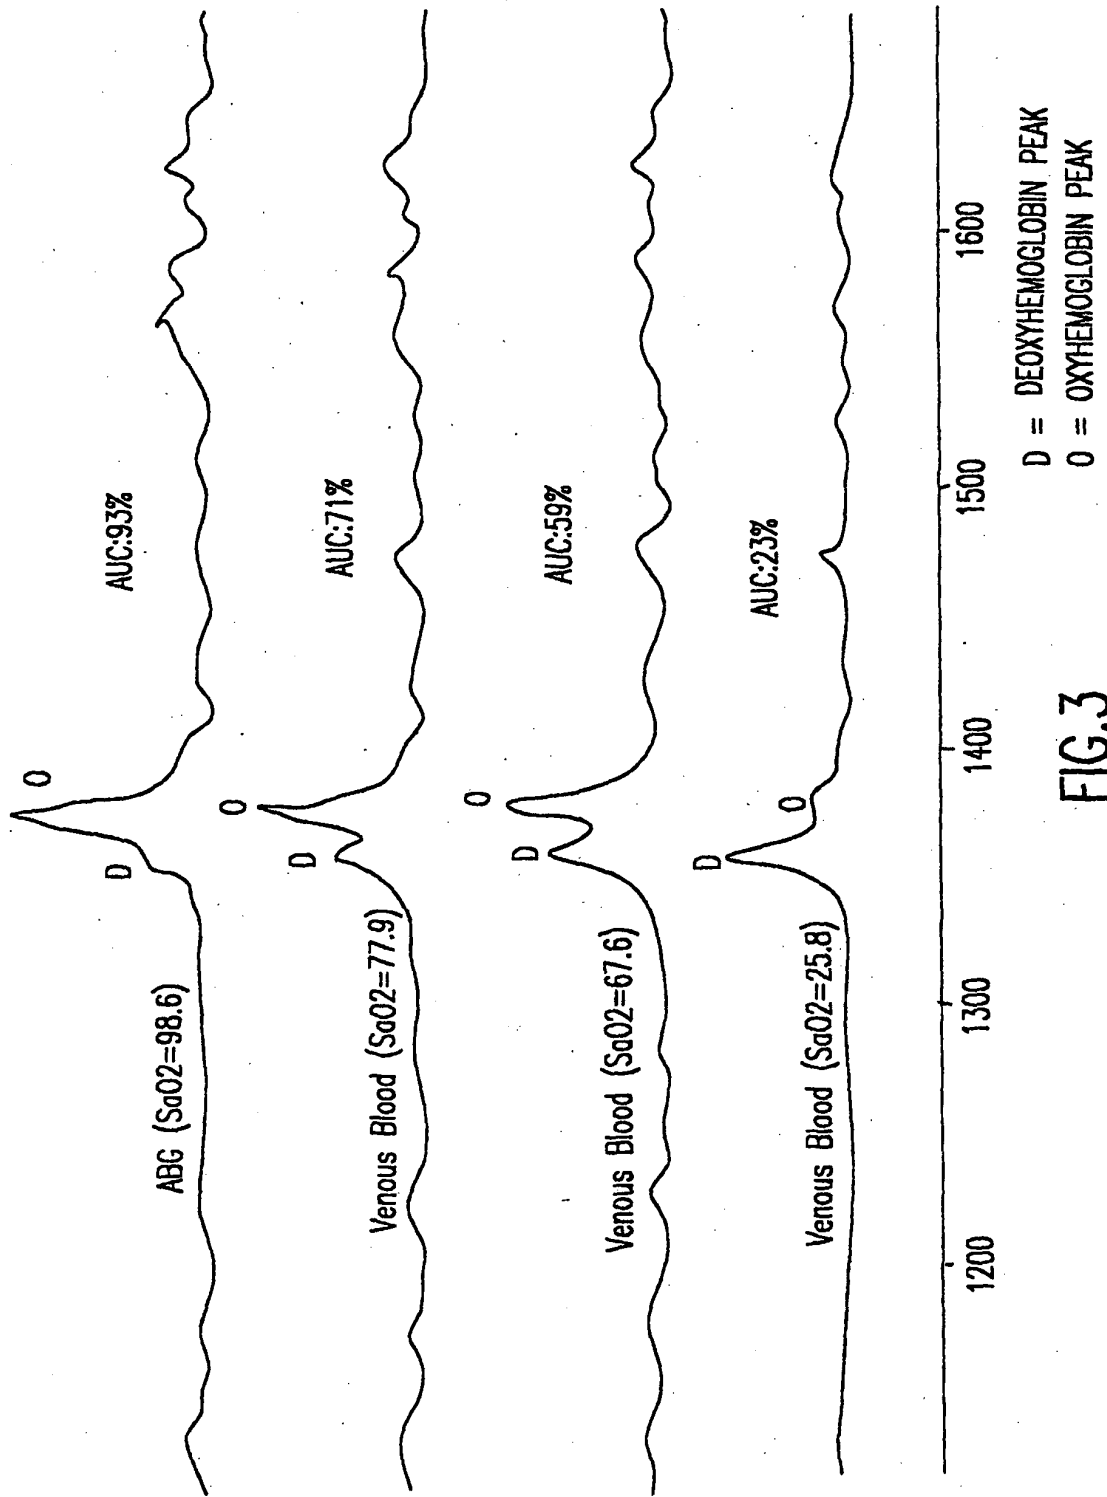


FIG.3

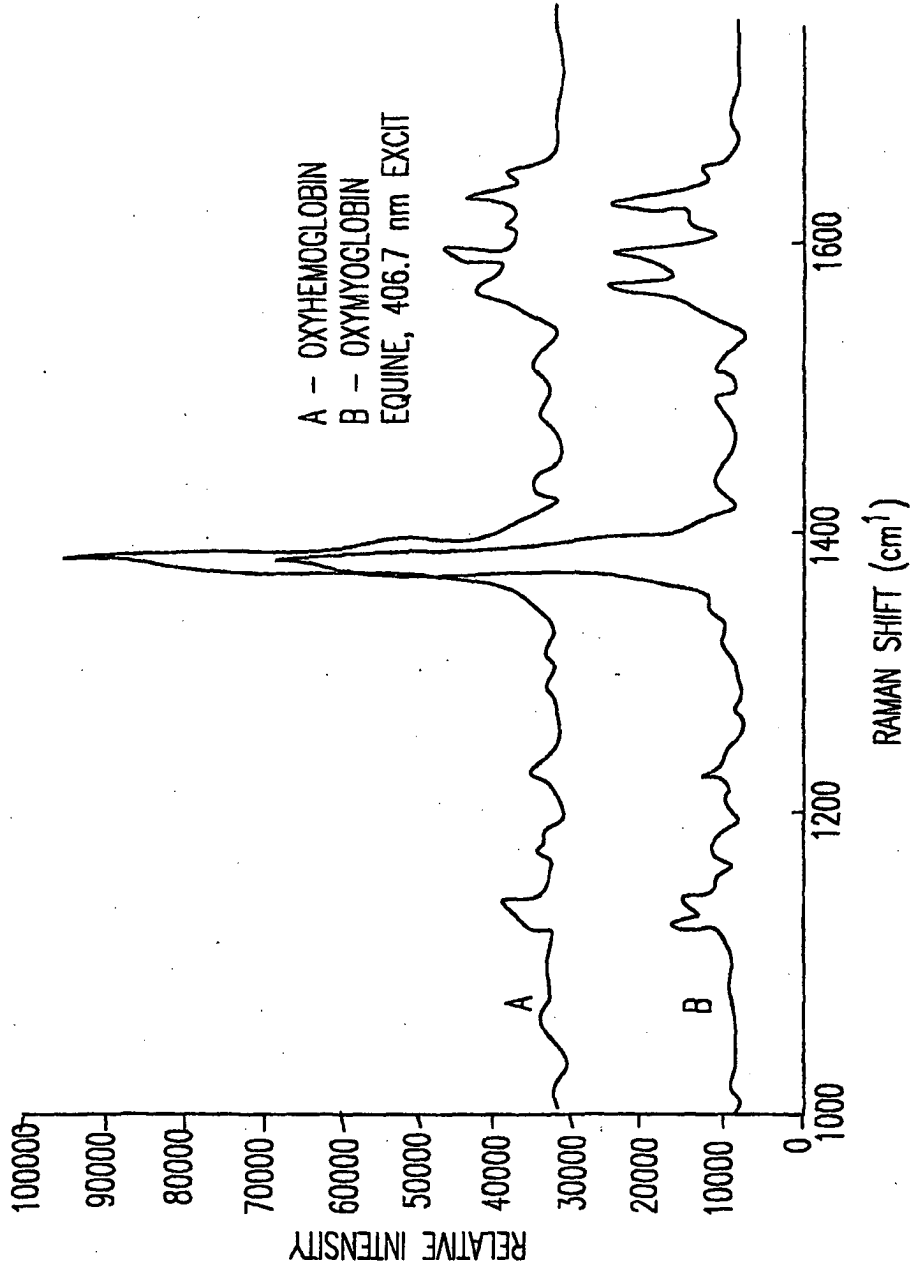


FIG.4

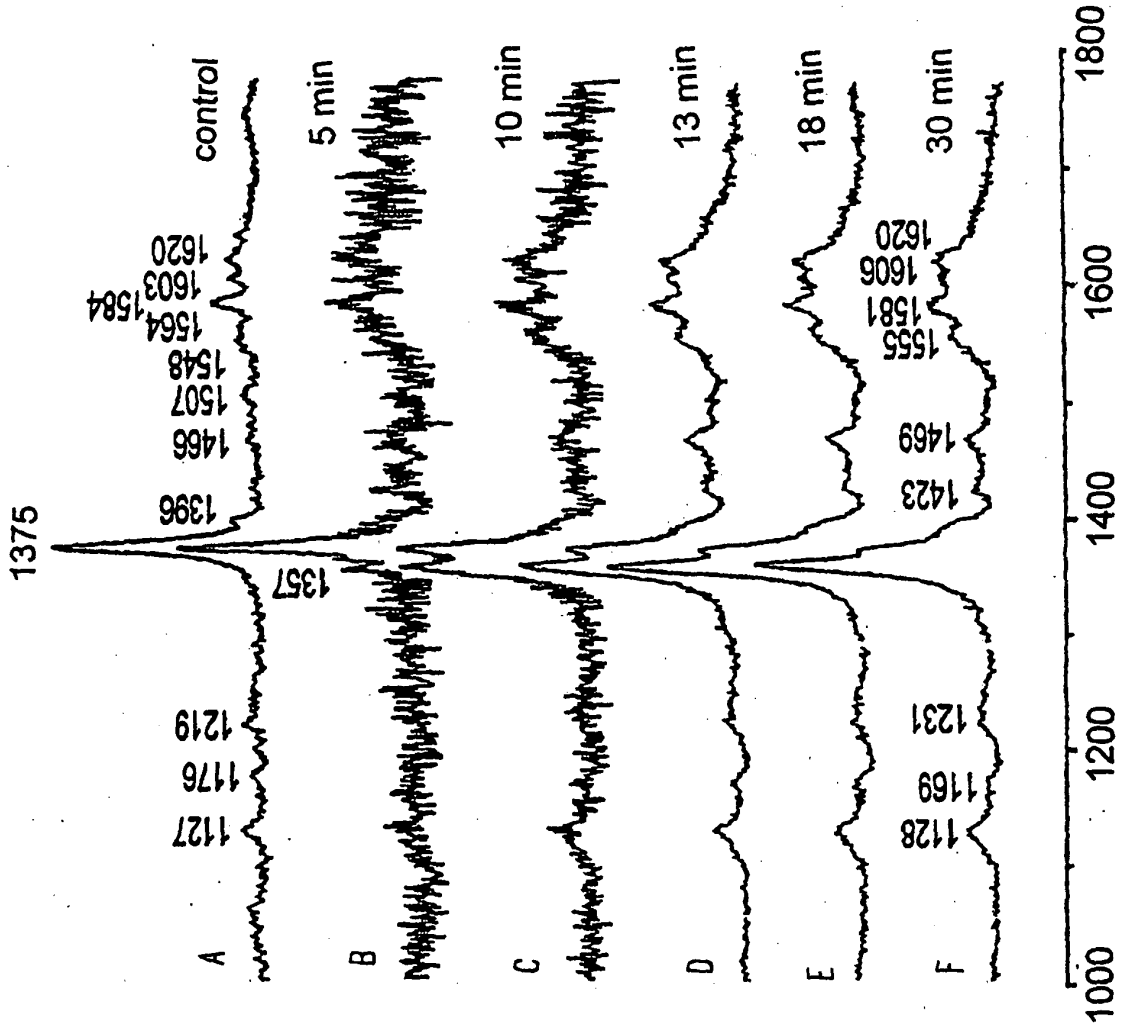


FIG.5

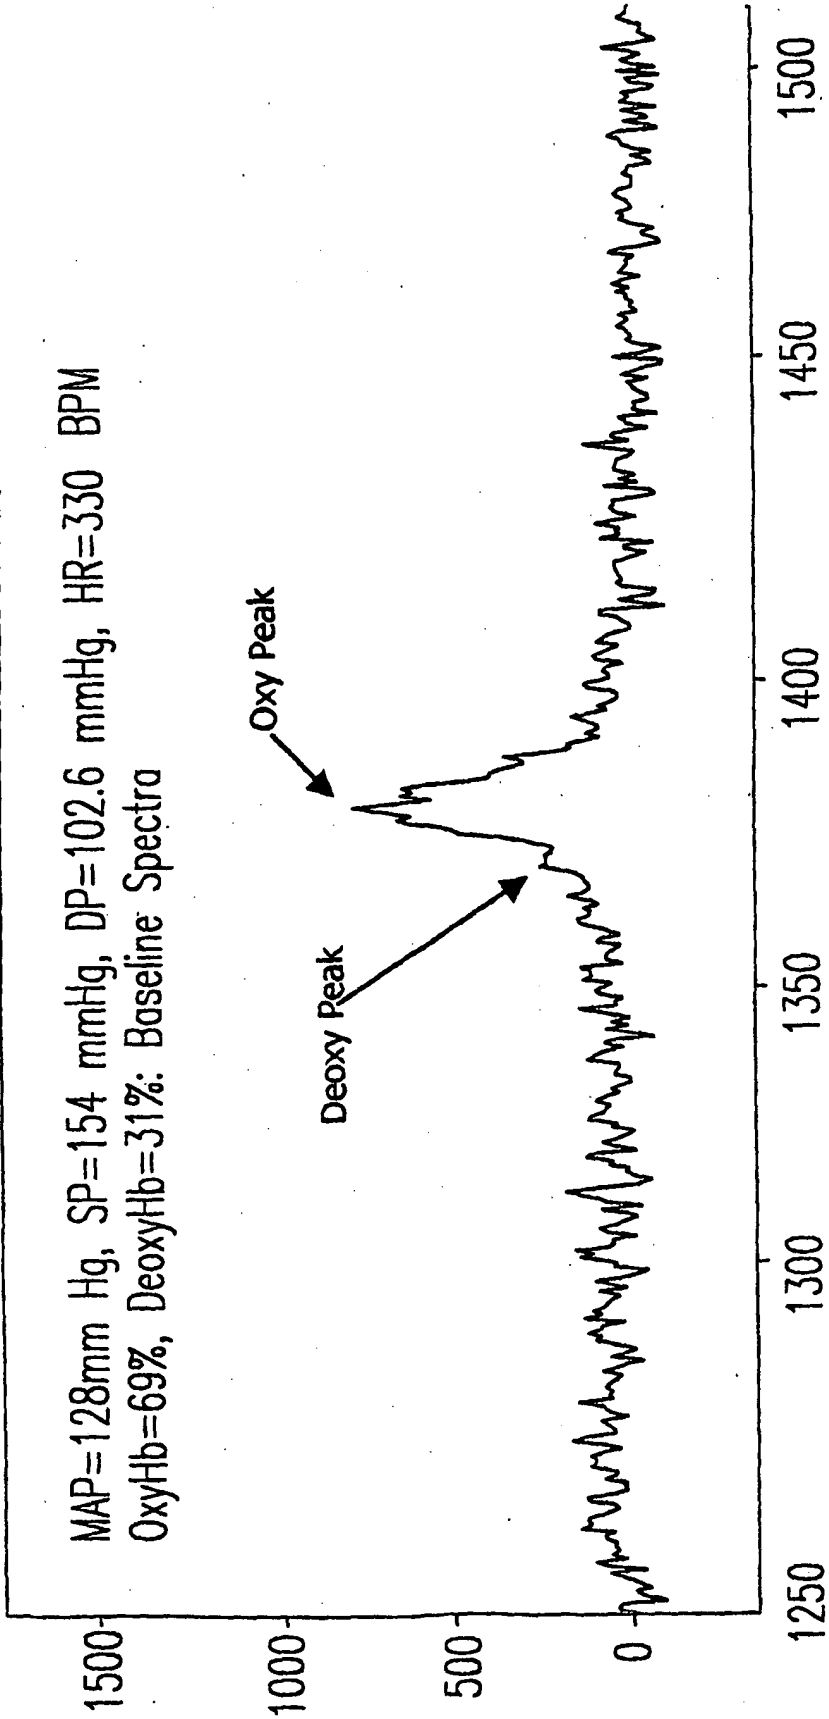


FIG.6

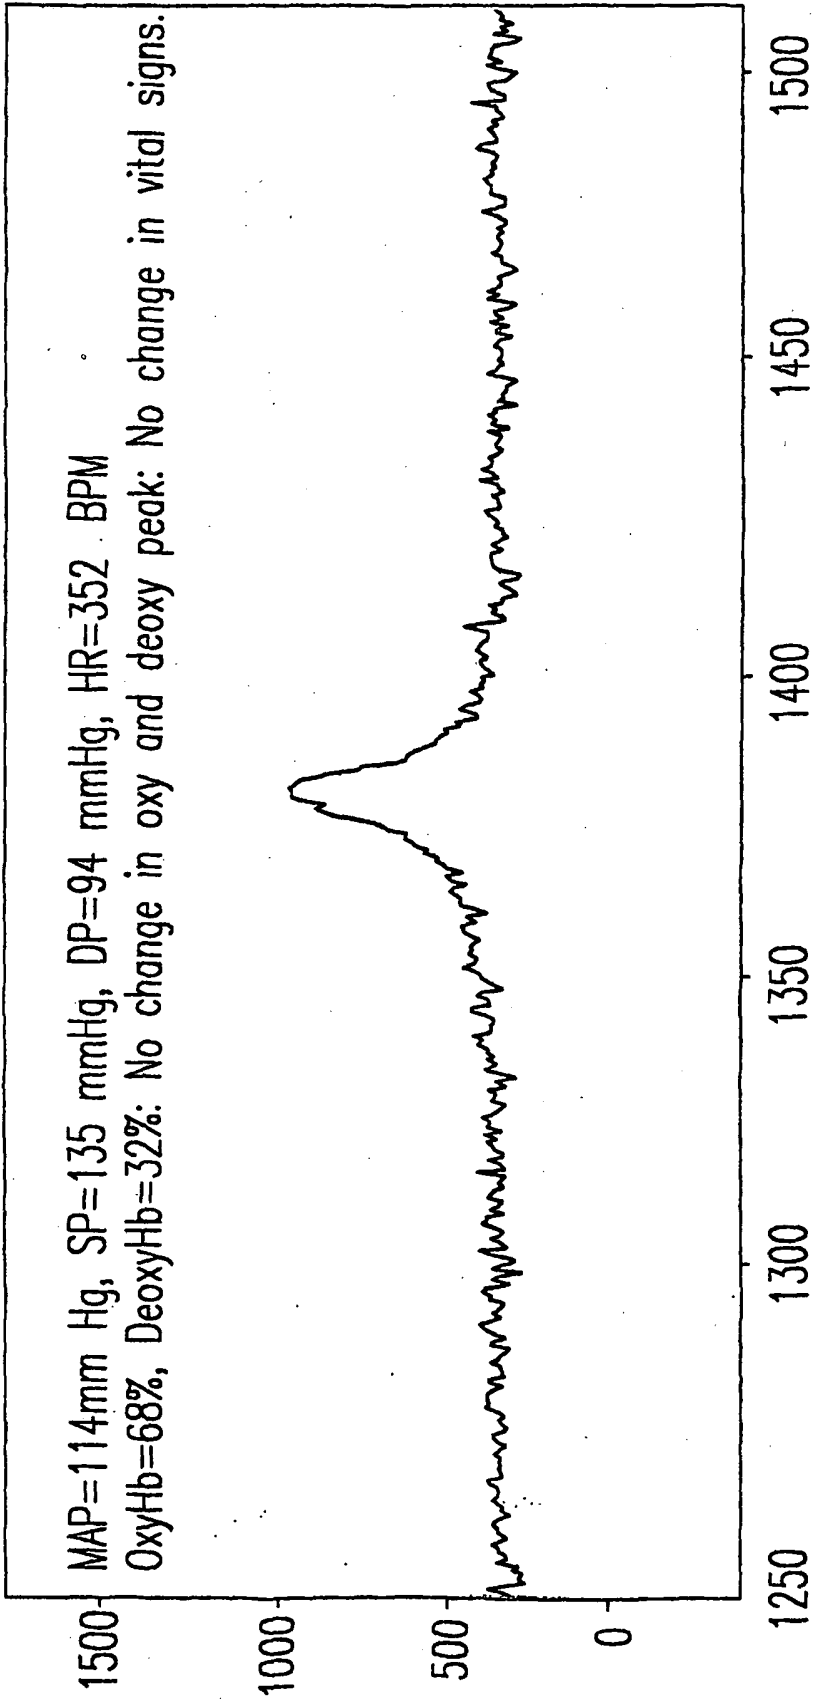


FIG.7

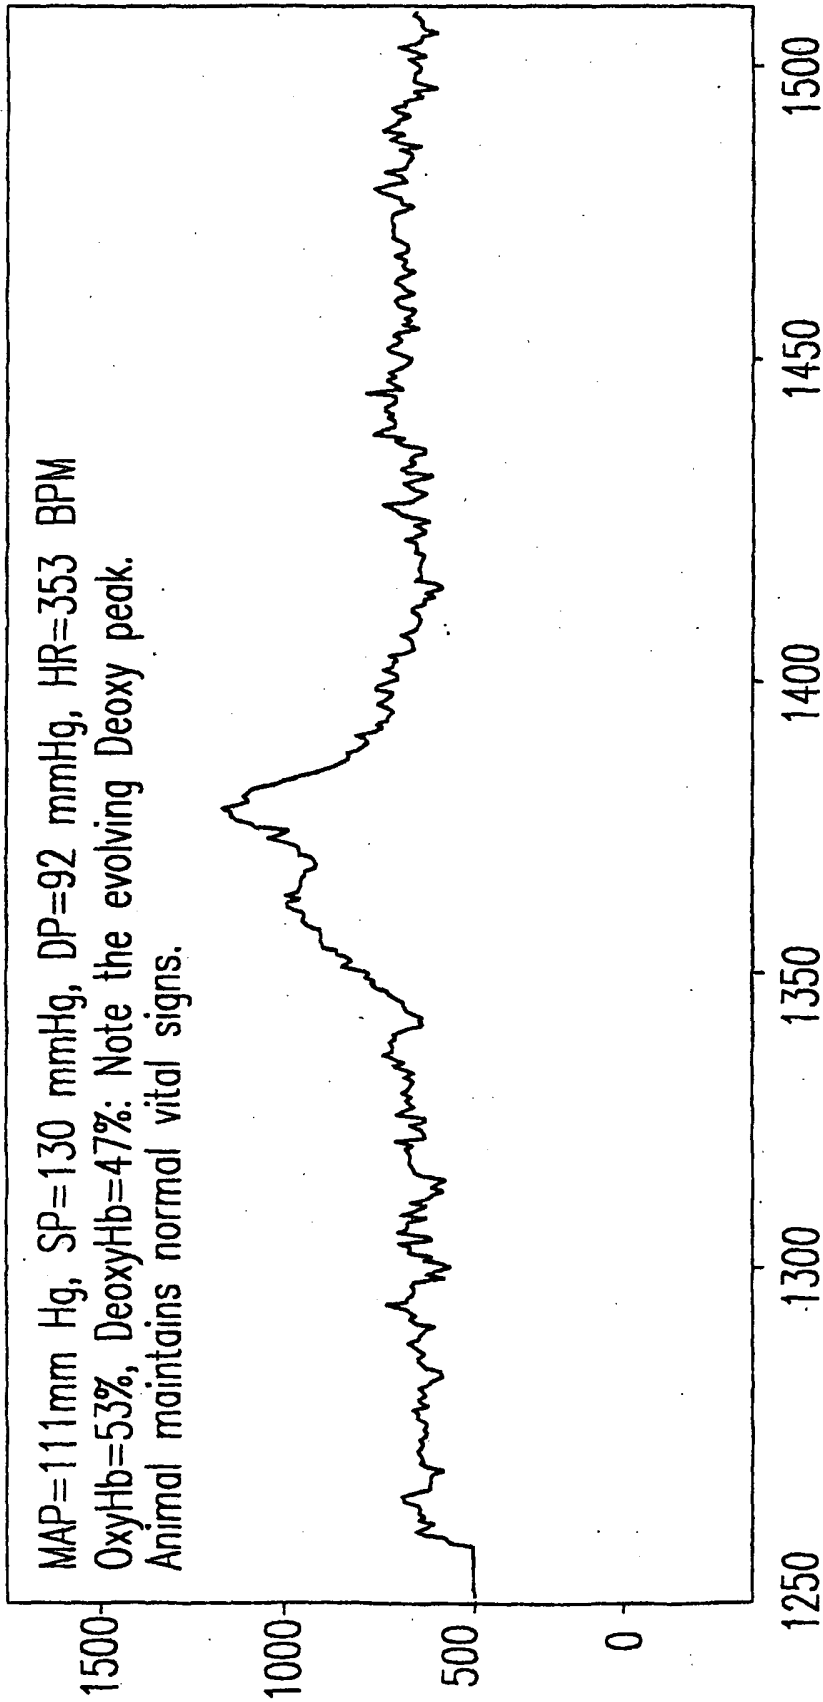


FIG.8

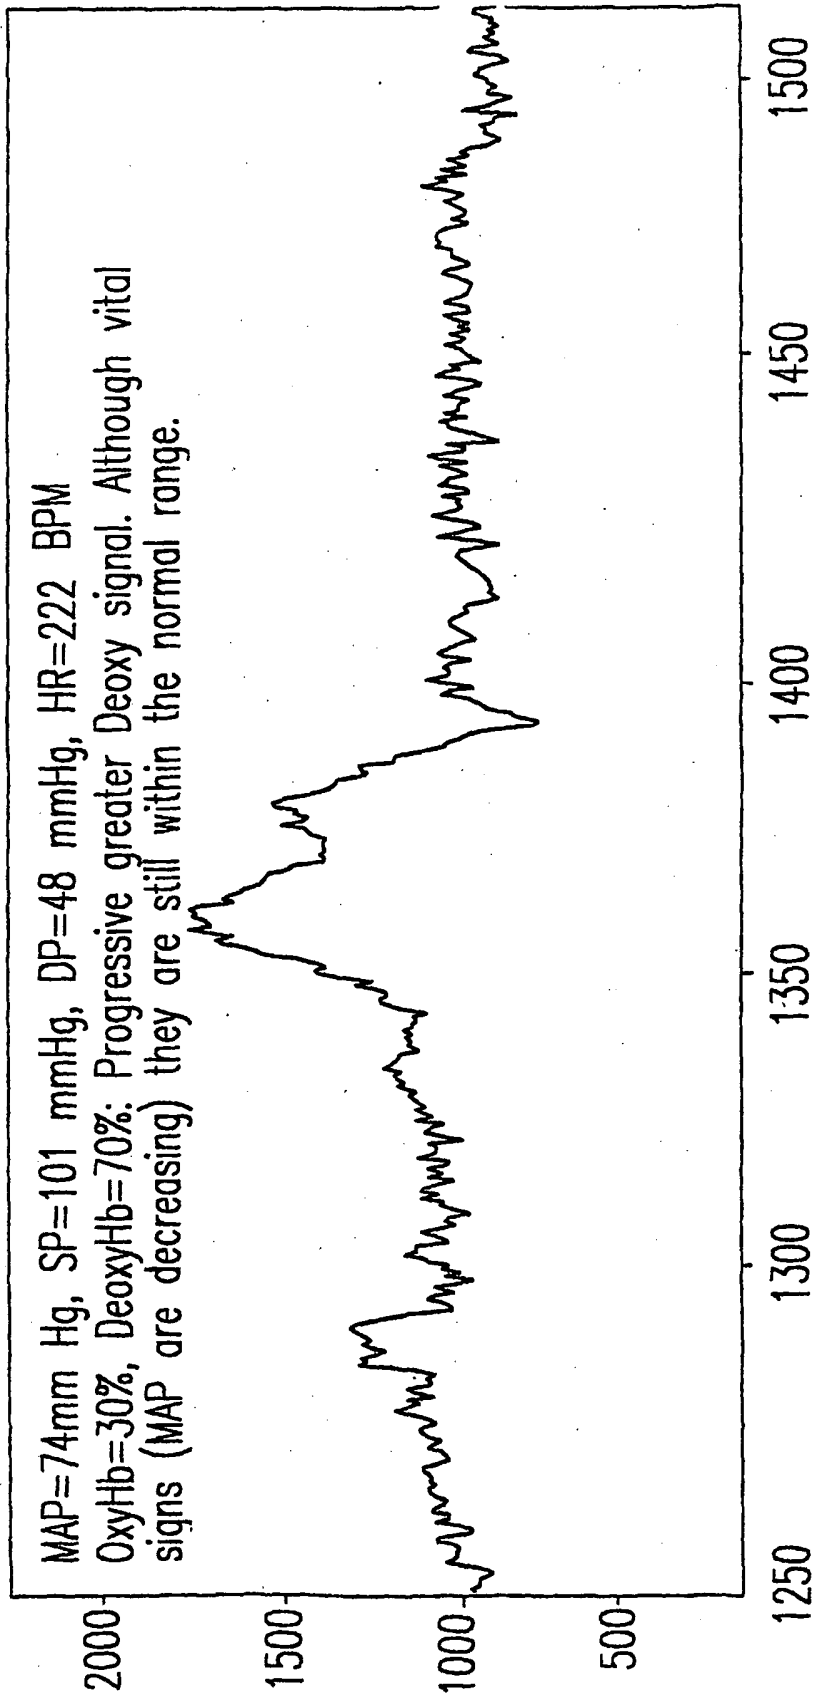


FIG.9

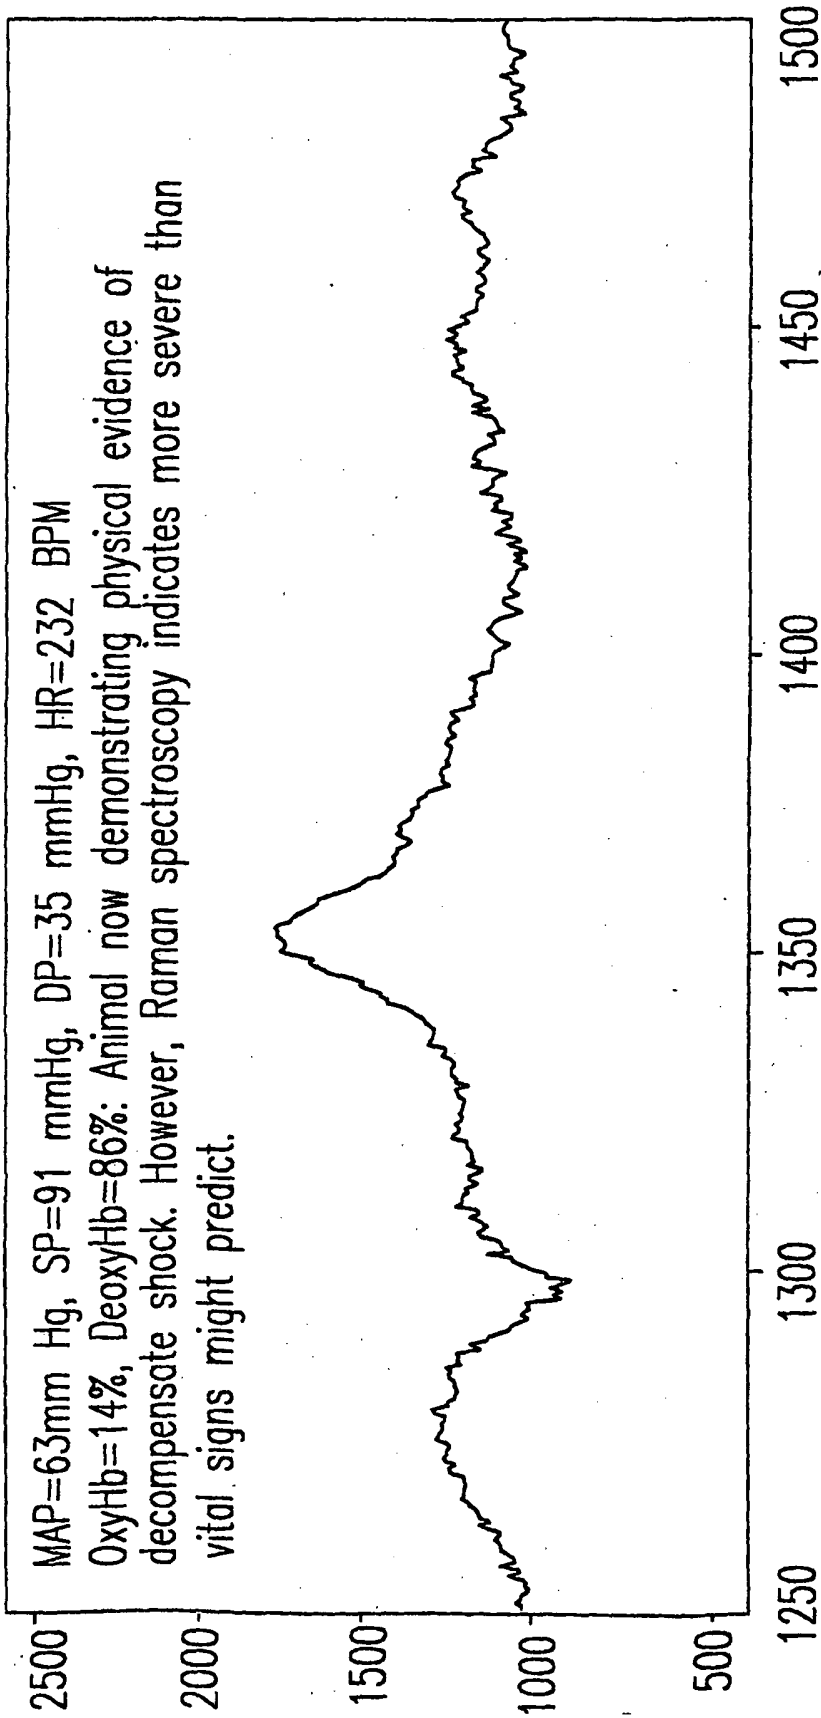


FIG.10

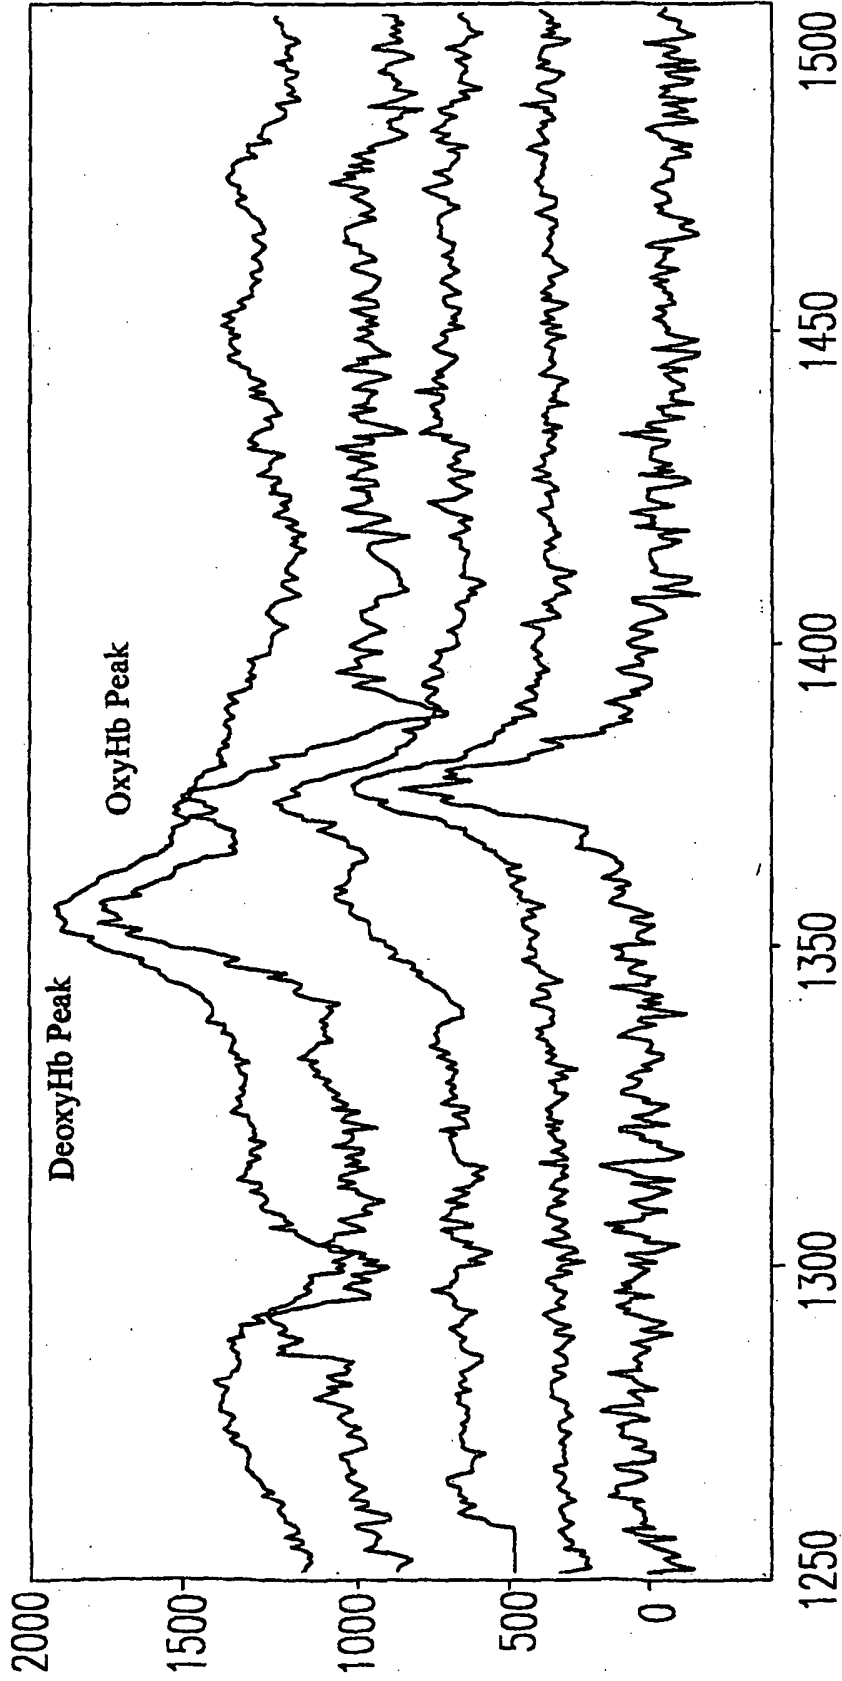


FIG.11


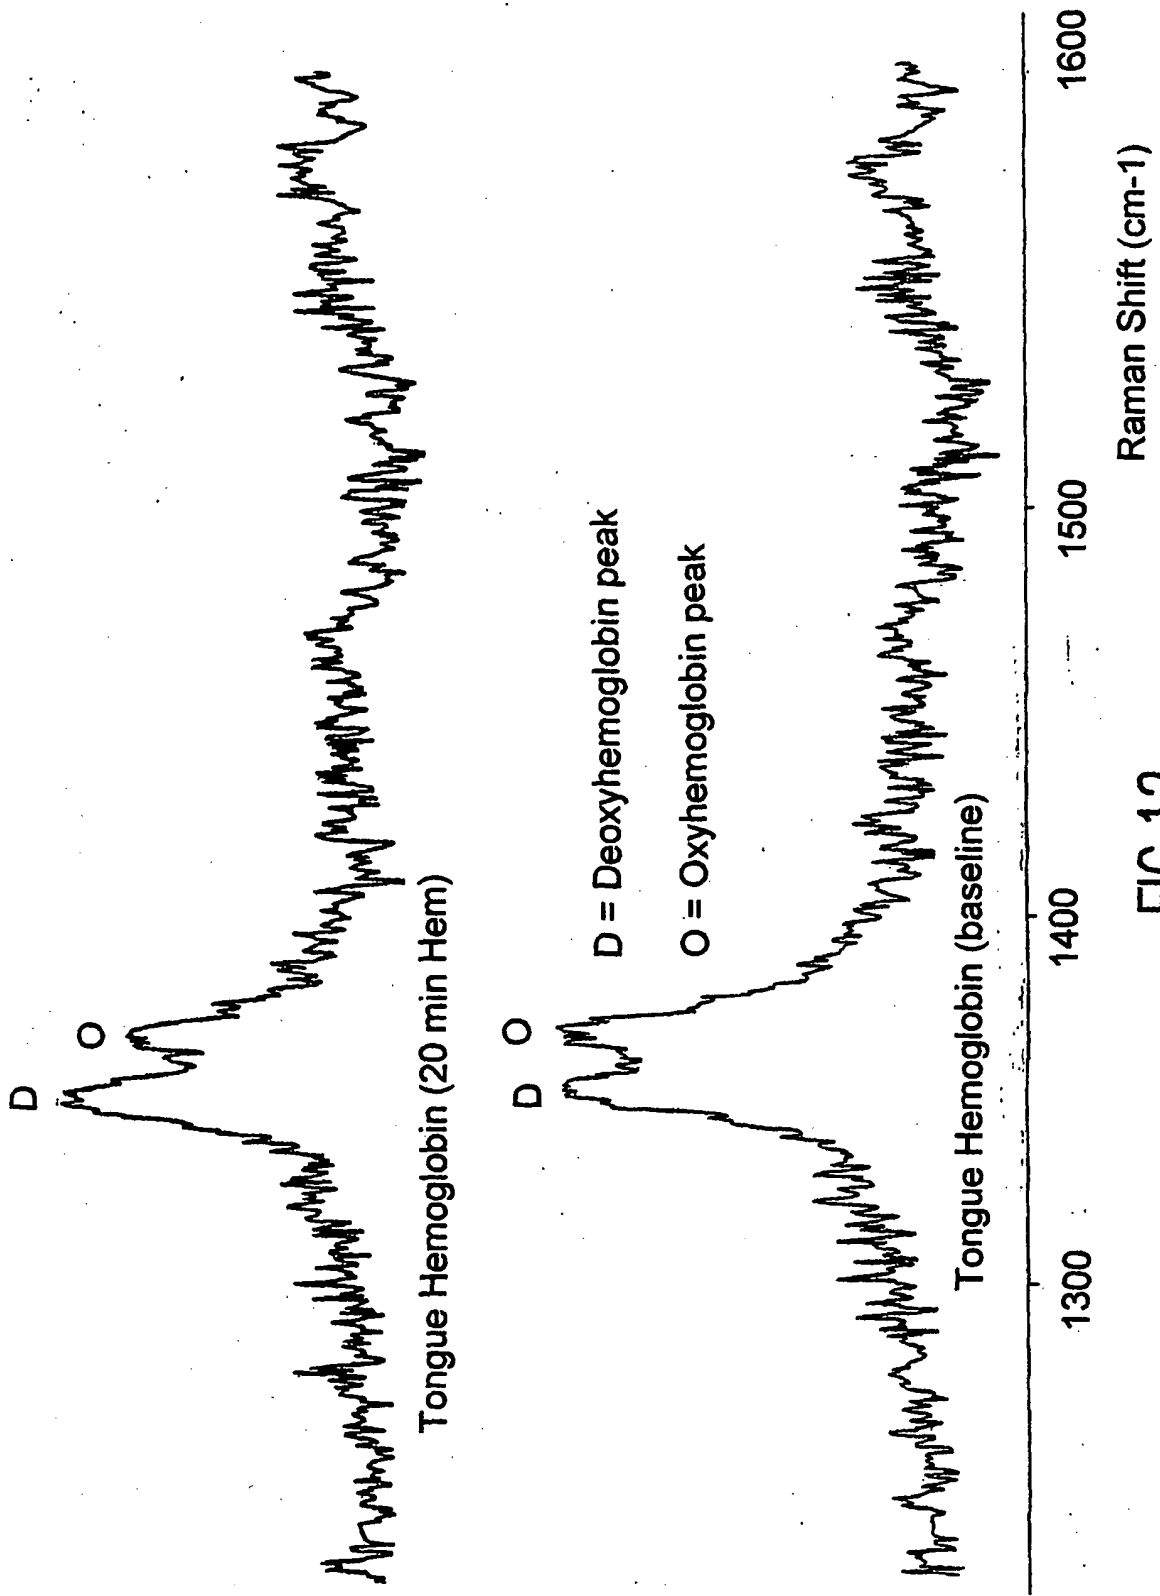


FIG.12

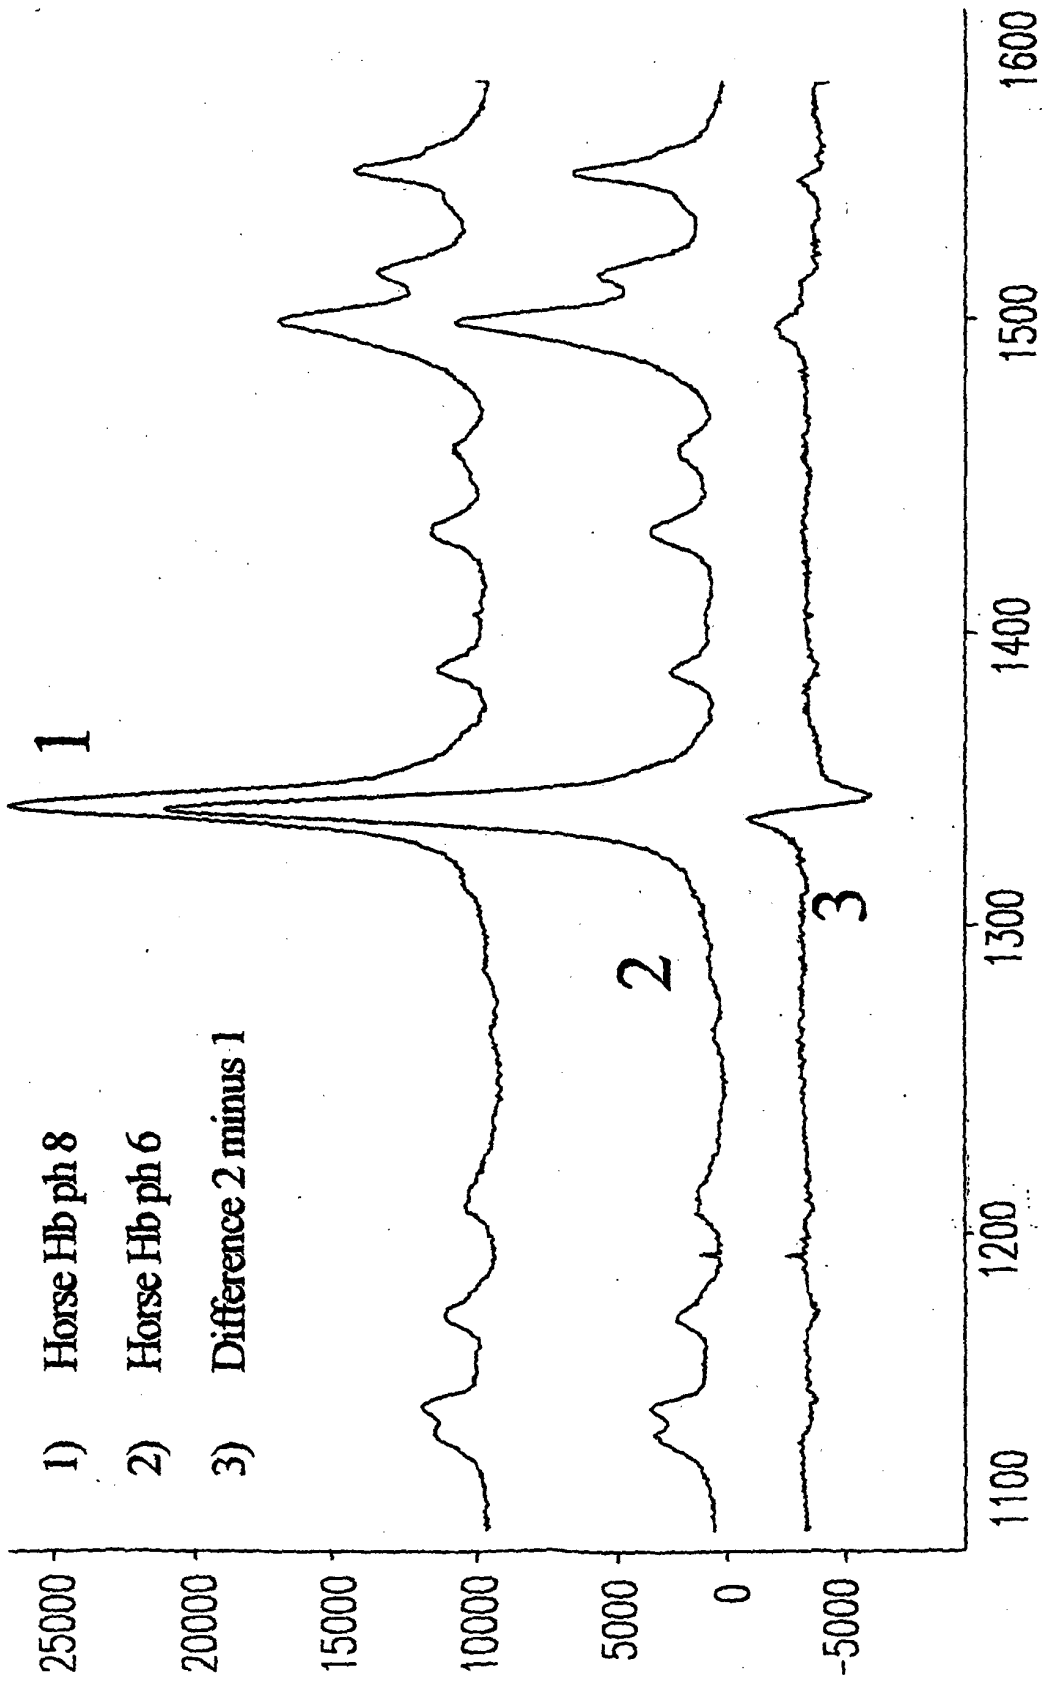

- 1) Horse Hb ph 8
- 2) Horse Hb ph 6
- 3) Difference 2 minus 1

FIG.13

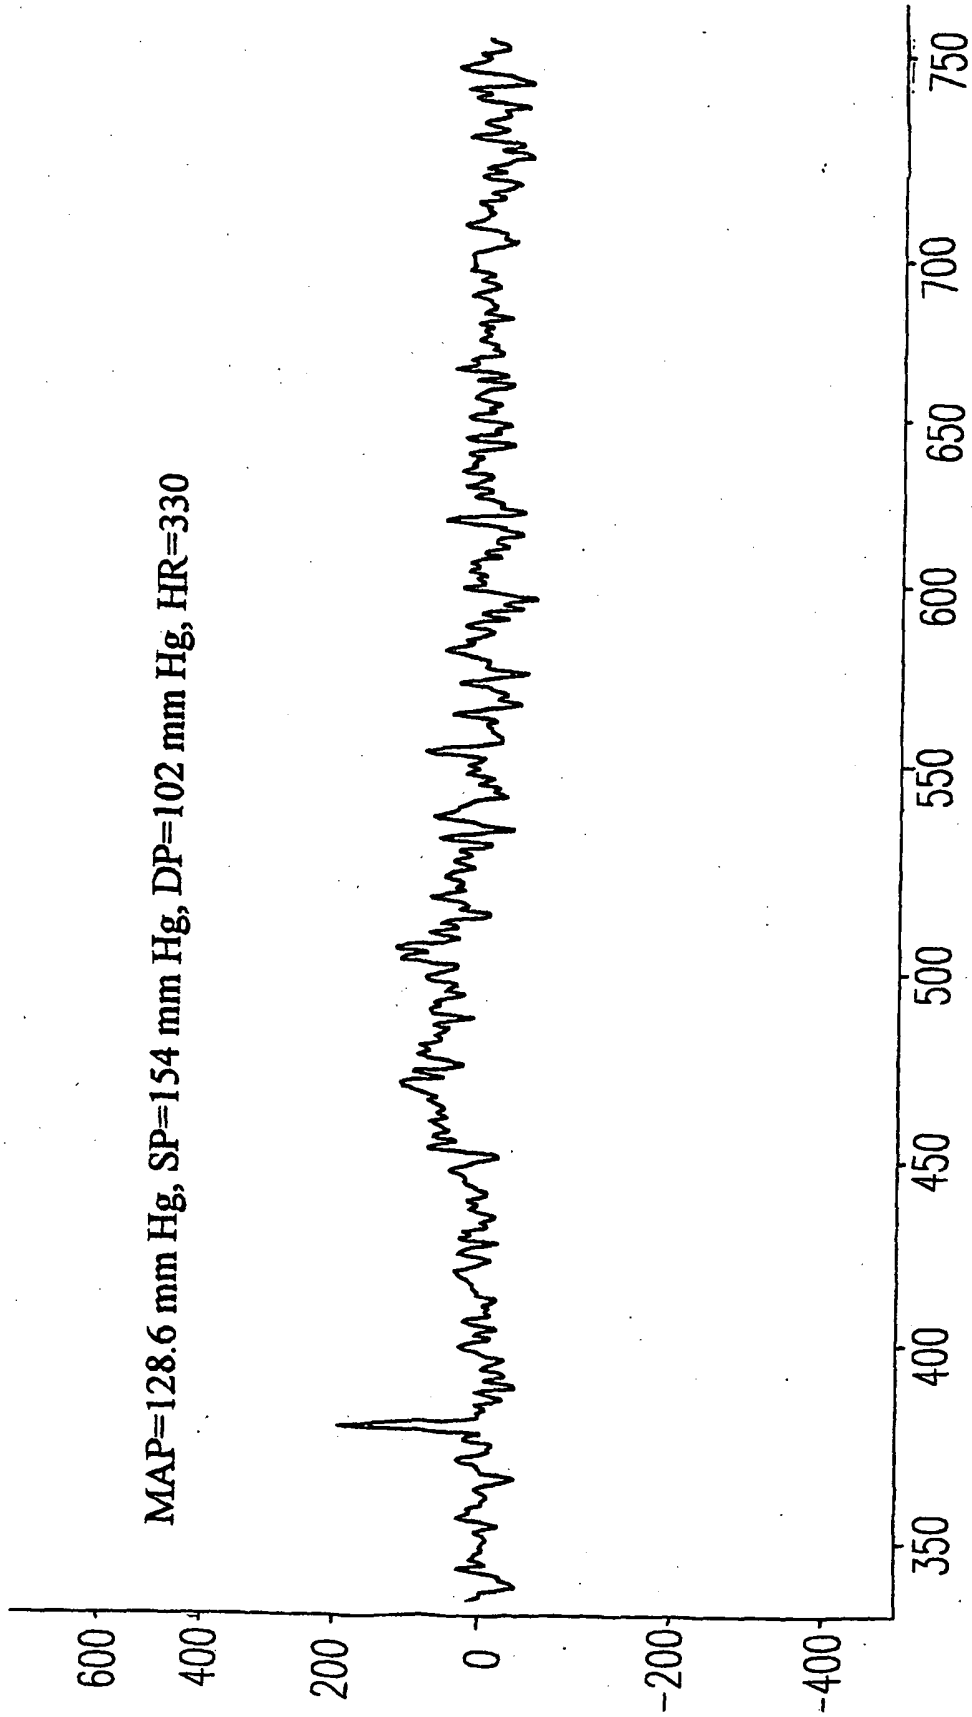


FIG.14

MAP=74 mm Hg, SP=101 mm Hg, DP=48 mm Hg, HR=222

Significant NADH fluorescence after 5 ml hemorrhage. Animal with relatively normal vital signs. Fluorescence indicated that critical dysoxia has occurred.

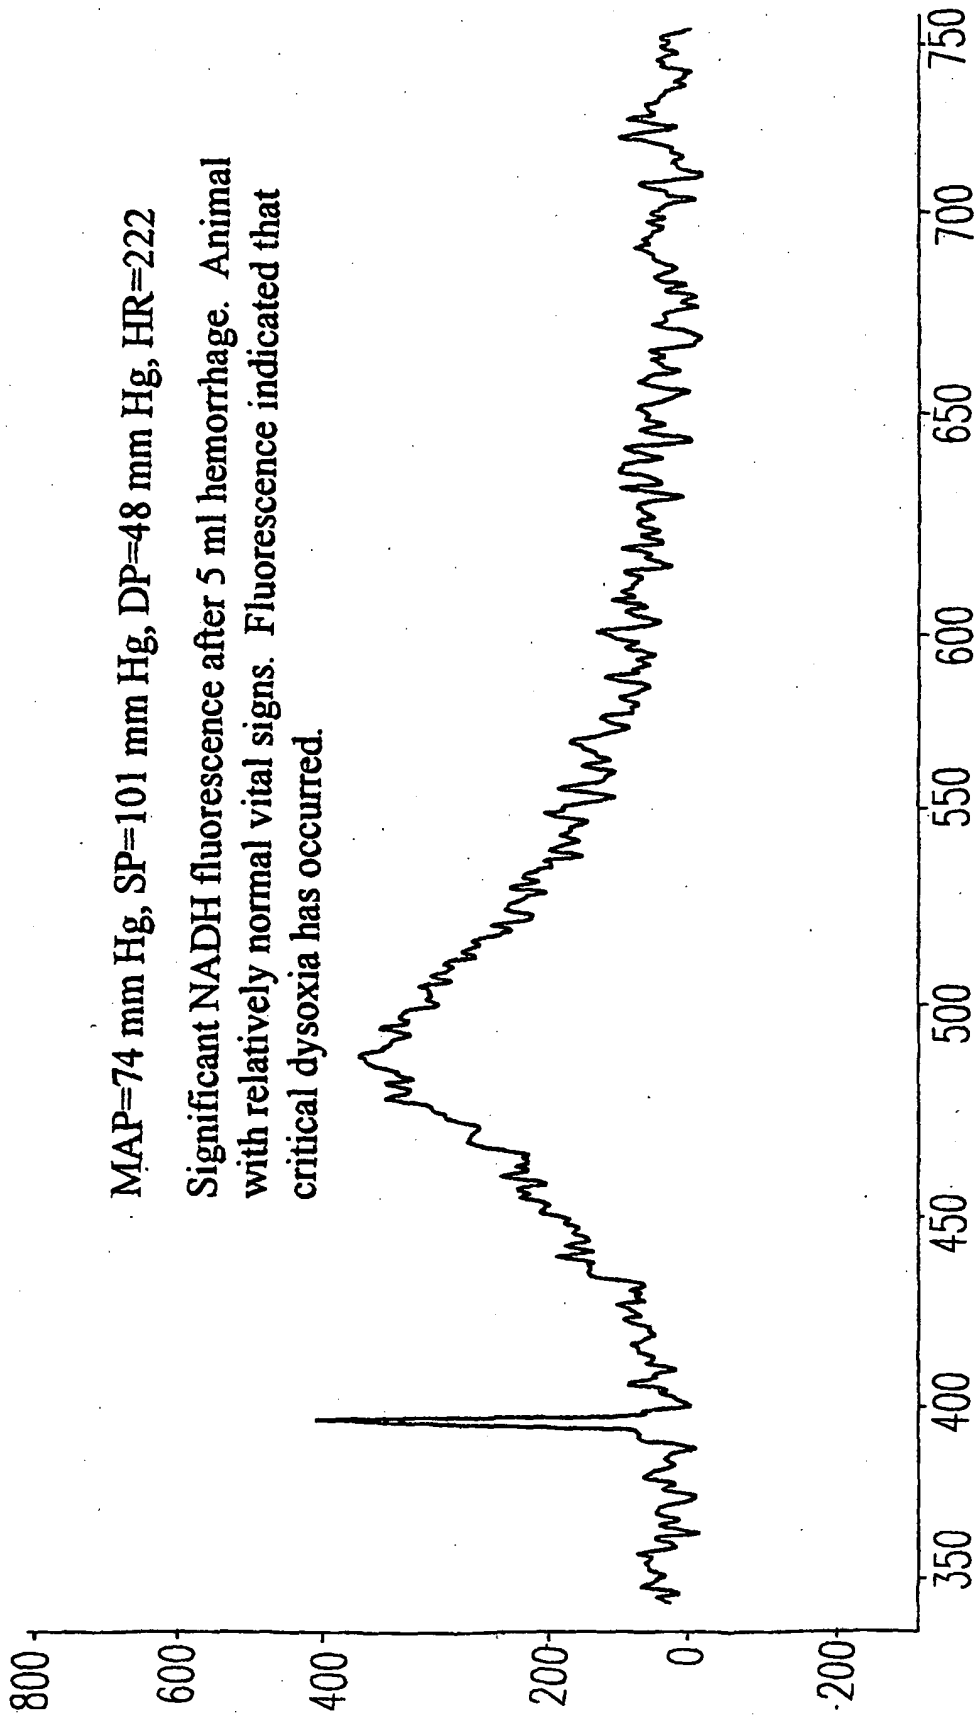


FIG.15

MAP=63 mm Hg, SP=91 mm Hg, DP=35 mm Hg, HR=232:

Increasing fluorescence indicates additional ischemia

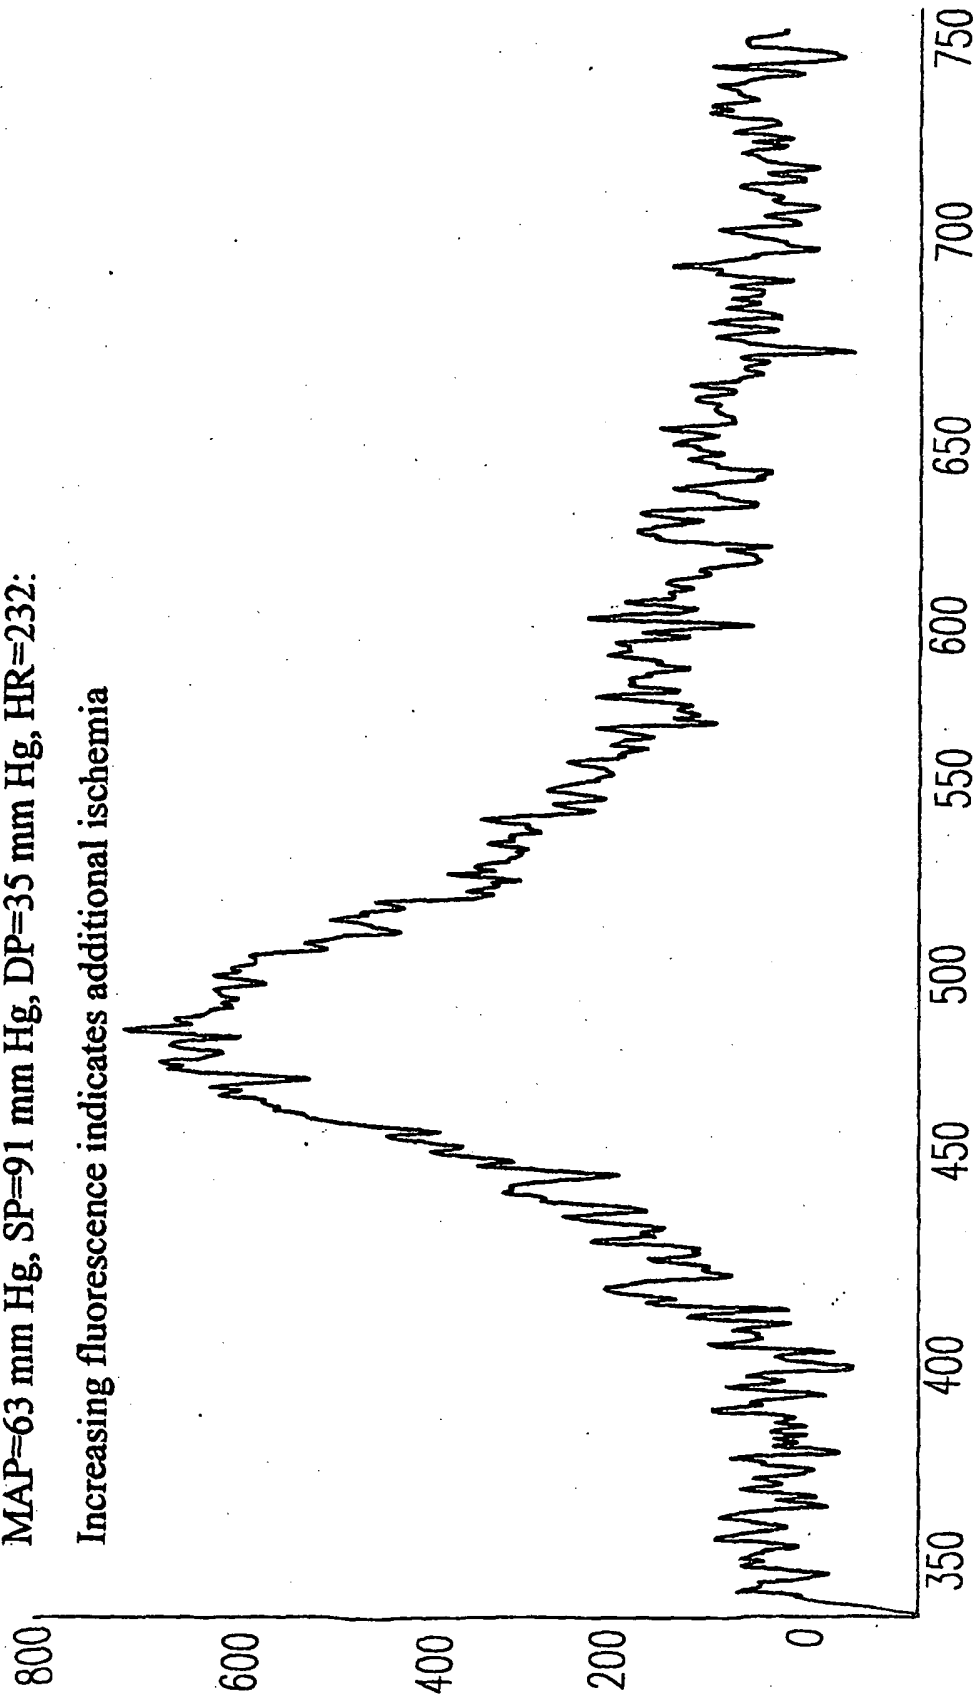


FIG.16

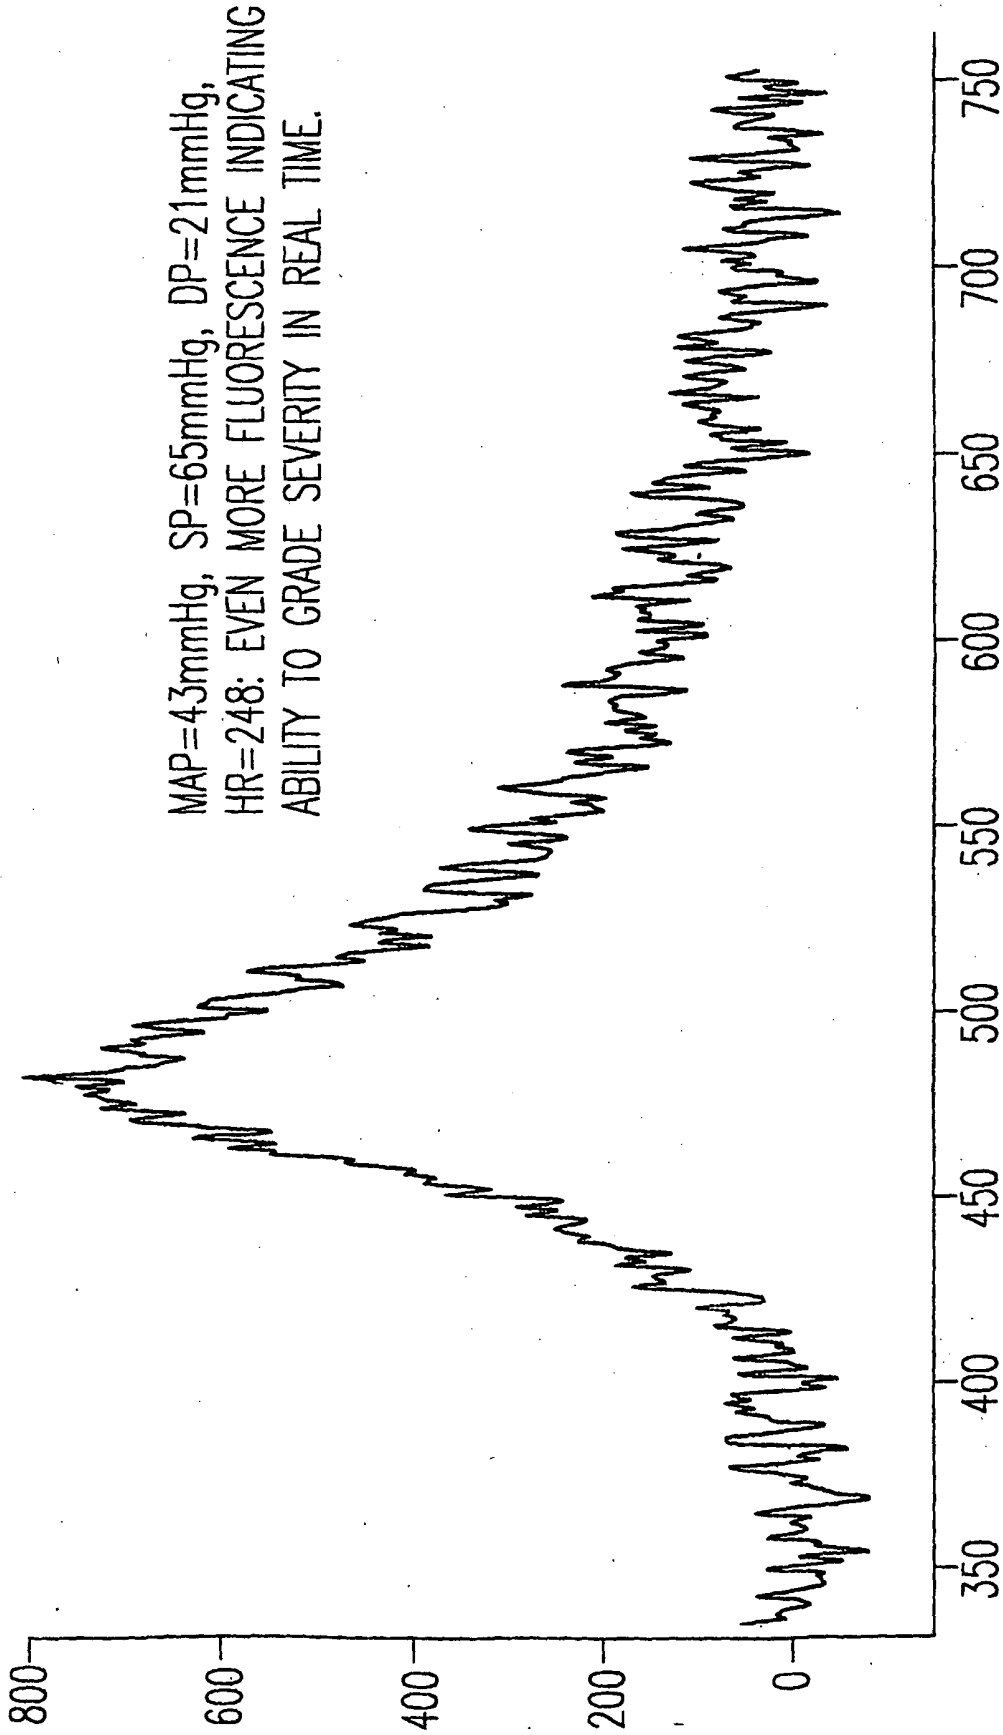


FIG.17

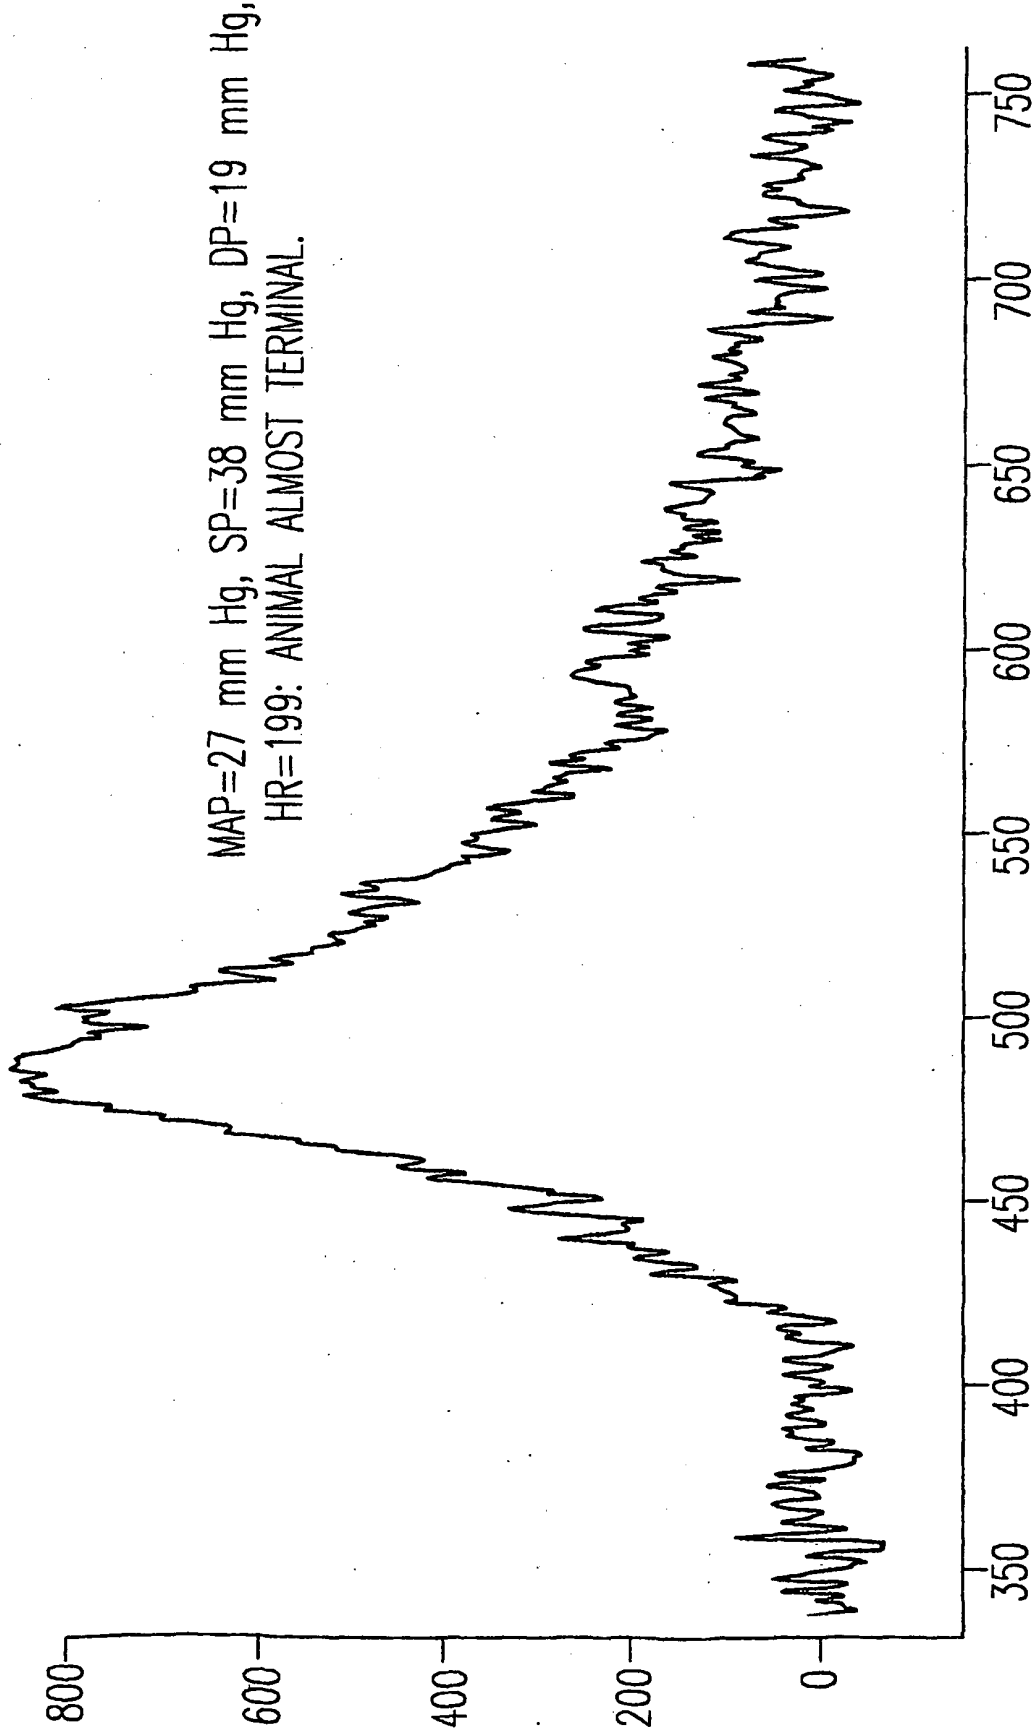


FIG.18

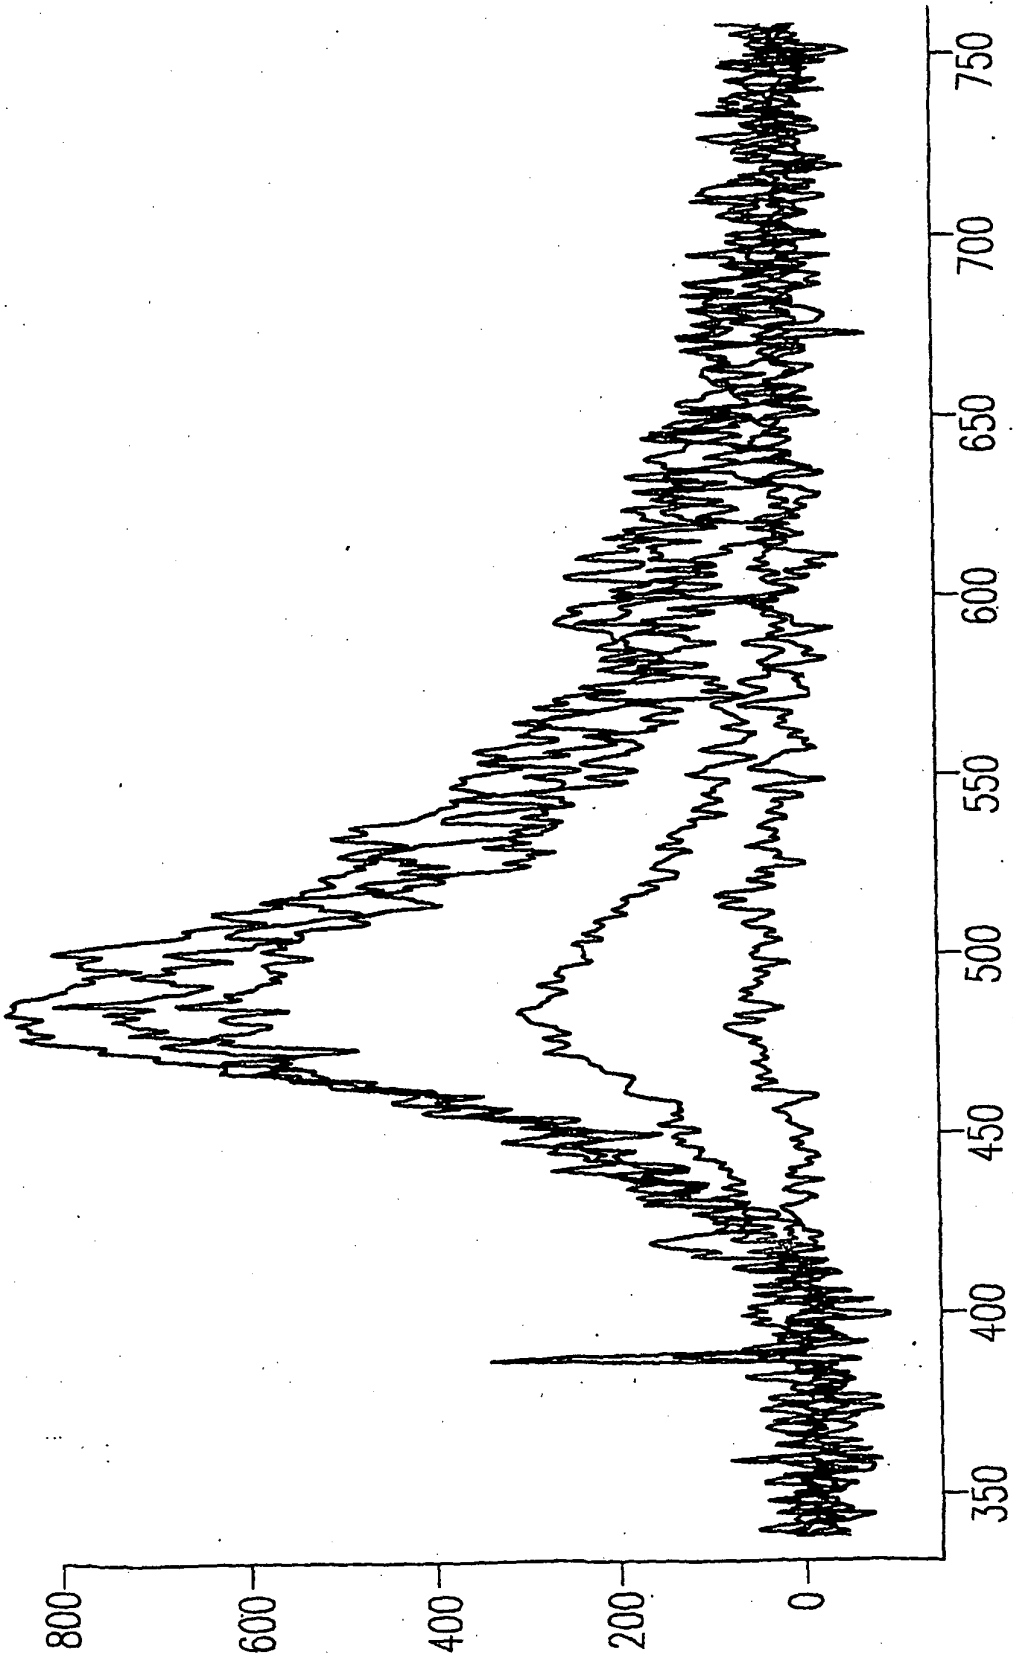


FIG.19

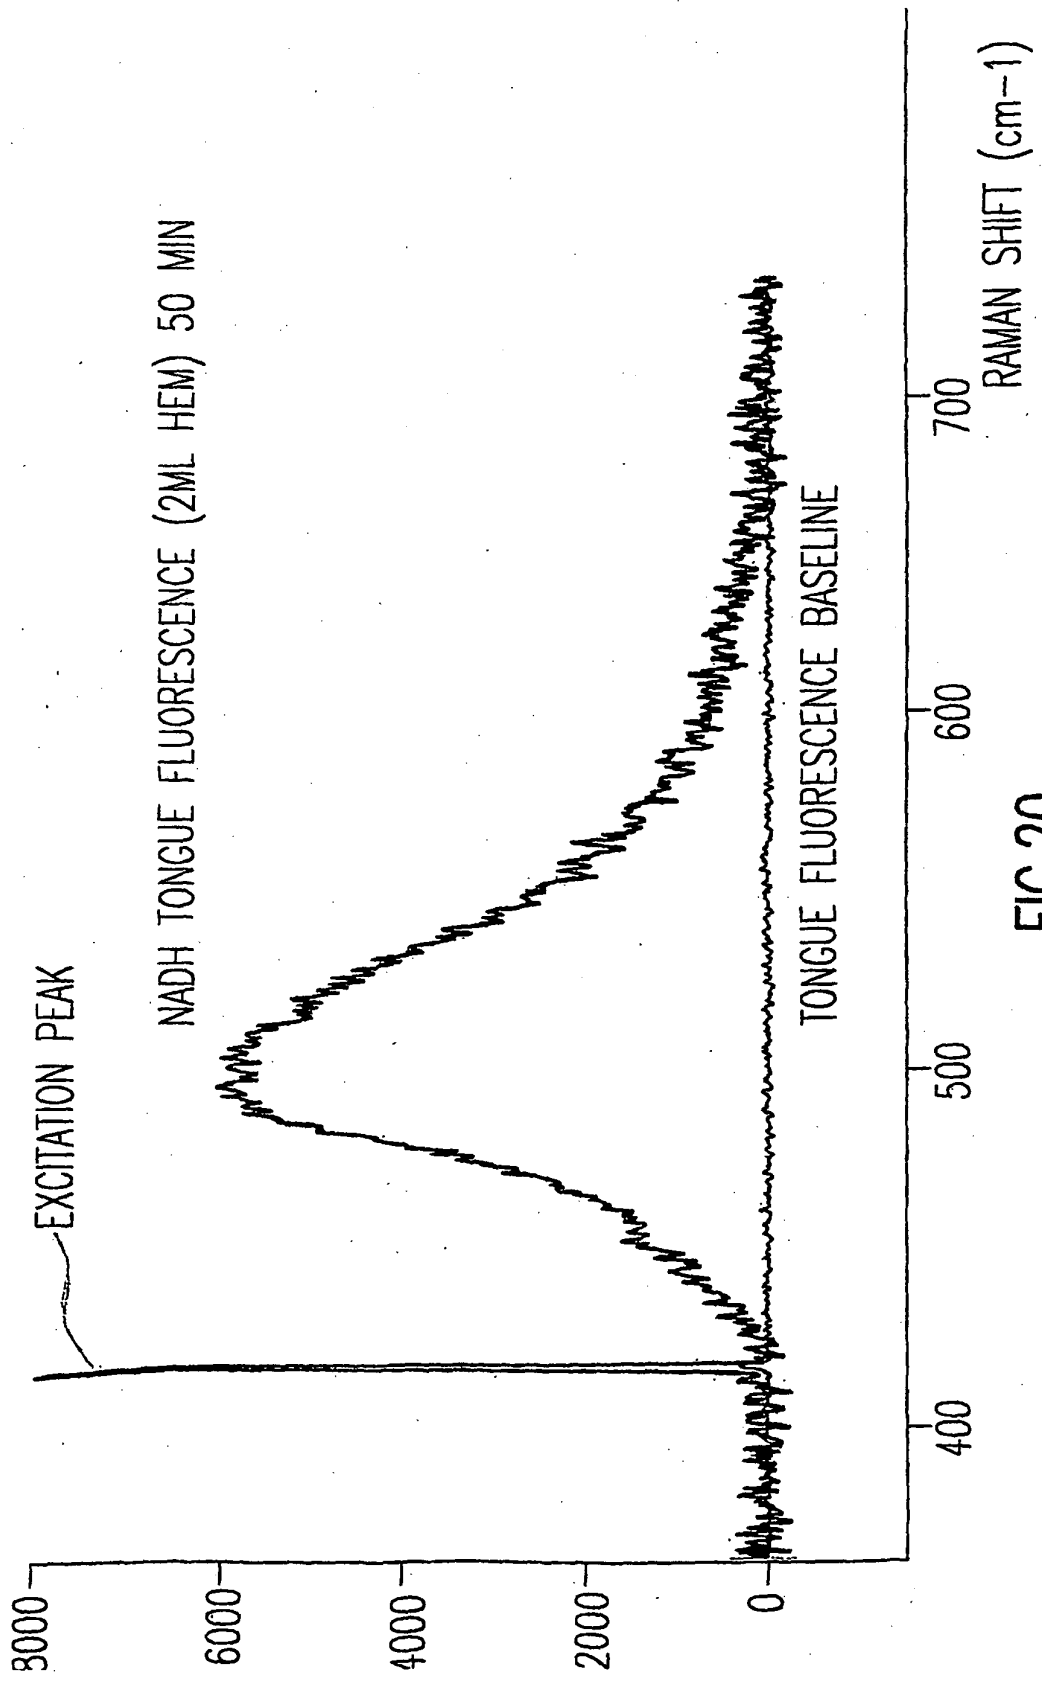


FIG.20

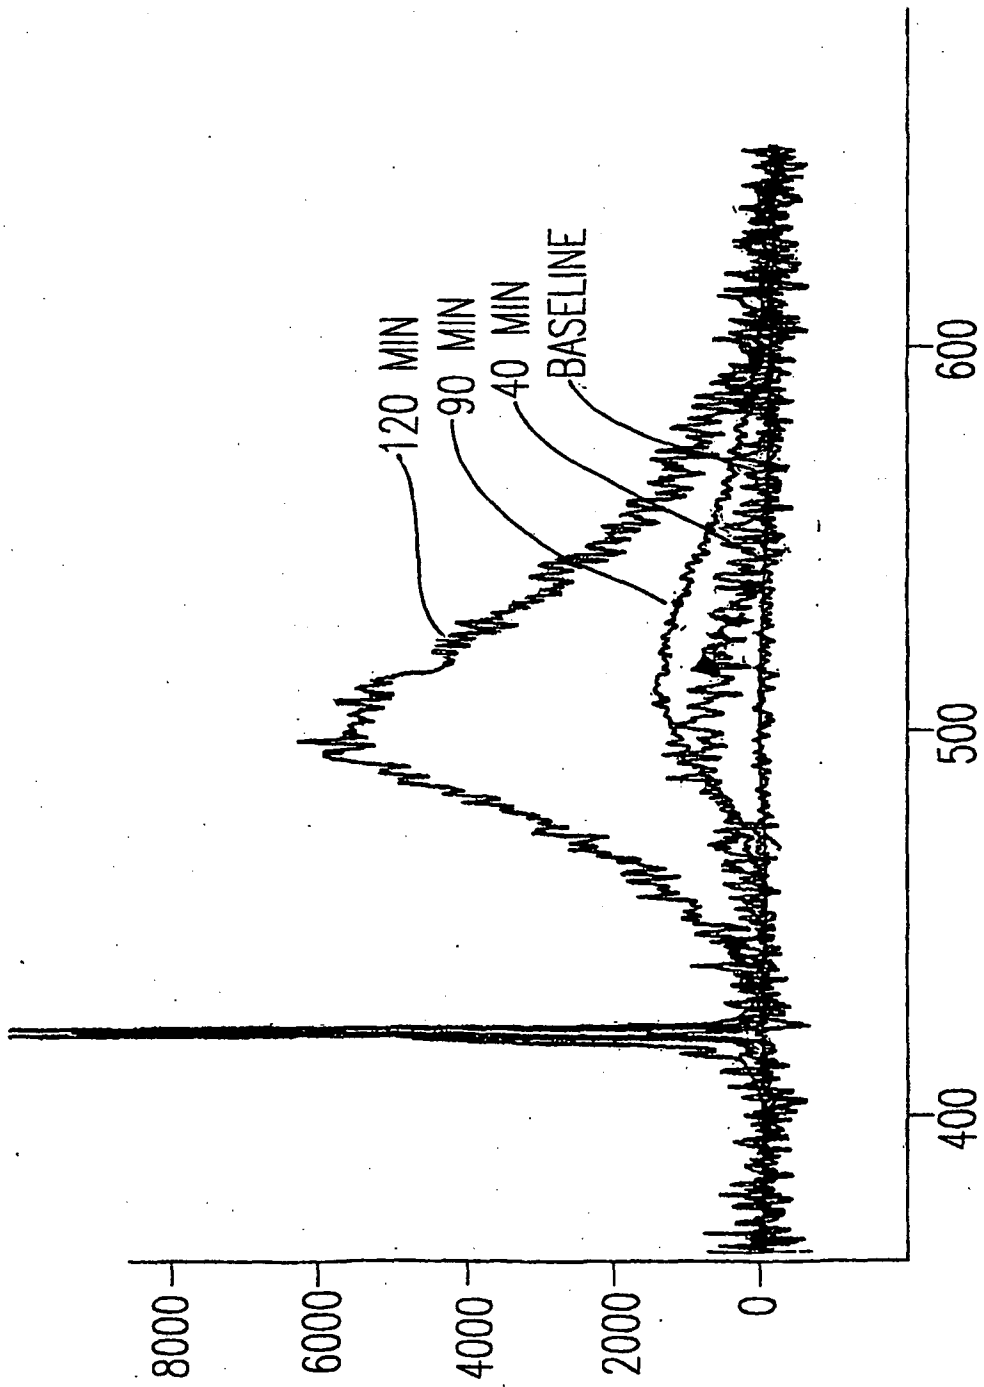


FIG.21

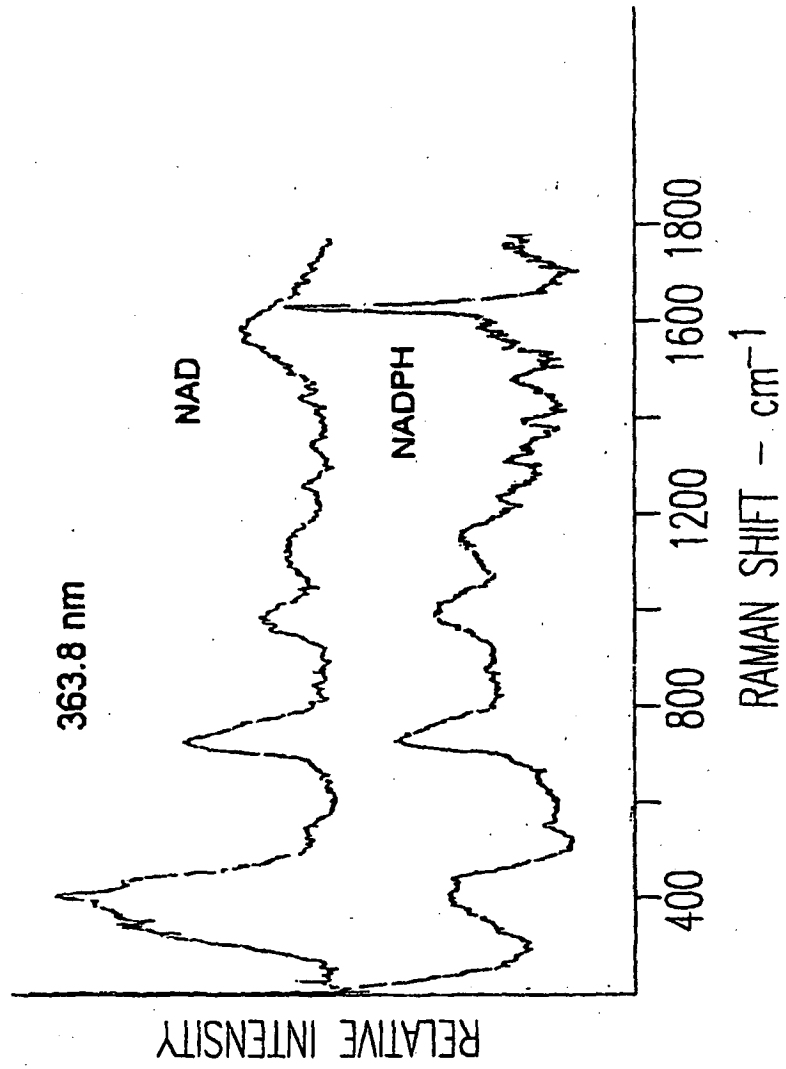


FIG.22A

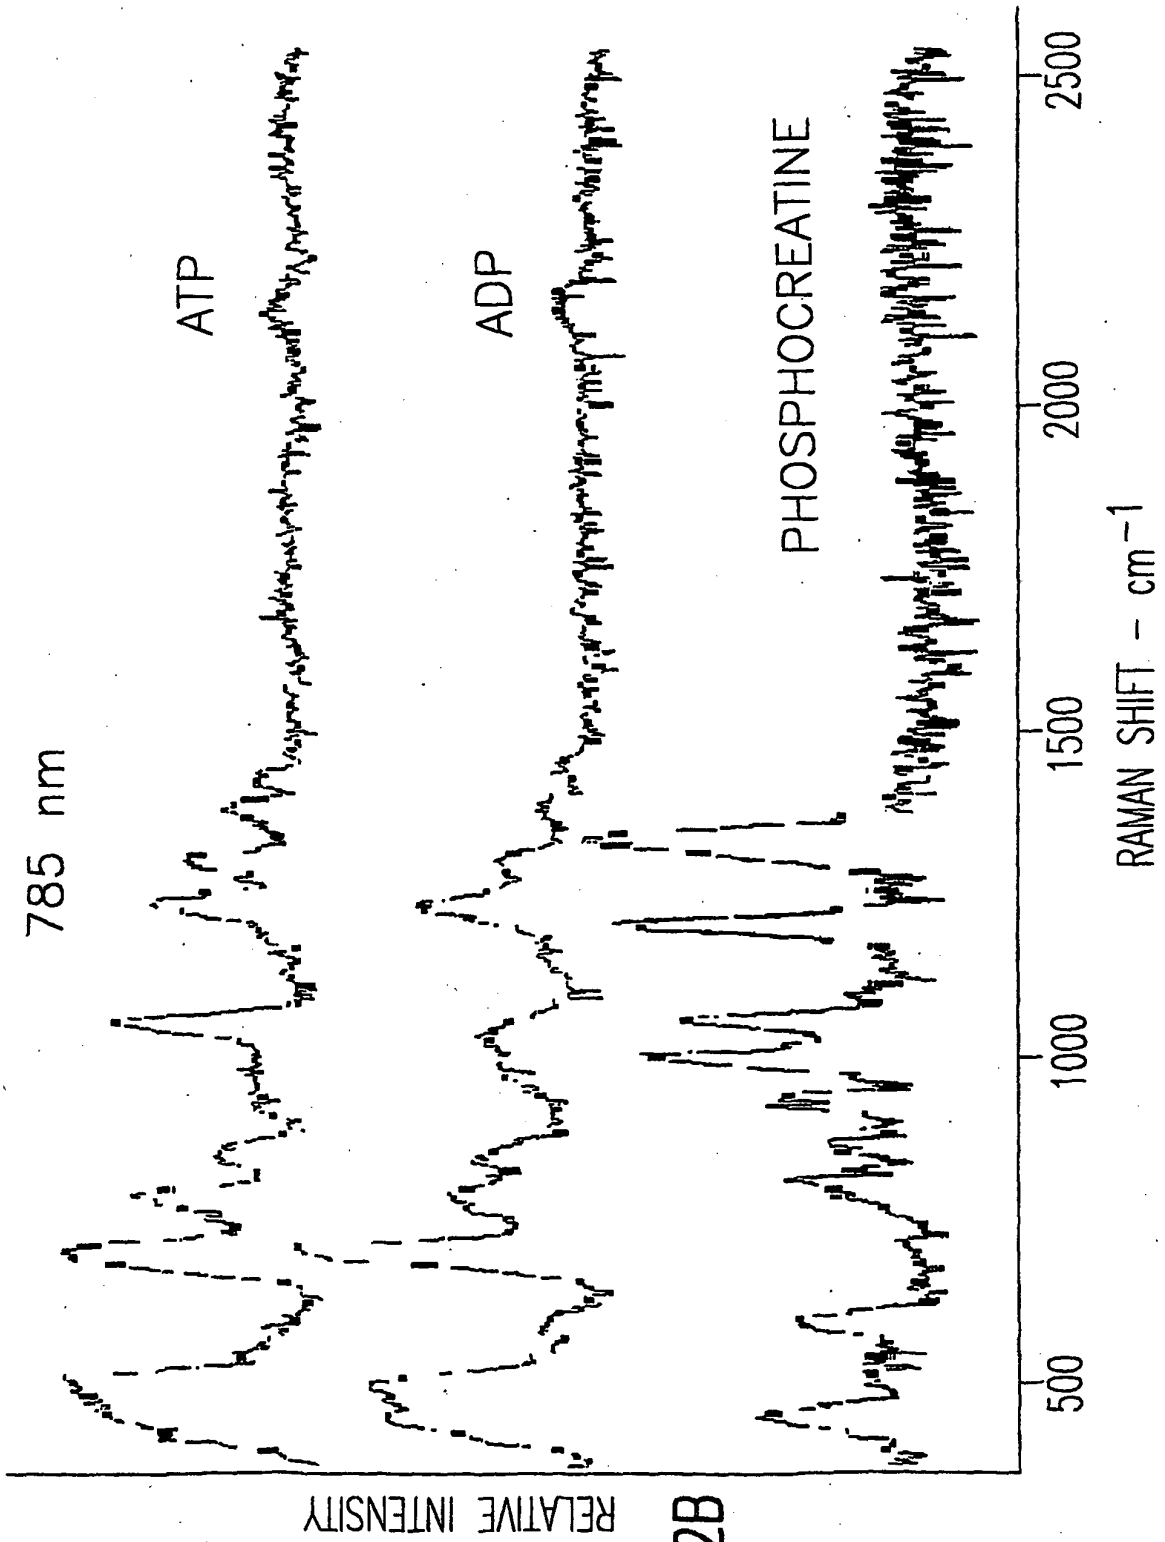


FIG. 22B

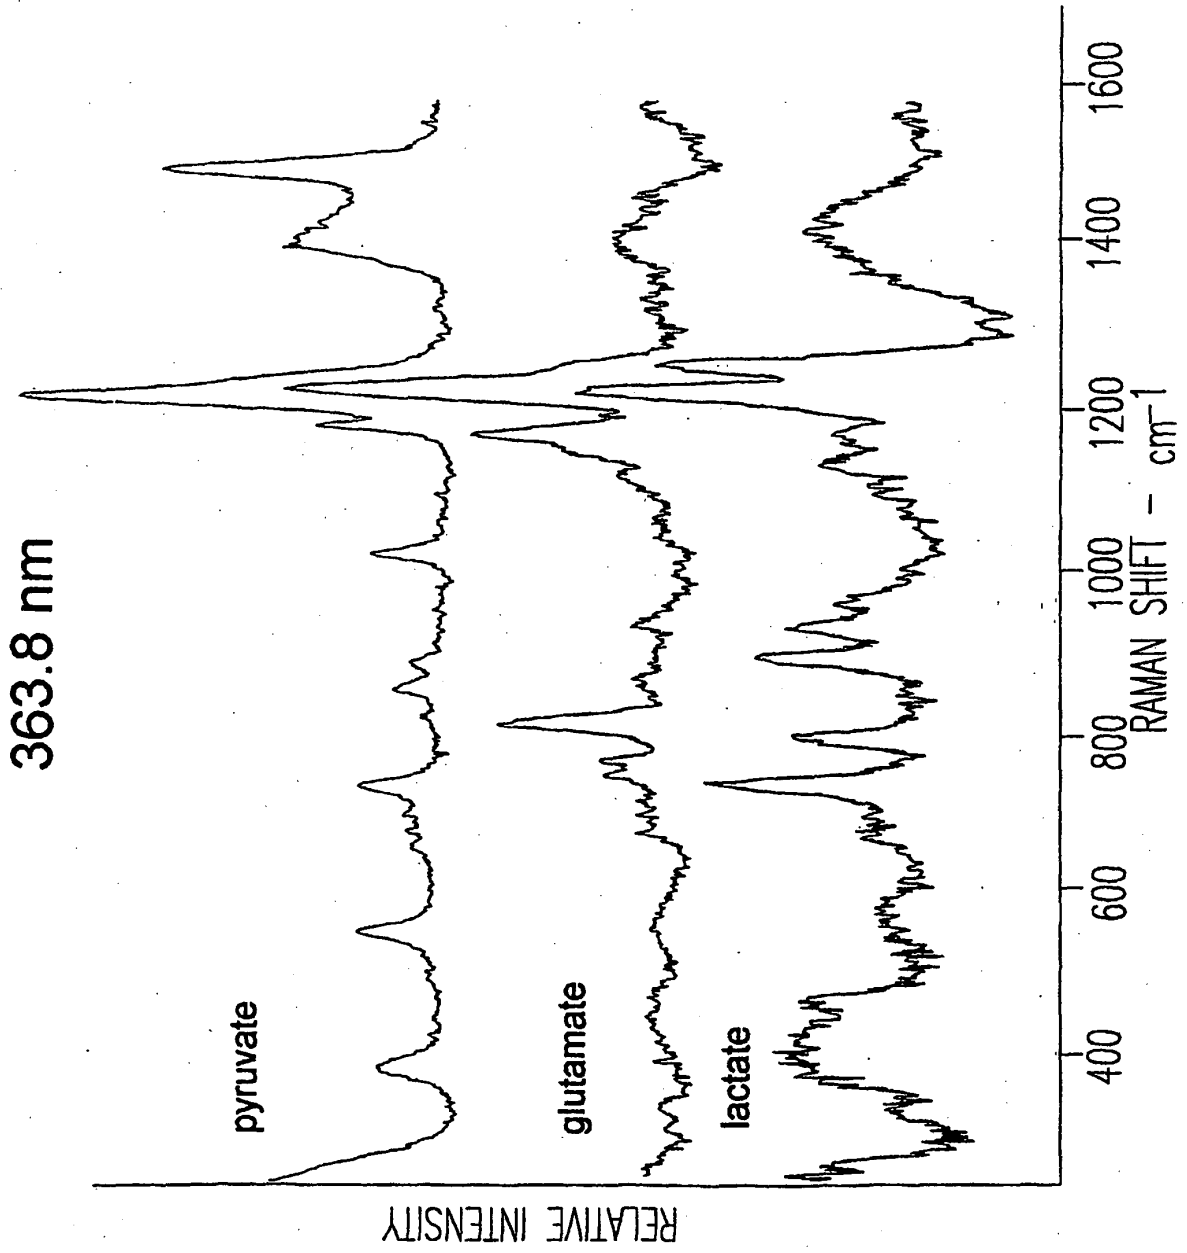


FIG.22C

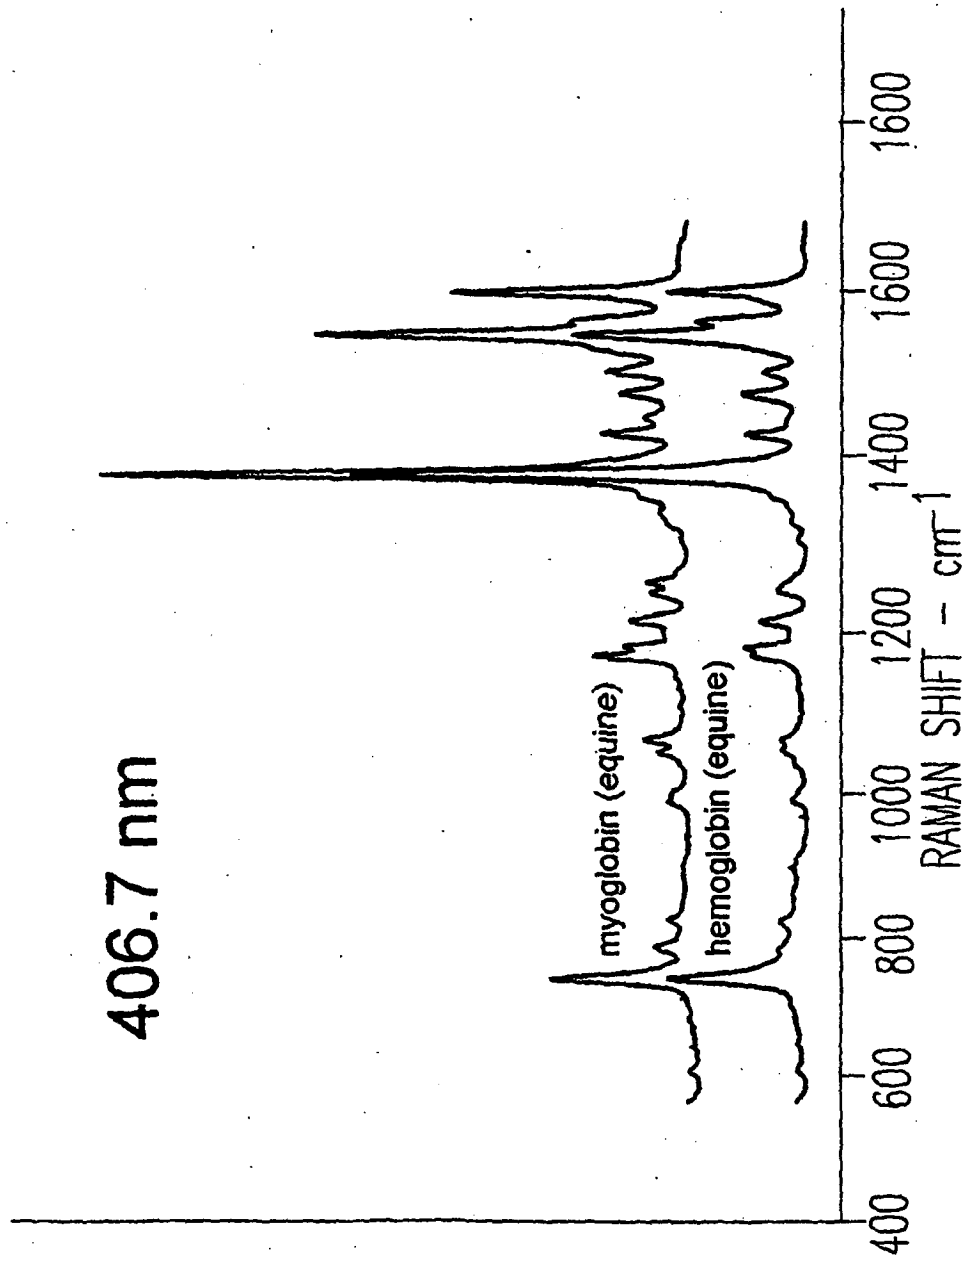


FIG.22D

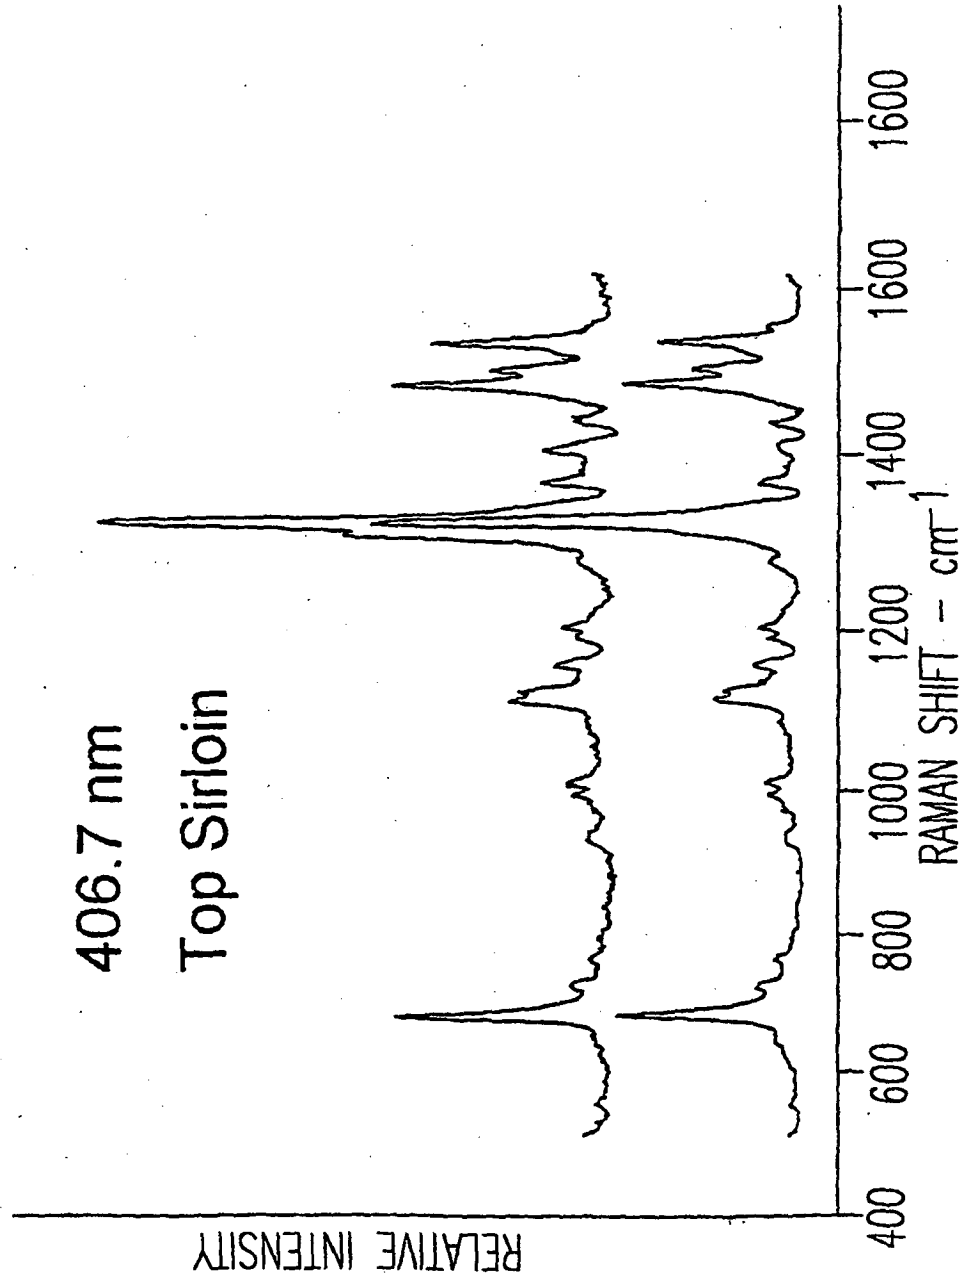


FIG.22E

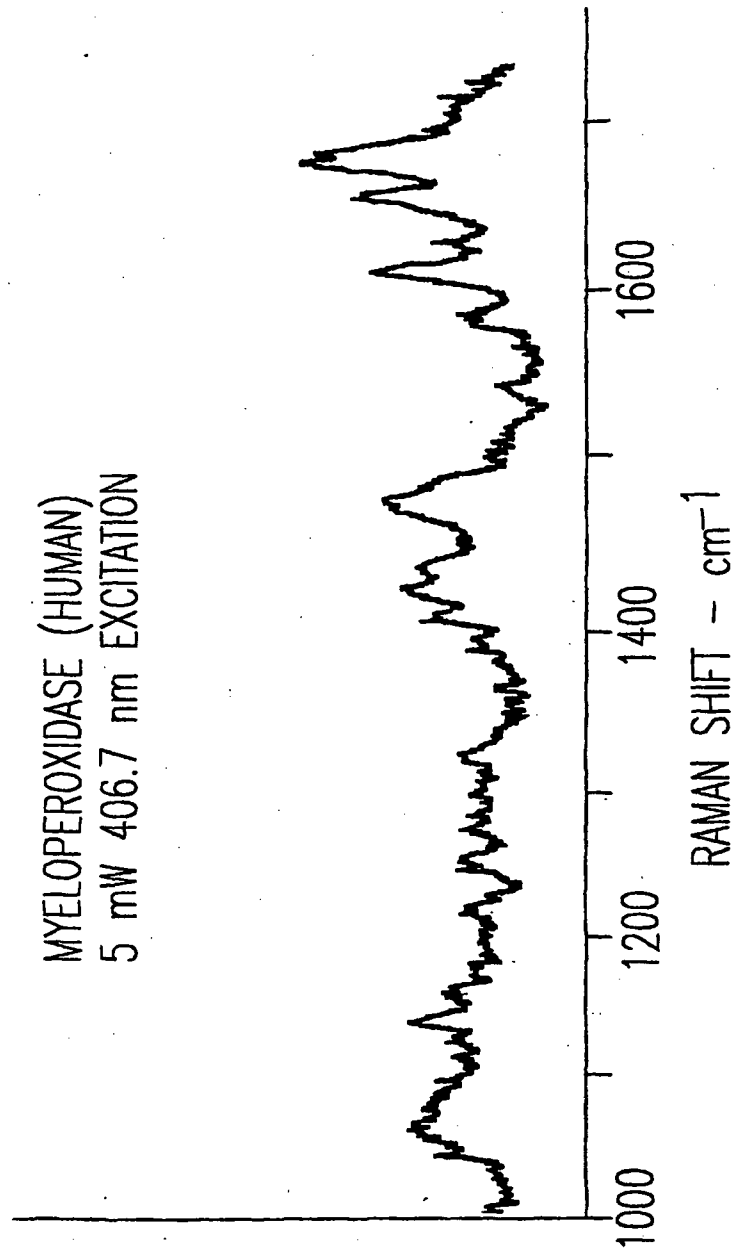


FIG.23

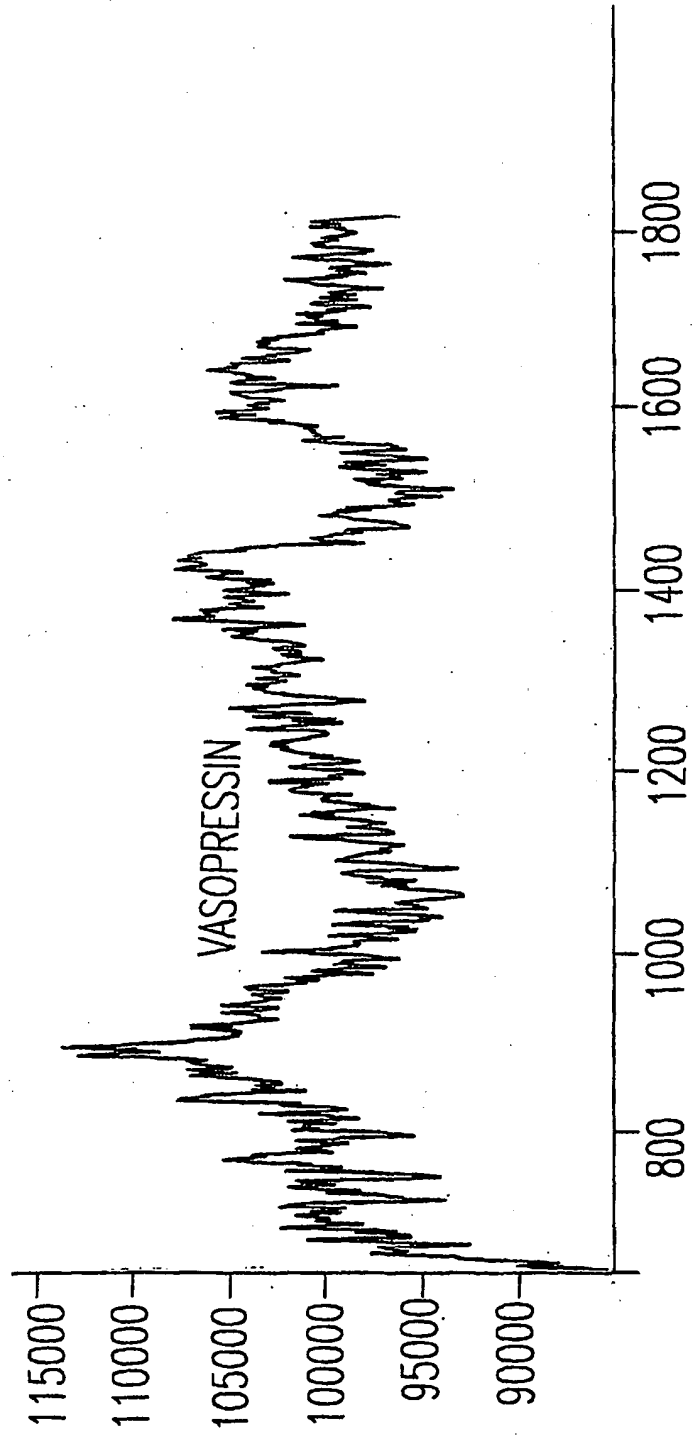


FIG.24

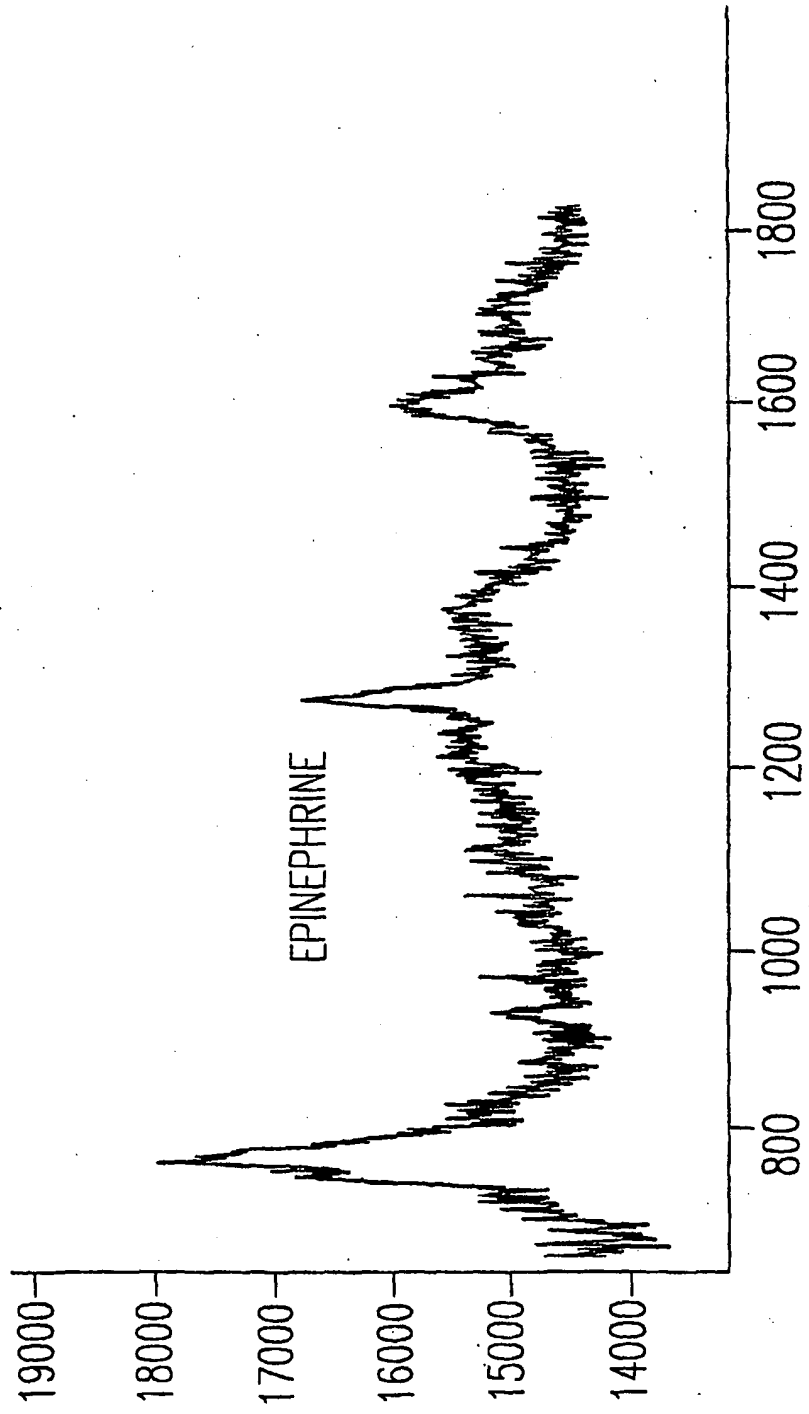


FIG.25

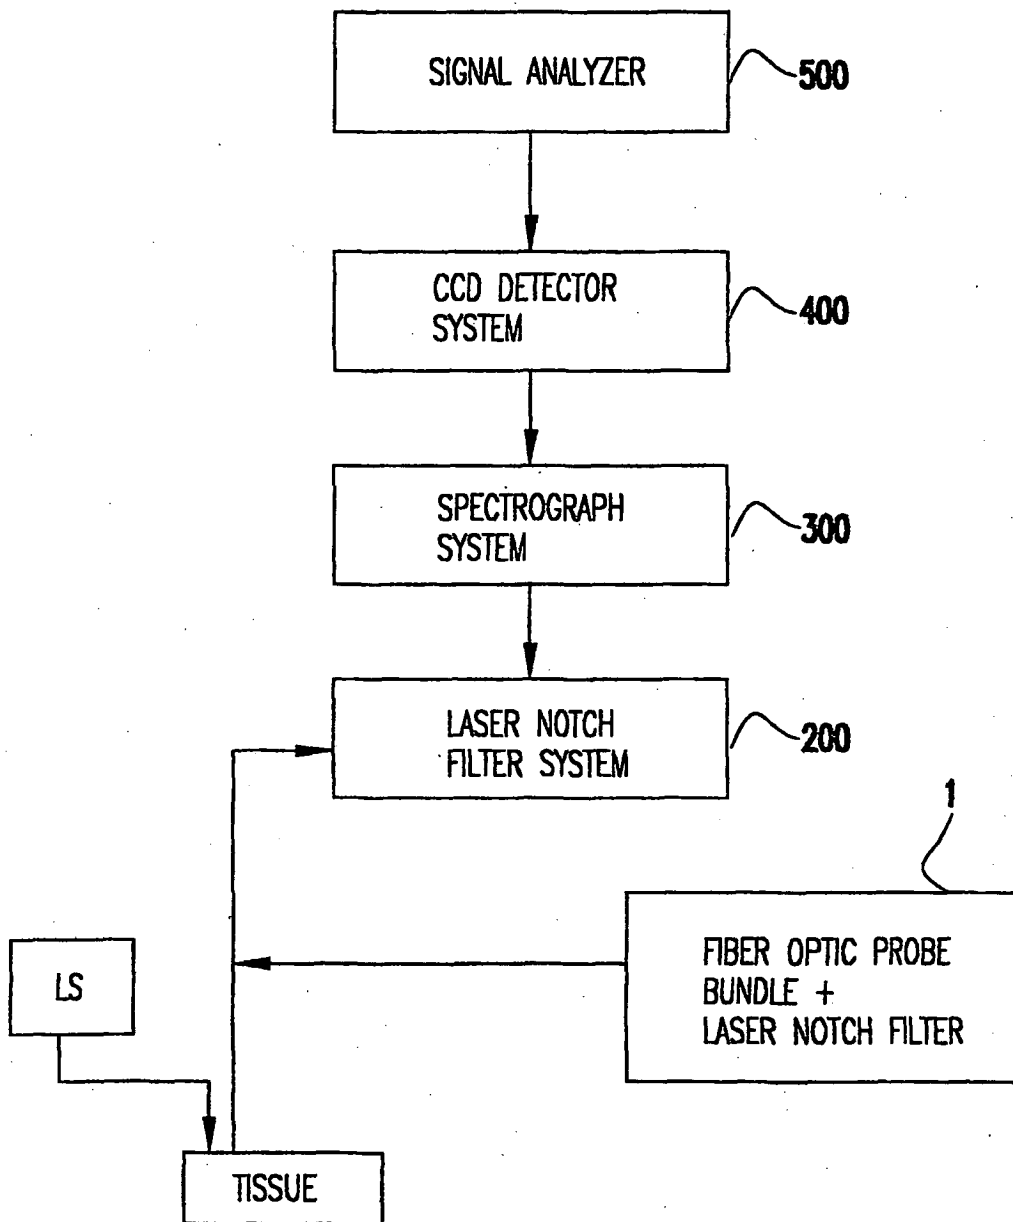


FIG.26A

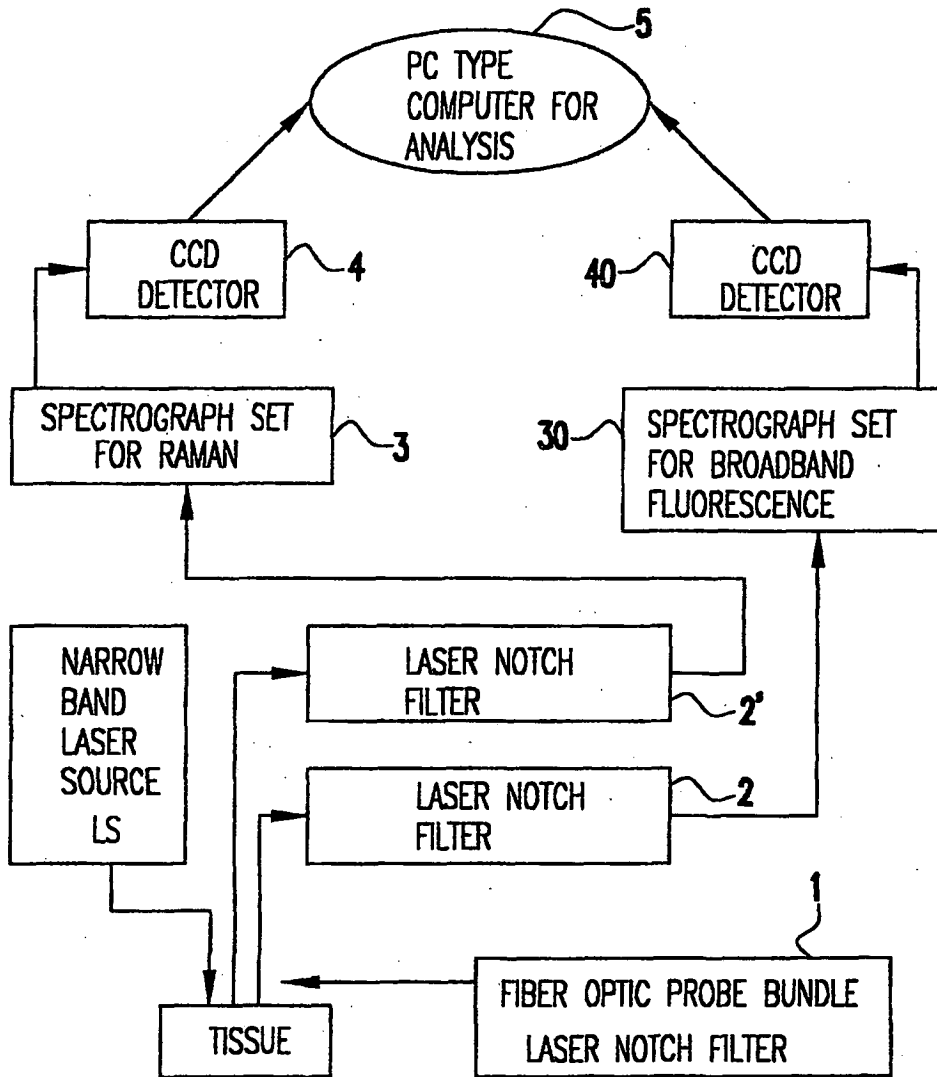


FIG.26B

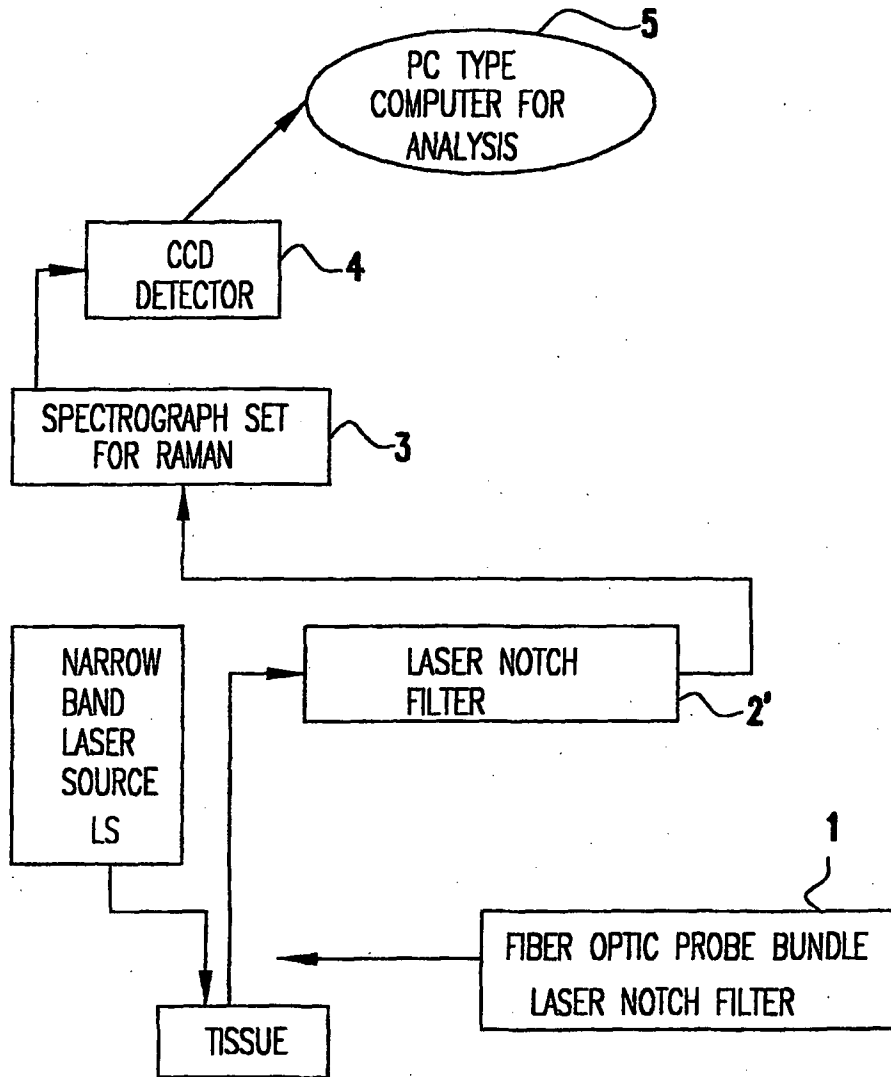


FIG.26C

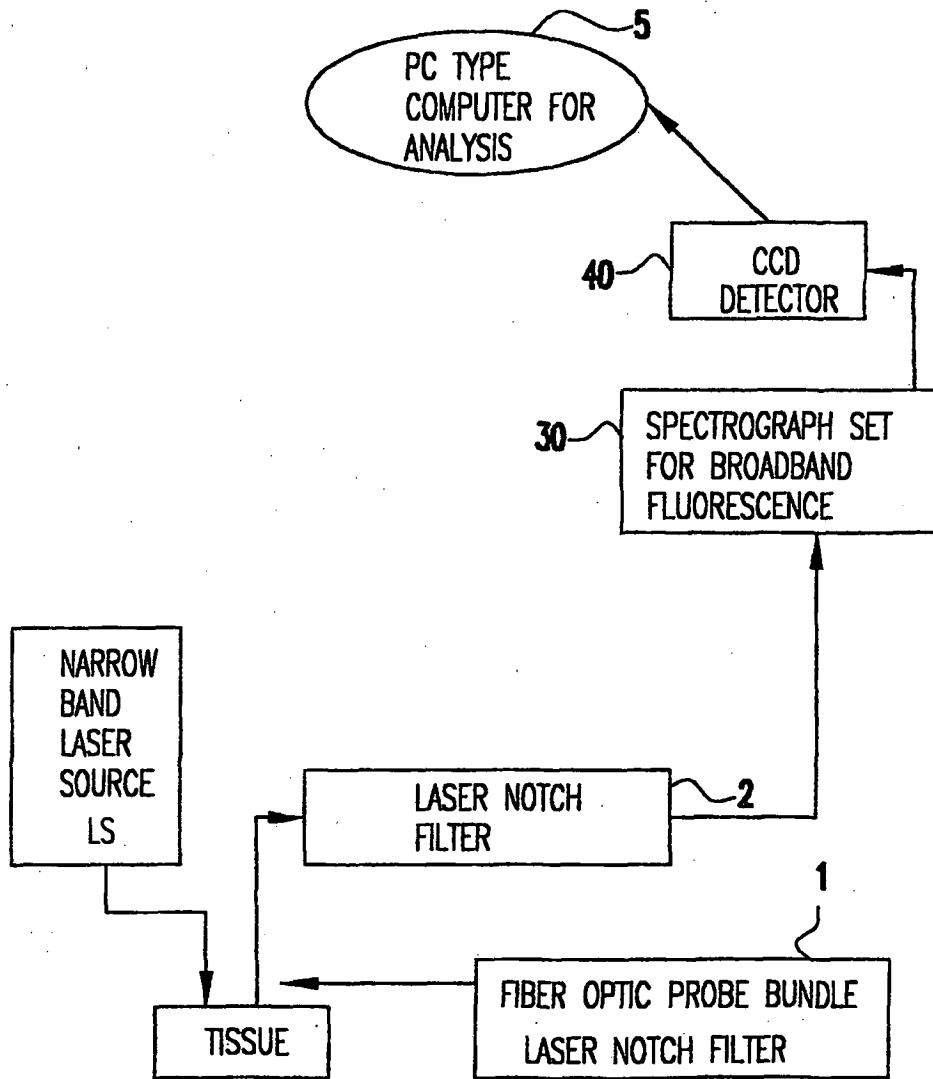


FIG.26D

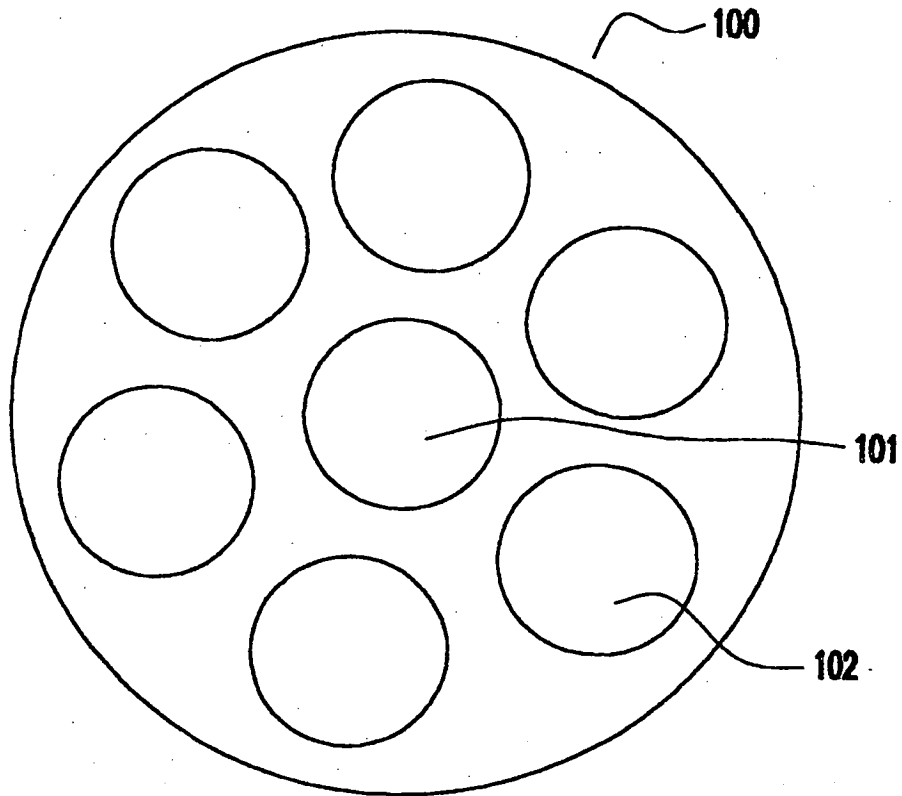


FIG.26E

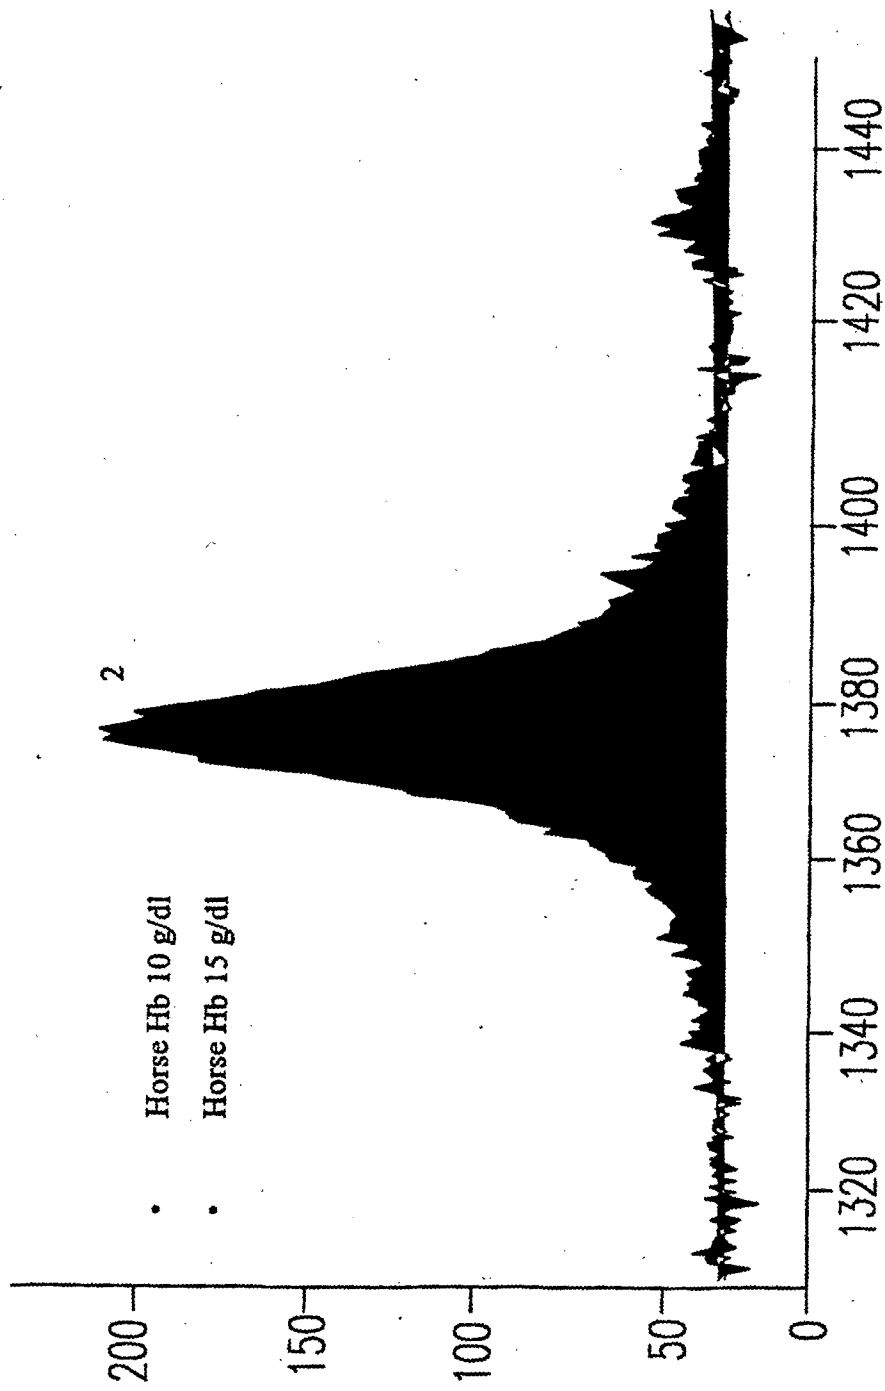


FIG.27

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Non-patent literature cited in the description

- Cellular metabolic consequences of altered perfusion. **HALJAMAE, H.** Update in Intensive Care and Emergency Medicine: Tissue oxygen utilization. Springer Verlag, 1991, 71-86 [0002] [0062]
- **ABOU-KHALIL, B. ; SCALEA, T.M. ; TROOSKIN, S.Z. ; HENRY, S.M. ; HITCHCOCK, R.** Hemodynamic responses to shock in young trauma patients; need for invasive monitoring. *Crit. Care Med.*, 1994, vol. 22, 633-639 [0002]
- **PORTER, J. ; IVATURY, R.** In search of optimal end points of resuscitation in trauma patients. *J. Trauma*, 1998, vol. 44, 908-914 [0003]
- **WARD, K.R. ; IVATURY, R.R. ; BARBEE, R.W.** Endpoints of resuscitation for the victim of trauma. *J. Intensive Care Med.*, 2001, vol. 16, 55-75 [0004]
- **WARD et al.** *J. INTENSIVE CARE MED.* [0004]
- **ABOU-KHALIL, B. ; SCALEA, T.M. ; TROOSKIN, S.Z. ; HENRY, S.M. ; HITCHCOCK, R.** Hemodynamic response to shock in young trauma patients: need for invasive monitoring. *Crit Care Med.*, 1994, vol. 22 (4), 633-9 [0004]
- **SCALEA, T.M. ; MALTZ, S. ; YELON, J. ; TROOSKIN, S.Z. ; DUNCAN, A.O ; SCALAFANI, S.J.** Resuscitation of multiple trauma and head injury: role of crystalloid fluids and inotropes. *Crit Care Med.*, 1994, vol. 22 (10), 1610-5 [0004]
- **IVATURY, R.R. ; SIMON, R.J. ; HAVRILIAK, D. ; GARCIA, C. ; GREEBARG, J. ; STAHL, W.M.** Gastric mucosal pH and oxygen delivery and oxygen consumption indices in the assessment of adequacy of resuscitation after trauma: a prospective, randomized study. *J. Trauma*, 1995, vol. 39 (1), 128-34 [0004]
- **SHOEMAKER, W.C. ; APPEL, P.L. ; KRAM, H.B.** Tissue oxygen debt as a determinant of lethal and nonlethal postoperative organ failure. *Crit. Care Med.*, 1988, vol. 16 (11), 1117-20 [0005]
- **SCALEA, T.M. ; HARTNETT, R.W. ; DUNCAN, A.O. ; ATRWEH, N.A. ; PHILLIPS, T.F. ; SCLAFANI, S.J. et al.** Central venous oxygen saturation: a useful clinical tool in trauma patients. *J. Trauma*, 1990, vol. 30 (12), 1539-43 [0007]
- **MCKINLEY, B.A. ; MARVIN R.G. ; COCANOUR, C.S. ; MOORE, F.A.** Tissue hemoglobin O₂ saturation during resuscitation of traumatic shock monitored using near infrared spectrometry. *J. Trauma*, 2000, vol. 48 (4), 637-42 [0007]
- **SIEGEMUND, M. ; VAN BOMMEL, J. ; INCE, C.** Assessment of regional tissue oxygenation. *Intensive Care Med.*, 1999, vol. 25 (10), 1044-60 [0007]
- **NAKAMOTO, K. ; CZERNUSZEWICZ, W.S.** Infrared Spectroscopy. *Methods in Enzymology*, 1993, vol. 226, 259-289 [0008]
- Application of NIR Spectroscopy to problems of tissue oxygenation. **PIANTADISU, C. ; PARSONS, W. ; GRIEBEL.** Update in Intensive Care and Emergency Medicine: Tissue oxygen utilisation. Springer Verlag, 1991, 41-44 [0008]
- **OWEN-REECE, H. ; SMITH, M. ; ELWELL, C.E. ; GOLDSTONE, J.C.** Near infrared spectroscopy. *Br J Anaesth*, 1999, vol. 82 (3), 418-26 [0008]
- **WEIL, M. ; NAKAGAWA, Y. ; TANG, W. et al.** Bilingual capnometry: A new noninvasive measurement for diagnosis and quantification of severity of circulatory shock. *Crit. Care Med.*, 1999, vol. 27, 1225-1229 [0009]
- **GAYESKI, T.E. ; HONIG, C.R.** Direct measurement of intracellular O₂ gradients; role of convection and myoglobin. *Adv Exp Med Biol*, 1983, vol. 159, 613-21 [0010]
- **VAN DER LAAN, L. ; COREMANS, A. ; INCE, C. ; BRUINING, H.A.** NADH videofluorimetry to monitor the energy state of skeletal muscle in vivo. *J. Surg. Res.*, 1998, vol. 74 (2), 155-60 [0013]
- **KINCAID, E.H. ; MILLER, P.R. ; MEREDITH, J.W. ; CHANG, M.C.** Enalaprilat improves gut perfusion in critically injured patients. *Shock*, 1998, vol. 9 (2), 79-83 [0014]
- **CATANIA, R.A. ; CHAUDRY, I.H.** Immunological consequences of trauma and shock. *Ann. Acad. Med. Singapore*, 1999, vol. 28 (1), 120-32 [0014]
- **RAMAN, C.V. ; KRISHNAN, K.S.** The colour of the sea. *Nature (London)*, 1928, vol. 121, 619 [0027]
- **HANLON, E.B. ; MANOHARAN, R. ; KOO, T.W. ; SHAFER, K.E. ; MOTZ, J.T. ; FITZMAURICE, M. et al.** Prospects for in vivo Raman spectroscopy. *Phys Med Biol*, 2000, vol. 45 (2), R1-59 [0027]
- **DIEM, M.** Introduction to modern vibrational spectroscopy. Wiley, 1993 [0027]
- **HANLON, E.B. ; MANOHARAN, R. ; KOO, T.W. ; SHAFER, K.E. ; MOTZ, J.T. ; FITZMAURICE, M. ; KRAMER, J.R. ; ITZKAN, I. ; DASARI, R.R. ; FELD, M.S.** Prospects for in vivo Raman spectroscopy. *Phys. Med. Biol.*, 2000, vol. 45, R1-R59 [0028]

- **SPIRO, T.G.** Resonance Raman spectroscopy: A new structure probe for biological chromophores. *Accts. Chem. Res.*, 1974, vol. 7, 339-344 [0032]
- **TERNER, J. ; EL-SAYE, M.A.** Time-resolved resonance Raman spectroscopy of photobiological and photochemical systems. *Accts. Chem. Res.*, 1985, vol. 18, 331-338 [0032]
- **J. TERNER ; T.G. SPIRO ; M. NAGUMO ; M.F. NICOL ; M.A. EL-SAYED.** Resonance Raman spectroscopy in the picosecond timescale: the CO hemoglobin photo-intermediate. *J. Amer. Chem. Soc.*, 1980, vol. 102, 3238-3239 [0040]
- **J. TERNER ; J.D. STONG ; T.G. SPIRO ; M. NAGUMO ; M.F. NICOL ; M.A. EL-SAYED.** Picosecond resonance Raman spectroscopic evidence for excited state spin conversion in carbonmonoxy-hemoglobin photolysis. *Proc. Natl. Acad. Sci. USA*, 1980, vol. 78, 1313-1317 [0040]
- **J. TERNER ; T.G. SPIRO ; D.F. VOSS ; C. PADDOCK ; R.B. MILES.** Picosecond resonance Raman spectroscopy of oxyhemoglobin photolysis. *J. Phys. Chem.*, 1982, vol. 86, 859-861 [0040]
- **LUCHETTE, F. ; ROBOINSON, B. ; FRIEND, L. ; MCCARTER, F. ; FRAME, S.B. ; JAMES, J.H.** Adrenergic antagonist reduce lactic acidosis in response to hemorrhagic shock. *J. Trauma*, 1999, vol. 46, 873-880 [0063]
- **SCHULZE, H.G. ; GREEK, L.S. ; BARBOSA, C.J. ; BLADES, M.W. ; GORZALKA, B.B. ; TURNER, R.F.B.** Measurement of some small-molecule and peptide neurotransmitters in-vitro using a fiber-optic probe with pulsed ultraviolet resonance Raman spectroscopy. *J. Neurosci. Meth.*, 1999, vol. 92, 15-24 [0064]
- **HAYWARD, R. ; LEFER, A.M.** Time course of endothelial-neutrophil interaction in splanchnic artery ischemia-reperfusion. *Am J Physiol*, 1998, vol. 275, H2080-6 [0078]
- **TAN, S. ; YOKOYAMA, Y. ; DICKENS, E. ; CASH, T.G. ; FREEMAN, B.A. ; PARKS, D.A.** Xanthine oxidase activity in the circulation of rats following hemorrhagic shock. *Free Radic Biol Med*, 1993, vol. 15 (4), 407-14 [0078]
- **JAKSCHIK, B.A. ; MARSHALL, G.R. ; KOURIK, J.L. ; NEEDLEMAN, P.** profile of circulating vasoactive substances in hemorrhagic shock and their pharmacologic manipulation. *J Clin Invest*, 1974, vol. 54 (4), 842-52 [0080]
- **LANZA, V. ; PALAZZADRIANO, M. ; SCARDULLA, C. ; MERCADANTE, S. ; VALDES, L. ; BELLANCA, G.** Hemodynamics, prolactin and catecholamine levels during hemorrhagic shock in dogs pretreated with ap prolactin inhibitor, (bromocriptine. *Pharmacol Res Commun.*, 1987, vol. 19 (4), 307-18 [0080]
- **YILMAZLAR, A. ; YILMAZLAR, T. ; OZCAN, B. ; KUTLAY, O.** Vasopressin, renin, and adrenocorticotrophic hormone levels during the resuscitation of hemorrhagic shock in dogs. *J Emerg Med*, 2000, vol. 18 (4), 405-8 [0080]
- **KITAJIMA, T. ; TANI, K. ; YAMAGUCHI, T. ; KUBOTA, Y. ; OKUHIRA, M. ; MIZUNO, T. et al.** Role of endogenous endothelin in gastric mucosal injury induced by hemorrhagic shock in rats. *Digestion*, 1995, vol. 56 (2), 111-6 [0080]
- **FUJIJOKA, S. ; ONO, Y. ; KANGAWA, K. ; OKADA, K.** Plasma concentration of adrenomedullin is increased in hemorrhagic shock in dogs. *Anesth Analg*, 1999, vol. 88 (2), 326-8 [0080]
- **LINDNER, K.H. ; STROHMENGER, H.U. ; ENSINGER, H. ; HETZEL, W.D. ; AHNEFELD, F.W. ; GEORGIEFF, M.** Stress hormone response during and after cardiopulmonary resuscitation. *Anesthesiology*, 1994, vol. 77 (4), 662-8 [0080]
- **LINDNER, K.H. ; HAAK, T. ; KELLER, A. ; BOTHNER, U. ; LURIE, K.G.** Release of endogenous vasopressors during and after cardiopulmonary resuscitation. *Heart*, 1996, vol. 75 (2), 145-50 [0080]
- **SCHULZE, H.G. ; GREEK, L.S. ; BARBOSA, C.J. ; BLADES, M.W. ; GORZALKA, B.B. ; TURNER, R.F.** Measurement of some small-molecule and peptide neurotransmitters in-vitro using a fiber-optic probe with pulsed ultraviolet resonance Raman spectroscopy. *J. Neurosci Methods*, 1999, vol. 92 (1-2), 15-24 [0081]

专利名称(译)	使用紫外线，近紫外和近红外共振拉曼光谱和荧光光谱对组织询问休克状态，危重疾病和其他疾病状态		
公开(公告)号	EP1304955B1	公开(公告)日	2008-12-17
申请号	EP2001951068	申请日	2001-07-13
[标]申请(专利权)人(译)	弗吉尼亚联邦大学		
申请(专利权)人(译)	弗吉尼亚联邦大学		
当前申请(专利权)人(译)	弗吉尼亚联邦大学		
[标]发明人	WARD KEVIN R BARBEE R WAYNE TERNER JAMES IVATURY RAO R HAWKRIDGE FRED		
发明人	WARD, KEVIN, R. BARBEE, R., WAYNE TERNER, JAMES IVATURY, RAO, R. HAWKRIDGE, FRED		
IPC分类号	A61B5/00 A61B6/00 G01N21/65		
CPC分类号	G01N21/65 A61B5/0071 A61B5/0075 A61B5/0084 A61B5/0086 A61B5/14539 A61B5/14546 A61B5/1455 A61B5/14551 A61B5/412 A61B5/445		
优先权	60/218055 2000-07-13 US		
其他公开文献	EP1304955A4 EP1304955A2		
外部链接	Espacenet		

摘要(译)

在急诊医学患者中，准确测量非休克，非缺血性，非炎症，非组织损伤，非免疫功能障碍状况的变化或缺乏是非常重要的，并且实际上提供了实时的方法。使用拉曼和/或荧光光谱以高精度准确表征患者的病情。测量时间大约为秒。使用拉曼光谱检查组织实现高精度测量。可以使用NADH荧光光谱法同时进行询问。对于微创，测量可以是非侵入性的。可以检测休克的临床前（超早期）状态，可以确定严重程度，并且可以确定旨在解决休克，缺血，损伤，炎症或免疫功能障碍状态的各种治疗的有效性。

