

(19)



(11)

**EP 1 699 514 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**25.09.2019 Bulletin 2019/39**

(51) Int Cl.:  
**A61M 16/00** <sup>(2006.01)</sup> **A61M 16/06** <sup>(2006.01)</sup>  
**A61B 5/00** <sup>(2006.01)</sup>

(21) Application number: **04802134.9**

(86) International application number:  
**PCT/AU2004/001833**

(22) Date of filing: **24.12.2004**

(87) International publication number:  
**WO 2005/063323 (14.07.2005 Gazette 2005/28)**

(54) **MECHANICAL VENTILATION IN THE PRESENCE OF SLEEP DISORDERED BREATHING**  
MECHANISCHE BEATMUNG BEI ATEMSTÖRUNGEN IM SCHLAF  
VENTILATION MECANIQUE POUR RESPIRATION PERTURBEE PENDANT LE SOMMEIL

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU MC NL PL PT RO SE SI SK TR**

- **BUCKLEY, Mark**  
North Ryde, New South Wales 2113 (AU)
- **SCHINDHELM, Klaus Henry**  
North Ryde, New South Wales 2113 (AU)

(30) Priority: **29.12.2003 US 533411 P**  
**18.02.2004 US 545658 P**

(74) Representative: **Vossius & Partner**  
**Patentanwälte Rechtsanwälte mbB**  
**Siebertstrasse 3**  
**81675 München (DE)**

(43) Date of publication of application:  
**13.09.2006 Bulletin 2006/37**

(73) Proprietor: **ResMed Pty Ltd**  
**Bella Vista, NSW 2153 (AU)**

(56) References cited:  
**EP-B1- 0 188 071** **EP-B1- 0 956 877**  
**WO-A1-00/47260** **WO-A1-03/039637**  
**WO-A1-2004/078246** **AU-B2- 703 829**  
**DE-A1- 10 164 446** **GB-A- 2 294 400**  
**JP-A- 2001 259 036** **JP-A- 2004 105 230**  
**US-A- 5 503 146** **US-A- 5 535 738**  
**US-A- 6 041 780** **US-B1- 6 213 119**  
**US-B1- 6 484 719** **US-B1- 6 532 960**

- (72) Inventors:
- **DOUGLAS, Robert**  
North Ryde, New South Wales 2113 (AU)
  - **UJHAZY, Anthony John**  
North Ryde, New South Wales 2113 (AU)
  - **RICHARDS, Glenn**  
North Ryde, New South Wales 2113 (AU)

**EP 1 699 514 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description**

[0001] This application claims the priority of U.S. provisional application No. 60/533,411 filed on December 29, 2003.

5 **1. FIELD OF THE INVENTION**

[0002] This invention relates to mechanical ventilation of sleep disordered breathing (SDB).

10 **2. BACKGROUND OF THE INVENTION**

[0003] A comprehensive background discussion of mechanical ventilation can be found in "Principles and Practice of Mechanical Ventilation" (1994) Edited by Martin J Tobin, published by McGraw-Hill Inc., ISBN 0-07-064943-7.

[0004] The use of nasal Continuous Positive Airway Pressure (CPAP) to treat Obstructive Sleep Apnea (OSA) was invented by Colin Sullivan, see U.S. Patent No. 4,944,310. Generally, the treatment involves providing a supply of air or breathable gas from a blower to a patient via an air delivery conduit and a patient interface. While treatment is effective, some patients find it uncomfortable. Improving patient comfort and compliance is a continuing challenge.

[0005] One way to improve comfort is to provide a more comfortable patient interface. In this regard, the ResMed MIRAGE™ masks have provided significant improvement in comfort. See U.S. Patent Nos. 6,112,746; 6,357,441; 6,581,602 and 6,634,358. A more recent development is the ResMed MIRAGE™ ACTIVA™ mask series. See International Patent Application WO 2001/97893.

[0006] In the early days of nasal CPAP systems for treating OSA, patients were first titrated in a clinical study to determine an optimal treatment pressure. Titration involves a patient sleeping overnight in a clinic and being tested with a mask and CPAP device. The treatment pressure provided by the CPAP device is adjusted until apneas are eliminated. The treatment pressure is usually in the range of 4-20cmH<sub>2</sub>O. A device would be set to that pressure and given to the patient to take home. A subsequent development was the automatically adjusting device that a patient could take home. The automatically adjusting device will raise and/or lower the treatment pressure based on indications of obstructive sleep apnea, such as snoring. Such devices are sometime generically referred to as Automatic Positive Airway Pressure (APAP) devices. See U.S. Patent Nos. 5,245,995; 6,398,739; and 6,635,021.

[0007] Another type of nasal CPAP device provides a first pressure during inhalation (sometimes termed an IPAP) and a second, lower pressure during exhalation (sometimes termed and EPAP). Examples of these include the ResMed VPAP™ series, and the Respironics BiPAP series. Bilevel CPAP devices may be prescribed for patients who do not comply with single pressure CPAP devices. Some patients perceive that the lower pressure during exhalation is more comfortable, at least while they are awake. A difficulty with these devices is deciding how to set the IPAP and EPAP pressures. If the EPAP is too low it may be insufficient to prevent obstructions, hence some clinicians may set the EPAP pressure to the pressure titrated during the sleep study. In those patients, the IPAP pressure, and thus the average pressure will be higher that that required to eliminate apneas.

[0008] Another form of automatically adjusting CPAP device is the ResMed AUTOSET™ SPIRIT™ device. In this device, the CPAP pressure is automatically increased or decreased in accordance with indications of flow limitation, such as flow flattening, snore, apnea and hypopnea. See U.S. Patent Nos. 5,704,345; 6,029,665; 6,138,675; and 6,363,933. An advantage of an automatically adjusting system is that over time the treatment pressure required may vary for a particular patient and a correctly functioning automatic system can obviate the need the patient to return for a subsequent sleep study. These patents also describe a method and apparatus for distinguishing between so-called "central" and obstructive apneas.

[0009] Another device for treating certain types of Sleep Disordered Breathing such as Cheyne-Stokes Respiration (CSR) is the ResMed AutoCS™ device. Among other things, this device provides a supply of air or breathable gas with a smooth comfortable waveform, sophisticated tracking of the patient's respiratory phase, and servo-control of patient ventilation. See U.S. Patent Nos. 6,484,719; 6,532,957; and 6,575,163 (the "AutoVPAP" patents). See also U.S. Patent No. 6,532,959.

[0010] Some OSA patients find treatment with the above devices uncomfortable and they become non-compliant with the therapy. Other patients such as cardiovascular patients with Congestive Heart Failure, patients with REM Hypoventilation, and patients with Respiratory Insufficiency could also benefit from a more comfortable and/or effective form of therapy.

[0011] US 6,213,119 B1 relates to an apparatus for the supply of breathable gas cyclically at an inspiratory pressure and a lower expiratory pressure substantially in synchronism with a patient's respiration. A controller detects transitions between inspiration and expiration via a flow signal to discriminate between the respiratory phases of the patient. A counter counts a first time duration commencing from the last transition to inspiration and whereby if the first time duration elapses before a transition to expiration is detected, the controller initiates the supply of a given expiratory pressure. Furthermore, a second counter counts a second time duration commenced from the last transition to inspiration detected

and signals the turbine to supply a given inspiratory pressure until the second time duration has elapsed even if during the second time duration a transition to expiration by the patient has occurred.

5 [0012] US 5,535,738 A relates to an apparatus for treatment of Obstructive Sleep Apnea Syndrome (OSAS), Chronic Obstructive Pulmonary Disorder (COPD) and other respiratory disorders. The apparatus applies separate and independent gains to flow rates of pressurized gas delivered to a patient during inspiratory and expiratory phases of a respiratory cycle to deliver the pressurized gas in proportion to the respective gains during inspiration and expiration. A base pressure may be applied in addition to the gain-modified pressures and an elevated pressure profile may be employed to assist or control inspiration.

10 [0013] US 5,503,146 A relates to continuous positive airway pressure (CPAP) respiratory therapy apparatus for treatment of apnea, hypopnea and other sleep disorders, and particularly to a standby control for automatically operating an air blower in CPAP apparatus. A blower is connected through a hose and a mask, such as a nasal mask or a nasal cannula, to the patient's respiratory airway. Initially, the blower is in a standby mode in which it is either turned off or, preferably, operated at a low speed. When a patient starts breathing through the mask, the blower is automatically switched to an operating mode. In the operating mode, the blower may be controlled to initially supply a low air pressure to the mask which either is increased after a sufficient time delay to allow the patient to fall asleep or is increased in response to the detection of a respiratory event such as apnea or hypopnea.

15 [0014] US 6,041,780 A relates to an apparatus for ventilating a patient wherein the inspiratory positive airway pressure (IPAP) is adjusted as a function of minute volume. The IPAP is gradually adjusted over extended periods of time in small increments to conform the patient's minute volume to a prescribed value. This gentle but effective approach ensures adequate ventilation while minimizing discomfort to the patient thereby rendering the system ideal for treating sleep disordered breathing in the homecare environment.

20 [0015] US 6,532,960 B1 relates to an apparatus and method for a bi-level positive airway pressure support in which the rise time from the expiratory positive airway pressure to the inspiratory positive airway pressure is automatically controlled by the pressure support system. The pressure support system includes a sensor, a control system, and a pressure generating system. The sensor monitors the patient's respiration to detect respiratory events, such as an apnea, hyponea or other disturbance, and the control system responds to the sensor information to adjust the rise time from the expiratory positive airway pressure to the inspiratory positive airway pressure gas pressure to maximize patient comfort and pressure support treatment effectiveness.

### 30 3. SUMMARY OF THE INVENTION

[0016] The invention provides apparatus as set out in the accompanying claims.

### 35 4. BRIEF DESCRIPTION OF THE DRAWINGS

[0017]

FIG. 1 depicts a structure of the preferred ventilator apparatus;

40 FIGS. 2A to 2D illustrate some exemplary waveforms delivered;

FIG. 3 is a pressure waveform template that is a function of a phase variable;

45 FIG. 4 is an inspiratory table of the inspiratory portion (0 - 0.5) of the waveform of the graph of FIG. 3;

FIG. 5 is an expiratory table of the expiratory portion (0.5 - 1) of the waveform of the graph of FIG. 3;

FIG. 6 is a block diagram;

50 FIG. 7 is another block diagram illustrating an application of pressure to a ventilator;

FIGS. 8A and 8B are illustrative functions for controlling swing as a function of an automatic SDB pressure determination process;

55 FIG. 9 is a graph illustrating control of median pressure by an automated SDB pressure detection process; and

FIG. 10 is a graph illustrating mouth leak detection.

## 5. DETAILED DESCRIPTION

### 5.1 HARDWARE

5 [0018] A device in accordance with an embodiment of the invention comprises a blower and blower-controller. The blower can deliver a supply of air at positive pressure 2-40 cmH<sub>2</sub>O, but generally in the range of 4-25 cmH<sub>2</sub>O to a patient interface via an air delivery conduit. The device also includes a flow sensor to measure the flow of air along the conduit, and pressure sensors to measure the pressure of air at the blower outlet. In one form, the device alternatively includes an additional pressure sensor to detect the pressure in the patient interface.

10 [0019] For example, a preferred embodiment of the invention is illustrated in FIG. 1. The ventilator device may include a servo-controlled blower 2, a flow sensor 4f, pressure sensor 4p, a mask 6, and an air delivery conduit 8 for connection between the blower 2 and the mask 6. Exhaust gas is vented via exhaust 13. Mask flow may be measured by a flow sensor, such as a pneumotachograph and differential pressure transducer to derive a flow signal F(t). Alternatively, the pneumotachograph may be replaced by a bundle of small tubes aligned in parallel with the flow from the blower with the pressure difference measured by the differential pressure transducer across the bundle. Mask pressure is preferably measured at a pressure tap using a pressure transducer to derive a pressure signal P<sub>mask</sub>(t). The pressure sensor 4p and flow sensor 4f have been shown only symbolically in FIG. 1 since it is understood that those skilled in the art would understand how to measure flow and pressure. Flow F(t) and pressure P<sub>mask</sub>(t) signals are sent to a controller or microprocessor 15 to derive a pressure request signal P<sub>Request</sub>(t). The controller or processor is configured and adapted to perform the methodology described in more detail herein. The controller or processor may include integrated chips, a memory and/or other instruction or data storage medium to implement the control methodology. For example, programmed instructions with the control methodology are either coded on integrated chips in the memory of the device or loaded as software. As those skilled in the art will recognize, analog devices may also be implemented in the control apparatus. The apparatus of FIG. 1 includes other sensors, communication interfaces and displays, a servo, etc., functional blocks the details of which are not necessary for an understanding of the present invention.

### 5.2 SYNCHRONY: TRIGGERING, CYCLING & PHASE DETERMINATION

30 [0020] In a device which varies treatment pressure throughout the respiratory cycle of the patient, it is more comfortable for the patient if the device varies the pressure in synchrony with patient efforts. As illustrated in FIG. 6, an overall device 64 constructed in accordance with the principles of our invention includes an automated therapeutic treatment pressure determination component module 60 which determines a treatment pressure component to treat SDB, and a waveform module 62 or process for setting or selecting a waveform (square, rounded, smooth, etc.) for modulating pressure in conjunction with the patient's respiratory cycle. Typically, the device will include a synchrony or triggering module 68 (controlled by fuzzy logic, pressure, patient effort, etc.) for determining states or the phase within the patient's respiratory cycle. Optionally, a central apnea detector 66 may be included.

35 [0021] In delivering pressure, the triggering module monitors the patient to make a determination of the patient's respiratory phase in order to synchronise the blower output with the patient's efforts. In one form, the determination is whether the patient is inhaling or exhaling (a discrete variable). In another form, the determination is of the proportion into the overall respiratory cycle of the patient (a periodic variable). Determination of phase may be made by some combination of pressure, flow and effort sensors. For example, in one form, when mask pressure drops below a threshold, the transition to inhalation is taken to have occurred and correspondingly when mask pressure rises above a threshold, the transition to exhalation is taken to have occurred. In another form, when patient respiratory flow exceeds a threshold, inhalation is taken to have started and when patient respiratory flow falls below a threshold, exhalation is taken to have started. In another form, patient respiratory phase is determined from analysing the shape of the respiratory flow curve and making a number of determinations as to the extent to which it is early inspiration, middle inspiration, late inspiration, early exhalation, mid-exhalation and late exhalation. See U.S. Patent Nos. 6,484,719; 6,532,957; and 6,575,163. Once a determination of phase has been made, the shape of waveform to be delivered can be decided.

40 [0022] In one embodiment, a phase determination may be based on elapsed time of the particular portion of the cycle (inspiration or expiration) relative to a predicted total time for that particular portion of the cycle. For example, the phase within the respiratory cycle is determined as a ratio of the elapsed time to the expected total time. Since the total time for the current cycle is not yet known, it is predicted by using an average time taken from a number of previous breaths, preferably taken from the previous five breaths of the patient. In the preferred embodiment, irregular breaths are excluded from the average. Thus, breaths of less than 150 milliseconds indicative of a cough or hiccup are excluded. Those skilled in the art will understand how to determine such a five breath average from a flow signal.

45 [0023] With the determination of a continuous phase and utilizing the waveform module 62, smooth pressure changes are then implemented utilizing a pressure waveform template for inspiration and expiration that may preferably be stored in tables or arrays. In general, the tables store scaling factors for a predetermined breath length that when multiplied by

a pressure amplitude in sequence will result in a pressure waveform that is represented by the scaling factors. Versions of these tables are illustrated in FIGS. 4 and 5 based on the smooth waveform of FIG. 3. As those skilled in the art will recognize, the tables may be substituted by mathematical equations rather than relying on a look-up operation. Moreover, although a sinusoidal rise/exponential decay curve is shown, the template may represent any shape of waveform, such as a square wave illustrated by the dashed lines of FIG. 3. Use of the phase variable ensures that each scaling factor (SF) of the table is utilized at an appropriate time in the patient's respiratory cycle, thereby compressing or expanding the time-length of the template. In this regard, the determined phase variable (elapsed time over total expected time) is used to scale the time-length of the template.

[0024] For these ends, a look-up operation that returns a pressure modulating function (Ins\_Waveform) utilizing such a phase and an inspiratory table or array may be accomplished with the following:

$$\text{Ins\_Waveform} = \text{Inspiratory\_Table} (\text{I-Location})$$

where:

Inspiratory\_Table is a function that returns a scaling factor from the table or array at a particular location determined by the I-Location function;

I-Location is a function that essentially identifies an inspiration phase variable within the current inspiration (i.e., the ratio of the elapsed inspiration time to the expected total inspiration time) of the patient as this relates to selecting an appropriate scaling factor from the table that will permit the delivered pressure to be modulated like that of a normal inspiration within the time scale of the patient's current predicted inspiration.

[0025] To accomplish this, the function returns an index of the inspiratory table as a function of (a) the current elapsed time of the inspiration (t\_switch), (b) the time-length of the inspiratory portion of the waveform of the waveform template, which may be the number of table or array entries over which the inspiratory portion of the waveform template has been recorded in the table (total\_entries); and (c) the predicted time for the inspiration portion of the respiratory cycle, i.e., the average inspiratory time (ave\_insp\_time). This index may be derived by the following formula:

$$\text{index} = \text{round} (t\_switch * \text{total\_entries} / \text{ave\_insp\_time})$$

[0026] Similarly, the look-up operation (Exp\_Waveform) on the expiratory table or array may be accomplished with the following functions:

$$\text{Exp\_Waveform} = \text{Expiratory\_Table} (\text{E-Location})$$

where:

Expiratory\_Table is a function that returns a scaling factor from the expiration table or array at a particular location determined by the E-Location function;

Much like the I-location function described above, E-Location is a function that essentially identifies an expiration phase variable within the current expiration of the patient (i.e., the ratio of the elapsed expiration time to the expected total expiration time) for the purpose of selecting an appropriate scaling factor from the table that will permit the delivered pressure to be modulated like that of a normal expiration but within the time scale of the patient's current predicted expiration.

[0027] To accomplish this, the function identifies an index of the expiratory table as a function of (a) the current elapsed time of the expiration (t\_switch), (b) the time-length of the expiratory portion of the waveform of the waveform template, which may be the number of table or array entries over which the expiratory portion of the waveform template has been recorded in the table (total\_entries); and (c) the predicted time for the inspiration portion of the respiratory cycle, i.e., the average inspiratory time (ave\_exp\_time). The index may be derived by the following formula:

$$\text{index} = \text{round} (t\_switch * \text{total\_entries} / \text{ave\_exp\_time})$$

Those skilled in the art will recognize that other formulas may be utilized for modulating the ventilation pressure, such as a more simple cycling and triggering between an IPAP and EPAP.

### 5.3 INDICATIONS OF SLEEP DISORDERED BREATHING (SDB)

[0028] There are a number indications which can be used to detect sleep disordered breathing including snore, apnea, hypopnea and the shape of the inspiratory flow-time curve.

#### 5.3.1 Snore

[0029] Snoring can be detected by a number of techniques as known in the art. For example, US Patents 5,245,995 (Sullivan et al.) and 5,704,345 (Berthon-Jones). For example a flow signal can be band-pass filtered in the frequency range of 30-300Hz and the intensity of the resultant signal determined.

[0030] Having detected snoring, a snore index can be calculated as described in the above patents. The index can be based on the intensity, frequency and duration of snoring. A "snore prevention pressure" can be defined as the minimum CPAP pressure necessary to prevent snoring.

#### 5.3.2 Apneas & hypopneas

[0031] Apneas can be detected using a number of techniques as known in the art. For example, US Patent 5,704,345 (Berthon-Jones) describes an apnea detector as follows: The average flow signal variance calculated over a moving time window is compared with a threshold by a level detector, to generate an "airflow-ceased" trigger. This starts a timer. If the trigger persists for more than 10 seconds, a comparator declares an apnea. The threshold may be a fixed value, typically 0.1 l/sec, or may be a chosen percentage (typically 10 or 20%) of the average ventilation over the last several minutes (typically 5 minutes). For convenience, instead of comparing the threshold with the square root of the variance, one can square the threshold, and compare with the variance directly.

[0032] Conversely, if airflow resumes before 10 seconds lapses, the timer is reset and no apnea is declared.

[0033] In one form, upon detection of an apnea, the device increases pressure until the apnea stops, or a predefined threshold is reached. In this way the pressure does not exceed safe levels. The amount of the increase in pressure can vary upon the pressure at which an apnea has occurred and the duration of the apnea. See US Patent 6,367,474 (Berthon-Jones et al.)

[0034] Hypopneas can be similarly detected, however with a higher threshold, such as 50% of the average ventilation.

#### 5.3.3 Flow limitation

[0035] Flow limitation can be detected by a number of techniques as known in the art. For example see US Patent 5,704,345 (Berthon-Jones) which describes using various flattening indices such as based on the mid-portion of the inspiratory flow-time curve. Other flattening indices are known. See US 6,814,073 (Wickham). A flow limitation prevention pressure can be defined as the minimum CPAP pressure necessary to prevent flow limitation. This pressure is not predetermined, but calculated continuously in conjunction with various flow flattening indices. Pressure is increased until the indices indicate that flattening has been eliminated. The pressure level at which the indices indicate that flattening is eliminated is taken to be the current "flow limitation prevention pressure". In one form of our invention, the current "flow limitation prevention pressure" is automatically decreased with time unless an indication of flow limitation is detected.

### 5.4 WAVEFORM SHAPE

[0036] Accordingly, the blower can deliver a generally square-shaped waveform, similar to that provided by the ResMed VPAP™ Series or a more rounded waveform, similar to that provided by the ResMed AUTOSET CS™ product (see U.S. Patent No. 6,532,959), for example, having a sinusoidal rise and exponential decay. Furthermore, the blower can adjust the shape of the waveform between square and more rounded to balance comfort and effectiveness (See U.S. Patent No. 6,553,992). In one form, for example, when delivering a generally square wave, the device provides a higher pressure during an inspiratory portion of the patient's respiratory cycle (IPAP) and a lower pressure during an expiratory portion of the patient's respiratory cycle (EPAP). In another form, for example, when delivering a more rounded waveform, a SWING and pressure setting are determined. The SWING is the difference between the highest and lowest pressures delivered to the patient. The pressure setting could be the base pressure in one form, or the peak pressure in another form.

## 5.5 SOME EMBODIMENTS OF OUR INVENTION

### 5.5.1 First Embodiment: Automatic IPAP

5 [0037] In accordance with a first embodiment of the invention, a device is adapted to provide a generally square waveform having settings for IPAP and EPAP in a manner similar to ResMed's VPAP III device. The device has a clinician-settable pressure setting for the difference between IPAP and EPAP,  $\Delta P$  (sometimes called Swing). The device monitors patient flow and determines a treatment pressure using the same algorithm as ResMed's AUTOSET SPIRIT device. See US Patent 5,704,345. Upon detection of the beginning of inspiration, as described above, the device provides  
10 a supply of air at the treatment pressure (IPAP = treatment pressure) and maintains that pressure throughout the inspiratory portion of the patients breathing cycle. Upon detection of the beginning of exhalation, the device decreases the supplied pressure to the treatment pressure less  $\Delta P$ .

[0038] In this way the advantages of the automatically adjusting CPAP algorithm are brought to a bi-level CPAP device.

### 15 5.5.2 Second Embodiment: Automatic EPAP or EEP

[0039] A second embodiment of the invention is similar to the first embodiment, except that the End Expiratory Pressure (EEP) or the EPAP pressure is automatically adjusted, and the IPAP is a fixed delta pressure above the EPAP.

### 20 5.5.3 Third Embodiment: Automatic mean pressure

[0040] A third embodiment of the invention is similar to the first embodiment, except that the mean or median pressures are automatically adjusted, and there is a fixed delta pressure between IPAP and EPAP.

### 25 5.5.4 Fourth embodiment: Automatic Swing Control

[0041] In accordance with another aspect of the invention, the therapeutic treatment pressure is used to control the pressure difference between IPAP and EPAP, or the "swing". For example, when the device determines that the treatment pressure is small, e.g., 5 cmH<sub>2</sub>O, then the swing is set to a small value, e.g., 0 or 1 cmH<sub>2</sub>O, and when the treatment  
30 pressure is large, e.g., 15cmH<sub>2</sub>O, the swing is set to a larger value, e.g., 3 or 4 cmH<sub>2</sub>O. In this way a device in accordance with the invention can be controlled to ensure that pressure never drops below a threshold, for example, 4 or 5 cmH<sub>2</sub>O. Such a form of control is illustrated by the function of FIG. 8A in which the swing is set as a function of detected therapeutic treatment pressure (APAP Treatment Pressure). An alternative function is illustrated in FIG. 8B in which the swing is restricted from falling below a minimum such as 1 cmH<sub>2</sub>O.

35 [0042] As illustrated in FIG. 7, if an event of central apnea is detected, swing may be increased or decreased based on several conditions. For example, it may be reduced if partial obstruction is not detected. Alternatively, if based on an historic analysis of flow data performed by the device or a classification preset by a clinician, the current patient is a hypoventilator (has experienced hypoventilation), the swing may be increased, for example, by a step up in the swing by a predetermined amount. Alternatively, if based on an historic analysis of flow data performed by the device or  
40 a classification preset by a clinician the current patient is a hyperventilator or CV patient, the swing may be decreased, for example, by stepping down the swing by a predetermined amount.

### 5.5.5 Fifth embodiment: "Shark-fin" waveform

45 [0043] A fifth embodiment of the invention is similar to embodiments one to three, except that instead of providing a generally square pressure-time waveform, the waveform has a "shark-fin" shape as indicated in Fig. 2D, 3, 4 & 5.

### 5.5.6 Sixth Embodiment: Automatic IPAP and EPAP

50 [0044] In accordance with a sixth aspect of the invention, IPAP and EPAP are separately automatically adjusted. In this form of the invention, two pressure levels are calculated automatically. The first pressure is the minimum pressure necessary to prevent apneas and hypopneas. The second pressure is the minimum pressure necessary to prevent flow flattening. The EEP or EPAP is set to the first pressure and the IPAP is set to the second pressure.

[0045] The first pressure is calculated using the apnea and snore detectors described above. The second pressure is calculated from flow flattening or roundness indices as described above. The second pressure is controlled to be at  
55 least equal to the first pressure, preferably 1-2 cmH<sub>2</sub>O greater than the first pressure. In addition there is a predetermined maximum difference between the first and second pressures.

[0046] In one form, absent an indication of apnea or hypopnea the EPAP pressure is decreased. Similarly in one form,

absent an indication of flow flattening the IPAP pressure is decreased.

5.5.7 Other embodiments

5 [0047] The minimum pressure,  $P_0$ , delivered to the patient may be automatically controlled in conjunction with the pressure calculated by the automatic algorithms  $P_{therapeutic}$  and an amplitude,  $A$ , calculated from the desired delta pressure between IPAP and EPAP. With regard to the preferred pressure delivery formula  $P(t)$  illustrated above, such implementations may be achieved by setting  $P_0$  in alternative ways as follows:

10

$$P_0 = \begin{cases} P_{therapeutic} \\ P_{therapeutic} - A \\ P_{therapeutic} - \frac{A}{2} \\ P_{therapeutic} - kA \end{cases}$$

15

20

[0048] In the first, the therapeutic adjustments generated from the SDB detection routine discussed above are applied to the end expiratory or baseline pressure. In the second, therapeutic adjustments are applied to the peak or end inspiratory pressure. In the third, therapeutic pressure is applied to the mean. Those skilled in the art will recognize that each of the first three may be derived by the fourth formula by setting adjustment variable  $K$  appropriately. In one form, a waveform template function, such as one illustrated in FIG. 3 (either the solid smooth waveform or the dashed square wave), may be modified for purposes of applying the therapeutic adjustments to either the baseline, peak or median by adjusting the y-axis of the template to vary from either 0 to 1, -1 to 0, or -0.5 to 0.5 respectively. In such an embodiment,  $P_0$  may be adjusted directly by the therapeutic pressure determination process.

30 [0049] Similarly, as illustrated in the flow chart of FIG. 7, an embodiment of a bi-level device having IPAP and EPAP, the apparatus may increase the EPAP pressure as a function of apnea duration determined in the apnea detector 74.

[0050] Several examples of resulting waveforms that may be generated by a device in accordance with various embodiments of the invention are illustrated in FIGS. 2A-2D. In FIG. 2A a square wave is generated based on a fixed swing. The average of the ventilation pressure modulation gradually rises and then falls over time as a result of the automated detection of a therapeutic pressure that may be applied to the baseline, peak or median as previously discussed.

35 [0051] In FIG. 2B, the therapeutic pressure is applied to the peak pressure or swing of a square wave while the baseline is held fixed resulting in a gradually increased and then decreased swing or peak. This may be accomplished by varying or controlling the peak and/or the swing as a function of the therapeutic pressure, while maintaining the baseline pressure fixed.

40 [0052] In FIG. 2C, the automatically detected therapeutic pressure is applied to the baseline pressure or the swing of a square wave. This may be accomplished by varying or controlling the baseline and/or the swing as a function of the therapeutic pressure while maintaining the peak pressure fixed.

[0053] In FIG. 2D, the automatic control described above with regard to FIG. 2A is illustrated with a smoother waveform function. Those skilled in the art will recognize that the control described in FIGS. 2A to 2C can also be applied to the smooth waveform function illustrated in FIG. 2D with results similar to that of FIGS. 2A to 2C respectively.

5.6 OTHER ASPECTS

5.6.1 Mouth leak detection

50 [0054] In one form, the apparatus includes mouth leak detection apparatus, particularly useful for detection of mouth leak when a nasal mask is used. During such treatment when a patient's mouth is open, typically occurring during exhalation, air delivered to the nasal mask may escape through the mouth, through the nose, and out the mouth if the mouth is opened. This is illustrated in the graph of FIG. 10. Thus, the apparatus may include a module, such as a software module or process, that receives a signal indicative of total leak from the mask, as well as a signal indicating whether the patient is inhaling or exhaling. Additionally or alternatively, the software module receives a signal which includes markers indicating trigger and cycle time points. The mouth leak detection software module analyzes the total leak signal and determines whether or not there is a mouth leak, or that the mouth has opened resulting when leak increases

55

coincident with exhalation. Such openings or mouth leak determinations may be counted and with the advent of a certain number of such events, which may be recorded, an indicator or warning from the device may inform the user or patient that a full face mask should be used. Alternatively, as illustrated in FIG. 7, in the presence of leak, the EPAP pressure or end expiratory pressure may be reduced to reduce mouth leak or any other detected mask leak. In one form, the software module integrates the total leak flow during inhalation to calculate total inhalation leak volume. A similar calculation is made to determine total leak exhalation volume. If the leak exhalation volume is greater than the leak inhalation volume by a threshold value, then the software module determines that mouth leak is present or that the mouth is opening or open during exhalation. The following equations may be used:

$$LV_i = avg_{Xbreaths} \left( \int_{t=trigger}^{t=cycle} Leak dt \right)$$

$$LV_e = avg_{Xbreaths} \left( \int_{t=cycle}^{t=trigger} Leak dt \right)$$

*if  $LV_e > LV_i + LV_{threshold}$  then mouth leak*

Once leak flow has been detected, the result may be flagged by generating a warning such as an audible or visible alarm, or recording the event in a data log.

#### 5.6.2 Advantages of our invention

**[0055]** The advantages of our invention are many. Many patients find the delivery of high levels of positive pressure uncomfortable, and this may disturb sleep quality. The positive pressure delivered by prior art devices can lead to mask leaks, mouth leaks, upper airway symptoms, air swallowing and difficulty exhaling. A principle of treatment is to deliver the minimal possible effective pressure. An APAP device is designed to deliver the minimal possible effective pressure, which may vary within a night and from night to night. Bilevel devices have been used to reduce pressure during exhalation. Apparatus in accordance with an embodiment of the invention combines the features of APAP with bi-level ventilation to reduce mean pressure and increase comfort.

**[0056]** A disadvantage of bi-level ventilators, such as BiPAP, for providing comfortable therapy in OSA is the rate of pressure change at the transition from exhalation to inhalation and from inhalation to exhalation. A device in accordance with an embodiment of the invention utilises a more gradual change in pressure delivery during a breath, and copies flow rates observed during normal quiet breathing.

#### 5.6.3 Work of Breathing (WOB)

**[0057]** In patients with poor lung compliance, work of breathing is a significant contributor to energy expenditure. OSA coexists with reduced lung compliance in some disease states, notably congestive heart failure (CHF) where SDB is present in 50-65% of patients. In CHF, CPAP has been demonstrated to improve heart function through a variety of mechanisms. CPAP is poorly tolerated in this group. A device in accordance with an embodiment of the invention offers advantages of CPAP plus the ability to decrease WOB. The bi-level waveforms used by a device in accordance with an embodiment of the invention reduce muscle work required for ventilation. A device in accordance with an embodiment of the invention may be useful in reducing metabolic rate and hence demands on the left ventricle.

**[0058]** Central apneas are a feature of worsening congestive heart failure and may require a different Positive Airway Pressure (PAP) therapy, for example, that provided by the AUTOSSET CS™ device discussed above. A device in accordance with an embodiment of the invention can monitor the frequency of central apneas and provide a warning to the patient or clinician that a different form of treatment is indicated.

**[0059]** Regular CPAP may be difficult to use in CHF due to increased intrathoracic pressure impeding venous return and reducing systolic blood pressure. The bi-level waveforms and peak mean pressures only when necessary used by a device in accordance with an embodiment of the invention will lead to a reduction in this side effect of PAP in CHF.

**[0060]** Non-Invasive ventilators are generally set a pressure that normalise ventilation throughout the night. In Rapid Eye Movement (REM) sleep, physiologic changes in respiratory drive, respiratory muscle tone and upper airway tone

predispose to added reductions in ventilation compared to other sleep states. Ventilation required during other sleep states may be considerably less. In a device in accordance with an embodiment of the invention, the EPAP pressures are lower during non-REM sleep.

**[0061]** In some patients, particularly those with obesity hypoventilation and other causes of hypercapnic respiratory failure, the increased Upper Airway (UA) resistance encountered in REM is an important factor in observed reduction in ventilation. In a device in accordance with an embodiment of the invention, EEP is raised in response to airflow flattening in order to counter the effect which a changing UA resistance may have on ventilation. Thus, in a device in accordance with an embodiment of the invention, by using the minimum necessary EEP required to keep upper airway patency, mean pressures are reduced leading to increased comfort.

**[0062]** Compliance is an issue with low rates of acceptance of therapy with some conditions such as amyotrophic lateral sclerosis and obstructive airways disease. An important factor is expiratory pressure. A device in accordance with an embodiment of the invention provides for a gradual elevation in expiratory pressures, and lowest possible mean pressures during therapy.

**[0063]** Many prior art ventilators use non-physiologic waveforms. While a fast rise-time is important for some patients, for other patients it is more important to have a comfortable waveform. Hence a device in accordance with an embodiment of the invention provides a range of waveforms including more rounded, physiologic shaped waveforms with, for example, a slow falling pressure. The slow falling pressure can be particularly useful for Chronic Obstructive Pulmonary Disorder (COPD).

**[0064]** Although the invention has been described with reference to various embodiments as described above, it is to be understood that these embodiments are merely illustrative of the application of the various principles of the invention. Numerous modifications, in addition to the illustrative embodiments of the invention discussed herein, may be made and other arrangements may be devised without departing from the scope of the invention.

**[0065]** For example other automatic CPAP algorithms may be used to determine the treatment pressure, such as  $P_{crit}$  (for example, as described in U.S. Patent No. 5,645,053 (Remmers et al.).

## Claims

1. An apparatus adapted for treatment of sleep disordered breathing comprising:

a blower (2) for providing to a patient a supply of air at a treatment pressure in phase with the patient's respiratory breathing cycle, the respiratory breathing cycle including an expiratory phase and an inspiratory phase;  
a patient interface (6),

an air delivery conduit (8) for delivering air from the blower to the patient interface, and  
means (4p, 4f, 15) for detecting the pressure in the patient interface, the flow of air provided to the patient through the patient interface, and transitions between inspiration and expiration of the patient's breathing cycle;  
a controller (15) for determining a first index and a second index from pressure or flow detected by said means, the first index being indicative of one or more of apnea, hypopnea and snoring, and the second index being indicative of flow limitation; and calculating a first pressure from the first index and calculating a second pressure from the second index the first pressure being provided during the expiratory phase of the patient's breathing cycle and the second pressure being provided during the inspiratory phase of the patient's breathing cycle.

2. The apparatus according to claim 1, wherein the first pressure is an EPAP or EEP pressure.

3. The apparatus according to claim 1 or 2, wherein the second pressure is an IPAP pressure.

4. The apparatus according to any one of claims 1-3, wherein the second pressure is greater than or equal to the first pressure.

5. The apparatus according to claim 4, wherein there is a predetermined maximum pressure difference between the first pressure and the second pressure.

6. The apparatus according to claims 1-5, wherein the first pressure and the second pressure have a maximum value of about 25 cmH<sub>2</sub>O.

7. The apparatus according to any one of claims 1-6, wherein the first pressure and the second pressure have a minimum value of about 4 cmH<sub>2</sub>O.

8. The apparatus according to any one of claims 1-7, wherein the controller causes the blower to provide the supply of air at positive pressure in accordance with a pressure-time template.
- 5 9. The apparatus according to claim 8, wherein the pressure-time template is a square wave.
10. The apparatus according to claim 8, wherein the pressure-time template is a shark-fin wave.
11. The apparatus according to claims 8-10, wherein the pressure-time template is stored in look-up tables or arrays.
- 10 12. The apparatus according to any one of claims 1-11, wherein the controller further causes the blower to decrease the first pressure in the absence of the detection of a sleep disordered breathing event indicated by the first index.
- 15 13. The apparatus according to any one of claims 1-12, wherein the controller further causes the blower to decrease the second pressure in the absence of the detection of a sleep disordered breathing event indicated by the second index.

### Patentansprüche

- 20 1. Vorrichtung, die zur Behandlung schlafbezogener Atemstörungen geeignet ist und aufweist:
- ein Gebläse (2) zum Bereitstellen einer Luftzufuhr für einen Patienten mit einem Behandlungsdruck phasengleich mit dem Atemzyklus des Patienten, wobei der Atemzyklus eine Expirationsphase und eine Inspirationsphase aufweist;
- 25 eine Patientenschnittstelle (6),  
eine Luftabgabeleitung (8) zum Abgeben von Luft vom Gebläse zur Patientenschnittstelle und  
Mittel (4p, 4f, 15) zum Detektieren des Drucks in der Patientenschnittstelle, des Luftdurchflusses, der für den Patienten über die Patientenschnittstelle bereitgestellt wird, und von Übergängen zwischen Inspiration und Expiration des Atemzyklus des Patienten;
- 30 eine Steuerung (15) zum Bestimmen eines ersten Index und eines zweiten Index anhand von Druck oder Durchfluss, die durch die Mittel detektiert werden, wobei der erste Index Apnoe, Hypopnoe und/oder Schnarchen angibt und der zweite Index Durchflusseinschränkung angibt; und Berechnen eines ersten Drucks anhand des ersten Index sowie Berechnen eines zweiten Drucks anhand des zweiten Index, wobei der erste Druck während der Expirationsphase des Atemzyklus des Patienten bereitgestellt wird und der zweite Druck während der Inspirationsphase des Atemzyklus des Patienten bereitgestellt wird.
- 35
2. Vorrichtung nach Anspruch 1, wobei der erste Druck ein EPAP- oder EEP-Druck ist.
3. Vorrichtung nach Anspruch 1 oder 2, wobei der zweite Druck ein IPAP-Druck ist.
- 40 4. Vorrichtung nach einem der Ansprüche 1 bis 3, wobei der zweite Druck gleich oder größer als der erste Druck ist.
5. Vorrichtung nach Anspruch 4, wobei eine vorbestimmte maximale Druckdifferenz zwischen dem ersten Druck und dem zweiten Druck vorliegt.
- 45 6. Vorrichtung nach Anspruch 1 bis 5, wobei der erste Druck und der zweite Druck einen Maximalwert von etwa 25 cm H<sub>2</sub>O haben.
7. Vorrichtung nach einem der Ansprüche 1 bis 6, wobei der erste Druck und der zweite Druck einen Minimalwert von etwa 4 cm H<sub>2</sub>O haben.
- 50 8. Vorrichtung nach einem der Ansprüche 1 bis 7, wobei die Steuerung veranlasst, dass das Gebläse die Luftzufuhr mit positivem Druck in Übereinstimmung mit einer Druck-Zeit-Schablone bereitstellt.
- 55 9. Vorrichtung nach Anspruch 8, wobei die Druck-Zeit-Schablone eine Rechteckwelle ist.
10. Vorrichtung nach Anspruch 8, wobei die Druck-Zeit-Schablone eine Haifischflossenwelle ist.

## EP 1 699 514 B1

11. Vorrichtung nach Anspruch 8 bis 10, wobei die Druck-Zeit-Schablone in Nachschlagetabellen oder Arrays gespeichert ist.
- 5 12. Vorrichtung nach einem der Ansprüche 1 bis 11, wobei die Steuerung ferner veranlasst, dass das Gebläse den ersten Druck bei fehlender Detektion eines durch den ersten Index angegebenen schlafbezogenen Atemstörungsereignisses verringert.
- 10 13. Vorrichtung nach einem der Ansprüche 1 bis 12, wobei die Steuerung ferner veranlasst, dass das Gebläse den zweiten Druck bei fehlender Detektion eines durch den zweiten Index angegebenen schlafbezogenen Atemstörungsereignisses verringert.

### Revendications

- 15 1. Appareil adapté pour le traitement de la respiration perturbée pendant le sommeil comprenant :
- un ventilateur (2) pour fournir à un patient une alimentation en air à une pression de traitement en phase avec le cycle respiratoire de respiration du patient, le cycle respiratoire de respiration comportant une phase expiratoire et une phase inspiratoire ;
- 20 une interface patient (6),  
un conduit d'apport en air (8) pour apporter de l'air du ventilateur à l'interface patient, et  
des moyens (4p, 4f, 15) pour détecter la pression dans l'interface patient, l'écoulement d'air fourni au patient à travers l'interface patient, et des transitions entre une inspiration et une expiration du cycle de respiration du patient ;
- 25 une unité de commande (15) pour déterminer un premier indice et un second indice à partir d'une pression ou d'un écoulement détecté par lesdits moyens, le premier indice étant indicatif d'un ou plusieurs apnées, hypopnées et ronflements, et le second indice étant indicatif d'une limitation d'écoulement ; et calculer une première pression à partir du premier indice et calculer une seconde pression à partir du second indice, la première pression étant fournie pendant la phase expiratoire du cycle de respiration du patient et la seconde pression étant fournie pendant la phase inspiratoire du cycle de respiration du patient.
- 30
2. Appareil selon la revendication 1, dans lequel la première pression est une pression positive expiratoire ou une pression en fin d'expiration.
- 35 3. Appareil selon la revendication 1 ou 2, dans lequel la seconde pression est une pression positive inspiratoire.
4. Appareil selon l'une quelconque des revendications 1 à 3, dans lequel la seconde pression est supérieure ou égale à la première pression.
- 40 5. Appareil selon la revendication 4, dans lequel il y a une différence de pression maximale prédéterminée entre la première pression et la seconde pression.
6. Appareil selon les revendications 1 à 5, dans lequel la première pression et la seconde pression ont une valeur maximale d'environ 25 cm H<sub>2</sub>O.
- 45 7. Appareil selon l'une quelconque des revendications 1 à 6, dans lequel la première pression et la seconde pression ont une valeur minimale d'environ 4 cm H<sub>2</sub>O.
8. Appareil selon l'une quelconque des revendications 1 à 7, dans lequel l'unité de commande amène le ventilateur à fournir l'alimentation en air à pression positive conformément à un modèle pression-temps.
- 50 9. Appareil selon la revendication 8, dans lequel le modèle pression-temps est une onde carrée.
10. Appareil selon la revendication 8, dans lequel le modèle pression-temps est une onde en aileron de requin.
- 55 11. Appareil selon les revendications 8 à 10, dans lequel le modèle pression-temps est stocké dans tables ou tableaux à consulter.

## EP 1 699 514 B1

12. Appareil selon l'une quelconque des revendications 1 à 11, dans lequel l'unité de commande amène en outre le ventilateur à diminuer la première pression en l'absence de la détection d'une manifestation de respiration perturbée pendant le sommeil indiquée par le premier indice.

5 13. Appareil selon l'une quelconque des revendications 1 à 12, dans lequel l'unité de commande amène en outre le ventilateur à diminuer la seconde pression en l'absence de la détection d'une manifestation de respiration perturbée pendant le sommeil indiquée par le second indice.

10

15

20

25

30

35

40

45

50

55

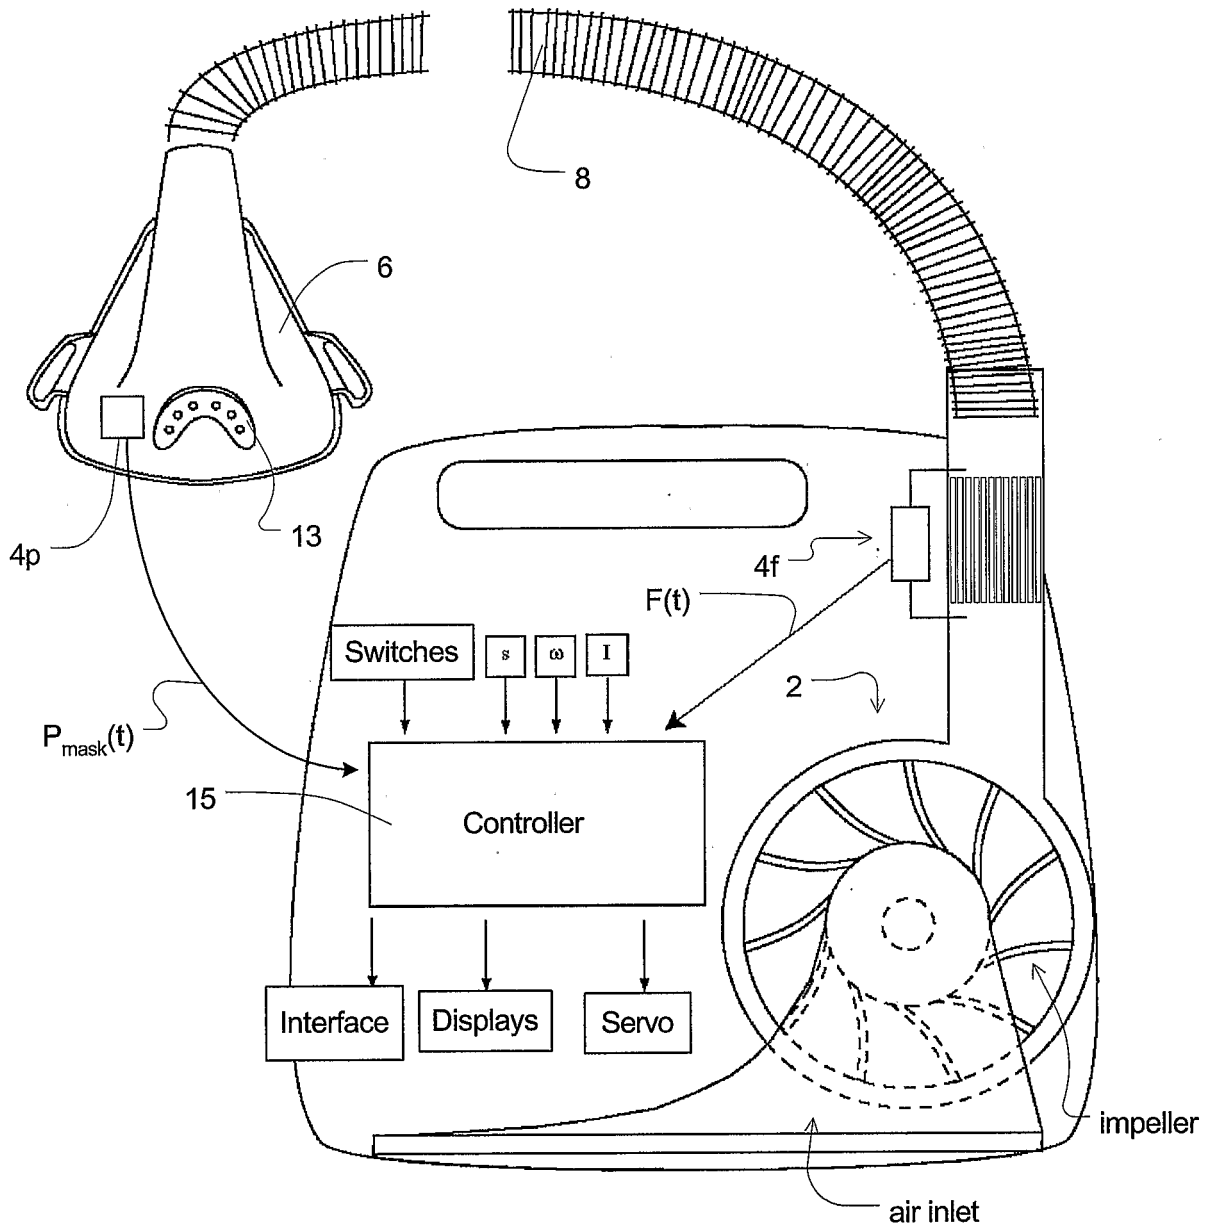


FIG. 1

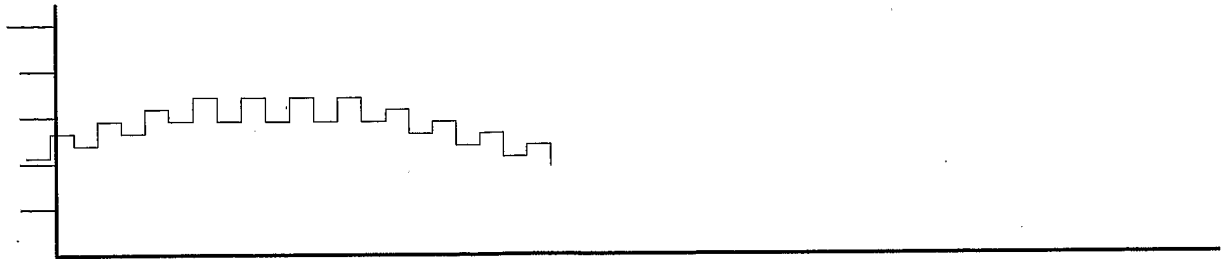


FIG. 2A

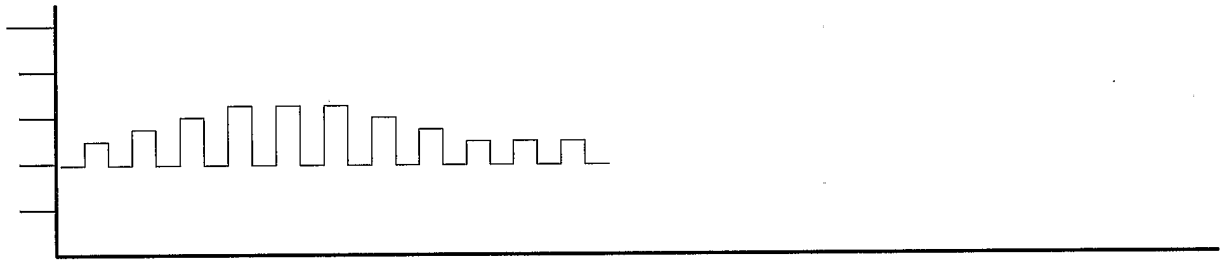


FIG. 2B

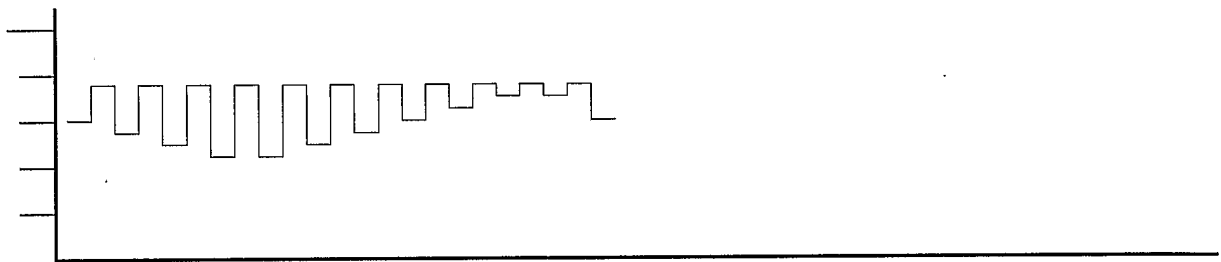


FIG. 2C



FIG. 2D

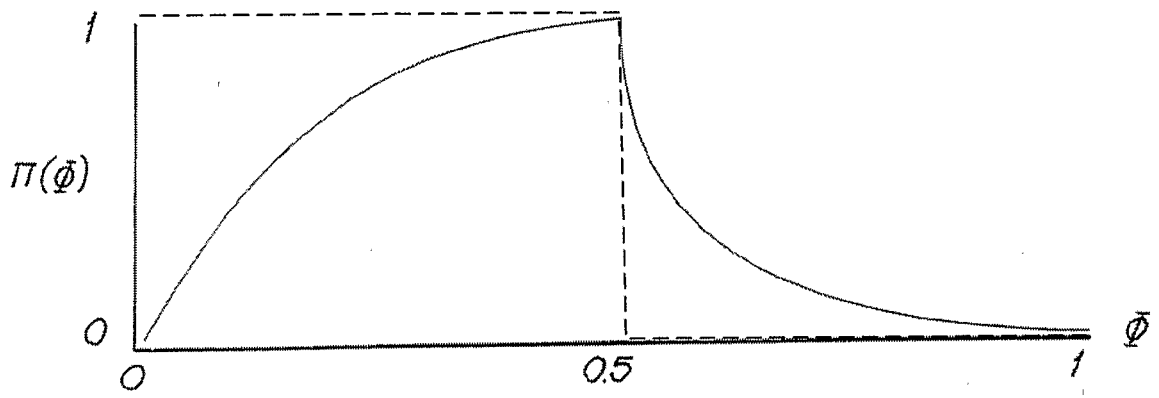


FIG. 3

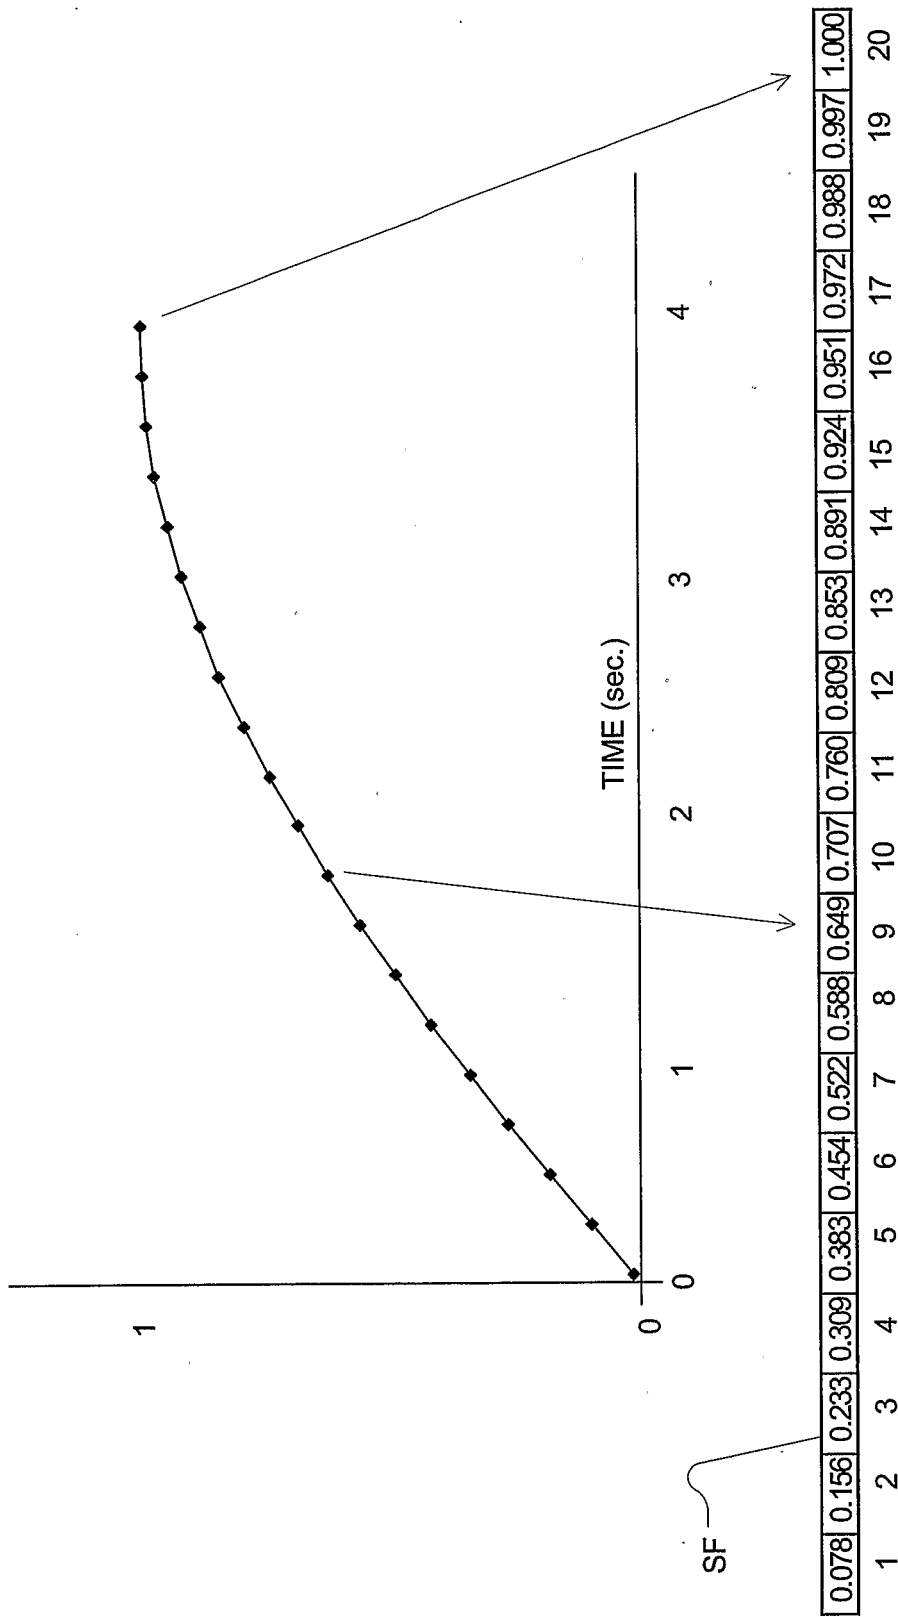


FIG. 4

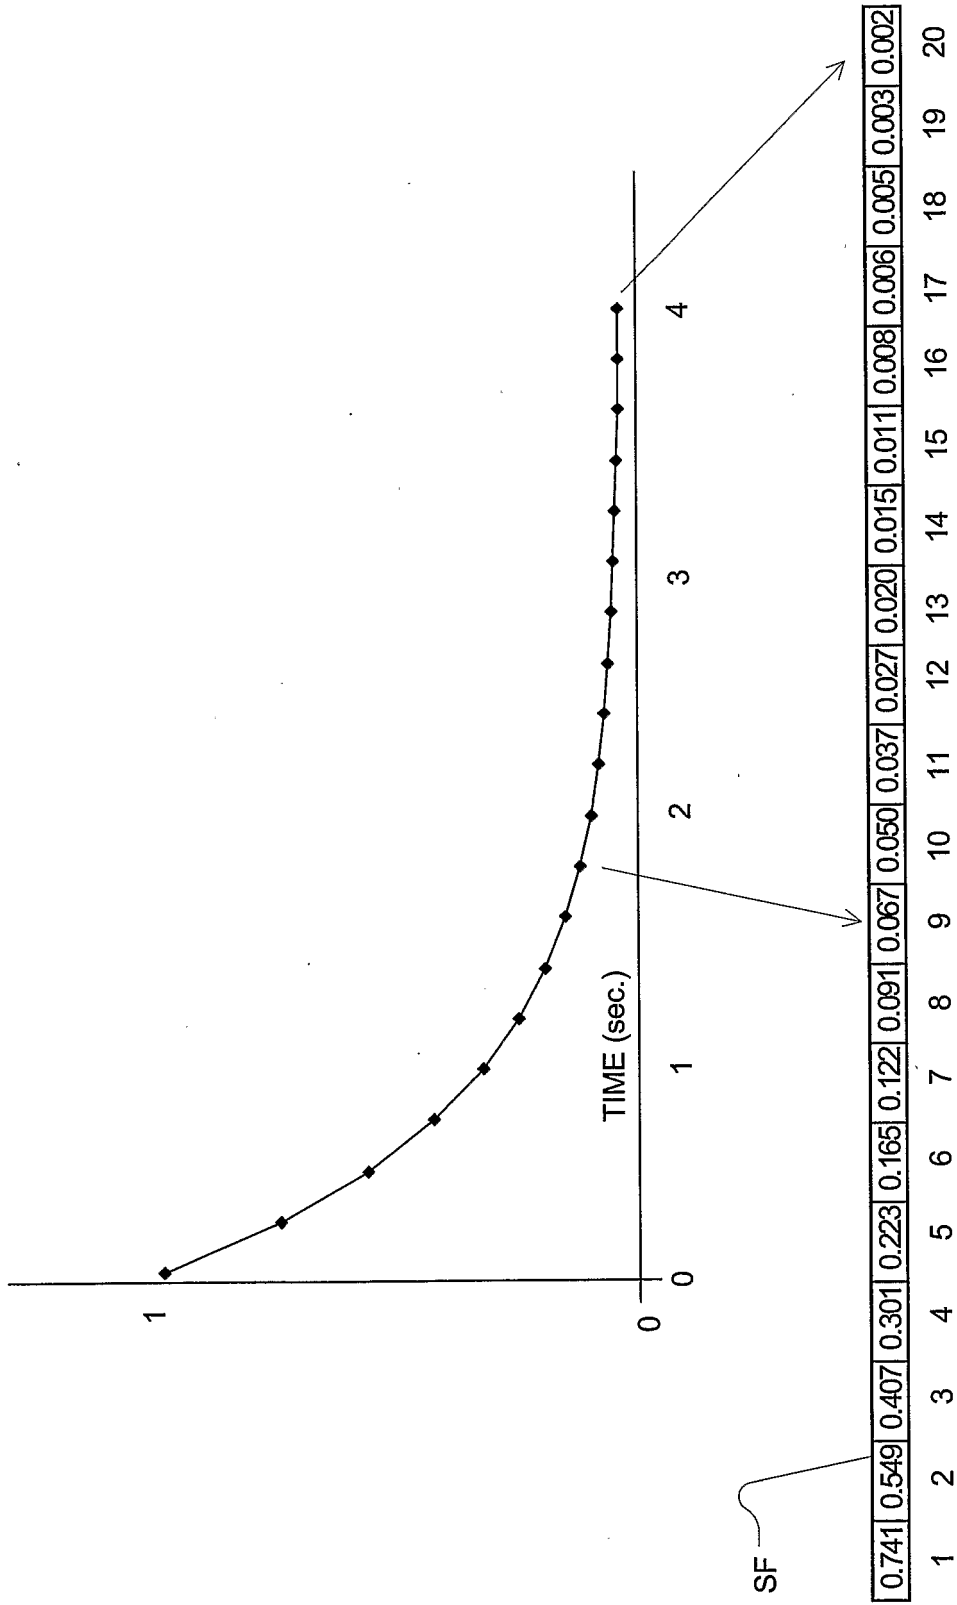


FIG. 5

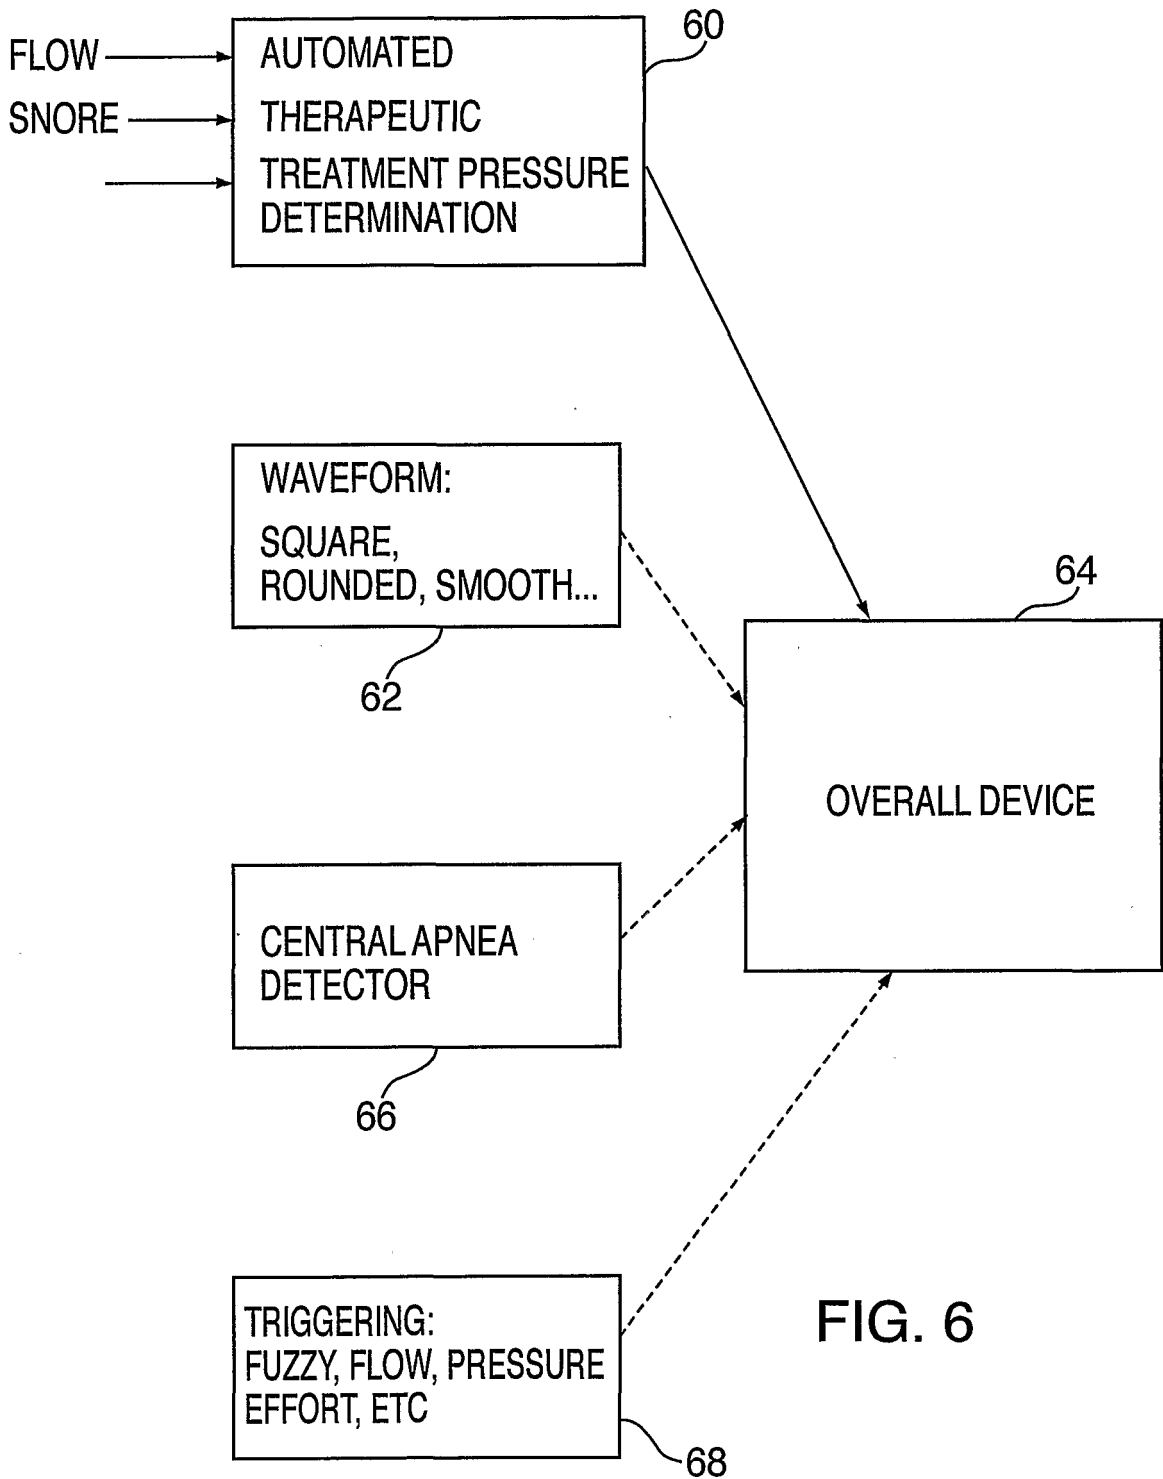


FIG. 6

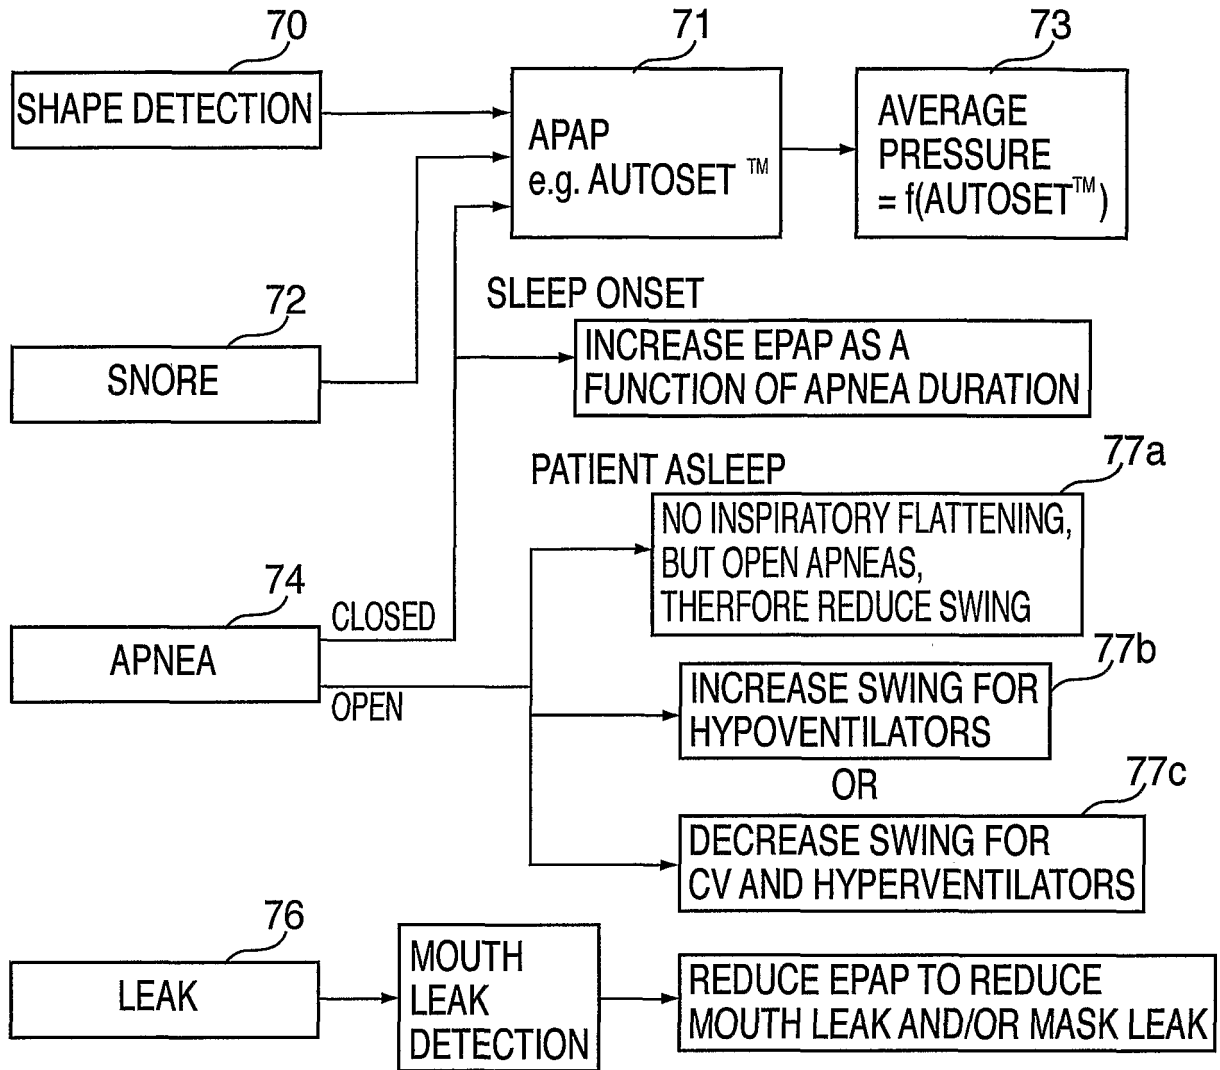


FIG. 7

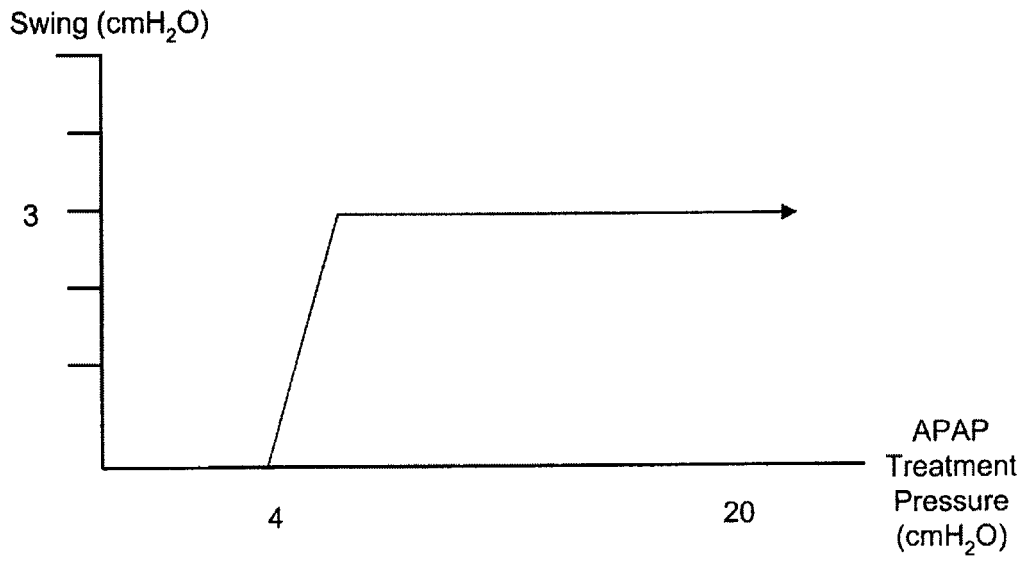


FIG. 8A

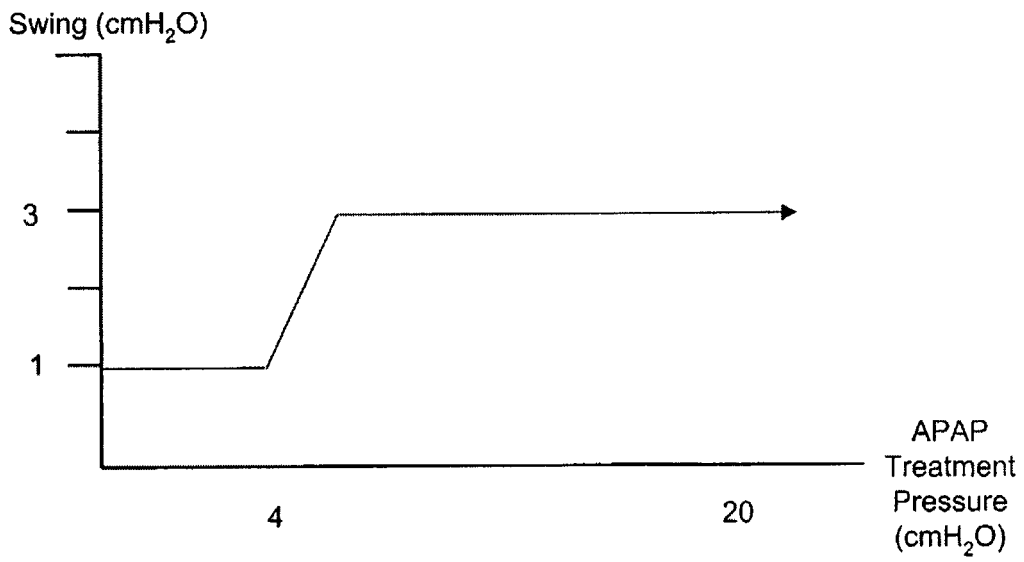


FIG. 8B

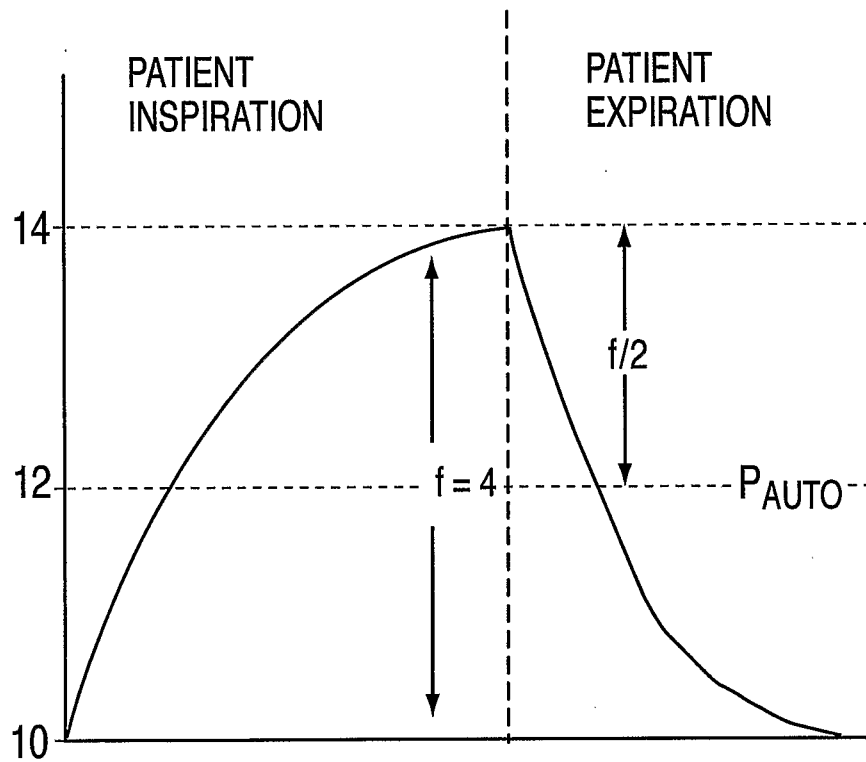


FIG. 9

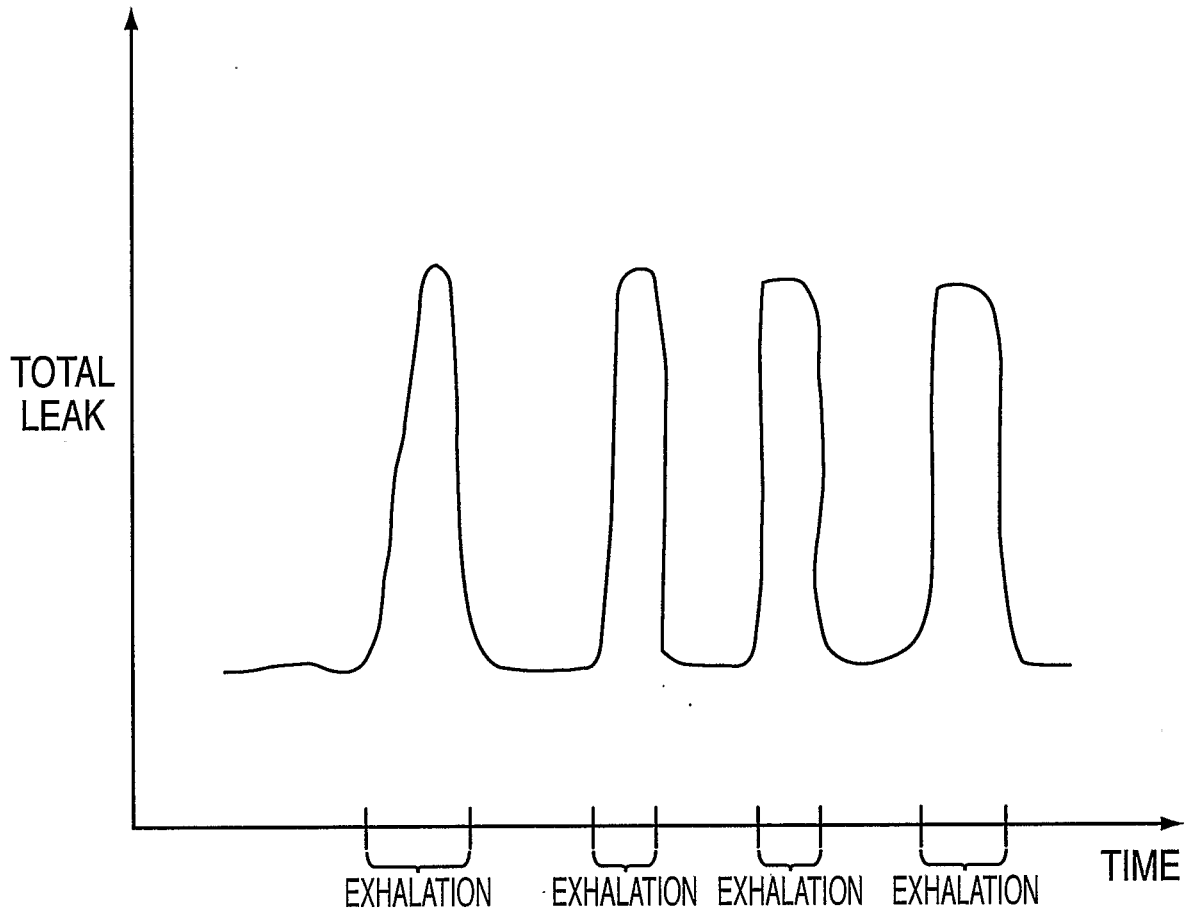


FIG. 10

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 60533411 B [0001]
- US 4944310 A [0004]
- US 6112746 A [0005]
- US 6357441 B [0005]
- US 6581602 B [0005]
- US 6634358 B [0005]
- WO 200197893 A [0005]
- US 5245995 A [0006] [0029]
- US 6398739 B [0006]
- US 6635021 B [0006]
- US 5704345 A [0008] [0029] [0031] [0035] [0037]
- US 6029665 A [0008]
- US 6138675 A [0008]
- US 6363933 B [0008]
- US 6484719 B [0009] [0021]
- US 6532957 B [0009] [0021]
- US 6575163 B [0009] [0021]
- US 6532959 B [0009] [0036]
- US 6213119 B1 [0011]
- US 5535738 A [0012]
- US 5503146 A [0013]
- US 6041780 A [0014]
- US 6532960 B1 [0015]
- US 6367474 B, Berthon-Jones [0033]
- US 6814073 B, Wickham [0035]
- US 6553992 B [0036]
- US 5645053 A, Remmers [0065]

**Non-patent literature cited in the description**

- **MARTIN J TOBIN.** Principles and Practice of Mechanical Ventilation. McGraw-Hill Inc, 1994 [0003]

专利名称(译)	存在睡眠呼吸障碍的机械通气		
公开(公告)号	<a href="#">EP1699514B1</a>	公开(公告)日	2019-09-25
申请号	EP2004802134	申请日	2004-12-24
[标]申请(专利权)人(译)	雷斯梅德有限公司		
申请(专利权)人(译)	瑞思迈LTD.		
[标]发明人	DOUGLAS ROBERT UJHAZY ANTHONY JOHN RICHARDS GLENN BUCKLEY MARK SCHINDHELM KLAUS HENRY		
发明人	DOUGLAS, ROBERT UJHAZY, ANTHONY JOHN RICHARDS, GLENN BUCKLEY, MARK SCHINDHELM, KLAUS HENRY		
IPC分类号	A61M16/00 A61M16/06 A61B5/00		
CPC分类号	A61M16/0051 A61M16/0069 A61M16/024 A61M16/06 A61M2016/0021 A61M2016/0027 A61M2016/0039 A61M2205/15 A61B5/4818 A61B5/4836 A61M16/0066 A61M16/0875		
优先权	60/533411 2003-12-29 US 60/545658 2004-02-18 US		
其他公开文献	EP1699514A1 EP1699514A4		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

一种用于控制CPAP设备的操作的方法。该设备具有鼓风机，患者接口，用于将空气从鼓风机传递到患者接口的空气输送管道，用于确定患者接口中的压力的传感器以及使空气以所需压力被输送的控制机构。连接到患者接口，并检测患者的呼吸循环的吸气和呼气之间的转换，以使鼓风机输出与患者的努力保持同步。在一种形式中，CPAP设备根据双级波形提供压力，其中该波形的至少一个表征参数根据睡眠呼吸障碍的指示自动调节。睡眠呼吸障碍的迹象可能是打nor，呼吸暂停，呼吸不足和流量受限中的一种或多种。

