



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11) **EP 1 168 959 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
29.11.2006 Bulletin 2006/48

(21) Application number: **00923420.4**

(22) Date of filing: **14.04.2000**

(51) Int Cl.:
A61B 5/00 (2006.01)

(86) International application number:
PCT/US2000/010269

(87) International publication number:
WO 2000/061000 (19.10.2000 Gazette 2000/42)

(54) **DEVICE FOR INDICATING QUALITY AND ACCURACY OF PHYSIOLOGICAL MEASUREMENTS**

GERÄT ZUR QUALITÄTS- UND GENAUIGKEITSANZEIGE VON PHYSIOLOGISCHEN
MESSUNGEN

DISPOSITIF PERMETTANT D'INDIQUER LA QUALITE ET LA PRECISION DE MESURES
PHYSIOLOGIQUES

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE**

(30) Priority: **14.04.1999 US 129170 P**

(43) Date of publication of application:
09.01.2002 Bulletin 2002/02

(73) Proprietor: **MALLINCKRODT INC.
Pleasanton, CA 94588 (US)**

(72) Inventors:
• **PORGES, Charles**
Orinda, CA 94563 (US)
• **BAKER, Clark**
Castro Valley, CA 94546 (US)

• **YORKLEY, Thomas, J.**
San Ramon, CA 94583 (US)
• **BERNSTEIN, Michael**
San Ramon, CA 94583 (US)
• **MANNHEIMER, Paul**
Danville, CA 94506 (US)

(74) Representative: **Grubert, Andreas**
Baker Botts
41 Lothbury Street
London EC2R 7HF (GB)

(56) References cited:
EP-A- 0 221 357 **EP-A- 0 571 225**
US-A- 4 858 615 **US-A- 4 942 877**
US-A- 5 503 148

EP 1 168 959 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

[0001] The present invention relates to physiological monitoring instruments and, in particular, monitors and sensors that include mechanisms for indicating a quality of detected signals and accuracy or confidence level of physiological measurements estimated from the signals.

[0002] Typically, for physiological monitoring instruments that include a monitor and a patient sensor, the monitor is unable to accurately determine a quality of a signal obtained from the sensor. The invention will be explained by reference to a preferred embodiment concerning pulse oximeter monitors and pulse oximetry sensors, but it should be realized the invention is applicable to any generalized patient monitor and associated patient sensor. The invention provides a way of more accurately determining a quality of a signal detected by a sensor; a way of determining a relative accuracy of a physiological characteristic derived or calculated from the signal; and a way of delineating a transition boundary between a normal signal for the sensor being used in its normal application, and a signal considered to be abnormal for the sensor being used, to allow a monitor to determine if the sensor is being misapplied.

[0003] Pulse oximetry is typically used to measure various blood flow characteristics including, but not limited to, the blood oxygen saturation of hemoglobin in arterial blood and the heartbeat of a patient. Measurement of these characteristics has been accomplished by the use of a non-invasive sensor that passes light through a portion of a patient's blood perfused tissue and photo-electrically senses the absorption and scattering of light in such tissue. The amount of light absorbed and scattered is then used to estimate the amount of blood constituent in the tissue using various algorithms known in the art. The "pulse" in pulse oximetry comes from the time varying amount of arterial blood in the tissue during a cardiac cycle. The signal processed from the sensed optical signal is a familiar plethysmographic waveform due to the cycling light attenuation.

[0004] The light passed through the tissue is typically selected to be of two or more wavelengths that are absorbed by the blood in an amount related to the amount of blood constituent present in the blood. The amount of transmitted light that passes through the tissue varies in accordance with the changing amount of blood constituent in the tissue and the related light absorption.

[0005] To estimate arterial blood oxygen saturation of a patient, conventional two-wavelength pulse oximeters emit light from two light emitting diodes (LEDs) into a pulsatile tissue bed and collect the transmitted light with a photodiode (or photo-detector) positioned on an opposite surface (i.e., for transmission pulse oximetry) or an adjacent surface (i.e., for reflectance pulse oximetry). The LEDs and photo-detector are typically housed in a reusable or disposable oximeter sensor that couples to a pulse oximeter electronics and display unit. One of the two LEDs' primary wavelength is selected at a point in the electromagnetic spectrum where the absorption of oxyhemoglobin (HbO_2) differs from the absorption of reduced hemoglobin (Hb). The second of the two LEDs' wavelength is selected at a different point in the spectrum where the absorption of Hb and HbO_2 differs from those at the first wavelength. Commercial pulse oximeters typically utilize one wavelength in the near red part of the visible spectrum near 660 nanometers (nm) and one in the near infrared (IR) part of the spectrum in the range of 880-940 nm.

[0006] Oxygen saturation can be estimated using various techniques. In one common technique, first and second photo-current signals generated by the photo-detector from red and infrared light are conditioned and processed to determine AC and DC signal components and a modulation ratio of the red to infrared signals. This modulation ratio has been observed to correlate well to arterial oxygen saturation. Pulse oximeters and sensors are empirically calibrated by measuring the modulation ratio over a range of in vivo measured arterial oxygen saturations (SaO_2) on a set of patients, healthy volunteers, or animals. The observed correlation is used in an inverse manner to estimate blood oxygen saturation (SpO_2) based on the measured value of modulation ratios. The estimation of oxygen saturation using modulation ratio is described in U.S. Patent No. 5,853,364, entitled "METHOD AND APPARATUS FOR ESTIMATING PHYSIOLOGICAL PARAMETERS USING MODEL-BASED ADAPTIVE FILTERING", issued December 29, 1998, and U.S. Patent No. 4,911,167, entitled "METHOD AND APPARATUS FOR DETECTING OPTICAL PULSES", issued March 27, 1990. The relationship between oxygen saturation and modulation ratio is further described in U. S. Patent No. 5,645,059, entitled "MEDICAL SENSOR WITH MODULATED ENCODING SCHEME," issued July 8, 1997. All three patents are assigned to the assignee of the present invention.

[0007] The accuracy of the estimates of the blood flow characteristics depends on a number of factors. For example, the light absorption characteristics typically vary from patient to patient depending on their physiology. Moreover, the absorption characteristics vary depending on the location (e.g., the foot, finger, ear, and so on) where the sensor is applied. Further, the light absorption characteristics vary depending on the design or model of the sensor. Also, the light absorption characteristics of any single sensor design vary from sensor to sensor (e.g., due to different characteristics of the light sources or photo-detector, or both). The clinician applying the sensor correctly or incorrectly may also have a large impact in the results, for example, by loosely or firmly applying the sensor or by applying the sensor to a body part which is inappropriate for the particular sensor design being used.

[0008] Some oximeter "qualify" measurements before displaying them on the monitor. One conventional technique processes (i.e., filters) the measured plethysmographic waveform and performs tests to detect and reject measurements perceived corrupted and inaccurate. Since oximeters are typically designed to be used with a wide variety of sensors having widely differing performance characteristics, the monitor signal "qualification" algorithms are necessarily crude, and often result in only superficial indications of signal quality, signal reliability, and ultimately a confidence level in a patient physiological characteristic estimated or calculated from the signal. In many instances, the monitor simply discards data associated with low quality signals, but otherwise gives no indication to a healthcare giver as to whether any physiological characteristic displayed on a monitor is highly reliable or not. Hence, the signal quality measurements obtained from such crude algorithms are relatively poor and convey little useful information to a caregiver.

[0009] U.S. Patent No. 4,942,877 discloses a device for measuring oxygen saturation degree in arterial blood, European Patent No. 0221357 discloses an electro-optical coupler for catheter oximeter, European Patent No. 0571225 discloses a measurement device and method of calibration, and U.S. Patent No. 4,848,615 discloses a catheter sensor and memory unit.

SUMMARY OF THE INVENTION

[0010] Accordingly, it is an object of the present invention to provide a patient monitor and sensor which includes means for accurately detecting a quality and accuracy of a signal detected by the sensor and for displaying this information on a monitor.

[0011] These and others objects of the invention are achieved by a monitor according to claim 1. The dependent claims include further enhancements. Each boundary defines a region of a signal quality diagram and corresponds to a different level of quality in the detected signals and accuracy or confidence level of physiological characteristic estimated from the detected signals. Boundaries can also be defined for and associated with different sensor types and monitor types. The boundaries are typically stored in a memory and accessed when required.

[0012] An embodiment of the invention provides a sensor for sensing at least one physiological characteristic of a patient. The sensor is connectable to a monitor that estimates a physiological condition from signals detected by the sensor. The sensor includes a detector for detecting the signals from the patient which are indicative of the physiological characteristic. The sensor is associated with a memory configured to store data that defines sensor signal specification boundaries for the detected signals. The boundaries are indicative of a quality of the signals and an accuracy of the physiological characteristic estimated from the signals by the monitor. The sensor further includes means for providing access to the memory to allow transmission of the data that defines the at least one sensor boundary to the monitor.

[0013] In an embodiment, the boundaries are indicative of a transition between a signal regime considered normal for the sensor in its usual application, and a signal regime considered to be abnormal. The normal regime can be one in which the sensor is likely to be properly applied to the patient and the abnormal regime can be one in which the sensor may have partially or entirely come off the patient.

[0014] The foregoing, together with other aspects of this invention, will become more apparent when referring to the following specification, claims, and accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015]

Fig. 1 shows a simplified block diagram of an embodiment of a pulse oximeter system;

Fig. 2A shows a diagram of a specific embodiment of a sensor;

Figs. 2B and 2C show diagrams of specific embodiments in which a memory is located within the sensor plug and within the sensor cable, respectively;

Fig. 2D shows a diagram of a specific embodiment of a monitor;

Fig. 3 shows a diagram of a simplified optical waveform detected by the sensor;

Fig. 4 shows a signal quality diagram that includes data of the measured DC and AC components;

Fig. 5 shows a signal quality diagram having defined regions corresponding to different confidence levels in the saturation estimate;

Fig. 6 shows a signal quality diagram having defined display and non-display regions (similar to those of Fig. 5) and transition zones;

Fig. 7 shows a flow diagram of an embodiment of the measurement posting process of the invention;

Fig. 8 shows a signal quality diagram with data collected from a patient population; and

Fig. 9 shows a signal quality diagram that includes ambiguity contours plotted over a portion of the display region.

DESCRIPTION OF THE SPECIFIC EMBODIMENTS

[0016] The invention is applicable to measurement (or estimation) of oxygen saturation of hemoglobin in arterial blood and patient heart rate. The invention will be described in detail with respect to an embodiment for pulse oximetry, but it needs to be realized that the invention has applicability to alternate patient monitoring characteristics, such as ECG, blood pressure, temperature, etc., and is not to be limited to only for use with oximetry or pulse oximetry.

[0017] Fig. 1 shows a simplified block diagram of an embodiment of a pulse oximeter system 100. System 100 includes a pulse oximeter (or monitor) 110 that couples via an electrical cable 128 to a sensor 130 that is applied to a patient 132. Sensor 130 includes a sensor cable 129 and a connector plug 120. The sensor further has first and second light sources (e.g., LEDs) and a photo-detector along with suitable components to couple these electro-optical components to the electrical cable 128.

[0018] As noted above, oxygen saturation can be estimated using various techniques. In one common technique, the optical signals are received by the photo-detector, and conditioned and processed by the oximeter to generate AC and DC components. These components are then used to compute a modulation ratio of the red to infrared signals. The computed modulation ratio is then indexed against a table to retrieve a saturation estimate corresponding to that modulation ratio.

[0019] Fig. 2A shows a diagram of a specific embodiment of sensor 130. Sensor 130 includes two or more LEDs 230 and a photodetector 240. Sensor 130 may optionally include a memory 236a and an interface 238. LEDs 230 receive drive signals that (i.e., alternately) activate the LEDs. When activated, the light from LEDs 230 passes into a patient's tissues 234. After being transmitted through or reflected from the tissues, the light is received by photo-detector 240. Photo-detector 240 converts the received light into a photocurrent signal, which is then provided to the subsequent signal-processing unit.

[0020] The sensor memory stores data representative of at least one sensor signal specification boundary and provides the sensor boundary when requested. Interface circuit 238 provides signal conditioning, and can also provide other functions. Through interface circuit 238, data is transferred to and from the sensor memory. Memory 236a and interface circuit 238 can be integrated within one integrated circuit for reduced size and cost.

[0021] The memory associated with the sensor can be physically located in a variety of places. First, it can be located on the body of the sensor, in a vicinity of the photodetector, LEDs, or other sensor components. Or, the memory can be in the sensor cable 129 or the sensor plug 122, or in an adapter module that connects to a front of an oximeter, to an oximeter cable, or to a sensor plug or cable.

[0022] Fig. 2B shows a diagram of a specific embodiment in which a memory 236b is located within the sensor plug 122. Memory 236b couples to and interfaces with external circuitry through some or all signal lines provided to the sensor plug.

[0023] Fig. 2C shows a diagram of a specific embodiment in which a memory 236c is located within the sensor cable 129. Again, memory 236c couples to and interfaces with external circuitry through a set of signal lines.

[0024] The memory 236 can be implemented as a random access memory (RAM), a FLASH memory, a programmable read only memory (PROM), an erasable PROM (EPROM), an electrically erasable PROM (EEPROM), a write once memory, or other memory technologies capable of write and read operations. In a specific embodiment, to preserve the data stored in the memory and prevent accidental erasure, the sensor memory can be written only once. This memory characteristic also prevents erasure of the data during sensor operation. A specific example of a memory device that can be written only once is a 2-wire EPROM device available from Dallas Semiconductor Corp.

[0025] Fig. 2D shows a diagram of a specific embodiment of monitor 110. A receiving circuit 250 couples to the sensor and the memory associated with the sensor for receiving signals detected by the sensor and data from the sensor memory. The receiving circuit 250 couples to a processing circuit 252 that processes the received signals to generate an estimate of a physiological characteristic. The processing circuit 252 can further generate an indication of the quality of the received signal and an indication of the accuracy of the estimated physiological characteristic. The estimated physiological characteristic and associated indications are provided to a display unit 254 for display to a user of the monitor.

[0026] Fig. 3 shows a diagram of a simplified optical waveform 300 detected by a sensor (e.g., sensor 130). Optical waveform 300 in Fig. 3 can represent the detected optical signal for either the red or infrared LED. As shown in Fig. 3, optical waveform 300 includes a periodic pattern that generally corresponds to a patient's heartbeat. For arrhythmia patient, the waveform may be aperiodic. Waveform 300 includes a series of peaks having a maximum value (Max) and a series of valleys having a minimum value (Min). The following quantities are defined:

$$AC = Max - Min ;$$

Eq. (1)

$$DC = \frac{(Max + Min)}{2}; \quad \text{Eq. (2)}$$

$$Modulation\ percentage\ (Mod\%) = 100 \cdot \left(\frac{AC}{DC} \right); \text{ and} \quad \text{Eq. (3)}$$

$$nAv\ (nanoAmperes\ virtual) = \frac{DC}{Instrument\ gain} \cdot \frac{50mA}{actual\ LED\ drive\ current\ in\ mA} \quad \text{Eq. (4)}$$

where Instrument gain is a gain value that is specific to the combination of the pulse oximeter and a particular sensor that is used during the detection of the pulses in waveform 300. The Instrument gain includes both the LED drive current and the amplification of the instrument. Nanoamperes virtual "normalizes" the signal to a 50 mA LED drive.

[0027] The modulation ratio of the red to infrared signals, sometimes referred to as the "ratio of ratios" (Ratrat), can be approximated as:

$$Ratrat \cong \frac{\left(\frac{AC_Red}{DC_Red} \right)}{\left(\frac{AC_IR}{DC_IR} \right)}; \quad \text{Eq. (5)}$$

where AC_Red and DC_Red are the respective AC and DC components of the red LED, and AC_IR and DC_IR are the respective AC and DC components of the infrared LED. Oxygenation derived from Ratrat using equation (5) is sufficiently accurate for many applications when the condition (AC << DC) is satisfied. Particularly, the approximation error is small when both AC terms in equation (5) are less than ten percent of the related DC terms (i.e., both red and infrared modulations are less than 10%).

[0028] As stated above, oxygen saturation is (inversely) related to Ratrat. The relationship between Ratrat and oxygen saturation is typically plotted as a curve (i.e., saturation versus Ratrat) and stored as a table in the memory within the oximeter. Subsequently, a calculated Ratrat is used to index the table to retrieve an entry in the table for the oxygen saturation estimate corresponding to that Ratrat. The estimation of oxygen saturation using Ratrat is further described in U.S. Patent Nos. 4,911,167, 5,645,059, and 5,853,364.

[0029] Generally, the Red terms are measured in the red part of the optical spectrum using the red LED, and the IR terms are measured in the infrared part of the optical spectrum using the infrared LED. The AC terms are generated by the blood pressure pulse and are somewhat related to "perfusion." The DC terms are (inversely) related to the "opacity" (or darkness) of the patient being monitored and are somewhat related to "translucence." Generally, the four terms in equation (5) are independent of each other. However, empirical studies suggest that the two DC terms are somewhat correlated (i.e., not wildly divergent), and patients who are "opaque" tend to be opaque in both the red and infrared parts of the spectrum. However, the two AC terms are typically not correlated (i.e., the AC terms can be quite divergent for a patient).

[0030] It has been determined that the magnitudes of the DC and AC components influence the accuracy of the saturation estimates and these magnitudes depend on the sensor design being used, the specifications of components used in the sensor, and how the sensor has been applied to the patient. The invention advantageously utilizes this knowledge to provide an oximeter system capable of providing indications of the accuracy and reliability of the saturation

estimates. Additional features are provided by the invention based on the analysis of the measured DC and AC components, as described below.

Fig. 4 shows a signal quality diagram that includes data of the measured DC and AC components. The vertical axis of the signal quality diagram corresponds to the modulation percentage (Mod%) which is calculated as shown in equation (3) for each of the red and infrared signals. The horizontal axis corresponds to the DC component and is in units of virtual nano Amperes (nAv) and is given by equation (4). As shown in Fig. 4, both vertical and horizontal axes are plotted on a logarithmic scale.

[0031] As noted above, the detected optical waveform includes an AC component and a DC component. The DC component is plotted on the horizontal axis and the ratio of AC to DC is expressed as a percentage (e.g., Mod%) and plotted on the vertical axis. Since two different optical signals are measured (i.e., for the red and infrared wavelengths), two points are generated and plotted on the signal quality diagram to uniquely identify the AC and DC components of both the red and infrared optical signals. In Fig. 4, the data points corresponding to the red wavelength are identified by a square and the data points corresponding to the infrared wavelength are identified by a diamond.

[0032] Fig. 4 shows the relative positions of two data points associated with two patients on the signal quality diagram. For a (stable) patient and over a short duration (i.e., of few pulses), all four Ratrat constituents (Red AC, DC; and Infrared AC, DC) remain approximately constant. The data points for patient A indicate a patient with low light levels (i.e., low DC component values) and low modulation (i.e., low Mod%).

These data points could correspond to data from, for example, a chubby, dark-skinned neonate who has poor perfusion, or a reflectance sensor applied to a poorly perfused site (i.e., on the foot). Conversely, the data points for patient B indicate a very translucent patient with good perfusion that results in high light levels.

[0033] The pair of data points for each patient, one data point for red wavelength and one for infrared wavelength, defines the patient's current (Ratrat) conditions. Equivalently, the pair of data points describes the oximeter's "operating point," when the oximeter is monitoring that patient. For a particular patient, the pair of data points can be used to estimate the patient's saturation using equation (5) and a table for saturation versus Ratrat. For example, the Ratrat for patient A is approximately 0.12/0.25 or 0.48. For a typical oximeter, this Ratrat corresponds to a saturation of approximately 100%. The Ratrat for patient B is approximately 6/7 or 0.86, which corresponds to a saturation of approximately 85%.

[0034] In an embodiment, for each particular combination of oximeter model and sensor model, data points are collected for numerous "patients." These data points can be collected under a controlled test environment where true oxygen saturation is known, and an accuracy of the saturation estimated from the red and infrared signals can be determined. Based on the collected data, the diagram can be partitioned into regions corresponding to different levels of quality and accuracy in the saturation estimate. The regions also indicate a quality of the detected signals. Each region is defined by a signal boundary.

[0035] The signal boundaries are dependent on many factors such as the monitor type, sensor type, specifications of components in the sensor (e.g., wavelength, LED characteristics), and other factors. In an embodiment, sensor specific boundaries are stored in the sensor memory or other locations associated with the sensor.

[0036] Fig. 5 shows a sensor signal quality diagram having defined regions corresponding to different confidence levels in the saturation estimate. A display region 510 defines a portion of the signal quality diagram associated with saturation estimates that satisfy a predetermined quality and accuracy level and merit posting (or displaying) on the monitor. Display region 510 includes the set of "patient conditions" resulting in sufficiently accurate saturation estimates for a particular application. Accordingly, when the data points fall within display region 510, the saturation estimate (which is derived from the data points) is posted. Conversely, when the data points fall outside display region 510 into a non-display region 512, the saturation estimate corresponding to these data points is not posted on the oximeter display. Non-display region 512 lies outside, and generally surrounds, display region 510.

[0037] The detected signal corresponding to the red LED is generally "weaker" than the detected signal from the infrared LED. Since this characteristic is known a priori, the oximeter can be designed to account for this difference. In one implementation, the red LED is associated with a first display region and the infrared LED is associated with a second display region. For example, referring to Fig. 5, the red display region is defined by lines 520, 522, 526, and 528, and the infrared display region is defined by lines 520, 524, 526, and 530. Since the red signals are generally weaker than the infrared signal, the boundary of the red display region tends to be closer to the lower left corner of the signal quality diagram.

[0038] The display region is generally dependent on numerous operating conditions. For example, ambient light typically adds to the detected optical signals (i.e., increases the DC components) and thus alters the display region. In this case, the display region can be adjusted to account for the contribution from (or distortion introduced by) ambient light. For example, display regions can be generated for typical office lighting conditions (i.e., 5000 lumens/meter² at 120 Hz AC) and for bright sunlight. The appropriate display region for the applicable operating condition is recalled for use (i.e., by the clinician or by the oximeter automatically based on sensed operating conditions).

[0039] Fig. 6 shows a signal quality diagram having defined display and non-display regions (similar to those of Fig. 5) and a transition zone 614. Transition zone 614 includes regions of the diagram that lie between the display and non-

display regions. The transition zone represents regions associated with a different (e.g., intermediate) quality and accuracy level than those of the display and non-display regions. A different set of criteria can be used when evaluating data points that fall within the transition zone, as described below.

[0040] The regions shown in Figs. 5 and 6 are only representatives of a particular oximeter/sensor combination and for a particular set of operating conditions. Each oximeter (or each oximeter model or type) is typically associated with its own set of display and non-display regions, which may differ from those shown in Figs. 5 and 6. Some oximeters may even have poorly defined non-display regions, where the boundaries vary depending on a set of factors. These factors include the signal-to-noise ratio (SNR) of the oximeter, the amount of ambient light, the wavelength of the sensor LEDs, and so on.

[0041] In an embodiment, the oximeter operates in accordance with the following set of rules:

- If both data points (i.e., for the red and infrared signals) fall within their respective display regions, the oximeter posts the result (e.g., the saturation estimate, and heart rate).
- If either data point falls within its non-display region, the oximeter does not post the result.
- In all other cases, the oximeter may or may not post the result. These cases include instances in which one of the signals falls in the transition zone and neither signal falls in the non-display region.

[0042] Thus, the saturation estimate is posted if the modulation percentage (Mod%) and the light level (DC components) for both the red and infrared wavelengths fall within the bounded areas of their respective display regions. In an embodiment, if the red signal falls within the red non-display region or if the infrared signal falls within the infrared non-display region, or both, then the oximeter does not post the saturation estimate. It can be noted that other sets of rules can also be applied. For example, in another embodiment, the result is posted if one of the data points falls within its display region and the other data point falls within the transition zone. In yet another embodiment, the oximeter posts the saturation estimate and also indicates either the regions in which the data points fall or a confidence level based on the regions in which the data points fall.

[0043] For clarity, Fig. 5 shows only display and non-display regions. These regions correspond to data points that are to be displayed and not displayed. However, additional regions can be defined within the signal quality diagram, with the additional regions corresponding to different confidence levels in the saturation estimate. Generally, the confidence level is high for data points that fall near the center of the diagram and decreases as the data points move away from the center. For the embodiment having multiple confidence levels, the oximeter can display the saturation estimate along with the confidence level.

[0044] For example, an "inactive" region can be defined and used to indicate when a sensor is not applied to a patient. The inactive region be used to detect and notify when the sensor has been removed (i.e., fallen off) the patient. The inactive region lies outside the display and transition regions, correlates to measurements from sensors that are not attached to patients, and typically comprises a portion of the non-display region. This region can be defined through simulation or through empirical measurements. The oximeter computes the data points in the manner described above. If the data points fall inside the inactive region, the oximeter displays an indication that the sensor has been removed from the patient.

[0045] Fig. 7 shows a flow diagram of an embodiment of the measurement display process of the invention. At a step 712, one or more signals indicative of a physiological parameter are detected. For an oximeter used to measure oxygen saturation, this detecting step may include, for example, receiving optical signals from two LEDs and conditioning these signals. At a step 714, the detected signal(s) are processed to generate intermediate data points. For oxygen saturation, this processing step may include filtering the data samples to generate DC and AC components, and using these components to generate the modulation percentage (Mod%). The intermediate data points would include filtered values for the DC component and computed values of the modulation percentage. The intermediate data points are then compared against a signal quality diagram (step 716). This diagram is generated previously, in a manner described above.

[0046] At step 718, it is determined whether the intermediate data points fall within the display region. If the answer is yes, the physiological parameter is estimated based on the detected and processed signal(s). For example, the oxygen saturation can be estimated from the computed Mod% for the two LEDs using equation (5). At step 722, the estimated physiological parameter is displayed, and the process terminates.

[0047] If it is determined at step 718 that the data points do not fall within the display region, a determination is made whether the data points fall within the inactive region (step 724). If the answer is yes, an error message is displayed at step 726. This error message may inform the clinician of the error data points (e.g., "ERROR MEASUREMENT"), provide a suggestion (e.g., "TRY ANOTHER SITE"), and so on. The process then terminates. In some embodiments of the invention, step 724 is not performed.

[0048] If it is determined at step 724 that the data points do not fall within the inactive region, a determination is made whether the data points fall within the non-display region, at a step 730. If the answer is yes, the measurement is not displayed. An error message may be displayed to inform the clinician. This error message may inform the clinician of

the invalid data points (e.g., "INVALID MEASUREMENT" or "WEAK SIGNAL"), provide a suggestion (e.g., "TRY ANOTHER SITE"), and so on. The process then terminates.

[0049] If it is determined at step 730 that the data points do not fall within the non-display region, a determination is made whether the data points fall within the transition region, at step 736. If the answer is yes, a warning message may be displayed to warn the clinician. This warning message may indicate that the data points are of questionable accuracy (e.g., "INACCURATE MEASUREMENT" or "WEAK SIGNAL"), provide a suggestion (e.g., "TRY ANOTHER SITE"), and so on. The physiological parameter may also be computed and displayed along with the warning message. The process then terminates. In some embodiments of the invention, step 736 is not performed.

[0050] Fig. 8 shows a signal quality diagram with data collected from a patient population. The patient data can be used to define the display and non-display regions, to characterize the patient population's mean modulation percentage and mean nAv for both red and infrared wavelengths, to characterize measurement ambiguity that is indicative of the instrument's accuracy, or a combination of the above. Ambiguity can be characterized as the mean error (i.e., bias error) of the instrument measurement and the stability (i.e., fluctuation or wander) of the readings.

[0051] The ambiguity, or estimated error, for various combinations of modulation and DC component are then plotted on the signal quality diagram. The average saturation, saturation bias, saturation wander, and ambiguity can be computed using equal weighting (i.e., giving the same importance for each data point) or unequal weighting that accounts for population statistics (i.e., giving less importance to data points that occur more rarely). Signal specification boundaries can also be obtained for a particular patient sub-population (e.g., perinatal patients) to further improve accuracy in the measurement reporting when the instrument is used for that particular patient sub-population.

[0052] Fig. 9 shows a signal quality diagram that includes ambiguity contours plotted over a portion of the display region. Each contour line corresponds to a particular ambiguity, in saturation points. As an example, at an infrared operating point of 10 nAv and three percent modulation, the plots show an ambiguity of between 10 and 12 saturation points. The contour lines can be generated by collecting data points, grouping the data points that have similar infrared DC components, and selecting a representative ambiguity for those data points. The selected ambiguities for the groups of data points are plotted as a two-dimensional contour plot.

[0053] In an embodiment, the largest ambiguity in each group is selected as representative of the group and a contour plot of the worse case ambiguity is generated. This information is useful, for example, in an oximeter having a guaranteed limit on the saturation ambiguity, and only data points within the guaranteed limit are posted. Other variations of the contour plots shown in Fig. 9 are possible. For example, contour plots can be generated for: (1) the worse case ambiguity, (2) the average ambiguity, (3) the worse case or average absolute value of the bias, (4) the worse case or average value of the wander, and others. The average ambiguity contour plots are generated based on the average of the ambiguities obtain for each group, and are useful for indicating typical ambiguity that is likely to occur for that modulation and infrared DC component.

[0054] The contour plots on the signal quality diagram can also be adjusted for, or take into account, different pulse rates and abnormal heart rhythms such as arrhythmias, premature ventricular contractions, bigeminy, fibrillation, cardiac arrest, and other cardiac pathologies.

[0055] The invention provides advantages not available in conventional oximeters. For example, by detecting data points corresponding to saturation estimates having a low degree of confidence and discarding these estimates (or indicating the low degree of confidence), the invention provides an oximeter having improved diagnostic accuracy and reliability. This ensures that the results relied upon by the clinician meet a predetermined reliability criteria. The invention may also be used to detect and notify when the sensor has been removed (i.e., fallen off) the patient, as described above.

[0056] The oximeter of the invention can also be used to assist the clinician take more accurate measurements. This is a particularly useful application of the invention since it is known that some clinicians move the sensor to various parts of the patient in an attempt to obtain better readings. To assist the clinician, the oximeter can be programmed to display an indicator signal that indicates whether a selected site is good or poor for application of the sensor. This prompt may also be used to assist a less experienced clinician administer the saturation measurement.

[0057] The invention can be used for various physiological measurements. The application of the invention to pulse oximetry has been described as only one preferred embodiment. The invention can also be applied to other physiological measurements such as ECG, blood pressure, temperature, heart rate, and so on. Accordingly, the invention is not to be limited for use only with oximetry or pulse oximetry. The foregoing description of the preferred embodiments is provided to enable any person skilled in the art to make or use the present invention. Various modifications to these embodiments will be readily apparent to those skilled in the art, and the generic principles defined herein may be applied to other embodiments without the use of further invention. For example, the invention can be applied to measurements of other physiological characteristics.

Claims

1. A monitor for providing an indication of an accuracy of an estimated physiological characteristic of a patient, the monitor (110) being connectable to a sensor (130) that detects signals indicative of at least one physiological characteristic of the patient (132), the monitor (110) comprising:

at least one receiving circuit (250) configured to receive the signals indicative of the at least one physiological characteristic and data defining a plurality of sensor signal specification boundaries for the detected signals, the boundaries being indicative of a quality of the signals detected by the sensor (130) and an accuracy of the physiological characteristic estimated from the detected signals;

at least one processing circuit (252) configured to estimate the physiological characteristic of the patient based on the received signals, compare the received signals against the sensor signal specification boundaries, and generate the indication of the accuracy of the estimated physiological characteristic; and means (254) for providing the indication of the accuracy of the estimated physiological characteristic to a user of the monitor (110),

wherein said at least one processing circuit (252) is configured to determine to display or not display the estimate of the physiological characteristic based on the signals and their relationship relative to the plurality of sensor signal specification boundaries and to a plurality of monitor boundaries preprogrammed into the monitor (110).

2. The monitor of claim 1, wherein the sensor signal specification boundaries are indicative of a transition between a signal regime considered normal for the sensor in its usual application and a signal regime considered to be abnormal.
3. The monitor of claim 2, wherein the at least one processing circuit (252) is further configured to determine whether the received signals are within the normal regime or the abnormal regime.
4. The monitor of claim 2, wherein the at least one processing circuit (252) is further configured to compute an indication of whether the sensor (130) is likely to be applied to patient (132) or has partially or entirely come off the patient (132).

5. A physiological monitoring system comprising a monitor (110) according to claim 1 and further comprising:

a sensor (130) that includes a detector for detecting signals from a patient which are indicative of at least one physiological characteristic of the patient;

a memory (236a) associated with the sensor (130) and configured to store data defining sensor signal specification boundaries for the detected signals.

6. A physiological monitoring system according to claim 5, wherein the boundaries are indicative of a transition between a signal regime considered normal for the sensor (130) in its usual application, and a signal regime considered to be abnormal.

7. A physiological monitoring system according to one of the claims 5-6, wherein said boundaries are characteristic of a model of the sensor (130).

8. A physiological monitoring system according to one of the claims 5-7, wherein said boundaries are characteristic of individual components used in making the sensor (130).

9. A physiological monitoring system according to one of the claims 5-8, further comprising means (254) for informing a user of the system as to whether the signal is normal or abnormal.

10. A physiological monitoring system according claim 9, wherein said means (254) for informing the user is an alarm that is triggered when the signal moves from said normal regime to said abnormal regime.

11. A physiological monitoring system according to claim 9 or 10, wherein said normal regime is one in which the sensor (130) is likely to be properly applied to the patient and said abnormal regime is one in which the sensor may have partially or entirely come off the patient.

12. A physiological monitoring system according to one of the claims 5-11, wherein the boundaries include limits for an AC modulation component of the signals.

13. A physiological monitoring system according to one of the claims 5-12, wherein the boundaries include limits for a DC component of the signals.
14. A physiological monitoring system according to one of the claims 5-13, wherein the monitor (110) calculates values from the signals, wherein the sensor signal specification boundaries constitute limits on the AC and DC components of the calculated values, and wherein the AC and DC components are dependent on either a physiological status of the patient, sensor type, or sensor location.
15. A physiological monitoring system according to one of the claims 5-14, wherein the signals detected from the patient include first and second sets of signals derived from detected light scattered from the patient, the light having first and second wavelengths, the signals derived from detected light each having an AC modulation component and a DC component, and the boundary including limits on the AC and DC components.
16. A physiological monitoring system according to claim 15, wherein the signals derived from detected light are indicative of an arterial oxygen saturation of the patient.
17. A physiological monitoring system according to one of the claims 5-16, wherein the memory comprises a digital memory (236a) configured to store a digital representation of the sensor signal specification boundaries, and wherein the physiological characteristic is arterial oxygen saturation.
18. A physiological monitoring system according to one of the claims 5-17, wherein the *monitor (110) displays an indication of the quality of the signals based on their relationship relative to the plurality of sensor boundaries and to a plurality of monitor boundaries preprogrammed into the monitor (110).

Patentansprüche

1. Überwachungsvorrichtung zum Bereitstellen einer Anzeige einer Genauigkeit einer geschätzten physiologischen Charakteristik eines Patienten, wobei die Überwachungsvorrichtung (110) mit einem Sensor (130) verbindbar ist, der Signale detektiert, die indikativ für zumindest eine physiologische Charakteristik des Patienten (132) sind, wobei die Überwachungsvorrichtung (110) umfasst:
 - zumindest eine Empfangsschaltung (250), konfiguriert zum Empfangen der Signale, die indikativ für die zumindest eine physiologische Charakteristik sind, sowie Daten, die eine Vielzahl von Sensorsignalspezifikationsgrenzen für die detektierten Signale definieren, wobei die Grenzen indikativ für eine Qualität der Signale sind, die vom Sensor (130) detektiert werden, sowie für eine Genauigkeit der physiologischen Charakteristik, geschätzt von den detektierten Signalen;
 - zumindest eine Verarbeitungsschaltung (252), konfiguriert zum Schätzen der physiologischen Charakteristik des Patienten, basierend auf den empfangenen Signalen, Vergleichen der empfangenen Signale gegen die Sensorsignalspezifikationsgrenzen, und Erzeugen der Anzeige der Genauigkeit der geschätzten physiologischen Charakteristik; und
 - Mittel (254) zum Bereitstellen der Anzeige der Genauigkeit der geschätzten physiologischen Charakteristik an einen Benutzer der Überwachungsvorrichtung (110),
- wobei die zumindest eine Verarbeitungsschaltung (252) konfiguriert ist, zu bestimmen, die Schätzung der physiologischen Charakteristik anzuzeigen oder nicht anzuzeigen, basierend auf den Signalen und deren Beziehung relativ zu der Vielzahl von Sensorsignalspezifikationsgrenzen und zu einer Vielzahl von Überwachungsgrenzen, vorprogrammiert in die Überwachungsvorrichtung (110).
2. Überwachungsvorrichtung nach Anspruch 1, bei welcher die Sensorsignalspezifikationsgrenzen indikativ sind für einen Übergang zwischen einer Signalordnung, die als normal für den Sensor in seiner üblichen Anwendung betrachtet wird, und einer Signalordnung, die als anormal betrachtet wird.
3. Überwachungsvorrichtung nach Anspruch 2, bei welcher die zumindest eine Verarbeitungsschaltung (252) ferner konfiguriert ist, zu bestimmen, ob die empfangenen Signale innerhalb der normalen Ordnung oder der anormalen Ordnung liegen.
4. Überwachungsvorrichtung nach Anspruch 2, bei welcher die zumindest eine Verarbeitungsschaltung (252) ferner

konfiguriert ist, eine Anzeige zu berechnen, ob es für den Sensor (130) wahrscheinlich ist, dass er am Patienten (132) angebracht ist, oder ob er sich teilweise oder vollständig vom Patienten (132) abgelöst hat.

- 5 5. Physiologisches Überwachungssystem, umfassend eine Überwachungsvorrichtung (110) gemäß Anspruch 1 und ferner umfassend:

10 einen Sensor (130), der einen Detektor beinhaltet zum Detektieren von Signalen von einem Patienten, welche
indikativ sind für zumindest eine physiologische Charakteristik des Patienten;
einen Speicher (236a), dem Sensor (130) zugewiesen und konfiguriert, Daten zu speichern, die Sensorsignal-
spezifikationsgrenzen für die detektierten Signale definieren.

- 15 6. Physiologisches Überwachungssystem nach Anspruch 5, bei welchem die Grenzen indikativ sind für einen Übergang zwischen einer Signalordnung, die als normal für den Sensor (130) in seiner üblichen Anwendung betrachtet wird, und einer Signalordnung, die als anormal betrachtet wird.

7. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 6, bei welchem die Grenzen charakteristisch für ein Modell des Sensors (130) sind,

- 20 8. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 7, bei welchem die Grenzen charakteristisch für individuelle Komponenten sind, die in der Herstellung des Sensors (130) verwendet werden.

9. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 8, ferner umfassend Mittel (254) zum Informieren eines Benutzers des Systems, ob das Signal normal oder anormal ist.

- 25 10. Physiologisches Überwachungssystem nach Anspruch 9, bei welchem die Mittel (254) zum Informieren des Benutzers ein Alarm sind, der ausgelöst wird, wenn sich das Signal von der normalen Ordnung zur anormalen Ordnung bewegt.

- 30 11. Physiologisches Überwachungssystem nach Anspruch 9 oder 10, bei welchem die normale Ordnung eine ist, in welcher es für den Sensor (130) wahrscheinlich ist, dass er richtig am Patienten angebracht ist, und die anormale Ordnung eine ist, in welcher der Sensor sich teilweise oder vollständig vom Patienten abgelöst haben kann.

- 35 12. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 11, bei welchem die Grenzen Grenzwerte beinhalten für eine Wechselstrommodulationskomponente der Signale.

13. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 12, bei welchem die Grenzen Grenzwerte beinhalten für eine Gleichstromkomponente der Signale.

- 40 14. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 13, bei welchem die Überwachungsvorrichtung (110) Werte von den Signalen berechnet, wobei die Sensorsignalspezifikationsgrenzen Grenzwerte bezüglich der Wechselstrom- und Gleichstromkomponenten der berechneten Werte darstellen, und wobei die Wechselstrom- und Gleichstromkomponenten abhängig sind von entweder einem physiologischen Status des Patienten, dem Sensortyp oder dem Sensorort.

- 45 15. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 14, bei welchem die vom Patienten detektierten Signale erste und zweite Gruppen von Signalen beinhalten, abgeleitet von detektiertem Licht, das vom Patienten gestreut wird, wobei das Licht erste und zweite Wellenlängen aufweist, wobei die Signale, die vom detektierten Licht abgeleitet sind, jeweils eine Wechselstrommodulationskomponente und eine Gleichstromkomponente aufweisen und die Grenze Grenzwerte bezüglich der Wechselstrom- und Gleichstromkomponenten beinhaltet.

- 50 16. Physiologisches Überwachungssystem nach Anspruch 15, bei welchem die Signale, die vom detektierten Licht abgeleitet sind, indikativ sind für eine arterielle Sauerstoffsättigung des Patienten.

- 55 17. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 16, bei welchem der Speicher einen digitalen Speicher (236a) umfasst, konfiguriert, eine digitale Darstellung der Sensorsignalspezifikationsgrenzen zu speichern, und wobei die physiologische Charakteristik die arterielle Sauerstoffsättigung ist.

18. Physiologisches Überwachungssystem nach einem der Ansprüche 5 bis 17, bei welchem die Überwachungsvor-

richtung (110) eine Anzeige der Qualität der Signale anzeigt, basierend auf deren Verhältnis relativ zur Vielzahl der Sensorgrenzen und zu einer Vielzahl von Überwachungsgrenzen, die in die Überwachungsvorrichtung (110) vorprogrammiert sind.

5

Revendications

10

1. Moniteur permettant de donner une indication d'une précision d'une caractéristique physiologique estimée d'un patient, le moniteur (110) pouvant être relié à un capteur (130) qui détecte des signaux indiquant au moins une caractéristique physiologique du patient (132), le moniteur (110) comprenant :

15

au moins un circuit de réception (250) configuré pour recevoir les signaux indiquant la au moins une caractéristique physiologique et les données définissant une pluralité de limites de spécification du signal du capteur pour les signaux détectés, les limites indiquant une qualité des signaux détectés par le capteur (130) et une précision de la caractéristique physiologique estimée à partir des signaux détectés ;
au moins un circuit de traitement (252) configuré pour estimer la caractéristique physiologique du patient en fonction des signaux reçus, pour comparer les signaux reçus par rapport aux limites de la spécification du signal du capteur, et pour générer l'indication de la précision de la caractéristique physiologique estimée ; et
un moyen (254) permettant de donner l'indication de la précision de la caractéristique physiologique estimée à un utilisateur du moniteur (110),

20

25

dans lequel ledit au moins un circuit de traitement (252) est configuré pour déterminer s'il faut afficher ou non l'estimation de la caractéristique physiologique en fonction des signaux et de leur relation par rapport à la pluralité de limites de spécification du signal du capteur et à une pluralité de limites du moniteur préprogrammées dans le moniteur (110).

30

2. Moniteur selon la revendication 1, dans lequel les limites de spécification du signal du capteur indiquent une transition entre un régime de signal considéré comme normal pour le capteur dans son application habituelle et un régime de signal considéré comme anormal.

35

3. Moniteur selon la revendication 2, dans lequel le au moins un circuit de traitement (252) est en outre configuré pour déterminer si les signaux reçus appartiennent au régime normal ou au régime anormal.
4. Moniteur selon la revendication 2, dans lequel le au moins un circuit de traitement (252) est en outre configuré pour calculer une indication permettant de savoir si le capteur (130) est susceptible d'être appliqué au patient (132) ou a partiellement ou intégralement quitté le patient (132).

40

5. Système de surveillance physiologique comprenant un moniteur (110) selon la revendication 1 et comprenant en outre :

45

un capteur (130) qui inclut un détecteur permettant de détecter les signaux provenant d'un patient qui indiquent au moins une caractéristique physiologique du patient ;
une mémoire (236a) associée au capteur (130), et configurée pour stocker des données définissant des limites de spécification du signal du capteur pour les signaux détectés.

50

6. Système de surveillance physiologique selon la revendication 5, dans lequel les limites indiquent une transition entre un régime de signal considéré comme normal pour le capteur (130) dans son application habituelle, et un régime de signal considéré comme anormal.

55

7. Système de surveillance physiologique selon l'une quelconque des revendications 5 et 6, dans lequel lesdites limites sont caractéristiques d'un modèle du capteur (130).
8. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 7, dans lequel lesdites limites sont caractéristiques des composants individuels utilisés lors de la fabrication du capteur (130).
9. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 8, comprenant en outre :

un moyen (254) permettant d'informer un utilisateur du système du fait que le signal est normal ou anormal.

10. Système de surveillance physiologique selon la revendication 9, dans lequel ledit moyen (254) permettant d'informer l'utilisateur est une alarme qui est déclenchée lorsque le signal passe dudit régime normal audit régime anormal.
- 5 11. Système de surveillance physiologique selon la revendication 9 ou 10, dans lequel ledit régime normal est un régime dans lequel le capteur (130) est susceptible d'être appliqué de façon adéquate au patient, et ledit régime anormal est un régime dans lequel le capteur peut avoir partiellement ou intégralement quitté le patient.
- 10 12. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 11, dans lequel les limites incluent des limites pour une composante de modulation CA des signaux.
- 15 13. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 12, dans lequel les limites incluent des limites pour une composante CC des signaux.
- 20 14. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 13, dans lequel le moniteur (110) calcule des valeurs à partir des signaux, dans lequel les limites de spécification du signal du capteur constituent les limites des composantes CA et CC des valeurs calculées, et dans lequel les composantes CA et CC dépendent d'un état physiologique du patient, du type de capteur, ou de l'emplacement du capteur.
- 25 15. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 14, dans lequel les signaux détectés provenant du patient incluent les premier et deuxième ensembles de signaux provenant de la lumière détectée diffusée provenant du patient, la lumière ayant des première et deuxième longueurs d'onde, les signaux provenant de la lumière détectée ayant chacun une composante de modulation CA et une composante CC, et la limite incluant des limites sur les composantes CA et CC.
- 30 16. Système de surveillance physiologique selon la revendication 15, dans lequel les signaux provenant de la lumière détectée indiquent une saturation artérielle en oxygène du patient.
- 35 17. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 16, dans lequel la mémoire comprend une mémoire numérique (236a), configurée pour enregistrer une représentation numérique des limites de spécification du signal du capteur, et dans lequel la caractéristique physiologique est la saturation artérielle en oxygène.
- 40 18. Système de surveillance physiologique selon l'une quelconque des revendications 5 à 17, dans lequel le moniteur (110) affiche une indication de la qualité des signaux en fonction de leur relation par rapport à la pluralité des limites du capteur et à une pluralité de limites du moniteur préprogrammées dans le moniteur (110).

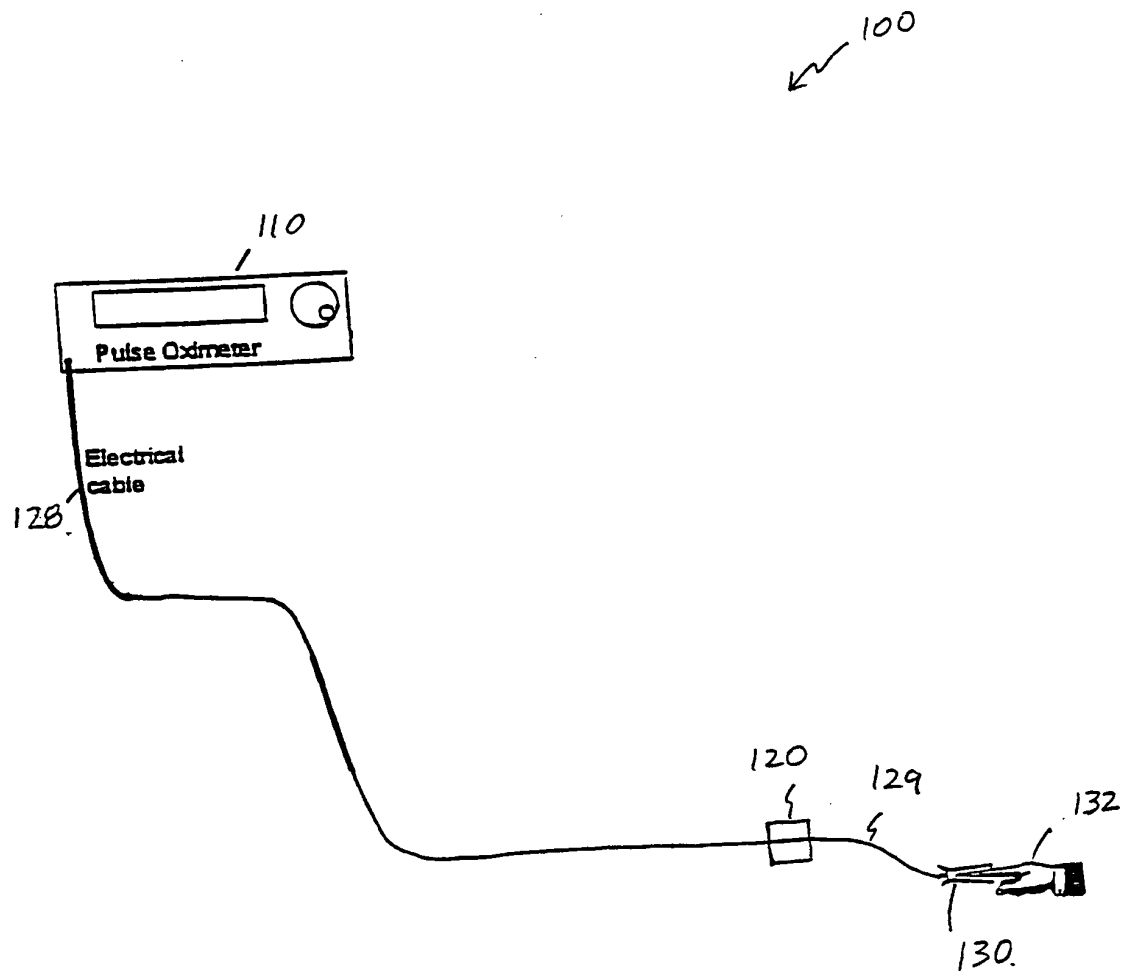


FIG. 1

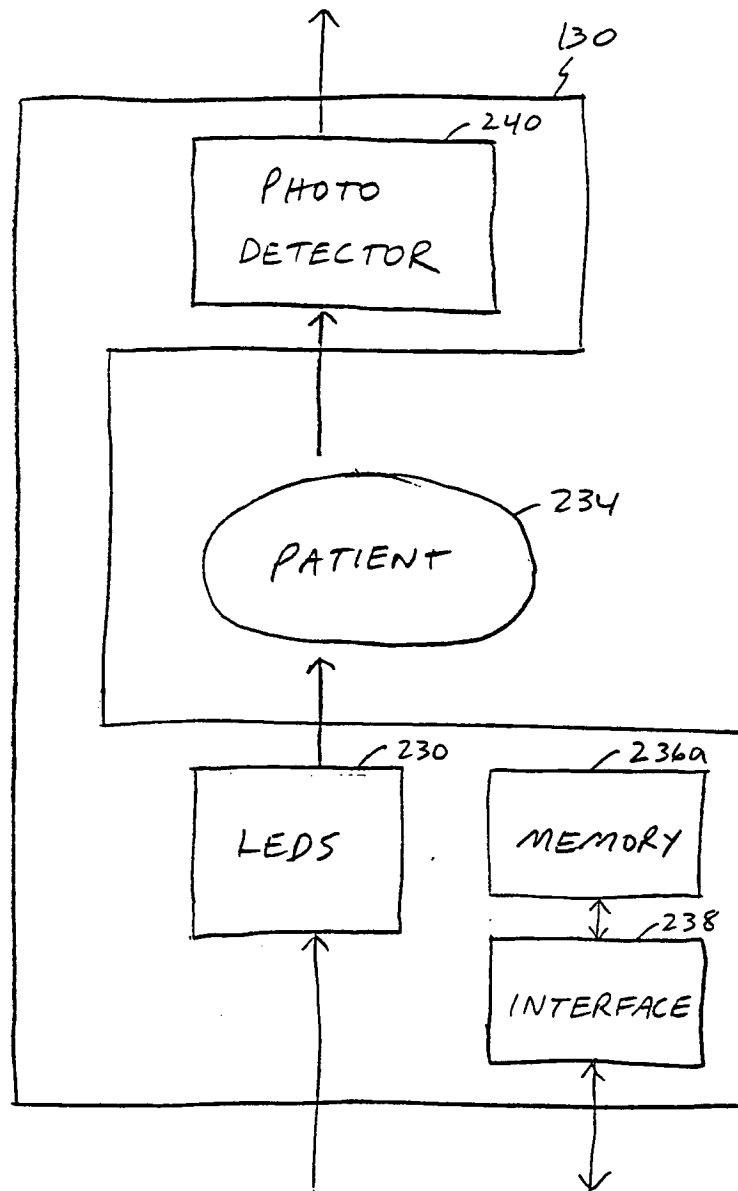


FIG. 2A

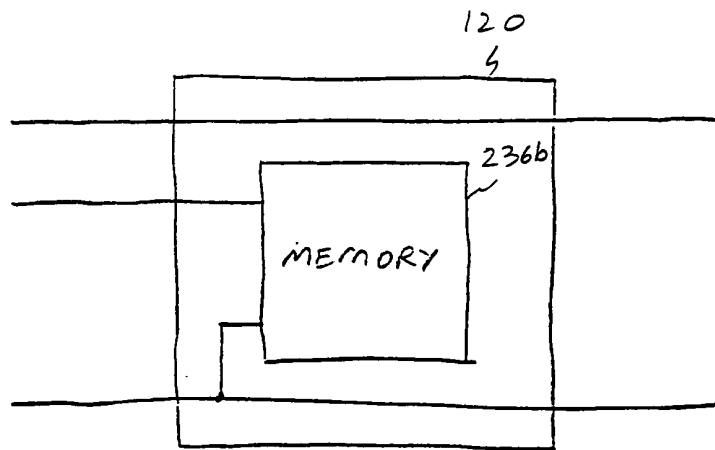


FIG. 2B

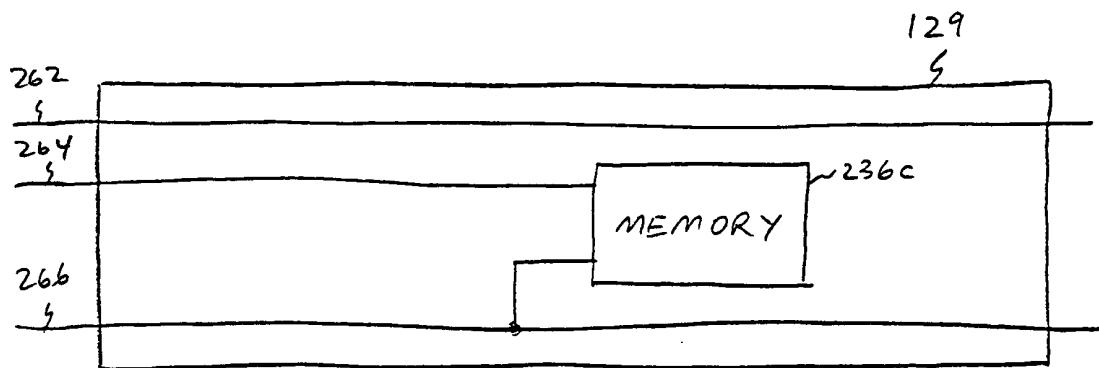


FIG. 2C

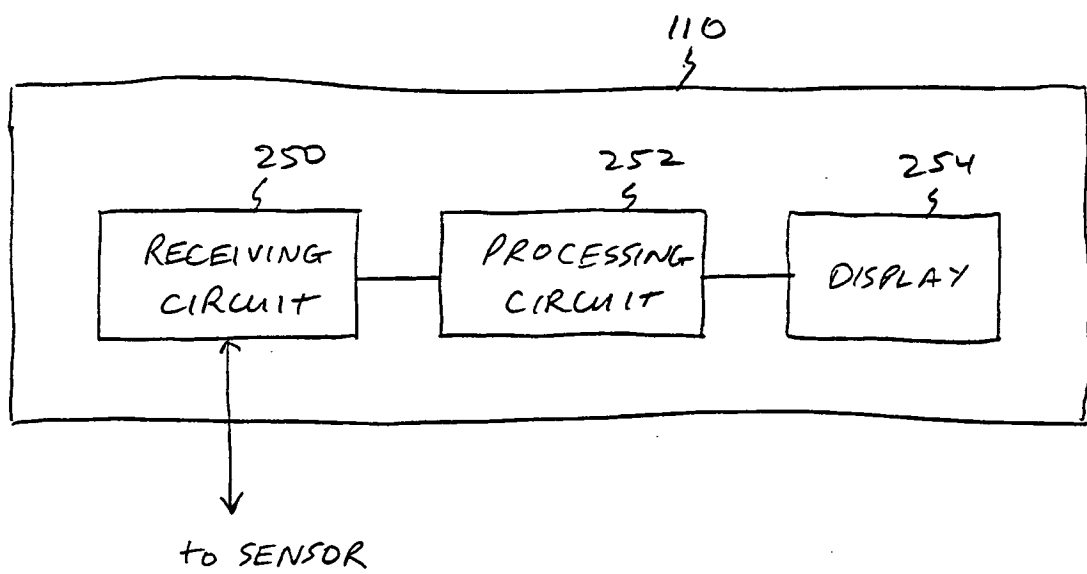


FIG. 2D

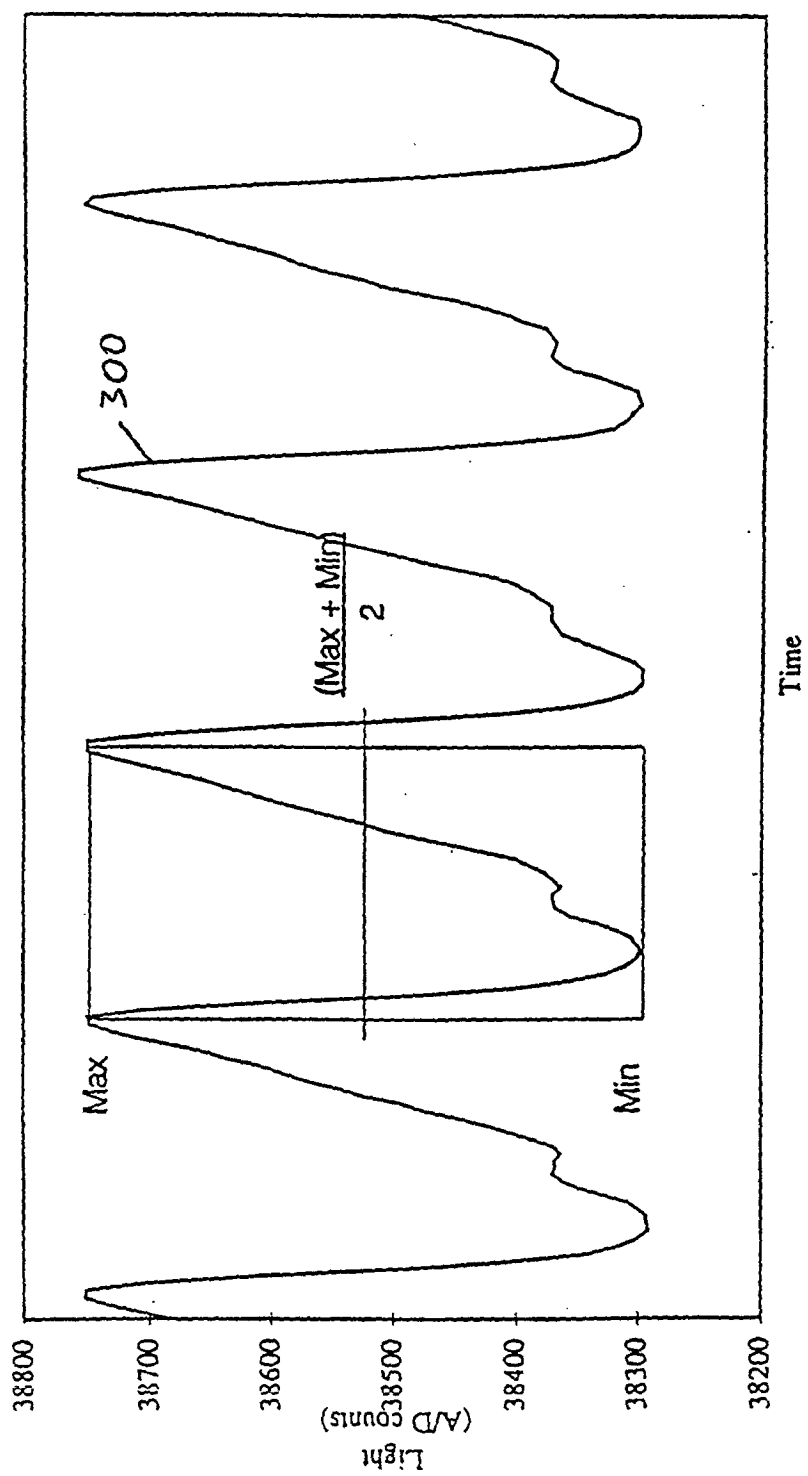


FIG. 3

SIGNAL QUALITY DIAGRAM

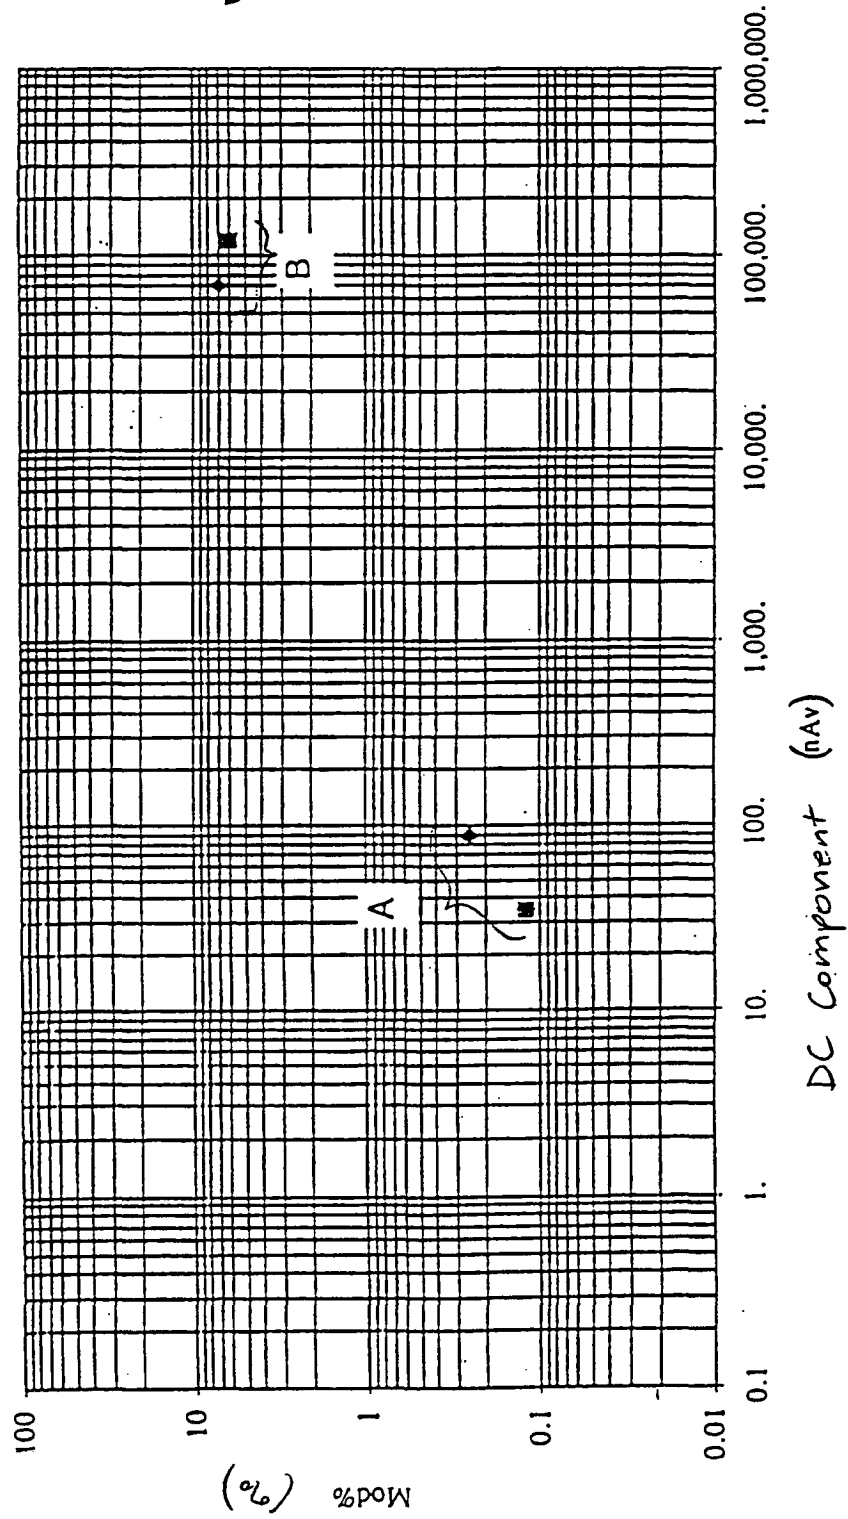


FIG. 4

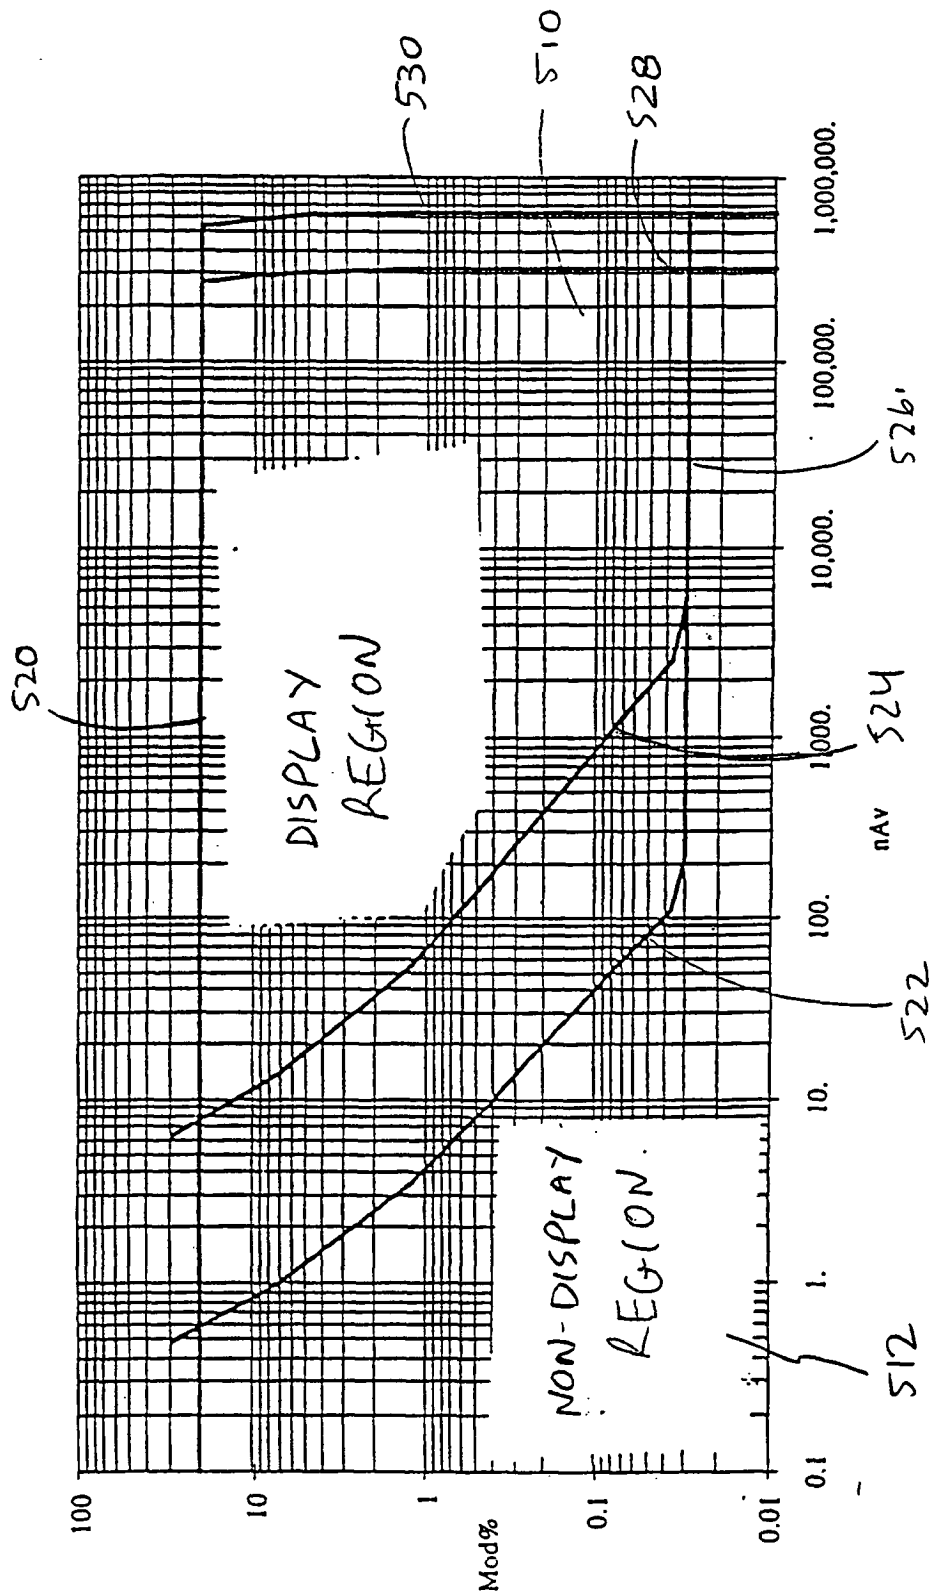


FIG. 5

SIGNAL QUALITY DIAGRAM

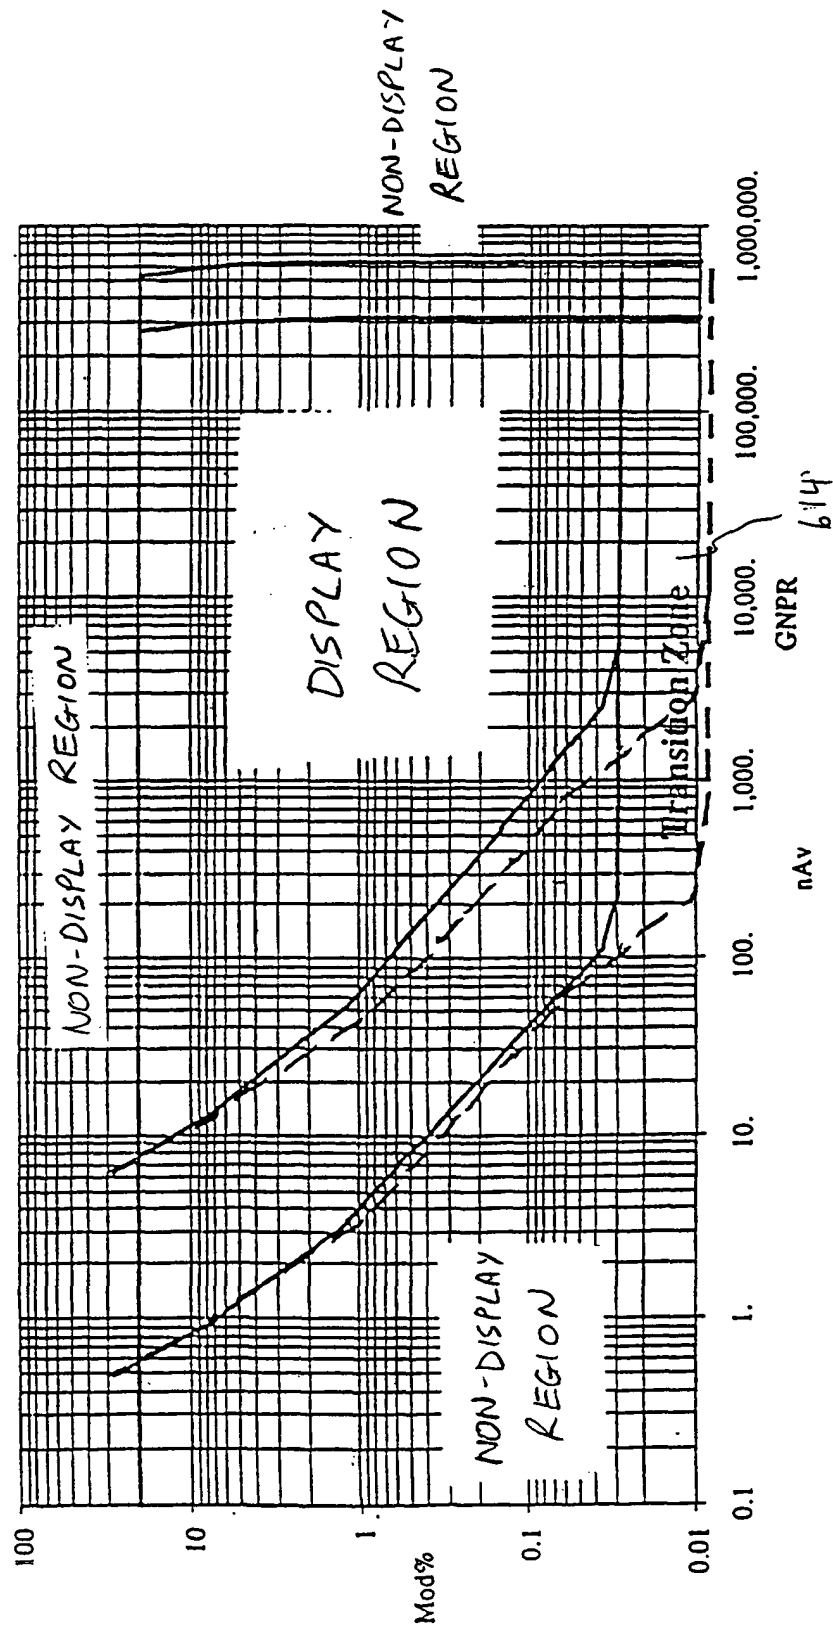


FIG. 6

XX

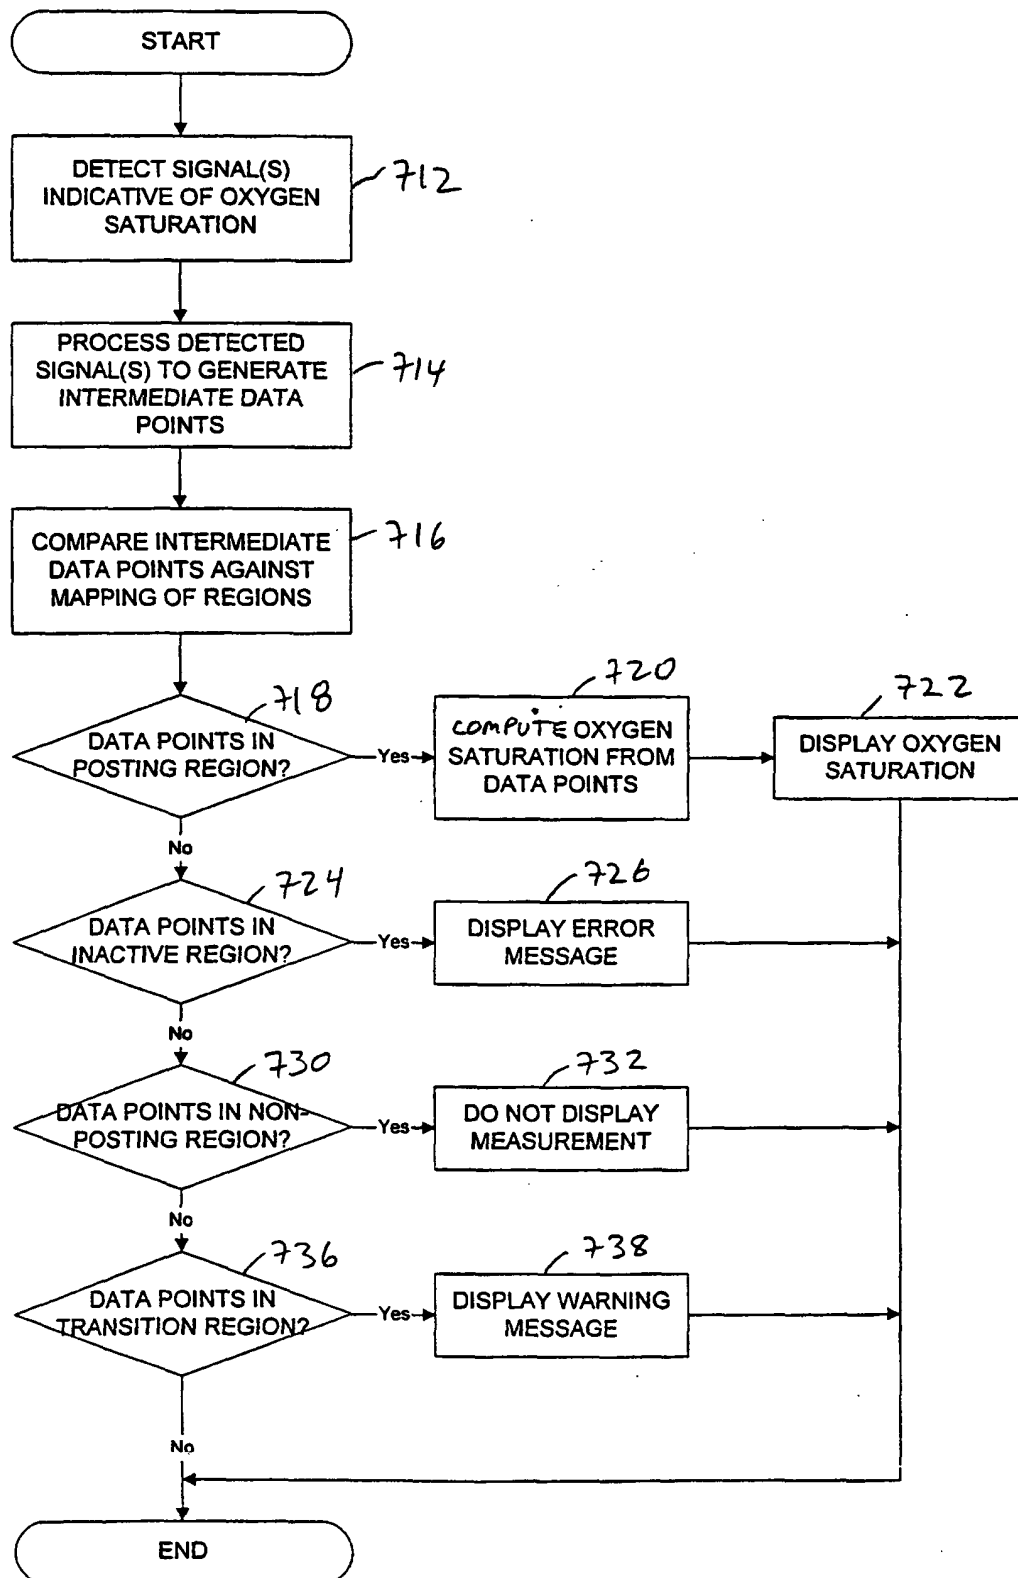


FIG. 7

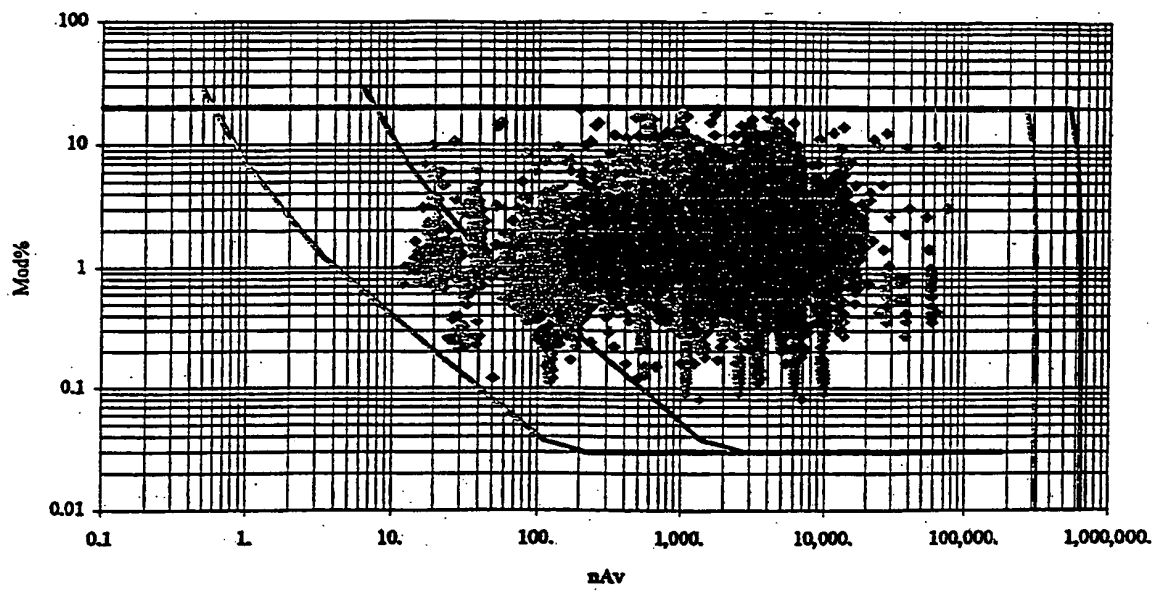


FIG. 8

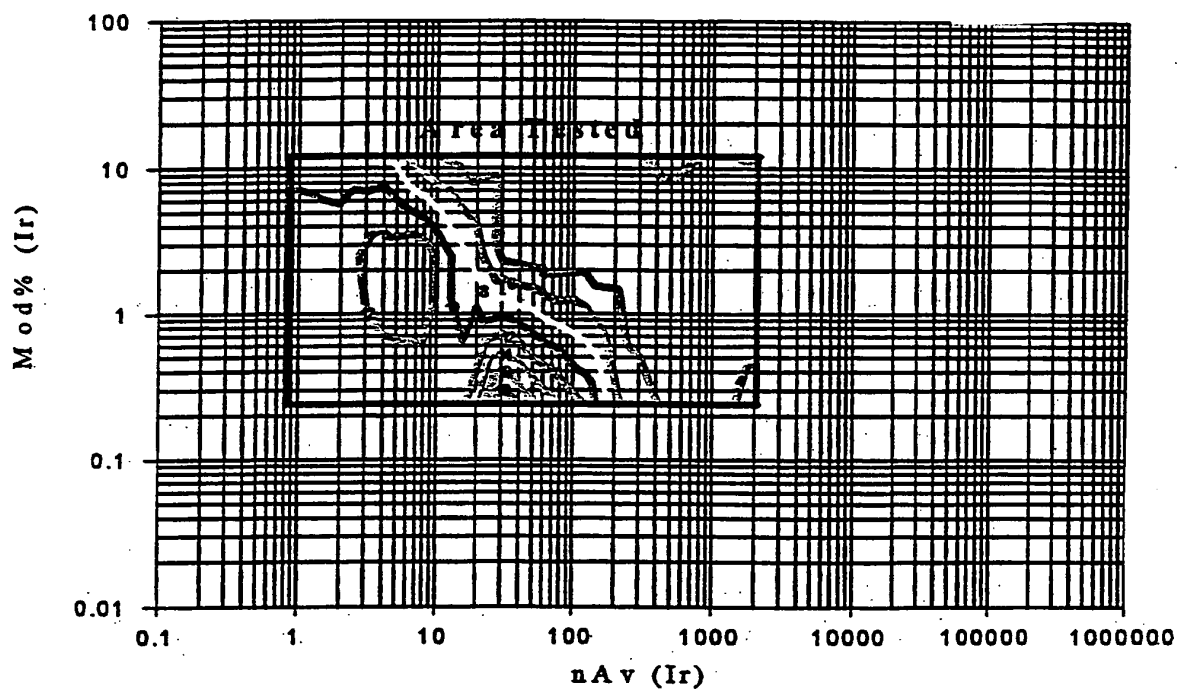


FIG. 9

专利名称(译)	用于指示生理测量的质量和准确度的装置		
公开(公告)号	EP1168959B1	公开(公告)日	2006-11-29
申请号	EP2000923420	申请日	2000-04-14
[标]申请(专利权)人(译)	马林克罗特公司		
申请(专利权)人(译)	马林克罗特INC.		
当前申请(专利权)人(译)	马林克罗特INC.		
[标]发明人	PORGES CHARLES BAKER CLARK YORKLEY THOMAS J BERNSTEIN MICHAEL MANNHEIMER PAUL		
发明人	PORGES, CHARLES BAKER, CLARK YORKLEY, THOMAS, J. BERNSTEIN, MICHAEL MANNHEIMER, PAUL		
IPC分类号	A61B5/00 G01N21/27 A61B5/0245 A61B5/145 A61B5/1455 G01N21/35		
CPC分类号	A61B5/14551 A61B5/7221 Y10T29/49117		
代理机构(译)	GRUBERT , ANDREAS		
优先权	60/129170 1999-04-14 US		
其他公开文献	EP1168959A1		
外部链接	Espacenet		

摘要(译)

用于生理监测系统的传感器和监测器具有指示估计的生理状况的准确性的能力。传感器感测患者的至少一个生理特征并且可连接到监视器，该监视器根据传感器检测到的信号估计生理状况。传感器包括用于检测来自患者的信号的检测器，其指示生理特征。传感器与存储器相关联，该存储器被配置为存储数据，该数据定义检测到的信号的至少一个传感器信号规范边界。边界表示信号的质量和由监视器根据信号估计的生理特征的准确度。传感器还包括用于提供对存储器的访问以允许将定义至少一个传感器边界的数据传输到监视器的装置。

$$AC = Max - Min;$$

$$Eq. (1)$$