

(19)



(11)

EP 1 504 713 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
30.07.2008 Bulletin 2008/31

(51) Int Cl.:
A61B 5/00 ^(2006.01) **A61B 5/055** ^(2006.01)
G21K 1/12 ^(2006.01) **A61B 5/05** ^(2006.01)
A61B 6/00 ^(2006.01)

(21) Application number: **04016056.6**

(22) Date of filing: **08.07.2004**

(54) **Navigation system for cardiac therapies**

Navigationssystem für Herztherapie

Système de navigation pour thérapies cardiaques

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PL PT RO SE SI SK TR**

(30) Priority: **14.07.2003 US 619216**

(43) Date of publication of application:
09.02.2005 Bulletin 2005/06

(73) Proprietor: **Surgical Navigation Technologies, Inc.**
Louisville,
Colorado 80020 (US)

(72) Inventors:
• **Verard, Laurent**
Superior
CO 80027 (US)

• **Hunter, Mark W.**
Broomfield
CO 80020 (US)
• **Bzostek, Andrew**
ERIE
CO 80516 (US)

(74) Representative: **Edlund, Fabian**
AWAPATENT AB
P.O. Box 11 394
404 28 Göteborg (SE)

(56) References cited:
EP-A- 0 930 046 **US-A- 5 353 795**
US-A- 5 377 678 **US-A1- 2001 036 245**
US-A1- 2003 074 011 **US-B1- 6 470 207**

EP 1 504 713 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD OF THE INVENTION

[0001] The present invention relates generally to image guided surgery, and more specifically, to systems for using one or more medical images to assist in navigating an instrument through internal body structures, in particular for navigating a catheter in a moving body structure, such as the heart, during a surgical procedure.

BACKGROUND OF THE INVENTION

[0002] Image guided medical and surgical procedures utilize patient images obtained prior to or during a medical procedure to guide a physician performing the procedure. Recent advances in imaging technology, especially in imaging technologies that produce highly-detailed, two, three, and four dimensional images, such as computed tomography (CT), magnetic resonance imaging (MRI), isocentric C-arm fluoroscopic imaging, positron emission tomography (PET), and ultrasound imaging (US) has increased the interest in image guided medical procedures.

[0003] At present, cardiac catheterization procedures are typically performed with the aid of fluoroscopic images. Two-dimensional fluoroscopic images taken intra-procedurally allow a physician to visualize the location of a catheter being advanced through cardiovascular structures. However, use of such fluoroscopic imaging throughout a procedure exposes both the patient and the operating room staff to radiation, as well as exposes the patient to contrast agents. Therefore, the number of fluoroscopic images taken during a procedure is preferably limited to reduce the radiation exposure to the patient and staff.

[0004] An image guided surgical navigation system that enables the physician to see the location of an instrument relative to a patient's anatomy, without the need to acquire real-time fluoroscopic images throughout the surgical procedure is generally disclosed in U.S. Patent No. 6,470,207, entitled "Navigational Guidance Via Computer-Assisted Fluoroscopic Imaging," issued October 22, 2002. In this system, representations of surgical instruments are overlaid on pre-acquired fluoroscopic images of a patient based on the position of the instruments determined by a tracking sensor.

[0005] Other types of procedures include the use of electro physiologic mapping catheters to map the heart based on measured electrical potentials. Such mapping catheters are useful in identifying an area of tissue that is either conducting normally or abnormally, however, some mapping catheters may not aid in actually guiding a medical device to a targeted tissue area for medical treatment.

[0006] Other procedures that could benefit from a navigation system include cardiac lead placement. Cardiac lead placement is important in achieving proper stimulation or accurate sensing at a desired cardiac location.

Endocardial is one type of lead placement procedure that is an internal procedure where coronary vein leads are generally implanted with the use of a guide catheter and/or a guide wire or stylet to achieve proper placement of the lead. Epicardial is another type of procedure that is an external procedure for cardiac lead placement that may also benefit from this navigation system. A coronary vein lead may be placed using a multi-step procedure wherein a guide catheter is advanced into the coronary sinus ostium and a guide wire is advanced further through the coronary sinus and great cardiac vein to a desired cardiac vein branch. Because the tip of a guide wire is generally flexible and may be preshaped in a bend or curve, the tip of the guide wire can be steered into a desired venous branch. The guide wire tip is directed with a steerable guide catheter, and with the appropriate pressure, it is manipulated into the desired vein branch.

[0007] A cardiac lead may therefore be advanced to a desired implant location using a guide wire extending entirely through the lead and out its distal end. Cardiac leads generally need to be highly flexible in order to withstand flexing motion caused by the beating heart without fracturing. A stiff stylet or guide wire provides a flexible lead with the stiffness needed to advance it through a venous pathway. Leads placed with the use of a stylet or guide wire are sometimes referred to as "over-the-wire" leads. Once the lead is placed in a desired location, the guide wire and guide catheter may be removed. A guide wire placed implantable lead is disclosed in U.S. Pat. No. 6,192,280, entitled "Guide wire Placed Implantable Lead With Tip Seal," issued February 20, 2001. A coronary vein lead having a flexible tip and which may be adapted for receiving a stylet or guide wire is disclosed in U.S. Pat. No. 5,935,160, entitled "Left ventricular access lead for heart failure pacing", issued August 10, 1999.

[0008] Also, pacing lead procedures currently performed today for use in heart failure treatment are not optimized. In this regard, the lead placement is not optimized due to the lack of having real-time anatomic information, navigation and localization information, hemodynamic data, and electrophysiological data. Thus, pacing leads are currently simply "stuffed" into the heart without any optimization being performed due to lack of information that can be used for this optimization.

[0009] Advancement of a guide catheter or an over-the-wire lead through a vessel pathway and through cardiac structures requires considerable skill and can be a time-consuming task. This type of procedure also exposes the patient to an undesirable amount of radiation exposure and contrast agent. Therefore, it is desirable to provide an image guided navigation system that allows the location of a guide catheter being advanced within the cardiovascular structures for lead placement to be followed in either two, three, or four dimensional space in real time. It is also desirable to provide an image guided navigation system that assists in navigating an instrument, such as a catheter, through a moving body structure or any type of soft tissue.

[0010] With regard to navigating an instrument through a moving body structure, difficulties arise in attempting to track such an instrument using known tracking technology as the instrument passes adjacent or through a moving body structure, since the virtual representation of the instrument may be offset from the corresponding anatomy when superimposed onto image data. Accordingly, it is also desirable to acquire image data and track the instrument in a synchronized manner with the pre-acquired image using gating or synchronization techniques, such as ECG gating or respiratory gating.

[0011] Other difficulties with cardiac procedures include annual check-ups to measure early indications for organ rejection in heart transplant patients. These indicators include white blood cells, chemical change, blood oxygen levels, etc. During the procedure, an endovascular biopsy catheter is inserted into the heart and multiple biopsies are performed in the septum wall of the heart. Again, during this procedure, radiation and contrast agent is utilized to visualize the biopsy catheter, thereby exposing both a patient and the doctor to potential excess radiation and contrast agents during the procedure. As such, it would also be desirable to provide an image guided navigation system that assists in performing this type of procedure in order to reduce radiation and contrast agent exposure.

[0012] Other types of surgical procedures also suffer from certain disadvantages. For example, with neurological diseases, these diseases are generally treated and accessed from the cranium down to the neurological site in order to reach tumors, ventricles, or treat different ailments, such as Parkinson's disease. This type of invasive procedure creates significant trauma, such as skull holes, dura opening, fiber destruction, and other cerebral structural damage or leakage. It is, therefore, also desirable to provide a minimally invasive approach to treat such ailments, which are accessible from either vascular or the cerebrospinal fluid tree. Document WO 02/064011 discloses a medical diagnostic device for three-dimensional medical imaging.

[0013] Other types of vascular techniques includes use of a device referred to as an intravascular ultrasound (IVUS) technique. This type of technique is typically used to visualize tissue and/or blood vessels within the patient. This technique involves the use of a disposable catheter that includes an ultrasound transducer positioned within the catheter in order to provide two-dimensional ultrasound images as the catheter is passed through a vessel. However, this type of vascular technique has various drawbacks. For example, this type of disposable IVUS catheter is extremely expensive. Moreover, the ultrasound transducer embedded within the catheter provides only visualization on one side of the catheter, typically orthogonal to the catheter body, and therefore does not provide any forward views or other views about the catheter. Thus, here again, it is also desirable to provide an improved intravascular ultrasound approach, which substantially reduces the cost and increases the field of view

of existing technologies. Still further, it is also desirable to register ultrasound image information with other or multiple image modalities, which are each registered to one another and viewed on a single or multiple displays.

SUMMARY OF THE INVENTION

[0014] In an embodiment, an image guided navigation system for navigating a region of a patient includes an imaging device, an instrument, a first tracking device, a controller and a display. The imaging device is positioned outside the patient and generates image data at the region of the patient. The instrument is navigated in the region of the patient. The first tracking device is attached to the instrument and is used to track the position of the instrument in the region of the patient. The controller generates virtual images along the navigated path of the instrument from the image data generated outside the patient. The display displays the virtual images.

[0015] In another embodiment, a sensor is attached to the instrument and senses a physiological parameter in the patient. The controller tracks the position of the instrument with the tracking device and receives the sensed physiological parameter from the sensor. The controller also estimates the optimized site and superimposes an icon representing the location of the optimized site and an icon representing the instrument, based on the sensed physiological parameter and the position of the instrument. The display displays the icon of the estimated optimized site and the icon representing the instrument in the patient.

[0016] A method includes capturing image data during the physiological event, registering the captured image data to the patient during the physiological event, and displaying the location of the instrument on the image data by superimposing an icon of the instrument on the image data.

[0017] A method for image guiding an instrument to an optimized site includes navigating the instrument in the patient, detecting a location of the instrument, sensing a physiological parameter with the instrument, automatically determining an optimized site to navigate the instrument to and displaying an icon of the optimized site and an icon of the location of the catheter.

[0018] Further areas of applicability of the present invention will become apparent from the detailed description provided hereinafter. It should be understood that the detailed description and specific examples, while indicating the preferred embodiments of the invention, are intended for purposes of illustration only.

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] The present invention will become more fully understood from the detailed description and the accompanying drawings, wherein:

[0020] Figure 1 is a diagram of a catheter navigation system according to the teachings of the present inven-

tion;

[0021] Figures 2a and 2b are diagrams representing undistorted and distorted views from a fluoroscopic C-arm imaging device;

[0022] Figure 3 is a logic block diagram illustrating a method for navigating a catheter during cardiac therapy;

[0023] Figures 4a and 4b are side partial cross-sectional views of a navigable catheter employed in cardiac therapies according to the teachings of the present invention;

[0024] Figure 5 is an axial cross-section view of the navigable catheter shown in Figures 4a and 4b;

[0025] Figure 6 is a logic block diagram illustrating a method for navigating and accessing a statistical atlas and employing the atlas for target suggestions according to the teachings of the present invention;

[0026] Figure 7 is a figure of a display illustrating data available for a landmark accessible by a user of the system;

[0027] Figure 8 is a figure of a display illustrating an adjustable icon or probe diameter;

[0028] Figure 9 is a figure of the display illustrating a straight projection along a direction of a first sensor in the navigable catheter;

[0029] Figure 10 is a figure of the display illustrating a splined projection or trajectory based on a shape of a curve of the navigable catheter;

[0030] Figure 11 is a logic block diagram illustrating a method for navigating the coronary sinus region of the heart;

[0031] Figure 12 is an image of a three-dimensional heart model used for cardiac therapy; and

[0032] Figure 13 is a logic block diagram illustrating in further detail a method for navigating the coronary sinus region of the heart;

[0033] Figures 14a and 14b are images of an ungated and a gated tracked catheter;

[0034] Figures 15a-15c illustrate a navigable catheter employed in cardiac therapies, according to the teachings of the present invention;

[0035] Figure 16 is another embodiment of a catheter employed in cardiac therapies, according to the teachings of the present invention;

[0036] Figure 17a and 17b illustrate a navigable biopsy instrument, according to the teachings of the present invention;

[0037] Figures 18a and 18b illustrate a prior art intravascular ultrasound (IVUS) catheter;

[0038] Figure 19 illustrates a virtual intravascular ultrasound catheter, according to the teachings of the present invention;

[0039] Figure 20 illustrates a virtual intravascular ultrasound system, according to the teachings of the present invention;

[0040] Figure 21 illustrates an exemplary catheter utilized according to the teachings of the present invention;

[0041] Figure 22 illustrates an exemplary tracking insert utilized with the catheter of Figure 21; and

[0042] Figure 23 illustrates the assembly of the insert and catheter of Figures 21 and 22 according to the teachings of the present invention.

5 DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0043] The following description of the preferred embodiment(s) is merely exemplary in nature and is in no way intended to limit the invention, its application, or uses. As indicated above, the present invention is directed at providing improved, non-line-of-site image-guided navigation of an instrument, such as a catheter, balloon catheter, implant, lead, stent, needle, guide wire, insert and/or capsule, that may be used for physiological monitoring, delivering a medical therapy, or guiding the delivery of a medical device in an internal body space, such as the heart or any other region of the body.

[0044] Figure 1 is a diagram illustrating an overview of an image-guided catheter navigation system 10 for use in non-line-of-site navigating of a catheter during cardiac therapy or any other soft tissue therapy. It should further be noted that the navigation system 10 may be used to navigate any other type of instrument or delivery system, including guide wires, needles, drug delivery systems, cell delivery systems, gene delivery systems and biopsy systems. Moreover, these instruments may be used for cardiac therapy or any other therapy in the body or be used to navigate or map any other regions of the body, such as moving body structures. However, each region of the body poses unique requirements to navigate, as disclosed herein. For example, the navigation system 10 addresses multiple cardiac, neurological, organ and other soft tissue therapies, including drug delivery, cell transplantation, gene delivery, electrophysiology ablations, transmyocardial vascularization (TMR), biopsy guidance, and virtual echography imaging.

[0045] The navigation system 10 may include an imaging device 12 that is used to acquire pre-operative or real-time images of a patient 14. The imaging device 12 is a fluoroscopic x-ray imaging device that may include a C-arm 16 having an x-ray source 18, an x-ray receiving section 20, an optional calibration and tracking target 22 and optional radiation sensors 24. The calibration and tracking target 22 includes calibration markers 26 (see Figures 2a-2b), further discussed herein. A C-arm controller 28 captures the x-ray images received at the receiving section 20 and stores the images for later use. The C-arm controller 28 may also control the rotation of the C-arm 16. For example, the C-arm 16 may move in the direction of arrow 30 or rotates about the long axis of the patient, allowing anterior or lateral views of the patient 14 to be imaged. Each of these movements involve rotation about a mechanical axis 32 of the C-arm 16. In this example, the long axis of the patient 14 is substantially in line with the mechanical axis 32 of the C-arm 16. This enables the C-arm 16 to be rotated relative to the patient 14, allowing images of the patient 14 to be

taken from multiple directions or about multiple planes. An example of a fluoroscopic C-arm x-ray imaging device 12 is the "Series 9600 Mobile Digital Imaging System," from OEC Medical Systems, Inc., of Salt Lake City, Utah. Other exemplary fluoroscopes include bi-plane fluoroscopic systems, ceiling fluoroscopic systems, cath-lab fluoroscopic systems, fixed C-arm fluoroscopic systems, isocentric C-arm fluoroscopic systems, 3D fluoroscopic systems, etc.

[0046] In operation, the imaging device 12 generates x-rays from the x-ray source 18 that propagate through the patient 14 and calibration and/or tracking target 22, into the x-ray receiving section 20. The receiving section 20 generates an image representing the intensities of the received x-rays. Typically, the receiving section 20 includes an image intensifier that first converts the x-rays to visible light and a charge coupled device (CCD) video camera that converts the visible light into digital images. Receiving section 20 may also be a digital device that converts x-rays directly to digital images, thus potentially avoiding distortion introduced by first converting to visible light. With this type of digital C-arm, which is generally a flat panel device, the optional calibration and/or tracking target 22 and the calibration process discussed below may be eliminated. Also, the calibration process may be eliminated or not used at all for cardiac therapies. Alternatively, the imaging device 12 may only take a single image with the calibration and tracking target 22 in place. Thereafter, the calibration and tracking target 22 may be removed from the line-of-sight of the imaging device 12.

[0047] Two dimensional fluoroscopic images taken by the imaging device 12 are captured and stored in the C-arm controller 28. Multiple two-dimensional images taken by the imaging device 12 may also be captured and assembled to provide a larger view or image of a whole region of a patient, as opposed to being directed to only a portion of a region of the patient. For example, multiple image data of a patient's leg may be appended together to provide a full view or complete set of image data of the leg that can be later used to follow contrast agent, such as Bolus tracking. These images are then forwarded from the C-arm controller 28 to a controller or work station 34 having a display 36 and a user interface 38. The work station 34 provides facilities for displaying on the display 36, saving, digitally manipulating, or printing a hard copy of the received images. The user interface 38, which may be a keyboard, mouse, touch pen, touch screen or other suitable device, allows a physician or user to provide inputs to control the imaging device 12, via the C-arm controller 28, or adjust the display settings of the display 36. The work station 34 may also direct the C-arm controller 28 to adjust the rotational axis 32 of the C-arm 16 to obtain various two-dimensional images along different planes in order to generate representative two-dimensional and three-dimensional images. When the x-ray source 18 generates the x-rays that propagate to the x-ray receiving section 20, the radiation sensors 24 sense the presence of radiation, which is forwarded to the C-

arm controller 28, to identify whether or not the imaging device 12 is actively imaging. This information is also transmitted to a coil array controller 48, further discussed herein. Alternatively, a person or physician may manually indicate when the imaging device 12 is actively imaging or this function can be built into the x-ray source 18, x-ray receiving section 20, or the control computer 28.

[0048] Fluoroscopic C-arm imaging devices 12 that do not include a digital receiving section 20 generally require the optional calibration and/or tracking target 22. This is because the raw images generated by the receiving section 20 tend to suffer from undesirable distortion caused by a number of factors, including inherent image distortion in the image intensifier and external electromagnetic fields. An empty undistorted or ideal image and an empty distorted image are shown in Figures 2a and 2b, respectively. The checkerboard shape, shown in Figure 2a, represents the ideal image 40 of the checkerboard arranged calibration markers 26. The image taken by the receiving section 20, however, can suffer from distortion, as illustrated by the distorted calibration marker image 42, shown in Figure 2b.

[0049] Intrinsic calibration, which is the process of correcting image distortion in a received image and establishing the projective transformation for that image, involves placing the calibration markers 26 in the path of the x-ray, where the calibration markers 26 are opaque or semi-opaque to the x-rays. The calibration markers 26 are rigidly arranged in pre-determined patterns in one or more planes in the path of the x-rays and are visible in the recorded images. Because the true relative position of the calibration markers 26 in the recorded images are known, the C-arm controller 28 or the work station or computer 34 is able to calculate an amount of distortion at each pixel in the image (where a pixel is a single point in the image). Accordingly, the computer or work station 34 can digitally compensate for the distortion in the image and generate a distortion-free or at least a distortion improved image 40 (see Figure 2a). A more detailed explanation of exemplary methods for performing intrinsic calibration are described in the references: B. Schuele, et al., "Correction of Image Intensifier Distortion for Three-Dimensional Reconstruction," presented at SPIE Medical Imaging, San Diego, California, 1995; G. Champeboux, et al., "Accurate Calibration of Cameras and Range Imaging Sensors: the NPBS Method," Proceedings of the IEEE International Conference on Robotics and Automation, Nice, France, May, 1992; and U.S. Patent No. 6,118,845, entitled "System And Methods For The Reduction And Elimination Of Image Artifacts In The Calibration Of X-Ray Imagers," issued September 12, 2000, the contents of which are each hereby incorporated by reference.

[0050] While the fluoroscopic imaging device 12 is shown in Figure 1, any other alternative 2D, 3D or 4D imaging modality may also be used. For example, any 2D, 3D or 4D imaging device, such as isocentric fluoroscopy, bi-plane fluoroscopy, ultrasound, computed tom-

ography (CT), multi-slice computed tomography (MSCT), magnetic resonance imaging (MRI), high frequency ultrasound (HIFU), positron emission tomography (PET), optical coherence tomography (OCT), intra-vascular ultrasound (IVUS), ultrasound, intra-operative CT or MRI may also be used to acquire 2D, 3D or 4D pre-operative or real-time images or image data of the patient 14. The images may also be obtained and displayed in two, three or four dimensions. In more advanced forms, four-dimensional surface rendering of the heart or other regions of the body may also be achieved by incorporating heart data or other soft tissue data from an atlas map or from pre-operative image data captured by MRI, CT, or echocardiography modalities. A more detailed discussion on optical coherence tomography (OCT), is set forth in U.S. Patent No. 5,740,808, issued April 21, 1998, entitled "Systems And Methods For Guiding Diagnostic Or Therapeutic Devices In Interior Tissue Regions" which is hereby incorporated by reference.

[0051] Image datasets from hybrid modalities, such as positron emission tomography (PET) combined with CT, or single photon emission computer tomography (SPECT) combined with CT, could also provide functional image data superimposed onto anatomical data to be used to confidently reach target sights within the heart or other areas of interest. It should further be noted that the fluoroscopic imaging device 12, as shown in Figure 1, provides a virtual bi-plane image using a single-head C-arm fluoroscope 12 by simply rotating the C-arm 16 about at least two planes, which could be orthogonal planes to generate two-dimensional images that can be converted to three-dimensional volumetric images. By acquiring images in more than one plane, an icon representing the location of a catheter or other instrument, introduced and advanced in the patient 14, may be superimposed in more than one view on display 36 allowing simulated bi-plane or even multi-plane views, including two and three-dimensional views.

[0052] These types of imaging modalities may provide certain distinct benefits and disadvantages for their use. For example, magnetic resonance imaging (MRI) is generally performed pre-operatively using a non-ionizing field. This type of imaging provides very good tissue visualization in three-dimensional form and also provides anatomy and functional information from the imaging. MRI imaging data is generally registered and compensated for motion correction using dynamic reference frames that are discussed herein.

[0053] Positron emission tomography (PET) imaging is generally a pre-operative imaging procedure that exposes the patient to some level of radiation to provide a 3D image. PET imaging provides functional information and also generally requires registration and motion correction using dynamic reference frames.

[0054] Computed tomography (CT) imaging is also generally a pre-operative technique that exposes the patient to a limited level of radiation. CT imaging, however, is a very fast imaging procedure. A multi-slice CT system

provides 3D images having good resolution and anatomy information. Again, CT imaging is generally registered and needs to account for motion correction, via dynamic reference frames.

5 [0055] Fluoroscopy imaging is generally an intra-operative imaging procedure that exposes the patient to certain amounts of radiation to provide either two-dimensional or rotational three-dimensional images. Fluoroscopic images generally provide good resolution and anatomy information. Fluoroscopic images can be either
10 manually or automatically registered and also need to account for motion correction using dynamic reference frames.

15 [0056] Ultrasound imaging is also generally intra-operative procedure using a non-ionizing field to provide either 2D, 3D, or 4D imaging, including anatomy and blood flow information. Ultrasound imaging provides automatic registration and does not need to account for any motion correction.

20 [0057] The navigation system 10 further includes an electromagnetic navigation or tracking system 44 that includes a transmitter coil array 46, the coil array controller 48, a navigation probe interface 50, an electromagnetic catheter 52 or any other type of instrument and a dynamic reference frame 54. It should further be noted
25 that the entire tracking system 44 or parts of the tracking system 44 may be incorporated into the imaging device 12, including the work station 34 and radiation sensors 24. Incorporating the tracking system 44 will provide an integrated imaging and tracking system. Any combination of these components may also be incorporated into
30 the imaging system 12, which again can include a fluoroscopic C-arm imaging device or any other appropriate imaging device.

35 [0058] The transmitter coil array 46 is shown attached to the receiving section 20 of the C-arm 16. However, it should be noted that the transmitter coil array 46 may also be positioned at any other location as well. For example, the transmitter coil array 46 may be positioned at
40 the x-ray source 18, within or atop the OR table 56 positioned below the patient 14, on siderails associated with the table 56, or positioned on the patient 14 in proximity to the region being navigated, such as on the patient's chest. The transmitter coil array 46 includes a plurality
45 of coils that are each operable to generate distinct electromagnetic fields into the navigation region of the patient 14, which is sometimes referred to as patient space. Representative electromagnetic systems are set forth in U.S. Patent No. 5,913,820, entitled "Position Location System," issued June 22, 1999 and U.S. Patent No. 5,592,939, entitled "Method and System for Navigating a Catheter Probe," issued January 14, 1997, each of
50 which are hereby incorporated by reference.

55 [0059] The transmitter coil array 46 is controlled or driven by the coil array controller 48. The coil array controller 48 drives each coil in the transmitter coil array 46 in a time division multiplex or a frequency division multiplex manner. In this regard, each coil may be driven sepa-

rately at a distinct time or all of the coils may be driven simultaneously with each being driven by a different frequency. Upon driving the coils in the transmitter coil array 46 with the coil array controller 48, electromagnetic fields are generated within the patient 14 in the area where the medical procedure is being performed, which is again sometimes referred to as patient space. The electromagnetic fields generated in the patient space induces currents in sensors 58 positioned in the catheter 52, further discussed herein. These induced signals from the catheter 52 are delivered to the navigation probe interface 50 and subsequently forwarded to the coil array controller 48. The navigation probe interface 50 provides all the necessary electrical isolation for the navigation system 10. The navigation probe interface 50 also includes amplifiers, filters and buffers required to directly interface with the sensors 58 in catheter 52. Alternatively, the catheter 52 may employ a wireless communications channel as opposed to being coupled directly to the navigation probe interface 50.

[0060] The catheter 52, as will be described in detail below, is equipped with at least one, and generally multiple, localization sensors 58. The catheter 54 is also generally a steerable catheter that includes a handle at a proximal end and the multiple location sensors 58 fixed to the catheter body and spaced axially from one another along the distal segment of the catheter 52. The catheter 52, as shown in Figure 1 includes four localization sensors 58. The localization sensors 58 are generally formed as electromagnetic receiver coils, such that the electromagnetic field generated by the transmitter coil array 46 induces current in the electromagnetic receiver coils or sensors 58. The catheter 52 may also be equipped with one or more sensors, which are operable to sense various physiological signals. For example, the catheter 52 may be provided with electrodes for sensing myopotentials or action potentials. An absolute pressure sensor may also be included, as well as other electrode sensors. The catheter 52 may also be provided with an open lumen, further discussed herein, to allow the delivery of a medical device or pharmaceutical/cell/gene agents. For example, the catheter 52 may be used as a guide catheter for deploying a medical lead, such as a cardiac lead for use in cardiac pacing and/or defibrillation or tissue ablation. The open lumen may alternatively be used to locally deliver pharmaceutical agents, cell, or genetic therapies.

[0061] In an alternate embodiment, the electromagnetic sources or generators may be located within the catheter 52 and one or more receiver coils may be provided externally to the patient 14 forming a receiver coil array similar to the transmitter coil array 46. In this regard, the sensor coils 58 would generate electromagnetic fields, which would be received by the receiving coils in the receiving coil array similar to the transmitter coil array 46. Other types of localization sensors or systems may also be used, which may include an emitter, which emits energy, such as light, sound, or electromagnetic radiation, and a receiver that detects the energy at a position away

from the emitter. This change in energy, from the emitter to the receiver, is used to determine the location of the receiver relative to the emitter. Other types of tracking systems include optical, acoustic, electrical field, RF and accelerometers. Accelerometers enable both dynamic sensing due to motion and static sensing due to gravity. An additional representative alternative localization and tracking system is set forth in U.S. Patent No. 5,983,126, entitled "Catheter Location System and Method," issued November 9, 1999, which is hereby incorporated by reference. Alternatively, the localization system may be a hybrid system that includes components from various systems.

[0062] The dynamic reference frame 54 of the electromagnetic tracking system 44 is also coupled to the navigation probe interface 50 to forward the information to the coil array controller 48. The dynamic reference frame 54 is a small magnetic field detector that is designed to be fixed to the patient 14 adjacent to the region being navigated so that any movement of the patient 14 is detected as relative motion between the transmitter coil array 46 and the dynamic reference frame 54. This relative motion is forwarded to the coil array controller 48, which updates registration correlation and maintains accurate navigation, further discussed herein. The dynamic reference frame 54 can be configured as a pair of orthogonally oriented coils, each having the same center or may be configured in any other non-coaxial coil configuration. The dynamic reference frame 54 may be affixed externally to the patient 14, adjacent to the region of navigation, such as on the patient's chest, as shown in Figure 1 or on the patient's back. The dynamic reference frame 54 can be affixed to the patient's skin, by way of a stick-on adhesive patch. The dynamic reference frame 54 may also be removably attachable to fiducial markers 60 also positioned on the patient's body and further discussed herein.

[0063] Alternatively, the dynamic reference frame 54 may be internally attached, for example, to the wall of the patient's heart or other soft tissue using a temporary lead that is attached directly to the heart. This provides increased accuracy since this lead will track the regional motion of the heart. Gating, as further discussed herein, will also increase the navigational accuracy of the system 10. An exemplary dynamic reference frame 54 and fiducial marker 60, is set forth in U.S. Patent No. 6,381,485, entitled "Registration of Human Anatomy Integrated for Electromagnetic Localization," issued April 30, 2002, which is hereby incorporated by reference. It should further be noted that multiple dynamic reference frames 54 may also be employed. For example, an external dynamic reference frame 54 may be attached to the chest of the patient 14, as well as to the back of the patient 14. Since certain regions of the body may move more than others due to motions of the heart or the respiratory system, each dynamic reference frame 54 may be appropriately weighted to increase accuracy even further. In this regard, the dynamic reference frame 54 attached to the

back may be weighted higher than the dynamic reference frame 54 attached to the chest, since the dynamic reference frame 54 attached to the back is relatively static in motion.

[0064] The catheter and navigation system 10 further includes a gating device or an ECG or electrocardiogram 62, which is attached to the patient 14, via skin electrodes 64, and in communication with the coil array controller 48. Respiration and cardiac motion can cause movement of cardiac structures relative to the catheter 54, even when the catheter 54 has not been moved. Therefore, localization data may be acquired on a time-gated basis triggered by a physiological signal. For example, the ECG or EGM signal may be acquired from the skin electrodes 64 or from a sensing electrode included on the catheter 54 or from a separate reference probe. A characteristic of this signal, such as an R-wave peak or P-wave peak associated with ventricular or atrial depolarization, respectively, may be used as a triggering event for the coil array controller 48 to drive the coils in the transmitter coil array 46. This triggering event may also be used to gate or trigger image acquisition during the imaging phase with the imaging device 12. By time-gating or event gating at a point in a cycle the image data and/or the navigation data, the icon of the location of the catheter 52 relative to the heart at the same point in the cardiac cycle may be displayed on the display 36, further discussed herein.

[0065] Additionally or alternatively, a sensor regarding respiration may be used to trigger data collection at the same point in the respiration cycle. Additional external sensors can also be coupled to the navigation system 10. These could include a capnographic sensor that monitors exhaled CO₂ concentration. From this, the end expiration point can be easily determined. The respiration, both ventilated and spontaneous causes an undesirable elevation or reduction (respectively) in the baseline pressure signal. By measuring systolic and diastolic pressures at the end expiration point, the coupling of respiration noise is minimized. As an alternative to the CO₂ sensor, an airway pressure sensor can be used to determine end expiration.

[0066] Briefly, the navigation system 10 operates as follows. The navigation system 10 creates a translation map between all points in the radiological image generated from the imaging device 12 and the corresponding points in the patient's anatomy in patient space. After this map is established, whenever a tracked instrument, such as the catheter 52 or pointing device is used, the workstation 34 in combination with the coil array controller 48 and the C-arm controller 28 uses the translation map to identify the corresponding point on the pre-acquired image, which is displayed on display 36. This identification is known as navigation or localization. An icon representing the localized point or instruments are shown on the display 36 within several two-dimensional image planes, as well as on three and four dimensional images and models.

[0067] To enable navigation, the navigation system 10

must be able to detect both the position of the patient's anatomy and the position of the catheter 52 or other surgical instrument. Knowing the location of these two items allows the navigation system 10 to compute and display the position of the catheter 52 in relation to the patient 14. The tracking system 44 is employed to track the catheter 52 and the anatomy simultaneously.

[0068] The tracking system 44 essentially works by positioning the transmitter coil array 46 adjacent to the patient space to generate a low-energy magnetic field generally referred to as a navigation field. Because every point in the navigation field or patient space is associated with a unique field strength, the electromagnetic tracking system 44 can determine the position of the catheter 52 by measuring the field strength at the sensor 58 location. The dynamic reference frame 54 is fixed to the patient 14 to identify the location of the patient in the navigation field. The electromagnetic tracking system 44 continuously recomputes the relative position of the dynamic reference frame 54 and the catheter 52 during localization and relates this spatial information to patient registration data to enable image guidance of the catheter 52 within the patient 14.

[0069] Patient registration is the process of determining how to correlate the position of the instrument or catheter 52 on the patient 14 to the position on the diagnostic or pre-acquired images. To register the patient 14, the physician or user may use point registration by selecting and storing particular points from the pre-acquired images and then touching the corresponding points on the patient's anatomy with a pointer probe 66. The navigation system 10 analyzes the relationship between the two sets of points that are selected and computes a match, which correlates every point in the image data with its corresponding point on the patient's anatomy or the patient space. The points that are selected to perform registration are the fiducial arrays or landmarks 60. Again, the landmarks or fiducial points 60 are identifiable on the images and identifiable and accessible on the patient 14. The landmarks 60 can be artificial landmarks 60 that are positioned on the patient 14 or anatomical landmarks that can be easily identified in the image data. The system 10 may also perform registration using anatomic surface information or path information, further discussed herein. The system 10 may also perform. 2D to 3D registration by utilizing the acquired 2D images to register 3D volume images by use of contour algorithms, point algorithms or density comparison algorithms, as is known in the art. An exemplary 2D to 3D registration procedure, as set forth in U.S. Serial No. 60/465,615, entitled "Method and Apparatus for Performing 2D to 3D Registration" filed on April 25, 2003, which is hereby incorporated by reference. The registration process may also be synched to an anatomical function, for example, by the use of the ECG device 62, further discussed herein.

[0070] In order to maintain registration accuracy, the navigation system 10 continuously tracks the position of the patient 14 during registration and navigation. This is

because the patient 14, dynamic reference frame 54, and transmitter coil array 46 may all move during the procedure, even when this movement is not desired. Therefore, if the navigation system 10 did not track the position of the patient 14 or area of the anatomy, any patient movement after image acquisition would result in inaccurate navigation within that image. The dynamic reference frame 54 allows the electromagnetic tracking device 44 to register and track the anatomy. Because the dynamic reference frame 54 is rigidly fixed to the patient 14, any movement of the anatomy or the transmitter coil array 46 is detected as the relative motion between the transmitter coil array 46 and the dynamic reference frame 54. This relative motion is communicated to the coil array controller 48, via the navigation probe interface 50, which updates the registration correlation to thereby maintain accurate navigation.

[0071] Turning now to Figure 3, a logic flow diagram illustrating an exemplary operation of the navigation system 10 is set forth in further detail. First, should the imaging device 12 or the fluoroscopic C-arm imager 12 not include a digital receiving section 20, the imaging device 12 is first calibrated using the calibration process 68. The calibration process 68 begins at block 70 by generating an x-ray by the x-ray source 18, which is received by the x-ray receiving section 20. The x-ray image 70 is then captured or imported at import block 72 from the C-arm controller 28 to the work station 34. The work station 34 performs intrinsic calibration at calibration block 74, as discussed above, utilizing the calibration markers 26, shown in Figures 2a and 2b. This results in an empty image being calibrated at block 76. This calibrated empty image is utilized for subsequent calibration and registration, further discussed herein.

[0072] Once the imaging device 12 has been calibrated, the patient 14 is positioned within the C-arm 16 between the x-ray source 18 and the x-ray receiving section 20. The navigation process begins at decision block 78 where it is determined whether or not an x-ray image of the patient 14 has been taken. If the x-ray image has not been taken, the process proceeds to block 80 where the x-ray image is generated at the x-ray source 18 and received at the x-ray receiving section 20. When the x-ray source 18 is generating x-rays, the radiation sensors 24 identified in block 82 activate to identify that the x-ray image 80 is being taken. This enables the tracking system 44 to identify where the C-arm 16 is located relative to the patient 14 when the image data is being captured.

[0073] The process then proceeds to decision block 84 where it is determined if the x-ray image acquisition will be gated to physiological activity of the patient 14. If so, the image device 12 will capture the x-ray image at this desired gating time. For example, the physiological change may be the beating heart, which is identified by ECG gating at block 86. The ECG gating enables the x-ray image acquisition to take place at the end of diastole at block 88 or at any other cycle. Diastole is the period of time between contractions of the atria or the ventricles

during which blood enters the relaxed chambers from systemic circulation and the lungs. Diastole is often measured as the blood pressure at the instant of maximum cardiac relaxation. ECG gating of myocardial injections also enables optimal injection volumes and injection rates to achieve maximum cell retention. The optimal injection time period may go over one heart cycle. During the injection, relative motion of the catheter tip to the endocardial surface needs to be minimized. Conductivity electrodes at the catheter tip may be used to maintain this minimized motion. Also, gating the delivery of volumes can be used to increase or decrease the volume delivered over time (i.e., ramp-up or ramp-down during cycle). Again, the image may be gated to any physiological change like the heartbeat, respiratory functions, etc. The image acquired at block 88 is then imported to the work station 34 at block 90. If it is not desired to physiologically gate the image acquisition cycle, the process will proceed from the x-ray image block 80 directly to the image import block 90.

[0074] Once the image is received and stored in the work station 34, the process proceeds to calibration and registration at block 92. First, at decision block 94, it is determined whether the imaging device 12 has been calibrated, if so, the empty image calibration information from block 76 is provided for calibration registration at block 92. The empty image calibration information from block 76 is used to correct image distortion by establishing projective transformations using known calibration marker locations (see Figures 2a and 2b). Calibration registration 92 also requires tracking of the dynamic reference frame 54. In this regard, it is first determined at decision block 96 whether or not the dynamic reference frame is visible, via block 98. With the dynamic reference frame 54 visible or in the navigation field and the calibration information provided, the work station 34 and the coil array controller 48, via the navigation probe interface 50 performs the calibration registration 92 functions. In addition to monitoring the dynamic reference frame 54, the fiducial array or landmarks 60 may also be used for image registration.

[0075] Once the navigation system 10 has been calibrated and registered, navigation of an instrument, such as the catheter 52 is performed. In this regard, once it is determined at decision block 100 that the catheter 54 is visible or in the navigation field at block 102, an icon representing the catheter 52 is superimposed over the pre-acquired images at block 104. Should it be determined to match the superimposed image of the catheter 52 with the motion of the heart at decision block 106, ECG gating at block 108 is performed. The catheter 52 may then be navigated, via navigation block 110 throughout the anatomical area of interest in the patient 14.

[0076] Turning to Figures 4-5, an exemplary catheter 52 is shown in further detail. The exemplary catheter, as shown in Figure 4a, includes an external flexible body 112 and a proximal handle 114. Positioned within the catheter 52 are the four sensing coils 58 disposed distally

in the catheter 52. The localization or sensing coils 58 are multi-layer and multi-turn coils, which are coupled to four sets of twisted pair conductors 116. The catheter 52 further includes a pull wire 118, which is used to control and guide the distal tip 120 of the catheter 52. Extending through the catheter 52 is a central lumen 122 that can be used to deliver and transport cells or drug therapy and leads for cardiac pacemakers. The central lumen 122, shown in Figure 4b retains a hypodermic needle 124 that can be used as the delivery instrument. The catheter 52 further includes electrode conductors 126 and an electrode tip ring 128 used to sense various electrical signals from the heart. Other sensors that can be attached to the catheter 52 include multiple electrode sensors, absolute pressure sensors, accelerometers and oxygen saturation sensors. For mapping catheters 52, micro-motion arrays, further discussed herein, may also be embedded to electronically control curvature of the catheter 52 to provide a semi-automated mapping procedure.

[0077] Turning to Figure 5, the axial cross-section of the catheter 52 is shown in further detail. The catheter 52 is again formed from the outer cover 112 that is formed from an extruded polymer having six directional splines 130. An internal extrusion 132 defines six chambers or lumens 134 between the internal extrusion 132 and external extrusion 112. Within four of the chambers 134 are the four twisted pair conductors 116, which are coupled to each of the coils or sensors 58. Located in another chamber 132 are the electrode conductors 126. The pull wire 118 is located in the remaining chamber 132. By adjusting the pull wire 118 along with the torque transferring splines 130, the directional catheter 52 can be positioned and steered as desired. Also, located within the center of the catheter 52 is the lumen 122 housing the hypodermic needle 124 having a central port 136 for passing cells, catheter leads and other items. Further details of the catheter 52, as well as other embodiments of the catheter 52 are set forth in U.S. Serial No. 10/299,484, entitled "Multi-Lumen Body for Medical Catheter and Leads," naming as inventors Kenneth Gardeski, Michael Leners and Jesus Casas-Bejar, filed November 19, 2002, which is hereby incorporated by reference. Again, the catheter 52 may include a lumen 122 open on both ends, which allows it to be used to deliver several cardiac therapies (e.g., to implant pacing leads, deliver drugs, to transplant cells into the myocardium, or to perform complex electrophysiological procedures, including ablation).

[0078] The navigation system 10 enhances minimally invasive cardiac therapies by making the procedure more intuitive. The catheter 52 can be used to implant pacing leads, perform cell transplantation, deliver drugs or perform ablations. The catheter 52 having navigation guidance, via sensors 58 provides enhanced outcomes by making lead placement more successful in difficult anatomies, by insuring cells are transplanted in the most viable myocardium within the infarct, etc. Moreover, use of the electrocardiogram device 62 enables further gating

of the drug deliver and cell delivery at the most optimum times for providing additional capabilities to the navigation system 10. The navigation system 10 can also be applied to non-cardiac therapies, such as neuro-vascular catheters, or oncology drug delivery applications, based on combined PET/CT (functional and anatomical) pre-operative data or pre-operative data from any other bio-imaging system for tumor identification and location. The navigation system 10 can also map on the display 36 the delivery of cell or drug therapy or other therapies that are annotated on 2D, 3D or 4D images or graphic displays. The navigation system 10 may also generate distribution maps on how the cell or drug delivery or other therapies are disbursed through the region of interest, such as the heart. These iso-contours or iso-dose contours display how therapy is disbursed through the tissue. For example, a bullseye type graphic may be displayed on the three-dimensional heart model with different concentric rings having different colors identifying the amount of drug therapy delivered to the noted regions.

[0079] The navigation system 10 can also be used and employed in several types of medical procedures and has several improvements and advantages over existing systems. The navigation system 10 provides application and methods for electromagnetic non-line-of-site navigation for catheter delivery of pacing leads. The navigation system 10 includes heuristics that are integrated into the software of the work station 34 to provide an algorithm for locating the coronary sinus, further discussed herein. The navigation system 10 provides for gating or timing of injections for cell transplantation in the infarcted myocardium as a substitute for anchoring. The cell delivery imaging modality is generally utilized as real-time MR. Real time MR allows catheter navigation while visualizing the infarcted region of the heart. Use of pre-operative perfusion MR images may also be used to clearly identify the infarct region, along with the quality of the infarct. The navigation system 10 also includes integrated programming functions in the work station 34 that are used to help identify optimum pacing sites, further discussed herein. Also, the navigation system 10 provides a simulated bi-plane or multi-plane fluoroscopy for cardiac applications with one-head systems and also catheter registration to the images, whether fluoroscopic or volume-rendered using MR, CT, and moving surfaces.

[0080] Turning now to Figure 6, an exemplary lead implant procedure 138 is shown in detail. While this procedure is described regarding implanting a lead for a pacemaker, it should again be noted that this process can be applied to any type of cardiac therapy as discussed herein, such as angioplasty, stenting, and ablation. The lead placement procedure disclosed herein is designed to reduce the procedure time and reduce the procedure costs and enable a physician to implant a lead quicker, safer and in a more precise optimized location. Delivery catheters 52 are, therefore, very important with cardiac resynchronization therapy. The catheter 52 and fluoroscopic images are used to find and cannulate the coro-

nary sinus. Once cannulated, a lead is delivered through the catheter 52 and into the cardiac veins.

[0081] Various types of catheters 52 may be utilized to deliver a lead to the desired cardiac location, via the central port 136 in the hypodermic needle 124. The catheter 52 may include the catheter electrode 128, which could be used to monitor the intra-cardiac electrical signals. Since each region in the heart has characteristic differences, these differences can be used to distinguish which region the catheter tip 120 is placed within the heart. In addition to monitoring intra-cardiac electrical signals, electrical impedance (high and low frequency) may also be monitored, via the electrode 128. This could be monitored continuously to highlight the cardiac impedance cycle. In this regard, it is believed that each region within the heart has a unique cardiac impedance and will have distinct characteristics. The cardiac impedance would, therefore, provide more information to be correlated with the sensors 58 and the catheter 52 in determining the location of the lead tip and can act as an anatomical landmark. The impedance signal could also be used to help determine if the lead is floating or lodged against the heart tissue.

[0082] Another type of sensor, which can be placed at the tip of the catheter 52 is an absolute pressure sensor, which can monitor hemo-dynamics. The intra-cardial pressure signal is an important signal in diagnostics and critical care monitoring. As a consequence, the characteristics of the pressure signal are well characterized for each region of the heart. For normal hearts, each region is distinctly characteristic with the sharp transitions between the upper and lower chambers of the heart. Taken with the electrode sensors 58 information, the location of the catheter tip 120 can be determined with a further high degree of confidence. These transition regions between the chambers of the heart could also be used as registration data points for 3-D heart models, further discussed herein.

[0083] The fluoro-enhanced implant procedure provides the physician with real-time location information of the catheter 52. An icon representing the catheter 52 is superimposed on the background of a 3-D heart model or atlas model. The electrode and/or pressure sensor information discussed above is used to correctly locate the catheter position within this heart model. In this regard, very specific locations can be searched out to provide reference points within the heart to fit the model space. The transition between regions of the heart are easily identified through changes in the morphology of the electrode and pressure signals. The transition regions are very sharp, making these regions excellent reference points or landmarks for the heart model. The possible reference points include the superior vena cava (SVC) to right atria transition, the tricuspid valve, and the left ventricular apex. As these reference points are located, the heart model is shrunk or stretched and rotated to match these reference points. Normally, the navigation system 10 will automatically locate the reference points

by monitoring the electrode and pressure sensors. This results in a visualization of the catheter 52 as it is moved through the heart model. Once the 3-D heart model placement is established, a mapping function can begin or a lead implant site chosen. The 3-D heart model will be scaled and rotated only within physiological bounds. Reference points outside of these bounds will generate an alert and require the physician to resolve the discrepancy.

[0084] An exemplary lead implant method or procedure 138 for identifying a lead implant site is illustrated in Figure 6. The procedure 138 includes a landmark identification process 140 that includes a number of steps at block 142, which depends on the number of landmarks needed or recognizable for a particular application. Included in this process 140 is catheter navigation, via block 144, which provides position and orientation information that is measured in real time, via the sensors 58 within catheter 52. As the catheter 52 is navigated, as set forth in block 144, additional data is gathered within the heart, via sensors positioned on the catheter 52 at block 146. As discussed, this additional data can include pressure, temperature, oxygen, impedance and electrophysiological information. By monitoring this additional data at block 146, landmarks or reference points within the heart can be identified and marked on the catheter fluoroscopic images at block 148. The process of collecting the landmarks can be a manual or automatic process by identifying the physical landmarks within the fluoroscopic image, based upon the received data from block 146, that identify distinct points or regions within the heart.

[0085] Once the multiple landmarks or reference points are identified in the heart, a 3-D heart model or atlas heart model is superimposed over the fluoroscopic images or modeled as a 3-D volume view by registering or translating the 3-D heart model in relation to the landmarks collected at block 148. This fusion occurs at block 150, which translates, rotates and scales the 3-D heart model, based upon the collected landmarks to provide a patient specific heart model that can be used for various procedures. Again, the heart model can be generated from an atlas model, as set forth in block 152 or it may be generated from an actual physiological image, such as from an MRI or a CT. Once the 3-D model has been scaled and registered to the landmarks, the controller or work station 34 provides navigation and road map information to direct the catheter 52 through the heart to a suggested or estimated optimized target site for lead placement at block 154. This target site can be identified on the 3-D model along with a real time view of an icon representing the catheter 52 moving toward the suggested target site. In this regard, the physician would know where the target is on the 3-D map or display 36 and can simply navigate the catheter 52 toward this target. The target site can be based on statistical maps that can suggest where lead placement should take place, depending on the pathology of the patient.

[0086] In addition to identifying a potential target site for lead placement, the navigation system 10 can also suggest sites for drug or cell delivery. Alternatively, the catheter 52 can be used as a mapping catheter 52. The position sensors 58 provide real time feedback on the catheter location in 3-D space, which is a requirement for accurate mapping. The mapping procedure is essentially an extension of the fluoro-enhanced implant approach, set forth in Figure 6. The mapping catheter 52 will be optimized for mapping and/or to implant, but the basic procedure remains the same.

[0087] Essentially, the 3-D heart model is calibrated using the same technique as shown in Figure 6, and the correctly scaled heart model becomes the basis for the initial mapping grid. With a micro-motion catheter, further discussed herein, the catheter is positioned at each mapping site in a semi-autonomous fashion with user intervention as needed. For catheters without micro-motion, the system would highlight on the display 36, the next mapping point, along with the actual catheter position. The user or physician would then manually manipulate or steer the catheter tip 120 to the identified location. Alternatively, the physician or user may choose each location and initiates a mapping measurement for that point. With a single electrode catheter 52, the intrinsic electrical amplitude, pacing threshold, and wall motion (contractility) can be measured. As the mapping progresses, a 3-D diagnostic map of the measured parameters are displayed alongside the 3-D model display. This method of mapping provides the capability of highlighting and detailing a number of heart defects, such as chronic infarct, chronic ischemia, perfusion defect, or aneurism. If a mapping or EP catheter 52 with multiple electrodes is used, such as electrode 128, this mapping system can generate and display inter-cardiac electrical activity and timing, along with exact catheter tip and electrode location in real time. The result is a 3-D electro-anatomical map reconstruction. The applications for this system includes mapping of ventricular and supra-ventricular arrhythmias, mapping of myocardial potential and conduction velocity, and depolarization mapping. Using multiple position sensors 58, with each sensor 58 associated with an electrode on the catheter 52, the navigation system 10 can be used to accurately measure the location of each electrode measurement providing improved mapping accuracy.

[0088] In addition to using a guide wire 118 to adjust or steer the catheter 52, micro-motion technology may also be used to precisely steer the catheter in an automated manner. In this regard, selective heating of a shaped memory metal enables and provides the ability to steer the catheter 52 or lead to a precise location. The micro-motion technology applies a VLSI film to a piece of shape memory metal to form an actuator. The VLSI film has a pattern of resistors in the range of 100-300 ohms. The film is attached to the metal and the electrode connections made to the computer controller, such as the work station 34. A small amount of current is applied

to one or multiple resistors, which generates a localized heating of the metal. This provides precise steering to a specific location within the heart. Also, a semi-automated mapping procedure can then take place to construct the electro-anatomical maps. In this regard, the micro-motion actuator is used to manipulate the catheter 52 to a desired set of mapping points automatically. With the addition of position sensors 58, real time feedback of the catheter curvature provides improved steering capabilities. Should it be desired, strain gages may also be applied to the actuator to provide additional real time feedback of the curved position. For example, micro-motion technology is available from Micro-Motion Sciences, which provides a controllable and steerable catheter, via the selective heating of a shaped memory metal that passes through the catheter 52. Micro-electron mechanical sensor (MEMS) technology, as well as nano technology may also be utilized for controlling the manipulation and steering of the catheter 52.

[0089] Again, fluoro pre-imaging of the patient is initially completed using the imaging system 12. Once completed, the navigation system 10 utilizes a three-dimensional volume rendered or wire frame model of the heart or other soft tissue that is registered to the patient 14. The heart model is scalable, morphed or registered using 2-D and 3-D image techniques to match the fluoro images and measured reference points are determined from the transitional signals on the electrical and pressure sensors associated with the catheter 52. The navigation system 10 then displays the three-dimensional heart model on the display 36. An icon of the catheter 52 is simultaneously displayed in correct relation to the model and fluoro images. As the session begins, the model is positioned based on the known placement of the dynamic reference frame 54 and the fluoro images captured by the imager 12. Once the catheter 52 is in range, it is displayed on the display 36 relative to the rendered heart model. Simultaneously, multiple views of the catheter 52 and heart model are available on the display 36 to aid in visualizing the catheter shape and position within the heart.

[0090] During the initial model scaling, the electrical and pressure signals are continuously monitored and displayed. At the transition from the superior vena cava to the right atrium, the electrical and pressure signal morphology changes. This transition is noted by the navigation system 10, along with the catheter position at the time of the transition. This position represents a reference point for the heart model. The heart model is then repositioned to match this reference point. The physician is given full control over this process. If necessary, the physician can manually set any of the heart model reference points. This is accomplished by manually placing the catheter 52 at the desired reference position and selecting the appropriate model reference point. This same process is repeated as the catheter 52 passes the tricuspid valve and into the right ventricle. This transition point marks an additional reference point for the model. At these reference positions, the model is stretched, rotat-

ed, and aligned to match the reference locations. A third reference point is the left ventricular apex. At this point, the physician should be able to easily manipulate the catheter 52 into the apex or mark this as a reference point.

[0091] At this point, the navigation system 10 displays a very accurate visual representation of the catheter placement within the heart model. The visual feedback allows the position and orientation of the catheter 52 to be manipulated with a high degree of confidence and accuracy. The 3-D model includes statistical atlas information that can be provided to the physician for improved outcome. The potential implant sites can be tested for good electrical characteristics and optimal sites selected. The catheter 52 is then used to guide the lead to the chosen site. A final fluoroscopic image can then be taken to assess excessive lead motion and lead tension.

[0092] It should also be noted that as long as the dynamic reference frame 54 is not moved, the catheter 52 can be re-introduced without needing to rescale the 3-D heart model. The calibration of the heart model is maintained. In this same way, a secondary catheter could be introduced with no loss and accuracy. Once the 3-D heart model is scaled and positioned, it remains accurate throughout the procedure.

[0093] Referring to Figure 7, an exemplary image 156 that is displayed on display 36 is illustrated. In the image 156, an icon 157 representing the position and location of the catheter 52 is shown navigating through the superior vena cava. In order to provide a road map to guide or suggest a possible path for the catheter 52, a target 158 may be illustrated and superimposed onto the pre-acquired image, as shown at reference numeral 158. At this specific landmark 158, data can either be manually or automatically downloaded from other sources, such as the catheter, lead, or pacemaker programmer to create a hyperlink with this virtual annotated landmark 158. By a simple mouse click (red arrow 160), all available data could be displayed by a pop-up window 162. This data includes information, such as temperature, pressure, oxygen level, or electro-physiological signals, as shown in windows 162. As such, a user or physician would simply refer to the virtual annotated landmarks 158 in the particular view and click on that landmark 158 to obtain the physiological information at that particular site. The catheter 52 will thus gather, store, and download data on patient morphology, electrical thresholds and other implant parameters that can be stored for later review.

[0094] The catheter 52 may also optionally be fitted with a fiberoptic imaging sensor. Fiberoptic imaging technology is available, for example, from Cardio Optics of Boulder, Colorado, which enables a catheter to view the heart and heart structures continuously through blood. This enables the physician or user to have an additional view of what is in front of the catheter 52, which can be displayed on display 36.

[0095] Turning to Figure 8, an additional exemplary image 164 that is displayed on display 36 is illustrated.

The image 164 includes an icon 166, representing the position and location of the catheter 52. The icon 166 has an enlarged probe diameter as compared to the icon 157, shown in Figure 7. This probe diameter of the icon 166 representing the catheter 52 is adjusted by way of probe diameter adjustment switches 168. By pressing the "+" button of the probe diameter switches 168, the probe diameter increases. Conversely, by pressing the "-" button, the probe diameter decreases. This enables the surgeon to adjust the probe diameter to a desired size providing further or enhanced visualization of the surgical procedure.

[0096] Referring now to Figure 9, an exemplary image 170 that is displayed on display 36 is illustrated. The image 170 includes an icon 172 representing the location and position of the catheter 52. The icon 172 further includes a straight projection portion 174 that projects straight along the direction of the first sensor 58 within the catheter 52. This straight projection 174 represents a straight projected trajectory of the catheter 52. The length of the projected icon portion 174 may be adjusted via projected length switches 176. Here again, the "+" button lengthens the straight projected icon 174, while the "-" button shortens the projected length of the icon 174. This estimated straight trajectory enables the surgeon to determine where the catheter 52 is traveling and how far or how much travel is necessary to reach a desired target along a straight path.

[0097] Turning now to Figure 10, an exemplary image 178 that is displayed on display 36 is illustrated. The image 178 includes an icon 180 representing the position and location of the catheter 52. The image 178 further includes a spline or curved projection 182, which is based upon the shape of the curved catheter 52, shown as icon 180. Here again, the projected length of the spline projection 182 is controlled by way of the projected length switches 176. This estimated curve projection enables the surgeon to determine where the catheter 52 will travel if the catheter 52 continues along its curved trajectory, further providing enhanced features for the surgeon navigating the catheter 52. The estimated curve is determined by use of known curve fitting algorithms that are adjustable based upon the type of catheter used and based upon the flexibility and material of the catheter 52. This enables estimated curved trajectories of the catheter 52 to be displayed to assist the user.

[0098] Referring now to Figure 11, an exemplary method or procedure 184 for navigating the catheter 52 to the coronary sinus region of the heart is illustrated. The procedure 184 begins at block 186, where the catheter navigation system 10 is set up. This set up includes connecting all of the appropriate hardware within the navigation system 10, as well as activating the various computers within the system 10. Once the navigation system 10 is set up at block 186, the procedure 184 proceeds to acquire an empty image at block 188. The acquisition of the empty image of the block 188 is similar to the calibration process 68, shown in Figure 3. In this regard, an

x-ray is taken by the imaging device 12 where intrinsic calibration is performed on this empty image to calibrate the imaging device 12. Radiation sensor 24 senses when the x-ray process has taken place at block 190. The resulting empty x-ray image is shown on display 36 and illustrated at block 192, which illustrates the calibration and tracking target 22. Again, the calibration process is an optional process depending on the medical procedure conducted or depending on the type of imaging system 12.

[0099] Once the navigation system 10 has been calibrated, the patient 14 is positioned within the imaging device 12 to capture various views of the patient 14. At block 194, an anterior/posterior anatomic image of the patient 14 is acquired by the imaging device 12. The image acquisition at block 194 may be gated via block 196 using the ECG 52 to trigger when the acquisition of the anterior/posterior image is acquired. The image acquisition may also be gated by any other physiological event. The anterior/posterior anatomic image of the coronary sinus region is shown at display 198. Once the anterior/posterior image is acquired at block 194, the lateral anatomic image of the patient 14 is acquired at block 200. Again, this image acquisition at block 200 may be gated, via block 196. The lateral image is shown in display block 202.

[0100] Once the anterior/posterior anatomic image is acquired at block 194 and the lateral anatomic image is acquired at block 200, the procedure 184 proceeds to block 204 where the acquired images are activated. In this regard, each image is displayed on display 36 as is shown in blocks 198 and 202. Once the images have been activated at block 204, the procedure proceeds to block 206, where the catheter 52 is navigated to the coronary sinus. To assist in this navigation of the catheter 52, atlas, template and additional information, via block 208 may be provided. The atlas information may include registering a three-dimensional atlas heart model, as shown in Figure 12, similar to the way discussed in Figure 6, to assist in navigating the catheter 52 to the coronary sinus. Templates may also be superimposed over the images 198 and 202 or over the three-dimensional heart model to provide a map for steering and guiding the catheter 52 through the coronary sinus region. The additional information provided at block 208 can also include an algorithm that is designed to direct the surgeon through various steps suggesting or estimating where the surgeon should be looking to guide the catheter 52 through the coronary sinus region. These steps may include providing various guide points within the template that identify on the display 36 where the catheter 52 should be navigated. As the catheter 52 reaches a particular suggested guide point, the system 10 can then prompt the surgeon to then go to the next guide point, thereby providing a roadmap to the surgeon through the coronary sinus region. The algorithm for locating the coronary sinus can increase the accuracy of pacing lead placement significantly, thereby providing reduced surgical time and

increased accuracy and efficiency.

[0101] Referring to Figure 12, an image 210 illustrating a three-dimensional atlas heart model 212 is illustrated. In the image 210, an icon 214 of the catheter 52 is illustrated passing through the heart model 212 to a cell delivery region 216. The region 216 can be highlighted on the heart model 212 to guide the surgeon to a particular region of the heart and, in this example, for cell delivery therapy. Again, the heart model 212 can also be used for any other cardiac procedure to assist the surgeon during pacing lead placement, ablation, stenting, etc.

[0102] Turning now to Figure 13, another exemplary method 220 for navigating a pacemaker lead placement in the heart using a catheter 52 or other instrument is illustrated. The method or procedure 220 is directed to performing image guided coronary sinus cannulation or any other procedure using the navigation catheter 52 or any other instrument in order to position the left heart lead at an optimal site. The navigation system 10 employs the navigation catheter 52 or any other instrument, such as insert or guide wire that carries one or more of the localization sensors 58, to provide information to the user, via display 36. The method 220 begins at block 222 where the particular organ or region of interest is identified. Any organ or soft tissue or region of the patient may be navigated using this disclosed method or procedure. As an exemplary procedure, the coronary sinus region of the heart will be described in further detail.

[0103] Once the organ or the heart has been identified, external or internal fiducial markers 60 may be placed on the heart at block 221. Alternatively, any type of anatomical landmark may also be used as the fiducial marker. Still further, contours or paths within the navigated organ may also be used as fiducial markers for the registration process. The procedure then proceeds to block 224 where image acquisition on this region of the patient is conducted. Again, the image acquisition can be from any type of imaging device and can be performed pre-operatively or intra-operatively using a fluoroscope 12, shown in Figure 1 or any other imaging devices, such as an ultrasound, MRI, CT, etc. The image acquisition process 224 may also be gated, via block 226 to a particular anatomical function. For example, ECG gating using the ECG 62 device may be utilized during the image acquisition 224 to insure that the image is captured or image data is used at a particular sequencing point, via ECG gating 226. In other words, the image may be captured at a particular point or time in a cycle or alternatively if real-time image data is captured over time, image data at a particular point along the time frame may be used, via ECG gating 226. By providing ECG gating 226, the navigation system 10 is able to track the instrument or catheter 52 that is synchronized with the pre-acquired images. In other words, this enables synchronization of the pre-acquired image with the instrument during navigation so that the virtual representation of the instrument or catheter 52 is aligned with the pre-acquired image.

[0104] Again, it should be noted that image acquisition

process 224 may be gated at block 226 to capture a specific image at a specific time or alternatively, the image data can be a streaming image data continuously captured and the gating 226 may be used to capture image data at a specific time or frame of the already captured image data in order to track the catheter 52. The ECG gating technique 226 also may include gating from any other physiological activity, which is directly or indirectly sensed, via the catheter 52 or other external sensors not associated with the catheter 52. Other types of physiological parameters or activities that can be sensed or used during gating block 226 include blood flow, electrophysiological, respiratory, cardiac, oxygen sensing, CO₂ sensing, etc.

[0105] Any soft tissue navigation can benefit from gating or synchronizing to an anatomical function, such as the heartbeat, respiratory, etc., as previously discussed. For example, referring to Figures 14a and 14b, a pre-acquired fluoroscopic image of the heart is illustrated with a virtual representation of the catheter 52. As shown in Figure 14a, the fluoroscopic image of the heart acquired with a real catheter is identified as reference numeral 228. The virtual representation of the navigating catheter 52, is shown as reference numeral 230. The superimposed catheter 230 does not match catheter 228 because it is not synched with the originally captured image 228. In other words, when the pre-acquired image 228 was captured, it was arbitrarily captured and not gated to a specific physiological event. Therefore, when the superimposed catheter 230 was localized to the pre-acquired images, it resulted in a mismatched or unsynched image. In contrast, referring to Figure 14b, using the ECG gating technique 226, since the navigation system 10 knows when the image 228 had been acquired in the particular heartbeat cycle, it is possible to sync the superimposed or virtual representation of the instrument 232 with the image 228 to generate a good match.

[0106] Returning to Figure 13, at block 234, one or multiple dynamic reference frames 54 are affixed to the patient 14, either internally, via a lead or externally, with an adhesive patch on the skin. The dynamic reference frames 54 may also include fiducial markers 60, as previously discussed and used for the registration process.

[0107] Images of the navigated organ, such as the heart 222, are acquired at block 224 during the procedure 220. Each of the images acquired at block 224 is registered to the patient at block 236, either manually using fluoroscopy, ultrasound, or other known techniques by using fiducial markers 60 that can be located on the pre-acquired images. Alternatively, if the fiducial markers 60 contain EM position sensors then automatic registration is possible. An exemplary sensor that includes both a dynamic reference frame and a fiducial marker, is set forth in U.S. Patent No. 6,381,485, entitled "Registration of Human Anatomy Integrated for Electromagnetic Localization", issued April 30, 2002, where is hereby incorporated by reference. In a case of pre-operative or intra-operative imaging, such as cardiac-gated MRI or CT, the

registration may also be gated at the same event during the heart cycle to optimize the registration accuracy at block 226.

[0108] There are various types of registration procedures to be utilized that can be optionally gated, via the ECG gating 226. Again, patient registration is the process of determining how to correlate the position of the instrument or catheter 52 in the patient 14 to the position on the pre-acquired or intra-operative acquired images. There are typically four different ways of registering the position of the catheter 52 in relation to the images acquired at block 224. The first registration procedure is point registration. With point registration, the pre-operative images acquired may be synchronized by the ECG gating block 226. To manually register the patient 14, the physician will select landmarks or particular points identified in the pre-acquired images and then touch the corresponding points in the patient's anatomy with the pointer probe 66. By selecting the internal or external landmarks on the anatomy or fiducial markers 60 that are identifiable in the pre-acquired images, it is possible to establish a relationship with the coordinate system for navigation. To perform an automated point registration process, the fiducial markers 60 may also include the dynamic reference frames 54.

[0109] The second type of registration is a surface registration technique. This technique is substantially similar to the point registration technique, except that the pointer probe 66 or the catheter 52 is dragged or passed along the patient's anatomy, either internally or externally. By using surface recognition software, as is known in the art, the navigated surface can be automatically matched with the corresponding surface in the pre-acquired image. Again, to increase accuracy further, this registration technique may also be synched to when the pre-acquired image was captured, via block 226.

[0110] Another technique for registering two different modalities is by a path registration technique using the EM catheter 52. When the EM catheter 52 penetrates a specific region in the anatomy, such as a vein, it is possible to store the location of the sensors 58, along the path by collecting the sensor data in synchronization with the heartbeat time (ECG gating 226). A virtual 3-dimensional curve can then be built to represent an actual cavity or vessel. Using known pattern recognition or distance map algorithms, it is then possible to locate and find the specific shape of that curve in the pre-operative scan or image and get an automatic path registration.

[0111] Examples of types of catheters used for the path type registration technique include spiral or balloon catheters, as illustrated in Figures 15a-15c and 16, respectively. As shown in Figure 15a, a spiral catheter 238 is illustrated that includes electromagnetic coil sensors 58 positioned spirally within the inner surface of the vein 240. The advantage of the spiral catheter, is that there is no blood obstruction within the vein 240 and no risk of balloon deflation issues. Figure 15b illustrates the data collection and virtual 3D curve 242 that is constructed

from the sensed signals, via spirally oriented sensors 58. The virtual 3-dimensional curve 244 is illustrated in Figure 15c, which represents the final 3D shaped vessel, based on the curve 242, which represents the vein that is to be matched with a segment vein in the pre-operative or intraoperative scan.

[0112] Turning to Figure 16, a balloon catheter 246 that includes a plurality of balloons 248, each having sensor coils 58 located therein, is illustrated. Here again, the balloons 248 fit in the vein 250 and center the coils 58 to match the 3-dimensional shape of the vein 250. Here again, this enables a final 3D shape of the vein 250 to be modeled and matched with a segmented vein in the pre-operative scan or intraoperative scan.

[0113] Another type of registration process, as previously discussed, involves the 2D/3D registration of a fluoroscopic image and a pre-op scan, which are each synchronized using the ECG gating technique 226. With both modality images acquired at the same time during a heartbeat, both images are then static and potentially matchable. This non-invasive method merges the 3D pre-operative scan with the 2D image. One way to automatically register the heart with fluoroscopy and CT or other imaging modality is to use the spinal vertebrae that is next to the heart itself as the anatomical landmark. The thoracic vertebrae are key landmarks to get the automatic 2D to 3D registration. In the alternative, angiography and the use of vessels themselves for registration between both modalities may also be utilized. Alternatively, known 3D to 3D or 4D to 4D registration may also be employed.

[0114] Returning to Figure 13, once the image acquired during the image acquisition phase 224 has been registered to the patient at block 236 using ECG gating techniques 226, the procedure proceeds to block 254 where the instrument or catheter 52 is tracked using the navigation system 10. Again, the navigation system 10 utilizes the electromagnetic tracking system 44 or any other type of tracking system, such as optical, acoustic, conductive, etc. From the tracking block 254, the process 220 includes block 256 that identifies the electromagnetic instrument, such as the catheter 52 or guide wire that is being tracked in the tracking block 254. Again, the instrument 52 may either receive or transmit electromagnetic signals enabling the tracking system 44 to identify the location of the instrument 52 relative to the patient 14 and relative to the pre-acquired images during the image acquisition block 224, via the registration block 236. This enables navigation of the catheter 52 or any other instrument relative to the pre-acquired images at block 258. Again, once the images from block 224 have been registered at block 236 and synchronization, via ECG gated block 226, the navigation catheter 52 is inserted into one of the patient's organs, such as the heart, via block 222 and its virtual representation is displayed on the images, via block 258.

[0115] Upon navigating the catheter 52, via block 258, the procedure 220 proceeds to block 260 where the procedure to find an optimized lead placement site is con-

ducted. As an input to this site selection procedure 260, additional sensors may be embedded in the catheter 52, in order to provide cardiac or anatomic function measurements, via internal sensors at block 262. These additional sensors may include an electrophysiological (EP) tip, pressure sensors, temperature sensors, accelerometers, Doppler transducers, tissue sensors, spectroscopy sensors and tracking sensors 58. By using the real-time data received from these sensors in association with the navigation images, the navigation system 10 assists the physician to identify key landmarks or estimated optimized sites on the images 224, such as the coronary sinus. The landmark selection may be manual or automatic by collecting and storing the information of the points on the image 224. Additionally or alternatively, the navigation system 10 may display one or more multiple color coded maps, via display 36, based on the data each sensor communicates to the navigation system 10. For example, temperature maps can be overlaid in real-time on the images 224, based on the temperature, the catheter 52 temperature sensor transmits. Also, the EP signal can be assigned to the collective points to assist the physician to make a decision where the coronary sinus is or is not.

[0116] Further information that can be delivered at block 262 includes a catheter or instrument information. In this regard, various catheters or instruments have flexibility or bending parameters, which enables different types of catheters to be navigated to different types of sites. This is sometimes referred to as a tortuosity factor. Navigating through a tortuous vascular structure generally requires a catheter to be very flexible and bendable without fracturing or failure. This type of information may also be delivered, via block 262 to insure that the proper catheter is being utilized to be navigated in the appropriate site. If it is determined that the site is too tortuous for the particular catheter utilized, the system will identify this to enable the surgeon to select a more appropriate catheter or instrument, via the tortuosity factor.

[0117] Multiple EM catheters 52 may also be utilized and positioned on the left and right side of the heart to track the motion of the left and right side of the heart in order to optimize the heart function and pacing performance. In this regard, both sides of the heart are tracked to insure that they are balanced in order to have the proper flow, thereby optimizing the lead placement based on knowing this balance.

[0118] Moreover, if the image acquisition 224 is based on an ultrasound image, or if the catheter includes an internal ultrasound transducer sensor then Doppler information is available to provide hemo-dynamic data relative to the position. In this regard, the hemo-dynamic information enables a physician to calculate ejection fractions in the cardiac area to determine the volume of blood and flow through the heart using the Doppler technique. By measuring the volume of blood moving in and out of the chambers, this also provides further cardiac or physiological measurements in order to optimize the lead

placement, via the information provided at block 262. In other words, by using a dynamic 3D ultrasound imaging modality or a Doppler sensor in the catheter 52, this enables a physician to visualize the anatomy in space over time. This spatio-temporal Doppler technique is useful for the hemo-dynamic studies and enables calculation of the ejection fraction in the cardiac area. By combining both anatomy information, hemo-dynamics from real-time spatio-temporal echography, localization and navigation technology to select an optimum lead placement at block 260, it is possible to significantly improve pacing performance and thus, patient outcome.

[0119] Thus, site selection at block 260 for the lead placement is optimized by providing an estimated optional site based on real-time anatomic or physiological information, navigation or localization information, hemo-dynamic data, and electrophysiological data, as opposed to simply stuffing the lead into the heart without any optimization. By improving the pacing performance of the therapy, the muscle is paced in its more normal function and overall heart function is improved. In contrast, if lead placement is not optimized, the heart may not function properly, thereby degrading other areas or muscles in the heart as they try to compensate for non-optimized performance.

[0120] An additional input to the site selection block 260 is a multi-patient database storage or atlas 264 that provides previously acquired patient information or an atlas template on the estimated lead placement site. This atlas can be created by recording information used during the lead placement procedure, based on the anatomy and functional data at block 262. This atlas template at block 264 may provide an estimated target that can be visualized on the display 36 as the catheter 52 is navigated during the site selection process 260. Also during the current procedure, this information is stored and recorded at block 264 to update and improve the atlas template. In other words, as you are collecting all of this information during the procedure 220, an atlas is created at block 264, which can then determine and give estimates of what the most likely and best place for lead placement is. The ultimate outcome is trying to locate the best location for lead placement in order to provide the best performance for the heart. For example, assuming that one hundred previous procedures on one hundred patients have been performed and the information was recorded during these procedures that identified the path and sites where the leads were placed for optimized performance, for the one hundred and first procedure, the physician will use the previously acquired one hundred procedures to further optimize the results. This will provide a path to guide the physician to an estimated optimized site, which can be accessed via the site selection process at block 260.

[0121] Based on the multiple maps (position EP, speed, temperature, hemo-dynamic, etc), the physician can identify the coronary sinus ostium and cannulate the coronary sinus. In this regard, at block 266, the cath-

eter 52 is guided to an estimated initial site location 268, via the site location storage block 270 that stores the estimated sites using information from blocks 262 and 264. Once in the coronary sinus, a contrast agent may be administered through the navigation catheter 52. Images of the coronary sinus can be acquired to create a new road map for lead placement. Again, these images can be gated or not, and acquired in 2D, 3D or 4D. Once the revised or updated road map is established and registered at block 236, the instrument, such as the catheter 52 or guide wire is used to select the branch for lead placement, via block 272 and target or site 274. During this procedure, the catheter 52 is pushed and visualized a real-time using images acquired during the contrast agent use. Again, in the coronary sinus ostium to the end lead placement site, this path is stored with the patient database 264 and will be displayed as an overlay on the image for future reference.

[0122] Once the branch 274 has been selected, via navigation system 10, an optimal site for the lead is selected at block 276 identified by estimated target or site 278. By tracking the catheter displacement with the position sensors 58 and by pacing the left heart, it is again possible to optimize the function of the heart. Also, with additional right heart catheter sensors, the overall cardiac function can be optimized, based on accelerometry gathered from the position sensors on both sides of the heart and by real-time measuring of the cardiac wall motion, thereby optimizing the lead site 278. Also, by using the other sensors or other imaging modalities, such as the ultrasound or Doppler, via either an ultrasound imaging device or Doppler sensor in the catheter 52, hemo-dynamic information is gathered. This information is also used to provide an optimized lead site 278. This optimized site 278 may be estimated and identified, via the target 278 or selected by the physician upon reviewing all of the information, via blocks 262 and 264.

[0123] Once the optimal site 278 of the lead placement has been selected, the location and path is stored in a computer and displayed on image 280. The lead can then be placed over the guide wire or through the catheter 52 and directed to the desired optimized site 278. A final check on the performance is evaluated before the procedure 220 is ended. In the event of a failure, lead dislodgement or other cause, the stored path 280 that has been acquired during the implantation procedure can be reused as a road map for the new lead placement. This can also be used and overlaid on future pre-acquired images as a 3D surgical road map for future patients.

[0124] Other uses of the procedure 220 may include an electromagnetic guided biopsy catheter 282, illustrated in Figures 17a and 17b. In this regard, every heart transplant patient undergoes an annual check-up to measure for early indicators of organ rejection in order to determine and confirm that the heart is still not rejected by the patient's body. These indicators include white blood cells, chemical charges, blood oxygen labels, etc. To make this determination, an endovascular biopsy

catheter is inserted into the heart and multiple biopsies are performed in the septum wall of the heart between the left and right side of the heart. In conventional tests, a fluoroscopic procedure is performed utilizing contrast agent and continuous fluoroscopic images are used to select approximately ten biopsy samples in the septum. Again, this leads to exposing the patient to radiation and contrast agents, which is undesirable. By providing an EM guided biopsy catheter 282, the procedure can be optimized and radiation and contrast agent use can be reduced or eliminated all together following the procedure similar to that disclosed in procedure 220.

[0125] The catheter 282 is similar to a standard endovascular biopsy catheter that includes a flexible shaft 284 having a distal biopsy end 286 with a plurality of biopsy graspers 288 to engage and capture a biopsy sample. Located at the proximal end of the catheter 282 is a fixed handle 290 and a movable portion 292, which articulates the graspers 288. Located within the shaft 284 are a plurality of electromagnetic sensors 294 that operate similar to the sensors 58 in the catheter 52. In this way, the shaft and the distal end of the catheter 282 may be tracked via the electromagnetic tracking system 44.

[0126] By utilizing the techniques set forth in the procedure 220, shown in Figure 13, along with the electromagnetic guided biopsy catheter 282, the distal end of the catheter 282 may be precisely guided to optimum sample sites in the septum without the constant radiation exposure and reduced or eliminated use of contrast agents. Moreover, by again building a database to create an atlas map, various optimized sample site locations can be identified in the pre-acquired images, so that the catheter 282 can simply be navigated to these sample sites to gather the biopsy tissue. Thus, only a couple of images are required to perform this task instead of using constant radiation to visualize the biopsy catheter and a more precise sampling can be achieved. It should further be noted that the biopsy catheter 282 may be utilized to biopsy other areas of the patient as well, such as the spine, cervical or other regions of a patient 14.

[0127] The procedure 220 may also be used for a catheter-based approach using the navigation system 10 to treat neurological disease. In this regard, today most of the neurological diseases are treated and accessed from the cranium down to the neurological site in order to treat diseases, such as tumors, ventricle blockages, Parkinson's, aneurysm, etc. However, this type of treatment results in significant trauma due to forming a skull hole, dura opening, fiber destruction, or other cerebral structural damage. Also, cell, drug, or gene delivery generally cannot be taken orally because the product delivered is destroyed by the digestive system. Therefore, site specific delivery is needed. A minimally invasive navigation approach is possible since all cerebral structures are accessible from either vascular or cerebrospinal fluid tree (CSF) access. By using the catheter 52 equipped with the EM sensors 58 that can be tracked by the EM tracking system 44 and by using the image registration techniques

236 to overlay the position of the catheter 52 onto a pre-operative (CT, MRI, etc.) and or intra-operative (fluoroscopy, ultrasound, etc) images, the catheter 52 may be steered from the jugular, groin, or spine all the way to the neurological site, via the endovascular or the cerebral fluid tree path. At the neurological site, treatment can then be delivered and provided.

[0128] For example, site specific therapy can be delivered, such as gene, drug, or cell delivery at the site specific area. For aneurysm treatment, a site specific biologic or embolic treatment can be delivered to attempt to correct the aneurysm. With Parkinson's disease, lead placement through the third and fourth ventricle using the cerebral fluid tree is possible. At the caudate nucleus, a biological patch delivery using the cerebral fluid tree is also possible. The procedure may also be used for shunt placement to correct an occlusion. Here again, instead of drilling a hole, a minimally invasive approach through either the endovascular or cerebrospinal tree is an option. Again, these types of neurological procedures may also be optimized by sensing various surrounding anatomical functions with the catheter 52 or other instrument to again optimize lead placement or optimize gene, cell or drug delivery by providing an estimated delivery site.

[0129] Turning now to Figures 18a and 18b, a prior art intravascular ultrasound (IVUS) catheter 296 is illustrated. The IVUS catheter 296 is a disposable catheter that includes an ultrasound transducer 298 that is typically used to visualize tissue and/or blood vessels in a minimally invasive approach. The IVUS catheter 296 is a disposable catheter that is also very costly. The transducer 298 enables visualization only from a side view plane 300 and does not provide a forward view 302 whatsoever. The single side view 300 is available with the catheter 296 positioned statically. Should the IVUS catheter 296 be rotated about arc 304, as illustrated in Figure 18b, various side view planes 300, 300', ... are available about the rotation axis 304.

[0130] Referring now to Figure 19, a virtual intravascular ultrasound (IVUS) catheter 306 according to the teachings of the present invention is illustrated. The virtual IVUS catheter 306 includes at least one electromagnetic tracking sensor 308 or multiple tracking sensors positioned along its shaft to again track the location of the virtual IVUS catheter 306 with the electromagnetic tracking system 44. Again, it should be noted that any other type of tracking system and sensors may also be utilized. The virtual IVUS catheter 306 is able to generate virtual IVUS views from an infinite number of planes or direction 310, 310', 310" from any angle or position relative to the catheter 306, further discussed herein.

[0131] Referring to Figure 20, a virtual IVUS system 312 according to the teachings of the present invention is illustrated, which includes the virtual IVUS catheter 306 having the sensor 308. The virtual IVUS system 312 works in combination with the navigation system 10 and employs the electromagnetic tracking system 44. With this type of configuration, an ultrasound imaging modality

may be used to replace the fluoroscopic imaging device 12 or the imaging device 12 may be used in combination with the ultrasound imaging modality. In this regard, a dynamic 3D ultrasound probe 314, such as the Phillips XMatrix probe, combined with an electromagnetic tracking sensor 316 is positioned outside the body of the patient 14 and connected to an ultrasound controller 317. The ultrasound controller 317 may be a separate controller or combined with the work station 34 and coil array controller 48. By using the 3D probe 314 with the electromagnetic sensor 316, the field of view of the probe 314 is calibrated to the EM coordinate system of the electromagnetic tracking system 44. By tracking the flexible EM catheter 306 equipped with at least one electromagnetic sensor 308, the controller 317 can generate a virtual IVUS view from that coil position, as illustrated in Figure 19. In other words, the dynamic 3D ultrasound imaging modality from the 3D ultrasound probe 314 allows a physician to visualize the anatomy in space over time. By tracking the flexible catheter 306 equipped with at least three EM coils 308, it is possible to superimpose the catheter 306 onto this spatio-temporal echographic image. The three coils of the catheter 306 represent the planes in the space over time from the perspective of the catheter 306. The equation of those planes may then be calculated to display the corresponding echographic spatio-temporal plane to visualize the catheter 306 in its entire shape in a real-time echographic image or from the point of view of the catheter.

[0132] Therefore, by providing a very cost effective catheter 306 that does not include an ultrasound transducer in the catheter, but uses the external ultrasound probe 314, virtual IVUS images can be produced and displayed at any angle or direction relative to the catheter 306 or from the catheter's point of view. This enables the physician to superimpose the catheter 306 onto the image 318, illustrated on display 36, as well as generate a field of views from the forward position of the catheter 306. The system also operates to either take a slice of the 3D ultrasound relative to its current location or it may also identify and generate a view of its total path that the catheter or instrument has transversed through. The system 312 also provides a look ahead view as it moves relative to the catheter 306. Basically, the system 312 creates slices based on the vessel position and views transverse to the vessel or axial to the vessel along curved paths or straight paths. Projected trajectories of the forward advance of the catheter 306 can also be tracked and superimposed on the image 318. It should also be noted that while a 3D ultrasound probe 314 has been discussed, a 4D probe or other imaging modalities, such as MRI, CT, OCT and spectroscopy may also be utilized to create the virtual views. Thus, by automatically registering the probe 314 having the sensor 316 relative to the catheter 306 having the sensor 308 using the navigation system 44, automatic registering between these two systems without requiring motion correction is available. Moreover, the ultrasound image, which is registered

via the probe 314 and catheter 306, may also be registered or linked with any other image modalities. In this regard, the ultrasound image modalities may be registered relative to fluoroscopic, MRI, CT, or other image modalities and displayed at one time on the display 36 to provide a further level of information.

[0133] In addition to providing a three-dimensional image volume, the ultrasonic probe 314 may also provide a three-dimensional Doppler volume by switching the ultrasound probe 314 to the spatio-temporal Doppler format. From this Doppler volume, the physician can visualize a metric or statistical measurements for blood flow or motion at the tip of the catheter 306. Again, this system would then not be visualizing an ultrasound image, but visualizing statistics or measurements. This information can be conveyed using color coded figures that are displayed on the display 36. For example; should the catheter 306 be guided through a blood vessel and the Doppler effect measure the volume of blood flow going through the vessel at a certain point, where there is an occlusion, there would be much smaller blood flow on one side of the occlusion than on the other. The quicker blood flow can be characterized by red on one side of the vessel and blue on the occluded side, thereby identifying where the occlusion is within the vessel. Other anatomical functions may also be sensed as previously discussed, such as pressure, temperature, etc and also visualized on the display 36. This again enables the navigation system 10 to identify an estimate site to navigate to and deliver a therapy (e.g., ablation).

[0134] In addition to navigating and visualizing the area of interest, the catheter 306 or other instrument may also deliver therapy at the point of interest. For example, the catheter 306 may delivery a drug, ablate, or deliver a lead or other device following the procedure 220. With drug delivery, a profusion model may be overlaid over the tracked image that models the flow of the drug depending on the dosage and type of drug delivered. This overlay can be color coded to identify the region that the drug will interact at the area of interest. Also, by providing sensors at the catheter 306, real-time monitoring of the drug delivery may also be visualized on the display 36, thereby providing real-time feedback on the diffusion through the tissue of the drug delivery. In this way, proper dosage of the drug delivery is achieved. These templates can also identify therapy effective zones, such as ablation zones in the area that the ablation may affect before the ablation is performed. This also provides an optimized procedure.

[0135] With all of the identified procedures, a dual delivery therapy may also be provided. For example, with drug therapy, some drugs require stimulation to activate the drugs, such as by heat, while other drugs may require a second drug to activate. Thus, the instrument or catheter utilized to navigate to the particular optimized site can both deliver the drug and also heat it using a heat probe or deliver a second drug in order to activate it and provide better performance. The drug delivery may also include magnetically conductive components, so that the

pattern or direction of where the drug delivery is applied is controlled, via a magnetically sensitive sensor attached to the catheter. The drug delivery or any other type of delivery, such as cell or gene delivery may also be gated or synched to an anatomical physiological function, such as the heartbeat, via the ECG monitor 62 or other devices. In this way, by gating the delivery to the particular cycle, proper placement and dosage of the drug, gene or cell delivery is also optimized.

[0136] The instruments may also deliver the drugs, genes or cells using a pattern delivery technique. With this type of technique, drugs may be delivered over a significant area. For example, a 9x9 grid spaced about 0.1 millimeters apart may be the delivery area. The catheter 52 may be provided with multiple delivery needles, such as 3x3 grouping of needles, thereby requiring only nine deliveries to fill the 9x9 area. This again delivers the drug to the needed area, thereby optimizing the result of the drug delivery and reducing the time for delivering the drug. Moreover, the catheter may also include a sensor to provide additional feedback on the delivery to again identify that a sufficient amount of drug has been delivered. In which case, the delivery plan may be able to be changed using this real-time feedback. This delivery plan can again include an icon representing where the drug delivery should take place that is determined by the navigation system 10.

[0137] Referring to Figures 21-23, an exemplary catheter, along with a delivery insert, which may be used with the navigation system and procedure disclosed herein is discussed in further detail. As illustrated in Figure 21, a catheter 326 is illustrated to include a delivery tube 328 and a handle 330 that defines a passage 332 in communication with the tube 328. As shown in Figure 22, a multi-sensor insert 334 is illustrated that includes four sensor coils 336. The insert 334 is electronically in communication with the navigation probe interface 50, similar to the catheter 52 illustrated in Figure 1. The insert 334 is operable to be slidably inserted within passage 332 defined in handle 330 in order to pass into delivery tube 328, as illustrated in Figure 23. The insert 334 enables the use of various conventional catheters, such as the catheter 326 without requiring further modification to existing catheters. In other words, use of the insert 334, having electromagnetic sensors 336 enables conventional catheters to be converted to a navigable tracked catheter by simply passing the insert 334 within the catheter 326. The insert 334 includes a cannula 338 to enable delivery of various therapies through the catheter 326 and insert 334 once the insert 334 has been navigated to the appropriate site, via the catheter 326. For example, a lead may be passed through the cannulation of the instrument 334 during a cardiac lead placement, as previously discussed.

[0138] The description of the invention is merely exemplary in nature and, thus, variations that do not depart from the gist of the invention are intended to be within the scope of the invention. Such variations are not to be regarded as a departure from the scope of the invention.

Claims

1. An image guided navigation system for navigating relative to a region of a patient, said image guided navigation system comprising:
 - an imaging device (314) positioned outside the patient and operable to generate image data of an interior of the region of the patient;
 - an instrument (306) operable to be navigated in the region of the patient;
 - a first tracking device (308) attached to the instrument and operable to be used to track the position of the instrument in the region of the patient;
 - a controller (317) connected to said imaging device (314) and said tracking device (308), and operable to generate, from said image data, virtual images of said interior along a navigated path of the instrument from the instrument's point of view; and
 - a display operable to display the virtual images.
2. The image guided navigation system according to claim 1, wherein said controller (317) is operable to generate virtual images from a look ahead view of the instrument.
3. The image guided navigation system according to claim 1, wherein said controller (317) is operable to control said imaging device based on the instrument position, so as to generate said virtual images.
4. The image guided navigation system as defined in Claim 1, wherein said imaging device is an ultrasonic probe and said controller is an ultrasonic controller.
5. The image guided navigation system as defined in Claim 1, wherein said imaging device is a 3D ultrasonic probe.
6. The image guided navigation system as defined in Claim 1, further comprising a second tracking device attached to said imaging device operable to be used to track the position of the imaging device.
7. The image guided navigation system as defined in Claim 6, wherein said controller is further operable to automatically register said image data from said imaging device by tracking said imaging device with said second tracking device to said instrument having said first tracking device.
8. The image guided navigation system as defined in Claim 1, wherein said virtual images include a plurality of image planes about a distal end of said instrument including a forward image plane.

9. The image guided navigation system as defined in Claim 1, wherein said instrument is further operable to deliver a therapy to the patient.
10. The image guided navigation system as defined in Claim 9, wherein said therapy is operable to be gated to a physiological event.
11. The image guided navigation system as defined in Claim 10, wherein said gated therapy is operable to be dual delivery of both therapy and a stimulus.
12. The image guided navigation system according to claim 1, further comprising at least one sensor attached to said instrument and operable to sense a physiological parameter in the patient; said controller being operable to track the position of the instrument with said tracking device and operable to receive the sensed physiological parameter from said sensor, said controller further being operable to estimate the optimized site and superimpose an icon representing the location of the optimized site and an icon representing the instrument, based on the sensed physiological parameter and on the position of the instrument; said display being operable to display the icon of the estimated optimized site and the icon representing the instrument in the patient.
13. The image guided navigation system as defined in Claim 1, wherein said instrument is selected from a group comprising a catheter, a guide wire, a stylet, an insert, a needle and a combination thereof.
14. The image guided navigation system as defined in Claim 1, wherein said tracking device is selected from at least one of an electromagnetic, optical, acoustic, and conductive tracking devices.
15. The image guided navigation system as defined in Claim 12, wherein said at least one sensor is an ultrasound transducer operable to generate a Doppler effect to provide hemo-dynamic physiological parameters.
16. The image guided navigation system as defined in Claim 12, wherein said at least one sensor is selected from at least one of a temperature sensor, pressure sensor, hemo-dynamic sensor, EP sensor, impedance sensor, accelerometer, tissue sensor, spectroscopy sensor and a combination thereof.
17. The image guided navigation system as defined in Claim 12, wherein said controller is further operable to generate an atlas map based on previously acquired optimized sites.
18. The image guided navigation system as defined in

Claim 17, wherein said atlas map is further utilized to estimate the optimized site.

19. The image guided navigation system as defined in Claim 12, wherein the optimized site is an optimized lead placement site in a coronary sinus region.
20. The image guided navigation system as defined in Claim 12, wherein said controller is further operable to register said image data with the patient using a registration technique selected from at least one of point registration, surface registration, path registration, 2D to 3D registration, 3D to 3D registration and 4D to 4D registration.
21. The image guided navigation system as defined in Claim 12, further comprising an anatomic gating device operable to sense a physiological event wherein said image data is gated to said physiological event and wherein registration by said controller is gated to said physiological event.
22. The image guided navigation system as defined in Claim 1, wherein said instrument is a guided biopsy catheter.
23. The image guided navigation system as defined in Claim 1, further comprising a tracking system operable to track said instrument by tracking said tracking device attached to said instrument.
24. The image guided navigation system as defined in Claim 23, wherein said tracking system is selected from a group comprising an electromagnetic tracking system, an optical tracking device, a conductive tracking system, a fiberoptic tracking system, and a combination thereof.

Patentansprüche

1. Bildgeführtes Navigationssystem zum Navigieren in Bezug auf eine Region eines Patienten, mit:

einer Bildgebungsvorrichtung (314), die sich außerhalb des Patienten befindet und so betreibbar ist, dass sie Bilddaten eines Inneren der Region des Patienten erzeugt;
einem Instrument (306), das so betreibbar ist, dass es in der Region des Patienten navigiert werden kann;
einer ersten Spurverfolgungsvorrichtung (308), die an dem Instrument angebracht ist und so betreibbar ist, dass sie zum Verfolgen der Position des Instruments in der Region des Patienten verwendet werden kann;
einem Steuergerät (317), das mit der Bildgebungsvorrichtung (314) und der Spurverfol-

- gungsvorrichtung (308) verbunden ist und so betreibbar ist, dass es aus den Bilddaten virtuelle Bilder des Inneren entlang einem navigierten Weg des Instruments von dem Standpunkt des Instruments aus erzeugt; und
einer Anzeigevorrichtung, die so betreibbar ist, dass sie die virtuellen Bilder anzeigt.
2. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** das Steuergerät (317) so betreibbar ist, dass es virtuelle Bilder aus einer Vorwärtssicht des Instruments erzeugt. 10
 3. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** das Steuergerät (317) so betreibbar ist, dass es die Bildgebungsvorrichtung aufgrund der Position des Instruments so steuert, dass sie die virtuellen Bilder erzeugt. 15
 4. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** die Bildgebungsvorrichtung eine Ultraschallsonde ist und das Steuergerät ein Ultraschall-Steuergerät ist. 20
 5. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** die Bildgebungsvorrichtung eine 3D-Ultraschallsonde ist. 25
 6. Bildgeführtes Navigationssystem nach Anspruch 1, das weiterhin eine zweite Spurverfolgungsvorrichtung aufweist, die an dem Instrument angebracht ist und so betreibbar ist, dass sie zum Verfolgen der Position der Bildgebungsvorrichtung verwendet werden kann. 30
 7. Bildgeführtes Navigationssystem nach Anspruch 6, **dadurch gekennzeichnet, dass** das Steuergerät weiterhin so betreibbar ist, dass es die Bilddaten automatisch aus der Bildgebungsvorrichtung registriert, indem es die Bildgebungsvorrichtung mit der zweiten Spurverfolgungsvorrichtung bis zu dem Instrument verfolgt, das die erste Spurverfolgungsvorrichtung hat. 35
 8. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** die virtuellen Bilder mehrere Bild-Ebenen um ein distales Ende des Instruments umfassen, unter anderem eine Vorwärtsbild-Ebene. 40
 9. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** das Instrument weiterhin so betreibbar ist, dass es den Patienten therapiert. 45
 10. Bildgeführtes Navigationssystem nach Anspruch 9, **dadurch gekennzeichnet, dass** die Therapie so eingerichtet ist, dass sie auf ein physiologisches Ereignis gegatet wird. 50
 11. Bildgeführtes Navigationssystem nach Anspruch 10, **dadurch gekennzeichnet, dass** die gegatete Therapie so eingerichtet ist, dass sowohl eine Therapie als auch eine Stimulation durchgeführt werden können. 55
 12. Bildgeführtes Navigationssystem nach Anspruch 1, das weiterhin mindestens einen Sensor aufweist, der an dem Instrument angebracht ist und so betreibbar ist, dass er einen physiologischen Parameter bei dem Patienten erfasst, wobei das Steuergerät so betreibbar ist, dass es die Position des Instruments mit der Spurverfolgungsvorrichtung verfolgt, und so betreibbar ist, dass es den erfassten physiologischen Parameter von dem Sensor empfängt, und weiterhin so betreibbar ist, dass es aufgrund des erfassten physiologischen Parameters und der Position des Instruments die optimierte Stelle ermittelt und ein Icon, das die Lage der optimierten Stelle darstellt, und ein Icon einblendet, das das Instrument darstellt, und die Anzeigevorrichtung so betreibbar ist, dass sie das Icon der ermittelten optimierten Stelle und das Icon anzeigt, das das Instrument in dem Patienten darstellt.
 13. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** das Instrument aus der Gruppe Katheter, Führungsdraht, kleine Sonde, Kanüle, Nadel und einer Kombination daraus gewählt ist.
 14. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** die Spurverfolgungsvorrichtung aus mindestens einer von elektromagnetischen, optischen, akustischen und leitenden Spurverfolgungsvorrichtungen gewählt ist.
 15. Bildgeführtes Navigationssystem nach Anspruch 12, **dadurch gekennzeichnet, dass** der mindestens eine Sensor ein Ultraschall-Wandler ist, der so betreibbar ist, dass er einen Doppler-Effekt erzeugt, um hämodynamische physiologische Parameter zu liefern.
 16. Bildgeführtes Navigationssystem nach Anspruch 12, **dadurch gekennzeichnet, dass** der mindestens eine Sensor aus mindestens einem der Sensoren Temperaturfühler, Drucksensor, hämodynamischer Sensor, EP-Sensor, Impedanzsensor, Beschleunigungsmesser, Gewebesensor, Spektroskopie-Sensor und einer Kombination daraus gewählt ist.
 17. Bildgeführtes Navigationssystem nach Anspruch

- 12, **dadurch gekennzeichnet, dass** das Steuergerät weiterhin so betreibbar ist, dass es aufgrund der vorher erfassten optimierten Stellen eine Atlaskarte erzeugt.
18. Bildgeführtes Navigationssystem nach Anspruch 17, **dadurch gekennzeichnet, dass** die Atlaskarte weiterhin zum Ermitteln der optimierten Stelle genutzt wird.
19. Bildgeführtes Navigationssystem nach Anspruch 12, **dadurch gekennzeichnet, dass** die optimierte Stelle eine optimierte Spitzenplatzierungsstelle in einer Region des Sinus coronarius ist.
20. Bildgeführtes Navigationssystem nach Anspruch 12, **dadurch gekennzeichnet, dass** das Steuergerät weiterhin so betreibbar ist, dass es die Bilddaten für den Patienten unter Verwendung eines Registrierungsverfahrens registriert, das aus mindestens einem der Registrierungsverfahren Punktregistrierung, Flächenregistrierung, Wegregistrierung, 2D/3D-Registrierung, 3D/3D-Registrierung und 4D/4D-Registrierung gewählt ist.
21. Bildgeführtes Navigationssystem nach Anspruch 12, das weiterhin eine Anatomisches-Gating-Vorrichtung aufweist, die so betreibbar ist, dass sie ein physiologisches Ereignis erfasst, wobei die Bilddaten auf das physiologische Ereignis gateget werden und die Registrierung mit dem Steuergerät auf das physiologische Ereignis gateget wird.
22. Bildgeführtes Navigationssystem nach Anspruch 1, **dadurch gekennzeichnet, dass** das Instrument ein geführter Biopsiekatheter ist.
23. Bildgeführtes Navigationssystem nach Anspruch 1, das weiterhin ein Spurverfolgungssystem aufweist, das so betreibbar ist, dass es das Instrument durch Verfolgen der an dem Instrument angebrachten Spurverfolgungsvorrichtung verfolgt.
24. Bildgeführtes Navigationssystem nach Anspruch 23, **dadurch gekennzeichnet, dass** das Spurverfolgungssystem aus der Gruppe elektromagnetisches Spurverfolgungssystem, optisches Spurverfolgungssystem, leitendes Spurverfolgungssystem, faseroptisches Spurverfolgungssystem und einer Kombination daraus gewählt ist.
- un dispositif d'imagerie (314) positionné en dehors du patient et pouvant générer des données d'images d'une partie intérieure de la région du patient;
- un instrument (306) que l'on peut faire naviguer dans la région du patient;
- un premier dispositif de suivi (308) attaché à l'instrument et pouvant être utilisé pour suivre la position de l'instrument dans la région du patient;
- une unité de commande (317) connectée audit dispositif d'imagerie (314) et audit dispositif de suivi (308), et pouvant générer, à partir desdites données d'images, des images virtuelles de ladite partie intérieure le long d'un chemin navigué de l'instrument vu par l'instrument; et
- un écran pouvant afficher les images virtuelles.
2. Système de navigation guidé par images selon la revendication 1, dans lequel ladite unité de commande (317) est fonctionnelle pour générer des images virtuelles à partir d'une vue en avant de l'instrument.
3. Système de navigation guidé par images selon la revendication 1, dans lequel ladite unité de commande (317) est fonctionnelle pour commander ledit dispositif d'imagerie sur la base de la position de l'instrument, de manière à générer lesdites images virtuelles.
4. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel ledit dispositif d'imagerie est une sonde ultrasonore et ladite unité de commande est une unité de commande ultrasonore.
5. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel ledit dispositif d'imagerie est une sonde ultrasonore 3D.
6. Système de navigation guidé par images tel que défini dans la revendication 1, comprenant en outre un deuxième dispositif de suivi attaché audit dispositif d'imagerie pouvant être utilisé pour suivre la position du dispositif d'imagerie.
7. Système de navigation guidé par images tel que défini dans la revendication 6, dans lequel ladite unité de commande est en outre fonctionnelle pour enregistrer automatiquement lesdites données d'images provenant dudit dispositif d'imagerie en suivant ledit dispositif d'imagerie avec ledit deuxième dispositif de suivi audit instrument ayant ledit premier dispositif de suivi.
8. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel lesdites images virtuelles comportent une pluralité de plans

Revendications

1. Système de navigation guidé par images pour la navigation par rapport à une région d'un patient, ledit système de navigation guidé par images comprenant:
8. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel lesdites images virtuelles comportent une pluralité de plans

- d'images autour d'une extrémité distale dudit instrument y compris un plan d'image avant.
9. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel ledit instrument est en plus fonctionnel pour délivrer une thérapie au patient. 5
 10. Système de navigation guidé par images tel que défini dans la revendication 9, dans lequel ladite thérapie est fonctionnelle pour être synchronisée à un événement physiologique. 10
 11. Système de navigation guidé par images tel que défini dans la revendication 10, dans lequel ladite thérapie synchronisée est fonctionnelle pour être une livraison duale à la fois d'une thérapie et d'un stimulus. 15
 12. Système de navigation guidé par images selon la revendication 1 comprenant en outre au moins un capteur attaché audit instrument et fonctionnel pour détecter un paramètre physiologique dans le patient: 20

ladite unité de commande étant fonctionnelle pour suivre la position de l'instrument avec ledit dispositif de suivi et fonctionnelle pour recevoir le paramètre physiologique détecté à partir dudit capteur, ladite unité de commande étant en outre fonctionnelle pour estimer le site optimisé et superposer une icône représentant l'emplacement du site optimisé et une icône représentant l'instrument, sur la base du paramètre physiologique détecté et sur la position de l'instrument, 30

ledit écran étant fonctionnel pour afficher l'icône du site optimisé estimé et l'icône représentant l'instrument dans le patient. 35
 13. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel ledit instrument est sélectionné parmi un groupe comprenant un cathéter, un fil de guidage, un stylet, un insert, une aiguille et une combinaison de ceux-ci. 40
 14. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel ledit dispositif de suivi est sélectionné parmi au moins l'un de dispositifs de suivi électromagnétique, optique, acoustique, et conducteur. 45
 15. Système de navigation guidé par images tel que défini dans la revendication 12, dans lequel ledit au moins un capteur est un transducteur ultrasonore fonctionnel pour générer un effet Doppler pour fournir des paramètres physiologiques hémodynamiques. 50
 16. Système de navigation guidé par images tel que défini dans la revendication 12, dans lequel ledit au moins un capteur est sélectionné parmi au moins l'un d'un capteur de température, un capteur de pression, un capteur hémodynamique, un capteur EP, un capteur d'impédance, un accéléromètre, un capteur à tissus, un capteur spectroscopique, et une combinaison de ceux-ci. 55
 17. Système de navigation guidé par images tel que défini dans la revendication 12, dans lequel ladite unité de commande est en plus fonctionnelle pour générer une carte d'atlas sur la base des sites optimisés précédemment acquis.
 18. Système de navigation guidé par images tel que défini dans la revendication 17, dans lequel ladite carte d'atlas est en plus utilisée pour estimer le site optimisé.
 19. Système de navigation guidé par images tel que défini dans la revendication 12, dans lequel le site optimisé est un site de placement de conducteur optimisé dans une région du sinus coronaire.
 20. Système de navigation guidé par images tel que défini dans la revendication 12, dans lequel ladite unité de commande est en plus fonctionnelle pour enregistrer lesdites données d'images avec le patient en utilisant une technique d'enregistrement sélectionnée parmi au moins l'un d'un enregistrement de point, d'un enregistrement de surface, d'un enregistrement de chemin, d'un enregistrement 2D à 3D, d'un enregistrement 3D à 3D et d'un enregistrement 4D à 4D.
 21. Système de navigation guidé par images tel que défini dans la revendication 12, comprenant en outre un dispositif de synchronisation anatomique fonctionnel pour détecter un événement physiologique dans lequel lesdites données d'images sont synchronisées audit événement physiologique et dans lequel l'enregistrement par ladite unité de commande est synchronisé audit événement physiologique.
 22. Système de navigation guidé par images tel que défini dans la revendication 1, dans lequel ledit instrument est un cathéter de biopsie guidé.
 23. Système de navigation guidé par images tel que défini dans la revendication 1, comprenant en outre un système de suivi fonctionnel pour suivre ledit instrument en suivant ledit dispositif de suivi attaché audit instrument.
 24. Système de navigation guidé par images tel que défini dans la revendication 23, dans lequel ledit système de suivi est sélectionné parmi un groupe com-

prenant un système de suivi électromagnétique, un dispositif de suivi optique, un système de suivi conducteur, un système de suivi à fibre optique, et une combinaison de ceux-ci.

5

10

15

20

25

30

35

40

45

50

55

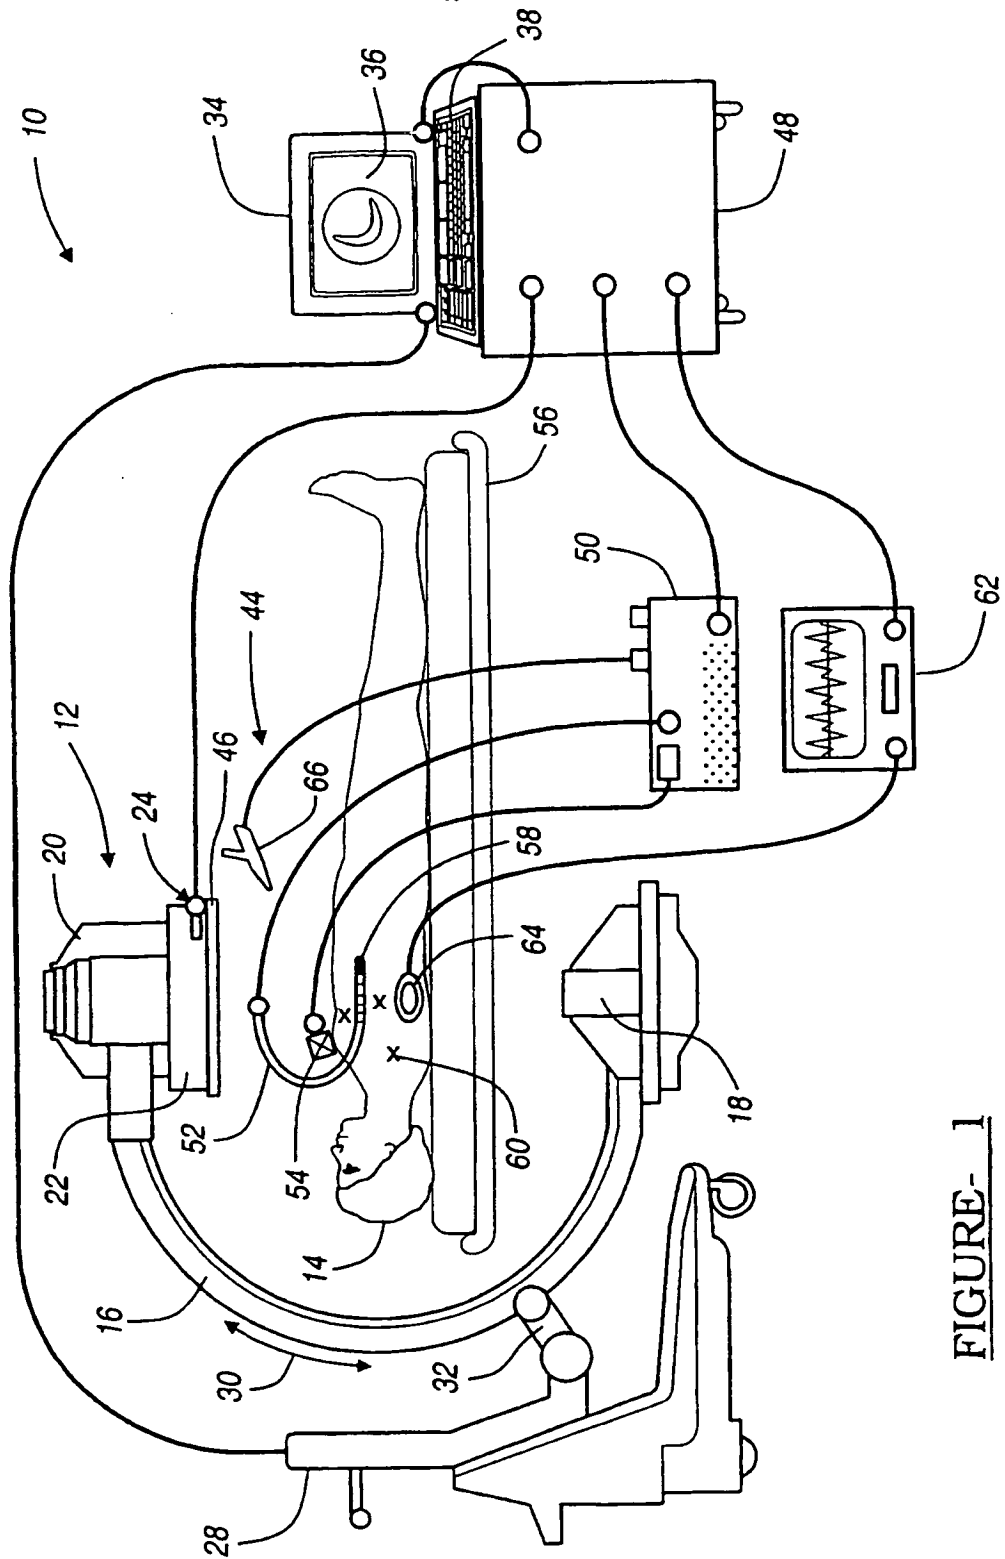


FIGURE- 1

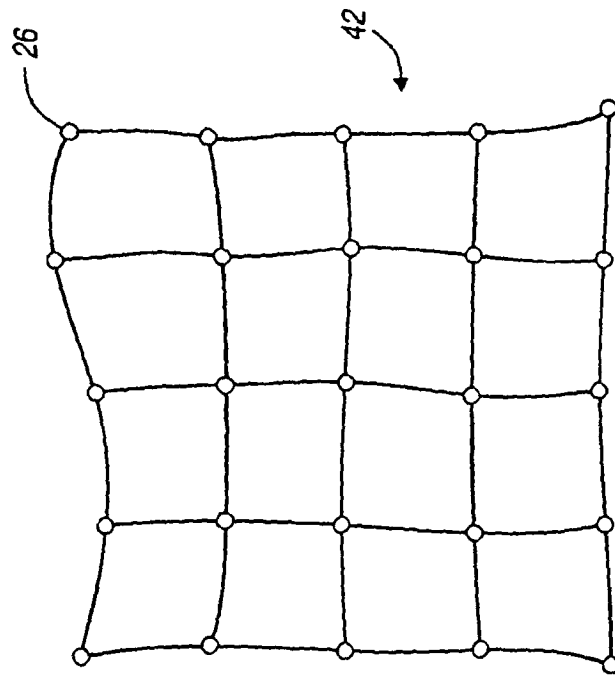


FIGURE 2B

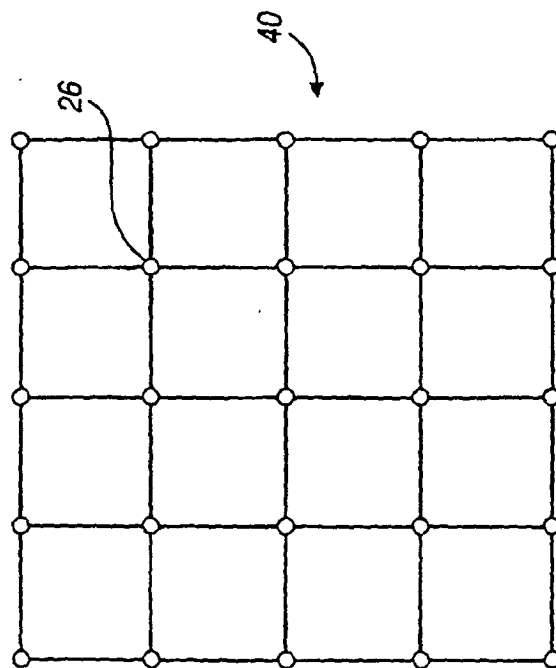


FIGURE 2A

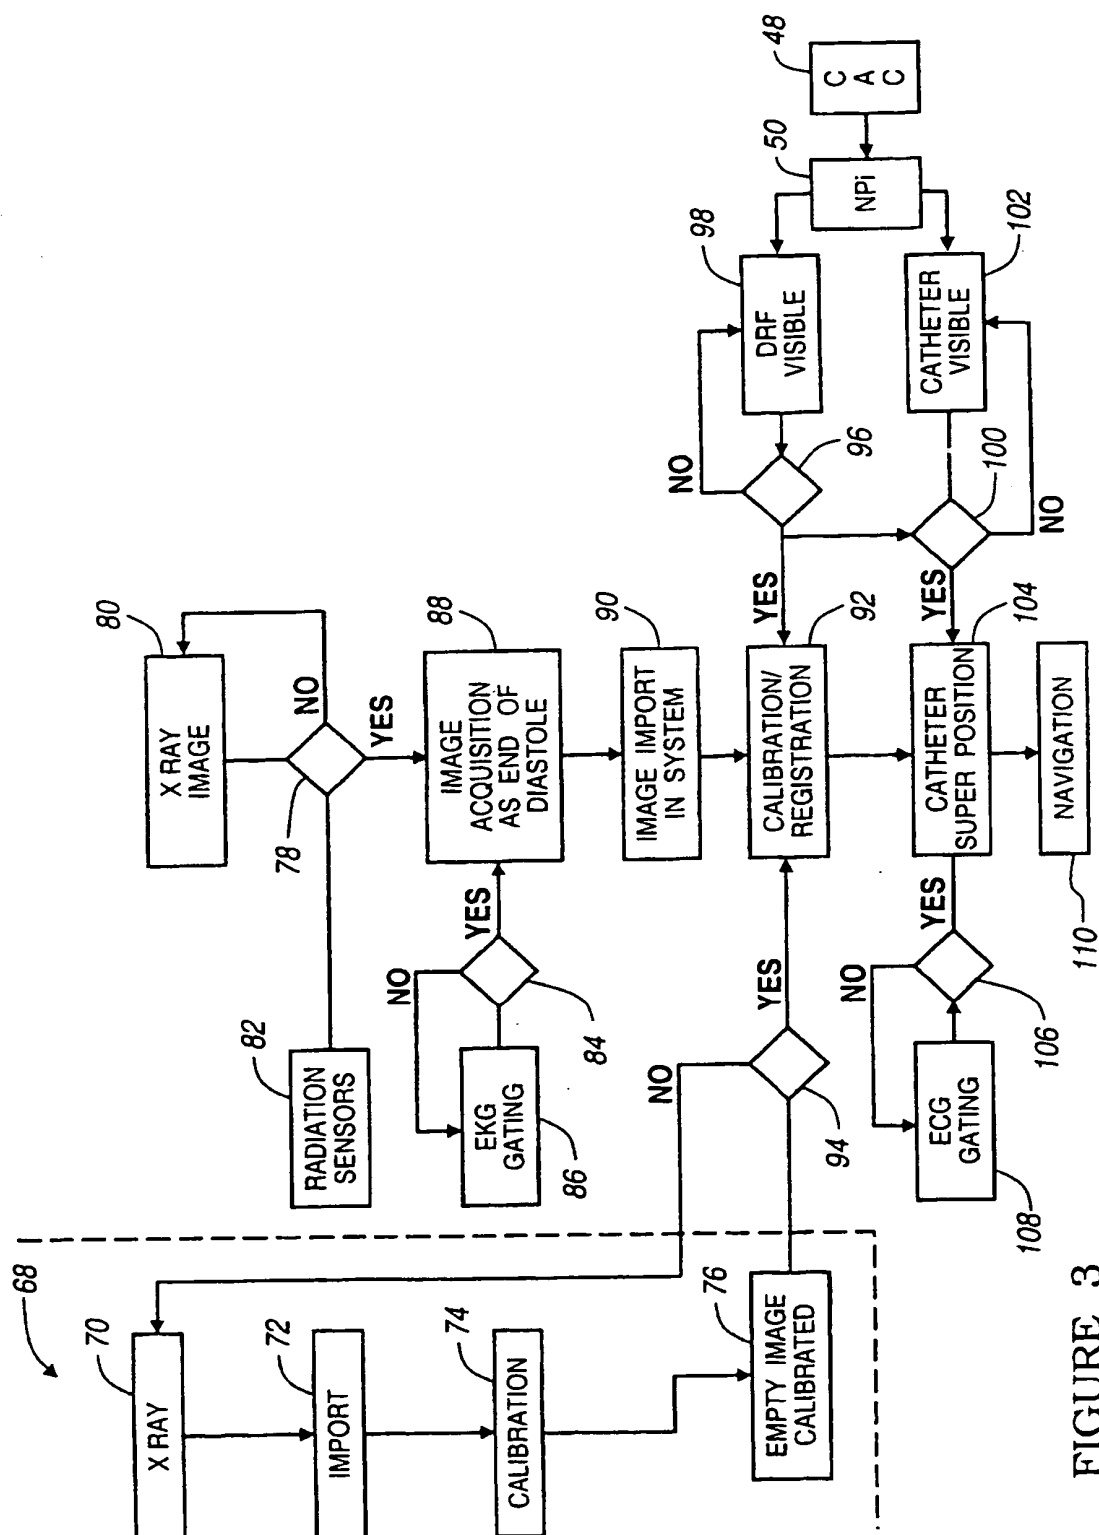


FIGURE 3

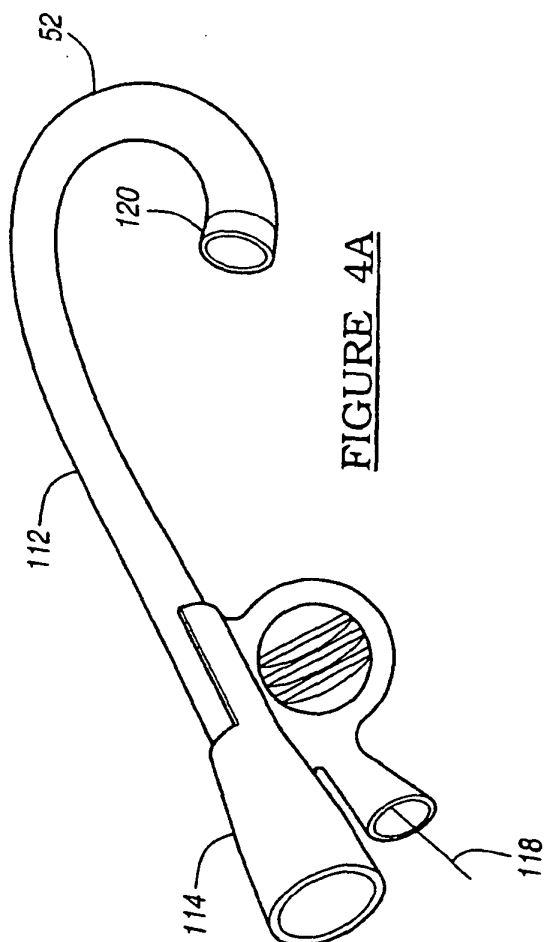


FIGURE 4A

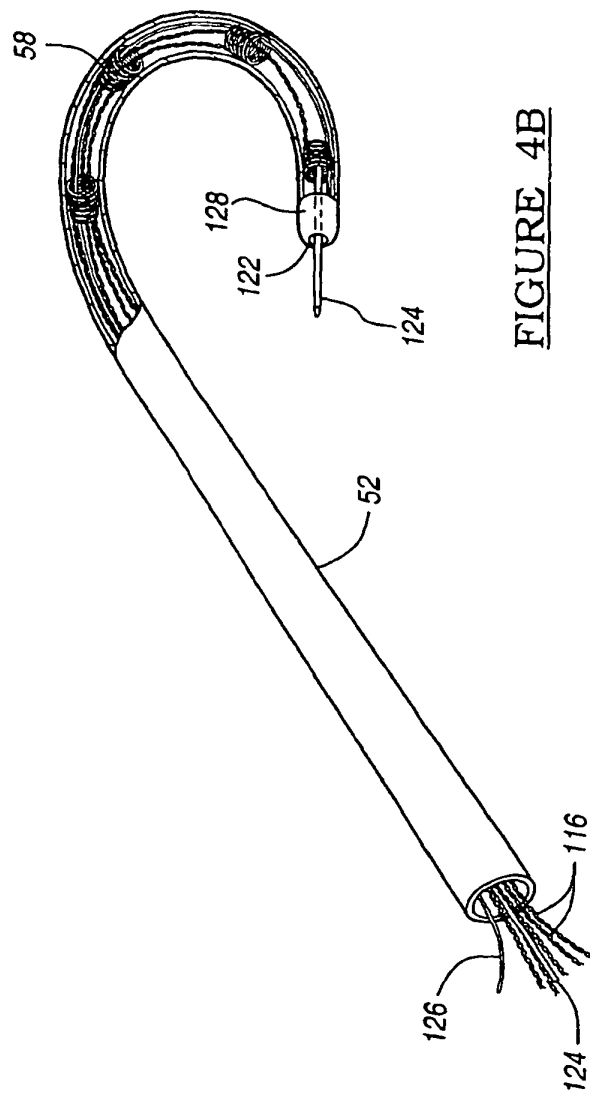


FIGURE 4B

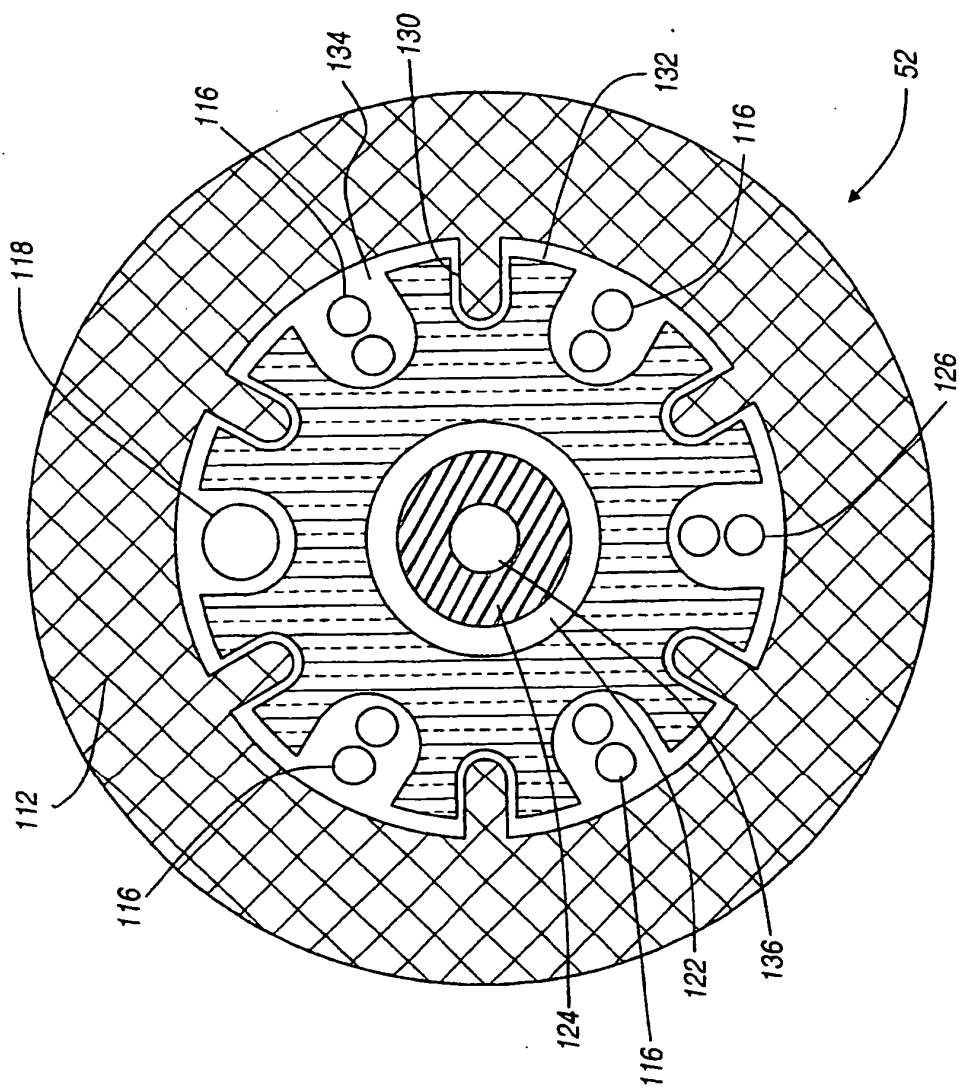


FIGURE 5

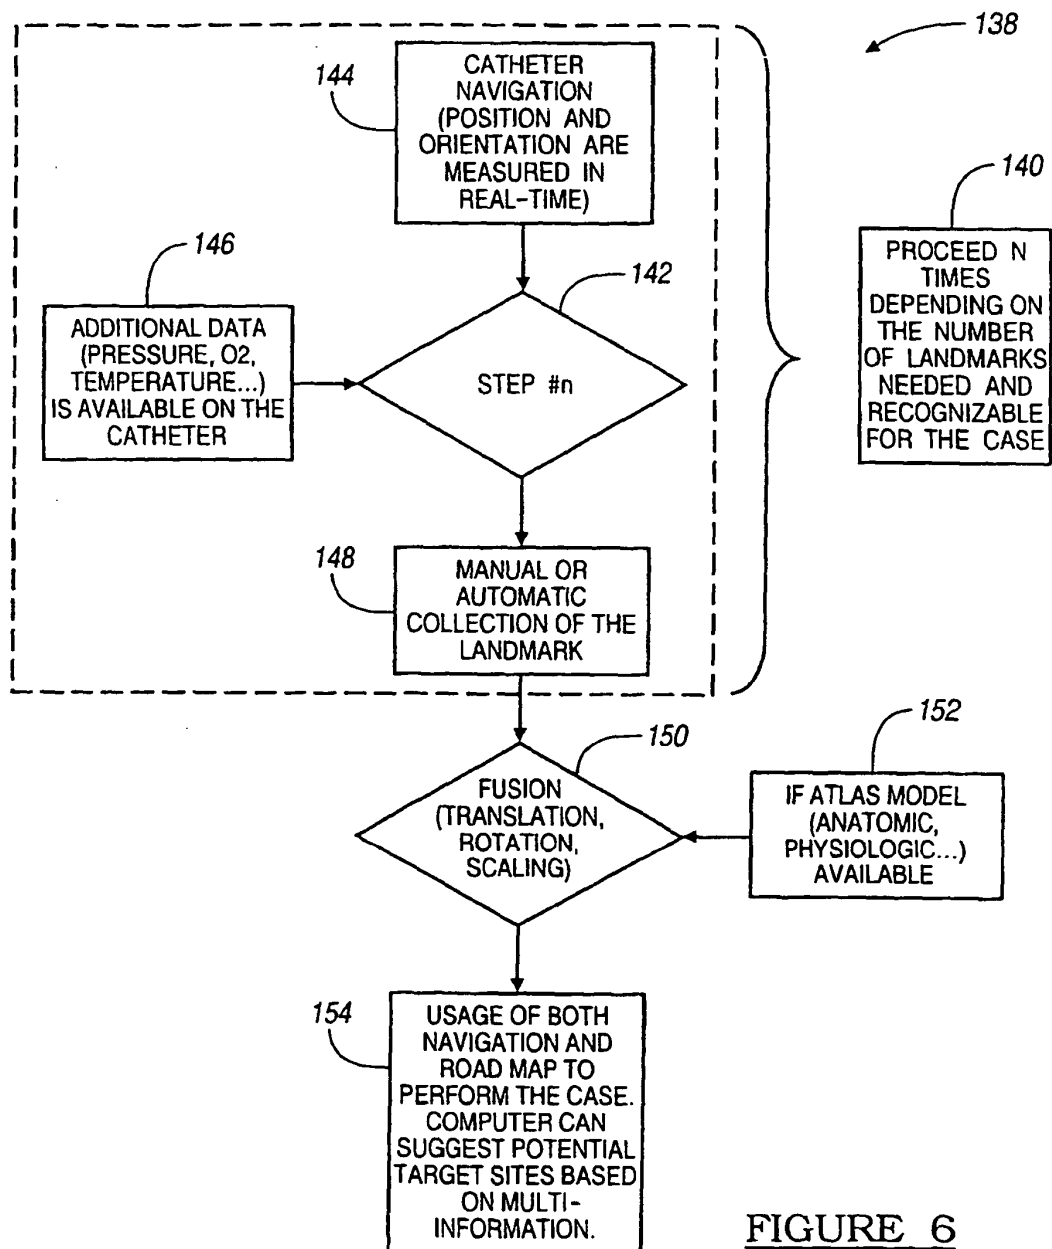


FIGURE 6

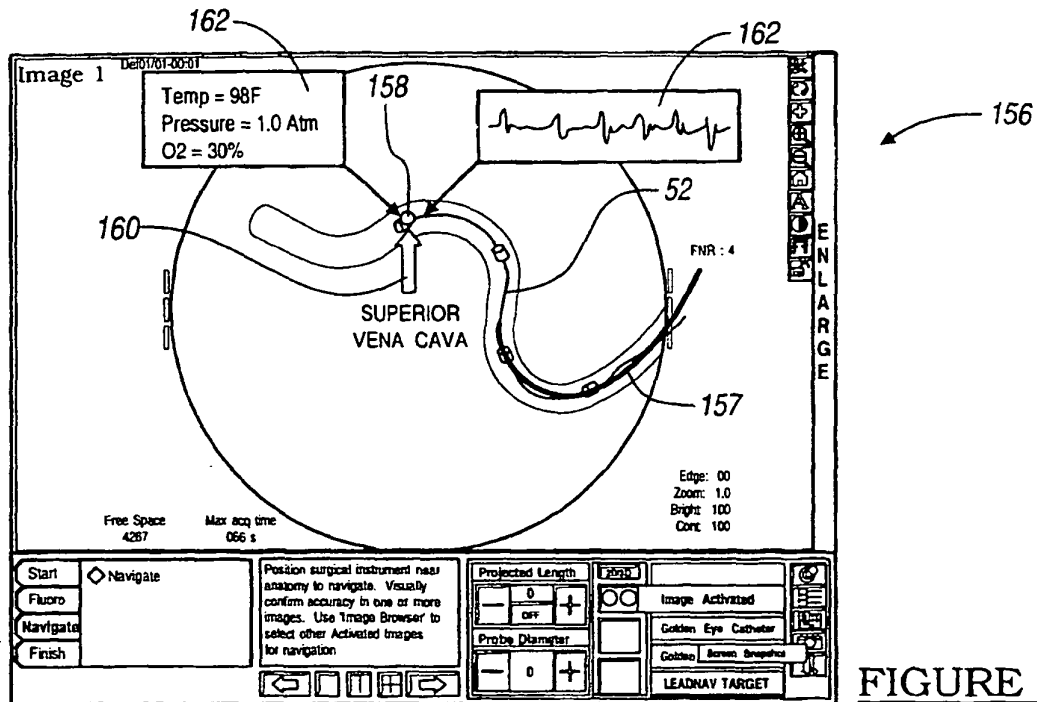


FIGURE 7

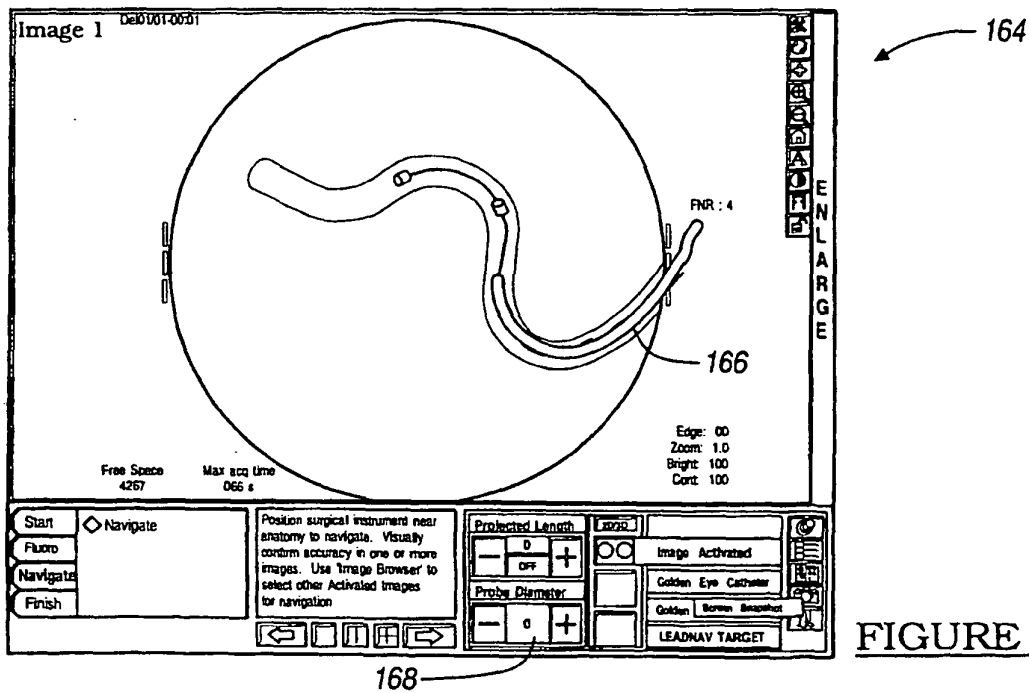


FIGURE 8

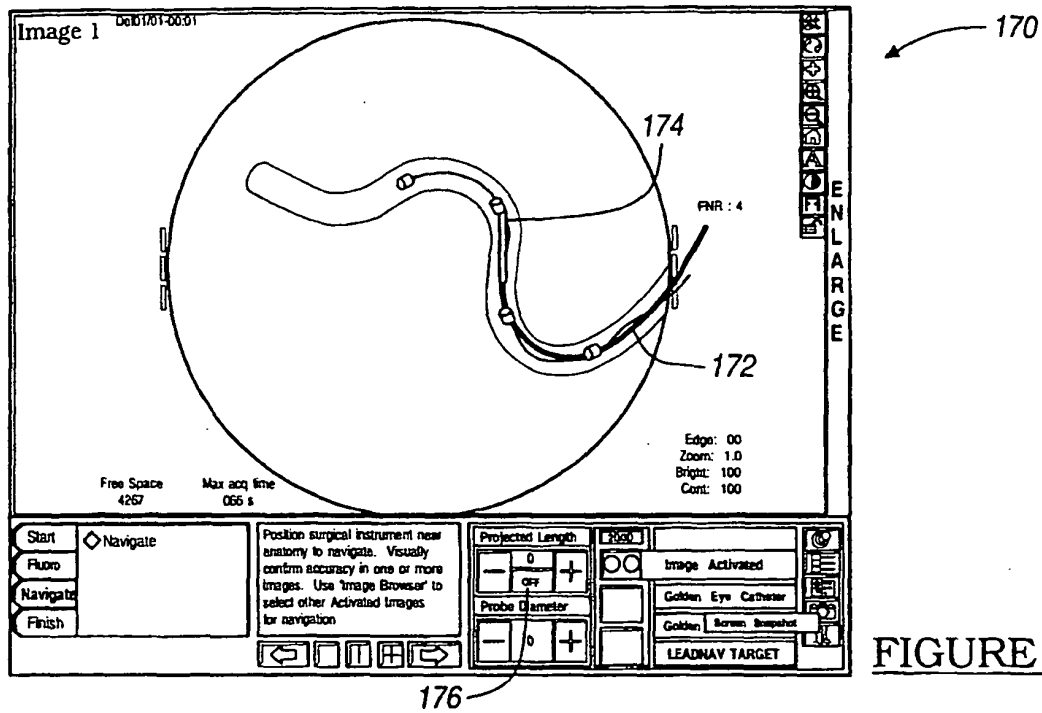


FIGURE 9

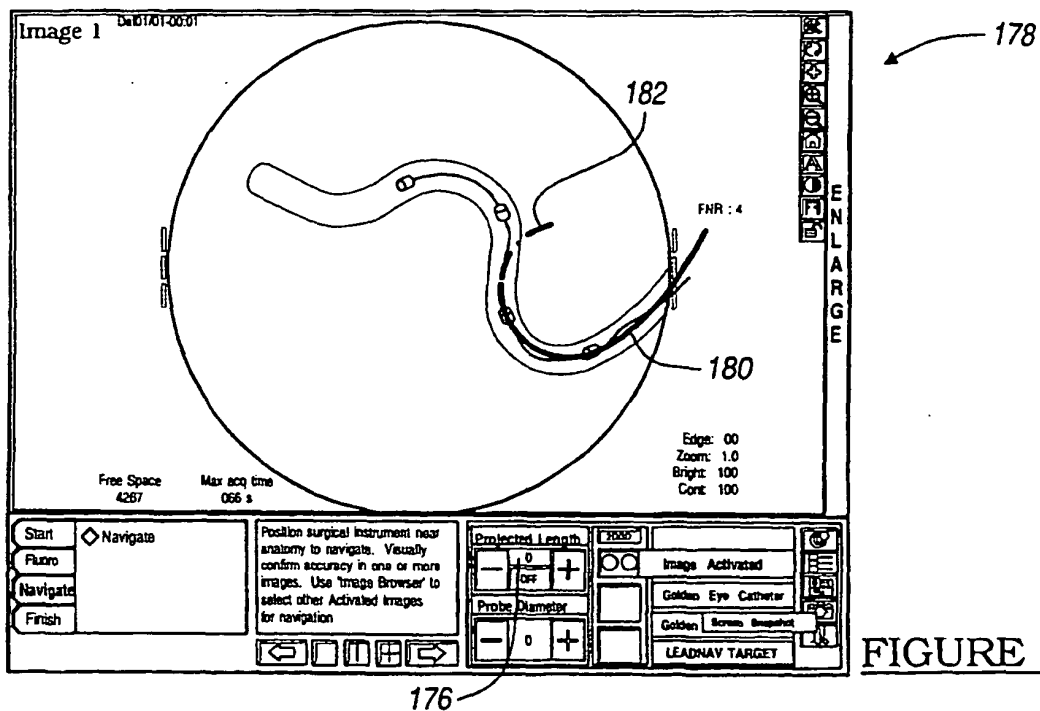


FIGURE 10

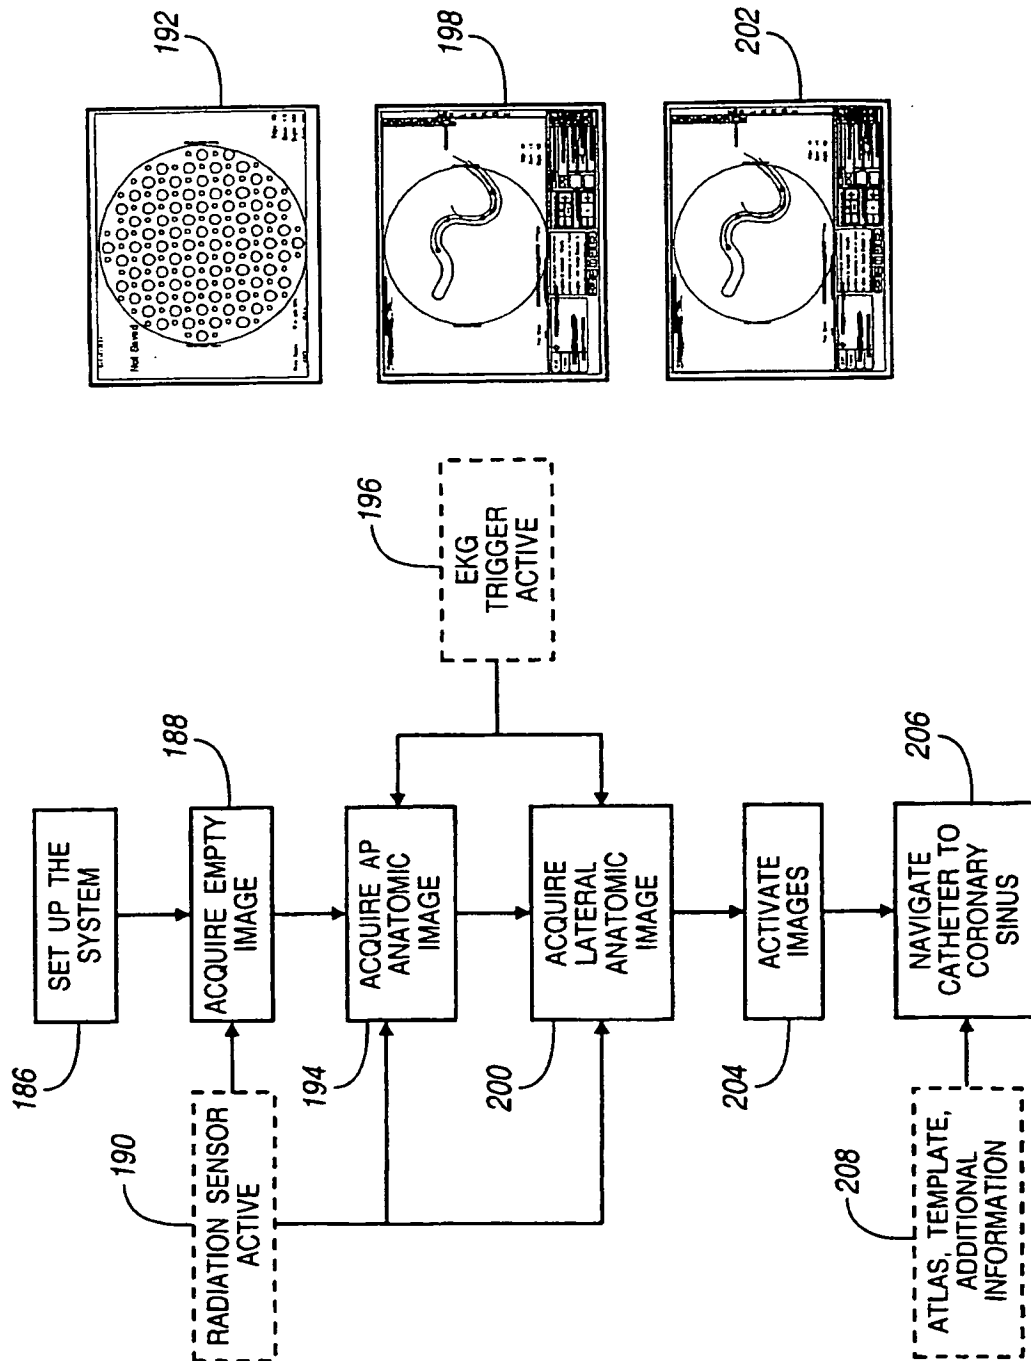


FIGURE 11

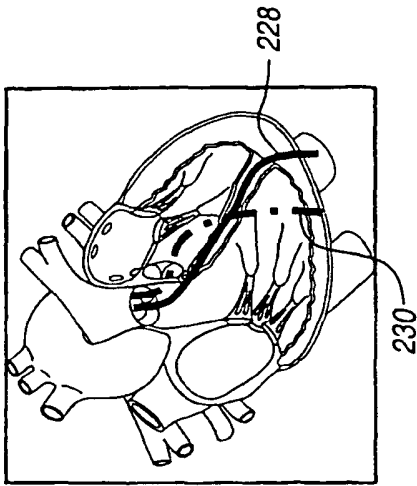


FIGURE 14A

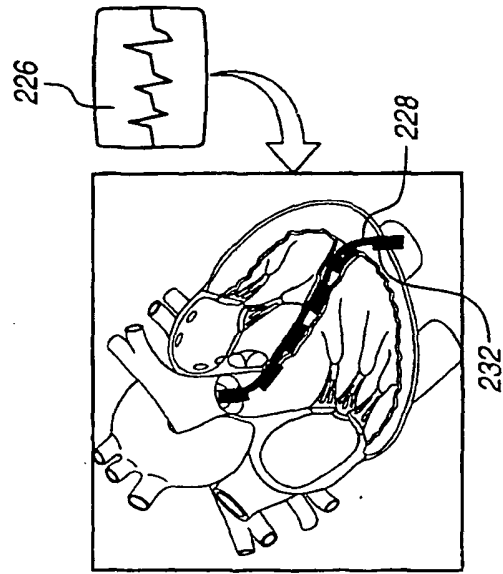


FIGURE 14B

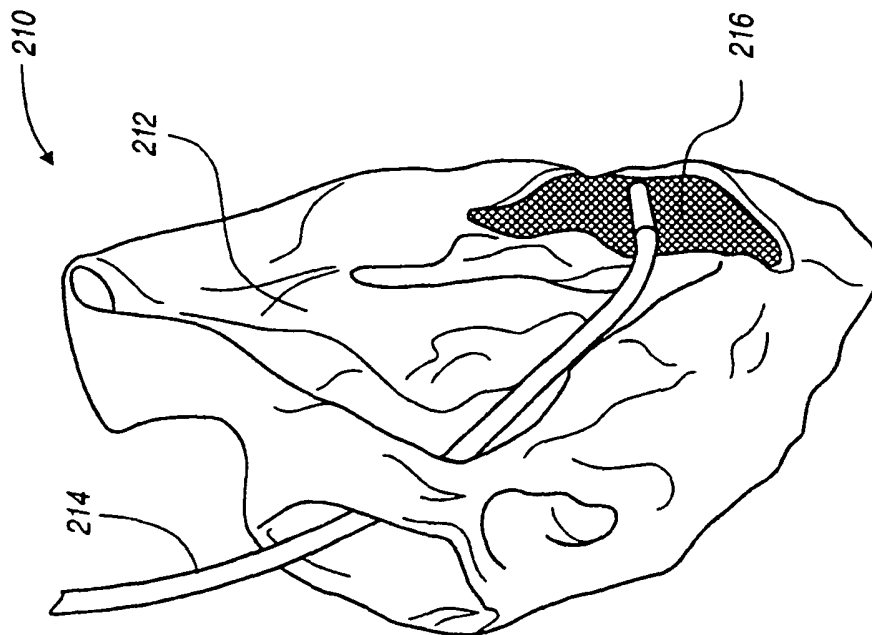


FIGURE 12

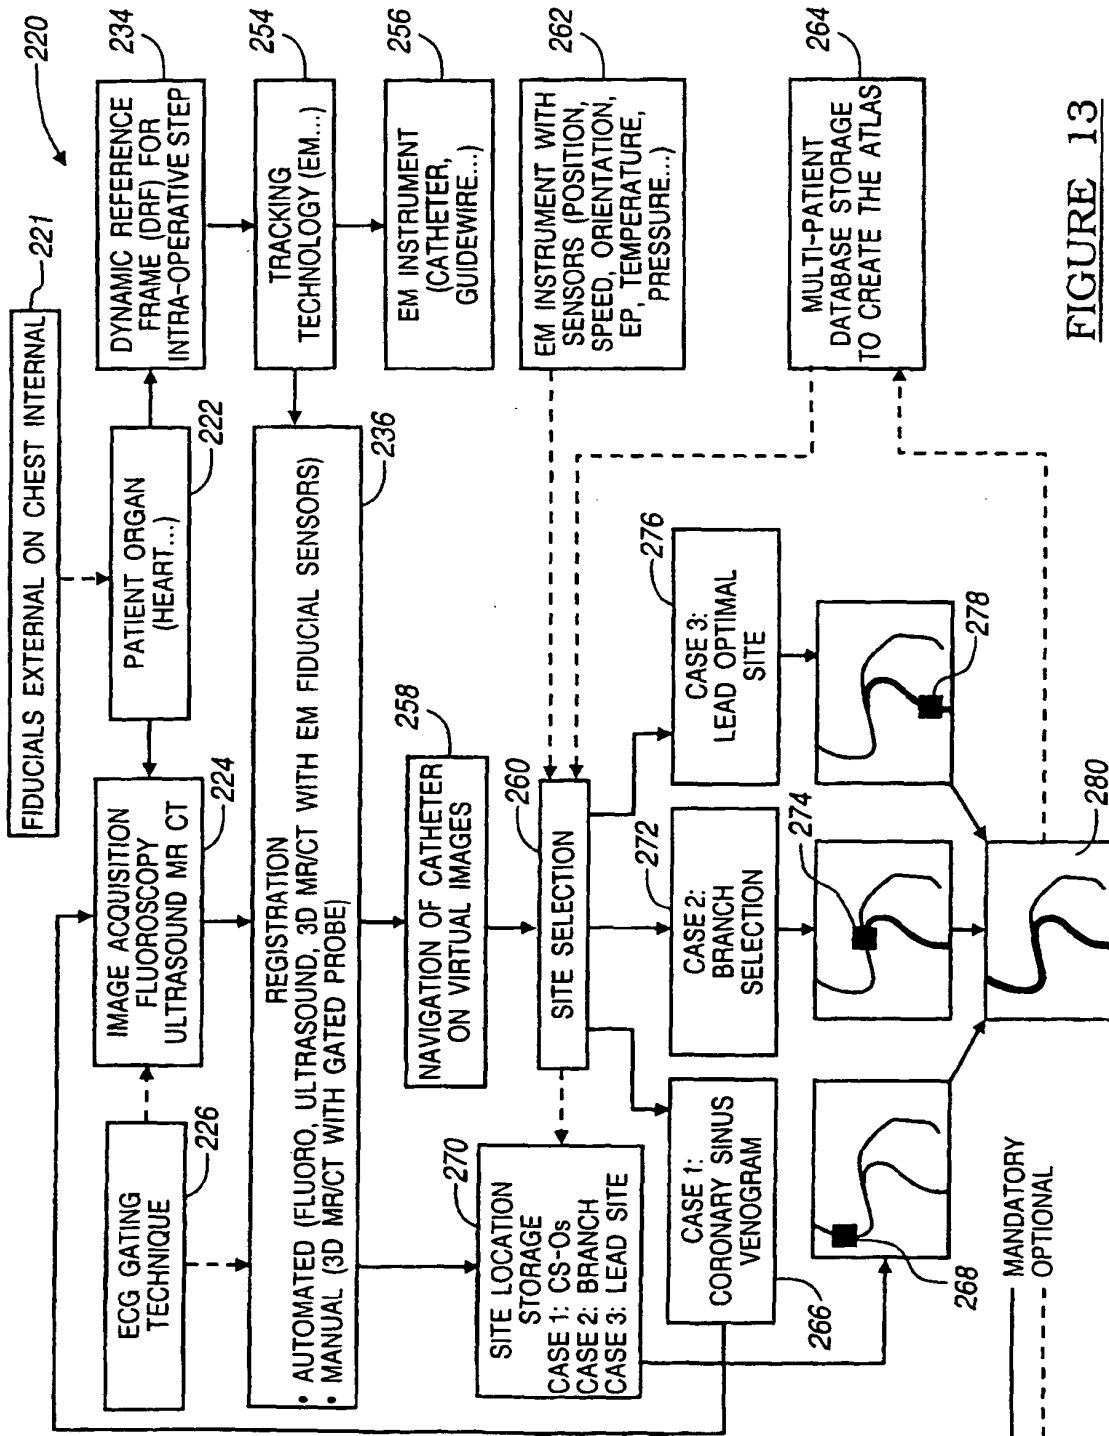


FIGURE 13

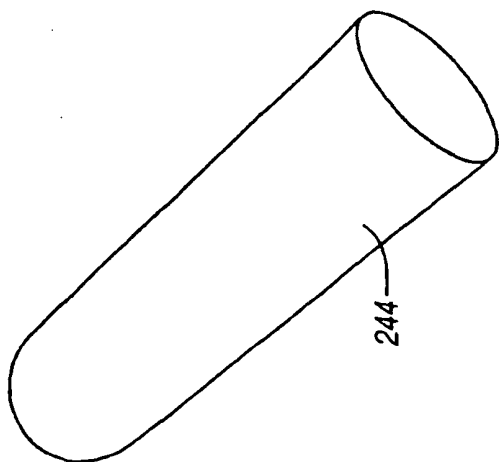


FIGURE 15C

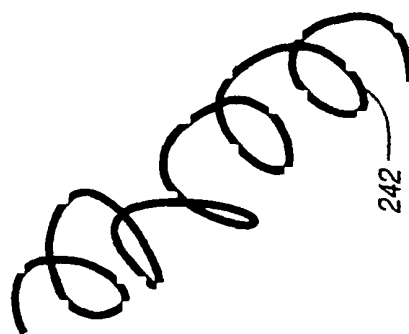


FIGURE 15B

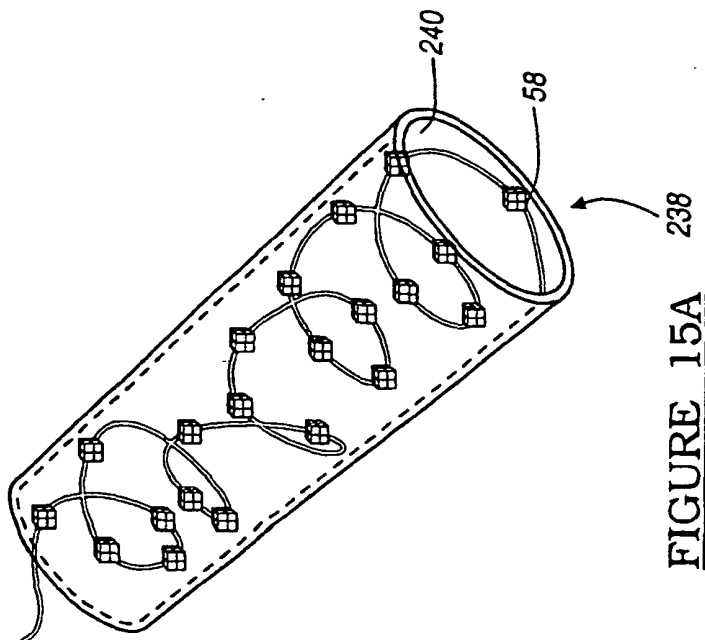


FIGURE 15A

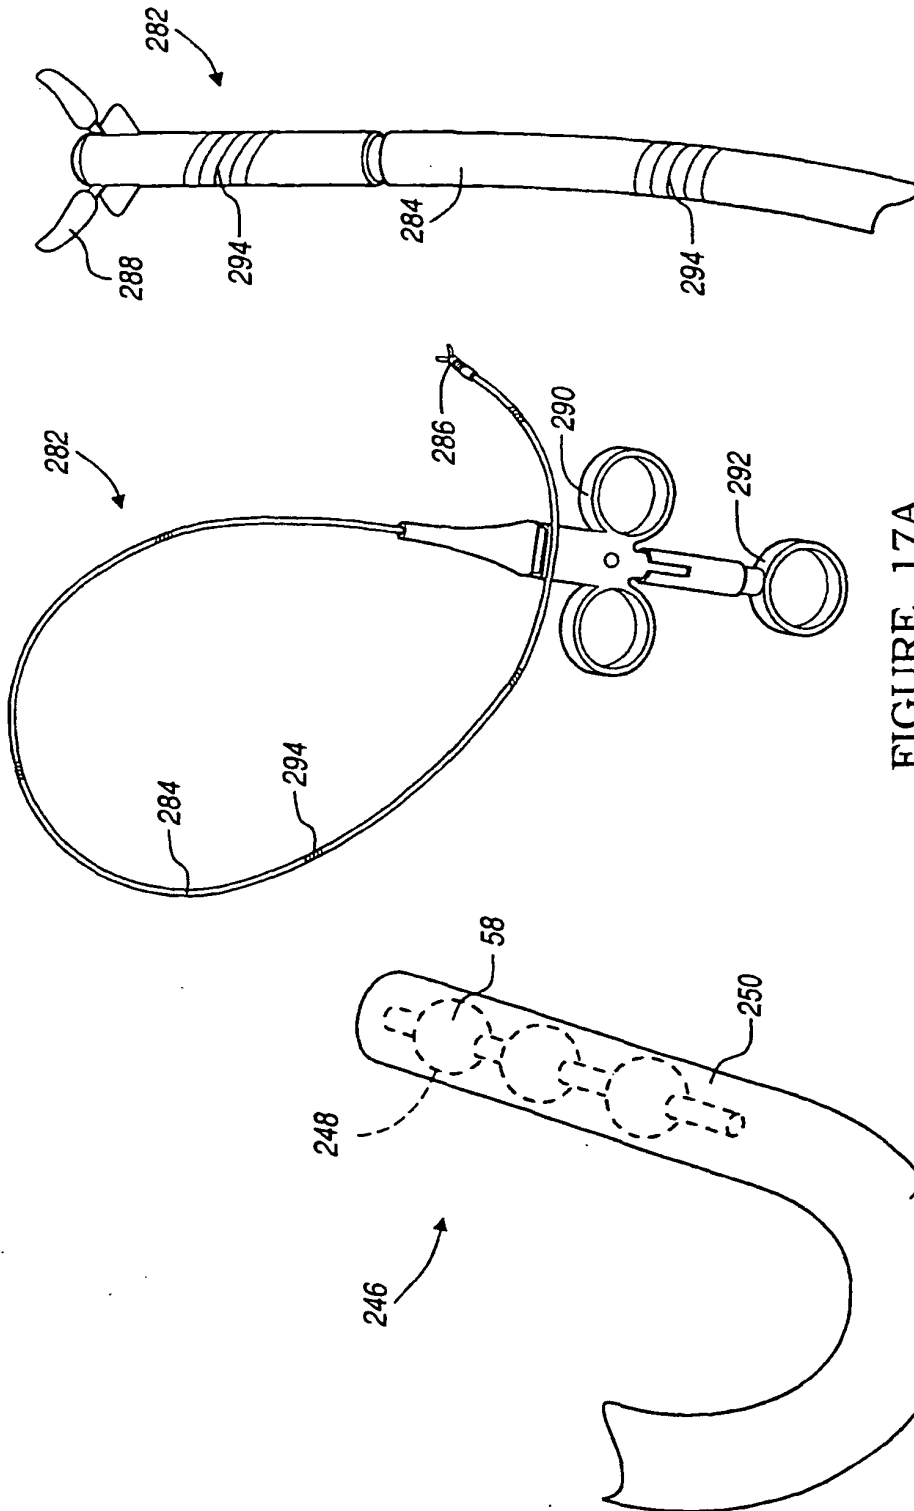


FIGURE 17B

FIGURE 17A

FIGURE 16

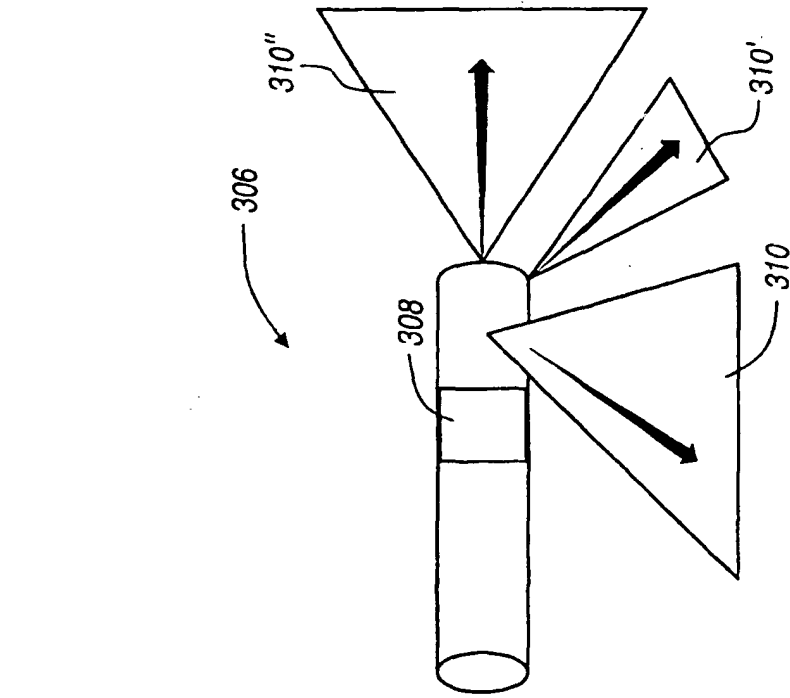


FIGURE 18A
(PRIOR ART)

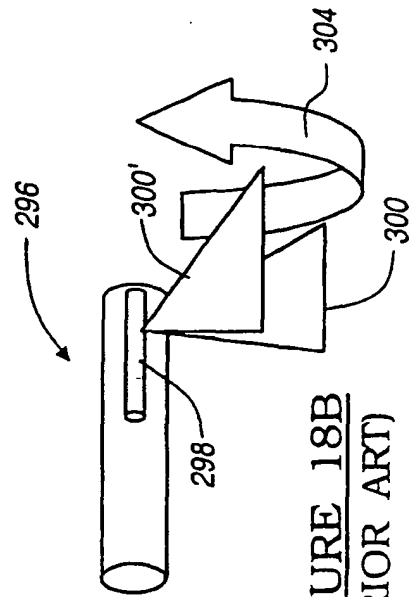


FIGURE 18B
(PRIOR ART)

FIGURE 19

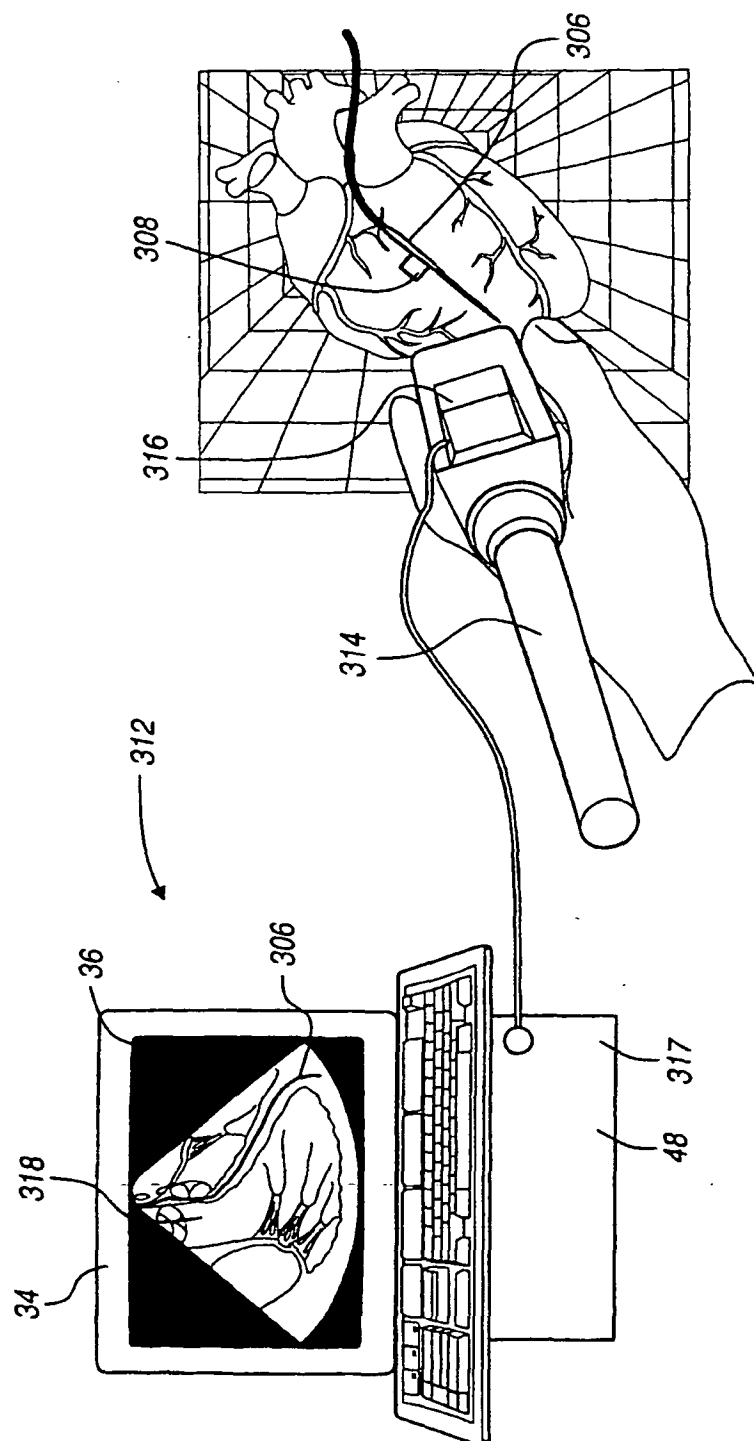


FIGURE 20

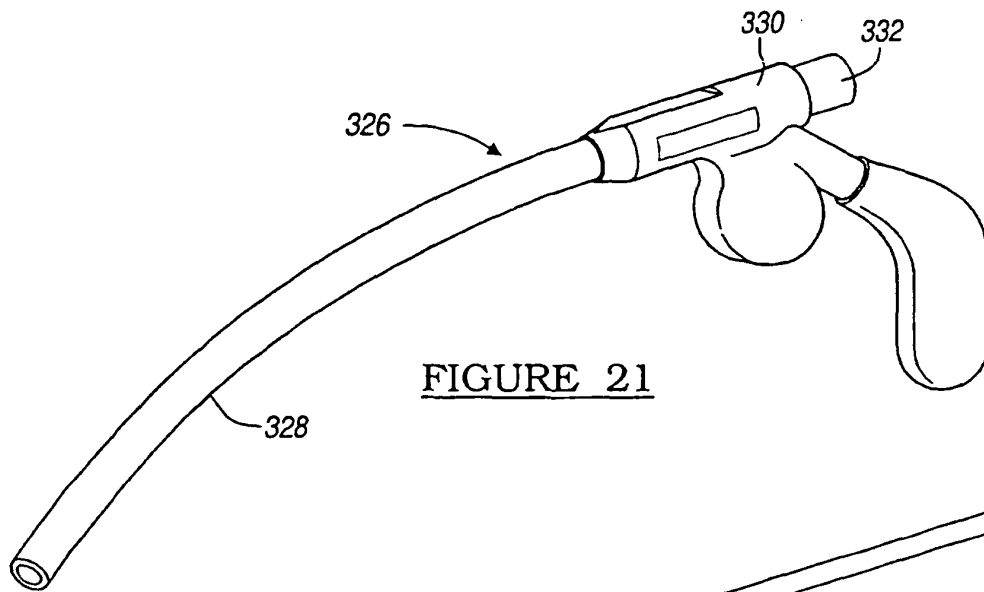


FIGURE 21

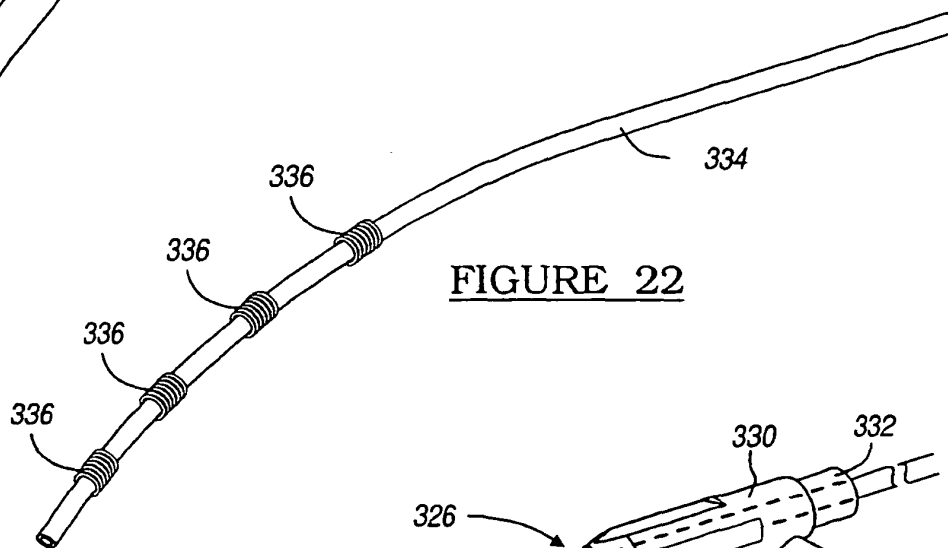


FIGURE 22

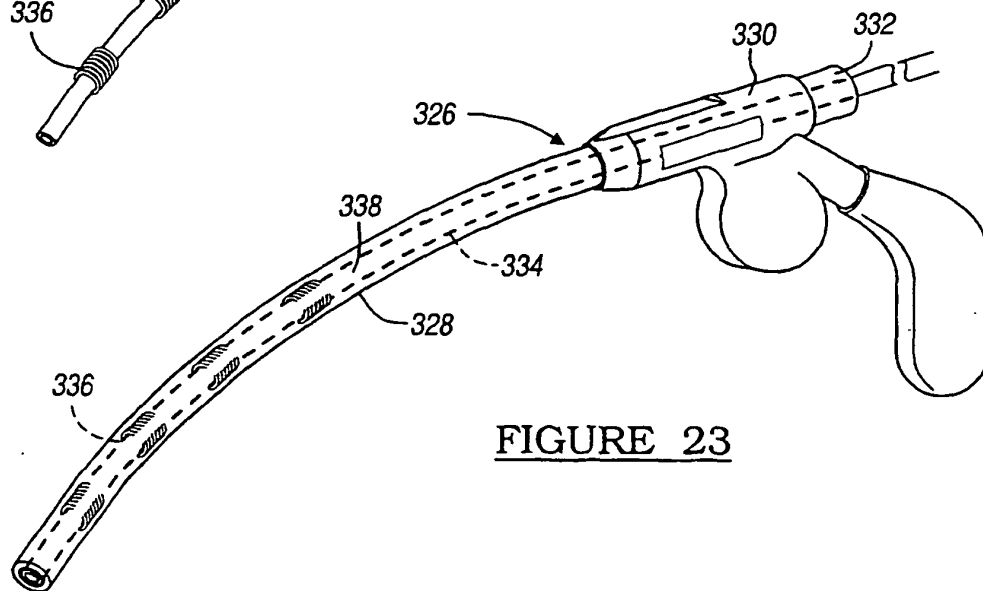


FIGURE 23

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6470207 B [0004]
- US 6192280 B [0007]
- US 5935160 A [0007]
- WO 02064011 A [0012]
- US 6118845 A [0049]
- US 5740808 A [0050]
- US 5913820 A [0058]
- US 5592939 A [0058]
- US 5983126 A [0061]
- US 6381485 B [0063] [0107]
- US 60465615 B [0069]
- US 10299484 B [0077]

Non-patent literature cited in the description

- **B. SCHUELE et al.** Correction of Image Intensifier Distortion for Three-Dimensional Reconstruction. *SPIE Medical Imaging*, 1995 [0049]
- **G. CHAMPLEBOUX et al.** Accurate Calibration of Cameras and Range Imaging Sensors: the NPBS Method. *Proceedings of the IEEE International Conference on Robotics and Automation*, May 1992 [0049]

专利名称(译)	用于心脏治疗的导航系统		
公开(公告)号	EP1504713B1	公开(公告)日	2008-07-30
申请号	EP2004016056	申请日	2004-07-08
[标]申请(专利权)人(译)	手术导航TECH		
申请(专利权)人(译)	手术导航TECHNOLOGIES, INC.		
当前申请(专利权)人(译)	手术导航TECHNOLOGIES, INC.		
[标]发明人	VERARD LAURENT HUNTER MARK W BZOSTEK ANDREW		
发明人	VERARD, LAURENT HUNTER, MARK W. BZOSTEK, ANDREW		
IPC分类号	A61B5/00 A61B5/055 G21K1/12 A61B5/05 A61B6/00 A61B1/005 A61B1/012 A61B5/0215 A61B5/06 A61B6/12 A61B17/00 A61B17/34 A61B19/00		
CPC分类号	A61B6/12 A61B1/00071 A61B1/0058 A61B1/012 A61B5/0215 A61B5/062 A61B5/068 A61B5/413 A61B5/7285 A61B5/743 A61B6/463 A61B6/507 A61B6/541 A61B8/4254 A61B10/06 A61B17/3478 A61B34/20 A61B34/25 A61B2017/00243 A61B2017/00247 A61B2018/00392 A61B2034/104 A61B2034/105 A61B2034/107 A61B2034/2051 A61B2034/2072 A61B2034/252 A61B2034/254 A61B2034/256 A61B2090/365 A61B2090/367 A61B2090/376 A61B2090/378		
优先权	10/619216 2003-07-14 US		
其他公开文献	EP1504713A1		
外部链接	Espacenet		

摘要(译)

用于导航患者区域的图像引导导航系统包括成像装置，跟踪装置，控制器和显示器。成像装置生成患者区域的图像。跟踪设备跟踪器械在患者区域中的位置。控制器基于仪器的位置将代表仪器的图标叠加到从成像装置产生的图像上。显示屏显示叠加仪器的图像。图像和登记过程可以与生理事件同步。控制器还可以提供并自动识别优化的站点以导航仪器。

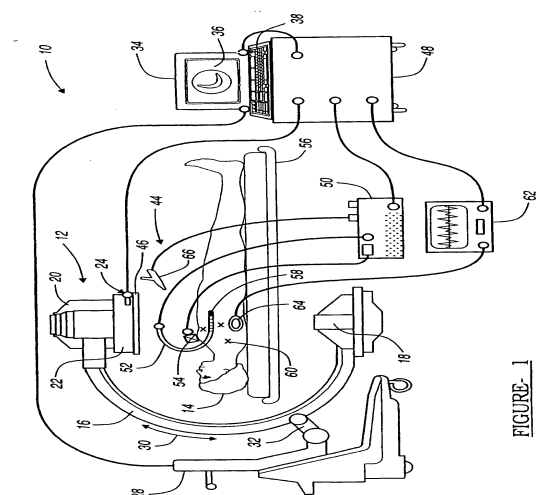


FIGURE 1