



(11) **EP 2 074 418 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
06.03.2013 Bulletin 2013/10

(51) Int Cl.:
G01N 29/24 (2006.01) **A61B 5/00** (2006.01)
G01N 21/17 (2006.01) **G01N 21/47** (2006.01)

(21) Application number: **07826422.3**

(86) International application number:
PCT/IB2007/053763

(22) Date of filing: **18.09.2007**

(87) International publication number:
WO 2008/038182 (03.04.2008 Gazette 2008/14)

(54) **Ultrasonic determination of optical absorption coefficients**

Bestimmung von optischen Absorptionskoeffizienten mittels Ultraschall

Détermination ultrasonore de coefficients d'absorption optiques

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR

(30) Priority: **29.09.2006 EP 06121524**

(43) Date of publication of application:
01.07.2009 Bulletin 2009/27

(73) Proprietor: **Koninklijke Philips Electronics N.V. 5621 BA Eindhoven (NL)**

(72) Inventors:
• **SAVERY, David NL-5656 AE Eindhoven (NL)**
• **JANKOVIC, Ladislav NL-5656 AE Eindhoven (NL)**
• **ANAND, Ajay NL-5656 AE Eindhoven (NL)**

(74) Representative: **Van Velzen, Maaïke Mathilde Philips Intellectual Property & Standards P.O. Box 220 5600 AE Eindhoven (NL)**

(56) References cited:
WO-A-2004/086965 US-A1- 2005 085 725

- **IRINA V LARINA ET AL: "Real-time optoacoustic monitoring of temperature in tissues; Optoacoustic monitoring of temperature in tissues" JOURNAL OF PHYSICS D. APPLIED PHYSICS, INSTITUTE OF PHYSICS PUBLISHING, BRISTOL, GB, vol. 38, no. 15, 7 August 2005 (2005-08-07), pages 2633-2639, XP020083247 ISSN: 0022-3727**
- **ANAND A ET AL: "Ultrasonic determination of three-dimensional spatial and temporal thermal distribution for therapy monitoring" 2006 IEEE INTERNATIONAL CONFERENCE ON ACOUSTICS, SPEECH, AND SIGNAL PROCESSING 14-19 MAY 2006 TOULOUSE, FRANCE, 19 May 2006 (2006-05-19), pages II-1108-II-1111, XP002472118 2006 IEEE International Conference on Acoustics, Speech, and Signal Processing (IEEE Cat. No. 06CH37812C) IEEE Piscataway, NJ, USA ISBN: 1-4244-0469-X**

EP 2 074 418 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The invention relates to a method, a record carrier, and an examination apparatus for the determination of an optical coefficient, particularly the optical absorption coefficient, at least one measuring location in an object.

[0002] The optical absorption and scattering properties of an object comprise valuable information about the material of the object and its chemical composition. In biological tissue, they allow for example to determine functional structures as well as pathophysiological states and regions. Several methods have therefore been proposed to measure the optical absorption coefficient (OAC) inside an object (cf. B.C. Wilson et. al.; "Indirect versus direct techniques for the measurement of the optical properties of tissues", *Photocem Photobiol.*, 46, 601-608 (1987); A.A. Oraevsky et. al., "Measurement of tissue optical properties by time-resolved detection of laser-induced transient stress", *Appl. Opt.* 36, 402 (1997)).

[0003] Furthermore, the US 2005/085725 A1 discloses various procedures to determine the concentration of glucose in a bolus of blood. In one of these procedures, the position of the bolus is first determined with an ultrasonic transducer, and the bolus is then irradiated with light pulses and simultaneously with a modulated ultrasonic beam. Absorption of the light induces a temperature increase which in turn changes the transit times of the ultrasonic waves. From measurements of these transit time changes, the light absorption coefficient at the bolus can be determined.

[0004] The WO 2004/086965 A relates to an apparatus in which a vessel section is irradiated with light of different wavelengths to determine different target analytes. The apparatus detects photoacoustic waves generated in the sample by the incident light intensity.

[0005] Moreover, it has been described in literature to irradiate a sample with a laser to generate photoacoustic waves which are detected by acoustic transducers (IRINA V LARINA ET AL: "Real-time optoacoustic monitoring of temperature in tissues; Optoacoustic monitoring of temperature in tissues" *JOURNAL OF PHYSICS D. APPLIED PHYSICS*, INSTITUTE OF PHYSICS PUBLISHING, BRISTOL, GB, vol. 38, no. 15, 7 August 2005, pages 2633-2639). This procedure shall be used to determine the temperature distribution in tissue during thermal therapy.

[0006] Finally, the generation of a three-dimensional temperature map in a sample from measurements of the variation of the speed of ultrasound has been reported (ANAND A ET AL: "Ultrasonic determination of three-dimensional spatial and temporal thermal distribution for therapy monitoring" 2006 IEEE INTERNATIONAL CONFERENCE ON ACOUSTICS, SPEECH, AND SIGNAL PROCESSING 14-19 MAY 2006 TOULOUSE, FRANCE, 19 May 2006, pages II-1108-II-1111).

[0007] Each of the mentioned technologies has however specific drawbacks which limit its use in practice.

[0008] Based on this background it was an object of

the present invention to provide means for the reliable determination of at least one characteristic optical coefficient in an object, particularly of the OAC in biological tissue.

5 **[0009]** This object is achieved by an examination apparatus according to claim 1, a method according to claim 6, and a record carrier according to claim 8. Preferred embodiments are disclosed in the dependent claims.

10 **[0010]** The examination apparatus according to the present invention serves for the determination of an optical coefficient, for example of the optical absorption coefficient (OAC) and/or the optical scattering coefficient, at at least one location in an object, wherein said location is called "measuring location" in the following. The apparatus comprises the following components:

- 15 - A light source for selectively sending a heating light beam to the measuring location, wherein the term "heating" shall indicate that the light beam induces a temperature increase when it is absorbed by the object. The light source may particularly comprise a laser that allows to generate beams of definite spectral composition and intensity with minimal divergence.
- 20 - An ultrasonic scanner for measuring the pulse echoes of ultrasonic pulses which were sent to the measuring location. As is well known to persons skilled in the art, the ultrasonic scanner typically comprises an ultrasound (US) generator for generating US pulses and an US receiver for recording pulse echoes, i.e. the reflections of ultrasonic pulses from structures inside the object. Typically, the US generator and the US receiver are realized by one transducer operating sequentially as generator and receiver.
- 25 - An "evaluation unit" for determining the optical coefficient of interest at the measuring location from first and second pulse echoes that were measured before and after a heating light beam was sent to the measuring location, respectively. The evaluation unit is typically realized by a microcomputer with dedicated hardware and/or software. It should be noted that the heating light beam may for example be followed by a period of no light emission during which the second pulse echoes are measured, or that it may for example be continued by a further light beam (particularly with same properties as the heating light beam) which prevails during the measurement of the second pulse echoes.

30 **[0011]** The examination apparatus allows to determine optical properties of a material with the help of an ultrasonic scanner, wherein the linkage between optical properties and ultrasonic measurement is the generation of heat due to the absorption of light. In particular, this mechanism comprises that the heating light beam will cause a temperature increase in the investigated object that is related to the optical properties of the material, particularly the -OAC. This temperature increase will in turn in-

duce changes in the speed of sound in the material which can be detected by the ultrasonic pulse echoes. An advantage of the apparatus resides in the fact that it uses a different physical quality, i.e. (ultra-)sound, that does not directly depend on the optical properties to be measured.

[0012] According to the invention, the evaluation unit further comprises a "temperature mapping module" for determining a spatial map of the temperature increase induced in the object by the heating light beam. A "spatial map" shall by definition refer to a mathematical mapping of a plurality of spatial locations to associated data (e.g. temperature values), wherein said spatial locations may particularly lie on a line or in a two-dimensional area. Preferably the spatial map comprises the complete path of the heating light beam inside the object.

[0013] The evaluation unit further comprises a "scatter mapping module" for estimating a map of the effective optical scattering properties in the object. The "effective optical scattering properties" typically summarize effects of absorption and scattering of light in the object and therefore determine how much of an incident light beam intensity will reach a target location inside the object. The scatter mapping module is preferably combined with the aforementioned temperature mapping module as the effective optical scattering properties can be inferred from the light-induced temperature increase (e.g. by comparing the temperature increases of adjacent locations with the same optical properties that are successively reached by the heating light beam).

[0014] Moreover, the evaluation unit comprises an "intensity estimation module" for determining the light intensity of the heating light beam at the measuring location. Preferably, said module is further designed such that it allows to determine this intensity not only a one location, but everywhere on the path of the heating light beam through the object. The intensity estimation module is preferably combined with the aforementioned scatter mapping module, as the knowledge of the effective optical scattering properties on the path of the heating light beam can be used to derive the light intensity at each point. It should be noted that, once the light intensity and the temperature increase at the measuring location are known, the optical absorption coefficient there can readily be estimated.

[0015] The light emitted by the light source may in principle have any spectral composition. Preferably, the heating light beam emitted by the light source comprises however only light of a given spectral composition, for example monochromatic light that is more or less sharply centered around one particular wavelength. In this case it is possible to investigate the spectral dependency of the optical coefficient of interest and/or to focus on effects that are known to appear at specific wavelengths only.

[0016] In the most general setup, the heating light beam and the ultrasonic pulses may be radiated into the object in completely different, independent directions. Preferably, the light source and the ultrasonic scanner

are however arranged such that they have parallel emission directions, i.e. that the heating light beam and the ultrasonic pulses travel in the same direction. In this case the measurements of the ultrasonic scanner will immediately reflect the conditions along the path of light propagation which simplifies the calculation of the optical coefficient of interest.

[0017] The examination apparatus may further comprise an injection device for injecting a contrast agent with specific light absorbing properties into the object. The injection device may for example comprise a syringe with associated equipment for a definite delivery of contrast agent into the vessel system of a patient. The location of the contrast agent inside the object can then be determined due to its specific optical properties, which allows to identify anatomical structures and/or specific (pathological or healthy) tissue components.

[0018] The invention further relates to a method for the determination of an optical coefficient at at least one measuring location in an object, wherein the method comprises the following steps:

- Measuring first pulse echoes of ultrasonic pulses sent to the measuring location.
- Sending a heating light beam to the measuring location.
- Measuring second pulse echoes of ultrasonic pulses sent to the measuring location after the heating light beam has been sent.
- Determining the optical coefficient of interest from the first and the second pulse echoes.

[0019] The method comprises in general form the steps that can be executed with an examination apparatus of the kind described above. Therefore, reference is made to the preceding description for more information on the details, advantages and improvements of that method.

[0020] In a preferred embodiment of the method, the optical coefficient of interest is determined at a plurality of locations inside the object, thus yielding a more or less densely sampled (one-, two- or three-dimensional) spatial map.

[0021] According to the method, a map of the temperature increase induced by the heating light beam inside the object is determined from the first and second pulse echoes. This temperature increase is directly proportional to the optical absorption coefficient and the light intensity at the considered location.

[0022] Furthermore, the intensity of the heating light beam is determined at least at the measuring location from the map of temperature increase. Knowing the light intensity that reached the measuring location allows to infer the optical absorption coefficient from the measured temperature increase. The determination of the light intensity at the measuring location may particularly comprise the determination of the effective optical scattering properties on the path of the heating light beam, which

can in turn be deduced from a comparison of the temperature increases in small regions with approximately constant optical properties.

[0023] Finally, the invention comprises a record carrier, for example a floppy disk, a hard disk, or a compact disc (CD), on which a computer program for the determination of an optical coefficient at at least one measuring location in an object is stored, wherein said program is adapted to execute a method of the aforementioned kind.

[0024] These and other aspects of the invention will be apparent from and elucidated with reference to the embodiment(s) described hereinafter. These embodiments will be described by way of example with the help of the accompanying drawings in which:

Figure 1 shows a principle sketch of an examination apparatus according to the present invention comprising a laser light source, an ultrasonic scanner, and an evaluation unit;

Figure 2 summarizes mathematical expressions relating to the measurement principle;

Figure 3 is a flow diagram of a typical examination procedure for the determination of the optical absorption coefficient in an object;

Figure 4 shows an exemplary pulse-echo waveform in an overview (top left) and in three enlarged windows;

Figure 5 shows the phase-shift in dependence on the depth inside an object determined from the data of Figure 4.

[0025] Like reference numbers in the Figures refer to identical or similar components.

[0026] When an optical wave propagates through tissue, it gets both attenuated and scattered. Attenuation, scattering and anisotropy define tissue properties within the diffusion approximation of the radiation transport concept, which describes light propagation under strong scattering conditions. The associated absorption and scattering coefficients are illumination wavelength dependent. Typical optical absorption coefficients (OAC) of a biological tissue for wavelengths in visible and near infrared (NIR) is $2\text{-}11\text{ cm}^{-1}$ for muscles, $1\text{-}5\text{ cm}^{-1}$ for blood and around 40 cm^{-1} for epidermis. The scattering coefficient is around 140 cm^{-1} for epidermis and $200\text{-}500\text{ cm}^{-1}$ for muscles. The OAC is known to give information not only about the nature of tissues, but also about their pathophysiological state (e.g. hemoglobin oxygen saturation, glucose level ($\lambda = 488\text{ nm}$)). Furthermore, as the wavelength-dependence of the OAC gives a very specific signature of the chemical components present in a medium, a mapping method to image the OAC of biological media could be of major interest for functional imaging. Moreover, with disease-specific optical agents to be injected in blood that absorb particularly specific wavelengths, the OAC of pathological regions can also have an enhanced contrast with respect to the background

OAC by using those compounds, enabling imaging in depth. For these reasons, a reliable and feasible method for the measurement of the OAC in an object is highly desirable.

[0027] When light, particularly laser light, shall be used to investigate the properties of living tissue, safety regulations have to be observed that dictate maximum allowed laser intensity at a given wavelength. A typical limit is 20 mJ/cm^2 per pulse (for ultra-short lasers) or 0.2 W/cm^2 for continuous wave (CW) at 532 nm laser wavelength, for instance, and it increases in the infrared wavelength regime reaching 40 mJ/cm^2 (per pulse) or 0.4 W/cm^2 (CW) at 1064 nm . It should however be noted that the safe use of significantly higher intensities (e.g. two orders of magnitude higher) has been demonstrated for certain applications. The aforementioned figures shall therefore not exclude the use of higher intensities in connection with the present invention.

[0028] The aforementioned (allowed) levels of light energy result in a heat deposition of typically a fraction of a Joule per cm^3 , and a temperature increase of a fraction of one Kelvin to a few Kelvin in an investigated tissue. The heat then gradually diffuses from the laser-absorbing thermal sources to the surrounding tissue. Regarding this light-induced temperature increase, it is known that the speed of sound, v , in biological tissue (with high water content) increases with temperature for temperature rises ΔT on the order of $10\text{-}15\text{ K}$ above normal body temperature ($37\text{ }^\circ\text{C}$). For small increases from the normal body temperature ($\Delta T < 10\text{ K}$), the dependence is nearly linear according to equation (1) of Figure 2, where $v_0 \approx 1540\text{ m/s}$ is the baseline speed of sound at normal body temperature and α_c is in the order of 0.1 \% K^{-1} . This acoustical feature has been used to map a temperature increase from a reference baseline using traditional pulse-echo ultrasonic imaging and elastography-inspired signal processing (cf. R. Seip, ES. Ebbini: "Non-invasive estimation of tissue temperature response to heating fields using diagnostic ultrasound", IEEE Transactions on Biomedical Engineering. Vol. 42, no.8, pp. 828-839, 1995).

[0029] Based on the above considerations, it is proposed here to use pulse-echo ultrasound (PEU) to image a laser-induced temperature increase, and to infer from that temperature increase the OAC inside an object of interest. Assuming that the relation between a map of temperature increase and the OAC distribution is linear in space and time (the laser intensity being supposed to be uniform), PEU has the potential to reconstruct images of the OAC that can bring much information for diagnostic purposes.

[0030] Figure 1 shows a principle sketch of an examination apparatus that realizes the proposed approach. The apparatus is used to investigate the optical properties of an object 1, for example a tissue region under the skin of a patient, wherein an x,y-coordinate system has been drawn for purposes of reference. For simplicity, the following considerations will be limited to a sectional

plane through the object, though they may easily be generalized to the three-dimensional case. The examination apparatus comprises the following components:

- A laser light source 10 for illuminating the object 1 with a heating light beam 11 propagating along the x-direction.
- An ultrasonic scanner 20 that emits ultrasonic pulses along a z-direction that can, in the most general case, be diagonal with respect to the x,y-coordinate system and in particular with respect to the direction of light propagation. The US scanner 20 typically comprises an US transducer that first emits an ultrasonic pulse and then records the echoes of this pulse which return from the object after characteristic traveling times (Figure 4 shows an exemplary pulse-echo waveform recorded by such an ultrasonic scanner).
- An evaluation unit 30, for example a workstation, to which the ultrasonic scanner 20 and optionally also the laser light source 10 are coupled. The evaluation unit 30 comprises several modules 31-34 which may be realized by dedicated hardware or, preferably, by suited routines of a computer program.
- A display unit 40, for example a computer monitor, for showing measurement results like a map of the determined optical absorption coefficient OAC.

[0031] In the following, the basic principles of the proposed measurement approach will be explained with reference to the mathematical expressions summarized in Figure 2. According to the radiation transport approach, and specifically the diffusion approximation, the intensity $I(x, y)$ of a heating light beam at some depth x within a tissue relates to the incidence intensity I_0 at the incidence surface as expressed in equation (2), where it is assumed that the complete spatio-temporal intensity $I^*(x, y, t)$ is a product of a spatial and temporal function and wherein a plane wave configuration is assumed for the spatial part. The effective scattering coefficient μ_{eff} is defined as in equation (3), wherein μ_a , μ_s and g are absorption, scattering and anisotropy coefficients, respectively, which are in equation (2) assumed to be constant. For a real tissue they vary spatially and depend on the light illumination wavelength.

[0032] The temporal dependence $f(t)$ of the light illumination can be assumed to be instantaneous if the light pulses are temporally much shorter than the temperature diffusion speed. Another extreme is continuous wave illumination, when the diffusion processes after some transition time stabilize and the configuration is in a steady state.

[0033] Only a part of an incident light beam with intensity $I(r)$ at a position $\underline{r} = (x, y)$ within the tissue (cf. Figure 1) is absorbed, wherein the absorbed energy density q_{laser} is proportional to the optical absorption coefficient (OAC) μ_a . Considering absorption and illumination spectral properties in addition to their spatial distribution, the absorbed energy q_{laser} is given by

equation (4), which is in the following approximated by equation (5). Due to the absorbed energy density q_{laser} , each absorption centre will behave as a heat source.

[0034] The temperature distribution $T(\underline{r}, t)$ resulting from these heat sources can be derived from the bioheat equation (6), where p is the density, c the specific heat, k the heat conductivity, q_{laser} the light absorption term and q_{pm} a term that contains effects from perfusion and metabolic activity. For short time scales, the last term q_{pm} does not play an important role and can be neglected. Solving this equation for the case of a single spherical absorbing particle positioned within a non-absorbing tissue gives the temperature distribution of equation (7), assuming that the time t is large enough so that there is an ongoing heat diffusion process.

[0035] For short heating times, smaller than the characteristic diffusion times of tissue (which are on the order of seconds), the heat transfer equation (6) can be simplified to equation (8), in which t_{laser} represents the time the laser was on and ΔT represents the induced temperature rise. Knowing the values of p and c for the tissue type under consideration (e.g. from F. Duck: "Physical Properties of Tissue: A Comprehensive Reference Work", Elsevier Science & Technology Books), the laser on-time t_{laser} , the laser intensity $I = I(r)$ at the measuring location \underline{r} , and the temperature rise ΔT (measured from ultrasonic data), the optical absorption coefficient μ_a can be obtained from equation (8). In the following, it will therefore be explained how the missing data can be determined, i.e. (i) the temperature rise ΔT and (ii) the laser intensity $I(r)$.

[0036] When a region of tissue is heated, the resulting temperature change ΔT results in variations in the speed of sound. As a result, the backscattered ultrasound echoes (at radio-frequency RF) from the heated region undergo time shifts, and these time shifts can be mapped into apparent displacements u assuming a nominal constant speed v_0 of sound throughout the medium (typically 1540 m/s). In the following, it will be assumed that the apparent displacements will only depend on the direction z of propagation of the ultrasound beam, i.e. $u = u(z)$. The time dt that an US pulse needs to travel from a location z to the location $z+dz$ (cf. Figure 1) is described by equation (9). This time dt is interpreted by the US receiver as being caused by a travel of the sound with a constant speed v_0 from a shifted location $z+u(z)$ to a shifted location $z+u(z)+dz+du$, see equation (10). Combining equations (9) and (10) yields equation (11), from which equation (12) can be derived with the help of equation (1). The dimensionless quantity $du(z)/dz$ is referred to as "temperature-induced strain" as it is the spatial gradient of an apparent displacement. This temperature-induced strain is measured from the ultrasound RF backscatter data in a way well-known to persons skilled in the art. Pulse echo speckle measurements can thus be used to obtain a temperature map $\Delta T(\underline{r})$ of the tissue.

[0037] In addition, the pulse echo provides the tissue geometry and structure. The tissue geometry/structure

and its temperature rise map $\Delta T(\underline{r})$ are further sufficient to create an optical absorption and scattering map. To this purpose, the ratio of temperature increases at two nearby locations $\underline{r}_A = (x_A, y_A)$, $\underline{r}_B = (x_B, y_B)$ is considered in equation (13), wherein it is assumed that the material coefficients μ_a , ρ , c are approximately the same at the two locations (e.g. if \underline{r}_A and \underline{r}_B are chosen from the same type of tissue). Thus the effective scattering coefficient μ_{eff} that appears in equation (2) can be derived from the measured temperature increases $\Delta T(\underline{r}_A)$, $\Delta T(\underline{r}_B)$ and the measured distance $(x_B - x_A)$. Repeating this procedure for the whole object yields a map $\mu_{\text{eff}}(\underline{r})$ of effective scattering coefficients.

[0038] In the next step, the intensity $I(\underline{r})$ of a heating light beam that arrives at a location \underline{r} can be determined by integration of a generalized equation (2) with the help of the now known effective scattering coefficients $\mu_{\text{eff}}(\underline{r})$.

[0039] Finally, the OAC μ_a at location \underline{r} can be directly calculated from equation (8) as now both ΔT and $I(\underline{r})$ are known.

[0040] The described basic steps of the optical absorption mapping procedure can readily be expanded to a multi-layer tissue case by repeating the basic procedure for different transducer positions. An especially simplistic case is when the laser illumination comes from the transducer side (i.e. light propagation is along the pulse-echo line z in Figure 1). Since the pulse-echo provides inherently depth information (and thus separation between the locations \underline{r}_A and \underline{r}_B considered above), it is not required to know the tissue geometry/structure to find OAC tissue map.

[0041] Figure 3 shows the flow diagram of a typical measurement procedure with the examination apparatus of Figure 1 based on the principles explained above. The procedure starts at step 101 with an optional injection of a photoactive substance as a contrast agent into the body volume of interest. The contrast agent may particularly be targeting some specific tissue inside a patient. Examples of possible contrast agents are indocyanine green (ICG) and nanoparticles.

[0042] In the next step 102, a first pulse-echo signal is recorded with the ultrasonic scanner 20, from which a body structure image can optionally be determined in step 105.

[0043] After recording of the first pulse echoes, the object is illuminated with a heating laser light beam of initial intensity I_0 for the pulse duration t_{laser} in step 103. The heating light beam will induce an associated temperature increase ΔT in the illuminated regions of the object. Immediately after the illumination, a second image of pulse echoes is recorded with the ultrasonic scanner 20 in step 104. This image is preferably generated with the same imaging parameters (position of scanner, frequency, viewing angle etc.) as the first pulse-echo image of step 102.

[0044] The temperature-induced strain du/dz that is found in the second pulse-echo image with respect to the first pulse-echo image is evaluated in step 106 ac-

cording to equation (12) to derive the local temperature increases $\Delta T(\underline{r})$. This step 106 is performed in a "temperature mapping module" 31 of the evaluation unit 30 shown in Figure 1.

[0045] In the next step 107, the temperature map $\Delta T(\underline{r})$ and optionally also the structural image obtained at step 105 is used to determine a map $\mu_{\text{eff}}(\underline{r})$ of effective scattering coefficients according to equation (13). This step 107 is performed in a "scatter mapping module" 32 of the evaluation unit 30.

[0046] Based on the map $\mu_{\text{eff}}(\underline{r})$ of effective scattering coefficients, the light intensity distribution $I(\underline{r})$ throughout the object can be determined in step 108 based on the given initial light intensity I_0 and the direction of the heating light beam according to equation (2). This step 108 is performed in an "intensity mapping module" 33 of the evaluation unit 30.

[0047] In a final step 109, the desired map $\mu_a(\underline{r})$ of the OAC is determined with the help of equation (8) from the intensity $I(\underline{r})$ and the temperature increase $\Delta T(\underline{r})$ previously obtained. This step is performed in an "OAC mapping module" 34 of the evaluation unit 30. Additionally or alternatively to the OAC, other optical coefficients like the scattering coefficient μ_s could be determined as well.

[0048] In summary, the described method for acquiring optical absorption coefficients from ultrasonic pulse-echo images comprises the following basic steps:

1) An ultrasonic pulse-echo image is acquired before and shortly after the light illumination exposure, wherein one pulse-echo line before and after illumination can be sufficient for obtaining the OACs along the line.

2) The temperature change is identified in at least two spatially separated points which belong to a tissue section sharing the same OAC.

3) The optical absorption coefficient is obtained from the temperature change ratio between the aforementioned points and their separation, combined with at least one of the temperature changes and its depth information. The minimum required separation of the relevant points is only determined by the temperature acquiring process resolution.

[0049] Figure 4 shows exemplary pulse-echo waveforms obtained from an ink doped agar gel phantom of block-shape immersed into water (vertical axis: relative units; horizontal axis: pulse traveling time t). The ink was uniformly dispersed during the phantom fabrication process. Pulsed, nanosecond Nd:YAG, laser was shined from a side of the phantom, providing uniform illumination along the ultrasonic pulse-echo acquisition line as the US transducer was aligned along an edge of the phantom perpendicular to the light direction (corresponding to an axis z perpendicular to the x -axis in Figure 1). In the shown captured echo from the phantom (top left diagram), two signals - before and after laser illumination - are strongly overlapped and can be resolved only after

zooming-in as shown in the graphs 1, 2 and 3. According to these graphs 1, 2 and 3, the after illumination signal has a phase (time) shift (corresponding to the apparent displacement u considered above). Since the phase shift is cumulative, the after the illumination signal overlaps the before the illumination signal in the window 1 (graph 1), and gradually separates from it at larger depths (windows 2 and 3). The laser illumination is uniform along the phantom surface, resulting in a uniform temperature change. Therefore the phase shift increases/decreases linearly. Figure 5 shows in this respect a nearly linear drop in phase shift Φ (vertical axis) along the length of the phantom (horizontal axis, measured by the pulse traveling time t). Using equation (12), this corresponds to a 2 K temperature increase (assuming $\alpha_c = 0.001$ for the phantom) in the phantom following application of the laser pulse. The slope of the curve, $d\Phi/dt = -\alpha_c \omega_0 \Delta T$ (with $\omega_0 = 2\pi \cdot 10$ MHz), indicates a temperature rise in the phantom on the order of 1.7 K for a heated zone of 2 cm.

[0050] Finally it is pointed out that in the present application the term "comprising" does not exclude other elements or steps, that "a" or "an" does not exclude a plurality, and that a single processor or other unit may fulfill the functions of several means. The invention resides in each and every novel characteristic feature and each and every combination of characteristic features. Moreover, reference signs in the claims shall not be construed as limiting their scope.

Claims

1. An examination apparatus for the determination of an optical coefficient (μ_a) at at least one measuring location (r) in an object (1), comprising

- a light source (10) for selectively sending a heating light beam (11) to the measuring location;
- an ultrasonic scanner (20) for measuring the pulse echoes of ultrasonic pulses sent to the measuring location;
- an evaluation unit (30) for determining the optical coefficient (μ_a) at the measuring location from pulse echoes that were measured before and after sending a heating light beam to the measuring location,

wherein said evaluation unit (30) comprises:

- a) a temperature mapping module (31) for determining a spatial map of the temperature increase ($\Delta T(r)$) induced in the object (1) by the heating light beam (11);
- b) a scatter mapping module (32) for estimating a spatial map of the effective optical scattering properties ($\mu_{\text{eff}}(r)$) in the object (1);
- c) an intensity estimation module (33) for deter-

mining the light intensity ($I(r)$) of the heating light beam (11) at the measuring location.

2. The examination apparatus according to claim 1, **characterized in that** the optical coefficient comprises the optical absorption coefficient (μ_a) and/or the optical scattering coefficient (μ_s).

3. The examination apparatus according to claim 1, **characterized in that** the heating light beam (11) comprises only light of a given spectral composition.

4. The examination apparatus according to claim 1, **characterized in that** the light source (10) and the ultrasonic scanner (20) have parallel radiation directions.

5. The examination apparatus according to claim 1, **characterized in that** it comprises an injection device for injecting a contrast agent with specific light absorbing properties into the object (1).

6. A method for the determination of an optical coefficient (μ_a) at at least one measuring location (r) in an object (1), comprising

- measuring first pulse echoes of ultrasonic pulses sent to the measuring location;
- sending a heating light beam (11) to the measuring location;
- measuring second pulse echoes of ultrasonic pulses sent to the measuring location;
- determining the optical coefficient from the first and second pulse echoes, wherein
- a map of the temperature increase ($\Delta T(r)$) inside the object (1) is determined from the first and second pulse echoes;
- a spatial map of the effective optical scattering properties ($\mu_{\text{eff}}(r)$) in the object (1) is estimated;
- the intensity ($I(r)$) of the heating light beam (11) at the measuring location (r) is determined from the map of temperature increase ($\Delta T(r)$).

7. The method according to claim 6, **characterized in that** the optical coefficient is determined at a plurality of locations inside the object (1).

8. A record carrier on which a computer program for the determination of an optical coefficient (μ_a) at at least one measuring location (r) in an object (1) is stored, said program being adapted to execute a method according to claim 6.

Patentansprüche

1. Untersuchungsgerät zur Bestimmung eines opti-

schen Koeffizienten (μ_a) an mindestens einem Messort (r) in einem Objekt (1), wobei das Untersuchungsgerät Folgendes umfasst:

- eine Lichtquelle (10) zum selektiven Senden eines erwärmenden Lichtbündels (11) an den Messort; 5
- einen Ultraschallscanner (20) zum Messen der Impulsechos von an den Messort gesandten Ultraschallimpulsen; 10
- eine Evaluierungseinheit (30) zum Ermitteln des optischen Koeffizienten (μ_a) an dem Messort anhand der Impulsechos, die vor und nach dem Senden eines erwärmenden Lichtbündels an den Messort gemessen wurden, 15

wobei die genannte Evaluierungseinheit (30) Folgendes umfasst:

- a) ein Temperaturmapping-Modul (31) zum Ermitteln einer räumlichen Karte des Temperaturanstiegs ($\Delta T(r)$), der durch das erwärmende Lichtbündel (11) in das Objekt (1) induziert wurde; 20
- b) ein Streuungsmapping-Modul (32) zum Schätzen einer räumlichen Karte der effektiven optischen Streuungseigenschaften ($\mu_{\text{eff}}(r)$) in dem Objekt (1); 25
- c) ein Intensitätsschätzungsmodul (33) zum Ermitteln der Lichtintensität ($I(r)$) des erwärmenden Lichtbündels (11) an dem Messort. 30

2. Untersuchungsgerät nach Anspruch 1, **dadurch gekennzeichnet, dass** der optische Koeffizient den optischen Absorptionskoeffizienten (μ_a) und/oder den optischen Streukoeffizienten (μ_s) umfasst. 35
3. Untersuchungsgerät nach Anspruch 1, **dadurch gekennzeichnet, dass** das erwärmende Lichtbündel (11) nur Licht einer bestimmten spektralen Zusammensetzung umfasst. 40
4. Untersuchungsgerät nach Anspruch 1, **dadurch gekennzeichnet, dass** die Lichtquelle (10) und der Ultraschallscanner (20) parallele Strahlungsrichtungen haben. 45
5. Untersuchungsgerät nach Anspruch 1, **dadurch gekennzeichnet, dass** es eine Injektionsvorrichtung zum Injizieren eines Kontrastmittels mit bestimmten lichtabsorbierenden Eigenschaften in das Objekt (1) umfasst. 50
6. Verfahren zur Bestimmung eines optischen Koeffizienten (μ_a) an mindestens einem Messort (r) in einem Objekt (1), wobei das Verfahren Folgendes umfasst: 55

- Messen von ersten Impulsechos von an den Messort gesandten Ultraschallimpulsen;
- Senden eines erwärmenden Lichtbündels (11) an den Messort;
- Messen von zweiten Impulsechos von an den Messort gesandten Ultraschallimpulsen;
- Ermitteln des optischen Koeffizienten anhand der ersten und zweiten Impulsechos, wobei
- eine Karte des Temperaturanstiegs ($\Delta T(r)$) innerhalb des Objekts (1) anhand der ersten und zweiten Impulsechos ermittelt wird;
- eine räumliche Karte der effektiven optischen Streuungseigenschaften ($\mu_{\text{eff}}(r)$) in dem Objekt (1) geschätzt wird;
- die Intensität ($I(r)$) des erwärmenden Lichtbündels (11) an dem Messort (r) anhand der Karte des Temperaturanstiegs ($\Delta T(r)$) ermittelt wird.

7. Verfahren nach Anspruch 6, **dadurch gekennzeichnet, dass** der optische Koeffizient an einer Vielzahl von Orten innerhalb des Objekts (1) ermittelt wird.
8. Aufzeichnungsträger, auf dem ein Computerprogramm zur Bestimmung eines optischen Koeffizienten (μ_a) an mindestens einem Messort (r) in einem Objekt (1) gespeichert ist, wobei das genannte Programm vorgesehen ist, um ein Verfahren nach Anspruch 6 auszuführen.

Revendications

1. Appareil d'examen pour la détermination d'un coefficient optique (μ_a) à au moins un emplacement de mesure (r) dans un objet (1), comprenant :
 - une source lumineuse (10) pour envoyer sélectivement un faisceau lumineux chauffant (11) à l'emplacement de mesure ;
 - un échographe (20) pour mesurer les impulsions-échos d'impulsions supersoniques envoyées à l'emplacement de mesure ;
 - une unité d'évaluation (30) pour déterminer le coefficient optique (μ_a) à l'emplacement de mesure à partir d'impulsions-échos qui ont été mesurées avant d'envoyer, et après avoir envoyé, un faisceau lumineux chauffant à l'emplacement de mesure,
 dans lequel ladite unité d'évaluation (30) comprend :
 - a) un module de cartographie de température (31) pour déterminer une carte spatiale de l'augmentation de température ($\Delta T(r)$) provoquée dans l'objet (1) par le faisceau lumineux chauffant (11) ;
 - b) un module de cartographie de diffusion (32)

- pour estimer une carte spatiale des propriétés de diffusion optique effective ($\mu_{\text{eff}}(r)$) dans l'objet (1) ;
- c) un module d'estimation d'intensité (33) pour déterminer l'intensité lumineuse ($I(r)$) du faisceau lumineux chauffant (11) à l'emplacement de mesure. 5
2. Appareil d'examen selon la revendication 1, **caractérisé en ce que** le coefficient optique comprend le coefficient d'absorption optique (μ_a) et/ou le coefficient de diffusion optique (μ_s). 10
3. Appareil d'examen selon la revendication 1, **caractérisé en ce que** le faisceau lumineux chauffant (11) comprend seulement de la lumière d'une composition spectrale donnée. 15
4. Appareil d'examen selon la revendication 1, **caractérisé en ce que** la source lumineuse (10) et l'échographe (20) possèdent des directions de rayonnement parallèles. 20
5. Appareil d'examen selon la revendication 1, **caractérisé en ce qu'il** comprend un dispositif d'injection pour injecter un agent de contraste avec des propriétés spécifiques d'absorption de lumière (1). 25
6. Procédé pour la détermination d'un coefficient optique (μ_a) à au moins un emplacement de mesure (r) dans un objet (1), comprenant : 30
- mesurer des premières impulsions-échos d'impulsions supersoniques envoyées à l'emplacement de mesure ; 35
 - envoyer un faisceau lumineux chauffant (11) à l'emplacement de mesure ;
 - mesurer des secondes impulsions-échos d'impulsions supersoniques envoyées à l'emplacement de mesure ; 40
 - déterminer le coefficient optique à partir des premières et secondes impulsions-échos, dans lequel
 - une carte de l'augmentation de température ($\Delta T(r)$) à l'intérieur de l'objet (1) est déterminée à partir des premières et secondes impulsions-échos ; 45
 - une carte spatiale des propriétés de diffusion optique effective ($\mu_{\text{eff}}(r)$) dans l'objet (1) est estimée ; 50
 - l'intensité ($I(r)$) du faisceau lumineux chauffant (11) à l'emplacement de mesure (r) est déterminée à partir de la carte d'augmentation de température ($\Delta T(r)$). 55
7. Procédé selon la revendication 6, **caractérisé en ce que** le coefficient optique est déterminé à une pluralité d'emplacements à l'intérieur de l'objet (1).
8. Support d'enregistrement sur lequel un programme d'ordinateur pour la détermination d'un coefficient optique (μ_a) à au moins un emplacement de mesure (r) dans un objet (1) est stocké, ledit programme étant adapté pour exécuter un procédé selon la revendication 6.

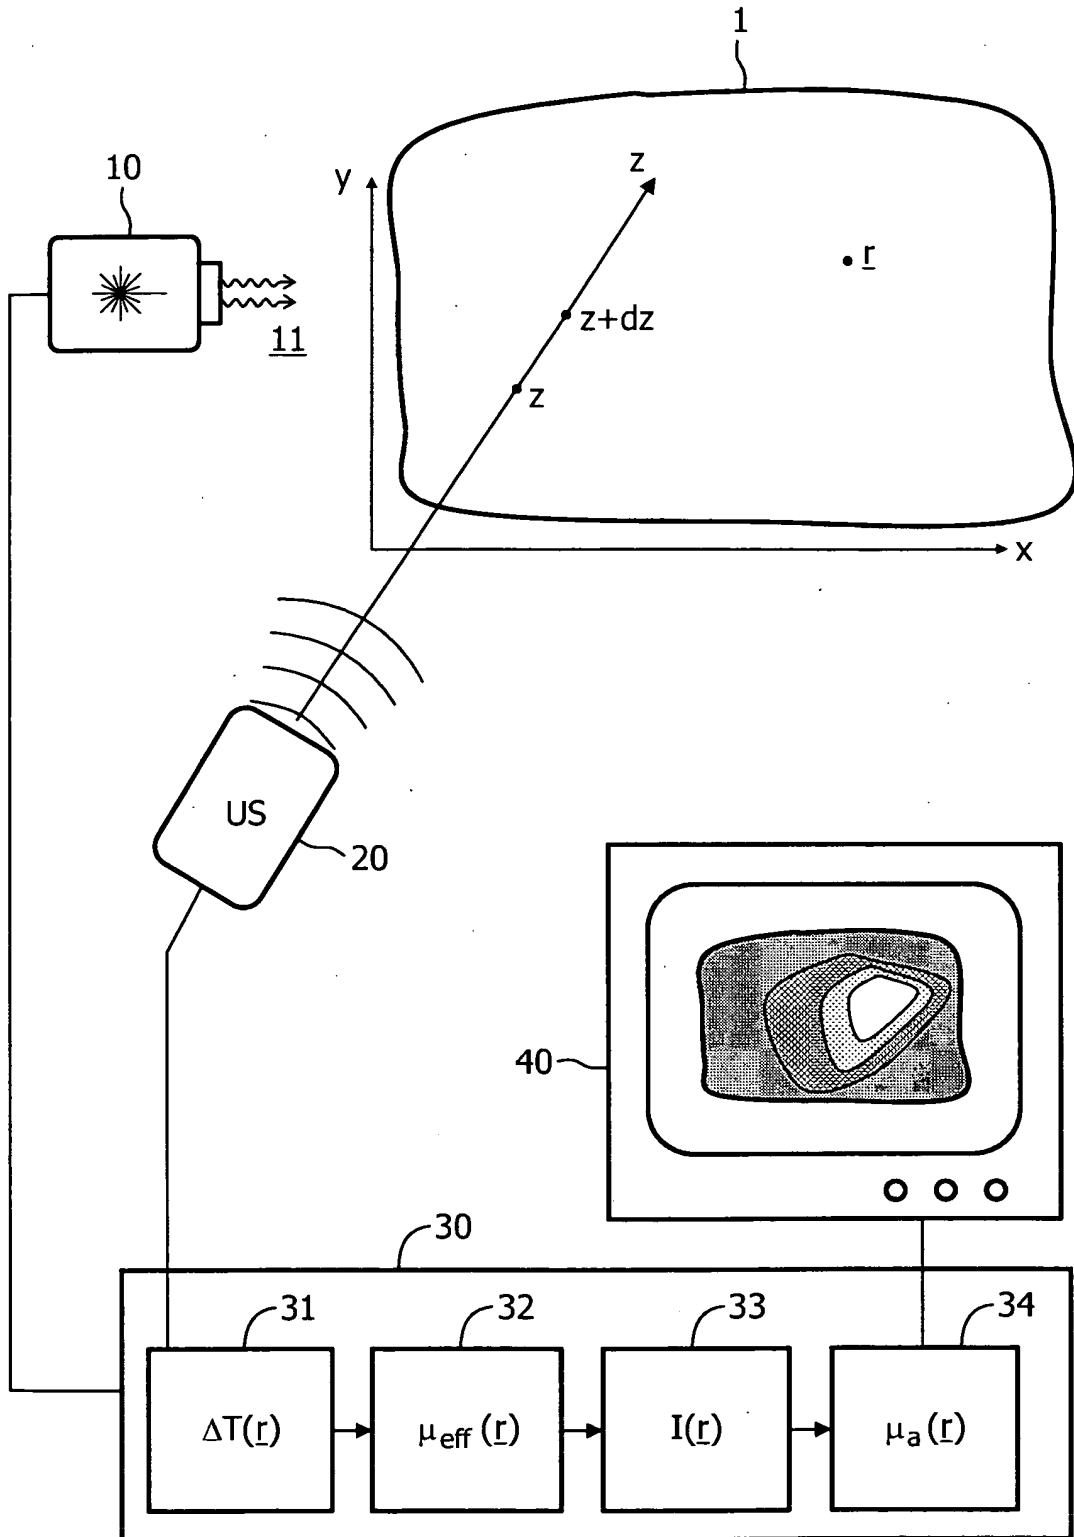


FIG. 1

$$v = v_0 \cdot (1 - \alpha_c \Delta T) \quad (1)$$

$$I^*(x,t) = I(x) \cdot f(t) = I_0 \exp(-\mu_{\text{eff}} x) \cdot f(t) \quad (2)$$

$$\mu_{\text{eff}} = \sqrt{3\mu_a (\mu_a + \mu_s(1-g))} \quad (3)$$

$$q_{\text{laser}} = \int \mu_a(r, \lambda) I(r, \lambda) d\lambda \quad (4)$$

$$q_{\text{laser}} = \mu_a(r) I(r, t) \quad (5)$$

$$\rho c \frac{\partial T}{\partial t} = \nabla(k \nabla T) + q_{\text{laser}} + q_{\text{pm}} \quad (6)$$

$$T(r,t) \propto \exp(-r^2/kt)/(kt)^{3/2} \quad (7)$$

$$\rho c \Delta T = \mu_a \cdot I(r) \cdot t_{\text{laser}} \quad (8)$$

$$dt = v(z) \cdot dz \quad (9)$$

$$dt = v_0 \cdot [(z+u(z)+dz+du)-(z+u(z))] \quad (10)$$

$$\frac{v(z)}{v_0} = 1 + \frac{du}{dz} \quad (11)$$

$$\Delta T = -\frac{1}{\alpha_c} \frac{du(z)}{dz} \quad (12)$$

$$\frac{\Delta T(r_A)}{\Delta T(r_B)} = \frac{(\mu_a/\rho c)_A I(r_A) t_{\text{laser}}}{(\mu_a/\rho c)_B I(r_B) t_{\text{laser}}} = \frac{I(r_A)}{I(r_B)} = \exp(\mu_{\text{eff}} (x_B - x_A)) \quad (13)$$

FIG. 2

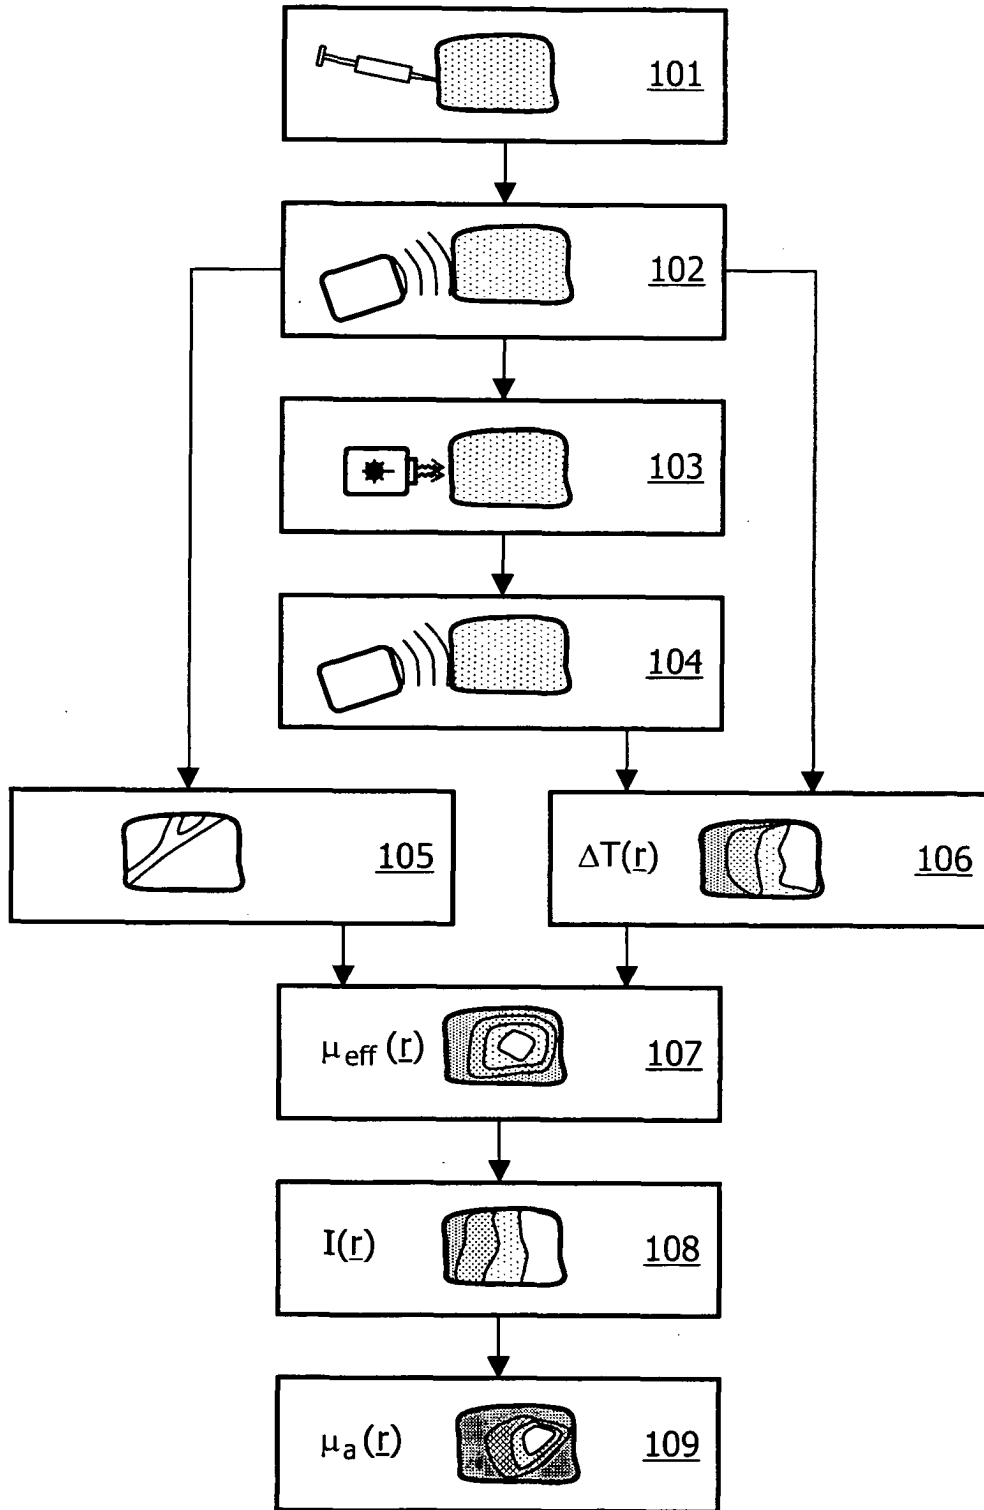


FIG. 3

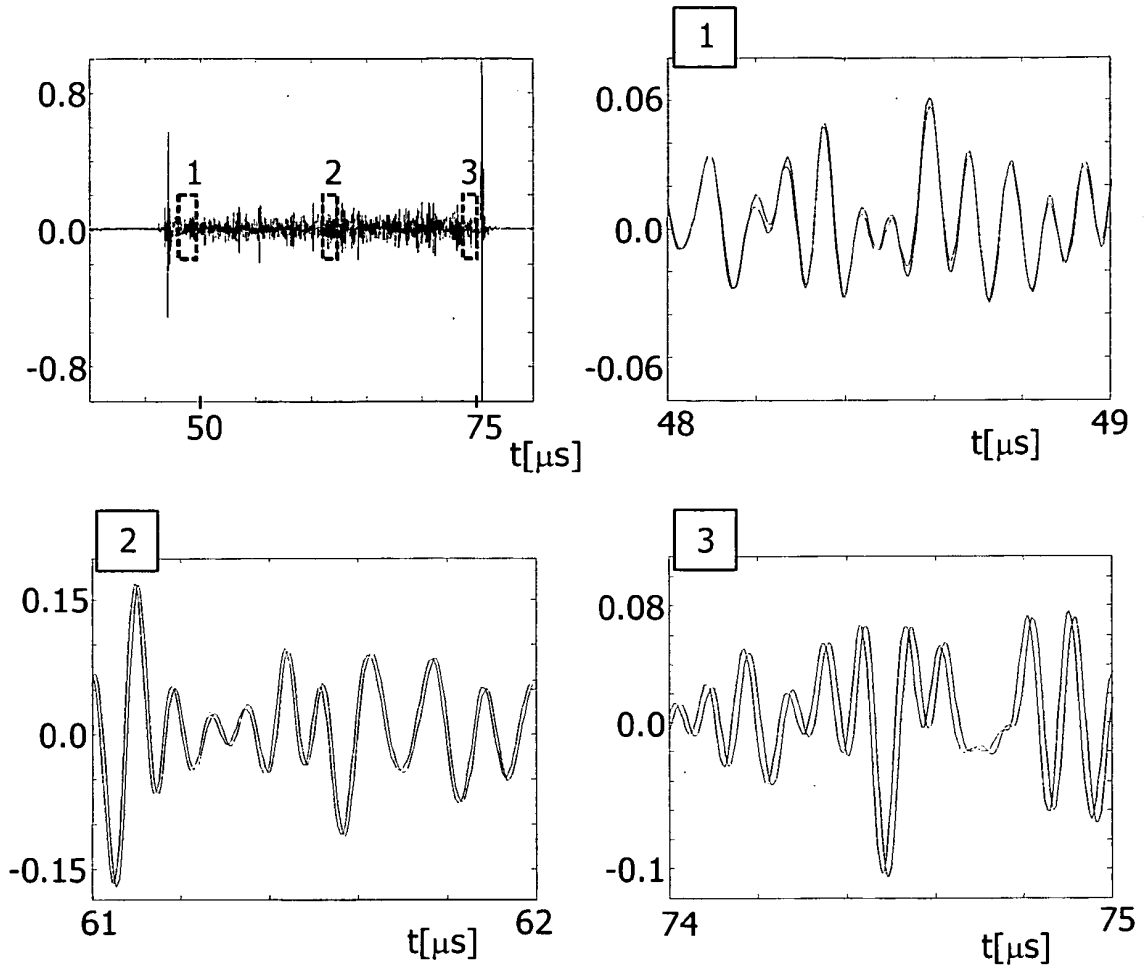


FIG. 4

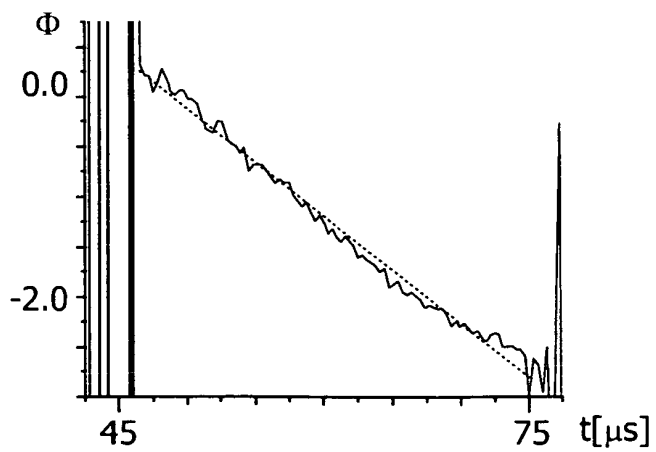


FIG. 5

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2005085725 A1 [0003]
- WO 2004086965 A [0004]

Non-patent literature cited in the description

- **B.C. WILSON.** Indirect versus direct techniques for the measurement of the optical properties of tissues. *Photochem Photobiol.*, 1987, vol. 46, 601-608 [0002]
- **A.A. ORAEVSKY.** Measurement of tissue optical properties by time-resolved detection of laser-induced transient stress. *Appl. Opt.*, 1997, vol. 36, 402 [0002]
- Real-time optoacoustic monitoring of temperature in tissues; Optoacoustic monitoring of temperature in tissues. **IRINA VLARINA et al.** JOURNAL OF PHYSICS D. APPLIED PHYSICS. INSTITUTE OF PHYSICS PUBLISHING, 07 August 2005, vol. 38, 2633-2639 [0005]
- **ANAND A et al.** Ultrasonic determination of three-dimensional spatial and temporal thermal distribution for therapy monitoring. *IEEE INTERNATIONAL CONFERENCE ON ACOUSTICS, SPEECH, AND SIGNAL PROCESSING*, 14 May 2006, II-1108-II-1111 [0006]
- **R. SEIP ; ES. EBBINI.** Noninvasive estimation of tissue temperature response to heating fields using diagnostic ultrasound. *IEEE Transactions on Biomedical Engineering*, 1995, vol. 42 (8), 828-839 [0028]
- **F. DUCK.** Physical Properties of Tissue: A Comprehensive Reference Work. Elsevier Science & Technology Books [0035]

专利名称(译)	超声波测定光学吸收系数		
公开(公告)号	EP2074418B1	公开(公告)日	2013-03-06
申请号	EP2007826422	申请日	2007-09-18
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	SAVERY DAVID JANKOVIC LADISLAV ANAND AJAY		
发明人	SAVERY, DAVID JANKOVIC, LADISLAV ANAND, AJAY		
IPC分类号	G01N29/24 A61B5/00 G01N21/17 G01N21/47		
CPC分类号	G01N29/2418 A61B5/0059 A61B5/0095 A61B8/08 G01N21/1702 G01N21/4795 G01N2021/1706 G01N2291/02466 G01N2291/02475		
优先权	2006121524 2006-09-29 EP		
其他公开文献	EP2074418A2		
外部链接	Espacenet		

摘要(译)

检查装置和方法技术领域本发明涉及一种检查装置和方法，用于确定光学系数，特别是像患者身体一样的物体（1）中的光学吸收系数（ μ_a ）。该装置包括超声扫描仪（20），用于在用来自（例如激光）光源（10）的加热光束（11）照射物体（1）之前和之后记录第一和第二脉冲回波。评估单元（30）基于在第二和第一脉冲回波之间出现的表现位移来确定由物体（1）内的加热光束（11）引起的温度增加（ $\Delta T(r)$ ）的图。此外，对物体（1）内部局部相邻温度增加的评估允许确定有效散射系数（ $\mu_{eff}(r)$ ）的图，从该图中光强度（ $I(r)$ ）在物体内部的分布（1）可以计算。最后，可以根据该位置处的光强度和温度增加来确定测量位置（ r ）处的期望光学吸收系数（ μ_a ）。

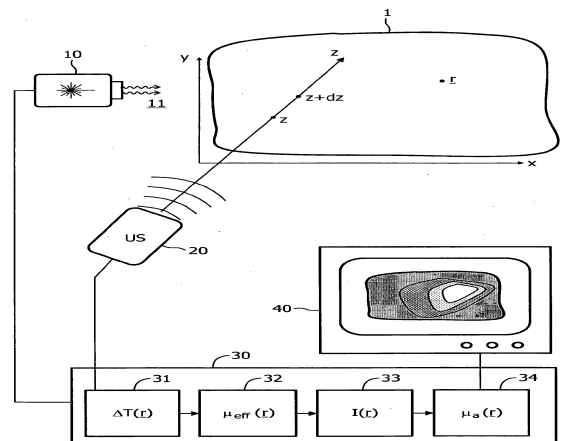


FIG. 1