



(11) **EP 3 263 084 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
03.01.2018 Bulletin 2018/01

(51) Int Cl.:
A61G 7/057 (2006.01) A61B 5/00 (2006.01)
A61F 7/100 (2006.01)

(21) Application number: **16207369.6**

(22) Date of filing: **29.12.2016**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
MA MD

- **KING, Catherine**
Batesville, Indiana 47006-9167 (US)
- **LAI, Samuel**
Batesville, Indiana 47006-9167 (US)
- **SALIBRA, Alisa Robinson**
Batesville, Indiana 47006-9167 (US)
- **STEBBINS, Kristen L.**
Batesville, Indiana 47006-9167 (US)
- **TALLENT, Dan R**
Batesville, Indiana 47006-9167 (US)
- **VENTROLA, Todd**
Batesville, Indiana 47006-9167 (US)
- **WILLIAMSON, Rachel**
Batesville, Indiana 46007-9167 (US)

(30) Priority: **01.07.2016 US 201662357554 P**

(71) Applicant: **Hill-Rom Services, Inc.**
Batesville, IN 47006-9167 (US)

(72) Inventors:
• **COLEMAN II, Leigh Scott**
Batesville, Indiana 47006-9167 (US)
• **KAIKENGER, Philippe**
Batesville, Indiana 47006-9167 (US)

(74) Representative: **Findlay, Alice Rosemary**
Reddie & Grose LLP
The White Chapel Building
10 Whitechapel High Street
London E1 8QS (GB)

(54) **MICROCLIMATE MANAGEMENT SYSTEM WITH WIRELESS SENSORS**

(57) A method for monitoring an environment for a patient on a patient support device can include: receiving a temperature reading from a wireless sensor coupled to a body of the patient; comparing the temperature read-

ing to air flowing through an airflow system associated with the patient support device; and modifying the air flowing through the airflow system.

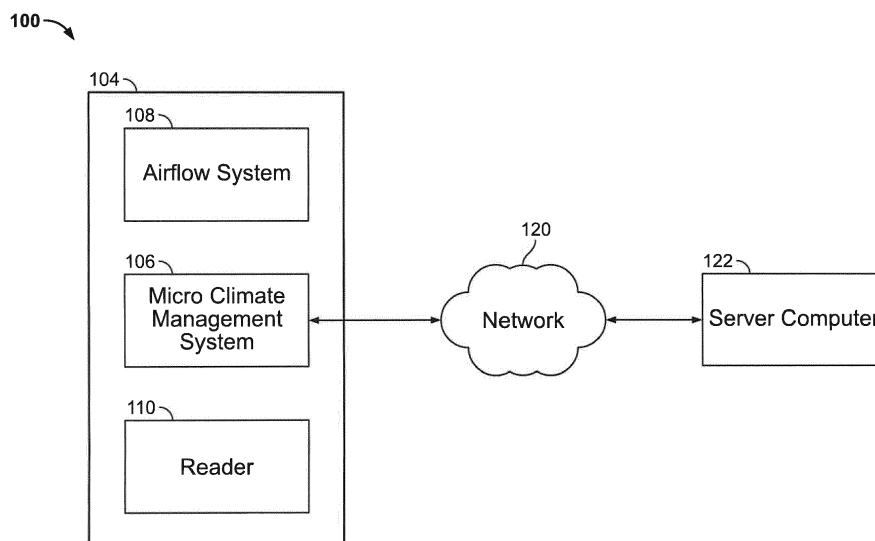


FIG. 1

EP 3 263 084 A1

Description

[0001] Patients lying on support devices, such as hospital bed mattresses, for extended periods of time are susceptible to the development of pressure ulcers (also known as decubitus ulcers or bedsores). Pressure ulcers are lesions often found adjacent bony or cartilaginous areas. Pressure ulcers may be caused by tissue forces, such as, for example, pressure, i.e., compression of tissues, shear force, and friction. Pressure ulcer formation may be exacerbated by the presence of excess body heat and/or moisture.

[0002] Embodiments of the disclosure are directed to a method for monitoring an environment for a patient on a patient support device can include: receiving a temperature reading from a wireless sensor coupled to a body of the patient; comparing the temperature reading to air flowing through an airflow system associated with the patient support device; and modifying the air flowing through the airflow system.

[0003] The invention will now be further described by way of example with reference to the accompanying drawings, in which:

Figure 1 shows an example environment including a patient support device and a microclimate management system.

Figure 2 shows additional details of the environment of Figure 1.

Figure 3 shows an example process diagram illustrating possible operation within the environment of Figure 1.

Figure 4 shows another example process diagram illustrating possible operation within the environment of Figure 1.

Figure 5 shows example physical components of the microclimate management system of Figure 1.

[0004] The present disclosure is directed to systems and methods for manipulating the environment for a patient in an ambulatory environment, such as a hospital or clinic setting. In some examples, the temperature of the patient is measured using wireless sensors at one or more points on the patient. A microclimate management system receives those temperature readings and can modify the environment surrounding the patient, such as temperature, relative humidity, etc.

[0005] Figures 1-2 show an example environment 100, such as a hospital or clinical setting. In this context, a patient support device 104, such as a mattress, provides support for a patient 210. One example of such a patient support device 104 is the TotalCare® P500 Intensive Care Bed manufactured by Hill-Rom of Batesville, Indiana. Other configurations are possible.

[0006] The patient support device 104 includes a microclimate management system 106 associated with the patient support device 104. The microclimate management system 106 is configured to monitor and modify the

environment surrounding the patient 210, as described further herein. For example, the microclimate management system 106 can be configured to modify the temperature and/or relative humidity surrounding the patient 210 to achieve desired clinical benefits.

[0007] To accomplish this functionality, the microclimate management system 106 controls an airflow system 108 associated with the patient support device 104. In this example, the microclimate management system 106 can modify an amount of air flowing through the airflow system 108 and/or a temperature and humidity of the air flowing therethrough. This, in turn, can modify a temperature of the patient 210 that is supported by the patient support device 104.

[0008] In one example, the microclimate management system 106 is configured in a manner described in U.S. Patent Published Application No. 2011/0024076 A1 to Lachenbruch et al. The Application discloses detailed examples of microclimate management systems.

[0009] The patient support device 104 is also associated with a reader 110 positioned within or adjacent to the patient support device 104. In this example, the reader 110 is configured to read information from one or more sensors associated with the patient 210.

[0010] For example, in one embodiment, one or more wireless patches or wireless sensors 220 are placed at desired locations on the body of the patient 210. For example, each wireless sensor 220 can include an adhesive portion that removably couples the wireless sensor 220 to the skin of the patient 210. The wireless sensor 220 can also include various components, such as a thermistor, a processor, memory, and/or a source of power like a battery. In other examples, the wireless sensor 220 can be without its own source of power (i.e., passive).

[0011] Although a single wireless sensor 220 is shown, multiple sensors can be used and positioned at different areas of the body of the patient 210. For example, multiple temperature sensors can be positioned at different parts of the body of the patient 210 to provide a more localized temperature. If, for instance, the hands and feet of the patient 210 are cold, then the heating could be increased (and vice versa if the hands and feet are warm). Likewise, other sensors, such as a galvanic skin response sensor that measures the electrical conductance of the skin, could be used to sense sweating by the patient 210, which would be an indication that the environment is too warm.

[0012] Further, multiple readers can be provided along the patient support device 104, if desired.

[0013] In this example, the wireless sensor 220 is configured to measure a temperature of the patient 210 at the positioned location. The temperature can be stored, and the reader 110 is configured to interrogate the wireless sensor 220 at desired intervals to read the measured temperature and communicate that temperature to the microclimate management system 106.

[0014] For example, the reader 110 can use different communication schemes, such as nearfield communica-

tion (NFC) to interrogate the wireless sensor 220. The reader 110 can be positioned within or adjacent to the patient support device 104 such that the reader 110 is in close enough proximity to read the wireless sensor 220.

[0015] In example embodiments, the wireless sensor 220 is configured in the manner described in U.S. Patent Application Serial No. 15/053,661 to Quinn. Other configurations are possible.

[0016] The reader 110 is programmed to communicate the temperature reading(s) to the microclimate management system 106. The microclimate management system 106, in turn, uses the temperature information to maintain the patient 210 within a desired environment. For example, if the temperature reading is high, the microclimate management system 106 can modify the temperature, humidity, and/or speed of the air flowing in the airflow system 108 in order to reduce a temperature of the patient 210.

[0017] In another example, the microclimate management system 106 can be programmed to manage temperature readings from multiple locations on the body of the patient 210 and modify airflow to areas associated various portions of the body to maintain desired temperatures at specific locations on the body. Further, the microclimate management system 106 can monitor a trend of the temperature(s) over time and use feedback mechanisms to accomplish a desired temperature, as described further below.

[0018] The microclimate management system 106 can also communicate the temperature information to a remote system, such as a server computer 122, through a network 120. For example, the server computer 122 can be a central server, such as caregiver station, that allows a caregiver to monitor the temperature reading(s) for the patient 210. Further, various alerting can be provided to the caregiver, such as if the temperature falls outside a given range. In another example, the server computer 122 can be an electronic medical record (EMR) repository, and the temperature reading(s) can be captured within the EMR for the patient 210. Other configurations are possible.

[0019] Referring now to Figure 3, an example process diagram 300 illustrating the operation within the environment 100 is shown.

[0020] At process 302, the patient's temperature (T1) is measured by the one or more wireless sensor 220. This is accomplished, as described above, by the wireless sensors taking one or more temperature measurements on the patient's body.

[0021] At process 306, the temperature (T2) and/or relative humidity of the air and the speed of the airflow (ϕ) being provided by the microclimate management system is determined.

[0022] At process 304, the microclimate management system analyzes this information over time (t): $f(T1, T2, \phi, t)$.

[0023] At process 308, the microclimate management system can heat or cool the air flowing through the airflow

system to increase or decrease the temperature of the patient. This can be done based upon an average of the temperatures provided by the wireless sensors (if more than one is used) and/or different zones within the airflow system can be used to increase or decrease the temperature at specific areas adjacent to the patient's body.

[0024] Likewise, at process 310, the microclimate management system can modify the speed of the airflow through the airflow system to accomplish desired heating or cooling.

[0025] The temperatures T1, T2 and airflow speed ϕ can be monitored over time, and the microclimate management system can modify heating or cooling (or airflow speed) as desired based upon these measurements.

This modification can be automated. In other examples, the modifications can be suggested to the caregiver, such as on a graphical user interface. The caregiver can then manually adjust the microclimate management system based upon the suggestions.

[0026] Referring now to Figure 4, another example process diagram 400 illustrating the operation within the environment 100 is shown.

[0027] The process diagram 400 is similar to the process diagram 300 described above, except that the patient's Braden score is determined at process 412. The Braden score is derived from a Braden Scale for Predicting Pressure Ulcer Risk, which is a tool that is used to measure the patient's risk of developing a pressure ulcer. Factors such as moisture of the skin, activity, mobility, nutrition, and friction/shear can be factored into deriving the score.

[0028] In one example, the Braden score is manually determined and provided to the microclimate management system. In another example, one or more automated processes (e.g., sensors used to collect factors like moisture, activity, etc.) are used to derive the Braden score.

[0029] At operation 404, the microclimate management system analyzes the Braden score (B) as part of the information used to determine modifications to the airflow temperature and speed: $f(T1, T2, \phi, t, B)$. The Braden score can be used as a check for the environment 100. For example, too much warming can be associated with pressure ulcer events - using the Braden score as one input into the system can help to assure that excessive heating is not provided by the microclimate management system.

[0030] In the examples provided herein, the various components of the environment 100 can be implemented as one or more computing devices. For example, the microclimate management system 106 can be a computing device. Other components, such as the reader, server computer, and wireless sensors, can also be implemented as one or more computing devices.

[0031] As illustrated in Figure 5, the microclimate management system 106 includes at least one central processing unit ("CPU") 502, a system memory 508, and a system bus 522 that couples the system memory 508

to the CPU 502. The system memory 508 includes a random access memory ("RAM") 510 and a read-only memory ("ROM") 512. A basic input/output system contains the basic routines that help to transfer information between elements within the microclimate management system 106, such as during startup, is stored in the ROM 512. The microclimate management system 106 further includes a mass storage device 514. The mass storage device 514 is able to store software instructions and data. A central processing unit, system memory and mass storage device similar to that in Figure 5 are also included in server computer 102.

[0032] The mass storage device 514 is connected to the CPU 502 through a mass storage controller (not shown) connected to the system bus 522. The mass storage device 514 and its associated computer-readable data storage media provide non-volatile, non-transitory storage for the microclimate management system 106. Although the description of computer-readable data storage media contained herein refers to a mass storage device, such as a hard disk or solid state disk, it should be appreciated by those skilled in the art that computer-readable data storage media can be any available non-transitory, physical device or article of manufacture from which the central display station can read data and/or instructions.

[0033] Computer-readable data storage media include volatile and non-volatile, removable and non-removable media implemented in any method or technology for storage of information such as computer-readable software instructions, data structures, program modules or other data. Example types of computer-readable data storage media include, but are not limited to, RAM, ROM, EPROM, EEPROM, flash memory or other solid state memory technology, CD-ROMs, digital versatile discs ("DVDs"), other optical storage media, magnetic cassettes, magnetic tape, magnetic disk storage or other magnetic storage devices, or any other medium which can be used to store the desired information and which can be accessed by the microclimate management system 106.

[0034] According to various embodiments, the microclimate management system 106 may operate in a networked environment using logical connections to remote network devices through the network 120, such as a wireless network, the Internet, or another type of network. The microclimate management system 106 may connect to the network 120 through a network interface unit 504 connected to the system bus 522. It should be appreciated that the network interface unit 504 may also be utilized to connect to other types of networks and remote computing systems. The microclimate management system 106 also includes an input/output controller 506 for receiving and processing input from a number of other devices, including a touch user interface display screen, or another type of input device. Similarly, the input/output controller 506 may provide output to a touch user interface display screen or other type of output device.

[0035] As mentioned briefly above, the mass storage device 514 and the RAM 510 of the microclimate management system 106 can store software instructions and data. The software instructions include an operating system 518 suitable for controlling the operation of the microclimate management system 106. The mass storage device 514 and/or the RAM 510 also store software instructions, that when executed by the CPU 502, cause the microclimate management system 106 to provide the functionality of the microclimate management system 106 discussed in this document. For example, the mass storage device 514 and/or the RAM 510 can store software instructions that, when executed by the CPU 502, cause the microclimate management system 106 to adjust a temperature and/or speed of airflow being provided to the patient.

[0036] Although various embodiments are described herein, those of ordinary skill in the art will understand that many modifications may be made thereto.

Claims

1. A method for monitoring an environment for a patient on a patient support device, the method comprising:
 - receiving a temperature reading from at least one wireless sensor on a body of the patient;
 - comparing the temperature reading to air flowing through an airflow system associated with the patient support device; and
 - modifying the air flowing through the airflow system.
2. The method of claim 1, further comprising:
 - providing the wireless sensor; and
 - allowing the wireless sensor to take one or more temperature readings at the body of the patient.
3. The method of either claim 1 or claim 2 further comprising positioning multiple wireless sensors on a body of the patient.
4. The method of claim 3, further comprising positioning the multiple wireless sensors at different areas of the body of the patient.
5. The method of claim 4, further comprising receiving from the multiple wireless sensors the one or more temperature readings at the different areas of the body.
6. The method of claim 4, further comprising receiving from the multiple wireless sensors the temperature readings at different areas of the body.
7. The method of either claim 5 or claim 6, further com-

prising modifying the air flowing through the airflow system based upon the temperature readings at the different areas of the body.

- 8. The method of any preceding claim, further comprising positioning a galvanic skin response sensor to detect sweating on the body of the patient. 5
- 9. The method of claim 8, further comprising increasing an air temperature or an air speed of the air flowing through the airflow system when the sweating is detected. 10
- 10. The method of any preceding claim, further comprising adjusting an air speed of the air flowing through the airflow system. 15
- 11. The method of any preceding claim, further comprising using a Braden score when comparing the temperature to the air flowing through the airflow system. 20
- 12. The method of any preceding claim wherein the at least one sensor is coupled to the body of the patient.
- 13. A system for monitoring an environment for a patient on a patient support device, the system comprising: 25
 - multiple wireless sensors configured to be placed on a body of the patient;
 - a controller programmed to receive temperature readings from the multiple wireless sensors; and 30
 - an airflow system associated with the patient support device, wherein the controller is programmed to modify air flowing through the airflow system based upon a comparison of the temperature readings to the air flowing through the airflow system. 35
- 14. The system of claim 13, wherein the multiple wireless sensors are positioned at different areas of the body. 40
- 15. The system of claim 14, wherein the controller is programmed to modify the air flowing through the airflow system based upon the temperature readings at the different areas of the body. 45

50

55

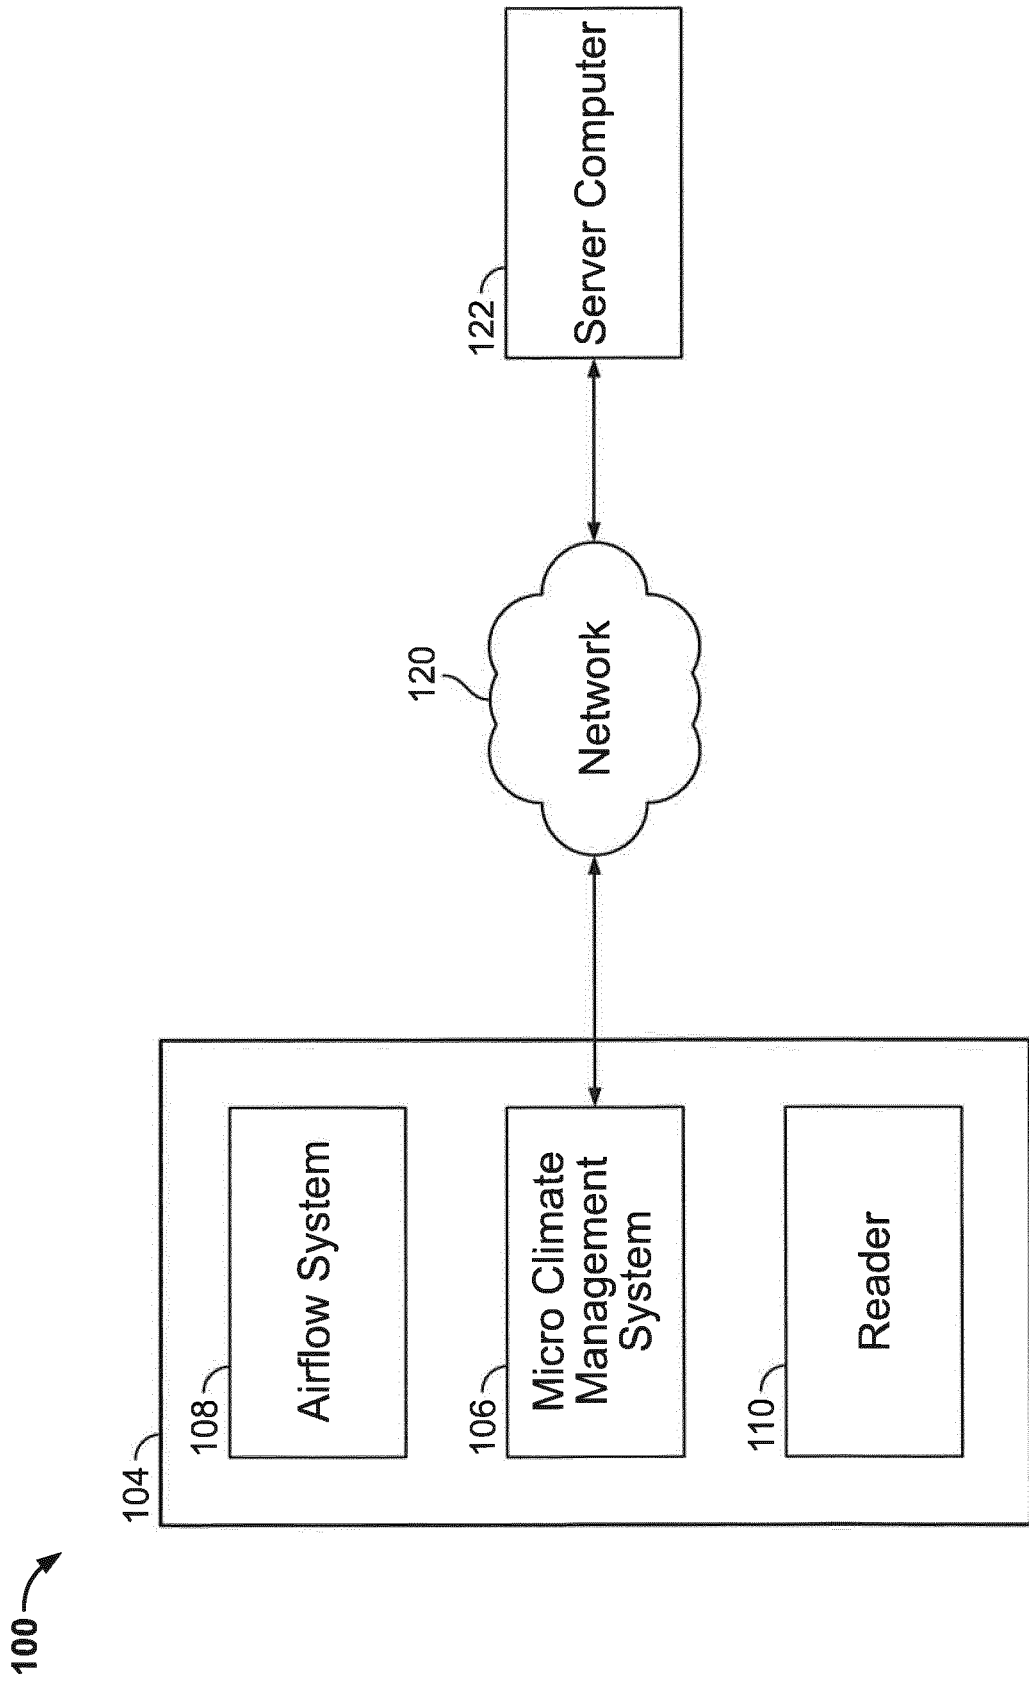


FIG. 1

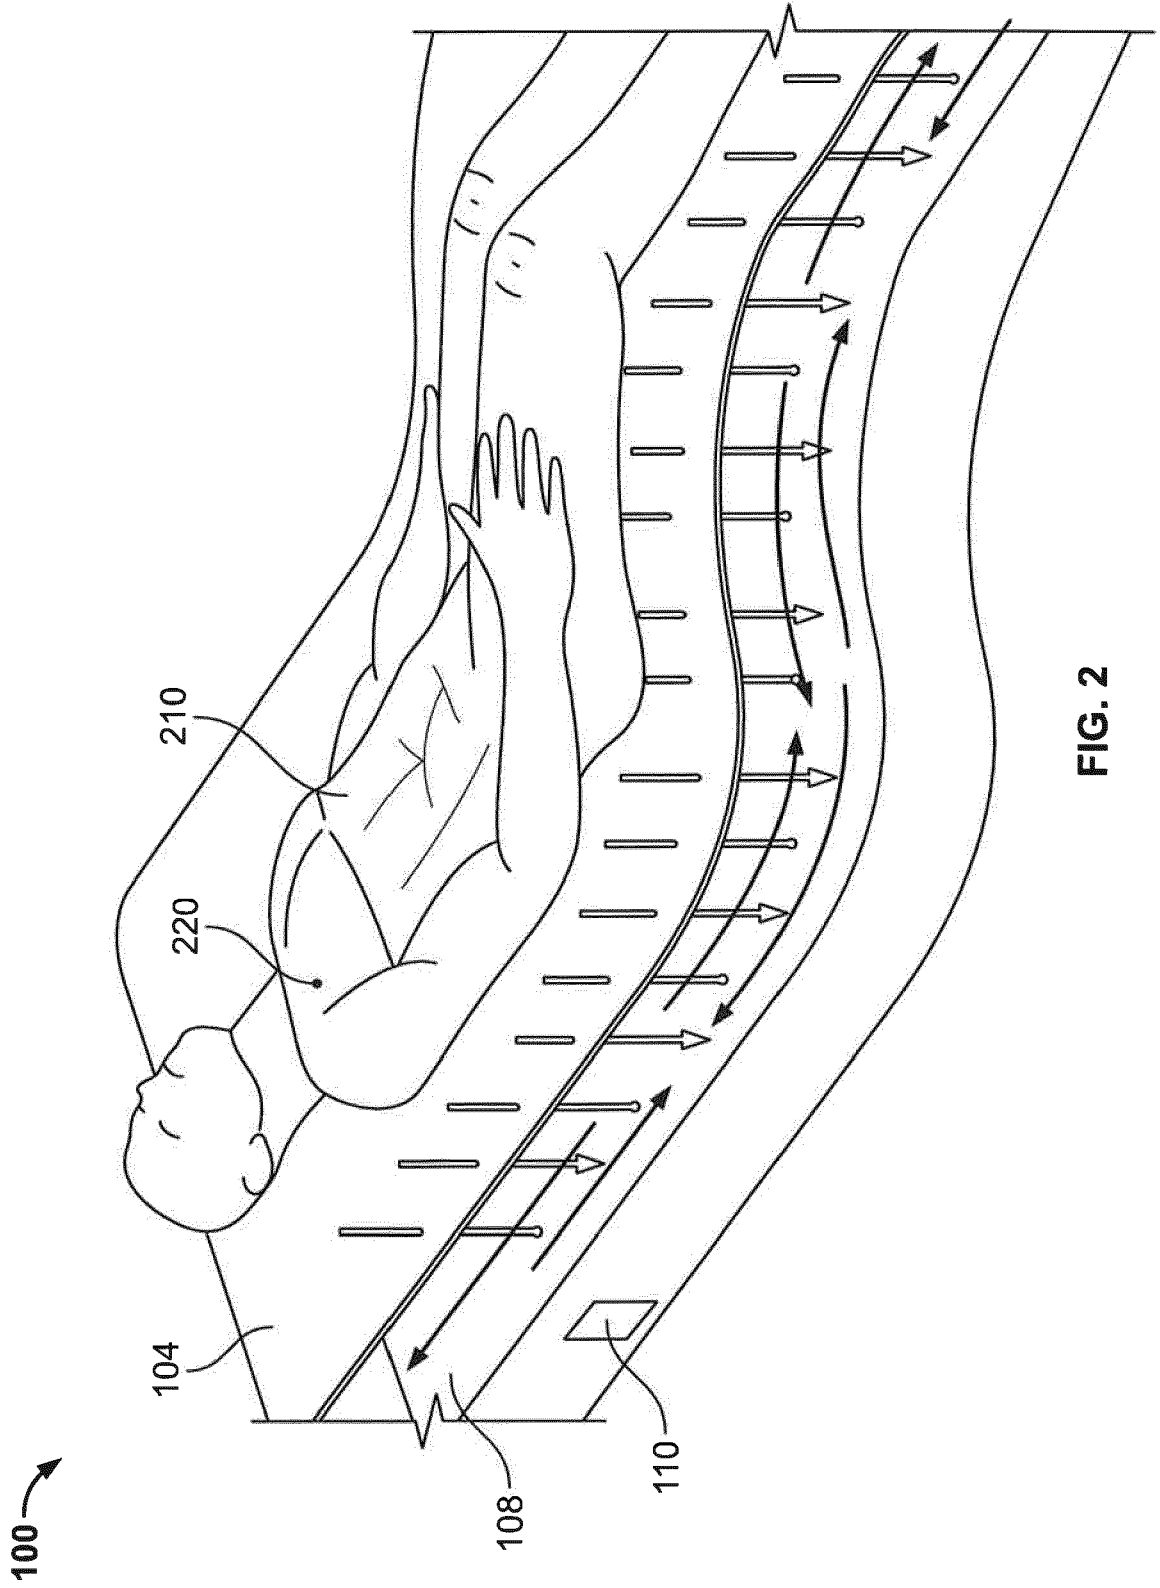


FIG. 2

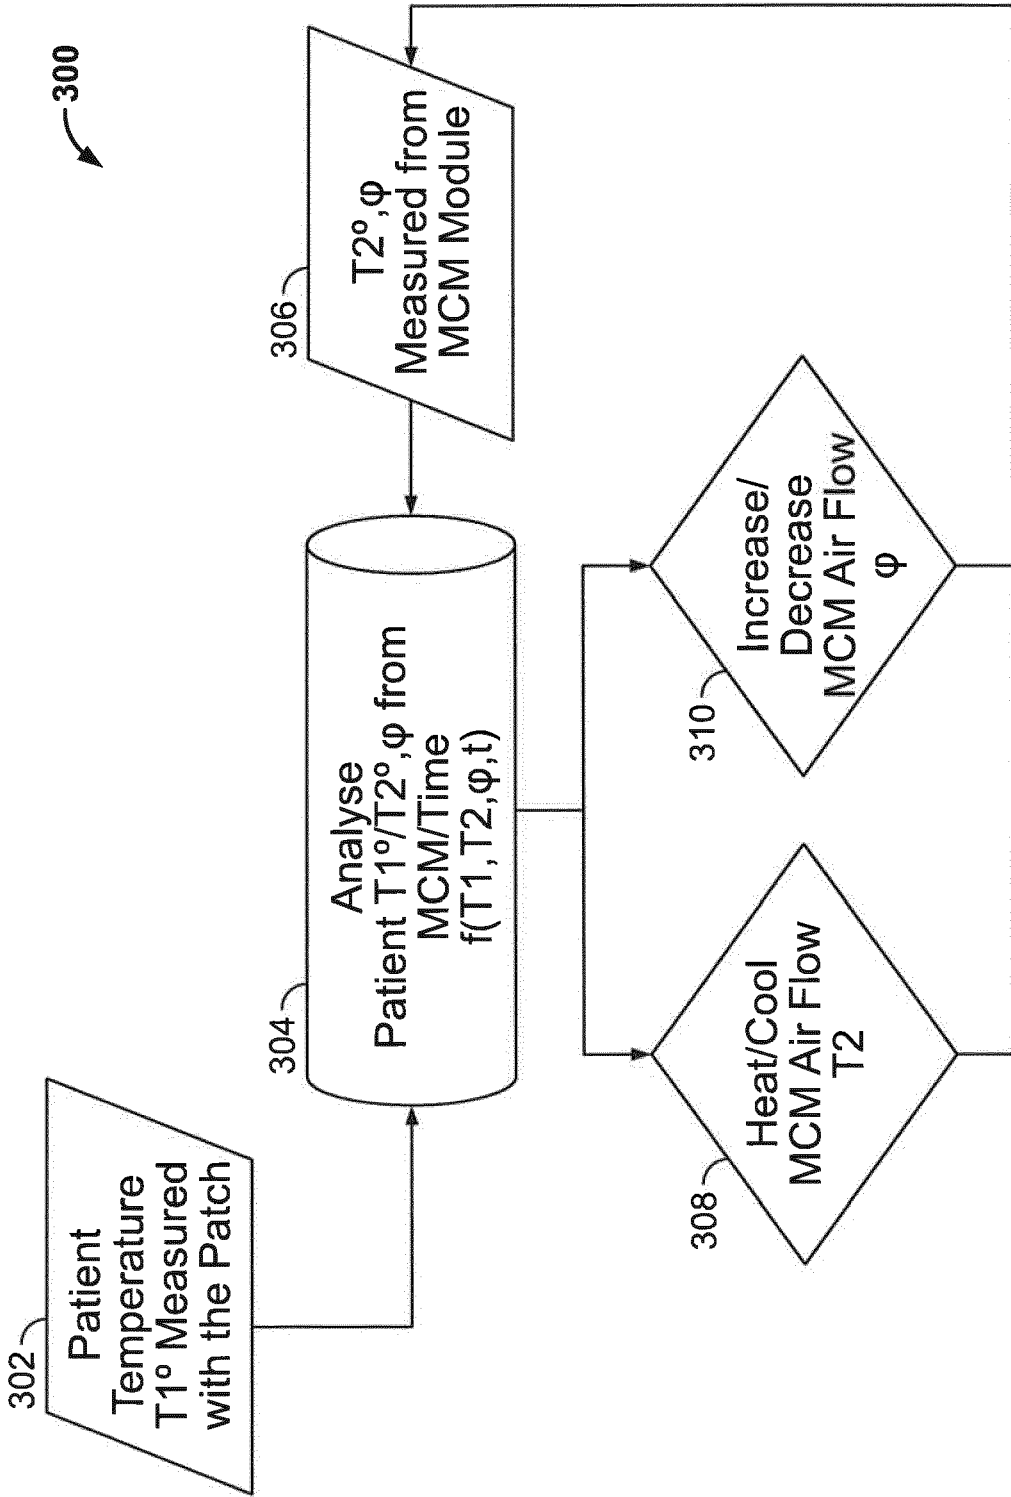


FIG. 3

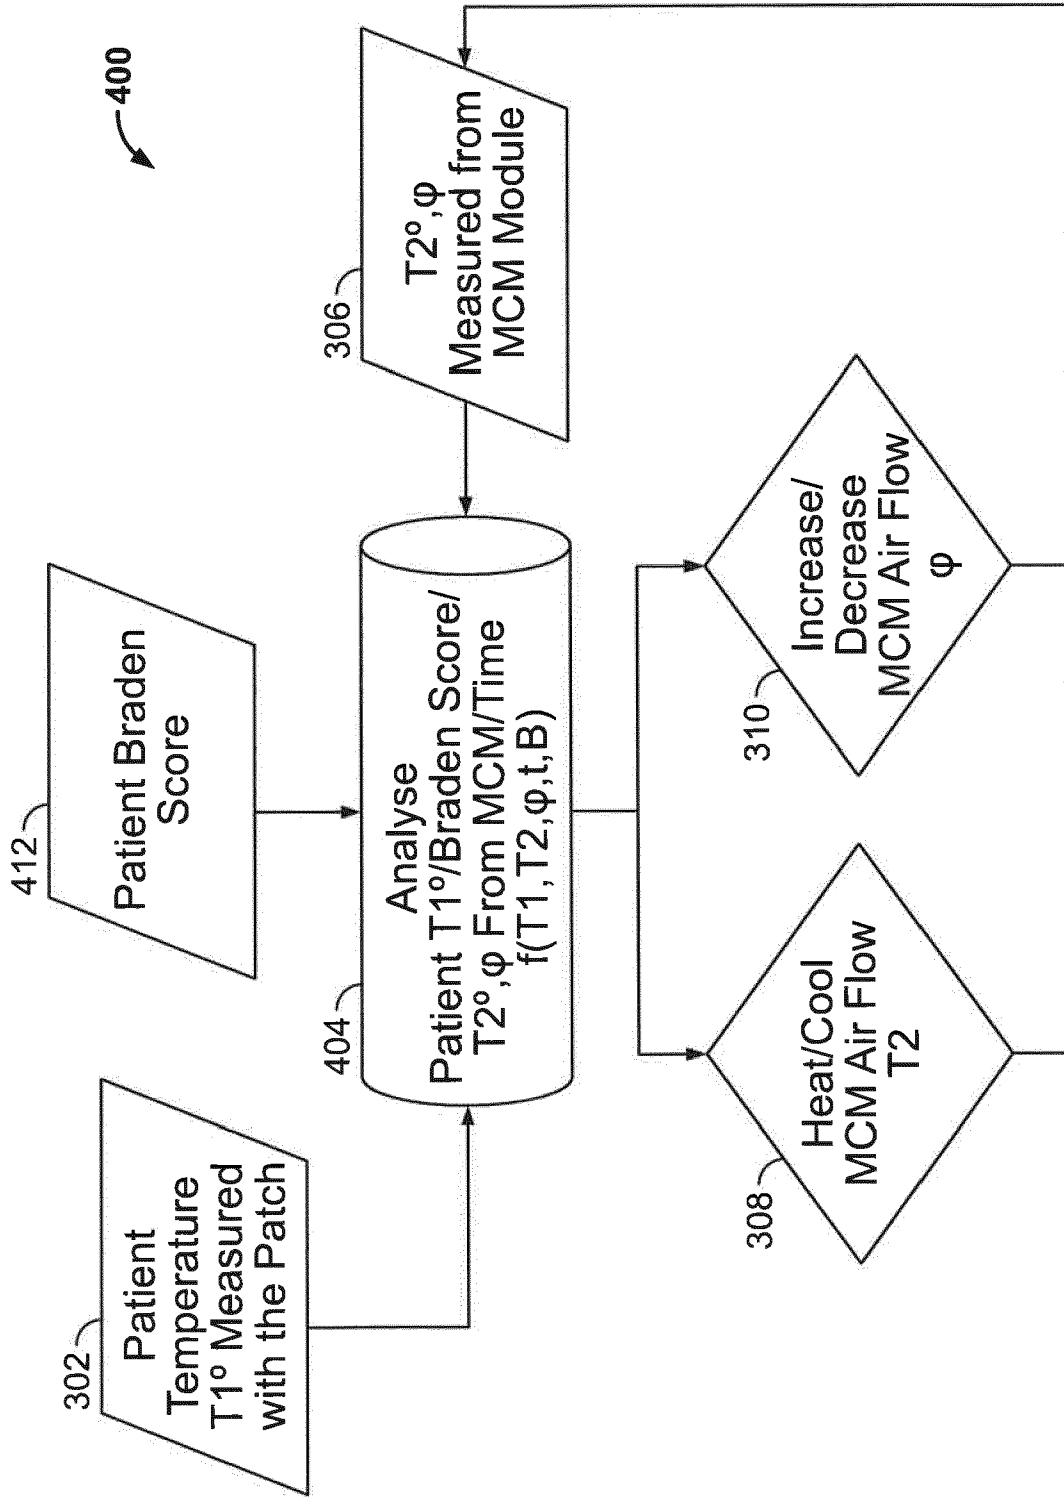


FIG. 4

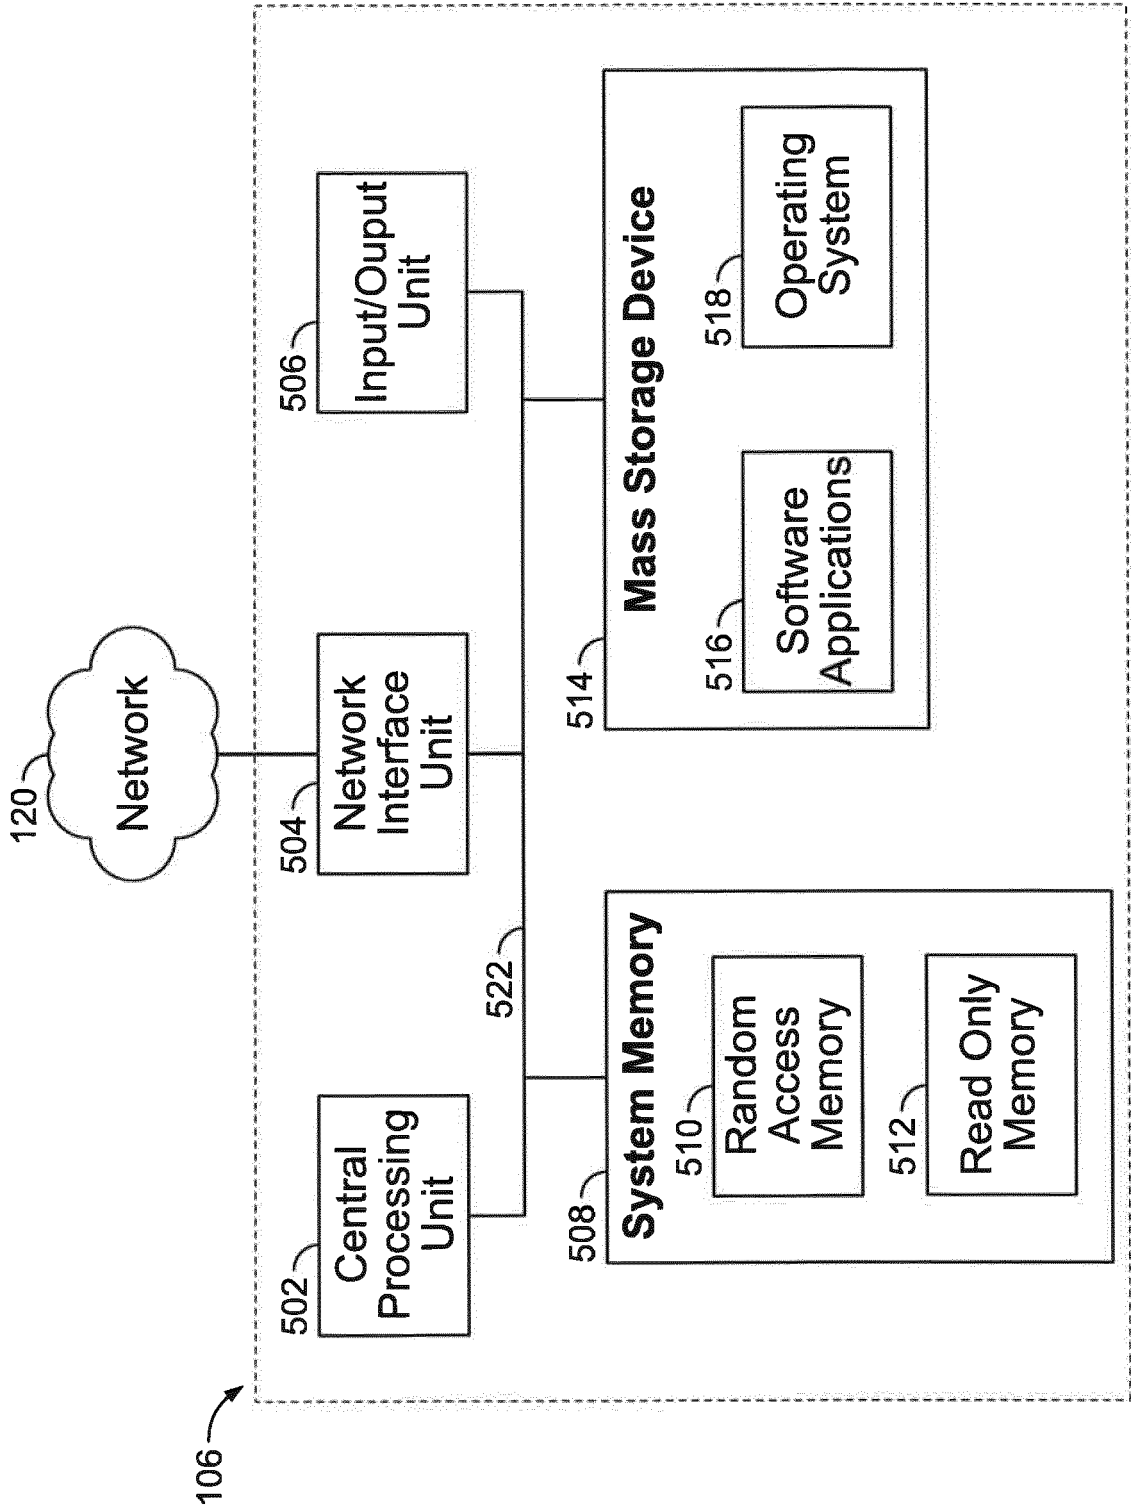


FIG. 5



EUROPEAN SEARCH REPORT

Application Number
EP 16 20 7369

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2011/263950 A1 (LARSON BARRETT J [US] ET AL) 27 October 2011 (2011-10-27) * paragraphs [0218] - [0220], [0272], [0273], [0101] * -----	1-15	INV. A61G7/057 A61B5/00 A61F7/00
X	US 2009/149927 A1 (KNEUER HARALD [US] ET AL) 11 June 2009 (2009-06-11) * paragraphs [0038], [0053] * -----	13,14	
A	WO 2009/129306 A1 (HILL ROOM SERVICES INC [US]; LACHENBRUCH CHARLES A [US]; DOUGLAS STEPH) 22 October 2009 (2009-10-22) * paragraph [0041]; figures 3,4 * -----	13	
A	US 2005/267339 A1 (BECKMANN UDO [DE] ET AL) 1 December 2005 (2005-12-01) * paragraph [0020]; figure 2 * -----	13,14	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61G A61B A61F
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 12 April 2017	Examiner Birlanga Pérez, J
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

1
EPO FORM 1503 03/02 (P04C01)

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 16 20 7369

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

12-04-2017

10

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2011263950 A1	27-10-2011	JP 2013526900 A	27-06-2013
		US 2011263950 A1	27-10-2011
		US 2016278691 A1	29-09-2016
		US 2016278692 A1	29-09-2016
		US 2016367170 A1	22-12-2016

US 2009149927 A1	11-06-2009	DE 102008057469 A1	10-09-2009
		US 2009149927 A1	11-06-2009
		US 2013198673 A1	01-08-2013
		US 2013217981 A1	22-08-2013
		US 2013282198 A1	24-10-2013

WO 2009129306 A1	22-10-2009	EP 2276437 A1	26-01-2011
		EP 2594234 A2	22-05-2013
		EP 2702966 A2	05-03-2014
		US 2011024076 A1	03-02-2011
		WO 2009129306 A1	22-10-2009

US 2005267339 A1	01-12-2005	DE 102004025797 B3	15-12-2005
		FR 2870707 A1	02-12-2005
		US 2005267339 A1	01-12-2005

15

20

25

30

35

40

45

50

55

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20110024076 A1, Lachenbruch [0008]
- US 053661 A, Quinn [0015]

专利名称(译)	带有无线传感器的微气候管理系统		
公开(公告)号	EP3263084A1	公开(公告)日	2018-01-03
申请号	EP2016207369	申请日	2016-12-29
[标]申请(专利权)人(译)	希尔 - 罗姆服务股份有限公司		
申请(专利权)人(译)	HILL-ROM SERVICES , INC.		
当前申请(专利权)人(译)	HILL-ROM SERVICES , INC.		
[标]发明人	COLEMAN II LEIGH SCOTT KAIKENDER PHILIPPE KING CATHERINE LAI SAMUEL SALIBRA ALISA ROBINSON STEBBINS KRISTEN L TALLENT DAN R VENTROLA TODD WILLIAMSON RACHEL		
发明人	COLEMAN II, LEIGH SCOTT KAIKENDER, PHILIPPE KING, CATHERINE LAI, SAMUEL SALIBRA, ALISA ROBINSON STEBBINS, KRISTEN L. TALLENT, DAN R VENTROLA, TODD WILLIAMSON, RACHEL		
IPC分类号	A61G7/057 A61B5/00 A61F7/00		
CPC分类号	A61G7/05784 A61G2203/46 A61G2210/70 A61B5/0002 A61F7/0053 A61B5/0024 A61B5/01 A61B5/0533 A61F2007/006 A61F2007/0064 A61F2007/0093		
优先权	62/357554 2016-07-01 US		
其他公开文献	EP3263084B1		
外部链接	Espacenet		

摘要(译)

一种用于在患者支撑装置上监测患者的环境的方法可以包括：从耦合到患者身体的无线传感器接收温度读数；将温度读数与流过与患者支撑装置相关的气流系统的空气进行比较；并改变流经气流系统的空气。

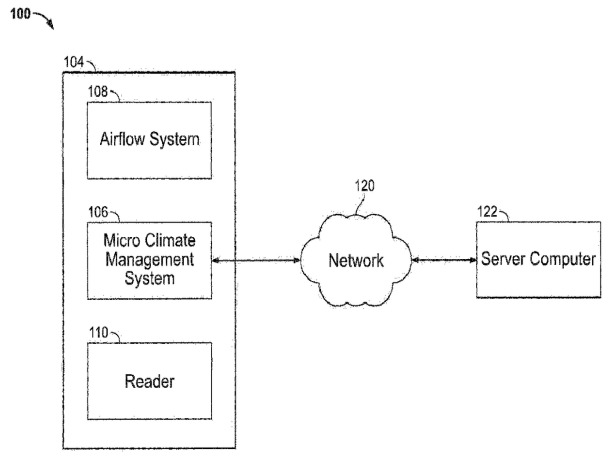


FIG. 1