

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
10 May 2002 (10.05.2002)

PCT

(10) International Publication Number
WO 02/36000 A1

(51) International Patent Classification⁷: **A61B 5/0402**,
5/00, 5/042, A61N 1/05

Street, Foreston, MN 56330 (US). **STROM, James**; 3740
McCracken Lake, Arden Hills, MN 55112 (US).

(21) International Application Number: PCT/US01/31465

(74) Agents: **MCMAHON, Beth, L.** et al.; Medtronic, Inc.
LC340, 710 Medtronic Parkway NE, Minneapolis, MN
55432 (US).

(22) International Filing Date: 5 October 2001 (05.10.2001)

(25) Filing Language: English

(81) Designated States (*national*): CA, JP.

(26) Publication Language: English

(84) Designated States (*regional*): European patent (AT, BE,
CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC,
NL, PT, SE, TR).

(30) Priority Data:
09/703,152 31 October 2000 (31.10.2000) US


Published:
— with international search report
— before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments

(71) Applicant: **MEDTRONIC, INC.** [US/US]; 710
Medtronic Parkway NE, Minneapolis, MN 55432 (US).

For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.

(72) Inventors: **BRABEC, Scott, J.**; 13822 211th Avenue
Northwest, Elk River, MN 55330 (US). **BRENNEN,
Kenneth, R.**; 160 Talmadge Way, Fridley, MN 55432
(US). **SCHINDELDECKER, William**; 15302 145th

(54) Title: SUBCUTANEOUS SPIRAL ELECTRODE FOR SENSING ELECTRICAL SIGNALS OF THE HEART

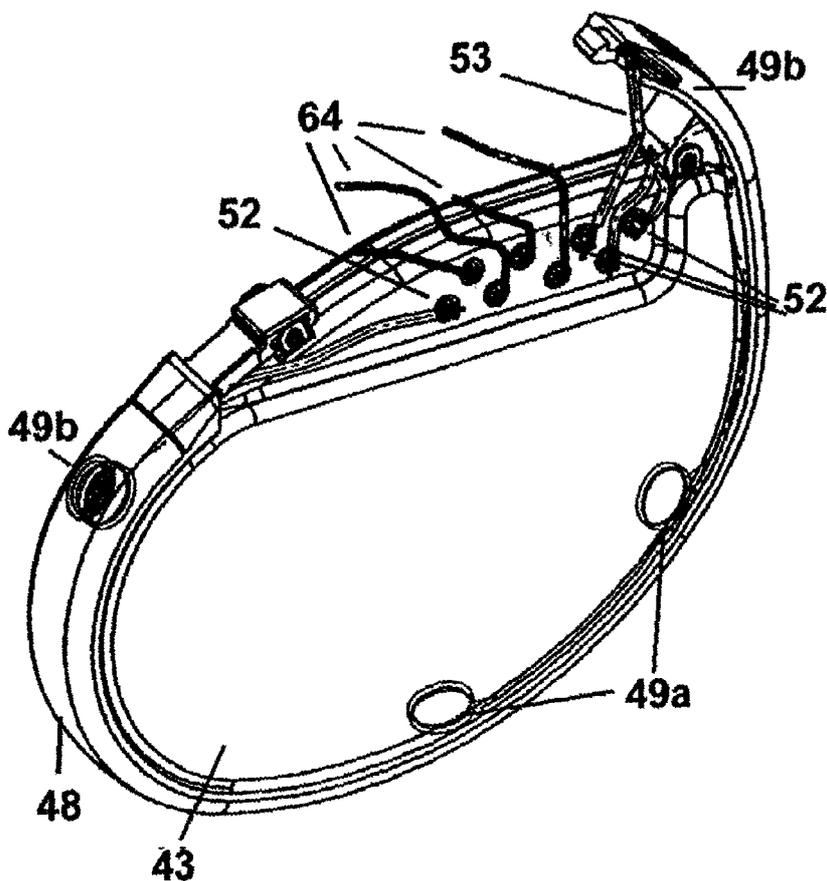

(57) Abstract: An implantable pace-
maker is provided with subcutaneous
spiral electrodes for sensing electrical
signals of the heart. Subcutaneous
spirals or spiral electrodes are
embedded individually into three
or four recessed casings placed in a
compliant surround that is attached
to the perimeter of the implanted
medical device. The electrodes are
electrically connected to the circuitry
of the implanted pacemaker and detect
cardiac depolarization waveforms
displayable as electrocardiographic
tracings on an external instrument such
as a programmer. The spiral electrode
constitutes the proximal end of a
continuous wire that upon egress from
the recessed casing is insulated using
insulative material.

WO 02/36000 A1

SUBCUTANEOUS SPIRAL ELECTRODE FOR SENSING ELECTRICAL SIGNALS OF THE HEART

5 FIELD OF THE INVENTION

The present invention relates generally to implantable pacemakers and more particularly to a subcutaneous electrode used to sense, record, and acquire electrocardiographic data and waveform tracings from an implanted pacemaker without the need for or use of surface (skin) electrodes. More particularly, the present invention relates to spiral electrodes
10 placed into recesses incorporated within a compliant, insulative "surround." Each spiral electrode becomes an integral element of a Subcutaneous Electrode Array or SEA that, in turn, detects cardiac depolarizations communicable and displayable by a portable device programmer.

15 BACKGROUND OF THE INVENTION

The electrocardiogram (ECG) is commonly used in medicine to determine the status of the electrical conduction system of the human heart. As practiced, an ECG recording device is commonly attached to the patient via ECG leads connected to pads arrayed on the patient's body so as to achieve a recording that displays the cardiac waveforms in any one
20 of 12 possible vectors.

Since the implantation of the first cardiac pacemaker, implantable medical device technology has advanced with the development of sophisticated, programmable cardiac pacemakers, pacemaker-cardioverter-defibrillator arrhythmia control devices and drug administration devices designed to detect arrhythmias and apply appropriate therapies. The
25 detection and discrimination between various arrhythmic episodes in order to trigger the delivery of an appropriate therapy is of considerable interest. Prescription for implantation and programming of the implanted device are based on the analysis of the PQRST electrocardiogram (ECG) and the electrogram (EGM). The waveforms are usually separated for such analysis into the P-wave and R-wave in systems that are designed to
30 detect the depolarization of the atrium and ventricle respectively. Such systems employ detection of the occurrence of the P-wave and R-wave, analysis of the rate, regularity, and onset of variations in the rate of recurrence of the P-wave and R-wave, the morphology of

the P-wave and R-wave and the direction of propagation of the depolarization represented by the P-wave and R-wave in the heart. The detection, analysis and storage of such EGM data within implanted medical devices are well known in the art. Acquisition and use of ECG tracing(s), on the other hand, has generally been limited to the use of an external ECG recording machine attached to the patient via surface electrodes of one sort or another.

The aforementioned ECG systems that utilize detection and analysis of the PQRST complex are all dependent upon the spatial orientation and number of electrodes available near or around the heart to pick up the depolarization wave front.

As the functional sophistication and complexity of implantable medical device systems increased over the years, it has become increasingly more important for such systems to include a system for facilitating communication between one implanted device and another implanted device and/or an external device, for example, a programming console, monitoring system, or the like. For diagnostic purposes, it is desirable that the implanted device be able to communicate information regarding the device's operational status and the patient's condition to the physician or clinician. State of the art implantable devices are available which can even transmit a digitized electrical signal to display electrical cardiac activity (e.g., an ECG, EGM, or the like) for storage and/or analysis by an external device. The surface ECG, however, has remained the standard diagnostic tool since the very beginning of pacing and remains so today.

To diagnose and measure cardiac events, the cardiologist has several tools from which to choose. Such tools include twelve-lead electrocardiograms, exercise stress electrocardiograms, Holter monitoring, radioisotope imaging, coronary angiography, myocardial biopsy, and blood serum enzyme tests. Of these, the twelve-lead electrocardiogram (ECG) is generally the first procedure used to determine cardiac status prior to implanting a pacing system; thereafter, the physician will normally use an ECG available through the programmer to check the pacemaker's efficacy after implantation. Such ECG tracings are placed into the patient's records and used for comparison to more recent tracings. It must be noted, however, that whenever an ECG recording is required (whether through a direct connection to an ECG recording device or to a pacemaker programmer), external electrodes and leads must be used.

Unfortunately, surface electrodes have some serious drawbacks. For example, electrocardiogram analysis performed using existing external or body surface ECG systems can be limited by mechanical problems and poor signal quality. Electrodes attached externally to the body are a major source of signal quality problems and analysis errors because of susceptibility to interference such as muscle noise, power line interference, high frequency communication equipment interference, and baseline shift from respiration. Signal degradation also occurs due to contact problems, ECG waveform artifacts, and patient discomfort. Externally attached electrodes are subject to motion artifacts from positional changes and the relative displacement between the skin and the electrodes. Furthermore, external electrodes require special skin preparation to ensure adequate electrical contact. Such preparation, along with positioning the electrode and attachment of the ECG lead to the electrode needlessly prolongs the pacemaker follow-up session. One possible approach is to equip the implanted pacemaker with the ability to detect cardiac signals and transform them into a tracing that is the same as or comparable to tracings obtainable via ECG leads attached to surface electrodes.

It is known in the art to monitor electrical activity of the human heart for diagnostic and related medical purposes. U.S. Pat. No. 4,023,565 issued to Ohlsson describes circuitry for recording ECG signals from multiple lead inputs. Similarly, U.S. Pat. No. 4,263,919 issued to Levin, U.S. Pat. No. 4,170,227 issued to Feldman, et al, and U.S. Pat. No. 4,593,702 issued to Kepski, et al, describe multiple electrode systems that combine surface EKG signals for artifact rejection.

The primary use for multiple electrode systems in the prior art appears to be vector cardiography from ECG signals taken from multiple chest and limb electrodes. This is a technique whereby the direction of depolarization of the heart is monitored, as well as the amplitude. U.S. Pat. No. 4,121,576 issued to Greensite discusses such a system.

Numerous body surface ECG monitoring electrode systems have been employed in the past in detecting the ECG and conducting vector cardiographic studies. For example, U.S. Pat. No. 4,082,086 issued to Page, et al., discloses a four electrode orthogonal array that may be applied to the patient's skin both for convenience and to ensure the precise orientation of one electrode to the other. U.S. Pat. No. 3,983,867 issued to Case describes a vector cardiography system employing ECG electrodes disposed on the patient in normal

locations and a hex axial reference system orthogonal display for displaying ECG signals of voltage versus time generated across sampled bipolar electrode pairs.

U.S. Pat. No. 4,310,000 to Lindemans and U.S. Pat. Nos. 4,729,376 and 4,674,508 to DeCote, incorporated herein by reference, disclose the use of a separate passive sensing reference electrode mounted on the pacemaker connector block or otherwise insulated from the pacemaker case in order to provide a sensing reference electrode that is not part of the stimulation reference electrode and thus does not have residual after-potentials at its surface following delivery of a stimulation pulse.

Moreover, in regard to subcutaneously implanted EGM electrodes, the aforementioned Lindemans U.S. Pat. No. 4,310,000 discloses one or more reference sensing electrode positioned on the surface of the pacemaker case as described above. U.S. Pat. No. 4,313,443 issued to Lund describes a subcutaneously implanted electrode or electrodes for use in monitoring the ECG.

U.S. Pat. No. 5,331,966 to Bennett, incorporated herein by reference, discloses a method and apparatus for providing an enhanced capability of detecting and gathering electrical cardiac signals via an array of relatively closely spaced subcutaneous electrodes (located on the body of an implanted device).

Patent application No XXXXX, "Surround Shroud Connector And Electrode Housings For A Subcutaneous Electrode Array And Leadless ECGs," by Ceballos et al., incorporated herein by reference, discloses an apparatus for providing a compliant surround circumferentially placed around the pacemaker 's perimeter and equipped with recesses for various types of electrodes used to detect cardiac depolarization waves. It is in conjunction with this compliant shroud that the present invention is practiced.

SUMMARY OF THE INVENTION

The present invention encompasses a Subcutaneous Electrode Spiral, Spiral Electrode, as a preferred embodiment, that is embedded individually into three or four recessed casings placed in a compliant surround that is attached to the perimeter of an implanted pacemaker. These electrodes are electrically connected to the circuitry of the implanted pacemaker and detect cardiac depolarization waveforms displayable as electrocardiographic tracings on the pacemaker Programmer screen when the

programming head is positioned above an implanted pacemaker (or other implanted device) so equipped with a leadless Subcutaneous Electrode Array (SEA).

The recessed casing is composed of a polymer. This casing has walls into which body fluid is allowed to flow so that the body fluid is above and around the spiral, spiral coil, which is maintained within the casing by a small circumferential well constructed into the base of the recessed casing. The spiral coil may be constructed from any of the titanium group of metals, as well as platinum, platinum alloys, or any of the platinum group of metals with or without alloying components. This spiral coil constitutes the proximal end of a continuous wire that, upon egress from the recessed casing, is insulated by tubular, insulative material such as silicone. The insulated tubular wiring fits into channel(s) located on the inner arc of the aforementioned compliant surround. The distal end of this wire is welded to a connector feedthrough assembly in contact with amplifier(s) in the microprocessor circuitry.

The present invention is designed to solve several problems that may be encountered in the use of subcutaneous electrodes generally. The electrical potentials from the cardiac depolarizations are very small, in the order of tens of microvolts. As a result, the signal that reaches the electrodes may have a low slew rate. Solid, plate electrodes exhibit noise spikes and potential drifts that are large in comparison to the cardiac signals. These plate electrodes themselves may be the major contributors to such noise. Contamination of electrode surfaces at the molecular level may cause extraneous voltage excursions large enough to interfere with the sensing function. Motion artifacts from the perturbation caused by fluid or tissue motion next to the surface has been demonstrated in tank tests, and represents a commonly observed phenomenon.

The present invention, in its preferred embodiment, solves these issues in that it is a spiral, subcutaneous electrode that can be attached to a pulse generator via a compliant surround and provide a reliable response. The electrode has a large surface area, is manufactured from low cost materials, and can be assembled in an inexpensive way. The surface of the electrode has no direct contact with body tissue and moving body fluids, but it is treated with electrode coatings such as platinum black or titanium nitride to enhance its signal-conducting and depolarization properties. Such enhancing coatings are important since, as time passes, the pacemaker and, with it, the electrodes become

encapsulated in scar tissue and thus come into indirect contact with the body tissue. Even indirect tissue contact may have a damping effect on the detection ability of the electrode if not treated with enhancing coatings.

5 The electrode, as designed, affords a continuous wire connection, without weld or bonds on the electrode surface. Moreover, the electrode is anchored in the device free of any chemical bonding that might cause potential excursions due to electro active species being released to the electrode surface. The portion of the electrode covered by the recessed casing is minimal thereby preventing any potential excursions caused by fluid creep or by trapped oxygen or hydrogen gradients, or P_H gradients. A second embodiment of the present invention employs a coiled electrode design that is manufactured in a rectangular configuration. This electrode has all the same electrical and signal detection properties as the spiral electrode and is constructed of the same materials and has the same enhancing coatings.

10 A third embodiment of the present invention uses a flat plated electrode embedded within the well of the recessed casing. To mechanically stabilize the electrode and reduce the possibility of electro kinetic potential disturbances on the electrode (due to tissue or fluid motion artifact), the bottom of the recess or well is patterned with a cross hatch of elevations and depressions with a minimum of contact area between the plate and the polymer used in the recessed casing. The purpose of the crosshatch is to support the electrode and provide fluid contact to the underside of the electrode interface.

15 A protective cap, vented to allow fluid ingress to the active electrode element, may be placed over the well containing the flat electrode. This cap applies pressure on the electrode, pressing it against the textured bottom of the recess or well, thus preventing motion of the electrode. This cap also serves to dampen any external fluid motion that might otherwise reach the electrode and cause electro kinetic potential transients. The electrodes' surfaces require protection during handling as well as to prevent contamination. A coating, such as may be provided by Dexamethazone Sodium Phosphate, provides such protection as well as enhancing the wetting of the electrode surface after implant. Conductive hydro gels, applied wet and allowed to dry, may also be applied to the electrode surfaces to protect them from damage during handling and prevent contamination.

The spacing of the electrodes in the present invention around the compliant surround provides maximal electrode spacing and, at the same time, appropriate insulation from the pacemaker casing due to the insulative properties of the surround and the cup recesses into which the electrodes are placed. The positioning maintains a maximum and equal distance
5 between the electrode pairs. Such spacing with the four-electrode embodiment maintains the maximum average signal due to the fact that the spacing of the two vectors is equal and the angle between these vectors is 90, as is shown in mathematical modeling. Such orthogonal spacing of the electrode pairs also minimizes signal variation. An alternate three-electrode embodiment has the electrodes arranged within the shroud in an equilateral
10 triangle along the perimeter of the implanted pacemaker. Vectors in this embodiment can be combined to provide adequate sensing of cardiac signals (ECGs).

The present invention allows the physician or medical technician to perform leadless follow-up that, in turn, eliminates the time it takes to attach external leads to the patient. Such timesavings can reduce the cost of follow-up, as well as making it possible for the
15 physician or medical technician to see more patients during each day. Though not limited to these, other uses include: Holter monitoring with event storage, arrhythmia detection and monitoring, capture detection, ischemia detection and monitoring (S-T elevation and suppression on the ECG), changes in QT interval, and transtelephonic monitoring.

20 BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an illustration of a body-implantable device system in accordance with the present invention, including a hermetically sealed device implanted in a patient and an external programming unit.

FIG. 2 is a perspective view of the external programming unit of FIG. 1.

FIG. 3 is a block diagram of the implanted device from FIG. 1.

FIG. 4 is a sectional view of surround shroud displaying electrical connections of the electrodes to the hybrid circuitry.

FIG. 5 is a cross sectional view of a spiral coil, which is one embodiment of an electrode practiced in the present invention.

FIG. 6 is a cross sectional view of spiral coil housed in a well at the base of a recessed casing.

FIG. 7 is a cross sectional view of a recessed cup that employs a cross hatch of elevations and depressions in the well at the base of the cup.

FIG. 8 is a cross sectional view of a vented protective cap fitting over and into the recessed cup.

5 FIG.9 is a cross sectional view of rectangular coil electrodes.

DETAILED DESCRIPTION OF THE DRAWINGS

FIG. 1 is an illustration of an implantable medical device system adapted for use in accordance with the present invention. The medical device system shown in FIG. 1
10 includes an implantable device 10a pacemaker in this embodiment which has been implanted in a patient 12. In accordance with conventional practice in the art, pacemaker 10 is housed within a hermetically sealed, biologically inert outer casing, which may itself be conductive so as to serve as an indifferent electrode in the pacemaker's pacing/sensing circuit. One or more pacemaker leads, collectively identified with reference numeral 14 in
15 FIG. 1 are electrically coupled to pacemaker 10 in a conventional manner and extend into the patient's heart 16 via a vein 18. Disposed generally near the distal end of leads 14 are one or more exposed conductive electrodes for receiving electrical cardiac signals and/or for delivering electrical pacing stimuli to heart 16. As will be appreciated by those of ordinary skill in the art, leads 14 may be implanted with its distal end situated in the
20 atrium and/or ventricle of heart 16.

Although the present invention will be described herein in one embodiment which includes a pacemaker, those of ordinary skill in the art having the benefit of the present disclosure will appreciate that the present invention may be advantageously practiced in connection with numerous other types of implantable medical device systems, and indeed
25 in any application in which it is desirable to provide a communication link between two physically separated components.

Also depicted in FIG. 1 is an external programming unit 20 for non-invasive communication with implanted device 10 via uplink and downlink communication channels, to be hereinafter described in further detail. Associated with programming unit
30 20 is a programming head 22, in accordance with conventional medical device programming systems, for facilitating two-way communication between implanted device

10 and programmer 20. In many known implantable device systems, a programming head
such as that depicted in FIG. 1 is positioned on the patient's body over the implant site of
the device (usually within 2- to 3-inches of skin contact), such that one or more antennae
within the head can send RF signals to, and receive RF signals from, an antenna disposed
5 within the hermetic enclosure of the implanted device or disposed within the connector
block of the device, in accordance with common practice in the art.

In FIG. 2, there is shown a perspective view of programming unit 20 in accordance
with the presently disclosed invention. Internally, programmer 20 includes a processing
unit (not shown in the Figures) that in accordance with the presently disclosed invention is
10 a personal computer type motherboard, e.g., a computer motherboard including an Intel
Pentium 3 microprocessor and related circuitry such as digital memory. The details of
design and operation of the programmer's computer system will not be set forth in detail in
the present disclosure, as it is believed that such details are well-known to those of
ordinary skill in the art.

15 Referring to FIG. 2, programmer 20 comprises an outer housing 60, which is
preferably made of thermal plastic or another suitably rugged yet relatively light-weight
material. A carrying handle, designated generally as 62 in FIG. 2, is integrally formed into
the front of housing 60. With handle 62, programmer 20 can be carried like a briefcase.

20 An articulating display screen 64 is disposed on the upper surface of housing 60.
Display screen 64 folds down into a closed position (not shown) when programmer 20 is
not in use, thereby reducing the size of programmer 20 and protecting the display surface
of display 64 during transportation and storage thereof.

25 A floppy disk drive is disposed within housing 60 and is accessible via a disk
insertion slot (not shown). A hard disk drive is also disposed within housing 60, and it is
contemplated that a hard disk drive activity indicator, (e.g., an LED, not shown) could be
provided to give a visible indication of hard disk activation.

30 As would be appreciated by those of ordinary skill in the art, it is often desirable to
provide a means for determining the status of the patient's conduction system. Normally,
programmer 20 is equipped with external ECG leads 24. It is these leads which are
rendered redundant by the present invention.

In accordance with the present invention, programmer 20 is equipped with an internal printer (not shown) so that a hard copy of a patient's ECG or of graphics displayed on the programmer's display screen 64 can be generated. Several types of printers, such as the AR-100 printer available from General Scanning Co., are known and commercially available.

In the perspective view of FIG. 2, programmer 20 is shown with articulating display screen 64 having been lifted up into one of a plurality of possible open positions such that the display area thereof is visible to a user situated in front of programmer 20. Articulating display screen is preferably of the LCD or electro-luminescent type, characterized by being relatively thin as compared, for example, a cathode ray tube (CRT) or the like.

As would be appreciated by those of ordinary skill in the art, display screen 64 is operatively coupled to the computer circuitry disposed within housing 60 and is adapted to provide a visual display of graphics and/or data under control of the internal computer.

Programmer 20 described herein with reference to FIG. 2 is described in more detail in U.S. Pat. No. 5,345,362 issued to Thomas J. Winkler, entitled "Portable Computer Apparatus With Articulating Display Panel," which patent is hereby incorporated herein by reference in its entirety. The Medtronic Model 9790 programmer is the implantable device-programming unit with which the present invention may be advantageously practiced.

FIG. 3 is a block diagram of the electronic circuitry that makes up pulse generator 10 in accordance with the presently disclosed invention. As can be seen from FIG. 3, pacemaker 10 comprises a primary stimulation control circuit 20 for controlling the device's pacing and sensing functions. The circuitry associated with stimulation control circuit 20 may be of conventional design, in accordance, for example, with what is disclosed Pat. No. 5,052,388 issued to Sivula et al., "Method and apparatus for implementing activity sensing in a pulse generator." To the extent that certain components of pulse generator 10 are conventional in their design and operation, such components will not be described herein in detail, as it is believed that design and implementation of such components would be a matter of routine to those of ordinary skill in the art. For example, stimulation control

circuit 20 in FIG. 3 includes sense amplifier circuitry 24, stimulating pulse output circuitry 26, a crystal clock 28, a random-access memory and read-only memory (RAM/ROM) unit 30, and a central processing unit (CPU) 32, all of which are well-known in the art.

Pacemaker 10 also includes internal communication circuit 34 so that it is capable
5 communicating with external programmer/control unit 20, as described in Fig. 2 in greater detail.

With continued reference to FIG. 3, pulse generator 10 is coupled to one or more leads 14 which, when implanted, extend transvenously between the implant site of pulse generator 10 and the patient's heart 16, as previously noted with reference to FIG. 1.

10 Physically, the connections between leads 14 and the various internal components of pulse generator 10 are facilitated by means of a conventional connector block assembly 11, shown in FIG. 1. Electrically, the coupling of the conductors of leads and internal electrical components of pulse generator 10 may be facilitated by means of a lead interface circuit 19 which functions, in a multiplexer-like manner, to selectively and dynamically
15 establish necessary connections between various conductors in leads 14, including, for example, atrial tip and ring electrode conductors ATIP and ARING and ventricular tip and ring electrode conductors VTIP and VRING, and individual electrical components of pulse generator 10, as would be familiar to those of ordinary skill in the art. For the sake of clarity, the specific connections between leads 14 and the various components of pulse
20 generator 10 are not shown in FIG. 3, although it will be clear to those of ordinary skill in the art that, for example, leads 14 will necessarily be coupled, either directly or indirectly, to sense amplifier circuitry 24 and stimulating pulse output circuit 26, in accordance with common practice, such that cardiac electrical signals may be conveyed to sensing circuitry 24, and such that stimulating pulses may be delivered to cardiac tissue, via leads 14. Also
25 not shown in FIG. 3 is the protection circuitry commonly included in implanted devices to protect, for example, the sensing circuitry of the device from high voltage stimulating pulses.

As previously noted, stimulation control circuit 20 includes central processing unit 32 which may be an off-the-shelf programmable microprocessor or micro controller, but in
30 the present invention is a custom integrated circuit. Although specific connections between CPU 32 and other components of stimulation control circuit 20 are not shown in

FIG. 3, it will be apparent to those of ordinary skill in the art that CPU 32 functions to control the timed operation of stimulating pulse output circuit 26 and sense amplifier circuit 24 under control of programming stored in RAM/ROM unit 30. It is believed that those of ordinary skill in the art will be familiar with such an operative arrangement.

5 With continued reference to FIG. 3, crystal oscillator circuit 28, in the presently preferred embodiment a 32,768-Hz crystal controlled oscillator, provides main timing clock signals to stimulation control circuit 20. Again, the lines over which such clocking signals are provided to the various timed components of pulse generator 10 (e.g., microprocessor 32) are omitted from FIG. 3 for the sake of clarity.

10 It is to be understood that the various components of pulse generator 10 depicted in FIG. 3 are powered by means of a battery (not shown) which is contained within the hermetic enclosure of pacemaker 10, in accordance with common practice in the art. For the sake of clarity in the Figures, the battery and the connections between it and the other components of pulse generator 10 are not shown.

15 Stimulating pulse output circuit 26, which functions to generate cardiac stimuli under control of signals issued by CPU 32, may be, for example, of the type disclosed in U.S. Pat. No. 4,476,868 to Thompson, entitled "Body Stimulator Output Circuit," which patent is hereby incorporated by reference herein in its entirety. Again, however, it is believed that those of ordinary skill in the art could select from among many various types
20 of prior art pacing output circuits that would be suitable for the purposes of practicing the present invention.

Sense amplifier circuit 24, which is of conventional design, functions to receive electrical cardiac signals from leads 14 and to process such signals to derive event signals reflecting the occurrence of specific cardiac electrical events, including atrial contractions
25 (P-waves) and ventricular contractions (R-waves). CPU provides these event-indicating signals to CPU 32 for use in controlling the synchronous stimulating operations of pulse generator 10 in accordance with common practice in the art. In addition, these event-indicating signals may be communicated, via uplink transmission, to external programming unit 20 for visual display to a physician or clinician.

30 Those of ordinary skill in the art will appreciate that pacemaker 10 may include numerous other components and subsystems, for example, activity sensors and associated

circuitry. The presence or absence of such additional components in pacemaker 10, however, is not believed to be pertinent to the present invention, which relates primarily to the implementation and operation of communication subsystem 34 in pacemaker 10, and an associated communication subsystem in external unit 20.

5 FIG. 4 is a sectional view of surround shroud 48 displaying electrical connections of the electrodes to the hybrid circuitry surrounded by insulators 43. Surround displays recessed cups 49b and electrical contacts 49a all of which are connected to the hybrid circuitry (not shown) via tubular wiring 53. Tubular wiring 53 is welded to feedthrough contacts 52 located on upper portion of the board holding the hybrid circuitry. Other contacts 64
10 electrically connect the atrial and ventricular pacing lead tip and ring to the hybrid circuitry.

FIG. 5 is a cross sectional view of spiral coil 61, which is the preferred embodiment of an electrode practiced in the present invention. Spiral coil 61 consists of a wire of titanium or any of the titanium group of metals, platinum, platinum alloy, or any
15 platinum group of metals whose surface may be treated by sputtering, platinization, ion milling, sintering, etching, or a combination of these processes to create a large specific surface area. Spiral coil 61a is designed to fit into recessed well 49c (see FIG. 6), within which spiral coil 61b rests. The protruding end of spiral coil 61c is manufactured continuous with tubular wiring 53 (see FIG. 6). The one-piece continuous design
20 eliminates an additional weld or connection at the actual electrode. The elimination of the weld in this area is significant, because it eradicates the possibility of two dissimilar metals interacting within the ionic environment and adding an erroneous signal to the system. Removing the weld also eliminates any intermetallics formed during the weld.

FIG. 6 is a cross sectional view of spiral coil 61 fitted into well 49c at the base of
25 recessed cup 49b that is fitted into compliant shroud 48 (see FIG 4). Thin film coatings via sputtering (porous TiN), platinization (platinum black), or applications of RuO, ion milling, sintering, etching, or a combination of these processes to create a large specific surface area may be used to treat the surface of spiral coil wire 61. Larger surface areas decrease the interfacial impedance, thereby allowing lower impedances at lower
30 frequencies, thereby increase the signal-to-noise ratio. Wire is manufactured of any of the

titanium group of metals, as well as platinum, platinum alloy, or any of the platinum group of metals, with or without alloying components.

The spaces around spiral coil 61 allow body fluid to flow around, between, and below the metal coils. Body fluids have conductive properties that allow cardiac depolarization waves to reach spiral electrode 61. The depolarization waves are detected as changes in electrical potential and transmitted via continuous tubular wire protected by insulator 63 as wire exits well 49c. Tubular material 53 keeps the wire insulated from other electrical potentials and protects the continuous wire. This continuous, conductive wire carries the signal(s) to the amplifier(s), hybrid circuitry, and microprocessor for processing and conversion into ECG tracings that may be printed by the printer located in programmer 20 (see FIG. 2). Compliant shroud 48 (see FIG. 4) serves to maintain the recessed cup in position relative to other coils which spacing is required for orthogonal or equilateral detection of the cardiac depolarization waves.

FIG. 7 is a cross sectional view of a recessed cup that employs a crosshatch of elevations and depressions 66 in well 49c at base of recessed cup 49b. These elevations and depressions are continuous with the polymer used in the recessed up and well. An alternative electrode embodiment, which may be used with the crosshatched base, employs a thin, solid, spherical electrode 68 that lies on top of crosshatch 66. Viewed from above, crosshatch 67 would appear as shown. Viewed again from above, individual elevations 66a appear as shown on the inset drawing. Turning again to the crosshatch, elevations and depressions 66 mechanically stabilize the electrode and reduce the possibility of electro kinetic potential disturbances on the electrode (tissue or fluid motion artifact). The pattern of crosshatched elevations and depressions provide a minimum contact area between the wire and the polymer used to form the recessed cup 49b and well 49c. The purpose of the crosshatch is to support electrode 68 while providing fluid contact around, between, and below underside of electrode. Body fluids have conductive properties that allow cardiac depolarization waves to reach electrode 68. Since thin, solid, spherical electrode 68 is not continuous with tubular wiring 53, small metal plate 65 bonded or welded to tubular wiring 53 is welded to underside of electrode 68.

Cardiac depolarization waves are detected as changes in electrical potential and transmitted via continuous tubular wire protected by insulator 63 as wire exits well 49c. A

tubular material 53 that keeps the wire insulated from other electrical potentials then protects the continuous wire. This conductive wire carries the signal(s) to the amplifier(s), hybrid circuitry, and microprocessor for processing and conversion into ECG tracings that are printed by the printer located in programmer 20 (FIG. 2). Compliant shroud 48 (see
5 FIG. 4) serves to maintain the recessed cup in position relative to other coils which spacing is required for orthogonal or equilateral detection of the cardiac depolarization waves.

FIG. 8 is a cross sectional view of vented protective cap 69a fitted over and into recessed cup 49b. Protective cap 69a is vented to allow fluid ingress to the active
10 electrode element and is placed over the well 69c containing active electrode 68. This cap slides into recessed cup 49b, contacts electrode 68 and applies pressure 70 on the electrode, pressing it against the crosshatched bottom 66 of well 49c, thus preventing motion of the electrode. The cap, constructed of a polymer such as urethane, also serves to dampen any external fluid motion that might otherwise reach the active element and
15 cause electro kinetic potential transients. A preferred design for the openings in the cap is one in which the support elements all run perpendicular to the elements of the coiled wire, i.e., radially as shown in the drawing 69a.

The ribs in cross section 69b are rounded on top to eliminate sharp edges, presenting a smooth appearance. The outer diameter of the protective cap is sized to
20 provide a sliding fit 69c into the well containing the electrode. The protective cap may then be bonded to the wall of the recessed casing 49b with a suitable bonding agent. The cap and the electrode well must accommodate the wire 53 leading to the hybrid circuitry. A small opening in the side of the recessed casing serves to carry tubular wire from electrode to hybrid circuitry. Insulator 63 serves as anchor for wire 53 while the bonding
25 material to small metal plate 65 serves as a seal.

FIG. 9 shows a cross sectional view of rectangular coil electrode 70 and 71, as well as a
perspective view 72 of the same electrode which is an alternative embodiment of the present invention. Rectangular coil 70 consists of a wire of titanium or any of the titanium
30 group of metals, platinum, platinum alloy, or any platinum group of metals whose surface may be treated by sputtering, platinization, ion milling, sintering, etching, or a combination of these processes to create a large specific surface area. Rectangular coil 70

is designed to fit into a rectangular recessed well 49c (modified from that shown in FIG. 6), within which rectangular coil 71 rests. The protruding end of rectangular coil 70a is manufactured continuous with tubular wiring 53 (see FIG. 6). The one-piece continuous design eliminates an additional weld or connection at the actual electrode. The
5 elimination of the weld in this area is significant, because it eradicates the possibility of two dissimilar metals interacting within the ionic environment and adding an erroneous signal to the system. Removing the weld also eliminates any intermetallics formed during the weld.

10 While particular embodiments of the present invention have been shown and described, modifications may be made, and it is therefore intended in the appended claims to cover all such changes and modifications that fall within the true spirit and scope of the invention.

CLAIMS

- 5 1. An implantable electrocardiographic data collection system for recording electrocardiographic data, the system comprising:
- a hermetically sealed case;
 - a plurality of subcutaneous spiral electrodes forming an array, mounted in a recessed casing formed about a periphery surface of the case; and
- 10 signal processing circuitry inside the case coupled to the electrodes via a connector feedthrough assembly in contact with amplifiers in a microprocessor circuitry.
2. The system of claim 1 wherein said recessed casing is composed of a polymer.
3. The system of claim 2 wherein the case includes walls into which body fluid is
- 15 allowed to flow so that the body fluid is above and around the spiral electrodes and is contained in the casing by a small circumferential well constructed into the base of said recessed casing.
4. The system according to claim 3 wherein the spiral electrodes include spiral coils
- 20 consisting of materials selected from the group of platinum, platinum alloys and platinum group of metals with or without alloy components.
5. The system according to claim 3 wherein said spiral electrodes include a spiral coil forming a proximal end of a continuous wire that upon egress from said recessed casing, is
- 25 insulated by tubular insulative materials.
6. The system according to claim 5 wherein said insulated tubular insulative material feeds into channels located on the inner arc on a compliant surround.

7. The system according to claim 5 wherein a distal end of said continuous wire is welded to connector feedthrough assembly in contact with amplifiers in a microprocessor secretary.

5 8. Apparatus for leadless acquisition of electrocardiographic data using an array of subcutaneous spiral electrodes to detect cardiac depolarization signals that are very small, and signals with low slew rates, the system comprising:

a hermetically sealed case;

10 a plurality of spiral subcutaneous electrodes attached to a pulse generator by a compliant surround, mounted in the periphery surface of the case; and signal processing circuitry inside the case and electrically coupled to the plurality of electrodes to detect cardiac signals and provide electrocardiographic data.

15 9. The apparatus of claim 8 wherein the surface of said plurality of spiral electrodes is isolated from direct contact with body tissue and moving body fluids.

20 10. The apparatus of claim 9 wherein said surface of said electrodes is treated with electrode coating such as platinum black or titanium nitride to enhance signal conducting and depolarization properties.

11. The apparatus of claim 9 wherein said plurality of said electrodes include a continuous wire connection without weld or bonds on the electrode surface.

25 12. The plurality of electrodes of claim 9 wherein said electrodes are anchored in the case, free of any chemical bonding, in a recessed section of the case.

13. The apparatus of claim 12 wherein a portion of said electrode that is covered by said recessed section is minimal to prevent potential excursions caused by fluid creep or by trapped oxygen or hydrogen gradient.

30 14. The apparatus of claim 9 wherein said electrodes include a coiled electrode design in a rectangular configuration.

15. The apparatus of claim 9 wherein said electrodes include a flat plated electrode embedded within a well of said recessed casing.

5 16. The apparatus of claim 15 wherein said flat plated electrode is stabilized against electromagnetic potential disturbances by structuring the bottom of said recessed casing patterned with a cross-hatch structure with elevations and depressions formed to have a minimum contact area between the plate and the polymer used in the recessed casing.

10 17. The apparatus of claim 16 wherein said cross-hatch structure supports said electrode and enables fluid contact with the underside of said electrode surface.

15 18. Apparatus of claim 9 wherein a protective cap is placed to allow fluid to ingress to the active electric element wherein said protective cap is placed over the recessed section containing said flat electrode.

19. The apparatus of claim 18 wherein said cap is structured to apply pressure on said electrode for pressing against said textured bottom of the recessed casing to prevent motion of said electrode.

20 20. The apparatus of claim 19 wherein said cap is structured to dampen external fluid motion that might otherwise reach said electrode and cause electroconnetic transience.

25 21. The apparatus of claim 9 wherein said electrode surface is treated with a coating to protect from contamination during handling.

22. The apparatus of claim 21 wherein said coating includes dexamethasone sodium phosphates to provide protection to enhance the wetting of the electrode surface after implant.

30 23. The apparatus of claim 22 wherein conductive hydro gels are applied to said electrode surface to protect from damage during handling and prevent contamination.

24. The apparatus of claim 8 wherein a spacing of said electrodes around a compliant surround provides maximum electrode spacing.

5 25. The apparatus of claim 24 wherein said spacing maintains a maximum average signal using two equal vectors.

26. The apparatus of claim 25 wherein said spacing of said equal vectors includes a 90° angle vector.

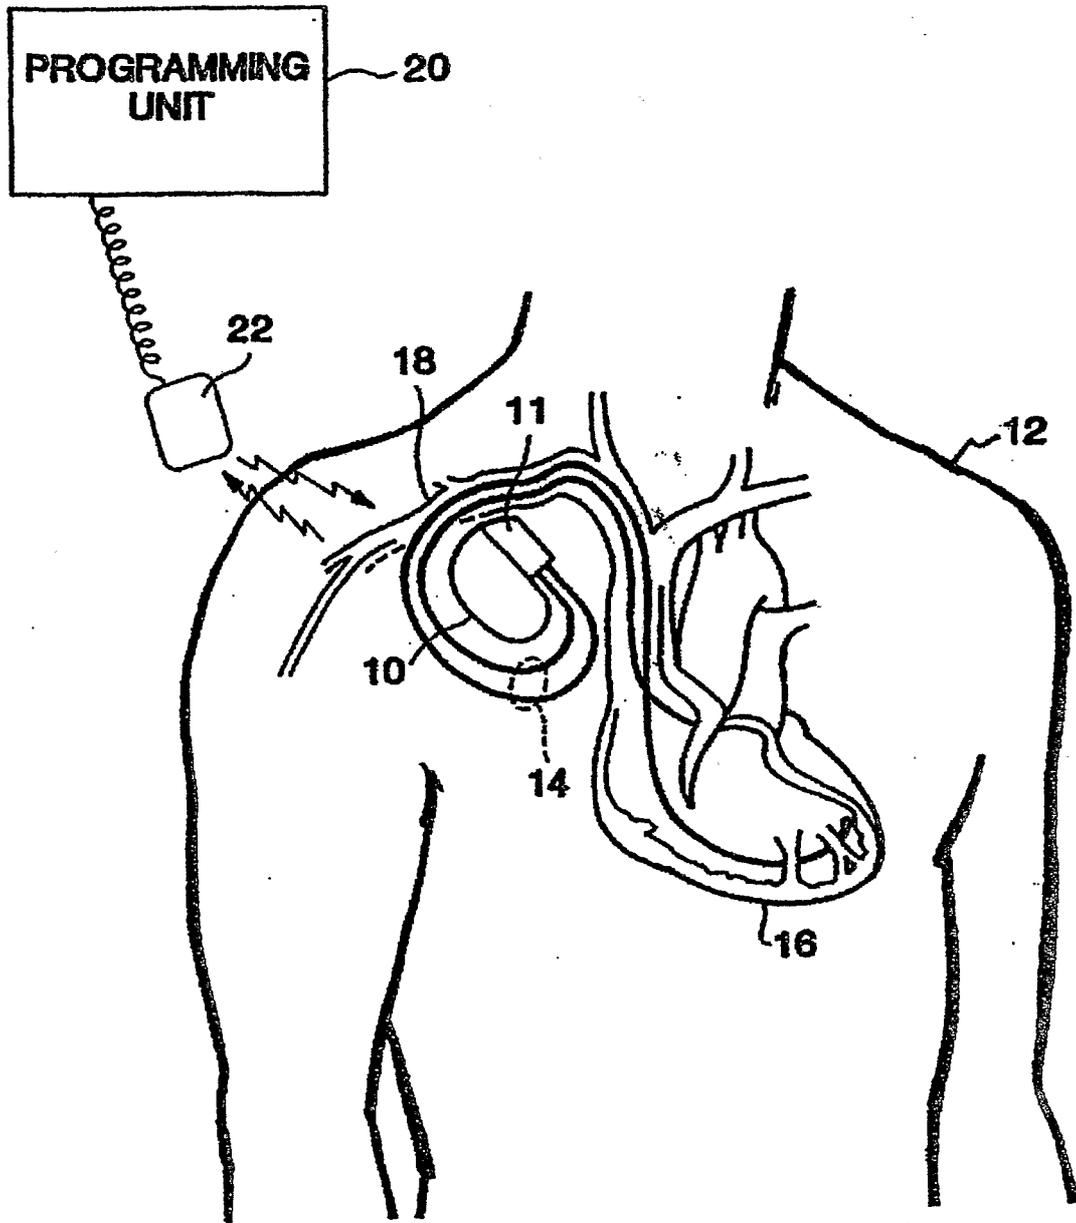


Figure 1

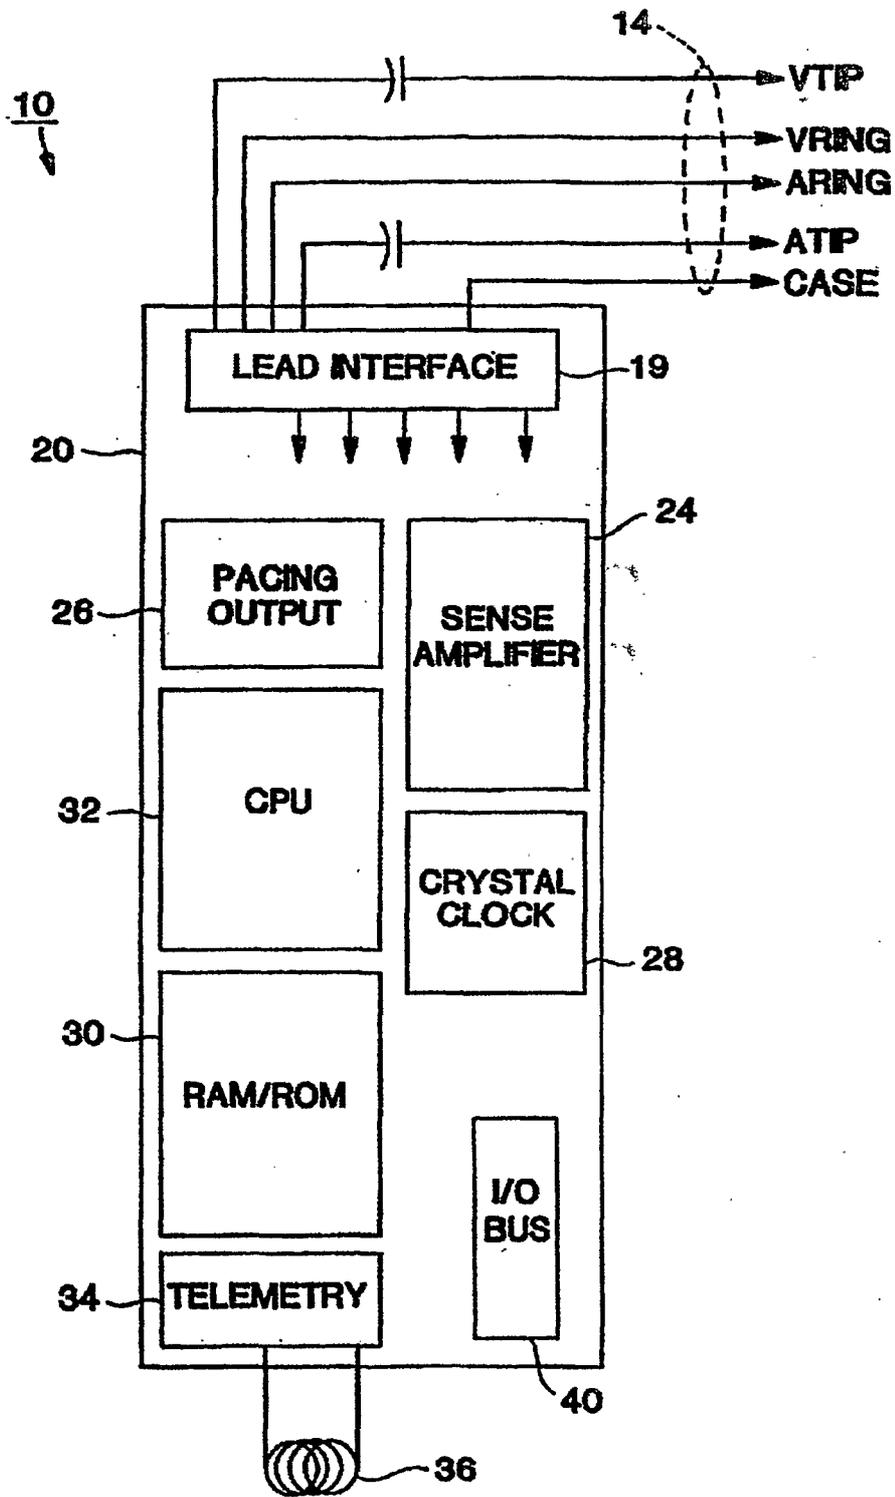


Figure 3

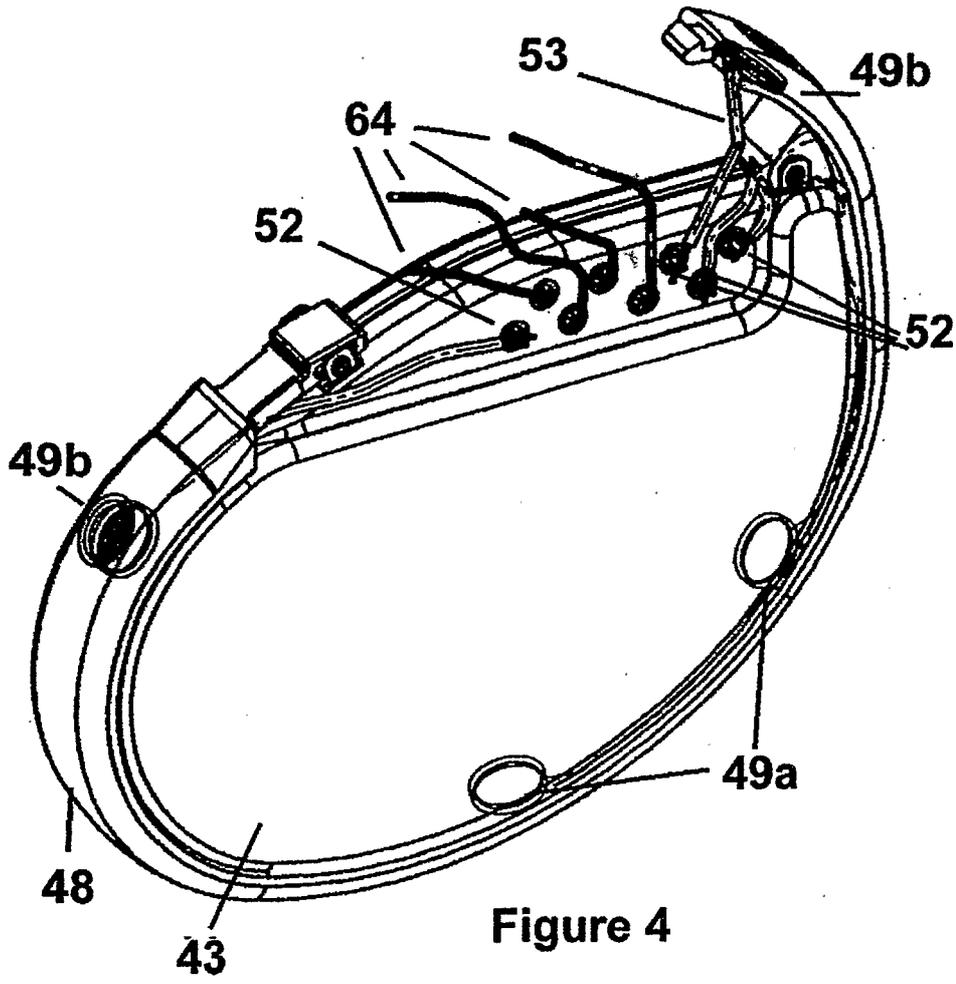


Figure 4

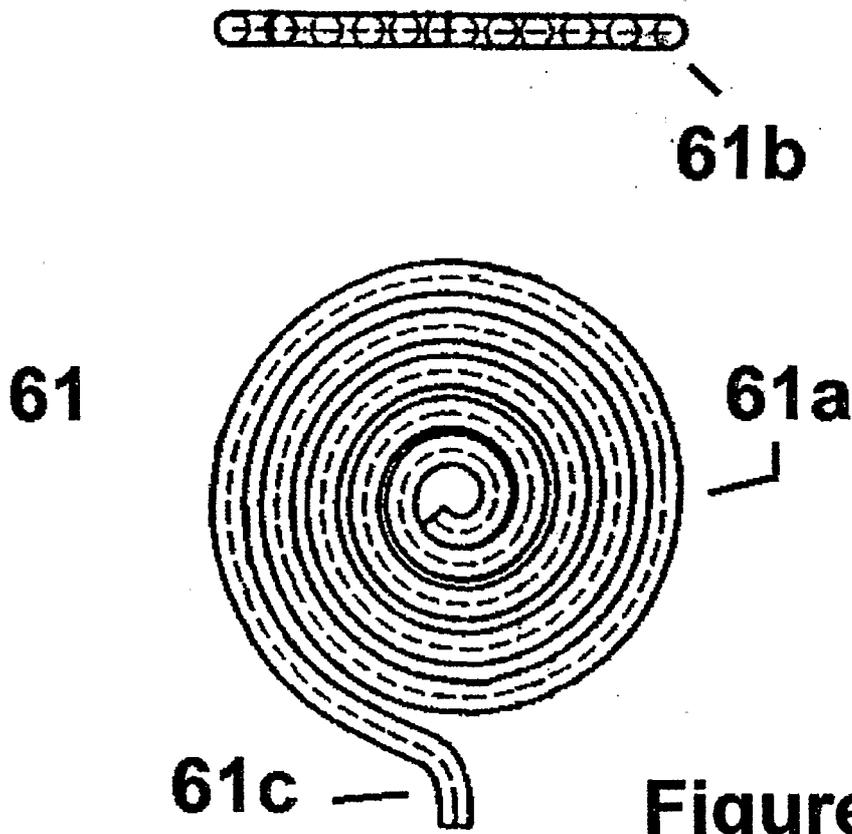


Figure 5

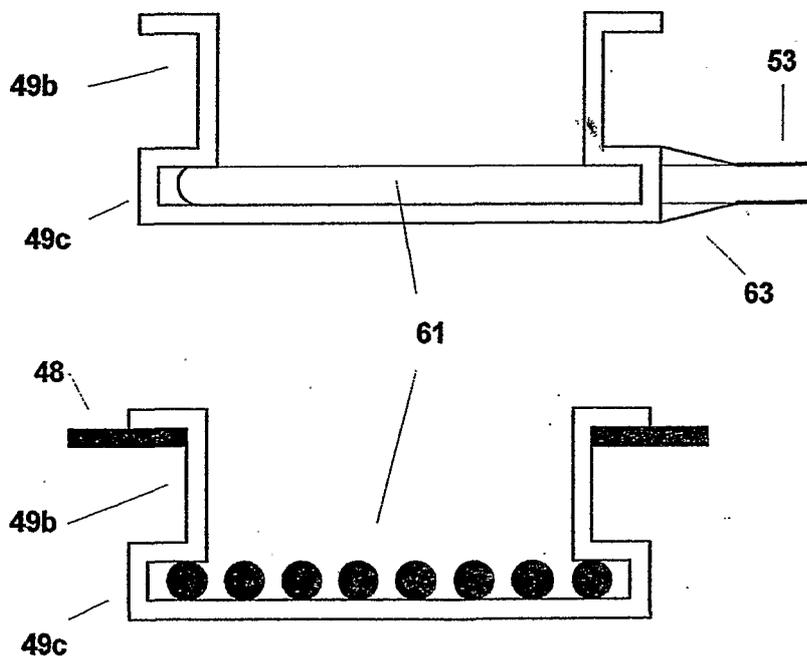


Figure 6

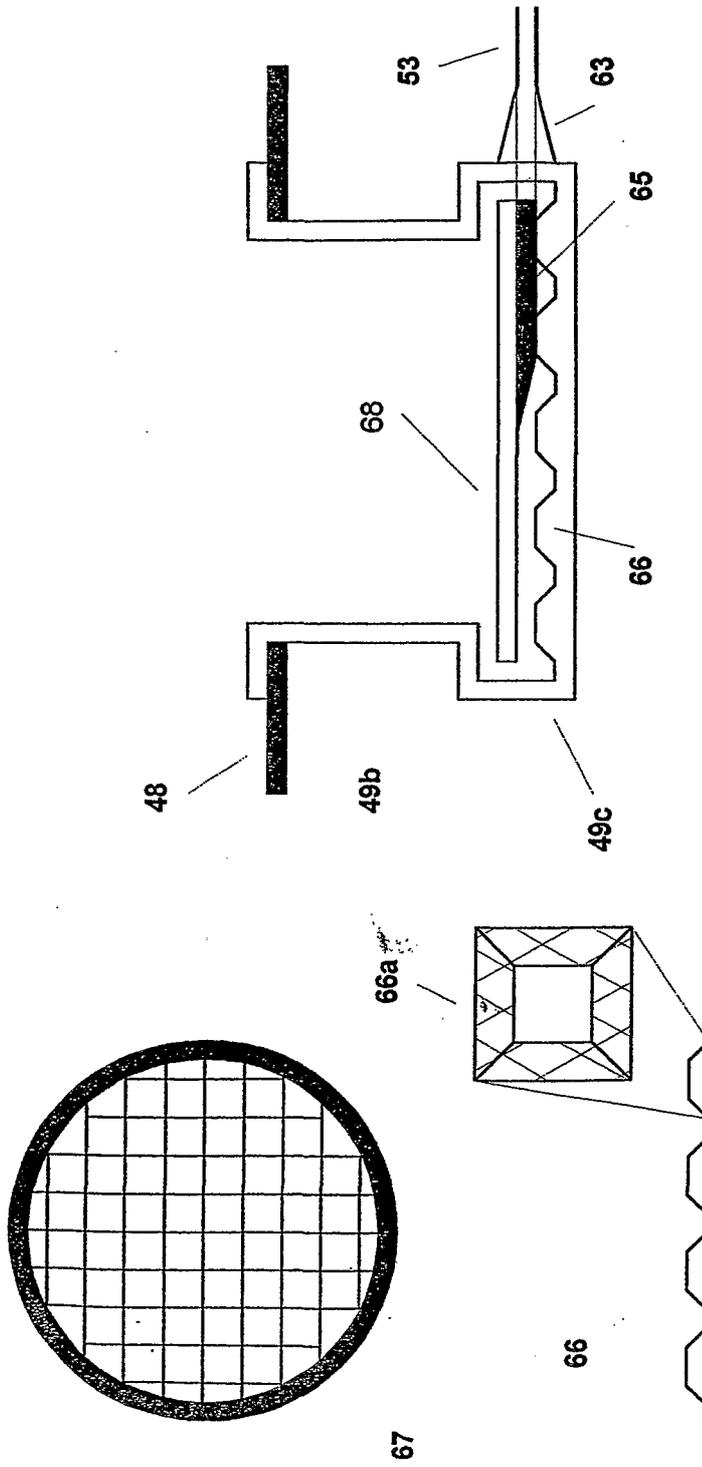


Figure 7

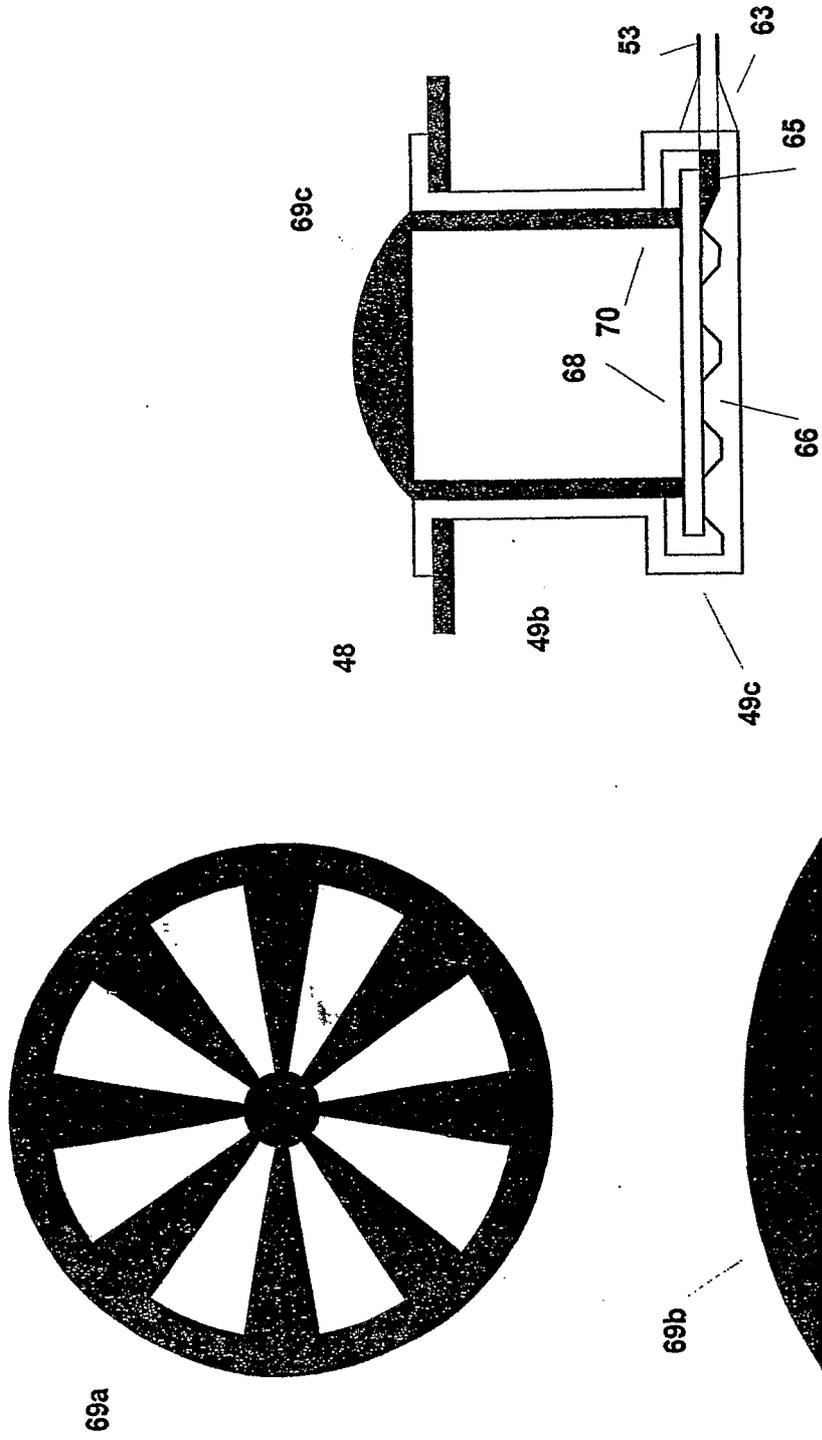


Figure 8

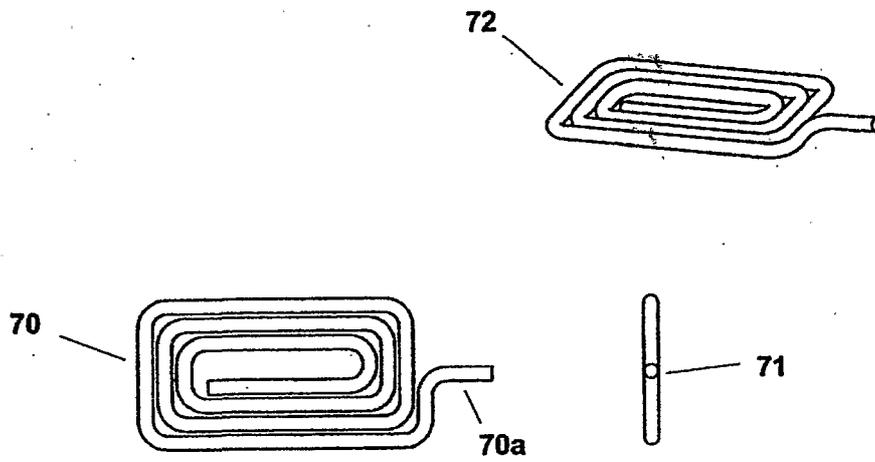


Figure 9

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US 01/31465

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61B5/0402 A61B5/00 A61B5/042 A61N1/05

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61B A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the International search (name of data base and, where practical, search terms used)
EPO-Internal, PAJ, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 0 941 695 A (CARDIAC PACEMAKERS) 15 September 1999 (1999-09-15) description fig 18 abstract	1,8
A	US 6 108 577 A (BENSER MICHAEL ERIC) 22 August 2000 (2000-08-22) description fig 5 column 1, line 57 -column 2, line 15	1,8
A	EP 0 460 324 A (CARDIAC PACEMAKERS) 11 December 1991 (1991-12-11) figure 18	8
P,A	WO 01 70331 A (MEDTRONIC INC) 27 September 2001 (2001-09-27) summary of invention	1,8
	-/--	

Further documents are listed in the continuation of box C. Patent family members are listed in annex.

* Special categories of cited documents:

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed
- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *Z* document member of the same patent family

Date of the actual completion of the international search 26 February 2002	Date of mailing of the international search report 05/03/2002
--	---

Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Authorized officer Papone, F
--	--

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US 01/31465

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
P, A	US 6 272 379 B1 (FISCHELL ROBERT E ET AL) 7 August 2001 (2001-08-07) claims 1-3; figures 1,3 ---	1,8
A	EP 0 472 411 A (TELECTRONICS NV) 26 February 1992 (1992-02-26) -----	

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 01/31465

Information on patent family members

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 0941695	A	15-09-1999	US 5313953 A	24-05-1994
			EP 0941695 A2	15-09-1999
			AU 659518 B2	18-05-1995
			AU 3044792 A	15-07-1993
			CA 2086713 A1	15-07-1993
			CA 2177184 A1	15-07-1993
			EP 0554208 A2	04-08-1993
			JP 6000167 A	11-01-1994
			US 5388578 A	14-02-1995
US 6108577	A	22-08-2000	AU 4664100 A	10-11-2000
			WO 0064534 A1	02-11-2000
EP 0460324	A	11-12-1991	US 5203348 A	20-04-1993
			CA 2027744 A1	07-12-1991
			DE 69026081 D1	25-04-1996
			EP 0460324 A2	11-12-1991
			JP 1851562 C	21-06-1994
			JP 4040966 A	12-02-1992
			JP 5067310 B	24-09-1993
			US 5545202 A	13-08-1996
			US 5603732 A	18-02-1997
			US 5342407 A	30-08-1994
			US 5230337 A	27-07-1993
			US 5360442 A	01-11-1994
WO 0170331	A	27-09-2001	WO 0170331 A2	27-09-2001
US 6272379	B1	07-08-2001	NONE	
EP 0472411	A	26-02-1992	US 5113869 A	19-05-1992
			EP 0472411 A1	26-02-1992

专利名称(译)	用于感测心脏电信号的皮下螺旋电极		
公开(公告)号	EP1331878A1	公开(公告)日	2003-08-06
申请号	EP2001977619	申请日	2001-10-05
[标]申请(专利权)人(译)	美敦力公司		
申请(专利权)人(译)	美敦力公司, INC.		
当前申请(专利权)人(译)	美敦力公司, INC.		
[标]发明人	BRABEC SCOTT J BRENNEN KENNETH R SCHINDELDECKER WILLIAM STROM JAMES		
发明人	BRABEC, SCOTT, J. BRENNEN, KENNETH, R. SCHINDELDECKER, WILLIAM STROM, JAMES		
IPC分类号	A61B5/0408 A61B5/00 A61B5/0402 A61B5/042 A61B5/0478 A61B5/0492 A61N1/05 A61N1/365		
CPC分类号	A61B5/6852 A61B5/0031 A61B5/0422 A61B5/7207 A61B2562/043 A61N1/05		
优先权	09/703152 2000-10-31 US		
其他公开文献	EP1331878B1		
外部链接	Espacenet		

摘要(译)

可植入起搏器设有皮下螺旋电极, 用于感测心脏的电信号。将皮下螺旋或螺旋电极单独地嵌入三个或四个凹入的壳体中, 所述壳体放置在柔性环绕中, 所述柔性环绕物附接到植入的医疗装置的周边。电极电连接到植入的起搏器的电路, 并检测可在诸如编程器的外部仪器上显示为心电图描记的心脏去极化波形。螺旋电极构成连续线的近端, 其在从凹入壳体出口时使用绝缘材料绝缘。