

(19)



(11)

EP 2 440 131 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:

04.04.2018 Bulletin 2018/14

(21) Application number: **10786673.3**

(22) Date of filing: **08.06.2010**

(51) Int Cl.:

A61M 25/01 (2006.01)	A61B 5/055 (2006.01)
A61B 5/00 (2006.01)	G01R 33/28 (2006.01)
A61B 34/10 (2016.01)	A61B 18/14 (2006.01)
A61B 17/00 (2006.01)	A61B 18/00 (2006.01)
A61B 34/00 (2016.01)	A61B 34/20 (2016.01)
A61B 90/00 (2016.01)	A61M 29/00 (2006.01)
A61M 25/00 (2006.01)	A61M 25/06 (2006.01)
A61M 25/09 (2006.01)	

(86) International application number:

PCT/US2010/037734

(87) International publication number:

WO 2010/144419 (16.12.2010 Gazette 2010/50)

(54) MRI-GUIDED INTERVENTIONAL SYSTEMS THAT CAN TRACK AND GENERATE DYNAMIC VISUALIZATIONS OF FLEXIBLE INTRABODY DEVICES IN NEAR REAL TIME

MRT-GESTEUERTE EINGRIFFSSYSTEME ZUR FAST IN ECHTZEIT ERFOLGENDEN VERFOLGUNG UND ERZEUGUNG DYNAMISCHER VISUALISIERUNGEN FLEXIBLER INTRAKORPORALER VORRICHTUNGEN

SYSTÈMES INTERVENTIONNELS GUIDÉS PAR IRM POUVANT LOCALISER DES DISPOSITIFS INTRACORPORELS SOUPLES ET GÉNÉRER DES VISUALISATIONS DYNAMIQUES DE CEUX-CI EN TEMPS QUASI RÉEL

(84) Designated Contracting States:

AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO SE SI SK SM TR

(30) Priority: **08.06.2009 US 185072 P**

16.06.2009 US 187323 P

23.06.2009 US 219638 P

13.11.2009 US 261103 P

(43) Date of publication of application:

18.04.2012 Bulletin 2012/16

(73) Proprietor: **MRI Interventions, Inc.**

Irvine, CA 92618 (US)

(72) Inventors:

- **GUTTMAN, Michael**
Potomac Falls
Virginia 20165 (US)

- **JENKINS, Kimble L.**
Memphis
Tennessee 38111 (US)

- **PIFERI, Peter**
Orange
California 92867 (US)

- **VIJ, Kamal**
Chandler
Arizona 85226 (US)

(74) Representative: **Yeadon IP Limited**

Leeds Innovation Centre
103 Clarendon Road
Leeds LS2 9DF (GB)

(56) References cited:

US-A1- 2002 058 868	US-A1- 2004 015 075
US-A1- 2005 054 910	US-A1- 2006 142 657
US-A1- 2009 118 610	

EP 2 440 131 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD OF THE INVENTION

[0001] The present invention relates to MRI-guided systems and may be particularly suitable for MRI-guided cardiac systems such as EP systems for treating Atrial Fibrillation (AFIB).

BACKGROUND OF THE INVENTION

[0002] Conventional Cardiac EP (ElectroPhysiology) Systems are X-ray based systems which use electroanatomical maps. Electroanatomical maps are virtual representations of the heart showing sensed electrical activity. Examples of such systems include the Carto® electroanatomic mapping system from Biosense Webster, Inc., Diamond Bar, CA, and the EnSite NavX® system from Endocardial Solutions Inc., St. Paul, MN.

[0003] However, there remains a need for MRI-guided systems that can use MRI to obtain details of tissue not provided by X-ray based systems and/or to reduce patient exposure to radiation associated with interventional (diagnostic and/or therapeutic) procedures. An MRI system using optical tracking is shown in US 2005/054910 A1 by Tremblay et al. (Sunnybrook).

SUMMARY OF EMBODIMENTS OF THE INVENTION

[0004] Embodiments of the invention are directed to MRI-guided systems that have a new operational platform. The invention is defined in claim 1 as a system and claim 19 as a computer program product.

[0005] Some embodiments are directed to systems include a circuit configured to: (a) generate at least one near real time (RT) MRI image of at least a portion of a heart of a patient using relevant anatomical scan planes associated with a 3-D MRI image space having a coordinate system; (b) identify coordinates associated with a location of at least a distal portion of at least one flexible intrabody catheter in the 3-D MRI image space; and (c) render interactive near RT visualizations of the at least one flexible catheter in the 3-D image space. The at least one flexible catheter is not required to be in any of the relevant anatomical scan planes used to obtain MR data for the at least one near RT MRI image and the distal end portion of the flexible catheter can take on a curvilinear shape.

[0006] Other embodiments are directed to MRI guided interventional systems. The systems include at least one flexible intrabody interventional or diagnostic medical device configured to be able to take on a non-linear shape and be introduced into a patient via a tortuous and/or natural lumen path, the at least one medical device having at least one tracking coil that is connected to a channel of the MRI scanner; a circuit adapted to communicate with and/or reside in an MRI Scanner; and a display with a User Interface in communication with the circuit con-

figured to display the visualizations during an MRI guided interventional procedure. The circuit is configured to: (a) obtain MR image data and generate a series of near real time (RT) MRI images of target anatomy of a patient during a surgical procedure using relevant anatomical scan planes associated with a 3-D MRI image space having a coordinate system; (b) identify coordinates associated with a location of at least a distal portion of the flexible intrabody medical device using the coordinate system of the 3-D MRI image space; and (c) render near RT interactive visualizations of the at least one flexible medical device in the 3-D image space with at least one near RT image of target patient anatomical structure and a registered pre-acquired volumetric model of the target anatomical structure of the patient. The circuit renders the visualizations to illustrate the at least one flexible medical device with a physical representation in the visualizations. The User Interface is configured to allow a user to (a) rotate the visualizations and (b) alter a displayed visualization to include only a near RT image of the target anatomy, to include the near RT image of the anatomy and the registered model of the anatomical structure, or to include only the registered model of the anatomical structure. The MRI Scanner is configured to interleave signal acquisition of tracking signals from the at least one tracking coil with image data for the near RT MRI images, and wherein the circuit is configured to electronically track the at least one flexible medical device in the 3-D image space independent of scan planes used to obtain the MR image data so that the at least one flexible device is not required to be in any of the relevant anatomical scan planes used to obtain MR image data for the at least one near RT MRI image, and wherein the distal end portion of the flexible medical device can take on a curvilinear shape.

[0007] Yet other embodiments are directed to MRI guided cardiac intervention systems. The systems include an MR Scanner having a plurality of channels; a plurality of flexible intrabody catheters, each having a plurality of tracking coils, each tracking coil of each catheter connected to a different MR Scanner channel; and at least one display in communication with the MR Scanner. The MR Scanner is configured to: (a) generate at least one near real time (RT) MRI image of at least a portion of a heart of a patient using relevant anatomical scan planes associated with a 3-D MRI image space having a coordinate system; (b) identify coordinates associated with a location of at least a distal portion of at least one flexible intrabody catheter in the 3-D MRI image space; and (c) render dynamic near RT visualizations of the at least one flexible catheter in the 3-D image space which show a volumetric pre-acquired model of the patient's heart registered to the imaging space with the near RT MRI image, wherein the at least one flexible catheter is not required to be in any of the relevant anatomical scan planes used to obtain MR image data for the at least one near RT MRI image, and wherein the distal end portion of the flexible catheter can take on a non-linear

shape.

[0008] The circuit may be configured to show at least one of a plurality of user-selectable tissue characteristic maps or data associated therewith on the model or the selected tissue characteristic map in lieu of the model on the display, wherein the display is in communication with a User Interface that is configured to allow a user to selectively turn one or more of the tissue characterization maps on and off. When on, the tissue characteristic map or data therefrom is aligned with and/or registered to the pre-acquired volumetric 3-D model of the patient's heart (or shown in lieu thereof). The selectable tissue characteristic maps include a plurality of the following: a thermal tissue characterization map; an edema tissue characterization map; a first delayed enhancement tissue characterization map; a second delayed enhancement tissue characterization map taken after the first delayed enhancement tissue characterization map; a hypoxic tissue characterization map; a vasculature map; a fibrous map; and an ischemic tissue characterization map.

[0009] Still other embodiments are directed to MRI guided cardiac interventional systems. The systems include: a display; a processor in communication with the display and adapted to communicate with a MRI scanner; electronic memory coupled to the processor; and computer program code residing in the memory that is executable by the processor for:

- (a) generating at least one near real time (RT) MRI image of at least a portion of a heart of a patient using relevant anatomical scan planes associated with a 3-D MRI image space having a coordinate system;
- (b) identifying coordinates associated with a location of at least a distal portion of at least one flexible intrabody catheter in the 3-D MRI image space to track a location of a distal end portion of the catheter;
- (c) rendering dynamic near RT visualizations of the at least one flexible catheter in the 3-D image space, wherein the at least one flexible catheter is not required to be in any of the relevant anatomical scan planes used to obtain MR data for the at least one near RT MRI image, and wherein the distal end portion of the flexible catheter can take on a non-linear shape;
- (d) displaying a graphical user interface (GUI) containing at least one of the visualizations within the display; and
- (e) allowing a user to alter the visualizations using the GUI to selectively show different tissue characteristic maps or data from the selected tissue characteristic map.

[0010] The computer program code that is executable by the processor may be further adapted to automatically define at least one scan plane used by the MRI scanner for a target catheter-tissue interface site before and/or during the ablating step based on the tracked location of

the of the catheter.

[0011] The tissue characterization map is color-coded to show scar or lesion formations associated with ablation sites created during the procedure.

[0012] Still other embodiments are directed to methods for carrying out an MRI-guided procedure. The methods include: (a) introducing a flexible intrabody medical device into a natural lumen or cavity of a patient during an MRI-guided procedure; (b) electronically obtaining tracking signals from tracking coils connected to an MR Scanner and attached to the flexible intrabody device during the MRI-guided procedure, wherein the intrabody device has a distal end portion that can take on a non-linear shape as it moves into position in the patient's body; (c) electronically identifying X, Y, Z coordinate locations in 3-D MRI image space of each of the tracking coils using the tracking signals; (d) obtaining MR image data and generating near RT MR images of the patient during the MRI-guided procedure; (e) obtaining a pre-acquired 3-D volumetric model of target anatomy of the patient and registering the model to the 3-D image space; and (f) generating near real time (RT) visualizations of the medical device showing: (i) the registered model of the patient's anatomy; (ii) a physical representation of at least a distal end portion of the medical device using the identified locations of the tracking coils; and (iii) at least one of the near RT MR images.

[0013] The method may further include electronically calculating a device-tissue interface location proximate a tip location of the device in the three dimensional image space using the identified locations of the tracking coils, wherein the calculating step projects axially forward a defined distance beyond the tip to define the device-tissue interface; and automatically defining at least one scan plane used to obtain the MR image data for the near RT images during and/or proximate in time to delivery of a therapeutic treatment and/or a diagnostic procedure.

[0014] The method may also or alternatively include electronically rotating the visualizations based on user input and electronically selectively altering a view of the displayed visualization based on user input so that the visualization includes the at least one flexible device with (a) only a near RT image of the target anatomy, (b) both the near RT image of the anatomy and the registered model of the anatomical structure, or (c) only the registered model of the anatomical structure.

[0015] Still other embodiments are directed to computer program products for facilitating an MRI-guided interventional therapy on a heart of a patient. The computer program product includes a computer readable storage medium having computer readable program code embodied in the medium. The computer-readable program code including: computer readable program code that computer readable program code that directs an MRI Scanner to obtain in an interleaved manner (i) tracking signal data from tracking coils associated with an intrabody flexible device and (ii) MR image data, both in the same 3-D image space with a coordinate system; com-

puter readable program code that generates near real time (RT) MRI image of at least a portion of target anatomy of a patient using relevant anatomical scan planes; computer readable program code that identifies spatial coordinates associated with a location of at least a distal end portion of at least one flexible intrabody medical device in the 3-D MRI image space using the tracking signal data; and computer readable program code that renders dynamic near RT visualizations of the at least intrabody flexible medical device in the 3-D image space with near RT MRI images, wherein the at least one device is not required to be in any of the relevant anatomical scan planes used to obtain MR image data for the at least one near RT MRI images, and wherein the distal end portion of the device can take on a non-linear shape.

[0016] Some embodiments of the present invention can provide 3D, 4D and/or 4D visualization systems of multiple data sources, (e.g., multiparametric data) of cardiac tissue to provide relevant tissue characterization data and/or cardiac status during a therapy so that ablation and/or other therapy can be more precisely delivered, confirmed and/or visualized. For example, with cardiac ablation systems the visualizations can be rendered with an accurate or "true" lesion pattern from the therapy and/or an associated change in a physiological state of cardiac tissue during the therapy based, at least in part, on MR image data.

[0017] Yet other embodiments are directed to MRI guided interventional systems that include a circuit in communication with a display with a User Interface. The circuit is configured to: (a) provide a patient planning map and allow a user to identify at least one target treatment site on the patient planning map using the User Interface; then (b) register the planning map in 3-D MRI image space prior to or during an MRI guided procedure; and (c) define locations of the at least one treatment site in 3-D MRI image space based on the registered planning map.

[0018] The circuit can be configured to accept user input via the User Interface to selectively fade and/or turn on and off a visual indication of the at least one target treatment site in position in 3-D MRI imaging space in rendered visualizations during an MRI guided procedure.

[0019] The circuit can be configured to allow a user to select whether to show tissue characterization data on the display in interactive visualizations during the MRI guided procedure in different viewing formats including: (a) on a registered map with near RT image data; or (b) in near RT images without a map in visualizations during an MRI guided procedure.

[0020] Embodiments of the invention are directed to systems, methods, User Interfaces and a processor configured to automatically obtain MR image data and tracking data for one or more intrabody flexible devices (e.g., catheters, probes, delivery devices, needles and the like). This data alone or with other physiologic or *a priori* data regarding a particular device and/or anatomy of a patient can be used to generate the visualizations in a

manner that visually shows (e.g., via color, opacity and/or intensity) target anatomical tissue using MR image data and a physical representation of at least a distal end portion of the at least one flexible device in near real time on a display during a surgical procedure.

[0021] Embodiments of the invention are particularly suitable for MRI-guided EP procedures for ablating tissue to arrhythmias such as AFIB or injecting therapeutics to treat heart failure.

[0022] The system may also be suitable for delivering a therapeutic agent or carrying out another treatment or diagnostic evaluation for any intrabody location, including, for example, the brain, heart, gastrointestinal system, genitourinary system, spine (central canal, the subarachnoid space or other region), vasculature or other intrabody location.

[0023] It is noted that any one or more aspects or features described with respect to one embodiment, may be incorporated in a different embodiment although not specifically described relative thereto. That is, all embodiments and/or features of any embodiment can be combined in any way and/or combination. Applicant reserves the right to change any originally filed claim or file any new claim accordingly, including the right to be able to amend any originally filed claim to depend from and/or incorporate any feature of any other claim although not originally claimed in that manner. These and other objects and/or aspects of the present invention are explained in detail in the specification set forth below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024]

Figure 1 is a schematic illustration of an MRI-guided system configured to show a device tissue interface using near RT MRI data according to embodiments of the present invention.

Figure 2 is a schematic illustration of an intrabody device with a tracking coil electrically connected to a Scanner channel according to embodiments of the present invention.

Figure 3 is a schematic illustration of an MRI system with a workstation and display according to embodiments of the invention.

Figure 4 is a circuit diagram of an exemplary tracking coil tuning circuit according to embodiments of the present invention.

Figures 5A-5D are contemplated screen shots of exemplary interactive visualizations with a physical representation of an intrabody flexible medical device according to embodiments of the present invention.

Figure 6 is a schematic illustration of a display with two viewing windows, one showing an interactive visualization and the other showing relevant near RT MRI image according to embodiments of the present invention.

Figures 7-21 are contemplated screen shots of exemplary visualizations and images on a display and UI controls that can be generated to facilitate an MRI guided procedure according to embodiments of the present invention.

Figures 22A and 22B are exemplary (contemplated) screen shots of an intrabody device (e.g., ablation catheter) with the device rendered as a physical representation and the MRI image being in close-up according to embodiments of the present invention.

Figures 23 and 24A-D are exemplary (contemplated) screen shots illustrating navigational indicia that can be used to help guide and/or position an intrabody device according to embodiments of the present invention.

Figures 25-28 are yet additional exemplary (contemplated) screen shots illustrating patient data and target (clinician identified) treatment zones that can provide information that can help drive clinical decisions according to embodiments of the present invention.

Figure 29 is a schematic illustration of an MRI-interventional suite according to embodiments of the present invention.

Figure 30A is an enlarged partial perspective view of a tip portion of an exemplary ablation catheter according to particular embodiments of the present invention.

Figure 30B is a cross-section of the tip portion of the catheter taken along lines 30B-30B in **Figure 30A**.

Figure 31 is an enlarged axial cross section of a tip portion of another example of an ablation catheter according to embodiments of the present invention.

Figure 32 is an enlarged cross-section of the catheter shown in **Figure 31**.

Figure 33 is an enlarged cross-section of the catheter shown in **Figure 31** taken along lines 33-33 in **Figure 31**. The **Figure 32** section view is taken at a location upstream of that shown in **Figure 33**.

Figure 34 is a flow chart of exemplary operations that can be used to carry out embodiments of the

present invention.

Figure 35 is a flow chart of exemplary operations that can be used to carry out additional aspects of embodiments of the present invention.

Figure 36 is a schematic illustration of a data processing circuit or system according to embodiments of the present invention.

Figure 37 is a schematic illustration of examples of different intrabody devices that can be used with embodiments of the present invention.

15 DETAILED DESCRIPTION OF EMBODIMENTS OF THE INVENTION

[0025] The present invention will now be described more fully hereinafter with reference to the accompanying drawings, in which embodiments of the invention are shown. This invention may, however, be embodied in many different forms and should not be construed as limited to the embodiments set forth herein; rather, these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey the scope of the invention to those skilled in the art. Like numbers refer to like elements throughout. It will be appreciated that although discussed with respect to a certain embodiment, features or operation of one embodiment can apply to others.

[0026] In the drawings, the thickness of lines, layers, features, components and/or regions may be exaggerated for clarity and broken lines (such as those shown in circuit or flow diagrams) illustrate optional features or operations, unless specified otherwise. In addition, the sequence of operations (or steps) is not limited to the order presented in the claims unless specifically indicated otherwise.

[0027] The terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting of the invention. As used herein, the singular forms "a", "an" and "the" are intended to include the plural forms as well, unless the context clearly indicates otherwise. It will be further understood that the terms "comprises" and/or "comprising," when used in this specification, specify the presence of stated features, steps, operations, elements, and/or components, but do not preclude the presence or addition of one or more other features, steps, operations, elements, components, and/or groups thereof. As used herein, the term "and/or" includes any and all combinations of one or more of the associated listed items.

[0028] Unless otherwise defined, all terms (including technical and scientific terms) used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. It will be further understood that terms, such as those defined in commonly used dictionaries, should be interpreted as

having a meaning that is consistent with their meaning in the context of the specification and relevant art and should not be interpreted in an idealized or overly formal sense unless expressly so defined herein. Well-known functions or constructions may not be described in detail for brevity and/or clarity.

[0029] It will be understood that when a feature, such as a layer, region or substrate, is referred to as being "on" another feature or element, it can be directly on the other element or intervening elements may also be present. In contrast, when an element is referred to as being "directly on" another feature or element, there are no intervening elements present. It will also be understood that, when a feature or element is referred to as being "connected" or "coupled" to another feature or element, it can be directly connected to the other element or intervening elements may be present. In contrast, when a feature or element is referred to as being "directly connected" or "directly coupled" to another element, there are no intervening elements present. Although described or shown with respect to one embodiment, the features so described or shown can apply to other embodiments.

[0030] The term "circuit" refers to an entirely software embodiment or an embodiment combining software and hardware aspects, features and/or components (including, for example, at least one processor and software associated therewith embedded therein and/or executable by and/or one or more Application Specific Integrated Circuits (ASICs), for programmatically directing and/or performing certain described actions or method steps). The circuit can reside in one location or multiple locations, it may be integrated into one component or may be distributed, e.g., it may reside entirely in an MR Scanner control cabinet, partially in the MR Scanner control cabinet, totally in a separate component or system such as a clinician workstation but communicate with MR Scanner electronics and/or in an interface therebetween, in a remote processor and combinations thereof.

[0031] The term "map" is used interchangeably with the term "model" and refers to a volumetric rendering of a patient's target anatomy. The term "tissue characterization (or characteristic) map" refers to a rendered volumetric (typically 3-D, 4-D or 4-DMP) visualization and/or image of a target anatomical structure or portion thereof showing one or more selected tissue parameters, conditions, or behaviors of cardiac tissue using MR image data, e.g., the tissue characterization map is a rendered partial or global anatomical map that shows at least one defined tissue characteristic of the target anatomy, e.g., heart or portion thereof (for example, the left atrium) in a manner that illustrates relative degrees or measures of the tissue characteristic(s) of interest, typically in different colors, opacities and/or intensities. Notably, a tissue characterization map or model is to be contrasted with an electroanatomical (EA) map or model which is based on sensed electrical activity of different regions of the heart rather than on MR image data. In some embodi-

ments, tissue data from an electroanatomical map and/or the tissue characteristic map or the map(s) themselves can be selectively turned on and off (on a display) or faded. A tissue characteristic map may be included with an EA model and/or two or more tissue characteristic maps may be merged into or shown as a composite map or may be shown overlying and aligned with one another. Thus, the visualizations can use one or both types of volumetric tissue maps, shown separately, overlaid on each other and/or integrated as a composite or superimposed map. The terms "fade" and "faded" refer to making the so-called feature less visually dominant in a visualization by dimming the intensity, color and/or opacity relative to other features in the visualization.

[0032] The actual visualization can be shown on a screen or display so that the map of the anatomical structure is in a flat 2-D and/or in 2-D what appears to be 3-D volumetric images with data representing features or electrical output with different visual characteristics such as with differing intensity, opacity, color, texture and the like. A 4-D map can either illustrate a 3-D anatomical structure (e.g., heart) with movement (e.g., a beating heart and/or a heart with blood flow, breathing lungs or other moving structure) or show additional information over a 3-D anatomic model of the contours of the heart or portions thereof. The term "heart" can include adjacent vasculature, e.g., the branching of the pulmonary veins.

[0033] The term "4-D multiparametric visualization" (4-DMP) means a 4-D visualization image (e.g., a 3-D image of a beating heart) with functional spatially encoded or correlated information shown on the visualization. The 4-DMP visualization can be provided with fMRI data and/or one or more tools used to provide the spatially correlated functional data (e.g., electrical) data of the heart based on the 3-D model of the tool. Again, the 3-D, 4-D and/or 4-DMP visualizations are not merely an MRI image or MRI images of the patient during a procedure but are rendered visualizations that can combine multiple sources of data to provide a visualization of spatially encoded function with anatomical shape. Thus, the visualizations can comprise a rendered model of the patient's target anatomy with a rendered visualization of at least one medical device in an intrabody location with respect to the model and along with near RT MRI image data of the anatomical structure. The figures may include prophetic examples of screen shots of visualizations and the like and do not necessarily represent actual screen shots of a surgical system/display.

[0034] The term "close-up" means that the associated image is shown enlarged relative to a global image or typical navigation view to show local tissue. The term "high-resolution" means that the image data is obtained with higher resolution than normal image data (usually requiring longer scan times and/or using an internal antenna to increase SNR). For example, the local tissue ablation views may be shown in higher resolution than MRI images in the navigation view. The term *en face* refers to a view through a tissue wall (e.g., myocardial

wall) and substantially parallel (tangent) to the surface.

[0035] The term "programmatically" means that the operation or step can be directed and/or carried out by a digital signal processor and/or computer program code. Similarly, the term "electronically" means that the step or operation can be carried out in an automated manner using electronic components rather than manually or using merely mental steps.

[0036] At least a portion of the intrabody medical device is tracked and its position identified in 3-D imaging space (e.g., X, Y, Z coordinates). Various location tracking means for the tool and/or registration means for the catheter to the imaging space can be employed. For example, the intrabody device can include fiducial markers or receive antennas combinations of same. The term "fiducial marker" refers to a marker that can be identified using electronic image recognition, electronic interrogation of MRI image data, or three-dimensional electrical signals to define a position and/or find the feature or component in 3-D space. The fiducial marker can be provided in any suitable manner, such as, but not limited to a geometric shape of a portion of the tool, a component on or in the tool, a coating or fluid-filled coating (or combinations of different types of fiducial markers) that makes the fiducial marker(s) MRI-visible that are active or passive (e.g., if passive, the marker does not provide MR signal) with sufficient intensity for identifying location and/or orientation information for the tool and/or components thereof in 3-D space. As will be discussed further below, in particular embodiments, the device comprises at least one tracking coil electrically connected to the MRI Scanner that generate signals that are detected (received) by the MR Scanner and used to identify respective locations of the coils in a 3-D coordinate system of the imaging space, and hence the device with such tracking coils, in the 3-D image space.

[0037] The terms "MRI or MR Scanner" are used interchangeably to refer to a Magnetic Resonance Imaging system and includes the magnet, the operating components, e.g., RF amplifier, gradient amplifiers and operational circuitry including, for example, processors (the latter of which may be held in a control cabinet) that direct the pulse sequences, select the scan planes and obtain MR data.

[0038] The term "RF safe" means that the device (e.g., catheter) and any (conductive) lead is configured to operate safely when exposed to RF signals, particularly RF signals associated with MRI systems, without inducing unplanned current that inadvertently unduly heats local tissue or interferes with the planned therapy. The term "MRI visible" means that the device is visible, directly or indirectly, in an MRI image. The visibility may be indicated by the increased SNR of the MRI signal proximate the device. The device can act as an MRI receive antenna to collect signal from local tissue and/or the device actually generates MRI signal itself, such as via suitable medical grade hydro-based coatings, fluid (e.g., aqueous fluid) filled channels or lumens. The term "MRI compatible"

means that the so-called component(s) is safe for use in an MRI environment and as such is typically made of a non-ferromagnetic MRI compatible material(s) suitable to reside and/or operate in a high magnetic field environment. The term "high-magnetic field" refers to field strengths above about 0.5 T, typically above 1.0T, and more typically between about 1.5T and 10T. Embodiments of the invention may be particularly suitable for 1.5T and/or 3.0T systems.

[0039] Generally stated, advantageously, the system can be configured so that the surgical space is the imaging space and the tracking is performed in the imaging space so that there is no requirement to employ a discrete tracking system that must then be registered to the imaging space. In some embodiments, the tracking is carried out in the same 3-D imaging space but the flexible intrabody medical device is tracked independent of the imaging scan planes used to obtain the MR image data for generating images of local anatomy and is shown as a physical representation in the visualization.

[0040] The term "near real time" refers to both low latency and high frame rate. Latency is generally measured as the time from when an event occurs to display of the event (total processing time). For tracking, the frame rate can range from between about 100 fps (frames per second) to the imaging frame rate. In some embodiments, the tracking is updated at the imaging frame rate. For near 'real-time' imaging, the frame rate is typically between about 1 fps to about 20 fps, and in some embodiments, between about 3 fps to about 7 fps. For lesion imaging, a new image can be generated about every 1-7s, depending on the sequence used. The low latency required to be considered "near real time" is generally less than or equal to about 1 second. In some embodiments, the latency for tracking information is about 0.01s, and typically between about 0.25-0.5s when interleaved with imaging data. Thus, with respect to tracking, visualizations with the location, orientation and/or configuration of a known intrabody device can be updated with low latency between about 1 fps to about 100 fps. With respect to imaging, visualizations using near real time MR image data can be presented with a low latency, typically within between about .01 ms to less than about 1 second, and with a frame rate that is typically between about 1-20 fps. Together, the system can use the tracking signal and image signal data to dynamically present anatomy and one or more intrabody devices in the visualization in near real-time. In some embodiments, the tracking signal data is obtained and the associated spatial coordinates are determined while the MR image data is obtained and the resultant visualization(s) with the intrabody device (e.g., flexible catheter using the tracking coil data) and the near RT MR image(s) is generated.

[0041] In some embodiments, MR image data is obtained during an active treatment such as during an ablation, delivery of a drug or other material, valve repair or replacement, lining repair, and the like, and the resultant visualization(s) with the flexible intrabody device used

for this treatment (e.g., catheter, needle and the like) along with one or more near RT MR images of local anatomy is substantially continuously rendered/generated. In some particular embodiments, the system is a cardiac EP system used to place a lesion pattern of transmural lesions that creates a desired electrical isolation in the cardiac tissue to treat the at-risk pathology/condition (e.g., AFIB). The ablations are not required to be followed in any particular direction or order. The ablation can be carried out to generate one or more continuous and/or contiguous lesions and/or several non-continuous or non-contiguous lesions. The lesions may be linear (whether straight or with a curvature such as circular or curvilinear).

[0042] The term "intrabody device" is used broadly to refer to any diagnostic or therapeutic medical device including, for example, catheters, needles (e.g., injection, suture, and biopsy), forceps (miniature), knives or other cutting members, ablation or stimulation probes, injection or other fluid delivery cannulas, mapping or optical probes or catheters, sheaths, guidewires, fiberscopes, dilators, scissors, implant material delivery cannulas or barrels, and the like, typically having a size that is between about 5 French to about 12 French, but other sizes may be appropriate.

[0043] **Figure 1** illustrates an MRI interventional system **10** with a scanner **10S** and a flexible intrabody medical device **80** proximate target tissue **100** at a device-tissue interface **100i**. The system **10** can be configured to electronically track the 3-D location of the device **80** in the body and identify and/or "know" the location of the tip portion **80t** of the device (e.g., the ablation or needle tip) in a coordinate system associated with the 3-D imaging space. As shown in **Figure 1**, the device **80** can include a plurality of spaced apart tracking members **82** on a distal end portion thereof. In a particular embodiment, the device **80** can be an ablation catheter and the tip can include an ablation electrode, ablation balloon, or other ablation source **80e** (typically at least one at a distal end portion of the device). Where used, the electrode can be both a sensing and ablation electrode.

[0044] The tracking members **82** can comprise miniature tracking coils, passive markers and/or a receive antenna. In a preferred embodiment, the tracking members **82** include at least one miniature tracking coil **82c** that is connected to a channel **IOch** of an MRI Scanner **10S** (**Figure 2**). The MR Scanner **10S** can be configured to operate to interleave the data acquisition of the tracking coils with the image data acquisition. The tracking data is typically acquired in a 'tracking sequence block' which takes about 10 msec (or less). In some embodiments, the tracking sequence block can be executed between each acquisition of image data (the latter can be referred to as an 'imaging sequence block'). So the tracking coil coordinates can be updated immediately before each image acquisition and at the same rate. The tracking sequence can give the coordinates of all tracking coils simultaneously. So, typically, the number of coils used to

track a device has substantially no impact on the time required to track them.

[0045] Embodiments of the present invention provide a new platform that can help facilitate clinical decisions during an MRI-guided procedure and can present near real time anatomical image data to the clinician in an interactive visualization **100v**. The visualizations **100v** (**Figures 5A-5D**) can be dynamically generated as the intrabody device **80** moves in the body into and/or about a target location, as a user rotates, crops or otherwise alters a displayed visualization or view and/or during an active therapy or diagnostic procedure step, e.g., while ablating at target lesion sites or while approaching and/or delivering a different therapeutic treatment, with minimal latent time between serial MRI image data acquisitions, typically less than about 5 seconds, typically substantially continuously with a minimal latent time of about 1 second or less, such as between about .001 seconds and 1 second. Together, the system **10** can use the tracking signal(s) and image signal data to dynamically track the device **80** (which is typically a plurality of devices) and present visualizations of the anatomy and one or more intrabody devices **80** in near real-time. Notably, while the at least one device is tracked in 3-D image space, the device is not required to be imaged and is not required to be in any of the relevant anatomical scan planes used to obtain MR data for the near RT MRI images.

[0046] The term "physical representation" means that a device is not actually imaged but rather rendered with a physical form in the visualizations. Typically, the physical representation is a partial physical representation which shows the distal end portion of the device in the body in the 3-D MR image space. The physical representation may be of any form including, for example, a graphic with at least one geometric shapes, icons and/or symbols. The physical representation is typically in 3-dimensional form. In some particular embodiments, the physical representation may be a virtual graphic substantial replica substantially corresponding to an actual shape and configuration of the physical appearance and/or configuration of a portion (e.g., distal end portion) of the associated device (see, e.g., **Figures 22A, 22B**). The physical representation can be electronically generated based on a *a priori* knowledge of the dimensions and configuration of the device. The tip and each tracking coil on a distal end of a particular device may be shown in a geometric shape (the same or different shapes, e.g., an arrow for the tip and a sphere or block or other (typically 3-D) geometric shape or shapes for tracking coils, each in its real location in the 3-D space and in its relative position on the device and each may be rendered with the same or a different color and with the same or a different shape. For example, the tip and each proximate tracking coil may be shown in a different color.

[0047] The term "tortuous" refers to a curvilinear pathway in the body, typically associated with a natural lumen such as vasculature. The term "dynamic visualizations" refers to a series of visualizations that show the move-

ment of the device(s) in the body and can show a beating heart or movement based on respiratory cycle and the like.

[0048] The term "pre-acquired" means that the data used to generate the model or map of the actual patient anatomy was obtained prior to the start of an active therapeutic or diagnostic procedure and can include immediately prior to but during the same MRI session or at an earlier time than the procedure (typically days or weeks before).

[0049] Embodiments of the present invention can be configured to guide and/or place flexible intrabody diagnostic and/or interventional devices in an MRI environment (e.g., interventional medical suite) to any desired internal region of interest of a subject, typically via a natural lumen and/or tortuous path so that the intrabody devices can take on different non-linear configurations/shapes as it moves into position through a target pathway (which may be a natural lumen or cavity). The subjects can be animal and/or human subjects.

[0050] Some embodiments of the invention provide systems that can be used to treat cardiac disorders such as arrhythmias including, but not limited to AFIB, or to repair or replace cardiac valves, repair, flush or clean vasculature and/or place stents, and/or to deliver stem cells or other cardio-rebuilding cells or agents or products into cardiac tissue, such as a heart wall, via a minimally invasive MRI guided procedure while the heart is beating (*i.e.*, not requiring a non-beating heart with the patient on a heart-lung machine). The cardiac procedures can be carried out from an inside of the heart or from an outside of the heart. The cardiac procedures may be directed to treating cardiac arrhythmias or heart failure (e.g., congestive heart failure, reduced heart function, and the like).

[0051] Embodiments of the system are also suitable for delivering a therapeutic agent or carrying out another treatment or diagnostic evaluation for other intrabody locations, including, for example, the brain, gastrointestinal system, genitourinary system, spine (central canal, the subarachnoid space or other region), vasculature or other intrabody locations. Additional discussion of exemplary target regions can be found at the end of this document.

[0052] To be clear, while detailed drawings of exemplary flexible devices **80** are shown for tracking coils for transseptal needles (septal puncture kit components) and mapping and/or ablation catheters for cardiac use, embodiments of the invention are not intended to be limited to these devices nor to cardiac use. Exemplary devices are listed above (and see, **Figure 37**). Exemplary (non-cardiac) intrabody locations are listed at the end of this document. For example, the device can be implemented as injection catheters or diagnostic biopsy needles and the like for any target anatomical location in the body. See, e.g., U.S. Patent Application Serial No. 10/769,994 (intramyocardial injection needle), U.S. Patent No. 7,236,816 (biopsy needle), and U.S. Patent No. 6,606,513 (transseptal needle). Examples of a loop catheter **80'**, mapping catheter **80''**, (deformable) ablation

catheter **80'**, and injection needle catheter **80'''** (one **80'''** view is an enlarged view of the needle with a tracking coil) are shown in **Figure 37**. The loop catheter and mapping catheter includes both tracking coils **82c** and sensing electrodes **180s**. All of the catheters may also include at least one tracking coil **82c** even if not shown in the example views.

[0053] The system **10** and/or circuit **60c** can calculate the position of the tip **80t** of the device as well as the shape and orientation of the flexible device based on a *priori* information on the dimensions and behavior of the device **80** (e.g., for a steerable device, the amount of curvature expected when a certain pull wire extension or retraction exists, distance to tip from different coils **82** and the like). Using the known information of the device **80** and because the tracking signals are spatially associated with the same X, Y, Z coordinate system as the MR image data, the circuit **60c** can rapidly generate visualizations showing a physical representation of the location of a distal end portion of the device **80** with near RT MR images of the anatomy.

[0054] In some embodiments, the tracking signal data is obtained and the associated spatial coordinates are determined while a circuit **60c** in the MRI Scanner **10S** (**Figure 2**) and/or in communication with the Scanner **10S** (**Figure 3**) obtains MR image data. The reverse operation can also be used. The circuit **60c** can then rapidly render the resultant visualization(s) **100v** (see, e.g., **Figures 5A-5D**) with the flexible device(s) **80** shown with a physical representation based on spatial coordinates of the devices in the 3-D imaging space identified using the associated tracking coil data and the near RT MR image(s).

[0055] As will be discussed further below, generally stated, in some embodiments, the circuit **60c** can be configured to allow a user (via a User Interface **25** associated with a display, for example) to selectively show or not show (e.g., turn on/off and/or fade) in one or more visualizations on a display one or more of at least four different data sets in either the rendered model **100M** or in near RT MRI images **100MRI** of relevant scan planes during a procedure. The model **100M** can be a planning model **37M** or different patient model.

[0056] The different data sets can include a first data set associated with a volumetric model or map **100M** of the patient (which may be shown in wire form), a second data set associated with tissue data maps **30** (e.g., tissue data based on image data such as edema, DHE and the like, and/or electroanatomical data), a third typically near-RT MRI scan (image) data set of relevant anatomic structure, and a fourth target site **55t** data set. As will be discussed further below, a pre-acquired patient planning map can be used to identify at least one target site **55t** and the planning map can be registered to the 3-D MRI image space which also registers the location of the target site in the 3-D space to allow the target site **55t** to be shown in the visualizations in proper 3-D space location in either or both the near RT images or in the rendered registered model. The model **100M**, the tissue data and

the target sites (and the images **100MRI**) can be turned "on" or "off" in the visualizations by a user and can be used to drive the MRI-guided procedure. For example, a "live" near RT MRI image of patient tissue can be shown in the visualization and a user (physician) can select to show at least one target treatment site in the image space in the near RT MRI image. The user may also show the model **100M** in wire form with or without tissue data (e.g., DHE or edema map data). For example, as a therapeutic device/catheter **80** approaches a target site, the model **100M** can be turned off or faded to a faint visibility with respect to near RT images can be shown. A user can also or alternatively select to show the target treatment sites **55t** in the near RT images **100MRI** without the model or with the model faded.

[0057] The circuit **60c** can be totally integrated into the MR Scanner **10S** (e.g., control cabinet), partially integrated into the MR Scanner **10S** or be separate from the MR Scanner **10S** but communicate therewith. If not totally integrated into the MR Scanner **10S**, the circuit **60c** may reside partially or totally in a workstation **60** and/or in remote or other local processor(s) and/or ASIC. **Figure 3** illustrates that a clinician workstation **60** can communicate with the MR Scanner **10S** via an interface **44**. Similarly, the device **80** in the magnet room can connect to the MR Scanner **10S** via an interface box **86** which may optionally be integrated into the patch panel **250**.

[0058] As shown in **Figures 2** and **3**, for example, the system **10** can include at least one (interactive) display **20** in communication with the circuit **60c** and/or the Scanner **10S**. The display **20** can be configured to display the interactive visualizations **100v**. The visualizations **100v** can be dynamic showing the movement of the device **80** relative to the intrabody anatomical structure shown by the displayed near-real time MRI image.

[0059] The system **10** can include a User Interface (UI) **25** with several UI controls **25c** (**Figure 7**), such as a graphic UI (GUI), in communication with the display **20** and may be configured to allow a user to select to show one or more pre-acquired or *in situ* generated maps and/or images **30** of target tissue including different tissue characterization maps and/or an optional EA map (or data from those maps) which can be shown in and/or with the visualization **100v**. For example, the system **10** can be configured to allow a user to select to show a map (or data from the map) of patient vasculature and/or fibrous tissue based on pre-acquired image data (such as segmented MRA (Magnetic Resonance Angiography) or other image slices) with the map or data therefrom being registered to and overlaid (superimposed) onto or incorporated into at least one of the models **100M** or images **100MRI** in the visualization and can be selectively turned on and off by a user. This information may help a clinician select a treatment site or avoid a treatment site or otherwise affect clinical choices. For example, for cardiac use, if vasculature with a relatively large blood flow is shown in a target lesion or injection space in cardiac tissue and/or if fibrous tissue is shown, a clinician may choose

another spot or, where ablation is the therapy, may ablate longer to form a transmural lesion. Further examples of display options will be discussed further below.

[0060] In some embodiments, the system/circuit can employ interactive application of non-selective saturation to show the presence of a contrast agent in near real-time scanning. This option can help, for example, during image-guided catheter navigation to target tissue that borders scar regions. See, e.g., Dick et al., Real Time MRI enables targeted injection of labeled stem cells to the border of recent porcine myocardial infarction based on functional and tissue characteristics, Proc. Intl. Soc. Mag. Reson. Med. 11, p. 365 (2003); Guttman et al., Imaging of Myocardial Infarction for Diagnosis and Intervention Using Real-Time Interactive MRI Without ECG-Gating or Breath-Holding, Mag. Reson. Med. 52: 354-361 (2004), and Dick and Guttman et al., Magnetic Resonance Fluoroscopy Allows Targeted Delivery of Mesenchymal Stem Cells to Infarct Borders in Swine, Circulation, 2003; 108:2899-2904, which describe, *inter alia*, imaging techniques used to show regions of delayed enhancement in (near) real-time scans.

[0061] **Figure 2** illustrates that the device **80** can include at least one conductor **81**, such as a coaxial cable, that connects a respective tracking coil **82c** to a channel **10ch** of the MR Scanner **10S**. The MR Scanner **10S** can include at least 16 separate channels, and typically more channels but may operate with less as well. Each device **80** can include between about 1-10 tracking coils, typically between about 2-6. The coils **82c** on a particular device **80** can be arranged with different numbers of turns, different dimensional spacing between adjacent coils **82c** (where more than one coil is used) and/or other configurations. The circuit **60c** can be configured to generate the device renderings based on tracking coil locations/positions relative to one another on a known device with a known shape and/or geometry or predictable or known changeable (deflectable) shape or form (e.g., deflectable end portion). The circuit can identify or calculate the actual shape and orientation of the device for the renderings based on data from a CAD (computer aided design) model of the physical device. The circuit can include data regarding known or predictable shape behavior based on forces applied to the device by the body or by internal or external components and/or based on the positions of the different tracking coils in 3-D image space and known relative (dimensional) spacing.

[0062] As shown in **Figure 3**, the display **20** can be provided in or associated with a clinician workstation **60** in communication with an MRI Scanner **10**. Other displays may be provided. The MRI Scanner **10S** typically includes a magnet **15** in a shielded room and a control cabinet **11** (and other components) in a control room in communication with electronics in the magnet room. The MRI Scanner **10S** can be any MRI Scanner as is well known to those of skill in the art. Examples of current commercial scanners include: GE Healthcare: Signa 1.5T/3.0T; Philips Medical Systems: Achieva 1.5T/3.0T;

Integra 1.5T; Siemens: MAGNETOM Avanto; MAGNETOM Espree; MAGNETOM Symphony; MAGNETOM Trio; and MAGNETOM Berio.

[0063] The tracking coils **82c** can each include a tuning circuit that can help stabilize the tracking signal for faster system identification of spatial coordinates. **Figure 4** illustrates an example of a tuning circuit **83** that may be particularly suitable for a tracking coil **82c** on a catheter. As shown, CON1 connects the coaxial cable to the tracking coil **82c** on a distal end portion of the device **80** while J1 connects to the MR Scanner channel **10ch**. The Scanner **10S** sends a DC bias to the circuit **83** and turns U1 diode "ON" to create an electrical short which creates a high impedance (open circuit) on the tracking coil to prevent current flow on the tracking coil and/or better tracking signal (stability). The tuning circuit can be configured to have a 50 Ohm matching circuit (narrow band to Scanner frequency) to electrically connect the cable to the respective MR Scanner channel. When the diode U1 is open, the tracking coil data can be transmitted to the MR Scanner receiver channel **10ch**. The C1 and C2 capacitors are large DC blocking capacitors. C4 is optional but can allow for fine tuning (typically between about 2-12 picofarads) to account for variability (tolerance) in components. It is contemplated that other tuning circuits and/or tracking signal stabilizer configurations can be used. The tuning circuit **83** can reside in the intrabody device **80** (such as in a handle or external portion), in a connector that connects the coil **82c** to the respective MRI scanner channel **10ch**, in the Scanner **10S**, in an interface box **86** (**Figure 2**), a patch panel **250** and/or the circuit **83** can be distributed among two or more of these or other components. Where multiple devices **80** are tracked concurrently (and rendered and shown in the visualizations), the circuit **60c** can correlate the respective tracking coils to the corresponding device and identify the different devices. Typically, the device identifiers are "unique" electronic identifiers with pre-defined values such as different resistance values.

[0064] In some embodiments, each tracking coil **82c** can be connected to a coaxial cable **81** having a length to the diode via a proximal circuit board (which can hold the tuning circuit and/or a decoupling/matching circuit) sufficient to define a defined odd harmonic/multiple of a quarter wavelength at the operational frequency of the MRI Scanner **10S**, e.g., $\lambda/4$, $3\lambda/4$, $5\lambda/4$, $7\lambda/4$ at about 123.3 MHz for a 3.0T MRI Scanner. This length may also help stabilize the tracking signal for more precise and speedy localization. The tuned RF coils can provide stable tracking signals for precise localization, typically within about 1 mm or less. Where a plurality (e.g., two closely spaced) adjacent tracking coils are fixed on a substantially rigid material, the tuned RF tracking coils **82** can provide a substantially constant spatial difference with respect to the corresponding tracking position signals.

[0065] The tracking sequence used in the system **10** can intentionally dephase signal perpendicular to the read-out direction to attenuate unwanted signal from 1)

bulk objects and 2) regions sensed by other signal sensitive parts of the catheter which couple to the tracking coil **82c** (e.g. the coaxial cable along the catheter shaft). This tends to leave only a sharp peak indicating the position of the tracking coil.

[0066] The tracking sequence block can include or consist of a plurality of (typically about three) repetitions of a small flip-angle excitation. Each repetition is designed to indicate the x, y or z component of the tracking coil coordinates in succession. Frequency encoding is used along the x-direction to obtain the x-coordinate, the y-direction for the y-coordinate, and the z-direction for the z-coordinate. When the frequency encoding is in the x-direction, the other two directions (y and z) are not spatially encoded, producing projection (spatially integrated) signals in those directions from all excitation regions. The dephasing gradient attempts to attenuate unwanted signal included in these projections. Once the tracking sequence block is complete, a spoiler gradient can be used to dephase any transverse signal remaining from the tracking before the imaging sequence block is executed.

[0067] The imaging sequence block obtains a portion, depending on the acceleration rate, of the data used to reconstruct an image of a single slice. If the acceleration rate is 1, then all of the data for an image is collected. If the acceleration rate is 2, then half is collected, etc. If multiple slices are activated, then each successive imaging block collects data for the next slice, in 'round robin' fashion. If any magnetization preparation (e.g., saturation pulses) is activated, these are executed after the tracking sequence block, immediately before the imaging sequence block.

[0068] Additional discussion of tracking means and ablation catheters can be found in U.S. Patent No. 6,701,176, and U.S. Provisional Application Serial No. 61/261,103. Exemplary ablation catheters will be discussed further below.

[0069] Referring now to **Figures 5A-5D** and **6**, examples of visualizations **100v** with a physical representation **80R** of the intrabody device **80**, a volumetric model **100M** of target anatomical structure and near real-time MRI images **100MRI**. The circuit **60c**/Scanner **10S** is configured to present a 3-D volumetric model of at least a portion of the patient's target anatomy (shown as the heart) **100M** in the visualization **100v** with the model registered to the 3-D imaging space along with a physical representation of at least the distal end portion of the at least one intrabody device **80R** in the imaging space. Optionally, the visualizations can be carried out to show the tracking coils in the physical representation of the distal end portion of the medical device in different colors using the identified location of the tracking coils and defined form factor and/or dimensional data regarding actual coil placement on the device.

[0070] The circuit **60c** can be configured to generate the visualizations **100v** with at least two visual reference planes **41**, **42** (shown with a third intersecting plane **43**) that are typically oblique or orthogonal to each other and

extend through at least a major portion of the visualization **100v**. The planes **41**, **42** (and **43**) can be transparent and/or translucent. They may be shown with different color perimeters that correspond to a respective two-dimensional image slice (which may be shown as thumbnails on the display also with a perimeter of similar or the same color).

[0071] The planes **41**, **42** can move relative to each other in the imaging space or may be locked together, in any case they can be configured to move relative to the model **100M** in the imaging space. As shown in **Figures 5A-5D**, a user can rotate and zoom the visualization **100v** which automatically adjusts the visualization shown on the display. As also shown, the flexible device **80** is not required to be in any of the relevant anatomical scan planes used to obtain MR data for the at least one near RT MRI image **100MRI** in the visualization and the distal end portion **80d** of the flexible device **80** can take on a curvilinear shape and the tip **80t** can be steered or guided into different target positions.

[0072] In some embodiments, as shown in **Figure 5D**, the circuit **60c** is configured to associate a tip location of the at least one device **80** with an arrow **82a** and render the visualization so that each tracking coil **82** on the distal end portion **80d** has a shape **82s** with a color, with each tracking coil **82** having a respective different color from the other tracking coils, and with a line or spline **82l** connecting the tip **82a** and the coils **82c** and the line **82l** is able to flex, bend and move to reflect movement of the device **80** in the visualizations **100v**. The system/circuit can be configured to display color-highlighted images generated using tracking coil data from the MR Scanner tracking coil channels so as to display the coils as color high-lighted features in the 3D rendering of the physical representation of the device (e.g., catheter).

[0073] **Figure 6** illustrates that the system **10** can be configured to show both the interactive visualization **100v** in one viewing window **20w₁** and an MRI image **100MRI** alone in a second viewing window **20w₂**. The MRI image **100MRI** in the second window **20w₂** is typically associated with the target anatomy location identified by a user in the interactive visualization **100v** in the first viewing window **20w₁**.

[0074] As shown in **Figure 7**, the display **20** can have a UI **25** which can be configured to allow a physician or other clinician to select whether to show near-real-time MR images of target tissue **100MRI** either with a model **100M** of the target anatomical structure (**Figure 7**) and/or in a separate viewing window (**Figures 6, 13-16**). The circuit **60** is in communication with at least one display **20** with the User Interface **25**.

[0075] The User Interface **25** can be configured to allow a user to alter the displayed visualization (fade) to include only a near RT image of the anatomy, to include the near RT image of the anatomy and the registered model of the heart, or to include only the registered model, see, for example, **Figure 7** showing both types of images in the visualization **100v** with **Figure 9** which shows

only the model **100M**. The UI **25** can be an on/off selection of these options or may "fade" from one viewing option to another. As shown, a virtual sliding control **25c** allows a user to change what is shown ((near) RTMRI **100MRI** to only the Model **100M**).

[0076] The circuit **60c** can also be configured to generate MRI images which show the device location in near real time (in the MR image space). The UI **25** can also be configured to allow a user to turn off and/or fade the renderings of the device **80** in and out of the visualizations with rendered views of the device versus actual images of the device to confirm location or for additional visual input. The device may include other fiducial markers (e.g., a passive marker or an active marker such as receive antenna) for facilitating the visual recognition in the MR image.

[0077] The UI **25** typically includes multiple GUI controls that can include a touch screen input control to allow a clinician/physician to select a region of interest in the map **100M** by placing a cursor or by touching the screen at a region of interest. This can cause the system to obtain real time MR image data of that region and provide the associated image on the display and/or define scan planes (which may be preset scan planes) at that location in space.

[0078] Referring again to **Figure 7**, for example, the display **20** can be in communication with a UI **25** that provides a plurality of user selectable different maps **30** so that the map or data therefrom can be "turned on and off" on the displayed 3-D anatomical map registered to the imaging space. The different maps can comprise a patient-specific 3-D (volumetric) anatomical map, and/or data that can be shown on the 3-D anatomical map, obtained in or registered to the MRI 3-D imaging space used during the MR guided procedure. For tissue characterization maps, the maps include spatially correlated tissue characterization data taken from MR image data incorporated therein as discussed above. The UI **25** can include multiple different GUI (Graphic User Input) controls **25c** for different functions and/or actions. The GUI controls **25c** may also be a toggle, a touch screen with direction sensitivity to pull in one direction or other graphic or physical inputs.

[0079] The user selectable patient-specific maps **30** including a plurality of tissue maps, typically including at least one, and more typically several types of, tissue characterization maps (or data associated with such maps to be shown (superimposed) on a registered anatomic model) associated with the procedure that can be selected for viewing by a user. The UI **25** can also include GUI controls that allow a user to select two or more of the tissue maps, with such data able to be shown together (overlaid and registered and/or as a composite image/map) or separately. As shown, the maps **30** and/or data therefrom, may include at least a plurality of the following:

(a) a regional evaluation scan map **32r** (**Figure 17**)

and/or a global evaluation scan map **32g** (**Figure 13**) which shows tissue information, e.g., actual lesion patterns in one region to allow a clinician to view regional ablation information (such as at the LA (left atrium), a PV (pulmonary vein) and the like);

(b) pre-procedure MRI cardiac scans **34**;

(c) DHE 1 (Delayed Hyper Enhancement) tissue characterization map **35a** taken at a first point in time (such as a week or just prior to the procedure) (**Figure 28**);

(d) DHE 2 tissue characterization map **35b** taken at a second point in time, such as during a procedure, potentially toward an end of the procedure (for cardiac ablation procedures that can be used to confirm complete electrical isolation of the PV (pulmonary veins) or other targets prior to terminating the procedure - alternatively the DHE 2 map can be associated with the end of a prior EP ablation procedure) (**Figure 27**);

(e) an EA (electroanatomical) map **35c** (**Figure 17**);

(f) an edema tissue characterization map **35d** (**Figure 19**);

(g) other tissue characterization maps **35e**, for example:

- (i) a composite thermal tissue characterization map that shows positions of increased temperature that were caused by ablation of tissue during the procedure;
- (ii) ischemic (oxygen deprived or lacking) tissue characterization map;
- (iii) hypoxic or necrotic tissue characterization map;
- (iv) fibrous tissue map;
- (v) vasculature map;
- (vi) cancer cell/tissue map (where cancer is the condition being treated);
- (vii) a fluid distribution map (for visualizing injected or otherwise delivered therapeutic fluid in local tissue of the target anatomical structure);
- (viii) light exposure maps;

(h) at least one procedure planning map **37M** with one or more target sites **37p** (also referred to interchangeably herein as sites **55t**) and a later tissue map showing actual sites **37a** (e.g., target and actual ablation sites) shown in different colors, opacities and/or intensities for ease of reference (see, e.g., **Figure 10**, red/darker spots associated with target and green or lighter spots associated with actual); and

(i) device views **36** that show the physical representation of the device **80** in the surgical/imaging space, e.g., with an ablation catheter **36a** shown in position and/or a mapping (loop) catheter **36b** as devices **80** shown in position (**Figures 9, 11**). These device maps **36** may be used/displayed, for example, during a navigation mode. The default action may be to show these devices at least in the navigation mode but a user can deselect this choice. The devices may also be "turned" off or faded or shown in wire grid or otherwise in the visualizations subject typically to user input.

[0080] The tissue maps **30** (or associated tissue data) are typically registered to the 3-D coordinate MRI image space (manually or via automatic electronic image alignment registration means) or obtained during the procedure so that the MR image data is in the 3-D MRI image space. In some embodiments, relevant image scan planes and MR image data of the patient can be imported and/or incorporated into one or more of the tissue maps so that the map(s) can be updated over time (including in real time) using MR image data correlated with the anatomical location on the (updated) tissue map **30** automatically or upon request by a user. EA maps can be generated using tracking and/or mapping catheters in the 3-D MRI image space which may provide a more accurate or timely EA map (without requiring registration of a pre-acquired map).

[0081] The tissue map(s) **30** can be generated using MR image data that shows normal and abnormal status, conditions and/or behavior of tissue or status of tissue in response to a treatment. For example, a tissue characterization map(s) can show a thermal profile in different colors (or gray scale) of cardiac tissue in a region of interest and/or globally. In other embodiments, a tissue characterization map can illustrate one or more of infarct tissue, other injured tissue such as necrotic or scar tissue, hypoxic, ischemic, edemic (e.g., having edema) and/or fibrotic tissue or otherwise impaired, degraded or abnormal tissue as well as normal tissue on an anatomical model of the heart. In yet other embodiments, the tissue maps can illustrate portions of the heart (e.g., LA or posterior wall) with lesser or greater wall motion, and the like.

[0082] In some embodiments, the system can be used to deliver a therapeutic to target anatomy using an injection needle or fluid delivery cannula. A fluid distribution map or data therefrom can be shown on the model **100M** or in the MRI image **100MRI** (without requiring the rendered model). For example, to treat heart failure, a therapeutic agent can be injected into one or more target locations in infarct or abnormal cardiac tissue. Typically, the injection is carried out in several spots to generate a desired coverage pattern or area/volume. The fluid distribution map can be used to confirm that desired coverage of the cardiac tissue was obtained based on the injections. If not, another ("clean-up") target site or sites can be identified and the sites can be injected with the

therapeutic agent. In other embodiments, a previous injection site may need additional volumes of the agent, so that same site can be treated again. The fluid distribution map can be generated based on MRI image data alone. In other embodiments, a fluid distribution map can be generated based on a known injection site or sites, and a known volume of injected agent (which may be measured in situ or based on a known flow rate and known time of injection). This data can be used to generate an estimated fluid distribution map. In other embodiments, a fluid distribution map can be generated based on both MR image data and injection amounts. In some embodiments, the system/circuit 60c can identify a spatial grouping of injection sites and electronically select a scan plane or scan planes that can be set through the injection sites to obtain near RT MRI image data or obtain image data after the injections (such as for a regional or global coverage evaluation prior to the end of the MRI-guided procedure). For cardiac injections for some heart repairs, a planning map **37M** identifying infarct tissue and normal (healthy) tissue boundaries can be used to identify target injection sites **55t**. This map **37M** can be registered to the MRI image space. A target site **55t** can be associated with the X, Y, Z location in the MRI image space. Near RT images **100MRI** can be generated during the injections (similar to the ablations) to allow a physician to see "live" the injection distribution or disbursement. This fluid distribution map can be electronically provided as a data set that can be selectively shown on the anatomical model **100M**. The therapeutic agent can be any suitable agent including, for example, stem cells (and may be directed to rebuilding cardiac tissue) and is MRI visible.

[0083] Other embodiments can generate light exposure maps to evaluate optical light exposure of target tissue (or light activated drugs in such tissue) similar to the fluid distribution map discussed above. The light exposure map can be based on an internal laser or other light source that exposes the tissue to non-ablative energy.

[0084] Whether a parameter or tissue characteristic is shown in a respective tissue map **30** as being impaired, degraded or otherwise abnormal or affected by a therapy versus normal or untreated can be based on the intensity of pixels of the tissue characteristic in the patient itself or based on predefined values or ranges of values associated with a population "norm" of typical normal and/or abnormal values, or combinations of the above.

[0085] Thus, for example, normal wall motion can be identified based on a comparison to defined population norms and different deviations from that normal wall motion can be shown as severe, moderate or minimal in different colors relative to tissue with normal wall motion.

[0086] In another example, a thermal tissue characterization map **30** can illustrate tissue having increased temperatures relative to other adjacent or non-adjacent tissue. Thus, for example, during or shortly after ablation, the lesioned tissue and tissue proximate thereto can have

increased temperatures relative to the non-lesioned temperature or tissue at normal body temperatures. Areas or volumes with increased intensity and/or intensity levels above a defined level can be identified as tissue that has been ablated. The different ablation sites **55t** can be shown on the map **30** as areas with increased temperatures (obtained at different times during the procedure) and incorporated into the thermal tissue characterization map **30** automatically and/or shown upon request.

[0087] In some embodiments, the tissue characteristic map **30** uses MR image data acquired in association with the uptake and retention of a (e.g., T-1 shortening) contrast agent. Typically, a longer retention in tissue is associated with unhealthy tissue (such as infarct tissue, necrotic tissue, scarred tissue and the like) and is visually detectable by a difference in image intensity in the MR image data, e.g., e.g. using a T1 weighted sequence, to show the difference in retention of one or more contrast agents. This is referred to as delayed enhancement (DE), delayed hyper-enhancement (DHE) or late gadolinium enhancement (LGE). As discussed above, in some embodiments, the system/circuit can employ interactive application of non-selective saturation to show the presence of a contrast agent in near real-time scanning. This option can help, for example, during image-guided catheter navigation to target tissue that borders scar regions. Thus, the DHE image data in a DHE tissue characterization map can be pre-acquired and/or may include near-RT image data.

[0088] The tissue map is typically a volumetric, 3-D or 4-D anatomical map that illustrates or shows tissue characterization properties associated with the volume as discussed above. The map can be in color and color-coded to provide an easy to understand map or image with different tissue characterizations shown in different colors and/or with different degrees of a particular characterization shown in gray scale or color coded. The term "color-coded" means that certain features or conditions are shown with colors of different color, hue or opacity and/or intensity to visually accentuate different conditions or status of tissue or different and similar tissue, such as, for example to show fluid distribution from an injected therapeutic or lesions in tissue versus normal or non-lesion or non-injected/affected tissue.

[0089] In some embodiments, the UI **25** can be configured to allow a clinician to increase or decrease the intensity or change a color of certain tissue characterization types, e.g., to show lesion tissue or tissue having edema with a different viewing parameter, e.g., in high-contrast color and/or intensity, darker opacity or the like. A treatment site, such as a lesion site(s) in/on the tissue characterization map **30** can be defined based on a position in three-dimensional space (e.g., where an electrode is located based on location detectors, such as tracking coils, when the ablation electrode is activated to ablate), but is typically also or alternately associated with MRI image data in associated scan planes to show an ablation site(s) in an MRI image. The MR image data

may also reflect a change in a tissue property after or during ablation during the procedure, e.g., DHE, thermal, edema and the like.

[0090] The circuit **60c** can be configured to generate a tissue map **37M** (**Figure 27**) that is a difference or a comparison map that is generated from a pre-procedure or start-of procedure tissue data and an intra-procedure tissue data to show the differences based on the procedure. The "before" and "after" maps can be electronically overlaid on a display and shown in different colors, opacities and/or intensities or corresponding pixel values from each image in a region of interest (ROI) can be subtracted to show a difference map or otherwise integrated into a composite map. Again, the UI **25** can allow a clinician to select or deselect (or toggle between) the before or after tissue characterization maps or adjust display preferences to allow a visual review of differences.

[0091] A regional update tissue map **32** can be used to evaluate whether target or actual treatment sites have been successfully treated, e.g., whether ablated locations have the desired transmural lesion formation. For example, the UI **25** can allow the clinician to select a high resolution or enlarged view of the actual ablated tissue merely by indicating on the interactive map **100M**, such as a regional evaluation tissue map, a desired region of interest (e.g., by pointing a finger, cursor or otherwise selecting a spot on the display). For example, a high resolution MR image of suspect tissue in the LSPV can be shown so that the physician can see actual tissue in the desired spot indicated on the tissue characterization map. New targets can be electronically marked on the map as needed and scan planes can be automatically electronically be selected, identified or otherwise associated with the new target location.

[0092] **Figure 13** shows the display **20** with side-by-side viewing windows, one window showing the visualization with the map **100M** (which may be a tissue characterization map) and the other window with at least one near RT MRI image of local tissue during an active treatment mode.

[0093] **Figures 22A** and **22B** illustrate two windows of the axial and *en face* views of local tissue. **Figure 22A** shows the tissue prior to ablation and **Figure 22B** shows the tissue during or after an ablation. For example, during an ablation mode the system can use a default viewing rule to display the near real time MR image data of the affected tissue during the treatment, e.g., ablation, typically showing both *en face* and side views of the local tissue and treatment (ablation tip) according to embodiments of the present invention. In certain embodiments, the interactive visualization map **100v** and/or model **100M** may not be displayed during all or some of the ablation.

[0094] Referring to **Figures 8, 12, and 25**, in some embodiments, the UI **25** can also include a user input control **25c** to allow a user to identify and/or select (e.g., mark) target ablation sites **55t** on a tissue planning map **37M** and subsequently provide planned and actual ablation

tissue maps **37a** or (which may be overlaid with different colors for easy comparison in viewing) or merged into a composite map that indicates both planned and actual sites (**Figure 10**).

5 [0095] **Figure 14, 17 and 21** illustrate enlarged (high resolution image) views of tissue that can be shown based on actual MR image data. This allows a physician to see the tissue that is targeted for treatment (e.g., ablation) prior to and/or during treatment (e.g., ablation).
10 This type of viewing can be carried out during a planning stage or to evaluate lesions after ablation rather than just during the treatment for tissue-specific data. In some embodiments, the enlarged image views can be shown in response to user input in the interactive visualization.
15 That is, the image views can be based on the placement of a target treatment site **55t** in or on the map **100M**.

[0096] **Figure 14** illustrates that a clinician (physician) can mark an area on the model **100M** of the interactive visualization **100v** shown as a circle toward the left side
20 of the left window. **Figure 15** shows that the lesion pattern may be incomplete. **Figure 16** illustrates that the marked area in **Figure 14** may define the scan plane for the close-up views in the right hand viewing window.

[0097] **Figures 10, 12 and 13** illustrate a "complete" planning map **37M** with a number of target ablation sites **37p/55t** for forming desired transmural lesions and/or electrical isolation patterns as selected by the physician (user). **Figure 10** illustrates both planned and actual treatment sites. After a planned ablation pattern is indicated, or as a mark or particular lesion site is selected
25 and/or placed on the planning map **37M**, a physician/user can review real-time MR image data of the spot and affirm the selected site is a desired target ablation site(s) **55t**. **Figure 8** illustrates that the display can show a planned ablation site pattern **55t** applied to the model **100M** along with near real time patient MRI data.
30

[0098] In some embodiments, the planned treatment (e.g., ablation) pattern can use an electronically generated (default) template based on a predefined condition to be treated and certain fiducials associated with the target anatomy. The template may also be based on a clinician-specific preference for such a condition that can be electronically stored for use over different patients. The template can be modified based on patient-specific anatomy or other information. The ablation pattern can be electronically "drawn" or marked on the model **100M**
35 prior to its registration in the image space. The system can be configured to electronically identify relevant scan planes for the different marked lesion sites or areas after registration in the image space or propose scan planes that match contour of local anatomy that will include the target ablation site(s).
40

[0099] **Figure 17** illustrates that the display can show the interactive visualization **100v** in one viewing window and that previous ablations in the indicated region can have an electronic associated scan plane(s) that can be used to define a new (or current) scan plane for regional evaluation of the lesion or other therapy.
45

[0100] Figure 20 shows that the visualization 100v can be used to confirm a desired therapy plan (ablation sites) and set a regional scan plane. Note also the difference from Figure 8 with the visualization showing the model more predominant than the MR image data according to user input.

[0101] The model/map 100M can be shown in wire grid form (Figure 9) or in varying intensity or opacity based on user input or default settings. Figure 9 also shows the near RT image data suppressed or not shown in the visualization 100v.

[0102] Figure 22A shows that scan planes for the therapeutic (e.g., ablation) view(s) can be automatically determined based on the identified location of the tracking coil(s) 82c as discussed above.

[0103] The circuit 60c can electronically define and pre-set scan planes associated with a respective target ablation site correlated to an actual location in 3-D space which is then electronically stored in electronic memory as pre-set scan planes for that target location. The MRI images in treatment-view mode (e.g., ablation-view mode) can automatically be displayed when the treatment device 80 reaches the corresponding physical location in the target anatomy (e.g., heart) during the procedure. The planned target sites 55t may also be used to define the physician view (3-D perspective), e.g., a preset view, whenever the treatment device 80 (e.g., ablation catheter) is in proximity to the defined location associated with the target site. Thus, the target sites 55t identified in the planning map 37M can be used to preset both

associated scan planes with real time MRI and the 3-D view for display without requiring further clinician input. [0104] During the procedure, as the distal end of the device 80 (e.g., ablation catheter) approaches a location that corresponds to a target treatment (e.g., ablation) site 55t, the circuit 60c (e.g., MR Scanner 10S) can automatically select scan planes that "snap to" the tip and/or distal end portion location using a scan plane defined "on the fly" based on the calculated location of the distal end portion of the device (typically selected so that the slice includes a region offset from and/or projected forward a distance beyond the device such as between about 0-4 mm, typically about 1-2 mm) and/or using one or more of the preset scan planes associated with that location to obtain real-time MR image data of the associated tissue. The scan planes can be adjusted in response to movement of the device (as typically detected by tracking coils) prior to or during treatment. Figure 11 indicates an auto-view using a recalled preset scan plane as the device 80 nears or contacts target tissue. In some embodiments, the system may automatically enable or disable ECG gating as necessary when defining scan planes, markers, recording electrograms, and the like.

[0105] In some embodiments, the snap-to scan plane(s) can be carried out based on the position of two closely spaced tracking coils 82c on a distal end of the device 80. The two coils 82c can be held on a relatively rigid substrate or catheter end with between about 2-10

turns/coil. The tracking coils 82c can be connected via a respective coaxial cable to the MR scanner 10S as noted above. The snap-to or projected scan plane can be projected a distance beyond the calculated tip location, such as between about 0-4 mm as discussed above. This embodiment may be particularly suitable for a deflectable end ablation catheter with a tip RF electrode. In other embodiments, such as for a loop catheter, the tracking coils 82c can be held on a loop end of the device and reside on a common plane. The circuit 60c can be configured to define the plane based on the location of at least three of the tracking coils 82c. The tissue-device interface for the snap-to location can be selected to be parallel and proximate the identified plane (e.g., between about 0-4 mm from the plane). In yet another embodiment, a device can have between about 1-20 tracking coils along its length (e.g., along a distal end portion thereof). The snap-to location can be based on a location that is tangent and in-line with at least two of the tracking coils (e.g., 2, 3, 4 coils on the shaft). The device may deflect and the position of at least some of the tracking coils may change relative to each other. This embodiment may be particularly suitable for a mapping catheter which has a mostly straight configuration but may have a curved portion.

[0106] For example, in some embodiments, the circuit 60c and/or MR Scanner 10S can adjust the scan planes if the physician moves the ablation catheter to obtain slices that show the ablation of the lesion including side and *en face* views showing near real-time MRI of the tissue being ablated. The scan planes are selected to include slices that are projected outward a distance axially along the line of the device to include relevant tissue. For an optimal or proper *en face* view the scan plane can be oriented to a plane that is substantially parallel to the target tissue surface (e.g., proximate a tip of the device). This can be done based on coordinates of the 3D segmentation / model relative to the tip position.

[0107] To obtain a slice with a relevant scan plane for the *en face* view, the device tip can be used to define one point and the circuit could identify a plurality of additional points (e.g., about three more points) on the surface of the model 100M. Those additional points can be a short radius away from the device tip (i.e., similar to a spoke and wheel pattern). Distance of the (three) radial points should be closely spaced relative to the center point, particularly for curved tissue surfaces (e.g., the cardiac walls being ablated or otherwise treated will usually be curved, and in some cases, even have complex curves like the PV ostia). Choosing this distance may be made with reference to typical human cardiac anatomy, the distance of those points may be between about 3 to 5mm. In some particular embodiments, the following steps may be used to obtain the *en face* views.

1. Project a line forward from the most distal tracking coils on the intrabody device.
2. Electronically generate (e.g., mark) a temporary

point where that projected line intersects the surface of the 3D model

3. Use that temporary point of intersection as the center of the "wheel" and calculate the location of three points on the rim of the wheel.

4. Prescribe a temporary plane that includes the three rim points.

5. Translate the temporary plane until the temporary center point becomes coterminous with the actual tip of the device (assuming that the tip is actually against the target tissue (e.g., cardiac wall).

6. Set the scan plane based on this calculated plane for the *en face* view.

[0108] It is noted that the above steps may not be suitable where the device is a loop catheter. When using a loop catheter as the intrabody device with the tracking coils, the physician typically ablates on the inside of the loop and the circuit can use the coordinates of the tracking coils on the loop catheter to describe the scan plane for the *en face* view.

[0109] In some embodiments, the system can keep track of the shortest line from the tip of the device to the registered model, and can even display this line in near real-time in the rendering(s). Then, with user input, e.g. on a button press, the circuit **60c** can define a plane tangent to the model surface for the *en face* view, or along this line for the axial view. Gating may be used. The axial view may be more robust as it cuts through the wall.

[0110] In addition to substantially continuous collection of "new" image data in the visualizations and/or ablation or other therapy view modes, the data can also be processed by algorithms and other means in order to generate and present back to the surgeon in near real-time or upon request, a continuously updated, patient specific anatomical tissue characterization map of the anatomy of interest.

[0111] **Figure 23** illustrates that the system can illustrate the location of the treatment device **80** with additional visual indicators and a "target" navigational indicium (e.g., mark) for visual help in navigation to the site.

[0112] **Figures 24A-24D** illustrate that the system can generate visual navigational markers for facilitating alignment using MRI-guidance.

[0113] In particular embodiments, during ablation, MR thermometry (2-D) can be used to show real-time ablation formation taking a slice along the catheter and showing the temperature profile increasing. It is contemplated that 2D and/or 3D GRE pulse sequences can be used to obtain the MR image data. However, other pulse sequences may also be used.

[0114] **Figures 18** and **19** illustrate examples of maps **30** of pre-acquired patient data that can be imported (and registered to the image space) for use during a cardiac interventional procedure, typically used as the map **100M** in the interactive visualization **100v**. As shown in **Figure 18**, an EA map can be obtained prior to (typically immediately prior to) the actual interventional procedure either

while the patient is in the MRI scanner or from an X-ray based system from which the EA map can be registered to a different map, such as a tissue characterization map **30** and shown on the display **20**. In some embodiments,

5 the tissue characterization map can include, incorporate, overlay or underlay data from or an EA map (which may be imported from an X-ray imaging modality or generated in an MRI Scanner) to define an integrated electro and tissue characterization combination map. The electrical activity can be detected via electrical activity sensors that can detect impedance or other electrical parameter that can sense fractionated or normal electrical activity in cardiac tissue as is known to those of skill in the art. The electroanatomical map or data therefrom, where used, can be registered to the visualization map **100M** (e.g., a different tissue-characterization map) so that MR data updates using MR data that is generated during the intervention can be generated and displayed on the integrated map.

20 **[0115]** Also, the UI **25** can be configured to allow a clinician to select or deselect the EA map (where used) so that the information from the EA map is electronically stripped or removed (and/or added back in) to the map **100M** as desired. In other embodiments, the map **100M** is maintained separate from the EA map, and if used, the EA map is shown in a separate window or screen apart from the tissue characterization map.

25 **[0116]** **Figures 21** and **27** show examples of MRI DHE tissue characterization maps. **Figure 21** shows a pre-procedure "planning" DHE image taken before, typically about 1 week before, the planned procedure. In some embodiments, a DHE image can be taken after a prior ablation procedure illustrating locations of incomplete electrical isolation/scar formation for helping plan the target sites for the current procedure. A planning map can be placed over the map in the visualization so that a user/physician can mark the target ablation sites **55t** as discussed above (which may in some embodiments also define preset scan planes and views before ablating during a procedure). **Figure 27** shows an intraprocedure DHE map that can be used to evaluate the ablation sites.

30 **[0117]** **Figure 28** illustrates that the map **100M** can be rendered to show locations of target and actual ablation sites (in different colors) to allow a clinician to evaluate the scar formations and/or variation from the planned procedure intra-procedure according to embodiments of the present invention.

35 **[0118]** The MRI Scanner **10S** (**Figures 1-3**) can be operated substantially continuously to provide image data that can be used to generate updated maps **100M** in the visualizations upon request or automatically. This operation can be "in the background", e.g., transparent to the user so as not to slow down the procedure while providing updated image and tracking data during the course of the procedure.

40 **[0119]** In some embodiments, the device-tissue interface **100i** (**Figure 1, 22A, 22B**) can be visualized with a T1-weighted FLASH sequence (T1w FLASH) to localize

the tip **80t**. RF or other ablative energy can be delivered and myocardial or other target tissue changes and lesion formation can be visualized in near real-time using a T2 weighted HASTE (T2w HASTE) sequence. Real Time (RT)-MRI sequence, T1w FLASH and T2w HASTE image slices can be aligned to allow visualization of the device **80** upon tissue contact or activation of the ablation energy to allow visualization of the device **80** (e.g., catheter), the device-tissue interface **100i** and/or the (myocardium) tissue while receiving the therapy, e.g., ablative energy.

[0120] In some particular embodiments, during navigation mode (rather than an ablation mode), the catheter **80** can be visualized using a different pulse sequence from that used in the high-resolution ablation mode, such as, for example, an RT MRI sequence using GRE or SSFP (e.g., TrueFISP) pulse sequence with about 5.5 fps), the tracking coils **82c** can be used for spatial orientation and positioning. Typical scan parameters for (near) real-time include: echo time (TE) 1.5 ms, repetition time (TR) 3.5 ms, a flip angle of about 45 degrees or about 12 degrees, slice thickness 5 mm, resolution 1.8 mm x 2.4 mm, parallel imaging with reduction factor (R) of 2. In some embodiments using SSFP, the flip angle is about 45 degrees.

[0121] Once the device position is deemed appropriate (using tracking coils **82c**), a pulse sequence at the associated scan plane can be used to generate high resolution visualization of the catheter tip **80t** and (myocardial) tissue interface. For example, a T1-weighted 3D FLASH sequence (T1w FLASH) as noted above. Myocardial or other target tissue images during ablation or other therapy can be acquired using an Inner Volume Acquisition (IVA) dark-blood prepared T2-weighted HASTE (T2w HASTE) or dark-blood prepared Turbo Spin Echo (TSE) sequence. Examples of HASTE and TSE sequence parameters include: TE=79ms/65ms, TR=3 heart beats, 3 contiguous slices with thickness of about 4 mm, resolution 1.25 mm x 1.78 mm/1.25 mm x 1.25 mm, fat saturation using SPAIR method, and parallel imaging with R=2, respectively.

[0122] Typical heart beat rates and free breathing can present imaging challenges. In some embodiments, (near) RT navigation imaging slices (e.g., GRE pulse sequence at 5.5 fps) can be aligned with high-resolution tissue interface slices (e.g., T1w FLASH) for visualization of the catheter-tissue interface. Subsequently, those slices obtained with T1w FLASH can be aligned with those obtained with dark-blood prepared T2w Haste images for myocardial tissue/injury characterization during energy delivery. This stepwise approach can allow confident localization of specific points within the atrium and while ablating tissue and simultaneously visualizing the tissue for near-real time assessment of tissue injury associated with lesion formation.

[0123] In some embodiments, slices acquired with different sequences can be interlaced to provide an interactive environment for catheter visualization and lesion

delivery, a UI can allow a user to toggle between these views or can alternate the views based on these image slices or navigation versus ablation or interventional modes/views. It is also noted that the sequences described herein are provided as examples of suitable sequences and it is contemplated that other known sequences or newly developed sequences may be used for cardiac ablation or other anatomy or interventional procedures.

[0124] **Figure 29** illustrates one particular embodiment using a cardiac MRI Interventional suite **19** with an integrated cable management system that connects multiple patient connected leads that remain in position even when a patient is translated in or out of a magnet bore on the gantry **16** (the magnet can be an open face or closed magnet configuration) to allow a clinician direct access to a patient. The other ends of the leads connect to power sources, monitors and/or controls located remote from the patient (typically in the control room not the magnet room). As shown in **Figure 29**, the MRI interventional suite **19** can include an IV pole **140** (typically attached to the scanner table/gantry **16**) and a connection block **150** of cables **200n** that are routed through a ceiling (e.g., they extend up, through and above a ceiling) (where "n" is typically between about 1-400, typically between about 5-100), that connect to patch bay **135** and/or **137**. Cabling **210n** for anesthesia cart **160** can also be routed through the ceiling (where n is typically between about 1-400, typically between about 5-100). The cabling **200n**, **210n** extends through the ceiling between the rooms **10a**, **10b** and can connect to the remote devices **500** through a patch panel **250**. In some embodiments foot pedal cabling **220n** can extend through a floor trough to the patch panel/second room **10b** as well (where "n" is typically between about 1-100 cables). For additional description of an exemplary cardiac suite, see U.S. Patent Application Serial No. 12/708,773. The cables may also alternately be routed under, on or over the floor, suspended on walls, employ wireless connections and the like (and combinations of same).

[0125] As is known to those of skill in the art, there are typically between about 60-100 lesions generated during a single patient cardiac (AFIB) EP procedure. Other cardiac procedures may only require about 1 ablation or less than 60. A typical patient interventional cardiac procedure lasts less than about 4 hours, e.g., about 1-2 hours. Each lesion site can be ablated for between about 30 seconds to about 2 minutes. Linear transmural lesions (such as "continuous" drag method lesions) may be generated or "spot" lesions may be generated, depending on the selected treatment and/or condition being treated. The continuous lesion may be formed as a series of overlapping spot ablation lesions or as a continuous "drag" lesion.

[0126] The system can include a monitoring circuit can automatically detect which devices are connected to the patient patch bay. One way this can be achieved is by using ID resistors in the patch bay and/or interface as

well as in various devices that connect thereto. The MRI scanner computer or processor or the clinician workstation module or processor can monitor resistors via connections CON1, CON2 and CON3. The devices **80** (**Figure 1**) can have built-in resistors that modify the resistance by lines that connect to CON1, CON2 and CON3. Variation in resistance values helps the monitor which device is connected. Once that determination is made the scanner may automatically load special acquisition parameters, display parameters and update the progress of the procedure to display on the display **20** such as at workstation **60** (**Figure 3**), for example.

[0127] Electrical isolation between the MR Scanner **10S** and the device **80** can be provided via low pass filters inside and outside the MRI suite. As is known to those of skill in the art, components in the MRI Suite can be connected to external components using a waveguide built into the RF shield that encloses the MRI suite. Where used, the ablation catheter **80a** can be an RF ablation catheter connected to an appropriate energy source, such as, for example, a Stockert 70 RF generator (Bio-sense Webster, Diamond Bar, CA, USA) with MR compatible interface circuits configured for 3T magnetic fields (where a 3T system is used). The system can comprise an EP Suite with a Siemens Verio system (Siemens Healthcare, Erlangen, Germany) or other suitable scanner as well as suitable external imaging coils, such as spine and/or body array coils as is known to those of skill in the art. Other ablation catheters including balloon (cryoablation), laser, ultrasound and RF array electrodes and the like may also be used. Other therapeutic catheters or devices may be used including an injection needle catheter and the like.

[0128] **Figures 30A, 30B, and 31-33** illustrate exemplary embodiments of a flexible (steerable) ablation catheter as the device **80**. The ablation catheter **80A** includes an elongated flexible housing or shaft **102** having a lumen **104** (**Figure 30B**) therethrough and includes opposite distal and proximal end portions, only the distal end portion **106** is illustrated. The distal end portion **106** includes a tip portion **101** that contains an ablation electrode **110** at its tip **80t** for ablating target tissue, and a pair of RF tracking coils **82c**, individually identified as **112, 114**. The distal end portion can include a second electrode for sensing local electrical signal or properties or the ablation electrode **110** can be bipolar and both ablate and sense. The proximal end portion of the catheter **80** is operably secured to a handle as is well known. The catheter shaft **102** is formed from flexible, bio-compatible and MRI-compatible material, such as polyester or other polymeric materials. However, various other types of materials may be utilized to form the catheter shaft **102**, and embodiments of the present invention are not limited to the use of any particular material. In some embodiments, the shaft distal end portion can be formed from material that is stiffer than the proximal end portion and/or a medial portion between the distal and proximal end portions.

[0129] The device **80** can be configured to reduce the

likelihood of undesired deposition of current or voltage in tissue. The device **80** can include RF chokes such as a series of axially spaced apart Balun circuits or other suitable circuit configurations. See, e.g., U.S. Patent No. 6,284,971 for additional description of RF-inhibiting coaxial cable that can inhibit RF-induced current.

[0130] The device **80** can include tracking coils **112, 114** (**Figures 30A, 30B, 31**) on a distal end portion. In some embodiments, the tracking coils **82c** reside upstream of the tip of the device (e.g., needle or ablation electrode). As shown in **Figures 30A, 30B** and **31**, the ablation catheter includes a pair of tracking coils that reside adjacent to but typically upstream of the ablation electrode **110** on the tip of the catheter **80t**) as all or some of tracking members **82** (**Figure 1**). The catheter **80** can include an RF wire **120** that connects the ablation electrode **110** to an RF generator (**Figures 30B, 31**).

[0131] The device **80** can comprise coaxial cables **81** that connect the tracking coils **82c** to the MR Scanner for tracking the location of the catheter in 3-D space. The cables or conductors **81** (and/or RF wire **120** where used) can include a series of back and forth segments (e.g., it can turn on itself in a lengthwise direction a number of times along its length), include stacked windings and/or include high-impedance circuits. See, e.g., U.S. Patent Application Serial Nos. 11/417,594; 12/047,832; and 12/090,583. The conductors (e.g., coaxial cables) **81** (and/or RF wire **120**, where used) can be co-wound in one direction or back and forth in stacked segments for a portion or all of their length.

[0132] In some embodiments, the ablation tip **80t** is provided with one or more exit ports **132** (**Figure 30A**) in communication with a fluid channel through which a fluid/solution (irrigant), such as saline, can flow before, during, and/or after the ablation of tissue. Fluid/solution is provided to the one or more exit ports **132** via an irrigation lumen **134** that extends longitudinally through the catheter shaft lumen **104** from the exit port(s) **132** to a handle. The irrigation lumen **134** is in fluid communication with a fluid/solution source at the proximal end portion **108** of the catheter shaft, typically at the handle. The fluid/solution can provide coolant and/or improve tissue coupling with the ablation electrode **110**.

[0133] In some embodiments, a pull wire **136** (**Figure 32, 33**) extends longitudinally within the catheter shaft lumen **104** from the distal end portion **106** to the handle at the catheter proximal end portion. The pull wire **136** extends longitudinally within a sleeve **138** (**Figure 32**) that is attached to the internal wall of the lumen **104**. The pull wire **136** is attached to the sleeve **138** near the distal end portion **106** of the catheter **80** and otherwise is slidably disposed within the sleeve. Pulling the pull wire **136** in a direction towards the handle causes the tip portion **101** of the catheter to articulate in one direction. Pushing the pull wire **136** in the opposite direction away from the handle causes the tip portion **101** to articulate in another different direction.

[0134] **Figures 32** and **33** are cross sectional views of

the distal end portion **101** of the illustrated catheter **80** according to some embodiments of the present invention. The sectional view shown in **Figure 32** is taken further upstream from that shown in **Figure 33**. **Figure 32** illustrates the location and configuration of the coaxial cables (generally referred to as element **60**) particularly referred to as **116**, **118**, **126** and **128** which are connected to the tracking coils **112**, **114**, **122** and **124**, respectively. Coils **122**, **124** are upstream of the portion of the device shown in **Figures 30A** and **30B**. **Figure 32** also illustrates the location and configuration of the RF wire **120** that is connected to the ablation tip electrode **110** and that provides RF energy to the ablation tip electrode **110**. **Figure 32** also illustrates the location of an exemplary thermocouple **130**, and the location of an irrigation lumen **134**. **Figure 33** illustrates the location and configuration of the coaxial cables **116**, **118** which are connected to the RF tracking coils **112**, **114**. **Figure 33** also illustrates the location and configuration of the RF wire **120** connected to the ablation tip electrode **110**, the location of thermocouple **130**, and the location of irrigation lumen **134**.

[0135] As discussed above with respect to **Figure 4**, each tracking coil circuit can include a PIN diode and DC blocking capacitor and is typically located within the handle, although in other embodiments, the tracking coil circuits can be located within the catheter shaft lumen **104** closer to a medial or distal end portion (not shown) or in an interface, connector or other location. Each tracking coil circuit can be electrically connected to an MRI scanner, and can reduce signal noise within a respective channel caused by undesired coupling during scanner operation. In some embodiments, the tracking coil circuit can produce about 100 ohms impedance across an RF tracking coil when the PIN diode is shorted, for example, by an MRI scanner during scanner operations.

[0136] In some embodiments of the present invention, RF tracking coils **112**, **114**, **122**, **124** may be between about 2-16 turn solenoid coils, typically 2-10 turn solenoid coils. However, other coil configurations may be utilized in accordance with embodiments of the present invention. Each of the RF tracking coils **112**, **114**, **122**, **124** can have the same number of turns or a different number of turns, or different ones of the RF tracking coils **112**, **114**, **122**, **124** can have different numbers of turns. It is believed that an RF tracking coil with between about 2-4 turns at 3.0 T provides a suitable signal for tracking purposes.

[0137] Embodiments of the present invention may be utilized in conjunction with navigation and mapping software features. For example, current and/or future versions of devices and systems described herein may include features with adaptive projection navigation and/or 3-D volumetric mapping technology, the latter may include aspects associated with U.S. Patent Application 10/076,882, which is incorporated herein by reference in its entirety.

[0138] **Figures 34** and **35** are flow charts of steps that can be implemented to carry out embodiments of the

present invention. Although the steps are shown in a particular order in these figures, neither the order of steps in these figures or the order of these figures is meant to indicate any required order in the implementation of one or more of the methods and/or method steps. Further, it will be appreciated that certain of the steps can be carried out simultaneously rather than serially and the blocks are stated for ease of discussion rather than as a limitation on how or when the operations are carried out.

[0139] A flexible intrabody medical device is introduced into a natural lumen or cavity of a patient during an MRI-guided procedure (block **200**). Tracking signals are electronically obtained from tracking coils connected to an MR Scanner and attached to the flexible intrabody device during the MRI-guided procedure. The intrabody device has a distal end portion that can take on a curvilinear shape as it moves into position in the patient's body (block **202**). X, Y, Z coordinate locations are electronically identified in 3-D MRI image space for each of the tracking coils using the tracking signals (block **204**). MR image data are obtained and near RT MR images of the patient are generated during the MRI-guided procedure (block **206**). A pre-acquired 3-D volumetric model of target anatomy of the patient is obtained and registered to the 3-D image space (block **208**). Near real time (RT) visualizations of the medical device are generated showing: (a) the model of the patient's anatomy; (b) a physical representation of at least a distal end portion of the medical device using the identified locations of the tracking coils; and (c) at least one of the near RT MR images (block **210**).

[0140] Optionally, a tip location and/or a device-tissue interface location proximate a tip location of the device in the three dimensional image space is electronically calculated using the identified locations of the tracking coils. The calculating step may project axially forward a defined distance (e.g., between about 0-4 mm, typically between about 0-2 mm) beyond the tip to define the device-tissue interface and at least one scan plane used to obtain the MR image data for the near RT images during and/or proximate in time to delivery of a therapeutic treatment and/or a diagnostic procedure is electronically defined using the calculated location (block **212**). A user (via a UI) may be able to select the desired projection forward distance for the scan plane/slice location. The system may include a default distance (e.g., the end of the tip or distance forward = about 0 or 0.1 mm) that can be adjusted prior to or during a procedure.

[0141] Optionally, the visualizations can be electronically rotated based on user input and electronically selectively altering a view of the displayed visualization based on user input so that the visualization includes the at least one flexible device with (a) only a near RT image of the target anatomy, (b) both the near RT image of the anatomy and the registered model of the anatomical structure, or (c) only the registered model of the anatomical structure (block **214**).

[0142] As shown in **Figure 35**, at least one tissue characterization map or data therefrom can be electronically

(programmatically) generated to render and display at least a portion of a patient's heart (e.g., the entire heart, the LA, or other desired region) (block 300). Optionally, the tissue characterization map is configured to be rotatable, zoomed, sectioned, cropped and a window can show associated MR image data for a requested region (block 303). User input can be accepted to indicate (mark) target ablation locations on the tissue characterization map or an EA map registered to image space (block 305). Optionally, a UI can allow a user to select a plurality of different tissue characterization maps that can be overlaid or shown separately or merged into a composite map (block 307). In response to the user input, the system can electronically and/or programmatically define relevant scan planes for each indicated target ablation location as preset scan planes (typically prior to initiating the ablation procedure) (block 310). The preset scan planes are for generating real time MRI when the ablation catheter is at the corresponding site. Although, the preset scan planes are described as defined by a UI that allows a clinician/physician to mark/indicate target ablation sites on a tissue characterization map, it is contemplated that the planning map can be another type of map, such as, for example, an electroanatomical map registered to the anatomical space.

[0143] In some embodiments, the UI can include a slide or toggle or other input means that allows a user to selectively fade between a view on a display with only the tissue characterization map, to a view with part Real-Time (RT) MR image data and part tissue characterization map and to a view with only RT MR image data (block 109) on the same viewing window.

[0144] During a procedure, the location of an intracardiac ablation catheter can be shown with respect to the registered map (block 315). Optionally, MR image data can substantially continuously be electronically obtained and used to update one or more respective tissue characterization maps during a therapy session (block 317). As the ablation portion of the catheter (e.g., electrode at tip) approaches one of the previously indicated target locations, the MRI Scanner is directed to scan ("snap to") the associated preset scan planes (block 320). Optionally, the MR Scanner can be programmatically directed to select scan planes that includes a slice that is aligned with an axial direction of the ablation catheter and that projects forward from the tip of the catheter (block 322). Also optionally, during ablation at least one real-time MR lesion image (close-up view) can be displayed based on tissue being ablated by the ablation catheter in a window on a display at the workstation (block 325). This may be a high resolution image of the local tissue using an internal receive antenna. Optionally, during the ablation, both an *en face* and side view of the lesion being formed in tissue can be displayed (block 326).

[0145] At least one tissue characterization map can be generated and displayed, color coded to illustrate the ablation lesions made during the procedure based on MR image data (block 330). Optionally, the tissue character-

ization map can be displayed with the (planned) indicated target ablation locations in a first color, intensity and/or opacity along with an updated tissue characterization map with MR image data showing actual ablated tissue locations in a different color (side by side or one over the other) (block 332).

[0146] Although described primarily herein with respect to Cardiac EP procedures using ablation electrodes, other ablation techniques can be used, such as, for example, laser ablation, thermal (heated liquid) ablation and cryoablation. Where used, the ablation catheter 80a can be an RF ablation catheter but can also or alternatively be configured to apply other ablations including cryogenic (e.g., cryoablation usually via an inflatable cryoballoon), laser, microwave, and even chemical ablation. In some embodiments, the ablation can be carried out using ultrasound energy. In particular embodiments, the ablation may be carried out using HIFU (High Intensity Focused Ultrasound). When MRI is used this is sometimes called Magnetic Resonance-guided Focused Ultrasound, often shortened to MRgFUS. This type of energy using a catheter to direct the energy to the target tissue can heat the tissue to cause necrosis.

[0147] Similarly, the systems and components can be useful for other MRI guided surgical intervention procedures, including, for example, delivering biologics or other drug therapies to target locations in cardiac or other tissue using MRI.

[0148] Some interventional tools may include an MRI receive antenna for improved SNR of local tissue. In some embodiments, the antenna has a focal length or signal-receiving length of between about 1-5 cm, and typically is configured to have a viewing length to receive MRI signals from local tissue of between about 1-2.5 cm. The MRI antenna can be formed as comprising a coaxial and/or triaxial antenna. However, other antenna configurations can be used, such as, for example, a whip antenna, a coil antenna, a loopless antenna, and/or a looped antenna. See, e.g., U.S. Patent Nos. 5,699,801; 5,928,145; 6,263,229; 6,606,513; 6,628,980; 6,284,971; 6,675,033; and 6,701,176. See also U.S. Patent Application Publication Nos. 2003/0050557; 2004/0046557; and 2003/0028095. Image data can also include image data obtained by a trans-esophageal antenna catheter during the procedure. See, e.g., U.S. Patent No. 6,408,202.

[0149] As discussed above, embodiments of the present invention may take the form of an entirely software embodiment or an embodiment combining software and hardware aspects, all generally referred to herein as a "circuit" or "module." Furthermore, the present invention may take the form of a computer program product on a computer-usable storage medium having computer-usable program code embodied in the medium. Any suitable computer readable medium may be utilized including hard disks, CD-ROMs, optical storage devices, a transmission media such as those supporting the Internet or an intranet, or magnetic storage devices. Some cir-

cuits, modules or routines may be written in assembly language or even micro-code to enhance performance and/or memory usage. It will be further appreciated that the functionality of any or all of the program modules may also be implemented using discrete hardware components, one or more application specific integrated circuits (ASICs), or a programmed digital signal processor or microcontroller. Embodiments of the present invention are not limited to a particular programming language.

[0150] Computer program code for carrying out operations of data processing systems, method steps or actions, modules or circuits (or portions thereof) discussed herein may be written in a high-level programming language, such as Python, Java, AJAX (Asynchronous JavaScript), C, and/or C++, for development convenience. In addition, computer program code for carrying out operations of exemplary embodiments may also be written in other programming languages, such as, but not limited to, interpreted languages. Some modules or routines may be written in assembly language or even micro-code to enhance performance and/or memory usage. However, embodiments are not limited to a particular programming language. It will be further appreciated that the functionality of any or all of the program modules may also be implemented using discrete hardware components, one or more application specific integrated circuits (ASICs), or a programmed digital signal processor or microcontroller. The program code may execute entirely on one (e.g., a workstation computer or a Scanner's computer), partly on one computer, as a stand-alone software package, partly on the workstation's computer or Scanner's computer and partly on another computer, local and/or remote or entirely on the other local or remote computer. In the latter scenario, the other local or remote computer may be connected to the user's computer through a local area network (LAN) or a wide area network (WAN), or the connection may be made to an external computer (for example, through the Internet using an Internet Service Provider).

[0151] The present invention is described in part with reference to flowchart illustrations and/or block diagrams of methods, apparatus (systems) and computer program products according to embodiments of the invention. It will be understood that each block of the flowchart illustrations and/or block diagrams, and combinations of blocks in the flowchart illustrations and/or block diagrams, can be implemented by computer program instructions. These computer program instructions may be provided to a processor of a general purpose computer, special purpose computer, or other programmable data processing apparatus to produce a machine, such that the instructions, which execute via the processor of the computer or other programmable data processing apparatus, create means for implementing the functions/acts specified in the flowchart and/or block diagram block or blocks.

[0152] These computer program instructions may also be stored in a computer-readable memory that can direct

a computer or other programmable data processing apparatus to function in a particular manner, such that the instructions stored in the computer-readable memory produce an article of manufacture including instruction means which implement the function/act specified in the flowchart and/or block diagram block or blocks.

[0153] The computer program instructions may also be loaded onto a computer or other programmable data processing apparatus to cause a series of operational steps to be performed on the computer or other programmable apparatus to produce a computer implemented process such that the instructions which execute on the computer or other programmable apparatus provide steps for implementing some or all of the functions/acts specified in the flowchart and/or block diagram block or blocks.

[0154] The flowcharts and block diagrams of certain of the figures herein illustrate exemplary architecture, functionality, and operation of possible implementations of embodiments of the present invention. In this regard, each block in the flow charts or block diagrams represents a module, segment, or portion of code, which comprises one or more executable instructions for implementing the specified logical function(s). It should also be noted that in some alternative implementations, the functions noted in the blocks may occur out of the order noted in the figures. For example, two blocks shown in succession may in fact be executed substantially concurrently or the blocks may sometimes be executed in the reverse order or two or more blocks may be combined, depending upon the functionality involved.

[0155] The workstation **60** and/or interface **44, 84**, or patch bay, may also include a decoupling/tuning circuit that allows the system to cooperate with an MRI scanner **10S** and filters and the like. See, e.g., U.S. Patent Nos. 6,701,176; 6,904,307 and U.S. Patent Application Publication No. 2003/0050557.

[0156] In some embodiments, the intrabody device **80** is configured to allow for safe MRI operation so as to reduce the likelihood of undesired deposition of current or voltage in tissue (inhibit or prevent undesired heating). The device **80** can include RF chokes such as a series of axially spaced apart Balun circuits or other suitable circuit configurations. See, e.g., U.S. Patent No. 6,284,971 for additional description of RF-inhibiting coaxial cable that can inhibit RF-induced current. The conductors connecting electrodes or other components on or in the catheter (or other interventional device) can also include a series of back and forth segments (e.g., the lead can turn on itself in a lengthwise direction a number of times along its length) and/or include high-impedance circuits. See, e.g., U.S. Patent Application Serial Nos. 11/417,594; 12/047,602; and 12/090,583.

[0157] Although not shown, in some embodiments, the device can be configured with one or more lumens and exit ports and can be used and/or deliver desired cellular, biological, and/or drug therapeutics to a target area.

[0158] **Figure 36** is a schematic illustration of a circuit

or data processing system that can be used with the system **10**. The circuits and/or data processing systems **190** may be incorporated in a digital signal processor in any suitable device or devices. As shown in **Figure 36**, the processor **410** communicates with and/or is integral with an MRI scanner **10S** and with memory **414** via an address/data bus **448**. The processor **410** can be any commercially available or custom microprocessor. The memory **414** is representative of the overall hierarchy of memory devices containing the software and data used to implement the functionality of the data processing system. The memory **414** can include, but is not limited to, the following types of devices: cache, ROM, PROM, EPROM, EEPROM, flash memory, SRAM, and DRAM.

[0159] **Figure 36** illustrates that the memory **414** may include several categories of software and data used in the data processing system: the operating system **449**; the application programs **450**; the input/output (I/O) device drivers **458**; and data **456**. The data **456** can also include device (ablation catheter) dimensions (e.g., distance of a tracking coil to the tip) and patient-specific image data **455**. **Figure 36** also illustrates the application programs **454** can include a Tracking Coil Location Identification Calculation Module **451**, a Visualization Rendering Module **452**, an Interactive Visualization (and UI) Module **453**, a Tissue Characterization Map Module **456**, and a Pre-Set Scan Plane to Target Ablation Site Module **454**, a and a UI Interface Module **453**.

[0160] As will be appreciated by those of skill in the art, the operating systems **449** may be any operating system suitable for use with a data processing system, such as OS/2, AIX, or zOS from International Business Machines Corporation, Armonk, NY, Windows CE, Windows NT, Windows95, Windows98, Windows2000, WindowsXP, Windows Vista, Windows7, Windows CE or other Windows versions from Microsoft Corporation, Redmond, WA, Palm OS, Symbian OS, Cisco IOS, VxWorks, Unix or Linux, Mac OS from Apple Computer, LabView, or proprietary operating systems. For example, VxWorks which can run on the Scanner's sequence generator for precise control of pulse sequence waveform timings.

[0161] The I/O device drivers **458** typically include software routines accessed through the operating system **449** by the application programs **450** to communicate with devices such as I/O data port(s), data storage **456** and certain memory **414** components. The application programs **450** are illustrative of the programs that implement the various features of the data processing system and can include at least one application, which supports operations according to embodiments of the present invention. Finally, the data **456** represents the static and dynamic data used by the application programs **450**, the operating system **449**, the I/O device drivers **458**, and other software programs that may reside in the memory **414**.

[0162] While the present invention is illustrated, for example, with reference to the Modules **451**, **452**, **453**, **454**, **456** being application programs in **Figure 35**, as will be

appreciated by those of skill in the art, other configurations may also be utilized while still benefiting from the teachings of the present invention. For example, the Modules and/or may also be incorporated into the operating system **449**, the I/O device drivers **458** or other such logical division of the data processing system. Thus, the present invention should not be construed as limited to the configuration of **Figure 36** which is intended to encompass any configuration capable of carrying out the operations described herein. Further, one or more of modules, *i.e.*, Modules **451**, **452**, **453**, **454**, **456** can communicate with or be incorporated totally or partially in other components, such as separate or a single processor, an MRI scanner **10S** or workstation **60**.

[0163] The I/O data port can be used to transfer information between the data processing system, the workstation, the MRI scanner, and another computer system or a network (e.g., the Internet) or to other devices controlled by the processor. These components may be conventional components such as those used in many conventional data processing systems, which may be configured in accordance with the present invention to operate as described herein.

[0164] Non-Limiting Examples of Tissue Characterization Maps will be discussed below.

Thermal Tissue Characterization Map

[0165] The thermal tissue characterization map can be based on thermal status at a given point in time or may be provided as a composite of heating of different tissue locations at different times (e.g., during and/or after ablation of different points at different times of the ablation procedure). The thermal map can be registered to a location of the internal ablation catheter (e.g., tip) at different times so that the location of the ablation catheter tip is correlated to the thermal activity/status at that location at that time as that is the time frame that the image data for that region illustrating increased thermal activity/heating is generated. That is, the image scan planes are taken to show the tissue at the location of the ablation catheter tip. The image scan planes are typically projected forward a known distance from the tracking coil so that the lesion tissue in front of the ablation tip is imaged.

[0166] The MR thermal data can be obtained using temperature imaging techniques (MR thermometry) to show temperature or phase variance. Examples of pulse sequences include, for example, SSFP and 2D GRE.

Vasculature Tissue Characterization Map

[0167] Segmented MRA (Magnetic Resonance Angiography) imaging volumes of a patient can be used to generate a vasculature tissue characteristic map which may indicate areas of increased blood flow and/or larger and smaller channels within the vasculature structure.

Fibrous Tissue Characterization Map

[0168] Contrast-based or non-contrast based MRI images of the patient can identify fibrous tissue in target tissue (e.g., the heart).

Contrast-Based Tissue Characterization Maps

[0169] Tissue damage can be shown or detected using MR image data based on contrast agents such as those agents that attach to or are primarily retained in one of, but not both, healthy and unhealthy tissue, e.g., the contrast agent is taken up by, attaches to, or resides or stays in one more than in the other so that MR image data will visually indentify the differences (using pixel intensity). The contrast agent can be one or more of any known or future developed biocompatible agent, currently typically gadolinium, but may also include an antibody or derivative or component thereof that couples to an agent and selectively binds to an epitope present in one type of tissue but not the other (e.g., unhealthy tissue) so that the epitope is present in substantially amounts in one type but not the other. Alternatively, the epitope can be present in both types of tissue but is not susceptible to bind to one type by steric block effects.

[0170] A tissue characteristic map registered to the imaging space can allow a clinician to assess both scar formation (isolation of the PV) and the volume of enhancement on a LA myocardial volume may indicate a poor outcome prediction and a clinician may decide to continue ablating or alter the ablation location or protocol (e.g., drive a clinical decision).

[0171] Examples of pulse sequences that can be used for delayed hyper-enhancement MRI include, for example, gradient echo, SSFP (steady state free precession) such as TrueFISP on Siemens MRI Scanners, FIESTA on GE MRI Scanners, and b-FFE on Philips MRI Scanners.

Edema Tissue Characterization Maps

[0172] After (and/or during) ablation, tissue will typically have edema. This can be detected in MRI using, for example, pulse sequences such as T2-weighted Turbo-Spin-Echo, HASTE (a Siemens term), SSFP, or T2-weighted gradient recalled echo (GRE).

[0173] Some tissue characterization maps may show edema and thermal maps overlaid or otherwise combined as a composite map that can be used to evaluate a procedure. For example, to visually assess whether there is complete or incomplete scar formation to isolate pulmonary veins. It is believed that complete scar formation to isolate PV is associated with a better prognosis for AFIB.

Heart Wall Motion Tissue Characterization Maps

[0174] MRI can be used to assess heart wall motion.

Abnormal motion can be visually indicated on the tissue characterization map. Examples of pulse sequences that may be used to determine heart wall motion include, for example, DENSE, HARP and MR tagging.

5 **[0175]** Thus, it will be appreciated that embodiments of the present invention are directed to systems, including hardware and/or software and related methodology to substantially continuously collect and construct, through-
10 out an MRI-guided cardiac procedure, e.g., an MRI-guided procedure, a patient-specific anatomical tissue characterization map or associated data that can be shown on a map of a target anatomical structure/region (e.g., a chamber of the heart such as the atrium). Embodiments of the system can generate and show in pre-set views and in near-real time during the procedure tissue while it is being treated, e.g., ablated.

15 **[0176]** While embodiments have been primarily discussed with respect to an MRI-guided cardiac system, the system can be used for other anatomical regions and deliver or apply other therapies as well as for diagnostic procedures. For example, the esophagus and anatomy near the esophagus, e.g., the aorta, coronary arteries, mediastinum, the hepatocobiliary system or the pancreas
20 in order to yield anatomic information about the structures in those areas, "pancreaticobiliary" structures (collectively the structures of the liver, gallbladder, bile ducts and pancreas), the tracheobronchopulmonary structure (structures including the lungs and the tracheobronchial tree), the nasopharynx system (e.g., a device
25 introduced transnasally may be adapted for evaluating the arterial circle of Willis and related vascular structures for abnormalities, for example congenital or other aneurysms), the proximal aerodigestive system or the thyroid, the ear canal or the Eustachian tube, permitting anatomic
30 assessment of abnormalities of the middle or inner ear, and further permitting evaluation of adjacent intracranial structures and lesions.

35 **[0177]** The systems and methods of the present invention may be particularly useful in those lesions whose extent is not readily diagnosed, such as basal cell carcinomas. These lesions may follow nerves into the orbit or into the intracranial area, extensions not evident with traditional imaging modalities to the surgeon undertaking the resection to provide real time information to the resecting surgeon or the surgeon performing a biopsy as to the likely areas of lymph node invasion.
40

[0178] It is also contemplated that the systems can be used in the "head and neck" which refers collectively to those structures of the ear, nose and throat and proximal aerodigestive system as described above, traditionally falling within the province of otorhinolaryngology. The term "head and neck," as used herein, will further include those structures of the neck such as the thyroid, the parathyroid, the parotid and the cervical lymph nodes, and
45 will include also the extracranial portions of the cranial nerves, including but not limited to the facial nerve, this latter nerve being included from its entry into the internal auditory meatus outward. The term "head and neck, as
50

used herein, will also include those structures of the orbit or of the globe, including the oculomotor muscles and nerves, lacrimal glands and adnexal structures. As used herein, the term "head and neck" will further include those intracranial structures in proximity to the aforesaid head and neck structures. These intracranial structures may include, as examples, the pituitary gland, the pineal gland, the nuclei of various cranial nerves, the intracranial extensions of the cranial nerves, the cerebellopontine angle, the arterial circle of Willis and associated vascular structures, the dura, and the meninges.

[0179] In yet other embodiments, the systems can be used in the genitourinary system, such as the urethra, prostate, bladder, cervix, uterus, and anatomies in proximity thereto. As used herein, the term "genitourinary" shall include those structures of the urinary tract, the male genital system and the female genital system. The urinary tract structures include the urethra, the bladder, the ureters, the kidney and related neural, vascular, lymphatic and adnexal structures. The male genital tract includes the prostate, the seminal vesicles, the testicles, the epididymis and related neural, vascular, lymphatic, ductal and adnexal structures. The female genital tract includes the vagina, the cervix, the non-gravid and gravid uterus, the fallopian tubes, the ovaries, the ova, the fertilized egg, the embryo and the fetus. The term "genitourinary" further refers to those pelvic structures that surround or support the abovementioned structures, such as the paraurethral tissues, the urogenital diaphragm or the musculature of the pelvic floor. The devices can be configured for transurethral placement for evaluation and treatment of female urinary incontinence or bleeding and may use high resolution images of the local tissue, e.g., different layers of the paraurethral tissues. It is understood, for example, that a clearly identified disruption in the muscle layers surrounding the urethra may be repaired surgically, but also must be guided by detailed anatomic information about the site of the abnormality. The devices may also be configured for placement in the genitourinary system such as into the ureter or renal pelvis, urinary tract, or transvaginal use in analysis of the vagina and anatomies in proximity thereto. For example, transvaginal or transcervical endouterine placement may be useful in the diagnosis of neoplasia, in the diagnosis and treatment of endometriosis and in the evaluation of infertility or diagnosis, treatment of pelvic disorders resulting in pelvic pain syndromes, evaluation/treatment of cervical and uterine malignancies and to determine their stages, obstetric use such as permitting anatomic evaluation of mother and fetus.

[0180] In another embodiment, the systems can be used for evaluating and/or treating the rectum or colon, typically by the transrectal route that can be inserted through the anus to a level within the rectum, sigmoid or descending colon where the designated anatomy can be visualized. For example, this approach may be used to delineate the anatomy of the prostate gland, and may further guide the biopsy or the extirpation of lesions un-

dertaken transrectally or transurethrally.

[0181] In other embodiments, the systems and methods of the present invention may be used for the evaluation, diagnosis or treatment of a structure in the gastrointestinal system, or for the evaluation, diagnosis or treatment of a region of the gastrointestinal anatomy. As used herein, the term "gastrointestinal" shall include structures of the digestive system including the esophagus, the stomach, the duodenum, jejunum and ileum (small intestine), the appendix and the colon. The term "gastrointestinal anatomy" shall refer to the structures of the gastrointestinal system as well as the surrounding supporting structures such as the mesentery and the enclosing structures such as the peritoneum, the diaphragm and the retroperitoneum. Disorders of the gastrointestinal system are well-known in the medical arts, as are disorders of the gastrointestinal anatomy. In an exemplary embodiment, the intrabody device may be passed into the stomach.

[0182] In other embodiments, the systems and methods of the present invention may be used for the evaluation, diagnosis and treatment of the vascular system. The vascular system is understood to include the blood vessels of the body, both arterial and venous. The vascular system includes both normal and abnormal blood vessels, named and unnamed vessels, and neovascularization. Access to the vascular system takes place using techniques familiar to practitioners of ordinary skill in the art. The present invention may be used in blood vessels of all size and the intrabody devices may be dimensionally adapted to enter smaller caliber vessels, such as those comprising the distal coronary circulation, the intracranial circulation, the circulation of the distal extremities or the distal circulation of the abdominal viscera. According to these systems and methods, furthermore, positioning a device within the vascular system may be useful for evaluating, diagnosing and treating conditions in structures adjacent to or in proximity to the particular vessel within which the device is situated. Such structures are termed "perivascular structures." As an example, a device placed within a coronary artery may provide information about the vessel itself and about the myocardium that is perfused by the vessel or that is adjacent to the vessel. A device thus positioned may be able to guide therapeutic interventions directed to the myocardial tissue, and may also be able to guide endovascular or extravascular manipulations directed to the vessel itself. It will be readily appreciated by those of ordinary skill in the art that a number of other applications exist or may be discovered with no more than routine experimentation using the systems and methods of the present invention within the vascular system.

[0183] It is understood that access to anatomic structures using the systems, devices modified to fit the intended purpose and anatomy, and methods of the present invention may be provided via naturally occurring anatomic orifices or lumens, as indicated in the examples above. It is further understood, however, that access to

anatomic structures using these systems and methods may be additionally provided using temporary or permanent orifices that have been created medically.

[0184] Further, the methods and systems may cooperate with robotic driven systems rather than manual systems.

[0185] The aforesaid embodiments are understood to be exemplary only. Other embodiments wherein devices may be used within body areas such as body canals, cavities, lumens, passageways, actual or potential spaces will be apparent to practitioners of ordinary skill in the relevant arts.

[0186] In the drawings and specification, there have been disclosed embodiments of the invention and, although specific terms are employed, they are used in a generic and descriptive sense only and not for purposes of limitation, the scope of the invention being set forth in the following claims. Thus, the foregoing is illustrative of the present invention and is not to be construed as limiting thereof. Although a few exemplary embodiments of this invention have been described, those skilled in the art will readily appreciate that many modifications are possible in the exemplary embodiments without materially departing from the novel teachings and advantages of this invention. Accordingly, all such modifications are intended to be included within the scope of this invention as defined in the claims. In the claims, means-plus-function clauses, where used, are intended to cover the structures described herein as performing the recited function and not only structural equivalents but also equivalent structures. Therefore, it is to be understood that the foregoing is illustrative of the present invention and is not to be construed as limited to the specific embodiments disclosed, and that modifications to the disclosed embodiments, as well as other embodiments, are intended to be included within the scope of the appended claims. The invention is defined by the following claims, with equivalents of the claims to be included therein.

Claims

1. An MRI-guided cardiac interventional system (10), comprising:

a circuit (60c) configured to: (a) generate near-real-time (RT) MRI images of at least a portion of a heart of a patient using relevant anatomical scan planes associated with a 3-D MRI image space having a coordinate system; (b) identify coordinates in the MRI image space coordinate system associated with the location of at least a distal portion of a flexible intrabody catheter (80) in the 3-D MRI image space using tracking coil data from tracking coils (82) on the distal end portion of the catheter (80); and (c) render interactive near-RT visualizations of at least the distal end portion of the catheter in the 3-D image

space with a three-dimensional physical representation (80R), wherein the catheter is not required to be in any of the relevant anatomical scan planes used to obtain MR data for the near-RT MRI images, and wherein the tracking coils (82) are connected to coaxial cables (81) that are each connected to different channels (IOCh) of an MRI scanner (10S), wherein the circuit directs the MRI scanner to generate a tracking sequence and an imaging sequence, and wherein the tracking sequence is carried out independently of the imaging sequence.

2. The system of Claim 1, wherein the circuit is further configured to provide a window on a display of a catheter-tip/tissue interface associated with the at least one flexible catheter, the window providing near-real-time high-resolution MRI images separate from the visualizations, and wherein the visualizations are provided in an adjacent separate window on the display, and wherein the tracking sequence comprises a plurality of small flip angle excitations with each repetition designed to indicate the X, Y or Z component of the tracking coil co-ordinates in succession.

3. The system of Claim 1 or claim 2, wherein the circuit is further configured to (i) provide a patient planning map with at least one target treatment site identified thereon registered to the 3-D MRI image space, wherein optionally the circuit is in communication with a display with a User Interface that allows a user to select whether to show the at least one target treatment site in the visualizations so that: (i) the at least one treatment site is shown with the near-RT MRI images without a model or with the model faded relative to the at least one treatment site and near-RT MRI images; or (ii) the at least one treatment site is shown with the planning map or other registered patient model and with the near-RT MRI images.

4. The system of any preceding Claim, wherein the flexible catheter has a tip end (80t) with at least two spaced-apart tracking coils (82c) residing a distance rearward of the tip (80t) on the distal end portion (80d) of the catheter, and wherein the circuit (60c) is configured to calculate the position of the tip of the catheter in the 3-D imaging space using the tracking coil signal data from the tracking coils (82c) and generate the physical representation of at least the distal end portion of the catheter in the visualizations based on at least one of the following: (i) known or predictable shape variation of the distal end portion of the flexible catheter; and (ii) the spatial relationship of the tracking coils with respect to each other and/or the tip of the catheter.

5. The system of any preceding Claim, wherein the cir-

- cuit is in communication with and/or integral with the MRI Scanner, and wherein the MRI Scanner substantially continuously interleaves obtaining tracking coil data with image data to generate the interactive visualizations with the physical representations of at least the distal end portion of the at least one catheter, and wherein the tracking sequence dephases signals perpendicular to a read-out direction in order to attenuate unwanted signals from 1) bulk objects and 2) regions sensed by signal-sensitive parts of the flexible catheter so as to leave a sharp peak indicating the position of the tracking coils, and wherein, once a tracking sequence is complete, a spoiler gradient can be used to dephase any transverse signal remaining before the image sequence is executed.
6. The system of any preceding Claim, wherein the circuit (60c) is in communication with at least one display (20) with a User Interface (25), and wherein the User Interface is configured to allow a user to selectively fade and/or turn on and off tissue characterization or electroanatomical data in at least one visualization either or both: (a) on a three-dimensional pre-acquired model of a patient's heart in the visualizations, the model shown in and/or registered to the 3-D imaging space; and/or (b) in the near-RT MR images without the pre-acquired model.
7. The system of any one of Claims 1 to 5, wherein the circuit is in communication with at least one display (20) with a User Interface (25), and wherein the User Interface is configured to allow a user to (i) selectively fade and/or turn on and off tissue characterization data or electroanatomical data in the visualizations and (ii) to show the tissue and/or electroanatomical data only with the near-RT MRI images in the visualizations or with a model and the near-RT MRI images in the visualizations.
8. The system of any preceding Claim, wherein the physical representation is substantially a 3-D replica representation of an actual physical configuration of at least a distal end portion (80d) of the catheter.
9. The system of any preceding Claim, wherein the circuit (60c) is configured to present a 3-D volumetric model (100M) of at least a portion of the patient's heart in the rendered visualizations with the model registered to the 3-D imaging space along with the physical representation (80R) of at least the distal end portion of the at least one catheter in the 3-D imaging space, optionally wherein the circuit is in communication with a display (20) and a User Interface (25), the User Interface being configured to allow a user to alter a displayed visualization to include only a near-RT image of the anatomy, to include the near-RT image of the anatomy and the registered model of the heart, or to include only the registered model of the heart, further optionally wherein the circuit is configured to show the model in the visualizations in one of a plurality of different selectable ways including at least two of: a cutaway, wireframe, translucent, color-coded or opaque configuration, according to user input using the User Interface.
10. The system of any preceding Claim, wherein the circuit is configured to render the visualizations to show a tip location of the catheter with a first three-dimensional shape and to show each tracking coil on the distal end portion with a second different three dimensional shape or shapes and a color, each tracking coil having a respective different color from the other tracking coils, and to render the visualizations and to include a line or spline connecting the tip and the coil shapes.
11. The system of any preceding Claim, wherein the circuit is configured to generate the visualizations with at least two visual reference planes (41, 42) that are oblique or orthogonal to each other, wherein optionally the circuit is in communication with a display (20) having a User Interface (25), and wherein the two planes are transparent and/or translucent with different-color perimeters and can move relative to the model and/or are locked to the model, and wherein the User Interface is configured to allow a user to rotate the model and move the reference planes to change the view of anatomy shown in the visualization.
12. The system of any preceding Claim, wherein the tracking sequence dephases signals perpendicular to a read-out direction in order to attenuate unwanted signals from 1) bulk objects and 2) regions sensed by signal-sensitive parts of the flexible catheter so as to leave a sharp peak indicating the position of the tracking coils, and wherein, once a tracking sequence is complete, a spoiler gradient can be used to dephase any transverse signal remaining before the image sequence is executed.
13. The system of any preceding Claim, wherein the circuit is configured to show a volumetric patient anatomical model (100M) of at least a portion of the heart and at least two orthogonal or oblique intersecting reference planes in the image space in the visualizations, the reference planes intersecting and extending across the patient model and the near-RT MRI images of local tissue, wherein the reference planes align with the anatomical scan planes.
14. The system of any preceding Claim, wherein the circuit is configured to allow a user to manipulate the

visualizations using a User Interface in communication with a display including to: rotate, crop or zoom the model in a respective visualization, and wherein the circuit automatically selects anatomically relevant scan planes to obtain MR image data in response thereto.

15. The system of any preceding Claim, wherein the catheter is a therapeutic catheter including at least one of an injection or ablation catheter with a catheter tip portion (80t), the circuit (60c) being in communication with a display, wherein the display comprises a close-up viewing window (20w₂) to show lesion forming or injection delivery, wherein the circuit automatically electronically directs a MRI Scanner to obtain image slices using scan planes that are based on a known position of the catheter tip portion, and wherein at least some of the images in the close-up viewing window are generated using high-resolution MR image data.

16. The system of any preceding Claim, further comprising a display with a User Interface (UI), wherein the UI (25) is configured to allow a user to select a dimensional offset of about 0-5 mm for an image scan plane that is projected forward a distance relative to the distal end portion and/or tip of the flexible catheter (80) identified using the tracking coil signal data, wherein the circuit calculates a catheter-tissue interface location of the flexible catheter in the MRI three-dimensional image space and uses the calculated interface location and the selected offset to automatically define at least one scan plane used to obtain the near-real-time MR image data, and wherein the calculated catheter/tissue interface is either (a) calculated to be tangent and substantially in line with at least two of the tracking coils, or (b) calculated as a plane in 3-D image space proximate a projected plane defined by at least three points associated with three different ones of the tracking coils (82).

17. The system of any preceding Claim, wherein the flexible catheter (80) is an injection or ablation catheter, and wherein the circuit (60c) calculates a scan plane location for an *en face* view at a catheter-tissue interface location of the catheter in the three-dimensional image space that is projected outwardly along the line of the catheter to be substantially parallel to tissue proximate the catheter-tissue interface, and wherein the calculated scan plane location is used to obtain the near-real-time MR image data during and/or proximate in time to an injection or ablation using the at least one catheter.

18. The system of any preceding Claim, wherein the circuit is in communication with a display (20) with a User Interface, and wherein the User Interface is configured to allow a user to select different pre-ac-

5

10

15

20

25

30

35

40

45

50

55

quired and/or *in situ* generated maps including at least two of the following for presentation of the selected map or data associated therewith on the at least one display, registered to or spatially aligned with the 3-D MRI image space:

- a thermal tissue characterization map;
- an edema tissue characterization map;
- a first delayed enhancement tissue characterization map;
- a second delayed enhancement tissue characterization map taken after the first delayed enhancement tissue characterization map;
- a hypoxic tissue characterization map;
- a vasculature tissue characteristic map;
- a fibrous tissue characteristic map;
- an ischemic tissue characterization map;
- a fluid distribution map;
- a light exposure map; and
- an electroanatomical map.

19. A computer program product for facilitating an MRI-guided interventional therapy in a patient, the computer program product comprising:

a computer-readable non-transitory storage medium having computer-readable program code embodied in the medium, the computer-readable program code comprising:

- computer-readable program code that directs an MRI Scanner to obtain in an interleaved manner (a) tracking signal data from tracking coils associated with an intrabody flexible device and (b) MR image data, both in the same 3-D image space with a coordinate system, wherein the tracking coils (82) are connected to coaxial cables (81) that are each connected to different channels (IOch) of an MRI scanner (10S), wherein the interleaving is carried out using a tracking sequence and an imaging sequence, and wherein the tracking sequence is carried out independently of the imaging sequence;
- computer-readable program code that generates near-real time (RT) MRI image data of at least a portion of target anatomy of a patient using relevant anatomical scan planes;
- computer-readable program code that identifies spatial coordinates associated with a location of at least a distal end portion of at least one flexible intrabody medical device in the 3-D MRI image space using the tracking signal data; and
- computer-readable program code that renders dynamic near-RT visualizations of

the intrabody flexible medical device in the 3-D image space with near-RT MRI images, wherein the device is not required to be in any of the relevant anatomical scan planes used to obtain the near-real time MR image data, and wherein the distal end portion of the device can vary in shape during the MRI-guided procedure.

20. The computer program product of Claim 19, further comprising:

computer-readable program code that calculates a catheter-tissue interface location proximate a tip location of the catheter in the three-dimensional MRI image space, the calculation being configured to mathematically project axially forward a defined distance beyond the tip to define the catheter-tissue interface, wherein the calculation of the catheter/tissue interface is carried out using X, Y, Z coordinates of the locations of the tracking coils in such a way as to place the location of the catheter-tissue interface a distance of about 0-4 mm beyond a calculated location of the tip of one or more of the flexible intrabody catheters, and wherein the calculated catheter/tissue interface is either (a) calculated to be tangent and substantially in line with at least two of the tracking coils, or (b) calculated as a plane in 3-D image space proximate a projected plane defined by at least three points associated with three different ones of the tracking coils (82); and

computer-readable program code that uses the calculated tissue interface location to automatically define at least one scan plane used by the MRI Scanner to obtain the MR image data during and/or proximate in time to delivery of a therapeutic treatment and/or a diagnostic procedure.

21. The computer program product of Claim 20, wherein the computer-readable program code that renders the dynamic visualizations further comprises computer-readable program code that provides a registered pre-acquired volumetric model of a patient's target anatomical structure in the visualizations, and wherein the tracking sequence dephases signals perpendicular to a read-out direction in order to attenuate unwanted signals from 1) bulk objects and 2) regions sensed by signal-sensitive parts of the flexible catheter (80) so as to leave a sharp peak indicating the position of the tracking coils, and wherein, once a tracking sequence is complete, a spoiler gradient can be used to dephase any transverse signal remaining before the image sequence is executed.

22. The computer program product of Claim 21, further

comprising computer-readable program code configured to allow a user to (a) rotate the visualizations and (b) alter a displayed visualization to include only near-RT image data of the target anatomy, to include the near-RT image data of the anatomy and the registered model of the anatomical structure, or to include only the registered model of the anatomical structure, and/or

further comprising computer-readable program code that allows a user to electronically mark or select target lesion sites on the model, and/or further comprising computer-readable program code that allows a user to electronically selectively display one or more tissue maps aligned with and/or registered to the volumetric model or displayed in lieu of the model, wherein the map selections include at least two of the following:

- a thermal tissue characterization map;
- an edema tissue characterization map;
- a delayed enhancement tissue characterization map taken at a first point in time;
- a delayed enhancement tissue characterization map taken at a second point in time after at least some ablation lesions are created in heart tissue;
- a vasculature tissue map;
- a fibrous tissue map;
- a hypoxic tissue characterization map;
- an ischemic tissue characterization map;
- a fluid distribution map;
- a light exposure map; and
- an electroanatomical map.

Patentansprüche

1. Ein MRT-geführtes Herz-Interventionssystem (10), das Folgendes beinhaltet:

einen Schaltkreis (60c), der zu Folgendem konfiguriert ist: (a) Erzeugen von Nah-Echtzeit(RT)-MRT-Bildern von mindestens einem Abschnitt eines Herzens eines Patienten unter Verwendung relevanter anatomischer Scan-Ebenen in Verbindung mit einem 3-D-MRT-Bildraum mit einem Koordinatensystem; (b) Identifizieren von Koordinaten in dem Koordinatensystem des MRT-Bildraums in Verbindung mit der Lage von mindestens einem distalen Abschnitt eines biegsamen im Körperinneren befindlichen Katheters (80) in dem 3-D-MRT-Bildraum unter Verwendung von Nachführungsdaten von Nachführungsspulen (82) am distalen Endabschnitt des Katheters (80); und (c) Rendering von interaktiven Nah-RT-Visualisierungen von mindestens dem distalen Endabschnitt des Katheters in dem 3-D-Bildraum

- mit einer dreidimensionalen physikalischen Darstellung (80R), wobei sich der Katheter nicht in einer der verwendeten relevanten anatomischen Scan-Ebenen befinden muss, die zum Gewinnen der MR-Daten für die Nah-RT-MRT-Bilder verwendet werden, und wobei die Nachführungsspulen (82) mit Koaxialkabeln (81) verbunden sind, die jeweils mit verschiedenen Kanälen (IOch) eines MRT-Scanners (10S) verbunden sind, wobei der Schaltkreis den MRT-Scanner anweist, eine Nachführungssequenz und eine Bildgebungssequenz zu erzeugen, und wobei die Nachführungssequenz unabhängig von der Bildgebungssequenz ausgeführt wird.
2. System gemäß Anspruch 1, wobei der Schaltkreis ferner dazu konfiguriert ist, ein Fenster auf einer Anzeige einer Schnittstelle zwischen Katheterspitze und Gewebe in Verbindung mit dem mindestens einen biegsamen Katheter bereitzustellen, wobei das Fenster Nah-Echtzeit-MRT-Bilder mit hoher Auflösung bereitstellt, die separat von den Visualisierungen sind, und wobei die Visualisierungen in einem benachbarten separaten Fenster auf der Anzeige bereitgestellt werden, und wobei die Nachführungssequenz eine Vielzahl von kleinen Kippwinkelanregungen beinhaltet, wobei jede Wiederholung dazu ausgelegt ist, die X-, Y- oder Z-Komponente der Nachführungsspulenkoordinaten nacheinander anzuzeigen.
 3. System gemäß Anspruch 1 oder Anspruch 2, wobei der Schaltkreis ferner zu Folgendem konfiguriert ist: (i) Bereitstellen einer Patientenplanungskarte mit mindestens einem darauf identifizierten Zielbehandlungsort, die zu dem 3-D-MRT-Bildraum registriert ist, wobei der Schaltkreis optional in Kommunikation mit einer Anzeige mit einer Benutzerschnittstelle steht, die es einem Benutzer gestattet auszuwählen, ob der mindestens eine Zielbehandlungsort in den Visualisierungen gezeigt werden soll, so dass: (i) der mindestens eine Behandlungsort mit den Nah-RT-MR-Bildern ohne ein Modell gezeigt wird oder mit dem im Verhältnis zu dem mindestens einen Behandlungsort und den Nah-RT-MR-Bildern ausgeblendeten Modell gezeigt wird; oder (ii) der mindestens eine Behandlungsort mit der Planungskarte oder einem anderen registrierten Patientenmodell und mit den Nah-RT-MR-Bildern gezeigt wird.
 4. System gemäß einem der vorhergehenden Ansprüche, wobei der biegsame Katheter ein Spitzenende (80t) mit mindestens zwei beabstandeten Nachführungsspulen (82c) aufweist, die sich rückwärts von der Spitze (80t) in einem Abstand am distalen Endabschnitt (80d) des Katheters befinden, und wobei der Schaltkreis (60c) dazu konfiguriert ist, die Position der Spitze des Katheters in dem 3-D-Bildgebungsraum unter Verwendung der Nachführungsspulen-Signaldaten von den Nachführungsspulen (82c) zu berechnen und die physikalische Darstellung von mindestens dem distalen Endabschnitt des Katheters in den Visualisierungen zu erzeugen, basierend auf mindestens einem der Folgenden: (i) der bekannten oder vorhersagbaren Variation der Gestalt des distalen Endabschnitts des biegsamen Katheters; und (ii) der räumlichen Beziehung der Nachführungsspulen zueinander und/oder zu der Spitze des Katheters.
 5. System gemäß einem der vorhergehenden Ansprüche, wobei der Schaltkreis in Kommunikation mit dem MRT-Scanner steht und/oder ein Teil davon ist und wobei der MRT-Scanner im Wesentlichen kontinuierlich das Gewinnen von Nachführungsspulendaten mit Bilddaten zum Erzeugen der interaktiven Visualisierungen mit den physikalischen Darstellungen von mindestens dem distalen Endabschnitt des mindestens einen Katheters verschachtelt, und wobei die Nachführungssequenz Signale, die im rechten Winkel zu einer Leserichtung stehen, aus der Phase bringt, um unerwünschte Signale von 1) Massenobjekten und 2) Regionen, die von signalempfindlichen Teilen des biegsamen Katheters abgetastet werden, abzuschwächen, damit ein scharfer Peak bleibt, der die Position der Nachführungsspulen anzeigt, und wobei, nachdem eine Nachführungssequenz abgeschlossen worden ist, ein Spoilergradient verwendet werden kann, um alle verbleibenden transversalen Signale aus der Phase zu bringen, bevor die Bildsequenz ausgeführt wird.
 6. System gemäß einem der vorhergehenden Ansprüche, wobei der Schaltkreis (60c) in Kommunikation mit mindestens einer Anzeige (20) mit einer Benutzerschnittstelle (25) steht und wobei die Benutzerschnittstelle so konfiguriert ist, dass sie es einem Benutzer gestattet, die Gewebecharakterisierungs- oder elektroanatomischen Daten in mindestens einer Visualisierung von den Folgenden oder in beiden davon selektiv auszublenden und/oder ein- und auszuschalten: (a) an einem dreidimensionalen zuvor akquirierten Modell eines Herzens eines Patienten in den Visualisierungen, dem in dem 3-D-Bildgebungsraum gezeigten und/oder zu diesem registrierten Modell; und/oder (b) in den Nah-RT-MR-Bildern ohne das zuvor akquirierte Modell.
 7. System gemäß einem der Ansprüche 1 bis 5, wobei der Schaltkreis in Kommunikation mit mindestens einer Anzeige (20) mit einer Benutzerschnittstelle (25) steht und wobei die Benutzerschnittstelle so konfiguriert ist, dass sie es einem Benutzer gestattet, (i) die Gewebecharakterisierungsdaten oder elektroa-

anatomischen Daten in den Visualisierungen selektiv auszublenden und/oder ein- und auszuschalten und (ii) die Gewebe- und/oder elektroanatomischen Daten nur mit dem Nah-RT-MR-Bildern in den Visualisierungen zu zeigen oder mit einem Modell und den Nah-RT-MR-Bildern in den Visualisierungen zu zeigen.

8. System gemäß einem der vorhergehenden Ansprüche, wobei die physikalische Darstellung im Wesentlichen eine 3-D-Nachbildungsdarstellung einer tatsächlichen physikalischen Konfiguration von mindestens einem distalen Endabschnitt (80d) des Katheters ist.
9. System gemäß einem der vorhergehenden Ansprüche, wobei der Schaltkreis (60c) dazu konfiguriert ist, ein volumetrisches 3-D-Modell (100M) von mindestens einem Abschnitt des Herzens des Patienten in den gerenderten Visualisierungen mit dem zu dem 3-D-Bildgebungsraum registrierten Modell zusammen mit der physikalischen Darstellung (80R) von mindestens dem distalen Endabschnitt des mindestens einen Katheters in dem 3-D-Bildgebungsraum darzustellen, wobei der Schaltkreis optional in Kommunikation mit einer Anzeige (20) und einer Benutzerschnittstelle (25) steht, wobei die Benutzerschnittstelle dazu konfiguriert ist, es einem Benutzer zu gestatten, eine angezeigte Visualisierung so zu verändern, dass sie nur ein Nah-RT-Bild der Anatomie einschließt, dass sie das Nah-RT-Bild der Anatomie und das registrierte Modell des Herzens einschließt oder dass sie nur das registrierte Modell des Herzens einschließt, wobei der Schaltkreis ferner optional dazu konfiguriert ist, das Modell in den Visualisierungen in einer von einer Vielzahl verschiedener auswählbarer Arten zu zeigen, u. a. mindestens zwei der Folgenden: einer Schnittmodell-, Drahtmodell-, durchscheinenden, farbkodierten oder opaken Konfiguration, je nach der Eingabe des Benutzers unter Verwendung der Benutzerschnittstelle.
10. System gemäß einem der vorhergehenden Ansprüche, wobei der Schaltkreis dazu konfiguriert ist, die Visualisierungen zu rendern, um eine Spitzenlage des Katheters mit einer ersten dreidimensionalen Gestalt zu zeigen und jede Nachführungsspule am distalen Endabschnitt mit einer zweiten verschiedenen dreidimensionalen Gestalt oder Gestalten und einer Farbe zu zeigen, wobei jede Nachführungsspule eine jeweils von den anderen Nachführungsspulen verschiedene Farbe aufweist, und die Visualisierungen zu rendern und eine Linie oder Spline, welche die Spitze und die Spulengestalten verbindet, einzuschließen.
11. System gemäß einem der vorhergehenden Ansprüche,

che, wobei der Schaltkreis dazu konfiguriert ist, die Visualisierungen mit mindestens zwei visuellen Bezugsebenen (41, 42), die schief oder orthogonal zueinander liegen, zu erzeugen,

5 wobei der Schaltkreis optional in Kommunikation mit einer Anzeige (20) mit einer Benutzerschnittstelle (25) steht und wobei die zwei Ebenen transparent und/oder durchscheinend mit in verschiedenen Farben erscheinenden Begrenzungslinien sind und sich im Verhältnis zu dem Modell bewegen können und/oder am Modell arretiert sind, und wobei die Benutzerschnittstelle dazu konfiguriert ist, es einem Benutzer zu gestatten, das Modell zu rotieren und die Bezugsebenen zu bewegen, um die in der Visualisierung gezeigte Ansicht der Anatomie zu ändern.

12. System gemäß einem der vorhergehenden Ansprüche, wobei die Nachführungssequenz Signale, die im rechten Winkel zu einer Leserichtung stehen, aus der Phase bringt, um unerwünschte Signale von 1) Massenobjekten und 2) Regionen, die von signalempfindlichen Teilen des biegsamen Katheters abgetastet werden, abzuschwächen, damit ein scharfer Peak bleibt, der die Position der Nachführungsspulen anzeigt, und wobei, nachdem eine Nachführungssequenz abgeschlossen worden ist, ein Spoilergradient verwendet werden kann, um alle verbleibenden transversalen Signale aus der Phase zu bringen, bevor die Bildsequenz ausgeführt wird.

13. System gemäß einem der vorhergehenden Ansprüche, wobei der Schaltkreis dazu konfiguriert ist, ein volumetrisches anatomisches Patientenmodell (100M) von mindestens einem Abschnitt des Herzens und mindestens zwei orthogonale oder schiefe, sich überschneidende Bezugsebenen in dem Bildraum in den Visualisierungen zu zeigen, wobei die Bezugsebenen sich überschneiden und sich über das Patientenmodell und die Nah-RT-MR-Bilder des lokalen Gewebes erstrecken, wobei die Bezugsebenen mit den anatomischen Scan-Ebenen ausgerichtet sind.

14. System gemäß einem der vorhergehenden Ansprüche, wobei der Schaltkreis dazu konfiguriert ist, es einem Benutzer zu gestatten, die Visualisierungen unter Verwendung einer Benutzerschnittstelle, die in Kommunikation mit einer Anzeige steht, zu manipulieren, u. a. zum: Rotieren, Abschneiden oder Zoomen des Modells in einer jeweiligen Visualisierung, und wobei der Schaltkreis automatisch anatomisch relevante Scan-Ebenen auswählt, um die MR-Bildern als Reaktion darauf zu erhalten.

15. System gemäß einem der vorhergehenden Ansprüche, wobei der Katheter ein therapeutischer Katheter ist, der mindestens einen von einem Injektions- oder Ablationskatheter mit einem Katheterspitzen-

abschnitt (80t) einschließt, wobei der Schaltkreis (60c) in Kommunikation mit einer Anzeige steht, wobei die Anzeige ein Nahaufnahme-Sichtfenster (20w₂) beinhaltet, um die Läsionsbildung oder das Zuführen der Injektion zu zeigen, wobei der Schaltkreis automatisch einen MRT-Scanner elektronisch anweist, Schichtbilder unter Verwendung von Scan-Ebenen, die auf einer bekannten Position des Katheterspitzenabschnitts basieren, zu erhalten, und wobei mindestens einige der Bilder in dem Nahaufnahme-Sichtfenster unter Verwendung von MR-Bilddaten mit hoher Auflösung erzeugt werden.

16. System gemäß einem der vorhergehenden Ansprüche, das ferner eine Anzeige mit einer Benutzerschnittstelle (UI) beinhaltet, wobei die UI (25) dazu konfiguriert ist, es einem Benutzer zu gestatten, eine Dimensionsverschiebung von etwa 0 bis 5 mm für eine Bildscan-Ebene auszuwählen, die über eine Entfernung im Verhältnis zu dem distalen Endabschnitt und/oder der Spitze des biegsamen Katheters (80) nach vorne projiziert wird, die unter Verwendung der Nachführungsspulen-Signaldaten identifiziert wurde, wobei der Schaltkreis eine Lage der Schnittstelle zwischen der Katheter-Gewebe-Schnittstellen-Lage des biegsamen Katheters in dem dreidimensionalen MRT-Bildraum berechnet und die berechnete Schnittstellenlage und die ausgewählte Verschiebung dazu verwendet, automatisch mindestens eine Scan-Ebene zu definieren, die zum Gewinnen der Nah-Echtzeit-MR-Bilddaten verwendet wird, und wobei die berechnete Katheter-Gewebe-Schnittstelle entweder (a) als eine Tangente und als im Wesentlichen in einer Linie mit mindestens zwei der Nachführungsspulen liegend berechnet wird oder (b) als eine Ebene in dem 3-D-Bildraum in der Nähe einer projizierten Ebene berechnet wird, die durch mindestens drei Punkte in Verbindung mit drei verschiedenen der Nachführungsspulen (82) definiert wird.

17. System gemäß einem der vorhergehenden Ansprüche, wobei der biegsame Katheter (80) ein Injektions- oder Ablationskatheter ist und wobei der Schaltkreis (60c) eine Lage der Scan-Ebene für eine Enface-Ansicht an einer Katheter-Gewebe-Schnittstellen-Lage des Katheters in dem dreidimensionalen Bildraum berechnet, die entlang der Linie des Katheters nach außen projiziert wird, so dass sie im Wesentlichen parallel zu dem Gewebe in der Nähe der Katheter-Gewebe-Schnittstelle ist, und wobei die berechnete Lage der Scan-Ebene zum Gewinnen der Nah-Echtzeit-MR-Bilddaten während und/oder in unmittelbarer zeitlicher Nähe einer Injektion oder Ablation unter Verwendung des mindestens einen Katheters verwendet wird.

18. System gemäß einem der vorhergehenden Ansprüche,

wobei der Schaltkreis in Kommunikation mit einer Anzeige (20) mit einer Benutzerschnittstelle steht und wobei die Benutzerschnittstelle dazu konfiguriert ist, es einem Benutzer zu gestatten, verschiedene zuvor akquirierte und/oder in situ erzeugte Karten auszuwählen, die mindestens zwei der Folgenden einschließen, zur Darstellung der gewählten Karte oder damit in Verbindung stehenden Daten auf der mindestens einen Anzeige, die zu dem 3-D-MRT-Bildraum registriert sind oder räumlich mit diesem ausgerichtet sind:

eine Thermal-Gewebecharakterisierungskarte;
 eine Ödem-Gewebecharakterisierungskarte;
 eine erste verzögerte Verstärkungs-Gewebecharakterisierungskarte;
 eine zweite verzögerte Verstärkungs-Gewebecharakterisierungskarte, aufgenommen nach der ersten verzögerten Verstärkungs-Gewebecharakterisierungskarte;
 eine hypoxische Gewebecharakterisierungskarte;
 eine Gefäßsystemgewebecharakteristikakarte;
 eine Fasergewebecharakteristikakarte;
 eine ischämische Gewebecharakterisierungskarte;
 eine Fluidverteilungskarte;
 eine Belichtungskarte; und
 eine elektroanatomische Karte.

19. Ein Computerprogrammprodukt zum Erleichtern einer MRT-geführten Interventionstherapie bei einem Patienten, wobei das Computerprogrammprodukt Folgendes beinhaltet:

ein nichtflüchtiges computerlesbares Speichermedium mit computerlesbarem Programmcode, der in dem Medium verkörpert ist, wobei der computerlesbare Programmcode Folgendes beinhaltet:

computerlesbaren Programmcode, der einen MRT-Scanner anweist, Folgendes in einer verschachtelten Weise zu gewinnen: (a) Nachführungssignaldaten von Nachführungsspulen in Verbindung mit einer im Körperinnern befindlichen biegsamen Vorrichtung und (b) MR-Bilddaten, beide in dem gleichen 3-D-Bildraum mit einem Koordinatensystem, wobei die Nachführungsspulen (82) mit Koaxialkabeln (81) verbunden sind, die jeweils mit verschiedenen Kanälen (IOch) eines MRT-Scanners (10S) verbunden sind, wobei die Verschachtelung unter Verwendung einer Nachführungssequenz und einer Bildgebungssequenz ausgeführt wird und wobei die Nachführungssequenz unabhängig von der Bildgebungssequenz

ausgeführt wird;
 computerlesbaren Programmcode, der Nah-Echtzeit(RT)-MRT-Bilddaten von mindestens einem Abschnitt der Zielanatomie eines Patienten unter Verwendung relevanter anatomischer Scan-Ebenen erzeugt;
 computerlesbaren Programmcode, der räumliche Koordinaten in Verbindung mit einer Lage von mindestens einem distalen Endabschnitt von mindestens einer im Körperinnern befindlichen biegsamen medizinischen Vorrichtung in dem 3-D-MRT-Bildraum unter Verwendung der Nachführungssignalen identifiziert; und
 computerlesbaren Programmcode, der dynamische Nah-RT-Visualisierungen der im Körperinnern befindlichen biegsamen medizinischen Vorrichtung in dem 3-D-Bildraum mit Nah-RT-MR-Bildern rendert, wobei die Vorrichtung nicht in einer der verwendeten relevanten anatomischen Scan-Ebenen sein muss, die zum Gewinnen der Nah-Echtzeit-MR-Bilddaten verwendet werden, und wobei der distale Endabschnitt der Vorrichtung während des MRT-geführten Verfahrens in seiner Gestalt variieren kann.

20. Computerprogrammprodukt gemäß Anspruch 19, das ferner Folgendes beinhaltet:

computerlesbaren Programmcode, der eine Katheter-Gewebe-Schnittstellen-Lage in der Nähe einer Spitzenlage des Katheters in dem dreidimensionalen MRT-Bildraum berechnet, wobei die Berechnung zum mathematischen Projizieren eines definierten Abstands axial nach vorne über die Spitze hinaus ausgeführt wird, um die Schnittstelle zwischen Katheter und Gewebe zu definieren, wobei die Berechnung der Schnittstelle zwischen Katheter und Gewebe unter Verwendung der X-, Y-, Z-Koordinaten der Lagen der Nachführungsspulen ausgeführt wird, und zwar auf eine solche Weise, dass die Lage der Schnittstelle zwischen Katheter und Gewebe in einem Abstand von etwa 0 bis 4 mm über eine berechnete Lage der Spitze hinaus von einem oder mehreren biegsamen im Körperinnern befindlichen Kathetern platziert wird, und wobei die berechnete Katheter-Gewebe-Schnittstelle entweder (a) als eine Tangente und als im Wesentlichen in einer Linie mit mindestens zwei der Nachführungsspulen liegend berechnet wird oder (b) als eine Ebene in dem 3-D-Bildraum in der Nähe einer projizierten Ebene berechnet wird, die durch mindestens drei Punkte in Verbindung mit drei verschiedenen der Nachführungsspulen (82) definiert wird; und

computerlesbaren Programmcode, der die berechnete Gewebeschnittstellenlage verwendet, um automatisch mindestens eine Scan-Ebene zu definieren, die von dem MRT-Scanner zum Gewinnen der MR-Bilddaten während der und/oder in unmittelbarer zeitlicher Nähe der Zuführung einer therapeutischen Behandlung und/oder eines diagnostischen Verfahrens verwendet wird.

21. Computerprogrammprodukt gemäß Anspruch 20, wobei der computerlesbare Programmcode, der die dynamischen Visualisierungen rendert, ferner computerlesbaren Programmcode beinhaltet, der ein registriertes zuvor akquiriertes volumetrisches Modell einer anatomischen Zielstruktur eines Patienten in den Visualisierungen bereitstellt, und wobei die Nachführungssequenz Signale, die im rechten Winkel zu einer Leserichtung stehen, aus der Phase bringt, um unerwünschte Signale von 1) Massenobjekten und 2) Regionen, die von signalempfindlichen Teilen des biegsamen Katheters (80) abgetastet werden, abzuschwächen, damit ein scharfer Peak bleibt, der die Position der Nachführungsspulen anzeigt, und wobei, nachdem eine Nachführungssequenz abgeschlossen worden ist, ein Spoilergradient verwendet werden kann, um alle verbleibenden transversalen Signale aus der Phase zu bringen, bevor die Bildsequenz ausgeführt wird.

22. Computerprogrammprodukt gemäß Anspruch 21, das ferner computerlesbaren Programmcode beinhaltet, der dazu konfiguriert ist, es einem Benutzer zu gestatten, (a) die Visualisierungen zu drehen und (b) eine angezeigte Visualisierung so zu verändern, dass sie nur Nah-RT-Bilddaten der Zielanatomie einschließt, dass sie die Nah-RT-Bilddaten der Anatomie und das registrierte Modell der anatomischen Struktur einschließt oder dass sie nur das registrierte Modell der anatomischen Struktur einschließt, und/oder

das ferner computerlesbaren Programmcode beinhaltet, der es einem Benutzer gestattet, Zielläsionsorte auf dem Modell elektronisch zu markieren oder auszuwählen, und/oder das ferner computerlesbaren Programmcode beinhaltet, der es einem Benutzer gestattet, eine oder mehrere Gewebekarten elektronisch selektiv anzuzeigen, die mit dem volumetrischen Modell ausgerichtet und/oder zu diesem registriert sind oder anstatt des Modells angezeigt werden, wobei die Kartenauswahl mindestens zwei der Folgenden einschließen:

- eine Thermal-Gewebecharakterisierungskarte;
- eine Ödem-Gewebecharakterisierungskarte;

te;
 eine zu einem ersten Zeitpunkt aufgenommene verzögerte Verstärkungs-Gewebecharakterisierungskarte;
 eine verzögerte Verstärkungs-Gewebecharakterisierungskarte, die zu einem zweiten Zeitpunkt, nachdem mindestens einige Ablationsläsionen in dem Herzgewebe vorgenommen worden sind, aufgenommen wird;
 eine Gefäßsystemgewebekarte;
 eine Fasergewebekarte;
 eine hypoxische Gewebecharakterisierungskarte;
 eine ischämische Gewebecharakterisierungskarte;
 eine Fluidverteilungskarte;
 eine Belichtungskarte; und
 eine elektroanatomische Karte.

Revendications

1. Système interventionnel cardiaque guidé par IRM (10), comprenant :

un circuit (60c) configuré pour : (a) générer des images IRM quasi en temps réel (RT) d'au moins une partie d'un coeur d'un patient à l'aide de plans de balayage anatomiques d'intérêt associés à un espace d'image IRM en 3D ayant un système coordonné ; (b) identifier des coordonnées dans le système coordonné d'espace d'image IRM associées à l'emplacement d'au moins une partie distale d'un cathéter intracorporel souple (80) dans l'espace d'image IRM en 3D à l'aide de données de bobines d'alignement issues de bobines d'alignement (82) sur la partie d'extrémité distale du cathéter (80) ; et (c) rendre des visualisations quasi en RT interactives d'au moins la partie d'extrémité distale du cathéter dans l'espace d'image en 3D avec une représentation physique tridimensionnelle (80R), le cathéter ne se trouvant pas nécessairement dans un plan de balayage anatomique d'intérêt utilisé pour obtenir des données IRM pour les images IRM quasi en RT, et les bobines d'alignement (82) étant connectées à des câbles coaxiaux (81) qui sont individuellement connectés à différents canaux (IOch) d'un appareil IRM (10S), le circuit dirigeant l'appareil IRM pour générer une séquence d'alignement et une séquence d'imagerie, et la séquence d'alignement étant réalisée indépendamment de la séquence d'imagerie.

2. Système de la revendication 1, dans lequel le circuit est en outre configuré pour fournir une fenêtre sur

un écran d'une interface pointe de cathéter/tissu associée à l'au moins un cathéter souple, la fenêtre fournissant des images IRM haute résolution quasi en temps réel séparées des visualisations, et les visualisations étant fournies dans une fenêtre séparée adjacente sur l'écran, et la séquence d'alignement comprenant une pluralité d'excitations à faible angle de bascule, chaque répétition étant conçue pour indiquer successivement la composante X, Y ou Z des coordonnées de bobines d'alignement.

3. Système de la revendication 1 ou de la revendication 2, dans lequel le circuit est en outre configuré pour (i) fournir une carte de planification de patient avec au moins un site de traitement cible identifié sur celle-ci et enregistré sur l'espace d'image en 3D, le circuit étant éventuellement en communication avec un écran avec une interface utilisateur qui permet à un utilisateur de choisir d'afficher ou non l'au moins un site de traitement cible dans les visualisations de sorte que : (i) l'au moins un site de traitement soit affiché avec les images IRM quasi en RT sans modèle ou avec le modèle estompé par rapport à l'au moins un site de traitement et aux images IRM quasi en RT ; ou (ii) que l'au moins un site de traitement soit affiché avec la carte de planification ou un autre modèle de patient enregistré et avec les images IRM quasi en RT.

4. Système de l'une quelconque des revendications précédentes, dans lequel le cathéter souple possède une extrémité en pointe (80t) avec au moins deux bobines d'alignement (82c) espacées disposées à une certaine distance en arrière de la pointe (80t) sur la partie d'extrémité distale (80d) du cathéter, et dans lequel le circuit (60c) est configuré pour calculer la position de la pointe du cathéter dans l'espace d'imagerie en 3D à l'aide des données de signal de bobines d'alignement issues des bobines d'alignement (82c) et générer la représentation physique d'au moins la partie d'extrémité distale du cathéter dans les visualisations sur la base d'au moins un des éléments suivants : (i) une variation de forme connue ou prévisible de la partie d'extrémité distale du cathéter souple ; et (ii) la relation spatiale des bobines d'alignement entre elles et/ou avec la pointe du cathéter.

5. Système de l'une quelconque des revendications précédentes, dans lequel le circuit est en communication avec l'appareil IRM et/ou solidaire de celui-ci, et dans lequel l'appareil IRM intercale sensiblement en continu l'obtention de données de bobines d'alignement avec des données d'image pour générer les visualisations interactives avec les représentations physiques d'au moins la partie d'extrémité distale de l'au moins un cathéter, et dans lequel la séquence d'alignement déphase des signaux perpen-

- diculaires à une direction de lecture afin d'atténuer des signaux non souhaités provenant 1) de masses et 2) de régions détectées par des parties sensibles aux signaux du cathéter souple de façon à laisser un pic aigu indiquant la position des bobines d'alignement, et dans lequel, une fois la séquence d'alignement effectuée, une impulsion de gradient peut être utilisée pour déphaser tout signal transversal résiduel avant l'exécution de la séquence d'image.
- 5
6. Système de l'une quelconque des revendications précédentes, dans lequel le circuit (60c) est en communication avec au moins un écran (20) avec une interface d'utilisateur (25), et dans lequel l'interface d'utilisateur est configurée pour permettre à un utilisateur d'estomper et/ou de mettre en marche et à l'arrêt, sélectivement, des données de caractérisation de tissu ou des données électro-anatomiques dans au moins une visualisation dans l'un ou l'autre ou l'ensemble des éléments suivants : (a) sur un modèle tridimensionnel acquis au préalable d'un coeur d'un patient dans les visualisations, le modèle étant présenté dans l'espace d'imagerie en 3D et/ou enregistré dans celui-ci ; et/ou (b) dans les images IRM quasi en RT sans modèle acquis au préalable.
- 10
7. Système de l'une quelconque des revendications 1 à 5, dans lequel le circuit est en communication avec au moins un écran (20) avec une interface d'utilisateur (25), et dans lequel l'interface d'utilisateur est configurée pour permettre à un utilisateur de (i) sélectivement estomper et/ou mettre en marche ou à l'arrêt des données de caractérisation de tissu ou des données électro-anatomiques dans les visualisations et (ii) présenter les données de tissu et/ou électro-anatomiques uniquement avec les images IRM quasi en RT dans les visualisations ou avec un modèle dans les images IRM quasi en RT dans les visualisations.
- 15
8. Système de l'une quelconque des revendications précédentes, dans lequel la représentation physique est sensiblement une représentation répliquée en 3D d'une configuration physique effective d'au moins une partie d'extrémité distale (80d) du cathéter.
- 20
9. Système de l'une quelconque des revendications précédentes, dans lequel le circuit (60c) est configuré pour présenter un modèle volumétrique en 3D (100M) d'au moins une partie du coeur du patient dans les visualisations rendues avec le modèle enregistré dans l'espace d'imagerie en 3D ainsi que la représentation physique (80R) d'au moins la partie d'extrémité distale de l'au moins un cathéter dans l'espace d'imagerie en 3D, dans lequel éventuellement le circuit est en communication avec un écran (20) et une interface d'utilisateur (25), l'interface d'utilisateur étant configurée pour permettre à un utilisateur de modifier une visualisation affichée pour inclure uniquement une image quasi en RT de l'anatomie, pour inclure l'image quasi en RT de l'anatomie et le modèle enregistré du coeur, ou pour inclure uniquement le modèle enregistré du coeur, dans lequel en outre, éventuellement, le circuit est configuré pour présenter le modèle dans les visualisations de l'une d'une pluralité de manières différentes sélectionnables, parmi lesquelles au moins deux des suivantes : une vue en transparence, une représentation filaire, une vue translucide, une configuration à code couleur ou opaque, selon l'entrée d'utilisateur à l'aide de l'interface d'utilisateur.
- 25
10. Système de l'une quelconque des revendications précédentes, dans lequel le circuit est configuré pour rendre les visualisations afin de présenter un emplacement de pointe du cathéter avec une première forme tridimensionnelle et de présenter chaque bobine d'alignement sur la partie d'extrémité distale avec au moins une deuxième forme tridimensionnelle différente et une couleur différente, chaque bobine d'alignement ayant une couleur respective différente des autres bobines d'alignement, et pour rendre les visualisations et inclure une ligne ou un spline reliant les formes de pointe et de bobines d'alignement.
- 30
11. Système de l'une quelconque des revendications précédentes, dans lequel le circuit est configuré pour générer les visualisations avec au moins deux plans de référence visuels (41, 42) qui sont obliques ou orthogonaux l'un par rapport à l'autre, dans lequel éventuellement le circuit est en communication avec un écran (20) ayant une interface d'utilisateur (25), et dans lequel les deux plans sont transparents et/ou translucides avec des périmètres de couleurs différentes et peuvent se déplacer par rapport au modèle et/ou sont figés sur le modèle, et dans lequel l'interface d'utilisateur est configurée pour permettre à un utilisateur d'effectuer une rotation du modèle et de déplacer les plans de référence pour modifier la vue de l'anatomie présentée dans la visualisation.
- 35
12. Système de l'une quelconque des revendications précédentes, dans lequel la séquence d'alignement déphase les signaux perpendiculaires à une direction de lecture afin d'atténuer des signaux non souhaités provenant 1) de masses et 2) de régions détectées par des parties sensibles aux signaux du cathéter souple de façon à laisser un pic aigu indiquant la position des bobines d'alignement, et dans lequel, une fois la séquence d'alignement effectuée, une impulsion de gradient peut être utilisée pour déphaser tout signal transversal résiduel avant l'exécution de la séquence d'image.
- 40
- 45
- 50
- 55

13. Système de l'une quelconque des revendications précédentes, dans lequel le circuit est configuré pour présenter un modèle anatomique de patient volumétrique (100M) d'au moins une partie du coeur et au moins deux plans de référence en intersection orthogonale ou oblique dans l'espace d'image dans les visualisations, les plans de référence se croisant et s'étendant à travers le modèle de patient et les images IRM quasi en RT de tissu local, les plans de référence étant alignés avec les plans de balayage anatomiques.
14. Système de l'une quelconque des revendications précédentes, dans lequel le circuit est configuré pour permettre à un utilisateur de manipuler les visualisations à l'aide d'une interface d'utilisateur en communication avec un écran, notamment de : faire tourner, découper ou agrandir le modèle dans une visualisation respective, et dans lequel le circuit sélectionne automatiquement les plans de balayage anatomiques d'intérêt pour obtenir des données d'image IRM en réponse à celles-ci.
15. Système de l'une quelconque des revendications précédentes, dans lequel le cathéter est un cathéter thérapeutique comprenant au moins l'un cathéter d'injection ou d'un cathéter d'ablation avec une partie en pointe de cathéter (80t), le circuit (60c) étant en communication avec un écran, l'écran comprenant une fenêtre de visualisation en gros plan (20w₂) pour montrer la formation de lésion ou l'administration d'injection, le circuit dirigeant électroniquement automatiquement un appareil IRM pour obtenir des coupes en image à l'aide de plans de balayage qui sont basés sur une position connue de la partie en pointe de cathéter, et au moins certaines des images dans la fenêtre de visualisation en gros plan étant générées à l'aide de données d'image IRM haute résolution.
16. Système de l'une quelconque des revendications précédentes, comprenant en outre un écran avec une interface d'utilisateur (UI), l'UI (25) étant configurée pour permettre à un utilisateur de choisir un décalage dimensionnel d'environ 0 à 5 mm pour un plan de balayage d'image qui est projeté vers l'avant à une certaine distance par rapport à la partie d'extrémité distale et/ou la pointe du cathéter souple (80) identifiée à l'aide des données de signal de bobines d'alignement, le circuit calculant un emplacement d'interface cathéter-tissu du cathéter souple dans l'espace d'image tridimensionnelle IRM et utilisant l'emplacement d'interface calculé et le décalage choisi pour définir automatiquement au moins un plan de balayage utilisé pour obtenir les données d'image IRM quasi en temps réel, et l'interface cathéter/tissu calculée étant soit (a) calculée pour être tangente et sensiblement en alignement avec au moins deux des bobines d'alignement, soit (b) calculée sous la forme d'un plan dans l'espace d'image en 3D à proximité d'un plan projeté défini par au moins trois points associés à trois bobines différentes des bobines d'alignement (82).
17. Système de l'une quelconque des revendications précédentes, dans lequel le cathéter souple (80) est un cathéter d'injection ou d'ablation, et dans lequel le circuit (60c) calcule un emplacement de plan de balayage pour une vue de face au niveau d'un emplacement d'interface cathéter-tissu du cathéter dans l'espace d'image tridimensionnelle qui est projeté vers l'extérieur le long de la ligne du cathéter pour être sensiblement parallèle au tissu à proximité de l'interface cathéter-tissu, et dans lequel l'emplacement de plan de balayage calculé est utilisé pour obtenir les données d'image IRM quasi en temps réel au cours et/ou à un moment proche d'une injection ou d'une ablation à l'aide de l'au moins cathéter.
18. Système de l'une quelconque des revendications précédentes, dans lequel le circuit est en communication avec un écran (20) avec une interface d'utilisateur, et dans lequel l'interface d'utilisateur est configurée pour permettre à un utilisateur de choisir des cartes acquises au préalable et/ou générées *in situ* différentes comprenant au moins deux des éléments suivants pour une présentation de la carte choisie ou de données associées à celle-ci sur l'au moins un écran, enregistrées dans l'espace d'image IRM en 3D ou spatialement alignées avec celui-ci :
- une carte de caractérisation de tissu thermique ;
 - une carte de caractérisation de tissu d'oedème ;
 - une première carte de caractérisation de tissu à renforcement retardé ;
 - une deuxième carte de caractérisation de tissu à renforcement retardé prise après la première carte de caractérisation de tissu à renforcement retardé ;
 - une carte de caractérisation de tissu hypoxique ;
 - une carte de caractéristique de tissu vasculaire ;
 - une carte caractéristique de tissu fibreux ;
 - une carte de caractérisation de tissu ischémique ;
 - une carte de distribution de fluide ;
 - une carte d'exposition à la lumière ; et
 - une carte électro-anatomique.
19. Produit de programme informatique destiné à faciliter une thérapie interventionnelle guidée par IRM chez un patient, le produit de programme informatique comprenant :
- un support de stockage non transitoire lisible par ordinateur dans lequel est intégré un code de programme lisible par ordinateur, le code de pro-

gramme lisible par ordinateur comprenant :

un code de programme lisible par ordinateur qui dirige un appareil IRM pour obtenir de manière intercalée (a) des données de signal d'alignement issues de bobines d'alignement associées à un dispositif intracorporel souple, et (b) des données d'image IRM, toutes dans le même espace d'image en 3D avec un système coordonné, les bobines d'alignement (82) étant connectées à des câbles coaxiaux (81) qui sont individuellement connectés à différents canaux (IOch) d'un appareil IRM (10S), l'intercalage étant réalisé à l'aide d'une séquence d'alignement et d'une séquence d'imagerie, et la séquence d'alignement étant réalisée indépendamment de la séquence d'imagerie ;

un code de programme lisible par ordinateur qui génère des données d'image IRM quasi en temps réel (RT) d'au moins une partie d'une anatomie cible d'un patient à l'aide de plans de balayage anatomiques d'intérêt ;

un code de programme lisible par ordinateur qui identifie des coordonnées spatiales associées à un emplacement d'au moins une partie d'extrémité distale d'au moins un dispositif médical intracorporel souple dans l'espace d'image en 3D à l'aide des données de signal d'alignement ; et

un code de programme lisible par ordinateur qui rend des visualisations quasi en RT dynamiques du dispositif médical intracorporel souple dans l'espace d'image en 3D avec les images IRM quasi en RT, le dispositif ne se trouvant pas nécessairement dans un plan de balayage anatomique d'intérêt utilisé pour obtenir les des données IRM quasi en temps réel, et la partie d'extrémité distale du dispositif pouvant varier en termes de forme au cours de la procédure guidée par IRM.

20. Produit de programme informatique de la revendication 19, comprenant en outre :

un code de programme lisible par ordinateur qui calcule un emplacement d'interface cathéter-tissu à proximité d'un emplacement de pointe du cathéter dans l'espace d'image IRM tridimensionnelle, le calcul étant configuré pour projeter mathématiquement axialement vers l'avant une distance définie au-delà de la pointe pour définir l'interface cathéter-tissu, le calcul de l'interface cathéter/tissu étant réalisé à l'aide de coordonnées X, Y, Z des emplacements des bobines

d'alignement de sorte à placer l'emplacement de l'interface cathéter-tissu à une distance d'environ 0 à 4 mm au-delà d'un emplacement calculé de la pointe d'au moins un des cathéters intracorporels souples, et l'interface cathéter/tissu calculée étant soit (a) calculée pour être tangente et sensiblement alignée avec au moins deux des bobines d'alignement, soit (b) calculée sous la forme d'un plan dans un espace d'image en 3D à proximité d'un plan projeté défini par au moins trois points associés à trois bobines différentes des bobines d'alignement (82) ; et un code de programme lisible par ordinateur qui utilise l'emplacement d'interface de tissu calculée pour définir automatiquement au moins un plan de balayage utilisé par l'appareil IRM pour obtenir les données d'image IRM au cours et/ou à un moment proche de l'administration d'un traitement thérapeutique et/ou d'une procédure diagnostique.

21. Produit de programme informatique de la revendication 20, dans lequel le code de programme lisible par ordinateur qui rend les visualisations dynamiques comprend en outre un code programme lisible par ordinateur qui fournit un modèle volumétrique acquis au préalable enregistré d'une structure anatomique cible d'un patient dans les visualisations, et dans lequel la séquence d'alignement déphase les signaux perpendiculaires à une direction de lecture afin d'atténuer les signaux non souhaités provenant 1) de masses et 2) de régions détectées par des parties sensibles aux signaux du cathéter souple (80) de façon à laisser un pic aigu indiquant la position des bobines d'alignement, et dans lequel, une fois la séquence d'alignement effectuée, une impulsion de gradient peut être utilisée pour déphaser tout signal transversal résiduel avant l'exécution de la séquence d'image.

22. Produit de programme informatique de la revendication 21, comprenant en outre un code de programme lisible par ordinateur configuré pour permettre à un utilisateur (a) d'effectuer une rotation des visualisations, et (b) de modifier une visualisation affichée pour inclure uniquement des données d'image quasi en RT de l'anatomie cible, pour inclure les données d'image quasi en RT de l'anatomie et le modèle enregistré de la structure anatomique, ou d'inclure uniquement le modèle enregistré de la structure anatomique, et/ou comprenant en outre un code de programme lisible par ordinateur qui permet à un utilisateur de marquer électroniquement ou de choisir des sites de lésion cibles sur le modèle, et/ou comprenant en outre un code de programme lisible par ordinateur qui permet à un utilisateur d'afficher électroniquement sélectivement au moins une carte

de tissu alignée avec et/ou enregistrée dans le modèle volumétrique ou affichée au lieu du modèle, les choix de cartes comprenant au moins deux des éléments suivants :

- 5 une carte de caractérisation de tissu thermique ;
- une carte de caractérisation de tissu d'oedème ;
- une carte de caractérisation de tissu à renforcement retardé prise à un premier moment ;
- 10 une carte de caractérisation de tissu à renforcement retardé prise à un deuxième moment après la création d'un moins quelques lésions d'ablation dans le tissu cardiaque ;
- une carte de caractéristique de tissu vasculaire ;
- 15 une carte caractéristique de tissu fibreux ;
- une carte de caractérisation de tissu hypoxique ;
- une carte de caractérisation de tissu ischémique ;
- une carte de distribution de fluide ;
- 20 une carte d'exposition à la lumière ; et
- une carte électro-anatomique.

25

30



35

40

45

50

55

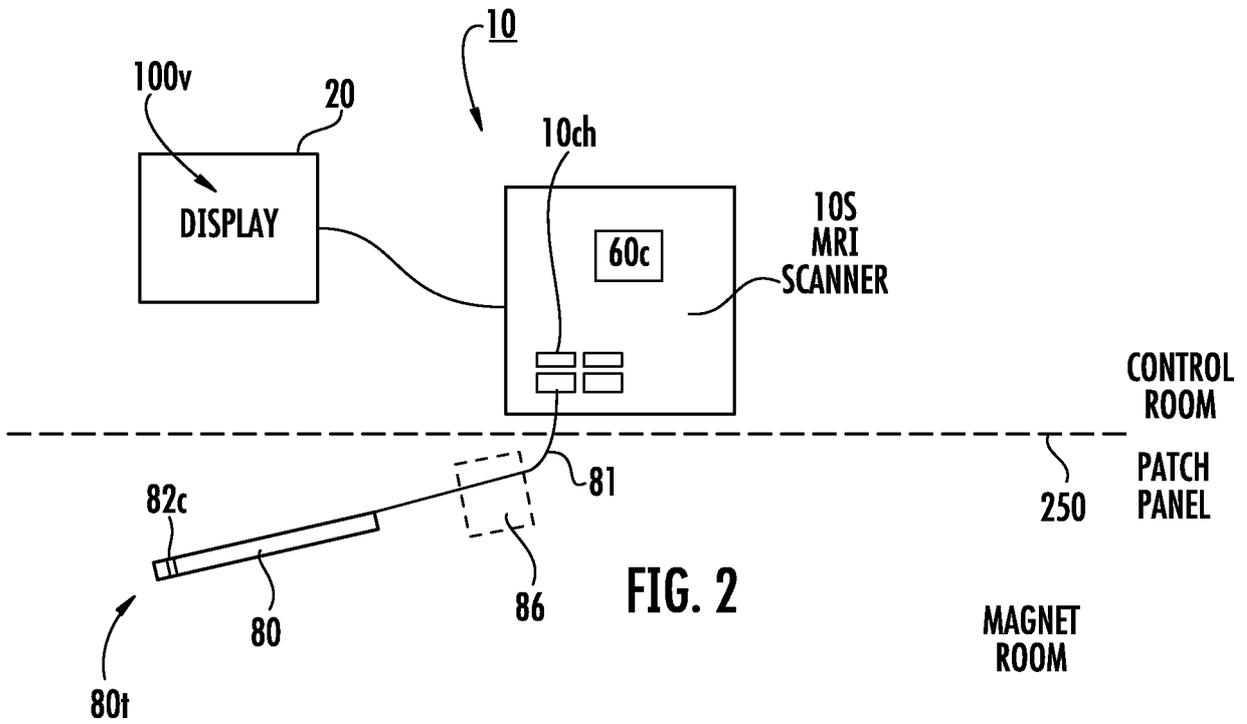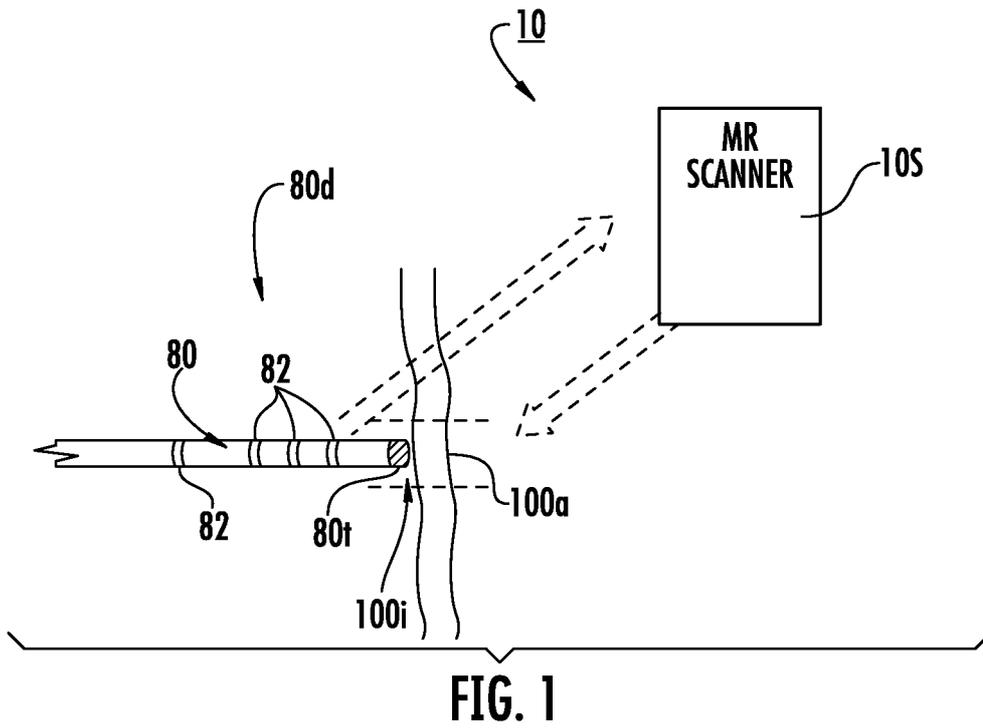

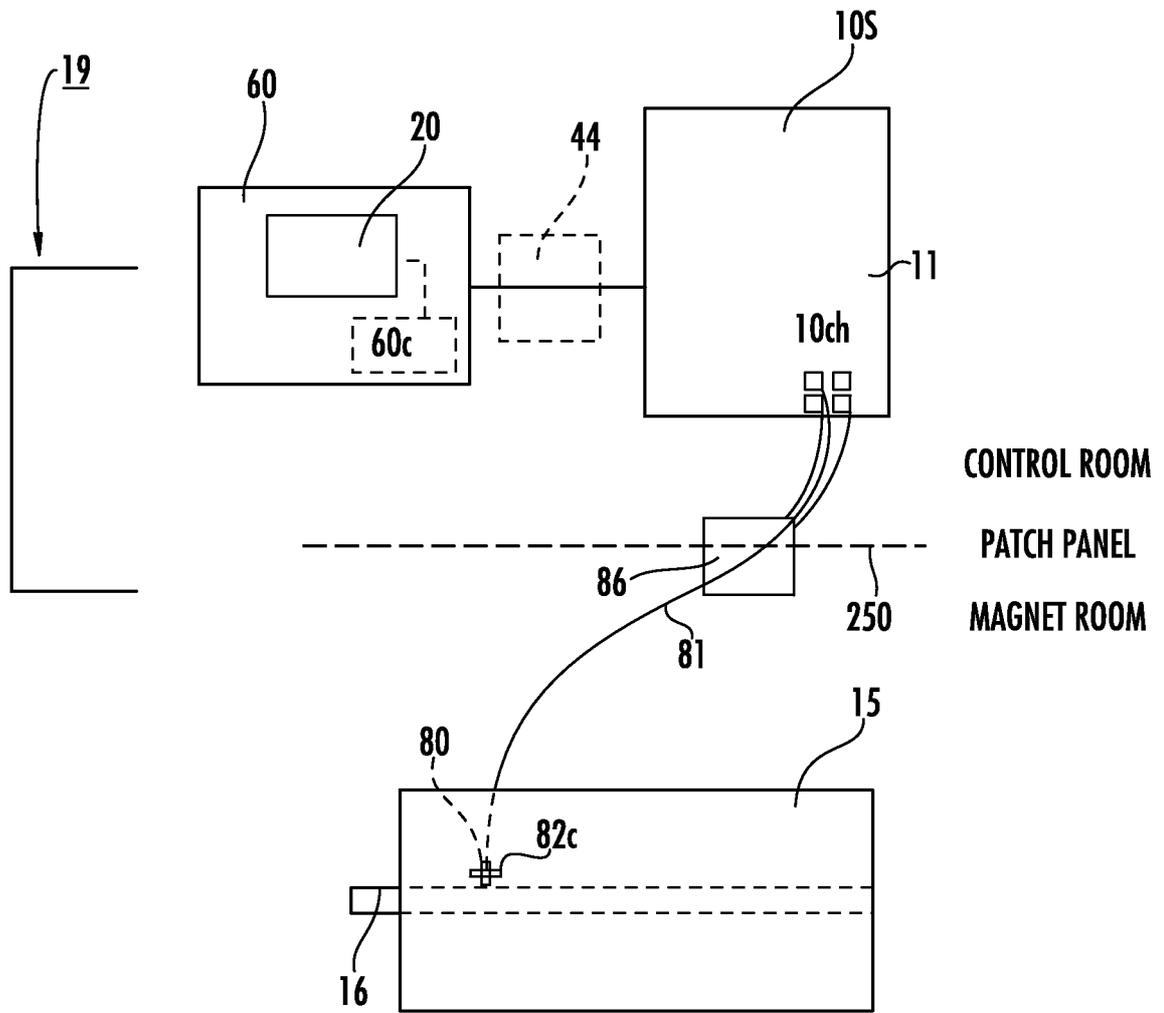


FIG. 3

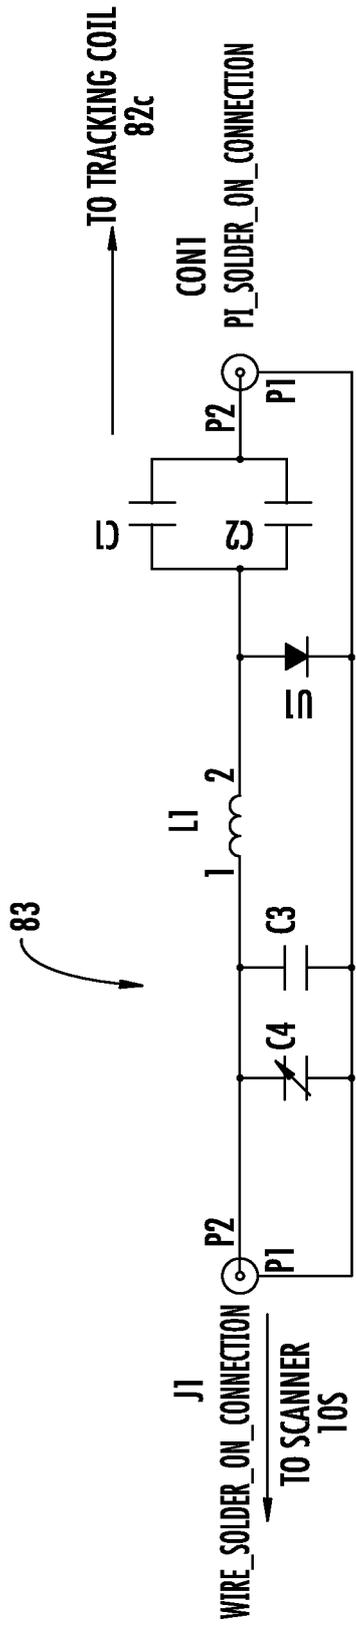


FIG. 4

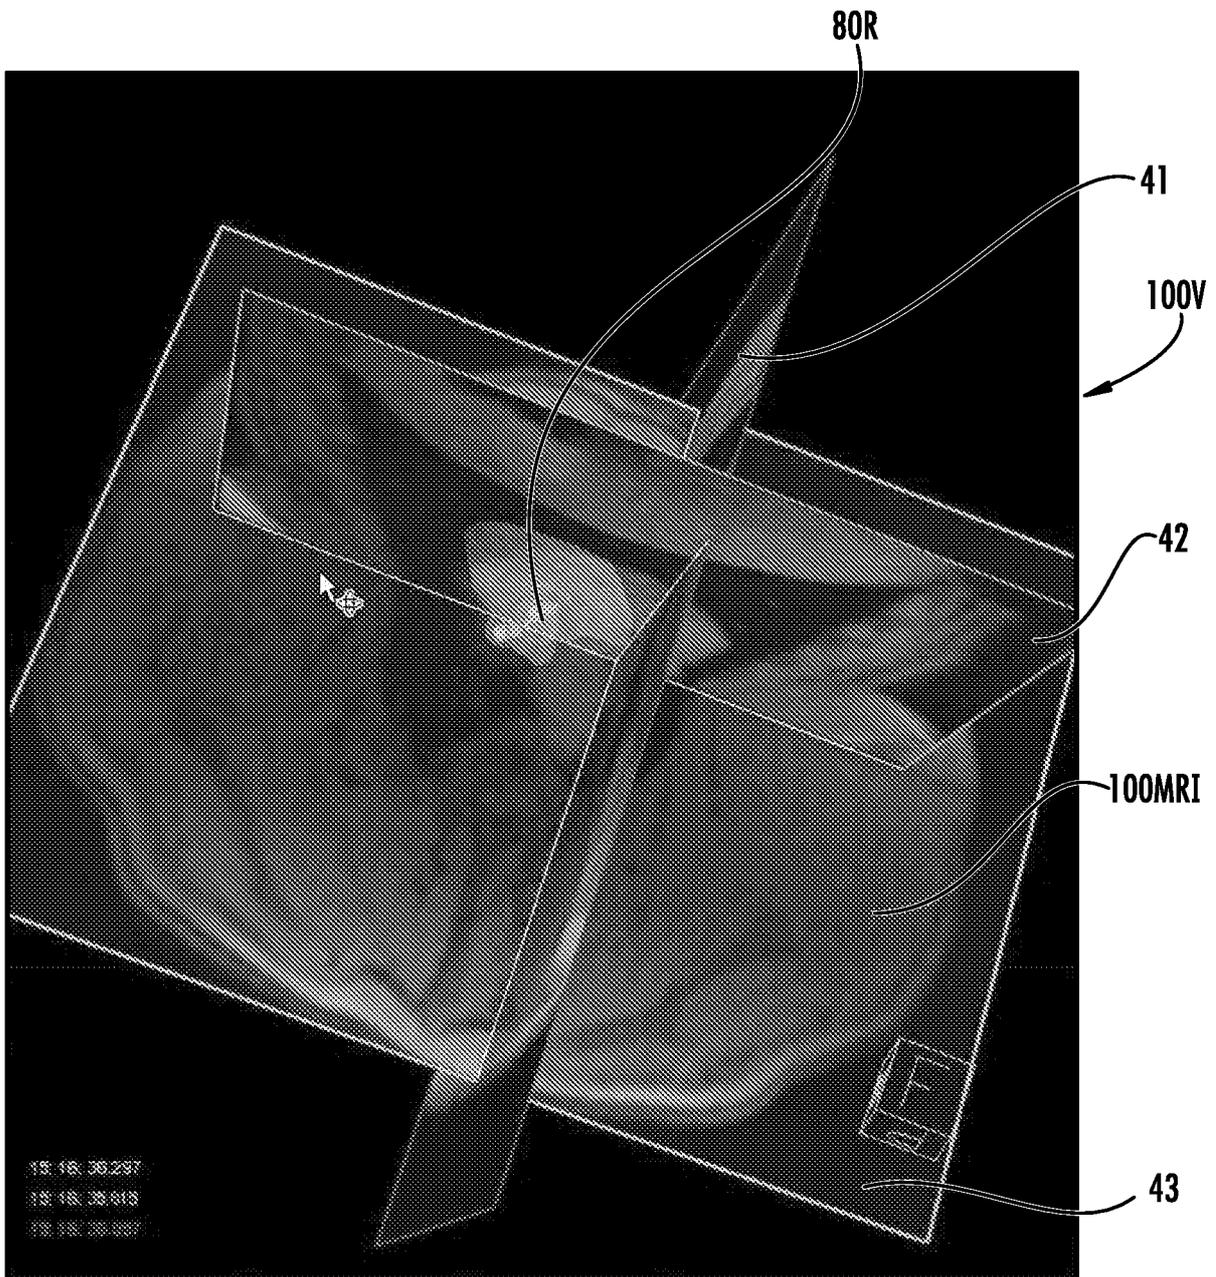


FIG. 5A

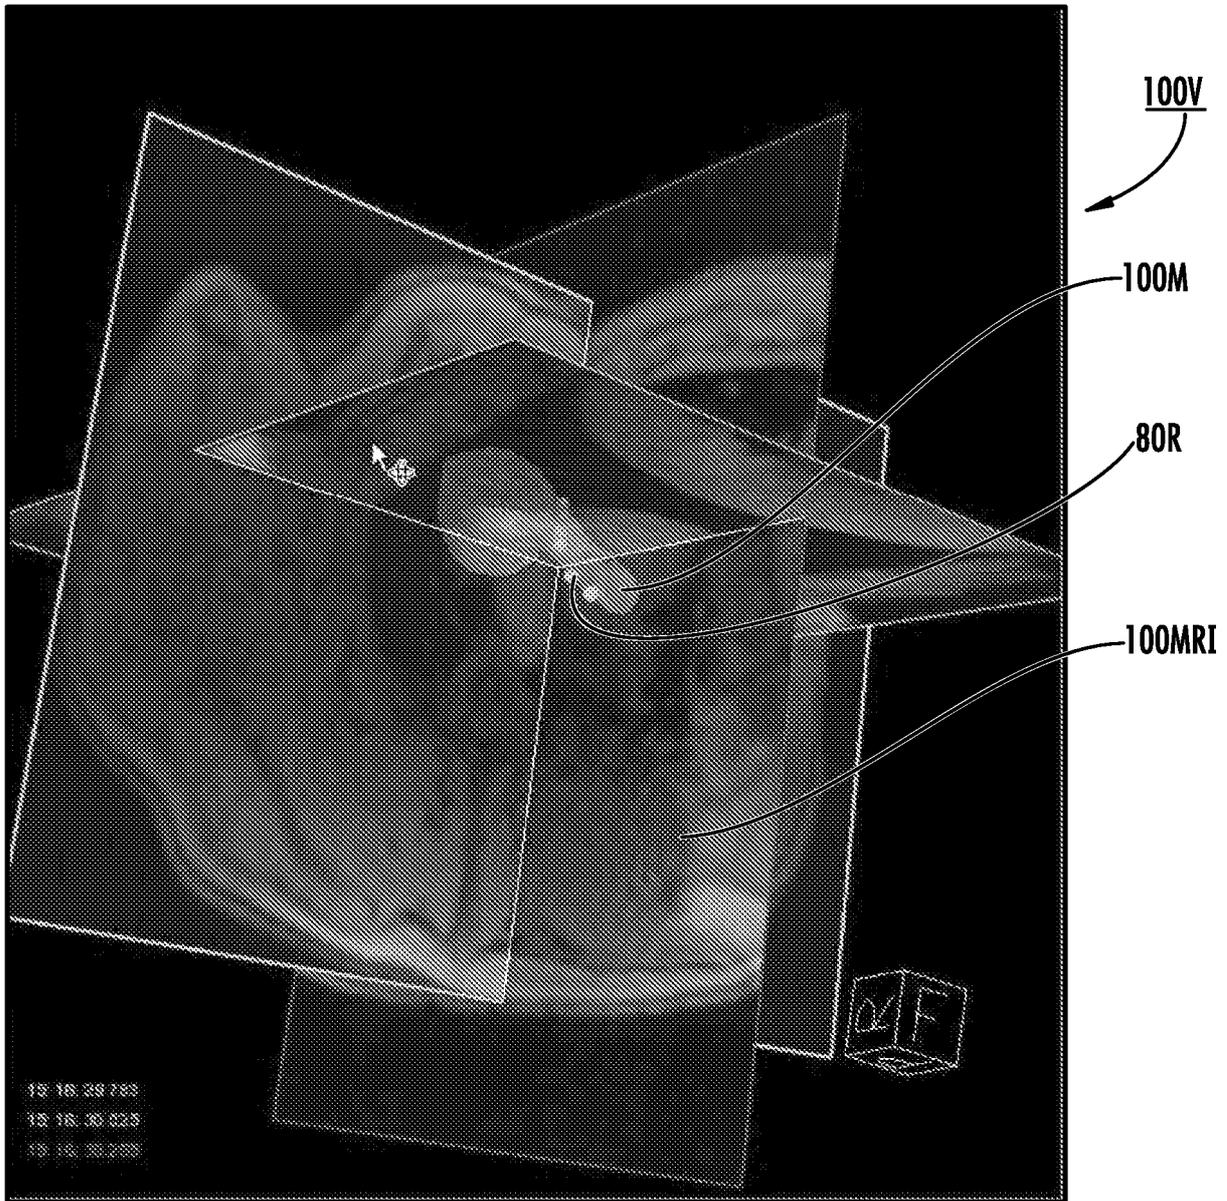


FIG. 5B

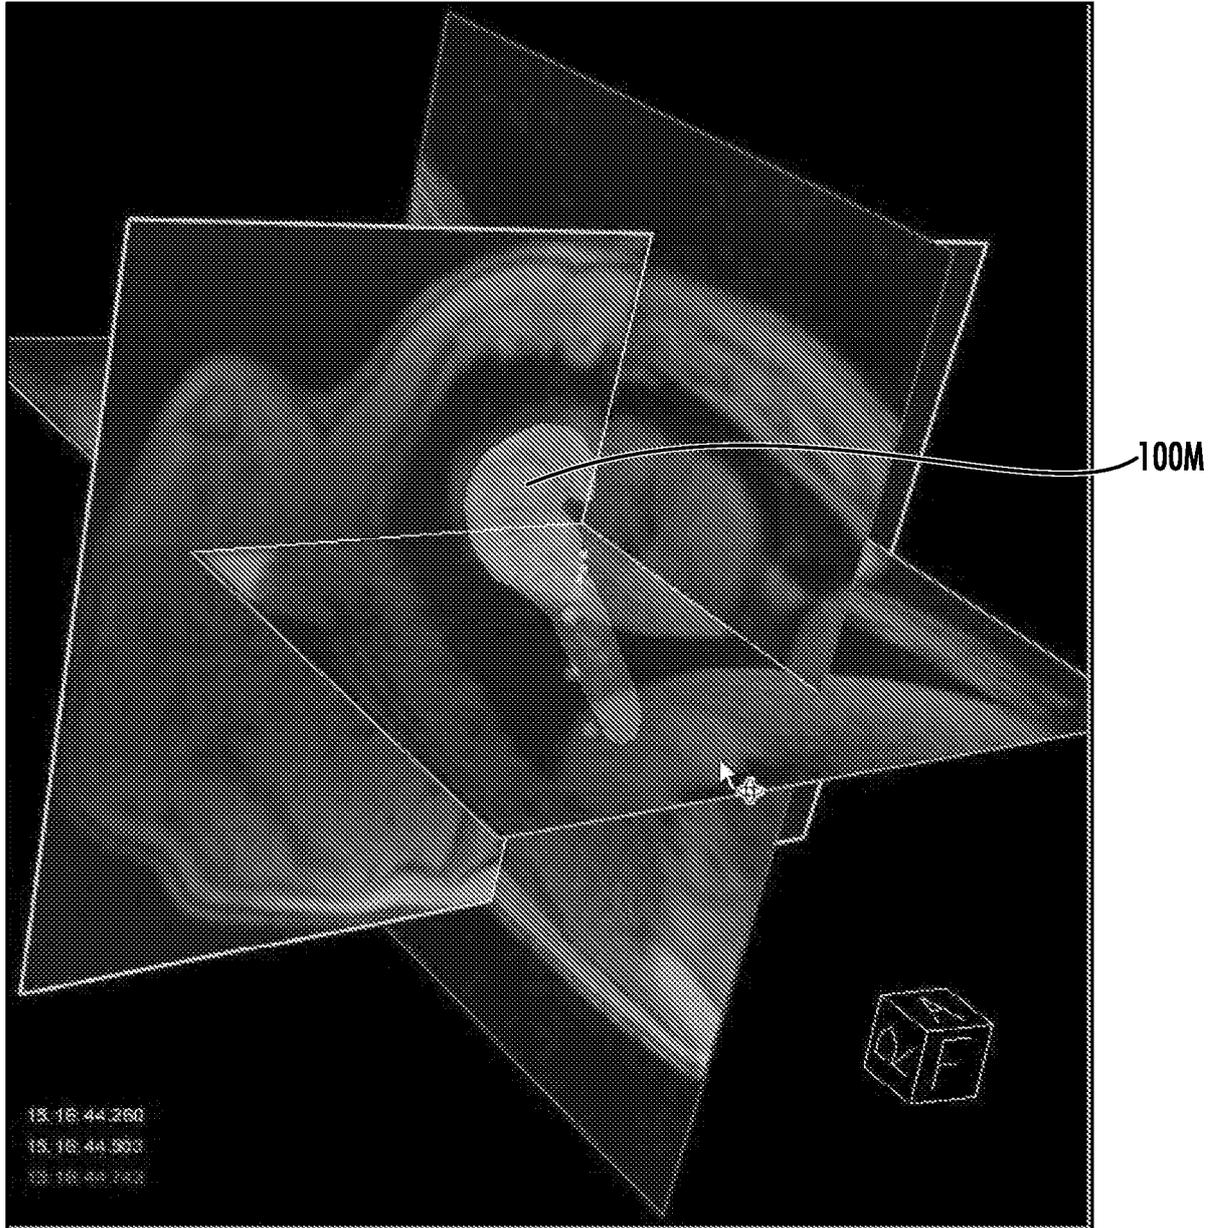


FIG. 5C

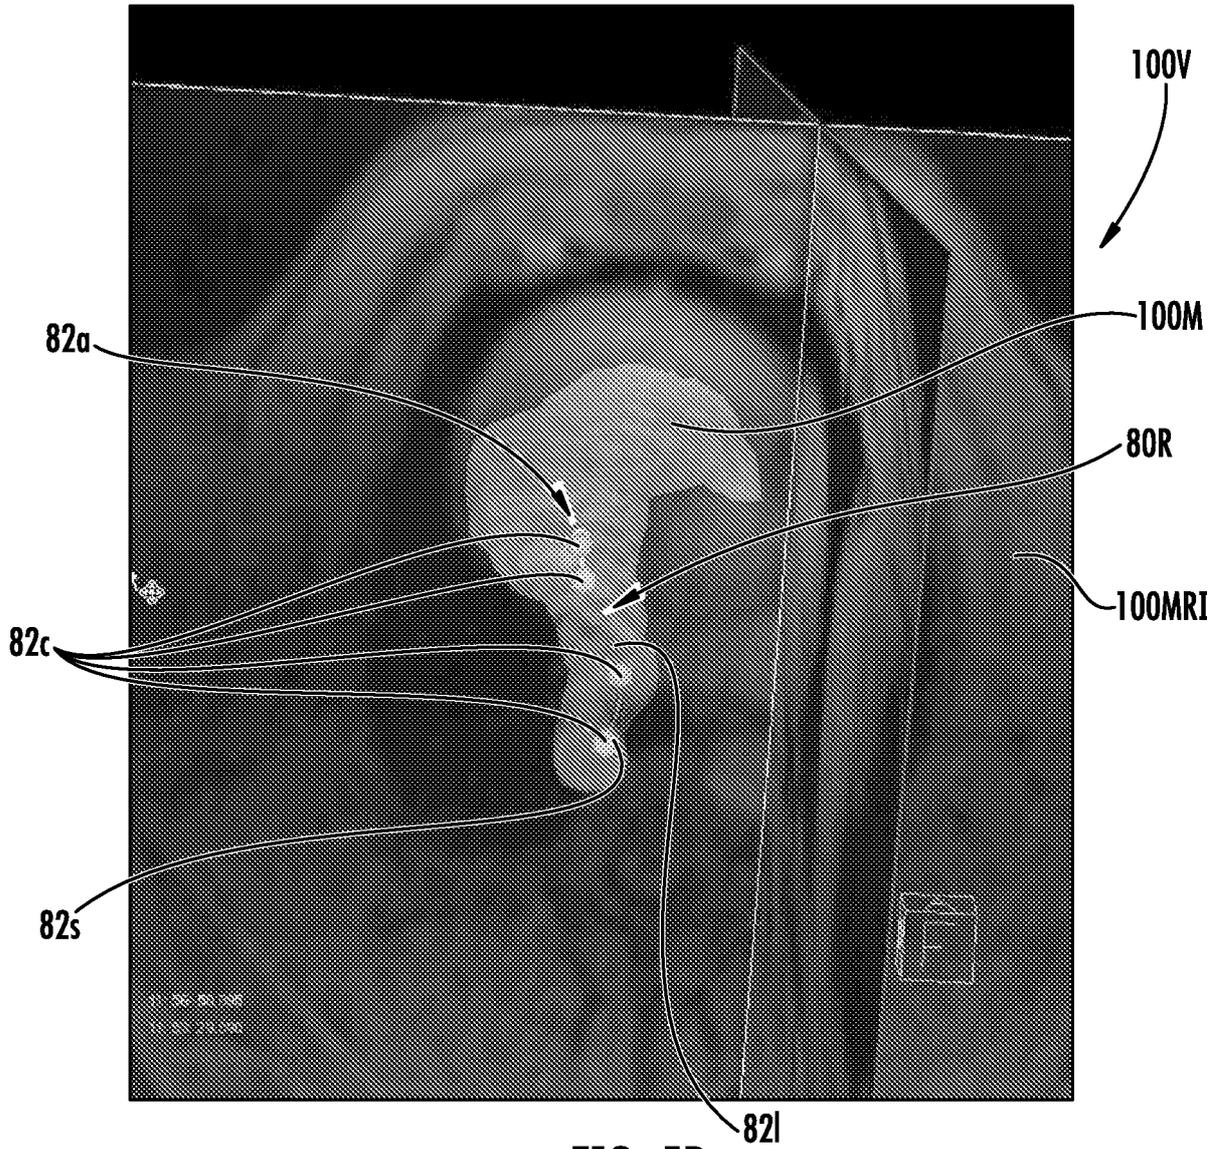
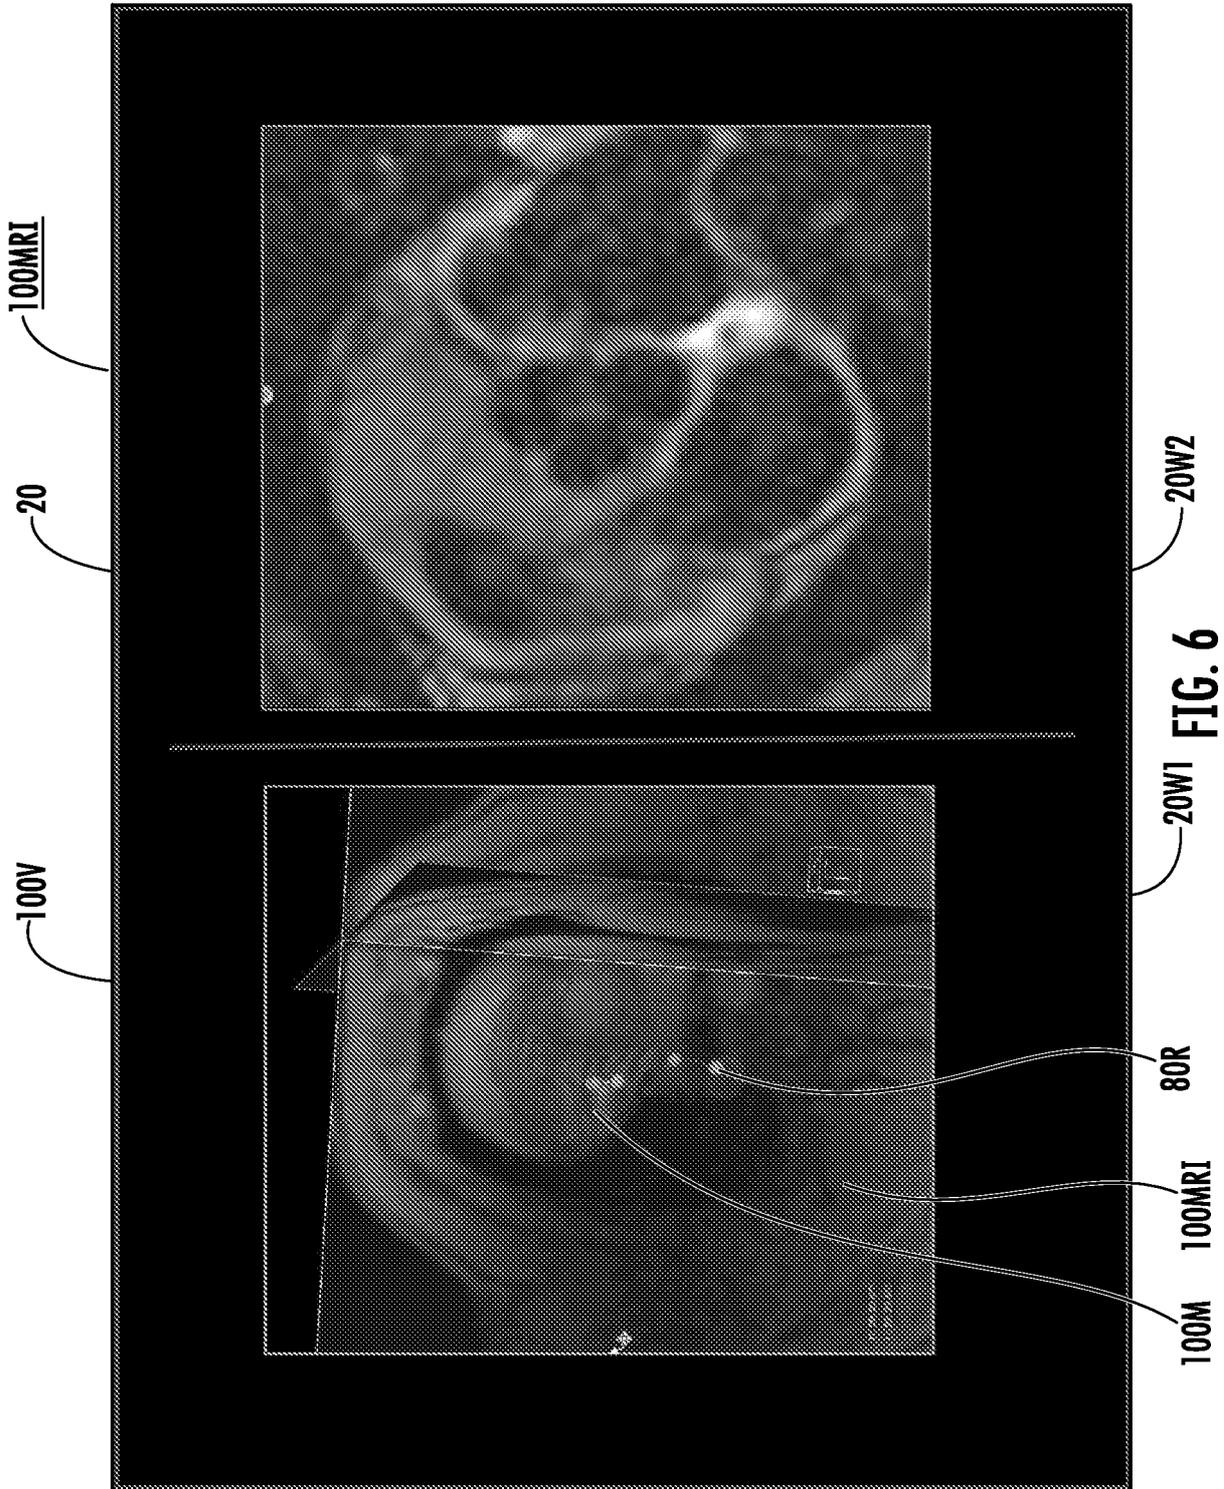
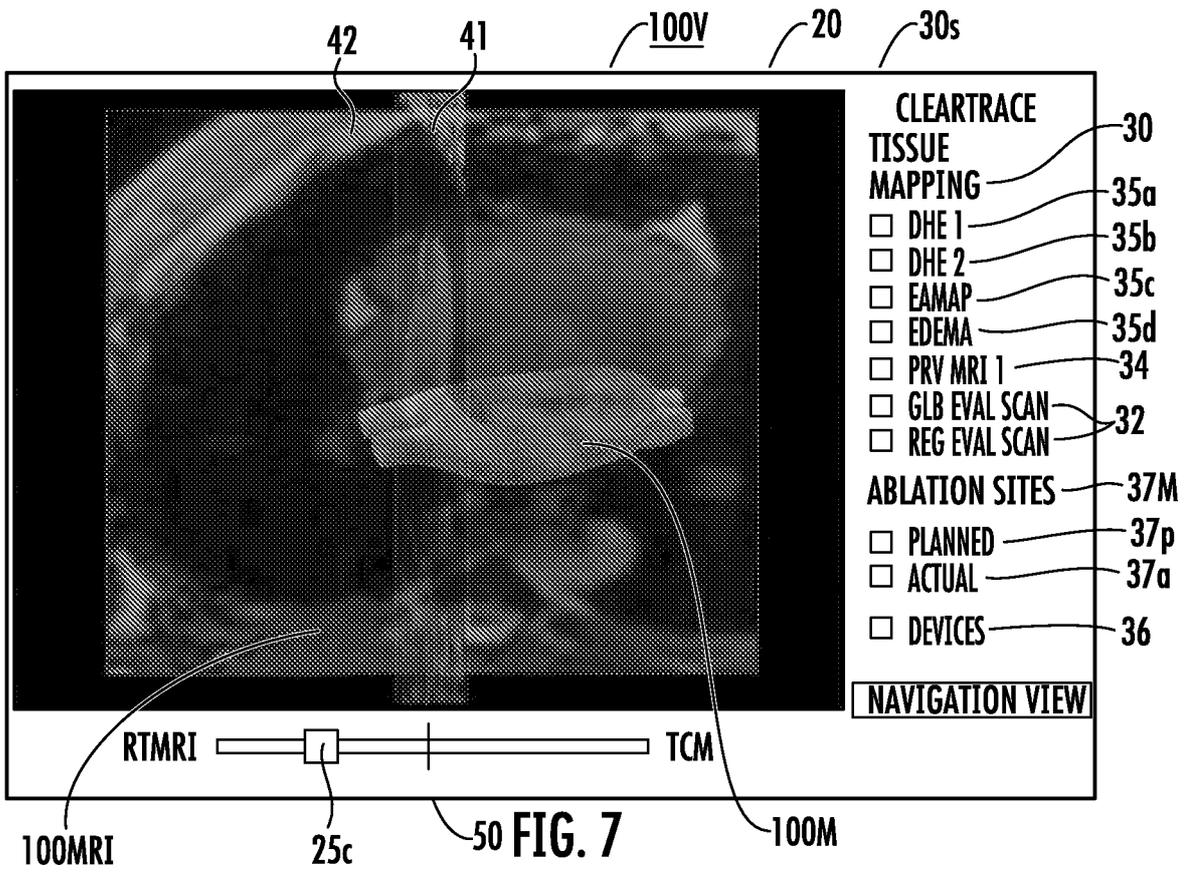
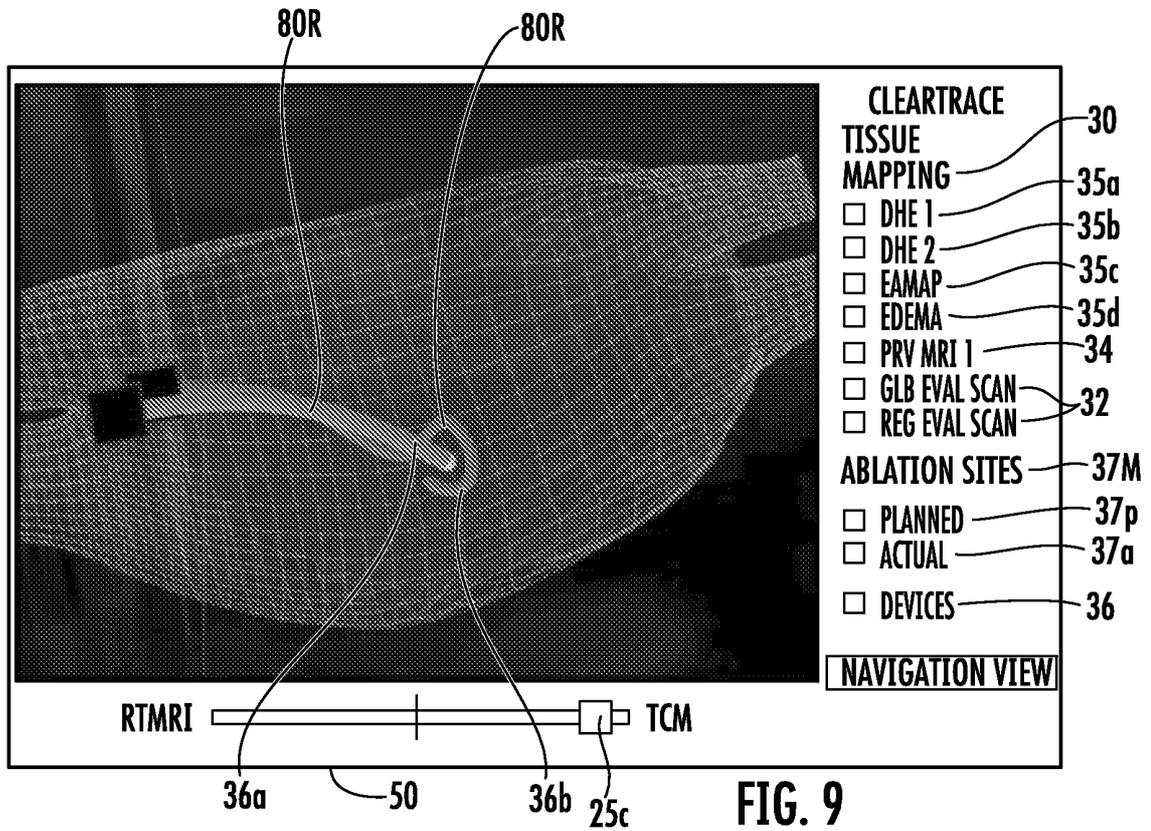
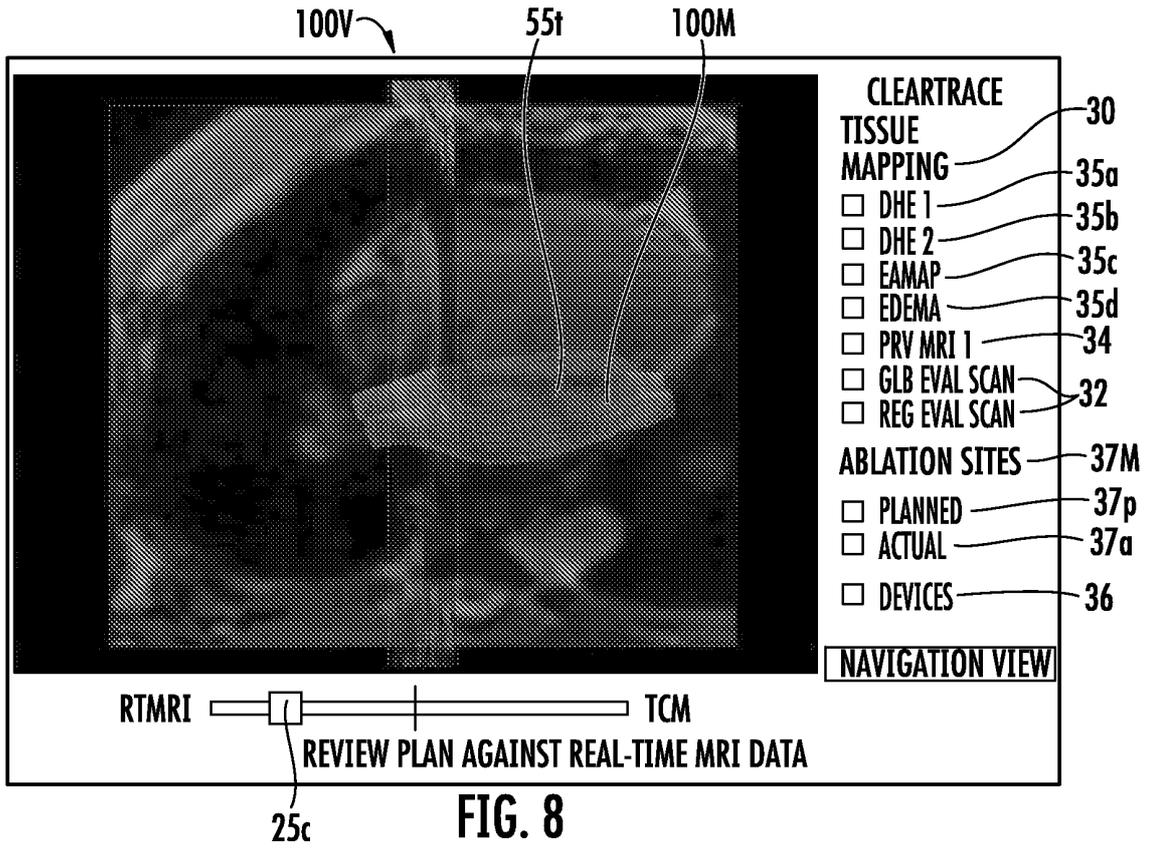
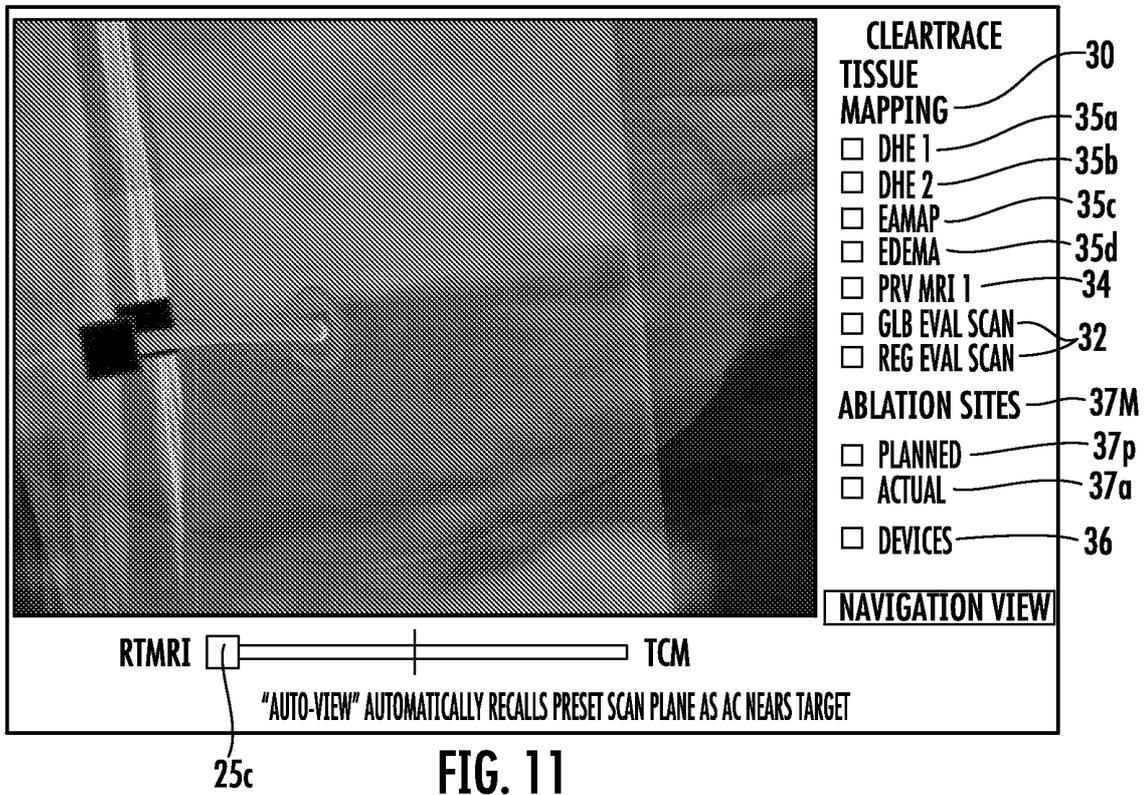
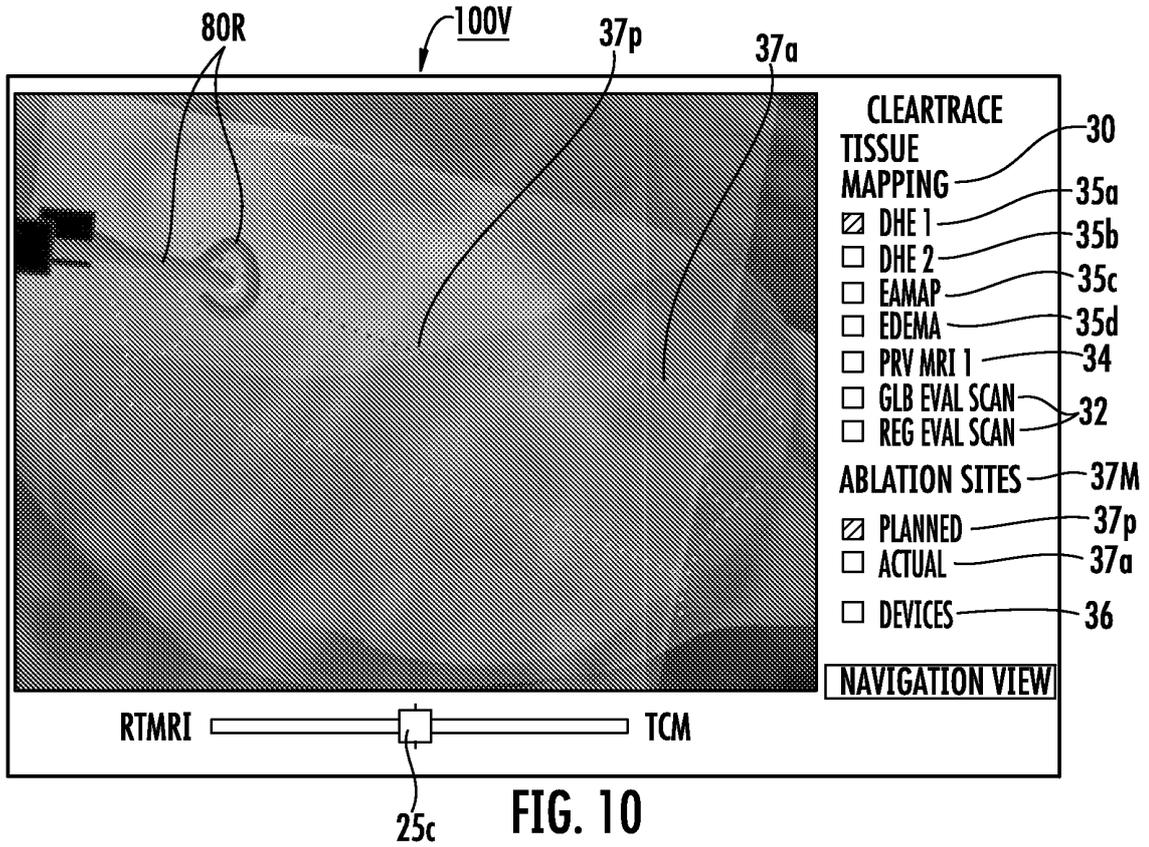


FIG. 5D









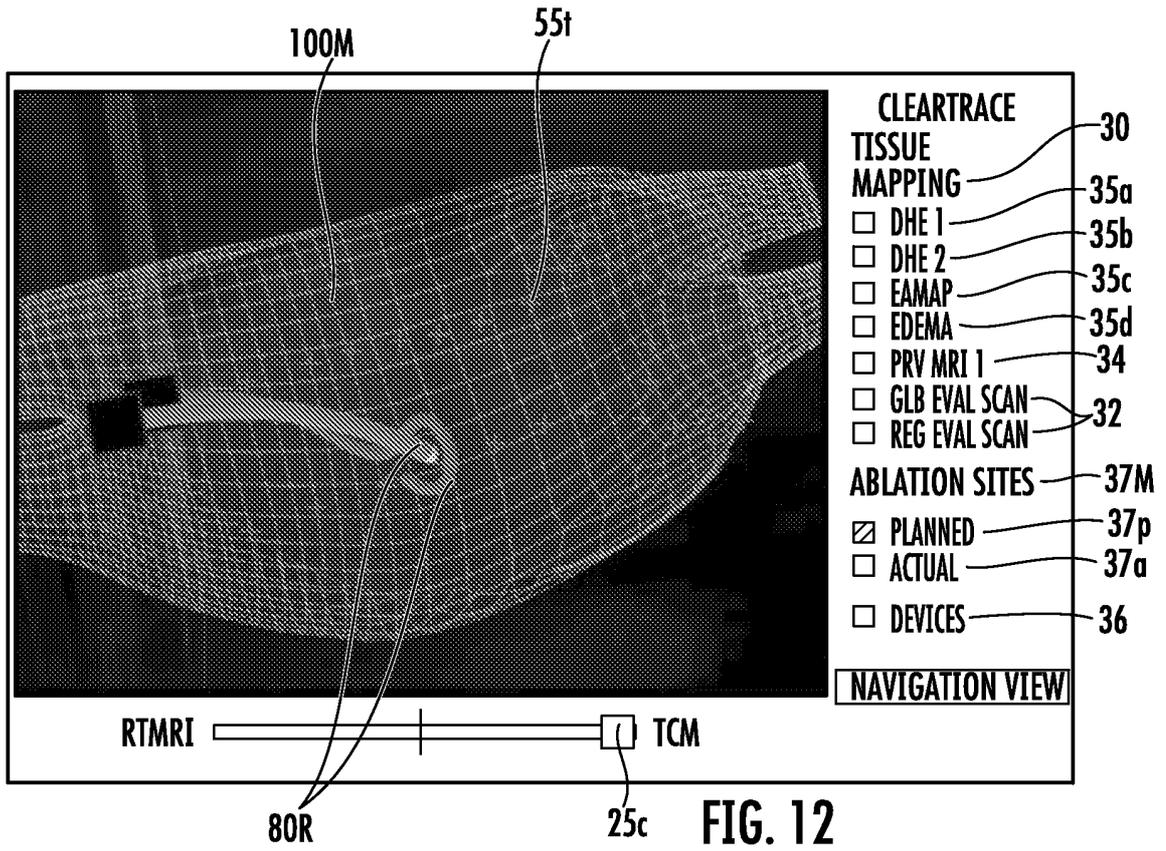


FIG. 12

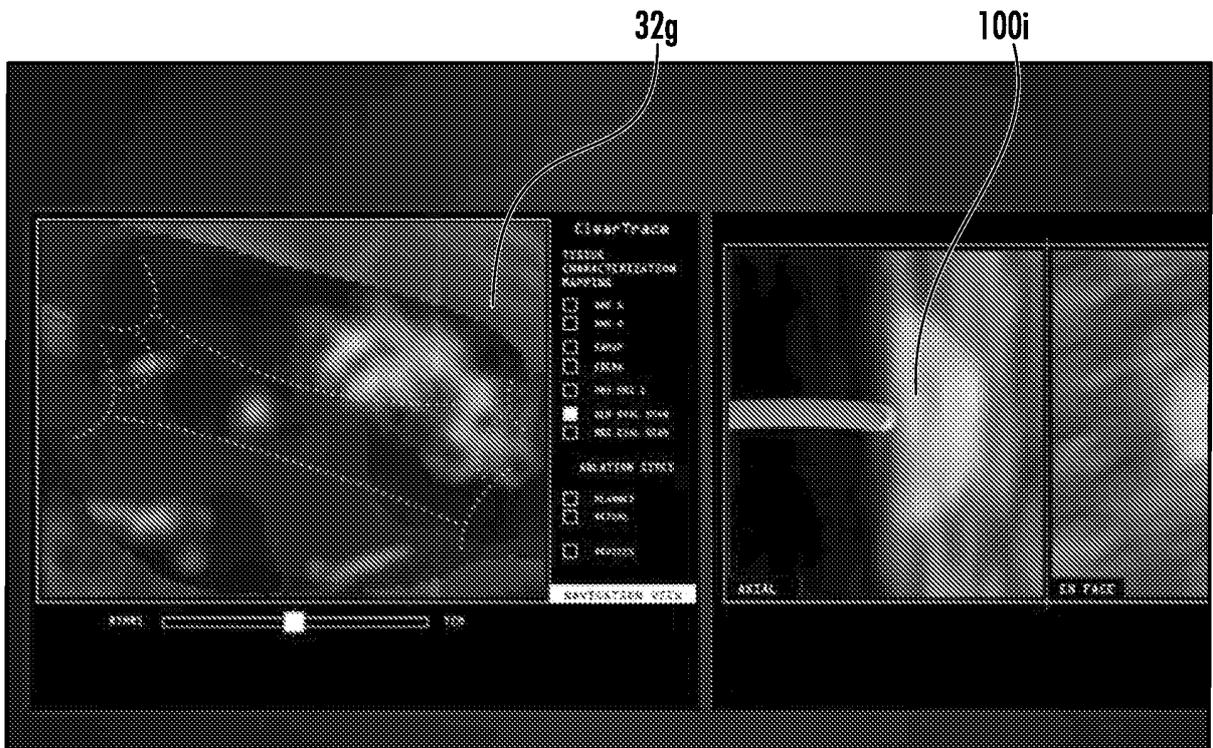


FIG. 13

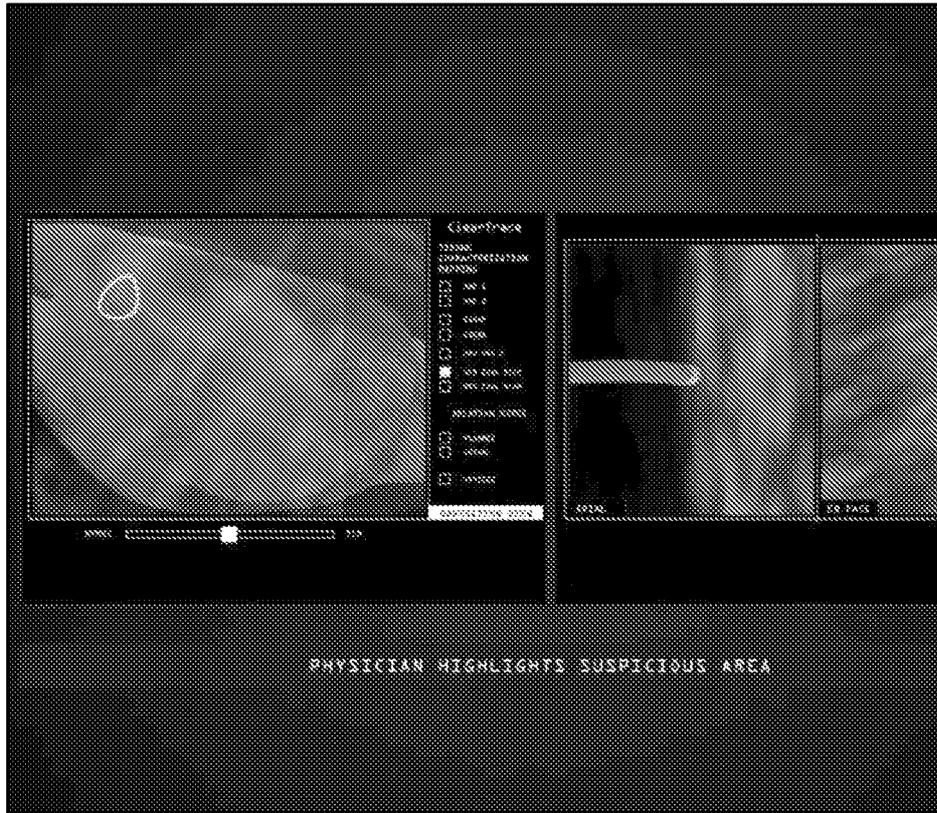


FIG. 14



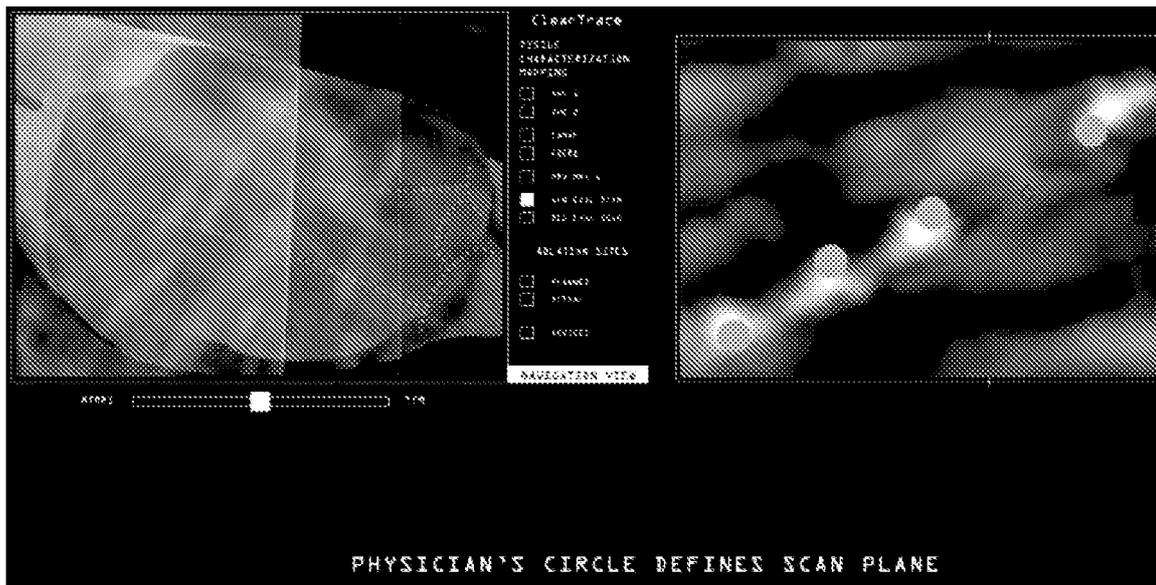



FIG. 15

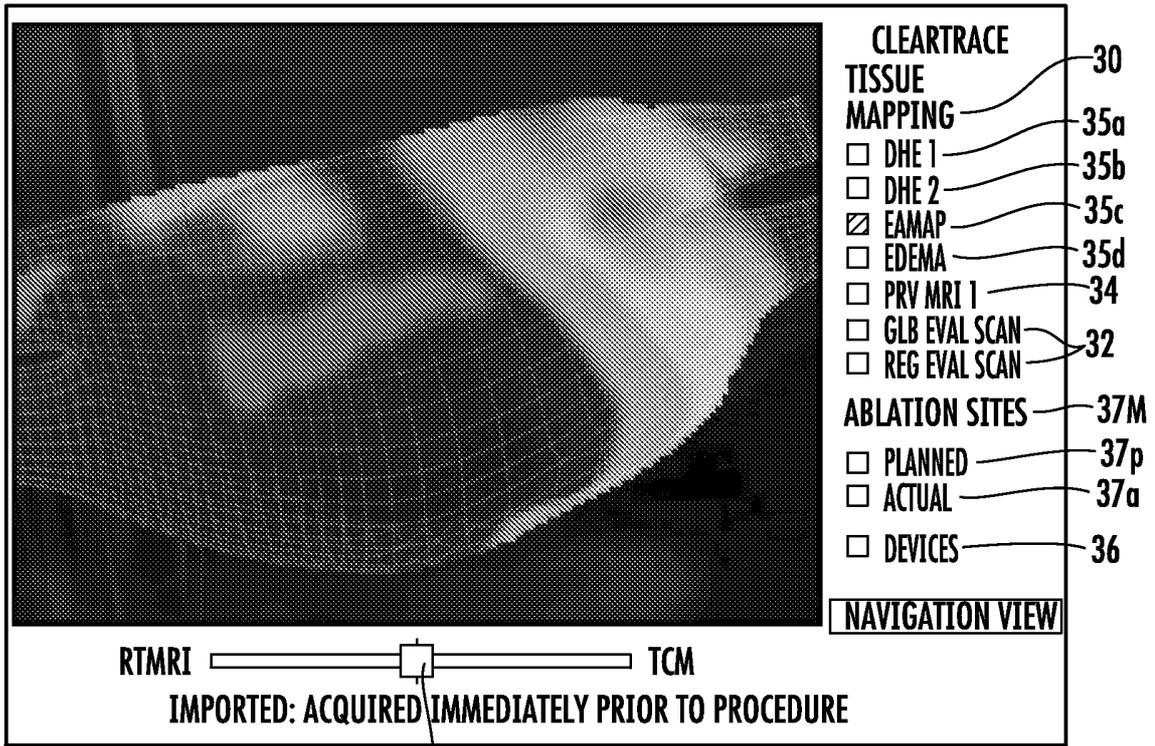


25c **FIG. 18**

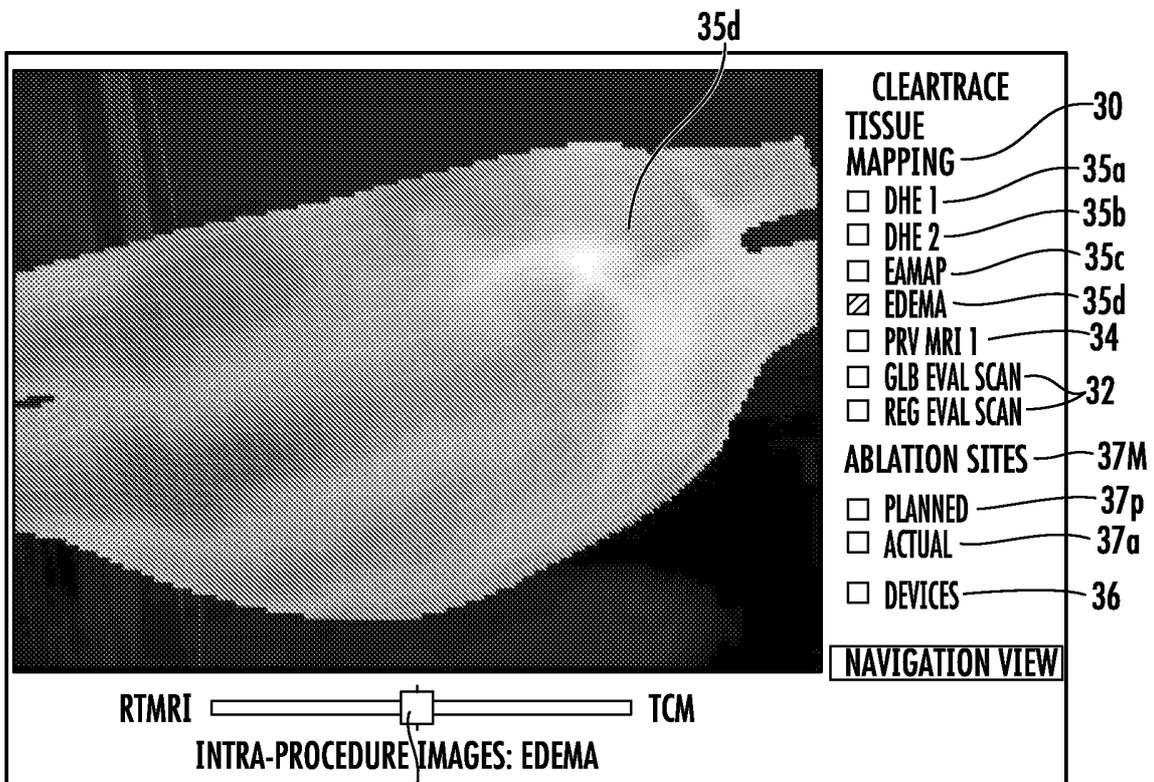

25c **FIG. 19**

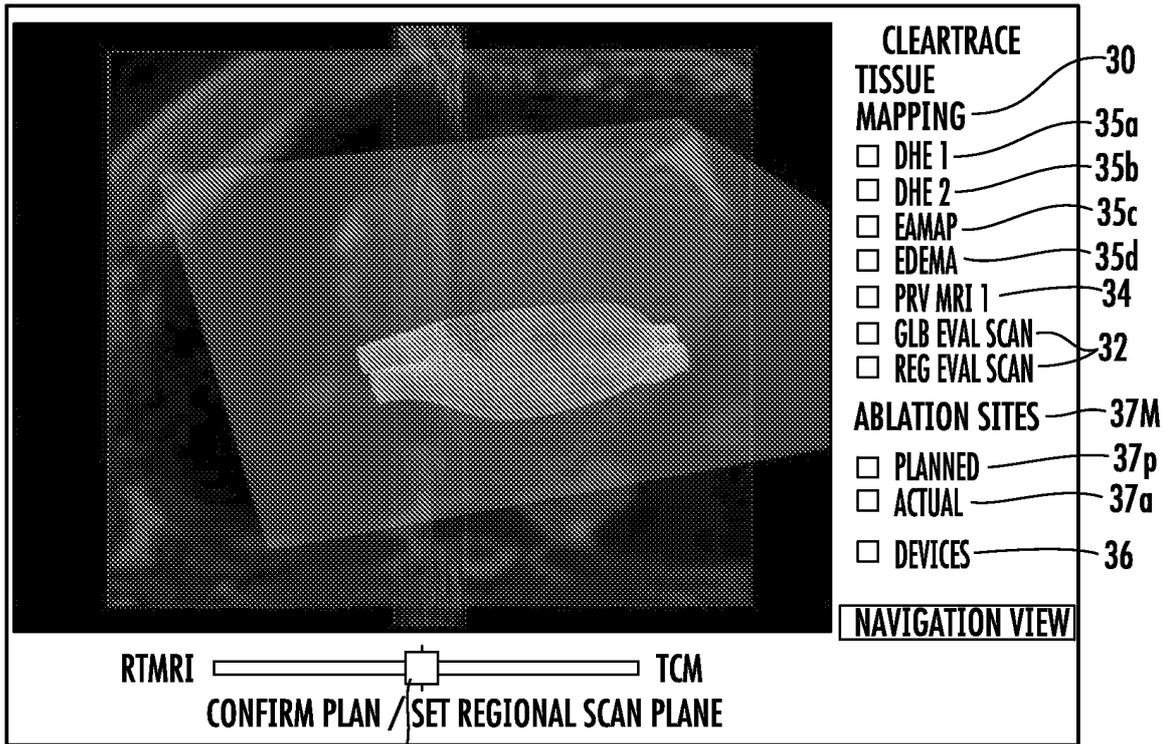

25c FIG. 20

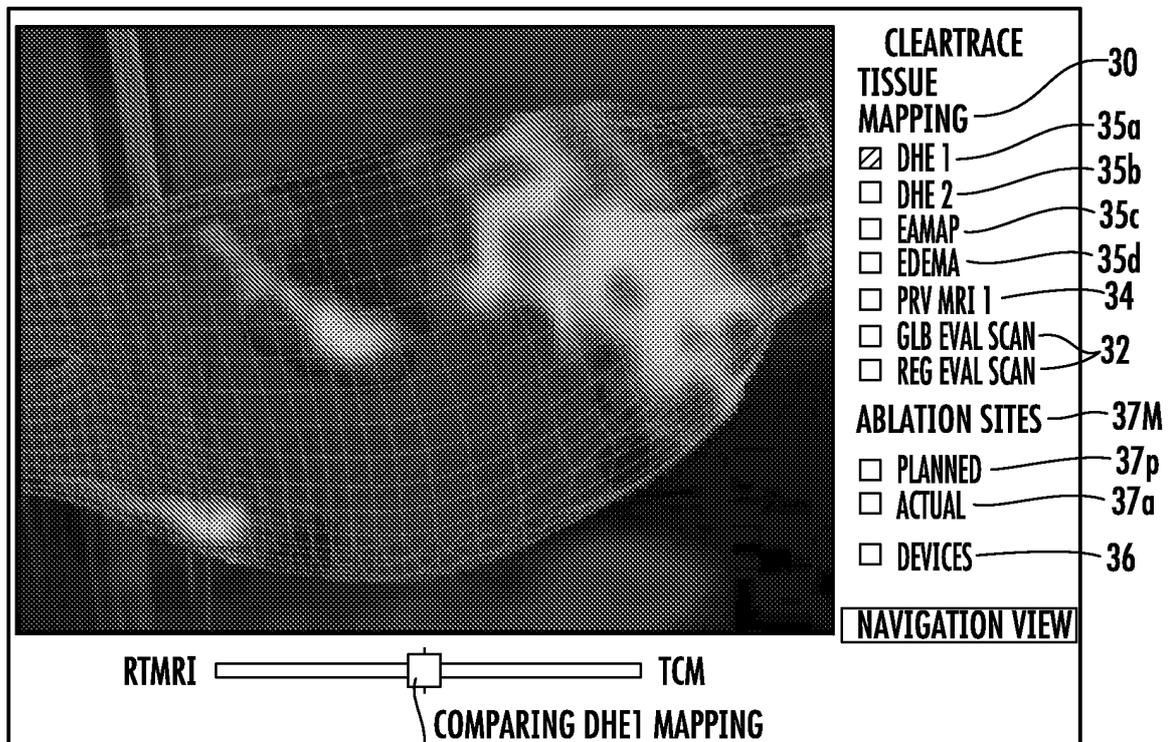

25c FIG. 21

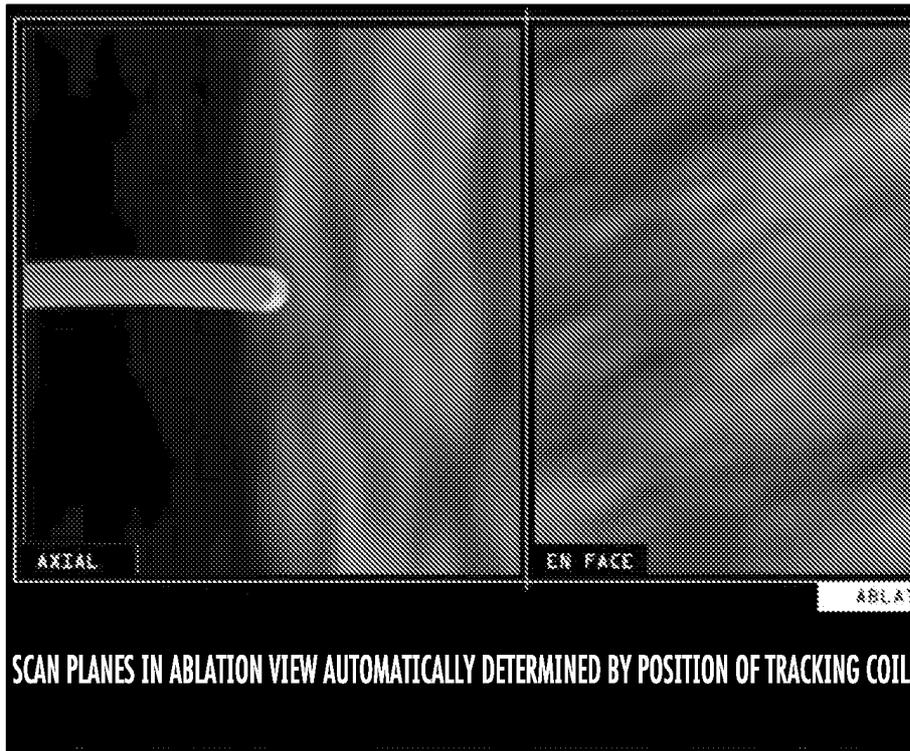


FIG. 22A

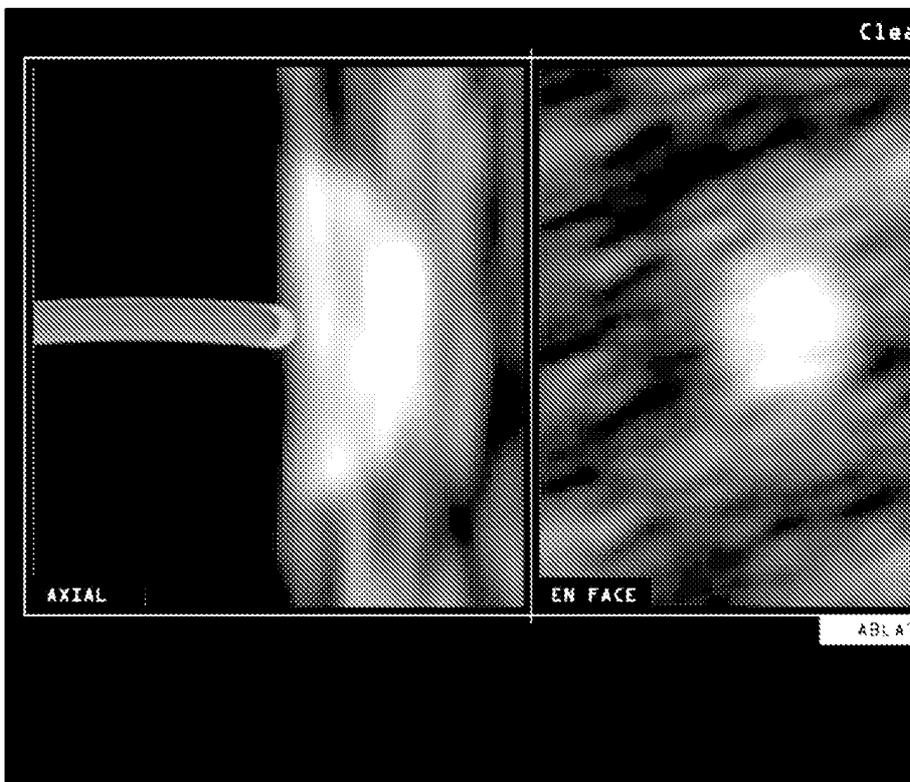


FIG. 22B

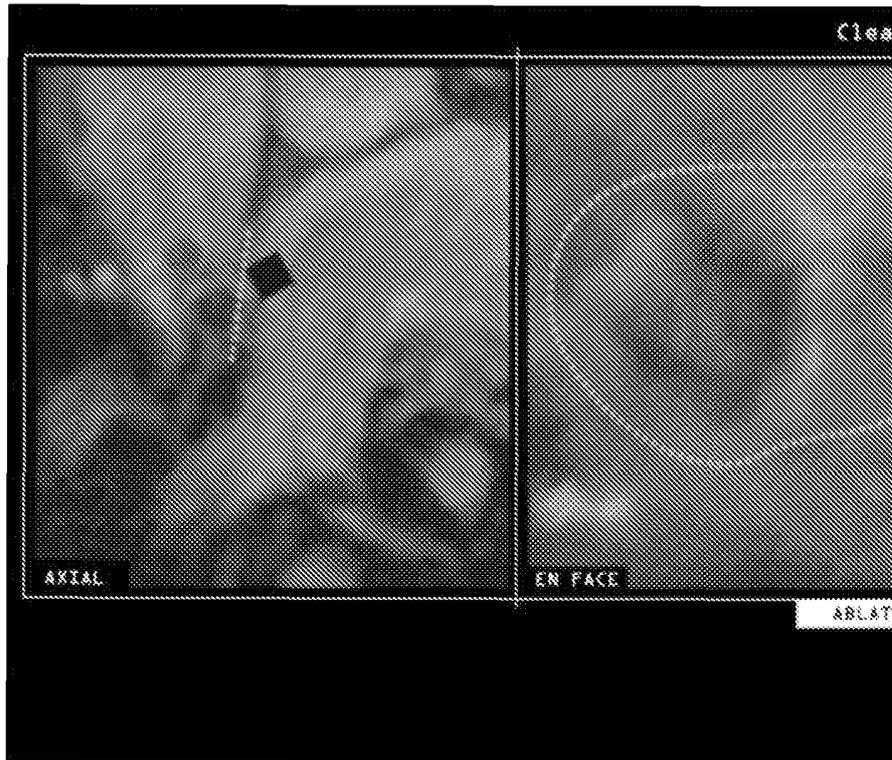


FIG. 23

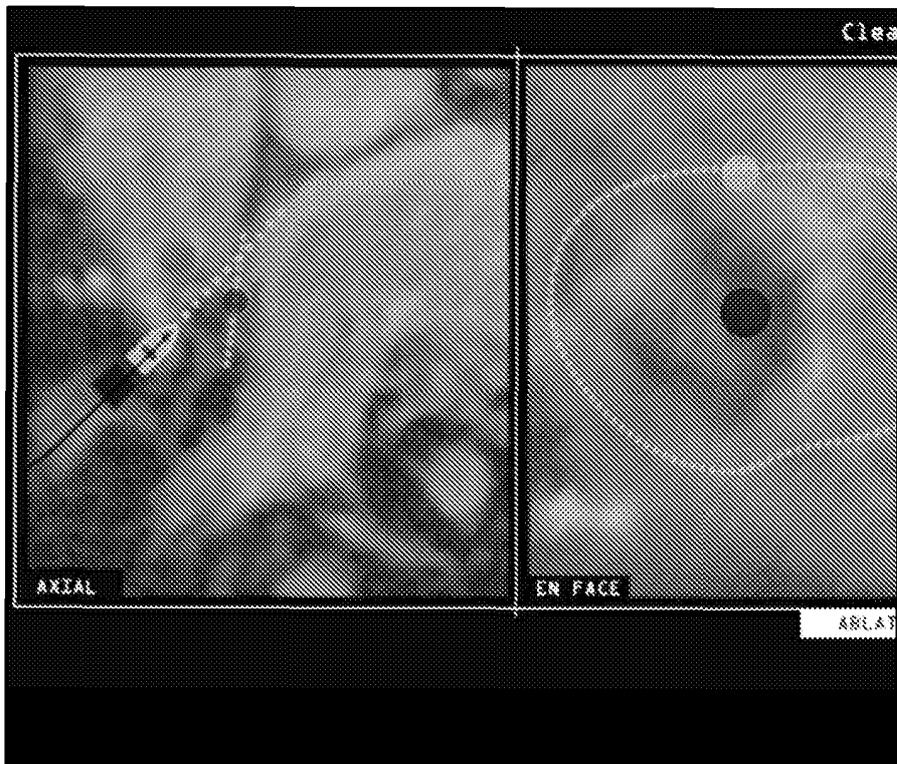


FIG. 24A

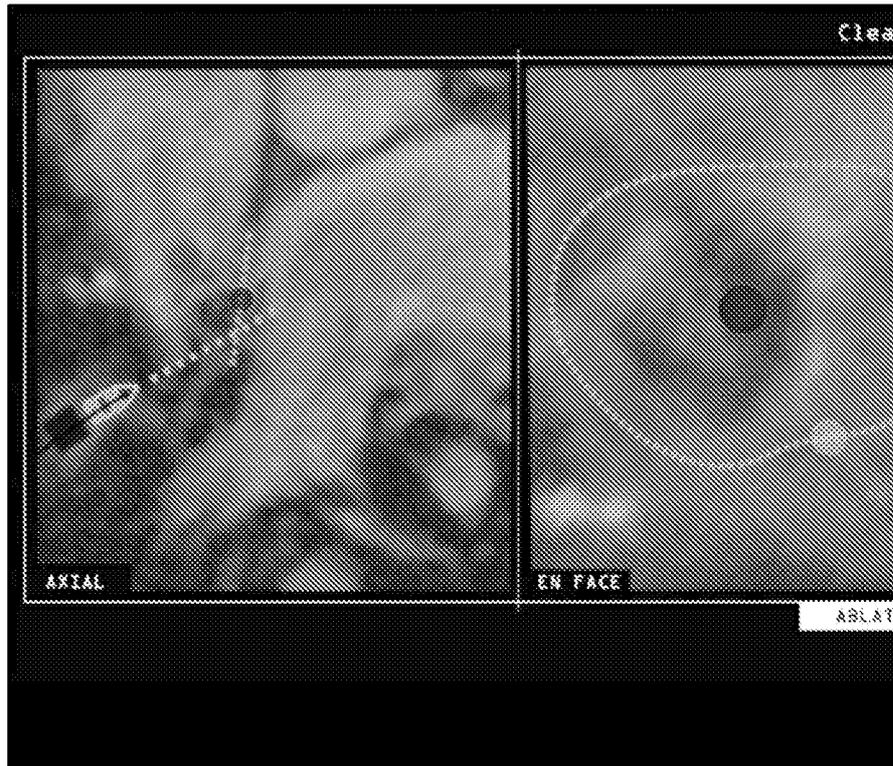


FIG. 24B

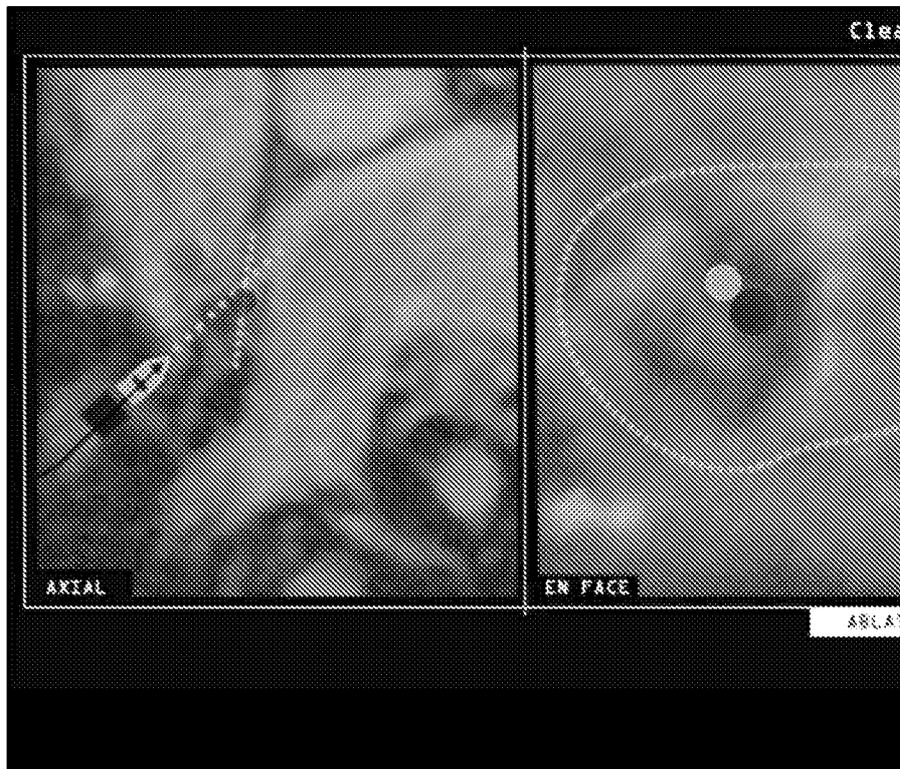


FIG. 24C

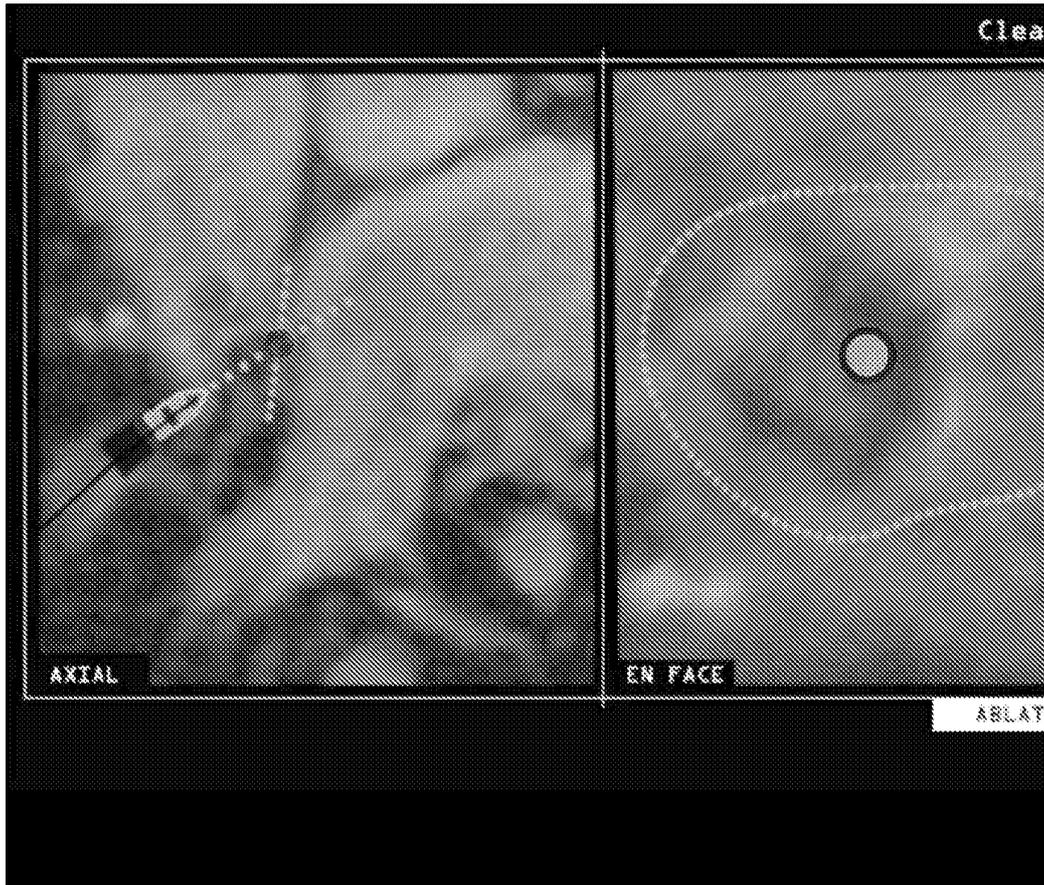


FIG. 24D



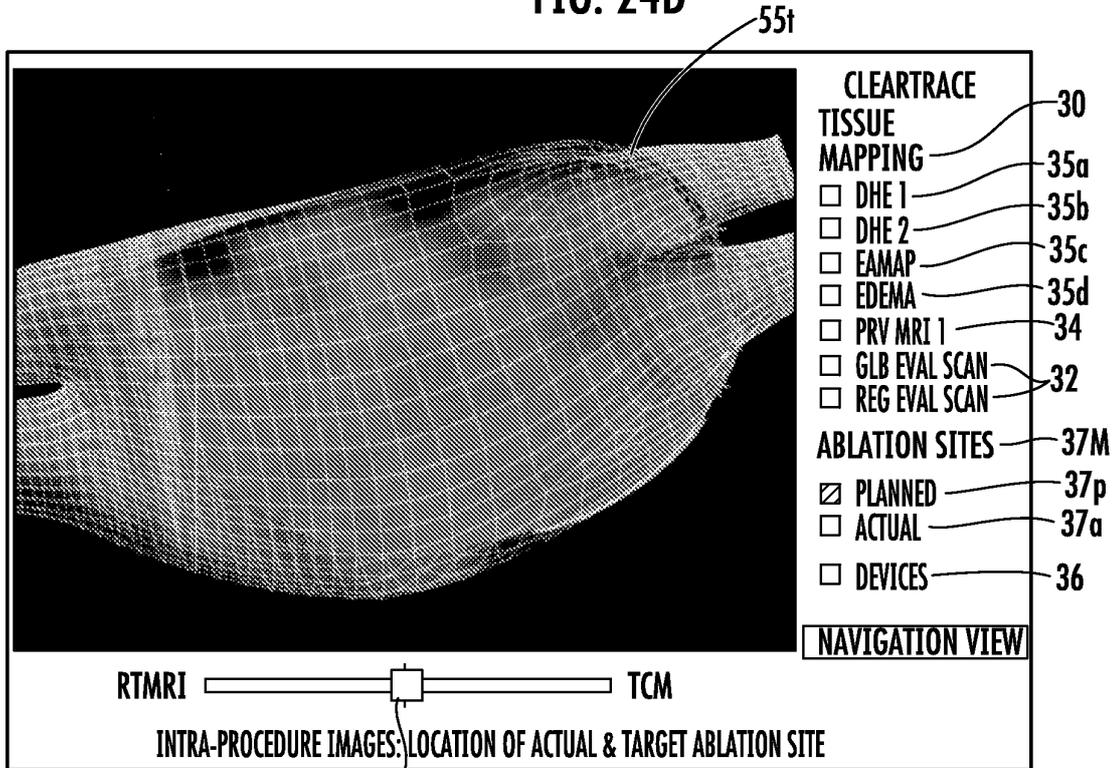


FIG. 25

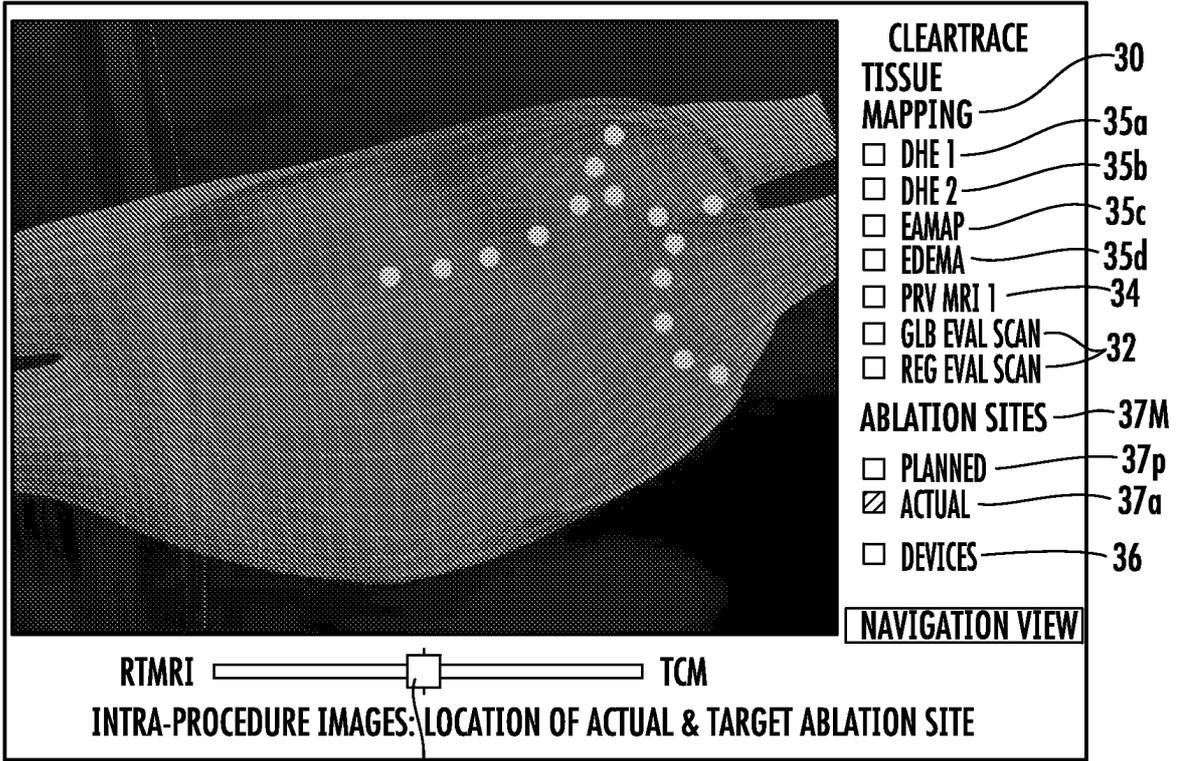

25c **FIG. 26**

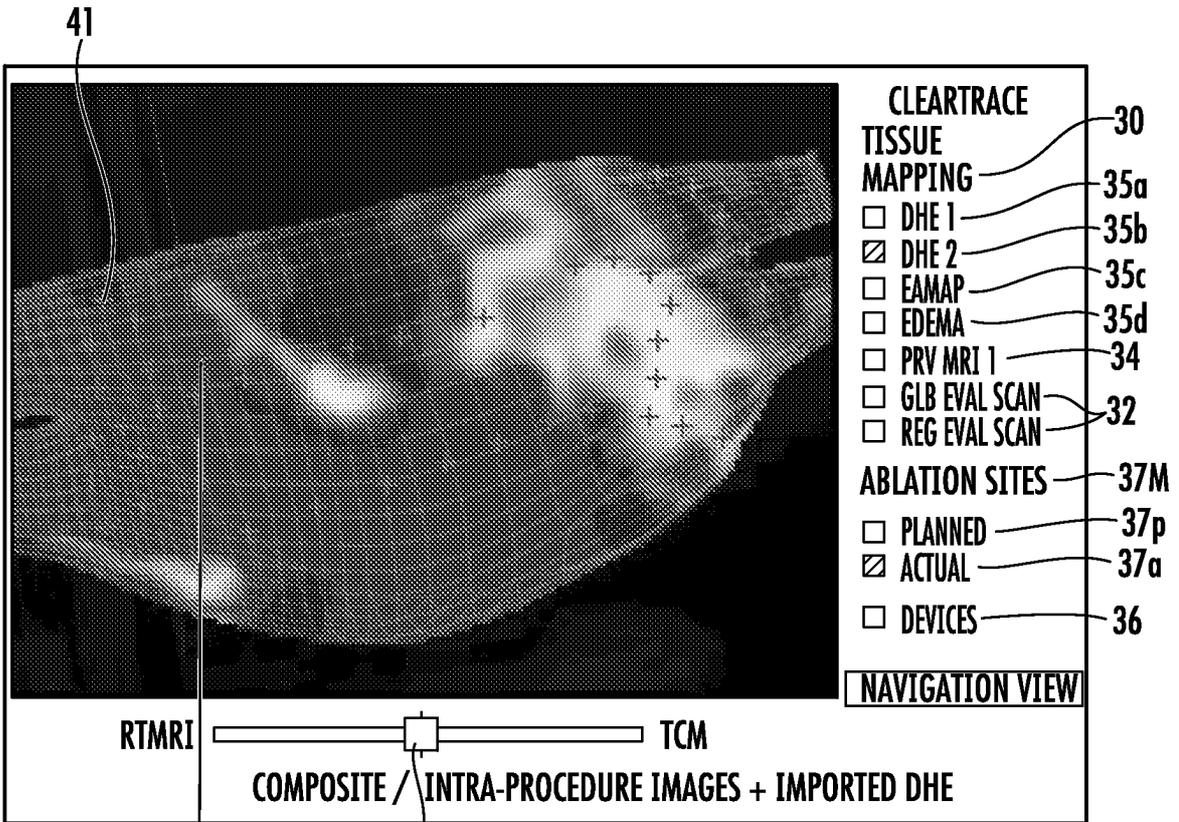

100M 25c **FIG. 27**

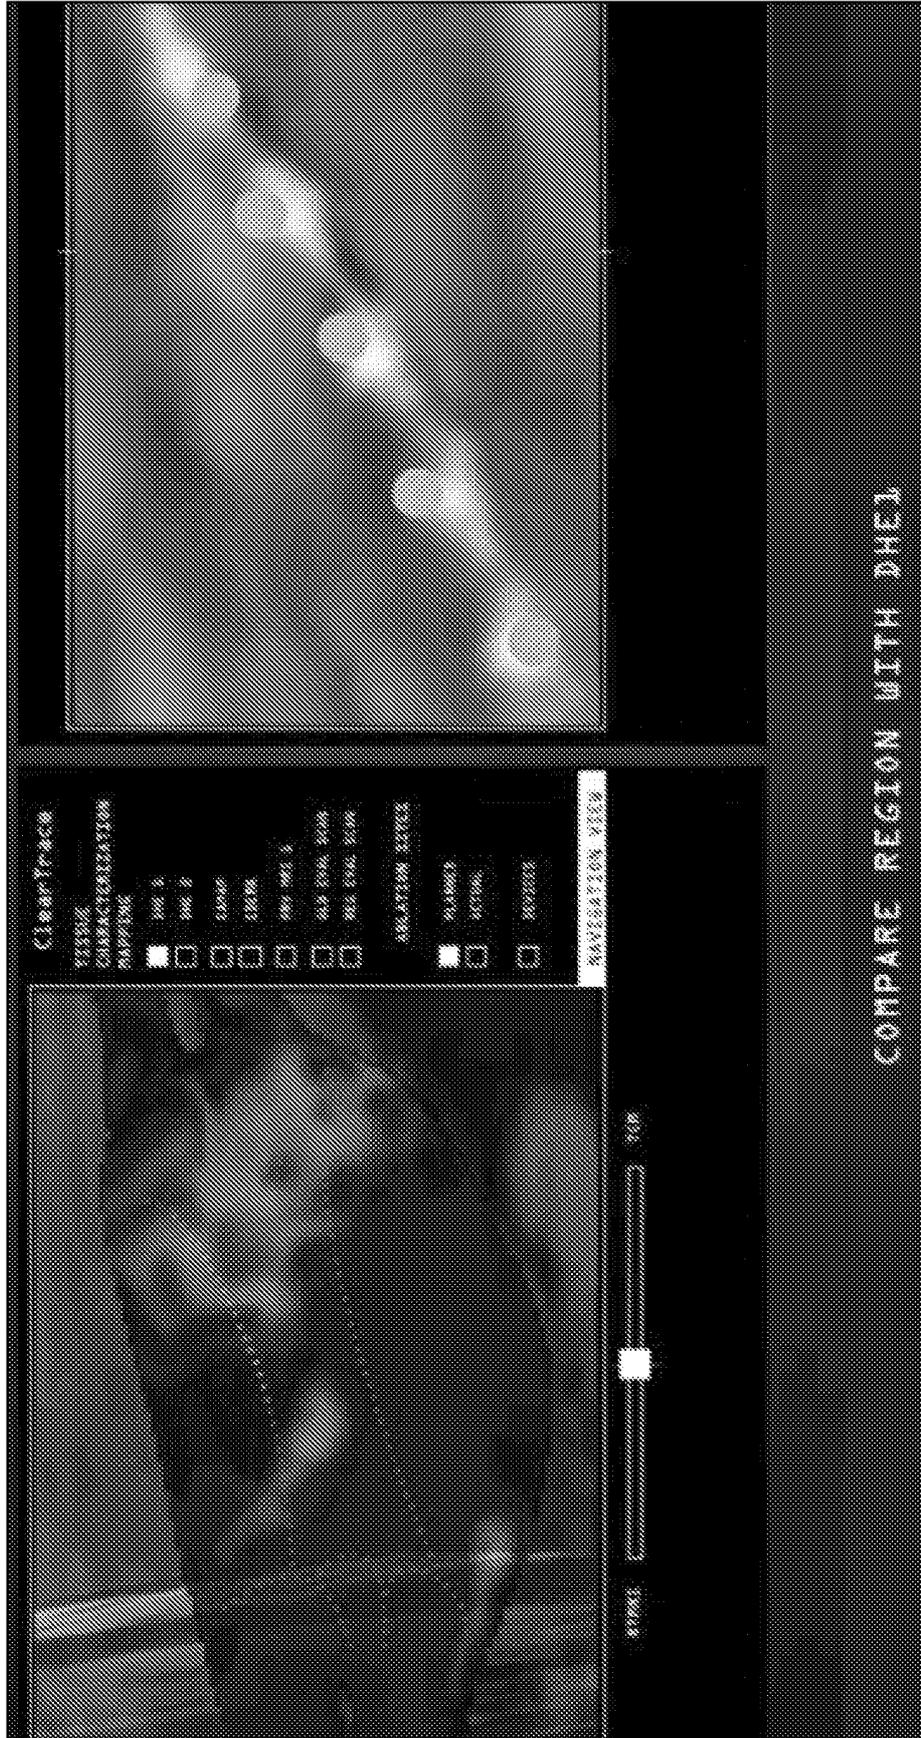
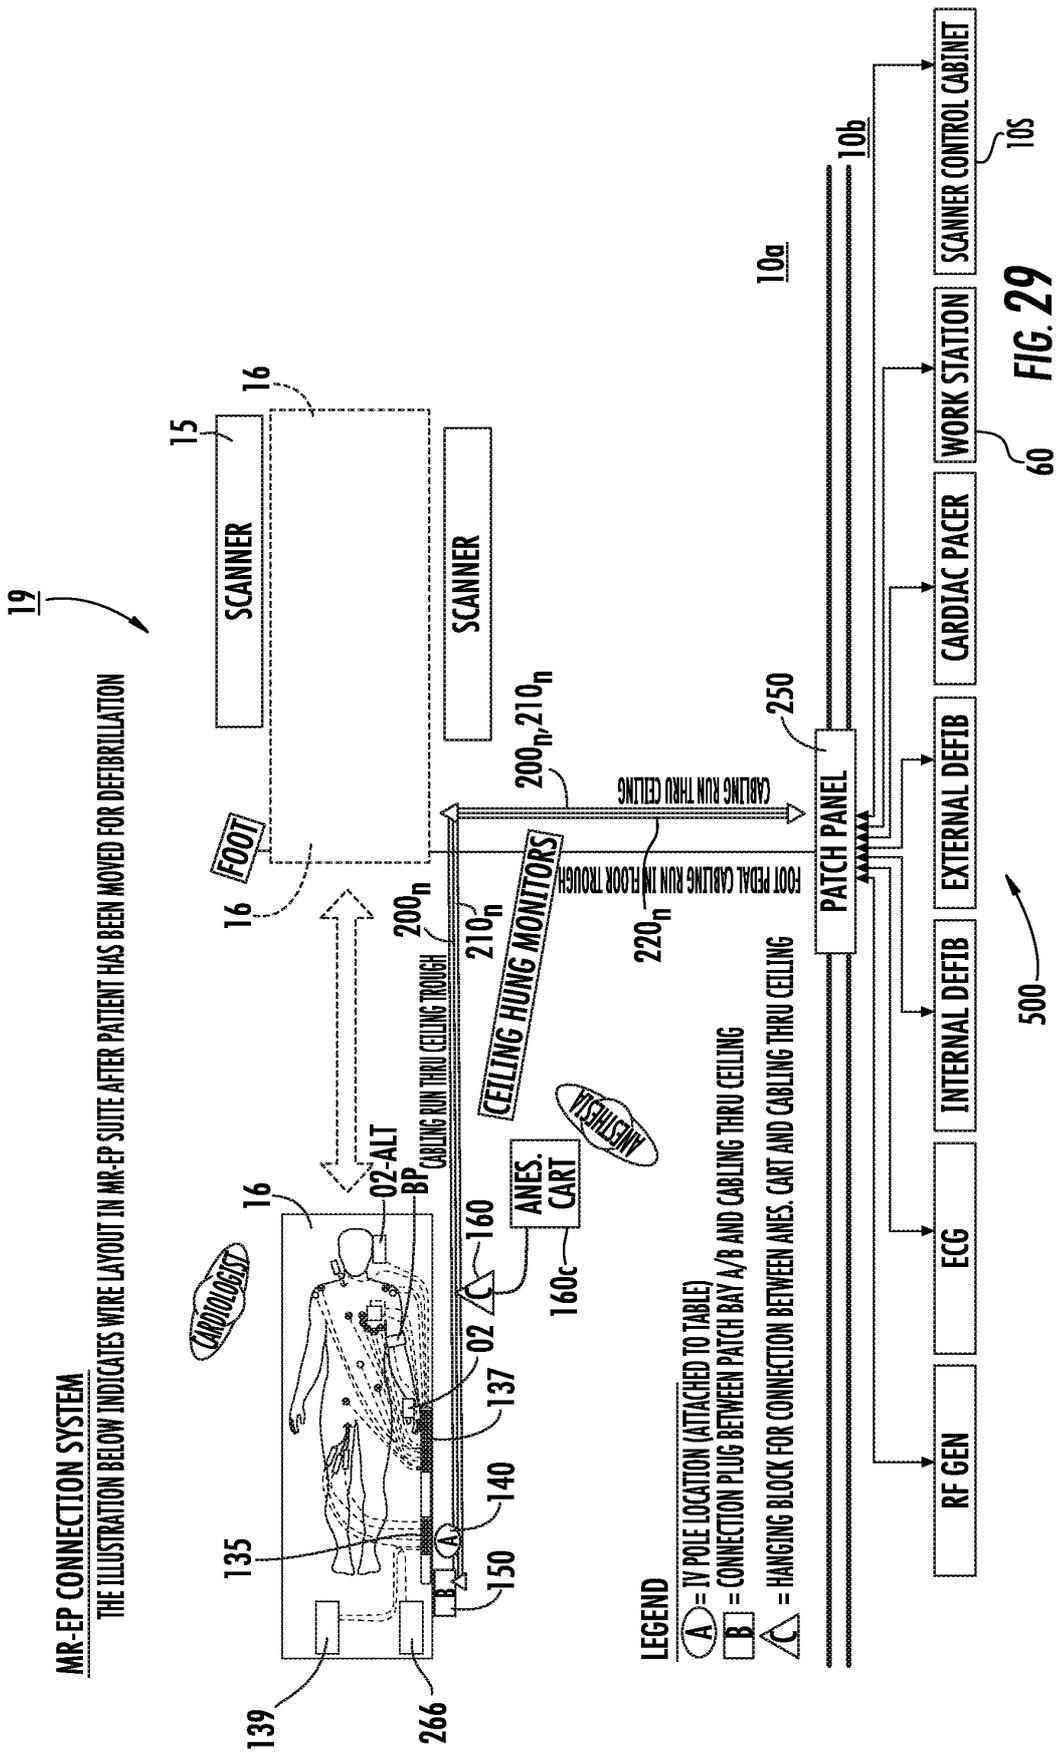
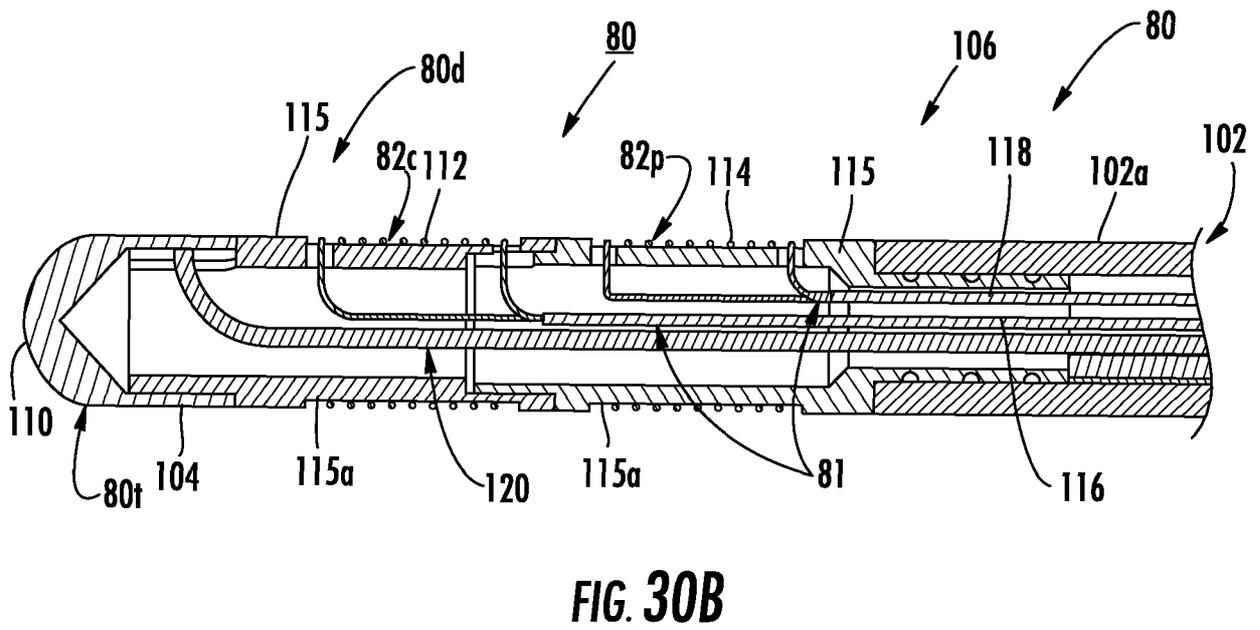
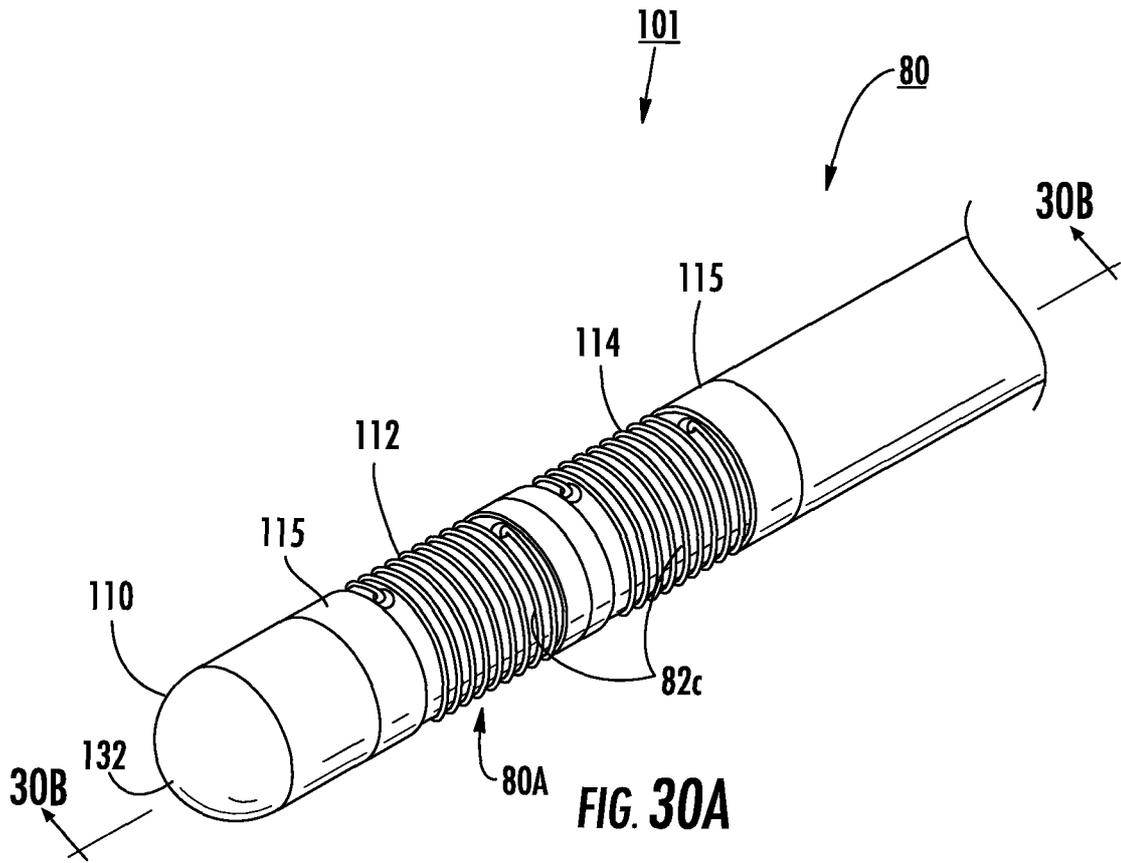


FIG. 28





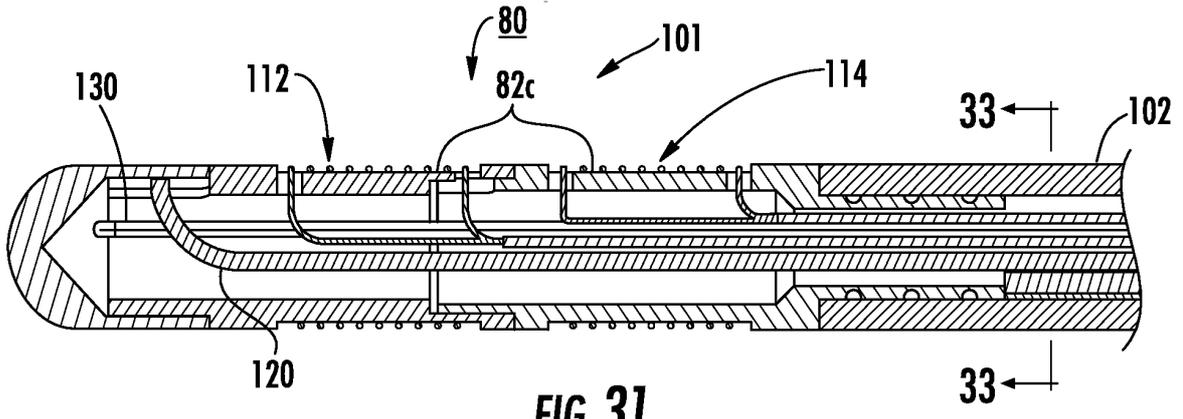


FIG. 31

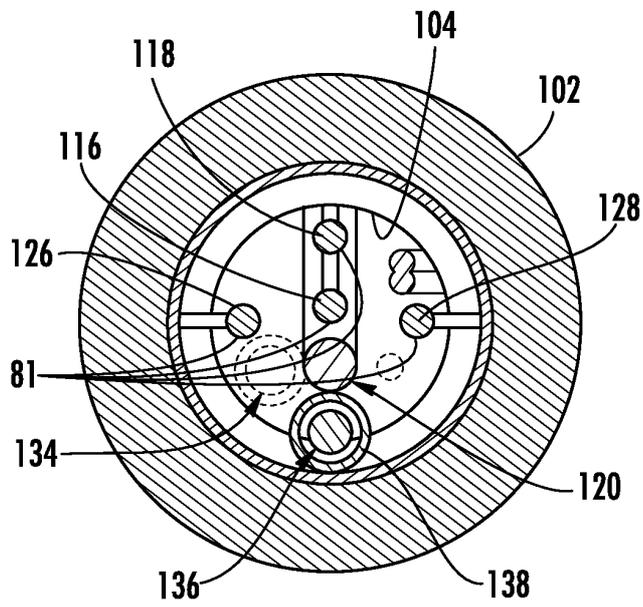


FIG. 32

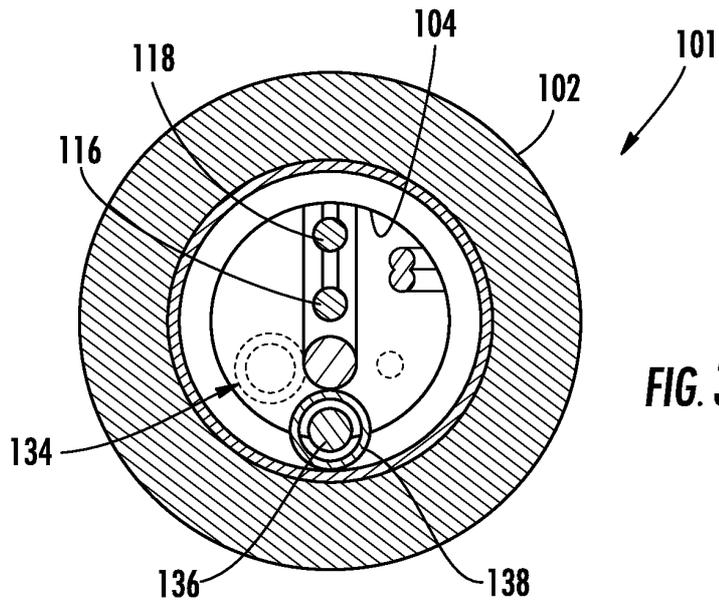


FIG. 33

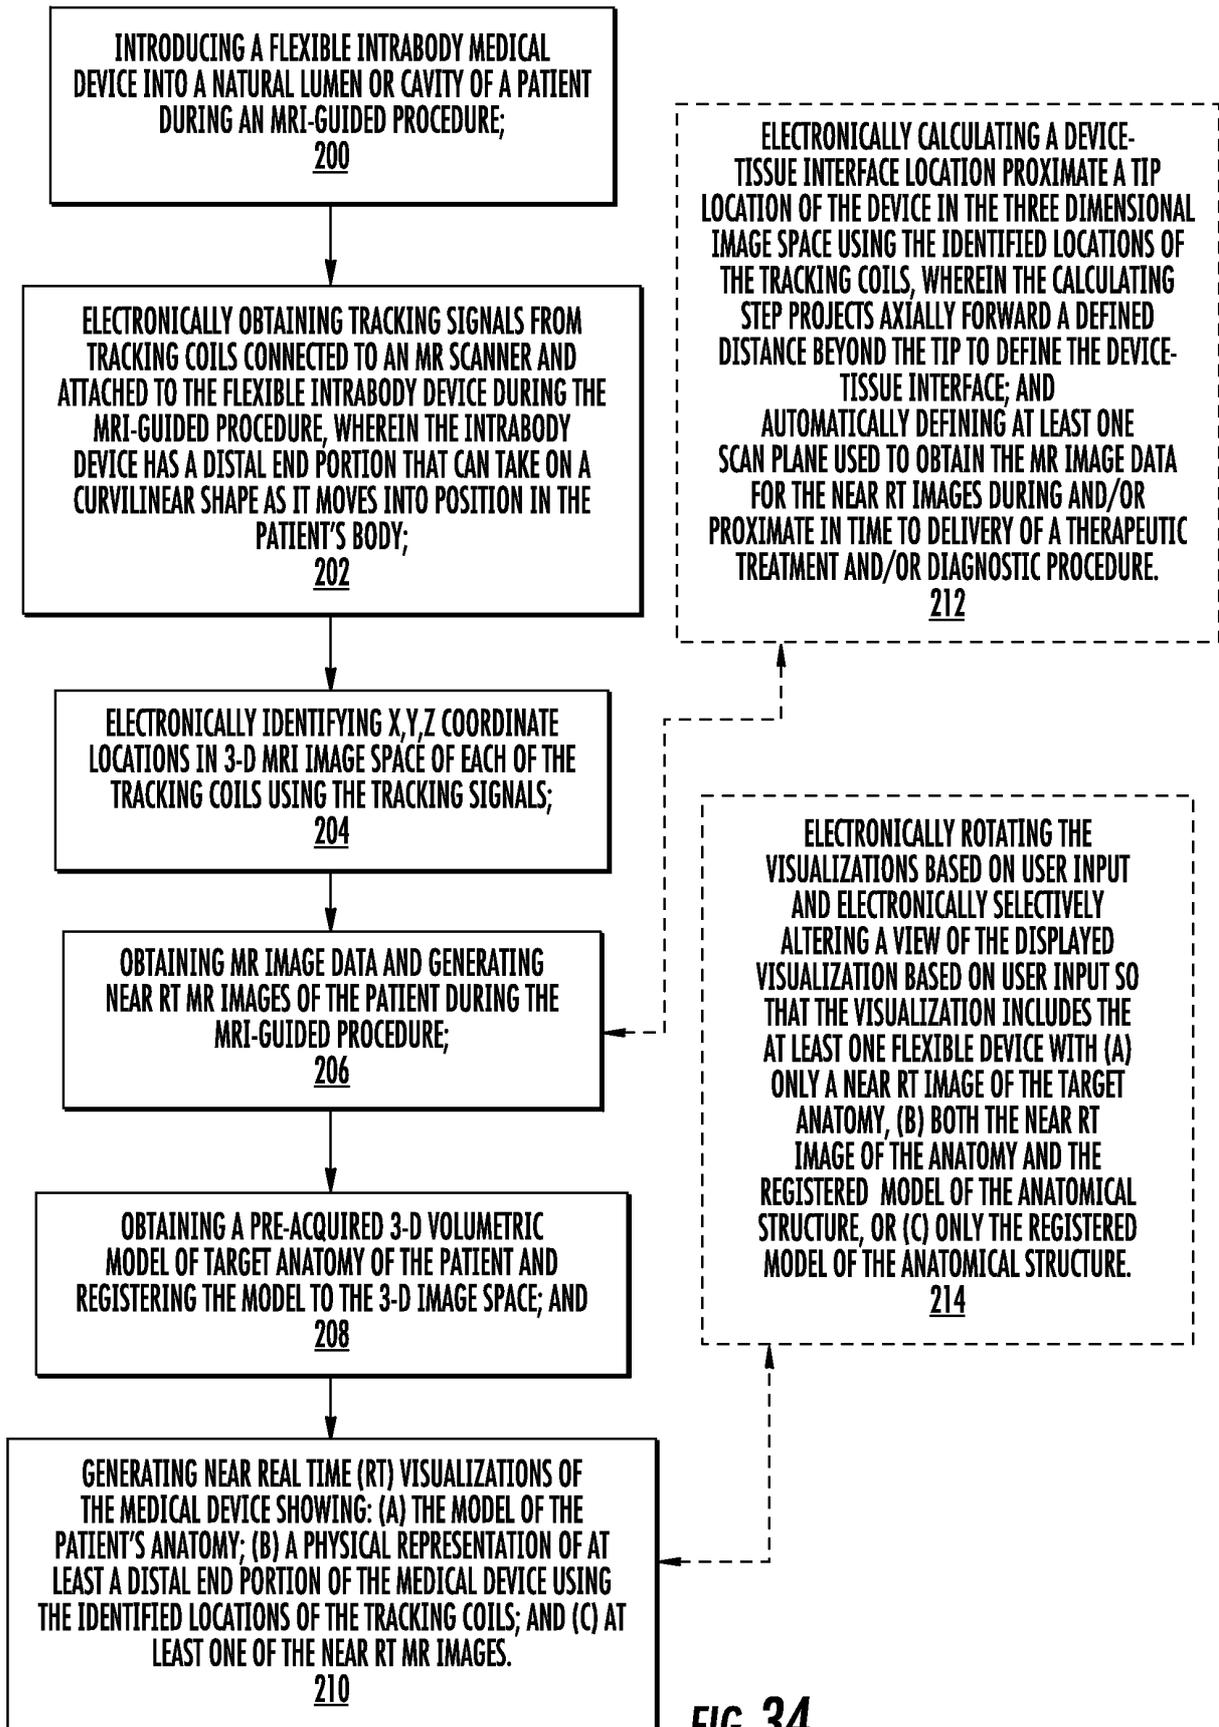
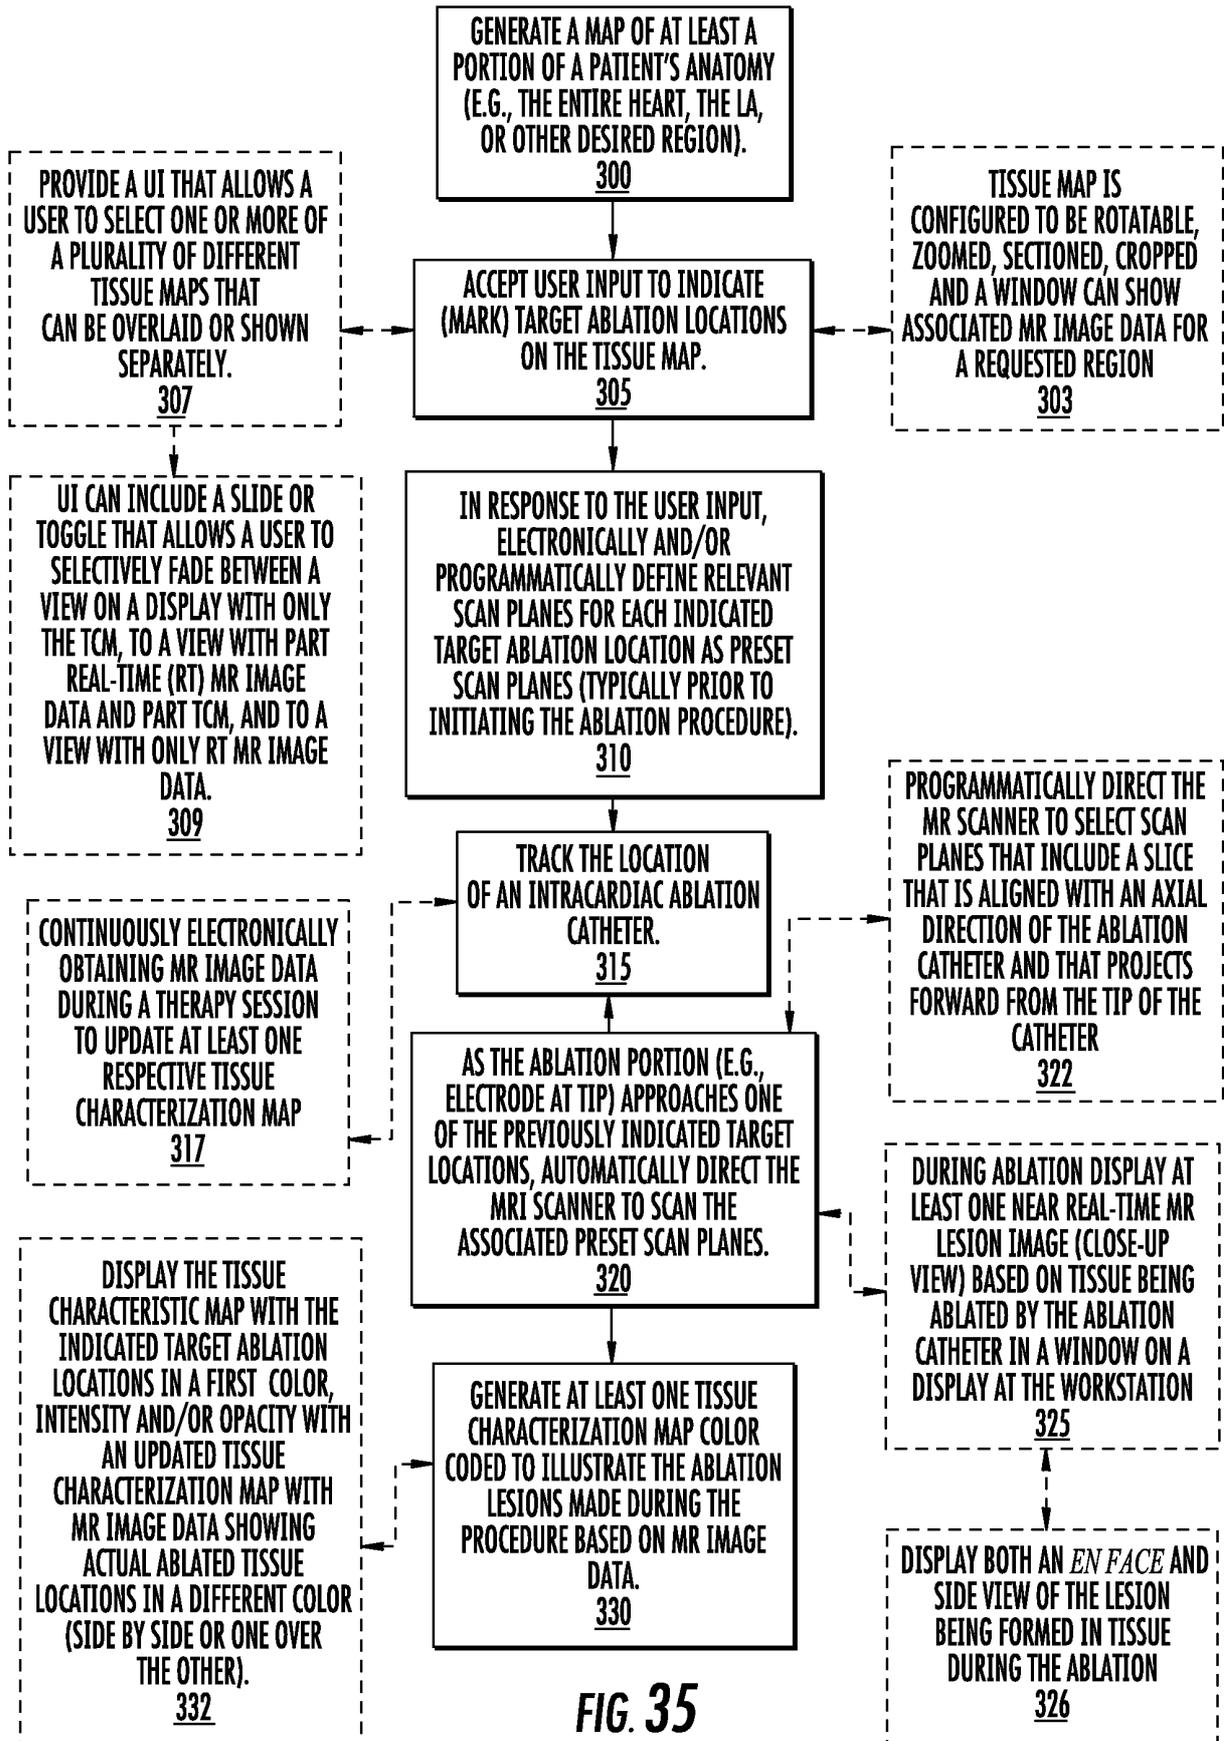


FIG. 34



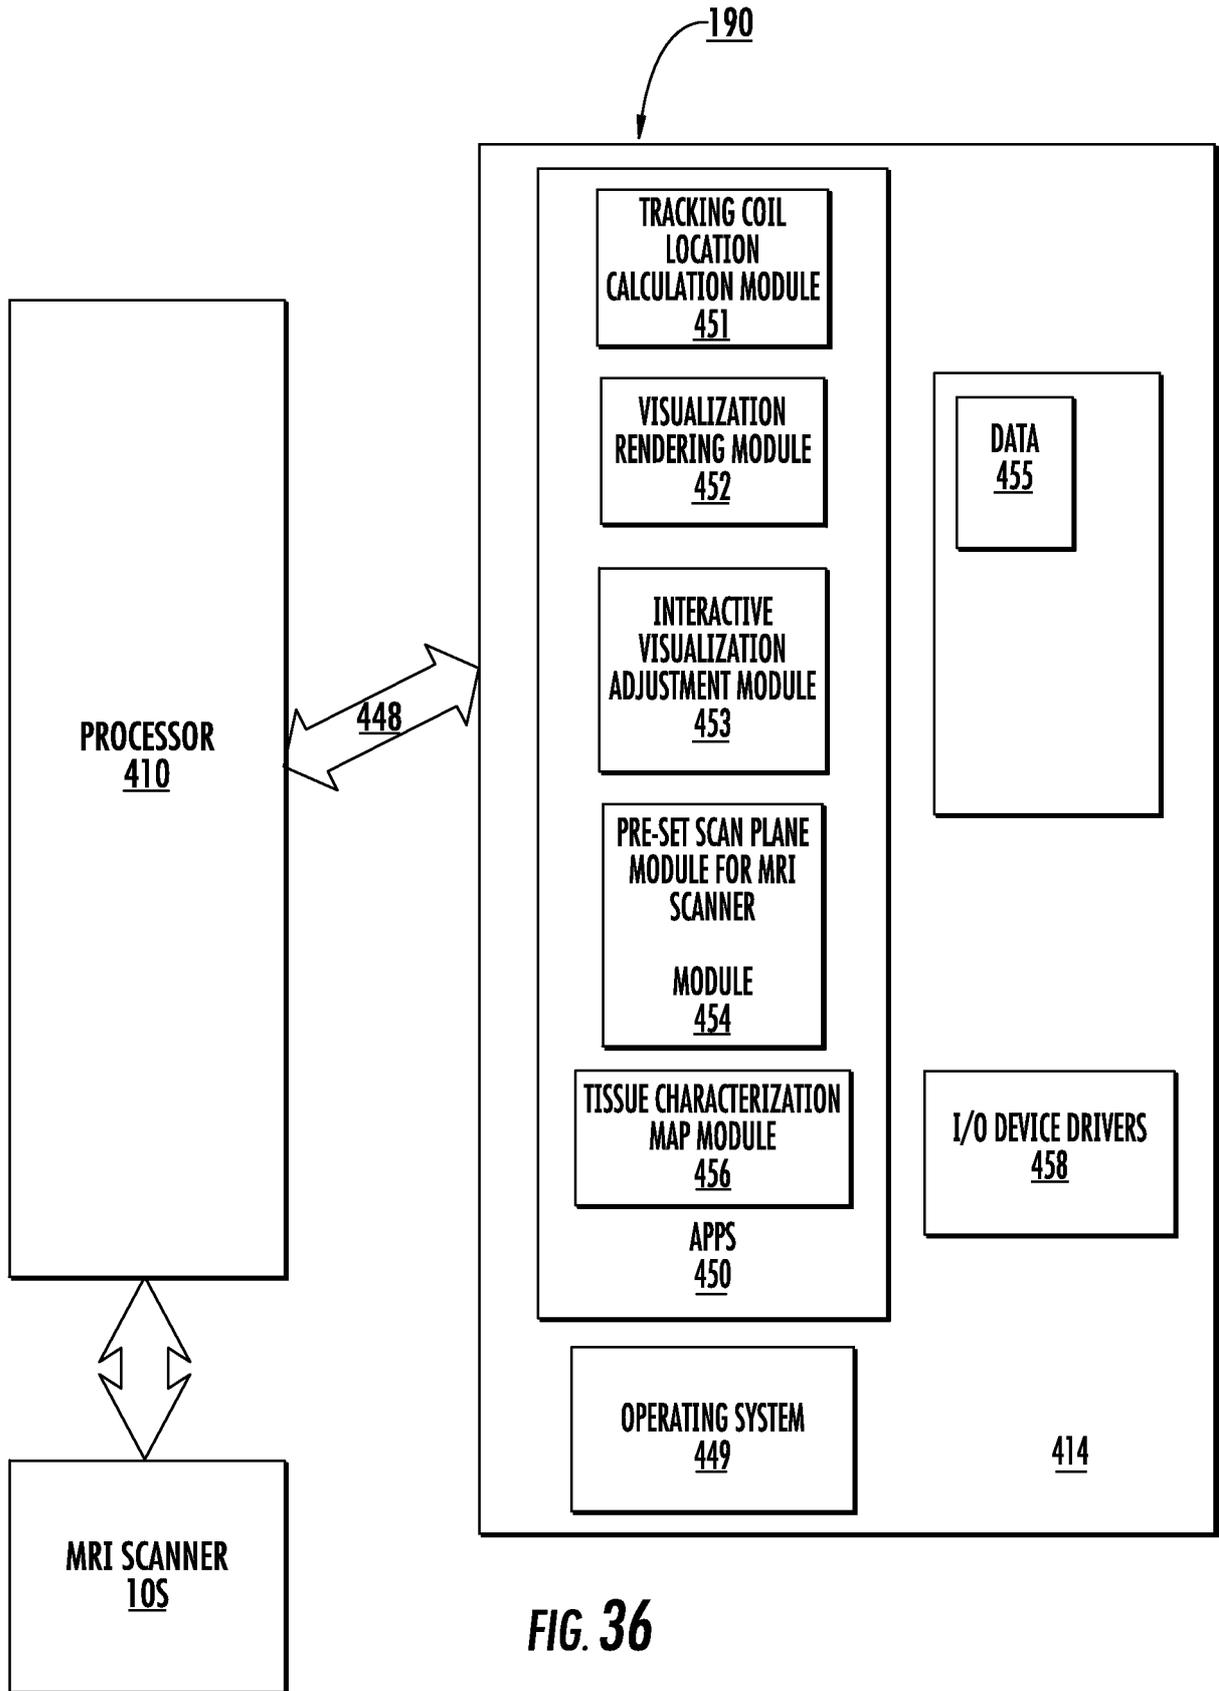


FIG. 36

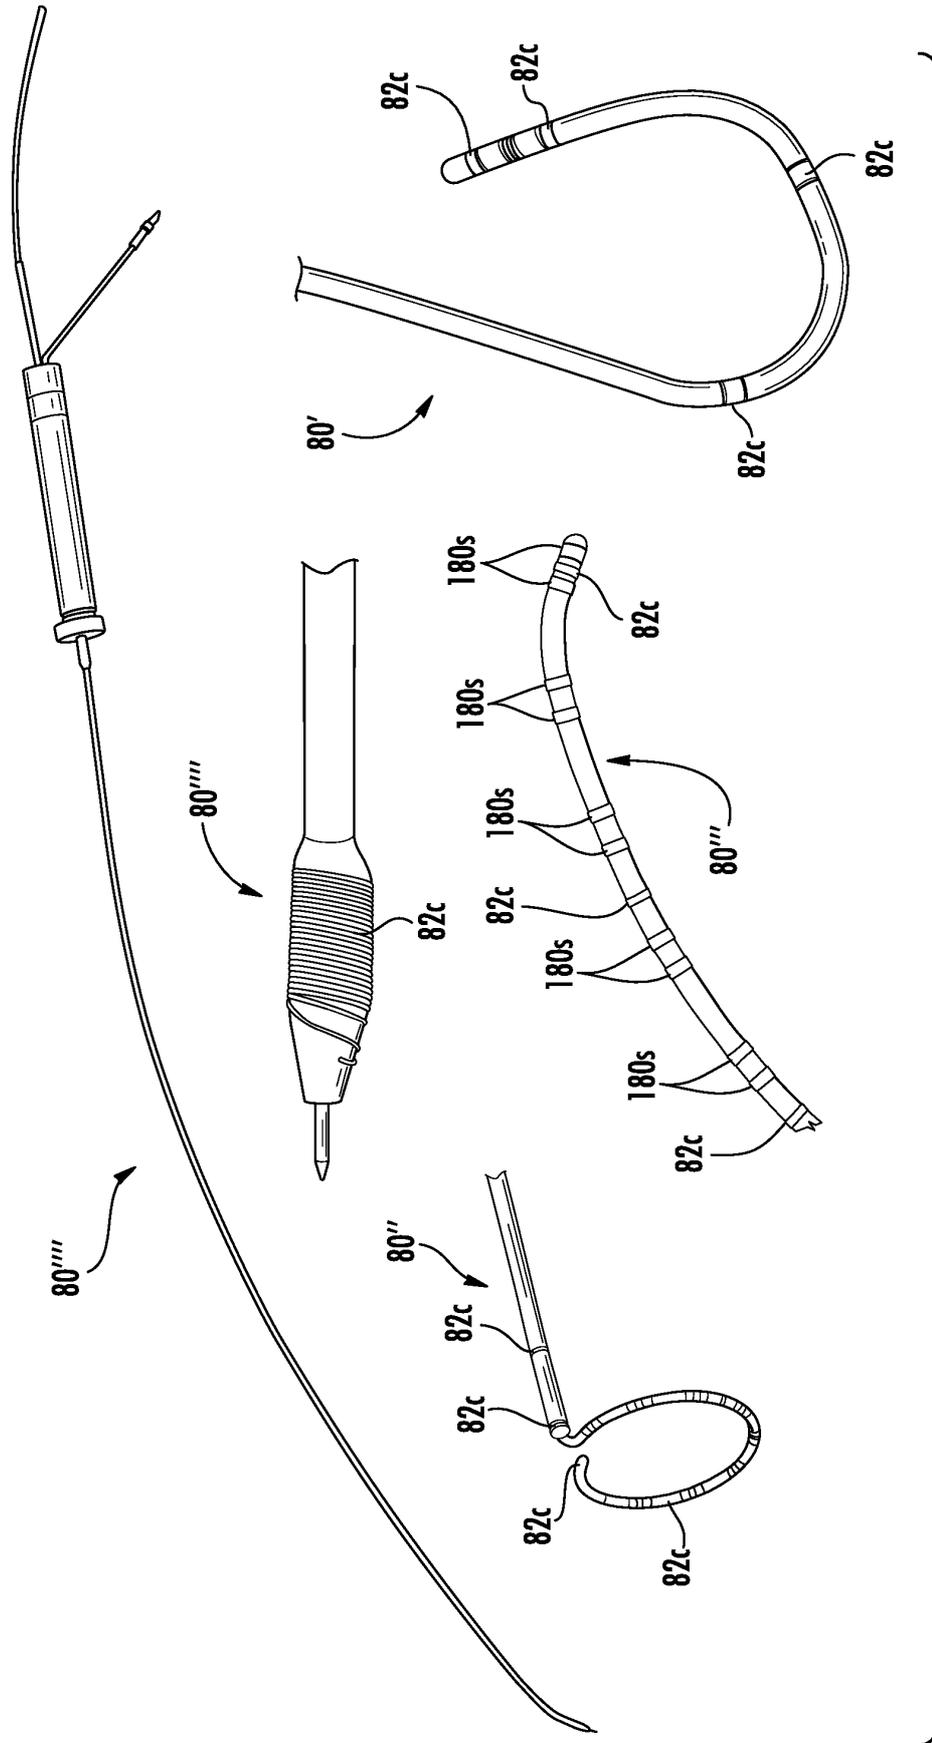


FIG. 37

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2005054910 A1, Tremblay [0003]
- US 769994 A [0052]
- US 7236816 B [0052]
- US 6606513 B [0052] [0148]
- US 6701176 B [0068] [0148] [0155]
- US 61261103 A [0068]
- US 708773 A [0124]
- US 6284971 B [0129] [0148] [0156]
- US 417594 A [0131] [0156]
- US 12047832 B [0131]
- US 12090583 B [0131] [0156]
- US 076882 A [0137]
- US 5699801 A [0148]
- US 5928145 A [0148]
- US 6263229 B [0148]
- US 6628980 B [0148]
- US 6675033 B [0148]
- US 20030050557 A [0148] [0155]
- US 20040046557 A [0148]
- US 20030028095 A [0148]
- US 6408202 B [0148]
- US 6904307 B [0155]
- US 12047602 B [0156]

Non-patent literature cited in the description

- **DICK et al.** Real Time MRI enables targeted injection of labeled stem cells to the border of recent porcine myocardial infarction based on functional and tissue characteristics. *Proc. Intl. Soc. Mag. Reson. Med.*, 2003, vol. 11, 365 [0060]
- **GUTTMAN et al.** Imaging of Myocardial Infarction for Diagnosis and Intervention Using Real-Time Interactive MRI Without ECG-Gating or Breath-Holding. *Mag. Reson. Med.*, 2004, vol. 52, 354-361 [0060]
- **DICK ; GUTTMAN et al.** Magnetic Resonance Fluoroscopy Allows Targeted Delivery of Mesenchymal Stem Cells to Infarct Borders in Swine. *Circulation*, 2003, vol. 108, 2899-2904 [0060]

专利名称(译)	MR控制的介入系统，用于实时跟踪和生成灵活的鼻腔内设备的动态可视化		
公开(公告)号	EP2440131B1	公开(公告)日	2018-04-04
申请号	EP2010786673	申请日	2010-06-08
[标]申请(专利权)人(译)	核磁共振成像介入技术有限公司		
申请(专利权)人(译)	MRI干预，INC.		
当前申请(专利权)人(译)	MRI干预，INC.		
[标]发明人	GUTTMAN MICHAEL JENKINS KIMBLE L PIFERI PETER VIJ KAMAL		
发明人	GUTTMAN, MICHAEL JENKINS, KIMBLE L. PIFERI, PETER VIJ, KAMAL		
IPC分类号	A61M25/01 A61B5/055 A61B5/00 G01R33/28 A61B34/10 A61B18/14 A61B17/00 A61B18/00 A61B34/00 A61B34/20 A61B90/00 A61M29/00 A61M25/00 A61M25/06 A61M25/09		
CPC分类号	A61B5/055 A61B5/415 A61B5/418 A61B18/1492 A61B34/10 A61B34/20 A61B34/25 A61B2017/00053 A61B2017/00243 A61B2018/00029 A61B2018/00839 A61B2018/1472 A61B2034/101 A61B2034/105 A61B2034/107 A61B2034/2051 A61B2034/252 A61B2090/374		
优先权	61/185072 2009-06-08 US 61/187323 2009-06-16 US 61/219638 2009-06-23 US 61/261103 2009-11-13 US		
其他公开文献	EP2440131A4 EP2440131A2		
外部链接	Espacenet		

摘要(译)

MRI引导的心脏介入系统被配置为在MRI引导的过程期间生成患者解剖结构和医疗装置的动态(交互式)可视化，并且还可以包括至少一个用户可选择的目标解剖结构的3-D体积(组织表征)图，例如，心脏的一个确定部分。

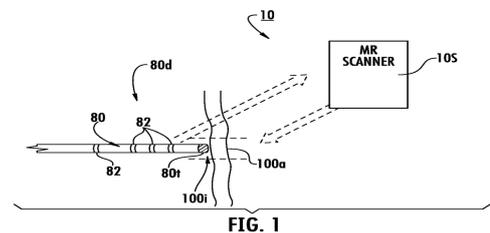


FIG. 1

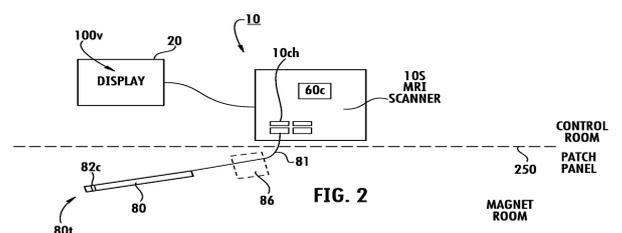


FIG. 2