

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
13 October 2011 (13.10.2011)

(10) International Publication Number
WO 2011/127063 A1

(51) International Patent Classification:
A61B 5/01 (2006.01)

(21) International Application Number:
PCT/US2011/031264

(22) International Filing Date:
5 April 2011 (05.04.2011)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/341,715 5 April 2010 (05.04.2010) US

(71) Applicant (for all designated States except US): **KAZ EUROPE SA** [CH/CH]; Chauderon 18, CH-1003 Lausanne (CH).

(72) Inventor; and

(75) Inventor/Applicant (for US only): **FRADEN, Jacob** [US/US]; 6250 Renaissance Avenue, San Diego, CA 92122 (US).

(74) Agents: **SIEGAL, Matthew, W.** et al.; Stroock & Stroock & Lavan LLP, 180 Maiden Lane, New York, NY 10038 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) Title: INSERTION DETECTOR FOR A MEDICAL PROBE

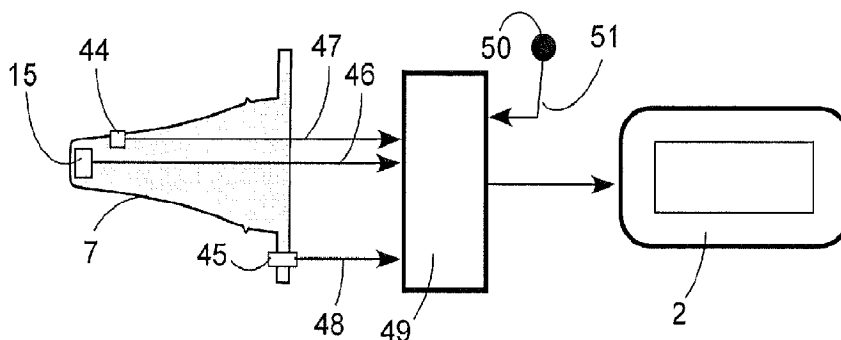


Fig. 11

(57) Abstract: An insertion detector for monitoring a position of a medical probe relative to a body cavity of a patient, the probe incorporates a proximity sensor that is responsive to a predetermined property of the patient's body. The proximity sensor may include a light emitter and a light detector. When the medical probe is inserted into the body cavity, a light flux between the light emitter and light detector is changed due to either obstruction by the cavity walls or reflection by the patient's skin. A response from the proximity sensor may be used to adjust a temperature measured from the body cavity to correct for errors due to non-insertion or partial insertion of the probe into the body cavity.

WO 2011/127063 A1

INSERTION DETECTOR FOR A MEDICAL PROBE

CROSS-REFERENCE TO RELATED APPLICATION

This application claims the priority of provisional U.S. patent application Serial No. 5 61/341,715 filed on 5 April, 2010, the disclosure of which is hereby incorporated by reference in its entirety.

FIELD OF THE INVENTION

The present invention relates generally to medical devices that use probes that come in close proximity to, or in contact with, a patient. More specifically, embodiments of the 10 invention relate to a device for detecting the insertion of the probe into a body cavity.

BACKGROUND OF THE INVENTION

A general body cavity medical probe may be inserted into the patient's body cavity for either measuring vital signs or for providing treatment. There are numerous type of general body cavity probes, such as a medical ear thermometer. General body cavity probes may 15 contain a functional module to perform the intended medical measurement or procedure. For a medical ear thermometer, the functional module may be an infrared ("IR") temperature sensor.

Temperature of an object, specifically of a living being such as a human or an animal, can be measured by thermal conduction or thermal radiation. For thermal conduction, a temperature sensing probe is brought into a physical contact with a surface of the living being. 20 For thermal radiation, a temperature sensing probe is brought near the surface of a the living being and aimed at the area of interest, such as within the open space of a body cavity. Naturally emanated electromagnetic radiation in the mid and far infrared spectral ranges is detected by an appropriate sensor, whose output signal indicates the surface temperature of an object. For both thermal conduction and thermal radiation measurement methods, the 25 temperature sensor is positioned inside or coupled to the medical probe.

Medical thermometers that operate by contact, for example, oral or rectal, may use a probe cover, for instance a sanitary probe cover. Thermal energy (i.e., heat) is transmitted

through the probe cover by thermal conduction, thus at least the portion of the probe cover material overlying the thermal sensor should be highly transmissive of thermal energy. Various conventional probe covers for contact thermometers are described in, for example, in U.S. Patent No. 4,159,766 issued to Kluge, which is hereby incorporated by reference in its entirety.

5 Medical thermometers that operate by radiation may also use a probe cover, because the possibility still exists of contact with the body of the patient. For example, when measuring the temperature of a tympanic membrane and the surrounding tissue inside the ear canal, the probe is inserted into the ear canal body cavity and may contact the wall of the ear canal. Before insertion, a probe cover may be installed onto the probe to envelop its parts that otherwise
10 might come in contact with the patient's skin. Such a cover provides sanitary protection against contamination of the probe by ear wax and other soiling biological compounds, and includes properties that promote accurate temperature measurement by the detection of infrared signal. Such properties include a good transparency of the front portion of the probe cover in at least the spectral range of interest, low directional distortion of optical rays, tight
15 manufacturing tolerances, stability of the optical properties during installation onto the probe, long term storage stability, etc. Probe covers for the IR thermometers are exemplified by U.S. Patent No. 5,088,834 issued to Howe et al. and U.S. Patent No. 5,163,418 issued to Fraden et al., both of which are hereby incorporated by reference in their entirety.

A probe cover may include one or more components such as polyethylene,
20 polypropylene, and copolymers thereof. Probe cover materials may also possess relatively low absorption of electromagnetic energy over a broad spectral range from visible to the far infrared.

Figure 1 is an example of a medical device having a probe intended for insertion into a body cavity, illustrating a perspective view of the infrared ear thermometer Model "Braun
25 4000" produced by Kaz, Inc., as known in the art. The example of FIG. 1 includes a thermometer body 1 having a display 2, a power button 3, a probe 7, a probe cover sensing switch 8, and a probe cover ejecting ring 5. Before measuring temperature, a reusable or disposable probe cover 6 is moved in a direction 12 to be positioned over probe 7. The probe cover has a skirt 9 and a groove 10. When installed onto probe 7, groove 10 engages with the

offset 11 that is part of the probe 7. This coupling will hold the probe cover 6 on the probe 7 during use. Skirt 9 actuates switch 8 to generate a signal going to the internal electronic circuit indicating a correct installation of the probe cover. If no probe cover is detected by the switch 8, the internal circuit may either warn the operator or make the thermometer inoperable to prevent an erroneous reading.

When a medical probe is used, either with or without a probe cover, it may be desirable to detect either a close proximity of the probe to the patient body surface, or to detect insertion of the probe into a body cavity, such as an ear canal. A shortcoming of the known art is that no medical thermometer has a capability of detecting the probe position relative to the ear canal. Therefore, a need exists to provide such a proximity measurement.

SUMMARY OF THE INVENTION

Embodiments of the invention relate generally to an apparatus and method for the proximity detection of a medical probe (e.g., a thermometer) to the surface of a living being. The embodiments should provide an accurate measurement, with or without the presence of a probe cover, by taking into account the detected proximity.

Therefore, as will be apparent from the foregoing description, embodiments of the invention include one or more of: a method or device for detection of the probe cover installation on a probe; a method or device for detecting proximity between the medical probe and a patient body surface; or a method or device to detect the insertion of a medical probe into the body cavity of a patient.

One or more embodiments of the invention provide a medical probe for insertion into a body cavity of a patient, such that the medical probe includes a probe body having a sidewall laterally circumscribing a longitudinal axis and enclosing an inner space, the sidewall having a proximal end and a distal end. Optionally, the distal end may be tapered relative to the proximal end. The medical probe also includes a sensor coupled to the probe to provide a signal relating to a condition of the body cavity of the patient, and a proximity sensor coupled to the probe, the proximity sensor configured to provide a signal indicating insertion of the probe into the body cavity. In some embodiments, the sensor may include a functional sensor

or a temperature sensor, and/or the sidewall may have an elongated shape adapted for insertion into an ear canal.

Optionally, the medical probe may be designed such that the proximity sensor includes an optical transmitter and an optical receiver positioned such that, when the medical probe is
5 positioned for insertion into the body cavity, the optical transmitter is positioned to transmit an optical signal toward an opening of the body cavity, including the edge thereof, and the optical receiver is positioned to receive the optical signal from the optical transmitter. The optical transmitter may be positioned to transmit toward a first position of the opening of the body cavity, and the optical receiver may be positioned to receive optical signals from a second
10 position of the opening of the body cavity.

As used throughout herein, for signals related at least to the proximity sensor, signals to or from the body cavity may include signals to or from portions of the patient adjacent to the body cavity, including wall portions and/or edge portions of the cavity.

Optionally, the transmitter may have a first optical axis, and the optical receiver may
15 have a second optical axis.

In another embodiment, the proximity sensor may further include a receiving light guide disposed within the inner space, the receiving light guide having a first end coupled to and protruding through the distal end of the sidewall, and a second end coupled to the optical receiver. Optionally, the receiving light guide may protrude through the distal end of the
20 sidewall at an angle that is pointed away from the proximal end of the sidewall.

In another embodiment, the proximity sensor may further include a transmitting light guide disposed within the inner space, the transmitting light guide having a first end coupled to and protruding through the distal end of the sidewall, and a second end coupled to the optical transmitter. Optionally, the transmitting light guide may protrude through the distal end of the
25 sidewall at an angle that is pointed away from the proximal end of the sidewall.

Optionally, the proximity sensor may include a translucent opto-coupler that protrudes through the sidewall, the opto-coupler including a first side disposed within the inner space, the first side being optically coupled to a light emitter and a light detector; and the opto-coupler

further including a second side disposed outside the inner space, wherein the second side protrudes through the wall of the probe.

In some embodiments, the medical probe may further include an electronic circuit coupled to the sensor and to the proximity sensor, the electronic circuit including a processor and a memory coupled to the processor, the memory storing software, such that the software, when executed by the processor, is configured to execute an algorithm to process signals from the sensor and the proximity sensor. The electronic circuit may further include an output device coupled to the processor, the output device configured to output a result of the algorithm.

The medical probe may further include an ambient temperature sensor electrically coupled to the electronic circuit and positioned outside of the inner space, such that the software, when executed by the processor, is further configured to execute an algorithm to process signals from the sensor, the proximity sensor and the ambient temperature sensor.

In one or more embodiments, the medical probe may be designed such that at least one of the transmitting light guide and receiving light guide comprises a plastic optical fiber. Alternatively, at least one of the transmitting light guide and receiving light guide includes a glass rod, or a polycarbonate rod. Optionally, at least one of the transmitting light guide and receiving light guide may include a rod coated with a coating material, wherein a refractive index of the coating material is lower than a refractive index of the rod. Optionally, the first end of at least one of the transmitting light guide and receiving light guide may include a lensing bulb. Optionally, an optical barrier may be disposed in the inner space between the optical transmitter and optical receiver. Optionally, the optical receiver is disposed within the inner space.

In one or more embodiments of the invention, the proximity sensor may operate by use of ultrasonic signals.

One or more embodiments of the invention provides a method for detecting an insertion of a medical probe into a body cavity of a patient, including the steps of: transmitting, from a transmitter, a signal toward an edge portion of the body cavity; receiving, at a receiver, a return

signal from an edge portion of the body cavity; and monitoring a flux of the return signal for a drop in strength, such that a path from the transmitter to the receiver is blocked when the medical probe is inserted into the body cavity such that the flux of the return signal decreases when the medical probe is inserted into the body cavity.

5 In another embodiment of a method for detecting an insertion of a medical probe, the medical probe having a longitudinal axis, into a body cavity of a patient along the longitudinal axis, the method includes the steps of: transmitting a signal along a first direction substantially perpendicular to the longitudinal axis; receiving a return signal from a second direction, the second direction substantially parallel to the first direction; and monitoring a flux of the return
10 signal for an increase in strength, such that the flux of the return signal increases in strength above a predetermined threshold when the medical probe is inserted into the body cavity.

 In another embodiment of a method of displaying the temperature of a body cavity of a living being, the method includes the steps of: measuring a base temperature of the cavity by use of a temperature sensor; measuring a proximity of the temperature sensor to the body
15 cavity; measuring an ambient temperature in an area adjacent to the temperature sensor; computing a computed temperature of the body cavity in accord with a predetermined function of the base temperature, the proximity, and the ambient temperature; and displaying the computed temperature.

 Optionally, the method may further detect the presence of a probe cover, and adjust the
20 computed temperature accordingly.

 Still other objects and advantages of the invention will in part be obvious and will in part be apparent from the specification. The invention accordingly includes the features of construction, combination of elements, and arrangement of parts which will be exemplified in the construction hereinafter set forth as well as the methods of construction and applying the
25 adhesive discussed herein, and the scope of the invention will be indicated in the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

 The above and still further objects, features and advantages of the present invention will become apparent upon consideration of the following detailed description of a specific

embodiment thereof, especially when taken in conjunction with the accompanying drawings wherein like reference numerals in the various figures are utilized to designate like components, and wherein:

Fig. 1 illustrates a perspective view of an ear thermometer as known in the art;

5 Fig. 2 illustrates a cross-sectional view of a probe having an optical proximity sensor when the probe is not inserted into the body cavity, according to an embodiment of the invention;

Fig. 3 illustrates a cross-sectional view of the probe having a proximity sensor when the probe is inserted into the body cavity, according to an embodiment of the invention;

10 Fig. 4 illustrates a cross-sectional view of the probe with a light conductive rod, according to an embodiment of the invention;

Fig. 5 illustrates a cross-sectional view of the probe with two light conductive rods, according to an embodiment of the invention;

15 Fig. 6 illustrates a cross-sectional view of the probe cover walls situated away from ear canal skin, according to an embodiment of the invention;

Fig. 7 illustrates a cross-sectional view of an effect of the probe cover pressing by the ear canal wall, according to an embodiment of the invention;

Fig. 8 is a timing diagram of the light flux at the light detector, according to an embodiment of the invention;

20 Fig. 9 illustrates a cross-sectional view of a probe with a single-mode light pipe, according to an embodiment of the invention;

Fig. 10 illustrates a cross-sectional view of a probe with a dual-mode light pipe, according to an embodiment of the invention; and

25 Fig. 11 illustrates a simplified block-diagram of an IR thermometer, according to an embodiment of the invention.

DETAILED DESCRIPTION

Embodiments of the invention achieve their objectives by adding a proximity sensor to a medical probe that may be coupled to a functional module. An example of a functional module is a temperature sensor (i.e., thermometer). The proximity sensor may be a combination of a light emitter and a light detector. In one embodiment, the light emitter and light detector are optically coupled to one another when the probe is positioned near to, but outside of the patient body cavity. However, when the probe is inserted into a body cavity, such as an ear canal, the optical coupling is modified and sensed by the light detector. In another embodiment, the light emitter and light detector are not substantially optically coupled to one another when the probe is positioned near to, but outside of the patient body cavity. However, when the probe is inserted into a body cavity, such as an ear canal, the optical coupling is modified and sensed by the light detector.

An output signal from the proximity sensor may be used by a calculation algorithm executed by a microcontroller in the medical device, for instance by adjusting a calculated and displayed temperature reading based upon measurements provided by the temperature sensor, the proximity sensor, and optionally an ambient air temperature measurement. For example, because the IR signal indicative of temperature is different when measured from the inside or outside of the ear canal, the temperature that is sent to a user display may be adjusted to account for the differing measurement positions as sensed by the proximity sensor. Alternatively, the operator may be warned about an incorrect probe position (e.g., when outside of the ear canal), or the temperature measuring and displaying process may be disabled until the medical probe is in the desired position (e.g., inside the ear canal). A display of such a warning may include a light (e.g., a red LED), an icon on an LCD panel, an audible signal (e.g., a beep or buzz), a vibration, or any combination thereof.

Some probes intended for insertion into a body cavity employ reusable or disposable probe covers. A probe cover for a medical probe is a sanitary envelope that forms a barrier between the instrument and the patient. For example, a probe cover may be coupled to an IR thermometer that is adapted to take temperature in an ear canal of a human or animal. Similar covers are applicable for use with any other body cavity or skin surface of a human or animal.

Generally, the material for an infrared thermometer probe cover is selected from the group of polymers which have significant transparency in the mid and far infrared range between 3 μm and 15 μm . The same material also has a range of light transmission (about 20% to about 90%) near and below the wavelength of 1 μm , that is in the visible and near-infrared spectral ranges.

5 Examples of the polymers are polyethylene, polypropylene, and copolymers of such. Thus, installed probe cover presents little attenuation to light over a broad spectral range.

Figure 2 shows a cross-sectional view of the probe 7 enveloped by the probe cover 6. The probe 7 is hollow inside, that is, it has an inner space. A longitudinal axis 24 is formed through the center of the probe 7. The probe 7 has a distal end 52 and proximal end 53. At the proximal end 53, there is a proximity sensor that includes a light emitter 19 and light detector 21. The emitter and detector preferably operate in a near-infrared spectral range.

10

Figure 2 illustrates probe 7 poised for insertion into the body cavity 35, in particular an ear canal. Light beam 36 emitted by the emitter 19 propagates along a direction toward area 37, and subsequently area 38, which are parts of the edge of the body cavity 35. Light beam 4 is reflected from area 37 toward area 38 and subsequently toward light detector 39 as a light beam 39. As long as probe cover 6 is substantially transparent to the light used by the proximity sensor, emitter 19 and detector 21 may be positioned behind the skirt 9 without a substantial loss in light intensity. The light level that is detected by the detector 21 when the probe cover 6 is placed over probe 7, with probe 7 being positioned away from body cavity 35, is measured and stored as a reference in an electronic circuit (described later) that may be connected to the detector 21. Intensity of light detected by detector 21 during insertion of probe 7 will be compared to the reference level. When the probe 7 is inserted into the body cavity 35, it substantially blocks reflection 4 so very little light reaches area 38. Blockage of reflection 4 is illustrated in Fig. 3. As a result, intensity of the light beam 39 is modified, that is the light is significantly reduced. The lower light intensity is detected by the detector 21 and sent to the electronic circuit that compares it with the stored reference. The circuit interprets the light reduction as an indication of the probe insertion into the ear canal.

15

20

25

Fig 4 depicts another embodiment of the optical proximity sensor. It includes a light transmitting first rod 17 positioned in the probe 7 inner space 14 and coupled to the light

detector 21. The rod 17 functions as a light guide, providing a low optical loss to light detector 21. The distal portion 20 of the probe 7 incorporates the IR sensor 15 that is connected to the external circuit by conductors 16. A distal end of the first rod 17 includes a first bulb 18 that protrudes through the probe wall 26. The bulb receives light reflected from the ear canal area 5 38. A proximal end of the rod 17 is optically coupled to the light detector 21. This embodiment has a better noise immunity because of a closer proximity between the first bulb 18 and the skin area 38.

The first rod 17 is fabricated of a material having high transparency in the wavelength used by the proximity sensor. Examples of such a material are glass and polycarbonate.

10 A further improvement in noise reduction and sensitivity is achieved when the emitting part of the optical proximity sensor is also moved toward the distal portion 20 of the probe 7 as illustrated in Fig. 5. A light transmitting second rod 40 is placed inside the probe 7. The rod 40 also functions as a light guide. Alternatively, a flexible plastic optical fiber light pipe may provide the light guide function rather than rod 40. Rod 40 ends with a second bulb 41 that 15 protrudes through the probe wall. Note that bulb 41 and bulb 18 are shaped to tend to maximize the flux of light emanated or received to/from areas 37 and 38, respectively. In other words, bulb 41 and bulb 18 should have lensing properties. To minimize optical coupling between the rods 17 and 40, a light barrier 42 may be positioned in between. The barrier 42 is a layer of an opaque material, such as metal, plastic or paper. To reduce light loss, rods 17 and 20 40 may be coated with a material having a refractive index lower than that of the rod material. For example, if the rods are made of borosilicate glass, the coatings may be fused silica. However, no coating should be applied onto the bulbs 18 and 41. The bulbs should have smooth slightly convex surfaces. The junctions of rod 40 with bulb 41, and rod 17 with bulb 18, are not limited to the shape shown in the figures, but may be shaped to reduce optical 25 losses.

Fig. 6 illustrates the first bulb 18 in contact with the probe cover wall 22. Note that light beam 32 passes through the probe cover wall 22 and at the point of contact 23 enters the first bulb 18 and further propagates along the rod 17 as the beam 33. Figure 7 illustrates that when the probe 7 is inserted into the ear canal, the ear canal walls 30 obstruct the entry contact

23 and the light beam 32 either disappears or becomes very weak.

Figure 8 illustrates an optical flux signature, showing a change in intensity over time at detector 21 as a probe is inserted into and removed from an ear canal. Before the probe cover is installed and the probe is far away from the patient skin, the detected light is very small.

5 Installation of a probe cover provides a weak but detectable coupling between the emitter 19 and detector 21 causing the light intensity to increase slightly. This phenomenon may be used by the electronic circuit as a manifestation of the probe cover installation. When the probe is brought into vicinity of the entrance to the ear canal, light is reflected more greatly from the skin and reaches its maximum when the probe tip is at the entrance. This is a manifestation of

10 the probe being just at the opening of the ear canal and that light magnitude may be used by the electronic circuit as a manifestation of the probe being at the entrance of the ear canal. When the probe is inserted into the ear canal, the optical obstruction by the ear canal walls causes the light intensity dropping to a very low level. This is a manifestation of the probe insertion. When the probe is being removed and while passing near the entrance to the ear canal, the light

15 magnitude again jumps to the highest level and when the probe is moved away from the body, light drops again to a low level. This sequence of modulation of the light intensity is interpreted by the electronic circuit as various positions of the probe with respect to the body cavity.

It should be clearly understood that there can be a multitude of optical arrangements for

20 monitoring a proximity between the probe and the body cavity. One practical embodiment is illustrated in Fig. 9 where the light detected is positioned on a circuit board 60 that is installed in an empty space 14 inside the probe 7. The light detector 21 is coupled to the outside of the probe 7 by a short (2-5 mm) light guide 61 that is fabricated of a clear material like glass or polycarbonate. Just as in the above-described embodiments, light intensity at the light guide 61

25 depends on its proximity to the ear canal wall 30. The light is partially or completely dimmed when the wall, 30, is pressed against the light guide 61 as shown in Fig. 9. This light guide 61 is called a “single-mode” light guide because it operates in one mode – receiving the incoming light from emitter 19.

A “dual-mode” mode light guide (opto-coupler) 43 is shown in Fig. 10 where both the

light emitter 19 and light detector 21 are positioned on a circuit board 60 in a mutually adjacent position. They are optically coupled to the opto-coupler 62 at its first side 55 while its second side 56 protruded through the probe wall 26. This opto-coupler 62 works for the light going out and coming in. Obviously, when the probe 7 is away from the patient skin, a baseline
5 optical coupling exists between the light emitter 19 and detector 21 and that baseline shall be stored in the electronic circuit for future reference. A light modulation in a dual-mode light guide 62 is different from a single-mode light modulation. Specifically, for a dual-mode light guide (opto-coupler), the light intensity becomes strongest when the probe 7 is inserted into the ear canal, it is of a medium value when the probe 7 is at the entrance of the ear canal and drops
10 down close to the baseline (previously stored in the electronic circuit) when the probe 7 is removed away from the patient.

To reduce possible interferences from ambient illumination and lower power consumption, the light emitter 19 preferably should be used in a pulsing mode. Then, the output from detector 21 should be gated to remove a d.c. component that is associated with the
15 ambient illumination. These functions are performed by the electronic circuit and are of a conventional nature well known in the art.

Regardless of the actual embodiment, the light intensity is generally modulated by three external factors: installation of the probe cover, proximity to the ear canal and insertion into the ear canal. Obviously, proximity sensors of the above embodiments are not the only possible
20 way of detecting insertion of the probe into an ear canal. Other embodiments of proximity sensors may be designed by employing physical effects of capacitance, ultrasonic and other couplings between the probe and ear canal walls. Since the coupling changes while the probe is being inserted into an ear canal, the proximity sensor responds with a change in the corresponding signal.

25 A proximity sensor generates a signal that is used by the electronic circuit for modifying operation of the medical device. Fig. 11 illustrates a simplified block-diagram of an IR ear thermometer having a probe 7, electronic circuit 49 and an output device which is the display 2. The probe 7 incorporates the IR sensor 15 for measuring a raw patient temperature, proximity sensor 44 and probe installation sensor 45. The raw patient temperature may be used as a base

temperature for further computations. These components are coupled to the electronic circuit 49 via respective conductors 46, 47, and 48. There is also an ambient temperature sensor 50 that sends its output signal to the circuit 49 via conductor 51. The ambient sensor 50 is positioned outside of the probe 7. The circuit 49 processes all signals according to the pre-programmed algorithm and sends a computed temperature number to display 2. The initial temperature T_B is computed by the circuit 49 from the signals received from the IR sensor 15 and probe installation sensor 45 (to correct for the probe cover IR transmission factor). The signal processing and temperature computation algorithms are well known to a person of skill in the art.

10 If a signal from the proximity sensor 44 indicates that the tip of probe 7 incorporating the IR sensor 15 is positioned inside the ear canal, the computed temperature T_B is sent to display 2. However, if a signal from the proximity sensor 44 indicates that the tip of probe 7 is positioned at the entrance of the ear canal, the initial temperature T_B represents the exterior skin rather than the interior of the ear canal and thus should be adjusted to compensate for a cooling effect by the ambient temperature. The cooling effect is negligible inside the ear canal but it is substantial at the entrance of the ear canal. The ambient temperature is monitored by use of the ambient sensor 50 whose signal allows circuit 49 to compute ambient temperature T_a . The adjusted temperature T_d may be calculated according to the following equation:

$$T_d = T_B + k(T_B - T_a), \quad (1)$$

20 where k is a constant having a typical value of 0.017. However, the actual value of k should be experimentally determined for every practical design. The adjusted temperature T_d is sent to the display 2.

In another embodiment, a signal from the proximity sensor 44 may be used to generate for the operator a warning alarm (by display 2 or by any other visual or acoustic human interface) if the probe 7 is not correctly positioned inside the ear canal.

25 While the invention has been particularly shown and described with reference to preferred embodiments thereof, it will be understood by those skilled in the art as described herein that various changes in form and details may be made to the disclosed embodiments

without departing from the spirit and scope of the invention. Accordingly, the invention is to be limited only by the scope of the claims and their equivalents.

CLAIMS

1. A medical probe for insertion into a body cavity of a patient, comprising:

5 a probe body having a sidewall laterally circumscribing a longitudinal axis and enclosing an inner space, the sidewall having a proximal end and a distal end;

a sensor coupled to the probe to provide a signal relating to a condition of the body cavity of the patient;

10 a proximity sensor coupled to the probe, the proximity sensor configured to provide a signal indicating proximity of the probe to the body cavity or insertion of the probe into the body cavity.

2. The medical probe of claim 1, wherein the distal end of the sidewall is tapered relative to the proximal end of the sidewall.

15 3. The medical probe of claim 1, wherein the proximity sensor comprises an optical transmitter and an optical receiver positioned such that, when the medical probe is positioned for insertion into the body cavity, the optical transmitter is positioned to transmit an optical signal toward an opening of the body cavity, and the optical receiver is positioned to receive the optical signal from the optical transmitter.

20 4. The medical probe of claim 3, wherein the optical transmitter is positioned to transmit toward a first position adjacent to the body cavity, and the optical receiver is positioned to receive optical signals from a second position adjacent to the body cavity.

25

5. The medical probe of claim 3, wherein the proximity sensor further comprises a receiving light guide disposed within the inner space, the receiving light guide having a first end coupled to and protruding through the distal end of the sidewall, and a second end coupled to the optical receiver.

5

6. The medical probe of claim 5, wherein the receiving light guide protrudes through the distal end of the sidewall at an angle that is pointed away from the proximal end of the sidewall.

10

7. The medical probe of claim 5, wherein the proximity sensor further comprises a transmitting light guide disposed within the inner space, the transmitting light guide having a first end coupled to and protruding through the distal end of the sidewall, and a second end coupled to the optical transmitter.

15

8. The medical probe of claim 7, wherein the transmitting light guide protrudes through the distal end of the sidewall at an angle that is pointed away from the proximal end of the sidewall.

9. A medical probe for insertion into a body cavity of a patient, comprising:

20

a probe body having a sidewall laterally circumscribing a longitudinal axis and enclosing an inner space, the sidewall having a proximal end and a distal end;

a functional sensor coupled to the probe to provide a signal relating to a condition of the body cavity of the patient;

25

a proximity sensor coupled to the probe, the proximity sensor configured

to provide a signal indicating proximity of the probe to the body cavity or insertion of the probe into the body cavity.

5 10. The medical probe of claim 1, wherein the sensor comprises a temperature sensor.

11. The medical probe of claim 1, wherein the proximity sensor comprises a translucent opto-coupler that protrudes through the sidewall, the opto-coupler comprising:

10 a first side disposed within the inner space, the first side being optically coupled to a light emitter and a light detector; and

a second side disposed outside the inner space, wherein the second side protrudes through the wall of the probe.

15 12. The medical probe of claim 1, further comprising:

an electronic circuit coupled to the sensor and to the proximity sensor, the electronic circuit comprising:

a processor; and

a memory coupled to the processor, the memory storing software,

20 wherein the software, when executed by the processor, is configured to execute an algorithm to process signals from the sensor and the proximity sensor; and

an output device coupled to the processor, the output device configured to output a result of the algorithm.

13. The medical probe of claim 12, further comprising:

an ambient temperature sensor electrically coupled to the electronic circuit and positioned outside of the inner space,

5 wherein the software, when executed by the processor, is further configured to execute an algorithm to process signals from the sensor, the proximity sensor and the ambient temperature sensor.

14. The medical probe of claim 1, wherein the proximity sensor comprises:

10 a light emitter having a first optical axis; and
a light detector having a second optical axis.

15. The medical probe of claim 7, wherein at least one of the transmitting light guide and receiving light guide comprises a plastic optical fiber.

15

16. The medical probe of claim 7, wherein at least one of the transmitting light guide and receiving light guide comprises a glass rod.

17. The medical probe of claim 7, wherein at least one of the transmitting light guide and receiving light guide comprises a polycarbonate rod.

20

18. The medical probe of claim 7, wherein at least one of the transmitting light guide

and receiving light guide comprises a rod coated with a coating material, wherein a refractive index of the coating material is lower than a refractive index of the rod.

- 5 19. The medical probe of claim 7, wherein the first end of at least one of the transmitting light guide and receiving light guide comprises a lensing bulb.
20. The medical probe of claim 7, further comprising an optical barrier disposed in the inner space between the optical transmitter and optical receiver.
- 10 21. The medical probe of claim 5, wherein the optical receiver is disposed within the inner space.
22. The medical probe of claim 1, wherein the proximity sensor operates by use of ultrasonic signals.
- 15 23. A medical probe for insertion into a body cavity of a patient, comprising:
a curved probe body comprising:
a sidewall laterally circumscribing a longitudinal axis and enclosing an inner space, the sidewall having a proximal end and a distal
20 end; and
a circumferential flange portion coupled to the proximal end of the sidewall, the flange portion having a surface substantially perpendicular to the longitudinal axis and facing the distal end;

an optical transmitter coupled to a first position on the flange portion, the optical transmitter oriented to transmit an optical signal toward the distal end of the sidewall;

5

an optical receiver coupled to a second position on the flange portion, the optical receiver oriented to receive an optical signal from the distal end of the sidewall;

a sensor coupled to the distal end of the probe to provide a signal relating to a condition of the body cavity of the patient, the sensor oriented to sense the condition along the longitudinal axis.

10

24. The medical probe of claim 23, wherein the distal end of the sidewall is tapered relative to the proximal end of the sidewall.

15

25. A method for detecting an insertion of a medical probe into a body cavity of a patient, comprising the steps of:

transmitting, from a transmitter, a signal toward the body cavity;

receiving, at a receiver, a return signal from a direction from the body cavity; and

monitoring a flux of the return signal for a change in strength,

20

wherein a path from the transmitter to the receiver is at least partially blocked when the medical probe is inserted into the body cavity such that the flux of the return signal changes when the medical probe is inserted into the body cavity.

26. The method of claim 25, wherein:

the return signal is received from a second position in a direction from the body cavity, wherein the second position is reflectively coupled to the first position along a path across an opening of the body cavity.

5

27. The method of claim 25, wherein the transmitted signal comprises pulses.

28. The method of claim 25, further comprising the step of generating a warning alarm if the medical probe is not correctly positioned inside the ear canal.

10

29. A method for detecting an insertion of a medical probe, the medical probe having a longitudinal axis, into a body cavity of a patient along the longitudinal axis, comprising the steps of:

15

transmitting a signal along a first direction angularly offset from the longitudinal axis;

receiving a return signal from a second direction, the second direction angularly offset from the longitudinal axis; and

monitoring a flux of the return signal for an increase in strength,

20

wherein the flux of the return signal changes in strength above a predetermined threshold when the medical probe is inserted into the body cavity.

30. A method of displaying the temperature of a body cavity of a living being, comprising the steps of:

measuring a base temperature of the cavity by use of a temperature sensor;

measuring a proximity of the temperature sensor to the body cavity;

5

measuring an ambient temperature in an area adjacent to the temperature sensor;

computing a computed temperature of the body cavity in accord with a predetermined function of the base temperature, the proximity, and the ambient temperature; and

displaying the computed temperature.

10

31. The method of claim 30, further comprising the step of detecting a presence of a probe cover, wherein the predetermined function further comprises a function of the presence of a probe cover.

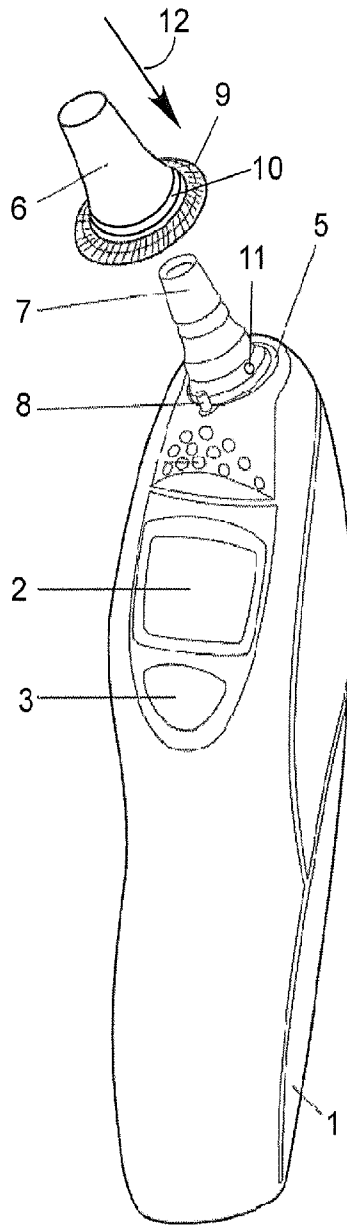


Fig. 1

Prior Art

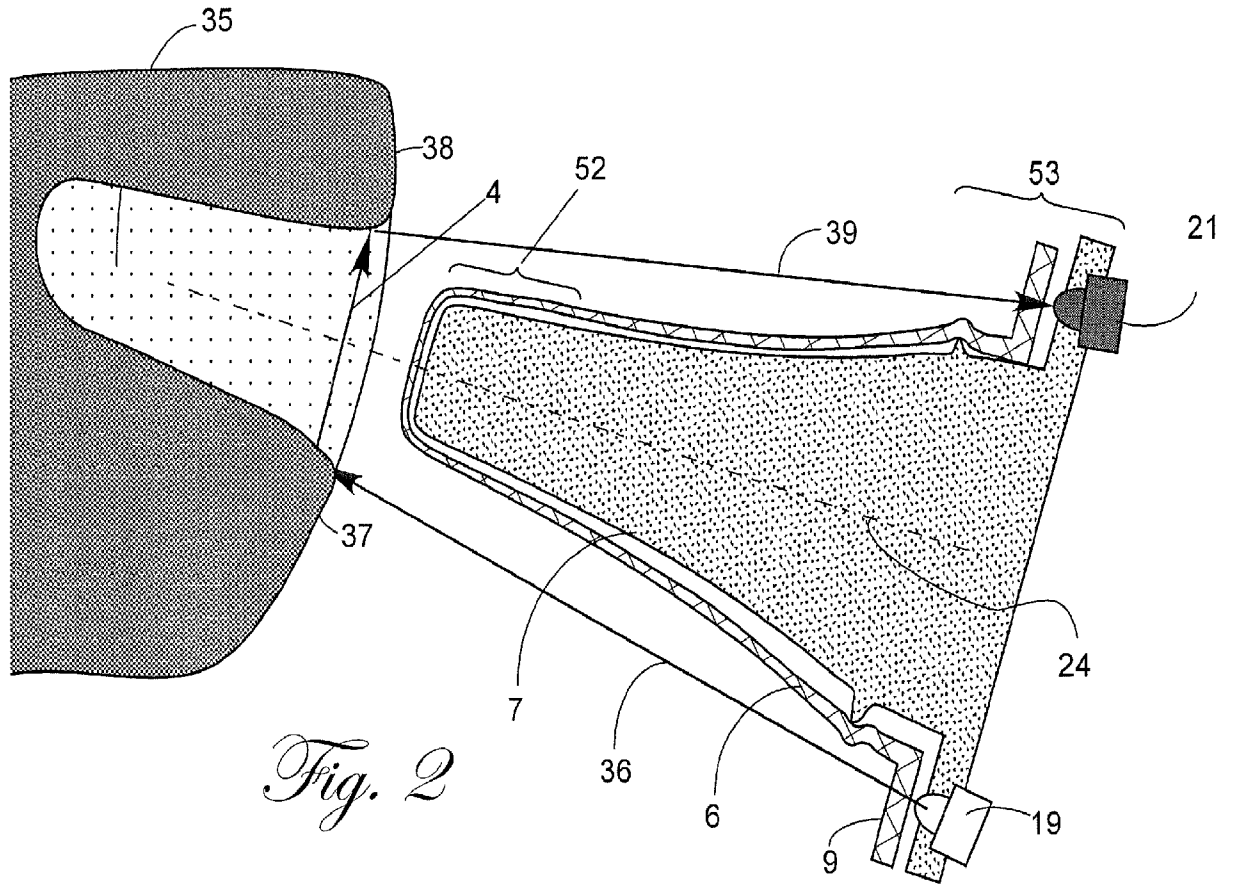


Fig. 2

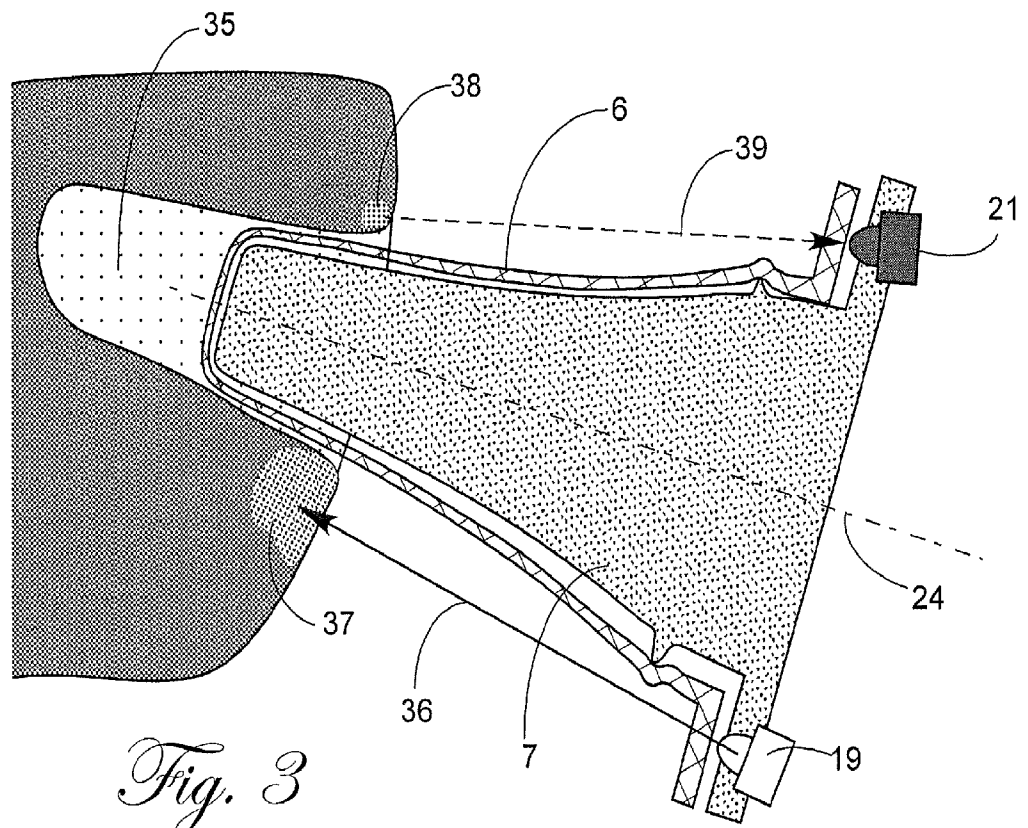


Fig. 3

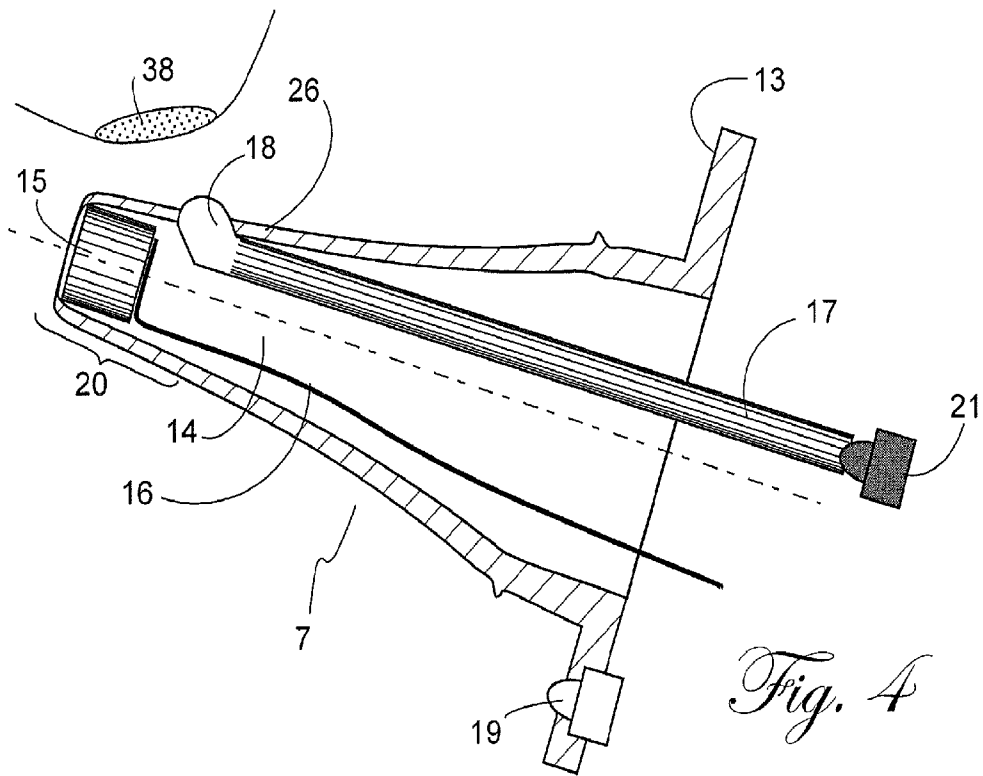


Fig. 4

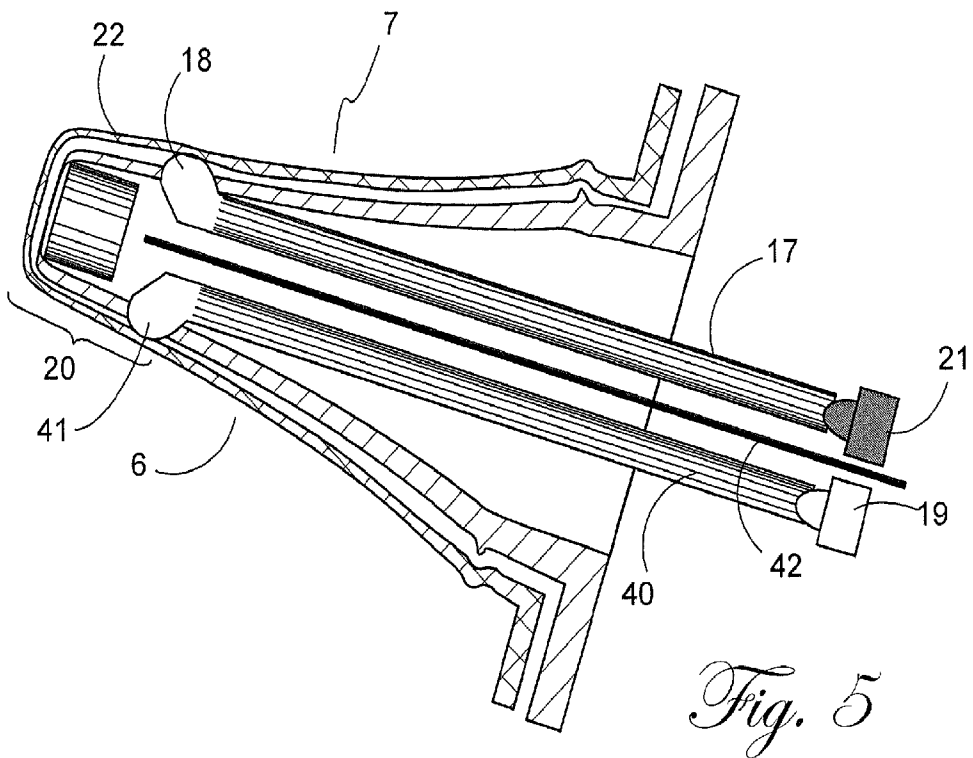


Fig. 5

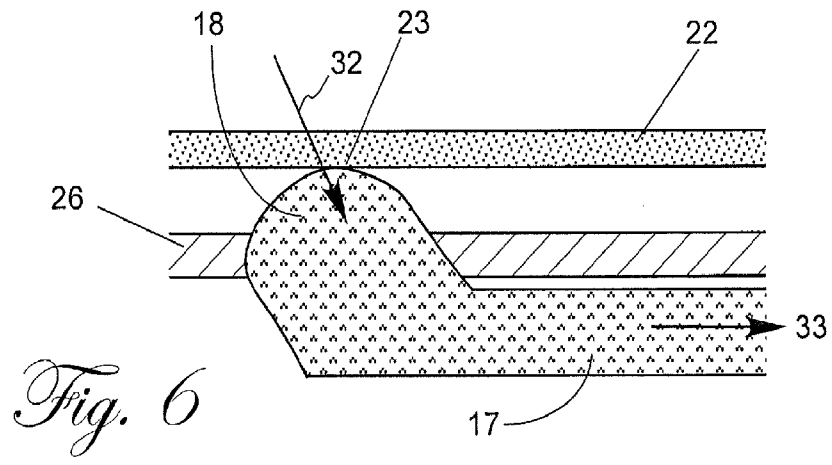


Fig. 6

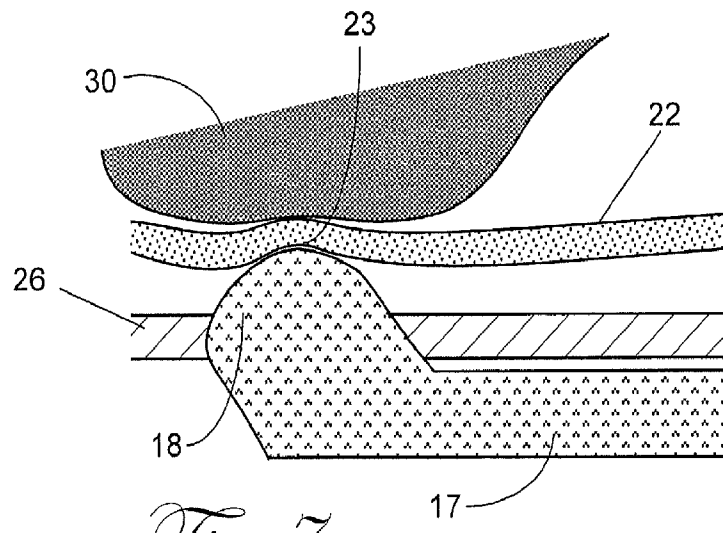


Fig. 7

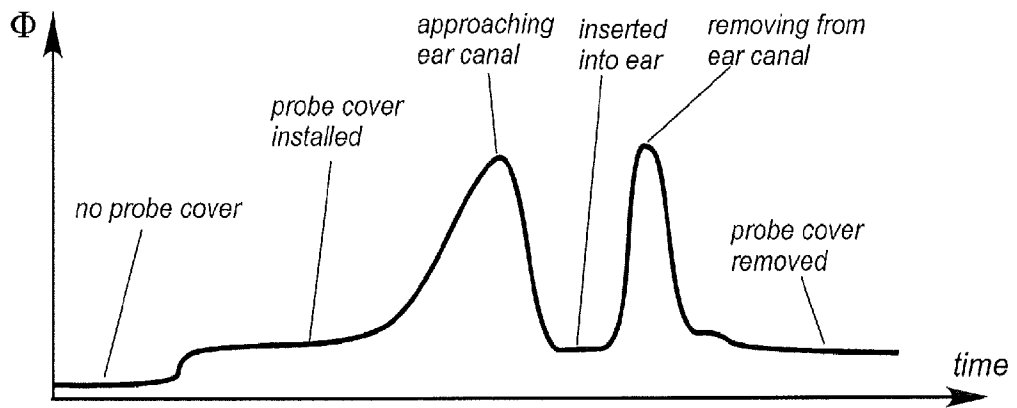


Fig. 8

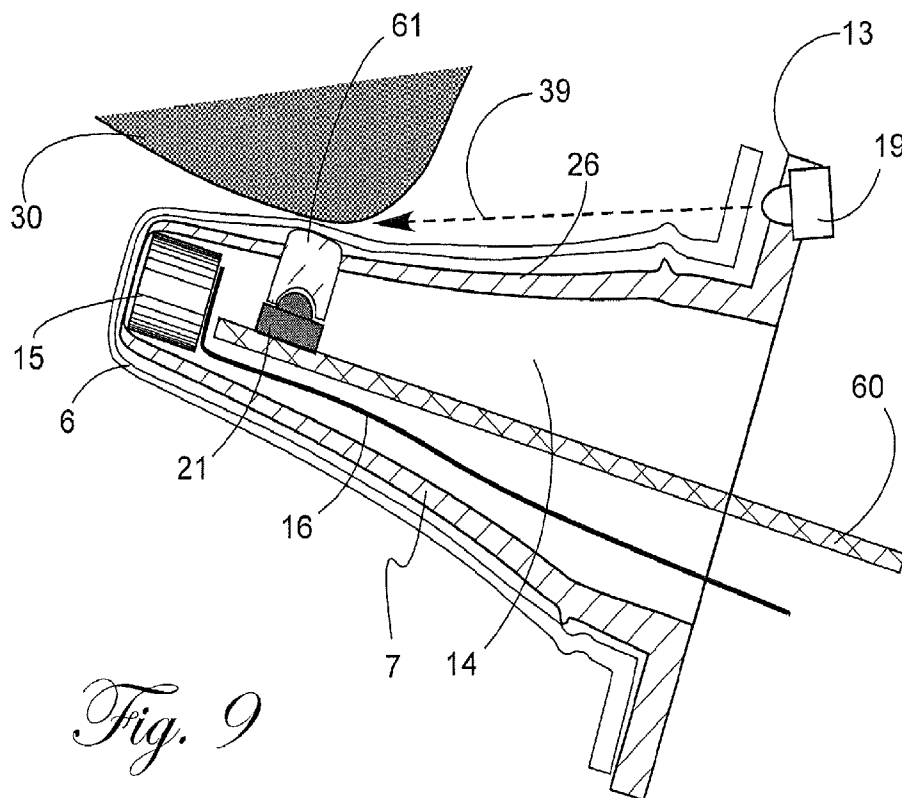


Fig. 9

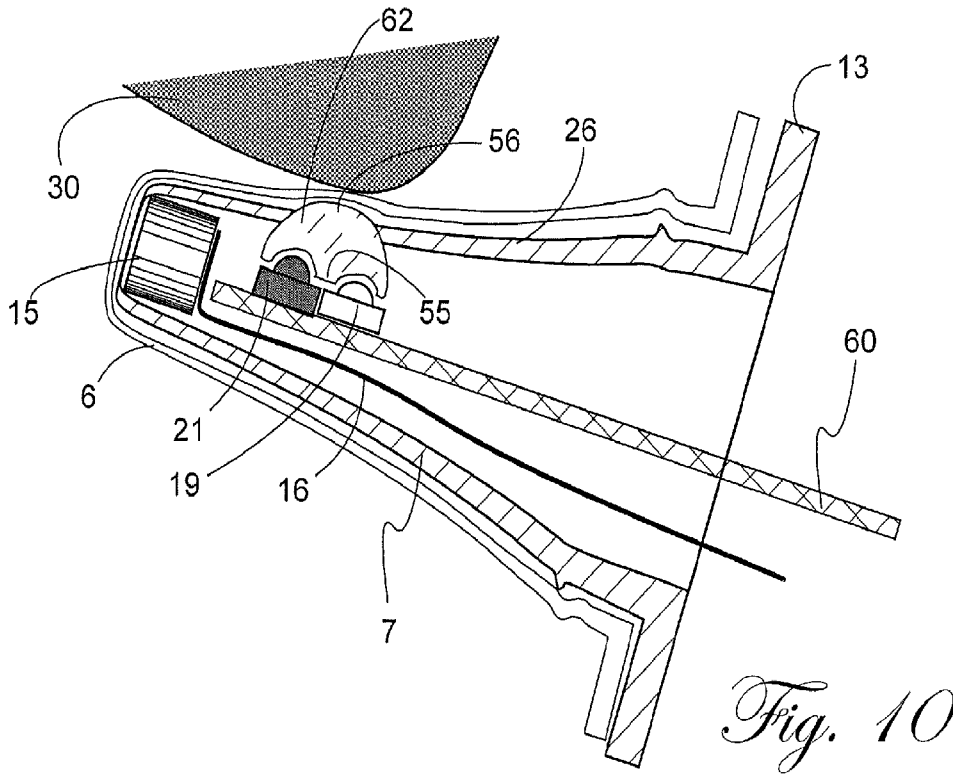


Fig. 10

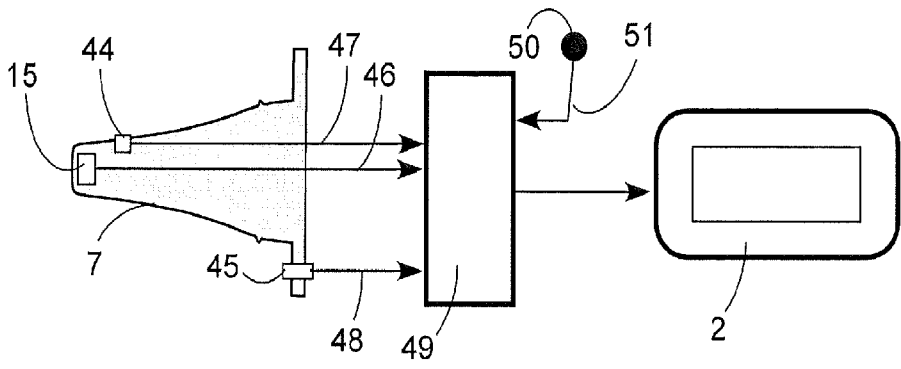


Fig. 11

INTERNATIONAL SEARCH REPORT

International application No. PCT/US2011/031264
--

A. CLASSIFICATION OF SUBJECT MATTER
 IPC(8) - A61B 5/01 (2011.01)
 USPC - 600/549
 According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
 IPC(8) - A61B 5/01, G01B 11/14, G01K 1/00, 1/08, 1/20 (2011.01)
 USPC - 600/549, 356/622, 374/100, 374/158

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
 Minesoft PatBase, Google Patents

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 7,314,310 B2 (MEDERO) 01 January 2008 (01.01.2008) entire document	1, 2, 9, 10, 12
-----		-----
Y		3-8, 11, 13-31
Y	US 2010/0043706 A1 (JUNG et al) 25 February 2010 (25.02.2010) entire document	3-8, 11, 14-21, 23-29
Y	US 5,926,269 A (VON DER ELTZ et al) 20 July 1999 (20.07.1999) entire document	17
Y	US 5,483,501 A (PARK et al) 09 January 1996 (09.01.1996) entire document	22, 27
Y	US 5,229,975 A (TRUESDELL et al) 20 July 1993 (20.07.1993) entire document	13, 30, 31

Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"E" earlier application or patent but published on or after the international filing date	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"O" document referring to an oral disclosure, use, exhibition or other means	"&" document member of the same patent family
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search 28 July 2011	Date of mailing of the international search report 02 AUG 2011
---	--

Name and mailing address of the ISA/US Mail Stop PCT, Attn: ISA/US, Commissioner for Patents P.O. Box 1450, Alexandria, Virginia 22313-1450 Facsimile No. 571-273-3201	Authorized officer: Blaine R. Copenheaver PCT Helpdesk: 571-272-4300 PCT OSP: 571-272-7774
---	---

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2011/031264

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

- 1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

- 2. Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

- 3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:
See Extra Sheet

- 1. As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
- 2. As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
- 3. As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

- 4. No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2011/031264

This application contains the following inventions or groups of inventions which are not so linked as to form a single general inventive concept under PCT Rule 13.1. In order for all inventions to be examined, the appropriate additional examination fees must be paid.

Group I, claims 1-22, 25-28, drawn to a medical probe and method for detecting insertion of a medical probe into the body of a patient, comprising a proximity sensor configured to provide a signal indicating proximity of the probe to the body cavity.

Group II, claims 23-24, 29, drawn to a medical probe comprising a curved probe body comprising a circumferential flange portion coupled to the proximal end,

the flange portion having a surface substantially perpendicular to the longitudinal axis and facing the distal end; an optical transmitter coupled to a first position on the flange portion, the

optical transmitter oriented to transmit an optical signal toward the distal end of the sidewall; an optical receiver coupled to a second position on the flange portion, the

optical receiver oriented to receive an angularly offset optical signal from the distal end of the sidewall.

Group III, claims 30-31, drawn to a method for displaying the temperature of a body cavity, comprising measuring an ambient temperature in an area adjacent to the temperature

sensor; computing a computed temperature of the body cavity in accord with a predetermined function including the ambient temperature; and displaying the computed temperature.

The inventions listed as Groups I, II and III do not relate to a single general inventive concept under PCT Rule 13.1 because, under PCT Rule 13.2, they lack the same or corresponding special technical features for the following reasons: the special technical feature of the Group I invention: a proximity sensor configured to provide a signal indicating proximity of the probe to the body cavity as claimed therein is not present in the invention of Groups II and III. The special technical feature of the Group II invention: a medical probe comprising a curved probe body comprising a circumferential flange portion coupled to the proximal end, the flange portion having a surface substantially perpendicular to the longitudinal axis and facing the distal end; an optical transmitter coupled to a first position on the flange portion, the optical transmitter oriented to transmit an optical signal toward the distal end of the sidewall; an optical receiver coupled to a second position on the flange portion, the optical receiver oriented to receive an angularly offset optical signal from the distal end of the sidewall as claimed therein is not present in the invention of Groups I or III. The special technical feature of the Group III invention: measuring an ambient temperature in an area adjacent to the temperature sensor; computing a computed temperature of the body cavity in accord with a predetermined function including the ambient temperature; and displaying the computed temperature as claimed therein is not present in the invention of Groups I or II.

Groups I, II and III lack unity of invention because even though the inventions of these groups require the technical feature of a medical probe for insertion into a body cavity of a patient, comprising a probe body having a sidewall laterally circumscribing a longitudinal axis and enclosing an inner space, the sidewall having a proximal end and a distal end; a sensor coupled to the probe to provide a signal relating to a condition of the body cavity of the patient, and generally a proximity sensor to indicate the probe body has been inserted in a body cavity, this technical feature is not a special technical feature as it does not make a contribution over the prior art in view of US 7,314,310 B2 (MEDERO) 01 January 2008 (01.01.2008) figures 1, 3; column 3, lines 29-31, 50-52; column 4. Lines 5-16, 65-67; col. 5, lines 1-5.

Since none of the special technical features of the Group I, II or III inventions are found in more than one of the inventions, unity of invention is lacking.

专利名称(译)	用于医疗探头的插入探测器		
公开(公告)号	EP2555670A4	公开(公告)日	2015-08-26
申请号	EP2011766597	申请日	2011-04-05
[标]申请(专利权)人(译)	卡兹欧洲公司		
申请(专利权)人(译)	KAZ EUROPE SA		
当前申请(专利权)人(译)	KAZ EUROPE SA		
[标]发明人	FRADEN JACOB		
发明人	FRADEN, JACOB		
IPC分类号	A61B5/01 A61B5/00 A61B5/06 G01J5/04 G01J5/06 G01K5/22 G01K13/00		
CPC分类号	A61B5/01 A61B5/065 A61B5/6817 A61B5/6886 A61B2562/0257 G01J5/021 G01J5/049 G01J5/0818 G01J5/089 G01J5/0896 G01J2005/068 G01K1/086 G01K13/004		
优先权	61/341715 2010-04-05 US		
其他公开文献	EP2555670A1		
外部链接	Espacenet		

摘要(译)

一种用于监测医疗探针相对于患者体腔的位置的插入检测器，该探针包括响应于患者身体的预定特性的接近传感器。接近传感器可包括光发射器和光检测器。当医用探针插入体腔时，光发射器和光检测器之间的光通量由于腔壁的阻碍或患者皮肤的反射而改变。来自接近传感器的响应可用于调节从体腔测量的温度，以校正由于探针未插入或部分插入体腔而导致的误差。