



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
**21.05.2008 Bulletin 2008/21**

(51) Int Cl.:  
**A61B 5/00 (2006.01) A61B 18/14 (2006.01)**

(21) Application number: **07254493.5**

(22) Date of filing: **16.11.2007**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR**  
Designated Extension States:  
**AL BA HR MK RS**

(72) Inventor: **Lee, James K.**  
**West Covina**  
**CA 91791 (US)**

(74) Representative: **Small, Gary James et al**  
**Carpmaels & Ransford**  
**43-45 Bloomsbury Square**  
**London WC1A 2RA (GB)**

(30) Priority: **17.11.2006 US 601065**


(71) Applicant: **Biosense Webster, Inc.**  
**Diamond Bar, CA 91765 (US)**

(54) **Improved catheter with omni-directional optical tip having isolated optical paths**

(57) A catheter enables real-time light measurements, for example, without limitation, diffuse reflectance, fluorescence, etc., from biological materials, such as tissue (including blood), while performing RF ablation. The catheter tip design isolates illumination and collection paths within the tip electrode such that light for illuminating the tissue of interest (e.g., cardiac tissue or blood) is isolated within the tip electrode from light that returns from the tissue to the catheter tip, and vice versa. Such a design advantageously avoids saturation of the optical detector, and ensures diffusion of the illumination light within the medium of interest. The catheter has a catheter body and a tip electrode with a shell wall and a hollow cavity. The shell wall has at least an illumination

opening and a collection opening. The catheter further includes a first fiber optic cable in communication with the illumination opening, and a second fiber optic cable in communication with the hollow cavity, wherein light emitted from the first fiber optic cable exits the tip electrode to reach tissue through the illumination opening in defining a first path and returns to the tip electrode from the tissue into the hollow cavity through the collection opening in defining a second path, the first and second paths being optically isolated from each other within the tip electrode. The invention also includes a method of making an ablation electrode tip defining isolated optical paths with in the tip electrode for light exiting the tip electrode and light returning to the tip electrode.

*FIG. 4A*

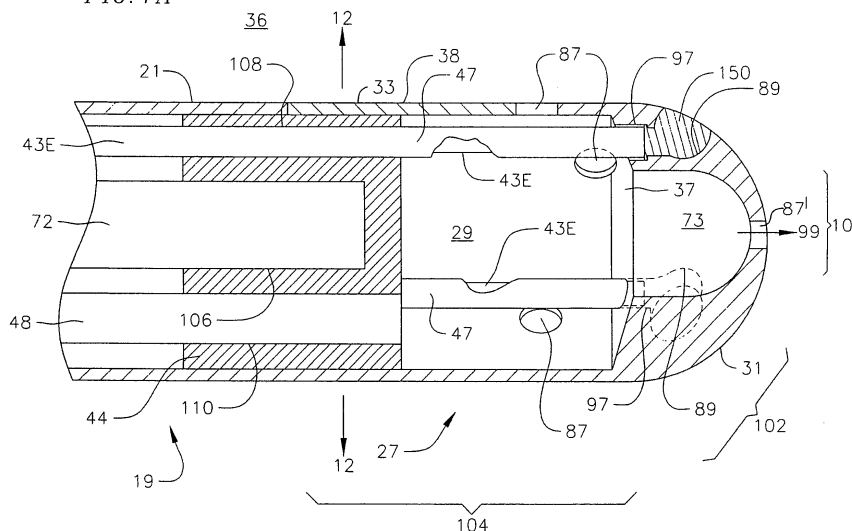

## Description

### FIELD OF INVENTION

**[0001]** The present invention relates to ablation catheters, and in particular to ablation catheters with optical monitoring of tissue.

### BACKGROUND

**[0002]** For certain types of minimally invasive medical procedures, real time information regarding the condition of the treatment site within the body is unavailable. This lack of information inhibits the clinician when employing catheter to perform a procedure. An example of such procedures is tumor and disease treatment in the liver and prostate. Yet another example of such a procedure is surgical ablation used to treat atrial fibrillation. This condition in the heart causes abnormal electrical signals, known as cardiac arrhythmias, to be generated in the endocardial tissue resulting in irregular beating of the heart.

**[0003]** The most frequent cause of cardiac arrhythmias is an abnormal routing of electricity through the cardiac tissue. In general, most arrhythmias are treated by ablating suspected centers of this electrical misfiring, thereby causing these centers to become inactive. Successful treatment, then, depends on the location of the ablation within the heart as well as the lesion itself. For example, when treating atrial fibrillation, an ablation catheter is maneuvered into the right or left atrium where it is used to create ablation lesions in the heart. These lesions are intended to stop the irregular beating of the heart by creating non-conductive barriers between regions of the atria that halt passage through the heart of the abnormal electrical activity.

**[0004]** The lesion should be created such that electrical conductivity is halted in the localized region (transmurality), but care should be taken to prevent ablating adjacent tissues. Furthermore, the ablation process can also cause undesirable charring of the tissue and localized coagulation, and can evaporate water in the blood and tissue leading to steam pops.

**[0005]** Currently, lesions are evaluated following the ablation procedure, by positioning a mapping catheter in the heart where it is used to measure the electrical activity within the atria. This permits the physician to evaluate the newly formed lesions and determine whether they will function to halt conductivity. It if is determined that the lesions were not adequately formed, then additional lesions can be created to further form a line of block against passage of abnormal currents. Clearly, post ablation evaluation is undesirable since correction requires additional medical procedures. Thus, it would be more desirable to evaluate the lesion as it is being formed in the tissue.

**[0006]** A known method for evaluating lesions as they are formed is to measure electrical impedance. Biochem-

ical differences between ablated and normal tissue can result in changes in electrical impedance between the tissue types. Although impedance is routinely monitored during electrophysiologic therapy, it is not directly related to lesion formation. Measuring impedance merely provides data as to the location of the tissue lesion but does not give qualitative data to evaluate the effectiveness of the lesion.

**[0007]** Another approach is to measure the electrical conductance between two points of tissue. This process, known as lesion pacing, can also determine the effectiveness of lesion therapy. This technique, however, measures the success or lack thereof from each lesion, and yields no real-time information about the lesion formation.

**[0008]** Thus, there is a need for a catheter that is capable of measuring lesion formation in real-time, if not monitoring tissue in general, and is adapted for use at most angles to the tissue. Moreover, where such measuring and detecting are accomplished through optical spectroscopy, there is a need for a catheter that can provide separate optical paths for illuminating the tissue and recapturing light from the tissue. The catheter should also be of a simplified but efficient design that allows for ease in manufacturing and reduced production labor and costs.

### SUMMARY OF THE INVENTION

**[0009]** The present invention is directed to a catheter that enables real-time light measurements, for example, without limitation, diffuse reflectance, fluorescence, etc., from biological materials, such as tissue (including blood), while performing RF ablation. The catheter tip design is implied but maintains isolated illumination and collection paths within the tip electrode for light to exit the catheter tip and interact with, if not travel through, the tissue of interest (e.g., cardiac tissue or blood) before returning to the catheter tip. Such a design advantageously avoids saturation of the optical detector, and ensures diffusion of the illumination light within the medium of interest.

**[0010]** The light recaptured by the catheter from the tissue conveys tissue parameters that can be evaluated using optical spectroscopy. These parameters include, without limitation, lesion formation, depth of penetration of lesion, and cross-sectional area of lesion, formation of char during ablation, recognition of char during ablation, recognition of char from non-charred tissue, formation of coagulum around the ablation site, differentiation of coagulated from non-coagulated blood, differentiation of ablated from healthy tissue, tissue proximity, evaluation of tissue health, status, and disease state, and recognition of steam formation in the tissue for prevention of steam pop.

**[0011]** In accordance with one aspect of the present invention, the catheter in one embodiment includes a catheter body and a tip electrode with a shell wall and a

hollow cavity, where the shell wall has at least an illumination opening and a collection opening. The catheter also has a first fiber optic cable in communication with the illumination opening and a second fiber optic cable in communication with the hollow cavity, wherein light emitted from the first fiber optic cable exits the tip electrode to reach tissue through the illumination opening in defining a first path and returns to the tip electrode from the tissue into the hollow cavity through the collection opening in defining a second path. Advantageously, the first and second paths in the tip electrode are optically isolated from each other.

**[0012]** In a more detailed embodiment, a catheter has a catheter body and a tip electrode adapted for ablating tissue. The tip electrode has a shell and a hollow cavity. The shell has multiple illumination openings into which light from emitting fiber optic cables is injected to illuminate tissue of interest. The illumination openings have a semi-spherical cross-section and may be filled with a material with optical scattering properties, e.g., a scattering agent-filled epoxy or plastic, to aid in the even distribution of light out of the openings. The shell also has multiple collection openings through which light recaptured from the tissue is collected in the hollow cavity. And one or more receiving fiber optic cables are provided to receive the light collected in the hollow cavity. Where the emitting fiber optic cables traverse the hollow cavity, a coating is provided on the cables to prevent light from leaking out of or into the cables for keeping the separate paths optically isolated within the tip electrode.

**[0013]** In accordance with a second aspect of the present invention, there is provided a catheter, comprising: a catheter body; a tip electrode distal the catheter body, the tip electrode having a shell wall and a hollow cavity, the shell wall having illumination openings and collection openings; at least one emitting fiber optic cable in communication with at least one of the illumination openings; at least one receiving fiber optic cable in communication with the hollow cavity, wherein light emitted from the at least one emitting fiber optic cable exits the tip electrode to reach tissue through at least the one illumination opening in defining a first path and returns to the tip electrode from the tissue into the hollow cavity through the collection opening in defining a second path, the first and second paths being optically isolated from each other within the tip electrode.

**[0014]** Preferably, the distal end of the at least one emitting fiber optic cable extends substantially into the at least one illumination opening. The receiving fiber optic cable may receive light in the hollow cavity and the tip of the electrode may be configured with a plurality of collection openings and illumination openings. There may be at least one emission fiber optic cable for a respective illumination opening. Preferably, the tip electrode is configured with at least four collection openings and three illumination openings.

**[0015]** As an omnidirectional illuminator and collector, the tip electrode in one embodiment has a first section

that is generally perpendicular to a longitudinal axis of the tip electrode, a second section that is at an angle between about 0 and 90 degrees with the longitudinal axis, and a third section that is generally parallel with the longitudinal axis. The collection and illumination openings may be configured in any of the first, second and/or third sections. In one embodiment, the collection openings are configured in the first and third sections, and the illumination openings are configured in the second section.

**[0016]** The tip electrode also includes an alignment plug that seals the hollow cavity. The plug has passages for the emitting and the receiving fiber optic cables extending therethrough, to stabilize the fiber optic cables and minimize stress that can cause breakage of the fiber optic cables.

**[0017]** The present invention is also directed to a method of making an ablation tip electrode that also functions as an omnidirectional illuminator and collector. The method includes providing a shell with a hollow cavity, configuring at least one collection opening in the shell, configuring at least illumination opening in the shell, providing an emitting fiber optic cable adapted to emit light into the illumination opening, providing a receiving fiber optic cable adapted to receive light collected in the hollow cavity, and providing an optical barrier between the emitting fiber optic cable and the hollow cavity.

**[0018]** The method may further include providing the illumination opening with a semi-spherical cross section and filling the illumination opening with a material having optical scattering property, for example, a scattering agent-filled epoxy or plastic, to aid in the even distribution of light out of the openings. The method may also further include forming a plug to seal with hollow cavity, wherein the plug is configured with passages for the fiber optic cables to extend through, and fixedly securing portions of the fiber optic cables in the passages to the plug.

**[0019]** The present catheter and method are designed to use light in conjunction with irrigation and the technology of RF ablation. Advantageously, the light used to monitor and assess the tissue (or a lesion formed in the tissue) is generally not affected by the portion of the electromagnetic radiation used for ablation. Moreover, the bandwidth used for monitoring and assessing also transmits through blood with minimal attenuations. The fiber optics are used and disposed in the catheter in a manner that avoids contact with tissue, which can increase the operative lifetime of the catheter and minimize damages caused by abrasion to the fiber optics. Furthermore, the alignment plug in the tip electrode secures the fiber optic cables with minimal bend or strain but increased angular coverage, which can minimize fiber optics breakage during assembly and use, as well as reduce nonlinear optical effects caused by orientation of the fiber optics. In addition, the use of fiber optics to emit and receive light is a generally temperature neutral process that adds little if any measurable heat to surrounding blood or tissue.

## BRIEF DESCRIPTION OF THE DRAWINGS

[0020] These and other features and advantages of the present invention will be better understood by reference to the following detailed description when considered in conjunction with the accompanying drawings wherein:

[0021] FIG. 1 is a side view of an embodiment of the catheter of the present invention.

[0022] FIG. 2A is a side cross-sectional view of an embodiment of a catheter body according to the invention, including the junction between the catheter body and intermediate section, taken along a first diameter.

[0023] FIG. 2B is a side cross-sectional view of an embodiment of a catheter body according to the invention, including the junction between the catheter body and intermediate section, taken along a second diameter generally perpendicular to the first diameter of FIG. 2A.

[0024] FIG. 3A is a side cross-sectional view of an embodiment of a catheter body according to the invention, including the junction between the intermediate section and a tip section, taking along a first diameter.

[0025] FIG. 3B is a side cross-sectional view of an embodiment of a catheter body according to the invention, including the junction between the intermediate section and a tip section, taking along a second diameter generally perpendicular to the first diameter of FIG. 3A.

[0026] FIG. 4A is a side cross sectional view of an embodiment of a catheter body according to the invention, including a junction between a plastic housing and a tip electrode, taken along a first diameter.

[0027] FIG. 4B is a side cross-sectional view of an embodiment of a catheter body according to the invention, including a junction between a plastic housing and a tip electrode, taken along the second diameter generally perpendicular to the first diameter of FIG. 4A;

[0028] FIG. 5 is a longitudinal cross-sectional view of an embodiment of an intermediate section of FIG. 3A, taken along line 5--5.

[0029] FIG. 6 is a perspective view of an embodiment of a tip electrode.

[0030] FIG. 7 is a longitudinal cross-sectional view of the tip electrode of FIG. 4A, taken along line 7-7.

[0031] FIG. 8 is a longitudinal cross-sectional view of the tip electrode of FIG. 4A, taken along line 8--8.

[0032] FIG. 9 is a longitudinal cross-sectional view of the tip electrode of FIG. 4A, taken along line 9--9.

[0033] FIG. 10 is a longitudinal cross-sectional view of the tip electrode of FIG. 4A, taken along line 10--10.

[0034] FIG. 11A is a side view of another embodiment of a tip section whose longitudinal axis is generally perpendicular to tissue surface.

[0035] FIG. 11 B is a side view of another embodiment of a tip section whose longitudinal axis is generally at an angle between zero and 90 to tissue surface.

[0036] FIG. 11C is a side view of another embodiment of a tip section whose longitudinal axis is generally parallel to tissue surface.

[0037] FIG. 12 is a longitudinal cross-sectional view of the plug within the tip electrode of FIG. 4A, taken along line 12-12.

[0038] FIG. 12A is a detailed cross-sectional view of an embodiment of a distal end of a lead wire anchored in a plug of a tip electrode.

[0039] FIG. 12B is a detailed cross-sectional view of an embodiment of distal ends of a thermocouple wire pair anchored in a plug of a tip electrode.

[0040] FIG. 12C is a detailed cross-sectional view of an embodiment of a distal end of a puller wire anchored in a plug of a tip electrode.

[0041] FIG. 13 is a schematic drawing showing components of an embodiment of an optical processing system for use with the catheter of the present invention.

## DETAILED DESCRIPTION OF THE INVENTION

[0042] The catheter 10 of the present invention is adapted to facilitate optically-based real-time assessment of ablation tissue characteristics, including without limitation, lesion formation, depth of penetration of the lesion, cross-sectional area of the lesion, formation of char during ablation, recognition of char during ablation, differentiation of char from non-charred tissue, formation of coagulum around the ablation site, differentiation of coagulated from non-coagulated blood, differentiation of ablated from healthy tissue, tissue proximity, and recognition of steam formation in the tissue for prevention of steam pop. These assessments are accomplished by measuring the light intensity at one or more wavelengths that is recaptured at the catheter resulting from the light radiated from the catheter tip onto ablated tissue. Fiber optic cables are provided in the catheter to transmit light to and from the catheter tip.

[0043] As shown in FIGS. 1-13, catheter 10 of the present invention comprises an elongated catheter body 12 having proximal and distal ends, a deflectable (uni- or bi-directionally) intermediate section 14 at the distal end of the catheter body 12, a tip section 36 at the distal end of the intermediate section, and a control handle 16 at the proximal end of the catheter body 12.

[0044] With additional reference to FIGs. 2A and 2B, the catheter body 12 comprises an elongated tubular construction having a single, axial or central lumen 18. The catheter body 12 is flexible, i.e., bendable, but substantially non-compressible along its length. The catheter body 12 can be of any suitable construction and made of any suitable material. A construction comprises an outer wall 22 made of an extruded plastic. The outer wall 22 may comprise an imbedded braided mesh of stainless steel or the like to increase torsional stiffness of the catheter body 12 so that, when the control handle 16 is rotated, the catheter body 12, the intermediate section 14 and the tip section 36 of the catheter 10 will rotate in a corresponding manner.

[0045] Extending through the single lumen 18 of the catheter body 12 are components, for example, wires,

tubes and/or cables. A single lumen catheter body can be preferred over a multi-lumen body because it has been found that the single lumen body permits better tip control when rotating the catheter. The single lumen permits the various components to float freely within the catheter body. If such wires, tube and cables were restricted within multiple lumens, they tend to build up energy when the handle is rotated, resulting in the catheter body having a tendency to rotate back if, for example, the handle is released, or if bent around a curve, to flip over, either of which are undesirable performance characteristics.

**[0046]** The outer diameter of the catheter body 12 is not critical, but is preferably no more than about 8 french, more preferably 7 french. Likewise the thickness of the outer wall 22 is not critical, but is thin enough so that the central lumen 18 can accommodate the aforementioned components. The inner surface of the outer wall 22 may be lined with a stiffening tube 20, which can be made of any suitable material, such as polyimide or nylon. The stiffening tube 20, along with the braided outer wall 22, provides improved torsional stability while at the same time minimizing the wall thickness of the catheter, thus maximizing the diameter of the central lumen 18. The outer diameter of the stiffening tube 20 is about the same as or slightly smaller than the inner diameter of the outer wall 22. Polyimide tubing may be preferred for the stiffening tube 20 because it may be very thin walled while still providing very good stiffness. This maximizes the diameter of the central lumen 18 without sacrificing strength and stiffness.

**[0047]** The catheter may have an outer wall 22 with an outer diameter of from about 0.090 inch to about 0.098 inch and an inner diameter of from about 0.061 inch to about 0.078 inch and a polyimide stiffening tube 20 having an outer diameter of from about 0.060 inch to about 0.077 inch and an inner diameter of from about 0.051 inch to about 0.069 inch.

**[0048]** Referring also to FIG. 5, the intermediate section 14 distal the catheter body 12 comprises a shorter section of tubing 19 having multiple lumens. The tubing 19 is made of a suitable non-toxic material that is preferably more flexible than the catheter body 12. A suitable material for the tubing 19 is braided or non-braided polyurethane. The outer diameter of the intermediate section 14, like that of the catheter body 12, is preferably no greater than about 8 french, more preferably 7 french. The size and number of the lumens are not critical. In an embodiment, the intermediate section 14 has an outer diameter of about 7 french (0.092 inch). The tubing 19 is multi-lumened, for example, with a first lumen 30, a second lumen 32, a third lumen 34 and a fourth lumen 35. In the illustrated embodiment, the lumens 30, 32 and 35 all have approximately the same diameter of about 0.22 inch, whereas the lumen 34 has a larger diameter of about 0.44 inch.

**[0049]** As shown in the embodiments of FIGs. 2A and 2B, the catheter body 12 that may be attached to the intermediate section 14 comprises an outer circumferen-

tial notch 24 configured in the proximal end of the tubing 19 that receives the inner surface of the outer wall 22 of the catheter body 12. The intermediate section 14 and catheter body 12 are attached by glue or the like. Before the intermediate section 14 and catheter body 12 are attached, the stiffening tube 20 is inserted into the catheter body 12. The distal end of the stiffening tube 20 is fixedly attached near the distal end of the catheter body 12 by forming a glue joint 23 with polyurethane glue or the like. Preferably a small distance, e.g., about 3 mm, is provided between the distal end of the catheter body 12 and the distal end of the stiffening tube 20 to permit room for the catheter body 12 to receive the notch 24 of the intermediate section 14. If no compression coil is used, a force is applied to the proximal end of the stiffening tube 20, and, while the stiffening tube 20 is under compression, a first glue joint (not shown) is made between the stiffening tube 20 and the outer wall 22 by a fast drying glue, e.g. cyanoacrylate. Thereafter, a second glue joint 26 is formed between the proximal ends of the stiffening tube 20 and outer wall 22 using a slower drying but stronger glue, e.g., polyurethane.

**[0050]** If desired, a spacer can be located within the catheter body between the distal end of the stiffening tube and the proximal end of the tip section. The spacer provides a transition in flexibility at the junction of the catheter body and intermediate section, which allows this junction to bend smoothly without folding or kinking. A catheter having such a spacer is described in U.S. patent application Ser. No. 08/924,616, entitled "Steerable Direct Myocardial Revascularization Catheter", the entire disclosure of which is incorporated herein by reference.

**[0051]** Extending from the distal end of the intermediate section 14 is the tip section 36 that includes a tip electrode 27 and a plastic housing 21, as shown in FIGs. 4A and 4B. The plastic housing 21, as also shown in FIGs. 3A and 3B, connects the tip electrode 27 and the tubing 19, and provides housing and/or transitional space for the components that extend into or through its lumen, as discussed further below. The plastic housing 21 is preferably made of polyetheretherketone (PEEK) and may be about 1 cm long. Its proximal end receives the outer circumferentially notched surface 17 of the tubing 19 of the intermediate section 14. The intermediate section 14 and the plastic housing 21 are attached by glue or the like. Components such as wires, cables and tubes that extend between the intermediate section 14 and the tip electrode 27 help keep the tip electrode in place.

**[0052]** In accordance with the present invention, the tip electrode 27 is adapted to function as an omnidirectional illuminator and collector for recapturing light that is radiated from the catheter tip onto ablated tissue. As shown in FIGs. 4A and 4B, the tip electrode comprises a shell wall 38 and a plug 44. The shell 38 is configured with a distal dome end 31 and an open proximal portion 33 in communication with a hollow cavity 29. In the illustrated embodiment, the shell wall 28 has a generally uniform thickness except at the distal dome end 31 where

the thickness is greater and surrounds a distal dome cavity 73 extending from a rim region 37 of the hollow cavity 29. The distal dome end 31 of the shell is atraumatic and adapted for contact with tissue. The open proximal end 33 is configured to receive the plug 44 which, among other functions, seals the hollow cavity 29.

**[0053]** The shell 38 and the plug 44 are formed from any suitable material that is opaque and/or reflective, and both thermally and electrically conductive which allows for radio frequency ablation using an RF generator. Such suitable materials include, without limitation, platinum-iridium, platinum, gold alloy, or palladium alloy.

**[0054]** The tip electrode 27 has different sections relative to its longitudinal axis 99 in rendering the tip omnidirectional for optical tissue monitoring. As shown in FIGs. 4A, 4B, and 6, there are a distal section 100, a mid-section 102 and a proximal section 104. The shell wall 38 of the distal section 100 is generally perpendicular to the axis 99. The shell wall of the mid-section 102 is generally at an angle ranging between zero and 90 degrees, preferably about 30 to 60 and more preferably about 45 degrees to the axis 99. The shell wall of the proximal section 104 is generally parallel with the axis 99. These differently-angled sections which have a generally smooth and atraumatic transition between each other enable the tip electrode 27 to operate as an illuminator and a collector for various angles between the tip section 36 and the tissue as shown in FIGs. 11A-11C.

**[0055]** The shell wall 38 has a plurality of holes or openings of various sizes, including illumination openings and collection openings for light to leave and re-enter the tip electrode 27. As discussed further below, the tip electrode 27 provides optically-isolated paths for light intended to illuminate tissue and for light that is received through the collection openings. Each section 100, 102, 104 of the tip electrode can have any number of illumination and/or collection openings as desired or appropriate, although the number is dependent in part on the size of the tip electrode and the size and number of fiber optic cables housed therein. In the illustrated embodiment, the distal section 100 has a collection opening 87' at the distal end of the tip electrode along the longitudinal axis 99 (FIG. 7). The mid-section 102 has three illumination openings 89 that are equi-angular from each other at about 120 degrees radially about the axis (FIG. 8). The proximal section 104 has three more collection openings 87 that are equi-angular from each other at about 120 degrees radially about the axis (FIG. 9). The three collection openings 87 are offset radially by about 20 degrees from the three illumination openings 89 in the mid-section 102. Also in the proximal section 104 further proximal to the three collection openings 87 are an additional three collection openings 87" (FIG. 10) that are equi-angular from each other at about 120 degrees about the axis. These three collection openings 87" are offset radially by about 40 degrees from the more distal collection openings 87 in the proximal section 104.

**[0056]** To efficiently illuminate the tissue of interest,

each of the illumination openings 89 has a generally curved cross-section. In the illustrated embodiment of FIG. 8, the cross-section has a semi-spherical apex 93 where the overall cross-section can be described as parabolic. The semi-spherical apex efficiently reflects light out of the opening 89 for a more even distribution of light from the distal dome end 31 of the tip electrode 27.

**[0057]** With reference to FIGs. 4A and 4B, light is delivered to the illumination openings 89 by one or more emitting fiber optic cables 43E whose distal ends are received in passages 97 extending longitudinally from the rim section 37 of the hollow cavity 49. The configuration of the passages further isolates the light from the cables 43E from the cavity 29, and vice versa. The illumination openings 89 may be filled with a material 150 with optical scattering properties, e.g., a scattering agent-filled epoxy or plastic to aid in the even distribution of light out of the openings 89. Accordingly, light is emitted omnidirectionally onto the tissue of interest from the distal end of the tip electrode with minimal loss to absorption within the tip dome structure and the material 150 used to scatter the light.

**[0058]** Light reentering the tip electrode from the tissue via the collection openings 87 is captured and reflected about in the hollow cavity 29. The distal dome cavity 33 connecting the opening 87' and the hollow cavity 29 is configured to optimize the amount of light received in the hollow cavity 29 through the collection opening 87'. At least one receiving fiber optic cable 43R extends into the hollow cavity to collect the light. It is noted that because each of the emitting fiber optic cables 43E traverses the hollow cavity 29 to reach the passage 97, each cable 43E has a coating 47 to optically isolate itself from the cavity, and vice versa. The coating can be an opaque but reflective buffer material, e.g., aluminum, gold and the like, so that light cannot penetrate the side wall of the fiber 43E either into the cavity 29 or from the cavity. The coating may extend the length of the fibers 43E throughout the catheter.

**[0059]** The fiber optic cables 43E and 43R are protectively housed in the catheter from the control handle 16 to the tip section 36. As shown in FIGs. 2B and 5, they extend through the central lumen 18 of the catheter 12, the third lumen 34 of the intermediate section 14, the plastic housing 21 and into the tip electrode 27.

**[0060]** In the disclosed embodiment, there are three illuminating cables 43E and one receiving cable 43R. The cables 43E function as light emitters by transmitting light to the tip electrode 37 from a remote light source. The cable 43R functions as a light receiver by collecting light from the hollow cavity 29 in the tip electrode 27. It is understood by one of ordinary skill in the art that optical waveguides and fiber optic cables in general serve to transmit optical energy from one end to the other, although these are not exclusive.

**[0061]** Formed of the same or comparable material as the shell 38, the plug 44 has a generally elongated cylindrical configuration having a predetermined length,

and a generally circular cross-section that matches the cross-section of the open proximal end 33 of the tip electrode 27. A distal portion of the plug 44 is press fitted, or fixed with solder into the open proximal end 33 to seal the hollow cavity 29, while a proximal portion of the plug 44 extends proximally from the tip electrode 27 for attachment to the housing 21.

**[0062]** In accordance with the present invention, blind holes and passages are provided in the plug 44 to allow components extending from the intermediate section 14 to be anchored to the plug or to pass through to the hollow cavity 29. In the illustrated embodiment of FIGs. 4A, 4B and 12, there are blind holes 102, 104 and 106 formed in the proximal surface of the plug in which distal ends of a lead wire 40, thermocouple wires 41 and 45 and a location sensor 72 are anchored, respectively. There are also passages 108, 112, 114, and 116 through which the fiber optic cables 43E and 43R extend, and a passage 110 through which an irrigation tube 48 extends into the hollow cavity of the tip electrode 29. The passages 108, 112 and 114 for three fiber optic cables 43E are generally aligned with the passages 97 leading to the illumination openings 89 in the shell wall 38 of the tip electrode. The portions of the components extending through the passages in the plug 44 are securely fixed in the passages to the plug 44 by glue, adhesive or the like. As such, the passages and the plug help align, stabilize and secure the various components extending through the plug 44. In particular, the passages help minimize stress on the cables 43E and 43R in their transition between the intermediate section 14 and the tip electrode 27.

**[0063]** In accordance with the present invention, illumination of tissue 111 and recapturing of the light from the tissue is accomplished by the omnidirectional tip electrode 27 whether the catheter 10 is generally perpendicular to the tissue (FIG. 11A), at an angle between about zero and ninety degrees (FIG. 11B), or generally parallel with the tissue (FIG. 11C). It is understood by one of ordinary skill in the art that the plurality and configuration of the sections 100, 102 and 104 and of the collection and illumination openings 87, 87' and 87" and 89 may be varied as appropriate or desired. The size and dimensions of each section may also be varied as appropriate or desired, as well as the shape of the openings, which can be round, oval, square, polygonal, flat (slit), or any combination of these shapes.

**[0064]** In operation, the catheter 10 emits light at its tip electrode 27 as provided by the fiber optic cables 43E at their distal ends which emit light into the illumination openings 89, where the semi-spherical apex 93 efficiently reflects light out of the opening 89 for a more even distribution of light from the distal dome end 31 of the tip electrode 27. As lesion 113 forms in the tissue 111 from ablation carried out by tip electrode 27 of the catheter 10 (or by another catheter), its characteristics are altered as understood by one of ordinary skill in the art. In particular, as the lesion is illuminated by light, the light is scattered and/or reflected back toward the tip electrode 27, where

such light having interacted or otherwise having been affected by the lesion bears qualitative and quantitative information about the lesion 113 as it is recaptured by the hollow cavity 29 via the collection openings 87, 87', 87" of the tip electrode. Light recaptured from the tissue is collected in the hollow cavity 29 of the tip electrode. The receiving fiber optic cable 43R receives the recaptured light which bears the qualitative and quantitative information and is transmitted to an optical processing system, as described below in further detail.

**[0065]** In accordance with the present invention, the tip electrode 27 provides separate optical paths for the light that illuminates tissue and the light recaptured from the tissue which are optically isolated from each other by the shell wall 38, the passages 97 and/or the coating 47 on the emitting fiber optic cables 43E. The optical path from the tip electrode to the tissue begins with light that is injected into the illumination openings 89 via the fiber optic cables 43E which is reflected by the semi-spherical apex 93 and diffusely scattered by the filler 150 into multiple angles and directions before exiting the illumination openings 89 of the tip electrode 37. Exiting the tip electrode 27 from the illumination openings 89, the light is incidental on the tissue of interest, interacts with the tissue and is reflected or scattered back to the tip electrode from the tissue. The separate optical path from the tissue back to the tip electrode begins with entry through the collection openings 87 and then collection in the hollow cavity 29 where the light is received by the fiber optic cable 43E.

**[0066]** It is understood that the fiber optic cables 43E and 43R may be any suitable optical wave guide wherein light introduced at one of the cable is guided to the other end of the cable with minimal loss. Each of the cables 43E and 43R may be a single fiber optic cable or fiber bundles. They may be single mode (also known as mono-mode or uni-mode), multi-mode (with step index or graded index) or plastic optical fiber (POF), depending on a variety of factors, including but not limited to transmission rate, bandwidth of transmission, spectral width of transmission, distance of transmission, diameter of cable, cost, optical signal distortion tolerance and signal attenuation, etc. Moreover, light delivery and collection may be accomplished with other devices, such as air-core fibers, hollow waveguides, liquid waveguides and the like.

**[0067]** Included in the present invention is a method for manufacturing the tip electrode 27. The method includes providing a rod of a suitable diameter and length, constructed of a suitable material that is thermally and electrically conductive which allows for radio frequency ablation using an RF generator. Such suitable material may include, without limitation, platinum-iridium, platinum, gold alloy, or palladium alloy. To form the shell 38, the distal end of the rod is turned to form the distal dome end 31 and the interior is drilled in the longitudinal direction of the rod from the proximal end 33 to form the hollow cavity 29 and the distal dome cavity 73. The term drilling as used herein includes mechanical drilling, chemical or

laser etching, or the like.

**[0068]** The passages 97 are also drilled in the rim region 37 from the proximal end 33 through the hollow cavity 29 toward the distal dome end 31. The illumination openings 89 are drilled radially from outside the shell 38 through to the passages 97. It is understood that the illumination openings 89 can be drilled before or after the drilling of the passages 97, so long as the two structures connect and are in communication, and in turn, the hollow cavity 29 and the outside of the tip electrode are in communication with each other via the passages 97 and the illumination openings 89.

**[0069]** The collection openings 87, 87', 87" are also drilled radially from outside the shell 38 so there is communication between outside the tip electrode and the hollow cavity 29. The openings 87 can be formed before or after the formation of the illumination openings 89 and passages 97.

**[0070]** To form the plug, a rod of the aforementioned suitable material with a suitable diameter and length is provided. The passages 108, 112, 114 and 116 for the fiber optic cables 43 are drilled. The plug is press-fitted or soldered into the proximal opening of the tip electrode, but preferably after the fiber optic cables 43E and 43R are received in the passages 108, 112, 114 and 116 and the fiber optic cables 43E are inserted into the passages 97. After the plug 44 is press-fitted or soldered into the shell 38, glue, adhesive or the like is injected into the passages 108, 112 and 116 to fix the portions of the fiber optic cables extending through the passages. These fixed portions secure the fiber optic cables, particularly those of cables 43E, stationary within the tip electrode as a measure against breakage in or detachment from the tip electrode. The blind holes and other passages in the plug can be drilled before or after the plug is press-fitted into the shell 38. Methods for manufacturing a shell and a plug are disclosed in 11/058,434; filed February 14, 2005, the entire disclosure of which is hereby incorporated by reference.

**[0071]** The shell 28 of the tip electrode 27 may have an actual length, i.e., from its distal end to its proximal end, between about 2.0 mm to about 8.0. The plug 44 of the tip electrode may have an actual length, i.e., from its distal end to its proximal end, between about 1.0 mm to about 4.0 mm. The tip electrode as a combination of the shell and the plug may have an actual length, i.e., from its distal end to its proximal end, between about 2.5 mm to about 11 mm. Preferably the tip electrode 27 has a diameter about the same as the outer diameter of the tubing 19 of the intermediate section 14.

**[0072]** To keep the collection openings of the tip electrode 27 generally free from obstruction from blood or other bodily fluids and tissue encountered by the tip electrode 37, the tip electrode is irrigated with fluid, e.g., saline, that is fed into the hollow cavity by an irrigation tube 48, as shown in FIG. 4A. The irrigation tube 48 extends through the central lumen 18 of the catheter body 12 (FIG. 2A), the fourth lumen 35 of the intermediate section 14

(FIG. 3), through the plastic housing 21 and passage 110 in the plug 44 (FIG. 12). The tube 48 is anchored in the passage 110 and in the fourth lumen 35 by polyurethane glue or the like. The proximal portion of the tube 48 extends through the control handle 16 and terminates in a luer hub 90 (FIG. 1) or the like at a location proximal to the control handle. In the disclosed embodiment, the irrigation tube 48 transitions from a smaller diameter at the distal end to a larger diameter at the proximal end. For example, a distal segment can be about 0.0155 x 0.0175 inches and a proximal segment can be about 0.024 x 0.28 inches. In practice, fluid may be injected by a pump (not shown) into the irrigation tube 48 through the luer hub 90, and into the hollow cavity 29 in the tip electrode 27, and out the collection openings. The infusion tube 48 may be made of any suitable material, and is preferably made of polyimide tubing.

**[0073]** In accordance with a feature of the present invention, the pump maintains the fluid at a positive pressure differential relative to outside the hollow cavity 29 so as to provide a constant unimpeded flow or seepage of fluid outwardly from the hollow cavity 29 which continuously flushes the collection openings and minimizes obstruction so light can freely pass through for the aforementioned light collection purposes. In addition to the above, the irrigation adaptation of the catheter 10 may serve other typical functions such as cooling the tip electrode and/or the ablation site and increasing conduction for deeper and larger lesions.

**[0074]** To energize the tip electrode 27 for RF ablation, the lead wire 40 is anchored in the plug 44. With reference to FIG. 1, 2A and 5, the lead wire 40 extends through the second lumen 32 of intermediate section 14, the central lumen 18 of the catheter body 12, and the control handle 16, and terminates at its proximal end in an input jack (not shown) that may be plugged into an appropriate monitor (not shown). The portion of the lead wire 40 extending through the central lumen 18 of the catheter body 12, control handle 16 and distal end of the intermediate section 14 is enclosed within a protective sheath 52, which can be made of any suitable material, preferably Teflon RTM.. The protective sheath 52 is anchored at its distal end to the distal end of the intermediate section 14 by gluing it in the lumen 32 with polyurethane glue or the like. The lead wire 40 is attached to the tip electrode 27 by any conventional technique. In the illustrated embodiment, connection of the lead wire 40 to the tip electrode 27 is accomplished, for example, by welding the distal end of the lead wire 40 into the blind hole 102 (FIGs. 12 and 12A) in the plug 44 of the tip electrode 27.

**[0075]** A temperature sensing means is provided for the tip electrode 27 in the disclosed embodiment. Any conventional temperature sensing means, e.g., a thermocouple or thermistor, may be used. With reference to FIGs 12. and 12B, a suitable temperature sensing means for the tip electrode 27 comprises a thermocouple formed by a wire pair. One wire of the wire pair is the copper wire 41, e.g., a number 40 copper wire. The other wire of the



wire pair is the constantan wire 45, which gives support and strength to the wire pair. The wires 41 and 45 of the wire pair are electrically isolated from each other except at their distal ends where they contact and are twisted together, covered with a short piece of plastic tubing 63, e.g., polyimide, and covered with epoxy. The plastic tubing 63 is then attached in the hole 104 of the plug 44, by epoxy or the like. As shown in FIGs. 2A, 3 and 5, the wires 41 and 45 extend through the second lumen 32 in the intermediate section 14. Within the catheter body 12 the wires 41 and 45 extend through the central lumen 18 within the protective sheath 52 along with the lead wires 40. The wires 41 and 45 then extend out through the control handle 16 and to a connector (not shown) connectable to a temperature monitor (not shown). Alternatively, the temperature sensing means may be a thermistor. A suitable thermistor for use in the present invention is Model No. AB6N2-GC14KA143T/37C sold by Thermometrics (New Jersey).

**[0076]** The embodiment of the catheter disclosed herein is uni-deflectional, having a single puller wire; however, it is understood by one of ordinary skill in the art that the catheter may be bidirectional with two puller wires. Referring to FIG. 2B, the puller wire 42 for deflecting the intermediate section 14 extends through the catheter body 12 and is anchored at its proximal end to the control handle 16. The puller wire is made of any suitable metal, such as stainless steel or Nitinol, and is preferably coated with Teflon.RTM. or the like. The coating imparts lubricity to the puller wire. The puller wire preferably has a diameter ranging from about 0.006 to about 0.010 inches. A compression coil 56 is situated within the catheter body 12 in surrounding relation to the puller wire. The compression coil 56 extends from the proximal end of the catheter body 12 to the proximal end of the intermediate section 14. The compression coil is made of any suitable metal, preferably stainless steel, and is tightly wound on itself to provide flexibility, i.e., bending, but to resist compression. The inner diameter of the compression coil is preferably slightly larger than the diameter of the puller wire 42. The Teflon.RTM. coating on the puller wire allows it to slide freely within the compression coil. If desired, particularly if the lead wire 40 is not enclosed by the protective sheath 52, the outer surface of the compression coils can be covered by a flexible, non-conductive sheath, e.g., made of polyimide tubing, to prevent contact between the compression coils and any other wires within the catheter body 12.

**[0077]** As shown in FIG. 2B, the compression coil 56 is anchored at its proximal end to the proximal end of the stiffening tube 20 in the catheter body 12 by glue joint 50 and at its distal end to the intermediate section 14 by glue joint 51. Both glue joints 50 and 51 preferably comprise polyurethane glue or the like. The glue may be applied by means of a syringe or the like through a hole made between the outer surface of the catheter body 12 and the central lumen 18. Such a hole may be formed, for example, by a needle or the like that punctures the outer

wall 22 of the catheter body 12 and the stiffening tube 20 which is heated sufficiently to form a permanent hole. The glue is then introduced through the hole to the outer surface of the compression coil 56 and wicks around the outer circumference to form a glue joint about the entire circumference of the compression coil.

**[0078]** With reference to FIGs. 2B and 5, the puller wire 42 extends into the first lumen 30 of the intermediate section 14. In the illustrated embodiment of FIG. 3B, the distal end of the puller wire 42 is anchored to the distal end side wall of the first lumen 30 of the tubing 19 of the intermediate section 14. The distal end of the puller wire 42 is anchored by means of a T-bar anchor 109 created by a metal tube 120, e.g., a short segment of hypodermic stock, that is fixedly attached, e.g. by crimping, to the distal end of the puller wire 42. The tube has a section that extends a short distance beyond the distal end of the puller wire 42. A cross-piece 121 made of a small section of stainless steel ribbon or the like is soldered or welded in a transverse arrangement to the distal end of the metal tube which is flattened during the operation. A notch is created in the side wall of tubing 19 resulting in an opening in the lumen 30 carrying the puller wire 42. The cross piece 121 lies transversely within the notch. Because the length of the ribbon forming the cross-piece 121 is longer than the diameter of the opening into the lumen 30, the anchor 109 cannot be pulled completely into the lumen 30. The notch is then sealed with polyurethane glue 122 or the like to give a smooth outer surface. The glue flows into the lumen 30 to fully secure the anchor. A t-bar anchor is described in US Patent No. 6468260, the entire disclosure of which is hereby incorporated by reference. Other means for anchoring the distal end of the puller wire 42 would be recognized by those skilled in the art and are included within the scope of the invention. For example, another blind hole 101 (FIG. 12C) may be formed in the proximal surface of the plug 44 in which the metal tube 120 at the distal end of the puller wire may be fixed by soldering.. Anchoring the puller wire 42 within the tip electrode 27 provides additional support, reducing the likelihood that the tip electrode 27 will fall off. Within the first lumen 30 of the intermediate section 14, the puller wire 42 extends through a plastic, preferably Teflon.RTM., sheath 81, which prevents the puller wire 42 from cutting into the wall of the intermediate section 14 when the intermediate section is deflected. Longitudinal movement of the puller wire 42 relative to the catheter body 12, which results in deflection of the tip section 36, is accomplished by suitable manipulation of the control handle 16. Suitable control handles are described in US Patent No. 6602242, the entire disclosure of which is hereby incorporated by reference.

**[0079]** In the illustrated embodiment, the tip section 36 carries an electromagnetic sensor 72, and as mentioned, the electromagnetic sensor may be carried in the plastic housing 21, with its distal end anchored in the blind hole 106 in the plug 44 as shown in FIGs. 4A, 4B and 12. The electromagnetic sensor 72 is connected to an electro-

magnetic sensor cable 74. As shown in FIGS. 2A and 5, the sensor cable 74 extends through the third lumen 34 of the tip section 36, through the central lumen 18 of the catheter body 12, and into the control handle 16. The electromagnetic sensor cable 74 then extends out the proximal end of the control handle 16 within an umbilical cord 78 (FIG. 1) to a sensor control module 75 that houses a circuit board (not shown). Alternatively, the circuit board can be housed within the control handle 16, for example, as described in U.S. Patent application Ser. No. 08/924,616, entitled "Steerable Direct Myocardial Revascularization Catheter", the disclosure of which is incorporated herein by reference. The electromagnetic sensor cable 74 comprises multiple wires encased within a plastic covered sheath. In the sensor control module 75, the wires of the electromagnetic sensor cable 74 are connected to the circuit board. The circuit board amplifies the signal received from the electromagnetic sensor 72 and transmits it to a computer in a form understandable by the computer by means of the sensor connector 77 at the proximal end of the sensor control module 75, as shown in FIG. 1. Because the catheter can be designed for single use only, the circuit board may contain an EPROM chip which shuts down the circuit board approximately 24 hours after the catheter has been used. This prevents the catheter, or at least the electromagnetic sensor, from being used twice. Suitable electromagnetic sensors for use with the present invention are described, for example, in U.S. Pat. Nos. 5,558,091, 5,443,489, 5,480,422, 5,546,951, 5,568,809, and 5,391,199 and International Publication No. WO 95/02995, the disclosures of which are incorporated herein by reference. An electromagnetic mapping sensor 72 may have a length of from about 6 mm to about 7 mm and a diameter of about 1.3 mm.

**[0080]** With reference to FIG. 13, an optical processing system 126 for optically evaluating ablation tissue using the catheter 10 is illustrated. A light source 128 supplies a broadband (white; multiple wavelengths) light and/or laser light (single wavelength) radiation to the tip section 36 of the catheter 10 via cable 127 which is split by a beamsplitter 131 outputting to the emitting cables 43E. The light bearing lesion qualitative information from the tip section is transmitted by the receiving cable 43R to a detection component 130. The detection component may comprise, for example, a wavelength selective element 131 that disperses the collected light into constituent wavelengths, and a quantification apparatus 140. The at least one wavelength selective element 131 includes optics 132, as are known in the art, for example, a system of lenses, mirrors and/or prisms, for receiving incident light 134 and splitting it into desired components 136 that are transmitted into the quantification apparatus 140.

**[0081]** The quantification apparatus 140 translates measured light intensities into an electrical signal that can be processed with a computer 142 and displayed graphically to an operator of the catheter 10. The quantification apparatus 140 may comprise a charged coupled

device (CCD) for simultaneous detection and quantification of these light intensities. Alternatively, a number of different light sensors, including photodiodes, photomultipliers or complementary metal oxide semiconductor (CMOS) detectors may be used in place of the CCD converter. Information is transmitted from the quantification device 140 to the computer 142 where a graphical display or other information is generated regarding parameters of the lesion. A suitable system for use with the catheter 10 is described in U.S. Application Serial No. 11/281179 and Serial No. 11/281853, the entire disclosures of which are hereby incorporated by reference.

**[0082]** The preceding description has been presented with reference to presently preferred embodiments of the invention. Workers skilled in the art and technology to which this invention pertains will appreciate that alterations and changes in the described structure may be practiced without meaningfully departing from the principal, spirit and scope of this invention. In that regard, the tip electrode may be configured with illumination and/or collection openings without regard to the configuration or location of the various sections of the tip electrode. Moreover, the tip electrode may be modified such that any type and number of openings can be placed anywhere on the tip electrode. For example, there could be multiple openings on the most distal section of the tip dome instead of a single opening, or there could be an illumination opening instead of a receiving opening. In addition, the openings can be of any shape, and are only limited by manufacturing methods available, such as laser drilling, photo-chemical etching, EDM machining, etc.

**[0083]** Accordingly, the foregoing description should not be read as pertaining only to the precise structures described and illustrated in the accompanying drawings, but rather should be read consistent with and as support to the following claims which are to have their fullest and fair scope.

## Claims

### 1. A catheter, comprising:

- a catheter body ;
- a tip electrode distal the catheter body, the tip electrode having a shell wall and a hollow cavity, the shell wall having at least an illumination opening and a collection opening;
- a first fiber optic cable in communication with the illumination opening;
- a second fiber optic cable in communication with the hollow cavity;

wherein light emitted from the first fiber optic cable exits the tip electrode to reach tissue through the illumination opening in defining a first path and returns to the tip electrode from the tissue into the hollow cavity through the collection opening in defining

- a second path, the first and second paths being optically isolated from each other within the tip electrode.
2. A catheter of claim 1, wherein the tip electrode further comprises a tube to provide fluid to flush the collection opening. 5
  3. A catheter of claim 1, wherein the first path includes (a) passage through the emitting fiber optic cable and (b) exit to outside the tip electrode through the illumination opening, and wherein the second path includes (a) passage through the collection opening, (b) collection in the hollow cavity, and (c) passage through the receiving fiber optic cable. 10
  4. A catheter of claim 1, wherein one of the fiber optic cables extends through the hollow cavity and is optically isolated from the hollow cavity. 15
  5. A catheter of claim 4, wherein the one fiber optic cable is optically isolated by a coating of reflective buffer material thereon. 20
  6. A catheter of claim 1, wherein the illumination opening has a semi-spherical cross section. 25
  7. A catheter of claim 1, wherein the illumination opening is filled with an optically scattering material. 30
  8. A catheter of claim 1, wherein the shell has a longitudinal axis and a first, second and third sections, the first section being generally perpendicular to the longitudinal axis, the second section being generally at an angle between about zero and 90 degrees to the longitudinal axis, and the third section being generally parallel to the longitudinal axis. 35
  9. A catheter of claim 8, wherein the first section has the collection opening and the second section has the illumination opening and the third section has another opening. 40
  10. A catheter of claim 8, wherein the first section is distal of the second section which is distal of the third section. 45
  11. A catheter of claim 8, wherein the first section has the collection opening, the second section has the illumination opening. 50
  12. A catheter of claim 8, wherein the second section has multiple illumination openings, and the third section has multiple collection openings, and wherein the openings within each section is equi-angular from each other about the longitudinal axis. 55
  13. A catheter of claim 1, wherein the hollow cavity includes a distal dome cavity.
  14. A catheter of claim 1, wherein the tip electrode include a plug sealing the hollow cavity.
  15. A catheter of claim 14, wherein the plug has passages through which fiber optic cables extend.
  16. A catheter of claim 15, wherein the fiber optic cables are fixed to the plug within the passages.
  17. A catheter of claim 1, wherein the tip electrode is adapted for RF ablation.
  18. A catheter of claim 8, wherein the angle of the second section is about 45 degrees.
  19. A catheter of claim 1, further comprising a deflectable intermediate section between the catheter body and the tip electrode.
  20. A catheter of claim 1, further comprising a temperature sensor.
  21. A catheter of claim 1, further comprising a location sensor.
  22. A method of making an omnidirectional tip electrode with isolated optical paths, comprising:
    - providing a shell with a hollow cavity;
    - configuring at least one collection opening in the shell wall;
    - configuring at least illumination opening in the shell wall;
    - providing an emitting fiber optic cable adapted to emit light into the illumination opening; and
    - providing a receiving fiber optic cable adapted to light collected in the hollow cavity;
    - providing an optical barrier between the emitting fiber optic cable and the hollow cavity.
  23. A method of claim 22, further comprising configuring a passage in the shell wall that connects with the illumination opening, wherein the passage receives a distal end of the emitting fiber optic cable.
  24. A method of claim 22, wherein the illumination opening has a semi-spherical cross section.
  25. A method of claim 22, wherein the shell has a wall defining a distal end and an open proximal end and the method further comprises forming a plug to seal with hollow cavity, wherein the plug is configured with passages for the fiber optic cables to extend through.
  26. A method of claim 25, further comprising fixedly securing portions of the fiber optic cables in the pas-

sages to the plug.

27. A method of claim 22, wherein the shell is made of thermally and electrically conductive material. 5
28. A method of claim 25, wherein the shell and the plug are made of thermally and electrically conductive material.
29. A method of claim 25, further comprising filling the illumination opening with a material having optical scattering property. 10
30. A method of claim 29, wherein the material is a scattering agent-filled epoxy or plastic to aid in the even distribution of light out of the opening. 15
31. A catheter, comprising:
- a catheter body; 20
  - a tip electrode distal the catheter body, the tip electrode having a shell wall and a hollow cavity, the shell wall having illumination openings and collection openings;
  - at least one emitting fiber optic cable in communication with at least one of the illumination openings; 25
  - at least one receiving fiber optic cable in communication with the hollow cavity; 30
- wherein light emitted from the at least one emitting fiber optic cable exits the tip electrode to reach tissue through at least the one illumination opening in defining a first path and returns to the tip electrode from the tissue into the hollow cavity through the collection opening in defining a second path, the first and second paths being optically isolated from each other within the tip electrode. 35

40

45

50

55

FIG.1

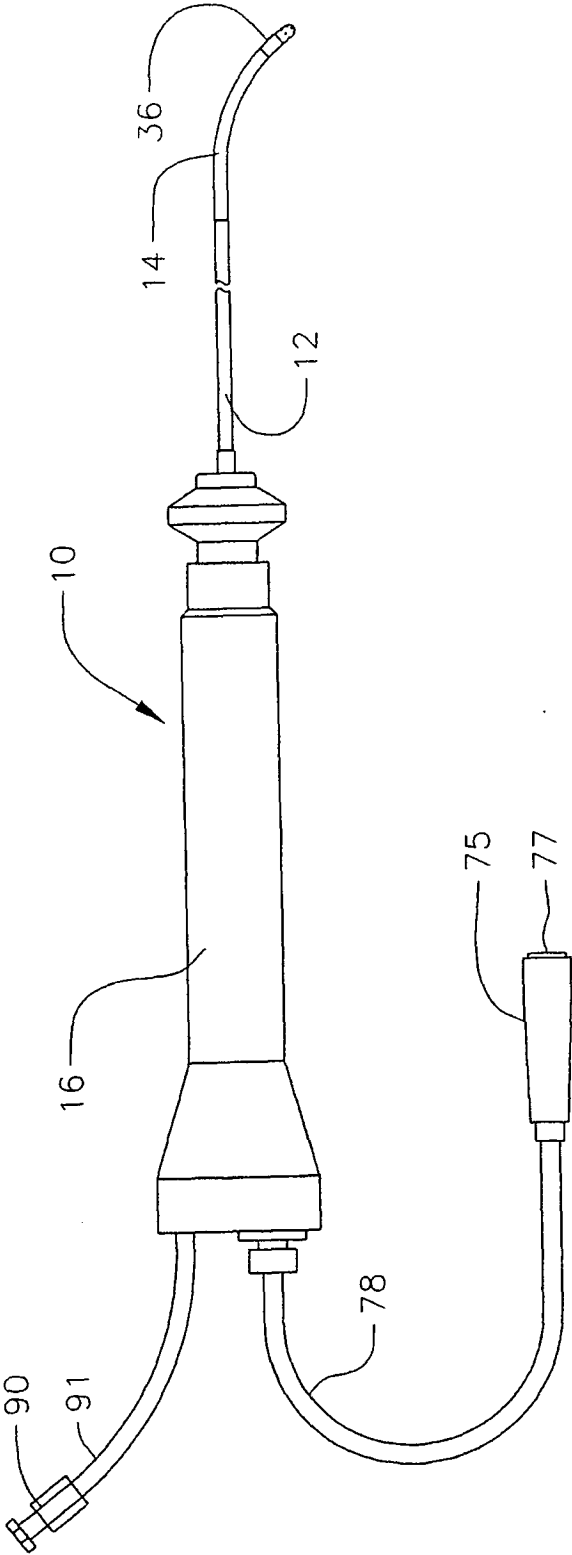


FIG. 2A

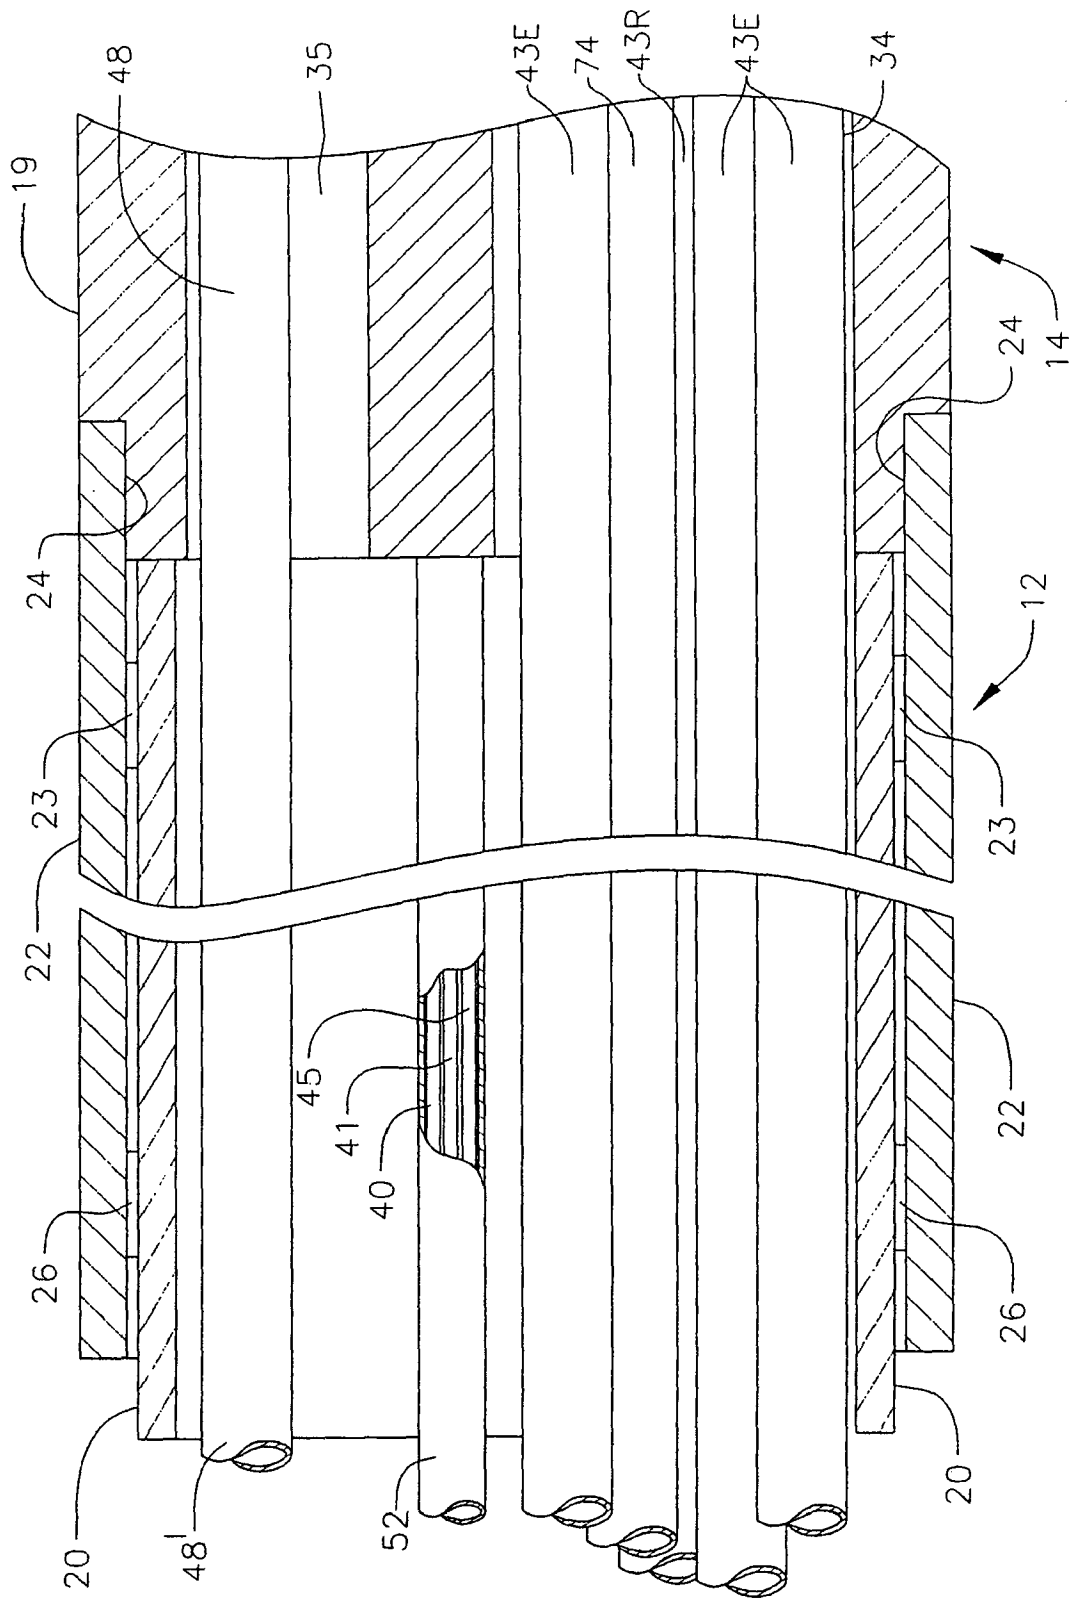
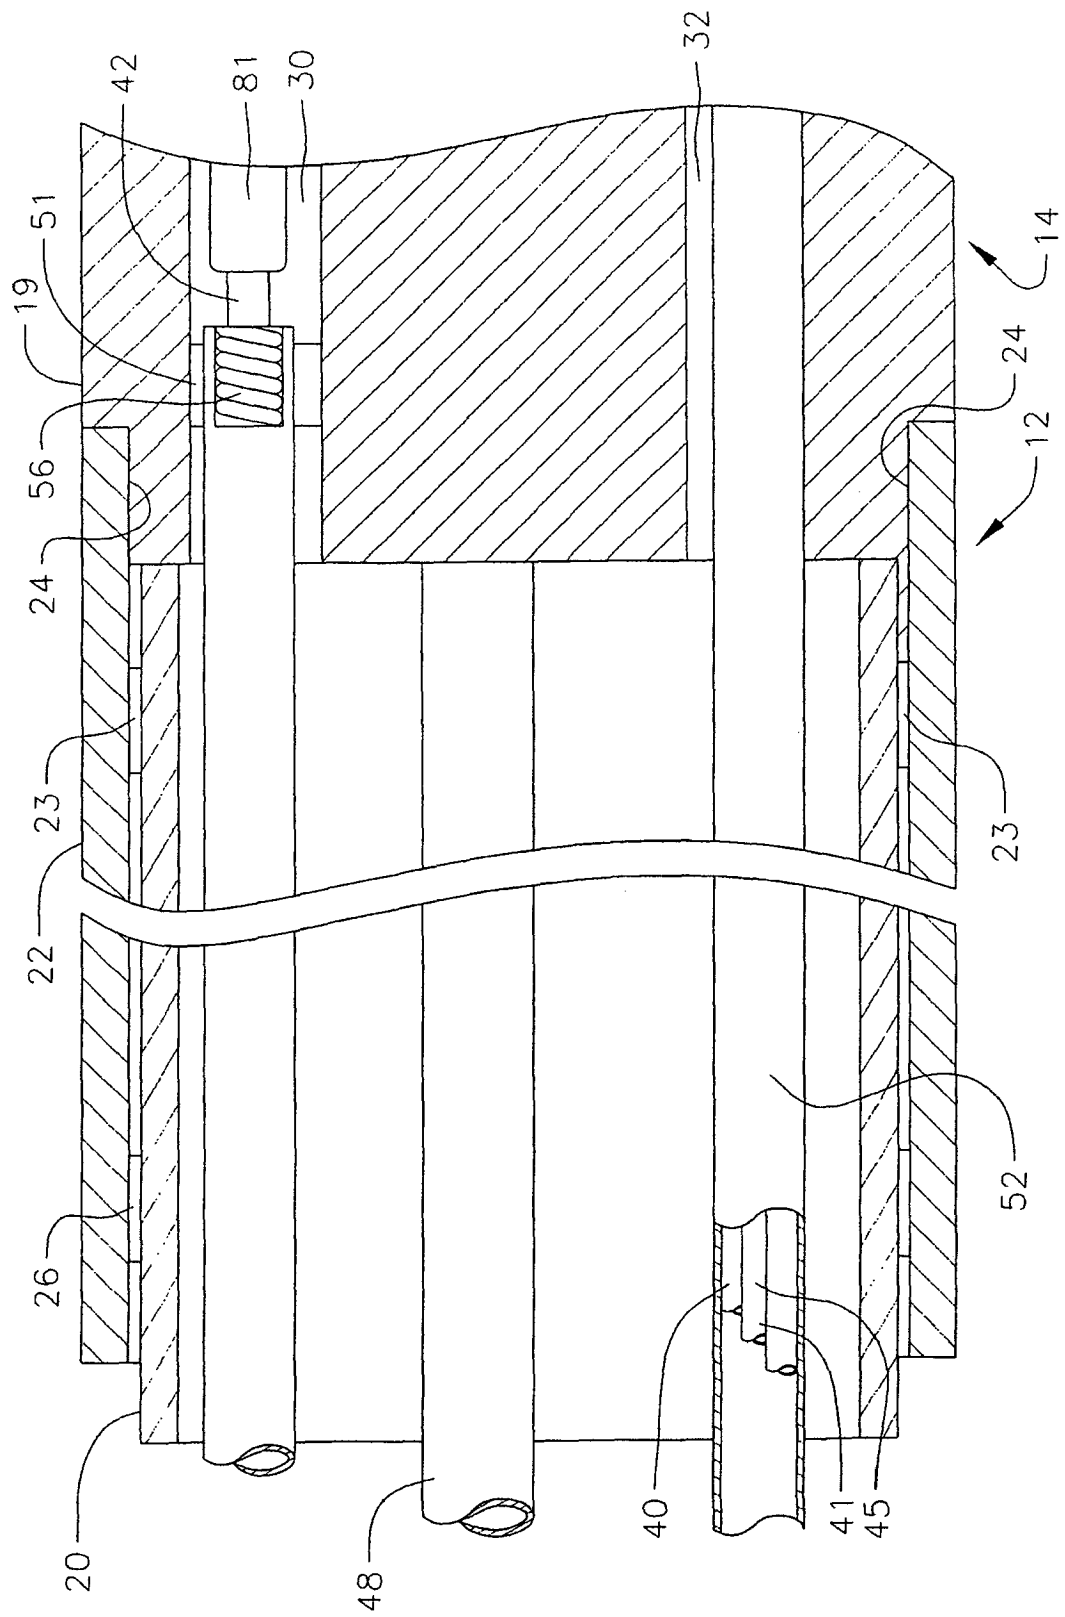
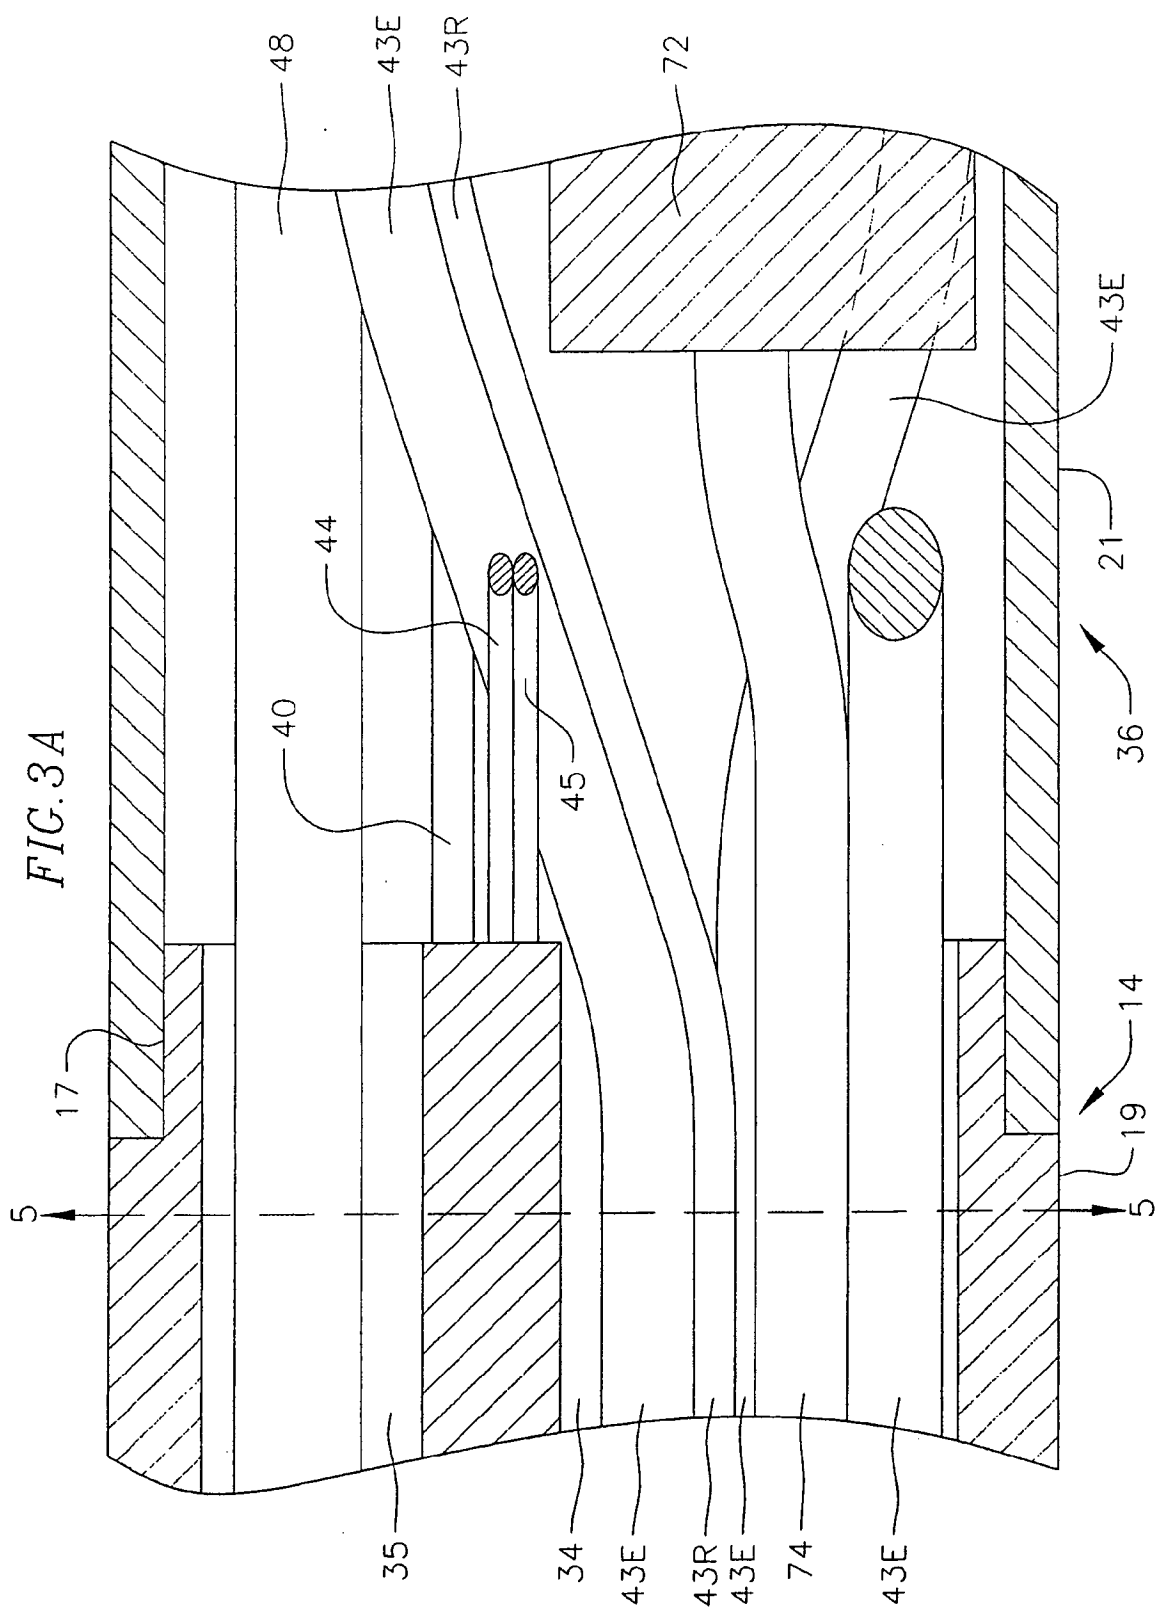
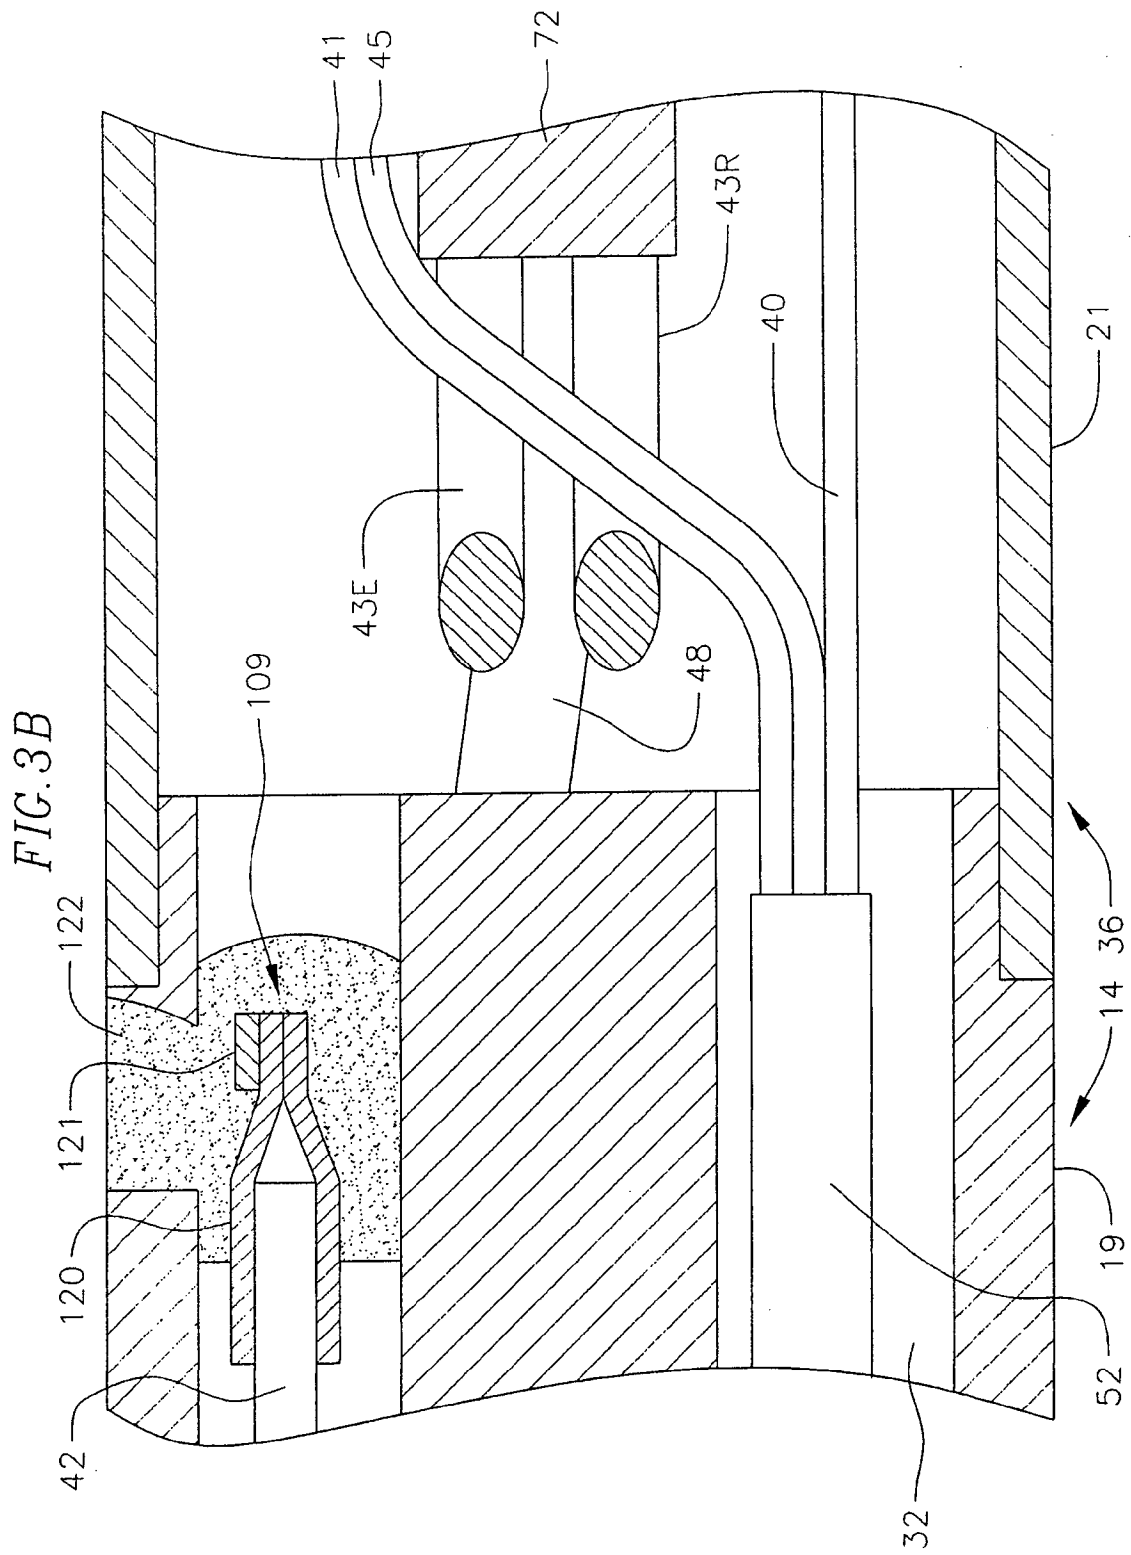



FIG. 2B









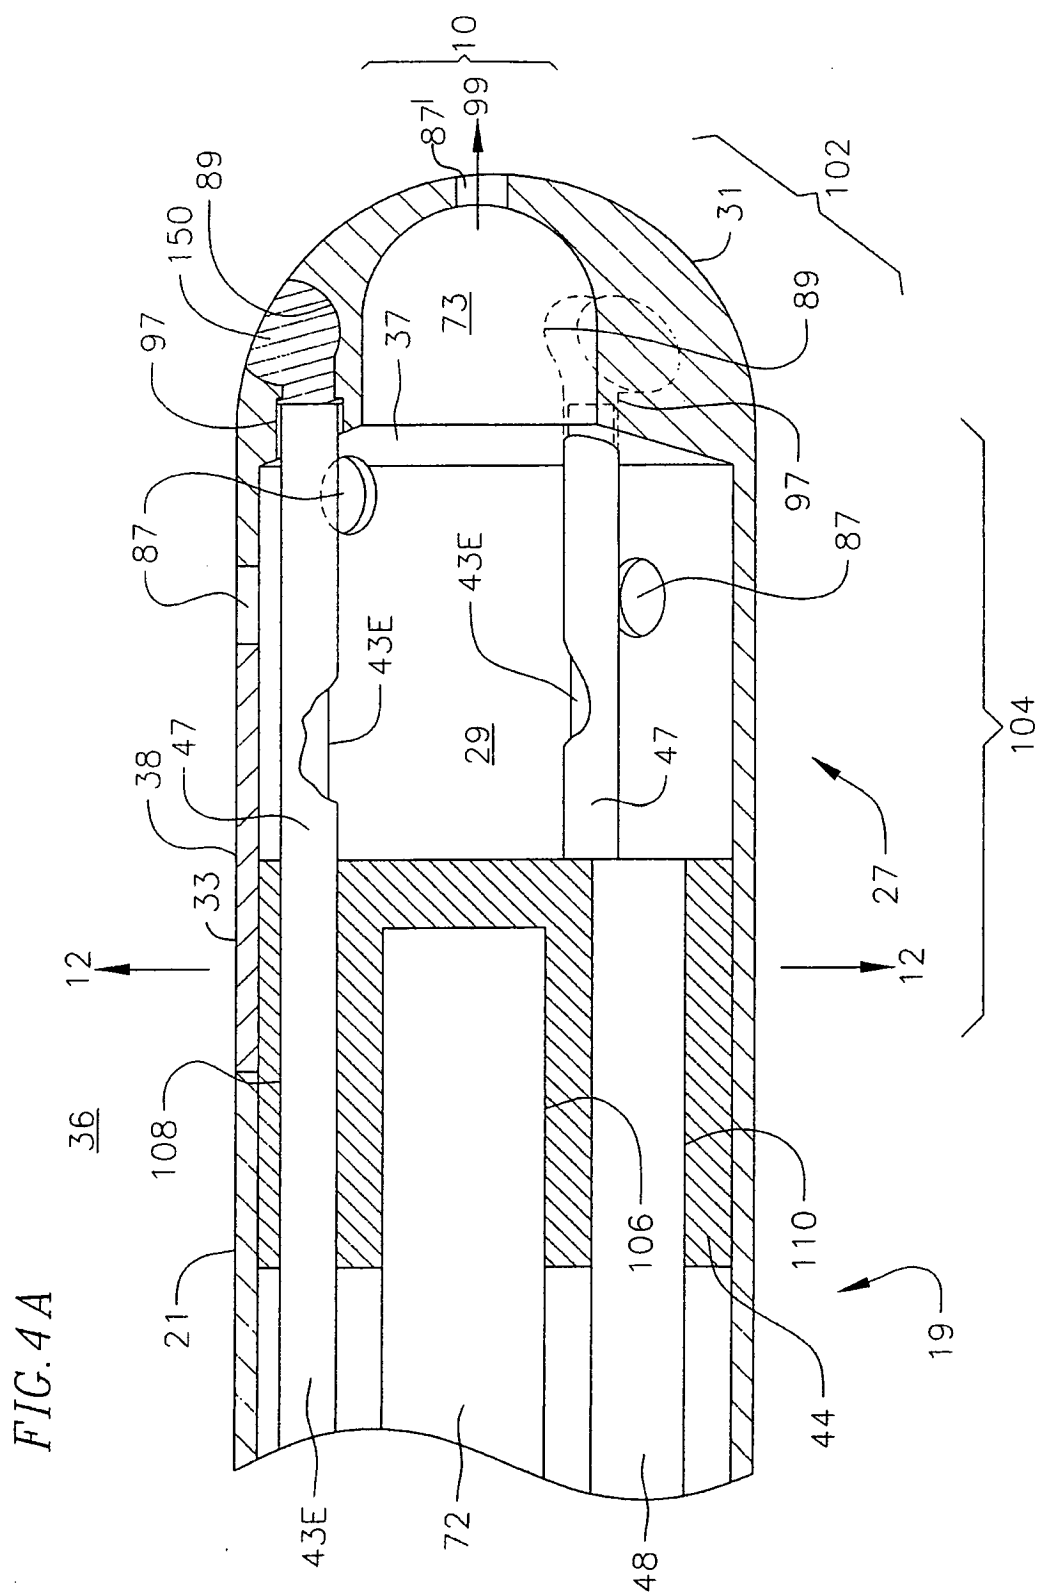

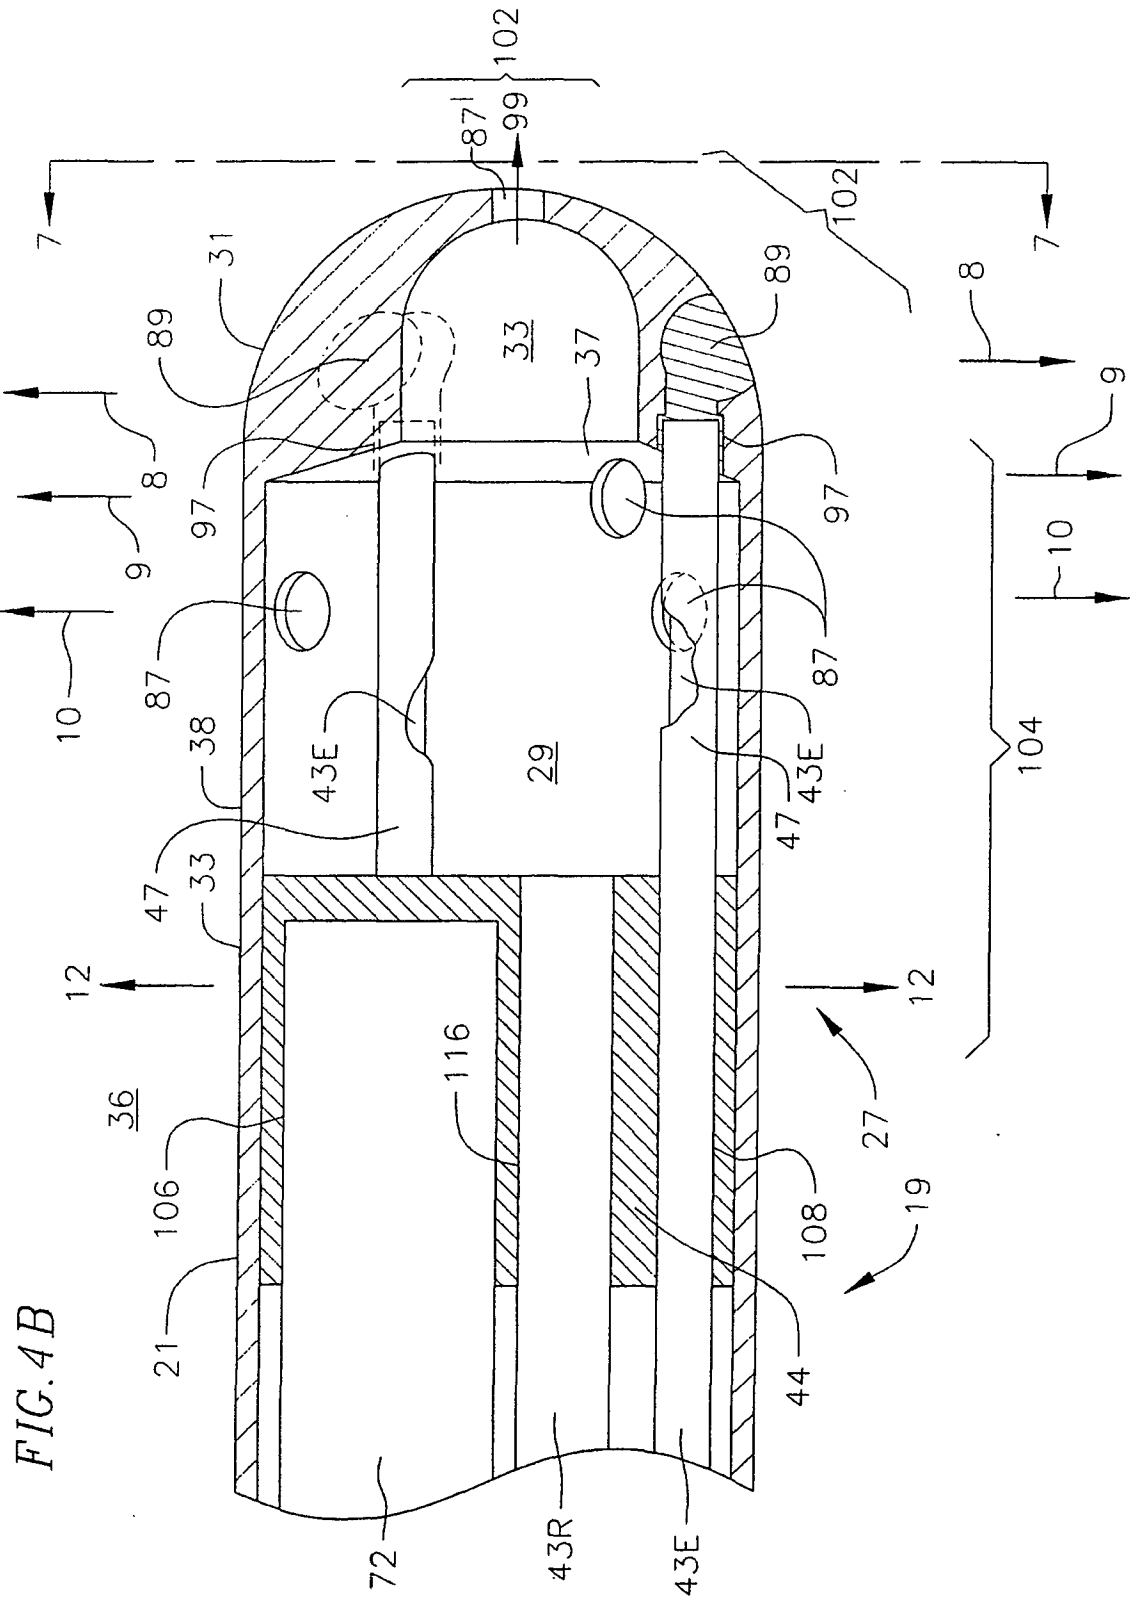


FIG. 5

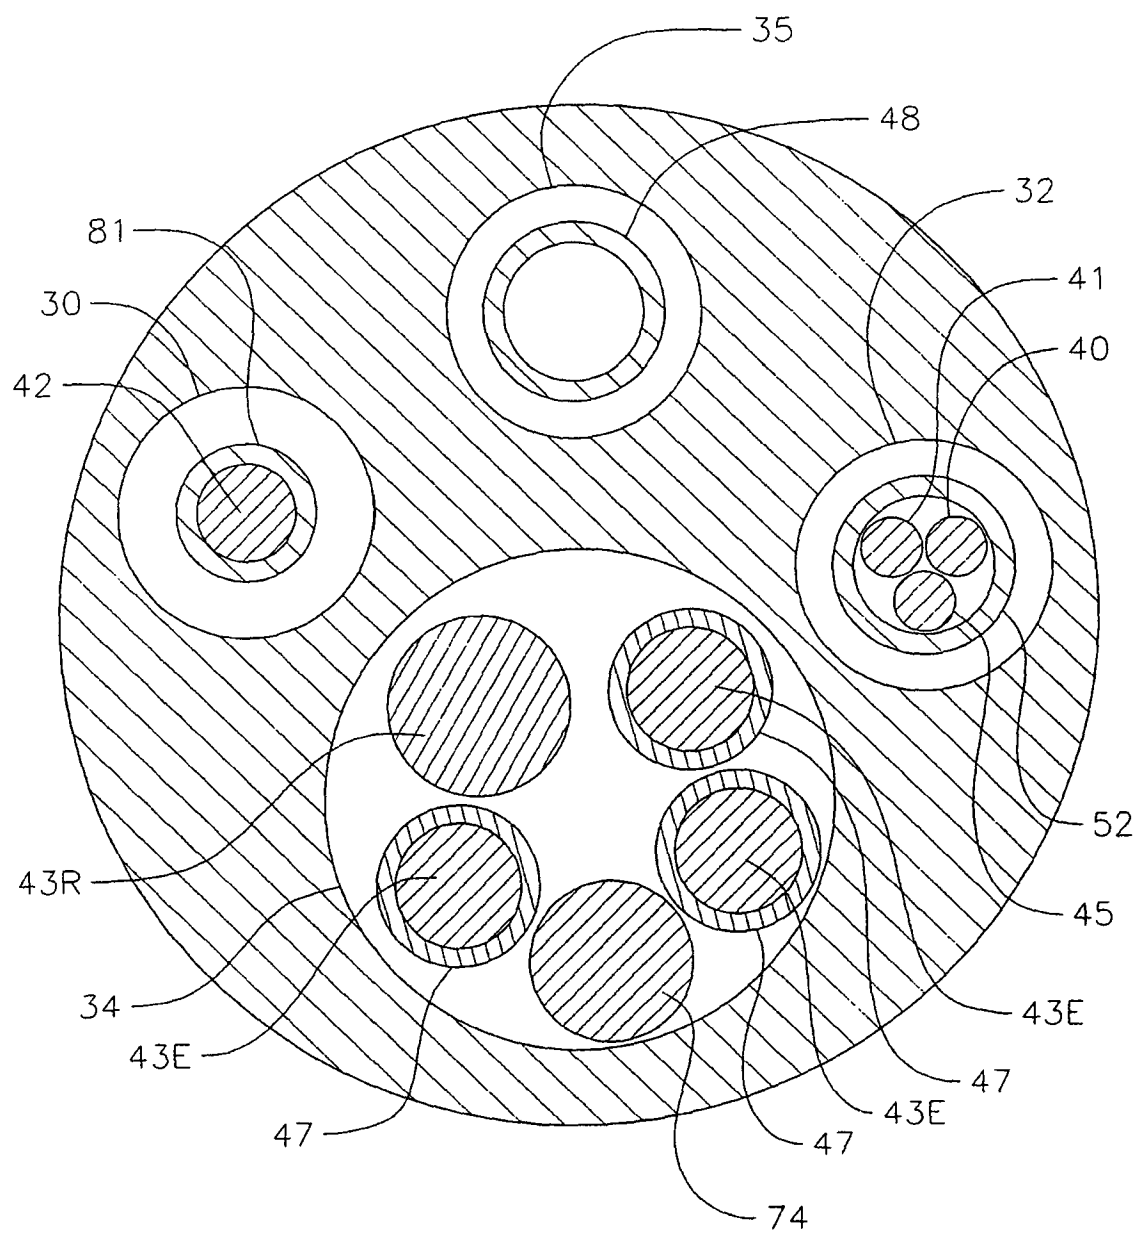
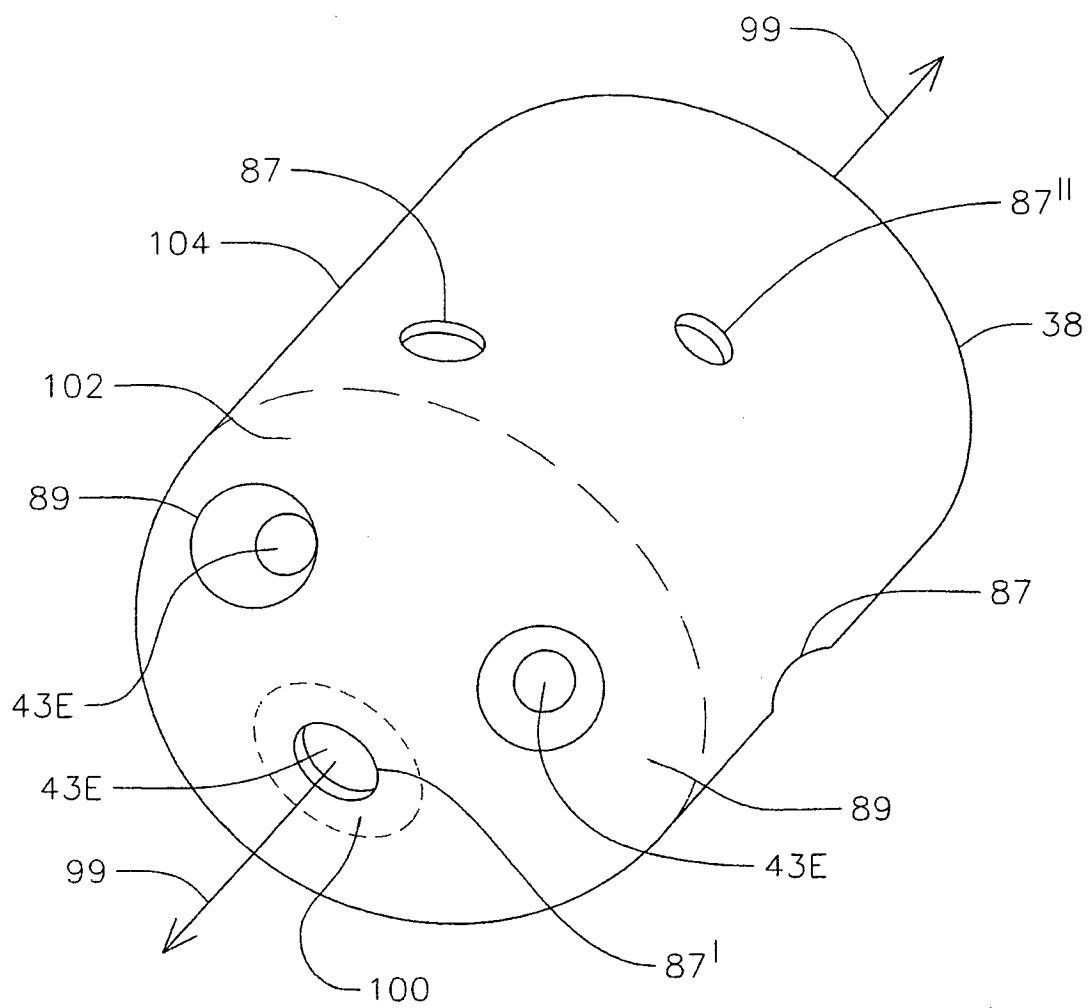


FIG. 6



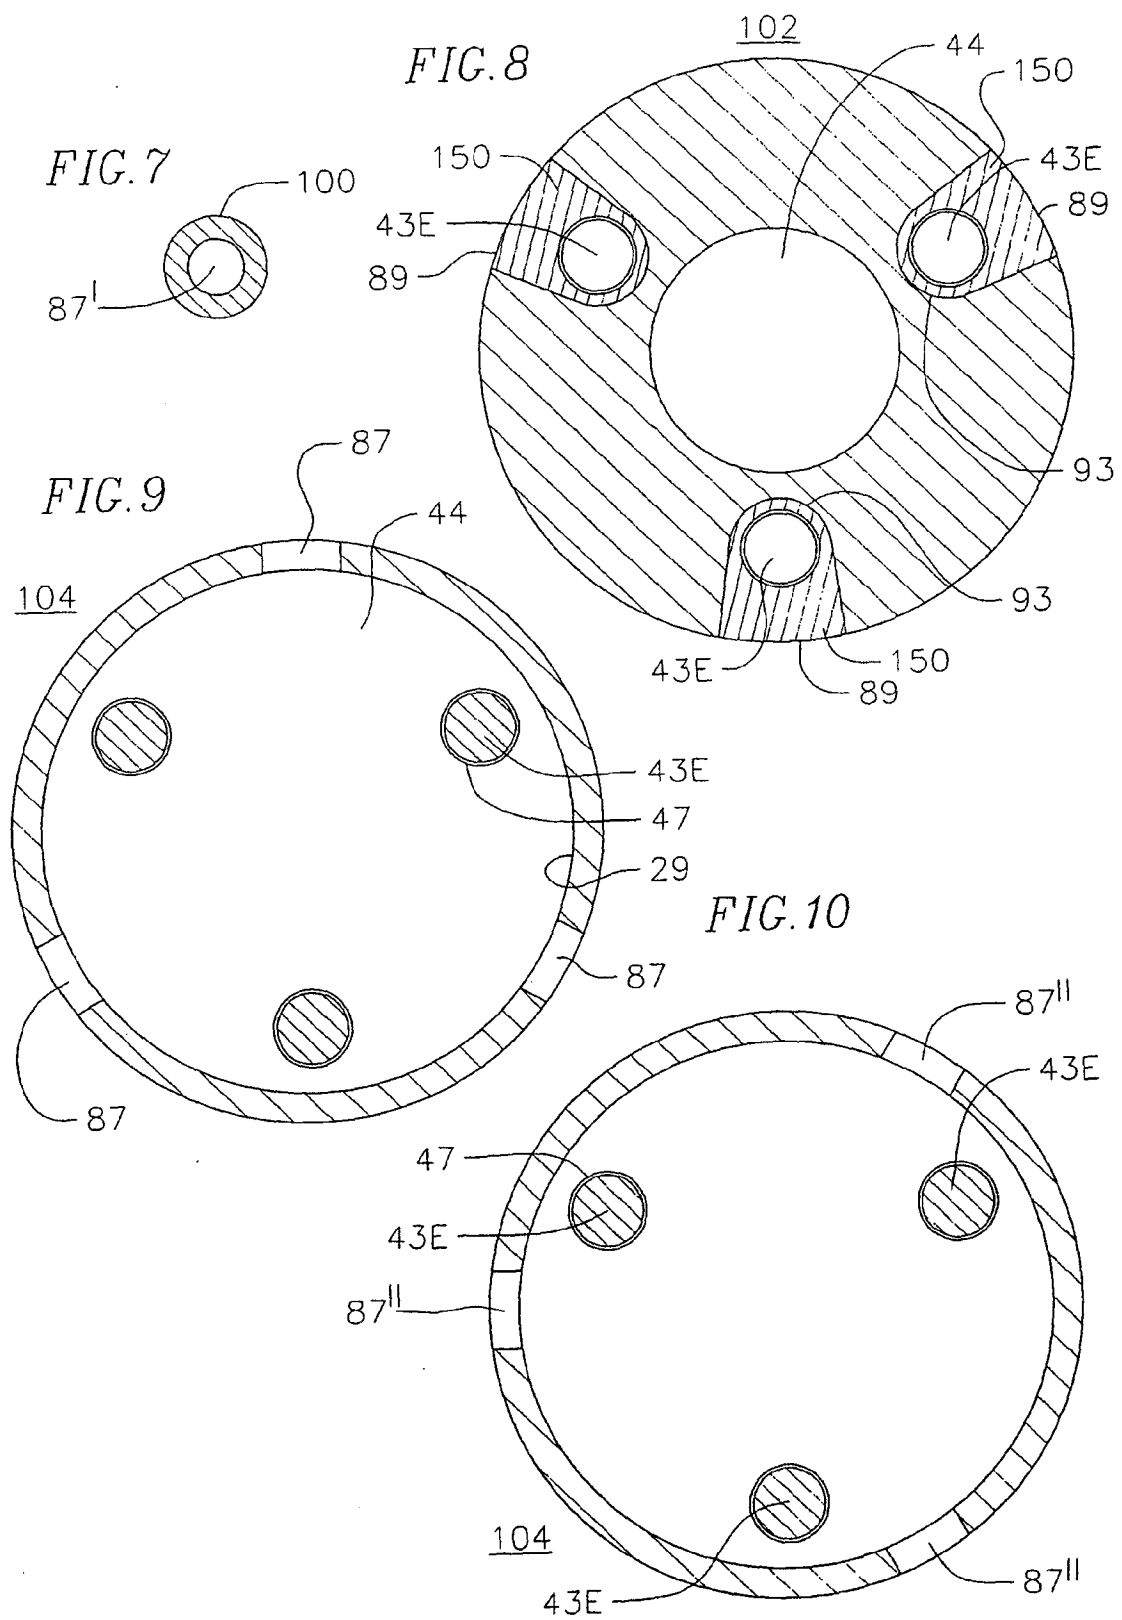


FIG. 11A

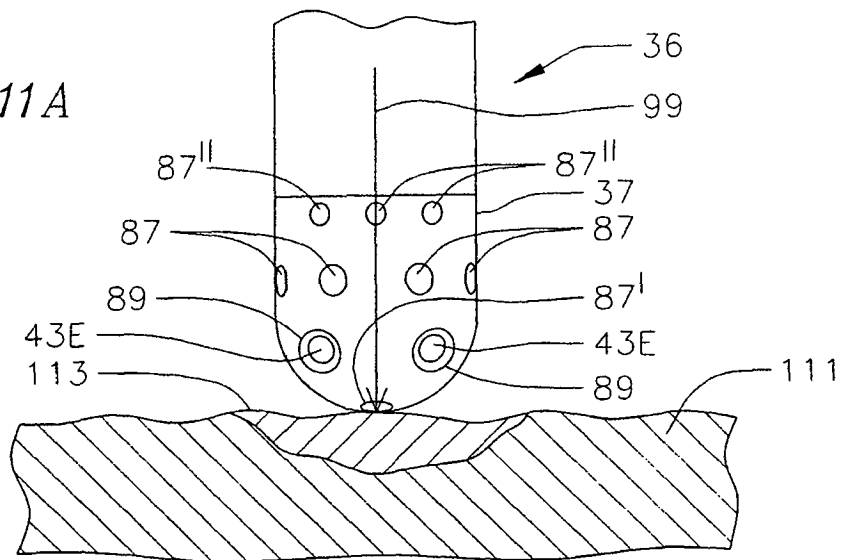


FIG. 11B

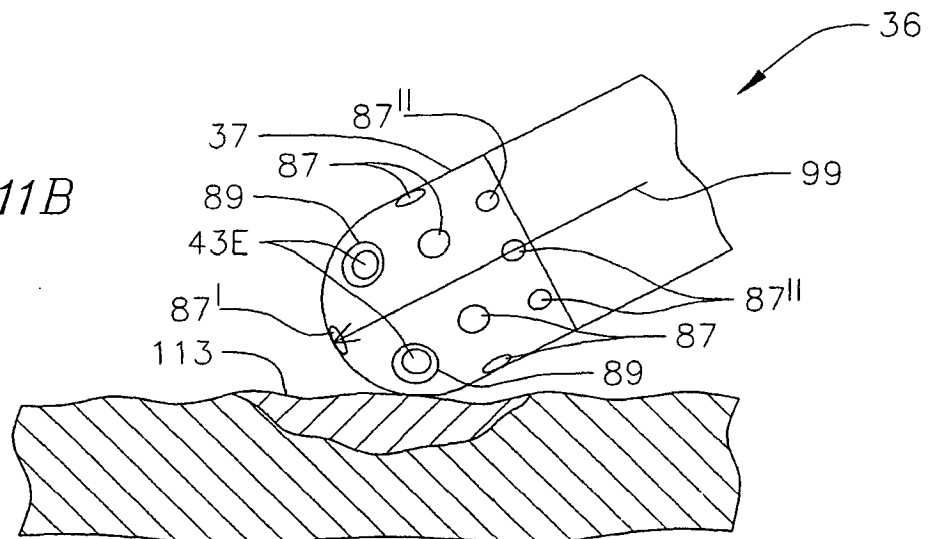


FIG. 11C

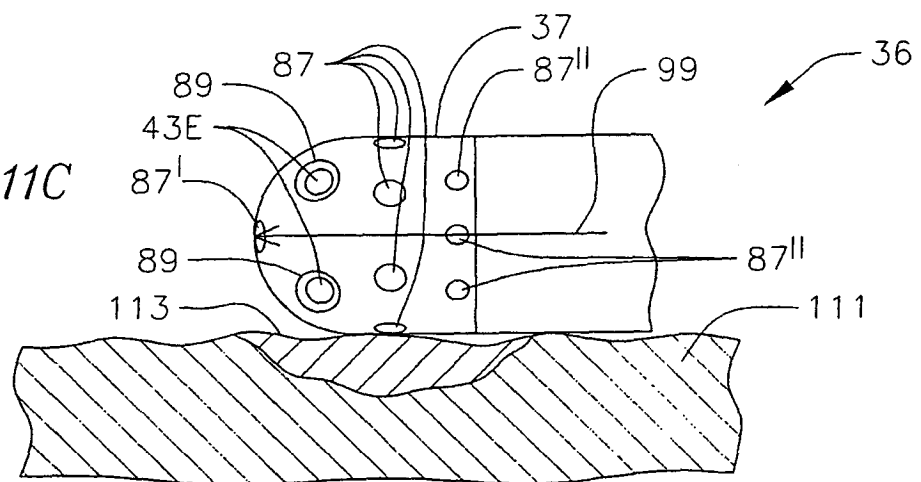


FIG. 12

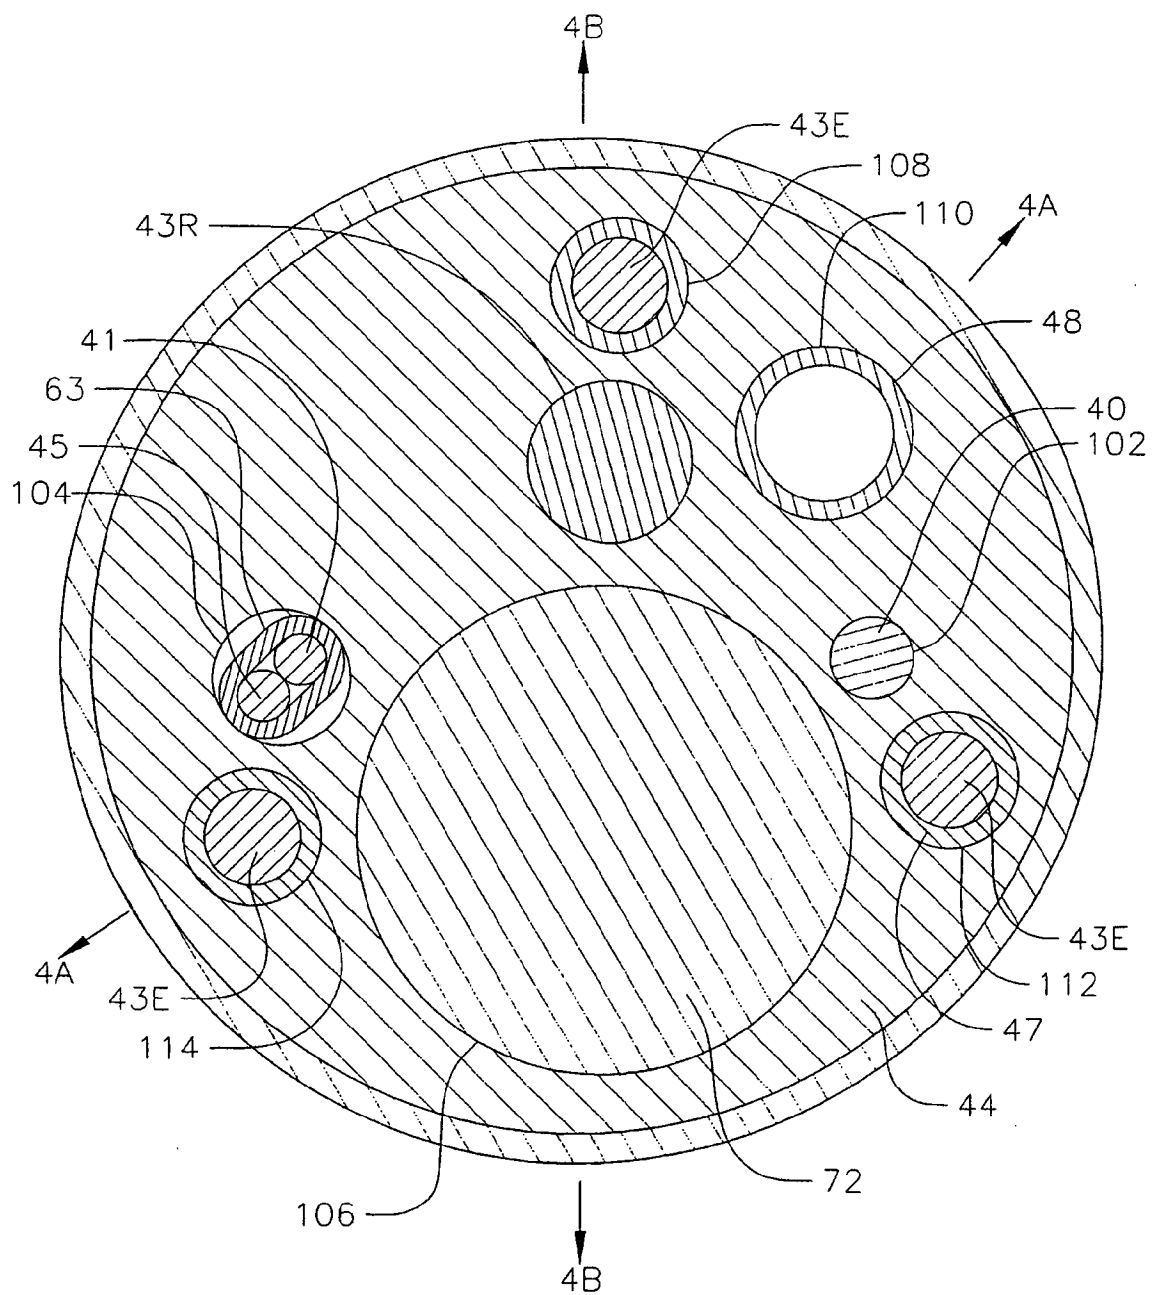




FIG.12A

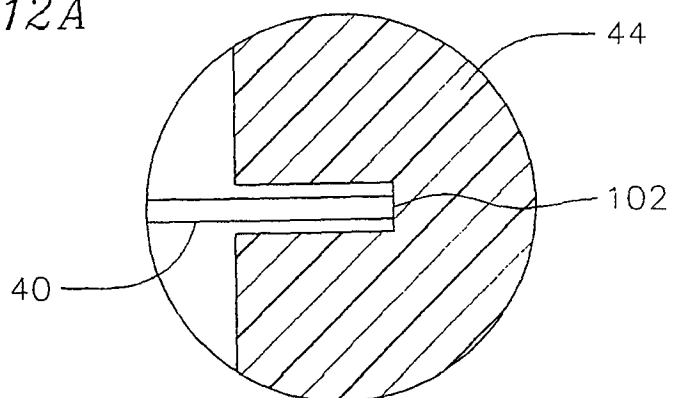


FIG.12B

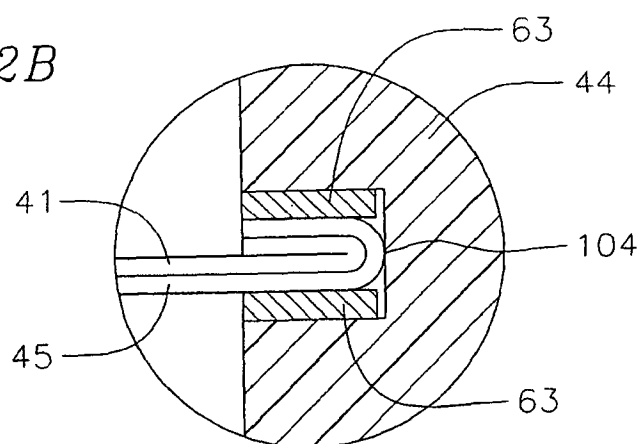


FIG.12C


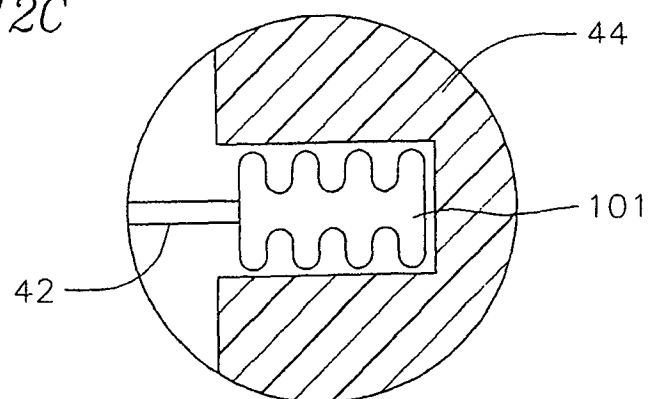


FIG. 13



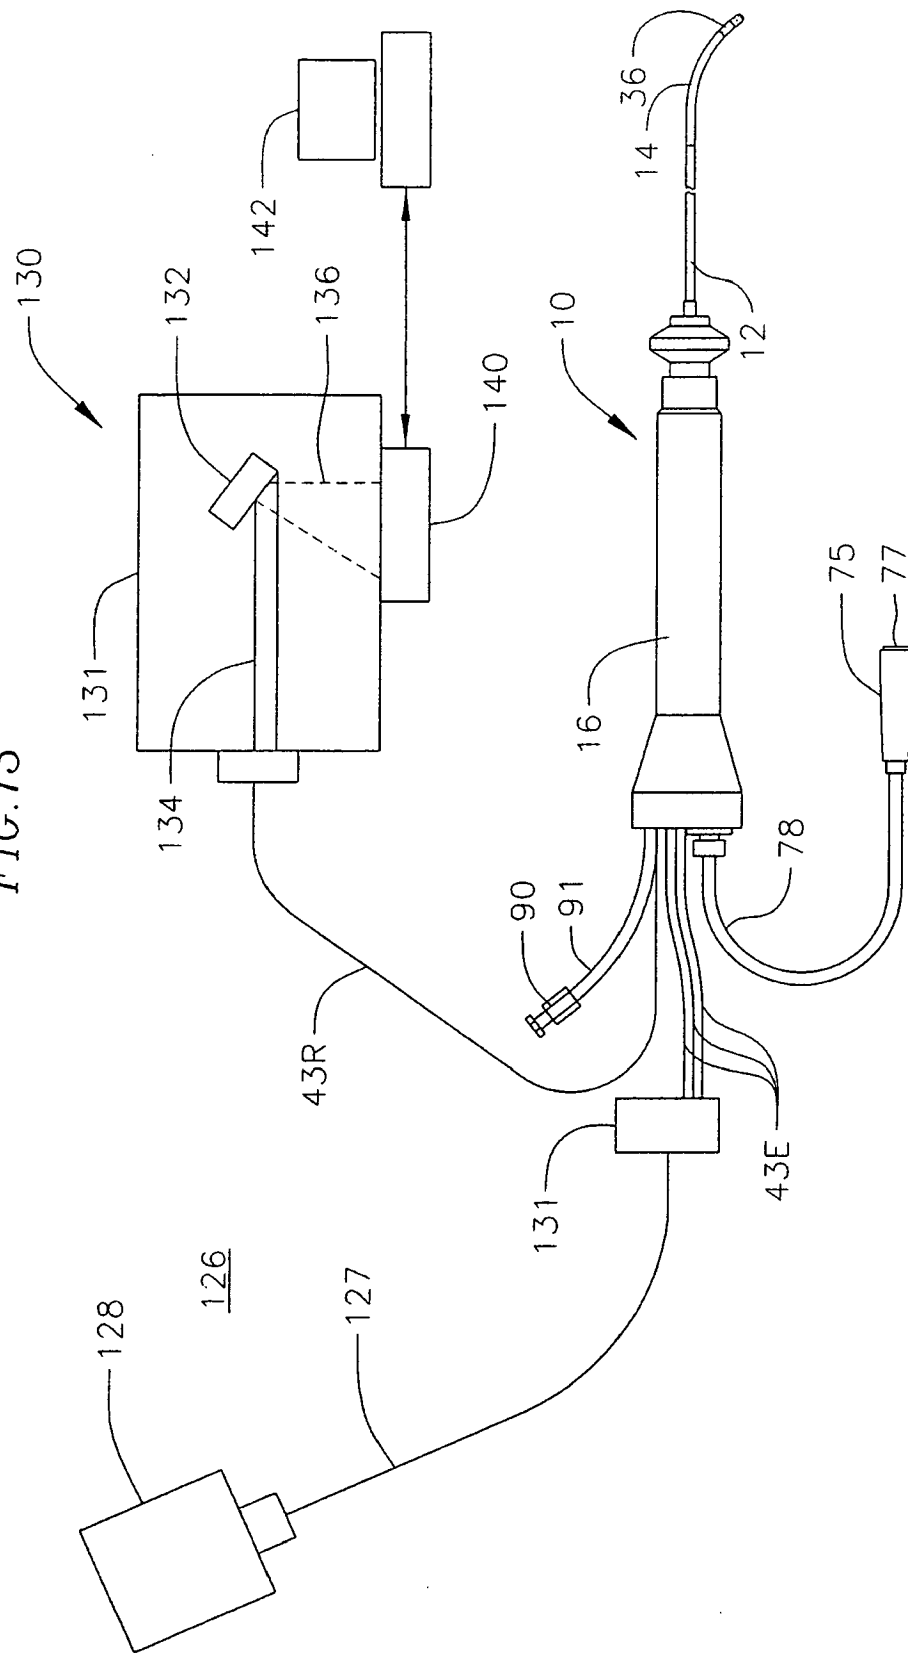

European Patent  
Office

## EUROPEAN SEARCH REPORT

Application Number  
EP 07 25 4493

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
A	US 2006/122587 A1 (SHARAREH SHIVA [US]) 8 June 2006 (2006-06-08) * abstract; figure 1 * * paragraphs [0002], [0012], [0013], [0020], [0021], [0023] * -----	1-31	INV. A61B5/00 A61B18/14
A	US 2003/040657 A1 (YAMAYA KOJI [JP] ET AL) 27 February 2003 (2003-02-27) * abstract; figures 1,2 * * paragraphs [0007], [0011], [0013], [0121], [0133] * -----	1-31	
A	EP 0 195 375 A (MASSACHUSETTS INST TECHNOLOGY [US]) 24 September 1986 (1986-09-24) * abstract; figures 1,1A * * pages 11,19-22 * * pages 29,37-38 * -----	1-31	
A	US 2006/229515 A1 (SHARAREH SHIVA S [US] ET AL) 12 October 2006 (2006-10-12) * abstract; figure 2(b) * * paragraph [0059] * -----	1-31	TECHNICAL FIELDS SEARCHED (IPC) A61B
A	WO 2005/051215 A (ELEKTA AB PUBL [SE]; ERIKSSON OLA [SE]; WAARDELL KARIN [SE]; ANDERSSON) 9 June 2005 (2005-06-09) * abstract; figures 5,16 * * pages 4-5 * * pages 15-18 * -----	1-31	
A	US 5 964 757 A (PONZI DEAN M [US]) 12 October 1999 (1999-10-12) * abstract; figure 2B * * columns 7-9 * -----	1-31	
A	US 2006/030844 A1 (KNIGHT BRADLEY P [US] ET AL) 9 February 2006 (2006-02-09) * the whole document * -----	1-31	
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 31 January 2008	Examiner MOLINA SILVESTRE, A
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

 4  
EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 07 25 4493

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.  
The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

31-01-2008

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2006122587 A1	08-06-2006	NONE	
US 2003040657 A1	27-02-2003	NONE	
EP 0195375 A	24-09-1986	AT 111711 T	15-10-1994
		AT 167792 T	15-07-1998
		DE 3650071 D1	27-10-1994
		DE 3650071 T2	01-06-1995
		DE 3650688 D1	06-08-1998
		DE 3650688 T2	25-03-1999
		NO 861136 A	16-01-1987
		US 5290275 A	01-03-1994
US 2006229515 A1	12-10-2006	CA 2588390 A1	26-05-2006
		CA 2588402 A1	26-05-2006
		EP 1827281 A1	05-09-2007
		WO 2006055733 A1	26-05-2006
		WO 2006055741 A1	26-05-2006
WO 2005051215 A	09-06-2005	NONE	
US 5964757 A	12-10-1999	DE 69837799 T2	31-01-2008
		EP 0900549 A1	10-03-1999
		JP 11188103 A	13-07-1999
US 2006030844 A1	09-02-2006	EP 1781200 A2	09-05-2007
		WO 2006017517 A2	16-02-2006

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 924616 A [0050] [0079]
- WO 11058434 A [0070]
- US 6468260 B [0078]
- US 6602242 B [0078]
- US 5558091 A [0079]
- US 5443489 A [0079]
- US 5480422 A [0079]
- US 5546951 A [0079]
- US 5568809 A [0079]
- US 5391199 A [0079]
- WO 9502995 A [0079]
- US 281179 A [0081]
- US 11281853 B [0081]

专利名称(译)	具有全向光学尖端的改进的导管具有隔离的光学路径		
公开(公告)号	<a href="#">EP1922991A1</a>	公开(公告)日	2008-05-21
申请号	EP2007254493	申请日	2007-11-16
[标]申请(专利权)人(译)	韦伯斯特生物官能公司		
申请(专利权)人(译)	生物传感韦伯斯特, INC.		
当前申请(专利权)人(译)	生物传感韦伯斯特, INC.		
[标]发明人	LEE JAMES K		
发明人	LEE, JAMES K.		
IPC分类号	A61B5/00 A61B18/14		
CPC分类号	A61B18/1492 A61B5/0075 A61B5/0084 A61B5/01 A61B5/065 A61B2017/00057 A61B2017/00084 A61B2018/00172 A61B2018/00577 A61B2018/00642 A61B2018/00773 A61B2018/00791 A61B2018/00982 A61B2034/2051 A61B2090/397 A61B2218/002 A61B2562/12 A61B2562/223 A61M25/0147 Y10T29/49002		
优先权	11/601065 2006-11-17 US		
其他公开文献	EP1922991B1		
外部链接	<a href="#">Espacenet</a>		

# 摘要(译)

导管能够进行实时光测量,例如但不限于漫反射,荧光等,来自生物材料,例如组织(包括血液),同时进行RF消融。导管尖端设计隔离尖端电极内的照明和收集路径,使得用于照射感兴趣组织(例如,心脏组织或血液)的光在尖端电极内与从组织返回到导管尖端的光隔离,并且副反之亦然。这种设计有利地避免了光学检测器的饱和,并确保照明光在感兴趣的介质内的扩散。导管具有导管主体和尖端电极,尖端电极具有壳壁和空腔。壳壁至少具有照明开口和收集开口。导管还包括与照明开口连通的第一光纤线缆和与中空腔体连通的第二光纤线缆,其中从第一光纤线缆发射的光离开尖端电极以通过照明开口到达组织。限定第一路径并通过收集开口从组织返回到尖端电极进入空腔,从而限定第二路径,第一和第二路径在尖端电极内彼此光学隔离。本发明还包括一种制造消融电极尖端的方法,该消融电极尖端限定了在尖端电极中的离散电极,用于从尖端电极射出的光和返回到尖端电极的光。

