



(51) International Patent Classification:

A61B 5/00 (2006.01) G06F 17/00 (2006.01)
G06F 19/00 (2011.01)

(21) International Application Number:

PCT/US2017/018530

(22) International Filing Date:

17 February 2017 (17.02.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(72) Inventor; and

(71) Applicant: HAGAR, Amit [US/US]; 2512 E Rock Creek
Drive, Bloomington, Indiana 47401-6824 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,
HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR,
KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG,
MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM,
PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC,
SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR,
TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,

UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to the identity of the inventor (Rule 4.17(i))
- as to applicant's entitlement to apply for and be granted a
patent (Rule 4.17(ii))
- of inventorship (Rule 4.17(iv))

Published:

- with international search report (Art. 21(3))
- with amended claims and statement (Art. 19(1))

(54) Title: SYSTEMS AND METHODS FOR OPTIMIZING DIAGNOSTICS AND THERAPEUTICS WITH METABOLIC
PROFILING

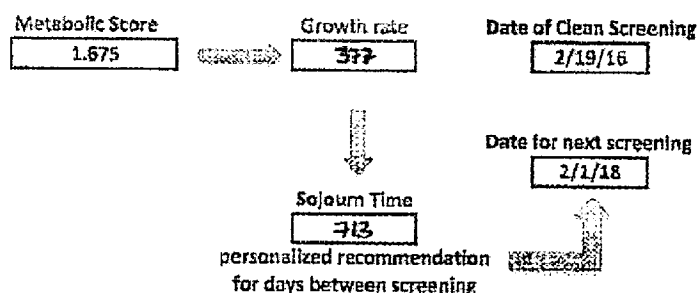


FIG. 6

(57) Abstract: The present disclosure is directed towards methods for calculating disease progression rates and sojourn times of solid tumors from metabolic markers and using this calculation to optimize patient-specific diagnosis, scheduling of screening procedures, and dosage or frequency of treatment.



SYSTEMS AND METHODS FOR OPTIMIZING DIAGNOSTICS AND THERAPEUTICS WITH METABOLIC PROFILING

FIELD OF THE DISCLOSURE

[0001] This disclosure relates to personalized medicine. More specifically, this disclosure relates to a method for optimizing diagnostics and therapeutics of solid tumors with patient specific disease progression rates and sojourn times using metabolic profiling in an exercising setup.

BACKGROUND

[0002] Current decision-making processes on scheduling of diagnostic and screening procedures, or dosage and frequency regimes for therapeutic procedures for Breast, Colon, Prostate, lung, and other solid tumors, are based on epidemiological data for patient categories discriminated by age, genetic risk, family history, and few personal clinical features which may limit the sensitivity of the screening apparatus, or the efficacy of the respective treatment.

[0003] One unknown in these decision-making processes is the patient-specific sojourn time of the disease in the phase to which the diagnostic or therapeutic procedure is intended to apply. The sojourn time is a function of the progression rate of the disease, and many of these procedures are optimal and most effective when synchronized with this rate. Lack of appropriate methods to predict progression rates for individual patients is the reason why sojourn times remain unknown. As a result, patients are often treated with “one size fits all” strategy, in which the sojourn times are calculated via statistical averages from the population. The best example for this strategy is the recent recommendation from the US Preventive Service Task Force that all women between 50 and 74 should go through bi-annual mammogram screening. This recommendation may be optimal to some women, but will fail to early-detect those with fast progression rate, and will lead to unnecessary stress and excess radiation in those with slow progression rate.

[0004] Since the progression rates of solid tumors vary considerably between diagnosed patients, additional discriminatory measurements would have profound prognostic, diagnostic and therapeutic value, particularly for personalized medicine, and will ultimately lead to more informative diagnoses and more effective treatments and prognostics.

[0005] Contrary to global measures like BMI, which is mostly non-indicative for personalized medicine, the intracellular metabolic balance between oxidative phosphorylation, or OXPHOS (the production of ATP in the mitochondria by burning Pyruvate with Oxygen) and

Glycolysis (the production of ATP in the cytosol by the breakdown of Pyruvate to Lactate without Oxygen) strongly affects disease progression rates, directly through biosynthesis and indirectly through enhancement of immune response, and thus provides a valuable personal diagnostic and therapeutic discriminant for the above decision-making processes. A possible context where this balance can become evident and measurable is aerobic exercise, where energy from aerobic and non-aerobic metabolism is concurrently produced in the skeletal muscles, yet while athletes use some metabolic markers during aerobic exercise to customize their training zones, so far there is no attempt to measure the intracellular metabolic balance between OXPHOS and Glycolysis in vivo in humans. Current research in animal models does involve measurement of this metabolic balance, but is directed solely at drug discovery, and not at predicting patient-specific progression rates and sojourn times in animals or in humans.

[0006] Thus, there remains a considerable need for methods that can conveniently predict patient-specific disease progression rates and sojourn times with metabolic markers, so that they can be incorporated into the current decision-making processes on prognostics, diagnostics and therapeutics of solid tumors.

SUMMARY

[0007] Embodiments herein concerns methods for optimizing diagnostics, and therapeutic procedures in a human patient, comprising the steps of measuring the level of at least one metabolic marker in a patient, and calculating disease progression rates and sojourn times, predicting at least one incident selected from the group consisting of: diagnosis, timing of screening procedures, a type of treatment, a dosage of treatment, and a frequency of treatment.

[0008] In some embodiments, methods for optimizing diagnostics, and therapeutic procedures may include further the steps of providing the patient with an exercising equipment, allowing the patient to exercise on the exercising equipment for a period of time. Some embodiments may further include the step of adjusting an exercise level of the patient to the patient's age and heart rate and/or the step of entering the measurement of the at least one metabolic marker to an algorithm.

[0009] In accordance with these embodiments, certain metabolic markers may include, but not limited to, glucose, lactate, and pyruvate. In some embodiments, a patient may be fasted for at least 8 hour.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The above mentioned and other features and objects of this disclosure, and the manner of attaining them, will become more apparent and the disclosure itself will be better understood by reference to the following description of exemplary embodiments of the disclosure taken in conjunction with the accompanying drawings, wherein:

[0011] FIG. 1 represents a possible embodiment of two components of the measurement setup;

[0012] FIG. 2 describes the Lactate clearance curve drawn from curve fitting the 10 measurement points with a 3rd degree polynomial (Cubic Spline) using standard curve fitting software;

[0013] FIG. 3. depicts the integral calculated by a standard curve fitting software;

[0014] FIG. 4 depicts a possible embodiment of the computer interface allowing the user to input the data from the measurement protocol (b) into the 1st algorithm in (c) that calculates the patient's metabolic score [MET];

[0015] FIG. 5 depicts the 2nd algorithm in (c) for calculating the predicted growth rate (the doubling time, measured in days, [DT]) from the patient's metabolic score [MET]; and

[0016] FIG. 6 depicts a possible embodiment of the computer interface for the 3rd algorithm in (c) that computes the sojourn time [DAYS] and the receptive optimized frequency for a diagnostic procedure for a given [DT].

[0017] Corresponding reference characters indicate corresponding parts throughout the several views. Although the drawings represent embodiments of the present disclosure, the drawings are not necessarily to scale and certain features may be exaggerated in order to better illustrate and explain the present disclosure. The exemplification set out herein illustrates exemplary embodiments of the disclosure, in various forms, and such exemplifications are not to be construed as limiting the scope of the disclosure in any manner.

DETAILED DESCRIPTION

[0018] The embodiment disclosed below is not intended to be exhaustive or limit the disclosure to the precise form disclosed in the following detailed description. Rather, the embodiments are chosen and described so that others skilled in the art may utilize its teachings.

[0019] One of ordinary skill in the art will realize that the embodiments provided can be implemented in hardware, software, firmware, and/or a combination thereof. Programming code according to the embodiments can be implemented in any viable programming language such as

C, C++, HTML, XHTML, JAVA or any other viable high-level programming language, or a combination of a high-level programming language and a lower level programming language.

[0020] As used herein, the modifier “about” used in connection with a quantity is inclusive of the stated value and has the meaning dictated by the context (for example, it includes at least the degree of error associated with the measurement of the particular quantity). When used in the context of a range, the modifier “about” should also be considered as disclosing the range defined by the absolute values of the two endpoints. For example, the range “from about 2 to about 4” also discloses the range “from 2 to 4.”

[0021] Where a range of values is provided, it is understood that each intervening value, to the tenth of the unit of the lower limit unless the context clearly dictates otherwise, between the upper and lower limit of that range and any other stated or intervening value in that stated range is encompassed within the present disclosure. The upper and lower limits of these smaller ranges may independently be included in the smaller ranges is also encompassed within the present disclosure, subject to any specifically excluded limit in the stated range. Where the stated range includes one or both of the limits, ranges excluding either or both of those included limits are also included in the present disclosure.

[0022] Unless defined otherwise, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which the present disclosure belongs. Although any methods and materials similar or equivalent to those described herein can also be used in the practice or testing of the present disclosure, a limited number of the exemplary methods and materials are described herein.

[0023] It must be noted that as used herein and in the appended claims, the singular forms “a”, “an”, and “the” include plural referents unless the context clearly dictates otherwise.

[0024] A therapeutically effective amount is an amount of a biologically active compound that has a single or cumulative beneficial effect on the health or well being of a patient.

[0025] The concept of measuring intracellular metabolic markers in humans during exercise and, based on a functional relation between these markers and sojourn times of solid tumors, using these markers to calculate disease progression rates and sojourn times to optimize diagnostics and therapeutic procedures, customizing these procedures to the individual patient.

[0026] Embodiments include a method for measuring metabolic markers in humans and calculating progression rates and sojourn times therefrom, comprising: (a) a measurement set up of (i) a reclined bike or a treadmill; (ii) Lactate and Glucose Analyzers; (iii) a human subject fasting at least 8 hrs; (b) a measurement protocol comprising the steps of: (i) 15 minutes of

incremental aerobic exercise, adjusted to the subject's age and Heart Rate at rest and calculated via Karvonen formula $[(220 - \text{age} - \text{HR}_{\text{rest}}) * P\% + \text{HR}_{\text{rest}}]$, from $P=50\%$ through $P=55\%$, $P=60\%$, $P=65\%$ and up to $P=70\%$ of personal Maximal Heart Rate, spending 3 minutes in each Heart Rate level, followed by 15 minutes of rest; (ii) measurements of Lactate serum concentration at Minute 0, 3, 6, 9, 12, 15, 18, 21, 24, and 30; and (iii) measurements of average power output in Watt at Minute 3, 6, 9, 12, and 15; (c) three algorithms.

[0027] Some embodiments may include a computer interface that allows entering the results from the measurement protocol (b) as input to the algorithms from (c).

[0028] Some embodiments may include an algorithm from step (c) that takes as an input the patient's age and the measurements in protocol (b)(ii-iii) and gives as an output the patient's metabolic score.

[0029] Some embodiments may include an algorithm that takes as input the metabolic score above and gives as an output the personal progression rate of the disease (doubling time in days).

[0030] Some embodiments may include an Algorithm that takes as an input the personal progression rate above and yields as an output the sojourn time of the disease between two designated time points of a particular clinical procedure, so that a schedule for a diagnostic procedure, or a dosage and a frequency for a therapeutic procedure, can be calculated based on this sojourn time

[0031] In a preferred embodiment of the present disclosure, the measurement setup described above involves a human subject who can independently perform the measurement protocol described above, either at home or at the physician office, and subsequently receive recommendation for personal scheduling, dosage, or frequency of diagnostic or therapeutic procedures, based on the personal sojourn time calculated from the subject's metabolic score.

[0032] The present disclosure is designed so that the three algorithms that can be implemented with data from the measurement protocol (b) either by using the computer interface or by incorporating these algorithms as hardware into one or more components of the measurement setup in (a)(i-ii), so that the data from the setup will be automatically fed into the concatenated chain of algorithms at the end of the protocol.

[0033] Various objects, features, aspects, and advantages of the present disclosure will become more apparent from the following detailed description of preferred embodiments of the present disclosure, along with the accompanying drawings in which like numerals represent like components.

[0034] FIG. 1 represents a possible embodiment of two components of the measurement setup ((a) and (b)).

[0035] FIG. 2 describes the Lactate clearance curve drawn from curve fitting the 10 measurement points with a 3rd degree polynomial (Cubic Spline) using standard commercial curve fitting software from. The data points are those obtained from using the apparatus in FIG. 1 on the human subject who follows the measurement protocol (b).

[0036] FIG. 3 depicts the integral calculated by the Algorithm on that curve (the area below it) between point 0 (the initial time point of the measurement protocol (b)) and point 30 (the final time point of the measurement protocol in (b)).

[0037] FIG. 4 depicts a possible embodiment of the computer interface allowing the user to input the data from the measurement protocol (b) into the first algorithm. This algorithm works as follows:

[0038] Algorithm I:

[0039] Step 1: Calculate the integral on the Lactate clearance curve (figure 6) in each 3 minutes interval between 0 and 15, and divide it by $W/100$, where W is the average Watt output, read from the apparatus in Figure 1 during each 3-minute segment, in 10 seconds intervals.

[0040] Step 2: Sum the 5 normalized area segments in Step 1.

[0041] Step 3: Calculate the integral on the Lactate clearance curve in the interval between minute 15 and 30.

[0042] Step 4: Sum results from Step 2 and Step 3. This is the total normalized area [LAC]

[0043] Step 5: Calculate the age correction factor [Age] by subtracting 50 from the human subject current age. [Age] can be negative.

[0044] Step 6: Multiply result from Step 6 with

$$([Age]/100+1)$$

[0045] Step 7: Given the range of Lactate serum concentration in humans and the nature of the measurement protocol (b), the final result is a positive number between 0 and 3, designating the subject's metabolic score [MET].

[0046] FIG. 5 depicts the algorithm for calculating the predicted growth rate (the doubling time [DT], measured in days) from the subject's metabolic score [MET]. The algorithm works as follows:

[0047] Algorithm II:

[0048] Step 1: Calculate the doubling time [DT] from the metabolic score [MET] given by Algorithm I (Step 7) using the formula:

$$[DT] = 10^{(a-b*\log_{10}[MET])}$$

where the range of these parameters for a 95% confidence level (in this particular embodiment for Invasive Ductal Carcinoma) is.

[0049]

$$a = 3.53 \pm 0.11 \quad \text{and} \quad b = 4.71 \pm 0.41$$

[0050] FIG. 6 depicts a possible embodiment of the computer interface for the algorithm that computes the sojourn time for a given [DT]. In the example presented here, a subject whose screening result is normal at a given date can use the predicted progression rate [DT] to calculate the sojourn time of the disease under the assumption that the disease exists but the screening apparatus failed to detect it because it is below or at the detection threshold. With this sojourn time the next schedule for screening can be decided using the following steps:

[0051] Algorithm III:

[0052] Step 1: Calculate sojourn time [DAYS] with

$$[DAYS] = [DT] * (([RFN]*\text{LOG}_2([FN]/[T]) + [RTN]*\text{LOG}_2([TN]))$$

[0053] Here [T] represents the threshold of detection of the screening apparatus in mm³, ([T]=8 for digital mammography of breast tumor) and the adjustable nominators in the LOG₂ ([FN] and [TN]) represent a target volume of the tumor in mm³ deemed appropriate for diagnostic purposes (in the embodiment in figure 6, [FN]=9 for the false negative case and [TN]=1 for the true negative case).

[0054] Thus the first part of the sum in each sojourn time (“([RFN]*LOG₂([FN]/[T])”) is calculated under the assumption that the current normal mammogram is false negative and the tumor is at most at detection threshold, and the second part of the sum in each sojourn time (“([RTN]*LOG₂([TN])”) is calculated under the assumption that the current normal mammogram is true negative but the tumor is below detection threshold, at 1mm³.

[0055] The normalizing adjustable factors 0<[RFN]<1 and [RTN]=1-[RFN] represent the statistical rate of false and true negatives of the screening apparatus, respectively (in the case of digital mammography for this particular embodiment, and according to the National Cancer Institute, [RFN] ranges between 10% and 20%).

[0056] The parameters [T] [FN] [TN] in Steps (1) of Algorithm III can be adjusted according to the specific disease, the sensitivity of the screening apparatus for that disease, and the risk-aversion of the patient.

[0057] Step 2: use [DAYS] to decide the optimal next screening date, now based on the personal sojourn time and the sensitivity of the screening apparatus, according to the following table (based on [RFN], [RTN], [FN], [TN] in the case of invasive ductal carcinoma):

If [DAYS]>730, next screening date is in 2 years

If [DAYS]<200 days, next screening date is in 6 months

If $200 < [\text{DAYS}] < 730$, the next screening date is [DAYS] days from current date

[0058] Since [DT] is calculated using the personalized metabolic score [MET], the scheduling interval may differ from the average “one size fits all” recommendation. Embodiments ensure it will be customized to the individual patient. This possible embodiment thus shows how this disclosure allows the physician and the subject to replace the prevailing decision making process on scheduling of screening which is based on an “average” sojourn time in the population with a personalized decision making process which is customized to the individual subject. The benefit of this customized process is that subjects whose sojourn time is shorter than the average could now decide to schedule their screening frequency accordingly and would have a higher probability to early detect the disease upon onset, while subjects whose sojourn time is longer than the average could now decide to avoid unnecessary stress and excess radiation by scheduling their screening less frequently.

[0059] The reduction to practice of the disclosure to other types of solid tumors may require changes in the parameters (a,b) of Algorithm II, due to known differences in cell growth in different tissues. The parameters [T] [FN] [TN] in Algorithm III will vary with the detection thresholds and the false negative rates of the respective screening modality in each disease, all this without changing any of the Independent or Dependent Claims.

[0060] Thus, specific compositions and methods of optimizing diagnostics and therapeutic schedules with metabolic profiling have been disclosed. It should be apparent, however, to those skilled in the art that many more modifications besides those already described are possible without departing from the inventive concepts herein. The inventive subject matter, therefore, is not to be restricted except in the spirit of the disclosure. Moreover, in interpreting the disclosure, all terms should be interpreted in the broadest possible manner consistent with the context. In particular, the terms "comprises" and "comprising" should be interpreted as referring to elements, components, or steps in a non-exclusive manner, indicating that the referenced

elements, components, or steps may be present, or utilized, or combined with other elements, components, or steps that are not expressly referenced.

[0061] While this disclosure has been described as having an exemplary design, the present disclosure may be further modified within the spirit and scope of this disclosure. This application is therefore intended to cover any variations, uses, or adaptations of the disclosure using its general principles. Further, this application is intended to cover such departures from the present disclosure as come within known or customary practice in the art to which this disclosure pertains.

[0062] Furthermore, the connecting lines shown in the various figures contained herein are intended to represent exemplary functional relationships and/or physical couplings between the various elements. It should be noted that many alternative or additional functional relationships or physical connections may be present in a practical system. However, the benefits, advantages, solutions to problems, and any elements that may cause any benefit, advantage, or solution to occur or become more pronounced are not to be construed as critical, required, or essential features or elements. The scope is accordingly to be limited by nothing other than the appended claims, in which reference to an element in the singular is not intended to mean “one and only one” unless explicitly so stated, but rather “one or more.” Moreover, where a phrase similar to “at least one of A, B, or C” is used in the claims, it is intended that the phrase be interpreted to mean that A alone may be present in an embodiment, B alone may be present in an embodiment, C alone may be present in an embodiment, or that any combination of the elements A, B or C may be present in a single embodiment; for example, A and B, A and C, B and C, or A and B and C.

[0063] In the detailed description herein, references to “one embodiment,” “an embodiment,” “an example embodiment,” etc., indicate that the embodiment described may include a particular feature, structure, or characteristic, but every embodiment may not necessarily include the particular feature, structure, or characteristic. Moreover, such phrases are not necessarily referring to the same embodiment. Further, when a particular feature, structure, or characteristic is described in connection with an embodiment, it is submitted that it is within the knowledge of one skilled in the art with the benefit of the present disclosure to affect such feature, structure, or characteristic in connection with other embodiments whether or not explicitly described. After reading the description, it will be apparent to one skilled in the relevant art(s) how to implement the disclosure in alternative embodiments.

[0064] Furthermore, no element, component, or method step in the present disclosure is intended to be dedicated to the public regardless of whether the element, component, or method step is explicitly recited in the claims. No claim element herein is to be construed under the provisions of 35 U.S.C. § 112(f), unless the element is expressly recited using the phrase “means for.” As used herein, the terms “comprises,” “comprising,” or any other variation thereof, are intended to cover a non-exclusive inclusion, such that a process, method, article, or apparatus that comprises a list of elements does not include only those elements but may include other elements not expressly listed or inherent to such process, method, article, or apparatus.

WHAT IS CLAIMED IS:

1. A method for optimizing diagnostics and therapeutic procedures for solid tumors in a human patient by measuring metabolic markers during exercise, the method comprising the steps of:
 - measuring the level of at least one metabolic marker in a patient during exercise; and
 - calculating disease progression rates and sojourn times based on a functional relation between these markers and disease progression rates and sojourn time;
 - predicting at least one incident selected from the group consisting of: diagnosis, timing of screening procedures, a type of treatment, a dosage of treatment, a timing of treatment, and a frequency of treatment.
2. The method of claim 1, further comprising the steps of:
 - providing the patient with an exercising equipment;
 - allowing the patient to exercise on the exercising equipment for a period of time.
3. The method of claim 2, further comprising the step of:
 - adjusting an exercise level of the patient to the patient's age and heart rate.
4. The method of any one of the claims 1-3, further comprising the step of:
 - entering the measurement of the at least one metabolic marker to an algorithm.
5. The method of any one of the claims 1-4, wherein the at least one metabolic marker comprises glucose, lactate, and pyruvate.
6. The method of any one of claims 1-5, wherein the patient has been fasted for at least 8 hours.
7. The method of any one of claims 1-6, wherein an algorithm is used to calculate the patient's metabolic score from the measured metabolic marker.
8. The method of any one of claims 1-7, wherein an algorithm is used to predict the personal progression rate and sojourn time from the patient's metabolic score.
9. The method of any one of claims 1-8, wherein an algorithm is used to calculate the optimal frequency of a diagnostic procedure or the optimal dosage and frequency of a therapeutic procedure from the progression rate and sojourn time.

AMENDED CLAIMS
received by the International Bureau on 18 May 2017 (18.05.2017)

WHAT IS CLAIMED IS:

1. A method for optimizing diagnostics and therapeutic procedures for solid tumors in a human patient by measuring metabolic markers during exercise, the method comprising the steps of:
 - measuring the level of at least one metabolic marker in a patient during exercise; and
 - calculating disease progression rates and sojourn times based on a functional relation between at least one metabolic marker and disease progression rates and sojourn time;
 - predicting at least one incident selected from the group consisting of: diagnosis, timing of screening procedures, a type of treatment, a dosage of treatment, a timing of treatment, and a frequency of treatment.
2. The method of claim 1, further comprising the steps of:
 - providing the patient with an exercising equipment;
 - allowing the patient to exercise on the exercising equipment for a period of time.
3. The method of claim 2, further comprising the step of:
 - adjusting an exercise level of the patient to the patient's age and heart rate.
4. The method of any one of the claims 1-3, further comprising the step of:
 - entering the measurement of the at least one metabolic marker to an algorithm.
5. The method of any one of the claims 1-4, further comprising of an algorithm to calculate the patient's metabolic score from the measured metabolic marker.
6. The method of any one of the claims 1-5, further comprising of an algorithm to predict the personal progression rate and sojourn time from the patient's metabolic score.
7. The method of any one of the claims 1-6, further comprising of an algorithm to calculate the optimal frequency of a diagnostic procedure or the optimal dosage and frequency of a therapeutic procedure from the progression rate and sojourn time.

STATEMENT UNDER ARTICLE 19 (1)

Bloomington, IN, May 22nd 2017

Attention PCT

Receiving the international search report, transmitted to me on May 18, I have followed the text in that letter which says:

The applicant is entitled, if he so wishes, to amend the claims of the international application

Given that claim 5-9 in the original application from Feb 17 2017 were unsearchable, I have replaced these five claims with the following 3 claims 5*-7*:

Original claims

5. The method of any one of the claims 1-4, wherein the at least one metabolic marker comprises glucose, lactate, and pyruvate.
6. The method of any one of claims 1-5, wherein the patient has been fasted for at least 8 hours.
7. The method of any one of claims 1-6, wherein an algorithm is used to calculate the patient's metabolic score from the measured metabolic marker.
8. The method of any one of claims 1-7, wherein an algorithm is used to predict the personal progression rate and sojourn time from the patient's metabolic score.
9. The method of any one of claims 1-8, wherein an algorithm is used to calculate the optimal frequency of a diagnostic procedure or the optimal dosage and frequency of a therapeutic procedure from the progression rate and sojourn time.

Amended claims


- 5*. The method of any one of the claims 1-4, further comprising of an algorithm to calculate the patient's metabolic score from the measured metabolic marker.
- 6*. The method of any one of the claims 1-5, further comprising of an algorithm to predict the personal progression rate and sojourn time from the patient's metabolic score.
- 7*. The method of any one of the claims 1-6, further comprising of an algorithm to calculate the optimal frequency of a diagnostic procedure or the optimal dosage and frequency of a therapeutic procedure from the progression rate and sojourn time.

The amended claims are now drafted in accordance of rule 6.4(a), are not multiply dependent and are thus searchable.

With this statement I hope to have answered the concerns of the International Search Report

Respectfully,

Amit Hagar



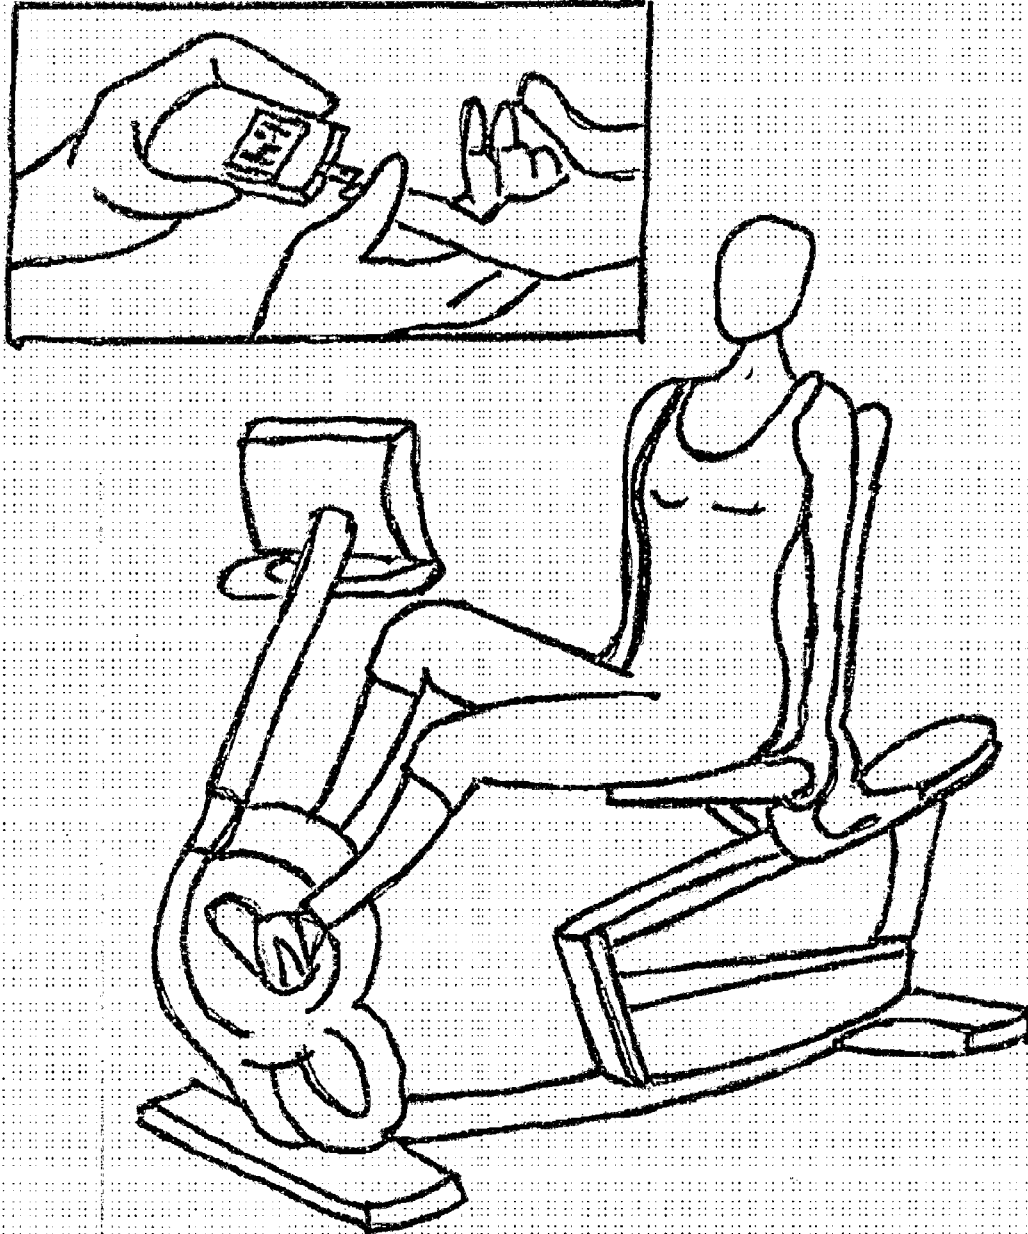


FIG. 1

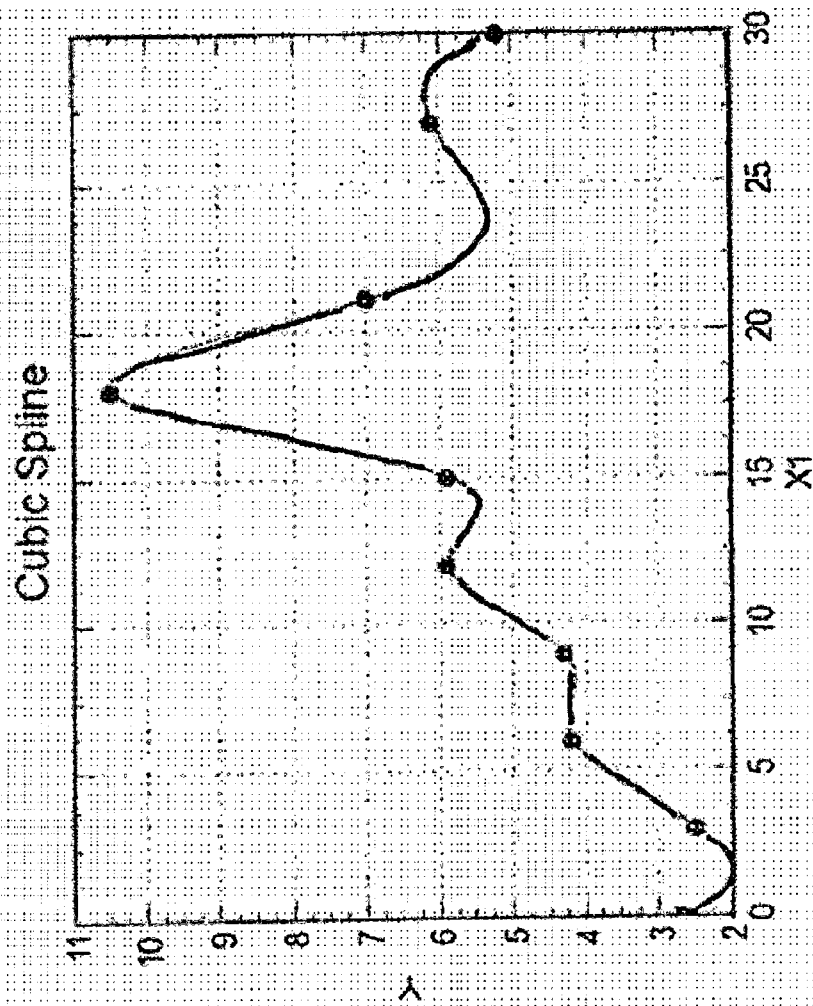


FIG. 2

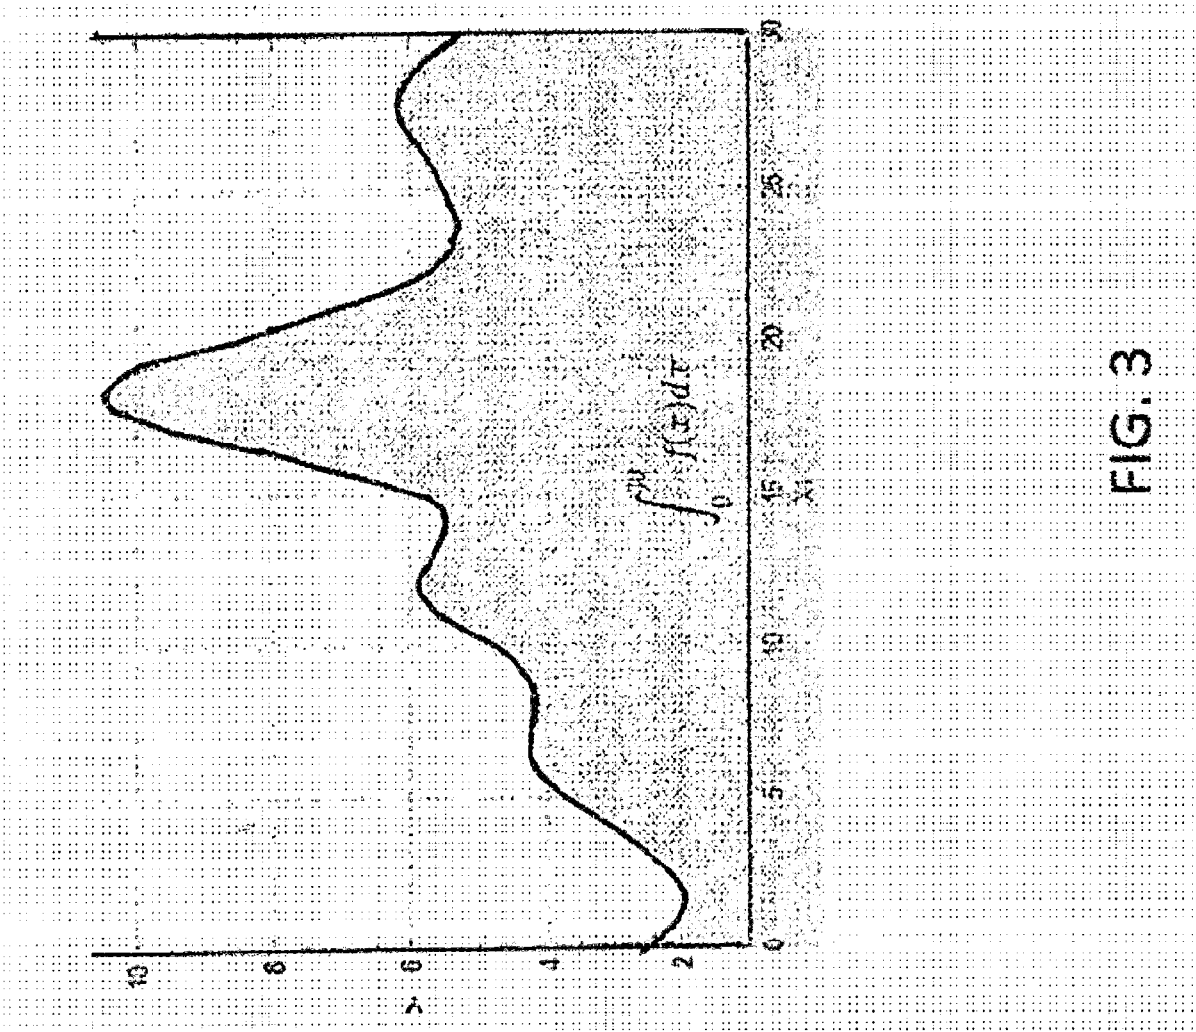


FIG. 3

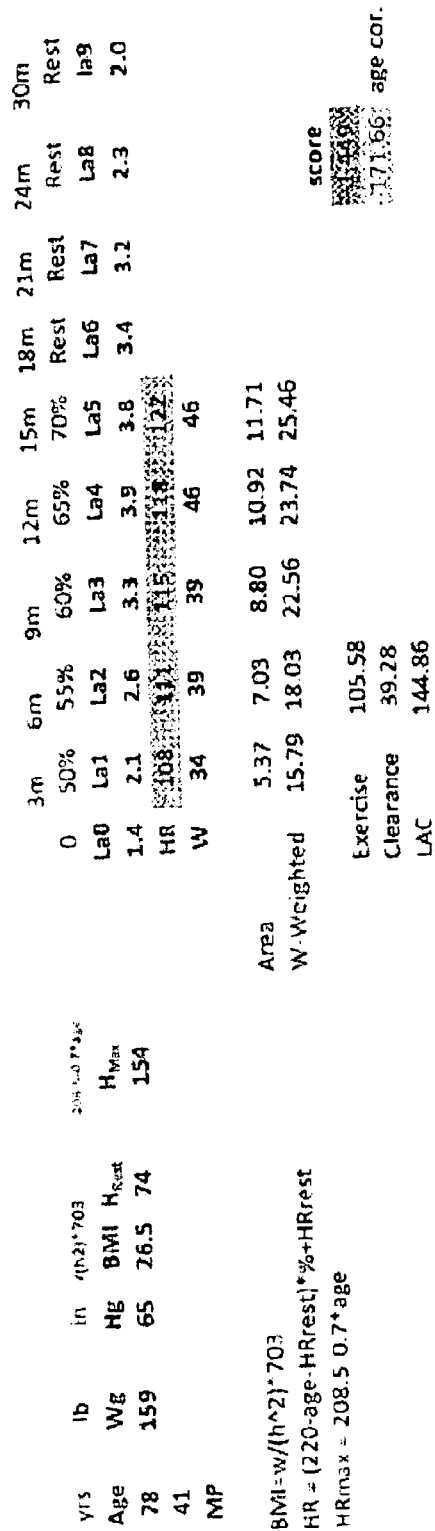


FIG. 4

$$[DT] = 10^{(a-b \cdot \log(MET))}$$

where the range of these parameters for a 95% confidence level (in this particular embodiment for Invasive Ductal Carcinoma) is:

$$a = 3.53 \pm 0.11 \quad \text{and} \quad b = 4.71 \pm 0.41$$

FIG. 5

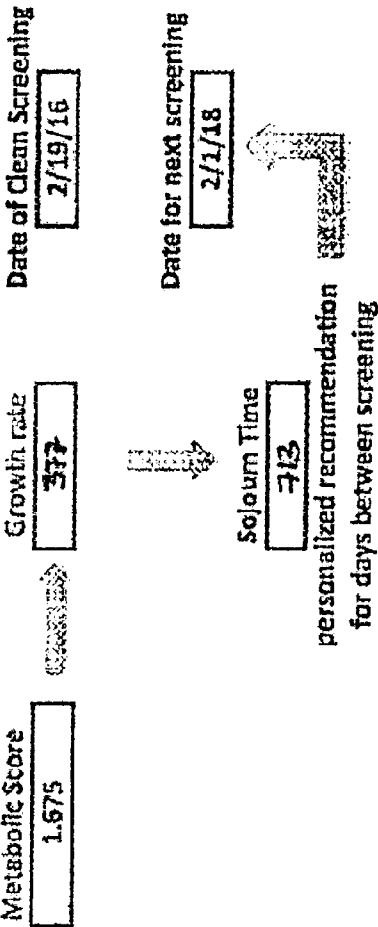


FIG. 6

INTERNATIONAL SEARCH REPORT

International application No.:

PCT/US17/18530

A. CLASSIFICATION OF SUBJECT MATTER

IPC - A61B5/00; G06F19/00; G06F17/00 (2017.01)

CPC - A61B5/4842; A61B5/4866; A61B5/7275; G06F19/345

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 00/78208 A1 (SPECTRX, INC.) 28 December 2000, page 7 lines 10-16, claims 14-17	1-4
A	WO 2015/042476 A1 (GEORGIA TECH RESEARCH CORPORATION) 26 March 2015, paragraphs [0070]-[0072]	1-4
A	US 7,343,197 B2 (SHUSTERMAN, V) 11 March 2008, column 6 lines 20-55, claim 35	1-4

☐ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

19 April 2017 (19.04.2017)

Date of mailing of the international search report

15 MAY 2017

Name and mailing address of the ISA/

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Shane Thomas

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US17/18530

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☒ Claims Nos.: 5-9
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

专利名称(译)	代谢曲线优化诊断和治疗的系统和方法		
公开(公告)号	EP3582678A1	公开(公告)日	2019-12-25
申请号	EP2017897115	申请日	2017-02-17
[标]发明人	HAGAR AMIT		
发明人	HAGAR, AMIT		
IPC分类号	A61B5/00 G06F19/00 G06F17/00		
CPC分类号	A61B5/02 A61B5/14532 A61B5/14542 A61B5/14546 A61B5/222 A61B5/4842 A61B5/4866 A61B5/4884 A63B21/00 G16H20/30 G16H50/20 G16Z99/00 A61B5/7275 A63B24/0075 G06F3/0484 G06F40/205 G06Q30/02 G06Q30/0277 G06Q50/10 G16C20/70 H04L67/26 H04M1/72552 H04M1/72577 H04W4/12 H04W4/23		
外部链接	Espacenet		

摘要(译)

本公开针对用于从代谢标记物计算疾病进展率和实体瘤的停留时间并使用该计算来优化患者特异性诊断，筛查程序的时间表以及治疗剂量或频率的方法。