



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
25.10.2000 Bulletin 2000/43

(51) Int. Cl.⁷: **A61B 5/11**

(21) Application number: 00108575.2

(22) Date of filing: 19.04.2000

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE**
Designated Extension States:
AL LT LV MK RO SI

(72) Inventors:
• **Kondo, Shinji**
Kariya-shi, Aichi-ken 448-0001 (JP)
• **Urano, Hirohide**
Kariya-shi, Aichi-ken 448-0855 (JP)

(30) Priority: 20.04.1999 JP 1122399

(74) Representative:
**Winter, Brandl, Fürniss, Hübner, Röss,
Kaiser, Polte,
Partnerschaft
Patent- und Rechtsanwaltskanzlei
Bavariaring 10
80336 München (DE)**


(71) Applicants:
• **KYOHO MACHINE WORKS Ltd.**
Toyota-shi, Aichi-ken (JP)
• **Kabushiki Gaisya K-AND-S**
Kariya-shi, Aichi-kwn 448-0001 (JP)

(54) **Monitoring depth of anaesthesia of a patient**

(57) A physiological data system (101,102,103,104) for monitoring the anesthetic depth of a patient measures a signal (S) based on the pulse wave of the patient, and measures the sweat rate. If during surgery the patient's condition changes, an operating doctor will

immediately notice a change in the sweat rate displayed by the system, so that corrective measures can be taken.

FIG. 10

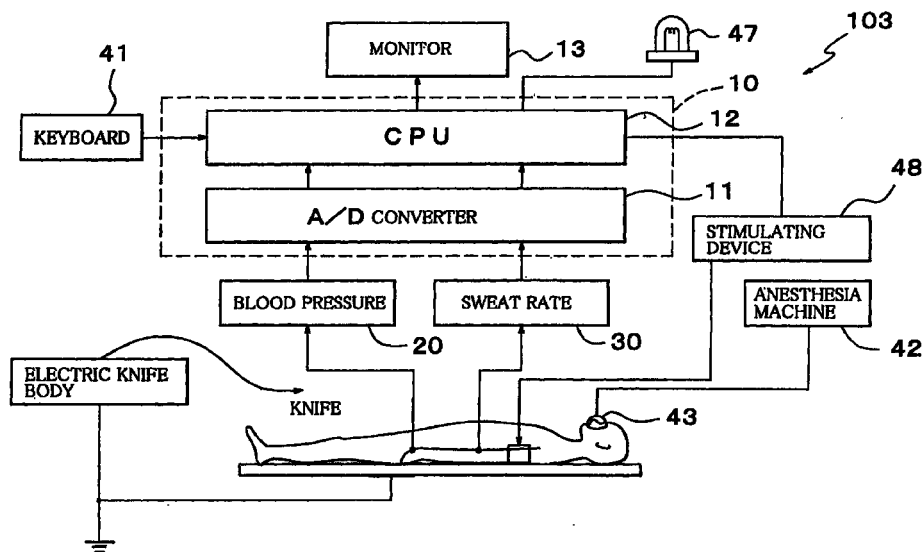

Description

BACKGROUND OF THE INVENTION

1. Field of the Invention

[0001] The present invention relates to a biological data observation system that monitors the anesthetic depth of a patient.

2. Description of the Related Art

[0002] To anesthetize a patient during a surgery, an anesthetic gas is continuously supplied to, for example, a mask placed over the patient's mouth. If the amount of the anesthetic gas supplied is excessively small, the anesthetic depth of the patient becomes insufficient, so that the patient feels pains during the surgery. Conversely, if the anesthetic depth of a patient is excessive, the patient may fall into narcosis. Therefore, in the conventional biological data observation systems, the blood pressure of a patient is measured and displayed on a monitor. While referring to a blood pressure transition curve displayed on the monitor, an anesthesiologist adjusts the anesthetic dosage.

[0003] In general, the biological data related to movements or conditions of a heart, such as blood pressure and the like, responds to administration of an anesthetic with a delay. Therefore, monitoring only the transition of blood pressure of a patient poses a danger of a delay in coping with a change in the patient's condition or a change in the patient's anesthetic depth. Furthermore, the blood pressure hardly change (the change is very little) in response to a stimulus given to a patient even if the patient feels a pain. Therefore, with a system that measures only blood pressure transition, it is difficult to monitor the degree of a pain that a patient feels.

SUMMARY OF THE INVENTION

[0004] Accordingly, it is an object of the invention to provide a biological data observation system capable of observing the anesthetic depth of a patient with an increased accuracy.

[0005] To achieve the aforementioned and other objects, the invention provides a biological data observation system for monitoring an anesthetic depth of a patient, the system including a first measuring device that measures a first biological data based on an amount of perspiration of the patient. The system also includes a data processor that substantially continuously receives the data measured by the first measuring device, and that determines a transition of the data, and an indicator that externally indicates the transition of the data determined by the data processor.

[0006] Perspiration or sweating is generally divided into emotional sweating and thermal sweating. The

emotional sweating is known to be greatly affected by the autonomic nervous system. In the description below, the emotional sweating and the thermal sweating are collectively referred to as "perspiration" or "sweating". In a condition where autonomic nerves are inhibited, such as an anesthetized condition or the like, the amount of perspiration or the sweat rate is less than that in a normal condition (where the autonomic nerves are not inhibited), and increases upon a stimulus. In general, such an emotional sweat rate change is caused by control of autonomic nerve control prior to a subjective symptom. That is, perspiration is governed by autonomic nerves, and the sweat rate of a patient sensitively changes in relation to a stimulus applied to the patient, the anesthetic depth of the patient, or the like. Therefore, the system of the invention makes it possible to detect a sign of a change in the anesthetic depth based on transition of the sweat rate. Furthermore, when a stimulus is applied to an anesthetized patient in order to observe a response of the patient, the system makes it possible to observe a pain felt by the patient in terms of the sweat rate, which is quantitative data.

[0007] Thus, since the system of the invention measures the sweat rate of a patient as well as the patient's pulse wave, the system makes it possible to more accurately observe the anesthetic depth of a patient during a surgery.

[0008] Further, by measuring transition of the patient's pulse wave (blood pressure or the like), the system also makes it possible to observe movements or conditions of the patient's heart in relation to an anesthetic agent.

[0009] Although this summary does not describe all the features of the present invention, it should be understood that any combination of the features stated in the dependent claims is within the scope of the present invention.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The foregoing and further objects, features and advantages of the present invention will become apparent from the following description of preferred embodiments with reference to the accompanying drawings, wherein like numerals are used to represent like elements and wherein:

FIGURE 1 is a block diagram of a biological data observation system according to a first embodiment of the invention;

FIGURE 2 is a block diagram of a blood pressure measuring device;

FIGURE 3 is a partially cutaway perspective view of a capsule of a sweat rate detecting device;

FIGURE 4 is a graph indicating transitions of blood pressure data and sweat rate data;

FIGURE 5 is a flowchart illustrating a procedure of combining a blood pressure signal and a sweat rate

signal;

FIGURE 6 is a graph for illustrating an intermediate step of data processing;

FIGURE 7A is a graph indicating transition of blood pressure data;

FIGURE 7B is a graph indicating transition of sweat rate data;

FIGURE 7C is a graph indicating transition of composite data based on the blood pressure data and the sweat rate data;

FIGURE 8 is a conceptual diagram of data tables stored in a ROM;

FIGURE 9 is a block diagram of a biological data observation system according to a second embodiment of the invention;

FIGURE 10 is a block diagram of a biological data observation system according to a third embodiment of the invention; and

FIGURE 11 is a block diagram of a biological data observation system according to a fourth embodiment of the invention;

DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

[0011] Preferred embodiments of the invention will be described hereinafter with reference to the accompanying drawings.

[0012] A first embodiment of the invention will be described with reference to FIGURES 1 to 8.

[0013] As shown in FIGURE 1, in a biological data observation system 101, output lines of a blood pressure measuring device 20 and a sweat rate measuring device 30 are connected to a data processing device 10.

[0014] A construction of the blood pressure measuring device 20 is illustrated in FIGURE 2. The blood pressure measuring device 20 measures the blood pressure of a patient through calculation of the patient's pulse wave (heart beats, pulses) based on a predetermined converting equation according to a generally-termed blood pressure waveform continuous measurement method. Specifically, an air-filled cuff band 21 is placed around a finger of the patient. While a photoelectrical capacity pulse wave is detected by using a photoelectric light transmitter 22 and a photoelectric light receiver 23 that are disposed at opposite sides of the patient's finger, the cuff pressure is adjusted to balance with the intravascular pressure by controlling the output of a cuff pump 24. In this condition, the blood pressure waveform is continuously measured, and is outputted as a blood pressure signal (for example, an analog signal).

[0015] As shown in FIGURE 3, the sweat rate measuring device 30 is provided with a capsule 31. The capsule 31 is attached to the patient so that an opening 32A of a recess 32 formed in the capsule 31 is closed by a skin surface of the patient. A peripheral surface of the

capsule 31 is provided with a supply opening 33 and a discharge opening 34 that communicate with the recess 32. The recess 32 is supplied with, for example, a low-humidity nitrogen gas at a constant flow rate, from a tank (not shown) via the supply opening 33 and a rubber tube 33A connected thereto. A hygrometer (not shown) is provided in partway of a rubber tube 34A connected to the discharge opening 34, thereby measuring the humidity of discharged air. A thermometer and a heater/cooler (e.g., a Peltier device) are provided in the capsule 31. The heater/cooler is controlled so as to maintain a constant temperature in the recess 32. Based on outputs from the hygrometer and the thermometer, the absolute humidity is detected. The detected absolute humidity is outputted as an analog signal (sweat rate signal).

[0016] FIGURE 4 indicates transitions of blood pressure data (Line A) and sweat rate data (Line B).

[0017] When an anesthetic gas is supplied to a patient (at the point a in FIGURE 4), the sweat rate decreases. The blood pressure also decrease, but responds to administration of an anesthetic with a delay. The amount of the anesthetic gas is increased up to a predetermined amount, and then becomes a steady state where the amount of the supplied gas is constant. After that (point b in FIGURE 4), the sweat rate become stable. If the anesthetic depth is insufficient (light), the sweat rate sensitively changes when a stimulus is applied to the patient (points c and c' in FIGURE 4). Because the sweat rate sensitively changes according to "pain" which is one of stimulus autonomic nerves. Meanwhile the blood pressure does not change at the points c and c' in FIGURE 4. Therefore, it is possible to monitor the anesthetic depth of the patient by measuring the sweat rate. After a surgery (point d in FIGURE 4), the sweat rate increase because the patient comes out from the anesthetic. Since this invention measures the sweat rate of the patient during the surgery, it is possible to determine that the patient has come out from the anesthetic when the sweat rate reaches the sweat rate which has been memorized at the beginning of the surgery.

[0018] The data processing device 10 has an A/D converter 11, and thereby converts the blood pressure signal and the sweat rate signal into digital signals, and inputs them into ports of a CPU 12. Upon power-up, the CPU 12 loads a program from a ROM (not shown) provided in the data processing device 10. In this embodiment, CPU 12 also executes data processing as illustrated in the flowchart of FIGURE 5 to calculate blood pressure data P1, sweat rate data S1, and composite data PS (described in detail below) so that perform more precise evaluation of the anesthetic depth.

[0019] Blood pressure data P1, sweat rate data S1 and composite data obtained during an anesthetized condition and a normal condition are pre-stored in the ROM in the data processing device 10, as standard data, with parameters of, for example, age, sex, body

weight and the like. The standard data is prepared beforehand by, for example, an experienced anesthesiologist actually collecting blood pressure data, sweat rate data and composite data at the time of administration of an anesthetic to patients, and aggregating or summarizing the collected data. The standard data is provided in the form of data tables as indicated in FIGURE 8.

[0020] The data processing device 10 is connected to a monitor 13 (e.g., CRT) for externally displaying contents of measurement and processing.

[0021] A biological data observing method according to this embodiment will be described in detail with reference to FIGURE 5.

[0022] Before administration of an anesthetic to a patient, the system 101 is set on the patient. More specifically, the cuff band 21 of the blood pressure measuring device 20 and the capsule 31 of the sweat rate measuring device 30 are attached to the patient's body, and then the data processing device 10, the blood pressure measuring device 20 and the sweat rate measuring device 30 are powered on. Subsequently, the patient's age, sex and body weight are inputted to the data processing device 10 from a keyboard 41.

[0023] When the biological data observation system 101 is activated, the blood pressure signal from the blood pressure measuring device 20 and the sweat rate signal from the sweat rate measuring device 30 are converted into digital signals by the A/D converter 11, and then are inputted to the data processing device 10. In accordance with the program loaded upon the power-up, the CPU 12 writes the input blood pressure signal and the input sweat rate signal as a variable P1 and a variable S1 into predetermined memory areas (STEP 1 in FIGURE 5). Hereinafter, these data are referred to as "blood pressure data P1" and "sweat rate data S1" for easier description.

[0024] Next, the CPU 12 combines the blood pressure data P1 and the sweat rate data S1 (STEP 2 in FIGURE 5). In this embodiment, composite data PS is calculated as in equations (1) to (4).

$$P2 = C1 \times P1 \quad (1)$$

$$S2 = C2 \times S3 \quad (2)$$

$$S3 = 1 - \exp(C3 \times S1) \quad (3)$$

$$PS = P2 + S2 \quad (4)$$

where C1 and C2 are positive constants, and C3 is a negative constant (C1 > 0, C2 > 0, C3 < 0).

[0025] The relationship between the sweat rate data S1 and the value S3 determined by equation (3) is indicated in FIGURE 6.

[0026] After calculating the composite data PS, the CPU 12 causes the monitor 13 connected to the data processing device 10 to draw time-transition curves of

the blood pressure data P1, the sweat rate data S1 and the composite data PS (STEP 3 in FIGURE 5). Examples of displayed transition curves of the blood pressure data P1, the sweat rate data S1 and the composite data PS are shown in FIGURES 7A, 7B and 7C, respectively. If necessary, it is possible to display on the monitor 13 personal data (age, body weights and the like) inputted to the data processing device 10 from the keyboard 41, and the standard data of blood pressure data P1 and sweat rate data S1 and composite data PS for the normal condition and the anesthetized condition (stored in the ROM of the data processing device 10) based on the personal data, as well as transition curves as shown in FIGURES 7A to 7C.

[0027] After the transition curves displayed on the monitor 13 become stable, the blood pressure data P1, the sweat rate data S1 and the composite data PS are all compared with the standard data. In this embodiment, it is assumed that the data of the patient accords with (conforms to) the standard data. If an actual measurement greatly differs from the standard data due to individual patient difference, the difference between the actual measurement and the standard data is inputted to the data processing device 10 by using the keyboard 41. The difference may be displayed as a correction value on the monitor 13.

[0028] After that, the mask 43 connected to an anesthesia machine 42 is attached to the patient, and then the anesthesia machine 42 is activated. Then, an anesthetic gas is supplied via the mask 43, so that the anesthetic enters the patient's blood via the respiratory system. When the anesthetic in blood reaches the patient's brain, the brain sends a signal to autonomic nerves so that the sweat rate decreases. In response, the humidity in the recess 32 of the capsule 31 decreases. Therefore, the transition curves of the sweat rate data S1 and the composite data PS exhibit rightward decreasing tendencies as indicated in stage X1 in FIGURES 7B and 7C. In this stage, however, the blood pressure transition curve normally remains horizontal (exhibits substantially no change) as shown in FIGURE 7A since the blood pressure delays in responding to the anesthetic administration.

[0029] As the anesthetic depth increases with increases in the uptake of the anesthetic into the patient's body, the sweat rate data S1 and the composite data PS become quite low as indicated in a stage X2 in FIGURES 7B and 7C.

[0030] If the amount of the anesthetic supplied becomes excessive, the sweat rate data S1 becomes lower than the standard data. In that case, the transition curves of the sweat rate data S1 and the composite data PS change as indicated at a time point Y1 in FIGURES 7B and 7C. Therefore, a sign of a change in the patient's condition can be detected.

[0031] In this embodiment, the value S3 is determined from the sweat rate data S1 by the exponential function as in equation (3). The value S3 changes cor-

responding to the sweat rate data S1 as indicated in FIGURE 6. That is, the value S3 sharply rises in a range where the sweat rate data S1 is relatively small. Therefore, small changes occurring in the range of relatively small sweat rate data S1 can be reflected in the value S3. Since the value S3 is loaded on the blood pressure data P1 in equation (4) to generate the composite data PS, small changes in the sweat rate (FIGURE 7B) are also displayed as changes in the composite data PS on the monitor 13 as shown in FIGURE 7C. The degree of rising of the curve of S3 in FIGURE 6 (the gradient of a broken line L in FIGURE 6) can be adjusted by changing the value of constant C3 in equation (3).

[0032] The value S3 changes as indicated in FIGURE 6, and does not exceed 1 regardless of how much the sweat rate increases. Furthermore, since the value S3 is loaded on the blood pressure data P1 to generate the composite data PS, the composite data PS changes between the transition curve of the blood pressure (two-dot chain line A in FIGURE 7C) and a curve (a chain line B in FIGURE 7C) offset from the blood pressure transition curve. Therefore, even if the sweat rate greatly changes, the transition of the blood pressure is reflected as overall changes in the transition curve of the composite data PS.

[0033] The blood pressure data P1, the sweat rate data S1 and the composite data PS of the patient become stable and substantially equal to the standard data prepared for the anesthetized condition, a stimulus (e.g., an electric stimulus) is applied to the patient. For example, if electric stimuli are given at time points Y2, Y3 in FIGURES 7A to 7C, the sweat rate data S1 and the composite data PS change as indicated in FIGURES 7B and 7C. Thus, this embodiment makes it possible to observe pains of the patient quantitatively based on the sweat rate. If the sweat rate data S1 becomes excessively large, it is considered that the patient feels a pain, and then the amount of anesthetic supplied is slightly increased. Therefore, the embodiment makes it possible to relatively precisely and easily observe the condition of a patient, in comparison with observation based on facial features of a patient.

[0034] After the anesthetic depth becomes stable, the surgery is started (for example, a body area concerned is cut by an electric knife 44). In the system 101 of this embodiment, by observing the composite data PS displayed on the monitor 13, an operating doctor or the like can simultaneously observe for a sign of a change in the anesthetic depth based on the transition of the sweat rate and can observe the anesthetic depth based on the transition of the blood pressure, at a glance. Therefore, the burden on operating doctors during a surgery decreases. If the sweat rate becomes out of a predetermined range, a doctor will realize a change in the patient's condition during the surgery, merely by observing changes in the sweat rate displayed on the monitor 13. Therefore, the doctor or the like can promptly take an appropriate measure. After that, the

doctor or the like can understand how the patient's condition changes as a result of the measure, by observing the transition of the blood pressure displayed on the monitor 13.

5 **[0035]** In this embodiment, it is also possible to display only the transition curve of the composite data PS on the monitor 13.

[0036] A second embodiment of the biological data observation system of the invention will be described with reference to FIGURE 9. Only constructions that distinguish the second embodiment from the first embodiment will be described.

10 **[0037]** In a biological data observation system 102 of the second embodiment, an electromagnetic valve 45 for adjusting the flow of an anesthetic gas is provided in partway of an anesthetic gas supplying line 42A extending between an anesthesia machine 42 and a mask 43. The electromagnetic valve 45 is driven by a valve drive circuit 46. The valve drive circuit 46 adjusts the extent of opening of the electromagnetic valve 45 based on an instruction from a CPU 12.

15 **[0038]** In this embodiment, the control of the system 102 is switched to an automatic mode, for example, when the anesthetic depth becomes stable and the surgery is to be started. The supply of an anesthetic is increased (or decreased), for example, if both the blood pressure data P1 and the sweat rate data S1 become abnormally large (or small), i.e., become out of predetermined ranges, that is, if the composite data PS becomes abnormally large (or small), i.e., becomes out of a predetermined range. Thus, the supply of the anesthetic gas can be automatically adjusted to a predetermined amount, so that the anesthetic depth of a patient can be kept in a stable state and the burden on an operating doctor can be reduced.

20 **[0039]** In this embodiment, the amount of supply of the anesthetic is changed based on changes in the composite data in order to perform the control with an increased precision. However, it is also possible to change the amount of supply of the anesthetic when one of the blood pressure data and the sweat rate data exhibits an abnormal change.

25 **[0040]** A third embodiment of the biological data observation system of the invention will be described with reference to FIGURE 10. Constructions that distinguish the third embodiment from the first embodiment will be described below.

30 **[0041]** In a biological data observation system 103 of the third embodiment, a warning light 47 and a simulating device 48 are connected to a data processing device 10. A CPU 12 provided in the data processing device 10 turns on the data processing device 10 and the simulating device 48 when the composite data PS assumes an abnormal value. When the simulating device 48 applies an electric current stimulus to the patient, responses to the stimulus are detected by a blood pressure measuring device 20 and a sweat rate measuring device 30. If the composite data PS does not

increase in response to the electric current stimulus, it can be determined that the anesthetic depth is excessively great. Therefore, more precise evaluation of the anesthetic depth becomes possible. Furthermore, the turning-on of the warning light 47 calls attention of the doctors and nurses. Therefore, a sudden change in the patient's condition can be promptly coped with.

[0042] In this embodiment, the warning light 47 and the simulating device 48 may be activated when one of the blood pressure data P1 and the sweat rate data S1 assumes an abnormal value, instead of the composite data PS assuming an abnormal value.

[0043] A fourth embodiment of the biological data observation system of the invention will be described with reference to FIGURE 11. Constructions that distinguish the fourth embodiment from the first embodiment will be described below.

[0044] In a biological data observation system 104 of the fourth embodiment, a brain wave sensor 51, a vascular flow sensor 52 and a body temperature sensor 53 are connected to a data processing device 10. When at least one (e.g., three) of the data from these sensors, the blood pressure data P1, the sweat rate data S1 and the composite data PS assumes an abnormal value, it is determined that a change in the patient's condition has occurred. By referring to increased number of kinds of data, changes in the patient's condition can be more accurately observed. Furthermore, when the system 104 determines abnormal data, it is also possible to produce, for example, a warning sound from the data processing device.

[0045] Although in the foregoing embodiments, an anesthetic agent is supplied in the form of an anesthetic gas, the invention is also applicable to a case where an anesthetic agent is administered by drip infusion or the like.

[0046] Furthermore, although in the foregoing embodiments, measured data regarding the pulse wave is converted into a blood pressure signal before being inputted to the data processing device 10, measured data regarding the pulse wave may also be directly inputted and subjected to data processing.

[0047] While the present invention has been described with reference to what are presently considered to be preferred embodiments thereof, it is to be understood that the present invention is not limited to the disclosed embodiments or constructions. On the contrary, the present invention is intended to cover various modifications and equivalent arrangements.

Claims

1. A biological data observation system (101, 102, 103, 104) for monitoring an anesthetic depth of a patient, characterized by comprising:

first measuring means (30) for measuring a first

biological data (S) based on an amount of perspiration of the patient;

data processing means (10) for substantially continuously receiving the data measured by the first measuring means (30) and for determining a transition of the data; and means (13) for externally indicating the transition of the data determined by the data processor means (10).

2. A system according to claim 1, characterized by further comprising second measuring means (20) for measuring a second biological data (P) based on a pulse wave of the patient, wherein the data processing means (10) substantially continuously receive the data measured by the second measuring means (20) and for determining a transition of the data.

3. A system according to claim 2, characterized in that the data processing means (10) calculates a third biological data (PS) based on the first biological data (S) and the second biological data (P).

4. A system according to claim 2 or 3, characterized by further comprising:

an anesthesia device (42) that is capable of substantially continuously administering an anesthetic agent to the patient; and anesthetic administration control means (46) for calculating a third biological data (PS) based on the first biological data (S) and the second biological data (P), and for adjusting an amount of the anesthetic agent administered by the anesthesia device (42), based on the third biological data (PS) calculated.

5. A system according to any one of claims 2 to 4, characterized by further comprising warning means (10, 47) for outputting a warning signal when at least one of the first biological data (S) and the second biological data (P) becomes out of a predetermined range.

6. A system according to any one of claims 2 to 5, characterized by further comprising electric current stimulation means (48) for giving an electric current stimulus to the patient when at least one of the first biological data (S) and the second biological data (P) becomes out of a predetermined range.

7. A system according to any one of claims 2 to 6, characterized in that the second biological data (P) is heart beats.

8. A system according to any one of claims 2 to 6, characterized in that the second biological data (P)

is a blood pressure.

9. A system according to any one of claims 1 to 8, characterized in that the means (13) for externally indicating the transition of the data is display means. 5

10

15

20

25

30

35

40

45

50

55

FIG. 1

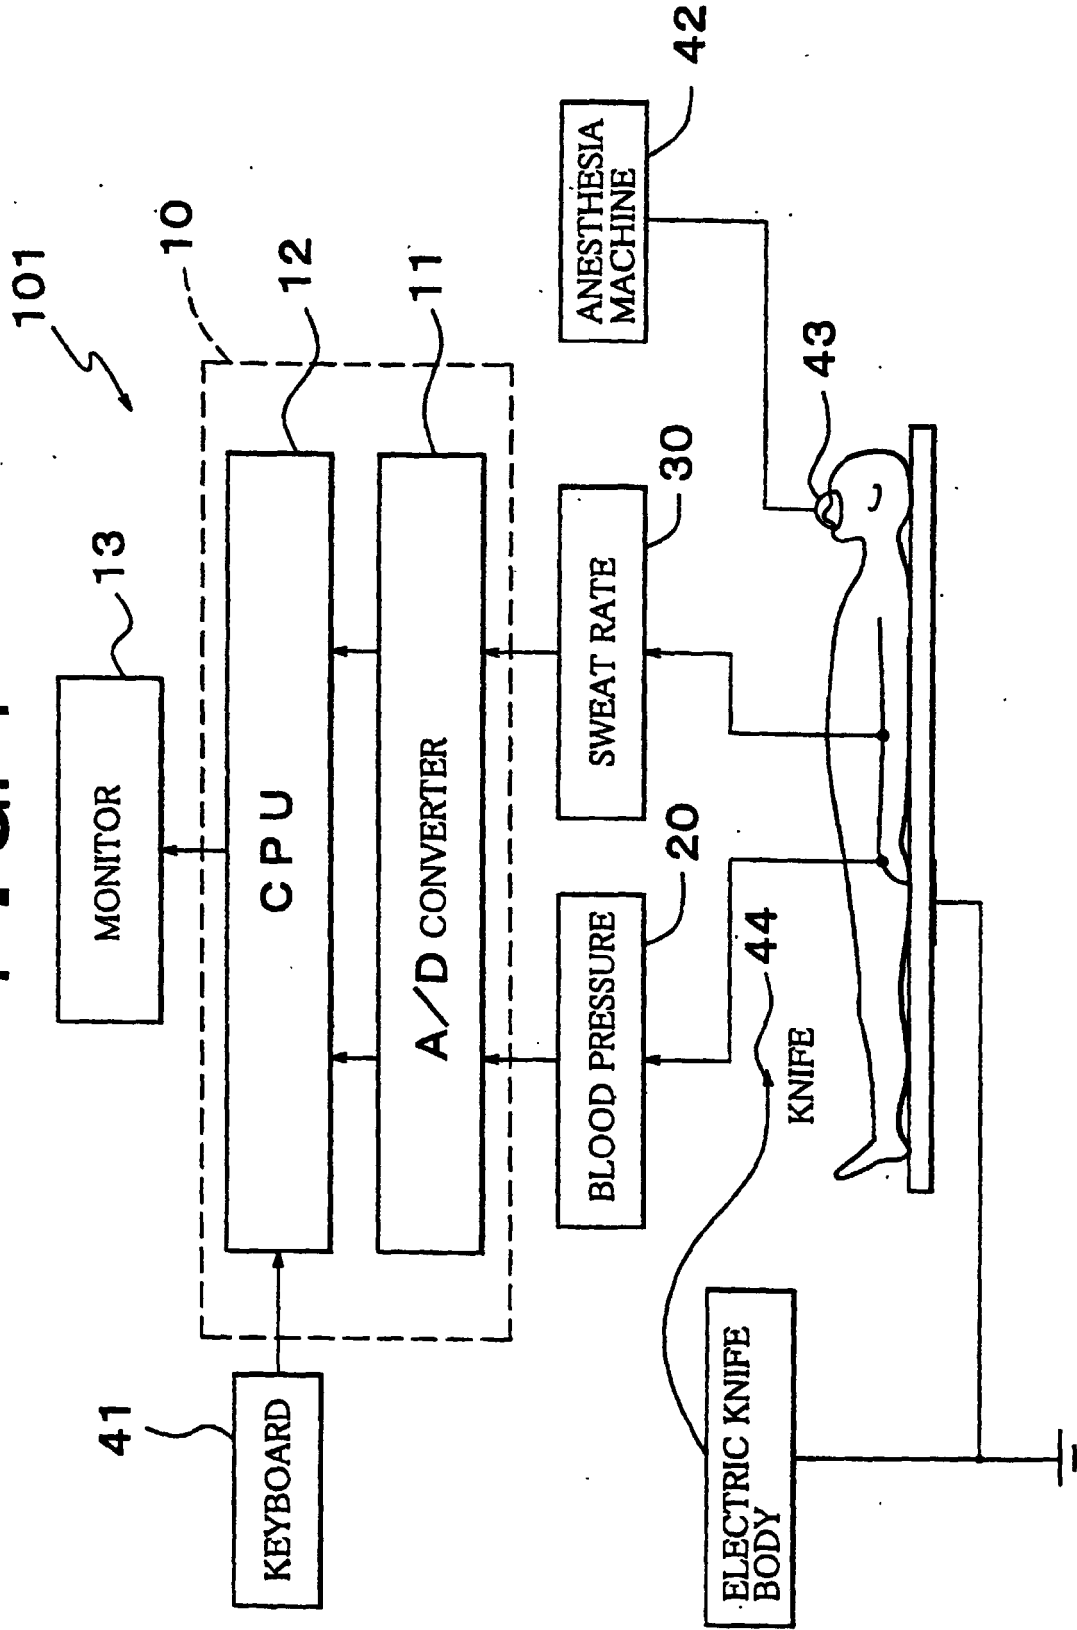


FIG. 2

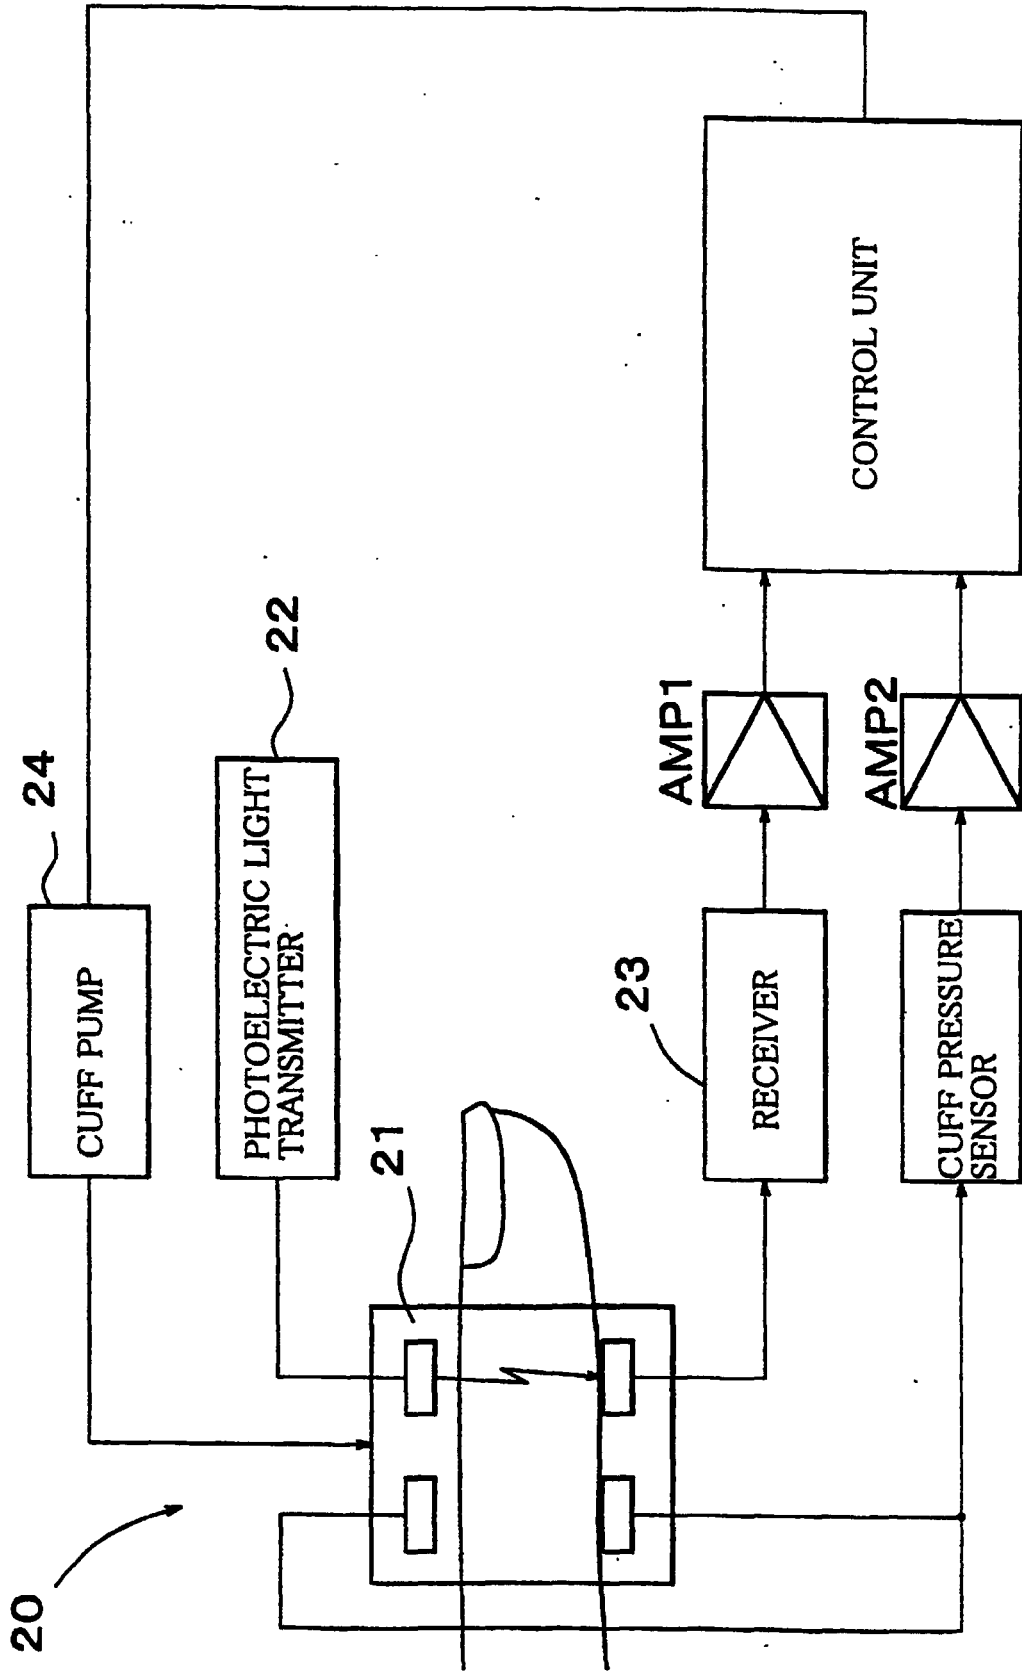


FIG. 3

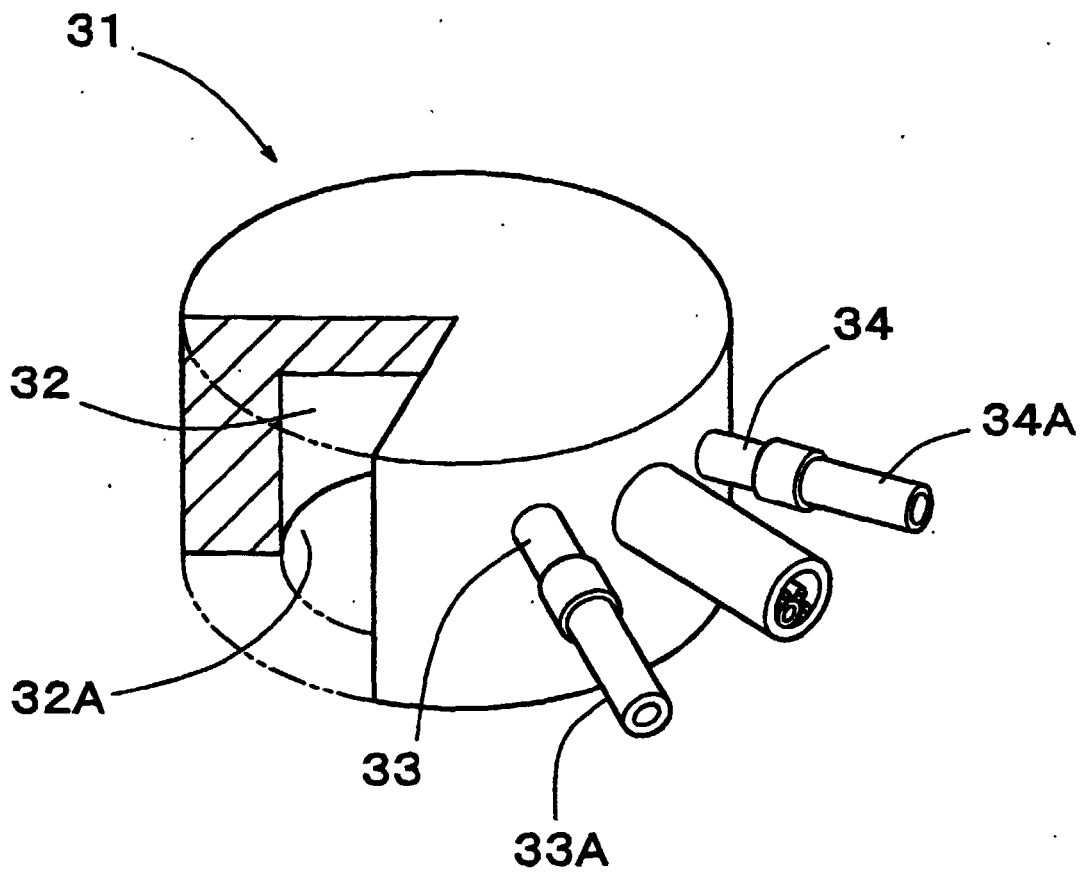


FIG. 4

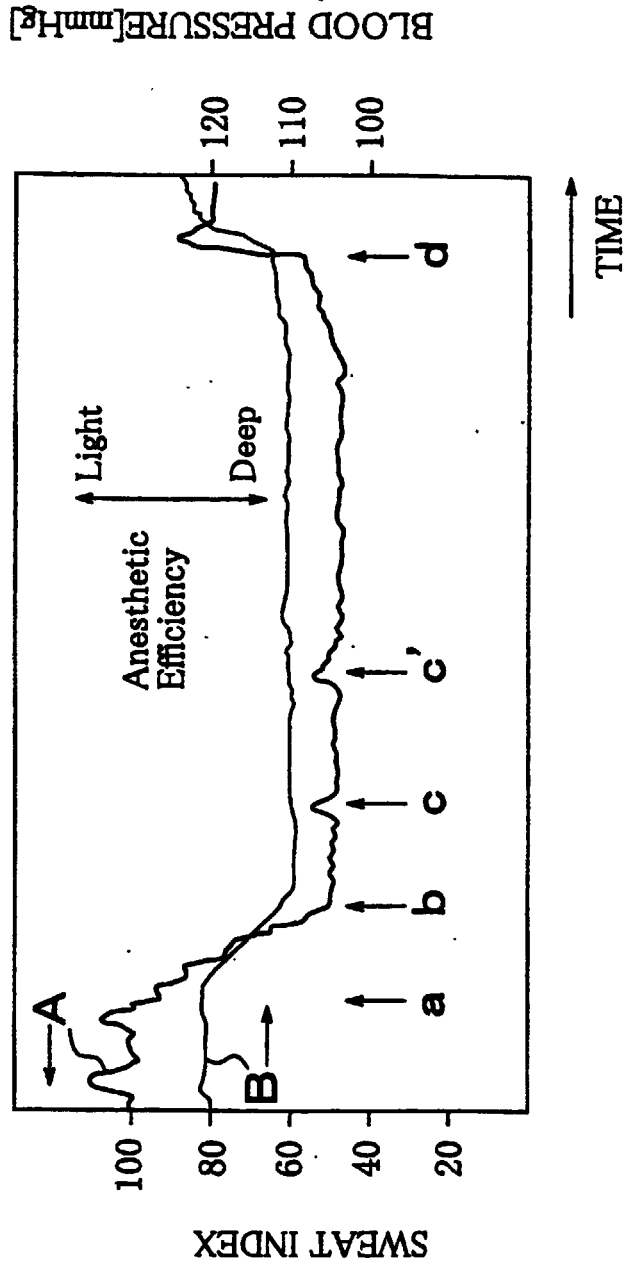


FIG. 5

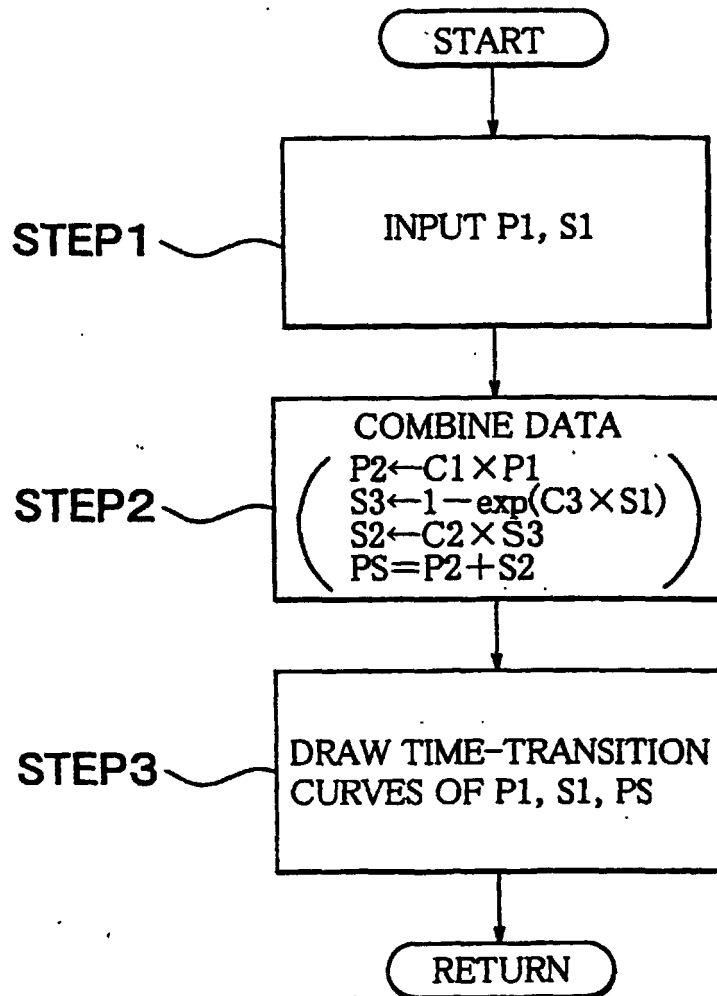


FIG. 6

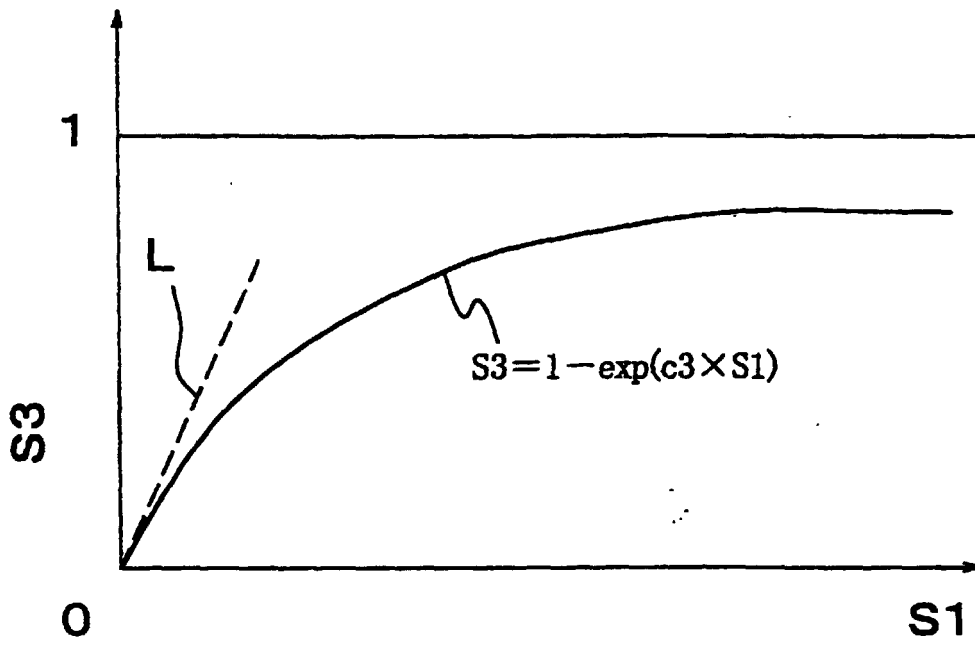


FIG. 7A

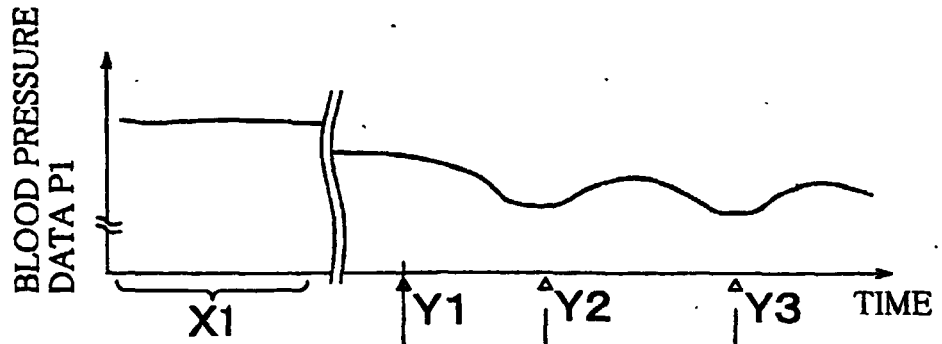


FIG. 7B

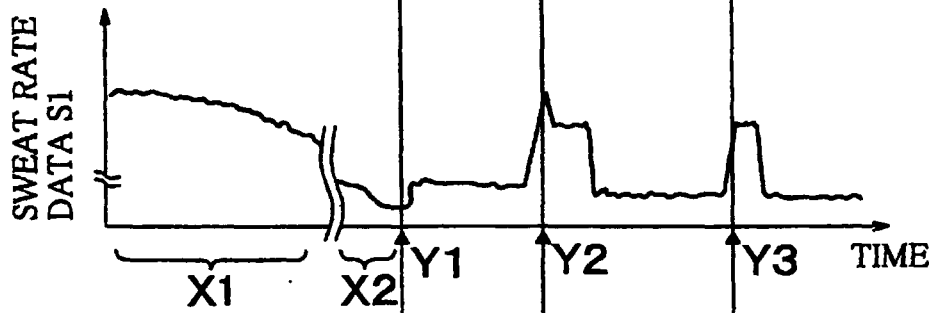


FIG. 7C

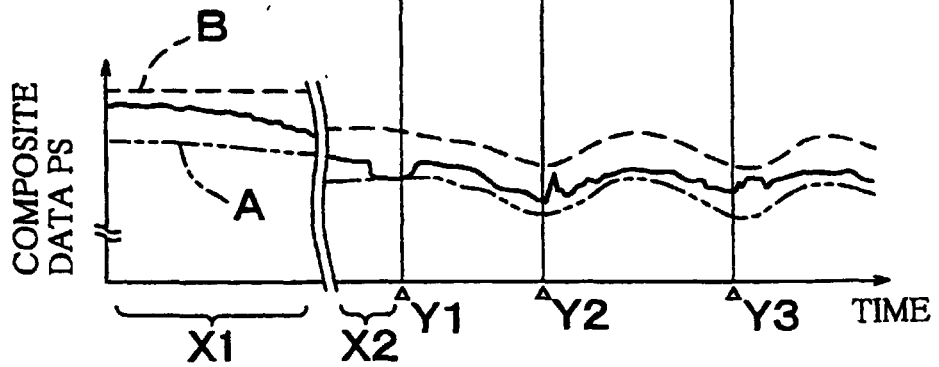


FIG. 8

BLOOD PRESSURE DATA		COMPOSITE DATA		SWEAT RATE DATA				FEMALE
		AGE	MALE	10~19	20~29	30~39		
WEIGHT		30~39 [kg]	OO mg/sec					
		40~49 [kg]	X X mg/sec			*		
		50~59 [kg]				**		
							

*(Upper Column):Normal

** (Lower Column):Anesthetized

FIG. 9

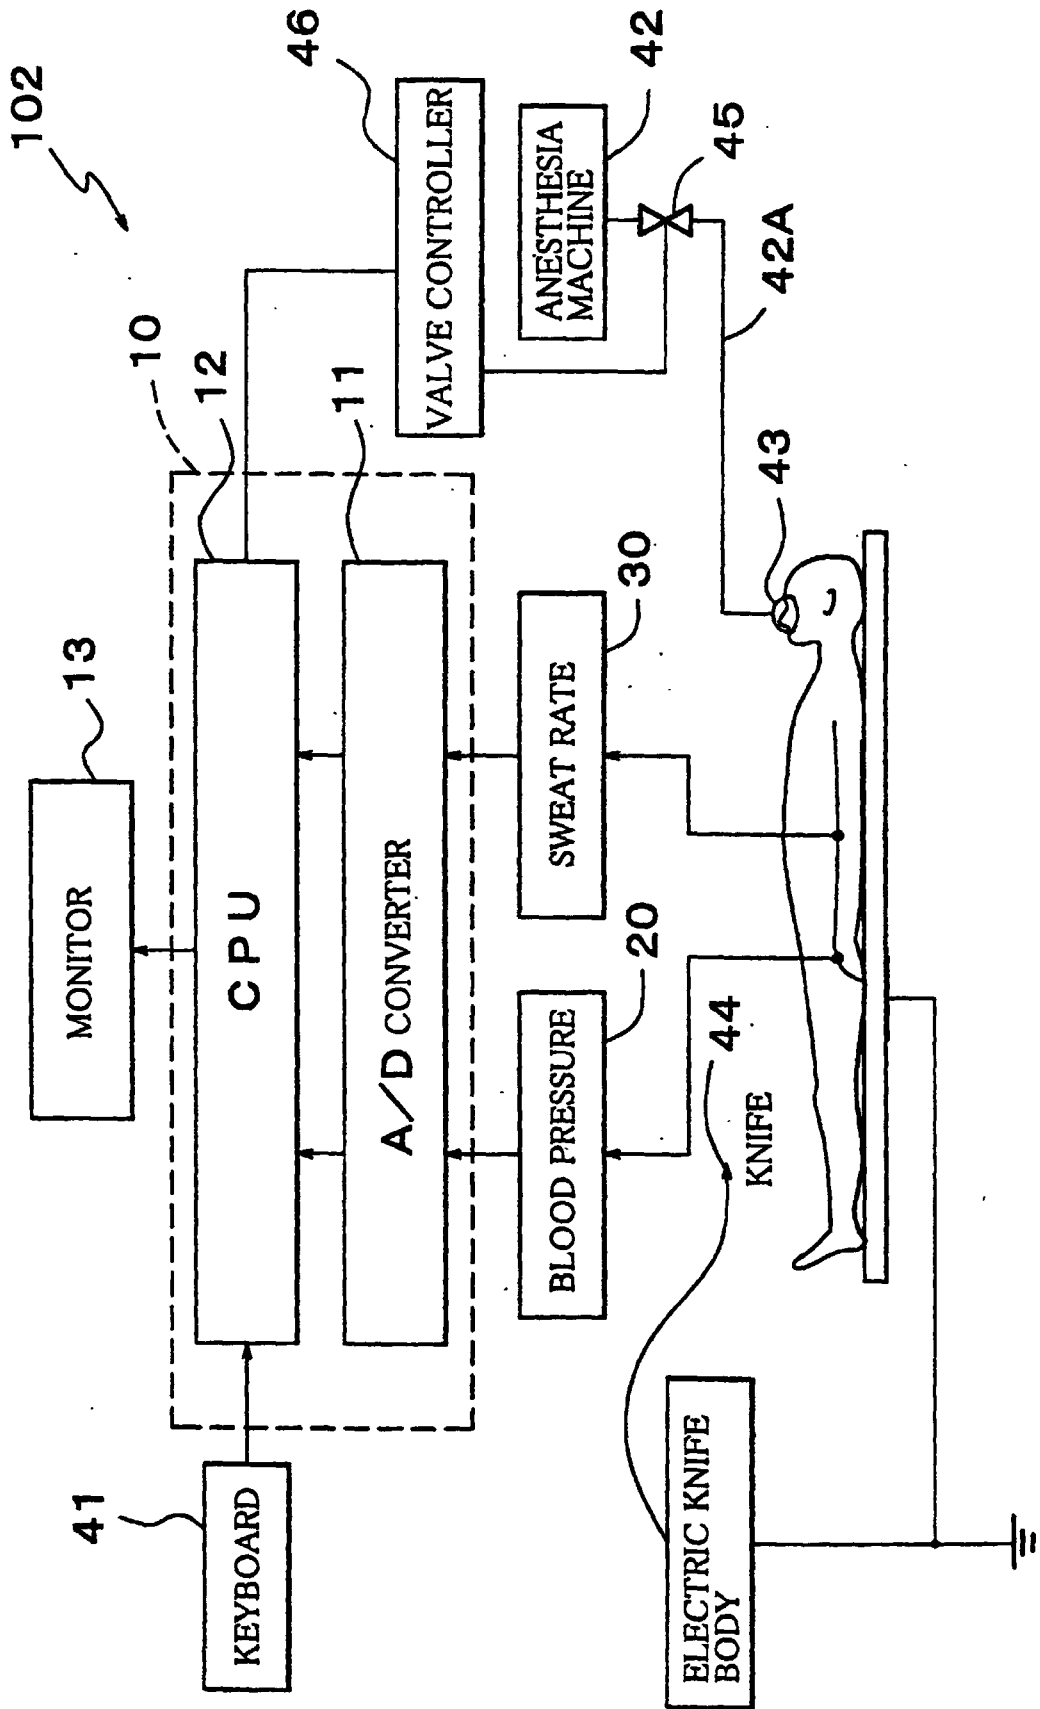


FIG. 10


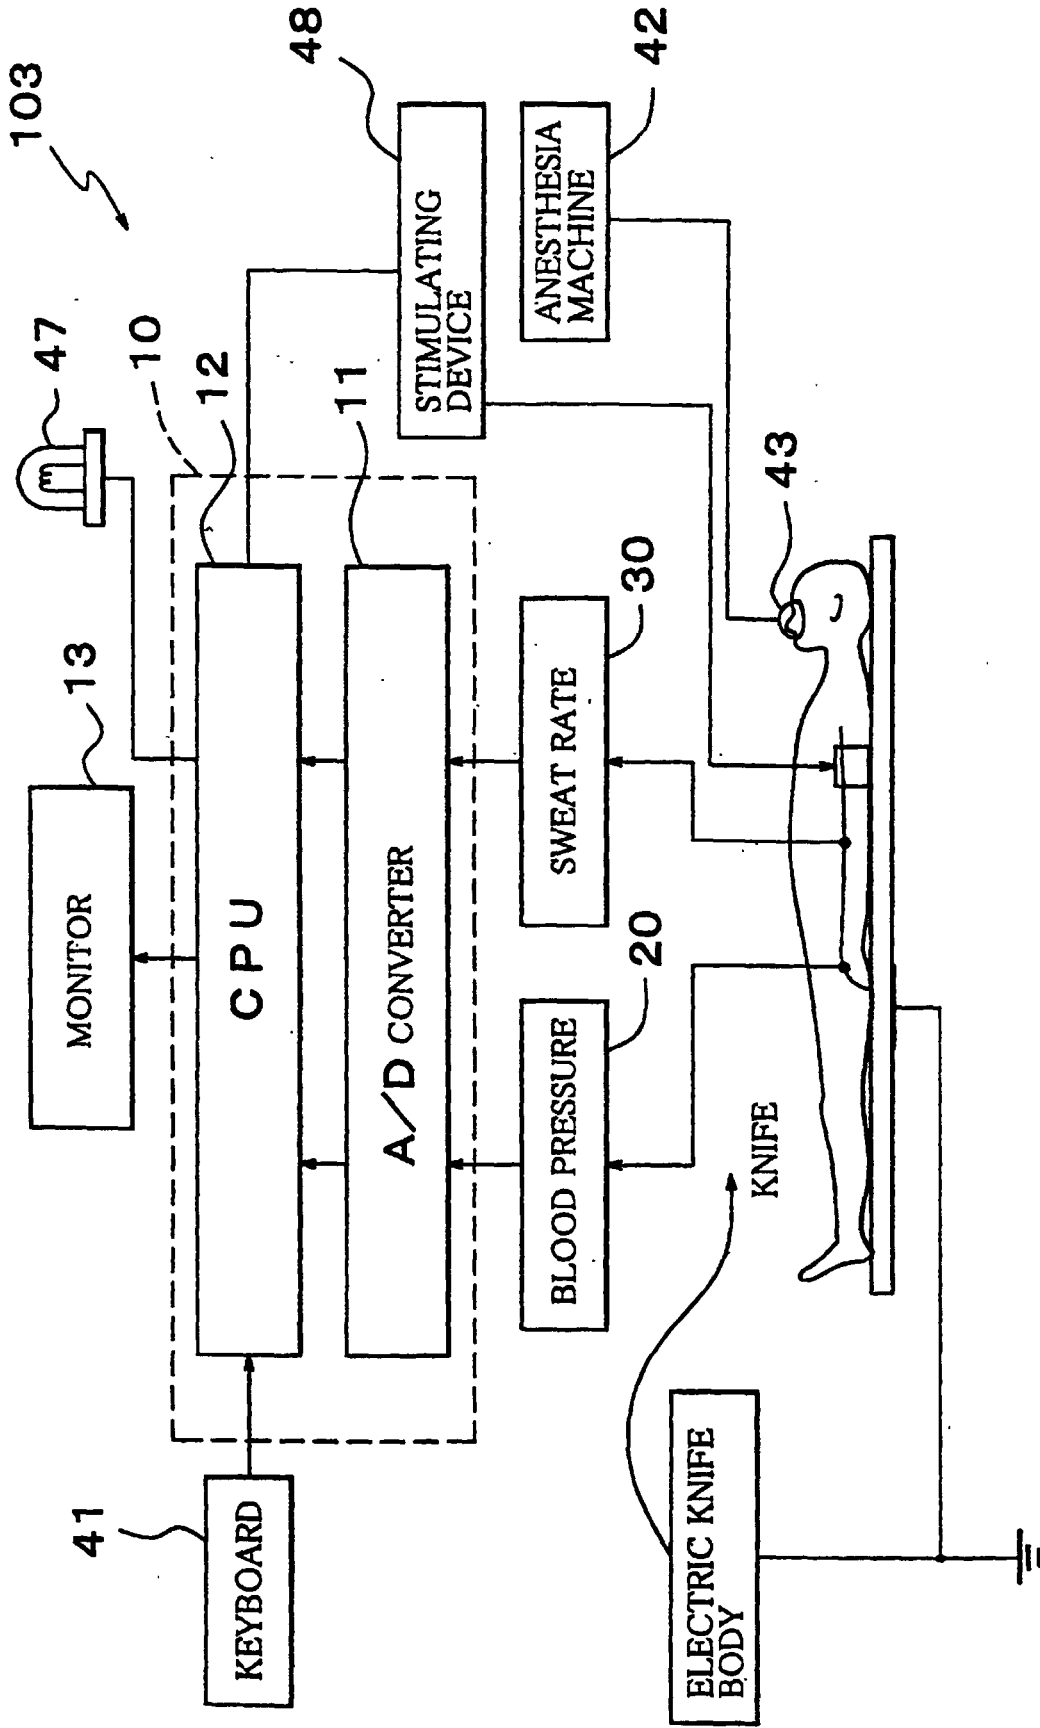


FIG. 11



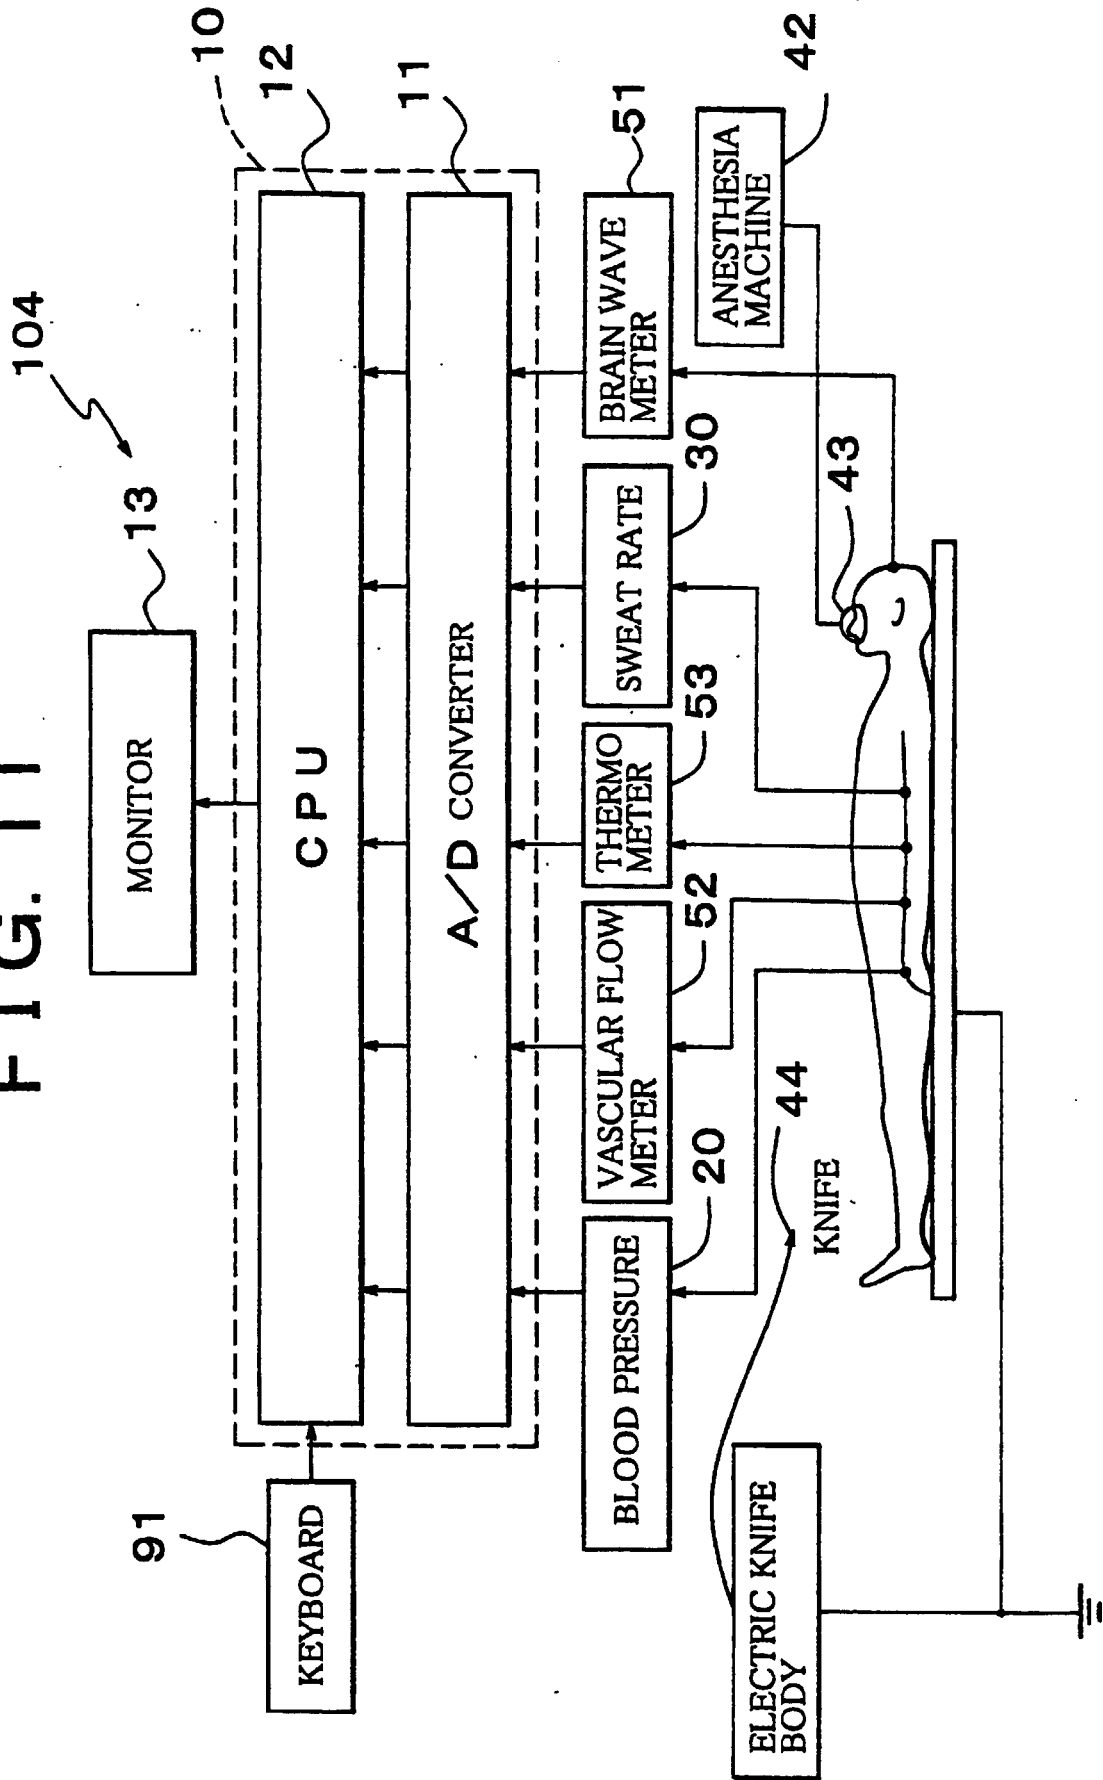

European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 00 10 8575

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.CI.7)
X	EP 0 149 866 A (ANTEC SYSTEMS LTD.) 31 July 1985 (1985-07-31) * page 5, line 14 - line 26 * * page 11, line 12 - page 13, line 9 * * page 32, line 11 - page 36, line 18 * ---	1-4,6-8	A61B5/11
A	EP 0 787 506 A (J.J. RODIERA OLIVE) 6 August 1997 (1997-08-06) * column 1, line 1 - line 17 * * column 7, line 3 - line 32 * * column 8, line 41 - column 9, line 59 * ---	1,2,4-8	
A	US 4 013 067 A (H. KRESSE ET AL.) 22 March 1977 (1977-03-22)	1-3,5,7	
A	* column 1, line 7 - line 36 * * column 3, line 3 - column 4, line 48 * ---	8	
A	US 4 805 636 A (D.T. BARRY ET AL.) 21 February 1989 (1989-02-21) * column 1, line 21 - line 30 * * column 2, line 57 - column 3, line 9 * * column 5, line 7 - line 46 * -----	1,6	
			TECHNICAL FIELDS SEARCHED (Int.CI.7)
			A61B
The present search report has been drawn up for all claims			
Place of search		Date of completion of the search	Examiner
THE HAGUE		10 August 2000	Rieb, K.D.
CATEGORY OF CITED DOCUMENTS			
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03/82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 00 10 8575

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

10-08-2000

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 149866	A	31-07-1985	AT 20699 T	15-08-1986
			AT 42187 T	15-05-1989
			AU 580982 B	09-02-1989
			AU 547294 B	17-10-1985
			AU 7682881 A	06-05-1982
			CA 1193504 A	17-09-1985
			CA 1199846 C	28-01-1986
			DE 3174936 D	21-08-1986
			DE 3177031 D	24-05-1989
			EP 0050983 A	05-05-1982
			IL 64119 A	31-10-1985
			JP 57103624 A	28-06-1982
			JP 3021223 A	30-01-1991
			US 4502490 A	05-03-1985
			US 4600015 A	15-07-1986
EP 787506	A	06-08-1997	AU 702835 B	04-03-1999
			AU 6520296 A	05-03-1997
			JP 2000507111 T	13-06-2000
			US 5957860 A	28-09-1999
			CA 2201148 A	20-02-1997
			WO 9705923 A	20-02-1997
US 4013067	A	22-03-1977	DE 2430788 B	02-10-1975
			DK 278775 A,B,	27-12-1975
			FR 2284304 A	09-04-1976
			GB 1502679 A	01-03-1978
			IT 1039035 B	10-12-1979
			JP 51025391 A	01-03-1976
			NL 7506220 A	30-12-1975
			SE 7507029 A	29-12-1975
US 4805636	A	21-02-1989	NONE	

专利名称(译)	监测患者的麻醉深度		
公开(公告)号	EP1046373A1	公开(公告)日	2000-10-25
申请号	EP2000108575	申请日	2000-04-19
[标]申请(专利权)人(译)	KABUSHIKI GAISYA钾和硫		
申请(专利权)人(译)	巨峰机械厂有限公司. KABUSHIKI GAISYA K-AND-S		
当前申请(专利权)人(译)	巨峰机械厂有限公司. KABUSHIKI GAISYA K-AND-S		
[标]发明人	KONDO SHINJI URANO HIROHIDE		
发明人	KONDO, SHINJI URANO, HIROHIDE		
IPC分类号	A61B5/00 A61B5/11		
CPC分类号	A61B5/1106 A61B5/4266 A61B5/4821 A61B2505/05 A61B2562/029		
代理机构(译)	冬季, 布兰德, 弗尼斯, HÜBNER, ROESS, KAISER, polte, PARTNERSHIP		
优先权	1999112223 1999-04-20 JP		
其他公开文献	EP1046373B1		
外部链接	Espacenet		

摘要(译)

用于监测患者的麻醉深度的生理数据系统 (101,102,103,104) 基于患者的脉搏波测量信号 (S) , 并测量出汗率。如果在手术期间患者的病情发生变化, 手术医生会立即注意到系统显示的出汗率变化, 以便采取纠正措施。

