


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : A61N 5/06	A1	(11) International Publication Number: WO 00/64536	
(21) International Application Number: PCT/US00/10814 (22) International Filing Date: 21 April 2000 (21.04.00) (30) Priority Data: 60/130,497 22 April 1999 (22.04.99) US (71) Applicant: PAREL, Jean-Marie [US/US]; 332 N.E. 92 Street, Miami Shores, FL 33138 (US). (72) Inventors: MANNS, Fabrice; 1258 South Alhambra Circle #3, Coral Gables, FL 33146 (US). ROBINSON, David; 308 Medical Plaza, 4320 Wornall Road, Kansas City, MO 64111 (US). MILNE, Peter; 36 S.W. 27th Road, Miami, FL 33129 (US). DENHAM, David, B.; 7251 S.W. 52nd Court, Miami, FL 33143-5912 (US). GONZALEZ-CIRRE, Xochitl; Calle del Granado 2, Esc. 1, 501, E-28005 Madrid (ES). (74) Agents: MORDUCH, Ruth, N. et al.; Pillsbury Madison & Sutro, LLP, 1100 New York Avenue, N.W., Washington, DC 20005 (US).		(43) International Publication Date: 2 November 2000 (02.11.00)	
		(81) Designated States: AU, CA, JP, KR, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).	
		Published <i>With international search report.</i>	

(54) Title: INTRAOPERATIVE MONITORING OF TEMPERATURE-INDUCED TISSUE CHANGES WITH A HIGH-RESOLUTION DIGITAL X-RAY SYSTEM DURING THERMOTHERAPY

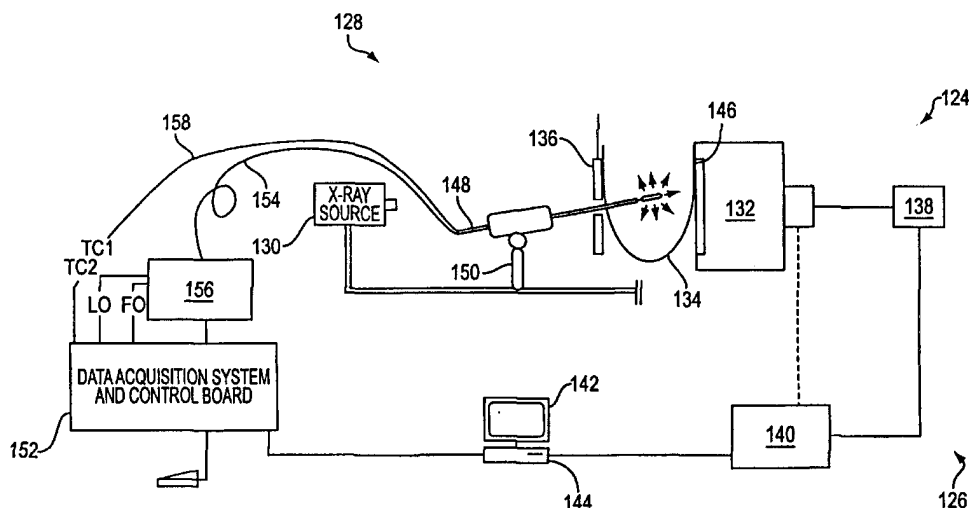

(57) Abstract

A method of thermally inducing and monitoring changes to localized regions of tissue illuminating a volume of tissue with a first beam of X-rays, detecting the portions of the first beam of X-rays that passed through the volume of tissue, generating a first X-ray image signal from the portions of X-rays of the first beam detected, applying heat to at least a localized region of tissue within the volume of tissue after the illuminating and after the detecting, illuminating the volume of tissue with a second beam of X-rays, detecting portions of the second beam of X-rays that passed through the volume of tissue during the illuminating with the second beam of X-rays, generating a second X-ray image signal from the portions of X-rays of the second beam detected and generating a difference image signal based upon a comparison of the first and second X-ray image signals. The difference image signal provides information of changes in X-ray attenuation by localized regions of tissue within the volume of tissue due to the application of heat.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon	KR	Republic of Korea	PL	Poland		
CN	China	KZ	Kazakhstan	PT	Portugal		
CU	Cuba	LC	Saint Lucia	RO	Romania		
CZ	Czech Republic	LI	Liechtenstein	RU	Russian Federation		
DE	Germany	LK	Sri Lanka	SD	Sudan		
DK	Denmark	LR	Liberia	SE	Sweden		
EE	Estonia			SG	Singapore		

INTRAOPERATIVE MONITORING OF TEMPERATURE-INDUCED TISSUE CHANGES WITH A HIGH-RESOLUTION DIGITAL X-RAY SYSTEM DURING THERMOTHERAPY

5 The U.S. Government has a paid-up license in this invention and the right in limited circumstances to require the patent owner to license others on reasonable terms as provided for by the terms of Grant or Contract No.: USAMRDC/AIBS#2459, log #B4340289, 9/15/94 to 9/14/96, awarded by the Department of Defense

10 **BACKGROUND OF THE INVENTION**

1. Field of the Invention

 This invention pertains to intraoperative monitoring methods and devices, and more particularly to intraoperative monitoring devices and methods for monitoring temperature-induced changes to tissue with high
15 resolution digital X-ray imaging and inducing the changes to the tissue.

2. Discussion of Related Art

 Various types of thermotherapy have been considered, and/or applied to the treatment of cancers. Laser interstitial thermotherapy (LITT) has received attention as a surgical procedure for the treatment of cancer tumors,
20 and particularly with respect to liver, head, neck and breast cancer.

 Laser interstitial thermotherapy is a surgical procedure for the treatment of cancer tumors in which near infra-red laser energy is delivered to the tumor site inside the body through a flexible fiber-optic probe. Some fiber

optic probes in use terminate with a light diffusing tip. The infra-red laser radiation is absorbed by the tumor cells, which results in a temperature increase and subsequent cell death of the tumor cells. The temperature distribution around the light-diffusing tip, and thus the extent of cell-death, is a function of the laser parameters, treatment time, tumor size, and shape, fiber optic tip geometry, optical properties of the tumor, and blood perfusion rates in both compressed and uncompressed treatment sites.

The treatment parameters (e.g., wavelength, power, duration, tip geometry, and tip location and orientation) must be selected so as to minimize collateral damage to healthy tissue surrounding the tumor, yet still must ensure reliable total tumor destruction. Because of tissue inhomogeneities, and inter-patient variability of the physical and biological properties of tumors, intraoperative monitoring of the treatment effect is highly desirable. Currently, intraoperative monitoring of LITT is conducted with magnetic resonance imaging (MRI) or three-dimensional ultra-sound, or by measuring the temperature at discrete locations *in-situ* with thermo-couples or thermo-sensing fluorescent probes.

Intraoperative monitoring with MRI has numerous disadvantages which include being expensive and not being able to be used with metal protected light guides which are currently used for the LITT probe. Three-dimensional ultra-sound imaging techniques are currently at an experimental stage and have not been sufficiently developed. *In situ* thermo-couples or fluorescence-based temperature probes only provide temperatures at a relatively small number of points throughout the tissue being monitored. Currently, only fluorescence-based temperature probes are approved by the FDA for clinical use.

SUMMARY OF THE INVENTION

It is thus an object of this invention to provide an intraoperative monitoring device and method used in conjunction with diagnostic procedures.

5 It is another object of this invention to provide an intraoperative monitoring device and method used in conjunction with stereotactic X-ray mammography.

It is another object of this invention to provide an intraoperative monitoring method and device that provides a high resolution X-ray image of temperature-induced changes to tissue during thermotherapy.

10 It is another object of this invention to provide an intraoperative monitoring device and method that provides a high resolution temperature map of tissue during thermotherapy.

It is another object of this invention to provide a method of thermotherapy which includes real-time monitoring of temperature induced
15 changes to tissue during thermotherapy using X-ray imaging for feedback information used during the thermotherapy.

The above, and related objects of this invention are realized by providing a device for monitoring thermally-induced changes to localized regions of tissue which has an X-ray illumination source, an X-ray detector, a
20 data storage unit in communication with the X-ray detector, an image comparison unit in comparison with at least the data storage unit and an image display unit in communication with the image comparison unit. The X-ray illumination source and the X-ray detector are arranged to reserve a space therebetween for accommodating tissue to be monitored. Preferably, the tissue
25 to be monitored is a portion of a patient's body which is being monitored during the surgical procedure. The X-ray detector produces a plurality of X-ray image data signals, each of which corresponds to an X-ray image of the

portion of the patient's body being monitored. Preferably, the X-ray detector produces a digital X-ray image data signal. The X-ray image data signal corresponds to a two-dimensional image of the portion of the patient's body being monitored in a preferred embodiment, and corresponds to a three-
5 dimensional X-ray image of the portion of the patient's body in another preferred embodiment.

The image comparison unit compares X-ray image values between corresponding spatial points of first and second X-ray image signals to provide a resultant X-ray image signal based on the comparison. Preferably, the image
10 comparison unit subtracts pixel values between corresponding spatial points of first and second X-ray image signals, providing a measure of the change in intensity of the received X-ray signal at each point within the digital X-ray image signals. The resultant image signal is then one particular example of a difference image signal that is generated by the image comparison unit and
15 then displayed on an image display unit to provide real-time information concerning the temperature distribution and changes in temperature throughout the portion of the patient's body being monitored. The images also provide information corresponding to the volume of denatured tissue. In the preferred embodiment, both the data storage unit and image comparison unit are
20 implemented within a personal computer or workstation.

Another preferred embodiment of the present invention is directed to a device for causing thermally-induced changes to localized regions of tissue. The device according to this preferred embodiment has an X-ray illumination source, an X-ray detector, a data storage unit in communication with the X-ray
25 detector, a thermotherapy heating assembly, an image comparison unit in communication with at least the data storage unit and an image display unit in communication with the image comparison unit. The combination of X-ray illumination source, X-ray detector, data storage unit, image comparison unit, and image display unit are constructed and arranged in a manner similar to the

monitoring device summarized above. The thermotherapy heating assembly may be selected from currently known devices and may include a laser irradiation devices, microwave irradiation devices, radio frequency irradiation device, or an ultra-sound energy source. In the preferred embodiment, the thermotherapy heating assembly is a laser interstitial thermotherapy assembly. There are laser interstitial thermotherapy assemblies known in the art that are suitable for use with the device for causing thermally-induced changes to localized regions of tissue, in accordance with this invention. For example, the laser interstitial thermotherapy devices described in Robinson, David S. et al, "Interstitial Laser Hyperthermia Model Development for Minimally Invasive Therapy of Breast Carcinoma", *J. Am Coll Surg*, 1998, reprint pages 284-292; Milne, Peter J. et al, "Development of Stereotactically Guided Laser Interstitial Thermotherapy of Breast Cancer: In Situ Measurement and Analysis of the Temperature Field in Ex Vivo and In Vivo Adipose Tissue," *Lasers in Surgery and Medicine*, 2000, reprint 26:67-75; and Manns, Fabrice et al, "In Situ Temperature Measurements With Thermocouple Probes During Laser Interstitial Thermotherapy (LTT): Quantification and Correction of a measurement Artifact," *Lasers in Surgery and Medicine*, Vol. 23, No. 2, 1998, reprint pages 94-103 are suitable: the entire content of each is incorporated herein by references.

Another preferred embodiment of this invention is directed to a method of thermally inducing and monitoring changes to localized regions of tissue, including illuminating a volume of tissue with a first beam of X-rays, detecting portions of the first beam of X-rays that pass through localized regions of tissue within the volume of tissue, generating a first X-ray image signal from the portions of the first X-ray beam detected, and applying heat to at least a localized region of tissue within the volume of tissue. A preferred embodiment of the method is directed to thermally inducing and monitoring changes to tumors in breast cancer patients. After applying the heat, the volume of tissue is illuminated with a second beam of X-rays. X-rays from a

second beam of X-rays that pass through the volume of tissue that includes the localized regions, e.g., through the tumors, are detected and a second X-ray image signal is generated therefrom. In the preferred embodiment, the first X-ray image signal is stored in a data storage unit and then retrieved for
5 generating a resultant image signal which preferably is a difference image signal based upon a comparison of the first and second X-ray image signals. In a preferred embodiment, the first and second X-ray image signals and the difference image signal are digital signals and the difference image signal is formed by subtracting each pixel value of the first X-ray image signal from a
10 spatially corresponding pixel of the second X-ray image signal. Each X-ray image signal is correlated with the detected X-ray intensity corresponding to the particular spatial point, and the difference image signal corresponds to an intensity change in the detected X-rays for each corresponding difference image point. The difference image signal is rendered as a difference image
15 and displayed on an image display device, preferably, to provide real-time feedback to the surgeon applying thermotherapy. The surgeon can then determine whether to alter the thermotherapy parameters, maintain the thermotherapy, or terminate the thermotherapy with the aid of the temperature change information displayed on the image display device.

20 If the surgeon decides to continue the thermotherapy, the volume of tissue is illuminated with a third beam of X-rays. (The X-ray beams may be along the same or modified paths relative to the volume of tissue.) The X-rays from the third beam that pass through the volume of tissue are detected and a third X-ray image signal is generated therefrom. The second and third beam of
25 X-rays may be separated in time by a period in which there is no illumination of X-rays, or it may be a continuous illumination classified as contiguous time periods. Continuous illumination is currently less preferable than intermittent illumination due to safety concerns regarding the total X-ray dose applied to the patient.

The first X-ray image signal is again retrieved from the data storage unit and used as a static reference image signal to produce a second difference image signal by subtracting each corresponding pixel of the first and second image signals. The second difference image signal is then rendered and
5 displayed as an updated difference image which provides updated information to the surgeon, preferably in real time. The surgeon can then use the temperature change information displayed to reassess the status of the thermotherapy to determine whether to alter, continue or terminate the thermotherapy.

10 This process is repeated until the surgeon determines that the thermotherapy should be terminated. In this embodiment, the difference image signal is always generated by retrieving the same static reference image signal from the data storage unit and subtracting it from the updated measurement signal.

15 The above detailed description of a succession of measurements is by way of example. The reader should recognize from the teachings herein that the scope and spirit of the invention includes the general concepts and not the particular order of observing and responding to the observations.

In an alternative embodiment, all method steps are the same as those
20 noted above, except that a static reference image signal is not used to generate the difference image signal. In this preferred embodiment, the first X-ray image signal is replaced by the second X-ray image signal after the first difference image signal is generated. Similarly, the second X-ray image signal stored in the data storage unit is replaced with the third X-ray image signal
25 after the second difference image signal is generated. This process is repeated until the surgeon determines that the thermotherapy should be terminated. This case provides a dynamic reference image signal for forming the difference image signal in which the dynamic reference image signal is updated after each succeeding illumination.

In alternative embodiments, one may combine both static and dynamic processes for generating the difference image signals. For example, the reference image signal may be maintained in memory without being replaced for one, two or more successive illuminations, followed by being updated
5 either frequently, such as with a pure dynamic reference image signal, or intermittently, again being a mix of dynamic and static processes.

Another embodiment of the invention is directed to a method of destroying cancerous tissue by forming a first X-ray image of a portion of a patient's body, applying heat to a localized region of the portion of the
10 patient's body, forming a second X-ray image of the portion of the patient's body subsequent to applying heat to the localized region of the portion of the patient's body, and generating a difference image based on a comparison of the first X-ray image data to the second X-ray image data. The surgeon then modifies the application of heat based on information obtained from the
15 difference image. In a preferred embodiment, the first and second X-ray images and the difference X-ray image are high resolution, three-dimensional digital X-ray images. Preferably, the comparison is a subtraction of the first X-ray image from the second X-ray image. The illumination with successive X-ray beams, detecting, generating X-ray image signals, and generating
20 successive difference image signals is repeated as the surgeon requires until he terminates the thermotherapy.

BRIEF DESCRIPTION OF THE DRAWINGS

These and other objects and advantages of the invention will become more apparent and more readily appreciated, from the following detailed
25 description of the presently preferred exemplary embodiments of the invention taken in conjunction with the accompanying drawings, of which:

FIGURE 1 is a schematic illustration for explaining general concepts of the invention;

FIGURE 2 is a schematic illustration of a device for causing and monitoring thermally induced changes to localized regions of tissue in accordance with a preferred embodiment of the invention;

FIGURE 3A is a partially cut-away view of a probe within a heating
5 assembly in a preferred embodiment of this invention;

FIGURE 3B is a side view of an end of the probe illustrated in FIGURE 3A;

FIGURE 4 is a schematic illustration of applying heat to a tumor in accordance with the preferred embodiment of this invention;

10 FIGURE 5 is a flowchart illustrating a preferred embodiment of a method according to this invention;

FIGURE 6 is a flowchart illustrating another preferred embodiment of a method according to the invention;

15 FIGURE 7 is a graph showing average X-ray intensity in the region of interest (diffusing fiber experiment);

FIGURE 8 is a graph showing average X-ray intensity in the region of interest (bare fiber experiment);

FIGURE 9 is a schematic illustration of the region of interest with respect to a thermotherapy probe for the experiments of FIGURES 7 and 8;

20 FIGURE 10 shows graphs of changes of average X-ray intensity as a function of time for experimental regions of interest as illustrated in FIGURE 9;

FIGURE 11 illustrates desired hypothermic effects in accordance with the invention;

FIGURE 12 is a plot of intensity data as a function of time over entire images taken every thirty seconds during an experiment in accordance with the invention;

FIGURE 13 is a plot of intensity data as a function of time over whole
5 images taken every six seconds in accordance with the invention;

FIGURE 14 is a plot of maximum pixel intensities in an experiment in accordance with the invention for thirty second firing sequence of the laser;

FIGURE 15 is a graph of maximum pixel intensities as a function of time in a second experiment for six second firing sequences of the laser;

10 FIGURE 16A illustrates transfer function as a function of intensity on a linear scale;

FIGURE 16B illustrates a transfer function vs. intensity change on a logarithmic scale;

FIGURE 16C illustrates a transfer function vs. intensity change for a
15 desired function;

FIGURE 17A is an initial subtracted image on a linear scale for data taking in accordance with a preferred embodiment of this invention;

FIGURE 17B is an initial subtracted image on a logarithmic scale for data taken in accordance with a preferred embodiment of this invention;

20 FIGURE 18A is a subtracted image after 3 minutes of laser firing on the linear scale for data taken in accordance with a preferred embodiment of this invention (difference image);

FIGURE 18B is a subtracted image on a logarithmic scale corresponding to the case of FIGURE 18A (difference image);

FIGURE 19A is a subtracted image after 7 minutes of laser firing on a linear scale for data taken in accordance with a preferred embodiment of this invention (difference image);

FIGURE 19B is a subtracted image after 7 minutes of laser firing on a logarithmic scale for the case corresponding to FIGURE 19A (difference image);

FIGURE 20A is a subtracted image after 4 minutes of cooling down on a linear scale for data taken in accordance with a preferred embodiment of this invention (difference image);

FIGURE 20B is a subtracted image on a logarithmic scale for the case corresponding to FIGURE 20A (difference image);

FIGURE 21A is a subtracted image after 7 minutes of cooling down on a linear scale for data taken in accordance with a preferred embodiment of this invention (difference image); and

FIGURE 21B is a subtracted image on a logarithmic scale corresponding to the case of FIGURE 21A (difference image).

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

We first explain the general concepts of the invention with reference to FIGURE 1. FIGURE 1 is a schematic illustration of a volume of tissue 100 which contains a localized region of tissue 102. In the preferred embodiments, the localized region of tissue 102 is a tumor formed of cancerous tissue. The volume of tissue 100 is illuminated with a collimated beam of X-rays 104 illustrated schematically in FIGURE 1 as a heavy arrow and also labeled I_0 representing the intensity of the collimated X-ray beam. The collimated X-ray beam 104 has a plurality of beam portions, one of which is labeled 106 in

FIGURE 1, that pass through a portion of the volume of tissue 100 for a distance 108 before reaching the depth of the tumor 102. The tumor 102 is represented as having a simple structure in FIGURE 1 for the purpose of illustrating the general concept of the invention. For facilitating the explanation, the tumor 102 has a uniform thickness 110 along the direction of the path of the X-ray beam 104. In FIGURE 1, the X-ray beam is illustrated as a collimated beam to facilitate the discussion. The X-ray beams emitted by sources currently used are diverging beams. Portions of the X-ray beam such as 106 pass through the volume of tissue 100 without passing through the tumor 102 and emerge from the volume of tissue 100 at an opposing side 112 of the volume of tissue 100. Again, for facilitating the explanation of the general concepts of the invention, the volume of tissue 100 is also assumed to have a simple structure in which it has a uniform width which is the sum of the distances 108 to reach the tumor 102, plus the distance 110 in order to pass by or through the tumor 102, plus the distance 114 to pass from an opposing end 116 of the tumor 102 to exit the volume of tissue 100 at the opposing end 112 of the volume of tissue 100.

It is well established that electromagnetic radiation has a dual nature in which it can be thought of as a collection of a plurality of photons, or may be thought of as an electromagnetic wave or waves. The particle view is convenient to imagine that the X-ray beam is a collection of a large number of particles, i.e., photons, in which some of the plurality of photons traverse a path which misses the tumor 102, while another plurality of photons traverse a path through the volume of tissue 100 and then pass through the tumor 102. Photons traveling along a path 106 miss the tumor 102 and exit the volume of tissue 100 at the opposing end 112 after traveling through a distance of tissue which is the sum of the distances 108, plus 110, plus 114. In this illustrative example, the collection of all photons which pass above the tumor 102 in FIGURE 1 and exit the opposing end 112 of the volume of tissue 100 together form an intensity sub-beam 118, as illustrated in FIGURE 1, without passing

through a tumor 102. Similarly, a portion of the X-ray beam 104 that passes through the volume of tissue 100 to emerge at the opposing end 112 below the tumor 102, as illustrated in FIGURE 1, without passing through the tumor 102 forms a sub-beam intensity 120. A portion of the X-ray beam 104 which
 5 passes through a length of tissue 108 before reaching the tumor 102, and passes through the length 110 of tumor 102, followed by passing through another length of tissue 114, emerges as an X-ray beam component 122.

Conventional X-ray observation techniques rely on the fact that the tumor tissue 102 attenuates and/or absorbs X-rays more than the surrounding
 10 tissue in the volume of tissue 100. Consequently, if the X-ray beam 104 entering the volume 100 is uniform when it enters the volume, the beam portions 118 and 120 will be more intense than the beam portion 122, due to additional attenuation and/or absorption by the tumor 102. The inventors recognized that the temperature-dependent attenuation and/or absorption of
 15 X-rays by tissue can be utilized to provide improved diagnostic methods and devices as well as to provide methods and devices for a combination of therapeutic and diagnostic techniques.

The above-described schematic illustration can also be modeled mathematically. The incident intensity is represented as I_0 and the detected
 20 intensity at a position x, y , in the plane perpendicular to the figure at opposing end 112 of the volume of tissue 100, is represented as

$$I_d(x, y) = I_0 e^{-\int \mu(x, y, z) dz} \quad (1)$$

where $\mu(x, y, z)$ is the attenuation coefficient at each three-dimensional point within the volume of tissue.

25 Upon selecting a coordinate system in which the plane orthogonal to the plane of FIGURE 1 at the opposing end 112 of the volume of tissue 100 is

an X-Y plane and the Z-direction is the direction of travel of the X-ray beam, the lengths 108, 110 and 114 are represented as z_1 , z_2 and z_3 , respectively. In the model illustrated in FIGURE 1, a photon passing along the line 106 and exiting the volume of tissue 100 at the opposing end 112 is assumed to

5 traverse a substantially homogeneous region of tissue in which the attenuation coefficient is constant in the Z-direction, and represented by μ_1 . The intensity of X-rays passing through a portion of the volume of tissue 100 within the region 118 is then represented as

$$I_2 = I_0 e^{-\mu_1(z_1 + z_2 + z_3)} \quad (2)$$

10 where the integration performed along the Z-direction leads to the factor $z_1 + z_2 + z_3$ in the exponential which is simply the total distance traveled through the volume of tissue 100 in the Z-direction. Similarly, the intensity of X-rays emerging at the region 122 that pass through two regions of normal tissue, as well as passing through the tumor, is represented as

$$15 \quad I_1 = I_0 e^{-\mu_1(z_1 + z_3) - \mu_2 z_2} \quad (3)$$

where μ_2 is the attenuation coefficient within the tumor which is substantially constant along the Z-direction, the attenuation coefficient μ_2 is generally different from the attenuation coefficient μ_1 .

Generally, the tumor 102 attenuates X-rays more than that of

20 surrounding healthy tissue. This is the case when the tumor is breast cancer. In that case, to a first approximation, one can assume that the healthy tissue causes essentially no attenuation to the beam of X-rays, while X-rays passing through the tumor are attenuated more strongly. In this approximation, equations 2 and 3 become

$$I_2 = I_0 \quad (4)$$

$$I_1 = I_0 e^{-\mu_2 Z_2} \quad (5)$$

respectively.

The inventors recognized that certain types of tissue have a temperature variation in its attenuation of X-rays. This can be represented in the above-noted illustrative model by an attenuation coefficient which varies with temperature. For example, a linear variation with temperature of the temperature coefficient $\mu = \mu_0 + bT$ leads to a temperature-dependent intensity

$$I_1(T) = I_0 e^{-\mu_0 Z_2} e^{-bT Z_2} \quad (6)$$

at the region 122. As one can see from equation 6, the intensity I_1 varies with temperature. If there was no variation in X-ray attenuation properties of the tumor with respect to changes in temperature, then b would be equal to zero, and the second factor in equation 6 would be equal to unity. In that case, comparing the intensity of X-rays sent through the tumor at different temperatures would lead to substantially the same intensity. However, since there is a temperature variation in the attenuation properties of X-rays by the tumor, the intensity according to equation 6 at a temperature T_1 is different from that of another temperature T_2 . This temperature-dependent variation in X-ray attenuation by the tumor can be exploited by observing the change in intensity I_1 as the temperature changes. For example, the ratio of the intensity at temperature T_2 to the intensity at temperature T_1 , according to equation 6 can be represented as

$$\frac{I_1(T_2)}{I_1(T_1)} = e^{-bZ_2(T_2 - T_1)} \quad (7)$$

If there were no temperature variation in the X-ray attenuation coefficient of the tumor 102, equation 7 would be equal to unity. The deviations from unity signify the temperature variations in the intensity of X-rays passing through the tumor 102. The ratio of intensities in this case is
5 taken as a measure to recognize the change in intensity of X-rays passing through the tumor 102 with changes in temperature. However, the invention includes generally comparing the changes in intensity of X-rays passing through tumors that are correlated with changes in temperature and changes induced by temperature. For example, another useful method of comparing
10 the changes of intensity of X-rays passing through the tumor with changes in temperature is to subtract the intensity values. There are innumerable measures that one may use to implement the general concept of comparing the intensity of X-rays passing through the tumor at one temperature to the intensity of X-rays passing through the tumor at another temperature. This
15 invention is directed generally to the concept of utilizing such a change in X-ray intensity with a change in temperature in methods and devices.

The following detailed description of the preferred embodiments of the methods and apparatuses of this invention will refer particularly to the application of laser interstitial thermotherapy (LITT) which is a surgical
20 procedure for the treatment of cancer tumors where near infra-red laser energy is delivered to the tumor site inside the body through a flexible fiber-optic probe that has a light diffusing tip. The inventors have found that the temperature increase generated during LITT will cause a change in the X-ray density of the heated tissue which is detectable in accordance with this
25 invention. In addition, thermal denaturation causes a variation in tissue X-ray density which is detectable according to this invention. The LITT procedure will be described in detail in the preferred embodiment; however, the general concepts of the invention include other mechanisms now known, and later developed which lead to heating tumor tissue. For example, lasers which
30 irradiate tissue with electromagnetic radiation in regions other than the near

infra-red region, microwave sources of radiation, radio frequency sources, and ultra-sound energy sources are all mechanisms that can be used to heat tumor tissue. Furthermore, the heat sources may be internally applied heat sources such as the LITT method, or they may be external sources.

5 In addition, the preferred embodiments describe applications to breast cancer in particular detail. However, it is anticipated that other forms of tissue monitoring and treatment is included within the general concept of the invention. For example, the inventors anticipate that choroidal tumors of the eye, prostate cancer, and liver cancer are also particularly suitable for tumor
10 monitoring and treatment according to this invention. The inventors anticipate that this invention is generally applicable to monitoring temperature changes in localized regions of tissue whenever the localized regions of tissue have a temperature variation in X-ray attenuation compared to a surrounding volume of tissue.

15 An example of a thermal therapy device in accordance with a preferred embodiment of this invention is illustrated in FIGURE 2, and labeled generally by reference numeral 124. The thermal therapy device 124 has a monitoring unit 126 and a heating assembly 128. The monitoring unit 126 has an X-ray illumination source 130 and an X-ray detector 132 disposed proximate to the
20 X-ray illumination source 130. A space is reserved between an X-ray illumination source 130 and X-ray detector 132 for accommodating tissue to be monitored, and/or treated, such as a portion of a person's body. In the example illustrated in FIGURE 2, a woman's breast 134 is arranged between the X-ray illumination source 130 and the X-ray detector 132 for the treatment
25 and treatment monitoring of breast cancer. A compression plate 136 compresses the patient's breast 134 in contact with the X-ray detector 132. The monitoring unit 126 has a data storage unit 138 that is in communication with the X-ray detector 132. The monitoring unit 126 also has an image comparison unit 140 that is in communication with at least the data storage

unit 138 (*see*, the dashed line in FIGURE 2). In an embodiment of the invention, the image comparison unit 140 is in communication with both the X-ray detector 132 and the data storage unit 138. The image comparison unit 140 is in communication with an image display unit 142. The image display
5 unit 142 may be a separate specially designed display unit, or may be the monitor of a personal computer or workstation 144. Each of the image comparison unit 140 and data storage unit 138 may be separate dedicated components, or may be implemented on the personal computer or workstation 144. Furthermore, the image comparison unit 140 may be a stand-alone
10 special function component, or may be implemented by programming the personal computer 144. Special function stand-alone units typically allow one to optimize performance, but at a higher cost.

In the preferred embodiment, the X-ray detector 132 is a digital detector that produces a digital X-ray image signal. The invention is not
15 limited to digital X-ray detectors, and includes analog detectors producing analog X-ray image signals. In the preferred embodiment, the X-ray detector 132 has a fluorescent screen 146 which fluoresces in the visible region of the electromagnetic spectrum upon being struck by X-rays from X-ray illumination source 130.

20 The light emitted by the fluorescent screen is detected by an array of CCD elements in the preferred embodiment. Furthermore, a preferred embodiment will typically have optical components arranged between the fluorescent screen and the CCD array (not shown in the drawings) in order to condense and focus the fluorescing light onto the CCD detector. There are
25 high-resolution digital X-ray imaging devices currently on the market for treating and monitoring breast cancer which are suitable for use according to this invention. Preferably, the monitoring unit 126 employs a three-dimensional X-ray imaging system, such as stereotactic X-ray imaging. The MAMMOVISION[®] system 85200G-2 produced by Fischer Imaging Company

was found to be suitable for use in the monitoring unit 126. The U.S. Patents Nos. 5,078,142; 5,365,562; 5,526,394; and 5,917,881, each of which is incorporated by reference herein in their entirety, describe details of various aspects of X-ray imaging systems suitable for application in the monitoring
5 unit 126.

In the preferred embodiment, the heating assembly 128 is a laser interstitial thermal therapy assembly. The LITT assembly 128 has a MAMMOGRAPHIC thermal ablative therapy probe 148 attached to sled 150 which is controlled by a data acquisition system and control unit 152. An
10 optical fiber 154 is attached to the probe 148 to transport the laser energy from the laser 156. In a preferred embodiment, the laser is a continuous wave Nd:YAG laser. The invention anticipates that other lasers such as semiconductor lasers and gas lasers will be used in particular applications. Furthermore, it is anticipated that pulsed lasers may be suitable in some
15 applications. The LITT assembly 128 also has a plurality of thermocouples 158. The insertion portion of the probe 148 is shown in more detail in FIGURES 3A and 3B. The outer layers of the probe 148 are cut-away in cross-section in FIGURE 3A to show a cross-sectional view of the quartz diffusing cap 160 and a cross-sectional view of the stainless steel tube 162.
20 The probe 148 has two thermocouples 164 and 166, respectively. The optical fibre 168 is exposed in the cut-away view of the quartz diffusing cap 160 and stainless steel tube 162. FIGURE 3B shows a side view corresponding to FIGURE 3A. FIGURE 4 is a schematic illustration of the probe 148 inserted into a tumor 170 within a surrounding volume of tissue 172.

25 FIGURE 5 illustrates a preferred embodiment of a method of thermally inducing and monitoring changes to localized regions of tissue, in accordance with the invention. A region of tissue 134 arranged between the X-ray illumination source 130 and the X-ray detector 142 is illuminated with a first beam of X-rays (*see*, FIGURE 2 in conjunction with FIGURE 5). The X-ray

detector 132 detects a plurality of portions of the first beam of X-rays after they have passed through the volume of tissue 134. The X-ray detector 132 generates a first X-ray image signal from a plurality of portions of X-rays detected from the first beam of X-rays. In a preferred embodiment, the first X-ray image signal is a digital signal. However, the general concept of the invention includes generating an analog X-ray image signal, rather than a digital X-ray image signal.

In a first preferred embodiment of a method of thermally inducing and monitoring changes to localized regions of tissue in accordance with the invention, the first X-ray image signal generated is a static reference X-ray image signal which is stored in a data storage unit 138 for later retrieval.

Heat is then applied to the tissue using an appropriate heating assembly for thermal therapy. For example, heat may be applied with the LITT assembly 128 illustrated in FIGURE 2. However, as noted above, the heat application assembly may be selected according to the particular use from known heating assemblies such as various laser assemblies, microwave heating, radio frequency heating or ultrasound heating assemblies.

The tissue 134 is then illuminated with a second beam of X-rays at a second time. The X-ray detector 132 detects a plurality of portions of the second beam of X-rays that pass through the volume of tissue from the second beam of X-rays. The X-ray detector generates a second X-ray image signal from the plurality of portions of the second X-ray beam detected, which is preferably a digital X-ray image signal.

A resultant image signal is generated based upon a comparison between the first and second X-ray image signals generated. In a preferred embodiment, the resultant image signal is a difference image signal generated by subtracting each pixel of image data of the first digital X-ray image signal from each corresponding pixel of the second digital X-ray image signal. When

the digital X-ray image signals are rendered as two-dimensional, and/or three-dimensional images, the pixel-by-pixel subtraction will correspond to subtractions at the same spatial location within the corresponding two-dimensional and/or three-dimensional image. Although the difference image
5 signal generated is based upon a subtraction of image values in the preferred embodiment, the general concept of the invention is not limited to only subtracting image values. For example, a ratio between corresponding values could be taken, or innumerable other mathematical operations could be performed, as suitable, such as dividing all values by a normalization factor,
10 etc. Furthermore, groups of pixels may first be combined in various ways, such as pixel averaging prior to the generating a difference image signal. The image may be preprocessed by two-dimensional and/or three-dimensional Fourier transformation and comparing the images in the spatial-frequency domain either with or without prior spatial filtering.

15 The difference image signal is rendered as an image, preferably rendered as a real-time image on a display screen to provide information during thermal therapy. The displayed image of the difference signal provides information on the size and/or volume of localized regions of tissue, such as denatured tissue, as well as the rate of temperature changes or temperature-
20 induced changes and the corresponding relative temperatures. The user may employ the displayed information to determine whether desired regions of tissue are receiving enough, or too much, heat, as well as determining the extent of tissue necrosis due to the thermal therapy. The displayed image may be utilized by the user to determine whether to continue the thermal therapy
25 and to determine whether the heat application parameters need to be altered. For example, the amount of heat applied may be increased, or decreased, or the location where the heat is being applied may be altered.

If the user determines that the thermal therapy should continue, heat is again applied to the tissue. The heat application may be a continuous process

in which the successive applications of heat may be considered to be contiguous time intervals. Alternatively, the heat may be applied in separate intervals, separated by periods in which no heat is applied to the tissue by the heat application assembly.

5 The region of tissue is then illuminated with another beam of X-rays in which portions are detected by the X-ray detector after they pass through the tissue. The beams of X-rays illuminating the tissue may be discrete illumination periods separated by non-illumination periods, or may be contiguous time periods forming a continuous illumination by X-rays
10 classified in time intervals. The X-rays detected after the third illumination beam of X-rays lead to a third digital X-ray image signal generated according to the preferred embodiment of the invention. The same reference X-ray signal is retrieved from the data storage unit as was previously retrieved from the data storage unit. In this embodiment of the invention, the same reference
15 X-ray image signal is used to generate difference image signals a plurality of times. This reference X-ray signal is thus called a static reference X-ray signal to indicate that it will remain unchanged for at least a plurality of difference image signals generated.

 After retrieving the static reference X-ray image signal from the data
20 storage unit and generating a second resultant image signal, preferably a difference image signal, it is then rendered on a display screen. In the preferred embodiment, the user has the displayed image available to update determinations on size and/or volume of the cancerous and/or necrotic tissue as well as a temperature map, or map of temperature-induced changes, and
25 temperature change map within the tissue area of observation. This process may then be repeated numerous times until the surgeon determines that the thermal therapy should be terminated.

 The general concepts of the invention include generating both two-dimensional, and three-dimensional X-ray image signals (e.g., stereotactic X-

ray imaging), and generating the corresponding resultant X-ray image signals. In a preferred embodiment, three-dimensional X-ray image signals are produced. In the case in which three-dimensional image signals are produced by geometric triangulation methods, at least two X-ray beams through a given point within the illumination tissue must be detected. In order to obtain such data, the X-ray illumination source and/or detector may be moved relative to a tissue being illuminated, or there may be a plurality of illumination sources and/or X-ray detection elements.

FIGURE 6 illustrates another preferred embodiment of a method of thermally inducing and monitoring changes to localized regions of tissue in accordance with the invention. The description of the method of the preferred embodiment in FIGURE 5 carries over to many of the steps illustrated in FIGURE 6. In the embodiment of FIGURE 6, the reference signal generated and stored in the data storage unit is a dynamic reference signal which is updated subsequent to each resultant image signal that is generated. After generating the resultant image signal, rendering and displaying the resultant image, determining the physical properties of the localized regions of tissue, and deciding to continue with thermal therapy, the second X-ray image signal replaces the first X-ray image signal in the data storage unit to become the updated dynamic reference signal. Heat is then applied to the tissue, followed by illumination of the tissue with a third beam of X-rays. The third beam of X-rays is detected after passing through the tissue illuminated with the X-rays, and a third X-ray signal is generated. The dynamic reference X-ray image signal is retrieved from the data storage unit and subtracted, pixel by pixel, from the third X-ray image signal to generate a second difference image signal. The second difference image signal is rendered and displayed on a display unit for a user to determine the various physical properties of the localized regions of tissue. If the surgeon determines that thermal therapy should continue, the third X-ray image signal replaces the previously X-ray signal in the data storage unit to become the up-dated dynamic reference image signal. This

process is continued repeatedly until the surgeon determines that thermal therapy should be terminated.

5 The preferred embodiments illustrated in FIGURES 5 and 6 describe using either a static reference X-ray image signal, or a dynamic reference X-ray image signal. The general concept of the invention includes a combination of both static and reference image signals in which the reference signal may be static for a period of time, dynamically updated and then could become static again to provide an unlimited range of possible combinations between the two limits.

10 The following subsections describe several experiments conducted with apparatuses and methods according to the concepts and embodiments of this invention.

MAMMOVISION EXPOSURE EXPERIMENTS ON LASER TREATMENT OF PORCINE TISSUE

15 This subsection describes preliminary imaging experiments using the MAMMOVISION System (85200G-2, Fischer Imaging Co, Denver, CO) during laser-irradiation of porcine fatty tissue with a 980 nm diode laser (AOC 25, AOC Medical Systems, South Plainfield, NJ).

The Experimental Method:

20 A 20 x 8 x 3 cm piece of fatty porcine tissue with the skin was compressed at room temperature of 25°C with the MAMMOVISION compression paddle. In a first experiment, an optical fiber with a diffusing tip with a diameter of 1.7 mm (REM series B) was inserted in the tissue after making a path with a stainless steel trocar. After the initial scout and stereo
25 images were taken to ensure that the fiber was within view of the camera, we began the auto-firing sequence. The sequence was set to take exposures every 30 seconds, although the system actually took exposures every 32 seconds.

The generator settings were 25 kV, 100 mA, and 90 mAs. The laser was fired continuously at 10 W starting after the first auto-firing exposure for approximately 9 minutes. After approximately 2 minutes, we moved the fiber back so that the tip would appear in the images. After the 18th exposure we
5 turned off the laser and continued to take exposures for 2 minutes.

In a second experiment a bare fiber with a 0.6 mm diameter was used (3M series B). The experimental procedure was the same as with the diffusing fiber. The generator settings were 25 kV, 100 mA, and 50 mAs. The laser was fired from between the third and 15th exposures and again took images for two
10 minutes of the cooling down period. It should also be noted that we varied the laser power from 5 to 10 W after one minute and from 10 to 15 W after another two minutes.

In order to measure quantitatively the difference between the exposures, the average intensity (in arbitrary units corresponding to X-ray
15 density) in a region of interest surrounding the optical fibers (~30 x 20 mm for the diffusing tip and ~26 x 18 mm for the bare fiber) was recorded for each image.

Results and Conclusion:

The average intensity of the region of interest increases approximately
20 linearly during laser treatment of the tissue (FIGURES 7 and 8). The rates at which the average intensity increases are 34 units/min for the diffusing tip experiment and 54 units/min for the bare fiber experiment. After stopping the laser, the average intensities of the regions of interest decrease, although not to their initial levels. Both the average intensity increase during laser treatment
25 and the decrease after laser treatment are higher in the bare fiber experiment.

Note:

The increases in the average intensity may either be a result of changes in the tissue density or to the camera's sensitivity to heat.

**CONTINUATION OF MAMMOVISION EXPOSURE EXPERIMENTS
ON LASER TREATMENT OF PORCINE TISSUE**

5

This section describes a continuation of the preliminary imaging experiments with the MAMMOVISION System (85200G-2, Fischer Imaging Co., Denver, CO) during laser irradiation of fatty porcine tissue with a 980 nm diode laser (AOC 25, AOC Medical Systems, South Plainfield, NJ).

10 **The Experimental Method:**

A 20 x 8 x 3 cm piece of fatty porcine tissue with the skin was compressed at room temperature of 25 °C with the MAMMOVISION compression paddle. An optical fiber (REM Series B) with a diffusing tip of diameter 1.7 mm was inserted in the tissue after making a path with a stainless steel trocar (2.1 mm diameter). The laser was fired for 6 minutes at 10 W after the first image was taken and turned off for the remainder of the experiment.

After the initial stereo images were taken to ensure that the fiber was within view of the camera, we began the auto-firing sequence. The sequence was set to take images every 30 seconds for the first 30 exposures, although the system actually took exposures every 32 seconds. At this point (approximately 15 minutes into the experiment), the auto-firing sequence was set to take exposures every 6 seconds.

The difference between the exposures was measured quantitatively by obtaining the average intensity (in arbitrary units corresponding to the optical density) in different regions of interests above and below the optical fiber (see, FIGURE 9). Regions directly surrounding the fiber were not studied

because the fiber appears to shift through the images and its appearance in a region where it was not initially placed would skew the average intensity.

Results:

The following graphs in FIGURE 10 illustrate the average intensity
5 increases during the firing of the laser (the first six minutes) and decrease and level off during the remainder of the experiment. In general, the regions closer to the optical fiber show a more significant increase in average intensity during the laser irradiation than the regions further away.

Conclusion:

10 Although the fluctuations in average intensities of the regions of interest appear small, the increases correspond with the time that the laser is on. This suggests that the increase in average intensity is correlated to the laser irradiation (possibly by its thermal effects). Since the regions further away from the optical fiber show smaller increases than the closer regions, it
15 appears that the effect of the laser irradiation on the tissue decreases with distance. The average intensities decrease after the laser is stopped and eventually level off. This may be caused by the temperature in the tissue dropping after irradiation and reaching an equilibrium.

MAMMOVISION EXPOSURE STABILITY EXPERIMENTS OF THE PMMA CALIBRATION PHANTOM

20 This subsection describes stability experiments conducted with the MAMMOVISION System (85200G-2, Fischer Imaging Co., Denver, CO) on the PMMA calibration phantom (10 x 10 x 4 cm) studied to determine if there are changes in average intensity of the 50 x 50 mm images produced by the
25 CCD camera with time during the auto-firing sequence. The effect of an additional PMMA plate behind the calibration phantom is also presented.

The Experimental Method:

The 10 x 10 x 4 cm PMMA calibration block at room temperature (25°C) was held in place before the MAMMOTEST camera with the compression paddle. In a first experiment, the auto-firing sequence was set to take exposures every 30 seconds for approximately 15 minutes (after the initial scout and stereo images were taken). The initial scout was taken in the Autoexposure mode and its parameters were used in the sequential firing. The generator was set manually at 25 kV, 280 mAs, and 100 mA for the sequential firing. The first image was accidentally taken at automatic generator settings and was not included in the data discussed below. In the second experiment, the auto-firing sequence was set to take exposures every 6 seconds for 3 minutes. The generator settings were set manually at 26 kV, 280 mAs, 100 mA.

The minimum, maximum, and average pixel value of these images were recorded. The maximum pixel intensities of the center 40 x 40 mm area of the 50 x 50 mm whole image was then compared to that of the entire image to avoid potential edge effects (*see*, FIGURE 11). A Turbo C program was written to determine the value and location of the pixel with the maximum intensity.

The final experiment compared the effect of placing an additional 0.5 cm PMMA plate, which will be used in the tissue phantom holder, between the camera and the phantom on the average pixel intensity. Three images (an initial scout and two stereo images) were taken at generator settings of 26 kV, 380 mAs, 100 mA.

Results:

The average intensity of the images in the first and second experiments are within 0.5% and 0.2%, respectively (FIGURES 12 and 13). The standard deviations of the average intensities are too small to be visible in FIGURES 12

AND 13. The maximum pixel intensities in both experiments show large variations. Much of these variations disappear when analyzing the center 40 x 40 mm region, suggesting that the artifact causing these variations occurs more frequently in the edges of the images (*see*, FIGURES 14 and 15). In the five
5 images where the variations were still apparent in the 40 x 40 mm region, the variations do not appear in a 30 x 30 mm center region. The minimum intensity values remained virtually unchanged in the center region (Tables 1-2). According to Tables 3-4, the maximum intensity occurs on the same few
10 pixels throughout the experiment. In both experiments, the maximum intensity value occurs mostly on pixel coordinates (628, 1020, maximum intensity ~ 3170) and (1018, 179, maximum intensity ~ 2400).

The average of the average intensities of the images taken in the last experiment with the additional PMMA plate is 1393, or 66% of the value without the plate, which indicates that the plate introduces a significant
15 attenuation. However, this effect may be compensated for by using other X-ray generator parameters.

Conclusion:

These experiments demonstrate that the pixel intensities of the sequential images are stable, with the exception of a few pixels.

Note:

20 The minimum pixel intensity is zero and corresponds to total attenuation (i.e., no X-ray photons reaching the camera) and a white image. The maximum pixel intensity is 4095 and corresponds to no attenuation (i.e., all X-ray photons reaching the camera) and a black image. Each pixel
25 corresponds to an area of approximately 50 x 50 μm .

Table 1: Pixel intensity data of Experiment 1 (30 s firing rate, 25 kV, 280 mAs, 100 mA)

(RMS [root mean square] represents the standard deviation of the intensity
5 over the whole image)

Time	Whole image (50 x 50 mm)				Center region (40 x 40 mm)			
	Minimum	Maximum	Average	RMS	Minimum	Maximum	Average	RMS
0	1060	3186	1588.83	19.56	1060	2024	1588.44	18.93
32	1060	2232	1589.25	19.65	1076	2142	1588.16	18.98
64	1073	2297	1588.7	19.66	1073	2106	1588.18	19.01
96	1076	3209	1588.63	19.66	1060	2219	1588.75	19.01
128	1052	2341	1588.51	19.8	1052	2197	1587.89	19.04
160	1014	2318	1587.98	19.83	1014	2222	1587.37	19.06
192	1036	3158	1587.71	19.91	1036	2139	1587.09	18.98
224	951	3219	1587.25	19.95	951	2125	1586.55	19.02
256	949	3192	1586.98	20.05	949	2193	1586.25	19.08
288	859	2204	1587.07	20.01	947	2204	1586.32	19.05
320	897	3502	1586.83	20.18	934	3502	1586.03	19.27

Time	Whole image (50 x 50 mm)				Center region (40 x 40 mm)			
	Minimum	Maximum	Average	RMS	Minimum	Maximum	Average	RMS
352	891	2194	1586.47	20.13	891	2056	1585.71	19.09
384	971	3170	1585.91	20.24	971	2204	1584.96	19.09
416	944	3436	1585.87	20.25	944	3436	1584.96	19.15
448	931	2216	1584.92	20.2	931	2104	1583.94	19.1
480	985	2225	1584.96	20.27	985	2207	1584.04	19.13
512	1151	2225	1585.21	20.26	1151	2117	1584.21	19.11
544	1048	3179	1585.47	20.37	1048	2119	1584.44	19.13
576	918	3162	1584.84	20.41	918	2093	1583.78	19.16
608	951	2406	1583.94	20.36	951	2146	1582.9	19.15
640	1191	2429	1584.76	20.41	1231	2134	1583.59	19.15
672	1176	3151	1584.53	20.45	1227	2141	1583.36	19.1
704	1098	3145	1584.13	20.45	1098	2102	1582.93	19.11
736	1088	2407	1583.24	20.4	1088	2154	1582.07	19.1
768	975	2406	1583.32	20.49	975	2203	1582.05	19.13
800	995	2377	1581.26	20.45	995	2192	1580.01	19.11
832	1004	2415	1580.55	20.45	1004	2128	1579.27	19.08

Table 2: Pixel intensity data of Experiment 2 (6 s firing rate, 26 kV, 280 mAs, 100 mA)

(RMS [root mean square] represents the standard deviation of the intensity over the whole image)

5

Time	Whole image (50 x 50 mm)				Center region (40 x 40 mm)			
	Minimum	Maximum	Average	RMS	Minimum	Maximum	Average	RMS
0	1382	2901	2080.01	23.82	1382	2752	2079.76	22.47
7	1399	2881	2080.18	23.87	1399	2751	2079.8	22.46
14	1388	2903	2080.72	23.97	1388	2780	2080.48	22.45
21	1379	4095	2080.84	24.22	1379	4095	2080.53	22.78
28	1366	3565	2080.8	24.04	1366	2743	2080.49	22.38
35	1413	3983	2081.27	24.38	1442	3983	2081.01	0.78
42	1046	3588	2080.22	24.18	1444	2814	2079.87	22.44
49	1417	3613	2080.01	24.2	1434	2764	2079.68	22.46
56	1379	3611	2078.74	24.26	1379	2774	2078.39	22.5
63	1352	3584	2077.06	24.29	1352	2747	2076.59	22.47
70	1380	2896	2076.6	24.29	1380	2806	2076.18	22.53
77	1415	2834	2077.31	24.32	1438	2798	2076.82	22.49
84	1368	2879	2077.58	24.35	1368	2774	2077.09	22.47

Time	Whole image (50 x 50 mm)				Center region (40 x 40 mm)			
	Minimum	Maximum	Average	RMS	Minimum	Maximum	Average	RMS
91	1390	3566	2078.24	24.49	1390	2759	2077.75	22.53
98	1371	3330	2078.91	24.4	1371	2800	2078.4	22.49
105	1405	2893	2078.73	24.48	1405	2790	2078.15	22.53
112	1382	2895	2079.08	24.53	1382	2784	2078.54	22.54
119	1419	4095	2078.55	24.85	1444	4095	2077.98	23.11
126	1407	2919	2079.31	24.6	1441	2755	2078.69	22.57
133	1390	2915	2078.88	24.63	1390	2772	2078.28	22.52
140	1401	2917	2078.76	24.68	1401	2779	2078.13	22.61
147	1282	2913	2079.35	24.64	1282	2802	2078.74	22.54
154	1291	2879	2079.54	24.73	1291	2745	2078.91	22.63
161	1285	2872	2079.84	24.77	1285	2787	2079.16	22.62
168	1314	2855	2079.93	24.77	1314	2729	2079.24	22.62
175	1288	2898	2079.87	24.8	1288	2723	2079.19	22.71
182	1297	2903	2079.39	24.8	1297	2744	2078.68	22.58
189	1271	2880	2078.14	24.83	1271	2744	2077.43	22.65
196	1262	2866	2078.02	24.86	1262	2746	2077.29	22.6

Table 3: Values and pixel coordinates of maximum intensities

Experiment 1				Experiment 2			
Time	Maximum	X- coordinate	Y- coordinate	Time	Maximum	X- coordinate	Y- coordinate
0	3186	628	1020	0	2901	1018	179
32	3209	628	1020	7	2881	1018	179
64	2297	966	681	14	2903	1018	179
96	2232	970	63	21	4095	834	798
128	2341	966	681	28	3565	628	1020
160	2318	977	754	35	3983	634	341
192	3158	628	1020	42	3588	628	1020
224	3219	628	1020	49	3613	628	1020
256	3192	628	1020	56	3611	628	1020
288	2204	162	534	63	3584	628	1020
320	3502	669	304	70	2896	1018	179
352	2194	977	754	77	2834	1018	179
384	3170	628	1020	84	2879	1018	179
416	3436	396	195	91	3566	628	1020
448	2216	977	754	98	3330	628	1020
480	2225	977	754	105	2893	1018	179

Experiment 1				Experiment 2			
Time	Maximum	X- coordinate	Y- coordinate	Time	Maximum	X- coordinate	Y- coordinate
512	2225	970	63	112	2895	1018	179
544	3179	628	1020	119	4095	912	171
576	3162	628	1020	126	2919	1018	179
608	2406	1018	179	133	2915	1018	179
640	2429	1018	179	140	2917	1018	179
672	3151	628	1020	147	2913	1018	179
704	3145	628	1020	154	2879	1018	179
736	2407	1018	179	161	2872	964	65
768	2406	1018	179	168	2855	1018	179
800	2377	1018	179	175	2898	1018	179
832	2415	1018	179	182	2903	1018	179
				189	2880	1018	179
				196	2866	1018	179

**ANALYSIS OF THERMALLY-INDUCED CHANGES IN
MAMMOVISION IMAGES BY PIXEL AVERAGING**

This subsection describes test results that display changes in sequential images taken with the MAMMOVISION System on the PMMA calibration phantom and on laser-irradiated fatty porcine tissue.

The images taken with the MAMMOVISION system are 50 x 50 mm images containing 1024 x 1024 pixels with each pixel corresponding to a 50 x 50 μm area. Since the desired target volume is 30 mm in diameter, the main region of interest (ROI) during treatment is a 30 x 30 mm area in the image.

- 5 These data in ASCII (text) files containing the intensity for each pixel are 5 MB each. These files are too large to handle when dealing with multiple images. In addition, the resolution of the images is much greater for each image than is necessary for thermal imaging; where a resolution on the order of 1 x 1 mm is sufficient. It is therefore beneficial to convert the images from
- 10 1024 x 1024 pixels to a smaller resolution by averaging blocks of the 1024 x 1024 into one pixel (*see*, Table 4). Another benefit of reducing the resolution is removing the noise effects generated by a few unstable pixels.

Table 4: Number of pixels and resolution of averaged images

Number of Pixels	Size of Averaged Block	Pixel Size of Averaged Images	Number of Pixels in 30 x 30 mm ROI
1024 x 1024 (no averaging)	1 x 1	50 x 50 μm	600 x 600
512 x 512	2 x 2	0.1 x 0.1 mm	300 x 300
256 x 256	4 x 4	0.2 x 0.2 mm	150 x 150
128 x 128	8 x 8	0.4 x 0.4 mm	75 x 75
64 x 64	16 x 16	0.8 x 0.8 mm	37 x 37

Stability of 1024 x 1024 Images:

- 15 In a previous experiment (*see*, above), the average pixel intensity of the entire 1024 x 1024 image of the PMMA calibration phantom is shown to be

stable within 0.5% in the sequential-firing mode. The purpose of this study was to quantify the stability of each pixel.

The Experimental Method:

The PMMA calibration block (10 x 10 x 4 cm) was held in place
5 before the MAMMOVISION (85200G-2, Fischer Imaging Co., Denver, CO) camera with the compression paddle at room temperature (25 °C). The initial scout was taken at 0° in the Autoexposure mode and its parameters were used in the subsequent firing. The generator was set manually at 25 kV, 280 mAs, and 100 mA for the sequential firing. The auto-firing sequence was set to take
10 exposures every 30 seconds for approximately 14 minutes for a total of 27 images. A Turbo C program was written to find pixels that changed in intensity by more than 20% between two successive images.

Results:

The analysis of the 27 1024 x 1024 images revealed that only 90 pixels
15 showed significant variation (>20%) at least once during the experiment (Table 5). The maximum number of pixels that changed by more than 20% from one image to the next was 19. This analysis corroborates the earlier findings that the pixel intensities of the sequential images are stable, with the exception of a small percentage of pixels.

Table 5: Coordinates of pixels with intensity change greater than 20%

X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change	X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change
15	538	3	23.2	711	1011	4	131.5
157	110	2	22.6	716	12	1	23.4
162	534	10	38.8	731	805	2	34.4
181	473	4	44.5	743	241	2	22.2
208	521	10	30.1	745	646	8	46.5
212	584	14	32.6	749	358	5	40.0
227	23	3	25.1	774	970	2	23.1

X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change	X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change
234	992	1	-30.4	778	703	2	22.2
253	516	1	20.4	789	938	6	27.3
302	275	6	-39.6	808	527	1	44.2
305	652	4	23.1	809	415	3	22.8
312	601	7	52.3	825	586	2	24.9
327	474	6	40.9	830	238	1	20.2
329	1004	6	34.6	847	127	1	21.3
340	768	3	50.0	854	630	8	44.8

X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change	X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change
344	408	1	24.6	892	604	4	32.2
389	885	3	75.5	903	670	1	20.7
395	4	7	36.2	903	832	4	26.7
396	195	2	115.6	909	714	1	21.5
421	882	1	22.8	912	208	1	20.5
457	899	5	28.9	924	663	8	92.5
459	906	3	38.3	926	164	5	48.4
472	488	4	33.6	928	468	3	22.7

X- coordinate	Y- coordinate	Number of Occurrences	Maximum Percent Change	X- coordinate	Y- coordinate	Number of Occurrences	Maximum Percent Change
476	324	1	-20.8	929	983	7	75.4
484	304	2	24.2	932	474	6	38.5
484	584	1	20.4	935	986	3	28.3
493	178	1	25.8	942	262	1	23.8
494	770	4	66.6	947	400	2	20.8
528	113	1	-21.7	964	65	6	59.7
536	853	4	61.4	966	681	1	20.1
571	217	2	56.2	970	63	5	89.5

X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change		X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change
572	1001	2	22.5		976	958	3	26.9
603	162	2	31.0		978	25	1	20.7
614	906	6	32.4		979	161	1	27.9
624	153	1	20.2		981	234	1	27.2
628	1020	10	99.6		986	281	1	24.7
635	724	1	23.8		987	878	2	21.3
653	66	4	25.5		994	221	8	42.1
660	978	4	35.3		995	53	2	-28.6

X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change	X-coordinate	Y-coordinate	Number of Occurrences	Maximum Percent Change
669	303	2	34.4	997	91	3	23.2
669	304	2	123.3	1000	791	1	24.5
669	388	2	22.3	1003	809	7	36.5
670	304	2	62.2	1014	669	4	25.6
674	388	1	23.7	1017	280	1	27.7
682	0	4	83.9	1018	179	2	56.1
686	947	2	22.9	1022	898	13	31.0

Table 5: Coordinates of pixels with intensity change greater than 20%

Stability of 128 x 128 Images

This subsection describes results of quantifying the stability of the
5 pixel intensities of 128 x 128 averaged images.

The Experimental Method:

The images used in the previous analysis were converted from 1024 x
1024 pixel images into 128 x 128 pixel images by averaging 8 x 8 pixel blocks
into one pixel, by using a Turbo C program. These images were then analyzed
10 by another Turbo C program to find pixels that changed in intensity by more
than 2%.

Results:

In the 27 128 x 128 pixel images, only 8 pixels showed variation of
greater than 2% (*see*, Table 6). The maximum variation was 3.3%, which was
15 in a pixel that increased by that percentage in one image and then decreased to
approximately its original value in the next image. No other pixel showed
more than a 2% change more than once. The maximum number of pixels
changing by more than 2% between two consecutive images was 2. These
results indicate that any image changes of more than 5% in 128 x 128 images
20 will be significant (above noise level) during laser-irradiation.

Table 6: Coordinates and image number of pixels with over 2% intensity change in the 128 x 128 images

X-coordinate	Y-coordinate	Image number	Percent change
6	73	4	-2.04
10	59	15	-2.07
35	96	20	2.13
49	24	15	2.16
78	127	24	2.15
83	38	11	-3.12
83	38	12	3.44
92	5	3	2.17
120	73	17	2.03

Colorized Display of Changes in Laser-Irradiated Tissue:

This subsection describes displaying the changes in X-ray intensity of laser-irradiated tissue in color according to this invention.

The Analytical Method:

The images of the laser-irradiated fatty porcine tissue were obtained from a previous experiment. A 20 x 8 x 3 cm piece of fatty porcine tissue with the skin was compressed at room temperature of 25 °C with the MAMMOVISION compression paddle. An optical fiber (REM Series B) with a diffusing tip of diameter 1.7 mm was inserted in the tissue after making a

path with a stainless steel trocar (2.1 mm diameter). The laser was fired for 6 minutes at 10 W after the first image was taken and turned off for the remainder of the experiment.

After the initial stereo images were taken to ensure that the fiber was within view of the camera, we began the auto-firing sequence. The sequence was set to take images ever 30 seconds for the first 30 exposures, although the system actually took exposures every 32 seconds.

These images were then converted to 128 x 128 pixel images and each image was subtracted from the first image. These images were then colorized using MICROCAL ORIGIN to show changes around the fiber with time. Two color scales are compared: linear and logarithmic.

Results:

In FIGURES 17A-21B, the changes in the tissue surrounding the fiber are evident. The changes are more apparent in the logarithmic scale than in the linear scale. Movement of the fiber during the experiment cause the red and white regions at the original location of the fiber and the dark blue region at the actual location of the fiber.

Conclusion

From the stability analysis of the 128 x 128 pixel images of the calibration phantom, it can be assumed that intensity changes above 5% are assumed to be due either to thermal expansion or to tissue movement. These changes show that X-ray images can be utilized to monitor tissue changes during laser irradiation in accordance with this invention..

Although the images presented here are in a logarithmic scale to highlight the changes around the fiber, the scale will not amplify the temperature range of most interest to hyperthermia when the intensity changes

are correlated with temperature (*see*, FIGURES 16A, 16B and 16C). The temperature range that needs to be monitored most closely in this embodiment of the invention is between 55 and 65 °C, which is expected to be in the middle or higher (red) end of the range of intensity changes. Temperatures
5 above 65°C do not need to be monitored by temperature. In order to amplify the correct temperature range, a more suitable transfer function may be developed to be converted to a color scale (*see*, FIGURES 16A-21B).

Note:

The minimum pixel intensity is zero and corresponds to total
10 attenuation (i.e., no X-ray photons reaching the camera) and a white image. The maximum pixel intensity is 4095 and corresponds to no attenuation (i.e., all X-ray photons reaching the camera) and a black image. After the images are subtracted, the maximum possible intensity range is from -4095 to 4095. Each pixel corresponds to an area of approximately 50 x 50 µm in the 1024 x
15 1024 pixel images and to approximately 0.4 x 0.4 mm in the 128 x 128 pixel images.

STABILITY TEST OF MAMMOVISION EXPOSURES OF PORCINE TISSUE

This subsection presents an analysis of a stability test of the
20 MAMMOVISION System (85200G-2, Fischer Imaging Co., Denver, CO) exposures on fatty porcine tissue during the auto-firing sequence in accordance with this invention.

The Experimental Method:

An approximately 20 x 8 x 3 cm piece of fatty porcine tissue with the
25 skin was compressed at room temperature 20°C with the MAMMOVISION compression paddle. The initial scout was taken in the Autoexposure mode and its parameters were used in the sequential firing. The generator was set

manually at 25 kV, 50 mAs, and 100 mA for the following images in the sequential firing. The auto-firing sequence was set to take exposures every 30 seconds for approximately 15 minutes (after the initial scout and stereo images were taken).

- 5 The images obtained from this sequence were converted from 1024 x 1024 pixel images into 128 x 128 pixel images by averaging 8 x 8 pixel blocks into one pixel, by using a Turbo C program. These images were then analyzed by another Turbo C program to find pixels that changed in intensity by more than 2%.

10 **Results:**

- In the 32 128 x 128 pixel images, only 3 pixels showed variation of greater than 2% (*see*, Table 7). The maximum variation was 8.8%. All three pixels increased by more than 2% in one image and then returned to approximately the original value in the following image. These results
- 15 indicate that any image changes of more than 5% in the 128 x 128 images will be significant (above noise level).

Table 7: Coordinates and image number of pixels with over 2% intensity change in the 128 x 128 images

X-coordinate	Y-coordinate	Image number	Percent change
111	90	6	8.79
111	90	7	-8.16
15	70	8	5.00
15	70	9	-4.95
107	18	24	4.11

X-coordinate	Y-coordinate	Image number	Percent change
107	18	25	-3.98

Conclusion:

This analysis corroborates the earlier findings that the 128 x 128 pixel images are stable, although those findings indicated that there were no changes above 5% while the results from this analysis indicate that one pixel changed above 5%. This discrepancy may be explained by the relatively low generator mAs value (50 mAs) in this experiment compared to that of the previous experiment (280 mAs), since increasing the mAs value increases contrast. Changes above 5% can be assumed to be due either to thermal expansion or to tissue movement.

Note:

The minimum pixel intensity is zero and corresponds to total attenuation (i.e., no X-ray photons reaching the camera) and a white image. The maximum pixel intensity is 4095 and corresponds to no attenuation (i.e., all X-ray photons reaching the camera) and a black image. Each pixel corresponds to an area of approximately 50 x 50 μm in the 1024 x 1024 pixel images and to approximately 0.4 x 0.4 mm in the 128 x 128 pixel images.

Although only the presently preferred embodiments have been described in detail above, people with ordinary skill in the art will readily appreciate from the teachings herein that many modifications are possible in the exemplary embodiments without materially departing from the novel teachings and advantages of this invention.

WE CLAIM:

1. A method of thermally inducing and monitoring changes to localized regions of tissue, comprising:

illuminating a volume of tissue with a first beam of X-rays at a first time;

detecting a plurality of portions of said first beam of X-rays that passed through said volume of tissue during said illuminating with said first beam of X-rays;

generating a first X-ray image signal from said plurality of portions of X-rays of said first beam detected;

applying heat to at least a localized region of tissue within said volume of tissue after said illuminating and after said detecting;

illuminating said volume of tissue with a second beam of X-rays at a second time;

detecting a plurality of portions of said second beam of X-rays that passed through said volume of tissue during said illuminating with said second beam of X-rays;

generating a second X-ray image signal from said plurality of portions of X-rays of said second beam detected; and

generating a resultant image signal based upon a comparison of said first and second X-ray image signals,

wherein said resultant image signal contains information of changes in X-ray attenuation by localized regions of tissue within said volume of tissue due to said application of heat.

2. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1,

wherein said generating first and second X-ray image signals generates digital X-ray image signals corresponding to respective digital X-ray images, each digital X-ray image comprising a plurality of image pixels, and

said generating a resultant signal performs a pixel-by-pixel subtraction of corresponding pixel values to produce a difference image signal, said pixel values corresponding to respective X-ray intensities detected.

3. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, further comprising:

storing said first X-ray image signal prior to illuminating said volume of tissue with said second beam of X-rays at said second time; and

retrieving said first X-ray image signal from storage for use in said generating said difference image signal based upon said comparison of said first and second X-ray image signals.

4. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, further comprising:

rendering a visual image of said difference image signal generated; and

altering the application of heat in response to said rendered visual image.

5. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 4, further comprising determining a size of one of said localized regions of tissue within said volume of tissue based on said visual image of said difference image signal rendered, wherein said one of said localized regions of tissue corresponds to cancerous tissue.

6. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 5, further comprising determining a termination of thermotherapy based on said size of said one of said localized regions of tissue determined.

7. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, further comprising:

illuminating said volume of tissue with a third beam of X-rays at a third time;

detecting a plurality of portions of said third beam of X-rays that have passed through said volume of tissue;

generating a third X-ray image signal from said plurality of portions of X-rays of said third beam detected; and

generating a second resultant image signal based upon a comparison of said first and third X-ray image signals,

wherein said first X-ray image signal provides a static reference signal for generating successive resultant image signals after successive illuminating, detecting and generating X-ray image signals.

8. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, further comprising:

illuminating said volume of tissue with a third beam of X-rays at a third time;

detecting a plurality of portions of said third beam of X-rays that passed through said volume of tissue;

generating a third X-ray image signal from said plurality of portions of X-rays of said third beam detected; and

generating a second resultant image signal based upon a comparison of said second and third X-ray image signals,

wherein said second X-ray image signal provides a dynamically updated reference signal.

9. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, wherein said applying heat to said at least a localized region of tissue within said volume of tissue comprises irradiating said localized region of tissue with a laser.

10. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, wherein said applying heat to said at least a localized region of tissue within said volume of tissue comprises irradiating said localized region of tissue with a microwave energy source.

11. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, wherein said applying heat to at least a localized region of tissue within said volume of tissue comprises irradiating said localized region of tissue with a radio-frequency energy source.

12. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, wherein said applying heat to at least a localized region of tissue within said volume of tissue comprises heating said localized region of tissue with an ultrasound energy source.

13. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 1, wherein said volume of tissue is a woman's breast and said localized region of tissue includes cancerous tissue.

14. A method of thermally inducing and monitoring changes to localized regions of tissue, comprising:

illuminating a volume of tissue with a first pair of X-ray beams during a first period of time, each X-ray beam of said first pair of X-ray beams being incident upon said volume of tissue from angles that are different from each other;

detecting a plurality of portions of each X-ray beam of said first pair of X-ray beams that passed through said volume of tissue during said illuminating with said first pair of X-ray beams;

generating a first three-dimensional X-ray image signal from said plurality of portions of each X-ray beam of said first pair of X-ray beams detected;

applying heat to at least a localized region of tissue within said volume of tissue after said illuminating and after said detecting;

illuminating a volume of tissue with a second pair of X-ray beams during a second period of time, each X-ray beam of said second pair of X-ray beams being incident upon said volume of tissue from angles that are different from each other;

detecting a plurality of portions of each X-ray beam of said second pair of X-ray beams that passed through said volume of tissue during said illuminating with said second pair of X-ray beams;

generating a second three-dimensional X-ray image signal from said plurality of portions of each X-ray beam of said second pair of X-ray beams detected; and

generating a three-dimensional resultant image signal based upon a comparison of said first and second X-ray image signals,

wherein said three-dimensional resultant image signal contains information of changes to localized regions of tissue within said volume of tissue due to said application of heat.

15. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14,

wherein said generating first and second three-dimensional X-ray image signals generates digital X-ray image signals corresponding to

respective three-dimensional digital X-ray images, each three-dimensional digital X-ray image comprising a plurality of image pixels, and

said generating a resultant image signal performs a pixel-by-pixel subtraction of corresponding pixel values to produce a difference image signal, said pixel values corresponding to respective X-ray intensities detected.

16. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, further comprising:

storing said first three-dimensional X-ray image signal prior to illuminating said volume of tissue with said second pair of X-ray beams at said second period of time; and

retrieving said first three-dimensional X-ray image signal from storage for use in said generating said resultant image signal based upon said comparison of said first and second three-dimensional X-ray image signals.

17. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, further comprising:

rendering a visual image of said three-dimensional resultant image signal generated; and

altering the application of heat in response to said rendered visual image.

18. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 17, further comprising

determining a size of one of said localized regions of tissue within said volume of tissue based on said visual image of said three-dimensional resultant image signal rendered, wherein said one of said localized regions of tissue corresponds to cancerous tissue.

19. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 18, further comprising determining a termination of thermotherapy based on said size of said one of said localized regions of tissue determined.

20. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, further comprising:

illuminating said volume of tissue with a third pair of X-ray beams during a third period of time, each X-ray beam of said third pair of X-ray beams being incident upon said volume of tissue from angles that are different from each other;

detecting a plurality of portions of each X-ray beam of said third pair of X-ray beams that passed through said volume of tissue during said illuminating with said third pair of X-ray beams;

generating a third three-dimensional X-ray image signal from said plurality of portions of each X-ray beam of said third pair of X-ray beams detected; and

generating a second resultant image signal based upon a comparison of said first and third three-dimensional X-ray image signals,

wherein said first three-dimensional X-ray image signal provides a static reference signal for generating successive resultant image signals after successive illuminating, detecting and generating X-ray image signals.

21. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, further comprising:

illuminating said volume of tissue with a third pair of X-ray beams during a third period of time, each X-ray beam of said third pair of X-ray beams being incident upon said volume of tissue from angles that are different from each other;

detecting a plurality of portions of each X-ray beam of said third pair of X-ray beams that passed through said volume of tissue during said illuminating with said third pair of X-ray beams;

generating a third three-dimensional X-ray image signal from said plurality of portions of each X-ray beam of said third pair of X-ray beams detected; and

generating a second resultant image signal based upon a comparison of said second and third three-dimensional X-ray image signals,

wherein said second three-dimensional X-ray image signal provides a dynamically updated reference signal.

22. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, wherein said applying heat to said at least a localized region of tissue within said volume of tissue comprises irradiating said localized region of tissue with a laser.

23. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, wherein said applying heat to said at least a localized region of tissue within said volume of tissue comprises irradiating said localized region of tissue with a microwave energy source.

24. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, wherein said applying heat to said at least a localized region of tissue within said volume of tissue comprises irradiating said localized region of tissue with a radio-frequency energy source.

25. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, wherein said applying heat to said at least a localized region of tissue within said volume of tissue comprises heating said localized region of tissue with an ultrasound energy source.

26. A method of thermally inducing and monitoring changes to localized regions of tissue according to claim 14, wherein said volume of tissue is a woman's breast and said localized region of tissue includes cancerous tissue.

27. A method of destroying cancerous tissue, comprising:

forming a first X-ray image of a portion of a patient's body;

applying heat to a localized region of said portion of said patient's body, said localized region being selected based upon information from said first X-ray image;

forming a second X-ray image of said portion of said patient's body subsequent to applying heat to said localized region of said portion of said patient's body;

generating a resultant image based on a comparison of said first X-ray image to said second X-ray image at corresponding locations within said first and second images; and

modifying said application of heat based upon said resultant image generated.

28. A method of destroying cancerous tissue according to claim 27, wherein said applying heat is an application of interstitial laser hyperthermia.

29. A method of destroying cancerous tissue according to claim 28, wherein said first and second X-ray images are high resolution three-dimensional digital X-ray images and said modifying said application of heat includes changing a laser power of a laser probe disposed in said portion of said patient's body.

30. A method of destroying cancerous tissues according to claim 27, wherein said comparison is a subtraction of said first X-ray image data from said second X-ray image data to produce a difference image.

31. A device for monitoring thermally induced changes to localized regions of tissue, comprising:

an X-ray illumination source;

an X-ray detector disposed proximate said X-ray illumination source and reserving a space therebetween for accommodating tissue to be monitored, said X-ray detector producing a plurality of X-ray image data signals corresponding to a plurality of X-ray images, each said X-ray image being taken at a different time;

a data storage unit in communication with said X-ray detector, said data storage unit receiving and storing at least one of said plurality of X-ray image signals produced by said X-ray detector;

an image comparison unit in communication with at least said data storage unit out of said data storage unit and said X-ray detector, said image comparison unit comparing said at least one X-ray image signal to a second X-ray image signal of said plurality of X-ray signals at corresponding X-ray image locations and producing a resultant X-ray image signal; and

an image display unit in communication with said image comparison unit, said image display unit displaying the resultant X-ray image that provides information corresponding to said thermally-induced changes to said localized regions of said tissue.

32. A device for monitoring thermally induced changes to localized regions of tissue according to claim 31, wherein said image comparison unit subtracts said at least one X-ray image signal retrieved from said data storage unit from said second X-ray image signal of said plurality of X-ray signals at corresponding X-ray image locations.

33. A device for monitoring thermally-induced changes to localized regions of tissue according to claim 32, wherein said plurality of X-ray image data signals produced by said X-ray detector are digital signals.

34. A device for monitoring thermally-induced changes to localized regions of tissue according to claim 33, wherein said image comparison unit is a programmable computer programmed to perform said subtraction for each pair of corresponding pixels.

35. A device for causing thermally-induced changes to localized regions of tissue, comprising:

an X-ray illumination source;

an X-ray detector disposed proximate said X-ray illumination source and reserving a space therebetween for accommodating tissue to be monitored, said X-ray detector producing a plurality of X-ray image data signals corresponding to a plurality of X-ray images, each said X-ray image being taken at a different time;

a data storage unit in communication with said X-ray detector, said data storage unit receiving and storing at least one of said plurality of X-ray image signals produced by said X-ray detector;

a thermotherapy heating assembly disposed proximate said space reserved between said X-ray illumination source and said X-ray detector; and

an image comparison unit in communication with at least said data storage unit out of said data storage unit and said X-ray detector, said image

comparison unit comparing said at least one X-ray image signal after being retrieved from said data storage unit to a second X-ray image signal of said plurality of X-ray signals at corresponding X-ray image locations and producing a resultant X-ray image signal; and

an image display unit in communication with said image comparison unit, said image display unit displaying a resultant X-ray image that provides information corresponding to said thermally-induced changes to said localized regions of said tissue.

36. A device for causing thermally-induced changes to localized regions of tissue according to claim 35, wherein said image comparison unit subtracts said at least one X-ray image signal retrieved from said data storage unit from said second X-ray image signal of said plurality of X-ray signals at corresponding X-ray image locations to produce a difference X-ray image signal.

37. A device for causing thermally-induced changes to localized regions of tissue according to claim 36, wherein said plurality of X-ray image data signals produced by said X-ray detector are digital signals.

38. A device for causing thermally-induced changes to localized regions of tissue according to claim 37, wherein said image comparison unit is a programmable computer programmed to perform said subtraction for each pair of corresponding pixels.

39. A device for causing thermally-induced changes to localized regions of tissue according to claim 35, wherein said thermotherapy heating assembly comprises a laser.

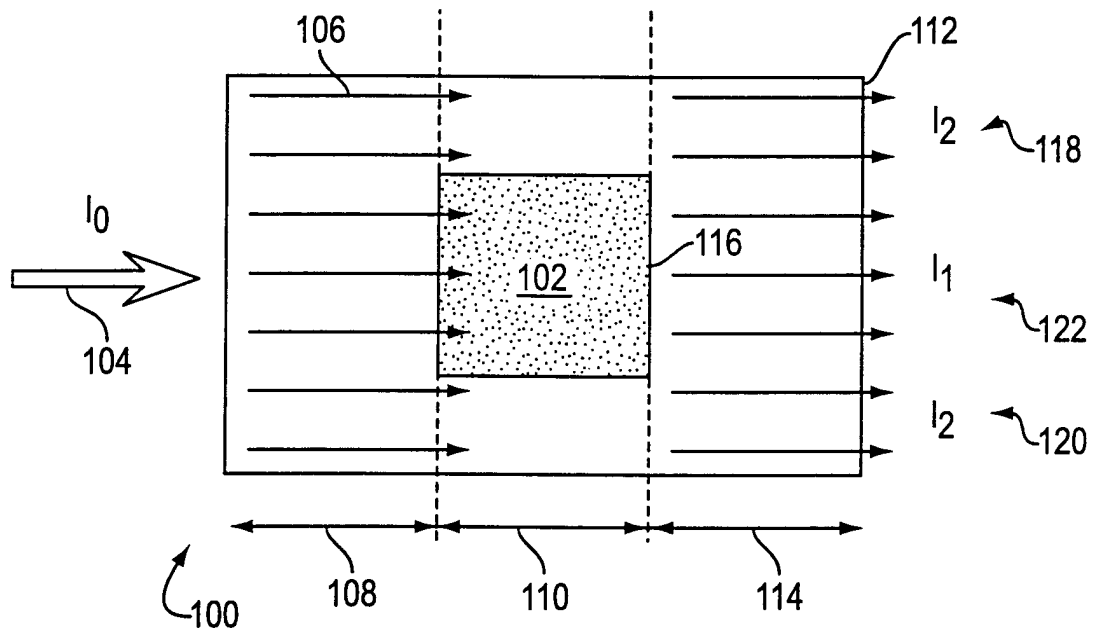


FIG. 1

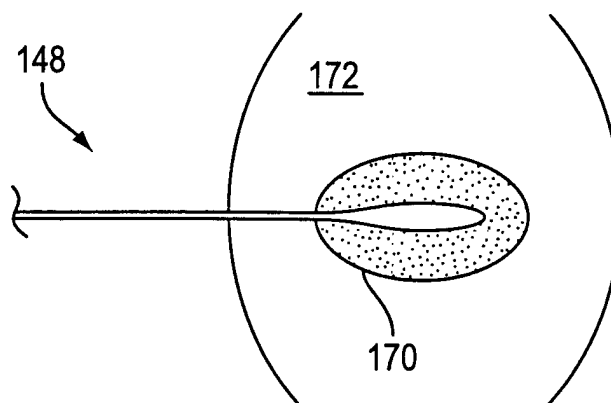


FIG. 4

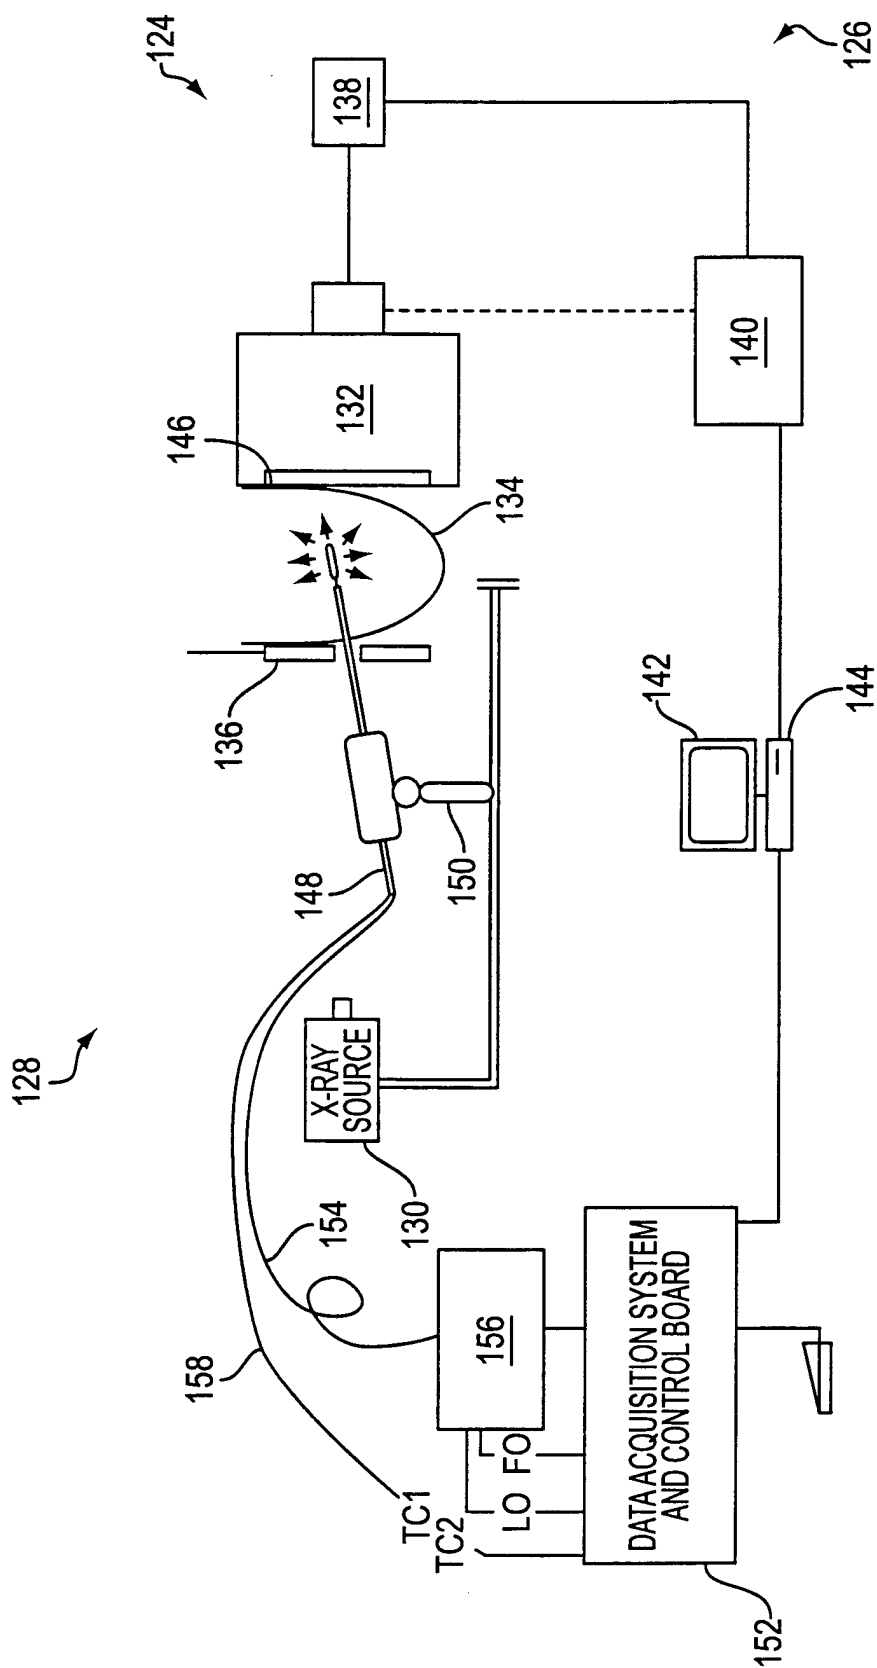


FIG. 2

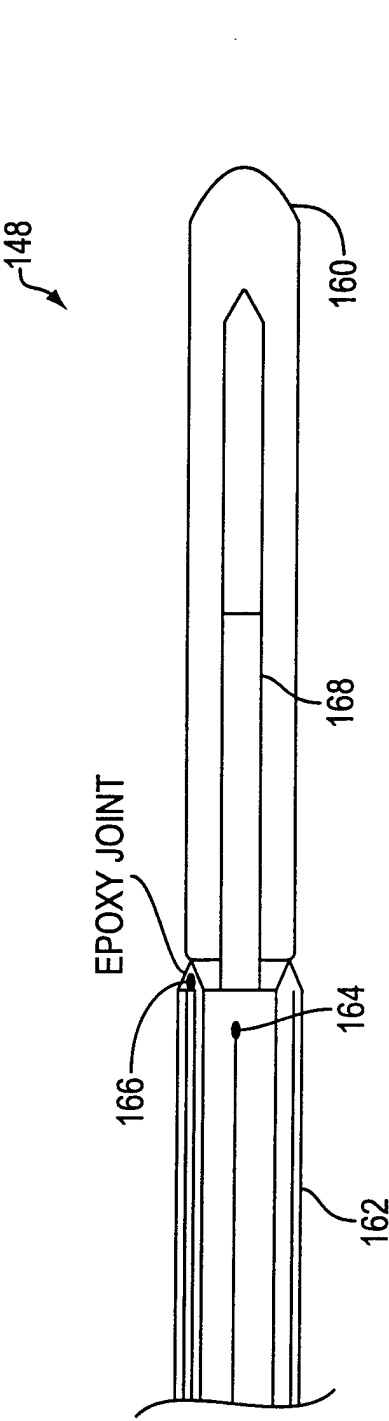


FIG. 3A

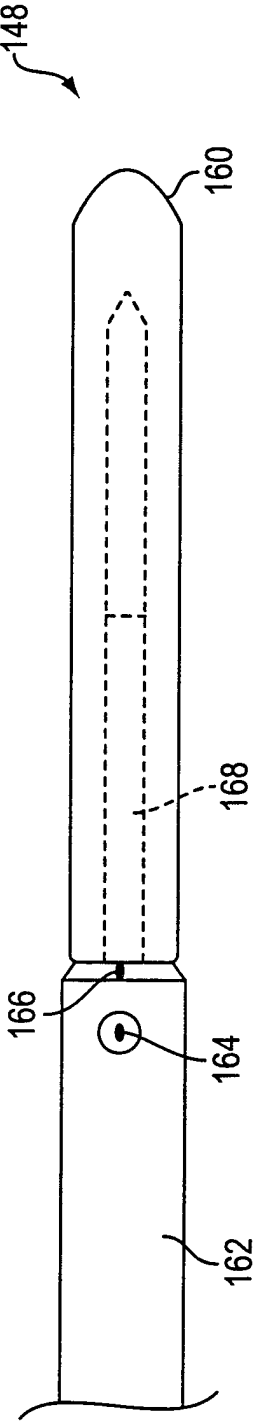


FIG. 3B

4/31

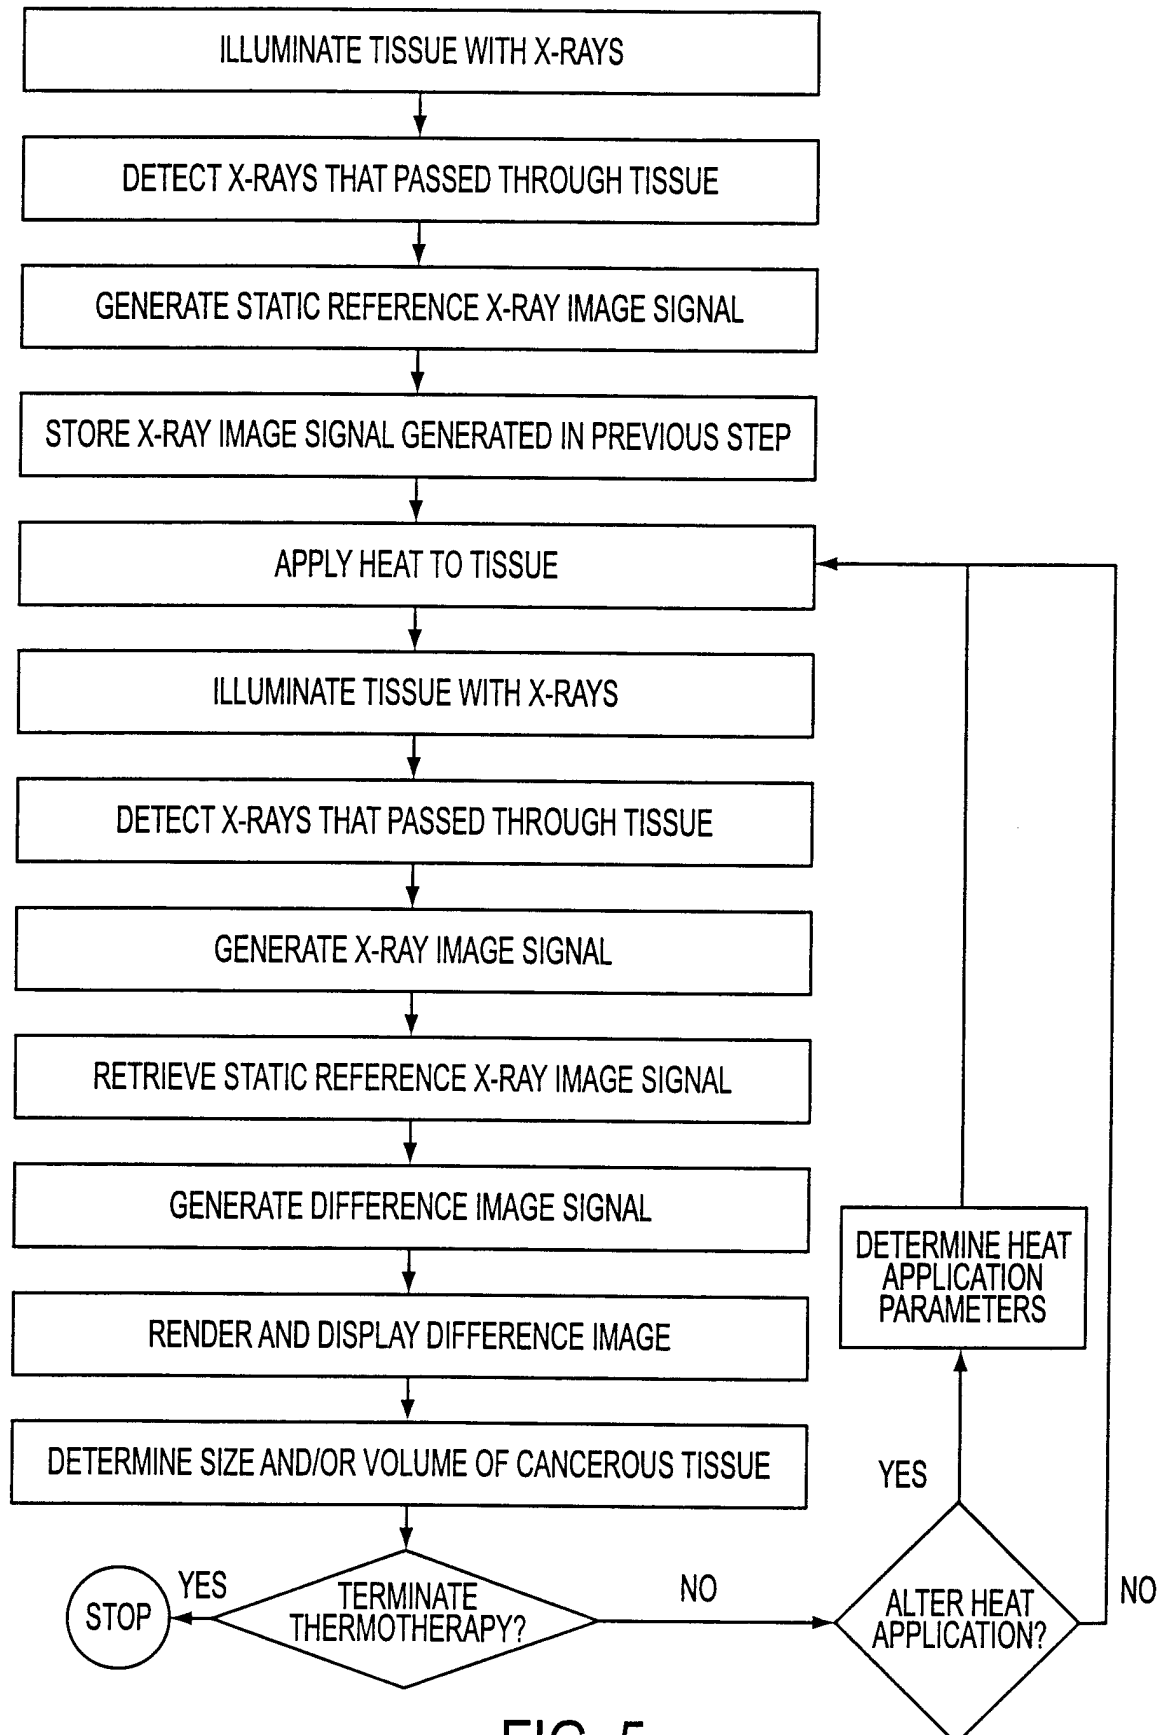


FIG. 5

5/31

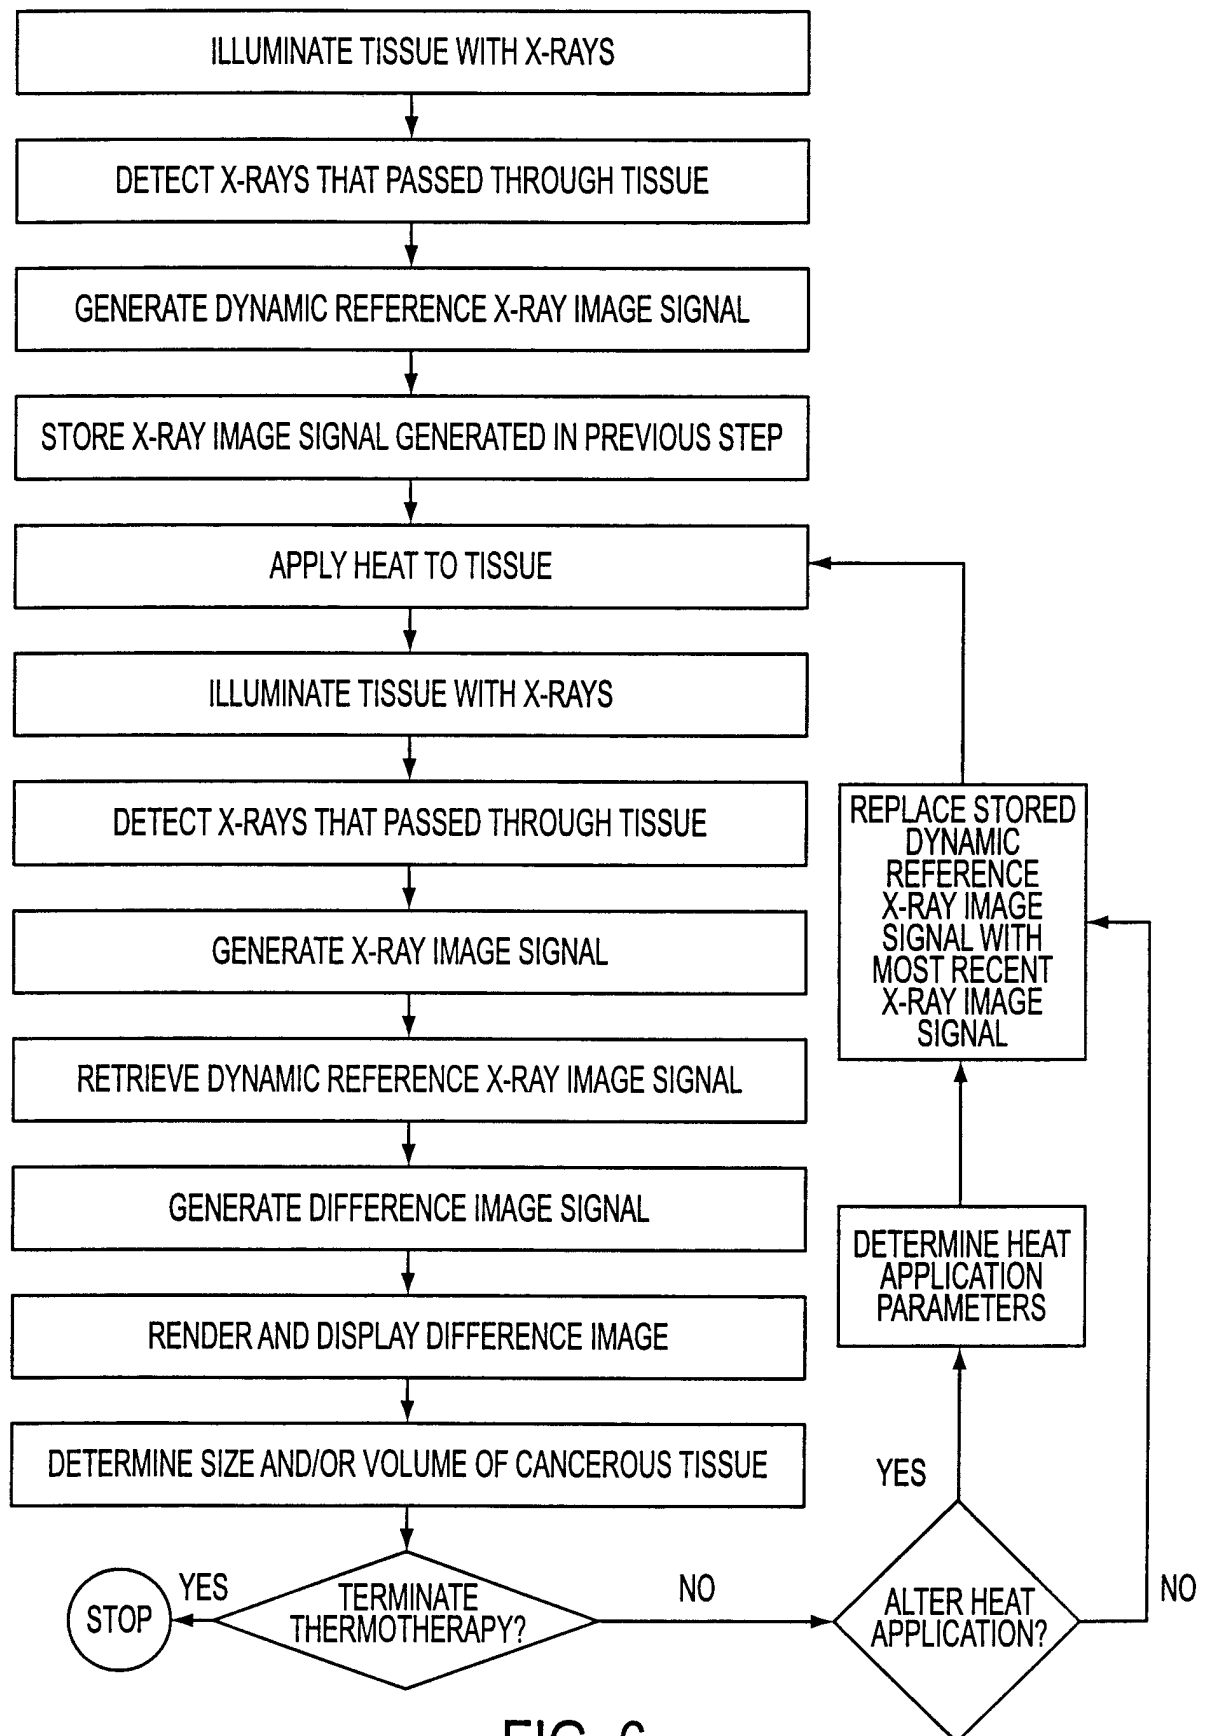


FIG. 6

6/31

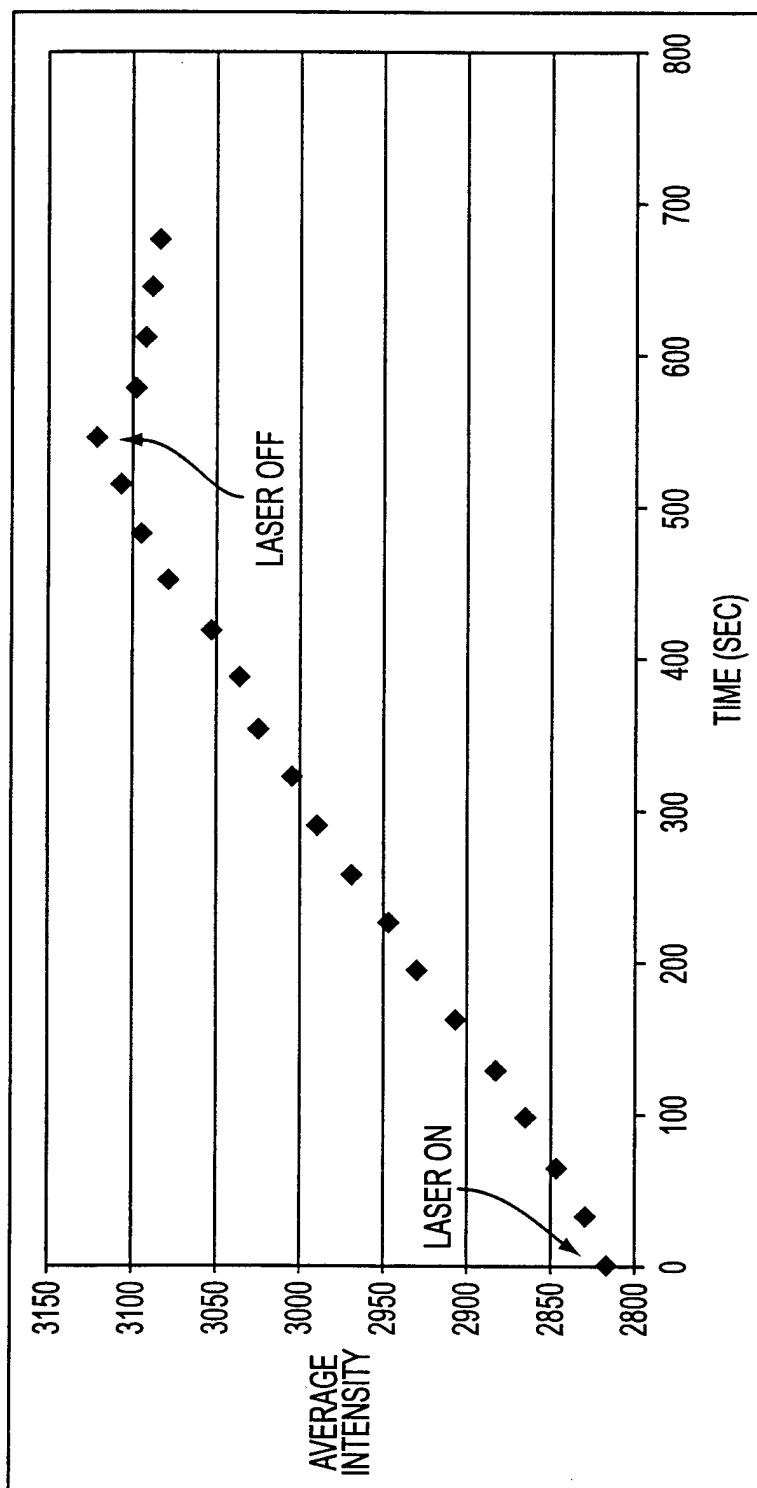


FIG. 7

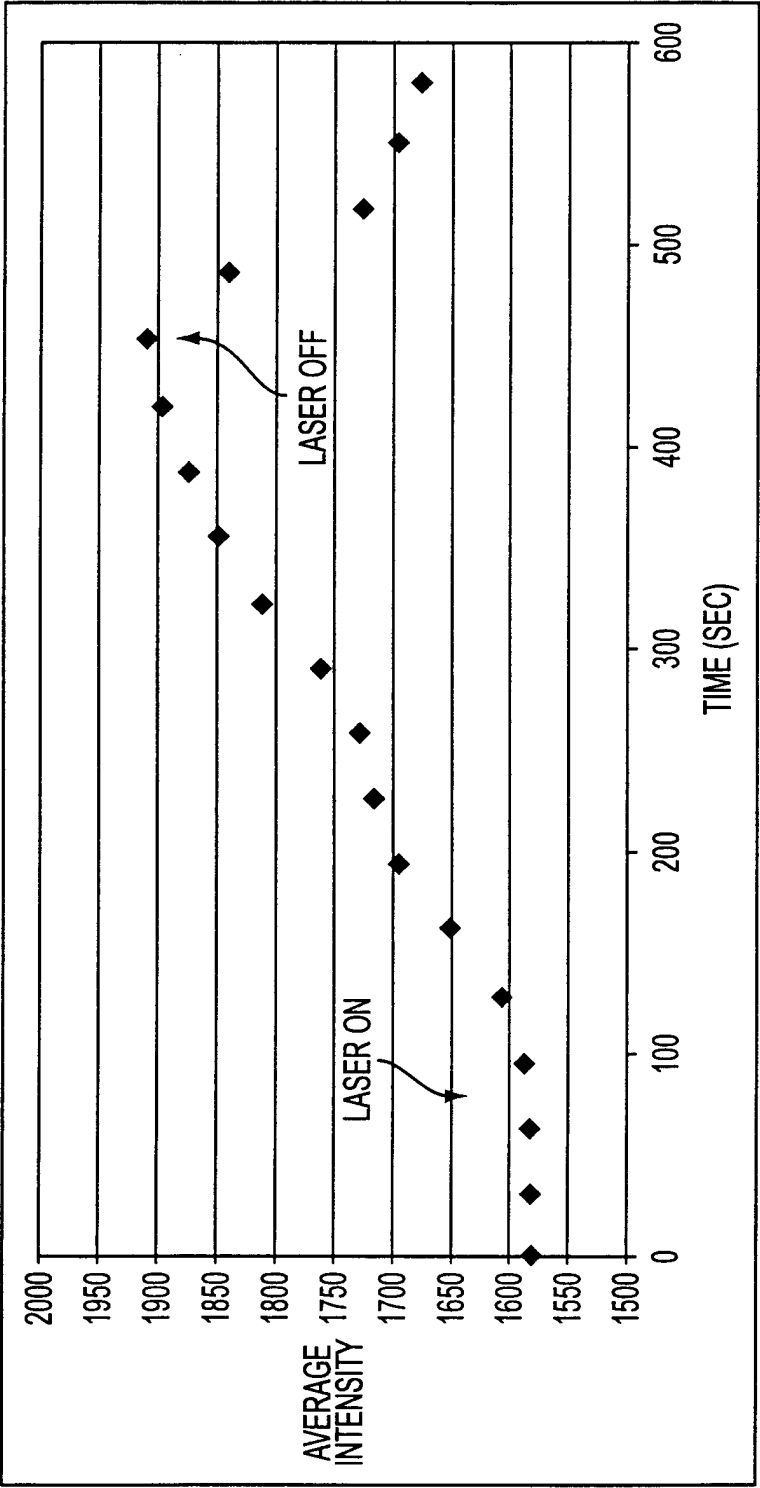


FIG. 8

8/31

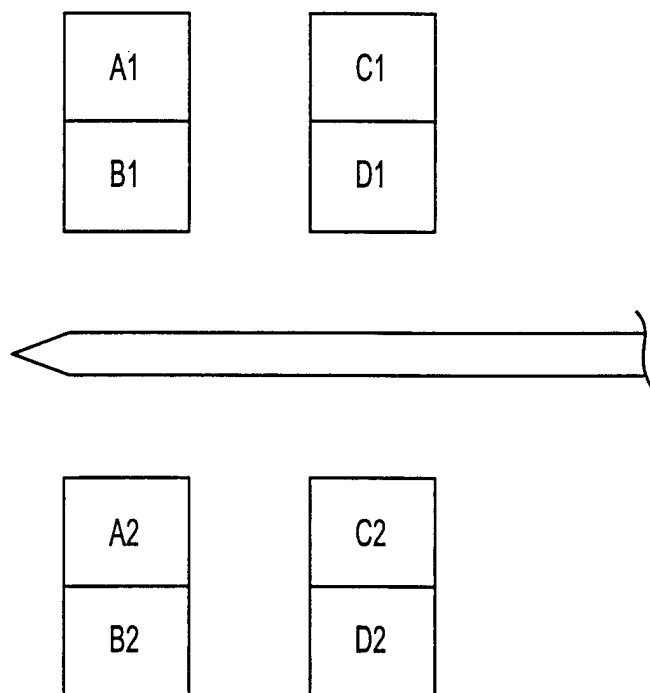


FIG. 9

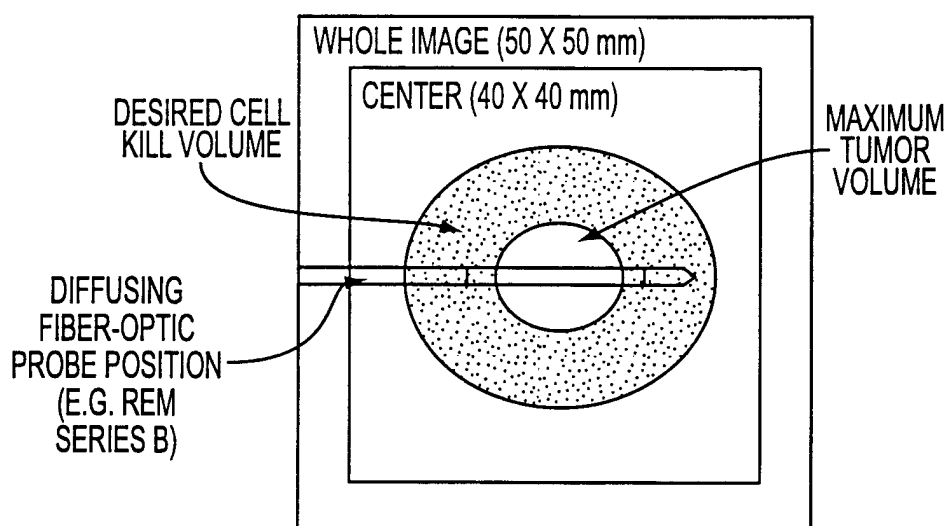


FIG. 11

9/31

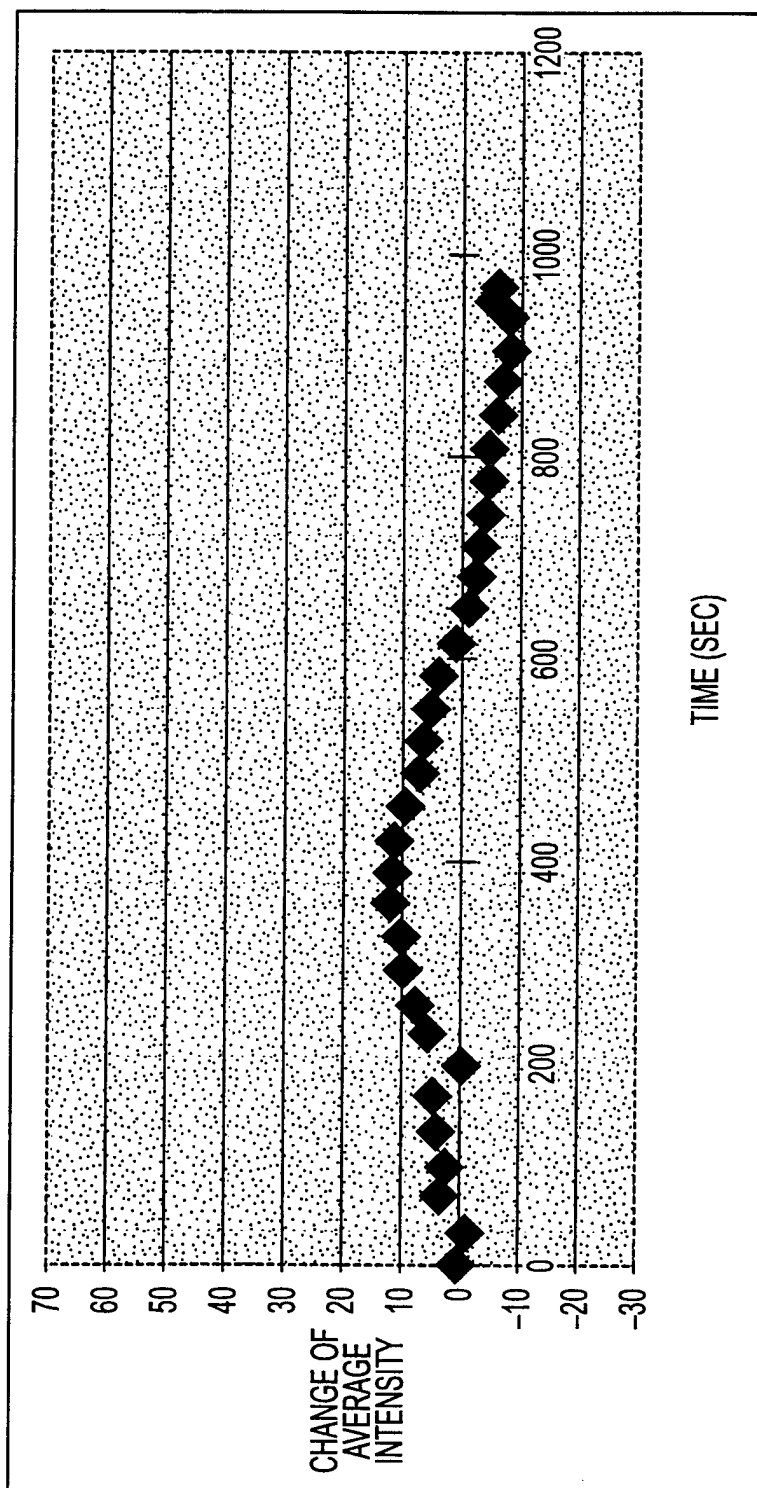


FIG. 10A

10/31

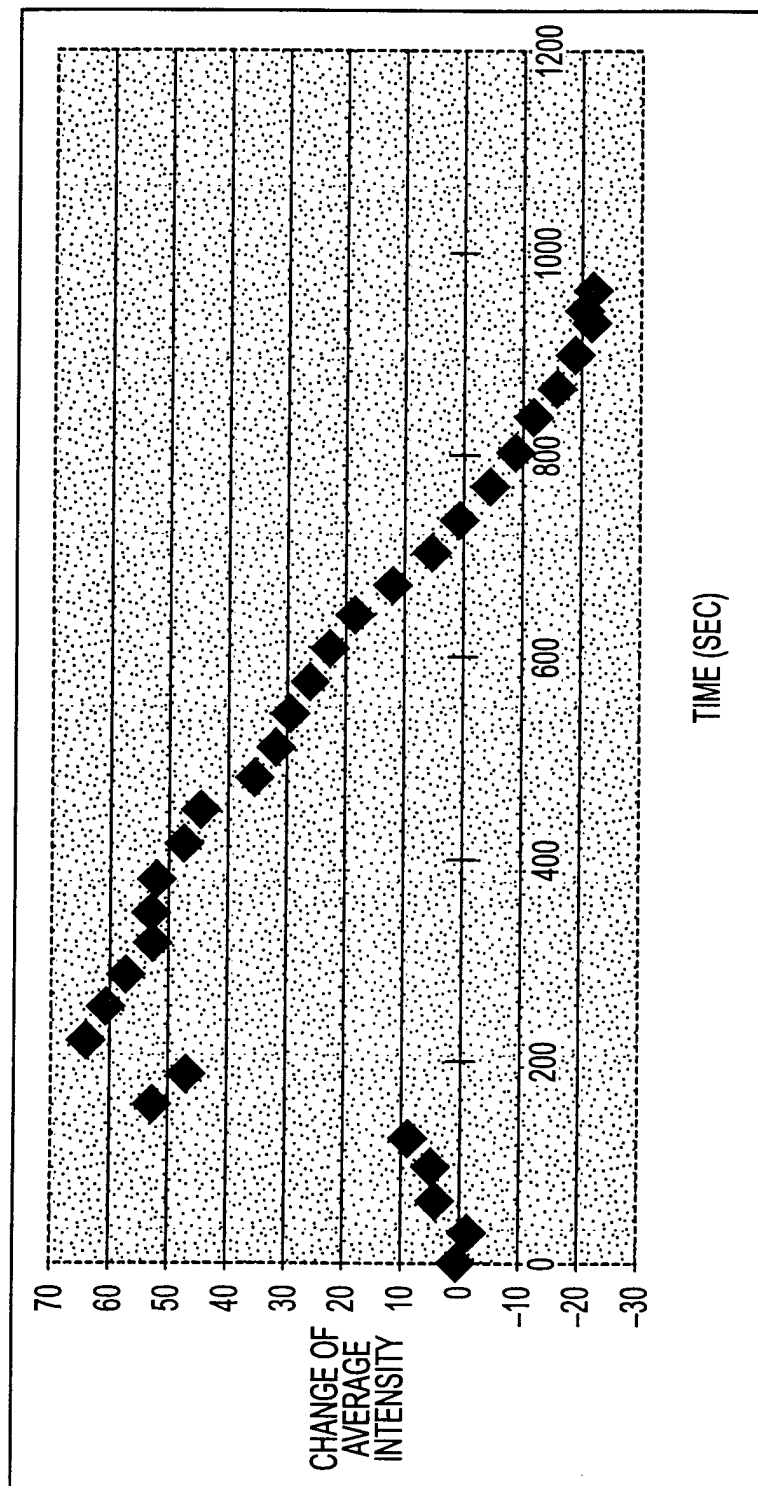


FIG. 10B

11/31

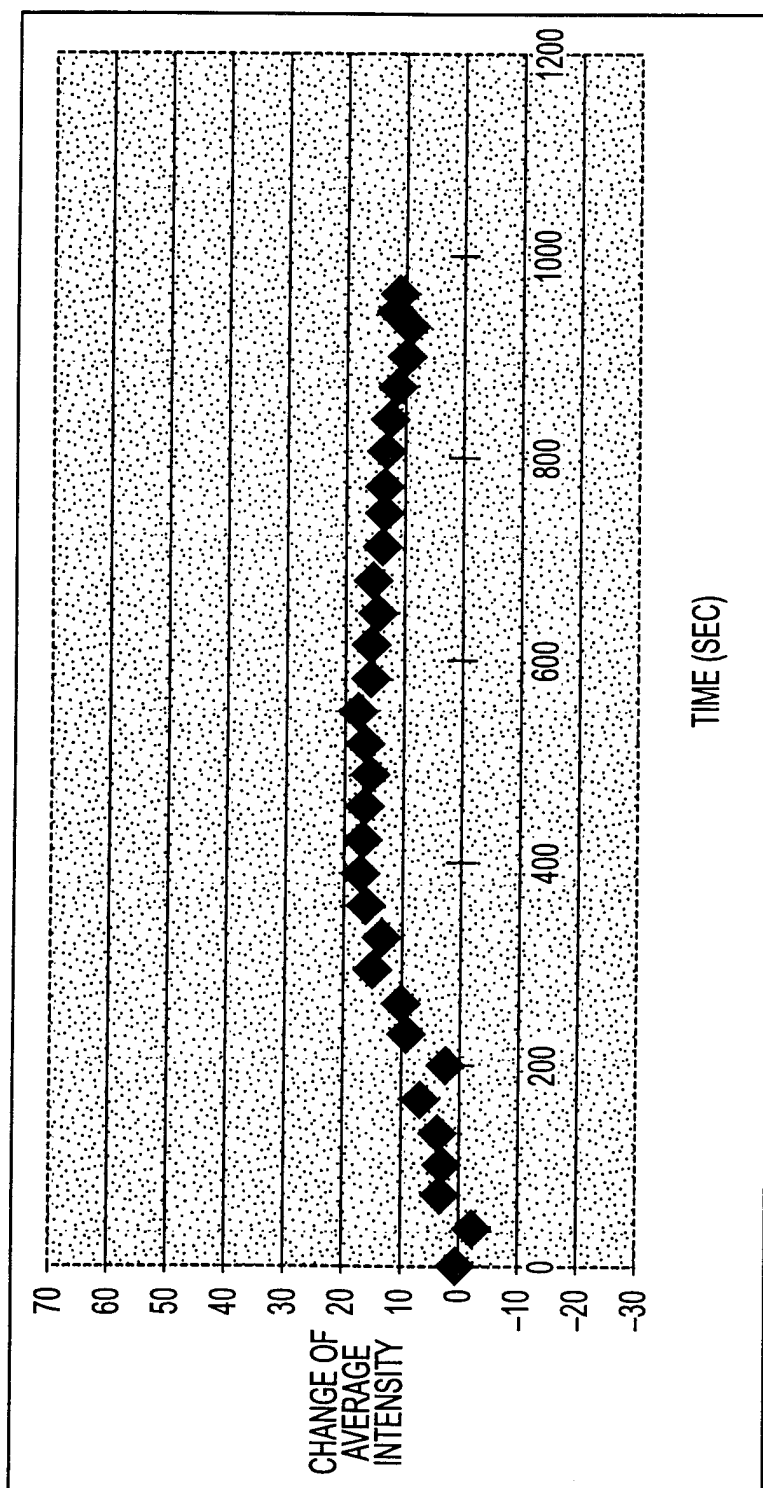


FIG. 10C

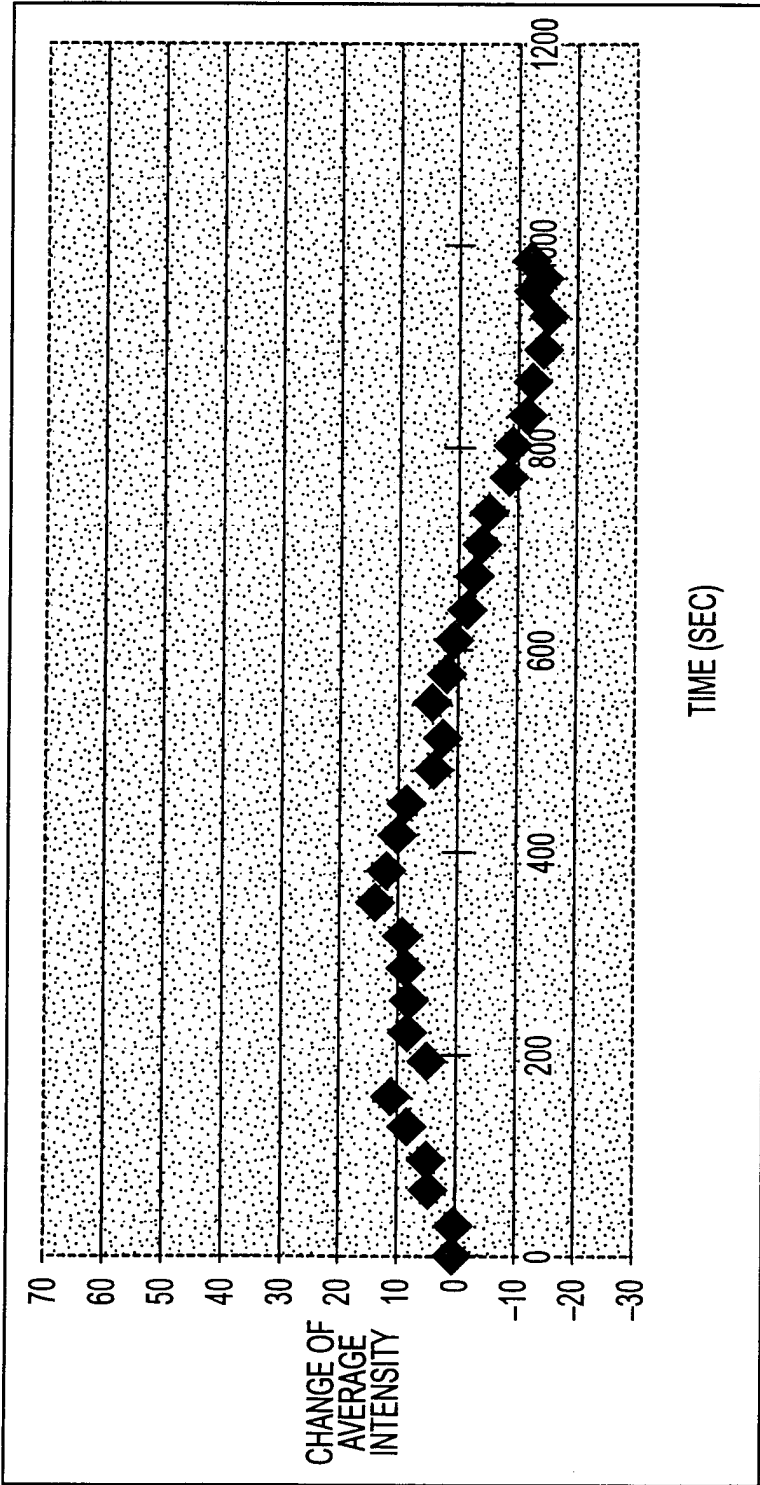


FIG. 10D

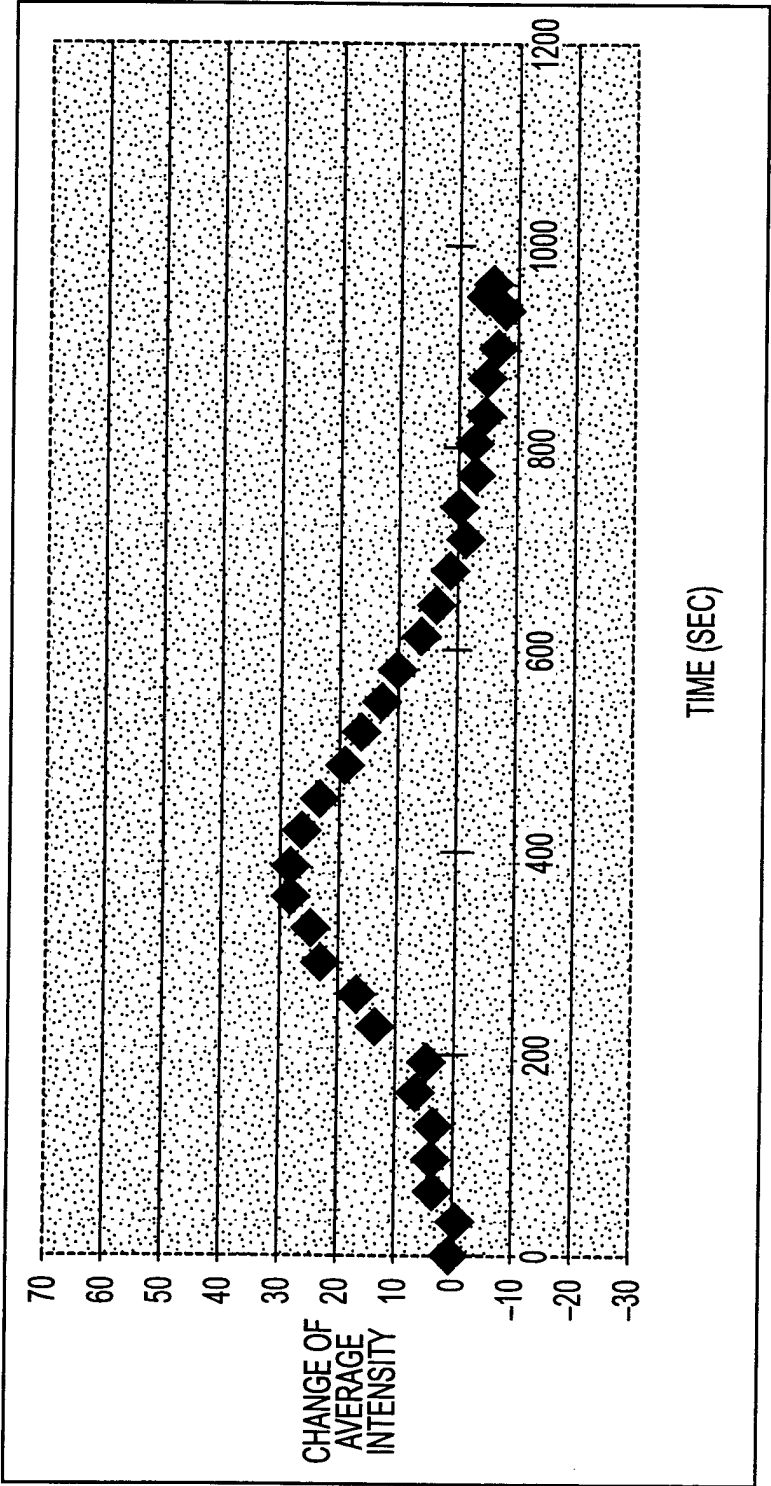


FIG. 10E

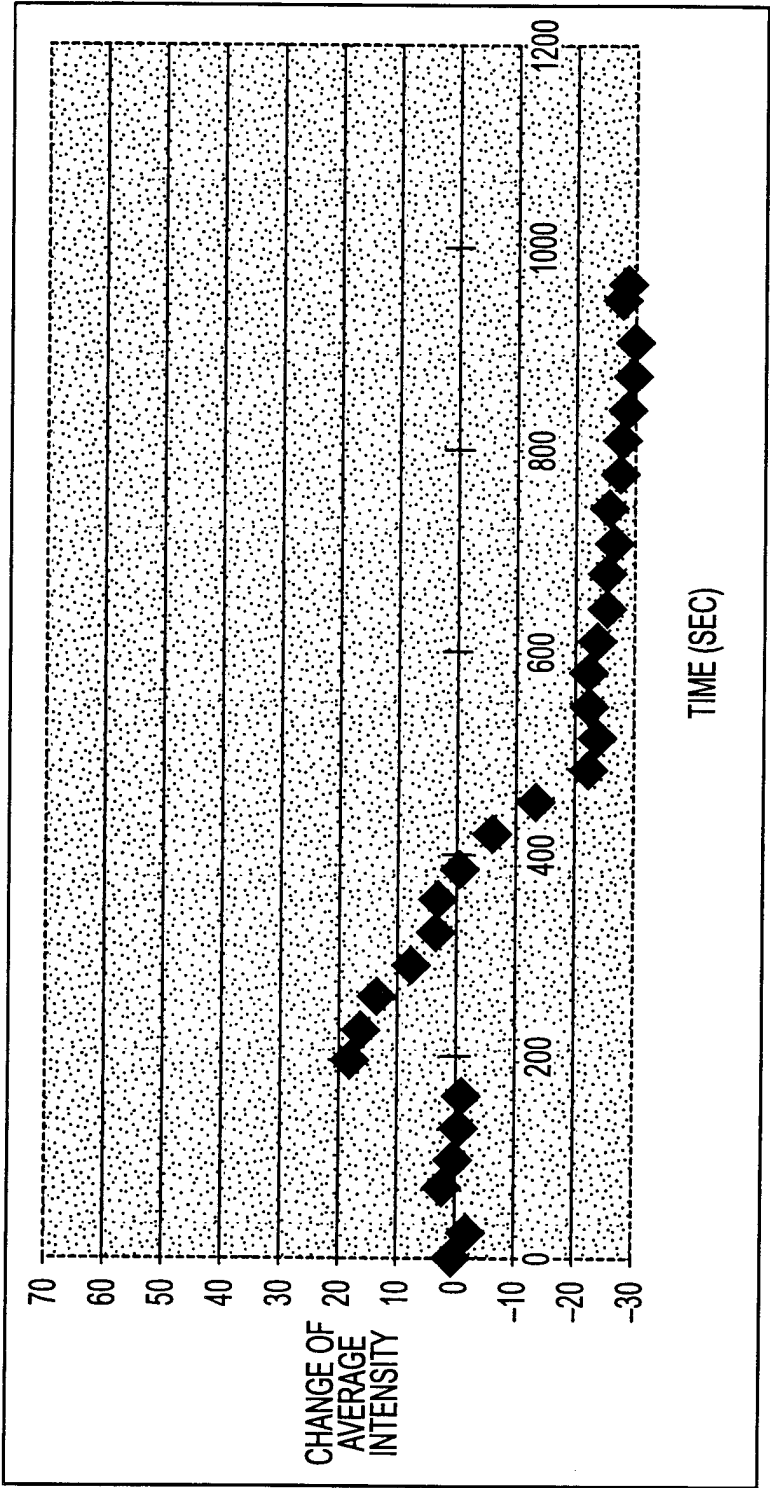


FIG. 10F

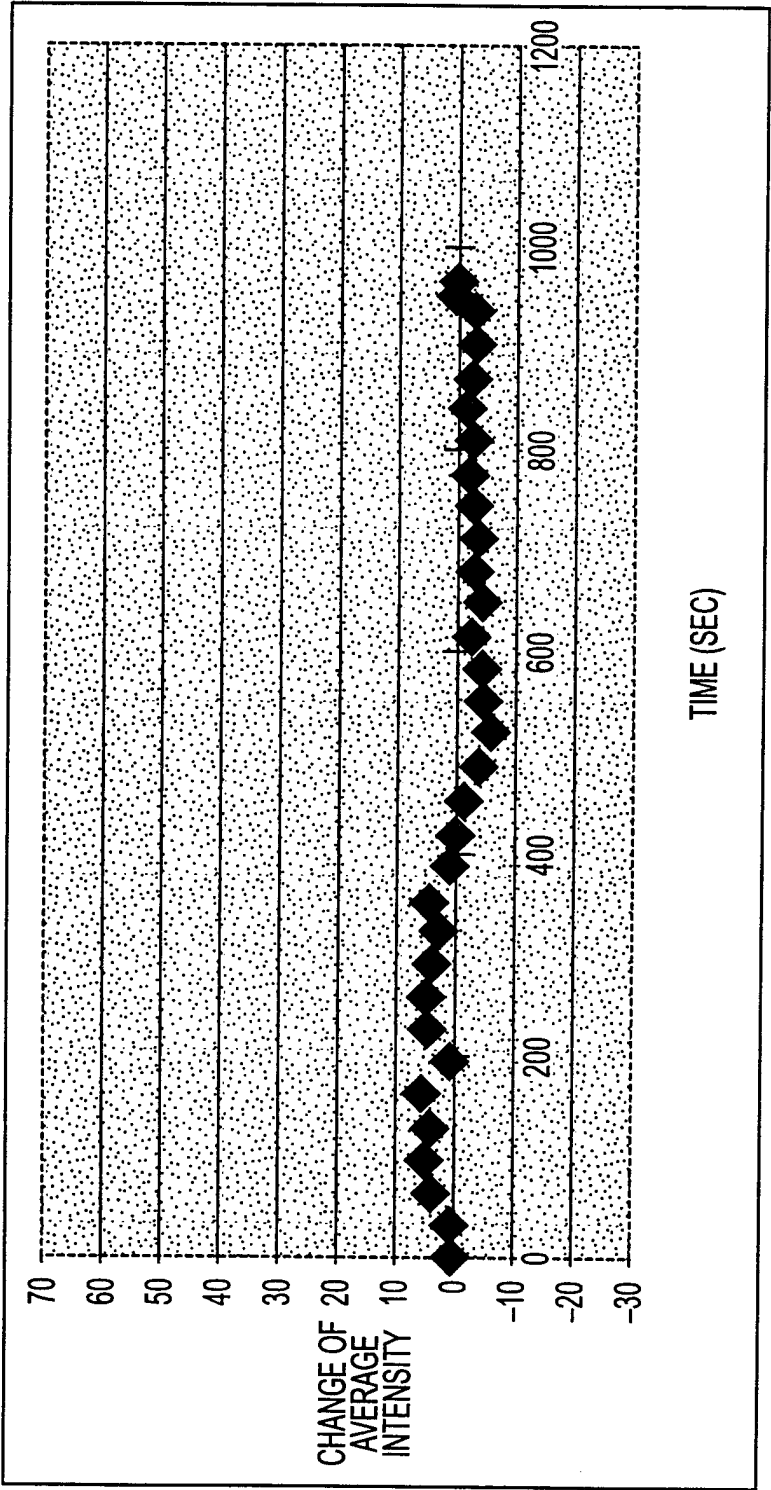


FIG. 10G

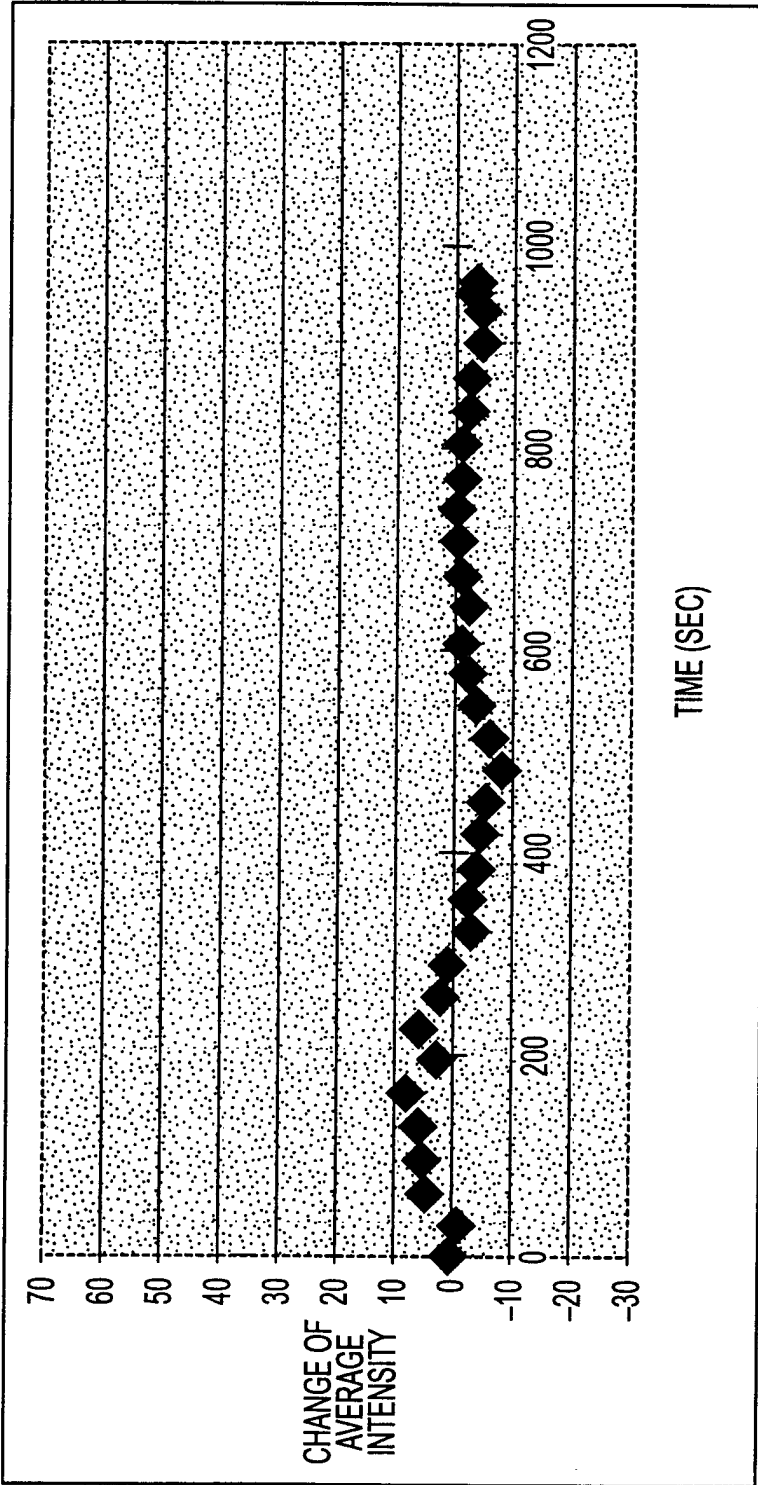


FIG. 10H

17/31

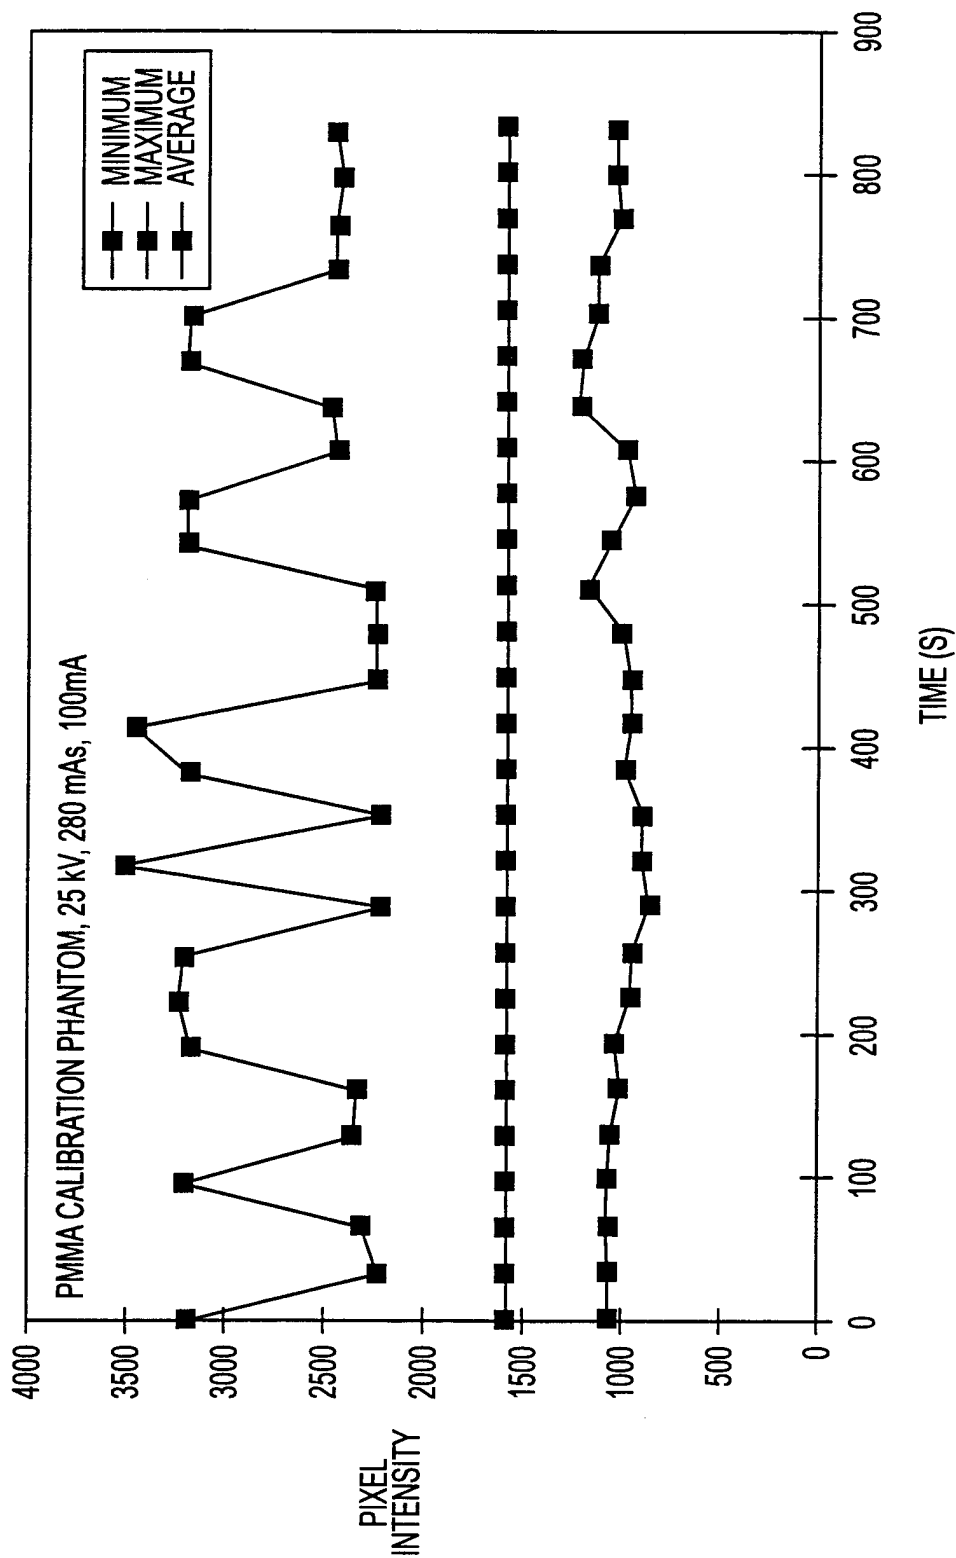


FIG. 12

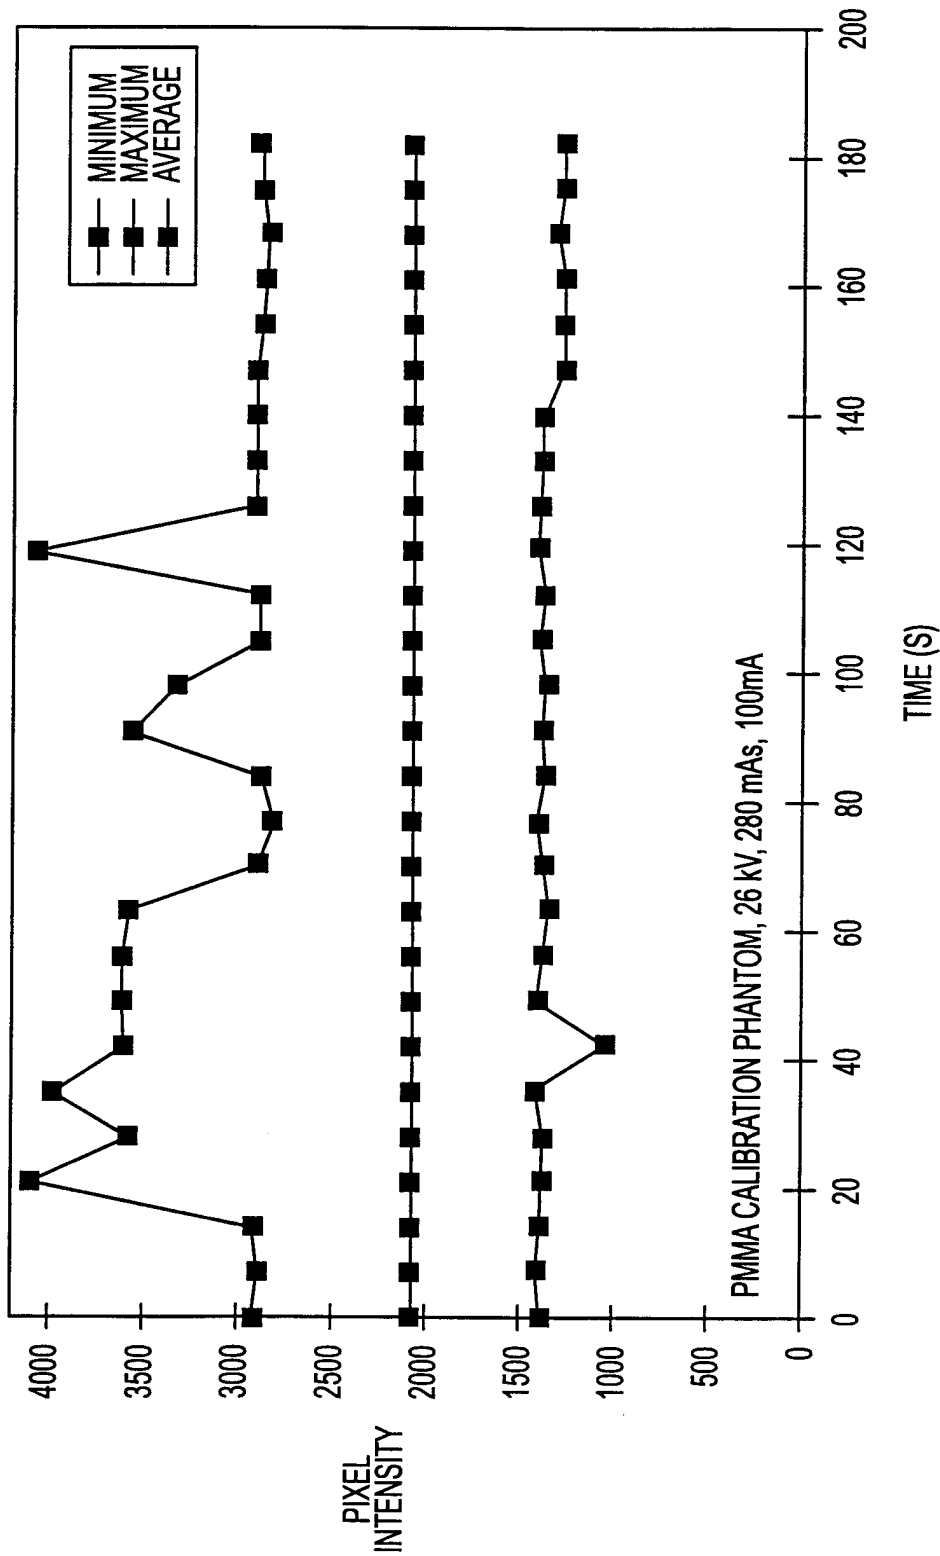


FIG. 13

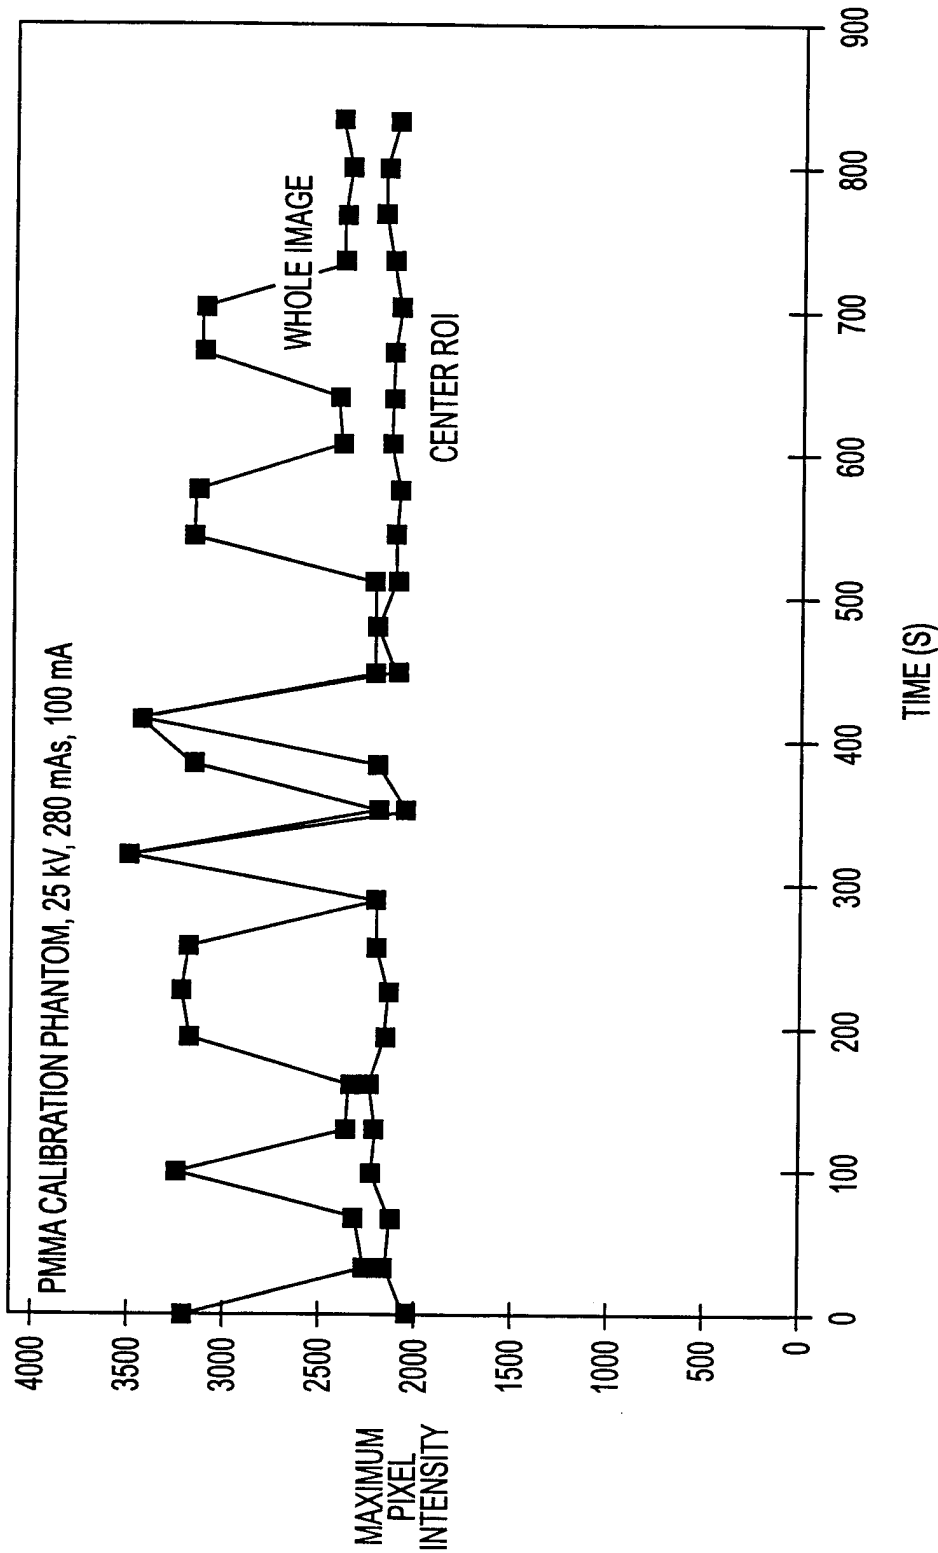


FIG. 14

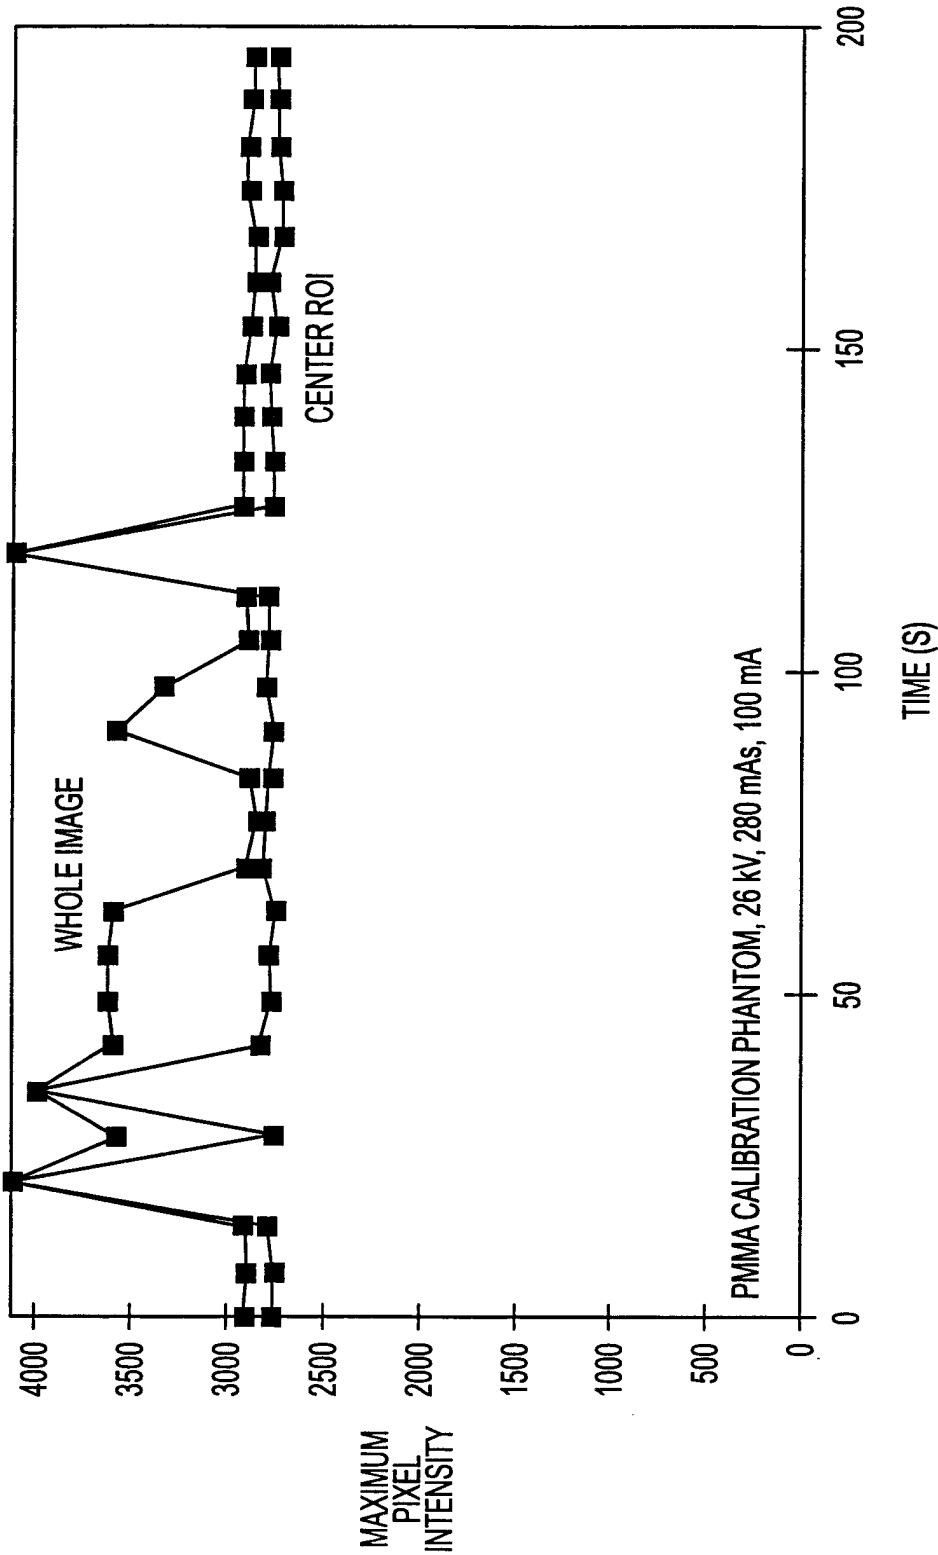


FIG. 15

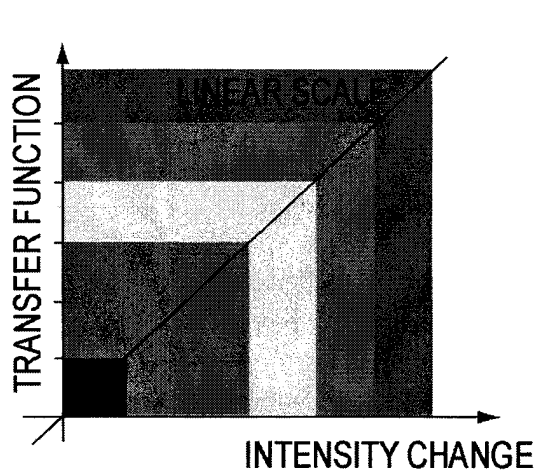


FIG. 16A

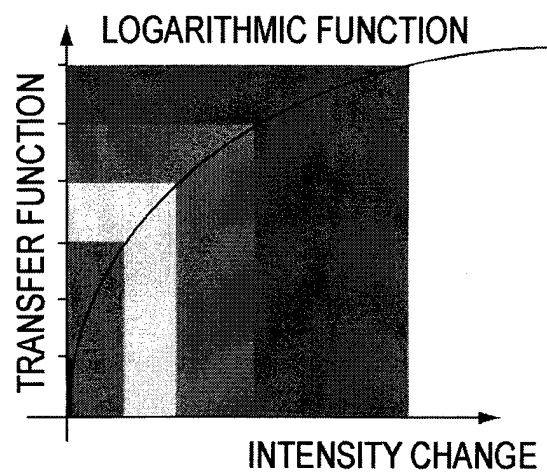


FIG. 16B


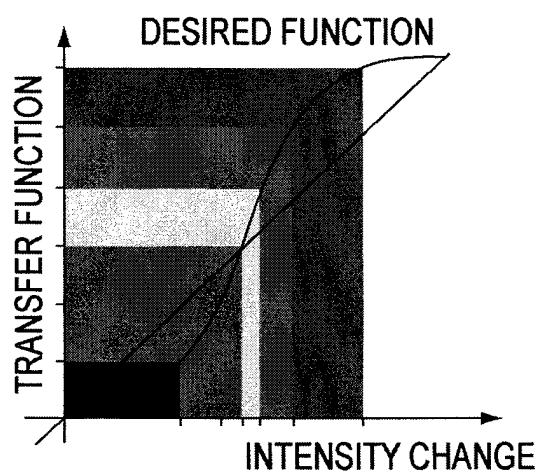


FIG. 16C

22/31

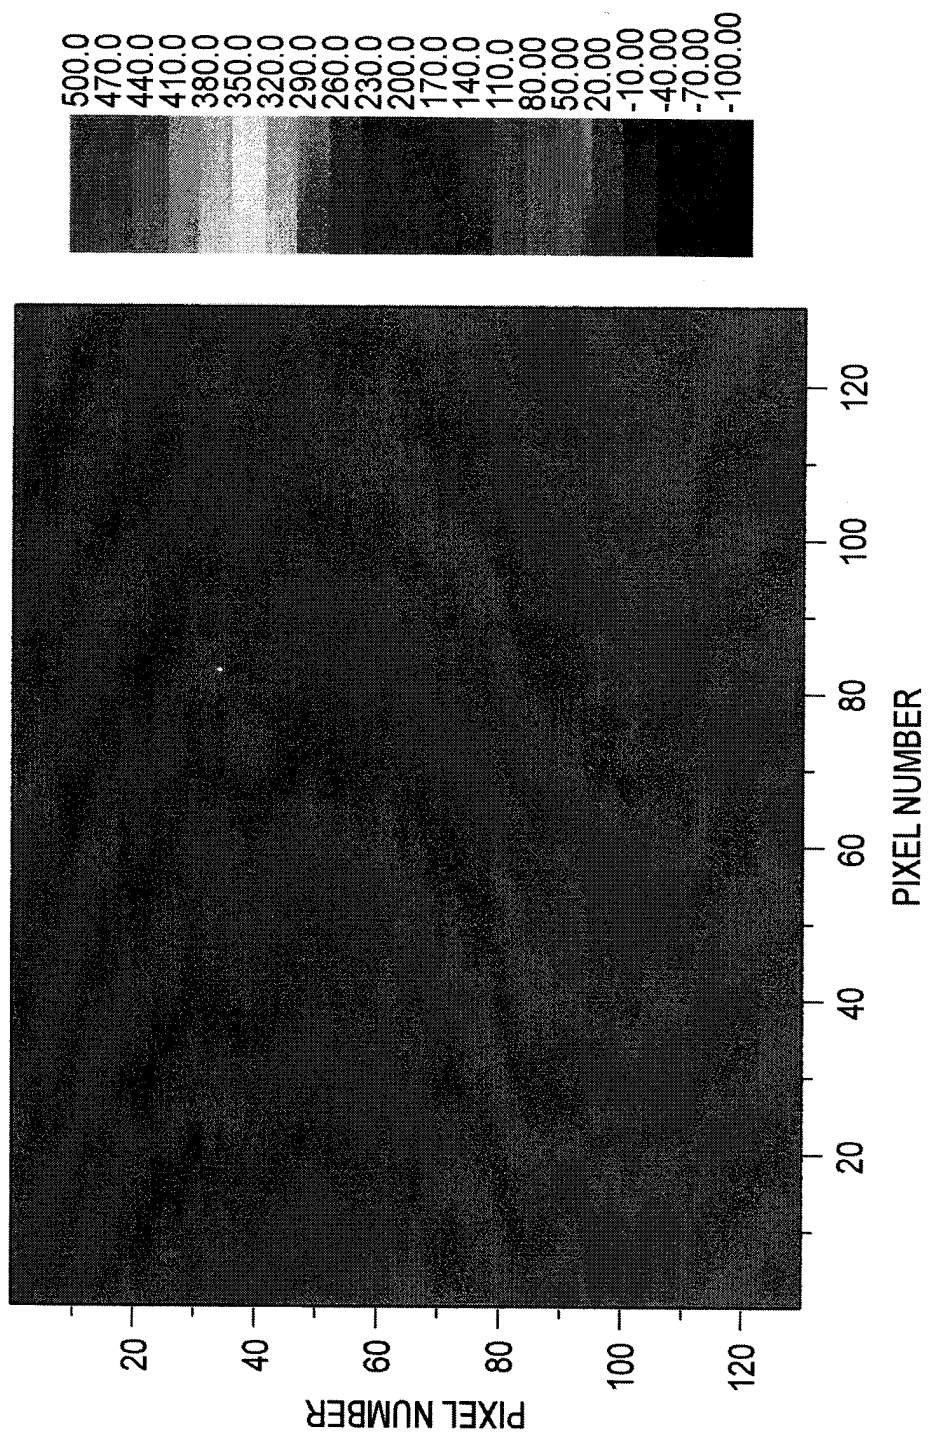

23/31

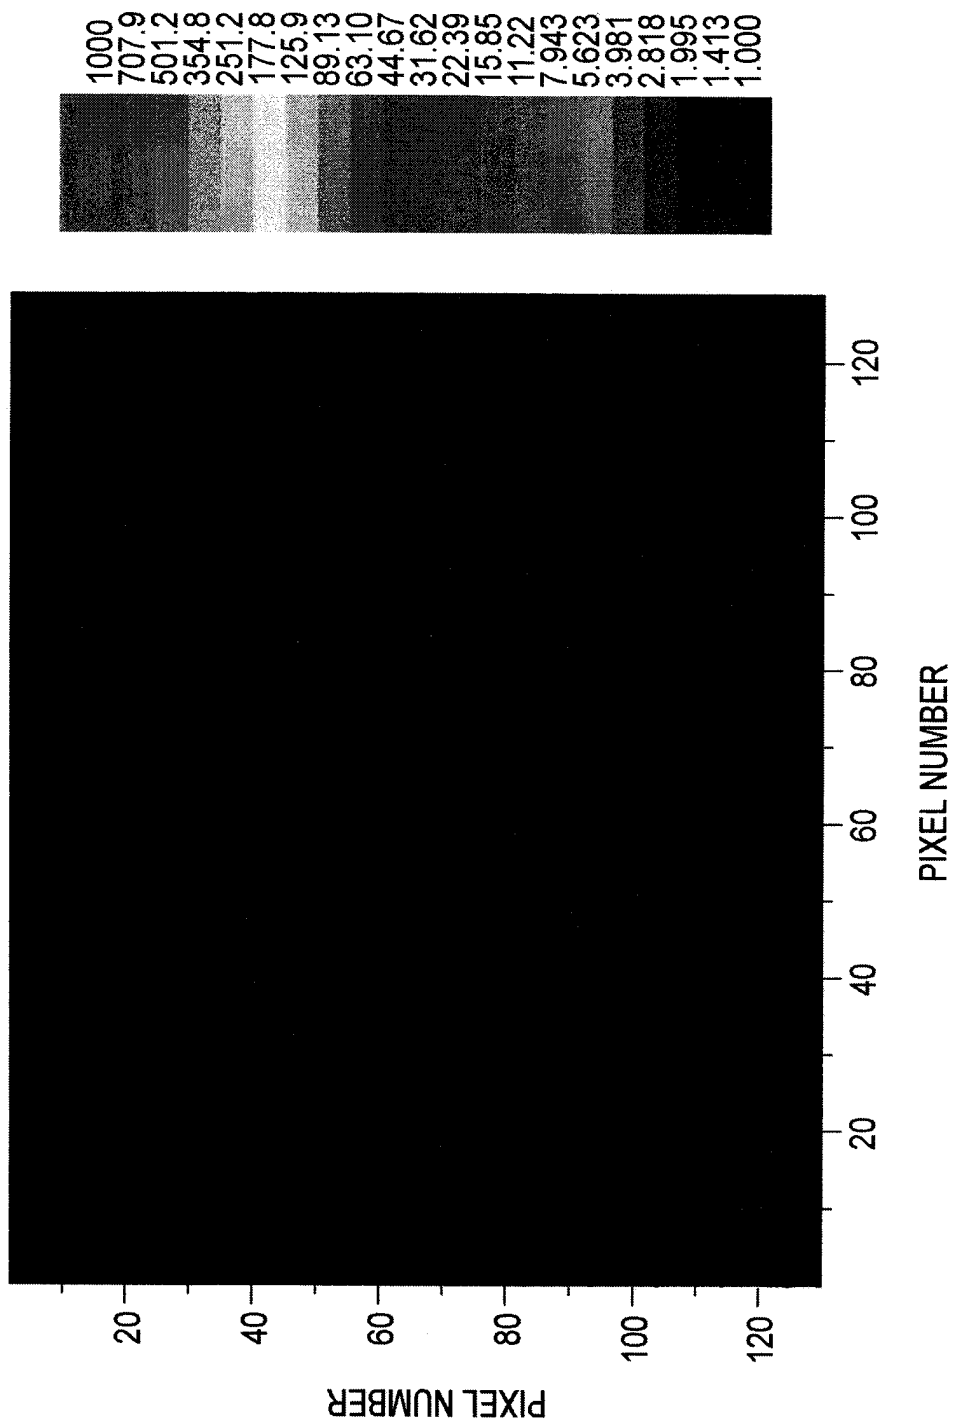


FIG. 17B

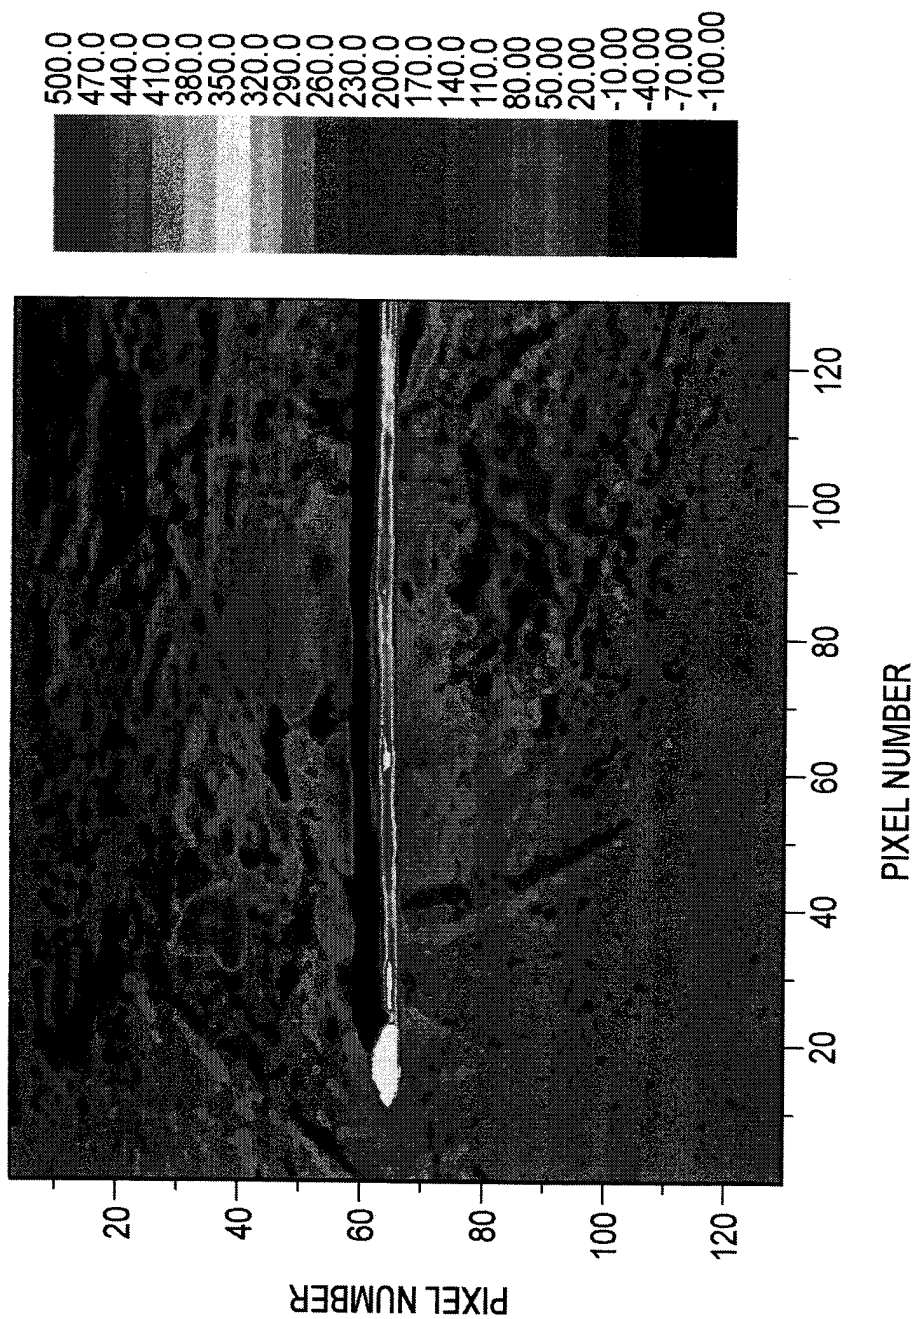


FIG. 18A

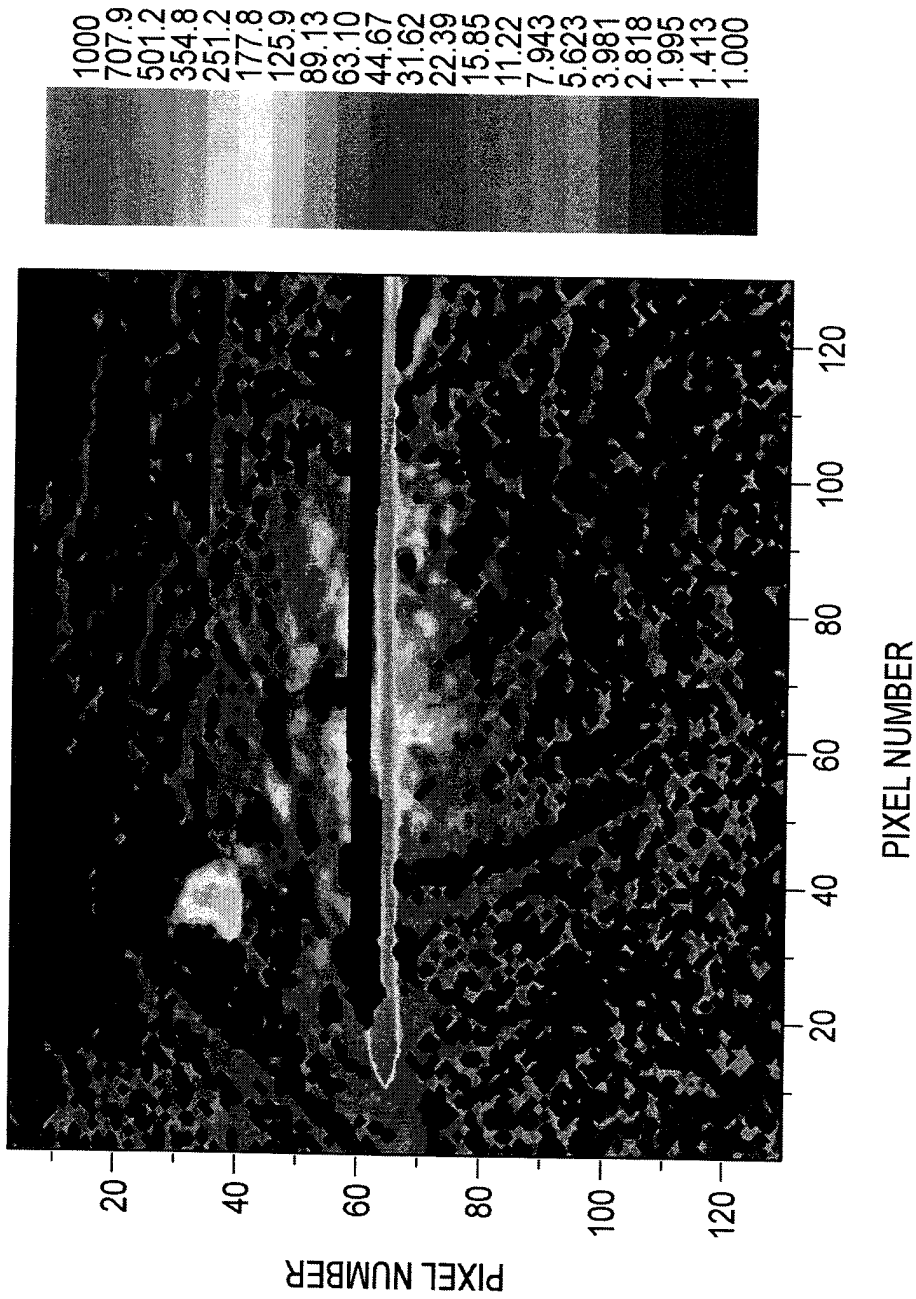


FIG. 18B

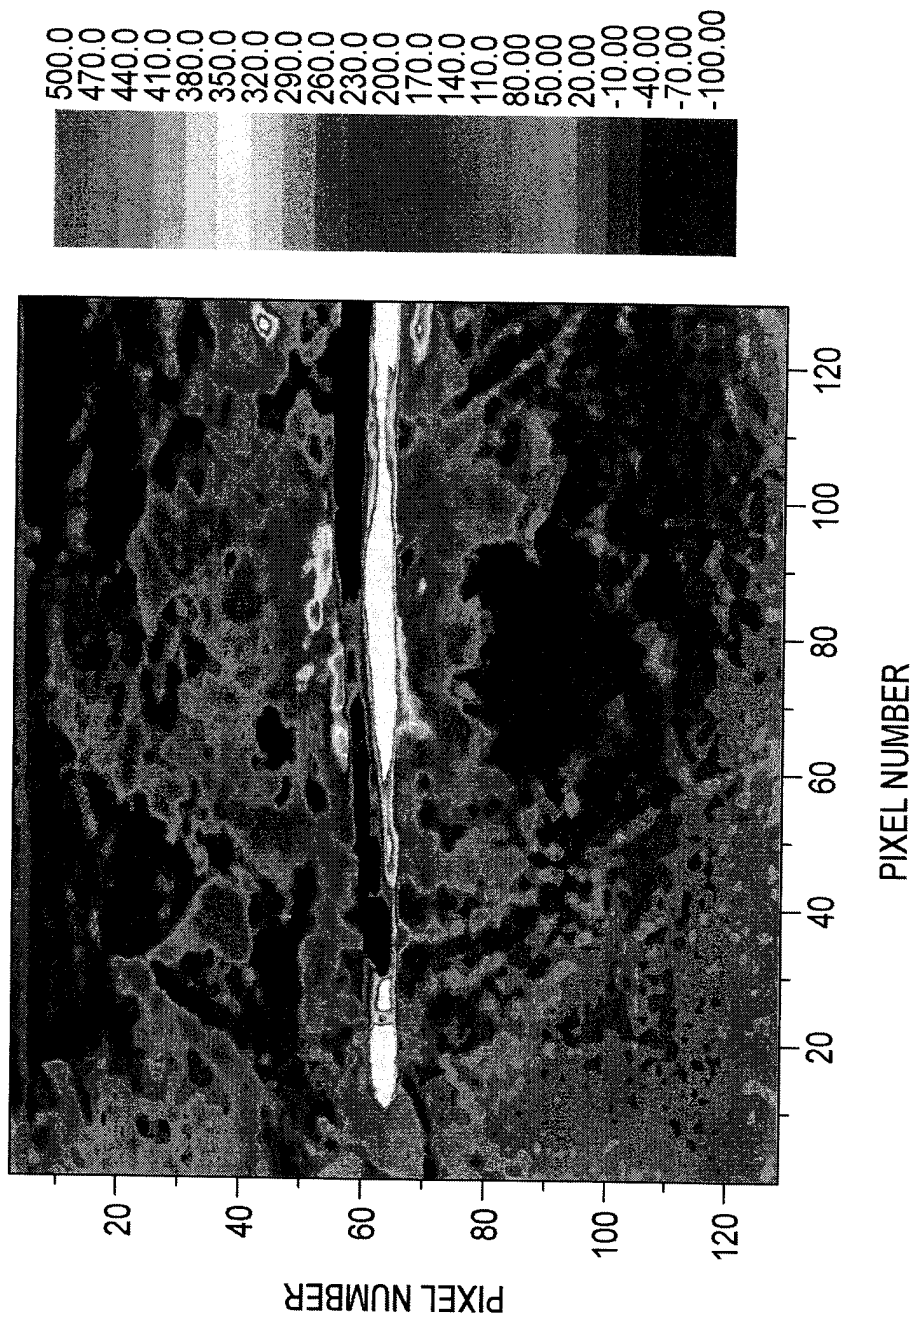
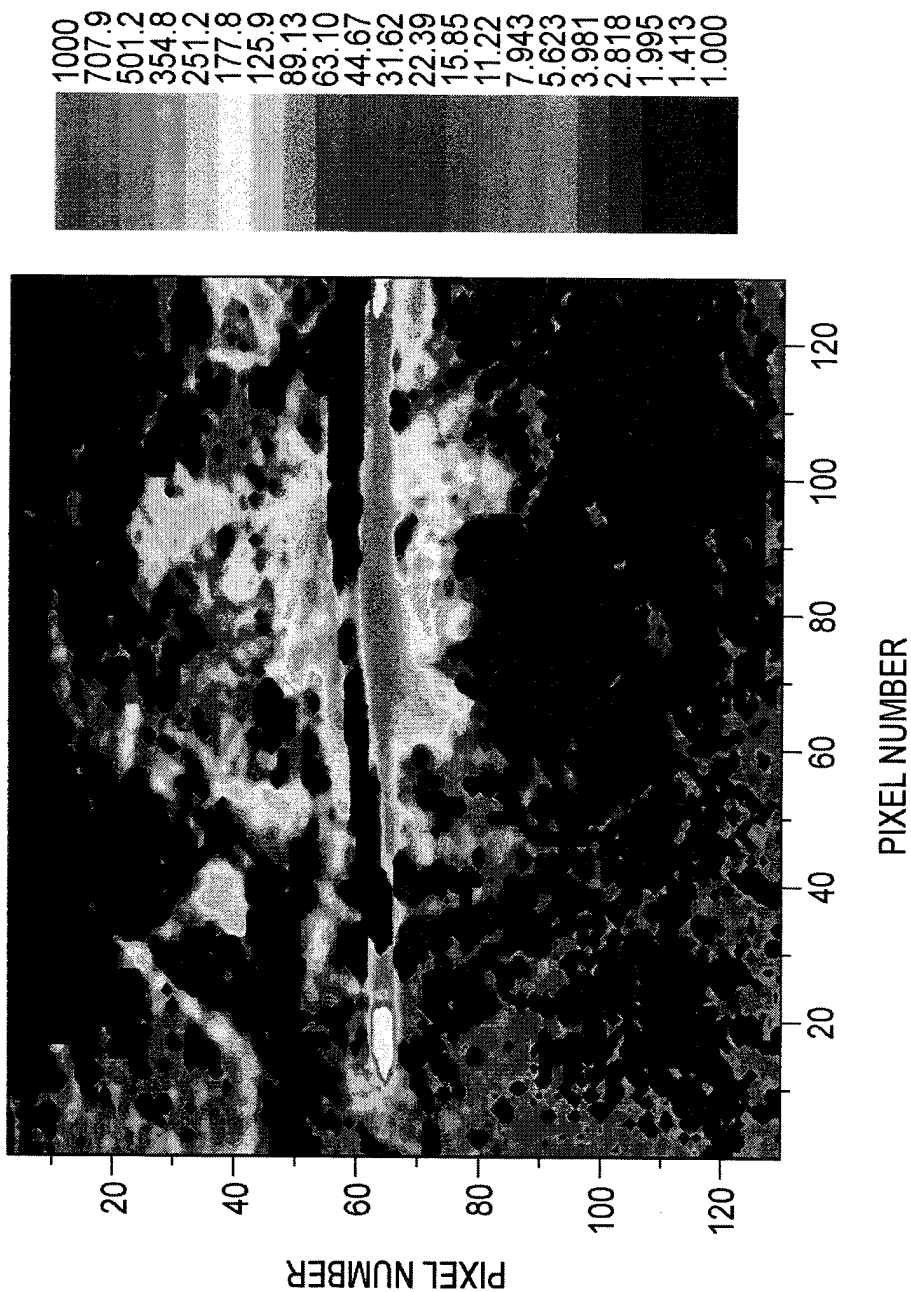


FIG. 19A



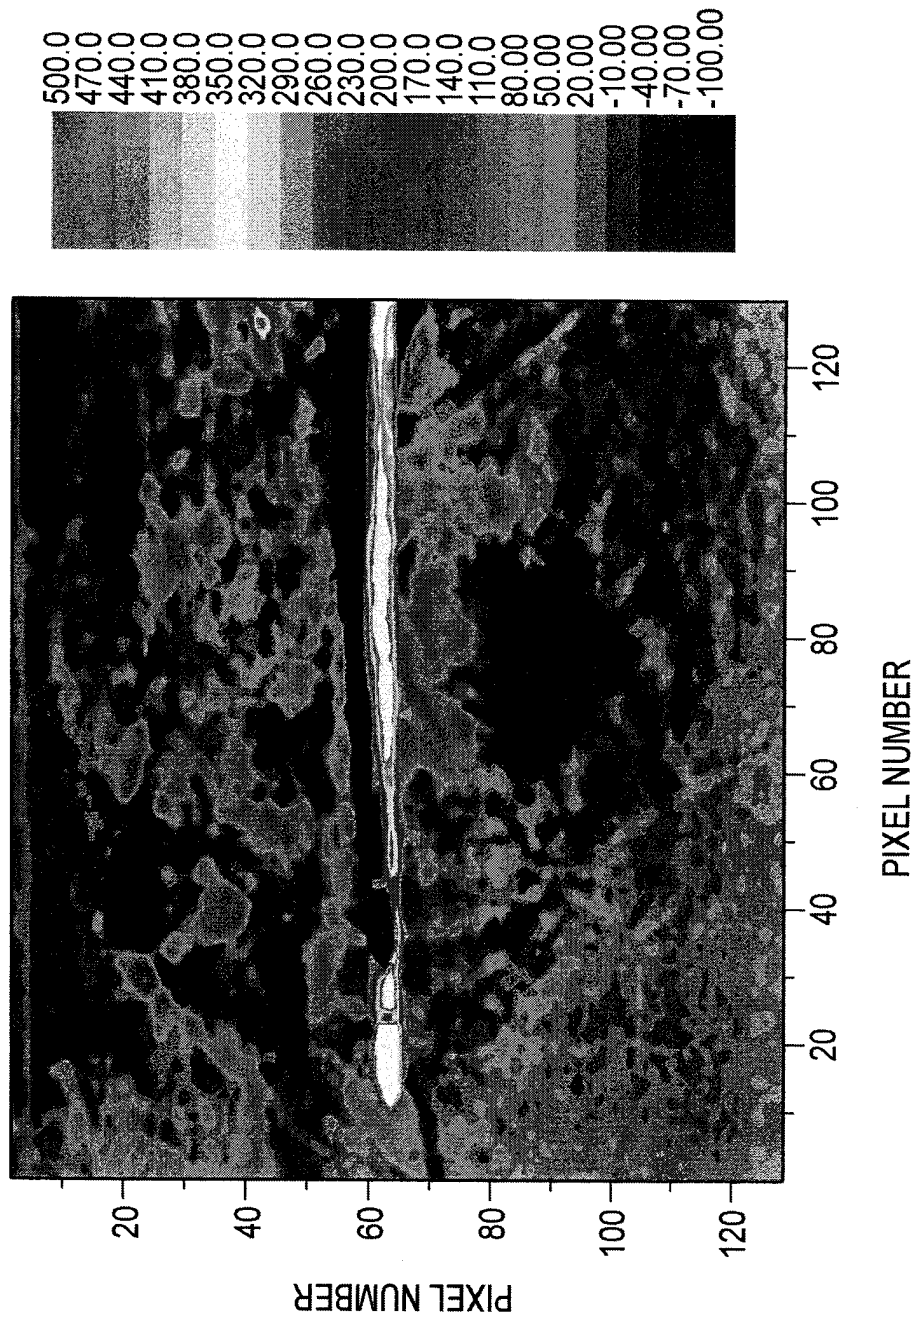


FIG. 20A

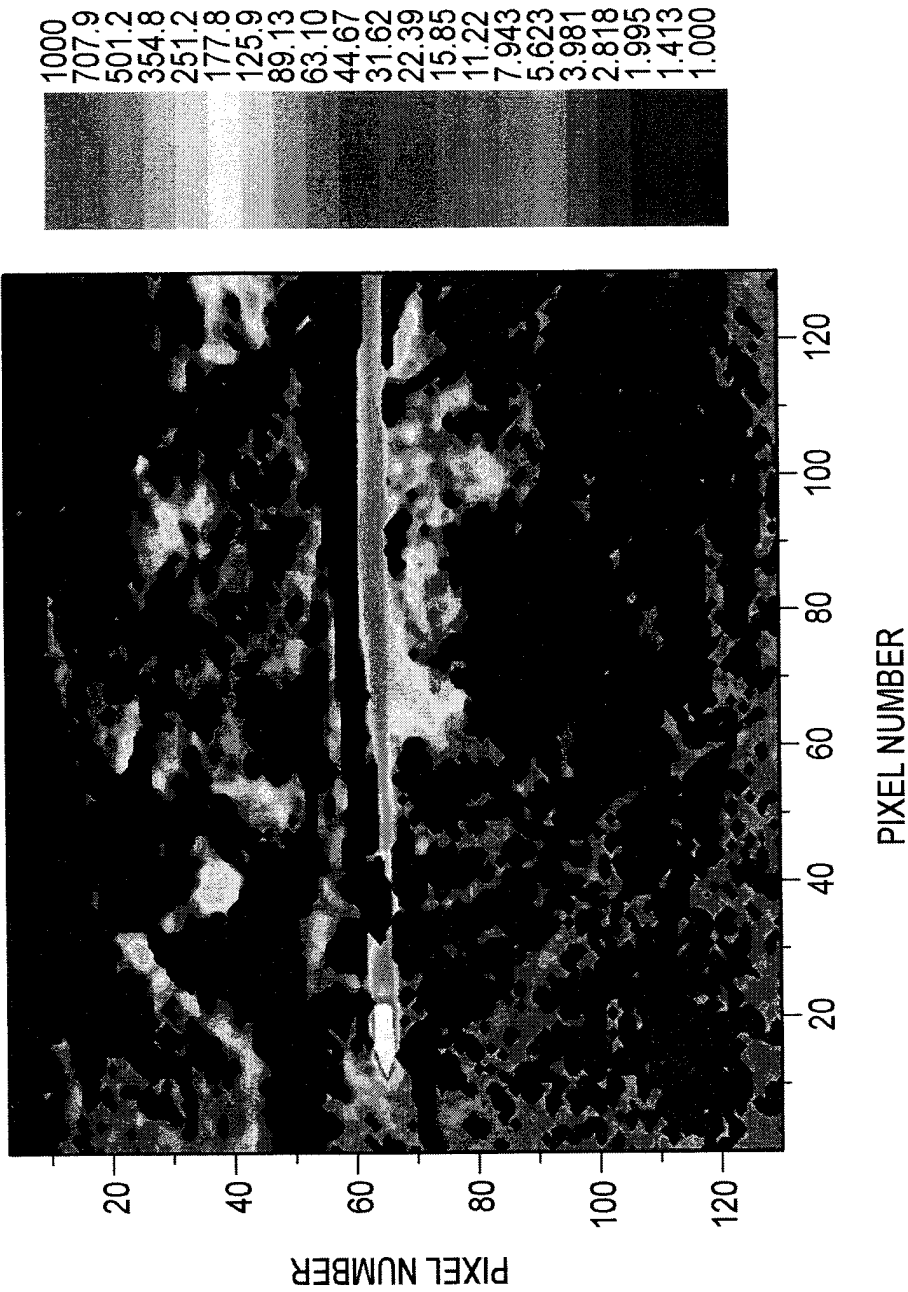


FIG. 20B

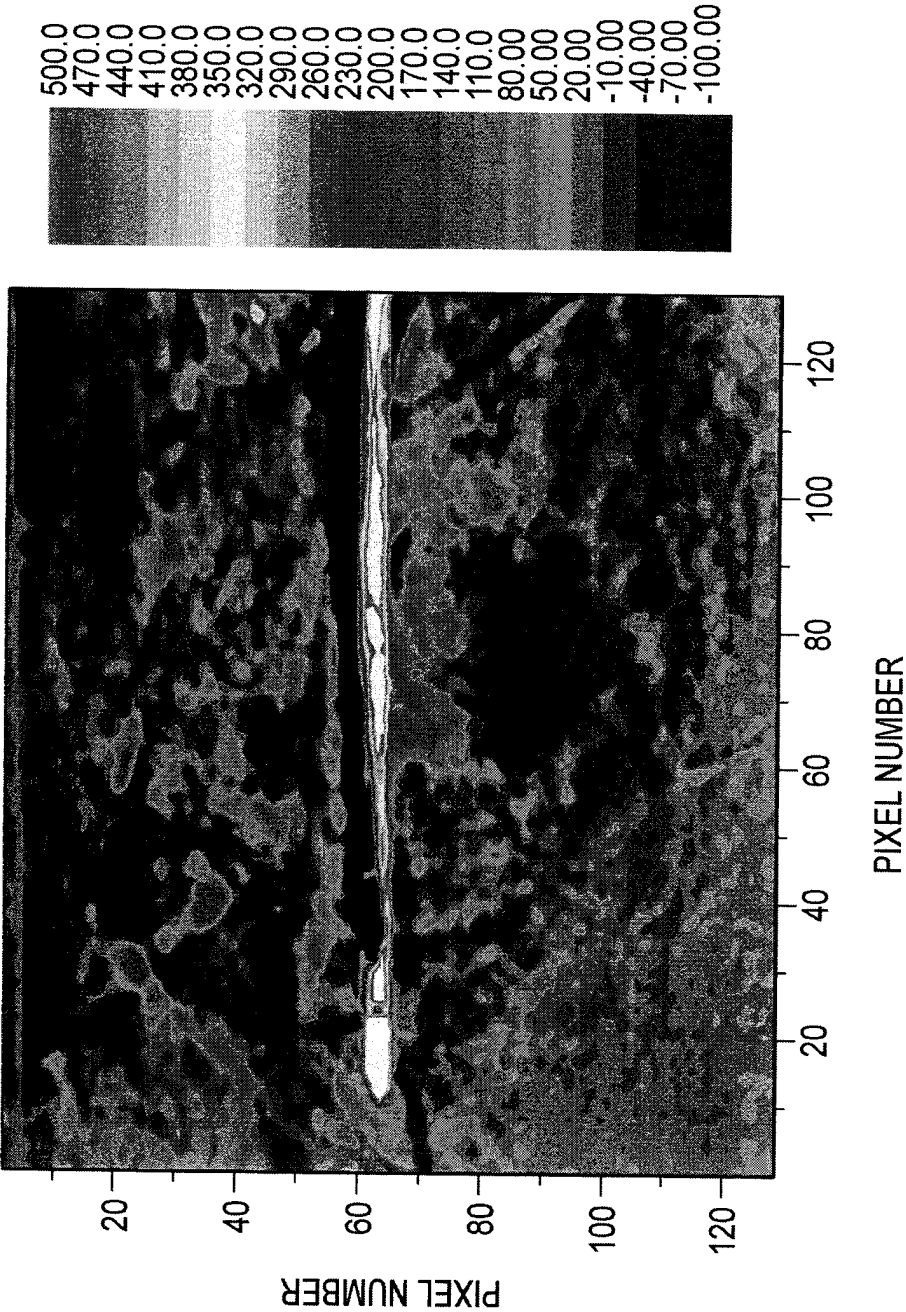


FIG. 21A

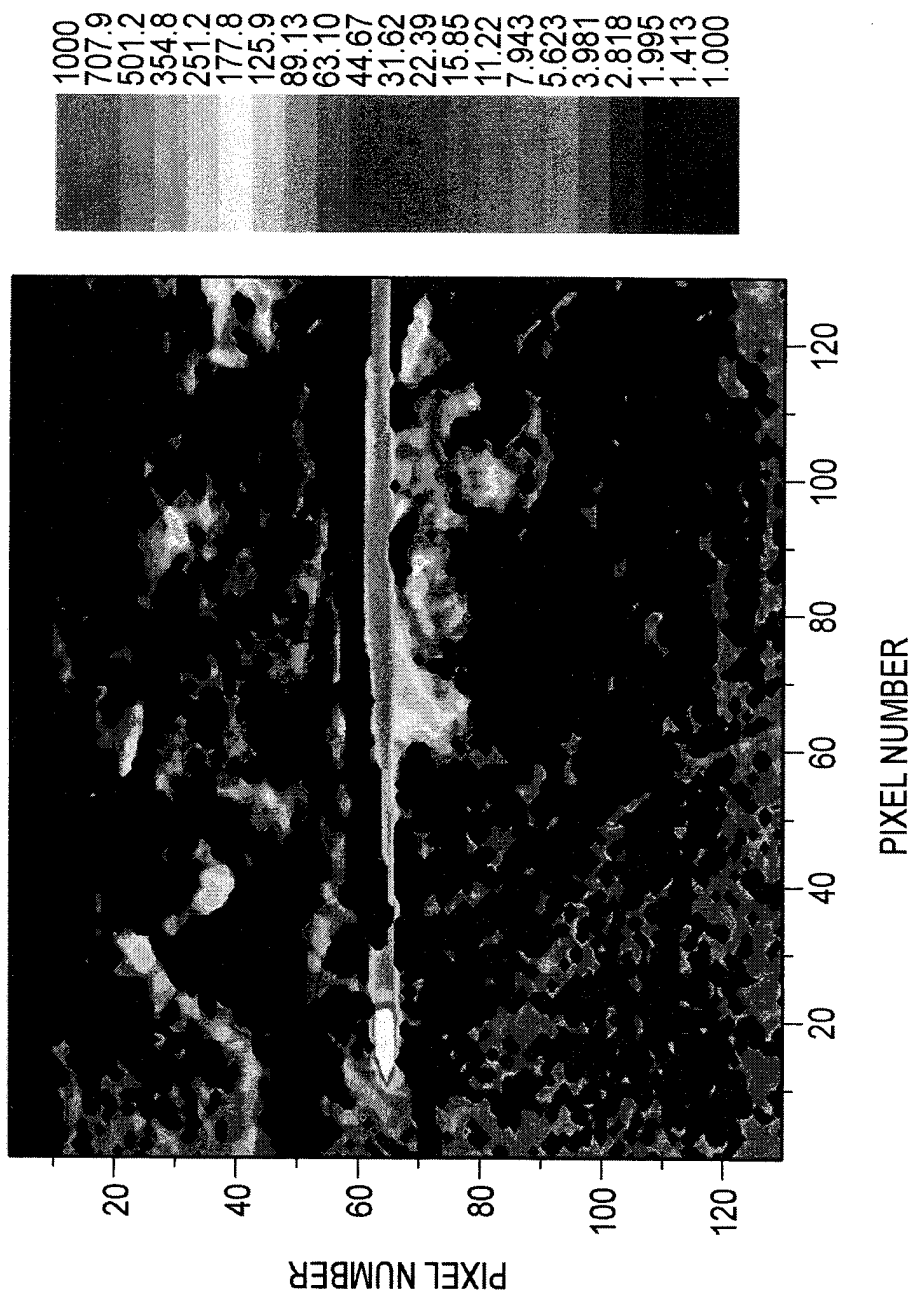


FIG. 21B

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 00/10814

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61N5/06

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61N A61B G01K

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, INSPEC

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	FALLONE B.G ET AL: "Noninvasive thermometry with a clinical x-ray CT scanner" MEDICAL PHYSICS, vol. 9, no. 5, - September 1982 (1982-09) pages 715-721, XP002144150 Page 720: section "Image subtraction"	31-39
Y	JENNE J.W. ET AL.: "CT on-line monitoring of HIFU therapy" 1997 IEEE ULTRASONICS SYMPOSIUM PROCEEDINGS, vol. 2, - October 1997 (1997-10) pages 1377-1380, XP002144151 Toronto the whole document --- -/--	31-39

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

2 August 2000

Date of mailing of the international search report

17/08/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Petter, E

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 00/10814

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 97 20193 A (DORNIER MED SYSTEMS INC) 5 June 1997 (1997-06-05) page 4, line 2 -page 6, line 31 ----	31-39
A	ZAMENHOF R.G. ET AL: "Comments on "Noninvasive thermometry with a clinical CT x-ray scanner" MEDICAL PHYSICS, vol. 10, no. 3, - May 1983 (1983-05) page 374 XP002144152 the whole document ----	31
A	US 5 370 121 A (REICHENBERGER HELMUT ET AL) 6 December 1994 (1994-12-06) column 1, line 34 - line 42 column 3, line 21 - line 31 -----	31

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 00/10814

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9720193 A	05-06-1997	AU 1062397 A EP 0864075 A JP 2000501530 T US 6067371 A	19-06-1997 16-09-1998 08-02-2000 23-05-2000
US 5370121 A	06-12-1994	DE 4229817 A FR 2695470 A JP 6189954 A	10-03-1994 11-03-1994 12-07-1994

专利名称(译)	在热疗期间使用高分辨率数字X射线系统对温度诱导的组织进行术中监测		
公开(公告)号	EP1171202A1	公开(公告)日	2002-01-16
申请号	EP2000926246	申请日	2000-04-21
[标]申请(专利权)人(译)	迈阿密大学		
申请(专利权)人(译)	迈阿密大学		
当前申请(专利权)人(译)	迈阿密大学		
[标]发明人	MANNS FABRICE ROBINSON DAVID MILNE PETER DENHAM DAVID B GONZALEZ CIRRE XOCHITL PAREL JEAN MARIE		
发明人	MANNS, FABRICE ROBINSON, DAVID MILNE, PETER DENHAM, DAVID B. GONZALEZ-CIRRE, XOCHITL PAREL, JEAN-MARIE		
IPC分类号	A61B5/00 A61B17/00 A61B18/24 A61N5/06		
CPC分类号	A61N5/0601 A61B5/015 A61B2017/00084 A61B2018/2005		
优先权	60/130497 1999-04-22 US		
外部链接	Espacenet		

摘要(译)

一种热诱导和监测组织局部区域变化的方法，用第一束X射线照射一定体积的组织，检测穿过组织体积的第一束X射线的部分，产生第一X - 从检测到的第一光束的X射线部分射出图像信号，在照射之后和检测之后将热量施加到组织体积内的至少组织的局部区域，用第二光束照射组织的体积。X射线，检测在用第二束X射线照射期间穿过组织体积的第二X射线束的部分，从X射线的X射线部分产生第二X射线图像信号。第二光束检测并基于第一和第二X射线图像信号的比较产生差分图像信号。差异图像信号提供由于施加热量导致的组织体积内的组织的局部区域的X射线衰减变化的信息。