




- (51) International Patent Classification:
A61H 31/00 (2006.01) *A61B 5/00* (2006.01)
- (21) International Application Number:
PCT/US2016/057198
- (22) International Filing Date:
14 October 2016 (14.10.2016)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
14/885,952 16 October 2015 (16.10.2015) US
- (63) Related by continuation (CON) or continuation-in-part (CIP) to earlier application:
US 14/885,952 (CON)
Filed on 16 October 2015 (16.10.2015)
- (71) Applicant: **ZOLL CIRCULATION, INC.** [US/US]; 2000 Ringwood Avenue, San Jose, CA 95131 (US).
- (72) Inventors: **JOSHI, Nikhil, S.**; 2000 Ringwood Avenue, San Jose, CA 95131 (US). **HARRIS, Melanie, L.**; 2000 Ringwood Avenue, San Jose, CA 95131 (US). **REYNOLDS, Byron, J.**; 2000 Ringwood Avenue, San Jose, CA 95131 (US).
- (74) Agent: **CROCKETT, K., David**; Crockett & Crockett, PC, 6B Liberty, Suite 145, Vlliso Viejo, CA 92656 (US).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU,

[Continued on next page]

(54) Title: AUTOMATED CHEST COMPRESSION DEVICE

(57) Abstract: A device for compressing the chest of a cardiac arrest victim.

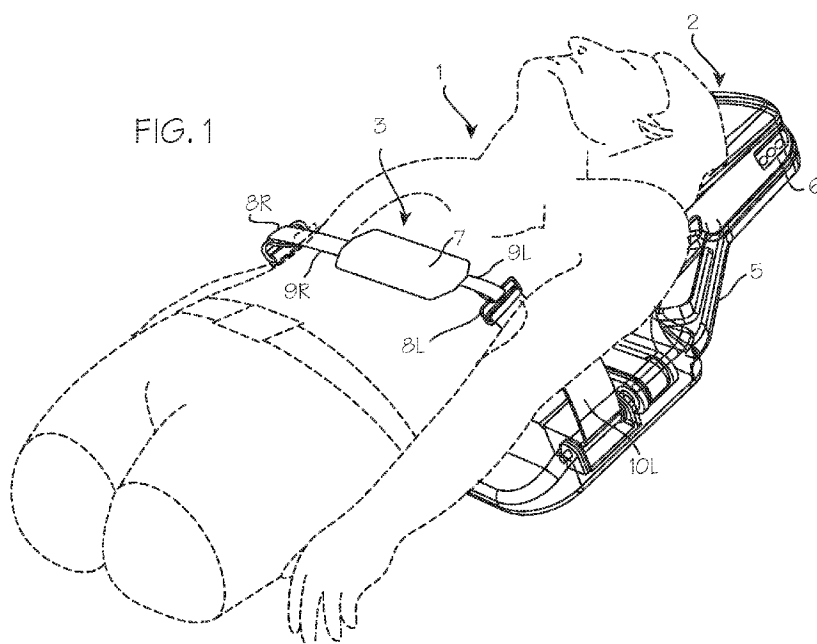



TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*

Automated Chest Compression Device

Field

[0001] The inventions described below relate to the field of CPR.

Background

[0002] Cardiopulmonary resuscitation (CPR) is a well-known and valuable method of first aid used to resuscitate people who have suffered from cardiac arrest. CPR requires repetitive chest compressions to squeeze the heart and the thoracic cavity to pump blood through the body. In efforts to provide better blood flow and increase the effectiveness of bystander resuscitation efforts, various mechanical devices have been proposed for performing CPR. In one variation of such devices, a belt is placed around the patient's chest and the belt is used to effect chest compressions, for example our commercial device, sold under the trademark AUTOPULSE®. Our own patents, Mollenauer, et al., Resuscitation Device Having A Motor Driven Belt To Constrict/Compress The Chest, U.S. Patent 6,142,962 (Nov. 7, 2000); Sherman, et al., CPR Assist Device with Pressure Bladder Feedback, U.S. Patent 6,616,620 (Sep. 9, 2003); Sherman, et al., Modular CPR assist device, U.S. Patent 6,066,106 (May 23, 2000); and Sherman, et al., Modular CPR assist device, U.S. Patent 6,398,745 (Jun. 4, 2002); Jensen, Lightweight Electro-Mechanical Chest Compression Device, U.S. Patent 7,347,832 (March 25, 2008) and Quintana, et al., Methods and Devices for Attaching a Belt Cartridge to a Chest Compression Device, U.S. Patent 7,354,407 (April 8, 2008), show chest compression devices that compress a patient's chest with a belt. Each of these patents is hereby incorporated by reference in their entirety.

[0003] These devices have proven to be valuable alternatives to manual CPR, and evidence is mounting that they provide circulation superior to that provided by manual CPR, and also result in higher survival rates for cardiac arrest victims. The devices provide Chest compressions at resuscitative rates and depths. A resuscitative rate may be any rate of compressions considered effective to induce blood flow in a cardiac arrest victim, typically 60 to 120 compressions per minute (the CPR Guidelines 2010 recommends 80 to 100 compression per minute), and a resuscitative depth may be any depth considered effective to induce blood flow, and typically 1.5 to 2.5 inches (the CPR Guidelines 2010 recommends about 2 inches per compression).

[0004] The AUTOPULSE® chest compression device uses a belt, which is releasably attached to a drive spool with the housing of the device. In a convenient arrangement, a spline is secured to the belt, and the spline fits into a slot in the drive spool of the device. The drive spool is accessible from the bottom, or posterior aspect, of the device. Before use, a fresh belt is fitted to the device, and this requires lifting the device to insert the spline into the drive spool. The patient is then placed on the housing of the device, and the belt is secured over the chest of the patient. Opposite ends of the belt are held together, over the chest of the patient, with hook and loop fasteners. The arrangement has proven effective for treating cardiac arrest victims and convenient to use. Other belt-based CPR compressions devices have been proposed, but not implemented in clinical use. Lach, Resuscitation Method and Apparatus, U.S. Patent 4,770,164 (Sep. 13, 1988) secures a belt around a patient by threading it under a first roller, then under a second roller, over the patient, back under the first roller, and then to a large roller disposed on one side of the patient. The belt is secured to the roller with hook and loop fasteners, and is

sized to the patient by the operator of the device. Kelly, Chest Compression Apparatus for Cardiac Arrest, U.S. Patent 5,738,637 (Apr. 14, 1998) uses a belt that is bolted at its midpoint to the underside of a backboard, than secured to a scissor-mechanism on the patient's chest with hook and loop fasteners. Belt installation is not convenient in either device. A new, more convenient arrangement of the drive components and belt is disclosed in this application.

[0005] Another feature of our AUTOPULSE® CPR chest compression device is the ability of the control system to hold the compression belt at the height of compression. The AUTOPULSE® can operate to perform compression in repeated compression cycles comprising a compression stroke, an high compression hold, a release period, and an inter-compression hold. No other automated CPR chest compression device is capable of holding compressions at a high threshold of compression. The method of operating the AUTOPULSE® device to accomplish compressions in cycles of compression, hold, and release is covered by our previous patent, Sherman, et al., Modular CPR assist device to hold at a threshold of tightness, U.S. Patent 7,374,548 (May 20, 2008). The holding periods are accomplished with a brake operably connected to the motor drive shaft of the device, which can be energized to stop the drive shaft to lock the belt in place about the patient. A new, more energy-efficient braking system is disclosed in this application.

[0006] On occasion, a chest compression device must be used on a patient at the same time that doctors want to take x-rays of the patient's chest. This is not possible if the radiopaque metal components of the chest compression device (the motor and drive train) are located directly under the load distributing portion of the compression belt, which overlies the patient's chest and heart when properly installed, so that the radiopaque component are also located

under the heart. This means that radiopaque component are in the field of view of the x-ray machine.

Summary

[0007] The devices and methods described below provide for a belt-driven chest compression device in which the compression belt is readily replaceable. The chest compression device includes a platform which houses drive components, and a compression belt which is connected to the drive components through releasably attachable couplings near the upper surface of the device. Removal and replacement of the belt may be accomplished while a patient is disposed on the housing. This arrangement helps avoid twisting of the belt and facilitates removal and replacement of the belt. Installation of the belt is simpler than our prior AUTOPULSE® device, and is tensioned upon installation by the user. To ensure that compression cycles start from an optimum low level of tightness, without slack, the control system of the device may control the device to loosen the belt upon start-up and thereafter draw the belt to the slack take-up position, or to tighten the belt upon start-up while monitoring an indicator of tightness (motor current, load on a load cell, strain on the belt), and conditionally tighten the belt to a slack take-up position (if the belt is loose initially) or reverse and loosen the belt and then tighten the belt while monitoring an indicator of tightness, to tighten the belt to a slack take-up position (if the initial tightness exceeds the desired tightness of a slack take-up position).

[0008] A brake is used to provide the holding periods during operation of the device. The brake comprises a parking pawl, with a pawl and park gear arrangement, with a park gear fixed to a component in the drive train, and a pawl operable to obstruct the park gear.

[0009] The arrangement of components in the device provides for a radiolucent region of the device, which underlies the heart of the patient when the device is installed properly on a cardiac arrest victim. For example, the compression belt may be driven by laterally located drive spools, which extend superiorly in the device to drive train components disposed superiorly to the compression belt (and, thus, superiorly to the heart of the patient when the device is installed).

Brief Description of the Drawings

[0010] Figure 1 illustrates the CPR chest compression device installed on a patient.

[0011] Figure 2 is a perspective view of the CPR chest compression device, illustrating the connection between the compression belt and intermediate straps at a point above the housing.

[0012] Figure 3 illustrates the single-piece compression belts which may be used in the compression device of Figure 1.

[0013] Figure 4 is a perspective view of drive train of the compression device, including the motor and drive shaft, drive belts, and secondary or planetary drive spools.

[0014] Figure 5 is an end view of drive spool, drive belts, and secondary drive spools.

[0015] Figures 6, 7, 8, 9 and 10 illustrate alternative drive trains for rotating the drive spools.

[0016] Figures 11, 12 and 13 illustrate improved braking mechanisms for use with the drive train of Figure 4 and other chest compression devices.

Detailed Description

[0017] Figure 1 shows the chest compression device fitted on a patient 1. The chest compression device 2 applies compressions with the compression belt 3. The chest compression device 2 includes a belt drive platform 4 sized for placement under the thorax of the patient, upon which the patient rests during use and which provides a housing 5 for the drive train and control system for the device. The control system, embedded anywhere in the device, can include a processor and may be operable to control tightening operation of the belt and to provide output on a user interface disposed on the housing. Operation of the device can be initiated and adjusted by a user through a control panel 6 and a display operated by the control system to provide feedback regarding the status of the device to the user.

[0018] The belt includes a wide load-distribution section 7 at the mid-portion of the belt and left and right belt ends 8R and 8L (shown in the illustration as narrow pull straps 9R and 9L), which serve as tensioning portions which extend from the load distributing portion, posteriorly relative to the patient, to drive spools within the housing. The left and right belt ends are secured to intermediate straps 10R and 10L, with loops 11R and 11L (for example, square loops, as illustrated). When fitted on a patient, the load distribution section is disposed over the anterior chest wall of the patient, and the left and right belt ends extend posteriorly over the right and left axilla of the patient to connect to their respective lateral drive spools shown in Figure 2.

[0019] Figure 2 shows the chest compression device in isolation, including the belt drive platform and housing. As illustrated in Figure 2, the intermediate straps 10R and 10L are secured at one end to the loops, and secured at the other end to planetary drive spools 12R and 12L disposed laterally

on either side of the housing. The planetary or lateral drive spools are in turn driven by a motor also disposed within the housing, through various belts and gears described below. The intermediate straps are attached to the planetary or lateral spools such that, upon rotation of the spools, the intermediate straps are pulled posteriorly, spooled upon the lateral spools, thereby drawing the compression belt downward to compress the chest of the patient. The intermediate straps can be fixed to the planetary or lateral drive spools in any suitable manner. The intermediate straps may be flexible and floppy, or they may be self-supporting (that is, they remain in vertical orientation, without other support, when the platform is horizontal) so long as they are still flexible enough so they may be wrapped around the drive spools.

[0020] The belt 3, as shown in Figure 3, comprises the load distribution section 7 and left and right belt ends 8R and 8L in the form of left and right pull straps 9R and 9L. The load distribution section is sized and dimensioned to cover a significant portion of the anterior surface of a typical patient's chest. The pull straps are narrow, relative to the load distribution section, to limit material requirements of the associated spools, but the belt ends may be made in the same width as the load distribution section. Corresponding hook sections and loop sections (13R, 13L) on the left and right belt ends secure the compression belt to the loops (11R, 11L) and thus to the intermediate straps 10R and 10L. The pull straps are fitted through the loops, folded together and secured with hook and loop fasteners or other releasable attachment system (that is, attachment systems that can be operated to quickly attach and detach the two parts without tools). The hook and loop fasteners together with the loops provide a convenient means for releasably securing the compression belt to the intermediate straps, in conjunction with double loop sliders illustrated in Figure 1, but other

convenient means of releasably attaching the belt ends to the intermediate straps may be used (such as matching center release buckle components (seat belt buckles), side release buckles (back pack buckles) cam buckles, belt buckles, etc. may be used). (The belt may instead be attached directly to the drive spools.) One size belt may be used for patients of various sizes, or belts of various sizes can be provided for use with the device depending on the size of the patient. The initial tightness of the belt is established by a CPR provider who pulls the straps through the double loop sliders and attaches hook and loop segments together (the system may establish a slack take-up position for the belt, as described below, after the CPR provider has secured the belt to the buckles). The belt is preferably a one-piece belt, but can be provided as a two-piece belt with overlapping load-distribution sections which can be applied by first laying one side over the patient's chest and next laying the other side over the first side, and securing the two sections together (with, for example, corresponding hook and loop fasteners). Also, the belt may be configured as a two-piece belt having two pieces (for example, where a first pull strap is one piece, and a second pull strap together with a load distribution section constitutes a second piece) secured together with a coupling mechanism (for example, a releasable coupling mechanism, a buckle, or Velcro hook and loop fasteners or clamps or other convenient means of releasably attaching the belt). The pull straps may be releasably attached directly to the drive spools or to intermediate straps. The coupling mechanism may be located at various locations along the pull strap. The provision of the coupling mechanism may facilitate installation of the device, and minimize material requirements for construction of the device. A bladder may be incorporated into the load-distribution section 7.

[0021] The belt ends may be attached directly to the drive spools, using a spline and slot arrangement disclosed in our prior U.S. Patent, Quintana, et al., Methods And Devices For Attaching A Belt Cartridge To A Chest Compression Device, U.S. Patent 8,740,823 (Jun. 3, 2014). The belt ends may be attached directly to the drive spools using any suitable fastener, clamp or connecting means. The belt and its attachments to the drive spools need not be symmetrical. For example, the belt may comprise a tensioning portion or strap adapted for direct connection to the drive spool on one side, and also comprise a tensioning portion or strap adapted for an indirect connection to the drive spool, through an intermediate strap, on the other side.

[0022] The drive spools have a first segment engaging the drive belts, and a second segment, extending inferiorly from the first segment, which engages the intermediate straps or belt ends. The space between the drive spools, on a corresponding coronal plane and inferior to the drive belts, is unoccupied by drive train components or other radiopaque components and thus constitutes the radiolucent window mentioned above.

[0023] In use, a CPR provider will apply the compression device to a cardiac arrest victim. The CPR provider will place the cardiac arrest victim on the housing 5, and secure the belt ends 8R and 8L to the respective left and right intermediate straps (or directly to the drive spools), with the patient already on the anterior surface of the housing, so that there is no need for access to the bottom surface of the device. Where the compression belt is a one-piece belt, at least one of the belt ends is secured to its corresponding drive spool (directly) or intermediate strap after the patient is placed on the platform. Where the belt is an asymmetrical belt (with one end adapted for direct connection to a drive spool, and the other end adapted for indirect connection

through an intermediate strap or a pull strap), then the user will secure one belt end to the drive spool and the other belt end to the intermediate strap. Where the belt is a two-piece belt, with overlapping load-distribution sections, the user will, before or after securing the belt end to the drive spools, lay one side over the patient's chest and lay the other side over the first side to complete the assembly. Where the belt is a two-piece belt having two pieces coupled to one another, for example, with one of the straps releasably attached to the load distribution section and the other strap fixed to the load distribution section, the user will before or after securing the belt end to the drive spools or intermediate straps, connect the two pieces together. With the belt in place, the CPR provider initiates operation of the chest compression device to repeatedly compress the chest of the patient to a depth and at a rate suitable for resuscitation. If the belt must be replaced after the patient is placed on the platform, the CPR provider can readily detach the compression belt from the intermediate straps or the drive spools and install a new compression belt by securing the belt end of the new compression belt to the intermediate straps or drive spool. This can be done without removing the patient from the housing, which saves a significant amount of time compared to prior art systems and minimizes the delay in initiating chest compressions attendant to belt replacement. With the belt in place, the CPR provider initiates operation of the device to cause repeated cycles of tightening and loosening of the belt about the thorax of the patient. Should the belt become damaged, or twisted during use (the front-loading device should make twisting less likely), the CPR provider interrupts operation of the device to replace the belt, detaches the right belt end from the right intermediate strap or right drive spool, and detaches the left belt end from left intermediate straps or the left drive spool, while the patient remains on the platform.

[0024] The benefits of the compression belt and intermediate straps arrangement, with a releasable attachment to the intermediate straps, can be achieved in combination with the benefits of additional inventions described below, or they may be achieved in isolation. The benefits of the compression belt and releasable attachment to the drive spools, can be achieved in combination with the benefits of additional inventions described below, or they may be achieved in isolation.

[0025] Figure 4 is a perspective view of drive train of the compression device, including the drive shaft, drive belts, and planetary drive spools, which operably connects the motor 20 and its motor shaft to the compression belt. The drive train comprises a first drive shaft 21 (in this case, an extension of the motor shaft or the output shaft of any reduction gears) and a first gear 22 (a sun gear) which in turn is fixed to the first drive shaft. The first/sun gear engages a second/planetary gear 23 which in turn is fixed to a second drive shaft 24. (The motor shaft, first and second drive shafts, gears and drive spools are supported in a channel beam which extends across the device, providing support for the components and the housing.) Rotation of the first drive shaft 21 in one direction results in counter-rotation (rotation in the opposite direction) of the second drive shaft 24. The first and second drive shafts thus rotate in opposite directions. The first and second drive shafts 21 (left) and 24 (right) are connected to the first and second lateral drive spools 12R and 12L through drive belts 25R and 25L, such that rotation of the first and second shafts results in rotation of the first and second lateral drive spools, which in turn spool the intermediate straps (or belt ends) to cause tightening of the compression belt about the chest of the patient. As illustrated in Figure 4, the drive shafts may comprise toothed wheels (driving pulleys) and the drive spools

may comprise toothed wheels (driven pulleys), and the drive belt is a toothed drive belt. The motor shaft can be connected to the first drive shaft 21 directly or through reduction gears in a gear box 26. A brake 27 may be operably connected to the drive train at any appropriate point, and several embodiments of preferred brakes are shown in more detail in Figures 11, 12 and 13.

[0026] As depicted in Figure 4, the drive shafts 21 (left) and 24 (right) are disposed asymmetrically about the inferior/superior centerline of the device, but the drive spools may be disposed symmetrically. The belts provide a convenient linkage between the toothed wheels, and may be replaced with comparable components such as chains, with corresponding sprockets on the drive shafts (21, 24) and first and second lateral drive spools 12R and 12L, or worm gears interconnecting drive shaft (or shafts) with the lateral drive spools.

[0027] In the arrangement of Figure 4, a single motor is used to drive both drive shafts and both drive spools, without a direct connection to the compression belt, which is one system which enables the anterior releasable attachment system for the compression belt. In this arrangement, the motor 20, battery 28, and control system are located superiorly to the portion of the lateral drive spools 12R and 12L to which the intermediate straps or belt ends are secured (in our current AUTOPULSE® compression device, the motor drive shaft is located on the same transverse plane as the lateral spindles) thus leaving an open, unoccupied space in the inferior portion of the device which is devoid of radiopaque components. This open, unoccupied space is located beneath (posterior to) the load distributing band. Thus, when the compression device is installed on the patient, this unoccupied space is located under the heart of the patient, and provides a clear, radiolucent window for imaging the heart with fluoroscopy, x-

rays or CT scanning. When installed on the patient, motor and drive shafts which drive the belts are located superiorly to the region of the housing underlying the compression belt, corresponding to the region of the patient's heart, and the drive spools, though they extend inferiorly into the superior/inferior level of the heart, are laterally displaced from the centerline of the housing (and, correspondingly, from the centerline of the patient's body). The benefits of the drive train illustrated in Figure 4 can be obtained in combination with the front-loaded compression belt of Figure 1, or with other belt attachment mechanisms. Also, the benefits of the radiolucent window can be achieved with other arrangements of the drive train, so long as the drive train components are displaced along the superior/superior axis of the device (superiorly or inferiorly) from the area of the platform which underlies the patient's heart during use (for example, two motors may be used, with one motor operably connected to each drive spool, or directly to each drive shaft).

[0028] Figure 5 is an end view of the drive shaft (from the inferior end of the device), drive belts, and secondary drive spools shown in Figure 4, including the drive shafts 21 (left) and 24 (right), lateral drive spools 12R and 12L, drive belts 25R and 25L and the motor 20. During the compression stroke, the motor is operated to turn each drive spool sufficiently to pull the intermediates straps (or belt ends) downward to the extent necessary to achieve compression at the desired depth. This may vary with the diameter of the drive spools. Preferably, the drive spools 12R and 12L are about 0.75" (2 cm) in diameter, and rotate about 2.5 rotations on each compression stroke (drive spool 12R will rotate counter-clockwise when viewed from the inferior view of Figure 5 and drive spool 12L will rotate clockwise, in this arrangement) to pull the intermediate straps (or belt ends) downwardly

(posteriorly, relative to a patient laying supine on the housing) about 1 to 2 inches (2.5 to 5 cm) to obtain a chest compression of the desired depth of 2 inches (5 cm). The drive spools 12R and 12L may be made with a larger diameter, such that it takes less rotation, such as half of a complete rotation, to spool the intermediate straps (or belt ends) only partially around the drive spools, to pull the intermediate straps (or belt ends) downward to the extent necessary for adequate compression. In this arrangement, the intermediate straps can be made of a fairly stiff material, such that they are self-supporting and stand vertically above the housing when not attached to the belt.

[0029] The drive train can be varied, while still achieving the benefits of arrangement which permits attachment of the belt to the drive train from the front or side of the housing. For example, as shown in Figure 6, the linkage between the drive spools can be provided with a rack and pinion system, with drive pinions (toothed wheels) 31R and 31L, and right and left racks 32R and 32L and right and left driven pinions 33R and 33L. (Various arrangements can be used to properly rotate the drive spools, including a single pinion with a reversing gear at one of the drive spools, or disposition of the belt end/intermediate strap on opposite sides of the drive spools, as shown in Figure 8.) As shown in Figure 7, the linkage between the drive shafts can drive the left and right drive shafts and the left and right drive spools 12R and 12L through drive straps 34R and 34L. The drive straps in this system spool about the drive shafts, and also about the left and right drive spools 12R and 12L (a single drive shaft may be used in this embodiment).

[0030] In operation, rotation of the drive shafts will result in spooling of the drive straps 34R and 34L on the drive shafts 31R and 31L, which will result in rotation of drive spools 12R and 12L, and thus result in tightening of the

compression belt. This system may use the natural resilience of the chest to expand the compression belt in the release phase of the compression cycle, while the motor operates to allow unspooling of the drive straps 34R and 34L about the drive shafts 31R and 31L coincident with the spooling of the drive straps 34R and 34L about the drive spools 12R and 12L.

[0031] Figure 8 shows a drive train in which both the right and left belts are driven by a single drive shaft, with each drive belt causing rotation of its associated drive spool in opposite directions, with one of the drive spool/intermediate strap (or belt ends) connections disposed on the inside (medial) portion of the drive spool to ensure that rotation of the drive spool results in spooling of the intermediate strap (or belt ends) on the drive spool. Each of these drive trains can be used in a system in which the compression belt is releasably or permanently attached to the drive train from the front of the device, or the side of the device, thus allowing installation, removal and replacement of the belt while the patient is on the platform. (Analogous to the usage relating to automobiles, the drive train is the group of components that operate to deliver power to the belt, exclusive of the motor).

[0032] Figure 9 shows a drive train similar to the drive train of Figure 5, in which the lateral drive spools 12R and 12L of Figure 5 are replaced with sprocketed spools 35R and 35L. The sprocketed spools engage corresponding perforations in the intermediate straps (or belt ends), and pull the intermediate straps (or belt ends) downward when rotated in a first direction, thus tightening the belt, and push the intermediate straps (or belt ends) upward when rotated in the opposite direction, thus loosening the belt. Corresponding tensioning spools 36R and 36L are provided immediately adjacent to the sprocketed spools 35R and 35L, to force the

perforated intermediate straps (or belt ends) into engagement with a sprocket of the sprocketed spools.

[0033] In each of the drive trains illustrates in Figures 5 through 9, levers may be used in lieu of a large diameter drive spool, and would function to pull the intermediate straps (or belt ends) posteriorly. Levers attached to the intermediate straps, driven by the same mechanisms proposed for the lateral drive spools, will pull the intermediate straps posteriorly to tighten the belt.

[0034] Figure 10 shows a drive train for driving the compression belt using a ring gear and pinion. In this system, the ring gear 37 takes the place of the rack of the drive train of Figure 6 described above, to transfer power from the motor and drive shaft to the lateral drive spools. In this system, drive pinion 31 drives the ring gear, in alternating clockwise and counterclockwise rotations, which in turn drive the driven pinions 33R and 33L and their translating output pinions 38R and 38L, which in turn drive the drive spools 12R and 12L in back and forth rotations to pull down and push up, or spool and unspool, the intermediate straps 10R and 10L (or belt ends) (not shown). The ring gear is preferably located superiorly to the inferior portion of the drive spools which engage the intermediate straps (or belt ends), so that, when a patient is disposed on the device, with the belt properly positioned over the thorax, the ring gear does not lie in the region of the housing which underlies the patient's heart.

[0035] Finally, the drive spools can be replaced with any convenient lever mechanism, driven through appropriate linkages by the motor, and operable to pull the intermediate straps (or belt ends) downwardly and push the intermediate straps (or belt ends) upwardly (or at least allow upward motion on recoil of the patient's thorax), while obtaining the

benefit of maintaining an empty space in the "heart" region of the housing. The spools, however, are a convenient implementation of a leveraging mechanism.

[0036] The compression device preferably operates to provide cycles of compression which include a compression down-stroke, a high compression hold, a release period, and an inter-compression hold. The hold periods are accomplished through operation of a brake operable to very quickly stop the rotating components of the drive train. Any brake may be used, including the cam brake or wrap spring brake previously proposed for use in a chest compression device, or the motor can be stalled or electronically balanced to hold it during hold periods. Figure 11 illustrates an improved braking mechanism that may be used with the drive train of Figure 4. The braking mechanism comprises a parking pawl mechanism, similar to parking pawls used in automotive transmissions. The parking pawl 41 and associated park gear (a notched wheel or ratchet wheel) 42 can be located at any point in the drive train or motor shaft, with the park gear non-rotatably fixed to any rotating component, and is shown in Figure 11 fixed to the motor shaft 21, between the motor 20 and the gear box 26. The pawl 41 is operated by a solenoid actuator 43 and solenoid plunger 44 or other actuator (for example, a motor may be used to swing the pawl into contact with the park gear), which is fixed relative to the drive shaft. To brake and stop the drive train the control system operates the solenoid to force the pawl into interfering contact with the park gear, and to release the drive train the control system operates the solenoid to withdraw the pawl from the park gear. Preferably, the pawl is spring-biased away from the park gear, so that if the solenoid fails the pawl will be withdrawn from interference with the park gear. In this case, the solenoid is operated to force the pawl toward the park gear during the entire hold period. Alternatively, the pawl is shifted by

action of a spring into interfering contact, and remains in interfering contact until the solenoid is powered to withdraw the pawl, so that battery power is not needed to hold the pawl in interfering contact. Alternatively, the pawl may be unbiased, so that, after being shifted by action of the solenoid into interfering contact, it remains in its interfering position until withdrawn, so that battery power need not be consumed to hold the brake in position (but may be applied to hold the brake in position), and is only applied to shift the pawl into interfering contact with the park gear and withdraw the pawl.

[0037] Various parking pawl mechanisms may be used. As illustrated in Figure 12, another suitable parking pawl mechanism includes the park gear 42, the solenoid plunger 44 and pawl 41 which directly engages the park gear and serves as the pawl. To brake and stop the drive train the control system operates the solenoid to force the pawl into interfering contact with the park gear, and to release the drive train the control system operates the solenoid to withdraw the pawl from the park gear. As illustrated in Figure 13, another suitable parking pawl mechanism includes the park gear 42, a sliding pawl 45, and cam 46. The cam is turned with a rotary solenoid 47, which engages the follower 48 to push the pawl into interfering contact with the park gear. The cam may have an eccentric profile, however the portion of the cam lobe in contact with the follower when the cam is in the locked and/or unlocked position is circular (for example, a non-circular cam lobe with an isodiametric top radius, where a radius of a contact point with the follower is a substantially fixed radius relative to the cam shaft) so that forces applied to the cam by the follower will not cause the cam to rotate. This allows the cam lobe portions associated with locking and unlocking to maintain a stable position. The follower rests on an equal radial segment or

portion of the cam lobe during engagement of the pawl with the park gear to maintain a stable position and minimize disengagement force to release the park gear. If the motor is powered in the locked position, the power required to rotate the cam to unlock the pawl is constant, minimized and/or decreasing. Once the pawl is forced into interfering contact with the park gear, no battery power is required to hold the pawl in interfering contact with the park gear. Power is required to disengage the pawl, but no battery power is required to hold the pawl away from the park gear. The pawls of the braking mechanisms are controlled by the control system, which is further programmed to operate the solenoid to force the pawl into interfering contact with the pawl gear to brake the drive train, and thus hold the compression belt at a set threshold of tightness during a period of the compression cycle, such as the high compression hold period of the compression cycle or the inter-compression hold period of the compression cycle. Once the pawl is forced into interfering contact with the park gear, no battery power is required to hold the pawl in interfering contact with the park gear. Power may be required to disengage the pawl, but no battery power is required to hold the pawl away from the park gear.

[0038] In use, a CPR provider will apply the device to a cardiac arrest victim, and initiate operation of the device. In applying the device, the CPR provider will secure each belt end to its corresponding intermediate belt (or directly to a corresponding drive spool). Initial tightness of the belt is not critical, as the control system will operate to cinch the belt to achieve an appropriate tightness for the start of compressions. After placement of the belt, the CPR provider initiates operation of the device through the control panel. Upon initiation, the control system will first test the tightness of the belt. To accomplish this, the control system is programmed to first loosen the belt (the intermediate

straps (or belt ends) will be set to a position to provide enough band length to accommodate this, and can be initially partially spooled) to ensure that it is slack, then tighten the belt until it sensed that the belt is tight to a first, low threshold of tightness (a slack-take up position or pre-tensioned position). The control system will sense this through a suitable system, such as a current sensor, associating a spike in current drawn by the motor with the slack take-up position. When the belt is tight to the point where any slack has been taken up, the motor will require more current to continue to turn under the load of compressing the chest. The expected rapid increase in motor current draw (motor threshold current draw) is measured through a current sensor, a voltage divider circuit or the like. This spike in current or voltage is taken as the signal that the belt has been drawn tightly upon the patient and the paid-out belt length is an appropriate starting point. (The exact current level which indicates that the motor has encountered resistance consistent with slack take-up will vary depending on the motor used and the mass of the many components of the system.) Where the belt or other system component is fitted with an encoder assembly, an encoder measurement at this point is zeroed within the system (that is, taken as the starting point for belt take-up). The encoder then provides information used by the system to determine the change in length of the belt from this pre-tightened or "pre-tensioned" position.

[0039] Various other means for detecting slack take-up may be used. The control system can also determine the slack-take up position by analyzing an encoder scale on a moving component of the system (associating a slow-down in belt motion with the slack take-up position), a load sensor on the platform (associating a rapid change in sensed load with the

slack take-up position), or with any other means for sensing slack take-up.

[0040] As an alternative mode of operation, the control system can be programmed to initially tighten the belt while detecting the load on the belt through a motor current sensor (or other means for detecting slack take up), and, upon detecting slack take up, such as a load in excess of a predetermined threshold, loosening the belt to slack and then tightening the belt to detect the slack take-up position, or, upon detecting the load below the predetermined threshold, continue to tighten the belt to the slack take-up position. Thus, the device, when modified to accomplish pre-tensioning, can comprise the platform for placement under a thorax of the patient, the compression belt adapted to extend over an anterior chest wall of the patient, a motor operably connected to the belt through a drive train and capable of operating the drive train repeatedly to cause the belt to tighten about the thorax of the patient and loosen about the thorax of the patient; and a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, and said control system is further operable to pre-tension the compression belt, prior to performing the repeated cycles of compression, by operating the motor to loosen the belt, and then operating the motor to tighten the belt until the belt is tightened to a slack take-up position. Also, the control system may be programmed to initially tighten the belt, detect the slack take-up position, and, without the loosening step, proceeding to operate the device to provide CPR chest compressions.

[0041] In each of the operations described in paragraphs 38 through 40, the control system may be programmed such that, upon detection of the slack take-up position, the control system may pause operation of the system to await user input

to initiate compression cycles, or to proceed immediately to initiate compression cycles without further operator input. The benefits of the pre-tensioning operations described in the preceding paragraphs can be achieved in combination with the benefits of additional embodiments described above, including the laterally disposed drive spools and the anterior attachment of the compression belt to the drive spool, or they may be achieved in isolation, such as with chest compression belts comprising a single drive spool attached to a single location on the compression belt, or a single drive spool connected to a motor directly or through a single linkage.

[0042] Once the slack-take up position is achieved, the control system associates the belt position with the slack take-up position. This can be achieved by detecting an encoder position of an encoder, and associating the encoder position with the slack take-up position of the belt, or detecting the position of a compression monitor fixed to the belt and associating this position with the slack take-up position of the belt. If the encoder position is used to track the unspooled length of the belt, which corresponds to the desired compression depth, the control system will be programmed to operate the motor and brake to provide repeated compression cycles which include tightening the belt to a high threshold of tightness (based upon the length of belt spooled on the lateral drive spool, which corresponds to the compression depth achieved), holding the belt tight momentarily at the high, loosening the belt, and holding the belt at the slack take-up position momentarily, where the slack take-up position has been determined in reference to the encoder position. If a compression monitor is used to track the compression depth achieved by the compression device, the control system will be programmed to operate the motor and brake to provide repeated compression cycles which include tightening the belt to a high threshold of tightness (based on

the compression depth as measured by the compression monitor, or determined from signals generated by the compression monitor), holding the belt tight momentarily at the high threshold, loosening the belt, and holding the belt at the slack take-up position momentarily, where the slack take-up position has been determined in reference to the compression monitor zero point which was associated with the slack take-up position.

[0043] Where a compression monitor is used to determine the compression state achieved by the system and provide feedback for control of the system, the compression sensor can comprise an accelerometer based compression monitor such as the compression monitor described in Halperin, et al., CPR Chest Compression Monitor, U.S. Patent 6,390,996 (May 21, 2002), as well as Palazzolo, et al., Method of Determining Depth of Chest Compressions During CPR, U.S. Patent 7,122,014 (Oct. 17, 2006), or the magnetic field based compression monitor described in Centen, et al., Reference Sensor For CPR Feedback Device, U.S. Pub. 2012/0083720 (Apr. 5, 2012). The compression monitor typically includes sensors for generating signals corresponding to the depth of compression achieved during CPR compressions, and associated hardware/control system for determining the depth of compression based on these signals. The components of the compression monitor system may be incorporated into the belt, or the sensors may be incorporated into the belt while the associated hardware and control system are located elsewhere in the device, or integrated into the main control system that operates the compression belt. While controlling the device to perform repeated cycles of compression, the control system may use the compression signals or depth measurement provided by the compression sensor or compression monitor to control operation of the device. The control system can operate to tighten the belt until the depth of compression achieved by the system, as

determined from the compression signals, indicates that the compression belt has pushed the anterior chest wall downward (in the anterior direction, toward the spine) to a desired predetermined compression depth (typically 1.5 to 2.5 inches). The desired depth is predetermined in the sense that it is programmed into the control system, or determined by the control system, or input by an operator of the system).

[0044] The control system may comprise at least one processor and at least one memory including program code with the memory and computer program code configured with the processor to cause the system to perform the functions described throughout this specification. The various functions of the control system may be accomplished in a single computer or multiple computers, and may be accomplished by a general purpose computer or a dedicated computer, and may be housed in the housing or an associated defibrillator.

[0045] While the preferred embodiments of the devices and methods have been described in reference to the environment in which they were developed, they are merely illustrative of the principles of the inventions. The elements of the various embodiments may be incorporated into each of the other species to obtain the benefits of those elements in combination with such other species, and the various beneficial features may be employed in embodiments alone or in combination with each other. Other embodiments and configurations may be devised without departing from the spirit of the inventions and the scope of the appended claims.

We claim:

1. A device for compressing a chest of a patient comprising:

a platform for placement under a thorax of the patient;

a compression belt adapted to extend over an anterior chest wall of the patient, said belt comprising a load distribution section and right belt end and a left belt end;

a motor operably connected to the belt through a drive train, said motor capable of operating the drive train repeatedly to cause the belt to tighten about the thorax of the patient and loosen about the thorax of the patient; wherein

the drive train comprises a right drive spool and a left drive spool, said right drive spool and left drive spool disposed laterally in the platform, and a linkage operably connecting the motor to said right drive spool and left drive spool; and

the right belt end and the left belt end are releasably attachable to the right drive spool and left drive spool, respectively, at attachment points accessible from anterior or lateral sides of the platform, such that the right belt end and left belt end may be attached to the right drive spool and the left drive spool while the platform is disposed under the patient.

2. The device of claim 1, wherein:

the drive train comprises right and left intermediate straps fixed to right and left drive spools, and the right and left belt ends comprise releasable attachment means for releasably attaching the right and left belt ends to the right and left intermediate straps.

3. The device of claim 2, wherein the right and left intermediate straps are substantially self-supporting yet sufficiently flexible that they may be spooled on the right and left drive spools.

4. The device of any of the preceding claims, further comprising right and left splines disposed on the right and left belt ends, and slots in the right and left drive spools for receiving the right and left splines to releasably attach the right and left belt ends to the right and left drive spools.

5. The device of any of the preceding claims, wherein the linkage comprises a drive belt operably connecting the motor to the right drive spool and a drive belt operably connecting the motor to the left drive spool.

6. The device of any of the preceding claims, wherein the linkage comprises a drive chain operably connecting the motor to the right drive spool and a drive chain operably connecting the motor to the left drive spool.

7. The device of any of the preceding claims, wherein the drive train comprises a first drive shaft connected to the motor, a sun gear disposed on the drive shaft, with said sun gear engaging a planetary gear which is fixed to a second drive shaft, a first drive belt, drive chain, rack or strap connecting the first drive shaft to one of the left and right drive spools, and a second drive belt, drive chain, rack or strap connecting the second drive shaft to the other of the left and right drive spools.

8. The device of any of the preceding claims, wherein the drive train comprises a first drive shaft connected to the motor, a first drive belt, drive chain or rack connecting the first drive shaft to one of the left and right drive spools, and a second drive belt, drive chain or rack connecting the

first drive shaft to the other of the left and right drive spools.

9. The device of any of the preceding claims, further comprising a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, and said control system is further operable to pre-tension the compression belt, prior to performing the repeated cycles of compression, by operating the motor to loosen the belt, and then operating the motor to tighten the belt until the belt is tightened to a slack take-position.

10. The device of any of the preceding claims, further comprising a compression monitor with sensors secured to the compression belt, said compression monitor operable to determine the depth of compression achieved by the chest compression device, wherein the control system is further programmed to control operation of the compression belt based on the chest compression depth determined by the compression monitor.

11. The device of claim 10, wherein the control system is further programmed to control operation of the compression belt to achieve a predetermined compression depth as determined by the compression monitor.

12. The device of any of the preceding claims wherein the platform is characterized by an inferior/superior axis corresponding to the inferior/superior axis of a patient on which the device is used, and characterized by a medial/lateral axis corresponding to the medial/lateral axis of a patient on which the device is used, wherein:

the motor and drive train are disposed in a first region of the device along the inferior/superior axis, and the drive spools extend into a second region of the device

along the inferior/superior axis, said second region displaced from the first region and located inferiorly to the first region, and the drive spools are spaced laterally from the inferior/superior centerline of the device, thereby defining a radiolucent space within the housing devoid of radiopaque components;

such that said radiolucent space is disposed, when the device is installed under a patient with the compression belt spanning the anterior chest wall of the patient, under the heart of the patient.

13. The device of claim 1, wherein the drive spools have a first segment engaging the linkage, and a second segment, extending inferiorly from the first segment, which engages the belt ends, defining a space between the drive spools, on a coronal plane and inferior to the belt which is unoccupied by drive train components.

14. A method of performing chest compression on a patient, said method comprising the steps of:

providing a device for compressing a chest of a patient, said device comprising:

a platform for placement under a thorax of the patient;

a compression belt adapted to extend over an anterior chest wall of the patient, said belt comprising a load distribution section and right and left belt ends;

a drive train operably connected to the belt for repeatedly tightening and loosening the belt around the chest of the patient;

a motor operably connected to the belt through a drive train, said motor capable of operating the drive train repeatedly to cause the belt to tighten about the

thorax of the patient and loosen about the thorax of the patient; wherein

the drive train comprises a right drive spool and a left drive spool, said right drive spool and left drive spool disposed laterally in the housing, and a linkage operably connecting the motor to said right drive spool and left drive spool; and

the right belt end and the left belt end are releasably attachable to the right drive spool and left drive spool, respectively, at attachment points accessible from anterior or lateral sides of the platform, such that the right belt end and left belt end may be attached to the right drive spool and the left drive spool while the platform is disposed under the patient;

placing the patient on the platform, with the anterior side of the platform in contact with the thorax of the patient;

thereafter, while the patient is disposed on the platform, attaching the right belt end to the right drive spool, and attaching the left belt end to the left drive spool; and

initiating operation of the device to cause repeated cycles of tightening and loosening of the belt about the thorax of the patient.

15. The method of claim 14 further comprising the steps of:

manually tightening the belt about the thorax of the patient to an initial tightness; and

operating the device to loosen the belt to ensure that the belt is slack, and thereafter tightening the belt to a first, low threshold of tightness, and associating

the position of the belt with a slack-take up position, and thereafter operating the device to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, while detecting the depth of compressions achieved by the belt with a compression sensor secured to the compression belt.

Remove compression sensor stuff. Convert to method

16. The method of claim 15 further comprising the steps of:

providing a depth compression sensor fixed to the compression belt and operable to generate compression signals corresponding the depth of compression achieved by the compression belt; and

operating the motor to achieve chest compressions of a predetermined depth as determined from the compression signals.

17. The method of claim 15 further comprising the steps of:

operating the device to limit loosening of the compression belt between compressions to the slack take-up position.

18. A method of claim 14 further comprising the steps of:

interrupting operation of the device to replace the belt, detaching the right belt end from the right drive spool, and detaching the left belt end from the left drive spool, while the patient remains on the platform.

19. A device for compressing a chest of a patient comprising:

a platform for placement under a thorax of the patient, characterized by an anterior/posterior axis corresponding to the anterior/posterior axis of a

patient on which the device is used, and characterized by an inferior/superior axis corresponding to the inferior/superior axis of a patient on which the device is used;

a compression belt adapted to extend over an anterior chest wall of the patient, said belt comprising a load distribution section, and right and left belt ends;

right and left drive spools laterally displaced from an inferior/superior centerline of the platform, said right and left drive spools operably connected to the right and left belt ends such that rotation of the right and left drive spools results in pulling the right and left belt ends posteriorly, for repeatedly tightening and loosening the belt around the chest of the patient;

a motor operably connected to the right and left drive spools, through a drive train, said motor operable to rotate the right and left drive spools.

20. The device of claim 19 wherein the drive train comprises:

a first drive belt, drive chain, rack or strap connecting a first drive shaft to one of the left and right drive spools, and a second drive belt, drive chain, rack or strap connecting a second drive shaft to the other of the left and right drive spools.

21. The device of claim 19, wherein:

the drive train comprises right and left intermediate straps fixed to right and left drive spools and the right and left belt ends.

23. The device of claim 21, wherein the right and left intermediate straps are substantially self-supporting yet

sufficiently flexible that they may be spooled on the right and left drive spools.

24. The device of claim 19, wherein the drive train comprises a first drive shaft connected to the motor, a sun gear disposed on the drive shaft, with said sun gear engaging a planetary gear which is fixed to a second drive shaft, a first drive belt, drive chain, rack or strap connecting the first drive shaft to one of the left and right drive spools, and a second drive belt, drive chain, rack or strap connecting the second drive shaft to the other of the left and right drive spools.

25. The device of any of claims 21 through 24, further comprising a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, and said control system is further operable to pre-tension the compression belt, prior to performing the repeated cycles of compression, by operating the motor to loosen the belt, and then operating the motor to tighten the belt until the belt is tightened to a slack take-position.

26. The device of any of claims 21 through 25, further comprising a compression monitor with sensors secured to the compression belt, said compression monitor operable to determine the depth of compression achieved by the chest compression device, wherein the control system is further programmed to control operation of the compression belt based on the chest compression depth determined by the compression monitor.

27. The device of 26, wherein the control system is further programmed to control operation of the compression belt to achieve a predetermined compression depth as determined by the compression monitor.

28. The device of any of claims 21 through 27 wherein the platform is characterized by an inferior/superior axis corresponding to the inferior/superior axis of a patient on which the device is used, and characterized by a medial/lateral axis corresponding to the medial/lateral axis of a patient on which the device is used, wherein:

the motor and drive train are disposed in a first region of the device along the inferior/superior axis, and the drive spools extend into a second region of the device along the inferior/superior axis, said second region displaced from the first region and located inferiorly to the first region, and the drive spools are spaced laterally from the inferior/superior centerline of the device, thereby defining a radiolucent space within the housing devoid of radiopaque components;

such that said radiolucent space is disposed, when the device is installed under a patient with the compression belt spanning the anterior chest wall of the patient, under the heart of the patient.

29. The device of any of claims 21 through 28, wherein the drive spools have a first segment engaging the linkage, and a second segment, extending inferiorly from the first segment, which engages the belt ends, defining a space between the drive spools, on a coronal plane and inferior to the belt which is unoccupied by drive train components.

30. The device of claim 1, wherein:

one of the belt ends is connected to the load distribution section and is adapted for direct connection to a drive spool, and

the other of the belt ends is releasably coupled to the load distribution section and is adapted for connection to a drive spool.

31. A device for compressing a chest of a patient comprising:

a platform for placement under a thorax of the patient;

a compression belt adapted to extend over an anterior chest wall of the patient;

a motor operably connected to the belt through a drive train, said motor capable of operating the drive train repeatedly to cause the belt to tighten about the thorax of the patient and loosen about the thorax of the patient; wherein

a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, wherein said control system is further operable to pre-tension the compression belt, prior to performing the repeated cycles of compression, by operating the motor to loosen the belt, and then operating the motor to tighten the belt until the belt is tightened to a slack take-up position.

32. The device of claim 31 wherein:

the drive train comprises a right drive spool and a left drive spool and a linkage operably connecting the motor to said right drive spool and left drive spool.

33. The device of claim 31 wherein:

the belt comprises a right belt end and a left belt end;

the drive train comprises a right drive spool and a left drive spool, said right drive spool and left drive spool disposed laterally in the platform, and a linkage operably connecting the motor to said right drive spool and left drive spool; and

the right belt end and the left belt end are releasably attachable to the right drive spool and left drive spool, respectively, at attachment points accessible from anterior or lateral sides of the platform, such that the right belt end and left belt end may be attached to the right drive spool and the left drive spool while the platform is disposed under the patient.

34. The device of claim 31, wherein:

the drive train comprises right and left intermediate straps fixed to right and left drive spools, and the right and left belt ends comprise releasable attachment means for releasably attaching the right and left belt ends to the right and left intermediate straps.

35. The device of claim 34, wherein the right and left intermediate straps are substantially self-supporting yet sufficiently flexible that they may be spooled on the right and left drive spools.

36. The device of any of the preceding claims 31 through 35, further comprising right and left splines disposed on the right and left belt ends, and slots in the right and left drive spools for receiving the right and left splines to releasably attach the right and left belt ends to the right and left drive spools.

37. The device of any of the preceding claims 31 through 36, wherein the linkage comprises a drive belt operably connecting

the motor to the right drive spool and a drive belt operably connecting the motor to the left drive spool.

38. The device of any of the preceding claims 31 through 36, wherein the linkage comprises a drive chain operably connecting the motor to the right drive spool and a drive chain operably connecting the motor to the left drive spool.

39. The device of any of the preceding claims 31 through 36, wherein the drive train comprises a first drive shaft connected to the motor, a sun gear disposed on the drive shaft, with said sun gear engaging a planetary gear which is fixed to a second drive shaft, a first drive belt, drive chain, rack or strap connecting the first drive shaft to one of the left and right drive spools, and a second drive belt, drive chain, rack or strap connecting the second drive shaft to the other of the left and right drive spools.

40. The device of any of the preceding claims 31 through 36, wherein the drive train comprises a first drive shaft connected to the motor, a first drive belt, drive chain or rack connecting the first drive shaft to one of the left and right drive spools, and a second drive belt, drive chain or rack connecting the first drive shaft to the other of the left and right drive spools.

41. The device of any of the preceding claims 31 through 40, wherein:

the control system is further programmed to initially tighten the belt while detecting a load on the belt in excess of a predetermined threshold, loosen the belt to slack and then tighten the belt to detect the slack take-up position.

42. The device of any of the preceding claims 31 through 41, wherein:

the control system is further programmed to initially tighten the belt while detecting the load on the belt, and, upon detecting the load below the predetermined threshold, continue to tighten the belt to the slack take-up position.

43. A device for compressing a chest of a patient comprising:

a platform for placement under a thorax of the patient;

a compression belt adapted to extend over an anterior surface of the chest of the patient;

a drive train operably connected to the belt for repeatedly tightening and loosening the belt around the chest of the patient;

a motor operably connected to the drive train, said motor capable of operating the drive train to cause the belt to tighten about the chest of the patient and loosen about the chest of the patient in repeated compression cycles;

a brake for stopping and holding the drive train during a compression cycle, said brake comprising a park gear non-rotatably fixed to a rotating component of the drive train or motor, and a parking pawl disposed in relation to the park gear such that it can be moved into interfering contact with the park gear during a compression cycle.

44. The device of claim 43 wherein:

the rotating component is a drive shaft driven by the motor.

45. The device of any of claims 43 through 44 further comprising:

a solenoid operably fixed to the pawl, said solenoid operable to force the pawl into interfering contact with the park gear; and

a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, wherein the control system is further operable to force the pawl into interfering contact with the park gear, and to withdraw the pawl from the park gear, to provide hold periods during the cycles of compression.

46. The device of any of claims 43 through 45 wherein:

the pawl is spring biased away from the park gear.

47. The device of any of claims 43 through 45 wherein:

the pawl is spring biased into interfering contact with the park gear; and the device further comprises

a solenoid operably fixed to the pawl, said solenoid operable to withdraw the pawl from interfering contact with the park gear; and

a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, wherein the control system is further operable to withdraw the pawl from interfering contact with the park gear.

48. The device of any of claims 43 through 47 wherein:

the pawl is a sliding pawl; and the device further comprises:

a cam having an eccentric profile, said cam operable to force the pawl into interfering contact with the park gear; and

a control system operable to control operation of the motor to tighten and loosen the compression belt in repeated cycles of compression about the thorax of the patient, and said control system is further operable to operate the cam to force the pawl into interfering contact with the park gear.

49. The device of claim 48 wherein:

the cam has an isodiametric top radius.

50. The device of claim 48 through 49 further comprising:

a rotary solenoid operably connected to the cam, wherein the control system is operable to rotate the rotary solenoid in order to operate the cam.

51. A device for compressing a chest of a patient comprising:

a platform for placement under a thorax of the patient;

a compression belt adapted to extend over an anterior surface of the chest of the patient, said belt comprising right and left belt ends;

right and left drive spools laterally displaced from an inferior/superior centerline of the platform, said right and left drive spools operably connected to the right and left belt ends such that rotation of the

right and left drive spools results in spooling of the right and left belt ends upon the corresponding drive spool, for repeatedly tightening and loosening the belt around the chest of the patient;

a motor operably connected to the right and left drive spools, through a drive train, said motor operable to rotate the right and left drive spools;

wherein the platform is characterized by an inferior/superior axis corresponding to the inferior/superior axis of a patient on which the device is used, and an inferior/superior centerline, and characterized by a medial/lateral axis corresponding to the medial/lateral axis of a patient on which the device is used, wherein:

the motor and drive train are disposed in a first region of the device along the inferior/superior axis, and the drive spools extend into a second region of the device along the inferior/superior axis, said second region displaced from the first region, and the drive spools are spaced laterally from the inferior/superior centerline of the device, thereby defining a radiolucent space within the housing devoid of radiopaque components;

such that said radiolucent space is disposed, when the device is installed under a patient with the compression belt spanning the anterior surface of the chest of the patient, under the heart of the patient.

1/5

FIG. 1

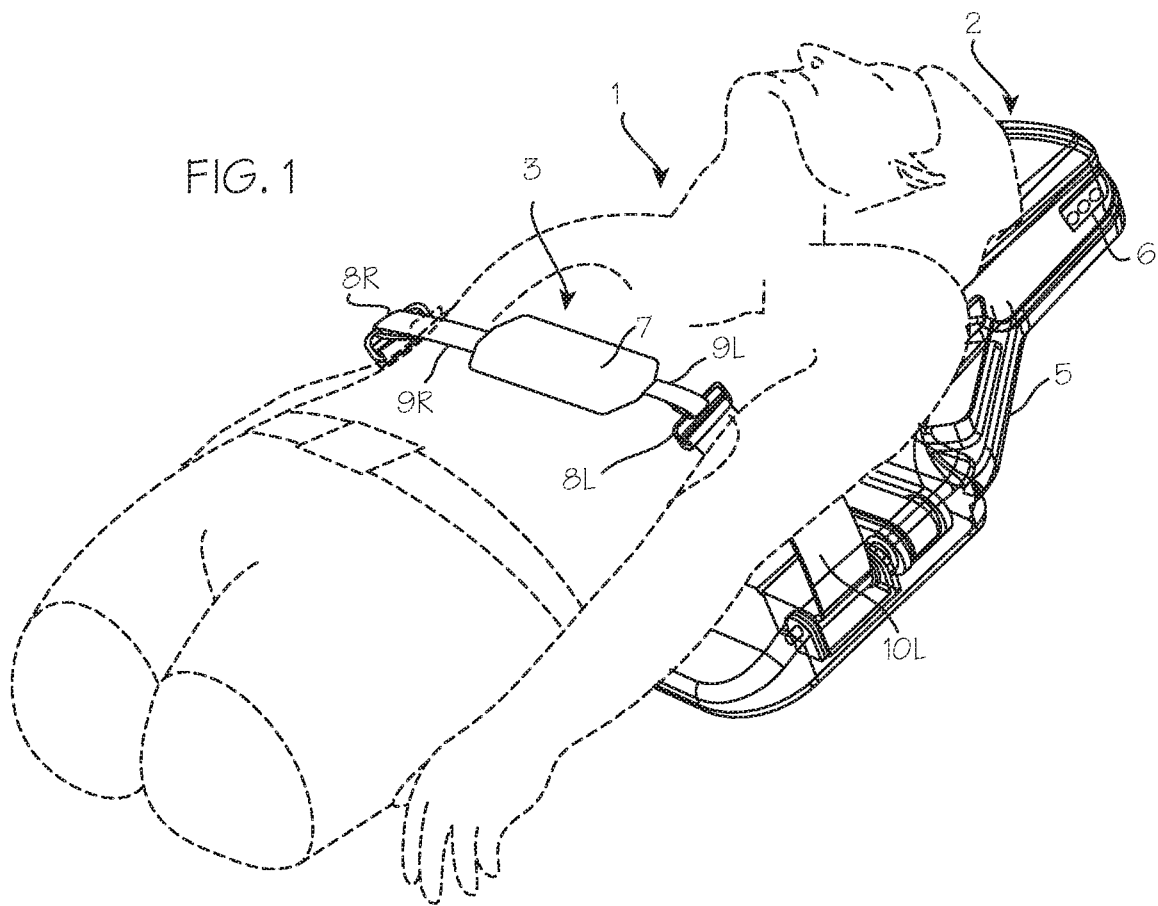


FIG. 2

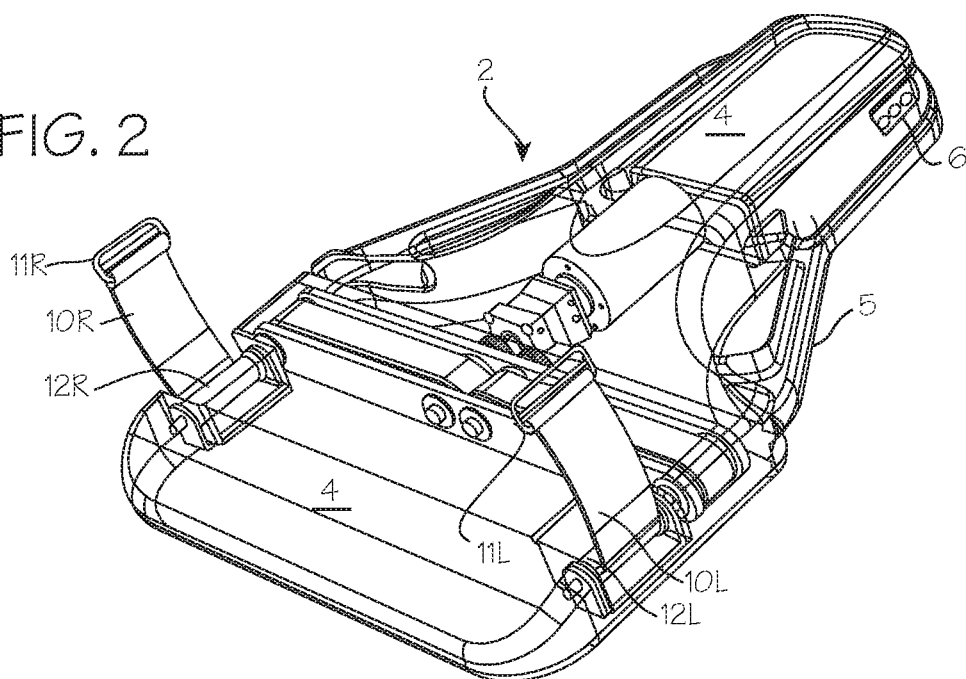


FIG. 3

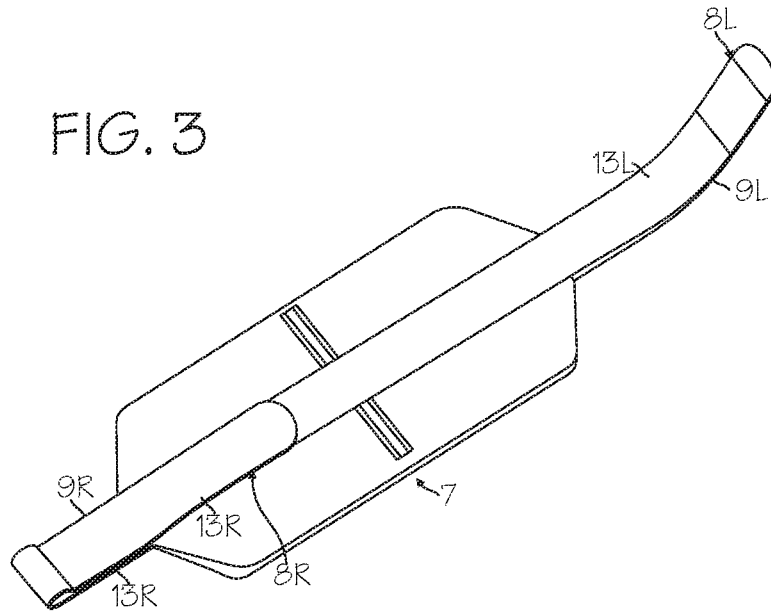


FIG. 4

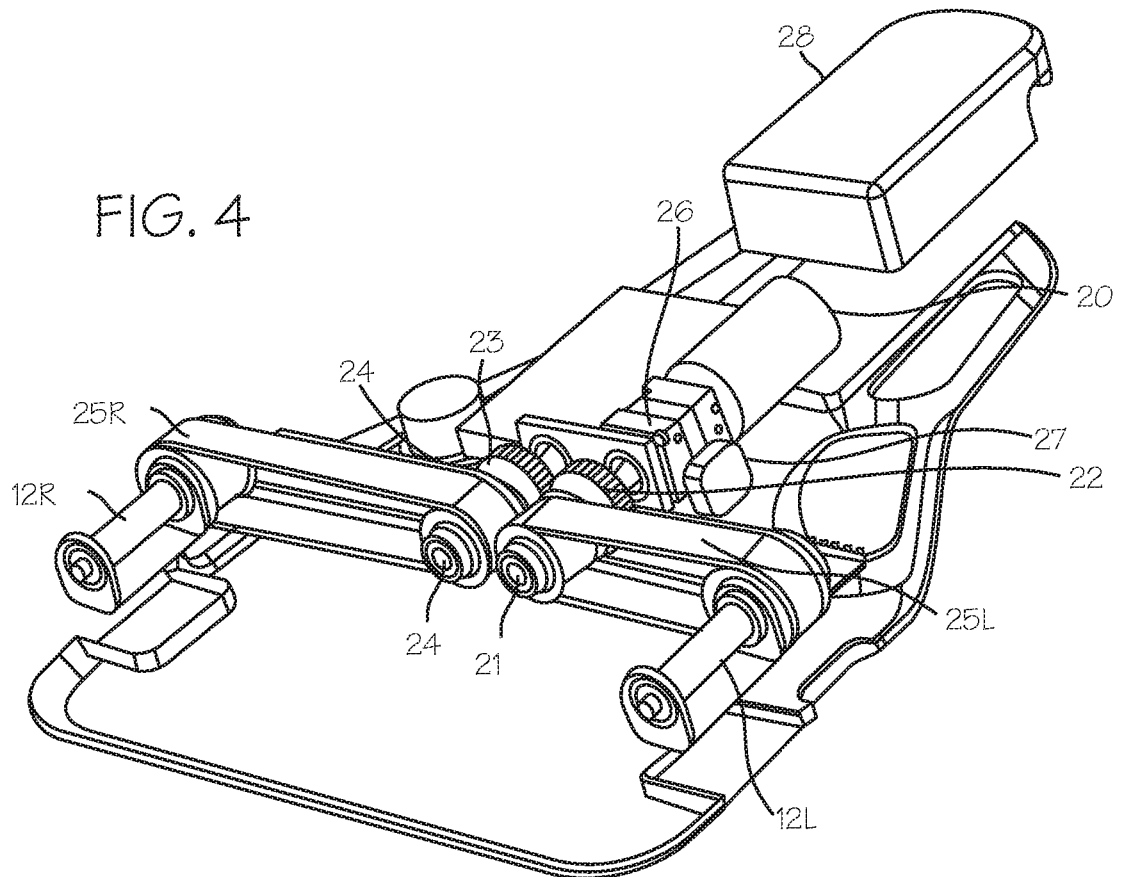


FIG. 5

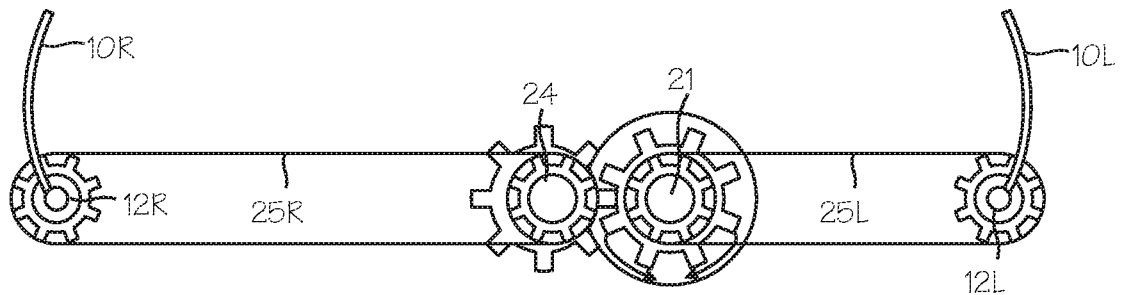


FIG. 6

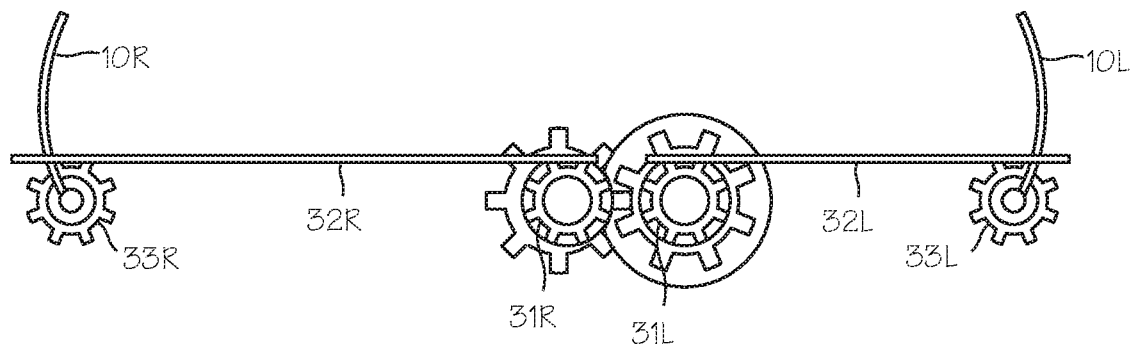


FIG. 7

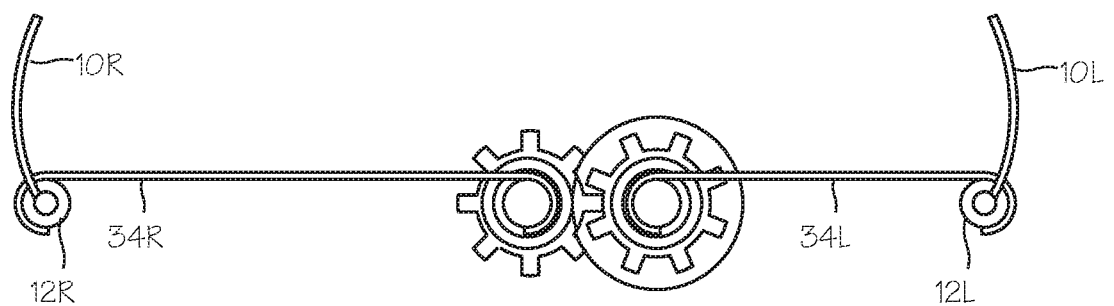


FIG. 8

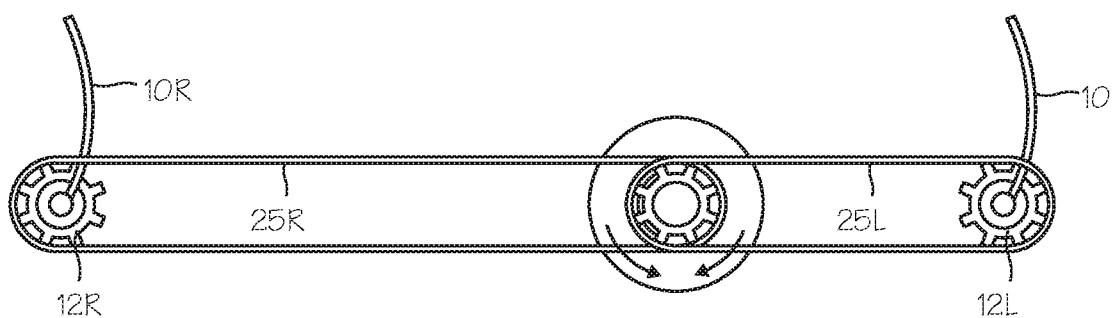


FIG. 9

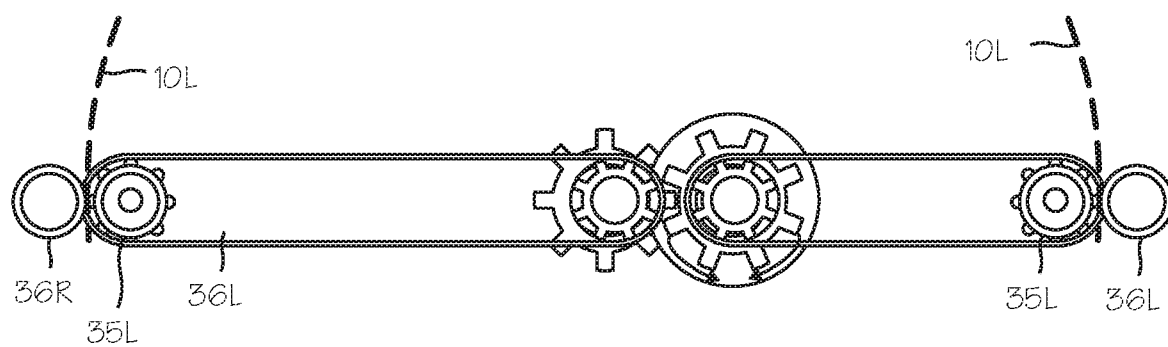


FIG. 10

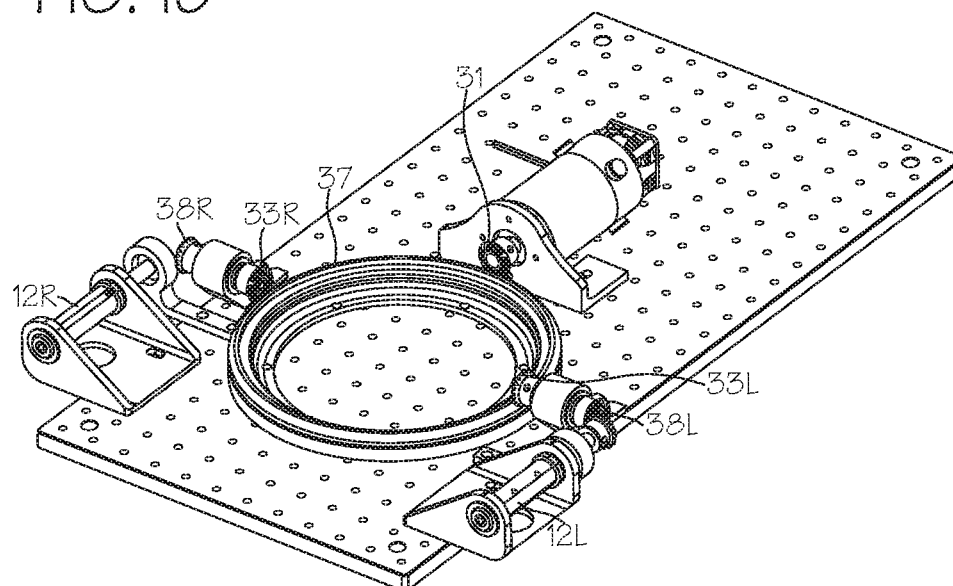


FIG. 11

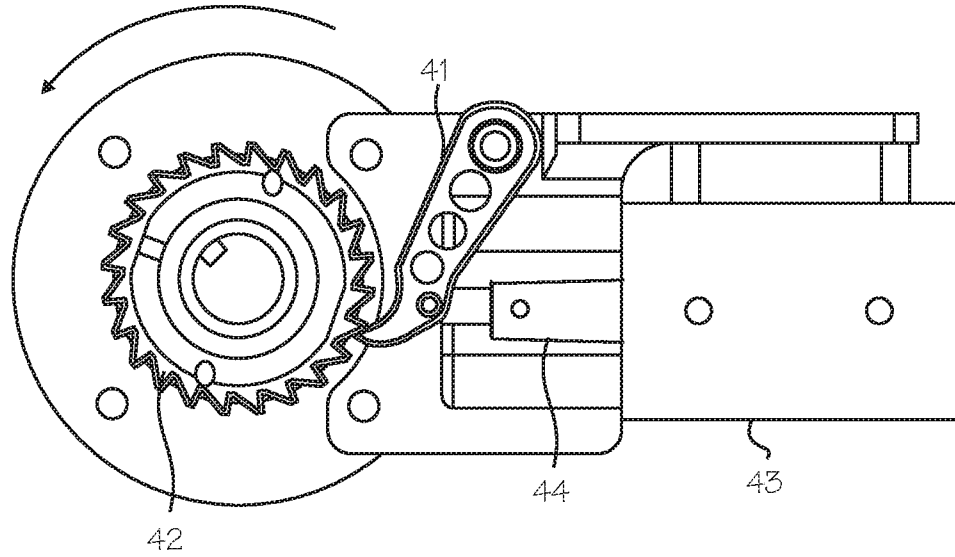


FIG. 12


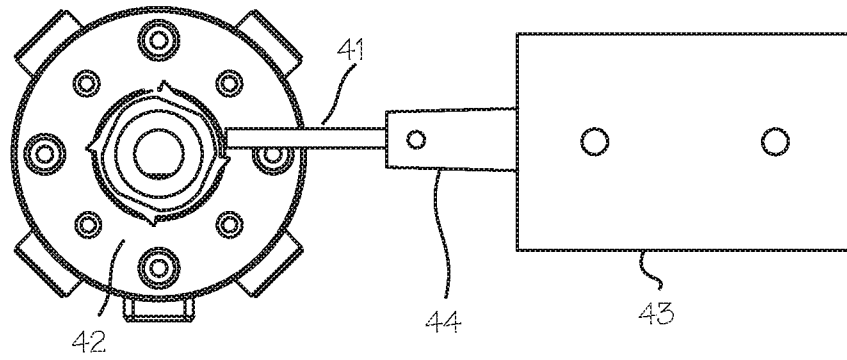


FIG. 13

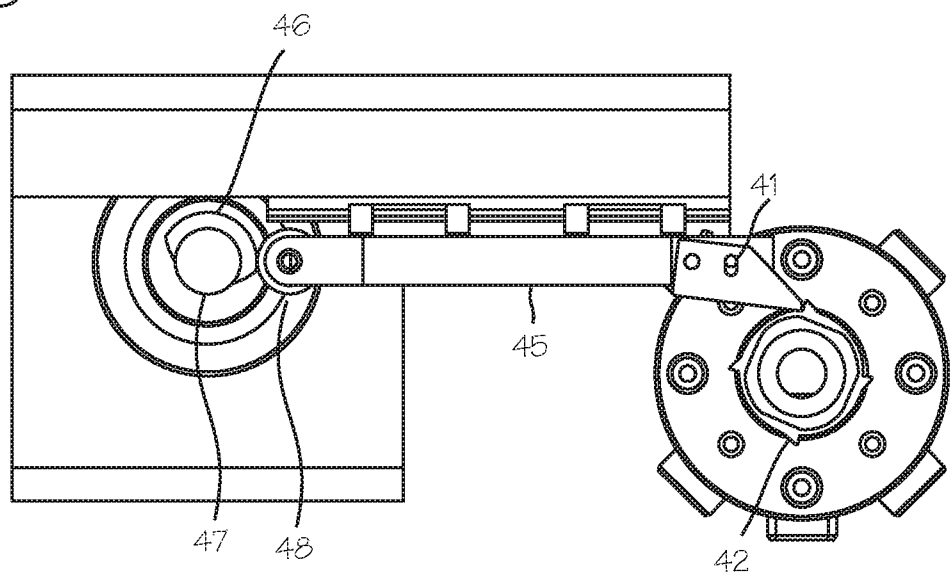

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2016/057198**A. CLASSIFICATION OF SUBJECT MATTER****A61H 31/00(2006.01)i, A61B 5/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHEDMinimum documentation searched (classification system followed by classification symbols)
A61H 31/00; A61B 5/00Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
Korean utility models and applications for utility models
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)
eKOMPASS(KIPO internal) & keywords: chest compression, motor, drive spool, belt, tight, loose, repeat, brake, radiolucent**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2014-0236054 A1 (ZOLL CIRCULATION, INC.) 21 August 2014 See claims 1-9; figures 1-8.	1-4, 13, 19-21, 23-25 , 30-36, 43-45, 51
A	US 8062239 B2 (SHERMAN, D. R. et al.) 22 November 2011 See claims 1-10; figures 1-12b.	1-4, 13, 19-21, 23-25 , 30-36, 43-45, 51
A	US 8641647 B2 (ILLINDALA, U. K. V. et al.) 04 February 2014 See claims 1-14; column 5, lines 15-16.	1-4, 13, 19-21, 23-25 , 30-36, 43-45, 51
A	US 6869408 B2 (SHERMAN, D. R. et al.) 22 March 2005 See entire document.	1-4, 13, 19-21, 23-25 , 30-36, 43-45, 51
A	US 2008-0146975 A1 (HO, C. H. et al.) 19 June 2008 See entire document. *Note: Claim 22 is missing in this application.	1-4, 13, 19-21, 23-25 , 30-36, 43-45, 51



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

09 February 2017 (09.02.2017)

Date of mailing of the international search report

16 February 2017 (16.02.2017)

Name and mailing address of the ISA/KR

International Application Division

Korean Intellectual Property Office

189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea



Facsimile No. +82-42-481-8578

Authorized officer

CHO, Ki Yun

Telephone No. +82-42-481-5655



Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 14-18
because they relate to subject matter not required to be searched by this Authority, namely:
Claims 14-18 pertain to methods for treatment of the human body and thus relate to a subject-matter which this International Searching Authority is not required to search under PCT Article 17(2)(a)(i) and PCT Rule 39.1(iv).
2. ☒ Claims Nos.: 11,27,49
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
Claims 11,27,49 directly or indirectly refer to one of the unsearchable claims which do not comply with PCT Rule 6.4(a).
3. ☒ Claims Nos.: 5-10,12,26,28-29,37-42,46-48,50
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2016/057198

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2014-0236054 A1	21/08/2014	US 2005-0080363 A1 US 2008-0045867 A1 US 2010-0174216 A1 US 2014-0309564 A1 US 7270639 B2 US 9398998 B2	14/04/2005 21/02/2008 08/07/2010 16/10/2014 18/09/2007 26/07/2016
US 8062239 B2	22/11/2011	AU 2003-271345 A1 AU 2003-271345 B2 AU 2006-230724 A1 AU 2009-200833 A1 AU 2009-200833 B2 AU 2011-201820 A1 AU 2011-201820 B2 CA 2333510 A1 CA 2588503 A1 CA 2775937 A1 EP 1091721 A1 EP 1091721 B1 EP 1929988 A2 EP 1929988 A3 EP 1929988 B1 EP 2298268 A2 EP 2298268 A3 JP 2003-520053 A JP 2009-183723 A JP 4375903 B2 US 2002-0156401 A1 US 2004-0193076 A1 US 2008-0300516 A1 US 2012-0130290 A1 US 2014-0221884 A1 US 6066106 A US 6398745 B1 US 6709410 B2 US 7374548 B2 US 8690805 B2 WO 99-62458 A1	29/01/2004 20/07/2006 09/11/2006 19/03/2009 20/01/2011 19/05/2011 14/06/2012 09/12/1999 09/12/1999 09/12/1999 18/04/2001 23/01/2008 11/06/2008 21/01/2009 13/07/2011 23/03/2011 22/06/2011 02/07/2003 20/08/2009 02/12/2009 24/10/2002 30/09/2004 04/12/2008 24/05/2012 07/08/2014 23/05/2000 04/06/2002 23/03/2004 20/05/2008 08/04/2014 09/12/1999
US 8641647 B2	04/02/2014	EP 2755622 A1 JP 2014-526949 A US 2013-0072830 A1 US 2014-0155793 A1 WO 2013-040470 A1	23/07/2014 09/10/2014 21/03/2013 05/06/2014 21/03/2013
US 6869408 B2	22/03/2005	EP 1131036 A1 EP 1131036 B1 EP 1685820 A1 EP 1685820 B1	12/09/2001 05/04/2006 02/08/2006 15/09/2010

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2016/057198

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		JP 2002-529150 A	10/09/2002
		JP 4276788 B2	10/06/2009
		US 2003-0009115 A1	09/01/2003
		US 2005-0165335 A1	28/07/2005
		US 2009-0069726 A1	12/03/2009
		US 6447465 B1	10/09/2002
		US 7166082 B2	23/01/2007
		US 7722554 B2	25/05/2010
		WO 00-27336 A1	18/05/2000
US 2008-0146975 A1	19/06/2008	US 2013-0079688 A1	28/03/2013
		US 8337436 B2	25/12/2012
		US 9155678 B2	13/10/2015

专利名称(译)	自动胸部按压设备		
公开(公告)号	EP3362026A4	公开(公告)日	2019-03-27
申请号	EP2016856350	申请日	2016-10-14
[标]申请(专利权)人(译)	佐尔循环公司		
申请(专利权)人(译)	ZOLL循环, INC.		
当前申请(专利权)人(译)	ZOLL循环, INC.		
[标]发明人	JOSHI NIKHIL S HARRIS MELANIE L REYNOLDS BYRON J		
发明人	JOSHI, NIKHIL, S. HARRIS, MELANIE, L. REYNOLDS, BYRON, J.		
IPC分类号	A61H31/00 A61B5/00		
CPC分类号	A61H31/005 A61H31/006 A61H2011/005 A61H2201/018 A61H2201/1445 A61H2201/1604 A61H2201/1623 A61H2201/501 A61H2201/5043 A61H2201/5061 A61H2201/5064		
代理机构(译)	POTTER CLARKSON LLP		
优先权	14/885952 2015-10-16 US		
其他公开文献	EP3362026A1		
外部链接	Espacenet		

摘要(译)

一种用于压缩心脏骤停受害者胸部的装置。