



(11) **EP 3 441 937 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
22.04.2020 Bulletin 2020/17

(51) Int Cl.:
G06T 7/00 (2017.01) **A61B 5/00** (2006.01)
A61B 5/042 (2006.01) **A61B 5/055** (2006.01)

(21) Application number: **17382559.7**

(22) Date of filing: **08.08.2017**

(54) **A COMPUTER IMPLEMENTED METHOD FOR CALCULATING VALUES INDICATIVE FOR THE LOCAL SPATIAL STRUCTURE OF CONDUCTING PROPERTIES OF HEART MUSCLE TISSUE AND COMPUTER PROGRAMS THEREOF**

COMPUTERIMPLEMENTIERTES VERFAHREN ZUR BERECHNUNG VON WERTEN, DIE AUF DIE LOKALE RÄUMLICHE STRUKTUR VON LEITENDEN EIGENSCHAFTEN VON HERZMUSKELGEWEBE HINWEISEN, UND COMPUTERPROGRAMME DAFÜR

PROCÉDÉ? MIS EN OEUVRE PAR ORDINATEUR POUR CALCULER DES VALEURS INDICATIVES DE LA STRUCTURE SPATIALE LOCALE DE PROPRIÉTÉS CONDUCTRICES DES TISSUS DU MUSCLE CARDIAQUE ET PROGRAMMES INFORMATIQUES ASSOCIÉS

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(43) Date of publication of application:
13.02.2019 Bulletin 2019/07

(73) Proprietors:
• **ADAS3D MEDICAL, SL**
08036 Barcelona (ES)
• **Hospital Clínic de Barcelona**
08036 Barcelona (ES)

(72) Inventors:
• **STEGHÖFER, Martin**
08009 Barcelona (ES)
• **SERRA DEL MOLINO, Luis**
08035 Barcelona (ES)
• **PLANES CID, Javier**
25005 Lleida (ES)
• **BERRUEZO SÁNCHEZ, Antonio**
08017 Barcelona (ES)

(74) Representative: **Juncosa Miró, Jaime et al**
Torner, Juncosa i Associats, S.L.
Gran Via de les Corts
Catalanes, 669 bis, 1^o, 2^a
08013 Barcelona (ES)

(56) References cited:
EP-A1- 2 755 185 WO-A1-2016/014949

- **SERRA L ET AL: "Identification of border-zone corridors in the left ventricle using the core expansion method", PROCEEDINGS OPTICAL DIAGNOSTICS OF LIVING CELLS II, SPIE, US, vol. 10160, 26 January 2017 (2017-01-26), pages 1016011-1016011, XP060081653, ISSN: 0277-786X, DOI: 10.1117/12.2255817 ISBN: 978-1-5106-1354-6**
- **Kivanc Yalin ET AL: "Cardiac Magnetic Resonance for Ventricular Arrhythmia Therapies in Patients with Coronary Artery Disease Corresponding Author", Journal of Atrial Fibrillation, July 2015 (2015-07), XP055416348, Retrieved from the Internet: URL: <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC5135117/pdf/jafib-08-01242.pdf> [retrieved on 2017-10-17]**
- **J. FERNANDEZ-ARMENTA ET AL: "Three-Dimensional Architecture of Scar and Conducting Channels Based on High Resolution ce-CMR: Insights for Ventricular Tachycardia Ablation", CIRCULATION: ARRHYTHMIA AND ELECTROPHYSIOLOGY, vol. 6, no. 3, 17 May 2013 (2013-05-17), pages 528-537, XP055152264, ISSN: 1941-3149, DOI: 10.1161/CIRCEP.113.000264**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 3 441 937 B1

Description**Technical Field**

5 **[0001]** The present invention is directed, in general, to methods for characterizing heart muscle tissue. In particular, the invention relates to a computer implemented method, and computer programs thereof, for calculating values indicative for the local spatial structure of conducting properties of heart muscle tissue.

Background of the Invention

10 **[0002]** When heart muscle tissue becomes fibrotic due to a heart attack, myocardopathy or any other reason, it changes its electrical conducting properties. This conductivity (how diseased cells are organized in the heart, that is, the resulting topological and morphological structure of the fibrotic tissue) is important to understand arrhythmias. Having an idea of the conductivity of a patient's heart tissue in a minimally invasive way (a scan) is key to help to decide on its treatment.

15 **[0003]** Obtaining a 3D data of the heart muscle is possible using MRI, CT, echography, nuclear imaging, electroanatomical mapping, or other image acquisition technologies.

[0004] There are known some patent application in this field.

20 **[0005]** US-A1-2017178403 provides a system for computational localization of fibrillation sources. In some implementations, the system performs operations comprising generating a representation of electrical activation of a patient's heart and comparing, based on correlation, the generated representation against one or more stored representations of hearts to identify at least one matched representation of a heart. The operations can further comprise generating, based on the at least one matched representation, a computational model for the patient's heart, wherein the computational model includes an illustration of one or more fibrillation sources in the patient's heart. Additionally, the operations

25 can comprise displaying, via a user interface, at least a portion of the computational model.

[0006] US-A1-2017068796 discloses a method and system for simulating patient-specific cardiac electrophysiology including the effect of the electrical conduction system of the heart. A patient-specific anatomical heart model is generated from cardiac image data of a patient.

30 **[0007]** The electrical conduction system of the heart of the patient is modeled by determining electrical diffusivity values of cardiac tissue based on a distance of the cardiac tissue from the endocardium. A distance field from the endocardium surface is calculated with sub-grid accuracy using a nested-level set approach. Cardiac electrophysiology for the patient is simulated using a cardiac electrophysiology model with the electrical diffusivity values determined to model the Purkinje network of the patient.

35 **[0008]** EP-A2-2672889 discloses a method of planning a patient-specific cardiac procedure including receiving three-dimensional imaging data of a patient's heart, simulating at least one of electrophysiological or electromechanical activity of at least a portion of the patient's heart using the three-dimensional imaging data, and planning the patient-specific cardiac procedure based on the simulating. The cardiac procedure is for providing a preselected alteration of at least one of electrophysiological or electromechanical behavior of the patient's heart.

40 **[0009]** EP-B1-2950270 discloses a computer implemented method for identifying channels from representative data in a 3D volume. The method comprises identifying, in a 3D volume, a zone of a first type (H) and a zone of a second type (BZ) and: automatically identifying as a candidate channel (bz) a path running through the zone of a second type (BZ) and extending between two points of the zone of a first type (H); and automatically performing, on a topological space (H_and_BZ_topo), homotopic operations between the candidate channel (bz) and paths (h) running only through the zone of a first type (H), and if the result of said homotopic operations is that the candidate channel (bz) is not

45 homotopic to any path running only through the zone of a first type (H) identifying the candidate channel (bz) as a constrained channel.

[0010] Regarding non-patent literature, L. Serra et al., "Identification of border-zone corridors in the left ventricle using the Core Expansion method," 12th Int. Symposium on Medical Information Processing and Analysis, Pro. of SPIE vol. 10160, 2017, discloses a method for automatic identification of border-zone corridors in MRI images for tachycardia ablation, with classification of tissues into 3 different types and use of iterative morphological operations to expand the core/scar of infarcted tissue to identify the closest border-zone to the scar, prone to contain conductive re-entrant channels.

50 **[0011]** There is a need for an automated method to obtain the structure of the fibrosis of the muscle using 3D medical images or data acquired via an acquisition technology in order to provide a basis with which to identify the arrhythmic substrate. This is useful to stratify patients according to the condition of their hearts from cardiac MRI, to decide on their treatment (for example to establish their responsiveness to an implantable defibrillator or to plan catheter ablation procedures).

55 **[0012]** Cardiac arrhythmias are caused by slow-conducting electrical circuits that use the abnormal structure of the

myocardium that results from disease or infarction. The slow conduction of the electrical circuits is responsible for an electrical wave that is out of sync with the main wave responsible for the contraction of the ventricle. The asynchronous wave disrupts the healthy contraction of the myocardium, and this generates arrhythmia.

[0013] These electrical circuits join areas of healthy tissue and run through corridors within, see Fig. 1, Border-Zone (BZ) tissue (these corridors will be referred as re-entrant Conducting Channels or CC). In order for the slow wave to propagate and disrupt the main electrical activity, it needs to run through conducting tissue embedded within electrically isolating tissue. This tissue can be either scar *core* (dead myocytes that no longer conduct), or the *wall of the endocardium and epicardium*, and/or the *mitral valve*. The electrical isolation has to fulfill several characteristics in order to be the basis of a wave for a CC:

- It needs to run for a minimum distance to allow sufficient time to have passed so that the main electrical wave has passed and the healthy myocytes are excitable again.
- It needs a certain topology and morphology with a minimum amount of isolating tissue surrounding the CC. The isolating tissue can be either totally or partially covering the CC.

[0014] CCs that are totally covered for a minimum distance are highly likely to contribute to an arrhythmogenic event. However, the ability of partially covered CCs to contribute to arrhythmogenic events depends on several morphological factors, which are analyzed in present invention.

Description of the Invention

[0015] Present invention describes a method to obtain a measure of the local spatial structure of conducting properties of muscle tissue from medical images or from data acquired by a catheter or another data acquisition technology. This measure is associated with pathological conduction pathways in the tissue, and therefore can be used to help with automatically identifying potential re-entrant conducting channels (CCs) that are the cause of arrhythmia. The method works by analyzing the spatial distribution of tissue properties (obtained by interpreting the output of an acquisition method, e.g., absorption of X-rays, water content or retention of a contrast agent) in the local neighborhoods of several given points and creating output values for each of those points indicating their respective conductive structure properties.

[0016] To that end, the present invention provides a computer implemented method for calculating values indicative for the local spatial structure of conducting properties of heart muscle according to claim 1.

[0017] According to the proposed method, said acquisition technology may comprise an image acquisition technology such as Computed Tomography (CT) or Magnetic Resonance Imaging (MRI), among others, or may comprise a data acquisition technology including a medical instrument measuring voltage, by contact, of the heart muscle tissue, such as a catheter.

[0018] In an embodiment, the plurality of points are sampling points on a CC previously detected. Alternatively, the plurality of points are sampling points contained in a part of, or the whole, ROI.

[0019] In an embodiment, step a) further comprises using domain-specific geometric information of the heart muscle tissue, said domain-specific geometric information at least including an orientation of the cardiac wall of the heart muscle tissue.

[0020] In an embodiment, the ROI consists of a 3D volume enclosed by a topological 2-manifold. In this case, the plurality of rays are straight-line segments from the given initial point to a first point of intersection of the rays with the manifold. In another embodiment, the ROI consists of a triangular surface mesh. In this case, the plurality of rays are straight line segments within the triangles, said segments being joint at the triangular edges by sharing one edge point and having the vertically opposed angles equal.

[0021] Preferably, the sequence of sampling points is limited to a given length of the plurality of rays. Besides, the sequence of sampling points is defined according to a set of distances defined for each ray of the plurality of rays, said set of distances comprising a sequence with ascending distance from the given initial point.

[0022] According to the proposed method, the cited step e) may be performed by averaging the associated values of each ray using weights derived from the geometry of the rays or, alternatively, by statistically processing relative frequencies of the ray classification.

[0023] In a particular embodiment, the spatial distribution comprises different values representing electrical functionality of the heart muscle tissue, wherein a first of said different values, or Healthy, represents tissue with normal electrical functionality; a second of said different values, or Border-Zone, represents tissue with abnormal electrical behavior; and a third of said different values, or Core, represents tissue with no electrical functionality.

[0024] According to this particular embodiment, the associated ray value of each ray is provided by traversing the sampling points and their associated values starting from the given initial point and reporting information about the finding of a first value of a given category within the cited Healthy, Border-Zone and Core categories.

[0025] Moreover, the associated ray value of each ray can be provided according to the following rules: if the values

corresponding to all sampling points of the ray are Border-Zone, then Border-Zone is assigned; otherwise, the value of the closest sampling point whose value isn't Border-Zone, is assigned. The reduced single point value in this embodiment is defined as follows: if there is at least one ray value Healthy, then 0; otherwise, by calculating a core surrounding parameter as weighted relative frequency of core rays or by calculating the single point value from the core surrounding parameter using an affine-linear function and clipping the result at a certain lower and upper threshold.

[0026] According to said particular embodiment, the method may further create a volume image of the single point value by assigning to all voxels of the ROI whose value is Border-Zone the reduced value obtained in step e) and by assigning to all other voxels the value 0, and further visualizing the created volume image by means of volume rendering or a marching cubes calculation or using the created volume image for further processing.

[0027] Even, according to said particular embodiment, the method may further create sampling points on a given CC centerline such that there are sampling points on every end point and bifurcation and the line segments between sampling points are short enough; calculate the single point value at every one of said created sampling points, interpolated linearly between the latter; and numerically integrate the single point value over the whole trajectory of the CC centerline, providing a centerline's single point value.

[0028] In yet another embodiment of the proposed method, a distance to a non-Border-Zone point is recorded, wherein there is no limit of the ray length; and a directionality analysis is performed on the rays by applying a statistical procedure thereof such as a Principal Component Analysis, PCA.

[0029] Other embodiments of the invention that are disclosed herein also include software programs to perform the method embodiment steps and operations summarized above and disclosed in detail below. More particularly, a computer program product is one embodiment that has a computer-readable medium including computer program instructions encoded thereon that when executed on at least one processor in a computer system causes the processor to perform the operations indicated herein as embodiments of the invention.

Brief Description of the Drawings

[0030] The previous and other advantages and features will be more fully understood from the following detailed description of embodiments, with reference to the attached figures, which must be considered in an illustrative and non-limiting manner, in which:

Fig. 1 illustrates the different types of CCs that can be found in heart muscle tissue and characterized by the present invention.

Fig. 2 schematically illustrates a general method workflow with their inputs and outputs for calculating values indicative for the local spatial structure of conducting properties of heart muscle tissue according to the proposed invention.

Fig. 3 is a perspective illustration of a ray on a triangular mesh representing a curved strip as a sequence of rectangles being formed by two triangles each, according to an embodiment of the present invention.

Fig. 4 illustrates an example of the results obtained by the core distance process, according to an embodiment of the present invention. The figure illustrates rays in several directions probing for Core presence and recording its distance (Ray 0: 1, Ray 1: 5, Ray 2: ∞ , Ray 3: ∞ , Ray 4: ∞ , Ray 5: 10, Ray 6: 5, Ray 7: 2).

Fig. 5 illustrates an example of the intermediate results obtained from the directionality analysis process, according to an embodiment of the present invention. Fig. 5a represents the input of the point value reduction (rays with assigned values); Fig. 5b represents the point set used in PCA (central point displaced in ray directions by distances proportional to ray values); and Fig. 5c represents the principal components of the point set from Fig. 5b.

Detailed Description of the Invention and of Preferred Embodiments

[0031] Fig. 2 shows the main components of the workflow implemented by the proposed invention, with their inputs and outputs, for calculating values indicative for the local spatial structure of conducting properties of heart muscle tissue. The proposed method extracts information about the structure surrounding any of a given finite set of points 200 by processing spatial distribution of a value related to tissue properties in the following way:

[0032] For every point of said given set of points 200 whose Channelicity (i.e. a measure of the local spatial structure of conducting properties of muscle tissue) has to be calculated, the method executes the following steps via a processor of a computer system (not illustrated):

1. Ray Classification:

EP 3 441 937 B1

- Span rays 201 starting from the given initial point in multiple 3D directions, providing a structure with a plurality of rays with a given geometry.
- Define 202 a sequence of sampling points on each of the rays of the structure.
- Map 203 the value of the spatial distribution to the sampling points.
- Assign 204 every ray a single value based on the mapped values, the absolute positions of the sampling points and the positions of the sampling points relative to each ray of the structure (distance to ray base), providing an associated ray value.

2. Reduction to point value (205):

A single value (scalar or vector) is calculated from the ray geometries and their associated ray value.

[0033] Following, the different inputs and output of the method and the different components workflow will be detailed:

Inputs and Output

[0034] The method needs the following data as input:

- A Region of Interest (ROI), which preferably is a subspace of \mathbb{R}^3 in which there exists a path of finite length between every pair of points. This mostly rules out very complex geometries like fractals, but also limits the ROIs to path-connected spaces. The latter limitation can be overcome in many real-world cases by running the whole method several times on suitable subsets of the whole ROI and the corresponding subsets of the point set 200. Examples for such ROIs include the myocardium of a full heart or a single heart chamber as well as a two-dimensional surface representation of a heart chamber (ignoring transmural information).
- The spatial distributions of acquired information in the ROI, assigning a value to every point of the ROI. This can be a scalar field, vector field, another distribution or combinations of them. In the following, it will be referred to the Cartesian product of the underlying distribution functions as one single "spatial distribution". A typical example for the spatial distribution would be a 3D image from a medical imaging device with trilinear interpolation on the cuboids between the voxel centers.
- A finite set of points 200 whose single point value (i.e. the Channelicity) is to be calculated. All points 200 must fall into the ROI.

[0035] The output of the method is a single "Channelicity" value for each point of the input point set 200.

Step 201: Ray Spanning

[0036] Input:

- Coordinates of one point p of the set or plurality of points 200 whose Channelicity is to be calculated
- (Optional) Domain-specific geometric information

[0037] Output:

- A finite sequence c of n_r normalized vectors representing ray directions

[0038] The algorithm implemented by the proposed method spans n_r rays (providing said structure with a particular geometry) by defining their ray directions c as normalized vectors (magnitude 1) tangential to the ROI in the given point p .

[0039] Usually a general-purpose algorithm for Sphere Point Picking on the unit sphere (e.g. [1], [2] or [3]) is used to create the direction vectors. These algorithms attempt to create a distribution of the direction vectors on the unit sphere that is uniform as possible.

[0040] But depending on the application other algorithms may be used in order to achieve a specific distribution of directions. The algorithm may also take into account the point position p as well as additional domain-specific geometric information, e.g. the orientation of the cardiac wall in order to have a lower density of rays perpendicular to the wall than in the electrophysiologically more relevant tangential directions.

Step 202: Sampling of ray trajectories

[0041] Input:

- Coordinates of the point p whose Channelicity is to be calculated.
- The sequence c of n_r normalized vectors representing ray directions (output of step 201).

[0042] Output:

- One sequence $s(i)$ of $n_s(i)$ sampling points for every ray index i .
- One sequence $g(i)$ of the distances of each of the $n_s(i)$ sampling points from the initial point p for every ray index i .

- Ray trajectory definition:

[0043] Graphically, a maximal ray from a point p in a direction $c(i)$ is a path starting from p in direction c and continuing as straight as the ROI allows it (locally minimizing distances) infinitely or until it cannot continue straight within the ROI anymore.

Formal definition:

[0044] A ray from a point p is a continuous function r from a left-closed interval I (starting from 0) to the ROI with $r(0) = p$ and the geodesic property fulfilled for all s in the interior of I . The geodesic property at a point s is fulfilled, if and only if there is a neighborhood V of s such that for all s_1 and s_2 in V $d_{\text{intrinsic}}(r(s_1), r(s_2)) = d(s_1, s_2)$ with $d_{\text{intrinsic}}$ being the intrinsic metric on the ROI induced by the Euclidian metric on \mathbb{R}^3 and d being the Euclidian metric on \mathbb{R} .

[0045] A maximal ray from p in direction $c(i)$ is a ray r with $r'(0) = c(i)$ (if the domain contains more than one point) that is maximal according to the following partial of rays: A ray is greater or equal, than a second ray, if and only if its domain is greater or equal and it coincides with the other ray on the intersection of their domains.

Detailed definition and interpretation:

[0046] A path is a continuous function q from an Interval $I=[a,b]$ of \mathbb{R} to the ROI S . A path is called a path between x_0 and x_1 , if and only if $q(a)=x_0$ and $q(b)=x_1$. The length of a path is defined as the supremum of the lengths of all possible rectifications of the path, wherein the length of a rectification is defined as the distance between all subsequent point pairs of the rectification according to the metric used in \mathbb{R}^3 .

[0047] This induces the following intrinsic metric $d_{\text{intrinsic}}$ on the ROI: The distance between two points p_1 and p_2 in the ROI is defined as the infimum of the lengths of all finite paths between p_1 and p_2 . Since all path lengths are non-negative numbers and by requirement of the ROI there exists a path with finite length between all points in ROI, the infimum exists and is always a non-negative real number. It can be shown that the function $d_{\text{intrinsic}}$ also fulfills the other requirements for being a metric, which is omitted here.

[0048] A ray from p is a continuous function r from a closed or right-open interval I starting from 0 (i.e. it has the form $[0, a]$, or $[0, a[$ or $[0, \infty[$ for $a \in \mathbb{R}$) to the ROI with $r(0) = p$ and the geodesic property fulfilled for all s in the interior of I (i.e. $]0, a[$ or $]0, \infty[$). The geodesic property at a point s is fulfilled, if and only if there is a neighborhood V of s such that $d_{\text{intrinsic}}(r(s_1), r(s_2)) = d(s_1, s_2)$ for all s_1 and s_2 in V with d being the Euclidean metric on \mathbb{R} . Note that this requirement also implies a natural parameterization (function parameter represents arc length).

[0049] A partial order on the set of rays can be defined like this: A ray r_b is greater or equal than a ray r_a , if and only if the domain of ray r_b is a non-strict superset of the domain of ray r_a and their values coincide on the intersection of their domains. Graphically, both rays start out with the same trajectory, but r_b may continue further than ray r_a . From now on, the method is only interested in rays that are maximal elements according to this order.

[0050] A ray in direction $c(i)$ is a ray r which is either differentiable in 0 with $r'(0) = c(i)$ or defined only on the point 0.

[0051] For many real-world cases of ROIs there is exactly one maximal ray for each given initial point and direction. However, that unique maximal ray may be of length 0 (if the direction points into a direction in which the ROI doesn't extend), so in cases of more complex ROIs care has to be taken to select ray directions that are compatible with the ROI in the sense that they produce non-trivial rays. For example, if the ROI consists of a 2-manifold, the rays have to be within the tangential plane of the ROI in the ray's initial point.

[0052] However, in some pathological ROI sets there might be more than one maximal ray for a given initial point and direction. In applications that allow such ROIs, the proposed method must employ an additional criterion to choose one maximal ray in a deterministic manner.

Examples of rays in different ROIs:

5 [0053] Using the whole \mathbb{R}^3 space as ROI, a maximal ray starting from p in a given direction $c(i)$ is simply a straight geometric ray: $Ray_{p,c(i)}(m) = p + m * c(i)$ for $m \in [0, \infty[$.

[0054] In any 2-dimensional affine-linear subspace of \mathbb{R}^3 the maximal rays are either straight geometric rays (if the direction is within the subspace) or single points (if the direction points out of the subspace).

10 - Computational calculation of ray trajectories

3D Volume Enclosed by Topological 2-Manifold:

15 [0055] In the case of 3D volumes enclosed by topological 2-manifold, like e.g. the myocardium volume enclosed by a closed surface mesh defined by a segmentation process, a ray is a straight-line segment from the given initial point to the first point of intersection s of the ray with the manifold: $Ray_{p,c(i)}(m) = p + m * c(i)$ for $m \in [0, d(s, p)]$, with d being the Euclidian 3D metric.

Triangular Surface Mesh:

20 [0056] Maximal rays on triangular surface meshes are one-dimensional polygonal curves. They consist of straight line segments within the triangles. The segments are joint at the triangle edges by sharing one edge point and having the vertically opposed angles (between ray and triangle edge, measured in their respective triangle) equal. The sequence is continued indefinitely until it possibly encounters a simple edge (one that forms part of only one triangle). If such a simple edge is reached by the ray, the ray's intersection with the simple edge is the end point of the ray. Otherwise the
25 ray is of infinite length. Fig. 3 shows an example of such type of ROI. As can be seen in the figure, the equal opposite angles between ray and edge are marked with a crisscross pattern. One can observe that the ray is no longer straight in this case, but follows the curvature of the strip, changing its direction at every transition between rectangles (but not at the edges within rectangles) in order to follow the curvature, but keeping its downward tendency given by the initial ray direction (drawn as arrow). The initial point is marked as a filled circle and the end point at the ray's intersection with
30 a simple edge is marked as an empty circle.

- Sampling

35 [0057] For every ray index i a discrete set of distances is defined, represented as sequence $g(i)$ of ascending distances from the point p .

[0058] The trajectory of the maximal ray $Ray_{p,c(i)}$ from the given point p in the given direction $c(i)$ is evaluated at each value of $g(i)$:

$$40 \quad s(i)(j) = Ray_{p,c(i)}(g(i)(j)) \text{ for each } j$$

[0059] Those are the sampling points on the maximal ray defined by the point p and the direction $c(i)$.

45 Step 203: Mapping

[0060] Input:

- The sequences $s(i)$ of $n_s(i)$ sampling points from the previous step 202.
- The spatial distribution representing the tissue properties.

50 [0061] Output:

- One sequence $v(i)$ of values for every ray i , corresponding to the $n_s(i)$ sampling points $s(i)$.

55 [0062] The input field is evaluated at every one of the $n_s(i)$ sampling points $s(i)(j)$ on every ray i . Depending on the definition of the field, this may include interpolation and/or other mathematical operations. For example, if the continuous field is defined as trilinear interpolation of a 3-D image, in this step the interpolation has to be performed on every one of the sampling points.

Step 204: Ray values

[0063] Input:

- 5 • Coordinates of the point p whose Channelicity is to be calculated
- The sequences $s(i)$ of the $n_s(i)$ sampling points from step 2020.
- The sequences $g(i)$ of the $n_s(i)$ distances of the sampling points from the initial point from step 202.
- The sequences $v(i)$ of the $n_s(i)$ mapped values from 203.

10 [0064] Output:

- A sequence w of the n_r ray classifications.

[0065] The mapped values of every sampling point and the location of the sampling points, both in absolute coordinates and relative to the point p , are used to produce a single classification for every ray.

[0066] Examples of this process include traversing the sampling points and their associated values starting from the ray origin and reporting information about the finding of the first value of a given category (for example as specified in following sections, Ray Classification: Contact with non-BZ tissue and Core Distance).

20 Step 205: Reduction to Point Value

[0067] Input:

- 25 • Coordinates of the point p whose Channelicity is to be calculated.
- The sequence c of n_r normalized vectors representing ray directions (output of 201).
- The sequence w of ray classifications for the n_r rays from 204.
- (Optional) Domain-specific geometric information.

30 [0068] Output:

- One single point classification value.

[0069] The classifications of all the rays as well as geometric information about the rays and (optionally) addition domain-specific geometric information are used to produce a single classification for the input point p .

35 [0070] For example, this step can consist of averaging the ray classification values, possibly using weights derived from the geometric information (e.g. giving rays running tangential to the cardiac wall a higher weight than transmural rays due to anisotropic electrical properties). Another example is statistical processing of the relative frequencies of ray classifications, again possibly using weights derived from the geometric information.

40 Local Channelicity

[0071] One particular example embodiment of the proposed method is the calculation of a measure of how enclosed within isolating tissue a point is.

45 [0072] The spatial distribution input is a ternary scalar field containing the values H (Healthy), BZ (Border-Zone) and K (Core). Those values represent the electrical functionality of the myocardium tissue. Zones of "healthy" tissue represent tissue that works mostly normal, "border-zone" represents tissue with abnormal electrical behavior (mostly slowed electrical propagation) and "core" represents tissue with no active electrical functionality (only passive conduction, if any).

[0073] This field is usually derived from a medical image with injected contrast that shows the tissue functionality as gray value, for example gadolinium-enhanced magnetic resonance images. A simple way to obtain the spatial distribution of the functionality from such an image is to apply trilinear interpolation to the image and classify the interpolated values within the myocardium by using two thresholds. Values below the lower threshold are classified as H, values between the lower and the upper threshold are classified as BZ and values above the upper threshold are classified as K.

55 - Ray Classification: Contact with non-BZ tissue

[0074] The rays of step 201 are defined as a fixed number of rays (typically 30, however other amounts of rays are also possible) that are distributed as uniformly as possible using a Sphere Point Picking algorithm.

[0075] The sampling points of step 202 are distributed equidistantly (e.g. at distance of half the voxel spacing) from

EP 3 441 937 B1

the ray base to a fixed length (typically 3.5 mm).

[0076] The ray value of step 204 can be assigned according to the following rules:

- If the values corresponding to all sampling points are BZ, then BZ.
- Otherwise, the value of the closest sampling point whose value isn't BZ.

[0077] If there are less sampling points than expected (because the ray touches the border of the ROI, e.g. rays 7 and 8 in the example below), process the ray as if there was an additional sampling point with the value K at the end, in order to account for the fact that the space outside of the ROI is considered non-conducting.

Example 1:

[0078]

	Sampling Point							→	Ray value
	1	2	3	4	5	6	7		
Ray 1	BZ	BZ	BZ	BZ	BZ	BZ	BZ	→	BZ
Ray 2	BZ	BZ	BZ	BZ	BZ	BZ	H	→	H
Ray 3	BZ	BZ	BZ	BZ	BZ	BZ	K	→	K
Ray 4	BZ	BZ	BZ	H	H	BZ	K	→	H
Ray 5	K	K	BZ	BZ	K	K	BZ	→	K
Ray 6	BZ	BZ	K	K	BZ	BZ	H	→	K
Ray 7	BZ	BZ	BZ	BZ	BZ	-	-	→	K
Ray 8	BZ	BZ	H	BZ	BZ	-	-	→	H

- Point Value Reduction: Core Surrounding

[0079] The point value (called "Local Channelicity" in this particular exemplary embodiment) of the reduction (step 205) can be defined as follows:

- If there is at least one ray value H, then 0.
- Otherwise, the following procedure is applied:
 - Calculate the "Core Surrounding" as weighted relative frequency of Core rays. The weights are a function that varies affine-linearly with the angle between the ray and the cardiac wall's tangential plane.
 - Calculate the "Local Channelicity" using an affine-linear function defined by the mappings $[a \rightarrow 0]$ and $[b \rightarrow 1]$ (with a typically being 15% and b being 40%) and cutting off values below 0% and above 100%.

Example 2:

[0080]

Healthy Rays	Border-Zone Rays	Core Rays	Core Surrounding	Local Channelicity
0	19	1	5%	0%
0	17	3	15%	0%
0	12	8	40%	100%
0	8	12	60%	100%
0	15	5	25%	40%
1	14	5	25%	0%

- Application: Volume Channelicity

[0081] In order to obtain a Volume Channelicity image, a volume image is created according to the following rules: All voxels, whose ternary spatial distribution value is BZ, are assigned the value calculated by the algorithm presented in the previous section 'Point Value Reduction: Core Surrounding'. All other voxels are assigned the value 0. The resulting distribution of tissue with possibly arrhythmogenic properties can be visualized using volume rendering or surface rendering after performing a marching cubes calculation, or used for further processing in the detection of CCs.

- Application: Filter channels detected in layers

[0082] The Local Channelicity also allows filtering out false positives of CCs detected by an external CC detection algorithm. This can be done by applying a threshold filter to a Channelicity value of the CC. The CC's Channelicity may be calculated as follows.

[0083] A centerline of a CC is sampled with a high enough resolution, having sampling points on every bifurcation (if there are branches) and at every end point. This is done by putting initial sampling points on every end point and bifurcation and iteratively subdividing the linear segments between sampling points until all segments have a length below a given threshold. The Local Channelicity is calculated at every sampling point and interpolated linearly between sampling points. The Local Channelicity is then integrated numerically over the whole trajectory of the CC's centerline. The resulting value is the centerline's Channelicity.

[0084] Since the Local Channelicity is between 0% (=0) and 100% (=1), a centerline's Channelicity can be between 0, when the Local Channelicity is 0% everywhere, and the length of the centerline's trajectory, if the Local Channelicity is 100% everywhere.

[0085] For example, a centerline of 10 mm length and a constant Local Channelicity of 0% (no arrhythmogenicity anywhere) have a Channelicity of 0 mm. A centerline of 10 mm length and a constant Local Channelicity of 100% (completely arrhythmogenic everywhere) have a Channelicity of 10 mm. A centerline of 10 mm length with a constant Local Channelicity of 50% everywhere has a Channelicity of 5 mm. A centerline of 10 mm length with a Local Channelicity of 100% during half of its trajectory and 0% during the other half has a Channelicity of 5 mm, too.

Method instances using Propagation Range

[0086] This section describes another particular example embodiment of the proposed method. While the method described in the 'Ray Classification: Contact with non-BZ tissue' section performs only a qualitative evaluation of the conductive properties in each direction, a quantitative evaluation of the excitation wave's "range" (e.g. until it touches a nonconductive obstacle, or the distance a stimulus can travel in that direction within a certain time limit) is also possible. The obtained quantitative information can help to improve the point reduction's robustness and level of detail (see following section 'Continuous Core Surrounding') or even enable new point reduction techniques that use the quantitative information for directionality analyses (section 'Directionality Analysis').

- Ray Classification: Range

Core Distance:

[0087] This "Ray Classification" method is similar to the one introduced in the 'Ray Classification: Contact with non-BZ tissue' section in that it traverses every ray from the initial point until it discovers anything different from BZ. However, instead of just recording the tissue type discovered, it records the distance to the non-BZ point, if K is found, or infinity, if H is found. That can be interpreted as the distance to the closest K tissue that can be reached in the particular direction without having to pass through H first. In contrast to said previous method, there is no fixed limit of the ray length: Sampling points are placed on the ray equidistant sections until the ray leaves the ROI. Fig. 4 shows an example using this method.

[0088] Like in the 'Ray Classification: Contact with non-BZ tissue' section, an additional implicit sampling point with the value K is assumed at the end of the ray.

Example 3:

[0089]

BZ	BZ	BZ	BZ	BZ	BZ	H	→	∞
----	----	----	----	----	----	---	---	---

(continued)

BZ	BZ	BZ	BZ	BZ	BZ	K	→	6
BZ	BZ	BZ	H	H	BZ	K	→	∞
K	K	BZ	BZ	K	K	BZ	→	0
BZ	BZ	K	K	BZ	BZ	H	→	2

Intensity-based Range (Simulation):

[0090] This "Ray Classification" method determines for every ray the distance that a stimulus can travel in that direction within a fixed timeframe. It does so by performing a one-dimensional Eikonal-type simulation, with the propagation velocity at every sampling point being determined by the value of the input scalar field at that point and inverse velocities being interpolated in between.

[0091] The simulation starts at time 0, for which the stimulus wavefront is at position 0 from the ray origin. It proceeds until a fixed simulation time t_{end} is reached and returns the distance that the stimulus has travelled in the duration.

[0092] For every segment between the sampling points $s(i)(j)$ and $s(i)(j+1)$ of geodesic ray segment length $x=g(i)(j+1) - g(i)(j)$ the quadratic relationship between position and local activation time of the stimulus within the segment is calculated by calculating the stimulus velocities v_a and v_b at the two end points $s(i)(j)$ and $s(i)(j+1)$, respectively, using the pixel intensities from the mapping step and assuming an affine-linear distribution of the inverse velocities (time per distance) in between. If the total time of the segment, defined as sum of times of all segments up to the current one, is lower than the given simulation time t_{end} , then the simulation proceeds to the next segment. Otherwise the quadratic position-time relationship is used to determine the exact distance, at which the stimulus is a time t_{end} , end the value is returned as result.

[0093] The exact relationship between pixel intensity and stimulus propagation velocity depends on the chosen model, but is usually a monotonically decreasing function approximating 0 when the pixel intensity of dense scar is reached.

- Reduction to Point Value

Continuous Core Surrounding:

[0094] The calculation of the Core Surrounding in 'Point Value Reduction: Core Surrounding' section takes into account only the discrete classification of rays (Core vs. Non-Core, blocked vs. conducting). However, with the additional range information, obtained from the methods in 'Ray Classification: Range' section a similar calculation can be performed using the range as indicator of how well the tissue conducts a stimulus locally in a given direction. Instead of using a weighted relative frequency of Core rays, which would be equivalent to a weighted average of the indicator function of Core rays (1 for Core rays, 0 for other rays), a weighted average of a continuous value can be used. For this purpose, the range obtained from the Ray Classification is transformed by a continuous monotonically decreasing function.

Directionality Analysis

[0095] The ray ranges calculated in 'Ray Classification: Range' section can be used to perform a directionality analysis that tells how strongly the excitation wave is guided in one particular direction and which direction that is. Thereto, in an embodiment, Principal Component Analysis (PCA) or similar techniques can be applied to a point set that is calculated in the following manner: For every ray the method creates a point that is displaced from the central point in ray direction by a distance proportional to the ray range.

[0096] The Principal Components (PC) produced by the PCA are ordered by their magnitude. The direction of the largest PC is used as direction for the output vector. The ratio between the largest PC and the second largest PC is used as magnitude for the output vector.

[0097] The proposed invention can be implemented by means of software elements, hardware elements, firmware elements, or any suitable combination of them. If implemented in software, the functions may be stored on or encoded as one or more instructions or code on a computer-readable medium.

[0098] Computer-readable media include computer storage media. Storage media may be any available media that can be accessed by a computer. By way of example, and not limitation, such computer-readable media can comprise RAM, ROM, EEPROM, CD-ROM or other optical disk storage, magnetic disk storage or other magnetic storage devices, or any other medium that can be used to carry or store desired program code in the form of instructions or data structures and that can be accessed by a computer. Disk and disc, as used herein, includes compact disc (CD), laser disc, optical disc, digital versatile disc (DVD), floppy disk and Blu-ray disc where disks usually reproduce data magnetically, while

discs reproduce data optically with lasers. Combinations of the above should also be included within the scope of computer-readable media. Any processor and the storage medium may reside in an ASIC. The ASIC may reside in a user terminal. In the alternative, the processor and the storage medium may reside as discrete components in a user terminal.

5 **[0099]** As used herein, computer program products comprising computer-readable media including all forms of computer-readable medium except, to the extent that such media is deemed to be non-statutory, transitory propagating signals.

[0100] The scope of the present invention is defined in the following set of claims.

10 References

[0101]

15 [1] J. M. Cook, "Technical Notes and Short Papers: Rational Formulae for the Production of a Spherically Symmetric Probability Distribution," Mathematical Tables and Other Aids to Computation, vol. 11, pp. 81-82, 1957.

[2] G. Marsaglia, "Choosing a Point from the Surface of a Sphere," The Annals of Mathematical Statistics, vol. 43, no. 2, pp. 645-646, 1972.

[3] "Sphere Point Picking," [Online]. Available: <http://mathworld.wolfram.com/SpherePointPicking.html>.

20

Claims

1. A computer implemented method for calculating values indicative for the local spatial structure of conducting properties of heart muscle tissue, using a continuous region of interest, ROI, where it is considered that there may exist a conducting channel, CC, wherein each point of the ROI is associated with a value of a given spatial distribution assigning a value to every point of the ROI representing the tissue properties acquired via an acquisition technology, the method comprising performing, by a processor of a computer system, for each one of a plurality of points (200) within the ROI, the following steps:

30

a) spanning (201) a plurality of rays starting from the given point within the ROI in multiple 3-D directions by at least using coordinates of a reference coordinate system of the point, providing a structure with a plurality of rays with a given geometry;

b) defining (202) a sequence of sampling points on each ray of said structure;

c) mapping (203) the value of the spatial distribution on each defined sampling point of each ray of the structure;

35

d) classifying (204) each ray of the structure by assigning to each ray a single value based on:

the mapped values,

the absolute positions within said reference coordinate system of the sampling points, and

the positions of the sampling points relative to each ray of the structure, providing an associated ray value;

40

and

e) reducing (205) each structure to a single point value in view of the geometry of the rays and their associated ray value, wherein said single point value is indicative of a local spatial structure of conducting properties of an area of heart muscle tissue.

45

2. The method of claim 1, wherein the plurality of points (200) are sampling points on a CC previously detected or sampling points being contained in a part of or the whole ROI.

3. The method of claim 1, wherein said step a) further comprises using domain-specific geometric information of the heart muscle tissue, said domain-specific geometric information at least including an orientation of the cardiac wall of the heart muscle tissue.

50

4. The method of previous claims, wherein:

55

said acquisition technology comprising an image acquisition technology comprising at least Computed Tomography, CT, or Magnetic Resonance Imaging, MRI; or

said acquisition technology comprising a data acquisition technology including a medical instrument measuring voltage, by contact, of the heart muscle tissue.

5. The method of claim 1, wherein the ROI consists of:

a 3D volume enclosed by a topological 2-manifold, the plurality of rays being straight-line segments from the given initial point to a first portion of intersection of the rays with the manifold; or
 a triangular surface mesh, the plurality of rays being straight line segments within the triangles, said segments being joint at the triangular edges by sharing one edge point and having the vertically opposed angles equal.

6. The method of claim 1, wherein the sequence of sampling points is limited to a given length of the plurality of rays.

7. The method of claim 1 or 6, wherein the sequence of sampling points is defined according to a set of distances defined for each ray of the plurality of rays, said set of distances comprising a sequence with ascending distance from the given initial point.

8. The method of claim 4, wherein said spatial distribution comprises different values representing electrical functionality of the heart muscle tissue, wherein a first of said different values, or Healthy, represents tissue with normal electrical functionality; a second of said different values, or Border-Zone, represents tissue with abnormal electrical behavior; and a third of said different values, or Core, represents tissue with no electrical functionality.

9. The method of claim 8, wherein the associated ray value of each ray is provided by traversing the sampling points and their associated values starting from the given initial point, and reporting information about the finding of a first value of a given category within the cited Healthy, Border-Zone and Core categories.

10. The method of claim 8 or 9, wherein the associated ray value of each ray is provided according to the following rule:

if the values corresponding to all sampling points of the ray are Border-Zone, then Border-Zone is assigned; otherwise, the value of the closest sampling point whose value is not Border-Zone is assigned.

11. The method of claim 10, wherein the reduced single point value is defined according to:

if there is at least one ray value Healthy, then 0; otherwise, by:

calculating a core surrounding parameter as weighted relative frequency of core rays; and calculating the single point value from the core surrounding parameter using an affine-linear function and clipping the result at a certain lower and upper threshold.

12. The method of claim 1, wherein step e) is performed by averaging the associated values of each ray using weights derived from the geometry of the rays or by statistically processing relative frequencies of the ray classification.

13. The method of claim 8, further comprising:

creating a volume image of the single point value by assigning to all voxels of the ROI whose value is Border-Zone the reduced value obtained in step e) and by assigning to all other voxels the value 0; and further performing a marching cubes calculation for visualizing the created volume image or using the created volume image for further processing.

14. The method of claim 8, further comprising:

creating sampling points on a given CC centerline such that there are sampling points on every end point and bifurcation and the line segments between sampling points are short enough; and calculating the single point value at every one of said created sampling points, interpolated linearly between the latter; and numerically integrating the single point value over the whole trajectory of the CC centerline, providing a center-line's single point value.

15. The method of claim 10, further comprising:

recording a distance to a non-Border-Zone point, wherein there is no limit of the ray length; and

performing a directionality analysis on the rays by applying a statistical procedure thereof, the statistical procedure including a Principal Component Analysis, PCA.

- 5 16. A non-transitory computer readable medium including code instructions which, when executed by a computer, cause the computer to carry out the steps of the method of any of the previous claims.

Patentansprüche

- 10 1. Computerimplementiertes Verfahren zur Berechnung von Werten, die auf die lokale räumliche Struktur von leitenden Eigenschaften von Herzmuskelgewebe hinweisen, unter Verwendung eines kontinuierlichen Zielbereichs, ROI, wobei von der Existenz eines leitenden Kanals, CC, ausgegangen wird, wobei jeder Punkt des ROI mit einem Wert einer gegebenen räumlichen Anordnung verknüpft ist, wodurch jedem Punkt des ROI ein Wert, der die über eine Erfassungstechnologie ermittelten Gewebeeigenschaften darstellt, zugeordnet wird, und wobei das Verfahren die Durchführung der folgenden Schritte für jeden einer Vielzahl von Punkten (200) innerhalb des ROI durch den
- 15 Prozessor eines Computersystems umfasst:
- a) Aufspannen (201) einer Vielzahl von Strahlen, ausgehend von dem gegebenen Punkt innerhalb des ROI in mehrere 3-D-Richtungen durch mindestens die Verwendung von Koordinaten eines Bezugskordinatensystems des Punkts, und dadurch Bereitstellung einer Struktur mit einer Vielzahl von Strahlen mit einer gegebenen Geometrie;
- 20 b) Definieren (202) einer Folge von Abtastpunkten auf jedem Strahl der genannten Struktur;
- c) Abbilden (203) des Werts der räumlichen Anordnung auf jedem definierten Abtastpunkt eines jeden Strahls der Struktur;
- 25 d) Klassifizieren (204) eines jeden Strahls der Struktur, indem jedem Strahl ein eindeutiger Wert basierend auf Folgendem zugeordnet wird:
- den abgebildeten Werten,
den absoluten Positionen der Abtastpunkte innerhalb des genannten Bezugskordinatensystems, und
- 30 den Positionen der Abtastpunkte relativ zu den einzelnen Strahlen der Struktur, und dadurch Bereitstellen eines zugehörigen Strahlenwerts; und
- e) Reduzieren (205) einer jeden Struktur auf einen Einzelpunktwert hinsichtlich der Geometrie der Strahlen und ihres zugehörigen Strahlenwerts, wobei der genannte Einzelpunktwert auf eine lokale räumliche Struktur von leitenden Eigenschaften eines Bereichs von Herzmuskelgewebe hinweist.
- 35 2. Verfahren nach Anspruch 1, wobei die Vielzahl von Punkten (200) Abtastpunkte in einem CC sind, die zuvor erfasst wurden, oder Abtastpunkte, die in einem Teil des ROI oder dem gesamten ROI enthalten sind.
- 40 3. Verfahren nach Anspruch 1, wobei der genannte Schritt a) ferner die Verwendung von bereichsspezifischen geometrischen Informationen des Herzmuskelgewebes umfasst, wobei die genannten bereichsspezifischen geometrischen Informationen zumindest eine Orientierungsangabe der Herzwand des Herzmuskelgewebes enthalten.
4. Verfahren nach den vorstehenden Ansprüchen, wobei:
- 45 die genannte Erfassungstechnologie eine Bilderfassungstechnologie bestehend aus mindestens Computertomographie, CT, oder Magnetresonanztomographie, MRT, umfasst; oder
- die genannte Erfassungstechnologie eine Datenerfassungstechnologie, bestehend aus einem medizinischen Instrument, das durch Kontakt die Spannung des Herzmuskelgewebes misst, umfasst.
- 50 5. Verfahren nach Anspruch 1, wobei der ROI aus Folgendem besteht:
- einem 3D-Volumen, das von einer topologischen 2-Mannigfaltigkeit umschlossen ist, wobei die Vielzahl von Strahlen geradlinige Segmente vom gegebenen Ausgangspunkt bis zu einem ersten Schnittbereich der Strahlen mit der Mannigfaltigkeit sind; oder
- 55 einem dreieckigen Flächennetz, wobei die Vielzahl der Strahlen geradlinige Segmente innerhalb der Dreiecke sind, wobei die genannten Segmente an den Dreieckskanten durch einen gemeinsamen Kantenpunkt verbunden sind und die vertikal entgegengesetzten Winkel gleich sind.

6. Verfahren nach Anspruch 1, wobei die Folge der Abtastpunkte auf eine gegebene Länge der Vielzahl von Strahlen begrenzt ist.
- 5 7. Verfahren nach Anspruch 1 oder 6, wobei die Folge von Abtastpunkten nach einer Reihe von für jeden Strahl der Vielzahl von Strahlen festgelegten Abständen definiert ist, wobei die genannte Reihe von Abständen eine Folge mit aufsteigender Entfernung von dem gegebenen Ausgangspunkt umfasst.
- 10 8. Verfahren nach Anspruch 4, wobei die genannte räumliche Anordnung verschiedene Werte umfasst, die die elektrische Funktionsfähigkeit des Herzmuskelgewebes darstellen, wobei ein erster der genannten verschiedenen Werte, oder Gesund, Gewebe mit normaler elektrischer Funktionsfähigkeit darstellt; ein zweiter der genannten verschiedenen Werte, oder Grenzbereich, Gewebe mit abnormalem elektrischen Verhalten darstellt; und ein dritter der genannten verschiedenen Werte, oder Kernwert, Gewebe mit keinerlei elektrischer Funktionsfähigkeit darstellt.
- 15 9. Verfahren nach Anspruch 8, bei dem der zugehörige Strahlenwert eines jeden Strahls dadurch bereitgestellt wird, dass die Abtastpunkte und ihre zugehörigen Werte ausgehend von dem gegebenen Ausgangspunkt durchlaufen werden und Informationen über die Erfassung eines ersten Werts einer gegebenen Kategorie innerhalb der genannten Kategorien Gesund, Grenzbereich und Kernbereich übermittelt werden.
- 20 10. Verfahren nach Anspruch 8 oder 9, wobei der zugehörige Strahlenwert eines jeden Strahls nach folgender Regel bereitgestellt wird:
- wenn die allen Abtastpunkten des Strahls entsprechenden Werte Grenzbereich sind, dann wird Grenzbereich zugeordnet;
andernfalls wird der Wert des nächstliegenden Abtastpunktes, dessen Wert nicht Grenzbereich ist, zugeordnet.
- 25 11. Verfahren nach Anspruch 10, wobei der reduzierte Einzelpunkt看wert folgendermaßen definiert wird:
- wenn mindestens ein Strahlenwert Gesund ist, ist der Wert 0;
andernfalls durch:
- 30 Berechnen eines Kernumgebungsparameters als gewichtete relative Häufigkeit von Kernstrahlen; und
Berechnen des Einzelpunkt看wertes aus dem Kernumgebungsparameter unter Verwendung einer affin-linearen Funktion und Beschneiden des Ergebnisses an einer bestimmten unteren und oberen Schwelle.
- 35 12. Verfahren nach Anspruch 1, wobei Schritt e) durch Mittelung der zugehörigen Werte eines jeden Strahls unter Verwendung von aus der Geometrie der Strahlen abgeleiteten Gewichten oder durch statistische Verarbeitung relativer Häufigkeiten der Strahlenklassifizierung erfolgt.
- 40 13. Verfahren nach Anspruch 8, ferner umfassend:
- Erstellen eines Volumenbilds des Einzelpunkt看wertes indem allen Voxeln des ROI, deren Wert Grenzbereich ist, der in Schritt e) erhaltene reduzierte Wert und allen anderen Voxeln der Wert 0 zugeordnet wird; und
ferner Erstellen einer Marching-Cubes-Berechnung zur Visualisierung des erzeugten Volumenbilds oder Verwendung des erzeugten Volumenbilds zur weiteren Verarbeitung.
- 45 14. Verfahren nach Anspruch 8, ferner umfassend:
- Erzeugen von Abtastpunkten auf einer gegebenen CC-Mittellinie, so dass sich an jedem Endpunkt und jeder Gabelung Abtastpunkte befinden und die Liniensegmente zwischen den Abtastpunkten kurz genug sind; und
Berechnen des Einzelpunkt看wertes an jedem der erzeugten Abtastpunkte, wobei zwischen diesen linear interpoliert wird; und
numerische Integration des Einzelpunkt看wertes über die gesamte Bahn der CC-Mittellinie, wodurch sich der Einzelpunkt看wert einer Mittellinie ergibt.
- 50 15. Verfahren nach Anspruch 10, ferner umfassend:
- Aufzeichnen eines Abstands zu einem Nichtgrenzbereich-Punkt, wobei die Strahlenlänge nicht begrenzt ist; und
Durchführen einer Richtwirkungsanalyse der Strahlen durch Anwendung eines statistischen Verfahrens, wobei
- 55

das statistische Verfahren eine Hauptkomponentenanalyse, HKA, umfasst.

16. Nichtflüchtiges, computerlesbares Medium mit Code-Befehlen, die, bei Ausführung durch einen Computer diesen veranlassen, die Schritte des Verfahrens nach einem der vorstehenden Ansprüche abzuarbeiten.

5

Revendications

10

1. Une méthode mise en œuvre dans un ordinateur pour calculer les valeurs indicatives pour la structure spatiale locale de propriétés conductrices du tissu du muscle cardiaque, en utilisant une région d'intérêt continue, ROI, où il est jugé qu'un canal conducteur peut exister, CC, dans laquelle chaque point du ROI est associé à une valeur d'une certaine distribution spatiale attribuant une valeur à chaque point du ROI représentant les propriétés du tissu acquises par le biais d'une technologie d'acquisition, la méthode comportant, qu'un processeur d'un système informatique effectue, pour chacun d'une pluralité de points (200) dans le ROI, les étapes suivantes :

15

a) étendre (201) une pluralité de rayons partant du certain point dans le ROI dans de multiples directions 3D par l'utilisation au moins de coordonnées d'un système de coordonnées de référence du point, en offrant une structure ayant une pluralité de rayons ayant une certaine géométrie ;

20

b) définir (202) une séquence de points d'échantillonnage sur chaque rayon de cette structure ;

c) configurer (203) la valeur de la distribution spatiale sur chaque point d'échantillonnage de chaque rayon de la structure ;

d) classifier (204) chaque rayon de la structure en attribuant à chaque rayon une seule valeur basée sur :

25

les valeurs configurées,

les positions absolues dans ce système de coordonnées de référence des points d'échantillonnage, et

les positions des points d'échantillonnage relatifs à chaque rayon de la structure offrant une valeur de rayon associée ; et

30

e) réduire (205) chaque structure à une seule valeur de point au vu de la géométrie des rayons et leur valeur de rayon associée, dans laquelle cette seule valeur de point est indicative de la structure spatiale locale de propriétés conductrices d'une région du tissu du muscle cardiaque.

35

2. La méthode de la revendication 1, dans laquelle la pluralité de points (200) sont des points d'échantillonnage sur un CC préalablement détecté ou des points d'échantillonnage étant contenus dans une partie ou le tout de ROI.

3. La méthode de la revendication 1, dans laquelle cette étape a) comporte en plus l'utilisation d'informations géométriques spécifiques du domaine du tissu du muscle cardiaque, ces informations géométriques spécifiques du domaine comprenant au moins une orientation de la paroi cardiaque du tissu du muscle cardiaque.

40

4. La méthode des revendications précédentes, dans laquelle :

cette technologie d'acquisition comporte une technologie d'acquisition d'image comportant au moins la tomographie assistée par ordinateur, CT, ou l'imagerie par résonance magnétique, MRI ; où

45

cette technologie d'acquisition comporte une technologie d'acquisition de données comprenant un instrument médical mesurant le voltage, par contact, du tissu du muscle cardiaque.

5. La méthode de la revendication 1, dans laquelle le ROI consiste en :

50

un volume 3D entouré par un collecteur topologique à 2 voies, la pluralité de rayons étant des segments en ligne droite à partir du certain point initial à une première portion d'intersection des rayons avec le collecteur ; où un maillage de surface triangulaire, la pluralité des rayons étant des segments en ligne droite à l'intérieur des triangles, ces segments étant joints aux bords triangulaires en partageant un point de bord et ayant les angles verticalement opposés égaux.

55

6. La méthode de la revendication 1, dans laquelle la séquence des points d'échantillonnage est limitée à une certaine longueur de la pluralité de rayons.

7. La méthode de la revendication 1 ou 6 dans laquelle la séquence de points d'échantillonnage est définie confor-

EP 3 441 937 B1

mément à une série de distances définies pour chaque rayon de la pluralité de rayons, cette série de distances comportant une séquence ayant une distance ascendante depuis le certain point initial.

5 8. La méthode de la revendication 4, dans laquelle cette distribution spatiale comporte différentes valeurs représentant la fonctionnalité électrique du tissu du muscle cardiaque, dans laquelle une première de ces différentes valeurs, ou Saine, représente le tissu ayant une fonctionnalité électrique normale ; une deuxième de ces valeurs différentes, ou Zone Limite, représente le tissu ayant un comportement électrique anormal ; et une troisième de ces différentes valeurs, ou Noyau, représente le tissu sans fonctionnalité électrique.

10 9. La méthode de la revendication 8, dans laquelle la valeur de rayon associée est fournie en parcourant les points d'échantillonnage et leurs valeurs associées depuis le certain point initial et en rapportant les informations sur le résultat d'une première valeur d'une certaine catégorie dans les catégories indiquées Saine, Zone Limite et Noyau.

15 10. La méthode de la revendication 8 ou 9, dans laquelle la valeur de rayon associée de chaque rayon est fournie conformément à la règle suivante :

si les valeurs correspondant à tous les points d'échantillonnage du rayon sont Zone Limite, alors la Zone Limite est attribuée ;
20 autrement, la valeur du point d'échantillonnage la plus rapprochée dont la valeur n'est pas Zone Limite est attribuée.

11. La méthode de la revendication 10, dans laquelle la valeur de seul point réduite est définie conformément à :

25 s'il y a au moins une valeur de rayon Saine, alors 0 ;
autrement, par :

le calcul d'un paramètre entourant le noyau comme fréquence relative pondérée de rayons noyaux ; et
le calcul de la valeur d'un seul point à partir du paramètre entourant le noyau en utilisant une fonction
30 linéaire proche et en rapprochant le résultat à un certain seuil inférieur ou supérieur.

12. La méthode de la revendication 1, dans laquelle l'étape e) est effectuée en faisant la moyenne des valeurs associées de chaque rayon en utilisant des poids dérivés de la géométrie des rayons ou en traitant statistiquement les fréquences relatives de la classification de rayons.

35 13. La méthode de la revendication 8, comportant en plus :

la création d'une image de volume de la valeur d'un seul point en attribuant à tous les voxels du ROI dont la valeur est Zone Limite, la valeur réduite obtenue dans l'étape e) et en attribuant à tous les voxels la valeur 0 ; et en réalisant un calcul complémentaire de marching cubes pour afficher l'image de volume créée ou en utilisant
40 l'image de volume créée pour un traitement ultérieur.

14. La méthode de la revendication 8, comportant en plus :

45 la création de points d'échantillonnage sur une certaine ligne centrale CC de sorte qu'il y ait des points d'échantillonnage sur chaque point d'extrémité et que la bifurcation et les segments de ligne entre les points d'échantillonnage soient suffisamment courts ; et
calculer la valeur de seul point à chacun de ces points d'échantillonnage créés, interpolés linéalement entre ces derniers ; et
intégrer numériquement la valeur de seul point sur toute la trajectoire de la ligne centrale de CC, en offrant une
50 valeur de seul point de ligne centrale.

15. La méthode de la revendication 10, comportant en plus :

55 enregistrer une distance à un point non Zone Limite, dans laquelle il n'y a pas de limite de longueur de rayon ; et effectuer une analyse directionnelle sur les rayons en appliquant une procédure statistique de celle-ci, la procédure statistique comprenant une Analyse de Composant Principal, PCA.

16. Un moyen lisible par ordinateur non transitoire comprenant des instructions de codes qui, lorsqu'elles sont exécutées

EP 3 441 937 B1

par un ordinateur, font que l'ordinateur effectue les étapes de la méthode d'une quelconque des revendications précédentes.

5

10

15

20

25

30

35

40

45

50

55

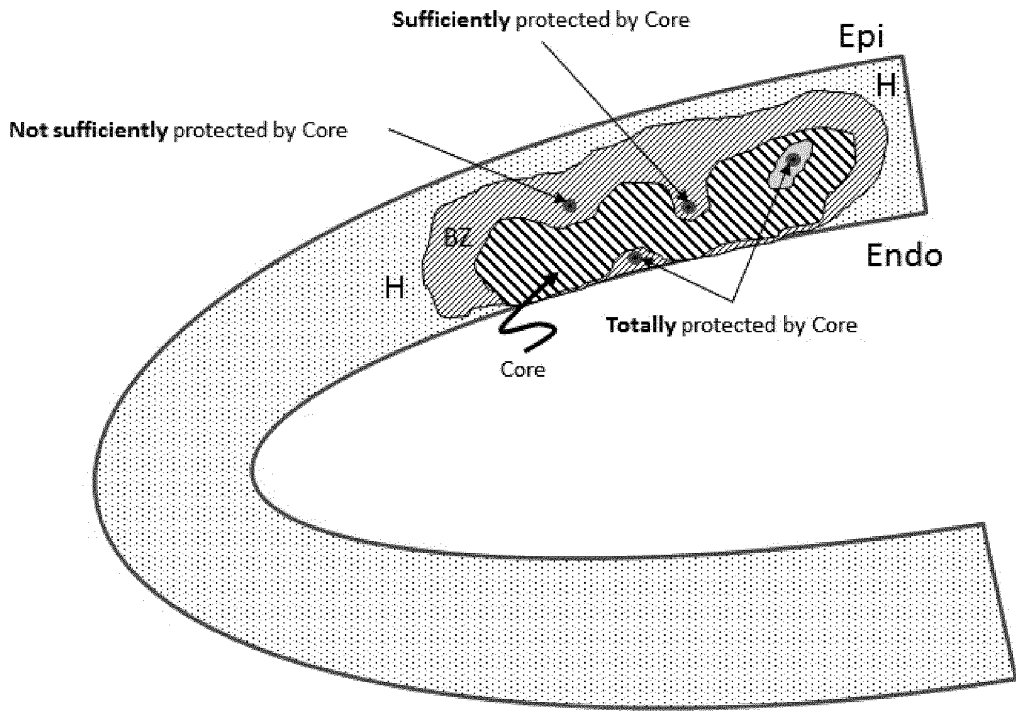


Fig. 1

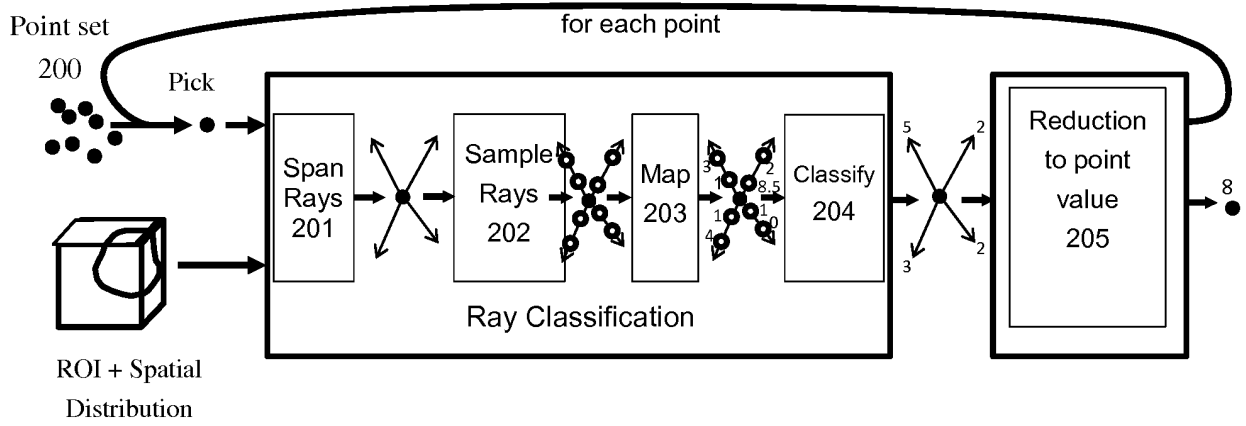


Fig. 2

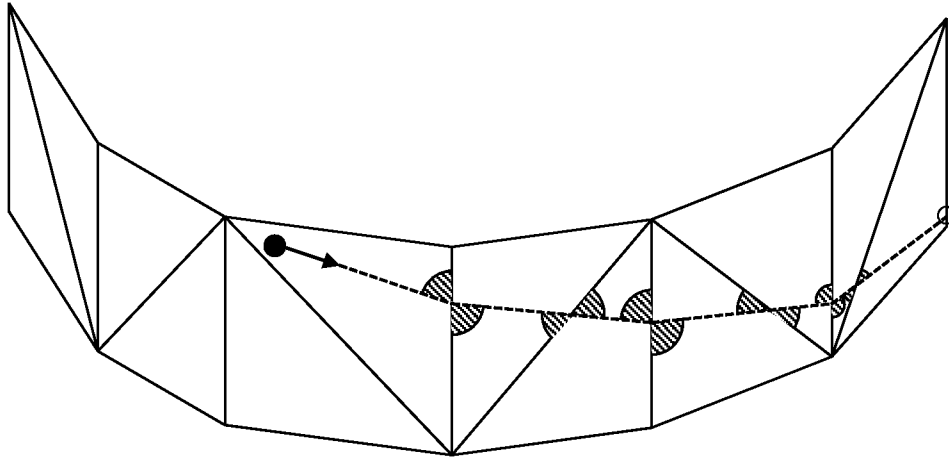


Fig. 3

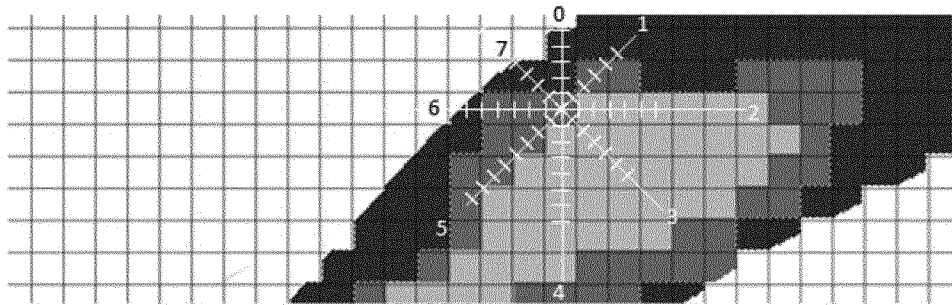


Fig. 4



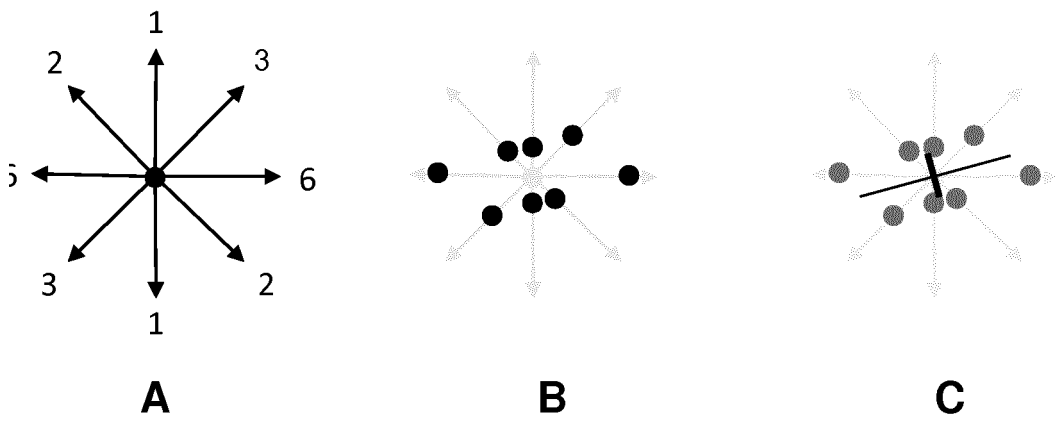


Fig. 5

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2017178403 A1 [0005]
- US 2017068796 A1 [0006]
- EP 2672889 A2 [0008]
- EP 2950270 B1 [0009]

Non-patent literature cited in the description

- **L. SERRA et al.** Identification of border-zone corridors in the left ventricle using the Core Expansion method. *Symposium on Medical Information Processing and Analysis, Pro. of SPIE*, 2017, vol. 10160 [0010]
- **J. M. COOK.** Technical Notes and Short Papers: Rational Formulae for the Production of a Spherically Symmetric Probability Distribution. *Mathematical Tables and Other Aids to Computation*, 1957, vol. 11, 81-82 [0101]
- **G. MARSAGLIA.** Choosing a Point from the Surface of a Sphere. *The Annals of Mathematical Statistics*, 1972, vol. 43 (2), 645-646 [0101]
- *Sphere Point Picking*, <http://mathworld.wolfram.com/SpherePointPicking.html> [0101]

专利名称(译)	计算心脏组织主导特性局部空间结构点的值的计算机实现方法及其计算机程序		
公开(公告)号	EP3441937B1	公开(公告)日	2020-04-22
申请号	EP2017382559	申请日	2017-08-08
[标]申请(专利权)人(译)	拉布拉多医疗 巴塞罗那大学		
申请(专利权)人(译)	拉布拉多医疗, S.L. 医院门诊部巴塞罗那 巴塞罗那大学		
当前申请(专利权)人(译)	医院门诊部巴塞罗那		
[标]发明人	STEGHOFER MARTIN SERRA DEL MOLINO LUIS PLANES CID JAVIER BERRUEZO SANCHEZ ANTONIO		
发明人	STEGHÖFER, MARTIN SERRA DEL MOLINO, LUIS PLANES CID, JAVIER BERRUEZO SÁNCHEZ, ANTONIO		
IPC分类号	G06T7/00 A61B5/00 A61B5/042 A61B5/055		
CPC分类号	A61B5/0044 A61B5/042 A61B5/055 A61B5/7264 G06T7/0012 G06T2207/10081 G06T2207/10088 G06T2207/30048 G06K9/3233 G06T15/06 G06T15/08		
其他公开文献	EP3441937A1		
外部链接	Espacenet		

摘要(译)

该方法包括在认为可能存在CC的情况下使用连续ROI，该ROI的每个点与给定空间分布的值相关联，该方法包括针对每个点（200）内的多个点（200）。ROI：使用每个点的参考坐标系的坐标在多个3-D方向上跨多个ROI内的多个射线（201），从而为结构提供多个具有给定几何形状的射线；在所述结构的每条射线上定义采样点的序列；将空间分布的值映射（203）在结构的每个射线的每个定义的采样点上；通过分配单个值对结构的每条射线进行分类（204），提供相关的射线值；鉴于所述几何形状及其相关的射线值，将每个结构减小（205）为单点值。

