




- (51) **International Patent Classification:**
A61B 5/097 (2006.01) *A61B 5/00* (2006.01)
A61B 5/08 (2006.01)
- (21) **International Application Number:**
PCT/US2012/071085
- (22) **International Filing Date:**
20 December 2012 (20.12.2012)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
61/578,811 21 December 2011 (21.12.2011) US
- (71) **Applicant:** CAPNIA, INC. [US/US]; 2445 Faber Place, Suite 250, Palo Alto, CA 94303 (US).
- (72) **Inventors:** WONDKA, Anthony, D.; 45 Plymouth Court, San Ramon, CA 94582 (US). BHATNAGAR, Anish; 916 Governors Bay Drive, Redwood City, CA 94065 (US).
- (74) **Agents:** O'SULLIVAN, Desmond, P. et al.; Morrison & Foerster LLP, 12531 High Bluff Drive, Suite 100, San Diego, CA 92130-2040 (US).
- (81) **Designated States** (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) **Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:
— without international search report and to be republished upon receipt of that report (Rule 48.2(g))

(54) **Title:** COLLECTION AND ANALYSIS OF A VOLUME OF EXHALED GAS WITH COMPENSATION FOR THE FREQUENCY OF A BREATHING PARAMETER

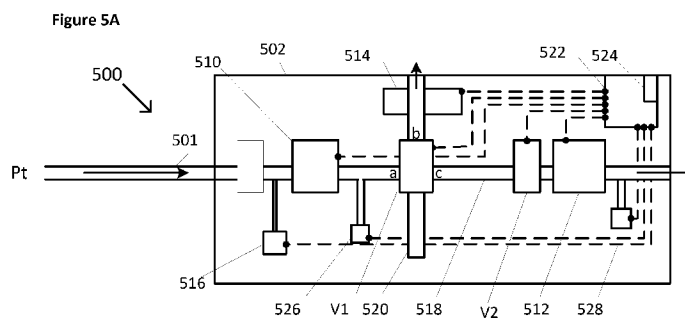

(57) **Abstract:** Apparatuses are described to accurately determine a gas concentration of a sample of a patient's breath. The apparatuses may include a sample compartment, a breath speed analyzer, a gas analyzer, and a processor. The sample compartment includes an inlet that receives the breath. The breath speed analyzer determines the speed of a portion of the breath. The gas analyzer determines a gas concentration. The processor includes an algorithm that determines a degree of non-homogeneity of the sample based on the speed, and a corrected gas concentration based on the degree of non-homogeneity. In some variations, the gas correction is determined independently of patient cooperation. Apparatuses may be tuned based on the intended population's expected breathing pattern ranges such that the sample compartment is filled with a homogenous end-tidal gas sample regardless of an individual's breathing pattern. These apparatuses are useful, for example, for end-tidal CO analysis. Methods are also described.



COLLECTION AND ANALYSIS OF A VOLUME OF EXHALED GAS WITH COMPENSATION FOR THE FREQUENCY OF A BREATHING PARAMETER

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Provisional Application No. 61/578,811, filed December 21, 2011, the disclosure of which is incorporated herein in its entirety.

FIELD OF THE INVENTION

[0002] Described here are devices and methods for the analysis of breath exhalant for diagnostic purposes. More specifically, devices and methods for sampling and analysis of gas from a person's breath for correlation to and diagnosis of an underlying physiologic condition are described.

BACKGROUND

[0003] There are two general techniques employed for obtaining a person's breath for gas analysis. In a first technique a person can cooperatively breathe into an instrument, which receives the gas for analysis. In a second technique an instrument can obtain a gas sample from the person's airway independent of the person's cooperation. In either technique, achieving a precise collection and precise analysis of a gas from a specific portion of the breathing cycle can be challenging, given the often random and erratic nature of a breathing pattern. For example, reliably measuring breath CO at exactly the end-tidal portion of exhalation, with high levels of accuracy and precision (for example <0.5ppm accuracy), has proven difficult. Typically, a measurement of breath CO₂ is used to determine the end-tidal portion of the breath, and gas from that portion of the breath can be sampled and analyzed accordingly. Using an end-tidal CO₂ signal is a convenient approach in that the technology is well known, and provides an instantaneous measurement of the breath waveform. However, in order to obtain accuracy and precision in the remainder of the overall system, the instrumentation considers only some of the possible external factors that may be useful.

[0004] Typically, a constant flow rate is employed for withdrawing the gas from the person, for a fixed collection time, and placing the drawn sample in a fixed volume sample compartment. When using this approach, there may be breath pattern related inaccuracies. For example, some of the sample compartment may have non-end-tidal gas in it, or only a fraction of the end-tidal portion of the breath might get sampled and stored in the sample compartment for analysis. While the repeatability at a certain breath rate is very good, the accuracy may vary as the breath rate varies, because of the pneumatics and timing of the system.

[0005] Therefore, it may be beneficial to improve on the accuracy of known systems in a way that is equally accurate across a range of breath patterns and breath rates. To this end, various approaches and algorithms have been conceived and described herein.

BRIEF SUMMARY

[0006] Described herein are breath gas analyzers that achieve an accurate compositional analysis of a breath-borne gas from a specific portion of a breath. The system can accommodate a wide range of breathing patterns and rates without losing accuracy. The system can assure that enough volume of gas is obtained for the analysis to be sufficiently accurate, and that the gas obtained is from the desired portion of the breath, and is representative of the entire desired portion of the breath. In some variations, these advantages are achieved by modulating the gas sampling flow rate depending on the breath pattern, and/or by obtaining gas samples from the desired portion of the breath for multiple breaths until a threshold volume of gas is obtained for analysis, and/or by applying a correction factor to the computed result to compensate for heterogeneity of the sampled gas. In addition to these methods for obtaining target volumes of gas, some variations may identify the desired portion of the breath in order to accurately sample the correct portion of the breath and/or tune the system to always collect for analysis a substantially homogeneously end-tidal sample regardless of breathing pattern.

[0007] To achieve the above features, variations of a breath analyzer or method for analyzing breath may include one or more of the following benefits: identification of different sub-portions of an expiratory phase; accurate sample collection from a desired sub-portion of the expiratory phase; assured collection of a predetermined quantity of gas

for analysis by a gas composition analyzer; reliability and repeatable for a wide variety of breathing patterns that are expected to be encountered.

[0008] In one variation, a method for breath analysis comprises measuring a time-related parameter of a person's breathing pattern, collecting gas from a target portion of at least one of the person's breaths into a sample compartment having a target volume, adjusting the gas collection based on the time-based-parameter, and analyzing the collected gas to determine a compositional parameter of the gas. In further variations, adjusting the gas collection can include at least one selected from the group consisting of: (1) adjusting the gas collection speed, (2) adjusting the number of breaths the gas is collected from, and (3) adjusting for the homogeneity of the collected gas with a correction factor. In yet further variations, the time-based-parameter comprises at least one parameter selected from the group consisting of: (1) breath rate, (2) end-tidal time period, (3) expiratory time period, (4) inspiratory time period, (5) breath period. In further variations, the target portion of the breath comprises the end-tidal portion and the compositional parameter comprises carbon monoxide. In further variations, the target portion of the breath comprises at least one phase selected from the group consisting of: (1) an expiratory phase; (2) an end-tidal phase; (3) a beginning portion of exhalation; (4) a middle portion of exhalation; (5) a last portion of exhalation; (6) a post-expiratory period; and (7) an inspiratory pause. In further variations, measuring a time-based parameter comprises at least one technique selected from the group consisting of: (1) capnometry, (2) monitoring airway pressure, (3) monitoring airway temperature, (4) monitoring airway flow, (5) plethysmography, (6) monitoring sound, and (7) monitoring exhaled oxygen. In yet further variations, the time-based-parameter is differentiated to determine a time period of a target breath portion. Further variations may include defining a start time and an end time for collecting the gas, wherein defining a start time and an end time comprises comparing the measured breath parameter against at least one selected from the group consisting of: (1) a threshold amplitude of the measured breath parameter; (2) a threshold time period of the measured breath parameter, (3) a peak value of the measured breath parameter, (4) a substantially zero value of the measured breath parameter, (5) a negative value of the measured breath parameter, (6) a change in slope of the measured breath parameter, and (7) a change in sign of the measured breath parameter. Other variations may include defining a start time and an end time for collecting the gas wherein defining a start time and an end time

comprises calculating a rate of change of the measured breath parameter and comparing it to at least one selected from the group consisting of: (1) a threshold value of the rate of change; (2) a zero value of the rate of change; (3) a first rate of change against a second rate of change; (4) a negative slope approaching zero; (5) a positive slope approaching zero; (6) a peak positive value of the rate of change; (7) a peak negative value of the rate of change; (8) an increasing rate of change; (9) a decreasing rate of change; and (10) a sign change of the rate of change. In further variations, collecting the gas further comprises applying a sampling cannula in communication with the sample compartment to the person's airway, and applying a vacuum to the sampling cannula. Further variations may include isolating the sample compartment with an inlet valve, and opening the inlet valve to begin collecting the gas from the target breath portion and closing the inlet valve to finish collecting the gas from the target breath portion. In further variations, the gas collected in the sample compartment comprises at least a portion of a breath from which the time-based breath parameter is measured. In further variations, the gas collected in the sample compartment comprises at least a portion of a breath that is not a breath from which the time-based breath parameter is measured.

[0009] In another variation, a method for breath analysis comprises identifying a time period of a portion of a breath, collecting a gas sample from the portion in a sample compartment having a target volume, wherein the gas sample is drawn into the compartment using a flow mechanism, and wherein a flow rate of the mechanism is based on the identified time period, and analyzing the collected gas sample for compositional analysis.

[0010] In another variation, a method for breath analysis comprises measuring an end-tidal time period of a person's breathing pattern with a breath sensor, collecting gas from the end-tidal period of at least one of the person's breaths into a sample compartment having a target volume with a flow mechanism, wherein the collection flow rate of the flow mechanism is adjusted based on the measured end-tidal time period and selected to substantially fill the target volume with gas from the end-tidal period, and analyzing the collected gas to determine a compositional parameter of the gas.

[0011] In another variation, a method for breath analysis comprises the steps (a) identifying a time period of a portion of a breath, (b) collecting a gas sample from the

portion in a sample compartment having a target volume, wherein the gas sample is drawn into the compartment using a flow mechanism, (c) wherein (a) and (b) are repeated for a number of times, wherein the number of times is determined at least in part by the identified time period, and (d) analyzing the collected gas sample for compositional analysis.

[0012] In another variation, a method for breath analysis comprises (a) measuring an end-tidal time period of a person's breathing pattern with a breath sensor, (b) collecting gas from the end-tidal period of the person's breath into a sample compartment having a target volume using a flow mechanism, (c) wherein (a) and (b) are repeated until the compartment is substantially filled with gas from end-tidal periods, and (d) analyzing the collected gas to determine a compositional parameter of the gas. In another variation, the method includes tuning the breath collection system to always collect a substantially homogeneously end-tidal sample, regardless of breathing pattern

[0013] Also described herein are various breath gas analyzers. In one variation, an apparatus for analyzing gas in a target portion of a person's breath cycle comprises a sample compartment of a target volume, a pneumatic system operable to collect gas from a person's breath and deliver the gas to the sample compartment, a breath sensor operable to measure a time-based-parameter of the target portion of the person's breath, a control system operable to adjust the pneumatic system based on the time-based-breath parameter, and an analyzer for analyzing the gas composition. In further variations, a gas flow system adjustment is provided that comprises at least one adjustment selected from the group consisting of: (1) an adjustable speed flow generator; (2) a processor configured to execute an algorithm that varies the number of breaths gas is collected from, and (3) a processor configured to execute an algorithm to adjust for the homogeneity of the collected gas with a correction factor. In further variations, the time-based-component comprises at least one component selected from the group consisting of: (1) a breath rate, (2) an end-tidal time period, (3) an expiratory time period, (4) an inspiratory time period, and (5) a breath period. In further variations, the target portion of the breath comprises the end-tidal portion and the gas analyzer comprises a carbon monoxide analyzer. In further variations, the target portion of the breath comprises at least one portion selected from the group consisting of: (1) an expiratory phase; (2) an

end-tidal phase; (3) a beginning portion of exhalation; (4) a middle portion of exhalation; (5) a last portion of exhalation; (6) a post expiratory phase; and (7) an inspiratory pause. In further variations, the breath sensor comprises at least one selected from the group consisting of: (1) a capnometer, (2) an airway pressure transducer, (3) an airway temperature sensor, (4) an airway flow sensor, (5) a plethysmograph, (6) a microphone, (7) an oxygen sensor, and (8) an ultrasonic sensor. In further variations, the apparatus further comprises (1) a differentiator adapted to differentiate the signal from the breath sensor and (2) a processor, wherein the processor executes an algorithm to correlate the differentiated signal to the target portion of the breath cycle. In further variations, the apparatus further comprises a processor, wherein the processor executes an algorithm to determine the start time and end time for collecting the gas, wherein the algorithm comprises a comparison of the measured breath parameter against at least one selected from the group consisting of: (1) a threshold value, (2) a threshold time period, (3) a peak value, (4) a substantially zero value, (5) a negative value, (6) a change in slope, and (7) a change in sign. In further variations, the apparatus comprises a differentiator to determine a rate-of-change of the measured breath parameter, and a processor to execute an algorithm, wherein the algorithm comprises a comparison of the rate of change with at least one selected from the group consisting of: (1) a threshold value; (2) a zero value; (3) a first rate of change against a second rate of change; (4) a negative slope approaching zero; (5) a positive slope approaching zero; (6) a peak positive value; (7) a peak negative value; (8) an increasing rate of change; (9) a decreasing rate of change; and (10) a sign change of the rate of change. In further variations, the apparatus further comprises a sampling cannula attachable at a first end to the gas analysis apparatus and engageable at a second end to the person's airway; and a flow generator adapted to draw gas from the person's airway through the sampling cannula to the sample compartment. In further variations, the apparatus comprises a valve system arranged to isolate the sample compartment, wherein the control system controls the valve system to permit gas from the target breath portion to enter the sample compartment. In further variations, the control system is further adapted to deliver gas to the sample compartment from the measured breath. In further variations, the control system is further adapted to deliver gas to the sample compartment from a breath after the measured breath.

[0014] In another variation, a breath gas analyzer for analyzing gas in a target portion of a person's breath comprises a breath sensor for identifying the target portion of the breath cycle, a processor for determining the time period of the target portion, wherein the time period is determined at least in part from the identified portion, a gas collection compartment of a target volume, a pneumatic system for delivering a gas sample from the target portion of the breath to the gas collection compartment, a control system for adjusting the gas delivery rate of the pneumatic system based on the determined time period, and a gas analyzer for analyzing the composition of the gas.

[0015] In another variation, a breath gas analyzer for analyzing gas in the end-tidal portion of a person's breath comprises a breath sensor for identifying the end-tidal period of the breath cycle, a processor for determining the time period of the end-tidal period, wherein the time period is determined at least in part from the identified portion, a gas collection compartment of a target volume, a vacuum source for drawing a gas sample from the end-tidal period of the breath to the gas collection compartment, a control system for adjusting the flow rate of the vacuum source based on the determined end-tidal time period to substantially fill the compartment with end-tidal gas, and a gas analyzer for analyzing the composition of the gas.

[0016] In another variation, a breath gas analyzer for analyzing gas in a target portion of a person's breath, comprises a breath sensor for identifying the target portion of the breath cycle, a processor for determining the time period of the target portion, wherein the time period is determined at least in part from the identified portion, a gas collection compartment of a target volume, a pneumatic system for delivering a gas sample from the target portion of the breath to the gas collection compartment, a control system and algorithm for controlling the pneumatic system to deliver gas until the compartment is substantially filled with gas from the target breath portion, and a gas analyzer for analyzing the composition of the gas.

[0017] In another variation, a breath gas analyzer for analyzing gas in a target portion of a person's breath comprises a breath sensor for identifying the target portion of the breath cycle, a processor for determining the time period of the target portion, wherein the time period is determined at least in part from the identified portion, a gas collection compartment of a target volume, a pneumatic system for capturing a gas sample from the

target portion of the breath into the gas collection compartment, a processor for executing an algorithm for applying a correction factor to the captured gas sample, wherein the correction factor is based on the determined time period of the target breath portion to correct for the non-homogeneity of the captured gas, and a gas analyzer for analyzing the composition of the gas.

[0018] In another variation, a method for breath analysis comprises (a) identifying a time period of an end-tidal portion of a breath, (b) collecting the end-tidal portion in a sample tube having a sample volume, wherein a time of collection is based on the identified time period, (c) repeating steps (a) and (b) until the sample volume is filled with a plurality of end-tidal portions from a respective plurality of breaths, and (d) analyzing the collected plurality of end-tidal portions to determine the concentration of a gas.

[0019] In another variation, a breath gas analyzer comprises a system operable to measure at least one characteristic of a patient's breath, a processor operable to determine a starting and an ending point of an end-tidal portion of the breath, wherein the determination is based upon the at least one characteristic, a sample tube comprising a proximal end, a distal end, a first valve coupled to the proximal end, a second valve coupled to the distal end, and a sample volume, wherein the sample volume is configured to store a plurality of end-tidal breath portions from a respective plurality of breaths, and a sensor for analyzing the concentration of a gas in the stored plurality of end-tidal breaths.

[0020] In another variation, a method of collecting an end-tidal portion of a patient's breath comprises identifying a starting point of the end-tidal portion, opening a container configured to collect the end-tidal portion, wherein the container is opened to correlate to the identified starting point of the end-tidal portion, identifying an ending point of the end-tidal portion, and closing the container, wherein the container is closed to correlate to the identified ending point of the end-tidal portion.

[0021] In another variation, a gas measurement correction database for determining a gas concentration at an inlet of an apparatus is populated by a method that may include measuring a plurality of gas concentrations in the apparatus for a respective plurality of known gas concentrations at the inlet (wherein the gas concentrations are measured at a

plurality of breath rates), deriving a first plurality of polynomial equations (wherein each of the first plurality of polynomial equations fits the measured gas concentrations of a respective one of the plurality of breath rates and wherein each of the first plurality of polynomial equations comprises a coefficient at each order of the equation), deriving a second plurality of polynomial equations (wherein each of the second plurality of polynomial equations fits the coefficients of a respective order of the first plurality of polynomial equations wherein each of the second plurality of polynomial equations comprises a coefficient at each order of the equation), and recording each of the coefficients of the second plurality of polynomial equations in the database. The first plurality of polynomial equations may comprise a plurality of linear equations. The plurality of breath rates may be at least five in number. The plurality of breath rates may include breath rates of 10 breaths per minute, 20 breaths per minute, 30 breaths per minute, 40 breaths per minute, and 50 breaths per minute. The second plurality of polynomial equations may comprise a plurality of quadratic equations. The coefficients of the second plurality of polynomial equations may comprise a first plurality of coefficients and a second plurality of coefficients, wherein the first plurality of coefficients correspond to breath rates at or below a predetermined breath rate and the second plurality of coefficients correspond to breath rates at or above the predetermined breath rate. The predetermined breath rate may be 30 bpm. The second plurality of polynomial equations may comprise a first plurality of quadratic equations and a second plurality of quadratic equations, wherein each of the first plurality of quadratic equations fits the first plurality of coefficients at each order, and wherein each of the second plurality of quadratic equations fits the second plurality of coefficients at each order. The plurality of known gas concentrations at the inlet may comprise three in number. The plurality of known gas concentrations at the inlet may comprise at least one selected from each of the following: a region of relatively low breath rate, a region of relatively high breath rate, and a region of intermediate breath rate.

[0022] In another variation, a method for determining a gas concentration of a patient's breath at an inlet of an apparatus may comprises determining a breath rate of the patient, measuring a gas concentration in the apparatus, accessing a database to obtain a first plurality of coefficients corresponding to the patient's breath rate, deriving a first plurality of polynomial equations based on the first plurality of coefficients, deriving a second

plurality of coefficients by inputting the breath rate into each of the first plurality of polynomial equations, deriving a compensation equation using the second plurality of coefficients, and determining the gas concentration at the inlet by inputting the measured gas concentration into the compensation equation. Each of the first plurality of polynomial equations may be a quadratic equation and the first plurality of coefficients may be three in number. The compensation equation may be linear and the second plurality of coefficients may be two in number. The database may include a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breath rates at or below a predetermined breath rate and the second subset of coefficients correspond to breath rates at or above the predetermined breath rate. The predetermined breath rate may be 30 bpm.

[0023] In another variation, an apparatus for analyzing a gas concentration of a patient's breath may comprise a gas analyzer that measures a gas concentration in the apparatus, an inlet that receives the patient's breath, a breath speed analyzer that determines a breathing parameter frequency of the patient's breath, a database comprising a plurality of coefficients corresponding to a plurality of breathing parameter frequencies, and a processor containing a non-transitory computer readable medium containing executable instructions that when executed perform a method of determining the gas concentration of the patient's breath at the inlet of the apparatus, wherein the method includes accessing the database to obtain a first plurality of coefficients based on the patient's breathing parameter frequency, deriving a first plurality of polynomial equations based on the first plurality of coefficients, deriving a second plurality of coefficients by inputting the breathing parameter frequency into each of the first plurality of polynomial equations, deriving a compensation equation using the second plurality of coefficients, and determining the inlet gas concentration by inputting the measured gas concentration into the compensation equation. The first plurality of polynomial equations may be a quadratic equation and the first plurality of coefficients may be three in number. The compensation equation may be linear and the second plurality of coefficients may be two in number. The database may comprise a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the

predetermined breathing parameter frequency. The predetermined breathing parameter frequency may be 30 bpm.

[0024] In another variation, a method for determining a gas concentration of a patient's breath at an inlet of an apparatus includes determining a breathing parameter frequency of the patient, measuring a gas concentration in the apparatus, accessing a database to obtain a plurality of coefficients based on whether the patient's breathing parameter frequency is at, above, or below a predetermined breathing parameter frequency, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below the predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency, deriving a compensation equation using the plurality of coefficients, and determining the gas concentration at the inlet by inputting the measured gas concentration into the compensation equation. The predetermined breathing parameter frequency may be 30 bpm.

[0025] In another variation, an apparatus for analyzing a gas concentration of a patient's breath may comprise a gas analyzer that measures a gas concentration in the apparatus, an inlet that receives the patient's breath, a breath speed analyzer that determines a breathing parameter frequency of the patient's breath, a database comprising a plurality of coefficients corresponding to a plurality of breathing parameter frequencies, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency, and a processor containing a non-transitory computer readable medium containing executable instructions that when executed perform a method of determining the gas concentration of the patient's breath at the inlet of the apparatus, the method including accessing the database to obtain a plurality of coefficients based on whether the patient's breathing parameter frequency is at, above, or below the predetermined breathing parameter frequency, deriving a compensation equation based on the plurality of coefficients, and determining the inlet gas

concentration by inputting the measured gas concentration into the compensation equation. The predetermined breathing parameter frequency may be 30 bpm.

[0026] In another variation, a method for determining a gas concentration of a patient's breath at an inlet of an apparatus may comprise determining a breathing parameter frequency of the patient, measuring a gas concentration in the apparatus, accessing a database to obtain a plurality of coefficients corresponding to the patient's breathing parameter frequency, deriving a compensation equation using the plurality of coefficients, and determining the gas concentration at the inlet by inputting the measured gas concentration into the compensation equation. The compensation equation may be a polynomial equation. The compensation equation may be linear. The database may comprise a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency. The predetermined breathing parameter frequency may be 30 bpm.

[0027] In another variation, an apparatus for analyzing a gas concentration of a patient's breath comprises a gas analyzer that measures a gas concentration in the apparatus, an inlet that receives the patient's breath, a breath speed analyzer that determines a breathing parameter frequency of the patient's breath, a database comprising a plurality of coefficients corresponding to a plurality of breathing parameter frequencies, and a processor containing a non-transitory computer readable medium containing executable instructions that when executed perform a method of determining the gas concentration of the patient's breath at the inlet of the apparatus, the method comprising accessing the database to obtain a plurality of coefficients based on the patient's breathing parameter frequency, deriving a compensation equation using the plurality of coefficients, and determining the inlet gas concentration by inputting the measured gas concentration into the compensation equation. The compensation equation may be a polynomial equation. The polynomial equation may be a linear equation. The database may comprise a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to

breathing parameter frequencies at or above the predetermined breathing parameter frequency. The predetermined breathing parameter frequency may be 30 bpm.

[0028] In another variation, an apparatus for collecting gas from a patient's breath comprises a sample volume, a flow generator comprising a sampling flow rate (wherein the flow generator may completely, or nearly completely, fill the sample volume with an end-tidal portion of the patient's breath when the patient's breath has a determined breathing parameter frequency), and a processor configured to discard a gas collected from the patient's if a breathing parameter frequency of the patient exceeds the predetermined breathing parameter frequency. The flow generator may be a pump. The end-tidal period of the patient's breath may be assumed to be a fraction such as one quarter of a breath period of the patient, wherein the breath period comprises one inspiratory and expiratory cycle of the patient's breath.

[0029] In another variations, an apparatus for analyzing a gas concentration of a sample of a patient's breath may comprise a sample compartment with an inlet that receives the patient's breath, a breath speed analyzer that determines the speed of a portion of the patient's breath, a gas analyzer that determines a gas concentration of the gas in the sample compartment, and a processor comprising an algorithm that determines a corrected gas concentration based on the speed of a portion of the patient's breath, wherein the corrected gas concentration is determined independently of patient cooperation.

[0030] In another variation, an apparatus for analyzing a gas concentration of a sample of a patient's breath may comprise a sample compartment with an inlet that receives the patient's breath, a breath speed analyzer that determines the speed of a portion of the patient's breath, a gas analyzer that determines a gas concentration of the gas in the sample compartment, and a processor comprising an algorithm, wherein the algorithm determines a degree of non-homogeneity of the breath sample in the sample compartment based on the speed of a portion of the patient's breath, wherein the algorithm determines a corrected gas concentration based on the degree of non-homogeneity, and wherein the corrected gas concentration is determined independently of patient cooperation.

[0031] In another variation, an apparatus for analyzing a gas concentration of a sample of a patient's breath may comprise a breathing parameter frequency measuring sensor, an algorithm comprising a defined maximum breathing parameter frequency, a sample compartment with a volume and with an inlet that receives the patient's breath, a gas analyzer that determines a gas concentration of the gas in the sample compartment, and a sampling flow rate control unit that delivers the sample from the patient into the sample compartment at a desired rate, wherein the sample compartment volume and the desired rate are determined based on the defined maximum breathing parameter frequency.

BRIEF DESCRIPTION OF THE DRAWINGS

[0032] Figure 1 graphically describes a typical breath waveform based on a carbon dioxide measurement taken on gas drawn from a breath.

[0033] Figure 2 graphically describes a typical breath waveform based on an airway pressure measurement taken at the proximal airway.

[0034] Figures 3A-3C graphically describe how breath CO may vary with the phase of the breath and one variation of using capnometry or airway pressure to identify the end-tidal period of the breath. Figure 3A describes the CO level in the breath for different phases of the breathing cycle. Figure 3B describes the CO₂ level in the breath for different phases of the breathing cycle and threshold values to identify the end-tidal period. Figure 3C describes the proximal airway breathing pressure for different phases of the breathing cycle and threshold values to identify the end-tidal period.

[0035] Figure 4A describes a capnometry signal for different phases of the breathing cycle and one variation of a differential of the signal for identifying different portions of the breath. Figure 4B describes an airway pressure signal for different phases of the breathing cycle and one variation of a differential of the signal for identifying different portions of the breath.

[0036] Figure 5A describes schematically an overview of one variation of a breath capturing system. Figure 5B describes schematically an overview of another variation of a breath capturing system.

[0037] Figure 6 provides a collection of graphs illustrating the phase shift associated with using capnometry to identify and collect a breath sample.

[0038] Figure 7 provides a collection of graphs illustrating the phase shift associated with using airway pressure monitoring to identify and collect a breath sample.

[0039] Figures 8-9G describe one variation of a breath analysis device using a breath rate correction factor to correct for breath rate related variations in the heterogeneity of the sampled gas, when using a fixed sampling flow rate with a fixed sampling time and a fixed sample collection tube volume. Figure 8 is a graph of a capnometry signal for a sequence of breaths. Figure 9A is a graph of a breath capnometry waveform representative of a nominal breath rate. Figure 9B is a graph of a breath capnometry waveform representative of a relatively fast breath rate. Figure 9C describes the system of Figures 5A or 5B capturing an end-tidal gas sample from the breath shown in Figure 9A. Figure 9D describes the system of Figures 5A or 5B capturing an end-tidal gas sample from the breath shown in Figure 9B. Figure 9E shows use of a breath rate correction factor to compensate for non-homogeneity of the captured gas sample, using a breath simulator and known CO gas input, with and without a correction factor applied. Figure 9F describes an alternate configuration of the system shown in Figure 9D in which the end-tidal sample is placed in the valve V1 side of the sample tube. Figure 9G describes the system of Figures 9C and 9D in which a breath is captured from a relatively slow breath rate.

[0040] Figures 10A-10B describe one variation of a method of modulated multiple breath sampling for capturing a targeted volume of end-tidal gas and subsequent gas analysis. Figure 10A is a schematic flow diagram describing the multiple breath sampling technique. Figure 10B illustrates a graph of the number of breaths that may be necessary to fill an exemplary sample volume for a series of breath rates.

[0041] Figures 11A-11F describe one variation of a breath-rate-modulated multiple breath sampling technique for capturing a targeted volume of end-tidal gas and subsequent gas analysis. Figure 11A graphically describes the capnometry signal and sample capture valve position, of an exemplary breath rate modulated multiple breath sampling protocol. Figures 11B-11F describe the pneumatic system described in Figures

5A or 5B for an exemplary end-tidal gas capture. Figure 11B describes the pneumatic gas capture system of Figure 5A or 5B with end-tidal gas from the first breath being captured. Figure 11C describes the pneumatic gas capture system of Figures 5A or 5B with the second breath being staged for capturing. Figure 11D describes the pneumatic gas capture system of Figures 5A or 5B with end-tidal gas from the second breath being captured. Figure 11E describes the pneumatic gas capture system of Figures 5A or 5B with the third breath being staged for capturing. Figure 11F describes the pneumatic gas capture systems of Figures 5A or 5B with end-tidal gas from the third breath being captured.

[0042] Figures 12A-B describe one variation of a method of modulated variable sampling flow rate for capturing a targeted volume of end-tidal gas and subsequent gas analysis. Figure 12A describes a schematic flow diagram of the sequence of operation of a breath-rate-modulated variable sampling flow rate technique. Figure 12B illustrates a graph of a sampling flow rate versus corresponding end-tidal time periods for an example sample volume.

[0043] Figures 13A-13F describe one variation of a breath-rate-modulated variable sampling flow rate technique for capturing a targeted volume of end-tidal gas for subsequent analysis. Figure 13A graphically describes a breath capnometry signal for a relatively fast breath rate. Figure 13B graphically describes a breath capnometry signal for a relatively slow breath rate. Figure 13C describes a pneumatic diagram of the gas collection system for the breath shown in Figure 13A for an exemplary end-tidal gas capture, adjusted to a relatively fast sampling flow rate. Figure 13D describes a pneumatic diagram of the gas collection system for the breath shown in Figure 13B, adjusted to a relatively slow sampling flow rate. Figure 13E describes using a capnometry signal to determine an average end-tidal time of previous breaths and a respective adjustment of the sampling flow rate to collect the targeted volume of end-tidal gas from a single subsequent breath. Figure 13F describes using an airway pressure signal to determine a projected end-tidal time from a measurement of a pre-end-tidal period, and a respective adjustment of the sampling flow rate to collect the targeted volume of end-tidal gas from the breath.

[0044] Figures 14A and 14B describe derivation and use of correction factor equations to adjust for the heterogeneity of end-tidal gas. Figure 14A is a graph illustrating ETCO ppm as a function of breath rate. Figure 14B provides a table with some exemplary breath rate correction factor equations.

[0045] Figure 15A illustrates a method for creating a look-up table to convert measured ETCO at a given breath rate to a corrected ETCO. Figure 15B provides a graph of ETCO accuracy. Figure 15C provides a graph comparing slope and offset to breath rate. Figure 15D provides a graph comparing slope and offset to breath rate. Figure 15E provides a look-up table and some exemplary compensation equations.

[0046] Figure 16A illustrates a method of determining a gas sampling rate of a flow generator to correlate to an upper limit breath rate and predetermined sampling volume. Figure 16B illustrates the pneumatic gas capture system of Figures 5A or 5B drawing a patient's breath at an upper limit breath rate. Figure 16C illustrates the pneumatic gas capture system of Figures 5A or 5B drawing a patient's breath at a breath rate below an upper limit breath rate.

DETAILED DESCRIPTION

[0047] Described here are devices and methods for capturing and analyzing an exhaled breath. In some variations, one or more breathing parameters are measured to identify the different constituent portions of a breath and the respective time periods, and a pneumatic system is used for capturing the portion of exhaled breath in a sampling tube using an identified time period. In some variations, one or more valves and/or flow control mechanisms—such as a vacuum pump, for example—are used to regulate the flow rate of gas drawn into the sampling tube. In some variations, the captured portion of breath is analyzed for indications of a patient's physiological state.

[0048] A portion of a breath may include an end-tidal portion, a beginning portion, a middle portion, and an end portion of an exhaled breath. Measured breathing parameters may include one or more of carbon dioxide, oxygen, airway pressure, airway temperature, breath flow rate, and breath pressure. Identifying the time period of a portion of a breath may include identifying approximately the start and termination of that time period.

[0049] In some variations of a multiple breath end-tidal sample collection algorithm, the number of samples collected varies with the breath rate, in order to fill a fixed sample collection volume with the complete end-tidal portion of the breath(s). In some variations of a variable sampling vacuum rate algorithm, vacuum rate is modulated based on a breath rate, allowing the sample collected to be the entire end-tidal section of the breath.

[0050] The composition of exhaled gas may vary corresponding to different stages of the expiratory period. For example, gas sampled near the end of exhalation may be representative of gas that has most recently diffused out of the blood stream into the alveoli. In the example shown in Figure 1, described below, the expiratory period is divided into two portions: pre-end-tidal and end-tidal. During the pre-end-tidal portion, gas from the conducting airways and from the distal portions of the lung are expelled, and during the end-tidal portion, gas that has freshly diffused into the alveolar volume is expelled. A diagnostic gas sample may be best taken from the end-tidal period, for example when attempting to diagnose a physiologic condition in the blood stream, such as hyperbilirubinemia or hemolysis. For explanatory purposes, exemplary variations for sampling end-tidal gas for end-tidal CO measurement are given below, however the principles apply to other diagnostic purposes.

[0051] Figure 1 graphically describes a typical breathing pattern 100 from the perspective of a carbon dioxide (CO₂) signal measured in breath drawn from the person's airway, such as from their nose, as a function of time, with time on the horizontal axis, and CO₂ level on the vertical axis. During the expiratory phase CO₂ is expelled, hence the CO₂ level increases. During the inspiratory phase, ambient air occupies the nose, hence the measured CO₂ drops to essentially zero. There may be a variety of shapes to a breath CO₂ curve, based on the person's breathing pattern, their age, how they are breathing and any underlying acute or chronic medical conditions. Some curves may show the following sub-portions for the expiratory phase: (1) a beginning portion of low or no CO₂ because the gas may simply be gas from the proximal airway devoid of CO₂, (2) a middle portion showing CO₂ rapidly increasing from zero to the CO₂ level at the distal segments of the lungs, (3) an end-portion showing a plateauing or leveling off of the CO₂, representing the CO₂ coming from the alveoli for that exhaled breath, and (4) potentially a constant peak level at the very end of the expiratory period. However, there can be

many other curves different from this classic curve. Peak CO₂ levels may be 4-6% during the end-tidal period and close to or equal to zero during the inspiratory period.

[0052] In some variations, the level of CO₂ in an exhaled breath is used to determine the duration of a period of a breath. In further variations, a duration of a period of breath may be characterized by a start and a termination of that period. In some variations, a CO₂ level is used to determine a start or a termination of a period of a breath. In other variations, a first time derivative of a CO₂ level is used to determine a start or a termination of a period of a breath. In yet other variations, a second time derivative of a CO₂ level is used to determine a start or a termination of a period of a breath. In some variations, a combination of CO₂ levels and CO₂ level time derivatives may be used to determine a start or a termination of a period of a breath. In some variations, a start of an end-tidal period may be determined by a change in the first time derivative of a CO₂ level of the exhaled breath, such as a sudden decrease in the first time derivative of the CO₂ level. In some variations, a decrease in the first time derivative of the CO₂ level is more than a 10% decrease. In some variations, a decrease in the first time derivative of the CO₂ level is more than a 25% decrease. In some variations, the derivative will approach or become zero showing very little rate of change or a peak plateau, respectively. In other variations, the start of an end-tidal period may be determined by a large second time derivative of the CO₂ level. In some variations, a termination of an end-tidal period may be determined by a maximum CO₂ level, which may be detected or confirmed by a change in the sign of the first time derivative of the CO₂ level as the derivative becomes negative (associated with a drop of the CO₂ level from its peak value). In further variations, a start of a beginning period may be determined by a sudden increase in the first time derivative of the CO₂ level. In other variations, the start of a beginning period may be determined by an increase in the CO₂ level from zero CO₂ level. In some variations, the increase in CO₂ level may be non-zero, such as near-zero or from a baseline. In some variations, a termination of a middle period may be determined by a change in the first time derivative of a CO₂ level of the exhaled breath, such as a sudden decrease in the first time derivative of the CO₂ level. In some variations, a CO₂ level, first time derivative thereof, second time derivative thereof, or a combination of the foregoing may be used to determine the start and termination of one or more periods.

[0053] Figure 2 graphically describes a typical breathing signal 200 from the perspective of measured airway pressure, showing a negative pressure during inspiratory phase and a positive pressure during expiratory phase. During at rest breathing, the peak expiratory pressure may correspond to the middle of the expiratory phase and the start of the end-tidal period. In Figures 1 and 2, TI, TE, TPET, TET, TPE represent inspiratory time, expiratory time, pre-end-tidal time, end-tidal time, and post expiratory time respectively. An inspiratory pause may also be present (not shown), in which lung muscle movement during inspiration is paused before the expiratory period begins. Peak inspiratory pressure may be -1 to -4 cwp during restful breathing, and up to -15 cwp during heavier breathing, and peak expiratory pressure may be +0.5 to +2.0 cwp during restful breathing and up to +10 cwp during heavier breathing when measured at the entrance to the nostrils. One of skill in the art will readily recognize that the cwps given here are exemplary and that other cwps may be present without deviating from the scope of this disclosure.

[0054] In some variations, airway pressure is used to determine a start or a termination of a period of a breath. In other variations, a first time derivative of an airway pressure is used to determine a start or a termination of a period of a breath. In yet other variations, a second time derivative of an airway pressure is used to determine a start or a termination of a period of a breath. In some variations, a combination of airway pressures and airway pressure time derivatives may be used to determine a start or a termination of a period of a breath. In some variations, a start of an end-tidal period is determined by maximum airway pressure, that is, by a zero first time derivative of the airway pressure. In some variations, a termination of an end-tidal period may be determined by zero airway pressure. In some variations, an airway pressure, first time derivative thereof, second time derivative thereof, or a combination of the foregoing may be used to determine the start and termination of one or more periods.

[0055] In some variations, the breath sensor monitors the person's breathing over time, and trends the breathing pattern by determining a continually updated value that is characteristic of the breathing pattern. For example, peak positive values of a breathing signal may be measured and updated for each breath. Peak values may be compared with previous peak values. Peak values may be averaged over a previous number of multiple breaths. Similarly, time-related aspects of the breaths may be trended, such as the

expiratory time. Various breath-related events that are not normal breaths may be identified and exception algorithms may exist in order to not include these non-normal breath events inadvertently in deterministic steps. For example, the characteristic waveform of a sneeze, cough, stacked breath, or non-full breath may be defined in advance or based on monitoring of a particular patient, and when detected by the breathing sensor, excepted from the appropriate deterministic algorithms.

[0056] Figures 3A-3C describe in more detail one variation of using a breath signal to identify a portion of the breath cycle for capturing a desired sample for compositional analysis. In the example shown, a capnometry signal or an airway pressure signal is used to identify the end-tidal portion of the expiratory phase for measurement of end-tidal CO₂. In Figure 3A, the breath CO₂ level 300 is represented, showing how CO₂ varies with the breath cycle, where the peak CO₂ value corresponds to the end-tidal period. The peak CO₂ value 310 is the value of interest, as it is the most closely correlated to the CO₂ level in the blood. In the capnometry example 330 in Figure 3B, time and amplitude threshold values are established to determine the beginning and end of the end-tidal period. YA and YB are the CO₂ amplitudes at the slope transition point and peak level respectively, representing the beginning and ending end-tidal CO₂ amplitudes respectively. XA and XB are the durations of the pre-end-tidal period and expiratory period respectively, measured from t1', the start of the expiratory period as defined by an increase from the baseline CO₂ level. Thresholds Y1, Y2, X1 and X2 can be respectively established from and based on trending, averaging, pattern recognition or other protocols of YA, YB, XA and XB, for example a percentage of a moving average trended value with exceptions disregarded. In the airway pressure example 360 of Figure 3C, YC represents the peak amplitude, corresponding to the start of the end-tidal period, and XA and XB represent the duration of the pre-end-tidal period and the expiratory period. Thresholds X1, X2 and Y1 are established from and based on trending, averaging, pattern recognition or other protocols of XA, XB and YC respectively, and threshold Y2 is established based on the zero pressure. For example, end-tidal gas sample collection can begin, with the appropriate phase shift, when nasal pressure reaches the peak value, or Y1, or at the midpoint of expiratory phase, XB/2, based on trending, reaches zero, and end when nasal pressure becomes negative, or zero, or when it reaches Y2, or after a time delay of XB, or after a time delay based on previously measured expiratory time. Measuring breathing

airflow or proximal airway temperature provides very similar information to airway pressure, and these signals can also be used in the manner previously described to determine the different portions of the breathing curve and the end-tidal period. In addition other breath measurements can be made to discern the breathing pattern, such as sound, ultrasound, vibrations, and plethysmography.

[0057] The threshold techniques described in Figures 3B and 3C can be highly reliable when the breath pattern is relatively constant and non-erratic. However, in non-constant or erratic breathing situations, capnometry and airway pressure may not reliably distinguish the beginning and end of the end-tidal period. For example capnometry may have difficulty in reliably identifying exactly the transition between the pre-end-tidal and end-tidal periods, because this transition may look different for different breathing patterns. For example, the slope of CO₂ increase during the expiratory phase may be constant without the transition point from a first slope to a second slope in Figure 3B. Or, there may be more than two CO₂ slopes during the expiratory phase hence more than one transition, making it potentially arbitrary to determine which slope transition corresponds to the beginning of the expiratory phase. The foregoing are merely examples of potential difficulties in identifying the beginning of the end-tidal period, and other issues are possible. A proximal airway pressure signal, with the appropriate algorithms, may improve reliability over capnometry in that rarely would there be more than one peak exhalation pressure for a given breath, making this marker a reliable marker. Similarly, the transition from positive pressure to zero pressure, with the appropriate zeroing algorithms, may reliability correlate to the end of the end-tidal period. Therefore, using proximal airway pressure sensing may provide enhanced fidelity and in addition may substantially lower cost. Nonetheless, airway pressure may also be limited in its fidelity.

[0058] Figures 4A and 4B indicate another variation using capnometry and proximal airway pressure to measure the breathing pattern and identify different portions of the breathing pattern, including the end-tidal period. Figure 4A is a graph 400 of exhaled carbon dioxide and the rate of change (first derivative) of exhaled carbon dioxide. (CO₂ is represented by line 410 and the derivative of CO₂ is represented by line 420.) In Figure 4A the breath CO₂ is measured and the measurement is differentiated instantaneously in real time. By observing instant changes in slope and comparing against the appropriate

threshold values (such as the threshold values described herein), the start of the end-tidal period can be reliably identified. And by observing rapid changes from a positive to a negative differentiated value, the end of the end-tidal period can be reliably identified. In addition to distinguishing the end-tidal period, other portions of the breath phase can be identified using this technique. In other variations, a second differential of the measured signal can be utilized to further improve the fidelity or reliability of identifying an exact portion of the breath pattern.

[0059] Figure 4B is another variation using measured proximal airway pressure, differentiated in real time. Figure 4B is a graph 450 of proximal airway pressure and the rate of change (first derivative) of the proximal airway pressure. (Airway pressure is represented by line 460 and the derivative of airway pressure is represented by line 470.) A first zero value 472 of dPA/dt subsequent to a positive value indicates the peak airway pressure at time t_2 corresponding to the start of the end-tidal period. A second zero value 474 of dPA/dt subsequent to a negative value indicates a zero airway pressure value at time t_3 corresponding to the end of the expiratory end-tidal period. In addition to manipulating a capnometry or airway pressure signal in this manner, other breath parameters can be likewise manipulated. Examples of such other parameters include breathing gas temperature, humidity, airflow, sound and others. Although end-tidal CO gas analysis is described in the examples herein, it should be understood the systems and methods can apply to sampling and analyzing other gases from other portions of the breathing cycle.

[0060] For some breath analysis applications, a minimum quantity of gas volume is required by the gas composition analyzer in order for it to provide an accurate analysis. One technique for obtaining the gas sample for analysis is to collect the gas in a temporary storage compartment while it is being drawn from the patient. The storage compartment is sized to a known volume to meet the volume requirement of the gas composition analyzer, and for convenience, the compartment can be a fixed or constant volume. After the compartment is filled with the desired gas, the gas in the compartment can then be sent to the composition analyzer for analysis. The gas stored and analyzed may be purely from the targeted portion of exhalation in order to achieve an accurate analysis. Therefore, the system may be capable of obtaining that volume of gas from the

correct part of the breath, under a wide variety of breathing patterns, and yet still collect the requisite quantity of gas for the analyzer to be accurate.

[0061] Figure 5A describes schematically an overview one variation of a device for capturing exhaled breath, including a sampling cannula 501 and a gas sample collection and analysis instrument 502. Gas may be drawn from the patient, for example using the sampling cannula 501 and a flow generator 512. The flow rate of the flow generator may be measured by a flow transducer, for example a pressure sensor array, 526 and 528, arranged similarly to pneumotach. The measured flow rate may be used as a closed loop feedback control to control the flow generator flow rate. A breath sensor, such as a capnometer 510 or a pressure sensor 526, may be used to measure the breathing pattern in real time. Gas from the desired portion of the breath is captured and isolated in the storage collection compartment 518. Gas entering the storage compartment is controlled by at least one valve V1, for example with a common port c always open, and a second open port, either a to collect gas or b to isolate the storage compartment. There may be a valve V2 between V1 and the flow generator to participate with V1 in isolating the storage compartment. Gas not being captured for analysis is channeled away from the storage compartment via a bypass conduit 520. The captured gas is sent from the storage compartment through a gas composition analyzer 514, such as a CO sensor. A control system 522 with a microprocessor 524 controls the system with the associated algorithms. The flow generator can be a vacuum or pressure pump, such as a diaphragm pump, or another type of flow generating device such as a vacuum source, a Venturi from a positive pressure source, or a syringe pump. Valves to manage gas routing can be an arrangement of 3 way 2 position valves or can be an arrangement of 4 way 3 position valves. Capnometer 510, if used, measures the breathing pattern instantaneously using infrared (IR). The gas composition analyzer can be an electrochemical sensor with a reaction time, or a gas chromatographer, or a mass spectrometer. Other variations may use different analyzers. The sample storage compartment can be a small bore inner diameter tube or conduit of considerable length in order to minimize the cross section which may reduce gas molecule interaction along the length of the conduit. The sampling cannula may be a silicone or PVC tube with an inner diameter of .020-.080". Pressure sensor 516 is an additional pressure sensor that may be used in tandem with 526 so that a flow rate can be determined, in addition to using it for airway pressure measurement.

Flow rate can be used to adjust the pump speed in some variations that utilize a variable flow rate. Pressure sensor 516 can also be utilized for ambient information where the breathing curve is measured by pressure instead of capnometry. In some variations, an instantaneous carbon monoxide sensor is used as the breath sensor, in place of a capnometer or an airway pressure sensor. Other instantaneous breath sensors may also be used.

[0062] Figure 5B describes additional details about the pneumatic operation of the system shown in Figure 5A (see also Figure 9C below). For similar features in Figure 5A, a discussion is not repeated here. A bypass tube 536 allows the gas being drawn from the patient or from ambient to bypass the sample tube 518 during times which the sample tube may be isolated from these gases. In this arrangement, valve V1 may be closed at port a and valve V2 may be open at port b to allow flow from b through c. A flow generator may be used to draw the sampling gas through the bypass type. A push tube 532 may be used to push the end-tidal sample in the sample tube 518 out of the sample tube to the sensor 514, at which time valves V1 and V3 are each open at port b and V2 is closed at port a. Valve V4 switches the source gas from patient gas to ambient gas by opening port b, when it is desired to not contaminate the internal gas pathways with patient gas or for purging the system.

[0063] In some variations, the pneumatic system shown in Figures 5A and 5B above may include a removable sampling compartment (not shown). For example, sample tube 518 may be removable from the system. In this way, the pneumatic system may be able to fill a sample tube with a desired gas, and the sample tube may be analyzed at another location, or preserved for later analysis. In other variations, the gas may be routed from the sample tube to a removable sampling compartment. In this variation, the compartment may replace the analyzer or otherwise be positioned so that it can be removed and/or replaced.

[0064] Figure 6 provides a collection 600 of graphs illustrating the phase shift associated with using capnometry to identify and collect a breath sample in one variation of a device for capturing exhaled breath. The top graph 610 illustrates actual breath phase (inspiration/expiration). The middle graph 630 illustrates CO₂ concentration. The bottom graph 660 illustrates valve position. The travel time for gas to travel from the person to

the capnometer through the sampling cannula is represented by $t\alpha$. Therefore the capnometry signal shows a beginning of exhalation slightly after the true beginning of exhalation. The travel time for the gas to exit the capnometer and begin to enter the sample collection compartment is represented by $t\beta$. Therefore the sample compartment isolation valve V1 opens to position at a time $t(1)$, $t\beta$ after detection of the start of the end-tidal period by the capnometer, for the sample collection time $t(s)$.

[0065] Figure 7 provides a collection 700 of graphs illustrating the phase shift associated with using airway pressure monitoring to identify and collect a breath sample in one variation of a device for capturing exhaled breath. The top graph 710 illustrates actual breath phase (inspiration/expiration). The middle graph 730 illustrates airway pressure. The bottom graph 750 illustrates valve position. The phase shift between the actual breath, and the pressure is $t\phi$, approximately equal to the distance of travel divided by the speed of sound, hence is relatively instantaneous. The travel time for the gas to exit the person's airway and begin to enter the sample collection compartment is represented by $t\delta$. Therefore the valve V1 opens to position a at time $t(1')$, which is $t\delta$ after detection of the start of the end-tidal period by the capnometer, for the sample collection time $t(s)$.

[0066] In the following discussion, reference is made to the device for capturing exhaled breath described above with respect to Figures 5A and 5B. It should be noted that other devices could be used to determine a duration of a period of an exhaled breath and capture that period of breath without deviating from the scope of the disclosure.

[0067] In a first variation of a breath-rate-modulated variable, shown in Figures 8-9G, a correction factor is applied to the gas composition analysis result to compensate for non-homogeneity of the captured gas sample. The system in the example shown analyzes end-tidal CO gas by identifying the end-tidal period using capnometry, and uses a fixed gas sampling time and sampling flow rate. Figure 8 is a graph 800 of a capnometry signal for a series of breaths. The capnometry signal is used to identify a good breath to sample and to identify the end-tidal period, with the most recent breath on the right end, and the oldest breath on the left end of the graph. Breaths 1 through 3 are monitored and assessed for meeting a qualification criteria, and if met, the end-tidal portion of breath 4 is sampled for analysis.

[0068] Figure 9A is a graph 900 of a nominal case corresponding to Figure 8 in which breath number 4's end-tidal period matches the sampling time $t(s1)$. Figure 9C illustrates the arrangement 930 of a pneumatic system for capturing the gas described in the nominal case shown in Figure 9A, in which gas from the end-tidal period of Breath 4 completely fills the sample collection compartment volume $V(s1)$. In Figure 9C, the pre-end tidal of Breath 4 can be seen to the right of $V2$, out of the sample compartment. The inspiratory portion of Breath 5 can be seen to the left of $V1$, out of the sample compartment.

[0069] In the graph 910 of Figure 9B, the sampling time $t(s1)$ is greater than the end-tidal period. The arrangement 940 shown in Figure 9D, corresponding to the graph of Figure 9B, comprises both end-tidal gas from breath 4 and inspiratory gas from breath 5. For example, if the system is tuned for a 1 second end-tidal time with a sample collection time of 1 second, and the actual end-tidal time is 1 second, then the sample gas is homogeneous with respect to the different portions of the expiratory phase, and the analysis may be most accurate (see Figures 9A and 9C). However, if the person's end-tidal period becomes shorter or longer in duration, the sample compartment may miss some of the end-tidal gas or may include some non-end-tidal gas, respectively, which may inevitably lead to inaccuracies in the analysis, which can be corrected for by application of the gas heterogeneity breath-rate correction factor. For example, if the end-tidal time is 0.5 seconds, the sample compartment may be 50% filled with pure end-tidal gas from the entire end-tidal period plus 50% filled with inspiratory gas, thereby diluting the concentration of the CO in the sample compartment. Assuming the CO of the gas sample from inspiratory phase is known, for example 0.25ppm, and assuming the analyzer's measurement result is 1.25ppm CO, and the known ambient CO is 0.25ppm, then the sample contains 50% of 0.0ppm CO, and 50% of 1.0ppm CO for a corrected CO of 0.5ppm CO. In this case the correction factor is .5. In the example shown in Figure 9B, the sampling time $t(s1)$ is greater than the end-tidal period. The captured gas sample shown in Figure 9D corresponding to Figure 9B comprises both end-tidal gas from breath 4 and inspiratory gas from the next breath.

[0070] The resultant CO analysis at 60 bpm shown by the solid line in the graph in Figure 9E shows a 15% error due to dilution of the sample, however application of the breath rate dependent correction factor shown by the dotted line achieves 2% accuracy in this

example. The correction factor may be a linear equation with a slope and offset value applied to all breath rates across the operating range of the device.

[0071] Figure 9E describes a graph 950 of accuracy versus breath rate from an end-tidal CO analyzer, using a breath simulator and a known CO gas concentration input, and a mathematical correction formula. The solid curve in the graph 950 in Figure 9E at 40 bpm describes the resulting accuracy of the CO analysis of the sample collected. In the example shown, the sample tube volume and gas sample flow rate are sized and set respectively to completely fill the sample tube of end-tidal gas from the complete end-tidal period, for an end-tidal period of 500 milliseconds corresponding to 30 breaths per minute with a 1:1 I:E ratio (“Inspiratory: Expiratory”). As can be seen in the graph, the curve is very accurate at breath rates below 30 bpm, because at 30 bpm the sample tube is completely filled with homogenous end-tidal gas, and below 30 bpm, the sample tube is also filled with homogenous end-tidal gas, although not from the entire end-tidal period. However, above 30 bpm, the sample tube comprises gas from the entire end-tidal period of the breath sampled, plus some gas from before or after the end-tidal period because the end-tidal periods at these breath rates are shorter in duration than the gas sampling time, therefore resulting in a negative slope in the curve due to the dilution. As can be seen in the corrected curve, the results at breath rates greater than 30 are accurately adjusted with the correction factor. The accuracy between 10 and 30 bpm may not be linear because at 10 bpm the sample tube contains the very end of the end-tidal gas, which might be slightly higher in CO concentration than the average throughout the end-tidal period, whereas at 30 bpm, the sample tube contains the gas from the entire end-tidal period. The general equation describing the relationship between measured and actual gas is $x = My + B$, for example $x = 0.0074y + 0.07$, where x is the measured ETCO, M is the slope of the equation, y is breath rate corrected ETCO, and B is the equation y intercept or offset. Therefore $ETCO_{(corrected)} = [ETCO_{(measured)} - \text{offset}] / \text{slope}$.

[0072] Figure 9F describes an alternate configuration 960 of the system shown in Figure 9D in which the end-tidal sample is placed in the valve V1 side of the sample tube. This is a similar configuration to Figure 9D, except a portion of the expiratory end-tidal period of breath 4 is captured in the sample instead of the inspiratory phase (as shown in the configuration of Figure 9D). Figure 9G illustrates configuration 970 of the system of

Figures 9C and 9D in which a breath is captured from a slow breath rate. In the configuration of Figure 9G, some end-tidal gas is not captured in the sample tube in the area past V2.

[0073] Figure 10A illustrates a method 1000 for sampling multiple breaths to collect a targeted volume of end-tidal gas. Method 1000 optionally begins with step 1002, flushing the system with ambient air. This may not be necessary every time the method is performed. Method 1000 continues with collecting a first end-tidal sample 1004. A valve on a sampling tube is opened at the appropriate time to correlate with the beginning of the end-tidal period. The variation depicted in Figure 10A indicates the valve is open to correlate with a second plateau of the first derivative of the carbon dioxide concentration, but other variations may use alternative triggers for the beginning of the end-tidal period, such as those described in this disclosure. The valve on a sampling tube is closed at the appropriate time to correlate with the end of the end-tidal period. The variation depicted in Figure 10A indicates the valve is closed to correlate with a zero of the first derivative of the carbon dioxide concentration, but other variations may use alternative triggers for the end of the end-tidal period, such as those described in this disclosure. The method with step 1006 to determine the volume of gas captured in step 1004. The variation depicted in Figure 10A indicates the volume based on the pump speed and valve open time, but other mechanisms could equivalently be used. The captured volume is then compared to the sample tube volume to determine if the sample tube is filled. If not, Step 1008 repeats the capturing step of 1004 and the comparison of step 1006 until the sample volume is filled. Then the method, in step 1010, pushes the collected volume to a CO analyzer. In some variations, the collected volume may be pushed to a different type of gas analyzer, or pushed to a removable storage tube for delivery to a lab or other analyzing facility.

[0074] As described above, in order to compensate for any breath rate or breath pattern and still obtain the desired sample volume and gas purity, multiple breaths may be sampled. The number of breaths will depend on the breath pattern and the compartment volume. Figure 10B illustrates a graph 1020 of the number of breaths that may be necessary to fill a sample volume. For exemplary purposes, the sample compartment is 2.5ml, the sample flow rate is 100ml/min, and assuming end-tidal gas is being analyzed, 3

breaths are needed to be sampled for example at a breath rate of 30 breaths per minute, etc. It should be understood that varying the sample compartment, flow rate, etc. may lead to a different graph. Graph 1020 provides an easy reference to determine how many breaths may be necessary to fill the compartment tube. Although the variation of Figure 10B depicts breaths sampled as whole numbers (and, thus, a step-function graph), other variations may use a continuous graph line, thereby indicating that a partial breath (in addition to one or more full breaths) will be captured to fill the sample volume. This information may be utilized to close the sample compartment valve at an appropriate time.

[0075] Figures 11A-11F graphically describe the method of Figures 10A-10B using the apparatus of Figure 5A or 5B, for explanatory purposes. It should be noted that any number of apparatuses could be used to capture a specific portion of breath without deviating from the scope of the present disclosure.

[0076] Figure 11A illustrates a graph 1100 showing the carbon dioxide levels of a series of breaths. After identifying and assessing the first three breaths, the system decides to begin collecting samples from the fourth breath, labeled breath 1. Depending on the prevailing breath pattern, the appropriate number of end-tidal periods are sampled to collect the requisite volume. The breaths may be first verified that they meet necessary criteria for sampling, resulting in either multiple consecutive breaths, or non-consecutive breaths. Figure 11A also illustrates a graph 1105 of the valve state of the valve V1 on the inlet to the sample tube. While the first three breaths (“breath -3” to “breath -1”) are verified, the inlet to the sample tube is closed (“b open”). When the system determines to sample breath 1, the inlet to the valve is opened (“a open”) to allow the sample tube to collect the end-tidal period of breath 1. As can be seen in Figure 11A, there is a phase shift (time offset) from the beginning of the end-tidal period to the opening of the inlet valve. This may reflect a finite time required for the breath to travel from the patient to the inlet valve, as described above. When the end-tidal period is over, the inlet valve is again closed. The open and closing of the inlet valve is then repeated for two further breaths.

[0077] After storing each sample, before the next sample is stored, the gas being drawn from the patient is channeled to bypass the storage compartment. These configurations of

the system is illustrated in Figures 11B to 11F. In configuration 1110 of Figure 11B, gas from the first breath's end-tidal phase begins to be stored in the sample tube. In configuration 1120 of Figure 11C, the gas after the first breath's end-tidal phase (i.e., the second breath's inspiratory and pre-end tidal phases) is channeled through the bypass tube. In configuration 1130 of Figure 11D, gas from the second breath's end-tidal phase begins to be stored in the compartment. In configuration 1140 of Figure 11E, the gas after the second breath's end-tidal phase (i.e., the third breath's inspiratory and pre-end tidal phases) is channeled through the bypass tube. In configuration 1150 of Figure 11F, gas from a third breath's end-tidal phase begins to be stored in the compartment, after which the compartment is completely filled with pure end-tidal gas from multiple breaths. After this, sample collection can end, and the gas in the storage compartment can be sent to the gas analyzer for compositional analysis. In one variation the sample compartment can be volumetrically sized for a gas sample drawn from a single end-tidal period that is associated with the longest possible end-tidal duration imaginable. All other breath rates will result in sampling gas from more than one breath. In a further variation, in some clinical applications it might be desired to size the storage compartment so that the system always samples at least a few breaths or samples breathing for at least 30 seconds, in order to collect an average reading over a period of time, to dampen the effect of any breath-to-breath perturbations in the actual gas composition.

[0078] Figures 12A illustrates a method 1200 of capturing a breath using a variable pump speed to collect a targeted volume of end-tidal gas. Method 1200 optionally begins with step 1202, flushing the system with ambient air. This may not be necessary every time the method is performed. Method 1200 continues with measuring an end-expiratory time 1204. In the variation of method 1200, the end-expiratory time could be measured using a capnometry signal, differential of capnometry signal, or a pressure signal. In other variations, the end-expiratory time could be measured in a different way, such as those described herein. Method 1200 then continues with step 1206, adjusting the speed of the pump based on the measured end-expiratory time in step 1204. Method 1200 then continues to step 1208, where the valve is opened when an end-tidal sample reaches the valve. The valve may remain open for the duration of the measured end-tidal time, and then is shut to capture the sample when the end-tidal time has passed. Then the method, in step 1210, pushes the collected volume to a CO analyzer. In some variations, the

collected volume may be pushed to a different type of gas analyzer, or pushed to a removable storage tube for delivery to a lab or other analyzing facility.

[0079] As described above, in order to compensate for any breath rate or breath pattern variability and still obtain the desired sample volume, the sample flow rate may be adjusted. Figure 12B illustrates a graph 1220 of a sampling flow rate that corresponds to an end-tidal period. For exemplary purposes, the sample storage compartment is 1.25ml and the end-tidal portion of a particular breath is 1 second in duration. In that example, the sample flow rate is adjusted to be 1.25ml/second or 75ml/minute in order to collect a 1.25ml sample of gas sampled from the complete end-tidal period. It should be understood that varying the sample compartment, flow rate, etc. may lead to a different graph.

[0080] Figures 13A-13F describe the method of Figures 12A-12B using the apparatus of Figures 5A or 5B, with two breathing cases for comparison. It should be noted that any number of apparatuses could be used to capture a specific portion of breath without deviating from the scope of the present disclosure. Graph 1300 in Figure 13A represents "Case A," a relatively fast breath. Graph 1310 in Figure 13B represents "Case B," a relatively slow breath. Case A and B result in relatively short and long end-tidal times respectively. In configurations 1320 and 1330 of Figures 13C and 13D, respectively, the system has a fixed sample compartment volume, $V(s)$, for example 1.0ml. It will be understood that other volumes of sample tubes may be used without deviating from the scope of the disclosure. In Case A (Figures 13A and 13C), the end-tidal duration is 0.4 seconds and hence the sampling flow rate is adjusted to 150ml/min, in order to draw a 1.0ml gas sample in 0.4 seconds. In Case B (Figures 13B and 13D), the end-tidal duration is 0.833 seconds and hence the sampling flow rate is adjusted to 50ml/min in order to draw a 1.0ml gas sample in 0.833 seconds. Therefore, in both Case A and B, the entire end-tidal period is sampled for analysis, rather than just a portion of the end-tidal period, and the sample collection compartment contains pure end-tidal gas and is 100% filled with end-tidal gas. The correct amount of gas, 1ml, may be sent to the gas CO analyzer in both cases for an accurate analysis. In other embodiments, the gas may be pushed to a different type of gas analyzer, or pushed to a removable storage tube for delivery to a lab or other analyzing facility. The speed of the pump can be precisely

regulated by modulating the voltage or current driving the pump, based on look up tables in associated software. In some embodiments, the speed of the pump may be precisely regulated using a closed loop feedback control system by measuring the flow rate of the fluid, for example using a pneumotach as described in Figure 5A and 5B, and adjusting the speed of the pump by adjusting the current based on the measured flow rate. In some embodiments, a look up table may be used to apply a current to the pump depending on the desired flow rate, then, in addition, a pneumotach feedback loop may be used to make fine adjustments to the current to precisely obtain the exact flow rate needed.

[0081] Figure 13E illustrates a graph 1340 which describes the variable sampling flow rate technique of Figure 12A when capnometry is used to measure the breathing pattern, showing a series of breaths with the most recent breath on the right end of the graph. After determination of an average end-tidal time from a series of preceding breaths (Breaths 1-3), the sample flow rate is adjusted from a baseline default sampling flow rate of $Q(d)$ to sampling flow rate of $Q(s)$, equal to the compartment volume $V(s1)$ divided by the projected end-tidal time or sampling time $t(s)$. Using the closed loop control of the flow generator, the flow is fine tune adjusted until it equals $Q(s)$ (during Breath 4). Then gas from the end-tidal period of a subsequent breath (Breath 5) is drawn at flow rate $Q(s)$ and brought into the sample collection compartment. Additionally, the end-tidal time of the breath that was sampled can be measured to confirm it was equal to $t(s)$ in order to validate the integrity of the sample. If the breath was erratic not conforming to $t(s)$, then the sample can be discarded and the procedure repeated.

[0082] Figure 13F illustrates a graph 1350 which describes the variable sampling flow rate technique of Figure 12A when using airway pressure to measure the breathing pattern, showing a series of breaths with the most recent breath on the right end of the graph. In the example shown, end-tidal gas from breath 3 is sampled for analysis. The sample flow rate can be adjusted in a variety of ways. In one variation, the end-tidal time can be predicted from earlier breaths and the flow rate adjusted accordingly prior to drawing the sample from the targeted breath. In other variations, an adjustment to the flow rate can be made instantaneously based on the pre-end-tidal duration $T(e)$ after $T(e)$ is measured and known.

[0083] In some variations, a measured gas concentration may be adjusted to approximate an actual gas concentration. Such adjustments may account for variations in the fidelity of a breath sampling apparatus over a range of breath rates. The measured concentration may be modified using a correction equation, which may be specific to the apparatus being used, but may also be usable across various apparatuses. In some variations, the correction equation is formulated to cover a range of breath rates. In some variations, a breath rate and a measurement of a gas concentration in the apparatus may be sufficient to approximate the actual concentration of the gas at an inlet of the apparatus using a correction equation.

[0084] Figure 14A is a graph 1400 illustrating ETCO ppm as a function of breath rate. In the example shown the actual ETCO ppm is 4.1 ppm. Graph 1400 depicts three curves: a measured value, a breath rate corrected value, and an actual value. The actual value may represent a gas concentration at the inlet to a breath sampling apparatus. The measured value may represent a gas concentration measured at another point in the breath sampling apparatus, such as an outlet. The breath rate corrected value may represent the measured value of the gas concentration after it has been adjusted. To generate graph 1400, four measurements of gas concentration may be taken for four breath rates: 10 bpm, 30 bpm, 40 bpm, and 60 bpm. As graph 1400 illustrates, the breath rate corrected value approximates or matches the actual value. The breath rate may be corrected using one or more breath rate correction factor equations.

[0085] Table 1420 in Figure 14B provides some exemplary breath rate correction factor equations. Each equation relates the measured gas concentration (y) to the breath rate (x). In one variation, the breath rate correction factor equation is linear. In further variations, the breath rate correction factor comprises multiple linear equations, with each equation providing a correction for a specific range of breath rates. Using different ranges may improve the fidelity of the correction. In another variation, the breath rate correction factor equation is a quadratic equation. In further variations, multiple quadratic equations may be used for multiple breath rate ranges.

[0086] In some variations, the coefficients of a linear or quadratic equation are determined by using a breath simulator. In such variations, the breath simulator provides a known concentration of a gas at the inlet to a breath sampling apparatus at a known

breath rate. From the breath rate and the deviation of measured gas concentration at another location of the sampling apparatus from known gas concentration at the inlet, a rate factor equation is derived by fitting the measurements to an equation. For example, the embodiment depicted in Figure 14A may provide a deviation for each discrete breath rate. The deviation at each breath rate can be extrapolated to produce one or more equations spanning the operating range. In this way, a measured gas concentration can be corrected to approximate an actual gas concentration for any breath rate within the operating range.

[0087] Further variations may provide adjustments for a range of measured gas concentrations to a range of corrected gas concentrations over a range of breath rates. In one variation, a method for deriving a breath rate correction equation may include deriving multiple polynomial equations that span the ranges of measured gas concentrations, actual gas concentrations, and breath rates and utilizing the polynomial equations to populate a look-up table. In other variations, an apparatus may include a processor that references a look-up table to determine a polynomial equation for a given breath rate, where the polynomial equation provides a corrected gas concentration for a measured gas concentration at the given breath rate. In this way, variations of the present disclosure may beneficially provide for determining a gas concentration in a patient's breath independently of patient cooperation. That is, the gas concentration may be determined for patients who are unwilling or unable to regulate their breathing to correlate to a "normal" breathing pattern.

[0088] Figure 15A illustrates method 1500 for creating a look-up table to convert measured ETCO at a given breath rate to a corrected ETCO, in accordance with one variation. The method may begin by establishing ETCO accuracy for discrete breath rates and for discrete known gas concentrations (step 1502). In the variation shown in Figure 15A, the discrete breath rates and gas concentrations are taken to span an operating range, but it should be understood that the discrete breath rates or gas concentrations need not span the entire range. In some variations, the discrete breath rates may cover a subset of the operating range and the method may extrapolate that subset to a broader range, if necessary. For example, a look-up table covering an

operating range of 8 bpm to 60 bpm may, in one variation, be populated by taking measurements at 10 bpm, 30 bpm, and 50 bpm.

[0089] Although ETCO is specifically discussed with respect to Figures 15A-E, the disclosure is not limited to ETCO. In other variations, the methods described herein may be applied to other gases and/or breath stages and multiple gas concentrations. Other influencing variables may also be included in the database creation, such as different operating temperatures, different secondary gas levels, or the like.

[0090] In some embodiments, the look-up table may be populated by drawing a known ETCO through an inlet of an apparatus and then measuring the ETCO at another point in the apparatus. The procedure may be repeated for multiple breath rates.

[0091] A specific variation of establishing ETCO accuracy, such as in step 1502, is depicted in graph 1520 of Figure 15B. Graph 1520 illustrates a measured gas concentration (y axis, "Measured ETCO") for three known CO concentrations (x axis, "Actual CO"). The measurements are repeated across five breath rates: 10 bpm, 20 bpm, 30 bpm, 40 bpm, and 50 bpm; and at three gas concentrations: 0.91 ppm, 9.70 ppm and 24.4 ppm. Although the variation of Figure 15B shows five specific breath rates and three gas concentrations, other variations may use a different number and/or different rates and concentrations.

[0092] Returning to Figure 15A, method 1500 continues with step 1504. At this step, accuracy equations for discrete breaths are established. As used herein, "an accuracy equation" can be understood to be a polynomial equation that fits the measured gas concentrations to actual gas concentrations of a breath rate, wherein data "fits" an equation when the data is interpolated, extrapolated, or smoothed. The equation need not correlate with the data correctly and may approximate the data. The degree of approximation may be determined by the requirements of a specific application.

[0093] In some variations, non-polynomial equations may be used to describe the relationships, such as logarithmic equations, exponential equations, or other equations. Specific accuracy equations are illustrated in graph 1520 of Figure 15B. For each of the breath rates, a linear equation is derived that approximates "Actual CO" to "Measured

ETCO” across all “Actual CO” concentrations. The linear equation is derived by fitting the known CO concentrations and measured ETCO concentrations for each breath rate.

[0094] Although the variation in Figure 15B illustrates a linear equation, other variations may include polynomial equations of higher orders. For example second, third, and fourth order polynomial equations. In some variations, the maximum order may be one less than the number of measurements taken. For example, three measurements were taken in the embodiment illustrated in Figure 15B and so the maximum order for the polynomial equation may be two (i.e., a quadratic equation). In Figure 15B, the measurements resulted in a linear equation, but need not have. However, a linear equation may be beneficial because it may require less computing resources to solve. In some variations, the measurements may be fit to an equation of less than the maximum order. In such variations, it may be beneficial to fit the measurements to a “best-fit” equation of a lower order to reduce the need for computing resources.

[0095] Referring again to Figure 15A, method 1500 then moves to step 1506 and establishes a continuous relationship between the accuracy equations and breath rate. In this step, the coefficients are collated by the order in each of the breath rate accuracy equations. For each order, the coefficients for that order and each coefficient’s corresponding breath rate is used to determine the continuous relationship.

[0096] Figures 15C and 15D illustrate two such comparisons. Figure 15C illustrates graph 1530 which plots the slope (M) and offset (b) of the linear accuracy equations with the discrete breath rates between 10 and 30. Similarly, Figure 15D illustrates graph 1535 which plots the slope and offset of the linear accuracy equations with the discrete breath rates between 30 and 50. Two separate ranges may allow for lower order equations to be derived for the coefficients, thereby reducing the amount of computer resources necessary to solve the equations. Further, by reducing the breath rates to two separate ranges, the fidelity of the system may be improved. For example, Figure 15C and 15D illustrate two equations which have a constant second derivative. A higher order polynomial equation may result in a non-constant second derivative, thereby resulting in possible wide variances in the region of a measured concentration.

[0097] Although Figure 15C and 15D depict a separation of the breath rates into two ranges, other variations may not separate the breath rates into ranges. Other variations may separate the breath rates into three, four, or five, or more than five ranges.

[0098] Returning to Figure 15A, method 1500 continues with determining equations for the slope and offset of the accuracy equations based on the continuous relationship established, step 1508. In some embodiments, steps 1506 and 1508 may be performed at the same time, that is, determining the relationships between the continuous relationship may result in determining the slope and offset equations. Figure 15C and 15D illustrate quadratic equations derived from the relationship between the coefficients of the accuracy equations and the breath rates. Each of the quadratic equations in Figures 15C and 15D has a coefficient at each order (which may include a coefficient = 0 in some variations). These coefficients are used in the next step of method 1500.

[0099] Although Figures 15C and 15D illustrate quadratic equations, polynomial equations of other orders may be used. For example, first order (linear), third order, fourth order, fifth order, sixth order, or higher order polynomial equations could be used. The maximum order of the polynomial equations may be the number of discrete breath rates minus one. As in Figures 15C and D, the polynomial equations could comprise lower orders than the maximum orders. This may improve fidelity if some discrete regions of the curve can represent a lower order curve. This may also reduce the use of computing resources because the difficulty of solving a polynomial equation increases as the order increases.

[0100] Returning again to Figure 15A, Step 1510 sets up a look table based on the coefficient equations determined in the previous step. Referring now to the exemplary embodiment in Figure 15E, the look up table can be found on the bottom of Table 1540. For a given breath rate (less than or equal 30 or greater than 30), coefficients for each order of quadratic equation can be identified. There are two equations derived for each of slope and for offset. Because slope and offset are determined by quadratic equations in Figures 15A-E, the look-up table includes three coefficients for each of slope and offset at each breath rate.

[0101] Figure 15E also provides one variation of correcting a measured gas concentration. Once a breath rate is determined, the relevant coefficients are determined. Once the relevant coefficients are determined, the equations for slope and offset can be determined. Using the breath rate, actual values for slope and offset can be determined. These values are then used to calculate the corrected concentration using the following formula:

$$\text{ETCO}_{(\text{BR Corrected})} = [\text{ETCO}_{(\text{Measured})} - b]/M$$

[0102] It should be understood that the above equation may vary if the number of coefficients of the accuracy equation is varied. For example, the variation of Figure 15E had two coefficients. Thus, the above equation results from solving a linear equation (two coefficients). If more coefficients are used, then a solution to a higher order equation may be necessary. The solution may be obtained using any mathematical technique capable of solving for an unknown variable in a higher order equation.

[0103] When the apparatus is in use, should the measured breath rate or measured gas concentration be outside of the ranges defined by the above procedure, the apparatus may react in a variety of ways, depending on the details of the clinical application. The apparatus may not compute a corrected ETCO result and notify the user that the measured parameters are outside of the apparatus's range. The apparatus may compute the corrected ETCO despite being out of range, and provide the result to the user while notifying the user that the accuracy of the result may be less accurate because the measured parameters are outside of the operating range. In some variations, the apparatus may simply compute a result by extrapolating with the appropriate equations. In this way, variations of the present disclosure may beneficially provide for determining a gas concentration in a patient's breath independently of patient cooperation. That is, the gas concentration may be determined for patients who are unwilling or unable to regulate their breathing to correlate to a "normal" breathing pattern.

[0104] In some variations, the entire set of values within an operating range may be tested in advance, and a look-up database created based on the results. For example, breath rates of 10, 11, 12 and so on to 50 bpm (for example), at gas concentrations of 1.0, 1.1, 1.2 and so on to 25.0ppm can be pre-tested. When the device is in use, the corrected

gas concentration can be obtained by finding the appropriate value in the database for the measured breath rate and measured gas concentration. In some variations, a combined approach is used such as pre-testing all breath rates but only a set of discrete gas concentrations within or near the operating range.

[0105] While the above embodiment describes the use of breath rate as the breathing pattern parameter used in the corrections, it is understood that rather than breath rate, the same embodiment may be accomplished with any breathing pattern related parameter. Examples of other parameters include expiratory time, end-tidal time, inspiratory time, inspiratory:expiratory ratio, tidal volume, minute volume, airway pressure amplitude, capnometry signal amplitude, and the duration of the positive slope of the capnometry signal.

[0106] In some variations, a method of determining a gas concentration at the inlet of an apparatus may include determining the patient's breath rate and measuring the concentration of the patient's breath somewhere else in the apparatus. As used herein, measured a gas in an apparatus can be understood to mean measuring anywhere within the apparatus, such as at an outlet or an interior point in the apparatus, such as in a tube or compartment. With the measured gas concentration, a database can be accessed to obtain a plurality of coefficients corresponding to the patient's breath rate. In the example of Figure 15E, the plurality of coefficients are separated by breath rate into two regions: at or below 30 bpm, or at or above 30 bpm. Other variations may arrange the coefficient's differently. Once the coefficients are obtained, the method may derive a first plurality of polynomial equations (in Figure 15A-E, the first polynomial equations are quadratic). These equations provide coefficients for second plurality of equations (in Figure 15A-E, the second polynomial equations are linear), where the coefficients are then used to form a compensation equation (in Figure 15A-E, the compensation equation is linear). The compensation equation is then used to adjust the measured gas concentration to determine the gas concentration at the inlet.

[0107] In some variations, an apparatus may include a processor for carrying out the above method of determining a gas concentration at the inlet of an apparatus. The apparatus may also include a measuring point, a gas analyzer for determining a gas concentration at the measuring point, an inlet, and a breath speed analyzer. The processor

may access a database stored on a non-transitory computer readable medium, where the database includes a plurality of coefficients for each breath rate in the operating range.

[0108] In some variations, a sampling system may be tuned for an upper limit breath rate. For a given sample volume (sample volume may be determined to meet specifications of a particular application), the flow rate of a flow generator, such as a pump, may be configured to fill the entire sample volume with end-tidal gas for the upper limit breath rate. For breath rates lower than the upper limit breath rate, the sample volume is completely filled with end-tidal gas, albeit not all of the end-tidal gas for that breath. In further variations, the system may include an upper limit cut-off that limits sampling to breaths at or below the upper limit. In this way, these variations may beneficially prevent non-end-tidal gas from entering the sample volume. Thus, variations of the present disclosure may beneficially provide for determining a gas concentration in a patient's breath independently of patient cooperation. That is, the gas concentration may be determined for patients who are unwilling or unable to regulate their breathing to correlate to a "normal" breathing pattern.

[0109] In some variations, a gas sampling flow rate may be determined to fit the requirements of a particular application. For example, an upper limit for normal breathing may be described by a breath frequency parameter, such as 60 bpm. However, for certain patients (such as neonates, for example), a normal breath rate may exceed 60 bpm. In such an instance, the upper limit may be higher, such as at 100 bpm. Similarly, the sample volume may be chosen to reflect the needs of a particular application. In some variations, other frequency parameters may be chosen, such as inspiratory time, breath period, expiratory time, end-tidal time, capnometer signal rise duration, or another parameter that describes at least a portion of the patient's breathing. In some variations, an instantaneous carbon monoxide sensor is used.

[0110] Figure 16A illustrates method 1600 of determining a gas sampling rate of a flow generator to correlate to an upper limit breath rate and predetermined sampling volume. Method 1600 begins with step 1602: defining an upper limit for the breath rate (BR). As discussed above, the upper limit may be determined to meet the requirements of a specific application.

[0111] Method 1600 continues with step 1604, defining a desired sample volume ($V(s)$). In the variation of method 1600, the sample volume is sized for adequate and reliable analysis. In other variations, the sample volume may be sized to factor in other considerations.

[0112] Method 1600 continues with step 1606, determining the gas sampling flow rate ($Q(S)$). In the variation of method 1600, the flow generator is a pump, but other flow generators could be used, such as the examples described herein. The gas sampling flow rate may be calculated to fill the desired sample volume at the upper limit breath rate.

[0113] In some variations, the sampling flow rate is calculated from the following equation $Q(S) = T_{ET} / V(S)$, wherein T_{ET} is the estimated end-tidal period and is a function of the breath rate. In some variations, T_{ET} may be assumed to be half of the expiratory time, which itself may be assumed to be half of the breath period (inspiratory and expiratory periods). The breath period (seconds) is $60 / \text{breath rate}$. For example, if the upper limit breath rate is 60 bpm, then T_{ET} may be assumed to be 0.25 seconds. If the sample volume in this example is 0.5 ml, then the sampling flow rate is 2 ml per second.

[0114] Figure 16B illustrates the pneumatic gas capture system of Figures 5A or 5B in configuration 1620. Configuration 1620 includes the gas sampling rate of the pump configured for an upper limit breath rate, and where the patient's breath rate is at the upper limit. As can be seen in Figure 16B, the sample volume is entirely filled with end-tidal gas and there is no end-tidal gas outside of the sample volume.

[0115] Figure 16C illustrates the pneumatic gas capture system of Figures 5A or 5B in configuration 1640. Configuration 1640 includes the gas sampling rate of the pump configured for an upper limit breath rate, and where the patients' breath rate is below the upper limit. As can be seen in Figure 16C, the sample volume is entirely filled with end-tidal gas, but there is end-tidal gas from the breath outside of the sample volume. Figure 16C illustrates the end-tidal gas outside of the sample volume as located downstream (to the right) of $V2$. However, in other embodiments, the end-tidal gas outside of the sample volume may be located upstream (to the left) of $V1$, or a combination of upstream of $V1$ or downstream of $V2$. In this way, variations of the present disclosure may beneficially provide for determining a gas concentration in a patient's breath independently of patient

cooperation. That is, the gas concentration may be determined for patients who are unwilling or unable to regulate their breathing to correlate to a “normal” breathing pattern.

[0116] Some variations include elements and functionality from individual variations described above, that is, some variations may combine different elements of the different variations described above. For example, a user interface of the apparatus may allow the user to enter a certain patient parameter, such as a patient type, for example adult or infant, or for example premature neonate or full term infant. The control system of the apparatus will select a preferred breath rate compensation methodology, selected from the embodiments described above, and use that methodology accordingly. In some variations, the apparatus may, for example, use the embodiment described in Figure 16 in which the system is tuned for a breath rate of 60 bpm, therefore collecting an undiluted end-tidal sample for any breath rate at or below 60 bpm and therefore not requiring breath rate compensation. The variation may further allow for collection of breath rates above 60 bpm, where a breath rate compensation algorithm is invoked. The breath rate compensation algorithm could for example be the collection of end-tidal gas from two breaths in order to fill the sample tube such as described in relation to Figures 10A-11F, or can be the use of a polynomial equation correction factor such as described in relation to Figures 15A-15E.

[0117] In the foregoing descriptions of variations of the invention, the examples provided are illustrative of the principles of the invention, and that various modifications, alterations, and combinations can be made by those skilled in the art without departing from the scope and spirit of the invention. Any of the variations of the various breath measurement and sampling devices disclosed herein can include features described by any other breath measurement and sampling devices or combination of breath measurement and sampling devices herein. Accordingly, it is not intended that the invention be limited, except as by the appended claims. For all of the variations described above, the steps of the methods need not be performed sequentially.

CLAIMS

What is claimed is:

1. A gas measurement correction database for determining a gas concentration at an inlet of an apparatus, the database stored on a non-transitory computer readable medium, the database populated by a method comprising:

measuring a plurality of gas concentrations in the apparatus for a respective plurality of known gas concentrations at the inlet, wherein the gas concentrations are measured at a plurality of breath rates;

deriving a first plurality of polynomial equations, wherein each of the first plurality of polynomial equations fits the measured gas concentrations of a respective one of the plurality of breath rates, and wherein each of the first plurality of polynomial equations comprises a coefficient at each order of the equation;

deriving a second plurality of polynomial equations, wherein each of the second plurality of polynomial equations fits the coefficients of a respective order of the first plurality of polynomial equations, and wherein each of the second plurality of polynomial equations comprises a coefficient at each order of the equation; and

recording each of the coefficients of the second plurality of polynomial equations in the database.

2. The database of claim 1, wherein the first plurality of polynomial equations comprises a plurality of linear equations.

3. The database of claims 1 or 2, wherein the plurality of breath rates is at least five in number.

4. The database of any of claims 1 to 3, wherein the plurality of breath rates comprises breath rates of 10 breaths per minute, 20 breaths per minute, 30 breaths per minute, 40 breaths per minute, and 50 breaths per minute.

5. The database of any of claims 1 to 4, wherein the second plurality of polynomial equations comprises a plurality of quadratic equations.

6. The database of any of claims 1 to 5, wherein the coefficients of the second plurality of polynomial equations comprise a first plurality of coefficients and a second plurality of coefficients, wherein the first plurality of coefficients correspond to breath rates at or below a predetermined breath rate and the second plurality of coefficients correspond to breath rates at or above the predetermined breath rate.

7. The database of claim 6, wherein the predetermined breath rate is 30 bpm.

8. The database of claims 6 or 7, wherein the second plurality of polynomial equations comprise a first plurality of quadratic equations and a second plurality of quadratic equations, wherein each of the first plurality of quadratic equations fits the first plurality of coefficients at each order, and wherein each of the second plurality of quadratic equations fits the second plurality of coefficients at each order.

9. The database of any of claims 1 to 8, wherein the plurality of known gas concentrations at the inlet comprises three in number.

10. The database of any of claims 1 to 9, wherein the plurality of known gas concentrations at the inlet comprises at least one selected from each of the following: a region of relatively low breath rate, a region of relatively high breath rate, and a region of intermediate breath rate.

11. A method for determining a gas concentration of a patient's breath at an inlet of an apparatus, the method comprising:

determining a breath rate of the patient;

measuring a gas concentration in the apparatus;

accessing a database to obtain a first plurality of coefficients corresponding to the patient's breath rate;

deriving a first plurality of polynomial equations based on the first plurality of coefficients;

deriving a second plurality of coefficients by inputting the breath rate into each of the first plurality of polynomial equations;

deriving a compensation equation using the second plurality of coefficients; and

determining the gas concentration at the inlet by inputting the measured gas concentration into the compensation equation.

12. The method of claim 11, wherein each of the first plurality of polynomial equations is a quadratic equation and the first plurality of coefficients is three in number.

13. The method of claims 11 or 12, wherein the compensation equation is linear and the second plurality of coefficients is two in number.

14. The method of any of claims 11 to 13, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breath rates at or below a predetermined breath rate and the second subset of coefficients correspond to breath rates at or above the predetermined breath rate.

15. The method of claim 14, wherein the predetermined breath rate is 30 bpm.

16. An apparatus for analyzing a gas concentration of a patient's breath, the apparatus comprising:

a gas analyzer that measures a gas concentration in the apparatus;

an inlet that receives the patient's breath;

a breath speed analyzer that determines a breathing parameter frequency of the patient's breath;

a database comprising a plurality of coefficients corresponding to a plurality of breathing parameter frequencies; and

a processor containing a non-transitory computer readable medium containing executable instructions that when executed perform a method of determining the gas concentration of the patient's breath at the inlet of the apparatus, the method comprising:

accessing the database to obtain a first plurality of coefficients based on the patient's breathing parameter frequency;

deriving a first plurality of polynomial equations based on the first plurality of coefficients;

deriving a second plurality of coefficients by inputting the breathing parameter frequency into each of the first plurality of polynomial equations;
deriving a compensation equation using the second plurality of coefficients; and
determining the inlet gas concentration by inputting the measured gas concentration into the compensation equation.

17. The apparatus of claim 16, wherein each of the first plurality of polynomial equations is a quadratic equation and the first plurality of coefficients is three in number.

18. The apparatus of claims 16 or 17, wherein the compensation equation is linear and the second plurality of coefficients is two in number.

19. The apparatus of any of claims 16 to 18, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency.

20. The apparatus of claim 19, wherein the predetermined breathing parameter frequency is 30 bpm.

21. A method for determining a gas concentration of a patient's breath at an inlet of an apparatus, the method comprising:
determining a breathing parameter frequency of the patient;
measuring a gas concentration in the apparatus;
accessing a database to obtain a plurality of coefficients based on whether the patient's breathing parameter frequency is at, above, or below a predetermined breathing parameter frequency, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below the predetermined breathing parameter

frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency;
deriving a compensation equation using the plurality of coefficients; and
determining the gas concentration at the inlet by inputting the measured gas concentration into the compensation equation.

22. The method of claim 21, wherein the predetermined breathing parameter frequency is 30 bpm.

23. An apparatus for analyzing a gas concentration of a patient's breath, the apparatus comprising:

a gas analyzer that measures a gas concentration in the apparatus;

an inlet that receives the patient's breath;

a breath speed analyzer that determines a breathing parameter frequency of the patient's breath;

a database comprising a plurality of coefficients corresponding to a plurality of breathing parameter frequencies, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency; and

a processor containing a non-transitory computer readable medium containing executable instructions that when executed perform a method of determining the gas concentration of the patient's breath at the inlet of the apparatus, the method comprising:

accessing the database to obtain a plurality of coefficients based on whether the patient's breathing parameter frequency is at, above, or below the predetermined breathing parameter frequency;

deriving a compensation equation based on the plurality of coefficients;

and

determining the inlet gas concentration by inputting the measured gas concentration into the compensation equation.

24. The apparatus of claim 23, wherein the predetermined breathing parameter frequency is 30 bpm.

25. A method for determining a gas concentration of a patient's breath at an inlet of an apparatus, the method comprising:

determining a breathing parameter frequency of the patient;

measuring a gas concentration in the apparatus;

accessing a database to obtain a plurality of coefficients corresponding to the patient's breathing parameter frequency;

deriving a compensation equation using the plurality of coefficients; and

determining the gas concentration at the inlet by inputting the measured gas concentration into the compensation equation.

26. The method of claim 25, wherein the compensation equation is a polynomial equation.

27. The method of claim 26, wherein the compensation equation is linear.

28. The method of any of claims 25 to 27, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency.

29. The method of claim 28, wherein the predetermined breathing parameter frequency is 30 bpm.

30. An apparatus for analyzing a gas concentration of a patient's breath, the apparatus comprising:

a gas analyzer that measures a gas concentration in the apparatus;

an inlet that receives the patient's breath;

a breath speed analyzer that determines a breathing parameter frequency of the patient's breath;

a database comprising a plurality of coefficients corresponding to a plurality of breathing parameter frequencies; and

a processor containing a non-transitory computer readable medium containing executable instructions that when executed perform a method of determining the gas concentration of the patient's breath at the inlet of the apparatus, the method comprising:

accessing the database to obtain a plurality of coefficients based on the patient's breathing parameter frequency;

deriving a compensation equation using the plurality of coefficients; and

determining the inlet gas concentration by inputting the measured gas concentration into the compensation equation.

31. The apparatus of claim 30, wherein the compensation equation is a polynomial equation.

32. The apparatus of claim 31, wherein the polynomial equation is a linear equation.

33. The apparatus of any of claims 30 to 32, wherein the database comprises a first subset of coefficients and a second subset of coefficients, wherein the first subset of coefficients correspond to breathing parameter frequencies at or below a predetermined breathing parameter frequency and the second subset of coefficients correspond to breathing parameter frequencies at or above the predetermined breathing parameter frequency.

34. The apparatus of claim 33, wherein the predetermined breathing parameter frequency is 30 bpm.

35. An apparatus for collecting gas from a patient's breath comprising a sample volume;

a flow generator comprising a sampling flow rate, wherein the flow generator completely fills the sample volume with an end-tidal portion of the patient's breath when the patient's breath has a predetermined breathing parameter frequency; and

a processor configured to discard a gas collected from the patient's if a breathing parameter frequency of the patient exceeds the predetermined breathing parameter frequency.

36. The apparatus of claim 35, wherein the flow generator is a pump.

37. The apparatus of claims 35 or 36, wherein the end-tidal period of the patient's breath is assumed to be one quarter of a breath period of the patient, wherein the breath period comprises one inspiratory and expiratory cycle of the patient's breath.

38. An apparatus for analyzing a gas concentration of a sample of a patient's breath, the apparatus comprising:

a sample compartment with an inlet that receives the patient's breath;

a breath speed analyzer that determines the speed of a portion of the patient's breath;

a gas analyzer that determines a gas concentration of the gas in the sample compartment; and

a processor comprising an algorithm that determines a corrected gas concentration based on the speed of a portion of the patient's breath, wherein the corrected gas concentration is determined independently of patient cooperation.

39. An apparatus for analyzing a gas concentration of a sample of a patient's breath, the apparatus comprising:

a sample compartment with an inlet that receives the patient's breath;

a breath speed analyzer that determines the speed of the portion of the patient's breath;

a gas analyzer that determines a gas concentration of the gas in the sample compartment; and

a processor comprising an algorithm, wherein the algorithm determines a degree of non-homogeneity of the breath sample in the sample compartment based on the speed

of a portion of the patient's breath, wherein the algorithm determines a corrected gas concentration based on the degree of non-homogeneity, and wherein the corrected gas concentration is determined independently of patient cooperation.

40. An apparatus for analyzing a gas concentration of a sample of a patient's breath, the apparatus comprising:

a breathing parameter frequency measuring sensor;

an algorithm comprising a defined maximum breathing parameter frequency;

a sample compartment with a volume and with an inlet that receives the patient's breath;

a gas analyzer that determines a gas concentration of the gas in the sample compartment; and

a sampling flow rate control unit that delivers the sample from the patient into the sample compartment at a desired rate, wherein the sample compartment volume and the desired rate are determined based on the defined maximum breathing parameter frequency.

Figure 1

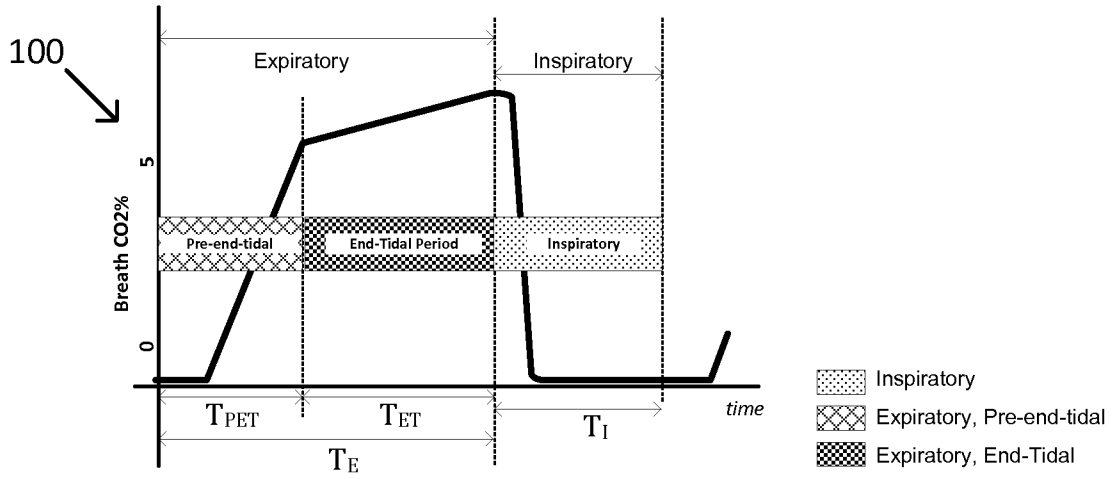


Figure 2

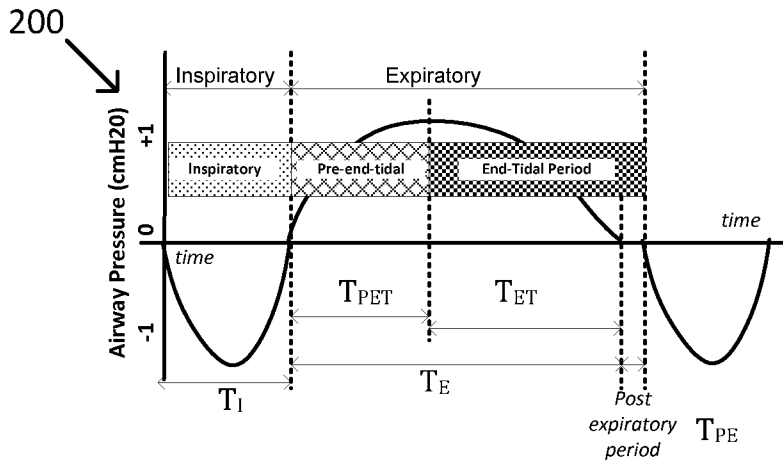


Figure 3A

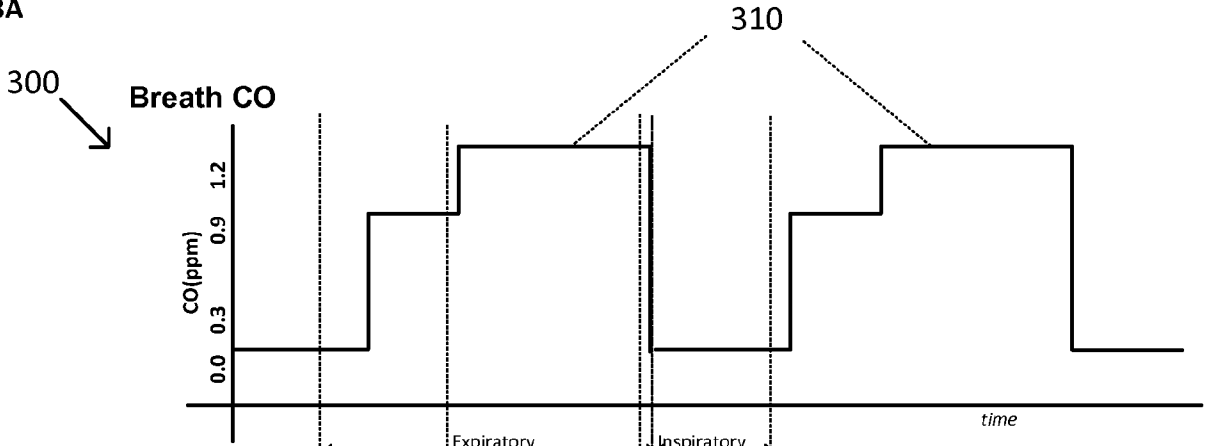


Figure 3B

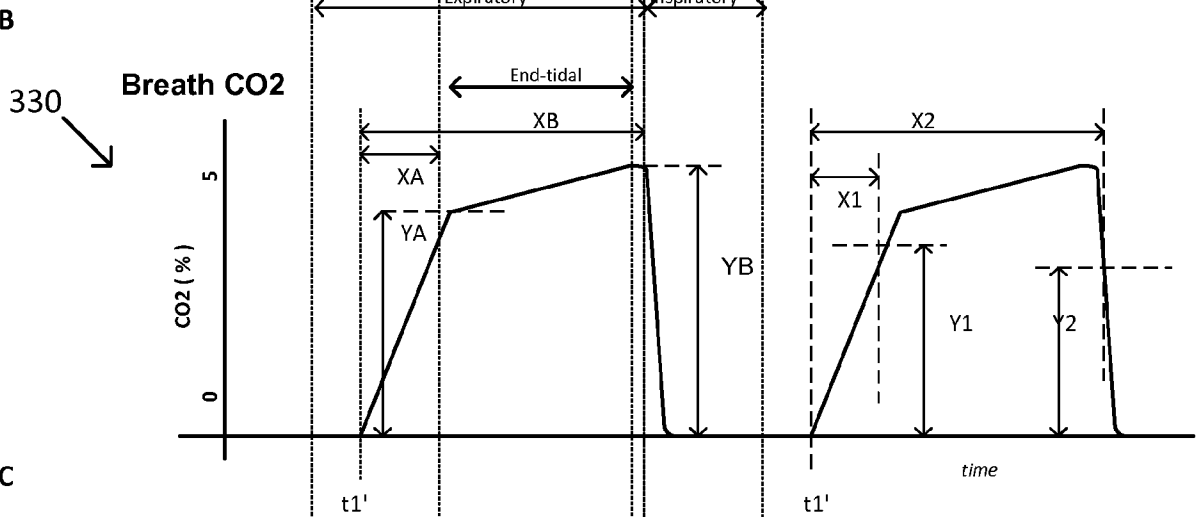


Figure 3C

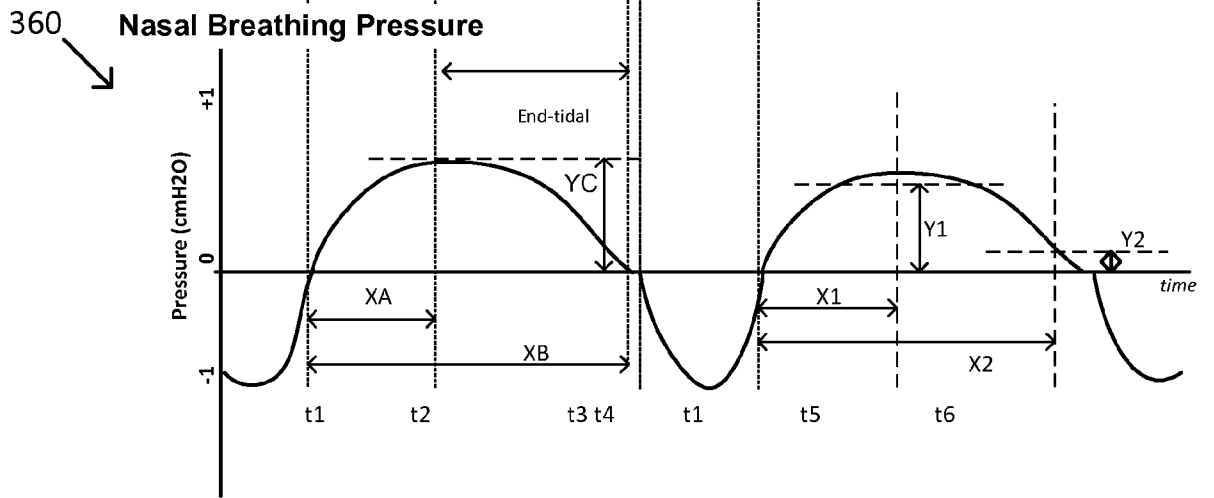


Figure 4A

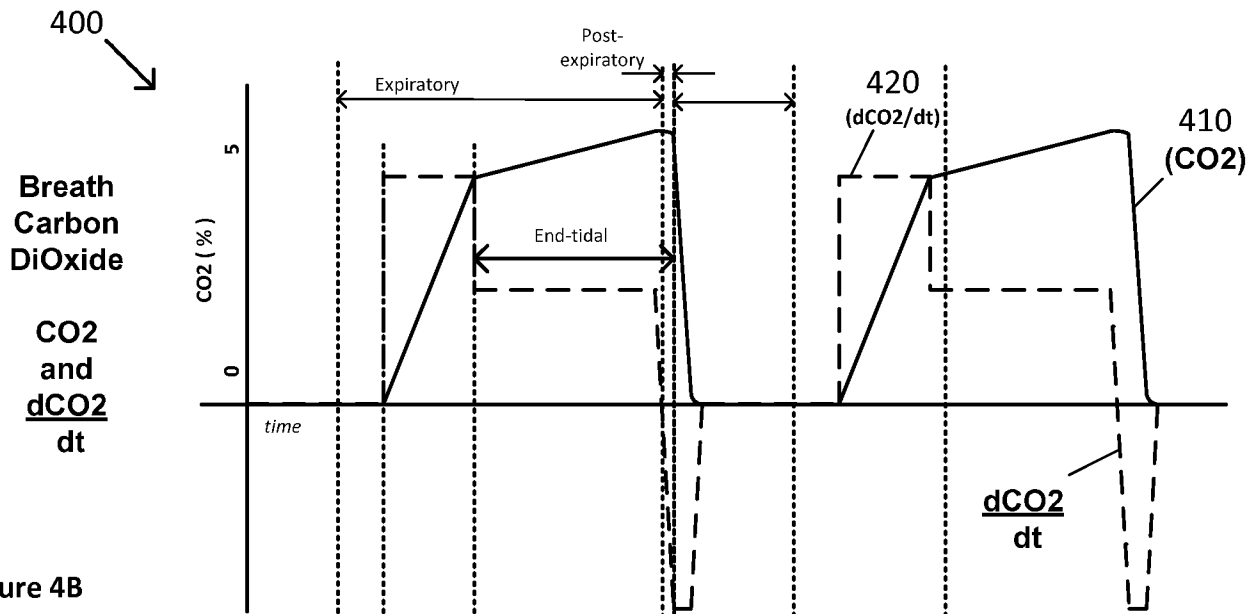


Figure 4B

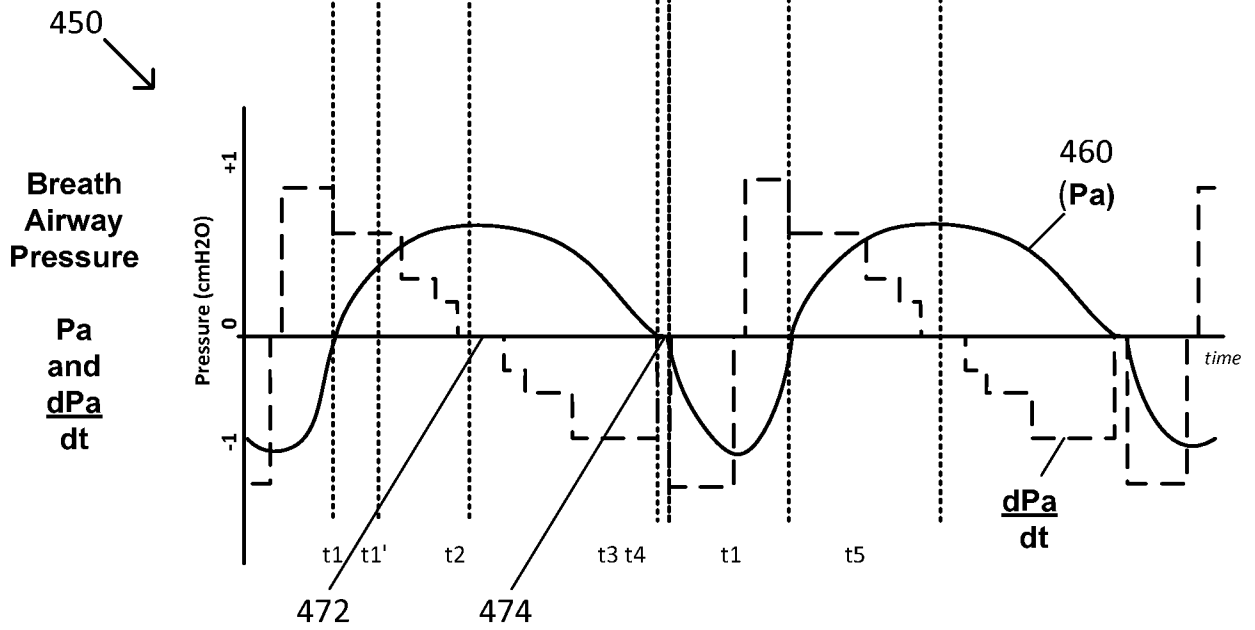


Figure 5A

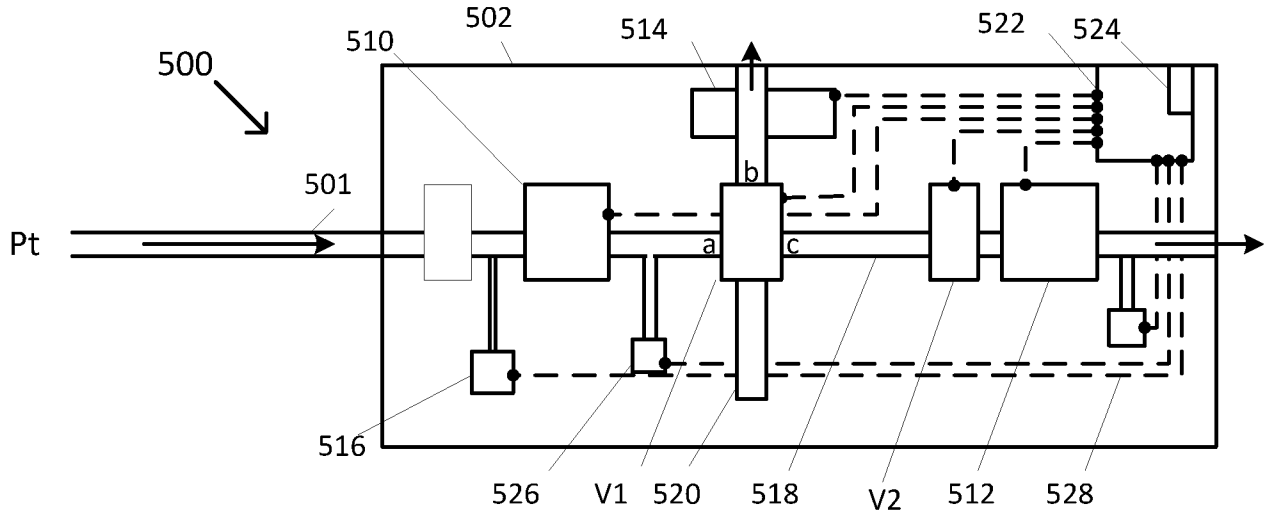


Figure 5B

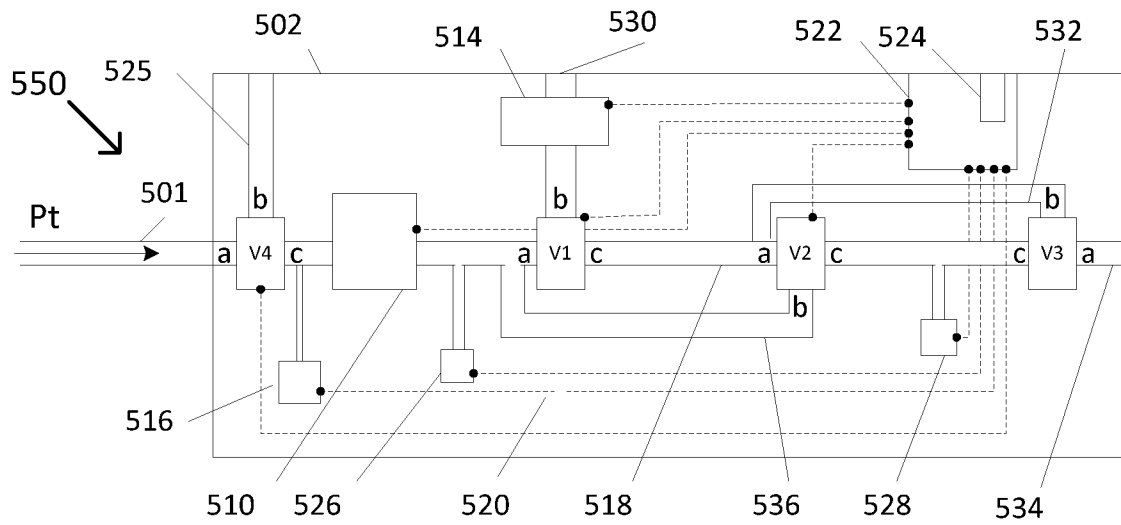


Figure 6

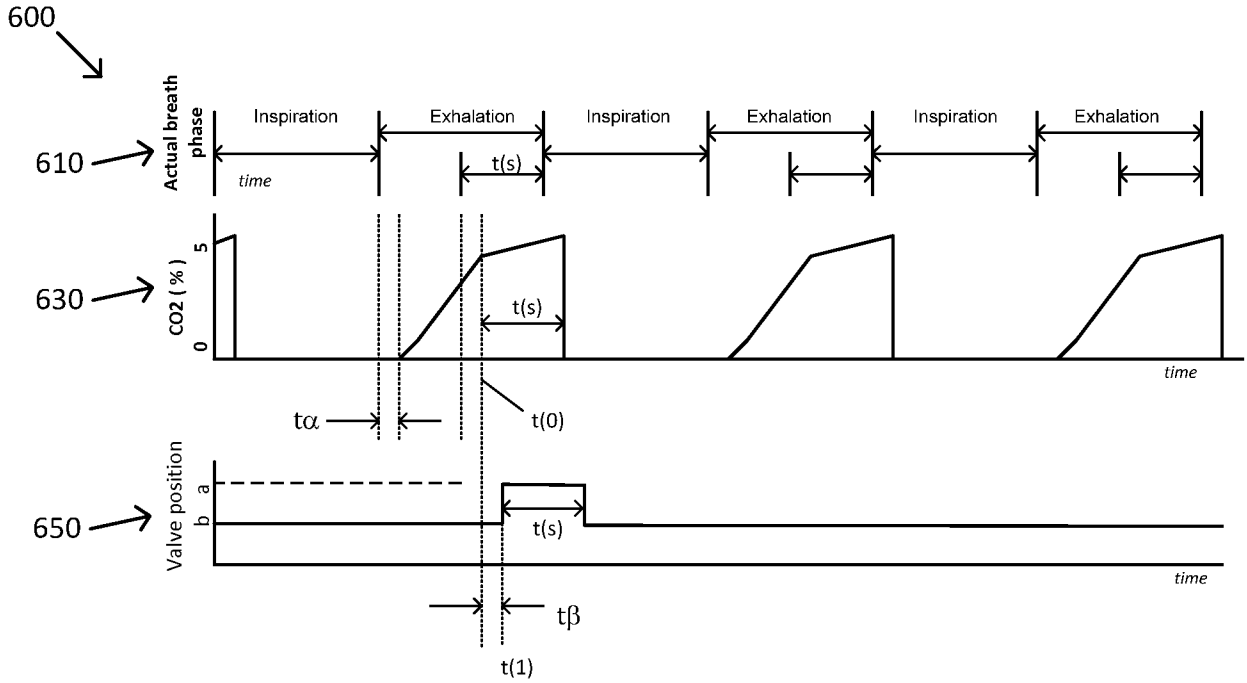


Figure 7

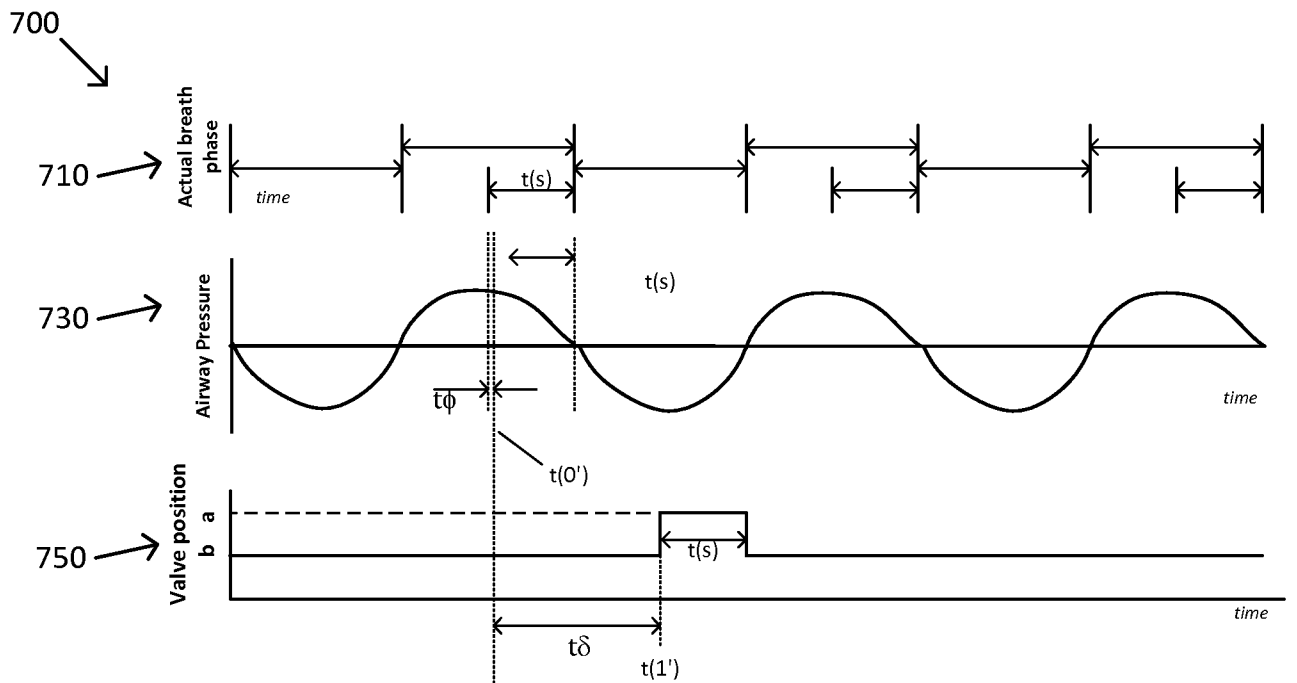


Figure 8

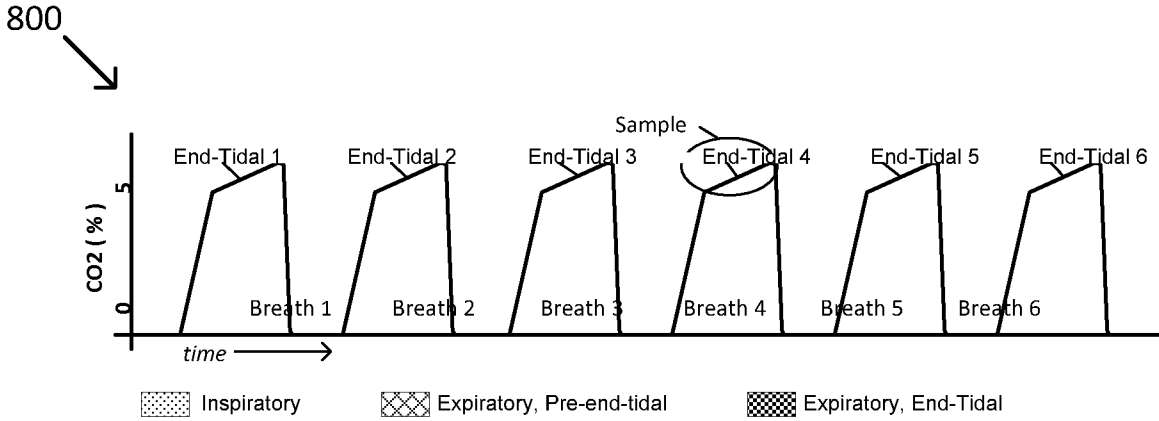


Figure 9A

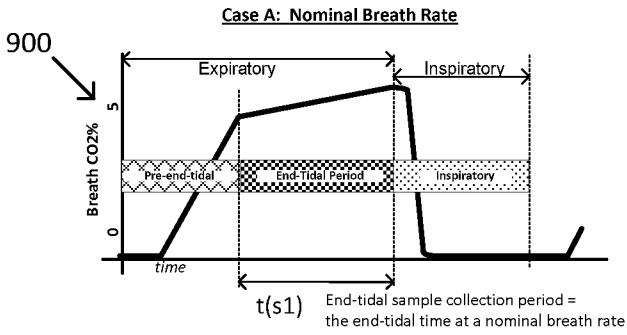


Figure 9B

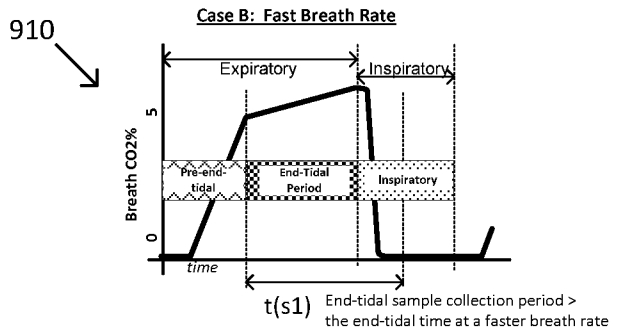


Figure 9C

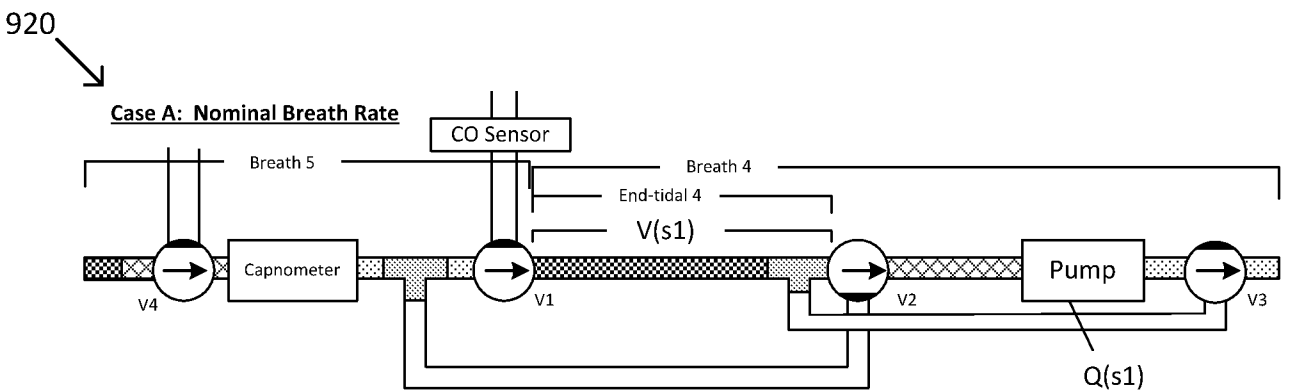


Figure 9D

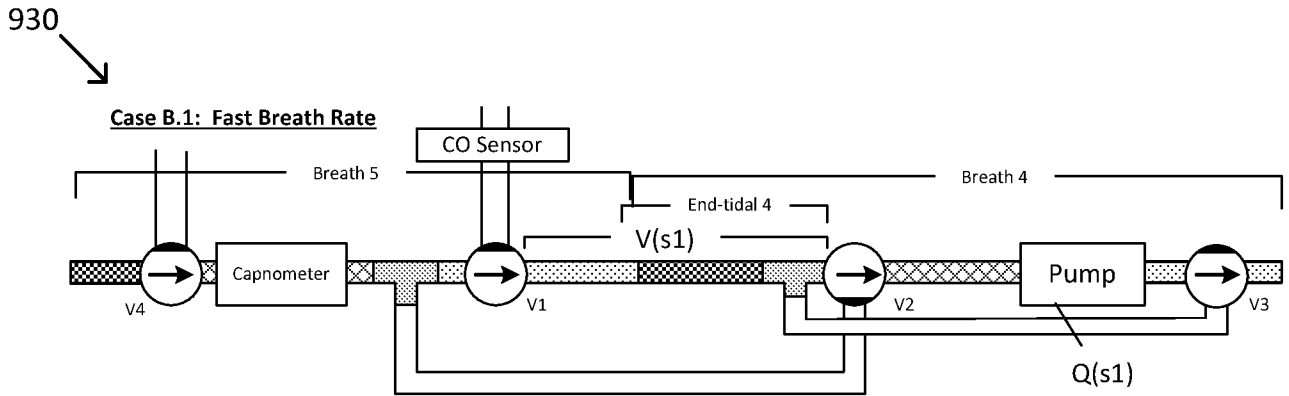


Figure 9E

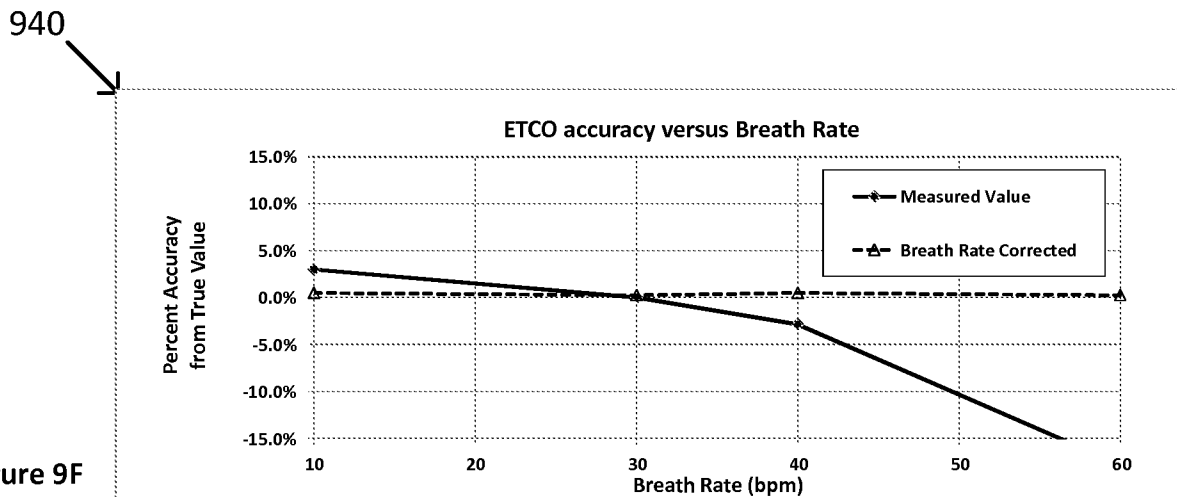


Figure 9F


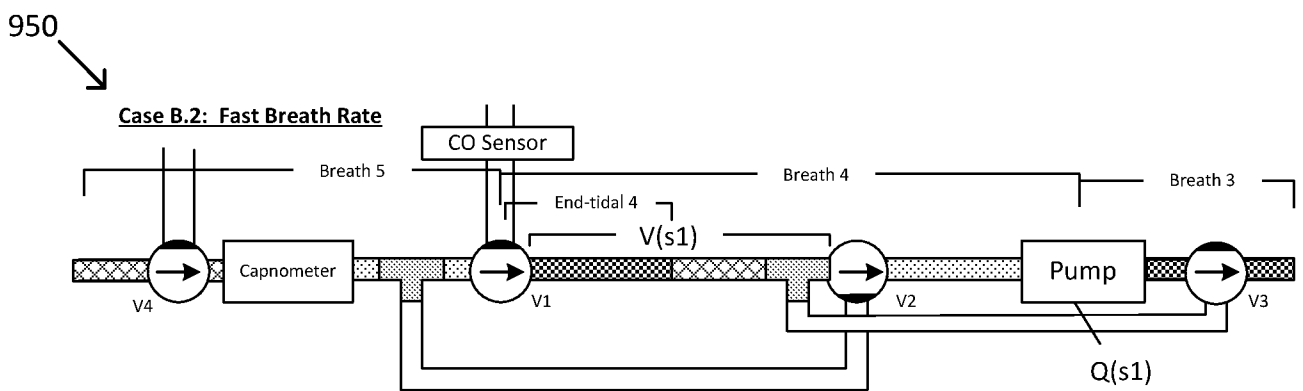



Figure 9G

960

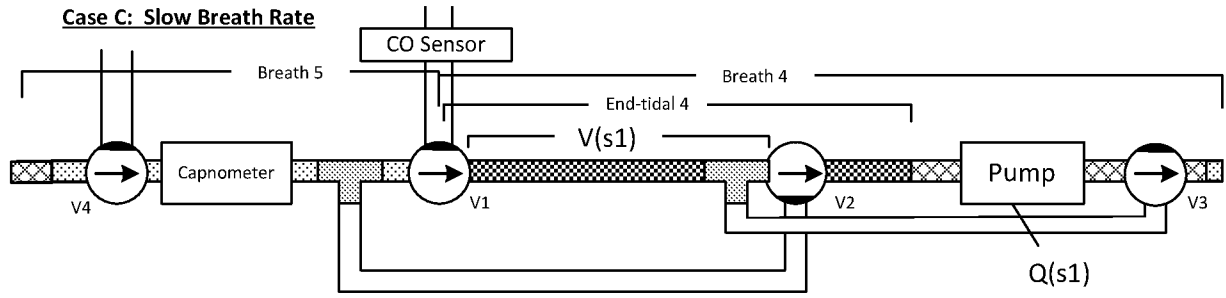

9/20

Figure 10A

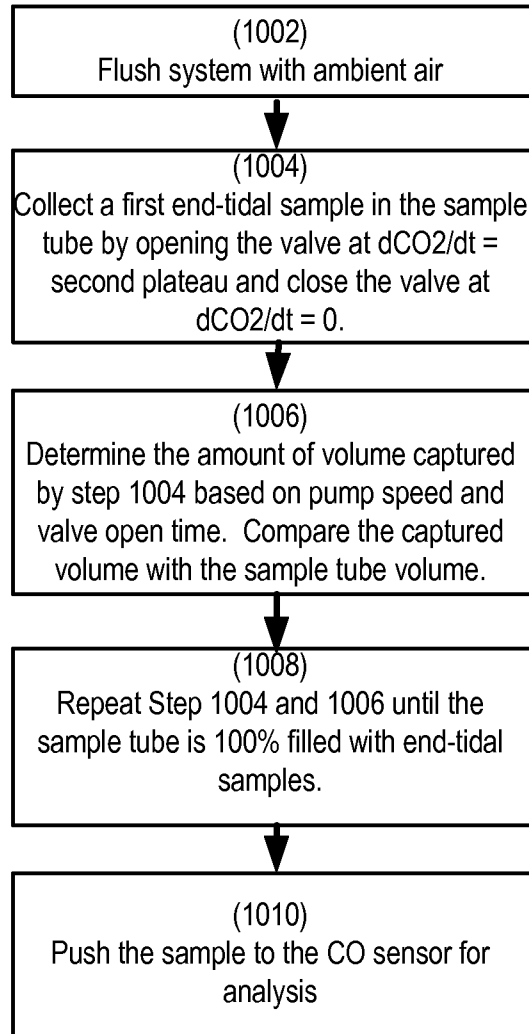1000
↓**MULTIPLE SAMPLE CAPTURE
TECHNIQUE**

10/20

Figure 10B

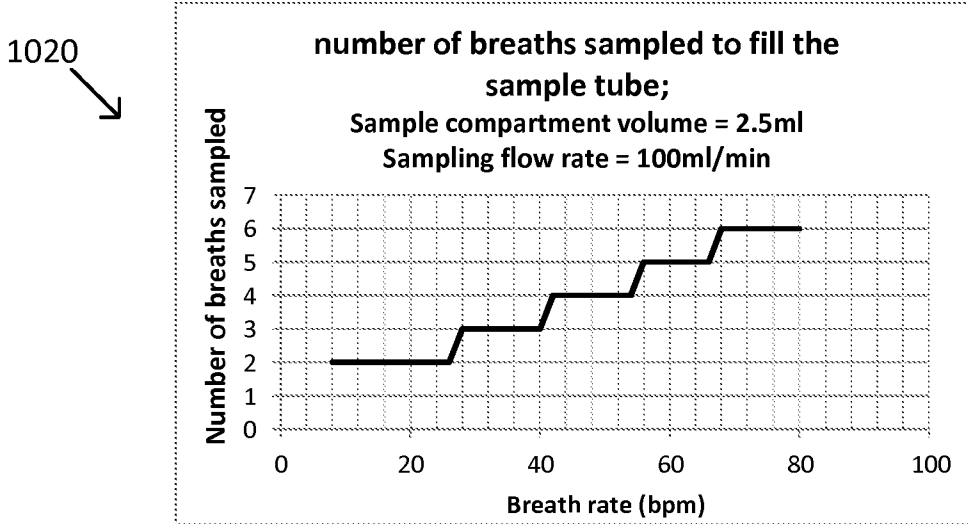


Figure 11A


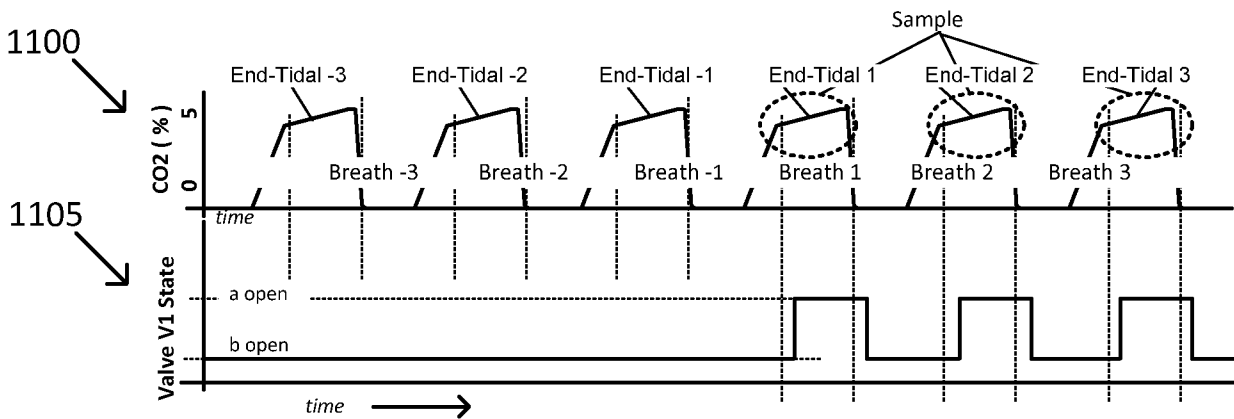


Figure 11B

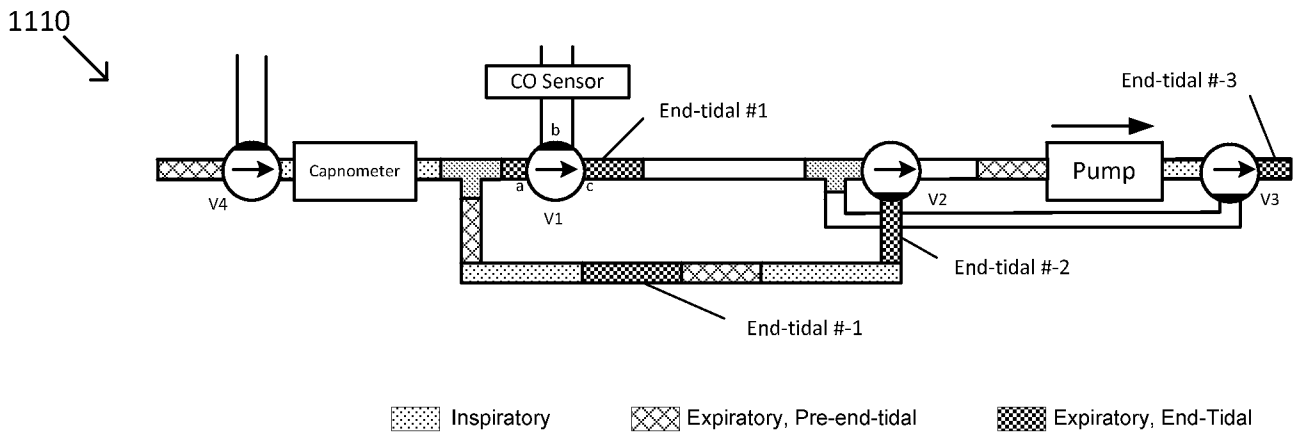

11/20

Figure 11C

1120

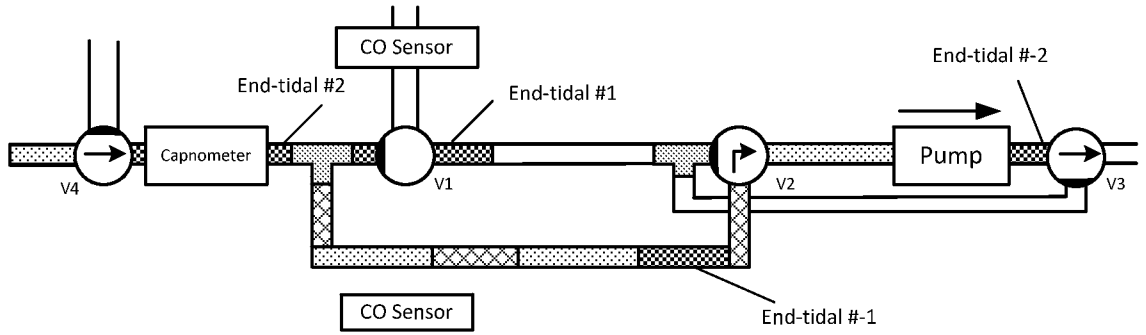


Figure 11D

1130

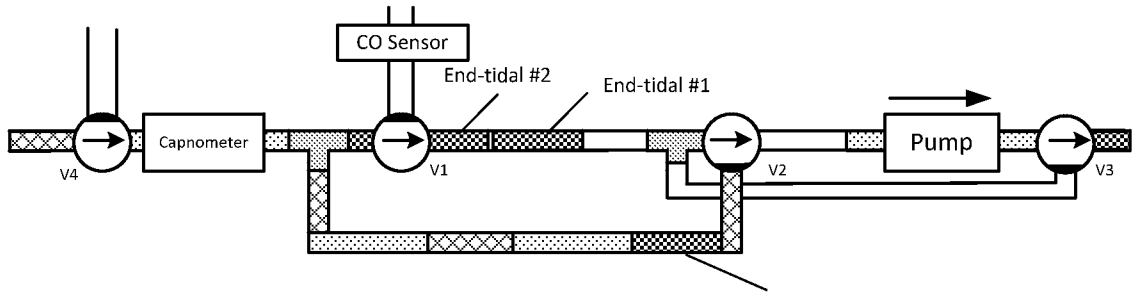


Figure 11E

1140


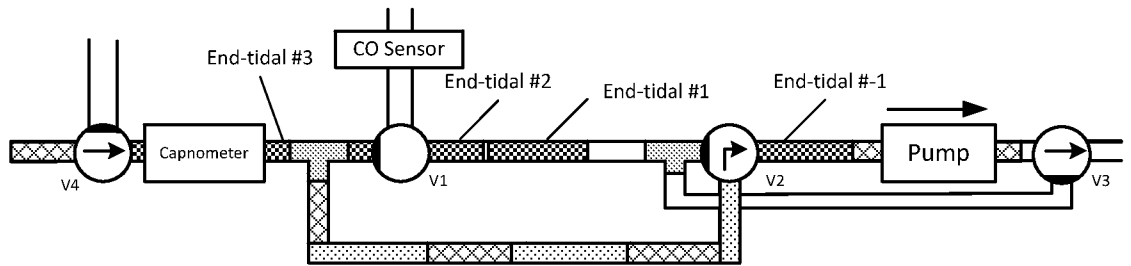



Figure 11F

1150

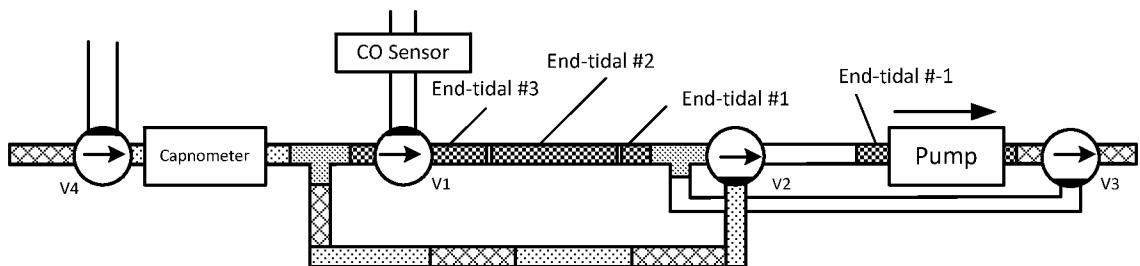

12/20

Figure 12A

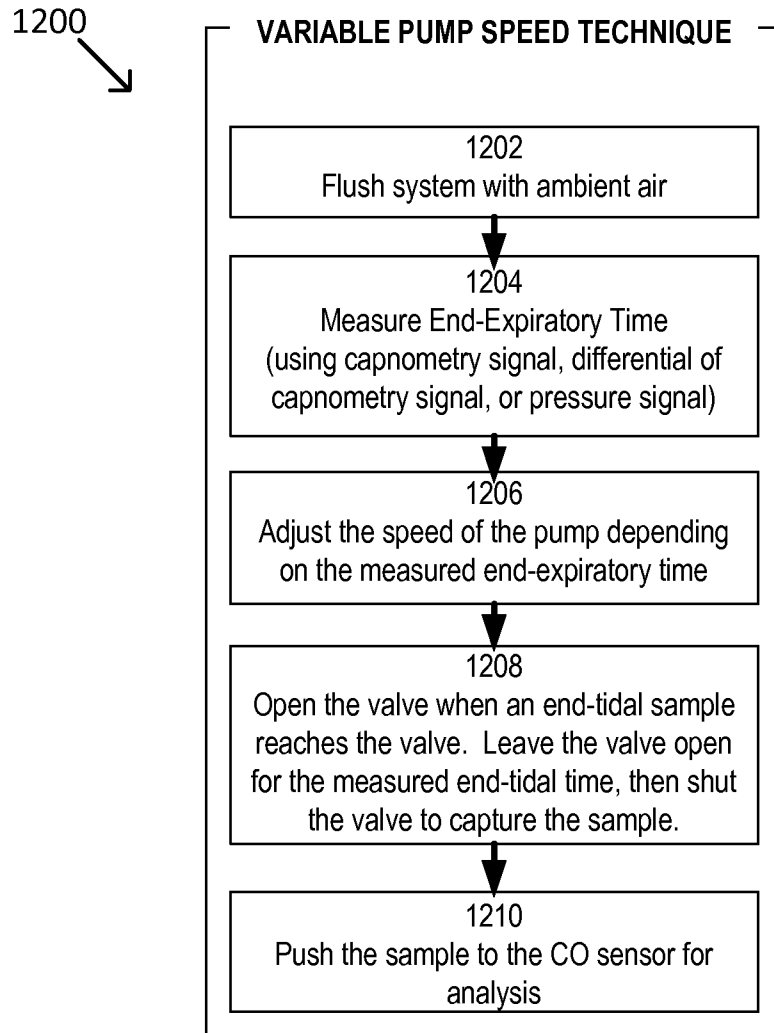

13/20

Figure 12B

1220 ↘

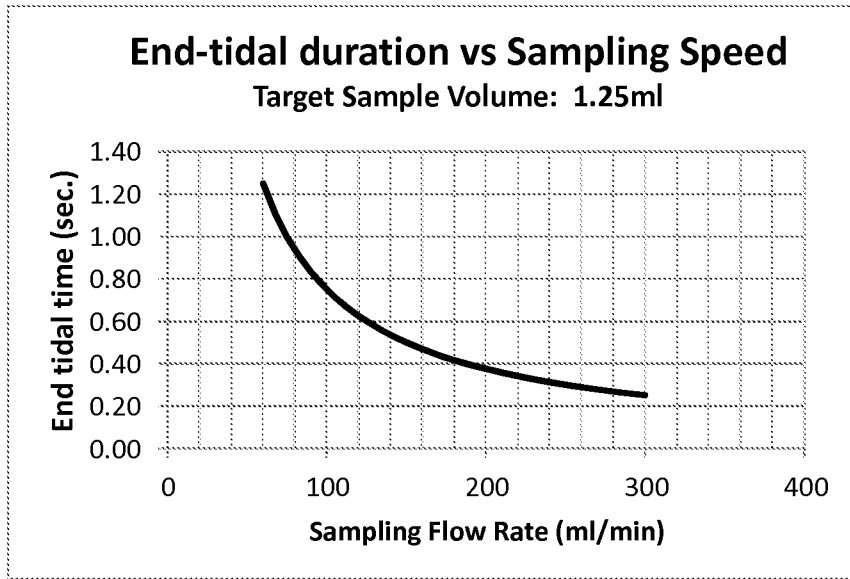


Figure 13A

1300

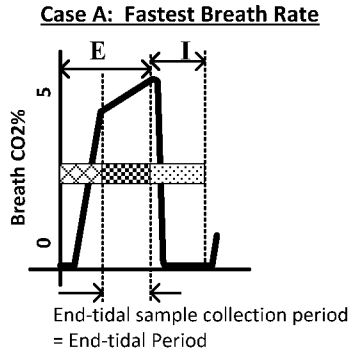


Figure 13B

1310

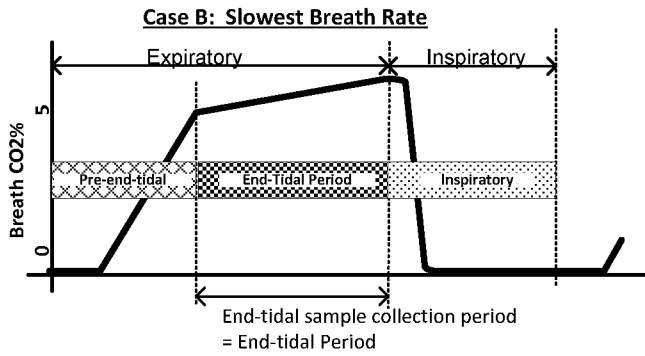


Figure 13C

1320

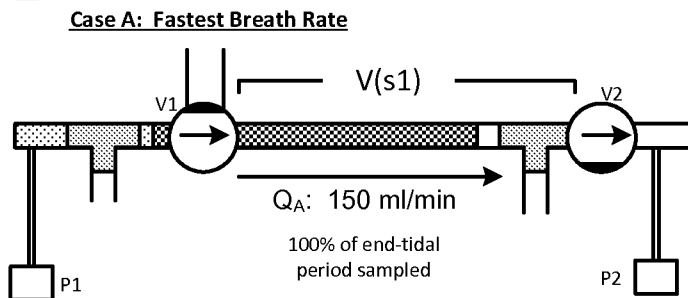


Figure 13D

1330

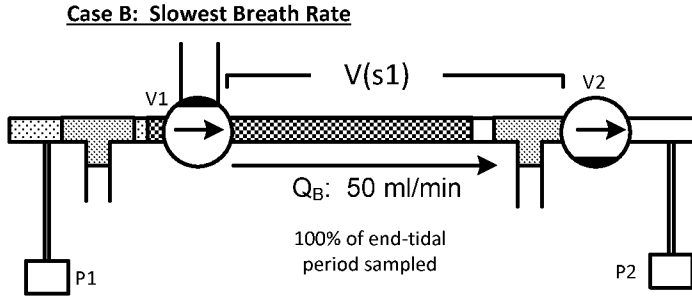


Figure 13E

1340


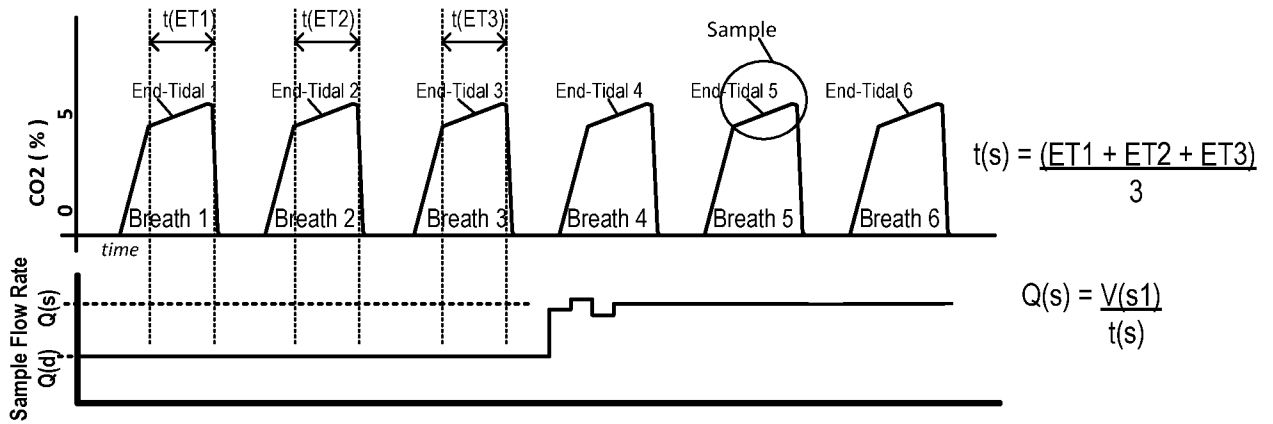


Figure 13F

1350

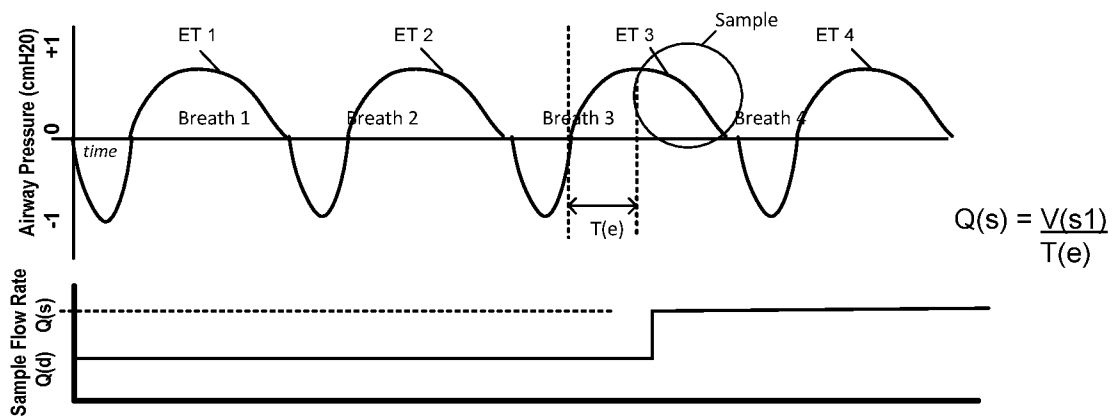

16/20

Figure 14A

1400

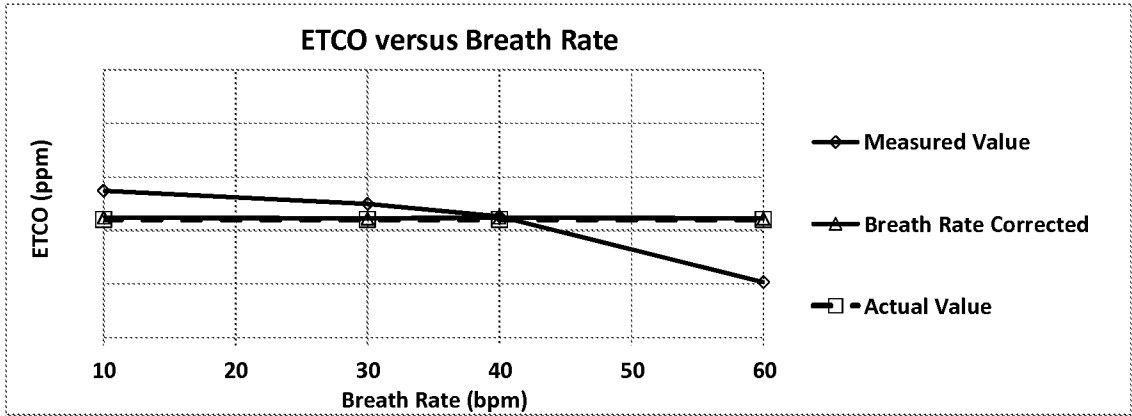


Figure 14B

1420

Linear Breath Rate Correction Factor Equations	
Breath Rate (bpm)	Equations
10 - 30	$y = -M1x + b1$
31 - 40	$y = -M2x + b2$
41 - 60	$y = -M3x + b3$
Polynomial Breath Rate Correction Factor Equations	
Breath Rate (bpm)	Equation
10 - 60	$y = -Ax^2 + Bx + C$
y = ETCO; x = Breath Rate; M = slope; b = y intercept (or offset); A,B&C = polynomial equation constants.	

17/20

Figure 15A

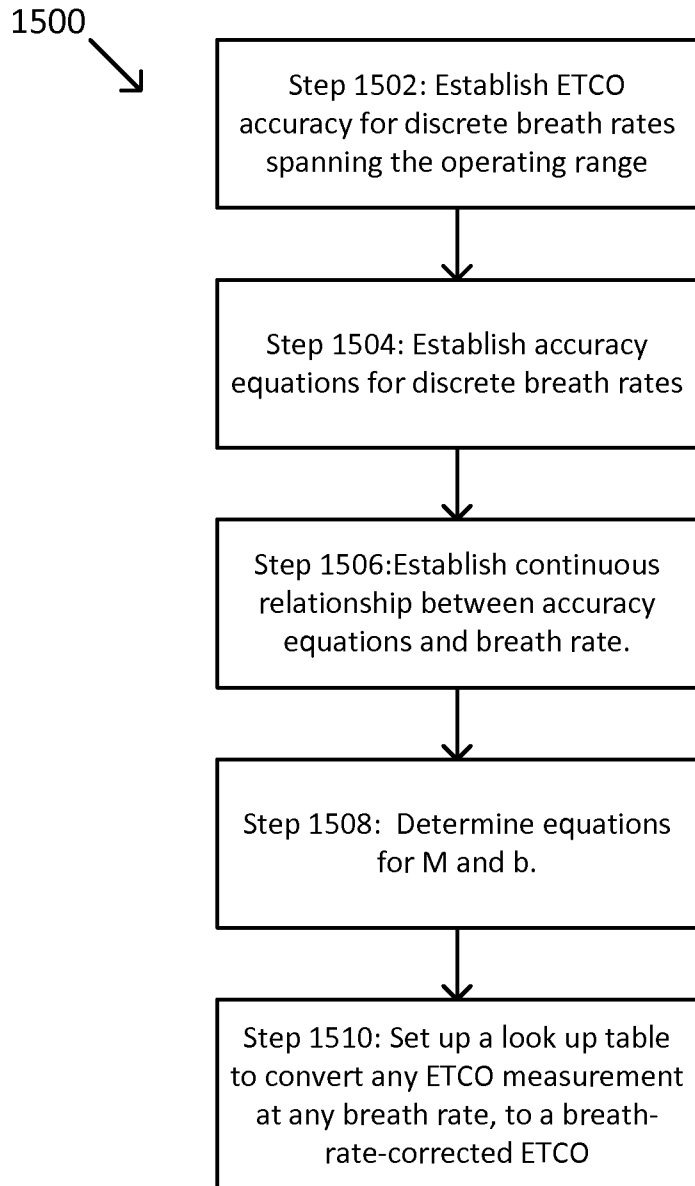


Figure 15B

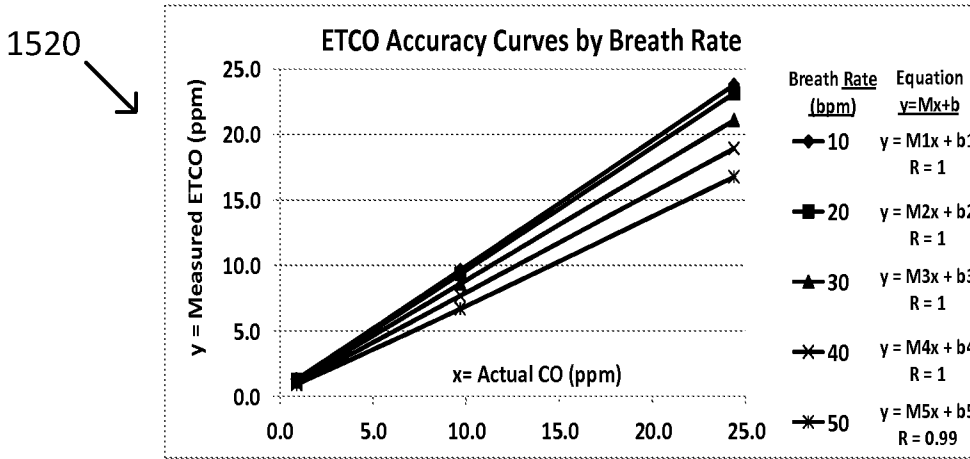


Figure 15C

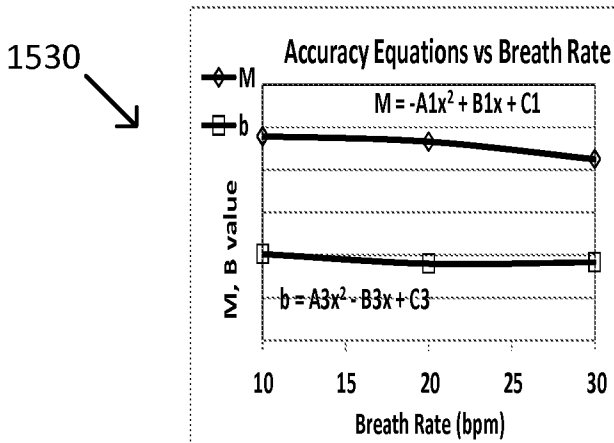


Figure 15D

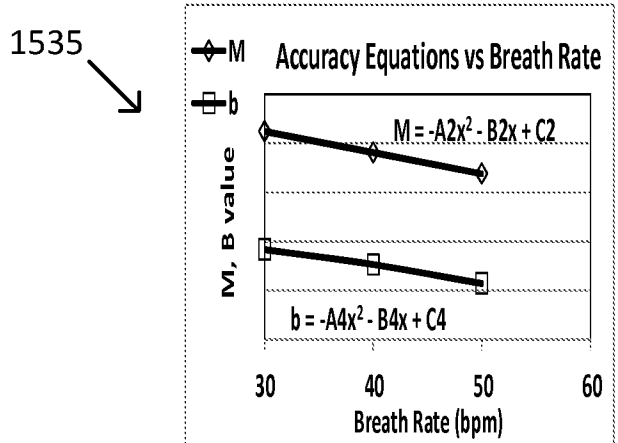


Figure 15E

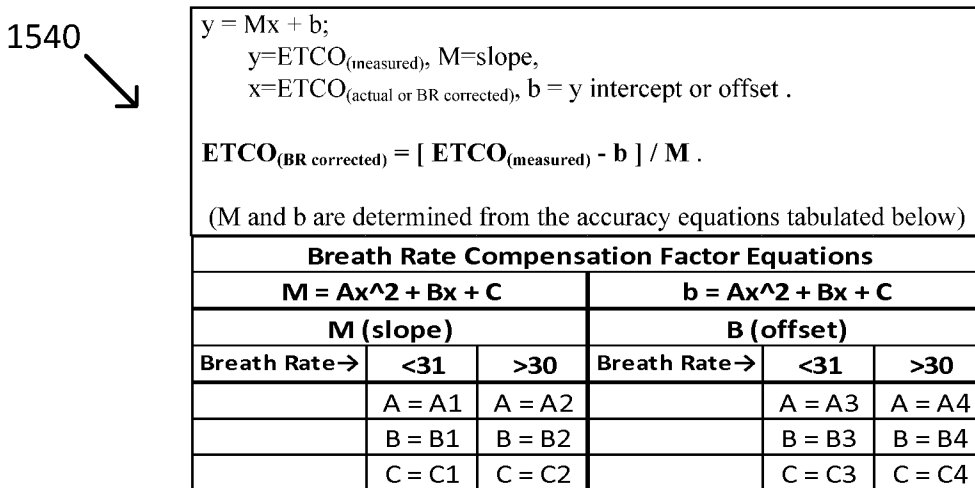


Figure 16A

1600

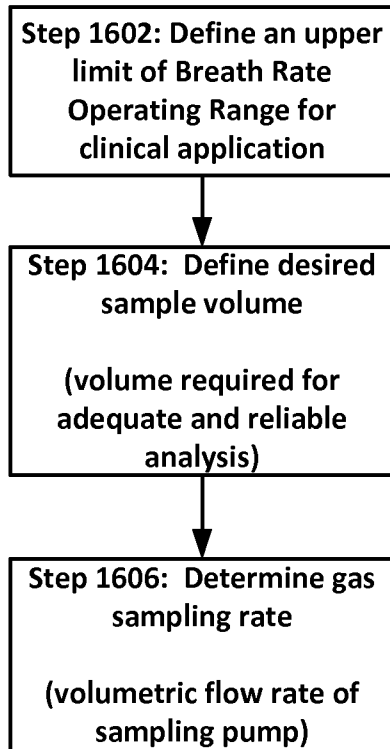


Figure 16B

1620

System samples at fastest breath rate


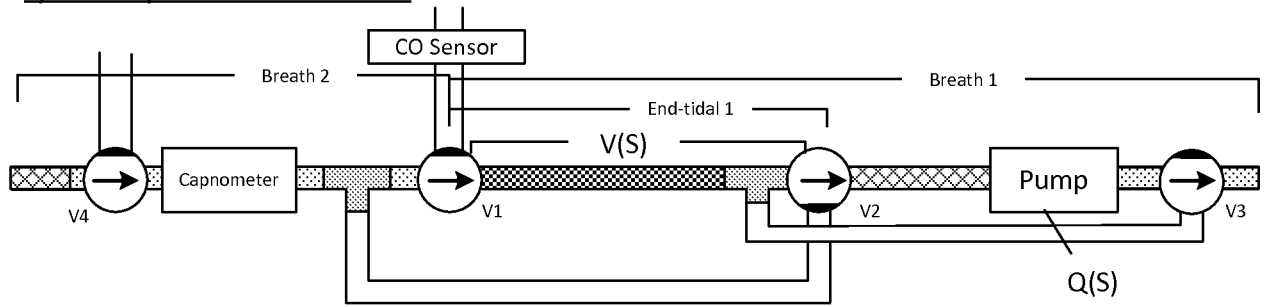


Figure 16C

1640

System samples at slower than fastest breath rate

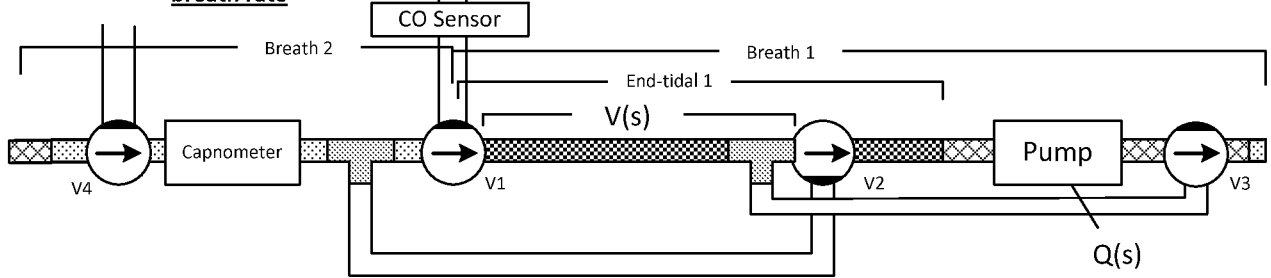

专利名称(译)	呼吸参数频率补偿用于校正呼出气体收集和分析的数据库		
公开(公告)号	EP2794033A4	公开(公告)日	2016-03-30
申请号	EP2012860711	申请日	2012-12-20
[标]申请(专利权)人(译)	卡普尼亚公司		
申请(专利权)人(译)	碳酸血症, INC.		
当前申请(专利权)人(译)	碳酸血症, INC.		
[标]发明人	WONDKA ANTHONY D BHATNAGAR ANISH		
发明人	WONDKA, ANTHONY, D. BHATNAGAR, ANISH		
IPC分类号	A62B27/00 A61B5/00 A61B5/08 A61B5/083 A61B5/097		
CPC分类号	A61B5/097 A61B5/0816 A61B5/082 A61B5/0836 A61B5/7225 A61B5/7285 A61B5/7292		
代理机构(译)	WITTE, WELLER & PARTNER 专利律师 MBB		
优先权	61/578811 2011-12-21 US		
其他公开文献	EP2794033A2		
外部链接	Espacenet		

摘要(译)

描述了用于精确确定患者呼吸样本的气体浓度的装置。该装置可包括样品室, 呼吸速度分析仪, 气体分析仪和处理器。样品室包括接收呼吸的入口。呼吸速度分析仪确定呼吸的一部分的速度。气体分析仪确定气体浓度。处理器包括基于速度确定样品的非均匀度的算法, 以及基于非均匀度的校正气体浓度。在一些变型中, 独立于患者合作确定气体校正。可以基于预期群体的预期呼吸模式范围来调整装置, 使得样本隔室充满均匀的呼气末气体样本, 而不管个体的呼吸模式如何。这些装置可用于例如呼气末CO分析。还描述了方法。