

(19)



(11)

EP 2 830 501 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:

18.05.2016 Bulletin 2016/20

(51) Int Cl.:

G01R 33/30 (2006.01)	G01R 33/46 (2006.01)
G01R 33/48 (2006.01)	A61B 5/00 (2006.01)
A61B 6/00 (2006.01)	A61B 5/055 (2006.01)
A61N 5/10 (2006.01)	A61B 6/03 (2006.01)
G01R 33/58 (2006.01)	

(21) Application number: **13722540.5**

(22) Date of filing: **22.03.2013**

(86) International application number:
PCT/IB2013/052292

(87) International publication number:
WO 2013/144802 (03.10.2013 Gazette 2013/40)

(54) QUALITY ASSURANCE APPARATUS AND METHOD FOR MAGNETIC RESONANCE BASED RADIATION THERAPY PLANNING

QUALITÄTSSICHERUNGSVORRICHTUNG UND VERFAHREN ZUR PLANUNG EINER STRAHLENTHERAPIE AUF MAGNETRESONANZBASIS

APPAREIL ET PROCÉDÉ D'ASSURANCE QUALITÉ DESTINÉS À UN PROGRAMME DE RADIOTHÉRAPIE BASÉE SUR LA RÉSONANCE MAGNÉTIQUE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **KOTYS, Melanie, Suzanne**
5656 AE Eindhoven (NL)
- **DEVARAJ, Ajit**
5656 AE Eindhoven (NL)

(30) Priority: **28.03.2012 US 201261616548 P**

(74) Representative: **Steffen, Thomas**
Philips Intellectual Property & Standards
High Tech Campus 5
5656 AE Eindhoven (NL)

(43) Date of publication of application:
04.02.2015 Bulletin 2015/06

(73) Proprietor: **Koninklijke Philips N.V.**
5656 AE Eindhoven (NL)

(56) References cited:
US-A1- 2003 212 320 US-A1- 2009 226 066
US-A1- 2010 021 029 US-A1- 2010 066 372
US-A1- 2011 229 055 US-B1- 7 056 019

(72) Inventors:
• **FOXALL, David, Leslie**
5656 AE Eindhoven (NL)

EP 2 830 501 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The following relates generally to medical imaging and therapy planning using magnetic resonance imaging. It finds particular application in conjunction with quality assurance of magnetic resonance imaging and medical phantoms, and will be described with particular reference thereto. However, it will be understood that it also finds application in other usage scenarios and is not necessarily limited to the aforementioned application.

[0002] Radiation therapy (RT), brachytherapy and pre-surgical planning involves the use of medical images to determine the best procedure to destroy cancerous tumors. In RT, high energy beams are planned to intersect a target, e.g. a tumor, from multiple angles such that the cumulative radiation dose at the tumor is sufficient to kill the tumor tissue, but the dose from any one angle or beam path is below the threshold so as not to kill non-tumor tissue along the path. High energy beam systems used in RT are either gamma ray systems (e.g. Gamma Knife), electron beam systems (e.g. LINAC), charged particle therapy systems, a proton therapy systems, X-ray therapy systems or external beam radiation systems. In brachytherapy systems, radioactive devices are implanted in the body at the site of the tumor to locally deliver treatment. In surgery, a plan is developed to resect the tumor in the least invasive way. In order to plan for these therapies spatially accurate images are needed. Computed Tomography (CT) images are often used, because CT images are geometrically accurate. However, CT involves the use of x-rays, while magnetic resonance (MR) does not employ x-rays. MR also discriminates soft tissue better than CT. Radiation Therapy also includes the evaluation of radiation treatments with the changes that occur in the tissues at the target site. For example, vital tumor tissue, edema tissue, and necrotic tissue are evaluated differently. However, the magnetic fields and gradients tend to have geometric non-linearities or distortions, particularly towards the periphery of the imaging region. As long as these non-linearities or distortions are accurately mapped to the periphery, resultant images are linear and accurate, even at the edges.

[0003] In order to generate an effective radiation therapy plan, the distortions of the magnetic fields are measured and evaluated to determine if there has been any change. Where the distortions change and a prior distortion correction is applied, the inaccuracies in the planning images are most pronounced towards the edges. Radiation therapy plans are dependent on the geometric accuracy of the MR images. The magnetic field distortion can be significantly changed by small metallic, particularly ferrous, parts such as paper clips, iron filings, coinage, screws, nails, etc. which can slip undetected into the magnet bore.

[0004] The US 2010/80066372 A1 discloses a phantom for use in quality control measurement of a fully integrated magnetic resonance/PET scanner. The phantom features radiation activity distributed throughout an electrically conductive binder. Suitably, the binder is elastomeric and includes carbon fibers distributed throughout it to set the conductivity of the phantom to a desired level. The phantom is applicable to various multimodality integrated medical imaging systems such as MR/SPECT and MR/CT in addition to MR/PET

[0005] _The US 2011/0229055 A1 discloses a phantom for determining the alignment of two or more imaging apparatuses. The phantom comprises a vessel, wherein a cavity is defined by the inner surfaces of the vessel. The cavity is for holding a fluid therein. Two or more rods extend through the cavity, the rods being non-parallel with one another. The US 2009/0226066 A1 discloses a method of determining component misalignment in a multi-modality imaging system including imaging a plurality of target objects with a first modality unit to generate a tomographic image data set and imaging the plurality of targets with a second modality unit to generate an emission image data set. The method also includes determining a location of the target objects in the emission image data set to produce emission target object location coordinates, calculating a positional alignment vector for each target object based on the emission target object location coordinates, and aligning the multi-modality imaging system based on the positional alignment vectors.

[0006] The US 2003/0212320 A1 discloses a method of determining linear and angular displacements of a first coordinate system of a field of view of a first imaging system relative to a second a coordinate system of a field of view of a second imaging system, the method comprising: providing a phantom having a plurality of fiducial regions that can be imaged by both imaging systems; acquiring first and second images of the phantom with the first and second imaging systems wherein spatial coordinates of features in the first and second images reference the first and second coordinate systems respectively; determining positions of a plurality of features of the fiducials in the first image and spatial coordinates of the same features in the second image; and using the coordinates to determine the linear and angular displacements.

[0007] The US 2010/0021029 A1 discloses systems and methods for characterizing spatial distortions in location data determined by an imaging system, for example as employed in imaged guided therapy. A three dimensional phantom is custom formed for a desired imaging space of a given imaging system. The phantom includes a large plurality of control points fixed rigidly in space to a high degree of known accuracy. The phantom is fixed to a stereotactic frame defining a known calibrated reference or zero and imaged.

[0008] The US 7056019 B1 discloses a phantom system providing for the testing of diagnostic machines in a safe and efficient manner. First provided is a transparent cubic test device having a cylindrical aperture extending all the way to the rear face. The test device has a plurality of centered lines, making four equal squares on each face of the test system. There is a plurality of small bores positioned at all intersections of the scored white lines. A probe cylinder may

receive and hold a probe. The cube has additional apertures to hold tissue testing and calibrating devices.

[0009] The present application provides a regular quality assurance process which provides RT planning assurance such that any MR images used in the RT planning process are within an acceptable tolerance. Typically, phantoms are used to determine the geometric accuracy of a MR image. Prior phantoms were often a 2D grid phantoms which were positioned and imaged in different planes, e.g. 3 orthogonal planes. The distortion mapping using a 2D phantom involves repeated imaging with physical movement of the phantom to represent possible imaging planes. The process of multiple images and repeated physical movement of the phantom use valuable clinical time and staff resources. In addition, 2D phantoms did not measure distortion spanning the entire 3D imaged volume, only the positions in which the 2D phantom is placed. The 3D phantoms employed for MR scanner calibration are very heavy, i.e. 45-90 kg (100-200 lbs.). Heavy phantoms are difficult to move physically, and often involve multiple persons and/or mechanical lifts to safely move the phantom into position. Due to the weight, such phantoms may not measure the entire field of view. Current industry standards call for manually lifted containers and packages to about 18 kg (40 lbs) or less. Lighter weights are more easily moved by an individual and are less likely to result in back or other injuries. There are currently no mandatory standards for quality assurance of MR images used in RT planning, but standards are expected to develop and are beneficial for the RT planning process.

[0010] The following discloses a new and improved medical image phantom and quality assurance process for magnetic resonance imaging used in radiation planning which addresses the above referenced issues, and others.

[0011] In accordance with one aspect, a system for quality assurance of a magnetic resonance (MR) imaging device used in magnetic resonance based radiation therapy planning includes a phantom weighing less than 18.2 kg (40 lbs.). The phantom includes a three dimensional spatial distribution of MR and CT imagable elements located in an MR and CT inert foam support, and an MR and CT inert external support structure which surrounds and hermetically seals the foam support. The spatial distribution is sized to completely fill an imaging volume of the magnetic resonance imaging device.

[0012] In accordance with another aspect, a method of quality assurance using a phantom for radiation therapy planning includes manually lifting a medical imaging phantom which weighs less than 18.2 kg into a magnetic resonance (MR) imaging device. The medical imaging phantom includes a three dimensional spatial distribution of MR and CT imagable elements located in an MR and CT inert foam support, and an MR and CT inert external support structure which surrounds and hermetically seals the foam support. The spatial distribution is sized to completely fill an imaging volume of the magnetic resonance imaging device. An MR phantom image is acquired with the MR imaging device. The locations of the imagable elements from the MR phantom image are compared with locations of the imagable elements in a previously acquired CT reference image.

[0013] In accordance with another aspect, a medical imaging phantom weighing less than 18.2 kg (40 lbs.) includes a three dimensional spatial distribution of MR and CT imagable elements located in an MR and CT inert support, and an MR and CT inert external support structure which surrounds and hermetically seals the support. The spatial distribution is sized to completely fill an imaging volume of a magnetic resonance imaging device.

[0014] One advantage resides in a regular, e.g. daily, calibration.

[0015] Another advantage is a lightweight and durable phantom which spans a imaging volume in one imaging data acquisition.

[0016] Another advantage is the low cost, low weight, and high stability of a medical imaging phantom.

[0017] Another advantage resides in the ease of lifting and using the phantom on a daily basis by a single person.

[0018] Another advantage is that the medical imaging phantom does not require a high degree of accuracy to manufacture, but is highly accurate.

[0019] Another advantage is the detection of MR geometric distortions in a full MR imaging volume.

[0020] Another advantage is the quality assurance provided for MR based radiation therapy.

[0021] Still further advantages will be appreciated to those of ordinary skill in the art upon reading and understanding the following detailed description.

[0022] The invention may take form in various components and arrangements of components, and in various steps and arrangement of steps. The drawings are only for purposes of illustrating the preferred embodiments and are not to be construed as limiting the invention.

FIGURE 1 schematically illustrates an embodiment of the medical imaging phantom.

FIGURES 2A-B illustrates various regularly spaced materials tested in the phantom to measure the spatial distortions.

FIGURE 3 schematically illustrates one embodiment of the quality assurance system.

FIGURE 4 flowcharts an embodiment of a phantom calibration.

FIGURE 5 flowcharts an embodiment of a magnetic resonance phantom quality assurance.

FIGURE 6 flowcharts an embodiment of radiation therapy quality assurance.

[0023] With reference to FIGURE 1, an embodiment of a medical imaging phantom **10** is shown. The medical imaging

phantom **10** includes a three dimensional spatial distribution of magnetic resonance and CT imaggable elements **12** in a magnetic resonance and CT inert foam support **14**. The three dimensional spatial distribution can include lattices such as cubic lattices, hexagonal lattices, concentric spheres, concentric cylinders, radial grids, combinations, placement of the imaggable elements on the null points and planes of spherical harmonic functions and the like. The active material of the imaggable elements **12** is held in containers such as soft-gel capsules, which are inserted into wells in the support foam **14**. In one embodiment, the imaggable elements are placed in about 2.5 cm (1 inch) intervals in the x and y directions on sheets of foam. Sheets of foam, approximately 2.5 cm (1 inch) thick are stacked. The size of the intervals can be varied according to the spatial dimensions measured for distortions and the degree of quality to be assured. The sheets of foam ease manufacturing constraints. In one embodiment, the containers of the active material are oval shaped, but can be circular, cylindrical, or any regular shape, particularly shapes whose geometric center is easily calculated. One example includes sealed glass micro-bulbs of the type used in high resolution spectrometers. Another example is over the counter laxative or vitamin E soft-gel capsules. The amount of active material in each capsule is uniform, but can vary. Pharmaceutical standards are sufficient for the dosage such as a standard size 5 capsule. The tolerance of the spacing is about +/- .0508 cm or greater. The tolerance can be large compared with the accuracy, because the accuracy is calibrated by a phantom reference image and not the phantom itself. The chosen spatial distribution of the imaggable elements can help reduce the computational aspects of determining the actual position of the imaggable elements in the MR phantom image.. The larger tolerance also reduces the manufacturing complexity and cost.

[0024] The foam support **14** provides support to the imaggable elements **12** while adding minimal weight. The size of the phantom **10** and the amount of foam and the foam weight to fill the phantom determine the phantom weight. The design provides a phantom less than about 18 kg (40 lbs.) and fills the MR imaging volume. The MR imaging volume spans the entire region in the bore of the MR imaging device where the MR gradient coils are designed to generate linear magnetic field gradients. The low weight permits easy loading and movement by a single individual. In one embodiment, the phantom measures 40 cm x 40 cm x 40 cm and weighs less than 9 kg. The size of the phantom is limited by the bore openings of the imaging devices which use the phantom. The shape of the phantom can be cubic, rectilinear, cylindrical, elliptically cylindrical, or approximate the shape of human anatomy. Foam such as polystyrene, polyethylene, polyvinylchloride (PVC), closed cell foam rubber or polyimide can be used which reduces the overall weight of the phantom. Other foam materials include non-plastic foam such as aerogel. The foam can be molded or cut to the necessary dimensions. Alternatives to foam can include paper, cardboard, balsa wood, and the like. The characteristics of the foam support include moisture proofing, strength, rigidity, wear resistance, low MR signal, and permeability to radio frequency waves.

[0025] The foam support **14** is surrounded by a magnetically inert external support structure **16**, such as acrylic plastic sheets which is hermetically sealed. Other materials for the external support structure include polytetrafluoroethylene (e.g. Teflon), polyoxymethylene (e.g. Delrin), polycarbonate, nylon, fiberglass composite, plywood, etc. The external support structure **16** prevents damage to the foam and shifting of the imaggable elements and enhances durability and stability of the phantom. Optionally, a desiccant can be sealed inside the phantom. Other optional features include feet attached to the base of the phantom to level the phantom after loading in the imaging device. Another optional feature is the inclusion of levelers in two directions such as bubble levels. The levelers can be relative to the support structure or a reference column **18**. Another optional feature are guidelines recessed on the outside of the phantom. The guidelines can be used to align the phantom to an external laser bridge system commonly used to align patient marking in RT.

[0026] Within the foam support **14** is the reference column **18**, such as an acrylic plastic circular or rectilinear tube filled with a material visible to CT and MR imaging devices such as water. The column **18** can be located in a position between any two walls of the external support structure. The column **18** provides a spatial reference and reduces the computational aspects of locating the imaggable elements **12**. The material in the reference column provides a strong signal reference to a central magnetic resonance frequency and for radio frequency power calibration. The reference column also provides a geometric reference in the image planes. The material in the reference column can be the same as the imaggable elements or different.

[0027] In FIGURES 2A-2B, various imaggable elements used in the phantom to measure the spatial distortions are shown in a study. FIGURE 2A shows an MR image of three different materials while FIGURE 2B shows a corresponding CT image of the same materials. The images are of a polystyrene tray with a section of vitamin E soft-gel capsules (i.e. E section), sodium docusate soft-gel capsules (i.e. S section), and calcium docusate soft-gel capsules (i.e. C section). In the MR image, the E section is barely visible while the brightest image is from the S section, followed by the C section. All sections are fairly visible in the CT image, particularly the S section or sodium docusate. The active material of the imaggable elements include commercially available materials at a low cost such as fish oil. A property of the active material includes contrast in both the CT and MR image.

[0028] FIGURE 3 schematically illustrates one embodiment of the quality assurance system **20**. The system **20** includes an x-ray computed tomography (CT) medical imaging device **22**, a magnetic resonance (MR) imaging device **23**, and a radiation treatment device **24**. The imaging devices can be combinations devices or separate devices. Combination devices are typically inherently registered while separate devices require a registration step. Initially, the phantom **10** is

loaded into the bore of the CT imaging device **22** for a full volume image or map filled by the entire phantom **10**. The CT medical imaging device **22** can be at a manufacturing site or can be connected to a network **25** at a medical site which transmits the image and other data. The CT imaging device generates a phantom reference image which shows the actual locations of imagable element **12**. The CT phantom reference image or a map of the geometric centers of the elements **12** based thereon is unique to the calibrated phantom. The phantom and the CT image have unique identifiers that identify them as a corresponding pair. If the CT phantom image is generated remotely, it can be stored on a computer readable storage medium which is shipped with the phantom.

[0029] For daily calibration of the MR imaging device **23**, the phantom **10** is loaded into the MR imaging device and accurately positioned in the field of view. The MR imaging device generates a quality assurance image. The phantom reference image and/or quality assurance image are stored in a data store. The data store can be in local memory, disk, or in a storage management system **26** such as a Picture Archiving and Communication System (PACS), a Radiology Information System (RIS), and the like.

[0030] A workstation **28** connects to the network **25** and a healthcare practitioner activates the quality assurance module **30** using at least one input device **32**. The workstation **28** includes an electronic processor or electronic processing device **34**, a display **36** device which displays the phantom reference image, quality assurance image, and/or quality assurance results, menus, panels, and user controls, and the at least one input device **32** which inputs the healthcare practitioner selections. The workstation **28** can be a desktop computer, a laptop, a tablet, a mobile computing device, a smartphone, and the like. The input device **32** can be a keyboard, a mouse, a microphone, touch screen, and the like. The display device includes one or more of a LCD display, an LED display, a plasma display, a projection display, a touch screen display, and the like.

[0031] The quality assurance module **30** is suitably embodied by an electronic data processing device, such as the electronic processor or electronic processing device **32** of the workstation **28**, or by a network-based server computer operatively connected with the workstation **28** by the network **25**, or so forth. Moreover, the disclosed phantom imaging and comparison are suitably implemented as a non-transitory storage medium storing instructions (e.g., software) readable by an electronic data processing device and executable by the electronic data processing device to perform the disclosed quality assurance techniques.

[0032] The quality assurance module **30** manages and performs the process of quality assurance of the MR imaging device for radiation therapy planning. The process of quality assurance includes the imaging of the phantom by the CT and MR imaging devices, comparison of the phantom images, and the reporting of the results of the quality assurance process. The quality assurance module includes tracking the use of the phantom, the generated phantom reference image, the identification of the phantom, the generated phantom quality assurance image, the currency of the images, how the images are compared, and the amount of distortion of the quality assurance image based on the reference image. Results are displayed to the healthcare practitioner through the display device. Results can include recommendations of success or failure, any remedial actions and/or related informational items.

[0033] With reference to FIGURE 4, an embodiment of the phantom reference image or template creation is flowcharted. In a step **40**, a CT imaging device is initiated and a CT image of the phantom is acquired. The phantom reference image is a 3D volume image of the elements **12**. A template is generated from the phantom reference image in the following steps.

[0034] In a step **42**, the 3D CT image is searched to locate the elements **12**. The reference column **18** and the a priori known expected intervals and tolerances provide references which reduce the computational aspects of finding the actual positions of the imagable elements. Each element is located based on the contrast of the CT image, and any a priori information available. The search can be performed as a coarse segmentation or estimate of the elements using a geometric shape such as a cube.

[0035] A template is generated in a step **44**. The centers of each imagable element are identified using a centering function such as a center of mass and represented in spatial coordinates. The centering function minimizes the error associated with variability of the size and placement of each regularly spaced material. For example, a soft-gel capsule will vary within certain tolerances both in material and in size. By using the center instead of the edges the reference location is more easily identified and associated with other reference locations.

[0036] The template of the centers of the elements **12**, and/or the CT phantom reference image are stored in a step **46**. The phantom reference image and/or template can be stored in the storage management system **26**. The template can include the phantom identification either obtained from the phantom reference image and/or manual entry.

[0037] With reference to FIGURE 5, an embodiment of the phantom quality assurance for the MR imaging device is flowcharted. In a step **48**, the phantom is accurately positioned in the field of view and the MR imaging device is initiated to acquire the MR phantom quality assurance image. The reference column such as an internal tube filled with material can optionally provide a reference to the acquisition process. Optionally, in the step **48**, the signal from the center tube is used to perform a central frequency calibration and/or an RF power calibration. In a step **49**, the CT phantom reference image is acquired, and in a step **50**, the CT phantom reference image and MR quality assurance image are registered.

[0038] The CT phantom reference image is segmented in a step **51**. The CT image is segmented into unit cells based on the phantom design specifications and registration markers. Each unit cell contains one imagable element. In a step

52, the template is generated from the segmented unit cells.

[0039] In a step 54, a search is performed for the imagable elements in the MR image by correlating the location of each template location with the associated unit cells in the MR QA image. The three dimensional ordered distribution of elements are contrasted in the MR image. Each imagable element is located. The reference column and other a priori information about the spatial distribution reduce the computational aspects of locating the imagable elements. The center of each imagable element is computed and compared with the coordinate of the corresponding template or CT phantom reference image element. For example, the center of each element in the template is represented in Cartesian coordinates as (x,y,z) . The corresponding coordinates of the element, $(\bar{x},\bar{y},\bar{z})$, in the MR image can be represented as $\bar{v} = v + \eta_v(v)$ where v is any one of the spatial dimensions (x,y,z) and η_v represents the induced distortion and is given by

10 $\eta_v(x, y, z) = \frac{B_v^N(r, \theta, \phi)}{G_v^L}$, where B_v^N is the non-linear magnetic field due to the v gradient channel expressed in spherical harmonics as:

$$15 \quad B_v^N(r, \theta, \phi) = B_{x(1,0)}(r, \theta, \phi) + \sum_{n=2} \sum_m B_{x(n,m)}(r, \theta, \phi)$$

and

$$20 \quad B_{x(n,m)}(r, \theta, \phi) = r^n [a_{v(n,m)} \cos(m\phi) + b_{v(n,m)} \sin(m\phi)] P_{(n,m)}(\cos \theta)$$

where (r, θ, ϕ) are spherical coordinates. Here, $a_{v(n,m)}$ and $b_{v(n,m)}$ are spherical harmonic co-efficients of degree n and order m . Similarly, $P_{(n,m)}$ is the associated Legendre polynomial of degree n and order m . G_v^L is the linear part of the v gradient channel and is given by $G_x^L = a_{x(1,1)}$, $G_y^L = b_{y(1,1)}$, $G_z^L = a_{z(1,0)}$. A maximum correlation is computed which provides the shift or distortion in 3 dimensions in a step 55.

[0040] Using the computed difference between each center of the element in the MR image and the center of the element in the template or CT phantom reference image, a distortion map is generated in a step 56. The distortion map includes the differences in the centers between the CT phantom reference or template and the MR image. The distortion map can interpolate for all points in the field of view. In a step 58, the distortion map is stored.

[0041] An embodiment of the quality assurance (QA) of MR for radiation therapy planning is flowcharted in FIGURE 6. The QA method includes both steps performed by the healthcare practitioner, those performed by a medical imaging device and/or quality assurance module, and those performed by the healthcare practitioner and guided by the quality assurance module. The quality assurance module guides the overall process beginning in a step 60.

[0042] The quality assurance module verifies the currency of the CT phantom reference map in a step 62. Verifying the currency of the CT phantom includes comparing the date of any stored phantom reference image with the current date and the expected interval based and the recommended standard. For example, if the CT phantom reference image is expected to be updated whenever the phantom is new and/or replaced, or annually, then a new phantom reference image is acquired if the image data is older than one year or if the phantom identification has changed. The phantom identification can be a physical label on the phantom and can also be a label which is contrasted in the image. The identification can be written and/or encoded such as a barcode.

[0043] If a new phantom reference image is to be created, then the quality assurance module can direct the healthcare practitioner to load the phantom into the CT imaging device in a step 64. The phantom is loaded in the imaging area or field of view of the CT imaging device such that a full volume CT image is filled by the phantom. Optional levelers and feet on the phantom aid the healthcare practitioner in the placement and orientation of the phantom in the imaging device. The quality assurance module can optionally demonstrate the process with a short video displayed with the display device or simply provide written instructions. The CT phantom reference map is created in a step 66 and as described with reference to FIGURE 4.

[0044] The currency of the MR QA is checked in a step 68. The currency of the MR QA includes a different periodicity than the CT phantom reference image such as daily. The quality assurance module can optionally verify the schedule for MR RT planning images and modify the periodicity. For example, if no MR RT planning images are scheduled for the day or if a MR QA image has already been acquired based on a MR QA image date, then a MR QA image acquisition is unnecessary.

[0045] If a new MR QA image is indicated, then the phantom is loaded into the MR imaging device in a step 70 by the healthcare practitioner. The phantom is placed in the bore of the imaging device such that the imaging volume is filled

by the phantom. The placement and orientation of the phantom in the imaging device include the step **64** the same as or similar to the loading of the phantom in the CT imaging device. If the devices are a hybrid device and share a common field of view, then the loading is the same. If the devices are separate, then the loading is similar.

[0046] In a step **72**, the phantom identifier is verified. Verification can include visual identification by the healthcare practitioner, entry of an identifier code into the system via the user input device, use of a label included in the phantom quality assurance image, and the like.

[0047] The phantom QA is performed in a step **74** as described in reference to FIGURE 5. The step returns a distortion map. The distortion map includes the computed differences between the CT phantom reference image or template and the MR phantom image or MR QA image. The distortion map represents changes in the spatial coordinates of the MR device which can occur in a MR RT image.

[0048] The distortion map is checked in a step **76**. Threshold values are employed to determine if the distortions are within acceptable levels for quality assurance. The distortion map can be displayed via the display device as graphical images and/or statistical graphs and/or numeric representations such as mean, variance, maximum variance, mean variance, and the like. The magnitude of the distortions or degree of shift can be displayed using color contrasts. Visualizations of the distortions are facilitated in any arbitrary plane by the interpolation included in the distortion map. The display plane can be extracted from a 3D matrix resulting from the interpolated distortion map.

[0049] If distortions are not within acceptable levels, then the system provides notice in a step **78**. Notice can include display of a message on the display device **36**. Notice can include recording statistics or other information regarding the measured distortions for future analysis. Notice can also include display of the distortion map. The step can provide iterative corrections and return to earlier steps to determine whether corrections are effective. If distortions are within or have been brought within acceptable levels, then notification occurs in a step **80**.

[0050] If the centers match within a predefined tolerance, a calibration successful message is generated on the display **36** in a step **80**. The calibration successful message can include display of the distortion map and/or other statistics relevant to radiation therapy planning.

[0051] The generated distortion map can also be generated by comparing a user acquired CT image of the phantom with the stored CT reference image of the phantom, which provides a quality check on the mechanical integrity of the phantom. The distortion maps can also be compared over time such as over the course of a patient's treatment. For example, a statistic such as a minimum, mean, maximum can be plotted to compute the differences in distortion values for each imagable element.

[0052] It is to be appreciated that in connection with the particular illustrative embodiments presented herein certain structural and/or function features are described as being incorporated in defined elements and/or components. However, it is contemplated that these features may, to the same or similar benefit, also likewise be incorporated in other elements and/or components where appropriate. It is also to be appreciated that different aspects of the exemplary embodiments may be selectively employed as appropriate to achieve other alternate embodiments suited for desired applications, the other alternate embodiments thereby realizing the respective advantages of the aspects incorporated therein.

[0053] It is also to be appreciated that particular elements or components described herein may have their functionality suitably implemented via hardware, software, firmware or a combination thereof. Additionally, it is to be appreciated that certain elements described herein as incorporated together may under suitable circumstances be stand-alone elements or otherwise divided. Similarly, a plurality of particular functions described as being carried out by one particular element may be carried out by a plurality of distinct elements acting independently to carry out individual functions, or certain individual functions may be split-up and carried out by a plurality of distinct elements acting in concert. Alternately, some elements or components otherwise described and/or shown herein as distinct from one another may be physically or functionally combined where appropriate.

Claims

1. A system (20) comprising:

a magnetic resonance (MR) imaging device (**23**) having an imaging volume of the MR imaging device; and a phantom for quality assurance of the magnetic resonance (MR) imaging device (**23**), the phantom (**10**) weighing less than 18.2 kg (40 lbs.), and including:

a three dimensional spatial distribution of MR and computer tomography (CT) imagable elements (**12**) located in an MR and CT inert foam support (**14**), the spatial distribution being sized to completely fill the imaging volume; and

an MR and CT inert external support structure (**16**) which surrounds and hermetically seals the foam support. **characterised by** a reference column for spatial referencing of the imagable elements, the reference column

being filled with material which provides a strong signal reference to a central magnetic resonance frequency of the MR imaging device.

2. The system (20) according to claim 1, further including:

one or more processors configured to:

acquire (50) an MR image of the phantom with the MR imaging device (23);
identify locations of the imagable elements in the MR phantom image;
compare (56) the locations of the imagable elements from the MR phantom image with locations of the imagable elements in a previously acquired CT reference image.

3. The system (20) according to claim 2, wherein the one or more processors are further configured to:

acquire the CT reference image of the phantom from a CT imaging device;
register the CT reference image and the MR image;
segment the CT image into unit cells based on the spatial distribution of imagable elements such that each imagable element is in one unit cell;
generate a template which includes the location of each imagable element;
correlate the location of each imagable element in the template with an associated volume in the MR image;
compute the maximum correlation; and
generate a distortion map based on the maximum correlation.

4. The system according to any one of claims 1-3, wherein the material further provides at least one of:

a strong signal reference for radio frequency power calibration; and a geometric reference in image planes.

5. The system according to any one of claims 2-4, wherein the one or more processors are further configured to:

compare an acquired CT image of the phantom with the previously acquired CT reference image.

6. The system according to any one of claims 2-5, further including:

a non-transitory computer readable medium storage carrying at least one of the CT phantom image or the MR phantom image.

7. The system (20) according to any one of claims 1-6, wherein the magnetic resonance imaging device generates images used in radiation therapy planning.

8. The system (20) according to any one of claims 1-7, wherein the phantom (10) includes at least 40 cm in each of three spatial dimensions.

9. The system (20) according to any one of claims 1-8, wherein the phantom further includes at least one of:

a desiccant sealed inside the phantom;
feet attached to the base of the phantom which level the phantom;
levels in two directions which indicate the level of the phantom; and
guidelines recessed on the outside of the phantom.

10. The system (20) according to any one of claims 1-9, wherein the foam support (14) includes at least one of:

polystyrene;
polypropylene;
polyvinylchloride (PVC);
closed cell foam rubber;
aerogel;
paper;
cardboard;

balsa wood;
polyethylene; and
polyimide.

5 11. The system (20) according to any one of claims 1-10, wherein the external support structure (16) includes at least one of:

acrylic plastic;
polytetrafluoroethylene;
10 polyoxymethylene;
polycarbonate;
polythene;
polypropylene;
nylon;
15 fiberglass composite; and
plywood.

12. A method of quality assurance using a phantom for radiation therapy planning, comprising:

20 manually lifting (70) a medical imaging phantom which weighs less than 18.2 kg into a magnetic resonance (MR) imaging device, and the medical imaging phantom includes:

a three dimensional spatial distribution of MR and CT imagable elements (12) located in an MR and computer
tomography (CT) inert foam support (14), the spatial distribution being sized to completely fill an imaging
25 volume of the magnetic resonance imaging device;
a reference column, for spatial referencing of the imagable elements, the reference column being filled with
material which provides a strong signal reference to a central magnetic resonance frequency of the MR
imaging device; and
an MR and CT inert external support structure (16) which surrounds and hermetically seals the foam support;
30 acquiring (50) an MR phantom image with the MR imaging device, wherein the signal reference of the
reference column is used for the spatial referencing of the imagable elements, wherein the acquiring of the
MR phantom image with the MR imaging device comprises identifying the signal reference to the central
magnetic resonance frequency;
35 comparing (56) the locations of the imagable elements from the MR phantom image with locations of the
imagable elements in a previously acquired CT reference image.

13. The method according to claims 12, further including:

acquiring the CT reference image of the phantom from a CT imaging device;
40 registering the CT reference image and the MR image;
segmenting the CT image into unit cells based on the spatial distribution of imagable elements such that each
imagable element is in one unit cell;
generating a template which includes the location of each imagable element;
correlating the location of each imagable element in the template with an associated volume in the MR image;
45 computing the maximum correlation; and
generating a distortion map based on the maximum correlation.

14. The method according to claim 12, wherein distortion maps generated over time are compared.

50 15. The method according to any one of claims 12-14, further including:

calculating the centers of each imagable element in MR coordinates $\overline{(x, y, z)}$ using CT coordinates (x, y, z) , rep-
resented as $\overline{\mathbf{v}} = \mathbf{v} + \eta_{\mathbf{v}}(x, y, z)$ where \mathbf{v} is any one of the spatial dimensions (x, y, z) , and $\eta_{\mathbf{v}}$ represents the induced
55 distortion and is given by $\eta_{\mathbf{v}}(x, y, z) = \frac{\mathbf{B}_{\mathbf{v}}^N(r, \theta, \phi)}{G_{\mathbf{v}}^L}$, where $\mathbf{B}_{\mathbf{v}}^N$ is the non-linear magnetic field due to the
 \mathbf{v} gradient channel expressed in spherical harmonics as:

$$\mathbf{B}_0^N(r, \theta, \phi) = \mathbf{B}_{x(1,0)}(r, \theta, \phi) + \sum_{n=2} \sum_m \mathbf{B}_{x(n,m)}(r, \theta, \phi)$$

5 and

$$\mathbf{B}_{x(n,m)}(r, \theta, \phi) = r^n [\mathbf{a}_{v(n,m)} \cos(m\phi) + \mathbf{b}_{v(n,m)} \sin(m\phi)] \mathbf{P}_{(n,m)}(\cos \theta)$$

10 where (r, θ, ϕ) are spherical coordinates, $\mathbf{a}_{v(n,m)}$ and $\mathbf{b}_{v(n,m)}$ are spherical harmonic coefficients of degree n and order m , and $\mathbf{P}_{(n,m)}$ is the associated Legendre polynomial of degree n and order m .

16. The method according to any one of claims 12-15, further including:

15 verifying (72) the phantom of the first image is the same as the phantom of the second image based on an identity of the phantom; and displaying on the display device a message that the calibration is successful.

17. The method according to any one of claims 12-16, wherein wherein the acquiring of the MR phantom image with the MR imaging device further comprises at least one of:

identifying a signal reference for radio frequency power calibration; and identifying a geometric reference in image planes.

25

Patentansprüche

1. System (20), das Folgendes umfasst:

30 eine Magnetresonanz- (MR) Bildgebungsrichtung (23) mit einem Bildgebungsvolumen der MR-Bildgebungsrichtung; und ein Phantom zur Qualitätssicherung der Magnetresonanz- (MR) Bildgebungsrichtung (23), wobei das Phantom (10) weniger als 18,2 kg (40 lbs) wiegt und Folgendes umfasst:

35 eine dreidimensionale räumliche Verteilung von mit MR und Computertomographie (CT) darstellbaren Elementen (12), angeordnet in einem MR- und CT-inerten Schaumträger (14), wobei die räumliche Verteilung bemessen ist, um das Bildgebungsvolumen vollständig zu füllen; und eine MR- und CT-inerte externe Stützstruktur (16), die den Schaumträger umgibt und hermetisch abdichtet,

40 **gekennzeichnet durch** eine Referenzsäule zum räumlichen Referenzieren der darstellbaren Elemente, wobei die Referenzsäule mit Material gefüllt ist, das eine starke Signalreferenz auf eine zentrale Magnetresonanzfrequenz der MR-Bildgebungsrichtung bereitstellt.

2. System (20) nach Anspruch 1, das weiterhin Folgendes umfasst:

45 einen oder mehrere Prozessoren, die konfiguriert sind zum:
Erfassen (50) eines MR-Bilds des Phantoms mit der MR-Bildgebungsrichtung (23);
Identifizieren von Orten der darstellbaren Elemente in dem MR-Phantombild;
50 Vergleichen (56) der Orte der darstellbaren Elemente aus dem MR-Phantombild mit Orten der darstellbaren Elemente in einem zuvor erfassten CT-Referenzbild.

3. System (20) nach Anspruch 2, wobei der eine oder mehrere Prozessoren weiterhin konfiguriert sind zum:

55 Erfassen des CT-Referenzbilds des Phantoms von einer CT-Bildgebungsrichtung;
Registrieren des CT-Referenzbilds mit dem MR-Bild;
Segmentieren des CT-Bilds in Einheitszellen basierend auf der räumlichen Verteilung von darstellbaren Ele-

EP 2 830 501 B1

menten, so dass sich jedes darstellbare Element in einer Einheitszelle befindet;
Erzeugen einer Vorlage, die den Ort jedes darstellbaren Elements enthält;
Korrelieren des Orts jedes darstellbaren Elements in der Vorlage mit einem zugehörigen Volumen in dem MR-Bild;
5 Berechnen der maximalen Korrelation; und
Erzeugen einer Verzerrungskarte basierend auf der maximalen Korrelation.

4. System nach einem der Ansprüche 1 bis 3, wobei das Material weiterhin mindestens eines von Folgendem bereitstellt:

10 eine starke Signalreferenz zur Hochfrequenzleistungskalibrierung; und
eine geometrische Referenz in Bildebenen.

5. System nach einem der Ansprüche 2 bis 4, wobei der eine oder mehrere Prozessoren weiterhin konfiguriert sind zum:

15 Vergleichen eines erfassten CT-Bilds des Phantoms mit dem zuvor erfassten CT-Referenzbild.

6. System nach einem der Ansprüche 2 bis 5, das weiterhin Folgendes umfasst:

20 einen nicht-flüchtigen computerlesbaren Mediumspeicher, in dem mindestens entweder ein CT-Phantombild
oder das MR-Phantombild gespeichert ist.

7. System (20) nach einem der Ansprüche 1 bis 6, wobei die Magnetresonanz-Bildgebungsvorrichtung Bilder erzeugt,
die bei der Strahlentherapieplanung verwendet werden.

25 8. System (20) nach einem der Ansprüche 1 bis 7, wobei das Phantom (10) mindestens 40 cm in jeder von drei
räumlichen Dimensionen umfasst.

9. System (20) nach einem der Ansprüche 1 bis 8, wobei das Phantom weiterhin mindestens eines von Folgendem
umfasst:

30 ein innerhalb des Phantoms verschlossenes Trocknungsmittel;
an der Basis des Phantoms angebrachte Füße, die das Phantom nivellieren;
Ebenen in zwei Richtungen, die die Ebene des Phantoms angeben; und
auf der Außenseite des Phantoms eingelassene Führungslinien.

35 10. System (20) nach einem der Ansprüche 1 bis 9, wobei der Schaumträger (14) mindestens eines von Folgendem
umfasst:

40 Polystyrol;
Polypropylen;
Polyvinylchlorid (PVC);
geschlossenzelligen Schaumstoff;
Aerogel;
Papier;
45 Pappe;
Balsaholz;
Polyethylen; und
Polyimid.

50 11. System (20) nach einem der Ansprüche 1 bis 10, wobei die externe Stützstruktur (16) eines von Folgendem umfasst:

55 Akrylkunststoff;
Polytetrafluoroethylen;
Polyoxymethylen;
Polycarbonat;
Polyäthylen;
Polypropylen;
Nylon;

Glasfaserverbundstoff;
Sperrholz.

12. Verfahren der Qualitätssicherung unter Verwendung eines Phantoms zur Strahlentherapieplanung, umfassend:

manuelles Heben (70) eines Phantoms zur medizinischen Bildgebung, das weniger als 18,2 kg wiegt, in eine Magnetresonanz- (MR) Bildgebungsvorrichtung, und wobei das Phantom zur medizinischen Bildgebung Folgendes umfasst:

eine dreidimensionale räumliche Verteilung von mit MR und CT darstellbaren Elementen (12), angeordnet in einem MR- und Computertomographie- (CT) inerten Schaumträger (14), wobei die räumliche Verteilung bemessen ist, um ein Bildgebungsvolumen der Magnetresonanz-Bildgebungsvorrichtung vollständig zu füllen;

eine Referenzsäule zum räumlichen Referenzieren der darstellbaren Elemente, wobei die Referenzsäule mit Material gefüllt ist, das eine starke Signalreferenz auf eine zentrale Magnetresonanzfrequenz der MR-Bildgebungsvorrichtung bereitstellt; und

eine MR- und CT-inerte externe Stützstruktur (16), die den Schaumträger umgibt und hermetisch abdichtet; Erfassen (50) eines MR-Phantombilds mit der MR-Bildgebungsvorrichtung, wobei die Signalreferenz der Referenzsäule zum räumlichen Referenzieren der darstellbaren Elemente verwendet wird, wobei das Erfassen des MR-Phantombilds mit der MR-Bildgebungsvorrichtung das Identifizieren der Signalreferenz auf eine zentrale Magnetresonanzfrequenz umfasst;

Vergleichen (56) der Orte der darstellbaren Elemente aus dem MR-Phantombild mit Orten der darstellbaren Elemente in einem zuvor erfassten CT-Referenzbild.

13. Verfahren nach Anspruch 12, das weiterhin Folgendes umfasst:

Erfassen des CT-Referenzbilds des Phantoms von einer CT-Bildgebungsvorrichtung;

Registrieren des CT-Referenzbilds mit dem MR-Bild;

Segmentieren des CT-Bilds in Einheitszellen basierend auf der räumlichen Verteilung von darstellbaren Elementen, so dass sich jedes darstellbare Element in einer Einheitszelle befindet;

Erzeugen einer Vorlage, die den Ort jedes darstellbaren Elements enthält;

Korrelieren des Orts jedes darstellbaren Elements in der Vorlage mit einem zugehörigen Volumen in dem MR-Bild;

Berechnen der maximalen Korrelation; und

Erzeugen einer Verzerrungskarte basierend auf der maximalen Korrelation.

14. Verfahren nach Anspruch 12, wobei die über die Zeit erzeugten Verzerrungskarten verglichen werden.

15. Verfahren nach einem der Ansprüche 12 bis 14, das weiterhin Folgendes umfasst:

Berechnen des Zentrums jedes darstellbaren Elements in MR-Koordinaten $(\bar{x}, \bar{y}, \bar{z})$ unter Verwendung von CT-Koordinaten (x, y, z) , dargestellt als $\bar{v} = v + \eta_v(x, y, z)$, wobei v eine der räumlichen Dimensionen (x, y, z) ist und

η_v die induzierte Verzerrung darstellt und gegeben ist durch $\eta_v(x, y, z) = \frac{B_v^N(\tau, \theta, \phi)}{G_v^L}$, wobei B_v^N das

nicht-lineare Magnetfeld aufgrund des v Gradientenkanals ist, ausgedrückt in sphärischen Harmonischen als:

$$B_v^N(\tau, \theta, \phi) = B_{x(1,0)}(\tau, \theta, \phi) + \sum_{n=2} \sum_m B_{x(n,m)}(\tau, \theta, \phi)$$

und

$$B_{x(n,m)}(\tau, \theta, \phi) = r^n [a_{v(n,m)} \cos(m\phi) + b_{v(n,m)} \sin(m\phi)] P_{(n,m)}(\cos\theta)$$

wobei (τ, θ, ϕ) sphärische Koordinaten sind, $a_{v(n,m)}$ und $b_{v(n,m)}$ sphärische harmonische Koeffizienten des Grads

EP 2 830 501 B1

n und der Ordnung m sind, und $P_{(n,m)}$ das zugehörige Legendre-Polynom des Grads n und der Ordnung m ist.

16. Verfahren nach einem der Ansprüche 12 bis 15, das weiterhin Folgendes umfasst:

5 Verifizieren (72), dass das Phantoms des ersten Bilds das gleiche ist wie das Phantom des zweiten Bilds, basierend auf einer Identität des Phantoms; und
Anzeigen einer Meldung auf der Anzeigevorrichtung, dass die Kalibrierung erfolgreich war.

10 17. Verfahren nach einem der Ansprüche 12 bis 16, wobei das Erfassen des MR-Phantombilds mit der MR-Bildgebungsvorrichtung weiterhin mindestens eines von Folgendem umfasst:

Identifizieren einer Signalreferenz für die Hochfrequenzleistungskalibrierung; und
Identifizieren einer geometrischen Referenz in Bildebenen.

15

Revendications

1. Système (20), comprenant :

20 un dispositif d'imagerie par résonance magnétique (MR) (23) possédant un volume d'imagerie du dispositif d'imagerie par MR ; et
un fantôme pour assurance de qualité du dispositif d'imagerie par résonance magnétique (MR) (23), le fantôme (10) pesant moins de 18,2 kg (40 livres), et incluant :

25 une distribution spatiale tridimensionnelle d'éléments pouvant être imagés par MR et par tomographie par ordinateur (CT) (12) situés dans un support en mousse inerte de MR et de CT (14), la distribution spatiale étant dimensionnée pour remplir complètement le volume d'imagerie ; et

une structure de support externe inerte de MR et de CT (16) qui entoure et scelle hermétiquement le support en mousse ;

30 **caractérisé par** une colonne de référence pour référencement spatial des éléments pouvant être imagés, la colonne de référence étant remplie avec un matériau qui fournit une référence de signal fort à une fréquence de résonance magnétique centrale du dispositif d'imagerie par MR.

35 2. Système (20) selon la revendication 1, incluant en outre :

un ou plusieurs processeurs configurés pour :

acquérir (50) une image par MR du fantôme avec le dispositif d'imagerie par MR (23) ;

identifier des localisations des éléments pouvant être imagés dans l'image de fantôme par MR ;

40 comparer (56) les localisations des éléments pouvant être imagés à partir de l'image de fantôme par MR à des localisations des éléments pouvant être imagés dans une image de référence par CT acquise auparavant.

45 3. Système (20) selon la revendication 2, dans lequel le ou les processeurs sont en outre configurés pour :

acquérir l'image de référence par CT du fantôme à partir d'un dispositif d'imagerie par CT ;

faire coïncider l'image de référence par CT et l'image par MR ;

segmenter l'image par CT en cellules unitaires en fonction de la distribution spatiale d'éléments pouvant être imagés de telle sorte que chaque élément pouvant être imagé soit dans une cellule unitaire ;

50 générer un modèle qui inclut la localisation de chaque élément pouvant être imagé ;

corrélérer la localisation de chaque élément pouvant être imagé dans le modèle avec un volume associé dans l'image par MR ;

calculer la corrélation maximum ; et

55 générer une carte de distorsion en fonction de la corrélation maximum.

4. Système selon l'une quelconque des revendications 1 à 3, dans lequel le matériau fournit en outre au moins l'une parmi :

EP 2 830 501 B1

une référence de signal fort pour étalonnage de puissance de radiofréquence ; et
une référence géométrique dans des plans d'image.

5 5. Système selon l'une quelconque des revendications 2 à 4, dans lequel le ou les processeurs sont en outre configurés pour :

comparer une image par CT acquise du fantôme à l'image de référence par CT acquise auparavant.

10 6. Système selon l'une quelconque des revendications 2 à 5, incluant en outre :

un stockage non transitoire à support lisible par ordinateur portant au moins l'une parmi l'image de fantôme par CT ou l'image de fantôme par MR.

15 7. Système (20) selon l'une quelconque des revendications 1 à 6, dans lequel le dispositif d'imagerie par résonance magnétique génère des images utilisées dans la planification de radiothérapie.

8. Système (20) selon l'une quelconque des revendications 1 à 7, dans lequel le fantôme (10) inclut au moins 40 cm dans chacune de trois dimensions spatiales.

20 9. Système (20) selon l'une quelconque des revendications 1 à 8, dans lequel le fantôme inclut en outre au moins l'un parmi :

un déshydratant scellé à l'intérieur du fantôme ;
des pieds fixés à la base du fantôme qui mettent le fantôme de niveau ;
25 des niveaux dans deux directions qui indiquent le niveau du fantôme ; et
des lignes guides évidées sur l'extérieur du fantôme.

30 10. Système (20) selon l'une quelconque des revendications 1 à 9, dans lequel le support en mousse (14) inclut au moins l'un parmi :

du polystyrène ;
du polypropylène ;
du chlorure de polyvinyle (PVC) ;
du caoutchouc en mousse à alvéoles fermées ;
35 de l'aérogel ;
du papier ;
du carton ;
du bois balsa ;
du polyéthylène ; et
40 du polyimide.

11. Système (20) selon l'une quelconque des revendications 1 à 10, dans lequel la structure de support externe (16) inclut au moins l'un parmi :

45 du plastique acrylique ;
du polytétrafluoroéthylène ;
du polyoxyméthylène ;
du polycarbonate ;
du polythène ;
50 du polypropylène ;
du nylon ;
un composite de fibre de verre ; et
du contreplaqué.

55 12. Procédé d'assurance de qualité utilisant un fantôme pour planification de radiothérapie, comprenant :

le levage manuel (70) d'un fantôme d'imagerie médicale qui pèse moins de 18,2 kg dans un dispositif d'imagerie par résonance magnétique (MR), et le fantôme d'imagerie médicale inclut :

une distribution spatiale tridimensionnelle d'éléments pouvant être imagés par MR et par CT (12) situés dans un support en mousse inerte de MR et de tomodensitométrie (CT) (14), la distribution spatiale étant dimensionnée pour remplir complètement un volume d'imagerie du dispositif d'imagerie par résonance magnétique ;

une colonne de référence, pour référencement spatial des éléments pouvant être imagés, la colonne de référence étant remplie avec un matériau qui fournit une référence de signal fort à une fréquence de résonance magnétique centrale du dispositif d'imagerie par MR ; et

une structure de support externe inerte de MR et de CT (16) qui entoure et scelle hermétiquement le support en mousse ;

l'acquisition (50) d'une image de fantôme par MR avec le dispositif d'imagerie par MR, dans lequel la référence de signal de la colonne de référence est utilisée pour le référencement spatial des éléments pouvant être imagés, dans lequel l'acquisition de l'image de fantôme par MR avec le dispositif d'imagerie par MR comprend l'identification de la référence de signal à la fréquence de résonance magnétique centrale ; la comparaison (56) des localisations des éléments pouvant être imagés à partir de l'image de fantôme par MR à des localisations des éléments pouvant être imagés dans une image de référence par CT acquise auparavant.

13. Procédé selon la revendication 12, incluant en outre :

l'acquisition de l'image de référence par CT du fantôme à partir d'un dispositif d'imagerie par CT ;
la mise en coïncidence de l'image de référence par CT et de l'image par MR ;
la segmentation de l'image par CT en cellules unitaires en fonction de la distribution spatiale d'éléments pouvant être imagés de telle sorte que chaque élément pouvant être imagé soit dans une cellule unitaire ;
la génération d'un modèle qui inclut la localisation de chaque élément pouvant être imagé ;
la corrélation de la localisation de chaque élément pouvant être imagé dans le modèle avec un volume associé dans l'image par MR ;
le calcul de la corrélation maximum ; et
la génération d'une carte de distorsion en fonction de la corrélation maximum.

14. Procédé selon la revendication 12, dans lequel des cartes de distorsions générées au fil du temps sont comparées.

15. Procédé selon l'une quelconque des revendications 12 à 14, incluant en outre :

le calcul des centres de chaque élément pouvant être imagé dans des coordonnées de MR $(\overline{x, y, z})$ en utilisant des coordonnées de CT (x, y, z) , représentées sous la forme $\overline{v} = v + \eta_v(x, y, z)$ où v est l'une quelconque des dimensions spatiales (x, y, z) , et η_v représente la distorsion induite et est donné par

$$\eta_v(x, y, z) = \frac{B_v^N(r, \theta, \phi)}{G_v^L}$$

où B_v^N est le champ magnétique non linéaire dû au canal de gradient v exprimé en harmoniques sphériques par :

$$B_v^N(r, \theta, \phi) = B_{x(1,0)}(r, \theta, \phi) + \sum_{n=2} \sum_m B_{x(n,m)}(r, \theta, \phi)$$

et

$$B_{x(n,m)}(r, \theta, \phi) = r^n [a_{v(n,m)} \cos(m\phi) + b_{v(n,m)} \sin(m\phi)] P_{(n,m)}(\cos \theta)$$

où (r, θ, ϕ) sont des coordonnées sphériques, $a_{v(n,m)}$ et $b_{v(n,m)}$ sont des coefficients d'harmoniques sphériques de degré n et d'ordre m , et $P_{(n,m)}$ est le polynôme de Legendre associé de degré n et d'ordre m .

EP 2 830 501 B1

16. Procédé selon l'une quelconque des revendications 12 à 15, incluant en outre :

la vérification (72) que le fantôme de la première image est le même que le fantôme de la seconde image en fonction d'une identité du fantôme ; et

5 l'affichage, sur le dispositif d'affichage, d'un message indiquant que l'étalonnage est réussi.

17. Procédé selon l'une quelconque des revendications 12 à 16, dans lequel l'acquisition de l'image de fantôme par MR avec le dispositif d'imagerie par MR comprend en outre au moins l'une parmi :

10 l'identification d'une référence de signal pour l'étalonnage de puissance de radiofréquence ; et
l'identification d'une référence géométrique dans des plans d'image.

15

20

25

30

35

40

45

50

55

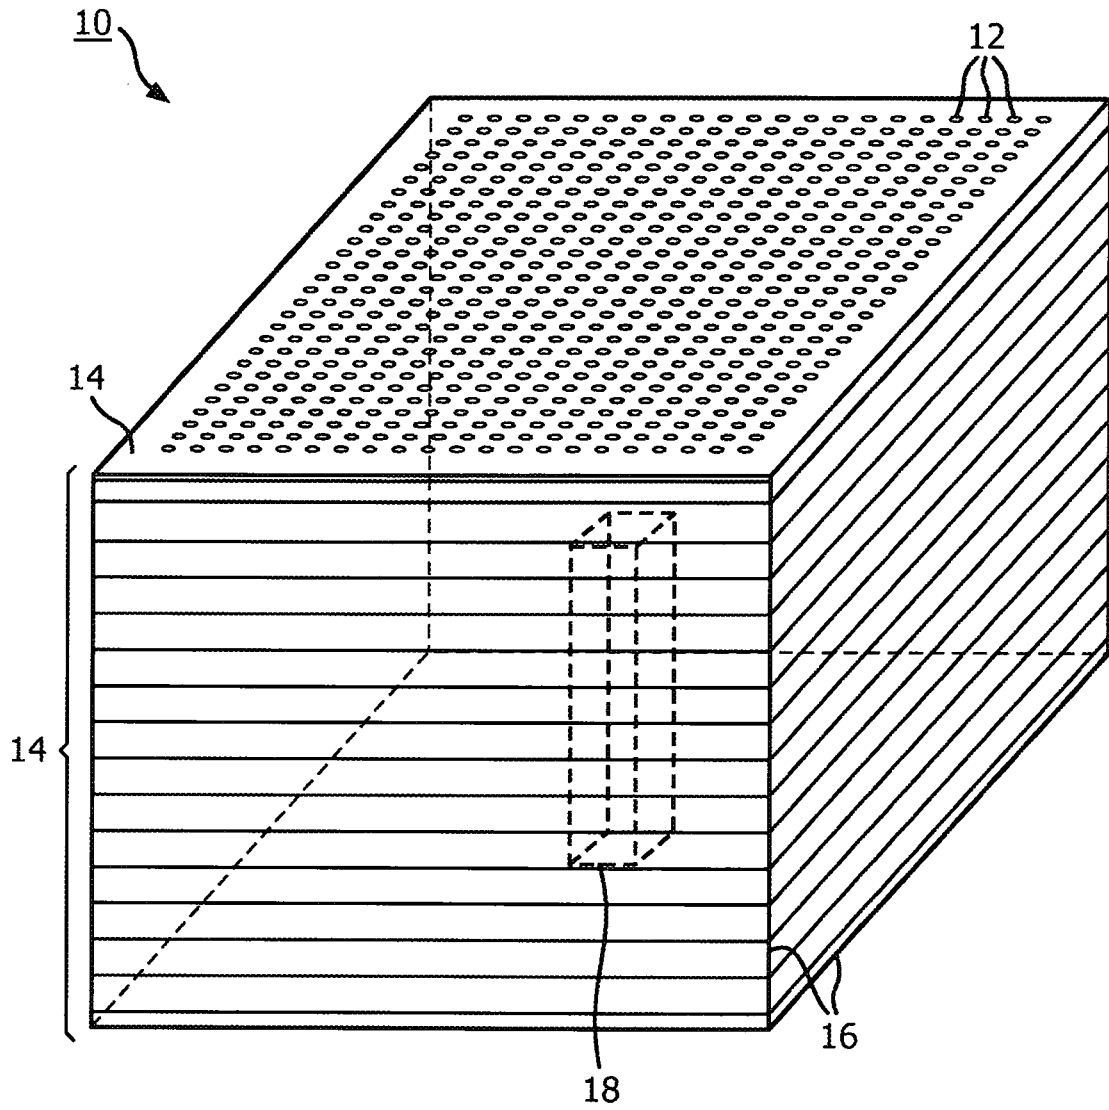


FIG. 1

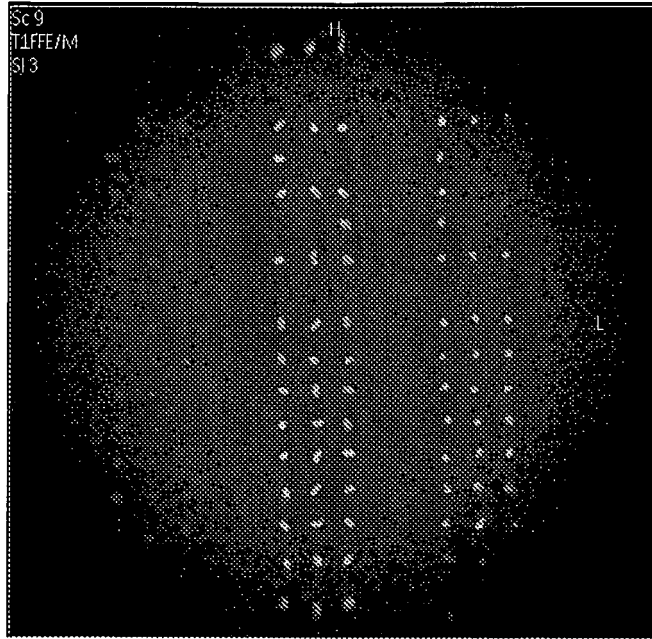


FIG. 2A

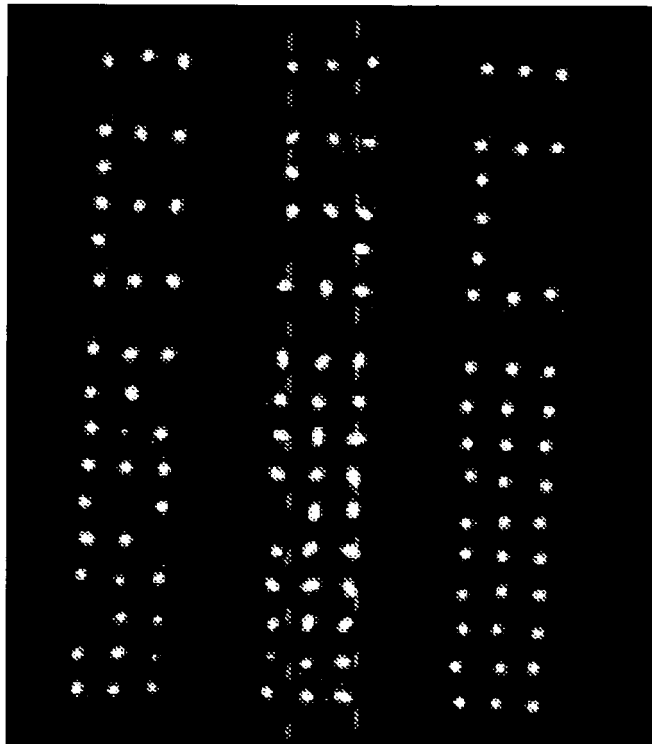


FIG. 2B

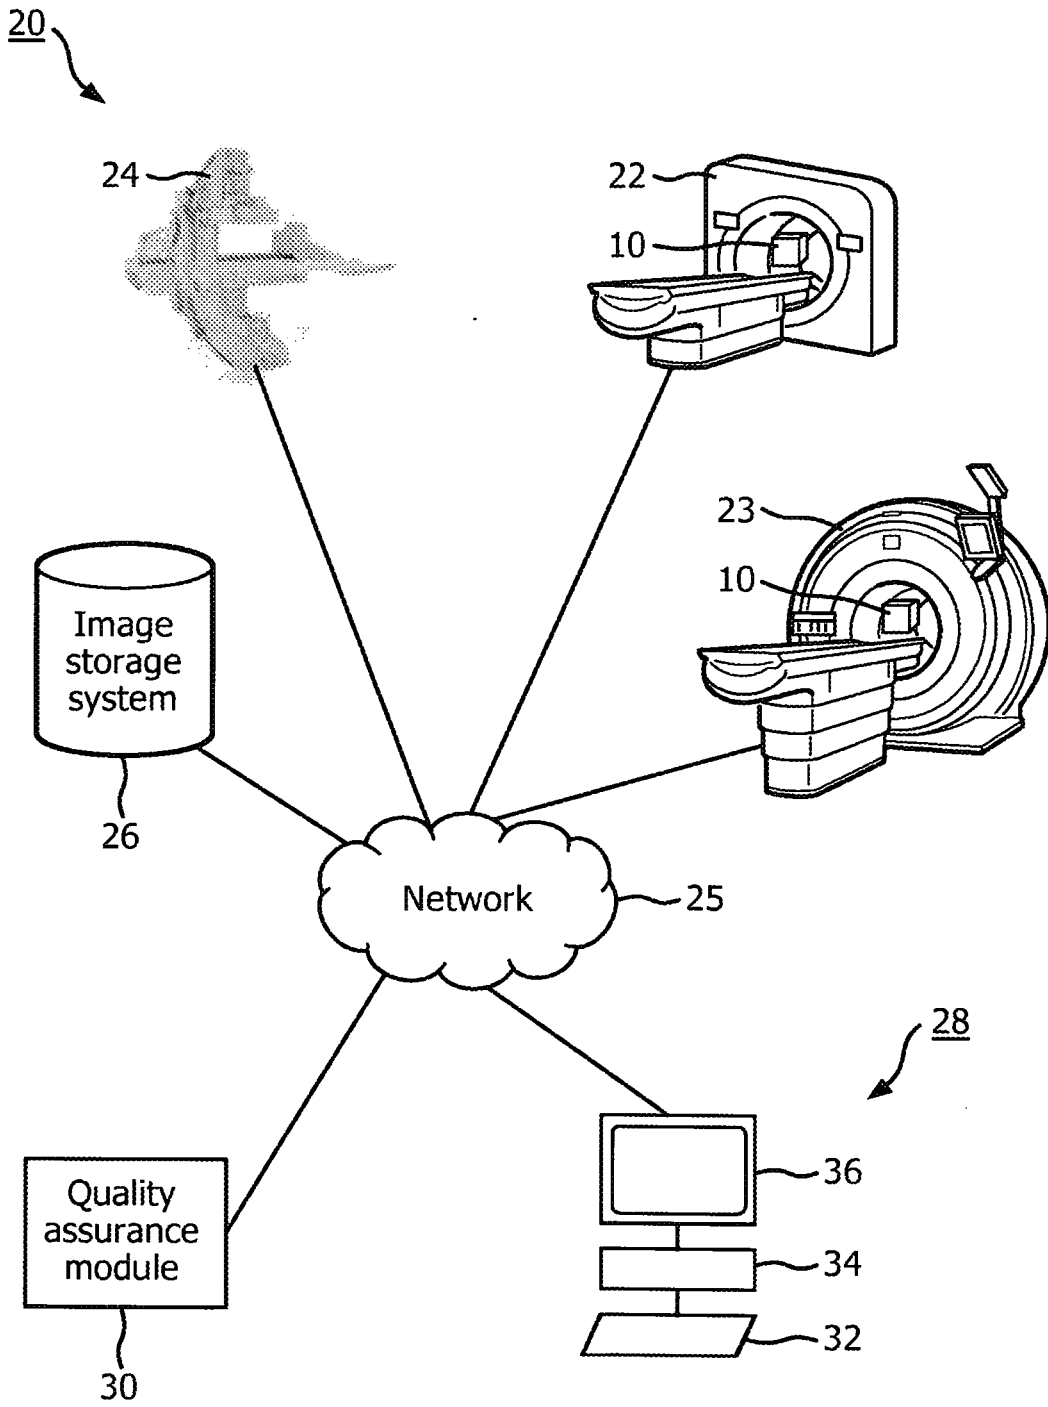


FIG. 3

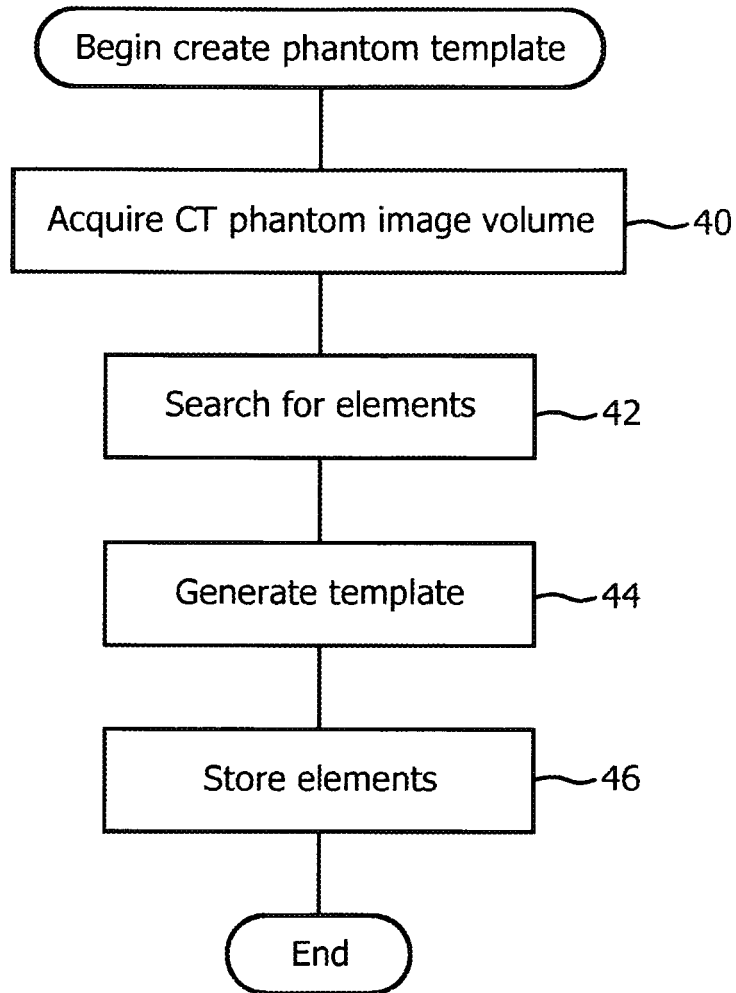


FIG. 4

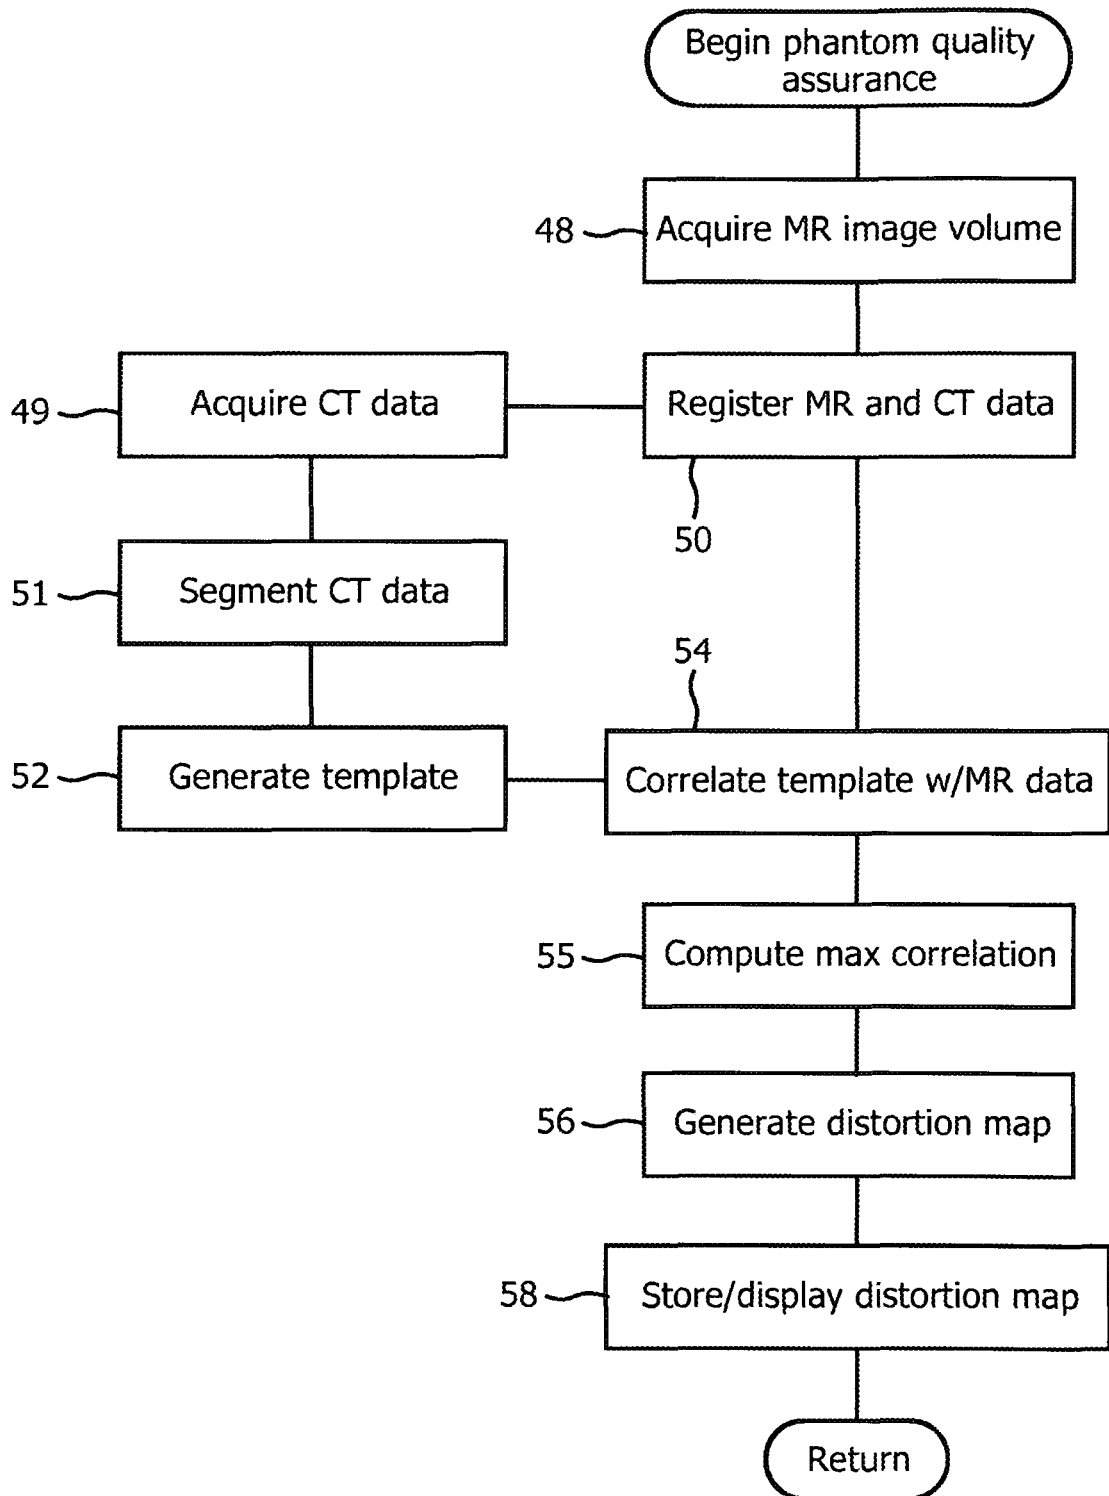


FIG. 5

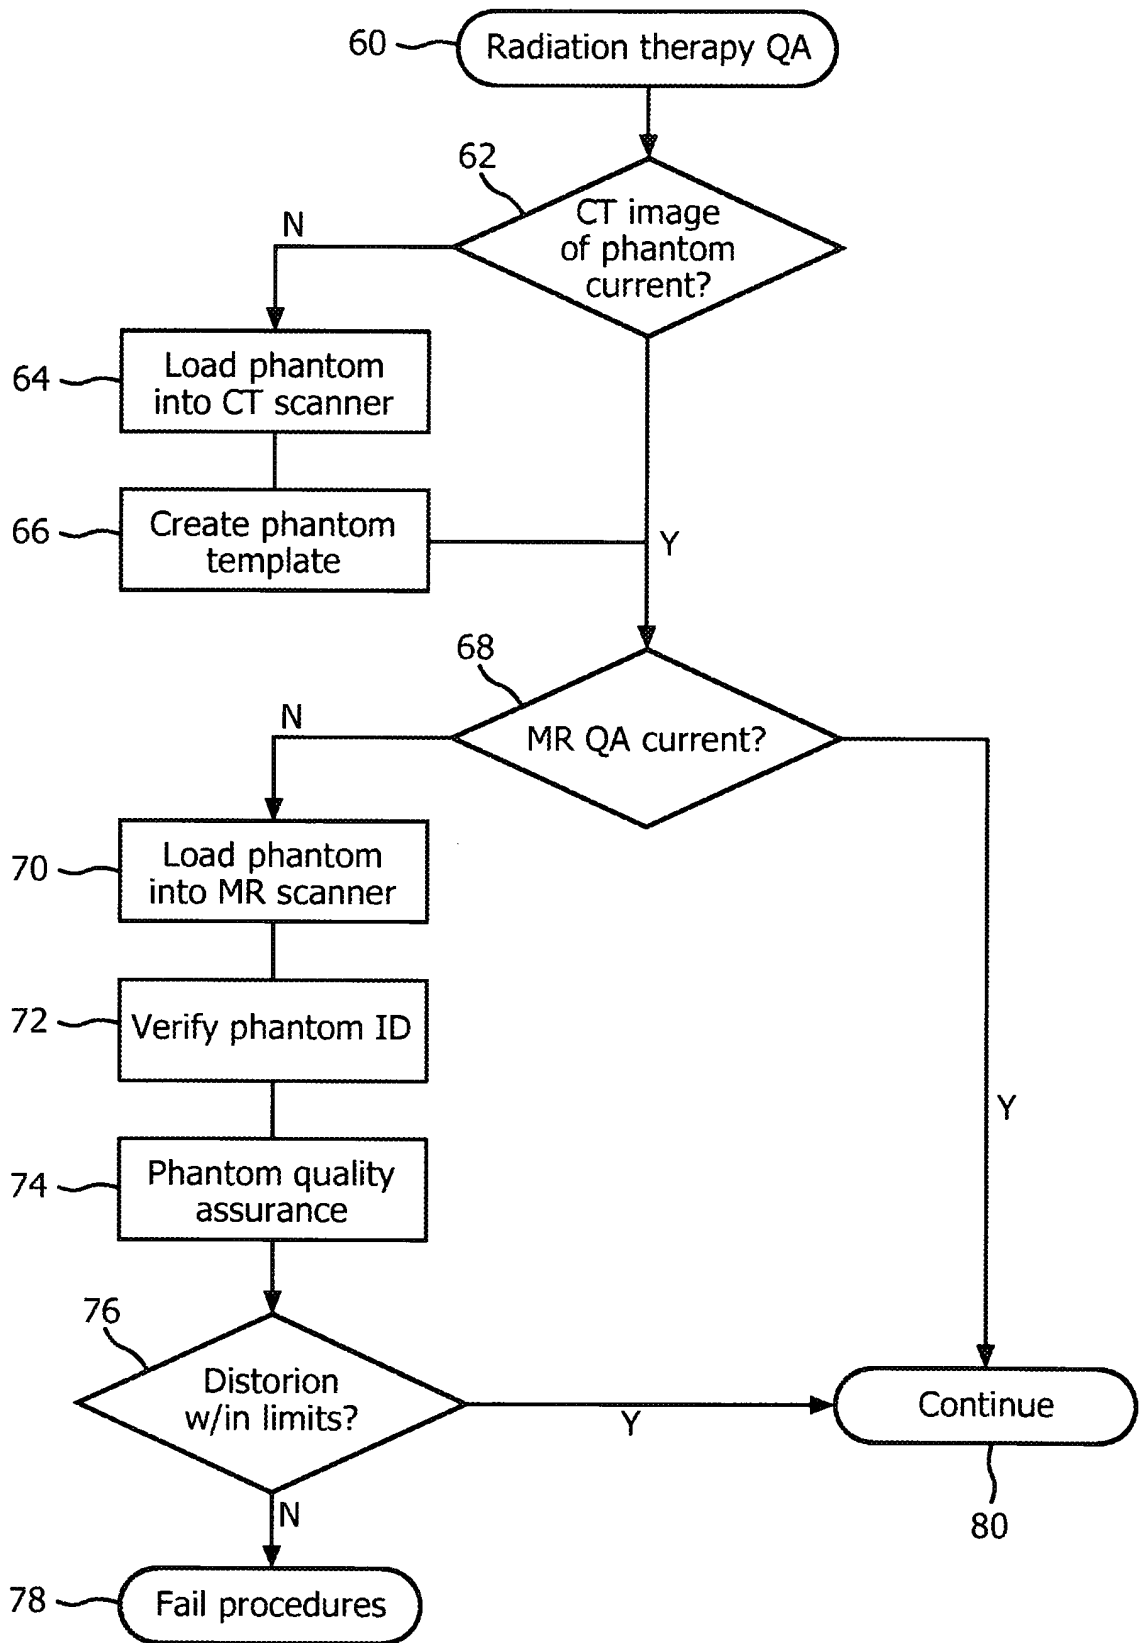


FIG. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 201080066372 A1 [0004]
- US 20110229055 A1 [0005]
- US 20090226066 A1 [0005]
- US 20030212320 A1 [0006]
- US 20100021029 A1 [0007]
- US 7056019 B1 [0008]

专利名称(译)	基于磁共振的放射治疗计划的质量保证装置和方法		
公开(公告)号	EP2830501B1	公开(公告)日	2016-05-18
申请号	EP2013722540	申请日	2013-03-22
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	FOXALL DAVID LESLIE KOTYS MELANIE SUZANNE DEVARAJ AJIT		
发明人	FOXALL, DAVID, LESLIE KOTYS, MELANIE, SUZANNE DEVARAJ, AJIT		
IPC分类号	G01R33/30 G01R33/46 G01R33/48 A61B5/00 A61B6/00 A61B5/055 A61N5/10 A61B6/03 G01R33/58		
CPC分类号	G01R33/583 A61B5/0035 A61B5/055 A61B6/032 A61B6/583 A61B2560/0228 A61N5/1039 A61N2005/1076 G01R33/30 G01R33/46 G01R33/4812 G01R33/58		
代理机构(译)	STEFFEN , THOMAS		
优先权	61/616548 2012-03-28 US		
其他公开文献	EP2830501A1		
外部链接	Espacenet		

摘要(译)

用于基于磁共振的放射治疗计划中的磁共振 (MR) 成像装置 (23) 的质量保证的系统 (20) 包括体重量小于18.2kg (40lbs) 的体模 (10) 。体模包括位于MR和CT惰性泡沫支撑件 (14) 中的MR和CT可成像元件 (12) 的三维空间分布，以及围绕并气密密封泡沫支撑件的MR和CT惰性外部支撑结构 (16) 。 。空间分布的大小适于完全填充磁共振成像设备的成像体积。